EPA 600/R-12/623 September 2012 | www.epa.gov/ord

United States
Environmental Protection
Agency

Interlaboratory Validation of the Leaching Environmental Assessment Framework (LEAF) Method 1313 and Method 1316

SCIENCE

Office of Research and Development

EPA/600/R-12/623
September 2012

Interlaboratory Validation of the Leaching Environmental Assessment Framework (LEAF) Method 1313 and Method 1316

Andrew C. Garrabrants[1], David S. Kosson[1], Leonard Stefanski[2], Rossane DeLapp[1], Paul F.A.B. Seignette[3], Hans A. van der Sloot[4], Peter Kariher[5], and Mark Baldwin[6]

[1] Vanderbilt University
Civil and Environmental Engineering
Nashville, TN 37235

[2] North Carolina State University
Department of Statistics
Raleigh, NC 27695

[3] Energy Research Centre of the Netherlands
Biomass, Coal and Environmental Research
1755 ZG Petten, the Netherlands

[4] Hans van der Sloot Consultancy
1721 BV Langedijk, the Netherlands

[5] ARCADIS-US, Inc.
Research Triangle Park, NC 27711

[6] U.S. Environmental Protection Agency
Office of Solid Waste and Emergency Response
Washington, DC 20460

Category III / Applied Research

Contract No. EP-C-09-027
Work Assignment No. 3-07

Prepared for
Susan A. Thorneloe
U.S. Environmental Protection Agency
Office of Research and Development
National Risk Management Research Laboratory
Air Pollution Prevention and Control Division
Research Triangle Park, NC 27711

Notice

The U.S. Environmental Protection Agency through its Office of Research and Development partially funded and managed the research described here under Contract Number EP-C-09-27 coordinated by ARCADIS-US, Inc. This report has been subjected to the Agency's peer and administrative review and has been approved for publication as an EPA document.

ACKNOWLEDGMENTS

This interlaboratory validation study was conducted under the United States Environmental Protection Agency (EPA) Contract Number EP-C-09-27 coordinated by ARCADIS-US, Inc. (ARCADIS). Organization of the validation study was a collaborative effort of ARCADIS, Vanderbilt University (VU), EPA Office of Solid Waste and Emergency Response (OSWER) and EPA Office of Research and Development (ORD). Partial financial support was provided by the U.S. Department of Energy, Office of Environmental Management under Cooperative Agreement Number DE-FC01-06W07053 entitled 'The Consortium for Risk Evaluation with Stakeholder Participation III' awarded to Vanderbilt University.

Material preparation and distribution were carried out jointly by ARCADIS and VU. All chemical analyses of leaching eluate solutions were conducted at VU. Development and review of statistical approaches were performed at North Carolina State University.

The authors gratefully acknowledge the following laboratories and contact leads for donating time, effort, and support as participating laboratories in the validation study:

Energy Research Centre of the Netherlands, Petten, the Netherlands (Rob Comans)

DHI, Hørsholm, Denmark (Ole Hjelmar)

Oak Ridge National Laboratory, Oak Ridge, TN (Catherine Mattus)

The Ohio State University, Columbus, OH (Zuzana Bohrerova)

Pacific Northwest National Laboratory, Richland, WA (Eric Pierce and Michelle Valenta)

Savannah River National Laboratory, Aiken, SC (Charles Crawford and Kimberly Roberts)

Test America Inc., Nashville, TN (Johnny Mitchell)

The University of Missouri, Rolla, MO (Jianmin Wang)

The University of Wisconsin, Madison, WI (James Tinjum)

URS Corporation, Inc., Austin, TX (Mandi Richardson)

The authors also thank Gregory Helms (EPA OSWER), Richard Benware (EPA OSWER), and Susan Thorneloe (EPA ORD) for guidance and significant contributions to the success of this program.

ABSTRACT

This document summarizes the results of an interlaboratory study conducted to generate precision estimates for two parallel batch leaching methods which are part of the Leaching Environmental Assessment Framework (LEAF) and are under review by the U.S. Environmental Protection Agency (EPA) Office of Solid Waste and Emergency Response for potential inclusion into the EPA's *Test Methods for Evaluating Solid Waste, Physical/Chemical Methods* (SW-846).

- *Method 1313: Liquid-Solid Partitioning as a Function of Eluate pH using a Parallel Batch Extraction Procedure*
- *Method 1316: Liquid-Solid Partitioning as a Function of Liquid-to-Solid Ratio using a Parallel Batch Extraction Procedure*.

For each of the two methods, the interlaboratory study targeted ten participating laboratories and three study materials – a coal combustion fly ash, a cementitious solidified waste analog, and a contaminated smelter site soil. Method precision was evaluated using repeatability relative standard deviation (RSD_r) and reproducibility relative standard deviation (RSD_R) of eluate concentrations obtained from the interlaboratory study.

The mean repeatability were determined to be 13% RSD_r for Method 1313 and 8% RSD_r for Method 1316. This level of within-laboratory precision means that variation of test replicates from a single operator would be less than 13% for Method 1313 and 8% for Method 1316. Method repeatability was consistent with the repeatability found for a European standard (EN) single-batch extraction test, EN 12457-2. Mean method reproducibility was determined to be 28% RSD_R for Method 1313 and 19% RSD_R for Method 1316 indicating the potential variation in multi-laboratory results on the same material. Reproducibility precision was consistent with the reported median reproducibility estimate for EN 12457-2 and was considerably better than the mean reproducibility value reported for the EPA's Toxicity Characteristic Leaching Procedure (TCLP; SW-846 Method 1311).

In parallel to the validation of the LEAF methods, the study materials were tested by the Energy Research Centre of the Netherlands and DHI, Denmark using two European technical specification for pH-dependence leaching currently in process of standardization through the Comité Européen de Normalisation (CEN). Although similar in structure and intent to Method 1313, these two tests differ from each other and from Method 1313 in the way that the final pH is achieved. Comparisons of the CEN test data to Method 1313 robust confidence limits showed that there is little to no operational difference in the pH-dependent leaching results from the three study materials. The findings of this study provide confidence that Method 1313 and Method 1316 provide the characteristic leaching behavior that is intended by the LEAF leaching methods with a high degree of precision.

EXECUTIVE SUMMARY

The potential impact on the environment when a solid material is either disposed or otherwise applied to the land has traditionally been measured through the use of one or more leaching tests. The current United States Environmental Protection Agency (EPA) protocol to classify waste materials as "hazardous" to the environmental is the Toxicity Characteristic Leaching Procedures (TCLP; EPA, 1992a) which simulates a plausible worst-case mismanagement scenario of co-disposal with municipal solid waste. While this approach has merits for classification purposes, a more flexible and robust methodology could provide the EPA and the waste management community with a uniform basis for leaching characterization that is applicable over a wide range of waste types and release scenarios. Thus, the EPA Office of Solid Waste and Emergency (OSWER) has initiated a review of the leaching test methods contained within the Leaching Environmental Assessment Framework (LEAF) for potential inclusion into EPA's compendium of laboratory methods, *Test Methods for Evaluating Solid Waste, Physical/Chemical Methods*, also known as SW-846. The LEAF methods have been developed in collaboration between Vanderbilt University (VU), the Energy Research Centre of the Netherlands (ECN) and DHI with support and guidance from ARCADIS-US, Inc. (ARCADIS) and EPA's Office of Research and Development (ORD). As opposed to simulating a particular release scenario, these leaching methods challenge a solid material to a broad range of leaching conditions that may plausibly occur in the course of waste management, focusing on those key parameters that control equilibrium and mass transport from solid materials. The LEAF approach provides considerable flexibility in that no specific leaching scenario is imposed, but the methods rather focus on intrinsic leaching characteristics, so that the results may be applied and used to compare scenarios representing a range of plausible management options.

As part of the review for SW-846, documentation is required regarding the precision (i.e., repeatability and reproducibility) of the methods for various types of potential waste materials. This precision data is intended to provide perspective on the variation in test method results that may be anticipated (i) when a single laboratory performs the method on homogenous replicates of the same material sample, or (ii) when multiple laboratories perform the test on replicate samples of a single material. In addition, the precision data supports the development of regulatory guidance on the use of the method and can be used to establish criteria for acceptable laboratory method performance. This report summarizes the results of an interlaboratory method validation study to generate precision information for two of the four LEAF leaching methods:[1]

- *Method 1313: Liquid-Solid Partitioning as a Function of Eluate pH using a Parallel Batch Extraction Procedure*
- *Method 1316: Liquid-Solid Partitioning as a Function of Liquid-to-Solid Ratio using a Parallel Batch Extraction Procedure*.

These two methods are parallel batch leaching procedures designed to determine the liquid-solid partitioning between a solid material and a leaching solution under conditions approaching equilibrium and as a function of final extract pH (Method 1313) or liquid-to-solid ratio (Method 1316). These

[1] Although the LEAF methods are numbered in a manner consistent with SW-846, these methods are currently considered preliminary versions of EPA Methods which have not yet been endorsed by EPA pending method validation and final review.

methods involve preparation of fine-grained subsamples of the study material by sieving and crushing (as appropriate to yield subsamples with 85% by mass less than specified grain size), parallel batch extractions of the material using common laboratory equipment, and filtration to prepare eluate solutions[2] for chemical analysis. Due to the procedural similarities of these methods, validation of both Method 1313 and Method 1316 is documented in a single report.

The structure of the validation study followed the two-phase approach recommend by EPA's *Guidance for Methods Development and Methods Validation for the RCRA Program* (EPA, 1992b). The minimum guidelines for the validation study were to provide for testing of three materials at six participating laboratories. While exact values for materials and laboratories may differ, these guidelines are consistent with AOAC recommendations for validation studies and the study design suggested in ASTM International (ASTM) E691 *Standard Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method* (ASTM 1986). Recognizing that participating laboratories would donate time and support for the project and a certain level of attrition would be anticipated, additional laboratories were targeted in order to provide for a minimum of six laboratories completing any phase of the validation study. ARCADIS provided project management and served as the validation reference laboratory due to considerable experience with the test methods (EPA 2006, 2008, 2009). In order to minimize variation in test results due to different analytical techniques and operators, all chemical analysis was conducted at VU by ICP-OES using EPA Method 6010 (EPA 2010). The study design as well as all material handling approaches and analytical procedures with data quality indicator (DQI) goals were written into a quality assurance project plan (QAPP) which was signed and approved by quality assurance representatives of ARCADIS and the EPA.

Three materials, that span a range of material types considered relevant by the EPA for waste management, were chosen for the validation. These materials included a coal combustion fly ash (material code EaFA), a solidified waste analog (material code SWA) and a contaminated soil from a smelter facility (material code CFS). Prior to distribution to the participating laboratories, these materials were processed (e.g., crushed to specified particle size) and homogenized at either ARCADIS or VU. Subsamples of homogenized material were shipped to each laboratory. The total contents of major, minor, and trace constituents in each of study materials were determined at ARCADIS by a combination of x-ray fluorescence spectroscopy (XRFS) and digestion following EPA Methods 3052 and 3051. Digestates were chemically analyzed at VU by inductively coupled plasma–optical emission spectroscopy (ICP-OES) to determine the total contents in the solid materials. XRFS data for twelve subsamples of homogenized material were used to assess the homogeneity of the samples prior to distribution. DQIs for total contents were well within the goals established in the QAPP for EaFA and SWA. The initial DQIs for homogenization of CFS were outside of the desired range; however, removal of carbon from XRFS list of major analytes improved the DQI for CFS. The rationale for removal of total carbon is that XRFS is not a preferred method for determination of total carbon which is better analyzed by combustion methods. With the improvement to the homogeneity DQIs for CFS, all materials were considered sufficiently homogenous prior to distribution to the participating laboratories.

[2] This report uses the LEAF terminology where "eluate" refers to the solution resulting from a leaching test whereas "leachate" refers to the solution collected from or measured in the field. The distinction between terms is made to minimize confusing when comparing laboratory data to field data.

In the first phase of the validation study, ten participating laboratories were asked to demonstrate method proficiency by conducting both Method 1313 and Method 1316 in triplicate on a single study material. During testing, participating laboratories recorded laboratory data in Microsoft® Excel spreadsheets provided to the laboratories as templates for data collection. Filtered and preserved eluates solutions from leaching tests carried out at participating laboratories were shipped to VU for chemical analysis. The leaching results from individual laboratories were compared to the results of six test replicates conducted on the same material by ARCADIS serving as a reference laboratory. Nine of the ten initial laboratories completed the proficiency demonstration phase and all laboratories were passed on to the second phase. In the second phase testing, participating laboratories were requested to prepare eluate solutions for two additional materials following the same approach as in first phase. In all, approximately ten participating laboratories participated in each phase of the study and generated eluate solutions for 27 to 36 test replicates[3] of either nine eluate solutions for Method 1313 or five eluate solutions for Method 1316. Data management and analysis of this large data set was conducted using LeachXS™, a software program developed specifically for data management, visualization, and modeling of leaching data.

Ten inorganic analytes from each material were chosen for processing to generate statistical and precision measurements. The list of selected constituents differed based on the leaching behavior of each material, but included eight constituents (i.e., antimony, arsenic, barium, boron, calcium, molybdenum, selenium and vanadium) common to all study materials. Leachates generated by the participating laboratories were shipped to VU where eluates concentrations were determined by ICP-OES following standard quality assurance/quality control procedures as specified in the QAPP, including calibration checks, blanks and analytical spikes. In all, the DQIs for eluate solution analysis were much better than the DQI goals established in the QAPP and provided confidence that the measured eluate concentrations were valid within an analytical uncertainty of about 5%. Method blanks (i.e., extract solutions without solid material that follow through the leaching test procedure) were checked for potential sources of contamination during testing. Although approximately 20% of the eluate solutions were potentially affected by high concentrations in method blanks and were eligible for removal or "filtering" from the data set, a comparison the results for filtered and non-filtered data sets showed little to no impact of filtering on preliminary precision statistics. Therefore, no eluate data was filtered due to method blank concentrations. Some data was filtered, however, due to identified procedural or operator errors. For example, Method 1313 data was filtered because (i) high sulfur in all eluate solutions interfering with barium leaching, (ii) boron contamination due to caustic stored in borosilicate glass, (iii) obvious errors in pH measurements most notable at extremes of the pH scale. In all, the amount of data that was "filtered for cause" was less than 20% of the total data set and in no case resulted in less than six laboratories reporting data.

For each method, the results for each material were processed using $\log_{10}$ transformation and linear interpolation/extrapolation of measured extract concentrations to yield a set of data used in statistical analysis. Statistical measurement included (i) means and standard deviations at each target extraction specified in the methods, (ii) 95% prediction limits about the mean of the reference laboratory data, (iii)

[3] The number of data points collected for each pH target included data from six test replicates conducted by the reference laboratory plus triplicate analysis conducted by the participating laboratories (e.g., the minimum value of 27 considers 21 data points from triplicate test runs of the seven participating laboratories plus six test replicates from the reference laboratory).

95% robust confidence limits (RCLs) about the median of the laboratory means, (iv) estimates of repeatability and reproducibility, and (v) the Horwitz ratio (e.g., the ratio of reproducibility relative standard deviation to that predicted as a function of concentration by the Horwitz equation). Prediction limits and robust confidence intervals, respectively, showed the ranges of leaching concentration that would capture 95% of the data for the reference laboratory performing replicate tests and for additional laboratories testing the same material. In the literature, Horwitz ratios ($HorRat_R$), which adjust for the natural tendency of analytical methods to have higher relative standard deviations as concentrations decrease, have been used to provide a cutoff value (i.e., $0.5 < HorRat_R < 2.0$) for "acceptability" of the variation associated with an analytical method. However, the Horwitz ratio was used in this study only to highlight precision results where analytical performance did not adequately describe the observed variability.

Source of variation in the validation results were based on feedback from the participating laboratories, precision statistics, and the assessment of Horwitz ratios. The identified sources of variation included errors in pH measurement (e.g., inadequate pH meter calibration, waiting to measure pH after solid-liquid phase separation) and material heterogeneity, in some materials, due to time lag between distribution of study materials and testing. The median values of Method 1313 precision for eight analytes common to all three study materials were 13% RSD_r for repeatability and 28% RSD_R for reproducibility. Therefore, single operator replication of Method 1313 would be within 13% while test results for multiple laboratories performing Method 1313 on the same material would be within 28%. For Method 1316, the median precision values were slightly better for the same set of analytes at 8% RSD_r repeatability and 19% RSD_R reproducibility indicating that single operator variation would be 8% and the variation in results from multiple laboratories would be within 19%. Since the EPA does not specify precision criteria for "acceptability" of a test method, no conclusion regarding the acceptability of these methods could be made. However, the repeatability and reproducibility for both methods were consistent with or better than similar precision estimates derived for a European standard (EN) single-batch leaching test, EN 12457 part 2 (van der Sloot et al. 2001) and considerably lower than the mean reproducibility value reported for TCLP (EPA 1992a). Therefore, Method 1313 and Method 1316 can be performed with the same or better precision as other currently active standardized leaching procedures.

In parallel to the interlaboratory validation study, research laboratories in the Netherlands and Denmark measured the pH-dependent leaching of the three study materials using two European technical standard (TS) leaching tests currently undergoing standardization through the Comité Européen de Normalisation (CEN). These two pH-dependence leaching tests, CEN/TS 14429 and CEN/TS 14997, are similar in structure and approach to Method 1313; however, minor procedural differences exists between all of these tests in how pH is controlled in the final eluate and the distribution of pH values across the range of environmental pH. CEN/TS 14429 allows for initial addition of dilute acid and base solutions in the same way as Method 1313; however, leaching solutions are introduced in three equal fractions over the first two hours of the test. This approach applied to wastes in the CEN/TS 14429 test has become the basis for leaching tests developed under ISO technical committee TC 190 for Soil Quality. Rather than initial acid or base additions, CEN/TS 14997 specifies the use of automatic pH control to adjust and maintain pH over the duration of the test. The results of the CEN TS testing were plotted against the 95% robust confidence limits derived from interlaboratory testing of Method 1313. For nearly 30 metal analytes from each of the three study materials, CEN leaching test concentrations agreed extremely well with the 95% robust confidence limits (RCLs) for Method 1313 indicating little to no difference in the performance of

Method 1313 and European pH-dependent leaching tests. Small deviations for three example analytes could be explained by material heterogeneity (e.g., aging effects, incomplete dissolution of metal salts in SWA), oxidation of leaching solutions in open vessels during CEN/TS 14997, or storage of strong reagents in containers made of incompatible materials. Overall, excellent agreement between the three tests supports the fact that Method 1313 is an appropriate leaching procedure for determining the pH-dependent leaching from solid materials.

ABBREVIATIONS

ANC	acid neutralization capacity
ANOVA	analysis of variance
ASTM	ASTM International (formerly American Society for Testing and Materials)
BNC	base neutralization capacity
CEN	European Committee for Standardization (Comité Européen de Normalisation)
CFS	contaminated field soil
df	degrees of freedom
DHI	DHI, Hørsholm, Denmark
DIC	dissolved inorganic carbon
DOC	dissolved organic carbon
DQI(s)	data quality indicator(s)
EaFA	coal combustion fly ash
ECN	Energy Research Centre of the Netherlands (Petten, the Netherlands)
EN	European standard test method
EPA	United States Environmental Protection Agency
EU	European Union
HDPE	high density polyethylene
$HorRat_R$	reproducibility Horwitz ratio
IC	ion chromatography
ICP-MS	inductively coupled plasma-mass spectroscopy
ICP-OES	inductively coupled plasma-optical emission spectroscopy
IQR	interquartile range
ISO	International Organization for Standardization
LEAF	Leaching Environmental Assessment Framework
L/S	liquid-to-solid ratio [mL/g, dry mass basis]
LSP	liquid-solid partitioning
M	median of laboratory means
MAD	median absolute deviation
MDL	method detection limit
ML	minimum level of quantification
MSDS	material safety data sheet
ORD	Office of Research and Development
OSWER	Office of Solid Waste and Emergency Response
ORCR	Office of Resource Conservation and Recovery
PL(s)	prediction limit(s)
$PRSD_R$	predicted reproducibility relative standard deviation
QAPP	quality assurance project plan
QA/QC	quality assurance/quality control

RCL(s)	robust confidence limit(s)
RCRA	Resource Conservation and Recovery Act
RL(s)	reproducibility limit(s)
RSD(s)	relative standard deviation(s)
RSD_r	repeatability relative standard deviation
RSD_R	reproducibility relative standard deviation
s_r	standard deviation associated with repeatability
s_R	standard deviation associated with reproducibility
SWA	solidified waste analog
SW-846	EPA methods compendium, *Test Methods for Evaluating Solid Waste, Physical/Chemical Methods*
TC	toxicity characteristic
TS	technical specification
XRFS	x-ray fluorescence spectroscopy

TABLE OF CONTENTS

Acknowledgments ..... **ii**
Abstract ..... **iii**
Executive Summary ..... **iv**
Abbreviations ..... **ix**
List of Figures ..... **xiv**
List of Tables ..... **xv**
Introduction **1**
Study Objectives **3**
Method Descriptions **3**
Method 1313: Liquid-Solid Partitioning as a Function of Eluate pH using a Parallel Batch Extraction Procedure 3
Method 1316: Liquid-Solid Partitioning as a Function of Liquid-Solid using a Parallel Batch Extraction Procedure 4
Data Management of LEAF Test Results 4
Validation Study Overview **4**
Project Organization 5
Selection and Maintenance of Participating Laboratories 5
Phase I - Initial Demonstration of Proficiency 6
Evaluation of Phase I Data and Analyte Selection 6
Phase II – Generation of Method Validation Results 6
Calculation of Precision Statistics 6
95% Prediction Limits (PLs) *7*
95% Robust Confidence Limits (RCLs) *7*
Standard Deviations about the Mean *7*
Coefficient of Variation (CVs) *7*
Horwitz Ratio *7*
Relative Standard Deviations *7*
Study Materials **8**
Coal Combustion Fly Ash 8
Solidified Waste Analog 8
Contaminated Field Soil 9
Total Content of Study Materials 9
Analytical Methods **11**
Supplemental Analysis for Reference Laboratory Eluates 12
Inductively Coupled Plasma – Mass Spectroscopy *12*
Total Carbon Analysis *12*
Data Processing **13**
Method Blank Analysis and Data Filtering 13
Data Transformation and Linear Interpolation/Extrapolation to Target Values 13
Statistical Calculations **14**
95% Prediction Limits (PLs) based on Reference Laboratory Results 14
95% Robust Confidence Limits (RCLs) based on the Median of Laboratory Mean Data 15
Estimates of Variance Components and Standard Deviations 16
Preliminary Calculations and Example ANOVA Table *17*
Variance Components and Standard Deviations *17*

Repeatability and Reproducibility 18
Horwitz Ratio (HorRat) 18
Reproducibility Limit 19
Phase I Laboratory Feedback (Methods 1313 and 1316) 20
QA/QC Summary 21
Homogeneity of Study Materials 21
Analytical QA/QC 22
Method Blank Analysis 23
Data Filtering for Cause 23
Analyte Selection and Data Transforms 24
Method 1313 Results and Analysis 26
Acid/base Neutralization Capacity (Titration Curve) 26
Statistical Analysis of pH-dependent Leaching 27
Interpolation/Extrapolation of Log_{10}-transformed Data 29
Prediction Limit and Robust Confidence Limits 31
Standard Deviations and Coefficients of Variation 34
Method 1313 Repeatability and Reproducibility 35
Method 1316 Results and Analysis 41
pH Response as a Function of L/S 41
Statistical Analysis of L/S-dependent Leaching Data 42
Interpolation/Extrapolation of Log_{10}-transformed Data 42
Prediction Limit and Robust Confidence Limit -based Statistical Analysis 42
Standard Deviations and Coefficients of Variation 44
Method 1316 Repeatability and Reproducibility 44
Comparison of Method Precision to Standardized Leaching Methods 50
TCLP (SW-846 Method 1311) Reproducibility 50
EN 12457 Validation 50
Precision Distributions and Comparisons 50
Precision as a Function of Analyte 51
Precision as a Function of Test Parameters 51
Precision as a Function of Material 51
Comparison of Analogous EU Leaching Test Results to Method 1313 Validation Statistics 55
EU Test Method Descriptions (CEN/TS 14429 and CEN/TS 14497) 55
Comparison of EU Test Results to Method 1313 Statistics 56
Summary and Conclusions 58
Procedural Considerations 59
Data Validation Approach 60
Repeatability and Reproducibility 60
References 61

Appendices

Appendix A. Method 1313
Appendix B. Method 1316
Appendix C. Quality Assurance Project Plan
Appendix D. Blank Analysis and Data Filtering
Appendix E. Method 1313 Results

Appendix F. Method 1316 Results
Appendix G. Comparison of EU pH-dependence Tests to Method 1313 RCLs
Appendix H. Summary of Analytical QA/QC for Selected Analytes
Appendix I: Detailed QA/QC Reports for ICP-OES Analytes[4]

[4] Appendix I contains all of the details of the ICP-OES analysis and QA/QC results for each measured constituent in each provided analytical solution (i.e., filtered and preserved eluate sample). Therefore, due to its size, the appendix is made available electronically by request to the authors, through the link to the document page on the EPA website, or as a download at http://vanderbilt.edu/leaching.

LIST OF FIGURES

Figure 1. Acid/base neutralization capacity for Method 1313 study materials. 26
Figure 2. Antimony statistical analysis for Method 1313 Phase I material EaFA. 28
Figure 3. Comparison of Method 1313 collected data (left) and interpolated data (right). 29
Figure 4. Linear interpolation of log_{10}-transformed Method 1313 data showing potential for increasing data scatter when interpolating along steep slopes. 30
Figure 5. Agreement between 95% prediction limits (95% PL) about the mean of the reference laboratory data and 95% robust confidence limits (95% RCL) based on the median of laboratory means. 32
Figure 6. Propagation of variability due to linear interpolation of arsenic concentrations in Method 1313 samples of SWA. 33
Figure 7. Example standard deviation intervals about the mean and coefficients of variation for Method 1313 materials. 35
Figure 8. Method 1313 repeatability and reproducibility of antimony. 36
Figure 9. Method 1313 repeatability and reproducibility of molybdenum. 37
Figure 10. Interpolated data for Method 1313 for chromium in EaFA (left) and antimony in SWA (right). 38
Figure 11. Eluate pH for Method 1316 Study Materials. 41
Figure 12. Agreement between 95% prediction limits (95% PL) about the mean of the reference laboratory data and 95% robust confidence limits (95% RCL) based on the median of laboratory means. 43
Figure 13. Standard deviation intervals about the mean (left) and coefficients of variation (right) for Method 1316 materials. 45
Figure 14. Method 1316 repeatability and reproducibility of vanadium. 46
Figure 15. Method 1316 repeatability and reproducibility of boron. 47
Figure 16. Method precision as a function of selected analytes in comparison to precision values reported for EN 12457-2, shown as “EN” (van der Sloot et al. 2001) and TCLP (EPA 1992a). 52
Figure 17. Method precision as a function of test parameter in comparison to precision values reported for EN 12457 (van der Sloot et al. 2001) and TCLP (EPA 1992a). 53
Figure 18. Method precision as a function of material in comparison to precision values reported for EN 12457 (van der Sloot et al. 2001) and TCLP (EPA 1992a). 54
Figure 19. Leaching results from CEN tests compared to Method 1313 RL values. 57

LIST OF TABLES

Table 1. Summary of the Number of Targeted and Validation Laboratories 5
Table 2. Mix Formulation for Solidified Waste Analog (SWA) Material. 9
Table 3. Total Content of Study Materials. 10
Table 4. MDLs and MLs for ICP-OES. 11
Table 5. MDLs and MLs for ICP-MS. 12
Table 7. MDLs and MLs for Total Carbon Analysis. 13
Table 8. Constants C_n for Constructing the Robust Confidence Limits 16
Table 9. Example ANOVA Table 17
Table 10. Homogeneity QA/QC for Total Content Derived from XRFS 22
Table 11. DQI Goals and Overall Results 22
Table 12. DQIs for ICP-OES Analysis Selected Analytes 23
Table 13. Overview of Eluates Filtered for Cause 24
Table 14. Candidate ICP-OES Analytes and Selected Analytes for Statistical Analysis. 25
Table 15. Method 1313 Repeatability (RSD_r) across Study Materials 39
Table 16. Method 1313 Reproducibility (RSD_R) across Study Materials 40
Table 17. Method 1316 Repeatability (RSD_r) across Study Materials. 48
Table 18. Method 1316 Reproducibility (RSD_R) across Study Materials 49

INTRODUCTION

Leaching tests have traditionally been used to estimate the leaching potential of waste or other materials for situations where the material is placed in a landfill or used on the land. Leach testing is designed to assess the potential for contaminant release and the likelihood of groundwater contamination resulting from land application of wastes and other materials. In the literature, over 50 different leaching tests have been identified (van der Sloot et al., 1997) with many individual testing approaches developed for the evaluation of particular materials or specific management applications. For example, the United States Environmental Protection Agency (EPA) currently promulgates Method 1311 (EPA, 1992a), the Toxicity Characteristic Leaching Procedure (TCLP), for screening of hazardous wastes and support of land use decisions. Rather than establishing individual tests for each specific application, a more robust and flexible approach would allow for broad-based use of a limited set of leaching tests, designed to determined intrinsic leaching characteristics of wastes and other solid materials, providing leaching results that can be compared between material types and applied to a wide range of leaching conditions and release scenarios.

The Leaching Environmental Assessment Framework (LEAF) is a set of leaching test methods, scenario-based leaching assessment mass transfer models, and information management tools designed to provide more accurate estimates of constituent leaching under field conditions than current approaches based on single-extraction tests. The methodology for leaching assessment using LEAF is based on a tiered testing approach (Kosson et al., 2002) that can account for the impact of environmental conditions on leaching. Unlike TCLP and other simulation-based approaches currently in wide use, the LEAF leaching tests are characterization methods intended to generate intrinsic leaching behavior data for a material over a broad range of test conditions that encompasses the range of plausible waste management conditions. Key parameters that affect leaching include pH, the ratio of liquid leachant to solid material, and the form (e.g., particle size) of the waste material. The resulting data can be applied to assess leaching potential under anticipated field conditions for a range of management scenarios. Currently, the LEAF test methods are under review by the EPA Office of Solid Waste and Emergency Response (OSWER) for inclusion into the EPA's "T*est Methods for Evaluating Solid Waste, Physical/Chemical Methods*" (SW-846), the compendium of laboratory methods. A final stage in the review process is the determination of method precision, specifically repeatability and reproducibility, through interlaboratory validation to ensure that method performance is not limited to the individual operator or laboratory that developed the method.

Method precision is a measure of the variability among test results conducted on the same material or type of material as defined in ASTM International (ASTM) E1488 *Standard Practice for Statistical Procedures to Use in Developing and Applying Test Methods* (ASTM, 2002). Precision is commonly conveyed in terms of method repeatability and method reproducibility. Repeatability refers to the closeness of agreement between independent results obtained with the same method on identical test material, under the same conditions (Currie and Svehla, 1994). Method repeatability represents a measure of the expectations of the method to provide similar results of replicate test runs conducted by the same laboratory expressed through a "within-laboratory" standard deviation. Reproducibility refers to the closeness of agreement between independent results obtained with the same method on identical test

material but under different conditions (Currie and Svehla, 1994). Method reproducibility provides an estimate of the variability that might be expected when different laboratories measure the same property on the same material and is typically expressed as a reproducibility standard deviation.

This report provides method validation results for the following two LEAF leaching methods:[1]

- *Method 1313: Liquid-Solid Partitioning as a Function of Eluate pH using a Parallel Batch Extraction Procedure*
- *Method 1316: Liquid-Solid Partitioning as a Function of Liquid-to-Solid Ratio using a Parallel Batch Extraction Procedure*

The validation study for Method 1313 and Method 1316 is based on the two-phase approach suggested by the EPA's *Guidance for Methods Development and Methods Validation for the RCRA Program* (EPA 1992b). Within the EPA guidance, there are no pre-established precision criteria for acceptability of a method; therefore, no conclusion can be made on the acceptability of the LEAF methods based solely on precision. However, perspective on a reasonable level of precision may be found in currently accepted leaching procedures. For example, interlaboratory studies to provide precision estimates for TCLP showed a mean reproducibility of 74% relative standard deviation (RSD) with a range of RSD between 17 and 118% (EPA, 1992a). The intent of the interlaboratory study for Method 1313 and Method 1316 is to provide the precision statistics for these test methods which may be used to support the establishment of initial performance guidelines and the development of regulatory guidance on the use of these methods.

Since the LEAF methods have been developed to determine characteristic or intrinsic leaching behavior of a solid material, the results from a single material should be comparable between similar test methods designed with the same intent. As part of the validation study, two European laboratories determined the pH-dependent leaching characteristics of the study materials using two different pH-dependent leaching protocols being developed and adopted by the European environmental community.[2] Favorable comparison of Method 1313 results to the results derived from European Union (EU) pH-dependent leaching tests is intended to provide support that Method 1313 adequately accomplishes the goal of providing extraction eluates[3] that can be used to determine liquid-solid partitioning of wide variety of solid material types.

---

[1] Although the LEAF methods are numbered in a manner consistent with SW-846, these methods are currently considered preliminary versions of EPA Methods which have not yet been endorsed by EPA pending method validation and final review.

[2] The comparative European methods are designated as "technical specifications" with a TS designation, indicating a method definition has resulted from a multi-national consensus process and has been approved by a CEN technical committee. The TS designation, however, means that interlaboratory validation studies to assess precision have not yet been conducted and that public comment and consensus approval by CEN members will be repeated when performance characteristics are available. A TS designation does not carry the status of a European standard (EN), but may be adopted as national standard.

[3] This report uses the LEAF terminology where "eluate" refers to the solution resulting from a leaching test whereas "leachate" refers to the solution collected from or measured in the field. The distinction between terms is made to minimize confusion when comparing laboratory data to field data.

STUDY OBJECTIVES

The objectives of the method validation studies were to: (i) determine the method precision through assessment of method repeatability and reproducibility from extraction results using these methods over a range of potential waste materials; and (ii) compare the results of Method 1313 to standardized leaching methods for pH-dependent leaching under development and used in Europe.

METHOD DESCRIPTIONS

The validation results for these two methods are grouped into a single report due to the procedural similarity of these parallel batch methods and their use in conjunction with one another to assess leaching potential. Method 1313 and Method 1316 are parallel batch procedures intended to characterize the liquid-solid partitioning at conditions approaching equilibrium as a function of final extract pH and liquid-to-solid ratio (L/S), respectively. The test parameters and values specified in these methods have been described in a background information document on the LEAF leaching methods (Garrabrants et al., 2010). The following paragraphs briefly describe these methods; full-text versions are presented in Appendix A (Method 1313) and Appendix B (Method 1316).

Method 1313: Liquid-Solid Partitioning as a Function of Eluate pH using a Parallel Batch Extraction Procedure

Method 1313 is an equilibrium-based leaching test designed to provide eluate solutions representing the liquid-solid partitioning (LSP) curve of constituents as a function of eluate pH. The procedure consists of nine parallel batch extractions at targeted pH values and one extraction at the natural pH[4] of the material. The solid material may require particle size reduction by crushing in order to facilitate the approach to solid-liquid equilibrium within a reasonable extraction timeframe. Dilute acid or base in deionized water is added to each extraction according to a pre-test titration in order to achieve final extract pH values at specified target values ranging between 2 and 13 at an L/S of 10 mL/g-dry. The extraction contact time ranges from 24 to 72 hours based on the grain size of the "as tested" material (i.e., the material after any particle size reduction or air drying required to improve the handling of the "as received" material). The pH and conductivity of the final extract solution are recorded and vacuum- or pressure-assisted filtration is used to separate the liquid and solid phases prior to chemical analysis of the eluate. Eluate concentrations for constituents of interest are plotted as a function of eluate pH allowing for comparison to quality control and assessment limits. Eluate concentrations may also be interpolated to the target pH values to provide a uniform basis for comparison of results as the recorded eluate pH is likely to differ slightly from target values within specified pH tolerances.

[4] The natural pH (also referred to as "own pH") is the final eluate pH response of a deionized water extraction of a solid material (i.e., no acid or base added) conducted at an L/S 10 mL/g-dry.

Method 1316: Liquid-Solid Partitioning as a Function of Liquid-Solid using a Parallel Batch Extraction Procedure

Method 1316 is an equilibrium-based leaching test intended to provide eluate solutions over a range of L/S values from 10 to 0.5 mL/g-dry using five parallel batch extractions in DI water. No acid or base is added to the extractions so that the results can indicate changes in eluate pH with L/S. Particle size reduction of the solid material may be required in order to facilitate the approach to solid-liquid equilibrium. The contact time for the extractions ranges from 24 to 72 hours based on grain size. The pH and conductivity of the final extract solution are recorded. Solid and liquid phases are separated by vacuum- or pressure-assisted filtration and prepared for chemical analysis. This method provides information on the changes in equilibrium chemistry (i.e., ionic strength, constituent concentrations) as the L/S approaches values found within the solid phase pore solution.

Data Management of LEAF Test Results

For each of the LEAF methods, a data template in the form of a Microsoft® Excel spreadsheet is available and recommended to assist with method execution (e.g., calculations for the amounts of water and acid to be added to Method 1313 extracts based on sample mass, moisture content and titration curve information) as well as uniform recording of pertinent bench-scale and analytical data. Each data template also serves as an upload interface into the materials database contained within LeachXS Lite™, a limited capability version of LeachXS™.[5]

The Lite version of LeachXS is a freely licensed software program, focused primarily on data management and report facilitation, which was developed, in part, to facilitate EPA coal combustion residue reports (Sanchez et al., 2006; Sanchez et al., 2008, Kosson et al., 2009). The LeachXS Lite version allows users to import leaching test data from the LEAF methods into a materials database, compare test results to user defined indicator lines (e.g., quality control indicators or regulatory limits), and output Excel spreadsheets as tabular data and consistently formatted graphs for comparison between data sets (e.g., test replicates of the same material or of different materials). LeachXS Lite can be used with LEAF testing results from any applicable material and is not restricted to use for coal combustion residues. The free version does not include the advanced formatting, statistical calculations, or geochemical and reactive transport modeling capabilities of the full LeachXS version.

VALIDATION STUDY OVERVIEW

A two-phase validation study based on EPA's *Guidance for Methods Development and Methods Validation for the RCRA Program* (EPA, 1992b) was completed for each test method. This guidance document recommends that precision statistics be based on test results from a minimum of three materials conducted in triplicate by a minimum of three participating laboratories. The minimum number of laboratories in the study was deemed too small to produced adequate statistical analysis, so the guideline of at least six participating laboratories as recommended in ASTM E691 *Standard Practice for*

[5] The development of the LEAF methods, data templates, and LeachXS Lite™ is the result of collaboration between EPA, Vanderbilt University, the Energy research Centre of the Netherlands and DHI (Denmark). These materials are available free of charge at www.vanderbilt.edu/leaching.

Conducting an Interlaboratory Study to Determine the Precision of a Test Method (ASTM, 1987) was adopted for this study. The design and execution of this validation study was supported by a quality assurance project plan (QAPP) which described all material handling procedures and data quality goals. The QAPP is presented Appendix C as approved by the EPA Office of Research and Development.

Project Organization

ARCADIS-US, Inc. (ARCADIS) was selected as the reference laboratory for this study based, in part, on previous demonstration of proficiency (Sanchez et al., 2006; Sanchez et al., 2008; Kosson et al., 2009). In order to minimize variations in test method results stemming from different analytical approaches, equipment and operators, all eluate chemical analysis was conducted at Vanderbilt University (VU) using inductively coupled plasma-optical emission spectroscopy (ICP-OES). The EPA ORD served as project manager while the EPA Office of Resource Conservation and Recovery (ORCR) within EPA OSWER was responsible for maintaining lines of communications with participating laboratories and for gathering and assembling feedback on the methods from the participating laboratories.

Selection and Maintenance of Participating Laboratories

A wide range of participating laboratories (e.g., academic, government and commercial laboratories) were asked to donate time, personnel and support for this study. Each laboratory completing the entire validation study was asked to perform each test method in triplicate on three materials. In parallel, the reference laboratory submitted six test replicates of each test for chemical analysis.

Based on the *pro bono* nature of the laboratory participation, a certain level of attrition was expected throughout the course of the study. Therefore, ten laboratories for each phase of the study were targeted in order to maintain the minimum of six participating laboratories stated in the ASTM guidance. A summary of the number of targeted laboratories and the number of laboratories used in the validation study for each method and material is presented in Table 1.

Table 1. Summary of the Number of Targeted and Validation Laboratories.

Method	Materials	Target Laboratories	Validation Laboratories
Method 1313	Coal Combustion Fly Ash	11	10
	Solidified Waste Analog	10	8
	Contaminated Field Soil	10	8
Method 1316	Coal Combustion Fly Ash	11	10
	Solidified Waste Analog	10	8
	Contaminated Field Soil	10	8

Each laboratory was identified by a number to provide anonymity when reporting data. During Phase I of the study, only nine of the ten participating laboratories returned eluates for analysis. Laboratory Three (L03) was unable to participate due to unanticipated funding problems. In order to maintain a number of laboratories that would provide for attrition, an eleventh laboratory was added so that Phase I testing could be completed with ten participants. For Phase II testing, eight of the remaining ten laboratories returned samples for analysis. Laboratory Eight (L08) and Laboratory Two (L02) were unable to return eluates for one or both Phase II materials citing resource limitations.

Phase I - Initial Demonstration of Proficiency

Laboratories initially selected to participate in the study were asked to demonstrate proficiency and familiarization with the new methods by conducting triplicate test runs of both Method 1313 (nine or ten extracts per replicate) and Method 1316 (five extracts per replicate) on a single material and submitting filtered and preserved eluates to VU for chemical analysis. The reference laboratory conducted six test replicates. All in-laboratory data (e.g., extract setup calculations, eluate pH and conductivity measurements) were recorded and entered into Excel data templates by the participating or reference laboratories. The Excel data templates were provided to the laboratories by the study organizers to ensure proper archiving of all pertinent test data. Feedback from participating laboratories, in the form of written questionnaires and conference call discussions, was used to refine the test methods for Phase II in order to clarify any unclear procedures or descriptions.

Evaluation of Phase I Data and Analyte Selection

The laboratory data and eluate concentrations resulting from Phase I testing were imported into LeachXS by VU for initial statistical analysis and data graphing. Screening to pass participating laboratories on to Phase II of the study was based on visual comparison of eluate concentrations from participating laboratories to the results of six test replicates prepared by a reference laboratory. In addition, the results of Phase I were used to develop initial estimates and procedures for calculation of variance within and between laboratories as the statistical basis for quantifying method precision.

Phase II – Generation of Method Validation Results

Laboratories passing the Phase I portion of the validation were asked to continue participation by testing two additional materials by providing filtered eluates and laboratory data from triplicate test runs of both Method 1313 and Method 1316 conducted on two additional materials. As in Phase I, all in-laboratory data (e.g., extract setup calculations, eluate pH and conductivity measurements) were recorded by the participating laboratories in the form of Excel data templates.

Calculation of Precision Statistics

For each material and test, participating laboratories were required to complete the laboratory data sections of the provided Excel data template. When chemical analysis was complete and validated by VU analytical staff, eluate concentrations were amended to the data template which was used to upload test method and analytical data into LeachXS. The approach for analysis of validation data included standard statistical calculations consistent with the methodologies presented in EPA and ASTM guidance and the recommendations of the International Standards Organization (ISO) *Accuracy (Trueness and Precision) of Measurement Methods and Results* (ISO, 1994). This data assessment approach was recommended by collaborators at North Carolina State University and approved by EPA through the QAPP review process.

The statistical equations were implemented into a statistics module developed for LeachXS by collaborators at ECN. The statistics module allows the user to merge datasets from the materials database (e.g., each replicate of results from a single test of a method at a single laboratory is a separate dataset) and calculate parametric and non-parametric statistics. The output was saved as an .xml file that then was uploaded back into LeachXS for data processing and visualization. Using the standard statistical functions implemented in LeachXS for this project, the following statistics were derived from interpolated eluate concentrations and used to describe the validation data:

- ***95% Prediction Limits (PLs)***
  Prediction limits were calculated using the reference laboratory data and used to create an interval above and below the mean of the reference laboratory data. The interval about the mean indicates the range within which future data from the reference laboratory would fall at the 95% probability level.

- ***95% Robust Confidence Limits (RCLs)***
  Confidence Limits using robust statistical approaches (Huber, 1968; Daszykowski et al, 2007) were derived and used to create an interval about the median of the laboratory means. The interval represents the range of response for the mean of a laboratory at the 95% probability level.

- ***Standard Deviations about the Mean***
  Standard deviations associated with "within laboratory", "between laboratory" and "overall" variance factors were derived from the calculations used in a one-way analysis of variance (ANOVA). These standard deviations were used to create intervals about the mean of the data set to represent the range of uncertainty associated with each variance factor in the ANOVA. Since not formal ANOVA was conducted, the significance statistics from the F-distribution was not calculated.

- ***Coefficient of Variation (CVs)***[6]
  Coefficients of variation are presented as standard deviations for "within laboratory", "between laboratory" and "overall" variance factors normalized to the mean test output value in order to compare relative contributions from these variance sources.

- ***Horwitz Ratio***
  The Howitz Ratio is a statistic that was introduced to predict the inherent variability of chemical analyses as a function of concentration value (Horwitz and Albert, 2006). The Horwitz Ratio for reproducibility ($HorRat_R$) was calculated from the "overall" CV, often associated with reproducibility. In this report, the Horwiz Ratio was used only to assess if eluate concentration analysis near the method detection limit was a potentially significant source of variability in the test results.

- ***Relative Standard Deviations***
  The CVs for "within laboratory" and "overall" variance factors are used to represent method precision, respectively, as repeatability relative standard deviation (RSD_r) and reproducibility relative standard deviation (RSD_R).

Method precision, based on RSD_r and RSD_R values, were determined for ten selected analytes in each of the three study materials. Using the method precision data for eight analytes common to all study materials, distributions of method repeatability and reproducibility results as a function of test parameters (i.e., pH for Method 1313 and L/S for Method 1316), analytes, and study materials were compared to precision statistics published for accepted leaching tests.

---

[6] This report uses the terms "coefficients of variation" (CVs) and "relative standard deviations" (RSDs). Although mathematically equivalent, these terms are used in the report to differentiate the analysis of variance sources (i.e., CVs for "within laboratory", "between laboratory" and "overall" standard deviations) from measures of method precision determined as the repeatability relative standard deviation (RSD_r) and reproducibility relative standard deviation (RSD_R).

STUDY MATERIALS

Three study materials – a coal combustion fly ash, a laboratory-formulated solidified waste material and field contaminated soil – were chosen for the methods validation of Method 1313 and Method 1316 in order to challenge the method performance for a range of typical waste types. The three materials were either collected from the field or created in the laboratory prior to homogenization and distribution to the participating laboratories.

Coal Combustion Fly Ash

A coal combustion fly ash (identified by material code EaFA) was used as the Phase I test material in order for participating laboratories to demonstrate proficiency with the test methods. A large sample of fly ash was collected in twenty-five, 5-gallon buckets from a coal-fired power plant located in the United States. Samples were homogenized by ARCADIS using coning and quartering techniques. The homogenized fly ash was returned to 5 gallon buckets and subsamples from three of the 25 buckets were taken for total content analysis by Method 3052/ICP-OES. Once homogenization was verified through comparison of total content subsamples, the fly ash was further divided into 1-kg portions placed into 1-L high density polyethylene (HDPE) containers for distribution to the laboratories. Six randomly selected 1-L containers (6 kg) were sent to each participating laboratory for triplicate testing of Method 1313 and Method 1316. The reference laboratory retained 12 randomly selected containers (12 kg), enough material to conduct six replicates of each test. Major species in the EaFA fly ash include Al, Fe, K, Si, and total of inorganic and organic carbon while minor species included B, Ca, Mg, Na, S, and Ti.

Solidified Waste Analog

For Phase II of the validation study, a cementitious material representing a solidified waste stream was created at VU and distributed to the study participants. The solidified waste analog (identified by material code SWA) was comprised of a powdered solid binder (Type I portland cement, class C coal combustion fly ash, and ground granulated blast furnace slag) and waste water at a water/binder ratio of 0.41 (m/m). The waste water used was tap water spiked with powdered metal oxides or metal nitrates of antimony, arsenic, barium, chromium, lead and selenium (Fisher Scientific). Final mix formulation in weight percent of the cured product is shown in Table 2.

The SWA material was mixed with shovels and hoes in an open trough until evenly blended. The cementitious material was packed into a series of 10-cm diameter by 20-cm long cylindrical molds and cured in a moist environment for at least 28 days. In preparation for batch testing, approximately 72 kg of cured solidified material was size reduced to maximum particle size of < 2 mm in a two-stage crushing process. The entire 72-kg batch of particle-size reduced material was homogenized in a barrel mixer and divided into a series of 1-L HDPE jars, each containing approximately 1 kg of material. Six randomly selected 1-L containers (6 kg) were distributed to each of the participating laboratories while 12 randomly selected containers (12 kg) were sent to the reference laboratory. Subsamples from five of the 2-liter jars were taken for total content analysis by Method 3052/ICP-OES. The major species in SWA included Al, Ca, Fe, Mg, Si, Na, and total carbon while Sb, As, B, Ba, Cr, P, K, Se, Sr, S, and Ti were detected as minor species.

Table 2. Mix Formulation for Solidified Waste Analog (SWA) Material.

Component	SWA (% by mass)
Type I portland cement	6
Class C fly ash	33
Blast furnace slag	33
Tap Water	26.3
$Na_2HAsO_4 \cdot 7H_2O$	0.11
$Ba(NO_3)_2$	0.06
K_2CrO_4	0.11
KCl	0.06
$Pb(NO_3)_2$	0.06
Sb_2O_3	0.06
$NaSeO_4$	0.08
NaOH	0.03
CH_3OONa	0.06
$NaNO_3$	0.01
$Na_2CO_3 \cdot H_2O$	1.03

Contaminated Field Soil

The other material tested in Phase II of the method validation study was a soil contaminated with heavy metals collected from a smelter site located in the United States. Approximately 320 kg of contaminated field soil (identified by material code CFS) was collected in 5-gallon plastic buckets and shipped to ARCADIS for processing. The entire batch of soil was sieved to pass a 2-mm opening in order to remove large rocks and other refuse and transferred to a clean blue plastic tarp for mixing by coning and quartering. After homogenization, the soil was divided into 1-L HDPE jars containing approximately 1-kg each for distribution to the participating laboratories. Each participating laboratory received six randomly selected jars (6 kg) of soil to be used in testing while the reference laboratory retained 12 randomly selected jars (12 kg). Subsamples from 12 randomly selected containers were taken for total mercury analysis and an additional three subsamples taken for total content analysis by Method 3052/ICP-OES. Total content analysis of CFS material showed that major species included Al, Ca, Cu, Fe, K, Si, Na, S, and Zn while minor species included As, Pb, Mg, Mn and Ti.

Total Content of Study Materials

The total contents of constituents in the three study materials are presented in Table 3. For the purposes of interpreting total content and describing these materials, analytes may be grouped into major, minor, and trace species as follows:

- Major species – analytes with total content of at least 10,000 mg/kg (i.e., 1 % by mass)
- Minor species – analytes with total content less than 10,000 mg/kg but at least 1,000 mg/kg
- Trace species – analytes with total content less than 1,000 mg/kg.

Total contents are based on either x-ray fluorescence spectrometry (XRFS) or a combination of microwave digestion of solid subsamples, performed by ARCADIS following EPA Method 3052 (EPA 1996) with chemical analysis of digestates conducted by ICP-OES at VU following EPA Method 6010 (EPA 2007b). All reported total content values for trace and minor species shown in Table 1 were

determined by EPA Method 3052/ICP-OES with the exception of boron. Since metaborate is added during the digestion process in Method 3052, total boron was reported as determined by EPA Method 3051 (EPA 2007A).

Table 3. Total Content of Study Materials.

Analyte	Symbol	EaFA mg/kg	SWA mg/kg	CFS mg/kg
Aluminum[a]	Al	130,000	59,000	34,000
Antimony	Sb	1.5	2,100	490
Arsenic	As	63	1,100	1,900
Barium	Ba	830	3,000	810
Beryllium	Be	15	3.5	0.39
Boron[b]	B	1,400	3,600	610
Cadmium	Cd	3.5	2.6	310
Calcium[a]	Ca	8,700	220,000	46,000
Carbon, inorganic[c]	TIC	1,400	2,000	600
Carbon, organic[c]	TOC	148,000	5,000	27,000
Chromium	Cr	120	1,200	240
Cobalt	Co	62	18	110
Copper	Cu	130	67	60,000a
Iron[a]	Fe	40,000	21,000	87,000
Lead	Pb	39	330	6,000[a]
Lithium	Li	84	4.3	1.80
Magnesium	Mg	3,700	33,000[a]	5,300
Manganese	Mn	110	900	1,700
Molybdenum	Mo	15	7.6	710
Nickel	Ni	89	25.0	80.0
Phosphorus	P	490	2,000	380
Potassium	K	18,000[a]	7,000	11,000[a]
Selenium	Se	24	1,300	52.0
Silicon[a]	Si	230,000	120,000	150,000
Sodium	Na	5,700	40,000[a]	11,000[a]
Strontium	Sr	610	1,300	280
Sulfur	S	1,500	8,200	64,000[a]
Thallium	Tl	0.91	1.1	29.0
Titanium	Ti	6,200	4,400	2,200
Vanadium	V	220	100	58.0
Zinc	Zn	100	86	25,000[a]

Notes:

All total content determinations by digestion using EPA Method 3052 and ICP-OES unless noted.

[a] Total content by XRFS (SOP No. 5003.3)

[b] Total boron by digestion using EPA Method 3051 (EPA, 2007a)

[c] Total organic and inorganic carbon by catalytic combustion EPA Method 9060 (EPA, 2004)

For the total content of major species in Table 2, total content was determined by XRFS conducted at ARCADIS on twelve subsamples of homogenized study material using a Philips model PW 2404 XRFS (PANalytical B.V., Almelo, the Netherlands) following a standard operating procedure (SOP), SOP No. 5003.3, maintained by ARCADIS. The RSDs for the twelve subsamples of study material formed a measure of the homogeneity of the material prior to distribution to the participating laboratories.

ANALYTICAL METHODS

In order to minimize uncertainties associated with participating laboratories applying different analytical techniques and analytical quality control, each participating laboratory was asked to ship preserved analytical solutions (i.e., filtered eluates with 1% by volume Optima grade nitric acid) under chain of custody to VU for chemical analysis. All eluates were analyzed at VU to minimized variability in the results associated with individual analytical methods and quality assurance/quality control (QA/QC) assessments. The concentrations of metal analytes were measured by ICP-OES (SW-846 Method 6010) on a Varian ICP Model 720-ES (Agilent Technologies, Santa Clara, CA). Table 4 presents the ICP-OES analytes and associated method detection limit (MDL) and minimum level of quantification (ML), determined by the analytical laboratory according to the EPA *Technical Support Document for the Assessment of Detection and Quantitation Approaches* (EPA 2003).[7]

Table 4. MDLs and MLs for ICP-OES.

Symbol	MDL (µg/L)	ML (µg/L)	Symbol	MDL (µg/L)	ML (µg/L)	Symbol	MDL (µg/L)	ML (µg/L)
Al	1.0	3.2	Cu	3.7	11.8	Se	15.0	47.7
Sb	7.5	23.9	Fe	2.0	6.4	Si	1.1	3.5
As	11.0	35.0	Pb	6.8	21.6	Na	2.5	8.0
Ba	1.0	3.2	Li	1.9	6.0	Sr	1.0	3.2
Be	1.7	6.0	Mg	1.0	3.2	S	6.8	21.6
B	1.0	3.2	Mn	2.0	6.4	Tl	4.6	14.6
Cd	2.2	7.0	Mo	1.2	3.8	Ti	2.0	6.4
Ca	2.6	8.3	Ni	1.8	5.7	V	1.5	4.8
Cr	1.2	3.8	P	3.7	11.8	Zn	1.0	3.2
Co	1.8	5.7	K	1.6	5.1			

Concentrations measured at values less than the MDL were reported as "non-detected," but set to a value equal to ½ the MDL value for plotting and data analysis. Concentrations measured at less than the ML but greater than the MDL are reported as "estimated values."

The ICP-OES analytical range for trace metals was calibrated using five-point standard curves whereas seven-point standard curves were used for major component analytical ranges between approximately 0.1 mg/L and 500 mg/L. During analysis of solutions, blanks and calibration check standards (~0.5 mg/L) were monitored every 10 to 20 samples with the requirement that recoveries be within 20% of the specified value. Analyses were performed on undiluted samples when possible and samples were diluted gravimetrically to within the targeted analytical range when necessary using 1% (v/v) Optima grade nitric acid (Fisher Scientific) in deionized water. Yttrium at 10 mg/L was used as an internal standard. Analytical matrix spikes were checked for three test positions for each triplicate analysis of a laboratory

[7] The analytical data quality indicators for this report are based on the guidelines established by the EPA Office of Water and include establishing a method detection limit (MDL) and minimum level of quantitation (ML) based on standard deviation of seven non-consecutive analyses of a low-concentration standard analytical solution. However, the EPA Office of Resource Conservation and Recovery (ORCR) has recommended that practitioners establish a lower limit of quantitation (LLOQ) for analytes of concern as a demonstration of quantitation capability at low analyte concentration levels. The LLOQ demonstration is a performance-based validation of recovery from a spiked analytical solution typically at concentration levels approximating the lowest calibration standard.

data set. For each analytical matrix spike, a volume of 500 µL of a 10 mg/L standard solution was added to 5 mL of sample aliquot.

Supplemental Analysis for Reference Laboratory Eluates

For the eluates resulting from the six test replicates conducted by the reference laboratory, the standard chemical characterization by ICP-OES was supplemented with analysis of Cs, Sn, and U by inductivity coupled plasma-mass spectroscopy (ICP-MS) and analysis of dissolved inorganic carbon (DIC) and dissolved organic carbon (DOC) by total carbon analysis. Supplemental analysis was conducted to address specific regulatory concerns (e.g., Cs, Sn, and U) and to document the dissolution of carbon species which can significantly influence leaching concentrations.

Prediction limits at the 95% probability level were calculated for all analytes (i.e., supplemental analytes plus ICP-OES analytes) from chemical analysis of the six reference laboratory test replicates to illustrate the range of within-laboratory data obtained during the validation study. The full set of analytical data is presented in Appendices E (Method 1313) and F (Method 1316) for the reference laboratory test results.

Inductively Coupled Plasma – Mass Spectroscopy

ICP-MS analysis following SW-846 Method 6020 (EPA 2007c) was carried out at VU using a Perkin Elmer model ELAN DRC II (Perkin Elmer, Waltham, MA) in standard mode. Initially, analyses for 10:1 dilutions were performed to minimize total dissolved loading to the instrument. Additional dilutions at 100:1 and 1000:1 were analyzed if the calibration range was exceeded with the 10:1 dilution. Internal standards consisting of 50 µL of a 10 mg/L indium (for mass range below 150) and bismuth (for mass range over 150) were added to 10 mL of sample aliquot prior to analysis. MDLs and MLs for ICP-MS analyses as determined by the analytical laboratory are shown in Table 5.

Table 5. MDLs and MLs for ICP-MS.

Symbol	MDL (µg/L)	ML (µg/L)
Cs	0.49	1.6
Sn	0.70	2.2
U	0.30	1.0

Total Carbon Analysis

Total carbon analysis following SW-846 Method 9060 (EPA, 2004) for all eluates was performed on a Shimadzu model TOC-V CPH/CPN (Shimadzu Scientific Instruments Inc., Columbia, MD) to determine the concentrations of DIC and DOC. Five-point calibration curves, for both DIC and non-purgeable DOC analyses, were generated for an analytical range between 5 ppm and 100 ppm with an acceptable correlation coefficient of at least 0.995. After every 10 samples, an analytical blank and calibration check standards at approximately 1 mg/L were measured and compared to acceptable QA/QC criteria. The recovery on standard checks was required to be greater than 85%. MDLs and MLs for DIC and DOC analyses as determined by the analytical laboratory are shown in Table 7.

Table 6. MDLs and MLs for Total Carbon Analysis.

Symbol	MDL (µg/L)	ML (µg/L)
DIC	130	410
DOC	170	550

DATA PROCESSING

Data processing includes all operations used to prepare collected data for use in statistical analyses including data validation (e.g., assessment of method blanks and associated data filtering) and transformation and interpolation to target pH values.

Method Blank Analysis and Data Filtering

As specified in both Method 1313 and Method 1316, each laboratory provided analytical solutions representing method blank extractions (i.e., extraction conducted without solid material, but otherwise carried through the process with the equipment and handling procedures as extractions with solid material). These method blanks were chemically analyzed by ICP-OES along with the test extractions and the results were used to identify potential sources of contamination (e.g., contact surfaces, contaminated reagents) that might bias the results of the test extractions. For cases where the method blanks or other process variables (e.g., pH, L/S) indicated that analyte concentrations in the test extractions may have been biased, removal or "filtering" of the corresponding test extraction result from the statistical analysis was considered. A more detailed discussion of method blank analysis and data filtering are presented in the results section.

Data Transformation and Linear Interpolation/Extrapolation to Target Values

Statistical analyses were performed on $\log_{10}$ transformed concentration results which had been interpolated to the target pH or L/S values designated in the respective methods. Log transformation is common statistical practice to lessen the impacts of extreme data values and render distributions closer to normal, thereby enhancing the suitability of statistical methods based on the normal distribution.

For Method 1313 data, interpolation of results to the target pH values was necessary to adjust for the tolerance in final pH value (± 0.5 pH units) and the strong effect of pH on eluate concentration for many elements. In some cases, extrapolation to either the lowest or highest target value was necessary.

Method 1316 data were reported at the target L/S values so that interpolation had little to no effect, but was carried out in order to adhere to a uniform data processing procedure. However, participating laboratories found it difficult, for some materials, to separate solid and liquid phases in low L/S extractions so that sufficient eluate volume was recovered for ICP-OES analysis. Thus, eluate solutions at an L/S value of 0.5 were not returned for two laboratories for EaFA, seven laboratories for SWA, and one laboratory for CFS. For these data sets, unrestricted extrapolation to target L/S values would result in extrapolated used in the statistical analysis where no laboratory data was provided and extrapolation was limited to only those points within 10% of an L/S value (e.g., ±0.1 L/S at target L/S of 1). Limited extrapolation prevented creation of interpolated or extrapolated data when a test position eluate was not submitted for chemical analysis by a participating laboratory.

In all cases, linear interpolation and extrapolation of the $\log_{10}$ transformed data was based on the concentrations recorded at the two data points nearest to the target value. For example, if data are returned with eluate pH values of 2.2, 4.2 and 5.2, the eluate concentration values at pH 2.2 and 4.2 are used to extrapolate to a target pH of 2.0 and interpolate to a target pH of 4.0.

The algorithm for interpolation is as follows:

> Given a set of coordinate data $\{ (x_i, y_i) : i = 1,...n \}$ sorted by the first coordinate (so that $x_1 < x_2 < \cdots < x_n$) and a *target* x-value, call it x_T, an interpolated/extrapolated y-value, call it y_T, is calculated as:
>
> $$y_T = a_T + b_T x_T$$
>
> where:
>
> - if $x_T < x_1$, then $b_T = (y_2 - y_1) / (x_2 - x_1)$ and $a_T = y_2 - b_T x_2$ (extrapolation from the two points with closest x-values);
> - if $x_T \geq x_n$, then $b_T = (y_n - y_{n-1}) / (x_n - x_{n-1})$and $a_T = y_n - b_T x_n$ (extrapolation from the two points with closest x-values);
> - if $x_{j-1} \leq x_T < x_j$, then $b_T = (y_j - y_{j-1}) / (x_j - x_{j-1})$and $a_T = y_j - b_T x_j$ (interpolation from the two closest points surrounding x_T).

For each analyte, statistical analysis of interpolated, $\log_{10}$ transformed concentration results focused on determination of the following statistical output.

STATISTICAL CALCULATIONS

All statistical calculations were implemented within a module of LeachXS. The module is designed to allow the user to aggregate or merge individual data sets (i.e., test replicates) into a single data set in order to output statistical analyses and/or interpolated/extrapolated data as an .xml file. The .xml file can then be imported back into the LeachXS materials database for visualization and comparison to other data sets.

95% Prediction Limits (PLs) based on Reference Laboratory Results

Using only the reference laboratory data set of six test replicates, a prediction interval for the mean of the data set at each target pH was constructed using standard normal distribution-based prediction approaches at a 95% prediction level (Rao, 1998; Ellison, 2009).

Suppose that there are n replicate laboratory measurements $y_1,...,y_n$. The sample mean ($\bar{y}$) and sample standard deviation(s) of these measurements are:

$$\bar{y} = (1/n)\sum_{i=1}^{n} y_i \text{ and}$$

$$s = \sqrt{[1/(n-1)]\sum_{i=1}^{n}(y_i - \bar{y})^2} .$$

The prediction interval is divided into an upper limit (PL_{upper}) and a lower limit (PL_{lower}) calculated as:

$$PL_{lower} = \bar{y} - t \cdot s\sqrt{1 + 1/n}$$

$$PL_{upper} = \bar{y} + t \cdot s\sqrt{1 + 1/n}$$

where t is the upper 0.025 critical value from the t distribution with n-1 degrees of freedom; the area to the right of t is 0.025, often denoted in literature as t (n-1, 0.025).

95% Robust Confidence Limits (RCLs) based on the Median of Laboratory Mean Data.

RCLs are defined as intervals about the median of the laboratory means constructed using robust confidence limits (Huber, 1968; Daszykowski et al., 2007) delineate the reproducibility operating characteristics across laboratories. In the case where 95% RCLs are calculated, one would expect 95% of all laboratories to produce a mean $\log_{10}$-transformed concentration value of three replicates to fall within these bounds. In order to lessen the impact of outlying results from a small subset of laboratories and, thus, to also facilitate identification of laboratories producing discrepant results, the limits were calculated substituting robust measures of location and scale, the median and median absolute deviation (MAD), for their more common non-robust counterparts, the mean and standard deviation (Maronna et al., 2006). This substitution also requires modification of the usual t-distribution critical values commonly seen in confidence and prediction intervals to ensure the desired coverage probabilities. The robust limits and the method of calculating adjusted critical values are described below.

For each laboratory data set, the arithmetic mean of the laboratory replicates is calculated as denoted by $\bar{y}_1,\ldots,\bar{y}_n$ where the subscript refers to the laboratory number. Note that in most cases $n=10$ for the targeted ten participating laboratories, but this number may differ when data are missing or filtered. The robust confidence limits depend on the median of the laboratory means (M) and the median absolute deviation MAD of this group of means:

$$M = \text{median}\{\bar{y}_1,\ldots,\bar{y}_n\},$$

$$MAD = \text{median}\{|\bar{y}_1 - \text{M}|,\ldots,|\bar{y}_n - \text{M}|\}.$$

The robust confidence intervals are constructed of an upper limit (RCL_{upper}) and a lower limits (RCL_{lower}) using the formulae

$$RCL_{lower} = M - 1.96\, C_n\, (1.4826)\, MAD,$$

$$RCL_{upper} = M + 1.96\, C_n\, (1.4826)\, MAD,$$

where the constants C_n for n = 4,..., 12, 100, 200 are given in Table 8.

The factor 1.4826 in the formulas for the robust confidence limits scales the MAD so that it is an unbiased estimator of the population standard deviation in large sample sizes when the data are normally distributed. The factor 1.96 is the 0.025 upper-tail critical value of the standard normal distribution commonly seen in formulas for 95% confidence intervals based on the sample mean and sample standard deviation. Although it would be mathematically equivalent to combine the product of C_n, 1.96 and 1.4826 into a single constant, keeping them separate makes evident that interpretation of the constants C_n in Table 8 as correction factors that: (i) adjust for small sample sizes (in a manner similar to the way that the t-distribution critical values adjust for small sample sizes relative to the standard normal critical values); and (ii) accommodate the fact that limits are constructed using the sample median and sample MAD (scaled by 1.4826) instead of the sample mean and sample standard deviation as estimators of the population mean and standard deviation.

Table 7. Constants C_n for Constructing the Robust Confidence Limits.

n	C_n	n	C_n	n	C_n	n	C_n
4	1.6233	12	1.2100	26	1.0967	76	1.0300
5	1.8633	13	1.2233	30	1.0833	100	1.0233
6	1.4433	14	1.1833	31	1.0833	101	1.0233
7	1.5033	15	1.1833	40	1.0633	200	1.0100
8	1.3300	16	1.1567	41	1.0633	201	1.0100
9	1.3500	20	1.1233	50	1.0500		
10	1.2567	21	1.1233	51	1.0500		
11	1.2700	25	1.1033	75	1.0300		

Because the median and scaled MAD values are consistent estimators of the mean and standard deviation of the normal distribution, the constants C_n are approximately 1 for very large sample sizes. Close inspection of Table 8 reveals that the constants decrease monotonically to 1 as n increases for all odd values of n, and for all even values of n, but that the change from neighboring even to odd n is not decreasing. This phenomenon results from the alternating definition of the median for odd and even sample sizes and diminishes in magnitude with increasing sample size.

The constants C_n were determined by Monte Carlo simulation so that the limits have the desired coverage properties when the laboratory means are a random sample from a normal distribution. Specifically, for each value of n in Table 8, one million samples of size n were generated from a standard normal distribution. For each sample, the fractions of the sample values lying between limits of the form $M \pm 1.96\ C_n\ (1.4826)$ MAD for a dense grid of values C_n were calculated. These fractions were then averaged over the one million samples and the value of c was identified that resulted in the average fraction being closest to 0.95 (and was always within 0.001 of 0.95). The Monte Carlo variation in the reported values of C_n is less than the number of decimal places displayed.

Although the constants were generated in such a manner that the intervals have a very precise interpretation for normally distributed data, their robustness (stemming from the use of the median and MAD) ensures their utility for identifying aberrant values from a set of data more generally then for just normally distributed data.

Estimates of Variance Components and Standard Deviations

The variance components are estimated using the approach of a standard random effects one-way ANOVA model in which the laboratories are considered the "treatments." The notation and formulas that follow are the same as in the book by Rao (1998; see in particular Section 14.3 and Box 14.2, pp 650-653).

The "within laboratory" standard deviation is associated with the repeatability of the method and is a statistical estimate of variability of replicate measurements from the same laboratory based on pooled information for all laboratories. Therefore, within-laboratory standard deviation is not specific to any particular laboratory. The "overall" standard deviation is associated with the reproducibility of the method and is used to indicate the combined effects of within-laboratory and between-laboratory variances.

Preliminary Calculations and Example ANOVA Table

In most cases, $t = 10$ laboratories and $n_i = 3$ or 6 for the participating laboratories and reference laboratory, respectively. However, these numbers can vary with missing (filtered) data.

$Y_{i,j}$ = the jth replicate measurement from the ith laboratory, $j = 1,...,n_i$, $i = 1,...,t$.

$$N = \sum_{i=1}^{t} n_i \qquad Y_{i,+} = \sum_{j=1}^{n_i} Y_{i,j} \qquad \overline{Y}_{i,+} = \frac{Y_{i,+}}{n_i}$$

$$Y_{+,+} = \sum_{i=1}^{t}\sum_{j=1}^{n_i} Y_{i,j} \qquad \overline{Y}_{+,+} = \frac{Y_{+,+}}{N} \qquad CM = \frac{Y_{+,+}^2}{N}$$

Sums of Squares – Defining Formulas and Calculation Formulas

$$\mathrm{SS[TOT]} = \sum_{i=1}^{t}\sum_{j=1}^{n_i}\left(Y_{i,j} - \overline{Y}_{+,+}\right)^2 = \left(\sum_{i=1}^{t}\sum_{j=1}^{n_1} Y_{i,j}^2\right) - CM$$

$$\mathrm{SS[T]} = \sum_{i=1}^{t}\sum_{j=1}^{n_i}\left(\overline{Y}_{i,+} - \overline{Y}_{+,+}\right)^2 = \left(\sum_{i=1}^{t}\frac{Y_{i,+}^2}{n_i}\right) - CM$$

$$\mathrm{SS[E]} = \sum_{i=1}^{t}\sum_{j=1}^{n_i}\left(Y_{i,j} - \overline{Y}_{i,+}\right)^2 = \mathrm{SS[TOT]} - \mathrm{SS[T]}$$

Table 8 shows how the preliminary calculations described above fit into the ANOVA table. The table proportions the overall or total error into sources of variation and accounts at each level for the degrees of freedom (*df*), the sum of square errors and mean square errors.

Table 8. Example ANOVA Table

Source of Variation	*df*	Sum of Squares	Mean Squares	F
Treatments	$t - 1$	SS[T]	MS[T]=SS[T]/*df*	F_{calc} = MS[T]/MS[E]
Error	$N - 1$	SS[E]	MS[E]=SS[E]/*df*	
Total	$N - 1$	SS[TOT]		

Variance Components and Standard Deviations

The "within laboratory" variance component, v_w, is simply the MS[E] term derived in the ANOVA table. The standard deviation associated with repeatability, s_r, is determined as the square root of the within-laboratory variance component:

$$s_r = \sqrt{v_w} = \sqrt{MS[E]}$$

The variance component associated with between-laboratory variance is:

$$(s_L)^2 = \frac{\mathrm{MS[T]} - \mathrm{MS[E]}}{D}$$

$$\text{where } D = \frac{1}{t-1}\left(\sum_i^t n_i - \frac{\sum_i^t n_i^2}{\sum_i^t n_i}\right).$$

The standard deviation associated with between-laboratory variance, s_L, is calculated as the square root of the between-laboratory variance component:

$$s_L = \sqrt{\frac{\mathrm{MS[T]} - \mathrm{MS[E]}}{D}}$$

In some cases, the between laboratories variance component may be negative and when it is, the variance value is set to zero. Although there are more complicated ways of dealing with the negative variance component problem, these approaches are not warranted in this application.

The total or overall variance component is the sum of the within-laboratory and between-laboratory variance components and the standard deviation associated with the overall variance, s_R, is associated with the method reproducibility:

$$s_R = \sqrt{(s_r)^2 + (s_L)^2}$$

Because the term, s_L, includes a divisor normalizing the variance to the average number of observations per laboratory, the approach is numerically consistent with the approach for calculating repeatability and reproducibility standard deviations in ASTM E691 *Standard Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method* (ASTM, 1987).

Repeatability and Reproducibility

The statistic that is associated with the repeatability of a method is the repeatability relative standard deviation, RSD_r, which is calculated as the within-laboratory standard deviation on a percentage basis and normalized to the overall mean value. The RSD_r is numerically equivalent to the within-laboratory coefficient of variation.

$$RSD_r = \frac{s_r}{|Y_{+,+}|} \times 100\%$$

The statistic that is associated with the reproducibility of a method is the reproducibility relative standard deviation, RSD_R, which is a percentage-based measure of the overall standard deviation to the mean value and numerically equivalent to the overall coefficient of variation.

$$RSD_R = \frac{s_R}{|Y_{+,+}|} \times 100\%$$

Horwitz Ratio (HorRat)

The Horwitz equation is an empirical relationship, based on data from a wide variety of analytical methods, which indicates how the precision is predicted to change with concentration levels (Horwitz and Albert, 2006; Mandel, 1991). When applied to the RSD_R values, the Horwitz equation takes the form:

$$PRSD_R = 2 \cdot C^{-0.15}$$

where $PRSD_R$ is the predicted Horwitz relative standard deviation (%) and
C is the concentration on a decimal fraction basis (e.g., 1 mg/L = 10^{-6})

The ratio of the calculated RSD_R value to the predicted value ($PRSD_R$) using the Horwitz equation (Horwitz and Albert, 2006; Mandel, 1991) is the reproducibility Horwitz Ratio ($HorRat_R$).

$$HorRat_R = \frac{RSD_R}{PRSD_R}$$

The Horwitz Ratio is used to account for the natural tendency for analytical replicate standard deviations to increase as the central concentration value decreases. In analytical chemistry, the HorRat values are used as a rough estimate of the analytical method precision with $HorRat_R$ values between 0.5 and 2.0 typically considered to represent "acceptable" analytical methods (Horwitz and Albert, 2006; Linsinger and Josephs, 2006). However, in the current method validation study, the observed overall standard deviation is a combination of the variability imposed by the extraction method (i.e., Method 1313 or Method 1316) and the analytical method, as well as the reference material heterogeneity. Thus, the Horwitz Ratio for reproducibility is used in this report only to assess of whether inherent precision associated with concentration levels accounts for a majority of the variation in the test results. Thus, $HorRat_R$ values greater than 2.0 do not indicate an unacceptable test method but simply indicate variability over-and-above that of the analytical method.

Reproducibility Limit

The reproducibility limit (R) was used to create an interval of possible results about the mean of the LEAF method data ($\bar{y}$) to show the consistency between LEAF methods results and analogous EU leaching methods.

ISO defines reproducibility limit as "the value less than or equal to which the absolute difference between two test results obtained under reproducibility conditions may be expected to be within a probability of 95%" (ISO, 1994). The reproducibility limit (R) is derived from the reproducibility standard deviation according to:

$$R = t \cdot \sqrt{2} \cdot s_R$$

where t is the Student's t-distribution value required for the 1-α level of confidence and the appropriate number of degrees of freedom, and

s_R is the reproducibility standard deviation.

Following the suggestion of Ellison et al. (2009), the value of t was approximated as $t=2$ to approach the Student's t-distribution value limit for a large number of degrees of freedom at the 95% confidence level. Thus, the R at the 95% confidence limit is calculated as:

$$R = 2.8 \cdot s_R$$

The reproducibility limit is applicable to data where errors are considered normally distributed and, thus, the calculation of reproducibility limit was conducted as a $\log_{10}$-tranform. For each pH target (Method 1313) or L/S target (Method 1316), the reproducibility limits above and below the mean of the validation

data (RL_{upper} and RL_{lower}, respectively) were calculated using the validation study mean ($\bar{y}$) and the reproducibility standard deviation for the $\log_{10}$-tranformed data ($S_{R,log}$):

$$RL_{upper} = \log(\bar{y}) + 2.8 \cdot S_{R,\log} \text{ and}$$

$$RL_{lower} = \log(\bar{y}) - 2.8 \cdot S_{R,\log}$$

When compared to the reproducibility limit interval (RL), the results from EU methods that fall within the reproducibility limit interval about the mean may be considered statistically equivalent to the results of the LEAF method.

PHASE I LABORATORY FEEDBACK (METHODS 1313 AND 1316)

The objectives of the method validation study Phase I were (i) to allow participating laboratories the opportunity to demonstrate proficiency in performing Method 1313 and Method 1316 on the EaFA fly ash material and (ii) to generate feedback from the participating laboratories on the clarity and usability of the test method and Excel data templates provided for method setup calculations and recording laboratory data/observations.

Prior to shipment of any samples, participant laboratories were offered the opportunity to participate in a series of conference call meetings addressing an overview presentation and briefing on the interlaboratory validation study procedures and details of the test method.[8] While not all laboratories participating in all conference calls, the majority of laboratories participated in at least one conference call. For each material in each method, a package consisting of a designated quantity of the reference material, material descriptions and material safety data sheet (MSDS), method validation instructions, and sample tubes and adhesive labels for eluate analytical samples and archiving was shipped to each laboratory. Feedback on the clarity and operability of the test methods was solicited through a request of participating laboratories to complete an enclosed questionnaire. The primary observations from the information conference call discussions and questionnaire feedback from the participant laboratories included:

- Training – Overviews of the test method procedures, in the form of a Microsoft PowerPoint® presentation delivered during a conference call briefing, proved to be a valued aspect of the study. This feedback suggests the future need for some form(s) of training materials (e.g., presentation, videos, etc.) to provide an introduction to the methods.
- Method Clarity – Several typos and unclear passages were highlighted. Specific procedural clarifications were needed to add tolerances about the contact times for each particle size.
- Data Templates – Although the Excel spreadsheets were seen as a useful data management tool, several suggestions were received for clarifying the instructions for using each data template.
- pH Measurement – More clearly indicating that timely measurement of final eluate pH directly after collecting aliquots or after completion of the filtration step was needed. Initially, some laboratories were waiting a prolonged interval (e.g., days) before measuring final pH, which

[8] See http://vanderbilt.edu/leaching for more information on LEAF including test methods, data templates, and data management approaches.

resulted in an apparent drift in pH in unpreserved samples. A revision to the test method has been made to require measurement of final pH within 1 hour of completion of the extraction step.

- pH Meter Calibration – In addition to timely pH measurement, an accurately calibrated pH meter is crucial. The pH calibration standards used in typical two- or three-point pH meter calibrations (e.g., pH values of 4, 7, and 10) do not cover the full pH range required in the test method. The effect of pH measurement inaccuracies is especially evident at extreme values where pH measurements may be extrapolated up to 3 pH units beyond common calibration standards. Therefore, a wider calibration range is needed with additional pH buffer standards solutions, which are available at a variety of pH values between pH 1.68 and 12.45.
- Storage of Stock Solutions – Stock solutions of sodium hydroxide or potassium hydroxide should not be stored in borosilicate glass containers because of the possibility of solution contamination with boron from the leaching of the glass container which can result in interference with data interpretation.

As a direct result of these consultations, revisions to the method text and data templates were made between Phase I and Phase II of the validation study to address typos and suggested clarifications, contact time interval thresholds, pH measurement timing and calibrations, and compatibility of containers for stock reagent solutions. None of these revisions were considered to have changed the procedure or affected the results of the validation. The revised Method 1313 and Method 1316 texts are including as Appendix A and Appendix B of this report, respectively.

QA/QC SUMMARY

Quality assurance/quality control methodologies in this report include statistical analysis of total contents replicates, replication and spike recovery analysis during chemical analysis by ICP-OES, method blank analysis, and general visual data consistency checks. QA/QC ensured that (i) study materials were adequately homogenized prior to distribution to participating laboratories, (ii) chemical analyses of eluate samples were of sufficient quality, (iii) the reported data was not influenced by outside sources of contamination to a significant degree.

Homogeneity of Study Materials

Homogeneity of collected and processed study material was determined by the RSDs of triplicate total content analyses following either XRFS or EPA Method 3052/ICP-OES. The DQI goals for acceptable homogeneity were that RSD values from XRFS of replicate material subsamples would be less than 10% for major species, 20% for minor species and 50% for trace species. Table 10 shows the overall mean RSD and completeness (percentage of measured values complying with the RSD goal) as derived from XRFS of total content in each of the three study materials.

Both EaFA and SWA meet and exceed the criteria for homogeneity established in the QAPP. Based solely on the data shown in Table 10, the 47% RSD for CFS is driven by XRFS analysis of two minor species – chromium and magnesium – with very large RSD values. Since magnesium is not used as a selected analyte, removal of magnesium from the homogeneity assessment results in a mean RSD for minor analytes in CFS of 25% with a minor analyte completeness of 83% and an overall completeness of 80%. These DQI values for homogeneity were considered close enough to the DQI goals to conclude that all study materials were homogenous prior to distribution to the participating laboratories.

Table 9. Homogeneity QA/QC for Total Content Derived from XRFS

Analyte Type	Total Content (mg/kg)	DQI Goal for RSD	Mean RSD		
			EaFA	SWA	CFS
Major Species	≥ 10,000	< 10%	1.4%	1.1%	7.4%
Minor Species	< 10,000 to ≥ 1,000	< 20%	3.9%	3.6%	47%
Trace Species	< 1,000	< 50%	23%	11%	34%
		Overall Completeness	95%	100%	77%

Analytical QA/QC

DQI goals and overall results for critical measurements are shown in Table 11. The results for precision were calculated as that overall mean of RSD values for parameters with more than two replicates (i.e., ICP-OES and ICP-MS analyses, XRFS, and moisture content). Completeness was determined as the percentage of valid measurements meeting DQI goals out of the total number of measurements. The table shows that the DQI goals established in the QAPP were obtained or exceeded on a global basis in the validation study except for XRFS analysis as discussed earlier.

For the selected analytes used in the validation study, chemical analysis of eluate solutions was determined using ICP-OES data; therefore, QA/QC focused primarily on validation of ICP-OES eluate concentrations. Summary DQI results for ICP-OES analyses for each material by material, analyte and test are provided in Appendix H while full analytical QA/QC is presented in Appendix I.[9]

Table 10. DQI Goals and Overall Results

Measurement	Method	Goals		Overall Results	
		Precision	Completeness	Precision	Completeness
ICP-OES	EPA Method 6010	±10%	>90%	2%	99%
pH, conductivity	Electrode	±2%	100%	2%	100%
moisture content	ASTM D2216-05	±10%	100%	0.2%	100%
XRFS	SOP No. 5003.3	±10%	100%	14%	91%

The breakdown of the DQIs for ICP-OES analysis of eluate solutions by method and material shown in Table 12 indicates that, although some analytes are more difficult to quantify, data quality is consistently better than DQI goals for all analytes. While measurement of some analytes (e.g., antimony, arsenic) tended toward higher RSDs than that of other analytes (e.g., calcium, barium, boron), the mean RSD for any and all analytes was less than the DQI goal of 10%.

[9] Appendix I contains all of the details of the ICP-OES analysis and QA/QC results for each measured constituent in each provided analytical solution (i.e., filtered and preserved eluate sample). Therefore, due to its size, the appendix is made available electronically by request to the authors, through the link to the document page on the EPA website, or as a download at http://vanderbilt.edu/leaching.

Table 11. DQIs for ICP-OES Analysis Selected Analytes.

Analyte	Mean RSD	Std Dev Mean RSD	Mean Completeness	Max Spike Recovery	Min Spike Recovery	Materials
Antimony	4.2%	2.0%	97.4%	118%	83%	EaFA, SWA, CFS
Arsenic	3.9%	1.7%	97.8%	120%	84%	EaFA, SWA, CFS
Barium	1.2%	0.6%	99.9%	120%	80%	EaFA, SWA, CFS
Boron	1.4%	0.6%	99.9%	118%	81%	EaFA, SWA, CFS
Cadmium	1.1%	0.4%	99.8%	118%	86%	CFS
Calcium	1.2%	0.6%	100.0%	117%	81%	EaFA, SWA, CFS
Chromium	2.6%	1.5%	98.5%	117%	86%	EaFA, SWA
Cobalt	2.9%	1.4%	99.8%	118%	83%	EaFA, SWA
Lead	1.3%	0.5%	99.3%	112%	85%	CFS
Molybdenum	2.6%	1.7%	98.7%	119%	81%	EaFA, SWA, CFS
Selenium	2.8%	1.6%	98.2%	120%	82%	EaFA, SWA, CFS
Vanadium	2.1%	1.0%	99.9%	118%	83%	EaFA, SWA, CFS

During analysis of eluate solutions, analytical blanks and continuing calibration check standards (~0.5 mg/L) were monitored every 10 to 20 samples. All calibration checks were within 20% of the specified value and analytical blanks were measured at less than the ML. Analytical matrix spikes were checked for three test positions of each set of triplicate eluates with spike recoveries ranging between 80% and 120%. These results are consistent with the goals established in the QAPP and indicate that QA/QC goals for calibration checks, blanks and analytical spikes were met in all cases.

Method Blank Analysis

The LEAF test methods specify the procedure for conducting blank extractions (i.e., QAQC extractions without solid material) in order to assess the importance of potential sources of contamination such as reagents or equipment surfaces. During analysis of Phase I eluate concentrations, observable analyte concentrations were measured in the method blanks for both Method 1313 and Method 1316. The process of determining if these blanks represented a significant impact on the statistical results of this study is presented in Appendix D.

An algorithm was developed to "filter" the test data by removing test positions where the associated blank concentrations were 20% or greater of the eluate concentrations. The algorithm resulted in removal of less than 20% of the data used in the statistical analysis for each analyte (average 6.9%; standard deviation of 7.3%). However, comparison of data spread parameters between filtered and non-filtered data indicated no overall effect in statistics due to blank analysis data filtering. Therefore, data filtering based on method blank analysis was not considered in Phase II of the validation study.

Data Filtering for Cause

While filtering because of high method blank concentration was not considered to significantly affect the statistical results, inconsistencies in the comparison of data were observed which lead to procedural or other external sources of errors. For analytes where these error sources were identified (e.g., high sulfur in L04 samples for the EaFA material for Method 1313 resulting in low barium eluate concentrations due to precipitation of $BaSO_4$), eluates were "filtered for cause" as shown in Table 13. The primary sources of filtering for cause is improper pH measurement due potentially to calibration to a narrower set of buffer solutions than the pH range to be analyzed. In all, filtering for cause represented removal of less than 20% of the data for any analyte in any data set.

Table 12. Overview of Eluates Filtered for Cause

Material	Laboratory	Position(s)	Replicate(s)	Analyte(s)	Rationale for Filtration
Method 1313					
EaFA	L04 Ref	T01-T09 T01	A, B, C A, B, C	Barium Boron	High sulfur precipitates $BaSO_4$ NaOH stored in borosilicate glass
SWA	L02 L05	T01-T09 T01-T09	A, B, C A, B, C	All All	Inconsistent pH measurement Inconsistent pH measurement
CFS	-	-	-	-	No filtering for cause required
Method 1316					
EaFA	L05 L10 L11	T01-T05 T01-T05 T01-T05	A, B, C A A, B, C	All All All	Inconsistent pH measurement Inconsistent pH measurement Inconsistent pH measurement
SWA	L05	T01-T05	A, B, C	All	L/S offset due to moisture content
CFS	-	-	-	-	No filtering for cause required

ANALYTE SELECTION AND DATA TRANSFORMS

A screening evaluation of the reference laboratory Method 1313 and Method 1316 data for each of the three study materials is presented in Table 14. Check marks in the table indicate analytes for reference laboratory Method 1313 results with no more than 3 test positions below the MDL value or Method 1316 results with no more than 1 test position below the MDL value. Selected analytes are indicated by yellow highlighting. Toxicity characteristic (TC) priority metals based on the RCRA program are shown in red. Based on the ICP-OES results of the reference laboratory concentrations, a set of 10 analytes for each material was selected for statistical evaluation.

The selection of analytes for statistical analysis considered: (i) relevance to potential risks to human health and the environment (e.g., TC metals), (ii) representativeness of the range of characteristic pH-dependent leaching behaviors as a function of pH, and (iii) concentrations at sufficient level to allow a single undiluted ICP-OES analysis. Priority was given to analytes present in all three materials so that comparisons across material types could be made.

Table 13. Candidate ICP-OES Analytes and Selected Analytes for Statistical Analysis.

Analyte	Symbol	M1313 EaFA	M1313 SWA	M1313 CFS	M1316 EaFA	M1316 SWA	M1316 CFS
Aluminum	Al	✔	✔	✔	✔	✔	✔
Antimony	Sb	✔	✔	✔	✔	✔	✔
Arsenic	As	✔	✔	✔	✔	✔	✔
Barium	Ba	✔	✔	✔	✔	✔	✔
Beryllium	Be						
Boron	B	✔	✔	✔	✔	✔	✔
Cadmium	Cd			✔	✔		✔
Calcium	Ca	✔	✔	✔	✔	✔	✔
Chromium	Cr	✔	✔		✔	✔	
Cobalt	Co		✔		✔		✔
Copper	Cu			✔			✔
Iron	Fe		✔			✔	
Lead	Pb	✔		✔		✔	✔
Lithium	Li	✔	✔	✔	✔	✔	✔
Magnesium	Mg	✔	✔	✔	✔		✔
Manganese	Mn		✔		✔		✔
Molybdenum	Mo	✔	✔	✔	✔	✔	✔
Nickel	Ni		✔		✔		✔
Phosphorus	P	✔	✔	✔	✔	✔	✔
Potassium	K	✔	✔	✔	✔	✔	✔
Selenium	Se	✔	✔	✔	✔	✔	✔
Silicon	Si	✔	✔	✔	✔	✔	✔
Sodium	Na	✔	✔	✔	✔	✔	✔
Strontium	Sr	✔	✔	✔	✔	✔	✔
Sulfur	S	✔	✔	✔	✔	✔	✔
Thallium	Tl			✔	✔		✔
Titanium	Ti						
Vanadium	V	✔	✔	✔	✔	✔	✔
Zinc	Zn			✔	✔	✔	✔
Total Selected Analytes		**10**	**10**	**10**	**10**	**10**	**10**

Notes:

TC priority metals are shown in red text.

✔ indicates analytes with no more than three Method 1313 test positions below MDL or one Method 1314 test position below MDL (based on reference laboratory results).

Yellow shade indicates analytes selected for statistical analysis.

METHOD 1313 RESULTS AND ANALYSIS

Acid/base Neutralization Capacity (Titration Curve)

One of the outcomes of performing Method 1313 on a material is that the neutralization capacity of the material is determined by the amount of acid or base added to each extraction and the resultant eluate pH response. Figure 1 shows the acid neutralization capacity (ANC) and base neutralization capacity (BNC) of each of the study materials as a function of the eluate pH for the collected Method 1313 data from the participating and reference laboratories.

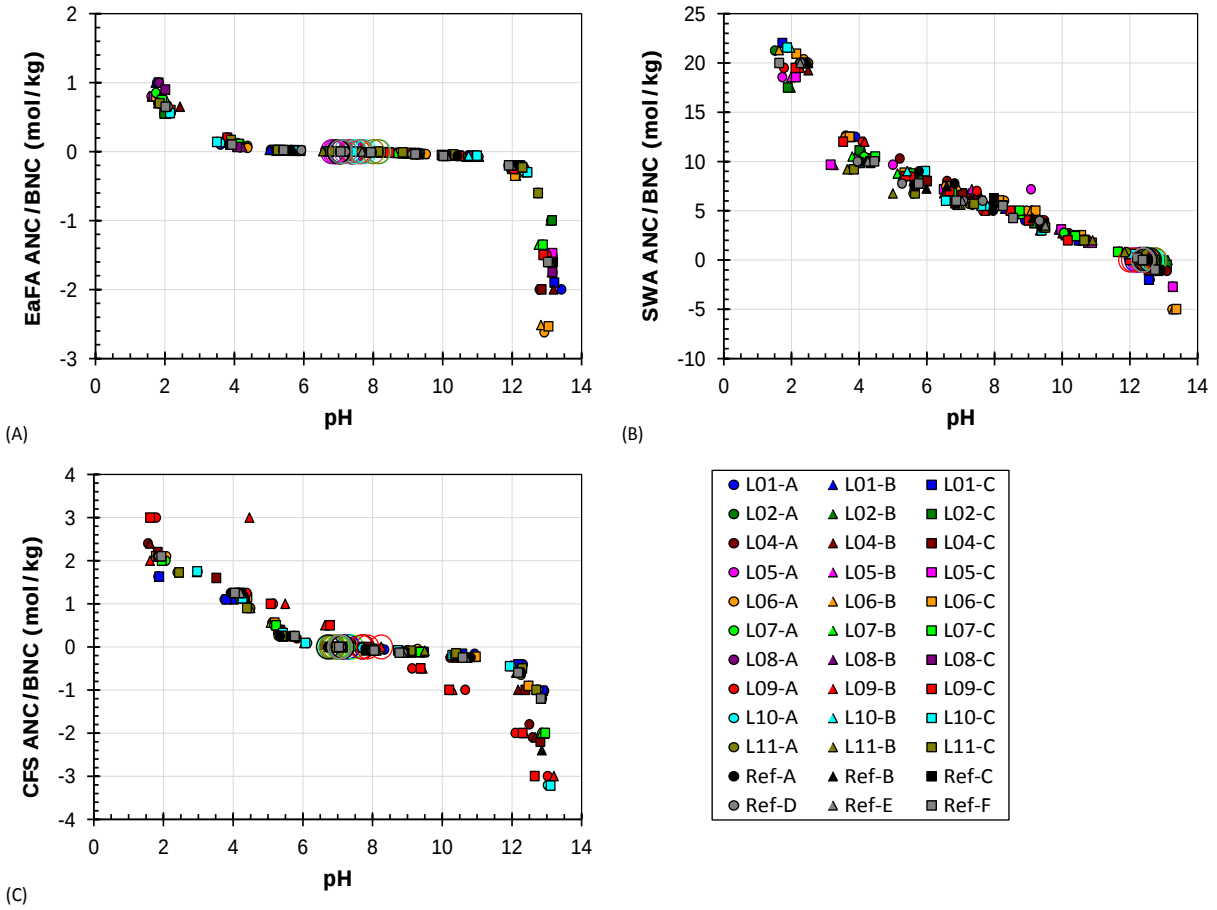

Figure 1. Acid/base neutralization capacity for Method 1313 study materials.

Note: Data shown for (A) EaFA coal combustion fly ash, (B) SWA solidified waste analog, and (C) CFS contaminated field soil. Addition of base is indicated by negative values on the y-axis.

Also shown in the figure are color-coded, large open circles which denote the natural pH measurement at an ANC/BNC equal to 0 mol/kg. ANC indicates the amount of buffer capacity that the material has with regard to acid addition; conversely the base neutralization capacity BNC is a measure of the buffering capacity of the material to base addition. Typically, ANC is reported in moles of acid per kg of material and BNC is expressed as a negative ANC on a continuum scale.

Of the three study materials, the SWA material (Figure 1B) is the most alkaline with a natural pH between pH 12 and 13) whereas both EaFA (Figure 1A) and CFS (Figure 1C) are much less alkaline with natural pH values between 6.5 and 8. Due to the alkalinity of the SWA material, the amount of acid required to decrease the final eluate pH of SWA to the lowest target pH of 2.0 was approximately 20 mol/kg. This value is significantly higher than the amounts of acid required to titrate CFS or EaFA to a target pH of 2.0, respectively, 2 mol/kg and 1 mol/kg.

Statistical Analysis of pH-dependent Leaching

For Phase II of the Method 1313 validation study, the experimental results of Phase I were combined with those results from conducting Method 1313 on two additional materials, SWA solidified waste analog and CFS contaminated field soil, to generate statistics related to method repeatability and reproducibility. The results of statistical analysis for three study materials tested using Method 1313 (i.e., EaFA coal combustion fly ash, SWA solidified waste analog, and CFS contaminated field soil) are presented as six-panel figures in Appendix E. Each figure shows the results of statistical analysis for a single selected analyte in each material (e.g., calcium in EaFA, boron in SWA). In the discussion below, selected panels from these figures are used to illustrate the key observations of the method validation.

Antimony in EaFA study material is presented in Figure 2 for illustrative purposes. The panels in the figure include:

Panel A – Collected data from participating laboratories that have been "filtered for cause" according to the blank analysis and filtration rules presented in Appendix D. Open circles around certain data points indicate the natural pH for each test replicate.

Panel B – Comparison of reference laboratory mean (green dots) and 95% prediction limit (PL; green dashed lines) to median of all laboratory means (red squares) and 95% robust confidence limit (RCL; red solid lines). The 95% prediction limits provide the bounds within which 95% of additional test replicates conducted by the reference laboratory would fall. The 95% confidence interval represents that bounds within which the mean concentration value from 95% of laboratories would fall.

Panel C – Overlay of the RCLs from Panel B against the interpolated/extrapolated data.

Panel D – Overall data mean (red dots) with standard deviations intervals about the mean associated with "within-laboratory" variance (green short-dashed line), "between-laboratory" variance (blue long-dashed line), and overall variance (gold solid line).

Panel E – The coefficient of variation corresponding to the "within-laboratory" (green short-dashed line), "between-laboratory" (blue long-dashed line) and "overall" (gold solid line) standard deviations as a percentage of the mean analyte concentration.

The sixth panel of each figure is a legend indicating color-coding by participating laboratory and shape-coding for test replicates applied to the collected (Panel A) and interpolated/extrapolated data (Panel C).

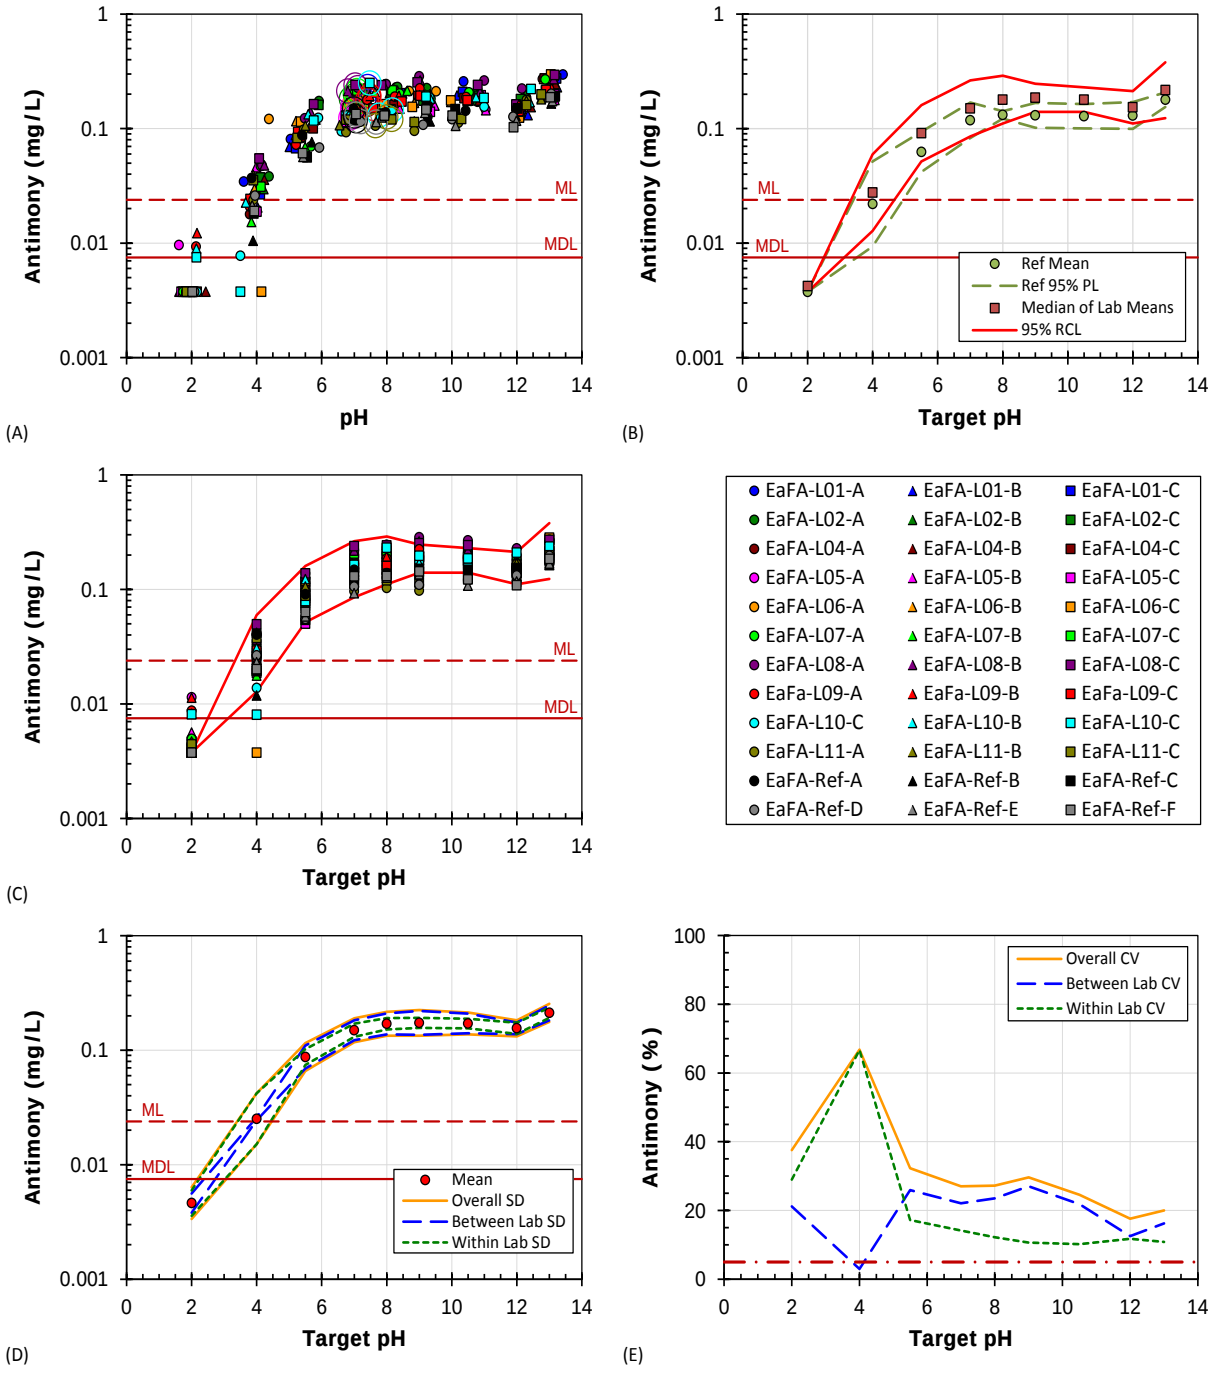

Figure 2. Antimony statistical analysis for Method 1313 Phase I material EaFA.

Note: Data shown for (A) collected data as a function of pH; (B) reference laboratory mean and 95% prediction limits (PL; green, dashed line) compared to the median of laboratory means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated laboratory data; (D) intervals for "overall" (gold line), "between laboratory" (blue, dashed line) and pooled "within laboratory" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between laboratory" and "within laboratory" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

Interpolation/Extrapolation of Log_{10}-transformed Data

Linear interpolation and extrapolation was chosen for its simplicity and ability to be understood easily and replicated. However, the method may contribute to the variability of some analytes in a narrow pH domain where the concentration curve varies over an order of magnitude or more as a function of eluate pH. Comparison of the data shown in Figure 3 illustrates the effect of interpolation and extrapolation on organizing the data for statistical analysis.

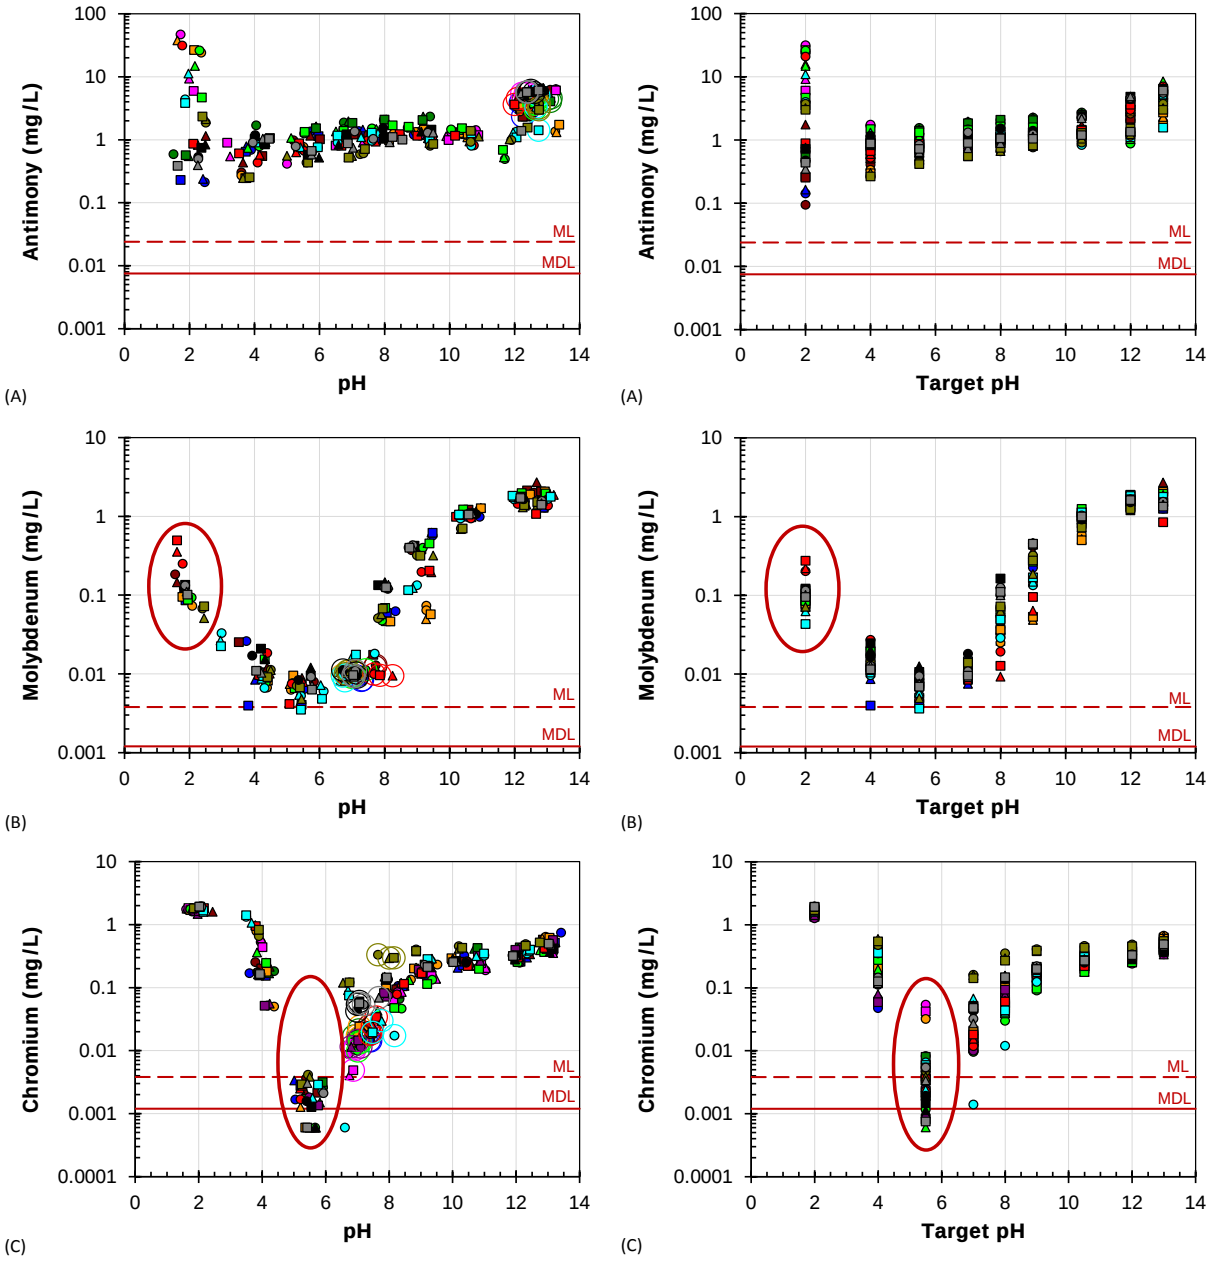

Figure 3. Comparison of Method 1313 collected data (left) and interpolated data (right).

Note: Data shown for (A) Sb in SWA material showing no significant change to variability, (B) Mo in CFS material showing minor degree of induced variability, and (C) Cr in EaFA showing significant variability as a creation of points in data "trough". Large red circles highlight examples of significant variability due to the interpretation approach.

Since Method 1313 does not call for automatic pH-control but specifies an allowable pH-tolerance about a target pH, the collected data (Figure 3A) vary with both pH and concentration. Interpolation and extrapolation of results to the target values allowed for statistical analysis at common points in the response curve of concentration as a function of pH and for comparison of different data sets at common pH values.

How variability is introduced through the interpolation/extrapolation process can be illustrated using the Method 1313 aluminum data from the SWA material. In Figure 4, eluate aluminum concentrations collected from the participating laboratories are plotted as greyed open dots along with a solid grey line indicating a visual "best fit" line of the collected data. Although not correlated to any particular mathematical function, the best fit line represents the general function of concentration versus pH to be referred to as "the function line". The blue and green lines in the figure indicate potential pairings of data which might represent candidate pairs for interpolation.

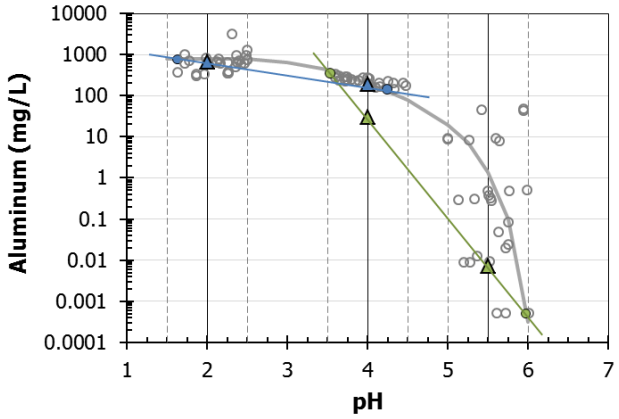

Figure 4. Linear interpolation of log_{10}-transformed Method 1313 data showing potential for increasing data scatter when interpolating along steep slopes.

The curvature of the function line related to the blue linear interpolation data set is shallow and the points interpolated to target pH values of 2.0 and 4.0 (blue triangles) display consistency with the clusters of collected data (grey open dots). However, interpolation along the green line where the curvature of the function line is steep can result in interpolated points that induce scatter in the data set. Two cases are shown in the example.

- The additional scatter from interpolation may be consistent with the variability of the collected data (see interpolated data point for target pH 5.5). This is likely to occur when the curvature of the function line is steep and small experimental errors in pH measurement can result in significant variation in collected concentration data.
- The introduced scatter due to interpolation may provide variability not provided by the collected data (e.g., at target pH 4.0).

Ideally, interpolation along the overall function line, as opposed to linearly between data points, would not induce such variability. However, interpolation along the function line would require extensive knowledge of the function line for each test replicate and, therefore, is not practical for this study. Thus,

linear interpolation and extrapolation was chosen for its simplicity and transparency despite the potential to scatter data when interpolation is conducted along steeply curved function lines.

Prediction Limit and Robust Confidence Limits

A selection of mean-based prediction limits for the reference laboratory data and median-based robust confidence limits for all data are shown in Figure 5 for various study materials. These graphs cover a broad spectrum of the statistical results. The full set of graphs is included in Appendix E.

The 95% prediction limits (PL; green dashed line) define a band of data about the reference laboratory mean (green dot) that delineates a repeatability operating characteristic for the reference laboratory in the sense that one would expect 95% of all replicate measurements made by the reference laboratory to lie within these bounds. However, this does not mean that an entire test replicate data set would fall within the bounds of the prediction limits for each of the nine target pH values since the parallel extractions in Method 1313 are independent. The 95% robust confidence limits (RCL; red solid lines) were calculated by merging all laboratory data, calculating the median of the laboratory means and setting the 95% confidence interval about that median.

The width of the robust confidence limits, or the interval between the upper and lower RCL plotted at a target pH, was approximately a factor of 2 in the pH domains of good repeatability for all analytes. Greater width was observed for the RCL when (i) the analyte concentration as a function of pH was at a local minimum (e.g., between pH 5.5 and 7.0 for As), and (ii) when the slope of the change in $\log_{10}$(concentration) as a function of pH was greater than 5 (e.g., at pH $\leq$ 4.0 and $\geq$ 12.0 for As). The width for the PL generally was either similar to or smaller for the PL as compared to the width of the RCL for all elements.

In general, there was good agreement between the PL and the RCL which indicates that the reference laboratory data are consistent with the data set as a whole. Figure 5 shows that the PL intervals for calcium in EaFA (Figure 5A left) and arsenic in CFS (Figure 5A right) fall directly within the RCL intervals and do not extend past the bounds of the RCL. Less agreement was seen for other species (Figure 5B and C) and associated with measured values near or less than the MDL.

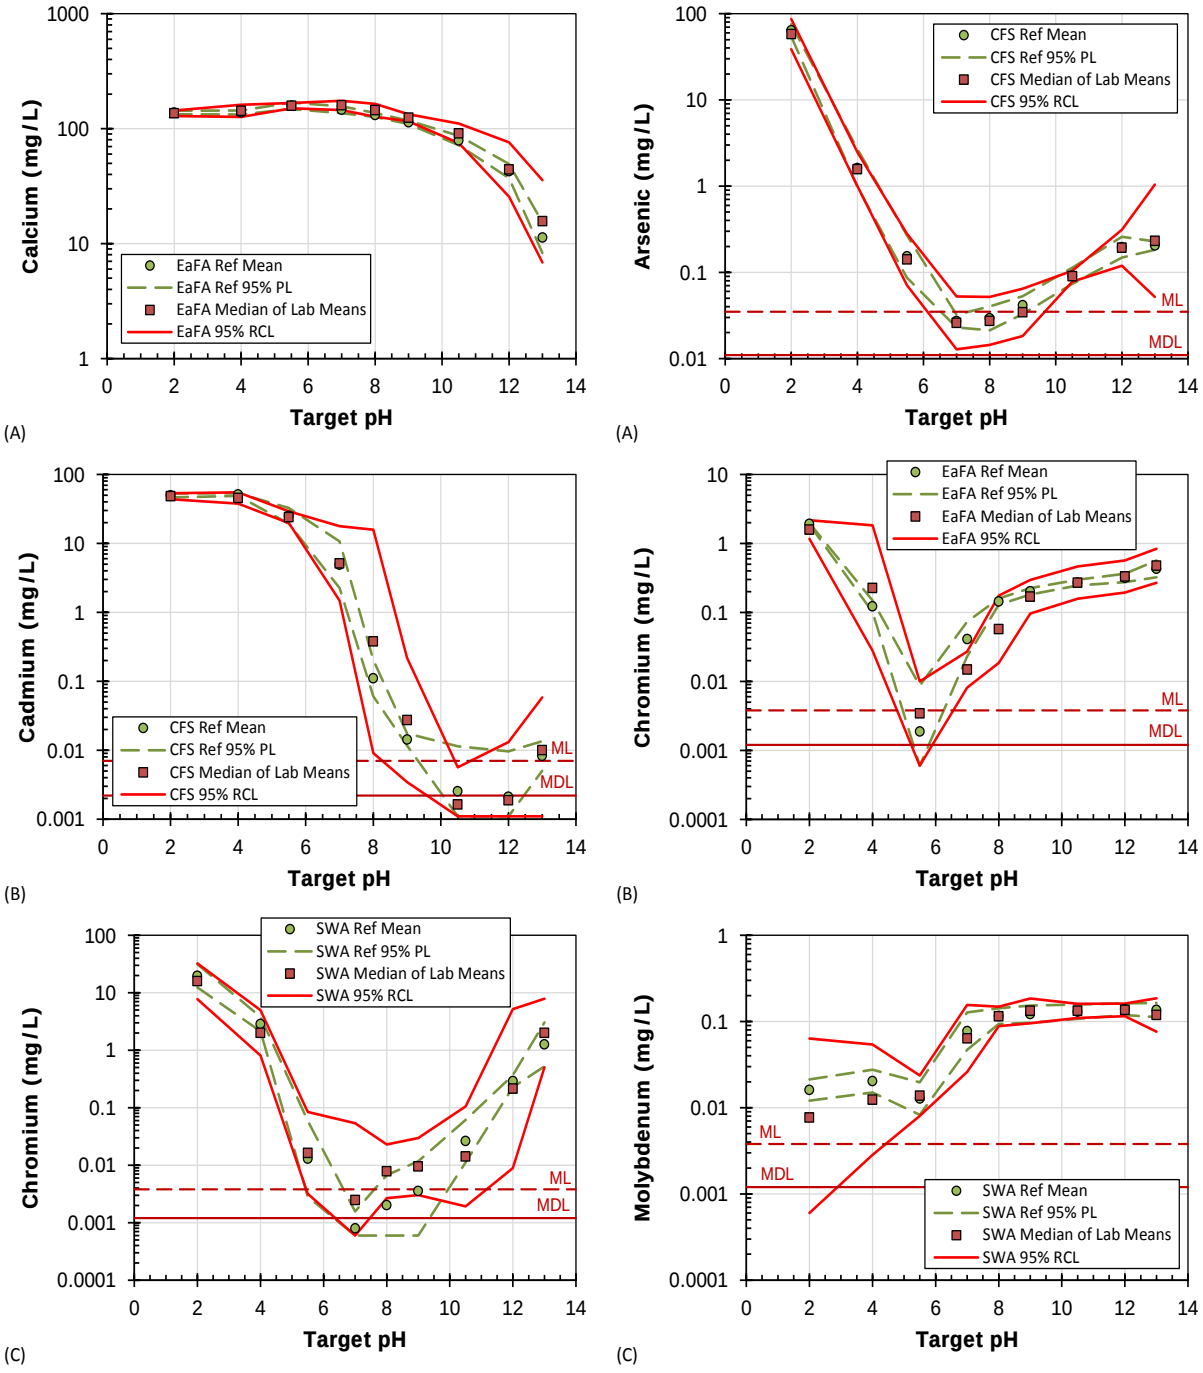

Figure 5. Agreement between 95% prediction limits (95% PL) about the mean of the reference laboratory data and 95% robust confidence limits (95% RCL) based on the median of laboratory means.

Note: Data shown for (A) high level agreement, (B) median level agreement, and (C) lowest level of agreement.

Some of the variability seen between PL and RCL data is introduced through the linear interpolation/extrapolation process. The propagation of variability due to interpolation of collected data is clearly shown when looking at Method 1313 data for arsenic in SWA (Figure 6). In the pH range

between 9 and 12, the collected participating laboratory data for arsenic follows a well-defined "U-shaped" function line (yellow dashed line in Figure 6A). Because interpolation is conducted linearly between target pH values (e.g., 9, 10.5 and 12), the resulting interpolated concentrations (Figure 6B) spread significantly at pH targets of 10.5 and 12. The data for the reference laboratory are pushed into the "bowl" of the U-shaped trend at pH 10.5 such that the mean of the reference laboratory data is noticeably higher than the median of laboratory means for the data set as whole (see Figure 6C). In addition, the considerable spread in the interpolated data (Figure 6B) at pH 12 is caused by the interpolation to a nearly vertical function line. This spread in the interpolated data results in a broader than expected range of concentrations and a wider than expected 95% robust confidence interval at pH 12.

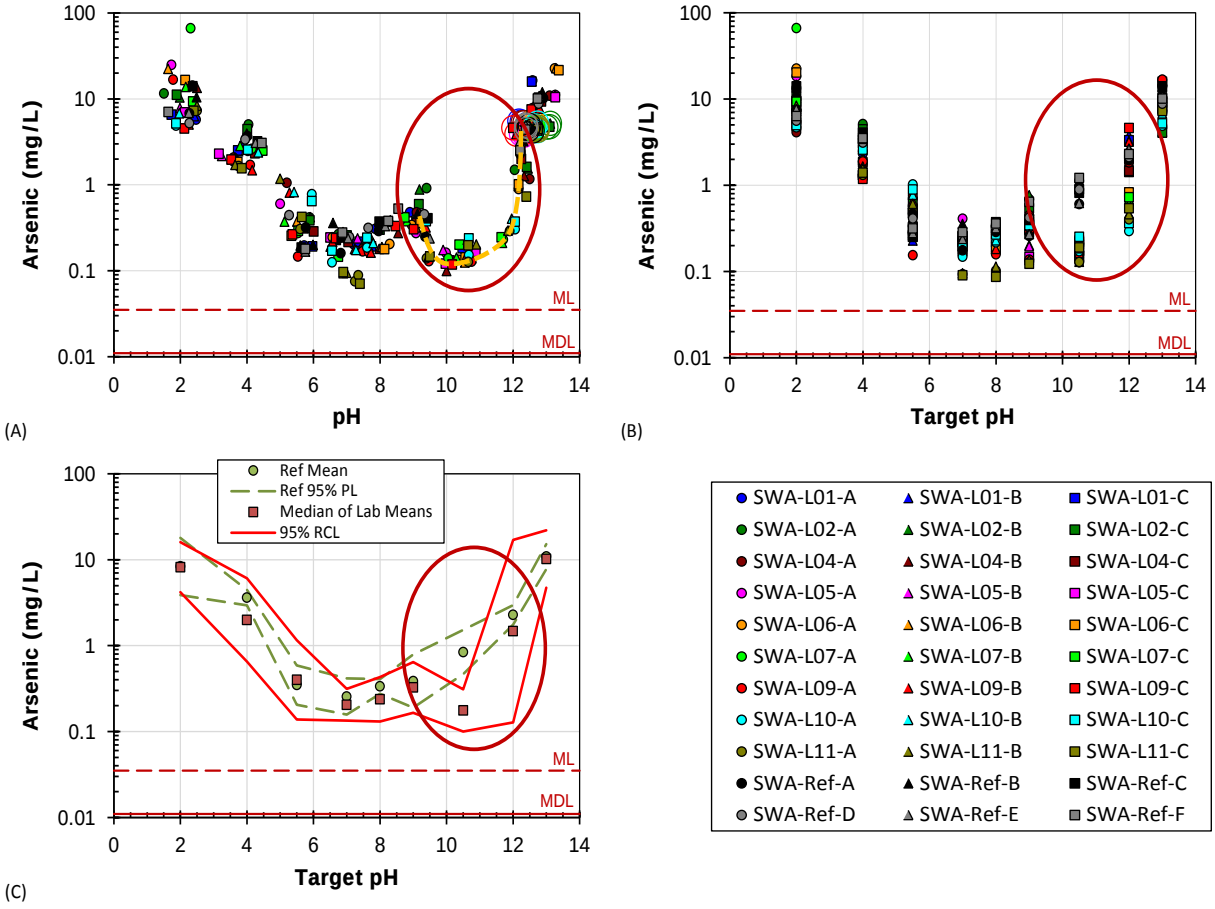

Figure 6. Propagation of variability due to linear interpolation of arsenic concentrations in Method 1313 samples of SWA.

Note: Data shown for (A) collected data showing "tight" function line (yellow dashed line) along a U-shaped trough in the LSP curve, (B) interpolated data with missing trough due to linear interpolation of reference laboratory data, and (C) in consistency of 95% prediction limits based on reference laboratory data to 95% RCL of all data. Large red circles highlight examples of significant variability due to the interpretation approach.

While the linearly interpolating/extrapolating data to target values does appear to induce variability in the data set, the effect is limited to those narrow portions of the pH-dependence release curve with steep slopes. Thus, species with Method 1313 results that are not a strong function of pH (e.g., boron, calcium) and portions of the pH-dependence curves that are relatively insensitive to pH are not affected to a

significant degree. In addition, steep portions of the pH-dependence curve tend to occur at the extremes of the pH range (e.g., pH 2 and 13) where the pH regime does not represent the majority of environmental conditions.

Visual comparison of collected and interpolated data for the selected ten analytes and the three test materials revealed that only nine target pH values between pH 4 and 12 show obvious increased variability due to interpolation. This represents 4% of the 210 potential pH target values between pH 4 and 12 (i.e., seven target values from ten selected analytes in three study materials). The minimum and maximum data points collected for each target pH value and study material were 27 and 36, respectively[10] and only a few of these data points at any target pH were affected. All of the affected target pH values represent minima of the pH-dependence curve which tends toward higher interpolated values (e.g., Figure 5) and a conservative estimate of release (i.e., over-predicts leaching). None of the suspect target values occur at maxima on the pH dependence curve. Therefore, while the introduction of variability caused by the linear interpolation/extrapolation of $\log_{10}$ transformed data represents an interesting phenomenon of the method validation approach, the variability has little bearing on the precision of the method and is unlikely to significantly influence environmental decisions that are made based on interpolated data.

Standard Deviations and Coefficients of Variation

The standard deviation intervals about the overall data mean indicate the variance in data associated with (i) within-laboratory statistics associated with repeatability, (ii) between-laboratory statistics, and (iii) with overall method performance associated with method reproducibility. When compared to the overall coefficient of variation, the coefficients of variation for the between-laboratory and within-laboratory standard deviation provide a sense of whether the overall variability (reproducibility) can be attributed to within-laboratory (repeatability) or between laboratory variation components. Figure 7 shows standard deviation above and below the mean value and coefficients of variation for selected analytes in three study materials.

The within-laboratory standard deviations (repeatability) are generally less than the standard deviations associated with between-laboratory or overall (reproducibility) standard deviations. The overall coefficients of variation range from approximately 5% to over 100% and, to a large extent, are dependent on the slope of the pH-dependence curve. The coefficient of variation for between-laboratory standard deviation is generally higher than the coefficient of variation for within-laboratory standard deviation. Of the data shown in Figure 7, the coefficients of variation for within-laboratory standard deviation tend to be relatively consistent with analytical uncertainty (~5% RSD) for calcium in the EaFA and for cadmium in CFS and molybdenum in SWA where the pH-dependence curve is relatively flat. Coefficients of variation increase where the slope of the pH-dependence curve is steep (see Figure 7B at pH 8), when the extract concentration is near or less than the MDL (see Figure 6B at pH 10-12) or when operational difficulties, such as gel formation in SWA at pH < 4, increased analytical sample heterogeneity (see Figure 7C).

[10] The number of data points collected for each pH target included data from six test replicates conducted by the reference laboratory plus triplicate analysis conducted by the participating laboratories (e.g., the minimum value of 27 considers 21 data points from triplicate test runs of the seven participating laboratories plus six test replicates from the reference laboratory).

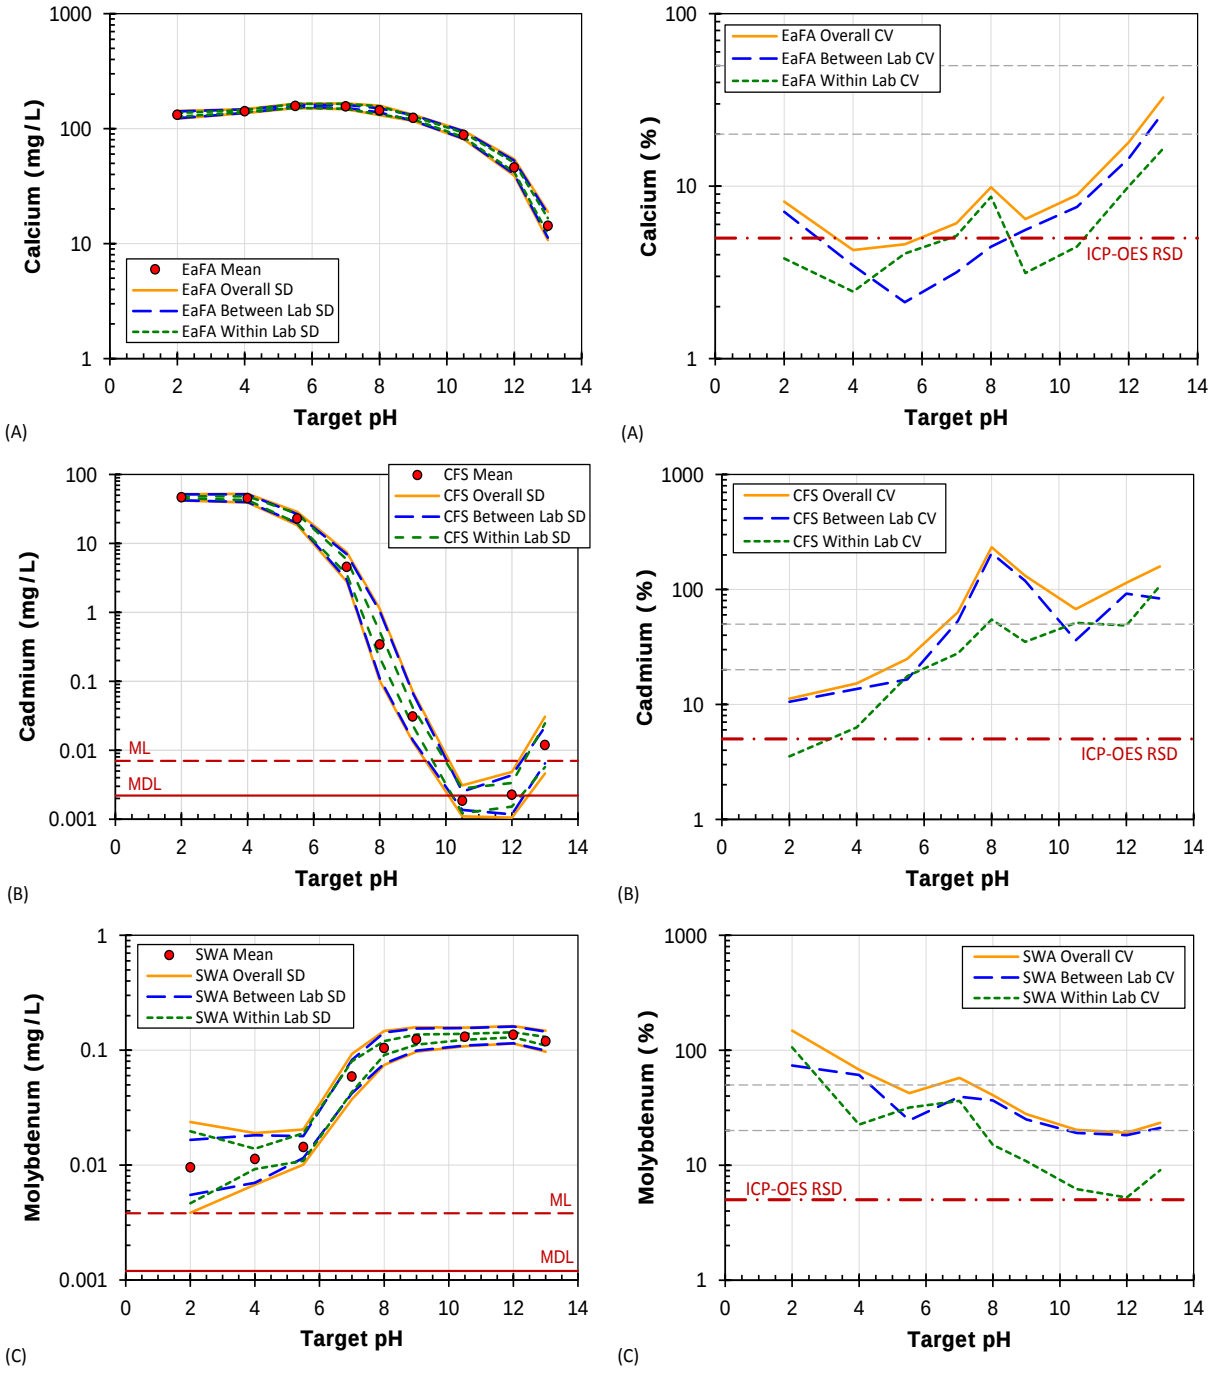

Figure 7. Example standard deviation intervals about the mean and coefficients of variation for Method 1313 materials.

Method 1313 Repeatability and Reproducibility

Using the above mean-based statistics, comparisons of repeatability and reproducibility statistics among the three study materials (i.e., EaFA, SWA, and CFS) are presented for antimony in Figure 8 and molybdenum in Figure 9. Figures for the remaining analytes are presented in Appendix E. In each

figure, the mean, and the overall standard deviation interval about that mean, show the various levels and forms of the pH-dependent behavior over a broad pH range (Panel A). Both the repeatability relative standard deviation (RSD_r), which is the within-laboratory coefficient of variation, (Panel B) and the reproducibility relative standard deviation (RSD_R) which is the overall coefficient of variation (Panel C) are plotted as a function of target pH. The Horwitz Ratio for reproducibility relative standard deviation ($HorRat_R$) is plotted in Panel D for each material as a function of target pH.

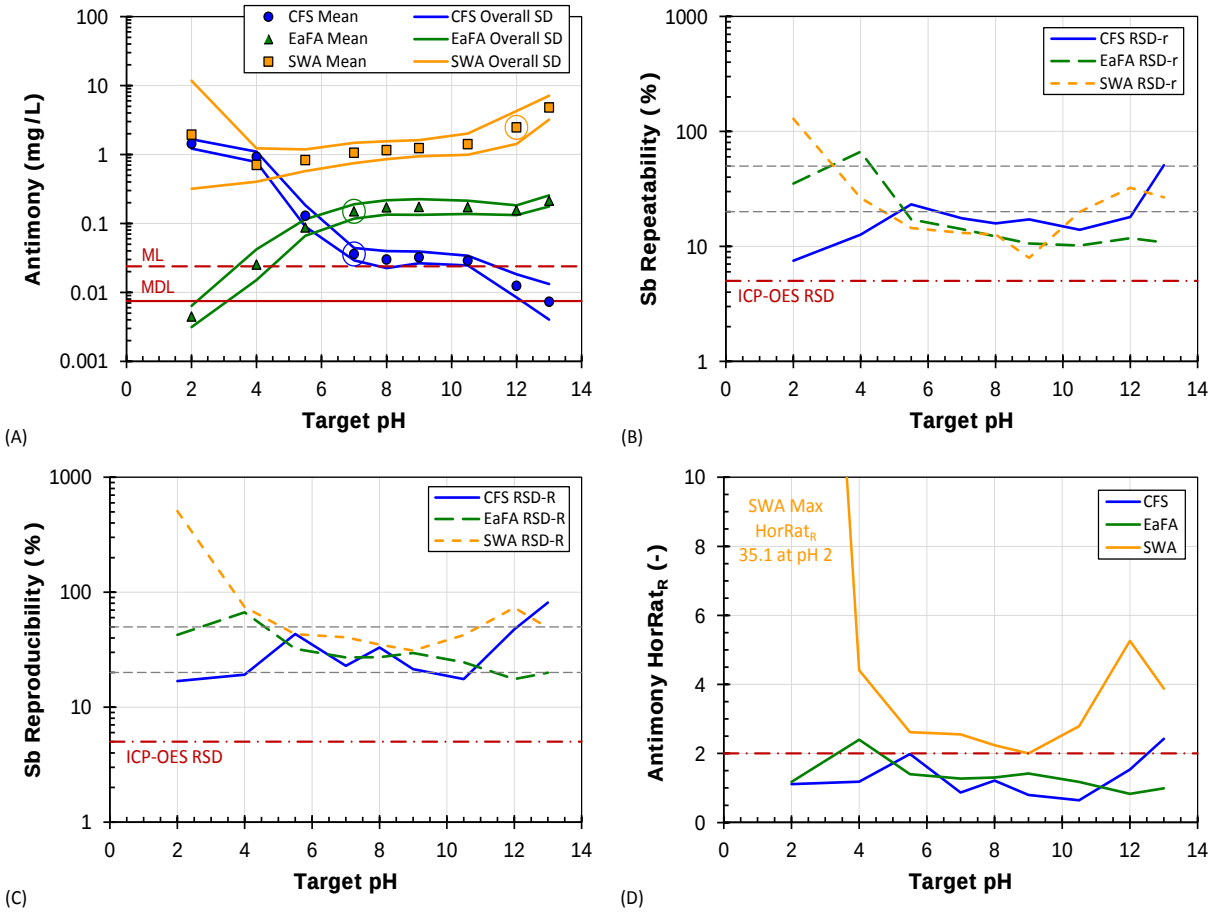

Figure 8. Method 1313 repeatability and reproducibility of antimony.

Note: Date shown for (A) overall standard deviation intervals about the mean, (B) repeatability relative standard deviation (RSR_r), (C) reproducibility relative standard deviation (RSD_R), (D) Horwitz ratio. Grey dashed line in panels (B) and (C) indicate 20% and 50% reference lines for repeatability and reproducibility.

The repeatability of Method 1313 for antimony (Figure 8B) is approximately 10-20% for the majority of the pH range with an increase to 20-100% at low pH for SWA and CFS. Method reproducibility (Figure 8C) shows a similar pattern with reproducibility of 20-50% with SWA reproducibility increasing to about 500% at pH 2. In the case of SWA, several participating laboratories mentioned the formation of a gel-like eluate at pH values less than 4. This gel presented difficulties for the participating laboratories during filtration and for the analytical laboratory during analysis. Thus, larger standard deviations could be expected where the gel was observed.

In Figure 9, the repeatability and reproducibility of Method 1313 were consistent with the observations for antimony. Method repeatability (Figure 9B) ranged from approximately 5% in the alkaline range, where Mo solubility as a function of pH is relatively flat (Figure 9A), to 20-50% in the acidic range. Reproducibility values (Figure 9C) were between 20 and 50% over the pH range with values in excess of 100% for SWA gel formation (i.e., at low pH) or when the slope of the pH-dependent function line was steep (i.e., CFS pH 8-9).

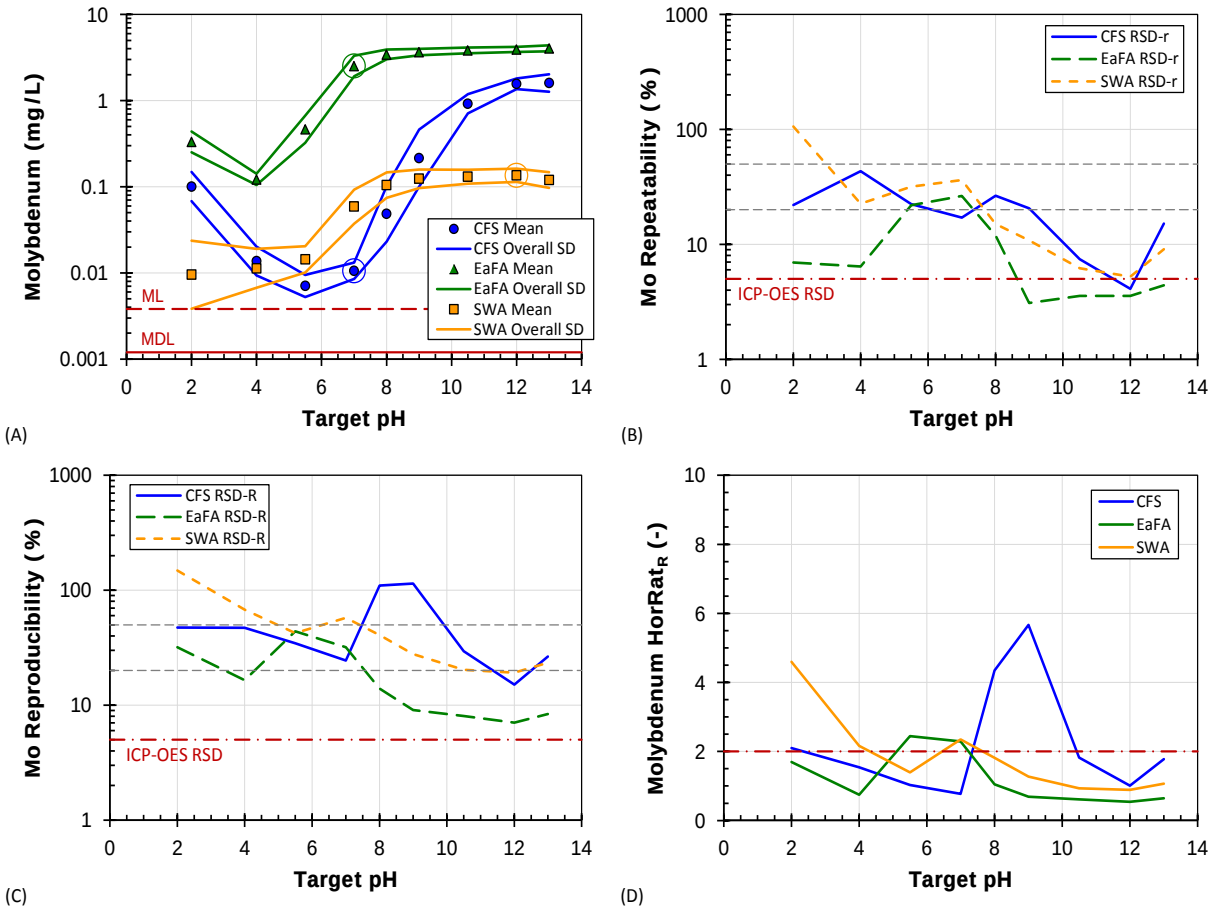

Figure 9. Method 1313 repeatability and reproducibility of molybdenum.

Note: Data shown for (A) overall standard deviation intervals about the mean, (B) repeatability relative standard deviation (RSD_r), (C) reproducibility relative standard deviation (RSD_R), (D) Horwitz ratio. Grey dashed line in panels (B) and (C) indicate 20% and 50% reference lines for repeatability and reproducibility.

Calculation of Horwitz ratios showed that the $HorRat_R$ values tend to be less than or approximately 2 for most target pH values and for all analytes. Higher values of $HorRat_R$ can be explained for most cases, by sample heterogeneities, sample preparation, and gel formation in SWA at low pH, or sections of the pH-dependent release curve with steep curvature (i.e., high potential for variability introduced through the interpolation/extrapolation process).

Method precision for Method 1313 is shown in terms of relative standard deviations for repeatability (Table 15) and reproducibility (Table 16). For each analyte and pH target, the RSD_r or RSD_R represents

the method precision calculated from the validation data. The precision data in these summary tables should not be taken out of context of the LSP trendlines, but should be compared to the pH-dependent LSP curve data in order to relate method precision for a particular analyte in a study material estimated at a target pH to the features of the LSP curve. As an example, the comparison between RSD_R data for chromium leaching in EaFA (Table 16) and the interpolated EaFA data for chromium (Figure 10A) shows that RSD_R values pass through a maximum of 205% as trend in the LSP passes through a minimum and approaches the ML and MDL values. However, for antimony in SWA (Figure 10B), the high variability in results is obvious for the pH target of 2.0 where gel formation presented difficulties in filtration. Caution should be exercised when attempting to extend the method precision data presented in Table 15 and Table 16 to other matrices due the association between estimated method precision values and the shape/slope of the LSP curve.

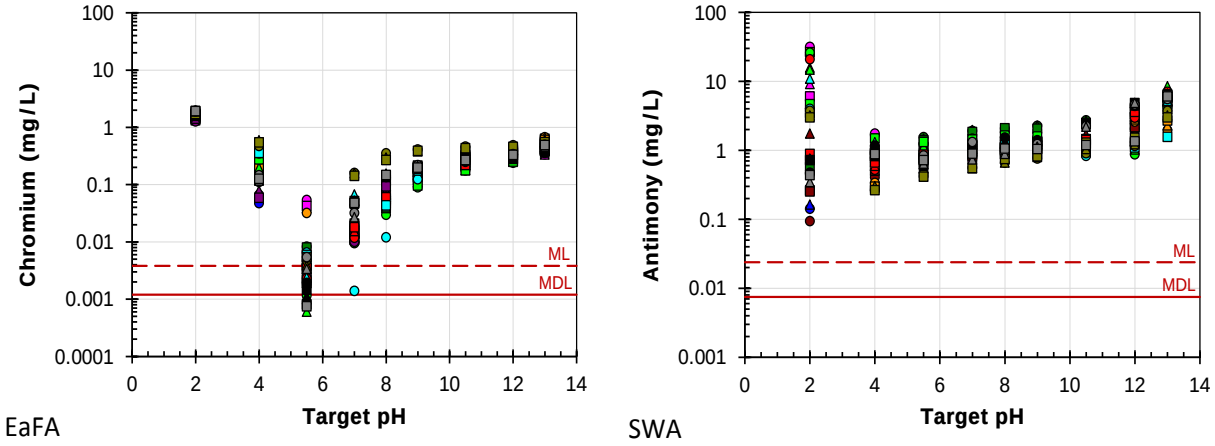

Figure 10. Interpolated data for Method 1313 for chromium in EaFA (left) and antimony in SWA (right).

Examination of the Method 1313 data has shown that high RSDR value may result from (a) concentration data near or below the quantitation limit, (b) LSP for an analyte that are a strong function of pH, hence, small deviations in pH measurement can result in large variation in concentrations, (c) significant curvature in the LSP trendline, for which linear interpolation of log10 transformed data may increase variability, and (d) sample heterogeneity induced by either material preparation or gel formation in the SWA extract. For each of the reproducibility RSD_R in Table 16 greater than 50%, superscripts are used to indicate these primary functional explanations associated with these precision values.

In summary, the median RSD_r for Method 1313 shown in Table 15 ranges from 3% for calcium in CFS to 66% for chromium in SWA. The median RSD_R presented in Table 16 was slightly higher than the RSD_r, ranging from 6% for boron in EaFA to 144% for chromium in SWA. The overall method precision for Method 1313, taken across all validation data (i.e., all pH targets, all analytes and all materials), was determined to be 13% RSD_r and 28% RSD_R.

Table 14. Method 1313 Repeatability (RSD_r) across Study Materials

		RSD_r (%) at Target pH Value									
EaFA – Coal Combustion Fly Ash											
Analyte	**Symbol**	**2.0**	**4.0**	**5.5**	**7.0**	**8.0**	**9.0**	**10.5**	**12.0**	**13.0**	**Med**
Antimony	Sb	29	67	17	14	12	11	10	12	11	**12**
Arsenic	As	11	11	14	15	18	14	12	9	15	**14**
Barium	Ba	7	8	4	4	8	9	21	12	41	**8**
Boron	B	3	3	4	6	9	3	3	4	5	**4**
Calcium	Ca	4	2	4	5	9	3	4	10	17	**4**
Chromium	Cr	7	34	103[a,b]	89[b,c]	31	13	10	9	11	**13**
Cobalt	Co	5	3	11	29	50	38	16	1	NA	**14**
Molybdenum	Mo	7	6	22	26	12	3	4	4	4	**6**
Selenium	Se	10	21	13	16	15	7	4	4	4	**10**
Vanadium	V	12	17	10	11	15	11	12	7	7	**11**
SWA – Solidified Waste Analog											
Analyte	**Symbol**	**2.0**	**4.0**	**5.5**	**7.0**	**8.0**	**9.0**	**10.5**	**12.0**	**13.0**	**Med**
Antimony	Sb	129[d]	26	14	13	13	8	20	32	27	**20**
Arsenic	As	59[b,d]	20	35	19	20	31	22	34	22	**22**
Barium	Ba	65[d]	10	11	7	7	8	11	14	106[b]	**11**
Boron	B	28	6	8	10	9	7	9	16	18	**9**
Calcium	Ca	46	7	12	5	8	18	28	36	60[b]	**18**
Chromium	Cr	67[d]	29	74[b]	99[a,c]	76[a,c]	66[a,c]	53[a,b]	42	59[b]	**66**
Cobalt	Co	38	10	16	57	41	37	16	7	18	**18**
Molybdenum	Mo	106[a,d]	23	32	36	15	11	6	5	9	**15**
Selenium	Se	41	7	9	5	6	10	5	5	10	**7**
Vanadium	V	94[b,d]	29	10	5	6	10	8	14	17	**10**
CFS – Contaminated Field Soil											
Analyte	**Symbol**	**2.0**	**4.0**	**5.5**	**7.0**	**8.0**	**9.0**	**10.5**	**12.0**	**13.0**	**Med**
Antimony	Sb	8	13	23	18	16	17	14	18	43	**17**
Arsenic	As	8	24	29	19	25	16	9	12	29	**19**
Barium	Ba	15	13	9	7	6	4	13	27	108[a,b]	**13**
Boron	B	6	4	8	7	8	7	5	11	12	**7**
Cadmium	Cd	4	6	18	28	55[b]	35	51[a]	49	108[a]	**35**
Calcium	Ca	5	4	4	3	2	2	3	3	8	**3**
Lead	Pb	6	5	12	17	26	15	45	32	152[c]	**17**
Molybdenum	Mo	22	43	22	17	27	21	7	4	15	**21**
Selenium	Se	9	6	12	14	14	9	9	12	20	**12**
Vanadium	V	8	12	4	4	3	3	3	5	7	**4**

Notes: NA = method precision not available (all concentrations set to ½ MDL)

Superscripts indicate functional explanations for repeatability greater than 50% RSD_r:

a = concentration approaching or below ML

b = LSP is strong function of pH at target pH

c = significant curvature in LSP trendline (e.g., approaching local minima or maxima)

d = sample heterogeneity due to gel formation in SWA extracts

Table 15. Method 1313 Reproducibility (RSD_R) across Study Materials

		RSD_R (%) at Target pH Value									
EaFA – Coal Combustion Fly Ash											
Analyte	**Symbol**	**2.0**	**4.0**	**5.5**	**7.0**	**8.0**	**9.0**	**10.5**	**12.0**	**13.0**	**Med**
Antimony	Sb	38	67[a,b]	32	27	27	30	25	18	20	**27**
Arsenic	As	64[b]	37	57[a,c]	50[a,c]	41	40	28	43	47	**43**
Barium	Ba	9	20	14	11	11	21	28	23	68	**20**
Boron	B	6	5	6	6	9	5	7	13	27	**6**
Calcium	Ca	8	4	5	6	10	6	9	18	33	**8**
Chromium	Cr	14	100[b]	205[a,c]	155[b,c]	100[b,c]	41	28	22	22	**41**
Cobalt	Co	7	8	15	85[b]	159[a, b]	51[a]	24	1	NA	**19**
Molybdenum	Mo	32	16	44	32	14	9	8	7	8	**14**
Selenium	Se	52[b]	43	32	35	32	21	8	7	9	**32**
Vanadium	V	27	32	26	40	43	47	40	15	13	**32**
SWA – Solidified Waste Analog											
Analyte	**Symbol**	**2.0**	**4.0**	**5.5**	**7.0**	**8.0**	**9.0**	**10.5**	**12.0**	**13.0**	**Med**
Antimony	Sb	508[d]	74[d]	43	40	35	31	42	73	49	**43**
Arsenic	As	75[b,d]	58[b,d]	59[b]	41	47	62[c]	124[c]	122[b]	51[b]	**59**
Barium	Ba	91[d]	20	26	17	16	21	38	51[c]	136[b]	**26**
Boron	B	66[d]	26	25	16	14	9	18	110[c]	54[c]	**25**
Calcium	Ca	61[d]	23	28	23	25	29	94[c]	115[b]	133[b]	**29**
Chromium	Cr	89[d]	70[d]	277[b]	198[a,c]	144[a,c]	108[a,c]	149[a,b]	227[b]	102[b]	**144**
Cobalt	Co	58[d]	26	43	82[b]	68[a,b]	50[a]	59[a]	8	19	**50**
Molybdenum	Mo	148[a,d]	68[d]	42	58[b,c]	41	28	20	19	23	**41**
Selenium	Se	77[d]	25	27	19	18	19	20	19	22	**20**
Vanadium	V	175[b,d]	53[c,d]	37	27	25	26	42	47	26	**37**
CFS – Contaminated Field Soil											
Analyte	**Symbol**	**2.0**	**4.0**	**5.5**	**7.0**	**8.0**	**9.0**	**10.5**	**12.0**	**13.0**	**Med**
Antimony	Sb	17	19	43	23	33	21	18	47	74[a]	**23**
Arsenic	As	71[b]	26	37	31	37	24	25	30	85[b]	**31**
Barium	Ba	136[a,c]	19	26	26	20	14	22	35	280[a,b]	**26**
Boron	B	7	12	9	9	10	14	9	15	24	**10**
Cadmium	Cd	11	15	25	63[b,c]	233[b]	132[a,b]	68[a]	114[a]	158[a]	**68**
Calcium	Ca	7	7	7	5	5	6	6	7	51[c]	**7**
Lead	Pb	16	10	19	42	112[c]	53[c]	80[c]	50	350[c]	**50**
Molybdenum	Mo	47	47	35	24	110[b,c]	114[b]	30	15	26	**35**
Selenium	Se	30	11	17	16	19	19	28	21	46	**19**
Vanadium	V	14	27	20	21	20	19	25	28	54	**21**

Notes: NA = method precision not available (all concentrations set to ½ MDL)
Superscripts indicate functional explanations for reproducibility greater than 50% RSD_R:

a = concentration approaching or below ML
b = LSP is strong function of pH at target pH
c = significant curvature in LSP trendline (e.g., approaching local minima or maxima)
d = sample heterogeneity due to gel formation in SWA extracts

METHOD 1316 RESULTS AND ANALYSIS

The Method 1316 results for testing the EaFA fly ash material in Phase I were combined with the results for SWA solidified waste analog and CFS contaminated field soil testing in Phase II.

pH Response as a Function of L/S

The results of Method 1316 include the natural pH response as a function of L/S as shown in Figure 11 for each of the three study materials. For EaFA (Figure 11A) and CFS (Figure 11C) the natural pH is not a strong function of L/S ratio and ranges between 6.5 and 8.0. The natural pH of SWA (Figure 11B), however, increases from approximately 12.7 to nearly 13 as L/S ratios decrease from 10 to 1 mL/g. In addition, the alkaline nature of SWA is evident from the high pH values at natural pH.

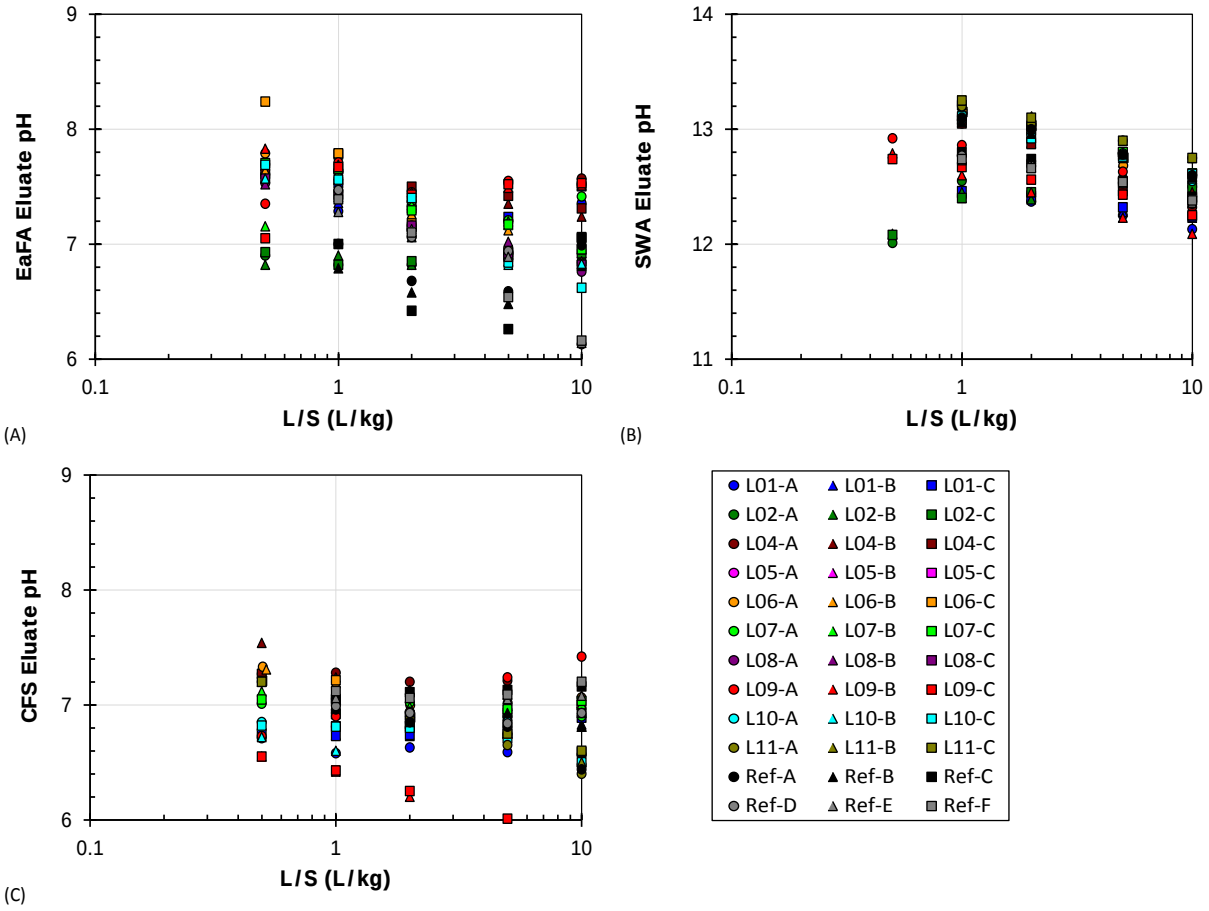

Figure 11. Eluate pH for Method 1316 Study Materials.

Note: (A) EaFA coal combustion fly ash, (B) SWA solidified waste analog, and (C) CFS contaminated field soil.

Statistical Analysis of L/S-dependent Leaching Data

The results of statistical analysis for three study materials tested using Method 1316 (i.e., EaFA coal combustion fly ash, SWA solidified waste analog, and CFS contaminated field soil) are presented as six-panel figures in Appendix F. Each figure shows the results of statistical analysis for a single selected analyte in each material (e.g., calcium in EaFA, boron in SWA). In the discussion below, selected panels from these figures will be used to generalize the overall results of the method validation.

Interpolation/Extrapolation of Log_{10}-transformed Data

Method 1316 data are reported at the target L/S and, therefore, no data interpolation to the target L/S value was necessary. However, in order to avoid extrapolation of data to a target L/S of 0.5 mL/g when no data at that target value were reported, extrapolation in the LeachXS statistics module was restricted to data values within 10% of the target L/S.

Prediction Limit and Robust Confidence Limit -based Statistical Analysis

A selection of mean-based prediction limits for the reference laboratory data and median-based robust confidence limits for all data is shown in Figure 12 for various study materials. These graphs cover a broad spectrum of the statistical results.

For most of the analytes in Method 1316 validation, the 95% PL (green dashed lines) fall within the bounds of the 95% RCL intervals (red solid lines) and the mean of the reference laboratory data (green dots) corresponds well with the median of the laboratory means (red squares). In this context, these observations show that there is good agreement between reference laboratory data and the data set as a whole. In Figure 12, the panels in rows A and B show agreement at a high level and average level, respectively. Such consistency was observed for nearly all CFS and most EaFA analytes. Panels in row C indicate that, in some cases, the 95% PL limit was greater than the 95% RCL although the agreement between reference laboratory mean and the data set RCL intervals was reasonable. This pattern infers that within-laboratory replication for some analytes in SWA and EaFA materials is the main source of overall variability in the data. Within-laboratory replication variability was most likely due to heterogeneity of the study material.

As with the RCL values for Method 1313, the width of the RCL intervals was approximately a factor of 2 for analytes with good repeatability. Greater width was observed for the RCL at low L/S (see antimony in CFS and boron in EaFA, both in row B). The width for the PL generally was either similar to or smaller for the PL than for the RCL for most analytes.

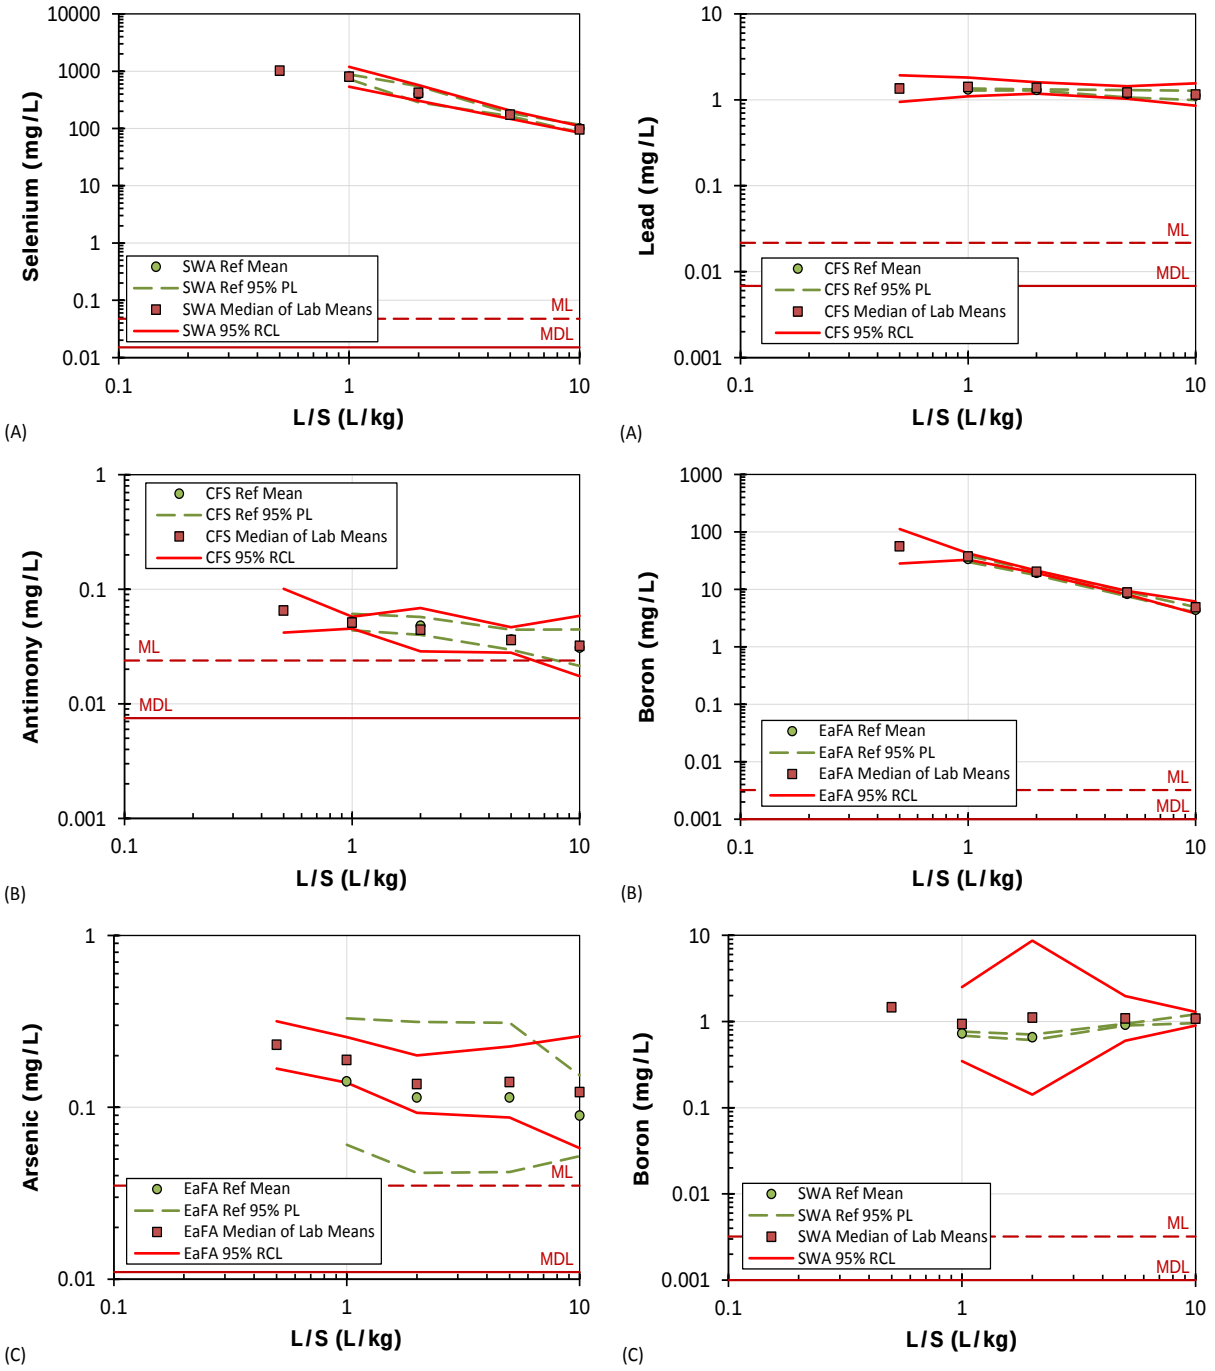

Figure 12. Agreement between 95% prediction limits (95% PL) about the mean of the reference laboratory data and 95% robust confidence limits (95% RCL) based on the median of laboratory means.

Note: Data shown for (A) high level agreement, (B) median level agreement, and (C) lowest level of agreement.

Standard Deviations and Coefficients of Variation

Following the analytes in the left side of Figure 12 through the analysis process, the analyte standard deviation intervals about the mean and coefficients of variation are shown in Figure 13.

The standard deviation intervals about the overall data mean indicate the variance in data associated with (i) within-laboratory statistics associated with repeatability, (ii) between-laboratory statistics, and (iii) with overall method performance associated with method reproducibility. The coefficient of variation for each of these standard deviation values provides a relative measure if the overall variability (reproducibility) is due to within-laboratory (repeatability) or between laboratory variation components.

In the cases of analytes with good agreement between PL and RCLs (e.g., arsenic in SWA and antimony in CFS), the within-laboratory standard deviations (repeatability) are less than the variance associated with between-laboratory or the overall (reproducibility) standard deviations and the between-laboratory coefficient of variation represents a large portion of the overall variation (Figure 13, row A and B). However, when the PL interval is wider than the RCL interval (e.g., arsenic in EaFA), the within-laboratory standard deviation (repeatability) is greater than the between-laboratory standard deviation. Thus, the within-laboratory coefficient of variation drives the overall variability (Figure 13, row C). In general, the overall coefficient of variation was between 20-50% which is consistent with Method 1313 observations.

Method 1316 Repeatability and Reproducibility

Repeatability and reproducibility values for the three study materials (i.e., EaFA, SWA, and CFS) were calculated based on the standard deviations and are presented in Figure 14 and Figure 15 for vanadium and boron, respectively. In each of these figures, the mean and the overall standard deviation interval about that mean show the various levels and forms of the L/S-dependent behavior (panel A). The repeatability relative standard deviation (RSD_r; i.e., the within-laboratory coefficient of variation) and the reproducibility relative standard deviation (RSD_R; i.e., the overall coefficient of variation) are plotted as a function of L/S in panels B and C. The reproducibility $HorRat_R$ is plotted for each material as a function of L/S in panel D.

Overall, repeatability values were approximately 5-20% whereas reproducibility was more variable at 5-50% for most analytes. Reproducibility values for SWA were generally higher than the other two materials. Given the fact that SWA is a highly alkaline material subject to carbonation over time, the heterogeneities associated with storing SWA prior to testing may explain the higher reproducibility values.

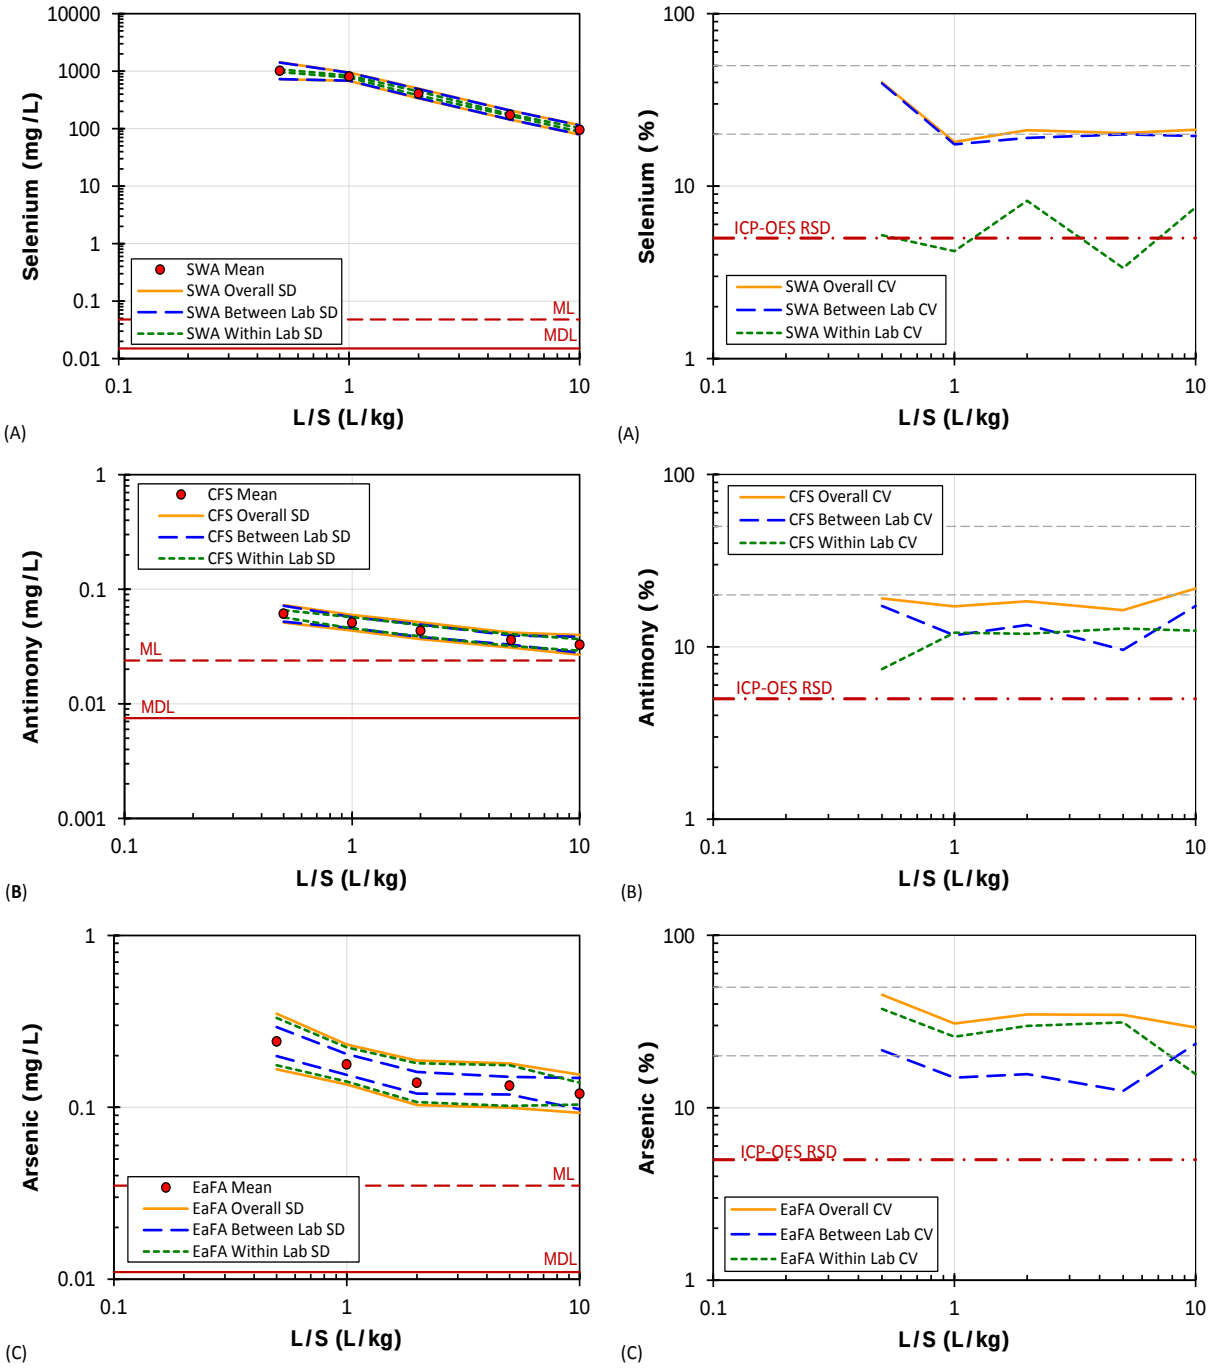

Figure 13. Standard deviation intervals about the mean (left) and coefficients of variation (right) for Method 1316 materials.

Note: Data shown for (A) selenium in SWA, (B) antimony in CFS, and (C) arsenic in EaFA.

The reproducibility Horwitz ratios shown in Figure 14D and Figure 15D are generally less than or approximately 2 across the L/S range. For most analytes, the $HorRat_R$ values increase above 2 at L/S = 0.5 mL/g which likely is due to procedural difficulties in separating solid and liquids via filtration.

Higher values of $HorRat_R$ are seen in the SWA material for antimony, barium, boron, calcium and selenium which can be explained by sample heterogeneities in addition to the above filtration issue.

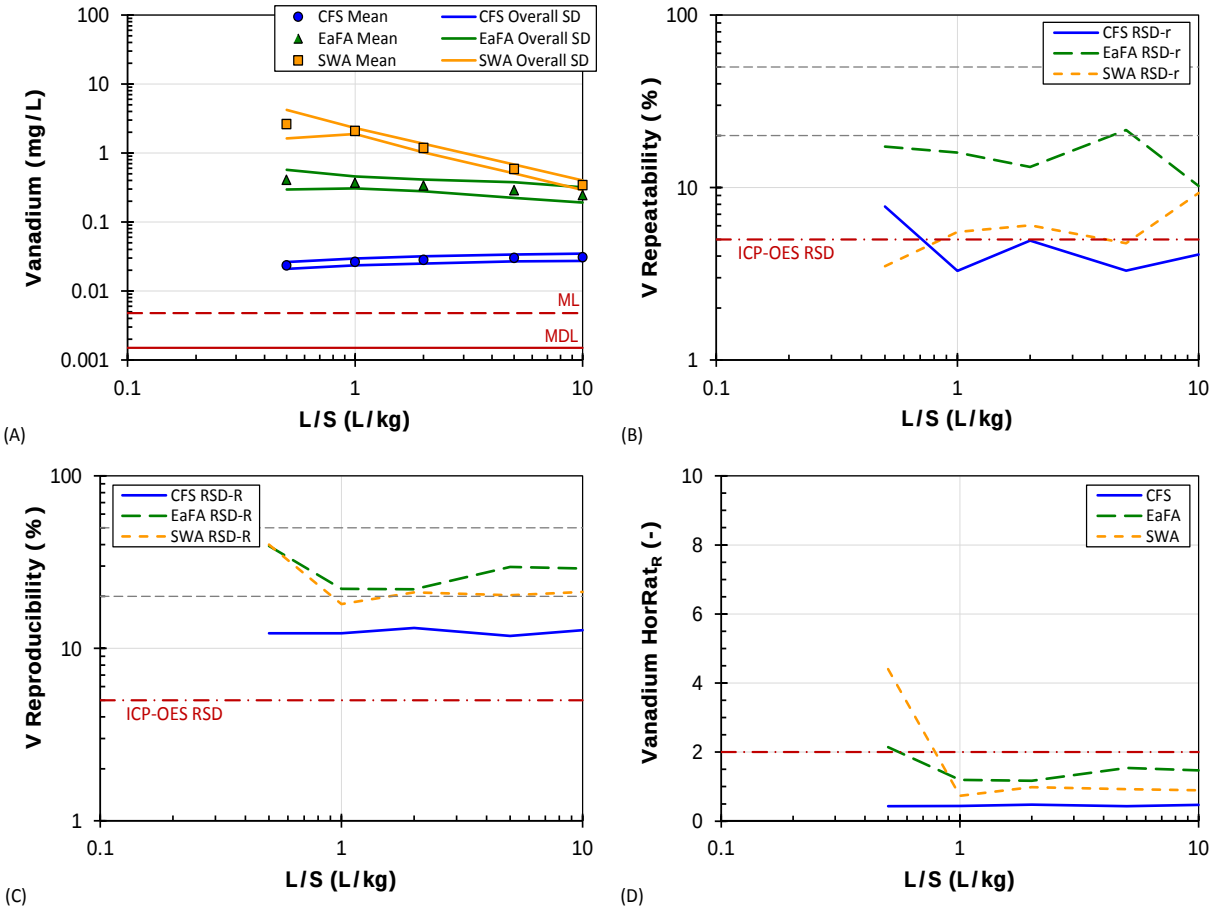

Figure 14. Method 1316 repeatability and reproducibility of vanadium.

Note: Data shown for (A) overall standard deviation intervals about the mean, (B) repeatability relative standard deviation (RSD_r), (C) reproducibility relative standard deviation (RSD_R), (D) Horwitz ratio. Grey dashed line in panels (B) and (C) indicate 20% and 50% reference lines for repeatability and reproducibility.

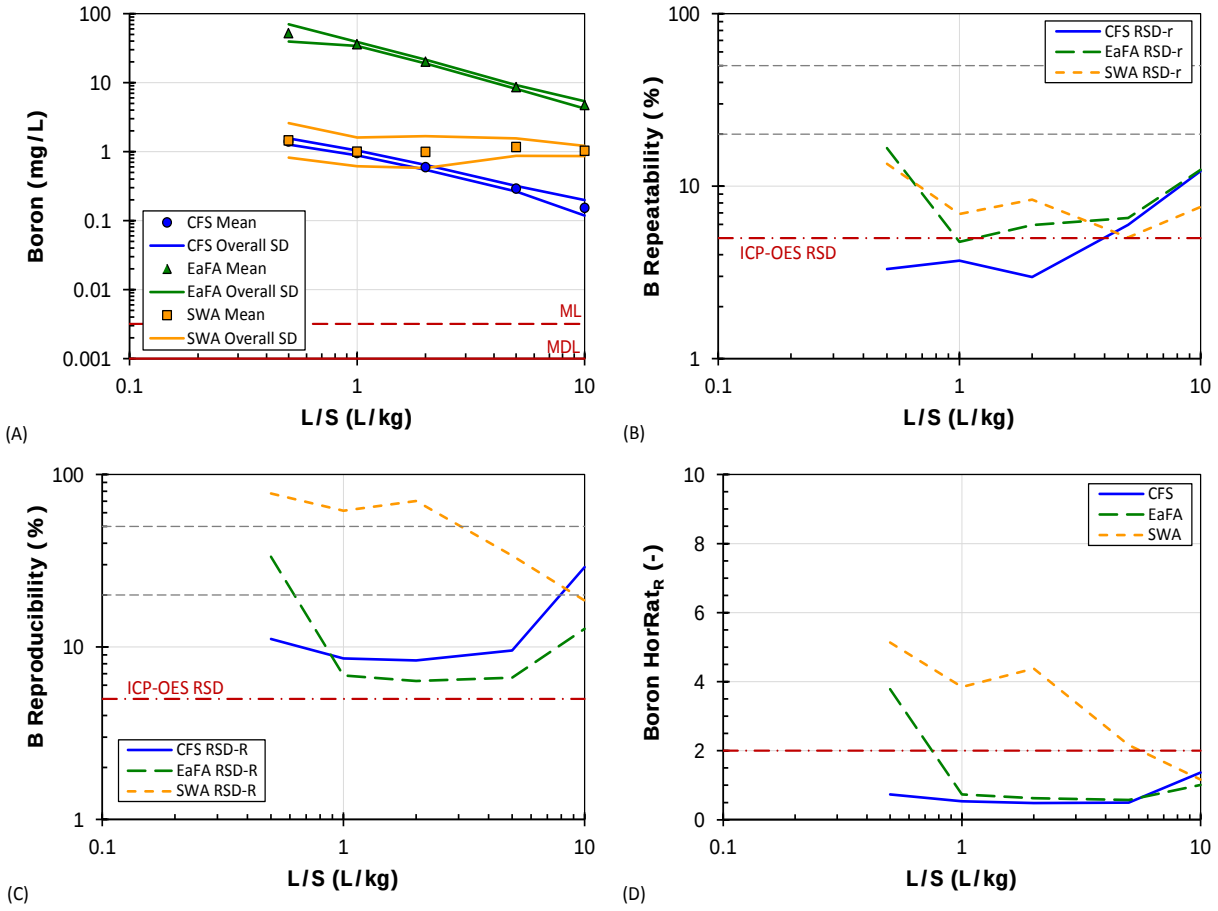

Figure 15. Method 1316 repeatability and reproducibility of boron.

Note: Data shown for (A) overall standard deviation intervals about the mean, (B) repeatability relative standard deviation (RSD_r), (C) reproducibility relative standard deviation (RSD_R), (D) Horwitz ratio. Grey dashed line in panels (B) and (C) indicate 20% and 50% reference lines for repeatability and reproducibility.

A summary of Method 1316 repeatability and reproducibility values for each of the analytes in the validation study are presented as RSD_r and RSD_R, respectively, in Table 17 and Table 18. The median RSD_r for Method 1316 ranged from 2% for calcium in CFS to 36% for chromium in EaFA while RSD_R ranged from 6% for Ca in CFS to 62% for boron in SWA. Overall, the precision of Method 1316 was slightly better than Method 1313, most likely due to the fact that pH is not manipulated (i.e., there is no addition of acid or base), thus, the buffering of the solid material controls pH. The median precision estimates for Method 1316, including all L/S target values, all analytes and all study materials, were 8% RSD_r and 19% RSD_R.

Table 16. Method 1316 Repeatability (RSD_r) across Study Materials.

		RSD_r (%) at Target L/S Value (mL/g-dry)					
EaFA – Coal Combustion Fly Ash							
Analyte	**Symbol**	**0.5**	**1.0**	**2.0**	**5.0**	**10.0**	**Med**
Antimony	Sb	15	13	12	24	14	**16**
Arsenic	As	37	26	30	31	16	**28**
Barium	Ba	14	8	7	7	5	**8**
Boron	B	17	5	6	7	12	**9**
Calcium	Ca	12	6	6	6	5	**7**
Chromium	Cr	31	34	37	36	46	**36**
Cobalt	Co	101	15	20	19	24	**20**
Molybdenum	Mo	10	6	7	7	4	**7**
Selenium	Se	21	8	9	12	7	**11**
Vanadium	V	17	16	13	22	10	**16**
SWA – Solidified Waste Analog							
Analyte	**Symbol**	**0.5**	**1.0**	**2.0**	**5.0**	**10.0**	**Med**
Antimony	Sb	5	8	6	8	10	**8**
Arsenic	As	35	8	11	7	13	**11**
Barium	Ba	4	10	27	7	12	**10**
Boron	B	13	7	8	5	8	**8**
Calcium	Ca	7	9	5	6	13	**7**
Chromium	Cr	4	9	39	6	8	**8**
Cobalt	Co	16	15	18	NA	NA	**16**
Molybdenum	Mo	6	6	4	5	7	**6**
Selenium	Se	5	4	8	3	8	**5**
Vanadium	V	3	6	6	5	9	**6**
CFS – Contaminated Field Soil							
Analyte	**Symbol**	**0.5**	**1.0**	**2.0**	**5.0**	**10.0**	**Med**
Antimony	Sb	7	12	12	13	12	**12**
Arsenic	As	10	13	12	16	15	**13**
Barium	Ba	6	4	5	2	4	**4**
Boron	B	3	4	3	6	12	**4**
Cadmium	Cd	4	4	4	4	4	**4**
Calcium	Ca	3	2	3	2	2	**2**
Lead	Pb	3	4	7	10	4	**4**
Molybdenum	Mo	9	8	10	10	14	**10**
Selenium	Se	2	3	3	9	9	**3**
Vanadium	V	8	3	5	3	4	**4**

Notes: NA = method precision not available (all concentrations set to ½ MDL).

Table 17. Method 1316 Reproducibility (RSD_R) across Study Materials.

		RSD_r (%) at Target L/S Value (mL/g-dry)					
EaFA – Coal Combustion Fly Ash							
Analyte	**Symbol**	**0.5**	**1.0**	**2.0**	**5.0**	**10.0**	**Med**
Antimony	Sb	39	15	14	24	20	**20**
Arsenic	As	45	31	35	35	29	**35**
Barium	Ba	25	16	12	12	9	**12**
Boron	B	33	7	6	7	13	**7**
Calcium	Ca	22	9	7	8	8	**8**
Chromium	Cr	78	38	37	46	63	**46**
Cobalt	Co	101	29	25	33	43	**33**
Molybdenum	Mo	36	8	8	8	6	**8**
Selenium	Se	37	24	24	24	20	**24**
Vanadium	V	39	22	22	30	29	**29**
SWA – Solidified Waste Analog							
Analyte	**Symbol**	**0.5**	**1.0**	**2.0**	**5.0**	**10.0**	**Med**
Antimony	Sb	5	24	45	75	31	**31**
Arsenic	As	65	34	22	19	22	**22**
Barium	Ba	175	41	103	23	36	**41**
Boron	B	78	62	70	34	19	**62**
Calcium	Ca	42	24	52	8	15	**24**
Chromium	Cr	5	22	70	15	18	**18**
Cobalt	Co	107	41	23	NA	NA	**41**
Molybdenum	Mo	59	28	25	38	33	**33**
Selenium	Se	40	18	21	20	21	**24**
Vanadium	V	61	11	15	16	17	**16**
CFS – Contaminated Field Soil							
Analyte	**Symbol**	**0.5**	**1.0**	**2.0**	**5.0**	**10.0**	**Med**
Antimony	Sb	19	17	18	16	22	**18**
Arsenic	As	24	21	24	32	32	**24**
Barium	Ba	13	14	15	14	16	**14**
Boron	B	11	9	8	10	29	**10**
Cadmium	Cd	10	9	9	10	9	**9**
Calcium	Ca	8	6	5	6	6	**6**
Lead	Pb	10	12	14	15	17	**14**
Molybdenum	Mo	19	13	16	18	18	**18**
Selenium	Se	11	10	7	11	15	**11**
Vanadium	V	12	12	13	12	13	**12**

Notes: NA = method precision not available (all concentrations set to ½ MDL).

COMPARISON OF METHOD PRECISION TO STANDARDIZED LEACHING METHODS

There are no precision criteria for method acceptance in either the EPA guidance on RCRA program validation studies or the ASTM standard practice for interlaboratory studies. Therefore, judgments on the acceptability of the LEAF methods validated in the report cannot be made. However, the precision estimates of Method 1313 and Method 1316 (i.e., RSD_r and RSD_R values) may be compared to the precision results from accepted and standardized leaching tests in order to provide context as to the level of precision attained in this validation study. The following two standardized tests form the basis of comparison to Method 1313 and Method 1316:

TCLP (SW-846 Method 1311) Reproducibility

Reproducibility data is provided in the TCLP method for cadmium, chromium and lead contained in three study materials – ammonia lime still bottoms, a mixture of American Petroleum Institute separator sludge and electroplating waste, and fossil fuel fly ash. Each of the three study materials was tested with both the acetic acid and buffered acetic acid extraction fluids specified in the test method. In the sense that TCLP uses an acid solution to manipulate extract pH, the TCLP procedure is somewhat similar to a single target value extraction of Method 1313 and it is reasonable to assume that the precision estimates could be similar. However, the final pH of the TCLP extraction is not controlled nor recorded so that direct comparison of leaching results often is not possible. As a result of interlaboratory validation of TCLP, the mean %RSD for reproducibility was reported as 74% with a range of 17-118% (EPA, 1992a).

EN 12457 Validation

EN 12457 is European Standard consisting of a four-part batch leaching procedure in which particle size reduced material is extracted with deionized or demineralized water at room temperature. Parts 1, 2 and 4 of the standard are single-batch extractions at difference L/S ratios and particle size requirements. Part 3 consists of a two-step test with re-extraction of the recovered material from the first L/S 2.0 mL/g extraction in a second extraction step at L/S of 8.0 mL/g (cumulatively the L/S is equal to 10 mL/g). In comparison to the LEAF methods, EN 12457-2 is most similar to the L/S 10 target extractions in Method 1316 and the natural pH extraction of Method 1313.

The performance characteristics of the single-batch extraction leaching test, EN 12457-2, was validated in an interlaboratory study using 12-14 laboratories across Europe and seven materials, including municipal solid waste incinerator filter cake, sewage sludge, contaminated soil, chemical sludge, sand blasting waste, incinerator bottom ash, and metallurgical slag. The precision data shown Table 2 of the EN 12457 part 2 (CEN, 2001) method precision section includes relative standard deviations for repeatability and reproducibility. The median precision estimates for EN 12457-2 are 10% RSD_r and 33% RSD_R, with ranges of 2-77% and 7-124% for repeatability and reproducibility, respectively.

Precision Distributions and Comparisons

The distribution of RSD_r and RSD_R values for Method 1313 and Method 1316 are shown in the form of "box and whisker" plots in Figure 16 through Figure 18. The distributions in these figures were derived from the method precision results in Table 17 and Table 18. Details on the values used in the distribution plots are presented in Appendix E for Method 1313 validation and Appendix F for Method 1316 validation. In each distribution, the "box" in Figure 15 through Figure 17 represents the IQR (i.e., 25^{th} to 75^{th} percentiles) of the data with a horizontal line within the box displaying the median value. The

"whiskers" above and below the box indicate the maximum and minimum data in the data set, respectively. Also shown in these figures are the distribution of RSD values used to represent TCLP precision (blue distribution) and the RSD_r and RSD_R distributions from reported for EN 12457 validation (red distribution).

Precision as a Function of Analyte

In Figure 16, the distributions of Method 1313 and Method 1316 precision estimates are shown as a function of each analyte. These distributions represent the precision estimates for all study materials and all test positions (i.e., nine target pH values for Method 1313 and five L/S values for Method 1316) for each common analyte. The figure shows that when precision is broken down by analyte, the IQRs for all analytes are similar. However, the extreme values of the distribution for arsenic, barium, molybdenum and antimony appear to be higher than for the other analytes. The analytical QA/QC for arsenic and selenium were slightly higher than the other analytes (see Table 12) indicating that, although all analytes passed basic QA/QC, some interference in eluate analysis might be the cause of wider precision distributions. Also, total content analysis indicated greater variability for antimony, barium, and molybdenum, potentially indicating greater material heterogeneity with respect to these analytes. The median values of precision and IQRs for Method 1313 and Method 1316 are consistent with the precision distribution from EN 12457-2. The IQRs for Method 1313 and Method 1316 precision is considerably lower than that reported in the TCLP precision data.

Precision as a Function of Test Parameters

The distribution of precision estimates for all analytes and study materials measured for a specific target test position (i.e., pH values for Method 1313 and L/S values for Method 1316) are shown in Figure 17. As noted in the Method 1313 results, the highest precision estimates for Method 1313 occur at the extremes of the pH range (e.g., pH = 2 or pH = 13.0) where errors in pH measurement are likely and LSP concentrations may change drastically over a small pH interval. Comparison to standardized leaching test precision at these pH extremes is not reasonable in that EN and TCLP are most similar to extraction at natural pH or acid extraction in the near-neutral pH range. Within the near-neutral range, Method 1313 precision compares favorably with EN 12457-2 precision and is much better than the precision reported for TCLP. Method 1316 repeatability is fairly consistent across the target L/S range; however, reproducibility shows a wider range of precision for low L/S extractions which may be due to the fact that there is less data at L/S =0.5 mL/g-dry than at other L/S values. Again, the precision distributions are in good agreement with those of EN 12457-2 and considerable lower than those of TCLP.

Precision as a Function of Material

Method 1313 and Method 1316 precision data are presented in Figure 18 as a function of study material. Of the three study materials, SWA showed the highest RSD_r and RSD_R distributions while EaFA showed the lowest. Given the nature of the materials and the fact that SWA was created by mixing contaminants by hand into a large batch of cementitious materials, these precision values are not surprising. The median Method 1313 and Method 1316 data shown in Figure 18 are consistent with the median precision for EN 12457-2 and well below the mean %RSD value reported for TLCP.

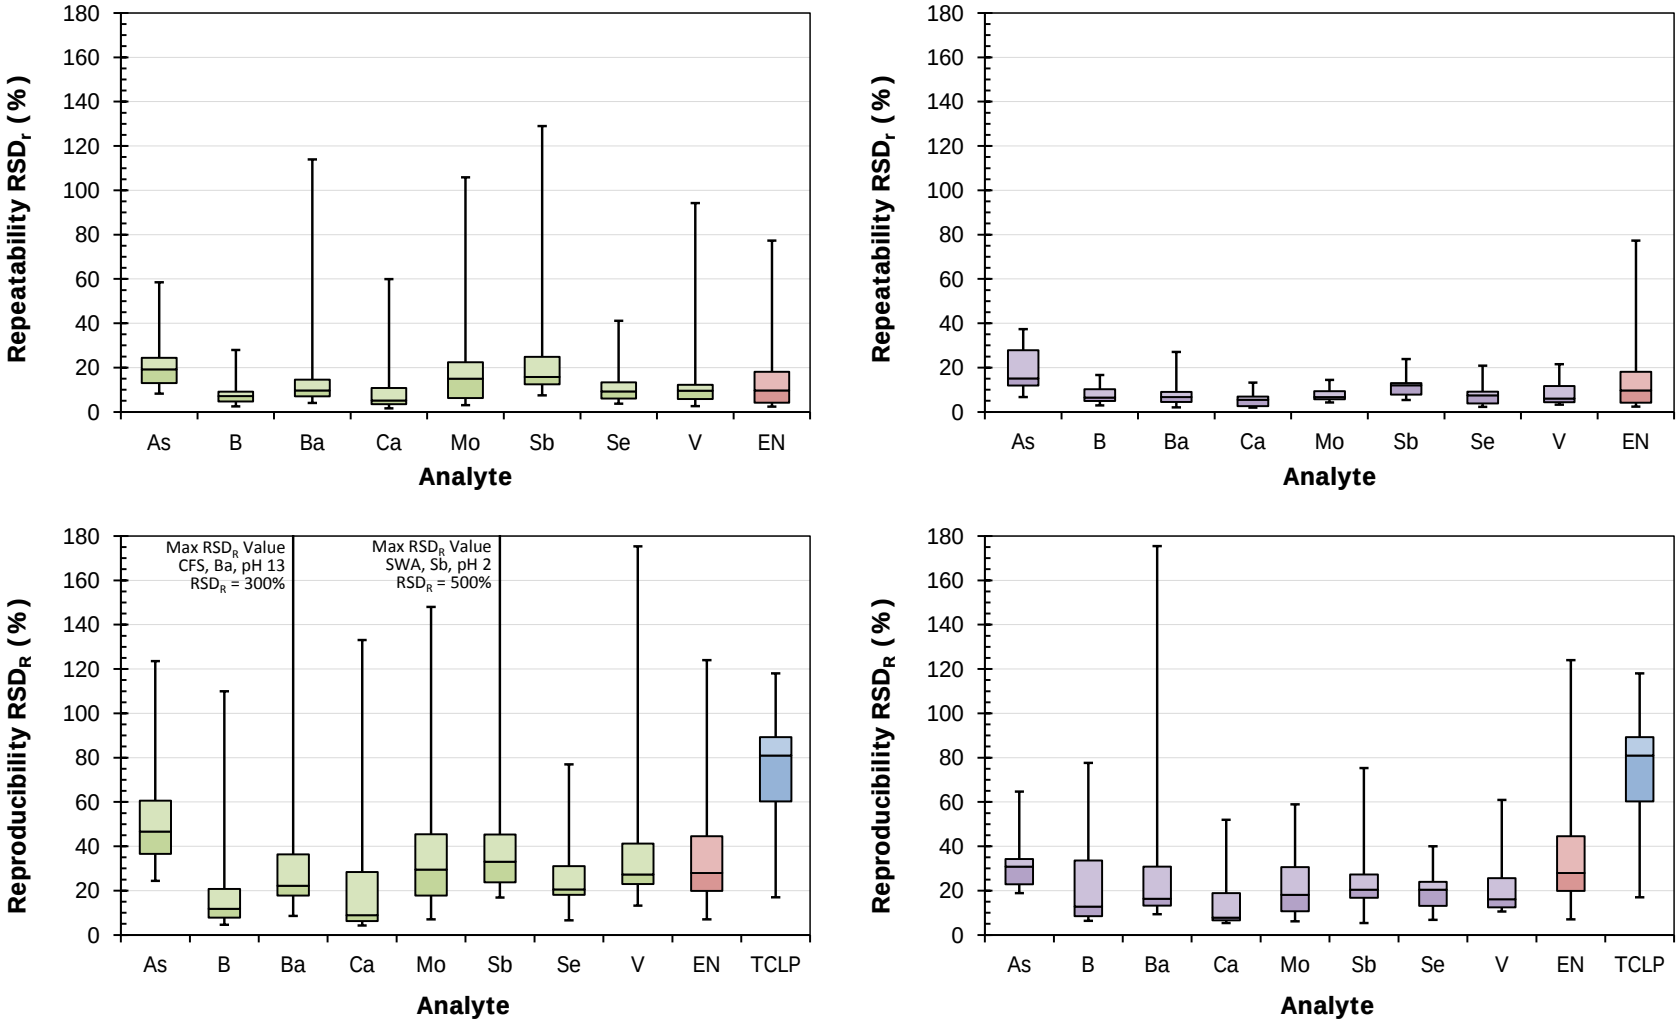

Figure 16. Method precision as a function of selected analytes in comparison to precision values reported for EN 12457-2, shown as "EN" (van der Sloot et al. 2001) and TCLP (EPA 1992a).

Note: Repeatability RSD_r (top) and reproducibility RSD_R (bottom) shown for Method 1313 (left) and Method 1316 (right). Box and whisker plots show the 25th, 50th (median) and 75th percentiles of precision data with whiskers indicating maximum and minimum values.

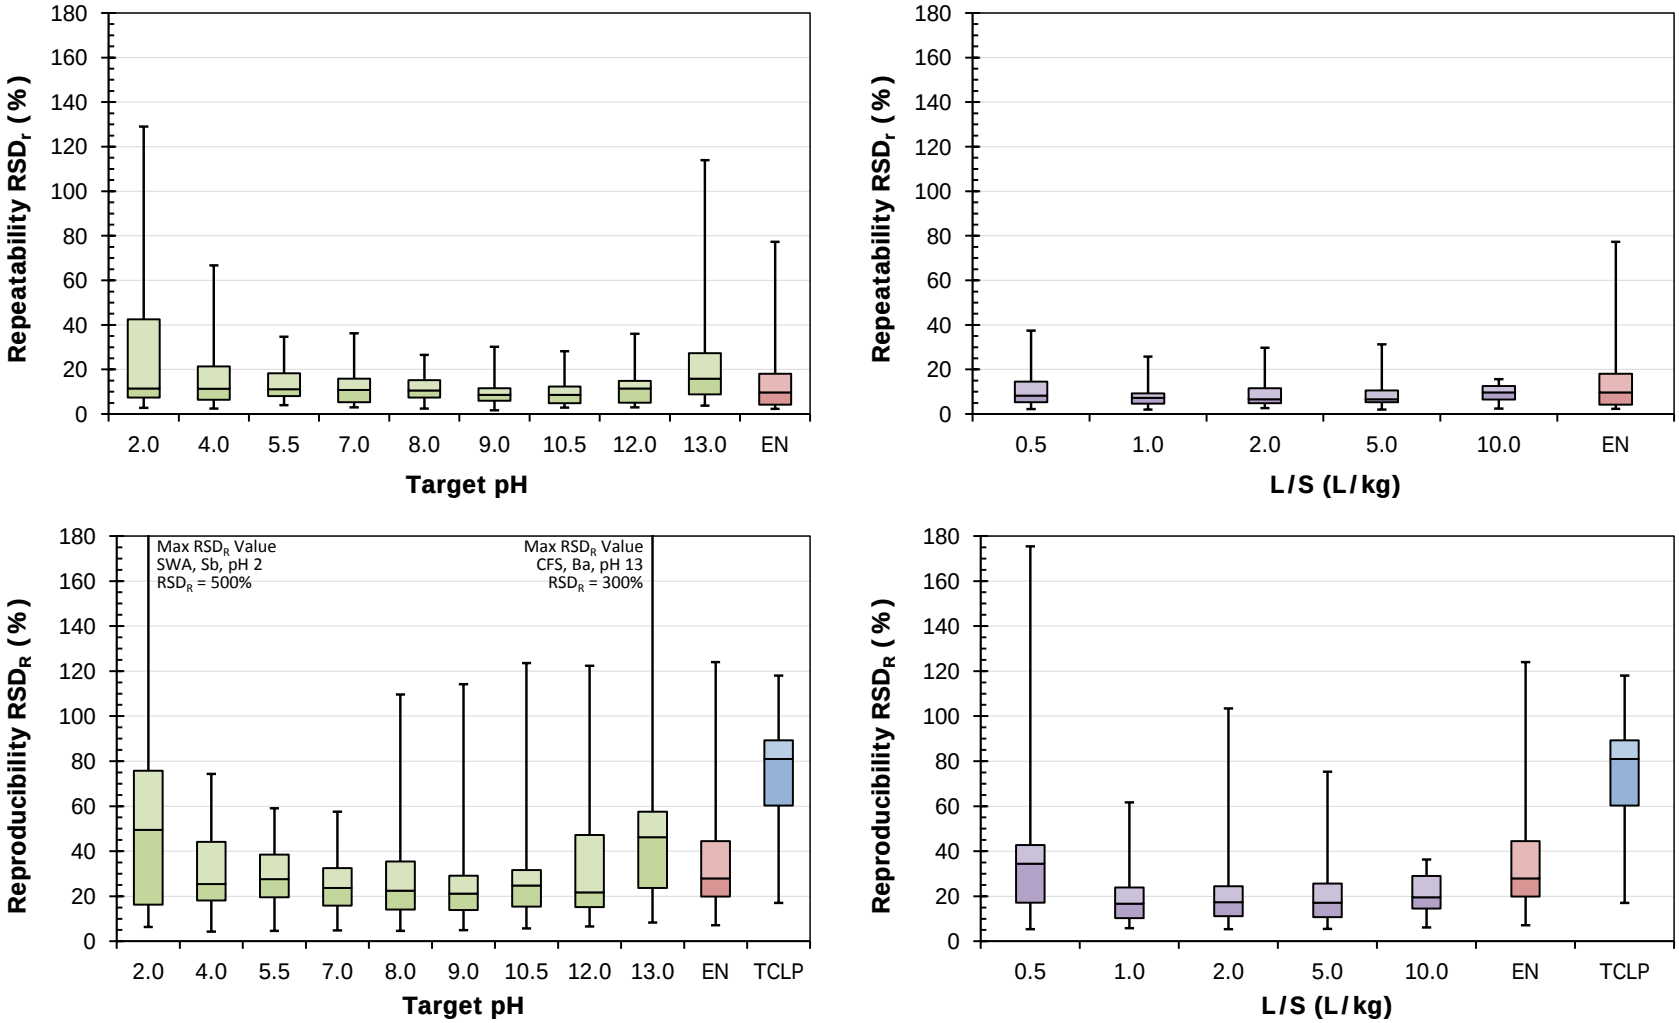

Figure 17. Method precision as a function of test parameter in comparison to precision values reported for EN 12457 (van der Sloot et al. 2001) and TCLP (EPA 1992a).

Note: Repeatability RSD_r (top) and reproducibility RSD_R (bottom) shown for Method 1313 (left) and Method 1316 (right). Box and whisker plots show the 25th, 50th (median) and 75th percentiles of precision data with whiskers indicating maximum and minimum values.

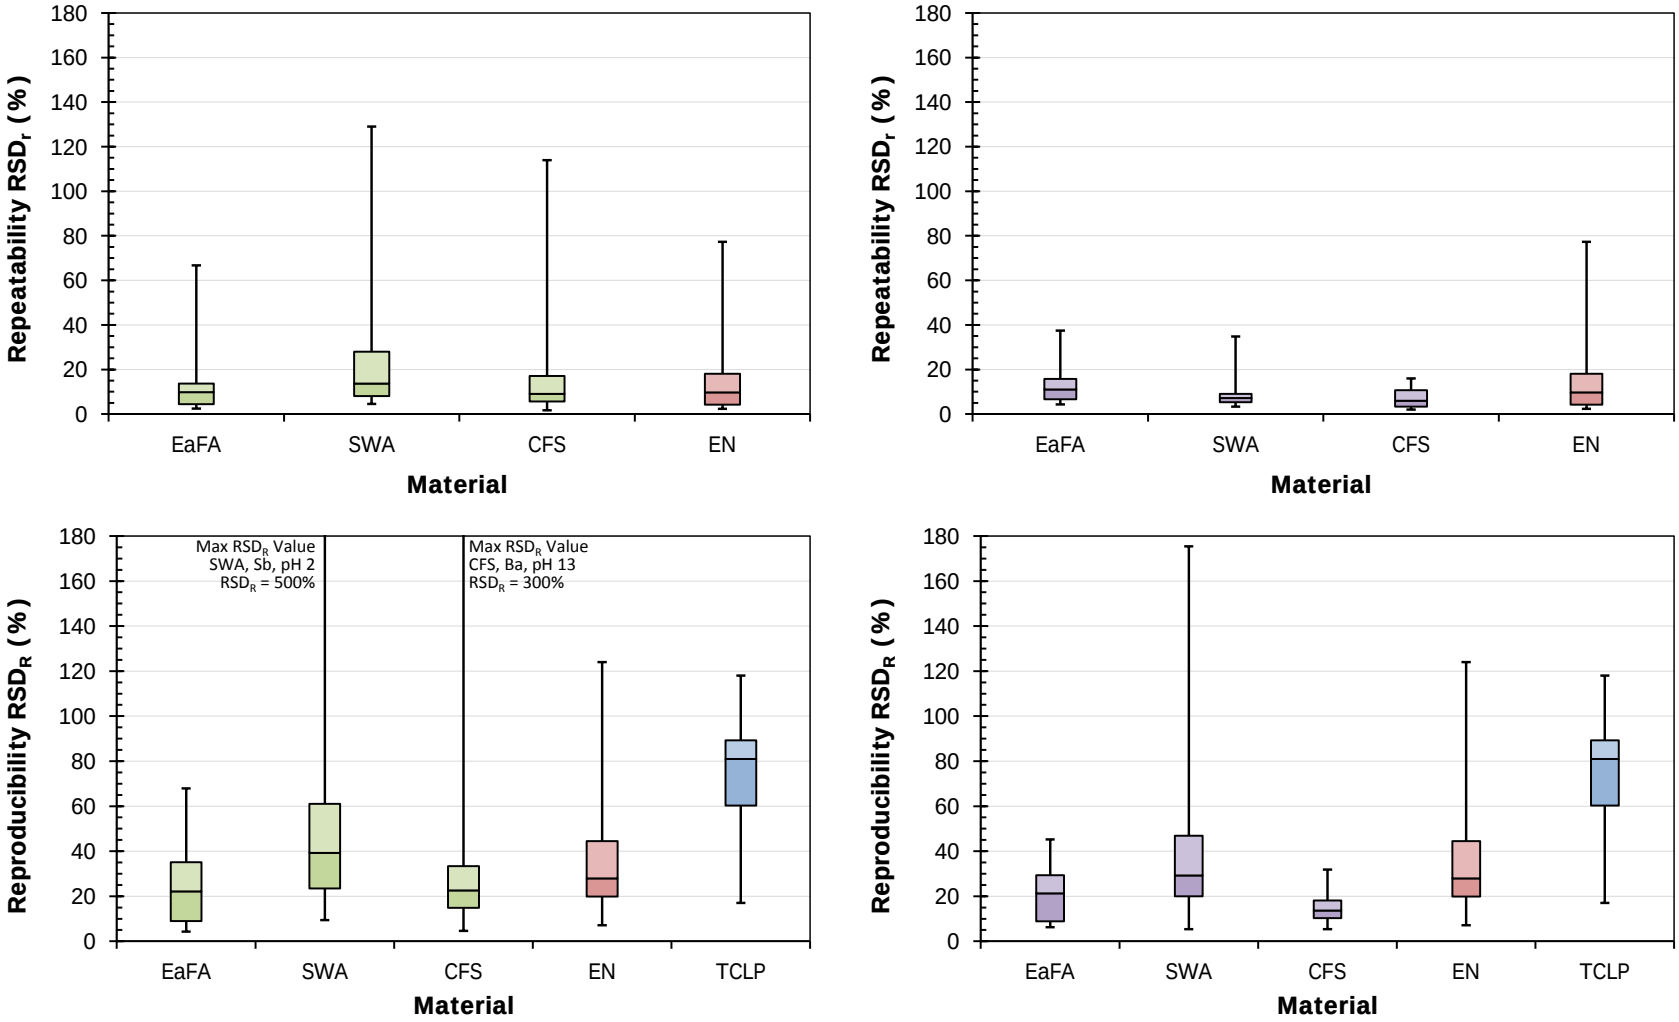

Figure 18. Method precision as a function of material in comparison to precision values reported for EN 12457 (van der Sloot et al. 2001) and TCLP (EPA 1992a).

Note: Repeatability RSD_r (top) and reproducibility RSD_R (bottom) shown for Method 1313 (left) and Method 1316 (right). Box and whisker plots show the 25th, 50th (median) and 75th percentiles of precision data with whiskers indicating maximum and minimum values.

COMPARISON OF ANALOGOUS EU LEACHING TEST RESULTS TO METHOD 1313 VALIDATION STATISTICS

Two European laboratories, the Energy Research Centre of the Netherlands (ECN) and DHI Denmark, offered time and effort to conduct European test methods for pH-dependent release for comparison to Method 1313. The two test methods are technical specifications[15] of the Comité Européen de Normalisation (CEN). Although initially designed to test waste materials, the approach of these methods has been adapted under the International Standards Organization (ISO) program for soils and soil materials (ISO/TS 21267, 2007).

EU Test Method Descriptions (CEN/TS 14429 and CEN/TS 14497)

Separate sample portions are extracted in parallel at a fixed L/S ratio of 10 mL/g in dilute acid or base solutions in order to reach stationary pH values at the end of the extraction period. Sample portions of 15, 30, or 60 g (depending on sample heterogeneity and volumes of extractant required for chemical analysis) are prepared to have a grain size with 95% (m/m) less than 1 mm. Any particle size reduction is conducted by crushing. At least eight final pH values are required, covering at the minimum the range pH 4 – pH 12 (including the lowest value ≤4 and the highest value ≥12). The maximum pH differential between final pH points shall not exceed 1.5 pH units. The amounts of acid or base needed to cover the pH range can be derived from the results of a preliminary titration, from available experimental data on the material to be tested or from an arbitrary division of the predetermined maximum consumption of acid and base. The tests are carried out at a fixed contact time of 48 hours at which time equilibrium conditions are assumed for most constituents. The equilibrium condition is verified by a pH difference of less than 0.3 pH units between measurements taken after 44 hours and 48 hours. The results are expressed in mg/L of constituents for each final pH value. The quantity of acid or base that is added is recorded for each final pH value in moles of H^+/kg of dry material with base additions expressed as negative values.

The primary difference between these two EU methods is how the extraction solution is introduced to the test portion:

- CEN/TS 14429 – Test portions are contacted with extraction solutions in a closed vessel with acid/base introduction through initial addition of extraction fluid. At the start of the test, the extraction solutions are prepared and divided evenly into three fractions. A fraction of extraction solution is added to the extraction bottle at the start of the test, after 30 minutes, and after 2 hours.
- CEN/TS 14497 – Test portions are placed into an open vessel with reagent water and acid/base is introduced via automated pH control. The method specifies that acid or base addition between

[15] The comparative European methods are designated as "technical specifications" with a TS designation, denoting a method definition has resulted from a multi-national consensus process and has been approved by a CEN technical committee. The TS designation, however, means that interlaboratory validation studies to assess precision have not yet been conducted and that public comment and consensus approval by CEN members will be repeated when performance characteristics are available. A TS designation does not carry the status of a European standard (EN), but may be adopted as national standard.

cumulative extraction times of 44 and 48 hours shall not exceed 2% of maximum of the total acid/base addition at 48 hours.

Comparison of EU Test Results to Method 1313 Statistics

The EU methods differ little in approach and basic structure from Method 1313. Eluate concentrations from CEN/TS 14429 and 14997 are, therefore, expected to be consistent with the results of the Method 1313. Notable procedural differences between EU tests and Method 1313 include (i) open vessels in CEN/TS 14997 as opposed to closed vessels in Method 1313 and (ii) repeated opening of extraction bottles during CEN/TS 14429 to add leachant. Open and vented bottles would release gases evolved during leaching and allow contact of the extraction slurries with the atmosphere, potentially leading to oxidation of eluates which would otherwise be reducing and neutralization of pH in alkaline slurries due to carbonation. In addition, open extraction vessels allow for the release of CO_2 from carbonated materials which when trapped within closed vessels could lead to chelation of arsenic and increase in measured arsenic concentrations.

EU method results were plotted as a function of eluate pH and compared against the 95% reproducibility limit (RL) calculated using Method 1313. Figure 19 shows the comparison of EU data to the mean and RL intervals for a selection of analytes and study materials while the full set of comparisons for a wide suite of analytes is presented in Appendix G. In general, the agreement between the pH-dependent leaching data from CEN tests and the RL intervals derived from Method 1313 data is very good for most analytes in the three study materials.

Each row in the Figure 19 contains data for one of the three study materials with the left-hand panel showing a typical level of agreement between Method 1313 RL and the CEN data; and the right-hand panel showing a case with less than typical agreement. Based, in part, on observations seen in reviewing Method 1313 data for the participating laboratories, potential sources for the differences in agreement between EU and Method 1313 data may include (i) heterogeneity between laboratory samples due to storage and use at the participating laboratories (see barium in EaFA), (ii) oxidation of reducing materials in open extraction vessels during CEN/TS 14997 (see arsenic in SWA), and (iii) storage of caustic reagents in borosilicate glass (see boron in CFS). Provided that these potential sources of variation are accounted for, the data from CEN/TS 14429 and 14997 are essentially the same as those determined by Method 1313.

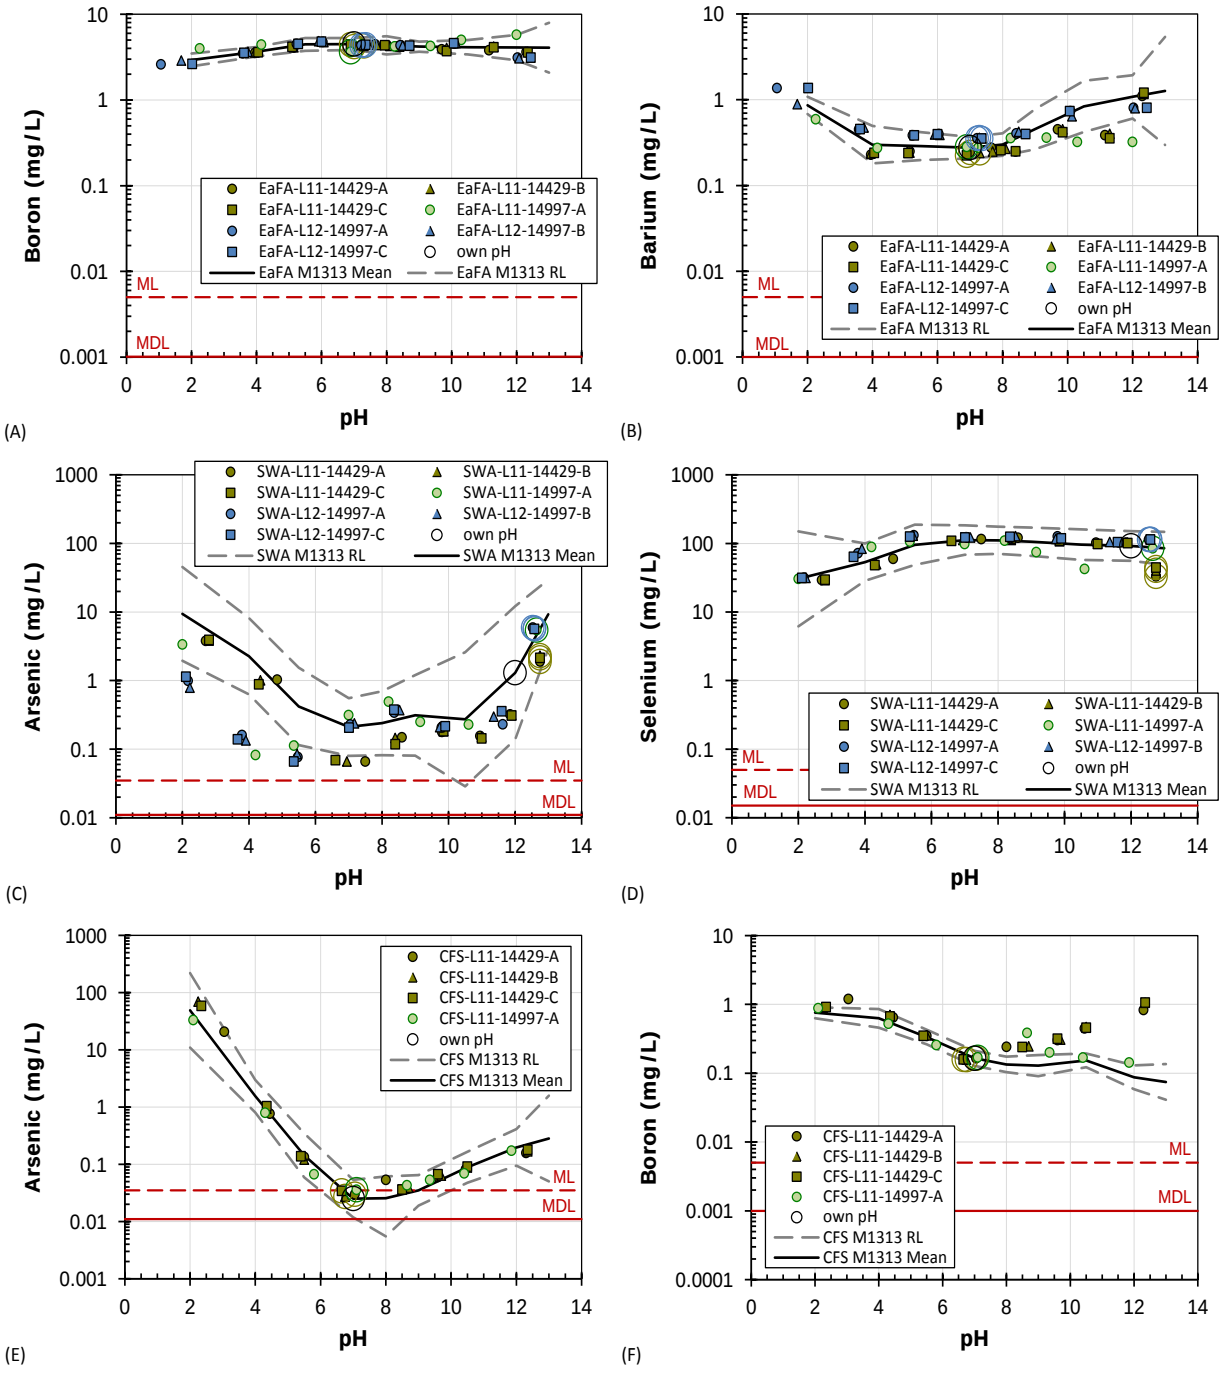

Figure 19. Leaching results from CEN tests compared to Method 1313 RL values.

Note: Data shown for (A) boron in EaFA, (B) barium in EaFA, (C) arsenic in SWA, (D) selenium in SWA, (E) arsenic in CFS and (F) boron in CFS.

SUMMARY AND CONCLUSIONS

The precision of LEAF Method 1313 and Method 1316 have been derived from interlaboratory testing using three different study materials. Method 1313 and Method 1316 are leaching test methods that characterize the liquid-solid partitioning at equilibrium between a solid material and a contacting leaching solution as functions of pH or liquid-solid ratio, respectively. The three material types were intended to challenge the performance of the method over the range of materials seen in waste management activities. For each test method, ten participating laboratories were asked to provide filtered and preserved eluates from triplicate tests runs on each of the study materials. Although the number of participating laboratories varied for each study material, seven to eleven laboratories provided data for each test method. ARCADIS-US, Inc. served as a reference laboratory and provided six test replicates of each material for both methods. Eluates were chemically analyzed by inductively coupled plasma-optical emission spectroscopy at Vanderbilt University in order to select a list of ten analytes for further study based on concentration levels and EPA significance.

The collection and management of the large data set was achieved using standardized Excel templates in conjunction with LeachXS data evaluation software. The results were processed using $\log_{10}$ transformation and linear interpolation/extrapolation to yield a set of data used in statistical analysis. Statistical measurements of data spread, within-laboratory standard deviation, between-laboratory standard deviation and overall standard deviation were calculated for ten selected analytes from each material. The reference laboratory data were used to develop intervals for 95% prediction limits about the mean which were compared to 95% robust confidence limits about the median of all the means from each laboratory. For Method 1313 test data, the process of linear interpolation of collected data was shown to induce variance in some analytes with strongly changing pH-dependence curves. Interpolation was necessary for normalize collected data, that varied with both pH and concentration, to Method 1313 target pH values. However, the interpretation approach was not considered to affect the ability of the test to be used for regulatory purposes as no significant deviation was seen in environmentally relevant pH ranges (e.g., between pH 5 and pH 9) and at maxima of the pH-dependence curve. Measurement of extreme pH values, calibration of pH meters to a narrow pH range, and reagent storage practices were seen as potential, and more common, sources of variation in test results.

Variance components were calculated based on the equations of a one-way analysis of variance in order to determine within-laboratory, between-laboratory and overall standard deviations. Repeatability and reproducibility statistics were derived from the within-laboratory and overall standard deviation values, respectively. Using the data from the eight analytes common to all materials, the overall median values of precision were estimated as the repeatability relative standard deviation (RSD_r) and reproducibility relative standard deviation (RSD_R). The median values of RSD_r were 13% for Method 1313 and 8% for Method 1316 while the median values of RSD_R were 28% for Method 1313 and 19% for Method 1316. The repeatability values indicate the expected results variation for a single operator conducting test replicates on the same materials sample while the reproducibility values represent the variation of test results for multiple laboratories conducting the test methods on a homogenized sample of material.

These precision values and the interquartile ranges of the repeatability and reproducibility as functions of selected analytes, independent method parameters (e.g., pH or liquid-solid ratio), and materials were found to be in agreement with the median precision values reported for validation of the European

standard EN 12457-2 (van der Sloot et al, 2001). The median RSD_R values for both Method 1313 and Method 1316 were considerably lower than the mean reproducibility RSD reported for TCLP (EPA 1992a).

In order to compare pH-dependence results from Method 1313 to those of similar leaching methods in use throughout the European Union, two European laboratories were asked to test the validation study materials using CEN/TS 14429 and CEN/TS 14997. These pH-dependence leaching methods are standardized through the Comité Européen de Normalisation as technical specifications which are available for adoption as national standards but have yet to undergo interlaboratory validation. The eluate concentration results of CEN/TS 14429 and 14997 were compared directly with the 95% RCL intervals from Method 1313. The comparisons showed only minor differences in eluate concentrations for a minority of analytes which are likely due to sample heterogeneity during storage prior to testing and oxidation during leaching in open vessels. In general, the good agreement between Method 1313 and EU leaching procedures indicated that all three methods adequately characterized the pH-dependent leaching behavior of constituents in the three study materials.

Based on the method validation results and comparison presented in this report, the following statements regarding LEAF Method 1313 and Method 1316 may be made:

Procedural Considerations

- Accurate pH measurements are essential to the performance of these methods, especially Method 1313. Measurement of pH should consider appropriate instrument calibration, standardization with buffer solutions that span the resultant extract pH range to the greatest degree possible and proper pH measurement techniques. Measurements should be taken as rapidly as practical after gross solid-liquid phase separation (e.g., settling or centrifugation) to avoid carbonation of alkaline solutions with limited pH buffering capacity.
- Reagents should be prepared fresh before each run of these test methods. If reagents are to be stored, containers made from compatible materials must be used (e.g., strong bases should not be stored in borosilicate glass if boron is considered to be a constituent of concern).
- The data templates are recommended for use with Method 1313 and Method 1316 to provide uniform calculations, data collection, and data input into LeachXS which greatly facilitates management of large data sets. LeachXS Lite is a simplified, free version of LeachXS that can assist method users with method implementation as well as data management, graphing and reporting.
- Sample heterogeneity was cited as a potential cause of high variation in precision data for SWA material. Heterogeneity can result from variations in the solid material (e.g., resulting from hand mixing of SWA or incomplete dissolution of metal salts in the matrix), aging of the cured materials, or by exposure of leaching solutions to the atmosphere (e.g., oxidation during open vessel leaching in CEN/TS 14997). More rigorous solid material handling of the heterogeneous SWA material and changes in the CEN methods to limit exposure of leaching solutions to the atmosphere may lead to improvements in leaching data consistency.

Data Validation Approach

- Although the linear interpolation/extrapolation used with Method 1313 may introduce some degree of variability to the statistical analysis, the effects are limited to areas of the pH-dependence curve with a steep slope or significant curvature. The introduced variability has been shown to occur at local minima in concentration as a function of pH or at extreme (very low or very high) pH values which are anticipated to occur infrequently in the environment. Therefore, variability induced by linearization is not expected to impact the use of the method as part of decision making processes.
- The data evaluation methods used (e.g., data filtering, interpolation and extrapolation, statistical analysis) appear to be robust and provide a useful basis for evaluation of the results.

Repeatability and Reproducibility

- Repeatability of these methods generally is expected to be approximately 5-15% of the mean concentration value which is consistent with the variability associated with many chemical analytical methods. Reproducibility is expected to be approximately within a factor of 2 (e.g., the mean ± 50%) in the pH and L/S domains with good repeatability. Greater width in Method 1313 reproducibility relative standard deviation is expected at the extremes of pH and when there are steep changes in analyte concentrations as a function of pH. For Method 1316, the reproducibility relative standard deviation is expected to increase at low L/S values.
- Observed reproducibility was consistent with prior experience across multiple laboratories during method development.
- The repeatability and reproducibility results suggest that sample heterogeneity is likely to be the dominant source of variability associated with broader use of these leaching test methods. As sample heterogeneity is an issue intrinsic to the study of waste materials, there should be no implications of this finding to the broader use of the LEAF methods.
- Commercial and non-commercial laboratories should be readily able to implement Method 1313 and Method 1316 for a wide range of material types with a degree of repeatability and reproducibility consistent with current regulatory leaching methods in the U.S. and Europe.

REFERENCES

ASTM Standard E691 (1987) "Standard Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method," ASTM International, West Conshohocken, PA, 1987.

ASTM Standard E1488 (2002) "Standard Guide for Statistical Procedures to Use in Developing and Applying Test Methods," ASTM International, West Conshohocken, PA, 1987.

CEN (2001) EN 12457 Characterization of Waste – Leaching – Compliance Test for Leaching of Granular Waste Materials and Sludges – Part 2: One stage batch test at a liquid to solid ratio of 10 L/kg for materials with particle size below 4 mm (with or without size reduction), CEN, Brussels, Belgium.

CEN/TS 14429 (2005) Characterization of Waste – Leaching Behaviour Tests – Influence of pH on Leaching with Initial Acid/base Addition, CEN, Brussels, Belgium.

CEN/TS 14997 (2005) Characterization of Waste – Leaching Behaviour Tests – Influence of pH on Leaching with Continuous pH Control, CEN, Brussels, Belgium.

Currie, L.A. and G. Svehla (1994) "Nomenclature for the presentation of results of chemical analysis (IUPAC recommendations 1994)," *Pure and Applied Chemistry*, 66(3), 595-608.

Daszykowski, M., K. Kaczmarek, Y. Vander Heyden, and B. Walczak (2007) "Robust statistics in data analysis – A review of basic concept," *Chemometrics and Intelligent Laboratory Systems*, 85, 203-219.

Ellison, S.L.R., V.J. Barwick, and T.J.D. Farrant (2009) *Practical Statistics for the Analytical Scientist: A Bench Guide*, 2nd Edition, RSC Publishers, Cambridge, UK, 268 pp.

EPA (1992a) SW-846 Method 1311 "Toxicity Characteristic Leaching Procedure," Test Methods for Evaluating Solid Waste, Physical/Chemical Methods (SW-846), U.S. Environmental Protection Agency, http://www.epa.gov/osw/hazard/testmethods/sw846/pdfs/1311.pdf.

EPA (1992b) Guidance for Methods Development and Methods Validation for the RCRA Program. U.S. Environmental Protection Agency, http://www.epa.gov/osw/hazard/testmethods/pdfs/methdev.pdf.

EPA (1996) SW-846 Method 3052 "Microwave Assisted Acid Digestion of Siliceous and Organically Based Matrices," Test Methods for Evaluating Solid Waste, Physical/Chemical Methods (SW-846), U.S. Environmental Protection Agency, http://www.epa.gov/osw/hazard/testmethods/sw846/pdfs/3052.pdf.

EPA (2003) "Technical Support Document for the Assessment of Detection and Quantitation Approaches", U.S. Environmental Protection Agency, Office of Water, February 2003.

EPA (2004) SW-846 Method 9060 "Total Organic Carbon," Test Methods for Evaluating Solid Waste, Physical/Chemical Methods (SW-846), U.S. Environmental Protection Agency, http://www.epa.gov/osw/hazard/testmethods/sw846/pdfs/9060a.pdf.

EPA (2007a) SW-846 Method 3051 "Microwave Assisted Acid Digestion of Sediments, Sludges, Soils, and Oils," Test Methods for Evaluating Solid Waste, Physical/Chemical Methods (SW-846), U.S. Environmental Protection Agency, http://www.epa.gov/osw/hazard/testmethods/sw846/pdfs/3051.pdf.

EPA (2007b) SW-846 Method 6010 "Inductively Coupled Plasma-Atomic Emission Spectroscopy," Test Methods for Evaluating Solid Waste, Physical/Chemical Methods (SW-846), U.S. Environmental Protection Agency, http://www.epa.gov/osw/hazard/testmethods/sw846/pdfs/6010c.pdf.

EPA (2007c) SW-846 Method 6020 "Inductively Coupled Plasma-Mass Spectroscopy," Test Methods for Evaluating Solid Waste, Physical/Chemical Methods (SW-846), U.S. Environmental Protection Agency, http://www.epa.gov/osw/hazard/testmethods/sw846/pdfs/6020a.pdf.

EPA (2007d) SW-846 Method 9056 "Determination of Inorganic Anions by Ion Chromatography," Test Methods for Evaluating Solid Waste, Physical/Chemical Methods (SW-846), U.S. Environmental Protection Agency, http://www.epa.gov/osw/hazard/testmethods/sw846/pdfs/9056a.pdf.

Garrabrants, A.C., D.S. Kosson, H.A. van der Sloot, F. Sanchez, and O. Hjelmar (2010) "Background information for the Leaching Environmental Assessment Framework (LEAF) Test Methods," EPA-600/R-10/170, U.S. Environmental Protection Agency, Air Pollution Prevention and Control Division, December 2010.

Huber, P.J. (1968) "Robust confidence limits," *Probability Theory and Related Fields*, 10(4), 269-278.

Horwitz, W and R. Albert (2006) "The Horwitz ratio (HorRat): A useful index of method performance with respect to precision," *Journal of AOAC International*, 89(4), 1095-1109.

ISO/TS 21267-4 (2007) Soil Quality – Leaching Procedures for Subsequent Chemical and Ecotoxicological Testing of Soil and Soil Materials – Part 4: Influence of pH on Leaching with Initial Acid/base Addition, ISO, Geneva, Switzerland.

ISO (1994) ISO 5725-1 Accuracy (Trueness and Precision) of Measurement Methods and Results – Part 1: General Principles and Definitions, International Organization for Standards, Geneva, Switzerland.

Kosson, D.S., F. Sanchez, P. Kariher, L.H. Turner, R. DeLapp, and P. Seignette (2009) "Characterization of Coal Combustion Residues from Electric Utilities – Leaching and Characterization Data," EPA-600/R-09/151, U.S. Environmental Protection Agency, Air Pollution Prevention and Control Division, December 2009.

Kosson, D.S, H.A. van der Sloot, F. Sanchez and A.C. Garrabrants (2002) "An integrated framework for evaluating leaching in waste management and utilization of secondary materials," *Environmental Engineering Science*, 19(3), 159-204.

Linsinger, T.P.J. and R.D. Josephs (2006) "Limitations of the application of the Horwitz equation," *Trends in Analytical Chemistry*, 25(11), 1125-1130.

Mandel, J. (1991) "The validation of measurement through interlaboratory studies", *Chemometrics and Intelligent Laboratory Systems*, 11, 109-119.

Maronna, R., D. Martin, and V. Yohai (2006) *Robust Statistics: Theory and Methods*", John Wiley & Sons, Ltd., Chichester, UK.

Rao, P.V. (1998) *Statistical Research Methods in the Life Sciences*, Duxbury Press, Pacific Grove CA.

Sanchez, F., R. Keeney, D. Kosson, and R. DeLapp (2006) "Characterization of Mercury-enriched Coal Combustion Residues from Electric Utilities using Enhanced Sorbents for Mercury Control," EPA-600/R-06/008, U.S. Environmental Protection Agency, Air Pollution Prevention and Control Division, February 2006.

Sanchez, F., D. Kosson, R. Keeney, R. DeLapp, L. Turner and P. Kariher (2008) "Characterization of Coal Combustion Residues from Electric Utilities using Wet Scrubbers for Multi-pollutant Control," EPA-600/R-08/077, U.S. Environmental Protection Agency, Air Pollution Prevention and Control Division, July 2008.

van der Sloot, H.A., L. Heasman, and P. Quevauviller (1997) *Harmonization of Leaching/Extraction Tests*, Elsevier Science, Amsterdam.

van der Sloot, H.A., O. Hjelmar, J. Berre Hansen, J. Woitke, P. Lepom, R. Leschber, B. Bartet, and N. Debrucker (2001) Validation of CEN/TC 292 Leaching Tests and Eluate Analysis Methods PrEN 12457 Part 1-4, ECN-C-01-117, ENV 13370 and ENV 12506 in Co-operation with CEN/TC 308.

Appendix A. Method 1313

DRAFT METHOD 1313[1]

LIQUID-SOLID PARTITIONING AS A FUNCTION OF EXTRACT pH USING A PARALLEL BATCH EXTRACTION PROCEDURE

SW-846 is not intended to be an analytical training manual. Therefore, method procedures are written based on the assumption that they will be performed by analysts who are formally trained in at least the basic principles of chemical analysis and in the use of the subject technology.

In addition, SW-846 methods, with the exception of required method use for the analysis of method-defined parameters, are intended to be guidance methods which contain general information on how to perform an analytical procedure or technique which a laboratory can use as a basic starting point for generating its own detailed Standard Operating Procedure (SOP), either for its own general use or for a specific project application. The performance data included in this method are for guidance purposes only, and are not intended to be and must not be used as absolute quality control (QC) acceptance criteria for purposes of laboratory quality control or accreditation.

1.0 SCOPE AND APPLICATION

1.1 This method is designed to provide aqueous extracts representing the liquid-solid partitioning (LSP) curve as a function of pH for inorganic constituents (e.g., metals and radionuclides), semi-volatile organic constituents (e.g., polycyclic aromatic hydrocarbons or PAHs) and non-volatile organic constituents (e.g., dissolved organic carbon) in solid materials. The LSP curve is evaluated as a function of final extract pH at a liquid-to-solid ratio (L/S) of 10 mL extractant/g dry sample (g-dry) and conditions that approach liquid-solid chemical equilibrium. This method also yields the acid/base titration and buffering capacity of the tested material at an L/S of 10 mL extractant/g-dry sample. The analysis of extracts for dissolved organic carbon and the solid phase for total organic carbon allow for the evaluation of the impact of organic carbon release and the influence of dissolved organic carbon on the LSP of inorganic constituents.

1.2 This method is intended to be used as part of an environmental leaching assessment for the evaluation of disposal, beneficial use, treatment effectiveness and site remediation options. The method is not required by federal regulations to determine whether waste passes or fails the toxicity characteristic as defined at 40 CFR 261.24.

1.3 This method is suitable for assessing the leaching potential of a wide range of solid materials. Examples of solid materials include: industrial wastes, soils, sludges, combustion residues, sediments, stabilized materials, construction materials, and mining wastes.

1.4 This method is a leaching characterization method that is used to provide values for intrinsic material parameters that control leaching of inorganic and some organic

[1] This method has been derived from the SR002 procedure (Ref. 2) using EPA reviewed and accepted methodologies (see Refs. 4-6). The method is analogous to pH-dependence methods CEN/TS14429 (Ref. 8) and CEN/TS14997 (Ref. 9) developed for the Comité Européen de Normalisation (CEN).

species under equilibrium conditions. This test method is intended as a means for obtaining a series of extracts of a solid material (i.e., the eluates), which may be used to estimate the LSP (e.g., solubility and release) of constituents as a function of pH under the laboratory conditions described in the method. Eluate constituent concentrations may be used in conjunction with information regarding environmental management scenarios to estimate the anticipated leaching concentrations, and release rate and extent for individual material constituents under the management conditions evaluated. Eluate constituent concentrations generated by this method may also be used along with geochemical speciation modeling to infer the mineral phases that control the LSP in the pore structure of the solid material.

1.5 This method is not applicable for characterizing the release of volatile organic analytes (e.g., benzene, toluene, xylenes).

1.6 The relationships between eluate concentrations observed from this method and field leachate must be considered in the context of the material being tested and the field scenario being evaluated. This method provides solutions with concentrations considered indicative of leachates under field conditions at comparable ranges of pH for the case when the LSP is controlled by aqueous phase saturation of the constituent of interest. When LSP is controlled by the amount of the constituent present in the solid that may dissolve (i.e., for highly soluble species), the mass released (mg/kg), rather than the concentration, is indicative of field conditions.[2]

1.7 The maximum concentration of constituent released over the range of method pH conditions ($2 \leq pH \leq 13$) may be considered an estimate of the maximum possible release of the constituent under field leaching conditions for intermediate time frames (because the method pH range will encompass and typically exceed the field pH range, using pH values both greater than and less than the field pH range). .

1.8 The solvents used in this method include dilute solutions of nitric acid (HNO_3) and potassium hydroxide (KOH) in reagent water.

1.9 Analysts are advised to take reasonable measures to ensure that the sample is homogenized to the extent practical, prior to employment of this method. Particle-size reduction may provide additional assurance of sample homogenization and also facilitate achievement of equilibrium during the test procedure. Table 1 of this method designates a recommended minimum dry mass of sample to be added to each extraction vessel and the associated extraction contact time as a function particle diameter. If the heterogeneity of the sample is suspected as the cause of unacceptable precision in replicate test results or is considered significant based on professional judgment, the sample mass used in the test procedure may be increased to a greater minimum dry mass than that shown in Table 1 with the amount of extractant increased proportionately to maintain the designated L/S.

1.10 In the preparation of solid materials for use in this method, particle-size reduction of samples with a large grain size is performed in order to enhance the approach towards equilibrium under the designated contact time interval of the extraction process. The

[2] The concentrations of soluble species (e.g., Na, K, Cl, B) may not be controlled by aqueous phase saturation, but by the liquid-to-solid ratio. In such cases, the mass released is consistent with field conditions and the field leachate concentrations (mg/L) could be estimated by adjusting the mass release (mg/kg) for the field L/S (L/kg). Alternatively for these cases, leachate concentrations may be more consistent with L/S-dependent testing using Method 1314 or Method 1313.

extract contact time for samples reduced to a finer maximum particle size will consequently be shorter (see Table 1).

1.11 Prior to employing this method, analysts are advised to consult the base method for each type of procedure that may be employed in the overall analysis (e.g., Methods 9040, 9045, and 9050, and the determinative methods for the target analytes), QC acceptance criteria, calculations, and general guidance. Analysts also should consult the disclaimer statement at the front of the manual and the information in Chapter Two for guidance on the intended flexibility in the choice of methods, apparatus, materials, reagents, and supplies, and on the responsibilities of the analyst for demonstrating that the techniques employed are appropriate for the analytes of interest, in the matrix of interest, and at the concentration levels of concern.

In addition, analysts and data users are advised that, except where explicitly specified in a regulation, the use of SW-846 methods is not mandatory in response to Federal testing requirements. The information contained in this method is provided by EPA as guidance to be used by the analyst and the regulated community in making judgments necessary to generate results that meet the data quality objectives for the intended application. Guidance on defining data quality objectives can be obtained at http://www.epa.gov/QUALITY/qs-docs/g4-final.pdf

1.12 Use of this method is restricted to use by, or under supervision of, properly experienced and trained personnel. Each analyst must demonstrate the ability to generate acceptable results with this method as described in Section 9.5.

2.0 SUMMARY OF METHOD

This method consists of nine parallel extractions of a particle size-reduced solid material at target pH values spanning the range from pH 2 to 13, with pH control by adition of dilute acid or base and reagent water. A flowchart for performing this method is shown in Figure 1. Particle-size reduction of the material to be tested is performed according to Table 1. A schedule of acid and base additions is formulated from a pre-test titration curve or prior knowledge indicating the required equivalents/g acid or base to be added to the series of extraction vessels so as to yield a series of eluates having specified pH values in the range of 2-13. In addition to the nine test extractions, three method blanks without solid sample are carried through the procedure in order to verify that analyte interferences are not introduced as a consequence of reagent impurities or equipment contamination. The twelve bottles (i.e., nine test positions and three method blanks) are tumbled in an end-over-end fashion for a specified contact time, which depends on the particle size of the sample (see Table 1). At the end of the specified contact interval, the liquid and solid phases are roughly separated via settling or centrifugation. Extract pH and specific conductivity measurements are then made on an aliquot of the liquid phase and the remaining bulk of the eluate is clarified by either pressure or vacuum filtration. Analytical samples of the filtered eluate are collected and preserved as appropriate for the desired chemical analyses. The eluate concentrations of COPCs are determined and reported. In addition, COPC concentrations may be plotted as a function of eluate pH and compared to quality control and assessment limits for the interpretation of method results.

3.0 DEFINITIONS

3.1 Constituent of potential concern (COPC) — A chemical species of interest, which may or may not be regulated, but may be characteristic of release-controlling properties of the sample geochemistry.

3.2 Release — The dissolution or partitioning of a COPC from the solid phase to the aqueous phase during laboratory testing (or under field conditions). In this method, mass release is expressed in units of mg COPC/kg dry solid material.

3.3 Liquid-solid partitioning (LSP) — The distribution of COPCs between the solid and liquid phases at the conclusion of the extraction.

3.4 Liquid-to-solid ratio (L/S) — The fraction of the total liquid volume (including the moisture contained in the “as used” solid sample) to the dry mass equivalent of the solid material. L/S is typically expressed in volume units of liquid per dry mass of solid material (mL/g-dry).

3.5 “As-tested” sample — The solid sample at the conditions (e.g., moisture content and particle-size distribution) present at the time of the start of the test procedure. The “as-tested” conditions will differ from the "as-received" sample conditions if particle-size reduction and drying were necessarily performed.

3.6 Dry-mass equivalent — The mass of “as-tested” (i.e., “wet”) sample that equates to the mass of dry solids plus associated moisture, based on the moisture content of the “as-tested” material. The dry-mass equivalent is typically expressed in mass units of the “as-tested” sample (g).

3.7 Refer to Chapter One and the equipment manufacturers’ instructions for definitions that may be relevant to this procedure.

4.0 INTERFERENCES

4.1 Solvents, reagents, glassware, and other sample processing hardware may yield artifacts and/or interferences to sample analysis. All of these materials must be demonstrated to be free from interferences under the conditions of the analysis by analyzing method blanks. Specific selection of reagents and purification of solvents by distillation in all-glass systems may be necessary. Refer to each method to be used for specific guidance on quality control procedures and to Chapters Three and Four for general guidance on the cleaning of laboratory apparatus prior to use.

4.2 If potassium is a COPC, the use of KOH as a base reagent will interfere with the determination of actual potassium release. In this case, sodium hydroxide (NaOH) of the same grade and normality may be used as a substitute.

5.0 SAFETY

5.1 This method does not address all safety issues associated with its use. The laboratory is responsible for maintaining a safe work environment and a current awareness file of OSHA regulations regarding the safe handling of the chemicals listed in this method. A reference file of material safety data sheets (MSDSs) should be available to all personnel involved in these analyses.

5.2 During preparation of extracts and processing of extracts, some waste materials may generate heat or evolve potentially harmful gases when contacted with acids and bases. Adequate prior knowledge of the material being tested should be used to establish appropriate personal protection and workspace ventilation.

6.0 EQUIPMENT AND SUPPLIES

The mention of trade names or commercial products in this manual is for illustrative purposes only, and does not constitute an EPA endorsement or exclusive recommendation for use. The products and instrument settings cited in SW-846 methods represent those products and setting used during the method development or subsequently evaluated by the Agency. Glassware, reagents, supplies, equipment, and setting other than those listed in this manual may be employed provided that method performance appropriate for the intended application has been demonstrated and documented. This section does not list common laboratory glassware (e.g., beakers and flasks) which nonetheless may be required to perform the method.

6.1 Extraction vessels

6.1.1 Twelve wide-mouth bottles (i.e., nine for test positions plus three for method blanks) constructed of inert material, resistant to high and low pHs and interaction with COPCs as described in the following sections.

6.1.1.1 For the evaluation of inorganic COPCs, bottles made of high density polyethylene (HDPE) (e.g., Nalgene #3140-0250 or equivalent), polypropylene (PP), or polyvinyl chloride (PVC) are recommended.

6.1.1.2 For the evaluation of non-volatile organic and mixed organic/inorganic COPCs, bottles made of glass or Type 316 stainless steel are recommended. Polytetra-fluoroethylene (PTFE) is not recommended for non-volatile organics due to the sorption of species with high hydrophobicity (e.g., PAHs). Borosilicate glass is recommended over other types of glass, especially when inorganic analytes are of concern.

6.1.2 The extraction vessels must be of sufficient volume to accommodate both the solid sample and an extractant volume, based on an L/S of 10 ± 0.5 mL extractant/g-dry. The head space in the bottle should be minimized to the extent possible when semi-volatile organics are COPCs. For example, Table 1 indicates that 250-mL volume bottles are recommended when the minimum 20 g-dry mass equivalent is contacted with 200 mL of extractant.

6.1.3 The vessel must have a leak-proof seals that can sustain end-over-end tumbling for the duration of the designated contact time.

6.1.4 If centrifugation is anticipated to be beneficial for initial phase separation, the extraction vessels should be capable of withstanding centrifugation at 4000 ± 100 rpm for a minimum of 10 ± 2 min. Alternately, samples may be extracted in bottles that do not meet this centrifugation specification (e.g., Nalgene I-Chem #311-0250 or equivalent) and the solid-liquid slurries transferred into appropriate centrifugation vessels for phase separation as needed.

6.2 Balance — Capable of 0.01-g resolution for masses less than 500 g.

6.3 Rotary tumbler — Capable of rotating the extraction vessels in an end-over-end fashion at a constant speed of 28 ± 2 rpm (e.g., Environmental Express, Charlestown, SC or equivalent).

NOTE: The holding capacity of tumblers may vary and modifications (e.g., packing or bottle-holding inserts) may be necessary to accommodate the extraction vessels.

6.4 Filtration apparatus — Pressure or vacuum filtration apparatus composed of appropriate materials so as to maximize the collection of extracts and minimize loss of the COPCs (e.g., Nalgene #300-4000 or equivalent) (see Sec. 6.1).

6.5 Filtration membranes — Composed of polypropylene or equivalent material with an effective pore size of 0.45-µm (e.g., Gelman Sciences GH Polypro #66548 from Fisher Scientific or equivalent).

6.6 pH Meter — Laboratory model with the capability for temperature compensation (e.g., Accumet 20, Fisher Scientific or equivalent) and a minimum resolution of 0.1 pH units.

6.7 pH combination electrode — Composed of chemically-resistant materials.

6.8 Conductivity meter — Laboratory model (e.g., Accumet 20, Fisher Scientific or equivalent), with a minimum resolution of 5% of the measured value.

6.9 Conductivity electrodes — Composed of chemically-resistant materials.

6.10 Adjustable-volume pipettor — Oxford Benchmate series or equivalent The necessary delivery range will depend on the buffering capacity of the solid material and acid/base strength used in the test.

6.11 Disposable pipettor tips

6.12 Centrifuge (recommended) — Capable of centrifuging the extraction vessels at a rate of 4000 ± 100 rpm for 10 ± 2 min.

7.0 REAGENTS AND STANDARDS

7.1 Reagent-grade chemicals must be used in all tests. Unless otherwise indicated, it is intended that all reagents conform to the specifications of the Committee on Analytical Reagents of the American Chemical Society, where such specification are available. Other grades may be used, provided it is first ascertained that the reagents are of sufficiently

high purity to permit use without lessening the accuracy of the determination. Inorganic reagents and extracts should be stored in plastic to prevent interaction of constituents from glass containers.

7.2 Reagent water must be interference free. All references to water in this method refer to reagent water unless otherwise specified.

7.3 Nitric acid (2.0 N), HNO_3 – Trace-metal grade or better, purchased at strength or prepared by diluting concentrated nitric acid with reagent water. Alternate normality solutions may be used as necessary. In such cases, the amounts of HNO_3 solution added to samples should be adjusted based on the equivalents required in the schedule of acid/base additions (see Sec. 11.3).

7.4 Potassium hydroxide (1.0 N), KOH – ACS grade, purchased at strength or prepared by diluting concentrated potassium hydroxide solution with reagent water, or otherwise by dissolving 56.11 g of solid potassium hydroxide in 1 L of reagent water. Alternate normality solutions may be used as necessary. In such cases, the amounts of KOH solution added to samples should be adjusted based on the equivalents required in the schedule of acid/base additions (see Sec. 11.3).

7.5 Consult Methods 9040 and 9050 for additional information regarding the preparation of reagents required for pH and specific conductance measurements.

8.0 SAMPLE COLLECTION, PRESERVATION, AND STORAGE

8.1 See the introductory material to Chapter Three “Inorganic Analytes” and Chapter Four “Organic Analytes.”

8.2 All solid samples should be collected using an appropriate sampling plan.

8.3 All containers should be composed of materials that minimize interaction with COPCs. For further information, see Chapters Three and Four.

8.4 Preservatives should not be added to samples before extraction.

8.5 Samples can be refrigerated, unless refrigeration results in an irreversible physical change to the sample.

8.6 Analytical extracts or leachates should be preserved according to the guidance given in the individual determinative methods for the COPCs.

8.7 Extract holding times should be consistent with the holding times specified in the individual determinative methods for the COPCs.

9.0 QUALITY CONTROL

9.1 Refer to Chapter One for guidance on quality assurance (QA) and quality control (QC) protocols. When inconsistencies exist between QC guidelines, method-specific QC criteria take precedence over both technique-specific criteria and those criteria given in Chapter One, and technique-specific QC criteria take precedence over the criteria in Chapter

One. Any effort involving the collection of analytical data should include development of a structured and systematic planning document, such as a Quality Assurance Project Plan (QAPP) or a Sampling and Analysis Plan (SAP), which translates project objectives and specifications into directions for those that will implement the project and assess the results. Each laboratory should maintain a formal quality assurance program. The laboratory should also maintain records to document the quality of the data generated. All data sheets and quality control data should be maintained for reference or inspection.

9.2 In order to demonstrate the purity of reagents and sample contact surfaces, method blanks should be tested at the extremes of the acid and base additions, as well as when only reagent water (no acid or base addition) is used for extraction.

9.3 The analysis of extracts should follow appropriate QC procedures, as specified in the determinative methods for the COPCs. Refer to Chapter One for specific quality control procedures.

9.4 Unless the "as-received" samples are part of a time-dependent (e.g., aging) study, solid materials should be processed and tested within one month of their receipt.

9.5 Initial demonstration of proficiency (IDP)

Leachate methods are not amenable to typical initial demonstrations of proficiency as reference materials with known values are usually not available. However, prior to using this method an analyst should have documented proficiency in the skills required for successful implementation of the method. For example, skill should be demonstrated in the use of an analytical balance, the determination of pH using methods 9040 and 9045 and the determination of conductance using method 9050.

10.0 CALIBRATION AND STANDARDIZATION

10.1 The balance should be calibrated and certified at a minimum annually or in accordance with laboratory policy.

10.2 Prior to measurement of eluate pH, the pH meter should be calibrated using a minimum of two standards that bracket the range of pH measurements. Refer to Methods 9040 and 9045 for additional guidance.

10.3 Prior to measurement of eluate conductivity, the meter should be calibrated using at least one standard at a value greater than the range of conductivity measurements. Refer to Method 9050 for additional guidance.

11.0 PREPARATORY PROCEDURES

A flowchart for the method procedure is presented in Figure 1. Microsoft Excel data templates are available to aid in collection and archiving of laboratory and analytical data.[3]

[3] These Excel templates form the basis for uploading method data into the data management program, LeachXS Lite™. Both the data templates and LeachXS Lite are available at http://vanderbilt.edu/leaching.

11.1 Particle-size reduction (if required)

11.1.1 In this method, particle-size reduction is used for sample homogenization and to prepare large-grained samples for extraction so that the approach toward liquid-solid equilibrium is enhanced and mass transport through large particles is minimized. A longer extract contact time is required for larger maximum particle-size designations. This method designates three maximum particle sizes and associated contact times (see Table 1). The selection of an appropriate maximum particle size from this table should be based on professional judgment regarding the practical effort required to size-reduce the solid material.

11.1.2 Particle-size reduction of "as received" samples may be achieved through crushing, milling or grinding with equipment made from chemically-inert materials. During the reduction process, care should be taken to minimize the loss of sample and potentially volatile constituents in the sample.

NOTE: Crushing of oversize material is preferred to milling or grinding as the later techniques may result in heating of the sample material.

11.1.3 If the moisture content of the "as received" material is greater than 15% (wet basis), air drying or desiccation may be necessary. Oven drying is not recommended for the preparation of test samples due to the potential for mineral alteration and volatility loss. In all cases, the moisture content of the "as received" material should be recorded.

NOTE: If the solid material is susceptible to interaction with the atmosphere (e.g., carbonation, oxidation), drying should be conducted in an inert environment.

11.1.4 When the material appears to be of a relatively uniform particle size, calculate the percentage less than the sieve size as follows:

$$\%\ \text{Passing} = \frac{M_{sieved}}{M_{total}} \times 100\%$$

Where: M_{sieved} = mass of sample passing the sieve (g)
M_{total} = mass of total sample (g) (e.g., M_{sieved} + mass not passing sieve)

11.1.5 The fraction retained by the sieve should be recycled for further particle-size reduction until at least 85% of the initial mass has been reduced below the designated maximum particle size. Calculate and record the final percentage passing the sieve and the designated maximum particle size. For the uncrushable fraction of the "as received" material, record the fraction mass and nature (e.g., rock, metal or glass shards, etc).

11.1.6 Store the size-reduced material in an airtight container in order to prevent contamination via gas exchange with the atmosphere. Store the container in a cool, dark and dry place prior to use.

11.2 Determination of solids and moisture content

11.2.1 In order to provide the dry mass equivalent of the "as-tested" material, the solids content of the subject material should be determined. Often, the moisture content of the solid sample is recorded. In this method, the moisture content is determined and recorded on the basis of the "wet" or "as-tested" sample.

WARNING: The drying oven should be contained in a hood or otherwise properly ventilated. Significant laboratory contamination or inhalation hazards may result when drying heavily contaminated samples. Consult the laboratory safety officer for proper handling procedures prior to drying samples that may contain volatile, hazardous, flammable or explosive materials.

11.2.2 Place a 5–10-g sample of solid material into a pre-tared dish or crucible. Dry the sample to a constant mass at 105 ± 2 °C. Check for constant mass by returning the dish to the drying oven for twenty four hours, cooling to room temperature in a desiccator and re-weighing. The two mass readings should agree within the larger of 0.2% or 0.02 gram.

NOTE: The oven-dried sample is not used for the extraction and should be properly disposed once the dry mass is determined.

11.2.3 Calculate and report the solids content as follows:

$$SC = \frac{M_{dry}}{M_{test}}$$

Where: SC = solids content (g-dry/g)
M_{dry} = mass of oven-dried sample (g-dry)
M_{test} = mass of "as-tested" sample (g)

11.2.4 Calculate and report the moisture content (wet basis) as follows:

$$MC_{wet} = \frac{M_{test} - M_{dry}}{M_{test}}$$

Where: $MC_{(wet)}$ = moisture content on a wet basis (g_{H_2O}/g)
M_{dry} = mass of oven-dried sample (g-dry)
M_{test} = mass of "as-tested" sample (g)

11.3 Pre-test titration (if required)

In order to conduct the parallel batch test in Sec. 12.0, a schedule of acid and base additions should be formulated from either a pre-test titration or based on prior knowledge of the

acid/base titration curve of the sample. This section describes the procedure for obtaining a titration curve of the test material, when sufficient prior knowledge is unavailable.

If the schedule of acid and base additions will be generated from prior knowledge, proceed to Sec. 11.4. If the schedule of acid and base additions is already known, proceed to Sec. 12.0.

Figures 2-4 show example titration curves for a wide variety of solid materials. Table 2 indicates how these materials may be classified as (a) low alkalinity; (b) moderate alkalinity; or (c) high alkalinity in terms of the equivalents of acid required for obtaining final extraction pH values in the range of 2-13.

11.3.1 Predict the classification of the neutralization behavior of the solid material based on professional judgment, preliminary data, or the material examples shown in Table 2 and Figures 2-4.

11.3.2 Conduct a five-point parallel extraction test using 10-g-dry samples of the solid following the pre-test schedule shown in Table 3 for the chosen classification. Perform the extraction procedure in Sec. 12.0, omitting the filtration, method blanks, and analytical sample collection.

11.3.3 Plot the pre-test titration curve (e.g., the extract pH as a function of the equivalents of acid added) considering base equivalents as the negative sign of acid equivalents.

11.3.4 Reiterate the pre-test extraction, if necessary to expand or contract the pre-test titration until the 2-13 pH range can be resolved.

NOTE: Additional pre-test point(s) interpolating or extrapolating from the pre-test schedule may be necessary to provide adequate resolution in the titration curve.

11.3.5 Pre-test titration using provided Microsoft® Excel template

The “Pre-Test” worksheet in the accompanying Excel template may be used to calculate pre-test extraction formulations and plot the pre-test titration curve. Mandatory input data for the template includes:

a) particle size of the “as tested” material (see Sec. 11.1);
b) solids content of the “as tested” material (see Sec. 11.2); and
c) five acid/base additions based on the predicted response classification of the solid material (see Sec. 11.3).

Enter the eluate pH and plot the pre-test titration curve. Compare the resulting titration curve to the target pH values as designated in Table 4.

11.4 Formulation of acid and base additions schedule

A schedule of acid and base additions is used in the main extraction procedure (Sec. 12.0) to set up nine extractions of the test material plus three method blanks. Based on either prior knowledge of the acid/base titration curve of the sample or the results of the pre-test

titration procedure in Sec. 11.3, formulate a schedule of test extractions using the example in Table 4 and the following steps.

11.4.1 Using the extraction parameters in Table 1, identify the recommended minimum dry-mass equivalent associated with the particle size of the "as-tested" sample. Calculate and record the amount of "as tested" material equivalent to the dry-material mass from Table 1 as follows:

$$M_{test} = \frac{M_{dry}}{SC}$$

Where: M_{test} = mass of "as-tested" solid equivalent to the dry-material mass (g)
M_{dry} = mass of dry material specified in the method (g-dry)
SC = solids content of "as-tested" material (g-dry/g)

11.4.2 Label Column A of the schedule table with consecutive numbers for the nine test positions (shown in Table 4 as "TXX" labels) and three method blanks (shown in Table 4 as "BXX" labels).

11.4.3 Select the nine target pH points as shown in Table 5 and enter this data into Column B of the schedule table. One of the nine target pH values should be with no acid or base addition in order to record the natural pH of the material. The target pH points shown in Table 5 allow for substitution of one optional target point if the natural pH of the solid material falls within the tolerance of another designated target pH. For example, if the natural pH is 11.8 and would satisfy the target pH of 12.0 ± 0.5, the optional target point of 10.5 ± 0.5 should be included.

11.4.4 For each test position, determine the equivalents of acid or base required to meet the target pH from the pre-test titration curve (see Sec. 11.3). Enter this data into Column C of the schedule table. Interpolate intermediate acid additions on the pre-test titration curve using linear interpolation or other regression techniques.

NOTE: Linear interpolation will have some inherent error, which may result in an extract pH that falls outside of the target pH tolerance. Additional pre-test points interpolating or extrapolating from the pre-test schedule in Table 3 may be necessary to provide adequate resolution of the titration curve.

11.4.5 Enter the acid volumes in Column D and base volumes in Column E of the schedule after converting the equivalents of acid and base to volume as follows:

$$V_{a/b} = \frac{Eq_{a/b}}{N_{a/b}}$$

Where: $V_{a/b}$ = volume of acid or base to be entered in the schedule table (mL)
$Eq_{a/b}$ = equivalents of acid or base selected for the target pH as determined from the pre-test titration curve (meq/g)
$N_{a/b}$ = normality of the acid or base solution (meq/mL)

11.4.6 In Column F of the schedule table, calculate the volume of moisture contained in the "as tested" sample as follows:

$$V_{W,sample} = \frac{M_{test} \times (1 - SC)}{\rho_w}$$

Where: $V_{W,sample}$ = volume of water in the "as tested" sample (mL)
M_{test} = mass of the "as tested" sample (g)
SC = solids content of the "as tested" sample (g-dry/g)
ρ_w = density of water (1.0 g/mL at room temperature)

11.4.7 In Column G of the schedule table, calculate the volume of reagent water required to bring each extraction to a L/S of 10 mL/g-dry solid as follows:

$$V_{RW} = M_{dry} \times LS - V_{W,sample} - V_{a/b}$$

Where: V_{RW} = volume of reagent water required to complete L/S (mL)
M_{dry} = dry mass equivalent of solid sample (g)
LS = liquid-to-dry-solid ratio (10 mL/g)
$V_{W,sample}$ = volume of water in "as used" sample (mL)
$V_{a/b}$ = volume of acid or base for the extraction recipe (mL)

11.4.8 Method Blanks

In the schedule table, include three additional extractions for processing method blanks. Method blanks extractions are performed using the same equipment, reagents, and extraction process as the test positions, but without solid sample. The three method blanks should include:

a) reagent water (B01 in Table 4);
b) reagent water + maximum volume of acid in the schedule (B02 in Table 4); and
c) reagent water + maximum volume of base in the schedule (B03 in Table 4).

NOTE: If multiple materials or replicate tests are carried out in parallel, only one set of method blanks is necessary.

11.4.9 Schedule formulation using Excel template

The "Test Data" worksheet in the provided Excel template may be used to automatically calculate a schedule of acid and base additions, as well as to plot the response eluate pH and conductivity as a function of acid addition. Mandatory input data for the template includes:

a) particle size of the "as tested" material (see Sec. 11.1);
b) solid content of the "as tested" material (see Sec. 11.2); and
c) nine acid/base additions determined from the pre-test titration curve with respect to target pH values designated in Table 5.

Subsequent to the extraction procedure, eluate pH, conductivity, and oxidation/reduction potential (optional) for up to three replicates may be entered and plotted as a function of acid added.

12.0 EXTRACTION PROCEDURE

Use the schedule of acid and base additions (Sec. 11.4) as a guide to set up nine test extractions and three method blanks as follows:

12.1 Label nine bottles with test position numbers and three bottles with method blank labels according to the schedule of acid and base additions (see Column A in Table 4).

12.2 Use the extraction parameters in Table 1 to identify the recommended dry-mass equivalent associated with the particle size of the "as tested" sample. Calculate and record the amount of "as tested" material equivalent to the identified dry mass from Table 1 as follows:

$$M_{test} = \frac{M_{dry}}{SC}$$

Where: M_{test} = mass of "as tested" solid equivalent to g of dry material (g)
M_{dry} = mass of dry material specified in method (g)
SC = solids content of "as tested" material (g/g)

12.3 Place the dry equivalent mass (± 0.1 g) of the "as tested" sample, calculated above, into each of the nine test position extraction vessels.

NOTE: Do NOT put solid material in the method blank extraction vessels.

12.4 Add the appropriate volume of reagent water (± 5% of target value) to both the test position and method blank extraction vessels, as specified in the schedule for the L/S makeup (see Column G in Table 4).

12.5 Add the appropriate volume of acid or base (± 1% of target value) to each vessel, using a continuously adjustable pipettor, as designated in the schedule for acid/base addition (see Column D and Column E in Table 4).

12.6 Tighten the leak-proof lid on each bottle and tumble all extraction vessels (i.e., test positions and method blanks) in an end-over-end fashion at a speed of 28 ± 2 rpm at room temperature (20 ± 2 °C). The contact time for this method will vary depending on the sample particle size as shown in Table 1.

NOTE: The length of the contact time is designed to enhance the approach toward liquid-solid equilibrium. Longer contact times are required for larger particles to compensate for the effects of intra-particle diffusion. See Table 1 for recommended contact times based on particle size.

12.7 Remove the extraction vessels from the rotary tumbler and clarify the solutions by allowing the bottles to stand for 15 ± 5 min. Alternately, centrifuge the extraction vessels at 4000 ± 100 rpm for 10 ± 2 min.

12.8 For each extract vessel, decant a minimum volume (~ 5 mL) of clear, unpreserved supernatant into a clean container.

12.9 Measure and record the pH, specific conductivity, and oxidation-reduction potential (ORP) of the extracts (see Methods 9040, 9045, and 9050).

NOTE: Measurement of pH, conductivity and ORP should be taken within 15 minutes of eluate processing (Sec. 12.8) to avoid neutralization of the solution due to exposure to carbon dioxide, especially when alkaline materials are tested.

NOTE: The measurement of ORP is optional, but strongly recommended, especially when testing materials where oxidation is likely to change the LSP of COPCs.

12.10 Separate the solid from the remaining liquid in each extraction vessel by pressure or vacuum filtration through a clean 0.45-µm pore size membrane (Sec. 6.5). The filtration apparatus may be exchanged for a clean apparatus as often as necessary until all liquid has been filtered.

NOTE: If COPCs which might be lost under vacuum (e.g., mercury) are suspected, the samples should be pressure-filtered using an inert gas (e.g., nitrogen or argon).

12.11 Immediately, preserve and store the volume(s) of eluate required for chemical analysis. Preserve all analytical samples in a manner that is consistent with the determinative chemical analyses to be performed.

13.0 DATA ANALYSIS AND CALCULATIONS (EXCEL TEMPLATE)

13.1 Data reporting

13.1.1 Figure 5 shows an example of a data sheet that may be used to report the concentration results of this method. At a minimum, the basic test report should include:

a) Name of the laboratory
b) Laboratory technical contact information

c) Date at the start of the test
d) Name or code of the solid material
e) Particle size (85 wt% less than)
f) Type of acid and/or base used in test
g) Extraction contact time (h)
h) Ambient temperature during extraction (°C)
i) Eluate specific information (see Sec. 13.1.2 below)

13.1.2 The minimum set of data that should be reported for each eluate includes:

a) Eluate sample ID
b) Mass of "as tested" solid material used (g)
c) Moisture content of material used (g_{H_2O}/g)
d) Volume (mL) and normality (N) of acid and/or base used
e) Volume of water added (mL)
f) Target pH
g) Measured final eluate pH
h) Measured eluate conductivity (mS/cm)
I) Measured ORP (mV) (optional)
j) Concentrations of all COPCs
k) Analytical QC qualifiers as appropriate

13.2 Data interpretation (optional)

13.2.1 Acid/base neutralization curve

Plot the pH of each extract as a function of the equivalents of acid or base added per dry gram of material to generate an acid/base neutralization curve.

NOTE: For materials in which both acid and base were used, equivalents of base can be presented as the opposite sign of acid equivalents (i.e., 5 meq/g-dry of base would correspond to -5 meq/g-dry of acid).

The titration curve can be interpreted as showing the amount of acid or base that is needed to shift the pH of the subject material. This is helpful when evaluating field scenarios where the pH of leachates is not buffered by the acidity or alkalinity of the solid material.

13.2.2 LSP curve

An LSP curve can be generated for each COPC following chemical analyses of all extracts by plotting the target analyte concentration in the liquid phase as a function of the measured extract pH for each extract. As an example, Figure 6 illustrates the LSP curves for arsenic and selenium from a coal combustion fly ash and indicates the limits of quantitation and the natural concentration response.

13.2.2.1 The lower limit of quantitation (LLOQ) of the determinative method for each COPC may be shown as a horizontal line. COPC concentrations below this line indicate negligible or non-quantitative concentrations.

NOTE: This method is for the generation of extract solution and does not specify any particular analytical method. Since the lower limit of quantitation is highly dependent on both chosen analytical method and the solution matrix, it should be determined as part of an analytical QA/QC plan.

13.2.2.2 Natural response is defined as the eluate pH and COPC concentration measured when the solid material is extracted with reagent water at an L/S of 10 mL/g-dry. The natural response values can be shown on the LSP curve as a vertical line from the *x*-axis (at the replicate average natural pH) intersected with a horizontal line (at the replicate average COPC concentration). Alternatively, the natural response can be indicated in results using a different symbol from other results.

13.2.2.3 The values on the curve indicate the eluate concentration of the constituent of interest at an L/S of 10 mL/g-dry over a pH range. The shape of the LSP curve is indicative of the speciation of the COPC in the solid phase with four characteristic LSP curve shapes (i.e., relative locations of maxima and minima) presented schematically in Figure 7.

Cationic Species (e.g., Cd) — The LSP curve of cationic species typically has a maximum concentration in the acidic pH range that decreases to lower values at alkaline pH.

Amphoteric Species (e.g., Pb, Cr(III), Cu.) — The LSP curves tend to be similar in shape to cationic LSP curves with greater concentrations in the acidic pH range. However, the concentrations pass through a minimum in the near neutral to slightly acid pH range only to increase again for alkaline pH values. Typically, the increase at high pH is due to the solubility of hydroxide complexes (e.g., $[Pb(OH_3)]^-$).

Oxyanionic Species (e.g. $[AsO_4]^-$, $[SeO_4]^-$, $[MnO_4]^-$) — The LSP curves often show maxima in the neutral to slightly alkaline range.
Highly Soluble Species (e.g., Na^+, K^+, Cl^-) — The LSP curve is only a weak function of pH.

The idealized LSP curves in Figure 7 can be compared with the general shape of the test data to infer the speciation of the COPC in the solid matrix. Concentration results from this method may be simulated with geochemical speciation models to infer the mineral phases, adsorption reactions, and soluble complexes that control the release of the COPC (see Ref. 1).

14.0 METHOD PERFORMANCE

14.1 Performance data and related information are provided in SW-846 methods only as examples and guidance. The data do not represent required performance criteria for users of the methods. Instead, performance criteria should be developed on a project-specific basis, and the laboratory should establish in-house QC performance criteria for the application

of this method. These performance data are not intended to be and must not be used as absolute QC acceptance criteria for purposes of laboratory accreditation.

14.2 Interlaboratory validation of this method was conducted using a coal combustion fly ash (material code EaFA), a contaminated smelter site soil (material code CFS) and a solidified waste analog (material code SWA). The median values and inner quartile ranges (IQRs) for repeatability and reproducibility were determined for eluate concentration results across all study materials and pH target values (see Table 3). More details on the interlaboratory validation may be found in Ref. 7.

14.3 Refs. 2 and 3 may provide additional guidance and insight on the use, performance and application of this method.

15.0 POLLUTION PREVENTION

15.1 Pollution prevention encompasses any technique that reduces or eliminates the quantity and/or toxicity of waste at the point of generation. Numerous opportunities for pollution prevention exist in laboratory operations. The EPA has established a preferred hierarchy of environmental management techniques that places pollution prevention as the management option of first choice. Whenever feasible, laboratory personnel should use pollution prevention techniques to address their waste generation. When wastes cannot be feasibly reduced at the source, the Agency recommends recycling as the next best option.

15.2 For information about pollution prevention that may be applicable to laboratories and research institutions consult Less is Better: Laboratory Chemical Management for Waste Reduction available from the American Chemical Society's Department of Government Relations and Science Policy, 1155 16th St., N.W. Washington, D.C. 20036, http://portal.acs.org/portal/fileFetch/C/WPCP_012290/pdf/WPCP_012290.pdf.

16.0 WASTE MANAGEMENT

The Environmental Protection Agency requires that laboratory waste management practices be conducted consistent with all applicable rules and regulations. The Agency urges laboratories to protect the air, water, and land by minimizing and controlling all releases from hoods and bench operations, complying with the letter and spirit of any sewer discharge permits and regulations, and by complying with all solid and hazardous waste regulations, particularly the hazardous waste identification rules and land disposal restrictions. For further information on waste management, consult The Waste Management Manual for Laboratory Personnel available from the American Chemical Society at the address listed in Sec. 14.2.

17.0 REFERENCES

1. H. A. van der Sloot, P.F.A.B. Seignette, J.C.L. Meeussen, O. Hjelmar and D.S. Kosson, (2008), “A Database, Speciation Modeling and Decision Support Tool for Soil, Sludge, Sediments, Wastes and Construction Products: LeachXS™- ORCHESTRA,” in Venice 2008: Second International Symposium on Energy from Biomass and Waste, Venice, Italy, 17-20 November 2008 (also see www.leaching.com).

2. D.S. Kosson, H.A. van der Sloot, F. Sanchez and A.C. Garrabrants (2002) “An Integrated Framework for Evaluating Leaching in Waste Management and Utilization of Secondary Materials,” Environmental Engineering Science, 19(3) 159-204.

3. A.C. Garrabrants, D.S. Kosson, H.A. van der Sloot, F. Sanchez and O. Hjelmar (2010) “Background Information for the Leaching Environmental Assessment Framework (LEAF) Test Methods,” EPA/600/R-10-170, U.S. Environmental Protection Agency, Washington, DC, December 2010.

4. F. Sanchez, R. Keeney, D.S. Kosson and R. DeLapp (2006) “Characterization of Mercury-Enriched Coal Combustion Residues from Electric Utilities Using Enhanced Sorbents for Mercury Control,” EPA-600/R-06/008, U.S. Environmental Protection Agency, Washington DC, February 2006.

5. F. Sanchez, D.S. Kosson, R. Keeney, R. DeLapp, L. Turner and P. Kariher (2008) “Characterization of Coal Combustion Residues from Electric Utilities Using Wet Scrubbers for Multi-Pollutant Control,” EPA-600/R-08/077, U.S. Environmental Protection Agency, Washington DC, July 2008.

6. D.S. Kosson, F. Sanchez, P. Kariher, L.H. Turner, R. DeLapp and P. Seignette (2009) “Characterization of Coal Combustion Residues from Electric Utilities – Leaching and Characterization Data,” EPA-600/R-09/151, U.S. Environmental Protection Agency, Washington DC, December 2009.

7. A.C. Garrabrants, D.S. Kosson, L. Stefanski, R. DeLapp, P.F.A.B. Seignette, H.A. van der Sloot, P. Kariher, and M. Baldwin (2012) “Interlaboratory Validation of the Leaching Environmental Assessment (LEAF) Method 1313 and Method 1316,” DRAFT, U.S. Environmental Protection Agency, Washington DC, April 2012.

8. CEN/TS 14429 (2005) Characterization of Waste – Leaching Behaviour Tests – Influence of pH on Leaching with Initial Acid/base Addition, Comité Européen de Normalisation, Brussels, Belgium.

9. CEN/TS 14429 (2005) Characterization of Waste – Leaching Behaviour Tests – Influence of pH on Leaching with Continuous pH Control, Comité Européen de Normalisation, Brussels, Belgium.

18.0 TABLES, DIAGRAMS, FLOW CHARTS, AND VALIDATION DATA

The following pages contain the tables and figures referenced by this method.

TABLE 1

EXTRACTION PARAMETERS AS FUNCTION OF MAXIMUM PARTICLE SIZE

Particle Size (85 wt% less than) (mm)	US Sieve Size	Minimum Dry Mass (g-dry)	Contact Time (h)	Suggested Vessel Size (mL)
0.3	50	20 ± 0.02	24 ± 2	250
2.0	10	40 ± 0.02	48 ± 2	500
5.0	4	80 ± 0.02	72 ± 2	1000

TABLE 2

MATERIAL NEUTRALIZATION CLASSIFICATIONS

Neutralization Classification	Material Types
Low Alkalinity	soils; sediments; CCR fly ash; CCR bottom ash; coal milling rejects; MSWI fly ash, MSWI bottom ash; sewage sludge amended soil
Moderate Alkalinity	soils; wood preserving waste; MSWI bottom ash; steel slag; electric arc furnace dust; MSW compost; nickel sludge; Portland cement mortar
High Alkalinity	Portland cement clinker; steel blast furnace slag, solidified waste (fly ash, blast furnace slag, Portland cement)

NOTE: CCR = Coal combustion residue
MSWI = Municipal solid waste incinerator

TABLE 3

PRE-TEST TITRATION: ACID EQUIVALENT SCHEDULE

Neutralization Classification	Equivalents of Acid (meq/g-dry)				
	Bottle 1	Bottle 2	Bottle 3	Bottle 4	Bottle 5
Low Alkalinity	-2.0	-1.0	0	1.0	2.0
Moderate Alkalinity	-2.0	0	2.0	5.0	10.0
High Alkalinity	0	5.0	10.0	15.0	25.0

NOTE: 1) Base additions shown as opposite sign of acid equivalents.
2) Additional pre-test point(s) interpolating or extrapolating from the pre-test schedule may be necessary to provide adequate resolution in the titration curve.

TABLE 4

EXAMPLE SCHEDULE OF ACID AND BASE ADDITIONS

A	B	C	D	E	F	G
Test position	Target extract pH	Equivalents of Acid (meq/g-dry)	Volume of 2N HNO_3 (mL)	Volume of 1N KOH (mL)	Volume of moisture in sample (mL)	Volume of reagent water (mL)
T01	13.0	-1.10	-	22.0	2.22	176
T02	12.0	-0.75	-	15.0	2.22	183
T03	10.5	-0.38	-	7.60	2.22	190
T04	9.0	-0.15	-	3.0	2.22	195
T05	8.0	-0.05	-	1.0	2.22	197
T06	Natural	0	-	-	2.22	198
T07	5.5	0.12	1.20	-	2.22	197
T08	4.0	0.90	9.00	-	2.22	189
T09	2.0	3.10	31.0	-	2.22	167
B01	QA/QC	0	-	-	-	200
B02	QA/QC	3.10	31.0	-	-	169
B03	QA/QC	-1.10	-	22.0	-	178

NOTE: 1) This schedule is based on “as tested” sample mass of 22.2±0.1 g (i.e., equivalent “as tested” mass for a 20.0 g-dry sample at a solids content of 0.90 g-dry/g).
2) In this example, the natural pH is assumed to be 7.0±0.5.
3) Test positions marked B01, B02, and B03 are method blanks of reagent water, reagent water + maximum acid addition, and reagent water + maximum base addition, respectively.

Data modified from Ref. 2.

TABLE 5

FINAL EXTRACT PH TARGETS

pH Target	Rationale
?	Natural pH at L/S 10 mL/g-dry (no acid/base addition)
2.0±0.5	Provides estimates of total or available COPC content
4.0±0.5	Lower pH limit of typical management scenario
5.5±0.5	Typical lower range of industrial waste landfills
7.0±0.5	Neutral pH region; high release of oxyanions
8.0±0.5	Endpoint pH of carbonated alkaline materials
9.0±0.5	Minimum of LSP curve for many cationic and amphoteric COPCs
12.0±0.5	Maximum in alkaline range for LSP curves of amphoteric COPCs
13.0±0.5	Upper bound (field conditions) for amphoteric COPCs
10.5±0.5	Substitution if natural pH falls within range of a mandatory target

TABLE 6

MEDIAN METHOD PRECISION ACROSS STUDY MATERIALS

		Repeatability		Reproducibility	
Analyte	Symbol	Median $\%RSD_r$	IQR $\%RSD_r$	Median $\%RSD_R$	IQR $\%\ RSD_R$
Antimony	Sb	16%	12-25%	33%	24-45%
Arsenic	As	19%	13-24%	47%	37-61%
Barium	Ba	10%	7-15%	22%	18-36%
Boron	B	7%	5-9%	12%	8-21%
Calcium	Ca	5%	4-11%	9%	6-28%
Molybdenum	Mo	15%	6-23%	30%	18-46%
Selenium	Se	9%	6-13%	21%	18-31%
Vanadium	V	10%	6-12%	27%	23-41%
Median of Medians		10%	4-25%	26%	6-61%

Data taken from Ref. 7.

FIGURE 1

METHOD FLOWCHART

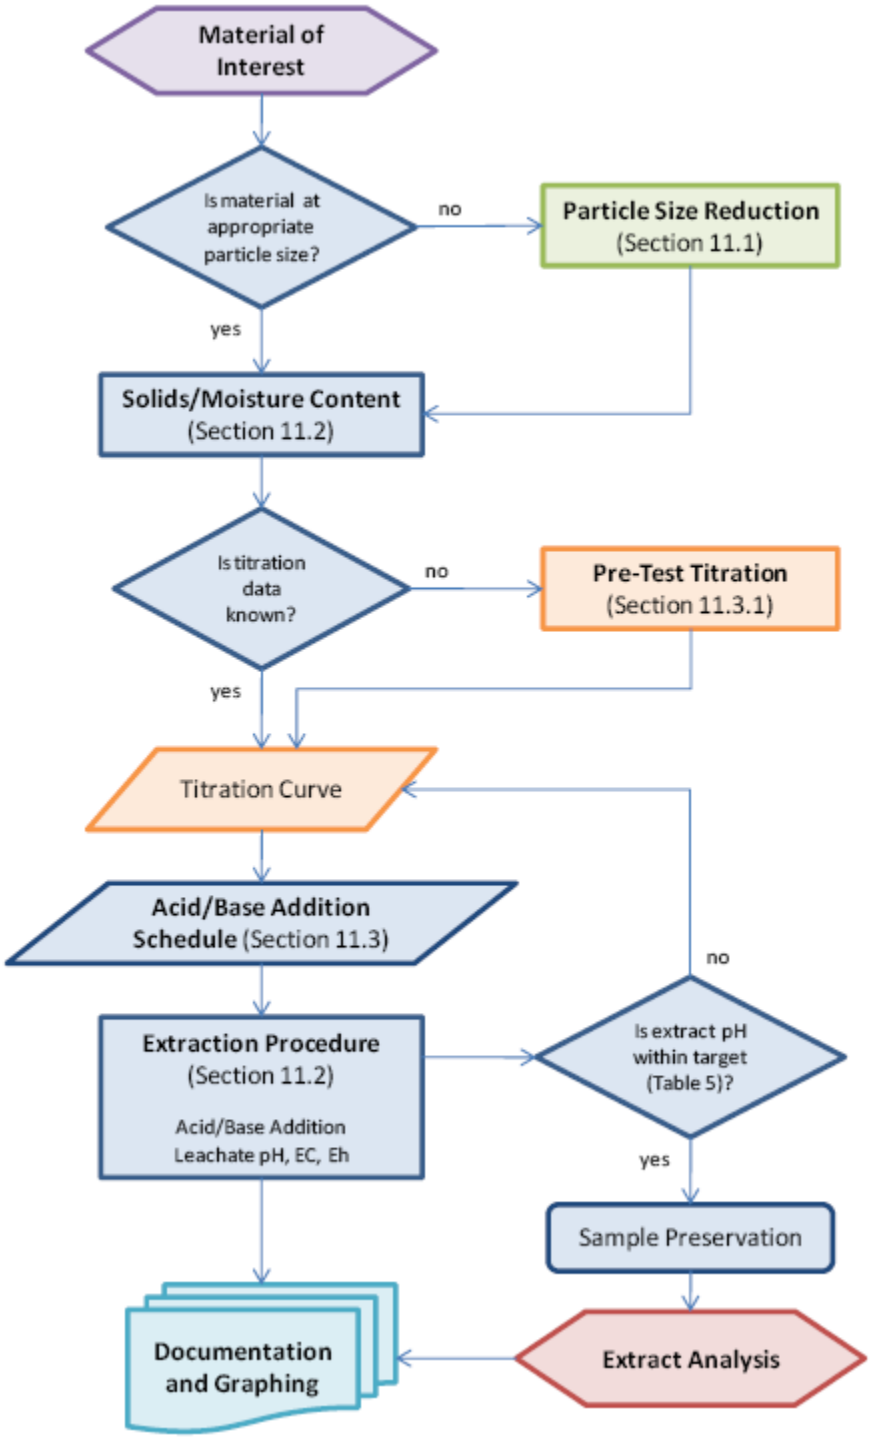

FIGURE 2

EXAMPLE TITRATION CURVES FOR SELECTED “LOW ALKALINITY” WASTES

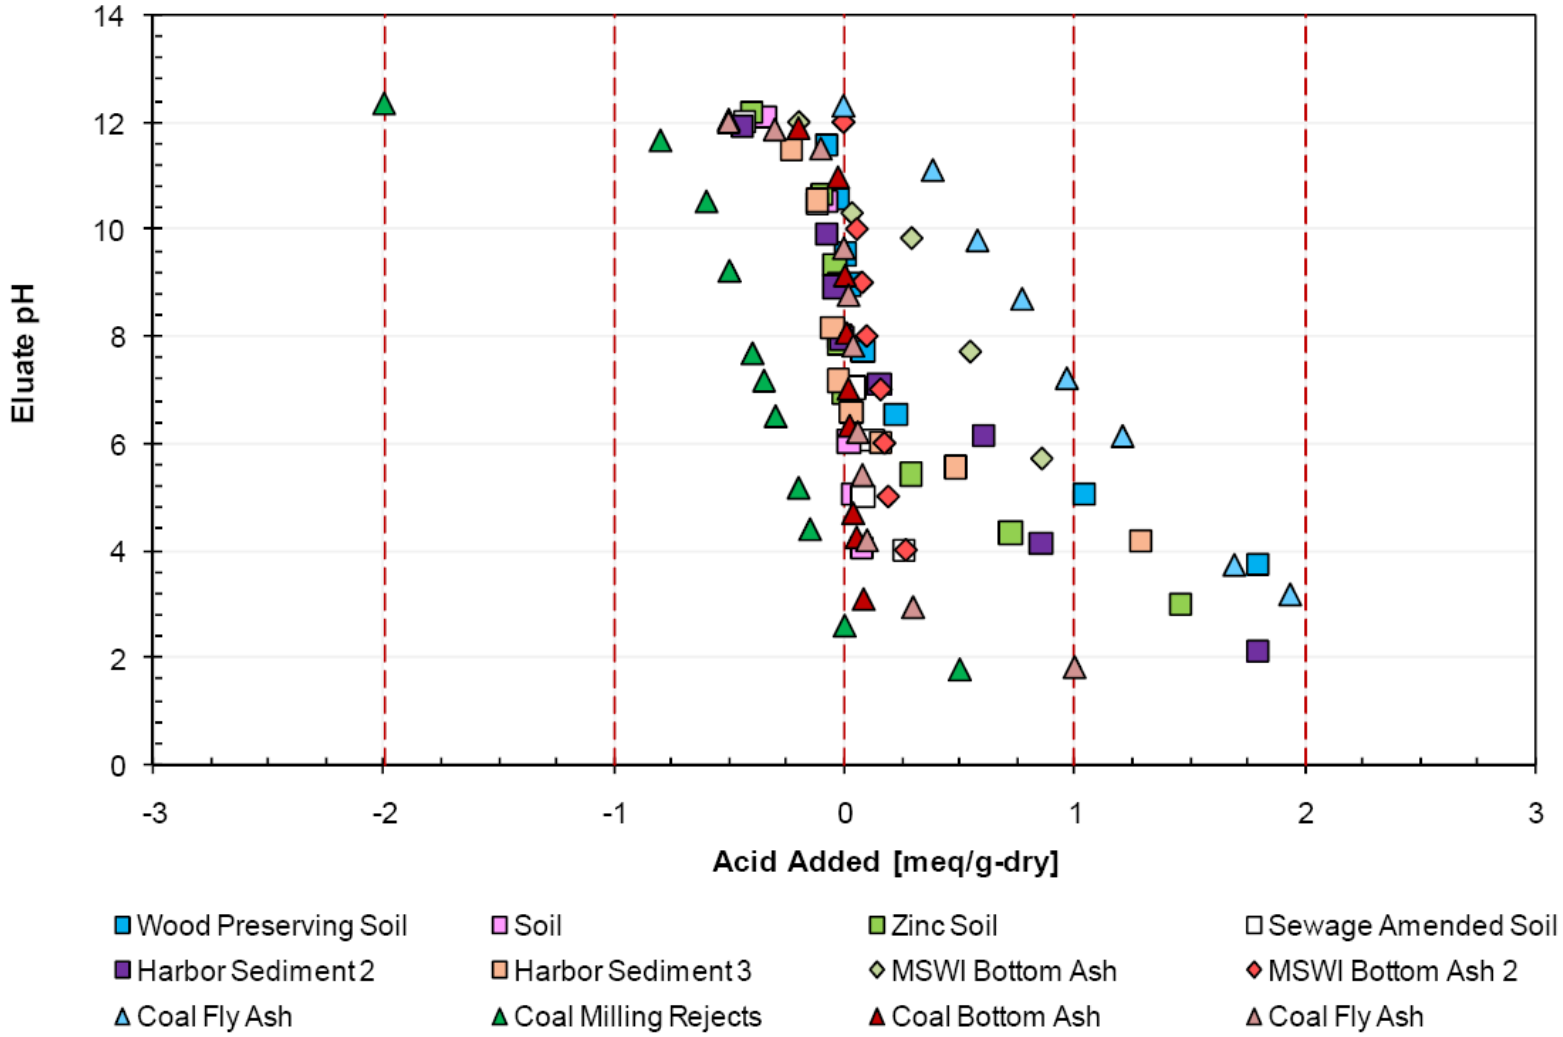

Some data taken LeachXS database (Ref. 1).

FIGURE 3

EXAMPLE TITRATION CURVES FOR SELECTED “MODERATE ALKALINITY” WASTES

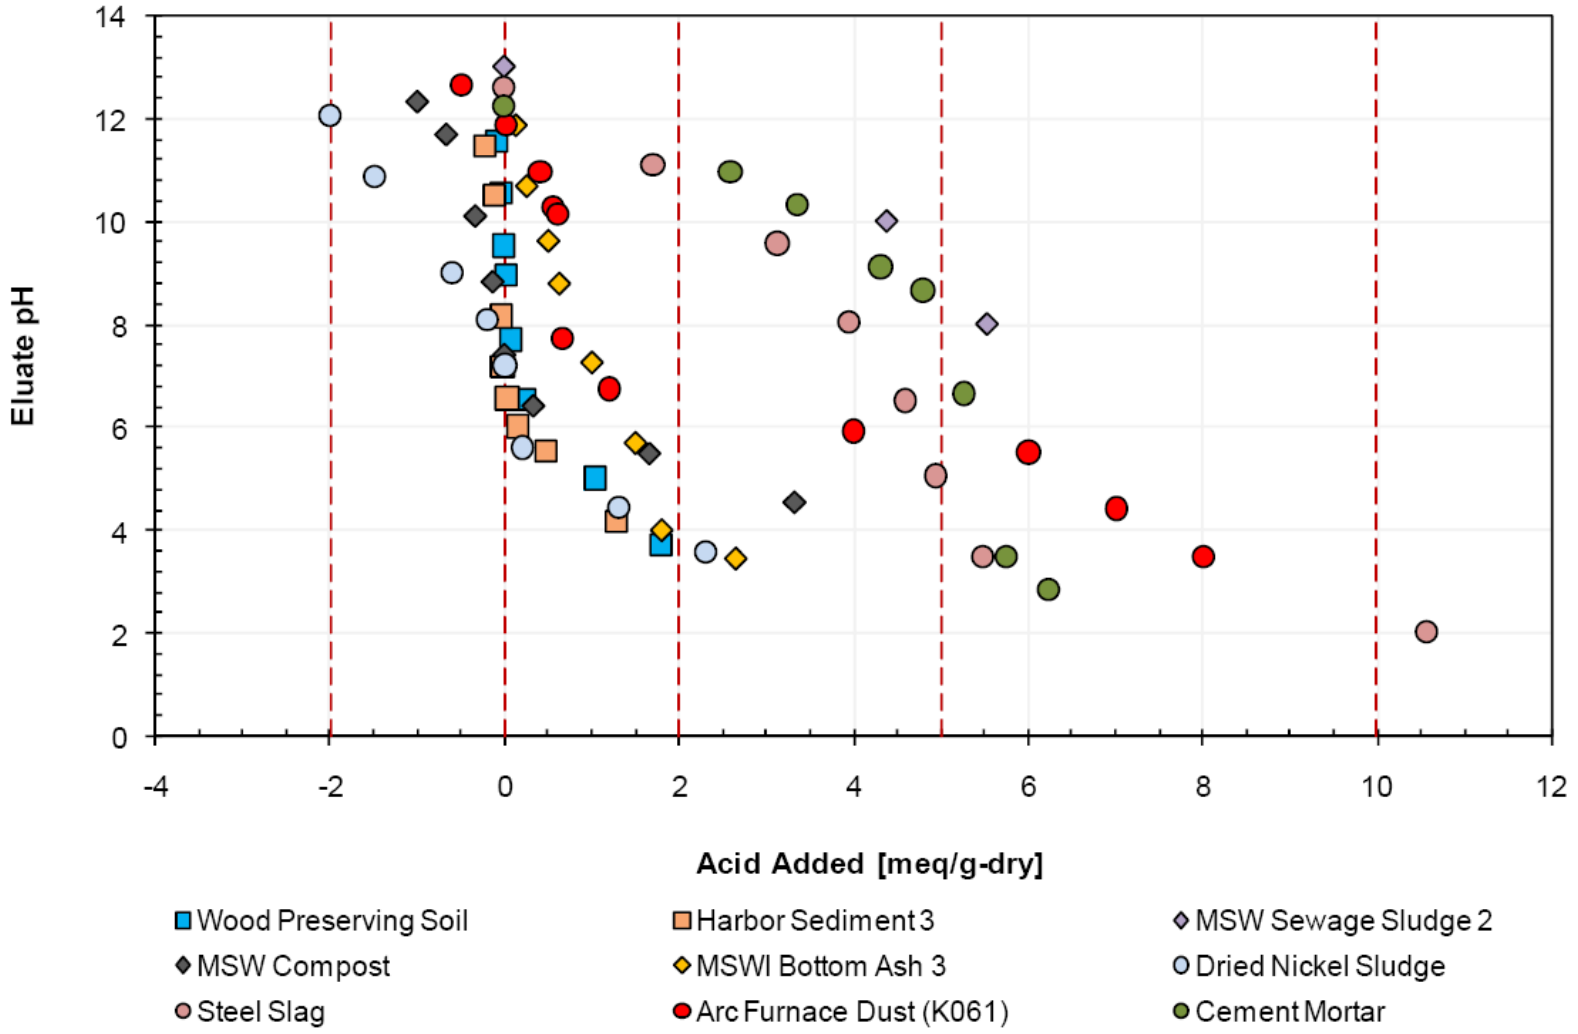

Some data taken from LeachXS database (Ref. 1).

FIGURE 4

EXAMPLE TITRATION CURVES FOR SELECTED “HIGH ALKALINITY” WASTES

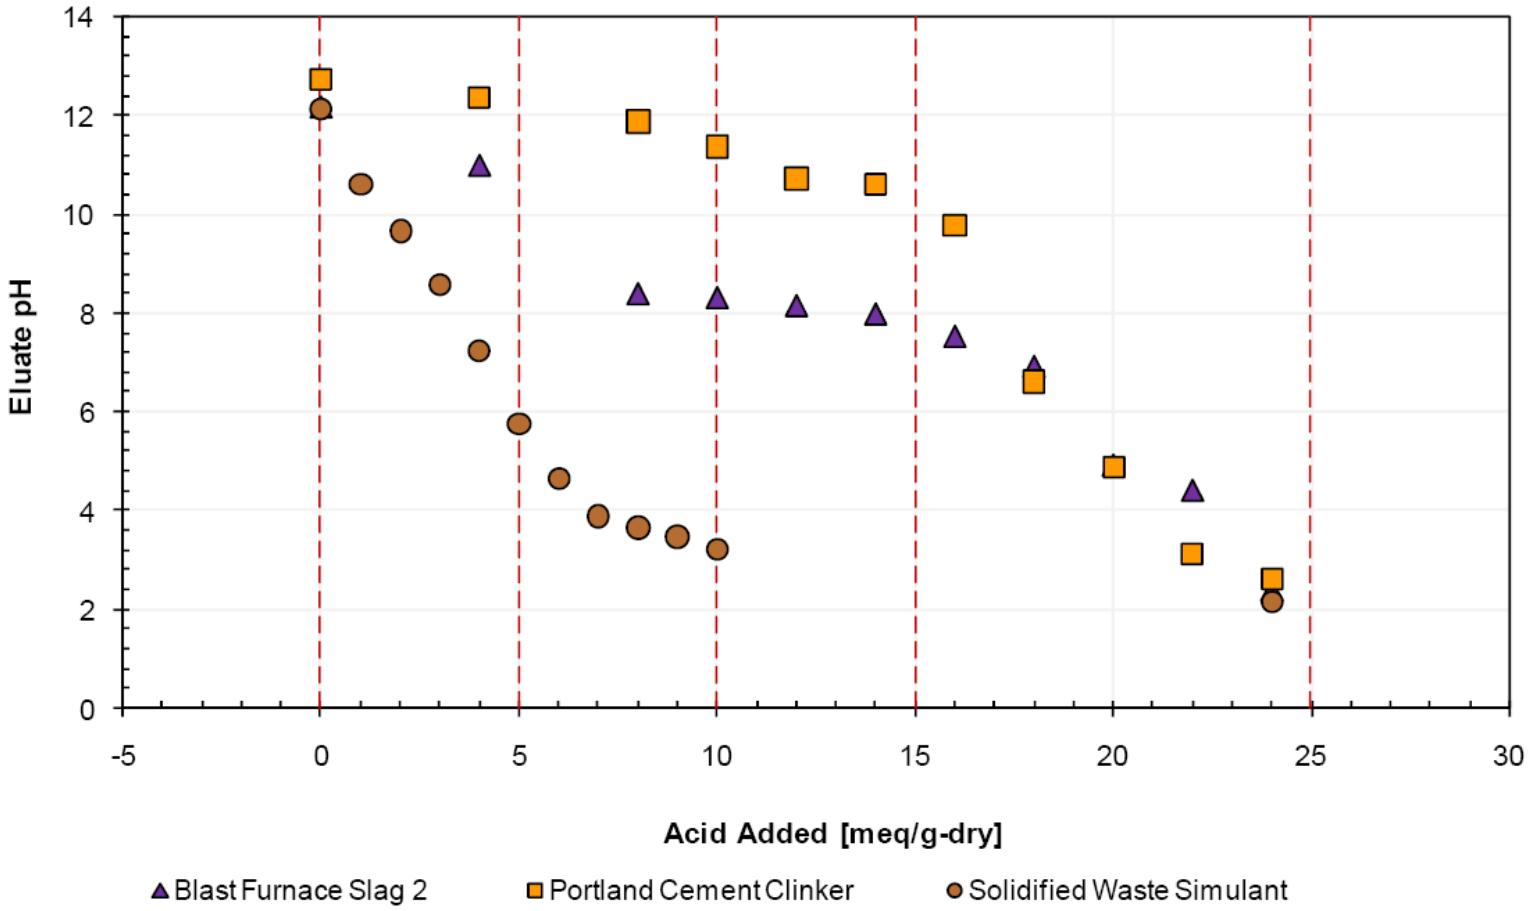

Some data taken from LeachXS database (Ref. 1).

FIGURE 5

EXAMPLE DATA REPORT FORMAT

EPA METHOD 1313
Report of Analysis

ABC Laboratories
123 Main Street
Anytown, USA
Contact: John Smith
(555) 111-1111

Client Contact: Susan Jones
(555) 222-2222

Material Code:	**XYZ**	Particle Size:	88% passing 2-mm sieve
Material Type:	Coal Combustion Fly Ash	Contact Time:	48 hours
Date Received:	10/1/20xx	Lab Temperature:	21 ± 2 °C
Test Date:	11/1/20xx	Acid Used:	Nitric acid
Report Date:	12/1/20xx	Base Used:	Sodium hydroxide

Test Position	Replicate	Value	Units	Method	Note
T01	**A**				
	Eluate Sample ID	**XYZ-1313-T01-A**			
	Solid Material	40.0	g		
	Moisture Content	0.01	g		
	Water Added	386.0	g_{H_2O}/g		
	Acid Added	14.0	mL		
	Acid Strength	2.0	mL		
	Base Added	-	N		
	Base Strength	1.0	mL		
	Target pH	2.0 ± 0.5	-		
	Eluate pH	1.89	-	EPA 9040	
	Eluate Conductivity	12.6	mS/c	EPA 9050	
	Eluate ORP	203	mv		

Chemical Analysis	Value	Units	QC Flag	Method	Date	Dilution Factor
Al	216.0	mg/L		EPA 6020	11/7/20xx	1000
As	0.64	mg/L		EPA 6020	11/7/20xx	10
Cl	< 4.13	mg/L	U	EPA 9056	11/9/20xx	1

Test Position	Replicate	Value	Units	Method	Note
T02	**A**				
	Eluate Sample ID	**XYZ-1313-T02-A**			
	Solid Material	40.0	g		
	Moisture Content	0.01	g		
	Water Added	400.0	g_{H_2O}/g		
	Acid Added	14.0	mL		
	Acid Strength	2.0	mL		
	Base Added	-	N		
	Base Strength	1.0	mL		
	Target pH	4.0 ± 0.5	-		
	Eluate pH	3.86	-	EPA 9040	Natural pH
	Eluate Conductivity	0.99	mS/c	EPA 9050	
	Eluate ORP	180	mv		

Chemical Analysis	Value	Units	QC Flag	Method	Date	Dilution Factor
Al	449.0	mg/L		EPA 6020	11/7/20xx	1000
As	0.979	mg/L		EPA 6020	11/7/20xx	10
Cl	< 4.13	mg/L	U	EPA 9056	11/7/20xx	1

QC Flag Key: U Value below lower limit of quantitation as reported (< "LLOQ")

FIGURE 6

EXAMPLE LSP CURVES FROM A COAL COMBUSTION FLY ASH SHOWING ASSESSMENT ZONES FOR A LANDFILL SCENARIO

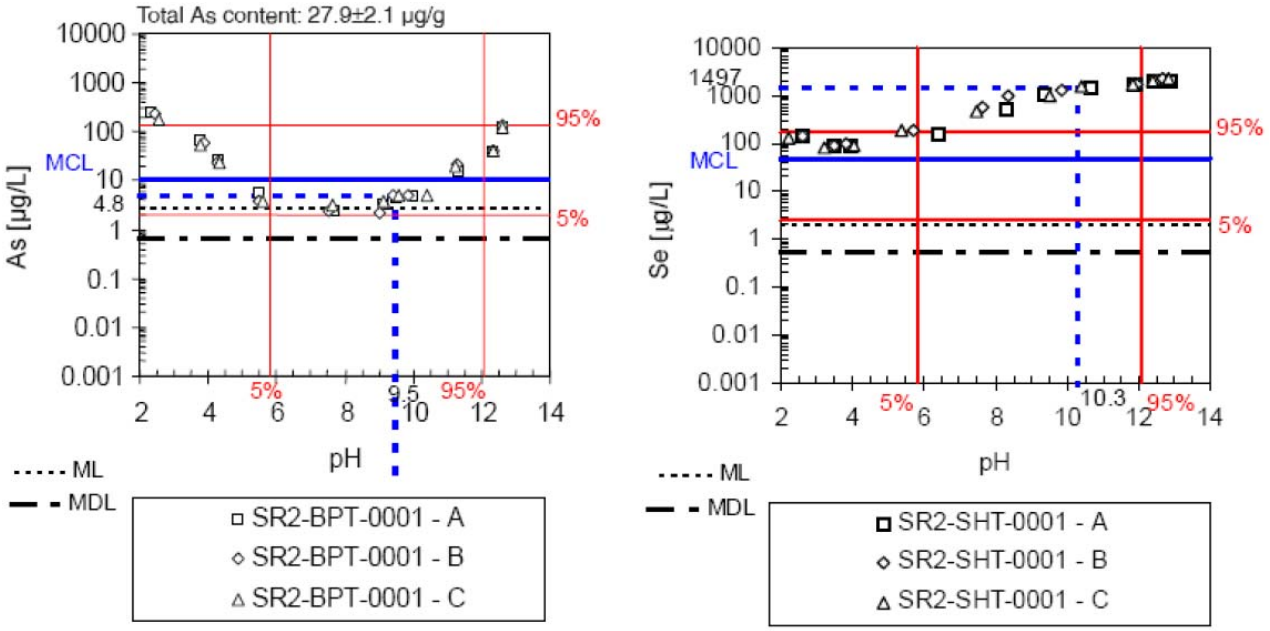

Figure taken from Ref. 4.

FIGURE 7

SCHEMATIC LSP CURVES OF CATIONIC, AMPHOTERIC, AND OXYANIONIC SPECIES

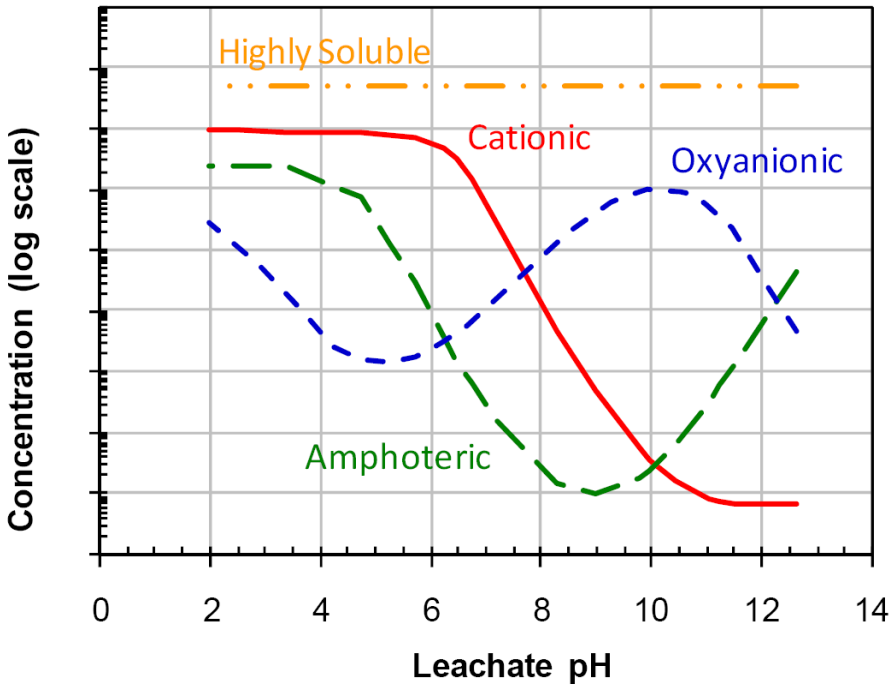

Figure taken from Ref. 2.

Appendix B. Method 1313

DRAFT METHOD 1316[1]

LIQUID-SOLID PARTITIONING AS A FUNCTION OF LIQUID-TO-SOLID RATIO IN SOLID MATERIALS USING A PARALLEL BATCH PROCEDURE

SW-846 is not intended to be an analytical training manual. Therefore, method procedures are written based on the assumption that they will be performed by analysts who are formally trained in at least the basic principles of chemical analysis and in the use of the subject technology.

In addition, SW-846 methods, with the exception of required method use for the analysis of method-defined parameters, are intended to be guidance methods which contain general information on how to perform an analytical procedure or technique which a laboratory can use as a basic starting point for generating its own detailed Standard Operating Procedure (SOP), either for its own general use or for a specific project application. The performance data included in this method are for guidance purposes only, and are not intended to be and must not be used as absolute QC acceptance criteria for purposes of laboratory quality control or accreditation.

1.0 SCOPE AND APPLICATION

1.1 This method is designed to provide the liquid-solid partitioning (LSP) of inorganic constituents (e.g., metals, radionuclides) and non-volatile organic constituents (e.g., polycyclic aromatic hydrocarbons (PAHs), dissolved organic carbon) at the natural pH of the solid material as a function of liquid-to-solid ratio (L/S) under conditions that approach liquid-solid chemical equilibrium. Table 1 shows the range of target L/S values tested under this method.

1.2 The eluate concentrations at a low L/S provide insight into pore solution composition either in a granular bed (e.g., soil column) or in the pore space of low-permeability material (e.g., solidified monolithic or compacted granular fill). In addition, analysis of eluates for dissolved organic carbon and of the solid phase for total organic carbon allow for evaluation of the impact of organic carbon release and the influence of dissolved organic carbon on the LSP of inorganic constituents.

1.3 This method is intended to be used as part of environmental leaching assessment for the evaluation of disposal, beneficial use, treatment effectiveness and site remediation. The method is not required by federal regulations to determine whether waste passes or fails the toxicity characteristic as defined at 40 CFR 261.24.

1.4 This method is suitable to a wide range of solid materials. Example solid materials include industrial wastes, soils, sludges, combustion residues, sediments, stabilized materials, construction materials, and mining wastes.

[1] This method has been derived from the SR003 procedure (Ref. 1) using EPA reviewed and accepted methodologies (see Refs. 3-5). The method is analogous to batch L/S-dependence method EN12457 (Ref. 7) developed for the Comité Européen de Normalisation (CEN).

1.5 This method is a leaching characterization method used to provide intrinsic material parameters that control leaching of inorganic species under equilibrium conditions. This test method is intended as a means for obtaining an extract (i.e., the eluate) of a solid material which may be used to estimate the solubility and release of inorganic constituents under the laboratory conditions described in this method. Extract concentrations may be used in conjunction with information regarding environmental management scenarios to estimate anticipated leaching concentrations, and release rate and extent for individual material constituents in the management scenarios evaluated. Extract concentrations may also be used along with geochemical speciation modeling to infer the mineral phases that control the LSP in the pore structure of the solid material.

1.6 This method is not applicable to characterize the release of volatile organic analytes.

1.7 This method provides solutions that are considered to be indicative of leachate under field conditions only where the field leaching pH and L/S ranges are encompassed by the laboratory extract final conditions and the LSP is controlled by aqueous-phase saturation of the constituent of interest. When LSP is controlled by the amount of the constituent present in the solid that may dissolve (i.e., for highly soluble species), the mass released (mg/kg), rather than the concentration, is indicative of field conditions.

1.8 The solvent used in this method is reagent water

1.9 Analysts are advised to take reasonable measures to ensure that the sample is homogenized to the extent practical prior to employment of this method. Particle-size reduction may provide additional assurance of sample homogenization. Table 2 designates a minimum dry equivalent mass of sample to be added to each extraction vessel and the associated extraction contact time as a function maximum particle diameter. If the heterogeneity of the sample is suspected as the cause of unacceptable levels of precision in replicate test results or is considered significant based on professional judgment, the sample mass used in the test procedure may be increased to a greater minimum dry equivalent mass than shown in Table 1 with the amount of extractant increased proportionately to maintain the designated L/S.

1.10 In the preparation of solid materials for use in this method, particle-size reduction of samples with large grain size is used to enhance the approach towards liquid-solid equilibrium under the designated contact time interval of the extract process. The extract contact time for samples reduced to a finer maximum particle size will be shorter.

1.11 Prior to employing this method, analysts are advised to consult the base method for each type of procedure that may be employed in the overall analysis (e.g., Methods 9040, 9045), quality control (QC) acceptance criteria, calculations, and general guidance. Analysts also should consult the disclaimer statement at the front of the manual and the information in Chapter Two for guidance on the intended flexibility in the choice of methods, apparatus, materials, reagents, and supplies, and on the responsibilities of the analyst for demonstrating that the techniques employed are appropriate for the analytes of interest, in the matrix of interest, and at the levels of concern.

In addition, analysts and data users are advised that, except where explicitly specified in a regulation, the use of SW-846 methods is not mandatory in response to Federal testing requirements. The information contained in this method is provided by EPA as guidance to be

used by the analyst and the regulated community in making judgments necessary to generate results that meet the data quality objectives for the intended application.

1.12 Use of this method is restricted to use by, or under supervision of, properly experienced and trained personnel. Each analyst must demonstrate the ability to generate acceptable results with this method as described in Section 9.5.

2.0 SUMMARY OF METHOD

This method consists of five parallel extractions of a particle-size reduced solid material in reagent water over a range of L/S values from 0.5 to 10 mL eluent/g dry material (see Table 1). In addition to the five test extractions, a method blank without solid sample is carried through the procedure in order to verify that analyte interferences are not introduced as a consequence of reagent impurities or equipment contamination (If multiple materials or replicate tests are carried out in parallel, only one set of method blanks is necessary). In total, six bottles (i.e., five test positions and one method blank) are tumbled in an end-over-end fashion for a specified contact time based on the maximum particle size of the solid (see Table 2). At the end of the contact interval, the liquid and solid phases are roughly separated via settling or centrifugation. Extract pH and specific conductance measurements are then taken on an aliquot of the liquid phase. The bulk of the eluate is clarified by pressure or vacuum filtration in preparation for constituent analysis. Analytical aliquots of the extracts are collected and preserved accordingly based on the determinative methods to be performed. The eluate constituent concentrations are plotted as a function of L/S and compared to QC and assessment limits.

3.0 DEFINITIONS

3.1 Release — The dissolution or partitioning of a constituent of potential concern (COPC) from the solid phase to the aqueous phase during laboratory testing (or under field conditions). In this method, mass release is expressed in units of mg COPC/kg dry solid material.

3.2 Constituent of potential concern (COPC) — A chemical species of interest, which may or may not be regulated, but may be characteristic of release-controlling properties of the sample geochemistry.

3.3 Liquid-solid partitioning (LSP) — The distribution of COPCs between the solid and liquid phases at the conclusion of the extraction.

3.4 Liquid-to-solid ratio (L/S) — the fraction of the total liquid volume (including the moisture contained in the “as used” solid sample) to the dry mass equivalent of the solid material. L/S is typically expressed in volume units of liquid per dry mass of solid material (mL/g-dry).

3.5 “As-tested” sample — The solid sample at the conditions (e.g., moisture content and particle-size distribution) present at the time of the start of the test procedure. The “as-tested” conditions will differ from the "as-received" sample conditions if particle-size reduction and drying were necessarily performed.

3.6 Dry-mass equivalent — The mass of “as-tested” (i.e., “wet”) sample that equates to the mass of dry solids plus associated moisture, based on the moisture content of the “as-tested” material. The dry-mass equivalent is typically expressed in mass units of the “as-tested” sample (g).

3.7 Refer to Chapter One and equipment manufacturers’ instructions for definitions that may be relevant to this procedure.

4.0 INTERFERENCES

4.1 Solvents, reagents, glassware, and other sample processing hardware may yield artifacts and/or interferences to sample analysis. All of these materials must be demonstrated to be free from interferences under the conditions of the analysis by analyzing method blanks. Specific selection of reagents and purification of solvents by distillation in all-glass systems may be necessary. Refer to each method to be used for specific guidance on quality control procedures and to Chapters Three and Four for general guidance on the cleaning of laboratory apparatus prior to use.

5.0 SAFETY

5.1 This method does not address all safety issues associated with its use. The laboratory is responsible for maintaining a safe work environment and a current awareness file of OSHA regulations regarding the safe handling of the chemicals listed in this method. A reference file of material safety data sheets (MSDSs) should be available to all personnel involved in these analyses.

6.0 EQUIPMENT AND SUPPLIES

The mention of trade names or commercial products in this manual is for illustrative purposes only, and does not constitute an EPA endorsement or exclusive recommendation for use. The products and instrument settings cited in SW-846 methods represent those products and setting used during the method development or subsequently evaluated by the Agency. Glassware, reagents, supplies, equipment, and setting other than those listed in this manual may be employed provided that method performance appropriate for the intended application has been demonstrated and documented.

This section does not list common laboratory glassware (e.g., beakers and flasks).

6.1 Extraction vessels

6.1.1 Six wide-mouth bottles (i.e., five for test positions plus one for a method blank) constructed of an inert material resistant to high and low pH conditions or interaction with the constituents of interest.

6.1.1.1 For the evaluation of inorganic COPCs, bottles composed of high density polyethylene (HDPE) (e.g., Nalgene #3140-0250 or equivalent), polypropylene (PP), or polyvinyl chloride (PVC) are recommended.

6.1.1.2 For the evaluation of non-volatile organic and mixed organic/inorganic COPCs, equipment composed of glass or Type 316 stainless steel is recommended. PTFE is not recommended for non-volatile organics, due sorption of species with high hydrophobicity (e.g., PAHs). Borosilicate glass is recommended over other types of glass, especially when inorganic analytes are of concern.

6.1.2. The extraction vessels must be of sufficient volume to accommodate both the solid sample and an extractant volume based on the schedule of L/S values shown in Table 1. For example, a 500-mL bottle is recommended when 100 g dry equivalent mass is contacted with 200 mL of eluent (see T03 in Table 1).

6.1.3 The vessels must have a leak-proof seals that can sustain end-over-end tumbling for the duration of the designated contact time.

6.1.4 If centrifugation is anticipated to be beneficial for initial phase separation, the extraction vessels should be capable of withstanding centrifugation at 4000 ± 100 rpm for a minimum of 10 ± 2 min. Alternately, samples may be extracted in bottles that do not meet this centrifugation specification (e.g., Nalgene I-Chem #311-0250 or equivalent) and the solid-liquid slurries transferred into appropriate centrifugation vessels for phase separation as needed.

6.2 Balance — Capable of 0.01-g resolution for masses less than 500 g.

6.3 Rotary tumbler — Capable of rotating the extraction vessels in an end-over-end fashion at a constant speed of 28 ± 2 rpm (e.g., Environmental Express, Charlestown, SC or equivalent).

NOTE: The holding capacity of tumblers may vary and modifications (e.g., packing or bottle-holding inserts) may be necessary to accommodate the extraction vessels.

6.4 Filtration apparatus — Pressure or vacuum filtration apparatus composed of appropriate materials so as to maximize the collection of extracts and minimize loss of the COPCs (e.g., Nalgene #300-4000 or equivalent) (see Sec. 6.1).

6.5 Filtration membranes — Composed of polypropylene or equivalent material with an effective pore size of 0.45-µm (e.g., Gelman Sciences GH Polypro #66548 from Fisher Scientific or equivalent).

6.6 pH Meter — Laboratory model with the capability for temperature compensation (e.g., Accumet 20, Fisher Scientific or equivalent) and a minimum resolution of 0.1 pH units.

6.7 pH combination electrode — Composed of chemically-resistant materials.

6.8 Conductivity meter — Laboratory model (e.g., Accumet 20, Fisher Scientific or equivalent), with a minimum resolution of 5% of the measured value.

6.9 Conductivity electrodes — Composed of chemically-resistant materials.

6.10 Adjustable-volume pipettor — Oxford Benchmate series or equivalent The necessary delivery range will depend on the buffering capacity of the solid material and acid/base strength used in the test.

6.11 Disposable pipettor tips.

6.12 Centrifuge (recommended) — Capable of centrifuging the extraction vessels at a rate of 4000 ± 100 rpm for 10 ± 2 min.

7.0 REAGENTS AND STANDARDS

7.1 Reagent-grade chemicals must be used in all tests. Unless otherwise indicated, it is intended that all reagents conform to the specifications of the Committee on Analytical Reagents of the American Chemical Society, where such specification are available. Other grades may be used, provided it is first ascertained that the reagents are of sufficiently high purity to permit use without lessening the accuracy of the determination. Inorganic reagents and extracts should be stored in plastic to prevent interaction of constituents from glass containers.

7.2 Reagent water must be interference free. All references to water in this method refer to reagent water unless otherwise specified.

7.3 Consult Methods 9040 and 9050 for additional information regarding the preparation of reagents required for pH and specific conductance measurements.

8.0 SAMPLE COLLECTION, PRESERVATION, AND STORAGE

8.1 See the introductory material to Chapter Three “Inorganic Analytes” and Chapter Four “Organic Analytes.”

8.2 All solid samples should be collected using an appropriate sampling plan.

8.3 All containers should be composed of materials that minimize interaction with solution COPCs. For further information, see Chapters Three and Four.

8.4 Preservatives should not be added to samples before extraction.

8.5 Samples can be refrigerated, unless refrigeration results in an irreversible physical change to the sample.

8.6 Analytical extracts or leachates should be preserved according to the guidance given in the individual determinative methods for the COPCs.

8.7 Extract holding times should be consistent with the holding times specified in the individual determinative methods for the COPCs.

9.0 QUALITY CONTROL

9.1 Refer to Chapter One for guidance on quality assurance (QA) and quality control (QC) protocols. When inconsistencies exist between QC guidelines, method-specific QC criteria take precedence over both technique-specific criteria and those criteria given in Chapter One, and technique-specific QC criteria take precedence over the criteria in Chapter One. Any effort involving the collection of analytical data should include development of a structured and systematic planning document, such as a Quality Assurance Project Plan (QAPP) or a Sampling and Analysis Plan (SAP), which translates project objectives and specifications into directions for those that will implement the project and assess the results. Each laboratory should maintain a formal quality assurance program. The laboratory should also maintain records to document the quality of the data generated. All data sheets and quality control data should be maintained for reference or inspection.

9.2 In order to demonstrate the purity of reagents and sample contact surfaces, a method blank (e.g., a bottle without solid material but with eluent carried through the extraction, filtration and analytical sample preparation process) should be tested.

9.3 The analysis of extracts should follow appropriate QC procedures, as specified in the determinative methods for the COPCs. Refer to Chapter One for specific quality control procedures.

9.4 Solid materials should be tested within one month of receipt unless the project requires that the "as-received" samples are tested sooner (e.g., the material is part of a time-dependent study or the material may change during storage due to oxidation or carbonation).

9.5 Initial demonstration of proficiency (IDP)

Leachate methods are not amenable to typical initial demonstrations of proficiency as reference materials with known values are usually not available. However, prior to using this method an analyst should have documented proficiency in the skills required for successful implementation of the method. For example, skill should be demonstrated in the use of an analytical balance, the determination of pH using methods 9040 and 9045 and the determination of conductance using method 9050.

10.0 CALIBRATION AND STANDARDIZATION

10.1 The balance should be calibrated and certified at a minimum annually or in accordance with laboratory policy.

10.2 Prior to measurement of eluate pH, the pH meter should be calibrated using a minimum of two standards that bracket the range of pH measurements. Refer to Methods 9040 and 9045 for additional guidance.

10.3 Prior to measurement of eluate conductivity, the meter should be calibrated using at least one standard at a value greater than the range of conductivity measurements. Refer to Method 9050 for additional guidance.

11.0 PREPARATORY PROCEDURES

A flowchart of the method is presented in Figure 1. Microsoft Excel data templates are available to aid in collection and archiving of laboratory and analytical data.[2]

11.1 Particle-size reduction (if required)

11.1.1 In this method, particle-size reduction is used to prepare large-grained samples for extraction so that the approach toward liquid-solid equilibrium is enhanced and mass transport through large particles is minimized. A longer extract contact time is required for larger maximum particle-size designations. This method designates three maximum particle sizes and associated contact times (see Table 2). The selection of an appropriate maximum particle size from this table should be based on professional judgment regarding the practical effort required to size reduce the solid material.

11.1.2 Particle-size reduction of "as received" sample may be achieved through crushing, milling or grinding with equipment made from chemically inert materials. During the reduction process, care should be taken to minimize loss of sample and potentially volatile constituents in the sample.

NOTE: Crushing of oversize material is preferred to milling or grinding as the later techniques may result in heating of the sample material.

11.1.3 If the moisture content of the "as-received" material is greater than 15% (wet basis), air drying or desiccation may be necessary. Oven drying is not recommended for preparation of test samples due to the potential for mineral alteration. In all cases, the moisture content of the "as received" material should be recorded.

NOTE: If the solid material is susceptible to interaction with the atmosphere (e.g., carbonation, oxidation), drying should be conducted in an inert environment.

11.1.4 When the material seems to be of a relatively uniform particle size, calculate the percentage less than the sieve size as follows:

$$\%\ Passing = \frac{M_{sieved}}{M_{total}} \times 100\ \%$$

Where: M_{sieved} = mass of sample passing the sieve (g)
M_{total} = mass of total sample (g) (e.g., M_{sieved} + mass not passing sieve)

11.1.5 The fraction retained by the sieve should be recycled for further particle-size reduction until at least 85% of the initial mass has been reduced below the designated maximum particle size. Calculate and record the final percentage passing

[2] These Excel templates form the basis for uploading method data into the data management program, LeachXS Lite™. Both the data templates and LeachXS Lite are available at http://vanderbilt.edu/leaching.

the sieve and the designated maximum particle size. For the uncrushable fraction of the "as received" material, record the fraction mass and nature (e.g., rock, metal or glass shards, etc).

11.1.6 Store the size-reduced material in an airtight container in order to prevent contamination via gas exchange with the atmosphere. Store the container in a cool, dark and dry place prior to use.

11.2 Determination of solids and moisture content

11.2.1 In order to provide the dry mass equivalent of the "as-tested" material, the solids content of the subject material should be determined. Often, the moisture content of the solid sample is recorded. In this method, the moisture content is determined and recorded on the basis of the "wet" or "as-tested" sample.

WARNING: The drying oven should be contained in a hood or otherwise properly ventilated. Significant laboratory contamination or inhalation hazards may result when drying heavily contaminated samples. Consult the laboratory safety officer for proper handling procedures prior to drying samples that may contain volatile, hazardous, flammable or explosive materials.

11.2.2 Place a 5–10-g sample of solid material into a pre-tared dish or crucible. Dry the sample to a constant mass at 105 ± 2 °C. Check for constant mass by returning the dish to the drying oven for twenty four hours, cooling to room temperature in a desiccator and re-weighing. The two mass readings should agree within the larger of 0.2% or 0.02 gram.

NOTE: The oven-dried sample is not used for the extraction and should be properly disposed of once the dry mass is determined.

11.2.3 Calculate and report the solids content as follows:

$$SC = \frac{M_{dry}}{M_{test}}$$

Where: SC = solids content (g-dry/g)
M_{dry} = mass of oven-dried sample (g-dry)
M_{test} = mass of "as-tested" sample (g)

11.2.4 Calculate and report the moisture content (wet basis) as follows:

$$MC_{wet} = \frac{M_{test} - M_{dry}}{M_{test}}$$

Where: $MC_{(wet)}$ = moisture content on a wet basis (g_{H_2O}/g)
M_{dry} = mass of oven-dried sample (g-dry)
M_{test} = mass of "as-tested" sample (g)

11.3 Extraction setup schedule (Microsoft® Excel template provided)

An Excel template accompanies this method and may be used to set up the extraction schedule. If using the provided template, disregard Sec. 11.3 and proceed to the extraction procedure Sec. 11.4.

11.3.1 Using the schedule shown in Table 1 as a guide, set up five test extractions and one method blank. The mass of solids in an extraction may be scaled to minimize headspace in each extraction vessel. However, the volume of eluent should always be based on the target L/S in Column B of Table 1.

11.3.2 Calculate and record the amount of "as-tested" material equivalent to the dry mass in Column D of Table 1 as follows:

$$M_{test} = \frac{M_{dry}}{SC}$$

Where: M_{test} = mass of "as-tested" solid equivalent to the dry-material mass (g)
M_{dry} = mass of dry material specified in the method (g-dry)
SC = solids content of "as-tested" material (g-dry/g)

11.3.3 Calculate and record the volume of moisture contained in the "as-tested" sample in Column E of Table 1 as follows:

$$V_{W,sample} = \frac{M_{test} \times (1 - SC)}{\rho_w}$$

Where: $V_{W,sample}$ = volume of water in the "as tested" sample (mL)
M_{test} = mass of the "as tested" sample (g)
SC = solids content of the "as tested" sample (g-dry/g)
ρ_w = density of water (1.0 g/mL at room temperature)

11.3.4 Calculate and record the volume of reagent water required to bring each extraction to the target L/S in Column F of Table 1 as follows:

$$V_{RW} = M_{dry} \times LS - V_{W,sample}$$

Where: V_{RW} = volume of reagent water required to complete L/S (mL)
M_{dry} = dry mass equivalent of solid sample (g)
LS = liquid-to-dry-solid ratio (10 mL/g)
$V_{W,sample}$ = volume of water in "as used" sample (mL)

The size of the extraction bottle should be sufficient to contain the combined volume of solid material and eluent, ideally with a minimum amount of headspace.

12.0 EXTRACTION PROCEDURE

12.1 Label five bottles with test position numbers and an additional bottle as a method blank according to Column A in Table 1.

12.2 Place the dry-mass equivalent (± 0.1 g) of "as-tested" sample as shown in Column D in Table 1 into each of the five test position extraction vessels.

NOTE: Do not put solid material in the method blank extraction vessel

12.3 Add the appropriate volume (± 0.5 mL) of reagent water to both the test position and method blank extraction vessels as specified in Column F of Table 1.

12.4 Tighten the leak-proof lid on each bottle and tumble all extractions (i.e., test positions and method blanks) in an end-over-end fashion at a speed of 28 ± 2 rpm at room temperature (20 ± 2 °C). The contact time for this method will vary depending on the maximum particle size as shown in Table 2.

NOTE: The length of the contact time is designed to enhance the approach toward liquid-solid equilibrium. Longer contact times are required for larger particles to compensate for the effects of intra-particle diffusion. See Table 2 for required contact times based on the maximum particle size.

12.5 Remove the extraction vessels from the rotary tumbler and clarify the extracts by allowing the bottles to stand for 15 ± 5 min. Alternately, centrifuge the extraction vessels at 4000 ± 100 rpm for 10 ± 2 min.

NOTE: If clarification is significantly incomplete after settling or centrifugation, eluate measurements for pH, conductivity, and oxidization-reduction potential (ORP) may be taken on filtered samples. In this case, perform the filtration in 12.7 prior to eluate measurement in 12.6 and note the deviation from the written procedure.

CAUTION: Following separation from the solid phase, eluate samples lack the buffering provided by the solid phase and therefore may be susceptible to pH change resulting from interaction with air.

12.6 For each extraction vessel, decant a minimum volume (~ 5 mL) of clear, unpreserved supernatant into a clean container.

12.7 Measure and record the pH, specific conductivity, and oxidation-reduction potential (ORP) of the extracts (see Methods 9040, 9045, and 9050).

NOTE: Measurement of pH, conductivity and ORP should be taken within 15 minutes of eluate processing (Sec. 12.8) to avoid neutralization of the solution due to exposure to carbon dioxide, especially when alkaline materials are tested.

NOTE: The measurement of ORP is optional, but strongly recommended, especially when testing materials where oxidation is likely to change the LSP of COPCs.

12.8 Separate the solid from the remaining liquid in each extraction vessel by pressure or vacuum filtration through a clean 0.45-µm pore size membrane (Sec. 6.5). The filtration apparatus may be exchanged for a clean apparatus as often as necessary until all liquid has been filtered.

12.8 Immediately, preserve and store the volume(s) of eluate required for chemical analysis. Preserve all analytical samples in a manner that is consistent with the determinative chemical analyses to be performed.

13.0 DATA ANALYSIS AND CALCULATIONS (EXCEL TEMPLATE PROVIDED)

13.1 Data reporting

13.1.1 Figure 2 shows an example of a data sheet that may be used to report the concentration results of this method. This example is included in the Excel template. At a minimum, the basic test report should include:

a) Name of the laboratory
b) Laboratory contact information
c) Date at the start of the test
d) Name or code of the solid material
e) Particle size (85 wt% less than)
f) Ambient temperature during extraction (°C)
g) Extraction contact time (h)
h) Eluate specific information (see Sec. 13.1.2 below)

13.1.2 The minimum set of data that should be reported for each eluate includes:

a) Eluate sample ID
b) Target L/S (mL/g-dry)
c) Mass of “as tested” solid material used (g)
d) Moisture content of material used (g_{H_2O}/g)
e) Volume of eluent used (mL)
f) Measured final eluate pH
g) Measured eluate conductivity (mS/cm)
h) Measured ORP (mV) (optional)
i) Concentrations of all COPCs
j) Analytical QC qualifiers as appropriate

13.2 Data interpretation and presentation (optional)

13.2.1 LSP curve

13.2.1.1 A constituent LSP curve can be generated for each COPC after chemical analysis of all extracts by plotting the constituent concentration in the liquid phase as a function of L/S used for each extraction. The curve indicates the equilibrium concentration of the COPC as a function of L/S at the natural pH.

13.2.1.2 The lower limit of quantitation (LLOQ) for the analytical technique for each COPC may be shown as a horizontal line. COPC concentrations below this line indicate negligible or non-quantitative concentrations.

NOTE: The LLOQ is highly matrix dependent and should be determined as part of a QA/QC plan.

13.2.1.3 Figure 3 provides example LSP curves as a function of L/S for a coal combustion fly ash and a coal combustion flue gas desulfurization filter cake.

14.0 METHOD PERFORMANCE

14.1 Performance data and related information are provided in SW-846 methods only as examples and guidance. The data do not represent required performance criteria for users of the methods. Instead, performance criteria should be developed on a project-specific basis, and the laboratory should establish in-house QC performance criteria for the application of this method. These performance data are not intended to be and must not be used as absolute QC acceptance criteria for purposes of laboratory accreditation.

14.2 Interlaboratory validation of this method was conducted using a coal combustion fly ash (material code EaFA), a contaminated smelter site soil (material code CFS) and a solidified waste analog (material code SWA). The median values and inner quartile ranges (IQRs) for repeatability and reproducibility were determined for eluate concentration results across all study materials and pH target values (see Table 3). More details on the interlaboratory validation may be found in Ref. 6.

14.3 Refs. 1 and 2 may provide additional guidance and insight on the use, performance and application of this method.

15.0 POLLUTION PREVENTION

15.1 Pollution prevention encompasses any technique that reduces or eliminates the quantity and/or toxicity of waste at the point of generation. Numerous opportunities for pollution prevention exist in laboratory operations. The EPA has established a preferred hierarchy of environmental management techniques that places pollution prevention as the management option of first choice. Whenever feasible, laboratory personnel should use pollution prevention techniques to address their waste generation. When wastes cannot be feasibly reduced at the source, the Agency recommends recycling as the next best option.

15.2 For information about pollution prevention that may be applicable to laboratories and research institutions consult Less is Better: Laboratory Chemical Management for Waste Reduction available from the American Chemical Society's Department of Government Relations and Science Policy, 1155 16th St., N.W. Washington, D.C. 20036, http://portal.acs.org/portal/fileFetch/C/WPCP_012290/pdf/WPCP_012290.pdf.

16.0 WASTE MANAGEMENT

The Environmental Protection Agency requires that laboratory waste management practices be conducted consistent with all applicable rules and regulations. The Agency urges laboratories to protect the air, water, and land by minimizing and controlling all releases from hoods and bench operations, complying with the letter and spirit of any sewer discharge permits and regulations, and by complying with all solid and hazardous waste regulations, particularly the hazardous waste identification rules and land disposal restrictions. For further information on waste management, consult The Waste Management Manual for Laboratory Personnel available from the American Chemical Society at the address listed in Sec. 15.2.

17.0 REFERENCES

1. D.S. Kosson, H.A. van der Sloot, F. Sanchez and A.C. Garrabrants (2002) “An Integrated Framework for Evaluating Leaching in Waste Management and Utilization of Secondary Materials,” Environmental Engineering Science, 19(3) 159-204.

2. A.C. Garrabrants, D.S. Kosson, H.A. van der Sloot, F. Sanchez and O. Hjelmar (2010) “Background Information for the Leaching Environmental Assessment Framework (LEAF) Test Methods,” EPA/600/R-10-170, U.S. Environmental Protection Agency, Washington, DC, December 2010.

3. F. Sanchez, R. Keeney, D.S. Kosson and R. DeLapp (2006) “Characterization of Mercury-Enriched Coal Combustion Residues from Electric Utilities Using Enhanced Sorbents for Mercury Control,” EPA-600/R-06/008, U.S. Environmental Protection Agency, Washington DC, February 2006.

4. F. Sanchez, D.S. Kosson, R. Keeney, R. DeLapp, L. Turner and P. Kariher (2008) “Characterization of Coal Combustion Residues from Electric Utilities Using Wet Scrubbers for Multi-Pollutant Control,” EPA-600/R-08/077, U.S. Environmental Protection Agency, Washington DC, July 2008.

5. D.S. Kosson, F. Sanchez, P. Kariher, L.H. Turner, R. DeLapp and P. Seignette (2009) “Characterization of Coal Combustion Residues from Electric Utilities – Leaching and Characterization Data,” EPA-600/R-09/151, U.S. Environmental Protection Agency, Washington DC, December 2009.

6. A.C. Garrabrants, D.S. Kosson, L. Stefanski, R. DeLapp, P.F.A.B. Seignette, H.A. van der Sloot, P. Kariher, and M. Baldwin (2012) “Interlaboratory Validation of the Leaching Environmental Assessment (LEAF) Method 1313 and Method 1316,” DRAFT, U.S. Environmental Protection Agency, Washington DC, April 2012.

7. EN12457 (2001) Characterization of Waste – Leaching – Compliance Test for Leaching of Granular Waste Materials and Sludges, Comité Européen de Normalisation, Brussels, Belgium.

18.0 TABLES, DIAGRAMS, FLOW CHARTS, AND VALIDATION DATA

The following pages contain the tables and figures referenced by this method

TABLE 1

EXAMPLE SCHEDULE FOR EXTRACTION SETUP

A	B	C	D	E	F	G
Test Position	Target LS	Minimum Dry Mass (g-dry)	Mass of "As-Tested" Sample (g)	Moisture in "As-Tested" Sample (mL)	Volume of Reagent Water (mL)	Recommended Bottle Size (mL)
T01	10.0	20	22.2	2.2	198	250
T02	5.0	40	44.4	4.4	196	250
T03	2.0	100	111.1	11.1	189	500
T04	1.0	200	222.2	22.2	178	500
T05	0.5	400	444.4	44.4	156	1000
B03	QC	–			200	250
Total		–	844.4		1120	

NOTE: 1) This schedule assumes a target liquid volume of 200 mL.
2) This schedule is based on “as tested” solids content of 0.90 g-dry/g.
3) Test position marked B01 is a method blank of reagent water.

Table data modified from Ref. 1.

TABLE 2

EXTRACTION PARAMETERS AS FUNCTION OF MAXIMUM PARTICLE SIZE

Particle Size (85% less than) (mm)	US Sieve Size	Minimum Dry Mass (g-dry)	Contact Time (h)	Recommended Vessel size (mL)
0.3	50	20 ± 0.05	24 ± 2	250
2.0	10	40 ± 0.1	48 ± 2	500
5.0	4	80 ± 0.1	72 ± 2	1000

TABLE 3

MEDIAN METHOD PRECISION ACROSS STUDY MATERIALS

		Repeatability		Reproducibility	
Analyte	Symbol	Median $\%RSD_r$	IQR $\%RSD_r$	Median $\%RSD_R$	IQR $\%\ RSD_R$
Antimony	Sb	12%	8-13%	21%	17-27%
Arsenic	As	15%	12-28%	31%	23-34%
Barium	Ba	7%	5-9%	16%	13-30%
Boron	B	7%	5-10%	13%	9-34%
Calcium	Ca	6%	3-7%	8%	7-19%
Molybdenum	Mo	7%	6-9%	18%	11-31%
Selenium	Se	8%	4-9%	20%	13-24%
Vanadium	V	6%	4-12%	16%	13-26%
Median of Medians		7%	3-28%	17%	7-34%

Data taken from Ref. 6.

FIGURE 1

METHOD FLOWCHART

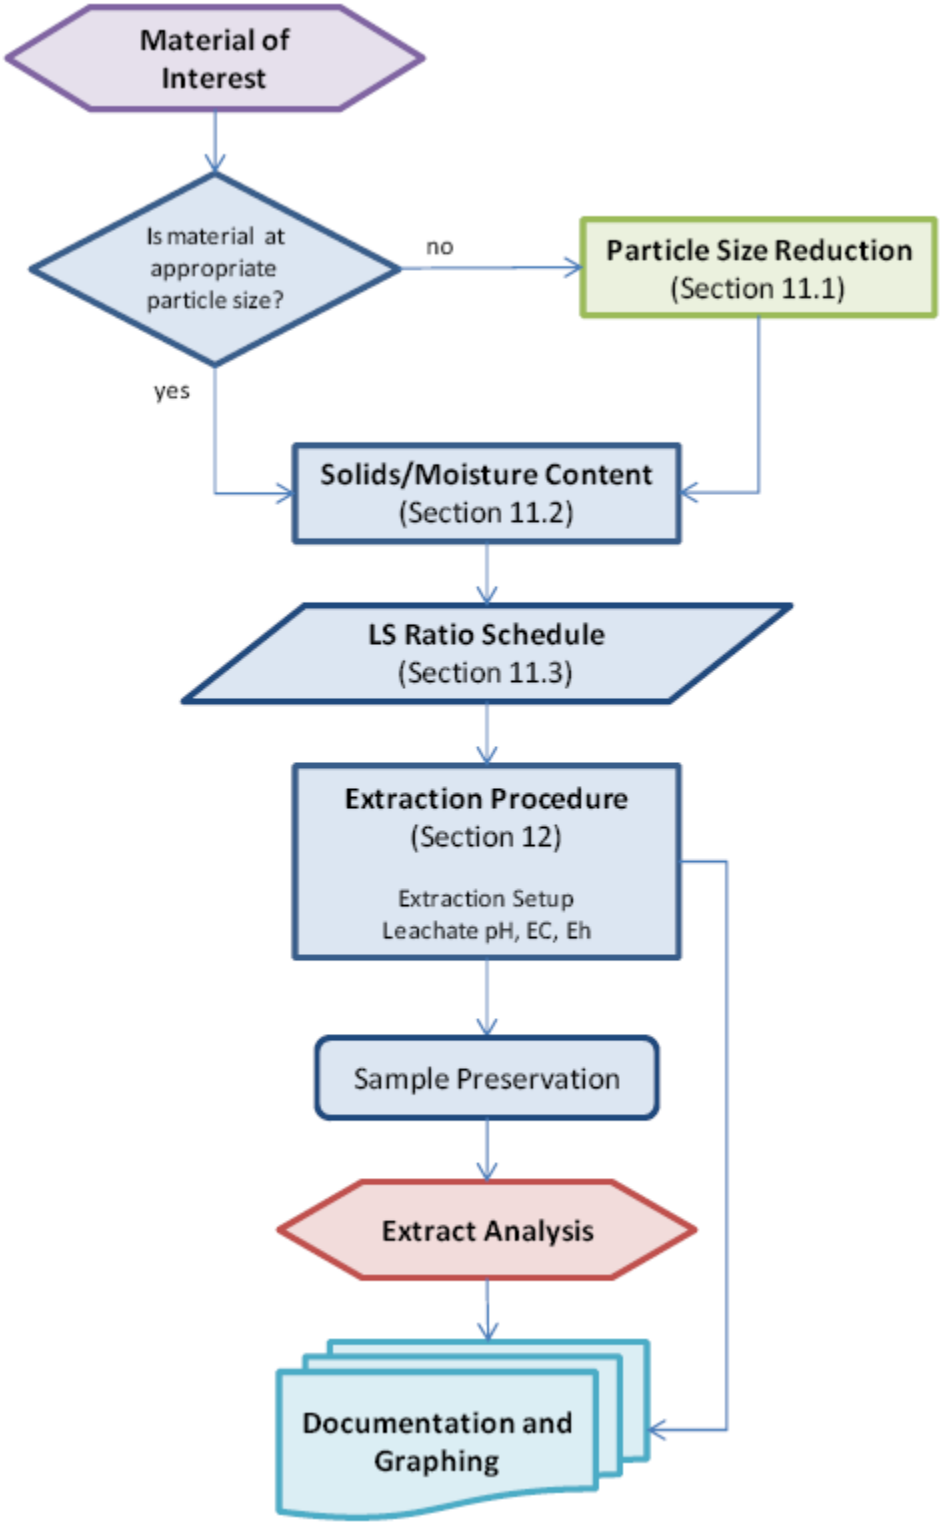

FIGURE 2

EXAMPLE DATA REPORTING SHEET

EPA METHOD 1316
Report of Analysis

ABC Laboratories
123 Main Street
Anytown, USA
Contact: John Smith
(555) 111-1111

Client Contact: Susan Jones
(555) 222-2222

Material Code:	**FAX**	Particle Size:	88% passing 2-mm sieve
Material Type:	Coal Combustion Fly Ash	Contact Time:	860 g
Date Received:	10/1/20xx	Lab Temperature:	21 ± 2 °C
Test Start Date:	11/1/20xx	Eluent Used:	ASTM Type II Water
Report Date:	12/1/20xx		

Test Position	Replicate	Value	Units	Method	Note
T01	**A**				
	Eluate Sample ID	**XYZ-1316-T01-A**			
	Solid Material	40.0	g		
	Moisture Content	0.01	g_{H_2O}/g		
	Water Added	386.0	mL		
	Target L/S	10.0	mL/g-dry		
	Eluate pH	1.89	–	EPA 9040	
	Eluate Conductivity	12.6	mS/cm	EPA 9050	
	Eluate ORP	203	mv		

Chemical Analysis	Value	Units	QC Flag	Method	Date	Dilution Factor
Al	216.0	mg/L		EPA 6020	11/7/20xx	1000
As	7.64	mg/L		EPA 6020	11/7/20xx	10
Cl	< 4.13	mg/L	U	EPA 9056	11/9/20xx	1

Test Position	Replicate	Value	Units	Method	Note
T02	**A**				
	Eluate Sample ID	**XYZ-1316-T02-A**			
	Solid Material	20.0	g		
	Moisture Content	0.01	g_{H_2O}/g		
	Water Added	400.0	mL		
	Target L/S	5.0	mL/g-dry		
	Eluate pH	3.86		EPA 9040	
	Eluate Conductivity	0.99	mS/cm	EPA 9050	
	Eluate ORP	180	mv		

Chemical Analysis	Value	Units	QC Flag	Method	Date	Dilution Factor
Al	449.0	mg/L		EPA 6020	11/7/20xx	1000
As	97.9	mg/L		EPA 6020	11/7/20xx	10
Cl	< 4.13	mg/L	U	EPA 9056	11/7/20xx	1

QC Flag Key: U Value below lower limit of quantitation as reported (< "LLOQ")

FIGURE 3

EXAMPLE CONCENTRATON RESULTS FROM A COAL COMBUSTION FLY ASH AND FLUE-GAS DESULFURIZATION FILTER CAKE

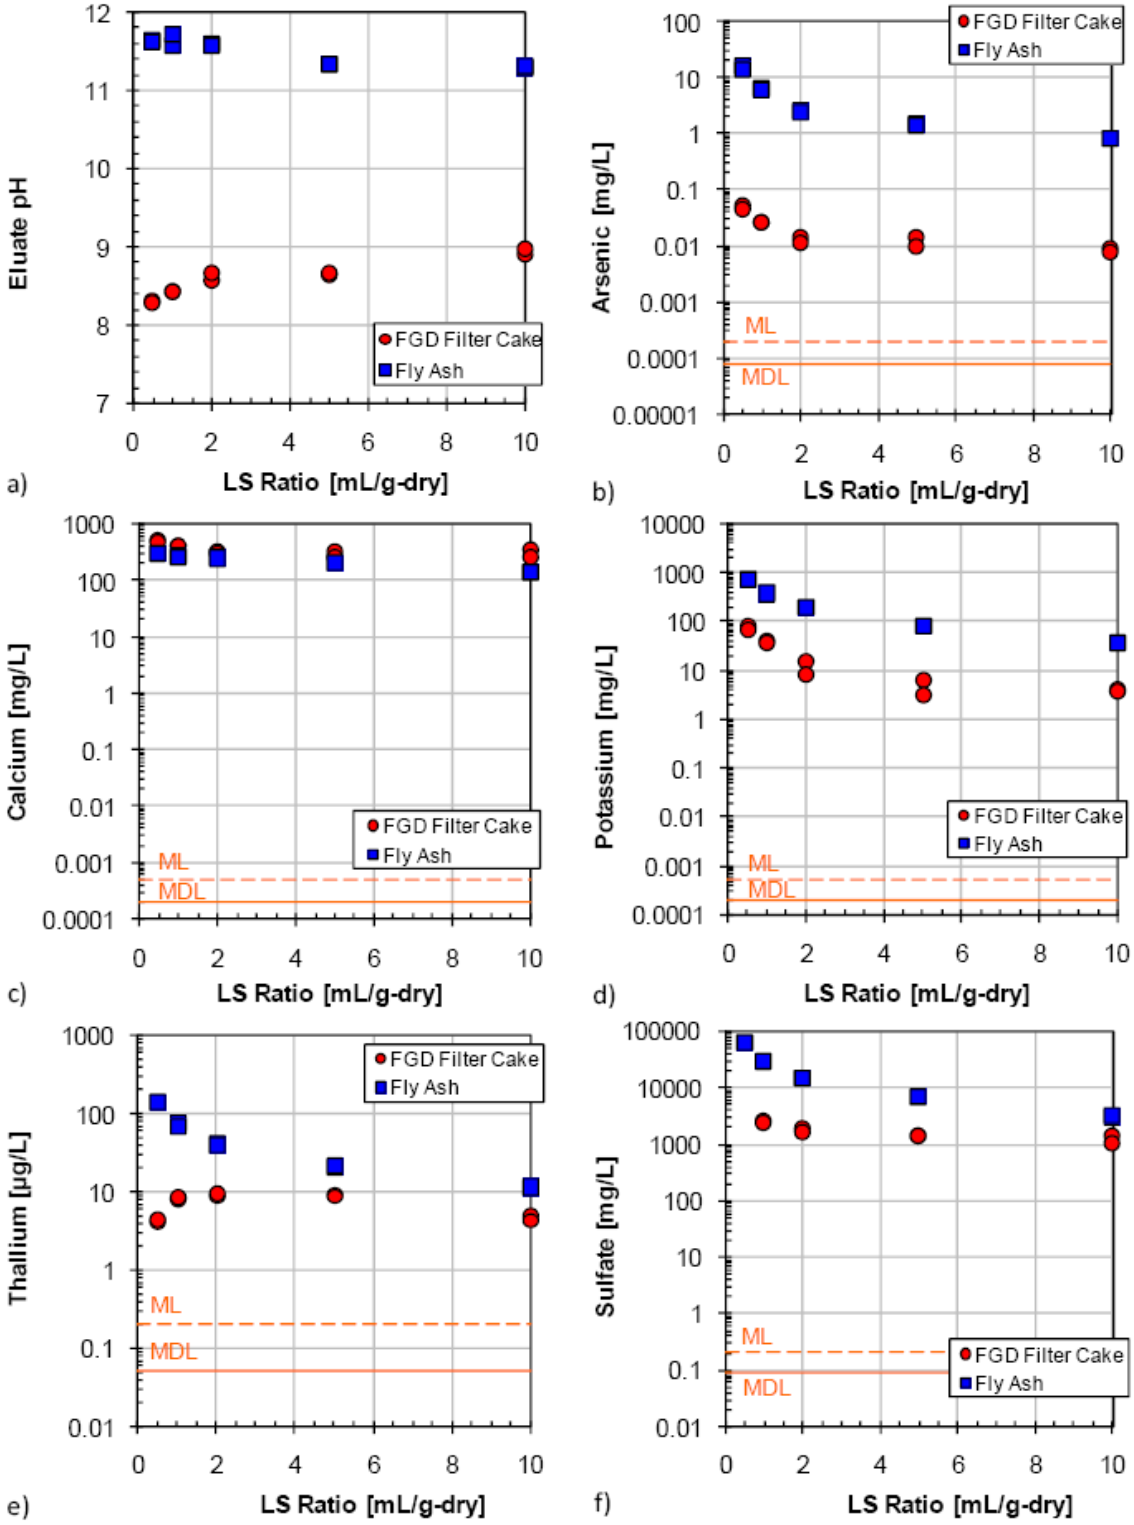

Appendix C. Quality Assurance Project Plan

QAPP for the EPA Interlaboratory Validation Study of Proposed SW846 Leaching Methods

Quality Assurance Project Plan
Category III / Technology Development
Draft

Contract No. EP-C-09-027
Work Assignment No. 2-7

November 2011

10/25/2011
Peter Kariher Date
ARCADIS U.S., Inc
Work Assignment Leader

10/25/2011
Libby Nessley Date
ARCADIS U.S., Inc.
Quality Assurance Officer

11/22/11
Susan Thorneloe Date
U.S. Environmental Protection Agency
Work Assignment Manager

11/22/11
Richard Shores Date
U.S. Environmental Protection Agency
Chief, Emissions Characterization & Prevention Branch

11/22/11
Robert Wright Date
U.S. Environmental Protection Agency
Quality Assurance Representative

QAPP for the EPA Interlaboratory Validation Study of Proposed SW846 Leaching Methods

Quality Assurance Project Plan
Category III / Technology Development
Final

Prepared for:
Susan Thorneloe
U.S. Environmental Protection Agency
National Risk Management Research Laboratory
Air Pollution Prevention and Control Division
Atmospheric Protection Branch
Research Triangle Park, NC 27711

Prepared by:
ARCADIS U.S., Inc.
4915 Prospectus Drive
Suite F
Durham
North Carolina 27713
Tel 919 544 4535
Fax 919 544 5690

Our Ref.:
RN990272.0007

Date:
November 2011

Appendices ii

List of Figures iii

List of Acronyms and Abbreviations iii

Distribution List vi

1. Project Objectives and Organization 1

1.1 Purpose 1

1.2 Project Objectives 2

2. Project Organization 4

3. Experimental Approach 9

3.1 Task I: Preparing Homogenized CCR 11

3.2 Task II: Leaching of the CCR by Reference Laboratory and the Intercomparison Laboratories 14

3.3 Task III: Determination of the Reproducibility of Each Method 16

3.4 Task IV: Testing of Select Materials for Leaching by SW-846 Methods 1311 (TCLP) and 1312 (SPLP) 16

3.5 Task V: Testing of Fly Ashes and Cement Kiln Dust for Radionuclide Testing by Germanium Detector 17

4. Sampling Procedures 18

4.1 Sample Custody Procedures 18

4.2 CCR, and Leaching Reference Material Samples 19

4.2.1 Physical and Chemical Characterization Samples 19

4.2.2 Leaching Study Samples 20

4.3 Leachate Collection 20

5. Testing and Measurement Protocols to be Used for Reference Material Characterization and Eluate Characterization 23

5.1 Physical Characterization 23

5.1.1 pH and Conductivity 23

5.1.2 Moisture Content and Loss on Ignition (LOI) 23

5.2 Chemical Characterization 24

5.2.1 Dissolved Organic Carbon / Dissolved Inorganic Carbon (DOC/DIC) and Elemental Carbon / Organic Carbon (EC/OC) 24

5.2.2 Mercury by Thermal Decomposition and Cold Vapor Atomic Adsorption (TD-CVAA) Method 7473 25

5.2.3 Other Metals (ICP) 25

5.2.4 X-Ray Fluorescence (XRF) 29

5.2.5 XRF Detection Limits 30

5.2.6 Radionuclide Testing of CCRs using Ge-Detector 32

6. Quality Assurance/Quality Control 34

6.1 Data Quality Indicator Goals 34

6.2 QC Sample Types 35

7. Data Reduction, Validation, and Reporting 36

7.1 Data Analysis 36

7.2 Chemical (ICP, XRF, AE-OES, OC/EC) and Physical (Moisture) Characterization 41

7.3 Radionuclide Characterization 42

8. Assessments 44

9. References 46

Appendices

Appendix A Participating Laboratories

Appendix B Example Method Template Spreadsheet

Appendix C Documentation Sent to Each Participating Laboratory

List of Tables

Table 3-1. MDLs and RLs of the Metals to be Evaluated during the Validation Study 12

Table 3-2. Characterization Testing to Establish Homogeneity of the CCR 13

Table 3-3. Tentative Schedule for Interlaboratory Validation of Pre Method 1313 and Pre Method 1316 16

Table 4-1. Final Extract pH Targets 20

Table 4-2. Example Schedule for Extraction Setup 21

Table 5-1. MDL and MLQ of Total Organic Carbon Analyzer 24

Table 5-2. Method Detection Limits (MDLs) and Minimum Level of Quantification (ML) for ICP-OES Analysis on Liquid Samples* 28

Table 5-3. XRF Reporting and Detection Limits 31

Table 6-1. Data Quality Indicator Goals 34

Table 8-1. PEA Parameters and Ranges 44

List of Figures

Figure 2-1. Project Organizational Chart 5

List of Acronyms and Abbreviations

AA	atomic adsorption
ANOVA	analysis of variance
APPCD	Air Pollution Prevention and Control Division
ARCADIS	ARCADIS, U.S., Inc.
CCR(s)	coal combustion residue(s)
CCV	continuing calibration verification
COPC(s)	constituent(s) of potential concern
CVAA	cold vapor atomic adsorption
DIC	dissolved inorganic carbon
DOC	dissolved organic carbon

DQI	data quality indicator
EC	elemental carbon
EPA	U.S. Environmental Protection Agency
FGD	flue-gas desulfurization
FWHM	full width at half maximum
g	gram
HPGe	high purity germanium
IC	inorganic carbon
ICP	inductively couple plasma
ICV	initial calibration verification
LOI	loss on ignition
MDA	minimum detectable activity
MDL	method detection limit
mL	milliliter
ML	minimum level of quantification
MLQ	minimum level of quantification
MS	mass-spectrometry
NA	not applicable
NCSU	North Carolina State University
NIST	National Institute of Science and Technology
NPOC	non-purgeable organic carbon
OC	organic carbon
OES	optical emission spectroscopy
ORCR	Office of Resource Conservation and Recovery
ORD	Office of Research and Development
OSR	Office of Solid Waste
QAPP	quality assurance project plan
RL	reporting limit
RPD	relative percent difference
RSD	relative standard deviation
SPLP	synthetic precipitation leaching procedure

SW-846	EPA Test Methods for Evaluating Solid Waste, Physical/Chemical Methods
TCLP	toxicity characteristic leaching procedure
TD	thermal decomposition
TSA	technical system audit
XRF	X-ray fluorescence spectrometry

Distribution List

Copies of this plan and all revisions will be initially sent to the following individuals. It is the responsibility of the U.S. Environmental Protection Agency (EPA) Work Assignment Manager and of the ARCADIS, U.S., Inc. (ARCADIS) Work Assignment Leader to make copies of the plan available to all field personnel.

Susan Thorneloe, EPA Work Assignment Manager. Office of Research and Development, National Risk Management Research Laboratory, Air Pollution Prevention and Control Division, Research Triangle Park, NC.

Phone: (919) 541-2709
Email: thorneloe.susan@epa.gov

Robert Wright, EPA Quality Assurance Officer. Office of Research and Development, National Risk Management Research Laboratory, Air Pollution Prevention and Control Division, Research Triangle Park, NC.

Phone: (919) 541-4502
Email: wright.bob@epa.gov

Peter Kariher, ARCADIS Work Assignment Leader. Research Triangle Park, NC.

Phone: (919) 541-5740
Email: peter.kariher@arcadis-us.com

Libby Nessley, ARCADIS Quality Assurance Officer. Durham, NC.

Phone: (919) 544-4535 x258
Email: libby.nessley@arcadis-us.com

Dr. David Kosson, Methods Development. Vanderbilt University, Nashville, TN.

Phone: (615) 322-1064
Email: David.Kosson@vanderbilt.edu

Dr. Florence Sanchez, Methods Development. Vanderbilt University, Nashville, TN.

Phone: (615) 322-5135
E-mail: Florence.Sanchez@vanderbilt.edu

Dr. Andrew Garrabrants, Methods Development. Vanderbilt University, Nashville, TN.

Phone: (615) 322-7226
Email: Andrew.Garrabrants@vanderbilt.edu

Dr. Hans van der Sloot, Methods Development. Hans van der Sloot Consultancy, The Netherlands.

Phone: +31(0)226-341607
Email: hans@vanderslootconsultancy.nl

Dr. Leonard A Stefanski, Statistical Consultant. North Carolina State University, Raleigh, NC.

Phone: (919) 515-1945
Email: stefanski@stat.ncsu.edu

1. Project Objectives and Organization

1.1 Purpose

The Air Pollution Prevention and Control Division (APPCD) of EPA's Office of Research and Development (ORD) is conducting research to evaluate potential leaching and cross media transfers of mercury and other constituents of potential concern (COPCs) resulting from the management of coal combustion residues (CCRs) resulting from wider use of state-of-the art air pollution control technology. This research was cited as a priority in EPA's Mercury Roadmap (http://www.epa.gov/mercury/roadmap.htm) to ensure that one environmental problem is not being traded for another. The objective is to understand the fate of mercury and other COPCs and ensure that emissions being controlled in the flue gas at power plants are not later being released depending upon how the CCRs are managed.

As part of this research effort, individual leaching test methods have been developed for inclusion into SW846. These methods were adapted by Dr. David Kosson, Dr. Florence Sanchez, and Dr. Andrew Garrabrants of Vanderbilt University, and their consultant, Dr. Hans van der Sloot from The Netherlands, from the publication titled *An Integrated Framework for Evaluating Leaching in Waste Management and Utilization of Secondary Materials* (Kosson et al., 2002, Environmental Engineering Science, Volume 19, Number 3, 159-203). Four test methods have been developed as preliminary versions of EPA methods[1] and can be found at http://www.vanderbilt.edu/leaching/downloads.html. The four leaching test methods include:

1. Pre Method 1313: Liquid-Solid Partitioning as a Function of Extract pH for Constituents in Solid Materials using a Parallel Batch Extraction Procedure

2. Pre Method 1314: Liquid-Solid Partitioning as a Function of Liquid-Solid Ratio for Constituents in Solid Materials using an Up-flow Percolation Column Procedure

3. Pre Method 1315: Mass Transfer Rates of Constituents in Monolithic or Compacted Granular Materials using a Semi-dynamic Tank Leaching Procedure

4. Pre Method 1316: Liquid-Solid Partitioning as a Function of Liquid-Solid Ratio for Constituents in Solid Materials using a Parallel Batch Extraction Procedure

[1] Preliminary Version denotes that this method has not been endorsed by EPA but is under consideration for inclusion into SW-846.

Multilaboratory validation data is necessary for a method to be considered for inclusion in SW-846 (per *Guidance for Methods Development and Validation for the RCRA Program)*. This Quality Assurance Project Plan (QAPP) is being written to cover the EPA Interlaboratory Validation Study of the above four proposed SW-846 leaching methods. A separate interlaboratory study will be performed for each of the four methods separately. Due to similarities in equipment and procedures, the first methods to be tested are Pre Method 1313 and Pre Method 1316.

1.2 Project Objectives

US EPA's Office of Resource Conservation and Recovery (ORCR) formerly the Office of Solid Waste (OSW) requires that an interlaboratory validation be conducted for a method to be considered for inclusion into SW-846. This QAPP will detail the process by which each of the four proposed leaching methods will be validated by at least five, and up to ten, different laboratories to establish reproducibility.

The determination of laboratory reproducibility is the final stage in the method development process, prior to the submission of the method for ORCR review. By reproducibility, the Agency means that multiple operators and multiple laboratories should be able to obtain comparable performance data on split samples using the method. It is necessary to demonstrate that satisfactory method performance is not limited to the individual operator or laboratory that developed the method. The minimum number of laboratories that are needed to participate in a multilaboratory method validation is three, with preferably more. Developers of new methods need to do a limited multilaboratory evaluation and provide the individual laboratory and summary performance data in the method submission.

This QAPP is a replacement of the QAPP approved on June 21, 2010 (QTRAK# 03069-A00244). This QAPP will provide details of the following tasks:

- Preparation and characterization of the CCR by APPCD's on-site laboratory support contractor, ARCADIS, prior to distributing to each laboratory participating in the validation study (Task 1)

- Leaching of CCR and other method validation materials (by the proposed SW846 method) by ARCADIS (to establish the baseline results) and by each participating laboratory. All leachates will be submitted to Vanderbilt University for analysis (Task 2)

- Determination of the reproducibility (variability between laboratories), repeatability (single-operator precision) and accuracy of each method (Task 3)

- Leaching of 5 fly ash, 3 scrubber sludge, the 3 other validation materials (foundry sand, solid waste analog, and contaminated field soil), and a cement kiln dust sample using SW-846 Method 1311 "Toxicity Characteristic Leaching Procedure" (EPA, 1992) and SW-846 Method 1312 "Synthetic

Precipitation Leaching Procedure" (EPA, 1994) with analysis for metals by ICP-OES for comparison with the proposed new leaching methods (Task 4)

- Vanderbilt will perform radionuclide testing on 35 fly ash samples, 6 flue-gas desulfurization (FGD) gypsum and 1 cement kiln dust samples to determine uranium species and concentrations by the measurement of Beta and Gamma decay particles (Task 5)

2. Project Organization

The organizational chart for this project is shown in Figure 2-1. The roles and responsibilities of the project personnel are discussed in the following paragraphs. In addition, contact information is also provided. Appendix A identifies the nine laboratories participating in this interlaboratory validation study.

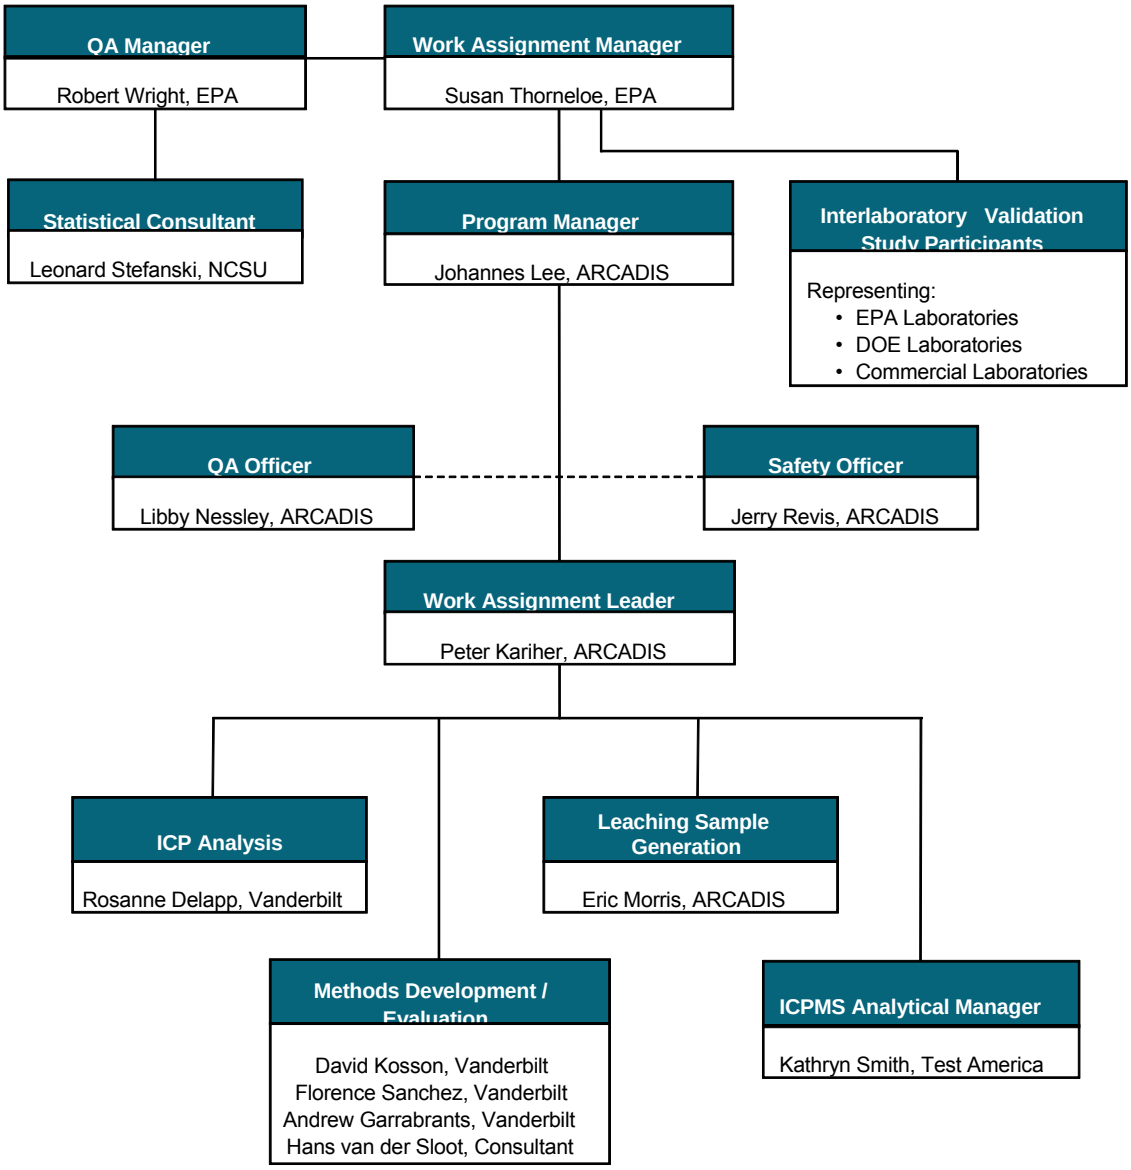

Figure 2-1. Project Organizational Chart

EPA Work Assignment Manager, Susan Thorneloe: The EPA WA Manager is responsible for communicating the scope of work, and is the primary party responsible for review and approval of this QAPP and all other deliverables under this work assignment. The EPA WA Manager is responsible for providing ARCADIS with the various CCR to be used for this interlaboratory validation study. Ms. Thorneloe will also send requests to a number of EPA, DOE and commercial laboratories asking for participation in this interlaboratory study, and will be responsible for making the final selection of which laboratories will be included in the study. She will receive the laboratory data packages, and oversee the evaluation of the results by Vanderbilt, ARCADIS, and the NCSU statistician.

Phone: (919) 541-2709
E-mail: thorneloe.susan@epamail.epa.gov

EPA QA Representative, Robert Wright: The EPA QA Representative will be responsible for reviewing and approving this QAPP. This project has been assigned a QA category III and may be audited by EPA QA. Mr. Wright is responsible for coordinating any EPA audits.

Phone (919) 541-4502
E-mail: wright.bob@epamail.epa.gov

ARCADIS Work Assignment Leader, Peter Kariher: The ARCADIS WA Leader is responsible for preparing project deliverables and managing the work assignment. He will ensure the project meets scheduled milestones and stays within budgetary constraints agreed upon by EPA. The WA Leader is also responsible for communicating any delays in scheduling or changes in cost to the EPA WA Manager as soon as possible. Mr. Kariher, along with Dr. Kosson (Vanderbilt) and Dr. Stefanski (NCSU) will review the laboratory data packages.

Phone (919) 541-5740
E-mail: peter.kariher@arcadis-us.com

ARCADIS Inorganic Laboratory Manager, Peter Kariher: In addition to being the WA Leader, Peter Kariher is also responsible for the operation of EPA's in-house Inorganic Laboratory. Mr. Kariher is responsible for preparation of this QAPP, and will prepare the homogenized CCR(s) to be used in the interlaboratory validation study. He will perform the characterization and leaching of each CCR by Pre-Methods 1313 and 1316 prior to distributing the CCR to the labs for comparative analysis. Mr. Kariher will operate the mercury analyzer and ion chromatograph, and for the leaching studies and mercury and metals analyses, will be supported by one technician: John Foley. Mr. Kariher will perform SW-846 Method 3052 digestion of solid CCR samples and also be responsible for mercury analysis of samples by CVAA. John Foley will perform the leaching tests. Mr. Kariher will submit the remaining Method 3052 digestates to the subcontract analytical laboratory, Test America-Savannah for ICP/MS analysis of the other target metals. He will also be involved with the EPA WAM and the Vanderbilt University methods developers in evaluating the results.

Phone (919) 541-5740
E-mail: peter.kariher@arcadis-us.com

Test America-Savannah Analytical Manager, Kathryn Smith: Ms. Smith will review and validate the ICP/MS results for total content digest samples and report them to Mr. Kariher.

Phone (912) 354-7858
E-mail: kathye.smith@testamericainc.com

ARCADIS Designated QA Officer, Libby Nessley: The ARCADIS QA Manager, Libby Nessley, has been assigned QA responsibilities for this work assignment. Ms. Nessley will be responsible for reviewing this QAPP prior to submission to EPA QA for review. Ms. Nessley will perform an internal data quality audit on at least 10% of the ARCADIS reported data. In addition, she will perform a Technical System Audit (TSA) if requested by the EPA WAM or the ARCADIS WAL. All QA/QC related problems will be reported directly to the ARCADIS WAL, Peter Kariher.

Phone: (919) 544-4535
E-mail: libby.nessley@arcadis-us.com

Vanderbilt University, Methods Development, Professors David Kosson, Florence Sanchez, Andrew Garrabrants, and Rossane Delapp; Consultant, Methods Development, Hans van der Sloot: Dr. Kosson in cooperation with Dr. Florence Sanchez, Dr. Andrew Garrabrants, and Dr. Hans van der Sloot developed the leachability methods being evaluated during this interlaboratory validation study. All leachates will be sent to Vanderbilt University for analysis by ICP-OES. Ms. Rossane Delapp will assist in the analysis of the leachates for determination of the non-mercury metals concentrations and will develop the LeachXS Lite analytical database for sample data viewing and reporting. Ms. Delapp will also be responsible for the reference lab application of Pre-Methods 1313, 1314, 1315 and 1316. Drs. Kosson, Sanchez, Garrabrants, and van der Sloot will be available to consult with the EPA WAM and ARCADIS Inorganic Laboratory Manager regarding the evaluation of the interlaboratory comparative results for each of the proposed SW846 methods. Dr. Kosson, Dr. Garrabrants, Mr. Kariher (ARCADIS) and Dr. Stefanski (NCSU) will review the laboratory data packages.

Dr. David Kosson
Phone: (615) 322-1064
E-mail: David.Kosson@vanderbilt.edu

Dr. Florence Sanchez
Phone: (615) 322-5135
E-mail: Florence.Sanchez@vanderbilt.edu

Dr. Andrew Garrabrants
Phone: (615) 322-7226
E-mail: Andrew.Garrabrants@vanderbilt.edu

Dr. Hans van der Sloot
Phone: +31(0)226-341607
E-mail: hans@vanderslootconsultancy.nl

Ms. Rossane Delapp
Phone: (615) 322-1064
E-mail: rossane.c.delapp@vanderbilt.edu

ARCADIS Project Manager, Johannes Lee: The ARCADIS Project Manager, Johannes Lee, has been assigned financial, contractual and managerial responsibilities for this work assignment. Mr. Lee will be responsible for communications with the EPA project officer, the oversight of financial status, and fulfilling contractual requirements.

Phone: (919) 544-4535
E-mail: johannes.lee@arcadis-us.com

ARCADIS Safety Officer, Jerry Revis: The ARCADIS Safety Officer, Jerry Revis, has been assigned the safety supervisor responsibilities for this work assignment. Mr. Revis will be responsible for reviewing safety plans, performing periodic safety inspections, communicating with the EPA safety office, and oversight of safety operations.

Phone: (919) 544-4535
E-mail: jerry.revis@arcadis-us.com

North Carolina State University (NCSU), Statistical Consultant, Dr. Leonard A Stefanski: Dr. Stefanski will provide statistical consultation on the planning and implementation of interlaboratory study to ensure validity of the collected data. He will also provide advice on the choice and application of statistical methods used to analyze the study data, and on the interpretation of results obtained from the statistical analyses. Dr. Stefanski will report to Mr. Wright, the EPA QA Representative. He will assist Dr. Kosson (Vanderbilt) and Mr. Kariher (ARCADIS) in reviewing the laboratory data packages.

Phone: 919-515-1945
E-mail: stefanski@stat.ncsu.edu

3. Experimental Approach

This interlaboratory comparison will include a comparison of leaching test methods performance by a reference laboratory (either ARCADIS or Vanderbilt) and minimum of six participant laboratories (see Appendix A; nine participant laboratories are currently planned) based on testing of three different materials for each leaching test method to be evaluated. The goal of this study is to determine intra-laboratory and inter-laboratory reproducibility for the four test methods under development. Following is a list of key elements for regulatory methods development as specified in the SW-846 guidance document, and the applicability of each element for this study:

Element 1: Identification of Scope and Application and Regulatory Need

The methods being developed through this study are intended to provide improved leaching characterization of wastes and other materials for use and disposal under a range of field exposure conditions by considering the materials physical characteristics that effect water flow (e.g., granular or monolithic and thus controlling whether water flows through or around the material), and potential field conditions (i.e., pH, water contact mode, liquid-solid ratio). These methods are planned to be applicable for assessments where use of other leaching test methods are not statutorily required.

Element 2: QA/QC Requirements

QA/QC requirements for each method under development are indicated within each method description and are consistent with SW-846 requirements. QA/QC requirements for this study are indicated in this QAPP.

Element 3: Analytical Approach

This study is to evaluate leaching tests (e.g., aqueous extraction tests) that are operationally defined and intended to provide estimation of underlying physical and chemical phenomena controlling constituent release from a solid material to contacting water. Thus, the method of analysis selected for leaching test eluates (i.e., ICP-OES) was a method that was suitably efficient and sensitive for the purposes of this study (see Section 5.2.3). Additional characterization of materials to be tested is being carried out using other analytical techniques (see Section 5).

Element 4: Method/Instrument Sensitivity

Method/instrument sensitivity is based on the chemical analysis technique for leaching test eluates that is selected. This study uses previously standardized methods for chemical analysis.

Element 5: Method Optimization and Ruggedness Testing

An extensive study has been completed that provides an evaluation of related test methods development and optimization based on compilation and evaluation of results from international studies (van der Sloot, et al. 2010). This program is consistent with those findings.

Element 6: Accuracy, Precision and Repeatability (Clean Matrix)

Determination of accuracy is not possible for leaching tests because they are operationally defined and there is no absolute correct value that can be verified using an independent characterization technique. Precision and repeatability for a clean matrix is not possible because of the nature of the materials being evaluated. Instead, intra-laboratory and inter-laboratory repeatability and reproducibility is determined.

Element 7: Effect of Interferences

Method interferences for leaching test methods are either (i) difficulties in physical handling of materials and liquid-solid separation as part of the test method, or (ii) analytical interferences observed during chemical analysis of leaching test eluates. Physical handling and liquid-solid separation difficulties will be noted based on the experience of the participant and reference laboratories. Analytical interferences will be observed based on the analytical QA/QC program (See Section 5) but are not expected based on prior experience testing similar materials.

Element 8: Matrix Suitability

Not applicable.

Element 9: Quantitation and Detection Limits

Determination of quantitation and detection limits is not a goal of this study. Quantitiation and detection limits for the chemical analysis techniques to be used in this study are provided in Section 5.

Element 10: Laboratory Reproducibility

This element is the primary focus of this study and addressed as part of this QAPP.

Element 11: Document Submission and Workgroup Evaluation

Data reduction and evaluation is specified in this QAPP. The result will be separate detailed reports documenting results for each test method. An EPA methods workgroup has been formed for these methods following the SW-846 procedures. Mark Baldwin (EPA-OSWR) is the project's liaison with the SW-846 methods workgroup.

The experimental design addresses determining within and between laboratory reproducibility for a set of four leaching test methods. An unbalanced factorial design is being used with appropriate analysis of variance statistical techniques used for data evaluation (see Section 7). Each method will be challenged using three distinctly different materials (coal fly ash, blended Portland cement mortar that includes coal fly ash, metals contaminated soil), selected to reflect a broad range of material properties. Six analytes will be selected for each material to serve as the basis for evaluation. Each analyte will be selected to represent the range of leaching behavior (e.g., concentration as a function of pH and liquid-solid ratio) typically observed for the material being evaluated and be readily detected using a single analytical method (i.e., ICO-OES). Each method is being treated as a separate evaluation from the other methods. Each material evaluated will also be treated statistically as independent evaluations because of the wide range in leaching behavior of individual constituents from material to material (these variations can span several orders of magnitude). Within the statistical design for each method evaluated, the principal factor is testing laboratory (a minimum of 6 independent laboratories and a reference laboratory). The selection of a minimum of 6 independent laboratories is consistent with ASTM recommendations (ASTM, 1988). The reference laboratory and each independent laboratory will carry out the designated test method 6 times and 3 times, respectively, on each material to determine intra-laboratory reproducibility and inter-laboratory reproducibility based on intra-laboratory and inter-laboratory variance. Individual laboratory bias will be evaluated based on deviation from the mean values observed across all laboratories and the statistical significance of the deviation. Each analyte will be treated independently for statistical analysis purposes.

The following discussion is specific to a coal fly ash as an example of the approach that will be used for preparation and evaluation of all materials selected for the study. Coal fly ash from a single facility will be the first material used in this study.

3.1 Task I: Preparing Homogenized CCR

An energy facility, which participated with EPA in an earlier study, has agreed to provide twenty-five, 5-gallon buckets of raw ash for this interlaboratory validation study. The raw ash being supplied this time is from the same facility that was included in an EPA study focused on leaching characterization of a range of CCRs, thus providing extensive useful information on approximate testing results (EPA, 2009). ICP-OES was used to analyze these samples. A list of eight metals have been selected (As, Sb, Ba, B, Ca, Cr, Co,

Mo, Se, and V) as the focus of the intercomparison study, and their method detection limits (MDL) and quantitation or reporting limits (RL) are shown in Table 3-1. From the previous work, graphs have been generated showing the pH dependent concentration of each metal.

This section details how this CCR will be homogenized, split, and tested to ensure that each participating laboratory receives like samples for analysis.

Table 3-1. MDLs and RLs of the Metals to be Evaluated during the Validation Study

Metal	MDL (µg/L)	RL (µg/L)
As	11.0	35.0
Sb	8.00	25.4
Ba	1.00	3.18
B	1.00	3.18
Ca	2.6	8.3
Cr	1.00	3.18
Co	1.00	3.18
Mo	1.2	3.8
Se	15.0	47.7
V	1.5	4.8

A core sample will be taken from 12 of the 25 homogenized buckets and tested to establish homogeneity and to provide characterization data of the CCR. A summary of this testing is shown in Table 3-2. Detailed descriptions of each testing procedure are presented in Section 5. The initial homogeneity testing will be performed using the XRF analysis as the screening technique. Total mercury by thermal decomposition using the Lumex and total digestion methods will be used to further evaluate the CCR leaching reference material. Although further homogenization occurs for each method – as detailed below – this initial core sampling and characterization testing is used to verify that the starting material (which will be used for all validation testing) is indeed homogeneous. Previous results suggest that silicon, a major constituent of this fly ash, will differ by less than 1%. Other constituents can vary by up to 25%. Wider variation between core sample results would indicate that additional homogenization between buckets would be required before proceeding.

Table 3-2. Characterization Testing to Establish Homogeneity of the CCR

Method	Analytes	Number of Replicates
XRF / solids	Total metals content (%)	Single pellet of twelve core samples
Lumex / solids	Total mercury (Hg)	Triplicate analysis of each core sample
Method 3052 / liquids	Total metals	Four cores, selected randomly
Method 3051 / liquids	Total boron (B)	Four cores, selected randomly
Method 1313 / liquids	Leaching behavior by pH	Aliquots of the four, randomly selected cores
EC/OC* / solids	Elemental and organic carbon	Twelve cores, selected randomly

* Elemental carbon/organic carbon needed for accurate XRF calculations

The percent relative standard deviation (RSD) will be calculated with an RSD<10% for major constituents and RSD<20% for trace constituents considered sufficient homogeneity for use in the study.

Each of the proposed SW846 methods will be tested with this ash as the CCR. The detailed procedure for the further homogenization (to ensure that each laboratory is receiving the exact same material for each method being tested) and distribution for testing for each method is detailed below.

Method 1313: Approximately 40 kg (two 5-gallon pails) of material will be combined into a single mixing drum, mixed and then subdivided into approximately 1-kg (1 L) subsamples. Subdivision of the mixed batch into portions will be by coring or a similar method to ensure that potential stratification of the mixed batch does not bias the individual subsamples. The result of the homogenization will be approximately forty 1-L subsamples in 1-L wide mouth HDPE containers with screw top lids. Each participating laboratory will receive two randomly-selected 1-L subsamples for the purpose of carrying out 3 replicate Method 1313 tests on the designated material. Four randomly selected 1-L subsamples will be used to conduct 6 replicate Method 1313 tests by the referee laboratory (ARCADIS). The remaining unused subsamples will be archived. For Phase I testing, the designated material is a coal fly ash.

Method 1314: Approximately 60 kg (three 5-gallon pails) of material will be combined into a single mixing drum. Each batch will be mixed and then subdivided into approximately sixty 1-kg (1-L) subsamples. Subdivision of the mixed batch into subsamples will be by coring or similar method to insure that potential mixed batch stratification does not bias the individual subsamples. This homogenization process will result in approximately sixty 1-L subsamples in 1-L wide mouth HDPE containers with screw top lids. Each participating laboratory will receive four randomly-selected 1-L subsamples for the purpose of carrying out 3 replicate Method 1314 tests on the designated material. Eight randomly selected 1-L subsamples will be used to carry out 6 replicate Method 1314 tests by the referee laboratory (Vanderbilt). The remaining unused subsamples will be archived. For Phase I testing, the designated material is a coal fly ash.

Method 1315: Approximately 100 kg (five 5-gallon pails) of material will be combined to at most two batches to be blended in mixing drum. Each batch will be mixed and then subdivided into approximately one hundred

1-kg (1-L) subsamples. Subdivision of the mixed batch into subsamples will be by coring or similar method to insure that potential mixed batch stratification does not bias the individual subsamples. This procedure will result in approximately one hundred 1-L subsamples in 1-L wide mouth HDPE containers with screw top lids. Eight randomly selected 1-L subsamples will be provided to each participating laboratory for purpose of carrying out 3 replicate Method 1315 tests on the designated material. Sixteen randomly selected 1-L subsamples will be used to carry out 6 replicate Method 1315 tests by the referee laboratory (Vanderbilt). The remaining unused subsamples will be archived. For Phase I testing, the designated material is a coal fly ash.

Method 1316: Approximately 60 kg (three 5-gallon pails) of material will be combined into a single mixing drum. Each batch will be mixed and then subdivided into approximately one hundred 1-kg (1-L) subsamples. Subdivision of the mixed batch into subsamples will be by coring or similar method to insure that potential mixed batch stratification does not bias the individual subsamples. The homogenization process will result in approximately sixty 1-L subsamples in 1-L wide mouth HDPE containers with screw top lids. Four randomly selected 1-L subsamples will be provided to each participating laboratory for purpose of carrying out 3 replicate Method 1316 tests on the designated material. Eight randomly selected 1-L subsamples will be used to carry out 6 replicate Method 1316 tests by the referee laboratory (ARCADIS). The remaining unused subsamples will be archived. For Phase I testing, the designated material is a coal fly ash.

Overall Implications: Thirteen 5-gallon buckets of coal fly ash will be used; 260 1-L wide mouth HDPE jars are needed.

Use of Spiked Samples

Spiking of field generated samples with constituents of concern is generally not recommended because of the difficulty of achieving (i) uniform distribution of the constituent spike, and (ii) speciation of the spiked constituent within reference material that is representative of the speciation of the same constituent originally present. However, spiking of a laboratory-generated reference material (e.g., cement stabilized waste form) for specific constituents of interest is practical because the added spikes will be the primary source of the constituent of interest and uniform distribution can be achieved during the slurry mixing process used to create the sample material. Any spiked samples utilized in this study will be approved by the EPA WAM and fully documented in the project report.

3.2 Task II: Leaching of the CCR by Reference Laboratory and the Intercomparison Laboratories

ARCADIS, having extensive experience in these leaching methodologies as documented in earlier studies, will be responsible for producing the reference leaching data. Six of the cores (as described in Section 3.1 for the characterization testing) will be randomly selected as the replicates to be analyzed by the reference laboratory (ARCADIS or Vanderbilt) by the proposed SW846 method. These results will be compared to the

historical data available for this ash (as described in Section 3.1) to establish the reference results for the method being validated.

Each laboratory will be provided with the following:

1. An introductory letter reiterating the purpose of this study and the laboratory's participation

2. A copy of the SW846 method being validated

3. An amount of homogenized CCR which is adequate to conduct three test replicates

4. Method template spreadsheet

5. As recommended by ORCR, each lab will be asked to have their extractions performed by a single operator on a single instrument in a single batch to minimize variability inherent to the determinative method; all leaching test eluates will be analyzed by ICP-OES for selected constituents by Vanderbilt to minimize variability associated with the metals analysis step since the focus of this study is on the leaching test methods not chemical analysis.

The spreadsheet is very user-friendly and walks the participant through each step of the method and provides a standardized mechanism for data entry into a database for this study as well as comparing results of the materials tested in this study to results obtained from other studies. Appendix B contains a printout of the pages in the Method 1313 spreadsheet showing the instructions and each of the data entry sheets. Appendix C contains examples of the introductory letter, instruction sheet, questionnaires for Methods 1313 and 1316, chain-of-custody form, and a page of sample labels sent to each participating laboratory.

Each laboratory will be asked to perform the each of the four proposed methods in triplicate (e.g., 9 pH levels + 3 blanks per test = 36 leachates for Method 1313) within one month. The leachates are to be forwarded to Vanderbilt for analysis. In addition, they are to forward the completed data package to the EPA WAM and Vanderbilt, which will include:

- The completed electronic data report forms (provided as Microsoft® Excel spreadsheets)

- Photocopies or printouts of all raw data, laboratory notebook documentation, calculations, results and comments

- A completed questionnaire indicating any deviations from the prescribed method that were necessary, methodology clarifications needed or suggested, personnel time required to complete the method, and any other suggestions.

The tentative schedule for the interlaboratory validation of the method is shown in Table 3-3.

Table 3-3. Tentative Schedule for Interlaboratory Validation of Proposed SW-846 Methods

Milestone	Tentative Date
Receive ash from previously participating facility	Complete in 2010
Initial characterization and baseline testing	Completed in 2010
Lab's receive material for testing	Completed in 2010 and 2011
Labs send leachates to Vanderbilt for analysis	November 2011
Vanderbilt provides results to EPA	December 2011
Provide final reports for the methods testing	January 2012

3.3 Task III: Determination of the Reproducibility of Each Method

Following receipt of the completed data packages from each participating laboratory and the results of the leachate analyses from Vanderbilt, statistical determination of the reproducibility (variability between laboratories) and repeatability (single-operator precision) of each method will be determined. Leach testing results and feedback will be compiled with like data from other laboratories performing the same method, and will be submitted as part of a supportive data package for EPA ORCR method approval.

3.4 Task IV: Testing of Select Materials for Leaching by SW-846 Methods 1311 (TCLP) and 1312 (SPLP)

Testing of some selected CCRs and the materials from the interlaboratory methods validation study will be performed by ARCADIS using SW-846 Methods 1311 "Toxicity Characteristic Leaching Procedure (TCLP)" and 1312 "Synthetic Precipitation Leaching Procedure (SPLP)" for comparison with the proposed new SW-846 methods. Leachate will be sent to Vanderbilt for analysis by ICP-OES. Results from these experiments will be used to show the comparability of leaching behavior between these tests and the proposed new SW-846 methods. TCLP uses a glacial acetic acid and sodium hydroxide buffer solution with a pH of 4.93 ± 0.05 (Extraction Fluid #1) at a 20 to 1 solid to liquid ratio. SPLP uses a weak sulfuric and nitric acid solution with a pH of 4.2 ± 0.05 (Extraction Fluid #1) at a 20 to 1 liquid to solid ratio to simulate leaching for samples east of the Mississippi river. Samples will be tumbled for 18 hours and filtered to remove the solids. The extract will be preserved with 1% nitric acid and analyzed by Vanderbilt University using ICP-OES. Table 3-4 lists the samples currently selected for TCLP and SPLP testing.

Table 3-4. Sample Testing List for TCLP and SPLP

Sample Name	Sample Type
CaFA	Fly Ash
EaFA	Fly Ash
KFA	Fly Ash
UFA	Fly Ash
ZFA	Fly Ash
YSD	Spray Dryer Ash
MAD	FGD + Fly Ash Mix
DGD	Scrubber Sludge
CKD	Scrubber Sludge
SWA	Solid Waste Analog
CFS	Contaminated Field Soil
JaFS	Brass Foundry Sands
CKD	Cement Kiln Dust

3.5 Task V: Testing of Fly Ashes and Cement Kiln Dust for Radionuclide Testing by Germanium Detector

Vanderbilt will perform radionuclide testing on 35 fly ash samples and 1 cement kiln dust sample to determine uranium species and concentrations by the measurement of Beta and Gamma decay particles using a Germanium (Ge) detector made by ???.

4. Sampling Procedures

The following subsections describe the sampling procedures to be used for each task. Whenever possible, standard methods will be followed. In some cases, draft methods may be evaluated and implemented. Each method to be used will be cited and any deviations from the methods will be documented.

4.1 Sample Custody Procedures

The detailed procedures for preparing and distributing the homogenized CCR were presented in Section 3.1. The following types of samples will be generated during these tests:

1. Solid samples for leaching and radionuclide testing: fly ash, solid waste analog, contaminated field soil, brass foundry sands, scrubber sludge, and cement kiln dust

2. Post –leaching and post-thermal desorption of the CCR (solid samples)

3. Leachate samples (liquid samples) for Hg and other metals analysis

Each sample generated will be analyzed in-house or by outside laboratories. Chain-of-custody (COC) procedures will be required, which will include signing and dating of COCs to indicate receipt of samples, and archived of all COCs with other project documentation. CCRs will be logged as they are received by the ARCADIS WAL, Mr. Peter Kariher. Information regarding where each CCR originated and any other descriptive information available will be recorded in a dedicated laboratory notebook by Mr. Kariher. A core sample will be taken from each 5-gallon bucket of homogenized material and processed for physical and chemical characterization (see Section 3.1). All samples will be properly contained and identified with a unique sample ID and sample label. Chain-of-custody forms will be generated for all samples prior to transfer for analysis.

The sample labeling convention used to identify a particular solution consists of numerical identifiers for the material, lab, test method, and test position along with an alphabetical identifier for the test replicate. The layout for the sample label convention is as follows:

M*aa*-**L***bb*-**131***c*-**T***dd*-*e* (Test Positions T01 through T09)

M*aa*-**L***bb*-**131***c*-**B***dd*-*e* (QA/QC Blanks B01-B03)

"aa" is a two-digit number starting at zero that identifies the test material (e.g., the Phase I material is M01),

"bb" is a two-digit number starting at zero that identifies the participating laboratory (assigned randomly by EPA-ORCR),

"c" is a single digit number that completes the test method ID (i.e., 1313, 1314, 1315, 1316, TCLP, or SPLP),

"dd" is a two-digit number starting at zero that identifies the test position or QA/QC blank.

"e" is a single letter representing the test replicate (i.e., A, B or C).

Four sets of completed labels were provided to be used for labeling extraction vessels (for the tree replicates and a fourth set for replacements as needed) and two sets of 50-mL analytical samples.

For example. **M01-L02-1313-B02-C** would represent Phase I material being validated by the laboratory randomly identified as "02". The sample is from Method 1313, is blank 02, and replicate C.

Handling of CCR samples for the leaching tests (Task III) is described in detail in each of the proposed SW846 methods. These methods can be found on the Vanderbilt University website at http://www.vanderbilt.edu/leaching/downloads.html.

4.2 CCR, and Leaching Reference Material Samples

As mentioned, the objective of this validation study is to obtain information on the reproducibility of the preliminary versions of EPA methods for leaching Al, Sb, Ba, B, Cr, Co, Mg, and Zn from CCRs. The facility descriptions will include information on the history/origin of each method validation sample, facility process description, sample type, sampling location, sampling time and method, coal type, operating condition, and sample storage condition. Section 4.1 describes the sampling custody procedure.

4.2.1 Physical and Chemical Characterization Samples

A core sample will be taken from twelve of the 5-gallon buckets of the homogenized method validation material (as described in Section 3.1) and subjected to physical characterization measurements. These 12 core samples will be mixed together using a riffle splitter prior to XRF pellet preparation and analysis. To ensure a good homogeneity of the final composite sample that will be used for the XRF characterization, the first two composite samples exiting the splitter will be reintroduced at the top of the splitter. This procedure will be repeated at least 6 times. At the end, the two resulting homogeneous composite samples will be combined in the same sample container and stored until XRF testing. Method 3052 samples will also be performed on each of the method validation materials to determine variability for trace elements.

4.2.2 Leaching Study Samples

Method validation materials used for leaching studies will not require size reduction to acquire an adequate sample for testing due to the small particle size inherent in fly ash. The size reduction method is outlined in the leaching test methods (http://www.vanderbilt.edu/leaching/downloads.html). If the method validation materials are altered in any way prior to leaching studies, a representative sample will be submitted for physical and chemical characterization.

4.3 Leachate Collection

Each of the proposed SW-846 test methods will be used to conduct a leaching study. The proposed methods can be found on the Vanderbilt University website at http://www.vanderbilt.edu/leaching/downloads.html. Table 4-1 shows the extraction schedule and the range of tested pHs as outlined in the first study to be conducted on the *Preliminary Version of EPA Method 1313: Liquid-Solid Partitioning as a Function of Extract pH for Constituents in Solid Materials using a Parallel Batch Extraction Procedure*.

Table 4-1. Final Extract pH Targets for Method 1313

pH Target	Rationale
Will Vary*	Natural pH at LS 10 mL/g-dry (no acid/base addition)
2.0±0.5	Provides estimates of total or available COPC content
4.0±0.5	Lower pH limit of typical management scenario
5.5±0.5	Typical lower range of industrial waste landfills
7.0±0.5	Neutral pH region; high release of oxyanions
8.0±0.5	Endpoint pH of carbonated alkaline materials
9.0±0.5	Minimum of LSP curve for many cationic and amphoteric COPCs
12.0±0.5	Maximum in alkaline range for LSP curves of amphoteric COPCs
13.0±0.5	Upper bound (field conditions) for amphoteric COPCs
10.5±0.5	Substitution if natural pH falls within range of a mandatory target

*This is the pH of the material as received with only deionized water added (i.e., no acid or base addition).

Table 4-2 shows an example schedule for the extraction setup to be conducted on the *Preliminary Version of EPA Method 1316: Liquid-Solid Partitioning as a Function of Liquid-Solid Ratio for Constituents in Solid Materials using a Parallel Batch Extraction Procedure*.

Table 4-2. Example Schedule for Method 1316 Extraction Setup

A	B	C	D	E	F	G
Test Position	Target LS	Minimum Dry Mass (g-dry)	Mass of "As-Tested" Sample (g)	Moisture in "As-Tested" Sample (mL)	Volume of Reagent Water (mL)	Recommended Bottle Size (mL)
T01	10.0	20	22.2	2.2	198	250
T02	5.0	40	44.4	4.4	196	250
T03	2.0	100	111	11.1	189	500
T04	1.0	200	222	22.2	178	500
T05	0.5	400	444	44.4	156	1000
B01	QC	–			200	250
Total		–	844		1120	

NOTE: 1) This schedule assumes a target liquid volume of 200 mL.
2) This schedule is based on “as tested” solids content of 0.90 g-dry/g.
3) Test position marked B01 is a method blank of reagent water.

To demonstrate the versatility and robustness of the proposed new leach test methods, various solid materials other than CCRs were chosen for testing. Table 4-3 shows the proposed test methods and each of the materials to be tested. Table 4-4 gives a brief description of the various solid materials to be tested.

Table 4-3. Materials to be used with the Proposed New Leach Tests

Method	Materials
1313	Fly Ash (EaFA), CFS (Contaminated Field Soil), and SWA (Solid Waste Analog)
1314	CFS (Contaminated Field Soil) and JaFS (Brass Foundry Sands)
1315	SWA (Solid Waste Analog) and CFS (Contaminated Field Soil)
1316	Fly Ash (EaFA), CFS (Contaminated Field Soil), and SWA (Solid Waste Analog)

Table 4-3. Description of Materials for the Proposed New Leach Testing

Material	Description
EaFA	Fly ash from a 2.4 G Watt power plant burning eastern-bituminous coal
CFS	Contaminated field soil collected from an active copper and lead smelting site
SWA	Solid waste analog material containing Type I portland cement, class C coal combustion fly ash, and ground granulated blast furnace slag) and wastewater at a water/binder ratio of 0.41 (m/g). The wastewater used was tap water spiked with powdered metal oxides or metal nitrates of antimony, arsenic, barium, chromium, lead and selenium. This combined material was used to produce both solid monoliths and ground for 2-mm power
1316	Fly Ash (EaFA), CFS (Contaminated Field Soil), and SWA (Solid Waste Analog)
1316	Fly Ash (EaFA), CFS (Contaminated Field Soil), and SWA (Solid Waste Analog)

5. Testing and Measurement Protocols to be Used for Reference Material Characterization and Eluate Characterization

As part of the initial characterization of the raw fly ash CCR, ARCADIS will conduct physical and chemical characterization analyses. In addition, total metals will be analyzed by Test America, and the metals in the leaching extracts will be analyzed by Vanderbilt University. Whenever possible, standard methods will be used to perform required measurements. Standard methods are cited in each applicable section. Where standard methods are not available, operating procedures will be written to describe activities. In situations where method development is ongoing, activities and method changes will be thoroughly documented in dedicated laboratory notebooks.

5.1 Physical Characterization

5.1.1 pH and Conductivity

pH and conductivity will be measured on all aqueous extracts by the laboratory (reference and participant laboratories) carrying out the leaching test method. Conductivity is a measure of the ability of an aqueous solution to carry an electric current. This ability is dependent upon the presence of ions; on their total concentration, mobility, and variance; and on the temperature of the measurement.

pH of the leachates will be measured by using a combined pH electrode. A 3-point calibration will be done using National Institute of Science and Technology (NIST) traceable pH buffer solutions. The pH meter will be accurate and reproducible to 0.1 pH units with a range of 0 to 14.

Conductivity of the leachates will be measured using a standard conductivity probe. The conductivity probe will be calibrated using appropriate standard conductivity solutions for the conductivity range of concern. Conductivity meters are typically accurate to ±1% and have a precision of ±1%. The procedure to measure pH and conductivity will be as follows:

Following a gross separation of the solid and liquid phases by centrifugation or settling, a minimum volume of the supernatant to measure the solution pH and conductivity will be taken and poured in a test tube. The remaining liquid will be separated by pressure filtration and filtrates will be appropriately labeled, preserved, and stored for subsequent chemical analysis.

5.1.2 Moisture Content and Loss on Ignition (LOI)

Moisture content of the raw fly ash CCR will be determined using ASTM D 2216-05 (ASTM 2005) by ARCADIS. This method, however, is not applicable to the materials containing gypsum (calcium sulfate dihydrate or other compounds having significant amounts of hydrated water), since this material slowly

dehydrates at the standard drying temperature (110°C). This slow dehydration results in the formation of another compound (calcium sulfate hemihydrate) which is not normally present in natural material. The ASTM method allows cooling at 60 °C to prevent the conversion and will be used to determine the moisture content of materials containing gypsum.

Loss on ignition (LOI) will be performed on the raw fly ash CCR by placing dried samples in a furnace at 750 °C for 1 hour and measuring the mass lost during the combustion using ASTM D7348-08 (ASTM 2008).

5.2 Chemical Characterization

5.2.1 Dissolved Organic Carbon / Dissolved Inorganic Carbon (DOC/DIC) and Elemental Carbon / Organic Carbon (EC/OC)

Analyses of total dissolved organic carbon (DOC) and dissolved inorganic carbon (DIC) will be performed on the leachates as part of the baseline characterization by Vanderbilt University on a Shimadzu model TOC-V CPH/CPN combustion catalytic oxidation NDIR analyzer. Five-point calibration curves, for both inorganic (IC) and non-purgeable organic carbon (NPOC) analyses, are generated for an analytical range between 5 ppm and 100 ppm and are accepted with a correlation coefficient of at least 0.995. Reagent grade potassium hydrogen phthalate is used as the NPOC standard and sodium hydrogen carbonate is used as the IC standard. An analytical blank and check standard at approximately 10 ppm are run every 10 samples. The standard is required to be within 15% of the specified value. A new calibration curve is generated if the check standard measurement does not meet specification. A volume of approximately 16 mL of undiluted sample is loaded for analysis. Inorganic carbon analysis is performed first for the analytical blank and standard and then the samples. Total carbon (non-purgeable organic carbon) analysis follows with addition of 2M hydrochloric acid to a pH of 2 and a sparge gas flow rate of 50 mL/min. Method detection limit (MDL) and minimum level of quantification (MLQ) are shown in Table 5-1.

Table 5-1. MDL and MLQ of Total Organic Carbon Analyzer

	MDL (ppm)	MLQ (ppm)
IC	0.07	0.20
NPOC	0.09	0.20

Elemental carbon (EC) and organic carbon (OC) will be determined on the solids by ARCADIS using a Sunset Laboratory Carbon Aerosol Analysis Lab Instrument in EPA RTP Laboratory E-581A. This method is defined in NIOSH Method 5040 (CDC 2003). This equipment uses a furnace to heat the sample and combust the carbon to carbon dioxide. The carbon dioxide is reduced to methane and a FID is used to quantify the carbon emitted as the sample is heated from ambient to 870 °C over four heating steps.

Samples are prepared by weighing 3 grams of the CCR into a 500 mL Nalgene high-density polyethylene bottle. A 37 mm tarred pre-baked quartz filter is loaded into a 2.5 µm particulate sampler and attached to the bottle. The particulate sampler is connected to a vacuum source and a rotometer to control the flow at 4 liters per minute. The CCR material is aspirated onto the quartz filter for 5 minutes and the filter is reweighed to determine the mass loading. Duplicate filters are prepared for each material. Three analyses are performed on each filter. Blank filters are provided to determine background levels.

5.2.2 Mercury by Thermal Decomposition and Cold Vapor Atomic Adsorption (TD-CVAA) Method 7473

As part of the baseline characterization, mercury analysis of the solid materials will be carried out by ARCADIS using a thermal decomposition cold vapor atomic adsorption (TC/CVAA) according the EPA SW-846 Method 7473 (EPA 1998).

The Lumex RA-915+ Mercury Analyzer is a portable instrument capable of measuring mercury concentrations in air, liquids, and solids. Developed for use by the Russian Navy to detect elemental mercury leaks on submarines (mercury is used as ballast), the analyzer is capable of measuring 1 ng/m3. The instrument contains an internal sample pump, multi-pass optical cell and Zeeman Effect atomic adsorption detector tuned to a wavelength of 253.7 nm for the detection of mercury. The Zeeman effect atomic adsorption (AA) detector modulates the frequency of the source to eliminate matrix effects from air samples and enhance the detector sensitivity for mercury. An optional RP-91C high temperature (>750 °C) furnace can be used to convert any mercury species to elemental mercury for post combustion detection of total mercury in the solids. Since the detector can only measure elemental mercury directly, this technique is based on the thermal decomposition properties of mercury, as only elemental mercury can exist at these high temperatures. Under high temperatures, any oxidized mercury compounds are converted to elemental mercury.

To perform a mercury analysis on a solid sample, the solid of known mass is weighed into a quartz or stainless steel combustion boat. The combustion boat is then inserted into the furnace combustion chamber and as the elemental mercury is evolved from the sample, the detector measures the mass of mercury. The mass of mercury is directly proportional to the area under the peak, similar to the quantitation principle used in gas chromatography. By dividing the mass of mercury by the mass of sample introduced to the instrument, a mercury concentration can be derived. For wet samples, a moisture measurement of the solid must be determined to correct the mercury content to a dry basis.

5.2.3 Other Metals (ICP)

Test America Laboratories in Savannah, GA, will analyze a sample of the raw fly ash for the metal species total content using an Agilent ICP-MS with octopole reaction system (ORS). Vanderbilt University

(Department of Civil and Environmental Engineering) will analyze the metals content of the leachates using a Varian inductively couple plasma optical emission spectroscopy (ICP-OES).

Test America will conduct their total metal analyzes on an ICP-MS using EPA SW-846 Method 6020A (EPA 2007d). Metals and estimated instrument detection limits are listed in the method. The ICP will be profiled and calibrated for the target compounds and specific instrument detection limits will be determined. Mixed calibration standards will be prepared at least 5 levels. Each target compound will also be analyzed separately to determine possible spectral interference or the presence of impurities. Two types of blanks will be run with each batch of samples. A calibration blank is used to establish the analytical curve and the method blank is used to identify possible contamination from varying amounts of the acids used in the sample processing. Additional daily QC checks include an Initial Calibration Verification (ICV) and a Continuing Calibration Verification (CCV). The ICV is prepared by combining target elements from a standard source different than that of the calibration standard and at a concentration within the linear working range of the instrument. The CCV is prepared in the same acid matrix using the same standards used for calibration at a concentration near the mid-point of the calibration curve. A calibration blank and a CCV or ICV are analyzed after every tenth sample and at the end of each batch of samples. The CCV and ICV results must verify that the instrument is within 10% of the initial calibration with an RSD < 5% from replicate integrations. Procedures to incorporate the analysis of a MS/MSD for these CCR samples will be evaluated.

Vanderbilt University (Department of Civil and Environmental Engineering) will also conduct ICP-MS analyses on the reference laboratory leaching test eluates. This will provide a statistical assessment of precision for constituents that are not analyzed for in eluates by the participant laboratories. This will provide precision (intralaboratory, by ICP-MS and ICP-OES) for all elements of concern and reproducibility (interlaboratory, by ICP-OES) for a representative set of constituents. Inferences may be possible concerning the interlaboratory reproducibility for other elements, depending on the relative contributions to variance, between intralaboratory and interlaboratory effects.

A Perkin Elmer model ELAN DRC II will be used in both standard and dynamic reaction chamber (DRC) modes. Standard analysis mode will be used for all analytes except for As and Se, which will be run in DRC mode with 0.5 mL/min of oxygen as the reaction gas. Seven-point standard curves will be used for an analytical range between approximately 0.5 µg/L and 500 µg/L and completed before each analysis. Analytical blanks and analytical check standards at approximately 50 µg/L will be run every 10 to 20 samples and are required to be within 15% of the specified value. Samples for analysis will be diluted gravimetrically to within the targeted analytical range using 1% v/v Optima grade nitric acid (Fisher Scientific). Initially, analyses for 10:1 dilutions will be performed to minimize total dissolved loading to the instrument. Additional dilutions at 100:1 and 1000:1 will be analyzed if the calibration range is exceeded with the 10:1 dilution. 50 µL of a 10 mg/L internal standard consisting of indium (In) (for mass range below 150) and bismuth (Bi) (for mass range over 150) will be added to 10 mL of sample aliquot prior to analysis.

Analytical matrix spikes will be completed for one of each of the replicate eluates from Method 1313. For each analytical matrix spike, a volume between 10 µL and 100 µL of a 10 mg/L standard solution will be added to 10 mL of sample aliquot.

ICP-OES Analyses

ICP-OES analyses of aqueous samples from laboratory leaching tests will be carried out at Vanderbilt University (Department of Civil and Environmental Engineering) using a Varian ICP Model 720-ES. Five-point standard curves will be used for an analytical range between approximately 0.1 mg/L and 25 mg/L for trace metals. Seven-point standard curves will be used for an analytical range between approximately 0.1 mg/L and 500 mg/L for minerals. Analytical blanks and analytical check standards at approximately 0.5 mg/L will be run every 10 to 20 samples and are required to be within 15% of the specified value. Initially, analyses will be performed on undiluted samples to minimize total dissolved loading to the instrument. Samples for analysis will be diluted gravimetrically to within the targeted analytical range using 1% v/v Optima grade nitric acid (Fisher Scientific) if the maximum calibration is exceeded. Yttrium at 10 mg/L will be used as the internal standard. Analytical matrix spikes will be completed for three test positions from one of the replicate eluates from Method 1313. For each analytical matrix spike, a volume of 500 µL of a 10 mg/L standard solution will be added to 5 mL of sample aliquot.

Table 5-2 provides the element analyzed, method detection limit (MDL), and minimum level of quantification (ML). Analyte concentrations measured that are less than the ML and greater than the MDL are reported as estimated value using the instrument response.

Table 5-2. Method Detection Limits (MDLs) and Minimum Level of Quantification (ML) for ICP-OES Analysis on Liquid Samples*

Symbol	Units	MDL	ML
Al	µg/L	1.00	3.18
Sb	µg/L	8.00	25.4
As	µg/L	15.0	47.7
Ba	µg/L	1.00	3.18
Be	µg/L	5.00	15.9
B	µg/L	1.00	3.18
Cd	µg/L	6.00	19.1
Ca	µg/L	3.50	11.1
Cr	µg/L	1.00	3.18
Co	µg/L	1.00	3.18
Cu	µg/L	4.1	13.0
Fe	µg/L	2.90	9.22
Pb	µg/L	7.00	22.3
Li	µg/L	6.00	19.1
Mg	µg/L	1.00	3.18
Mn	µg/L	3.60	11.4
Mo	µg/L	1.00	3.18
Ni	µg/L	2.20	7.00
K	µg/L	1.50	4.77
P	µg/L	6.2	19.7
Se	µg/L	17.0	54.1
Si	µg/L	2.80	8.90
Ag	µg/L	18.00	57.2
Na	µg/L	3.50	11.1
Sr	µg/L	1.00	3.18
S	µg/L	8.30	26.4
Tl	µg/L	5.00	15.9
Sn	µg/L	17.0	54.1
Ti	µg/L	6.40	20.3
V	µg/L	1.30	4.13
Zn	µg/L	2.50	7.95
Zr	µg/L	2.70	8.59

* All elements indicated in Table 5.2 will be analyzed, however, only elements indicated in bold are reported as part of the leaching studies.

5.2.4 X-Ray Fluorescence (XRF)

X-Ray Fluorescence Spectrometry is used in the USEPA RTP, NC laboratories to analyze a sample of the raw fly ash for the determination of total content for the major elements. A Philips model PW 2404 wavelength dispersive instrument, equipped with a PW 2540 VRC sample changer, is used for these analyses. The manufacturer's software suite, "SuperQ", is used to operate the instrument, collect the data, and perform quantification.

The instrument was calibrated using a manufacturer-supplied set of calibration standards at the time of installation of the software plus a new X-ray tube. On a monthly basis, manufacturer-supplied drift correction standards are used to create an updated drift correction factor for each potential analytical line. On a monthly basis, a dedicated suite of QC samples are analyzed before and after the drift correction procedure. This data is used to update and maintain the instrument's QC charts. The SOP for this QC procedure (SOP No. 5003.3; "Procedure for the Philips PW 2404 XRF Monthly Drift Correction, Quality Control Stability Check, QC Chart Update, and Database Backup.") is maintained in a 3-ring binder located at the control module for the spectrometer, along with all other operational SOPs. Any deviations from these QC parameters will be documented to the EPA WAM.

The software suite's "Measure and Analyze" program collects and stores the sample data. This program has two basic modes of operation, "scan" and "channels". The scan mode is used to collect the bulk of the data. It operates in a stepwise scanning mode and uses the manufacturer supplied "IQ+" program to define operating parameters. IQ+ scans the available wavelength range using a series of 10 sub-scans that vary in terms of detector, radiant power, collimator crystal, and wavelength. While the instrument incorporates a sample rotation capability, this is not used by IQ+ since the time spent at any one wavelength is only a fraction of the pellet rotation time.

The channel mode is typically reserved for trace work. In this mode, the instrument moves to a specific wavelength and goniometer position and collects data for defined periods of time. These data collection periods are typically long enough to make use of the sample rotation function worth while. Other instrument operation parameters, such as tube power and crystal, are taken from the scan function parameters. The data collected in the channel mode is then incorporated into the sample's data file. The intent is to improve detection limits for certain trace elements that are often of interest at a small cost in analytical time.

Quantification is performed post-data collection using the program, "IQ+". IQ+ is a "first principles" quantification program that includes complex calculations to account for a wide variety of sample-specific parameters. For this reason, sample-specific calibrations are not necessary. This program calculates both peak heights and baseline values. The difference is then used, after adjustment by drift correction factors, for elemental quantification versus the calibration data. Interelement effects are possible and the software includes a library of such parameters. Data from secondary lines may be used for quantification where

interelement effects are significant or the primary peak is overloading the DAQ. Where the difference between the calculated peak height and baseline are of low quality, the program will not identify a peak and will not report results. IQ+ permits the inclusion of data from other sources by manual entry. Carbon is an example of this for these samples. Entry of other source data for elements indeterminable by XRF improves the mass balance.

5.2.5 XRF Detection Limits

Table 5-3 presents detection limit data in two forms, which are not mutually exclusive. The reporting limit is built into the software and reflects the manufacturer's willingness to report low-level data. Data listed under "detection limit" are based upon the short-term reproducibility of replicate analyses and are sample matrix specific. These calculations are likely to report higher detection limits for macro elements than what would be calculated where the same element is present at trace levels. In this data set, calcium is a likely example of this.

Table 5-3. XRF Reporting and Detection Limits

Analyte	Reporting Limit, µg/g	Detection Limit %, 2σ (wt. %)
Al	20	0.016
As	20	0.038
Ba	20	0.0084
Br	20	0.02
Ca	20	0.1
Cd	20	0.064
Ce	20	0.022
Cl	20	0.0046
Co	20	0.0024
Cr	20	0.0028
Cu	20	0.0014
F	20	0.082
Fe	20	0.034
Ga	20	0.0016
Ge	20	0.0014
K	20	0.0048
La	20	0.0054
Mg	20	0.01
Mn	20	0.0032
Mo	20	0.0026
Na	20	0.0076
Nb	20	0.0018
Ni	20	0.0048
Pb	20	0.0034
Px	20	0.004
Rb	20	0.0016
Sc	20	0.0016
Se	20	0.0018
Si	20	0.092
Sr	20	0.0016
Sx	20	0.05
Ti	20	0.003
V	20	0.0038
W	20	0.0036
Y	20	0.0018
Zn	20	0.0014
Zr	20	0.0024

5.2.6 Radionuclide Testing of CCRs using Ge-Detector

Fly ash, gypsum, and other CCRs were collected and assessed to determine their specific activity [Bq/kg]. Samples were taken from a variety of different sources to compare trends in radioactivity, such as that of bituminous and sub-bituminous CCRs. Samples will be analyzed using two High Purity Germanium (HPGe) photon detector with low energy detection capabilities, in a common geometry.

Detector 1: Ortec model GMX35P4 high purity germanium coaxial detector, 55.6 mm diameter, 79 mm length, 0.5 mm beryllium window, rated resolution 2.1 keV at 1332 keV, 31.5% relative efficiency at 1332 keV, GammaVision version 6.01 analytical software, 2003.

Detector 2: Canberra model BE3830 high purity germanium coaxial detector, 70 mm diameter, 30 mm length, 0.6 mm beryllium window, rated resolution 1.6 keV at 1332 keV, 27.9% relative efficiency at 1332 keV, Genie 2000 version 32.1 analytical software, 2009.

Project samples of fly ash and other coal combustion residues are received as dry materials and will be placed in plastic vials of approximately 250 ml and sealed to allow ingrowth of radon gas into equilibrium with its parent nuclide, as peaks from the radon progeny are key to identification of the parent nuclide. Sample containers are placed on the coaxial germanium photon detector systems and counted with shields closed. Traceable calibration standards in the same geometry had previously been counted on these systems to establish system calibrations. Samples are counted for times determined to be adequate to attain reasonable Minimum Detectable Activity (MDA) levels, 8 hours for fly ash and 12 hours for other residues. Results are given as values of activity per unit mass of sample, with associated uncertainties and MDA values. As MDAs are derived by pre-established regions on the gamma spectroscopy spectra which varies sample by sample, MDAs for a given nuclide on a particular system are slightly different for each sample but are generally consistent on a given detector for a stated geometry and count time. Fly ash samples are counted for 8 hrs, while all other samples are counted for 12 hr periods. The background characteristics of a number of photopeaks essential to the detection of U-238 and Th-232 decay series were determined over several weeks, and MDA levels were determined for each of the relevant regions.

The following photopeaks are used to determine activity in the U-238 decay series:

186 keV (Ra-226)
295 keV (Pb-214)
352 keV (Pb-214)
609 keV (Bi-214)
1754 keV (Bi-214)

The following photopeaks are used to determine activity in the Th-232 decay series:

583 keV (Tl-208)

911 keV (Ac-228)

Other photopeaks are evaluated regularly as naturally occurring peaks:

511 keV (various)
662 keV (Cs-137)
1460 keV (K-40)

6. Quality Assurance/Quality Control

6.1 Data Quality Indicator Goals

Data quality indicator (DQI) goals for critical measurements in terms of accuracy, precision and completeness are shown in Table 6-1. In addition, critical data quality indicator goals are inclusion of at least 6 independent laboratories in addition to the referee laboratory and 3 materials for each leaching test method evaluated.

These goals are based on past performance and will be assessed as the project is completed. Any deviations from these stated DQIs will be documented to the EPA WAM.

Table 6-1. Data Quality Indicator Goals

Measurement	Method	Accuracy	Precision	Completeness
ICP-OES constituents (e.g., As, B, Ba, Ca, Co, Cr, Mo, Sb, Se, V) Concentration	ICP-OES	±10%	±10%	>90%
pH, conductivity	Electrode	±2%	±2%	100%
Moisture	ASTM D2216-05	NA	±10%	100%
Hg	7470	±10%	±10%	90%
XRF	SOP No. 5003.3	±2%	±10%	100%
ICP/MS	6020	±10%	±10%	90%

NA = not applicable.

For the ICP-OES, accuracy is assessed using calibration verifications and laboratory control samples. Precision is assessed by replicate measurements. For the pH measurements, a standard of known pH will be checked prior to taking sample measurements. Precision is assessed by replicate measurements. There is not a standard reference material for moisture accuracy. Precision will again be assessed by replicate measurements.

In addition to the DQI goals shown in Table 6-1, homogeneity of the reference material will be considered acceptable if the following criteria are met by XRF. Major constituents are elements found at concentrations of more than 1%.

- RSD<10% for major constituents (greater than 1% total content)
- RSD<20% for minor constituents (greater than 0.1 to 1% total content)

- RSD<50% for trace constituents (less than 0.1 % total content.

Accuracy will be determined by calculating the percent bias from a known standard. Precision will be calculated as relative percent difference (RPD) between duplicate values and relative standard deviation (RSD) for parameters that have more than two replicates. Completeness is defined as the percentage of measurements that meet DQI goals of the total number measurements taken.

6.2 QC Sample Types

Types of QC samples used in this project will include blanks, spiked samples, replicates, and mass balance tests on the leaching reference material. For physical characterization testing, duplicate samples of the CCR, leaching reference material will be processed through each analysis. The initial criteria will be determined on the screening data (the six replicates conducted by the ARCADIS referee laboratory) through a statistical review. This is done by looking at the leaching curves and bounding the data by the 5^{th} and 95^{th} percentiles as predicted by linear interpolations. The individual criteria will be determined by OCRC, ORD, Vanderbilt, and ARCADIS when they conduct this same statistical review on the data collected by each laboratory.. As recommended by ORCR, each lab will be asked to have their extractions performed by a single operator on a single instrument in a single batch to minimize variability inherent to the determinative method; all leaching test eluates will be analyzed by ICP-OES for selected constituents by Vanderbilt to minimize variability associated with the metals analysis step since the focus of this study is on the leaching test methods not chemical analysis.

The EPA Metrology laboratory completes periodic and requested calibrations as described in SOPs and standard methods for equipment such as balances.

7. Data Reduction, Validation, and Reporting

7.1 Data Analysis

Interlaboratory comparisons of each method and material will be based on sets of analytes that are (i) representative of the range of characteristic behaviors anticipated for the material being tested and the test method being evaluated, and (ii) either analyzed as part of the laboratory procedure (e.g., pH) or analyzed as part of a single ICP-OES analytical method. Thus, it is anticipated that although some analytes will be common amongst different test materials being used in the interlaboratory comparisons, the complete set of analytes will likely be different for each test material because of different characteristic behaviors (e.g., as a function of pH and LS) and leaching concentrations relative to analytical detection limits. At least 6 analytes will be used as the basis for evaluation for each test material with priority given to analytes that are of regulatory interest and those that are major constituents of each test material. An initial set of analytes for each test material will be selected based on prior knowledge of the type of each test material selected (e.g., coal fly ash, cement stabilized waste, blast furnace slag). The final set of analytes for each test material will be selected based on the test method results obtained by the referee laboratory with the concurrence of the project team, including the EPA QA Representative, and prior to beginning analysis of samples from the participant laboratories.

The basis of the interlaboratory comparisons will be the dependent variables that are intended to be the information derived from each test procedure using the set of constituents selected for the test material being tested. The set of dependent variables for each test method are specified in the sub-sections that follow. The variance of the following additional analytes will be evaluated as reported by the referee laboratory and each participant laboratory to provide insights into material variability and methods implementation: moisture content, eluate pH, eluate conductivity.

Method 1313

The primary information to be derived from this test method is (i) the pH dependent leaching behavior of constituents of interest, and (ii) the pH titration curve of the material. The dependent variables that will serve as the basis for evaluation will be (i) material natural pH (as defined in the test method), (ii) eluate analyte concentration as determined for the method target pH values (i.e., 2.0, 4.0, 5.5, 7.0, 8.0, 9.0, 12.0, 13.0, natural pH, 10.5), and (iii) equivalents of acid or base required to be added to achieve the method target pH values (i.e., the pH titration curve). Variation in the actual pH about the target pH value of each eluate but within the tolerances specified in the test method will require interpolation or extrapolation of measured analyte concentration values to the precise target value. The initial method will be linear interpolation of the analyte concentration to the target pH value based on the log transform of the analyte concentration from the eluates having the nearest pH value greater than and less than the target value. If this method is found to provide poor representation of the overall pH dependent behavior of the analyte, then other interpolation

methods such as cubic splines or fifth-order polynomial fitting will be considered. The decision on the interpolation method will be based on the results obtained from the referee laboratory, prior to initiating evaluation of data from the participant laboratories. The same approach will be used for interpolation required to determine the equivalents of acid or base needed to be added to obtain the target eluate pH values. An ANOVA statistical evaluation (see below for ANOVA specification) will be used to evaluate the contributions to variance and method precision for the discrete values of the dependent variables at each target value of the appropriate independent variable.

An alternate method of data interpretation of the dependent variables will be based on the functional relationship of the dependent variable to the specified independent variable (i.e., analyte concentration as a function of pH or eluate pH as a function of acid or base addition). Thus, potential functional relationships (e.g., fifth order polynomials) will be regressed to the data set to provide a defined function to represent the overall result for each analyte. The contributions to variance in the resulting function then would serve as the basis for evaluating the method precision (see below for specification of statistical analysis of functional relationships).

Method 1314

The primary information to be derived from this test method is (i) the eluate pH and analyte concentration as a function of LS, and (ii) the cumulative release (i.e., mg of analyte per kg of material leached) of each analyte as a function of LS. The analyte concentration measured for eluates obtained at cumulative LS values of 0.2 and 0.5 can also be considered estimates of pore water composition and compared with similar estimates obtained from Method 1316. This interlaboratory comparison will be based on a complete characterization sampling scheme (Option A as specified in section 12.5.1.1 of the test method). The dependent variables that will serve as the basis for evaluation will be (i) eluate pH as determined at the method target LS values (i.e., 0.2, 0.5, 1.0, 1.5, 2.0, 4.5, 5.0, 9.5, 10.0), (ii) eluate analyte concentration as determined at the method target LS values, and (iii) cumulative analyte release as determined at the method target LS values. Variation in the actual LS about the target LS value of each eluate but within the tolerances specified in the test method will require interpolation or extrapolation of measured analyte concentration values to the precise target value. The initial method of interpolation considered will be linear interpolation of the analyte concentration to the target LS value based on the log transform of the analyte concentration from the eluates having the nearest LS value greater than and less than the target value. If this method is found to provide poor representation of the overall LS dependent behavior of the analyte, then other interpolation methods such as cubic splines or exponential decay or error function curves will be considered. A common approach will be used for interpolation of eluate pH to the target LS values. The decision on the interpolation method to be used will be based on the results obtained from the referee laboratory and prior to initiating evaluation of data from the participant laboratories. An ANOVA statistical evaluation (see below for ANOVA specification) will be used to evaluate the contributions to variance and method precision for the discrete values of the dependent variables at each target value of the appropriate independent variable.

An alternate method of data interpretation of the dependent variables will be based on the functional relationship of the dependent variable to the specified independent variable (i.e., analyte concentration as a function of LS or cumulative release as a function of LS). Thus, potential functional relationships (e.g., exponential decay, error function or polynomial functions) will be regressed to the data set to provide a defined function to represent the overall result for each analyte. The contributions to variance in the resulting function then would serve as the basis for evaluating the method precision (see below for specification of statistical analysis of functional relationships).

Method 1315

The primary information to be derived from this test method is (i) the eluate pH and analyte flux as a function of time, (ii) the cumulative release (i.e., mg of analyte per m^2 of material leached based on the external geometric surface area of exposed faces) of each analyte as a function of time, and (iii) the mean observed diffusivity[2] of each analyte when diffusion controlled release is indicated (see Section 13.2 of Method 1315). The dependent variables that will serve as the basis for evaluation will be (i) eluate pH as determined at each method leaching interval (i.e., cumulative leaching times of 0.08, 1.0, 2.0, 7.0, 14.0, 28.0, 42.0, 49.0 and 63.0 days; see Table 1 of Method 1315), (ii) eluate analyte concentration as determined for each method leaching interval, (iii) cumulative analyte release for each leaching interval, (iv) analyte mean flux over each leaching interval, and (v) observed diffusivity for each analyte when applicable. Interpolation for determined concentrations and derived values of cumulative release and flux should not be necessary as long as leaching intervals are maintained within tolerances specified in the test method. An analysis of variance (ANOVA) statistical evaluation (see below) will be used to evaluate the contributions to variance and method precision for the discrete values of the dependent variables at each target value of the appropriate independent variable.

Method 1316

The primary information to be derived from this test method is (i) the eluate pH and analyte concentration as a function of LS, and (ii) the release (i.e., mg of analyte per kg of material leached) of each analyte as a function of LS. The dependent variables that will serve as the basis for evaluation will be (i) eluate pH as determined at the method target LS values (i.e., 0.5, 1.0, 2.0, 5.0, 10.0), (ii) eluate analyte concentration as determined at the method target LS values, (iii) analyte release as determined at the method target LS values, and (iv) an estimate of analyte concentration at LS value of 0.2 which can also be compared with the

[2] There will be up to 9 individual observations of observed diffusivity (one for each leaching interval) from each replicate of each application of Method 1315 for each specified analyte. Thus, a mean and standard deviation will be reported for each observed diffusivity value.

analyte concentration at LS value of 0.2 from Method 1314. Discrete values of each analyte are measured at each LS value and therefore interpolation will not be needed; however extrapolation of the functional relationship of analyte concentration as a function of LS will be needed to estimate the concentration at LS of 0.2. Extrapolation of analyte concentration as a function of LS to LS of 0.2 will be accomplished by regressing a functional relationship (e.g., linear, exponential or polynomial) to measured analyte concentrations in eluates from other LS values. Different functional relationships may be necessary for different analytes. The decision on the interpolation method to be used will be based on the results obtained from the referee laboratory and prior to initiating evaluation of data from the participant laboratories. An ANOVA statistical evaluation (see below) will be used to evaluate the contributions to variance and method precision for the discrete values of the dependent variables at each target value of the appropriate independent variable.

Statistical Analysis of Variance

The basic method of data analysis is provided as follows in the context of Method 1313 for a single analyte and a single material. The same approach will be used for Methods 1314, 1315 and 1316, as well as for multiple materials. It assumes that the interpolation to target measurement values (i.e., target pH values for Method 1313 and target LS values for Method 1314) has been performed and determined to be acceptable as described in the section titled "Outlier Identification and Model Assumption Checking." In the definitions given as follows, the convention is that a “measurement” refers to a log-transformed analyte concentration or other dependent variable value:

$Y_{i,j,k} = k^{th}$ measurement at the j^{th} target pH for the i^{th} lab,

where

$i = 1,\ldots,M$ (M =number of labs in the study, where the reference lab is the M^{th}),

$j = 1,\ldots,9$ (the number of pH levels), and

$k = 1,2,3$ for participant labs 1 through $M-1; k = 1,\ldots,6$ for the reference lab M

The statistical model underlying the analysis of variance is a mixed-effects model with fixed effects for pH level, and random effects for labs and lab-by-pH interactions. Specifically,

$$Y_{i,j,k} = \mu + \alpha_j + \beta_i + \gamma_{i,j} + \varepsilon_{i,j,k}$$

where

μ and α_j are fixed effects, to model the overall mean response at different pH levels,

β_i and $\gamma_{i,j}$ are random effects that model differences among labs, and

$\varepsilon_{i,j,k}$ is a random error term that models variation among replicates within a particular lab and pH combination.

The standard assumptions for the model are that β_i, $\gamma_{i,j}$ and $\varepsilon_{i,j,k}$ are independent normal random variables with zero means and variances σ_β^2, σ_γ^2, and σ^2, respectively. The model will be fit to the data using appropriate routines in the established statistical software package, SAS.

Assessment of repeatability and reproducibility is made via the estimated variance components, with small values of estimated σ^2 indicating high repeatability, and small values of σ_β^2 and σ_γ^2 indicating high reproducibility.

Outlier Identification and Model Assumption Checking. The validity and utility of results from the statistical analysis depends on the assumptions underlying the statistical model and the integrity of the data. Thus the statistical analysis will be accompanied with an assessment of the suitability of the model and the data will checked for aberrant values (outliers).

Checking the Interpolation. Because labs are not likely to precisely hit the target values, and because analyte concentrations might depend sensitively to the realized pH values, a preliminary assessment of the realized pH values and an assessment of the interpolation method to target pH values will be performed.

Assessing the Realized pH Values. Differences between the target and realized pH will be assessed for all labs at all target pH values. This will include summary analyses of the mean differences to determine whether there are systematic tendencies to under- or over-shoot the target values for different labs or target pH values and an assessment of variation of those differences to determine whether labs tend to be equally close to the target values. These analyses can be done using analysis of variance models similar to those described above, although the intent here is simply to quantify the performance of the labs at hitting the target values, for the purpose of justifying the interpolation step.

Assessing the Interpolation. The purpose of the interpolation step is to provide a common basis for comparing the measured values. It is anticipated that the interpolation will have little effect on the final data analysis, although this is something that will be checked. The most straightforward way to check the sensitivity of the interpolation step is to compare the statistical analysis results obtained using different

methods of interpolation, say via linear, polynomial, and spline curve fitting. If the results are sensitive to the calibration method, then it is anticipated that a spline method will supplant the proposed linear interpolation. The interpolation also introduces a secondary source of departure from the basic analysis of variance model assumptions in the form of dependence between the interpolated measurements. This can be assessed using advanced modeling features of Proc Mixed in SAS.

Outlier Identification. Possible outliers will be identified using standard methods of plotting residuals and comparing laboratory-specific summary measures of variability. It should be emphasized that in a study of this nature (interlaboratory study) there are multiple notions of what constitutes an "outlier" and these also manifest themselves as other forms of model violations. For example, the random error term in the statistical model is usually assumed to have the same variance at all pH levels where it is known that the variance is different at different pH levels (and is also assumed to be the same at all laboratories). This is directly checked by comparing between pH and within lab sample variances which can also be accomplished using advanced features of SAS's Proc Mixed procedure. A lab with a much greater variance than other those of other labs is a candidate for being declared an outlying lab. Regardless of how alleged outliers are identified, their impact on the statistical results is most definitively assessed by direct comparison of statistical results obtained via separate analyses using the full data set and the "cleaned" data set (with outliers removed).

More Advanced Modeling Options. For Method 1313, we are interpolating to the target pH values to have a consistent comparison of measured concentrations in eluates. Although this approach appears to work quite well for the fly ash data obtained so far, this may not prove to be the case with future materials. If this occurs, the approach would be changed to compare “curves” rather than individual values, thus changing to functional analysis (where “functional” refers to the types of curve fits used, such as polynomials). The basic idea is to fit a smooth curve to the analyte concentration as a function of pH (using the realized pH values) and then to compare the curves so obtained within labs (to assess repeatability) and among labs (to assess reproducibility). The basic methods and techniques of functional data analysis are described in the seminal book by Ramsay and Silverman (1997).

7.2 Chemical (ICP, XRF, AE-OES, OC/EC) and Physical (Moisture) Characterization

These data are reduced and reports are generated automatically by the instrument software or through spreadsheets. The primary analyst will review 100% of the report for completeness and to ensure that quality control checks meet established criteria. If QC checks do not meet acceptance criteria, sample analysis must be repeated. A secondary review will be performed by the Inorganic Laboratory Manager and Vanderbilt University to validate the analytical report. If appropriate, certain chemical characterization data will be compared to the XRF analyses. In addition, the ARCADIS QA Officer will review at least 10% of the raw data generated by ARCADIS for completeness. Analytical data will be summarized in periodic reports to the ARCADIS WAL. The procedures for reduction, validation and reporting of the leaching experiments (Task III) are outlined in the methods (http://www.vanderbilt.edu/leaching/downloads.html). ARCADIS WAL

is responsible for the implementation of these procedures. ARCADIS and Vanderbilt University will be responsible for publishing results and reports. QA/QC activities will be mentioned in any published materials. A data quality report will be provided in the final report of this investigation.

Data generated for the leachate analysis and total composition are entered into a standard Excel spreadsheet to ease uploading into the Vanderbilt metals database from the ICP-MS and other analyses. This data along with QA/QC information can be viewed using the "LeachXS Lite" software program developed by Vanderbilt University and the Energy Research Centre of the Netherlands. This software tool will allow users to view the metals leaching information based on sample type, facility configuration, or CCR coal type, or validation laboratory. This data viewer and database program will be available to the public on-line when complete. In addition, all data generated from the interlaboratory validation study will be archived by APPCD along with other project documentation.

7.3 Radionuclide Characterization

A Quality Assurance (QA) program involving verification of energy and Full Width at Half Maximum (FWHM) for several key photopeaks will be implemented. The calibration standard used to establish the system efficiency as a function of energy will be counted for 5 minutes daily. The photopeak energy, full width at half-maximum (FWHM) and net peak area for Cs-137 (662 keV) will be measured and plotted, with the FWHM for the 1332 keV peak of Co-60, for both detector systems. Any value occurring outside of 3 standard deviations of the mean (established in a preliminary study of about 20 measurements) must be immediately recounted. If the recount values are within 3 standard deviations, the system may be used for sample counting; if not an investigation into the detector reliability must be performed and a diagnosis and correction of any problems carried out before samples are counted on this system.

This page intentionally left blank.

8. Assessments

Assessments and audits are an integral part of a quality system. This project is assigned a QA Category III and, while desirable, does not require a planned technical systems audit (TSA). The ARCADIS QA Officer may conduct a TSA at the request of either the EPA WAM or the ARCADIS WAL. Internal assessments will be performed by project personnel to ensure acquired data meet data quality indicator goals established in Section 6.

There are currently no planned performance evaluation audits but Table 8-1 lists the measurement parameters and expected ranges should EPA determine a PEA should be provided.

Table 8-1. PEA Parameters and Ranges

Analyte or Measurement	Method	Expected Range
As, B, Ba, Ca, Co, Cr, Mo, Sb, Se, V	ICP-OES/3052/6020A	1-100 µg/mL
Hg	7470A	0.25 to 10 ug/L
pH	Electrode	0-14

The ARCADIS QA Officer will perform an internal data quality audit on at least 10% of the reported data. Reported results will be verified by performing calculations using raw data and information recorded in laboratory notebooks.

This page intentionally left blank.

9. References

ASTM, 1988. *Standard Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method,* Designation: E 691-87 American Society for Testing and Materials, 1988.

ASTM, 2005. *Standard test methods for laboratory determination of water (moisture) content of soil and rock by mass,* Method D 2216-05, American Society for Testing and Materials, 2005

ASTM, 2008. *Standard test methods for loss on ignition (LOI) of solid combustion residues,* Method D 7348-08, American Society for Testing and Materials, 2008.

ASTM, 2009. *Standard test methods for carbon black—total and external surface area by nitrogen adsorption,* Method D 6556-09, American Society for Testing and Materials, 2009.

CDC 2003. *Diesel particulate matter (as elemental carbon)*, Method 5040, Centers for Disease Control, NIOSH Manual of Analytical Methods (NMAM), Fourth Edition, 2003.

EPA, 1992. Method 1311 “Toxicity Characteristic Leaching Procedure”. Test Methods for Evaluating Solid Waste, Physical/Chemical Methods (SW-846) U.S. Environmental Protection Agency, 1992.

EPA, 1994. Method 1312 “Synthetic Precipitation Leaching Procedure”. Test Methods for Evaluating Solid Waste, Physical/Chemical Methods (SW-846) U.S. Environmental Protection Agency, 1994.

EPA, 1996a. Method 3052 “Microwave Assisted Acid Digestion of Siliceous and Organically Based Matrices”. Test Methods for Evaluating Solid Waste, Physical/Chemical Methods (SW-846) U.S. Environmental Protection Agency, 1996.

EPA, 1998. Method 7473, “Mercury in Solids and Solutions by Thermal Decomposition, Amalgamation, and Atomic Absorption Spectrophotometry.” Test Methods for Evaluating Solid Waste, Physical/Chemical Methods (SW-846). U.S. Environmental Protection Agency, 1998.

EPA, 2002a. Characterization and Management of Residues from Coal-Fired Power Plants, Interim Report. EPA-600/R-02, 083, U.S. Environmental Protection Agency, December 2002.

EPA, 2002b. Reply to comments on EPA/OSW’s Proposed Approach to Environmental Assessment of CCRs. Discussed March 5, 2002.

EPA, 2006a. Sanchez, F., R. Keeney, D. S. Kosson, and R. Delapp, 2006. *Characterization of Mercury-Enriched Coal Combustion Residues from Electric Utilities Using Enhanced Sorbents for Mercury Control,*

EPA-600/R-06/008. Prepared for the U.S. Environmental Protection Agency – Air Pollution Prevention and Control Division, Contract No. EP-C-04-023, Work Assignment 1-31, February 2006. www.epa.gov/nrmrl/pubs/600r06008/600r06008.pdf (Accessed November 12, 2009)

EPA, 2006b. Standard Operating Procedure for the Determination of Hexavalent Chromium in Ambient Air Analyzed by Ion Chromatography (IC). December 2006. Internet address: http://www.epa.gov/ttn/amtic/airtox.html (Accessed November 12, 2009)

EPA, 2007a. 2005 Urban Air Toxics Monitoring Program (UATMP) – Hexavalent Chromium, U.S. Environmental Protection Agency, EPA-454/R-07-005, February 2007.

EPA, 2007b. Method 9056A "Determination of Inorganic Anions by Ion Chromatography". Test Methods for Evaluating Solid Waste, Physical/Chemical Methods (SW-846), U.S. Environmental Protection Agency, February 2007.

EPA, 2007c. Method 6010C "Inductively Coupled Plasma-Atomic Emission Spectrometry". Test Methods for Evaluating Solid Waste, Physical/Chemical Methods (SW-846), U.S. Environmental Protection Agency, February 2007.

EPA, 2007d. Method 6020A "Inductively Coupled Mass Spectrometry". Test Methods for Evaluating Solid Waste, Physical/Chemical Methods (SW-846), U.S. Environmental Protection Agency, February 2007.

EPA, 2008. Sanchez, F., R. Keeney, D. S. Kosson, and R. Delapp, 2006. *Characterization of Mercury-Enriched Coal Combustion Residues from Electric Utilities Using Wet Scrubbers for Multi-Pollutant Control,* EPA-600/R-08/077. Prepared for the U.S. Environmental Protection Agency – Air Pollution Prevention and Control Division, Contract No. EP-C-04-023, Work Assignment 4-26, July 2008. http://www.epa.gov/nrmrl/pubs/600r08077/600r08077.htm (Accessed October 18, 2011)

EPA 2009, Kosson, D., F. Sanchez, P. Kariher, L.H. Turner, R. Delapp and P. Seignette. Characterization of Coal Combustion Residues from Electric Utilities – Leaching and Characterization Data. U.S. Environmental Protection Agency, EPA-600/R-09/151, December 2009.

EPA. *Guidance for Methods Development and Validation for the RCRA Program.* http://www.epa.gov/epawaste/hazard/testmethods/pdfs/methdev.pdf, accessed October 18, 2011.

Kosson, D.S., van der Sloot, H.A., Sanchez, F. and Garrabrants, A.C., 2002a. An Integrated Framework for Evaluating Leaching in Waste Management and Utilization of Secondary Materials. *Environmental Engineering Science* 19(3):159-204, 2002.

Ramsay, J.O. and Silverman, B.W. (1997). Functional Data Analysis. Springer-Verlag (New York).

van der Sloot, et al., 2010 (draft). Evaluation of Ruggedness Testing Needs for the Percolation Test, pH Dependence Leaching Test and Monolith Leaching Tests based on Existing Information. The Energy Research Centre of The Netherlands.

Appendix A

Laboratory Shipping Address

Name	Affiliation	Shipping Address
James M. Tinjum	University of Wisconsin-Madison	James M. Tinjum, P.E., Ph.D. University of Wisconsin-Madison Department of Civil and Environmental Engineering 2214 Engineering Hall 1415 Engineering Drive Madison, WI 53706
Mandi Richardson	URS Corp.	Mandi Richardson URS Corporation 9400 Amberglen Blvd. Austin, TX 78729
Jianmin Wang	Missouri University of Science and Technology	Jianmin Wang Dept. of Civil, Architectural & Environmental Engineering 223 Butler Carlton Hall University of Missouri-Rolla (UMR) Rolla, MO 65409
Zuzana Bohrerova	The Ohio State University	Zuzana Bohrerova The Ohio State University 470 Hitchcock Hall 2070 Neil Avenue Columbus, OH 43210-1275
Catherine Mattus	DOE- Oak Ridge National Laboratory	Catherine Mattus Oak Ridge National Laboratory P.O Box 2008 1 Bethel Valley Road Oak Ridge, TN 37831-6181
Eric Pierce	DOE- Pacific Northwest National Laboratory	Eric M. Pierce 790 6th Street Richland, WA 99338

Charles Crawford	DOE-Savannah River National Laboratory	Charles L. Crawford Savannah River National Laboratory Bldg. 773-42A Savannah River Site Aiken, SC 29808 Needs to have an internal number attached to the box: PO# 0T0580
Hwidong Kim	University of Florida	Hwidong Kim 220 Black Hall Department of Environmental Engineering & Sciences University of Florida Gainesville, FL, 32611.
Johnny Mitchell	Test America (TVA)	Johnny Mitchell TestAmerica Laboratories – Nashville 2960 Foster Creighton Drive Nashville, TN 37204
Rosanne Delapp	Vanderbilt University	Rosanne Delapp Vanderbilt University Jacobs Hall 149 400 24th Avenue South Nashville, TN 37235
Prof. Dr. Rob N.J. Comans	ECN	Dr. Rob N.J. Comans ECN Biomass, Coal and Environmental Research Energy research Centre of the Netherlands Westerduinweg 3, NL-1755 LE PETTEN Neatherlands
Ole Hjelmar	DHI	Ole Hjelmar DHI Urban & Industrial Dept. Agern Allé 5 DK-2970 Hørsholm Denmark
Jenet T. Hattaway	University of North Carolina Charlotte	Civil & Environmental Engineering University of North Carolina Charlotte Cameron Bldg. Rm 267 9201 University City Blvd. Charlotte, NC 28223-0002

PRELIMINARY VERSION of EPA METHOD 1313

Liquid-Solid Partitioning as a Function of Extract pH using Parallel Batch Extractions

LeachXS™ Lite Data Template - Version 1.1, January 2010

PROJECT/MATERIAL TITLE SHEET

PROJECT INFORMATION

Project Code	
Project Sponsor	
Project Description	
Material Code	
Material Replicate	
Material Originator	
Material Description	

Test Method Lab		Date Complete	
Contact		Phone	
Analytical Lab		Date Complete	
Contact		Phone	

DATABASE INFORMATION

Name of Database	
Material Code	
Material Class	
Material Subclass	

SIGNATURES

Data Compiler:	_____	Date:	_____
Data Reviewer:	_____	Date:	_____
Approved by:	_____	Date:	_____
LeachXS™ Lite Upload:	_____	Date:	_____

COAL COMBUSTION RESIDUE CLASSIFICATIONS

PROJECT & MATERIAL CODES

Project Code		Auto-inserted from "Title Sheet"
Material Code		Auto-inserted from "Title Sheet"
Material Replicate		Auto-inserted from "Title Sheet"

LeachXS Database Information

Name of Database		Auto-inserted from "Title Sheet"
Material Code		Auto-inserted from "Title Sheet"

RESIDUE DESCRIPTION

CCR Category	
Fly Ash Type	
Residue Handling	
Citation	*please specify*

SOURCE DESCRIPTION

Coal Type	
Coal Region	
Facility	*please specify*
Facility Description	

PROCESS DESCRIPTION

Particulate Capture	
Scrubber Type	
FGD Scrubber Additive	
NO_x Control	
SO_3 Control	
Hg Sorbent Injection	

PRE METHOD 1313 LeachXS™ Lite Data Template

MOISTURE CONTENT (WET BASIS) AND SOLIDS CONTENT INSTRUCTIONS

Step 1: Enter the project, material and replicate codes as well as the name of the technician conducting the test.

Step 2: Measure and record the mass of an empty drying or suitable weighing dish as well as the dish containing 5-10 g the "wet" sample. Record data and time of measurement. Place dish and sample into over at 105±5 °C for a minimum of 24 hr.

Step 3: Remove dish and sample from oven and allow to cool to room temperature in a desiccator. Measure and record the mass of the dish and dry sample. Place the dish and sample back into the oven for at least another 24-hr period.

Step 4: Repeat cooling and measurement procedure as shown in Step 3 until constant mass of the dish and sample is accheived. Record this mass and the final date and time. Discard the sample.

Step 5: Moisture and solids content are calculated automatically. Mean SC cell may be linked to the solids content cells in Pre-Test data and Test Data sheets. Alternately, copy the Mean SC cell value to these sheets.

PRE METHOD 1313 LeachXS™ Lite Data Template

MOISTURE CONTENT (WET BASIS) AND SOLIDS CONTENT INSTRUCTIONS

	Code	Description *(optional)*	Test conducted by:
Project		Auto-inserted from "Title Sheet"	
Material		Auto-inserted from "Title Sheet"	
Test Replicate	A		

	Dish-1	Dish-2	Dish-3	Date	Time
Empty Dish [g]					
Dish + Sample [g]					
Dish + Dry Sample [g]					
Check (Dish + Dry Sample) [g]					
Moisture Content (MC) [g-water/g]					
Solids Content (SC) [g-dry/g]					

Mean MC = [g-water/g]

Mean SC = [g-dry/g]

MOISTURE CONTENT (WET BASIS) AND SOLIDS CONTENT INSTRUCTIONS

	Code	Description *(optional)*	Test conducted by:
Project		Auto-inserted from "Title Sheet"	
Material		Auto-inserted from "Title Sheet"	
Test Replicate	B		

	Dish-1	Dish-2	Dish-3	Date	Time
Empty Dish [g]					
Dish + Sample [g]					
Dish + Dry Sample [g]					
Check (Dish + Dry Sample) [g]					
Moisture Content (MC) [g-water/g]					
Solids Content (SC) [g-dry/g]					

Mean MC = [g-water/g]

Mean SC = [g-dry/g]

MOISTURE CONTENT (WET BASIS) AND SOLIDS CONTENT INSTRUCTIONS

	Code	Description *(optional)*	Test conducted by:
Project		Auto-inserted from "Title Sheet"	
Material		Auto-inserted from "Title Sheet"	
Test Replicate	C		

	Dish-1	Dish-2	Dish-3	Date	Time
Empty Dish [g]					
Dish + Sample [g]					
Dish + Dry Sample [g]					
Check (Dish + Dry Sample) [g]					
Moisture Content (MC) [g-water/g]					
Solids Content (SC) [g-dry/g]					

Mean MC = [g-water/g]

Mean SC = [g-dry/g]

PreMethod 1313 LeachXS™ Lite Data Template

PRE-TEST TITRATION INSTRUCTIONS

Step 1: Enter the project, material and replicate codes as well as the technician name. In order to initiate test extration setup, enter the maximum particle size, solids content, and reagent type and normality.

Step 2: Enter target acid or base additions from prior knowledge or from prediction of neutralization classifications in Draft Method 1313 Table 2 (note: base equivalents have a negative sign).

Step 3: Prepare five bottles, labelled P01 through P05, with solid material. Add reagent water and acid or base to the bottles according to the Schedule of Acid and Base Additions. Enter date and time that agitation of extracts begins.

Step 4: At the conclusion of the test, enter date and time that agitation ends. Record leachate pH. The pre-test titration curve for the material will be plotted automatically (**note:** axis adjustments may be necessary).

Step 5: From the pre-test titration, select the additions of acid and base required to complete the list of target pH (see Draft Method 1313 Table 5) plotted as horizontal blue dashed lines. These acid/base additions are to be entered into the "Test Data" sheet to create the Schedule of Acid and Base Additions.

PreMethod 1313 LeachXS™ Lite Data Template

METHOD 1313 PRE-TEST TITRATION

	Code	Description *(optional)*
Project		Auto-inserted from "Title Sheet"
Material		Auto-inserted from "Title Sheet"
Test Replicate	A	

Test conducted by:

	Date	Time
Test Start		
Test End		

Required Contact Time * [hr]

Solids Information

Particle Size (85 wt% less than)		mm
Minimum Dry Equivalent Mass *		g-dry
Solids Content (default = 1)		g-dry/g
Mass of "As Tested" Material / Extraction		g

* Data based on Draft Method 1313 Table 1.

Extraction Information

LS Ratio	10	mL/g-dry
Liquid Volume / Extraction	200	mL
Recommended Bottle Size *	250	mL
Temperature		°C

Reagent Information

Acid Type		
Acid Normality		meq/mL
Base Type		
Base Normality		meq/mL

Schedule of Acid and Base Addition (±0.05) additional extracts as needed

Test Position	P01	P02	P03	P04	P05	P06	P07	P08	P09	P10	
"As Tested" Solid [g] (±0.05g)	-	-	-	-	-	-	-	-	-	-	Total Solid g
Reagent Water [mL] (±5%)	-	-	-	-	-	-	-	-	-	-	Total Water mL
Acid Volume [mL] (±1%)	-	-	-	-	-	-	-	-	-	-	Total Acid mL
Base Volume [mL] (±1%)	-	-	-	-	-	-	-	-	-	-	Total Base mL
Acid Addition [meq/g]											
Eluate pH											

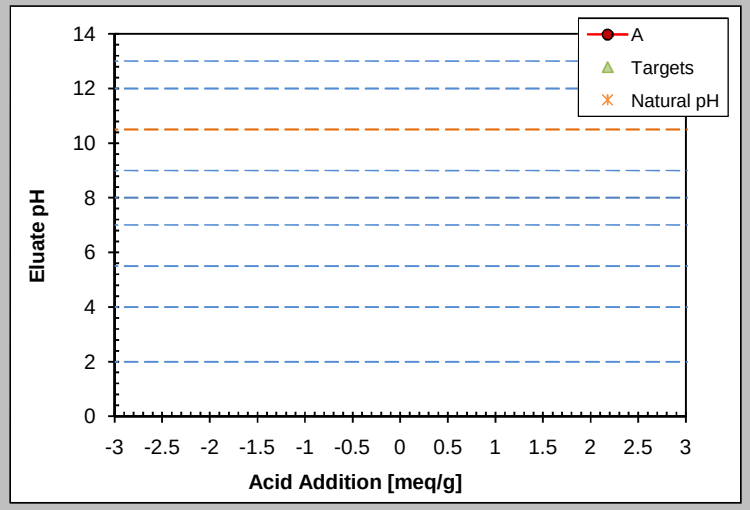

Acid Addition Required

[meq/g-dry]	pH Target		Rationale
0			Natural pH at LS 10 mL/g-dry (no acid/base addition)
	2.0	±0.5	Provides total or available content of COPCs
	4.0	±0.5	Lower pH limit of typical management scenario
	5.5	±0.5	Typical lower range of industrial waste landfills
	7.0	±0.5	Neutral pH region; high release of oxyanions
	8.0	±0.5	Endpoint pH of carbonated alkaline materials
	9.0	±0.5	Minimum of LSP curve for many cationic and amphoteric COPCs
	12.0	±0.5	Maximum in alkaline range for LSP curves of amphoteric COPCs
	13.0	±0.5	Upper bound (field conditions) for amphoteric COPCs
	10.5	±0.5	Substitution if natural pH falls within range of a mandatory pH target

Table 1 Extraction Parameters as a Function of Particle Size

Particle Size (85% less than) [mm]	US Sieve Size	Minimum Dry Equivalent [g-dry]	Contact Time [h]	Suggested Vessel Size [mL]
0.3	50	20±0.02	24±2	250
2	10	40±0.02	48±2	500
5	4	80±0.02	72±2	1000

Table 3 Pre-Test Tiration Schedule

Neutralization Classification	Acid or Base Addition [meq/g-dry]				
	P01	P02	P03	P04	P05
Low Alkalinity	-2	-1	0	1	2
Moderate Alkalinity	-2	0	2	5	10
High Alkalinity	0	5	10	15	25

Additional data points (e.g., T06, T07, T08 …) may be needed to provide titration curve resolution

PRE METHOD 1313 LeachXS™ Lite Data Template

EXTRACTION TEST INSTRUCTIONS

Step 1: Enter the project, material and replicate codes as well as the technician name. To initiate test setup, enter the maximum particle size, solids content, and reagent type and normality.

Step 2: Enter target acid or base additions from prior knowledge or from the pre-test titration (note: base equivalents have a negative sign).

Step 3: Add solid material to nine bottles, labelled T01 through T09. Label an additional three bottles as blanks (B01, B02, and B03). Add DI water and acid or base to eleven bottles (i.e,., T0x and B0x bottles) according to the Schedule of Acid and Base Additions. Enter date/time that extract agitation begins.

Note: If the acid or base is too dilute, large volume addition will be necessary. The acid or base normality may be adjusted for individual extractions.

Step 4: At the conclusion of the test, enter date and time that agitation ends. Record leachate information. Leachate pH and electrical conductivity (EC) will be plotted automatically (note: axis adjustments may be necessary).

Step 5: If the pH of the extract is within the target range and an analytical sample is to be saved, enter the letter "a" in the last row (font converts "a" to a check mark). If the extract will not be saved for chemical analysis, enter the letter "r" in the last row (font converts "r" to an X).

PRE METHOD 1313 LeachXS™ Lite Data Template

METHOD 1313 EXTRACTION DATA

	Code	Description *(optional)*
Project		Auto-inserted from "Title Sheet"
Material		Auto-inserted from "Title Sheet"
Test Replicate	A	

Test conducted by:

	Date	Time
Test Start		
Test End		

Required Contact Time * hr

Solids Information

Maximum Particle Size		mm
Minimum Dry Equivalent Mass *		g-dry
Solids Content (default = 1)		g-dry/g
Mass of "As Tested" Material / Extraction		g

* Data based on Draft Method 1313 Table 1.

Extraction Information

LS Ratio	10	mL/g-dry
Liquid Volume / Extraction	200	mL
Recommended Bottle Size *	250	mL
Temperature		°C

Nominal Reagent Information

Acid Type		
Acid Normality		meq/mL
Base Type		
Base Normality		meq/mL

Schedule of Acid and Base Addition

Test Position	T01	T02	T03	T04	T05	T06	T07	T08	T09	B01	B02	B03	totals	
"As Tested" Solid [g] (±0.05g)	-	-	-	-	-	-	-	-	-	no solid	no solid	no solid		g
Reagent Water [mL] (±5%)	-	-	-	-	-	-	-	-	-	-	-	-		mL
Acid Volume [mL] (±1%)	-	-	-	-	-	-	-	-	-	-	-	-		mL
Base Volume [mL] (±1%)	-	-	-	-	-	-	-	-	-	-	-	-		mL
Acid Normality [meq/mL]	-	-	-	-	-	-	-	-	-	-	-	-		
Base Normality [meq/mL]	-	-	-	-	-	-	-	-	-	-	-	-		

Target pH	13.0±0.5	12.0±0.5	10.5±0.5	9.0±0.5	8.0±0.5	7.0±0.5	5.5±0.5	4.0±0.5	2.0±0.5	Water	Acid	Base	
Acid Addition [meq/g]													
Eluate pH													
Eluate EC [mS/cm]													
Eluate Eh [mV]													
Meets pH criteria?													Enter "a" for "yes" or "r" for "no".
Notes													

PRE METHOD 1313 LeachXS™ Lite Data Template

METHOD 1313 EXTRACTION DATA

	Code	Description *(optional)*
Project		Auto-inserted from "Title Sheet"
Material		Auto-inserted from "Title Sheet"
Test Replicate	B	

Test conducted by:

	Date	Time
Test Start		
Test End		

Required Contact Time * hr

Solids Information

Maximum Particle Size		mm
Minimum Dry Equivalent Mass *		g-dry
Solids Content (default = 1)		g-dry/g
Mass of "As Tested" Material / Extraction		g

* Data based on Draft Method 1313 Table 1.

Extraction Information

LS Ratio	10	mL/g-dry
Liquid Volume / Extraction	200	mL
Recommended Bottle Size *	250	mL
Temperature		°C

Nominal Reagent Information

Acid Type		
Acid Normality		meq/mL
Base Type		
Base Normality		meq/mL

Schedule of Acid and Base Addition

Test Position	T01	T02	T03	T04	T05	T06	T07	T08	T09	B01	B02	B03	totals	
"As Tested" Solid [g] (±0.05g)	-	-	-	-	-	-	-	-	-	no solid	no solid	no solid		g
Reagent Water [mL] (±5%)	-	-	-	-	-	-	-	-	-	-	-	-		mL
Acid Volume [mL] (±1%)	-	-	-	-	-	-	-	-	-	-	-	-		mL
Base Volume [mL] (±1%)	-	-	-	-	-	-	-	-	-	-	-	-		mL
Acid Normality [meq/mL]	-	-	-	-	-	-	-	-	-	-	-	-		
Base Normality [meq/mL]	-	-	-	-	-	-	-	-	-	-	-	-		

Target pH	13.0±0.5	12.0±0.5	10.5±0.5	9.0±0.5	8.0±0.5	7.0±0.5	5.5±0.5	4.0±0.5	2.0±0.5	Water	Acid	Base
Acid Addition [meq/g]												
Eluate pH												
Eluate EC [mS/cm]												
Eluate Eh [mV]												
Save? (enter "a" or "r")												
Notes												

Note: If multiple replicate tests are carried out in parallel, only one set of method blanks is necessary.

PRE METHOD 1313 LeachXS™ Lite Data Template

METHOD 1313 EXTRACTION DATA

	Code	Description *(optional)*
Project		Auto-inserted from "Title Sheet"
Material		Auto-inserted from "Title Sheet"
Test Replicate	C	

Test conducted by:

	Date	Time
Test Start		
Test End		

Required Contact Time * hr

Solids Information

Maximum Particle Size		mm
Minimum Dry Equivalent Mass *		g-dry
Solids Content (default = 1)		g-dry/g
Mass of "As Tested" Material / Extraction		g

* Data based on Draft Method 1313 Table 1.

Extraction Information

LS Ratio	10	mL/g-dry
Liquid Volume / Extraction	200	mL
Recommended Bottle Size *	250	mL
Temperature	21	°C

Nominal Reagent Information

Acid Type		
Acid Normality		meq/mL
Base Type		
Base Normality		meq/mL

Schedule of Acid and Base Addition

Test Position	T01	T02	T03	T04	T05	T06	T07	T08	T09	B01	B02	B03	totals	
"As Tested" Solid [g] (±0.05g)	-	-	-	-	-	-	-	-	-	no solid	no solid	no solid		g
Reagent Water [mL] (±5%)	-	-	-	-	-	-	-	-	-	-	-	-		mL
Acid Volume [mL] (±1%)	-	-	-	-	-	-	-	-	-	-	-	-		mL
Base Volume [mL] (±1%)	-	-	-	-	-	-	-	-	-	-	-	-		mL
Acid Normality [meq/mL]	-	-	-	-	-	-	-	-	-	-	-	-		
Base Normality [meq/mL]	-	-	-	-	-	-	-	-	-	-	-	-		

Target pH	13.0±0.5	12.0±0.5	10.5±0.5	9.0±0.5	8.0±0.5	7.0±0.5	5.5±0.5	4.0±0.5	2.0±0.5	Water	Acid	Base
Acid Addition [meq/g]												
Eluate pH												
Eluate EC [mS/cm]												
Eluate Eh [mV]												
Save? (enter "a" or "r")												
Notes												

Note: If multiple replicate tests are carried out in parallel, only one set of method blanks is necessary.

Table 4 Extraction Parameters as a Function of Particle Size

Maximum Particle Size [mm]	US Sieve Size	Minimum Dry Equivalent [g-dry]	Contact Time [h]	Suggested Vessel Size [mL]
0.3	50	20±0.02	24±2	250
2	10	40±0.02	48±2	500
5	4	80±0.02	72±2	1000

Table 5 Final Extract pH Targets

pH Target	Rationale
varies	Natural pH at LS 10 mL/g-dry (no acid/base addition)
2.0±0.5	Provides total or available COPC content
4.0±0.5	Lower pH limit of typical management scenario
5.5±0.5	Typical lower range of industrial waste landfills
7.0±0.5	Neutral pH region; high release of oxyanions
8.0±0.5	Endpoint for carbonated alkaline materials
9.0±0.5	Minimum of LSP curve for many cationic and amphoteric COPCs
12.0±0.5	Maximum in alkaline range for LSP curves of amphoteric COPCs
13.0±0.5	Upper bound (field conditions) for amphoteric COPCs
10.5±0.5	Substitution if natural pH falls within another mandatory target

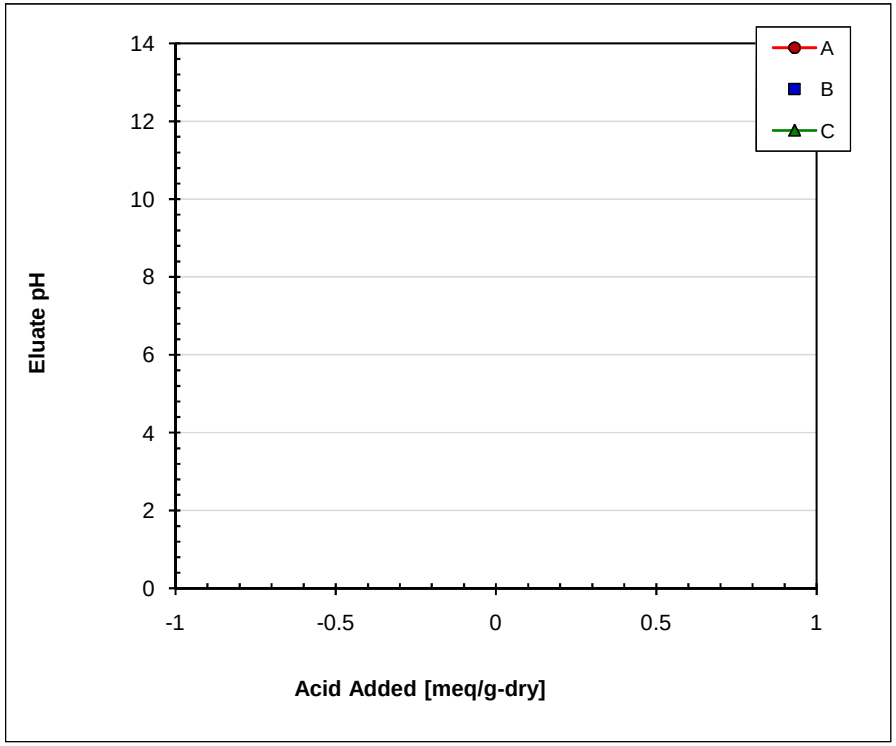

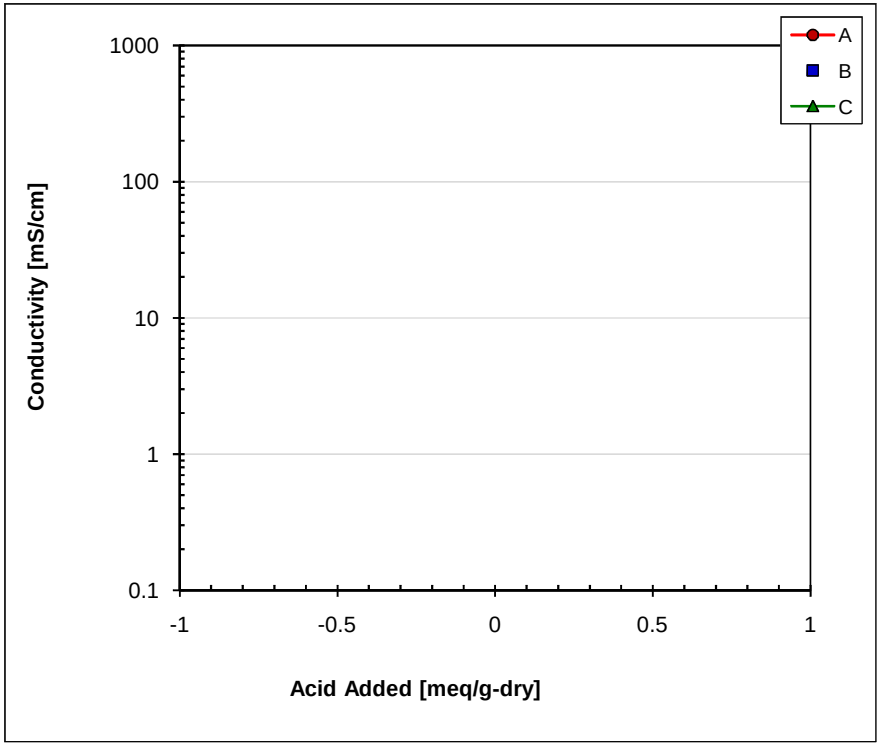

PreMethod 1313 LeachXS™ Lite Data Template

SELECTION OF ANALYTICAL SOLUTIONS

This page is for selection of a final set of nine extractions per test replicate from the "Lab Extractions" data. All data is manually input by the user based on if extraction meet the pH criteria.

METHOD 1313 SELECTED ANALYTICAL SOLUTIONS

	Code	Description *(optional)*
Project		Auto-inserted from "Title Sheet"
Material		Auto-inserted from "Title Sheet"

Test Replicate: A

Max Particle Size: mm
Solids Content: g-dry/g
Temperature: °C
Acid Type: *selected from drop-down menu*
Base Type: *selected from drop-down menu*
Lab Technician:

Test Position	T01	T02	T03	T04	T05	T06	T07	T08	T09	B01	B02	B03
Test Start Date												
Extraction Duration [hr]												
"As Tested" Solid [g]												
Reagent Water [mL]												
Acid Volume [mL]												
Base Volume [mL]												
Acid Normality [meq/mL]												
Base Normality [meq/mL]												
Acid Addition [meq/g]										Water	Acid	Base
Eluate pH												
Eluate EC [mS/cm]												
Eluate Eh [mV]												
Remarks												

Test Replicate: B

Max Particle Size: mm
Solids Content: g-dry/g
Temperature: °C
Acid Type: *selected from drop-down menu*
Base Type: *selected from drop-down menu*
Lab Technician:

Test Position	T01	T02	T03	T04	T05	T06	T07	T08	T09	B01	B02	B03
Test Start Date												
Extraction Duration [hr]												
"As Tested" Solid [g]												
Reagent Water [mL]												
Acid Volume [mL]												
Base Volume [mL]												
Acid Normality [meq/mL]												
Base Normality [meq/mL]												
Acid Addition [meq/g]										Water	Acid	Base
Eluate pH												
Eluate EC [mS/cm]												
Eluate Eh [mV]												
Remarks												

Test Replicate: C

Max Particle Size: mm
Solids Content: g-dry/g
Temperature: °C
Acid Type: *selected from drop-down menu*
Base Type: *selected from drop-down menu*
Lab Technician:

Test Position	T01	T02	T03	T04	T05	T06	T07	T08	T09	B01	B02	B03
Test Start Date												
Extraction Duration [hr]												
"As Tested" Solid [g]												
Reagent Water [mL]												
Acid Volume [mL]												
Base Volume [mL]												
Acid Normality [meq/mL]												
Base Normality [meq/mL]												
Acid Addition [meq/g]										Water	Acid	Base
Eluate pH												
Eluate EC [mS/cm]												
Eluate Eh [mV]												
Remarks												

Table 5	Final Extract pH Targets
pH Target	**Rationale**
varies	Natural pH at LS 10 mL/g-dry (no acid/base addition)
2.0±0.5	Provides total or available COPC content
4.0±0.5	Lower pH limit of typical management scenario
5.5±0.5	Typical lower range of industrial waste landfills
7.0±0.5	Neutral pH region; high release of oxyanions
8.0±0.5	Endpoint for carbonated alkaline materials
9.0±0.5	Minimum of LSP curve for many cationic and amphoteric COPCs
12.0±0.5	Maximum in alkaline range for LSP curves of amphoteric COPCs
13.0±0.5	Upper bound (field conditions) for amphoteric COPCs
10.5±0.5	Substitution if natural pH falls within another mandatory target

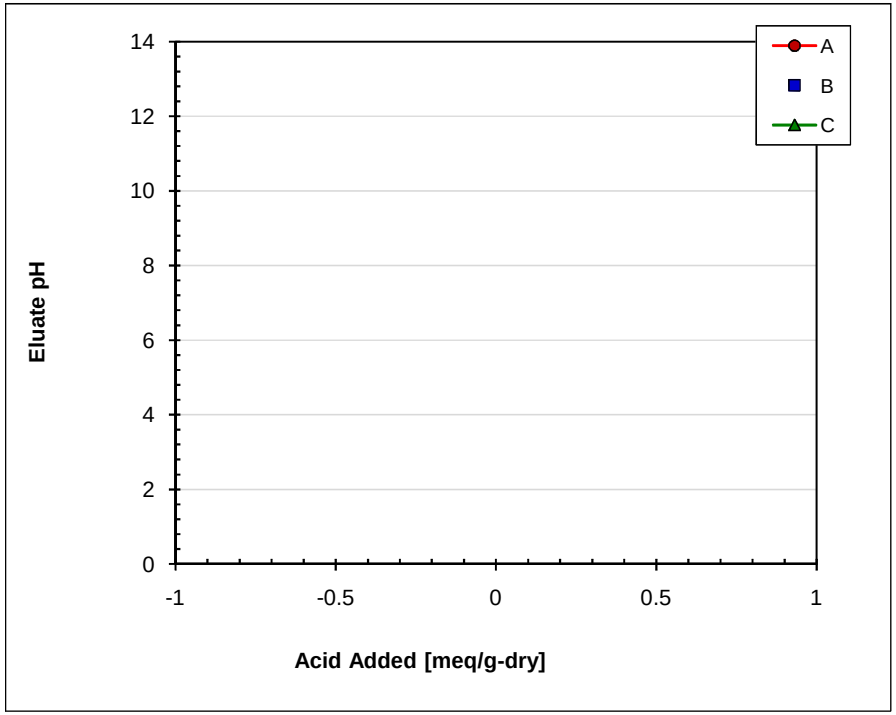

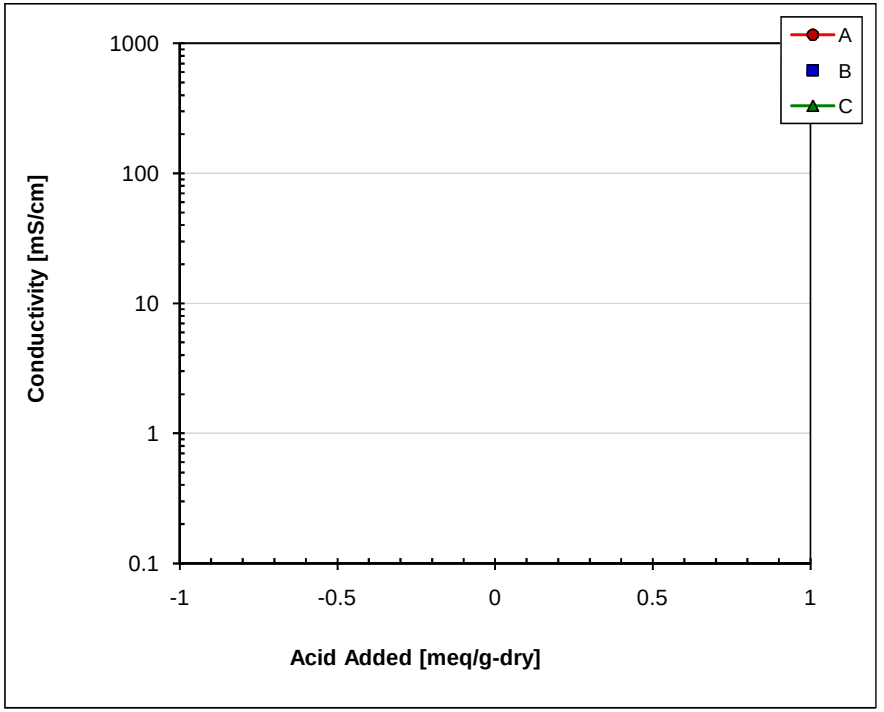

PreMethod 1313 LeachXS™ Lite Data Template

METHOD 1313 MASTER DATA LIST

QC Flags	
J	Value greater than calibration
E	Value between MDL and ML
U	Value less than MDL
U1/2	Value less than MDL (shown at 1/2 MDL)

	Code	Description *(optional)*
Project ID		Auto-inserted from "Title Sheet"
Material ID		Auto-inserted from "Title Sheet"
Test ID	1313	

	Acid Type	Base Type
Test Rep A		
Test Rep B		
Test Rep C		

MDL
ML
Analytical Method
Analysis Date
Analytical Lab Name

									Eluate Composition		
Sample ID	"As Tested" Solid	Moisture Content	Water Added	Acid Added	Acid Stength	Base Added	Base Stength	Acid Added	Eluate pH	Eluate Cond.	Eluate ORP
	g	g-H_2O/g	mL	mL	N	mL	N	meq/g-dry	s.u.	mS/cm	mV
-1313-T01-A											
-1313-T02-A											
-1313-T03-A											
-1313-T04-A											
-1313-T05-A											
-1313-T06-A											
-1313-T07-A											
-1313-T08-A											
-1313-T09-A											
-1313-T01-B											
-1313-T02-B											
-1313-T03-B											
-1313-T04-B											
-1313-T05-B											
-1313-T06-B											
-1313-T07-B											
-1313-T08-B											
-1313-T09-B											
-1313-T01-C											
-1313-T02-C											
-1313-T03-C											
-1313-T04-C											
-1313-T05-C											
-1313-T06-C											
-1313-T07-C											
-1313-T08-C											
-1313-T09-C											
-1313-B01-A	-	-						-			
-1313-B02-A	-	-						-			
-1313-B03-A	-	-						-			

PreMethod 1313 LeachXS™ Lite Data Template

Detection and Quantification Limits

Al	Sb	As	Ba	Be	B	Cd	Ca	Cs	Cr	Co	Cu

	1		2		3		4		5		6		7		8		9		10		11		12	
	Aluminum Al µg/L	QC	Antimony Sb µg/L	QC	Arsenic As µg/L	QC	Barium Ba µg/L	QC	Beryllium Be µg/L	QC	Boron B µg/L	QC	Cadmium Cd µg/L	QC	Calcium Ca µg/L	QC	Cesium Cs µg/L	QC	Chromium Cr µg/L	QC	Cobalt Co µg/L	QC	Copper Cu µg/L	QC

Fe	Pb	Li	Mg	Mn	Mo	Ni	P	K	Se	Si	Na

13		14		15		16		17		18		19		20		21		22		23		24	
Iron Fe µg/L	QC	Lead Pb µg/L	QC	Lithium Li µg/L	QC	Magnesium Mg µg/L	QC	Manganese Mn µg/L	QC	Molybdenum Mo µg/L	QC	Nickel Ni µg/L	QC	Phosphorus P µg/L	QC	Potassium K µg/L	QC	Selenium Se µg/L	QC	Silicon Si µg/L	QC	Sodium Na µg/L	QC

PreMethod 1313 LeachXS™ Lite Data Template

Sr	S	Tl	Sn	Ti	U	V	Zn	Hg	F	Cl	NO2

25		26		27		28		29		30		31		32		33		34		35		36	
Strontium Sr	QC	Sulfur S	QC	Thallium Tl	QC	Tin Sn	QC	Titanium Ti	QC	Uranium U	QC	Vanadium V	QC	Zinc Zn	QC	Mercury Hg	QC	Fluoride F	QC	Chloride Cl	QC	Nitrite NO2	QC
µg/L		µg/L		µg/L		µg/L		µg/L		µg/L		µg/L		µg/L		µg/L		µg/L		µg/L		µg/L	

Br	NO3	SO4	PO4	DIC	DOC	NH3

37		38		39		40		41		42		43	
Bromide Br		Nitrate NO3		Sulfate SO4		Phosphate PO4		Inorganic C DIC		Organic C DOC		Ammonia NH3	
µg/L	QC	µg/L	QC	µg/L	QC	µg/L	QC	µg/L	QC	µg/L	QC	µg/L	QC

UNITED STATES ENVIRONMENTAL PROTECTION AGENCY
WASHINGTON, D.C. 20460

OFFICE OF
SOLID WASTE AND
EMERGENCY RESPONSE

Dear Leach Validation Participant,

Welcome to the Phase I validation of PreMethods 1313 (pH dependent leach test) and 1316 (L/S ratio leach test). These methods represent a significant step forward in the science of modeling material leaching into the environment. As a participatory laboratory, your assistance in this effort will help ensure these methods are incorporated in EPA's publicly available method compendium *Test Methods for Evaluating Solid Waste Physical/Chemical Methods* (SW-846).

As you review the methods, along with the instructions and materials enclosed in this package, I would like to highlight a couple of key points. First, please make sure you downloand and review the most current version of PreMethods 1313 and 1316 along with the laboratory instruction sheet (enclosed) before running the methods (see www.vanderbilt.edu/leaching). Some minor changes and clarifications were recently made to the methods to help improve their usability. Second, please check the list of materials provided on the instruction sheet to ensure your kit is complete. Lastly, please note that since you will be shipping the extracted elluates to Vanderbilt University for analysis, it is important that you follow the preservation instructions to ensure accurate results.

From the start of this interlaboratory validation effort, one of our top priorities is to make sure we are being responsive to the needs of our participating labs. As such, please do not hesitate to contact me with any problem, issue, or concern you may have throughout this process. You can contact me by phone at 703-308-0157 or by email at baldwin.mark@epa.gov. Again on behalf of the EPA, I would like to thank you and your laboratory for your invaluable contribution to this validation effort.

Sincerely,

Mark Baldwin

Phase I of Method 1313/Method 1316 Validation

The subject material for Phase I of the Method 1313/Method 1316 inter-laboratory validation study is a coal combustion fly ash. A generic MSDS for coal fly ash is included with the material shipment.

The subject material may be treated as a well homogenized sample with 85% < 0.3 mm particle size. Thus:

- the minimum equivalent dry mass for Method 1313 and Method 1316 will be 20 g-dry and all extractions may be conducted in 250-mL bottles with the exception of two low liquid-solid (LS) ratio test positions, 1316-T04 and T05, which will likely require higher amounts of solid materials in a 500 mL bottles in order to ensure 50 mL analytical solutions
- no particle size reduction or sieve analysis is required for this Phase I sample

Although the titration curve should be developed as part of the method validation, baseline characterization has shown the titration curve for the Phase I material to be very sensitive to acid addition in the neutral range. Extreme care should be taken to provide exact volumes of acid addition during (i) the pre-test titration in order to produce an accurate titration curve and (ii) the extraction step in order to reproduce an acceptable final pH. Test positions that meet pH tolerances should be processed for chemical analysis and only those test positions that do not meet test position pH tolerances need to be rerun.

The kit supplied for the Phase I validation study includes:

- Four sets of completed bottle labels for each test replicate
- One chain of custody form
- Two questionnaires (one for each Method 1313 and Method 1316)

The sample labeling convention used to identify a particular solution consists of numerical identifiers for the material, lab, test method, and test position along with an alphabetical identifier for the test replicate. The layout for the sample label convention is as follows:

M*aa***L***bb***-131***c***-T***dd***-***e*** (Test Positions T01 through T09)

M*aa***L***bb***-131***c***-B***dd***-***e*** (QA/QC Blanks B01-B03)

"aa" is a two-digit number starting at zero that identifies the test material (e.g., the Phase I material is M01),

"bb" is a two-digit number starting at zero that identifies the participating laboratory (assigned randomly by EPA-ORCR),

"c" is a single digit number that completes the test method ID (i.e., 1313 or 1316),

"dd" is a two-digit number starting at zero that identifies the test position or QA/QC blank.

"e" is a single letter representing the test replicate (i.e., A, B or C).

Four sets of completed labels are provided to be used for labeling extraction vessels and two sets of 50-mL analytical samples. The remaining fourth set may be reserved for replacements as needed.

Instructions for Phase I Validation

On or before June 7, 2010:

1. Prepare 3 test replicates of extracts for the supplied sample material according to the most current versions of Method 1313 and Method 1316[1]. Use the Excel data templates to calculate extract "recipes" and return a completed Excel data template to the Vanderbilt project lead, Andy Garrabrants (A.Garrabrants@vanderbilt.edu) via email. Each method should be conducted as specified in the method draft to the extent possible; however, any necessary deviations should be recorded and a log of deviations returned with the Excel data template.

2. For each test position and QA/QC blank, collect two 50-mL analytical samples in the DigiTubes provided. Preserve each analytical sample with Optima grade (or similar purity) nitric acid to a final concentration of 1% (v/v). Each analytical sample should have a label (prefilled and provided) corresponding to its test position (e.g., T01-T09) and test replicate (e.g, A, B, and C).

3. Return one set test positions and QA/QC blanks in 50-mL DigiTubes for each Method 1313 and Method 1316 to Vanderbilt University for chemical analysis and retain the remaining set of samples onsite at least until the end of Phase I testing.

   Shipments should be sent no later than June 7, 2010 and a completed chain of custody form (provided) should be included. Please ship samples (Monday through Thursday pickup only as Vanderbilt cannot accept Saturday deliveries) to following address:

   Civil & Environmental Engineering
   Vanderbilt University
   c/o Rossane DeLapp
   Jacobs Hall 149
   400 24th Avenue South
   Nashville, TN 37235
   (615) 322-3189

   Please inform the ORCR study lead, Mark Baldwin (Baldwin.Mark@epa.gov), and Vanderbilt lead, Andy Garrabrants (A.Garrabrants@vanderbilt.edu), of your intended ship date so that arrangements may be made to receive the shipment.

4. Complete the method feedback questionnaire for each test method (available at www.vanderbilt.edu/leaching/downloads.html) and return it to Mark Baldwin by email no later than June 7, 2010.

Programmatic and technical questions may be directed to the ORCR lead, Mark Baldwin (Baldwin.Mark@epa.gov, 703-308-0157).

[1] The latest versions of these test methods and data templates may be downloaded at www.vanderbilt.edu/leaching/downloads.html. Although the procedures themselves are not changed in any way, the method drafts dated April 26, 2010 contain minor clarifications to the method which are intended to improve understanding of the method

Arcadis Geraghty and Miller
4915 Prospectus Drive
Durham, NC 27713
(919) 544-4535

CHAIN OF CUSTODY RECORD

Project Description: Phase I Lab Validation for 1313 and 131(Page 1 of 1
Arcadis G&M charge # : RN990271.0007.00001
Responsible EPA Party: Mark Baldwin
Responsible Arcadis Party: Peter Kariher

Sample ID	Date Collected	Sample Description		Number of Containers	Analyses Required	
Method 1313 Solid Material	04/26/10	1 Liter HDPE container of lab validaton material	approximately 1 kg	2	SW-846 Method 1313	
Method 1316 Solid Material	04/26/10	1 Liter HDPE container of lab validaton material	approximately 1 kg	4	SW-846 Method 1316	

Sample ID	Special Instructions

Report results to: Vanderbitl University

(phone) _____

(fax) _____

Samples shipped to: Civil & Environmental Engineering
Vanderbilt University
c/o Rossane DeLapp
Jacobs Hall 149
400 24th Avenue South
Nashville, TN 37235

Samples collected by: Peter H. Kariher
(signature) _____ Date: 4/26/2010

Samples relinquished by: _____
(signature) _____ Date: _____

Samples received by: _____
(signature) _____ Date: _____

Date shipped: 4/26/2010

M01-L01-1313-T01-A	**M01-L01-1313-T01-B**	**M01-L01-1313-T01-C**
M01-L01-1313-T02-A	**M01-L01-1313-T02-B**	**M01-L01-1313-T02-C**
M01-L01-1313-T03-A	**M01-L01-1313-T03-B**	**M01-L01-1313-T03-C**
M01-L01-1313-T04-A	**M01-L01-1313-T04-B**	**M01-L01-1313-T04-C**
M01-L01-1313-T05-A	**M01-L01-1313-T05-B**	**M01-L01-1313-T05-C**
M01-L01-1313-T06-A	**M01-L01-1313-T06-B**	**M01-L01-1313-T06-C**
M01-L01-1313-T07-A	**M01-L01-1313-T07-B**	**M01-L01-1313-T07-C**
M01-L01-1313-T08-A	**M01-L01-1313-T08-B**	**M01-L01-1313-T08-C**
M01-L01-1313-T09-A	**M01-L01-1313-T09-B**	**M01-L01-1313-T09-C**
M01-L01-1313-B01-A	**M01-L01-1313-B01-B**	**M01-L01-1313-B01-C**

Method Feedback Questionnaire

METHOD 1313: Liquid-Solid Partitioning as a Function of Eluate pH using a Parallel Batch Procedure

---

1. Please indicate the amount of time (in professional hours) required to complete the following steps of Method 1313:

Material Preparation (e.g., air drying, particle-size reduction, sieving)	_____ hrs
Pre-test Titration	_____ hrs
Extraction Setup (e.g., solids, water, acid/base additions)	_____ hrs
Eluate Processing (e.g., pH/cond, filtration, analytical prep)	_____ hrs

2. How would you rate the overall usability of Method 1313?

3. In total, how much time (in professional hours) was required to process three test replicates of the test material using Method 1313?

4. Were the overall goals and instructions provided with the sample material clearly laid out and easy to follow? If not, please suggest specific sections of the method where clarifications could be made.

5. Were the procedures in the method draft clearly laid out and easy to follow? If not, please suggest specific sections of the method where clarifications could be made.

6. Was the Excel data template clearly laid out and easy to follow? If not, please suggest specific sections of the data template where clarifications could be made.

7. In preparing solid samples for the method, what difficulties (if any) were encountered? How were these difficulties overcome?

8. While defining the pre-test titration curve, what difficulties (if any) were encountered? How were these difficulties overcome?

9. When using the Excel data template sheets, what difficulties (if any) were encountered? How were these difficulties overcome?

10. What difficulties (if any) did you encounter with acquiring or operating the required equipment?

11. How much time did it take technical personnel to become familiar with the method?

12. Please provide any general feedback (e.g., comments, edits, questions, software glitches, or concerns) below. Include any suggested modifications to the test procedure, the Excel data template or to the method draft.

Method Feedback Questionnaire

METHOD 1316: Liquid-Solid Partitioning as a Function of Liquid-Solid Ratio using a Parallel Batch Procedure

---

1. Please indicate the amount of time (in professional hours) required to complete the following steps of Method 1316:

Material Preparation (e.g., air drying, particle-size reduction, sieving)	_____ hrs
Extraction Setup (e.g., solids, water, acid/base additions)	_____ hrs
Eluate Processing (e.g., pH/cond, filtration, analytical prep)	_____ hrs

2. How would you rate the overall usability of Method 1316?

---

3. In total, how much time (in professional hours) was required to process three test replicates of the test material using Method 1316?

---

4. Were the overall goals and instructions provided with the sample material clearly laid out and easy to follow? If not, please suggest specific sections of the method where clarifications could be made.

---

5. Were the procedures in the method draft clearly laid out and easy to follow? If not, please suggest specific sections of the method where clarifications could be made.

6. Was the Excel data template clearly laid out and easy to follow? If not, please suggest specific sections of the data template where clarifications could be made.

7. In preparing solid samples for the method, what difficulties (if any) were encountered? How were these difficulties overcome?

8. When using the Excel data template sheets, what difficulties (if any) were encountered? How were these difficulties overcome?

9. What difficulties (if any) did you encounter with acquiring or operating the required equipment?

10. How much time did it take technical personnel to become familiar with the method?

11. Please provide any general feedback (e.g., comments, edits, questions, software glitches, or concerns) below. Include any suggested modifications to the test procedure, the Excel data template or to the method draft.

Appendix D. Blank Analysis and Data Filtering

TABLE OF CONTENTS

Method 1313 Method Blanks and Data Filtering D-1
Phase I Method Blanks D-1
Phase I Data Filtering D-3
Filtering for Cause D-3
Effect of Phase I Data Filtering on Statistical Analysis D-5
Phase II Method Blanks D-8
Phase II Data Filtering D-8
Method 1313 Filtration Summary D-8
Method 1316 Method BLanks and Data Filtering D-11
Phase I Method Blanks D-11
Phase I Data Filtering D-11
Phase II Method Blanks D-13
Phase II Data Filtering D-16
Method 1316 Filtering Summary D-17

Blank Analysis and Data Filtering

During the review of Phase I of Method 1313 and Method 1316 data, there were some data points and some data sets that were visually different than the bulk of the data. In addition, significant concentrations of some analytes were noted in the method blank eluates (extractions conducted with all reagents and procedures but without the subject material) which indicated some degree of external contamination. Therefore, a process was developed for filtering data that was considered "valid" based on either (i) known or suspected errors in performing the method or in following the validation study instructions, or (ii) interpretation of the blank concentrations and their effect on eluate concentrations.

Method 1313 Method Blanks and Data Filtering

Phase I Method Blanks

Method 1313 specifies that three method blank extractions should be conducted, preserved for analysis and interpreted as support that measured concentrations in the method test are not influenced by external sources of contamination. These three method blanks include:

- B01 – a method blank simulating the natural extraction condition (i.e., reagent water with no acid or base added),
- B02 – a method blank simulating the pH 2.0 target extraction without solid sample (i.e., same amount of acid added to reagent water), and
- B03 – a method blank simulating the pH 13.0 target extraction without solid sample (i.e., same amount of base added to reagent water).

Prior to analysis, all analytical solutions were preserved for ICP-OES analysis with Optima grade nitric acid to a final concentration of 1% (v/v).

Method blanks, for selected analytes of Method 1313 conducted on the Phase I EaFA material, are shown in Figure 1. In the figure, the maximum concentrations of method blanks with values above ICP-OES detection limits are shown. For the purposes of comparison, the minimum measured concentrations for each analyte are shown in the figure.

Several labs had higher than expected concentrations of some targeted constituents. Evaluation of the three method blanks show that contamination may introduced through the reagent water (e.g., antimony in L04 and L05), the acid used in the extraction (e.g., calcium in L04) or the base used in the extraction (e.g., boron in reference laboratory R(A-C)). Regardless of the source, contamination from external sources was seen as a potential influence on the validation statistics especially when extract concentrations were low.

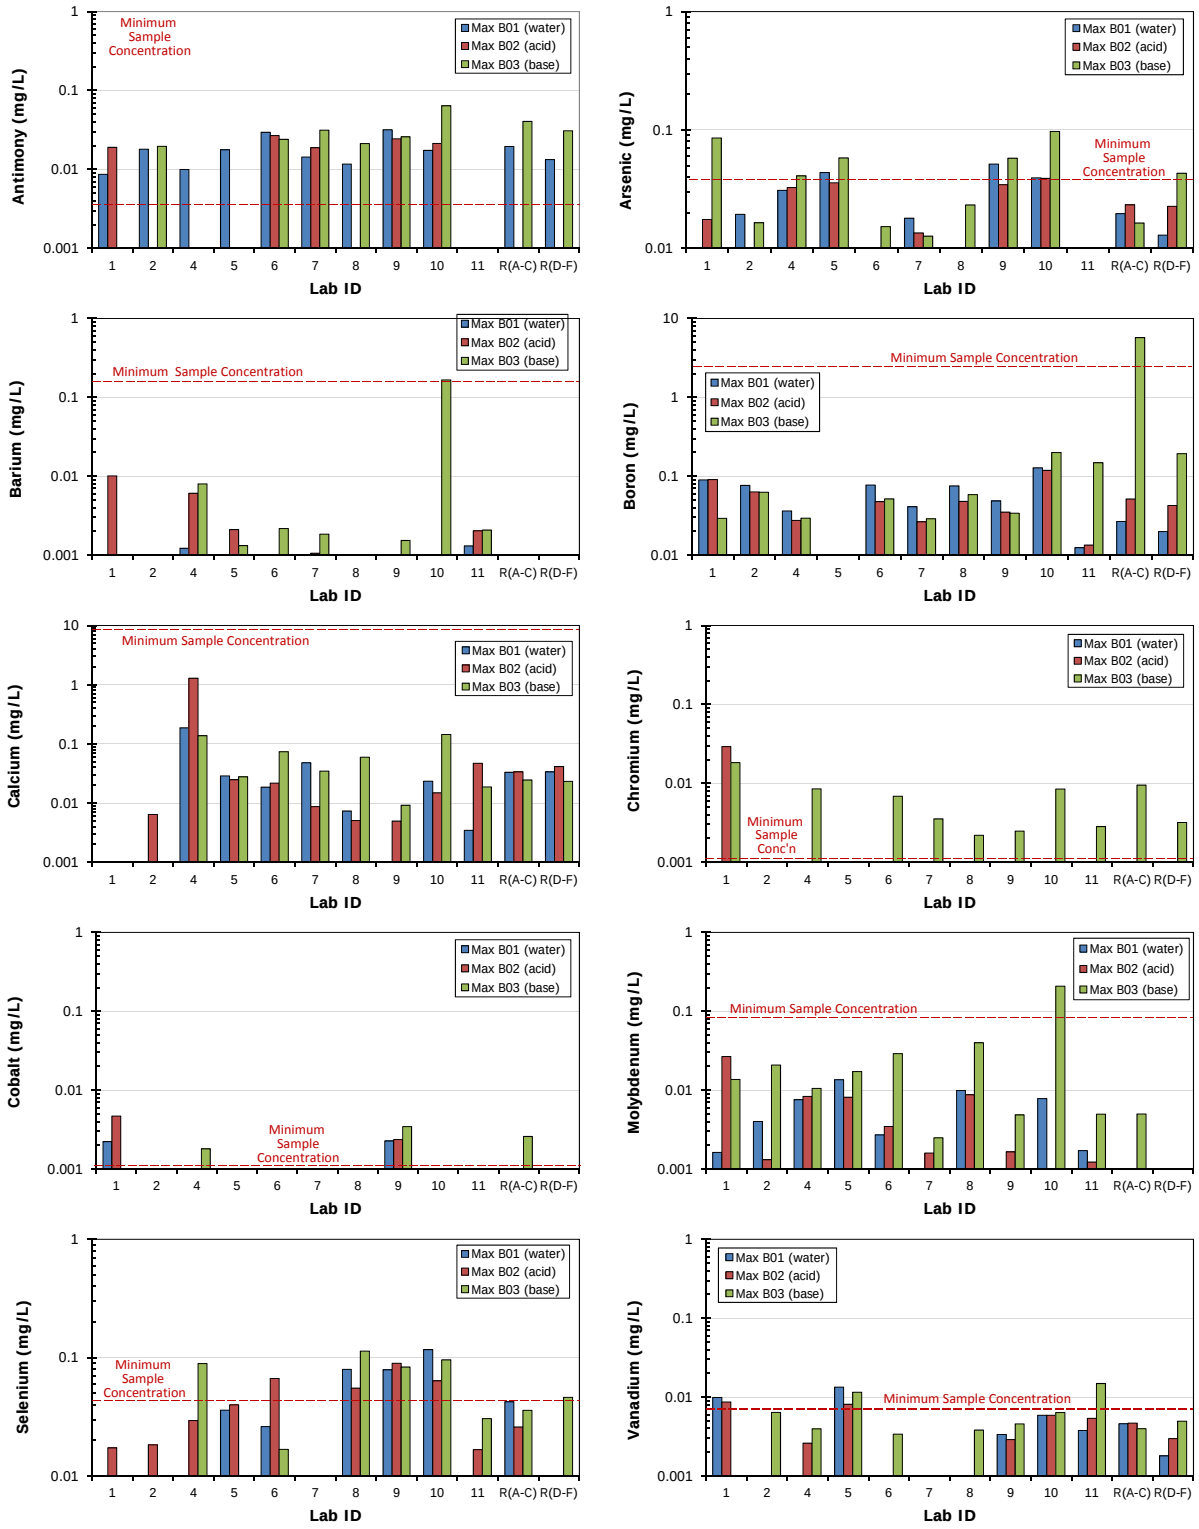

Figure 1. Maximum method blank concentrations for Method 1313 Phase I EaFA material. Note: B01 refers to method blank of reagent water, B02 refers to method blank of reagent water with the highest level of acid addition, and B03 refers to method blank of reagent water with the highest level of base addition. All solutions were preserved for chemical analysis with Optima grade nitric acid at 1% (v/v).

Phase I Data Filtering

An algorithm was developed to filter (remove) data from the data set if the concentration of an analyte in the corresponding blank was greater than 20 percent of the measured concentration in the test method eluate. This data filtering process was conducted to avoid confounding statistical analysis of the test results in analytical solutions where background contamination (e.g., through reagent water or acid/base reagents) represents a significant portion of the measured concentration. Table 1 presents the pH and replicates of data that did not pass the algorithm for checking blank concentrations to measured concentration values.

Filtering for Cause

Some data was filtered due to interferences introduced to the data set through procedural mistakes or laboratory practices. These interferences are not shown directly through blank analysis, but are identified by reviewing the collected data as a whole and through analysis of measured concentrations over the spectrum on ICP-OES analytes. Data sets where known causes of Method 1313 interferences were identified were filtered for cause. The following observations and data filtrations were made:

- Measured concentrations of boron from reference lab test samples and method blanks for replicate A, B and C were significantly higher that all other reported data. After discussion of reagent storage protocols with the laboratory representative, the source of boron concentration in the test samples was determined to come from storage of strong base reagents in borosilicate glass containers. Therefore, the boron data for pH 13 from the reference laboratory replicates A-C was filtered from the overall data set.

- High sulfur concentrations were measured in all Laboratory 4 method blanks (e.g., L04 acid, base and deionized water blanks). Sulfur contamination could result in interference with barium determinations in analytical samples due to precipitation of $BaSO_4$. Further check showed that all test solutions from L04 had similar sulfur concentrations. Therefore, all L04 Ba results were filtered for cause.

Table 1. Table of Filtered Test Positions Based on Blank Concentrations (20% critical value)

	Arsenic		Boron		Cobalt		Chromium		Molybdenum		Antimony		Selenium	
Lab ID	**pH**	**Reps**	**pH**	**Reps**	**pH**	**Reps**	**pH**	**Reps**	**pH**	**Reps**	**pH**	**Reps**	**pH**	**Reps**
Lab-01					8.0	A, B	5.5 4.0	A A	4.0	C	4.0	A, B, C		
Lab-02													4.0	B
Lab-04	7.0 5.5 4.0	A, B, C A, C A, C				A	5.5	B					4.0	A, B, C
Lab-05	8.0 7.0 5.5 4.0	A, B, C A, B, C A, B, C A, B, C	9.0		9.0	B, C					5.5 4.0 2.0	A,B,C C A	4.0	A, B, C
Lab-06					8.0	B, C	5.5	B			7.0 5.5 4.0	B B, C A, B, C A, B	4.0	A, B, C
Lab-07	7.0 5.5	B A			8.0	B	5.5	C	8.0		5.5 4.0	A, B, C A, B A, B, C		
Lab-08					8.0	B, C	5.5	A, C					4.0	A, B, C
Lab-09	8.0 7.0 5.5 4.0	A, B, C A, B, C A, B, C A, B, C			9.0 8.0	B, C B, C B	5.5	A	12.0		5.5 4.0 2.0	A, C A, B, C A, B, C A, B	5.5 4.0	A, B, C A, B, C
Lab-10	8.0 7.0 5.5 4.0	A, B, C A, B, C A, B, C A, B, C	10.5		9.0	A, B	7.0 5.5	A B	7.0 13.0		12.0 5.5 4.0 2.0	A, B, C A, B, C A, C A, B, C B, C	7.0 5.5 4.0	A A, B, C A, B, C
Lab-11					8.0	B, C							4.0	A, B, C
Ref	7.0 5.5 4.0	A, B, C, F A, B, C, D, F A, B, C, D, E, F	13.0 12.0	A, B, C A, B, C	8.0	B, C, D, E, F	5.5	A, C	13.0		12.0 5.5 4.0	A, B, C A, B, C, D, E, F A, B, C, D, E, F B	5.5 4.0	C A, B, C

Effect of Phase I Data Filtering on Statistical Analysis

The overall effect of data filtering on the number of observations available for statistical analysis is shown in Tables 2 by analyte and Table 3 by pH target point. These tables provide a summary of filtered values including the number of observations used in statistical analysis for each analyte and each target pH value.

Table 2. Data Point Summary by Analyte after Blank Filtering and Filtering for Cause.

By Analyte	As	B	Ba	Ca	Co	Cr	Mo	Sb	Se	V
Collected	324	324	324	324	324	324	324	324	324	324
Filtered	60	6	27	0	24	12	1	63	33	0
Used in Analysis	264	318	297	324	300	312	323	261	291	324

Table 3. Data Point Summary by Analyte and Target pH after Blank Filtering and Filtering for Cause.

By Target pH	As	B	Ba	Ca	Co	Cr	Mo	Sb	Se	V
Collected @ pH	36	36	36	36	36	36	36	36	36	36
13.0	36	33	33	36	36	36	36	30	36	36
12.0	36	33	33	36	36	36	36	24	36	36
10.5	36	36	33	36	34	36	36	36	36	36
9.0	36	36	33	36	29	36	36	36	36	36
8.0	27	36	33	36	21	36	36	35	36	36
7.0	19	36	33	36	36	35	36	32	35	36
5.5	19	36	33	36	36	26	36	17	29	36
4.0	19	36	33	36	36	35	35	20	11	36
2.0	36	36	33	36	36	36	36	31	36	36
Sum	264	318	297	324	300	312	323	261	291	324

Subsequent to data filtering, statistical analysis was carried out on both unfiltered and filtered data to determine the impact of data filtering on final results and conclusions. The impact of the overall effect of filtering data is illustrated by comparing mean-based and median-based statistics between filtered and non-filtered data sets. Figures 2 and 3 show the overall standard deviation interval about the mean (left) and 95% robust confidence interval about the median of lab means (right) for the eight analytes with data points filtered either for cause or because of blank analyses. Although filtration of arsenic data appears to have the greatest effect of all median-based statistics, the effect on mean-based statistics is on par with the other analytes. Overall, this comparison indicates that even a considerable amount of filtration has only a minor effect on statistical analysis and is unlikely to change the outcomes of the validation study. Therefore, in light of the significant effort required to filter the collected data into a filtered data set, filtration was no conducted for Method 1313 Phase II materials.

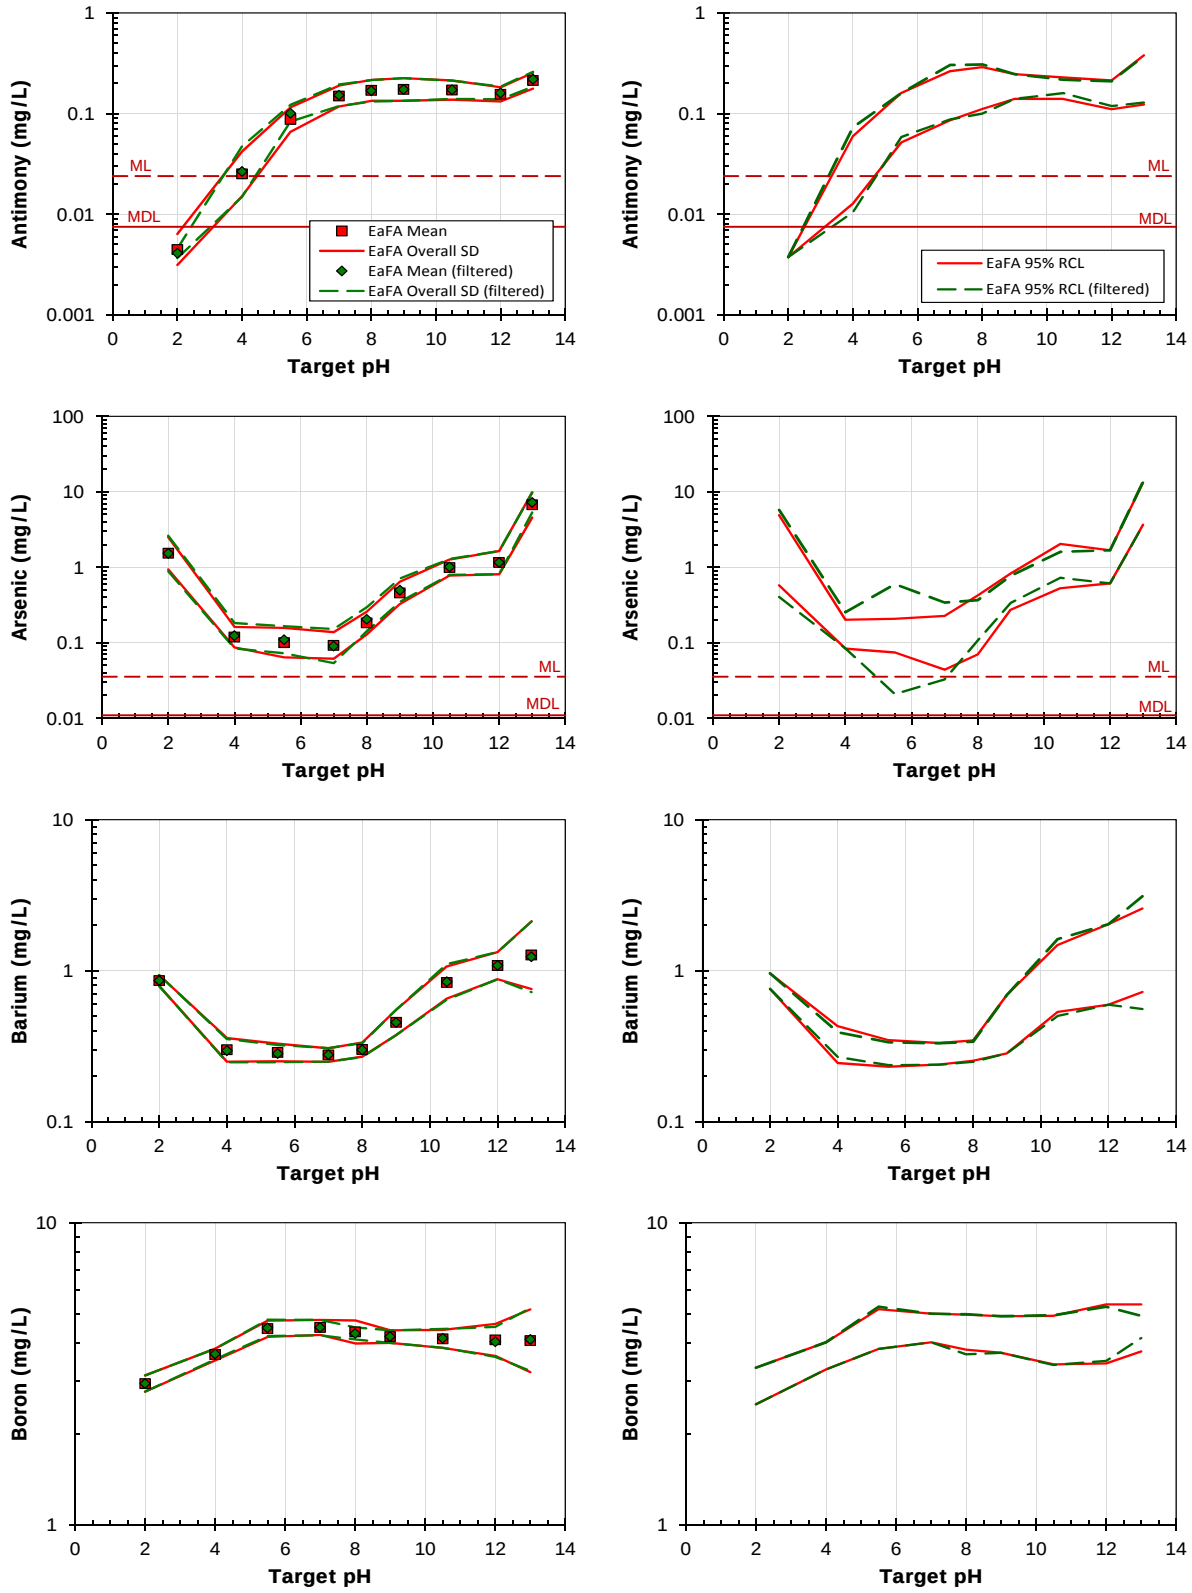

Figure 2. The effect of data filtration of Method 1313 Phase I EaFA results of mean-based (left) and median-based (right) statistical output.

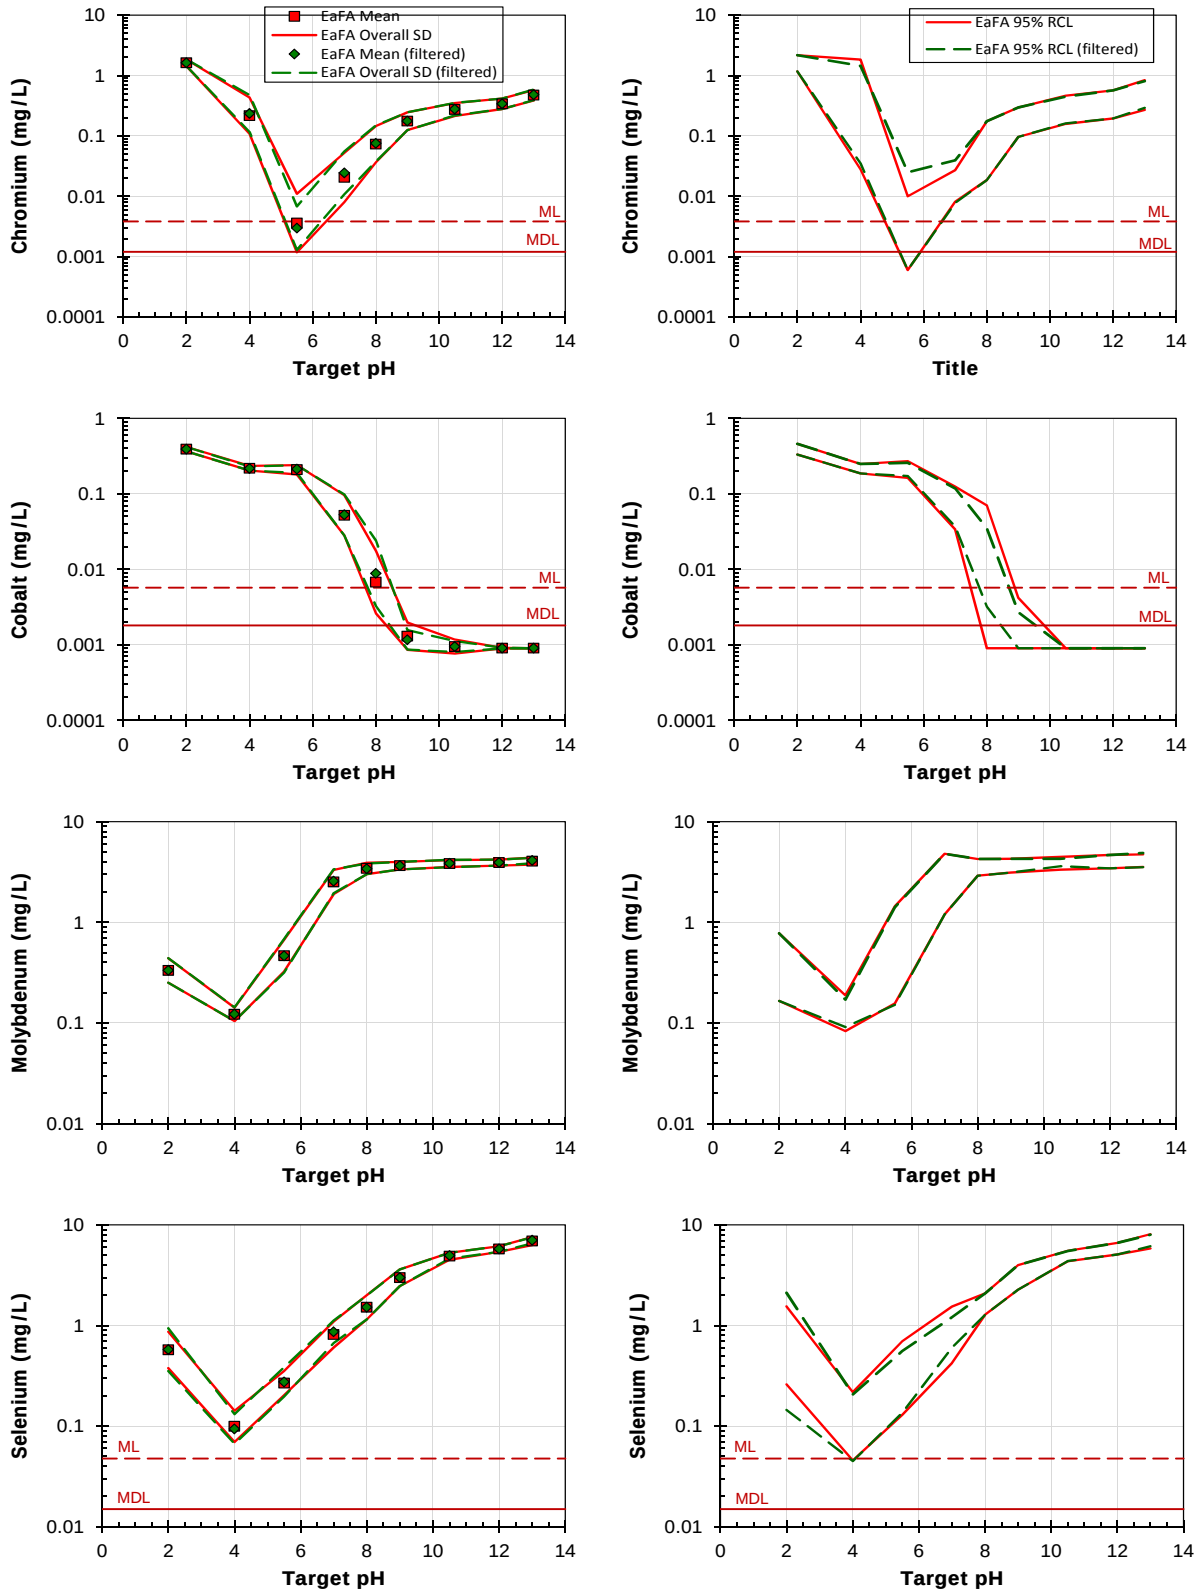

Figure 3. The effect of data filtration of Method 1313 Phase I EaFA results of mean-based (left) and median-based (right) statistical output.

Phase II Method Blanks

Recommendations of the Phase I study were that participating laboratories advancing to Phase II were asked to monitor their supply of reagent water and ensure that reagents were freshly prepared. As a result, the number of maximum blank concentrations above detection limits for Phase II SWA material (Figure 4) and CFS (Figure 5) were considerably less than in Phase II. Although no filtration based on method blank analysis was conducted, the presentation of maximum method blank concentrations shown in Figures 4 and 5 infer that very little filtration would have been necessary and any potential impact of statistical analysis these materials would be less than that seen in Phase I.

Phase II Data Filtering

For Method 1313 Phase II SWA material, one test position from each of two participating laboratories was filtered due to inconsistent pH values. All three replicates of test position T03 for L02 and T05 for L05 were filtered for cause. Based on the conclusion of the comparison of filtered versus non-filtered data conducted for Phase I, presentation of filtered versus non-filtered statistics for this minor data filtering was not warranted.

No data was filtered for cause for the Phase II CFS material.

Method 1313 Filtration Summary

Based on the above analyses, the final filtration scheme for Method 1313 data is shown in Table 4. With the exception of these data, all collected data was used in the statistical analysis for validation of Method 1313.

Table 4 Final Filtered Data for Method 1313 Statistical Analysis.

Material	Filtered Data
EaFA	• All L04 barium data (high sulfur) • Boron for reference lab pH 13 (base storage)
SWA	• L02 T03 replicates A, B, and C (pH) • L05 T05 replicates A, B, and C (pH)
CFS	None

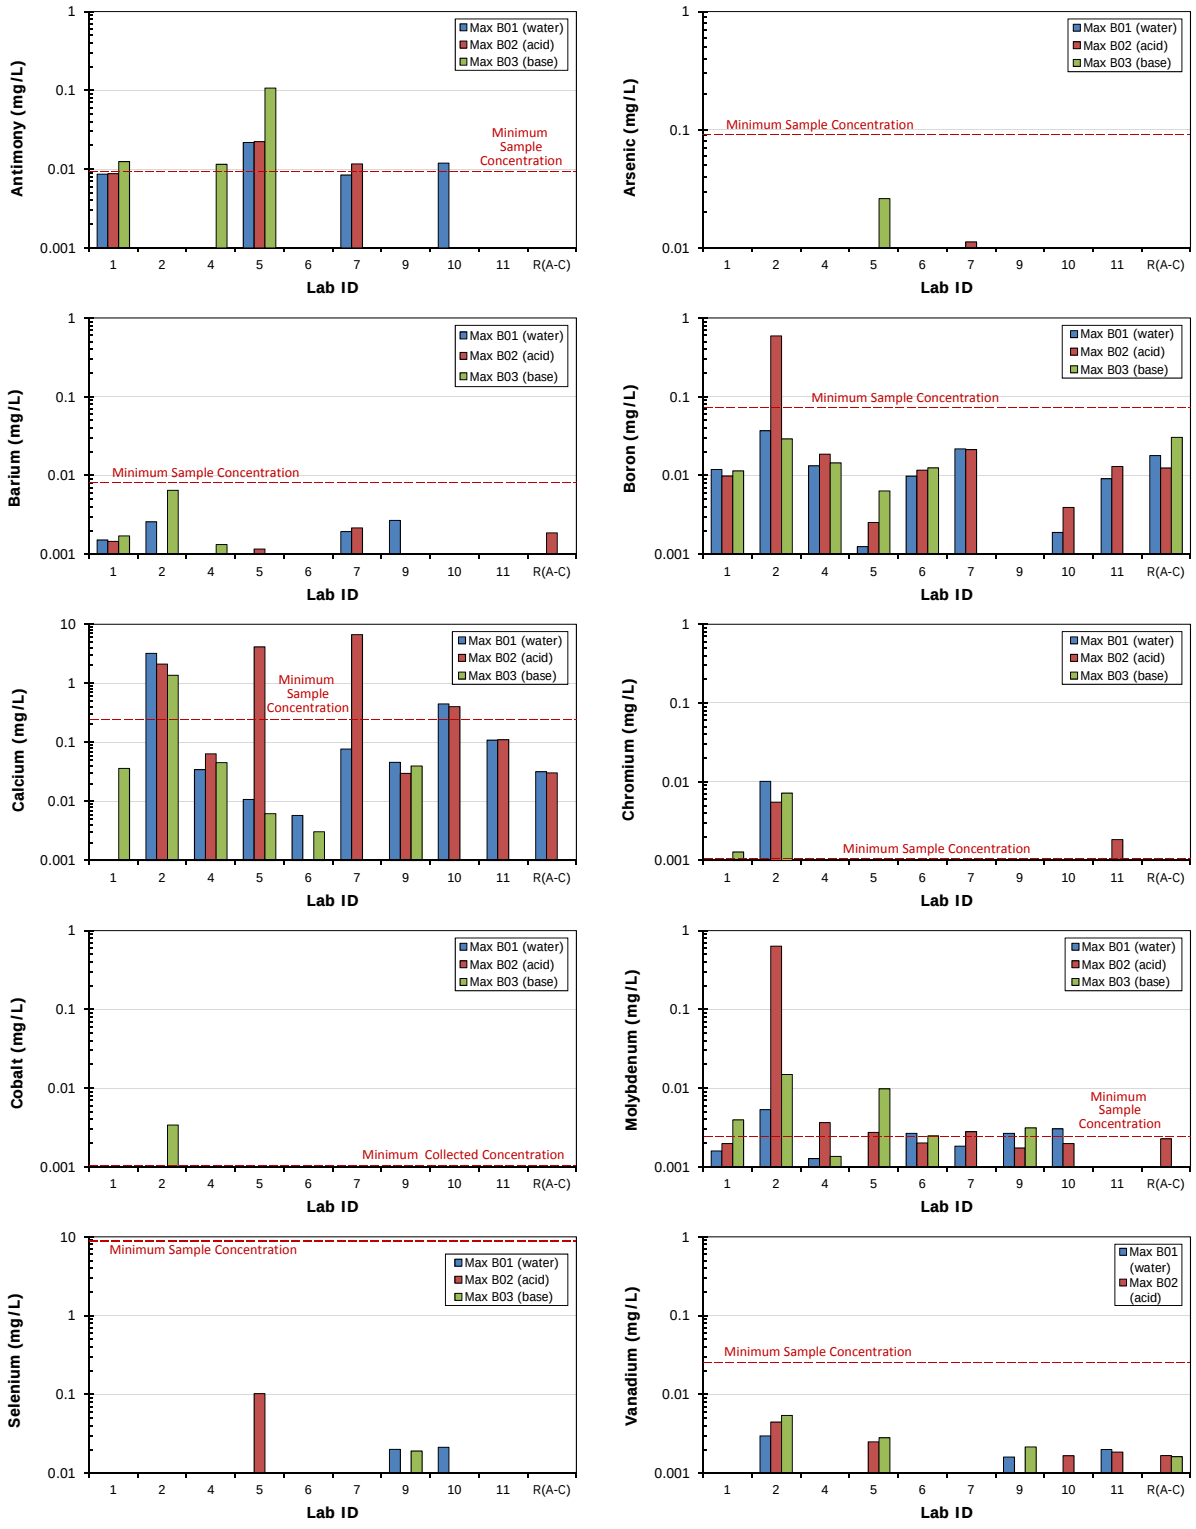

Figure 4. Maximum method blank concentrations for Method 1313 Phase II SWA material. Note: B01 refers to method blank of reagent water, B02 refers to method blank of reagent water with the highest level of acid addition, and B03 refers to method blank of reagent water with the highest level of base addition. All solutions were preserved for chemical analysis with Optima grade nitric acid at 1% (v/v)**.**

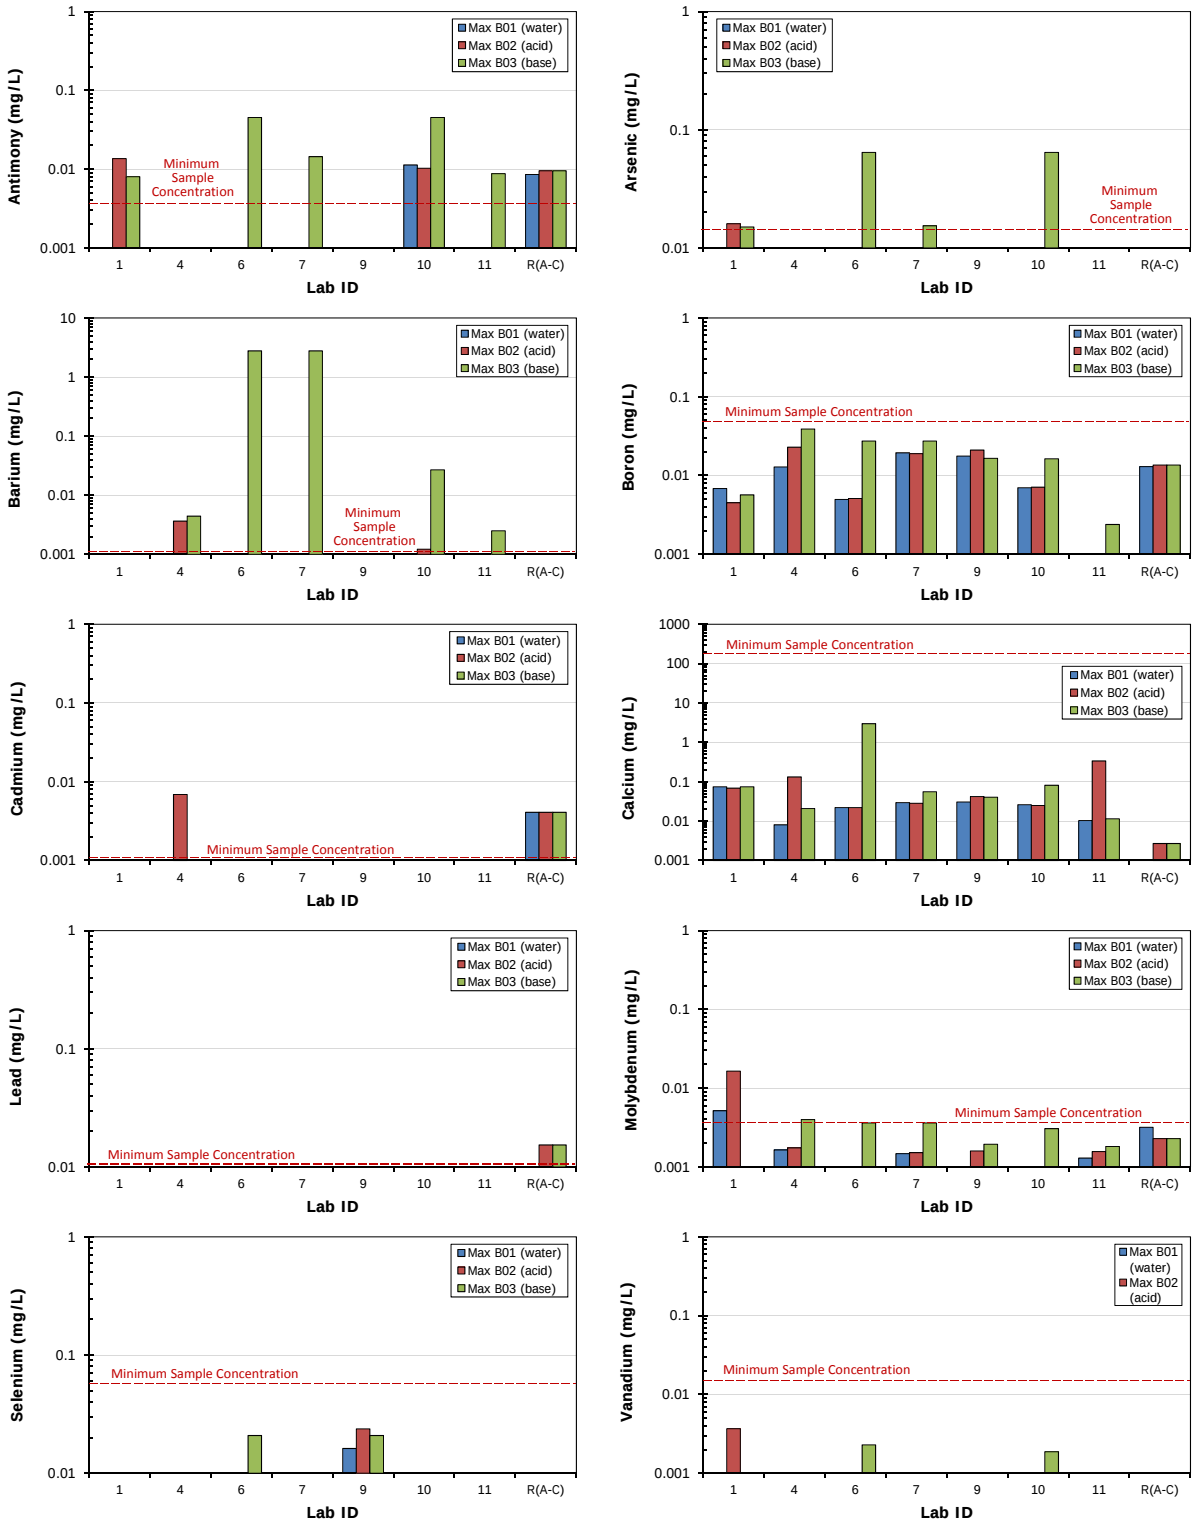

Figure 5. Maximum method blank concentrations for Method 1313 Phase II CFS material. Note: B01 refers to method blank of reagent water, B02 refers to method blank of reagent water with the highest level of acid addition, and B03 refers to method blank of reagent water with the highest level of base addition. All solutions were preserved for chemical analysis with Optima grade nitric acid at 1% (v/v).

METHOD 1316 METHOD BLANKS AND DATA FILTERING

Phase I Method Blanks

Since the solid material in Method 1316 is contacted only with reagent water, the single method blank for each replicate of the test is a reagent water sample carried through the extraction process. Method blanks for Phase I EaFA material are shown in Figure 6 along with the minimum test sample concentration from all participating labs. In all cases, the maximum method blank is no more than 1/10 the concentration of the minimum analytical sample, indicating that no blank filtering due to external sources of contamination would be necessary.

Phase I Data Filtering

As with Method 1313 Phase I, no data from Method 1316 Phase I on the EaFA material was filtered due to the method blank analysis. However, inspection of the collected data from all participating laboratory highlighted instances where pH measurement of eluates affects the concentration results of the Method 1316 data. The measured pH for all EaFA test samples is shown in Figure 7 along with examples of the degree to which variation in the recorded pH influences the concentration of analytes from the test. In the figure, three suspect data sets are highlighted with lines connecting the data in the set:

- L05 replicates A (fuchsia solid), B (fuchsia dashed) and C (fuchsia dotted)
- L10 replicate A (aqua solid)
- L11 replicates A (olive solid), B (olive dashed) and C (olive dotted)

These data sets were identified because the pH of the test replicate taken as a whole lie outside the band on the pH response of the entire dataset. However, no statistical process was taken to identify these data sets as outliers. Variations in pH are likely to be due to errors in pH meter calibration, standardization to known buffer solutions, or measurement procedure.

While the source of the pH variation is unknown, the effect of pH on the concentrations measured in Method 1316 is evident. For species where pH does not significantly affect concentration, there is little effect of pH measurement variation on the measured concentration in Method 1316 samples (see panel B in Figure 7). However, the suspect data is shown as outlying data when pH strongly influences analyte concentrations (see panels C and D in Figure 7). Given the pH data and effects shown in Figure 7, the three data sets were filtered from the data used for the statistical analysis of Method 1316.

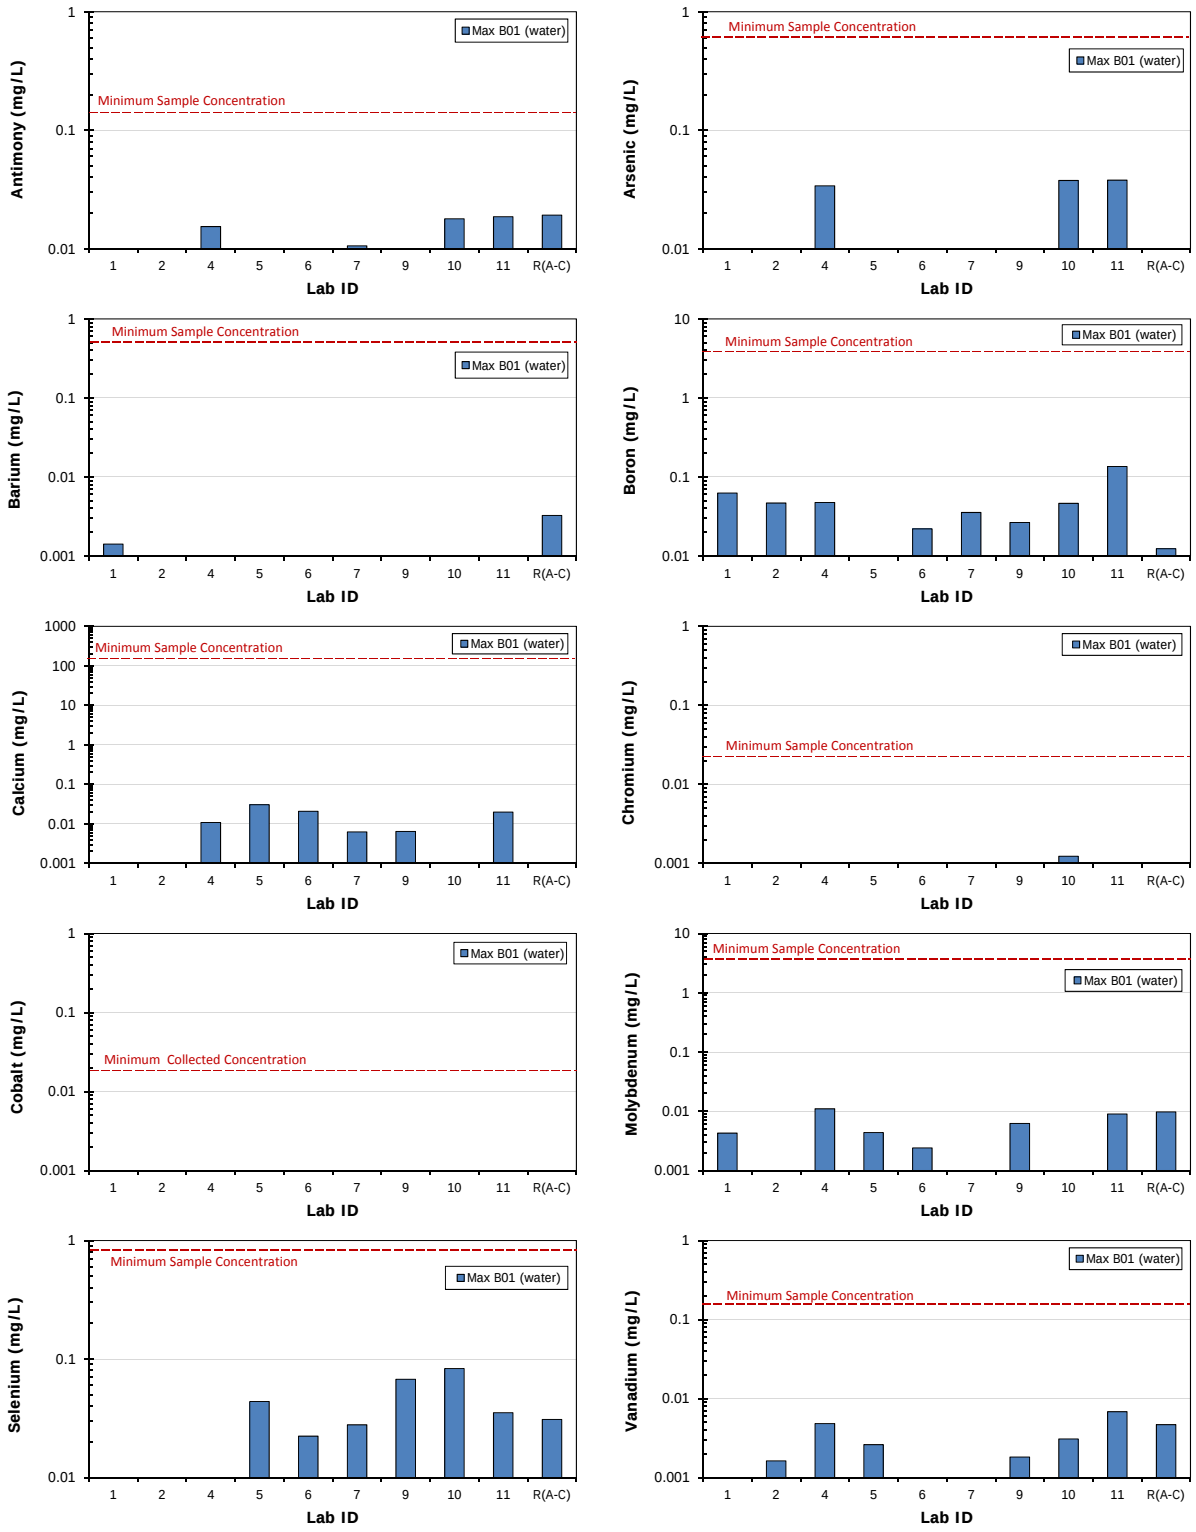

Figure 6. Maximum method blank concentrations for Method 1316 Phase I EaFA material. Note: All solutions were preserved for chemical analysis with Optima grade nitric acid at 1% (v/v)**.**

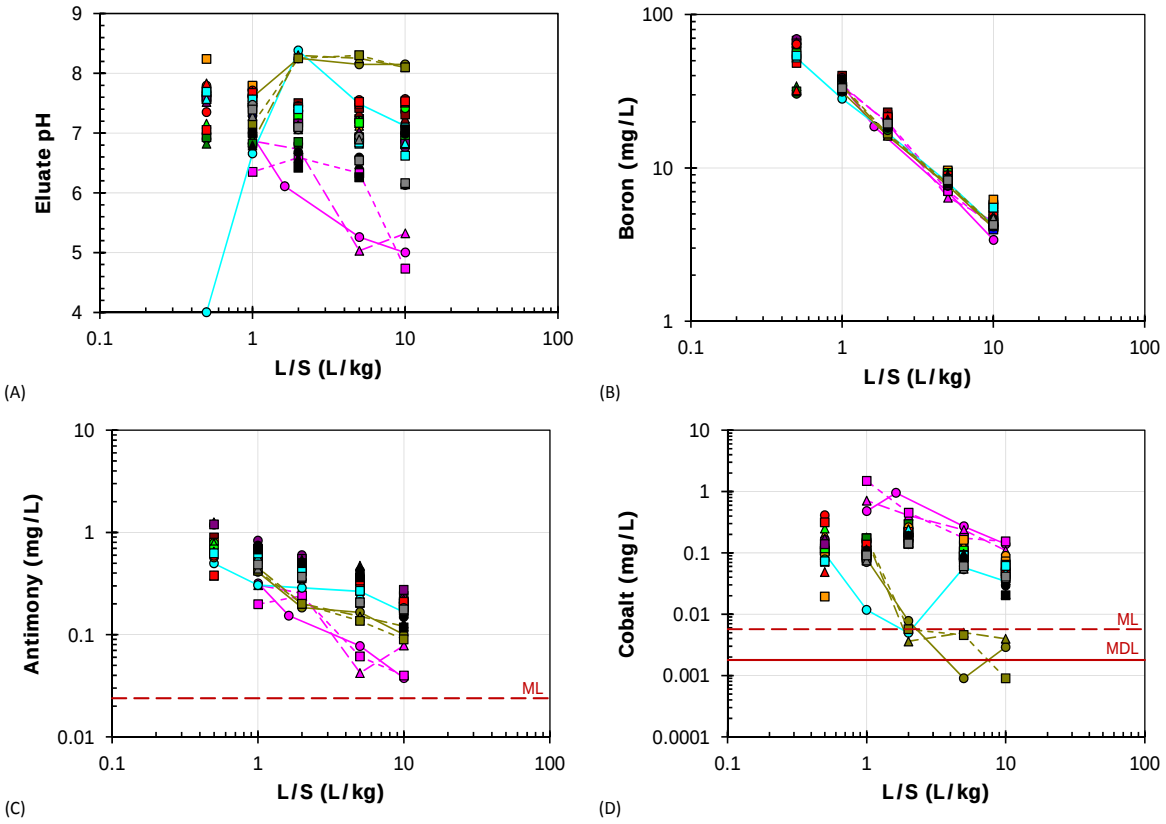

Figure 7. Effect of suspect Method 1316 pH measurement on EaFA concentration results. (A) eluate pH with lines connecting data with suspect measurements, (B) boron showing no observed effect, (C) antimony showing moderate effect, and (D) cobalt showing significant effect.

Phase II Method Blanks

Analysis of method blanks for Method 1316 Phase II SWA (Figure 8) and CFS (Figure 9) show that filtration due to blank concentrations may be warranted for a few species. For SWA, L02 methods blanks indicated calcium concentrations in excess of the minimum test sample concentration measure for all laboratories while L10 methods blanks showed a significant spike in cobalt. In method blanks for CFS, the method blanks for all laboratories with the exception of the reference laboratory had molybdenum within 1/10 of the minimum test sample concentration; however, it is unlikely that all samples would be filtered if the data was processed through the blank filtration algorithm used in Method 1313. Overall, this blank screening analysis for Method 1316 Phase II materials did not indicate that blank filtration was necessary.

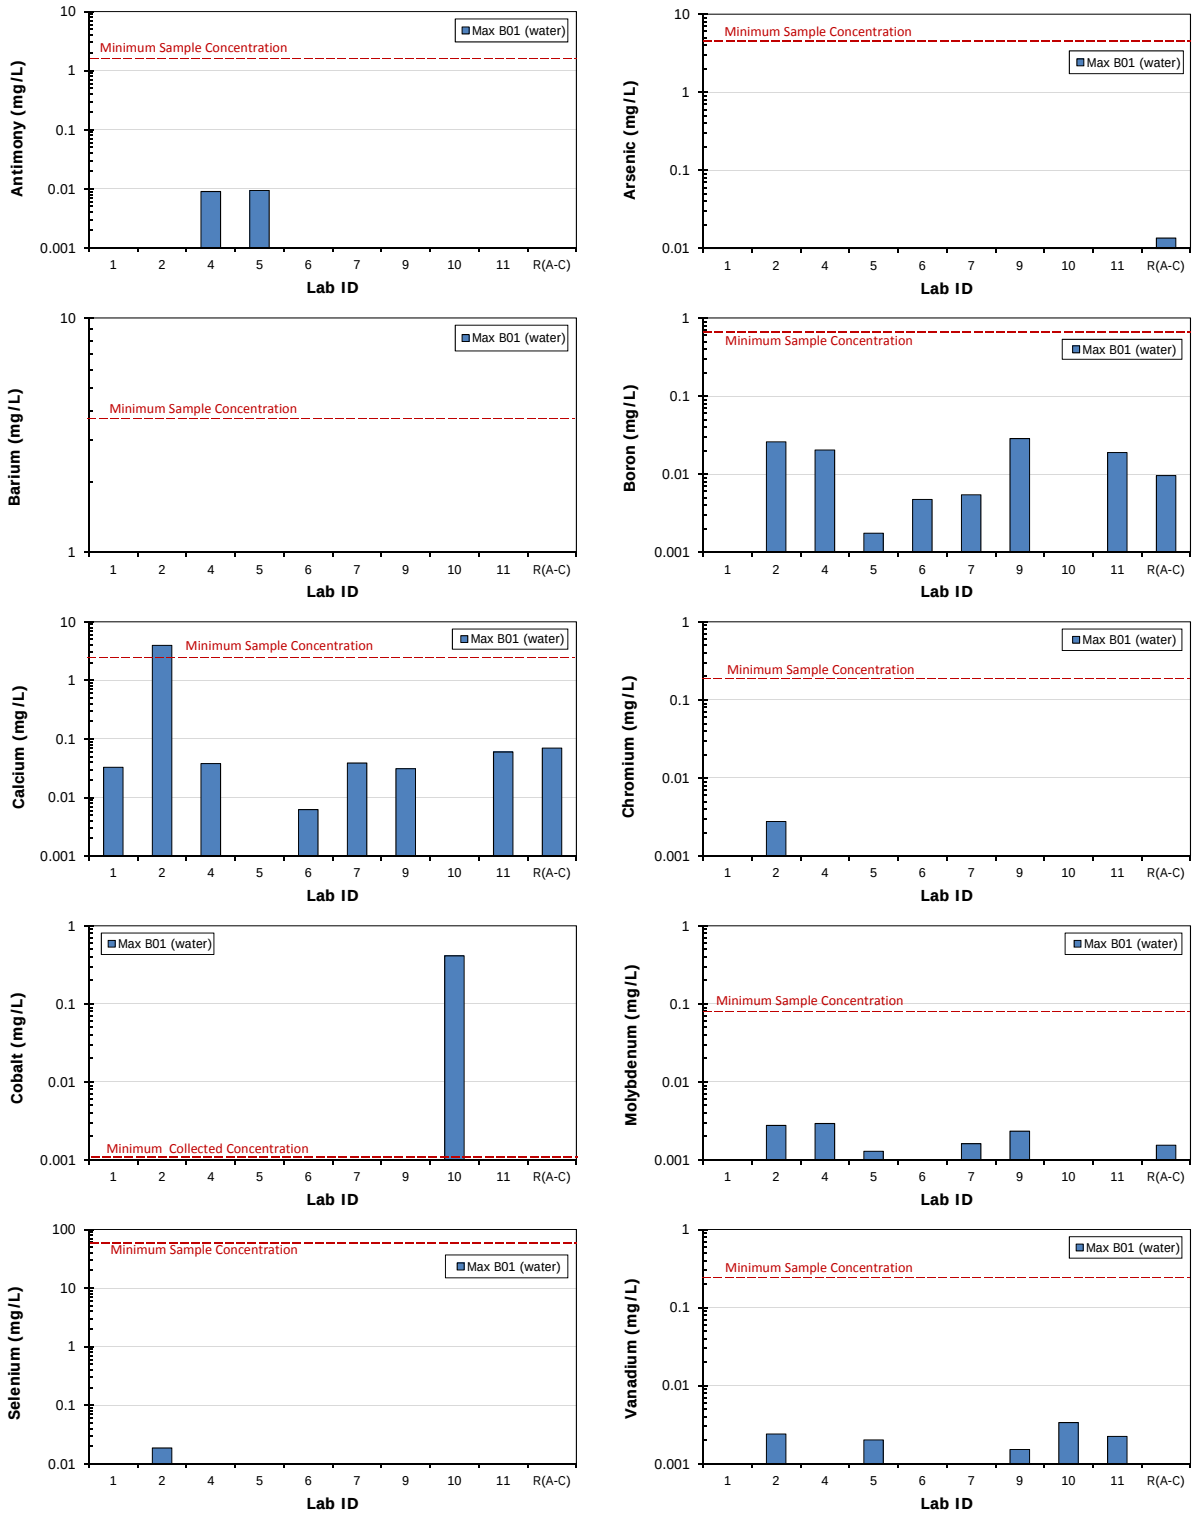

Figure 8. Maximum method blank concentrations for Method 1316 Phase II SWA material. Note: All solutions were preserved for chemical analysis with Optima grade nitric acid at 1% (v/v)**.**

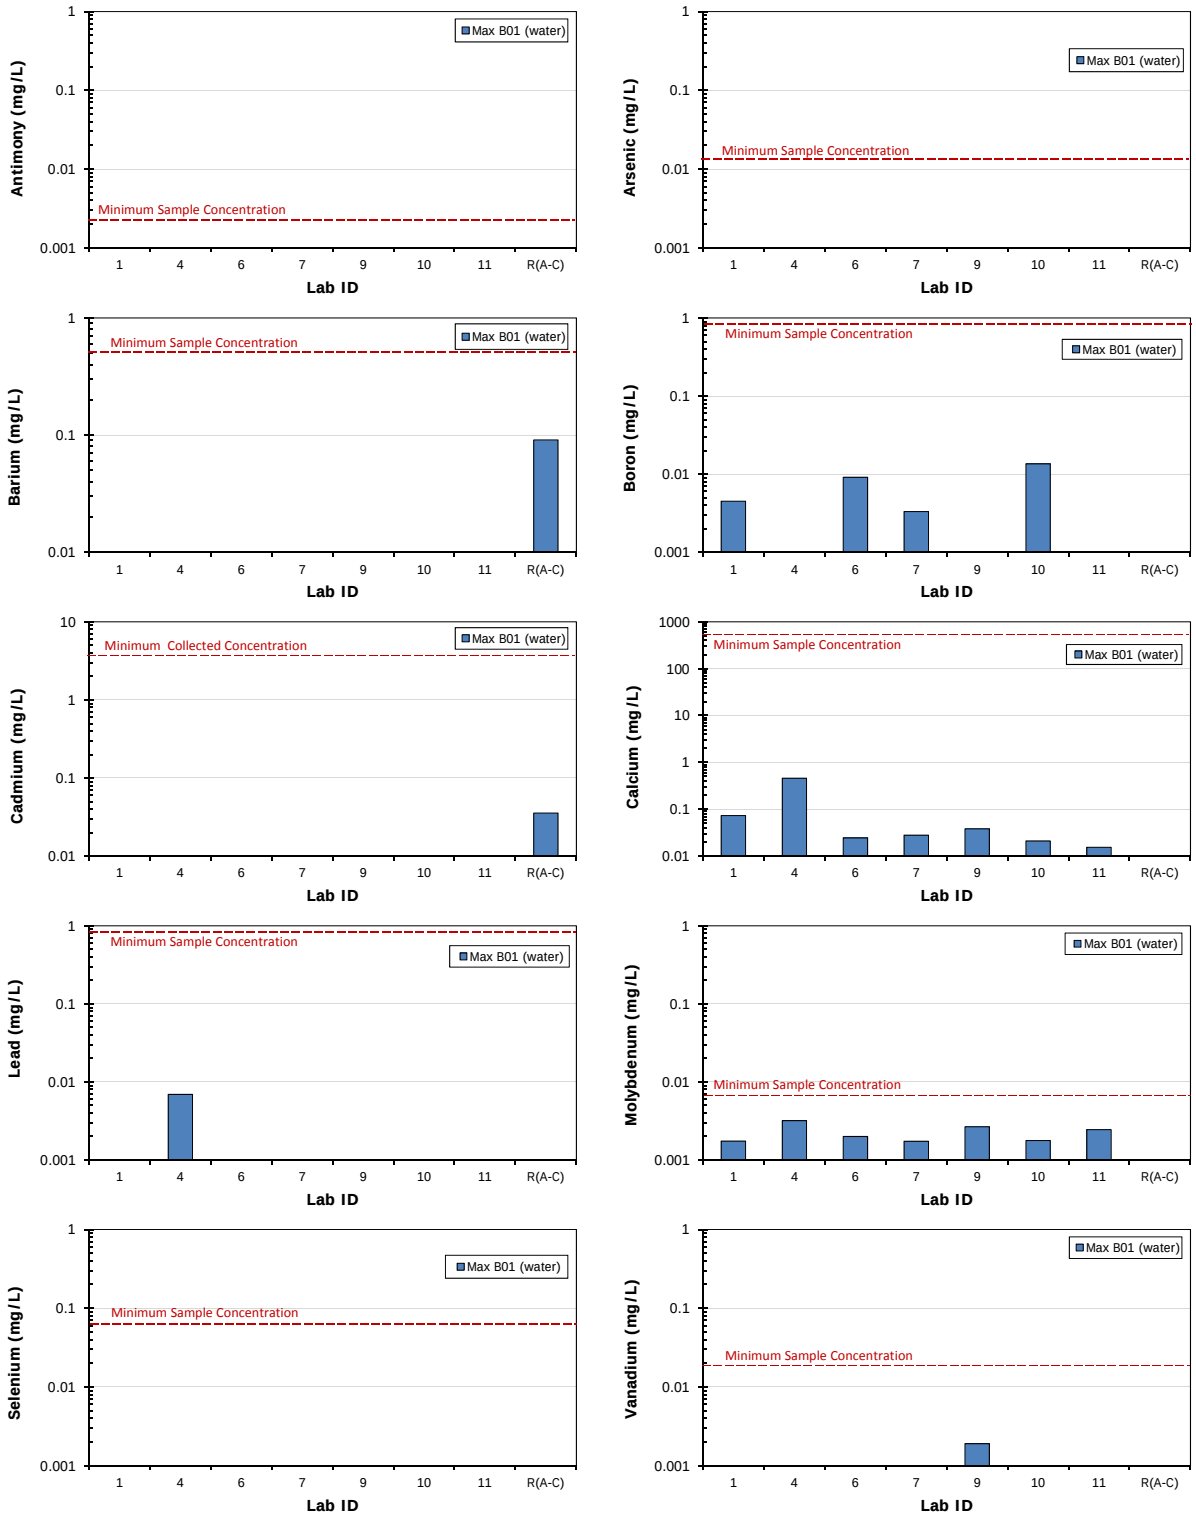

Figure 9. Maximum method blank concentrations for Method 1316 Phase II CFS material. Note: All solutions were preserved for chemical analysis with Optima grade nitric acid at 1% (v/v)**.**

Phase II Data Filtering

Although no data was filtered because of blank analysis for Method 1316 Phase II samples in either SWA or CFS materials, some data was filtered for cause. The L05 laboratory data recorded in the method data template indicated that L05 did not account for the significant amount of water entrained in the sample when conducting Method 1316. Thus, the final L/S of each extraction point is higher that would be expected and outside the specification required in the method. The shift in L/S along the horizontal axis can be seen graphically for the pink data (L05) in Figure 8.

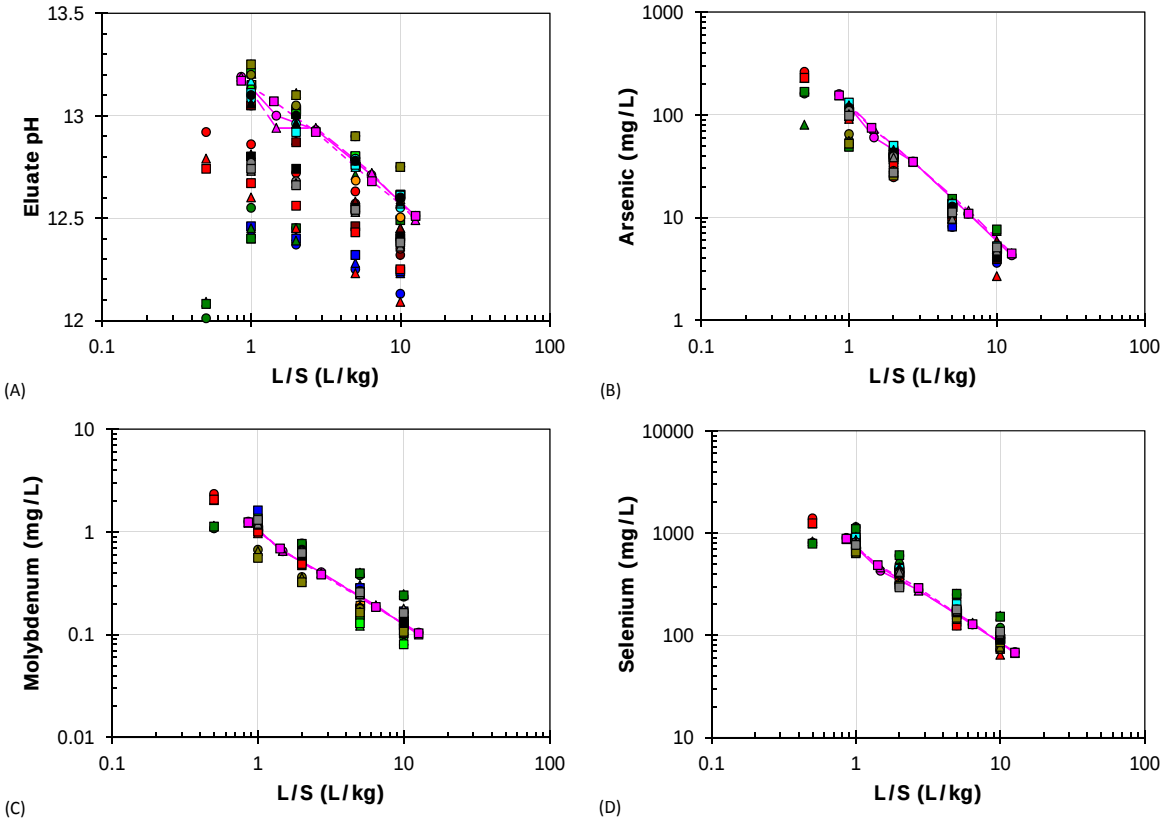

Figure 10. Effect of suspect Method 1316 L/S on SWA concentration results. (A) eluate pH with lines connecting data with suspect measurements, (B) arsenic showing no observed effect, (C) molybdenum showing no observed effect, and (D) selenium showing no observed effect.

The data in Figure 8 indicates that the shift in L/S of the L05 data does not affect the general trend of the data set for either pH or analyte concentration. Linear interpolation for the collected data to the target L/S points would result in data points consistent with the other participating laboratories. However, the L05 data was considered to not comply with the specifications of Method 1316 and, thus, the L05 data for all replicates of SWA material were filtered for cause from all analytes.

Method 1316 Filtering Summary

Based on the above analyses, the final filtration scheme for Method 1316 data is shown in Table 5. With the exception of these data, all collected data was used in the statistical analysis for validation of Method 1316.

Table 5 Final Filtered Data for Method 1316 Statistical Analysis.

Material	Filtered Data
EaFA	• L05 replicates A, B, C for all analytes (pH) • L10 replicate A for all analytes (pH) • L11 replicates A, B, and C for all analytes (pH)
SWA	• L05 replicates A, B, C for all analytes (L/S)
CFS	None

Appendix E. Method 1313 Results

TABLE OF CONTENTS

Method 1313 Statistical Analysis for Selected Analytes E-1
EaFA Fly Ash E-1
SWA Solidified Waste Analog E-11
CFS Contaminated Field Soil E-21
Method 1313 Reference Laboratory Eluate Results (ICP-OES and Supplemental Analysis) E-31
EaFA Fly Ash E-31
SWA Solidified Waste Analog E-36
CFS Contaminated Field Soil E-41
Method 1313 Repeatability and Reproducibility E-46
Material Comparison Graphs E-46
Precision Distribution Data E-54

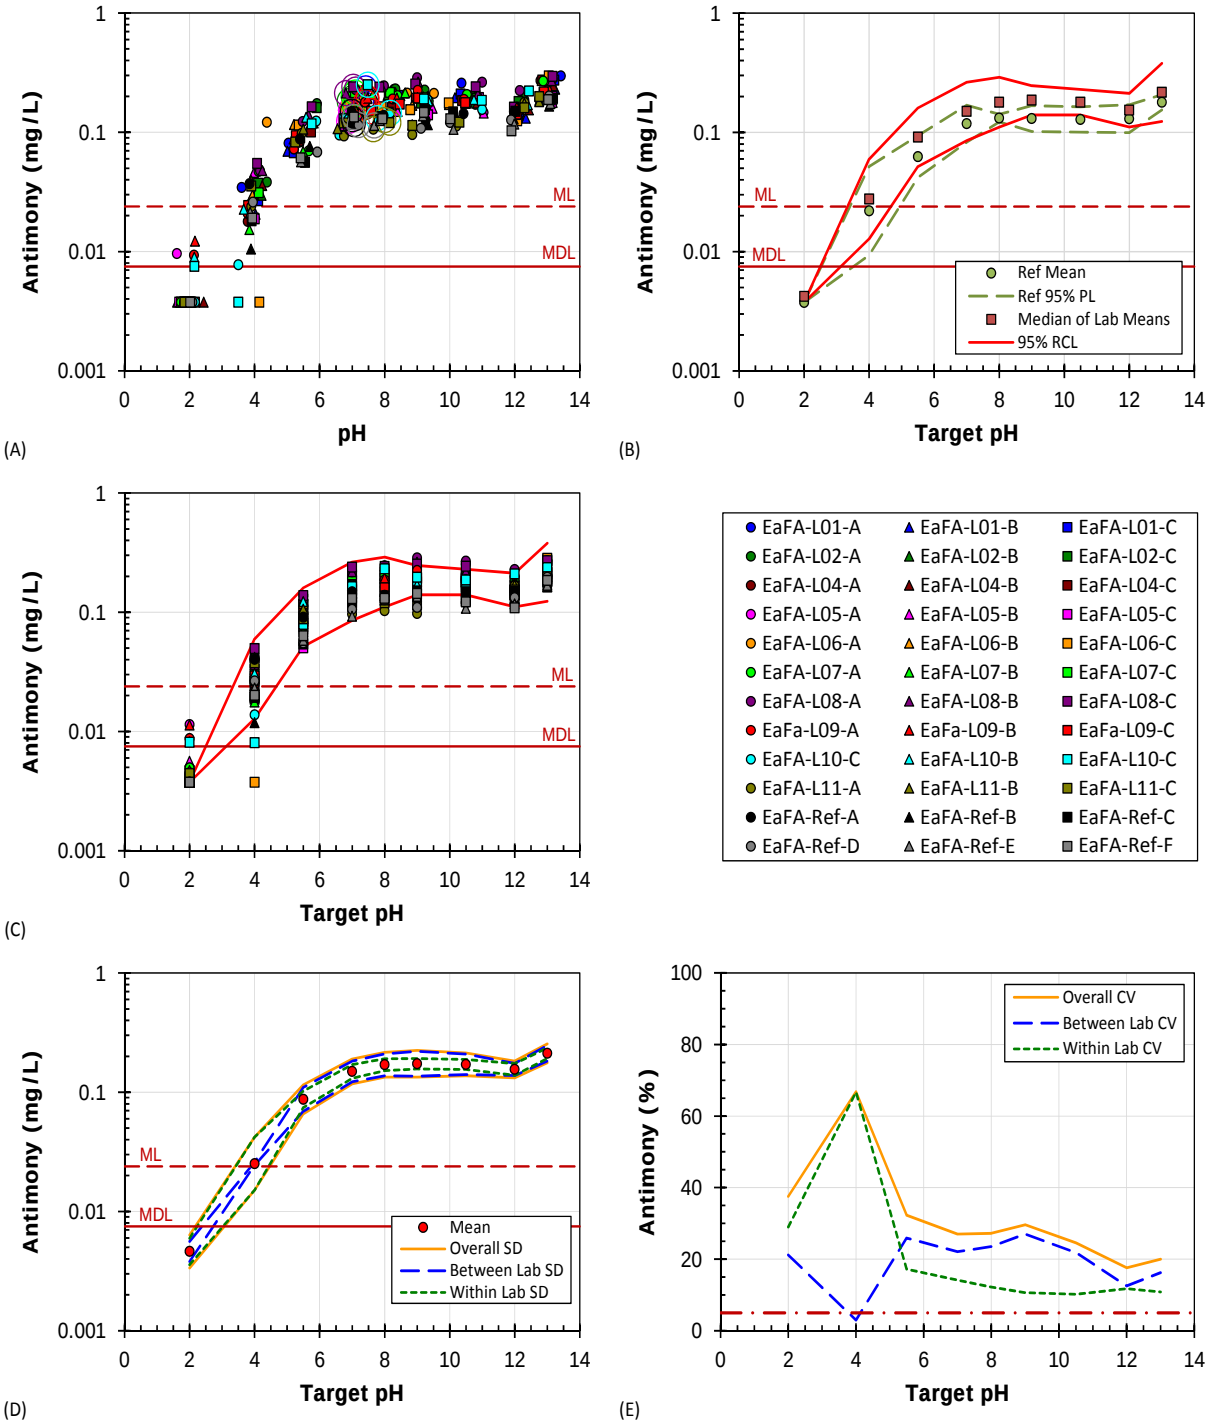

Figure 1. Antimony statistical analysis for Method 1313 Phase I material EaFA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

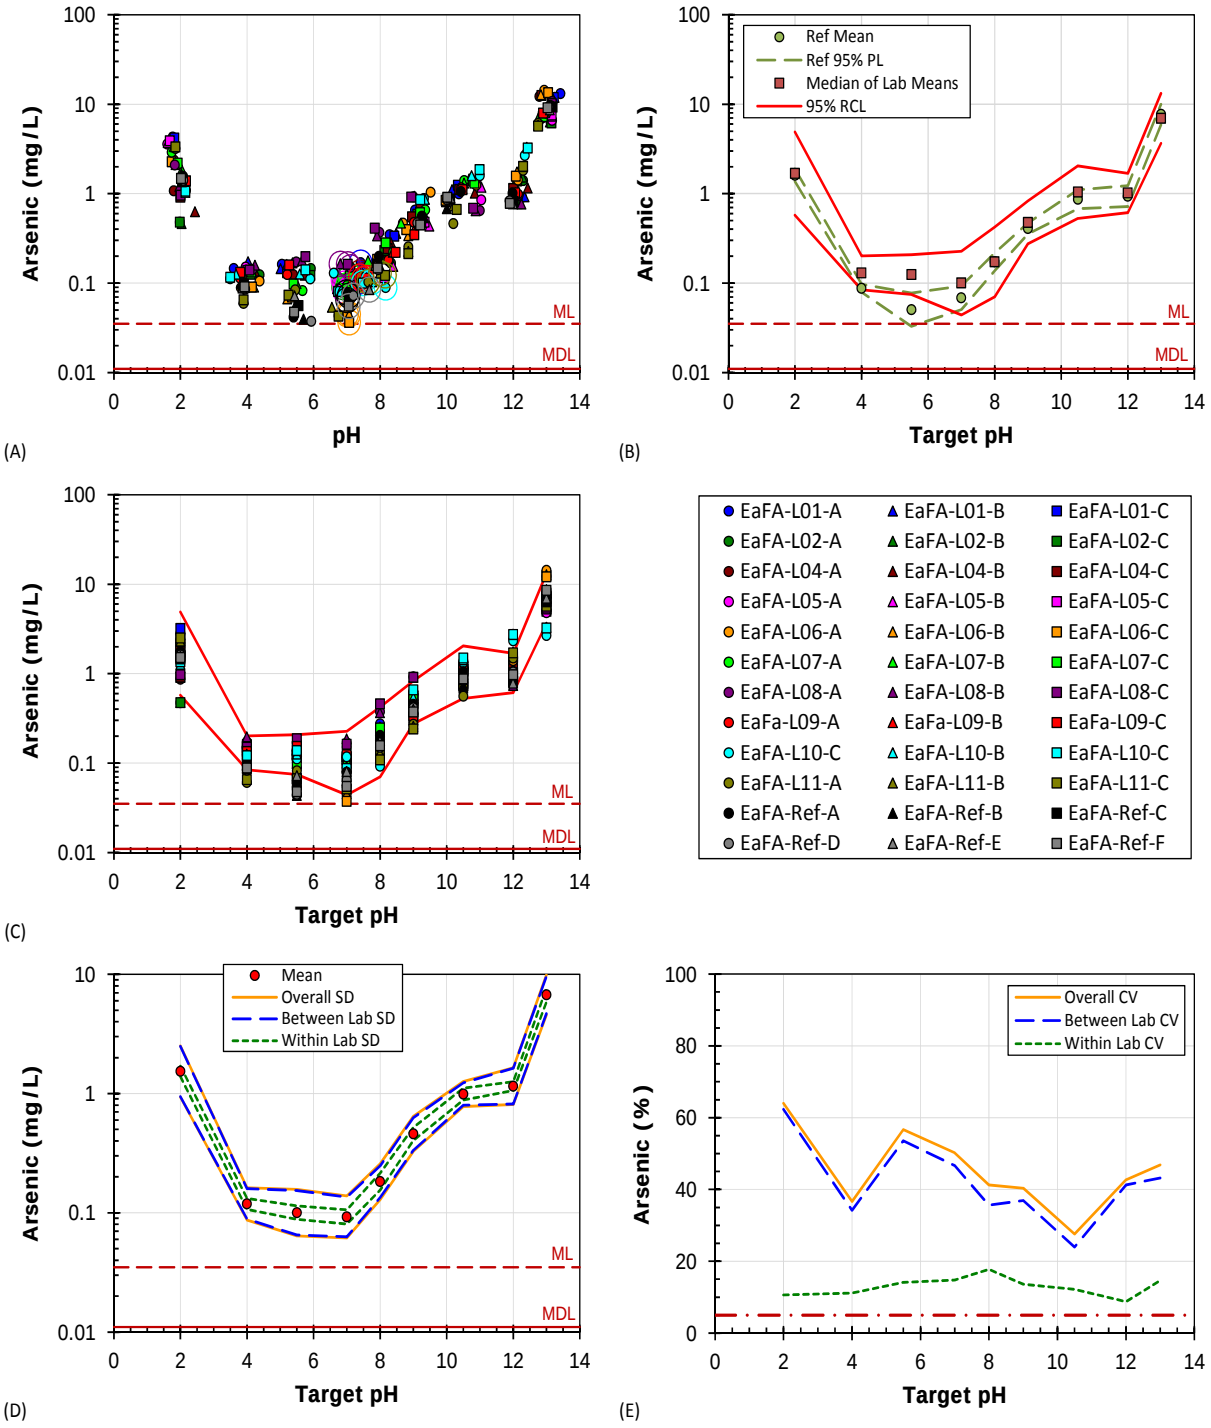

Figure 2. Arsenic statistical analysis for Method 1313 Phase I material EaFA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

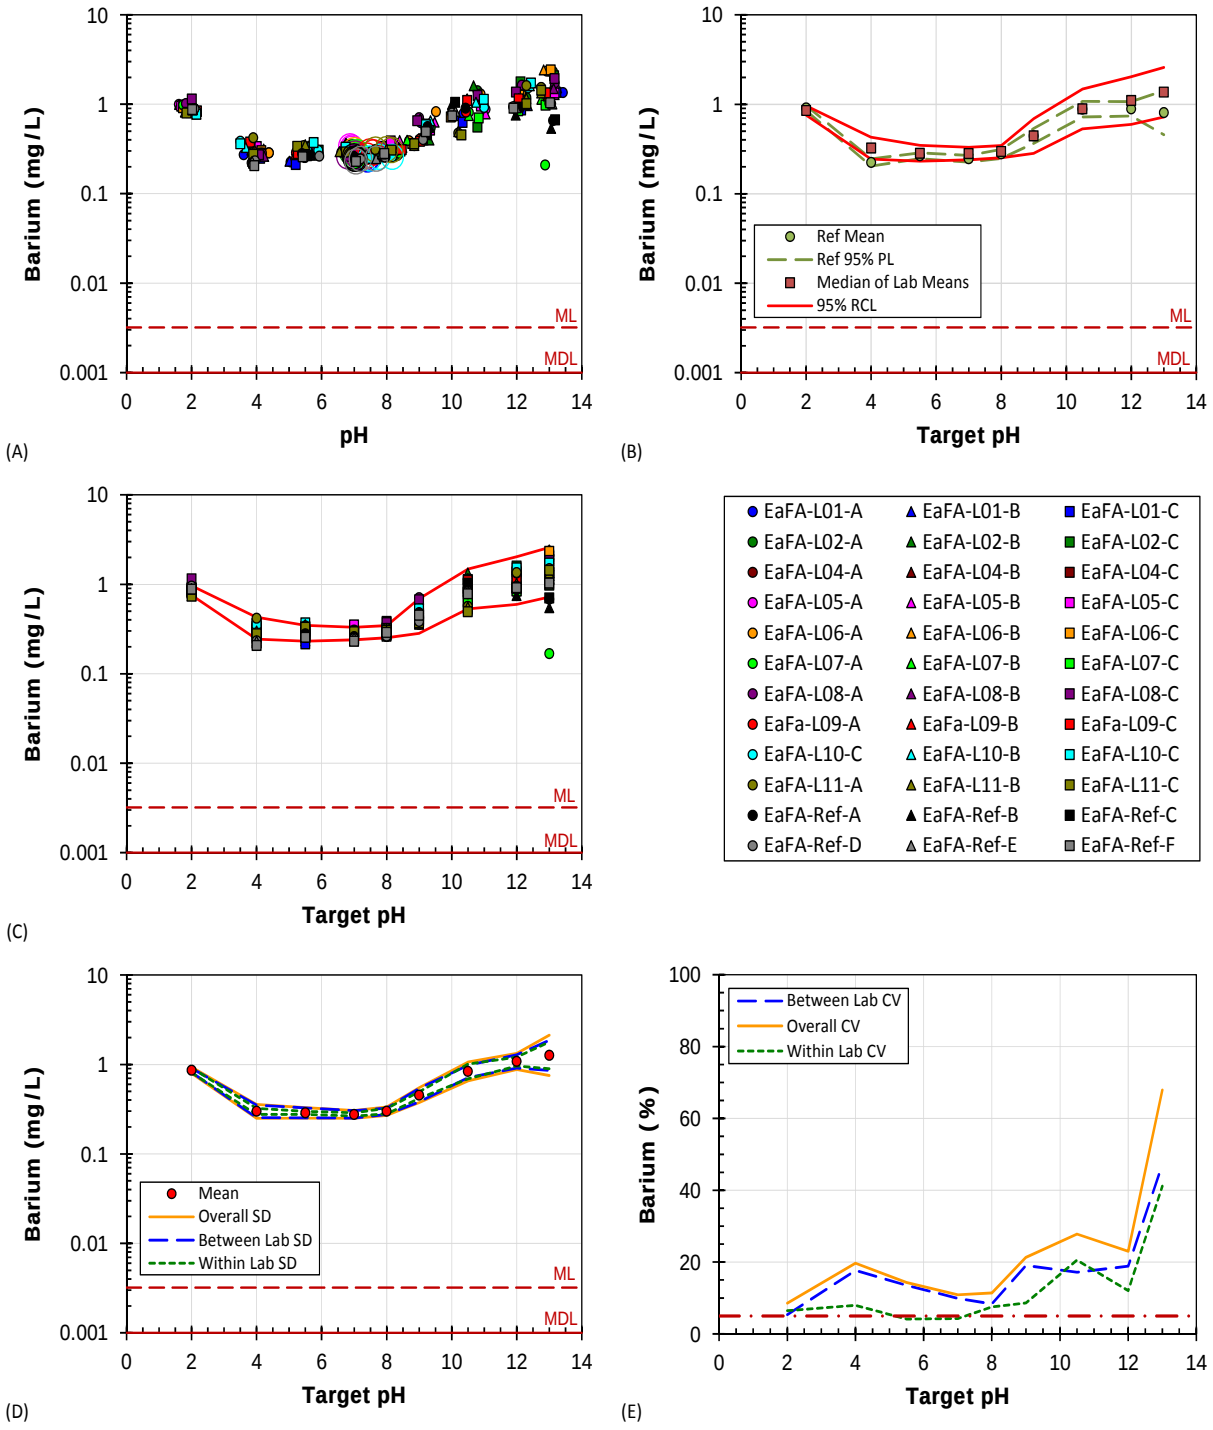

Figure 3. Barium statistical analysis for Method 1313 Phase I material EaFA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

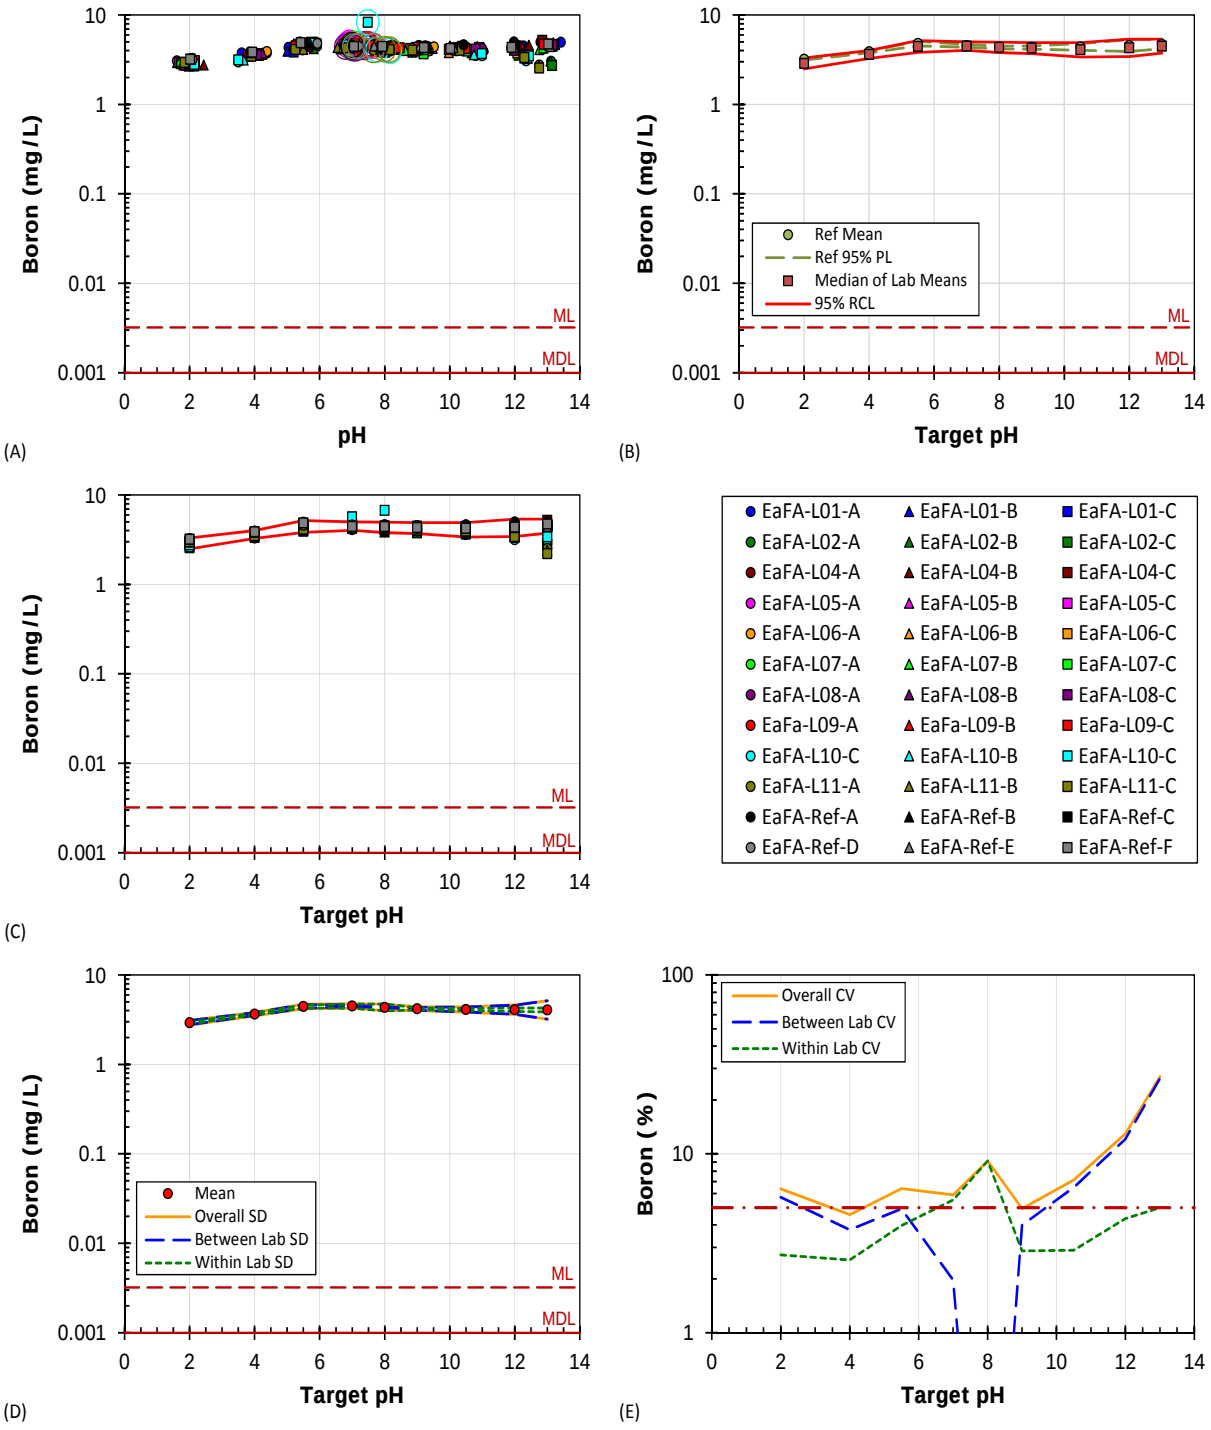

Figure 4. Boron statistical analysis for Method 1313 Phase I material EaFA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

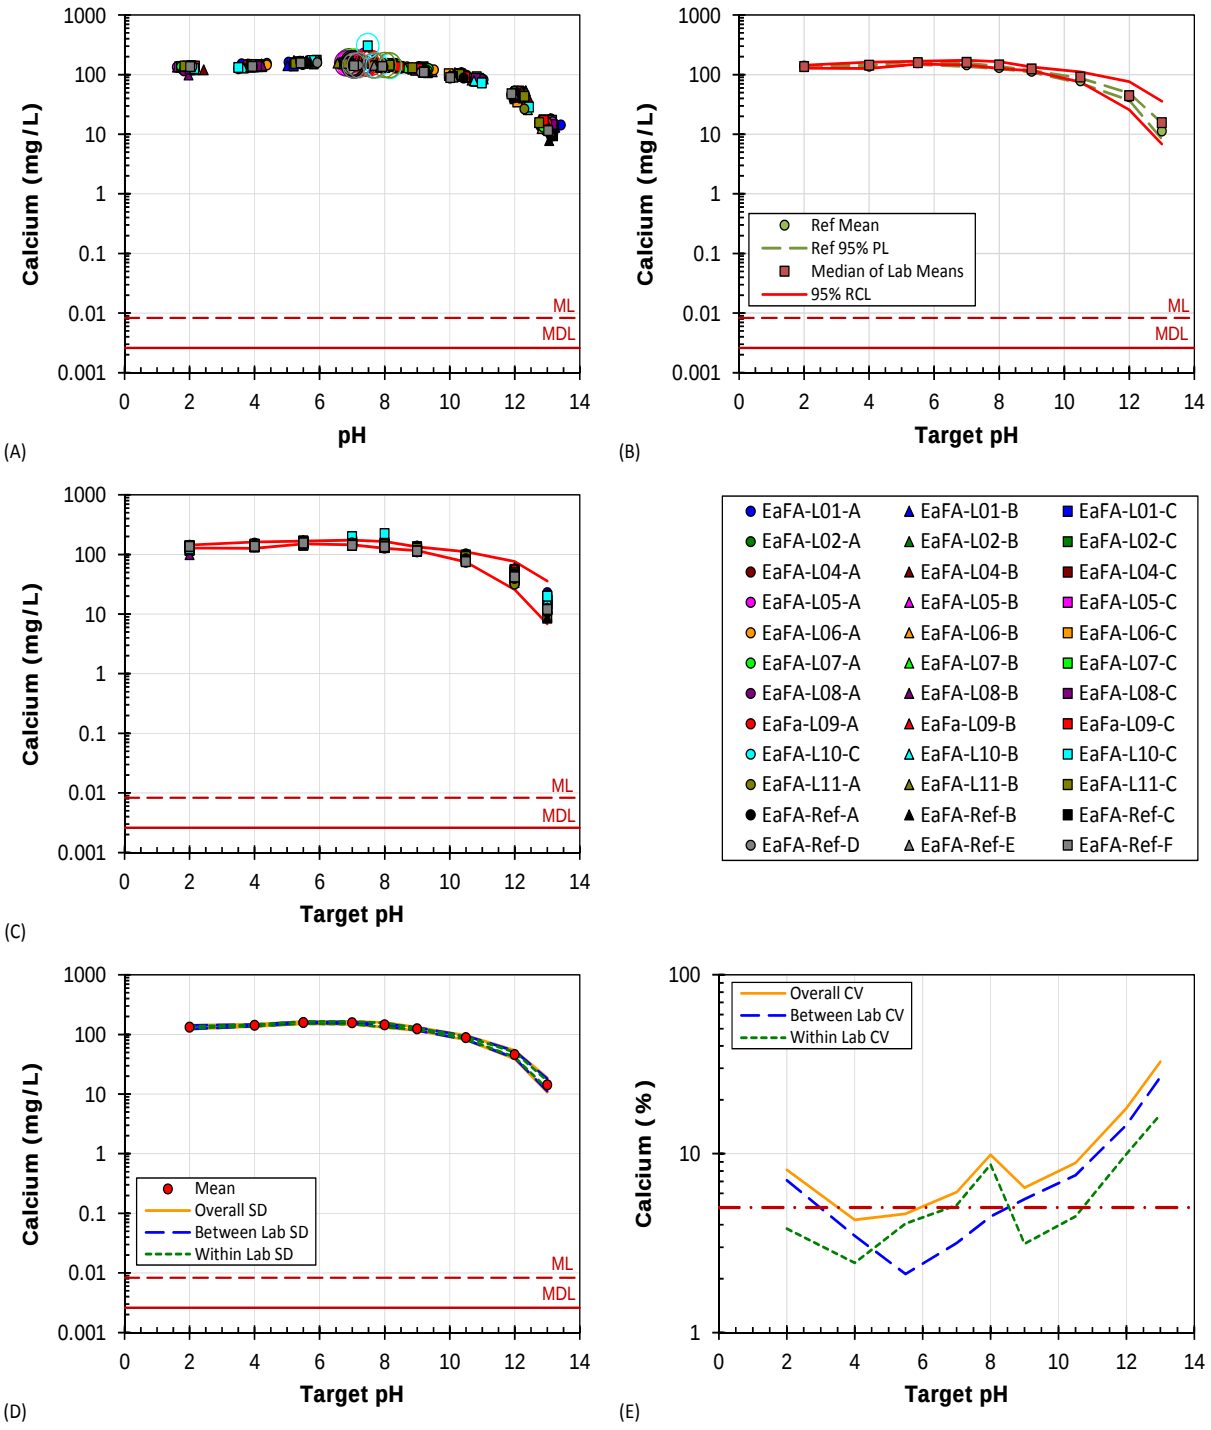

Figure 5. Calcium statistical analysis for Method 1313 Phase I material EaFA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

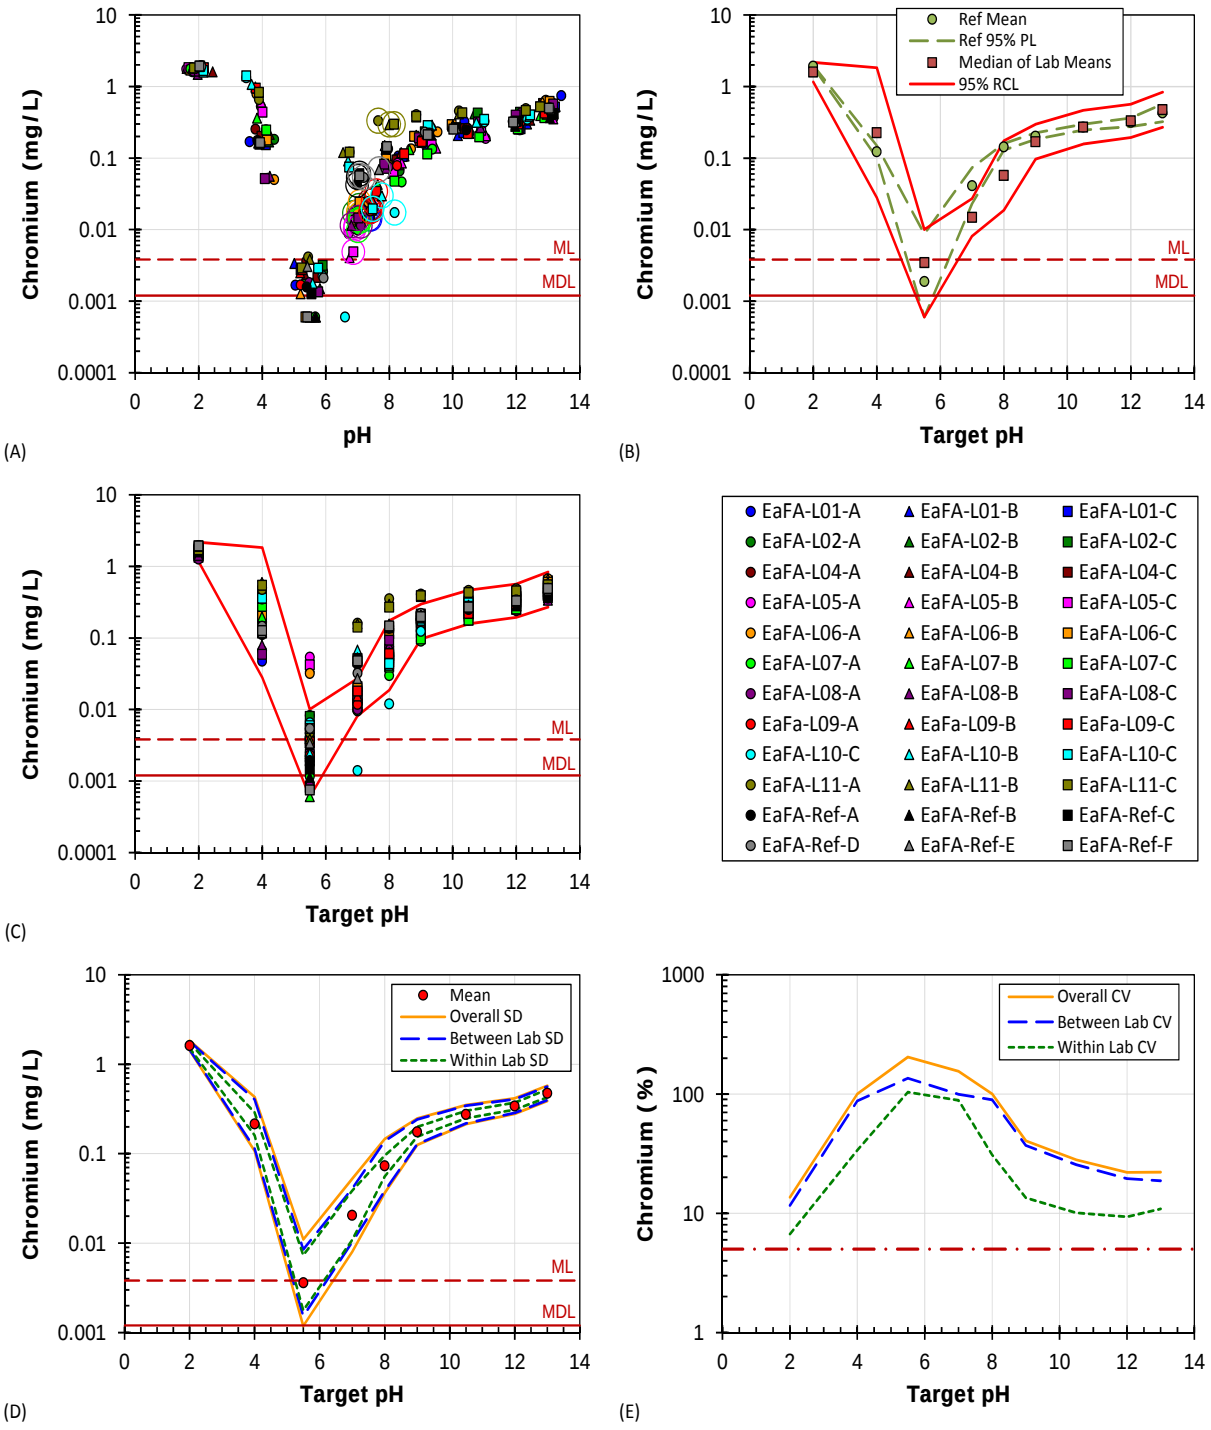

Figure 6. Chromium statistical analysis for Method 1313 Phase I material EaFA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

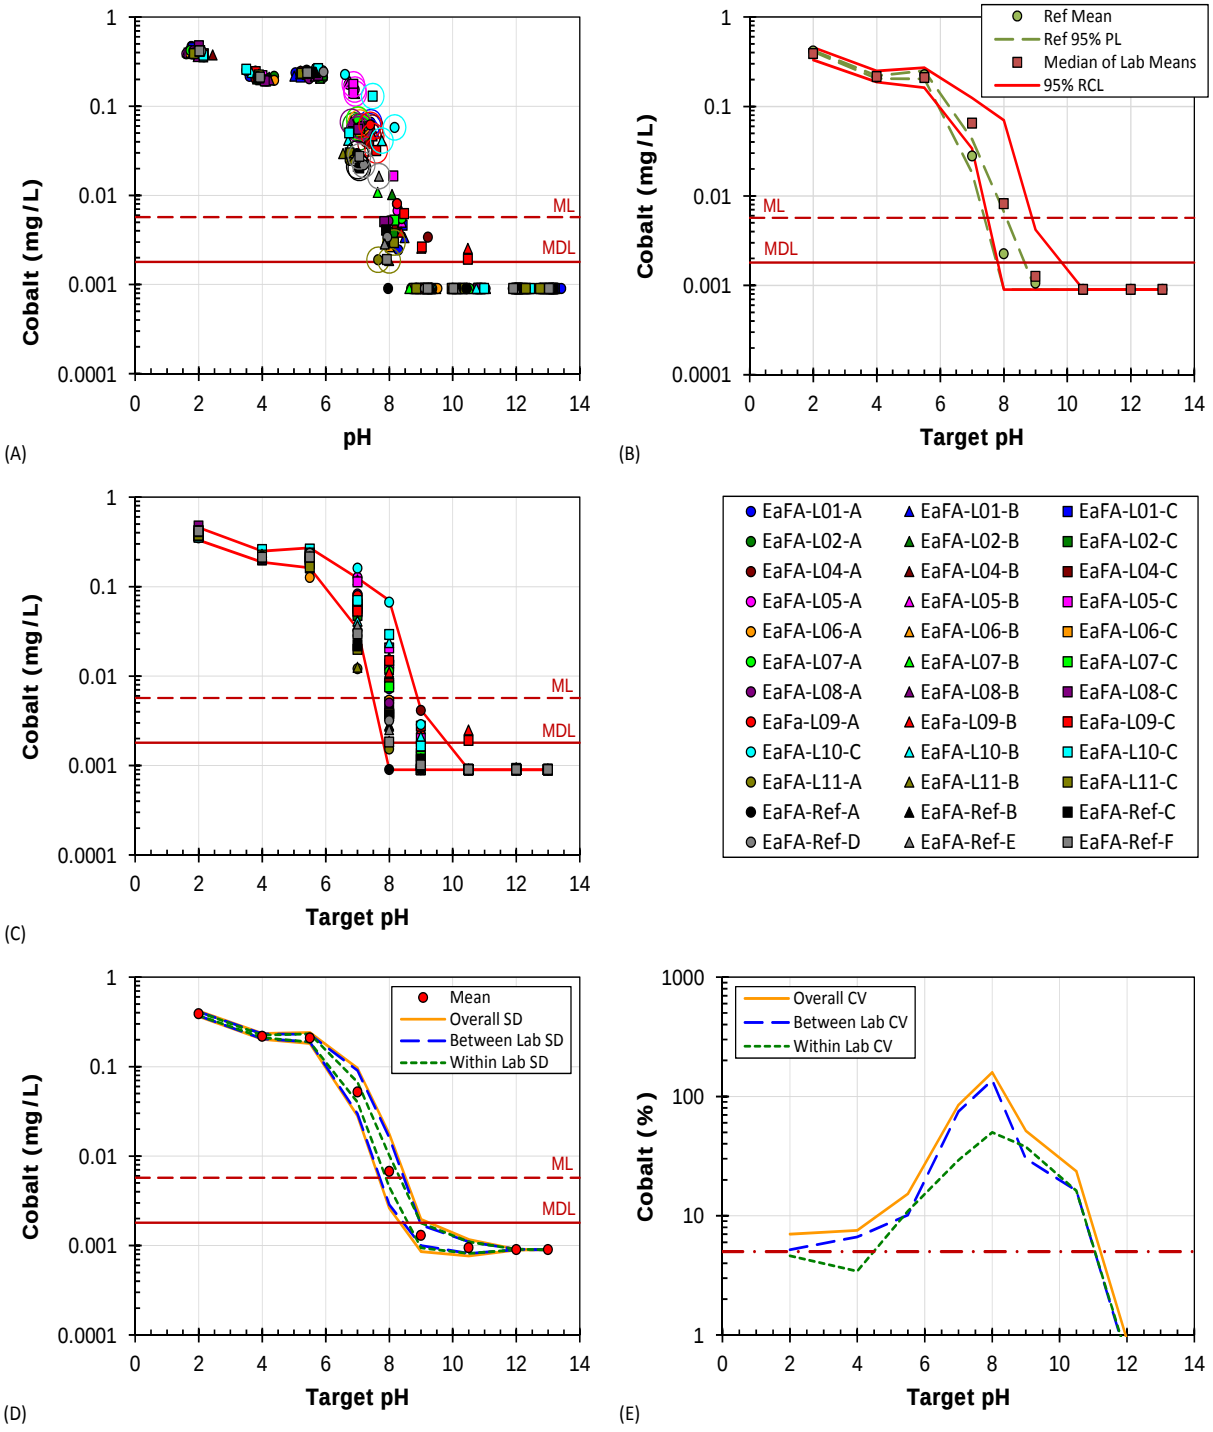

Figure 7. Cobalt statistical analysis for Method 1313 Phase I material EaFA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

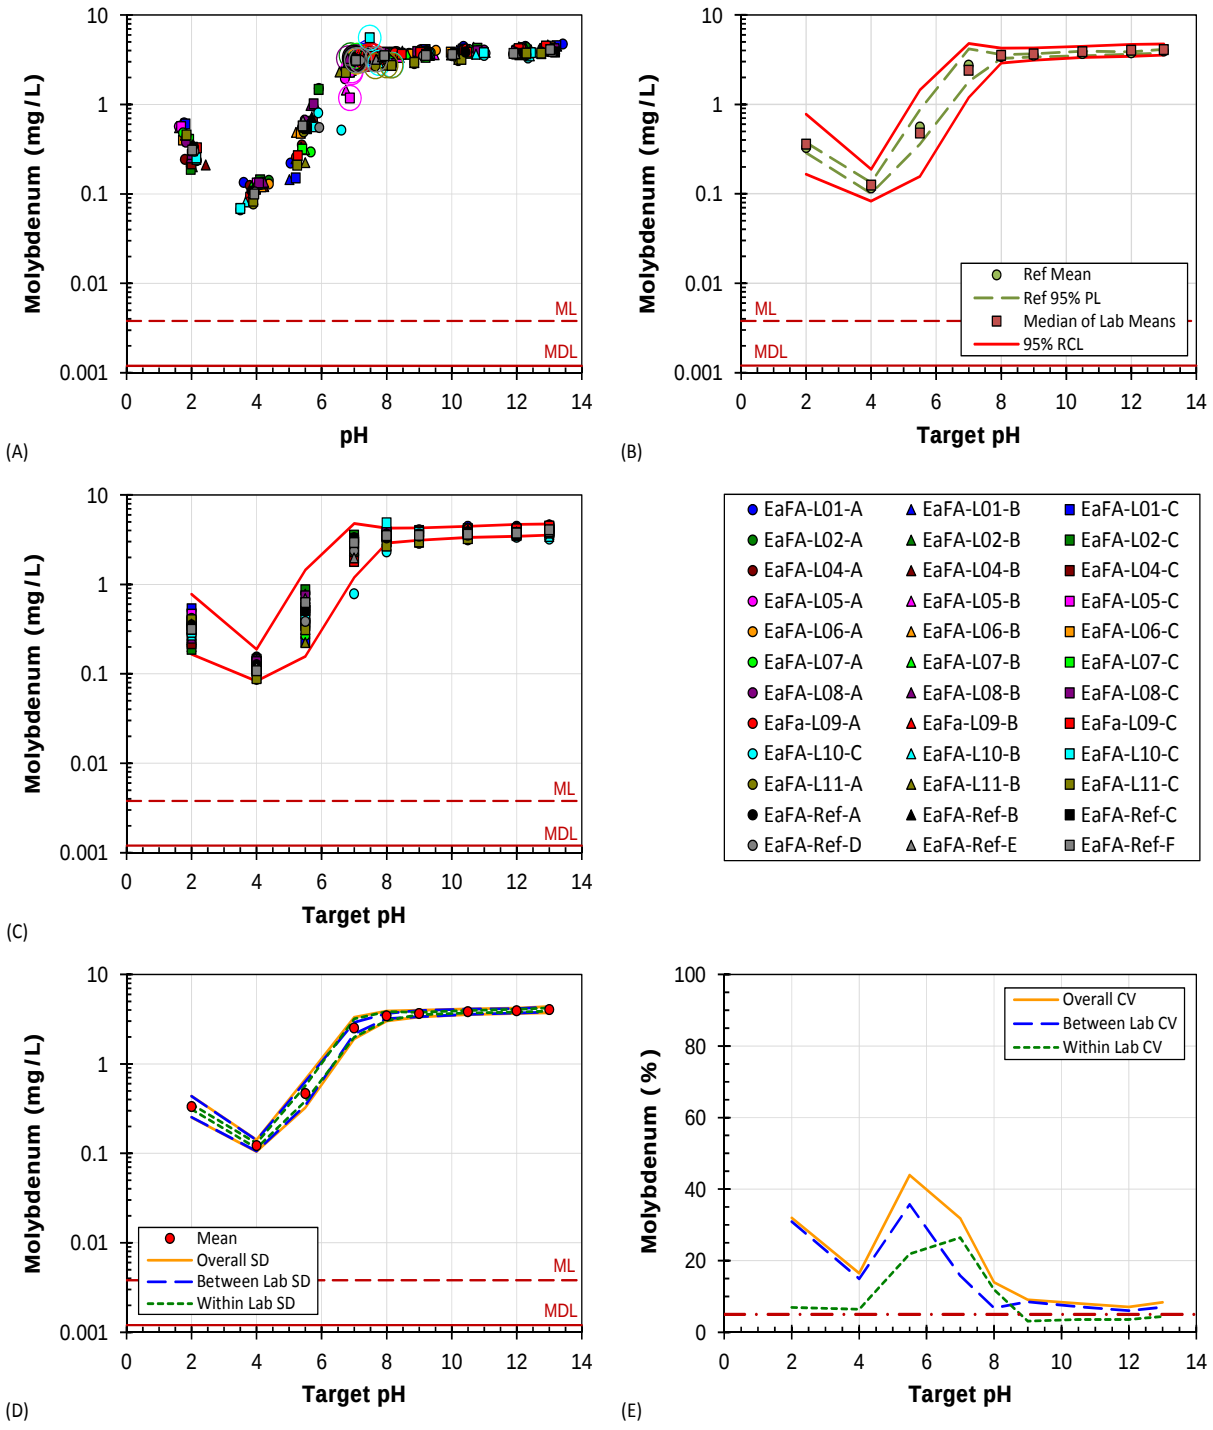

Figure 8. Molybdenum statistical analysis for Method 1313 Phase I material EaFA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

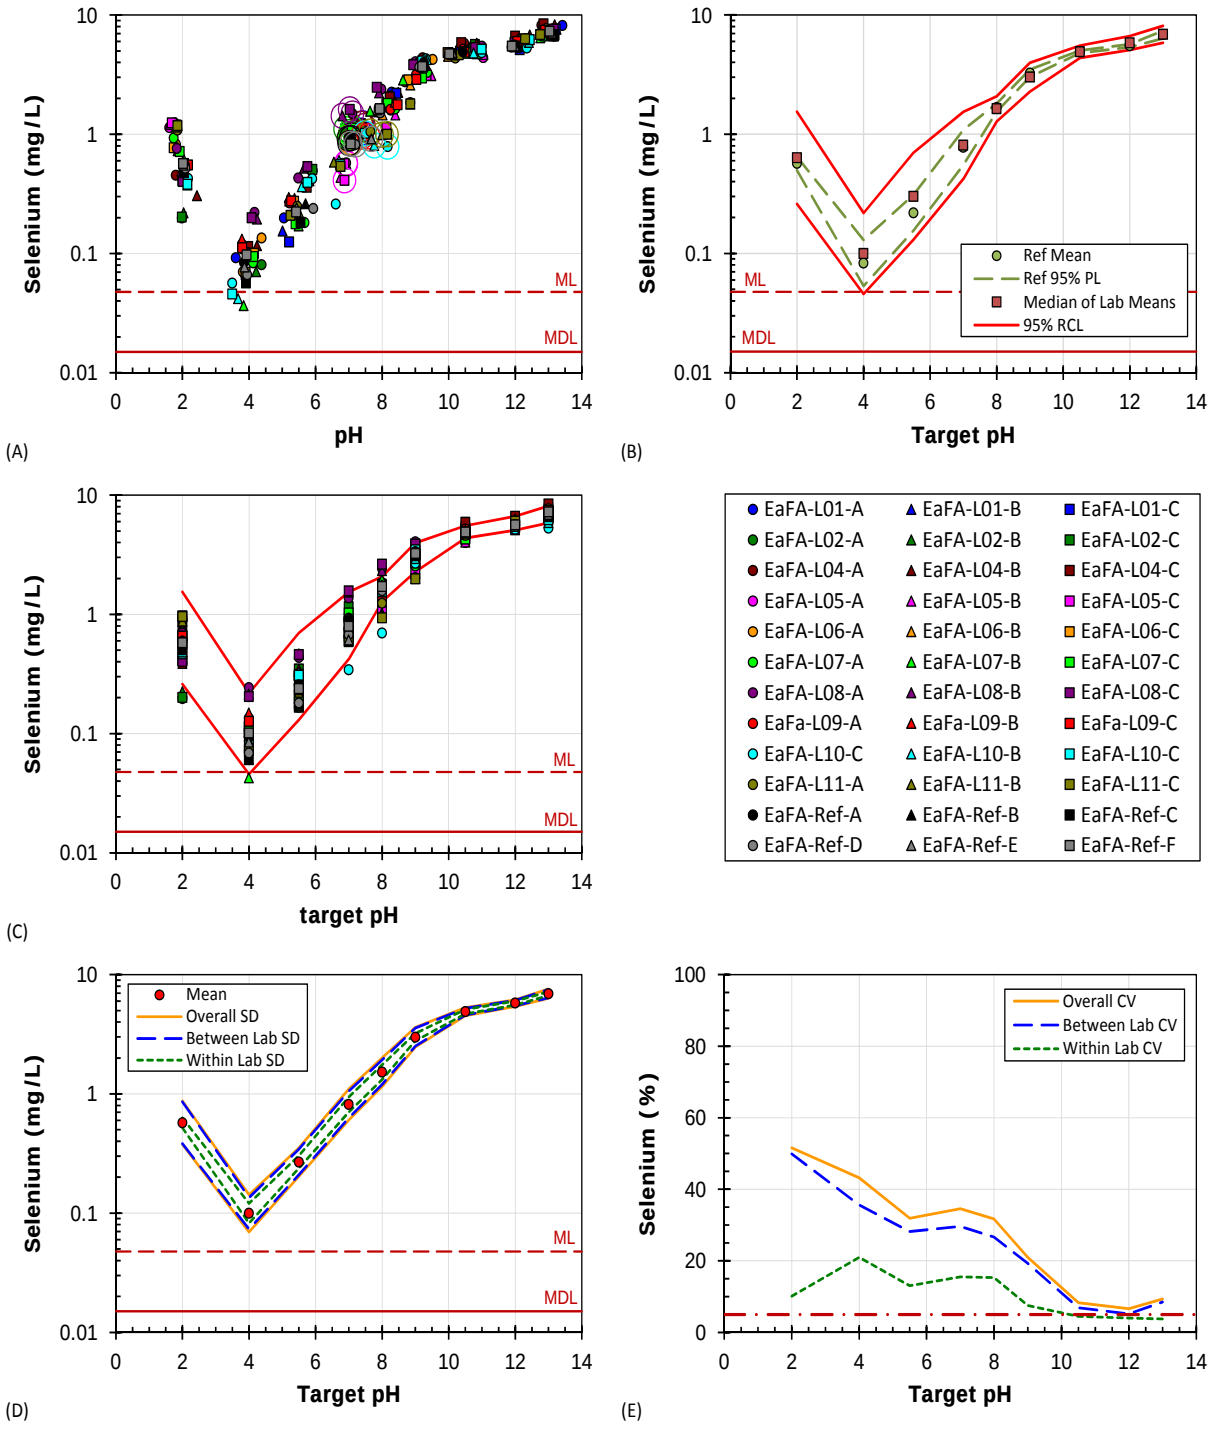

Figure 9. Selenium statistical analysis for Method 1313 Phase I material EaFA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

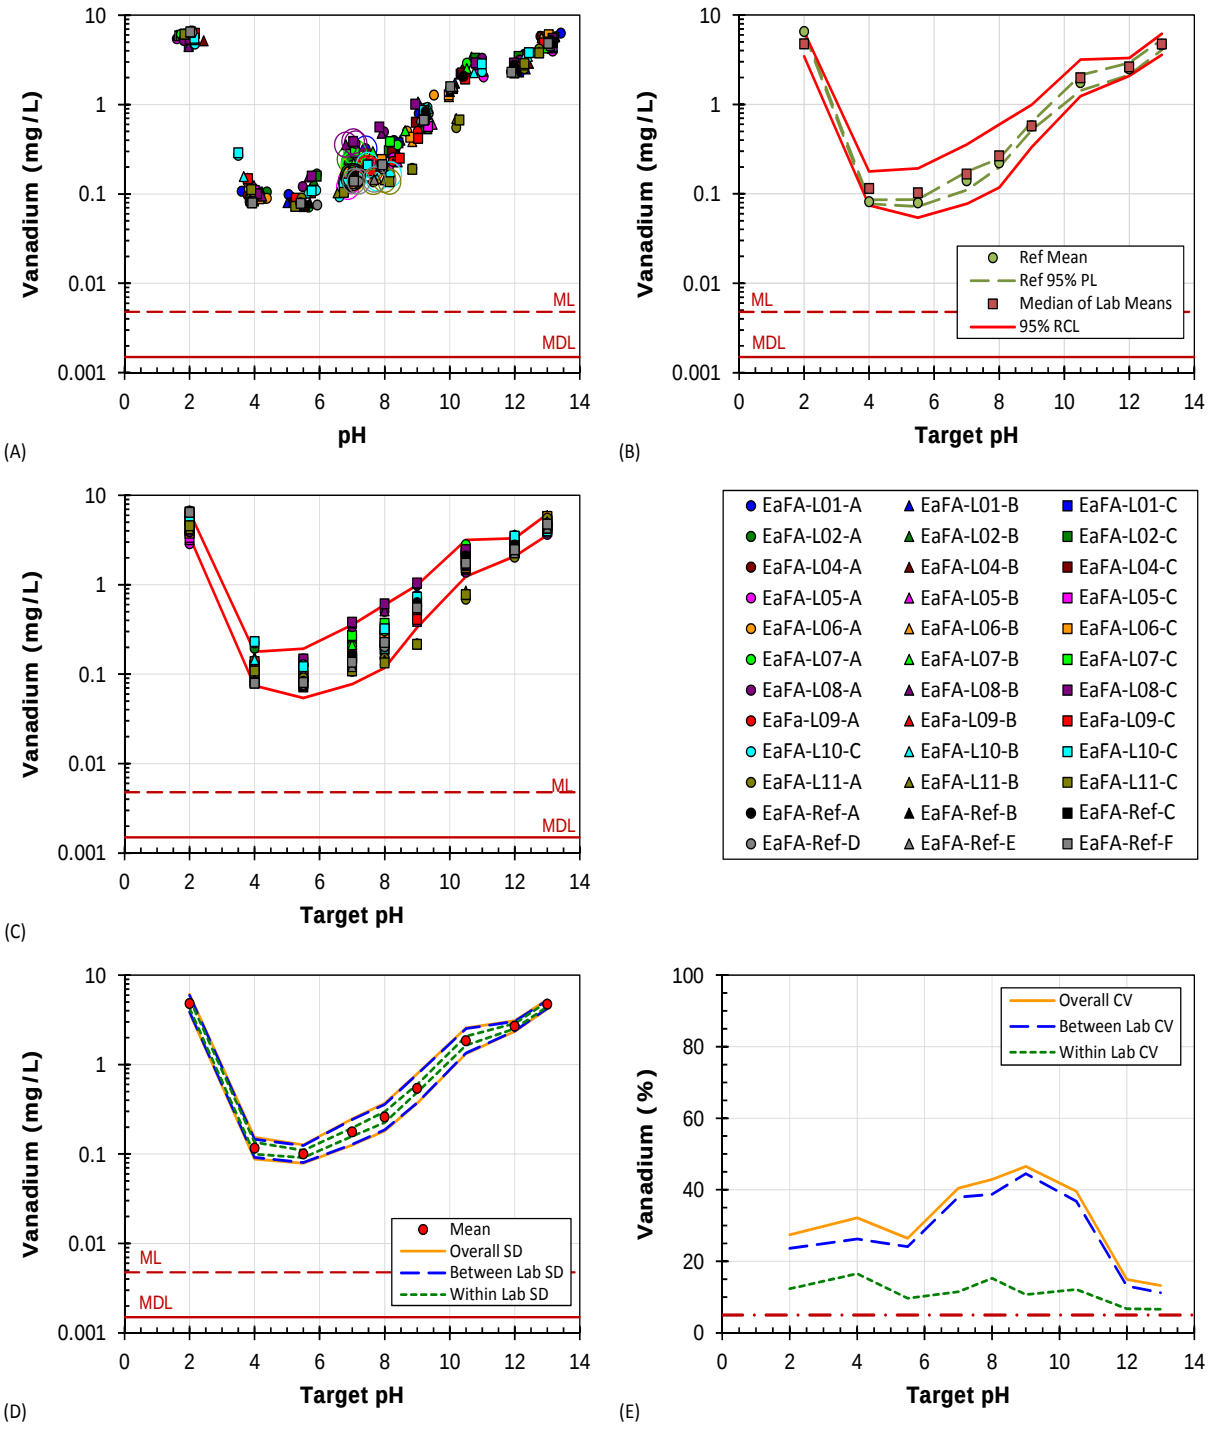

Figure 10. Vanadium statistical analysis for Method 1313 Phase I material EaFA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

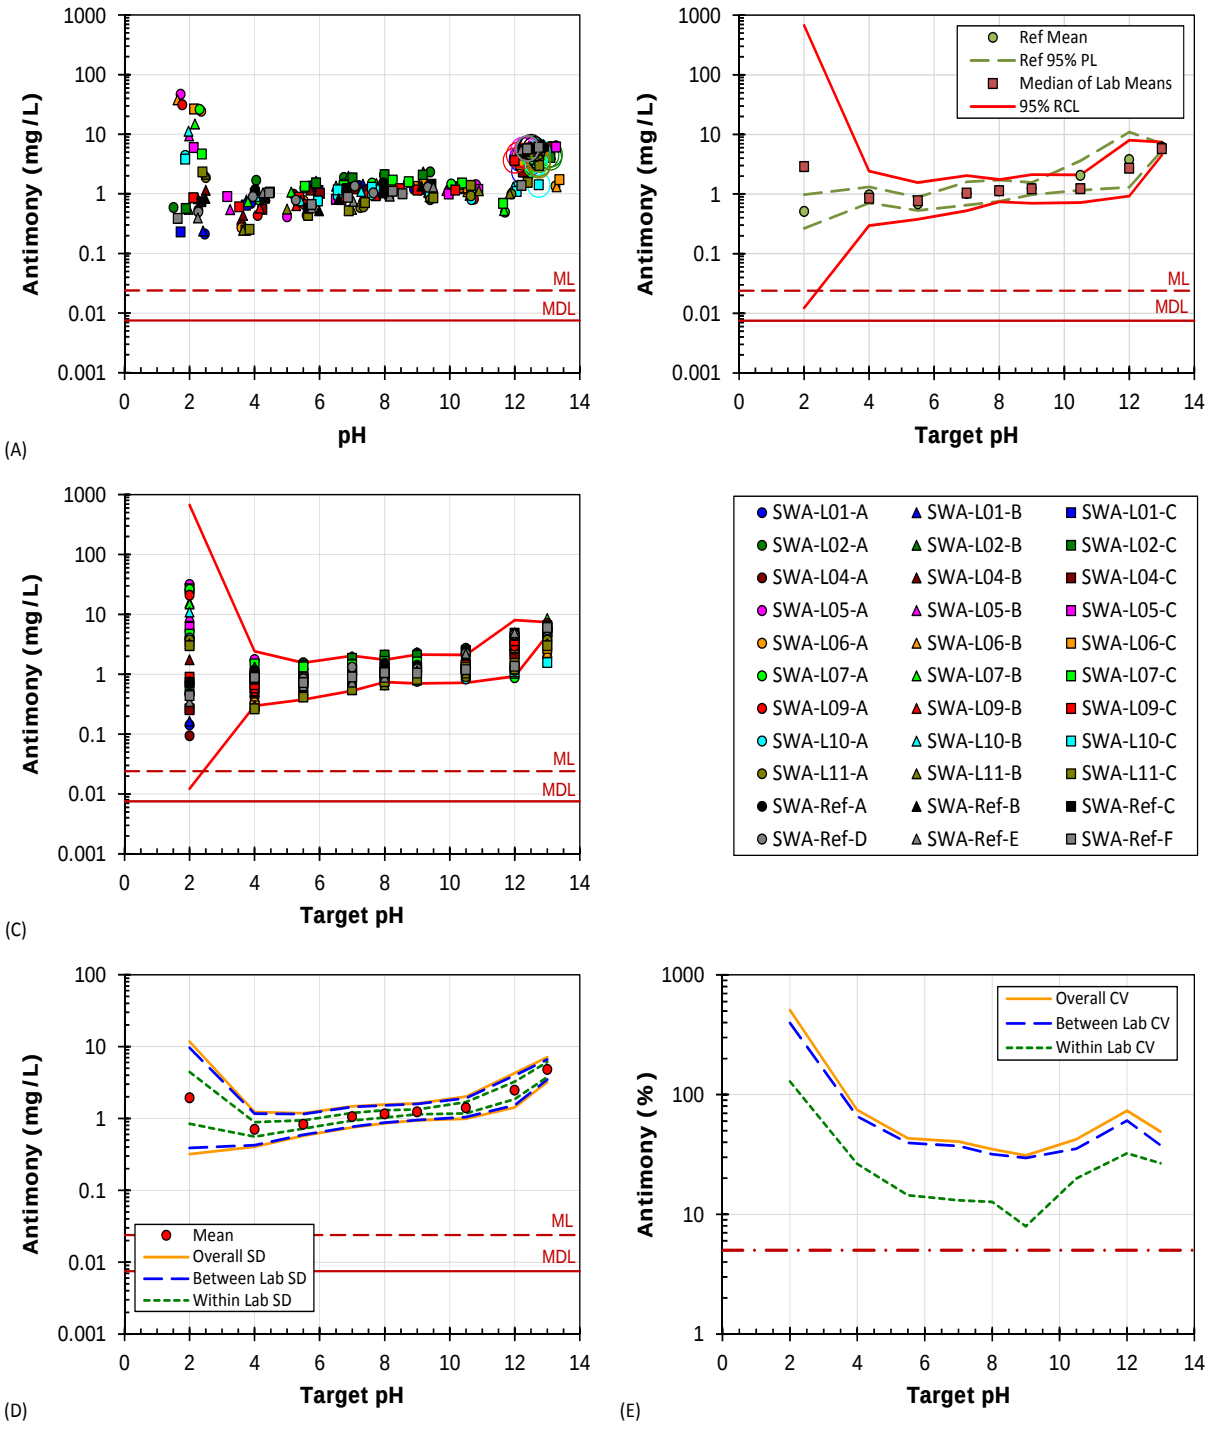

Figure 11. Antimony statistical analysis for Method 1313 Phase II material SWA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

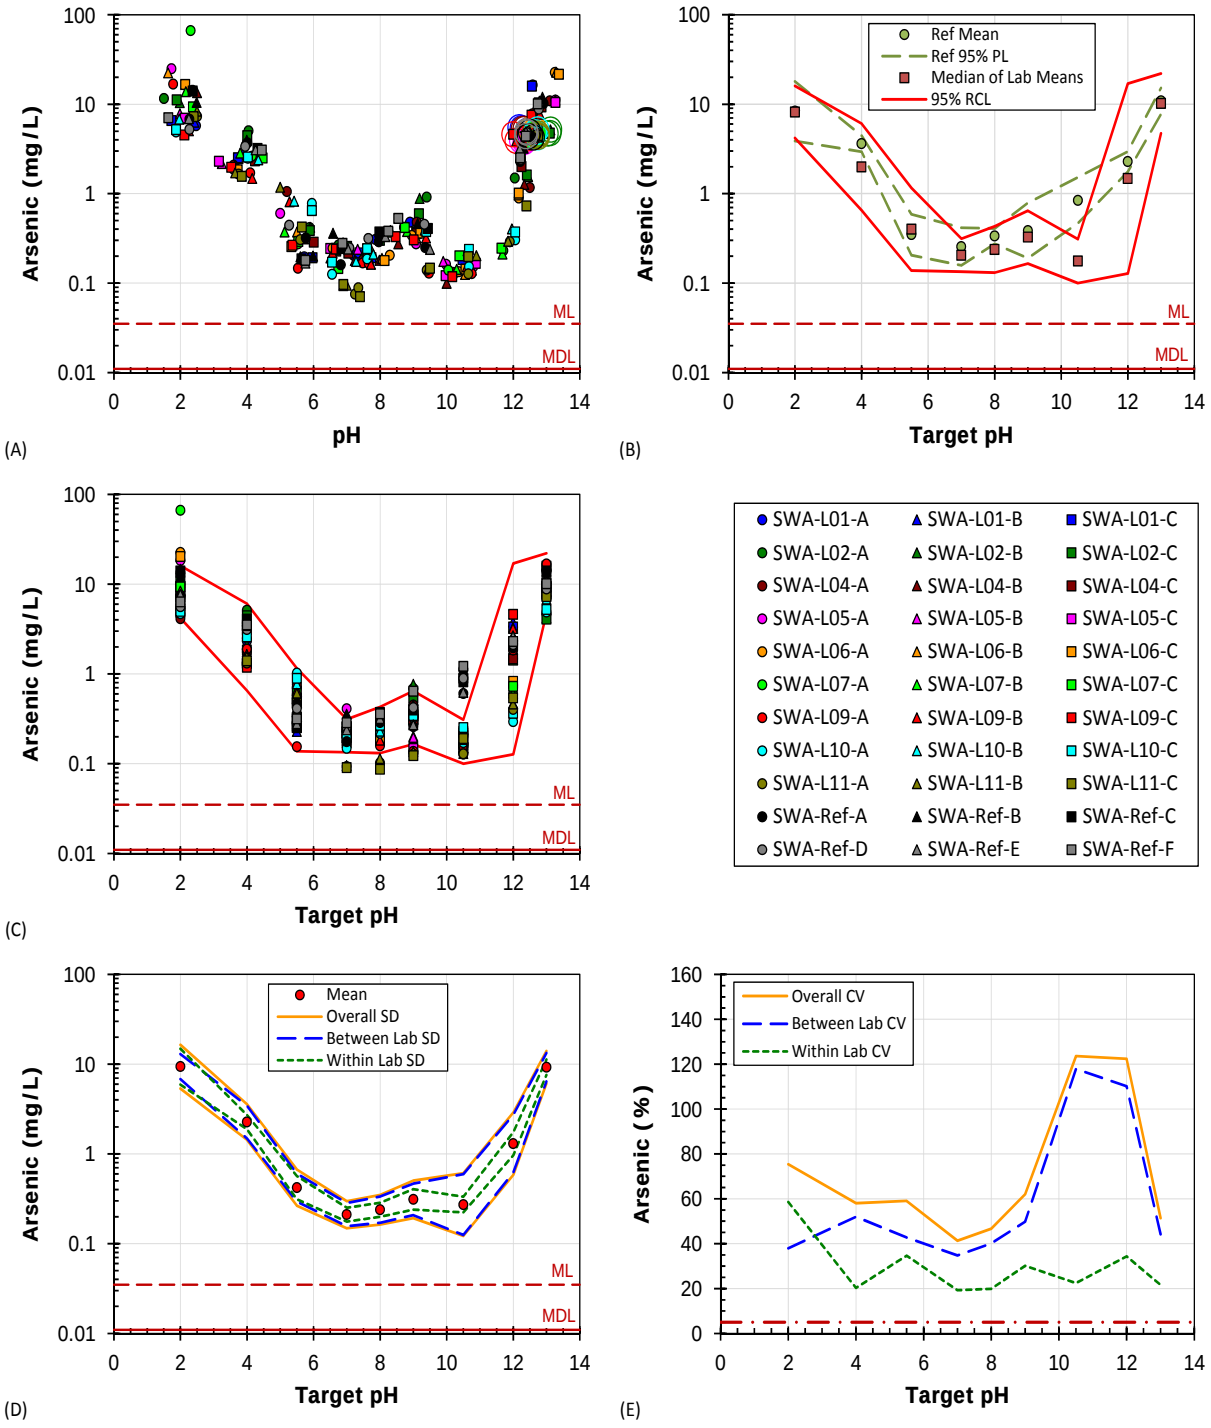

Figure 12. Arsenic statistical analysis for Method 1313 Phase II material SWA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

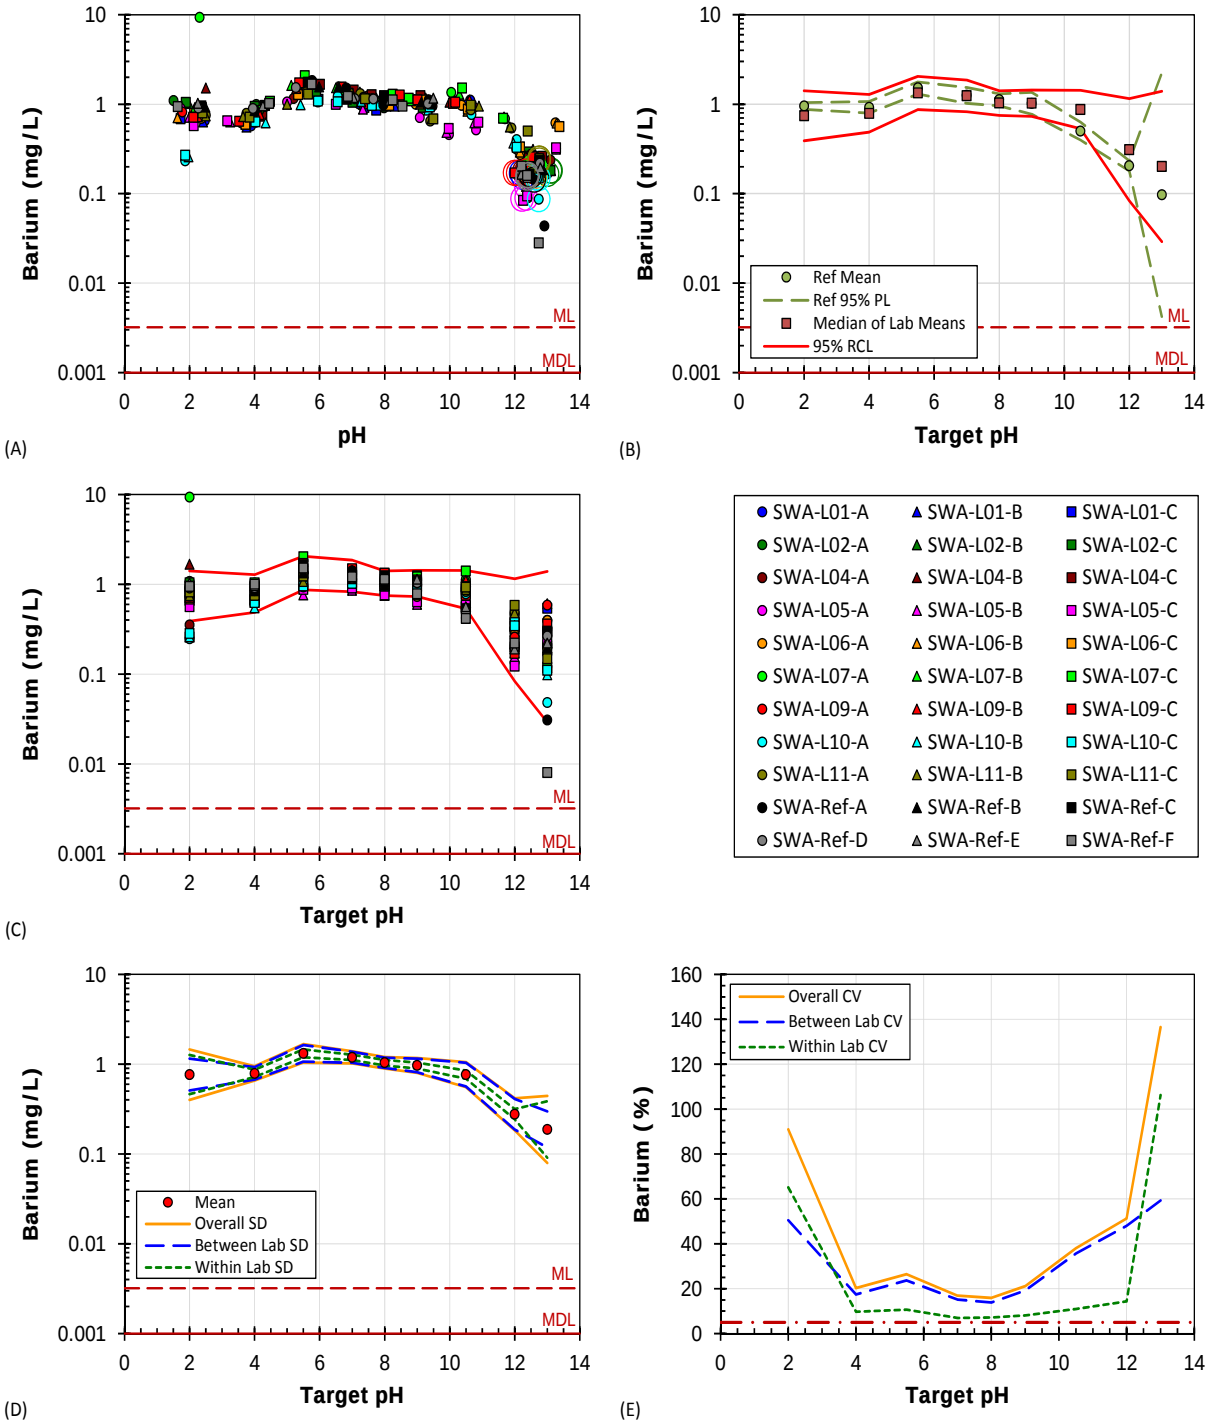

Figure 13. Barium statistical analysis for Method 1313 Phase II material SWA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

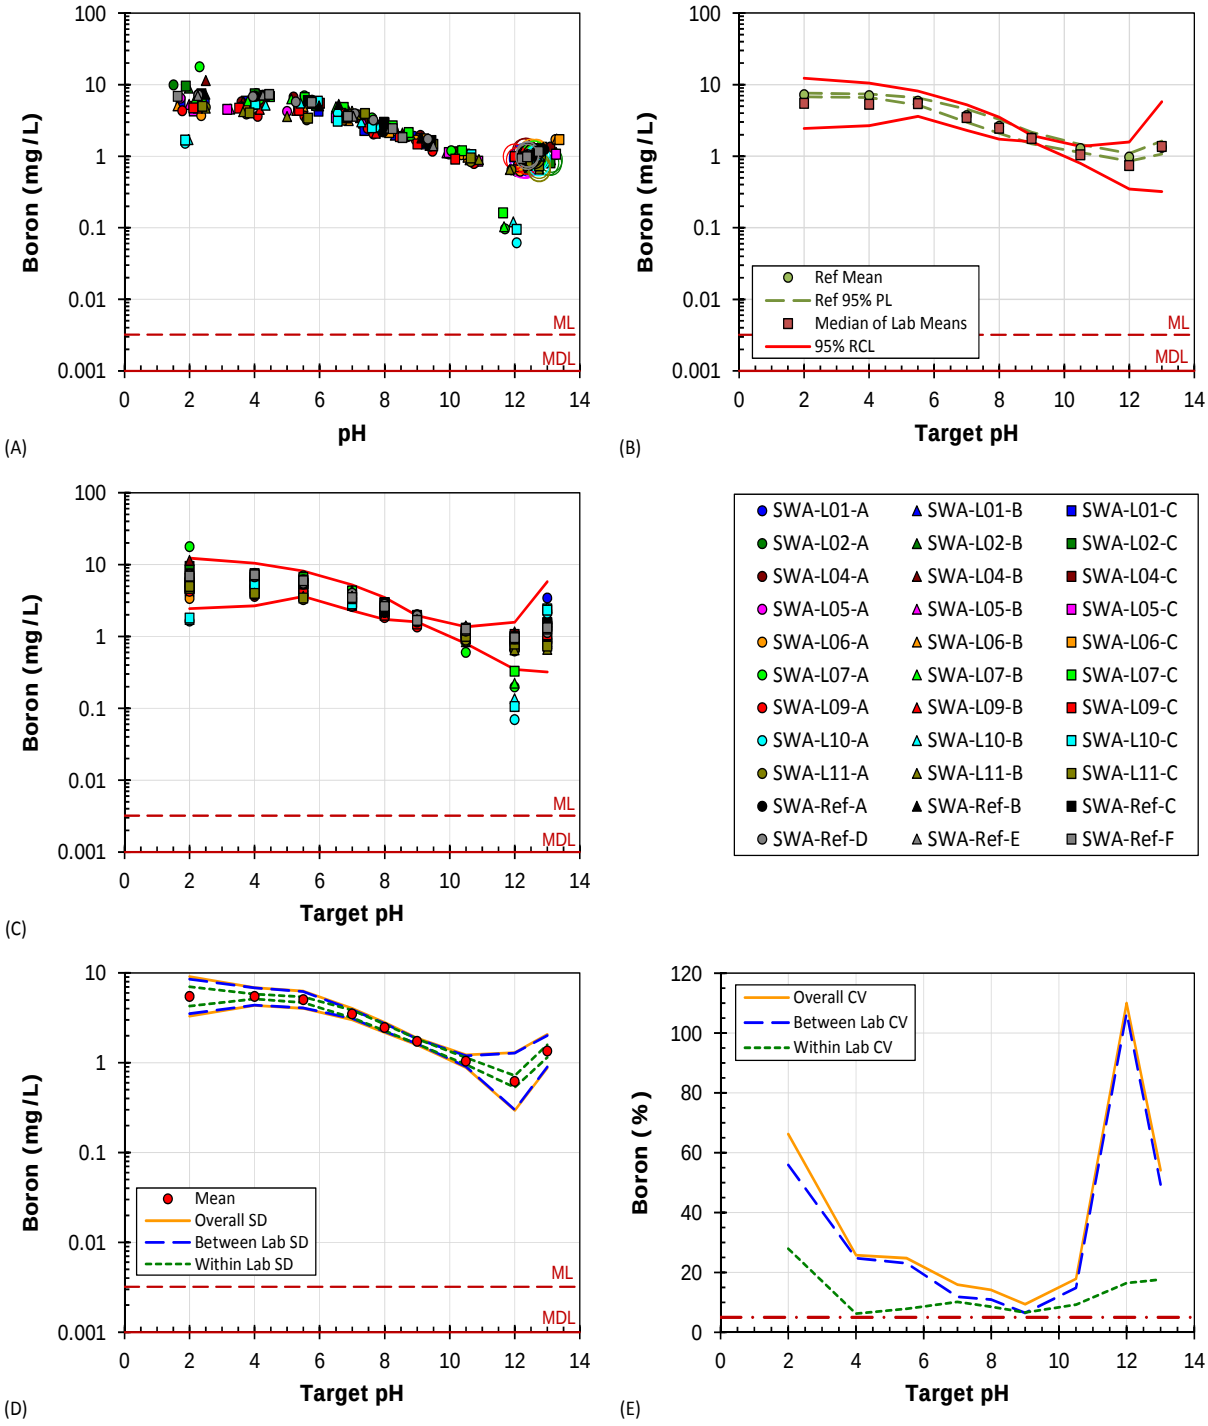

Figure 14. Boron statistical analysis for Method 1313 Phase II material SWA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

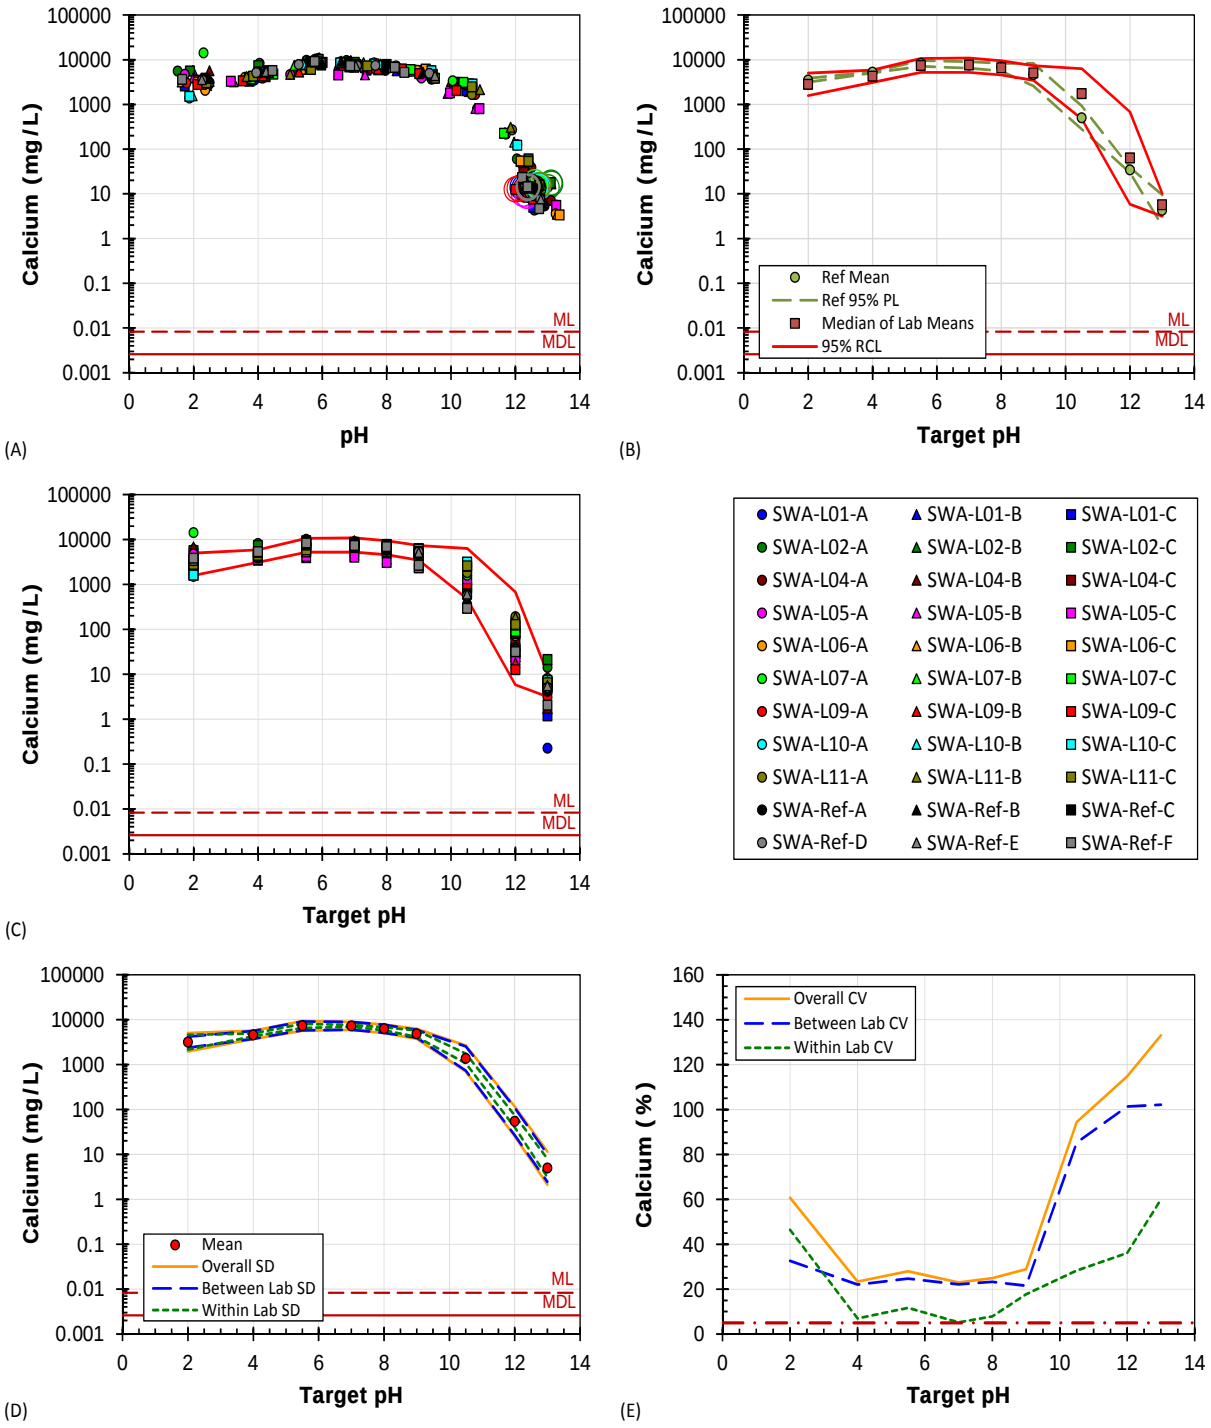

Figure 15. Calcium statistical analysis for Method 1313 Phase II material SWA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

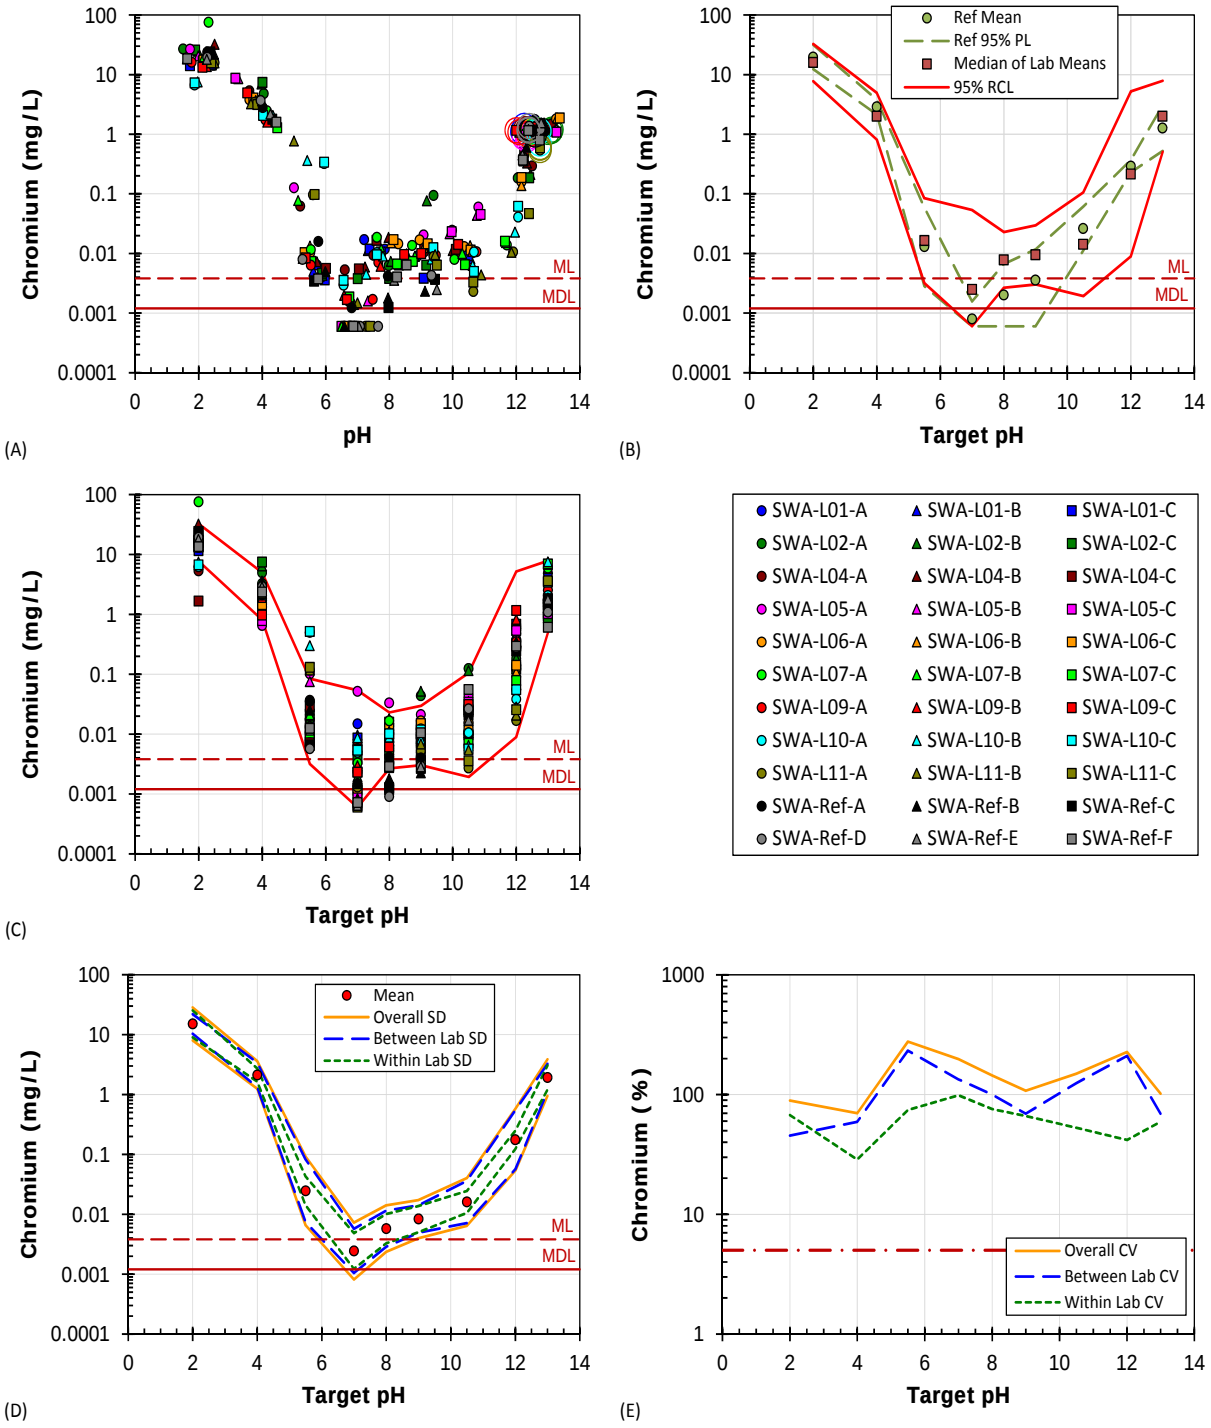

Figure 16. Chromium statistical analysis for Method 1313 Phase II material SWA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

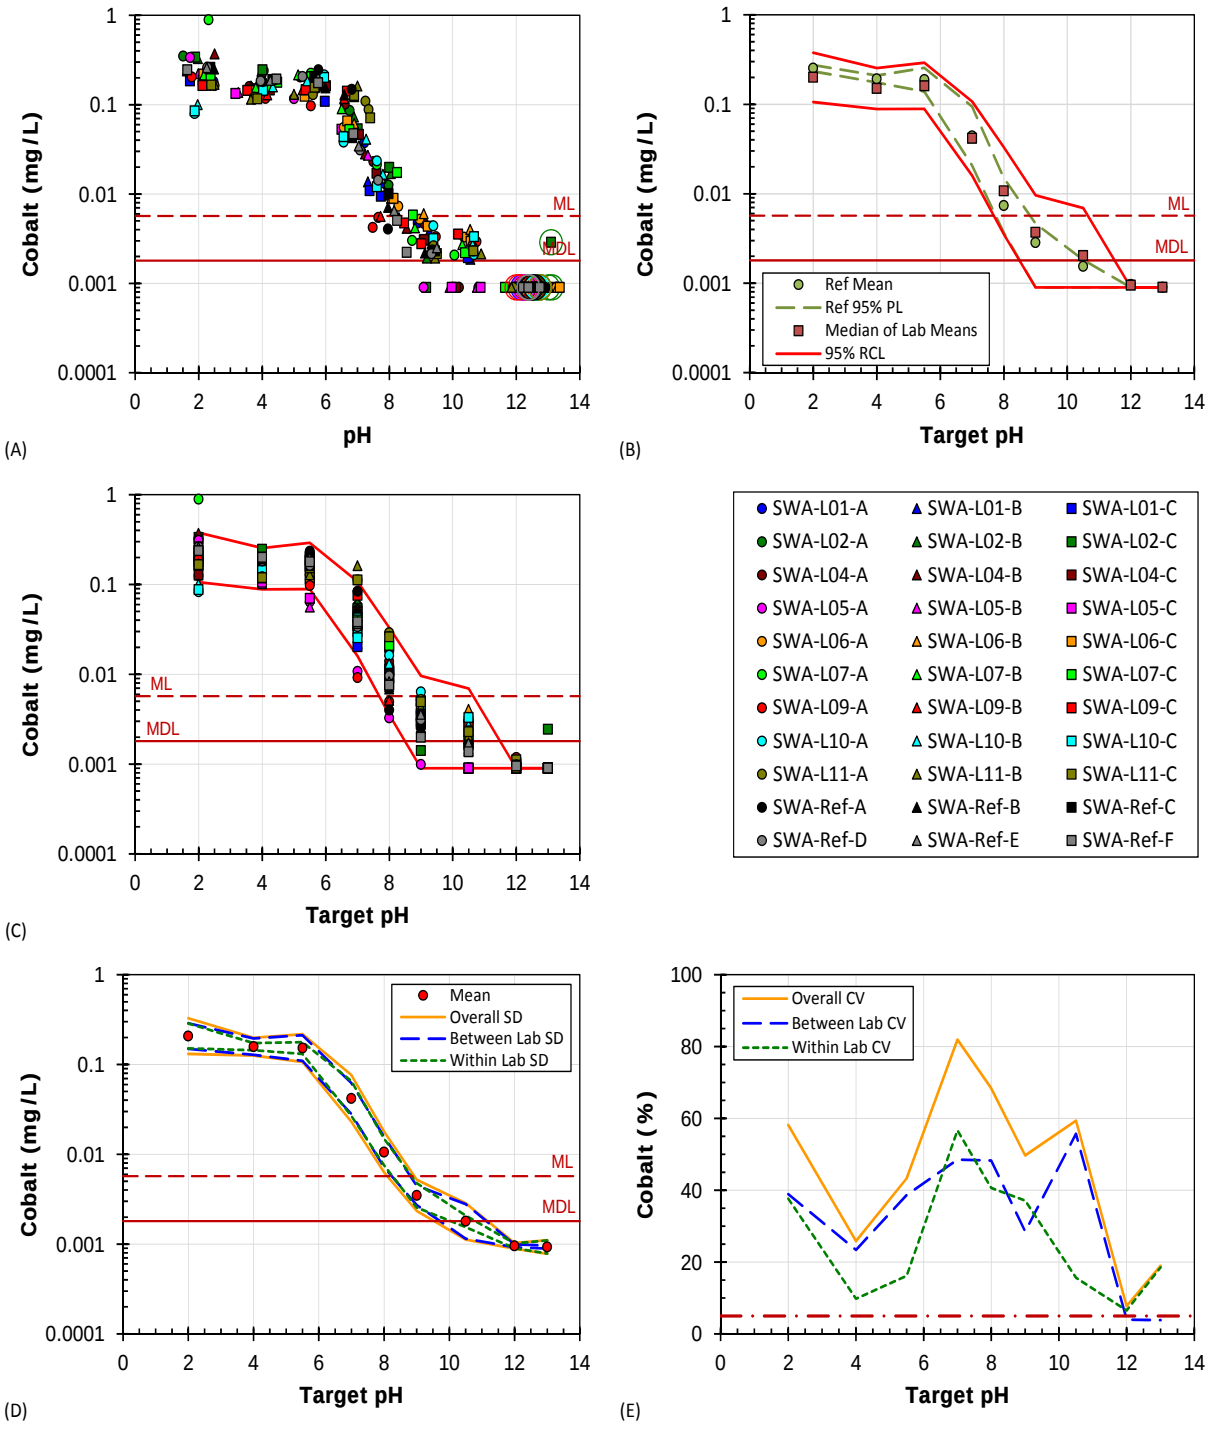

Figure 17. Cobalt statistical analysis for Method 1313 Phase II material SWA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

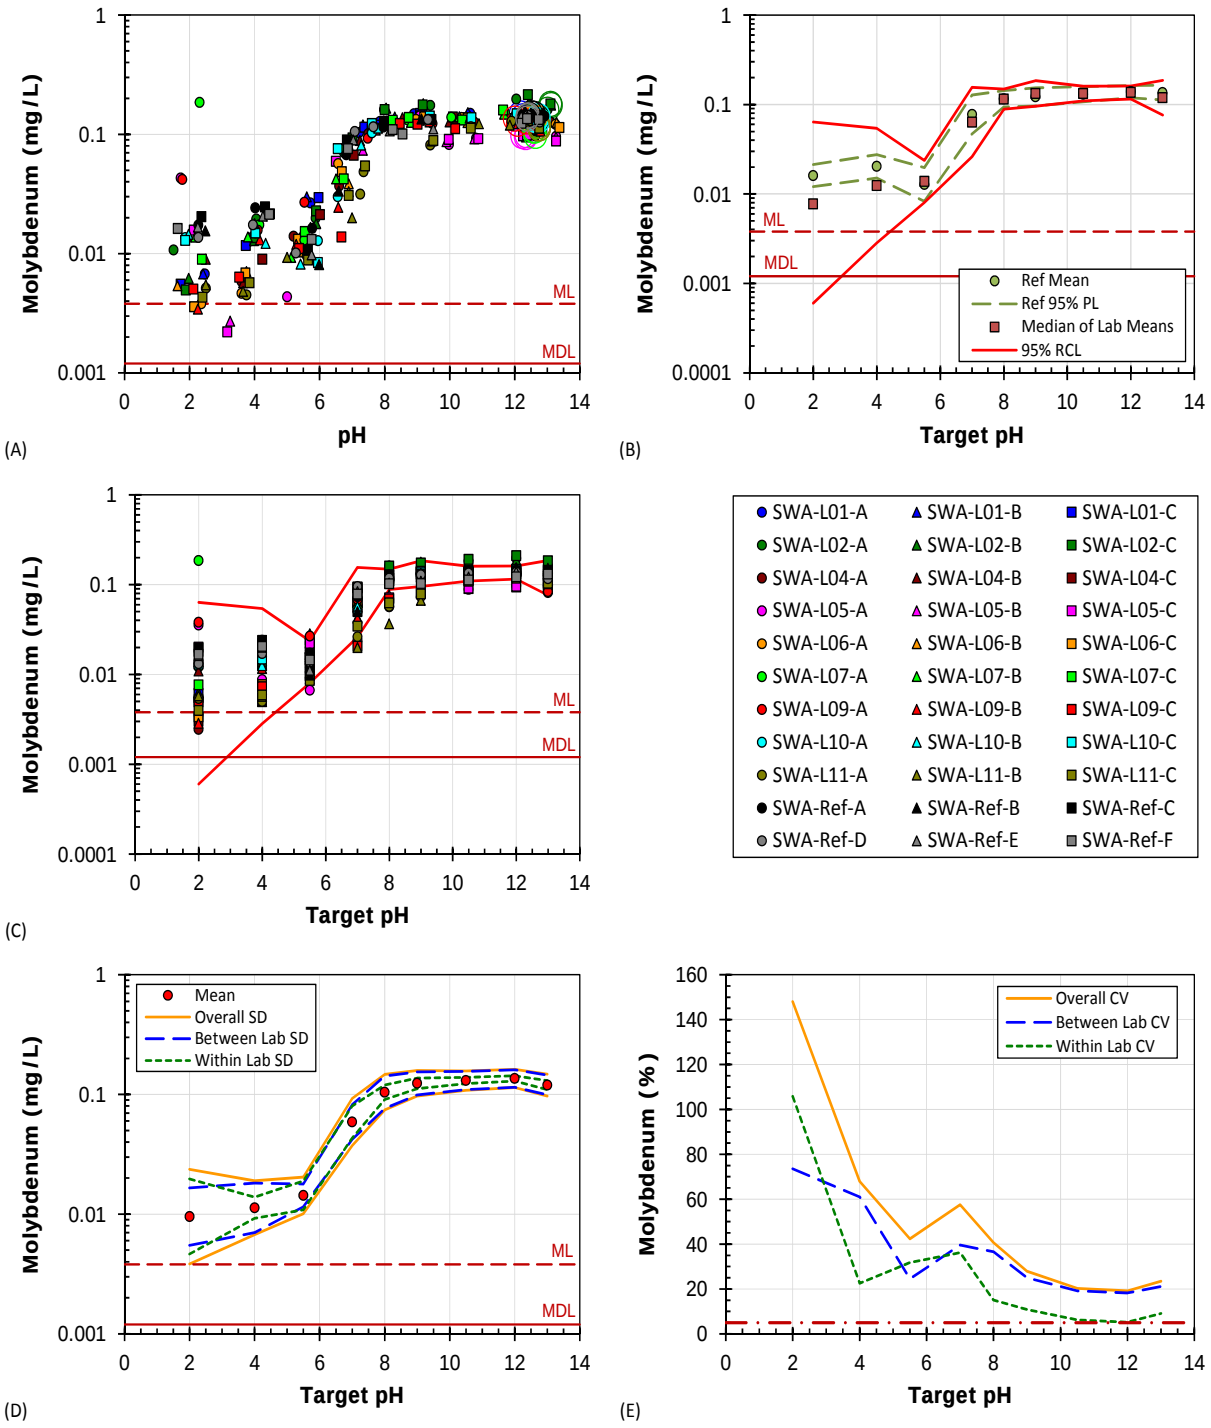

Figure 18. Molybdenum statistical analysis for Method 1313 Phase II material SWA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

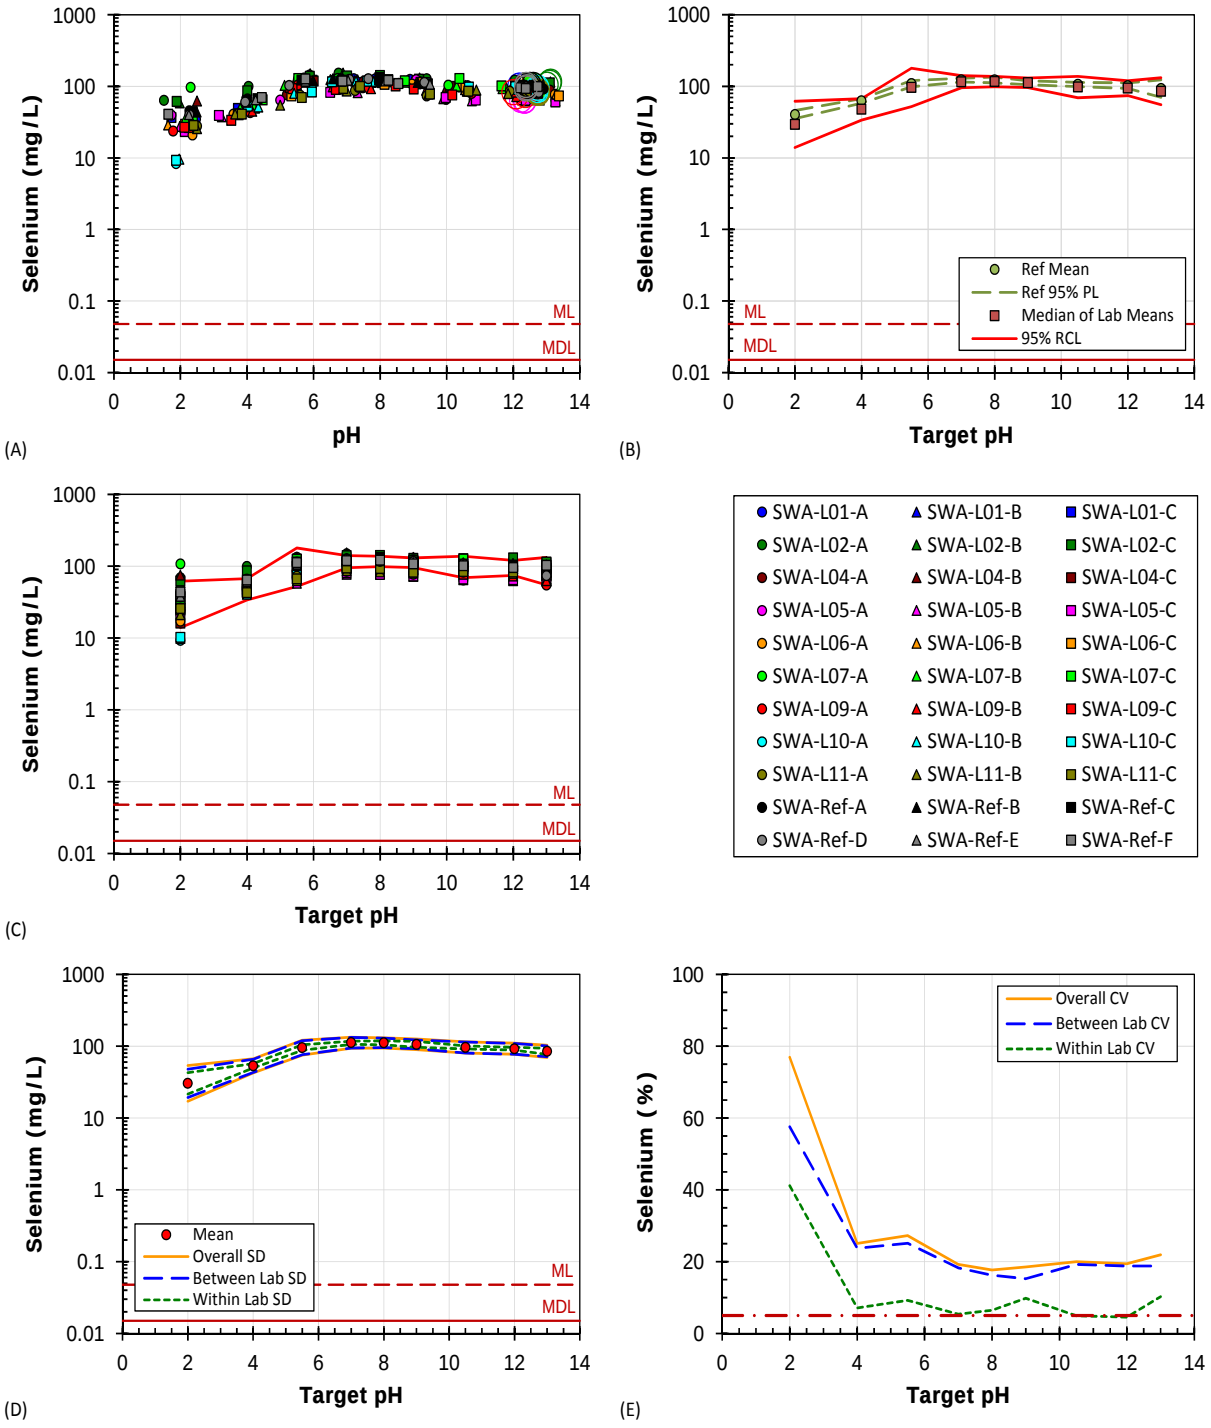

Figure 19. Selenium statistical analysis for Method 1313 Phase II material SWA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

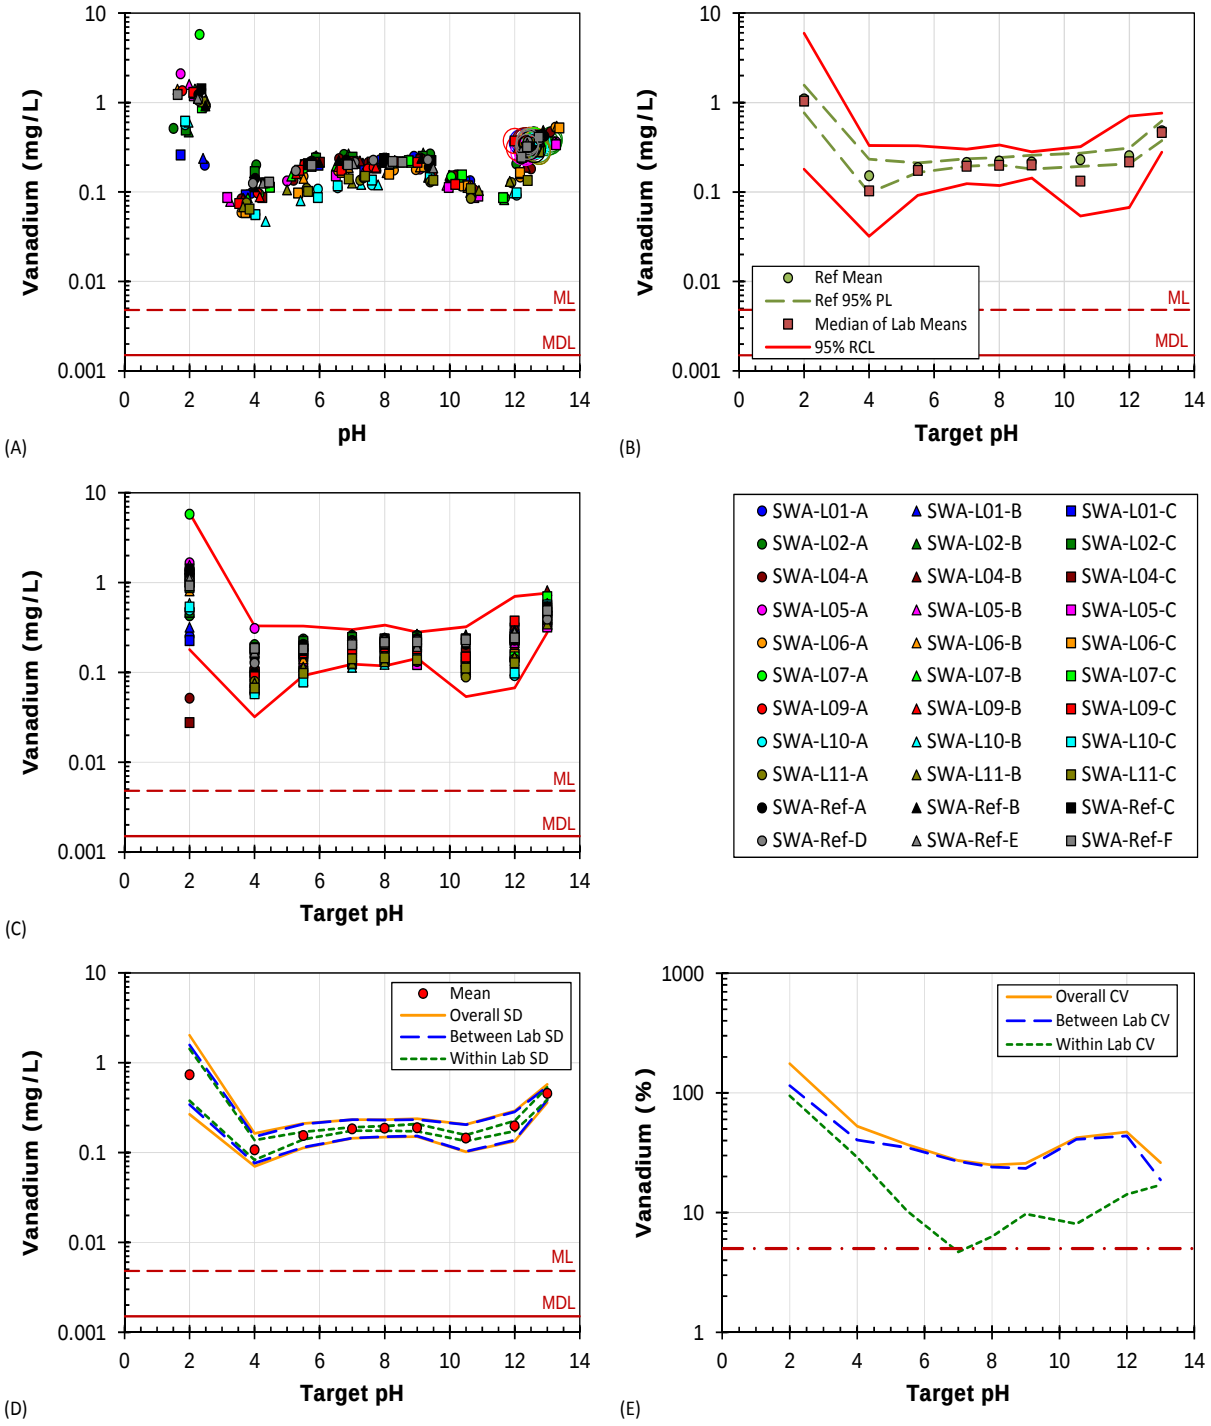

Figure 20. Vanadium statistical analysis for Method 1313 Phase II material SWA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

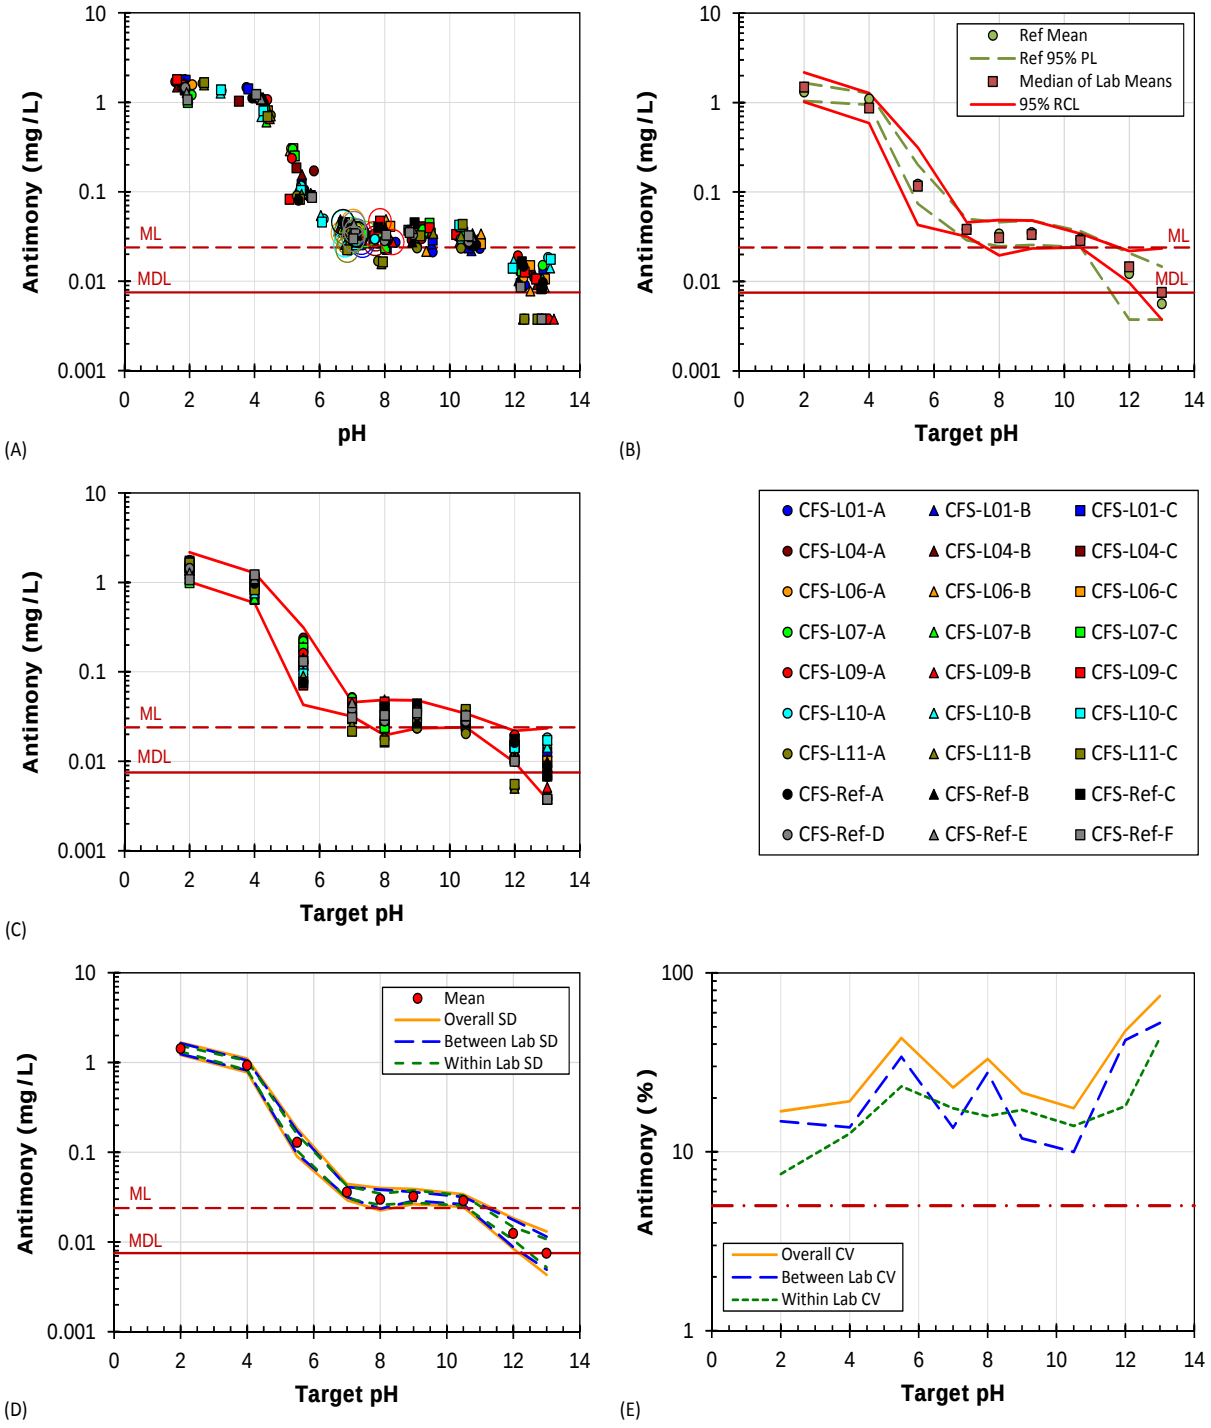

Figure 21. Antimony statistical analysis for Method 1313 Phase II material CFS. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

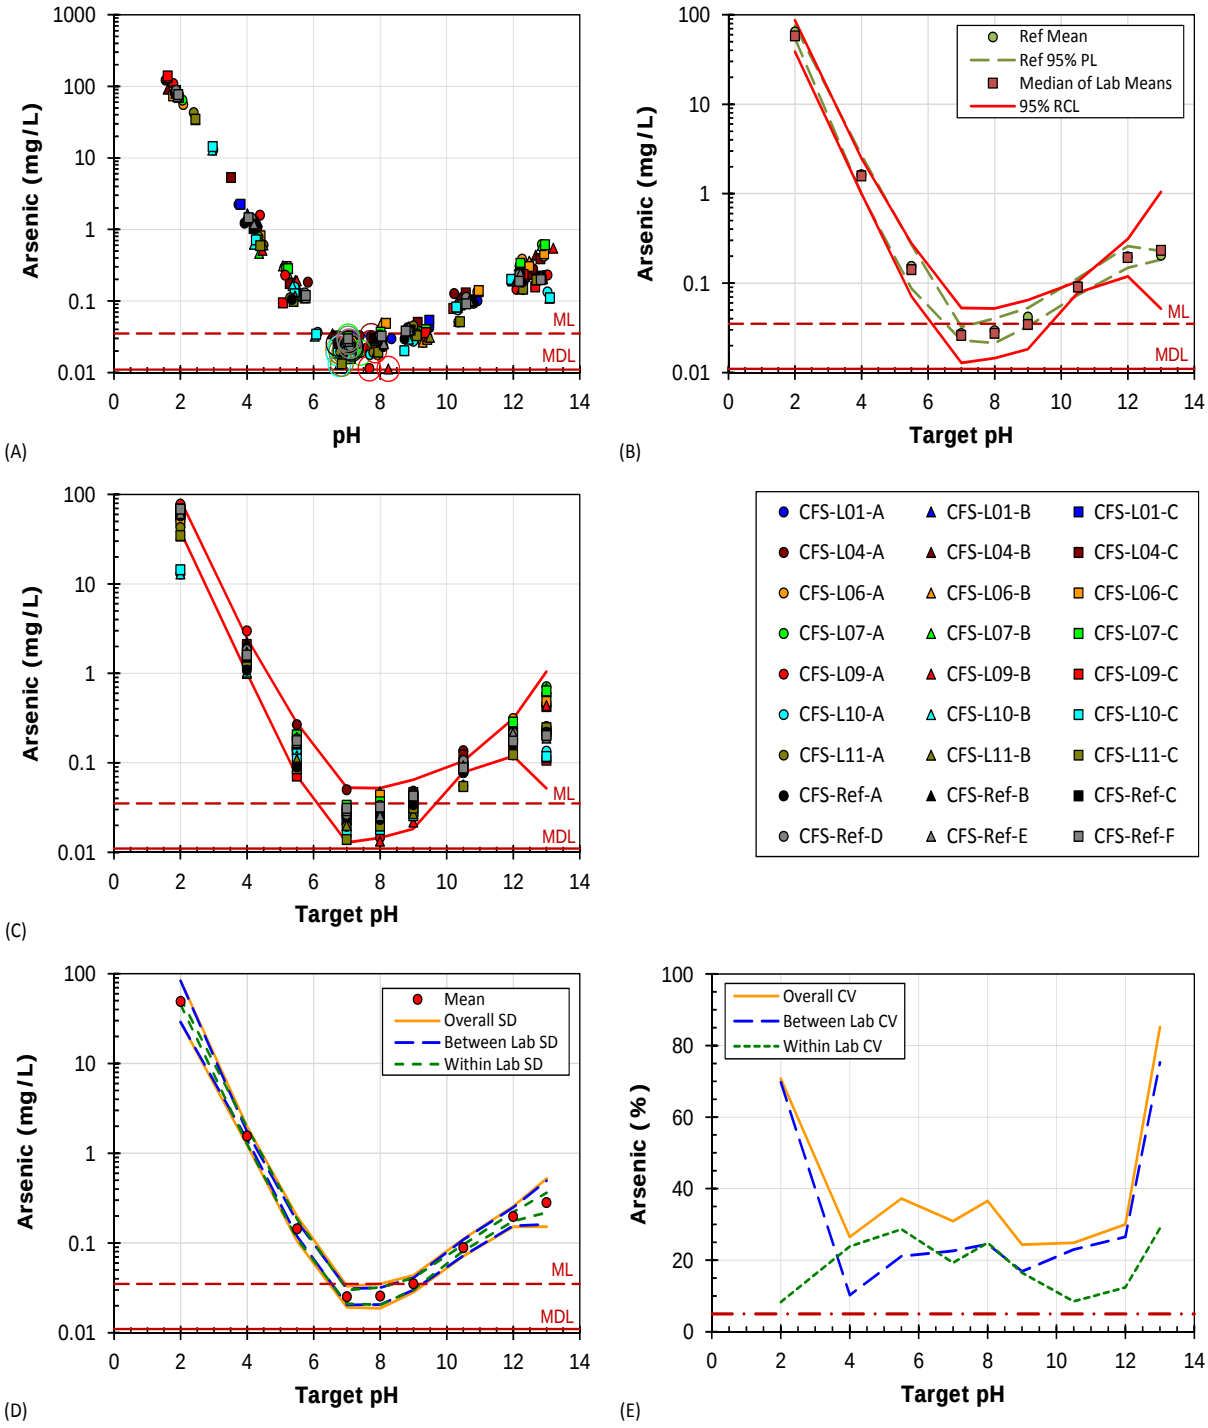

Figure 22. Arsenic statistical analysis for Method 1313 Phase II material CFS. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

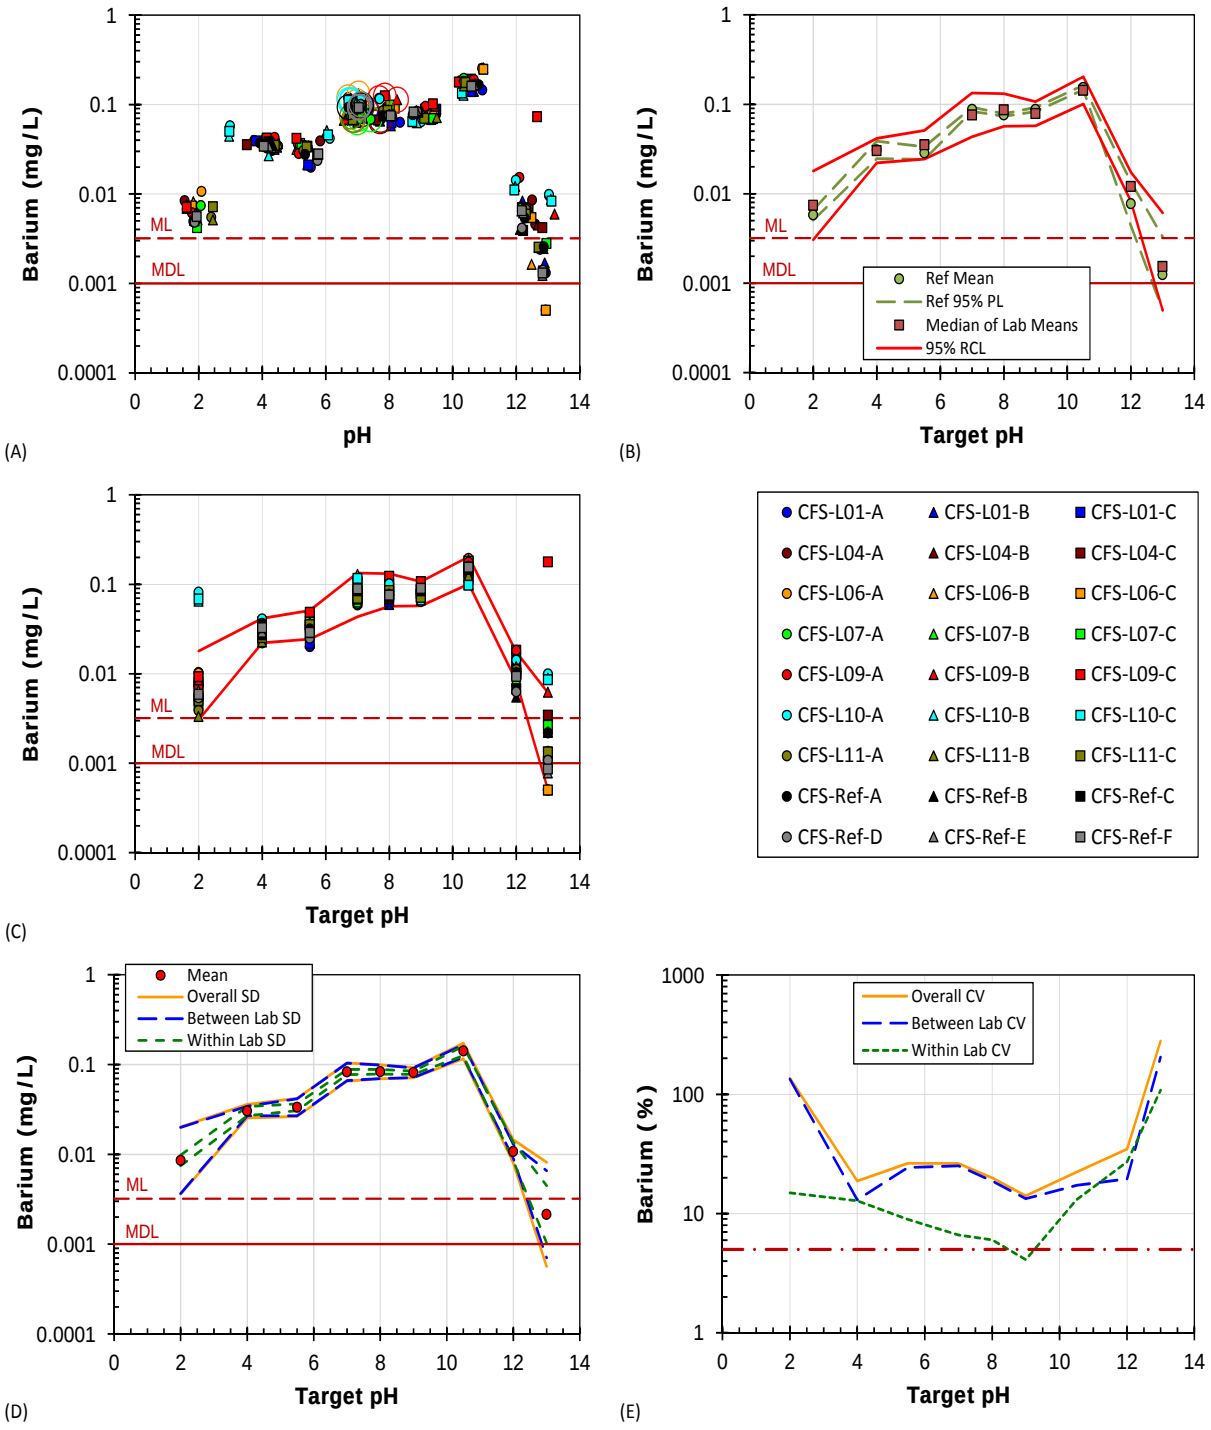

Figure 23. Barium statistical analysis for Method 1313 Phase II material CFS. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

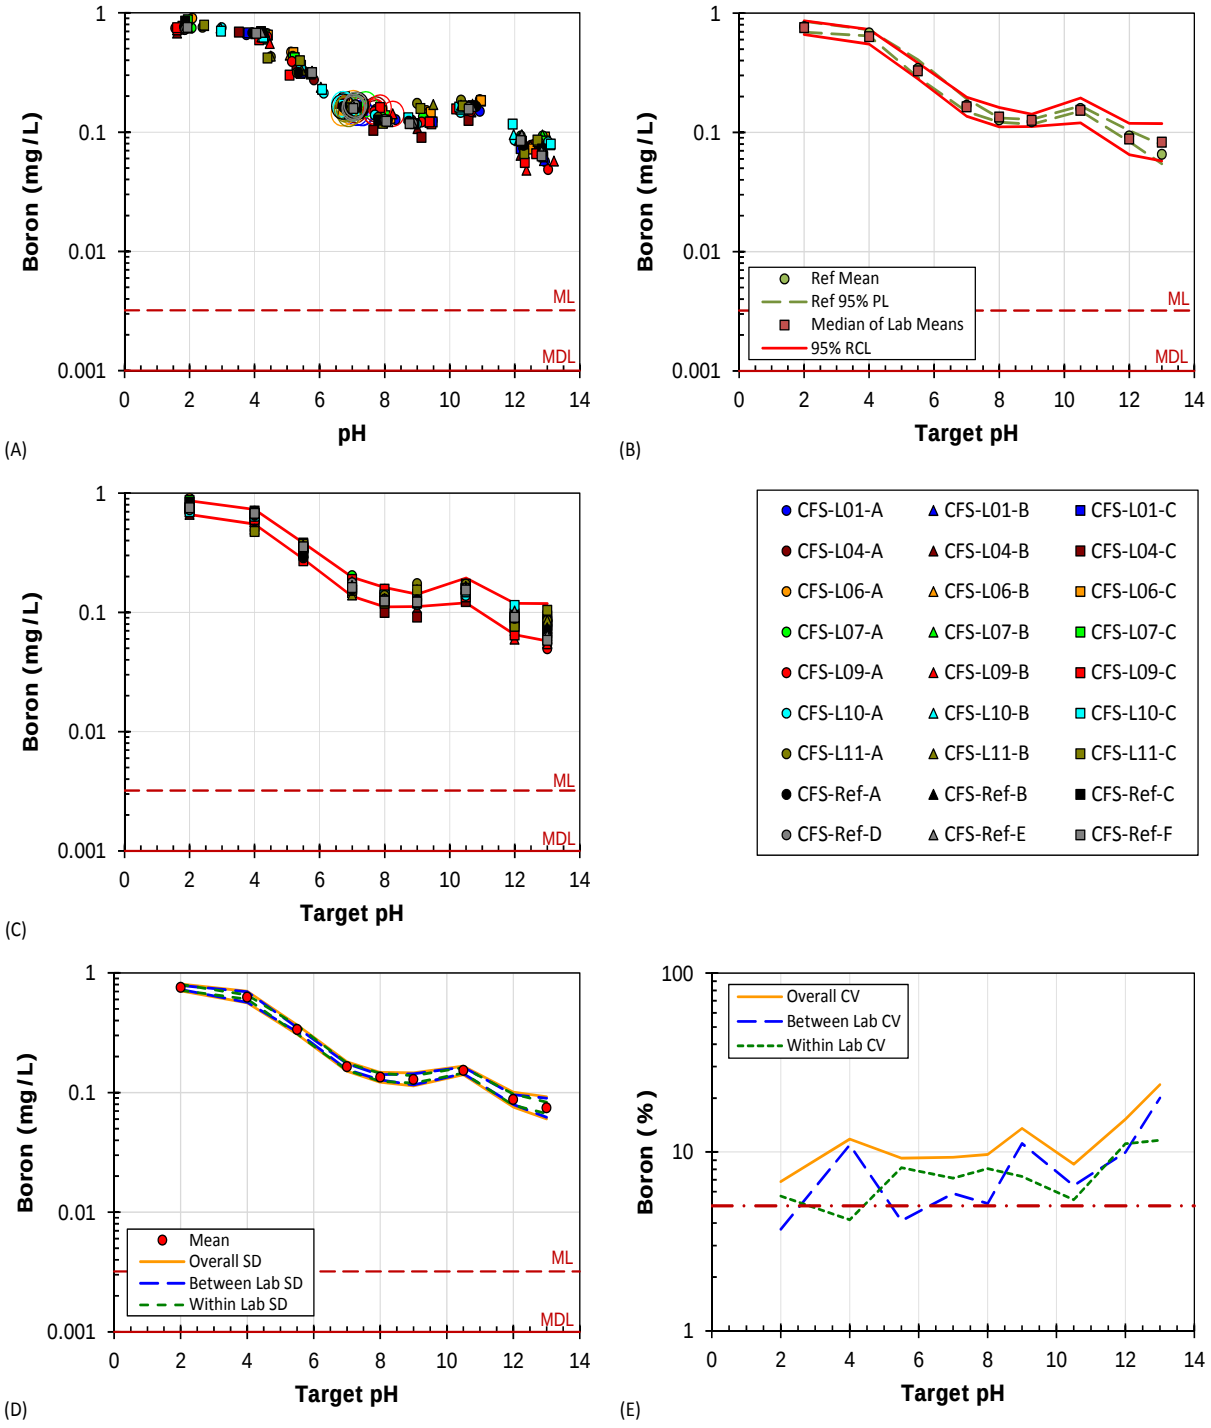

Figure 24. Boron statistical analysis for Method 1313 Phase II material CFS. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

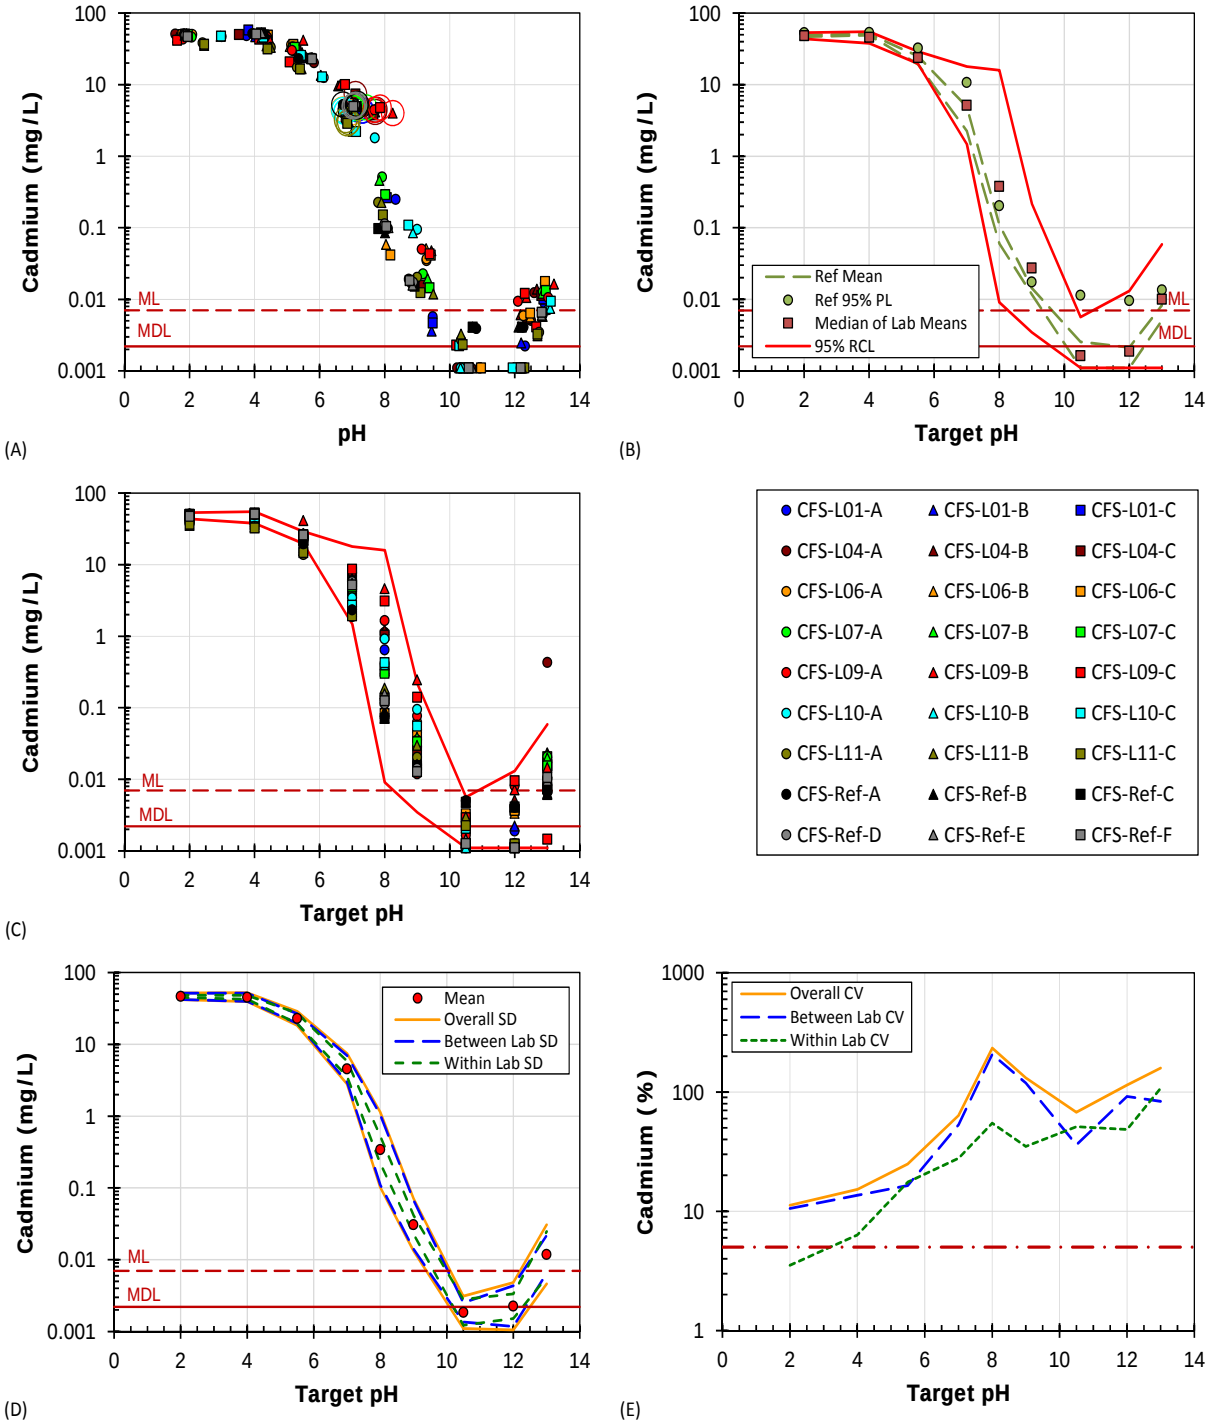

Figure 25. Cadmium statistical analysis for Method 1313 Phase II material CFS. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

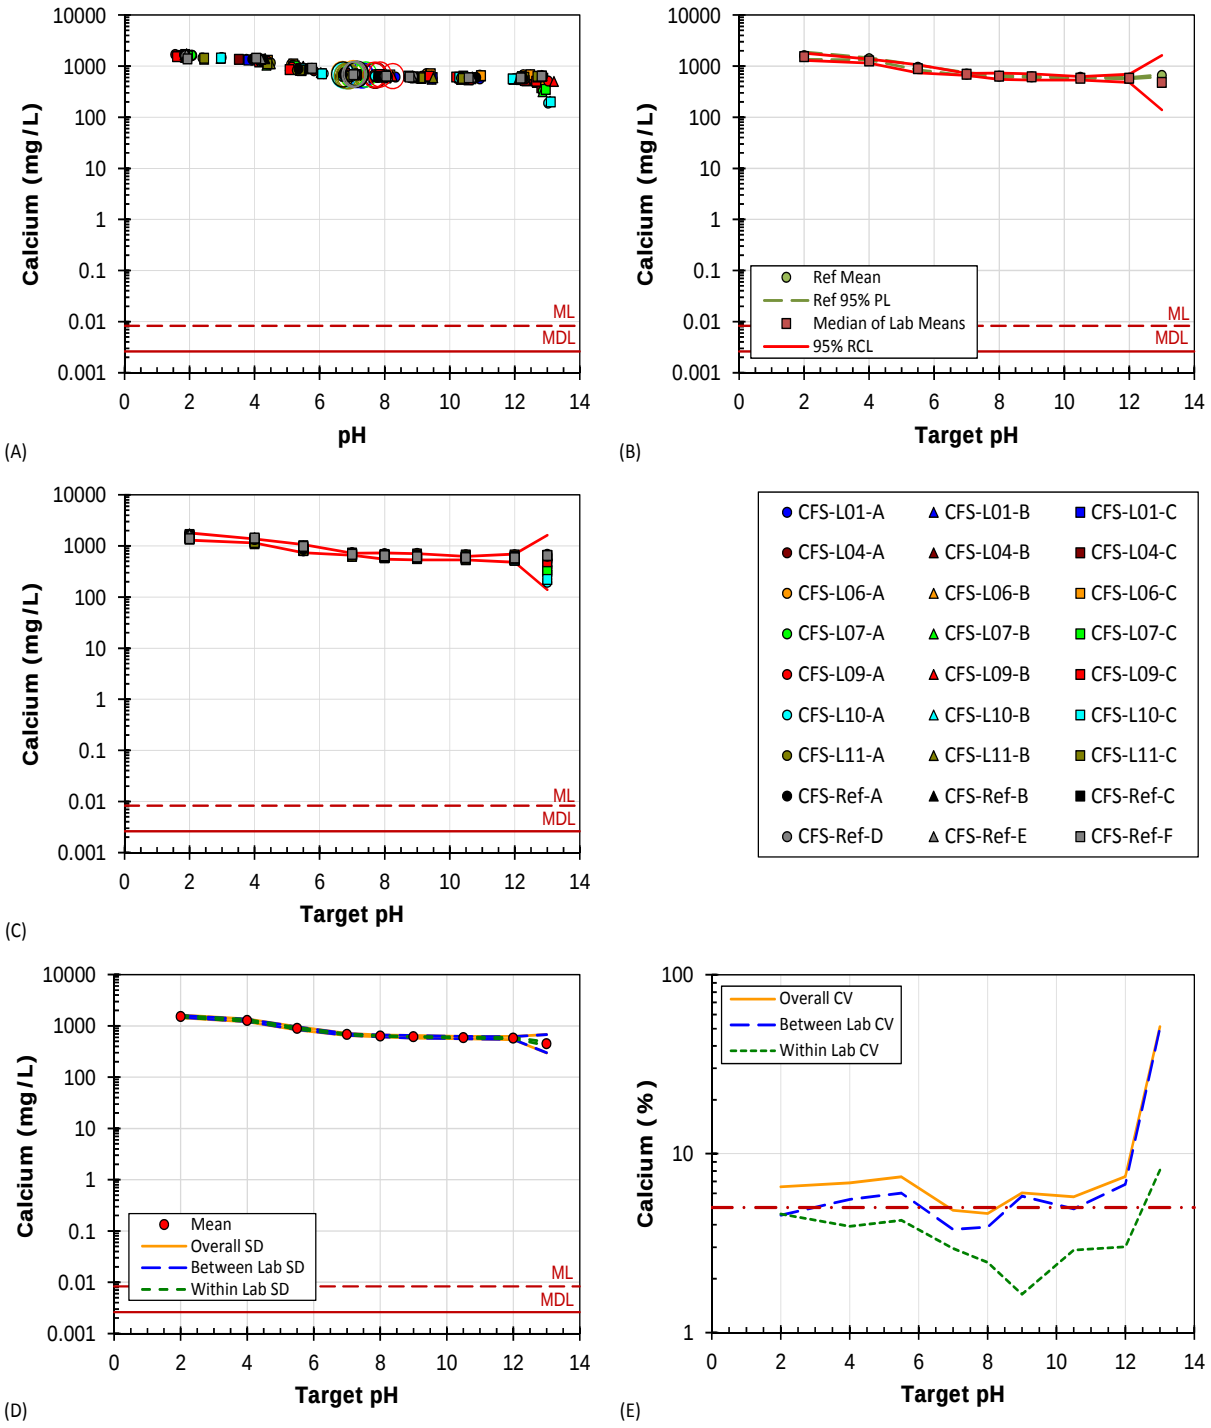

Figure 26. Calcium statistical analysis for Method 1313 Phase II material CFS. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

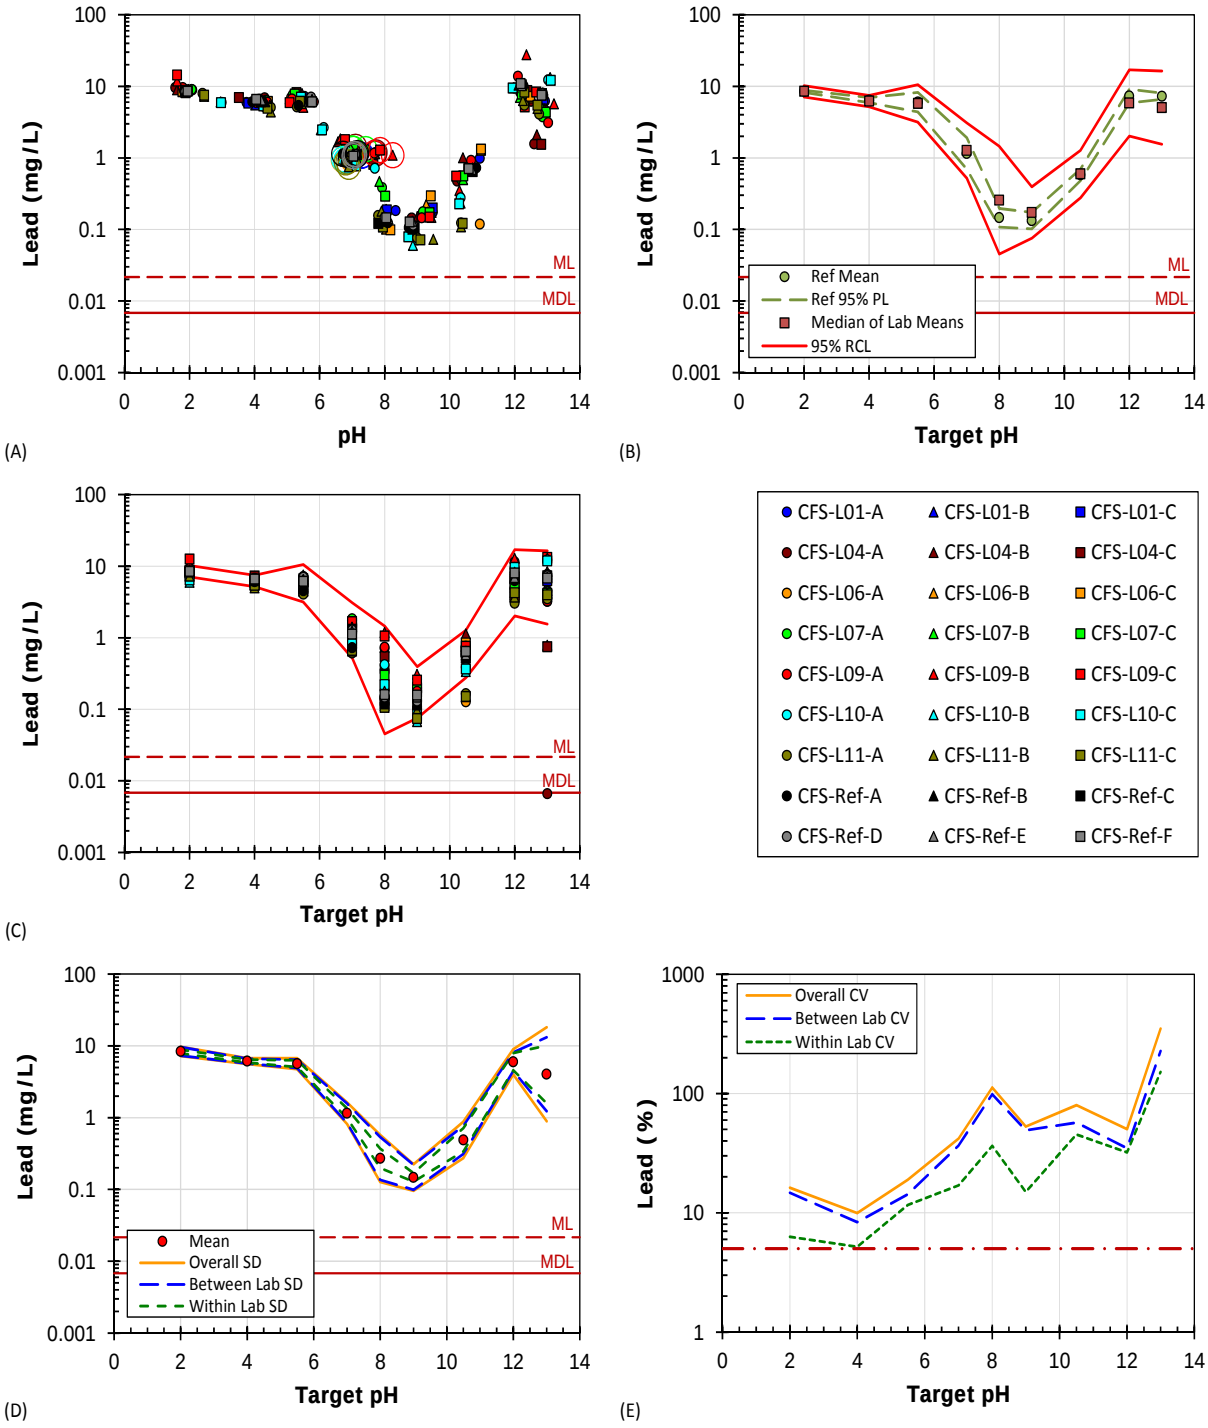

Figure 27. Lead statistical analysis for Method 1313 Phase II material CFS. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

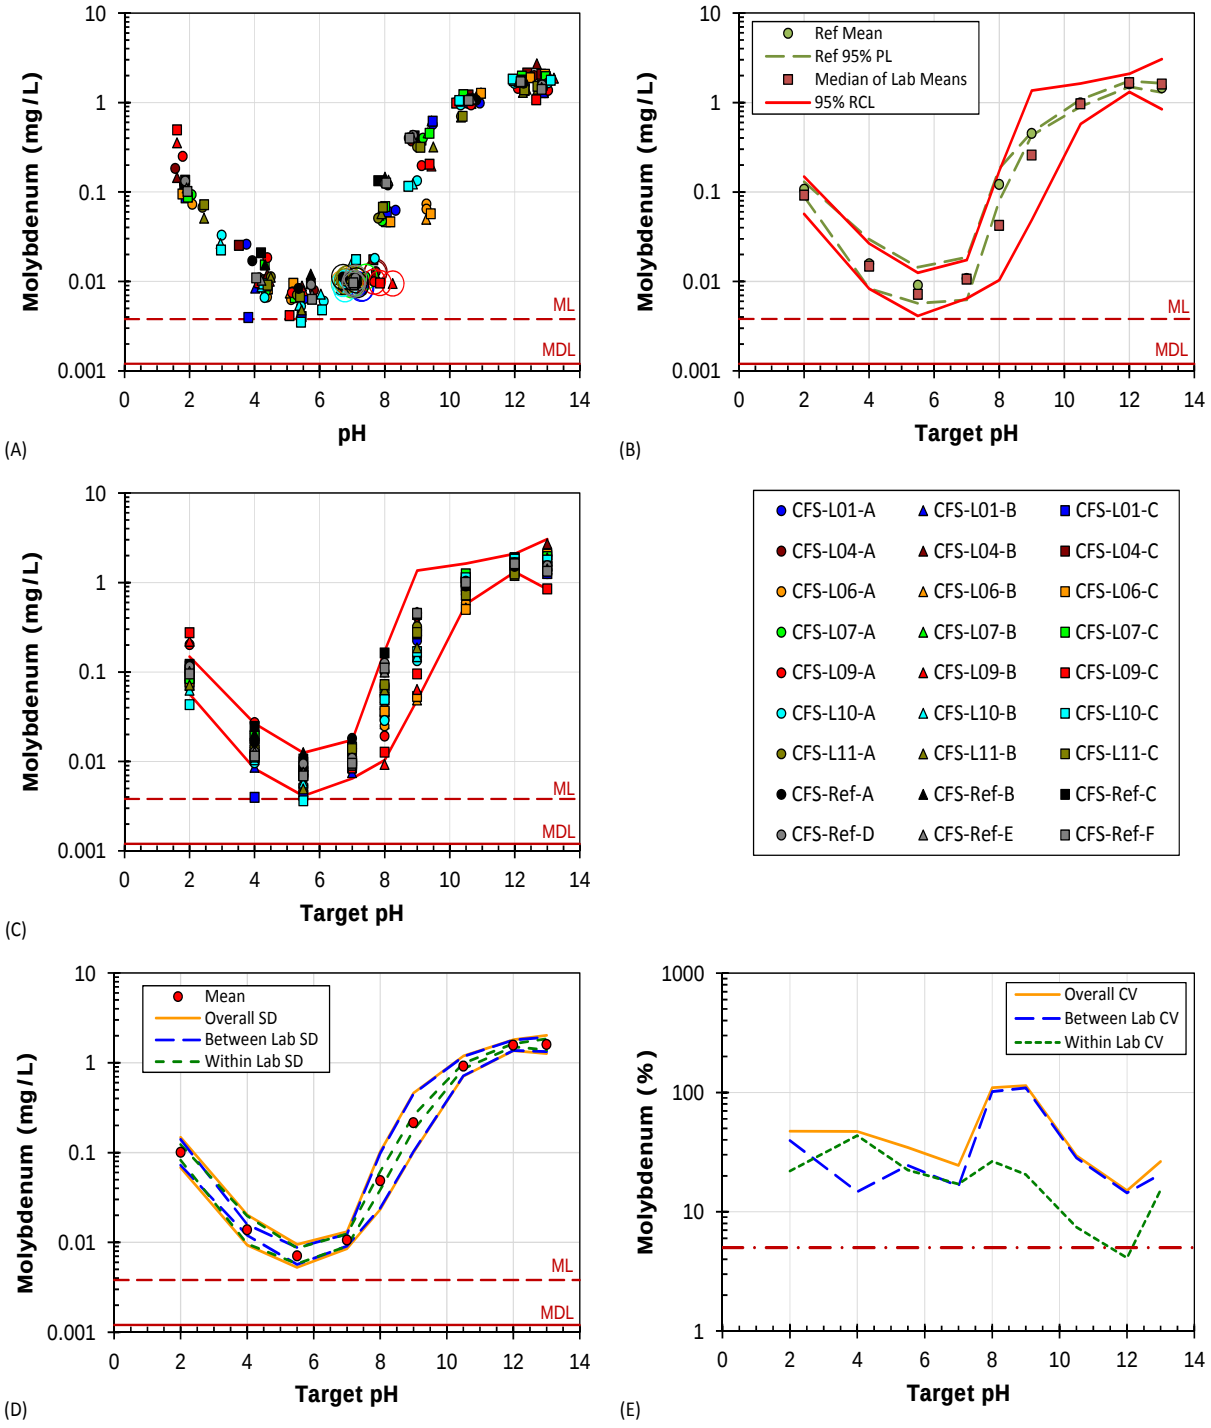

Figure 28. Molybdenum statistical analysis for Method 1313 Phase II material CFS. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

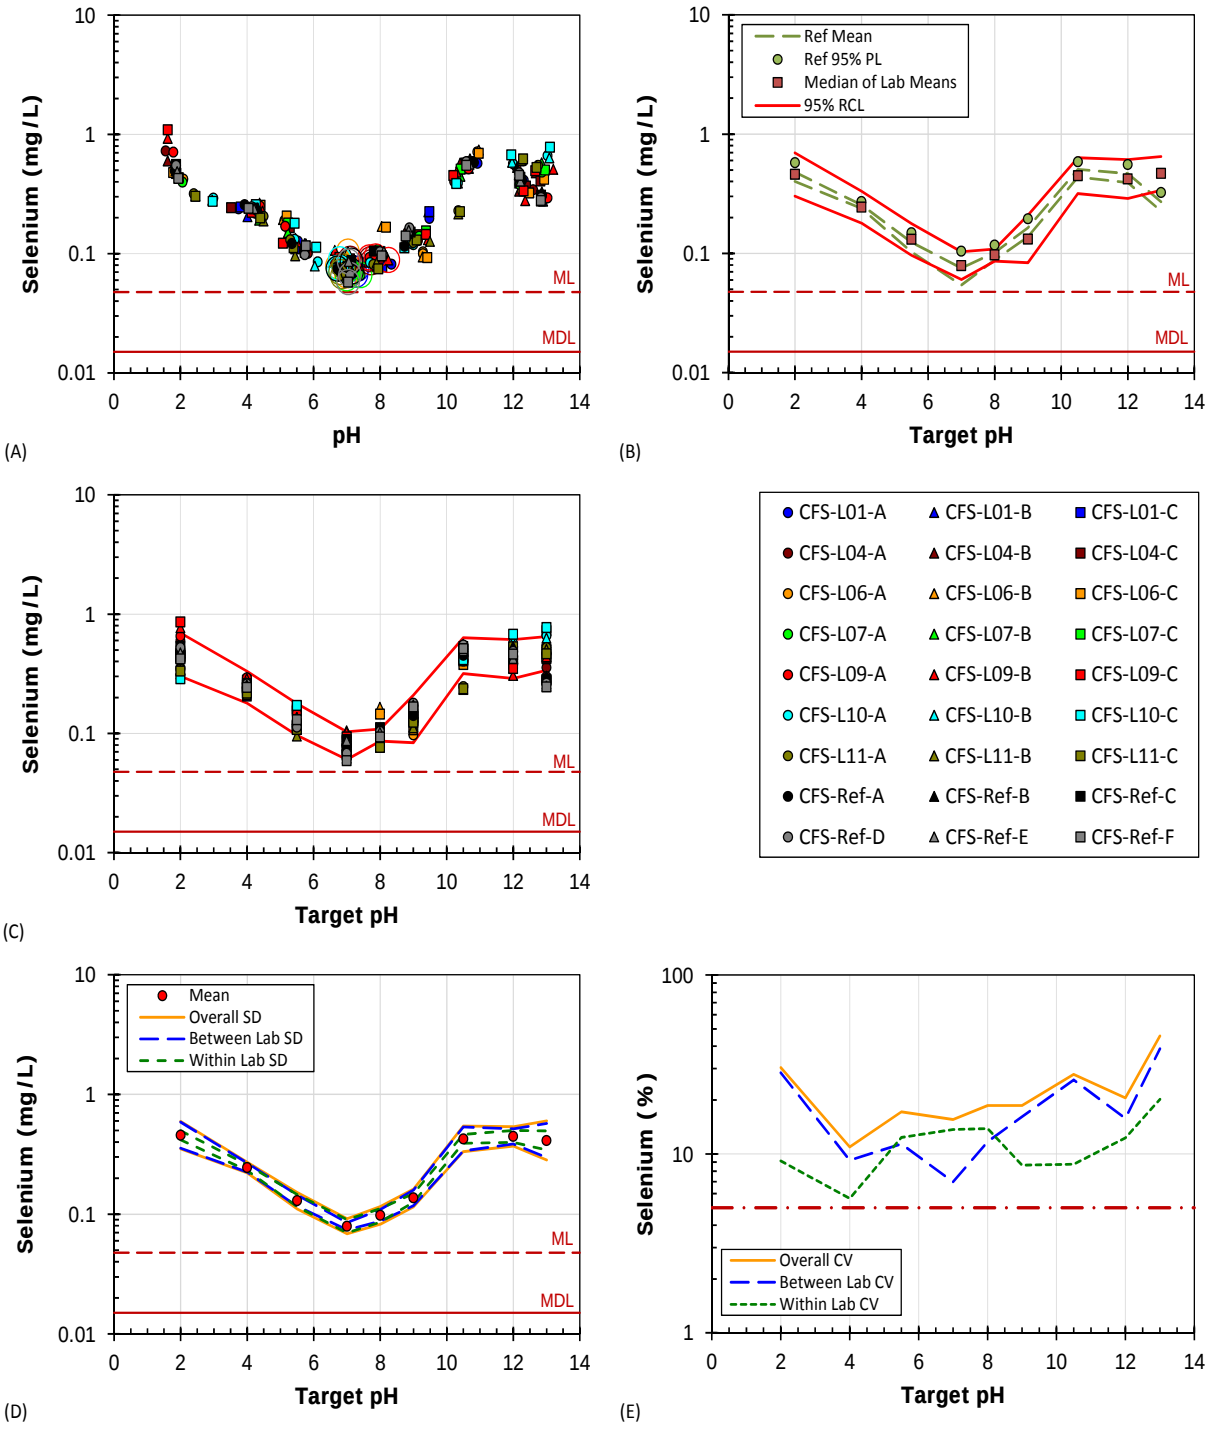

Figure 29. Selenium statistical analysis for Method 1313 Phase II material CFS. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

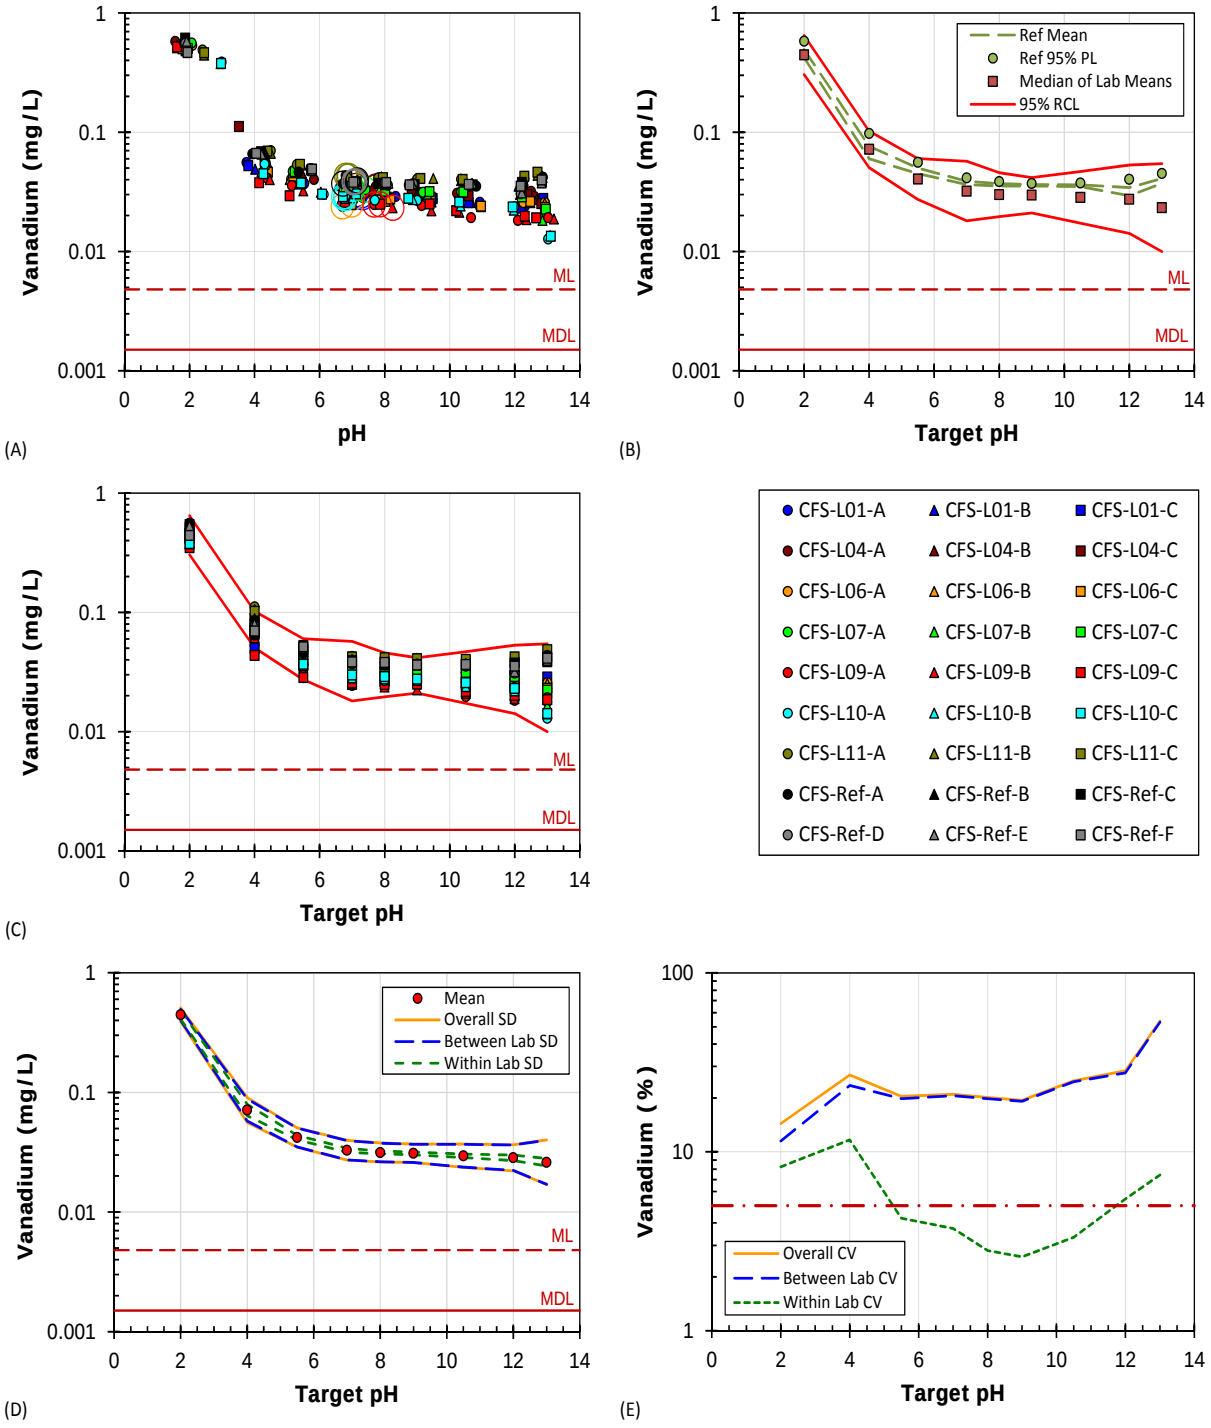

Figure 30. Vanadium statistical analysis for Method 1313 Phase II material CFS. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

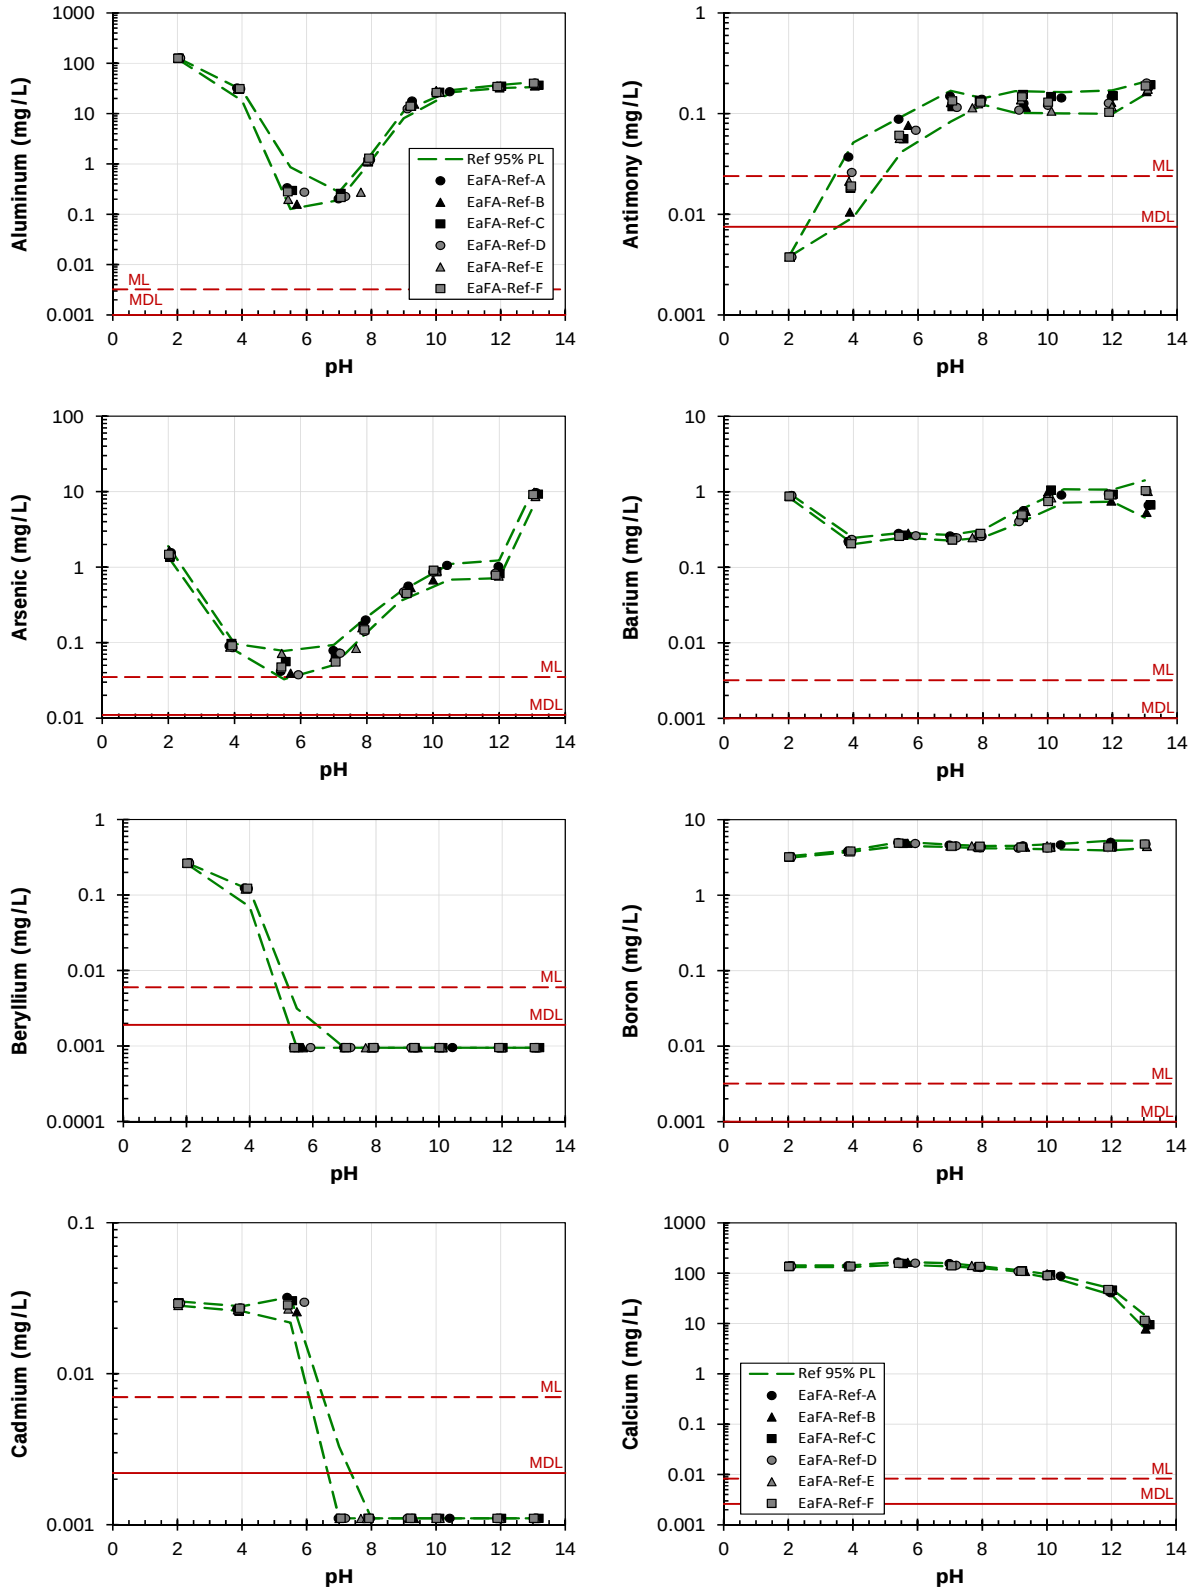

Figure 31. Reference lab data and 95% prediction limits for Method 1313 Phase I EaFA material.

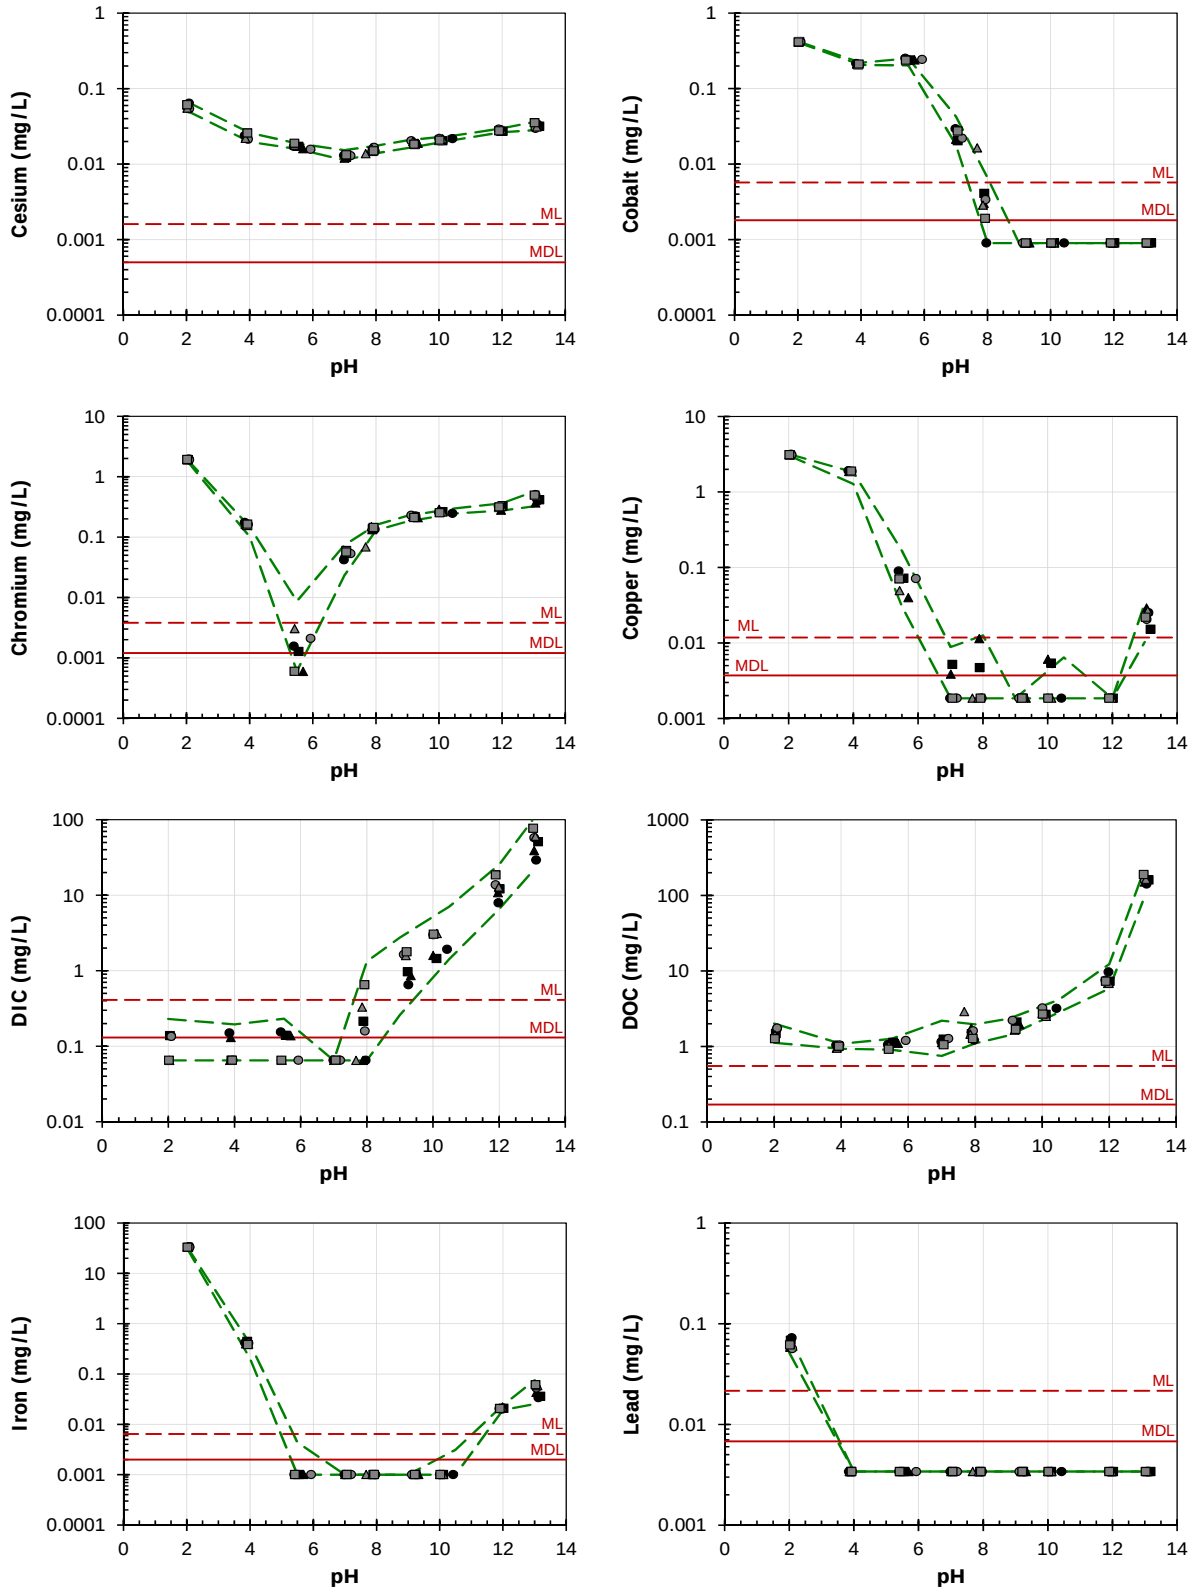

Figure 32. Reference lab data and 95% prediction limits for Method 1313 Phase I EaFA material.

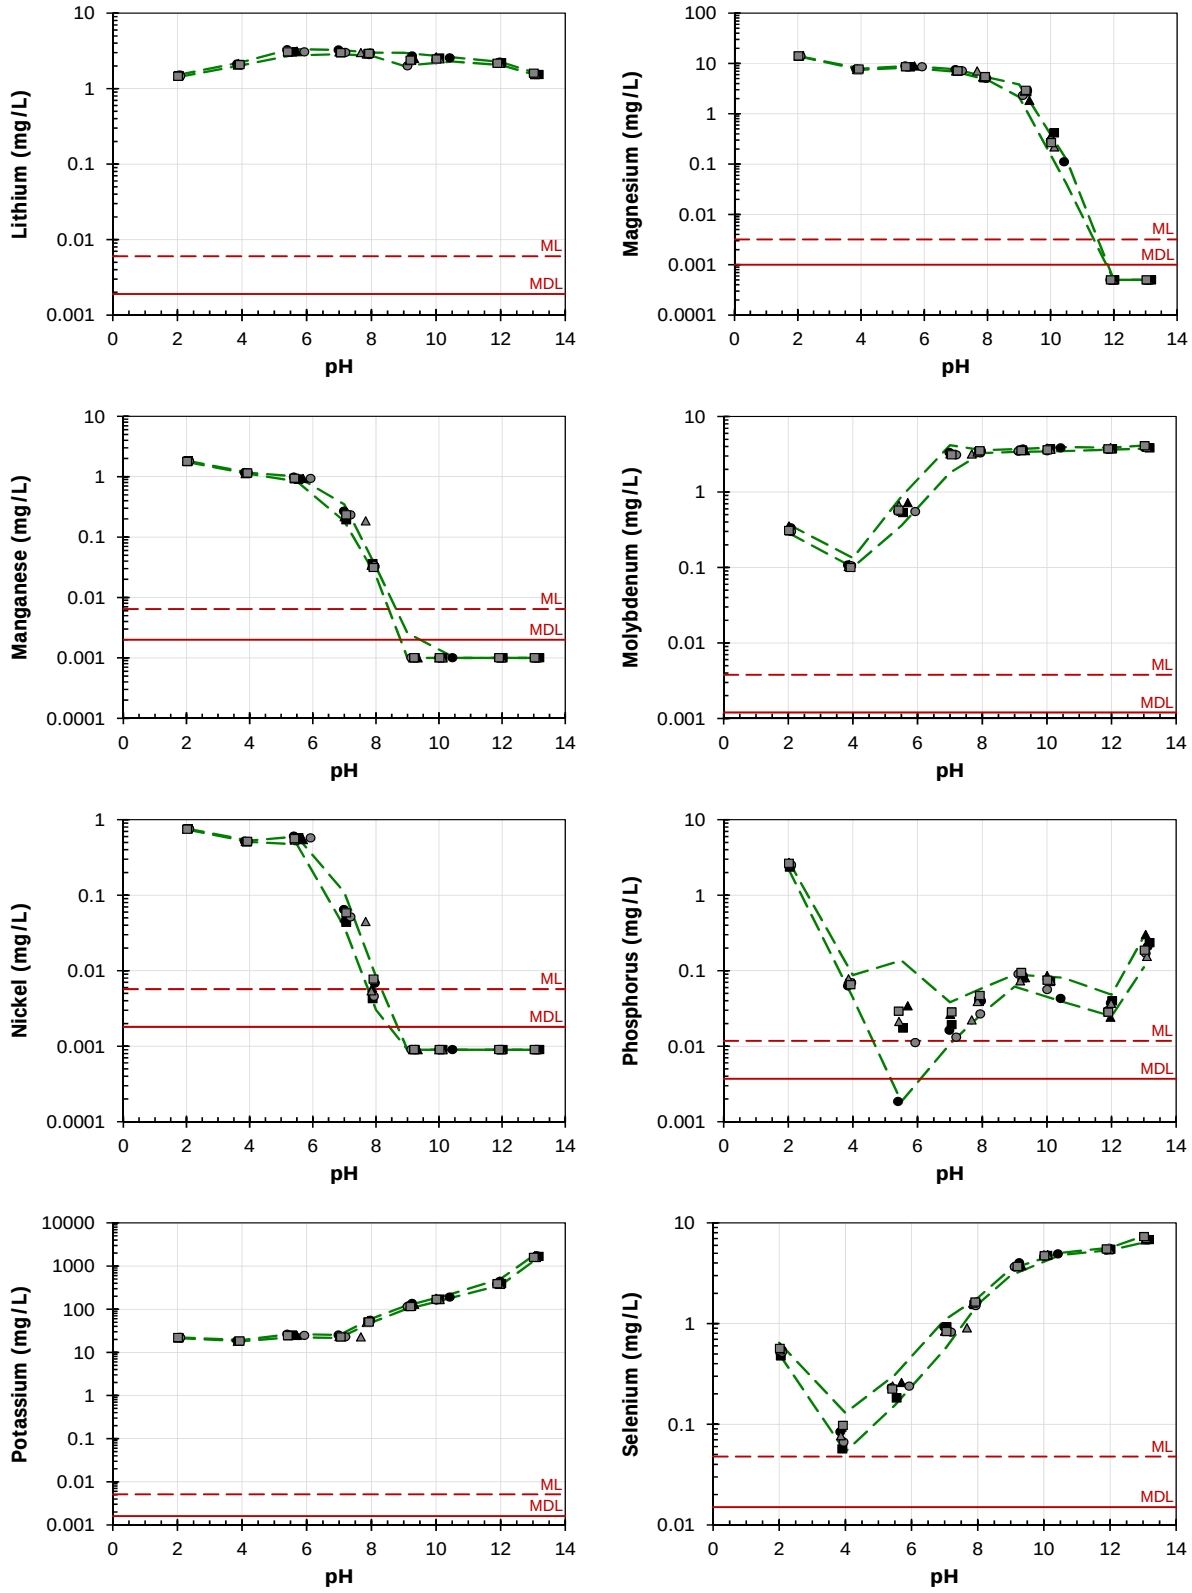

Figure 33. Reference lab data and 95% prediction limits for Method 1313 Phase I EaFA material.

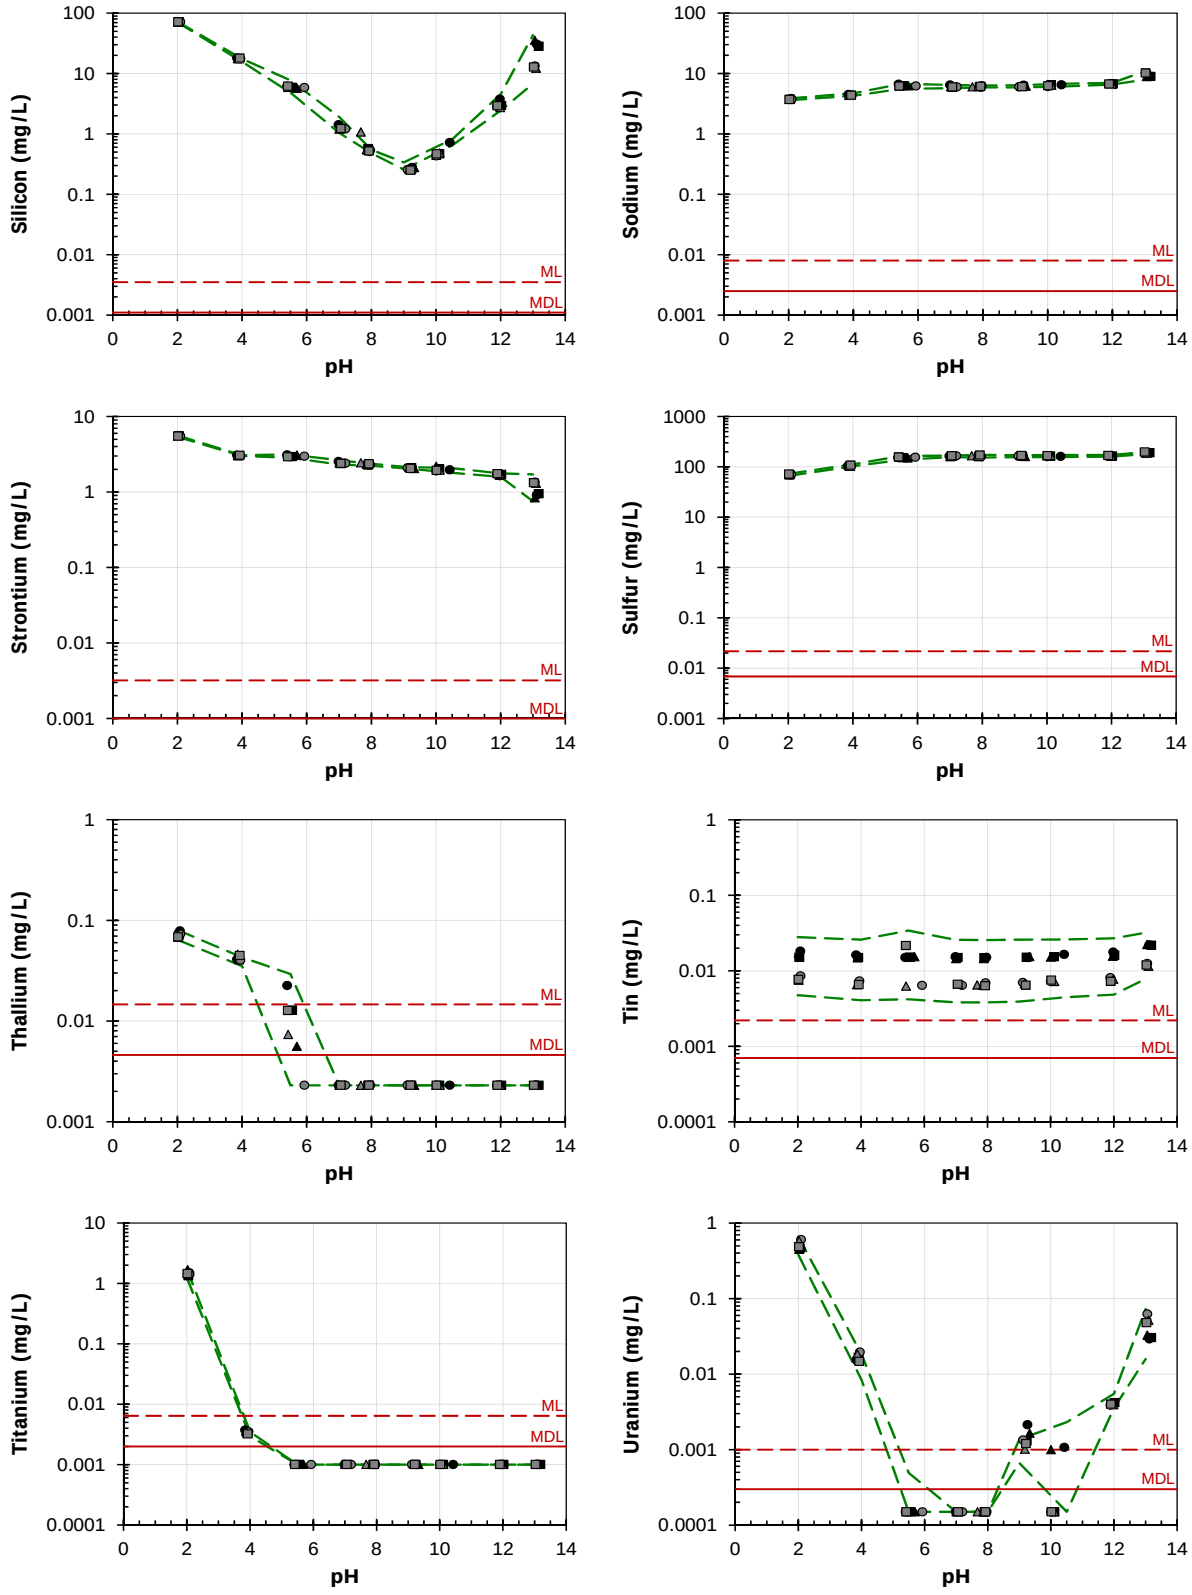

Figure 34. Reference lab data and 95% prediction limits for Method 1313 Phase I EaFA material.

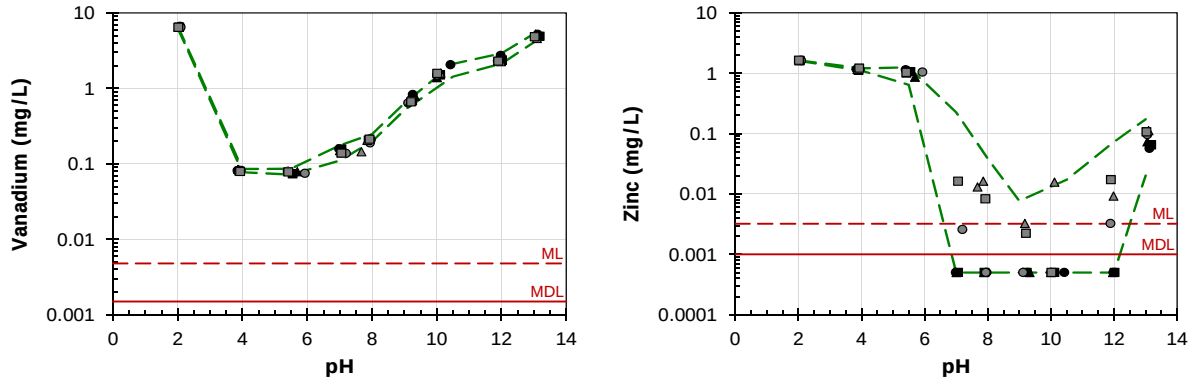

Figure 35. Reference lab data and 95% prediction limits for Method 1313 Phase I EaFA material.

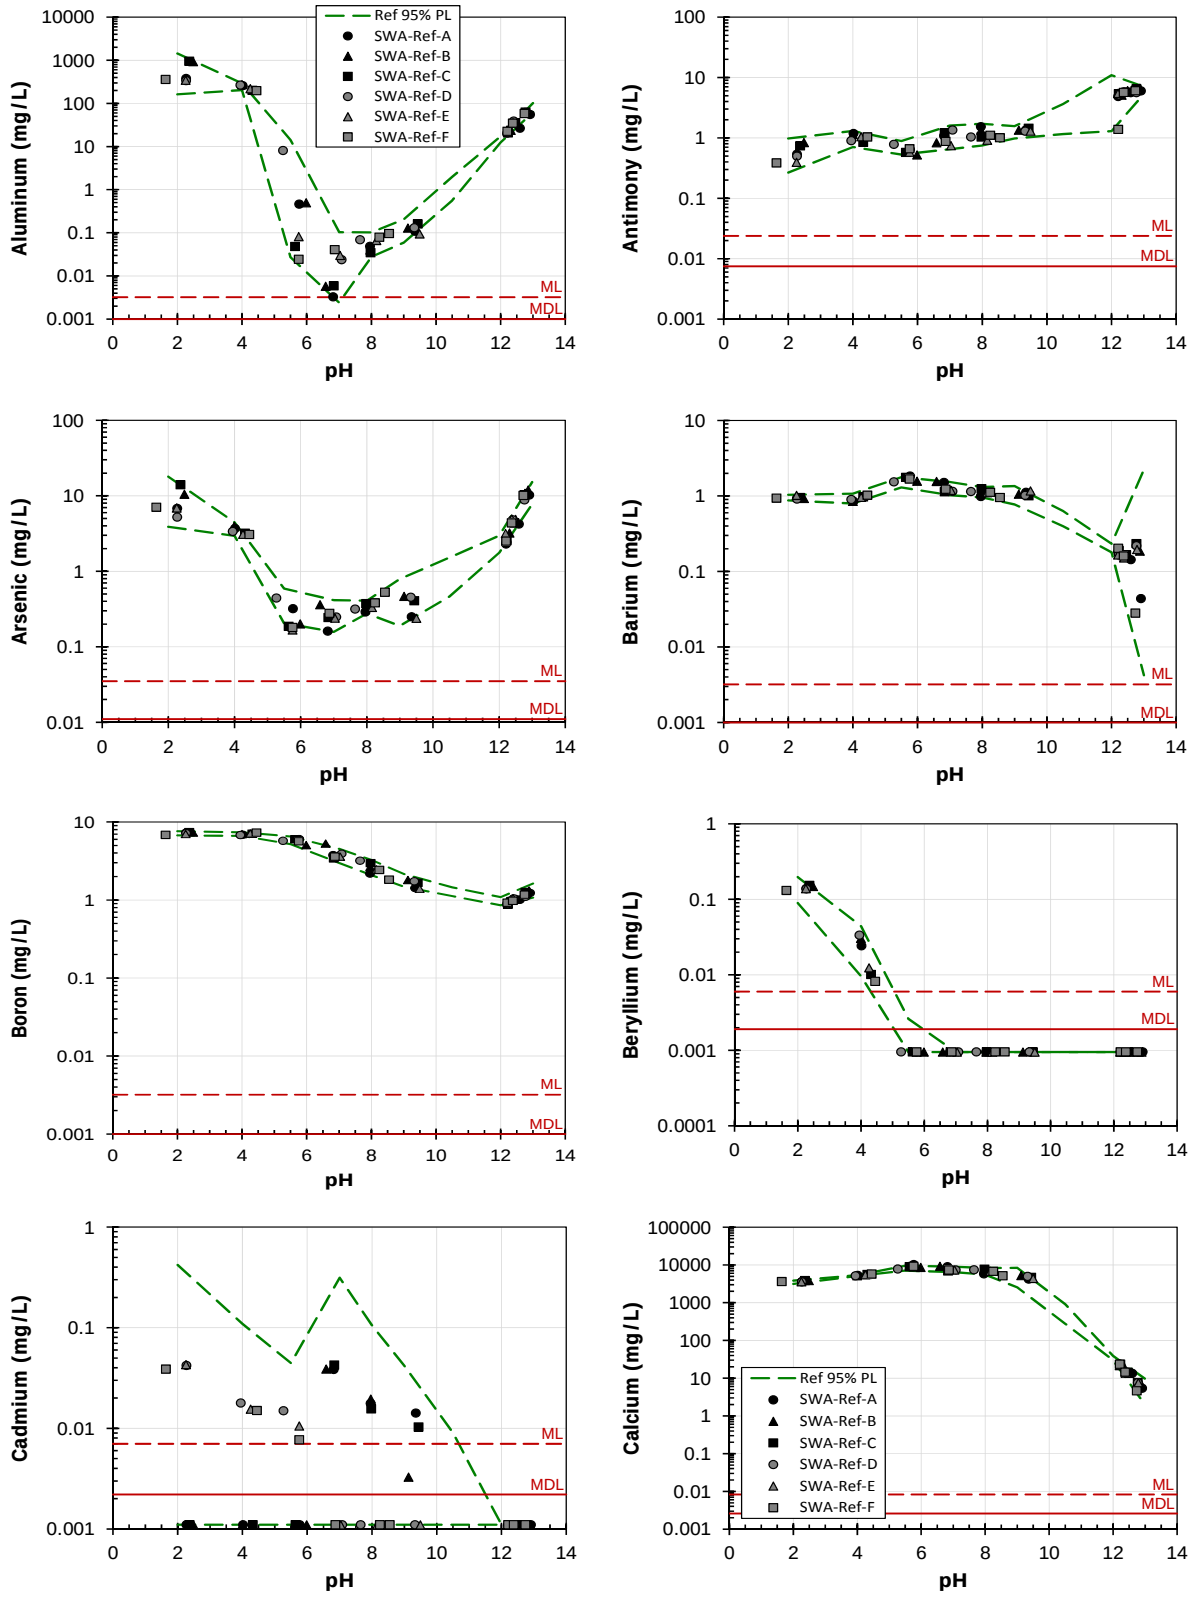

Figure 36. Reference lab data and 95% prediction limits for Method 1313 Phase II SWA material.

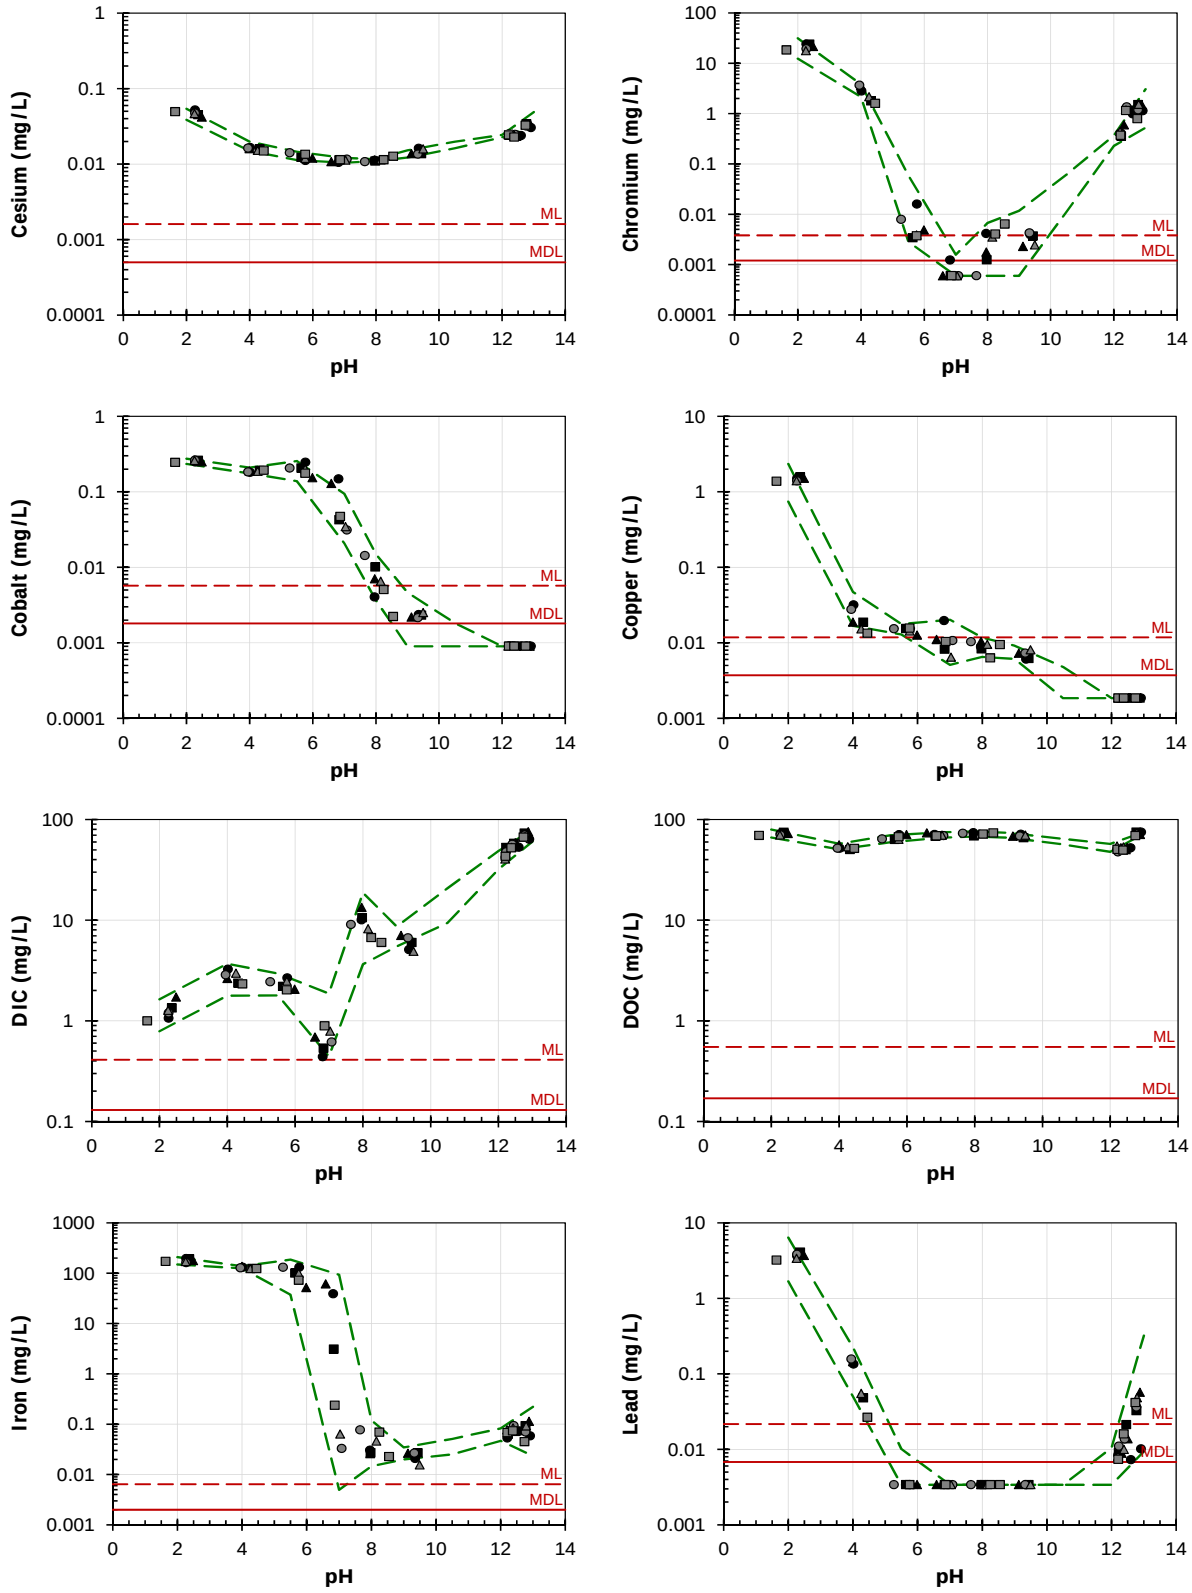

Figure 37. Reference lab data and 95% prediction limits for Method 1313 Phase II SWA material.

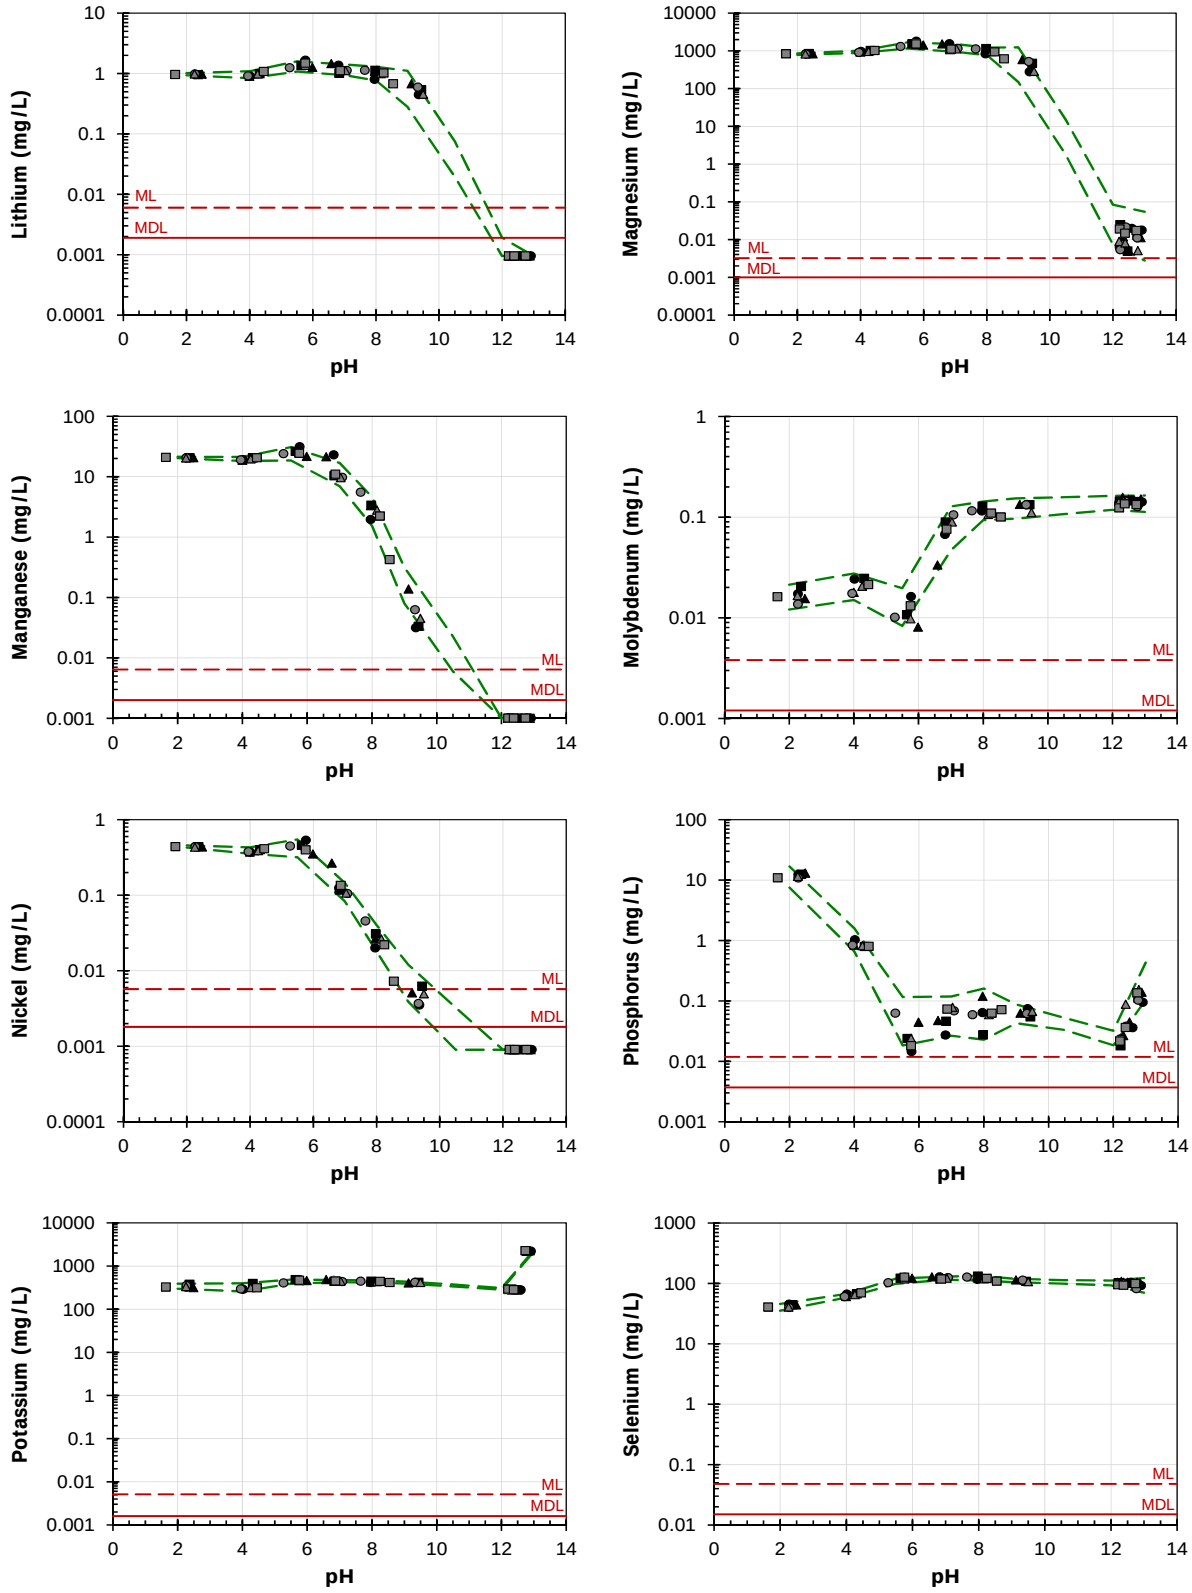

Figure 38. Reference lab data and 95% prediction limits for Method 1313 Phase II SWA material.

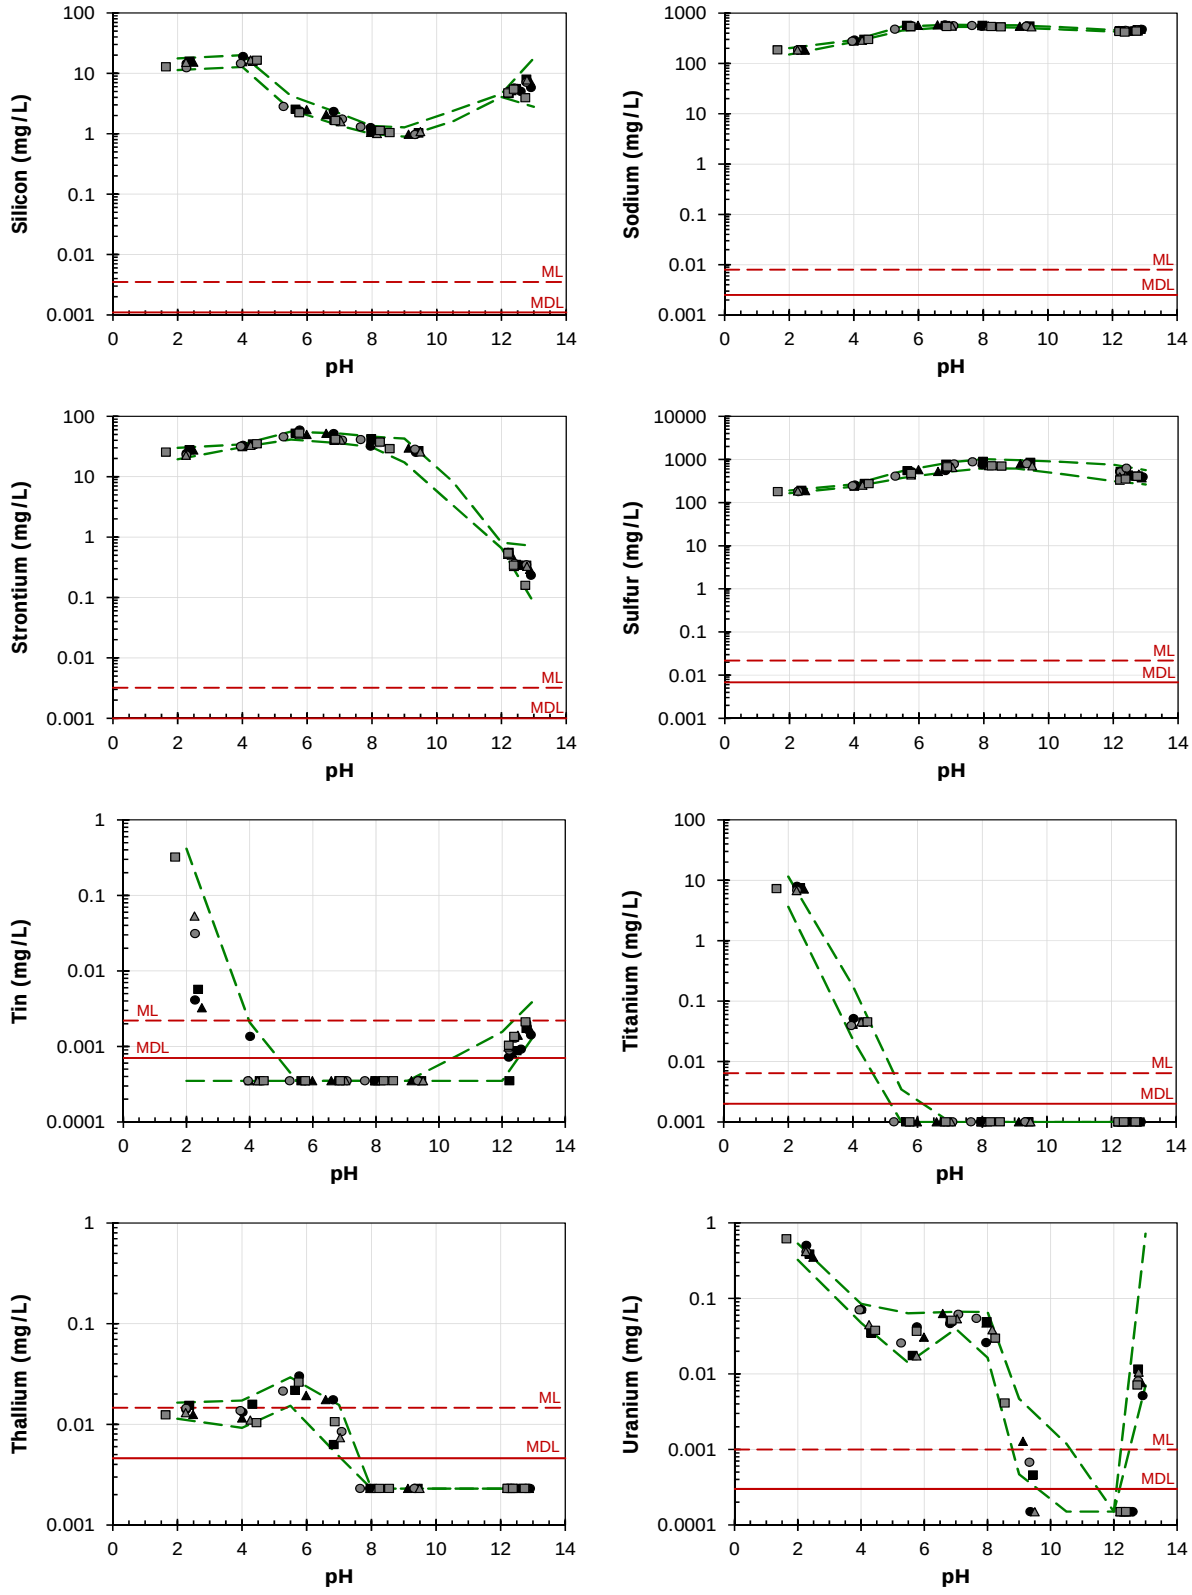

Figure 39. Reference lab data and 95% prediction limits for Method 1313 Phase II SWA material.

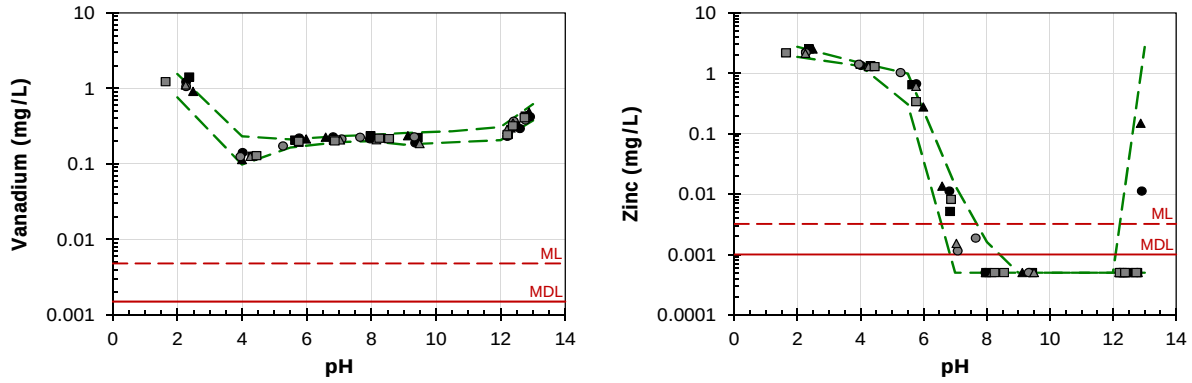

Figure 40. Reference lab data and 95% prediction limits for Method 1313 Phase II SWA material.

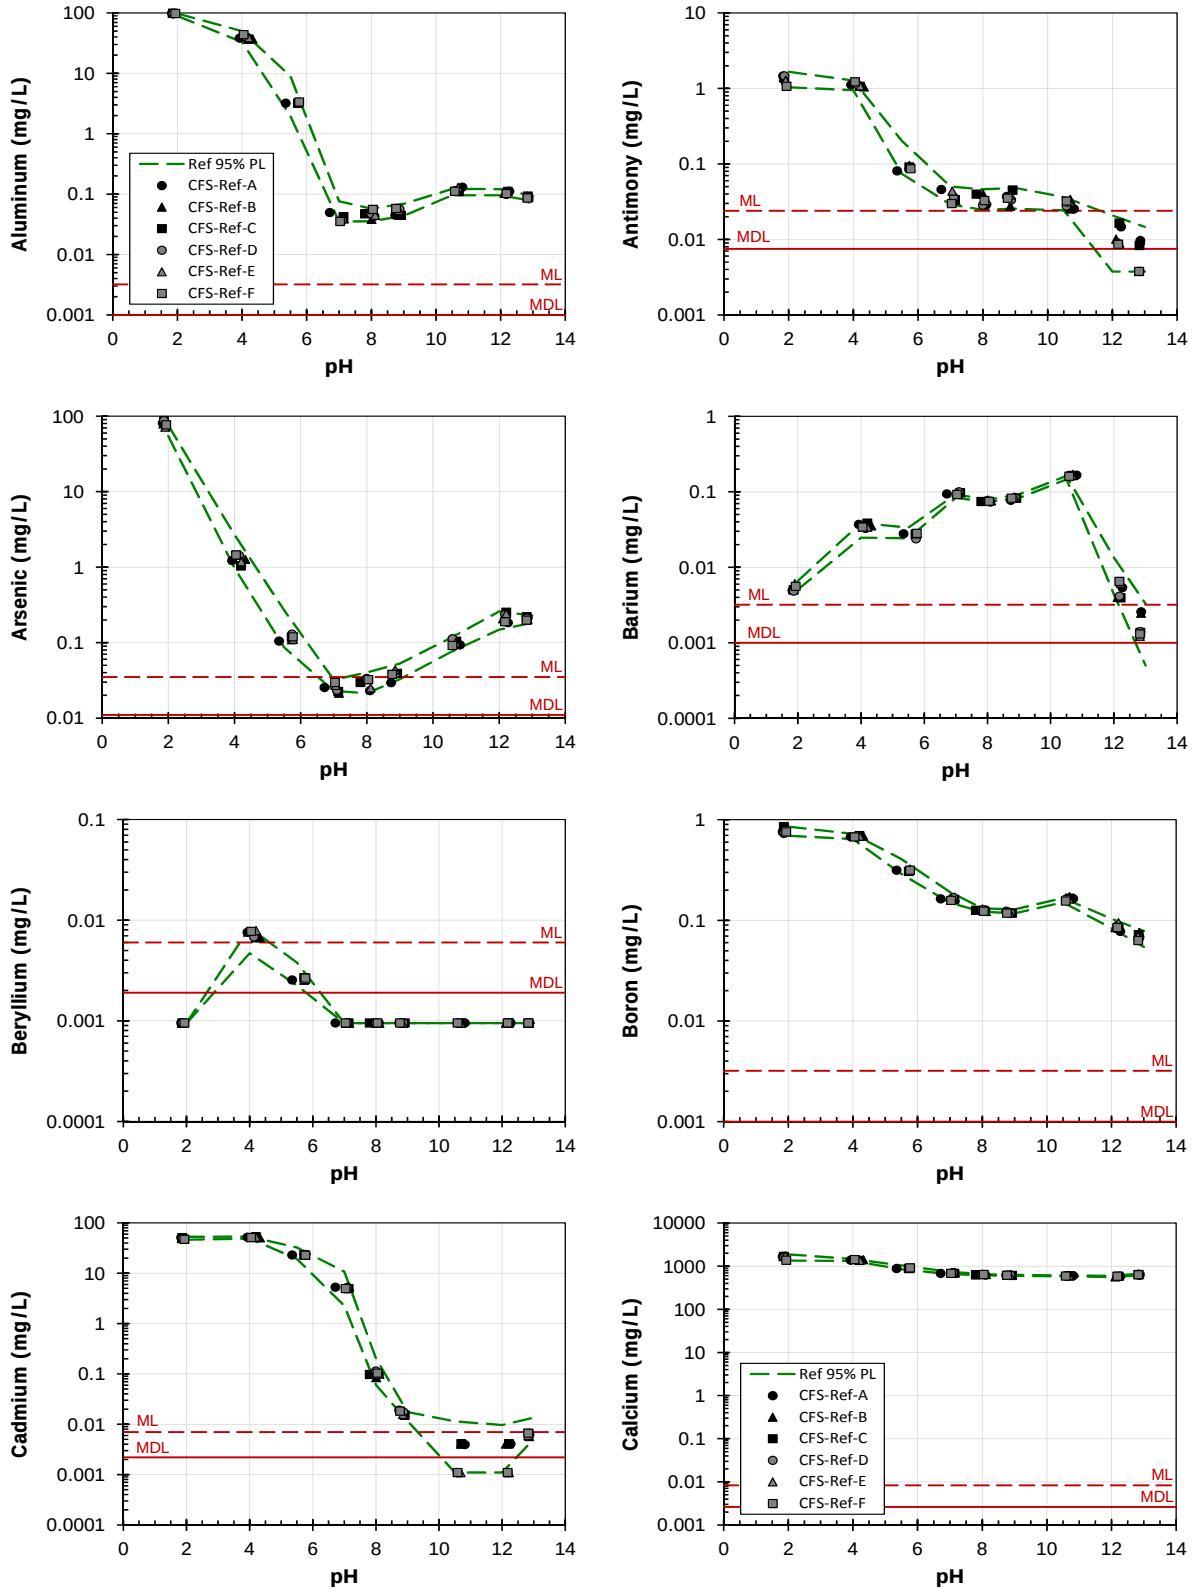

Figure 41. Reference lab data and 95% prediction limits for Method 1313 Phase II CFS material.

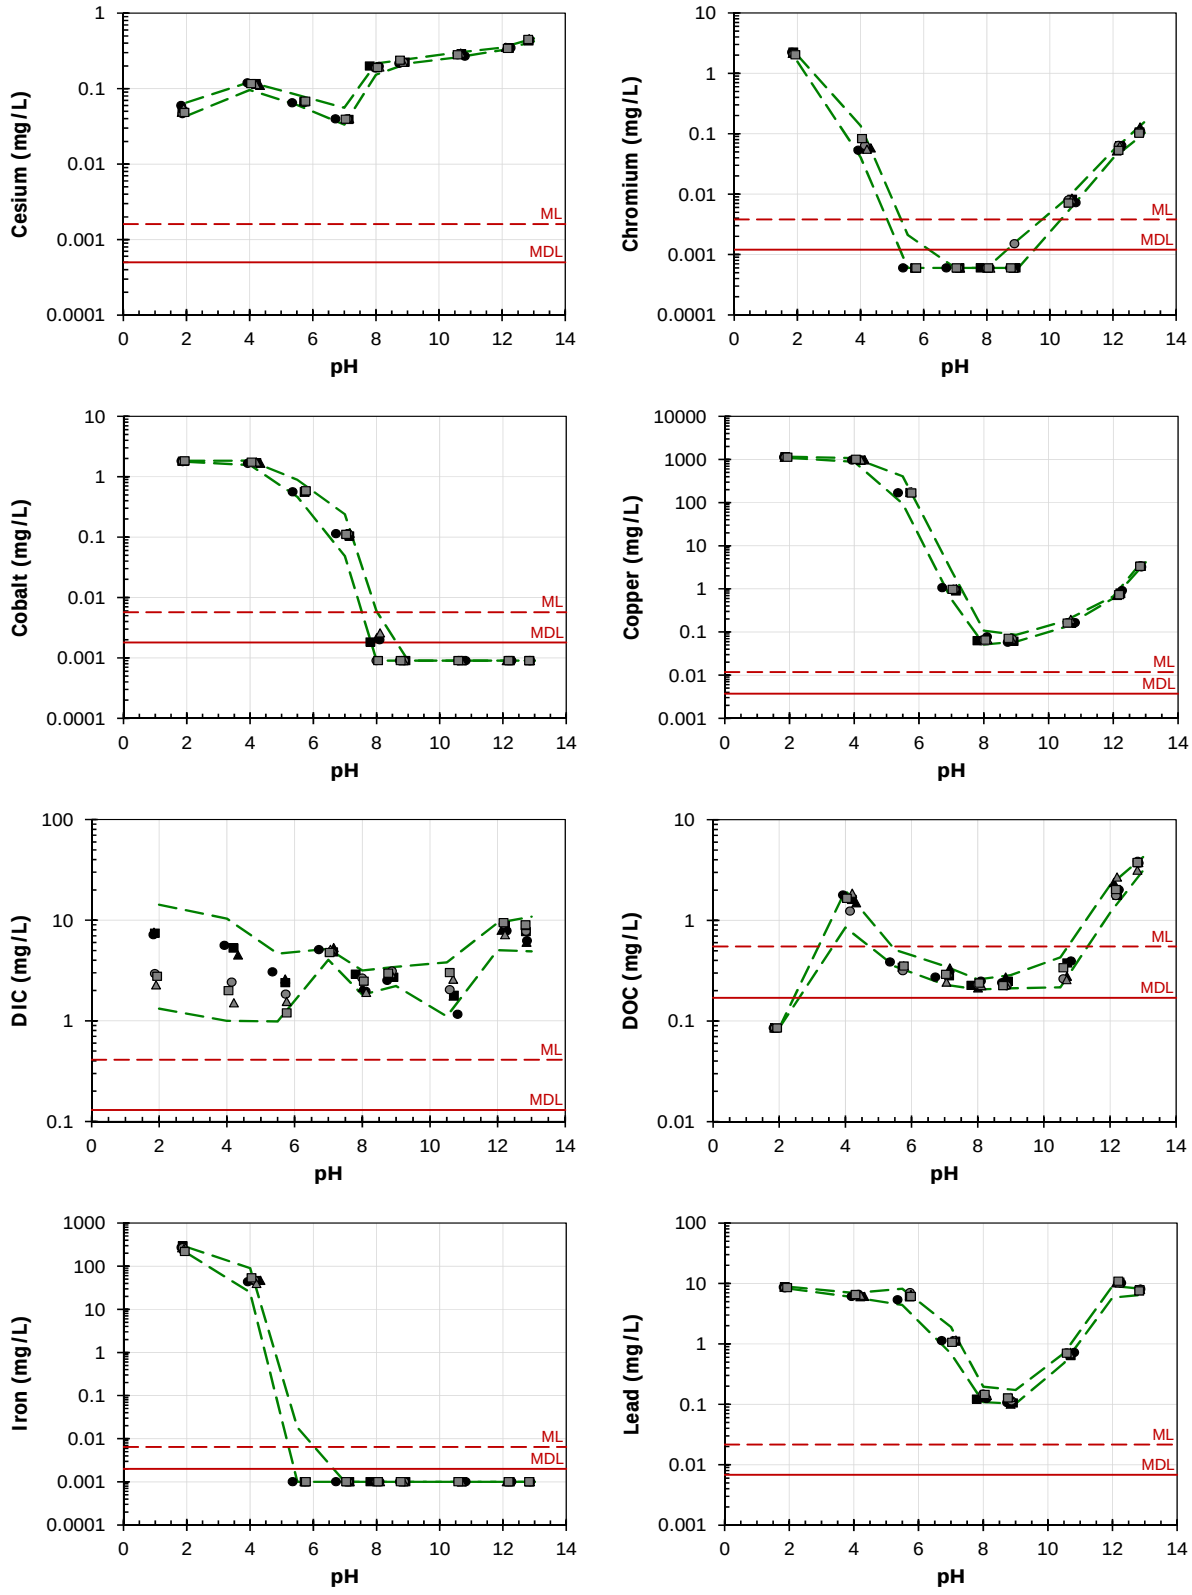

Figure 42. Reference lab data and 95% prediction limits for Method 1313 Phase II CFS material.

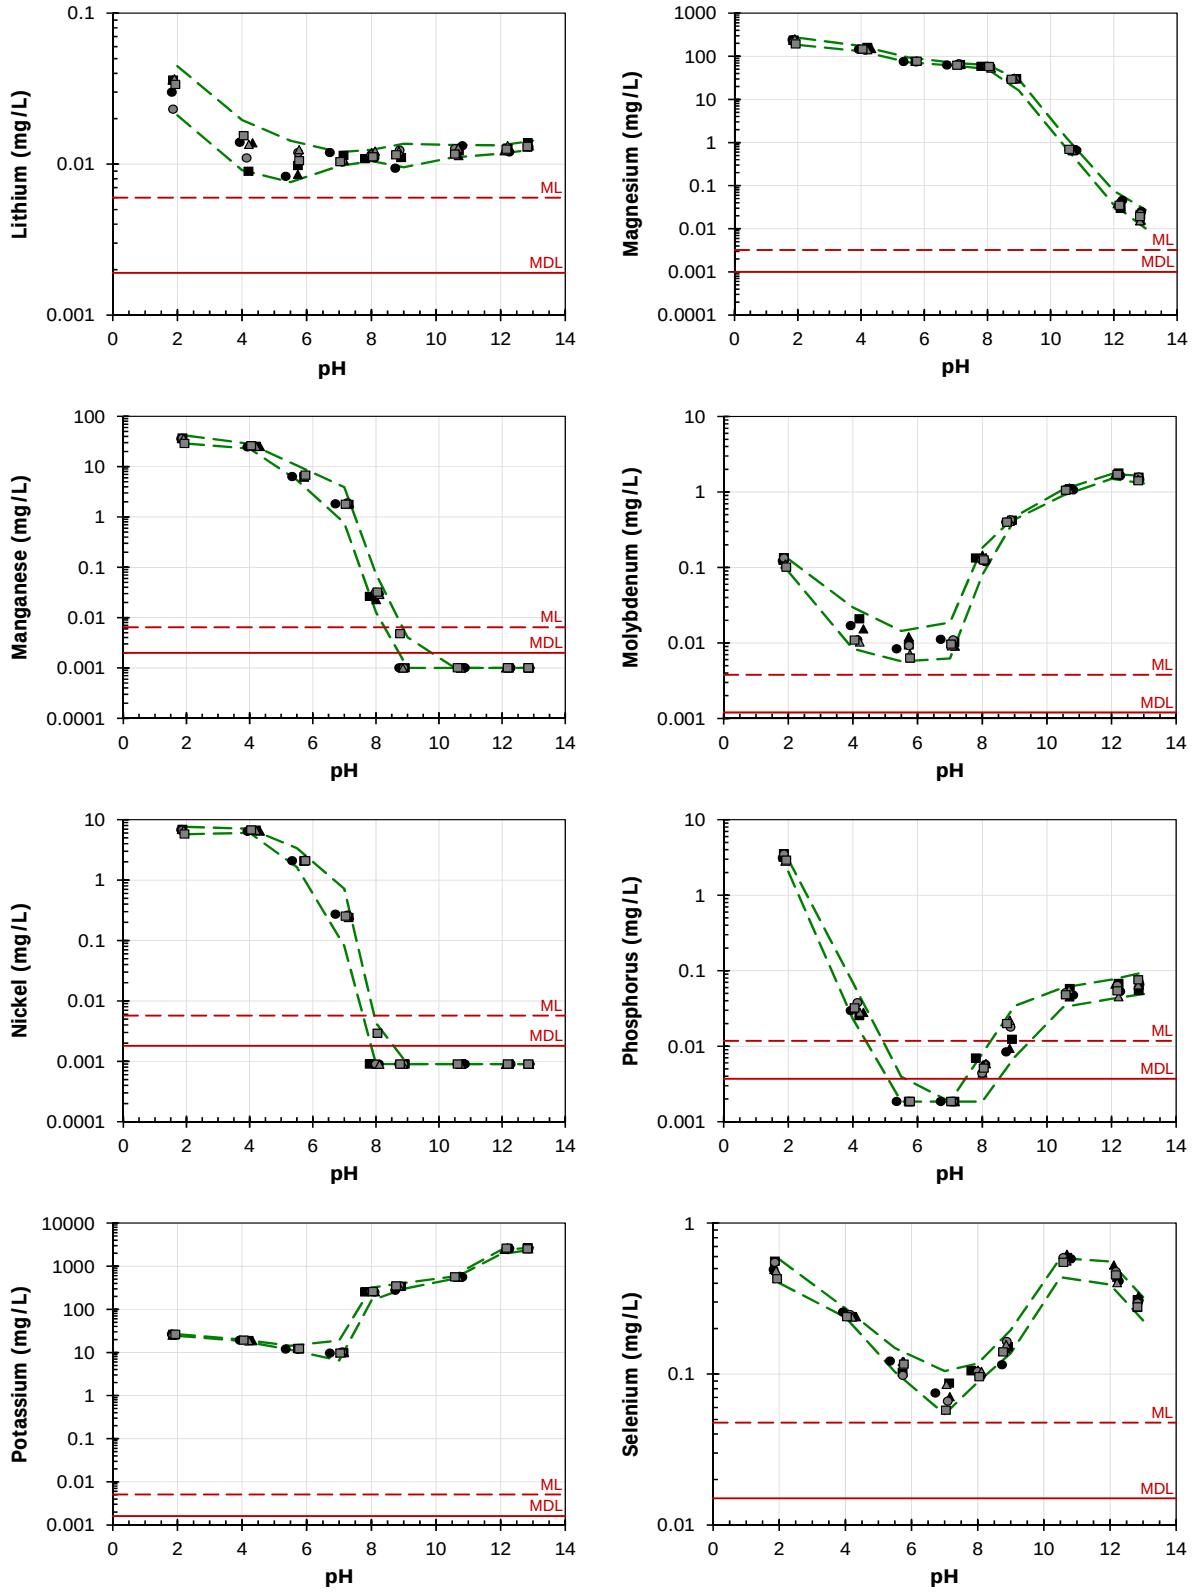

Figure 43. Reference lab data and 95% prediction limits for Method 1313 Phase II CFS material.

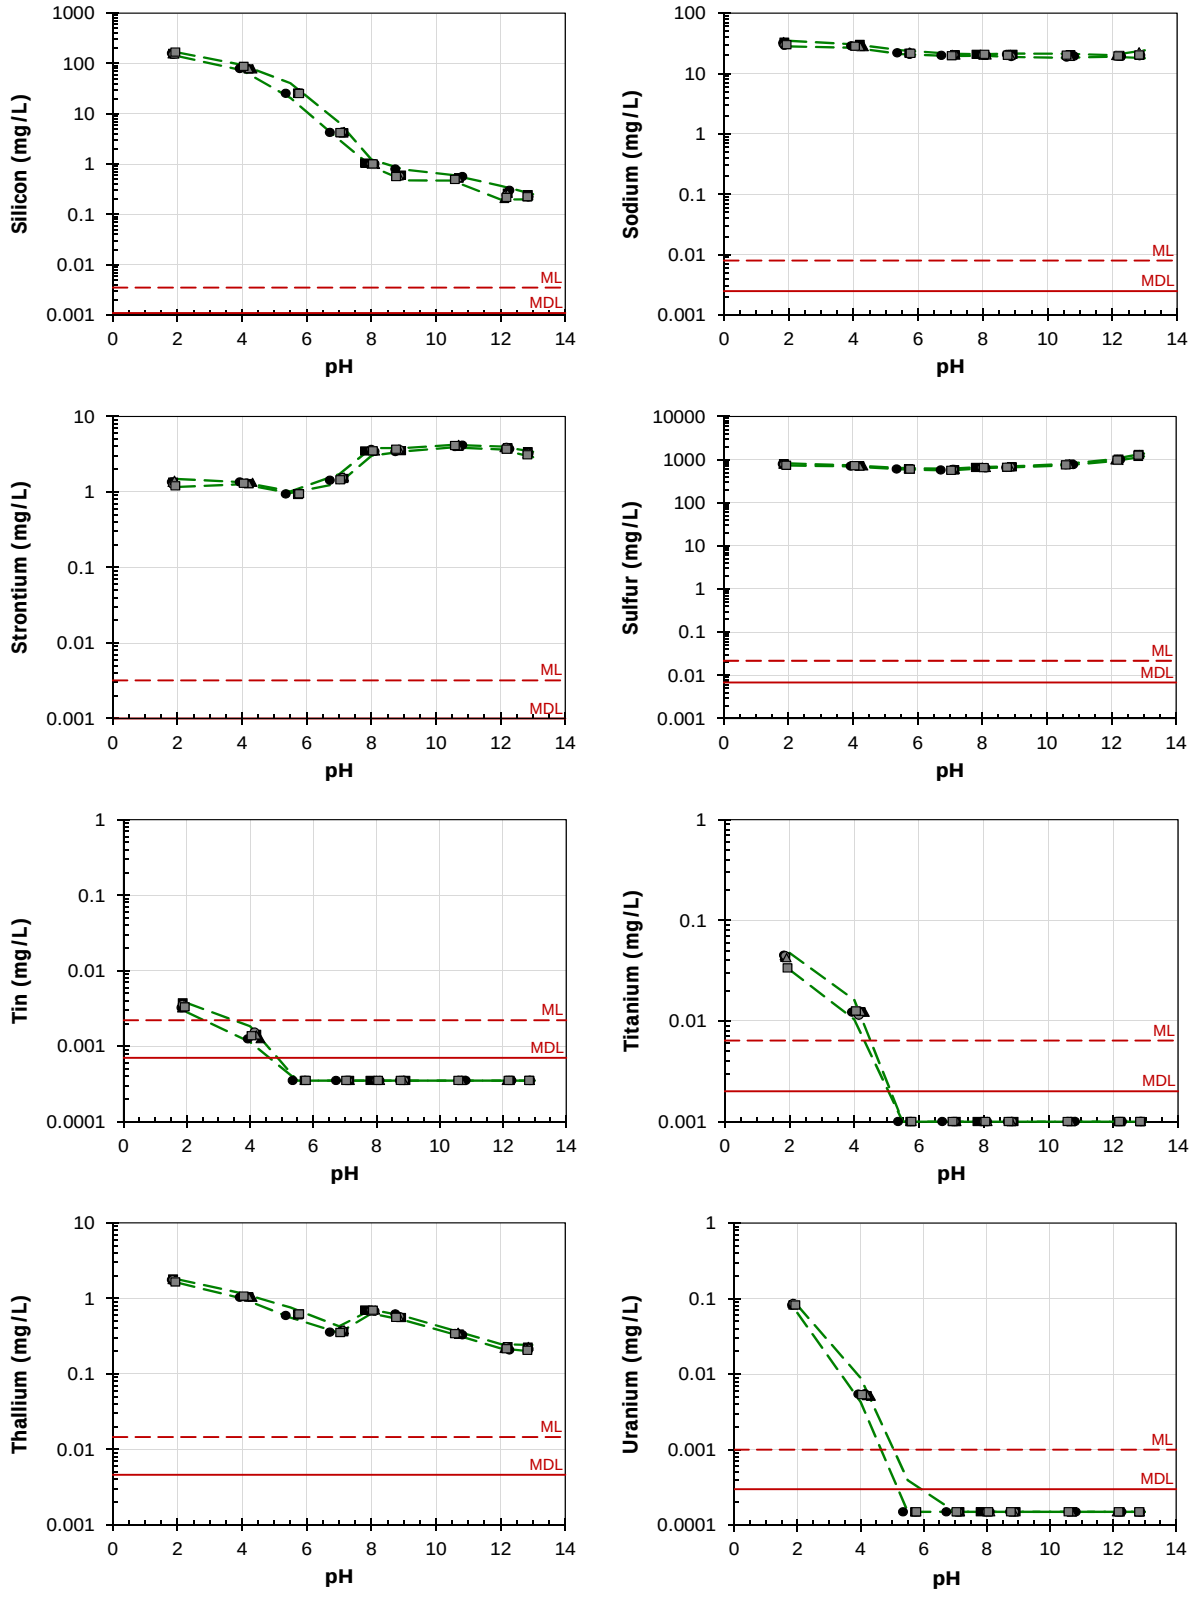

Figure 44. Reference lab data and 95% prediction limits for Method 1313 Phase II CFS material.

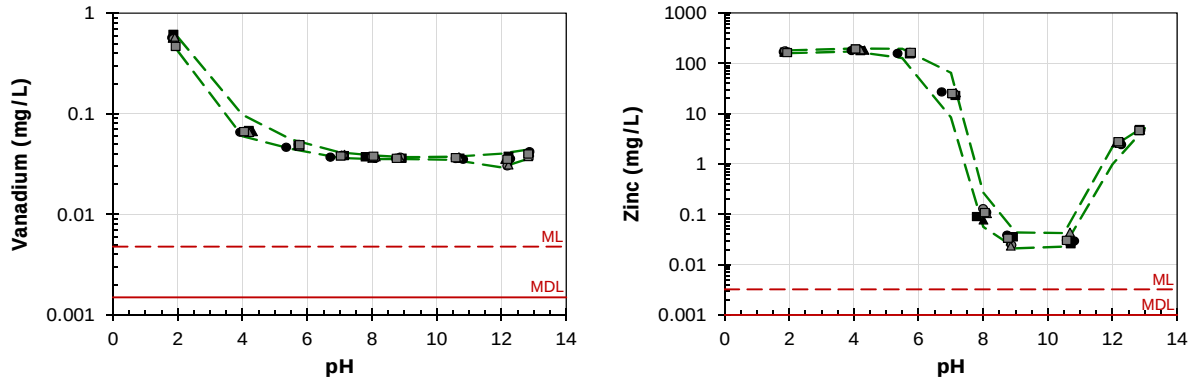

Figure 45. Reference lab data and 95% prediction limits for Method 1313 Phase II CFS material.

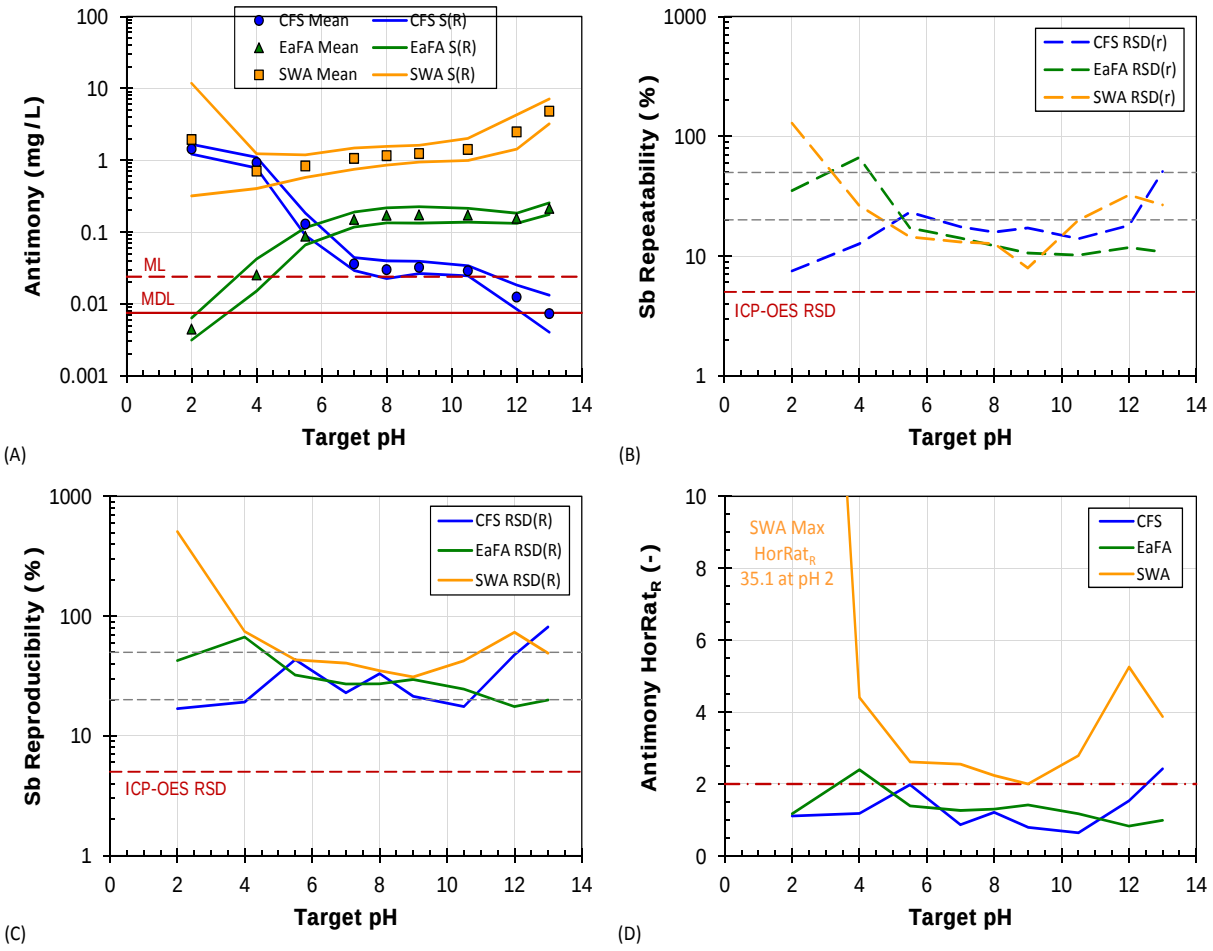

Figure 46. Antimony repeatability and reproducibility in Method 1313 materials: (A) reproducibility standard deviation interval about the mean of all data, (B) repeatability relative standard deviation (RSD_r) compared to approximate analytical uncertainty (ICP-OES RSD), (B) reproducibility relative standard deviation (RSD_R) compared to approximate analytical uncertainty (ICP-OES RSD), and (D) reproducibility Horwitz ratio ($HorRat_R$).

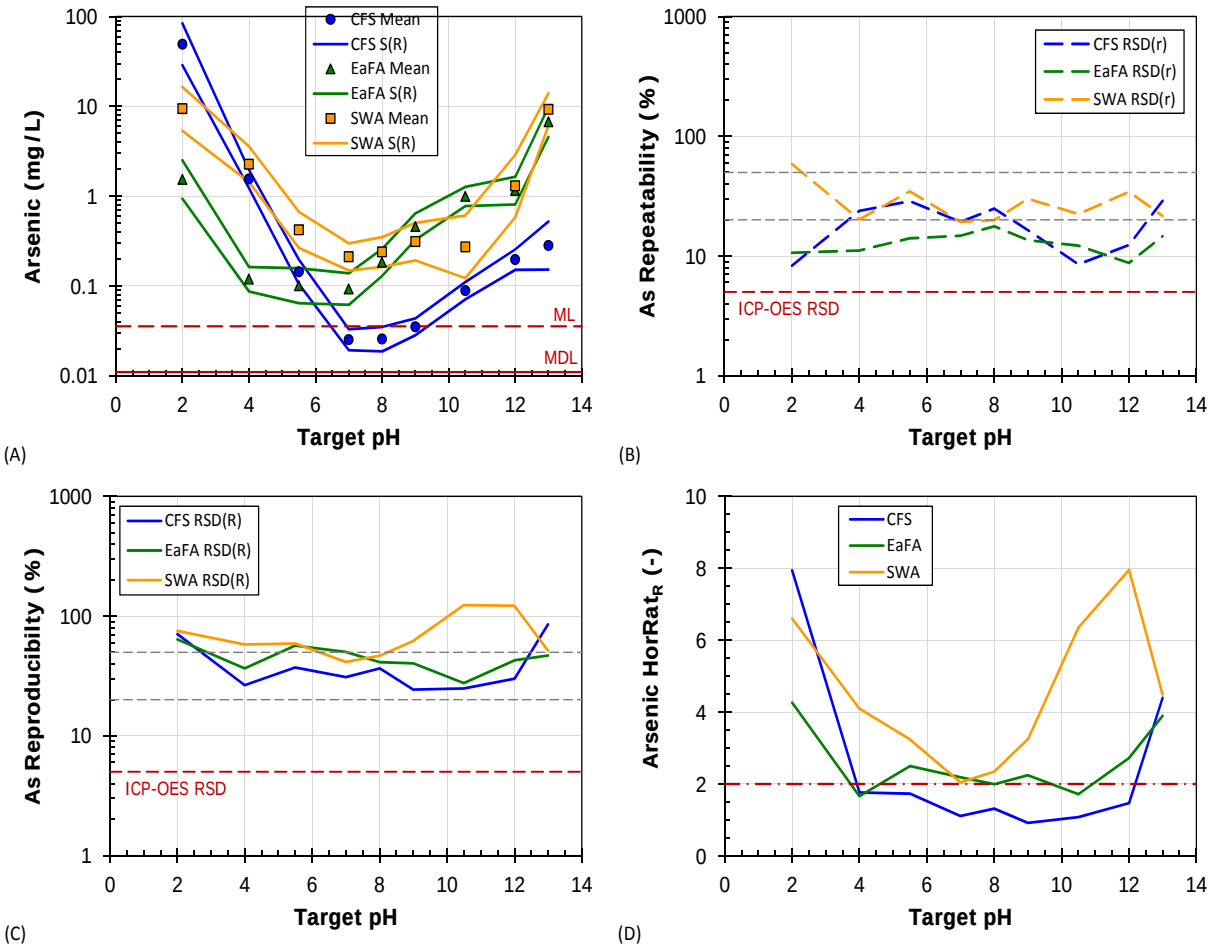

Figure 47. Arsenic repeatability and reproducibility in Method 1313 materials: (A) reproducibility standard deviation interval about the mean of all data, (B) repeatability relative standard deviation (RSD_r) compared to approximate analytical uncertainty (ICP-OES RSD), (B) reproducibility relative standard deviation (RSD_R) compared to approximate analytical uncertainty (ICP-OES RSD), and (D) reproducibility Horwitz ratio ($HorRat_R$).

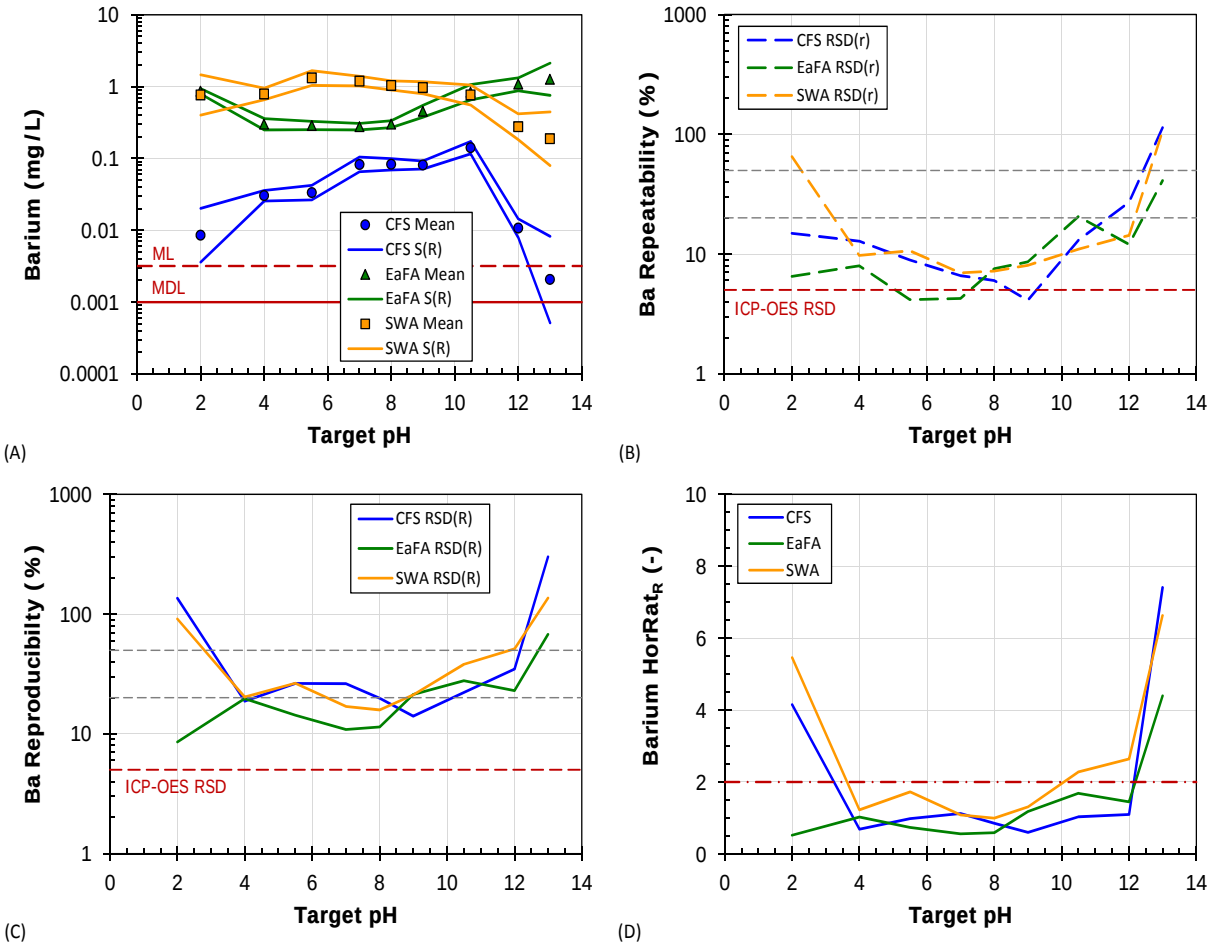

Figure 48. Barium repeatability and reproducibility in Method 1313 materials: (A) reproducibility standard deviation interval about the mean of all data, (B) repeatability relative standard deviation (RSD_r) compared to approximate analytical uncertainty (ICP-OES RSD), (B) reproducibility relative standard deviation (RSD_R) compared to approximate analytical uncertainty (ICP-OES RSD), and (D) reproducibility Horwitz ratio ($HorRat_R$).

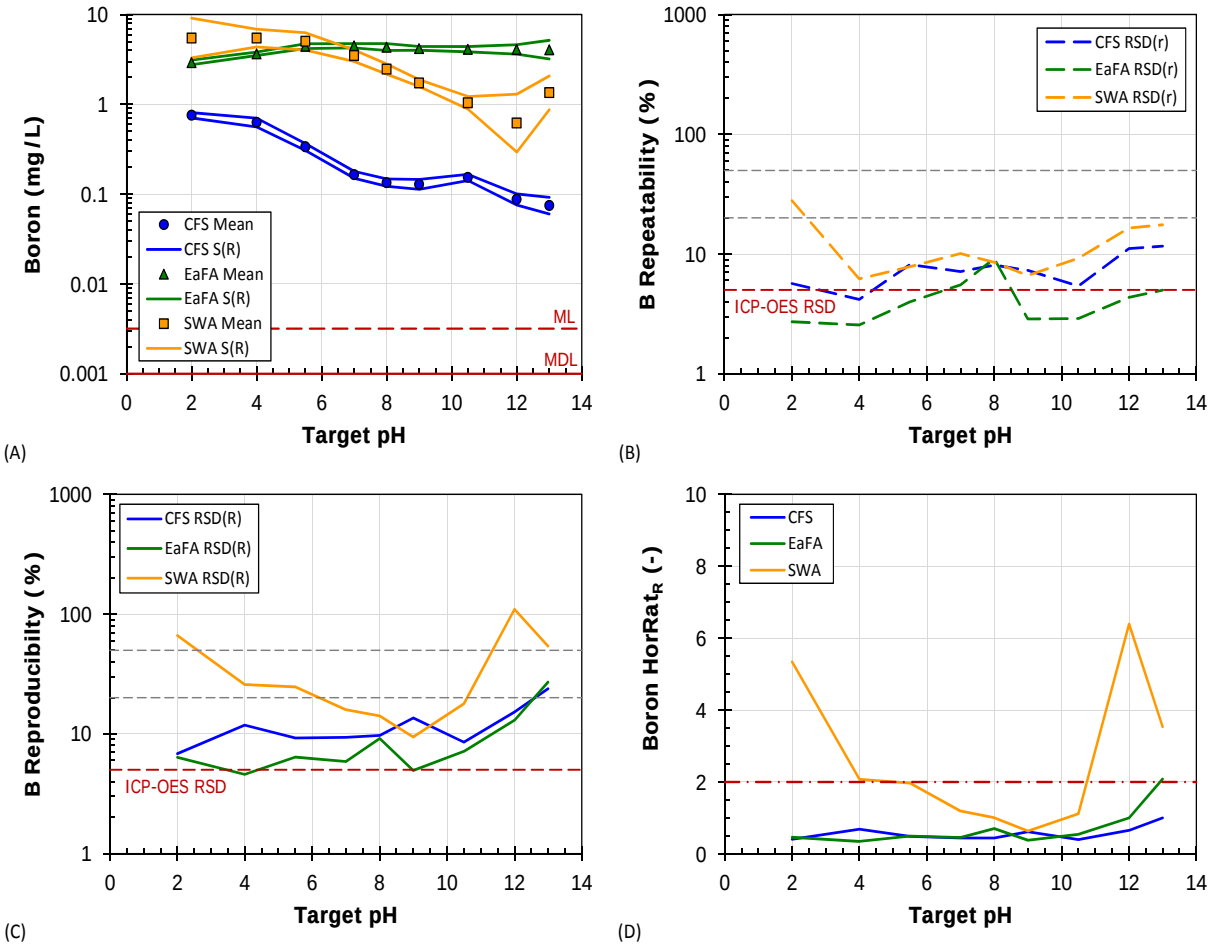

Figure 49. Boron repeatability and reproducibility in Method 1313 materials: (A) reproducibility standard deviation interval about the mean of all data, (B) repeatability relative standard deviation (RSD_r) compared to approximate analytical uncertainty (ICP-OES RSD), (B) reproducibility relative standard deviation (RSD_R) compared to approximate analytical uncertainty (ICP-OES RSD), and (D) reproducibility Horwitz ratio ($HorRat_R$).

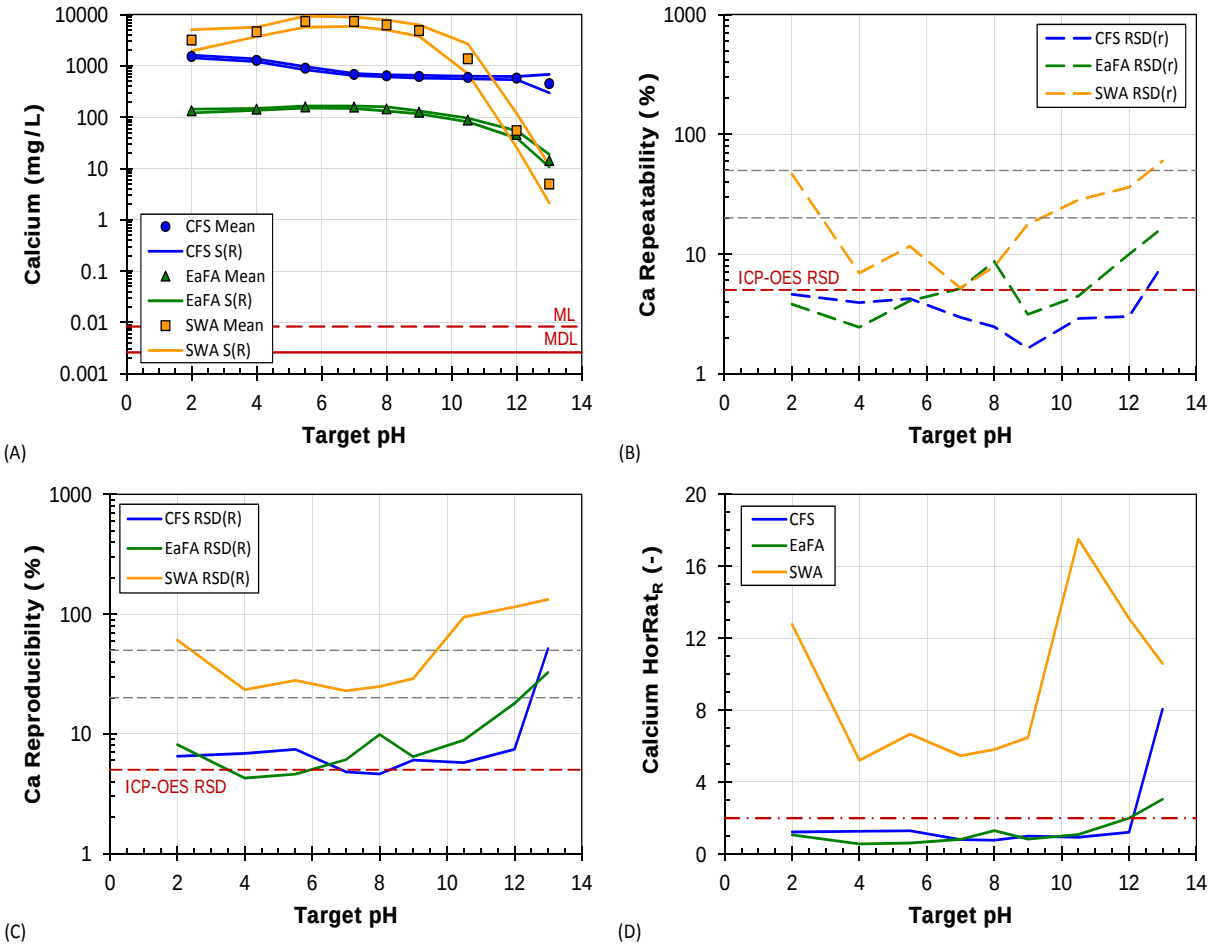

Figure 50. Calcium repeatability and reproducibility in Method 1313 materials: (A) reproducibility standard deviation interval about the mean of all data, (B) repeatability relative standard deviation (RSD_r) compared to approximate analytical uncertainty (ICP-OES RSD), (B) reproducibility relative standard deviation (RSD_R) compared to approximate analytical uncertainty (ICP-OES RSD), and (D) reproducibility Horwitz ratio ($HorRat_R$).

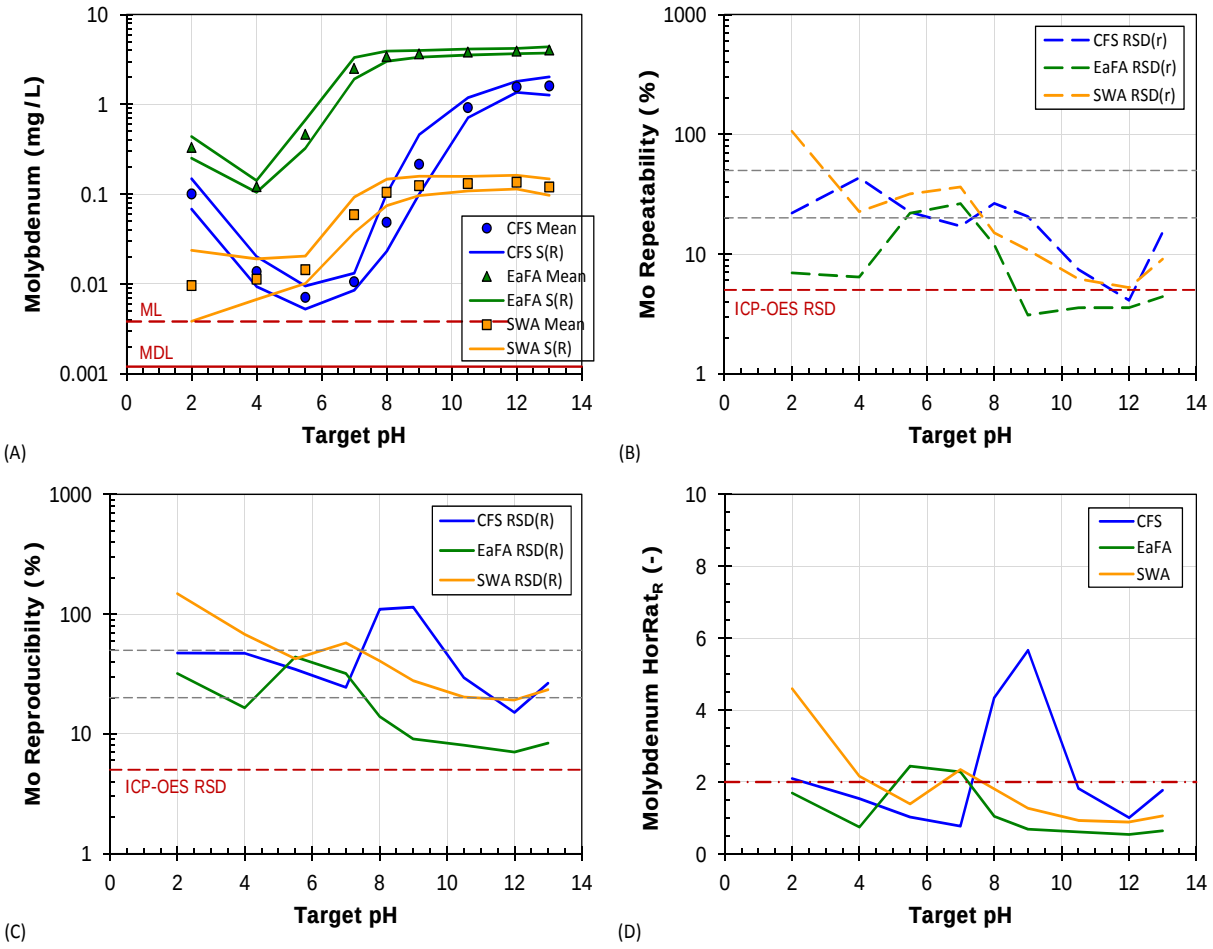

Figure 51. Molybdenum repeatability and reproducibility in Method 1313 materials: (A) reproducibility standard deviation interval about the mean of all data, (B) repeatability relative standard deviation (RSD_r) compared to approximate analytical uncertainty (ICP-OES RSD), (B) reproducibility relative standard deviation (RSD_R) compared to approximate analytical uncertainty (ICP-OES RSD), and (D) reproducibility Horwitz ratio ($HorRat_R$).

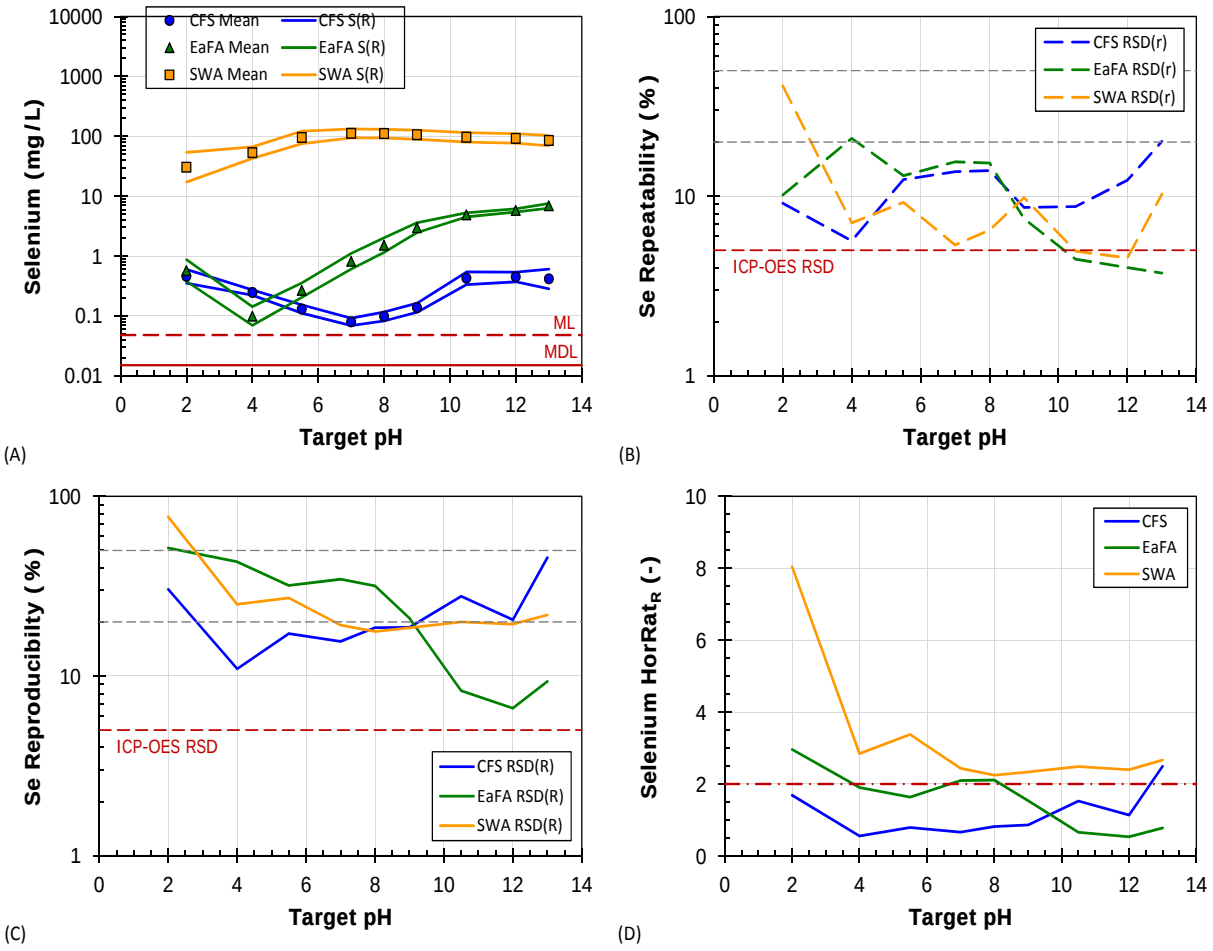

Figure 52. Selenium repeatability and reproducibility in Method 1313 materials: (A) reproducibility standard deviation interval about the mean of all data, (B) repeatability relative standard deviation (RSD_r) compared to approximate analytical uncertainty (ICP-OES RSD), (B) reproducibility relative standard deviation (RSD_R) compared to approximate analytical uncertainty (ICP-OES RSD), and (D) reproducibility Horwitz ratio ($HorRat_R$).

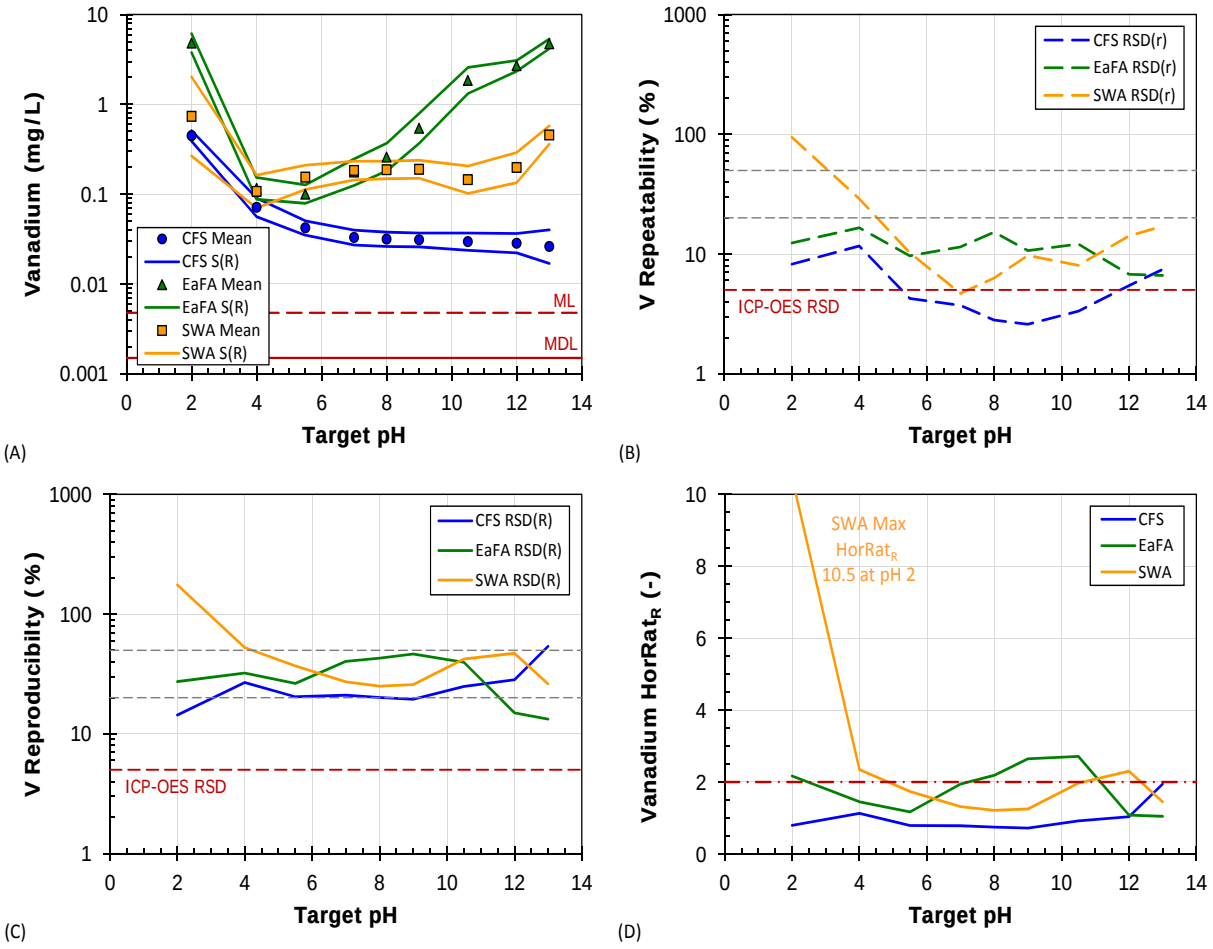

Figure 53. Vanadium repeatability and reproducibility in Method 1313 materials: (A) reproducibility standard deviation interval about the mean of all data, (B) repeatability relative standard deviation (RSD_r) compared to approximate analytical uncertainty (ICP-OES RSD), (B) reproducibility relative standard deviation (RSD_R) compared to approximate analytical uncertainty (ICP-OES RSD), and (D) reproducibility Horwitz ratio ($HorRat_R$).

Table 1. Method 1313 Repeatability (RSD_r) for Common Analytes in All Study Materials

		RSD_r Distribution Percentiles (%)					
Analyte	Symbol	Mean	Min	25th	Median	75th	Max
Antimony	Sb	23	8	12	16	25	129
Arsenic	As	20	8	13	19	24	59
Barium	Ba	21	4	7	10	15	108
Boron	B	8	3	5	7	9	28
Calcium	Ca	12	2	3	5	11	60
Molybdenum	Mo	19	3	6	15	22	106
Selenium	Se	11	4	6	9	13	41
Vanadium	V	13	3	6	10	12	94

Table 2. Method 1313 Reproducibility (RSD_R) for Common Analytes in All Study Materials

		RSD_R Distribution Percentiles (%)					
Analyte	Symbol	Mean	Min	25th	Median	75th	Max
Antimony	Sb	55	17	24	33	45	508
Arsenic	As	52	24	37	47	61	124
Barium	Ba	44	9	18	22	36	280
Boron	B	20	5	8	12	21	110
Calcium	Ca	27	4	6	9	28	133
Molybdenum	Mo	39	7	18	30	45	148
Selenium	Se	26	7	18	21	31	77
Vanadium	V	36	13	23	27	41	175

Table 3. Method 1313 Repeatability (RSD_r) by pH Target

	RSD_r Distribution Percentiles (%)					
pH	Mean	Min	25th	Median	75th	Max
2.0	30	3	7	11	42	129
4.0	16	2	6	11	21	67
5.5	14	4	8	11	18	35
7.0	12	3	5	11	16	36
8.0	12	2	7	11	15	27
9.0	10	2	6	9	12	30
10.5	10	3	5	9	12	28
12.0	13	3	5	11	15	36
13.0	26	4	9	16	27	108

Table 4. Method 1313 Reproducibility (RSD_R) by pH Target

	RSD_R Distribution Percentiles (%)					
pH	Mean	Min	25th	Median	75th	Max
2.0	74	6	16	49	76	508
4.0	31	4	18	25	44	74
5.5	29	5	20	28	38	59
7.0	25	5	16	24	33	58
8.0	27	5	14	23	35	110
9.0	26	5	14	21	29	114
10.5	30	6	15	25	32	124
12.0	37	7	15	22	47	122
13.0	57	8	24	46	58	280

Table 5. Method 1313 Repeatability (RSD_r) by Study Material

	RSD_r Distribution Percentiles (%)					
Material	Mean	Min	25th	Median	75th	Max
EaFA	11	2	4	10	14	67
SWA	23	5	8	14	28	129
CFS	14	2	6	9	17	108

Table 6. Method 1313 Reproducibility (RSD_R) by Study Material

	RSD_R Distribution Percentiles (%)					
Material	Mean	Min	25th	Median	75th	Max
EaFA	25	4	9	22	35	68
SWA	36	9	23	39	61	508
CFS	32	5	15	23	33	280

Appendix F. Method 1316 Results

TABLE OF CONTENTS

Method 1316 Statistical Analysis for Selected Analytes F-1
EaFA Fly Ash F-1
SWA Solidified Waste Analog F-11
CFS Contaminated Field Soil F-21
Method 1316 Reference Laboratory Eluate Results (ICP-OES and Supplemental Analysis) F-31
EaFA Fly Ash F-31
SWA Solidified Waste Analog F-36
CFS Contaminated Field Soil F-40
Method 1316 Repeatability and Reproducibility F-45
Material Comparison Graphs F-45
Precision Distribution Data F-54

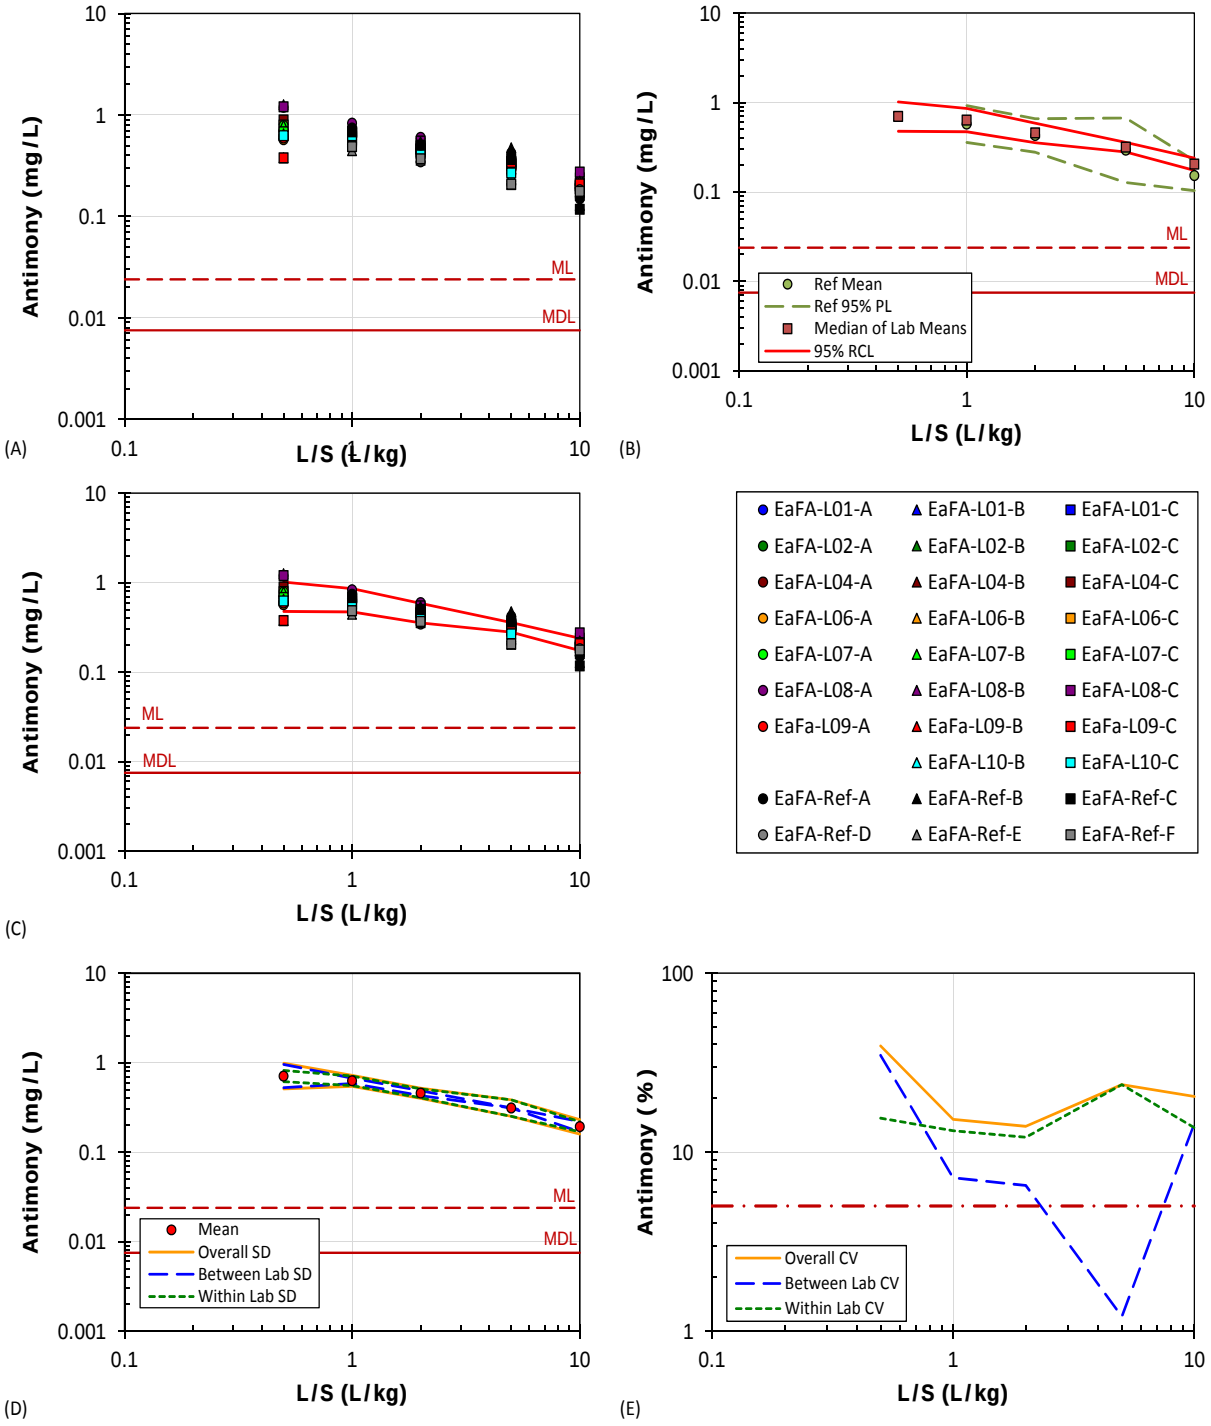

Figure 1. Antimony statistical analysis for Method 1316 Phase I material EaFA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

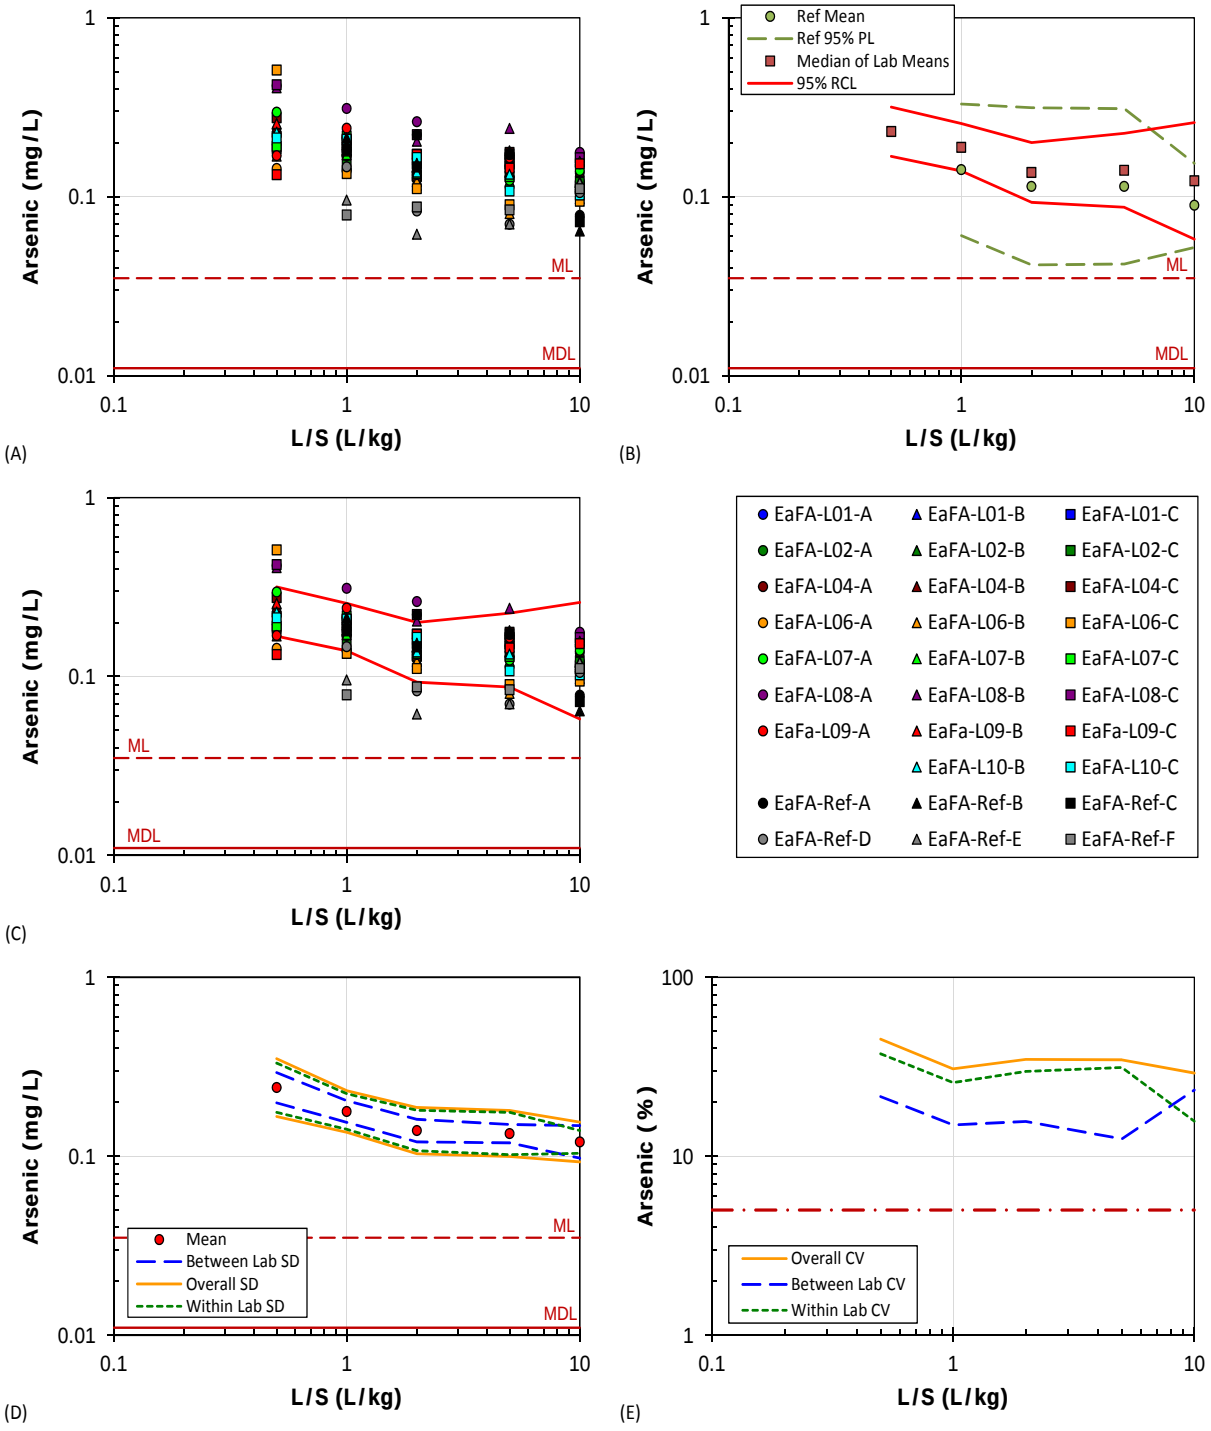

Figure 2. Arsenic statistical analysis for Method 1316 Phase I material EaFA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

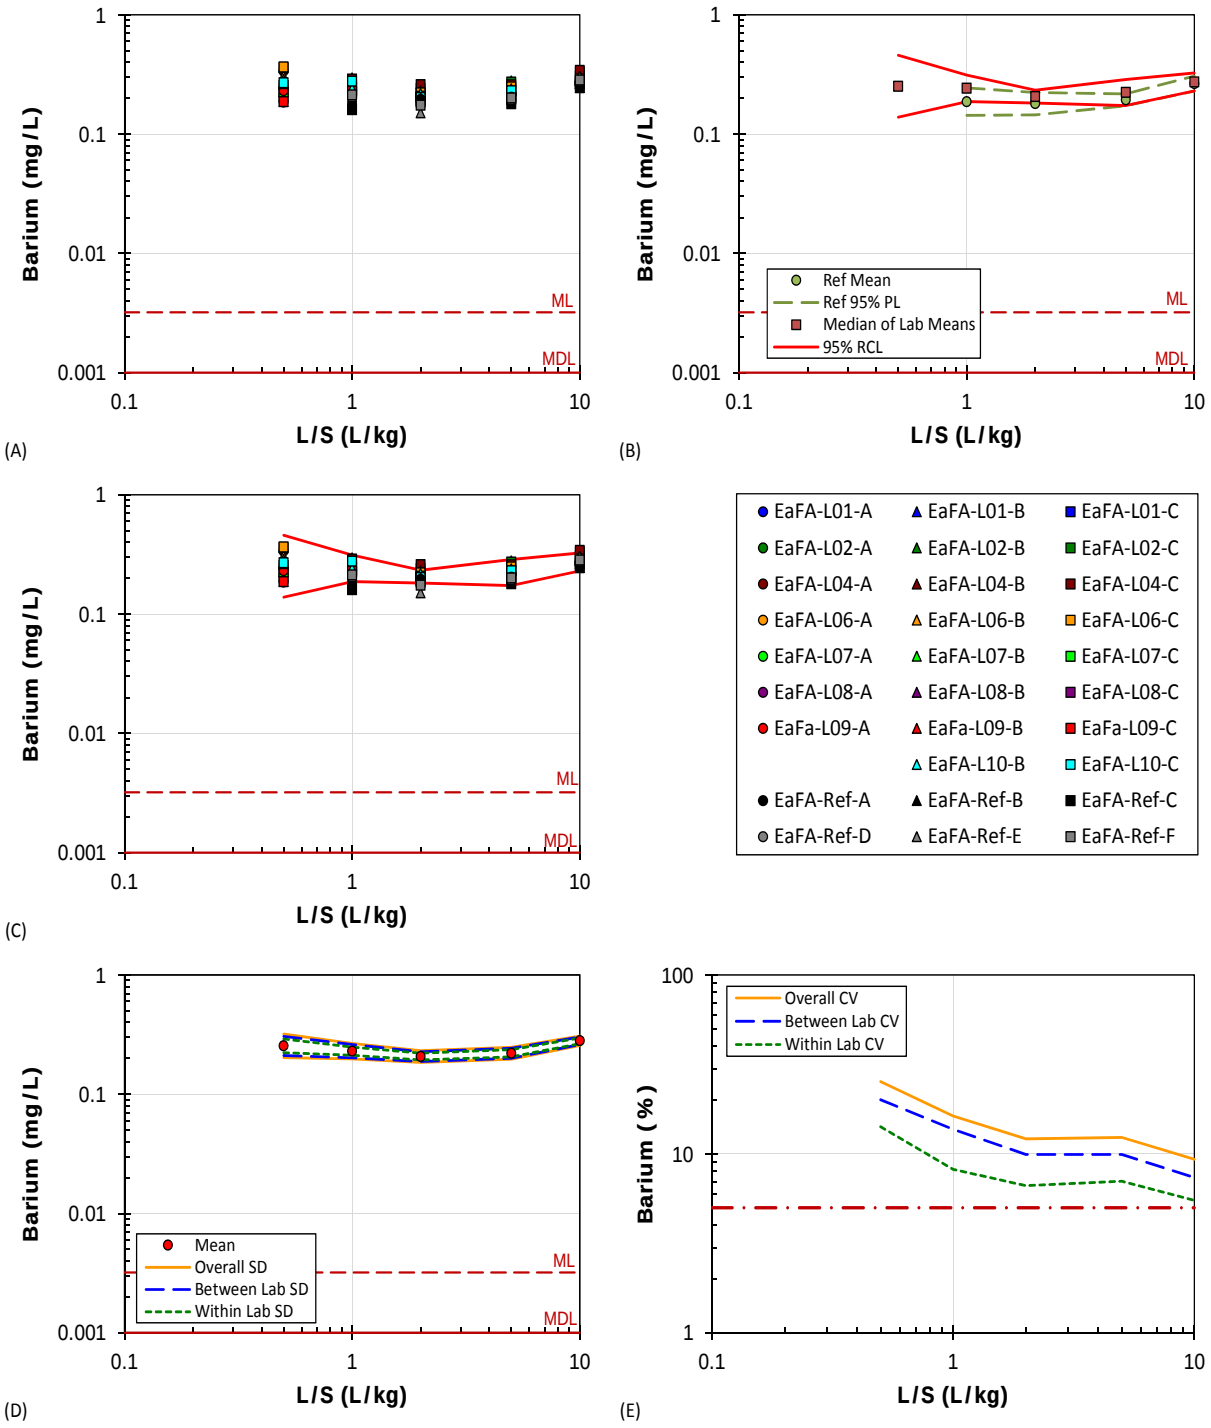

Figure 3. Barium statistical analysis for Method 1316 Phase I material EaFA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

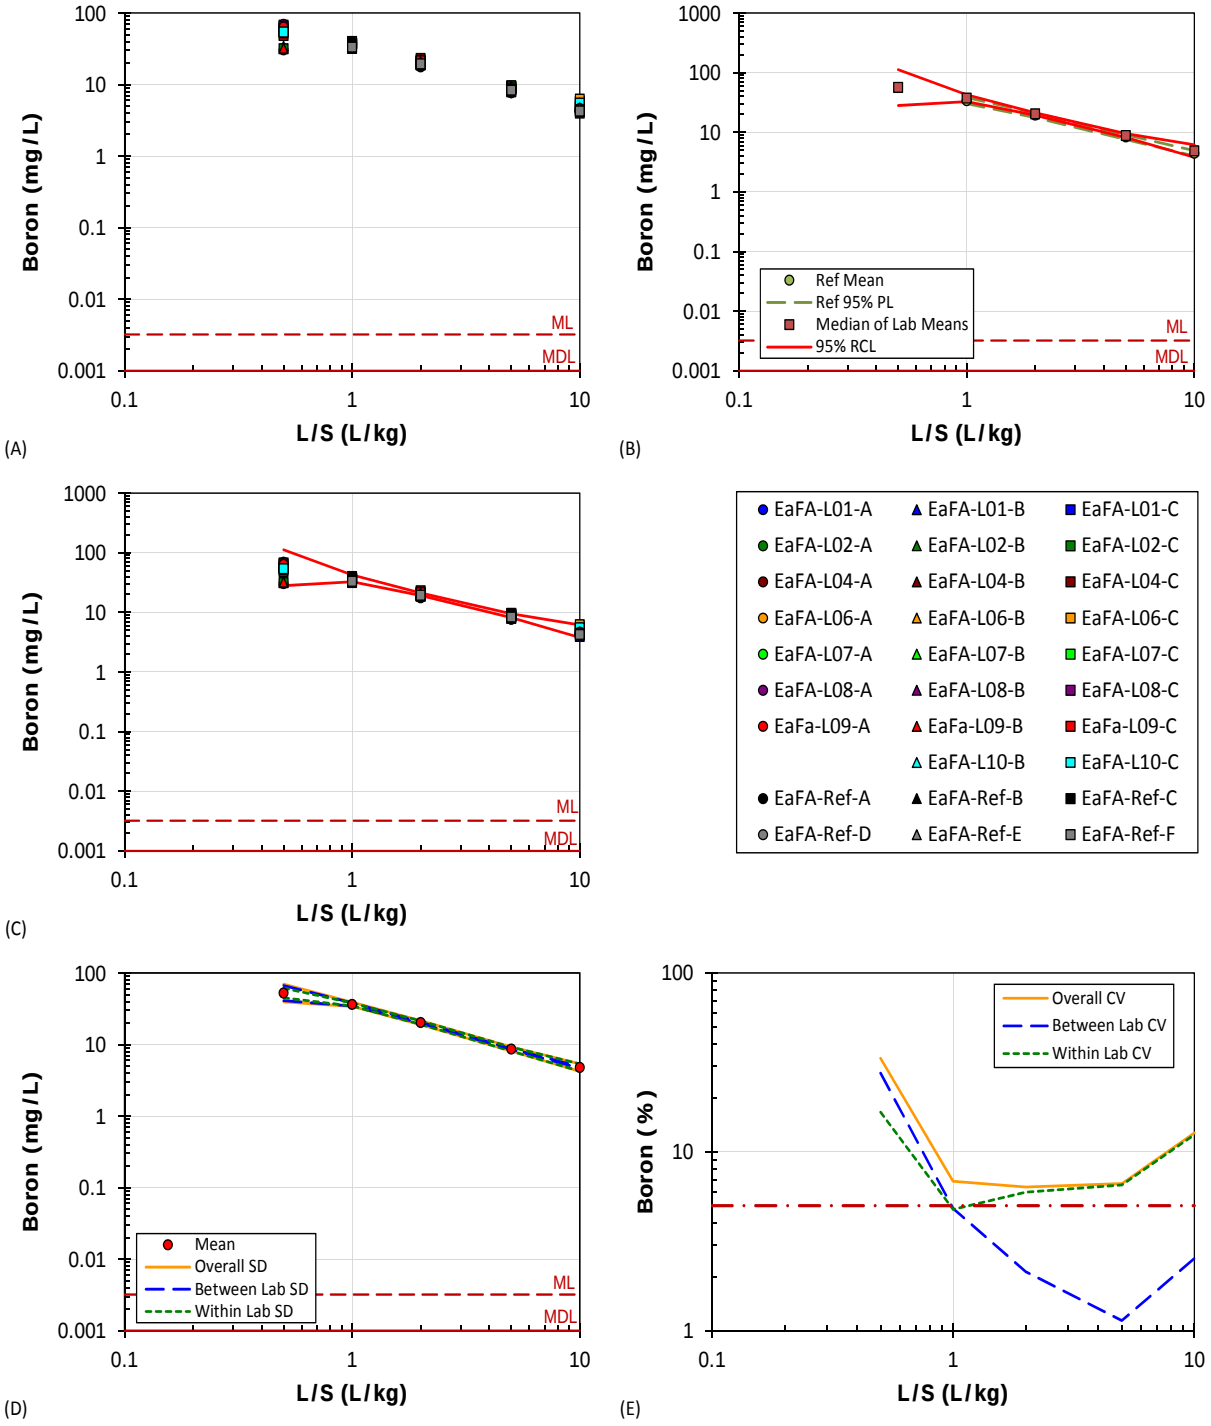

Figure 4. Boron statistical analysis for Method 1316 Phase I material EaFA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

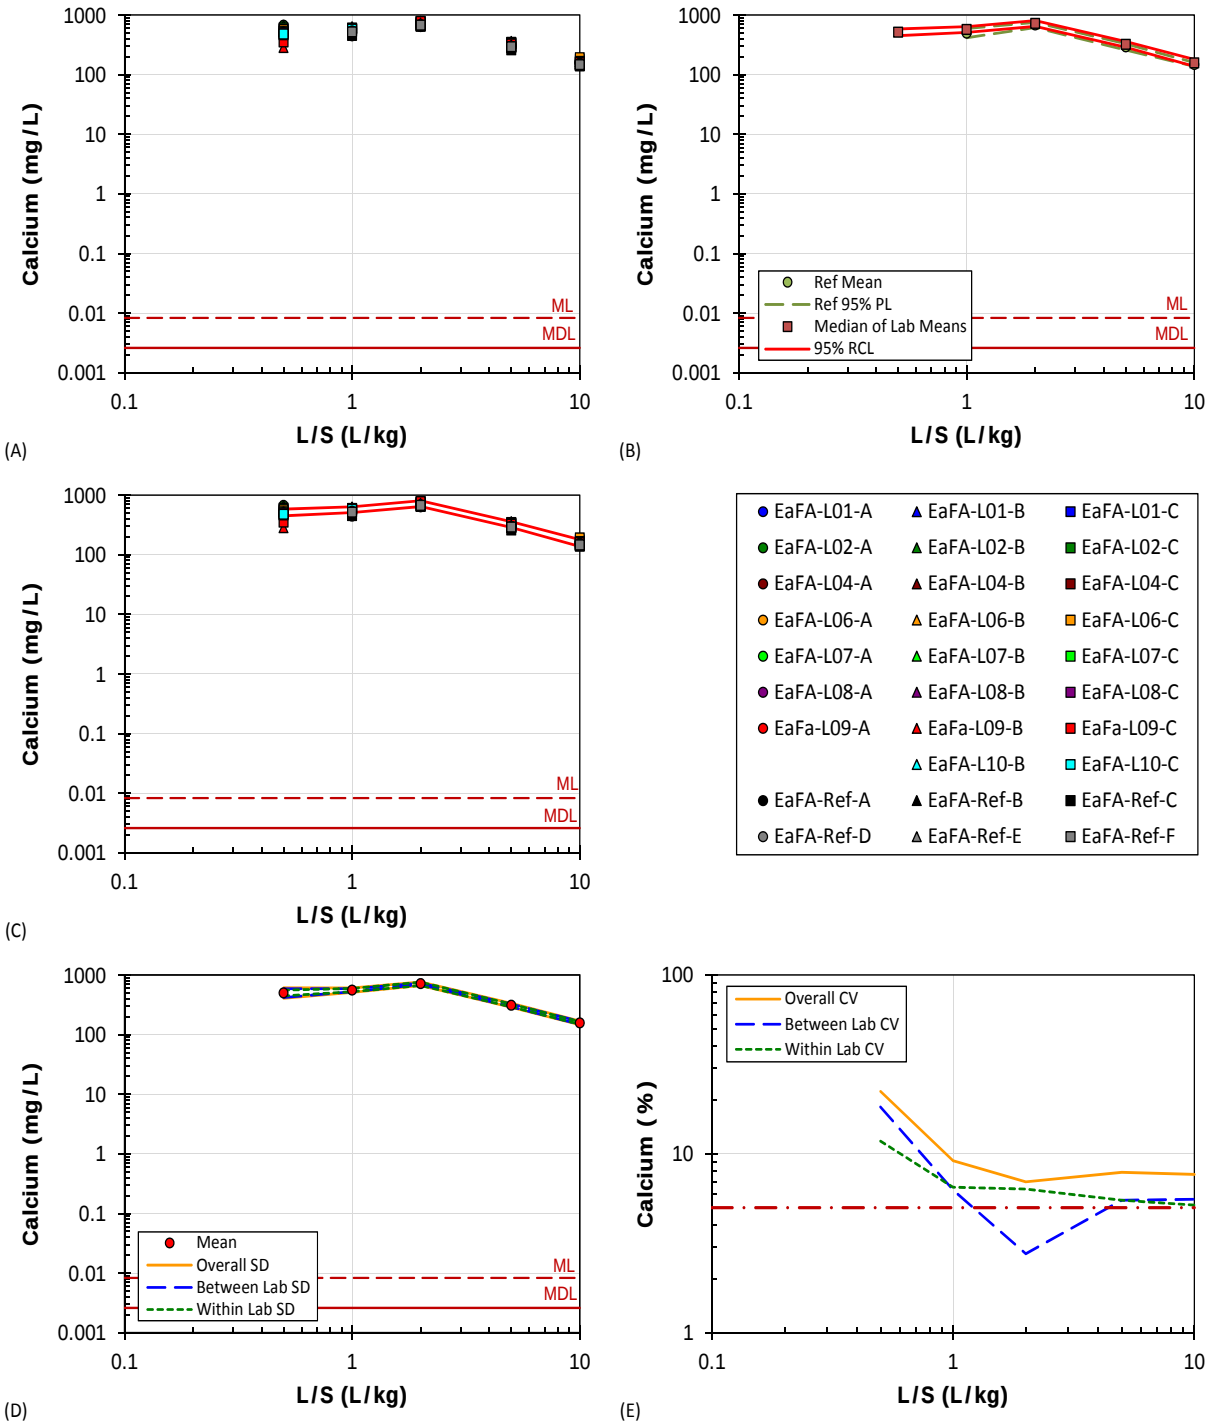

Figure 5. Calcium statistical analysis for Method 1316 Phase I material EaFA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

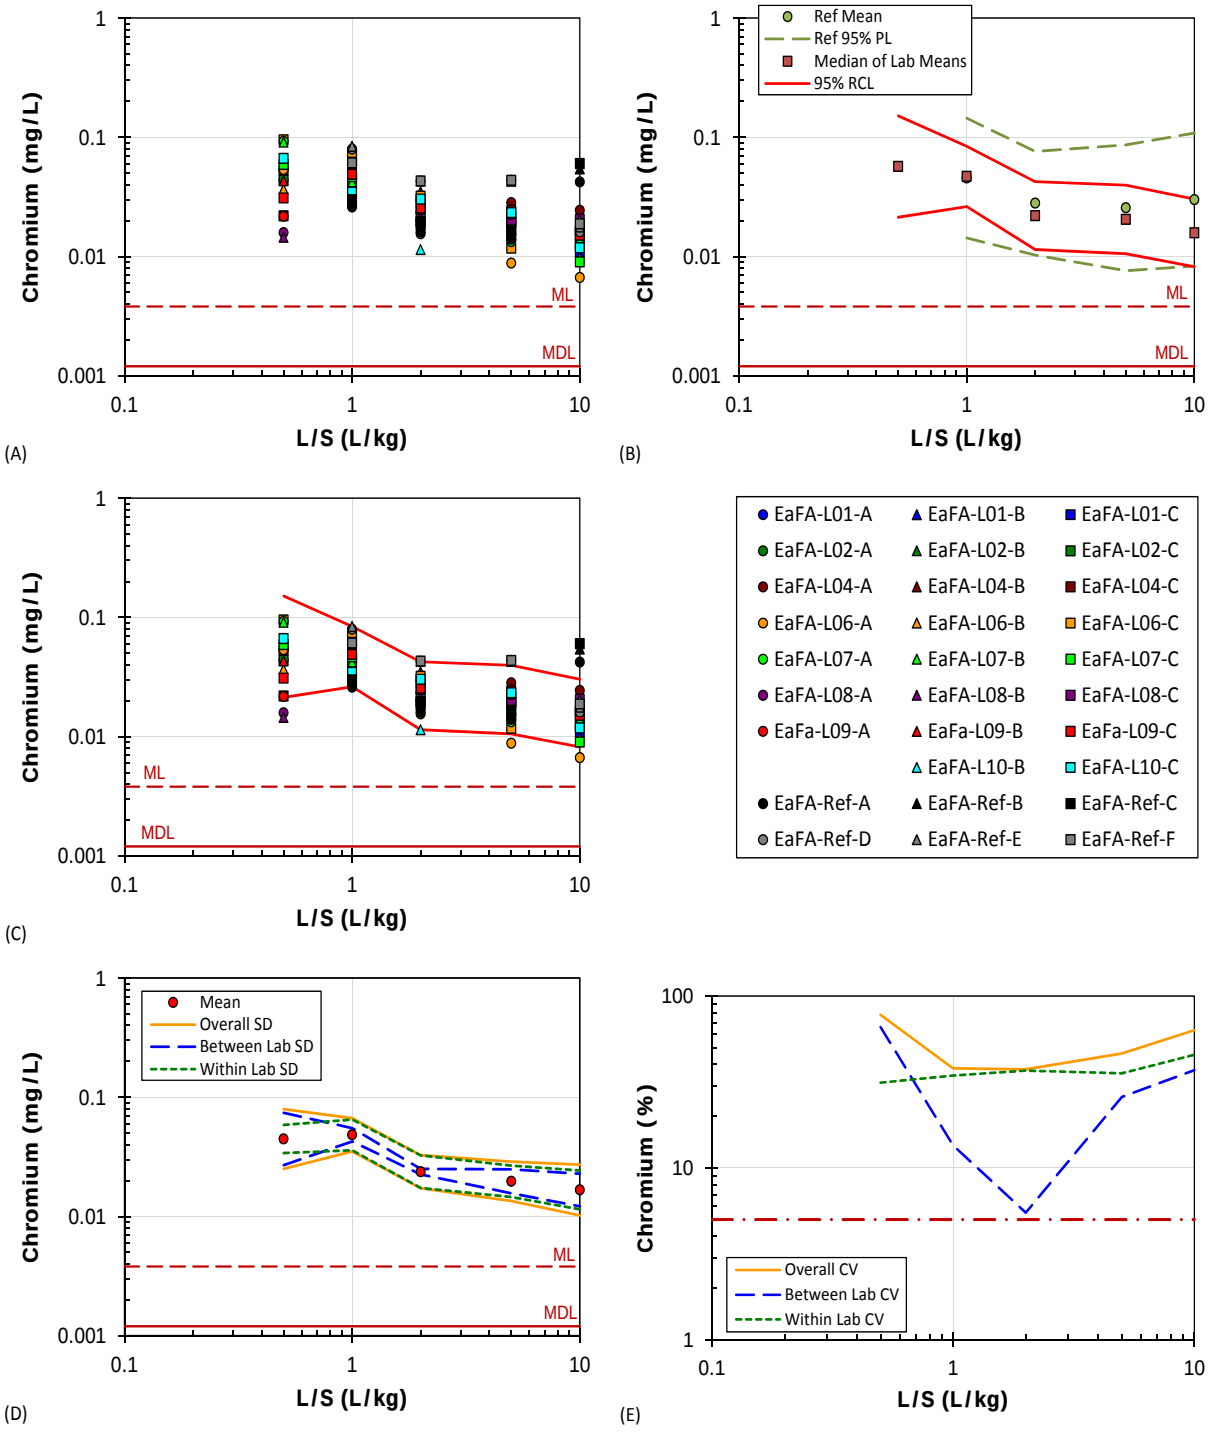

Figure 6. Chromium statistical analysis for Method 1316 Phase I material EaFA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

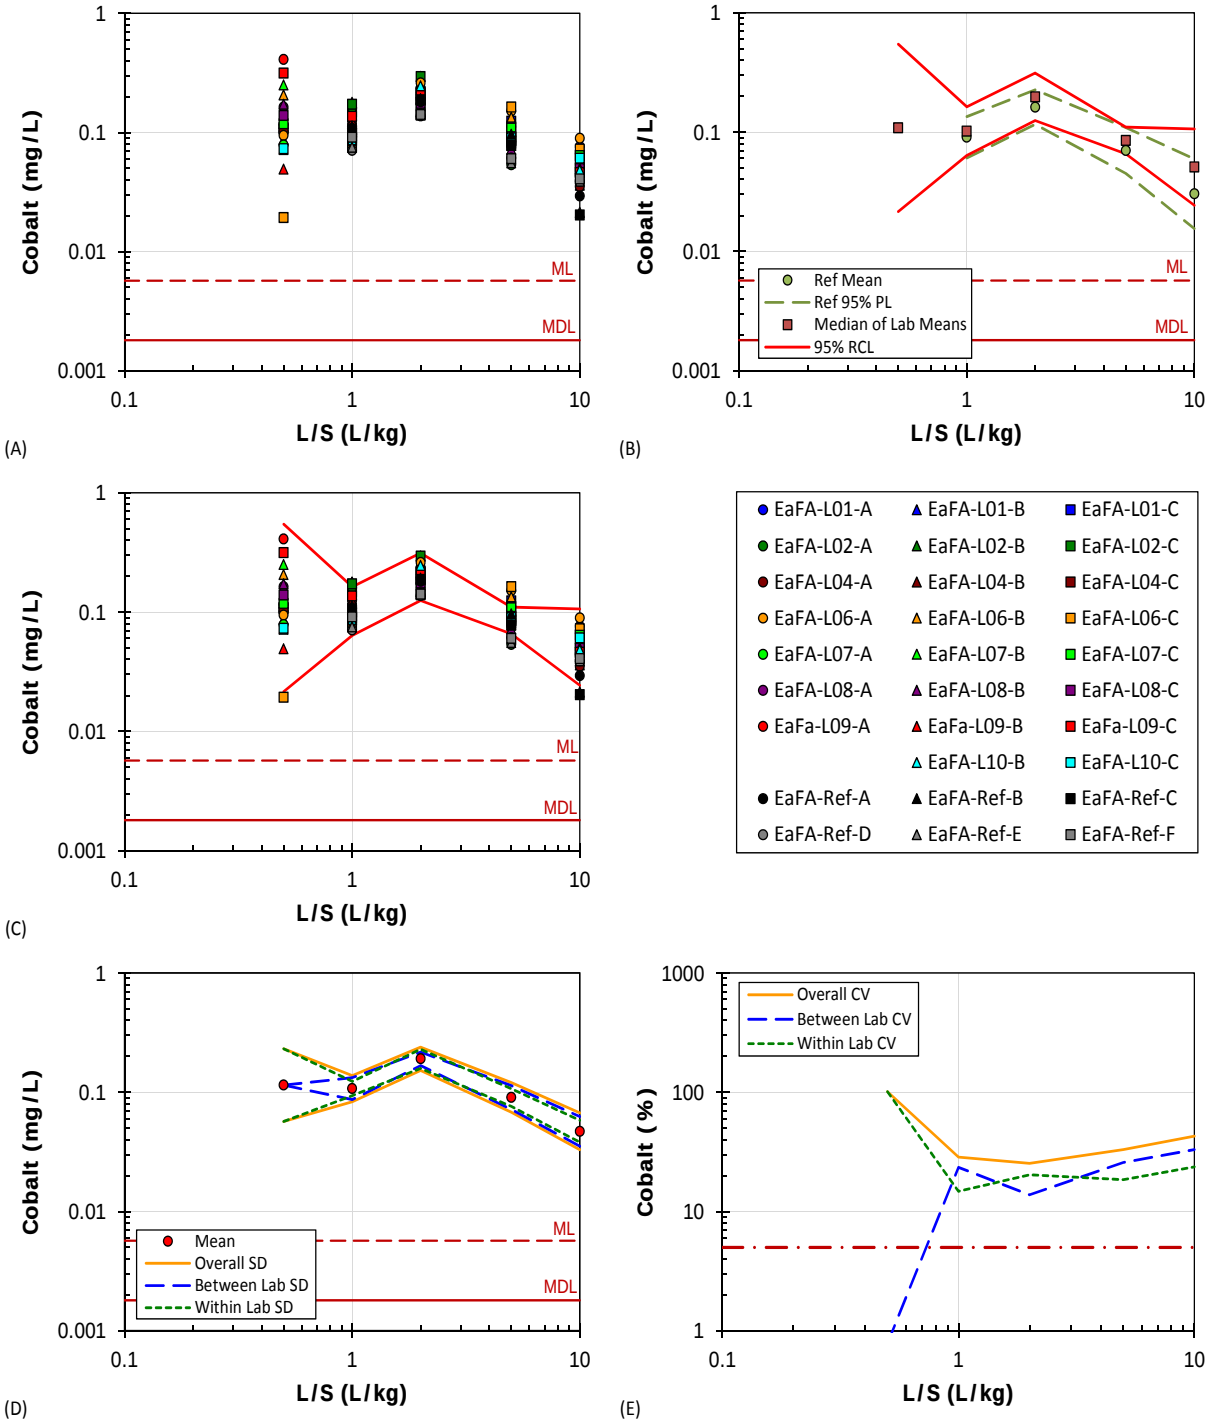

Figure 7. Cobalt statistical analysis for Method 1316 Phase I material EaFA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

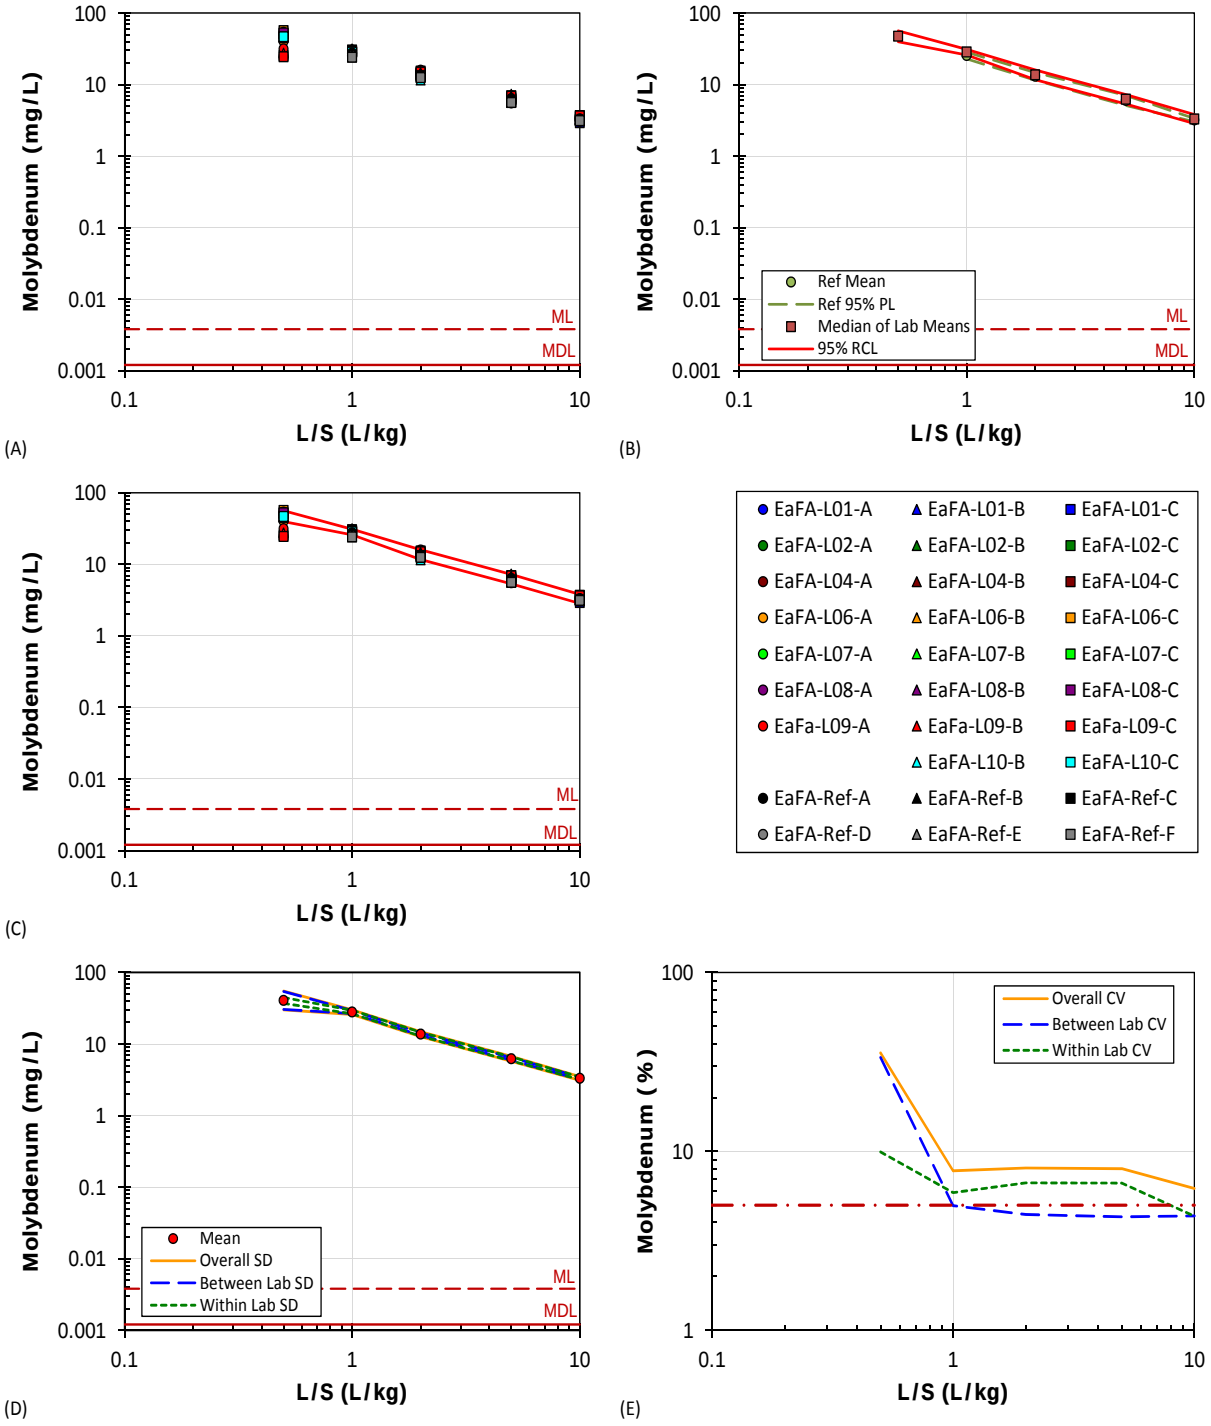

Figure 8. Molybdenum statistical analysis for Method 1316 Phase I material EaFA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

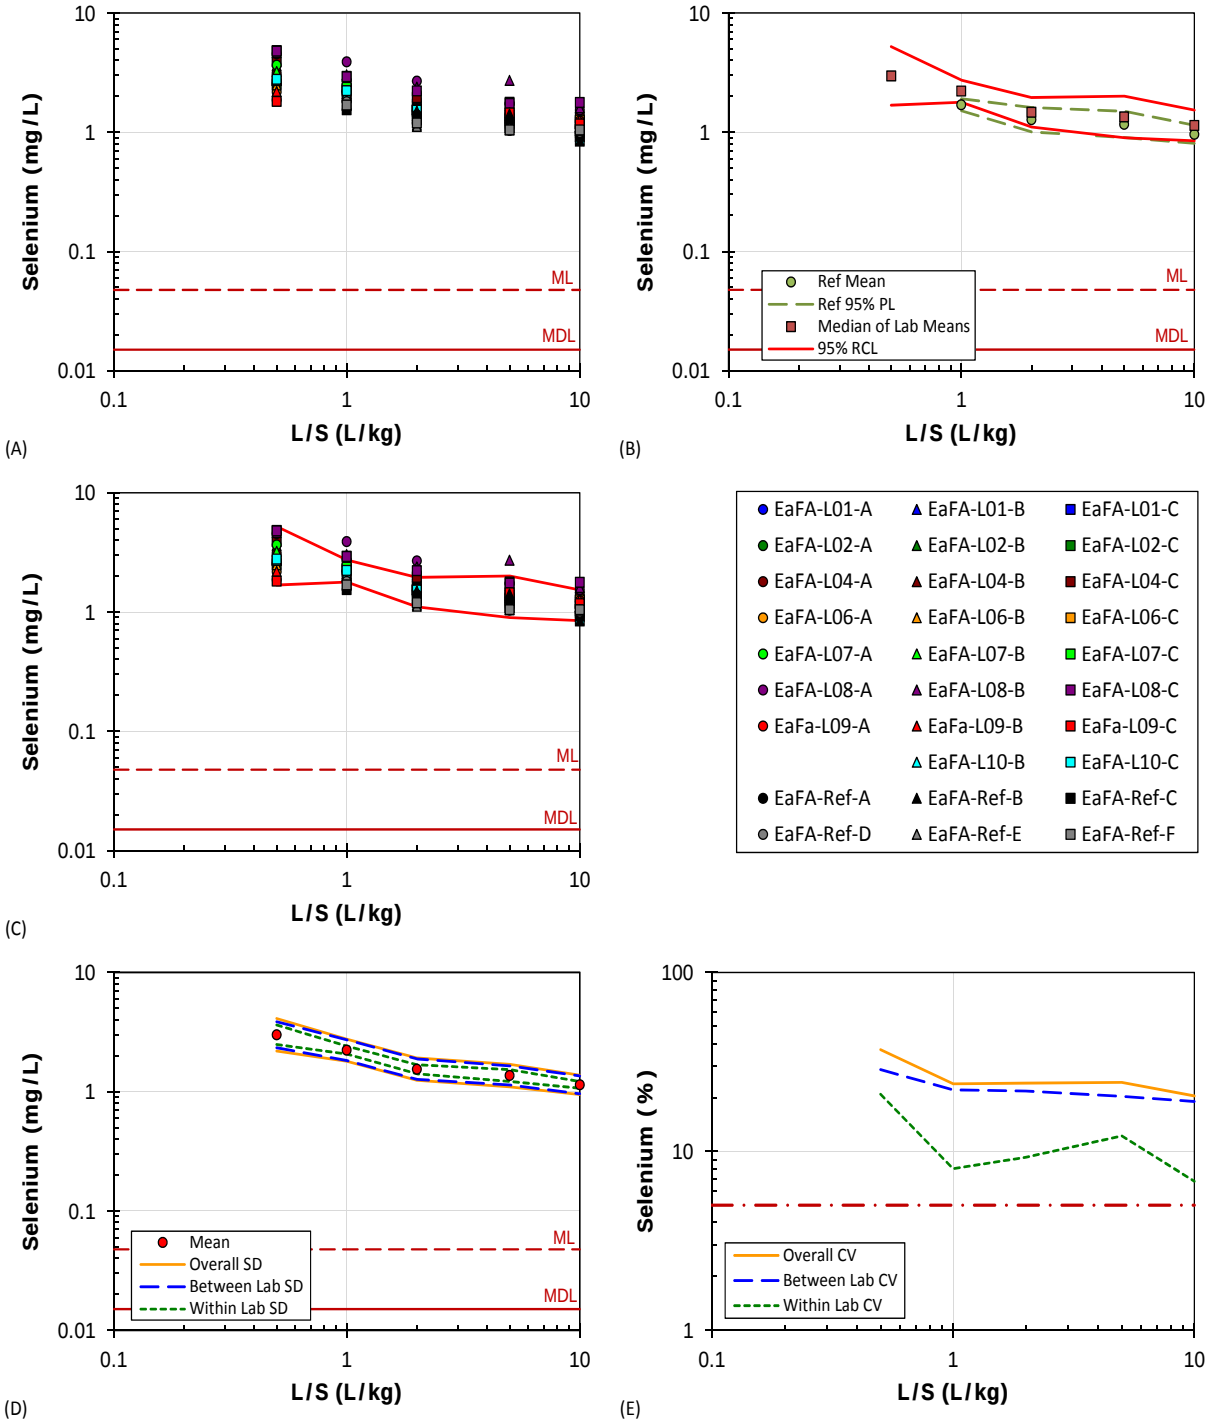

Figure 9. Selenium statistical analysis for Method 1316 Phase I material EaFA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

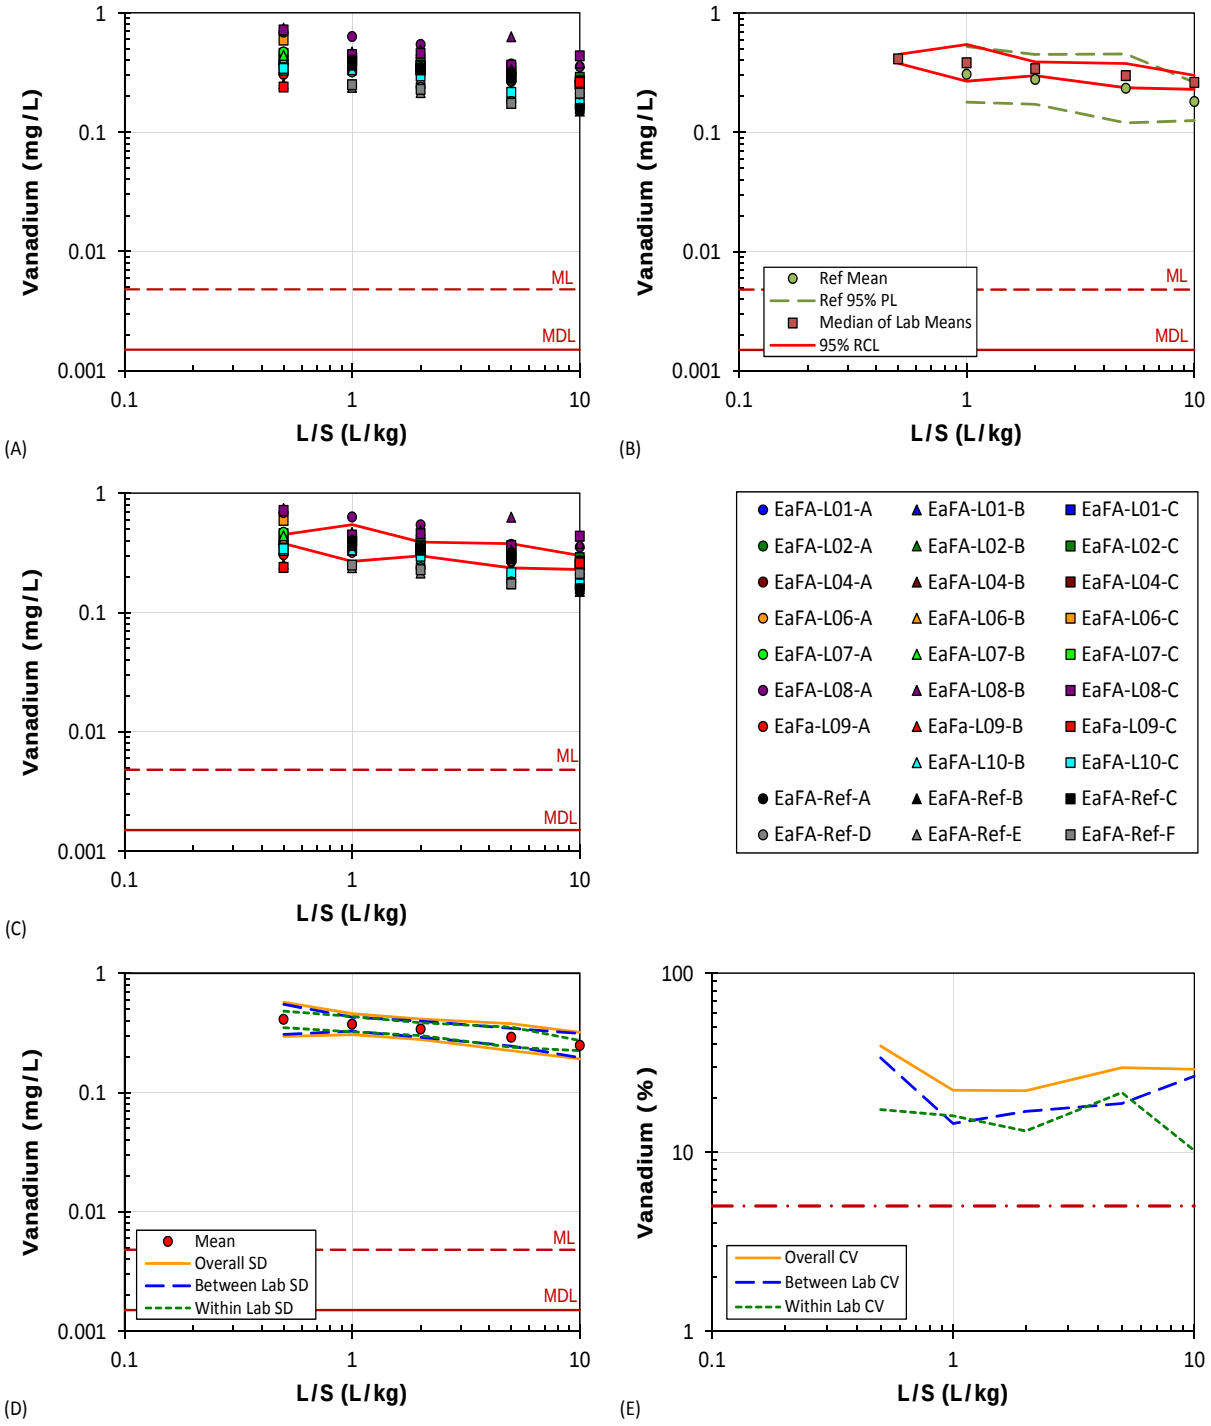

Figure 10. Vanadium statistical analysis for Method 1316 Phase I material EaFA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

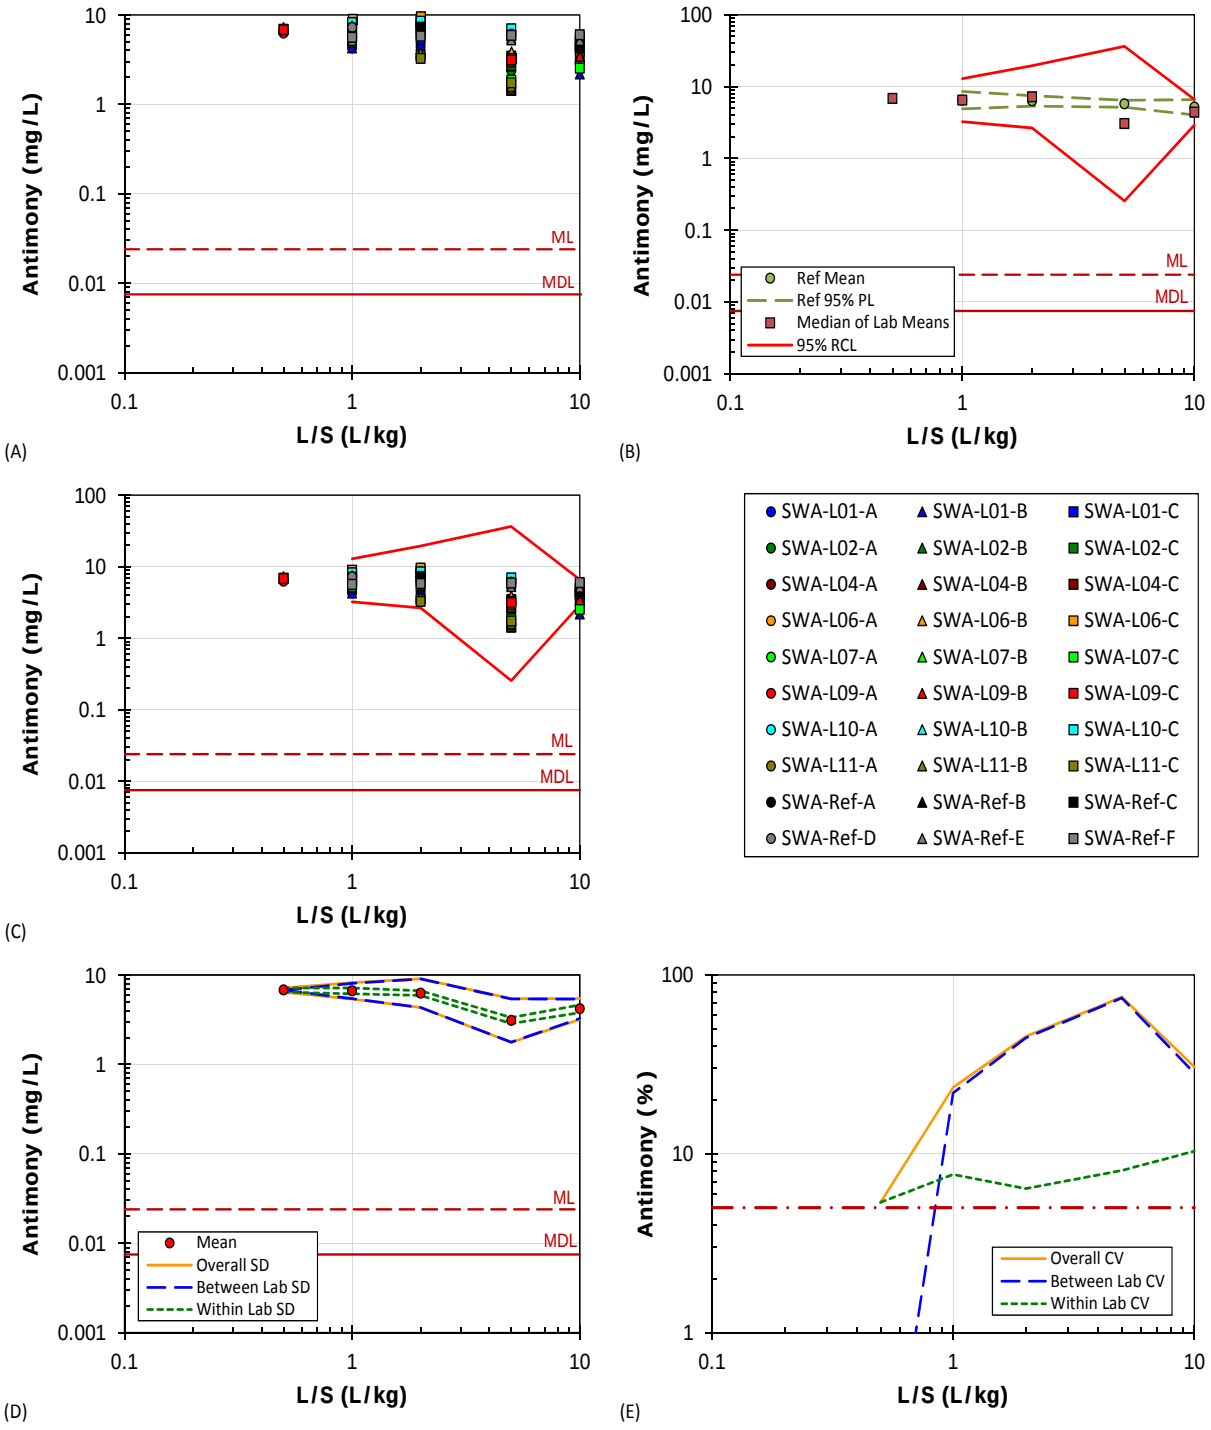

Figure 11. Antimony statistical analysis for Method 1316 Phase II material SWA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

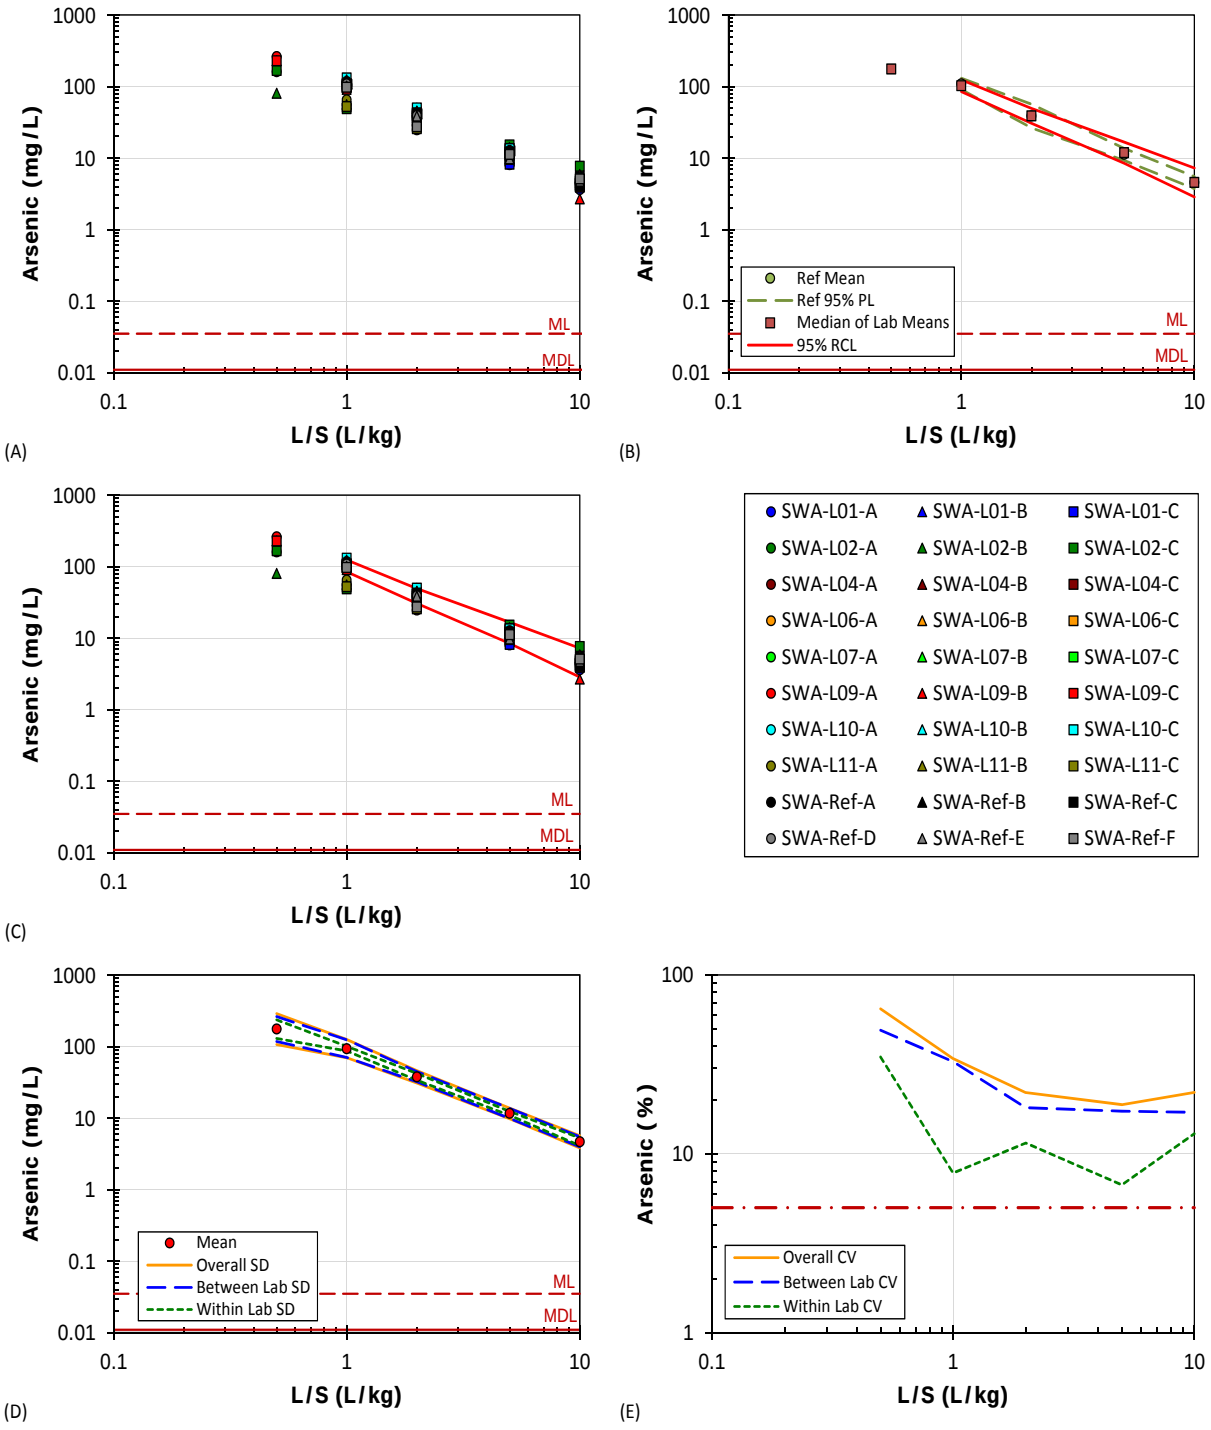

Figure 12. Arsenic statistical analysis for Method 1316 Phase II material SWA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

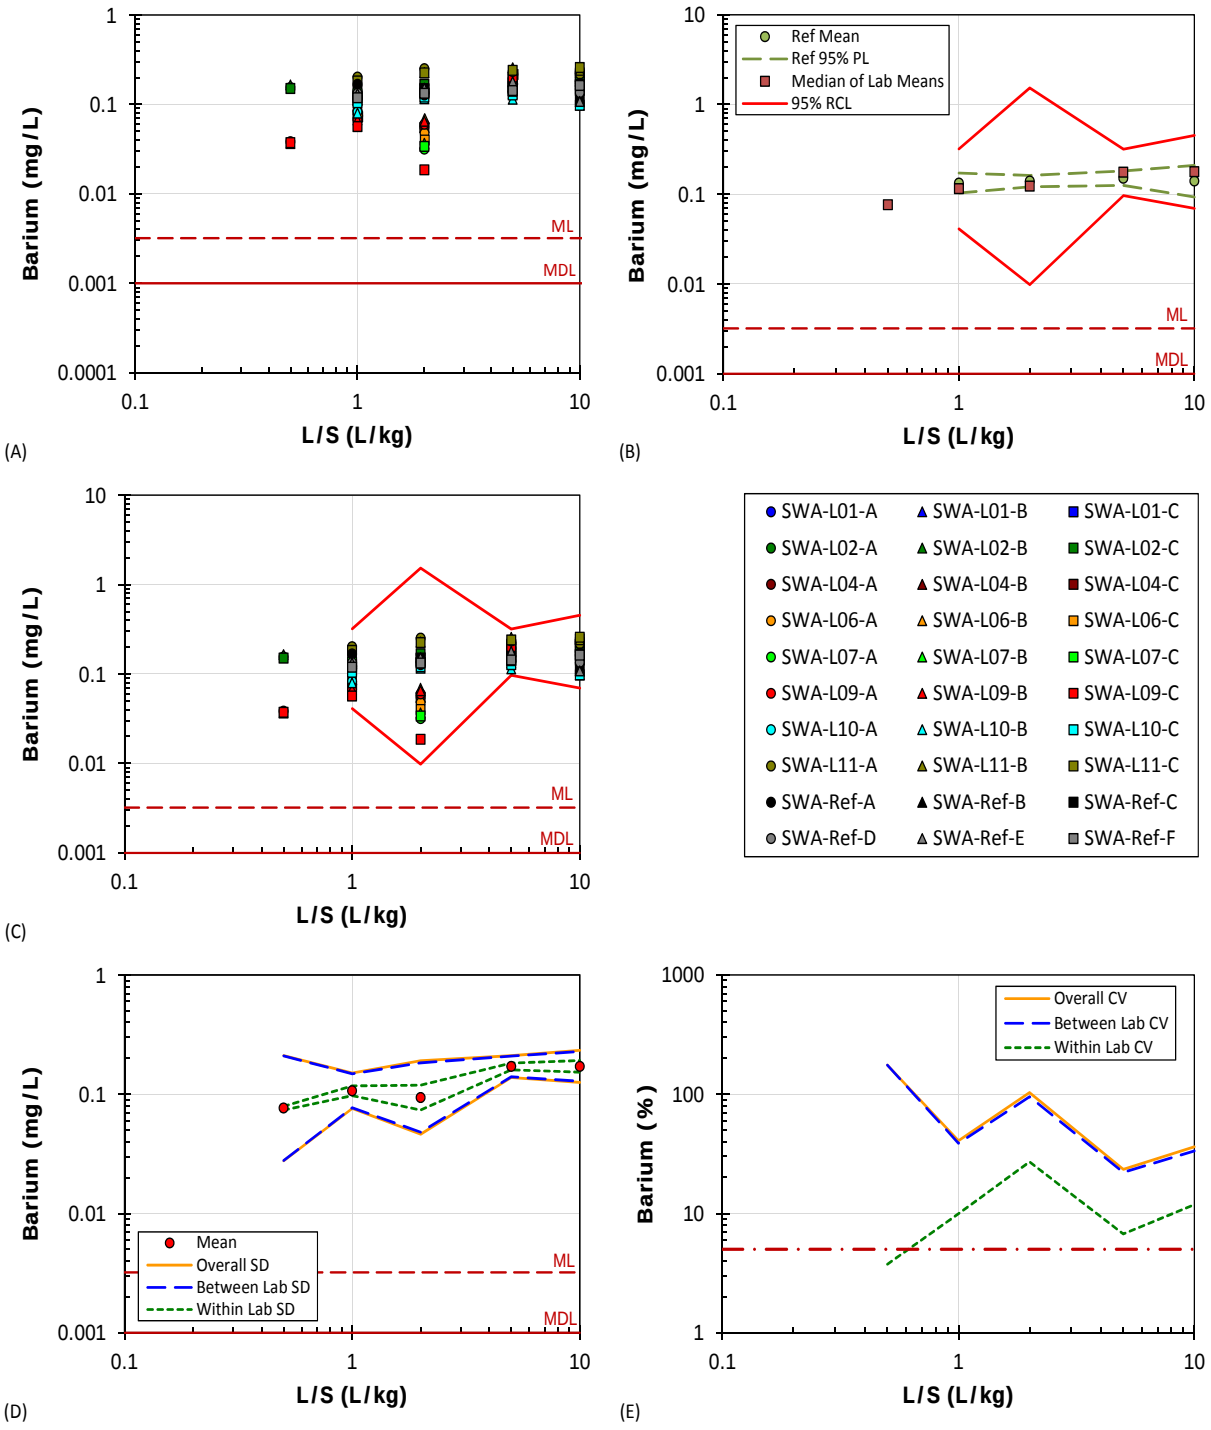

Figure 13. Barium statistical analysis for Method 1316 Phase II material SWA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

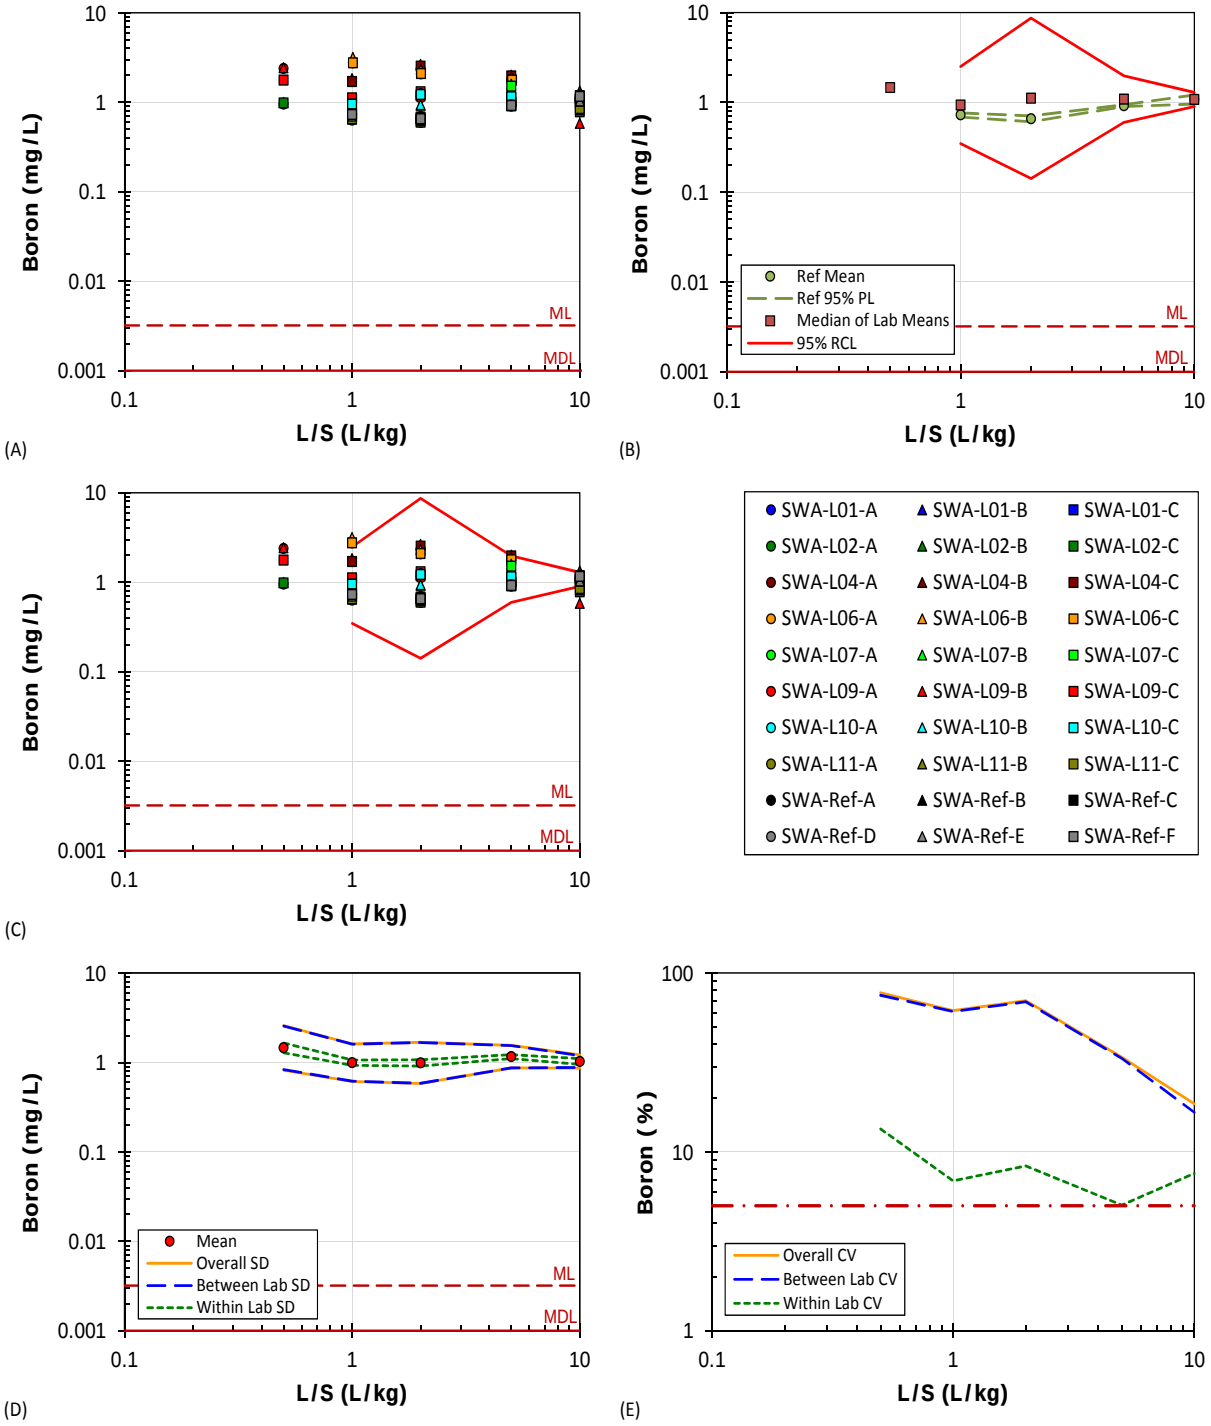

Figure 14. Boron statistical analysis for Method 1316 Phase II material SWA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

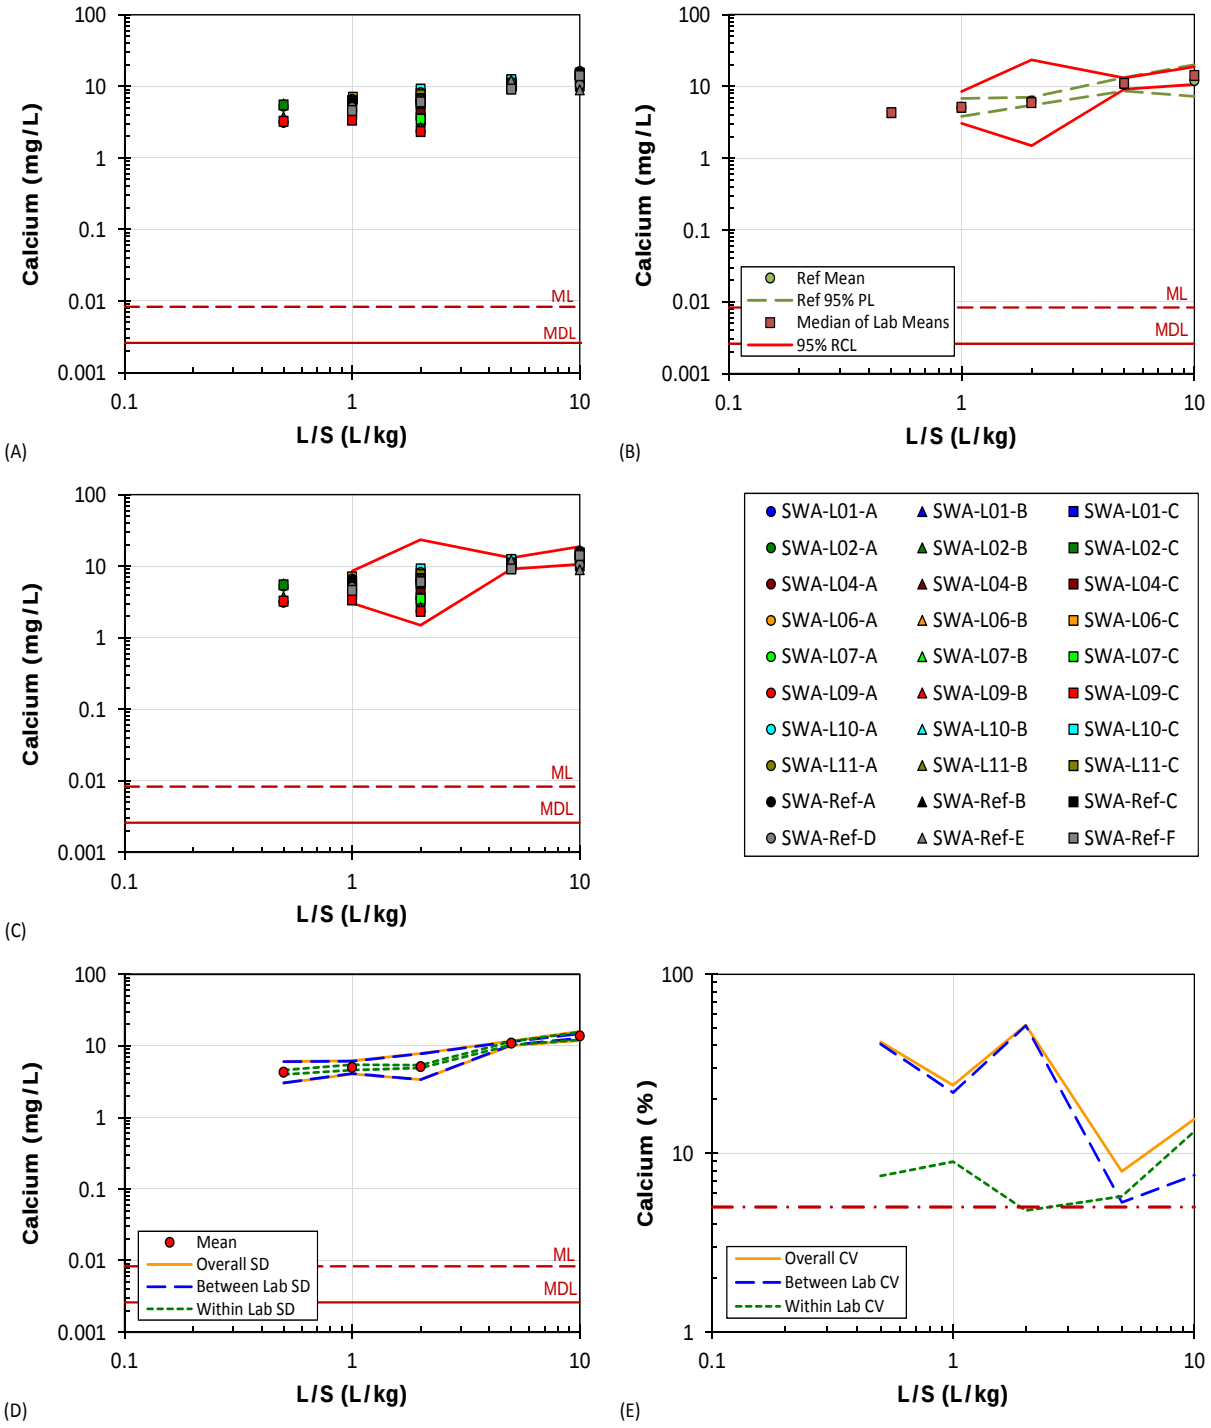

Figure 15. Calcium statistical analysis for Method 1316 Phase II material SWA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

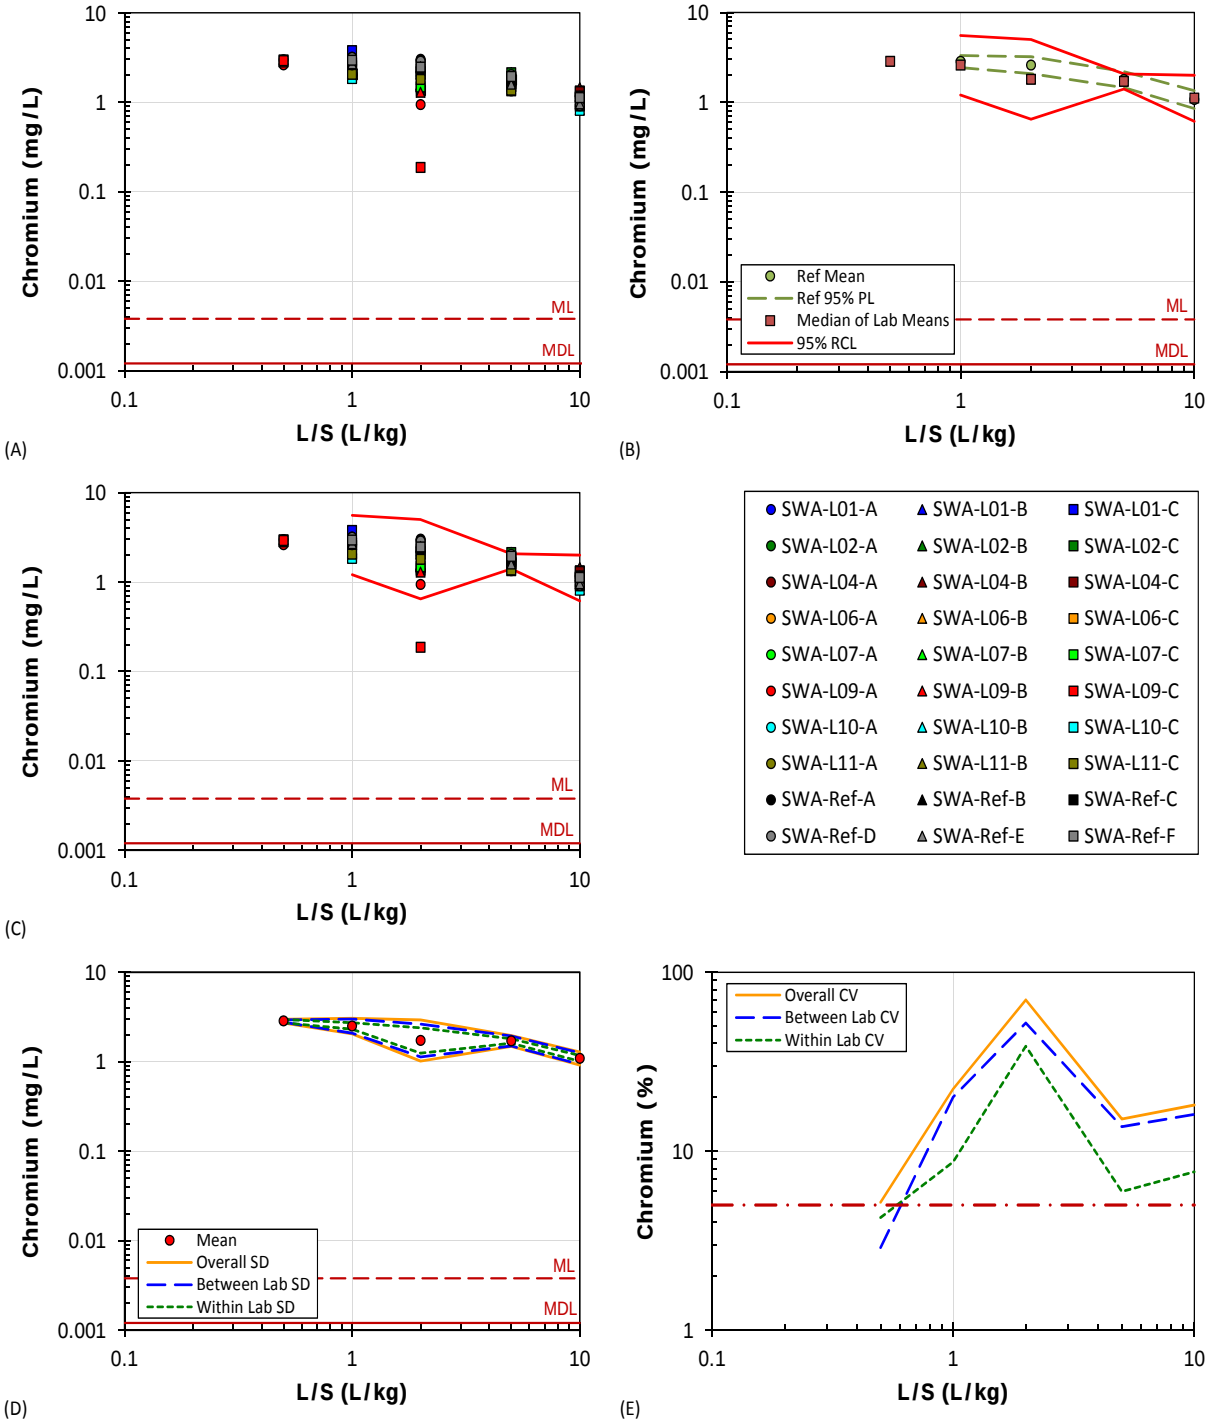

Figure 16. Chromium statistical analysis for Method 1316 Phase II material SWA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

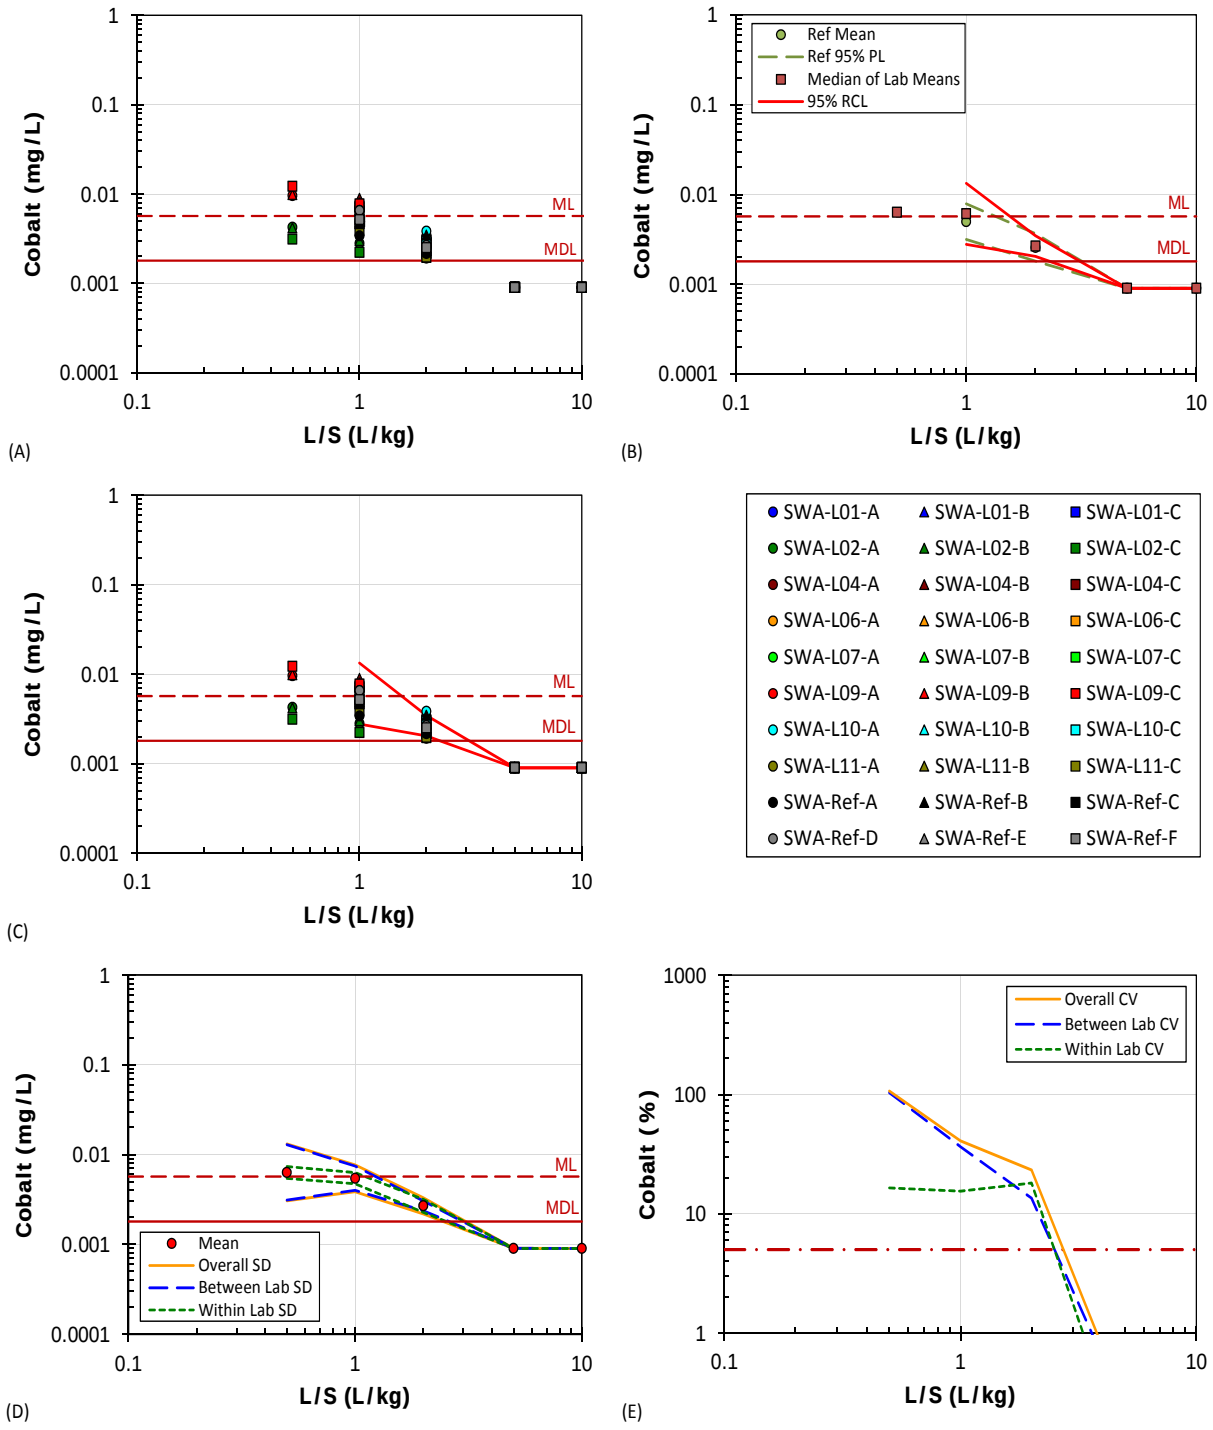

Figure 17. Cobalt statistical analysis for Method 1316 Phase II material SWA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

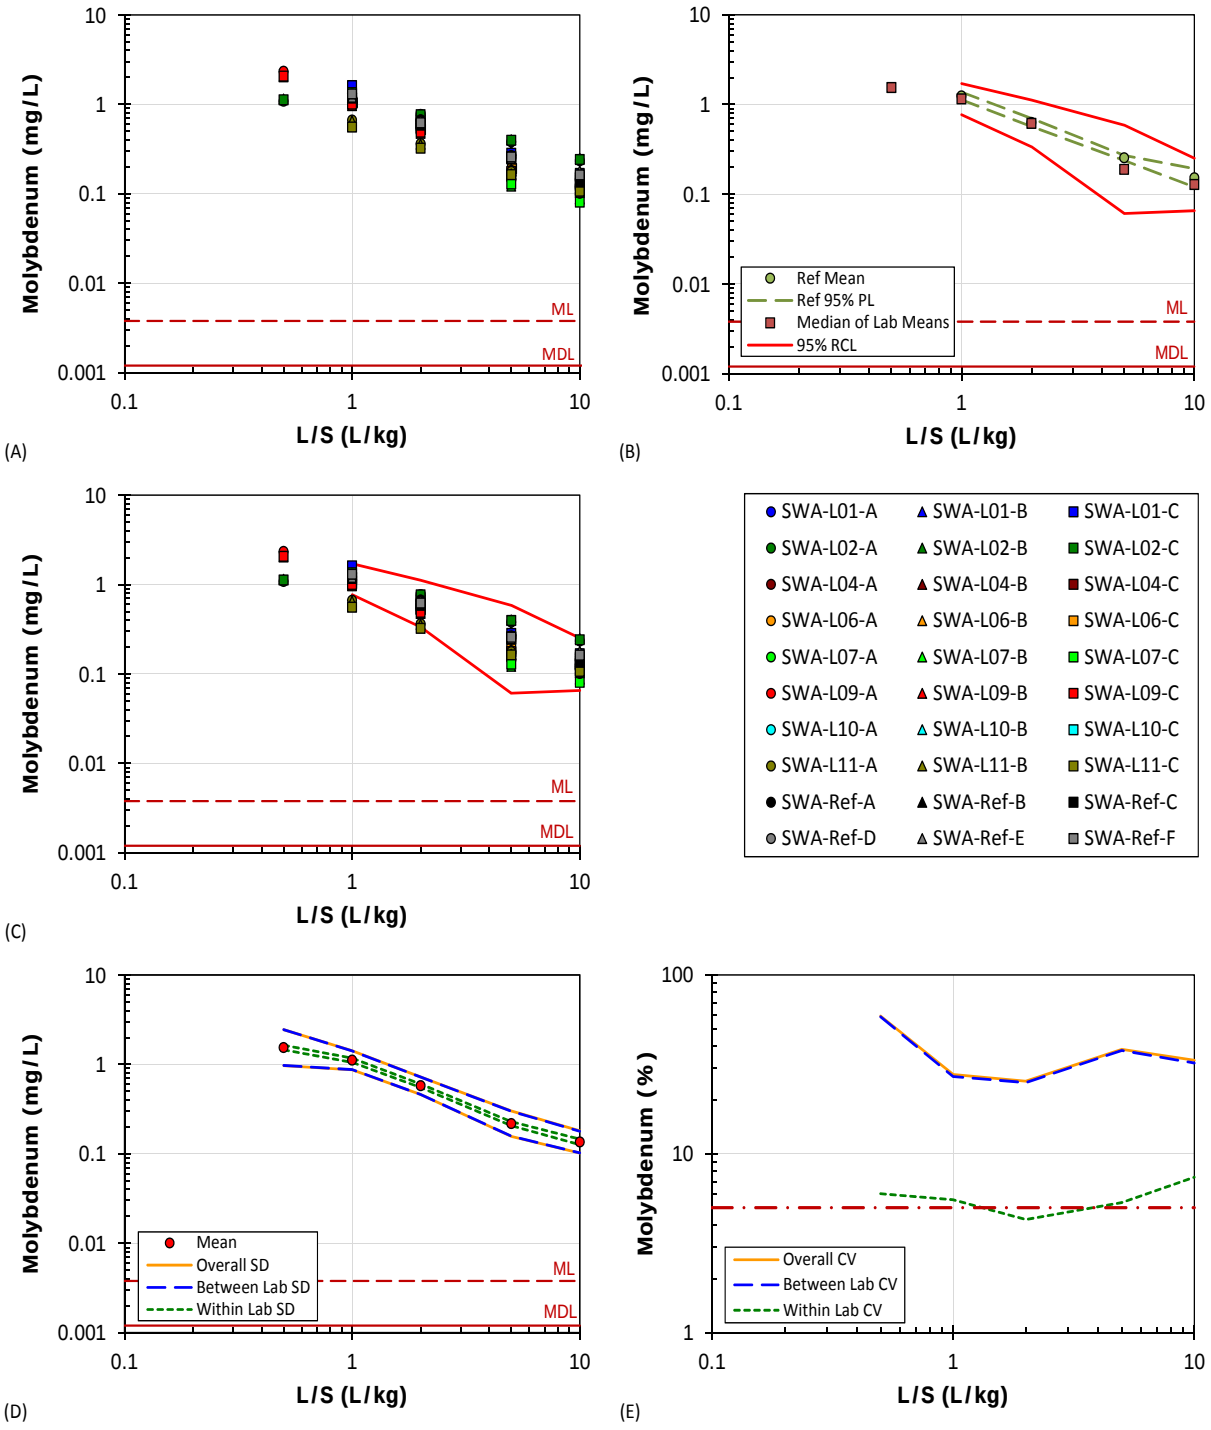

Figure 18. Molybdenum statistical analysis for Method 1316 Phase II material SWA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

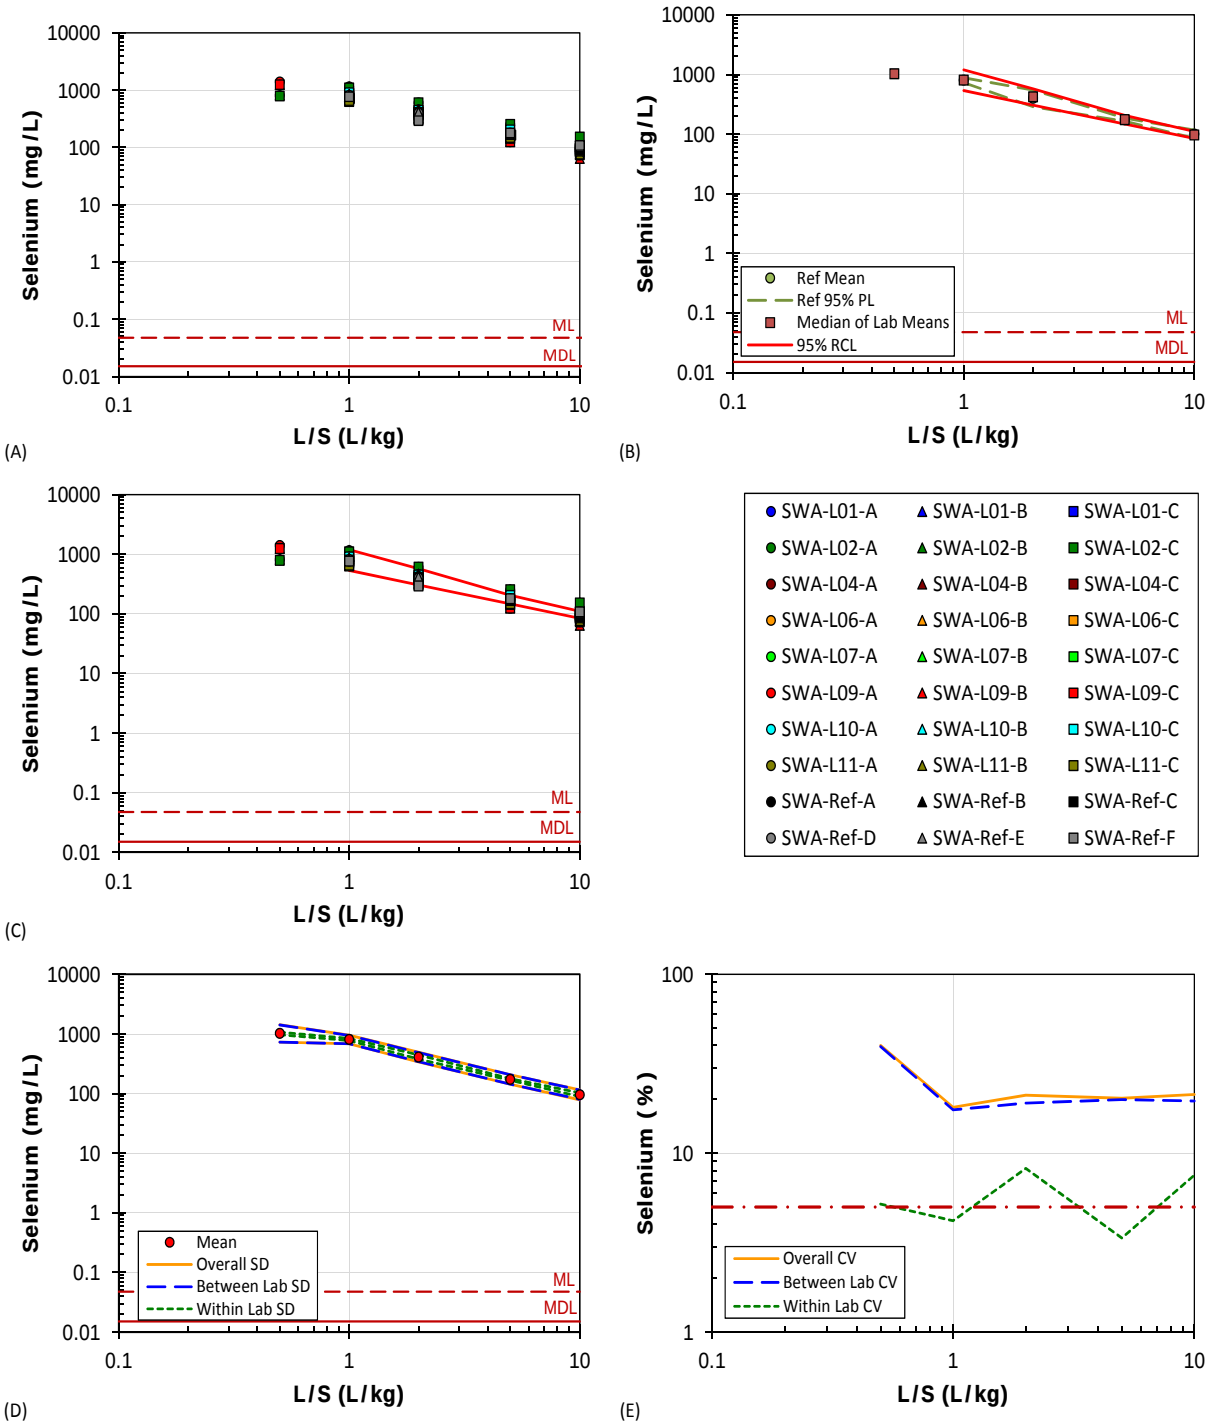

Figure 19. Selenium statistical analysis for Method 1316 Phase II material SWA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

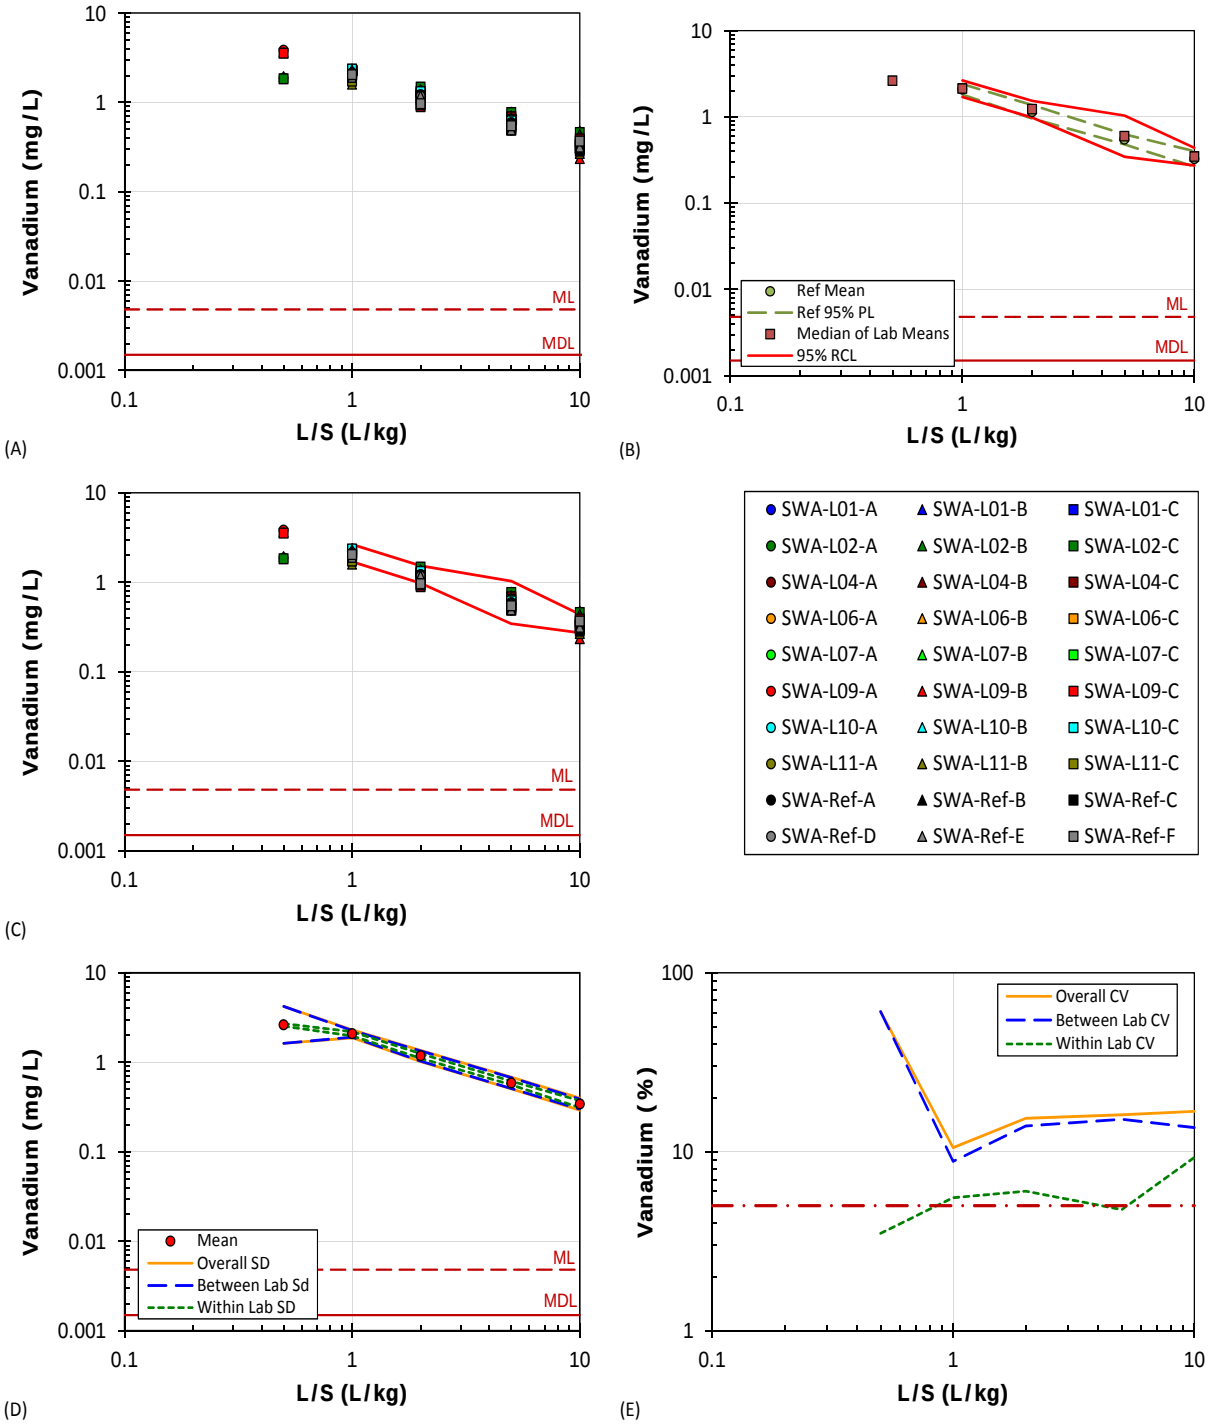

Figure 20. Vanadium statistical analysis for Method 1316 Phase II material SWA. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

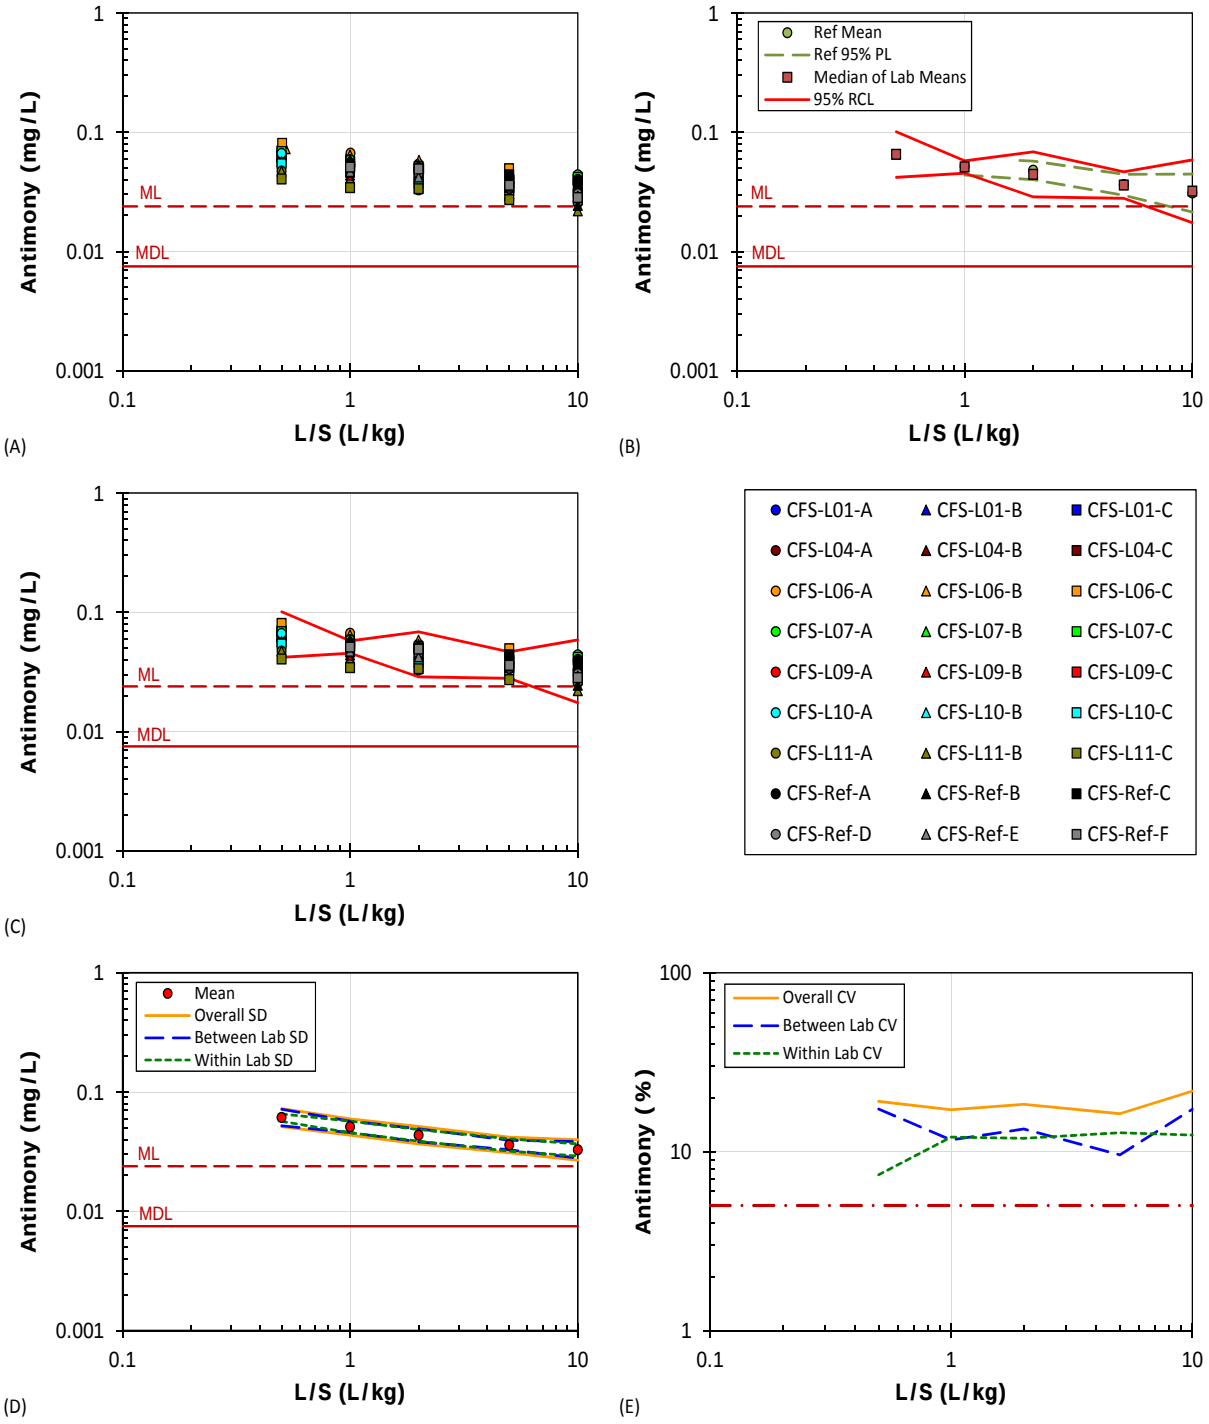

Figure 21. Antimony statistical analysis for Method 1316 Phase II material CFS. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

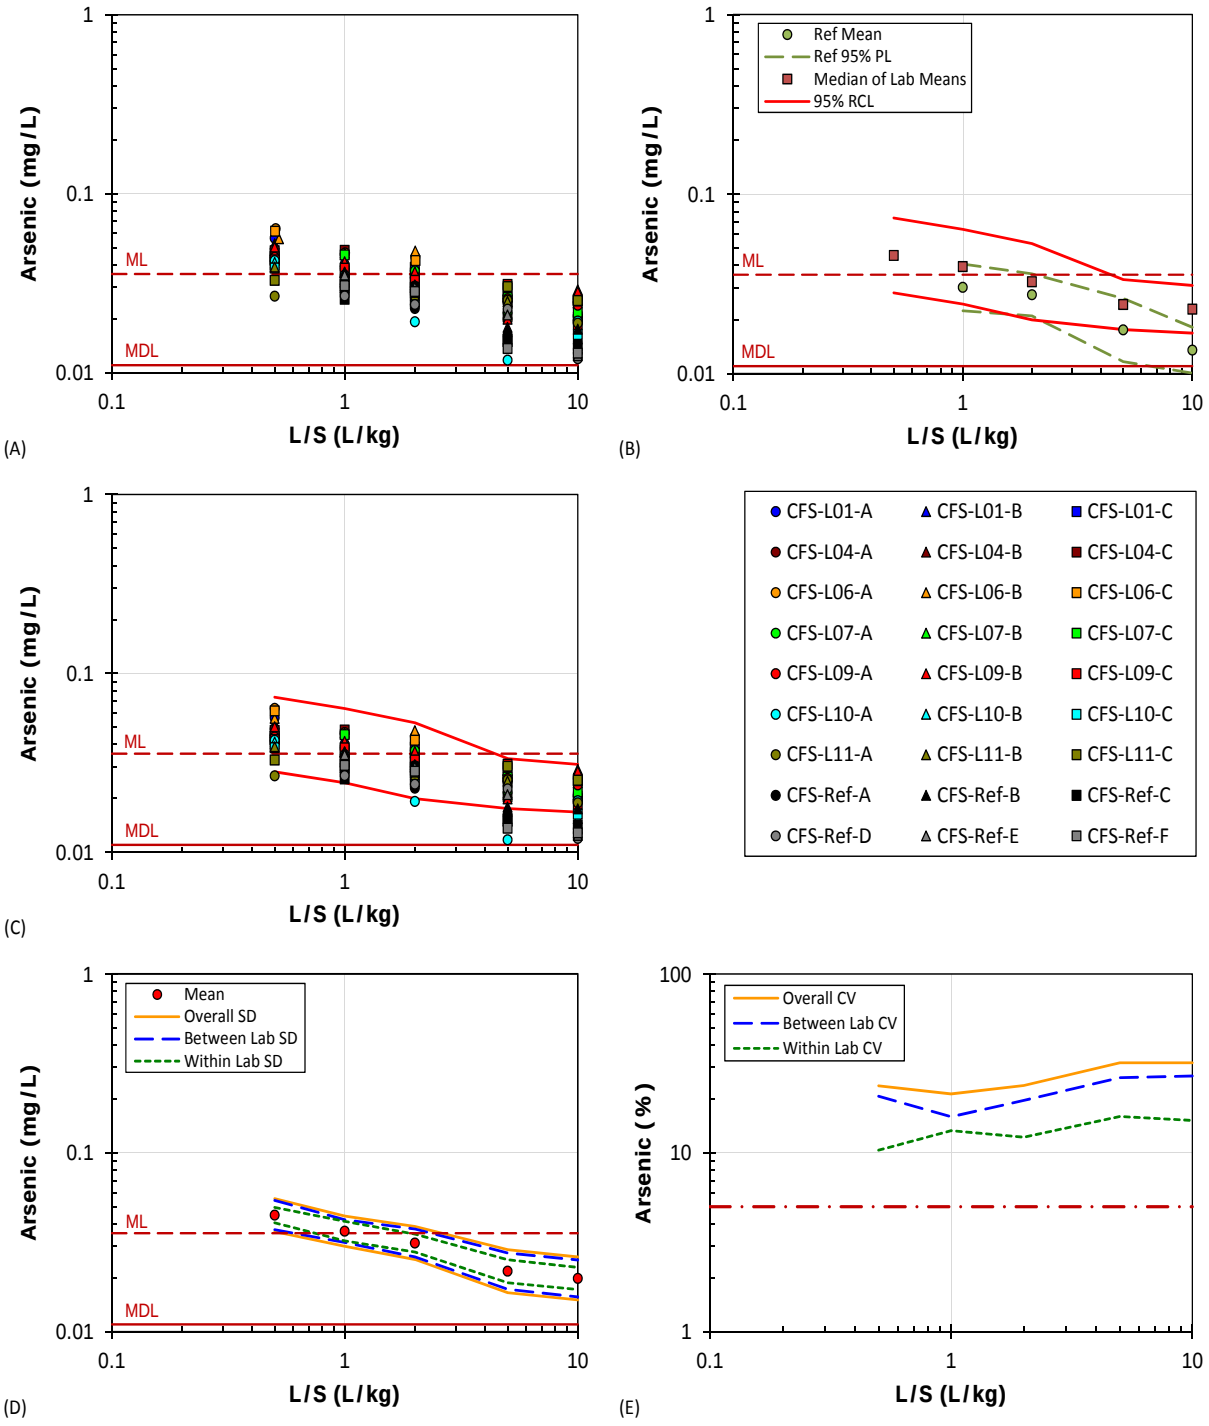

Figure 22. Arsenic statistical analysis for Method 1316 Phase II material CFS. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

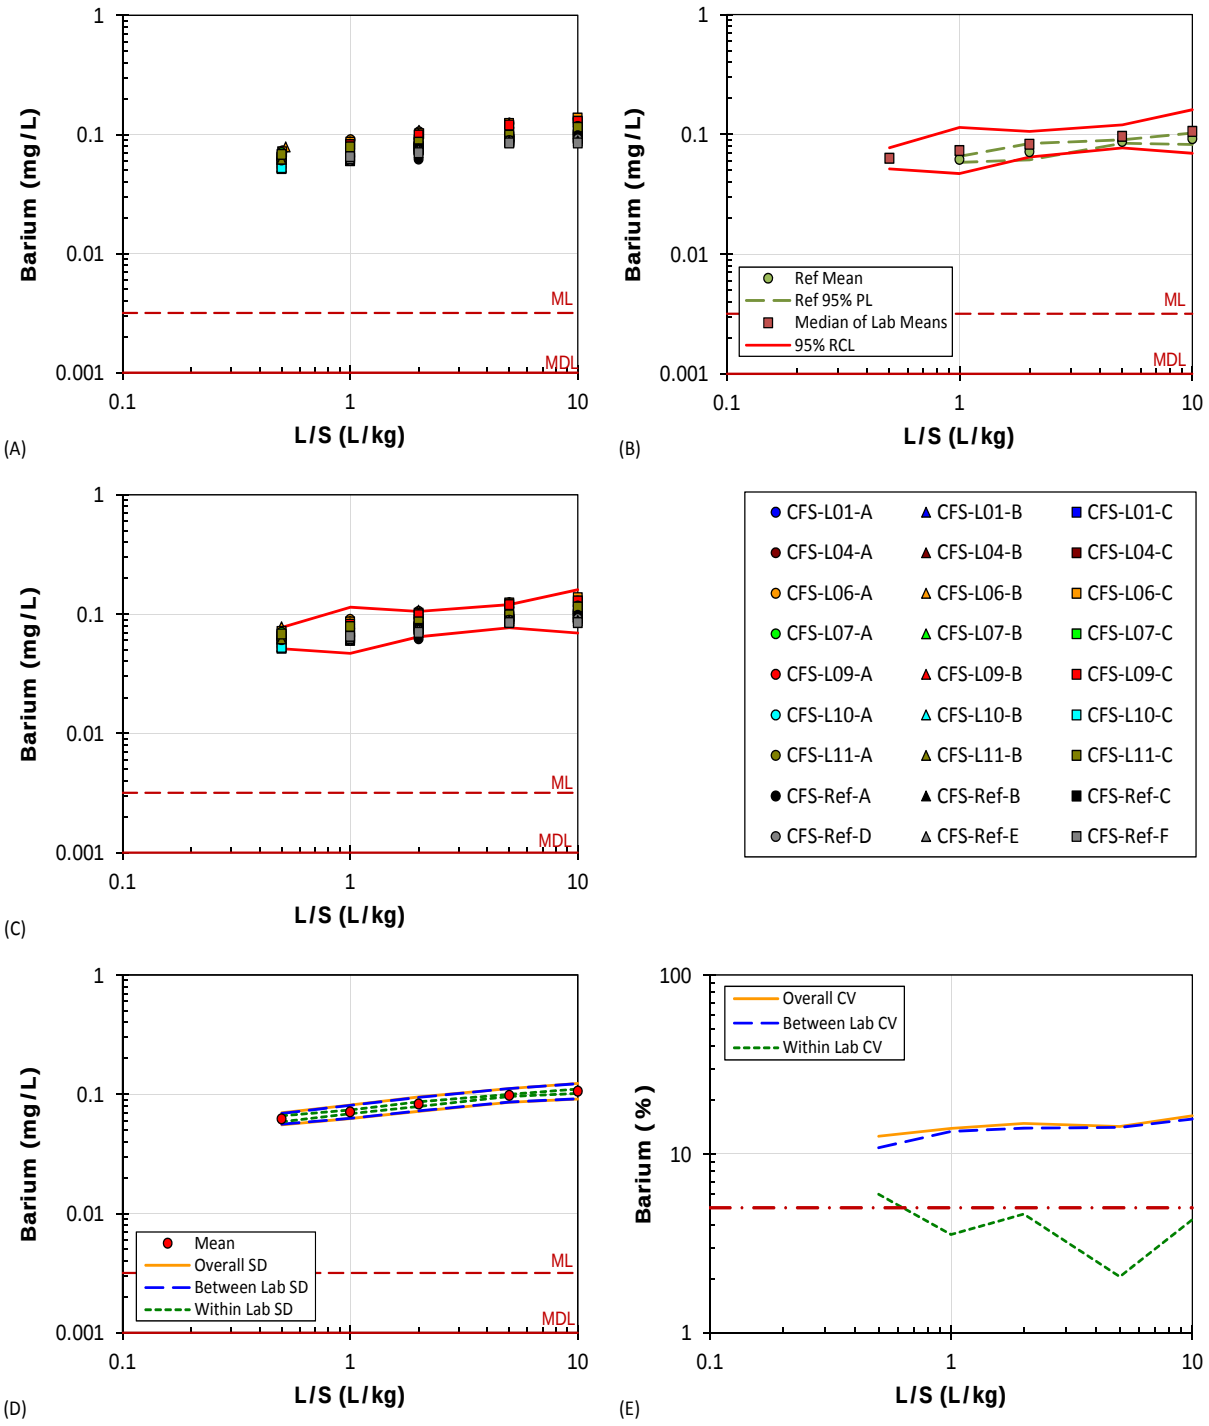

Figure 23. Barium statistical analysis for Method 1316 Phase II material CFS. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

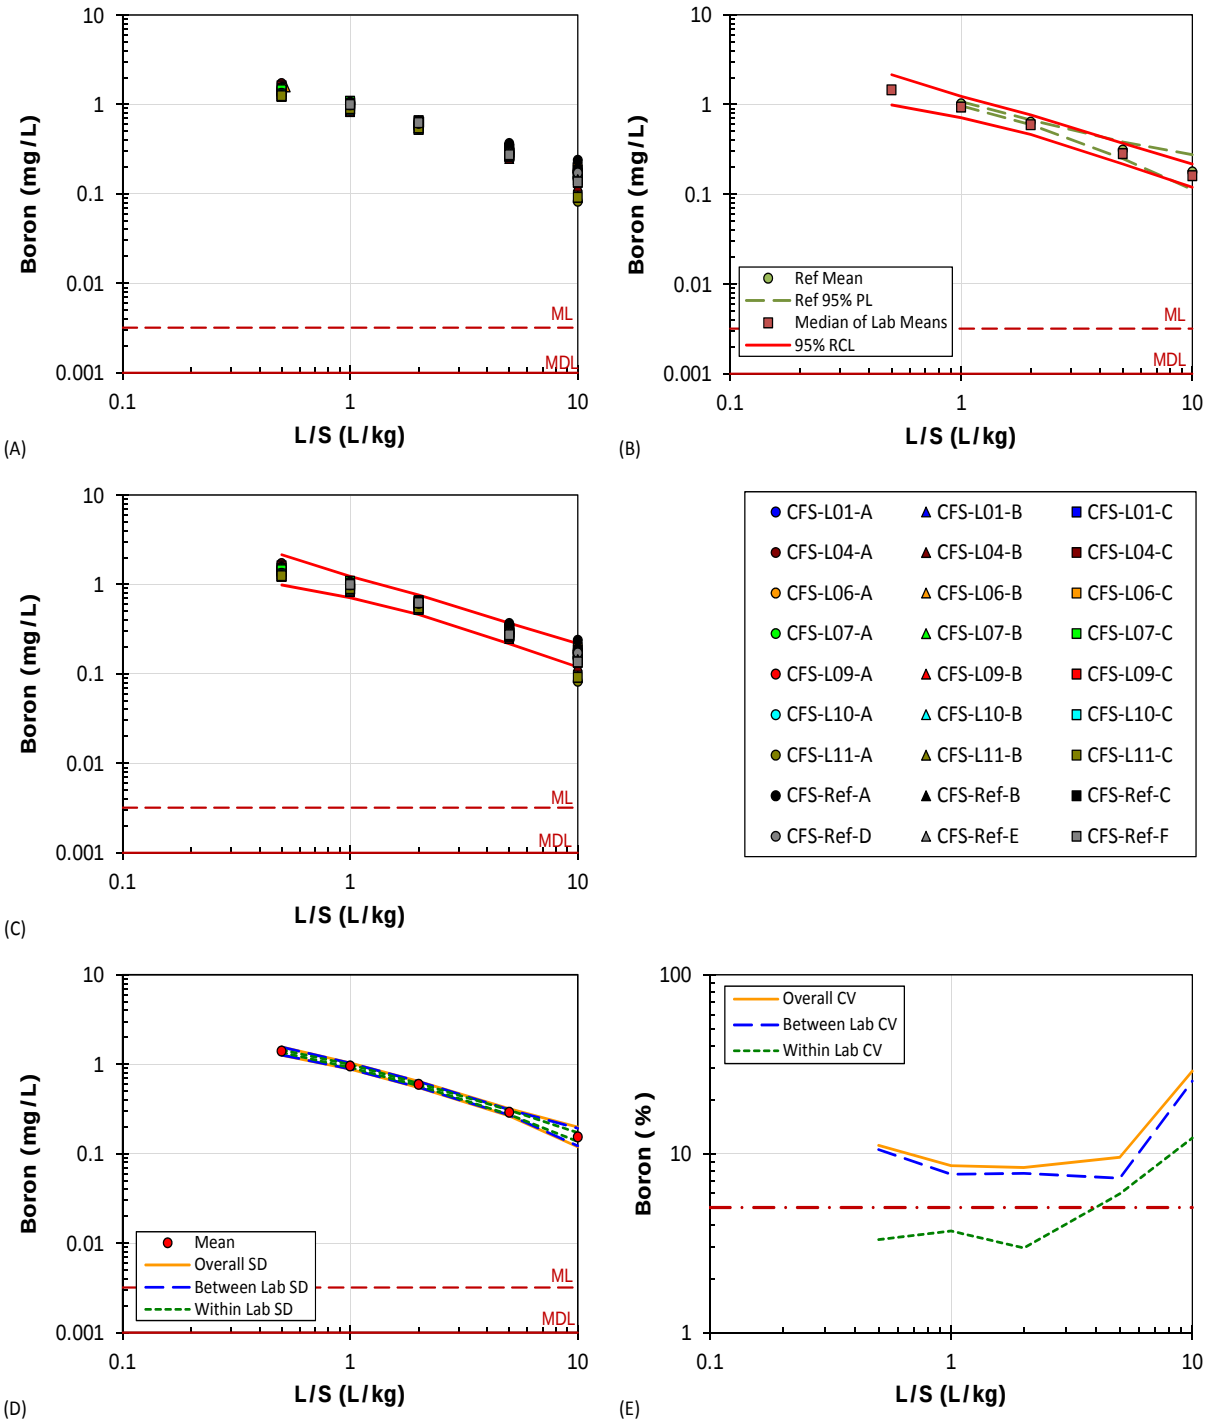

Figure 24. Boron statistical analysis for Method 1316 Phase II material CFS. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

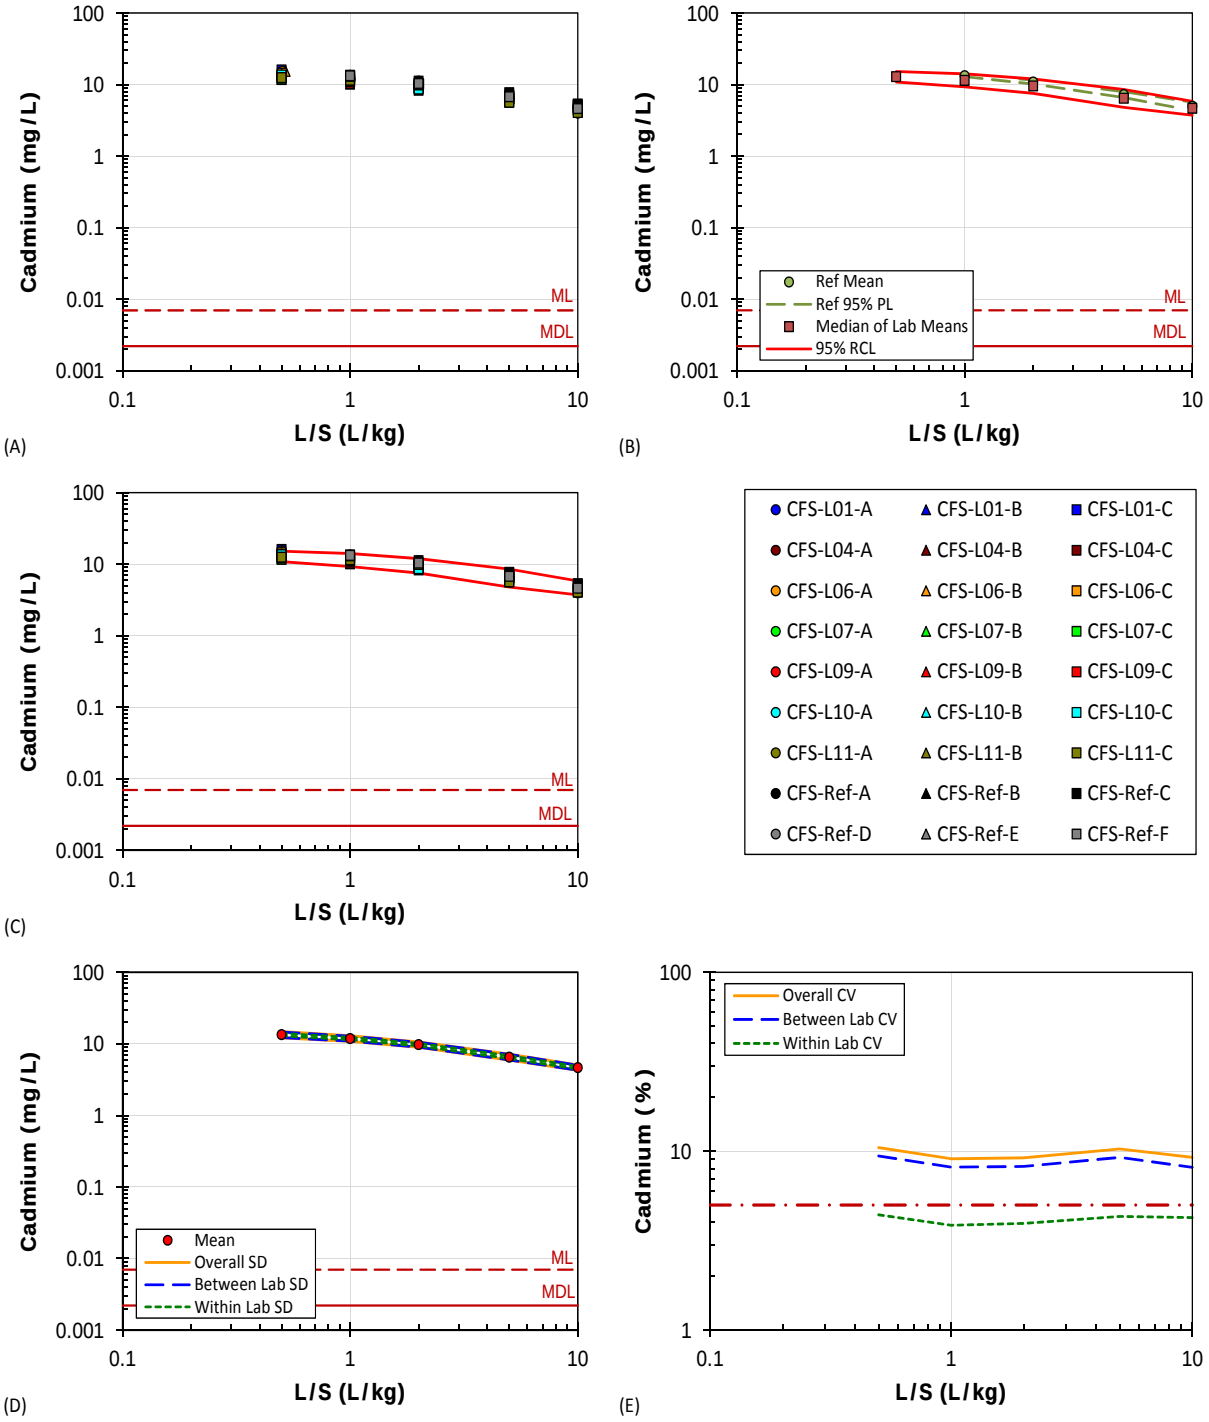

Figure 25. Cadmium statistical analysis for Method 1316 Phase II material CFS. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

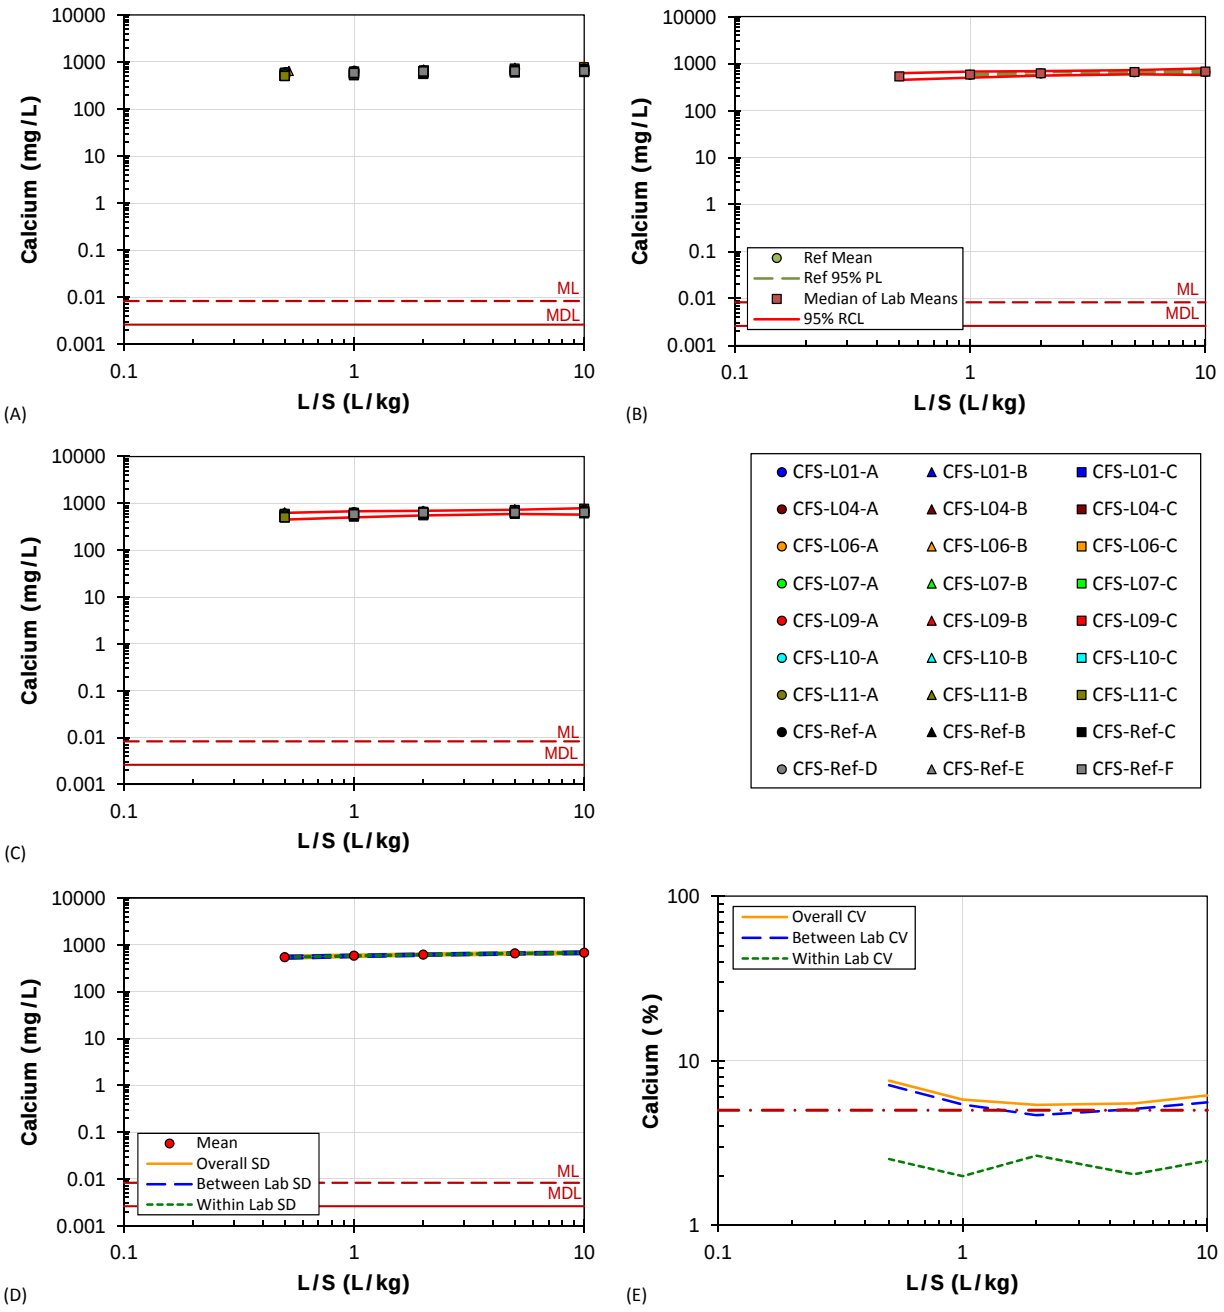

Figure 26. Calcium statistical analysis for Method 1316 Phase II material CFS. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

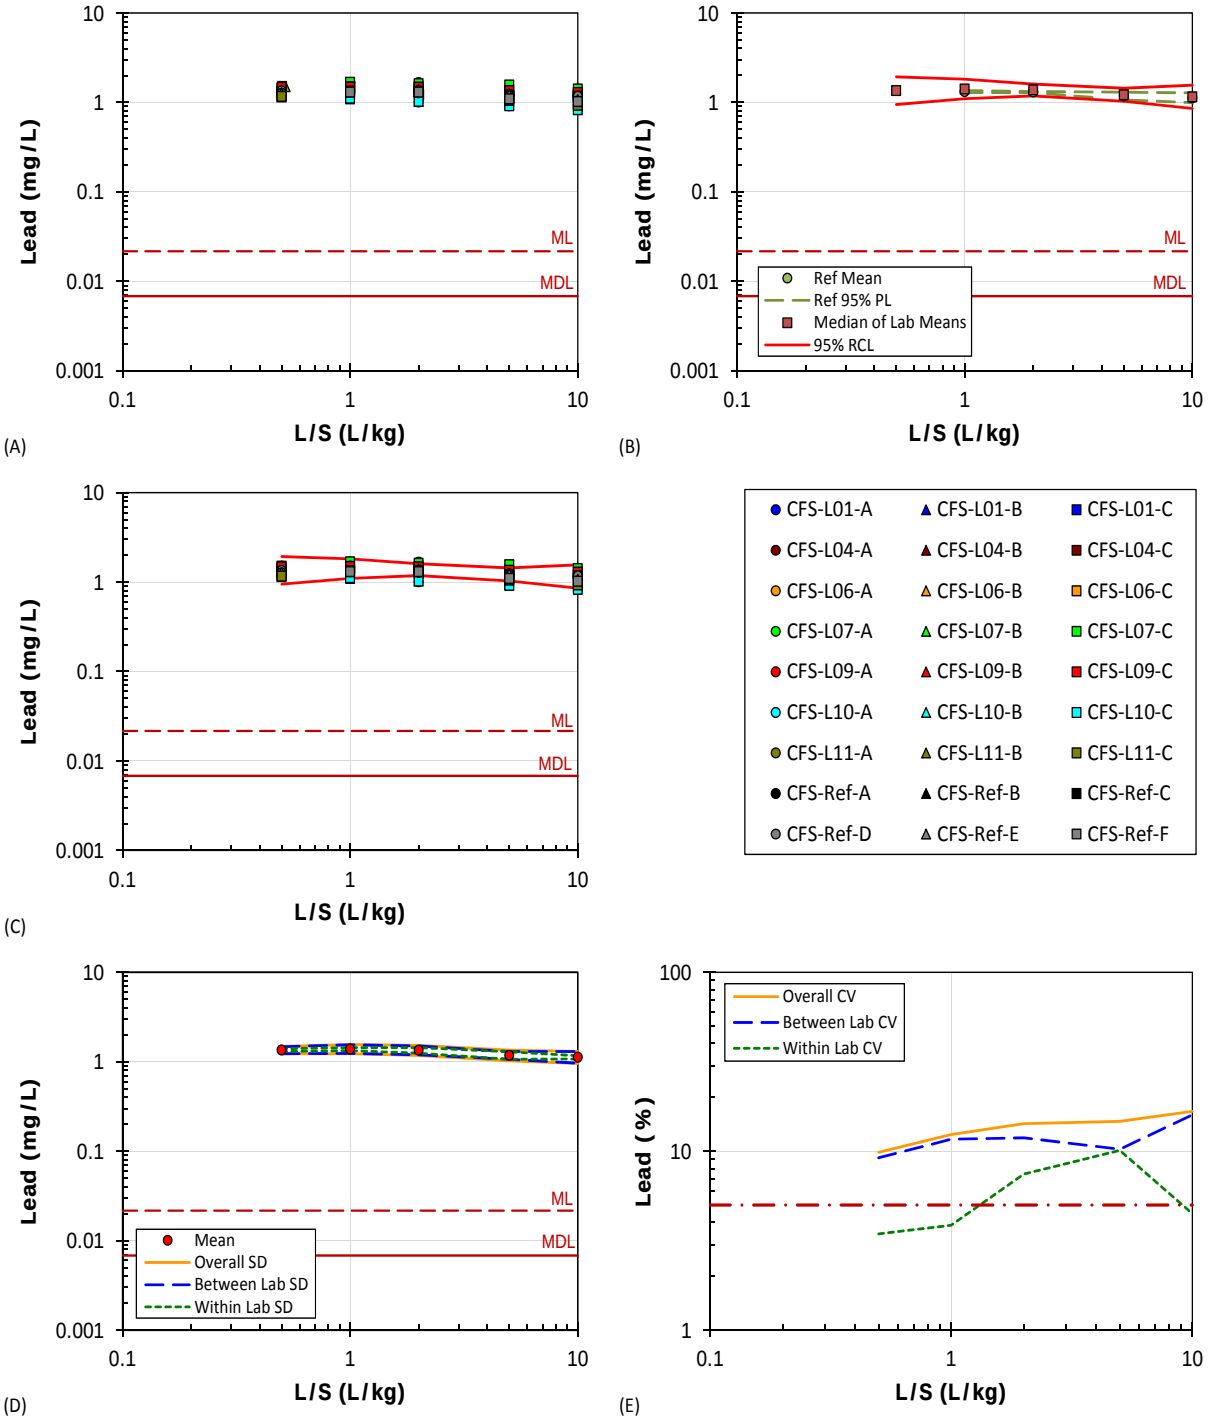

Figure 27. Lead statistical analysis for Method 1316 Phase II material CFS. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

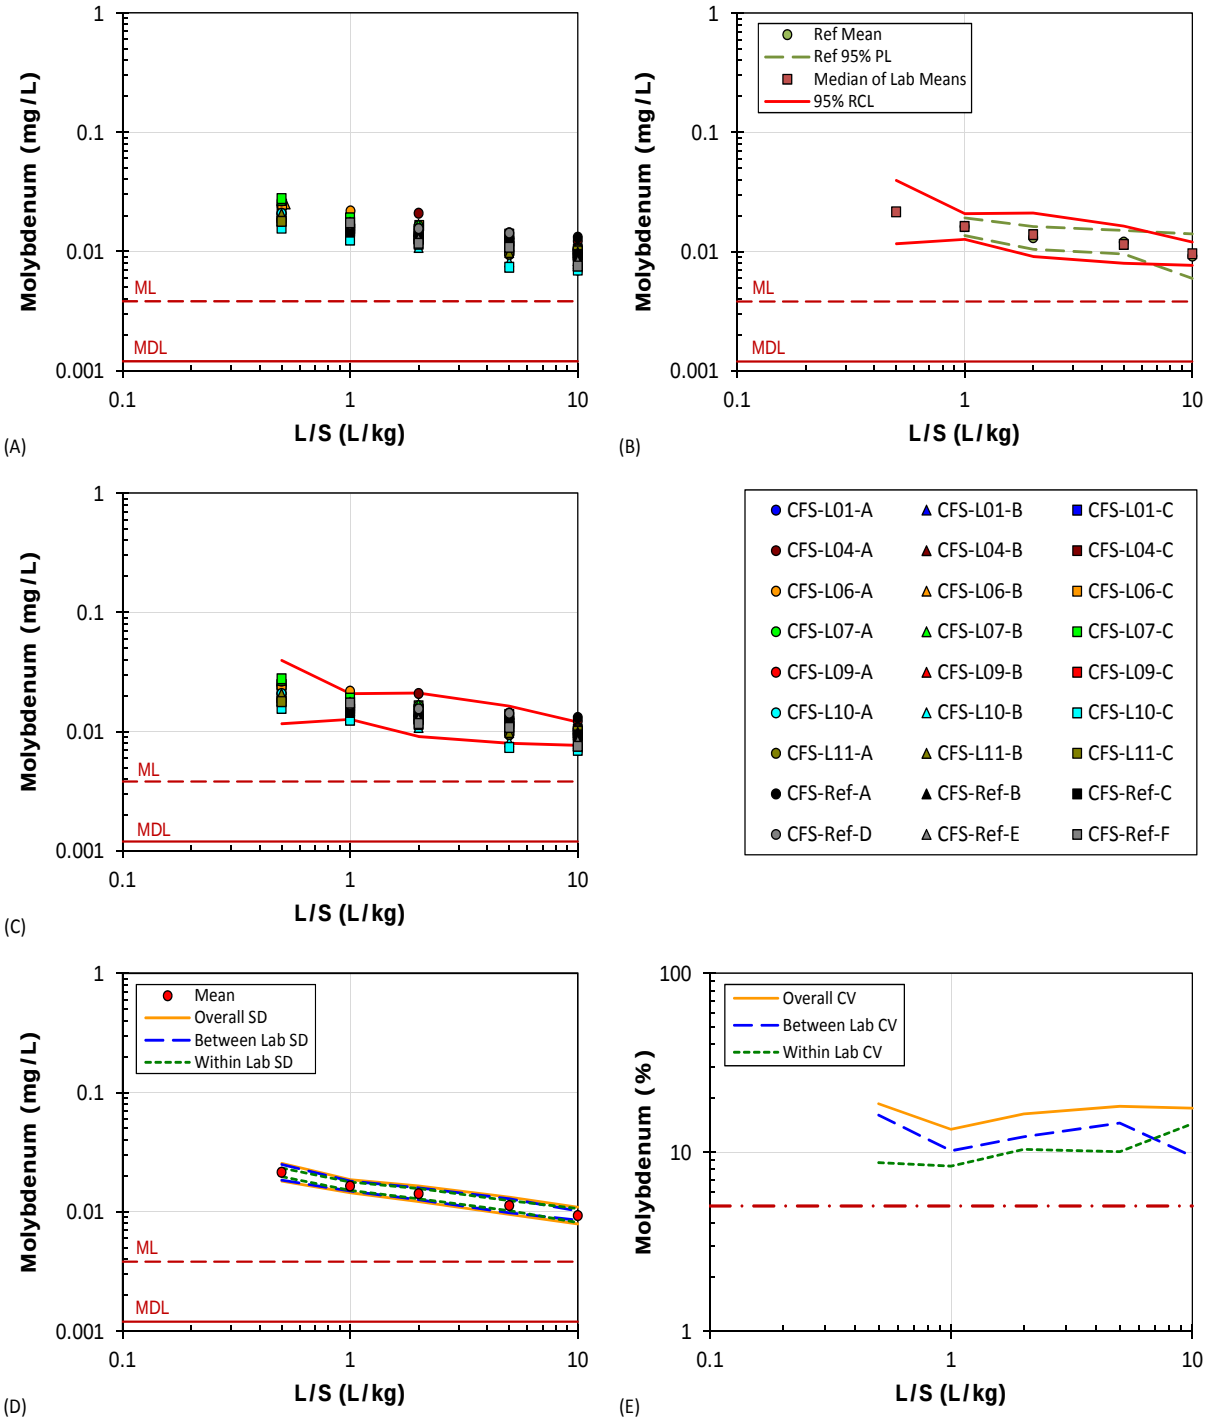

Figure 28. Molybdenum statistical analysis for Method 1316 Phase II material CFS. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

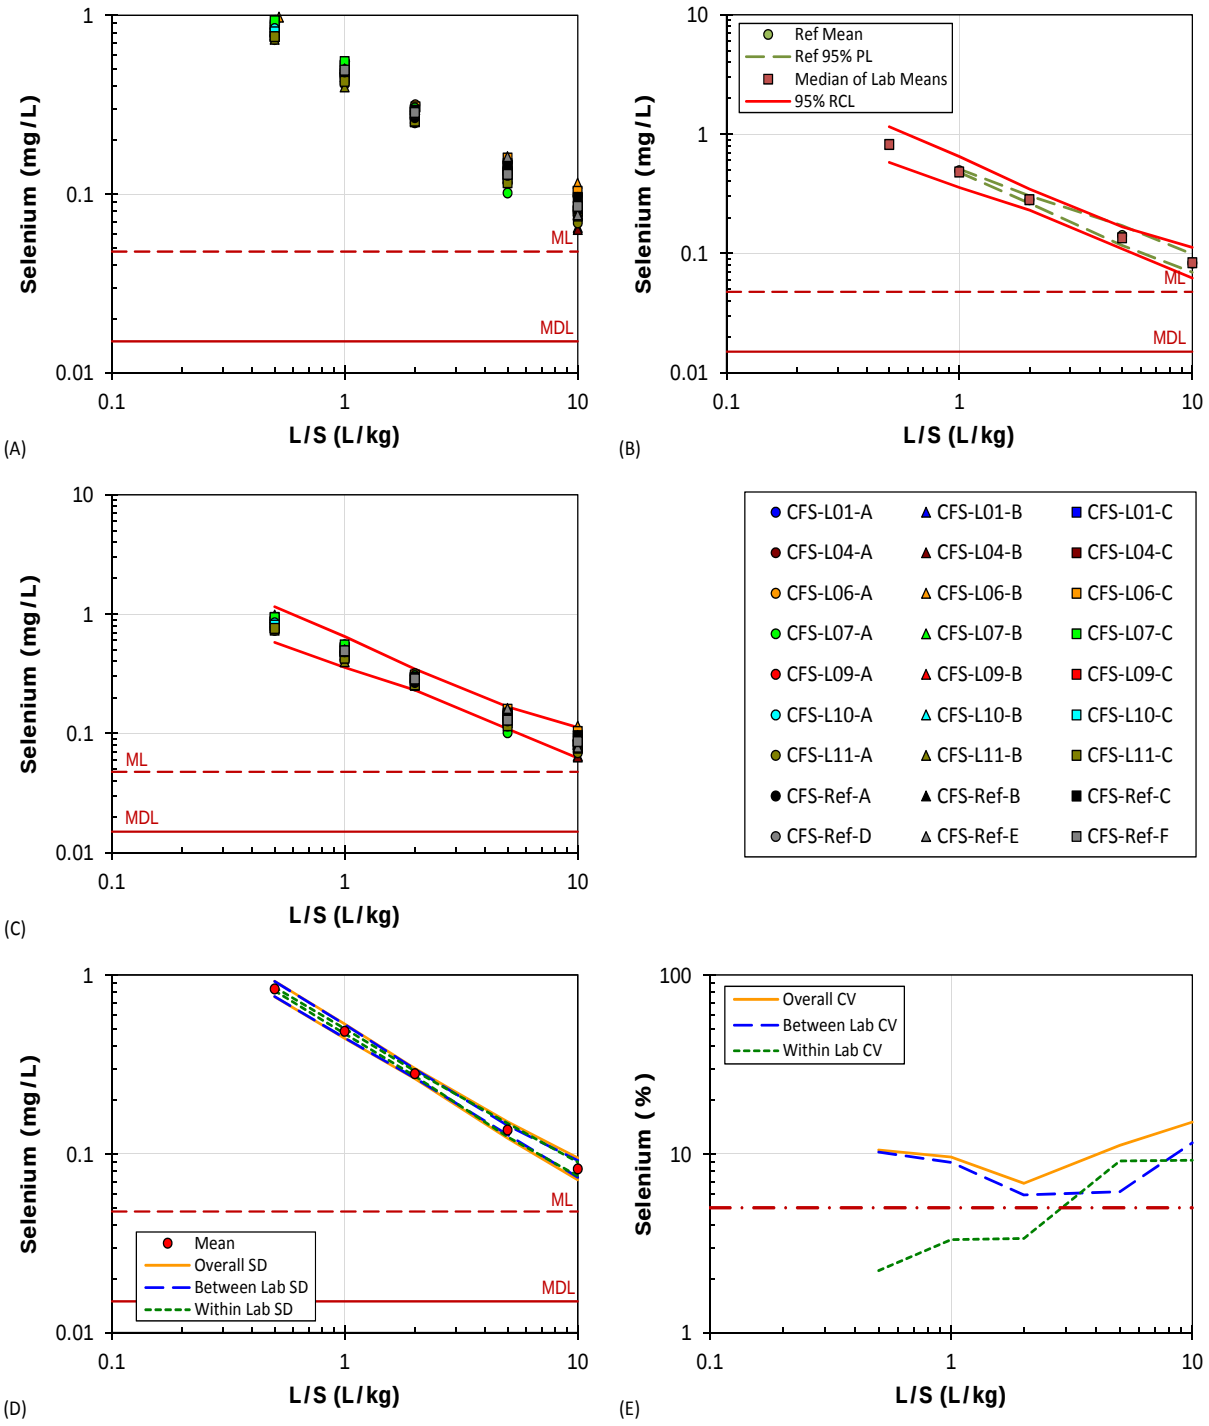

Figure 29. Selenium statistical analysis for Method 1316 Phase II material CFS. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

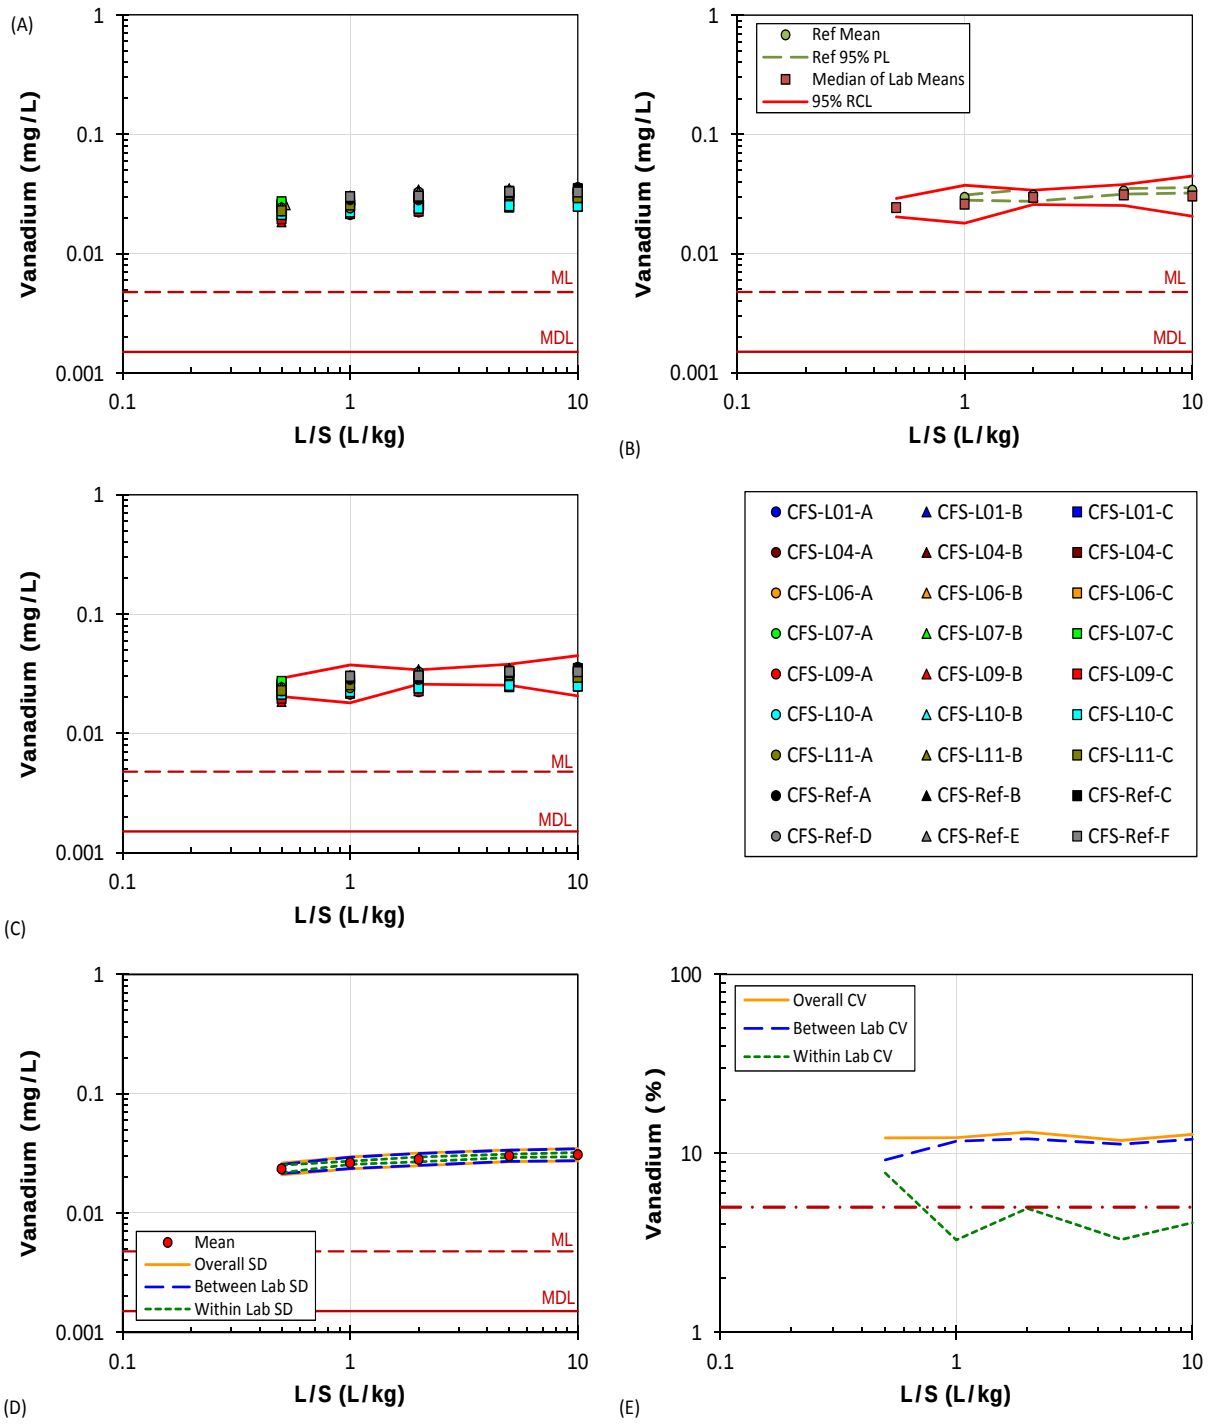

Figure 30. Vanadium statistical analysis for Method 1316 Phase II material CFS. (A) collected data as a function of pH; (B) reference lab mean and 95% prediction limits (PL; green, dashed line) compared to the median of lab means and median-based 95% robust confidence limits (RCL; red line); (C) 95% RCL intervals (red lines) shown with respect to interpolated lab data; (D) intervals for "overall" (gold line), "between lab" (blue, dashed line) and pooled "within labs" (green, dotted line) standard deviation about the mean of all data; (E) coefficient of variation for upper values of "overall", "between lab" and "within lab" standard deviation compared to 5% marker indicating a generalized analytical uncertainty.

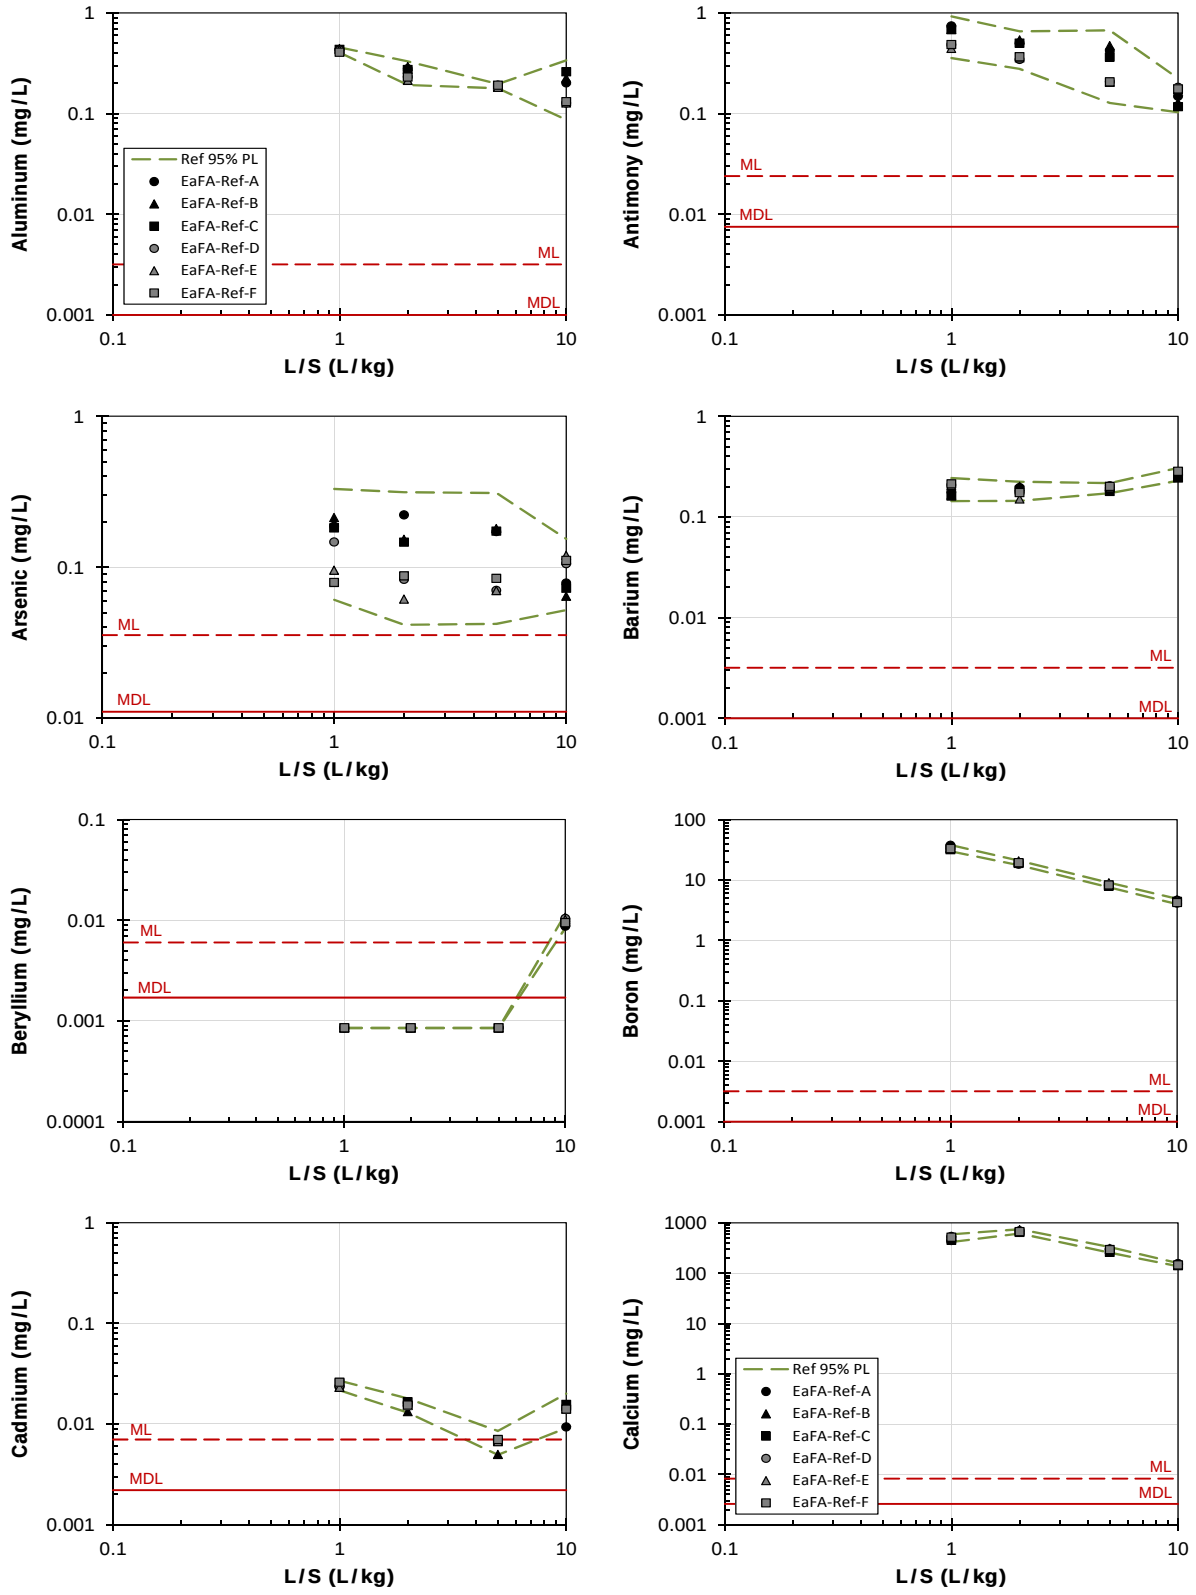

Figure 31. Reference lab data and 95% prediction limits for Method 1316 Phase I EaFA material.

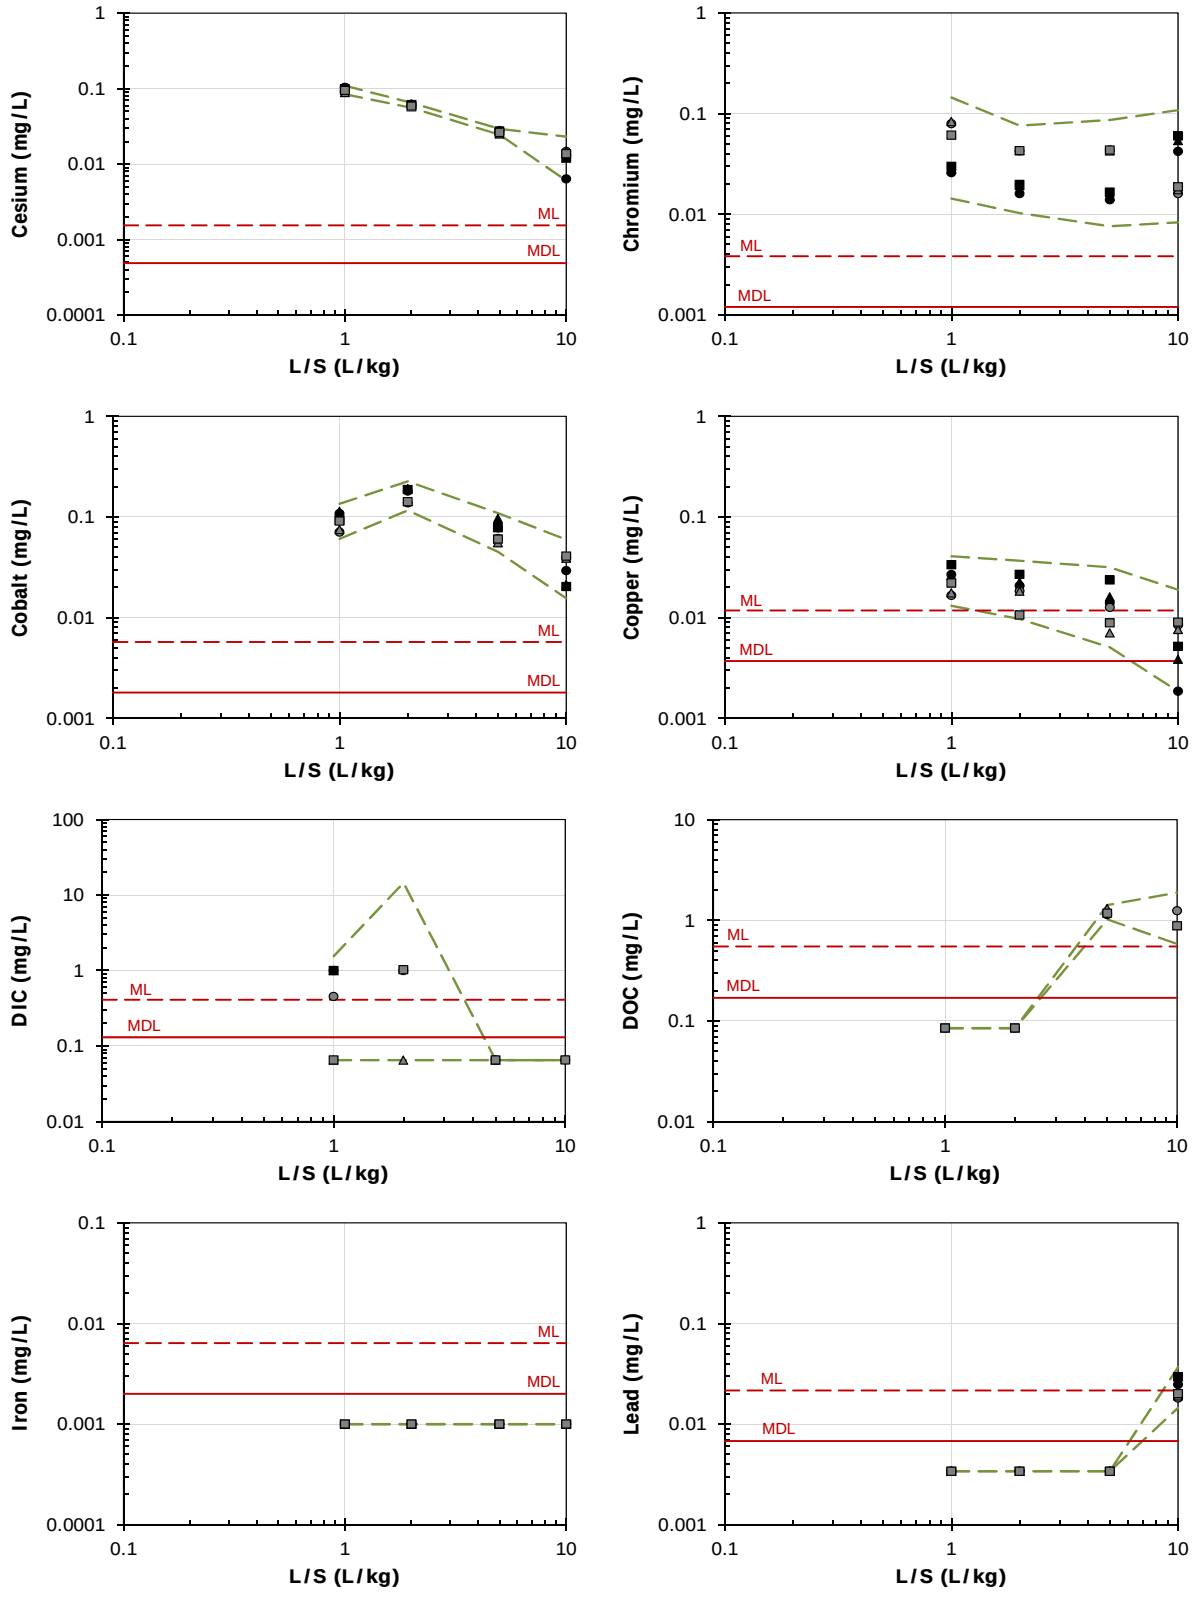

Figure 32. Reference lab data and 95% prediction limits for Method 1316 Phase I EaFA material.

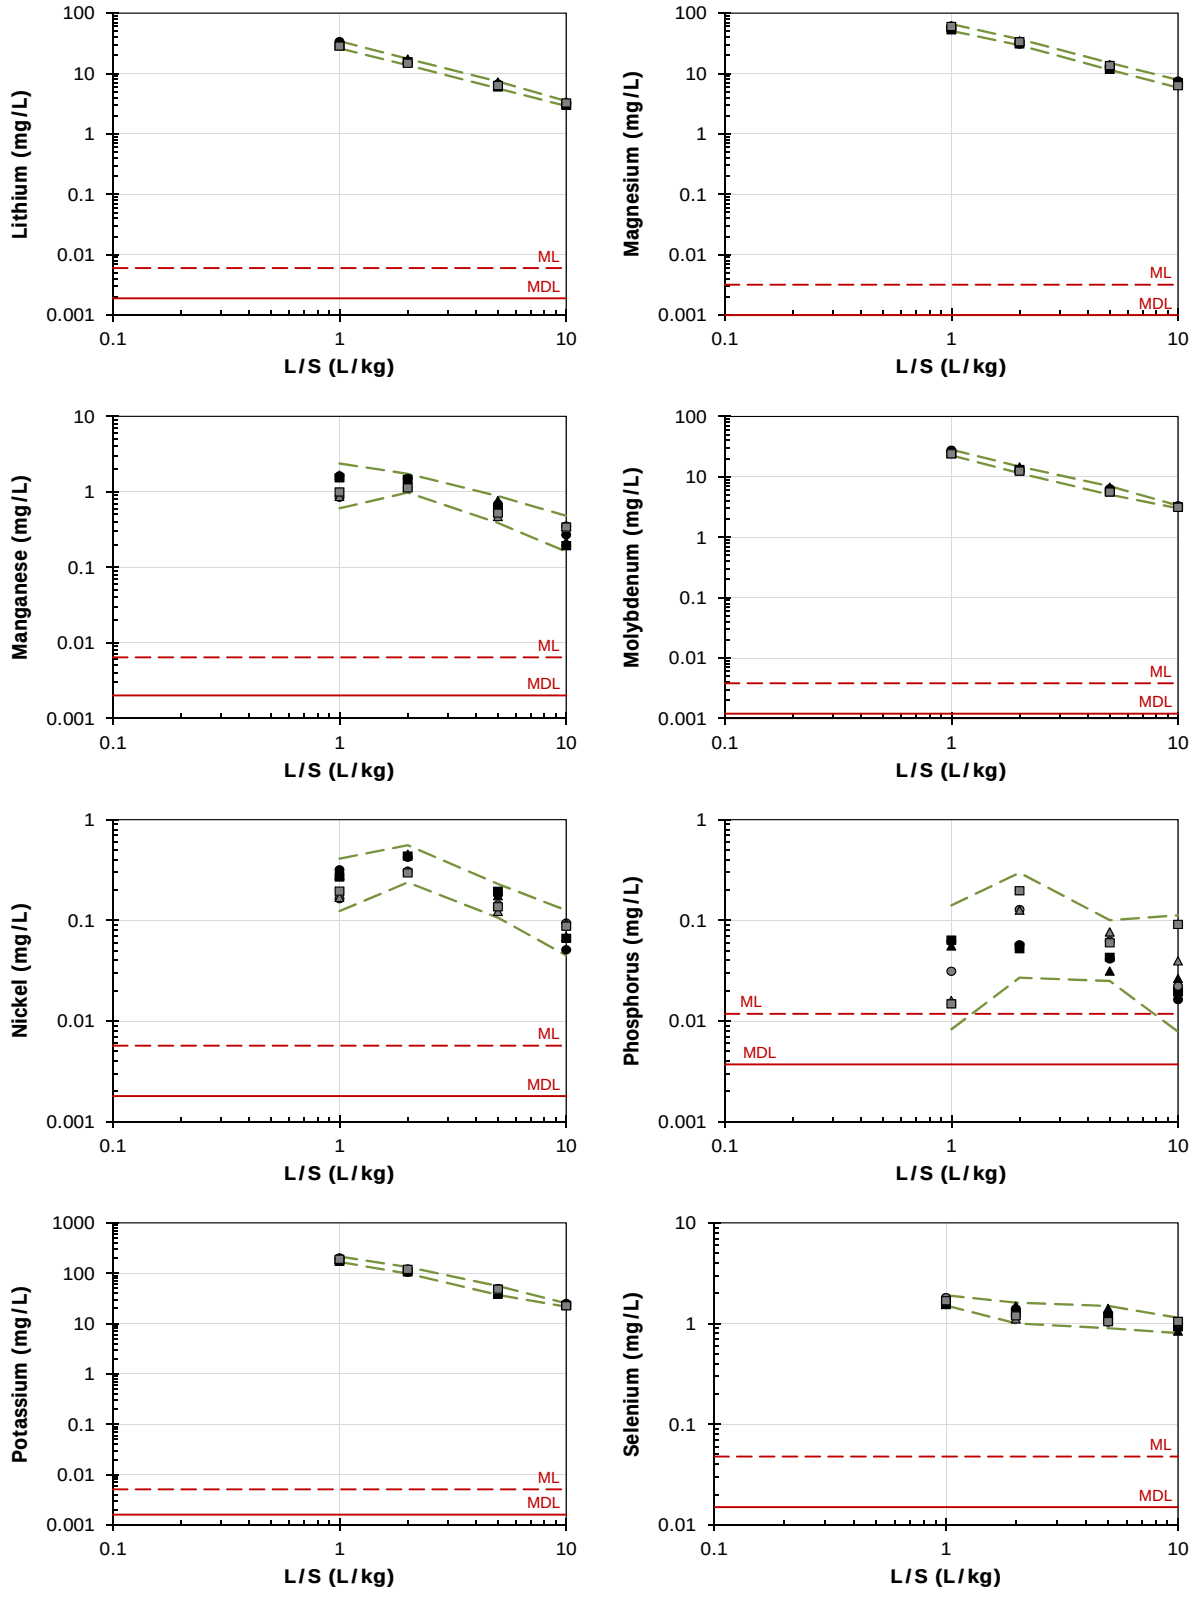

Figure 33. Reference lab data and 95% prediction limits for Method 1316 Phase I EaFA material.

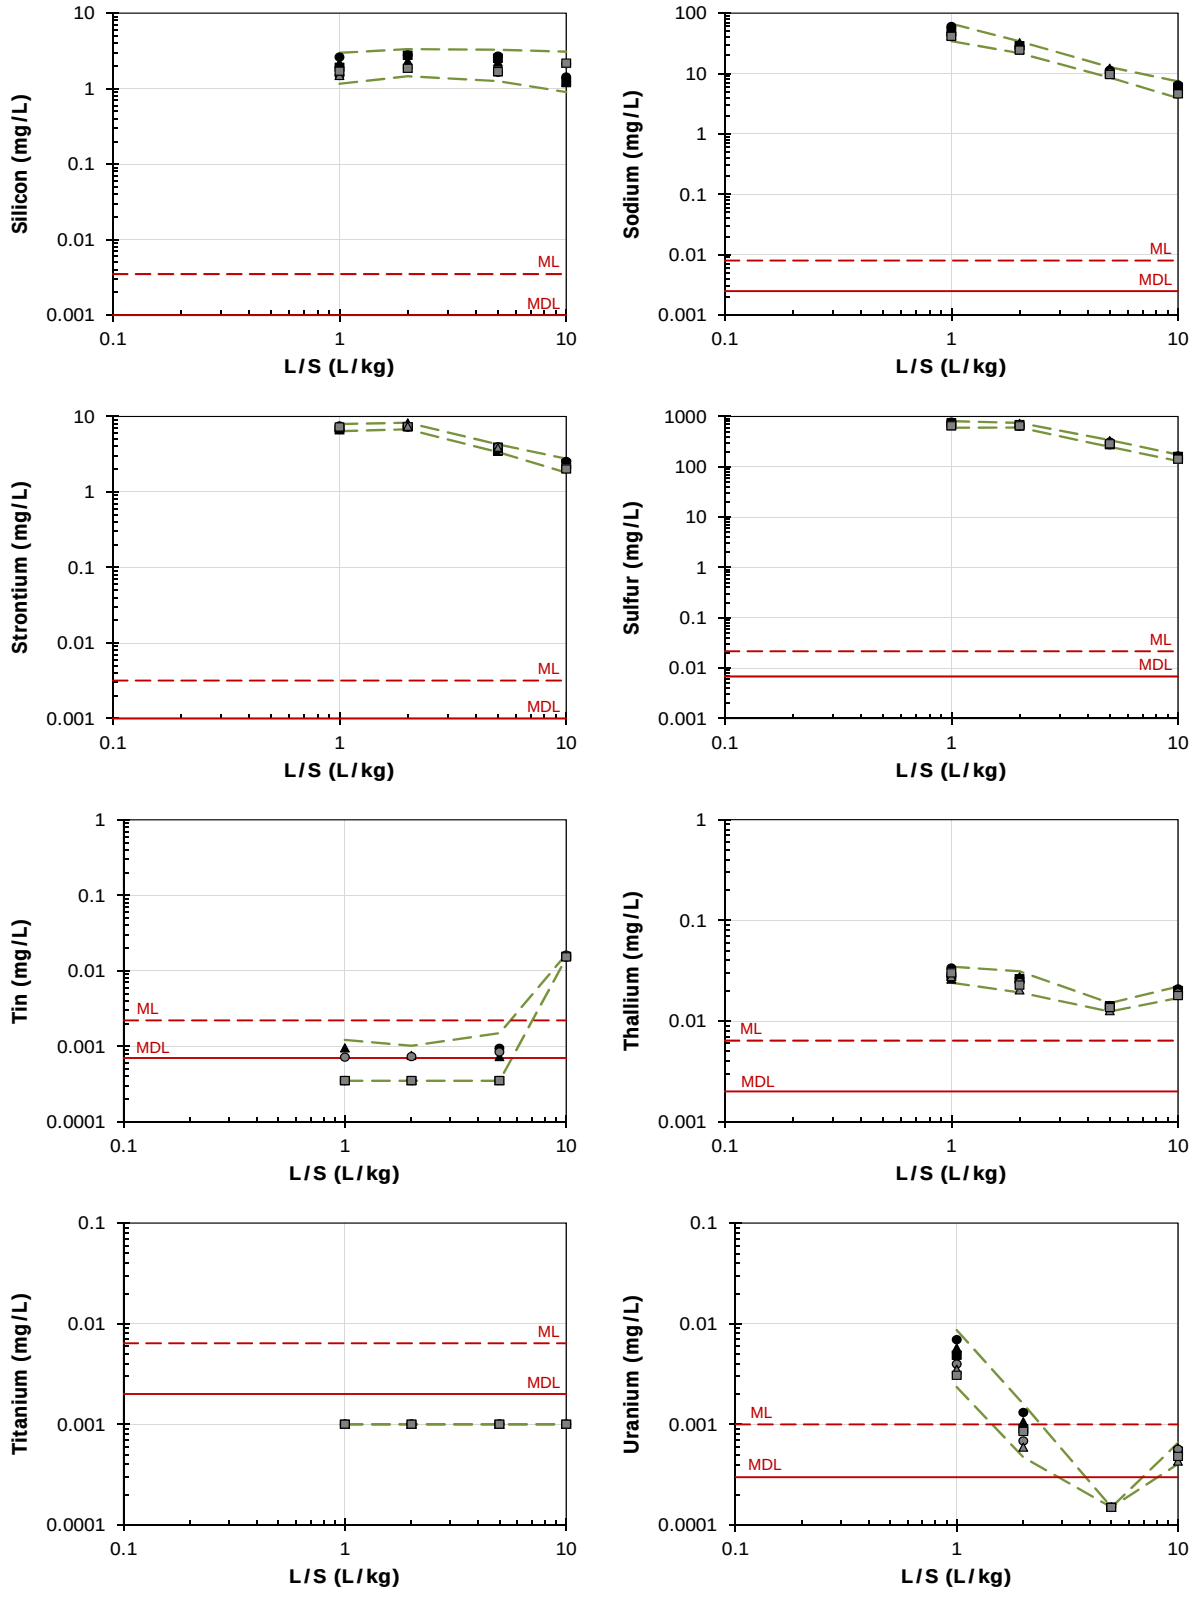

Figure 34. Reference lab data and 95% prediction limits for Method 1316 Phase I EaFA material.

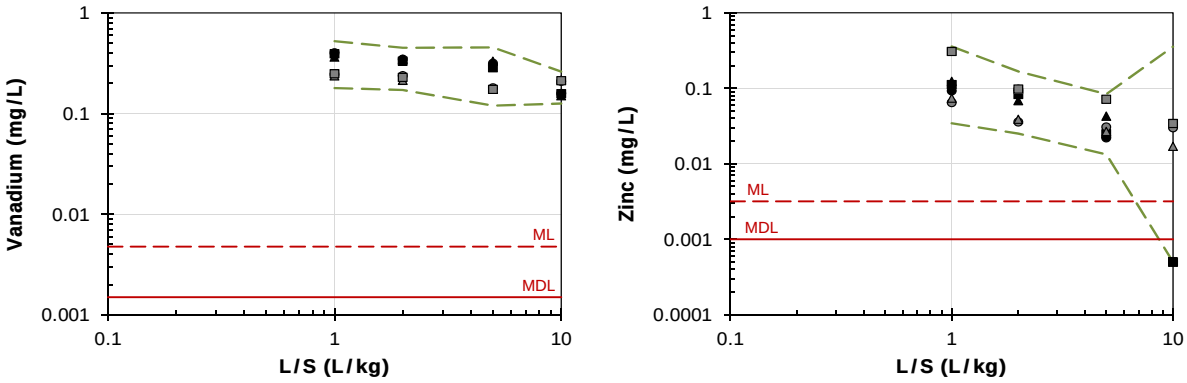

Figure 35. Reference lab data and 95% prediction limits for Method 1316 Phase I EaFA material.

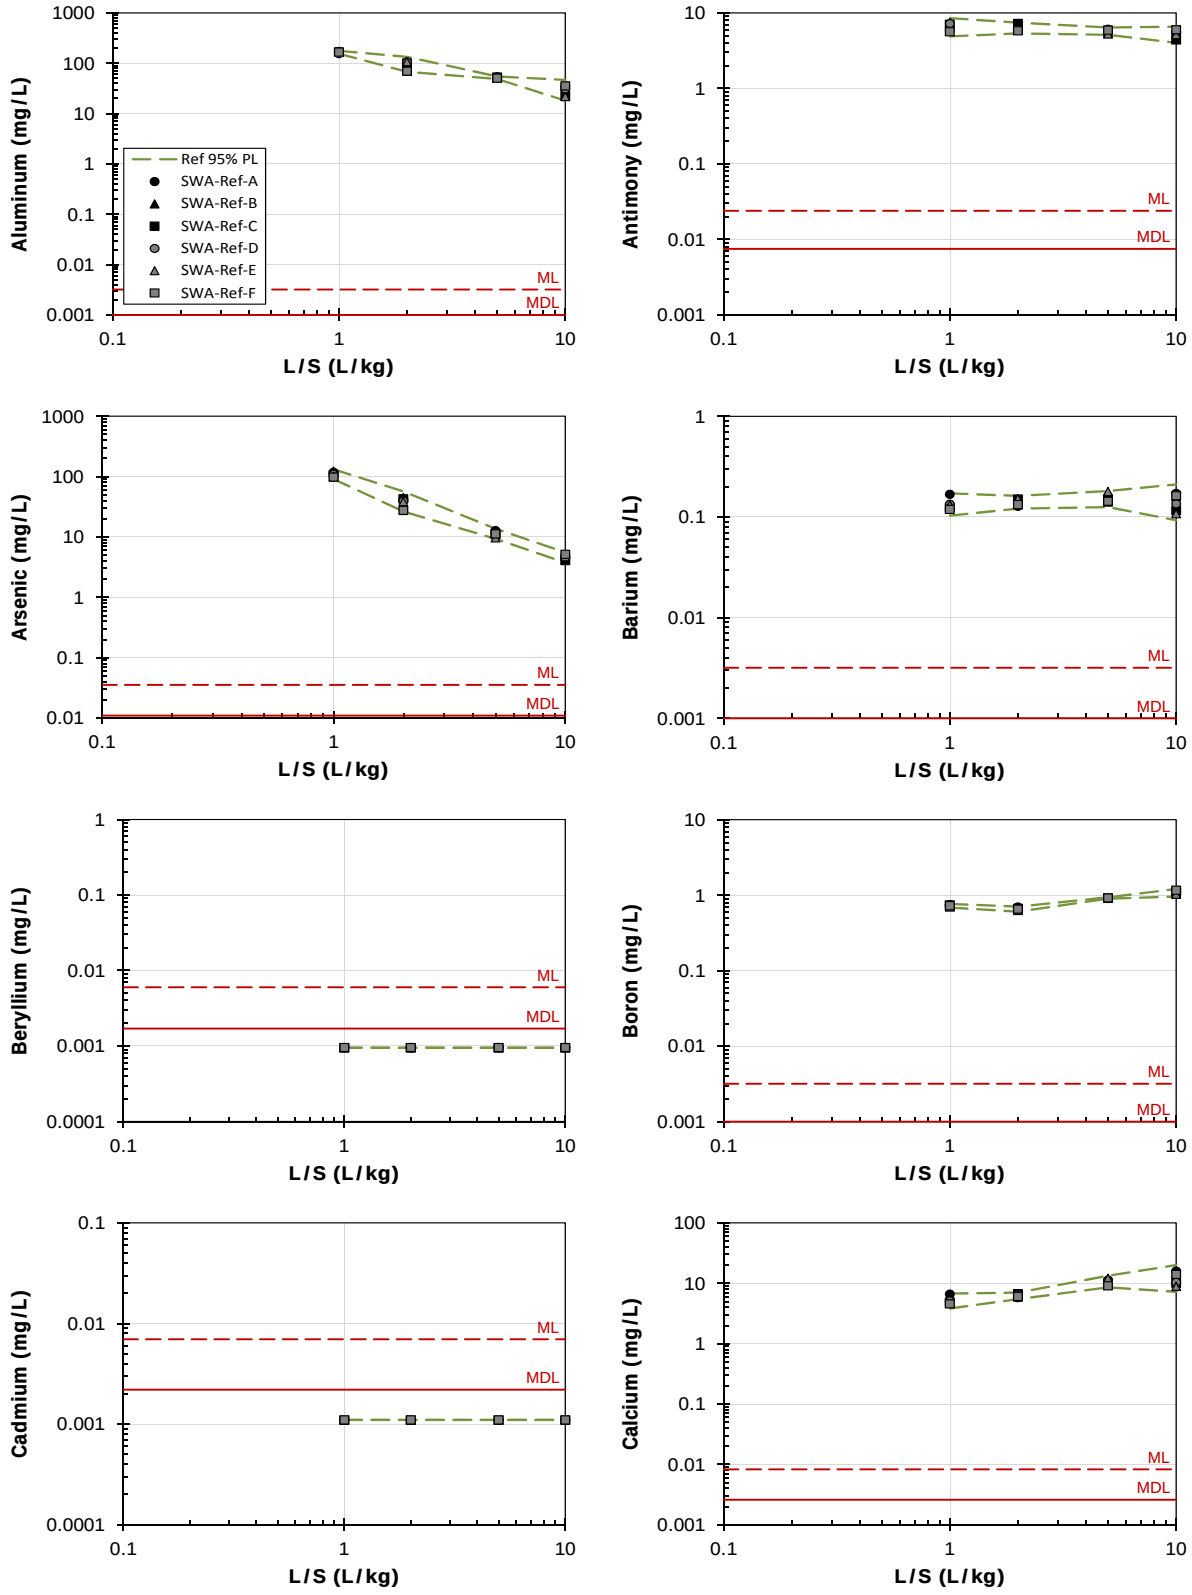

Figure 36. Reference lab data and 95% prediction limits for Method 1316 Phase II SWA material.

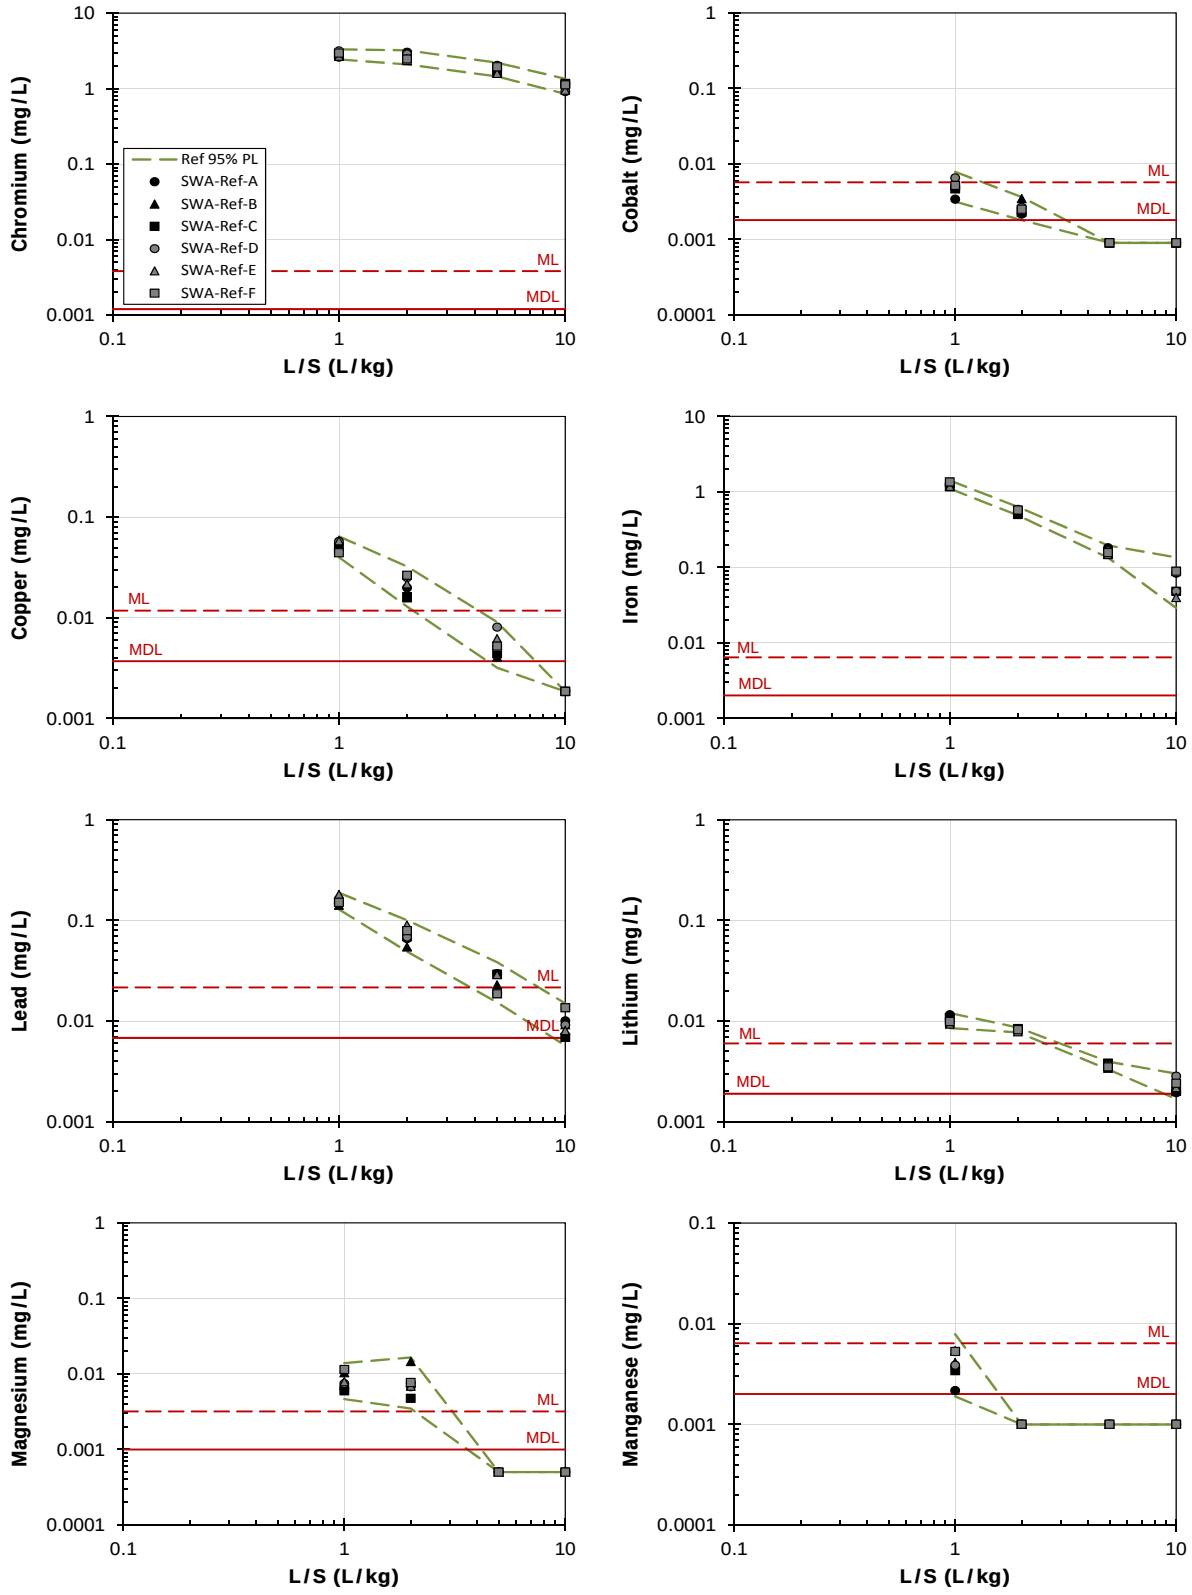

Figure 37. Reference lab data and 95% prediction limits for Method 1316 Phase II SWA material.

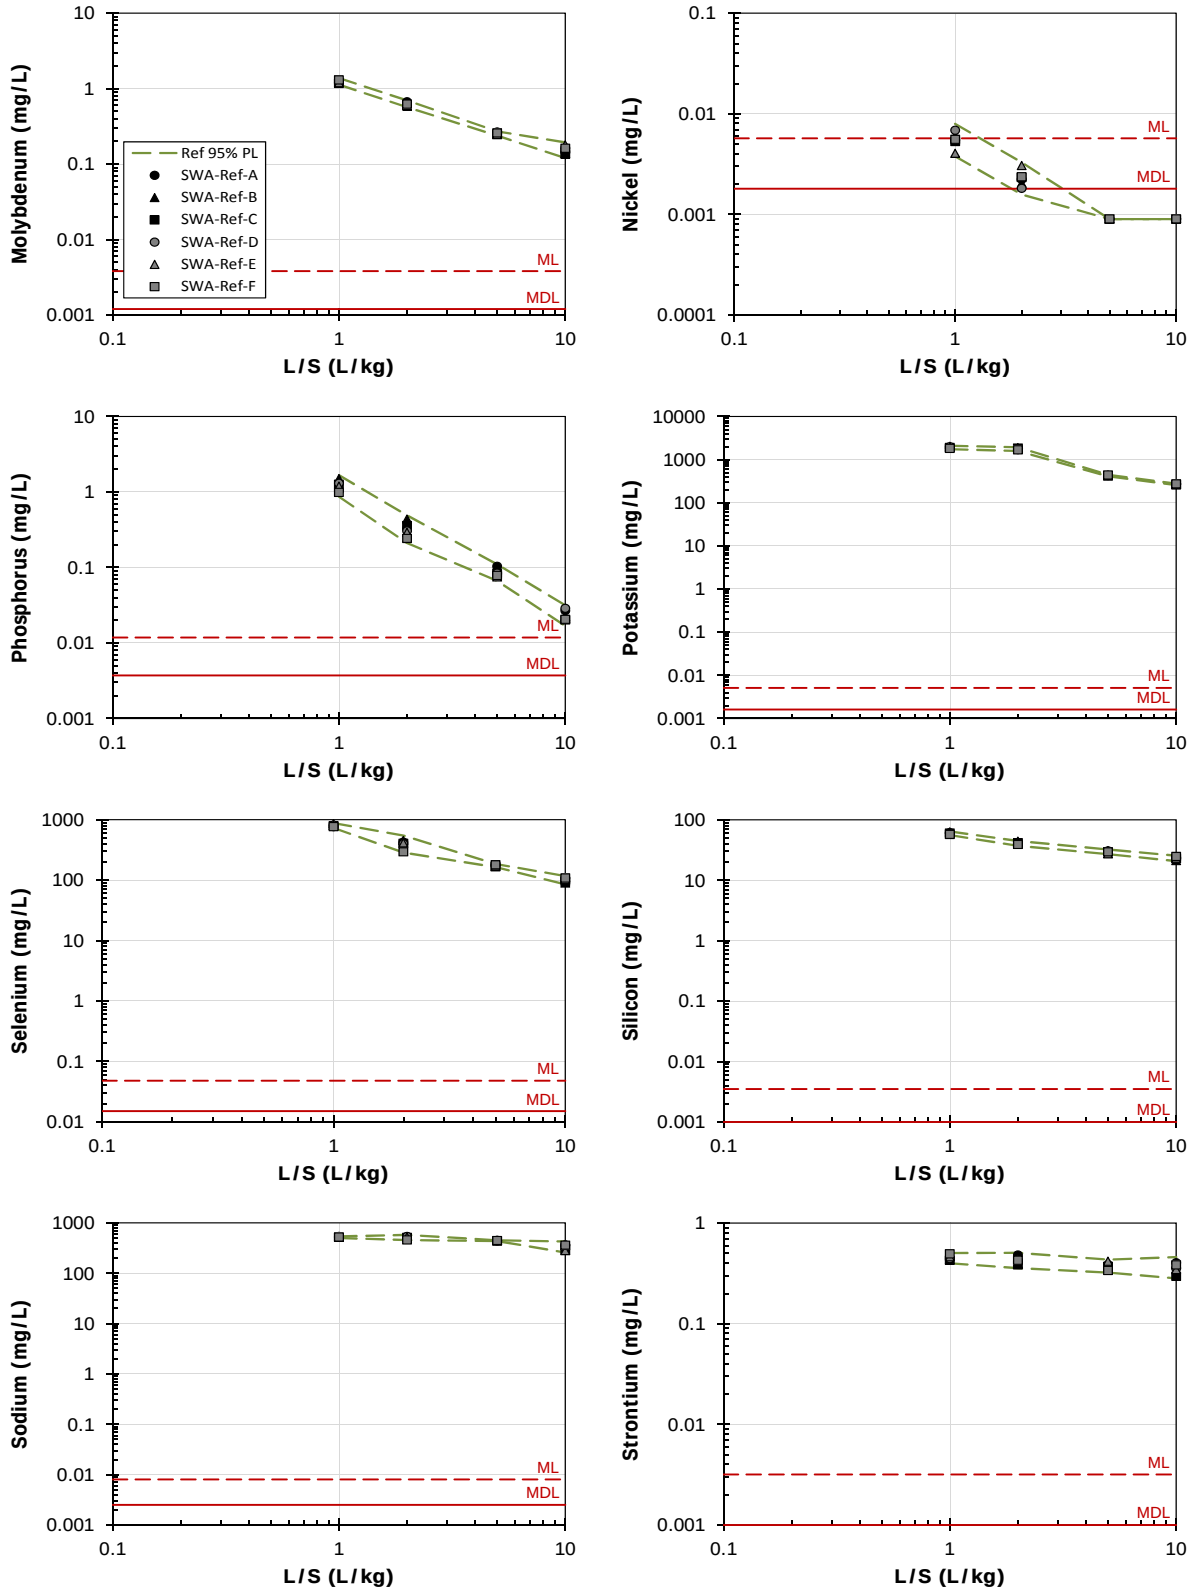

Figure 38. Reference lab data and 95% prediction limits for Method 1316 Phase II SWA material.

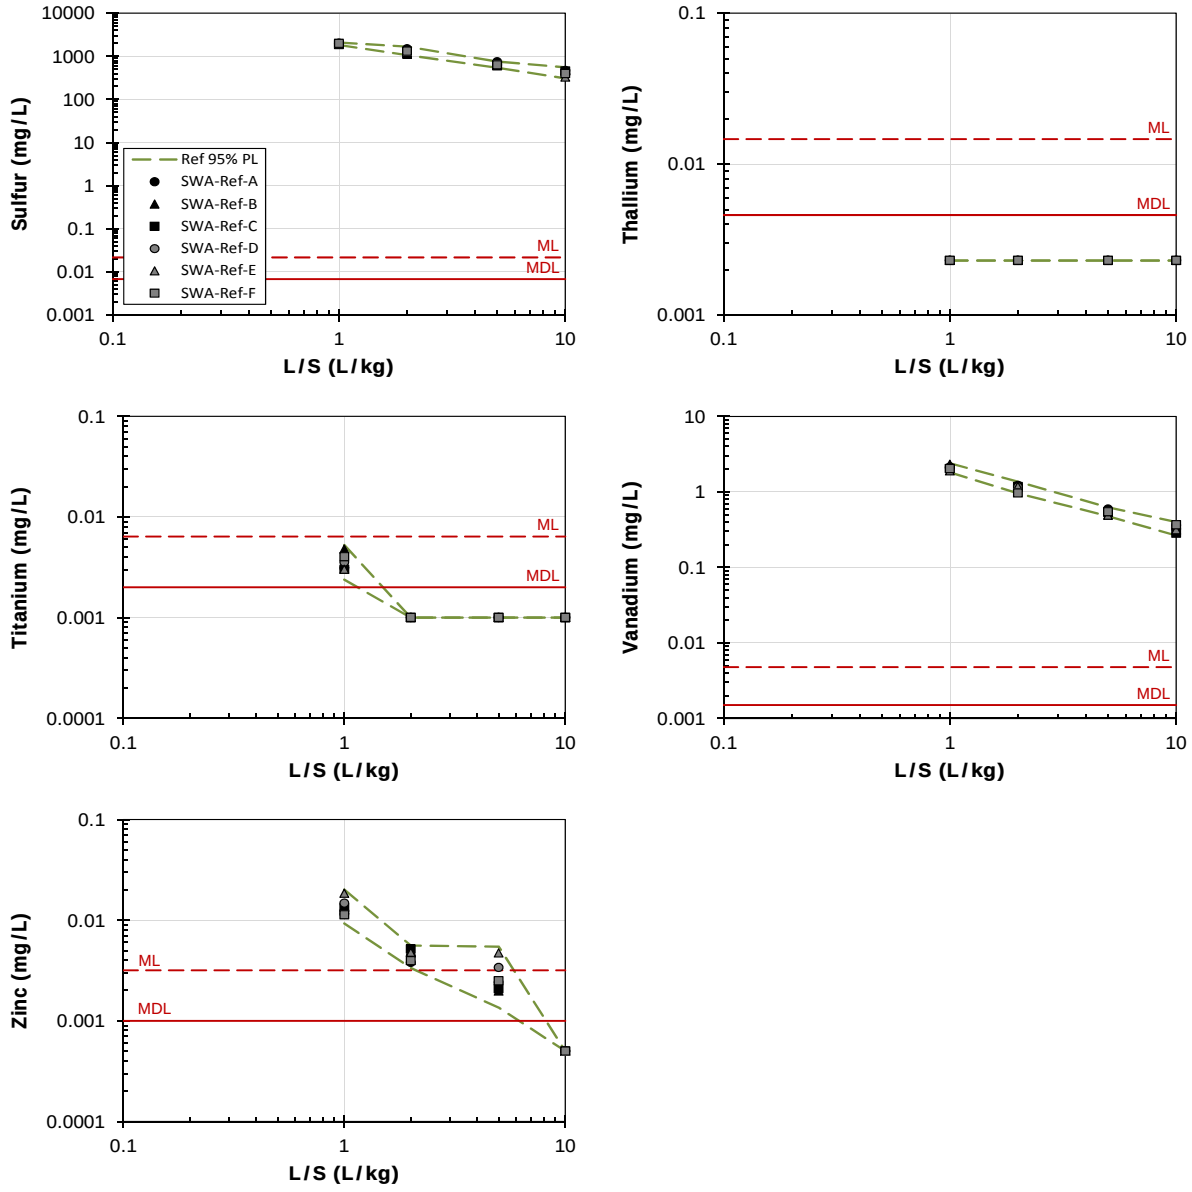

Figure 39. Reference lab data and 95% prediction limits for Method 1316 Phase II SWA material.

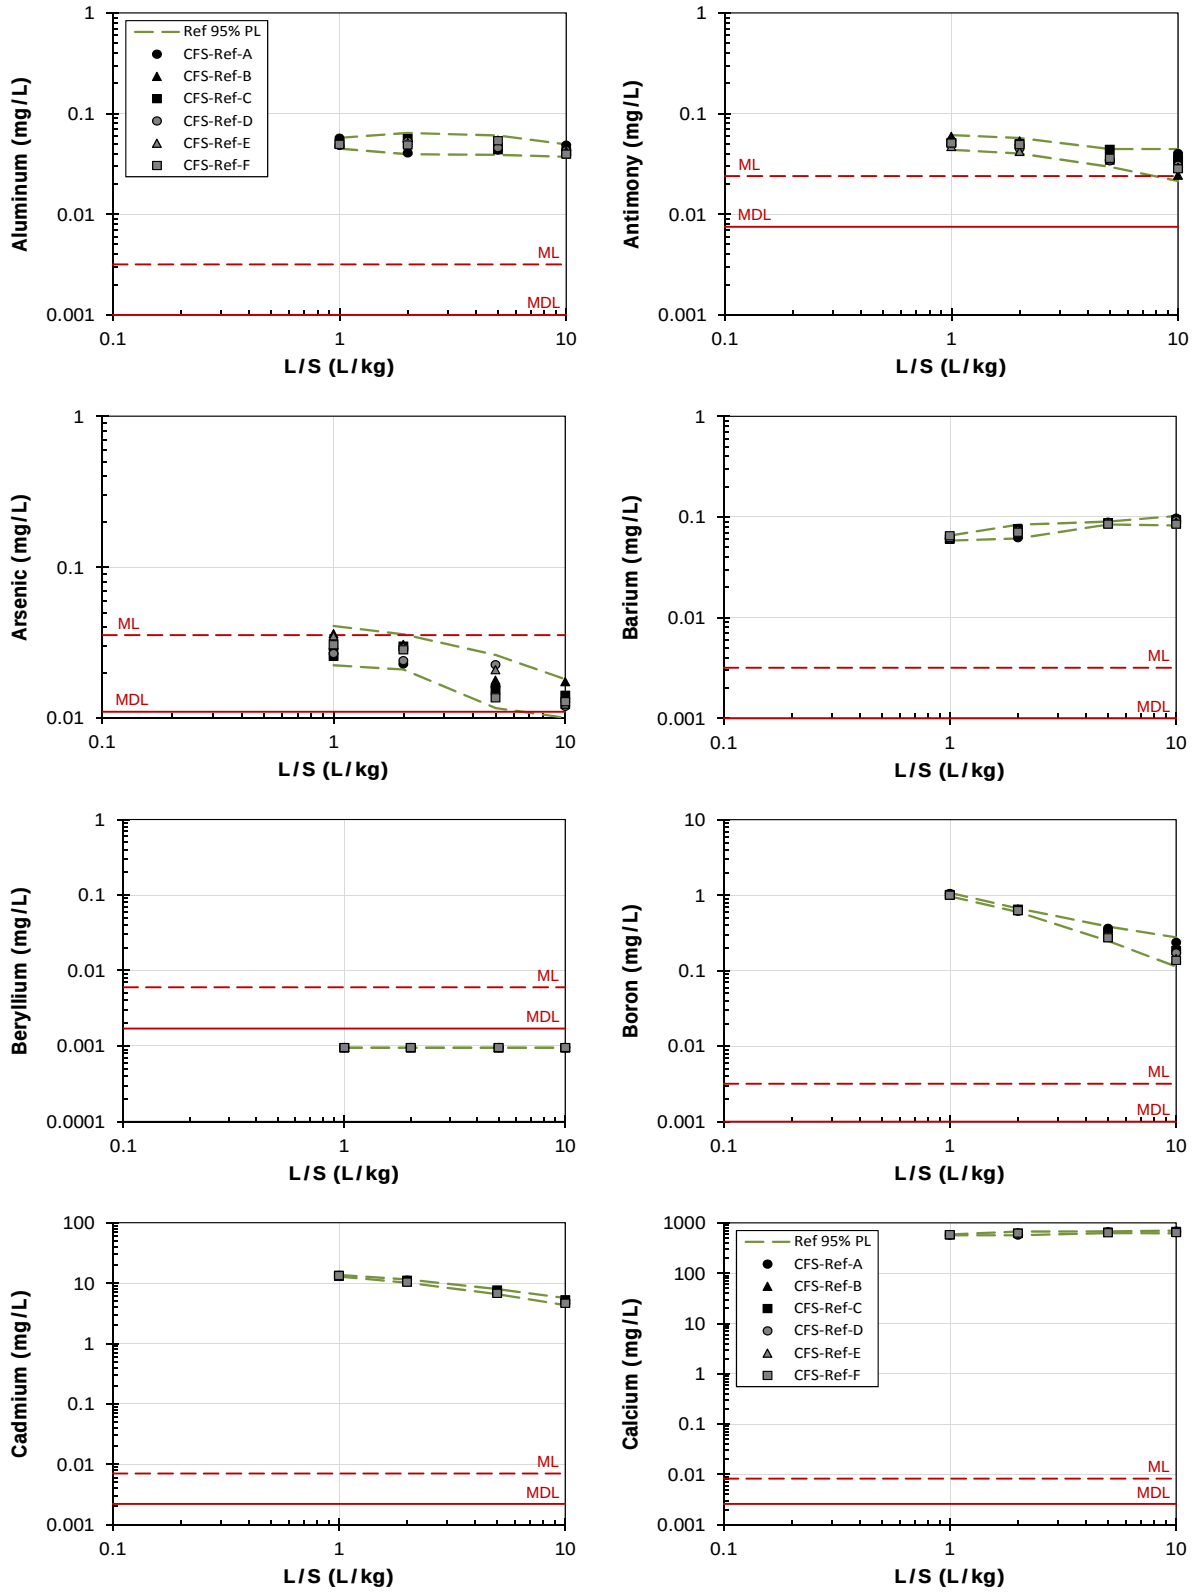

Figure 40. Reference lab data and 95% prediction limits for Method 1316 Phase II CFS material.

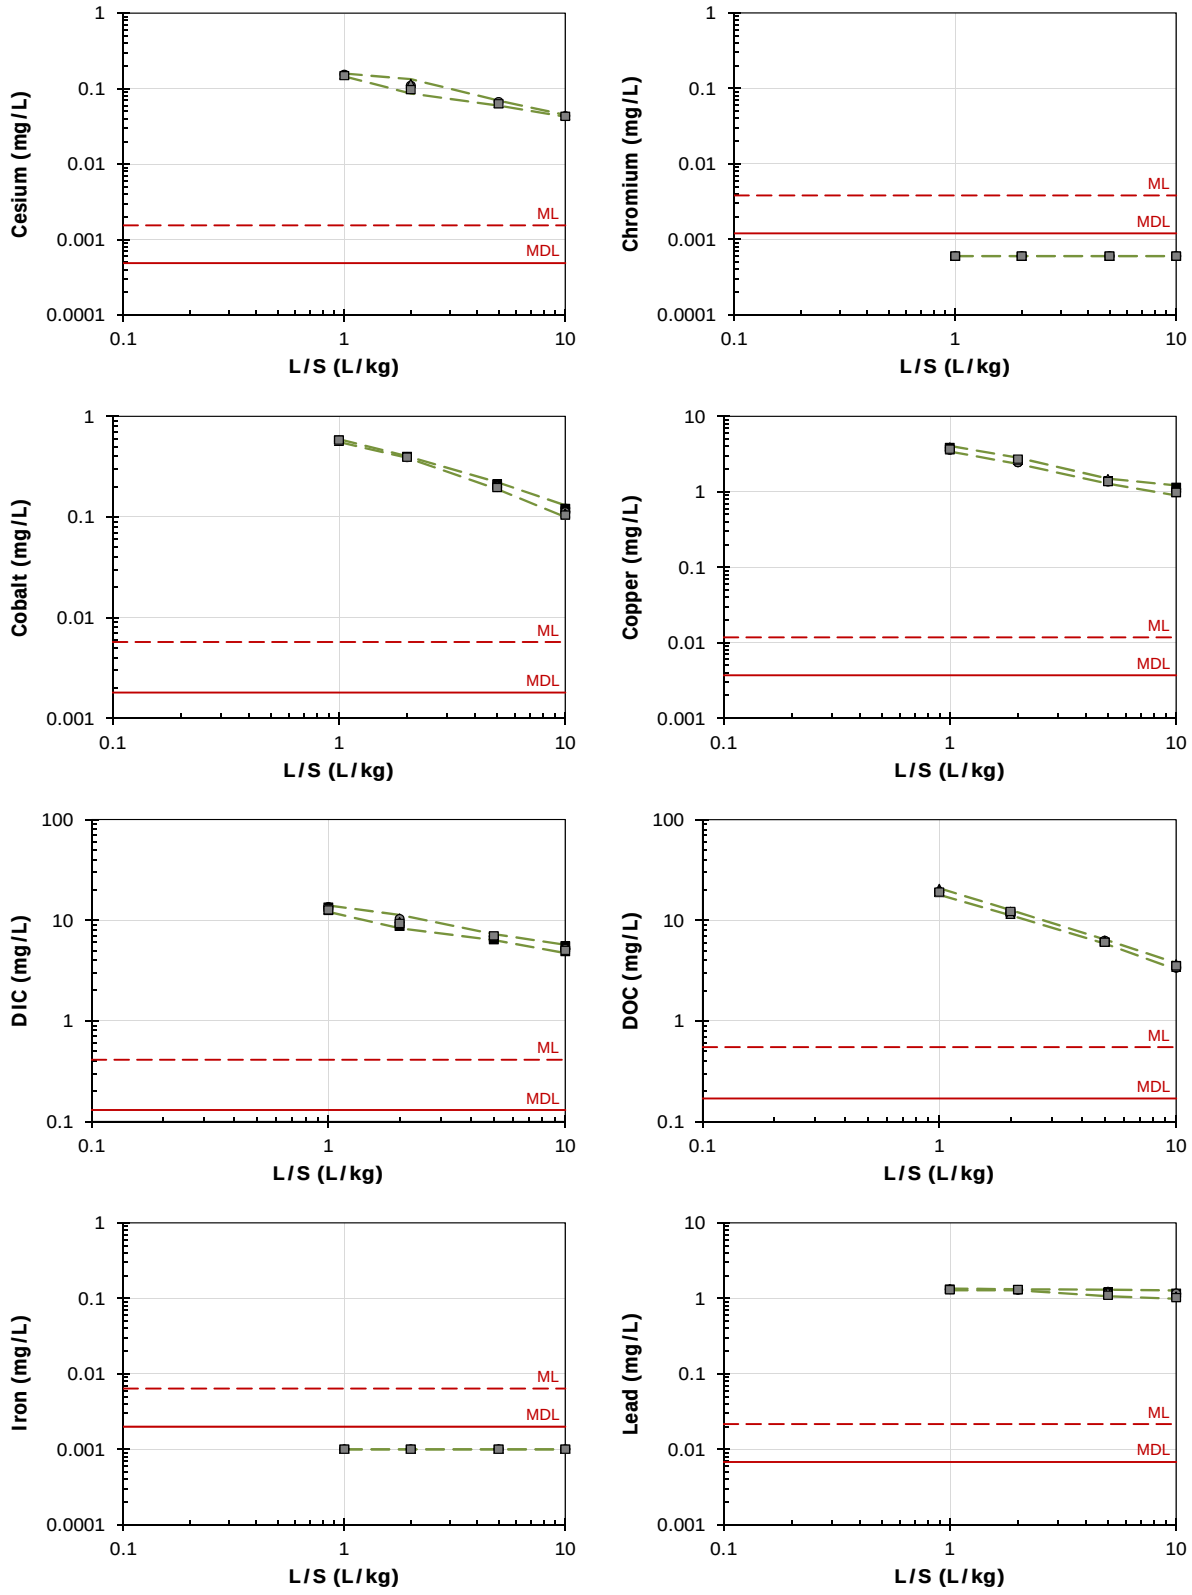

Figure 41. Reference lab data and 95% prediction limits for Method 1316 Phase II CFS material.

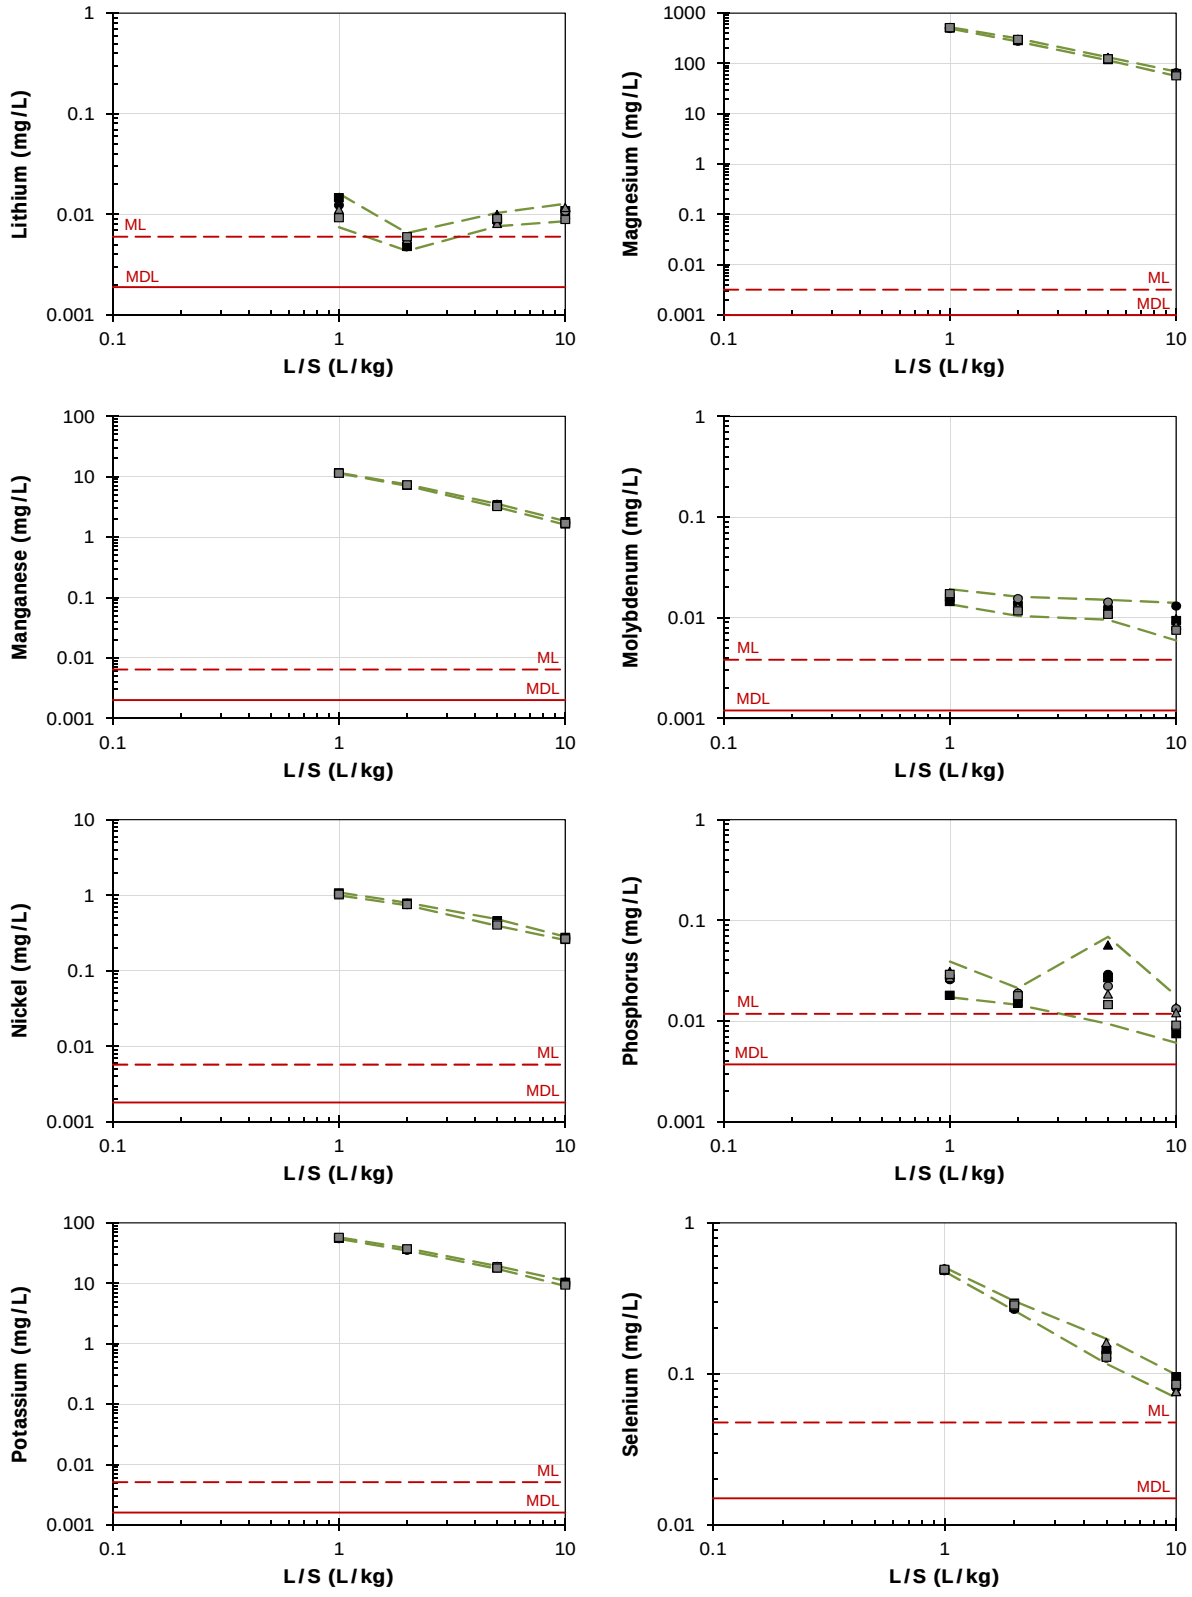

Figure 42. Reference lab data and 95% prediction limits for Method 1316 Phase II CFS material.

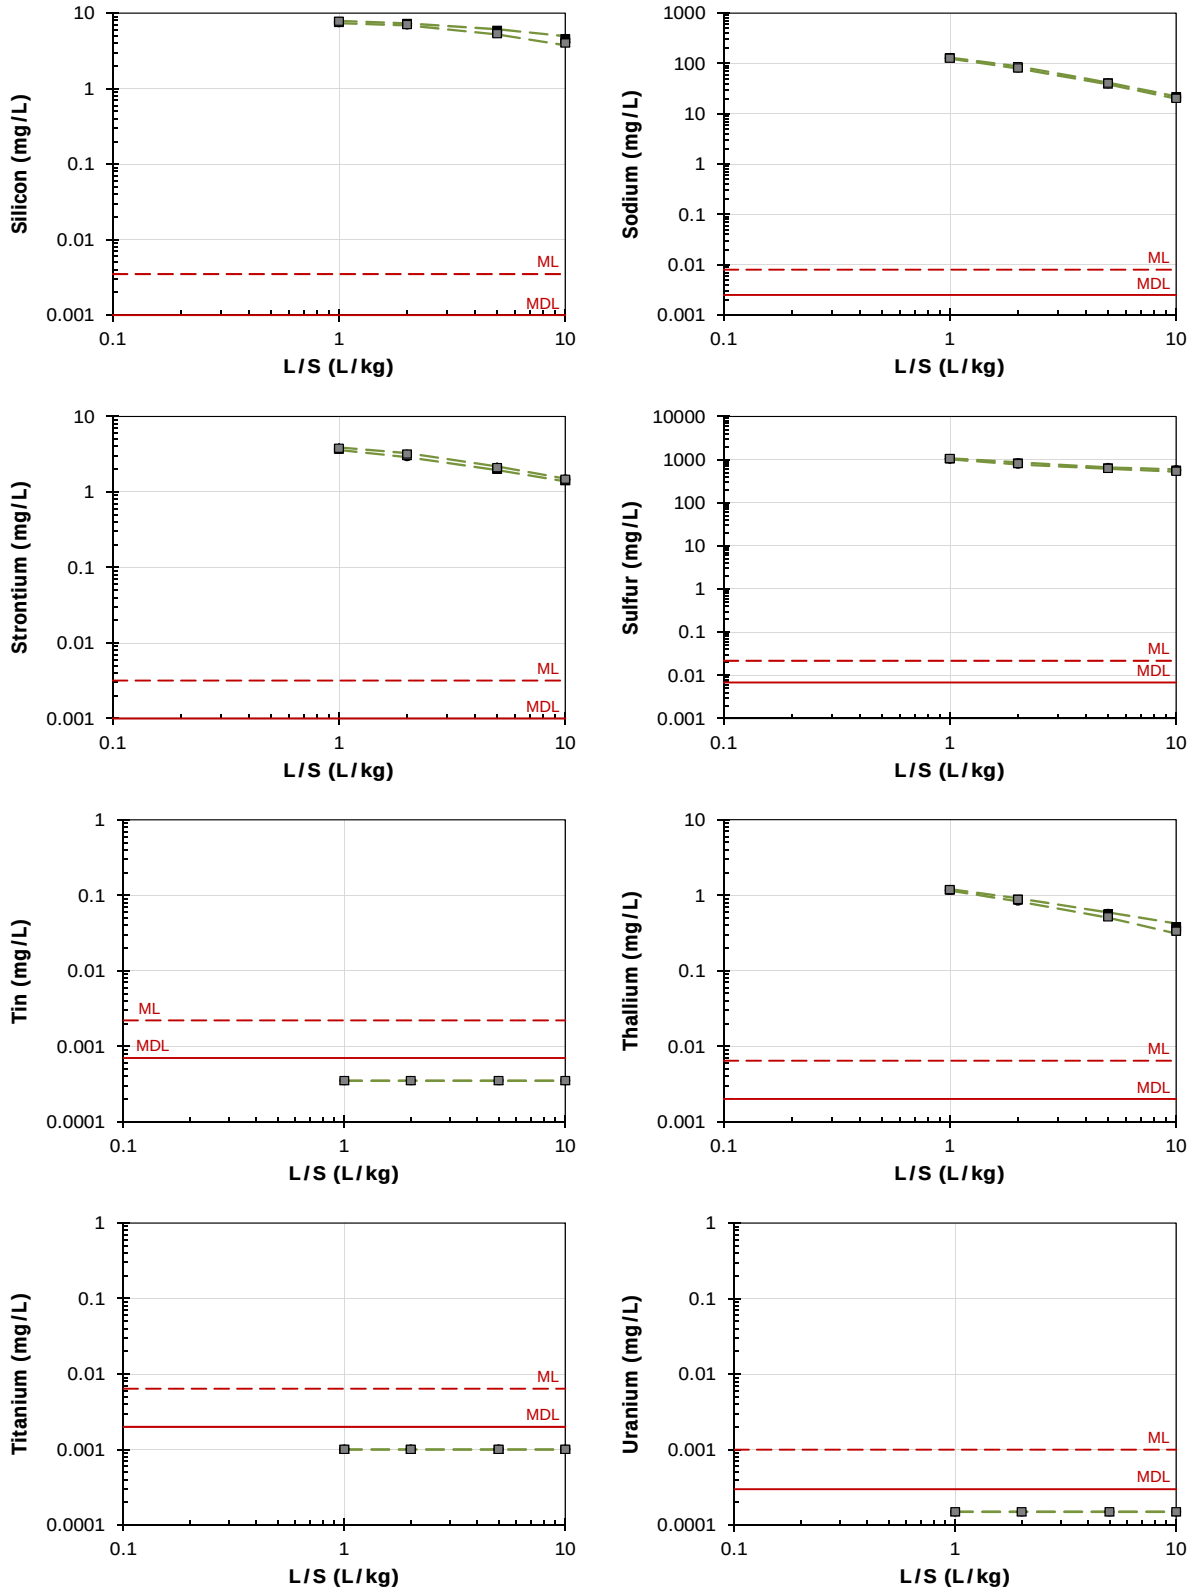

Figure 43. Reference lab data and 95% prediction limits for Method 1316 Phase II CFS material.

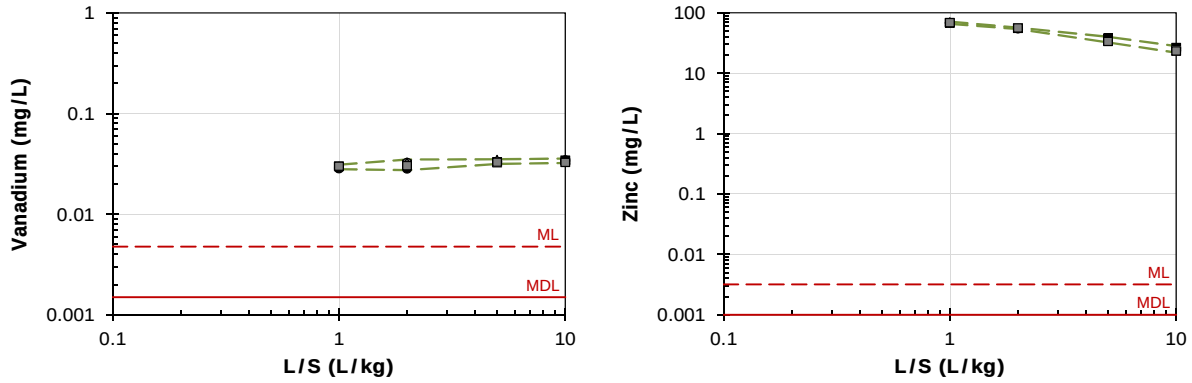

Figure 44. Reference lab data and 95% prediction limits for Method 1316 Phase II CFS material.

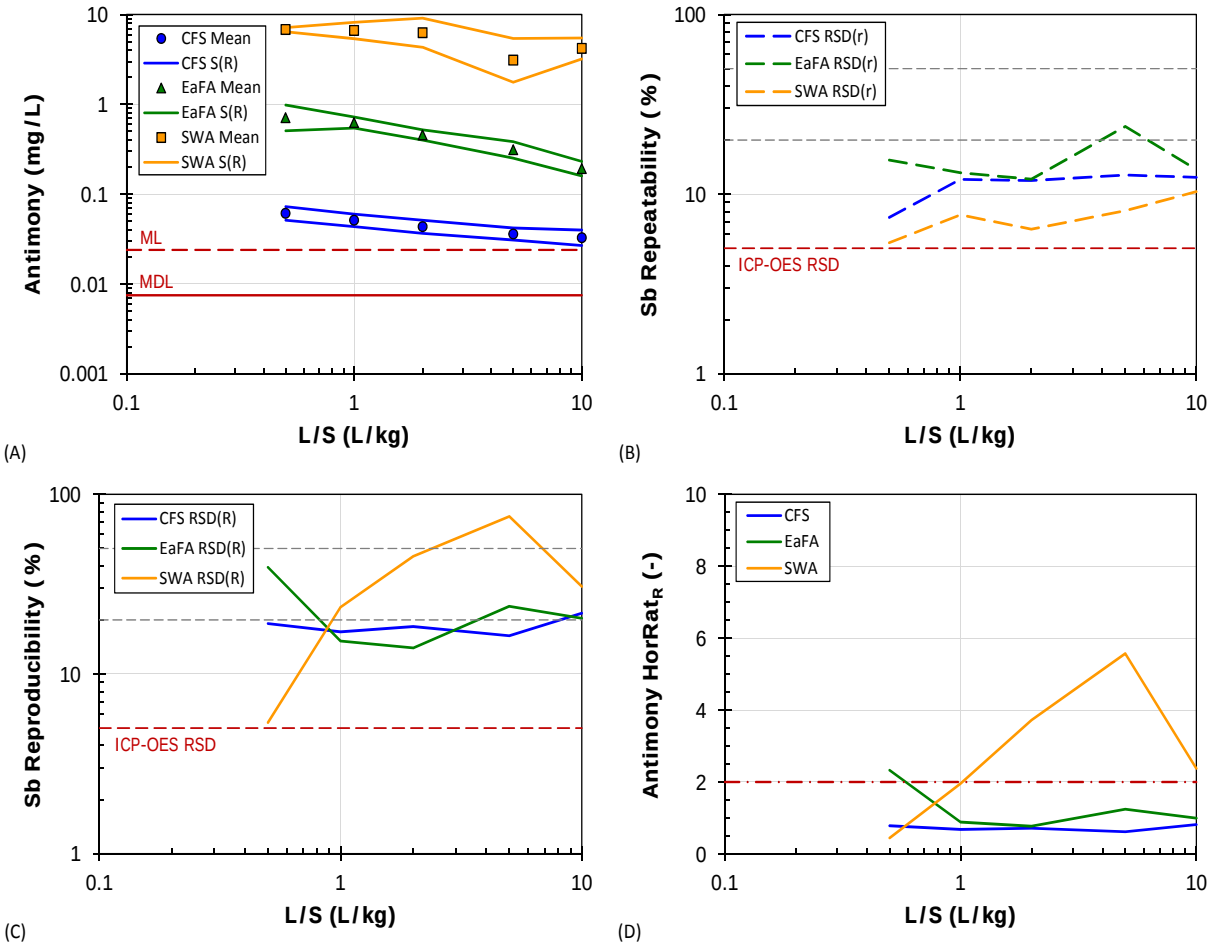

Figure 45. Antimony repeatability and reproducibility in Method 1316 materials: (A) reproducibility standard deviation interval about the mean of all data, (B) repeatability relative standard deviation (RSD_r) compared to approximate analytical uncertainty (ICP-OES RSD), (B) reproducibility relative standard deviation (RSD_R) compared to approximate analytical uncertainty (ICP-OES RSD), and (D) reproducibility Horwitz ratio ($HorRat_R$).

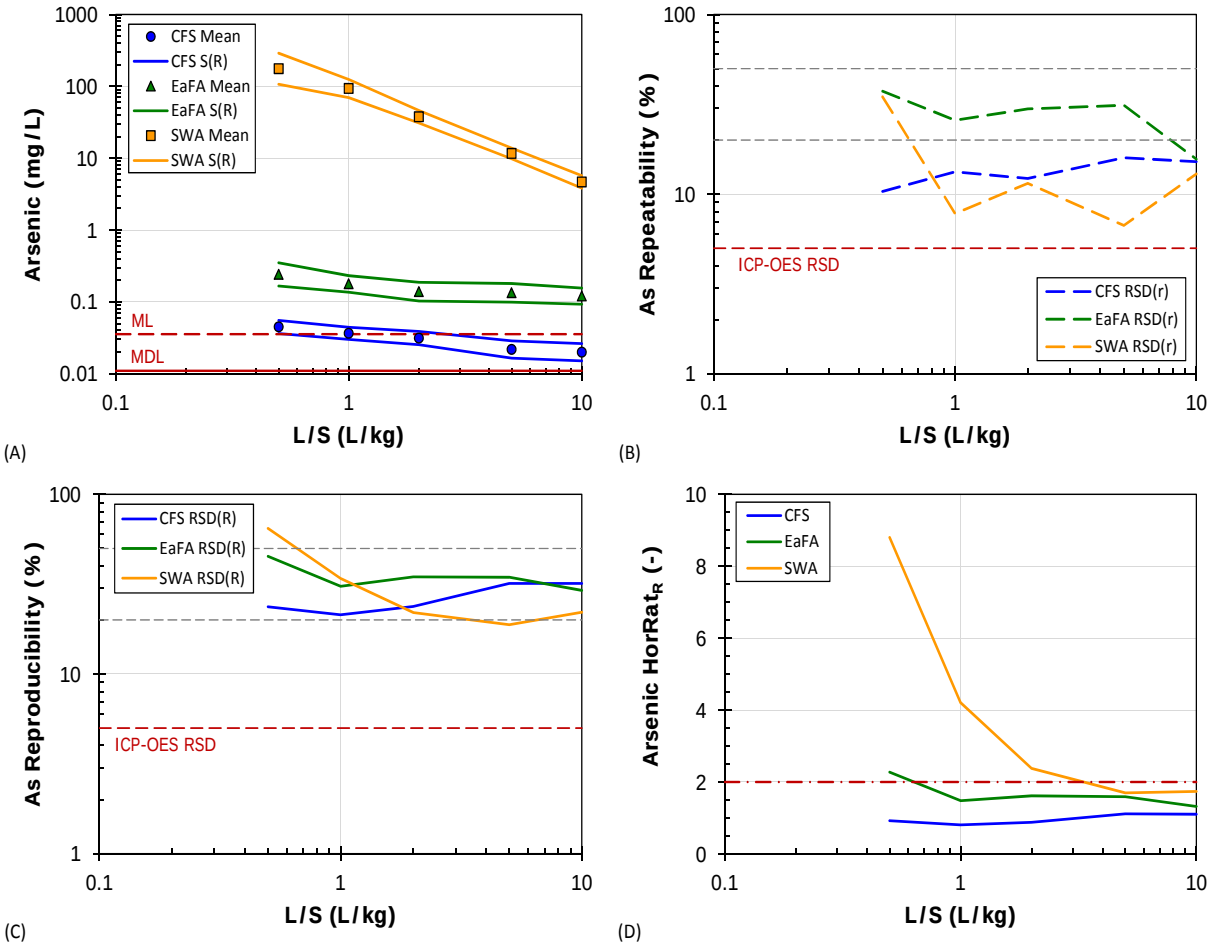

Figure 46. Arsenic repeatability and reproducibility in Method 1316 materials: (A) reproducibility standard deviation interval about the mean of all data, (B) repeatability relative standard deviation (RSD_r) compared to approximate analytical uncertainty (ICP-OES RSD), (B) reproducibility relative standard deviation (RSD_R) compared to approximate analytical uncertainty (ICP-OES RSD), and (D) reproducibility Horwitz ratio ($HorRat_R$).

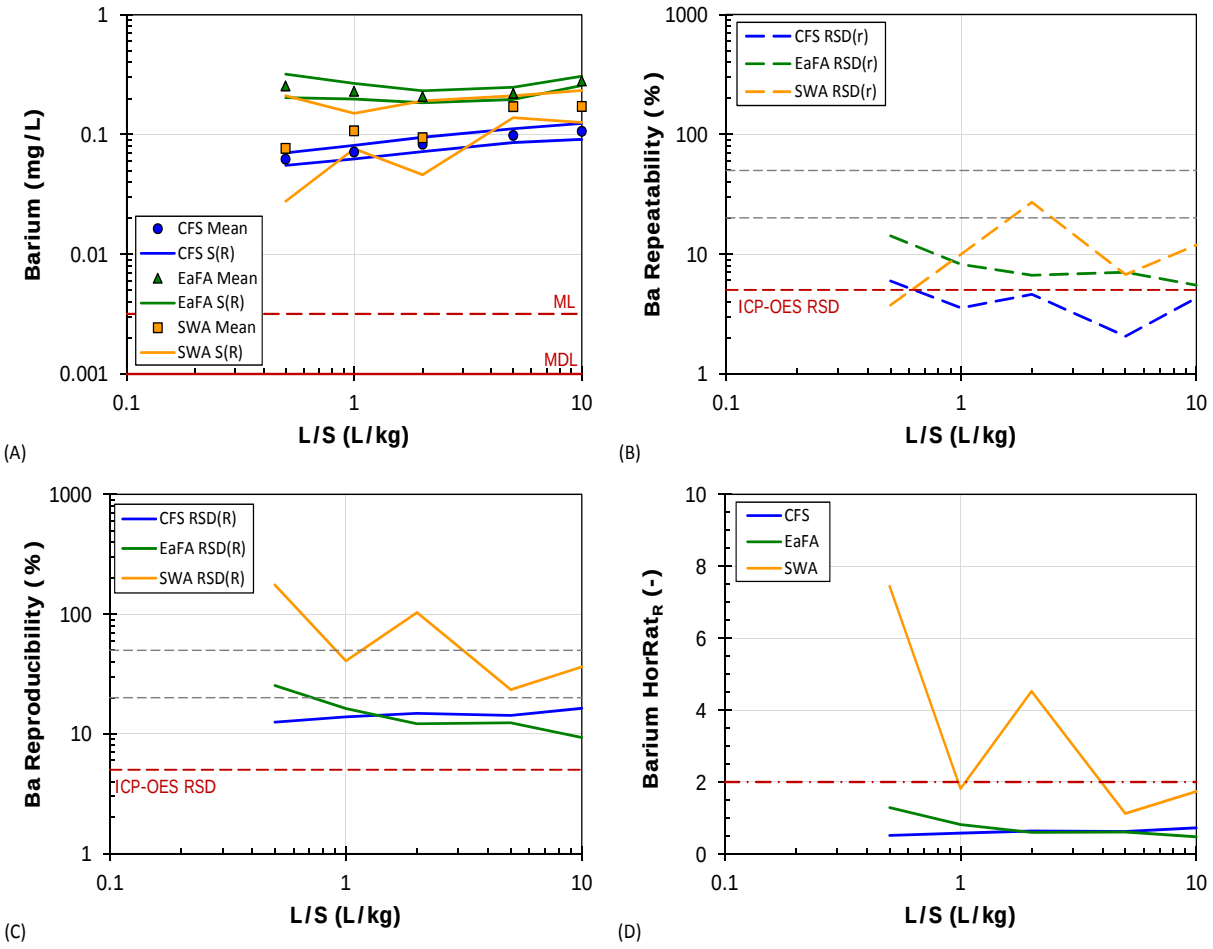

Figure 47. Barium repeatability and reproducibility in Method 1316 materials: (A) reproducibility standard deviation interval about the mean of all data, (B) repeatability relative standard deviation (RSD_r) compared to approximate analytical uncertainty (ICP-OES RSD), (B) reproducibility relative standard deviation (RSD_R) compared to approximate analytical uncertainty (ICP-OES RSD), and (D) reproducibility Horwitz ratio ($HorRat_R$).

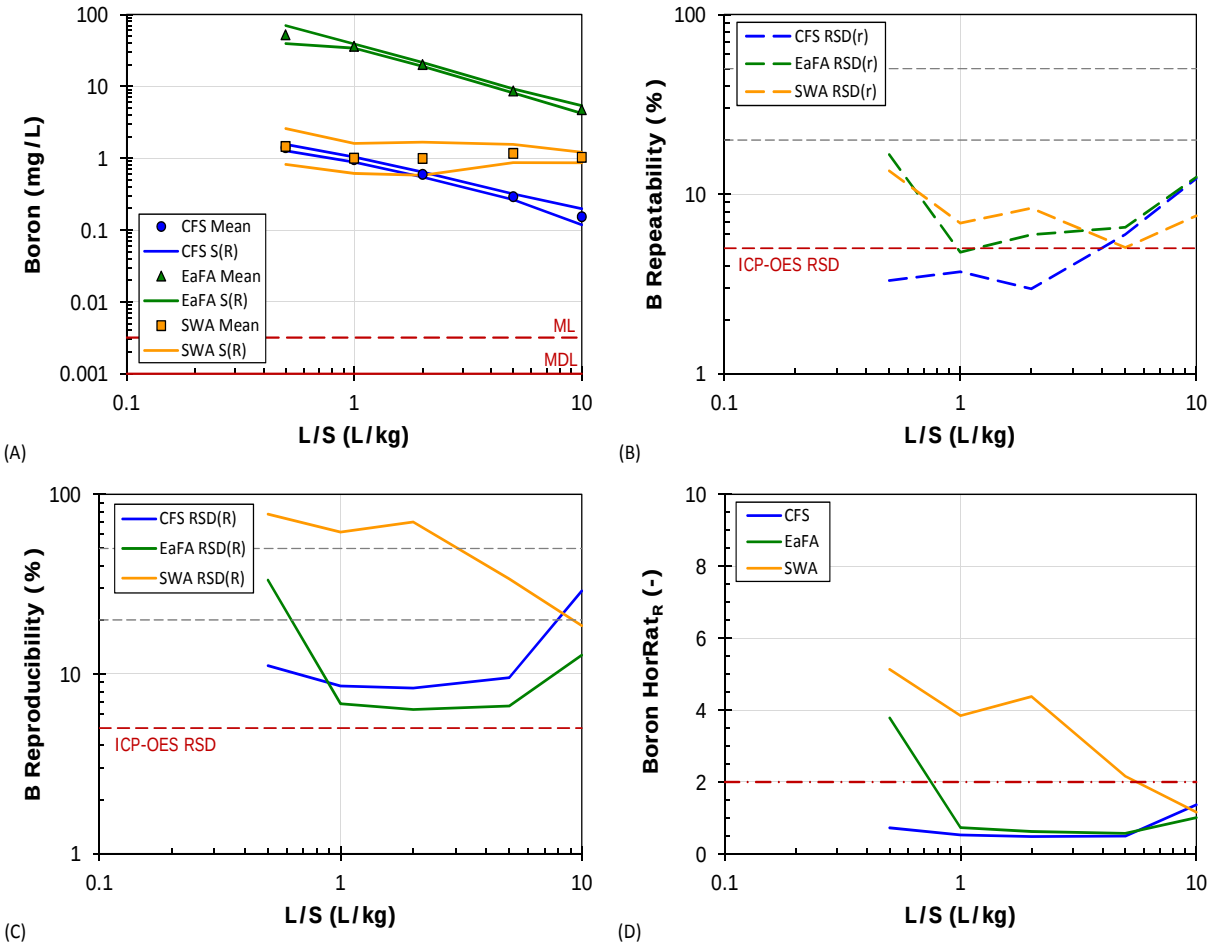

Figure 48. Boron repeatability and reproducibility in Method 1316 materials: (A) reproducibility standard deviation interval about the mean of all data, (B) repeatability relative standard deviation (RSD_r) compared to approximate analytical uncertainty (ICP-OES RSD), (B) reproducibility relative standard deviation (RSD_R) compared to approximate analytical uncertainty (ICP-OES RSD), and (D) reproducibility Horwitz ratio ($HorRat_R$).

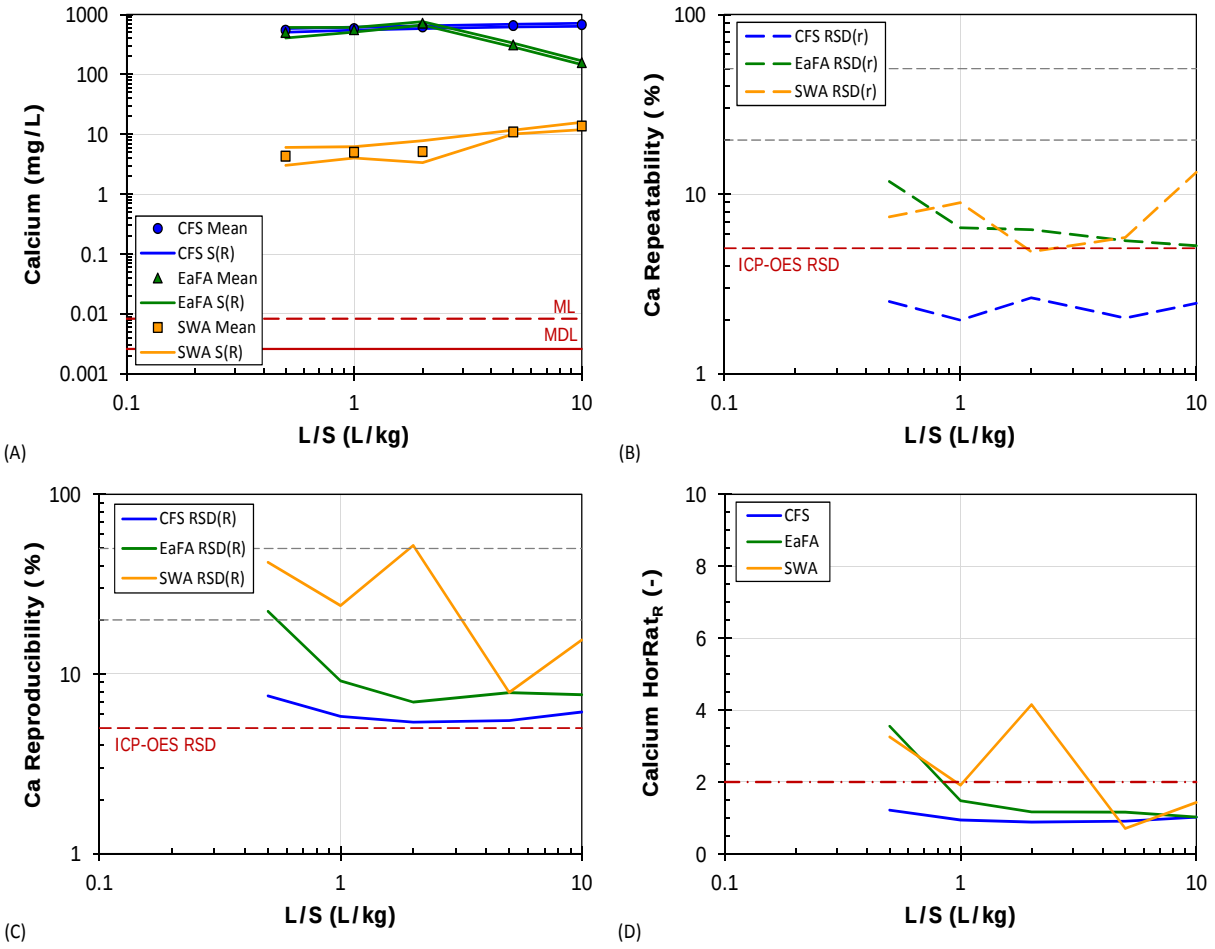

Figure 49. Calcium repeatability and reproducibility in Method 1316 materials: (A) reproducibility standard deviation interval about the mean of all data, (B) repeatability relative standard deviation (RSD_r) compared to approximate analytical uncertainty (ICP-OES RSD), (B) reproducibility relative standard deviation (RSD_R) compared to approximate analytical uncertainty (ICP-OES RSD), and (D) reproducibility Horwitz ratio ($HorRat_R$).

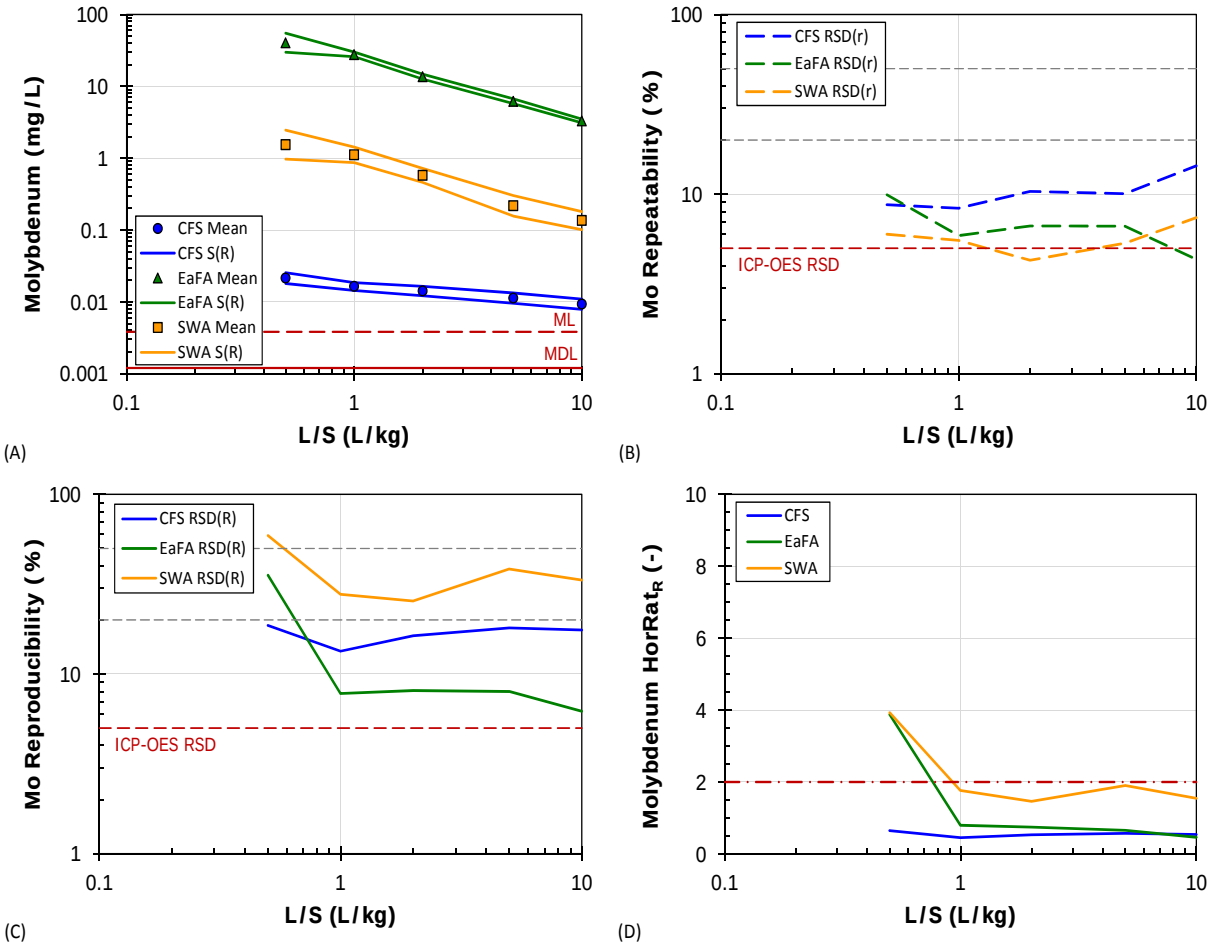

Figure 50. Molybdenum repeatability and reproducibility in Method 1316 materials: (A) reproducibility standard deviation interval about the mean of all data, (B) repeatability relative standard deviation (RSD_r) compared to approximate analytical uncertainty (ICP-OES RSD), (B) reproducibility relative standard deviation (RSD_R) compared to approximate analytical uncertainty (ICP-OES RSD), and (D) reproducibility Horwitz ratio ($HorRat_R$).

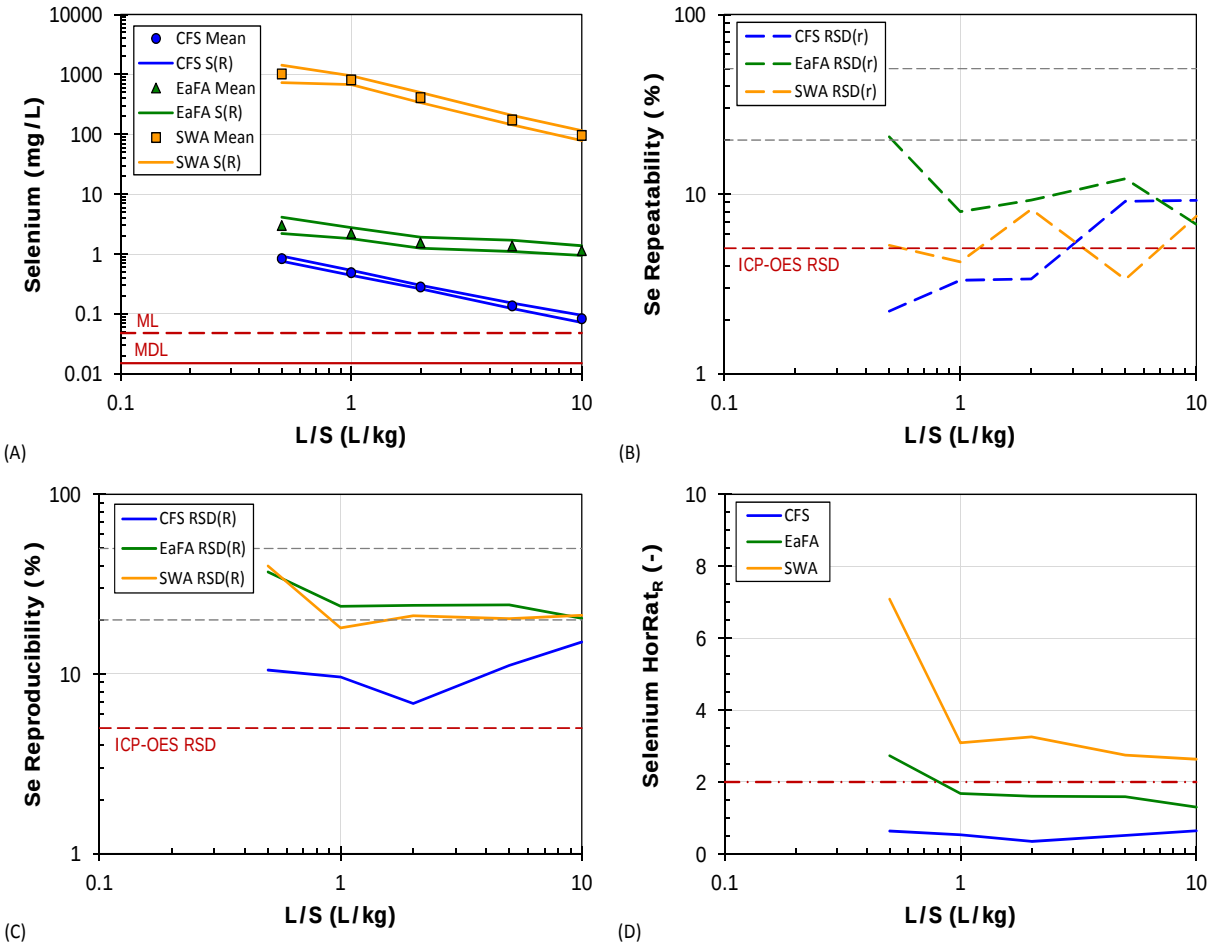

Figure 51. Selenium repeatability and reproducibility in Method 1316 materials: (A) reproducibility standard deviation interval about the mean of all data, (B) repeatability relative standard deviation (RSD_r) compared to approximate analytical uncertainty (ICP-OES RSD), (B) reproducibility relative standard deviation (RSD_R) compared to approximate analytical uncertainty (ICP-OES RSD), and (D) reproducibility Horwitz ratio ($HorRat_R$).

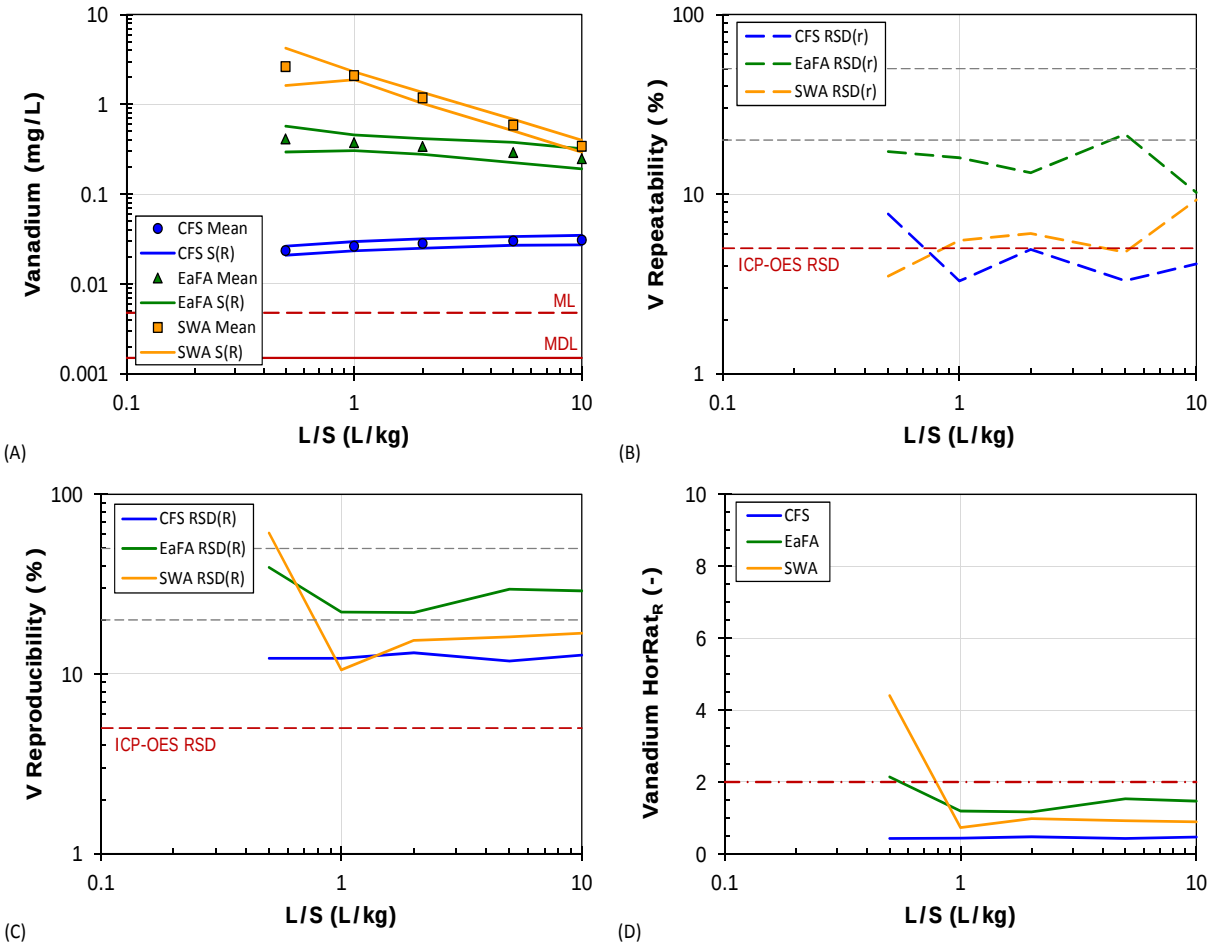

Figure 52. Vanadium repeatability and reproducibility in Method 1316 materials: (A) reproducibility standard deviation interval about the mean of all data, (B) repeatability relative standard deviation (RSD_r) compared to approximate analytical uncertainty (ICP-OES RSD), (B) reproducibility relative standard deviation (RSD_R) compared to approximate analytical uncertainty (ICP-OES RSD), and (D) reproducibility Horwitz ratio ($HorRat_R$).

Table 1. Method 1316 Repeatability (RSD_r) for Common Analytes in All Study Materials

		RSD_r Distribution Percentiles (%)					
Analyte	Symbol	Mean	Min	25th	Median	75th	Max
Antimony	Sb	12	5	8	12	13	24
Arsenic	As	19	7	12	15	28	37
Barium	Ba	8	2	4	7	9	27
Boron	B	8	3	5	7	10	17
Calcium	Ca	6	2	3	6	7	13
Molybdenum	Mo	8	4	6	7	9	14
Selenium	Se	8	2	4	8	9	21
Vanadium	V	9	3	4	6	12	22

Table 2. Method 1316 Reproducibility (RSD_R) for Common Analytes in All Study Materials

		RSD_R Distribution Percentiles (%)					
Analyte	Symbol	Mean	Min	25th	Median	75th	Max
Antimony	Sb	26	5	17	20	27	75
Arsenic	As	31	19	23	31	34	65
Barium	Ba	35	9	13	16	31	175
Boron	B	26	6	8	13	34	78
Calcium	Ca	15	5	7	8	19	52
Molybdenum	Mo	22	6	11	18	31	59
Selenium	Se	20	7	13	20	24	40
Vanadium	V	22	11	12	16	26	61

Table 3. Method 1316 Repeatability (RSD_r) by L/S Target (mL/g-dry)

	RSD_r Distribution Percentiles (%)					
L/S	Mean	Min	25th	Median	75th	Max
0.5	11	2	5	8	15	37
1.0	8	2	5	7	9	26
2.0	8	3	5	7	12	30
5.0	9	2	5	7	11	31
10.0	10	2	6	10	13	16

Table 4. Method 1316 Reproducibility (RSD_R) by L/S Target (mL/g-dry)

	RSD_R Distribution Percentiles (%)					
L/S	Mean	Min	25th	Median	75th	Max
0.5	38	5	17	34	43	175
1.0	20	6	10	17	24	62
2.0	25	5	11	17	24	103
5.0	21	6	11	17	26	75
10.0	20	6	14	20	29	36

Table 5. Method 1316 Repeatability (RSD_r) by Study Material

	RSD_r Distribution Percentiles (%)					
Material	Mean	Min	25th	Median	75th	Max
EaFA	13	4	7	11	16	37
SWA	8	3	5	7	9	35
CFS	7	2	3	6	11	16

Table 6. Method 1316 Reproducibility (RSD_R) by Study Material

	RSD_R Distribution Percentiles (%)					
Material	Mean	Min	25th	Median	75th	Max
EaFA	20	6	9	21	29	45
SWA	39	5	20	29	47	175
CFS	15	5	10	14	18	32

Appendix G. Comparison of EU pH-dependence Tests to Method 1313 RCLs

TABLE OF CONTENTS

EaFA Fly Ash F-1
SWA Solidified Waste Analog F-5
CFS Contaminated Field Soil F-9

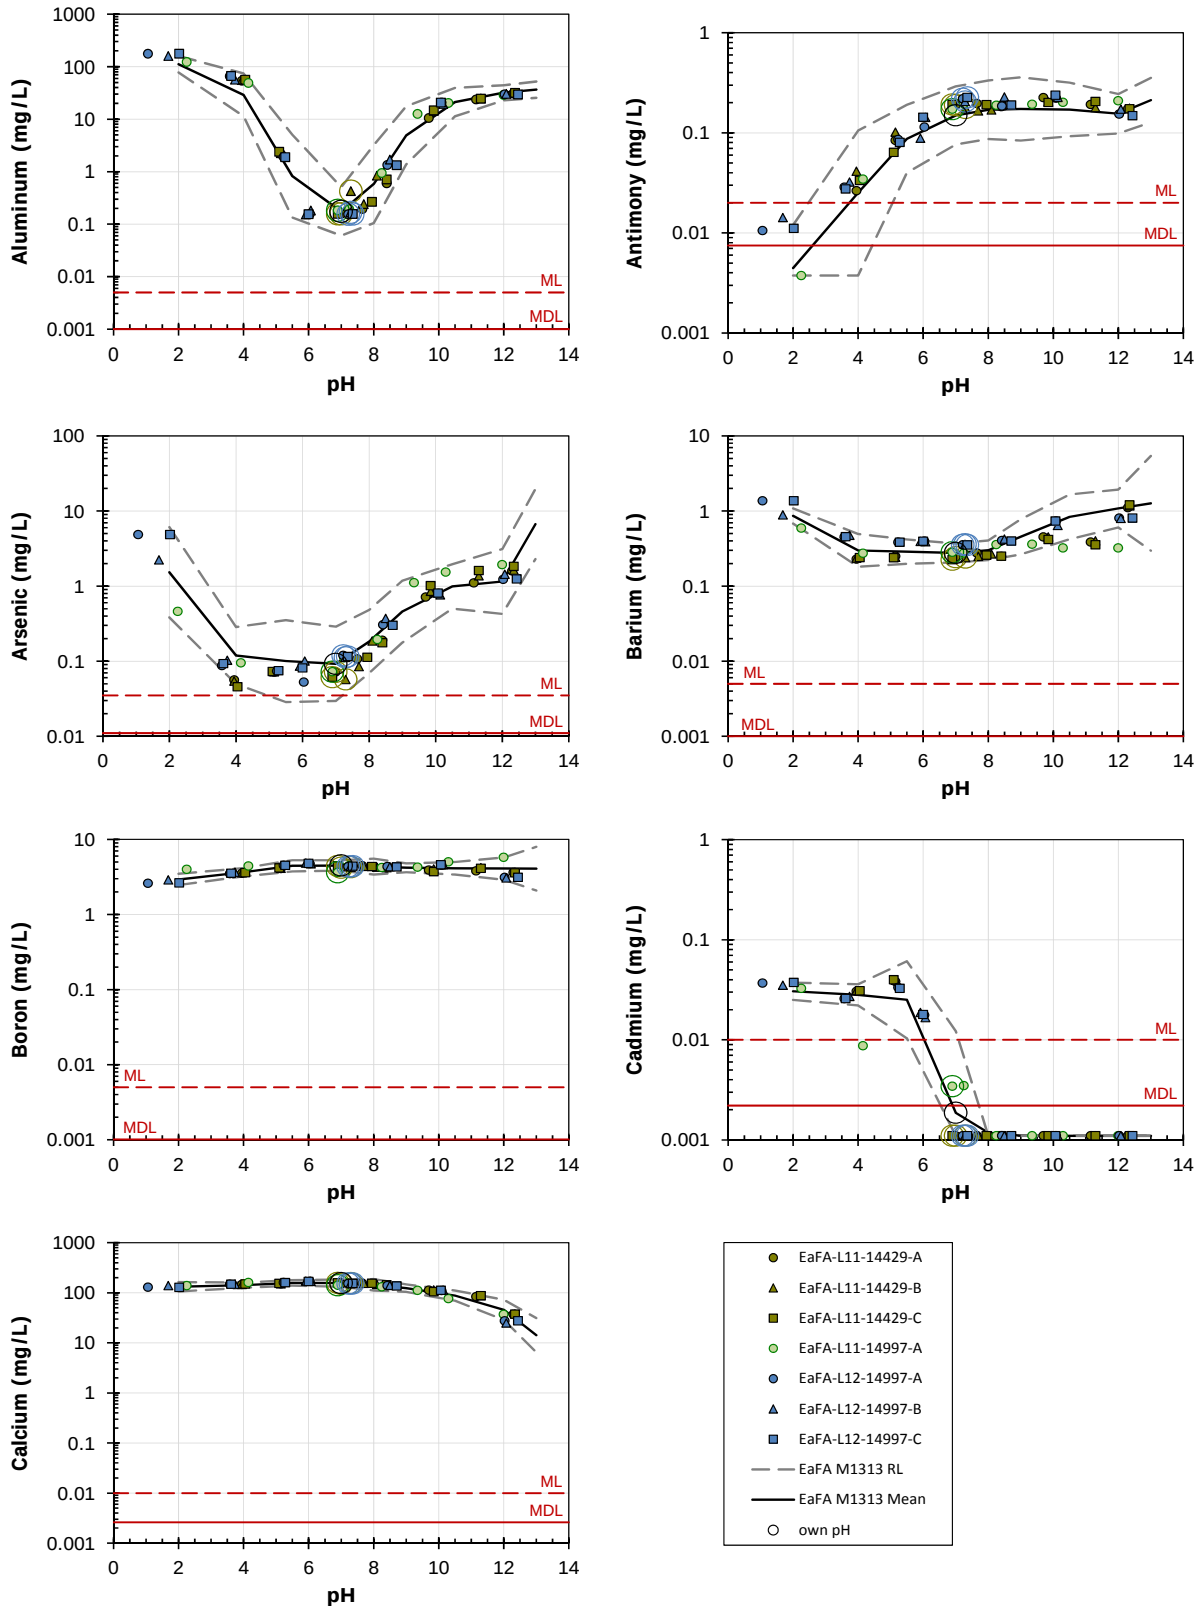

Figure 1. Comparison of CEN/TS 14429 and CEN/TS 14997 results on Phase I EaFA material to the Mean and reproducibility Limit (PL) Interval for Method 1313.

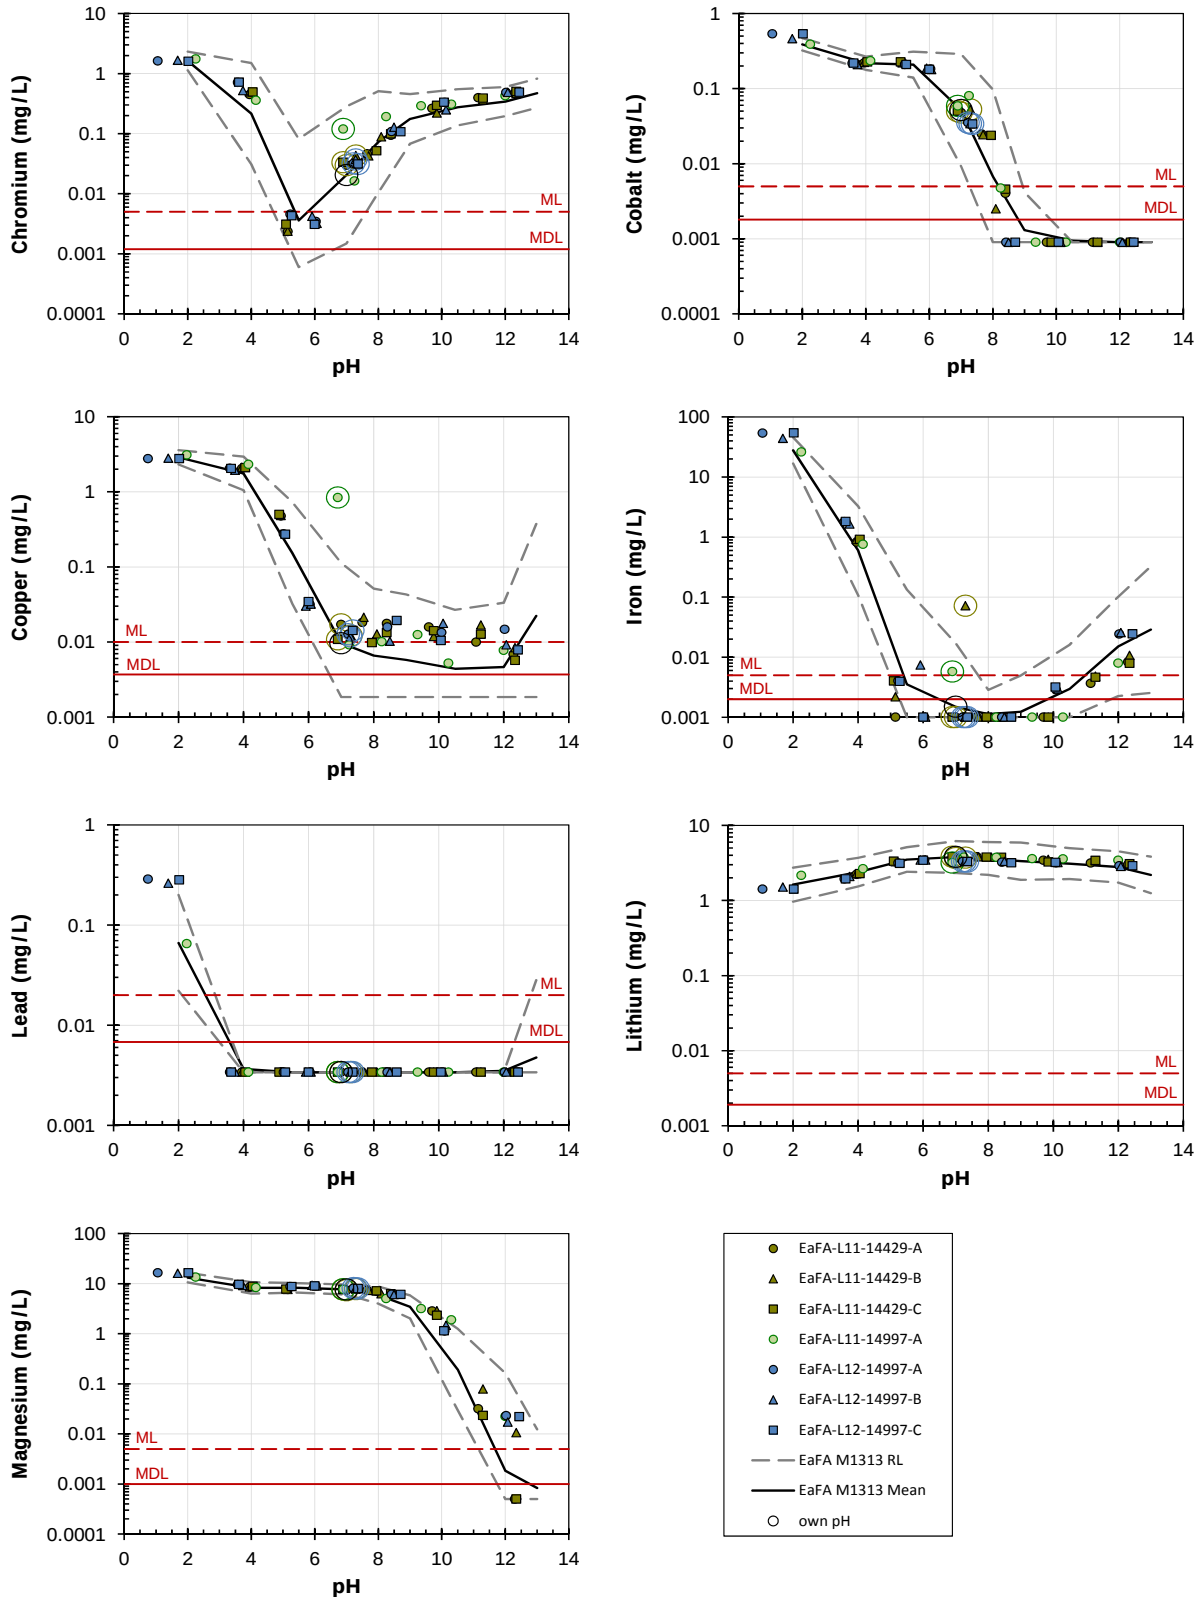

Figure 2. CEN/TS 14429 and CEN/TS 14997 results for EaFA material compared to the Method 1313 mean and reproducibility limit intervals (RLs).

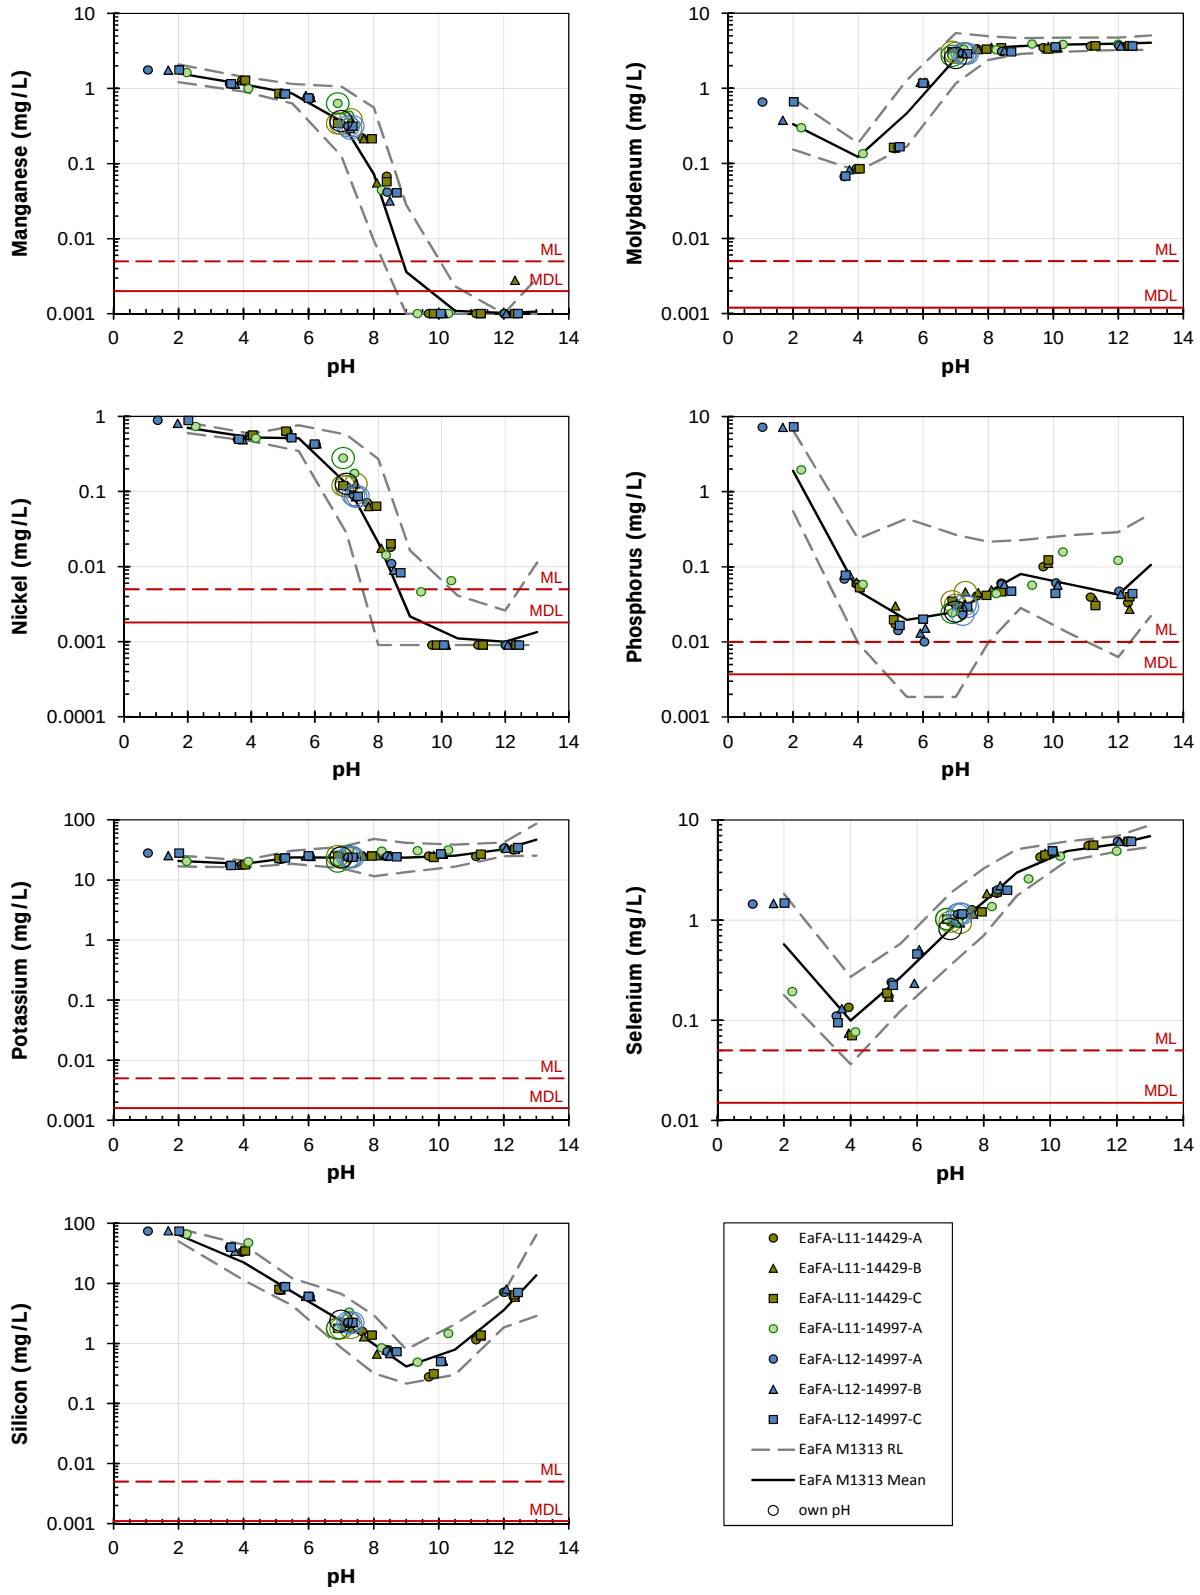

Figure 3. CEN/TS 14429 and CEN/TS 14997 results for EaFA material compared to the Method 1313 mean and reproducibility limit intervals (RLs).

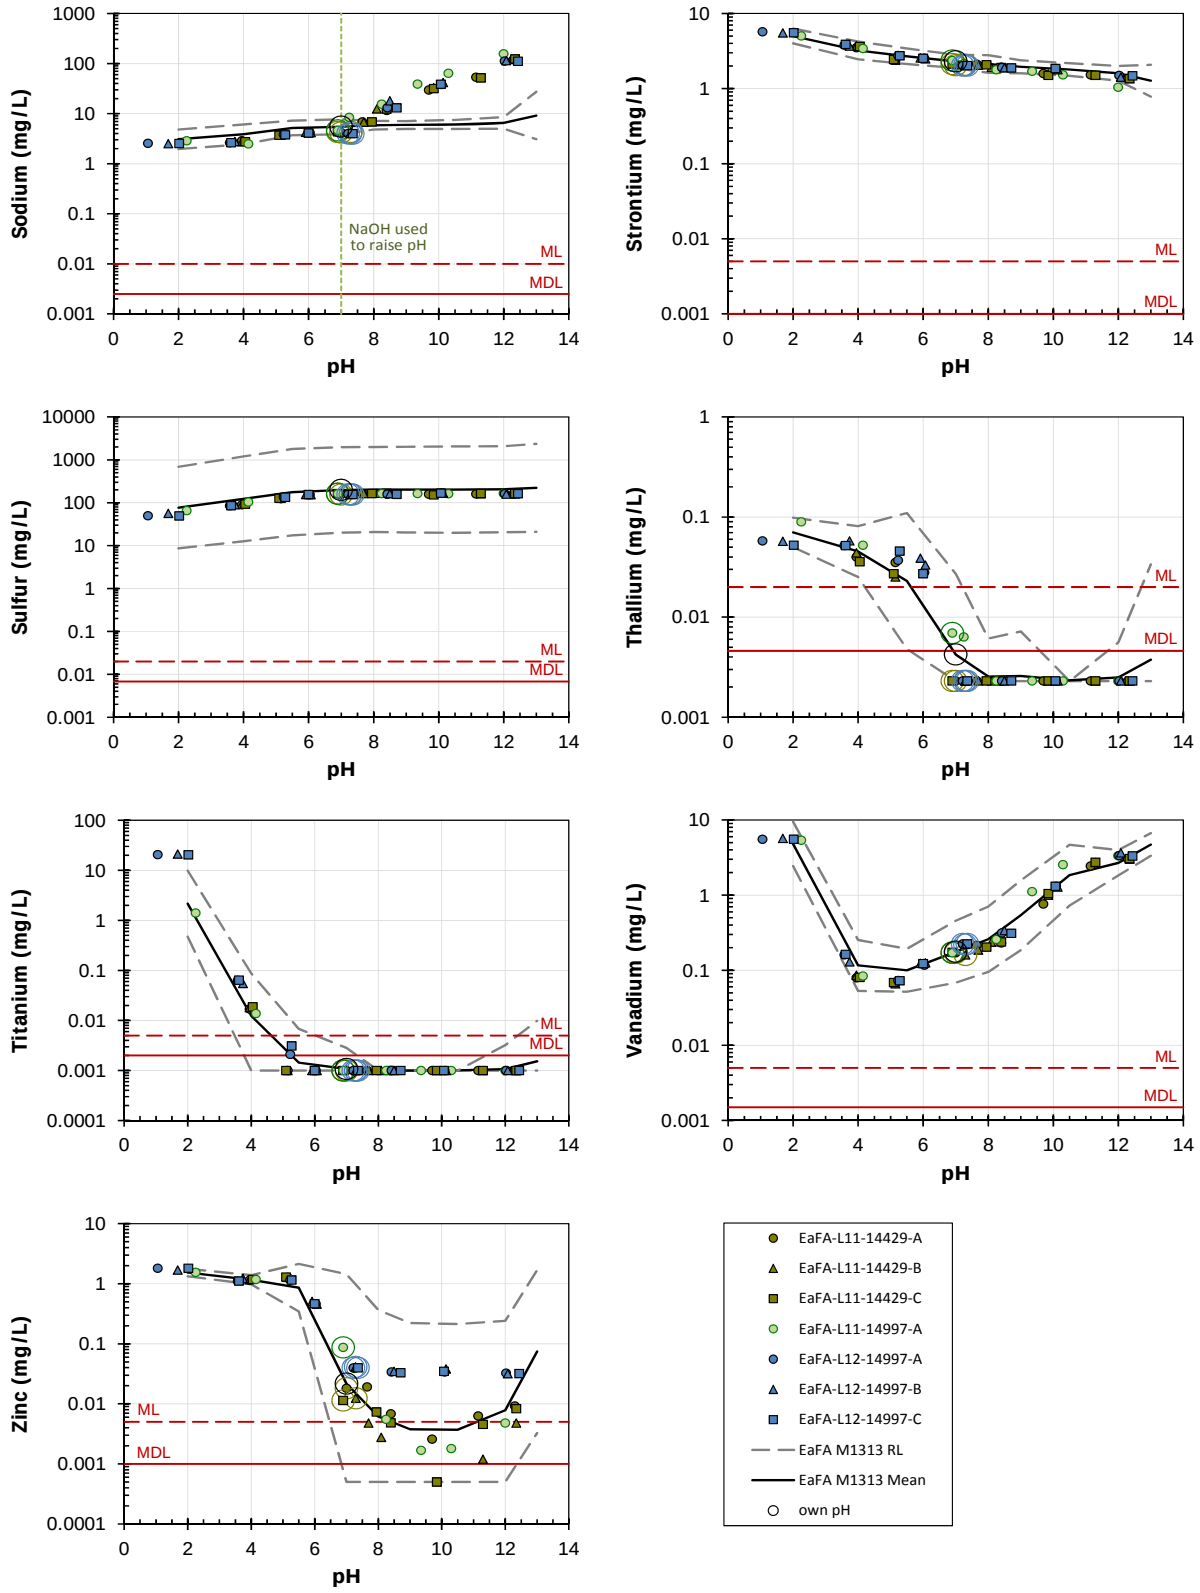

Figure 4. CEN/TS 14429 and CEN/TS 14997 results for EaFA material compared to the Method 1313 mean and reproducibility limit intervals (RLs).

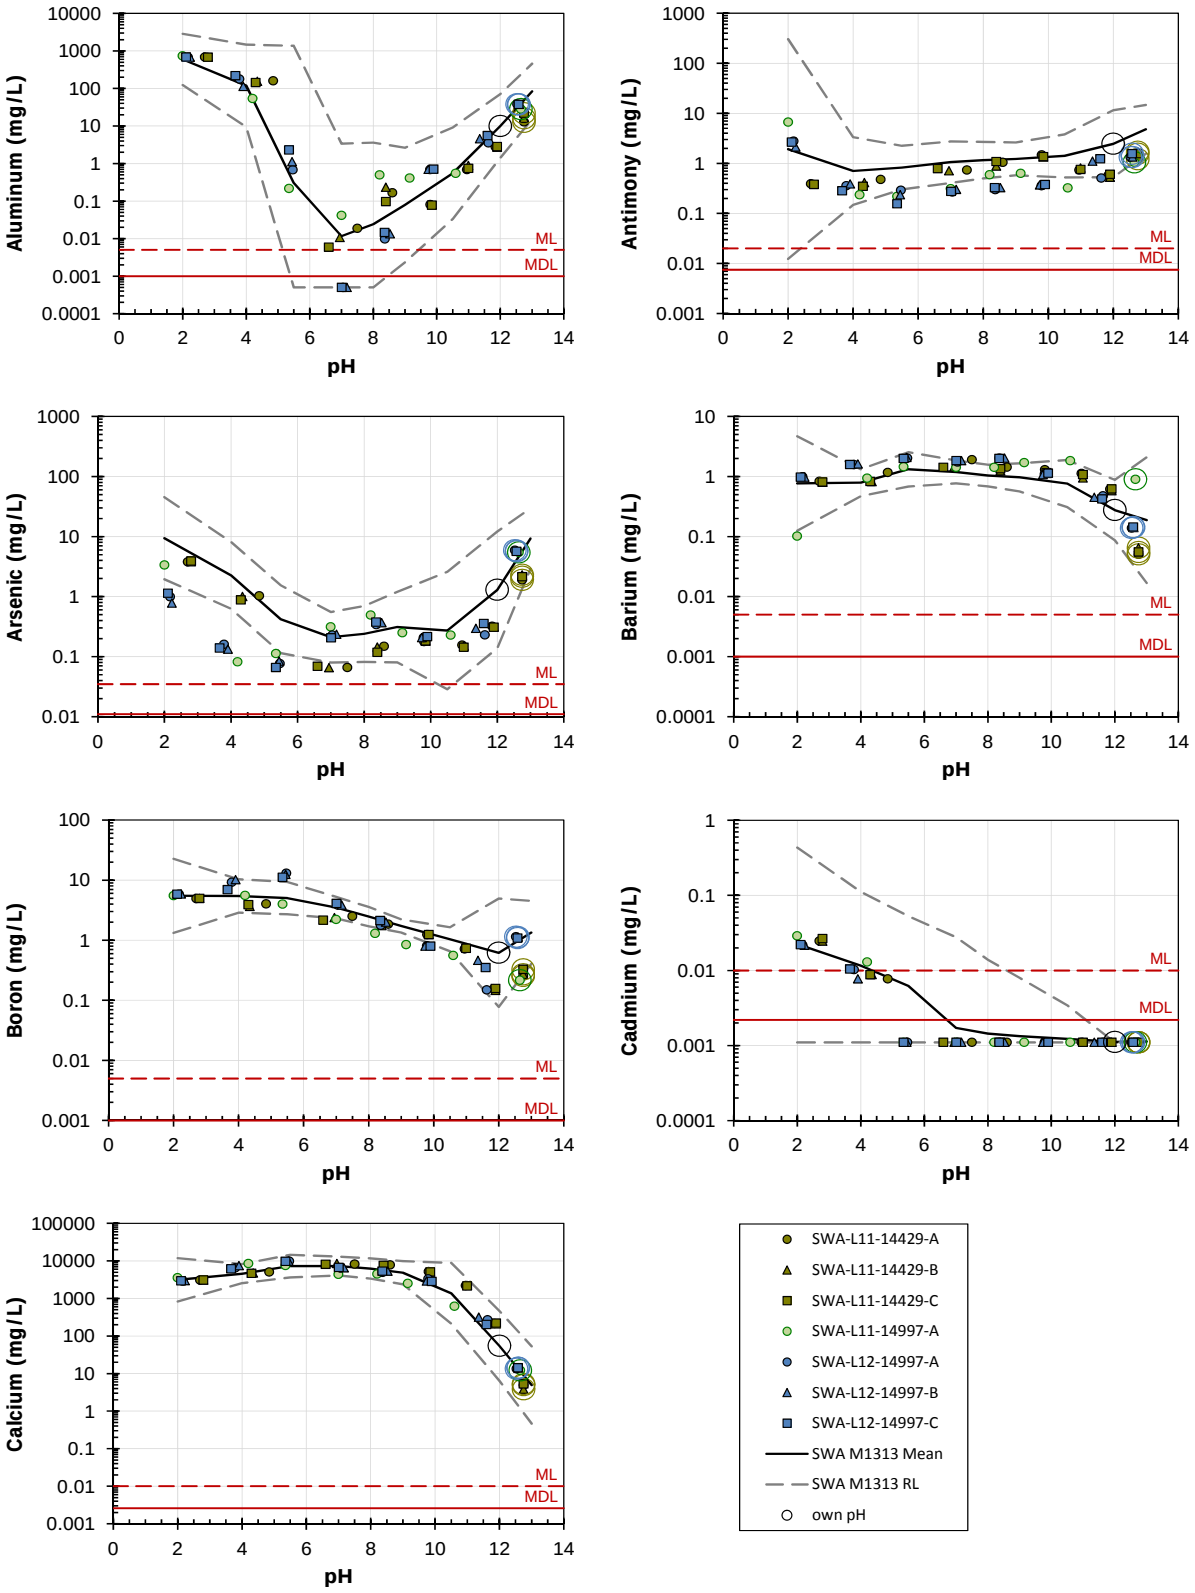

Figure 5. CEN/TS 14429 and CEN/TS 14997 results for SWA material compared to the Method 1313 mean and reproducibility limit intervals (RLs).

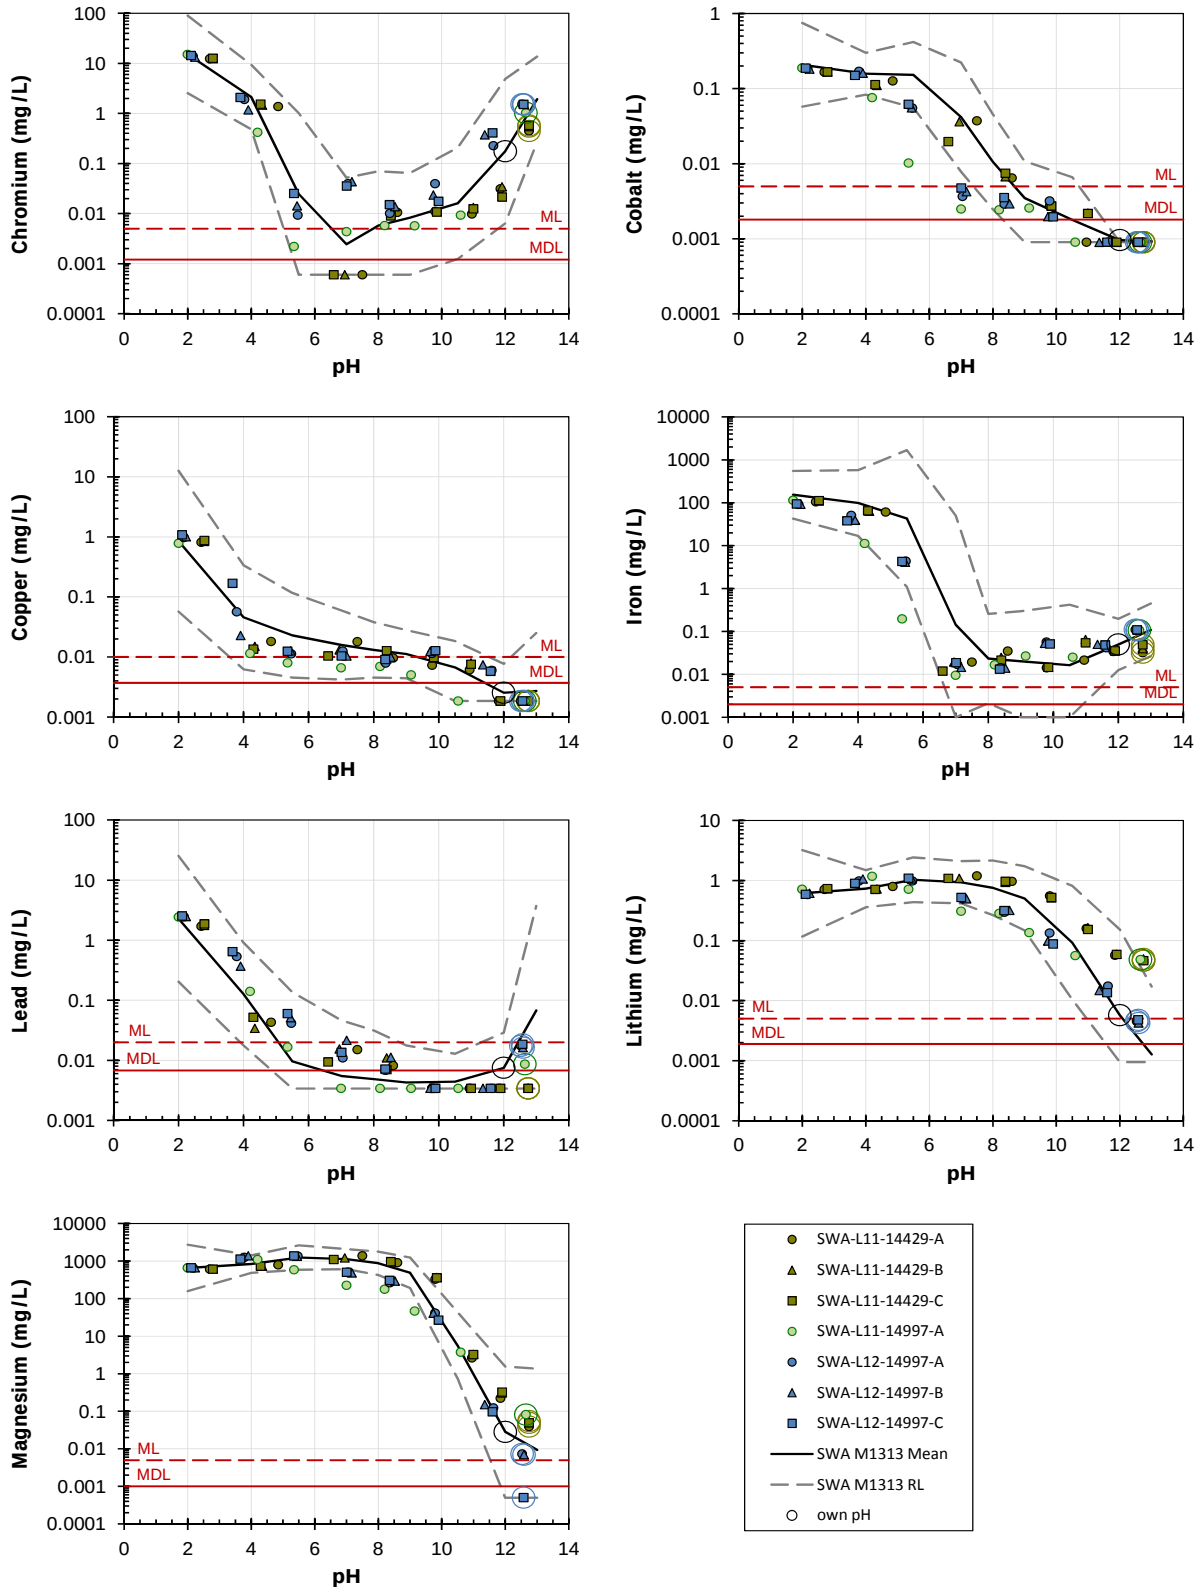

Figure 6. CEN/TS 14429 and CEN/TS 14997 results for SWA material compared to the Method 1313 mean and reproducibility limit intervals (RLs).

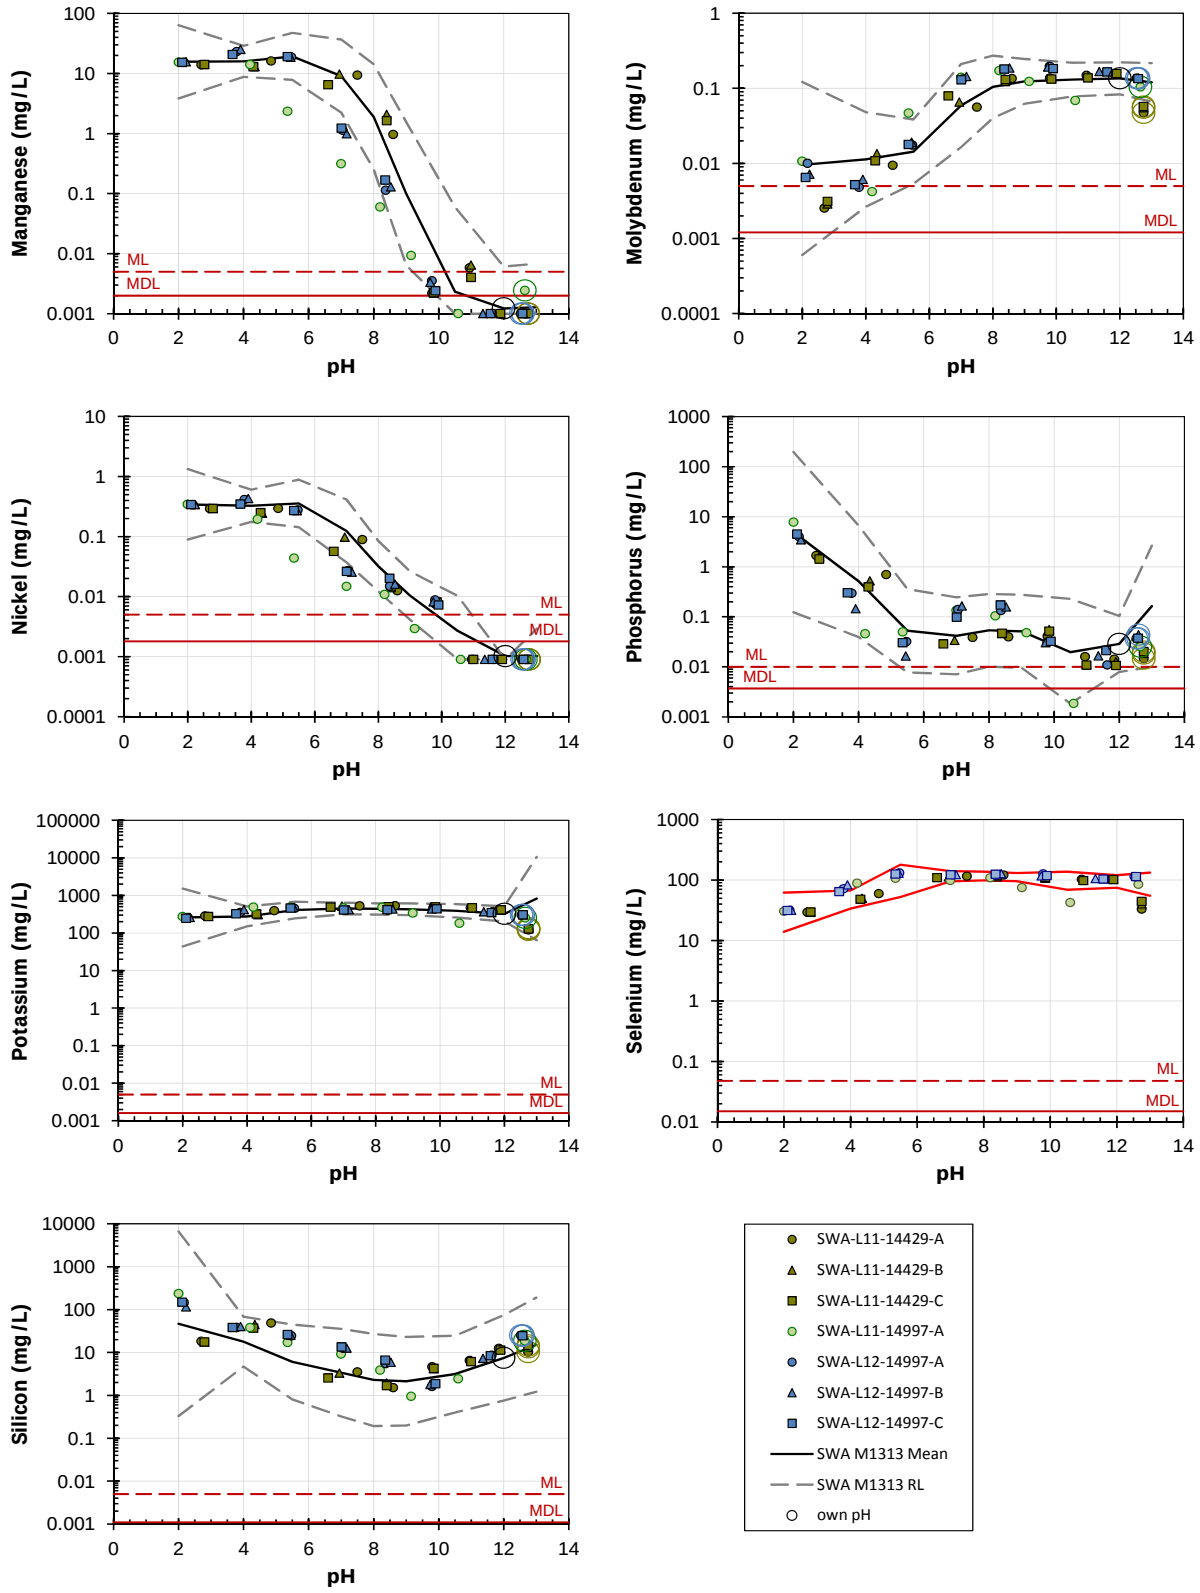

Figure 7. CEN/TS 14429 and CEN/TS 14997 results for SWA material compared to the Method 1313 mean and reproducibility limit intervals (RLs).

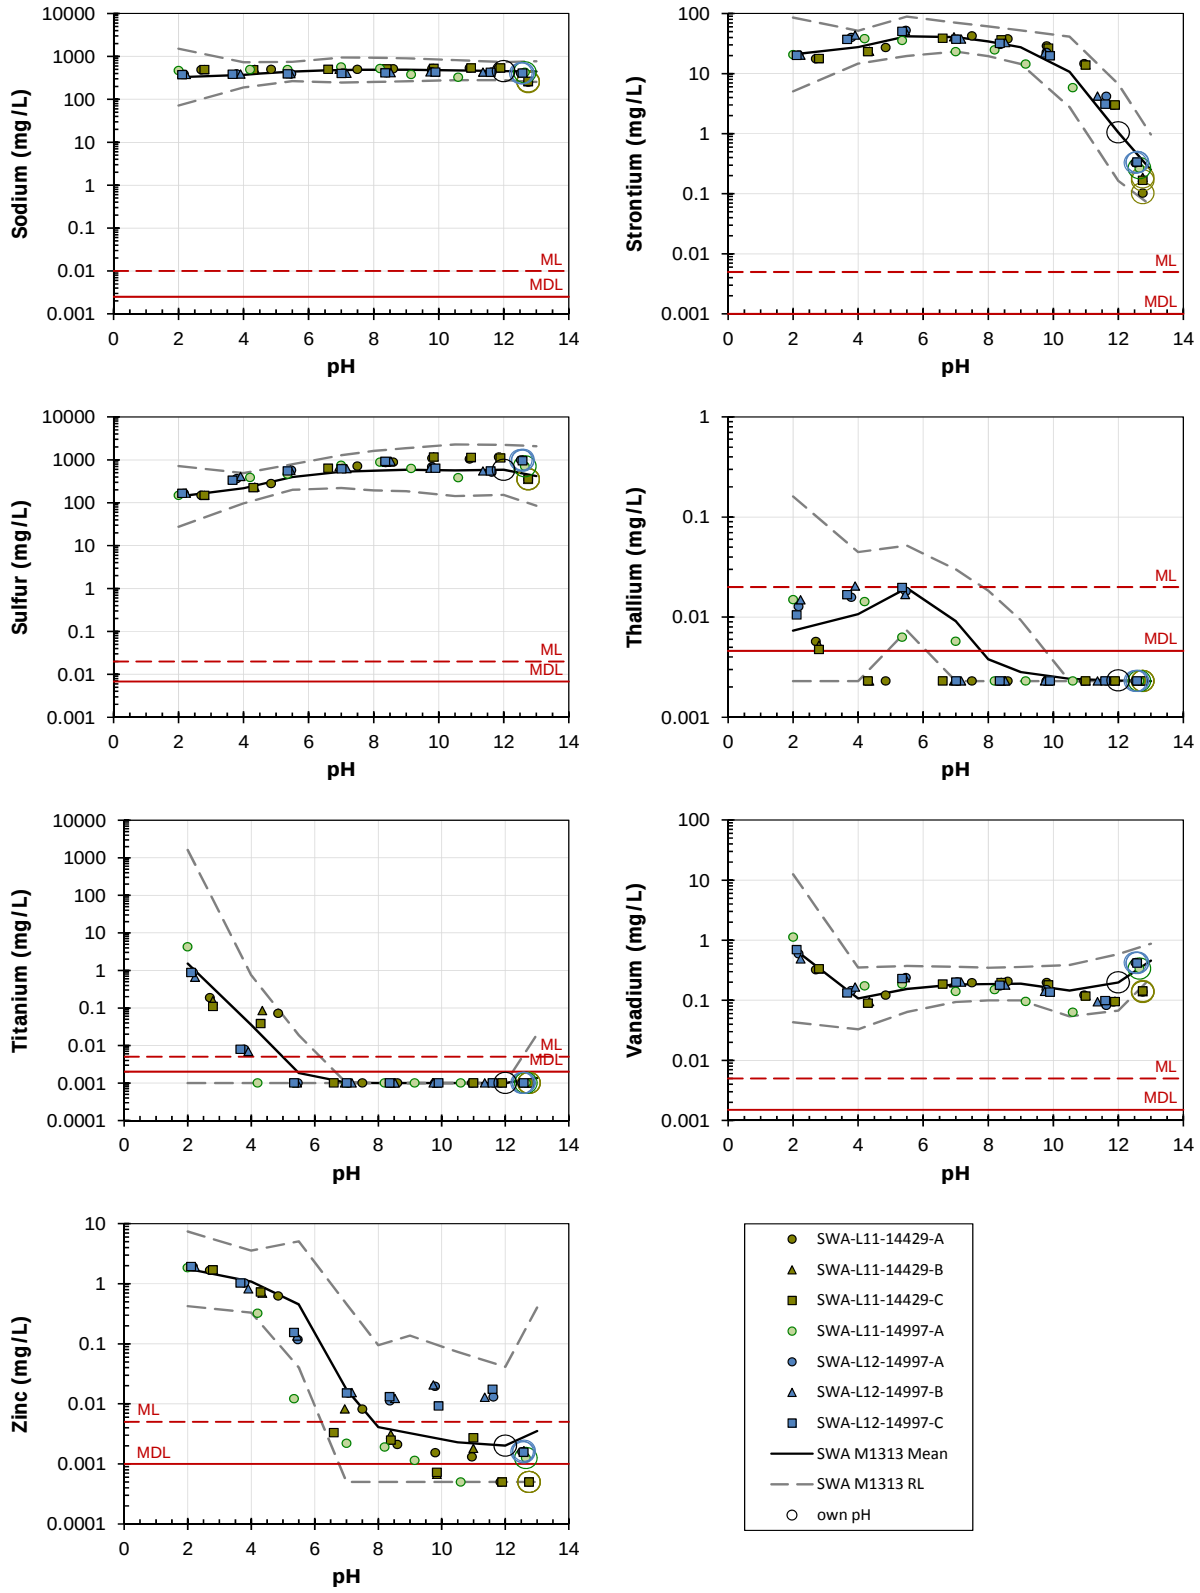

Figure 8. CEN/TS 14429 and CEN/TS 14997 results for SWA material compared to the Method 1313 mean and reproducibility limit intervals (RLs).

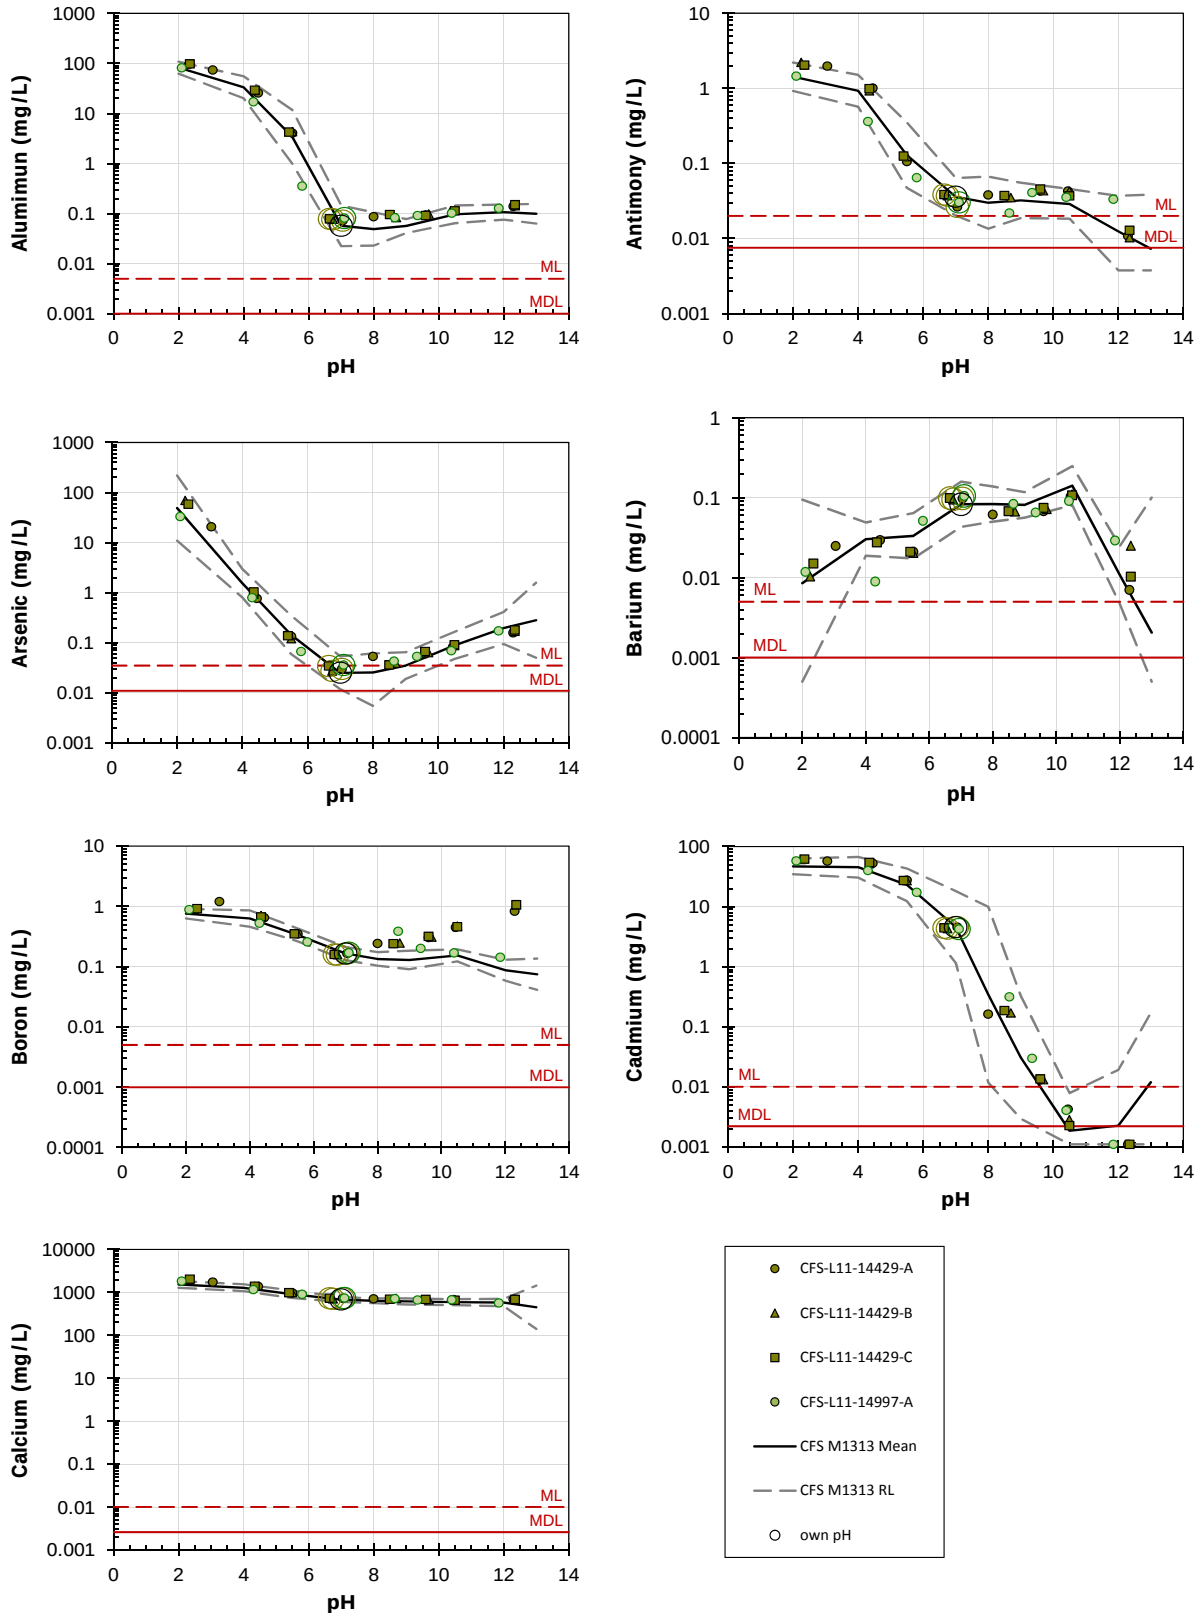

Figure 9. CEN/TS 14429 and CEN/TS 14997 results for CFS material compared to the Method 1313 mean and reproducibility limit intervals (RLs).

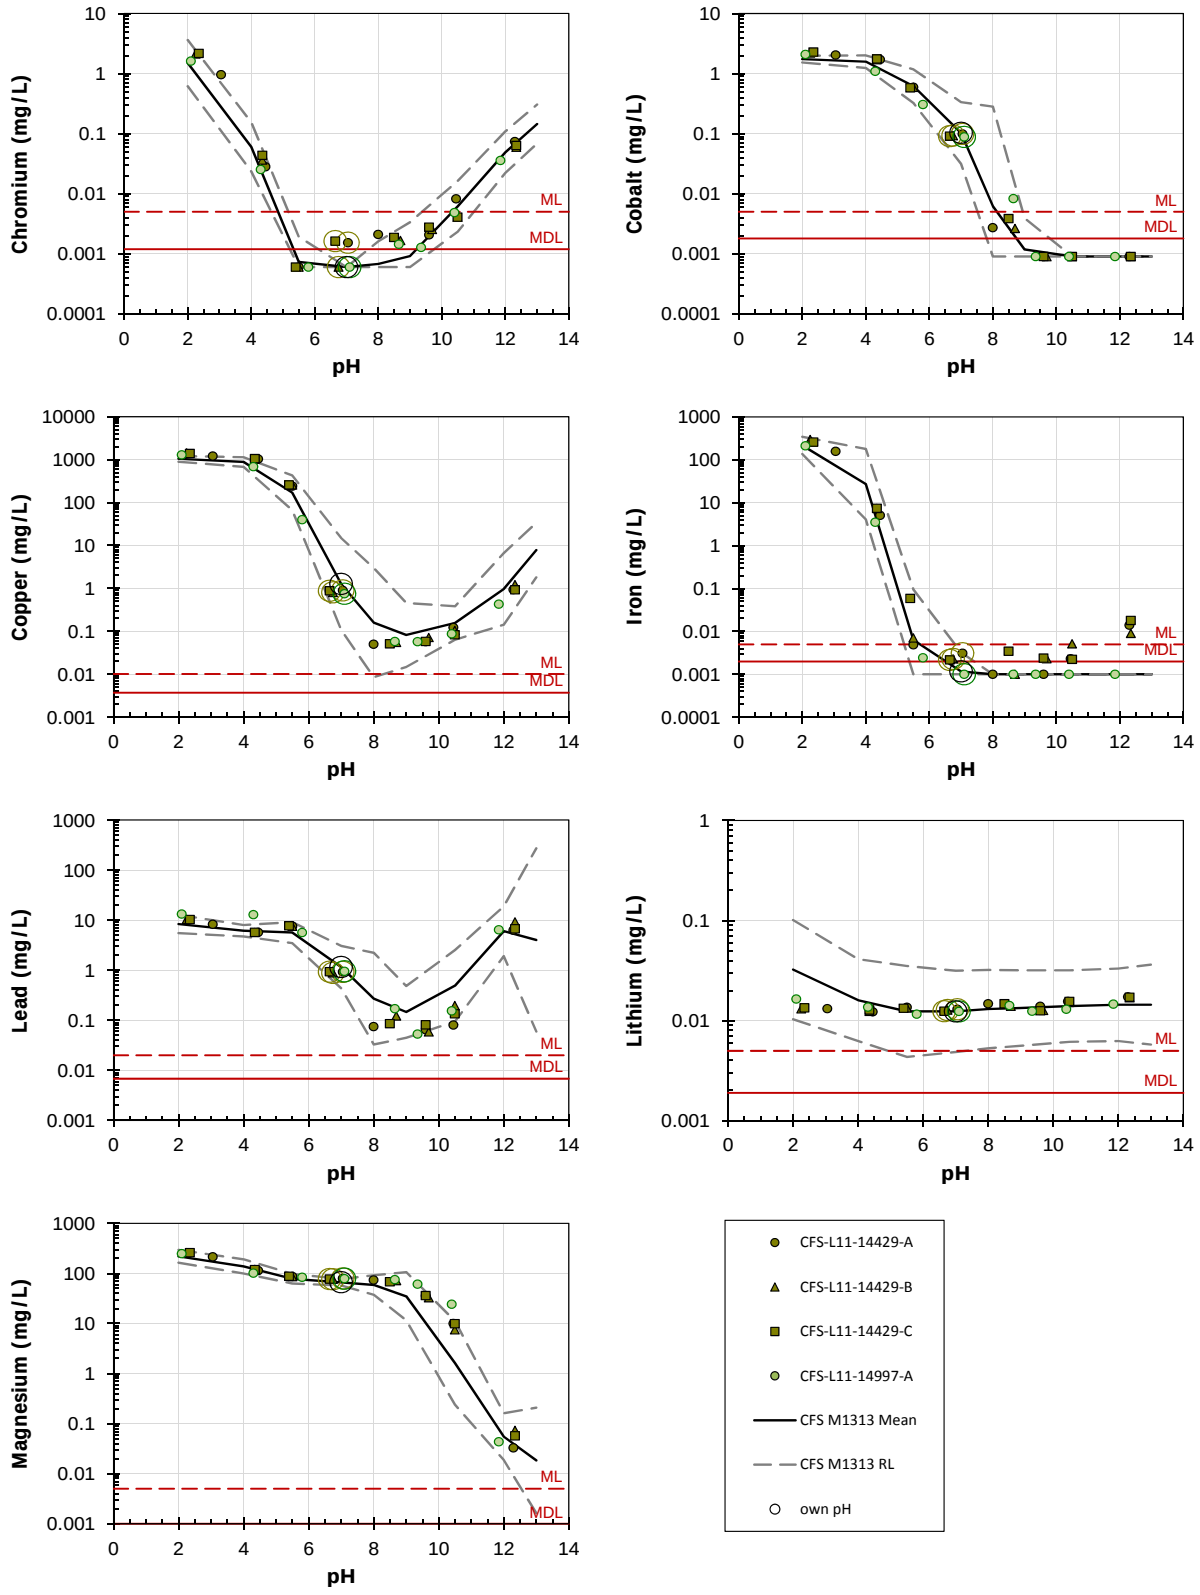

Figure 10. CEN/TS 14429 and CEN/TS 14997 results for CFS material compared to the Method 1313 mean and reproducibility limit intervals (RLs).

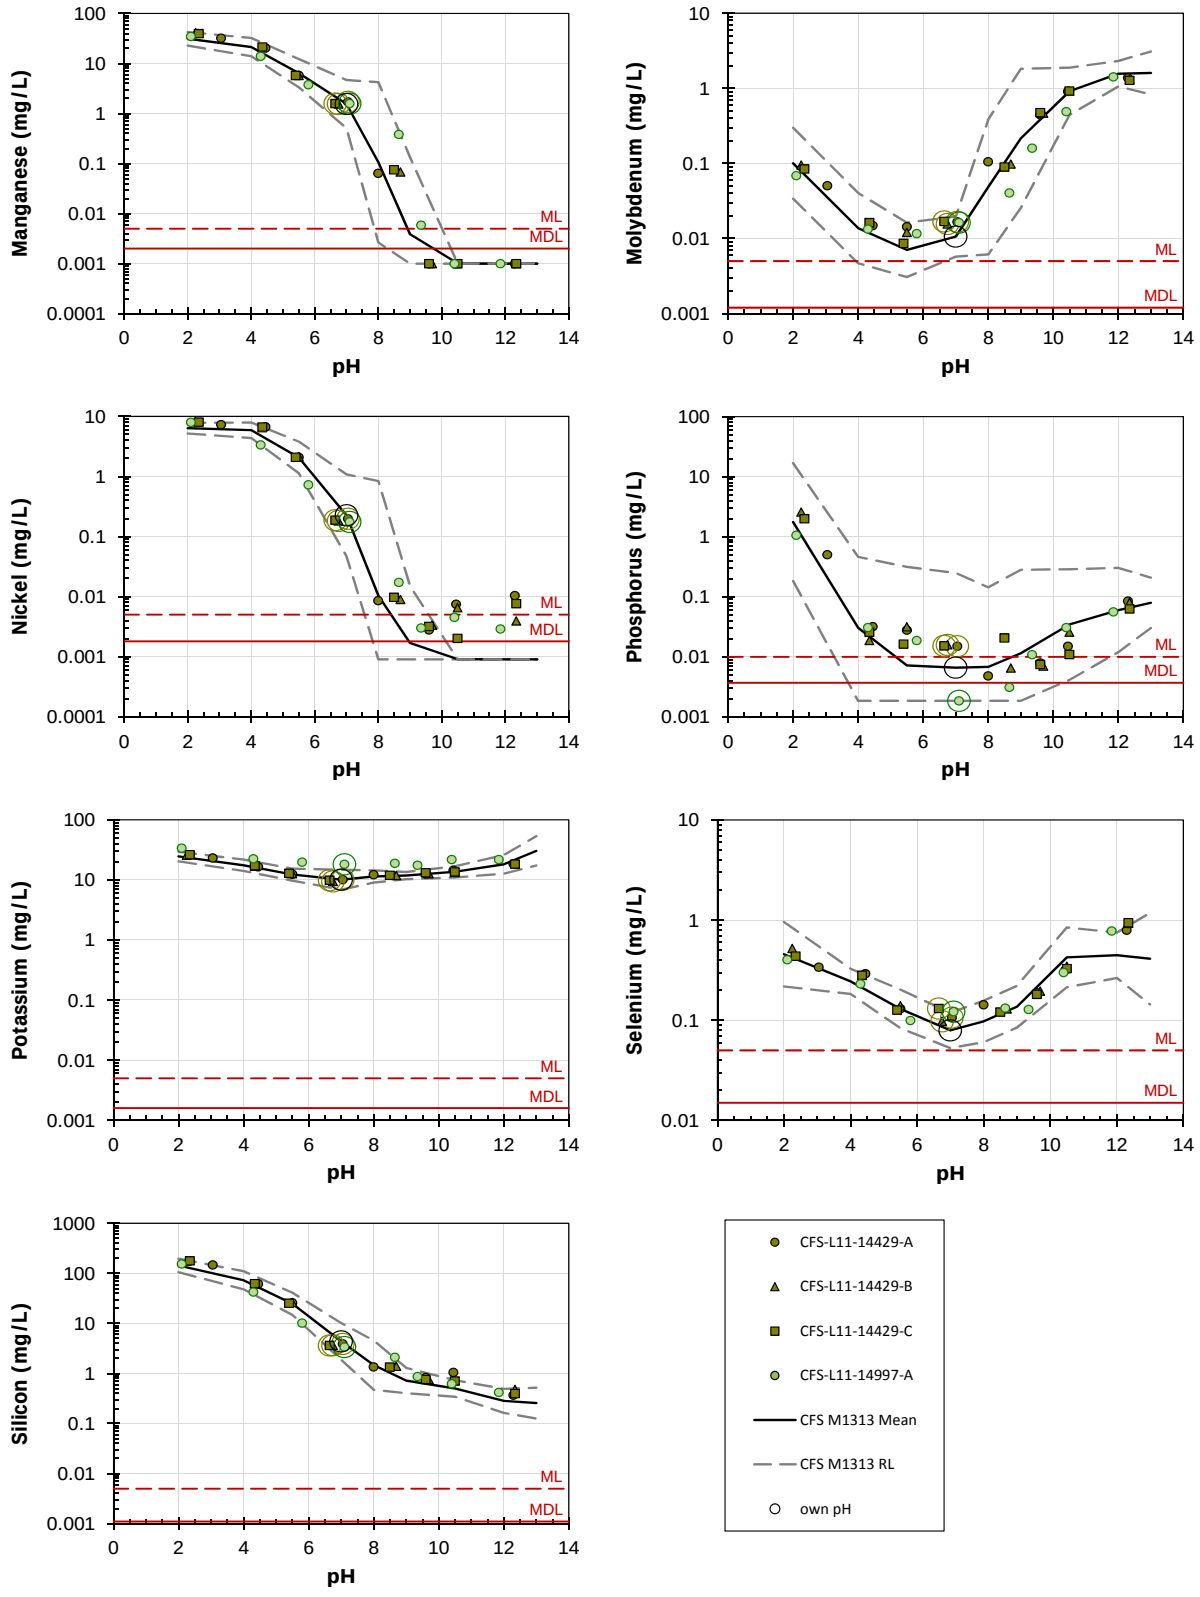

Figure 11. CEN/TS 14429 and CEN/TS 14997 results for CFS material compared to the Method 1313 mean and reproducibility limit intervals (RLs).

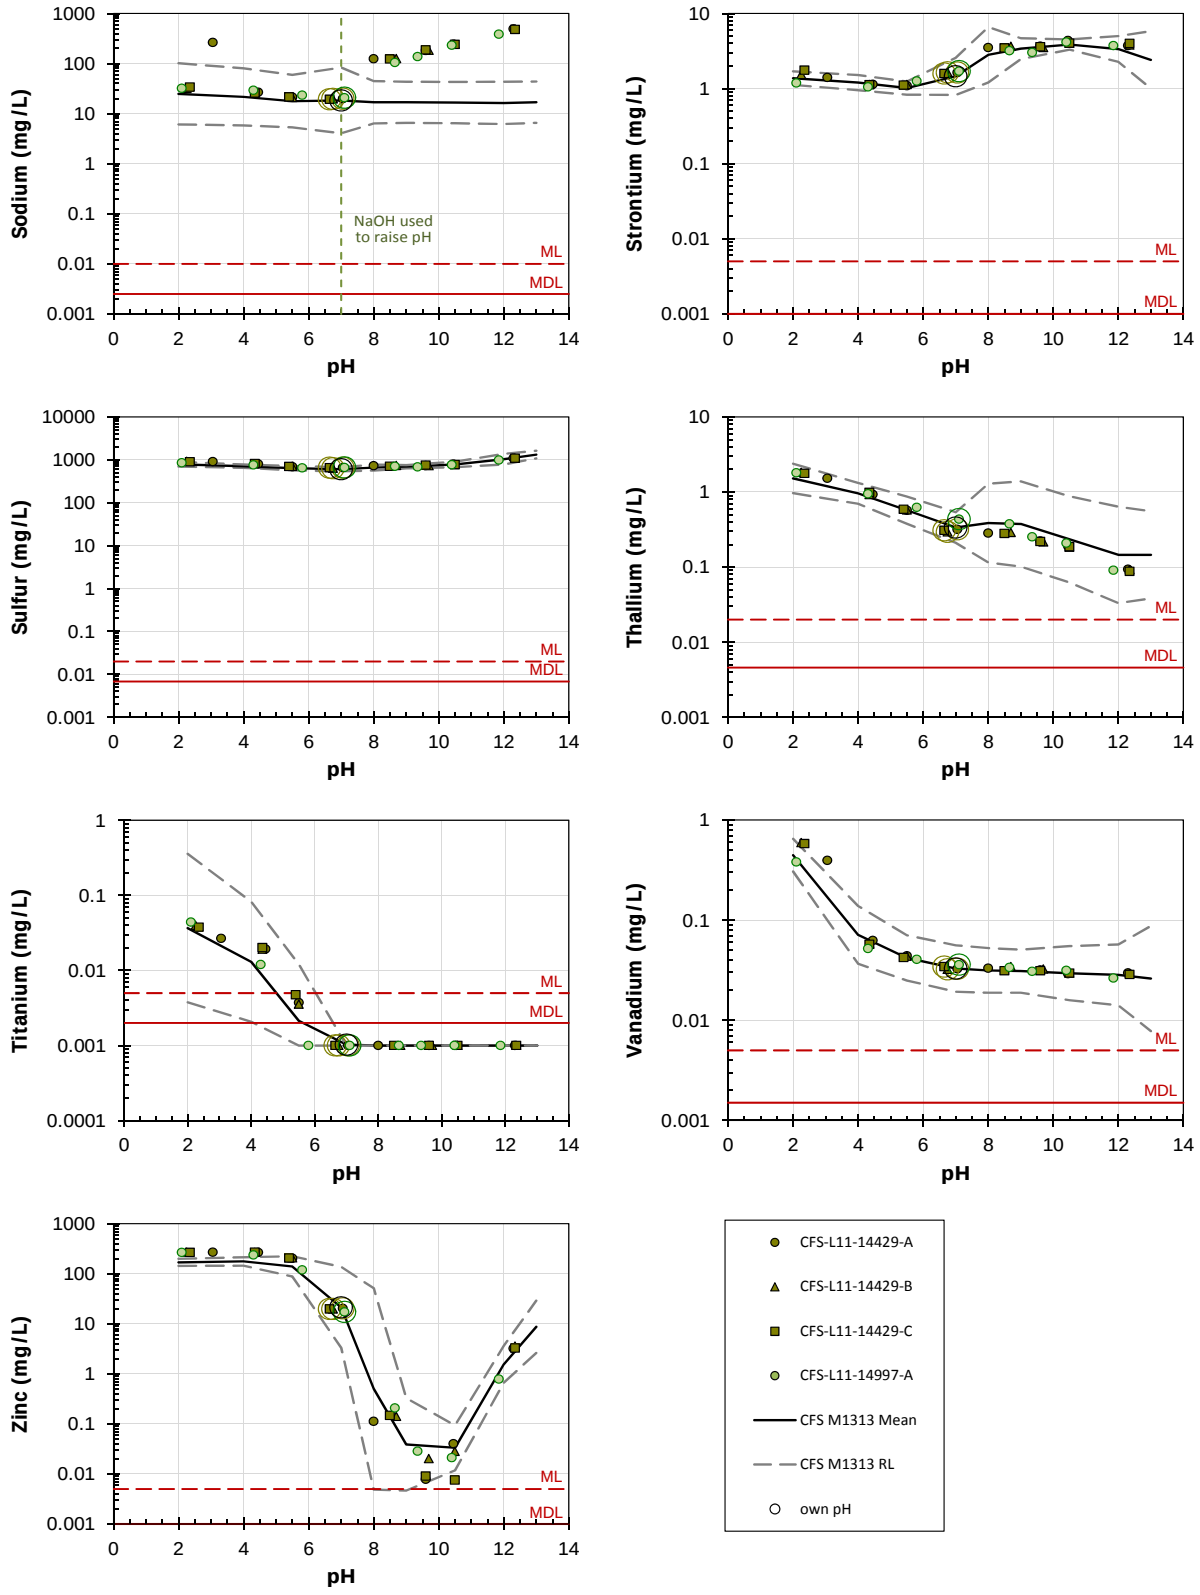

Figure 12. CEN/TS 14429 and CEN/TS 14997 results for CFS material compared to the Method 1313 mean and reproducibility limit intervals (RLs).

Appendix H. Summary of Analytical QA/QC for Selected Analytes

EaFA Coal Combustion Fly Ash
Method 1313

Overall Mean RSD	2.5%
Stdev of Mean RSDs	1.4%
Overall Mean Completeness	98%
Max Spike Recovery	118%
Min Spike Recovery	81%

Antimony
Sb

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	6.2%	1.4%	100.0%	105%	101%	
L02	5.0%	2.7%	96.3%	113%	106%	
L04	5.6%	2.9%	96.3%	115%	107%	
L05	5.8%	2.7%	96.3%	98%	94%	
L06	4.5%	3.0%	100.0%	100%	95%	
L07	5.6%	3.1%	96.3%	112%	97%	
L08	6.6%	3.3%	96.3%	101%	100%	
L09	5.5%	3.2%	92.6%	104%	102%	
L10	5.7%	2.8%	96.3%	102%	92%	
L11	5.6%	2.8%	92.6%	110%	97%	
Ref	5.5%	3.0%	96.3%	102%	92%	
Mean	5.6%		96.3%	115%	92%	Max-Min

Arsenic
As

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	4.7%	3.6%	96.3%	105%	101%	
L02	4.3%	2.8%	96.3%	112%	101%	
L04	3.5%	3.1%	100.0%	116%	107%	
L05	3.4%	2.9%	100.0%	93%	91%	
L06	4.5%	3.0%	96.3%	102%	96%	
L07	4.2%	3.2%	96.3%	101%	96%	
L08	4.8%	3.2%	96.3%	102%	98%	
L09	3.5%	2.7%	100.0%	100%	98%	
L10	4.0%	3.9%	92.6%	100%	90%	
L11	4.5%	3.6%	96.3%	108%	99%	
Ref	3.8%	2.6%	98.1%	101%	89%	
Mean	4.1%		97.2%	116%	89%	Max-Min

EaFA Coal Combustion Fly Ash
Method 1313

Boron
B

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	0.9%	0.8%	100.0%	88%	81%	
L02	2.3%	2.1%	100.0%	109%	95%	
L04	0.9%	0.6%	100.0%	86%	81%	
L05	1.3%	1.2%	96.3%	97%	86%	
L06	2.6%	2.7%	100.0%	100%	87%	
L07	2.1%	2.3%	100.0%	91%	84%	
L08	2.5%	2.4%	100.0%	91%	85%	
L09	1.2%	0.8%	100.0%	99%	84%	
L10	1.1%	0.8%	100.0%	92%	87%	
L11	0.8%	0.6%	100.0%	95%	89%	
Ref	0.9%	0.5%	100.0%	104%	82%	
Mean	1.5%		99.7%	109%	81%	Max-Min

Barium
Ba

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	0.7%	0.9%	100.0%	96%	90%	
L02	2.1%	2.4%	100.0%	101%	89%	
L04	1.5%	2.2%	100.0%	108%	100%	
L05	0.7%	0.7%	100.0%	93%	91%	
L06	2.6%	2.8%	100.0%	92%	86%	
L07	2.0%	2.5%	100.0%	111%	87%	
L08	2.2%	2.6%	100.0%	88%	87%	
L09	0.6%	0.5%	100.0%	92%	88%	
L10	0.7%	0.8%	100.0%	91%	81%	
L11	0.7%	0.5%	100.0%	95%	84%	
Ref	0.8%	0.6%	100.0%	92%	83%	
Mean	1.3%		100.0%	111%	81%	Max-Min

Calcium
Ca

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	0.8%	1.0%	100.0%	83%	81%	
L02	2.0%	2.2%	100.0%	90%	85%	
L04	0.6%	0.4%	100.0%	88%	81%	
L05	0.6%	0.7%	100.0%	86%	85%	
L06	2.6%	2.8%	100.0%	95%	89%	
L07	2.0%	2.5%	100.0%	99%	87%	
L08	2.1%	2.7%	100.0%	89%	85%	
L09	0.7%	0.5%	100.0%	87%	81%	
L10	1.0%	1.3%	100.0%	89%	82%	
L11	0.7%	0.3%	100.0%	90%	86%	
Ref	0.7%	0.4%	100.0%	91%	84%	
Mean	1.2%		100.0%	99%	81%	Max-Min

EaFA Coal Combustion Fly Ash
Method 1313

Chromium
Cr

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	1.8%	2.7%	100.0%	104%	99%	
L02	2.9%	2.6%	100.0%	106%	100%	
L04	1.1%	1.4%	100.0%	108%	102%	
L05	2.0%	2.6%	100.0%	98%	94%	
L06	3.3%	3.1%	100.0%	98%	94%	
L07	3.2%	3.7%	96.3%	98%	94%	
L08	3.6%	3.1%	100.0%	97%	95%	
L09	1.0%	0.9%	100.0%	103%	100%	
L10	1.7%	2.4%	55.6%	99%	89%	
L11	1.2%	1.8%	100.0%	107%	95%	
Ref	1.0%	0.8%	100.0%	99%	91%	
Mean	2.0%		96.0%	108%	89%	Max-Min

Cobalt
Co

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	1.7%	1.1%	100.0%	109%	105%	
L02	3.8%	3.8%	96.3%	108%	103%	
L04	1.6%	1.3%	100.0%	107%	100%	
L05	1.7%	1.4%	100.0%	100%	96%	
L06	3.6%	2.6%	100.0%	99%	96%	
L07	2.2%	2.4%	100.0%	112%	94%	
L08	2.8%	2.2%	100.0%	98%	97%	
L09	1.8%	2.1%	100.0%	104%	101%	
L10	2.8%	2.8%	100.0%	101%	91%	
L11	2.3%	2.3%	100.0%	106%	96%	
Ref	1.9%	1.7%	100.0%	102%	92%	
Mean	2.3%		99.7%	112%	91%	Max-Min

Molybdenum
Mo

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	1.2%	1.1%	100.0%	94%	92%	
L02	2.6%	2.8%	96.3%	108%	90%	
L04	0.8%	0.5%	100.0%	97%	89%	
L05	0.9%	0.8%	100.0%	90%	87%	
L06	2.8%	2.7%	100.0%	100%	83%	
L07	2.0%	2.2%	100.0%	106%	86%	
L08	2.9%	3.0%	100.0%	90%	87%	
L09	1.2%	0.7%	100.0%	103%	97%	
L10	0.9%	0.7%	100.0%	92%	84%	
L11	1.2%	1.2%	100.0%	98%	87%	
Ref	0.8%	0.5%	100.0%	108%	89%	
Mean	1.5%		99.7%	108%	83%	Max-Min

EaFA Coal Combustion Fly Ash
Method 1313

Selenium
Se

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	3.0%	2.8%	96.3%	91%	88%	
L02	3.4%	3.0%	92.6%	110%	83%	
L04	2.8%	3.2%	96.3%	114%	105%	
L05	2.7%	2.4%	100.0%	87%	84%	
L06	4.1%	3.0%	96.3%	98%	84%	
L07	3.4%	2.9%	100.0%	87%	85%	
L08	3.1%	2.9%	96.3%	90%	86%	
L09	2.9%	2.9%	96.3%	96%	88%	
L10	3.3%	2.3%	100.0%	88%	83%	
L11	3.3%	3.0%	96.3%	91%	82%	
Ref	2.5%	1.7%	100.0%	105%	92%	
Mean	3.1%		97.5%	114%	82%	Max-Min

Vanadium
V

	Mean RSD	Stdev RSD	Completeness	Rec Max	Rec Min	
L01	1.2%	1.3%	100.0%	97%	95%	
L02	2.6%	2.5%	100.0%	108%	93%	
L04	1.2%	1.2%	100.0%	103%	96%	
L05	1.2%	0.8%	100.0%	93%	91%	
L06	2.9%	2.7%	100.0%	101%	93%	
L07	2.4%	2.2%	100.0%	93%	90%	
L08	2.2%	2.0%	100.0%	92%	90%	
L09	1.0%	0.5%	100.0%	104%	101%	
L10	1.0%	0.6%	100.0%	91%	82%	
L11	1.5%	1.1%	100.0%	101%	90%	
Ref	1.5%	1.2%	100.0%	118%	92%	
Mean	1.7%		100.0%	118%	82%	Max-Min

SWA Solidified Waste Analog
Method 1313

Overall Mean RSD	1.9%
Stdev of Mean RSDs	0.9%
Overall Mean Completeness	100%
Max Spike Recovery	119%
Min Spike Recovery	82%

Antimony
Sb

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	2.0%	2.3%	100.0%	116%	103%	
L02	2.4%	2.5%	100.0%	100%	96%	
L04	2.2%	2.7%	100.0%	99%	92%	
L05	1.4%	1.4%	100.0%	106%	101%	
L06	2.5%	2.0%	100.0%	107%	89%	
L07	1.7%	1.9%	100.0%	103%	91%	
L09	1.9%	2.3%	100.0%	107%	94%	
L10	1.9%	1.6%	100.0%	111%	106%	
L11	3.2%	2.6%	100.0%	106%	99%	
Ref	1.7%	1.6%	100.0%	117%	95%	
Mean	2.1%		100.0%	117%	89%	Max-Min

Arsenic
As

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	2.7%	2.5%	100.0%	96%	85%	
L02	2.9%	2.4%	100.0%	112%	99%	
L04	3.1%	2.9%	96.4%	111%	107%	
L05	2.6%	2.6%	100.0%	95%	90%	
L06	2.9%	2.9%	96.7%	119%	118%	
L07	3.1%	2.5%	100.0%	119%	109%	
L09	2.7%	2.2%	100.0%	88%	84%	
L10	3.7%	2.7%	100.0%	106%	98%	
L11	4.0%	3.3%	96.3%	101%	96%	
Ref	2.5%	2.5%	100.0%	109%	85%	
Mean	3.0%		99.0%	119%	84%	Max-Min

SWA Solidified Waste Analog
Method 1313

Boron
B

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	0.7%	0.6%	100.0%	95%	93%	
L02	1.2%	0.8%	100.0%	105%	103%	
L04	0.7%	0.4%	100.0%	118%	112%	
L05	1.2%	1.5%	100.0%	95%	91%	
L06	1.6%	1.8%	100.0%	118%	114%	
L07	0.8%	0.7%	100.0%	116%	94%	
L09	0.8%	1.1%	100.0%	102%	92%	
L10	1.6%	1.6%	100.0%	106%	91%	
L11	2.2%	2.0%	100.0%	99%	92%	
Ref	0.9%	1.0%	100.0%	108%	92%	
Mean	1.1%		100.0%	118%	91%	Max-Min

Barium
Ba

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	1.6%	4.3%	96.3%	88%	87%	
L02	1.2%	1.1%	100.0%	96%	91%	
L04	0.6%	0.4%	100.0%	107%	99%	
L05	1.2%	1.6%	100.0%	90%	87%	
L06	1.6%	1.7%	100.0%	102%	96%	
L07	0.8%	0.6%	100.0%	102%	86%	
L09	1.1%	2.1%	100.0%	101%	98%	
L10	1.2%	1.7%	100.0%	98%	88%	
L11	1.5%	1.5%	100.0%	108%	85%	
Ref	0.9%	1.0%	100.0%	105%	93%	
Mean	1.1%		99.7%	108%	85%	Max-Min

Calcium
Ca

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	0.8%	0.7%	100.0%	91%	90%	
L02	1.1%	1.1%	100.0%	99%	92%	
L04	0.8%	0.4%	100.0%	97%	87%	
L05	1.2%	1.3%	100.0%	91%	87%	
L06	1.8%	2.0%	100.0%	95%	86%	
L07	0.8%	0.7%	100.0%	86%	84%	
L09	0.9%	1.2%	100.0%	117%	92%	
L10	1.0%	0.9%	100.0%	98%	85%	
L11	1.5%	1.8%	100.0%	85%	82%	
Ref	0.8%	0.7%	100.0%	95%	83%	
Mean	1.1%		100.0%	117%	82%	Max-Min

SWA Solidified Waste Analog
Method 1313

Chromium
Cr

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	3.9%	3.3%	100.0%	92%	90%	
L02	3.0%	3.3%	96.3%	103%	99%	
L04	3.2%	3.2%	100.0%	115%	111%	
L05	1.9%	1.8%	100.0%	98%	92%	
L06	2.5%	2.6%	100.0%	117%	109%	
L07	3.0%	3.3%	96.3%	103%	93%	
L09	2.7%	2.8%	100.0%	90%	86%	
L10	3.5%	2.9%	92.6%	111%	98%	
L11	2.2%	2.1%	100.0%	114%	102%	
Ref	1.5%	2.1%	100.0%	105%	92%	
Mean	2.6%		98.7%	117%	86%	Max-Min

Cobalt
Co

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	2.2%	2.4%	100.0%	99%	98%	
L02	2.2%	2.3%	100.0%	100%	97%	
L04	2.5%	2.3%	100.0%	117%	111%	
L05	3.1%	2.3%	100.0%	93%	92%	
L06	2.5%	2.1%	100.0%	118%	109%	
L07	2.6%	2.7%	100.0%	100%	92%	
L09	1.0%	0.7%	100.0%	101%	98%	
L10	3.0%	2.4%	100.0%	110%	98%	
L11	2.1%	2.5%	100.0%	107%	102%	
Ref	2.7%	2.7%	100.0%	103%	92%	
Mean	2.4%		100.0%	118%	92%	Max-Min

Molybdenum
Mo

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	2.8%	2.7%	100.0%	103%	103%	
L02	4.0%	3.0%	96.3%	109%	104%	
L04	2.2%	2.8%	100.0%	119%	112%	
L05	2.8%	2.2%	96.3%	99%	96%	
L06	3.6%	3.1%	100.0%	119%	111%	
L07	2.7%	2.6%	100.0%	107%	92%	
L09	3.4%	2.9%	100.0%	105%	102%	
L10	3.8%	3.2%	96.3%	113%	99%	
L11	4.6%	3.3%	96.3%	105%	94%	
Ref	3.4%	2.7%	98.1%	104%	92%	
Mean	3.3%		98.3%	119%	92%	Max-Min

SWA Solidified Waste Analog
Method 1313

Selenium
Se

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	0.6%	0.6%	100.0%	93%	85%	
L02	1.1%	0.8%	100.0%	88%	83%	
L04	0.6%	0.4%	100.0%	91%	87%	
L05	1.4%	2.2%	100.0%	97%	91%	
L06	2.0%	2.7%	96.7%	105%	94%	
L07	0.7%	0.7%	100.0%	99%	86%	
L09	0.8%	1.3%	100.0%	115%	105%	
L10	1.2%	1.7%	100.0%	99%	87%	
L11	1.7%	2.0%	100.0%	92%	86%	
Ref	0.6%	2.7%	100.0%	105%	87%	
Mean	1.0%		99.7%	115%	83%	Max-Min

Vanadium
V

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	1.2%	0.8%	100.0%	100%	99%	
L02	1.8%	1.1%	100.0%	113%	103%	
L04	1.1%	0.7%	100.0%	118%	113%	
L05	2.0%	2.0%	100.0%	92%	88%	
L06	2.2%	1.8%	100.0%	118%	110%	
L07	1.3%	0.8%	100.0%	106%	100%	
L09	1.4%	1.0%	100.0%	100%	97%	
L10	2.0%	1.9%	100.0%	114%	100%	
L11	2.3%	2.2%	100.0%	102%	88%	
Ref	1.2%	0.8%	100.0%	107%	94%	
Mean	1.6%		100.0%	118%	88%	Max-Min

CFS Contaminated Field Soil
Method 1313

Overall Mean RSD	2.8%
Stdev of Mean RSDs	1.9%
Overall Mean Completeness	98%
Max Spike Recovery	118%
Min Spike Recovery	82%

Antimony
Sb

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	4.6%	3.1%	92.6%	117%	111%	
L04	6.1%	3.5%	92.6%	118%	114%	
L06	6.6%	2.8%	96.3%	116%	111%	
L07	6.6%	3.2%	92.6%	115%	109%	
L09	7.2%	3.1%	92.6%	109%	98%	
L10	5.5%	2.9%	93.3%	98%	91%	
L11	7.1%	3.7%	92.6%	94%	87%	
Ref	6.6%	2.8%	94.4%	93%	83%	
Mean	6.3%		93.5%	118%	83%	Max-Min

Arsenic
As

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	4.7%	3.2%	96.3%	107%	105%	
L04	3.7%	2.8%	100.0%	118%	117%	
L06	3.4%	2.4%	100.0%	112%	112%	
L07	3.4%	2.6%	100.0%	117%	101%	
L09	4.1%	3.4%	96.3%	111%	103%	
L10	3.0%	3.1%	96.7%	102%	94%	
L11	4.3%	3.1%	100.0%	95%	87%	
Ref	4.7%	3.2%	98.1%	93%	87%	
	4.0%		98.4%	118%	87%	Max-Min

CFS Contaminated Field Soil
Method 1313

Boron
B

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	1.7%	1.4%	100.0%	108%	101%	
L04	1.7%	1.0%	100.0%	114%	108%	
L06	2.1%	2.6%	96.3%	118%	102%	
L07	1.3%	0.9%	100.0%	110%	104%	
L09	1.2%	0.8%	100.0%	108%	100%	
L10	1.1%	0.9%	100.0%	117%	110%	
L11	1.7%	1.8%	100.0%	94%	89%	
Ref	1.7%	1.4%	100.0%	96%	89%	
Mean	1.6%		99.6%	118%	89%	Max-Min

Barium
Ba

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	0.8%	0.8%	100.0%	90%	82%	
L04	1.4%	1.3%	100.0%	88%	83%	
L06	1.6%	2.0%	100.0%	94%	85%	
L07	0.9%	0.7%	100.0%	94%	89%	
L09	1.3%	1.8%	100.0%	108%	98%	
L10	0.7%	0.4%	100.0%	104%	97%	
L11	1.2%	1.4%	100.0%	89%	85%	
Ref	1.2%	1.1%	100.0%	111%	101%	
Mean	1.1%		100.0%	111%	82%	Max-Min

Cadmiun
Cd

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	1.4%	2.1%	100.0%	118%	110%	
L04	1.4%	1.1%	100.0%	115%	109%	
L06	1.5%	1.7%	100.0%	113%	107%	
L07	1.5%	1.5%	100.0%	110%	105%	
L09	1.1%	0.9%	100.0%	106%	95%	
L10	1.1%	1.5%	96.7%	96%	92%	
L11	1.1%	1.4%	100.0%	97%	94%	
Ref	1.1%	0.8%	100.0%	97%	86%	
Mean	1.2%		99.6%	118%	86%	Max-Min

CFS Contaminated Field Soil
Method 1313

Calcium
Ca

	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	1.1%	1.7%	100.0%	90%	89%	
L04	0.7%	0.7%	100.0%	92%	86%	
L06	1.4%	1.7%	100.0%	88%	82%	
L07	0.7%	0.5%	100.0%	90%	86%	
L09	0.6%	0.3%	100.0%	92%	85%	
L10	0.8%	0.4%	100.0%	87%	84%	
L11	1.0%	1.5%	100.0%	89%	83%	
Ref	1.0%	0.9%	100.0%	92%	84%	
Mean	0.9%		100.0%	92%	82%	Max-Min

Lead
Pb

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	0.9%	0.2%	100.0%	112%	94%	
L04	1.4%	1.4%	100.0%	98%	88%	
L06	2.7%	2.8%	96.3%	95%	89%	
L07	1.2%	1.1%	100.0%	92%	84%	
L09	1.1%	0.9%	100.0%	103%	99%	
L10	1.6%	1.8%	100.0%	97%	89%	
L11	1.4%	1.5%	100.0%	102%	95%	
Ref	1.7%	1.8%	100.0%	100%	85%	
Mean	1.5%		99.6%	112%	84%	Max-Min

Molybdenum
Mo

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	3.2%	3.1%	100.0%	111%	103%	
L04	3.4%	3.3%	96.3%	101%	96%	
L06	3.7%	4.0%	92.6%	91%	87%	
L07	3.1%	3.1%	100.0%	100%	91%	
L09	4.0%	4.1%	92.6%	93%	90%	
L10	4.3%	4.2%	93.3%	93%	88%	
L11	4.1%	3.8%	96.3%	89%	86%	
Ref	3.3%	3.1%	98.1%	107%	97%	
Mean	3.6%		96.4%	111%	86%	Max-Min

CFS Contaminated Field Soil
Method 1313

Selenium
Se

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	4.9%	2.7%	96.3%	99%	96%	
L04	4.7%	3.6%	96.3%	117%	111%	
L06	4.3%	2.1%	100.0%	112%	107%	
L07	3.9%	3.0%	92.6%	112%	96%	
L09	5.5%	3.2%	96.3%	100%	97%	
L10	5.0%	3.3%	93.3%	92%	87%	
L11	6.1%	2.9%	92.6%	90%	87%	
Ref	4.9%	1.8%	100.0%	103%	95%	
Mean	4.9%		96.4%	117%	87%	Max-Min

Vanadium
V

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	3.7%	2.5%	96.3%	115%	106%	
L04	2.9%	2.1%	100.0%	117%	110%	
L06	3.4%	2.2%	100.0%	112%	104%	
L07	3.7%	2.6%	100.0%	118%	110%	
L09	3.1%	1.8%	100.0%	104%	94%	
L10	3.8%	3.2%	96.7%	97%	89%	
L11	2.4%	1.9%	100.0%	104%	98%	
Ref	2.9%	1.6%	100.0%	106%	96%	
Mean	3.2%		99.2%	118%	89%	Max-Min

EaFA Coal Combustion Fly Ash
Method 1316

Overall Mean RSD	3.0%
Stdev of Mean RSDs	1.6%
Overall Mean Completeness	99%
Max Spike Recovery	120%
Min Spike Recovery	80%

Antimony
Sb

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	4.6%	2.3%	100.0%	104%	93%	
L02	3.8%	2.0%	100.0%	117%	110%	
L04	4.1%	2.5%	100.0%	117%	110%	
L05	4.9%	2.6%	100.0%	116%	102%	
L06	4.7%	2.0%	100.0%	106%	102%	
L07	3.8%	2.5%	100.0%	107%	105%	
L08	3.9%	2.9%	100.0%	109%	105%	
L09	5.0%	2.3%	100.0%	104%	100%	
L10	4.4%	2.6%	100.0%	95%	88%	
L11	4.1%	2.7%	100.0%	104%	99%	
Ref	6.2%	2.2%	100.0%	102%	96%	
Mean	4.7%		100.0%	117%	88%	Max-Min

Arsenic
As

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	7.5%	2.7%	100.0%	104%	94%	
L02	5.2%	3.1%	93.3%	115%	109%	
L04	5.6%	3.4%	93.3%	117%	112%	
L05	6.4%	4.2%	91.7%	113%	101%	
L06	6.1%	2.7%	93.3%	111%	104%	
L07	5.4%	3.1%	93.3%	109%	106%	
L08	5.4%	2.3%	100.0%	109%	105%	
L09	5.9%	2.6%	100.0%	104%	98%	
L10	6.1%	3.3%	93.3%	100%	92%	
L11	5.6%	3.0%	91.7%	103%	102%	
Ref	4.8%	3.0%	91.7%	117%	98%	
Mean	5.7%		94.4%	117%	92%	Max-Min

EaFA Coal Combustion Fly Ash
Method 1316

Boron
B

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	1.4%	0.9%	100.0%	86%	81%	
L02	2.4%	2.6%	100.0%	92%	88%	
L04	1.5%	0.5%	100.0%	91%	87%	
L05	1.8%	1.7%	100.0%	108%	87%	
L06	1.1%	0.9%	100.0%	94%	88%	
L07	1.4%	0.8%	100.0%	101%	87%	
L08	2.7%	2.9%	100.0%	90%	85%	
L09	2.0%	2.2%	100.0%	87%	84%	
L10	2.1%	1.6%	100.0%	90%	84%	
L11	1.4%	0.7%	100.0%	92%	87%	
Ref	1.3%	0.8%	100.0%	104%	88%	
Mean	1.7%		100.0%	108%	81%	Max-Min

Barium
Ba

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	1.0%	1.0%	100.0%	93%	83%	
L02	1.9%	2.1%	100.0%	104%	98%	
L04	0.8%	0.5%	100.0%	114%	110%	
L05	0.8%	0.6%	100.0%	101%	92%	
L06	1.4%	2.2%	100.0%	99%	94%	
L07	1.1%	1.1%	100.0%	100%	98%	
L08	2.3%	3.2%	100.0%	97%	95%	
L09	1.9%	2.8%	100.0%	94%	91%	
L10	1.7%	1.8%	100.0%	85%	80%	
L11	0.7%	0.4%	100.0%	96%	92%	
Ref	0.8%	1.1%	100.0%	97%	94%	
Mean	1.3%		100.0%	114%	80%	Max-Min

Calcium
Ca

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	1.1%	1.1%	100.0%	97%	91%	
L02	1.5%	1.4%	100.0%	91%	85%	
L04	1.0%	0.7%	100.0%	90%	86%	
L05	0.9%	0.5%	100.0%	90%	83%	
L06	1.6%	2.3%	100.0%	90%	83%	
L07	1.0%	1.0%	100.0%	85%	82%	
L08	2.4%	3.3%	100.0%	95%	85%	
L09	2.0%	2.5%	100.0%	89%	82%	
L10	1.5%	1.9%	100.0%	90%	83%	
L11	0.8%	0.5%	100.0%	93%	88%	
Ref	0.8%	1.2%	100.0%	93%	83%	
Mean	1.3%		100.0%	97%	82%	Max-Min

EaFA Coal Combustion Fly Ash
Method 1316

Chromium
Cr

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	5.0%	2.5%	100.0%	102%	92%	
L02	4.9%	2.4%	93.3%	112%	105%	
L04	4.1%	2.2%	100.0%	111%	106%	
L05	5.8%	2.5%	100.0%	109%	100%	
L06	4.3%	2.5%	100.0%	108%	101%	
L07	5.1%	2.9%	100.0%	107%	104%	
L08	5.4%	3.2%	100.0%	103%	101%	
L09	4.4%	2.6%	100.0%	103%	100%	
L10	4.8%	2.6%	100.0%	91%	86%	
L11	1.0%	0.5%	100.0%	100%	95%	
Ref	3.0%	1.6%	100.0%	111%	101%	
Mean	4.2%		99.4%	112%	86%	Max-Min

Cobalt
Co

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	4.1%	2.6%	100.0%	105%	95%	
L02	4.1%	2.8%	93.3%	111%	107%	
L04	3.3%	1.9%	100.0%	109%	103%	
L05	2.7%	2.1%	100.0%	110%	100%	
L06	2.9%	2.2%	100.0%	107%	101%	
L07	3.1%	2.2%	100.0%	106%	102%	
L08	3.3%	3.0%	100.0%	103%	101%	
L09	3.3%	2.0%	100.0%	103%	99%	
L10	3.4%	2.9%	100.0%	92%	87%	
L11	5.0%	2.2%	100.0%	101%	96%	
Ref	3.4%	1.8%	100.0%	111%	101%	
Mean	3.5%		99.4%	111%	87%	Max-Min

Molybdenum
Mo

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	1.1%	1.2%	100.0%	89%	83%	
L02	2.1%	2.2%	100.0%	110%	92%	
L04	1.0%	0.7%	100.0%	102%	94%	
L05	0.9%	0.8%	100.0%	105%	99%	
L06	1.4%	2.2%	100.0%	93%	82%	
L07	1.1%	1.0%	100.0%	95%	81%	
L08	2.2%	3.0%	100.0%	96%	83%	
L09	1.7%	2.5%	100.0%	95%	82%	
L10	1.5%	1.9%	100.0%	96%	87%	
L11	0.8%	0.5%	100.0%	88%	86%	
Ref	0.9%	1.2%	100.0%	99%	91%	
Mean	1.3%		100.0%	110%	81%	Max-Min

EaFA Coal Combustion Fly Ash
Method 1316

Selenium
Se

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	2.3%	1.3%	100.0%	97%	86%	
L02	4.6%	3.3%	93.3%	120%	102%	
L04	2.3%	0.9%	100.0%	110%	103%	
L05	2.9%	1.5%	100.0%	111%	101%	
L06	2.9%	1.1%	100.0%	106%	100%	
L07	2.2%	1.8%	100.0%	106%	100%	
L08	2.7%	3.2%	100.0%	107%	99%	
L09	2.5%	1.9%	100.0%	102%	96%	
L10	2.4%	2.5%	100.0%	95%	86%	
L11	2.7%	1.2%	100.0%	102%	96%	
Ref	3.0%	1.8%	100.0%	94%	87%	
Mean	2.8%		99.4%	120%	86%	Max-Min

Vanadium
V

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	1.3%	0.8%	100.0%	100%	91%	
L02	2.1%	2.1%	100.0%	112%	105%	
L04	1.6%	1.0%	100.0%	112%	107%	
L05	1.1%	1.0%	100.0%	110%	99%	
L06	1.8%	1.9%	100.0%	109%	103%	
L07	1.7%	0.9%	100.0%	109%	106%	
L08	2.7%	3.3%	100.0%	104%	102%	
L09	2.5%	2.6%	100.0%	108%	103%	
L10	2.0%	2.0%	100.0%	90%	84%	
L11	1.9%	1.0%	100.0%	100%	96%	
Ref	1.9%	1.3%	100.0%	111%	101%	
Mean	1.9%		100.0%	112%	84%	Max-Min

SWA Solidified Waste Analog
Method 1316

Overall Mean RSD	1.5%
Stdev of Mean RSDs	0.7%
Overall Mean Completeness	100%
Max Spike Recovery	120%
Min Spike Recovery	83%

Antimony
Sb

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	0.8%	0.3%	100.0%	95%	92%	
L02	1.3%	0.9%	100.0%	99%	95%	
L04	1.5%	1.3%	100.0%	114%	110%	
L05	1.1%	0.8%	100.0%	98%	91%	
L06	1.4%	1.1%	100.0%	92%	86%	
L07	1.2%	0.9%	100.0%	105%	84%	
L09	0.7%	0.3%	100.0%	92%	88%	
L10	0.9%	0.5%	100.0%	101%	92%	
L11	3.5%	3.1%	100.0%	93%	87%	
Ref	1.8%	1.5%	100.0%	104%	99%	
Mean	1.4%		100.0%	114%	84%	Max-Min

Arsenic
As

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	1.0%	0.4%	100.0%	109%	88%	
L02	1.1%	0.6%	100.0%	91%	85%	
L04	1.0%	0.6%	100.0%	97%	87%	
L05	1.4%	1.3%	100.0%	92%	88%	
L06	0.9%	0.5%	100.0%	92%	87%	
L07	0.6%	0.3%	100.0%	102%	84%	
L09	1.0%	0.8%	100.0%	92%	90%	
L10	1.0%	0.6%	100.0%	101%	90%	
L11	0.9%	0.4%	100.0%	99%	93%	
Ref	2.1%	2.0%	100.0%	105%	100%	
Mean	1.2%		100.0%	109%	84%	Max-Min

SWA Solidified Waste Analog
Method 1316

Boron
B

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	1.0%	0.3%	100.0%	108%	106%	
L02	0.9%	0.4%	100.0%	104%	94%	
L04	0.9%	0.6%	100.0%	104%	96%	
L05	1.0%	0.7%	100.0%	107%	86%	
L06	0.6%	0.5%	100.0%	118%	97%	
L07	0.7%	0.4%	100.0%	101%	91%	
L09	0.6%	0.3%	100.0%	98%	90%	
L10	1.0%	0.7%	100.0%	93%	88%	
L11	0.5%	0.2%	100.0%	94%	90%	
Ref	2.0%	1.9%	100.0%	105%	89%	
Mean	1.0%		100.0%	118%	86%	Max-Min

Barium
Ba

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	1.4%	1.3%	100.0%	86%	85%	
L02	0.7%	0.4%	100.0%	94%	85%	
L04	2.2%	2.4%	100.0%	120%	117%	
L05	1.4%	1.8%	100.0%	95%	90%	
L06	1.2%	1.2%	100.0%	94%	93%	
L07	0.9%	0.8%	100.0%	94%	85%	
L09	1.0%	0.6%	100.0%	95%	86%	
L10	0.9%	0.7%	100.0%	104%	95%	
L11	0.5%	0.5%	100.0%	100%	90%	
Ref	2.7%	2.1%	100.0%	93%	85%	
Mean	1.4%		100.0%	120%	85%	Max-Min

Calcium
Ca

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	1.2%	0.9%	100.0%	105%	101%	
L02	1.2%	0.7%	100.0%	92%	87%	
L04	1.3%	1.0%	100.0%	115%	92%	
L05	1.8%	1.4%	100.0%	94%	91%	
L06	1.9%	1.5%	100.0%	93%	88%	
L07	1.7%	1.8%	100.0%	93%	85%	
L09	2.4%	2.6%	100.0%	89%	87%	
L10	1.0%	0.6%	100.0%	112%	92%	
L11	0.5%	0.3%	100.0%	95%	91%	
Ref	3.1%	2.7%	100.0%	90%	86%	
Mean	1.8%		100.0%	115%	85%	Max-Min

SWA Solidified Waste Analog
Method 1316

Chromium
Cr

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	1.0%	0.7%	100.0%	103%	90%	
L02	0.9%	0.4%	100.0%	109%	92%	
L04	1.3%	0.9%	100.0%	102%	89%	
L05	1.4%	1.3%	100.0%	98%	94%	
L06	0.9%	0.3%	100.0%	108%	91%	
L07	0.8%	0.5%	100.0%	103%	99%	
L09	0.8%	0.4%	100.0%	95%	89%	
L10	0.7%	0.4%	100.0%	112%	108%	
L11	1.0%	0.4%	100.0%	92%	88%	
Ref	3.3%	3.0%	100.0%	87%	86%	
Mean	1.4%		100.0%	112%	86%	Max-Min

Cobalt
Co

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	3.8%	0.3%	100.0%	105%	101%	
L02	2.3%	1.0%	100.0%	105%	95%	
L04	7.7%	3.5%	100.0%	116%	108%	
L05	0.0%	0.0%	100.0%	92%	89%	
L06	3.8%	0.0%	100.0%	113%	110%	
L07	5.2%	2.1%	100.0%	93%	83%	
L09	7.4%	4.5%	100.0%	100%	93%	
L10	2.6%	1.9%	100.0%	111%	93%	
L11	0.0%	0.0%	100.0%	100%	99%	
Ref	1.8%	0.0%	100.0%	112%	103%	
Mean	3.3%		100.0%	116%	83%	Max-Min

Molybdenum
Mo

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	0.7%	0.4%	100.0%	112%	110%	
L02	0.9%	0.4%	100.0%	95%	89%	
L04	1.1%	0.6%	100.0%	117%	111%	
L05	1.4%	1.1%	100.0%	111%	106%	
L06	0.7%	0.3%	100.0%	117%	112%	
L07	1.1%	0.9%	100.0%	99%	92%	
L09	0.7%	0.4%	100.0%	103%	88%	
L10	1.1%	1.0%	100.0%	90%	84%	
L11	0.8%	0.5%	100.0%	100%	98%	
Ref	1.9%	1.7%	100.0%	113%	105%	
Mean	1.1%		100.0%	117%	84%	Max-Min

SWA Solidified Waste Analog
Method 1316

Selenium
Se

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	0.6%	0.3%	100.0%	113%	85%	
L02	0.8%	0.5%	100.0%	96%	88%	
L04	0.6%	0.3%	100.0%	118%	102%	
L05	0.9%	0.9%	100.0%	92%	86%	
L06	0.7%	0.4%	100.0%	96%	87%	
L07	0.5%	0.3%	100.0%	98%	87%	
L09	0.6%	0.3%	100.0%	101%	92%	
L10	0.8%	0.6%	100.0%	85%	83%	
L11	0.4%	0.1%	100.0%	109%	87%	
Ref	1.7%	0.0%	100.0%	99%	95%	
Mean	0.8%		100.0%	118%	83%	Max-Min

Vanadium
V

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	0.7%	0.4%	100.0%	105%	103%	
L02	0.9%	0.5%	100.0%	107%	103%	
L04	1.1%	0.6%	100.0%	112%	105%	
L05	1.5%	1.3%	100.0%	104%	94%	
L06	1.0%	0.6%	100.0%	115%	108%	
L07	0.7%	0.5%	100.0%	92%	83%	
L09	0.8%	0.3%	100.0%	102%	94%	
L10	0.7%	0.4%	100.0%	95%	90%	
L11	1.1%	0.5%	100.0%	94%	94%	
Ref	1.7%	1.6%	100.0%	111%	101%	
Mean	1.1%		100.0%	115%	83%	Max-Min

CFS Contaminated Field Soil
Method 1316

Overall Mean RSD	3.0%
Stdev of Mean RSDs	2.2%
Overall Mean Completeness	98%
Max Spike Recovery	115%
Min Spike Recovery	82%

Antimony
Sb

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	6.0%	3.3%	93.3%	102%	100%	
L04	4.9%	3.4%	93.3%	105%	103%	
L06	5.2%	3.7%	93.3%	101%	96%	
L07	5.3%	3.0%	93.3%	98%	96%	
L09	5.6%	2.5%	93.3%	103%	101%	
L10	5.7%	3.5%	93.3%	110%	97%	
L11	5.7%	2.9%	93.3%	89%	87%	
Ref	6.8%	3.5%	91.7%	113%	99%	
Mean	5.8%		93.0%	113%	87%	Max-Min

Arsenic
As

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	6.8%	3.3%	93.3%	106%	102%	
L04	7.4%	2.5%	93.3%	108%	102%	
L06	6.0%	2.6%	100.0%	104%	99%	
L07	4.4%	2.6%	100.0%	98%	96%	
L09	5.1%	2.3%	100.0%	103%	101%	
L10	6.5%	3.7%	100.0%	113%	99%	
L11	4.8%	2.2%	100.0%	90%	89%	
Ref	4.5%	2.9%	100.0%	113%	99%	
Mean	5.5%		98.5%	113%	89%	Max-Min

CFS Contaminated Field Soil
Method 1316

Boron
B

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	0.7%	0.5%	100.0%	97%	95%	
L04	1.1%	0.6%	100.0%	99%	97%	
L06	0.8%	0.4%	100.0%	98%	94%	
L07	1.2%	1.4%	100.0%	104%	93%	
L09	0.6%	0.4%	100.0%	104%	102%	
L10	1.0%	0.5%	100.0%	95%	93%	
L11	1.7%	1.2%	100.0%	92%	87%	
Ref	1.9%	1.3%	100.0%	108%	93%	
Mean	1.2%		100.0%	108%	87%	Max-Min

Barium
Ba

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	0.4%	0.3%	100.0%	96%	92%	
L04	0.7%	0.6%	100.0%	90%	87%	
L06	0.6%	0.3%	100.0%	109%	104%	
L07	1.2%	1.6%	100.0%	107%	97%	
L09	0.6%	0.4%	100.0%	108%	106%	
L10	0.8%	0.3%	100.0%	105%	98%	
L11	1.1%	1.0%	100.0%	94%	84%	
Ref	1.2%	1.1%	100.0%	115%	100%	
Mean	0.9%		100.0%	115%	84%	Max-Min

Cadmium
Cd

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	0.6%	0.4%	100.0%	110%	95%	
L04	0.5%	0.3%	100.0%	96%	89%	
L06	0.5%	0.3%	100.0%	90%	87%	
L07	1.3%	1.8%	100.0%	103%	85%	
L09	0.7%	0.4%	100.0%	96%	88%	
L10	0.7%	0.3%	100.0%	99%	95%	
L11	0.8%	0.5%	100.0%	103%	98%	
Ref	1.5%	1.4%	100.0%	103%	90%	
Mean	0.9%		100.0%	110%	85%	Max-Min

CFS Contaminated Field Soil
Method 1316

Calcium
Ca

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	0.7%	0.3%	100.0%	88%	83%	
L04	0.5%	0.2%	100.0%	92%	88%	
L06	0.5%	0.2%	100.0%	89%	85%	
L07	1.1%	1.5%	100.0%	89%	85%	
L09	0.7%	0.4%	100.0%	92%	87%	
L10	0.8%	0.3%	100.0%	91%	85%	
L11	0.7%	0.5%	100.0%	92%	82%	
Ref	1.1%	0.7%	100.0%	90%	86%	
Mean	0.8%		100.0%	92%	82%	Max-Min

Lead
Pb

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	0.8%	0.4%	100.0%	87%	83%	
L04	0.8%	0.7%	100.0%	87%	82%	
L06	0.7%	0.4%	100.0%	87%	83%	
L07	1.4%	1.3%	100.0%	95%	86%	
L09	0.6%	0.4%	100.0%	94%	93%	
L10	1.0%	0.4%	100.0%	98%	89%	
L11	1.1%	0.8%	100.0%	105%	90%	
Ref	1.9%	2.4%	95.8%	98%	83%	
Mean	1.1%		99.1%	105%	82%	Max-Min

Molybdenum
Mo

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	6.3%	5.0%	93.3%	98%	94%	
L04	5.5%	2.8%	100.0%	103%	100%	
L06	5.4%	2.5%	100.0%	98%	92%	
L07	6.3%	2.0%	100.0%	96%	94%	
L09	4.7%	2.5%	93.3%	101%	99%	
L10	4.3%	2.7%	100.0%	106%	97%	
L11	6.1%	3.3%	93.3%	98%	94%	
Ref	5.7%	2.8%	95.8%	114%	98%	
Mean	5.6%		96.9%	114%	92%	Max-Min

CFS Contaminated Field Soil
Method 1316

Selenium
Se

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	3.8%	2.3%	100.0%	101%	96%	
L04	4.9%	3.4%	93.3%	104%	102%	
L06	4.2%	3.5%	93.3%	98%	91%	
L07	4.9%	3.2%	93.3%	100%	95%	
L09	4.9%	3.2%	93.3%	101%	100%	
L10	4.4%	2.4%	100.0%	105%	93%	
L11	4.9%	2.9%	93.3%	94%	92%	
Ref	5.2%	2.4%	95.8%	109%	97%	
Mean	4.7%		95.4%	109%	91%	Max-Min

Vanadium
V

Lab#	Mean RSD	Stdev RSD	Complete	Spike Rec Max	Spike Rec Min	
L01	4.4%	2.6%	100.0%	97%	93%	
L04	2.6%	1.7%	100.0%	103%	101%	
L06	3.5%	2.1%	100.0%	97%	93%	
L07	4.5%	3.0%	100.0%	95%	93%	
L09	3.7%	1.7%	100.0%	101%	99%	
L10	3.6%	2.1%	100.0%	110%	96%	
L11	3.0%	2.4%	100.0%	101%	99%	
Ref	3.2%	1.9%	100.0%	114%	98%	
Mean	3.5%		100.0%	114%	93%	Max-Min

Appendix I. QA/QC Reports for Analytical Samples

TABLE OF CONTENTS ..... **I-i**

INTRODUCTION **I-1**

ORGANIZATION OF THE QA/QC TABLES **I-1**

DESCRIPTION OF THE COLUMNS IN THE ANALYTICAL QA/QC TABLES **I-1**

Method 1313: Liquid-Solid Partitioning as a Function of Eluate pH using a Parallel Batch Extraction Procedure

EaFA – Coal Combustion Fly Ash ***I-4***

L01 ..... I-4
L02 ..... I-33
L04 ..... I-62
L05 ..... I-91
L06 ..... I-120
L07 ..... I-149
L08 ..... I-178
L09 ..... I-207
L10 ..... I-236
L11 ..... I-265
Ref I-294

SWA – Solidified Waste Analog ***I-352***

L01 ..... I-352
L02 ..... I-381
L04 ..... I-410
L05 ..... I-439
L06 ..... I-468
L07 ..... I-497
L09 ..... I-526
L10 ..... I-555
L11 ..... I-584
Ref I-613

CFS – Contaminated Field Soil ***I-671***

L01 ..... I-671
L04 ..... I-700
L06 ..... I-729
L07 ..... I-758
L09 ..... I-787
L10 ..... I-816
L11 ..... I-845
Ref I-874

Method 1316: Liquid-Solid Partitioning as a Function of Liquid-Solid using a Parallel Batch Extraction Procedure

EaFA – Coal Combustion Fly Ash ***I-932***
L01 ..... I-932
L02 ..... I-961
L04 ..... I-990
L05 ..... I-1019
L06 ..... I-1048
L07 ..... I-1077
L08 ..... I-1106
L09 ..... I-1135
L10 ..... I-1164
L11 ..... I-1193
Ref I-1222

SWA – Solidified Waste Analog ***I-1280***
L01 ..... I-1280
L02 ..... I-1309
L04 ..... I-1338
L05 ..... I-1367
L06 ..... I-1396
L07 ..... I-1425
L09 ..... I-1454
L10 ..... I-1483
L11 ..... I-1512
Ref I-1541

CFS – Contaminated Field Soil ***I-1599***
L01 ..... I-1599
L04 ..... I-1628
L06 ..... I-1657
L07 ..... I-1686
L09 ..... I-1715
L10 ..... I-1744
L11 ..... I-1773
Ref I-1802

INTRODUCTION

The tables in this appendix present the quality assurance/quality control results for the analytical measurement of eluate concentrations from the preserved eluates submitted by each of the validation laboratories. The data shown in this appendix is applicable only to the analytical solutions measured by inductively coupled plasma – optical emissions spectrometry (ICP-OES) performed by Vanderbilt University (VU). The analytical methods, instrument calibration, and analytical QA/QC program followed throughout this project are detailed in the main report.

ORGANIZATION OF THE QA/QC TABLES

Each table in the appendix represents the final eluate solution concentrations for a single element from a single laboratory. The tables are ordered alphabetically by element symbol (e.g., "Al" for aluminum or "Sb" for antimony) for each validation laboratory code (e.g., "L01" for Laboratory 1 or "LRef" for reference laboratory) within each the leaching method (i.e., Method 1313 versus Method 1316). The information within each table is ordered by the test position number within each leaching method.

DESCRIPTION OF THE COLUMNS IN THE ANALYTICAL QA/QC TABLES

The following is a description of the columns in each table in the appendix.

Element (1st Column)

Element symbol identifiers based on the periodic chart.

Sample (2nd Column)

Coded identifier for each sample comprised of the following items separated by dashes:

- material code (e.g., "CFS", "SWA", or "JaFS")
- laboratory code (e.g., "L01" for Laboratory 1 or "LRef" for reference laboratory)
- method code (e.g., "1314" for Method 1314)
- test position number (e.g., "T01" for first eluate of the test)
- replicate letter (e.g., "A" for first test run)

Dilution Factor (3rd Column)

The dilution factor for the analytical sample measured in the instrument or the multiplier associated with calculating final eluate concentrations from analytical sample concentration. Typically for ICP-OES, full strength analytical samples are measured and the resultant dilution factor is "1". However, dilution factors of at least "10" are common for inductively coupled plasma – mass spectrometry (ICP-MS) analysis in order to minimize interferences from analytical solutions with high sodium and potassium content.

Sample Conc. in µg/L (4th Column)

The concentration of the analytical sample in µg/L as measured by the analytical method specified in the 14th Column.

Qualifier (5th Column)

A quality control qualifier used to flag analytical samples that are below the quantification or detection limits. The following table of qualifiers was used.

Qualifier	Meaning
E	Estimated value between the MDL and ML values
U	Non-detected values below the MDL
U1/2	Non-detected values below the MDL set to ½ the MDL for graphing purposes

Internal Review (6th Column)

A column used by the Vanderbilt University Laboratory Manager to mark issues with QA/QC for internal checks.

ICP-OES Conc. (7th Column)

The final eluate concentration used in the validation study determined by multiplying the analytical sample concentration (4th Column) by the dilution factor (3rd Column).

RSD (8th Column)

Relative standard deviation of the three analytical measurements of the sample analytical sample calculated automatically through instrument software. The RSD does not represent the relative standard deviation of replicate analysis using triplicate samples.

MDL (9th Column)

The method detection limit (MDL) in µg/L for the analysis using the analytical method specified in the 14th Column. The value is calculated by the VU laboratory manager based on the standard deviation of analysis of seven low-level standard solutions measured on seven non-consecutive days and the Student's *t*-distribution value for the seven replicates at the 99% confidence level (EPA, 2003).

$$MDL = S_{(n=7)} \times t_{(n-1=6,1-\alpha=0.99)}$$

where $S_{(n=7)}$ is the standard deviation of seven non-consecutive measurements (µg/L), and $t_{(n-1=6,1-\alpha=0.99)}$ is the Student *t*-distribution value for seven replicates at the 99% confidence level (3.14267).

ML (10th Column)

The estimated minimum level of quantification (ML) in µg/L for the analysis using the analytical method specified in the 14th Column. The value is calculated by the VU laboratory manager based on the previously calculated MDL (EPA, 2003).

$$ML = 3.18 \times MDL$$

Spike Conc. (11th Column) and Spike Volume (12th Column)

The concentration in µg/L of the standard solution used to spike analytical samples and the volume of the standard solution added to each analytical sample. When multiplied, these values provide the theoretical mass of an element that is spiked into an analytical sample.

$$M_{QA/QC\ spike} = C_{std} \times \left(V_{std} \times \frac{\mathrm{L}}{10^6\ \mu\mathrm{L}} \right)$$

where $M_{QA/QC\ spike}$ is the theoretical mass of spiked into the analytical sample (µg),
C_{std} is the concentration of the standard solution (µg/L), and
V_{std} is the volume of the standard solution added to the analytical sample (µL).

Spike Conc. (13th Column)

The concentration of the spiked analytical solution in µg/L as measured by the analytical method specified in the 14th Column.

Spike Recovery (14th Column)

The percentage of spiked mass recovered during analysis of the spiked solution. The spike recovery is calculated by the VU laboratory manager using the following formula:

$$\frac{\left(C_{QA/QC\ spike} - C_{sample}\right) \times V_{QA/QC\ spike}}{M_{QA/AC\ spike}} \times 100\%$$

where $C_{QA/QC\ spike}$ is the concentration of the spiked analytical sample (µg/L),
C_{sample} is the concentration of the analytical sample in the 4th Column (µg/L), and
$V_{QA/QC\ spike}$ is the final volume of the spiked analytical sample (L).

Instrument (15th Column)

The instrument used for the analytical measurement (e.g., "VU ICP-OES" denotes that the instrument was the Vanderbilt University Varian 620 ICP-OES).

Date/Time (16th Column)

The date and time that the analytical sample measurement was recorded by the instrument software. This column is used to uniquely identify each analysis and does not reflect the data and time of spiked solution measurement.

Filename (17th Column)

The name of the instrument output file where the analytical data is stored.

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	EaFA-L01-1313-T01-A	1	4.33E+04			4.33E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T02-A	1	3.22E+04			3.22E+04	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T03-A	1	2.03E+04			2.03E+04	2.2E-01	1.0E+00	3.2E+00	1000	100	2.13E+04	94%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T04-A	1	8.48E+03			8.48E+03	1.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T05-A	1	1.37E+03			1.37E+03	4.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T06-A	1	1.15E+02			1.15E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T07-A	1	2.29E+03			2.29E+03	2.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T08-A	1	2.94E+04			2.94E+04	2.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T09-A	1	1.34E+05			1.34E+05	4.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T01-B	1	3.84E+04			3.84E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T02-B	1	3.18E+04			3.18E+04	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T03-B	1	1.97E+04			1.97E+04	6.9E-01	1.0E+00	3.2E+00	1000	100	2.07E+04	97%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T04-B	1	8.19E+03			8.19E+03	2.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T05-B	1	1.36E+03			1.36E+03	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T06-B	1	1.36E+02			1.36E+02	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T07-B	1	2.82E+03			2.82E+03	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T08-B	1	3.04E+04			3.04E+04	1.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T09-B	1	1.33E+05			1.33E+05	2.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T01-C	1	3.75E+04			3.75E+04	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T02-C	1	2.83E+04			2.83E+04	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T03-C	1	2.18E+04			2.18E+04	4.7E-01	1.0E+00	3.2E+00	1000	100	2.27E+04	91%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T04-C	1	8.28E+03			8.28E+03	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T05-C	1	1.30E+03			1.30E+03	6.5E-01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T06-C	1	1.18E+02			1.18E+02	1.6E+00	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T07-C	1	2.31E+03			2.31E+03	8.5E-01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T08-C	1	2.71E+04			2.71E+04	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-T09-C	1	1.29E+05			1.29E+05	6.8E-01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.0E+01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	2.1E+01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	2.8E+01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	EaFA-L01-1313-T01-A	1	2.97E+02			2.97E+02	5.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T02-A	1	1.93E+02			1.93E+02	1.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T03-A	1	2.58E+02			2.58E+02	6.9E+00	7.5E+00	2.4E+01	10	325	3.68E+03	105%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T04-A	1	1.93E+02			1.93E+02	4.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T05-A	1	2.28E+02			2.28E+02	3.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T06-A	1	2.33E+02			2.33E+02	2.4E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T07-A	1	8.10E+01			8.10E+01	2.8E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T08-A	1	3.44E+01			3.44E+01	1.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T09-A	1	3.75E+00	U1/2		3.75E+00	7.3E+02	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T01-B	1	2.29E+02			2.29E+02	6.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T02-B	1	1.31E+02			1.31E+02	8.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T03-B	1	1.94E+02			1.94E+02	8.9E+00	7.5E+00	2.4E+01	10	325	3.55E+03	103%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T04-B	1	2.01E+02			2.01E+02	9.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T05-B	1	2.02E+02			2.02E+02	7.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T06-B	1	1.76E+02			1.76E+02	1.4E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T07-B	1	6.91E+01			6.91E+01	1.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T08-B	1	2.04E+01	E		2.04E+01	2.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T09-B	1	3.75E+00	U1/2		3.75E+00	3.9E+02	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T01-C	1	2.73E+02			2.73E+02	1.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T02-C	1	1.47E+02			1.47E+02	1.9E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T03-C	1	2.09E+02			2.09E+02	7.2E+00	7.5E+00	2.4E+01	10	325	3.51E+03	101%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T04-C	1	1.87E+02			1.87E+02	6.1E+00	7.5E+00	2.4E+01					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T05-C	1	2.04E+02			2.04E+02	1.3E+01	7.5E+00	2.4E+01					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T06-C	1	1.82E+02			1.82E+02	6.0E+00	7.5E+00	2.4E+01					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T07-C	1	6.74E+01			6.74E+01	3.5E+01	7.5E+00	2.4E+01					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T08-C	1	2.67E+01			2.67E+01	8.5E+01	7.5E+00	2.4E+01					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-T09-C	1	3.75E+00	U1/2		3.75E+00	3.4E+01	7.5E+00	2.4E+01					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-B01-A	1	8.66E+00	E		8.66E+00	9.1E+02	7.5E+00	2.4E+01					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-B02-A	1	1.90E+01	E		1.90E+01	7.0E+00	7.5E+00	2.4E+01					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1313-B03-A	1	3.75E+00	U1/2		3.75E+00	4.6E+01	7.5E+00	2.4E+01					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	EaFA-L01-1313-T01-A	1	1.31E+04			1.31E+04	8.5E-01	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T02-A	1	9.09E+02			9.09E+02	7.9E-01	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T03-A	1	9.94E+02			9.94E+02	2.1E+00	1.1E+01	3.5E+01	10	325	4.40E+03	105%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T04-A	1	6.53E+02			6.53E+02	4.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T05-A	1	3.47E+02			3.47E+02	9.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T06-A	1	1.69E+02			1.69E+02	9.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T07-A	1	1.62E+02			1.62E+02	9.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T08-A	1	1.45E+02			1.45E+02	7.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T09-A	1	4.28E+03			4.28E+03	9.0E-01	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T01-B	1	1.19E+04			1.19E+04	1.7E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T02-B	1	9.18E+02			9.18E+02	2.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T03-B	1	1.11E+03			1.11E+03	1.6E+00	1.1E+01	3.5E+01	10	325	4.41E+03	102%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T04-B	1	6.24E+02			6.24E+02	4.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T05-B	1	3.59E+02			3.59E+02	5.7E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T06-B	1	1.13E+02			1.13E+02	1.0E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T07-B	1	1.45E+02			1.45E+02	8.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T08-B	1	1.73E+02			1.73E+02	8.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T09-B	1	3.91E+03			3.91E+03	3.0E-01	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T01-C	1	1.18E+04			1.18E+04	8.8E-01	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T02-C	1	7.70E+02			7.70E+02	2.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T03-C	1	1.24E+03			1.24E+03	2.0E+00	1.1E+01	3.5E+01	10	325	4.52E+03	101%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T04-C	1	6.18E+02			6.18E+02	5.8E+00	1.1E+01	3.5E+01					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T05-C	1	3.35E+02			3.35E+02	3.5E+00	1.1E+01	3.5E+01					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T06-C	1	1.04E+02			1.04E+02	1.6E+01	1.1E+01	3.5E+01					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T07-C	1	1.30E+02			1.30E+02	1.5E+01	1.1E+01	3.5E+01					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T08-C	1	1.36E+02			1.36E+02	8.4E+00	1.1E+01	3.5E+01					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-T09-C	1	4.18E+03			4.18E+03	5.7E-01	1.1E+01	3.5E+01					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-B01-A	1	5.50E+00	U1/2		5.50E+00	8.6E+01	1.1E+01	3.5E+01					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-B02-A	1	5.50E+00	U1/2		5.50E+00	1.2E+03	1.1E+01	3.5E+01					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1313-B03-A	1	3.56E+01			3.56E+01	1.1E+02	1.1E+01	3.5E+01					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	EaFA-L01-1313-T01-A	1	4.95E+03			4.95E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T02-A	1	4.50E+03			4.50E+03	4.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T03-A	1	4.29E+03			4.29E+03	1.1E+00	1.0E+00	3.2E+00	1000	100	5.18E+03	88%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T04-A	1	4.55E+03			4.55E+03	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T05-A	1	4.30E+03			4.30E+03	4.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T06-A	1	4.73E+03			4.73E+03	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T07-A	1	4.33E+03			4.33E+03	2.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T08-A	1	3.77E+03			3.77E+03	5.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T09-A	1	2.77E+03			2.77E+03	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T01-B	1	4.66E+03			4.66E+03	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T02-B	1	4.33E+03			4.33E+03	8.0E-02	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T03-B	1	4.29E+03			4.29E+03	1.0E+00	1.0E+00	3.2E+00	1000	100	5.10E+03	81%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T04-B	1	4.22E+03			4.22E+03	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T05-B	1	4.34E+03			4.34E+03	9.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T06-B	1	4.52E+03			4.52E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T07-B	1	3.92E+03			3.92E+03	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T08-B	1	3.81E+03			3.81E+03	3.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T09-B	1	2.85E+03			2.85E+03	3.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T01-C	1	4.66E+03			4.66E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T02-C	1	4.05E+03			4.05E+03	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T03-C	1	4.31E+03			4.31E+03	9.2E-01	1.0E+00	3.2E+00	1000	100	5.16E+03	86%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T04-C	1	4.38E+03			4.38E+03	2.4E-01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T05-C	1	4.11E+03			4.11E+03	5.7E-01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T06-C	1	4.37E+03			4.37E+03	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T07-C	1	3.87E+03			3.87E+03	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T08-C	1	3.58E+03			3.58E+03	1.6E+00	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-T09-C	1	2.75E+03			2.75E+03	4.9E-01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-B01-A	1	8.97E+01			8.97E+01	2.9E+00	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-B02-A	1	9.08E+01			9.08E+01	7.4E-01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1313-B03-A	1	2.93E+01			2.93E+01	4.9E+00	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	EaFA-L01-1313-T01-A	1	1.35E+03			1.35E+03	7.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T02-A	1	9.72E+02			9.72E+02	8.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T03-A	1	7.87E+02			7.87E+02	9.9E-02	1.0E+00	3.2E+00	10	325	3.91E+03	96%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T04-A	1	6.21E+02			6.21E+02	1.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T05-A	1	3.29E+02			3.29E+02	4.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T06-A	1	2.42E+02			2.42E+02	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T07-A	1	2.27E+02			2.27E+02	1.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T08-A	1	2.72E+02			2.72E+02	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T09-A	1	9.74E+02			9.74E+02	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T01-B	1	1.52E+03			1.52E+03	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T02-B	1	9.61E+02			9.61E+02	9.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T03-B	1	7.46E+02			7.46E+02	5.9E-01	1.0E+00	3.2E+00	10	325	3.68E+03	90%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T04-B	1	5.98E+02			5.98E+02	1.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T05-B	1	3.27E+02			3.27E+02	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T06-B	1	2.47E+02			2.47E+02	1.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T07-B	1	2.30E+02			2.30E+02	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T08-B	1	2.67E+02			2.67E+02	1.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T09-B	1	9.43E+02			9.43E+02	1.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T01-C	1	1.36E+03			1.36E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T02-C	1	8.60E+02			8.60E+02	2.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T03-C	1	6.24E+02			6.24E+02	5.3E-01	1.0E+00	3.2E+00	10	325	3.54E+03	90%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T04-C	1	5.95E+02			5.95E+02	8.0E-01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T05-C	1	2.99E+02			2.99E+02	3.2E-01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T06-C	1	2.42E+02			2.42E+02	2.6E-01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T07-C	1	2.12E+02			2.12E+02	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T08-C	1	2.49E+02			2.49E+02	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-T09-C	1	9.48E+02			9.48E+02	3.6E-01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	3.4E+01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-B02-A	1	1.01E+01			1.01E+01	1.4E+01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	2.9E+00	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	EaFA-L01-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	1.4E+01	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	5.2E+02	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	2.2E+02	1.9E+00	6.0E+00	10	325	3.50E+03	108%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	2.3E+01	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	3.3E+02	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T07-A	1	2.26E+01			2.26E+01	2.1E+00	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T08-A	1	1.24E+02			1.24E+02	2.7E-01	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T09-A	1	2.64E+02			2.64E+02	2.3E-01	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	2.5E+01	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	1.6E+02	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	8.4E+01	1.9E+00	6.0E+00	10	325	3.40E+03	105%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	6.9E+01	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	9.8E+01	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	2.7E+02	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T07-B	1	2.56E+01			2.56E+01	1.2E+00	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T08-B	1	1.26E+02			1.26E+02	3.8E-01	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T09-B	1	2.63E+02			2.63E+02	1.1E+00	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	8.5E+00	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	2.1E+03	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	7.2E+01	1.9E+00	6.0E+00	10	325	3.38E+03	104%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	7.2E+01	1.9E+00	6.0E+00					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	5.2E+01	1.9E+00	6.0E+00					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	2.0E+02	1.9E+00	6.0E+00					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T07-C	1	2.09E+01			2.09E+01	6.8E-01	1.9E+00	6.0E+00					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T08-C	1	1.15E+02			1.15E+02	1.3E+00	1.9E+00	6.0E+00					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-T09-C	1	2.53E+02			2.53E+02	1.3E+00	1.9E+00	6.0E+00					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	3.6E+01	1.9E+00	6.0E+00					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	3.0E+02	1.9E+00	6.0E+00					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	9.5E+01	1.9E+00	6.0E+00					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	EaFA-L01-1313-T01-A	1	1.10E+00	U1/2		1.10E+00	1.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T02-A	1	1.10E+00	U1/2		1.10E+00	1.3E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	9.6E-01	2.2E+00	7.0E+00	10	325	3.66E+03	113%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T04-A	1	1.10E+00	U1/2		1.10E+00	7.7E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T05-A	1	1.10E+00	U1/2		1.10E+00	1.7E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T06-A	1	1.10E+00	U1/2		1.10E+00	2.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T07-A	1	3.34E+01			3.34E+01	2.3E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T08-A	1	2.84E+01			2.84E+01	1.0E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T09-A	1	3.32E+01			3.32E+01	7.9E-01	2.2E+00	7.0E+00				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T01-B	1	1.10E+00	U1/2		1.10E+00	5.8E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T02-B	1	1.10E+00	U1/2		1.10E+00	1.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	1.1E+01	2.2E+00	7.0E+00	10	325	3.54E+03	109%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T04-B	1	1.10E+00	U1/2		1.10E+00	2.2E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T05-B	1	1.10E+00	U1/2		1.10E+00	9.5E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T06-B	1	1.10E+00	U1/2		1.10E+00	4.4E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T07-B	1	3.00E+01			3.00E+01	7.9E-01	2.2E+00	7.0E+00				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T08-B	1	2.84E+01			2.84E+01	2.3E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T09-B	1	3.27E+01			3.27E+01	1.3E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T01-C	1	1.10E+00	U1/2		1.10E+00	6.1E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T02-C	1	1.10E+00	U1/2		1.10E+00	2.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	1.3E+01	2.2E+00	7.0E+00	10	325	3.52E+03	108%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T04-C	1	1.10E+00	U1/2		1.10E+00	8.3E+00	2.2E+00	7.0E+00					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T05-C	1	1.10E+00	U1/2		1.10E+00	1.1E+01	2.2E+00	7.0E+00					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T06-C	1	1.10E+00	U1/2		1.10E+00	1.1E+01	2.2E+00	7.0E+00					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T07-C	1	2.88E+01			2.88E+01	2.8E+00	2.2E+00	7.0E+00					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T08-C	1	2.56E+01			2.56E+01	9.2E-01	2.2E+00	7.0E+00					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-T09-C	1	3.17E+01			3.17E+01	6.0E-01	2.2E+00	7.0E+00					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	7.4E+00	2.2E+00	7.0E+00					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	7.0E+00	2.2E+00	7.0E+00					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1313-B03-A	1	1.10E+00	U1/2		1.10E+00	2.8E+01	2.2E+00	7.0E+00					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	EaFA-L01-1313-T01-A	1	1.43E+04			1.43E+04	1.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T02-A	1	5.15E+04			5.15E+04	1.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T03-A	1	1.07E+05			1.07E+05	7.7E-01	2.6E+00	8.3E+00	1000	100	1.08E+05	82%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T04-A	1	1.36E+05			1.36E+05	5.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T05-A	1	1.45E+05			1.45E+05	5.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T06-A	1	1.72E+05			1.72E+05	6.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T07-A	1	1.61E+05			1.61E+05	5.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T08-A	1	1.51E+05			1.51E+05	2.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T09-A	1	1.34E+05			1.34E+05	5.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T01-B	1	1.31E+04			1.31E+04	1.6E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T02-B	1	5.32E+04			5.32E+04	1.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T03-B	1	1.07E+05			1.07E+05	5.5E-01	2.6E+00	8.3E+00	1000	100	1.08E+05	81%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T04-B	1	1.29E+05			1.29E+05	3.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T05-B	1	1.44E+05			1.44E+05	3.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T06-B	1	1.60E+05			1.60E+05	4.9E-02	2.6E+00	8.3E+00				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T07-B	1	1.41E+05			1.41E+05	5.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T08-B	1	1.47E+05			1.47E+05	4.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T09-B	1	1.34E+05			1.34E+05	4.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T01-C	1	1.28E+04			1.28E+04	1.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T02-C	1	5.30E+04			5.30E+04	2.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T03-C	1	1.04E+05			1.04E+05	9.7E-01	2.6E+00	8.3E+00	1000	100	1.05E+05	83%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T04-C	1	1.34E+05			1.34E+05	1.2E+00	2.6E+00	8.3E+00					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T05-C	1	1.36E+05			1.36E+05	4.2E-01	2.6E+00	8.3E+00					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T06-C	1	1.60E+05			1.60E+05	1.4E-01	2.6E+00	8.3E+00					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T07-C	1	1.39E+05			1.39E+05	6.0E-01	2.6E+00	8.3E+00					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T08-C	1	1.36E+05			1.36E+05	1.4E+00	2.6E+00	8.3E+00					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-T09-C	1	1.30E+05			1.30E+05	2.7E-01	2.6E+00	8.3E+00					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-B01-A	1	1.30E+00	U1/2		1.30E+00	2.9E+02	2.6E+00	8.3E+00					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-B02-A	1	1.30E+00	U1/2		1.30E+00	8.8E+01	2.6E+00	8.3E+00					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1313-B03-A	1	1.30E+00	U1/2		1.30E+00	1.2E+02	2.6E+00	8.3E+00					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	EaFA-L01-1313-T01-A	1	7.45E+02			7.45E+02	1.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T02-A	1	4.08E+02			4.08E+02	1.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T03-A	1	3.23E+02			3.23E+02	8.6E-01	1.2E+00	3.8E+00	10	325	3.70E+03	104%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T04-A	1	1.62E+02			1.62E+02	9.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T05-A	1	1.06E+02			1.06E+02	6.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T06-A	1	1.41E+01			1.41E+01	1.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T07-A	1	1.66E+00	E		1.66E+00	3.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T08-A	1	1.69E+02			1.69E+02	2.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T09-A	1	1.81E+03			1.81E+03	4.2E-02	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T01-B	1	5.26E+02			5.26E+02	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T02-B	1	3.01E+02			3.01E+02	1.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T03-B	1	2.07E+02			2.07E+02	4.4E-01	1.2E+00	3.8E+00	10	325	3.44E+03	99%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T04-B	1	1.56E+02			1.56E+02	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T05-B	1	1.07E+02			1.07E+02	7.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T06-B	1	1.84E+01			1.84E+01	9.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T07-B	1	3.37E+00	E		3.37E+00	1.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T08-B	1	1.84E+02			1.84E+02	1.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T09-B	1	1.81E+03			1.81E+03	1.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T01-C	1	5.16E+02			5.16E+02	8.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T02-C	1	2.58E+02			2.58E+02	5.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T03-C	1	2.27E+02			2.27E+02	5.2E-01	1.2E+00	3.8E+00	10	325	3.46E+03	100%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T04-C	1	1.54E+02			1.54E+02	1.2E+00	1.2E+00	3.8E+00					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T05-C	1	1.05E+02			1.05E+02	1.1E+00	1.2E+00	3.8E+00					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T06-C	1	1.44E+01			1.44E+01	3.0E+00	1.2E+00	3.8E+00					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T07-C	1	2.73E+00	E		2.73E+00	5.3E+01	1.2E+00	3.8E+00					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T08-C	1	1.54E+02			1.54E+02	1.3E+00	1.2E+00	3.8E+00					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-T09-C	1	1.75E+03			1.75E+03	8.8E-02	1.2E+00	3.8E+00					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	4.4E+02	1.2E+00	3.8E+00					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	1.4E+02	1.2E+00	3.8E+00					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1313-B03-A	1	1.38E+00	E		1.38E+00	3.0E+00	1.2E+00	3.8E+00					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	EaFA-L01-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	2.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	3.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	3.8E+02	1.8E+00	5.7E+00	10	325	3.53E+03	109%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	5.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T05-A	1	2.44E+00	E		2.44E+00	2.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T06-A	1	6.61E+01			6.61E+01	2.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T07-A	1	2.36E+02			2.36E+02	1.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T08-A	1	2.15E+02			2.15E+02	1.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T09-A	1	4.66E+02			4.66E+02	8.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	2.0E+02	1.8E+00	5.7E+00	10	325	3.41E+03	105%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	1.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T05-B	1	3.36E+00	E		3.36E+00	3.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T06-B	1	5.34E+01			5.34E+01	3.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T07-B	1	2.17E+02			2.17E+02	1.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T08-B	1	2.17E+02			2.17E+02	9.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T09-B	1	4.62E+02			4.62E+02	3.4E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	2.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	1.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	2.2E+01	1.8E+00	5.7E+00	10	325	3.42E+03	105%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	9.3E+01	1.8E+00	5.7E+00					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T05-C	1	4.64E+00	E		4.64E+00	5.9E+01	1.8E+00	5.7E+00					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T06-C	1	5.96E+01			5.96E+01	3.0E+00	1.8E+00	5.7E+00					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T07-C	1	2.11E+02			2.11E+02	1.4E+00	1.8E+00	5.7E+00					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T08-C	1	1.99E+02			1.99E+02	2.7E+00	1.8E+00	5.7E+00					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-T09-C	1	4.53E+02			4.53E+02	4.4E-01	1.8E+00	5.7E+00					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-B01-A	1	2.23E+00	E		2.23E+00	3.6E+03	1.8E+00	5.7E+00					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-B02-A	1	4.66E+00	E		4.66E+00	1.1E+02	1.8E+00	5.7E+00					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	9.6E+01	1.8E+00	5.7E+00					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	EaFA-L01-1313-T01-A	1	7.64E+01			7.64E+01	4.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T02-A	1	5.03E+00	E		5.03E+00	5.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T03-A	1	7.26E+00	E		7.26E+00	1.9E+01	3.7E+00	1.2E+01	10	325	3.35E+03	103%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T04-A	1	1.06E+01	E		1.06E+01	5.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T05-A	1	9.16E+00	E		9.16E+00	6.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T06-A	1	1.28E+01			1.28E+01	9.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T07-A	1	6.21E+02			6.21E+02	2.4E-01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T08-A	1	1.88E+03			1.88E+03	1.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T09-A	1	2.93E+03			2.93E+03	4.9E-01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T01-B	1	6.49E+01			6.49E+01	5.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T02-B	1	5.03E+00	E		5.03E+00	2.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T03-B	1	1.85E+00	U1/2		1.85E+00	1.6E+02	3.7E+00	1.2E+01	10	325	3.19E+03	98%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T04-B	1	1.46E+01			1.46E+01	5.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T05-B	1	9.09E+00	E		9.09E+00	3.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T06-B	1	1.09E+01	E		1.09E+01	2.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T07-B	1	6.77E+02			6.77E+02	8.8E-01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T08-B	1	1.93E+03			1.93E+03	1.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T09-B	1	2.98E+03			2.98E+03	4.4E-01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T01-C	1	5.85E+01			5.85E+01	6.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T02-C	1	5.32E+00	E		5.32E+00	5.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T03-C	1	7.70E+00	E		7.70E+00	5.3E+00	3.7E+00	1.2E+01	10	325	3.21E+03	99%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T04-C	1	1.15E+01	E		1.15E+01	5.1E+01	3.7E+00	1.2E+01					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T05-C	1	1.15E+01	E		1.15E+01	2.1E+01	3.7E+00	1.2E+01					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T06-C	1	6.16E+00	E		6.16E+00	3.8E+01	3.7E+00	1.2E+01					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T07-C	1	5.73E+02			5.73E+02	3.4E-01	3.7E+00	1.2E+01					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T08-C	1	1.74E+03			1.74E+03	2.0E+00	3.7E+00	1.2E+01					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-T09-C	1	2.87E+03			2.87E+03	5.9E-01	3.7E+00	1.2E+01					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	7.5E+01	3.7E+00	1.2E+01					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	1.9E+02	3.7E+00	1.2E+01					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1313-B03-A	1	1.85E+00	U1/2		1.85E+00	1.3E+02	3.7E+00	1.2E+01					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	EaFA-L01-1313-T01-A	1	2.99E+01			2.99E+01	2.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T02-A	1	1.41E+01			1.41E+01	2.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	2.1E+01	2.0E+00	6.4E+00	1000	100	1.09E+03	109%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	6.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T07-A	1	8.71E+00			8.71E+00	4.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T08-A	1	3.85E+02			3.85E+02	3.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T09-A	1	4.15E+04			4.15E+04	2.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T01-B	1	3.25E+01			3.25E+01	2.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T02-B	1	6.19E+01			6.19E+01	2.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	2.1E+01	2.0E+00	6.4E+00	1000	100	1.06E+03	106%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T07-B	1	1.10E+01			1.10E+01	2.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T08-B	1	4.33E+02			4.33E+02	6.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T09-B	1	4.08E+04			4.08E+04	3.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T01-C	1	4.13E+01			4.13E+01	3.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T02-C	1	1.95E+01			1.95E+01	2.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	3.1E+02	2.0E+00	6.4E+00	1000	100	1.06E+03	106%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	2.2E+00	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	8.6E-01	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	9.4E+00	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T07-C	1	4.87E+00	E		4.87E+00	7.0E+00	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T08-C	1	3.54E+02			3.54E+02	8.7E-01	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-T09-C	1	4.08E+04			4.08E+04	2.1E-02	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-B02-A	1	2.79E+01			2.79E+01	2.2E+01	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1313-B03-A	1	1.07E+01			1.07E+01	1.2E+01	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	EaFA-L01-1313-T01-A	1	3.03E+01			3.03E+01	3.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T02-A	1	3.40E+00	U1/2		3.40E+00	3.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T03-A	1	3.40E+00	U1/2		3.40E+00	5.8E+01	6.8E+00	2.2E+01	10	325	3.35E+03	103%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T04-A	1	3.40E+00	U1/2		3.40E+00	1.6E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T05-A	1	3.40E+00	U1/2		3.40E+00	1.1E+03	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T06-A	1	3.40E+00	U1/2		3.40E+00	8.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T07-A	1	3.40E+00	U1/2		3.40E+00	2.1E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T08-A	1	3.40E+00	U1/2		3.40E+00	4.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T09-A	1	1.34E+02			1.34E+02	1.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T01-B	1	1.80E+01	E		1.80E+01	1.4E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T02-B	1	3.40E+00	U1/2		3.40E+00	1.6E+03	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T03-B	1	3.40E+00	U1/2		3.40E+00	2.2E+01	6.8E+00	2.2E+01	10	325	3.26E+03	100%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T04-B	1	3.40E+00	U1/2		3.40E+00	7.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T05-B	1	3.40E+00	U1/2		3.40E+00	1.2E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T06-B	1	3.40E+00	U1/2		3.40E+00	1.6E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T07-B	1	3.40E+00	U1/2		3.40E+00	9.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T08-B	1	3.40E+00	U1/2		3.40E+00	7.6E+04	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T09-B	1	1.26E+02			1.26E+02	7.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T01-C	1	9.58E+00	E		9.58E+00	4.7E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T02-C	1	3.40E+00	U1/2		3.40E+00	9.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T03-C	1	3.40E+00	U1/2		3.40E+00	9.2E+01	6.8E+00	2.2E+01	10	325	3.24E+03	99%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T04-C	1	3.40E+00	U1/2		3.40E+00	6.1E+01	6.8E+00	2.2E+01					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T05-C	1	3.40E+00	U1/2		3.40E+00	1.6E+02	6.8E+00	2.2E+01					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T06-C	1	3.40E+00	U1/2		3.40E+00	1.7E+03	6.8E+00	2.2E+01					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T07-C	1	3.40E+00	U1/2		3.40E+00	2.5E+02	6.8E+00	2.2E+01					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T08-C	1	3.40E+00	U1/2		3.40E+00	6.7E+01	6.8E+00	2.2E+01					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-T09-C	1	1.29E+02			1.29E+02	6.0E+00	6.8E+00	2.2E+01					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	1.3E+02	6.8E+00	2.2E+01					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	6.2E+01	6.8E+00	2.2E+01					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	2.0E+02	6.8E+00	2.2E+01					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	EaFA-L01-1313-T01-A	1	2.97E+03			2.97E+03	8.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T02-A	1	4.03E+03			4.03E+03	1.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T03-A	1	4.65E+03			4.65E+03	2.7E-01	1.9E+00	6.0E+00	10	325	8.10E+03	106%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T04-A	1	4.98E+03			4.98E+03	6.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T05-A	1	5.11E+03			5.11E+03	3.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T06-A	1	5.72E+03			5.72E+03	8.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T07-A	1	4.79E+03			4.79E+03	2.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T08-A	1	3.69E+03			3.69E+03	4.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T09-A	1	2.27E+03			2.27E+03	2.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T01-B	1	2.97E+03			2.97E+03	2.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T02-B	1	3.94E+03			3.94E+03	1.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T03-B	1	4.48E+03			4.48E+03	3.1E-01	1.9E+00	6.0E+00	10	325	8.00E+03	108%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T04-B	1	4.77E+03			4.77E+03	3.9E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T05-B	1	5.07E+03			5.07E+03	2.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T06-B	1	5.38E+03			5.38E+03	2.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T07-B	1	4.29E+03			4.29E+03	2.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T08-B	1	3.59E+03			3.59E+03	2.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T09-B	1	2.27E+03			2.27E+03	5.9E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T01-C	1	2.96E+03			2.96E+03	9.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T02-C	1	3.68E+03			3.68E+03	4.9E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T03-C	1	4.54E+03			4.54E+03	4.5E-01	1.9E+00	6.0E+00	10	325	8.40E+03	119%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T04-C	1	4.90E+03			4.90E+03	6.9E-01	1.9E+00	6.0E+00					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T05-C	1	4.83E+03			4.83E+03	2.8E-01	1.9E+00	6.0E+00					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T06-C	1	5.41E+03			5.41E+03	5.1E-01	1.9E+00	6.0E+00					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T07-C	1	4.22E+03			4.22E+03	6.8E-01	1.9E+00	6.0E+00					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T08-C	1	3.35E+03			3.35E+03	1.5E+00	1.9E+00	6.0E+00					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-T09-C	1	2.19E+03			2.19E+03	7.3E-01	1.9E+00	6.0E+00					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-B01-A	1	8.26E+00			8.26E+00	9.8E+00	1.9E+00	6.0E+00					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-B02-A	1	5.37E+00	E		5.37E+00	4.9E+00	1.9E+00	6.0E+00					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	2.1E+01	1.9E+00	6.0E+00					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	EaFA-L01-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	4.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	7.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	7.6E+01	2.0E+00	6.4E+00	10	325	3.39E+03	104%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	5.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T05-A	1	2.88E+01			2.88E+01	4.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T06-A	1	4.58E+02			4.58E+02	4.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T07-A	1	9.34E+02			9.34E+02	5.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T08-A	1	1.17E+03			1.17E+03	5.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T09-A	1	1.71E+03			1.71E+03	2.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T02-B	1	2.20E+00	E		2.20E+00	9.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	2.6E+01	2.0E+00	6.4E+00	10	325	3.29E+03	101%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T05-B	1	2.88E+01			2.88E+01	1.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T06-B	1	3.63E+02			3.63E+02	8.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T07-B	1	8.43E+02			8.43E+02	1.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T08-B	1	1.16E+03			1.16E+03	3.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T09-B	1	1.72E+03			1.72E+03	2.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	2.3E+02	2.0E+00	6.4E+00	10	325	3.28E+03	101%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	3.1E+00	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T05-C	1	2.57E+01			2.57E+01	5.6E-01	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T06-C	1	3.96E+02			3.96E+02	8.1E-01	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T07-C	1	8.39E+02			8.39E+02	1.3E+00	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T08-C	1	1.08E+03			1.08E+03	2.1E+00	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-T09-C	1	1.66E+03			1.66E+03	1.8E-01	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	5.4E+01	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	EaFA-L01-1313-T01-A	1	5.00E-01	U1/2		5.00E-01	2.5E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T02-A	1	5.00E-01	U1/2		5.00E-01	2.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T03-A	1	4.55E+02			4.55E+02	1.2E+00	1.0E+00	3.2E+00	1000	100	1.47E+03	102%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T04-A	1	3.31E+03			3.31E+03	7.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T05-A	1	4.65E+03			4.65E+03	4.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T06-A	1	7.99E+03			7.99E+03	7.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T07-A	1	8.21E+03			8.21E+03	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T08-A	1	7.83E+03			7.83E+03	8.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T09-A	1	1.43E+04			1.43E+04	3.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T01-B	1	5.00E-01	U1/2		5.00E-01	8.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T02-B	1	5.00E-01	U1/2		5.00E-01	1.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T03-B	1	4.72E+02			4.72E+02	3.0E+00	1.0E+00	3.2E+00	1000	100	1.59E+03	112%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T04-B	1	3.22E+03			3.22E+03	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T05-B	1	4.66E+03			4.66E+03	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T06-B	1	7.38E+03			7.38E+03	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T07-B	1	7.14E+03			7.14E+03	3.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T08-B	1	7.78E+03			7.78E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T09-B	1	1.44E+04			1.44E+04	9.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T01-C	1	5.00E-01	U1/2		5.00E-01	5.3E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T02-C	1	5.00E-01	U1/2		5.00E-01	8.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T03-C	1	3.63E+02			3.63E+02	8.3E-01	1.0E+00	3.2E+00	1000	100	1.34E+03	98%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T04-C	1	3.47E+03			3.47E+03	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T05-C	1	4.54E+03			4.54E+03	3.7E-01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T06-C	1	7.26E+03			7.26E+03	9.7E-01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T07-C	1	7.01E+03			7.01E+03	1.0E+00	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T08-C	1	7.25E+03			7.25E+03	2.1E+00	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-T09-C	1	1.40E+04			1.40E+04	3.6E-01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	5.5E+02	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	3.0E+02	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	7.9E+01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	EaFA-L01-1313-T01-A	1	4.72E+03			4.72E+03	1.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T02-A	1	4.45E+03			4.45E+03	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T03-A	1	4.46E+03			4.46E+03	5.3E-01	1.2E+00	3.8E+00	10	325	7.49E+03	93%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T04-A	1	4.08E+03			4.08E+03	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T05-A	1	3.91E+03			3.91E+03	5.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T06-A	1	3.75E+03			3.75E+03	7.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T07-A	1	2.21E+02			2.21E+02	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T08-A	1	1.34E+02			1.34E+02	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T09-A	1	6.21E+02			6.21E+02	5.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T01-B	1	4.49E+03			4.49E+03	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T02-B	1	4.21E+03			4.21E+03	2.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T03-B	1	4.01E+03			4.01E+03	1.0E+00	1.2E+00	3.8E+00	10	325	7.06E+03	94%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T04-B	1	3.96E+03			3.96E+03	7.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T05-B	1	3.93E+03			3.93E+03	6.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T06-B	1	3.48E+03			3.48E+03	8.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T07-B	1	1.45E+02			1.45E+02	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T08-B	1	1.31E+02			1.31E+02	2.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T09-B	1	5.80E+02			5.80E+02	2.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T01-C	1	4.53E+03			4.53E+03	1.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T02-C	1	3.89E+03			3.89E+03	3.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T03-C	1	4.13E+03			4.13E+03	8.7E-01	1.2E+00	3.8E+00	10	325	7.13E+03	92%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T04-C	1	4.09E+03			4.09E+03	3.2E-01	1.2E+00	3.8E+00					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T05-C	1	3.71E+03			3.71E+03	1.2E-01	1.2E+00	3.8E+00					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T06-C	1	3.40E+03			3.40E+03	9.7E-01	1.2E+00	3.8E+00					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T07-C	1	1.50E+02			1.50E+02	2.0E+00	1.2E+00	3.8E+00					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T08-C	1	1.23E+02			1.23E+02	1.2E+00	1.2E+00	3.8E+00					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-T09-C	1	6.03E+02			6.03E+02	7.8E-01	1.2E+00	3.8E+00					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-B01-A	1	1.63E+00	E		1.63E+00	1.1E+02	1.2E+00	3.8E+00					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-B02-A	1	2.67E+01			2.67E+01	1.7E+02	1.2E+00	3.8E+00					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1313-B03-A	1	1.37E+01			1.37E+01	2.5E+00	1.2E+00	3.8E+00					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	EaFA-L01-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	3.2E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	3.1E+02	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00	10	325	3.52E+03	108%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	5.1E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T05-A	1	9.25E+00			9.25E+00	2.2E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T06-A	1	1.53E+02			1.53E+02	1.0E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T07-A	1	5.95E+02			5.95E+02	4.0E-01	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T08-A	1	5.34E+02			5.34E+02	1.2E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T09-A	1	7.88E+02			7.88E+02	3.5E-01	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	3.9E+02	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	3.5E+02	1.8E+00	5.7E+00	10	325	3.40E+03	105%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	1.2E+03	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T05-B	1	7.22E+00			7.22E+00	3.5E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T06-B	1	1.14E+02			1.14E+02	1.7E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T07-B	1	5.45E+02			5.45E+02	1.9E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T08-B	1	5.31E+02			5.31E+02	6.3E-01	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T09-B	1	7.79E+02			7.79E+02	2.9E-01	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T01-C		9.00E-01	U1/2		9.00E-01	5.4E+02	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T02-C		9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T03-C		9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00	10	325	3.39E+03	104%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T04-C		9.00E-01	U1/2		9.00E-01	2.8E+02	1.8E+00	5.7E+00					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T05-C		7.25E+00			7.25E+00	7.1E+01	1.8E+00	5.7E+00					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T06-C		1.33E+02			1.33E+02	8.9E-01	1.8E+00	5.7E+00					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T07-C		5.26E+02			5.26E+02	2.0E+00	1.8E+00	5.7E+00					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T08-C		4.87E+02			4.87E+02	1.5E+00	1.8E+00	5.7E+00					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-T09-C		7.63E+02			7.63E+02	7.4E-01	1.8E+00	5.7E+00					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-B01-A		9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-B02-A		9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1313-B03-A		9.00E-01	U1/2		9.00E-01	2.2E+02	1.8E+00	5.7E+00					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	EaFA-L01-1313-T01-A	1	1.56E+02			1.56E+02	2.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T02-A	1	8.28E+00	E		8.28E+00	1.8E+02	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T03-A	1	2.77E+01			2.77E+01	1.0E+01	3.7E+00	1.2E+01	1000	100	1.12E+03	109%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T04-A	1	9.52E+01			9.52E+01	6.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T05-A	1	6.42E+01			6.42E+01	2.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T06-A	1	2.06E+01			2.06E+01	3.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T07-A	1	1.85E+00	U1/2		1.85E+00	2.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T08-A	1	3.68E+01			3.68E+01	1.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T09-A	1	5.30E+03			5.30E+03	1.8E-01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T01-B	1	1.57E+02			1.57E+02	3.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T02-B	1	2.06E+01			2.06E+01	3.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T03-B	1	6.36E+01			6.36E+01	2.2E+01	3.7E+00	1.2E+01	1000	100	1.13E+03	107%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T04-B	1	7.53E+01			7.53E+01	8.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T05-B	1	5.97E+01			5.97E+01	1.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T06-B	1	2.00E+01			2.00E+01	3.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T07-B	1	1.85E+00	U1/2		1.85E+00	2.4E+03	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T08-B	1	4.70E+01			4.70E+01	1.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T09-B	1	4.68E+03			4.68E+03	1.3E-01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T01-C	1	1.68E+02			1.68E+02	3.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T02-C	1	1.01E+01	E		1.01E+01	3.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T03-C	1	4.71E+01			4.71E+01	2.1E+01	3.7E+00	1.2E+01	1000	100	1.13E+03	108%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T04-C	1	6.41E+01			6.41E+01	7.0E+00	3.7E+00	1.2E+01					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T05-C	1	6.74E+01			6.74E+01	3.9E+00	3.7E+00	1.2E+01					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T06-C	1	1.97E+01			1.97E+01	5.3E+01	3.7E+00	1.2E+01					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T07-C	1	1.85E+00	U1/2		1.85E+00	2.5E+01	3.7E+00	1.2E+01					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T08-C	1	3.75E+01			3.75E+01	1.9E+01	3.7E+00	1.2E+01					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-T09-C	1	5.03E+03			5.03E+03	2.7E-01	3.7E+00	1.2E+01					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	3.0E+02	3.7E+00	1.2E+01					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-B02-A	1	1.48E+01			1.48E+01	1.6E+02	3.7E+00	1.2E+01					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1313-B03-A	1	3.42E+01			3.42E+01	5.8E+01	3.7E+00	1.2E+01					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	EaFA-L01-1313-T01-A	1	1.87E+06			1.87E+06	9.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T02-A	1	4.60E+05			4.60E+05	1.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T03-A	1	1.75E+05			1.75E+05	7.0E-01	1.6E+00	5.1E+00	1000	100	1.76E+05	83%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T04-A	1	1.06E+05			1.06E+05	2.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T05-A	1	6.49E+04			6.49E+04	4.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T06-A	1	2.42E+04			2.42E+04	3.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T07-A	1	2.17E+04			2.17E+04	3.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T08-A	1	1.82E+04			1.82E+04	5.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T09-A	1	2.18E+04			2.18E+04	3.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T01-B	1	1.86E+06			1.86E+06	8.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T02-B	1	4.54E+05			4.54E+05	8.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T03-B	1	1.53E+05			1.53E+05	7.9E-01	1.6E+00	5.1E+00	1000	100	1.54E+05	92%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T04-B	1	1.02E+05			1.02E+05	2.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T05-B	1	6.49E+04			6.49E+04	8.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T06-B	1	2.29E+04			2.29E+04	2.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T07-B	1	1.97E+04			1.97E+04	1.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T08-B	1	1.78E+04			1.78E+04	3.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T09-B	1	2.14E+04			2.14E+04	4.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T01-C	1	1.80E+06			1.80E+06	3.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T02-C	1	3.93E+05			3.93E+05	4.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T03-C	1	1.69E+05			1.69E+05	5.3E-01	1.6E+00	5.1E+00	1000	100	1.70E+05	88%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T04-C	1	1.04E+05			1.04E+05	5.0E-01	1.6E+00	5.1E+00					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T05-C	1	6.12E+04			6.12E+04	6.7E-01	1.6E+00	5.1E+00					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T06-C	1	2.31E+04			2.31E+04	5.5E-01	1.6E+00	5.1E+00					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T07-C	1	1.93E+04			1.93E+04	6.5E-01	1.6E+00	5.1E+00					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T08-C	1	1.67E+04			1.67E+04	1.0E+00	1.6E+00	5.1E+00					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-T09-C	1	2.12E+04			2.12E+04	8.1E-01	1.6E+00	5.1E+00					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-B01-A	1	1.11E+01			1.11E+01	1.1E+01	1.6E+00	5.1E+00					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-B02-A	1	1.86E+06			1.86E+06	1.6E+01	1.6E+00	5.1E+00					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1313-B03-A	1	1.40E+06			1.40E+06	7.0E-01	1.6E+00	5.1E+00					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	EaFA-L01-1313-T01-A	1	8.17E+03			8.17E+03	1.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T02-A	1	6.11E+03			6.11E+03	2.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T03-A	1	5.35E+03			5.35E+03	2.5E-01	1.5E+01	4.8E+01	10	325	8.23E+03	89%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T04-A	1	3.63E+03			3.63E+03	1.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T05-A	1	2.25E+03			2.25E+03	6.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T06-A	1	1.23E+03			1.23E+03	3.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T07-A	1	1.99E+02			1.99E+02	7.8E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T08-A	1	9.22E+01			9.22E+01	4.1E+01	1.5E+01	4.8E+01				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T09-A	1	1.24E+03			1.24E+03	2.2E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T01-B	1	7.61E+03			7.61E+03	2.8E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T02-B	1	5.77E+03			5.77E+03	1.6E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T03-B	1	4.72E+03			4.72E+03	7.2E-01	1.5E+01	4.8E+01	10	325	7.67E+03	91%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T04-B	1	3.60E+03			3.60E+03	1.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T05-B	1	2.24E+03			2.24E+03	1.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T06-B	1	1.08E+03			1.08E+03	1.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T07-B	1	1.54E+02			1.54E+02	2.8E+01	1.5E+01	4.8E+01				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T08-B	1	9.38E+01			9.38E+01	1.7E+01	1.5E+01	4.8E+01				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T09-B	1	1.16E+03			1.16E+03	2.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T01-C	1	7.64E+03			7.64E+03	2.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T02-C	1	5.12E+03			5.12E+03	3.4E-01	1.5E+01	4.8E+01				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T03-C	1	4.97E+03			4.97E+03	9.9E-01	1.5E+01	4.8E+01	10	325	7.84E+03	88%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T04-C	1	3.60E+03			3.60E+03	2.4E+00	1.5E+01	4.8E+01					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T05-C	1	2.20E+03			2.20E+03	1.3E-01	1.5E+01	4.8E+01					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T06-C	1	1.03E+03			1.03E+03	4.4E+00	1.5E+01	4.8E+01					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T07-C	1	1.25E+02			1.25E+02	3.2E+01	1.5E+01	4.8E+01					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T08-C	1	8.94E+01			8.94E+01	1.0E+01	1.5E+01	4.8E+01					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-T09-C	1	1.19E+03			1.19E+03	1.2E+00	1.5E+01	4.8E+01					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-B01-A	1	7.50E+00	U1/2		7.50E+00	4.9E+01	1.5E+01	4.8E+01					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-B02-A	1	7.50E+00	U1/2		7.50E+00	1.9E+02	1.5E+01	4.8E+01					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1313-B03-A	1	7.50E+00	U1/2		7.50E+00	2.9E+02	1.5E+01	4.8E+01					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	EaFA-L01-1313-T01-A	1	2.25E+04			2.25E+04	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T02-A	1	4.36E+03			4.36E+03	9.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T03-A	1	5.91E+02			5.91E+02	2.4E-01	1.1E+00	3.5E+00	1000	100	1.69E+03	110%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T04-A	1	3.36E+02			3.36E+02	1.6E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T05-A	1	6.55E+02			6.55E+02	5.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T06-A	1	3.27E+03			3.27E+03	4.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T07-A	1	9.62E+03			9.62E+03	3.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T08-A	1	2.00E+04			2.00E+04	4.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T09-A	1	6.93E+04			6.93E+04	3.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T01-B	1	1.80E+04			1.80E+04	1.5E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T02-B	1	3.23E+03			3.23E+03	1.7E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T03-B	1	4.57E+02			4.57E+02	7.0E-01	1.1E+00	3.5E+00	1000	100	1.52E+03	106%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T04-B	1	3.29E+02			3.29E+02	2.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T05-B	1	6.67E+02			6.67E+02	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T06-B	1	2.26E+03			2.26E+03	5.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T07-B	1	8.39E+03			8.39E+03	4.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T08-B	1	2.03E+04			2.03E+04	2.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T09-B	1	6.98E+04			6.98E+04	2.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T01-C	1	1.79E+04			1.79E+04	1.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T02-C	1	2.87E+03			2.87E+03	3.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T03-C	1	6.44E+02			6.44E+02	5.0E-01	1.1E+00	3.5E+00	1000	100	1.68E+03	104%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T04-C	1	3.37E+02			3.37E+02	8.6E-01	1.1E+00	3.5E+00					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T05-C	1	6.29E+02			6.29E+02	1.7E+00	1.1E+00	3.5E+00					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T06-C	1	2.46E+03			2.46E+03	3.5E-01	1.1E+00	3.5E+00					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T07-C	1	7.98E+03			7.98E+03	1.6E+00	1.1E+00	3.5E+00					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T08-C	1	1.86E+04			1.86E+04	1.5E+00	1.1E+00	3.5E+00					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-T09-C	1	6.79E+04			6.79E+04	3.4E-01	1.1E+00	3.5E+00					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-B01-A	1	3.54E+01			3.54E+01	9.3E+00	1.1E+00	3.5E+00					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-B02-A	1	2.38E+03			2.38E+03	1.1E+01	1.1E+00	3.5E+00					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1313-B03-A	1	7.81E+02			7.81E+02	1.9E+00	1.1E+00	3.5E+00					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	EaFA-L01-1313-T01-A	1	2.33E+04			2.33E+04	1.0E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T02-A	1	7.40E+03			7.40E+03	9.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T03-A	1	6.34E+03			6.34E+03	4.7E-01	2.5E+00	8.0E+00	1000	100	7.41E+03	107%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T04-A	1	5.77E+03			5.77E+03	3.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T05-A	1	5.48E+03			5.48E+03	4.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T06-A	1	5.62E+03			5.62E+03	7.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T07-A	1	4.82E+03			4.82E+03	1.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T08-A	1	3.93E+03			3.93E+03	3.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T09-A	1	3.09E+03			3.09E+03	2.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T01-B	1	2.13E+04			2.13E+04	1.4E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T02-B	1	7.21E+03			7.21E+03	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T03-B	1	5.64E+03			5.64E+03	4.4E-01	2.5E+00	8.0E+00	1000	100	6.57E+03	93%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T04-B	1	5.58E+03			5.58E+03	5.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T05-B	1	5.49E+03			5.49E+03	2.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T06-B	1	5.29E+03			5.29E+03	5.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T07-B	1	4.36E+03			4.36E+03	7.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T08-B	1	3.83E+03			3.83E+03	2.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T09-B	1	3.10E+03			3.10E+03	8.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T01-C	1	2.08E+04			2.08E+04	9.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T02-C	1	6.47E+03			6.47E+03	6.1E-02	2.5E+00	8.0E+00				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T03-C	1	5.83E+03			5.83E+03	5.0E-01	2.5E+00	8.0E+00	1000	100	6.80E+03	96%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T04-C	1	5.71E+03			5.71E+03	9.2E-01	2.5E+00	8.0E+00					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T05-C	1	5.19E+03			5.19E+03	4.7E-01	2.5E+00	8.0E+00					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T06-C	1	5.32E+03			5.32E+03	3.4E-01	2.5E+00	8.0E+00					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T07-C	1	4.29E+03			4.29E+03	6.4E-01	2.5E+00	8.0E+00					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T08-C	1	3.63E+03			3.63E+03	8.9E-01	2.5E+00	8.0E+00					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-T09-C	1	3.04E+03			3.04E+03	3.5E-01	2.5E+00	8.0E+00					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-B01-A	1	8.50E+00			8.50E+00	2.3E+00	2.5E+00	8.0E+00					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-B02-A	1	2.60E+00	E		2.60E+00	2.4E+00	2.5E+00	8.0E+00					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1313-B03-A	1	5.33E+02			5.33E+02	5.5E-01	2.5E+00	8.0E+00					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	EaFA-L01-1313-T01-A	1	1.65E+03			1.65E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T02-A	1	1.78E+03			1.78E+03	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T03-A	1	2.00E+03			2.00E+03	7.2E-01	1.0E+00	3.2E+00	1000	100	2.84E+03	84%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T04-A	1	1.98E+03			1.98E+03	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T05-A	1	1.98E+03			1.98E+03	5.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T06-A	1	2.33E+03			2.33E+03	5.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T07-A	1	2.76E+03			2.76E+03	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T08-A	1	2.99E+03			2.99E+03	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T09-A	1	5.30E+03			5.30E+03	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T01-B	1	1.41E+03			1.41E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T02-B	1	1.67E+03			1.67E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T03-B	1	1.79E+03			1.79E+03	1.0E+00	1.0E+00	3.2E+00	1000	100	2.64E+03	85%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T04-B	1	1.93E+03			1.93E+03	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T05-B	1	1.99E+03			1.99E+03	9.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T06-B	1	2.18E+03			2.18E+03	8.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T07-B	1	2.36E+03			2.36E+03	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T08-B	1	3.01E+03			3.01E+03	7.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T09-B	1	5.31E+03			5.31E+03	8.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T01-C	1	1.39E+03			1.39E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T02-C	1	1.56E+03			1.56E+03	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T03-C	1	1.80E+03			1.80E+03	6.7E-01	1.0E+00	3.2E+00	1000	100	2.63E+03	83%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T04-C	1	1.99E+03			1.99E+03	4.3E-01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T05-C	1	1.91E+03			1.91E+03	2.7E-01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T06-C	1	2.15E+03			2.15E+03	5.4E-01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T07-C	1	2.27E+03			2.27E+03	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T08-C	1	2.76E+03			2.76E+03	1.8E+00	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-T09-C	1	5.13E+03			5.13E+03	4.8E-01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	4.0E+01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.8E+01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	9.0E+01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	EaFA-L01-1313-T01-A	1	1.98E+05			1.98E+05	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T02-A	1	1.65E+05			1.65E+05	8.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T03-A	1	1.63E+05			1.63E+05	7.5E-02	6.8E+00	2.2E+01	1000	100	1.64E+05	88%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T04-A	1	1.63E+05			1.63E+05	5.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T05-A	1	1.59E+05			1.59E+05	4.8E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T06-A	1	1.64E+05			1.64E+05	5.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T07-A	1	1.26E+05			1.26E+05	2.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T08-A	1	9.93E+04			9.93E+04	4.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T09-A	1	5.41E+04			5.41E+04	5.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T01-B	1	1.86E+05			1.86E+05	1.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T02-B	1	1.61E+05			1.61E+05	1.3E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T03-B	1	1.55E+05			1.55E+05	3.9E-01	6.8E+00	2.2E+01	1000	100	1.56E+05	83%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T04-B	1	1.57E+05			1.57E+05	7.8E-02	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T05-B	1	1.58E+05			1.58E+05	2.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T06-B	1	1.56E+05			1.56E+05	1.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T07-B	1	1.13E+05			1.13E+05	4.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T08-B	1	9.84E+04			9.84E+04	9.0E-02	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T09-B	1	5.50E+04			5.50E+04	2.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T01-C	1	1.87E+05			1.87E+05	8.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T02-C	1	1.47E+05			1.47E+05	5.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T03-C	1	1.61E+05			1.61E+05	4.6E-01	6.8E+00	2.2E+01	1000	100	1.62E+05	94%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T04-C	1	1.63E+05			1.63E+05	8.6E-01	6.8E+00	2.2E+01					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T05-C	1	1.50E+05			1.50E+05	4.3E-01	6.8E+00	2.2E+01					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T06-C	1	1.57E+05			1.57E+05	1.0E-01	6.8E+00	2.2E+01					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T07-C	1	1.11E+05			1.11E+05	9.8E-01	6.8E+00	2.2E+01					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T08-C	1	9.21E+04			9.21E+04	1.2E+00	6.8E+00	2.2E+01					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-T09-C	1	5.31E+04			5.31E+04	2.2E-01	6.8E+00	2.2E+01					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	2.7E+02	6.8E+00	2.2E+01					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	1.1E+02	6.8E+00	2.2E+01					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1313-B03-A	1	1.31E+01	E		1.31E+01	2.0E+01	6.8E+00	2.2E+01					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	EaFA-L01-1313-T01-A	1	2.30E+00	U1/2		2.30E+00	1.4E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T02-A	1	2.30E+00	U1/2		2.30E+00	1.8E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T03-A	1	2.30E+00	U1/2		2.30E+00	1.4E+02	4.6E+00	1.5E+01	10	325	3.22E+03	99%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T04-A	1	2.30E+00	U1/2		2.30E+00	2.5E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T05-A	1	2.30E+00	U1/2		2.30E+00	2.5E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T06-A	1	2.30E+00	U1/2		2.30E+00	7.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T07-A	1	2.40E+01			2.40E+01	2.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T08-A	1	4.77E+01			4.77E+01	9.0E+00	4.6E+00	1.5E+01				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T09-A	1	7.40E+01			7.40E+01	7.7E+00	4.6E+00	1.5E+01				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T01-B	1	2.30E+00	U1/2		2.30E+00	2.9E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T02-B	1	2.30E+00	U1/2		2.30E+00	4.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T03-B	1	2.30E+00	U1/2		2.30E+00	3.8E+02	4.6E+00	1.5E+01	10	325	3.15E+03	97%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T04-B	1	2.30E+00	U1/2		2.30E+00	1.9E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T05-B	1	2.30E+00	U1/2		2.30E+00	8.1E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T06-B	1	2.30E+00	U1/2		2.30E+00	5.8E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T07-B	1	2.42E+01			2.42E+01	3.1E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T08-B	1	3.56E+01			3.56E+01	2.1E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T09-B	1	7.63E+01			7.63E+01	6.5E+00	4.6E+00	1.5E+01				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T01-C	1	2.30E+00	U1/2		2.30E+00	7.1E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T02-C	1	2.30E+00	U1/2		2.30E+00	6.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T03-C	1	2.30E+00	U1/2		2.30E+00	3.0E+01	4.6E+00	1.5E+01	10	325	3.12E+03	96%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T04-C	1	2.30E+00	U1/2		2.30E+00	3.8E+01	4.6E+00	1.5E+01					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T05-C	1	2.30E+00	U1/2		2.30E+00	6.4E+01	4.6E+00	1.5E+01					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T06-C	1	2.30E+00	U1/2		2.30E+00	1.2E+03	4.6E+00	1.5E+01					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T07-C	1	3.16E+01			3.16E+01	3.5E+01	4.6E+00	1.5E+01					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T08-C	1	3.73E+01			3.73E+01	1.4E+01	4.6E+00	1.5E+01					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-T09-C	1	7.82E+01			7.82E+01	5.6E+00	4.6E+00	1.5E+01					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	9.2E+01	4.6E+00	1.5E+01					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	1.5E+02	4.6E+00	1.5E+01					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	7.0E+01	4.6E+00	1.5E+01					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	EaFA-L01-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	6.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	4.5E+01	2.0E+00	6.4E+00	10	325	3.42E+03	105%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	2.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	1.5E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	6.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T08-A	1	1.27E+01			1.27E+01	3.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T09-A	1	1.08E+04			1.08E+04	2.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	9.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T02-B	1	1.66E+01			1.66E+01	4.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	2.1E+02	2.0E+00	6.4E+00	10	325	3.32E+03	102%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	6.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	5.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	1.8E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	5.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T08-B	1	1.30E+01			1.30E+01	4.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T09-B	1	9.16E+03			9.16E+03	6.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T01-C	1	4.96E+00	E		4.96E+00	9.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	4.6E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	7.0E+01	2.0E+00	6.4E+00	10	325	3.31E+03	102%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	2.2E+02	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	3.9E+01	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	1.8E+02	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T08-C	1	1.22E+01			1.22E+01	3.2E+00	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-T09-C	1	1.05E+04			1.05E+04	4.6E-01	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	2.2E+02	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1313-B03-A	1	2.30E+00	E		2.30E+00	8.8E+00	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	EaFA-L01-1313-T01-A	1	6.31E+03			6.31E+03	4.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T02-A	1	3.02E+03			3.02E+03	8.6E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T03-A	1	2.15E+03			2.15E+03	9.5E-01	1.5E+00	4.8E+00	10	325	5.31E+03	97%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T04-A	1	7.93E+02			7.93E+02	3.9E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T05-A	1	3.95E+02			3.95E+02	7.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T06-A	1	3.21E+02			3.21E+02	6.0E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T07-A	1	9.86E+01			9.86E+01	5.8E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T08-A	1	1.07E+02			1.07E+02	9.0E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T09-A	1	6.00E+03			6.00E+03	6.0E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T01-B	1	5.73E+03			5.73E+03	1.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T02-B	1	2.49E+03			2.49E+03	1.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T03-B	1	1.74E+03			1.74E+03	1.1E+00	1.5E+00	4.8E+00	10	325	4.88E+03	97%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T04-B	1	7.72E+02			7.72E+02	1.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T05-B	1	3.97E+02			3.97E+02	2.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T06-B	1	2.35E+02			2.35E+02	2.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T07-B	1	7.98E+01			7.98E+01	7.1E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T08-B	1	1.05E+02			1.05E+02	6.0E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T09-B	1	6.01E+03			6.01E+03	6.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T01-C	1	5.69E+03			5.69E+03	1.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T02-C	1	2.31E+03			2.31E+03	1.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T03-C	1	2.18E+03			2.18E+03	1.0E+00	1.5E+00	4.8E+00	10	325	5.27E+03	95%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T04-C	1	7.79E+02			7.79E+02	3.6E-01	1.5E+00	4.8E+00					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T05-C	1	3.72E+02			3.72E+02	1.1E+00	1.5E+00	4.8E+00					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T06-C	1	2.38E+02			2.38E+02	1.0E+00	1.5E+00	4.8E+00					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T07-C	1	8.01E+01			8.01E+01	8.8E-01	1.5E+00	4.8E+00					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T08-C	1	9.98E+01			9.98E+01	9.6E-01	1.5E+00	4.8E+00					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-T09-C	1	5.82E+03			5.82E+03	2.5E-01	1.5E+00	4.8E+00					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-B01-A	1	9.84E+00			9.84E+00	2.8E+01	1.5E+00	4.8E+00					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-B02-A	1	8.67E+00			8.67E+00	4.5E+00	1.5E+00	4.8E+00					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1313-B03-A	1	7.50E-01	U1/2		7.50E-01	1.2E+01	1.5E+00	4.8E+00					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	EaFA-L01-1313-T01-A	1	1.60E+02			1.60E+02	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 10:51 AM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T02-A	1	7.84E+00			7.84E+00	4.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 10:53 AM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T03-A	1	5.00E-01	U1/2		5.00E-01	1.1E+02	1.0E+00	3.2E+00	10	325	3.55E+03	109%	VU ICP-OES	6/9/10 10:55 AM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T04-A	1	6.71E+01			6.71E+01	3.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:18 PM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T05-A	1	4.08E+01			4.08E+01	3.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:20 PM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T06-A	1	2.03E+01			2.03E+01	4.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:00 AM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T07-A	1	1.23E+03			1.23E+03	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:01 AM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T08-A	1	1.16E+03			1.16E+03	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:22 PM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T09-A	1	1.63E+03			1.63E+03	7.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:23 PM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T01-B	1	4.06E+02			4.06E+02	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:16 AM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T02-B	1	3.27E+02			3.27E+02	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:18 AM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T03-B	1	2.27E+02			2.27E+02	6.4E-01	1.0E+00	3.2E+00	10	325	3.65E+03	105%	VU ICP-OES	6/9/10 11:19 AM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T04-B	1	6.54E+01			6.54E+01	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:21 AM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T05-B	1	4.12E+01			4.12E+01	2.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:23 AM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T06-B	1	2.38E+01			2.38E+01	2.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:24 AM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T07-B	1	1.30E+03			1.30E+03	4.5E-02	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:26 AM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T08-B	1	1.30E+03			1.30E+03	5.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:27 AM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T09-B	1	1.69E+03			1.69E+03	6.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:29 AM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T01-C	1	1.71E+02			1.71E+02	3.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:36 AM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T02-C	1	2.39E+01			2.39E+01	9.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:37 AM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T03-C	1	2.46E+01			2.46E+01	5.3E+00	1.0E+00	3.2E+00	10	325	3.45E+03	105%	VU ICP-OES	6/9/10 11:39 AM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T04-C	1	2.25E+01			2.25E+01	2.6E+00	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:41 AM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T05-C	1	2.38E+01			2.38E+01	5.3E+00	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:42 AM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T06-C	1	3.46E+01			3.46E+01	5.0E-01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:46 AM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T07-C	1	1.13E+03			1.13E+03	9.3E-01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:48 AM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T08-C	1	1.07E+03			1.07E+03	1.0E+00	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:50 AM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-T09-C	1	1.57E+03			1.57E+03	7.1E-01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 11:51 AM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-B01-A	1	3.23E+00			3.23E+00	2.7E+01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 10:46 AM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-B02-A	1	2.13E+01			2.13E+01	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 10:48 AM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1313-B03-A	1	3.80E+00			3.80E+00	6.2E+00	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 10:50 AM	EPA Interlab L01 1313-1316 EaFA

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	EaFA-L02-1313-T01-A	1	3.73E+04			3.73E+04	8.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T02-A	1	2.94E+04			2.94E+04	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T03-A	1	2.03E+04			2.03E+04	5.7E+00	1.0E+00	3.2E+00	1000	100	2.12E+04	90%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T04-A	1	4.62E+03			4.62E+03	3.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T05-A	1	2.70E+02			2.70E+02	4.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T06-A	1	1.64E+02			1.64E+02	3.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T07-A	1	1.72E+02			1.72E+02	7.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T08-A	1	3.06E+04			3.06E+04	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T09-A	1	1.19E+05			1.19E+05	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T01-B	1	3.75E+04			3.75E+04	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T02-B	1	3.10E+04			3.10E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T03-B	1	2.17E+04			2.17E+04	5.0E-01	1.0E+00	3.2E+00	1000	100	2.26E+04	94%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T04-B	1	4.15E+03			4.15E+03	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T05-B	1	5.02E+02			5.02E+02	2.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T06-B	1	1.34E+02			1.34E+02	1.0E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T07-B	1	5.40E+02			5.40E+02	4.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T08-B	1	2.92E+04			2.92E+04	2.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T09-B	1	1.17E+05			1.17E+05	1.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T01-C	1	3.29E+04			3.29E+04	8.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T02-C	1	2.90E+04			2.90E+04	8.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T03-C	1	2.07E+04			2.07E+04	1.3E+00	1.0E+00	3.2E+00	1000	100	2.16E+04	90%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T04-C	1	4.48E+03			4.48E+03	4.8E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T05-C	1	6.31E+02			6.31E+02	3.9E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T06-C	1	1.39E+02			1.39E+02	1.6E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T07-C	1	2.14E+02			2.14E+02	8.5E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T08-C	1	2.96E+04			2.96E+04	7.2E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-T09-C	1	1.07E+05			1.07E+05	1.9E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	7.2E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
Al	EaFA-L02-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	EaFA-L02-1313-T01-A	1	2.12E+02			2.12E+02	1.6E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T02-A	1	1.86E+02			1.86E+02	1.5E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T03-A	1	1.72E+02			1.72E+02	1.5E+01	7.5E+00	2.4E+01	10	325	3.64E+03	107%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T04-A	1	2.26E+02			2.26E+02	1.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T05-A	1	2.30E+02			2.30E+02	3.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T06-A	1	1.51E+02			1.51E+02	1.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T07-A	1	1.74E+02			1.74E+02	7.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T08-A	1	3.81E+01			3.81E+01	3.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T09-A	1	3.75E+00	U1/2		3.75E+00	3.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T01-B	1	2.27E+02			2.27E+02	2.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T02-B	1	2.02E+02			2.02E+02	7.4E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T03-B	1	1.95E+02			1.95E+02	6.4E+00	7.5E+00	2.4E+01	10	325	3.65E+03	106%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T04-B	1	1.99E+02			1.99E+02	2.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T05-B	1	2.03E+02			2.03E+02	5.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T06-B	1	1.95E+02			1.95E+02	8.6E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T07-B	1	1.20E+02			1.20E+02	1.0E+02	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T08-B	1	2.96E+01			2.96E+01	3.5E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T09-B	1	3.75E+00	U1/2		3.75E+00	3.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T01-C	1	1.90E+02			1.90E+02	9.9E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T02-C	1	1.81E+02			1.81E+02	1.4E+02	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T03-C	1	2.02E+02			2.02E+02	4.8E+00	7.5E+00	2.4E+01	10	325	3.86E+03	113%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T04-C	1	1.75E+02			1.75E+02	1.6E+01	7.5E+00	2.4E+01					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T05-C	1	2.06E+02			2.06E+02	5.4E+00	7.5E+00	2.4E+01					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T06-C	1	1.82E+02			1.82E+02	1.6E+01	7.5E+00	2.4E+01					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T07-C	1	1.61E+02			1.61E+02	1.6E+01	7.5E+00	2.4E+01					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T08-C	1	3.73E+01			3.73E+01	9.8E+00	7.5E+00	2.4E+01					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-T09-C	1	3.75E+00	U1/2		3.75E+00	8.7E+01	7.5E+00	2.4E+01					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-B01-A	1	1.80E+01	E		1.80E+01	1.1E+02	7.5E+00	2.4E+01					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-B02-A	1	3.75E+00	U1/2		3.75E+00	3.8E+02	7.5E+00	2.4E+01					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFA-L02-1313-B03-A	1	1.96E+01	E		1.96E+01	1.4E+02	7.5E+00	2.4E+01					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	EaFA-L02-1313-T01-A	1	6.39E+03			6.39E+03	1.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T02-A	1	1.40E+03			1.40E+03	1.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T03-A	1	1.33E+03			1.33E+03	6.6E+00	1.1E+01	3.5E+01	10	325	4.74E+03	105%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T04-A	1	5.97E+02			5.97E+02	7.9E-01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T05-A	1	1.67E+02			1.67E+02	1.5E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T06-A	1	1.12E+02			1.12E+02	1.7E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T07-A	1	1.45E+02			1.45E+02	5.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T08-A	1	1.24E+02			1.24E+02	1.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T09-A	1	4.78E+02			4.78E+02	1.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T01-B	1	6.32E+03			6.32E+03	1.5E-01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T02-B	1	1.53E+03			1.53E+03	3.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T03-B	1	1.45E+03			1.45E+03	2.5E+00	1.1E+01	3.5E+01	10	325	4.72E+03	101%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T04-B	1	5.55E+02			5.55E+02	3.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T05-B	1	1.86E+02			1.86E+02	1.2E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T06-B	1	1.11E+02			1.11E+02	1.3E+02	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T07-B	1	1.29E+02			1.29E+02	7.8E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T08-B	1	9.01E+01			9.01E+01	7.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T09-B	1	4.62E+02			4.62E+02	2.8E-01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T01-C	1	6.19E+03			6.19E+03	8.4E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T02-C	1	1.38E+03			1.38E+03	9.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T03-C	1	1.38E+03			1.38E+03	1.8E+00	1.1E+01	3.5E+01	10	325	5.01E+03	112%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T04-C	1	5.86E+02			5.86E+02	4.3E+00	1.1E+01	3.5E+01					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T05-C	1	2.30E+02			2.30E+02	1.3E+01	1.1E+01	3.5E+01					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T06-C	1	9.02E+01			9.02E+01	2.4E+01	1.1E+01	3.5E+01					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T07-C	1	1.21E+02			1.21E+02	9.3E+00	1.1E+01	3.5E+01					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T08-C	1	1.25E+02			1.25E+02	1.7E+01	1.1E+01	3.5E+01					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-T09-C	1	4.78E+02			4.78E+02	1.1E+01	1.1E+01	3.5E+01					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-B01-A	1	1.93E+01	E		1.93E+01	2.9E+01	1.1E+01	3.5E+01					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-B02-A	1	5.50E+00	U1/2		5.50E+00	1.3E+03	1.1E+01	3.5E+01					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
As	EaFA-L02-1313-B03-A	1	1.64E+01	E		1.64E+01	5.4E+01	1.1E+01	3.5E+01					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	EaFA-L02-1313-T01-A	1	3.03E+03			3.03E+03	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T02-A	1	3.66E+03			3.66E+03	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T03-A	1	3.53E+03			3.53E+03	7.9E+00	1.0E+00	3.2E+00	1000	100	4.54E+03	101%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T04-A	1	3.94E+03			3.94E+03	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T05-A	1	4.26E+03			4.26E+03	2.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T06-A	1	4.27E+03			4.27E+03	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T07-A	1	4.46E+03			4.46E+03	6.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T08-A	1	3.74E+03			3.74E+03	6.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T09-A	1	2.98E+03			2.98E+03	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T01-B	1	3.03E+03			3.03E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T02-B	1	3.59E+03			3.59E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T03-B	1	3.75E+03			3.75E+03	1.9E+00	1.0E+00	3.2E+00	1000	100	4.71E+03	95%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T04-B	1	4.02E+03			4.02E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T05-B	1	4.21E+03			4.21E+03	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T06-B	1	4.24E+03			4.24E+03	7.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T07-B	1	4.18E+03			4.18E+03	6.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T08-B	1	3.63E+03			3.63E+03	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T09-B	1	2.98E+03			2.98E+03	9.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T01-C	1	2.72E+03			2.72E+03	7.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T02-C	1	3.54E+03			3.54E+03	8.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T03-C	1	3.62E+03			3.62E+03	9.1E-01	1.0E+00	3.2E+00	1000	100	4.71E+03	109%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T04-C	1	4.00E+03			4.00E+03	1.6E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T05-C	1	4.31E+03			4.31E+03	5.4E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T06-C	1	4.57E+03			4.57E+03	1.7E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T07-C	1	4.75E+03			4.75E+03	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T08-C	1	3.66E+03			3.66E+03	4.4E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-T09-C	1	2.67E+03			2.67E+03	1.8E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-B01-A	1	7.66E+01			7.66E+01	2.2E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-B02-A	1	6.34E+01			6.34E+01	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
B	EaFA-L02-1313-B03-A	1	6.26E+01			6.26E+01	3.3E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	EaFA-L02-1313-T01-A	1	2.32E+03			2.32E+03	6.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T02-A	1	1.19E+03			1.19E+03	5.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T03-A	1	1.42E+03			1.42E+03	6.5E+00	1.0E+00	3.2E+00	10	325	4.45E+03	93%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T04-A	1	3.97E+02			3.97E+02	3.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T05-A	1	2.67E+02			2.67E+02	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T06-A	1	2.80E+02			2.80E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T07-A	1	2.77E+02			2.77E+02	6.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T08-A	1	2.86E+02			2.86E+02	1.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T09-A	1	8.47E+02			8.47E+02	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T01-B	1	2.36E+03			2.36E+03	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T02-B	1	1.06E+03			1.06E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T03-B	1	1.60E+03			1.60E+03	5.5E-01	1.0E+00	3.2E+00	10	325	4.50E+03	89%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T04-B	1	3.97E+02			3.97E+02	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T05-B	1	2.71E+02			2.71E+02	2.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T06-B	1	2.58E+02			2.58E+02	7.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T07-B	1	2.69E+02			2.69E+02	5.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T08-B	1	3.15E+02			3.15E+02	2.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T09-B	1	8.57E+02			8.57E+02	1.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T01-C	1	2.08E+03			2.08E+03	8.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T02-C	1	1.77E+03			1.77E+03	9.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T03-C	1	5.54E+02			5.54E+02	2.5E+00	1.0E+00	3.2E+00	10	325	3.82E+03	101%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T04-C	1	4.08E+02			4.08E+02	3.1E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T05-C	1	2.73E+02			2.73E+02	1.3E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T06-C	1	2.93E+02			2.93E+02	5.0E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T07-C	1	3.06E+02			3.06E+02	2.9E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T08-C	1	2.73E+02			2.73E+02	5.1E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-T09-C	1	8.20E+02			8.20E+02	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	2.1E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	7.7E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFA-L02-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	5.7E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	EaFA-L02-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	6.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	7.9E+02	1.9E+00	6.0E+00	10	325	3.40E+03	104%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	5.6E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	6.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T07-A	1	2.42E+00	E		2.42E+00	1.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T08-A	1	1.29E+02			1.29E+02	5.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T09-A	1	2.56E+02			2.56E+02	3.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	9.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	9.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	1.7E+02	1.9E+00	6.0E+00	10	325	3.38E+03	104%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	5.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	3.9E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	7.6E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T07-B	1	4.33E+00	E		4.33E+00	6.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T08-B	1	1.27E+02			1.27E+02	2.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T09-B	1	2.56E+02			2.56E+02	1.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	2.6E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	3.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	3.7E+02	1.9E+00	6.0E+00	10	325	3.59E+03	111%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	3.4E+02	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	5.0E+02	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	3.7E+02	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T07-C	1	2.60E+00	E		2.60E+00	6.3E+00	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T08-C	1	1.25E+02			1.25E+02	5.6E+00	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-T09-C	1	2.45E+02			2.45E+02	6.0E+00	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	6.1E+02	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	2.3E+02	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
Be	EaFA-L02-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	2.0E+01	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	EaFA-L02-1313-T01-A	1	1.10E+00	U1/2		1.10E+00	6.7E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T02-A	1	1.10E+00	U1/2		1.10E+00	3.7E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	4.6E+01	2.2E+00	7.0E+00	10	325	3.48E+03	107%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T04-A	1	1.10E+00	U1/2		1.10E+00	1.9E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T05-A	1	1.10E+00	U1/2		1.10E+00	3.7E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T06-A	1	1.10E+00	U1/2		1.10E+00	1.0E+02	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T07-A	1	2.37E+01			2.37E+01	6.2E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T08-A	1	3.19E+01			3.19E+01	1.5E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T09-A	1	3.08E+01			3.08E+01	1.1E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T01-B	1	1.10E+00	U1/2		1.10E+00	3.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T02-B	1	1.10E+00	U1/2		1.10E+00	7.3E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	2.8E+01	2.2E+00	7.0E+00	10	325	3.49E+03	107%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T04-B	1	1.10E+00	U1/2		1.10E+00	2.7E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T05-B	1	1.10E+00	U1/2		1.10E+00	1.0E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T06-B	1	1.10E+00	U1/2		1.10E+00	9.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T07-B	1	1.91E+01			1.91E+01	6.5E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T08-B	1	3.11E+01			3.11E+01	3.4E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T09-B	1	3.15E+01			3.15E+01	3.8E-01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T01-C	1	1.10E+00	U1/2		1.10E+00	6.9E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T02-C	1	1.10E+00	U1/2		1.10E+00	7.5E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	1.6E+01	2.2E+00	7.0E+00	10	325	3.66E+03	113%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T04-C	1	1.10E+00	U1/2		1.10E+00	9.5E+01	2.2E+00	7.0E+00					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T05-C	1	1.10E+00	U1/2		1.10E+00	9.9E+01	2.2E+00	7.0E+00					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T06-C	1	1.10E+00	U1/2		1.10E+00	9.6E+01	2.2E+00	7.0E+00					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T07-C	1	2.53E+01			2.53E+01	5.2E+00	2.2E+00	7.0E+00					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T08-C	1	3.09E+01			3.09E+01	6.2E+00	2.2E+00	7.0E+00					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-T09-C	1	2.94E+01			2.94E+01	9.8E+00	2.2E+00	7.0E+00					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	1.8E+01	2.2E+00	7.0E+00					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	1.1E+01	2.2E+00	7.0E+00					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFA-L02-1313-B03-A	1	1.10E+00	U1/2		1.10E+00	9.6E+01	2.2E+00	7.0E+00					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	EaFA-L02-1313-T01-A	1	1.79E+04			1.79E+04	4.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T02-A	1	4.85E+04			4.85E+04	5.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T03-A	1	7.67E+04			7.67E+04	5.5E+00	2.6E+00	8.3E+00	1000	100	7.76E+04	90%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T04-A	1	1.32E+05			1.32E+05	3.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T05-A	1	1.54E+05			1.54E+05	5.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T06-A	1	1.61E+05			1.61E+05	1.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T07-A	1	1.70E+05			1.70E+05	6.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T08-A	1	1.53E+05			1.53E+05	2.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T09-A	1	1.41E+05			1.41E+05	1.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T01-B	1	1.83E+04			1.83E+04	7.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T02-B	1	4.77E+04			4.77E+04	9.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T03-B	1	8.08E+04			8.08E+04	1.5E+00	2.6E+00	8.3E+00	1000	100	8.16E+04	85%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T04-B	1	1.33E+05			1.33E+05	4.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T05-B	1	1.52E+05			1.52E+05	5.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T06-B	1	1.52E+05			1.52E+05	7.8E+01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T07-B	1	1.51E+05			1.51E+05	4.6E+01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T08-B	1	1.50E+05			1.50E+05	2.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T09-B	1	1.41E+05			1.41E+05	6.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T01-C	1	1.70E+04			1.70E+04	8.1E+01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T02-C	1	4.77E+04			4.77E+04	8.9E+01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T03-C	1	7.74E+04			7.74E+04	1.9E+00	2.6E+00	8.3E+00	1000	100	7.83E+04	88%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T04-C	1	1.29E+05			1.29E+05	2.8E-01	2.6E+00	8.3E+00					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T05-C	1	1.52E+05			1.52E+05	3.5E-01	2.6E+00	8.3E+00					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T06-C	1	1.68E+05			1.68E+05	2.0E-01	2.6E+00	8.3E+00					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T07-C	1	1.73E+05			1.73E+05	2.4E-01	2.6E+00	8.3E+00					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T08-C	1	1.46E+05			1.46E+05	6.3E+00	2.6E+00	8.3E+00					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-T09-C	1	1.30E+05			1.30E+05	1.1E+01	2.6E+00	8.3E+00					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-B01-A	1	1.30E+00	U1/2		1.30E+00	3.7E+02	2.6E+00	8.3E+00					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-B02-A	1	6.39E+00	E		6.39E+00	2.0E+02	2.6E+00	8.3E+00					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFA-L02-1313-B03-A	1	1.30E+00	U1/2		1.30E+00	3.3E+02	2.6E+00	8.3E+00					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	EaFA-L02-1313-T01-A	1	5.93E+02			5.93E+02	6.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T02-A	1	4.51E+02			4.51E+02	3.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T03-A	1	3.70E+02			3.70E+02	7.3E+00	1.2E+00	3.8E+00	10	325	3.64E+03	101%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T04-A	1	2.56E+02			2.56E+02	2.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T05-A	1	6.59E+01			6.59E+01	4.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T06-A	1	2.12E+01			2.12E+01	9.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T07-A	1	2.57E+00	E		2.57E+00	9.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T08-A	1	1.82E+02			1.82E+02	6.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T09-A	1	1.80E+03			1.80E+03	8.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T01-B	1	5.98E+02			5.98E+02	7.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T02-B	1	4.84E+02			4.84E+02	7.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T03-B	1	4.16E+02			4.16E+02	2.8E-01	1.2E+00	3.8E+00	10	325	3.67E+03	100%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T04-B	1	2.40E+02			2.40E+02	6.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T05-B	1	6.13E+01			6.13E+01	1.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T06-B	1	1.52E+01			1.52E+01	9.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T07-B	1	1.50E+00	E		1.50E+00	8.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T08-B	1	1.68E+02			1.68E+02	3.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T09-B	1	1.80E+03			1.80E+03	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T01-C	1	5.28E+02			5.28E+02	7.8E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T02-C	1	4.34E+02			4.34E+02	8.8E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T03-C	1	4.26E+02			4.26E+02	1.9E+00	1.2E+00	3.8E+00	10	325	3.88E+03	106%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T04-C	1	2.32E+02			2.32E+02	6.9E-01	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T05-C	1	6.40E+01			6.40E+01	5.0E+00	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T06-C	1	1.70E+01			1.70E+01	4.3E+00	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T07-C	1	3.14E+00	E		3.14E+00	1.6E+01	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T08-C	1	1.84E+02			1.84E+02	5.3E+00	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-T09-C	1	1.67E+03			1.67E+03	1.1E+01	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	1.8E+02	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	2.8E+03	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFA-L02-1313-B03-A	1	6.00E-01	U1/2		6.00E-01	1.3E+02	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	EaFA-L02-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	5.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	2.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	2.4E+01	1.8E+00	5.7E+00	10	325	3.34E+03	103%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	8.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T05-A	1	5.10E+00	E		5.10E+00	2.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T06-A	1	4.43E+01			4.43E+01	3.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T07-A	1	2.09E+02			2.09E+02	7.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T08-A	1	2.15E+02			2.15E+02	1.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T09-A	1	4.04E+02			4.04E+02	4.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	6.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	1.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	5.1E+01	1.8E+00	5.7E+00	10	325	3.38E+03	104%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	6.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T05-B	1	1.02E+01			1.02E+01	5.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T06-B	1	5.94E+01			5.94E+01	9.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T07-B	1	2.05E+02			2.05E+02	5.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T08-B	1	2.11E+02			2.11E+02	2.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T09-B	1	4.01E+02			4.01E+02	5.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	1.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	3.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	2.8E+01	1.8E+00	5.7E+00	10	325	3.50E+03	108%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T05-C	1	3.83E+00	E		3.83E+00	2.8E+01	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T06-C	1	6.09E+01			6.09E+01	1.9E+00	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T07-C	1	2.23E+02			2.23E+02	9.3E-01	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T08-C	1	2.04E+02			2.04E+02	4.3E+00	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-T09-C	1	3.76E+02			3.76E+02	1.1E+01	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	1.0E+02	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	8.3E+01	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
Co	EaFA-L02-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	2.1E+02	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	EaFA-L02-1313-T01-A	1	1.85E+00	U1/2		1.85E+00	3.6E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T02-A	1	1.85E+00	U1/2		1.85E+00	1.6E+02	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T03-A	1	5.53E+00	E		5.53E+00	1.5E+02	3.7E+00	1.2E+01	10	325	3.24E+03	100%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T04-A	1	5.14E+00	E		5.14E+00	1.6E+02	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T05-A	1	4.26E+00	E		4.26E+00	3.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T06-A	1	1.85E+00	U1/2		1.85E+00	7.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T07-A	1	4.48E+01			4.48E+01	7.1E+00	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T08-A	1	2.03E+03			2.03E+03	5.2E-01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T09-A	1	2.98E+03			2.98E+03	7.5E-01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T01-B	1	1.42E+01			1.42E+01	1.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T02-B	1	7.80E+00	E		7.80E+00	5.9E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T03-B	1	1.85E+00	U1/2		1.85E+00	6.4E+04	3.7E+00	1.2E+01	10	325	3.26E+03	100%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T04-B	1	6.65E+00	E		6.65E+00	5.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T05-B	1	1.02E+01	E		1.02E+01	6.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T06-B	1	8.46E+00	E		8.46E+00	1.5E+02	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T07-B	1	1.18E+02			1.18E+02	3.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T08-B	1	1.99E+03			1.99E+03	2.1E+00	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T09-B	1	3.00E+03			3.00E+03	3.5E-01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T01-C	1	1.66E+01			1.66E+01	1.6E+02	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T02-C	1	1.02E+01	E		1.02E+01	7.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T03-C	1	5.80E+00	E		5.80E+00	1.3E+02	3.7E+00	1.2E+01	10	325	3.42E+03	105%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T04-C	1	1.85E+00	U1/2		1.85E+00	6.4E+01	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T05-C	1	4.40E+00	E		4.40E+00	1.1E+02	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T06-C	1	1.85E+00	U1/2		1.85E+00	1.1E+02	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T07-C	1	5.02E+01			5.02E+01	1.7E+01	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T08-C	1	1.99E+03			1.99E+03	7.1E+00	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-T09-C	1	3.00E+03			3.00E+03	4.8E+00	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	7.5E+02	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	1.5E+02	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFA-L02-1313-B03-A	1	1.85E+00	U1/2		1.85E+00	3.2E+02	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	EaFA-L02-1313-T01-A	1	1.92E+01			1.92E+01	2.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T02-A	1	1.37E+01			1.37E+01	3.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T03-A	1	1.01E+01			1.01E+01	7.6E+00	2.0E+00	6.4E+00	1000	100	1.05E+03	104%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T04-A	1	5.24E+00	E		5.24E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	6.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T06-A	1	9.14E+00			9.14E+00	6.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T07-A	1	5.24E+00	E		5.24E+00	1.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T08-A	1	5.64E+02			5.64E+02	3.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T09-A	1	2.65E+04			2.65E+04	7.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T01-B	1	1.00E+01			1.00E+01	3.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T02-B	1	1.31E+01			1.31E+01	1.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T03-B	1	1.14E+01			1.14E+01	5.2E+00	2.0E+00	6.4E+00	1000	100	1.06E+03	105%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	2.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T06-B	1	2.73E+00	E		2.73E+00	2.7E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T07-B	1	2.80E+00	E		2.80E+00	1.7E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T08-B	1	5.24E+02			5.24E+02	1.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T09-B	1	2.60E+04			2.60E+04	7.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T01-C	1	2.04E+01			2.04E+01	1.3E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T02-C	1	2.07E+01			2.07E+01	1.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T03-C	1	3.79E+00	E		3.79E+00	1.1E+01	2.0E+00	6.4E+00	1000	100	1.09E+03	109%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T04-C	1	6.79E+00			6.79E+00	3.0E+00	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T05-C	1	3.15E+00	E		3.15E+00	1.6E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T06-C	1	5.88E+00	E		5.88E+00	7.9E+00	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T07-C	1	4.67E+00	E		4.67E+00	2.6E+00	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T08-C	1	5.69E+02			5.69E+02	7.7E+00	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-T09-C	1	2.60E+04			2.60E+04	3.6E+00	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFA-L02-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	4.2E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	EaFA-L02-1313-T01-A	1	3.40E+00	U1/2		3.40E+00	1.9E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T02-A	1	3.40E+00	U1/2		3.40E+00	5.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T03-A	1	3.40E+00	U1/2		3.40E+00	5.1E+01	6.8E+00	2.2E+01	10	325	3.26E+03	100%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T04-A	1	3.40E+00	U1/2		3.40E+00	2.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T05-A	1	3.40E+00	U1/2		3.40E+00	7.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T06-A	1	3.40E+00	U1/2		3.40E+00	4.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T07-A	1	3.40E+00	U1/2		3.40E+00	1.0E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T08-A	1	3.40E+00	U1/2		3.40E+00	1.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T09-A	1	5.16E+01			5.16E+01	1.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T01-B	1	3.40E+00	U1/2		3.40E+00	1.4E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T02-B	1	3.40E+00	U1/2		3.40E+00	6.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T03-B	1	3.40E+00	U1/2		3.40E+00	2.2E+01	6.8E+00	2.2E+01	10	325	3.29E+03	101%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T04-B	1	3.40E+00	U1/2		3.40E+00	4.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T05-B	1	3.40E+00	U1/2		3.40E+00	4.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T06-B	1	3.40E+00	U1/2		3.40E+00	4.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T07-B	1	3.40E+00	U1/2		3.40E+00	9.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T08-B	1	3.40E+00	U1/2		3.40E+00	6.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T09-B	1	5.38E+01			5.38E+01	9.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T01-C	1	3.40E+00	U1/2		3.40E+00	8.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T02-C	1	3.40E+00	U1/2		3.40E+00	4.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T03-C	1	3.40E+00	U1/2		3.40E+00	5.7E+01	6.8E+00	2.2E+01	10	325	3.40E+03	105%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T04-C	1	3.40E+00	U1/2		3.40E+00	6.9E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T05-C	1	3.40E+00	U1/2		3.40E+00	1.9E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T06-C	1	3.40E+00	U1/2		3.40E+00	4.4E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T07-C	1	3.40E+00	U1/2		3.40E+00	1.8E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T08-C	1	3.40E+00	U1/2		3.40E+00	5.3E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-T09-C	1	5.08E+01			5.08E+01	1.5E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	7.0E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	8.6E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFA-L02-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	2.5E+02	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	EaFA-L02-1313-T01-A	1	2.30E+03			2.30E+03	4.6E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T02-A	1	2.98E+03			2.98E+03	3.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T03-A	1	3.05E+03			3.05E+03	6.9E+00	1.9E+00	6.0E+00	10	325	6.31E+03	100%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T04-A	1	3.94E+03			3.94E+03	1.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T05-A	1	4.27E+03			4.27E+03	3.2E-02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T06-A	1	4.24E+03			4.24E+03	1.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T07-A	1	4.33E+03			4.33E+03	6.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T08-A	1	2.92E+03			2.92E+03	6.0E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T09-A	1	1.91E+03			1.91E+03	2.9E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T01-B	1	2.34E+03			2.34E+03	4.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T02-B	1	2.96E+03			2.96E+03	1.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T03-B	1	3.32E+03			3.32E+03	6.9E-01	1.9E+00	6.0E+00	10	325	6.29E+03	92%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T04-B	1	3.94E+03			3.94E+03	4.8E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T05-B	1	4.20E+03			4.20E+03	3.6E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T06-B	1	5.15E+03			5.15E+03	8.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T07-B	1	4.96E+03			4.96E+03	6.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T08-B	1	2.88E+03			2.88E+03	3.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T09-B	1	1.90E+03			1.90E+03	5.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T01-C	1	1.80E+03			1.80E+03	8.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T02-C	1	2.41E+03			2.41E+03	9.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T03-C	1	3.21E+03			3.21E+03	2.1E+00	1.9E+00	6.0E+00	10	325	6.58E+03	104%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T04-C	1	3.85E+03			3.85E+03	2.4E-01	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T05-C	1	4.19E+03			4.19E+03	5.9E-01	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T06-C	1	4.43E+03			4.43E+03	4.8E-01	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T07-C	1	4.41E+03			4.41E+03	9.8E-02	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T08-C	1	2.73E+03			2.73E+03	3.0E+00	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-T09-C	1	1.71E+03			1.71E+03	1.3E+01	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-B01-A	1	9.51E+00			9.51E+00	2.0E+01	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-B02-A	1	8.45E+00			8.45E+00	3.8E+00	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
Li	EaFA-L02-1313-B03-A	1	7.81E+00			7.81E+00	1.6E+01	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	EaFA-L02-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	2.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	5.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	7.2E+01	2.0E+00	6.4E+00	10	325	3.25E+03	100%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T04-A	1	6.21E+00	E		6.21E+00	6.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T05-A	1	1.04E+02			1.04E+02	5.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T06-A	1	3.44E+02			3.44E+02	1.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T07-A	1	8.30E+02			8.30E+02	5.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T08-A	1	1.14E+03			1.14E+03	3.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T09-A	1	1.65E+03			1.65E+03	4.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	3.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00	10	325	3.23E+03	99%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T04-B	1	7.40E+00			7.40E+00	7.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T05-B	1	1.34E+02			1.34E+02	3.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T06-B	1	3.99E+02			3.99E+02	7.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T07-B	1	7.79E+02			7.79E+02	4.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T08-B	1	1.12E+03			1.12E+03	2.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T09-B	1	1.65E+03			1.65E+03	5.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	2.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	3.3E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	5.6E+01	2.0E+00	6.4E+00	10	325	3.39E+03	104%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T04-C	1	6.79E+00			6.79E+00	2.8E+00	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T05-C	1	1.17E+02			1.17E+02	4.9E-01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T06-C	1	4.22E+02			4.22E+02	8.1E-01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T07-C	1	8.58E+02			8.58E+02	3.3E-01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T08-C	1	1.09E+03			1.09E+03	4.9E+00	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-T09-C	1	1.40E+03			1.40E+03	2.5E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.9E+02	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	2.3E+02	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFA-L02-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	5.8E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	EaFA-L02-1313-T01-A	1	1.03E+01			1.03E+01	4.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T02-A	1	1.82E+01			1.82E+01	3.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T03-A	1	6.06E+01			6.06E+01	1.6E+01	1.0E+00	3.2E+00	1000	100	1.07E+03	101%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T04-A	1	3.69E+03			3.69E+03	4.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T05-A	1	6.81E+03			6.81E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T06-A	1	7.69E+03			7.69E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T07-A	1	8.30E+03			8.30E+03	6.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T08-A	1	8.18E+03			8.18E+03	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T09-A	1	1.38E+04			1.38E+04	7.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T01-B	1	2.82E+00	E		2.82E+00	1.2E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T02-B	1	1.21E+01			1.21E+01	9.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T03-B	1	6.77E+01			6.77E+01	1.1E+01	1.0E+00	3.2E+00	1000	100	1.08E+03	101%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T04-B	1	3.77E+03			3.77E+03	4.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T05-B	1	6.72E+03			6.72E+03	1.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T06-B	1	7.55E+03			7.55E+03	8.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T07-B	1	7.82E+03			7.82E+03	7.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T08-B	1	7.99E+03			7.99E+03	2.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T09-B	1	1.39E+04			1.39E+04	2.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T01-C	1	5.00E-01	U1/2		5.00E-01	9.3E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T02-C	1	5.00E-01	U1/2		5.00E-01	2.6E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T03-C	1	6.81E+01			6.81E+01	3.8E+00	1.0E+00	3.2E+00	1000	100	1.13E+03	106%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T04-C	1	3.69E+03			3.69E+03	1.2E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T05-C	1	6.72E+03			6.72E+03	8.1E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T06-C	1	8.20E+03			8.20E+03	9.3E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T07-C	1	8.70E+03			8.70E+03	3.8E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T08-C	1	7.64E+03			7.64E+03	2.9E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-T09-C	1	1.19E+04			1.19E+04	2.2E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-B01-A	1	2.43E+00	E		2.43E+00	2.7E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-B02-A	1	1.91E+00	E		1.91E+00	1.6E+02	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFA-L02-1313-B03-A	1	9.19E+00			9.19E+00	4.6E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	EaFA-L02-1313-T01-A	1	4.33E+03			4.33E+03	2.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T02-A	1	4.34E+03			4.34E+03	8.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T03-A	1	4.01E+03			4.01E+03	7.9E+00	1.2E+00	3.8E+00	10	325	7.20E+03	98%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T04-A	1	4.01E+03			4.01E+03	3.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T05-A	1	3.86E+03			3.86E+03	3.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T06-A	1	3.45E+03			3.45E+03	2.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T07-A	1	1.51E+03			1.51E+03	6.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T08-A	1	1.42E+02			1.42E+02	9.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T09-A	1	2.06E+02			2.06E+02	1.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T01-B	1	4.39E+03			4.39E+03	5.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T02-B	1	4.25E+03			4.25E+03	1.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T03-B	1	4.35E+03			4.35E+03	3.1E-01	1.2E+00	3.8E+00	10	325	7.26E+03	90%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T04-B	1	3.97E+03			3.97E+03	7.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T05-B	1	3.80E+03			3.80E+03	6.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T06-B	1	3.22E+03			3.22E+03	7.8E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T07-B	1	9.62E+02			9.62E+02	5.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T08-B	1	1.37E+02			1.37E+02	3.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T09-B	1	2.00E+02			2.00E+02	1.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T01-C	1	3.96E+03			3.96E+03	7.8E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T02-C	1	4.08E+03			4.08E+03	7.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T03-C	1	4.25E+03			4.25E+03	1.2E+00	1.2E+00	3.8E+00	10	325	7.77E+03	108%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T04-C	1	3.89E+03			3.89E+03	1.4E+00	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T05-C	1	3.84E+03			3.84E+03	5.5E-01	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T06-C	1	3.52E+03			3.52E+03	9.9E-01	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T07-C	1	1.47E+03			1.47E+03	5.5E-01	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T08-C	1	1.43E+02			1.43E+02	5.4E+00	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-T09-C	1	1.87E+02			1.87E+02	1.1E+01	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-B01-A	1	4.02E+00			4.02E+00	1.5E+01	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-B02-A	1	1.32E+00	E		1.32E+00	2.8E+02	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFA-L02-1313-B03-A	1	2.08E+01			2.08E+01	2.3E+01	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	EaFA-L02-1313-T01-A	1	2.21E+00	E		2.21E+00	2.9E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	2.0E+03	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	1.6E+02	1.8E+00	5.7E+00	10	325	3.36E+03	103%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T04-A	1	3.48E+00	E		3.48E+00	2.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T05-A	1	2.34E+01			2.34E+01	2.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T06-A	1	1.07E+02			1.07E+02	5.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T07-A	1	5.04E+02			5.04E+02	7.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T08-A	1	5.42E+02			5.42E+02	9.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T09-A	1	7.39E+02			7.39E+02	5.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	1.2E+04	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	1.2E+03	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	4.6E+02	1.8E+00	5.7E+00	10	325	3.38E+03	104%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T04-B	1	2.88E+00	E		2.88E+00	1.6E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T05-B	1	3.88E+01			3.88E+01	6.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T06-B	1	1.38E+02			1.38E+02	8.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T07-B	1	4.85E+02			4.85E+02	5.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T08-B	1	5.40E+02			5.40E+02	2.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T09-B	1	7.38E+02			7.38E+02	7.4E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T01-C		9.00E-01	U1/2		9.00E-01	4.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T02-C		9.00E-01	U1/2		9.00E-01	4.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T03-C		9.00E-01	U1/2		9.00E-01	4.7E+01	1.8E+00	5.7E+00	10	325	3.52E+03	108%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T04-C		9.00E-01	U1/2		9.00E-01	2.5E+02	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T05-C		3.09E+01			3.09E+01	1.1E+01	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T06-C		1.46E+02			1.46E+02	1.2E+00	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T07-C		5.22E+02			5.22E+02	1.1E+00	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T08-C		5.18E+02			5.18E+02	5.3E+00	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-T09-C		6.95E+02			6.95E+02	1.0E+01	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-B01-A		9.00E-01	U1/2		9.00E-01	8.4E+02	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-B02-A		2.40E+00	E		2.40E+00	4.4E+01	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFA-L02-1313-B03-A		9.00E-01	U1/2		9.00E-01	5.1E+02	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	EaFA-L02-1313-T01-A	1	6.93E+01			6.93E+01	2.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T02-A	1	6.84E+01			6.84E+01	2.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T03-A	1	5.89E+01			5.89E+01	2.5E+01	3.7E+00	1.2E+01	1000	100	1.11E+03	105%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T04-A	1	9.86E+01			9.86E+01	6.3E+00	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T05-A	1	4.13E+01			4.13E+01	2.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T06-A	1	6.14E+01			6.14E+01	1.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T07-A	1	5.62E+01			5.62E+01	3.2E+00	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T08-A	1	5.15E+01			5.15E+01	1.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T09-A	1	6.56E+02			6.56E+02	2.8E-01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T01-B	1	6.58E+01			6.58E+01	1.3E+00	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T02-B	1	5.65E+01			5.65E+01	6.2E+00	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T03-B	1	7.20E+01			7.20E+01	7.0E+00	3.7E+00	1.2E+01	1000	100	1.11E+03	104%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T04-B	1	1.16E+02			1.16E+02	4.8E+00	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T05-B	1	6.73E+01			6.73E+01	1.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T06-B	1	1.52E+01			1.52E+01	2.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T07-B	1	1.75E+01			1.75E+01	3.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T08-B	1	3.64E+01			3.64E+01	2.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T09-B	1	6.64E+02			6.64E+02	1.2E+00	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T01-C	1	4.67E+01			4.67E+01	4.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T02-C	1	5.54E+01			5.54E+01	2.9E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T03-C	1	6.01E+01			6.01E+01	2.8E+00	3.7E+00	1.2E+01	1000	100	1.18E+03	112%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T04-C	1	1.04E+02			1.04E+02	1.4E+00	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T05-C	1	9.16E+01			9.16E+01	1.2E+01	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T06-C	1	6.16E+01			6.16E+01	8.6E+00	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T07-C	1	5.44E+01			5.44E+01	1.3E+01	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T08-C	1	6.54E+01			6.54E+01	5.5E+00	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-T09-C	1	6.92E+02			6.92E+02	1.1E+01	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-B01-A	1	2.73E+01			2.73E+01	2.5E+01	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-B02-A	1	2.57E+01			2.57E+01	6.2E+00	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
P	EaFA-L02-1313-B03-A	1	4.07E+01			4.07E+01	1.0E+01	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	EaFA-L02-1313-T01-A	1	1.66E+06			1.66E+06	8.8E-02	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T02-A	1	4.68E+05			4.68E+05	4.9E-01	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T03-A	1	2.04E+05			2.04E+05	6.8E+00	1.6E+00	5.1E+00	1000	100	2.04E+05	82%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T04-A	1	1.07E+05			1.07E+05	3.0E+00	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T05-A	1	5.81E+04			5.81E+04	2.8E-01	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T06-A	1	2.48E+04			2.48E+04	1.4E+00	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T07-A	1	2.54E+04			2.54E+04	6.8E+00	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T08-A	1	1.97E+04			1.97E+04	7.8E-01	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T09-A	1	2.12E+04			2.12E+04	2.2E-01	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T01-B	1	1.68E+06			1.68E+06	6.9E-01	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T02-B	1	4.54E+05			4.54E+05	1.3E+00	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T03-B	1	2.25E+05			2.25E+05	1.7E+00	1.6E+00	5.1E+00	1000	100	2.26E+05	86%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T04-B	1	1.03E+05			1.03E+05	7.4E-01	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T05-B	1	5.26E+04			5.26E+04	4.0E-01	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T06-B	1	2.23E+04			2.23E+04	7.9E+01	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T07-B	1	2.18E+04			2.18E+04	4.8E+01	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T08-B	1	1.93E+04			1.93E+04	3.3E+00	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T09-B	1	2.12E+04			2.12E+04	1.8E-01	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T01-C	1	1.70E+06			1.70E+06	7.5E+01	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T02-C	1	5.07E+05			5.07E+05	8.5E+01	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T03-C	1	2.18E+05			2.18E+05	2.0E+00	1.6E+00	5.1E+00	1000	100	2.19E+05	81%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T04-C	1	1.00E+05			1.00E+05	3.1E-01	1.6E+00	5.1E+00					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T05-C	1	5.60E+04			5.60E+04	1.1E-01	1.6E+00	5.1E+00					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T06-C	1	2.60E+04			2.60E+04	8.2E-01	1.6E+00	5.1E+00					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T07-C	1	2.63E+04			2.63E+04	5.9E-01	1.6E+00	5.1E+00					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T08-C	1	1.85E+04			1.85E+04	5.1E+00	1.6E+00	5.1E+00					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-T09-C	1	1.93E+04			1.93E+04	1.2E+01	1.6E+00	5.1E+00					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-B01-A	1	1.01E+01			1.01E+01	1.8E+01	1.6E+00	5.1E+00					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-B02-A	1	2.71E+01			2.71E+01	1.5E+01	1.6E+00	5.1E+00					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
K	EaFA-L02-1313-B03-A	1	1.69E+06			1.69E+06	1.1E+00	1.6E+00	5.1E+00					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	EaFA-L02-1313-T01-A	1	6.88E+03			6.88E+03	1.2E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T02-A	1	6.26E+03			6.26E+03	2.0E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T03-A	1	5.14E+03			5.14E+03	7.2E+00	1.5E+01	4.8E+01	10	325	8.31E+03	98%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T04-A	1	3.43E+03			3.43E+03	5.2E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T05-A	1	1.83E+03			1.83E+03	1.4E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T06-A	1	1.05E+03			1.05E+03	5.5E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T07-A	1	4.93E+02			4.93E+02	1.2E+01	1.5E+01	4.8E+01			---		VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T08-A	1	8.05E+01			8.05E+01	2.9E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T09-A	1	1.98E+02			1.98E+02	2.0E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T01-B	1	6.99E+03			6.99E+03	1.2E-01	1.5E+01	4.8E+01			---		VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T02-B	1	6.29E+03			6.29E+03	1.6E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T03-B	1	5.63E+03			5.63E+03	4.4E-01	1.5E+01	4.8E+01	10	325	8.34E+03	83%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T04-B	1	3.28E+03			3.28E+03	3.7E-01	1.5E+01	4.8E+01			---		VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T05-B	1	1.69E+03			1.69E+03	2.2E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T06-B	1	9.81E+02			9.81E+02	8.1E+01	1.5E+01	4.8E+01			---		VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T07-B	1	4.07E+02			4.07E+02	6.6E+01	1.5E+01	4.8E+01			---		VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T08-B	1	7.03E+01			7.03E+01	4.2E+01	1.5E+01	4.8E+01			---		VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T09-B	1	2.19E+02			2.19E+02	9.9E-01	1.5E+01	4.8E+01			---		VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T01-C	1	6.67E+03			6.67E+03	8.3E+01	1.5E+01	4.8E+01			---		VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T02-C	1	5.91E+03			5.91E+03	9.0E+01	1.5E+01	4.8E+01			---		VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T03-C	1	5.64E+03			5.64E+03	2.4E+00	1.5E+01	4.8E+01	10	325	9.21E+03	110%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T04-C	1	3.40E+03			3.40E+03	1.8E-01	1.5E+01	4.8E+01					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T05-C	1	1.79E+03			1.79E+03	2.1E+00	1.5E+01	4.8E+01					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T06-C	1	1.11E+03			1.11E+03	2.7E+00	1.5E+01	4.8E+01					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T07-C	1	5.08E+02			5.08E+02	8.3E+00	1.5E+01	4.8E+01					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T08-C	1	9.63E+01			9.63E+01	1.8E+01	1.5E+01	4.8E+01					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-T09-C	1	2.02E+02			2.02E+02	1.7E+01	1.5E+01	4.8E+01					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-B01-A	1	7.50E+00	U1/2		7.50E+00	5.9E+02	1.5E+01	4.8E+01					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-B02-A	1	1.83E+01	E		1.83E+01	4.6E+01	1.5E+01	4.8E+01					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
Se	EaFA-L02-1313-B03-A	1	7.50E+00	U1/2		7.50E+00	1.0E+02	1.5E+01	4.8E+01					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	EaFA-L02-1313-T01-A	1	1.30E+04			1.30E+04	9.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T02-A	1	6.25E+03			6.25E+03	6.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T03-A	1	1.67E+03			1.67E+03	6.4E+00	1.1E+00	3.5E+00	1000	100	2.68E+03	101%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T04-A	1	4.46E+02			4.46E+02	3.7E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T05-A	1	1.19E+03			1.19E+03	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T06-A	1	2.23E+03			2.23E+03	1.8E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T07-A	1	6.71E+03			6.71E+03	7.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T08-A	1	2.12E+04			2.12E+04	4.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T09-A	1	6.82E+04			6.82E+04	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T01-B	1	1.31E+04			1.31E+04	9.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T02-B	1	6.31E+03			6.31E+03	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T03-B	1	1.85E+03			1.85E+03	8.8E-01	1.1E+00	3.5E+00	1000	100	2.71E+03	86%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T04-B	1	4.57E+02			4.57E+02	6.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T05-B	1	1.27E+03			1.27E+03	3.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T06-B	1	2.38E+03			2.38E+03	7.8E+01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T07-B	1	5.80E+03			5.80E+03	5.4E+01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T08-B	1	2.06E+04			2.06E+04	2.5E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T09-B	1	6.75E+04			6.75E+04	2.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T01-C	1	1.20E+04			1.20E+04	7.9E+01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T02-C	1	6.04E+03			6.04E+03	8.3E+01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T03-C	1	1.65E+03			1.65E+03	2.1E+00	1.1E+00	3.5E+00	1000	100	2.74E+03	109%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T04-C	1	4.41E+02			4.41E+02	6.0E-01	1.1E+00	3.5E+00					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T05-C	1	1.27E+03			1.27E+03	2.3E-01	1.1E+00	3.5E+00					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T06-C	1	2.59E+03			2.59E+03	5.1E-01	1.1E+00	3.5E+00					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T07-C	1	6.50E+03			6.50E+03	2.8E-01	1.1E+00	3.5E+00					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T08-C	1	2.16E+04			2.16E+04	5.2E+00	1.1E+00	3.5E+00					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-T09-C	1	6.71E+04			6.71E+04	3.4E+00	1.1E+00	3.5E+00					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-B01-A	1	3.19E+01			3.19E+01	1.4E+01	1.1E+00	3.5E+00					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-B02-A	1	5.50E-01	U1/2		5.50E-01	1.1E+02	1.1E+00	3.5E+00					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
Si	EaFA-L02-1313-B03-A	1	6.83E+03			6.83E+03	4.0E+00	1.1E+00	3.5E+00					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	EaFA-L02-1313-T01-A	1	6.67E+03			6.67E+03	6.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T02-A	1	6.15E+03			6.15E+03	7.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T03-A	1	5.46E+03			5.46E+03	7.6E+00	2.5E+00	8.0E+00	1000	100	6.41E+03	95%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T04-A	1	5.89E+03			5.89E+03	3.0E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T05-A	1	6.00E+03			6.00E+03	3.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T06-A	1	5.63E+03			5.63E+03	9.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T07-A	1	5.77E+03			5.77E+03	7.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T08-A	1	4.21E+03			4.21E+03	2.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T09-A	1	3.38E+03			3.38E+03	7.7E-02	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T01-B	1	6.60E+03			6.60E+03	8.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T02-B	1	6.02E+03			6.02E+03	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T03-B	1	5.90E+03			5.90E+03	5.5E-01	2.5E+00	8.0E+00	1000	100	6.88E+03	97%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T04-B	1	5.85E+03			5.85E+03	7.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T05-B	1	5.75E+03			5.75E+03	4.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T06-B	1	5.05E+03			5.05E+03	8.0E+01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T07-B	1	4.90E+03			4.90E+03	6.2E+01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T08-B	1	4.11E+03			4.11E+03	2.8E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T09-B	1	3.29E+03			3.29E+03	5.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T01-C	1	5.80E+03			5.80E+03	8.2E+01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T02-C	1	5.70E+03			5.70E+03	9.4E+01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T03-C	1	5.54E+03			5.54E+03	2.2E+00	2.5E+00	8.0E+00	1000	100	6.47E+03	93%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T04-C	1	5.73E+03			5.73E+03	3.2E-01	2.5E+00	8.0E+00					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T05-C	1	5.86E+03			5.86E+03	2.1E-01	2.5E+00	8.0E+00					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T06-C	1	5.90E+03			5.90E+03	9.9E-01	2.5E+00	8.0E+00					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T07-C	1	5.98E+03			5.98E+03	3.3E-01	2.5E+00	8.0E+00					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T08-C	1	3.96E+03			3.96E+03	4.4E+00	2.5E+00	8.0E+00					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-T09-C	1	3.06E+03			3.06E+03	1.2E+01	2.5E+00	8.0E+00					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-B01-A	1	1.25E+00	U1/2		1.25E+00	1.2E+02	2.5E+00	8.0E+00					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-B02-A	1	1.25E+00	U1/2		1.25E+00	1.6E+00	2.5E+00	8.0E+00					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
Na	EaFA-L02-1313-B03-A	1	5.67E+02			5.67E+02	5.3E-01	2.5E+00	8.0E+00					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	EaFA-L02-1313-T01-A	1	1.40E+03			1.40E+03	9.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T02-A	1	1.65E+03			1.65E+03	8.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T03-A	1	1.70E+03			1.70E+03	8.1E+00	1.0E+00	3.2E+00	1000	100	2.66E+03	96%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T04-A	1	2.06E+03			2.06E+03	2.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T05-A	1	2.21E+03			2.21E+03	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T06-A	1	2.31E+03			2.31E+03	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T07-A	1	2.70E+03			2.70E+03	7.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T08-A	1	3.26E+03			3.26E+03	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T09-A	1	5.43E+03			5.43E+03	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T01-B	1	1.42E+03			1.42E+03	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T02-B	1	1.65E+03			1.65E+03	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T03-B	1	1.85E+03			1.85E+03	1.1E+00	1.0E+00	3.2E+00	1000	100	2.69E+03	84%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T04-B	1	2.06E+03			2.06E+03	8.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T05-B	1	2.19E+03			2.19E+03	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T06-B	1	2.17E+03			2.17E+03	7.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T07-B	1	2.39E+03			2.39E+03	2.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T08-B	1	3.16E+03			3.16E+03	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T09-B	1	5.44E+03			5.44E+03	1.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T01-C	1	1.29E+03			1.29E+03	7.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T02-C	1	1.64E+03			1.64E+03	7.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T03-C	1	1.78E+03			1.78E+03	1.4E+00	1.0E+00	3.2E+00	1000	100	2.85E+03	107%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T04-C	1	2.00E+03			2.00E+03	1.7E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T05-C	1	2.20E+03			2.20E+03	3.1E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T06-C	1	2.43E+03			2.43E+03	8.7E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T07-C	1	2.81E+03			2.81E+03	5.2E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T08-C	1	3.11E+03			3.11E+03	5.9E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-T09-C	1	5.25E+03			5.25E+03	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	3.9E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.5E+02	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFA-L02-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	1.1E+02	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	EaFA-L02-1313-T01-A	1	1.90E+05			1.90E+05	6.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T02-A	1	1.74E+05			1.74E+05	6.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T03-A	1	1.56E+05			1.56E+05	6.3E+00	6.8E+00	2.2E+01	1000	100	1.57E+05	84%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T04-A	1	1.73E+05			1.73E+05	2.8E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T05-A	1	1.75E+05			1.75E+05	5.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T06-A	1	1.64E+05			1.64E+05	1.8E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T07-A	1	1.59E+05			1.59E+05	6.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T08-A	1	1.06E+05			1.06E+05	3.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T09-A	1	6.57E+04			6.57E+04	6.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T01-B	1	1.92E+05			1.92E+05	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T02-B	1	1.75E+05			1.75E+05	1.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T03-B	1	1.71E+05			1.71E+05	3.9E-01	6.8E+00	2.2E+01	1000	100	1.72E+05	87%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T04-B	1	1.72E+05			1.72E+05	3.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T05-B	1	1.71E+05			1.71E+05	3.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T06-B	1	1.53E+05			1.53E+05	7.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T07-B	1	1.38E+05			1.38E+05	5.7E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T08-B	1	1.07E+05			1.07E+05	2.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T09-B	1	6.58E+04			6.58E+04	2.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T01-C	1	1.78E+05			1.78E+05	8.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T02-C	1	1.73E+05			1.73E+05	9.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T03-C	1	1.70E+05			1.70E+05	2.2E+00	6.8E+00	2.2E+01	1000	100	1.71E+05	87%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T04-C	1	1.73E+05			1.73E+05	2.4E-01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T05-C	1	1.77E+05			1.77E+05	7.2E-02	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T06-C	1	1.79E+05			1.79E+05	7.2E-01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T07-C	1	1.68E+05			1.68E+05	2.3E-01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T08-C	1	1.07E+05			1.07E+05	5.1E+00	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-T09-C	1	6.32E+04			6.32E+04	9.0E+00	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	4.3E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	2.1E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
S	EaFA-L02-1313-B03-A	1	6.11E+01			6.11E+01	1.1E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	EaFA-L02-1313-T01-A	1	1.28E+01	E		1.28E+01	2.9E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T02-A	1	2.30E+00	U1/2		2.30E+00	3.9E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T03-A	1	2.30E+00	U1/2		2.30E+00	9.5E+00	4.6E+00	1.5E+01	10	325	3.23E+03	99%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T04-A	1	5.32E+00	E		5.32E+00	9.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T05-A	1	7.19E+00	E		7.19E+00	2.0E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T06-A	1	1.87E+01			1.87E+01	3.5E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T07-A	1	2.15E+01			2.15E+01	2.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T08-A	1	5.03E+01			5.03E+01	1.5E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T09-A	1	8.44E+01			8.44E+01	4.9E+00	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T01-B	1	2.30E+00	U1/2		2.30E+00	1.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T02-B	1	6.27E+00	E		6.27E+00	1.5E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T03-B	1	2.30E+00	U1/2		2.30E+00	4.1E+01	4.6E+00	1.5E+01	10	325	3.22E+03	99%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T04-B	1	5.12E+00	E		5.12E+00	1.2E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T05-B	1	2.30E+00	U1/2		2.30E+00	2.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T06-B	1	8.65E+00	E		8.65E+00	1.7E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T07-B	1	2.35E+01			2.35E+01	1.6E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T08-B	1	5.99E+01			5.99E+01	1.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T09-B	1	7.37E+01			7.37E+01	1.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T01-C	1	2.30E+00	U1/2		2.30E+00	1.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T02-C	1	2.30E+00	U1/2		2.30E+00	1.4E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T03-C	1	2.30E+00	U1/2		2.30E+00	1.5E+03	4.6E+00	1.5E+01	10	325	3.32E+03	102%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T04-C	1	1.19E+01	E		1.19E+01	1.2E+02	4.6E+00	1.5E+01					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T05-C	1	6.93E+00	E		6.93E+00	7.7E+01	4.6E+00	1.5E+01					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T06-C	1	1.52E+01			1.52E+01	7.3E+01	4.6E+00	1.5E+01					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T07-C	1	2.14E+01			2.14E+01	3.8E+01	4.6E+00	1.5E+01					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T08-C	1	5.57E+01			5.57E+01	2.1E+01	4.6E+00	1.5E+01					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-T09-C	1	7.01E+01			7.01E+01	1.4E+01	4.6E+00	1.5E+01					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	9.7E+03	4.6E+00	1.5E+01					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	1.4E+03	4.6E+00	1.5E+01					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFA-L02-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	1.5E+02	4.6E+00	1.5E+01					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	EaFA-L02-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	8.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	2.9E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	6.1E+01	2.0E+00	6.4E+00	10	325	3.37E+03	104%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	5.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	6.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	3.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T08-A	1	1.23E+01			1.23E+01	2.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T09-A	1	7.68E+02			7.68E+02	1.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	1.0E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00	10	325	3.35E+03	103%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	3.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	6.6E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	6.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T08-B	1	9.59E+00			9.59E+00	6.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T09-B	1	7.81E+02			7.81E+02	1.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	2.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	6.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	6.8E+02	2.0E+00	6.4E+00	10	325	3.49E+03	107%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	2.9E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	2.1E+02	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	5.3E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T08-C	1	1.25E+01			1.25E+01	1.3E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-T09-C	1	7.76E+02			7.76E+02	9.9E+00	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	2.7E+02	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFA-L02-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	4.7E+00	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	EaFA-L02-1313-T01-A	1	4.65E+03			4.65E+03	1.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T02-A	1	3.64E+03			3.64E+03	1.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T03-A	1	3.15E+03			3.15E+03	8.0E+00	1.5E+00	4.8E+00	10	325	6.35E+03	98%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T04-A	1	5.56E+02			5.56E+02	3.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T05-A	1	3.15E+02			3.15E+02	8.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T06-A	1	2.41E+02			2.41E+02	2.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T07-A	1	1.67E+02			1.67E+02	5.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T08-A	1	1.05E+02			1.05E+02	1.9E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T09-A	1	5.10E+03			5.10E+03	2.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T01-B	1	4.71E+03			4.71E+03	5.2E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T02-B	1	3.63E+03			3.63E+03	7.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T03-B	1	3.39E+03			3.39E+03	1.3E+00	1.5E+00	4.8E+00	10	325	6.41E+03	93%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T04-B	1	5.34E+02			5.34E+02	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T05-B	1	2.89E+02			2.89E+02	8.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T06-B	1	2.23E+02			2.23E+02	7.9E+01	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T07-B	1	1.41E+02			1.41E+02	5.6E+01	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T08-B	1	9.57E+01			9.57E+01	2.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T09-B	1	5.03E+03			5.03E+03	3.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T01-C	1	4.23E+03			4.23E+03	7.5E+01	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T02-C	1	3.44E+03			3.44E+03	7.6E+01	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T03-C	1	3.29E+03			3.29E+03	1.1E+00	1.5E+00	4.8E+00	10	325	6.81E+03	108%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T04-C	1	5.50E+02			5.50E+02	1.5E+00	1.5E+00	4.8E+00					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T05-C	1	3.05E+02			3.05E+02	1.2E+00	1.5E+00	4.8E+00					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T06-C	1	2.43E+02			2.43E+02	4.4E-01	1.5E+00	4.8E+00					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T07-C	1	1.58E+02			1.58E+02	1.3E+00	1.5E+00	4.8E+00					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T08-C	1	1.04E+02			1.04E+02	5.2E+00	1.5E+00	4.8E+00					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-T09-C	1	4.48E+03			4.48E+03	2.2E+01	1.5E+00	4.8E+00					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-B01-A	1	7.50E-01	U1/2		7.50E-01	1.6E+02	1.5E+00	4.8E+00					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-B02-A	1	7.50E-01	U1/2		7.50E-01	2.0E+02	1.5E+00	4.8E+00					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
V	EaFA-L02-1313-B03-A	1	2.36E+00	E		2.36E+00	3.6E+01	1.5E+00	4.8E+00					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	EaFA-L02-1313-T01-A	1	4.98E+01			4.98E+01	3.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/4/10 10:35 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T02-A	1	6.62E+00			6.62E+00	3.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/4/10 10:37 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T03-A	1	1.47E+01			1.47E+01	4.3E+00	1.0E+00	3.2E+00	10	325	3.47E+03	106%	VU ICP-OES	6/4/10 10:39 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T04-A	1	4.12E+00			4.12E+00	2.4E+01	1.0E+00	3.2E+00			---		VU ICP-OES	6/4/10 10:40 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T05-A	1	8.33E+00			8.33E+00	1.5E+01	1.0E+00	3.2E+00			---		VU ICP-OES	6/4/10 10:42 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T06-A	1	1.27E+01			1.27E+01	1.6E+01	1.0E+00	3.2E+00			---		VU ICP-OES	6/4/10 10:44 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T07-A	1	7.08E+02			7.08E+02	6.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/4/10 10:45 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T08-A	1	1.22E+03			1.22E+03	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/4/10 10:47 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T09-A	1	1.57E+03			1.57E+03	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/4/10 10:49 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T01-B	1	4.62E+01			4.62E+01	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/4/10 10:58 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T02-B	1	1.81E+01			1.81E+01	5.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/4/10 11:00 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T03-B	1	2.47E+00	E		2.47E+00	1.5E+01	1.0E+00	3.2E+00	10	325	3.46E+03	107%	VU ICP-OES	6/4/10 11:02 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T04-B	1	5.28E+00			5.28E+00	6.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/4/10 11:03 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T05-B	1	6.50E+00			6.50E+00	9.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/4/10 11:08 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T06-B	1	1.64E+01			1.64E+01	8.0E+01	1.0E+00	3.2E+00			---		VU ICP-OES	6/4/10 11:10 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T07-B	1	6.99E+02			6.99E+02	5.7E+01	1.0E+00	3.2E+00			---		VU ICP-OES	6/4/10 11:12 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T08-B	1	1.18E+03			1.18E+03	2.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/4/10 11:13 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T09-B	1	1.57E+03			1.57E+03	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/4/10 11:15 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T01-C	1	3.24E+01			3.24E+01	7.9E+01	1.0E+00	3.2E+00			---		VU ICP-OES	6/4/10 4:20 PM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T02-C	1	4.96E+00			4.96E+00	8.6E+01	1.0E+00	3.2E+00			---		VU ICP-OES	6/4/10 4:22 PM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T03-C	1	4.48E+00			4.48E+00	1.4E+01	1.0E+00	3.2E+00	10	325	3.63E+03	111%	VU ICP-OES	6/4/10 11:30 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T04-C	1	1.32E+01			1.32E+01	2.6E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:31 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T05-C	1	5.32E+00			5.32E+00	3.2E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:33 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T06-C	1	2.20E+01			2.20E+01	2.8E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:35 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T07-C	1	7.22E+02			7.22E+02	1.7E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:36 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T08-C	1	1.18E+03			1.18E+03	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:38 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-T09-C	1	1.55E+03			1.55E+03	3.7E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 11:40 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	6.4E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 10:30 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	5.3E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 10:32 AM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFA-L02-1313-B03-A	1	6.14E+00			6.14E+00	1.9E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 10:34 AM	EPA Interlab L02 1313-1316 EaFA

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	EaFA-L04-1313-T01-A	1	4.36E+04			4.36E+04	8.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T02-A	1	3.53E+04			3.53E+04	4.4E-01	1.0E+00	3.2E+00	1000	100	3.62E+04	98%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T03-A	1	2.40E+04			2.40E+04	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T04-A	1	1.19E+04			1.19E+04	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T05-A	1	9.64E+02			9.64E+02	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T06-A	1	1.62E+02			1.62E+02	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T07-A	1	9.97E+02			9.97E+02	1.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T08-A	1	3.61E+04			3.61E+04	2.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T09-A	1	1.16E+05			1.16E+05	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T01-B	1	4.44E+04			4.44E+04	5.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T02-B	1	3.64E+04			3.64E+04	6.8E-01	1.0E+00	3.2E+00	1000	100	3.74E+04	93%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T03-B	1	2.41E+04			2.41E+04	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T04-B	1	6.78E+03			6.78E+03	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T05-B	1	8.03E+02			8.03E+02	6.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T06-B	1	1.37E+02			1.37E+02	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T07-B	1	1.02E+03			1.02E+03	9.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T08-B	1	3.26E+04			3.26E+04	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T09-B	1	1.12E+05			1.12E+05	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T01-C	1	4.55E+04			4.55E+04	9.8E-02	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T02-C	1	3.61E+04			3.61E+04	5.0E-01	1.0E+00	3.2E+00	1000	100	3.71E+04	93%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T03-C	1	2.42E+04			2.42E+04	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T04-C	1	6.87E+03			6.87E+03	2.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T05-C	1	9.91E+02			9.91E+02	6.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T06-C	1	1.57E+02			1.57E+02	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T07-C	1	3.88E+02			3.88E+02	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T08-C	1	3.21E+04			3.21E+04	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-T09-C	1	1.12E+05			1.12E+05	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	2.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-B02-A	1	6.19E+00			6.19E+00	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1313-B03-A	1	3.66E+01			3.66E+01	5.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	EaFA-L04-1313-T01-A	1	2.71E+02			2.71E+02	6.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T02-A	1	1.55E+02			1.55E+02	2.8E+01	7.5E+00	2.4E+01	10	325	3.64E+03	107%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T03-A	1	1.91E+02			1.91E+02	1.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T04-A	1	1.65E+02			1.65E+02	1.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T05-A	1	1.68E+02			1.68E+02	1.6E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T06-A	1	1.62E+02			1.62E+02	1.5E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T07-A	1	8.27E+01			8.27E+01	9.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T08-A	1	1.79E+01	E		1.79E+01	5.5E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T09-A	1	3.75E+00	U1/2		3.75E+00	6.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T01-B	1	2.45E+02			2.45E+02	1.5E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T02-B	1	1.54E+02			1.54E+02	1.4E+01	7.5E+00	2.4E+01	10	325	3.88E+03	115%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T03-B	1	1.76E+02			1.76E+02	1.4E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T04-B	1	1.98E+02			1.98E+02	1.6E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T05-B	1	2.15E+02			2.15E+02	6.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T06-B	1	1.91E+02			1.91E+02	1.6E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T07-B	1	8.41E+01			8.41E+01	3.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T08-B	1	3.57E+01			3.57E+01	4.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T09-B	1	3.75E+00	U1/2		3.75E+00	1.5E+02	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T01-C	1	2.74E+02			2.74E+02	9.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T02-C	1	1.46E+02			1.46E+02	1.1E+01	7.5E+00	2.4E+01	10	325	3.66E+03	108%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T03-C	1	1.84E+02			1.84E+02	5.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T04-C	1	1.93E+02			1.93E+02	7.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T05-C	1	1.61E+02			1.61E+02	1.5E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T06-C	1	1.94E+02			1.94E+02	1.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T07-C	1	1.00E+02			1.00E+02	3.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T08-C	1	1.90E+01	E		1.90E+01	4.2E+02	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-T09-C	1	3.75E+00	U1/2		3.75E+00	7.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-B01-A	1	9.97E+00	E		9.97E+00	1.0E+02	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-B02-A	1	3.75E+00	U1/2		3.75E+00	7.3E+02	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1313-B03-A	1	3.75E+00	U1/2		3.75E+00	1.2E+02	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	EaFA-L04-1313-T01-A	1	1.22E+04			1.22E+04	8.4E-01	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T02-A	1	1.14E+03			1.14E+03	1.1E+00	1.1E+01	3.5E+01	10	325	4.68E+03	109%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T03-A	1	1.12E+03			1.12E+03	1.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T04-A	1	7.18E+02			7.18E+02	1.4E-01	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T05-A	1	2.73E+02			2.73E+02	3.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T06-A	1	1.30E+02			1.30E+02	1.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T07-A	1	1.24E+02			1.24E+02	5.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T08-A	1	1.32E+02			1.32E+02	2.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T09-A	1	1.07E+03			1.07E+03	9.0E-01	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T01-B	1	1.17E+04			1.17E+04	2.1E-01	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T02-B	1	1.15E+03			1.15E+03	1.2E+00	1.1E+01	3.5E+01	10	325	4.92E+03	116%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T03-B	1	1.01E+03			1.01E+03	6.4E-01	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T04-B	1	5.88E+02			5.88E+02	4.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T05-B	1	2.83E+02			2.83E+02	6.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T06-B	1	1.23E+02			1.23E+02	9.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T07-B	1	1.68E+02			1.68E+02	1.0E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T08-B	1	1.35E+02			1.35E+02	6.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T09-B	1	6.26E+02			6.26E+02	1.7E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T01-C	1	1.25E+04			1.25E+04	2.9E-01	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T02-C	1	1.14E+03			1.14E+03	1.4E+00	1.1E+01	3.5E+01	10	325	4.63E+03	107%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T03-C	1	1.11E+03			1.11E+03	9.4E-01	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T04-C	1	5.48E+02			5.48E+02	5.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T05-C	1	2.42E+02			2.42E+02	3.7E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T06-C	1	1.13E+02			1.13E+02	2.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T07-C	1	1.22E+02			1.22E+02	8.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T08-C	1	1.36E+02			1.36E+02	9.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-T09-C	1	9.12E+02			9.12E+02	8.6E-01	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-B01-A	1	3.09E+01	E		3.09E+01	2.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-B02-A	1	3.26E+01	E		3.26E+01	7.7E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1313-B03-A	1	4.09E+01			4.09E+01	3.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	EaFA-L04-1313-T01-A	1	4.99E+03			4.99E+03	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T02-A	1	4.52E+03			4.52E+03	6.8E-01	1.0E+00	3.2E+00	1000	100	5.39E+03	86%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T03-A	1	4.44E+03			4.44E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T04-A	1	4.48E+03			4.48E+03	3.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T05-A	1	4.61E+03			4.61E+03	2.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T06-A	1	4.61E+03			4.61E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T07-A	1	4.67E+03			4.67E+03	6.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T08-A	1	3.58E+03			3.58E+03	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T09-A	1	2.76E+03			2.76E+03	5.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T01-B	1	4.91E+03			4.91E+03	3.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T02-B	1	4.59E+03			4.59E+03	5.8E-01	1.0E+00	3.2E+00	1000	100	5.42E+03	83%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T03-B	1	4.42E+03			4.42E+03	2.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T04-B	1	4.45E+03			4.45E+03	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T05-B	1	4.46E+03			4.46E+03	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T06-B	1	4.65E+03			4.65E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T07-B	1	4.70E+03			4.70E+03	1.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T08-B	1	3.65E+03			3.65E+03	1.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T09-B	1	2.75E+03			2.75E+03	9.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T01-C	1	5.21E+03			5.21E+03	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T02-C	1	4.53E+03			4.53E+03	6.7E-01	1.0E+00	3.2E+00	1000	100	5.34E+03	81%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T03-C	1	4.45E+03			4.45E+03	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T04-C	1	4.33E+03			4.33E+03	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T05-C	1	4.47E+03			4.47E+03	5.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T06-C	1	4.58E+03			4.58E+03	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T07-C	1	4.96E+03			4.96E+03	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T08-C	1	3.63E+03			3.63E+03	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-T09-C	1	2.72E+03			2.72E+03	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-B01-A	1	3.63E+01			3.63E+01	2.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-B02-A	1	2.76E+01			2.76E+01	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1313-B03-A	1	2.95E+01			2.95E+01	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	EaFA-L04-1313-T01-A	1	7.05E+01			7.05E+01	1.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T02-A	1	1.17E+02			1.17E+02	5.6E-01	1.0E+00	3.2E+00	10	325	3.40E+03	101%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T03-A	1	1.28E+02			1.28E+02	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T04-A	1	2.93E+02			2.93E+02	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T05-A	1	3.46E+02			3.46E+02	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T06-A	1	3.35E+02			3.35E+02	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T07-A	1	3.21E+02			3.21E+02	3.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T08-A	1	2.08E+02			2.08E+02	2.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T09-A	1	2.06E+02			2.06E+02	1.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T01-B	1	6.02E+01			6.02E+01	4.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T02-B	1	1.22E+02			1.22E+02	3.4E-01	1.0E+00	3.2E+00	10	325	3.63E+03	108%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T03-B	1	1.35E+02			1.35E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T04-B	1	3.99E+02			3.99E+02	8.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T05-B	1	3.62E+02			3.62E+02	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T06-B	1	3.52E+02			3.52E+02	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T07-B	1	3.21E+02			3.21E+02	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T08-B	1	2.86E+02			2.86E+02	3.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T09-B	1	2.42E+02			2.42E+02	2.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T01-C	1	6.27E+01			6.27E+01	3.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T02-C	1	1.44E+02			1.44E+02	3.8E+00	1.0E+00	3.2E+00	10	325	3.39E+03	100%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T03-C	1	1.99E+02			1.99E+02	1.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T04-C	1	4.31E+02			4.31E+02	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T05-C	1	3.47E+02			3.47E+02	2.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T06-C	1	3.07E+02			3.07E+02	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T07-C	1	3.56E+02			3.56E+02	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T08-C	1	2.91E+02			2.91E+02	5.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-T09-C	1	2.33E+02			2.33E+02	3.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-B01-A	1	1.22E+00	E		1.22E+00	2.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-B02-A	1	6.07E+00			6.07E+00	3.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1313-B03-A	1	8.00E+00			8.00E+00	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	EaFA-L04-1313-T01-A	1	2.40E+00	E		2.40E+00	1.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	4.8E+01	1.9E+00	6.0E+00	10	325	3.51E+03	108%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	9.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	3.7E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	7.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T07-A	1	9.47E+00			9.47E+00	4.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T08-A	1	1.34E+02			1.34E+02	5.8E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T09-A	1	2.37E+02			2.37E+02	3.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	1.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	4.6E+01	1.9E+00	6.0E+00	10	325	3.72E+03	114%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	8.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	8.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	2.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T07-B	1	9.25E+00			9.25E+00	2.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T08-B	1	1.30E+02			1.30E+02	4.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T09-B	1	2.37E+02			2.37E+02	5.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T01-C	1	2.18E+00	E		2.18E+00	1.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00	10	325	3.49E+03	107%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	7.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	4.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	4.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T07-C	1	4.70E+00	E		4.70E+00	1.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T08-C	1	1.30E+02			1.30E+02	6.6E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-T09-C	1	2.35E+02			2.35E+02	1.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	2.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	7.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	3.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	EaFA-L04-1313-T01-A	1	1.10E+00	U1/2		1.10E+00	1.8E+02	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T02-A	1	1.10E+00	U1/2		1.10E+00	1.1E+02	2.2E+00	7.0E+00	10	325	3.51E+03	108%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	4.6E+02	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T04-A	1	1.10E+00	U1/2		1.10E+00	1.2E+03	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T05-A	1	1.10E+00	U1/2		1.10E+00	4.3E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T06-A	1	1.10E+00	U1/2		1.10E+00	5.8E+02	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T07-A	1	3.74E+01			3.74E+01	1.7E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T08-A	1	2.90E+01			2.90E+01	3.2E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T09-A	1	3.15E+01			3.15E+01	6.0E-01	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T01-B	1	1.10E+00	U1/2		1.10E+00	5.2E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T02-B	1	1.10E+00	U1/2		1.10E+00	4.8E+02	2.2E+00	7.0E+00	10	325	3.75E+03	115%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	7.1E+02	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T04-B	1	1.10E+00	U1/2		1.10E+00	4.1E+02	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T05-B	1	1.10E+00	U1/2		1.10E+00	3.1E+02	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T06-B	1	1.10E+00	U1/2		1.10E+00	1.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T07-B	1	3.71E+01			3.71E+01	1.3E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T08-B	1	3.00E+01			3.00E+01	1.1E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T09-B	1	3.09E+01			3.09E+01	1.9E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T01-C	1	1.10E+00	U1/2		1.10E+00	6.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T02-C	1	1.10E+00	U1/2		1.10E+00	2.5E+02	2.2E+00	7.0E+00	10	325	3.51E+03	108%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	2.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T04-C	1	1.10E+00	U1/2		1.10E+00	2.7E+02	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T05-C	1	1.10E+00	U1/2		1.10E+00	1.0E+03	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T06-C	1	1.10E+00	U1/2		1.10E+00	2.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T07-C	1	3.43E+01			3.43E+01	2.1E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T08-C	1	2.99E+01			2.99E+01	1.4E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-T09-C	1	3.15E+01			3.15E+01	1.3E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	1.7E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	1.4E+03	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1313-B03-A	1	1.10E+00	U1/2		1.10E+00	6.7E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	EaFA-L04-1313-T01-A	1	1.36E+04			1.36E+04	6.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T02-A	1	4.05E+04			4.05E+04	1.6E-01	2.6E+00	8.3E+00	1000	100	4.14E+04	83%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T03-A	1	9.18E+04			9.18E+04	8.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T04-A	1	1.23E+05			1.23E+05	5.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T05-A	1	1.43E+05			1.43E+05	7.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T06-A	1	1.54E+05			1.54E+05	2.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T07-A	1	1.56E+05			1.56E+05	5.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T08-A	1	1.33E+05			1.33E+05	6.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T09-A	1	1.21E+05			1.21E+05	3.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T01-B	1	1.47E+04			1.47E+04	2.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T02-B	1	3.92E+04			3.92E+04	2.0E-01	2.6E+00	8.3E+00	1000	100	4.01E+04	88%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T03-B	1	8.95E+04			8.95E+04	4.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T04-B	1	1.25E+05			1.25E+05	7.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T05-B	1	1.41E+05			1.41E+05	7.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T06-B	1	1.55E+05			1.55E+05	7.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T07-B	1	1.58E+05			1.58E+05	5.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T08-B	1	1.35E+05			1.35E+05	4.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T09-B	1	1.20E+05			1.20E+05	5.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T01-C	1	1.40E+04			1.40E+04	1.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T02-C	1	3.92E+04			3.92E+04	5.9E-01	2.6E+00	8.3E+00	1000	100	4.00E+04	81%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T03-C	1	9.32E+04			9.32E+04	5.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T04-C	1	1.22E+05			1.22E+05	4.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T05-C	1	1.39E+05			1.39E+05	3.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T06-C	1	1.52E+05			1.52E+05	6.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T07-C	1	1.68E+05			1.68E+05	5.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T08-C	1	1.35E+05			1.35E+05	7.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-T09-C	1	1.20E+05			1.20E+05	6.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-B01-A	1	1.86E+02			1.86E+02	6.9E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-B02-A	1	1.28E+03			1.28E+03	1.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1313-B03-A	1	1.38E+02			1.38E+02	4.3E+01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	EaFA-L04-1313-T01-A	1	5.40E+02			5.40E+02	3.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T02-A	1	3.32E+02			3.32E+02	8.8E-01	1.2E+00	3.8E+00	10	325	3.64E+03	102%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T03-A	1	2.58E+02			2.58E+02	2.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T04-A	1	1.90E+02			1.90E+02	5.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T05-A	1	9.70E+01			9.70E+01	1.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T06-A	1	1.94E+01			1.94E+01	5.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T07-A	1	3.61E+00	E		3.61E+00	6.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T08-A	1	2.52E+02			2.52E+02	4.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T09-A	1	1.61E+03			1.61E+03	6.5E-02	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T01-B	1	5.65E+02			5.65E+02	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T02-B	1	3.39E+02			3.39E+02	4.1E-01	1.2E+00	3.8E+00	10	325	3.85E+03	108%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T03-B	1	2.66E+02			2.66E+02	7.7E-02	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T04-B	1	1.73E+02			1.73E+02	3.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T05-B	1	8.08E+01			8.08E+01	1.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T06-B	1	1.87E+01			1.87E+01	1.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T07-B	1	2.24E+00	E		2.24E+00	5.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T08-B	1	2.15E+02			2.15E+02	5.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T09-B	1	1.61E+03			1.61E+03	5.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T01-C	1	5.76E+02			5.76E+02	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T02-C	1	3.52E+02			3.52E+02	8.1E-01	1.2E+00	3.8E+00	10	325	3.65E+03	102%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T03-C	1	2.56E+02			2.56E+02	3.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T04-C	1	1.74E+02			1.74E+02	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T05-C	1	9.35E+01			9.35E+01	1.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T06-C	1	2.45E+01			2.45E+01	2.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T07-C	1	2.14E+00	E		2.14E+00	7.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T08-C	1	2.01E+02			2.01E+02	4.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-T09-C	1	1.61E+03			1.61E+03	4.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	5.8E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	1.1E+02	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1313-B03-A	1	8.48E+00			8.48E+00	3.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	EaFA-L04-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	1.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00	10	325	3.26E+03	100%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T04-A	1	3.39E+00	E		3.39E+00	1.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T05-A	1	8.06E+00			8.06E+00	3.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T06-A	1	4.67E+01			4.67E+01	3.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T07-A	1	2.36E+02			2.36E+02	7.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T08-A	1	2.02E+02			2.02E+02	1.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T09-A	1	3.84E+02			3.84E+02	6.4E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	4.8E+01	1.8E+00	5.7E+00	10	325	3.48E+03	107%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	1.1E+03	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T05-B	1	7.41E+00			7.41E+00	1.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T06-B	1	5.74E+01			5.74E+01	3.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T07-B	1	2.35E+02			2.35E+02	1.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T08-B	1	2.03E+02			2.03E+02	8.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T09-B	1	3.75E+02			3.75E+02	8.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	1.9E+02	1.8E+00	5.7E+00	10	325	3.28E+03	101%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	8.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T05-C	1	4.76E+00	E		4.76E+00	5.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T06-C	1	3.82E+01			3.82E+01	1.9E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T07-C	1	2.35E+02			2.35E+02	8.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T08-C	1	2.02E+02			2.02E+02	3.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-T09-C	1	3.74E+02			3.74E+02	4.4E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	1.9E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	3.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1313-B03-A	1	1.81E+00	E		1.81E+00	6.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	EaFA-L04-1313-T01-A	1	8.48E+01			8.48E+01	1.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T02-A	1	1.85E+00	U1/2		1.85E+00	1.8E+02	3.7E+00	1.2E+01	10	325	3.26E+03	100%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T03-A	1	1.85E+00	U1/2		1.85E+00	4.7E+02	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T04-A	1	8.95E+00	E		8.95E+00	7.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T05-A	1	4.55E+00	E		4.55E+00	1.9E+02	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T06-A	1	8.58E+00	E		8.58E+00	6.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T07-A	1	2.39E+02			2.39E+02	1.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T08-A	1	2.00E+03			2.00E+03	9.8E-01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T09-A	1	2.74E+03			2.74E+03	1.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T01-B	1	1.42E+01			1.42E+01	5.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T02-B	1	1.85E+00	U1/2		1.85E+00	2.9E+02	3.7E+00	1.2E+01	10	325	3.48E+03	107%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T03-B	1	1.85E+00	U1/2		1.85E+00	1.0E+02	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T04-B	1	6.23E+00	E		6.23E+00	1.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T05-B	1	8.48E+00	E		8.48E+00	3.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T06-B	1	1.30E+01			1.30E+01	4.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T07-B	1	2.04E+02			2.04E+02	2.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T08-B	1	1.97E+03			1.97E+03	1.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T09-B	1	2.77E+03			2.77E+03	1.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T01-C	1	1.85E+00	U1/2		1.85E+00	2.4E+03	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T02-C	1	4.48E+00	E		4.48E+00	1.3E+02	3.7E+00	1.2E+01	10	325	3.26E+03	100%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T03-C	1	3.95E+00	E		3.95E+00	1.3E+02	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T04-C	1	1.85E+00	U1/2		1.85E+00	2.4E+02	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T05-C	1	1.04E+01	E		1.04E+01	4.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T06-C	1	9.57E+00	E		9.57E+00	4.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T07-C	1	7.31E+01			7.31E+01	5.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T08-C	1	1.94E+03			1.94E+03	1.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-T09-C	1	2.74E+03			2.74E+03	9.9E-02	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	6.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-B02-A	1	1.03E+01	E		1.03E+01	1.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1313-B03-A	1	8.60E+00	E		8.60E+00	6.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	EaFA-L04-1313-T01-A	1	6.41E+01			6.41E+01	2.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T02-A	1	1.51E+01			1.51E+01	3.3E+00	2.0E+00	6.4E+00	1000	100	1.03E+03	101%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T03-A	1	7.09E+00			7.09E+00	4.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	2.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T08-A	1	6.50E+02			6.50E+02	1.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T09-A	1	2.98E+04			2.98E+04	3.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T01-B	1	1.84E+01			1.84E+01	3.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T02-B	1	1.55E+01			1.55E+01	2.4E+00	2.0E+00	6.4E+00	1000	100	1.09E+03	108%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T03-B	1	6.68E+00			6.68E+00	1.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T04-B	1	2.80E+00	E		2.80E+00	1.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	3.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T06-B	1	2.50E+00	E		2.50E+00	2.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T07-B	1	4.01E+01			4.01E+01	1.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T08-B	1	5.08E+02			5.08E+02	9.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T09-B	1	2.67E+04			2.67E+04	6.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T01-C	1	1.39E+01			1.39E+01	3.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T02-C	1	1.28E+01			1.28E+01	1.4E+00	2.0E+00	6.4E+00	1000	100	1.02E+03	101%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T03-C	1	4.04E+00	E		4.04E+00	4.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T07-C	1	2.98E+00	E		2.98E+00	7.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T08-C	1	5.00E+02			5.00E+02	1.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-T09-C	1	2.83E+04			2.83E+04	6.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-B02-A	1	1.43E+01			1.43E+01	2.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1313-B03-A	1	9.81E+00			9.81E+00	5.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	EaFA-L04-1313-T01-A	1	3.40E+00	U1/2		3.40E+00	2.0E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T02-A	1	3.40E+00	U1/2		3.40E+00	8.4E+01	6.8E+00	2.2E+01	10	325	3.27E+03	100%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T03-A	1	3.40E+00	U1/2		3.40E+00	6.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T04-A	1	3.40E+00	U1/2		3.40E+00	3.4E+04	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T05-A	1	3.40E+00	U1/2		3.40E+00	5.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T06-A	1	3.40E+00	U1/2		3.40E+00	2.5E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T07-A	1	3.40E+00	U1/2		3.40E+00	1.1E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T08-A	1	3.40E+00	U1/2		3.40E+00	6.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T09-A	1	3.24E+01			3.24E+01	1.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T01-B	1	3.40E+00	U1/2		3.40E+00	3.0E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T02-B	1	3.40E+00	U1/2		3.40E+00	1.2E+02	6.8E+00	2.2E+01	10	325	3.48E+03	107%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T03-B	1	3.40E+00	U1/2		3.40E+00	4.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T04-B	1	3.40E+00	U1/2		3.40E+00	3.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T05-B	1	3.40E+00	U1/2		3.40E+00	3.1E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T06-B	1	3.40E+00	U1/2		3.40E+00	5.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T07-B	1	3.40E+00	U1/2		3.40E+00	1.1E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T08-B	1	3.40E+00	U1/2		3.40E+00	1.1E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T09-B	1	1.77E+01	E		1.77E+01	2.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T01-C	1	3.40E+00	U1/2		3.40E+00	2.5E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T02-C	1	3.40E+00	U1/2		3.40E+00	4.3E+02	6.8E+00	2.2E+01	10	325	3.25E+03	100%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T03-C	1	3.40E+00	U1/2		3.40E+00	3.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T04-C	1	3.40E+00	U1/2		3.40E+00	3.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T05-C	1	3.40E+00	U1/2		3.40E+00	8.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T06-C	1	3.40E+00	U1/2		3.40E+00	2.5E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T07-C	1	3.40E+00	U1/2		3.40E+00	4.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T08-C	1	3.40E+00	U1/2		3.40E+00	3.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-T09-C	1	3.23E+01			3.23E+01	5.8E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	3.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	7.7E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	1.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	EaFA-L04-1313-T01-A	1	2.48E+03			2.48E+03	6.2E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T02-A	1	3.13E+03			3.13E+03	2.6E-01	1.9E+00	6.0E+00	10	325	6.04E+03	90%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T03-A	1	3.54E+03			3.54E+03	9.6E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T04-A	1	3.66E+03			3.66E+03	5.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T05-A	1	3.80E+03			3.80E+03	7.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T06-A	1	3.83E+03			3.83E+03	5.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T07-A	1	3.69E+03			3.69E+03	6.2E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T08-A	1	2.34E+03			2.34E+03	6.9E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T09-A	1	1.54E+03			1.54E+03	8.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T01-B	1	2.50E+03			2.50E+03	1.2E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T02-B	1	3.23E+03			3.23E+03	1.7E-01	1.9E+00	6.0E+00	10	325	6.33E+03	95%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T03-B	1	3.48E+03			3.48E+03	1.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T04-B	1	3.62E+03			3.62E+03	1.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T05-B	1	3.74E+03			3.74E+03	1.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T06-B	1	3.90E+03			3.90E+03	7.0E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T07-B	1	3.72E+03			3.72E+03	2.8E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T08-B	1	2.43E+03			2.43E+03	2.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T09-B	1	1.55E+03			1.55E+03	8.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T01-C	1	2.54E+03			2.54E+03	8.6E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T02-C	1	3.17E+03			3.17E+03	8.2E-01	1.9E+00	6.0E+00	10	325	6.09E+03	90%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T03-C	1	3.53E+03			3.53E+03	5.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T04-C	1	3.52E+03			3.52E+03	2.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T05-C	1	3.66E+03			3.66E+03	4.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T06-C	1	3.76E+03			3.76E+03	6.9E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T07-C	1	3.94E+03			3.94E+03	3.2E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T08-C	1	2.43E+03			2.43E+03	5.6E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-T09-C	1	1.53E+03			1.53E+03	2.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-B01-A	1	2.78E+00	E		2.78E+00	5.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1313-B03-A	1	2.67E+00	E		2.67E+00	2.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	EaFA-L04-1313-T01-A	1	5.34E+00	E		5.34E+00	4.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00	10	325	3.31E+03	102%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T04-A	1	3.21E+00	E		3.21E+00	3.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T05-A	1	5.40E+01			5.40E+01	1.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T06-A	1	3.49E+02			3.49E+02	2.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T07-A	1	9.13E+02			9.13E+02	5.8E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T08-A	1	1.12E+03			1.12E+03	4.3E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T09-A	1	1.54E+03			1.54E+03	1.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00	10	325	3.51E+03	108%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T03-B	1	2.74E+00	E		2.74E+00	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T04-B	1	7.02E+00			7.02E+00	1.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T05-B	1	7.58E+01			7.58E+01	7.8E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T06-B	1	4.22E+02			4.22E+02	4.4E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T07-B	1	9.08E+02			9.08E+02	8.0E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T08-B	1	1.11E+03			1.11E+03	2.4E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T09-B	1	1.53E+03			1.53E+03	8.9E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	3.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	6.9E+01	2.0E+00	6.4E+00	10	325	3.29E+03	101%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T03-C	1	2.89E+00	E		2.89E+00	5.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T04-C	1	6.66E+00			6.66E+00	3.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T05-C	1	5.14E+01			5.14E+01	3.1E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T06-C	1	3.27E+02			3.27E+02	1.0E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T07-C	1	9.30E+02			9.30E+02	8.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T08-C	1	1.10E+03			1.10E+03	4.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-T09-C	1	1.52E+03			1.52E+03	7.4E-02	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-B02-A	1	2.29E+00	E		2.29E+00	1.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	2.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	EaFA-L04-1313-T01-A	1	4.84E+00			4.84E+00	6.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T02-A	1	2.83E+01			2.83E+01	2.2E+01	1.0E+00	3.2E+00	1000	100	1.01E+03	99%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T03-A	1	1.46E+02			1.46E+02	9.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T04-A	1	3.17E+03			3.17E+03	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T05-A	1	5.68E+03			5.68E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T06-A	1	7.79E+03			7.79E+03	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T07-A	1	8.23E+03			8.23E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T08-A	1	7.52E+03			7.52E+03	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T09-A	1	1.30E+04			1.30E+04	9.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T01-B	1	2.11E+00	E		2.11E+00	2.7E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T02-B	1	6.85E+01			6.85E+01	1.4E+01	1.0E+00	3.2E+00	1000	100	1.12E+03	105%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T03-B	1	4.16E+02			4.16E+02	2.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T04-B	1	3.73E+03			3.73E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T05-B	1	6.23E+03			6.23E+03	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T06-B	1	7.89E+03			7.89E+03	8.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T07-B	1	8.46E+03			8.46E+03	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T08-B	1	7.62E+03			7.62E+03	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T09-B	1	1.26E+04			1.26E+04	9.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T01-C	1	1.30E+01			1.30E+01	4.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T02-C	1	7.57E+01			7.57E+01	1.3E+01	1.0E+00	3.2E+00	1000	100	1.05E+03	98%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T03-C	1	4.68E+02			4.68E+02	2.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T04-C	1	3.63E+03			3.63E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T05-C	1	5.67E+03			5.67E+03	6.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T06-C	1	7.70E+03			7.70E+03	2.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T07-C	1	8.99E+03			8.99E+03	7.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T08-C	1	7.57E+03			7.57E+03	4.4E-02	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-T09-C	1	1.26E+04			1.26E+04	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-B01-A	1	6.59E+01			6.59E+01	8.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-B02-A	1	2.16E+02			2.16E+02	3.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1313-B03-A	1	1.91E+01			1.91E+01	5.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	EaFA-L04-1313-T01-A	1	4.25E+03			4.25E+03	3.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T02-A	1	3.99E+03			3.99E+03	2.7E-01	1.2E+00	3.8E+00	10	325	6.89E+03	89%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T03-A	1	4.01E+03			4.01E+03	4.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T04-A	1	3.90E+03			3.90E+03	3.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T05-A	1	3.67E+03			3.67E+03	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T06-A	1	3.28E+03			3.28E+03	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T07-A	1	3.52E+02			3.52E+02	1.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T08-A	1	1.24E+02			1.24E+02	3.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T09-A	1	2.43E+02			2.43E+02	5.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T01-B	1	4.16E+03			4.16E+03	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T02-B	1	4.10E+03			4.10E+03	8.9E-01	1.2E+00	3.8E+00	10	325	7.24E+03	97%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T03-B	1	4.02E+03			4.02E+03	1.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T04-B	1	3.85E+03			3.85E+03	1.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T05-B	1	3.68E+03			3.68E+03	3.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T06-B	1	3.25E+03			3.25E+03	1.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T07-B	1	3.30E+02			3.30E+02	9.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T08-B	1	1.21E+02			1.21E+02	8.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T09-B	1	2.10E+02			2.10E+02	1.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T01-C	1	4.23E+03			4.23E+03	6.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T02-C	1	4.02E+03			4.02E+03	5.5E-01	1.2E+00	3.8E+00	10	325	6.98E+03	91%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T03-C	1	3.99E+03			3.99E+03	2.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T04-C	1	3.77E+03			3.77E+03	1.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T05-C	1	3.59E+03			3.59E+03	4.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T06-C	1	3.25E+03			3.25E+03	5.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T07-C	1	6.49E+02			6.49E+02	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T08-C	1	1.12E+02			1.12E+02	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-T09-C	1	2.17E+02			2.17E+02	9.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-B01-A	1	7.57E+00			7.57E+00	3.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-B02-A	1	8.34E+00			8.34E+00	3.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1313-B03-A	1	1.05E+01			1.05E+01	3.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	EaFA-L04-1313-T01-A	1	4.25E+00	E		4.25E+00	1.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	8.7E+01	1.8E+00	5.7E+00	10	325	3.42E+03	105%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	1.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T04-A	1	3.09E+00	E		3.09E+00	5.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T05-A	1	1.39E+01			1.39E+01	3.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T06-A	1	1.04E+02			1.04E+02	8.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T07-A	1	6.07E+02			6.07E+02	1.9E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T08-A	1	5.06E+02			5.06E+02	7.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T09-A	1	7.08E+02			7.08E+02	6.4E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T01-B	1	5.55E+00	E		5.55E+00	8.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	5.4E+02	1.8E+00	5.7E+00	10	325	3.66E+03	112%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	8.9E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T04-B	1	3.06E+00	E		3.06E+00	6.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T05-B	1	1.80E+01			1.80E+01	2.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T06-B	1	1.35E+02			1.35E+02	3.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T07-B	1	6.07E+02			6.07E+02	3.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T08-B	1	5.14E+02			5.14E+02	1.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T09-B	1	7.00E+02			7.00E+02	1.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T01-C	1	7.37E+00			7.37E+00	5.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	7.4E+03	1.8E+00	5.7E+00	10	325	3.42E+03	105%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	1.8E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	3.2E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T05-C	1	1.41E+01			1.41E+01	9.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T06-C	1	9.50E+01			9.50E+01	1.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T07-C	1	5.91E+02			5.91E+02	6.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T08-C	1	5.13E+02			5.13E+02	6.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-T09-C	1	6.96E+02			6.96E+02	5.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	2.6E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	8.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1313-B03-A	1	4.73E+00	E		4.73E+00	3.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	EaFA-L04-1313-T01-A	1	1.45E+02			1.45E+02	3.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T02-A	1	6.04E+01			6.04E+01	3.4E+01	3.7E+00	1.2E+01	1000	100	1.07E+03	101%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T03-A	1	1.16E+01	E		1.16E+01	7.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T04-A	1	1.26E+02			1.26E+02	2.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T05-A	1	3.43E+01			3.43E+01	7.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T06-A	1	1.05E+02			1.05E+02	4.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T07-A	1	1.85E+00	U1/2		1.85E+00	2.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T08-A	1	4.95E+01			4.95E+01	1.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T09-A	1	1.61E+03			1.61E+03	4.2E-01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T01-B	1	2.11E+02			2.11E+02	1.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T02-B	1	9.07E+01			9.07E+01	9.8E+00	3.7E+00	1.2E+01	1000	100	1.21E+03	112%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T03-B	1	1.16E+02			1.16E+02	1.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T04-B	1	1.42E+02			1.42E+02	1.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T05-B	1	1.21E+02			1.21E+02	3.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T06-B	1	9.63E+01			9.63E+01	7.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T07-B	1	4.75E+01			4.75E+01	7.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T08-B	1	9.38E+01			9.38E+01	5.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T09-B	1	9.34E+02			9.34E+02	7.5E-01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T01-C	1	2.15E+02			2.15E+02	1.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T02-C	1	9.72E+01			9.72E+01	4.3E+01	3.7E+00	1.2E+01	1000	100	1.14E+03	104%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T03-C	1	1.02E+02			1.02E+02	8.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T04-C	1	1.63E+02			1.63E+02	6.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T05-C	1	9.89E+01			9.89E+01	2.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T06-C	1	8.47E+01			8.47E+01	1.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T07-C	1	8.71E+01			8.71E+01	3.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T08-C	1	8.18E+01			8.18E+01	1.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-T09-C	1	1.40E+03			1.40E+03	9.2E-02	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-B01-A	1	4.95E+01			4.95E+01	8.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-B02-A	1	1.58E+02			1.58E+02	3.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1313-B03-A	1	6.62E+01			6.62E+01	3.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	EaFA-L04-1313-T01-A	1	5.65E+04			5.65E+04	6.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T02-A	1	3.38E+04			3.38E+04	1.1E-01	1.6E+00	5.1E+00	1000	100	3.46E+04	85%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T03-A	1	2.72E+04			2.72E+04	4.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T04-A	1	2.59E+04			2.59E+04	1.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T05-A	1	2.54E+04			2.54E+04	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T06-A	1	2.44E+04			2.44E+04	7.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T07-A	1	2.46E+04			2.46E+04	4.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T08-A	1	1.74E+04			1.74E+04	2.3E-02	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T09-A	1	2.02E+04			2.02E+04	1.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T01-B	1	5.65E+04			5.65E+04	4.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T02-B	1	3.47E+04			3.47E+04	7.6E-01	1.6E+00	5.1E+00	1000	100	3.55E+04	84%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T03-B	1	2.70E+04			2.70E+04	9.1E-02	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T04-B	1	2.52E+04			2.52E+04	1.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T05-B	1	2.47E+04			2.47E+04	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T06-B	1	2.50E+04			2.50E+04	3.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T07-B	1	2.49E+04			2.49E+04	8.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T08-B	1	1.77E+04			1.77E+04	3.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T09-B	1	1.97E+04			1.97E+04	1.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T01-C	1	5.77E+04			5.77E+04	4.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T02-C	1	3.39E+04			3.39E+04	6.6E-01	1.6E+00	5.1E+00	1000	100	3.47E+04	81%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T03-C	1	2.71E+04			2.71E+04	3.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T04-C	1	2.52E+04			2.52E+04	1.4E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T05-C	1	2.46E+04			2.46E+04	6.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T06-C	1	2.44E+04			2.44E+04	8.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T07-C	1	2.64E+04			2.64E+04	6.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T08-C	1	1.78E+04			1.78E+04	4.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-T09-C	1	1.98E+04			1.98E+04	1.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-B01-A	1	1.61E+01			1.61E+01	1.5E+01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-B02-A	1	3.00E+01			3.00E+01	2.9E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1313-B03-A	1	2.57E+02			2.57E+02	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	EaFA-L04-1313-T01-A	1	8.20E+03			8.20E+03	1.5E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T02-A	1	6.49E+03			6.49E+03	4.8E-01	1.5E+01	4.8E+01	10	325	9.89E+03	105%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T03-A	1	5.76E+03			5.76E+03	4.7E-01	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T04-A	1	4.37E+03			4.37E+03	1.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T05-A	1	2.10E+03			2.10E+03	3.0E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T06-A	1	1.22E+03			1.22E+03	1.5E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T07-A	1	2.60E+02			2.60E+02	4.0E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T08-A	1	1.09E+02			1.09E+02	1.8E+01	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T09-A	1	4.53E+02			4.53E+02	3.5E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T01-B	1	8.25E+03			8.25E+03	4.9E-01	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T02-B	1	6.79E+03			6.79E+03	1.4E+00	1.5E+01	4.8E+01	10	325	1.05E+04	114%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T03-B	1	5.78E+03			5.78E+03	3.0E-01	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T04-B	1	3.85E+03			3.85E+03	2.4E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T05-B	1	2.05E+03			2.05E+03	1.8E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T06-B	1	1.17E+03			1.17E+03	2.6E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T07-B	1	2.89E+02			2.89E+02	4.2E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T08-B	1	1.16E+02			1.16E+02	1.6E+01	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T09-B	1	3.06E+02			3.06E+02	3.5E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T01-C	1	8.43E+03			8.43E+03	4.0E-01	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T02-C	1	6.64E+03			6.64E+03	7.7E-01	1.5E+01	4.8E+01	10	325	1.01E+04	106%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T03-C	1	5.85E+03			5.85E+03	1.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T04-C	1	3.85E+03			3.85E+03	1.2E-01	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T05-C	1	2.05E+03			2.05E+03	2.2E-01	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T06-C	1	1.22E+03			1.22E+03	1.9E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T07-C	1	3.58E+02			3.58E+02	5.3E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T08-C	1	1.14E+02			1.14E+02	1.7E+01	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-T09-C	1	4.09E+02			4.09E+02	6.3E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-B01-A	1	7.50E+00	U1/2		7.50E+00	3.0E+03	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-B02-A	1	7.50E+00	U1/2		7.50E+00	9.0E+01	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1313-B03-A	1	8.90E+01			8.90E+01	4.2E+01	1.5E+01	4.8E+01			---		VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	EaFA-L04-1313-T01-A	1	1.73E+04			1.73E+04	3.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T02-A	1	4.07E+03			4.07E+03	3.6E-01	1.1E+00	3.5E+00	1000	100	4.93E+03	86%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T03-A	1	9.44E+02			9.44E+02	6.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T04-A	1	3.72E+02			3.72E+02	4.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T05-A	1	8.21E+02			8.21E+02	6.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T06-A	1	2.15E+03			2.15E+03	7.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T07-A	1	7.57E+03			7.57E+03	1.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T08-A	1	2.27E+04			2.27E+04	6.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T09-A	1	6.30E+04			6.30E+04	1.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T01-B	1	1.63E+04			1.63E+04	3.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T02-B	1	4.27E+03			4.27E+03	1.0E-01	1.1E+00	3.5E+00	1000	100	5.16E+03	89%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T03-B	1	9.70E+02			9.70E+02	5.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T04-B	1	3.99E+02			3.99E+02	1.7E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T05-B	1	9.80E+02			9.80E+02	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T06-B	1	2.54E+03			2.54E+03	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T07-B	1	7.75E+03			7.75E+03	2.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T08-B	1	2.09E+04			2.09E+04	1.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T09-B	1	6.24E+04			6.24E+04	5.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T01-C	1	1.74E+04			1.74E+04	2.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T02-C	1	4.16E+03			4.16E+03	6.1E-01	1.1E+00	3.5E+00	1000	100	5.01E+03	85%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T03-C	1	7.59E+02			7.59E+02	1.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T04-C	1	3.81E+02			3.81E+02	3.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T05-C	1	7.43E+02			7.43E+02	8.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T06-C	1	2.06E+03			2.06E+03	8.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T07-C	1	7.27E+03			7.27E+03	3.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T08-C	1	2.06E+04			2.06E+04	3.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-T09-C	1	6.22E+04			6.22E+04	4.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-B01-A	1	4.38E+01			4.38E+01	5.8E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-B02-A	1	4.29E+01			4.29E+01	4.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1313-B03-A	1	6.34E+01			6.34E+01	1.6E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	EaFA-L04-1313-T01-A	1	3.68E+05			3.68E+05	3.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T02-A	1	1.56E+05			1.56E+05	2.6E-01	2.5E+00	8.0E+00	1000	100	1.57E+05	89%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T03-A	1	5.66E+04			5.66E+04	1.6E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T04-A	1	3.54E+04			3.54E+04	6.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T05-A	1	1.56E+04			1.56E+04	3.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T06-A	1	5.45E+03			5.45E+03	7.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T07-A	1	5.20E+03			5.20E+03	2.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T08-A	1	3.42E+03			3.42E+03	5.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T09-A	1	2.74E+03			2.74E+03	7.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T01-B	1	3.67E+05			3.67E+05	8.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T02-B	1	1.54E+05			1.54E+05	5.7E-01	2.5E+00	8.0E+00	1000	100	1.55E+05	85%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T03-B	1	5.55E+04			5.55E+04	8.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T04-B	1	2.93E+04			2.93E+04	8.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T05-B	1	1.51E+04			1.51E+04	1.5E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T06-B	1	5.50E+03			5.50E+03	6.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T07-B	1	5.43E+03			5.43E+03	3.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T08-B	1	3.62E+03			3.62E+03	5.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T09-B	1	2.62E+03			2.62E+03	2.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T01-C	1	3.66E+05			3.66E+05	4.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T02-C	1	1.44E+05			1.44E+05	6.2E-01	2.5E+00	8.0E+00	1000	100	1.45E+05	87%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T03-C	1	5.29E+04			5.29E+04	6.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T04-C	1	2.93E+04			2.93E+04	3.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T05-C	1	1.50E+04			1.50E+04	2.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T06-C	1	5.46E+03			5.46E+03	1.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T07-C	1	5.74E+03			5.74E+03	3.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T08-C	1	3.70E+03			3.70E+03	8.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-T09-C	1	2.73E+03			2.73E+03	2.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-B01-A	1	3.35E+01			3.35E+01	7.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-B02-A	1	9.02E+01			9.02E+01	9.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1313-B03-A	1	3.72E+05			3.72E+05	1.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	EaFA-L04-1313-T01-A	1	1.38E+03			1.38E+03	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T02-A	1	1.48E+03			1.48E+03	1.0E+00	1.0E+00	3.2E+00	1000	100	2.31E+03	83%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T03-A	1	1.76E+03			1.76E+03	9.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T04-A	1	1.96E+03			1.96E+03	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T05-A	1	2.10E+03			2.10E+03	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T06-A	1	2.17E+03			2.17E+03	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T07-A	1	2.63E+03			2.63E+03	2.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T08-A	1	2.99E+03			2.99E+03	8.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T09-A	1	4.68E+03			4.68E+03	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T01-B	1	1.35E+03			1.35E+03	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T02-B	1	1.42E+03			1.42E+03	4.1E-01	1.0E+00	3.2E+00	1000	100	2.34E+03	92%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T03-B	1	1.74E+03			1.74E+03	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T04-B	1	1.90E+03			1.90E+03	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T05-B	1	2.02E+03			2.02E+03	3.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T06-B	1	2.20E+03			2.20E+03	2.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T07-B	1	2.63E+03			2.63E+03	5.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T08-B	1	2.90E+03			2.90E+03	1.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T09-B	1	4.58E+03			4.58E+03	9.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T01-C	1	1.32E+03			1.32E+03	2.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T02-C	1	1.42E+03			1.42E+03	6.7E-01	1.0E+00	3.2E+00	1000	100	2.28E+03	86%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T03-C	1	1.75E+03			1.75E+03	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T04-C	1	1.87E+03			1.87E+03	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T05-C	1	2.02E+03			2.02E+03	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T06-C	1	2.21E+03			2.21E+03	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T07-C	1	2.72E+03			2.72E+03	3.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T08-C	1	2.93E+03			2.93E+03	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-T09-C	1	4.60E+03			4.60E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-B01-A	1	1.39E+00	E		1.39E+00	4.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-B02-A	1	5.17E+00			5.17E+00	1.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1313-B03-A	1	4.84E+00			4.84E+00	1.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	EaFA-L04-1313-T01-A	1	3.22E+06			3.22E+06	7.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T02-A	1	2.89E+06			2.89E+06	2.1E-01	6.8E+00	2.2E+01	1000	500	2.90E+06	87%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T03-A	1	2.76E+06			2.76E+06	3.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T04-A	1	2.75E+06			2.75E+06	3.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T05-A	1	2.55E+06			2.55E+06	1.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T06-A	1	2.70E+06			2.70E+06	1.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T07-A	1	2.35E+06			2.35E+06	3.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T08-A	1	1.56E+06			1.56E+06	8.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T09-A	1	9.17E+05			9.17E+05	9.3E-02	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T01-B	1	3.23E+06			3.23E+06	1.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T02-B	1	2.82E+06			2.82E+06	6.3E-01	6.8E+00	2.2E+01	1000	500	2.82E+06	87%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T03-B	1	2.75E+06			2.75E+06	2.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T04-B	1	2.72E+06			2.72E+06	1.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T05-B	1	2.61E+06			2.61E+06	9.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T06-B	1	2.70E+06			2.70E+06	7.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T07-B	1	2.35E+06			2.35E+06	3.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T08-B	1	1.60E+06			1.60E+06	7.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T09-B	1	8.98E+05			8.98E+05	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T01-C	1	3.12E+06			3.12E+06	3.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T02-C	1	2.64E+06			2.64E+06	1.1E+00	6.8E+00	2.2E+01	1000	500	2.65E+06	81%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T03-C	1	2.71E+06			2.71E+06	3.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T04-C	1	2.62E+06			2.62E+06	4.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T05-C	1	2.61E+06			2.61E+06	3.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T06-C	1	2.55E+06			2.55E+06	7.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T07-C	1	2.54E+06			2.54E+06	4.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T08-C	1	1.60E+06			1.60E+06	8.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-T09-C	1	8.89E+05			8.89E+05	6.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-B01-A	1	2.56E+06			2.56E+06	4.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-B02-A	1	2.54E+06			2.54E+06	1.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1313-B03-A	1	3.18E+06			3.18E+06	1.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	EaFA-L04-1313-T01-A	1	1.36E+01	E		1.36E+01	4.6E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T02-A	1	2.30E+00	U1/2		2.30E+00	2.9E+02	4.6E+00	1.5E+01	10	325	3.16E+03	97%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T03-A	1	2.30E+00	U1/2		2.30E+00	1.1E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T04-A	1	2.30E+00	U1/2		2.30E+00	2.4E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T05-A	1	2.30E+00	U1/2		2.30E+00	5.6E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T06-A	1	2.30E+00	U1/2		2.30E+00	6.2E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T07-A	1	3.34E+01			3.34E+01	6.8E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T08-A	1	4.92E+01			4.92E+01	1.1E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T09-A	1	6.67E+01			6.67E+01	8.0E+00	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T01-B	1	1.77E+01			1.77E+01	1.0E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T02-B	1	1.39E+01	E		1.39E+01	6.9E+01	4.6E+00	1.5E+01	10	325	3.37E+03	103%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T03-B	1	2.30E+00	U1/2		2.30E+00	3.0E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T04-B	1	2.30E+00	U1/2		2.30E+00	5.3E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T05-B	1	2.30E+00	U1/2		2.30E+00	2.3E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T06-B	1	2.30E+00	U1/2		2.30E+00	3.8E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T07-B	1	3.46E+01			3.46E+01	1.5E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T08-B	1	4.88E+01			4.88E+01	1.4E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T09-B	1	6.72E+01			6.72E+01	8.6E+00	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T01-C	1	1.25E+01	E		1.25E+01	1.1E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T02-C	1	2.30E+00	U1/2		2.30E+00	4.8E+02	4.6E+00	1.5E+01	10	325	3.20E+03	98%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T03-C	1	2.30E+00	U1/2		2.30E+00	2.3E+04	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T04-C	1	2.30E+00	U1/2		2.30E+00	8.3E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T05-C	1	2.30E+00	U1/2		2.30E+00	3.7E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T06-C	1	2.30E+00	U1/2		2.30E+00	1.6E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T07-C	1	2.92E+01			2.92E+01	8.0E+00	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T08-C	1	4.52E+01			4.52E+01	4.6E+00	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-T09-C	1	6.87E+01			6.87E+01	1.7E+00	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	3.5E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	7.7E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	5.7E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	EaFA-L04-1313-T01-A	1	4.22E+00	E		4.22E+00	3.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	7.9E+01	2.0E+00	6.4E+00	10	325	3.06E+03	94%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	1.6E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	3.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	6.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	7.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T08-A	1	1.59E+01			1.59E+01	5.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T09-A	1	1.83E+03			1.83E+03	7.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T01-B	1	2.28E+00	E		2.28E+00	2.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	6.0E+01	2.0E+00	6.4E+00	10	325	3.24E+03	100%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	1.5E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	1.0E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	1.0E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	8.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T07-B	1	1.57E+01			1.57E+01	5.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T08-B	1	1.19E+01			1.19E+01	4.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T09-B	1	1.05E+03			1.05E+03	4.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T01-C	1	2.16E+00	E		2.16E+00	5.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	7.0E+01	2.0E+00	6.4E+00	10	325	3.04E+03	94%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	6.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	7.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	8.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	1.7E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	2.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T08-C	1	1.06E+01			1.06E+01	4.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-T09-C	1	1.51E+03			1.51E+03	2.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1313-B03-A	1	2.18E+00	E		2.18E+00	1.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	EaFA-L04-1313-T01-A	1	5.79E+03			5.79E+03	3.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T02-A	1	2.82E+03			2.82E+03	2.9E-01	1.5E+00	4.8E+00	10	325	5.95E+03	96%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T03-A	1	2.51E+03			2.51E+03	8.2E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T04-A	1	9.08E+02			9.08E+02	6.9E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T05-A	1	3.22E+02			3.22E+02	2.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T06-A	1	2.30E+02			2.30E+02	2.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T07-A	1	8.83E+01			8.83E+01	5.9E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T08-A	1	9.64E+01			9.64E+01	1.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T09-A	1	5.45E+03			5.45E+03	5.4E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T01-B	1	5.55E+03			5.55E+03	6.2E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T02-B	1	2.88E+03			2.88E+03	3.9E-01	1.5E+00	4.8E+00	10	325	6.23E+03	103%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T03-B	1	2.50E+03			2.50E+03	1.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T04-B	1	6.77E+02			6.77E+02	4.9E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T05-B	1	3.29E+02			3.29E+02	1.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T06-B	1	2.30E+02			2.30E+02	4.8E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T07-B	1	8.62E+01			8.62E+01	1.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T08-B	1	8.91E+01			8.91E+01	3.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T09-B	1	5.16E+03			5.16E+03	4.9E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T01-C	1	5.72E+03			5.72E+03	6.2E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T02-C	1	2.88E+03			2.88E+03	1.2E+00	1.5E+00	4.8E+00	10	325	6.02E+03	97%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T03-C	1	2.26E+03			2.26E+03	4.8E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T04-C	1	6.31E+02			6.31E+02	4.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T05-C	1	2.96E+02			2.96E+02	9.1E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T06-C	1	2.24E+02			2.24E+02	1.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T07-C	1	1.03E+02			1.03E+02	2.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T08-C	1	8.33E+01			8.33E+01	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-T09-C	1	5.34E+03			5.34E+03	3.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-B01-A	1	7.50E-01	U1/2		7.50E-01	2.3E+01	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-B02-A	1	2.60E+00	E		2.60E+00	3.4E+01	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1313-B03-A	1	3.96E+00	E		3.96E+00	5.9E+01	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	EaFA-L04-1313-T01-A	1	2.29E+02			2.29E+02	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:09 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T02-A	1	2.87E+00	E		2.87E+00	3.5E+01	1.0E+00	3.2E+00	10	325	3.51E+03	108%	VU ICP-OES	6/24/10 11:10 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T03-A	1	5.00E-01	U1/2		5.00E-01	3.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:12 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T04-A	1	5.00E-01	U1/2		5.00E-01	2.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:13 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T05-A	1	5.00E-01	U1/2		5.00E-01	1.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:15 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T06-A	1	1.38E+01			1.38E+01	5.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:17 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T07-A	1	1.26E+03			1.26E+03	7.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:18 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T08-A	1	1.10E+03			1.10E+03	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:20 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T09-A	1	1.47E+03			1.47E+03	2.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:22 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T01-B	1	1.72E+02			1.72E+02	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:32 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T02-B	1	7.44E+00			7.44E+00	1.4E+01	1.0E+00	3.2E+00	10	325	3.75E+03	115%	VU ICP-OES	6/24/10 11:33 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T03-B	1	2.55E+00	E		2.55E+00	1.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:35 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T04-B	1	5.00E-01	U1/2		5.00E-01	8.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:36 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T05-B	1	3.97E+00			3.97E+00	2.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:38 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T06-B	1	1.83E+01			1.83E+01	3.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:40 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T07-B	1	1.26E+03			1.26E+03	6.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:41 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T08-B	1	1.12E+03			1.12E+03	5.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:43 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T09-B	1	1.44E+03			1.44E+03	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:45 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T01-C	1	1.44E+02			1.44E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:50 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T02-C	1	6.90E+00			6.90E+00	7.6E+00	1.0E+00	3.2E+00	10	325	3.52E+03	108%	VU ICP-OES	6/24/10 11:51 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T03-C	1	6.04E+00			6.04E+00	1.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:53 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T04-C	1	5.00E-01	U1/2		5.00E-01	8.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:55 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T05-C	1	3.15E+00	E		3.15E+00	8.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:56 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T06-C	1	1.39E+01			1.39E+01	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:58 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T07-C	1	1.09E+03			1.09E+03	6.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:59 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T08-C	1	1.12E+03			1.12E+03	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:01 PM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-T09-C	1	1.44E+03			1.44E+03	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:03 PM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	2.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:04 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-B02-A	1	1.15E+01			1.15E+01	8.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:05 AM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1313-B03-A	1	1.34E+01			1.34E+01	3.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 11:07 AM	EPA Interlab L04 1313-1316 EaFA

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	EaFA-L05-1313-T01-A	1	3.46E+04			3.46E+04	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T02-A	1	2.88E+04			2.88E+04	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T03-A	1	2.08E+04			2.08E+04	4.5E-01	1.0E+00	3.2E+00	1000	100	2.17E+04	92%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T04-A	1	8.07E+03			8.07E+03	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T05-A	1	3.45E+02			3.45E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T06-A	1	7.57E+01			7.57E+01	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T07-A	1	7.49E+01			7.49E+01	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T08-A	1	4.07E+04			4.07E+04	3.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T09-A	1	1.05E+05			1.05E+05	8.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T01-B	1	3.21E+04			3.21E+04	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T02-B	1	3.00E+04			3.00E+04	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T03-B	1	2.12E+04			2.12E+04	4.2E-01	1.0E+00	3.2E+00	1000	100	2.20E+04	88%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T04-B	1	9.00E+03			9.00E+03	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T05-B	1	4.13E+02			4.13E+02	2.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T06-B	1	7.34E+01			7.34E+01	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T07-B	1	1.49E+02			1.49E+02	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T08-B	1	4.19E+04			4.19E+04	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T09-B	1	1.13E+05			1.13E+05	6.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T01-C	1	3.47E+04			3.47E+04	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T02-C	1	3.12E+04			3.12E+04	8.0E-02	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T03-C	1	2.39E+04			2.39E+04	3.9E-01	1.0E+00	3.2E+00	1000	100	2.49E+04	101%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T04-C	1	8.18E+03			8.18E+03	5.2E-01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T05-C	1	2.10E+02			2.10E+02	9.9E-01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T06-C	1	3.29E+02			3.29E+02	1.4E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T07-C	1	7.48E+01			7.48E+01	4.5E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T08-C	1	3.98E+04			3.98E+04	6.9E-01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-T09-C	1	1.10E+05			1.10E+05	8.8E-01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	6.8E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	7.9E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	2.7E+02	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	2.2E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	1.6E+02	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	4.7E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	2.1E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	3.9E+02	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	6.8E+02	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	EaFA-L05-1313-T01-A	1	1.78E+02			1.78E+02	6.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T02-A	1	1.29E+02			1.29E+02	2.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T03-A	1	1.47E+02			1.47E+02	5.9E+00	7.5E+00	2.4E+01	10	325	3.20E+03	94%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T04-A	1	1.73E+02			1.73E+02	9.4E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T05-A	1	1.92E+02			1.92E+02	1.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T06-A	1	1.28E+02			1.28E+02	1.4E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T07-A	1	1.52E+02			1.52E+02	2.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T08-A	1	2.74E+01			2.74E+01	3.8E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T09-A	1	9.59E+00	E		9.59E+00	4.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T01-B	1	1.77E+02			1.77E+02	1.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T02-B	1	1.40E+02			1.40E+02	3.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T03-B	1	1.45E+02			1.45E+02	6.0E+00	7.5E+00	2.4E+01	10	325	3.29E+03	97%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T04-B	1	1.59E+02			1.59E+02	1.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T05-B	1	1.49E+02			1.49E+02	2.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T06-B	1	1.52E+02			1.52E+02	1.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T07-B	1	1.14E+02			1.14E+02	1.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T08-B	1	4.60E+01			4.60E+01	2.5E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T09-B	1	3.75E+00	U1/2		3.75E+00	1.4E+02	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T01-C	1	2.00E+02			2.00E+02	5.9E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T02-C	1	1.49E+02			1.49E+02	3.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T03-C	1	1.95E+02			1.95E+02	8.5E+00	7.5E+00	2.4E+01	10	325	3.37E+03	98%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T04-C	1	1.40E+02			1.40E+02	7.0E+00	7.5E+00	2.4E+01					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T05-C	1	1.47E+02			1.47E+02	1.7E+01	7.5E+00	2.4E+01					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T06-C	1	1.24E+02			1.24E+02	4.6E+00	7.5E+00	2.4E+01					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T07-C	1	1.58E+02			1.58E+02	8.6E+00	7.5E+00	2.4E+01					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T08-C	1	1.88E+01	E		1.88E+01	6.0E+01	7.5E+00	2.4E+01					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-T09-C	1	3.75E+00	U1/2		3.75E+00	1.7E+02	7.5E+00	2.4E+01					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-B01-A	1	1.77E+01	E		1.77E+01	7.6E+01	7.5E+00	2.4E+01					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-B02-A	1	3.75E+00	U1/2		3.75E+00	1.3E+02	7.5E+00	2.4E+01					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-B03-A	1	3.75E+00	U1/2		3.75E+00	6.0E+01	7.5E+00	2.4E+01					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-B01-B	1	1.75E+01	E		1.75E+01	2.2E+01	7.5E+00	2.4E+01					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-B02-B	1	3.75E+00	U1/2		3.75E+00	1.1E+02	7.5E+00	2.4E+01					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-B03-B	1	3.75E+00	U1/2		3.75E+00	2.7E+02	7.5E+00	2.4E+01					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-B01-C	1	7.55E+00	E		7.55E+00	6.7E+01	7.5E+00	2.4E+01					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-B02-C	1	3.75E+00	U1/2		3.75E+00	1.1E+02	7.5E+00	2.4E+01					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1313-B03-C	1	3.75E+00	U1/2		3.75E+00	3.7E+01	7.5E+00	2.4E+01					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	EaFA-L05-1313-T01-A	1	6.57E+03			6.57E+03	8.9E-01	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T02-A	1	9.06E+02			9.06E+02	1.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T03-A	1	8.52E+02			8.52E+02	3.4E+00	1.1E+01	3.5E+01	10	325	3.86E+03	93%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T04-A	1	4.68E+02			4.68E+02	3.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T05-A	1	1.76E+02			1.76E+02	6.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T06-A	1	8.16E+01			8.16E+01	1.8E+01	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T07-A	1	1.07E+02			1.07E+02	6.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T08-A	1	1.51E+02			1.51E+02	8.2E-01	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T09-A	1	3.57E+03			3.57E+03	9.9E-01	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T01-B	1	7.33E+03			7.33E+03	4.4E-01	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T02-B	1	9.08E+02			9.08E+02	2.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T03-B	1	1.18E+03			1.18E+03	1.0E+00	1.1E+01	3.5E+01	10	325	4.14E+03	91%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T04-B	1	4.33E+02			4.33E+02	4.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T05-B	1	1.53E+02			1.53E+02	1.5E+01	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T06-B	1	9.86E+01			9.86E+01	2.1E+01	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T07-B	1	9.81E+01			9.81E+01	2.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T08-B	1	1.40E+02			1.40E+02	1.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T09-B	1	3.71E+03			3.71E+03	3.2E-01	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T01-C	1	7.55E+03			7.55E+03	5.1E-01	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T02-C	1	8.93E+02			8.93E+02	6.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T03-C	1	1.35E+03			1.35E+03	1.8E+00	1.1E+01	3.5E+01	10	325	4.38E+03	93%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T04-C	1	4.79E+02			4.79E+02	2.6E-01	1.1E+01	3.5E+01					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T05-C	1	1.15E+02			1.15E+02	5.3E+00	1.1E+01	3.5E+01					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T06-C	1	1.10E+02			1.10E+02	1.3E+01	1.1E+01	3.5E+01					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T07-C	1	1.11E+02			1.11E+02	8.4E+00	1.1E+01	3.5E+01					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T08-C	1	1.37E+02			1.37E+02	6.2E+00	1.1E+01	3.5E+01					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-T09-C	1	3.89E+03			3.89E+03	3.7E-01	1.1E+01	3.5E+01					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-B01-A	1	3.84E+01			3.84E+01	3.2E+01	1.1E+01	3.5E+01					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-B02-A	1	3.34E+01	E		3.34E+01	6.2E+01	1.1E+01	3.5E+01					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-B03-A	1	5.80E+01			5.80E+01	3.4E+01	1.1E+01	3.5E+01					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-B01-B	1	4.36E+01			4.36E+01	3.4E+01	1.1E+01	3.5E+01					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-B02-B	1	3.57E+01			3.57E+01	6.4E+01	1.1E+01	3.5E+01					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-B03-B	1	4.67E+01			4.67E+01	4.0E+01	1.1E+01	3.5E+01					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-B01-C	1	3.32E+01	E		3.32E+01	3.6E+01	1.1E+01	3.5E+01					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-B02-C	1	2.34E+01	E		2.34E+01	5.0E+01	1.1E+01	3.5E+01					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1313-B03-C	1	2.94E+01	E		2.94E+01	3.4E+01	1.1E+01	3.5E+01					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	EaFA-L05-1313-T01-A	1	4.69E+03			4.69E+03	3.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T02-A	1	4.52E+03			4.52E+03	2.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T03-A	1	3.93E+03			3.93E+03	2.7E+00	1.0E+00	3.2E+00	1000	100	4.79E+03	86%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T04-A	1	4.42E+03			4.42E+03	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T05-A	1	4.58E+03			4.58E+03	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T06-A	1	4.91E+03			4.91E+03	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T07-A	1	4.96E+03			4.96E+03	6.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T08-A	1	3.79E+03			3.79E+03	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T09-A	1	3.06E+03			3.06E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T01-B	1	4.51E+03			4.51E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T02-B	1	4.37E+03			4.37E+03	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T03-B	1	4.32E+03			4.32E+03	2.3E+00	1.0E+00	3.2E+00	1000	100	5.29E+03	97%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T04-B	1	4.22E+03			4.22E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T05-B	1	4.42E+03			4.42E+03	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T06-B	1	4.71E+03			4.71E+03	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T07-B	1	4.78E+03			4.78E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T08-B	1	3.74E+03			3.74E+03	7.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T09-B	1	2.92E+03			2.92E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T01-C	1	4.51E+03			4.51E+03	9.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T02-C	1	4.36E+03			4.36E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T03-C	1	4.31E+03			4.31E+03	6.5E-01	1.0E+00	3.2E+00	1000	100	5.18E+03	87%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T04-C	1	4.26E+03			4.26E+03	1.9E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T05-C	1	4.31E+03			4.31E+03	8.5E-01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T06-C	1	4.66E+03			4.66E+03	1.3E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T07-C	1	4.59E+03			4.59E+03	3.3E-01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T08-C	1	3.65E+03			3.65E+03	1.8E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-T09-C	1	2.94E+03			2.94E+03	5.9E-01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.7E+02	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	5.2E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	4.4E-01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	1.6E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	9.1E-01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	3.1E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	EaFA-L05-1313-T01-A	1	1.55E+03			1.55E+03	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T02-A	1	9.93E+02			9.93E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T03-A	1	8.75E+02			8.75E+02	3.9E-01	1.0E+00	3.2E+00	10	325	3.84E+03	91%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T04-A	1	5.75E+02			5.75E+02	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T05-A	1	3.67E+02			3.67E+02	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T06-A	1	3.16E+02			3.16E+02	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T07-A	1	3.27E+02			3.27E+02	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T08-A	1	3.38E+02			3.38E+02	2.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T09-A	1	9.94E+02			9.94E+02	2.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T01-B	1	1.28E+03			1.28E+03	4.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T02-B	1	1.04E+03			1.04E+03	3.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T03-B	1	7.77E+02			7.77E+02	4.4E-01	1.0E+00	3.2E+00	10	325	3.80E+03	93%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T04-B	1	6.28E+02			6.28E+02	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T05-B	1	3.93E+02			3.93E+02	6.8E-02	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T06-B	1	3.27E+02			3.27E+02	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T07-B	1	3.68E+02			3.68E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T08-B	1	3.30E+02			3.30E+02	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T09-B	1	9.93E+02			9.93E+02	8.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T01-C	1	1.33E+03			1.33E+03	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T02-C	1	9.54E+02			9.54E+02	1.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T03-C	1	9.55E+02			9.55E+02	4.8E-01	1.0E+00	3.2E+00	10	325	3.91E+03	91%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T04-C	1	5.14E+02			5.14E+02	3.3E-01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T05-C	1	3.87E+02			3.87E+02	5.3E-01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T06-C	1	3.38E+02			3.38E+02	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T07-C	1	3.46E+02			3.46E+02	8.2E-01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T08-C	1	3.36E+02			3.36E+02	4.5E-01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-T09-C	1	9.50E+02			9.50E+02	3.6E-01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	8.0E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-B02-A	1	2.11E+00	E		2.11E+00	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-B03-A	1	1.11E+00	E		1.11E+00	9.9E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	2.7E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	5.7E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-B03-B	1	1.15E+00	E		1.15E+00	1.3E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	3.5E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	9.4E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1313-B03-C	1	1.32E+00	E		1.32E+00	1.9E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	EaFA-L05-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	1.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	1.7E+02	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	4.3E+01	1.9E+00	6.0E+00	10	325	3.21E+03	99%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	8.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	3.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T07-A	1	9.50E-01	U1/2		9.50E-01	3.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T08-A	1	1.45E+02			1.45E+02	2.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T09-A	1	2.39E+02			2.39E+02	9.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	8.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	2.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00	10	325	3.27E+03	100%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	1.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	1.9E+02	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	3.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T07-B	1	1.98E+00	E		1.98E+00	5.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T08-B	1	1.47E+02			1.47E+02	7.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T09-B	1	2.48E+02			2.48E+02	5.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	4.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	7.6E+03	1.9E+00	6.0E+00	10	325	3.39E+03	104%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	3.2E+02	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	2.4E+02	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T06-C	1	4.80E+00	E		4.80E+00	1.4E+01	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T07-C	1	9.50E-01	U1/2		9.50E-01	1.6E+01	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T08-C	1	1.47E+02			1.47E+02	7.4E-01	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-T09-C	1	2.47E+02			2.47E+02	1.0E+00	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	2.1E+01	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	5.1E+01	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-B01-B	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-B02-B	1	9.50E-01	U1/2		9.50E-01	1.0E+02	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-B03-B	1	9.50E-01	U1/2		9.50E-01	1.7E+01	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-B01-C	1	9.50E-01	U1/2		9.50E-01	1.2E+03	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-B02-C	1	9.50E-01	U1/2		9.50E-01	2.6E+02	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1313-B03-C	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	EaFA-L05-1313-T01-A	1	1.10E+00	U1/2		1.10E+00	2.2E+02	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T02-A	1	1.10E+00	U1/2		1.10E+00	2.0E+02	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	3.3E+01	2.2E+00	7.0E+00	10	325	3.17E+03	97%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T04-A	1	1.10E+00	U1/2		1.10E+00	3.0E+02	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T05-A	1	1.10E+00	U1/2		1.10E+00	3.5E+01	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T06-A	1	1.09E+01			1.09E+01	9.2E-01	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T07-A	1	1.47E+01			1.47E+01	3.9E+00	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T08-A	1	3.04E+01			3.04E+01	1.3E+00	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T09-A	1	3.39E+01			3.39E+01	1.4E+00	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T01-B	1	1.10E+00	U1/2		1.10E+00	1.2E+02	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T02-B	1	1.10E+00	U1/2		1.10E+00	4.0E+02	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	3.2E+01	2.2E+00	7.0E+00	10	325	3.28E+03	101%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T04-B	1	1.10E+00	U1/2		1.10E+00	5.0E+01	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T05-B	1	1.10E+00	U1/2		1.10E+00	3.8E+03	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T06-B	1	8.11E+00			8.11E+00	5.2E+00	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T07-B	1	2.16E+01			2.16E+01	7.5E-01	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T08-B	1	3.07E+01			3.07E+01	1.5E+00	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T09-B	1	3.49E+01			3.49E+01	1.1E+00	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T01-C	1	1.10E+00	U1/2		1.10E+00	2.9E+02	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T02-C	1	1.10E+00	U1/2		1.10E+00	1.5E+03	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	5.0E+01	2.2E+00	7.0E+00	10	325	3.37E+03	104%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T04-C	1	1.10E+00	U1/2		1.10E+00	3.5E+01	2.2E+00	7.0E+00					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T05-C	1	1.10E+00	U1/2		1.10E+00	3.6E+01	2.2E+00	7.0E+00					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T06-C	1	2.36E+01			2.36E+01	1.1E+01	2.2E+00	7.0E+00					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T07-C	1	7.96E+00			7.96E+00	2.8E+00	2.2E+00	7.0E+00					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T08-C	1	3.14E+01			3.14E+01	1.1E+00	2.2E+00	7.0E+00					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-T09-C	1	3.53E+01			3.53E+01	1.6E+00	2.2E+00	7.0E+00					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	2.1E+01	2.2E+00	7.0E+00					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	5.8E+01	2.2E+00	7.0E+00					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-B03-A	1	1.10E+00	U1/2		1.10E+00	5.6E+02	2.2E+00	7.0E+00					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-B01-B	1	1.10E+00	U1/2		1.10E+00	1.0E+02	2.2E+00	7.0E+00					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-B02-B	1	1.10E+00	U1/2		1.10E+00	3.1E+02	2.2E+00	7.0E+00					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-B03-B	1	1.10E+00	U1/2		1.10E+00	8.2E+01	2.2E+00	7.0E+00					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-B01-C	1	1.10E+00	U1/2		1.10E+00	4.5E+01	2.2E+00	7.0E+00					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-B02-C	1	1.10E+00	U1/2		1.10E+00	1.7E+02	2.2E+00	7.0E+00					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1313-B03-C	1	1.10E+00	U1/2		1.10E+00	1.3E+02	2.2E+00	7.0E+00					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	EaFA-L05-1313-T01-A	1	1.62E+04			1.62E+04	4.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T02-A	1	5.20E+04			5.20E+04	6.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T03-A	1	8.24E+04			8.24E+04	9.5E-02	2.6E+00	8.3E+00	1000	100	8.32E+04	85%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T04-A	1	1.16E+05			1.16E+05	7.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T05-A	1	1.40E+05			1.40E+05	1.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T06-A	1	1.58E+05			1.58E+05	1.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T07-A	1	1.61E+05			1.61E+05	5.5E-02	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T08-A	1	1.40E+05			1.40E+05	5.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T09-A	1	1.33E+05			1.33E+05	6.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T01-B	1	1.41E+04			1.41E+04	5.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T02-B	1	5.27E+04			5.27E+04	5.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T03-B	1	8.45E+04			8.45E+04	5.7E-01	2.6E+00	8.3E+00	1000	100	8.53E+04	86%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T04-B	1	1.11E+05			1.11E+05	7.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T05-B	1	1.29E+05			1.29E+05	2.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T06-B	1	1.57E+05			1.57E+05	9.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T07-B	1	1.56E+05			1.56E+05	1.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T08-B	1	1.38E+05			1.38E+05	2.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T09-B	1	1.33E+05			1.33E+05	1.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T01-C	1	1.43E+04			1.43E+04	5.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T02-C	1	5.16E+04			5.16E+04	3.6E-02	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T03-C	1	8.58E+04			8.58E+04	4.7E-01	2.6E+00	8.3E+00	1000	100	8.66E+04	86%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T04-C	1	1.19E+05			1.19E+05	4.3E-01	2.6E+00	8.3E+00					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T05-C	1	1.35E+05			1.35E+05	3.7E-01	2.6E+00	8.3E+00					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T06-C	1	1.55E+05			1.55E+05	1.1E+01	2.6E+00	8.3E+00					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T07-C	1	1.57E+05			1.57E+05	6.6E-01	2.6E+00	8.3E+00					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T08-C	1	1.41E+05			1.41E+05	5.5E-01	2.6E+00	8.3E+00					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-T09-C	1	1.35E+05			1.35E+05	7.3E-01	2.6E+00	8.3E+00					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-B01-A	1	2.84E+01			2.84E+01	1.6E+01	2.6E+00	8.3E+00					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-B02-A	1	1.10E+01			1.10E+01	7.3E+01	2.6E+00	8.3E+00					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-B03-A	1	2.32E+01			2.32E+01	1.0E+01	2.6E+00	8.3E+00					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-B01-B	1	1.10E+01			1.10E+01	6.9E+01	2.6E+00	8.3E+00					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-B02-B	1	2.48E+01			2.48E+01	3.2E+01	2.6E+00	8.3E+00					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-B03-B	1	2.79E+01			2.79E+01	9.5E+00	2.6E+00	8.3E+00					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-B01-C	1	2.87E+01			2.87E+01	1.5E+01	2.6E+00	8.3E+00					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-B02-C	1	1.39E+01			1.39E+01	3.4E+01	2.6E+00	8.3E+00					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1313-B03-C	1	2.33E+01			2.33E+01	2.3E+01	2.6E+00	8.3E+00					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	EaFA-L05-1313-T01-A	1	3.59E+02			3.59E+02	9.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T02-A	1	2.48E+02			2.48E+02	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T03-A	1	1.88E+02			1.88E+02	6.2E-01	1.2E+00	3.8E+00	10	325	3.26E+03	94%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T04-A	1	1.56E+02			1.56E+02	4.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T05-A	1	8.42E+01			8.42E+01	1.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T06-A	1	1.03E+01			1.03E+01	1.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T07-A	1	8.81E+00			8.81E+00	1.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T08-A	1	5.26E+02			5.26E+02	2.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T09-A	1	1.74E+03			1.74E+03	7.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T01-B	1	3.54E+02			3.54E+02	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T02-B	1	2.55E+02			2.55E+02	9.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T03-B	1	2.05E+02			2.05E+02	3.7E-01	1.2E+00	3.8E+00	10	325	3.35E+03	97%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T04-B	1	1.38E+02			1.38E+02	1.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T05-B	1	8.52E+01			8.52E+01	1.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T06-B	1	1.13E+01			1.13E+01	1.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T07-B	1	4.08E+00			4.08E+00	2.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T08-B	1	6.03E+02			6.03E+02	1.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T09-B	1	1.80E+03			1.80E+03	1.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T01-C	1	4.13E+02			4.13E+02	5.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T02-C	1	2.78E+02			2.78E+02	5.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T03-C	1	2.44E+02			2.44E+02	5.8E-01	1.2E+00	3.8E+00	10	325	3.44E+03	98%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T04-C	1	1.54E+02			1.54E+02	1.5E+00	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T05-C	1	6.13E+01			6.13E+01	1.3E+00	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T06-C	1	4.87E+00			4.87E+00	4.5E+00	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T07-C	1	1.34E+01			1.34E+01	4.4E+00	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T08-C	1	4.38E+02			4.38E+02	4.7E-01	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-T09-C	1	1.82E+03			1.82E+03	2.6E-01	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	1.5E+02	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	6.5E+01	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-B03-A	1	6.00E-01	U1/2		6.00E-01	1.4E+02	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-B01-B	1	6.00E-01	U1/2		6.00E-01	1.7E+02	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-B02-B	1	6.00E-01	U1/2		6.00E-01	9.7E+01	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-B03-B	1	6.00E-01	U1/2		6.00E-01	3.6E+02	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-B01-C	1	6.00E-01	U1/2		6.00E-01	5.7E+01	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-B02-C	1	6.00E-01	U1/2		6.00E-01	7.3E+01	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1313-B03-C	1	6.00E-01	U1/2		6.00E-01	1.8E+02	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	EaFA-L05-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	7.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	4.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	9.2E+01	1.8E+00	5.7E+00	10	325	3.13E+03	96%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	8.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T05-A	1	6.72E+00			6.72E+00	7.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T06-A	1	1.53E+02			1.53E+02	3.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T07-A	1	1.76E+02			1.76E+02	2.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T08-A	1	2.18E+02			2.18E+02	9.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T09-A	1	3.86E+02			3.86E+02	6.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	3.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	2.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	2.7E+01	1.8E+00	5.7E+00	10	325	3.19E+03	98%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	1.9E+02	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T05-B	1	4.97E+00	E		4.97E+00	4.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T06-B	1	1.39E+02			1.39E+02	2.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T07-B	1	1.91E+02			1.91E+02	2.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T08-B	1	2.18E+02			2.18E+02	8.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T09-B	1	4.06E+02			4.06E+02	2.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	4.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	8.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	1.6E+02	1.8E+00	5.7E+00	10	325	3.26E+03	100%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	6.3E+01	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T05-C	1	1.65E+01			1.65E+01	4.8E+00	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T06-C	1	1.76E+02			1.76E+02	1.0E+01	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T07-C	1	1.40E+02			1.40E+02	1.3E+00	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T08-C	1	2.20E+02			2.20E+02	1.0E+00	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-T09-C	1	3.95E+02			3.95E+02	7.6E-02	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	6.7E+01	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	6.8E+01	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	7.1E+02	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-B01-B	1	9.00E-01	U1/2		9.00E-01	5.3E+01	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-B02-B	1	9.00E-01	U1/2		9.00E-01	4.3E+02	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-B03-B	1	9.00E-01	U1/2		9.00E-01	1.2E+02	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-B01-C	1	9.00E-01	U1/2		9.00E-01	6.5E+01	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-B02-C	1	9.00E-01	U1/2		9.00E-01	9.9E+01	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1313-B03-C	1	9.00E-01	U1/2		9.00E-01	8.1E+02	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	EaFA-L05-1313-T01-A	1	2.65E+01			2.65E+01	2.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T02-A	1	4.77E+00	E		4.77E+00	4.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T03-A	1	8.12E+00	E		8.12E+00	2.5E+01	3.7E+00	1.2E+01	10	325	3.05E+03	94%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T04-A	1	7.12E+00	E		7.12E+00	1.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T05-A	1	1.02E+01	E		1.02E+01	1.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T06-A	1	1.20E+01			1.20E+01	2.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T07-A	1	9.97E+00	E		9.97E+00	1.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T08-A	1	2.29E+03			2.29E+03	6.8E-01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T09-A	1	3.05E+03			3.05E+03	7.7E-01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T01-B	1	2.87E+01			2.87E+01	9.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T02-B	1	1.85E+00	U1/2		1.85E+00	5.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T03-B	1	3.78E+00	E		3.78E+00	5.7E+01	3.7E+00	1.2E+01	10	325	3.12E+03	96%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T04-B	1	7.86E+00	E		7.86E+00	4.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T05-B	1	7.03E+00	E		7.03E+00	3.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T06-B	1	5.70E+00	E		5.70E+00	4.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T07-B	1	2.11E+01			2.11E+01	9.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T08-B	1	2.32E+03			2.32E+03	9.2E-01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T09-B	1	3.07E+03			3.07E+03	1.9E-01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T01-C	1	2.96E+01			2.96E+01	9.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T02-C	1	4.47E+00	E		4.47E+00	5.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T03-C	1	7.23E+00	E		7.23E+00	5.8E+01	3.7E+00	1.2E+01	10	325	3.17E+03	97%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T04-C	1	5.49E+00	E		5.49E+00	5.0E+01	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T05-C	1	7.57E+00	E		7.57E+00	3.2E+01	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T06-C	1	6.33E+01			6.33E+01	2.3E+01	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T07-C	1	1.21E+01			1.21E+01	2.1E+01	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T08-C	1	2.18E+03			2.18E+03	7.5E-01	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-T09-C	1	3.08E+03			3.08E+03	3.4E-01	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	7.4E+01	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	1.3E+04	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-B03-A	1	1.85E+00	U1/2		1.85E+00	2.2E+02	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-B01-B	1	1.85E+00	U1/2		1.85E+00	4.2E+02	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-B02-B	1	1.85E+00	U1/2		1.85E+00	1.0E+02	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-B03-B	1	1.85E+00	U1/2		1.85E+00	8.9E+01	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-B01-C	1	1.85E+00	U1/2		1.85E+00	1.7E+03	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-B02-C	1	1.85E+00	U1/2		1.85E+00	7.2E+02	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1313-B03-C	1	1.85E+00	U1/2		1.85E+00	1.9E+02	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	EaFA-L05-1313-T01-A	1	3.21E+01			3.21E+01	1.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T02-A	1	1.13E+01			1.13E+01	3.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T03-A	1	6.18E+00	E		6.18E+00	5.7E+00	2.0E+00	6.4E+00	1000	100	9.58E+02	95%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	4.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	7.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	5.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T08-A	1	1.09E+03			1.09E+03	6.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T09-A	1	3.07E+04			3.07E+04	2.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T01-B	1	3.91E+01			3.91E+01	1.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T02-B	1	1.20E+01			1.20E+01	1.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T03-B	1	4.94E+00	E		4.94E+00	2.4E+00	2.0E+00	6.4E+00	1000	100	9.86E+02	98%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	8.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	7.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	1.5E+02	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T08-B	1	1.24E+03			1.24E+03	5.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T09-B	1	3.50E+04			3.50E+04	2.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T01-C	1	3.45E+01			3.45E+01	2.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T02-C	1	1.19E+01			1.19E+01	3.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T03-C	1	4.00E+00	E		4.00E+00	1.4E+01	2.0E+00	6.4E+00	1000	100	1.00E+03	100%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	4.9E+02	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	4.0E+01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	7.8E+01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	6.7E+01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T08-C	1	9.61E+02			9.61E+02	1.0E+00	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-T09-C	1	3.33E+04			3.33E+04	8.3E-01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.7E+02	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-B03-A	1	3.19E+00	E		3.19E+00	5.4E+01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	1.1E+04	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	1.0E+02	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-B03-B	1	2.47E+00	E		2.47E+00	5.0E+00	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	3.2E+01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1313-B03-C	1	2.64E+00	E		2.64E+00	1.4E+01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	EaFA-L05-1313-T01-A	1	3.40E+00	U1/2		3.40E+00	1.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T02-A	1	3.40E+00	U1/2		3.40E+00	5.7E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T03-A	1	3.40E+00	U1/2		3.40E+00	6.5E+00	6.8E+00	2.2E+01	10	325	2.99E+03	92%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T04-A	1	3.40E+00	U1/2		3.40E+00	4.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T05-A	1	3.40E+00	U1/2		3.40E+00	7.6E+03	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T06-A	1	3.40E+00	U1/2		3.40E+00	1.3E+02	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T07-A	1	3.40E+00	U1/2		3.40E+00	7.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T08-A	1	3.40E+00	U1/2		3.40E+00	3.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T09-A	1	1.21E+02			1.21E+02	2.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T01-B	1	3.40E+00	U1/2		3.40E+00	1.5E+02	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T02-B	1	3.40E+00	U1/2		3.40E+00	3.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T03-B	1	3.40E+00	U1/2		3.40E+00	2.0E+01	6.8E+00	2.2E+01	10	325	3.10E+03	95%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T04-B	1	3.40E+00	U1/2		3.40E+00	1.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T05-B	1	3.40E+00	U1/2		3.40E+00	3.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T06-B	1	3.40E+00	U1/2		3.40E+00	2.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T07-B	1	3.40E+00	U1/2		3.40E+00	2.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T08-B	1	3.40E+00	U1/2		3.40E+00	5.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T09-B	1	1.33E+02			1.33E+02	5.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T01-C	1	3.40E+00	U1/2		3.40E+00	3.9E+02	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T02-C	1	3.40E+00	U1/2		3.40E+00	4.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T03-C	1	3.40E+00	U1/2		3.40E+00	3.4E+01	6.8E+00	2.2E+01	10	325	3.16E+03	97%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T04-C	1	3.40E+00	U1/2		3.40E+00	6.9E+01	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T05-C	1	3.40E+00	U1/2		3.40E+00	2.8E+02	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T06-C	1	3.40E+00	U1/2		3.40E+00	1.4E+02	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T07-C	1	3.40E+00	U1/2		3.40E+00	3.3E+01	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T08-C	1	3.40E+00	U1/2		3.40E+00	4.6E+01	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-T09-C	1	1.25E+02			1.25E+02	4.6E+00	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	4.6E+01	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	8.6E+01	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	5.1E+01	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-B01-B	1	3.40E+00	U1/2		3.40E+00	1.4E+01	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-B02-B	1	3.40E+00	U1/2		3.40E+00	7.3E+01	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-B03-B	1	3.40E+00	U1/2		3.40E+00	6.4E+01	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-B01-C	1	3.40E+00	U1/2		3.40E+00	1.9E+01	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-B02-C	1	3.40E+00	U1/2		3.40E+00	3.3E+01	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1313-B03-C	1	3.40E+00	U1/2		3.40E+00	6.6E+02	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	EaFA-L05-1313-T01-A	1	1.99E+03			1.99E+03	6.8E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T02-A	1	2.58E+03			2.58E+03	9.2E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T03-A	1	2.71E+03			2.71E+03	6.0E-01	1.9E+00	6.0E+00	10	325	5.49E+03	86%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T04-A	1	2.87E+03			2.87E+03	1.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T05-A	1	3.48E+03			3.48E+03	3.2E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T06-A	1	3.77E+03			3.77E+03	5.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T07-A	1	3.80E+03			3.80E+03	6.6E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T08-A	1	2.38E+03			2.38E+03	5.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T09-A	1	1.67E+03			1.67E+03	3.9E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T01-B	1	1.92E+03			1.92E+03	2.6E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T02-B	1	2.65E+03			2.65E+03	6.6E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T03-B	1	2.69E+03			2.69E+03	5.2E-01	1.9E+00	6.0E+00	10	325	5.47E+03	86%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T04-B	1	2.96E+03			2.96E+03	7.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T05-B	1	3.35E+03			3.35E+03	7.2E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T06-B	1	3.70E+03			3.70E+03	3.8E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T07-B	1	3.77E+03			3.77E+03	1.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T08-B	1	2.36E+03			2.36E+03	6.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T09-B	1	1.58E+03			1.58E+03	7.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T01-C	1	2.04E+03			2.04E+03	7.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T02-C	1	2.69E+03			2.69E+03	2.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T03-C	1	3.00E+03			3.00E+03	4.2E-01	1.9E+00	6.0E+00	10	325	5.84E+03	87%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T04-C	1	2.98E+03			2.98E+03	2.1E-01	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T05-C	1	3.42E+03			3.42E+03	5.8E-01	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T06-C	1	3.68E+03			3.68E+03	1.2E+01	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T07-C	1	3.73E+03			3.73E+03	8.5E-01	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T08-C	1	2.37E+03			2.37E+03	6.0E-01	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-T09-C	1	1.64E+03			1.64E+03	7.4E-01	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-B01-A	1	3.72E+00	E		3.72E+00	2.7E+01	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-B02-A	1	4.47E+00	E		4.47E+00	1.1E+01	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-B03-A	1	3.30E+00	E		3.30E+00	2.6E+01	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-B01-B	1	3.41E+00	E		3.41E+00	4.2E+01	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-B02-B	1	3.30E+00	E		3.30E+00	2.0E+01	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-B03-B	1	3.24E+00	E		3.24E+00	8.1E+00	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-B01-C	1	3.27E+00	E		3.27E+00	6.4E+01	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-B02-C	1	4.80E+00	E		4.80E+00	1.6E+01	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1313-B03-C	1	4.18E+00	E		4.18E+00	2.1E+01	1.9E+00	6.0E+00					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	EaFA-L05-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	9.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	9.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	3.9E+02	2.0E+00	6.4E+00	10	325	3.03E+03	93%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T05-A	1	8.49E+01			8.49E+01	2.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T06-A	1	5.82E+02			5.82E+02	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T07-A	1	6.20E+02			6.20E+02	7.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T08-A	1	9.97E+02			9.97E+02	1.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T09-A	1	1.53E+03			1.53E+03	4.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	7.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00	10	325	3.13E+03	96%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	2.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T05-B	1	8.04E+01			8.04E+01	9.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T06-B	1	5.36E+02			5.36E+02	1.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T07-B	1	6.28E+02			6.28E+02	8.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T08-B	1	9.78E+02			9.78E+02	3.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T09-B	1	1.59E+03			1.59E+03	1.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	8.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	6.6E+02	2.0E+00	6.4E+00	10	325	3.19E+03	98%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	6.2E+00	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T05-C	1	1.42E+02			1.42E+02	8.2E-01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T06-C	1	5.48E+02			5.48E+02	9.9E+00	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T07-C	1	5.59E+02			5.59E+02	1.0E+00	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T08-C	1	1.04E+03			1.04E+03	4.6E-01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-T09-C	1	1.59E+03			1.59E+03	2.0E-01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.0E+01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	6.2E-01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	9.6E+02	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	4.4E+02	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	1.3E+03	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1313-B03-C	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	EaFA-L05-1313-T01-A	1	5.00E-01	U1/2		5.00E-01	3.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T02-A	1	5.00E-01	U1/2		5.00E-01	2.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T03-A	1	5.13E+01			5.13E+01	1.6E+01	1.0E+00	3.2E+00	1000	100	1.00E+03	95%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T04-A	1	3.33E+03			3.33E+03	8.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T05-A	1	5.49E+03			5.49E+03	5.5E-02	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T06-A	1	7.17E+03			7.17E+03	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T07-A	1	7.16E+03			7.16E+03	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T08-A	1	8.17E+03			8.17E+03	8.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T09-A	1	1.29E+04			1.29E+04	8.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T01-B	1	5.00E-01	U1/2		5.00E-01	2.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T02-B	1	5.00E-01	U1/2		5.00E-01	8.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T03-B	1	5.73E+01			5.73E+01	1.6E+01	1.0E+00	3.2E+00	1000	100	1.06E+03	100%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T04-B	1	3.45E+03			3.45E+03	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T05-B	1	5.03E+03			5.03E+03	9.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T06-B	1	7.01E+03			7.01E+03	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T07-B	1	6.87E+03			6.87E+03	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T08-B	1	8.10E+03			8.10E+03	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T09-B	1	1.34E+04			1.34E+04	9.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T01-C	1	5.00E-01	U1/2		5.00E-01	6.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T02-C	1	5.00E-01	U1/2		5.00E-01	4.1E+02	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T03-C	1	8.21E+01			8.21E+01	1.0E+01	1.0E+00	3.2E+00	1000	100	1.09E+03	101%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T04-C	1	3.35E+03			3.35E+03	4.1E-01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T05-C	1	5.19E+03			5.19E+03	8.6E-01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T06-C	1	6.61E+03			6.61E+03	9.8E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T07-C	1	6.96E+03			6.96E+03	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T08-C	1	8.19E+03			8.19E+03	5.9E-01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-T09-C	1	1.31E+04			1.31E+04	1.6E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.6E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.3E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	5.8E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	3.2E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	2.3E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	1.8E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	2.6E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	6.4E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	EaFA-L05-1313-T01-A	1	3.95E+03			3.95E+03	2.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T02-A	1	4.01E+03			4.01E+03	8.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T03-A	1	3.74E+03			3.74E+03	2.8E-01	1.2E+00	3.8E+00	10	325	6.65E+03	90%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T04-A	1	3.73E+03			3.73E+03	2.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T05-A	1	3.72E+03			3.72E+03	1.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T06-A	1	2.29E+03			2.29E+03	6.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T07-A	1	1.94E+03			1.94E+03	3.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T08-A	1	1.17E+02			1.17E+02	2.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T09-A	1	5.68E+02			5.68E+02	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T01-B	1	4.03E+03			4.03E+03	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T02-B	1	4.01E+03			4.01E+03	1.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T03-B	1	3.80E+03			3.80E+03	1.9E-01	1.2E+00	3.8E+00	10	325	6.63E+03	87%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T04-B	1	3.60E+03			3.60E+03	5.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T05-B	1	3.34E+03			3.34E+03	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T06-B	1	2.40E+03			2.40E+03	3.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T07-B	1	1.44E+03			1.44E+03	5.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T08-B	1	1.18E+02			1.18E+02	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T09-B	1	5.47E+02			5.47E+02	6.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T01-C	1	4.03E+03			4.03E+03	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T02-C	1	4.08E+03			4.08E+03	8.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T03-C	1	3.99E+03			3.99E+03	5.2E-01	1.2E+00	3.8E+00	10	325	6.89E+03	89%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T04-C	1	3.78E+03			3.78E+03	1.4E+00	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T05-C	1	3.45E+03			3.45E+03	6.0E-01	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T06-C	1	1.18E+03			1.18E+03	1.2E+01	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T07-C	1	2.29E+03			2.29E+03	1.0E+00	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T08-C	1	1.32E+02			1.32E+02	1.8E+00	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-T09-C	1	5.66E+02			5.66E+02	4.6E-01	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-B01-A	1	1.04E+01			1.04E+01	6.2E+00	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-B02-A	1	8.14E+00			8.14E+00	1.7E+01	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-B03-A	1	1.72E+01			1.72E+01	1.3E+01	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-B01-B	1	1.35E+01			1.35E+01	1.9E+01	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-B02-B	1	6.99E+00			6.99E+00	9.3E+01	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-B03-B	1	1.44E+01			1.44E+01	1.7E+00	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-B01-C	1	1.35E+01			1.35E+01	2.3E+01	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-B02-C	1	4.36E+00			4.36E+00	7.6E+01	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1313-B03-C	1	1.11E+01			1.11E+01	3.6E+01	1.2E+00	3.8E+00					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	EaFA-L05-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	5.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T02-A	1	1.98E+00	E		1.98E+00	1.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	3.6E+02	1.8E+00	5.7E+00	10	325	3.05E+03	94%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T04-A	1	3.06E+00	E		3.06E+00	1.6E+02	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T05-A	1	2.20E+01			2.20E+01	1.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T06-A	1	3.42E+02			3.42E+02	2.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T07-A	1	4.02E+02			4.02E+02	4.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T08-A	1	5.09E+02			5.09E+02	5.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T09-A	1	6.87E+02			6.87E+02	4.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	2.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	5.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	1.2E+02	1.8E+00	5.7E+00	10	325	3.15E+03	97%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	1.8E+02	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T05-B	1	1.96E+01			1.96E+01	7.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T06-B	1	3.00E+02			3.00E+02	8.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T07-B	1	4.54E+02			4.54E+02	1.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T08-B	1	5.13E+02			5.13E+02	1.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T09-B	1	7.05E+02			7.05E+02	2.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T01-C	1	2.50E+00	E		2.50E+00	2.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	1.9E+02	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	1.5E+03	1.8E+00	5.7E+00	10	325	3.24E+03	100%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	1.9E+03	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T05-C	1	5.14E+01			5.14E+01	5.8E+00	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T06-C	1	4.45E+02			4.45E+02	1.2E+01	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T07-C	1	3.14E+02			3.14E+02	2.5E+00	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T08-C	1	5.21E+02			5.21E+02	1.2E+00	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-T09-C	1	7.01E+02			7.01E+02	3.4E-01	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	2.0E+03	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	6.8E+02	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-B01-B	1	9.00E-01	U1/2		9.00E-01	1.0E+02	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-B02-B	1	9.00E-01	U1/2		9.00E-01	4.7E+02	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-B03-B	1	9.00E-01	U1/2		9.00E-01	3.7E+02	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-B01-C	1	9.00E-01	U1/2		9.00E-01	2.4E+02	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-B02-C	1	9.00E-01	U1/2		9.00E-01	1.2E+02	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1313-B03-C	1	9.00E-01	U1/2		9.00E-01	8.3E+02	1.8E+00	5.7E+00					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	EaFA-L05-1313-T01-A	1	5.06E+01			5.06E+01	1.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T02-A	1	1.70E+01			1.70E+01	5.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T03-A	1	2.72E+01			2.72E+01	5.1E+01	3.7E+00	1.2E+01	1000	100	9.58E+02	93%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T04-A	1	6.14E+01			6.14E+01	1.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T05-A	1	1.51E+01			1.51E+01	3.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T06-A	1	5.09E+00	E		5.09E+00	1.0E+02	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T07-A	1	1.48E+01			1.48E+01	6.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T08-A	1	4.54E+01			4.54E+01	1.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T09-A	1	3.93E+03			3.93E+03	2.2E-01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T01-B	1	6.49E+01			6.49E+01	9.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T02-B	1	1.42E+01			1.42E+01	4.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T03-B	1	2.59E+01			2.59E+01	6.3E+01	3.7E+00	1.2E+01	1000	100	9.90E+02	96%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T04-B	1	2.78E+01			2.78E+01	1.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T05-B	1	2.48E+01			2.48E+01	5.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T06-B	1	7.85E+00	E		7.85E+00	6.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T07-B	1	9.80E+00	E		9.80E+00	1.0E+02	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T08-B	1	4.89E+01			4.89E+01	3.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T09-B	1	4.29E+03			4.29E+03	5.0E-01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T01-C	1	6.20E+01			6.20E+01	4.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T02-C	1	2.14E+01			2.14E+01	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T03-C	1	3.73E+01			3.73E+01	2.2E+01	3.7E+00	1.2E+01	1000	100	1.01E+03	97%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T04-C	1	5.11E+01			5.11E+01	3.6E+00	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T05-C	1	1.95E+01			1.95E+01	4.1E+01	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T06-C	1	1.44E+01			1.44E+01	5.2E+01	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T07-C	1	1.54E+01			1.54E+01	3.2E+01	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T08-C	1	4.29E+01			4.29E+01	1.1E+01	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-T09-C	1	4.31E+03			4.31E+03	5.4E-01	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-B01-A	1	7.30E+00	E		7.30E+00	4.9E+01	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	1.1E+05	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-B03-A	1	4.88E+01			4.88E+01	3.4E+01	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-B01-B	1	3.75E+00	E		3.75E+00	1.1E+02	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-B02-B	1	1.85E+00	U1/2		1.85E+00	1.1E+02	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-B03-B	1	6.44E+01			6.44E+01	7.6E-01	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-B01-C	1	1.02E+01	E		1.02E+01	7.4E+01	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-B02-C	1	1.85E+00	U1/2		1.85E+00	4.1E+01	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1313-B03-C	1	5.98E+01			5.98E+01	1.2E+01	3.7E+00	1.2E+01					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	EaFA-L05-1313-T01-A	1	1.55E+06			1.55E+06	1.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T02-A	1	3.74E+05			3.74E+05	1.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T03-A	1	1.79E+05			1.79E+05	8.2E-01	1.6E+00	5.1E+00	1000	100	1.80E+05	87%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T04-A	1	1.06E+05			1.06E+05	4.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T05-A	1	6.21E+04			6.21E+04	1.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T06-A	1	2.38E+04			2.38E+04	8.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T07-A	1	2.38E+04			2.38E+04	9.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T08-A	1	1.72E+04			1.72E+04	1.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T09-A	1	1.87E+04			1.87E+04	2.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T01-B	1	1.52E+06			1.52E+06	5.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T02-B	1	3.64E+05			3.64E+05	3.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T03-B	1	1.76E+05			1.76E+05	7.2E-01	1.6E+00	5.1E+00	1000	100	1.77E+05	83%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T04-B	1	1.08E+05			1.08E+05	5.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T05-B	1	6.07E+04			6.07E+04	6.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T06-B	1	2.29E+04			2.29E+04	3.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T07-B	1	2.34E+04			2.34E+04	1.6E+00	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T08-B	1	1.71E+04			1.71E+04	4.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T09-B	1	1.88E+04			1.88E+04	4.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T01-C	1	1.54E+06			1.54E+06	4.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T02-C	1	3.80E+05			3.80E+05	2.5E+00	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T03-C	1	1.83E+05			1.83E+05	2.6E-01	1.6E+00	5.1E+00	1000	100	1.84E+05	88%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T04-C	1	1.07E+05			1.07E+05	4.4E-01	1.6E+00	5.1E+00					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T05-C	1	6.17E+04			6.17E+04	2.8E-01	1.6E+00	5.1E+00					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T06-C	1	2.33E+04			2.33E+04	9.0E+00	1.6E+00	5.1E+00					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T07-C	1	2.33E+04			2.33E+04	7.4E-01	1.6E+00	5.1E+00					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T08-C	1	1.72E+04			1.72E+04	4.4E-01	1.6E+00	5.1E+00					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-T09-C	1	1.89E+04			1.89E+04	7.7E-01	1.6E+00	5.1E+00					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-B01-A	1	8.55E+01			8.55E+01	1.3E+00	1.6E+00	5.1E+00					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-B02-A	1	2.35E+02			2.35E+02	1.2E+00	1.6E+00	5.1E+00					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-B03-A	1	1.58E+06			1.58E+06	1.8E+00	1.6E+00	5.1E+00					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-B01-B	1	1.79E+02			1.79E+02	9.7E-01	1.6E+00	5.1E+00					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-B02-B	1	1.98E+02			1.98E+02	2.7E+00	1.6E+00	5.1E+00					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-B03-B	1	1.56E+06			1.56E+06	1.4E+00	1.6E+00	5.1E+00					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-B01-C	1	1.19E+02			1.19E+02	8.2E-01	1.6E+00	5.1E+00					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-B02-C	1	1.93E+02			1.93E+02	1.6E+00	1.6E+00	5.1E+00					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1313-B03-C	1	1.58E+06			1.58E+06	3.9E-01	1.6E+00	5.1E+00					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	EaFA-L05-1313-T01-A	1	6.64E+03			6.64E+03	6.4E-01	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T02-A	1	5.30E+03			5.30E+03	1.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T03-A	1	4.40E+03			4.40E+03	1.6E+00	1.5E+01	4.8E+01	10	325	7.23E+03	87%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T04-A	1	3.23E+03			3.23E+03	1.6E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T05-A	1	1.59E+03			1.59E+03	1.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T06-A	1	5.75E+02			5.75E+02	5.8E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T07-A	1	5.47E+02			5.47E+02	1.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T08-A	1	1.02E+02			1.02E+02	1.0E+01	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T09-A	1	1.14E+03			1.14E+03	1.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T01-B	1	6.67E+03			6.67E+03	1.0E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T02-B	1	5.43E+03			5.43E+03	8.3E-01	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T03-B	1	4.66E+03			4.66E+03	1.8E+00	1.5E+01	4.8E+01	10	325	7.39E+03	84%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T04-B	1	3.10E+03			3.10E+03	1.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T05-B	1	1.45E+03			1.45E+03	4.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T06-B	1	5.64E+02			5.64E+02	7.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T07-B	1	4.34E+02			4.34E+02	6.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T08-B	1	9.32E+01			9.32E+01	7.6E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T09-B	1	1.21E+03			1.21E+03	5.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T01-C	1	6.74E+03			6.74E+03	5.5E-01	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T02-C	1	5.68E+03			5.68E+03	1.0E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T03-C	1	5.13E+03			5.13E+03	9.9E-01	1.5E+01	4.8E+01	10	325	7.88E+03	85%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T04-C	1	3.12E+03			3.12E+03	1.9E-01	1.5E+01	4.8E+01					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T05-C	1	1.14E+03			1.14E+03	1.9E+00	1.5E+01	4.8E+01					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T06-C	1	4.11E+02			4.11E+02	2.0E+01	1.5E+01	4.8E+01					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T07-C	1	5.66E+02			5.66E+02	5.8E+00	1.5E+01	4.8E+01					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T08-C	1	1.00E+02			1.00E+02	3.4E+00	1.5E+01	4.8E+01					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-T09-C	1	1.25E+03			1.25E+03	1.5E+00	1.5E+01	4.8E+01					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-B01-A	1	3.33E+01	E		3.33E+01	2.1E+01	1.5E+01	4.8E+01					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-B02-A	1	3.84E+01	E		3.84E+01	6.7E+01	1.5E+01	4.8E+01					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-B03-A	1	7.50E+00	U1/2		7.50E+00	6.8E+01	1.5E+01	4.8E+01					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-B01-B	1	3.60E+01	E		3.60E+01	5.9E+01	1.5E+01	4.8E+01					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-B02-B	1	3.99E+01	E		3.99E+01	7.8E+01	1.5E+01	4.8E+01					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-B03-B	1	7.50E+00	U1/2		7.50E+00	5.8E+02	1.5E+01	4.8E+01					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-B01-C	1	2.39E+01	E		2.39E+01	6.8E+01	1.5E+01	4.8E+01					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-B02-C	1	2.53E+01	E		2.53E+01	7.7E+01	1.5E+01	4.8E+01					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1313-B03-C	1	7.50E+00	U1/2		7.50E+00	2.1E+02	1.5E+01	4.8E+01					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	EaFA-L05-1313-T01-A	1	9.02E+03			9.02E+03	7.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T02-A	1	3.25E+03			3.25E+03	8.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T03-A	1	1.22E+03			1.22E+03	5.2E-01	1.1E+00	3.5E+00	1000	100	2.20E+03	98%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T04-A	1	2.71E+02			2.71E+02	1.9E+00	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T05-A	1	8.07E+02			8.07E+02	4.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T06-A	1	3.60E+03			3.60E+03	8.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T07-A	1	4.30E+03			4.30E+03	4.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T08-A	1	2.44E+04			2.44E+04	1.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T09-A	1	5.77E+04			5.77E+04	7.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T01-B	1	9.79E+03			9.79E+03	8.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T02-B	1	3.09E+03			3.09E+03	9.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T03-B	1	1.25E+03			1.25E+03	1.4E+00	1.1E+00	3.5E+00	1000	100	2.21E+03	96%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T04-B	1	2.25E+02			2.25E+02	9.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T05-B	1	7.04E+02			7.04E+02	1.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T06-B	1	3.36E+03			3.36E+03	6.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T07-B	1	4.38E+03			4.38E+03	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T08-B	1	2.49E+04			2.49E+04	6.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T09-B	1	6.51E+04			6.51E+04	5.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T01-C	1	1.07E+04			1.07E+04	4.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T02-C	1	3.41E+03			3.41E+03	4.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T03-C	1	1.02E+03			1.02E+03	2.5E-01	1.1E+00	3.5E+00	1000	100	2.03E+03	101%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T04-C	1	2.64E+02			2.64E+02	6.8E-01	1.1E+00	3.5E+00					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T05-C	1	1.00E+03			1.00E+03	9.3E-01	1.1E+00	3.5E+00					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T06-C	1	3.89E+03			3.89E+03	1.3E+01	1.1E+00	3.5E+00					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T07-C	1	3.80E+03			3.80E+03	8.7E-01	1.1E+00	3.5E+00					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T08-C	1	2.49E+04			2.49E+04	1.1E+00	1.1E+00	3.5E+00					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-T09-C	1	6.23E+04			6.23E+04	3.4E-01	1.1E+00	3.5E+00					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-B01-A	1	5.50E-01	U1/2		5.50E-01	6.7E+00	1.1E+00	3.5E+00					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-B02-A	1	5.50E-01	U1/2		5.50E-01	1.2E+01	1.1E+00	3.5E+00					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-B03-A	1	2.37E+02			2.37E+02	8.4E+00	1.1E+00	3.5E+00					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-B01-B	1	5.50E-01	U1/2		5.50E-01	3.0E+01	1.1E+00	3.5E+00					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-B02-B	1	5.50E-01	U1/2		5.50E-01	3.2E+01	1.1E+00	3.5E+00					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-B03-B	1	3.37E+02			3.37E+02	1.1E+01	1.1E+00	3.5E+00					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-B01-C	1	5.50E-01	U1/2		5.50E-01	4.3E+01	1.1E+00	3.5E+00					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-B02-C	1	5.50E-01	U1/2		5.50E-01	1.5E+01	1.1E+00	3.5E+00					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1313-B03-C	1	2.53E+02			2.53E+02	2.9E+00	1.1E+00	3.5E+00					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	EaFA-L05-1313-T01-A	1	1.28E+04			1.28E+04	4.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T02-A	1	7.26E+03			7.26E+03	5.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T03-A	1	6.39E+03			6.39E+03	4.0E-01	2.5E+00	8.0E+00	1000	100	7.33E+03	94%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T04-A	1	6.35E+03			6.35E+03	2.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T05-A	1	6.44E+03			6.44E+03	6.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T06-A	1	6.51E+03			6.51E+03	3.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T07-A	1	6.54E+03			6.54E+03	7.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T08-A	1	4.38E+03			4.38E+03	7.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T09-A	1	3.75E+03			3.75E+03	1.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T01-B	1	1.28E+04			1.28E+04	3.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T02-B	1	7.30E+03			7.30E+03	4.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T03-B	1	6.38E+03			6.38E+03	2.5E-01	2.5E+00	8.0E+00	1000	100	7.45E+03	107%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T04-B	1	6.48E+03			6.48E+03	8.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T05-B	1	6.29E+03			6.29E+03	7.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T06-B	1	6.33E+03			6.33E+03	1.0E+00	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T07-B	1	6.45E+03			6.45E+03	1.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T08-B	1	4.33E+03			4.33E+03	3.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T09-B	1	3.55E+03			3.55E+03	3.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T01-C	1	1.27E+04			1.27E+04	4.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T02-C	1	7.24E+03			7.24E+03	6.4E-02	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T03-C	1	6.71E+03			6.71E+03	4.0E-01	2.5E+00	8.0E+00	1000	100	7.66E+03	95%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T04-C	1	6.38E+03			6.38E+03	5.0E-01	2.5E+00	8.0E+00					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T05-C	1	6.32E+03			6.32E+03	5.6E-01	2.5E+00	8.0E+00					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T06-C	1	6.33E+03			6.33E+03	1.2E+01	2.5E+00	8.0E+00					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T07-C	1	6.34E+03			6.34E+03	4.0E-01	2.5E+00	8.0E+00					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T08-C	1	4.33E+03			4.33E+03	9.9E-01	2.5E+00	8.0E+00					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-T09-C	1	3.58E+03			3.58E+03	7.1E-01	2.5E+00	8.0E+00					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-B01-A	1	2.43E+01			2.43E+01	4.2E-01	2.5E+00	8.0E+00					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-B02-A	1	2.64E+01			2.64E+01	8.8E-01	2.5E+00	8.0E+00					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-B03-A	1	6.65E+03			6.65E+03	2.2E+00	2.5E+00	8.0E+00					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-B01-B	1	1.85E+01			1.85E+01	2.9E+00	2.5E+00	8.0E+00					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-B02-B	1	2.21E+01			2.21E+01	3.2E+00	2.5E+00	8.0E+00					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-B03-B	1	6.61E+03			6.61E+03	1.2E+00	2.5E+00	8.0E+00					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-B01-C	1	2.70E+01			2.70E+01	1.7E+00	2.5E+00	8.0E+00					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-B02-C	1	2.26E+01			2.26E+01	2.9E+00	2.5E+00	8.0E+00					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1313-B03-C	1	6.93E+03			6.93E+03	5.7E-01	2.5E+00	8.0E+00					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	EaFA-L05-1313-T01-A	1	1.35E+03			1.35E+03	1.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T02-A	1	1.52E+03			1.52E+03	7.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T03-A	1	1.61E+03			1.61E+03	2.2E-01	1.0E+00	3.2E+00	1000	100	2.46E+03	84%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T04-A	1	1.81E+03			1.81E+03	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T05-A	1	2.07E+03			2.07E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T06-A	1	2.38E+03			2.38E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T07-A	1	2.40E+03			2.40E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T08-A	1	3.19E+03			3.19E+03	2.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T09-A	1	4.57E+03			4.57E+03	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T01-B	1	1.19E+03			1.19E+03	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T02-B	1	1.53E+03			1.53E+03	2.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T03-B	1	1.65E+03			1.65E+03	4.6E-01	1.0E+00	3.2E+00	1000	100	2.54E+03	89%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T04-B	1	1.73E+03			1.73E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T05-B	1	1.84E+03			1.84E+03	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T06-B	1	2.29E+03			2.29E+03	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T07-B	1	2.36E+03			2.36E+03	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T08-B	1	3.19E+03			3.19E+03	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T09-B	1	4.68E+03			4.68E+03	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T01-C	1	1.32E+03			1.32E+03	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T02-C	1	1.59E+03			1.59E+03	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T03-C	1	1.75E+03			1.75E+03	6.5E-01	1.0E+00	3.2E+00	1000	100	2.57E+03	83%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T04-C	1	1.84E+03			1.84E+03	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T05-C	1	1.98E+03			1.98E+03	9.4E-01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T06-C	1	2.35E+03			2.35E+03	9.9E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T07-C	1	2.28E+03			2.28E+03	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T08-C	1	3.14E+03			3.14E+03	1.7E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-T09-C	1	4.68E+03			4.68E+03	2.0E-01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.3E+03	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	3.3E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	2.2E+02	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	4.3E+02	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	7.3E+02	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-B03-B	1	1.25E+00	E		1.25E+00	8.1E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	9.4E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	3.3E+03	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	1.3E+02	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	EaFA-L05-1313-T01-A	1	1.71E+05			1.71E+05	4.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T02-A	1	1.62E+05			1.62E+05	7.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T03-A	1	1.53E+05			1.53E+05	1.3E-01	6.8E+00	2.2E+01	1000	100	1.54E+05	82%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T04-A	1	1.60E+05			1.60E+05	1.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T05-A	1	1.65E+05			1.65E+05	1.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T06-A	1	1.63E+05			1.63E+05	2.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T07-A	1	1.64E+05			1.64E+05	1.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T08-A	1	9.98E+04			9.98E+04	4.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T09-A	1	6.18E+04			6.18E+04	1.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T01-B	1	1.75E+05			1.75E+05	3.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T02-B	1	1.63E+05			1.63E+05	5.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T03-B	1	1.57E+05			1.57E+05	3.6E-01	6.8E+00	2.2E+01	1000	100	1.58E+05	87%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T04-B	1	1.58E+05			1.58E+05	4.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T05-B	1	1.54E+05			1.54E+05	2.8E-02	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T06-B	1	1.64E+05			1.64E+05	5.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T07-B	1	1.60E+05			1.60E+05	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T08-B	1	1.02E+05			1.02E+05	7.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T09-B	1	6.18E+04			6.18E+04	3.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T01-C	1	1.75E+05			1.75E+05	2.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T02-C	1	1.65E+05			1.65E+05	2.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T03-C	1	1.64E+05			1.64E+05	2.8E-01	6.8E+00	2.2E+01	1000	100	1.65E+05	86%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T04-C	1	1.63E+05			1.63E+05	6.8E-01	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T05-C	1	1.63E+05			1.63E+05	6.2E-01	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T06-C	1	1.60E+05			1.60E+05	1.3E+01	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T07-C	1	1.62E+05			1.62E+05	1.1E+00	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T08-C	1	9.92E+04			9.92E+04	1.0E+00	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-T09-C	1	6.34E+04			6.34E+04	1.7E-01	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-B01-A	1	1.53E+01	E		1.53E+01	5.5E+01	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	1.1E+03	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-B03-A	1	9.45E+02			9.45E+02	2.4E+01	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-B01-B	1	1.88E+01	E		1.88E+01	3.4E+01	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-B02-B	1	1.37E+01	E		1.37E+01	5.8E+01	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-B03-B	1	1.24E+03			1.24E+03	1.3E+00	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-B01-C	1	1.67E+01	E		1.67E+01	5.6E+01	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-B02-C	1	3.40E+00	U1/2		3.40E+00	2.1E+02	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1313-B03-C	1	1.07E+03			1.07E+03	3.1E+00	6.8E+00	2.2E+01					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	EaFA-L05-1313-T01-A	1	2.30E+00	U1/2		2.30E+00	1.0E+02	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T02-A	1	2.30E+00	U1/2		2.30E+00	2.5E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T03-A	1	2.30E+00	U1/2		2.30E+00	1.2E+02	4.6E+00	1.5E+01	10	325	2.99E+03	92%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T04-A	1	2.30E+00	U1/2		2.30E+00	5.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T05-A	1	2.30E+00	U1/2		2.30E+00	1.4E+02	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T06-A	1	2.30E+00	U1/2		2.30E+00	2.2E+02	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T07-A	1	7.12E+00	E		7.12E+00	1.5E+02	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T08-A	1	4.49E+01			4.49E+01	1.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T09-A	1	7.65E+01			7.65E+01	3.2E+00	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T01-B	1	2.30E+00	U1/2		2.30E+00	8.8E+02	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T02-B	1	2.30E+00	U1/2		2.30E+00	5.8E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T03-B	1	2.30E+00	U1/2		2.30E+00	9.3E+01	4.6E+00	1.5E+01	10	325	3.06E+03	94%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T04-B	1	2.30E+00	U1/2		2.30E+00	2.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T05-B	1	2.30E+00	U1/2		2.30E+00	5.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T06-B	1	2.30E+00	U1/2		2.30E+00	2.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T07-B	1	2.00E+01			2.00E+01	1.9E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T08-B	1	5.04E+01			5.04E+01	2.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T09-B	1	6.88E+01			6.88E+01	1.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T01-C	1	2.30E+00	U1/2		2.30E+00	9.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T02-C	1	2.30E+00	U1/2		2.30E+00	2.9E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T03-C	1	2.30E+00	U1/2		2.30E+00	6.7E+01	4.6E+00	1.5E+01	10	325	3.13E+03	96%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T04-C	1	2.30E+00	U1/2		2.30E+00	2.7E+01	4.6E+00	1.5E+01					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T05-C	1	2.30E+00	U1/2		2.30E+00	2.2E+01	4.6E+00	1.5E+01					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T06-C	1	3.11E+01			3.11E+01	4.5E+01	4.6E+00	1.5E+01					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T07-C	1	4.88E+00	E		4.88E+00	1.9E+02	4.6E+00	1.5E+01					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T08-C	1	5.31E+01			5.31E+01	1.1E+01	4.6E+00	1.5E+01					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-T09-C	1	8.25E+01			8.25E+01	2.2E+00	4.6E+00	1.5E+01					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	4.7E+01	4.6E+00	1.5E+01					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	1.6E+01	4.6E+00	1.5E+01					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	3.4E+01	4.6E+00	1.5E+01					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-B01-B	1	2.30E+00	U1/2		2.30E+00	2.1E+01	4.6E+00	1.5E+01					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-B02-B	1	2.30E+00	U1/2		2.30E+00	2.0E+01	4.6E+00	1.5E+01					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-B03-B	1	2.30E+00	U1/2		2.30E+00	4.9E+01	4.6E+00	1.5E+01					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-B01-C	1	2.30E+00	U1/2		2.30E+00	2.9E+01	4.6E+00	1.5E+01					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-B02-C	1	2.30E+00	U1/2		2.30E+00	1.4E+01	4.6E+00	1.5E+01					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1313-B03-C	1	2.30E+00	U1/2		2.30E+00	3.1E+01	4.6E+00	1.5E+01					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	EaFA-L05-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	9.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	7.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00	10	325	2.95E+03	91%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	2.0E+02	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	8.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T08-A	1	1.45E+01			1.45E+01	2.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T09-A	1	8.02E+03			8.02E+03	1.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	2.8E+02	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	2.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	6.3E+01	2.0E+00	6.4E+00	10	325	3.02E+03	93%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	4.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T08-B	1	1.49E+01			1.49E+01	4.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T09-B	1	8.31E+03			8.31E+03	4.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	2.8E+02	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	4.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	3.1E+01	2.0E+00	6.4E+00	10	325	3.04E+03	93%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T08-C	1	1.37E+01			1.37E+01	3.5E+00	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-T09-C	1	7.50E+03			7.50E+03	6.7E-01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	3.3E+01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	6.3E+01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-B03-A	1	2.62E+00	E		2.62E+00	4.9E+00	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	6.1E+01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	4.0E+01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	2.8E+00	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	2.9E+01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1313-B03-C	1	1.00E+00	U1/2		1.00E+00	3.9E+01	2.0E+00	6.4E+00					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	EaFA-L05-1313-T01-A	1	3.96E+03			3.96E+03	6.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T02-A	1	2.42E+03			2.42E+03	1.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T03-A	1	2.04E+03			2.04E+03	8.0E-02	1.5E+00	4.8E+00	10	325	5.04E+03	92%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T04-A	1	5.85E+02			5.85E+02	7.1E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T05-A	1	2.53E+02			2.53E+02	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T06-A	1	1.38E+02			1.38E+02	1.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T07-A	1	1.38E+02			1.38E+02	7.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T08-A	1	1.16E+02			1.16E+02	1.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T09-A	1	5.43E+03			5.43E+03	3.4E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T01-B	1	4.30E+03			4.30E+03	9.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T02-B	1	2.43E+03			2.43E+03	6.0E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T03-B	1	2.37E+03			2.37E+03	7.4E-01	1.5E+00	4.8E+00	10	325	5.32E+03	91%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T04-B	1	5.99E+02			5.99E+02	1.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T05-B	1	2.28E+02			2.28E+02	2.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T06-B	1	1.41E+02			1.41E+02	1.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T07-B	1	1.19E+02			1.19E+02	1.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T08-B	1	1.24E+02			1.24E+02	2.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T09-B	1	5.94E+03			5.94E+03	5.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T01-C	1	4.40E+03			4.40E+03	5.4E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T02-C	1	2.62E+03			2.62E+03	6.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T03-C	1	2.45E+03			2.45E+03	3.0E-01	1.5E+00	4.8E+00	10	325	5.47E+03	93%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T04-C	1	5.67E+02			5.67E+02	2.3E+00	1.5E+00	4.8E+00					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T05-C	1	1.93E+02			1.93E+02	1.6E+00	1.5E+00	4.8E+00					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T06-C	1	1.20E+02			1.20E+02	1.1E+01	1.5E+00	4.8E+00					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T07-C	1	1.44E+02			1.44E+02	2.8E+00	1.5E+00	4.8E+00					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T08-C	1	1.09E+02			1.09E+02	1.3E+00	1.5E+00	4.8E+00					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-T09-C	1	5.84E+03			5.84E+03	1.4E-01	1.5E+00	4.8E+00					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-B01-A	1	1.34E+01			1.34E+01	2.9E+00	1.5E+00	4.8E+00					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-B02-A	1	6.31E+00			6.31E+00	2.8E+01	1.5E+00	4.8E+00					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-B03-A	1	1.15E+01			1.15E+01	1.6E+01	1.5E+00	4.8E+00					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-B01-B	1	8.09E+00			8.09E+00	2.1E+01	1.5E+00	4.8E+00					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-B02-B	1	7.51E+00			7.51E+00	2.2E+01	1.5E+00	4.8E+00					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-B03-B	1	1.09E+01			1.09E+01	2.8E+01	1.5E+00	4.8E+00					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-B01-C	1	8.50E+00			8.50E+00	1.3E+01	1.5E+00	4.8E+00					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-B02-C	1	8.07E+00			8.07E+00	9.7E+00	1.5E+00	4.8E+00					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1313-B03-C	1	8.52E+00			8.52E+00	2.7E+01	1.5E+00	4.8E+00					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	EaFA-L05-1313-T01-A	1	1.04E+02			1.04E+02	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 11:56 AM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T02-A	1	5.17E+00			5.17E+00	7.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 11:58 AM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T03-A	1	4.38E+00			4.38E+00	3.3E+00	1.0E+00	3.2E+00	10	325	3.28E+03	101%	VU ICP-OES	7/29/10 1:40 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T04-A	1	5.30E+00			5.30E+00	8.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:01 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T05-A	1	6.74E+00			6.74E+00	7.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:03 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T06-A	1	2.06E+02			2.06E+02	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:04 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T07-A	1	3.81E+02			3.81E+02	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:06 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T08-A	1	1.18E+03			1.18E+03	8.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:08 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T09-A	1	1.55E+03			1.55E+03	9.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:09 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T01-B	1	1.08E+02			1.08E+02	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:21 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T02-B	1	5.10E+00			5.10E+00	1.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:23 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T03-B	1	3.41E+00			3.41E+00	1.1E+01	1.0E+00	3.2E+00	10	325	3.38E+03	104%	VU ICP-OES	7/29/10 12:24 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T04-B	1	1.13E+00	E		1.13E+00	6.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:26 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T05-B	1	5.67E+00			5.67E+00	6.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:27 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T06-B	1	1.37E+02			1.37E+02	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:29 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T07-B	1	6.96E+02			6.96E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:31 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T08-B	1	1.19E+03			1.19E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:32 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T09-B	1	1.57E+03			1.57E+03	6.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:34 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T01-C	1	9.25E+01			9.25E+01	2.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:46 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T02-C	1	6.50E+00			6.50E+00	1.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 12:47 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T03-C	1	1.49E+00	E		1.49E+00	6.3E+01	1.0E+00	3.2E+00	10	325	3.46E+03	106%	VU ICP-OES	7/29/10 12:49 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T04-C	1	3.49E+00			3.49E+00	4.5E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:50 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T05-C	1	1.17E+01			1.17E+01	6.9E-01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:52 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T06-C	1	8.02E+02			8.02E+02	9.8E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:54 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T07-C	1	1.44E+02			1.44E+02	9.0E-01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:55 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T08-C	1	1.20E+03			1.20E+03	7.5E-01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:57 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-T09-C	1	1.56E+03			1.56E+03	6.5E-01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:59 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-B01-A	1	3.86E+00			3.86E+00	1.4E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 11:51 AM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-B02-A	1	1.45E+01			1.45E+01	8.9E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 11:53 AM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-B03-A	1	1.07E+01			1.07E+01	6.6E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 11:55 AM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-B01-B	1	4.01E+00			4.01E+00	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:16 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-B02-B	1	9.40E+00			9.40E+00	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:18 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-B03-B	1	8.00E+00			8.00E+00	3.9E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:19 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-B01-C	1	7.18E+00			7.18E+00	9.2E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:41 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-B02-C	1	8.53E+00			8.53E+00	5.3E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:42 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1313-B03-C	1	1.72E+01			1.72E+01	2.0E+00	1.0E+00	3.2E+00					VU ICP-OES	7/29/10 12:44 PM	EPA Interlab L05 1313-1316 EaFA

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	EaFA-L06-1313-T01-A	1	3.77E+04			3.77E+04	7.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T02-A	1	3.41E+04			3.41E+04	7.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T03-A	1	2.08E+04			2.08E+04	3.8E-01	1.0E+00	3.2E+00	1000	100	2.18E+04	98%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T04-A	1	1.22E+04			1.22E+04	1.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T05-A	1	2.32E+03			2.32E+03	1.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T06-A	1	1.09E+02			1.09E+02	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T07-A	1	1.35E+04			1.35E+04	9.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T08-A	1	5.62E+04			5.62E+04	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T09-A	1	1.14E+05			1.14E+05	3.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T01-B	1	3.30E+04			3.30E+04	2.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T02-B	1	3.86E+04			3.86E+04	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T03-B	1	2.06E+04			2.06E+04	7.7E+00	1.0E+00	3.2E+00	1000	100	2.16E+04	100%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T04-B	1	3.92E+03			3.92E+03	2.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T05-B	1	6.58E+02			6.58E+02	9.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T06-B	1	1.16E+02			1.16E+02	2.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T07-B	1	5.64E+02			5.64E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T08-B	1	2.82E+04			2.82E+04	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T09-B	1	1.16E+05			1.16E+05	6.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T01-C	1	3.90E+04			3.90E+04	2.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T02-C	1	3.44E+04			3.44E+04	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T03-C	1	2.26E+04			2.26E+04	6.2E-01	1.0E+00	3.2E+00	1000	100	2.35E+04	89%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T04-C	1	4.35E+03			4.35E+03	6.4E-01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T05-C	1	6.98E+02			6.98E+02	2.0E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T06-C	1	1.35E+02			1.35E+02	4.8E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T07-C	1	6.15E+02			6.15E+02	6.9E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T08-C	1	2.91E+04			2.91E+04	3.3E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-T09-C	1	1.15E+05			1.15E+05	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	7.1E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	2.4E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	3.9E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	6.8E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	3.6E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	7.4E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	EaFA-L06-1313-T01-A	1	2.69E+02			2.69E+02	8.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T02-A	1	1.52E+02			1.52E+02	1.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T03-A	1	1.92E+02			1.92E+02	1.0E+01	7.5E+00	2.4E+01	10	325	3.33E+03	97%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T04-A	1	2.12E+02			2.12E+02	1.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T05-A	1	2.13E+02			2.13E+02	1.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T06-A	1	1.64E+02			1.64E+02	1.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T07-A	1	1.21E+02			1.21E+02	2.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T08-A	1	2.37E+01	E		2.37E+01	2.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T09-A	1	3.75E+00	U1/2		3.75E+00	8.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T01-B	1	2.71E+02			2.71E+02	3.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T02-B	1	1.38E+02			1.38E+02	1.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T03-B	1	1.71E+02			1.71E+02	1.5E+01	7.5E+00	2.4E+01	10	325	3.43E+03	100%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T04-B	1	1.67E+02			1.67E+02	1.8E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T05-B	1	1.47E+02			1.47E+02	6.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T06-B	1	1.48E+02			1.48E+02	1.6E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T07-B	1	1.16E+02			1.16E+02	2.9E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T08-B	1	2.97E+01			2.97E+01	3.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T09-B	1	3.75E+00	U1/2		3.75E+00	4.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T01-C	1	2.96E+02			2.96E+02	9.9E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T02-C	1	1.24E+02			1.24E+02	1.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T03-C	1	1.76E+02			1.76E+02	2.9E+00	7.5E+00	2.4E+01	10	325	3.26E+03	95%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T04-C	1	1.55E+02			1.55E+02	1.7E+01	7.5E+00	2.4E+01					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T05-C	1	1.63E+02			1.63E+02	3.6E+00	7.5E+00	2.4E+01					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T06-C	1	1.43E+02			1.43E+02	2.7E+01	7.5E+00	2.4E+01					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T07-C	1	1.15E+02			1.15E+02	1.6E+01	7.5E+00	2.4E+01					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T08-C	1	3.75E+00	U1/2		3.75E+00	1.2E+02	7.5E+00	2.4E+01					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-T09-C	1	3.75E+00	U1/2		3.75E+00	2.5E+01	7.5E+00	2.4E+01					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-B01-A	1	2.95E+01			2.95E+01	7.2E+01	7.5E+00	2.4E+01					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-B02-A	1	2.68E+01			2.68E+01	1.2E+02	7.5E+00	2.4E+01					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-B03-A	1	2.41E+01			2.41E+01	5.4E+01	7.5E+00	2.4E+01					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-B01-B	1	1.99E+01	E		1.99E+01	3.1E+01	7.5E+00	2.4E+01					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-B02-B	1	1.11E+01	E		1.11E+01	3.9E+01	7.5E+00	2.4E+01					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1313-B03-B	1	1.47E+01	E		1.47E+01	1.0E+02	7.5E+00	2.4E+01					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	EaFA-L06-1313-T01-A	1	1.42E+04			1.42E+04	8.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T02-A	1	1.42E+03			1.42E+03	1.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T03-A	1	1.24E+03			1.24E+03	1.8E+00	1.1E+01	3.5E+01	10	325	4.38E+03	97%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T04-A	1	1.04E+03			1.04E+03	2.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T05-A	1	4.66E+02			4.66E+02	1.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T06-A	1	4.47E+01			4.47E+01	2.9E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T07-A	1	1.05E+02			1.05E+02	2.7E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T08-A	1	8.85E+01			8.85E+01	1.6E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T09-A	1	2.36E+03			2.36E+03	3.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T01-B	1	1.28E+04			1.28E+04	3.9E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T02-B	1	1.74E+03			1.74E+03	1.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T03-B	1	8.13E+02			8.13E+02	9.1E+00	1.1E+01	3.5E+01	10	325	4.14E+03	102%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T04-B	1	3.38E+02			3.38E+02	6.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T05-B	1	1.48E+02			1.48E+02	6.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T06-B	1	4.46E+01			4.46E+01	2.4E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T07-B	1	6.63E+01			6.63E+01	1.4E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T08-B	1	8.91E+01			8.91E+01	2.2E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T09-B	1	2.12E+03			2.12E+03	7.4E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T01-C	1	1.35E+04			1.35E+04	3.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T02-C	1	1.57E+03			1.57E+03	1.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T03-C	1	8.38E+02			8.38E+02	1.4E+00	1.1E+01	3.5E+01	10	325	3.96E+03	96%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T04-C	1	3.96E+02			3.96E+02	2.0E+00	1.1E+01	3.5E+01					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T05-C	1	1.84E+02			1.84E+02	4.8E+00	1.1E+01	3.5E+01					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T06-C	1	3.63E+01			3.63E+01	5.3E+01	1.1E+01	3.5E+01					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T07-C	1	6.98E+01			6.98E+01	4.0E+01	1.1E+01	3.5E+01					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T08-C	1	9.01E+01			9.01E+01	2.3E+01	1.1E+01	3.5E+01					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-T09-C	1	2.27E+03			2.27E+03	2.1E+01	1.1E+01	3.5E+01					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-B01-A	1	5.50E+00	U1/2		5.50E+00	8.3E+01	1.1E+01	3.5E+01					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-B02-A	1	5.50E+00	U1/2		5.50E+00	2.8E+02	1.1E+01	3.5E+01					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-B03-A	1	5.50E+00	U1/2		5.50E+00	5.1E+02	1.1E+01	3.5E+01					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-B01-B	1	5.50E+00	U1/2		5.50E+00	5.1E+02	1.1E+01	3.5E+01					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-B02-B	1	5.50E+00	U1/2		5.50E+00	2.8E+01	1.1E+01	3.5E+01					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1313-B03-B	1	1.52E+01	E		1.52E+01	2.2E+01	1.1E+01	3.5E+01					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	EaFA-L06-1313-T01-A	1	4.25E+03			4.25E+03	7.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T02-A	1	4.03E+03			4.03E+03	7.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T03-A	1	3.89E+03			3.89E+03	3.7E-01	1.0E+00	3.2E+00	1000	100	4.76E+03	87%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T04-A	1	4.40E+03			4.40E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T05-A	1	4.06E+03			4.06E+03	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T06-A	1	4.39E+03			4.39E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T07-A	1	3.89E+03			3.89E+03	8.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T08-A	1	3.47E+03			3.47E+03	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T09-A	1	2.82E+03			2.82E+03	2.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T01-B	1	4.48E+03			4.48E+03	4.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T02-B	1	4.08E+03			4.08E+03	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T03-B	1	3.79E+03			3.79E+03	6.3E+00	1.0E+00	3.2E+00	1000	100	4.80E+03	100%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T04-B	1	3.83E+03			3.83E+03	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T05-B	1	3.83E+03			3.83E+03	8.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T06-B	1	4.38E+03			4.38E+03	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T07-B	1	4.74E+03			4.74E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T08-B	1	3.64E+03			3.64E+03	2.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T09-B	1	2.80E+03			2.80E+03	5.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T01-C	1	4.66E+03			4.66E+03	2.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T02-C	1	3.76E+03			3.76E+03	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T03-C	1	4.13E+03			4.13E+03	1.3E+00	1.0E+00	3.2E+00	1000	100	5.03E+03	90%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T04-C	1	4.22E+03			4.22E+03	8.6E-01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T05-C	1	4.35E+03			4.35E+03	3.8E-01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T06-C	1	4.56E+03			4.56E+03	6.9E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T07-C	1	4.63E+03			4.63E+03	8.0E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T08-C	1	3.53E+03			3.53E+03	2.5E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-T09-C	1	2.85E+03			2.85E+03	2.5E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-B01-A	1	7.71E+01			7.71E+01	5.5E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-B02-A	1	4.76E+01			4.76E+01	4.5E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-B03-A	1	5.17E+01			5.17E+01	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-B01-B	1	3.81E+01			3.81E+01	3.5E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-B02-B	1	2.44E+01			2.44E+01	3.6E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1313-B03-B	1	2.87E+01			2.87E+01	1.7E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	EaFA-L06-1313-T01-A	1	2.34E+03			2.34E+03	7.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T02-A	1	1.34E+03			1.34E+03	9.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T03-A	1	1.30E+03			1.30E+03	5.2E-01	1.0E+00	3.2E+00	10	325	4.10E+03	86%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T04-A	1	8.26E+02			8.26E+02	3.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T05-A	1	3.89E+02			3.89E+02	2.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T06-A	1	3.07E+02			3.07E+02	8.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T07-A	1	2.85E+02			2.85E+02	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T08-A	1	3.65E+02			3.65E+02	8.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T09-A	1	9.22E+02			9.22E+02	2.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T01-B	1	2.41E+03			2.41E+03	3.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T02-B	1	1.35E+03			1.35E+03	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T03-B	1	7.31E+02			7.31E+02	8.5E+00	1.0E+00	3.2E+00	10	325	3.72E+03	92%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T04-B	1	3.46E+02			3.46E+02	2.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T05-B	1	2.63E+02			2.63E+02	9.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T06-B	1	2.76E+02			2.76E+02	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T07-B	1	3.07E+02			3.07E+02	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T08-B	1	3.08E+02			3.08E+02	2.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T09-B	1	9.07E+02			9.07E+02	7.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T01-C	1	2.40E+03			2.40E+03	3.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T02-C	1	1.26E+03			1.26E+03	5.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T03-C	1	7.20E+02			7.20E+02	6.0E-01	1.0E+00	3.2E+00	10	325	3.53E+03	86%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T04-C	1	3.62E+02			3.62E+02	7.7E-01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T05-C	1	2.99E+02			2.99E+02	3.8E-01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T06-C	1	2.82E+02			2.82E+02	5.6E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T07-C	1	2.88E+02			2.88E+02	7.3E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T08-C	1	3.01E+02			3.01E+02	2.8E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-T09-C	1	9.11E+02			9.11E+02	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	8.6E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	3.7E+02	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-B03-A	1	1.92E+00	E		1.92E+00	6.4E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	1.4E+02	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	1.5E+02	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1313-B03-B	1	2.17E+00	E		2.17E+00	1.6E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	EaFA-L06-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	2.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	9.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	1.8E+02	1.9E+00	6.0E+00	10	325	3.19E+03	98%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	1.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	7.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	1.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T07-A	1	8.66E+01			8.66E+01	7.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T08-A	1	1.72E+02			1.72E+02	1.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T09-A	1	2.47E+02			2.47E+02	2.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	4.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	2.7E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	4.8E+01	1.9E+00	6.0E+00	10	325	3.32E+03	102%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	5.6E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	6.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T07-B	1	5.98E+00	E		5.98E+00	3.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T08-B	1	1.21E+02			1.21E+02	3.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T09-B	1	2.39E+02			2.39E+02	7.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	1.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	2.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	2.2E+02	1.9E+00	6.0E+00	10	325	3.17E+03	98%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	1.6E+02	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	1.8E+02	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	2.1E+02	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T07-C	1	6.09E+00			6.09E+00	1.0E+01	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T08-C	1	1.20E+02			1.20E+02	2.6E+00	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-T09-C	1	2.41E+02			2.41E+02	4.3E+01	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	2.9E+02	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	8.6E+01	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-B01-B	1	9.50E-01	U1/2		9.50E-01	1.2E+03	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-B02-B	1	9.50E-01	U1/2		9.50E-01	4.3E+02	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1313-B03-B	1	9.50E-01	U1/2		9.50E-01	6.8E+02	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	EaFA-L06-1313-T01-A	1	1.10E+00	U1/2		1.10E+00	4.6E+01	2.2E+00	7.0E+00			---		VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T02-A	1	1.10E+00	U1/2		1.10E+00	3.6E+00	2.2E+00	7.0E+00			---		VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	3.7E+01	2.2E+00	7.0E+00	10	325	3.22E+03	99%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T04-A	1	1.10E+00	U1/2		1.10E+00	5.2E+00	2.2E+00	7.0E+00			---		VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T05-A	1	1.10E+00	U1/2		1.10E+00	2.3E+01	2.2E+00	7.0E+00			---		VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T06-A	1	1.10E+00	U1/2		1.10E+00	6.6E+01	2.2E+00	7.0E+00			---		VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T07-A	1	2.94E+01			2.94E+01	9.5E-01	2.2E+00	7.0E+00			---		VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T08-A	1	2.61E+01			2.61E+01	1.4E+00	2.2E+00	7.0E+00			---		VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T09-A	1	3.09E+01			3.09E+01	2.5E+00	2.2E+00	7.0E+00			---		VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T01-B	1	1.10E+00	U1/2		1.10E+00	3.4E+01	2.2E+00	7.0E+00			---		VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T02-B	1	1.10E+00	U1/2		1.10E+00	1.8E+01	2.2E+00	7.0E+00			---		VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	2.4E+01	2.2E+00	7.0E+00	10	325	3.34E+03	103%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T04-B	1	1.10E+00	U1/2		1.10E+00	1.9E+01	2.2E+00	7.0E+00			---		VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T05-B	1	1.10E+00	U1/2		1.10E+00	1.5E+01	2.2E+00	7.0E+00			---		VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T06-B	1	1.10E+00	U1/2		1.10E+00	7.8E+02	2.2E+00	7.0E+00			---		VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T07-B	1	3.37E+01			3.37E+01	1.6E+00	2.2E+00	7.0E+00			---		VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T08-B	1	2.81E+01			2.81E+01	9.6E-01	2.2E+00	7.0E+00			---		VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T09-B	1	3.04E+01			3.04E+01	8.4E+01	2.2E+00	7.0E+00			---		VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T01-C	1	1.10E+00	U1/2		1.10E+00	2.8E+01	2.2E+00	7.0E+00			---		VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T02-C	1	1.10E+00	U1/2		1.10E+00	3.1E+01	2.2E+00	7.0E+00			---		VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	1.4E+01	2.2E+00	7.0E+00	10	325	3.20E+03	99%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T04-C	1	1.10E+00	U1/2		1.10E+00	2.3E+01	2.2E+00	7.0E+00					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T05-C	1	1.10E+00	U1/2		1.10E+00	1.6E+01	2.2E+00	7.0E+00					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T06-C	1	1.10E+00	U1/2		1.10E+00	1.5E+02	2.2E+00	7.0E+00					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T07-C	1	3.13E+01			3.13E+01	8.4E+00	2.2E+00	7.0E+00					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T08-C	1	2.74E+01			2.74E+01	1.7E+00	2.2E+00	7.0E+00					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-T09-C	1	3.10E+01			3.10E+01	4.0E+01	2.2E+00	7.0E+00					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	2.9E+01	2.2E+00	7.0E+00					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	1.6E+01	2.2E+00	7.0E+00					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-B03-A	1	1.10E+00	U1/2		1.10E+00	8.9E+01	2.2E+00	7.0E+00					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-B01-B	1	1.10E+00	U1/2		1.10E+00	2.0E+01	2.2E+00	7.0E+00					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-B02-B	1	1.10E+00	U1/2		1.10E+00	1.2E+01	2.2E+00	7.0E+00					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1313-B03-B	1	1.10E+00	U1/2		1.10E+00	4.4E+01	2.2E+00	7.0E+00					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	EaFA-L06-1313-T01-A	1	1.17E+04			1.17E+04	8.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T02-A	1	4.11E+04			4.11E+04	7.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T03-A	1	8.05E+04			8.05E+04	2.9E-01	2.6E+00	8.3E+00	1000	100	8.14E+04	89%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T04-A	1	1.19E+05			1.19E+05	6.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T05-A	1	1.35E+05			1.35E+05	7.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T06-A	1	1.62E+05			1.62E+05	1.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T07-A	1	1.45E+05			1.45E+05	8.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T08-A	1	1.49E+05			1.49E+05	5.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T09-A	1	1.36E+05			1.36E+05	2.6E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T01-B	1	1.24E+04			1.24E+04	2.7E+01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T02-B	1	3.84E+04			3.84E+04	5.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T03-B	1	9.62E+04			9.62E+04	8.7E+00	2.6E+00	8.3E+00	1000	100	9.72E+04	92%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T04-B	1	1.23E+05			1.23E+05	2.7E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T05-B	1	1.31E+05			1.31E+05	8.9E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T06-B	1	1.58E+05			1.58E+05	1.8E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T07-B	1	1.72E+05			1.72E+05	1.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T08-B	1	1.41E+05			1.41E+05	3.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T09-B	1	1.35E+05			1.35E+05	7.1E+01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T01-C	1	1.27E+04			1.27E+04	3.5E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T02-C	1	3.46E+04			3.46E+04	3.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T03-C	1	1.03E+05			1.03E+05	1.1E+00	2.6E+00	8.3E+00	1000	100	1.04E+05	95%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T04-C	1	1.27E+05			1.27E+05	3.3E-01	2.6E+00	8.3E+00					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T05-C	1	1.49E+05			1.49E+05	8.6E-01	2.6E+00	8.3E+00					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T06-C	1	1.65E+05			1.65E+05	6.1E+00	2.6E+00	8.3E+00					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T07-C	1	1.64E+05			1.64E+05	7.3E+00	2.6E+00	8.3E+00					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T08-C	1	1.38E+05			1.38E+05	2.7E+00	2.6E+00	8.3E+00					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-T09-C	1	1.36E+05			1.36E+05	1.2E+01	2.6E+00	8.3E+00					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-B01-A	1	1.86E+01			1.86E+01	3.0E+01	2.6E+00	8.3E+00					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-B02-A	1	1.83E+01			1.83E+01	4.2E+01	2.6E+00	8.3E+00					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-B03-A	1	6.85E+01			6.85E+01	2.7E+01	2.6E+00	8.3E+00					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-B01-B	1	1.82E+01			1.82E+01	1.7E+01	2.6E+00	8.3E+00					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-B02-B	1	2.17E+01			2.17E+01	3.6E+01	2.6E+00	8.3E+00					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1313-B03-B	1	7.38E+01			7.38E+01	5.9E+01	2.6E+00	8.3E+00					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	EaFA-L06-1313-T01-A	1	6.39E+02			6.39E+02	8.9E+00	1.2E+00	3.8E+00			---		VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T02-A	1	3.83E+02			3.83E+02	8.4E-01	1.2E+00	3.8E+00			---		VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T03-A	1	2.96E+02			2.96E+02	3.9E-01	1.2E+00	3.8E+00	10	325	3.40E+03	96%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T04-A	1	2.31E+02			2.31E+02	6.9E-01	1.2E+00	3.8E+00			---		VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T05-A	1	1.34E+02			1.34E+02	3.1E-01	1.2E+00	3.8E+00			---		VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T06-A	1	1.74E+01			1.74E+01	2.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T07-A	1	4.99E+01			4.99E+01	9.8E-01	1.2E+00	3.8E+00			---		VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T08-A	1	7.84E+02			7.84E+02	1.2E+00	1.2E+00	3.8E+00			---		VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T09-A	1	1.72E+03			1.72E+03	2.8E+00	1.2E+00	3.8E+00			---		VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T01-B	1	6.12E+02			6.12E+02	1.8E+01	1.2E+00	3.8E+00			---		VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T02-B	1	4.26E+02			4.26E+02	2.9E-01	1.2E+00	3.8E+00			---		VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T03-B	1	2.80E+02			2.80E+02	8.7E+00	1.2E+00	3.8E+00	10	325	3.47E+03	98%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T04-B	1	2.08E+02			2.08E+02	3.2E+00	1.2E+00	3.8E+00			---		VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T05-B	1	8.97E+01			8.97E+01	9.8E+00	1.2E+00	3.8E+00			---		VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T06-B	1	1.63E+01			1.63E+01	5.7E+00	1.2E+00	3.8E+00			---		VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T07-B	1	1.28E+00	E		1.28E+00	1.5E+02	1.2E+00	3.8E+00			---		VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T08-B	1	1.64E+02			1.64E+02	2.9E+00	1.2E+00	3.8E+00			---		VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T09-B	1	1.68E+03			1.68E+03	5.3E+01	1.2E+00	3.8E+00			---		VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T01-C	1	6.15E+02			6.15E+02	2.6E+00	1.2E+00	3.8E+00			---		VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T02-C	1	3.80E+02			3.80E+02	3.4E-01	1.2E+00	3.8E+00			---		VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T03-C	1	2.91E+02			2.91E+02	1.1E+00	1.2E+00	3.8E+00	10	325	3.35E+03	94%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T04-C	1	2.01E+02			2.01E+02	2.2E-01	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T05-C	1	1.07E+02			1.07E+02	1.4E+00	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T06-C	1	2.41E+01			2.41E+01	7.6E+00	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T07-C	1	6.00E-01	U1/2		6.00E-01	2.9E+02	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T08-C	1	1.78E+02			1.78E+02	2.1E+00	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-T09-C	1	1.69E+03			1.69E+03	1.3E+01	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	1.0E+02	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	3.0E+02	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-B03-A	1	6.86E+00			6.86E+00	3.6E+01	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-B01-B	1	6.00E-01	U1/2		6.00E-01	1.6E+03	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-B02-B	1	6.00E-01	U1/2		6.00E-01	2.0E+02	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1313-B03-B	1	6.83E+00			6.83E+00	6.5E+00	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	EaFA-L06-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	3.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	6.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	4.8E+01	1.8E+00	5.7E+00	10	325	3.13E+03	96%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	4.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T05-A	1	9.00E-01	U1/2		9.00E-01	1.8E+03	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T06-A	1	6.99E+01			6.99E+01	2.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T07-A	1	1.95E+02			1.95E+02	3.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T08-A	1	2.26E+02			2.26E+02	1.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T09-A	1	4.02E+02			4.02E+02	3.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	7.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	1.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	2.0E+01	1.8E+00	5.7E+00	10	325	3.22E+03	99%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	9.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T05-B	1	2.65E+00	E		2.65E+00	1.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T06-B	1	6.56E+01			6.56E+01	4.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T07-B	1	2.47E+02			2.47E+02	1.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T08-B	1	1.99E+02			1.99E+02	3.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T09-B	1	4.00E+02			4.00E+02	7.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	4.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	3.5E+01	1.8E+00	5.7E+00	10	325	3.11E+03	96%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	5.7E+01	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T05-C	1	4.45E+00	E		4.45E+00	5.5E+00	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T06-C	1	5.89E+01			5.89E+01	8.9E+00	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T07-C	1	2.36E+02			2.36E+02	6.8E+00	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T08-C	1	1.97E+02			1.97E+02	2.4E+00	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-T09-C	1	4.01E+02			4.01E+02	8.7E+00	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	8.2E+01	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	2.4E+01	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	3.1E+02	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-B01-B	1	9.00E-01	U1/2		9.00E-01	3.8E+01	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-B02-B	1	9.00E-01	U1/2		9.00E-01	2.1E+01	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1313-B03-B	1	9.00E-01	U1/2		9.00E-01	6.0E+01	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	EaFA-L06-1313-T01-A	1	8.34E+01			8.34E+01	9.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T02-A	1	4.05E+00	E		4.05E+00	2.7E+02	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T03-A	1	5.02E+00	E		5.02E+00	1.3E+02	3.7E+00	1.2E+01	10	325	3.06E+03	94%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T04-A	1	5.46E+00	E		5.46E+00	2.9E+04	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T05-A	1	1.85E+00	U1/2		1.85E+00	1.4E+02	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T06-A	1	1.85E+00	U1/2		1.85E+00	2.9E+02	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T07-A	1	1.67E+03			1.67E+03	1.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T08-A	1	2.34E+03			2.34E+03	1.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T09-A	1	2.90E+03			2.90E+03	3.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T01-B	1	7.01E+01			7.01E+01	2.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T02-B	1	2.00E+01			2.00E+01	6.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T03-B	1	1.85E+00	U1/2		1.85E+00	1.1E+02	3.7E+00	1.2E+01	10	325	3.18E+03	98%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T04-B	1	5.63E+00	E		5.63E+00	2.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T05-B	1	1.85E+00	U1/2		1.85E+00	3.9E+02	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T06-B	1	8.09E+00	E		8.09E+00	1.3E+02	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T07-B	1	1.35E+02			1.35E+02	4.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T08-B	1	1.94E+03			1.94E+03	1.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T09-B	1	2.89E+03			2.89E+03	4.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T01-C	1	9.20E+01			9.20E+01	4.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T02-C	1	1.85E+00	U1/2		1.85E+00	9.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T03-C	1	1.85E+00	U1/2		1.85E+00	3.0E+01	3.7E+00	1.2E+01	10	325	3.07E+03	94%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T04-C	1	1.85E+00	U1/2		1.85E+00	3.2E+02	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T05-C	1	4.82E+00	E		4.82E+00	1.1E+02	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T06-C	1	7.66E+00	E		7.66E+00	5.2E+01	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T07-C	1	1.39E+02			1.39E+02	6.7E+00	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T08-C	1	1.92E+03			1.92E+03	4.5E+00	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-T09-C	1	2.91E+03			2.91E+03	4.4E+01	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	8.5E+01	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	1.4E+02	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-B03-A	1	1.85E+00	U1/2		1.85E+00	6.2E+01	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-B01-B	1	1.85E+00	U1/2		1.85E+00	9.1E+02	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-B02-B	1	1.85E+00	U1/2		1.85E+00	2.7E+02	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1313-B03-B	1	1.85E+00	U1/2		1.85E+00	3.1E+02	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	EaFA-L06-1313-T01-A	1	2.29E+01			2.29E+01	1.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T02-A	1	2.54E+01			2.54E+01	2.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T03-A	1	8.76E+00			8.76E+00	3.6E+00	2.0E+00	6.4E+00	1000	100	9.86E+02	98%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T04-A	1	2.43E+00	E		2.43E+00	1.9E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T06-A	1	3.46E+01			3.46E+01	8.6E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T07-A	1	1.80E+02			1.80E+02	2.9E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T08-A	1	2.40E+03			2.40E+03	4.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T09-A	1	3.56E+04			3.56E+04	2.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T01-B	1	2.30E+01			2.30E+01	2.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T02-B	1	2.66E+01			2.66E+01	1.9E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	3.9E+01	2.0E+00	6.4E+00	1000	100	1.01E+03	101%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	1.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	7.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	3.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	5.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T08-B	1	4.50E+02			4.50E+02	1.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T09-B	1	3.53E+04			3.53E+04	6.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T01-C	1	2.54E+01			2.54E+01	6.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T02-C	1	2.10E+01			2.10E+01	2.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	2.9E+01	2.0E+00	6.4E+00	1000	100	9.73E+02	97%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	5.7E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	7.8E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	6.0E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	4.7E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T08-C	1	4.61E+02			4.61E+02	4.3E+00	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-T09-C	1	3.55E+04			3.55E+04	3.7E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	2.1E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	3.8E+02	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-B03-A	1	1.52E+01			1.52E+01	9.8E+00	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	8.5E+00	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	5.6E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1313-B03-B	1	1.42E+01			1.42E+01	1.2E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	EaFA-L06-1313-T01-A	1	1.55E+01	E		1.55E+01	8.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T02-A	1	3.40E+00	U1/2		3.40E+00	5.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T03-A	1	3.40E+00	U1/2		3.40E+00	6.5E+01	6.8E+00	2.2E+01	10	325	3.10E+03	95%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T04-A	1	3.40E+00	U1/2		3.40E+00	3.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T05-A	1	3.40E+00	U1/2		3.40E+00	8.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T06-A	1	3.40E+00	U1/2		3.40E+00	2.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T07-A	1	3.40E+00	U1/2		3.40E+00	2.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T08-A	1	3.40E+00	U1/2		3.40E+00	2.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T09-A	1	9.17E+01			9.17E+01	4.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T01-B	1	3.40E+00	U1/2		3.40E+00	1.0E+03	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T02-B	1	3.40E+00	U1/2		3.40E+00	1.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T03-B	1	3.40E+00	U1/2		3.40E+00	6.5E+01	6.8E+00	2.2E+01	10	325	3.21E+03	99%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T04-B	1	3.40E+00	U1/2		3.40E+00	5.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T05-B	1	3.40E+00	U1/2		3.40E+00	1.7E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T06-B	1	3.40E+00	U1/2		3.40E+00	1.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T07-B	1	3.40E+00	U1/2		3.40E+00	5.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T08-B	1	3.40E+00	U1/2		3.40E+00	3.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T09-B	1	9.52E+01			9.52E+01	1.1E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T01-C	1	3.40E+00	U1/2		3.40E+00	2.8E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T02-C	1	3.40E+00	U1/2		3.40E+00	3.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T03-C	1	3.40E+00	U1/2		3.40E+00	2.8E+01	6.8E+00	2.2E+01	10	325	3.09E+03	95%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T04-C	1	3.40E+00	U1/2		3.40E+00	3.3E+01	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T05-C	1	3.40E+00	U1/2		3.40E+00	8.6E+01	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T06-C	1	3.40E+00	U1/2		3.40E+00	3.9E+01	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T07-C	1	3.40E+00	U1/2		3.40E+00	1.8E+01	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T08-C	1	3.40E+00	U1/2		3.40E+00	2.5E+01	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-T09-C	1	1.01E+02			1.01E+02	1.1E+01	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	5.1E+01	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	2.7E+01	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	6.3E+01	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-B01-B	1	3.40E+00	U1/2		3.40E+00	5.5E+01	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-B02-B	1	3.40E+00	U1/2		3.40E+00	4.2E+01	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1313-B03-B	1	3.40E+00	U1/2		3.40E+00	3.3E+01	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	EaFA-L06-1313-T01-A	1	2.51E+03			2.51E+03	7.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T02-A	1	2.93E+03			2.93E+03	7.9E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T03-A	1	3.27E+03			3.27E+03	6.3E-01	1.9E+00	6.0E+00	10	325	6.00E+03	84%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T04-A	1	3.49E+03			3.49E+03	3.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T05-A	1	3.55E+03			3.55E+03	4.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T06-A	1	3.86E+03			3.86E+03	9.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T07-A	1	2.77E+03			2.77E+03	7.9E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T08-A	1	2.14E+03			2.14E+03	6.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T09-A	1	1.58E+03			1.58E+03	2.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T01-B	1	2.36E+03			2.36E+03	4.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T02-B	1	2.96E+03			2.96E+03	7.6E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T03-B	1	3.21E+03			3.21E+03	8.6E+00	1.9E+00	6.0E+00	10	325	6.24E+03	93%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T04-B	1	3.32E+03			3.32E+03	3.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T05-B	1	3.33E+03			3.33E+03	1.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T06-B	1	3.75E+03			3.75E+03	2.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T07-B	1	3.81E+03			3.81E+03	5.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T08-B	1	2.42E+03			2.42E+03	3.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T09-B	1	1.54E+03			1.54E+03	7.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T01-C	1	2.49E+03			2.49E+03	2.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T02-C	1	2.64E+03			2.64E+03	4.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T03-C	1	3.42E+03			3.42E+03	9.0E-01	1.9E+00	6.0E+00	10	325	6.15E+03	84%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T04-C	1	3.48E+03			3.48E+03	6.2E-01	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T05-C	1	3.79E+03			3.79E+03	2.3E-01	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T06-C	1	3.94E+03			3.94E+03	5.7E+00	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T07-C	1	3.68E+03			3.68E+03	7.6E+00	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T08-C	1	2.35E+03			2.35E+03	2.5E+00	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-T09-C	1	1.58E+03			1.58E+03	1.6E+01	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-B01-A	1	2.55E+00	E		2.55E+00	3.4E+01	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	1.0E+02	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	2.3E+02	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-B01-B	1	2.31E+00	E		2.31E+00	2.5E+01	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-B02-B	1	9.50E-01	U1/2		9.50E-01	4.4E+01	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1313-B03-B	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	EaFA-L06-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	2.6E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	8.2E+01	2.0E+00	6.4E+00	10	325	3.01E+03	93%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	6.6E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T05-A	1	1.21E+01			1.21E+01	8.5E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T06-A	1	4.30E+02			4.30E+02	6.3E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T07-A	1	8.96E+02			8.96E+02	7.9E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T08-A	1	1.21E+03			1.21E+03	7.0E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T09-A	1	1.57E+03			1.57E+03	2.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	2.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	3.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	1.6E+02	2.0E+00	6.4E+00	10	325	3.12E+03	96%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T04-B	1	4.70E+00	E		4.70E+00	5.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T05-B	1	6.26E+01			6.26E+01	7.5E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T06-B	1	4.31E+02			4.31E+02	1.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T07-B	1	8.70E+02			8.70E+02	8.2E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T08-B	1	1.02E+03			1.02E+03	2.5E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T09-B	1	1.55E+03			1.55E+03	7.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	4.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	8.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	1.5E+02	2.0E+00	6.4E+00	10	325	2.99E+03	92%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T04-C	1	4.30E+00	E		4.30E+00	2.9E+00	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T05-C	1	7.33E+01			7.33E+01	7.3E-01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T06-C	1	3.94E+02			3.94E+02	5.6E+00	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T07-C	1	8.29E+02			8.29E+02	5.1E+00	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T08-C	1	1.01E+03			1.01E+03	2.5E+00	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-T09-C	1	1.56E+03			1.56E+03	1.3E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	5.3E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	6.4E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	6.2E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	3.3E+02	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	EaFA-L06-1313-T01-A	1	5.00E-01	U1/2		5.00E-01	1.8E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T02-A	1	5.00E-01	U1/2		5.00E-01	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T03-A	1	5.73E+01			5.73E+01	3.0E+01	1.0E+00	3.2E+00	1000	100	1.07E+03	101%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T04-A	1	2.69E+03			2.69E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T05-A	1	4.07E+03			4.07E+03	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T06-A	1	7.86E+03			7.86E+03	6.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T07-A	1	7.52E+03			7.52E+03	5.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T08-A	1	9.47E+03			9.47E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T09-A	1	1.42E+04			1.42E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T01-B	1	5.00E-01	U1/2		5.00E-01	3.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T02-B	1	4.66E+00			4.66E+00	2.6E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T03-B	1	1.65E+03			1.65E+03	8.9E+00	1.0E+00	3.2E+00	1000	100	2.64E+03	99%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T04-B	1	3.82E+03			3.82E+03	3.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T05-B	1	5.62E+03			5.62E+03	9.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T06-B	1	7.93E+03			7.93E+03	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T07-B	1	9.25E+03			9.25E+03	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T08-B	1	7.73E+03			7.73E+03	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T09-B	1	1.40E+04			1.40E+04	6.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T01-C	1	5.00E-01	U1/2		5.00E-01	1.2E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T02-C	1	5.00E-01	U1/2		5.00E-01	1.0E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T03-C	1	1.72E+03			1.72E+03	7.9E-01	1.0E+00	3.2E+00	1000	100	2.53E+03	81%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T04-C	1	3.93E+03			3.93E+03	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T05-C	1	6.47E+03			6.47E+03	2.5E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T06-C	1	8.43E+03			8.43E+03	4.5E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T07-C	1	8.71E+03			8.71E+03	6.1E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T08-C	1	7.70E+03			7.70E+03	2.5E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-T09-C	1	1.43E+04			1.43E+04	1.9E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	7.1E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	5.4E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	1.5E+02	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	2.0E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	3.6E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1313-B03-B	1	2.24E+00	E		2.24E+00	3.9E+02	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	EaFA-L06-1313-T01-A	1	4.39E+03			4.39E+03	8.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T02-A	1	3.98E+03			3.98E+03	4.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T03-A	1	3.99E+03			3.99E+03	6.6E-01	1.2E+00	3.8E+00	10	325	6.92E+03	90%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T04-A	1	4.02E+03			4.02E+03	4.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T05-A	1	3.72E+03			3.72E+03	9.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T06-A	1	3.09E+03			3.09E+03	8.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T07-A	1	1.29E+02			1.29E+02	1.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T08-A	1	9.65E+01			9.65E+01	2.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T09-A	1	4.17E+02			4.17E+02	2.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T01-B	1	3.92E+03			3.92E+03	1.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T02-B	1	4.03E+03			4.03E+03	9.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T03-B	1	3.56E+03			3.56E+03	7.9E+00	1.2E+00	3.8E+00	10	325	6.81E+03	100%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T04-B	1	3.44E+03			3.44E+03	1.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T05-B	1	3.16E+03			3.16E+03	7.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T06-B	1	3.01E+03			3.01E+03	5.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T07-B	1	4.85E+02			4.85E+02	1.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T08-B	1	1.20E+02			1.20E+02	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T09-B	1	3.91E+02			3.91E+02	7.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T01-C	1	4.40E+03			4.40E+03	2.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T02-C	1	3.59E+03			3.59E+03	1.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T03-C	1	3.83E+03			3.83E+03	1.2E+00	1.2E+00	3.8E+00	10	325	6.54E+03	83%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T04-C	1	3.65E+03			3.65E+03	6.8E-01	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T05-C	1	3.62E+03			3.62E+03	1.3E+00	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T06-C	1	3.05E+03			3.05E+03	5.5E+00	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T07-C	1	4.74E+02			4.74E+02	7.9E+00	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T08-C	1	1.20E+02			1.20E+02	4.6E+00	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-T09-C	1	4.00E+02			4.00E+02	1.7E+01	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-B01-A	1	1.94E+00	E		1.94E+00	1.3E+02	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-B02-A	1	3.48E+00	E		3.48E+00	4.7E+01	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-B03-A	1	9.21E+00			9.21E+00	1.1E+01	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-B01-B	1	2.71E+00	E		2.71E+00	1.1E+02	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-B02-B	1	6.00E-01	U1/2		6.00E-01	6.8E+02	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1313-B03-B	1	1.25E+01			1.25E+01	2.4E+01	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	EaFA-L06-1313-T01-A	1	5.73E+00			5.73E+00	5.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	3.9E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T03-A	1	6.00E+00			6.00E+00	1.0E+02	1.8E+00	5.7E+00	10	325	3.18E+03	98%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	2.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T05-A	1	5.76E+00			5.76E+00	5.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T06-A	1	1.58E+02			1.58E+02	2.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T07-A	1	5.08E+02			5.08E+02	1.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T08-A	1	5.28E+02			5.28E+02	6.3E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T09-A	1	7.27E+02			7.27E+02	2.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T01-B	1	4.37E+00	E		4.37E+00	1.2E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T02-B	1	5.45E+00	E		5.45E+00	7.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T03-B	1	4.17E+00	E		4.17E+00	1.0E+02	1.8E+00	5.7E+00	10	325	3.26E+03	100%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T04-B	1	4.87E+00	E		4.87E+00	9.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T05-B	1	1.84E+01			1.84E+01	2.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T06-B	1	1.50E+02			1.50E+02	2.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T07-B	1	6.18E+02			6.18E+02	1.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T08-B	1	5.10E+02			5.10E+02	3.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T09-B	1	7.14E+02			7.14E+02	7.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T01-C	1	5.13E+00	E		5.13E+00	1.2E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	9.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T03-C	1	3.46E+00	E		3.46E+00	7.6E+01	1.8E+00	5.7E+00	10	325	3.16E+03	97%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	4.8E+02	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T05-C	1	2.27E+01			2.27E+01	2.0E+01	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T06-C	1	1.41E+02			1.41E+02	4.8E+00	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T07-C	1	5.91E+02			5.91E+02	7.5E+00	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T08-C	1	5.01E+02			5.01E+02	2.7E+00	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-T09-C	1	7.16E+02			7.16E+02	1.1E+01	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	1.9E+02	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	5.2E+01	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-B03-A	1	2.59E+00	E		2.59E+00	1.7E+02	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-B01-B	1	2.75E+00	E		2.75E+00	7.5E+01	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-B02-B	1	9.00E-01	U1/2		9.00E-01	2.0E+02	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1313-B03-B	1	3.24E+00	E		3.24E+00	1.1E+02	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	EaFA-L06-1313-T01-A	1	2.30E+02			2.30E+02	7.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T02-A	1	8.23E+01			8.23E+01	4.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T03-A	1	8.83E+01			8.83E+01	7.6E+00	3.7E+00	1.2E+01	1000	100	1.05E+03	96%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T04-A	1	1.92E+02			1.92E+02	2.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T05-A	1	1.13E+02			1.13E+02	4.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T06-A	1	7.16E+01			7.16E+01	9.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T07-A	1	6.83E+01			6.83E+01	5.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T08-A	1	8.93E+01			8.93E+01	1.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T09-A	1	3.01E+03			3.01E+03	2.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T01-B	1	1.74E+02			1.74E+02	2.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T02-B	1	6.36E+01			6.36E+01	4.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T03-B	1	1.01E+02			1.01E+02	1.2E+01	3.7E+00	1.2E+01	1000	100	1.11E+03	101%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T04-B	1	9.32E+01			9.32E+01	6.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T05-B	1	7.91E+01			7.91E+01	3.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T06-B	1	6.45E+01			6.45E+01	9.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T07-B	1	5.32E+01			5.32E+01	4.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T08-B	1	9.21E+01			9.21E+01	8.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T09-B	1	2.80E+03			2.80E+03	7.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T01-C	1	2.43E+02			2.43E+02	5.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T02-C	1	5.57E+01			5.57E+01	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T03-C	1	1.01E+02			1.01E+02	9.8E+00	3.7E+00	1.2E+01	1000	100	1.08E+03	98%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T04-C	1	9.32E+01			9.32E+01	7.7E-01	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T05-C	1	7.27E+01			7.27E+01	9.1E+00	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T06-C	1	6.94E+01			6.94E+01	1.2E+01	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T07-C	1	5.82E+01			5.82E+01	1.2E+01	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T08-C	1	8.02E+01			8.02E+01	7.7E+00	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-T09-C	1	2.97E+03			2.97E+03	1.3E+01	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-B01-A	1	3.68E+01			3.68E+01	6.4E+00	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-B02-A	1	4.13E+01			4.13E+01	1.3E+01	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-B03-A	1	5.18E+01			5.18E+01	1.3E+01	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-B01-B	1	4.76E+01			4.76E+01	7.1E+00	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-B02-B	1	3.72E+01			3.72E+01	2.7E+00	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1313-B03-B	1	5.23E+01			5.23E+01	2.0E+01	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	EaFA-L06-1313-T01-A	1	6.37E+04			6.37E+04	7.9E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T02-A	1	3.76E+04			3.76E+04	8.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T03-A	1	2.82E+04			2.82E+04	5.5E-01	1.6E+00	5.1E+00	1000	100	2.91E+04	85%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T04-A	1	2.75E+04			2.75E+04	3.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T05-A	1	2.62E+04			2.62E+04	8.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T06-A	1	2.69E+04			2.69E+04	9.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T07-A	1	2.12E+04			2.12E+04	6.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T08-A	1	1.86E+04			1.86E+04	9.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T09-A	1	2.23E+04			2.23E+04	3.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T01-B	1	5.90E+04			5.90E+04	3.9E+01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T02-B	1	3.92E+04			3.92E+04	1.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T03-B	1	2.64E+04			2.64E+04	9.6E+00	1.6E+00	5.1E+00	1000	100	2.73E+04	96%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T04-B	1	2.55E+04			2.55E+04	2.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T05-B	1	2.41E+04			2.41E+04	1.1E+01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T06-B	1	2.64E+04			2.64E+04	2.4E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T07-B	1	2.80E+04			2.80E+04	4.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T08-B	1	1.94E+04			1.94E+04	3.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T09-B	1	2.26E+04			2.26E+04	7.5E+01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T01-C	1	6.20E+04			6.20E+04	2.4E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T02-C	1	3.51E+04			3.51E+04	5.4E-02	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T03-C	1	2.84E+04			2.84E+04	7.3E-01	1.6E+00	5.1E+00	1000	100	2.92E+04	83%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T04-C	1	2.70E+04			2.70E+04	7.0E-01	1.6E+00	5.1E+00					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T05-C	1	2.75E+04			2.75E+04	4.6E-01	1.6E+00	5.1E+00					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T06-C	1	2.78E+04			2.78E+04	5.4E+00	1.6E+00	5.1E+00					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T07-C	1	2.67E+04			2.67E+04	8.1E+00	1.6E+00	5.1E+00					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T08-C	1	1.91E+04			1.91E+04	2.7E+00	1.6E+00	5.1E+00					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-T09-C	1	2.25E+04			2.25E+04	1.3E+01	1.6E+00	5.1E+00					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-B01-A	1	2.74E+01			2.74E+01	5.7E+00	1.6E+00	5.1E+00					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-B02-A	1	1.25E+01			1.25E+01	1.2E+01	1.6E+00	5.1E+00					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-B03-A	1	4.03E+02			4.03E+02	8.1E+00	1.6E+00	5.1E+00					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-B01-B	1	1.38E+01			1.38E+01	2.1E+01	1.6E+00	5.1E+00					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-B02-B	1	1.50E+01			1.50E+01	1.2E+01	1.6E+00	5.1E+00					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1313-B03-B	1	3.48E+02			3.48E+02	8.3E+00	1.6E+00	5.1E+00					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	EaFA-L06-1313-T01-A	1	7.68E+03			7.68E+03	8.3E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T02-A	1	6.07E+03			6.07E+03	1.2E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T03-A	1	5.01E+03			5.01E+03	8.9E-01	1.5E+01	4.8E+01	10	325	7.75E+03	84%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T04-A	1	4.23E+03			4.23E+03	2.7E-01	1.5E+01	4.8E+01			---		VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T05-A	1	2.76E+03			2.76E+03	1.9E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T06-A	1	9.36E+02			9.36E+02	2.6E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T07-A	1	1.35E+02			1.35E+02	1.3E+01	1.5E+01	4.8E+01			---		VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T08-A	1	6.99E+01			6.99E+01	2.1E+01	1.5E+01	4.8E+01			---		VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T09-A	1	8.22E+02			8.22E+02	3.0E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T01-B	1	7.18E+03			7.18E+03	3.5E+01	1.5E+01	4.8E+01			---		VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T02-B	1	6.40E+03			6.40E+03	1.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T03-B	1	4.49E+03			4.49E+03	9.3E+00	1.5E+01	4.8E+01	10	325	7.68E+03	98%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T04-B	1	2.59E+03			2.59E+03	3.6E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T05-B	1	1.45E+03			1.45E+03	1.0E+01	1.5E+01	4.8E+01			---		VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T06-B	1	8.54E+02			8.54E+02	4.9E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T07-B	1	2.76E+02			2.76E+02	5.6E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T08-B	1	9.81E+01			9.81E+01	2.4E+01	1.5E+01	4.8E+01			---		VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T09-B	1	7.27E+02			7.27E+02	7.3E+01	1.5E+01	4.8E+01			---		VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T01-C	1	7.40E+03			7.40E+03	4.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T02-C	1	5.71E+03			5.71E+03	9.8E-01	1.5E+01	4.8E+01			---		VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T03-C	1	4.82E+03			4.82E+03	4.2E-01	1.5E+01	4.8E+01	10	325	7.60E+03	86%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T04-C	1	2.85E+03			2.85E+03	2.3E+00	1.5E+01	4.8E+01					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T05-C	1	1.60E+03			1.60E+03	2.2E+00	1.5E+01	4.8E+01					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T06-C	1	8.61E+02			8.61E+02	3.2E+00	1.5E+01	4.8E+01					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T07-C	1	2.75E+02			2.75E+02	7.9E+00	1.5E+01	4.8E+01					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T08-C	1	1.00E+02			1.00E+02	1.4E+01	1.5E+01	4.8E+01					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-T09-C	1	7.68E+02			7.68E+02	1.3E+01	1.5E+01	4.8E+01					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-B01-A	1	1.69E+01	E		1.69E+01	1.8E+02	1.5E+01	4.8E+01					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-B02-A	1	7.50E+00	U1/2		7.50E+00	3.8E+01	1.5E+01	4.8E+01					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-B03-A	1	1.68E+01	E		1.68E+01	8.0E+01	1.5E+01	4.8E+01					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-B01-B	1	1.61E+01	E		1.61E+01	6.9E+01	1.5E+01	4.8E+01					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-B02-B	1	7.50E+00	U1/2		7.50E+00	7.7E+02	1.5E+01	4.8E+01					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1313-B03-B	1	7.50E+00	U1/2		7.50E+00	2.3E+02	1.5E+01	4.8E+01					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	EaFA-L06-1313-T01-A	1	2.21E+04			2.21E+04	7.7E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T02-A	1	4.52E+03			4.52E+03	8.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T03-A	1	1.68E+03			1.68E+03	1.8E-01	1.1E+00	3.5E+00	1000	100	2.57E+03	90%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T04-A	1	3.99E+02			3.99E+02	6.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T05-A	1	5.67E+02			5.67E+02	4.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T06-A	1	2.58E+03			2.58E+03	2.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T07-A	1	1.29E+04			1.29E+04	6.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T08-A	1	3.66E+04			3.66E+04	5.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T09-A	1	6.80E+04			6.80E+04	2.8E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T01-B	1	1.95E+04			1.95E+04	2.7E+01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T02-B	1	5.13E+03			5.13E+03	5.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T03-B	1	3.58E+02			3.58E+02	9.0E+00	1.1E+00	3.5E+00	1000	100	1.41E+03	105%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T04-B	1	3.60E+02			3.60E+02	2.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T05-B	1	7.86E+02			7.86E+02	1.0E+01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T06-B	1	2.41E+03			2.41E+03	1.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T07-B	1	6.47E+03			6.47E+03	6.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T08-B	1	1.81E+04			1.81E+04	2.9E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T09-B	1	6.73E+04			6.73E+04	4.5E+01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T01-C	1	2.31E+04			2.31E+04	3.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T02-C	1	4.71E+03			4.71E+03	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T03-C	1	3.78E+02			3.78E+02	6.6E-01	1.1E+00	3.5E+00	1000	100	1.34E+03	97%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T04-C	1	3.66E+02			3.66E+02	9.7E-01	1.1E+00	3.5E+00					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T05-C	1	9.18E+02			9.18E+02	9.9E-01	1.1E+00	3.5E+00					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T06-C	1	2.14E+03			2.14E+03	4.9E+00	1.1E+00	3.5E+00					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T07-C	1	6.64E+03			6.64E+03	7.8E+00	1.1E+00	3.5E+00					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T08-C	1	1.85E+04			1.85E+04	2.7E+00	1.1E+00	3.5E+00					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-T09-C	1	6.70E+04			6.70E+04	2.6E+01	1.1E+00	3.5E+00					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-B01-A	1	5.50E-01	U1/2		5.50E-01	1.9E+01	1.1E+00	3.5E+00					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-B02-A	1	5.50E-01	U1/2		5.50E-01	2.2E+01	1.1E+00	3.5E+00					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-B03-A	1	3.93E+02			3.93E+02	1.4E+01	1.1E+00	3.5E+00					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-B01-B	1	5.50E-01	U1/2		5.50E-01	1.7E+01	1.1E+00	3.5E+00					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-B02-B	1	5.50E-01	U1/2		5.50E-01	3.3E+01	1.1E+00	3.5E+00					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1313-B03-B	1	2.43E+02			2.43E+02	8.3E+00	1.1E+00	3.5E+00					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	EaFA-L06-1313-T01-A	1	3.17E+05			3.17E+05	5.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T02-A	1	1.58E+05			1.58E+05	8.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T03-A	1	5.75E+04			5.75E+04	2.5E-01	2.5E+00	8.0E+00	1000	100	5.84E+04	92%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T04-A	1	3.72E+04			3.72E+04	1.6E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T05-A	1	2.24E+04			2.24E+04	5.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T06-A	1	5.37E+03			5.37E+03	5.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T07-A	1	4.13E+03			4.13E+03	1.5E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T08-A	1	3.34E+03			3.34E+03	4.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T09-A	1	2.96E+03			2.96E+03	2.9E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T01-B	1	2.52E+05			2.52E+05	1.9E+01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T02-B	1	1.66E+05			1.66E+05	5.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T03-B	1	4.12E+04			4.12E+04	7.6E+00	2.5E+00	8.0E+00	1000	100	4.20E+04	82%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T04-B	1	2.40E+04			2.40E+04	3.5E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T05-B	1	1.34E+04			1.34E+04	1.0E+01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T06-B	1	5.26E+03			5.26E+03	2.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T07-B	1	5.41E+03			5.41E+03	6.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T08-B	1	3.64E+03			3.64E+03	4.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T09-B	1	3.07E+03			3.07E+03	7.5E+01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T01-C	1	3.26E+05			3.26E+05	3.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T02-C	1	1.50E+05			1.50E+05	4.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T03-C	1	4.45E+04			4.45E+04	1.0E+00	2.5E+00	8.0E+00	1000	100	4.53E+04	83%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T04-C	1	2.60E+04			2.60E+04	6.8E-01	2.5E+00	8.0E+00					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T05-C	1	1.51E+04			1.51E+04	4.4E-01	2.5E+00	8.0E+00					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T06-C	1	5.53E+03			5.53E+03	5.0E+00	2.5E+00	8.0E+00					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T07-C	1	5.31E+03			5.31E+03	8.1E+00	2.5E+00	8.0E+00					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T08-C	1	3.54E+03			3.54E+03	2.4E+00	2.5E+00	8.0E+00					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-T09-C	1	3.10E+03			3.10E+03	1.4E+01	2.5E+00	8.0E+00					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-B01-A	1	2.30E+01			2.30E+01	7.0E-01	2.5E+00	8.0E+00					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-B02-A	1	2.28E+01			2.28E+01	4.2E+00	2.5E+00	8.0E+00					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-B03-A	1	3.22E+05			3.22E+05	8.1E+00	2.5E+00	8.0E+00					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-B01-B	1	2.13E+01			2.13E+01	1.5E+00	2.5E+00	8.0E+00					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-B02-B	1	2.16E+01			2.16E+01	2.6E+00	2.5E+00	8.0E+00					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1313-B03-B	1	3.09E+05			3.09E+05	6.6E+00	2.5E+00	8.0E+00					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	EaFA-L06-1313-T01-A	1	1.44E+03			1.44E+03	7.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T02-A	1	1.57E+03			1.57E+03	1.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T03-A	1	1.76E+03			1.76E+03	6.5E-01	1.0E+00	3.2E+00	1000	100	2.64E+03	89%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T04-A	1	1.86E+03			1.86E+03	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T05-A	1	1.91E+03			1.91E+03	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T06-A	1	2.25E+03			2.25E+03	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T07-A	1	2.60E+03			2.60E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T08-A	1	3.88E+03			3.88E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T09-A	1	5.28E+03			5.28E+03	2.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T01-B	1	1.22E+03			1.22E+03	1.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T02-B	1	1.65E+03			1.65E+03	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T03-B	1	1.82E+03			1.82E+03	7.9E+00	1.0E+00	3.2E+00	1000	100	2.79E+03	97%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T04-B	1	1.98E+03			1.98E+03	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T05-B	1	1.95E+03			1.95E+03	7.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T06-B	1	2.30E+03			2.30E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T07-B	1	2.85E+03			2.85E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T08-B	1	2.94E+03			2.94E+03	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T09-B	1	5.18E+03			5.18E+03	3.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T01-C	1	1.56E+03			1.56E+03	2.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T02-C	1	1.45E+03			1.45E+03	9.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T03-C	1	1.97E+03			1.97E+03	1.2E+00	1.0E+00	3.2E+00	1000	100	2.84E+03	86%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T04-C	1	2.04E+03			2.04E+03	2.3E-01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T05-C	1	2.21E+03			2.21E+03	9.0E-01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T06-C	1	2.43E+03			2.43E+03	5.4E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T07-C	1	2.67E+03			2.67E+03	6.2E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T08-C	1	2.90E+03			2.90E+03	2.3E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-T09-C	1	5.26E+03			5.26E+03	5.2E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	2.1E+02	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	2.3E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-B03-A	1	2.13E+00	E		2.13E+00	4.1E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	2.7E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	4.1E+02	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1313-B03-B	1	1.81E+00	E		1.81E+00	1.9E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	EaFA-L06-1313-T01-A	1	1.87E+05			1.87E+05	8.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T02-A	1	1.81E+05			1.81E+05	6.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T03-A	1	1.70E+05			1.70E+05	5.9E-01	6.8E+00	2.2E+01	1000	100	1.71E+05	86%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T04-A	1	1.75E+05			1.75E+05	3.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T05-A	1	1.71E+05			1.71E+05	1.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T06-A	1	1.72E+05			1.72E+05	5.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T07-A	1	1.14E+05			1.14E+05	7.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T08-A	1	9.30E+04			9.30E+04	9.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T09-A	1	6.22E+04			6.22E+04	2.8E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T01-B	1	1.73E+05			1.73E+05	3.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T02-B	1	1.85E+05			1.85E+05	3.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T03-B	1	1.65E+05			1.65E+05	8.6E+00	6.8E+00	2.2E+01	1000	100	1.66E+05	97%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T04-B	1	1.62E+05			1.62E+05	2.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T05-B	1	1.58E+05			1.58E+05	9.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T06-B	1	1.70E+05			1.70E+05	2.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T07-B	1	1.62E+05			1.62E+05	6.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T08-B	1	1.05E+05			1.05E+05	3.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T09-B	1	6.14E+04			6.14E+04	7.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T01-C	1	1.86E+05			1.86E+05	3.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T02-C	1	1.67E+05			1.67E+05	7.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T03-C	1	1.78E+05			1.78E+05	3.0E-01	6.8E+00	2.2E+01	1000	100	1.79E+05	81%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T04-C	1	1.73E+05			1.73E+05	1.0E+00	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T05-C	1	1.80E+05			1.80E+05	6.4E-01	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T06-C	1	1.79E+05			1.79E+05	5.2E+00	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T07-C	1	1.57E+05			1.57E+05	7.4E+00	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T08-C	1	1.04E+05			1.04E+05	2.6E+00	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-T09-C	1	6.24E+04			6.24E+04	1.4E+01	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	1.2E+01	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	8.7E+00	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	6.3E+00	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-B01-B	1	3.40E+00	U1/2		3.40E+00	1.5E+01	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-B02-B	1	3.40E+00	U1/2		3.40E+00	8.8E+00	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1313-B03-B	1	3.40E+00	U1/2		3.40E+00	3.2E+01	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	EaFA-L06-1313-T01-A	1	9.37E+00	E		9.37E+00	8.2E+00	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T02-A	1	2.30E+00	U1/2		2.30E+00	1.9E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T03-A	1	2.30E+00	U1/2		2.30E+00	2.5E+02	4.6E+00	1.5E+01	10	325	3.08E+03	95%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T04-A	1	2.30E+00	U1/2		2.30E+00	7.9E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T05-A	1	2.30E+00	U1/2		2.30E+00	1.8E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T06-A	1	2.30E+00	U1/2		2.30E+00	2.0E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T07-A	1	4.74E+01			4.74E+01	3.5E+00	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T08-A	1	4.79E+01			4.79E+01	1.4E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T09-A	1	7.56E+01			7.56E+01	1.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T01-B	1	9.86E+00	E		9.86E+00	2.2E+03	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T02-B	1	2.30E+00	U1/2		2.30E+00	9.5E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T03-B	1	2.30E+00	U1/2		2.30E+00	2.9E+01	4.6E+00	1.5E+01	10	325	3.21E+03	99%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T04-B	1	2.30E+00	U1/2		2.30E+00	3.5E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T05-B	1	2.30E+00	U1/2		2.30E+00	5.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T06-B	1	1.27E+01	E		1.27E+01	4.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T07-B	1	4.25E+01			4.25E+01	1.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T08-B	1	5.08E+01			5.08E+01	1.1E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T09-B	1	7.10E+01			7.10E+01	1.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T01-C	1	1.24E+01	E		1.24E+01	6.4E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T02-C	1	2.30E+00	U1/2		2.30E+00	5.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T03-C	1	2.30E+00	U1/2		2.30E+00	7.2E+01	4.6E+00	1.5E+01	10	325	3.10E+03	95%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T04-C	1	2.30E+00	U1/2		2.30E+00	7.6E+02	4.6E+00	1.5E+01					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T05-C	1	2.30E+00	U1/2		2.30E+00	3.0E+02	4.6E+00	1.5E+01					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T06-C	1	2.30E+00	U1/2		2.30E+00	4.7E+01	4.6E+00	1.5E+01					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T07-C	1	3.44E+01			3.44E+01	3.0E+01	4.6E+00	1.5E+01					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T08-C	1	4.96E+01			4.96E+01	2.0E+01	4.6E+00	1.5E+01					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-T09-C	1	7.36E+01			7.36E+01	1.4E+01	4.6E+00	1.5E+01					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	1.8E+02	4.6E+00	1.5E+01					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	2.4E+01	4.6E+00	1.5E+01					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	3.8E+02	4.6E+00	1.5E+01					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-B01-B	1	2.30E+00	U1/2		2.30E+00	3.6E+02	4.6E+00	1.5E+01					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-B02-B	1	2.30E+00	U1/2		2.30E+00	6.3E+01	4.6E+00	1.5E+01					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1313-B03-B	1	2.30E+00	U1/2		2.30E+00	1.3E+02	4.6E+00	1.5E+01					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	EaFA-L06-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	7.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	7.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	7.4E+02	2.0E+00	6.4E+00	10	325	3.17E+03	97%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	9.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	4.5E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	4.3E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T07-A	1	6.71E+00			6.71E+00	9.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T08-A	1	2.66E+01			2.66E+01	2.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T09-A	1	4.64E+03			4.64E+03	2.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	7.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	1.1E+03	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00	10	325	3.27E+03	100%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	3.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	1.7E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T08-B	1	1.29E+01			1.29E+01	4.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T09-B	1	4.29E+03			4.29E+03	6.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T01-C	1	2.13E+00	E		2.13E+00	4.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	1.7E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	6.0E+02	2.0E+00	6.4E+00	10	325	3.12E+03	96%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	9.4E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	4.7E+02	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	9.1E+02	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T08-C	1	1.23E+01			1.23E+01	1.0E+00	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-T09-C	1	4.59E+03			4.59E+03	3.8E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	2.8E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	5.1E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	1.6E+02	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	3.9E+02	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	5.1E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	EaFA-L06-1313-T01-A	1	5.36E+03			5.36E+03	8.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T02-A	1	2.82E+03			2.82E+03	4.9E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T03-A	1	3.00E+03			3.00E+03	1.9E-01	1.5E+00	4.8E+00	10	325	6.00E+03	93%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T04-A	1	1.28E+03			1.28E+03	6.0E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T05-A	1	5.04E+02			5.04E+02	6.2E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T06-A	1	1.94E+02			1.94E+02	6.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T07-A	1	8.96E+01			8.96E+01	4.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T08-A	1	1.14E+02			1.14E+02	8.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T09-A	1	5.97E+03			5.97E+03	2.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T01-B	1	5.58E+03			5.58E+03	2.0E+01	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T02-B	1	3.02E+03			3.02E+03	4.4E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T03-B	1	1.23E+03			1.23E+03	7.8E+00	1.5E+00	4.8E+00	10	325	4.51E+03	101%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T04-B	1	3.84E+02			3.84E+02	3.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T05-B	1	2.15E+02			2.15E+02	8.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T06-B	1	1.65E+02			1.65E+02	1.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T07-B	1	8.42E+01			8.42E+01	2.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T08-B	1	8.56E+01			8.56E+01	4.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T09-B	1	5.93E+03			5.93E+03	7.2E+01	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T01-C	1	6.02E+03			6.02E+03	2.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T02-C	1	2.72E+03			2.72E+03	8.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T03-C	1	1.29E+03			1.29E+03	1.7E+00	1.5E+00	4.8E+00	10	325	4.32E+03	93%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T04-C	1	4.31E+02			4.31E+02	1.6E+00	1.5E+00	4.8E+00					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T05-C	1	2.42E+02			2.42E+02	2.0E+00	1.5E+00	4.8E+00					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T06-C	1	1.51E+02			1.51E+02	7.4E+00	1.5E+00	4.8E+00					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T07-C	1	8.75E+01			8.75E+01	5.1E+00	1.5E+00	4.8E+00					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T08-C	1	8.84E+01			8.84E+01	3.1E+00	1.5E+00	4.8E+00					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-T09-C	1	5.93E+03			5.93E+03	2.6E+01	1.5E+00	4.8E+00					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-B01-A	1	7.50E-01	U1/2		7.50E-01	2.2E+02	1.5E+00	4.8E+00					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-B02-A	1	7.50E-01	U1/2		7.50E-01	2.1E+02	1.5E+00	4.8E+00					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-B03-A	1	3.38E+00	E		3.38E+00	5.1E+01	1.5E+00	4.8E+00					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-B01-B	1	7.50E-01	U1/2		7.50E-01	1.3E+02	1.5E+00	4.8E+00					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-B02-B	1	7.50E-01	U1/2		7.50E-01	4.7E+02	1.5E+00	4.8E+00					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1313-B03-B	1	2.05E+00	E		2.05E+00	1.3E+02	1.5E+00	4.8E+00					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	EaFA-L06-1313-T01-A	1	2.50E+02			2.50E+02	6.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:36 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T02-A	1	1.84E+01			1.84E+01	2.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:38 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T03-A	1	5.40E+00			5.40E+00	1.1E+01	1.0E+00	3.2E+00	10	325	3.36E+03	103%	VU ICP-OES	6/7/10 2:40 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T04-A	1	8.08E+00			8.08E+00	4.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:41 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T05-A	1	1.33E+01			1.33E+01	3.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:43 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T06-A	1	2.81E+01			2.81E+01	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:45 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T07-A	1	1.17E+03			1.17E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:05 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T08-A	1	1.21E+03			1.21E+03	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:48 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T09-A	1	1.59E+03			1.59E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 2:50 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T01-B	1	2.43E+02			2.43E+02	1.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:06 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T02-B	1	4.57E+01			4.57E+01	2.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:03 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T03-B	1	4.64E+00			4.64E+00	7.6E+00	1.0E+00	3.2E+00	10	325	3.47E+03	107%	VU ICP-OES	6/7/10 3:04 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T04-B	1	5.85E+00			5.85E+00	9.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:06 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T05-B	1	8.25E+00			8.25E+00	2.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:08 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T06-B	1	3.06E+01			3.06E+01	5.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:09 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T07-B	1	1.25E+03			1.25E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:11 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T08-B	1	1.16E+03			1.16E+03	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:13 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T09-B	1	1.53E+03			1.53E+03	6.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:14 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T01-C	1	2.50E+02			2.50E+02	3.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:21 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T02-C	1	1.87E+01			1.87E+01	5.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:08 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T03-C	1	7.78E+00			7.78E+00	1.5E+01	1.0E+00	3.2E+00	10	325	3.35E+03	103%	VU ICP-OES	6/7/10 3:24 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T04-C	1	5.10E+00			5.10E+00	1.5E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 4:09 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T05-C	1	9.53E+00			9.53E+00	8.8E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 3:27 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T06-C	1	2.25E+01			2.25E+01	4.9E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 3:29 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T07-C	1	1.19E+03			1.19E+03	6.5E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 4:11 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T08-C	1	1.15E+03			1.15E+03	4.6E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 3:32 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-T09-C	1	1.54E+03			1.54E+03	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 3:34 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-B01-A	1	6.98E+00			6.98E+00	7.6E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:31 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-B02-A	1	1.10E+01			1.10E+01	1.4E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:33 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-B03-A	1	1.27E+01			1.27E+01	4.4E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:35 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-B01-B	1	9.92E+00			9.92E+00	7.2E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:56 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-B02-B	1	1.09E+01			1.09E+01	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:58 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1313-B03-B	1	1.84E+01			1.84E+01	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 2:59 PM	EPA Interlab L06 1313-1316 EaFA

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	EaFA-L07-1313-T01-A	1	2.46E+04			2.46E+04	4.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T02-A	1	3.18E+04			3.18E+04	9.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T03-A	1	2.24E+04			2.24E+04	5.5E-01	1.0E+00	3.2E+00	1000	100	2.34E+04	103%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T04-A	1	6.83E+03			6.83E+03	5.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T05-A	1	6.17E+02			6.17E+02	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T06-A	1	1.00E+02			1.00E+02	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T07-A	1	1.03E+03			1.03E+03	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T08-A	1	3.63E+04			3.63E+04	2.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T09-A	1	1.33E+05			1.33E+05	7.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T01-B	1	3.41E+04			3.41E+04	6.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T02-B	1	3.24E+04			3.24E+04	2.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T03-B	1	2.19E+04			2.19E+04	6.0E+00	1.0E+00	3.2E+00	1000	100	2.28E+04	90%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T04-B	1	3.39E+03			3.39E+03	4.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T05-B	1	3.94E+02			3.94E+02	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T06-B	1	1.83E+02			1.83E+02	9.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T07-B	1	1.01E+03			1.01E+03	4.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T08-B	1	4.58E+04			4.58E+04	3.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T09-B	1	1.30E+05			1.30E+05	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T01-C	1	3.26E+04			3.26E+04	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T02-C	1	2.98E+04			2.98E+04	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T03-C	1	2.01E+04			2.01E+04	3.6E-02	1.0E+00	3.2E+00	1000	100	2.10E+04	88%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T04-C	1	6.15E+03			6.15E+03	7.0E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T05-C	1	6.00E+02			6.00E+02	2.9E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T06-C	1	1.58E+02			1.58E+02	1.8E+03	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T07-C	1	9.80E+02			9.80E+02	6.3E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T08-C	1	3.61E+04			3.61E+04	4.5E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-T09-C	1	1.26E+05			1.26E+05	8.7E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.0E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	6.1E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	1.5E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	6.3E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	1.9E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	4.9E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	4.6E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	6.5E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	1.0E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	EaFA-L07-1313-T01-A	1	2.69E+02			2.69E+02	2.9E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T02-A	1	1.49E+02			1.49E+02	1.4E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T03-A	1	2.07E+02			2.07E+02	1.1E+01	7.5E+00	2.4E+01	10	325	3.46E+03	100%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T04-A	1	1.83E+02			1.83E+02	2.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T05-A	1	2.03E+02			2.03E+02	4.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T06-A	1	2.03E+02			2.03E+02	6.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T07-A	1	6.99E+01			6.99E+01	2.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T08-A	1	4.69E+01			4.69E+01	1.5E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T09-A	1	3.75E+00	U1/2		3.75E+00	2.7E+02	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T01-B	1	1.85E+02			1.85E+02	1.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T02-B	1	1.45E+02			1.45E+02	2.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T03-B	1	1.75E+02			1.75E+02	1.4E+01	7.5E+00	2.4E+01	10	325	3.83E+03	112%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T04-B	1	2.14E+02			2.14E+02	1.4E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T05-B	1	2.07E+02			2.07E+02	3.9E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T06-B	1	1.67E+02			1.67E+02	1.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T07-B	1	6.89E+01			6.89E+01	3.5E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T08-B	1	1.53E+01	E		1.53E+01	5.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T09-B	1	3.75E+00	U1/2		3.75E+00	1.9E+02	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T01-C	1	2.15E+02			2.15E+02	1.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T02-C	1	1.40E+02			1.40E+02	1.4E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T03-C	1	1.93E+02			1.93E+02	1.4E+01	7.5E+00	2.4E+01	10	325	3.35E+03	97%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T04-C	1	1.95E+02			1.95E+02	9.8E+00	7.5E+00	2.4E+01					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T05-C	1	2.16E+02			2.16E+02	1.1E+01	7.5E+00	2.4E+01					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T06-C	1	2.15E+02			2.15E+02	1.6E+02	7.5E+00	2.4E+01					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T07-C	1	9.03E+01			9.03E+01	2.3E+01	7.5E+00	2.4E+01					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T08-C	1	3.11E+01			3.11E+01	4.7E+00	7.5E+00	2.4E+01					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-T09-C	1	3.75E+00	U1/2		3.75E+00	2.8E+03	7.5E+00	2.4E+01					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-B01-A	1	3.75E+00	U1/2		3.75E+00	3.1E+02	7.5E+00	2.4E+01					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-B02-A	1	3.75E+00	U1/2		3.75E+00	1.9E+02	7.5E+00	2.4E+01					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-B03-A	1	3.15E+01			3.15E+01	4.3E+01	7.5E+00	2.4E+01					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-B01-B	1	1.43E+01	E		1.43E+01	1.6E+02	7.5E+00	2.4E+01					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-B02-B	1	1.89E+01	E		1.89E+01	5.3E+01	7.5E+00	2.4E+01					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-B03-B	1	2.57E+01			2.57E+01	1.1E+02	7.5E+00	2.4E+01					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-B01-C	1	3.75E+00	U1/2		3.75E+00	1.4E+03	7.5E+00	2.4E+01					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-B02-C	1	3.75E+00	U1/2		3.75E+00	2.0E+02	7.5E+00	2.4E+01					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1313-B03-C	1	1.17E+01	E		1.17E+01	5.9E+01	7.5E+00	2.4E+01					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	EaFA-L07-1313-T01-A	1	7.01E+03			7.01E+03	7.6E-01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T02-A	1	8.68E+02			8.68E+02	2.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T03-A	1	1.40E+03			1.40E+03	3.4E-01	1.1E+01	3.5E+01	10	325	4.59E+03	98%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T04-A	1	6.56E+02			6.56E+02	5.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T05-A	1	2.23E+02			2.23E+02	4.7E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T06-A	1	9.42E+01			9.42E+01	2.2E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T07-A	1	8.25E+01			8.25E+01	8.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T08-A	1	1.42E+02			1.42E+02	1.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T09-A	1	2.91E+03			2.91E+03	2.8E-01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T01-B	1	6.94E+03			6.94E+03	7.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T02-B	1	8.31E+02			8.31E+02	9.1E-01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T03-B	1	1.31E+03			1.31E+03	5.6E+00	1.1E+01	3.5E+01	10	325	4.58E+03	101%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T04-B	1	4.68E+02			4.68E+02	4.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T05-B	1	1.77E+02			1.77E+02	8.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T06-B	1	8.93E+01			8.93E+01	1.4E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T07-B	1	9.83E+01			9.83E+01	1.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T08-B	1	1.24E+02			1.24E+02	1.2E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T09-B	1	1.84E+03			1.84E+03	1.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T01-C	1	7.25E+03			7.25E+03	9.2E-01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T02-C	1	8.38E+02			8.38E+02	3.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T03-C	1	1.31E+03			1.31E+03	1.0E+00	1.1E+01	3.5E+01	10	325	4.41E+03	96%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T04-C	1	6.11E+02			6.11E+02	1.3E+01	1.1E+01	3.5E+01					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T05-C	1	2.81E+02			2.81E+02	1.3E+01	1.1E+01	3.5E+01					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T06-C	1	1.20E+02			1.20E+02	5.8E+02	1.1E+01	3.5E+01					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T07-C	1	9.71E+01			9.71E+01	1.4E+01	1.1E+01	3.5E+01					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T08-C	1	1.33E+02			1.33E+02	9.7E+00	1.1E+01	3.5E+01					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-T09-C	1	2.18E+03			2.18E+03	8.7E-01	1.1E+01	3.5E+01					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-B01-A	1	5.50E+00	U1/2		5.50E+00	2.1E+02	1.1E+01	3.5E+01					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-B02-A	1	5.50E+00	U1/2		5.50E+00	7.3E+01	1.1E+01	3.5E+01					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-B03-A	1	5.50E+00	U1/2		5.50E+00	5.3E+02	1.1E+01	3.5E+01					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-B01-B	1	1.79E+01	E		1.79E+01	6.6E+01	1.1E+01	3.5E+01					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-B02-B	1	5.50E+00	U1/2		5.50E+00	2.6E+02	1.1E+01	3.5E+01					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-B03-B	1	1.27E+01	E		1.27E+01	1.2E+02	1.1E+01	3.5E+01					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-B01-C	1	5.50E+00	U1/2		5.50E+00	2.7E+02	1.1E+01	3.5E+01					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-B02-C	1	1.35E+01	E		1.35E+01	1.5E+02	1.1E+01	3.5E+01					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1313-B03-C	1	1.16E+01	E		1.16E+01	6.3E+01	1.1E+01	3.5E+01					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	EaFA-L07-1313-T01-A	1	4.41E+03			4.41E+03	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T02-A	1	4.39E+03			4.39E+03	2.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T03-A	1	4.31E+03			4.31E+03	1.3E+00	1.0E+00	3.2E+00	1000	100	5.15E+03	84%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T04-A	1	3.95E+03			3.95E+03	6.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T05-A	1	4.32E+03			4.32E+03	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T06-A	1	4.38E+03			4.38E+03	3.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T07-A	1	4.43E+03			4.43E+03	1.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T08-A	1	3.64E+03			3.64E+03	7.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T09-A	1	2.84E+03			2.84E+03	6.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T01-B	1	4.08E+03			4.08E+03	7.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T02-B	1	4.29E+03			4.29E+03	4.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T03-B	1	3.96E+03			3.96E+03	6.3E+00	1.0E+00	3.2E+00	1000	100	4.84E+03	88%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T04-B	1	3.99E+03			3.99E+03	4.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T05-B	1	4.30E+03			4.30E+03	8.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T06-B	1	4.33E+03			4.33E+03	8.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T07-B	1	4.59E+03			4.59E+03	5.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T08-B	1	3.84E+03			3.84E+03	2.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T09-B	1	2.81E+03			2.81E+03	9.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T01-C	1	4.27E+03			4.27E+03	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T02-C	1	4.21E+03			4.21E+03	6.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T03-C	1	4.08E+03			4.08E+03	2.0E+00	1.0E+00	3.2E+00	1000	100	5.00E+03	91%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T04-C	1	3.68E+03			3.68E+03	4.6E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T05-C	1	4.20E+03			4.20E+03	2.6E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T06-C	1	4.76E+03			4.76E+03	1.3E+02	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T07-C	1	4.39E+03			4.39E+03	4.7E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T08-C	1	3.67E+03			3.67E+03	3.5E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-T09-C	1	2.89E+03			2.89E+03	4.3E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-B01-A	1	1.40E+01			1.40E+01	9.8E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-B02-A	1	1.37E+01			1.37E+01	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-B03-A	1	2.05E+01			2.05E+01	6.5E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-B01-B	1	4.11E+01			4.11E+01	5.3E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-B02-B	1	2.66E+01			2.66E+01	3.5E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-B03-B	1	2.88E+01			2.88E+01	3.6E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-B01-C	1	3.02E+01			3.02E+01	5.3E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-B02-C	1	1.92E+01			1.92E+01	2.9E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1313-B03-C	1	2.19E+01			2.19E+01	1.7E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	EaFA-L07-1313-T01-A	1	2.09E+02			2.09E+02	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T02-A	1	9.60E+02			9.60E+02	3.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T03-A	1	8.09E+02			8.09E+02	9.0E-01	1.0E+00	3.2E+00	10	325	3.71E+03	89%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T04-A	1	5.46E+02			5.46E+02	6.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T05-A	1	2.82E+02			2.82E+02	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T06-A	1	2.86E+02			2.86E+02	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T07-A	1	2.71E+02			2.71E+02	8.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T08-A	1	2.82E+02			2.82E+02	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T09-A	1	9.80E+02			9.80E+02	1.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T01-B	1	1.14E+03			1.14E+03	6.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T02-B	1	9.29E+02			9.29E+02	7.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T03-B	1	7.47E+02			7.47E+02	5.7E+00	1.0E+00	3.2E+00	10	325	4.35E+03	111%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T04-B	1	3.94E+02			3.94E+02	5.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T05-B	1	2.67E+02			2.67E+02	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T06-B	1	2.68E+02			2.68E+02	1.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T07-B	1	2.72E+02			2.72E+02	5.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T08-B	1	3.07E+02			3.07E+02	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T09-B	1	8.90E+02			8.90E+02	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T01-C	1	9.74E+02			9.74E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T02-C	1	8.46E+02			8.46E+02	3.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T03-C	1	7.01E+02			7.01E+02	9.5E-01	1.0E+00	3.2E+00	10	325	3.52E+03	87%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T04-C	1	5.02E+02			5.02E+02	8.2E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T05-C	1	2.89E+02			2.89E+02	4.7E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T06-C	1	2.90E+02			2.90E+02	1.3E+02	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T07-C	1	2.75E+02			2.75E+02	5.2E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T08-C	1	2.83E+02			2.83E+02	2.4E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-T09-C	1	9.26E+02			9.26E+02	1.0E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	4.5E+02	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	8.1E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-B03-A	1	1.75E+00	E		1.75E+00	9.8E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	1.0E+02	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-B02-B	1	1.06E+00	E		1.06E+00	5.5E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-B03-B	1	1.85E+00	E		1.85E+00	8.3E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	3.0E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	5.2E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1313-B03-C	1	1.57E+00	E		1.57E+00	7.6E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	EaFA-L07-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	4.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	1.1E+03	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	5.6E+02	1.9E+00	6.0E+00	10	325	3.27E+03	101%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	1.9E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	1.7E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	5.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T07-A	1	9.29E+00			9.29E+00	3.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T08-A	1	1.32E+02			1.32E+02	4.8E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T09-A	1	2.55E+02			2.55E+02	1.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	2.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	2.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	7.8E+01	1.9E+00	6.0E+00	10	325	3.66E+03	113%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	9.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	1.7E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T07-B	1	9.54E+00			9.54E+00	7.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T08-B	1	1.47E+02			1.47E+02	3.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T09-B	1	2.50E+02			2.50E+02	8.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	1.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	3.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	3.4E+02	1.9E+00	6.0E+00	10	325	3.15E+03	97%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	6.9E+01	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	2.8E+02	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	5.2E+01	1.9E+00	6.0E+00					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T07-C	1	9.11E+00			9.11E+00	3.7E+00	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T08-C	1	1.32E+02			1.32E+02	2.8E-01	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-T09-C	1	2.48E+02			2.48E+02	1.5E+00	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	5.1E+02	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	5.9E+01	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	3.7E+03	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-B01-B	1	9.50E-01	U1/2		9.50E-01	4.5E+02	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-B02-B	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-B03-B	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-B01-C	1	9.50E-01	U1/2		9.50E-01	1.8E+02	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-B02-C	1	9.50E-01	U1/2		9.50E-01	2.7E+01	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1313-B03-C	1	9.50E-01	U1/2		9.50E-01	3.5E+01	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	EaFA-L07-1313-T01-A	1	1.10E+00	U1/2		1.10E+00	1.9E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T02-A	1	1.10E+00	U1/2		1.10E+00	1.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	5.4E+00	2.2E+00	7.0E+00	10	325	3.27E+03	100%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T04-A	1	1.10E+00	U1/2		1.10E+00	8.9E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T05-A	1	1.10E+00	U1/2		1.10E+00	1.7E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T06-A	1	1.10E+00	U1/2		1.10E+00	4.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T07-A	1	3.37E+01			3.37E+01	2.0E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T08-A	1	2.61E+01			2.61E+01	3.5E-01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T09-A	1	2.99E+01			2.99E+01	1.5E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T01-B	1	1.10E+00	U1/2		1.10E+00	1.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T02-B	1	1.10E+00	U1/2		1.10E+00	8.4E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	6.6E+00	2.2E+00	7.0E+00	10	325	3.56E+03	109%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T04-B	1	1.10E+00	U1/2		1.10E+00	2.3E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T05-B	1	1.10E+00	U1/2		1.10E+00	2.0E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T06-B	1	1.10E+00	U1/2		1.10E+00	2.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T07-B	1	3.55E+01			3.55E+01	7.8E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T08-B	1	2.52E+01			2.52E+01	1.9E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T09-B	1	2.91E+01			2.91E+01	2.2E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T01-C	1	1.10E+00	U1/2		1.10E+00	1.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T02-C	1	1.10E+00	U1/2		1.10E+00	1.3E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	2.3E+01	2.2E+00	7.0E+00	10	325	3.15E+03	97%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T04-C	1	1.10E+00	U1/2		1.10E+00	1.6E+01	2.2E+00	7.0E+00					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T05-C	1	1.10E+00	U1/2		1.10E+00	1.9E+01	2.2E+00	7.0E+00					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T06-C	1	1.10E+00	U1/2		1.10E+00	5.0E-01	2.2E+00	7.0E+00					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T07-C	1	3.36E+01			3.36E+01	1.7E+00	2.2E+00	7.0E+00					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T08-C	1	2.60E+01			2.60E+01	8.9E-01	2.2E+00	7.0E+00					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-T09-C	1	2.88E+01			2.88E+01	8.5E-01	2.2E+00	7.0E+00					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	1.7E+01	2.2E+00	7.0E+00					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	5.5E+00	2.2E+00	7.0E+00					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-B03-A	1	1.10E+00	U1/2		1.10E+00	3.6E+01	2.2E+00	7.0E+00					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-B01-B	1	1.10E+00	U1/2		1.10E+00	1.7E+01	2.2E+00	7.0E+00					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-B02-B	1	1.10E+00	U1/2		1.10E+00	1.6E+01	2.2E+00	7.0E+00					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-B03-B	1	1.10E+00	U1/2		1.10E+00	1.4E+01	2.2E+00	7.0E+00					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-B01-C	1	1.10E+00	U1/2		1.10E+00	7.9E+00	2.2E+00	7.0E+00					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-B02-C	1	1.10E+00	U1/2		1.10E+00	8.4E+00	2.2E+00	7.0E+00					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1313-B03-C	1	1.10E+00	U1/2		1.10E+00	3.6E+01	2.2E+00	7.0E+00					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	EaFA-L07-1313-T01-A	1	1.31E+04			1.31E+04	7.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T02-A	1	5.28E+04			5.28E+04	5.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T03-A	1	9.68E+04			9.68E+04	4.2E-01	2.6E+00	8.3E+00	1000	100	9.77E+04	92%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T04-A	1	1.26E+05			1.26E+05	5.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T05-A	1	1.49E+05			1.49E+05	9.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T06-A	1	1.58E+05			1.58E+05	5.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T07-A	1	1.59E+05			1.59E+05	6.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T08-A	1	1.46E+05			1.46E+05	4.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T09-A	1	1.36E+05			1.36E+05	2.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T01-B	1	1.71E+04			1.71E+04	7.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T02-B	1	5.29E+04			5.29E+04	4.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T03-B	1	8.90E+04			8.90E+04	6.8E+00	2.6E+00	8.3E+00	1000	100	9.00E+04	99%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T04-B	1	1.30E+05			1.30E+05	4.8E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T05-B	1	1.56E+05			1.56E+05	4.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T06-B	1	1.62E+05			1.62E+05	7.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T07-B	1	1.66E+05			1.66E+05	6.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T08-B	1	1.48E+05			1.48E+05	1.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T09-B	1	1.35E+05			1.35E+05	1.5E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T01-C	1	1.74E+04			1.74E+04	1.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T02-C	1	5.16E+04			5.16E+04	9.1E-02	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T03-C	1	9.18E+04			9.18E+04	7.7E-01	2.6E+00	8.3E+00	1000	100	9.27E+04	87%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T04-C	1	1.12E+05			1.12E+05	8.1E+00	2.6E+00	8.3E+00					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T05-C	1	1.49E+05			1.49E+05	3.4E-01	2.6E+00	8.3E+00					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T06-C	1	1.63E+05			1.63E+05	1.4E+02	2.6E+00	8.3E+00					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T07-C	1	1.60E+05			1.60E+05	2.5E-01	2.6E+00	8.3E+00					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T08-C	1	1.46E+05			1.46E+05	4.6E-01	2.6E+00	8.3E+00					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-T09-C	1	1.36E+05			1.36E+05	3.9E-01	2.6E+00	8.3E+00					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-B01-A	1	6.32E+00	E		6.32E+00	3.1E+01	2.6E+00	8.3E+00					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-B02-A	1	6.33E+00	E		6.33E+00	8.2E+01	2.6E+00	8.3E+00					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-B03-A	1	3.16E+01			3.16E+01	2.9E+01	2.6E+00	8.3E+00					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-B01-B	1	2.56E+01			2.56E+01	1.1E+01	2.6E+00	8.3E+00					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-B02-B	1	5.69E+00	E		5.69E+00	6.4E+01	2.6E+00	8.3E+00					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-B03-B	1	3.46E+01			3.46E+01	2.9E+01	2.6E+00	8.3E+00					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-B01-C	1	4.79E+01			4.79E+01	2.1E+01	2.6E+00	8.3E+00					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-B02-C	1	8.68E+00			8.68E+00	4.6E+01	2.6E+00	8.3E+00					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1313-B03-C	1	1.30E+00	U1/2		1.30E+00	2.1E+02	2.6E+00	8.3E+00					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	EaFA-L07-1313-T01-A	1	4.03E+02			4.03E+02	3.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T02-A	1	2.71E+02			2.71E+02	4.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T03-A	1	2.23E+02			2.23E+02	3.5E-01	1.2E+00	3.8E+00	10	325	3.40E+03	98%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T04-A	1	1.33E+02			1.33E+02	6.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T05-A	1	4.64E+01			4.64E+01	2.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T06-A	1	9.80E+00			9.80E+00	2.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T07-A	1	6.00E-01	U1/2		6.00E-01	1.3E+02	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T08-A	1	2.47E+02			2.47E+02	2.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T09-A	1	1.75E+03			1.75E+03	2.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T01-B	1	3.93E+02			3.93E+02	6.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T02-B	1	2.95E+02			2.95E+02	4.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T03-B	1	2.21E+02			2.21E+02	6.3E+00	1.2E+00	3.8E+00	10	325	3.37E+03	97%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T04-B	1	1.32E+02			1.32E+02	5.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T05-B	1	4.29E+01			4.29E+01	2.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T06-B	1	1.37E+01			1.37E+01	1.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T07-B	1	6.00E-01	U1/2		6.00E-01	1.4E+03	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T08-B	1	3.64E+02			3.64E+02	1.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T09-B	1	1.73E+03			1.73E+03	1.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T01-C	1	3.65E+02			3.65E+02	7.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T02-C	1	2.55E+02			2.55E+02	2.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T03-C	1	1.98E+02			1.98E+02	1.6E-01	1.2E+00	3.8E+00	10	325	3.25E+03	94%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T04-C	1	1.14E+02			1.14E+02	7.5E+00	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T05-C	1	4.75E+01			4.75E+01	2.6E+00	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T06-C	1	1.33E+01			1.33E+01	1.6E+02	1.2E+00	3.8E+00					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T07-C	1	1.71E+00	E		1.71E+00	5.4E+01	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T08-C	1	2.45E+02			2.45E+02	3.4E-01	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-T09-C	1	1.76E+03			1.76E+03	6.4E-01	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	2.4E+02	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	1.3E+02	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-B03-A	1	3.05E+00	E		3.05E+00	6.1E+01	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-B01-B	1	6.00E-01	U1/2		6.00E-01	2.1E+02	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-B02-B	1	6.00E-01	U1/2		6.00E-01	2.1E+02	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-B03-B	1	1.86E+00	E		1.86E+00	8.9E+01	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-B01-C	1	6.00E-01	U1/2		6.00E-01	6.6E+01	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-B02-C	1	6.00E-01	U1/2		6.00E-01	4.5E+02	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1313-B03-C	1	3.54E+00	E		3.54E+00	4.1E+01	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	EaFA-L07-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	5.4E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	5.7E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00	10	325	3.15E+03	97%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	6.5E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T05-A	1	5.47E+00	E		5.47E+00	5.5E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T06-A	1	7.11E+01			7.11E+01	2.4E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T07-A	1	2.31E+02			2.31E+02	5.1E-01	1.8E+00	5.7E+00			---		VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T08-A	1	1.92E+02			1.92E+02	1.0E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T09-A	1	4.22E+02			4.22E+02	3.3E-01	1.8E+00	5.7E+00			---		VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	5.3E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	3.8E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	9.5E+01	1.8E+00	5.7E+00	10	325	3.65E+03	112%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	1.5E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T05-B	1	1.08E+01			1.08E+01	1.4E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T06-B	1	5.64E+01			5.64E+01	2.6E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T07-B	1	2.42E+02			2.42E+02	6.3E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T08-B	1	2.02E+02			2.02E+02	8.4E-01	1.8E+00	5.7E+00			---		VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T09-B	1	4.01E+02			4.01E+02	7.3E-01	1.8E+00	5.7E+00			---		VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	1.0E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	1.9E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	4.6E+01	1.8E+00	5.7E+00	10	325	3.04E+03	94%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	2.6E+01	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T05-C	1	5.26E+00	E		5.26E+00	5.8E+01	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T06-C	1	5.65E+01			5.65E+01	4.3E+03	1.8E+00	5.7E+00					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T07-C	1	2.27E+02			2.27E+02	6.5E-01	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T08-C	1	1.91E+02			1.91E+02	1.4E+00	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-T09-C	1	3.96E+02			3.96E+02	1.6E-01	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	1.3E+01	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	7.4E+01	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	7.4E+01	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-B01-B	1	9.00E-01	U1/2		9.00E-01	7.0E+01	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-B02-B	1	9.00E-01	U1/2		9.00E-01	6.1E+01	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-B03-B	1	9.00E-01	U1/2		9.00E-01	6.3E+01	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-B01-C	1	9.00E-01	U1/2		9.00E-01	5.3E+01	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-B02-C	1	9.00E-01	U1/2		9.00E-01	2.0E+01	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1313-B03-C	1	9.00E-01	U1/2		9.00E-01	7.6E+01	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	EaFA-L07-1313-T01-A	1	5.29E+00	E		5.29E+00	3.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T02-A	1	7.79E+00	E		7.79E+00	5.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T03-A	1	1.18E+01			1.18E+01	5.1E+00	3.7E+00	1.2E+01	10	325	3.15E+03	96%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T04-A	1	9.28E+00	E		9.28E+00	3.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T05-A	1	1.33E+01			1.33E+01	1.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T06-A	1	1.37E+01			1.37E+01	2.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T07-A	1	2.51E+02			2.51E+02	1.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T08-A	1	1.98E+03			1.98E+03	5.4E-01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T09-A	1	2.92E+03			2.92E+03	1.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T01-B	1	4.30E+01			4.30E+01	1.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T02-B	1	7.85E+00	E		7.85E+00	7.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T03-B	1	1.08E+01	E		1.08E+01	1.7E+01	3.7E+00	1.2E+01	10	325	3.16E+03	97%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T04-B	1	1.12E+01	E		1.12E+01	1.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T05-B	1	1.11E+01	E		1.11E+01	4.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T06-B	1	1.26E+01			1.26E+01	2.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T07-B	1	2.55E+02			2.55E+02	1.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T08-B	1	2.06E+03			2.06E+03	1.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T09-B	1	2.88E+03			2.88E+03	1.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T01-C	1	4.65E+01			4.65E+01	4.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T02-C	1	9.83E+00	E		9.83E+00	8.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T03-C	1	9.53E+00	E		9.53E+00	4.1E+01	3.7E+00	1.2E+01	10	325	3.05E+03	93%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T04-C	1	1.09E+01	E		1.09E+01	5.9E+01	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T05-C	1	1.21E+01			1.21E+01	4.9E+01	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T06-C	1	1.32E+01			1.32E+01	7.2E+01	3.7E+00	1.2E+01					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T07-C	1	2.41E+02			2.41E+02	1.5E+00	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T08-C	1	1.96E+03			1.96E+03	8.5E-01	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-T09-C	1	2.94E+03			2.94E+03	6.7E-01	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	7.5E+01	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	7.1E+01	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-B03-A	1	6.57E+00	E		6.57E+00	4.0E+01	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-B01-B	1	1.85E+00	U1/2		1.85E+00	1.1E+02	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-B02-B	1	1.85E+00	U1/2		1.85E+00	1.6E+02	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-B03-B	1	7.17E+00	E		7.17E+00	7.6E+01	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-B01-C	1	1.85E+00	U1/2		1.85E+00	1.1E+02	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-B02-C	1	1.85E+00	U1/2		1.85E+00	1.4E+02	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1313-B03-C	1	5.92E+00	E		5.92E+00	7.1E+01	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	EaFA-L07-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	9.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T02-A	1	2.77E+01			2.77E+01	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T03-A	1	5.15E+00	E		5.15E+00	5.5E+00	2.0E+00	6.4E+00	1000	100	1.08E+03	107%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	3.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	8.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	2.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T08-A	1	6.20E+02			6.20E+02	8.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T09-A	1	4.14E+04			4.14E+04	2.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T01-B	1	4.11E+01			4.11E+01	5.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T02-B	1	2.71E+01			2.71E+01	2.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T03-B	1	4.77E+00	E		4.77E+00	1.0E+01	2.0E+00	6.4E+00	1000	100	1.06E+03	105%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	5.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	4.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T06-B	1	1.75E+01			1.75E+01	3.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	1.4E+03	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T08-B	1	1.01E+03			1.01E+03	7.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T09-B	1	3.73E+04			3.73E+04	8.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T01-C	1	4.63E+01			4.63E+01	1.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T02-C	1	2.75E+01			2.75E+01	1.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T03-C	1	8.90E+00			8.90E+00	3.1E+00	2.0E+00	6.4E+00	1000	100	1.05E+03	104%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	8.5E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	9.9E+00	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	2.0E+02	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T08-C	1	6.39E+02			6.39E+02	9.6E-01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-T09-C	1	3.77E+04			3.77E+04	2.8E-01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.9E+02	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	4.8E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-B03-A	1	7.74E+00			7.74E+00	1.3E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-B03-B	1	9.59E+00			9.59E+00	3.4E+00	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	3.1E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	3.4E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1313-B03-C	1	9.01E+00			9.01E+00	3.0E+00	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	EaFA-L07-1313-T01-A	1	3.40E+00	U1/2		3.40E+00	5.0E+01	6.8E+00	2.2E+01			---		VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T02-A	1	3.40E+00	U1/2		3.40E+00	5.7E+01	6.8E+00	2.2E+01			---		VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T03-A	1	3.40E+00	U1/2		3.40E+00	1.2E+01	6.8E+00	2.2E+01	10	325	3.09E+03	95%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T04-A	1	3.40E+00	U1/2		3.40E+00	5.7E+01	6.8E+00	2.2E+01			---		VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T05-A	1	3.40E+00	U1/2		3.40E+00	5.2E+01	6.8E+00	2.2E+01			---		VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T06-A	1	3.40E+00	U1/2		3.40E+00	3.2E+01	6.8E+00	2.2E+01			---		VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T07-A	1	3.40E+00	U1/2		3.40E+00	3.9E+01	6.8E+00	2.2E+01			---		VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T08-A	1	3.40E+00	U1/2		3.40E+00	2.1E+01	6.8E+00	2.2E+01			---		VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T09-A	1	1.15E+02			1.15E+02	4.7E+00	6.8E+00	2.2E+01			---		VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T01-B	1	3.40E+00	U1/2		3.40E+00	4.5E+01	6.8E+00	2.2E+01			---		VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T02-B	1	3.40E+00	U1/2		3.40E+00	2.2E+01	6.8E+00	2.2E+01			---		VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T03-B	1	3.40E+00	U1/2		3.40E+00	6.0E+01	6.8E+00	2.2E+01	10	325	3.63E+03	111%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T04-B	1	3.40E+00	U1/2		3.40E+00	2.9E+01	6.8E+00	2.2E+01			---		VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T05-B	1	3.40E+00	U1/2		3.40E+00	3.9E+01	6.8E+00	2.2E+01			---		VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T06-B	1	3.40E+00	U1/2		3.40E+00	6.4E+01	6.8E+00	2.2E+01			---		VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T07-B	1	3.40E+00	U1/2		3.40E+00	4.5E+01	6.8E+00	2.2E+01			---		VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T08-B	1	3.40E+00	U1/2		3.40E+00	1.3E+01	6.8E+00	2.2E+01			---		VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T09-B	1	8.50E+01			8.50E+01	3.8E+00	6.8E+00	2.2E+01			---		VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T01-C	1	3.40E+00	U1/2		3.40E+00	1.7E+02	6.8E+00	2.2E+01			---		VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T02-C	1	3.40E+00	U1/2		3.40E+00	7.9E+00	6.8E+00	2.2E+01			---		VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T03-C	1	3.40E+00	U1/2		3.40E+00	4.5E+01	6.8E+00	2.2E+01	10	325	2.99E+03	92%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T04-C	1	3.40E+00	U1/2		3.40E+00	1.0E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T05-C	1	3.40E+00	U1/2		3.40E+00	1.4E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T06-C	1	3.40E+00	U1/2		3.40E+00	9.7E+00	6.8E+00	2.2E+01					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T07-C	1	3.40E+00	U1/2		3.40E+00	1.3E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T08-C	1	3.40E+00	U1/2		3.40E+00	1.6E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-T09-C	1	8.36E+01			8.36E+01	1.8E+00	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	4.8E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	3.8E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	1.8E+02	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-B01-B	1	3.40E+00	U1/2		3.40E+00	5.4E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-B02-B	1	3.40E+00	U1/2		3.40E+00	3.7E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-B03-B	1	3.40E+00	U1/2		3.40E+00	7.3E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-B01-C	1	3.40E+00	U1/2		3.40E+00	3.0E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-B02-C	1	3.40E+00	U1/2		3.40E+00	6.3E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1313-B03-C	1	3.40E+00	U1/2		3.40E+00	8.7E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	EaFA-L07-1313-T01-A	1	2.15E+03			2.15E+03	8.2E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T02-A	1	2.89E+03			2.89E+03	6.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T03-A	1	3.24E+03			3.24E+03	4.6E-01	1.9E+00	6.0E+00	10	325	6.07E+03	87%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T04-A	1	3.18E+03			3.18E+03	7.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T05-A	1	3.41E+03			3.41E+03	4.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T06-A	1	3.53E+03			3.53E+03	5.9E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T07-A	1	3.33E+03			3.33E+03	8.6E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T08-A	1	2.28E+03			2.28E+03	5.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T09-A	1	1.49E+03			1.49E+03	5.2E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T01-B	1	2.02E+03			2.02E+03	7.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T02-B	1	2.85E+03			2.85E+03	4.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T03-B	1	2.95E+03			2.95E+03	5.7E+00	1.9E+00	6.0E+00	10	325	5.87E+03	90%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T04-B	1	3.21E+03			3.21E+03	5.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T05-B	1	3.55E+03			3.55E+03	3.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T06-B	1	3.57E+03			3.57E+03	3.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T07-B	1	3.46E+03			3.46E+03	3.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T08-B	1	2.17E+03			2.17E+03	3.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T09-B	1	1.48E+03			1.48E+03	2.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T01-C	1	2.14E+03			2.14E+03	1.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T02-C	1	2.81E+03			2.81E+03	7.7E-02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T03-C	1	3.02E+03			3.02E+03	5.4E-01	1.9E+00	6.0E+00	10	325	5.76E+03	84%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T04-C	1	2.81E+03			2.81E+03	1.1E+01	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T05-C	1	3.40E+03			3.40E+03	6.0E-01	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T06-C	1	5.52E+03			5.52E+03	1.3E+02	1.9E+00	6.0E+00					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T07-C	1	3.34E+03			3.34E+03	8.1E-01	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T08-C	1	2.27E+03			2.27E+03	2.3E-01	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-T09-C	1	1.50E+03			1.50E+03	6.8E-01	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-B01-A	1	1.52E+01			1.52E+01	7.1E+00	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-B02-A	1	1.51E+01			1.51E+01	9.1E+00	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-B03-A	1	1.45E+01			1.45E+01	7.5E+00	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-B01-B	1	1.56E+01			1.56E+01	8.4E+00	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-B02-B	1	1.39E+01			1.39E+01	8.8E+00	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-B03-B	1	1.75E+01			1.75E+01	3.4E+00	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-B01-C	1	1.44E+01			1.44E+01	6.1E+00	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-B02-C	1	1.58E+01			1.58E+01	1.0E+00	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1313-B03-C	1	1.73E+01			1.73E+01	3.7E+00	1.9E+00	6.0E+00					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	EaFA-L07-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	2.9E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	5.1E+01	2.0E+00	6.4E+00	10	325	3.21E+03	99%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	5.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T05-A	1	9.43E+01			9.43E+01	1.5E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T06-A	1	4.67E+02			4.67E+02	5.8E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T07-A	1	8.76E+02			8.76E+02	6.6E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T08-A	1	1.15E+03			1.15E+03	6.5E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T09-A	1	1.69E+03			1.69E+03	1.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	4.9E+01	2.0E+00	6.4E+00	10	325	3.16E+03	97%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T04-B	1	6.50E+00			6.50E+00	6.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T05-B	1	1.51E+02			1.51E+02	5.5E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T06-B	1	4.24E+02			4.24E+02	1.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T07-B	1	8.83E+02			8.83E+02	5.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T08-B	1	1.19E+03			1.19E+03	5.1E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T09-B	1	1.65E+03			1.65E+03	8.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	4.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	2.9E+01	2.0E+00	6.4E+00	10	325	3.11E+03	96%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T05-C	1	8.83E+01			8.83E+01	2.8E-01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T06-C	1	3.93E+02			3.93E+02	1.4E+02	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T07-C	1	8.70E+02			8.70E+02	1.1E+00	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T08-C	1	1.15E+03			1.15E+03	4.8E-01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-T09-C	1	1.65E+03			1.65E+03	3.7E-01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	3.3E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	8.8E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	2.4E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	1.0E+02	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	5.6E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1313-B03-C	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	EaFA-L07-1313-T01-A	1	5.00E-01	U1/2		5.00E-01	1.1E+03	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T02-A	1	5.00E-01	U1/2		5.00E-01	1.3E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T03-A	1	1.31E+02			1.31E+02	4.4E+00	1.0E+00	3.2E+00	1000	100	1.16E+03	103%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T04-A	1	3.21E+03			3.21E+03	7.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T05-A	1	6.21E+03			6.21E+03	9.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T06-A	1	7.59E+03			7.59E+03	2.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T07-A	1	8.63E+03			8.63E+03	9.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T08-A	1	8.12E+03			8.12E+03	5.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T09-A	1	1.49E+04			1.49E+04	8.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T01-B	1	5.00E-01	U1/2		5.00E-01	1.7E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T02-B	1	5.00E-01	U1/2		5.00E-01	1.2E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T03-B	1	1.36E+02			1.36E+02	2.1E+00	1.0E+00	3.2E+00	1000	100	1.08E+03	94%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T04-B	1	3.44E+03			3.44E+03	5.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T05-B	1	7.03E+03			7.03E+03	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T06-B	1	7.75E+03			7.75E+03	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T07-B	1	8.86E+03			8.86E+03	2.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T08-B	1	8.55E+03			8.55E+03	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T09-B	1	1.44E+04			1.44E+04	2.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T01-C	1	5.00E-01	U1/2		5.00E-01	5.9E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T02-C	1	5.00E-01	U1/2		5.00E-01	3.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T03-C	1	1.11E+02			1.11E+02	7.1E+00	1.0E+00	3.2E+00	1000	100	1.10E+03	99%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T04-C	1	2.80E+03			2.80E+03	4.3E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T05-C	1	6.14E+03			6.14E+03	5.1E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T06-C	1	7.52E+03			7.52E+03	1.4E+02	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T07-C	1	8.66E+03			8.66E+03	1.7E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T08-C	1	8.08E+03			8.08E+03	5.0E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-T09-C	1	1.44E+04			1.44E+04	5.4E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.4E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	9.9E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-B03-A	1	6.25E+00			6.25E+00	1.4E+02	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	3.8E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	4.6E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	5.6E+02	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	4.3E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	8.4E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	2.6E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	EaFA-L07-1313-T01-A	1	4.06E+03			4.06E+03	4.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T02-A	1	4.12E+03			4.12E+03	9.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T03-A	1	4.13E+03			4.13E+03	5.7E-01	1.2E+00	3.8E+00	10	325	6.92E+03	86%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T04-A	1	3.79E+03			3.79E+03	4.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T05-A	1	3.68E+03			3.68E+03	7.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T06-A	1	3.12E+03			3.12E+03	6.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T07-A	1	2.94E+02			2.94E+02	7.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T08-A	1	1.27E+02			1.27E+02	3.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T09-A	1	4.80E+02			4.80E+02	4.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T01-B	1	3.70E+03			3.70E+03	7.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T02-B	1	4.01E+03			4.01E+03	4.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T03-B	1	3.72E+03			3.72E+03	6.1E+00	1.2E+00	3.8E+00	10	325	7.17E+03	106%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T04-B	1	3.62E+03			3.62E+03	4.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T05-B	1	3.63E+03			3.63E+03	6.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T06-B	1	3.17E+03			3.17E+03	1.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T07-B	1	3.12E+02			3.12E+02	6.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T08-B	1	1.21E+02			1.21E+02	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T09-B	1	3.61E+02			3.61E+02	7.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T01-C	1	4.03E+03			4.03E+03	2.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T02-C	1	4.01E+03			4.01E+03	7.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T03-C	1	3.89E+03			3.89E+03	7.4E-01	1.2E+00	3.8E+00	10	325	6.73E+03	87%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T04-C	1	3.36E+03			3.36E+03	5.6E+00	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T05-C	1	3.68E+03			3.68E+03	7.8E-01	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T06-C	1	3.49E+03			3.49E+03	1.5E+02	1.2E+00	3.8E+00					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T07-C	1	3.16E+02			3.16E+02	4.1E-01	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T08-C	1	1.29E+02			1.29E+02	1.1E+00	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-T09-C	1	4.06E+02			4.06E+02	6.1E-01	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	1.4E+02	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	7.6E+01	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-B03-A	1	6.00E-01	U1/2		6.00E-01	9.7E+01	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-B01-B	1	6.00E-01	U1/2		6.00E-01	3.7E+01	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-B02-B	1	6.00E-01	U1/2		6.00E-01	2.6E+02	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-B03-B	1	2.49E+00	E		2.49E+00	7.6E+01	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-B01-C	1	6.00E-01	U1/2		6.00E-01	2.5E+02	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-B02-C	1	1.60E+00	E		1.60E+00	1.4E+02	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1313-B03-C	1	2.01E+00	E		2.01E+00	2.0E+02	1.2E+00	3.8E+00					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	EaFA-L07-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	2.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	3.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	2.3E+03	1.8E+00	5.7E+00	10	325	3.15E+03	97%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	5.2E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T05-A	1	2.28E+01			2.28E+01	5.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T06-A	1	1.60E+02			1.60E+02	8.4E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T07-A	1	5.93E+02			5.93E+02	1.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T08-A	1	4.81E+02			4.81E+02	1.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T09-A	1	7.34E+02			7.34E+02	1.4E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	1.1E+03	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	2.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	8.4E+01	1.8E+00	5.7E+00	10	325	3.15E+03	97%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T04-B	1	4.32E+00	E		4.32E+00	1.9E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T05-B	1	4.49E+01			4.49E+01	3.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T06-B	1	1.36E+02			1.36E+02	3.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T07-B	1	6.15E+02			6.15E+02	5.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T08-B	1	4.85E+02			4.85E+02	3.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T09-B	1	7.12E+02			7.12E+02	1.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	9.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	2.6E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	2.3E+02	1.8E+00	5.7E+00	10	325	3.03E+03	93%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	3.6E+02	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T05-C	1	2.30E+01			2.30E+01	1.9E+01	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T06-C	1	1.27E+02			1.27E+02	1.8E+02	1.8E+00	5.7E+00					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T07-C	1	5.87E+02			5.87E+02	7.6E-01	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T08-C	1	4.77E+02			4.77E+02	5.8E-01	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-T09-C	1	7.03E+02			7.03E+02	2.5E-01	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	2.4E+01	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	4.5E+02	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	4.9E+02	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-B01-B	1	9.00E-01	U1/2		9.00E-01	1.9E+02	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-B02-B	1	9.00E-01	U1/2		9.00E-01	3.8E+02	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-B03-B	1	3.51E+00	E		3.51E+00	1.8E+02	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-B01-C	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-B02-C	1	9.00E-01	U1/2		9.00E-01	1.0E+02	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1313-B03-C	1	2.25E+00	E		2.25E+00	1.8E+02	1.8E+00	5.7E+00					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	EaFA-L07-1313-T01-A	1	6.82E+01			6.82E+01	1.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T02-A	1	5.03E+01			5.03E+01	7.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T03-A	1	6.60E+01			6.60E+01	7.7E+00	3.7E+00	1.2E+01	1000	100	1.04E+03	98%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T04-A	1	1.01E+02			1.01E+02	9.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T05-A	1	5.44E+01			5.44E+01	7.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T06-A	1	2.99E+01			2.99E+01	3.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T07-A	1	4.21E+01			4.21E+01	8.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T08-A	1	5.73E+01			5.73E+01	9.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T09-A	1	3.54E+03			3.54E+03	3.5E-01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T01-B	1	9.59E+01			9.59E+01	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T02-B	1	5.09E+01			5.09E+01	2.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T03-B	1	6.56E+01			6.56E+01	1.6E+01	3.7E+00	1.2E+01	1000	100	1.10E+03	104%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T04-B	1	9.33E+01			9.33E+01	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T05-B	1	5.18E+01			5.18E+01	1.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T06-B	1	3.69E+01			3.69E+01	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T07-B	1	4.65E+01			4.65E+01	1.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T08-B	1	7.09E+01			7.09E+01	6.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T09-B	1	2.42E+03			2.42E+03	1.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T01-C	1	1.16E+02			1.16E+02	1.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T02-C	1	4.41E+01			4.41E+01	1.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T03-C	1	6.36E+01			6.36E+01	2.1E+01	3.7E+00	1.2E+01	1000	100	1.01E+03	95%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T04-C	1	8.09E+01			8.09E+01	1.3E+01	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T05-C	1	5.29E+01			5.29E+01	1.3E+01	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T06-C	1	1.74E+01			1.74E+01	1.7E+02	3.7E+00	1.2E+01					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T07-C	1	4.38E+01			4.38E+01	2.7E+01	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T08-C	1	6.72E+01			6.72E+01	5.3E+00	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-T09-C	1	2.73E+03			2.73E+03	6.6E-01	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	3.0E+02	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-B02-A	1	1.51E+01			1.51E+01	3.1E+01	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-B03-A	1	1.36E+01			1.36E+01	5.7E+01	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-B01-B	1	8.52E+00	E		8.52E+00	9.1E+01	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-B02-B	1	6.56E+00	E		6.56E+00	1.2E+02	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-B03-B	1	2.02E+01			2.02E+01	4.7E+01	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-B01-C	1	5.31E+00	E		5.31E+00	1.3E+02	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-B02-C	1	3.86E+00	E		3.86E+00	1.0E+02	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1313-B03-C	1	1.85E+00	U1/2		1.85E+00	4.2E+02	3.7E+00	1.2E+01					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	EaFA-L07-1313-T01-A	1	5.04E+04			5.04E+04	7.6E-01	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T02-A	1	3.46E+04			3.46E+04	1.7E-01	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T03-A	1	2.91E+04			2.91E+04	5.9E-01	1.6E+00	5.1E+00	1000	100	3.01E+04	95%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T04-A	1	2.61E+04			2.61E+04	6.0E+00	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T05-A	1	2.58E+04			2.58E+04	1.4E-01	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T06-A	1	2.64E+04			2.64E+04	9.9E-01	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T07-A	1	2.64E+04			2.64E+04	7.7E-01	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T08-A	1	1.95E+04			1.95E+04	8.9E-01	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T09-A	1	2.38E+04			2.38E+04	4.9E-01	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T01-B	1	4.73E+04			4.73E+04	8.0E+00	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T02-B	1	3.42E+04			3.42E+04	9.7E-01	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T03-B	1	2.64E+04			2.64E+04	6.6E+00	1.6E+00	5.1E+00	1000	100	2.74E+04	92%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T04-B	1	2.59E+04			2.59E+04	5.6E+00	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T05-B	1	2.68E+04			2.68E+04	9.4E-01	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T06-B	1	2.68E+04			2.68E+04	2.3E-01	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T07-B	1	2.74E+04			2.74E+04	4.8E+00	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T08-B	1	1.92E+04			1.92E+04	5.7E-01	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T09-B	1	2.31E+04			2.31E+04	2.1E+00	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T01-C	1	5.09E+04			5.09E+04	1.1E+00	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T02-C	1	3.37E+04			3.37E+04	2.3E-01	1.6E+00	5.1E+00			---		VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T03-C	1	2.72E+04			2.72E+04	1.2E-01	1.6E+00	5.1E+00	1000	100	2.81E+04	89%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T04-C	1	2.28E+04			2.28E+04	9.4E+00	1.6E+00	5.1E+00					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T05-C	1	2.55E+04			2.55E+04	1.6E-01	1.6E+00	5.1E+00					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T06-C	1	2.35E+04			2.35E+04	1.4E+02	1.6E+00	5.1E+00					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T07-C	1	2.64E+04			2.64E+04	9.6E-01	1.6E+00	5.1E+00					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T08-C	1	1.96E+04			1.96E+04	6.0E-01	1.6E+00	5.1E+00					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-T09-C	1	2.29E+04			2.29E+04	3.3E-01	1.6E+00	5.1E+00					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-B01-A	1	1.18E+01			1.18E+01	5.1E+01	1.6E+00	5.1E+00					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-B02-A	1	9.73E+00			9.73E+00	1.1E+01	1.6E+00	5.1E+00					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-B03-A	1	1.93E+02			1.93E+02	5.3E+00	1.6E+00	5.1E+00					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-B01-B	1	1.43E+01			1.43E+01	2.7E+01	1.6E+00	5.1E+00					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-B02-B	1	1.30E+01			1.30E+01	2.2E+01	1.6E+00	5.1E+00					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-B03-B	1	1.94E+02			1.94E+02	2.8E+00	1.6E+00	5.1E+00					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-B01-C	1	1.31E+01			1.31E+01	9.0E+00	1.6E+00	5.1E+00					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-B02-C	1	1.25E+01			1.25E+01	2.1E+01	1.6E+00	5.1E+00					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1313-B03-C	1	1.84E+02			1.84E+02	3.2E+00	1.6E+00	5.1E+00					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	EaFA-L07-1313-T01-A	1	6.65E+03			6.65E+03	1.2E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T02-A	1	5.62E+03			5.62E+03	1.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T03-A	1	5.06E+03			5.06E+03	7.4E-01	1.5E+01	4.8E+01	10	325	7.83E+03	85%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T04-A	1	3.29E+03			3.29E+03	6.2E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T05-A	1	1.63E+03			1.63E+03	1.0E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T06-A	1	9.35E+02			9.35E+02	1.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T07-A	1	1.81E+02			1.81E+02	2.1E+01	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T08-A	1	8.34E+01			8.34E+01	1.0E+01	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T09-A	1	9.27E+02			9.27E+02	1.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T01-B	1	6.42E+03			6.42E+03	7.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T02-B	1	5.71E+03			5.71E+03	2.2E-01	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T03-B	1	4.77E+03			4.77E+03	5.8E+00	1.5E+01	4.8E+01	10	325	7.60E+03	87%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T04-B	1	2.84E+03			2.84E+03	4.0E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T05-B	1	1.56E+03			1.56E+03	1.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T06-B	1	1.01E+03			1.01E+03	2.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T07-B	1	1.70E+02			1.70E+02	1.3E+01	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T08-B	1	3.66E+01	E		3.66E+01	6.7E+01	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T09-B	1	6.14E+02			6.14E+02	2.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T01-C	1	6.66E+03			6.66E+03	1.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T02-C	1	5.49E+03			5.49E+03	1.8E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T03-C	1	4.71E+03			4.71E+03	3.2E-01	1.5E+01	4.8E+01	10	325	7.46E+03	85%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T04-C	1	2.95E+03			2.95E+03	8.6E+00	1.5E+01	4.8E+01					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T05-C	1	1.81E+03			1.81E+03	9.2E-01	1.5E+01	4.8E+01					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T06-C	1	1.13E+03			1.13E+03	1.7E+02	1.5E+01	4.8E+01					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T07-C	1	1.77E+02			1.77E+02	1.4E+01	1.5E+01	4.8E+01					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T08-C	1	9.43E+01			9.43E+01	1.5E+01	1.5E+01	4.8E+01					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-T09-C	1	7.16E+02			7.16E+02	3.3E+00	1.5E+01	4.8E+01					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-B01-A	1	7.50E+00	U1/2		7.50E+00	1.1E+02	1.5E+01	4.8E+01					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-B02-A	1	7.50E+00	U1/2		7.50E+00	1.3E+02	1.5E+01	4.8E+01					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-B03-A	1	7.50E+00	U1/2		7.50E+00	1.3E+02	1.5E+01	4.8E+01					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-B01-B	1	7.50E+00	U1/2		7.50E+00	2.0E+02	1.5E+01	4.8E+01					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-B02-B	1	7.50E+00	U1/2		7.50E+00	1.3E+03	1.5E+01	4.8E+01					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-B03-B	1	7.50E+00	U1/2		7.50E+00	3.3E+02	1.5E+01	4.8E+01					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-B01-C	1	7.50E+00	U1/2		7.50E+00	6.7E+02	1.5E+01	4.8E+01					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-B02-C	1	7.50E+00	U1/2		7.50E+00	2.5E+01	1.5E+01	4.8E+01					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1313-B03-C	1	7.50E+00	U1/2		7.50E+00	5.5E+02	1.5E+01	4.8E+01					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	EaFA-L07-1313-T01-A	1	1.30E+03			1.30E+03	3.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T02-A	1	3.49E+03			3.49E+03	2.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T03-A	1	1.16E+03			1.16E+03	4.9E-01	1.1E+00	3.5E+00	1000	100	2.10E+03	95%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T04-A	1	3.64E+02			3.64E+02	6.7E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T05-A	1	1.07E+03			1.07E+03	3.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T06-A	1	2.78E+03			2.78E+03	4.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T07-A	1	6.69E+03			6.69E+03	1.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T08-A	1	2.31E+04			2.31E+04	1.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T09-A	1	7.03E+04			7.03E+04	3.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T01-B	1	9.02E+03			9.02E+03	7.4E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T02-B	1	3.39E+03			3.39E+03	4.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T03-B	1	9.45E+02			9.45E+02	5.4E+00	1.1E+00	3.5E+00	1000	100	1.96E+03	102%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T04-B	1	4.45E+02			4.45E+02	5.9E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T05-B	1	1.40E+03			1.40E+03	9.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T06-B	1	2.53E+03			2.53E+03	1.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T07-B	1	6.79E+03			6.79E+03	5.5E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T08-B	1	2.79E+04			2.79E+04	1.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T09-B	1	6.85E+04			6.85E+04	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T01-C	1	9.86E+03			9.86E+03	8.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T02-C	1	3.64E+03			3.64E+03	3.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T03-C	1	1.28E+03			1.28E+03	5.7E-02	1.1E+00	3.5E+00	1000	100	2.19E+03	91%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T04-C	1	3.49E+02			3.49E+02	1.1E+01	1.1E+00	3.5E+00					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T05-C	1	1.21E+03			1.21E+03	5.1E-01	1.1E+00	3.5E+00					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T06-C	1	2.60E+03			2.60E+03	1.5E+02	1.1E+00	3.5E+00					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T07-C	1	6.85E+03			6.85E+03	8.8E-01	1.1E+00	3.5E+00					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T08-C	1	2.32E+04			2.32E+04	3.5E-01	1.1E+00	3.5E+00					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-T09-C	1	6.88E+04			6.88E+04	5.7E-01	1.1E+00	3.5E+00					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-B01-A	1	4.05E+01			4.05E+01	2.0E+02	1.1E+00	3.5E+00					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-B02-A	1	5.50E-01	U1/2		5.50E-01	3.4E+01	1.1E+00	3.5E+00					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-B03-A	1	5.50E-01	U1/2		5.50E-01	1.2E+03	1.1E+00	3.5E+00					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-B01-B	1	5.50E-01	U1/2		5.50E-01	5.4E+01	1.1E+00	3.5E+00					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-B02-B	1	5.50E-01	U1/2		5.50E-01	2.9E+02	1.1E+00	3.5E+00					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-B03-B	1	5.67E+00			5.67E+00	5.5E+01	1.1E+00	3.5E+00					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-B01-C	1	5.50E-01	U1/2		5.50E-01	5.7E+01	1.1E+00	3.5E+00					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-B02-C	1	5.50E-01	U1/2		5.50E-01	2.4E+02	1.1E+00	3.5E+00					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1313-B03-C	1	1.67E+00	E		1.67E+00	2.2E+02	1.1E+00	3.5E+00					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	EaFA-L07-1313-T01-A	1	3.26E+05			3.26E+05	2.4E-02	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T02-A	1	1.22E+05			1.22E+05	6.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T03-A	1	5.43E+04			5.43E+04	3.9E-01	2.5E+00	8.0E+00	1000	100	5.52E+04	90%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T04-A	1	2.84E+04			2.84E+04	6.4E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T05-A	1	1.28E+04			1.28E+04	6.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T06-A	1	5.38E+03			5.38E+03	8.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T07-A	1	5.14E+03			5.14E+03	3.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T08-A	1	3.74E+03			3.74E+03	1.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T09-A	1	3.11E+03			3.11E+03	4.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T01-B	1	2.96E+05			2.96E+05	4.6E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T02-B	1	1.19E+05			1.19E+05	3.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T03-B	1	4.98E+04			4.98E+04	5.2E+00	2.5E+00	8.0E+00	1000	100	5.10E+04	111%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T04-B	1	2.37E+04			2.37E+04	5.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T05-B	1	1.10E+04			1.10E+04	4.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T06-B	1	5.43E+03			5.43E+03	3.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T07-B	1	5.37E+03			5.37E+03	4.6E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T08-B	1	3.62E+03			3.62E+03	2.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T09-B	1	3.05E+03			3.05E+03	2.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T01-C	1	3.03E+05			3.03E+05	9.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T02-C	1	1.19E+05			1.19E+05	2.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T03-C	1	5.15E+04			5.15E+04	8.5E-01	2.5E+00	8.0E+00	1000	100	5.25E+04	95%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T04-C	1	2.52E+04			2.52E+04	1.0E+01	2.5E+00	8.0E+00					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T05-C	1	1.28E+04			1.28E+04	1.5E-01	2.5E+00	8.0E+00					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T06-C	1	5.42E+03			5.42E+03	1.3E+02	2.5E+00	8.0E+00					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T07-C	1	5.21E+03			5.21E+03	1.0E+00	2.5E+00	8.0E+00					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T08-C	1	3.72E+03			3.72E+03	4.5E-01	2.5E+00	8.0E+00					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-T09-C	1	3.11E+03			3.11E+03	1.1E+00	2.5E+00	8.0E+00					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-B01-A	1	3.85E+00	E		3.85E+00	2.7E+00	2.5E+00	8.0E+00					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-B02-A	1	3.36E+00	E		3.36E+00	1.4E+01	2.5E+00	8.0E+00					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-B03-A	1	3.09E+05			3.09E+05	3.3E+00	2.5E+00	8.0E+00					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-B01-B	1	5.64E+00	E		5.64E+00	7.1E+00	2.5E+00	8.0E+00					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-B02-B	1	3.82E+00	E		3.82E+00	2.2E+00	2.5E+00	8.0E+00					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-B03-B	1	3.20E+05			3.20E+05	1.4E-01	2.5E+00	8.0E+00					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-B01-C	1	3.79E+00	E		3.79E+00	1.0E+01	2.5E+00	8.0E+00					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-B02-C	1	3.42E+00	E		3.42E+00	7.3E+00	2.5E+00	8.0E+00					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1313-B03-C	1	3.16E+05			3.16E+05	2.5E-01	2.5E+00	8.0E+00					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	EaFA-L07-1313-T01-A	1	1.07E+03			1.07E+03	2.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T02-A	1	1.71E+03			1.71E+03	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T03-A	1	1.85E+03			1.85E+03	7.8E-01	1.0E+00	3.2E+00	1000	100	2.71E+03	86%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T04-A	1	1.91E+03			1.91E+03	4.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T05-A	1	2.09E+03			2.09E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T06-A	1	2.23E+03			2.23E+03	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T07-A	1	2.72E+03			2.72E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T08-A	1	3.27E+03			3.27E+03	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T09-A	1	5.56E+03			5.56E+03	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T01-B	1	1.38E+03			1.38E+03	7.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T02-B	1	1.71E+03			1.71E+03	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T03-B	1	1.72E+03			1.72E+03	6.7E+00	1.0E+00	3.2E+00	1000	100	2.68E+03	96%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T04-B	1	1.91E+03			1.91E+03	4.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T05-B	1	2.19E+03			2.19E+03	2.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T06-B	1	2.25E+03			2.25E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T07-B	1	2.80E+03			2.80E+03	5.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T08-B	1	3.53E+03			3.53E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T09-B	1	5.37E+03			5.37E+03	3.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T01-C	1	1.40E+03			1.40E+03	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T02-C	1	1.64E+03			1.64E+03	9.6E-02	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T03-C	1	1.73E+03			1.73E+03	5.8E-01	1.0E+00	3.2E+00	1000	100	2.59E+03	87%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T04-C	1	1.68E+03			1.68E+03	5.6E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T05-C	1	2.08E+03			2.08E+03	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T06-C	1	2.23E+03			2.23E+03	1.5E+02	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T07-C	1	2.71E+03			2.71E+03	1.0E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T08-C	1	3.26E+03			3.26E+03	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-T09-C	1	5.41E+03			5.41E+03	3.9E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.6E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	7.2E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	1.9E+02	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	3.9E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	1.8E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	2.7E+02	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	1.7E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	4.9E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	9.4E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	EaFA-L07-1313-T01-A	1	1.83E+05			1.83E+05	6.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T02-A	1	1.76E+05			1.76E+05	3.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T03-A	1	1.74E+05			1.74E+05	3.2E-01	6.8E+00	2.2E+01	1000	100	1.75E+05	91%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T04-A	1	1.65E+05			1.65E+05	6.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T05-A	1	1.69E+05			1.69E+05	6.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T06-A	1	1.67E+05			1.67E+05	6.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T07-A	1	1.43E+05			1.43E+05	7.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T08-A	1	1.03E+05			1.03E+05	7.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T09-A	1	6.13E+04			6.13E+04	2.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T01-B	1	1.73E+05			1.73E+05	7.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T02-B	1	1.73E+05			1.73E+05	4.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T03-B	1	1.62E+05			1.62E+05	5.9E+00	6.8E+00	2.2E+01	1000	100	1.63E+05	87%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T04-B	1	1.65E+05			1.65E+05	4.8E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T05-B	1	1.72E+05			1.72E+05	2.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T06-B	1	1.69E+05			1.69E+05	2.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T07-B	1	1.49E+05			1.49E+05	5.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T08-B	1	9.81E+04			9.81E+04	3.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T09-B	1	6.11E+04			6.11E+04	9.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T01-C	1	1.86E+05			1.86E+05	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T02-C	1	1.71E+05			1.71E+05	2.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T03-C	1	1.65E+05			1.65E+05	3.2E-01	6.8E+00	2.2E+01	1000	100	1.66E+05	91%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T04-C	1	1.47E+05			1.47E+05	9.3E+00	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T05-C	1	1.68E+05			1.68E+05	4.7E-01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T06-C	1	1.58E+05			1.58E+05	1.4E+02	6.8E+00	2.2E+01					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T07-C	1	1.45E+05			1.45E+05	8.3E-01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T08-C	1	1.03E+05			1.03E+05	6.0E-01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-T09-C	1	6.27E+04			6.27E+04	4.0E-01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	3.5E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	3.4E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-B03-A	1	8.89E+00	E		8.89E+00	1.0E+02	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-B01-B	1	3.40E+00	U1/2		3.40E+00	6.7E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-B02-B	1	3.40E+00	U1/2		3.40E+00	2.8E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-B03-B	1	3.40E+00	U1/2		3.40E+00	4.6E+02	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-B01-C	1	3.40E+00	U1/2		3.40E+00	3.0E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-B02-C	1	3.40E+00	U1/2		3.40E+00	7.2E+01	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1313-B03-C	1	7.46E+00	E		7.46E+00	1.4E+02	6.8E+00	2.2E+01					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	EaFA-L07-1313-T01-A	1	2.30E+00	U1/2		2.30E+00	4.2E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T02-A	1	2.30E+00	U1/2		2.30E+00	2.0E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T03-A	1	2.30E+00	U1/2		2.30E+00	5.6E+01	4.6E+00	1.5E+01	10	325	3.03E+03	93%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T04-A	1	2.30E+00	U1/2		2.30E+00	1.2E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T05-A	1	2.30E+00	U1/2		2.30E+00	5.9E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T06-A	1	2.30E+00	U1/2		2.30E+00	1.1E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T07-A	1	2.52E+01			2.52E+01	2.8E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T08-A	1	3.02E+01			3.02E+01	2.1E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T09-A	1	7.15E+01			7.15E+01	5.9E+00	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T01-B	1	2.30E+00	U1/2		2.30E+00	4.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T02-B	1	2.30E+00	U1/2		2.30E+00	9.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T03-B	1	2.30E+00	U1/2		2.30E+00	6.4E+01	4.6E+00	1.5E+01	10	325	3.53E+03	109%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T04-B	1	2.30E+00	U1/2		2.30E+00	5.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T05-B	1	2.30E+00	U1/2		2.30E+00	4.2E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T06-B	1	2.30E+00	U1/2		2.30E+00	1.2E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T07-B	1	2.04E+01			2.04E+01	3.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T08-B	1	4.26E+01			4.26E+01	3.4E+00	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T09-B	1	6.97E+01			6.97E+01	5.2E+00	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T01-C	1	2.30E+00	U1/2		2.30E+00	2.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T02-C	1	2.30E+00	U1/2		2.30E+00	3.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T03-C	1	2.30E+00	U1/2		2.30E+00	2.9E+01	4.6E+00	1.5E+01	10	325	2.95E+03	91%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T04-C	1	2.30E+00	U1/2		2.30E+00	1.0E+02	4.6E+00	1.5E+01					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T05-C	1	2.30E+00	U1/2		2.30E+00	8.8E+01	4.6E+00	1.5E+01					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T06-C	1	2.30E+00	U1/2		2.30E+00	8.7E+00	4.6E+00	1.5E+01					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T07-C	1	2.33E+01			2.33E+01	2.8E+01	4.6E+00	1.5E+01					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T08-C	1	3.50E+01			3.50E+01	5.2E+00	4.6E+00	1.5E+01					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-T09-C	1	7.37E+01			7.37E+01	7.1E+00	4.6E+00	1.5E+01					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	2.2E+00	4.6E+00	1.5E+01					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	8.8E+00	4.6E+00	1.5E+01					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	1.9E+02	4.6E+00	1.5E+01					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-B01-B	1	2.30E+00	U1/2		2.30E+00	4.0E+01	4.6E+00	1.5E+01					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-B02-B	1	2.30E+00	U1/2		2.30E+00	9.2E+01	4.6E+00	1.5E+01					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-B03-B	1	2.30E+00	U1/2		2.30E+00	5.7E+01	4.6E+00	1.5E+01					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-B01-C	1	2.30E+00	U1/2		2.30E+00	5.5E+01	4.6E+00	1.5E+01					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-B02-C	1	2.30E+00	U1/2		2.30E+00	4.6E+01	4.6E+00	1.5E+01					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1313-B03-C	1	2.30E+00	U1/2		2.30E+00	2.8E+02	4.6E+00	1.5E+01					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	EaFA-L07-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	9.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	6.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	2.6E+02	2.0E+00	6.4E+00	10	325	3.18E+03	98%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	2.3E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	5.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	2.5E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T08-A	1	1.47E+01			1.47E+01	4.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T09-A	1	6.14E+03			6.14E+03	5.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T01-B	1	2.03E+00	E		2.03E+00	1.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	7.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	3.9E+01	2.0E+00	6.4E+00	10	325	3.16E+03	97%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	9.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	1.5E+03	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T06-B	1	7.91E+00			7.91E+00	1.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T08-B	1	1.72E+01			1.72E+01	5.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T09-B	1	3.23E+03			3.23E+03	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	3.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	1.9E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	4.2E+02	2.0E+00	6.4E+00	10	325	3.08E+03	95%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	6.9E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	2.2E+02	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	1.7E+02	2.0E+00	6.4E+00					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T08-C	1	1.38E+01			1.38E+01	6.1E-01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-T09-C	1	3.80E+03			3.80E+03	4.5E-01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	6.7E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	7.6E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	6.4E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	2.9E+02	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-B02-B	1	2.43E+00	E		2.43E+00	1.9E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	1.4E+04	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	5.3E+02	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1313-B03-C	1	1.00E+00	U1/2		1.00E+00	3.2E+01	2.0E+00	6.4E+00					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	EaFA-L07-1313-T01-A	1	4.41E+03			4.41E+03	1.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T02-A	1	2.63E+03			2.63E+03	1.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T03-A	1	2.89E+03			2.89E+03	1.2E+00	1.5E+00	4.8E+00	10	325	5.88E+03	92%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T04-A	1	7.98E+02			7.98E+02	5.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T05-A	1	3.53E+02			3.53E+02	7.4E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T06-A	1	2.09E+02			2.09E+02	1.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T07-A	1	7.11E+01			7.11E+01	2.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T08-A	1	9.92E+01			9.92E+01	2.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T09-A	1	6.09E+03			6.09E+03	2.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T01-B	1	4.00E+03			4.00E+03	6.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T02-B	1	2.54E+03			2.54E+03	9.0E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T03-B	1	2.52E+03			2.52E+03	6.3E+00	1.5E+00	4.8E+00	10	325	5.53E+03	93%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T04-B	1	5.08E+02			5.08E+02	5.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T05-B	1	2.97E+02			2.97E+02	1.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T06-B	1	2.21E+02			2.21E+02	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T07-B	1	7.29E+01			7.29E+01	7.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T08-B	1	1.02E+02			1.02E+02	2.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T09-B	1	5.92E+03			5.92E+03	2.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T01-C	1	4.29E+03			4.29E+03	2.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T02-C	1	2.62E+03			2.62E+03	2.4E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T03-C	1	2.88E+03			2.88E+03	6.7E-01	1.5E+00	4.8E+00	10	325	5.82E+03	90%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T04-C	1	7.34E+02			7.34E+02	6.3E+00	1.5E+00	4.8E+00					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T05-C	1	3.85E+02			3.85E+02	1.0E+00	1.5E+00	4.8E+00					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T06-C	1	2.91E+02			2.91E+02	1.5E+02	1.5E+00	4.8E+00					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T07-C	1	7.31E+01			7.31E+01	3.2E+00	1.5E+00	4.8E+00					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T08-C	1	9.91E+01			9.91E+01	1.3E+00	1.5E+00	4.8E+00					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-T09-C	1	6.04E+03			6.04E+03	3.5E-01	1.5E+00	4.8E+00					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-B01-A	1	7.50E-01	U1/2		7.50E-01	6.3E+01	1.5E+00	4.8E+00					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-B02-A	1	7.50E-01	U1/2		7.50E-01	4.6E+02	1.5E+00	4.8E+00					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-B03-A	1	7.50E-01	U1/2		7.50E-01	1.5E+02	1.5E+00	4.8E+00					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-B01-B	1	7.50E-01	U1/2		7.50E-01	1.6E+02	1.5E+00	4.8E+00					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-B02-B	1	7.50E-01	U1/2		7.50E-01	4.5E+02	1.5E+00	4.8E+00					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-B03-B	1	7.50E-01	U1/2		7.50E-01	4.6E+03	1.5E+00	4.8E+00					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-B01-C	1	7.50E-01	U1/2		7.50E-01	1.2E+02	1.5E+00	4.8E+00					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-B02-C	1	7.50E-01	U1/2		7.50E-01	5.3E+01	1.5E+00	4.8E+00					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1313-B03-C	1	7.50E-01	U1/2		7.50E-01	2.3E+01	1.5E+00	4.8E+00					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	EaFA-L07-1313-T01-A	1	1.37E+00	E		1.37E+00	3.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:17 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T02-A	1	4.01E+00			4.01E+00	2.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 1:56 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T03-A	1	5.00E-01	U1/2		5.00E-01	3.5E+02	1.0E+00	3.2E+00	10	325	3.28E+03	101%	VU ICP-OES	6/4/10 1:58 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T04-A	1	5.00E-01	U1/2		5.00E-01	4.6E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:00 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T05-A	1	5.00E-01	U1/2		5.00E-01	1.3E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:01 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T06-A	1	2.11E+01			2.11E+01	3.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:03 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T07-A	1	1.25E+03			1.25E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:05 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T08-A	1	1.08E+03			1.08E+03	4.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:06 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T09-A	1	1.59E+03			1.59E+03	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:08 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T01-B	1	7.88E+01			7.88E+01	6.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:19 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T02-B	1	2.31E+00	E		2.31E+00	4.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:21 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T03-B	1	5.00E-01	U1/2		5.00E-01	1.1E+02	1.0E+00	3.2E+00	10	325	3.16E+03	97%	VU ICP-OES	6/4/10 2:23 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T04-B	1	5.00E-01	U1/2		5.00E-01	1.8E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:24 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T05-B	1	1.69E+00	E		1.69E+00	2.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:26 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T06-B	1	1.38E+01			1.38E+01	6.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:28 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T07-B	1	1.29E+03			1.29E+03	7.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:29 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T08-B	1	1.10E+03			1.10E+03	2.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:09 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T09-B	1	1.52E+03			1.52E+03	2.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:33 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T01-C	1	8.67E+01			8.67E+01	2.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:44 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T02-C	1	4.44E+00			4.44E+00	1.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 2:46 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T03-C	1	3.84E+01			3.84E+01	2.3E+00	1.0E+00	3.2E+00	10	325	3.17E+03	97%	VU ICP-OES	6/4/10 2:47 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T04-C	1	5.00E-01	U1/2		5.00E-01	9.0E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:49 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T05-C	1	5.00E-01	U1/2		5.00E-01	2.5E+02	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:51 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T06-C	1	1.95E+01			1.95E+01	3.8E+02	1.0E+00	3.2E+00					VU ICP-OES	6/9/10 2:17 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T07-C	1	1.25E+03			1.25E+03	4.6E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:54 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T08-C	1	1.08E+03			1.08E+03	4.4E-01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:56 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-T09-C	1	1.51E+03			1.51E+03	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:57 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	4.2E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 1:50 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.5E+02	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 1:51 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-B03-A	1	1.09E+01			1.09E+01	6.6E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 1:53 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	9.8E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:15 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-B02-B	1	1.17E+00	E		1.17E+00	5.0E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:16 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-B03-B	1	9.92E+00			9.92E+00	3.7E+00	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:18 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-B01-C	1	2.84E+00	E		2.84E+00	2.8E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:39 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	5.2E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:41 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1313-B03-C	1	8.35E+00			8.35E+00	1.7E+01	1.0E+00	3.2E+00					VU ICP-OES	6/4/10 2:43 PM	EPA Interlab L07 1313-1316 EaFA

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	EaFA-L08-1313-T01-A	1	3.54E+04			3.54E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T02-A	1	2.91E+04			2.91E+04	3.9E-02	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T03-A	1	1.93E+04			1.93E+04	1.2E+00	1.0E+00	3.2E+00	1000	100	2.02E+04	89%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T04-A	1	6.93E+03			6.93E+03	4.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T05-A	1	8.26E+02			8.26E+02	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T06-A	1	1.35E+02			1.35E+02	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T07-A	1	4.39E+02			4.39E+02	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T08-A	1	1.31E+04			1.31E+04	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T09-A	1	8.94E+04			8.94E+04	5.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T01-B	1	3.42E+04			3.42E+04	7.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T02-B	1	2.54E+04			2.54E+04	4.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T03-B	1	1.84E+04			1.84E+04	4.0E+00	1.0E+00	3.2E+00	1000	100	1.93E+04	84%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T04-B	1	7.35E+03			7.35E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T05-B	1	7.20E+02			7.20E+02	1.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T06-B	1	1.24E+02			1.24E+02	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T07-B	1	2.85E+02			2.85E+02	2.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T08-B	1	1.41E+04			1.41E+04	4.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T09-B	1	8.06E+04			8.06E+04	6.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T01-C	1	3.72E+04			3.72E+04	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T02-C	1	2.79E+04			2.79E+04	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T03-C	1	1.91E+04			1.91E+04	2.1E-01	1.0E+00	3.2E+00	1000	100	2.00E+04	98%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T04-C	1	1.86E+03			1.86E+03	1.5E+02	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T05-C	1	7.91E+02			7.91E+02	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T06-C	1	1.42E+02			1.42E+02	5.5E-01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T07-C	1	2.74E+02			2.74E+02	7.6E-01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T08-C	1	1.29E+04			1.29E+04	1.9E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-T09-C	1	5.04E+04			5.04E+04	1.2E+02	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	9.8E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	2.8E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	1.4E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	9.7E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	1.9E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	9.0E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	EaFA-L08-1313-T01-A	1	2.80E+02			2.80E+02	9.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T02-A	1	2.23E+02			2.23E+02	5.9E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T03-A	1	2.62E+02			2.62E+02	3.9E+00	7.5E+00	2.4E+01	10	325	3.50E+03	100%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T04-A	1	2.86E+02			2.86E+02	7.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T05-A	1	2.44E+02			2.44E+02	1.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T06-A	1	2.28E+02			2.28E+02	2.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T07-A	1	1.23E+02			1.23E+02	7.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T08-A	1	4.76E+01			4.76E+01	5.9E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T09-A	1	3.75E+00	U1/2		3.75E+00	8.8E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T01-B	1	2.70E+02			2.70E+02	1.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T02-B	1	1.79E+02			1.79E+02	8.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T03-B	1	2.09E+02			2.09E+02	9.9E+00	7.5E+00	2.4E+01	10	325	3.44E+03	100%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T04-B	1	2.63E+02			2.63E+02	9.4E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T05-B	1	2.42E+02			2.42E+02	2.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T06-B	1	2.13E+02			2.13E+02	8.4E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T07-B	1	1.40E+02			1.40E+02	1.8E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T08-B	1	4.76E+01			4.76E+01	3.6E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T09-B	1	3.75E+00	U1/2		3.75E+00	9.6E+03	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T01-C	1	2.94E+02			2.94E+02	2.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T02-C	1	1.62E+02			1.62E+02	9.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T03-C	1	2.40E+02			2.40E+02	1.3E+01	7.5E+00	2.4E+01	10	325	3.52E+03	101%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T04-C	1	5.47E+01			5.47E+01	1.9E+02	7.5E+00	2.4E+01					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T05-C	1	2.39E+02			2.39E+02	6.3E+00	7.5E+00	2.4E+01					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T06-C	1	2.41E+02			2.41E+02	7.8E+00	7.5E+00	2.4E+01					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T07-C	1	1.63E+02			1.63E+02	8.4E+00	7.5E+00	2.4E+01					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T08-C	1	5.48E+01			5.48E+01	2.3E+01	7.5E+00	2.4E+01					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-T09-C	1	3.75E+00	U1/2		3.75E+00	4.6E+01	7.5E+00	2.4E+01					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-B01-A	1	3.75E+00	U1/2		3.75E+00	1.3E+02	7.5E+00	2.4E+01					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-B02-A	1	3.75E+00	U1/2		3.75E+00	9.5E+01	7.5E+00	2.4E+01					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-B03-A	1	2.12E+01	E		2.12E+01	1.6E+02	7.5E+00	2.4E+01					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-B01-B	1	3.75E+00	U1/2		3.75E+00	8.6E+02	7.5E+00	2.4E+01					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-B02-B	1	3.75E+00	U1/2		3.75E+00	6.4E+02	7.5E+00	2.4E+01					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1313-B03-B	1	3.75E+00	U1/2		3.75E+00	2.3E+02	7.5E+00	2.4E+01					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	EaFA-L08-1313-T01-A	1	1.07E+04			1.07E+04	8.1E-01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T02-A	1	9.53E+02			9.53E+02	1.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T03-A	1	6.44E+02			6.44E+02	1.4E+00	1.1E+01	3.5E+01	10	325	3.90E+03	100%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T04-A	1	9.18E+02			9.18E+02	2.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T05-A	1	3.68E+02			3.68E+02	5.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T06-A	1	1.50E+02			1.50E+02	9.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T07-A	1	1.72E+02			1.72E+02	1.4E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T08-A	1	1.42E+02			1.42E+02	8.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T09-A	1	2.09E+03			2.09E+03	1.1E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T01-B	1	9.89E+03			9.89E+03	9.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T02-B	1	7.61E+02			7.61E+02	4.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T03-B	1	6.41E+02			6.41E+02	6.6E+00	1.1E+01	3.5E+01	10	325	3.82E+03	98%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T04-B	1	9.32E+02			9.32E+02	4.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T05-B	1	3.36E+02			3.36E+02	1.0E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T06-B	1	1.64E+02			1.64E+02	5.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T07-B	1	1.78E+02			1.78E+02	1.7E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T08-B	1	1.58E+02			1.58E+02	6.5E-01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T09-B	1	1.19E+03			1.19E+03	4.2E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T01-C	1	1.01E+04			1.01E+04	6.3E-01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T02-C	1	8.06E+02			8.06E+02	2.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T03-C	1	6.87E+02			6.87E+02	1.9E+00	1.1E+01	3.5E+01	10	325	3.99E+03	102%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T04-C	1	2.26E+02			2.26E+02	1.6E+02	1.1E+01	3.5E+01					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T05-C	1	4.09E+02			4.09E+02	3.9E+00	1.1E+01	3.5E+01					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T06-C	1	1.62E+02			1.62E+02	5.7E+00	1.1E+01	3.5E+01					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T07-C	1	1.97E+02			1.97E+02	1.8E+01	1.1E+01	3.5E+01					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T08-C	1	1.39E+02			1.39E+02	1.1E+01	1.1E+01	3.5E+01					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-T09-C	1	3.68E+02			3.68E+02	1.3E+02	1.1E+01	3.5E+01					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-B01-A	1	5.50E+00	U1/2		5.50E+00	2.4E+02	1.1E+01	3.5E+01					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-B02-A	1	5.50E+00	U1/2		5.50E+00	6.4E+02	1.1E+01	3.5E+01					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-B03-A	1	2.33E+01	E		2.33E+01	7.6E+01	1.1E+01	3.5E+01					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-B01-B	1	5.50E+00	U1/2		5.50E+00	9.3E+01	1.1E+01	3.5E+01					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-B02-B	1	5.50E+00	U1/2		5.50E+00	3.8E+02	1.1E+01	3.5E+01					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1313-B03-B	1	5.50E+00	U1/2		5.50E+00	2.4E+02	1.1E+01	3.5E+01					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	EaFA-L08-1313-T01-A	1	4.61E+03			4.61E+03	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T02-A	1	4.02E+03			4.02E+03	2.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T03-A	1	4.21E+03			4.21E+03	7.4E-01	1.0E+00	3.2E+00	1000	100	5.07E+03	87%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T04-A	1	4.00E+03			4.00E+03	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T05-A	1	4.25E+03			4.25E+03	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T06-A	1	4.22E+03			4.22E+03	3.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T07-A	1	4.07E+03			4.07E+03	1.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T08-A	1	3.70E+03			3.70E+03	1.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T09-A	1	2.73E+03			2.73E+03	4.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T01-B	1	4.50E+03			4.50E+03	8.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T02-B	1	3.77E+03			3.77E+03	4.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T03-B	1	3.97E+03			3.97E+03	8.0E-01	1.0E+00	3.2E+00	1000	100	4.88E+03	91%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T04-B	1	4.06E+03			4.06E+03	8.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T05-B	1	3.92E+03			3.92E+03	7.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T06-B	1	4.39E+03			4.39E+03	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T07-B	1	4.46E+03			4.46E+03	3.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T08-B	1	3.73E+03			3.73E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T09-B	1	2.82E+03			2.82E+03	2.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T01-C	1	4.64E+03			4.64E+03	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T02-C	1	4.03E+03			4.03E+03	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T03-C	1	4.13E+03			4.13E+03	4.4E-01	1.0E+00	3.2E+00	1000	100	4.98E+03	85%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T04-C	1	3.95E+03			3.95E+03	1.4E+02	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T05-C	1	4.24E+03			4.24E+03	9.6E-01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T06-C	1	4.33E+03			4.33E+03	6.0E-01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T07-C	1	4.68E+03			4.68E+03	1.0E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T08-C	1	3.59E+03			3.59E+03	2.1E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-T09-C	1	2.82E+03			2.82E+03	8.3E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-B01-A	1	7.53E+01			7.53E+01	4.4E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-B02-A	1	4.80E+01			4.80E+01	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-B03-A	1	5.84E+01			5.84E+01	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-B01-B	1	3.07E+01			3.07E+01	9.8E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-B02-B	1	1.88E+01			1.88E+01	1.6E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1313-B03-B	1	8.07E+00			8.07E+00	1.8E+02	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	EaFA-L08-1313-T01-A	1	1.72E+03			1.72E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T02-A	1	1.63E+03			1.63E+03	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T03-A	1	9.27E+02			9.27E+02	6.1E-01	1.0E+00	3.2E+00	10	325	3.80E+03	88%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T04-A	1	7.06E+02			7.06E+02	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T05-A	1	3.09E+02			3.09E+02	1.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T06-A	1	2.59E+02			2.59E+02	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T07-A	1	2.53E+02			2.53E+02	1.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T08-A	1	2.82E+02			2.82E+02	1.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T09-A	1	1.02E+03			1.02E+03	1.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T01-B	1	1.49E+03			1.49E+03	8.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T02-B	1	9.85E+02			9.85E+02	3.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T03-B	1	1.29E+03			1.29E+03	5.4E+00	1.0E+00	3.2E+00	10	325	4.11E+03	87%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T04-B	1	6.76E+02			6.76E+02	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T05-B	1	2.80E+02			2.80E+02	9.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T06-B	1	2.61E+02			2.61E+02	7.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T07-B	1	2.72E+02			2.72E+02	3.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T08-B	1	2.61E+02			2.61E+02	7.2E-02	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T09-B	1	8.04E+02			8.04E+02	4.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T01-C	1	1.93E+03			1.93E+03	9.3E-02	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T02-C	1	1.36E+03			1.36E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T03-C	1	1.25E+03			1.25E+03	3.9E-01	1.0E+00	3.2E+00	10	325	4.09E+03	87%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T04-C	1	1.76E+02			1.76E+02	1.5E+02	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T05-C	1	3.37E+02			3.37E+02	1.9E-01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T06-C	1	2.81E+02			2.81E+02	6.4E-02	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T07-C	1	2.91E+02			2.91E+02	5.8E-01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T08-C	1	2.72E+02			2.72E+02	2.6E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-T09-C	1	4.56E+02			4.56E+02	1.3E+02	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	6.2E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.0E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	1.4E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	1.5E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	1.6E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	3.4E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	EaFA-L08-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	1.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	2.9E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	1.0E+03	1.9E+00	6.0E+00	10	325	3.38E+03	104%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	3.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	1.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T07-A	1	5.99E+00	E		5.99E+00	1.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T08-A	1	9.70E+01			9.70E+01	3.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T09-A	1	2.20E+02			2.20E+02	2.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	7.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	1.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	2.7E+02	1.9E+00	6.0E+00	10	325	3.32E+03	102%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	9.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T07-B	1	4.32E+00	E		4.32E+00	7.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T08-B	1	1.01E+02			1.01E+02	3.0E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T09-B	1	1.80E+02			1.80E+02	6.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	3.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	1.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00	10	325	3.38E+03	104%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	6.8E+01	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	7.8E+01	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	2.6E+02	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T07-C	1	4.54E+00	E		4.54E+00	8.0E+00	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T08-C	1	9.89E+01			9.89E+01	2.8E+00	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-T09-C	1	1.15E+02			1.15E+02	1.1E+02	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	9.8E+01	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	1.7E+02	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	5.0E+02	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-B01-B	1	9.50E-01	U1/2		9.50E-01	3.3E+01	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-B02-B	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1313-B03-B	1	9.50E-01	U1/2		9.50E-01	7.6E+01	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	EaFA-L08-1313-T01-A	1	1.10E+00	U1/2		1.10E+00	6.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T02-A	1	1.10E+00	U1/2		1.10E+00	2.3E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	5.0E+01	2.2E+00	7.0E+00	10	325	3.35E+03	103%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T04-A	1	1.10E+00	U1/2		1.10E+00	7.6E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T05-A	1	1.10E+00	U1/2		1.10E+00	8.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T06-A	1	1.10E+00	U1/2		1.10E+00	1.9E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T07-A	1	3.03E+01			3.03E+01	1.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T08-A	1	3.13E+01			3.13E+01	2.8E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T09-A	1	3.03E+01			3.03E+01	1.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T01-B	1	1.10E+00	U1/2		1.10E+00	9.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T02-B	1	1.10E+00	U1/2		1.10E+00	6.9E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	3.3E+01	2.2E+00	7.0E+00	10	325	3.29E+03	101%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T04-B	1	1.10E+00	U1/2		1.10E+00	1.2E+02	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T05-B	1	1.10E+00	U1/2		1.10E+00	5.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T06-B	1	1.10E+00	U1/2		1.10E+00	7.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T07-B	1	3.13E+01			3.13E+01	8.2E-01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T08-B	1	3.18E+01			3.18E+01	1.8E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T09-B	1	2.59E+01			2.59E+01	4.0E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T01-C	1	1.10E+00	U1/2		1.10E+00	9.9E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T02-C	1	1.10E+00	U1/2		1.10E+00	5.7E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	6.6E+00	2.2E+00	7.0E+00	10	325	3.35E+03	103%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T04-C	1	1.10E+00	U1/2		1.10E+00	1.2E+01	2.2E+00	7.0E+00					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T05-C	1	1.10E+00	U1/2		1.10E+00	3.8E+01	2.2E+00	7.0E+00					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T06-C	1	1.10E+00	U1/2		1.10E+00	4.4E+01	2.2E+00	7.0E+00					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T07-C	1	3.16E+01			3.16E+01	2.7E+00	2.2E+00	7.0E+00					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T08-C	1	3.16E+01			3.16E+01	4.6E+00	2.2E+00	7.0E+00					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-T09-C	1	1.18E+01			1.18E+01	1.4E+02	2.2E+00	7.0E+00					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	3.5E+01	2.2E+00	7.0E+00					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	6.4E+01	2.2E+00	7.0E+00					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-B03-A	1	1.10E+00	U1/2		1.10E+00	8.2E+01	2.2E+00	7.0E+00					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-B01-B	1	1.10E+00	U1/2		1.10E+00	9.3E+01	2.2E+00	7.0E+00					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-B02-B	1	1.10E+00	U1/2		1.10E+00	4.1E+01	2.2E+00	7.0E+00					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1313-B03-B	1	1.10E+00	U1/2		1.10E+00	1.5E+01	2.2E+00	7.0E+00					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	EaFA-L08-1313-T01-A	1	1.35E+04			1.35E+04	7.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T02-A	1	4.07E+04			4.07E+04	3.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T03-A	1	8.27E+04			8.27E+04	1.4E+00	2.6E+00	8.3E+00	1000	100	8.36E+04	86%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T04-A	1	1.26E+05			1.26E+05	1.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T05-A	1	1.44E+05			1.44E+05	5.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T06-A	1	1.56E+05			1.56E+05	7.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T07-A	1	1.47E+05			1.47E+05	1.3E+01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T08-A	1	1.41E+05			1.41E+05	6.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T09-A	1	1.15E+05			1.15E+05	8.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T01-B	1	1.27E+04			1.27E+04	8.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T02-B	1	4.08E+04			4.08E+04	3.7E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T03-B	1	8.35E+04			8.35E+04	4.5E+00	2.6E+00	8.3E+00	1000	100	8.44E+04	85%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T04-B	1	1.23E+05			1.23E+05	3.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T05-B	1	1.32E+05			1.32E+05	9.9E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T06-B	1	1.54E+05			1.54E+05	7.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T07-B	1	1.63E+05			1.63E+05	2.7E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T08-B	1	1.41E+05			1.41E+05	3.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T09-B	1	9.86E+04			9.86E+04	3.9E+01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T01-C	1	1.45E+04			1.45E+04	2.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T02-C	1	4.20E+04			4.20E+04	1.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T03-C	1	8.65E+04			8.65E+04	7.2E-01	2.6E+00	8.3E+00	1000	100	8.74E+04	89%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T04-C	1	3.07E+04			3.07E+04	1.5E+02	2.6E+00	8.3E+00					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T05-C	1	1.43E+05			1.43E+05	3.6E-01	2.6E+00	8.3E+00					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T06-C	1	1.52E+05			1.52E+05	4.2E-01	2.6E+00	8.3E+00					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T07-C	1	1.66E+05			1.66E+05	7.3E-01	2.6E+00	8.3E+00					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T08-C	1	1.40E+05			1.40E+05	2.3E+00	2.6E+00	8.3E+00					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-T09-C	1	4.81E+04			4.81E+04	1.3E+02	2.6E+00	8.3E+00					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-B01-A	1	1.30E+00	U1/2		1.30E+00	4.0E+02	2.6E+00	8.3E+00					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-B02-A	1	4.03E+00	E		4.03E+00	6.5E+01	2.6E+00	8.3E+00					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-B03-A	1	5.96E+01			5.96E+01	3.4E+01	2.6E+00	8.3E+00					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-B01-B	1	7.31E+00	E		7.31E+00	4.5E+01	2.6E+00	8.3E+00					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-B02-B	1	5.03E+00	E		5.03E+00	2.1E+01	2.6E+00	8.3E+00					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1313-B03-B	1	1.84E+01			1.84E+01	1.4E+02	2.6E+00	8.3E+00					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	EaFA-L08-1313-T01-A	1	4.58E+02			4.58E+02	9.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T02-A	1	4.31E+02			4.31E+02	6.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T03-A	1	3.31E+02			3.31E+02	1.7E+00	1.2E+00	3.8E+00	10	325	3.45E+03	96%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T04-A	1	1.82E+02			1.82E+02	2.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T05-A	1	7.55E+01			7.55E+01	2.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T06-A	1	1.13E+01			1.13E+01	9.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T07-A	1	1.81E+00	E		1.81E+00	8.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T08-A	1	5.17E+01			5.17E+01	1.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T09-A	1	1.63E+03			1.63E+03	4.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T01-B	1	4.54E+02			4.54E+02	8.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T02-B	1	3.60E+02			3.60E+02	4.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T03-B	1	2.67E+02			2.67E+02	5.6E+00	1.2E+00	3.8E+00	10	325	3.34E+03	95%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T04-B	1	1.74E+02			1.74E+02	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T05-B	1	7.21E+01			7.21E+01	9.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T06-B	1	1.15E+01			1.15E+01	8.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T07-B	1	6.00E-01	U1/2		6.00E-01	6.4E+02	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T08-B	1	5.56E+01			5.56E+01	2.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T09-B	1	1.48E+03			1.48E+03	1.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T01-C	1	5.68E+02			5.68E+02	5.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T02-C	1	3.98E+02			3.98E+02	1.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T03-C	1	3.19E+02			3.19E+02	8.3E-01	1.2E+00	3.8E+00	10	325	3.46E+03	97%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T04-C	1	1.91E+02			1.91E+02	1.6E+02	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T05-C	1	8.19E+01			8.19E+01	9.1E-01	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T06-C	1	1.45E+01			1.45E+01	6.7E+00	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T07-C	1	1.34E+00	E		1.34E+00	8.4E+01	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T08-C	1	5.15E+01			5.15E+01	2.2E+00	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-T09-C	1	1.64E+03			1.64E+03	8.8E+01	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	6.7E+01	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	2.3E+02	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-B03-A	1	2.19E+00	E		2.19E+00	2.9E+01	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-B01-B	1	6.00E-01	U1/2		6.00E-01	2.4E+02	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-B02-B	1	6.00E-01	U1/2		6.00E-01	1.8E+02	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1313-B03-B	1	6.00E-01	U1/2		6.00E-01	2.5E+01	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	EaFA-L08-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	8.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	9.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	8.0E+01	1.8E+00	5.7E+00	10	325	3.16E+03	97%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	3.0E+03	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T05-A	1	5.17E+00	E		5.17E+00	3.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T06-A	1	5.91E+01			5.91E+01	6.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T07-A	1	2.03E+02			2.03E+02	1.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T08-A	1	1.94E+02			1.94E+02	8.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T09-A	1	4.19E+02			4.19E+02	1.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	1.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	1.2E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	2.1E+02	1.8E+00	5.7E+00	10	325	3.14E+03	97%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	4.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T05-B	1	4.06E+00	E		4.06E+00	5.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T06-B	1	6.65E+01			6.65E+01	2.9E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T07-B	1	2.17E+02			2.17E+02	3.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T08-B	1	1.97E+02			1.97E+02	4.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T09-B	1	3.60E+02			3.60E+02	4.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	3.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	6.0E+01	1.8E+00	5.7E+00	10	325	3.17E+03	98%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	2.9E+01	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T05-C	1	5.07E+00	E		5.07E+00	2.6E+01	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T06-C	1	5.49E+01			5.49E+01	5.6E+00	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T07-C	1	2.21E+02			2.21E+02	1.3E+00	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T08-C	1	1.92E+02			1.92E+02	2.4E+00	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-T09-C	1	1.75E+02			1.75E+02	1.3E+02	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	3.7E+01	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	1.6E+02	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	2.7E+01	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-B01-B	1	9.00E-01	U1/2		9.00E-01	2.9E+02	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-B02-B	1	9.00E-01	U1/2		9.00E-01	8.8E+01	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1313-B03-B	1	9.00E-01	U1/2		9.00E-01	8.9E+01	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	EaFA-L08-1313-T01-A	1	1.72E+01			1.72E+01	1.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T02-A	1	6.05E+00	E		6.05E+00	6.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T03-A	1	5.29E+00	E		5.29E+00	2.0E+01	3.7E+00	1.2E+01	10	325	3.12E+03	96%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T04-A	1	9.27E+00	E		9.27E+00	4.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T05-A	1	1.23E+01			1.23E+01	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T06-A	1	1.22E+01			1.22E+01	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T07-A	1	1.16E+02			1.16E+02	6.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T08-A	1	1.80E+03			1.80E+03	1.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T09-A	1	2.58E+03			2.58E+03	1.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T01-B	1	1.41E+01			1.41E+01	1.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T02-B	1	7.12E+00	E		7.12E+00	1.1E+02	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T03-B	1	1.85E+00	U1/2		1.85E+00	1.3E+02	3.7E+00	1.2E+01	10	325	3.06E+03	94%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T04-B	1	7.51E+00	E		7.51E+00	5.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T05-B	1	5.46E+00	E		5.46E+00	6.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T06-B	1	8.91E+00	E		8.91E+00	6.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T07-B	1	8.15E+01			8.15E+01	4.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T08-B	1	1.81E+03			1.81E+03	5.3E-01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T09-B	1	2.09E+03			2.09E+03	4.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T01-C	1	4.20E+01			4.20E+01	2.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T02-C	1	1.85E+00	U1/2		1.85E+00	5.2E+02	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T03-C	1	1.85E+00	U1/2		1.85E+00	1.4E+02	3.7E+00	1.2E+01	10	325	3.11E+03	96%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T04-C	1	1.85E+00	U1/2		1.85E+00	3.6E+02	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T05-C	1	1.85E+00	U1/2		1.85E+00	4.3E+02	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T06-C	1	6.26E+00	E		6.26E+00	5.8E+01	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T07-C	1	7.72E+01			7.72E+01	9.3E+00	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T08-C	1	1.82E+03			1.82E+03	6.8E-01	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-T09-C	1	1.49E+03			1.49E+03	8.1E+01	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	2.4E+02	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	4.0E+02	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-B03-A	1	1.85E+00	U1/2		1.85E+00	2.7E+03	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-B01-B	1	1.85E+00	U1/2		1.85E+00	4.6E+02	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-B02-B	1	1.85E+00	U1/2		1.85E+00	4.5E+01	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1313-B03-B	1	1.85E+00	U1/2		1.85E+00	1.3E+01	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	EaFA-L08-1313-T01-A	1	2.30E+01			2.30E+01	2.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T02-A	1	2.81E+01			2.81E+01	9.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T03-A	1	7.52E+00			7.52E+00	2.3E+00	2.0E+00	6.4E+00	1000	100	1.05E+03	105%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	1.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T08-A	1	2.83E+02			2.83E+02	4.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T09-A	1	4.09E+04			4.09E+04	2.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T01-B	1	1.42E+01			1.42E+01	1.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T02-B	1	2.79E+01			2.79E+01	4.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T03-B	1	4.98E+00	E		4.98E+00	1.0E+01	2.0E+00	6.4E+00	1000	100	1.03E+03	103%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	5.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	6.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T08-B	1	2.91E+02			2.91E+02	8.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T09-B	1	3.27E+04			3.27E+04	2.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T01-C	1	4.00E+01			4.00E+01	7.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T02-C	1	2.32E+01			2.32E+01	4.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T03-C	1	4.20E+00	E		4.20E+00	6.9E+00	2.0E+00	6.4E+00	1000	100	1.05E+03	104%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	5.6E+00	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	4.6E+00	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	3.8E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T08-C	1	3.18E+02			3.18E+02	2.3E+00	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-T09-C	1	1.62E+04			1.62E+04	1.0E+02	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	6.7E+00	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	2.9E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-B03-A	1	1.55E+01			1.55E+01	2.2E+00	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	6.1E+00	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	4.9E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1313-B03-B	1	2.13E+00	E		2.13E+00	2.4E+02	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	EaFA-L08-1313-T01-A	1	1.33E+01	E		1.33E+01	6.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T02-A	1	3.40E+00	U1/2		3.40E+00	2.0E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T03-A	1	3.40E+00	U1/2		3.40E+00	7.6E+01	6.8E+00	2.2E+01	10	325	3.19E+03	98%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T04-A	1	3.40E+00	U1/2		3.40E+00	5.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T05-A	1	3.40E+00	U1/2		3.40E+00	2.5E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T06-A	1	3.40E+00	U1/2		3.40E+00	2.0E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T07-A	1	3.40E+00	U1/2		3.40E+00	1.4E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T08-A	1	3.40E+00	U1/2		3.40E+00	2.3E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T09-A	1	1.50E+02			1.50E+02	1.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T01-B	1	3.40E+00	U1/2		3.40E+00	3.4E+03	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T02-B	1	3.40E+00	U1/2		3.40E+00	4.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T03-B	1	3.40E+00	U1/2		3.40E+00	1.5E+02	6.8E+00	2.2E+01	10	325	3.11E+03	96%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T04-B	1	3.40E+00	U1/2		3.40E+00	5.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T05-B	1	3.40E+00	U1/2		3.40E+00	4.1E+03	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T06-B	1	3.40E+00	U1/2		3.40E+00	5.2E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T07-B	1	3.40E+00	U1/2		3.40E+00	4.7E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T08-B	1	3.40E+00	U1/2		3.40E+00	8.1E+03	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T09-B	1	9.98E+01			9.98E+01	5.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T01-C	1	1.58E+01	E		1.58E+01	8.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T02-C	1	3.40E+00	U1/2		3.40E+00	8.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T03-C	1	3.40E+00	U1/2		3.40E+00	6.9E+01	6.8E+00	2.2E+01	10	325	3.18E+03	98%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T04-C	1	3.40E+00	U1/2		3.40E+00	9.7E+01	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T05-C	1	3.40E+00	U1/2		3.40E+00	7.9E+02	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T06-C	1	3.40E+00	U1/2		3.40E+00	1.8E+02	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T07-C	1	3.40E+00	U1/2		3.40E+00	1.6E+02	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T08-C	1	3.40E+00	U1/2		3.40E+00	2.7E+02	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-T09-C	1	5.50E+01			5.50E+01	1.5E+02	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	6.9E+01	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	2.0E+02	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	1.3E+02	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-B01-B	1	3.40E+00	U1/2		3.40E+00	5.3E+00	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-B02-B	1	3.40E+00	U1/2		3.40E+00	6.2E+02	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1313-B03-B	1	3.40E+00	U1/2		3.40E+00	1.1E+02	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	EaFA-L08-1313-T01-A	1	2.10E+03			2.10E+03	6.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T02-A	1	2.79E+03			2.79E+03	2.2E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T03-A	1	3.05E+03			3.05E+03	1.2E+00	1.9E+00	6.0E+00	10	325	5.74E+03	83%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T04-A	1	3.31E+03			3.31E+03	4.0E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T05-A	1	3.44E+03			3.44E+03	5.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T06-A	1	3.46E+03			3.46E+03	1.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T07-A	1	3.15E+03			3.15E+03	1.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T08-A	1	2.49E+03			2.49E+03	1.0E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T09-A	1	1.12E+03			1.12E+03	3.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T01-B	1	1.96E+03			1.96E+03	8.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T02-B	1	2.66E+03			2.66E+03	3.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T03-B	1	2.90E+03			2.90E+03	5.3E+00	1.9E+00	6.0E+00	10	325	5.73E+03	87%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T04-B	1	3.20E+03			3.20E+03	2.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T05-B	1	3.12E+03			3.12E+03	9.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T06-B	1	3.46E+03			3.46E+03	5.8E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T07-B	1	3.47E+03			3.47E+03	2.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T08-B	1	2.49E+03			2.49E+03	5.8E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T09-B	1	9.66E+02			9.66E+02	5.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T01-C	1	2.06E+03			2.06E+03	5.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T02-C	1	2.68E+03			2.68E+03	9.9E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T03-C	1	2.99E+03			2.99E+03	2.7E-01	1.9E+00	6.0E+00	10	325	5.77E+03	85%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T04-C	1	8.23E+02			8.23E+02	1.5E+02	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T05-C	1	3.40E+03			3.40E+03	1.3E-01	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T06-C	1	3.41E+03			3.41E+03	2.9E-01	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T07-C	1	3.50E+03			3.50E+03	6.8E-01	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T08-C	1	2.43E+03			2.43E+03	3.6E+00	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-T09-C	1	5.75E+02			5.75E+02	1.2E+02	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-B01-A	1	5.07E+01			5.07E+01	2.2E+00	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-B02-A	1	4.97E+01			4.97E+01	2.1E+00	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-B03-A	1	5.00E+01			5.00E+01	1.9E+00	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-B01-B	1	5.14E+01			5.14E+01	2.4E+00	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-B02-B	1	5.10E+01			5.10E+01	6.2E-01	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1313-B03-B	1	5.17E+01			5.17E+01	1.0E+00	1.9E+00	6.0E+00					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	EaFA-L08-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	8.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	6.0E+01	2.0E+00	6.4E+00	10	325	3.32E+03	102%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	8.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T05-A	1	6.99E+01			6.99E+01	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T06-A	1	4.47E+02			4.47E+02	7.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T07-A	1	8.54E+02			8.54E+02	1.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T08-A	1	1.02E+03			1.02E+03	3.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T09-A	1	1.40E+03			1.40E+03	3.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	7.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	7.0E+01	2.0E+00	6.4E+00	10	325	3.23E+03	99%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	8.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T05-B	1	6.94E+01			6.94E+01	9.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T06-B	1	4.65E+02			4.65E+02	3.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T07-B	1	9.21E+02			9.21E+02	3.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T08-B	1	1.07E+03			1.07E+03	8.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T09-B	1	1.18E+03			1.18E+03	6.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	3.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	2.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00	10	325	3.30E+03	102%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	3.1E+03	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T05-C	1	7.45E+01			7.45E+01	8.3E-01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T06-C	1	4.12E+02			4.12E+02	6.3E-01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T07-C	1	9.48E+02			9.48E+02	5.5E-01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T08-C	1	1.04E+03			1.04E+03	2.5E+00	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-T09-C	1	7.13E+02			7.13E+02	1.2E+02	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	5.0E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	4.3E+00	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	7.2E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	1.7E+02	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	EaFA-L08-1313-T01-A	1	1.52E+00	E		1.52E+00	3.1E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T02-A	1	2.89E+00	E		2.89E+00	2.1E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T03-A	1	6.30E+01			6.30E+01	5.6E+00	1.0E+00	3.2E+00	1000	100	1.02E+03	95%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T04-A	1	2.76E+03			2.76E+03	9.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T05-A	1	5.57E+03			5.57E+03	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T06-A	1	7.11E+03			7.11E+03	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T07-A	1	7.02E+03			7.02E+03	1.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T08-A	1	7.00E+03			7.00E+03	3.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T09-A	1	1.07E+04			1.07E+04	4.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T01-B	1	1.62E+00	E		1.62E+00	3.6E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T02-B	1	1.20E+00	E		1.20E+00	5.0E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T03-B	1	1.06E+02			1.06E+02	1.1E+01	1.0E+00	3.2E+00	1000	100	1.05E+03	94%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T04-B	1	2.86E+03			2.86E+03	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T05-B	1	5.27E+03			5.27E+03	1.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T06-B	1	7.22E+03			7.22E+03	3.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T07-B	1	7.90E+03			7.90E+03	2.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T08-B	1	7.10E+03			7.10E+03	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T09-B	1	1.12E+04			1.12E+04	2.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T01-C	1	4.25E+00			4.25E+00	2.2E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T02-C	1	5.00E-01	U1/2		5.00E-01	1.1E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T03-C	1	1.19E+02			1.19E+02	8.4E+00	1.0E+00	3.2E+00	1000	100	1.05E+03	93%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T04-C	1	7.57E+02			7.57E+02	1.6E+02	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T05-C	1	5.88E+03			5.88E+03	7.9E-01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T06-C	1	7.15E+03			7.15E+03	4.3E-01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T07-C	1	8.05E+03			8.05E+03	3.7E-01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T08-C	1	6.92E+03			6.92E+03	2.4E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-T09-C	1	5.77E+03			5.77E+03	1.2E+02	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	6.5E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	9.7E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	3.9E+03	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	1.9E+02	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	7.9E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	2.5E+02	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	EaFA-L08-1313-T01-A	1	4.19E+03			4.19E+03	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T02-A	1	4.12E+03			4.12E+03	5.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T03-A	1	4.05E+03			4.05E+03	3.9E-01	1.2E+00	3.8E+00	10	325	6.87E+03	87%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T04-A	1	3.95E+03			3.95E+03	2.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T05-A	1	3.76E+03			3.76E+03	4.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T06-A	1	3.30E+03			3.30E+03	8.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T07-A	1	6.66E+02			6.66E+02	1.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T08-A	1	1.35E+02			1.35E+02	2.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T09-A	1	3.78E+02			3.78E+02	1.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T01-B	1	3.99E+03			3.99E+03	7.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T02-B	1	3.89E+03			3.89E+03	4.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T03-B	1	3.81E+03			3.81E+03	3.1E+00	1.2E+00	3.8E+00	10	325	6.74E+03	90%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T04-B	1	3.96E+03			3.96E+03	3.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T05-B	1	3.49E+03			3.49E+03	9.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T06-B	1	3.27E+03			3.27E+03	4.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T07-B	1	9.70E+02			9.70E+02	3.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T08-B	1	1.34E+02			1.34E+02	9.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T09-B	1	2.52E+02			2.52E+02	4.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T01-C	1	4.19E+03			4.19E+03	5.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T02-C	1	3.92E+03			3.92E+03	1.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T03-C	1	3.97E+03			3.97E+03	4.7E-01	1.2E+00	3.8E+00	10	325	6.86E+03	89%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T04-C	1	1.04E+03			1.04E+03	1.5E+02	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T05-C	1	3.83E+03			3.83E+03	7.9E-01	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T06-C	1	3.34E+03			3.34E+03	6.3E-01	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T07-C	1	1.02E+03			1.02E+03	6.6E-01	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T08-C	1	1.32E+02			1.32E+02	2.6E+00	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-T09-C	1	1.11E+02			1.11E+02	1.2E+02	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-B01-A	1	9.91E+00			9.91E+00	4.9E+00	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-B02-A	1	8.75E+00			8.75E+00	2.7E+01	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-B03-A	1	3.98E+01			3.98E+01	9.5E+00	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-B01-B	1	9.23E+00			9.23E+00	7.1E+00	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-B02-B	1	7.33E+00			7.33E+00	2.7E+01	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1313-B03-B	1	1.36E+01			1.36E+01	6.2E+01	1.2E+00	3.8E+00					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	EaFA-L08-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	1.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	5.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00	10	325	3.23E+03	99%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	8.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T05-A	1	1.83E+01			1.83E+01	1.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T06-A	1	1.47E+02			1.47E+02	2.9E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T07-A	1	5.20E+02			5.20E+02	1.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T08-A	1	4.99E+02			4.99E+02	4.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T09-A	1	7.07E+02			7.07E+02	1.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	3.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	6.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	8.1E+01	1.8E+00	5.7E+00	10	325	3.16E+03	97%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	9.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T05-B	1	1.80E+01			1.80E+01	5.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T06-B	1	1.50E+02			1.50E+02	3.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T07-B	1	5.50E+02			5.50E+02	2.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T08-B	1	5.09E+02			5.09E+02	7.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T09-B	1	5.96E+02			5.96E+02	3.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	6.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	3.5E+01	1.8E+00	5.7E+00	10	325	3.22E+03	99%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	6.5E+00	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T05-C	1	1.44E+01			1.44E+01	9.7E+00	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T06-C	1	1.20E+02			1.20E+02	5.2E+00	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T07-C	1	5.50E+02			5.50E+02	1.9E+00	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T08-C	1	4.98E+02			4.98E+02	3.3E+00	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-T09-C	1	3.08E+02			3.08E+02	1.3E+02	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	2.5E+01	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	2.2E+02	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-B01-B	1	9.00E-01	U1/2		9.00E-01	3.0E+01	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-B02-B	1	9.00E-01	U1/2		9.00E-01	2.0E+01	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1313-B03-B	1	9.00E-01	U1/2		9.00E-01	6.4E+01	1.8E+00	5.7E+00					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	EaFA-L08-1313-T01-A	1	1.16E+02			1.16E+02	1.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T02-A	1	1.88E+01			1.88E+01	1.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T03-A	1	1.23E+01			1.23E+01	7.7E+01	3.7E+00	1.2E+01	1000	100	1.11E+03	110%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T04-A	1	1.29E+02			1.29E+02	2.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T05-A	1	6.10E+01			6.10E+01	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T06-A	1	1.36E+01			1.36E+01	5.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T07-A	1	1.38E+01			1.38E+01	7.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T08-A	1	1.40E+01			1.40E+01	2.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T09-A	1	3.02E+03			3.02E+03	1.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T01-B	1	8.07E+01			8.07E+01	2.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T02-B	1	2.80E+01			2.80E+01	1.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T03-B	1	1.67E+01			1.67E+01	3.1E+01	3.7E+00	1.2E+01	1000	100	1.09E+03	108%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T04-B	1	1.05E+02			1.05E+02	4.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T05-B	1	5.17E+01			5.17E+01	1.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T06-B	1	2.73E+01			2.73E+01	2.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T07-B	1	1.64E+01			1.64E+01	3.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T08-B	1	1.61E+01			1.61E+01	7.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T09-B	1	1.92E+03			1.92E+03	3.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T01-C	1	7.71E+01			7.71E+01	1.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T02-C	1	1.38E+01			1.38E+01	4.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T03-C	1	2.82E+01			2.82E+01	2.4E+01	3.7E+00	1.2E+01	1000	100	1.14E+03	112%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T04-C	1	2.60E+01			2.60E+01	2.2E+02	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T05-C	1	6.06E+01			6.06E+01	2.0E+01	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T06-C	1	3.27E+01			3.27E+01	3.1E+01	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T07-C	1	1.50E+01			1.50E+01	4.5E+01	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T08-C	1	1.96E+01			1.96E+01	2.7E+01	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-T09-C	1	6.63E+02			6.63E+02	1.3E+02	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	1.2E+02	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	4.7E+02	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-B03-A	1	1.97E+01			1.97E+01	1.6E+00	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-B01-B	1	1.85E+00	U1/2		1.85E+00	1.8E+03	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-B02-B	1	1.85E+00	U1/2		1.85E+00	1.6E+02	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1313-B03-B	1	1.85E+00	U1/2		1.85E+00	5.0E+02	3.7E+00	1.2E+01					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	EaFA-L08-1313-T01-A	1	5.16E+04			5.16E+04	9.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T02-A	1	3.37E+04			3.37E+04	2.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T03-A	1	2.68E+04			2.68E+04	1.2E+00	1.6E+00	5.1E+00	1000	100	2.76E+04	85%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T04-A	1	2.54E+04			2.54E+04	1.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T05-A	1	2.47E+04			2.47E+04	6.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T06-A	1	2.42E+04			2.42E+04	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T07-A	1	2.24E+04			2.24E+04	1.4E+01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T08-A	1	1.94E+04			1.94E+04	2.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T09-A	1	1.99E+04			1.99E+04	1.8E+01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T01-B	1	4.89E+04			4.89E+04	9.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T02-B	1	3.05E+04			3.05E+04	3.9E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T03-B	1	2.47E+04			2.47E+04	5.5E+00	1.6E+00	5.1E+00	1000	100	2.55E+04	82%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T04-B	1	2.48E+04			2.48E+04	1.4E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T05-B	1	2.26E+04			2.26E+04	9.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T06-B	1	2.41E+04			2.41E+04	9.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T07-B	1	2.50E+04			2.50E+04	2.7E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T08-B	1	1.94E+04			1.94E+04	6.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T09-B	1	1.66E+04			1.66E+04	4.5E+01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T01-C	1	5.15E+04			5.15E+04	3.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T02-C	1	3.16E+04			3.16E+04	1.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T03-C	1	2.59E+04			2.59E+04	3.5E-01	1.6E+00	5.1E+00	1000	100	2.67E+04	82%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T04-C	1	6.02E+03			6.02E+03	1.6E+02	1.6E+00	5.1E+00					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T05-C	1	2.48E+04			2.48E+04	5.9E-01	1.6E+00	5.1E+00					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T06-C	1	2.38E+04			2.38E+04	3.7E-01	1.6E+00	5.1E+00					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T07-C	1	2.52E+04			2.52E+04	6.0E-01	1.6E+00	5.1E+00					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T08-C	1	1.88E+04			1.88E+04	3.3E+00	1.6E+00	5.1E+00					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-T09-C	1	8.45E+03			8.45E+03	1.3E+02	1.6E+00	5.1E+00					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-B01-A	1	3.98E+01			3.98E+01	4.4E+00	1.6E+00	5.1E+00					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-B02-A	1	3.81E+01			3.81E+01	8.1E+00	1.6E+00	5.1E+00					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-B03-A	1	1.83E+02			1.83E+02	1.2E+01	1.6E+00	5.1E+00					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-B01-B	1	3.86E+01			3.86E+01	1.0E+01	1.6E+00	5.1E+00					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-B02-B	1	3.89E+01			3.89E+01	8.1E+00	1.6E+00	5.1E+00					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1313-B03-B	1	5.91E+01			5.91E+01	7.8E+01	1.6E+00	5.1E+00					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	EaFA-L08-1313-T01-A	1	7.52E+03			7.52E+03	1.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T02-A	1	6.06E+03			6.06E+03	6.1E-01	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T03-A	1	5.48E+03			5.48E+03	1.2E+00	1.5E+01	4.8E+01	10	325	8.28E+03	86%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T04-A	1	4.05E+03			4.05E+03	1.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T05-A	1	2.39E+03			2.39E+03	2.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T06-A	1	1.49E+03			1.49E+03	2.6E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T07-A	1	4.28E+02			4.28E+02	1.4E+01	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T08-A	1	2.21E+02			2.21E+02	8.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T09-A	1	7.61E+02			7.61E+02	1.1E+01	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T01-B	1	7.21E+03			7.21E+03	8.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T02-B	1	5.69E+03			5.69E+03	4.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T03-B	1	5.06E+03			5.06E+03	3.7E+00	1.5E+01	4.8E+01	10	325	7.97E+03	90%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T04-B	1	3.94E+03			3.94E+03	1.2E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T05-B	1	2.22E+03			2.22E+03	8.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T06-B	1	1.42E+03			1.42E+03	1.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T07-B	1	5.20E+02			5.20E+02	1.6E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T08-B	1	1.94E+02			1.94E+02	1.1E+01	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T09-B	1	4.88E+02			4.88E+02	4.0E+01	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T01-C	1	7.59E+03			7.59E+03	5.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T02-C	1	5.88E+03			5.88E+03	2.0E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T03-C	1	5.33E+03			5.33E+03	4.0E-01	1.5E+01	4.8E+01	10	325	8.26E+03	90%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T04-C	1	3.83E+03			3.83E+03	1.5E+02	1.5E+01	4.8E+01					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T05-C	1	2.47E+03			2.47E+03	5.7E-01	1.5E+01	4.8E+01					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T06-C	1	1.61E+03			1.61E+03	1.5E+00	1.5E+01	4.8E+01					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T07-C	1	5.34E+02			5.34E+02	1.9E+00	1.5E+01	4.8E+01					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T08-C	1	1.99E+02			1.99E+02	7.3E+00	1.5E+01	4.8E+01					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-T09-C	1	4.02E+02			4.02E+02	1.0E+02	1.5E+01	4.8E+01					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-B01-A	1	6.34E+01			6.34E+01	5.1E+01	1.5E+01	4.8E+01					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-B02-A	1	4.31E+01	E		4.31E+01	2.7E+01	1.5E+01	4.8E+01					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-B03-A	1	1.13E+02			1.13E+02	2.7E+01	1.5E+01	4.8E+01					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-B01-B	1	7.95E+01			7.95E+01	4.7E+01	1.5E+01	4.8E+01					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-B02-B	1	5.51E+01			5.51E+01	6.0E+01	1.5E+01	4.8E+01					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1313-B03-B	1	7.05E+01			7.05E+01	6.0E+01	1.5E+01	4.8E+01					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	EaFA-L08-1313-T01-A	1	1.79E+04			1.79E+04	8.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T02-A	1	6.02E+03			6.02E+03	1.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T03-A	1	2.05E+03			2.05E+03	1.3E+00	1.1E+00	3.5E+00	1000	100	2.89E+03	84%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T04-A	1	5.18E+02			5.18E+02	2.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T05-A	1	1.20E+03			1.20E+03	7.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T06-A	1	3.29E+03			3.29E+03	5.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T07-A	1	7.28E+03			7.28E+03	1.3E+01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T08-A	1	1.52E+04			1.52E+04	2.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T09-A	1	6.95E+04			6.95E+04	4.7E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T01-B	1	1.74E+04			1.74E+04	8.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T02-B	1	4.71E+03			4.71E+03	3.7E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T03-B	1	1.30E+03			1.30E+03	5.0E+00	1.1E+00	3.5E+00	1000	100	2.25E+03	95%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T04-B	1	5.25E+02			5.25E+02	1.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T05-B	1	1.19E+03			1.19E+03	9.8E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T06-B	1	3.52E+03			3.52E+03	7.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T07-B	1	7.90E+03			7.90E+03	2.9E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T08-B	1	1.56E+04			1.56E+04	1.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T09-B	1	6.27E+04			6.27E+04	1.8E+01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T01-C	1	1.76E+04			1.76E+04	2.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T02-C	1	5.27E+03			5.27E+03	1.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T03-C	1	1.38E+03			1.38E+03	4.5E-01	1.1E+00	3.5E+00	1000	100	2.29E+03	91%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T04-C	1	1.27E+02			1.27E+02	1.7E+02	1.1E+00	3.5E+00					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T05-C	1	1.41E+03			1.41E+03	6.8E-01	1.1E+00	3.5E+00					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T06-C	1	3.41E+03			3.41E+03	7.6E-01	1.1E+00	3.5E+00					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T07-C	1	8.07E+03			8.07E+03	7.9E-01	1.1E+00	3.5E+00					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T08-C	1	1.53E+04			1.53E+04	2.9E+00	1.1E+00	3.5E+00					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-T09-C	1	2.99E+04			2.99E+04	1.1E+02	1.1E+00	3.5E+00					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-B01-A	1	5.50E-01	U1/2		5.50E-01	1.7E+01	1.1E+00	3.5E+00					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-B02-A	1	3.20E+01			3.20E+01	1.3E+01	1.1E+00	3.5E+00					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-B03-A	1	1.57E+02			1.57E+02	1.6E+01	1.1E+00	3.5E+00					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-B01-B	1	5.50E-01	U1/2		5.50E-01	4.3E+01	1.1E+00	3.5E+00					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-B02-B	1	2.47E+01			2.47E+01	1.9E+01	1.1E+00	3.5E+00					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1313-B03-B	1	2.27E+03			2.27E+03	1.2E+02	1.1E+00	3.5E+00					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	EaFA-L08-1313-T01-A	1	3.04E+05			3.04E+05	1.4E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T02-A	1	1.33E+05			1.33E+05	3.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T03-A	1	5.49E+04			5.49E+04	1.3E+00	2.5E+00	8.0E+00	1000	100	5.58E+04	95%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T04-A	1	2.98E+04			2.98E+04	5.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T05-A	1	1.43E+04			1.43E+04	5.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T06-A	1	4.94E+03			4.94E+03	1.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T07-A	1	4.53E+03			4.53E+03	1.3E+01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T08-A	1	3.77E+03			3.77E+03	6.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T09-A	1	2.46E+03			2.46E+03	1.8E+01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T01-B	1	2.82E+05			2.82E+05	5.6E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T02-B	1	1.18E+05			1.18E+05	3.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T03-B	1	4.79E+04			4.79E+04	5.5E+00	2.5E+00	8.0E+00	1000	100	4.89E+04	96%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T04-B	1	2.85E+04			2.85E+04	1.7E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T05-B	1	1.30E+04			1.30E+04	9.6E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T06-B	1	4.89E+03			4.89E+03	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T07-B	1	4.92E+03			4.92E+03	2.6E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T08-B	1	3.77E+03			3.77E+03	3.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T09-B	1	2.04E+03			2.04E+03	4.8E+01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T01-C	1	2.93E+05			2.93E+05	6.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T02-C	1	1.17E+05			1.17E+05	9.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T03-C	1	4.91E+04			4.91E+04	3.7E-01	2.5E+00	8.0E+00	1000	100	5.00E+04	92%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T04-C	1	7.19E+03			7.19E+03	1.6E+02	2.5E+00	8.0E+00					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T05-C	1	1.42E+04			1.42E+04	2.6E-01	2.5E+00	8.0E+00					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T06-C	1	4.85E+03			4.85E+03	8.8E-01	2.5E+00	8.0E+00					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T07-C	1	5.00E+03			5.00E+03	1.2E+00	2.5E+00	8.0E+00					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T08-C	1	3.60E+03			3.60E+03	3.1E+00	2.5E+00	8.0E+00					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-T09-C	1	1.04E+03			1.04E+03	1.3E+02	2.5E+00	8.0E+00					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-B01-A	1	2.25E+01			2.25E+01	4.2E-01	2.5E+00	8.0E+00					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-B02-A	1	1.95E+01			1.95E+01	1.0E+01	2.5E+00	8.0E+00					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-B03-A	1	3.09E+05			3.09E+05	1.5E-01	2.5E+00	8.0E+00					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-B01-B	1	1.97E+01			1.97E+01	7.9E+00	2.5E+00	8.0E+00					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-B02-B	1	3.10E+01			3.10E+01	1.1E+01	2.5E+00	8.0E+00					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1313-B03-B	1	1.17E+05			1.17E+05	1.1E+02	2.5E+00	8.0E+00					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	EaFA-L08-1313-T01-A	1	1.45E+03			1.45E+03	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T02-A	1	1.63E+03			1.63E+03	5.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T03-A	1	1.88E+03			1.88E+03	5.1E-01	1.0E+00	3.2E+00	1000	100	2.77E+03	89%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T04-A	1	1.83E+03			1.83E+03	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T05-A	1	1.97E+03			1.97E+03	3.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T06-A	1	2.10E+03			2.10E+03	5.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T07-A	1	2.27E+03			2.27E+03	1.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T08-A	1	2.68E+03			2.68E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T09-A	1	5.13E+03			5.13E+03	5.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T01-B	1	1.38E+03			1.38E+03	7.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T02-B	1	1.58E+03			1.58E+03	4.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T03-B	1	1.79E+03			1.79E+03	3.1E+00	1.0E+00	3.2E+00	1000	100	2.66E+03	87%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T04-B	1	1.81E+03			1.81E+03	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T05-B	1	1.84E+03			1.84E+03	8.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T06-B	1	2.17E+03			2.17E+03	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T07-B	1	2.56E+03			2.56E+03	4.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T08-B	1	2.72E+03			2.72E+03	2.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T09-B	1	4.23E+03			4.23E+03	2.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T01-C	1	1.50E+03			1.50E+03	9.7E-02	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T02-C	1	1.62E+03			1.62E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T03-C	1	1.88E+03			1.88E+03	3.7E-01	1.0E+00	3.2E+00	1000	100	2.72E+03	84%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T04-C	1	4.84E+02			4.84E+02	1.5E+02	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T05-C	1	2.02E+03			2.02E+03	8.2E-01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T06-C	1	2.15E+03			2.15E+03	7.9E-01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T07-C	1	2.69E+03			2.69E+03	3.4E-01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T08-C	1	2.70E+03			2.70E+03	3.5E-01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-T09-C	1	2.66E+03			2.66E+03	8.3E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	6.4E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	4.8E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	3.4E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	1.9E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	4.3E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	EaFA-L08-1313-T01-A	1	1.74E+05			1.74E+05	9.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T02-A	1	1.56E+05			1.56E+05	1.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T03-A	1	1.52E+05			1.52E+05	1.4E+00	6.8E+00	2.2E+01	1000	100	1.53E+05	89%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T04-A	1	1.54E+05			1.54E+05	6.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T05-A	1	1.53E+05			1.53E+05	2.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T06-A	1	1.48E+05			1.48E+05	5.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T07-A	1	1.26E+05			1.26E+05	1.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T08-A	1	9.77E+04			9.77E+04	4.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T09-A	1	4.58E+04			4.58E+04	1.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T01-B	1	1.69E+05			1.69E+05	8.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T02-B	1	1.46E+05			1.46E+05	3.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T03-B	1	1.44E+05			1.44E+05	4.4E+00	6.8E+00	2.2E+01	1000	100	1.45E+05	86%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T04-B	1	1.52E+05			1.52E+05	2.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T05-B	1	1.42E+05			1.42E+05	9.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T06-B	1	1.50E+05			1.50E+05	2.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T07-B	1	1.41E+05			1.41E+05	2.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T08-B	1	9.98E+04			9.98E+04	4.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T09-B	1	3.96E+04			3.96E+04	4.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T01-C	1	1.76E+05			1.76E+05	3.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T02-C	1	1.51E+05			1.51E+05	1.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T03-C	1	1.51E+05			1.51E+05	2.9E-01	6.8E+00	2.2E+01	1000	100	1.52E+05	87%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T04-C	1	3.93E+04			3.93E+04	1.5E+02	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T05-C	1	1.54E+05			1.54E+05	3.9E-01	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T06-C	1	1.49E+05			1.49E+05	3.9E-01	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T07-C	1	1.44E+05			1.44E+05	8.4E-01	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T08-C	1	9.54E+04			9.54E+04	2.2E+00	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-T09-C	1	1.94E+04			1.94E+04	1.3E+02	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-B01-A	1	1.32E+01	E		1.32E+01	3.8E+01	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	2.0E+02	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-B03-A	1	1.33E+02			1.33E+02	1.6E+01	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-B01-B	1	1.38E+01	E		1.38E+01	7.6E+00	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-B02-B	1	1.68E+01	E		1.68E+01	5.4E+01	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1313-B03-B	1	1.15E+01	E		1.15E+01	5.0E+02	6.8E+00	2.2E+01					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	EaFA-L08-1313-T01-A	1	9.00E+00	E		9.00E+00	2.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T02-A	1	2.30E+00	U1/2		2.30E+00	1.0E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T03-A	1	2.30E+00	U1/2		2.30E+00	2.4E+03	4.6E+00	1.5E+01	10	325	3.12E+03	96%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T04-A	1	2.30E+00	U1/2		2.30E+00	4.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T05-A	1	2.30E+00	U1/2		2.30E+00	1.1E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T06-A	1	2.30E+00	U1/2		2.30E+00	9.8E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T07-A	1	3.19E+01			3.19E+01	5.1E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T08-A	1	6.44E+01			6.44E+01	1.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T09-A	1	8.17E+01			8.17E+01	2.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T01-B	1	2.30E+00	U1/2		2.30E+00	3.2E+03	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T02-B	1	6.57E+00	E		6.57E+00	1.0E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T03-B	1	2.30E+00	U1/2		2.30E+00	6.6E+01	4.6E+00	1.5E+01	10	325	3.09E+03	95%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T04-B	1	2.30E+00	U1/2		2.30E+00	1.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T05-B	1	2.30E+00	U1/2		2.30E+00	2.2E+03	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T06-B	1	7.97E+00	E		7.97E+00	1.7E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T07-B	1	3.68E+01			3.68E+01	2.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T08-B	1	5.80E+01			5.80E+01	6.5E+00	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T09-B	1	5.56E+01			5.56E+01	6.5E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T01-C	1	1.11E+01	E		1.11E+01	7.8E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T02-C	1	2.30E+00	U1/2		2.30E+00	1.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T03-C	1	2.30E+00	U1/2		2.30E+00	2.6E+02	4.6E+00	1.5E+01	10	325	3.13E+03	96%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T04-C	1	2.30E+00	U1/2		2.30E+00	9.6E+01	4.6E+00	1.5E+01					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T05-C	1	2.30E+00	U1/2		2.30E+00	1.4E+02	4.6E+00	1.5E+01					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T06-C	1	7.04E+00	E		7.04E+00	2.4E+02	4.6E+00	1.5E+01					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T07-C	1	3.73E+01			3.73E+01	5.2E+01	4.6E+00	1.5E+01					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T08-C	1	7.17E+01			7.17E+01	1.1E+01	4.6E+00	1.5E+01					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-T09-C	1	1.59E+01			1.59E+01	3.2E+02	4.6E+00	1.5E+01					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	3.9E+02	4.6E+00	1.5E+01					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	7.5E+00	4.6E+00	1.5E+01					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	4.5E+01	4.6E+00	1.5E+01					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-B01-B	1	2.30E+00	U1/2		2.30E+00	8.4E+01	4.6E+00	1.5E+01					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-B02-B	1	2.30E+00	U1/2		2.30E+00	4.3E+01	4.6E+00	1.5E+01					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1313-B03-B	1	2.30E+00	U1/2		2.30E+00	2.0E+01	4.6E+00	1.5E+01					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	EaFA-L08-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	5.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	4.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	9.0E+01	2.0E+00	6.4E+00	10	325	3.16E+03	97%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	9.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	1.8E+03	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	7.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T08-A	1	8.47E+00			8.47E+00	6.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T09-A	1	5.17E+03			5.17E+03	3.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	1.5E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	8.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	3.7E+01	2.0E+00	6.4E+00	10	325	3.09E+03	95%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	1.1E+03	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	1.1E+03	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	2.8E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	2.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T08-B	1	8.08E+00			8.08E+00	3.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T09-B	1	2.65E+03			2.65E+03	2.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	7.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	2.0E+03	2.0E+00	6.4E+00	10	325	3.15E+03	97%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	8.2E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	3.1E+02	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	6.6E+03	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	1.4E+03	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T08-C	1	8.97E+00			8.97E+00	9.1E+00	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-T09-C	1	8.10E+02			8.10E+02	1.1E+02	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	5.0E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	1.0E+02	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-B03-A	1	5.79E+00	E		5.79E+00	5.0E+00	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	1.6E+02	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	3.8E+01	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	1.0E+02	2.0E+00	6.4E+00					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	EaFA-L08-1313-T01-A	1	5.51E+03			5.51E+03	5.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T02-A	1	3.14E+03			3.14E+03	8.8E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T03-A	1	3.29E+03			3.29E+03	2.7E-01	1.5E+00	4.8E+00	10	325	6.20E+03	90%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T04-A	1	9.89E+02			9.89E+02	2.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T05-A	1	4.95E+02			4.95E+02	1.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T06-A	1	3.65E+02			3.65E+02	1.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T07-A	1	1.20E+02			1.20E+02	1.3E+01	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T08-A	1	9.88E+01			9.88E+01	1.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T09-A	1	5.19E+03			5.19E+03	1.2E+01	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T01-B	1	5.31E+03			5.31E+03	6.9E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T02-B	1	2.67E+03			2.67E+03	4.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T03-B	1	2.78E+03			2.78E+03	2.9E+00	1.5E+00	4.8E+00	10	325	5.76E+03	92%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T04-B	1	1.06E+03			1.06E+03	2.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T05-B	1	4.76E+02			4.76E+02	8.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T06-B	1	3.55E+02			3.55E+02	2.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T07-B	1	1.54E+02			1.54E+02	3.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T08-B	1	9.41E+01			9.41E+01	1.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T09-B	1	4.45E+03			4.45E+03	3.9E+01	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T01-C	1	5.49E+03			5.49E+03	9.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T02-C	1	2.91E+03			2.91E+03	1.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T03-C	1	2.92E+03			2.92E+03	2.2E-01	1.5E+00	4.8E+00	10	325	5.90E+03	92%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T04-C	1	2.73E+02			2.73E+02	1.6E+02	1.5E+00	4.8E+00					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T05-C	1	5.60E+02			5.60E+02	2.3E+00	1.5E+00	4.8E+00					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T06-C	1	3.87E+02			3.87E+02	6.2E-01	1.5E+00	4.8E+00					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T07-C	1	1.58E+02			1.58E+02	8.4E-01	1.5E+00	4.8E+00					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T08-C	1	9.99E+01			9.99E+01	1.3E+00	1.5E+00	4.8E+00					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-T09-C	1	2.39E+03			2.39E+03	1.0E+02	1.5E+00	4.8E+00					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-B01-A	1	7.50E-01	U1/2		7.50E-01	1.1E+02	1.5E+00	4.8E+00					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-B02-A	1	7.50E-01	U1/2		7.50E-01	6.2E+02	1.5E+00	4.8E+00					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-B03-A	1	3.82E+00	E		3.82E+00	3.0E+01	1.5E+00	4.8E+00					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-B01-B	1	7.50E-01	U1/2		7.50E-01	1.7E+03	1.5E+00	4.8E+00					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-B02-B	1	7.50E-01	U1/2		7.50E-01	2.4E+02	1.5E+00	4.8E+00					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1313-B03-B	1	7.50E-01	U1/2		7.50E-01	1.8E+02	1.5E+00	4.8E+00					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	EaFA-L08-1313-T01-A	1	1.03E+02			1.03E+02	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:38 AM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T02-A	1	2.45E+01			2.45E+01	3.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:40 AM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T03-A	1	1.53E+01			1.53E+01	4.0E+00	1.0E+00	3.2E+00	10	325	3.37E+03	103%	VU ICP-OES	6/7/10 1:34 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T04-A	1	1.09E+01			1.09E+01	1.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:43 AM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T05-A	1	1.53E+01			1.53E+01	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:36 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T06-A	1	3.21E+01			3.21E+01	6.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:46 AM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T07-A	1	9.84E+02			9.84E+02	1.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:48 AM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T08-A	1	1.13E+03			1.13E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:50 AM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T09-A	1	1.60E+03			1.60E+03	5.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:51 AM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T01-B	1	7.26E+01			7.26E+01	1.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:03 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T02-B	1	2.00E+01			2.00E+01	6.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:39 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T03-B	1	1.39E+01			1.39E+01	5.8E+00	1.0E+00	3.2E+00	10	325	3.29E+03	101%	VU ICP-OES	6/7/10 12:06 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T04-B	1	1.24E+01			1.24E+01	6.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:08 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T05-B	1	1.47E+01			1.47E+01	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:09 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T06-B	1	2.22E+01			2.22E+01	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:11 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T07-B	1	9.57E+02			9.57E+02	3.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:41 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T08-B	1	1.14E+03			1.14E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:14 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T09-B	1	1.72E+03			1.72E+03	3.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:16 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T01-C	1	1.17E+02			1.17E+02	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:23 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T02-C	1	2.17E+01			2.17E+01	5.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:24 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T03-C	1	1.76E+01			1.76E+01	4.4E+00	1.0E+00	3.2E+00	10	325	3.34E+03	102%	VU ICP-OES	6/7/10 12:26 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T04-C	1	3.05E+00	E		3.05E+00	2.0E+02	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:28 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T05-C	1	1.85E+01			1.85E+01	3.2E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:29 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T06-C	1	3.18E+01			3.18E+01	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:31 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T07-C	1	9.74E+02			9.74E+02	9.2E-01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:32 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T08-C	1	1.12E+03			1.12E+03	9.9E-01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 1:44 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-T09-C	1	7.76E+02			7.76E+02	9.4E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:36 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-B01-A	1	9.59E+00			9.59E+00	6.6E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:33 AM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-B02-A	1	5.07E+00			5.07E+00	2.4E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:35 AM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-B03-A	1	9.54E+00			9.54E+00	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:36 AM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-B01-B	1	7.95E+00			7.95E+00	7.9E+00	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:58 AM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-B02-B	1	1.36E+01			1.36E+01	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 11:59 AM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1313-B03-B	1	5.22E+00			5.22E+00	6.4E+01	1.0E+00	3.2E+00					VU ICP-OES	6/7/10 12:01 PM	EPA Interlab L08 1313-1316 EaFA

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	EaFa-L09-1313-T01-A	1	3.79E+04			3.79E+04	1.6E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T02-A	1	3.57E+04			3.57E+04	1.2E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T03-A	1	2.69E+04			2.69E+04	3.4E-01	1.00E+00	3.18E+00	1000	100	2.78E+04	90%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T04-A	1	4.61E+03			4.61E+03	8.3E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T05-A	1	7.11E+02			7.11E+02	1.2E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T06-A	1	1.39E+02			1.39E+02	5.6E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T07-A	1	1.51E+03			1.51E+03	4.0E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T08-A	1	6.69E+04			6.69E+04	4.1E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T09-A	1	1.23E+05			1.23E+05	5.3E-02	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T01-B	1	4.04E+04			4.04E+04	2.2E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T02-B	1	3.89E+04			3.89E+04	6.4E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T03-B	1	2.60E+04			2.60E+04	2.2E+00	1.00E+00	3.18E+00	1000	100	2.69E+04	91%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T04-B	1	4.40E+03			4.40E+03	2.3E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T05-B	1	1.35E+03			1.35E+03	5.8E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T06-B	1	1.88E+02			1.88E+02	9.6E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T07-B	1	1.78E+03			1.78E+03	3.6E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T08-B	1	6.79E+04			6.79E+04	3.8E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T09-B	1	1.22E+05			1.22E+05	1.2E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T01-C	1	4.00E+04			4.00E+04	9.2E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T02-C	1	3.79E+04			3.79E+04	1.1E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T03-C	1	2.51E+04			2.51E+04	4.0E-01	1.00E+00	3.18E+00	1000	100	2.60E+04	92%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T04-C	1	4.87E+03			4.87E+03	6.2E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T05-C	1	1.10E+03			1.10E+03	4.9E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T06-C	1	2.18E+02			2.18E+02	2.3E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T07-C	1	1.59E+03			1.59E+03	4.2E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T08-C	1	6.62E+04			6.62E+04	2.9E-02	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-T09-C	1	1.21E+05			1.21E+05	9.7E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.5E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.2E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
Al	EaFa-L09-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	1.2E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	EaFa-L09-1313-T01-A	1	2.22E+02			2.22E+02	8.6E+00	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T02-A	1	1.52E+02			1.52E+02	8.9E+00	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T03-A	1	1.88E+02			1.88E+02	1.1E+01	7.50E+00	2.39E+01	10	325	3.58E+03	104%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T04-A	1	2.25E+02			2.25E+02	8.4E+00	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T05-A	1	1.90E+02			1.90E+02	4.6E+00	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T06-A	1	1.79E+02			1.79E+02	3.3E+00	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T07-A	1	7.23E+01			7.23E+01	3.8E+01	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T08-A	1	2.08E+01	E		2.08E+01	2.0E+01	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T09-A	1	9.33E+00	E		9.33E+00	8.8E+01	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T01-B	1	2.11E+02			2.11E+02	1.1E+01	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T02-B	1	1.63E+02			1.63E+02	1.1E+01	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T03-B	1	1.74E+02			1.74E+02	4.3E+00	7.50E+00	2.39E+01	10	325	3.50E+03	102%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T04-B	1	1.96E+02			1.96E+02	1.4E+01	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T05-B	1	1.93E+02			1.93E+02	1.3E+01	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T06-B	1	1.93E+02			1.93E+02	5.1E+00	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T07-B	1	8.77E+01			8.77E+01	1.3E+01	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T08-B	1	2.45E+01			2.45E+01	4.6E+01	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T09-B	1	1.22E+01	E		1.22E+01	8.6E+01	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T01-C	1	2.17E+02			2.17E+02	5.3E+00	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T02-C	1	1.42E+02			1.42E+02	1.0E+01	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T03-C	1	1.77E+02			1.77E+02	1.2E+01	7.50E+00	2.39E+01	10	325	3.53E+03	103%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T04-C	1	1.94E+02			1.94E+02	3.3E+00	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T05-C	1	1.72E+02			1.72E+02	1.0E+01	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T06-C	1	1.50E+02			1.50E+02	6.0E+00	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T07-C	1	9.35E+01			9.35E+01	1.9E+01	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T08-C	1	2.42E+01			2.42E+01	3.0E+01	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-T09-C	1	3.75E+00	U1/2		3.75E+00	9.3E+00	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-B01-A	1	3.18E+01			3.18E+01	7.8E+01	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-B02-A	1	2.27E+01	E		2.27E+01	8.1E+01	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
Sb	EaFa-L09-1313-B03-A	1	2.59E+01			2.59E+01	9.7E+01	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	EaFa-L09-1313-T01-A	1	7.95E+03			7.95E+03	4.1E-01	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T02-A	1	9.89E+02			9.89E+02	3.9E+00	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T03-A	1	1.16E+03			1.16E+03	2.0E+00	1.10E+01	3.50E+01	10	325	4.40E+03	100%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T04-A	1	4.77E+02			4.77E+02	1.6E+00	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T05-A	1	1.81E+02			1.81E+02	7.6E+00	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T06-A	1	1.18E+02			1.18E+02	2.2E+01	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T07-A	1	1.25E+02			1.25E+02	1.2E+01	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T08-A	1	1.13E+02			1.13E+02	1.4E+00	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T09-A	1	1.32E+03			1.32E+03	6.4E-01	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T01-B	1	8.04E+03			8.04E+03	1.7E+00	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T02-B	1	1.02E+03			1.02E+03	1.7E+00	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T03-B	1	1.13E+03			1.13E+03	4.3E+00	1.10E+01	3.50E+01	10	325	4.32E+03	98%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T04-B	1	3.82E+02			3.82E+02	3.0E+00	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T05-B	1	2.22E+02			2.22E+02	4.1E+00	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T06-B	1	1.10E+02			1.10E+02	9.1E+00	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T07-B	1	1.61E+02			1.61E+02	1.3E+01	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T08-B	1	1.28E+02			1.28E+02	3.5E+00	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T09-B	1	1.38E+03			1.38E+03	8.0E-01	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T01-C	1	7.95E+03			7.95E+03	9.1E-01	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T02-C	1	1.02E+03			1.02E+03	7.1E-01	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T03-C	1	1.11E+03			1.11E+03	5.2E-01	1.10E+01	3.50E+01	10	325	4.36E+03	100%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T04-C	1	3.46E+02			3.46E+02	2.6E+00	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T05-C	1	2.20E+02			2.20E+02	4.5E+00	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T06-C	1	1.14E+02			1.14E+02	1.7E+01	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T07-C	1	1.59E+02			1.59E+02	1.2E+01	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T08-C	1	1.31E+02			1.31E+02	7.7E+00	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-T09-C	1	1.39E+03			1.39E+03	5.0E-01	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-B01-A	1	2.15E+01	E		2.15E+01	1.1E+01	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-B02-A	1	3.14E+01	E		3.14E+01	2.0E+01	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
As	EaFa-L09-1313-B03-A	1	2.76E+01	E		2.76E+01	4.0E+01	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	EaFa-L09-1313-T01-A	1	4.50E+03			4.50E+03	9.6E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T02-A	1	4.43E+03			4.43E+03	2.9E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T03-A	1	4.41E+03			4.41E+03	2.1E+00	1.00E+00	3.18E+00	1000	100	5.40E+03	99%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T04-A	1	4.17E+03			4.17E+03	1.5E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T05-A	1	4.41E+03			4.41E+03	1.9E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T06-A	1	4.57E+03			4.57E+03	8.3E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T07-A	1	4.57E+03			4.57E+03	2.9E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T08-A	1	3.58E+03			3.58E+03	3.5E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T09-A	1	3.07E+03			3.07E+03	4.1E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T01-B	1	4.66E+03			4.66E+03	1.4E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T02-B	1	4.67E+03			4.67E+03	1.2E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T03-B	1	4.41E+03			4.41E+03	8.4E-01	1.00E+00	3.18E+00	1000	100	5.25E+03	84%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T04-B	1	4.32E+03			4.32E+03	1.7E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T05-B	1	4.49E+03			4.49E+03	1.3E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T06-B	1	4.68E+03			4.68E+03	5.7E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T07-B	1	4.50E+03			4.50E+03	3.1E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T08-B	1	3.62E+03			3.62E+03	5.0E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T09-B	1	3.10E+03			3.10E+03	1.4E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T01-C	1	4.70E+03			4.70E+03	1.1E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T02-C	1	4.50E+03			4.50E+03	1.3E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T03-C	1	4.20E+03			4.20E+03	3.6E+00	1.00E+00	3.18E+00	1000	100	5.16E+03	96%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T04-C	1	4.33E+03			4.33E+03	1.3E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T05-C	1	4.30E+03			4.30E+03	1.7E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T06-C	1	4.62E+03			4.62E+03	1.8E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T07-C	1	4.50E+03			4.50E+03	5.8E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T08-C	1	3.62E+03			3.62E+03	2.5E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-T09-C	1	3.09E+03			3.09E+03	4.3E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-B01-A	1	3.67E+01			3.67E+01	2.8E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-B02-A	1	3.06E+01			3.06E+01	1.9E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
B	EaFa-L09-1313-B03-A	1	3.31E+01			3.31E+01	3.6E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	EaFa-L09-1313-T01-A	1	1.02E+03			1.02E+03	7.6E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T02-A	1	1.10E+03			1.10E+03	1.6E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T03-A	1	8.15E+02			8.15E+02	5.3E-01	1.00E+00	3.18E+00	10	325	3.80E+03	92%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T04-A	1	4.08E+02			4.08E+02	9.3E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T05-A	1	2.93E+02			2.93E+02	6.9E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T06-A	1	2.65E+02			2.65E+02	3.5E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T07-A	1	2.89E+02			2.89E+02	2.0E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T08-A	1	3.63E+02			3.63E+02	4.6E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T09-A	1	7.88E+02			7.88E+02	5.4E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T01-B	1	1.23E+03			1.23E+03	1.5E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T02-B	1	1.15E+03			1.15E+03	3.8E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T03-B	1	1.15E+03			1.15E+03	2.1E+00	1.00E+00	3.18E+00	10	325	4.02E+03	88%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T04-B	1	3.87E+02			3.87E+02	4.8E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T05-B	1	3.28E+02			3.28E+02	7.2E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T06-B	1	2.95E+02			2.95E+02	5.7E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T07-B	1	2.76E+02			2.76E+02	5.3E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T08-B	1	3.77E+02			3.77E+02	6.9E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T09-B	1	8.32E+02			8.32E+02	2.6E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T01-C	1	1.34E+03			1.34E+03	8.7E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T02-C	1	1.15E+03			1.15E+03	1.5E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T03-C	1	1.10E+03			1.10E+03	5.5E-01	1.00E+00	3.18E+00	10	325	4.02E+03	90%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T04-C	1	3.85E+02			3.85E+02	9.0E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T05-C	1	3.11E+02			3.11E+02	2.2E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T06-C	1	2.89E+02			2.89E+02	3.1E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T07-C	1	2.80E+02			2.80E+02	5.7E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T08-C	1	3.76E+02			3.76E+02	1.4E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-T09-C	1	8.38E+02			8.38E+02	2.7E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	4.9E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	6.8E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
Ba	EaFa-L09-1313-B03-A	1	1.53E+00	E		1.53E+00	1.2E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	EaFa-L09-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	1.1E+01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	1.8E+01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	4.0E+01	1.90E+00	6.00E+00	10	325	3.50E+03	108%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	2.9E+01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	2.0E+02	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T07-A	1	1.27E+01			1.27E+01	7.4E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T08-A	1	1.85E+02			1.85E+02	7.1E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T09-A	1	2.53E+02			2.53E+02	1.7E+00	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	8.7E+00	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	6.1E+01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	4.7E+01	1.90E+00	6.00E+00	10	325	3.41E+03	105%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	2.7E+02	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	3.4E+01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	8.4E+01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T07-B	1	1.57E+01			1.57E+01	7.3E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T08-B	1	1.88E+02			1.88E+02	4.3E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T09-B	1	2.53E+02			2.53E+02	4.0E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	2.6E+01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	2.4E+02	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	2.2E+02	1.90E+00	6.00E+00	10	325	3.44E+03	106%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	3.1E+02	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	5.2E+01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	1.3E+03	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T07-C	1	1.44E+01			1.44E+01	2.2E+00	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T08-C	1	1.87E+02			1.87E+02	4.3E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-T09-C	1	2.52E+02			2.52E+02	5.0E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	1.5E+02	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	3.4E+01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
Be	EaFa-L09-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	EaFa-L09-1313-T01-A	1	1.10E+00	U1/2		1.10E+00	1.1E+01	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T02-A	1	1.10E+00	U1/2		1.10E+00	4.0E+00	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	4.8E+00	2.20E+00	7.00E+00	10	325	3.50E+03	108%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T04-A	1	1.10E+00	U1/2		1.10E+00	1.0E+01	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T05-A	1	1.10E+00	U1/2		1.10E+00	8.9E+00	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T06-A	1	1.10E+00	U1/2		1.10E+00	7.6E+00	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T07-A	1	3.11E+01			3.11E+01	4.2E+00	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T08-A	1	2.23E+01			2.23E+01	3.5E+00	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T09-A	1	2.72E+01			2.72E+01	4.4E-01	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T01-B	1	1.10E+00	U1/2		1.10E+00	8.1E+00	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T02-B	1	1.10E+00	U1/2		1.10E+00	8.1E+00	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	7.6E+00	2.20E+00	7.00E+00	10	325	3.42E+03	105%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T04-B	1	1.10E+00	U1/2		1.10E+00	8.4E+00	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T05-B	1	1.10E+00	U1/2		1.10E+00	7.2E+00	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T06-B	1	1.10E+00	U1/2		1.10E+00	1.3E+00	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T07-B	1	3.07E+01			3.07E+01	8.8E-01	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T08-B	1	2.26E+01			2.26E+01	8.6E-01	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T09-B	1	2.71E+01			2.71E+01	1.9E+00	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T01-C	1	1.10E+00	U1/2		1.10E+00	1.5E+01	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T02-C	1	1.10E+00	U1/2		1.10E+00	1.2E+01	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	7.8E+00	2.20E+00	7.00E+00	10	325	3.45E+03	106%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T04-C	1	1.10E+00	U1/2		1.10E+00	8.2E+00	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T05-C	1	1.10E+00	U1/2		1.10E+00	4.6E+00	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T06-C	1	1.10E+00	U1/2		1.10E+00	7.4E+00	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T07-C	1	3.11E+01			3.11E+01	6.9E-01	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T08-C	1	2.29E+01			2.29E+01	8.8E-01	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-T09-C	1	2.68E+01			2.68E+01	2.0E+00	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	7.6E+00	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	1.0E+01	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
Cd	EaFa-L09-1313-B03-A	1	1.10E+00	U1/2		1.10E+00	1.0E+01	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	EaFa-L09-1313-T01-A	1	1.57E+04			1.57E+04	8.1E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T02-A	1	5.19E+04			5.19E+04	1.4E+00	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T03-A	1	1.01E+05			1.01E+05	5.0E-01	2.60E+00	8.30E+00	1000	100	1.02E+05	81%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T04-A	1	1.32E+05			1.32E+05	1.5E+00	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T05-A	1	1.46E+05			1.46E+05	8.5E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T06-A	1	1.62E+05			1.62E+05	4.7E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T07-A	1	1.60E+05			1.60E+05	7.3E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T08-A	1	1.49E+05			1.49E+05	4.1E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T09-A	1	1.40E+05			1.40E+05	4.6E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T01-B	1	1.68E+04			1.68E+04	1.3E+00	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T02-B	1	4.88E+04			4.88E+04	4.9E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T03-B	1	9.87E+04			9.87E+04	2.2E+00	2.60E+00	8.30E+00	1000	100	9.96E+04	87%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T04-B	1	1.30E+05			1.30E+05	6.3E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T05-B	1	1.44E+05			1.44E+05	8.9E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T06-B	1	1.61E+05			1.61E+05	7.9E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T07-B	1	1.58E+05			1.58E+05	3.9E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T08-B	1	1.49E+05			1.49E+05	7.5E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T09-B	1	1.41E+05			1.41E+05	7.4E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T01-C	1	1.71E+04			1.71E+04	4.8E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T02-C	1	4.73E+04			4.73E+04	4.7E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T03-C	1	9.26E+04			9.26E+04	5.3E-01	2.60E+00	8.30E+00	1000	100	9.34E+04	86%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T04-C	1	1.27E+05			1.27E+05	6.9E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T05-C	1	1.36E+05			1.36E+05	4.4E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T06-C	1	1.57E+05			1.57E+05	6.7E-02	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T07-C	1	1.57E+05			1.57E+05	1.1E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T08-C	1	1.45E+05			1.45E+05	7.3E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-T09-C	1	1.39E+05			1.39E+05	6.2E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-B01-A	1	1.30E+00	U1/2		1.30E+00	9.4E+01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-B02-A	1	1.30E+00	U1/2		1.30E+00	5.6E+01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
Ca	EaFa-L09-1313-B03-A	1	9.17E+00			9.17E+00	2.2E+01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	EaFa-L09-1313-T01-A	1	4.26E+02			4.26E+02	6.9E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T02-A	1	3.17E+02			3.17E+02	8.3E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T03-A	1	2.59E+02			2.59E+02	8.9E-02	1.20E+00	3.82E+00	10	325	3.59E+03	103%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T04-A	1	1.81E+02			1.81E+02	1.9E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T05-A	1	7.84E+01			7.84E+01	1.4E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T06-A	1	1.81E+01			1.81E+01	4.2E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T07-A	1	1.69E+00	E		1.69E+00	6.4E+01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T08-A	1	9.29E+02			9.29E+02	1.0E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T09-A	1	1.83E+03			1.83E+03	3.4E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T01-B	1	4.13E+02			4.13E+02	2.5E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T02-B	1	3.14E+02			3.14E+02	2.1E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T03-B	1	2.21E+02			2.21E+02	1.6E+00	1.20E+00	3.82E+00	10	325	3.47E+03	100%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T04-B	1	1.66E+02			1.66E+02	1.1E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T05-B	1	1.20E+02			1.20E+02	1.0E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T06-B	1	2.51E+01			2.51E+01	1.2E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T07-B	1	2.51E+00	E		2.51E+00	2.2E+01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T08-B	1	9.90E+02			9.90E+02	8.8E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T09-B	1	1.85E+03			1.85E+03	3.0E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T01-C	1	4.25E+02			4.25E+02	7.7E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T02-C	1	2.97E+02			2.97E+02	5.5E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T03-C	1	2.19E+02			2.19E+02	9.4E-01	1.20E+00	3.82E+00	10	325	3.49E+03	101%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T04-C	1	1.68E+02			1.68E+02	1.3E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T05-C	1	1.15E+02			1.15E+02	4.0E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T06-C	1	3.42E+01			3.42E+01	5.7E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T07-C	1	2.76E+00	E		2.76E+00	6.9E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T08-C	1	9.44E+02			9.44E+02	4.6E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-T09-C	1	1.82E+03			1.82E+03	2.1E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	7.9E+01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	2.5E+01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
Cr	EaFa-L09-1313-B03-A	1	1.49E+00	E		1.49E+00	1.4E+02	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	EaFa-L09-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	1.6E+02	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	1.9E+02	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	5.9E+01	1.80E+00	5.72E+00	10	325	3.38E+03	104%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	1.0E+02	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T05-A	1	8.06E+00			8.06E+00	3.6E+01	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T06-A	1	6.17E+01			6.17E+01	3.1E+00	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T07-A	1	2.45E+02			2.45E+02	5.7E-01	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T08-A	1	2.46E+02			2.46E+02	1.3E+00	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T09-A	1	3.91E+02			3.91E+02	3.9E-01	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	5.0E+01	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	2.2E+02	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T03-B	1	2.53E+00	E		2.53E+00	3.5E+01	1.80E+00	5.72E+00	10	325	3.28E+03	101%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T04-B	1	2.55E+00	E		2.55E+00	6.4E+01	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T05-B	1	3.86E+00	E		3.86E+00	2.1E+01	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T06-B	1	4.63E+01			4.63E+01	2.1E+00	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T07-B	1	2.31E+02			2.31E+02	1.0E+00	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T08-B	1	2.46E+02			2.46E+02	6.1E-01	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T09-B	1	3.91E+02			3.91E+02	4.1E-01	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	2.3E+02	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	7.2E+01	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T03-C	1	1.92E+00	E		1.92E+00	1.1E+02	1.80E+00	5.72E+00	10	325	3.30E+03	101%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T04-C	1	2.62E+00	E		2.62E+00	7.2E+01	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T05-C	1	6.25E+00			6.25E+00	2.1E+01	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T06-C	1	3.19E+01			3.19E+01	7.6E+00	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T07-C	1	2.35E+02			2.35E+02	1.6E+00	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T08-C	1	2.44E+02			2.44E+02	3.4E-01	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-T09-C	1	3.86E+02			3.86E+02	2.6E-01	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-B01-A	1	2.27E+00	E		2.27E+00	2.6E+01	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	2.4E+02	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
Co	EaFa-L09-1313-B03-A	1	3.46E+00	E		3.46E+00	9.1E+01	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	EaFa-L09-1313-T01-A	1	4.41E+01			4.41E+01	5.2E+00	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T02-A	1	4.10E+00	E		4.10E+00	2.9E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T03-A	1	6.47E+00	E		6.47E+00	2.5E+01	3.70E+00	1.18E+01	10	325	3.31E+03	102%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T04-A	1	7.27E+00	E		7.27E+00	7.1E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T05-A	1	1.07E+01	E		1.07E+01	1.9E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T06-A	1	1.01E+01	E		1.01E+01	5.4E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T07-A	1	3.42E+02			3.42E+02	6.1E-01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T08-A	1	2.40E+03			2.40E+03	1.4E+00	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T09-A	1	3.06E+03			3.06E+03	6.6E-01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T01-B	1	4.44E+01			4.44E+01	4.8E+00	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T02-B	1	7.86E+00	E		7.86E+00	4.0E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T03-B	1	6.81E+00	E		6.81E+00	5.8E+01	3.70E+00	1.18E+01	10	325	3.23E+03	99%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T04-B	1	7.65E+00	E		7.65E+00	2.2E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T05-B	1	9.09E+00	E		9.09E+00	4.2E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T06-B	1	9.76E+00	E		9.76E+00	3.4E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T07-B	1	4.25E+02			4.25E+02	1.9E+00	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T08-B	1	2.45E+03			2.45E+03	7.6E-01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T09-B	1	3.06E+03			3.06E+03	6.6E-01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T01-C	1	4.60E+01			4.60E+01	7.2E+00	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T02-C	1	7.99E+00	E		7.99E+00	1.8E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T03-C	1	4.03E+00	E		4.03E+00	1.9E+01	3.70E+00	1.18E+01	10	325	3.26E+03	100%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T04-C	1	7.54E+00	E		7.54E+00	1.7E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T05-C	1	7.53E+00	E		7.53E+00	6.4E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T06-C	1	1.11E+01	E		1.11E+01	3.9E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T07-C	1	3.78E+02			3.78E+02	7.2E-01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T08-C	1	2.38E+03			2.38E+03	3.9E-01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-T09-C	1	3.03E+03			3.03E+03	9.4E-01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	1.9E+02	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	1.0E+02	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
Cu	EaFa-L09-1313-B03-A	1	1.85E+00	U1/2		1.85E+00	2.3E+02	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	EaFa-L09-1313-T01-A	1	4.74E+01			4.74E+01	1.9E+00	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T02-A	1	2.96E+01			2.96E+01	1.2E+00	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T03-A	1	3.62E+00	E		3.62E+00	5.4E+00	2.00E+00	6.40E+00	1000	100	1.08E+03	108%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	6.8E+02	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	5.6E+03	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	6.9E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	3.1E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T08-A	1	2.98E+03			2.98E+03	8.7E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T09-A	1	3.11E+04			3.11E+04	2.1E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T01-B	1	5.27E+01			5.27E+01	2.9E+00	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T02-B	1	3.35E+01			3.35E+01	9.2E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T03-B	1	3.99E+00	E		3.99E+00	8.3E+00	2.00E+00	6.40E+00	1000	100	1.04E+03	104%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T04-B	1	4.81E+00	E		4.81E+00	3.0E+00	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	7.1E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	4.3E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T07-B	1	2.53E+00	E		2.53E+00	1.4E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T08-B	1	3.21E+03			3.21E+03	2.8E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T09-B	1	3.10E+04			3.10E+04	5.9E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T01-C	1	5.10E+01			5.10E+01	7.1E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T02-C	1	3.20E+01			3.20E+01	1.0E+00	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T03-C	1	3.96E+00	E		3.96E+00	3.7E+00	2.00E+00	6.40E+00	1000	100	1.05E+03	105%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	7.9E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T07-C	1	2.30E+00	E		2.30E+00	1.4E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T08-C	1	3.03E+03			3.03E+03	7.4E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-T09-C	1	3.05E+04			3.05E+04	4.0E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	5.1E+02	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	6.5E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
Fe	EaFa-L09-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	EaFa-L09-1313-T01-A	1	7.72E+00	E		7.72E+00	2.1E+02	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T02-A	1	3.40E+00	U1/2		3.40E+00	8.2E+02	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T03-A	1	3.40E+00	U1/2		3.40E+00	6.6E+01	6.80E+00	2.16E+01	10	325	3.35E+03	103%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T04-A	1	3.40E+00	U1/2		3.40E+00	3.4E+01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T05-A	1	3.40E+00	U1/2		3.40E+00	3.7E+02	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T06-A	1	3.40E+00	U1/2		3.40E+00	5.7E+02	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T07-A	1	3.40E+00	U1/2		3.40E+00	6.8E+01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T08-A	1	3.40E+00	U1/2		3.40E+00	4.3E+01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T09-A	1	6.92E+01			6.92E+01	6.3E+00	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T01-B	1	1.62E+01	E		1.62E+01	3.7E+01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T02-B	1	3.40E+00	U1/2		3.40E+00	6.2E+01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T03-B	1	3.40E+00	U1/2		3.40E+00	2.4E+02	6.80E+00	2.16E+01	10	325	3.23E+03	99%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T04-B	1	3.40E+00	U1/2		3.40E+00	6.4E+01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T05-B	1	3.40E+00	U1/2		3.40E+00	5.0E+01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T06-B	1	3.40E+00	U1/2		3.40E+00	8.6E+01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T07-B	1	3.40E+00	U1/2		3.40E+00	1.6E+02	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T08-B	1	3.40E+00	U1/2		3.40E+00	2.4E+01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T09-B	1	6.69E+01			6.69E+01	9.1E+00	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T01-C	1	3.40E+00	U1/2		3.40E+00	1.3E+03	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T02-C	1	3.40E+00	U1/2		3.40E+00	4.6E+01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T03-C	1	3.40E+00	U1/2		3.40E+00	2.9E+02	6.80E+00	2.16E+01	10	325	3.27E+03	100%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T04-C	1	3.40E+00	U1/2		3.40E+00	8.2E+01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T05-C	1	3.40E+00	U1/2		3.40E+00	2.2E+04	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T06-C	1	3.40E+00	U1/2		3.40E+00	9.6E+01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T07-C	1	3.40E+00	U1/2		3.40E+00	1.6E+02	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T08-C	1	3.40E+00	U1/2		3.40E+00	8.0E+01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-T09-C	1	6.87E+01			6.87E+01	8.3E+00	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	2.0E+03	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	6.5E+01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
Pb	EaFa-L09-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	3.6E+02	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	EaFa-L09-1313-T01-A	1	2.30E+03			2.30E+03	7.5E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T02-A	1	3.03E+03			3.03E+03	1.4E+00	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T03-A	1	3.53E+03			3.53E+03	5.4E-01	1.90E+00	6.00E+00	10	325	6.60E+03	94%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T04-A	1	3.71E+03			3.71E+03	7.6E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T05-A	1	3.99E+03			3.99E+03	7.0E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T06-A	1	4.18E+03			4.18E+03	2.7E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T07-A	1	3.85E+03			3.85E+03	4.7E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T08-A	1	2.34E+03			2.34E+03	5.3E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T09-A	1	1.86E+03			1.86E+03	9.0E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T01-B	1	2.40E+03			2.40E+03	1.1E+00	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T02-B	1	3.09E+03			3.09E+03	4.6E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T03-B	1	3.41E+03			3.41E+03	1.8E+00	1.90E+00	6.00E+00	10	325	6.41E+03	92%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T04-B	1	3.40E+03			3.40E+03	3.5E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T05-B	1	3.84E+03			3.84E+03	5.9E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T06-B	1	4.12E+03			4.12E+03	6.1E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T07-B	1	3.78E+03			3.78E+03	1.0E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T08-B	1	2.31E+03			2.31E+03	9.7E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T09-B	1	1.85E+03			1.85E+03	5.1E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T01-C	1	2.40E+03			2.40E+03	8.2E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T02-C	1	2.99E+03			2.99E+03	2.1E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T03-C	1	3.23E+03			3.23E+03	5.8E-01	1.90E+00	6.00E+00	10	325	6.32E+03	95%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T04-C	1	3.37E+03			3.37E+03	7.8E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T05-C	1	3.68E+03			3.68E+03	3.1E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T06-C	1	3.98E+03			3.98E+03	3.4E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T07-C	1	3.75E+03			3.75E+03	8.3E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T08-C	1	2.29E+03			2.29E+03	2.5E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-T09-C	1	1.82E+03			1.82E+03	8.0E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	2.4E+02	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
Li	EaFa-L09-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	7.4E+02	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	EaFa-L09-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	9.3E+00	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	5.6E+01	2.00E+00	6.40E+00	10	325	3.59E+03	110%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T04-A	1	4.35E+00	E		4.35E+00	8.9E+00	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T05-A	1	8.56E+01			8.56E+01	1.1E+00	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T06-A	1	4.51E+02			4.51E+02	4.1E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T07-A	1	9.80E+02			9.80E+02	1.2E+00	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T08-A	1	1.40E+03			1.40E+03	3.9E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T09-A	1	1.74E+03			1.74E+03	7.2E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	1.0E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	7.9E+03	2.00E+00	6.40E+00	10	325	3.47E+03	107%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T04-B	1	5.03E+00	E		5.03E+00	4.6E+00	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T05-B	1	3.73E+01			3.73E+01	1.2E+00	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T06-B	1	3.57E+02			3.57E+02	1.1E+00	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T07-B	1	9.73E+02			9.73E+02	8.4E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T08-B	1	1.40E+03			1.40E+03	4.9E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T09-B	1	1.74E+03			1.74E+03	2.0E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	5.2E+02	2.00E+00	6.40E+00	10	325	3.49E+03	107%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T04-C	1	4.06E+00	E		4.06E+00	4.0E+00	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T05-C	1	4.28E+01			4.28E+01	5.0E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T06-C	1	2.91E+02			2.91E+02	1.0E+00	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T07-C	1	9.75E+02			9.75E+02	9.1E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T08-C	1	1.38E+03			1.38E+03	1.5E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-T09-C	1	1.73E+03			1.73E+03	6.8E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	4.3E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	5.3E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
Mn	EaFa-L09-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	2.6E+02	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	EaFa-L09-1313-T01-A	1	5.00E-01	U1/2		5.00E-01	1.9E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T02-A	1	5.00E-01	U1/2		5.00E-01	4.0E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T03-A	1	4.12E+02			4.12E+02	5.4E-01	1.00E+00	3.18E+00	1000	100	1.49E+03	108%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T04-A	1	3.72E+03			3.72E+03	1.0E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T05-A	1	6.32E+03			6.32E+03	1.9E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T06-A	1	8.03E+03			8.03E+03	1.7E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T07-A	1	8.92E+03			8.92E+03	6.5E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T08-A	1	1.01E+04			1.01E+04	1.2E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T09-A	1	1.46E+04			1.46E+04	9.8E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T01-B	1	5.00E-01	U1/2		5.00E-01	1.4E+02	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T02-B	1	5.00E-01	U1/2		5.00E-01	2.1E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T03-B	1	3.57E+02			3.57E+02	4.3E+00	1.00E+00	3.18E+00	1000	100	1.40E+03	105%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T04-B	1	3.80E+03			3.80E+03	1.3E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T05-B	1	5.69E+03			5.69E+03	1.3E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T06-B	1	8.12E+03			8.12E+03	6.6E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T07-B	1	8.57E+03			8.57E+03	5.5E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T08-B	1	1.02E+04			1.02E+04	1.2E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T09-B	1	1.44E+04			1.44E+04	6.7E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T01-C	1	5.00E-01	U1/2		5.00E-01	6.5E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T02-C	1	5.00E-01	U1/2		5.00E-01	6.6E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T03-C	1	3.19E+02			3.19E+02	1.9E+00	1.00E+00	3.18E+00	1000	100	1.40E+03	108%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T04-C	1	3.92E+03			3.92E+03	9.0E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T05-C	1	5.52E+03			5.52E+03	5.5E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T06-C	1	8.04E+03			8.04E+03	6.8E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T07-C	1	8.57E+03			8.57E+03	1.1E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T08-C	1	9.91E+03			9.91E+03	5.7E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-T09-C	1	1.43E+04			1.43E+04	6.9E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	5.2E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	5.4E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
Mg	EaFa-L09-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	3.8E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	EaFa-L09-1313-T01-A	1	4.32E+03			4.32E+03	1.8E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T02-A	1	4.32E+03			4.32E+03	5.6E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T03-A	1	4.17E+03			4.17E+03	9.9E-01	1.20E+00	3.82E+00	10	325	7.37E+03	99%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T04-A	1	3.98E+03			3.98E+03	1.7E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T05-A	1	3.78E+03			3.78E+03	5.6E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T06-A	1	3.35E+03			3.35E+03	5.7E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T07-A	1	2.57E+02			2.57E+02	1.5E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T08-A	1	8.92E+01			8.92E+01	2.9E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T09-A	1	3.14E+02			3.14E+02	5.1E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T01-B	1	4.61E+03			4.61E+03	2.2E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T02-B	1	4.39E+03			4.39E+03	1.0E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T03-B	1	4.07E+03			4.07E+03	2.0E+00	1.20E+00	3.82E+00	10	325	7.23E+03	97%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T04-B	1	3.89E+03			3.89E+03	1.1E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T05-B	1	3.81E+03			3.81E+03	1.4E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T06-B	1	3.48E+03			3.48E+03	5.9E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T07-B	1	2.47E+02			2.47E+02	9.7E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T08-B	1	9.21E+01			9.21E+01	2.1E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T09-B	1	3.33E+02			3.33E+02	1.8E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T01-C	1	4.48E+03			4.48E+03	1.1E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T02-C	1	4.18E+03			4.18E+03	1.4E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T03-C	1	3.83E+03			3.83E+03	6.9E-01	1.20E+00	3.82E+00	10	325	7.17E+03	103%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T04-C	1	3.80E+03			3.80E+03	1.1E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T05-C	1	3.63E+03			3.63E+03	8.5E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T06-C	1	3.45E+03			3.45E+03	1.1E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T07-C	1	2.68E+02			2.68E+02	8.5E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T08-C	1	9.17E+01			9.17E+01	2.9E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-T09-C	1	3.27E+02			3.27E+02	6.2E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	3.7E+01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	6.5E+01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
Mo	EaFa-L09-1313-B03-A	1	6.00E-01	U1/2		6.00E-01	2.0E+02	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	EaFa-L09-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	7.4E+02	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T03-A	1	5.26E+00	E		5.26E+00	1.1E+02	1.80E+00	5.70E+00	10	325	3.41E+03	105%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T04-A	1	1.82E+00	E		1.82E+00	2.8E+02	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T05-A	1	2.63E+01			2.63E+01	2.1E+01	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T06-A	1	1.42E+02			1.42E+02	1.3E+00	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T07-A	1	6.14E+02			6.14E+02	3.9E-01	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T08-A	1	5.46E+02			5.46E+02	7.4E-01	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T09-A	1	7.17E+02			7.17E+02	6.2E-01	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	4.9E+02	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T02-B	1	2.17E+00	E		2.17E+00	1.3E+02	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	6.8E+01	1.80E+00	5.70E+00	10	325	3.31E+03	102%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T04-B	1	5.32E+00	E		5.32E+00	5.6E+01	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T05-B	1	9.61E+00			9.61E+00	4.3E+01	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T06-B	1	1.01E+02			1.01E+02	3.7E-01	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T07-B	1	6.02E+02			6.02E+02	6.1E-01	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T08-B	1	5.50E+02			5.50E+02	6.4E-01	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T09-B	1	7.16E+02			7.16E+02	6.7E-01	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T01-C		3.73E+00	E		3.73E+00	7.9E+01	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T02-C		9.00E-01	U1/2		9.00E-01	4.3E+01	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T03-C		9.00E-01	U1/2		9.00E-01	7.3E+01	1.80E+00	5.70E+00	10	325	3.34E+03	103%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T04-C		2.79E+00	E		2.79E+00	1.1E+02	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T05-C		1.64E+01			1.64E+01	2.8E+01	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T06-C		7.75E+01			7.75E+01	4.6E+00	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T07-C		6.04E+02			6.04E+02	1.1E+00	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T08-C		5.43E+02			5.43E+02	1.0E+00	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-T09-C		7.09E+02			7.09E+02	6.8E-01	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-B01-A		2.90E+00	E		2.90E+00	2.7E+01	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-B02-A		2.41E+00	E		2.41E+00	5.5E+01	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
Ni	EaFa-L09-1313-B03-A		2.36E+00	E		2.36E+00	1.7E+02	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	EaFa-L09-1313-T01-A	1	1.44E+02			1.44E+02	1.2E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T02-A	1	4.63E+01			4.63E+01	3.7E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T03-A	1	9.35E+01			9.35E+01	7.7E+01	3.70E+00	1.18E+01	1000	100	1.17E+03	108%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T04-A	1	6.76E+01			6.76E+01	2.9E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T05-A	1	4.00E+01			4.00E+01	1.3E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T06-A	1	1.28E+01			1.28E+01	9.0E+00	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T07-A	1	1.13E+01	E		1.13E+01	8.8E+00	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T08-A	1	3.83E+01			3.83E+01	3.9E+00	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T09-A	1	1.82E+03			1.82E+03	5.5E-01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T01-B	1	1.48E+02			1.48E+02	1.8E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T02-B	1	5.01E+01			5.01E+01	1.5E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T03-B	1	8.15E+01			8.15E+01	4.4E+01	3.70E+00	1.18E+01	1000	100	1.15E+03	107%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T04-B	1	6.79E+01			6.79E+01	3.2E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T05-B	1	5.66E+01			5.66E+01	9.4E+00	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T06-B	1	2.71E+01			2.71E+01	5.6E+00	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T07-B	1	7.40E+00	E		7.40E+00	9.2E+00	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T08-B	1	3.48E+01			3.48E+01	5.0E+00	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T09-B	1	1.89E+03			1.89E+03	4.6E-01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T01-C	1	1.10E+02			1.10E+02	1.7E+02	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T02-C	1	5.68E+01			5.68E+01	1.0E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T03-C	1	8.45E+01			8.45E+01	5.4E+01	3.70E+00	1.18E+01	1000	100	1.16E+03	107%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T04-C	1	6.76E+01			6.76E+01	2.8E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T05-C	1	3.96E+01			3.96E+01	8.2E+00	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T06-C	1	2.24E+01			2.24E+01	1.6E+00	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T07-C	1	3.30E+01			3.30E+01	8.2E+00	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T08-C	1	4.16E+01			4.16E+01	4.7E+00	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-T09-C	1	1.89E+03			1.89E+03	6.0E-01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-B01-A	1	4.65E+00	E		4.65E+00	2.4E+00	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	5.6E+00	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
P	EaFa-L09-1313-B03-A	1	1.20E+01			1.20E+01	1.3E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	EaFa-L09-1313-T01-A	1	1.85E+06			1.85E+06	6.3E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T02-A	1	5.28E+05			5.28E+05	1.2E+00	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T03-A	1	1.94E+05			1.94E+05	3.3E-01	1.60E+00	5.09E+00	1000	100	1.94E+05	89%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T04-A	1	9.81E+04			9.81E+04	8.4E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T05-A	1	5.94E+04			5.94E+04	5.2E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T06-A	1	2.54E+04			2.54E+04	5.8E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T07-A	1	2.48E+04			2.48E+04	1.1E+00	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T08-A	1	1.83E+04			1.83E+04	1.6E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T09-A	1	2.14E+04			2.14E+04	1.6E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T01-B	1	1.88E+06			1.88E+06	1.4E+00	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T02-B	1	5.19E+05			5.19E+05	6.9E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T03-B	1	1.85E+05			1.85E+05	2.2E+00	1.60E+00	5.09E+00	1000	100	1.86E+05	82%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T04-B	1	9.53E+04			9.53E+04	8.0E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T05-B	1	6.13E+04			6.13E+04	6.8E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T06-B	1	2.56E+04			2.56E+04	6.1E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T07-B	1	2.38E+04			2.38E+04	6.8E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T08-B	1	1.81E+04			1.81E+04	1.6E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T09-B	1	2.10E+04			2.10E+04	2.2E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T01-C	1	1.83E+06			1.83E+06	8.4E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T02-C	1	5.03E+05			5.03E+05	2.8E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T03-C	1	1.77E+05			1.77E+05	1.5E+00	1.60E+00	5.09E+00	1000	100	1.78E+05	88%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T04-C	1	9.31E+04			9.31E+04	4.3E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T05-C	1	5.88E+04			5.88E+04	7.5E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T06-C	1	2.46E+04			2.46E+04	1.5E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T07-C	1	2.37E+04			2.37E+04	1.3E+00	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T08-C	1	1.77E+04			1.77E+04	8.7E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-T09-C	1	2.08E+04			2.08E+04	1.1E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-B01-A	1	8.43E+01			8.43E+01	4.0E+00	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-B02-A	1	8.45E+01			8.45E+01	5.5E+00	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
K	EaFa-L09-1313-B03-A	1	1.91E+06			1.91E+06	9.2E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	EaFa-L09-1313-T01-A	1	6.95E+03			6.95E+03	1.3E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T02-A	1	5.79E+03			5.79E+03	1.9E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T03-A	1	5.17E+03			5.17E+03	7.9E-01	1.50E+01	4.77E+01	10	325	8.04E+03	88%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T04-A	1	3.14E+03			3.14E+03	2.5E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T05-A	1	1.61E+03			1.61E+03	1.8E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T06-A	1	9.55E+02			9.55E+02	1.0E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T07-A	1	2.65E+02			2.65E+02	1.7E+01	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T08-A	1	1.20E+02			1.20E+02	1.0E+01	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T09-A	1	5.37E+02			5.37E+02	1.4E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T01-B	1	7.37E+03			7.37E+03	1.5E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T02-B	1	6.16E+03			6.16E+03	6.6E-01	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T03-B	1	5.04E+03			5.04E+03	2.6E+00	1.50E+01	4.77E+01	10	325	7.96E+03	90%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T04-B	1	2.89E+03			2.89E+03	1.1E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T05-B	1	1.86E+03			1.86E+03	1.3E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T06-B	1	1.02E+03			1.02E+03	2.2E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T07-B	1	2.94E+02			2.94E+02	3.2E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T08-B	1	1.32E+02			1.32E+02	1.4E+01	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T09-B	1	5.71E+02			5.71E+02	3.9E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T01-C	1	7.43E+03			7.43E+03	1.0E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T02-C	1	5.99E+03			5.99E+03	7.3E-01	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T03-C	1	4.86E+03			4.86E+03	1.0E+00	1.50E+01	4.77E+01	10	325	7.97E+03	96%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T04-C	1	2.87E+03			2.87E+03	2.1E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T05-C	1	1.77E+03			1.77E+03	9.8E-01	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T06-C	1	9.57E+02			9.57E+02	1.4E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T07-C	1	2.75E+02			2.75E+02	6.9E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T08-C	1	1.12E+02			1.12E+02	1.4E+01	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-T09-C	1	5.53E+02			5.53E+02	2.9E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-B01-A	1	7.90E+01			7.90E+01	1.6E+01	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-B02-A	1	8.96E+01			8.96E+01	6.1E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
Se	EaFa-L09-1313-B03-A	1	6.41E+01			6.41E+01	2.9E+01	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	EaFa-L09-1313-T01-A	1	1.08E+04			1.08E+04	1.3E+00	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T02-A	1	3.30E+03			3.30E+03	9.6E-01	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T03-A	1	5.10E+02			5.10E+02	7.0E-01	1.10E+00	3.50E+00	1000	100	1.56E+03	105%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T04-A	1	3.91E+02			3.91E+02	1.4E+00	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T05-A	1	8.21E+02			8.21E+02	1.4E+00	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T06-A	1	2.26E+03			2.26E+03	1.2E+00	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T07-A	1	7.59E+03			7.59E+03	3.6E-01	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T08-A	1	3.88E+04			3.88E+04	6.1E-01	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T09-A	1	6.73E+04			6.73E+04	4.6E-01	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T01-B	1	1.11E+04			1.11E+04	2.3E+00	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T02-B	1	3.45E+03			3.45E+03	8.8E-01	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T03-B	1	5.85E+02			5.85E+02	2.4E+00	1.10E+00	3.50E+00	1000	100	1.60E+03	101%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T04-B	1	3.67E+02			3.67E+02	1.2E+00	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T05-B	1	6.04E+02			6.04E+02	1.5E-01	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T06-B	1	1.87E+03			1.87E+03	7.1E-02	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T07-B	1	8.43E+03			8.43E+03	5.3E-01	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T08-B	1	4.00E+04			4.00E+04	3.6E-01	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T09-B	1	6.81E+04			6.81E+04	1.0E+00	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T01-C	1	1.11E+04			1.11E+04	5.3E-01	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T02-C	1	3.32E+03			3.32E+03	5.1E-01	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T03-C	1	5.52E+02			5.52E+02	7.4E-01	1.10E+00	3.50E+00	1000	100	1.60E+03	105%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T04-C	1	3.36E+02			3.36E+02	5.5E-01	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T05-C	1	6.44E+02			6.44E+02	1.2E+00	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T06-C	1	1.58E+03			1.58E+03	6.5E-01	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T07-C	1	8.43E+03			8.43E+03	1.1E+00	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T08-C	1	3.96E+04			3.96E+04	6.1E-02	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-T09-C	1	6.76E+04			6.76E+04	7.5E-01	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-B01-A	1	4.48E+00			4.48E+00	3.5E+01	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-B02-A	1	4.51E+00			4.51E+00	3.3E+01	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
Si	EaFa-L09-1313-B03-A	1	1.20E+01			1.20E+01	2.2E+01	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	EaFa-L09-1313-T01-A	1	5.66E+03			5.66E+03	9.8E-01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T02-A	1	5.74E+03			5.74E+03	1.7E+00	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T03-A	1	5.74E+03			5.74E+03	2.3E-01	2.50E+00	8.00E+00	1000	100	6.58E+03	84%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T04-A	1	5.60E+03			5.60E+03	1.3E+00	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T05-A	1	5.58E+03			5.58E+03	7.6E-01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T06-A	1	5.62E+03			5.62E+03	3.4E-01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T07-A	1	5.26E+03			5.26E+03	7.2E-01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T08-A	1	3.52E+03			3.52E+03	5.7E-01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T09-A	1	3.26E+03			3.26E+03	1.9E-01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T01-B	1	6.05E+03			6.05E+03	1.4E+00	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T02-B	1	5.99E+03			5.99E+03	1.9E-01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T03-B	1	5.73E+03			5.73E+03	1.8E+00	2.50E+00	8.00E+00	1000	100	6.60E+03	87%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T04-B	1	5.45E+03			5.45E+03	5.7E-01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T05-B	1	5.50E+03			5.50E+03	1.4E+00	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T06-B	1	5.59E+03			5.59E+03	1.1E+00	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T07-B	1	5.15E+03			5.15E+03	2.5E-01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T08-B	1	3.50E+03			3.50E+03	4.1E-01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T09-B	1	3.28E+03			3.28E+03	1.9E-01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T01-C	1	6.05E+03			6.05E+03	5.2E-01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T02-C	1	5.68E+03			5.68E+03	5.1E-01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T03-C	1	5.38E+03			5.38E+03	9.0E-01	2.50E+00	8.00E+00	1000	100	6.27E+03	90%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T04-C	1	5.30E+03			5.30E+03	4.8E-01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T05-C	1	5.21E+03			5.21E+03	3.5E-01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T06-C	1	5.35E+03			5.35E+03	4.7E-01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T07-C	1	5.10E+03			5.10E+03	1.1E+00	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T08-C	1	3.44E+03			3.44E+03	2.5E-01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-T09-C	1	3.21E+03			3.21E+03	4.6E-01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-B01-A	1	2.11E+01			2.11E+01	1.8E+00	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-B02-A	1	2.02E+01			2.02E+01	3.0E+00	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
Na	EaFa-L09-1313-B03-A	1	4.02E+02			4.02E+02	1.4E+00	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	EaFa-L09-1313-T01-A	1	1.45E+03			1.45E+03	1.6E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T02-A	1	1.79E+03			1.79E+03	1.0E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T03-A	1	1.95E+03			1.95E+03	6.7E-01	1.00E+00	3.18E+00	1000	100	2.83E+03	88%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T04-A	1	2.04E+03			2.04E+03	1.3E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T05-A	1	2.15E+03			2.15E+03	1.2E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T06-A	1	2.28E+03			2.28E+03	7.7E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T07-A	1	2.70E+03			2.70E+03	7.4E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T08-A	1	3.99E+03			3.99E+03	2.7E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T09-A	1	5.29E+03			5.29E+03	1.6E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T01-B	1	1.52E+03			1.52E+03	2.2E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T02-B	1	1.74E+03			1.74E+03	5.4E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T03-B	1	1.89E+03			1.89E+03	2.1E+00	1.00E+00	3.18E+00	1000	100	2.77E+03	88%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T04-B	1	2.06E+03			2.06E+03	1.1E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T05-B	1	2.20E+03			2.20E+03	1.0E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T06-B	1	2.33E+03			2.33E+03	1.2E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T07-B	1	2.62E+03			2.62E+03	6.1E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T08-B	1	3.99E+03			3.99E+03	6.7E-02	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T09-B	1	5.23E+03			5.23E+03	6.1E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T01-C	1	1.49E+03			1.49E+03	1.3E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T02-C	1	1.69E+03			1.69E+03	1.2E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T03-C	1	1.80E+03			1.80E+03	1.2E+00	1.00E+00	3.18E+00	1000	100	2.75E+03	94%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T04-C	1	2.03E+03			2.03E+03	7.8E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T05-C	1	2.12E+03			2.12E+03	9.4E-02	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T06-C	1	2.32E+03			2.32E+03	3.7E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T07-C	1	2.61E+03			2.61E+03	4.0E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T08-C	1	3.90E+03			3.90E+03	1.2E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-T09-C	1	5.17E+03			5.17E+03	1.1E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	2.1E+02	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.7E+02	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
Sr	EaFa-L09-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	1.3E+02	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	EaFa-L09-1313-T01-A	1	1.69E+05			1.69E+05	9.4E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T02-A	1	1.63E+05			1.63E+05	1.1E+00	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T03-A	1	1.61E+05			1.61E+05	1.4E-01	6.80E+00	2.16E+01	1000	100	1.62E+05	83%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T04-A	1	1.58E+05			1.58E+05	9.3E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T05-A	1	1.58E+05			1.58E+05	8.1E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T06-A	1	1.57E+05			1.57E+05	5.4E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T07-A	1	1.32E+05			1.32E+05	5.8E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T08-A	1	8.42E+04			8.42E+04	4.1E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T09-A	1	6.17E+04			6.17E+04	4.5E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T01-B	1	1.83E+05			1.83E+05	1.8E+00	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T02-B	1	1.67E+05			1.67E+05	2.4E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T03-B	1	1.60E+05			1.60E+05	2.6E+00	6.80E+00	2.16E+01	1000	100	1.61E+05	87%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T04-B	1	1.60E+05			1.60E+05	4.5E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T05-B	1	1.59E+05			1.59E+05	4.5E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T06-B	1	1.59E+05			1.59E+05	4.1E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T07-B	1	1.32E+05			1.32E+05	4.4E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T08-B	1	8.59E+04			8.59E+04	3.9E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T09-B	1	6.32E+04			6.32E+04	6.6E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T01-C	1	1.81E+05			1.81E+05	6.7E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T02-C	1	1.64E+05			1.64E+05	5.2E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T03-C	1	1.53E+05			1.53E+05	7.1E-01	6.80E+00	2.16E+01	1000	100	1.54E+05	81%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T04-C	1	1.58E+05			1.58E+05	1.1E+00	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T05-C	1	1.53E+05			1.53E+05	3.5E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T06-C	1	1.58E+05			1.58E+05	7.9E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T07-C	1	1.34E+05			1.34E+05	8.4E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T08-C	1	8.61E+04			8.61E+04	1.2E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-T09-C	1	6.27E+04			6.27E+04	3.0E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	2.3E+02	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	1.3E+02	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
S	EaFa-L09-1313-B03-A	1	6.99E+00	E		6.99E+00	8.4E+01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	EaFa-L09-1313-T01-A	1	2.30E+00	U1/2		2.30E+00	6.9E+01	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T02-A	1	2.30E+00	U1/2		2.30E+00	2.8E+02	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T03-A	1	2.30E+00	U1/2		2.30E+00	1.9E+02	4.60E+00	1.46E+01	10	325	3.30E+03	101%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T04-A	1	7.44E+00	E		7.44E+00	8.5E+01	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T05-A	1	2.30E+00	U1/2		2.30E+00	1.2E+02	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T06-A	1	1.28E+01	E		1.28E+01	2.7E+01	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T07-A	1	2.94E+01			2.94E+01	1.1E+01	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T08-A	1	5.77E+01			5.77E+01	8.7E+00	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T09-A	1	9.11E+01			9.11E+01	4.2E+00	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T01-B	1	6.40E+00	E		6.40E+00	1.4E+02	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T02-B	1	2.30E+00	U1/2		2.30E+00	4.6E+02	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T03-B	1	2.30E+00	U1/2		2.30E+00	8.4E+01	4.60E+00	1.46E+01	10	325	3.18E+03	98%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T04-B	1	2.30E+00	U1/2		2.30E+00	2.8E+01	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T05-B	1	2.30E+00	U1/2		2.30E+00	6.6E+01	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T06-B	1	2.30E+00	U1/2		2.30E+00	4.6E+02	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T07-B	1	3.93E+01			3.93E+01	1.7E+01	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T08-B	1	5.47E+01			5.47E+01	3.5E+00	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T09-B	1	8.35E+01			8.35E+01	6.0E+00	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T01-C	1	6.08E+00	E		6.08E+00	9.1E+01	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T02-C	1	2.30E+00	U1/2		2.30E+00	7.6E+02	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T03-C	1	2.30E+00	U1/2		2.30E+00	1.7E+02	4.60E+00	1.46E+01	10	325	3.22E+03	99%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T04-C	1	2.30E+00	U1/2		2.30E+00	6.3E+01	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T05-C	1	2.30E+00	U1/2		2.30E+00	1.0E+03	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T06-C	1	2.30E+00	U1/2		2.30E+00	2.8E+02	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T07-C	1	4.09E+01			4.09E+01	2.1E+01	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T08-C	1	5.17E+01			5.17E+01	1.0E+01	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-T09-C	1	8.34E+01			8.34E+01	7.4E+00	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	9.0E+01	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	9.3E+01	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
Tl	EaFa-L09-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	2.0E+02	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	EaFa-L09-1313-T01-A	1	2.67E+00	E		2.67E+00	4.7E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	8.2E+01	2.00E+00	6.40E+00	10	325	3.46E+03	106%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	5.6E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	4.8E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T08-A	1	3.06E+01			3.06E+01	8.6E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T09-A	1	2.07E+03			2.07E+03	4.9E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T01-B	1	3.01E+00	E		3.01E+00	8.7E+00	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	4.6E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	4.5E+01	2.00E+00	6.40E+00	10	325	3.31E+03	102%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	3.6E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	7.1E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	5.5E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	5.5E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T08-B	1	3.35E+01			3.35E+01	1.6E+00	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T09-B	1	2.10E+03			2.10E+03	5.7E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T01-C	1	2.30E+00	E		2.30E+00	1.3E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	9.2E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.00E+00	6.40E+00	10	325	3.30E+03	102%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	8.8E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	5.2E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T08-C	1	3.26E+01			3.26E+01	2.1E+00	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-T09-C	1	2.06E+03			2.06E+03	7.7E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	4.4E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
Ti	EaFa-L09-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	4.3E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	EaFa-L09-1313-T01-A	1	4.87E+03			4.87E+03	1.4E+00	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T02-A	1	2.55E+03			2.55E+03	6.2E-01	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T03-A	1	1.95E+03			1.95E+03	7.7E-01	1.50E+00	4.77E+00	10	325	5.32E+03	104%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T04-A	1	4.99E+02			4.99E+02	7.7E-01	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T05-A	1	2.31E+02			2.31E+02	2.3E+00	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T06-A	1	1.86E+02			1.86E+02	4.2E-01	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T07-A	1	8.24E+01			8.24E+01	1.6E+00	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T08-A	1	1.34E+02			1.34E+02	1.2E+00	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T09-A	1	6.31E+03			6.31E+03	8.1E-01	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T01-B	1	5.04E+03			5.04E+03	1.1E+00	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T02-B	1	2.73E+03			2.73E+03	4.9E-01	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T03-B	1	2.03E+03			2.03E+03	1.9E+00	1.50E+00	4.77E+00	10	325	5.32E+03	101%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T04-B	1	4.28E+02			4.28E+02	1.4E+00	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T05-B	1	2.70E+02			2.70E+02	1.1E+00	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T06-B	1	1.94E+02			1.94E+02	1.0E+00	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T07-B	1	9.04E+01			9.04E+01	8.8E-01	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T08-B	1	1.50E+02			1.50E+02	7.6E-02	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T09-B	1	6.34E+03			6.34E+03	4.7E-01	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T01-C	1	4.88E+03			4.88E+03	1.3E+00	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T02-C	1	2.61E+03			2.61E+03	1.3E+00	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T03-C	1	1.93E+03			1.93E+03	8.1E-01	1.50E+00	4.77E+00	10	325	5.31E+03	104%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T04-C	1	4.19E+02			4.19E+02	1.6E+00	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T05-C	1	2.50E+02			2.50E+02	1.2E+00	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T06-C	1	1.80E+02			1.80E+02	2.6E-01	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T07-C	1	8.95E+01			8.95E+01	1.5E+00	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T08-C	1	1.48E+02			1.48E+02	1.0E+00	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-T09-C	1	6.25E+03			6.25E+03	1.0E-01	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-B01-A	1	2.51E+00	E		2.51E+00	5.3E+01	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-B02-A	1	7.50E-01	U1/2		7.50E-01	2.8E+01	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
V	EaFa-L09-1313-B03-A	1	4.56E+00	E		4.56E+00	5.0E+01	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	EaFa-L09-1313-T01-A	1	1.02E+02			1.02E+02	1.6E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:50 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T02-A	1	1.18E+01			1.18E+01	4.1E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:51 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T03-A	1	8.45E+00			8.45E+00	9.4E+00	1.00E+00	3.18E+00	10	325	3.63E+03	111%	VU ICP-OES	6/11/10 10:53 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T04-A	1	6.64E+00			6.64E+00	4.7E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:55 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T05-A	1	1.27E+01			1.27E+01	8.4E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:57 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T06-A	1	2.15E+01			2.15E+01	1.4E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:58 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T07-A	1	1.36E+03			1.36E+03	9.2E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:00 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T08-A	1	1.25E+03			1.25E+03	1.2E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:01 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T09-A	1	1.59E+03			1.59E+03	1.3E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:03 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T01-B	1	1.01E+02			1.01E+02	2.3E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:15 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T02-B	1	1.95E+01			1.95E+01	4.9E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:16 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T03-B	1	8.46E+00			8.46E+00	6.3E+00	1.00E+00	3.18E+00	10	325	3.52E+03	108%	VU ICP-OES	6/11/10 11:18 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T04-B	1	7.00E+00			7.00E+00	2.1E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:20 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T05-B	1	2.02E+01			2.02E+01	1.6E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:21 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T06-B	1	1.94E+01			1.94E+01	5.1E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:23 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T07-B	1	1.33E+03			1.33E+03	6.1E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:24 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T08-B	1	1.26E+03			1.26E+03	1.1E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:26 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T09-B	1	1.57E+03			1.57E+03	7.5E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:28 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T01-C	1	1.09E+02			1.09E+02	1.1E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:34 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T02-C	1	1.52E+01			1.52E+01	1.3E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:36 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T03-C	1	6.16E+00			6.16E+00	2.9E+00	1.00E+00	3.18E+00	10	325	3.55E+03	109%	VU ICP-OES	6/11/10 11:38 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T04-C	1	3.46E+00			3.46E+00	1.2E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:39 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T05-C	1	1.87E+01			1.87E+01	5.6E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:41 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T06-C	1	2.52E+01			2.52E+01	8.8E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:43 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T07-C	1	1.32E+03			1.32E+03	4.4E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:44 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T08-C	1	1.24E+03			1.24E+03	8.1E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:46 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-T09-C	1	1.56E+03			1.56E+03	3.8E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:48 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-B01-A	1	7.48E+00			7.48E+00	1.1E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:45 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-B02-A	1	1.04E+01			1.04E+01	2.9E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:46 AM	L09 1313-1316 EaFA
Zn	EaFa-L09-1313-B03-A	1	1.34E+01			1.34E+01	8.2E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 10:48 AM	L09 1313-1316 EaFA

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	EaFA-L10-1313-T01-A	1	1.09E+05			1.09E+05	3.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T02-A	1	3.27E+04			3.27E+04	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T03-A	1	2.45E+04			2.45E+04	9.8E-01	1.0E+00	3.2E+00	1000	100	2.54E+04	95%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T04-A	1	1.11E+04			1.11E+04	3.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T05-A	1	1.22E+02			1.22E+02	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T06-A	1	4.93E+02			4.93E+02	6.6E-02	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T07-A	1	2.71E+02			2.71E+02	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T08-A	1	7.33E+04			7.33E+04	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T09-A	1	1.06E+05			1.06E+05	3.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T01-B	1	1.11E+05			1.11E+05	1.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T02-B	1	3.60E+04			3.60E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T03-B	1	2.27E+04			2.27E+04	8.9E-01	1.0E+00	3.2E+00	1000	100	2.36E+04	89%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T04-B	1	1.15E+04			1.15E+04	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T05-B	1	1.56E+02			1.56E+02	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T06-B	1	1.30E+02			1.30E+02	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T07-B	1	5.65E+02			5.65E+02	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T08-B	1	6.58E+04			6.58E+04	2.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T09-B	1	1.07E+05			1.07E+05	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T01-C	1	1.20E+05			1.20E+05	3.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T02-C	1	3.59E+04			3.59E+04	2.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T03-C	1	2.46E+04			2.46E+04	3.5E-01	1.0E+00	3.2E+00	1000	100	2.55E+04	88%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T04-C	1	1.06E+04			1.06E+04	2.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T05-C	1	1.44E+02			1.44E+02	3.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T06-C	1	1.09E+02			1.09E+02	5.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T07-C	1	6.87E+02			6.87E+02	6.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T08-C	1	7.58E+04			7.58E+04	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-T09-C	1	1.11E+05			1.11E+05	2.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-B01-A	1	8.48E+00			8.48E+00	3.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-B02-A	1	1.06E+01			1.06E+01	1.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-B03-A	1	2.78E+01			2.78E+01	9.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	6.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	6.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1313-B03-C	1	3.69E+01			3.69E+01	5.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	EaFA-L10-1313-T01-A	1	5.84E+02			5.84E+02	2.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T02-A	1	1.62E+02			1.62E+02	1.6E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T03-A	1	1.55E+02			1.55E+02	1.0E+01	7.5E+00	2.4E+01	10	300	2.93E+03	92%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T04-A	1	1.87E+02			1.87E+02	1.6E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T05-A	1	1.45E+02			1.45E+02	2.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T06-A	1	9.45E+01			9.45E+01	1.5E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T07-A	1	1.24E+02			1.24E+02	7.9E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T08-A	1	7.73E+00	E		7.73E+00	2.1E+02	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T09-A	1	3.75E+00	U1/2		3.75E+00	8.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T01-B	1	5.51E+02			5.51E+02	7.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T02-B	1	1.70E+02			1.70E+02	9.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T03-B	1	1.88E+02			1.88E+02	8.8E+00	7.5E+00	2.4E+01	10	300	3.07E+03	96%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T04-B	1	1.82E+02			1.82E+02	1.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T05-B	1	1.31E+02			1.31E+02	7.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T06-B	1	1.22E+02			1.22E+02	6.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T07-B	1	1.33E+02			1.33E+02	2.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T08-B	1	2.26E+01	E		2.26E+01	4.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T09-B	1	8.95E+00	E		8.95E+00	1.4E+02	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T01-C	1	6.08E+02			6.08E+02	5.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T02-C	1	2.21E+02			2.21E+02	1.4E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T03-C	1	1.85E+02			1.85E+02	1.6E+01	7.5E+00	2.4E+01	10	300	3.25E+03	102%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T04-C	1	1.90E+02			1.90E+02	9.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T05-C	1	2.51E+02			2.51E+02	6.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T06-C	1	1.30E+02			1.30E+02	2.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T07-C	1	1.17E+02			1.17E+02	1.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T08-C	1	3.75E+00	U1/2		3.75E+00	2.6E+02	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-T09-C	1	7.50E+00	E		7.50E+00	6.4E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-B01-A	1	3.75E+00	U1/2		3.75E+00	9.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-B02-A	1	3.75E+00	U1/2		3.75E+00	8.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-B03-A	1	1.12E+01	E		1.12E+01	1.1E+02	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-B01-C	1	1.74E+01	E		1.74E+01	6.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-B02-C	1	3.75E+00	U1/2		3.75E+00	1.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1313-B03-C	1	1.42E+01	E		1.42E+01	4.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	EaFA-L10-1313-T01-A	1	1.83E+04			1.83E+04	8.2E-01	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T02-A	1	2.67E+03			2.67E+03	1.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T03-A	1	1.58E+03			1.58E+03	9.0E-01	1.1E+01	3.5E+01	10	300	4.28E+03	90%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T04-A	1	8.80E+02			8.80E+02	3.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T05-A	1	8.87E+01			8.87E+01	3.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T06-A	1	1.29E+02			1.29E+02	1.1E+01	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T07-A	1	1.11E+02			1.11E+02	2.9E+01	1.1E+01	3.5E+01				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T08-A	1	1.12E+02			1.12E+02	7.7E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T09-A	1	1.09E+03			1.09E+03	7.7E-01	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T01-B	1	1.86E+04			1.86E+04	9.7E-01	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T02-B	1	3.30E+03			3.30E+03	1.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T03-B	1	1.59E+03			1.59E+03	2.1E+00	1.1E+01	3.5E+01	10	300	4.53E+03	98%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T04-B	1	8.63E+02			8.63E+02	1.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T05-B	1	1.03E+02			1.03E+02	2.6E+01	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T06-B	1	8.62E+01			8.62E+01	6.7E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T07-B	1	1.26E+02			1.26E+02	2.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T08-B	1	1.25E+02			1.25E+02	7.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T09-B	1	1.03E+03			1.03E+03	1.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T01-C	1	1.99E+04			1.99E+04	3.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T02-C	1	3.23E+03			3.23E+03	4.8E-01	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T03-C	1	1.85E+03			1.85E+03	1.1E-01	1.1E+01	3.5E+01	10	300	4.85E+03	100%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T04-C	1	8.54E+02			8.54E+02	2.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T05-C	1	9.98E+01			9.98E+01	2.7E+01	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T06-C	1	8.06E+01			8.06E+01	6.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T07-C	1	1.40E+02			1.40E+02	1.5E+01	1.1E+01	3.5E+01				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T08-C	1	1.16E+02			1.16E+02	7.2E-01	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-T09-C	1	1.06E+03			1.06E+03	7.2E-01	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-B01-A	1	3.44E+01	E		3.44E+01	6.8E+01	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-B02-A	1	3.90E+01			3.90E+01	2.7E+01	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-B03-A	1	3.08E+01	E		3.08E+01	9.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-B01-C	1	3.94E+01			3.94E+01	8.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-B02-C	1	3.53E+01			3.53E+01	5.4E+01	1.1E+01	3.5E+01				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1313-B03-C	1	3.71E+01			3.71E+01	3.8E+01	1.1E+01	3.5E+01				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	EaFA-L10-1313-T01-A	1	4.96E+03			4.96E+03	2.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T02-A	1	3.06E+03			3.06E+03	1.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T03-A	1	3.50E+03			3.50E+03	1.0E+00	1.0E+00	3.2E+00	1000	100	4.37E+03	87%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T04-A	1	4.24E+03			4.24E+03	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T05-A	1	3.95E+03			3.95E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T06-A	1	4.15E+03			4.15E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T07-A	1	4.95E+03			4.95E+03	7.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T08-A	1	2.97E+03			2.97E+03	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T09-A	1	2.71E+03			2.71E+03	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T01-B	1	5.08E+03			5.08E+03	6.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T02-B	1	3.28E+03			3.28E+03	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T03-B	1	3.58E+03			3.58E+03	9.8E-01	1.0E+00	3.2E+00	1000	100	4.46E+03	88%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T04-B	1	4.21E+03			4.21E+03	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T05-B	1	4.09E+03			4.09E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T06-B	1	4.81E+03			4.81E+03	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T07-B	1	4.83E+03			4.83E+03	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T08-B	1	3.12E+03			3.12E+03	3.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T09-B	1	2.69E+03			2.69E+03	1.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T01-C	1	5.42E+03			5.42E+03	3.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T02-C	1	3.47E+03			3.47E+03	1.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T03-C	1	3.70E+03			3.70E+03	4.1E-01	1.0E+00	3.2E+00	1000	100	4.61E+03	92%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T04-C	1	4.10E+03			4.10E+03	2.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T05-C	1	8.30E+03			8.30E+03	3.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T06-C	1	4.64E+03			4.64E+03	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T07-C	1	4.85E+03			4.85E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T08-C	1	3.14E+03			3.14E+03	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-T09-C	1	2.80E+03			2.80E+03	8.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-B01-A	1	1.28E+02			1.28E+02	2.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-B02-A	1	1.19E+02			1.19E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-B03-A	1	1.54E+02			1.54E+02	3.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-B01-C	1	1.17E+02			1.17E+02	3.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-B02-C	1	9.93E+01			9.93E+01	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1313-B03-C	1	2.00E+02			2.00E+02	3.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	EaFA-L10-1313-T01-A	1	6.70E+03			6.70E+03	5.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T02-A	1	1.52E+03			1.52E+03	1.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T03-A	1	9.19E+02			9.19E+02	5.9E-01	1.0E+00	3.2E+00	10	300	3.35E+03	81%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T04-A	1	5.35E+02			5.35E+02	1.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T05-A	1	2.59E+02			2.59E+02	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T06-A	1	2.91E+02			2.91E+02	4.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T07-A	1	3.05E+02			3.05E+02	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T08-A	1	3.85E+02			3.85E+02	4.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T09-A	1	8.24E+02			8.24E+02	5.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T01-B	1	6.73E+03			6.73E+03	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T02-B	1	1.61E+03			1.61E+03	8.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T03-B	1	1.05E+03			1.05E+03	8.5E-01	1.0E+00	3.2E+00	10	300	3.65E+03	87%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T04-B	1	6.54E+02			6.54E+02	5.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T05-B	1	2.58E+02			2.58E+02	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T06-B	1	3.17E+02			3.17E+02	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T07-B	1	3.39E+02			3.39E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T08-B	1	3.28E+02			3.28E+02	1.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T09-B	1	7.75E+02			7.75E+02	3.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T01-C	1	7.18E+03			7.18E+03	3.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T02-C	1	1.72E+03			1.72E+03	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T03-C	1	1.14E+03			1.14E+03	5.6E-01	1.0E+00	3.2E+00	10	300	3.86E+03	91%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T04-C	1	5.91E+02			5.91E+02	3.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T05-C	1	2.47E+02			2.47E+02	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T06-C	1	3.29E+02			3.29E+02	6.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T07-C	1	3.71E+02			3.71E+02	2.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T08-C	1	3.60E+02			3.60E+02	2.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-T09-C	1	7.73E+02			7.73E+02	7.9E-02	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	2.3E+02	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-B03-A	1	1.47E+02			1.47E+02	9.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	3.9E+02	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	2.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1313-B03-C	1	1.67E+02			1.67E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	EaFA-L10-1313-T01-A	1	1.06E+02			1.06E+02	6.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	1.9E+02	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	3.6E+01	1.9E+00	6.0E+00	10	300	2.81E+03	94%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	2.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T06-A	1	5.22E+00	E		5.22E+00	2.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T07-A	1	4.05E+00	E		4.05E+00	9.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T08-A	1	1.91E+02			1.91E+02	7.0E-02	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T09-A	1	2.31E+02			2.31E+02	7.4E-02	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T01-B	1	1.09E+02			1.09E+02	4.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	5.7E+02	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00	10	300	3.00E+03	100%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	3.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	4.1E+03	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	3.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T07-B	1	6.60E+00			6.60E+00	2.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T08-B	1	1.86E+02			1.86E+02	2.6E-02	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T09-B	1	2.32E+02			2.32E+02	8.2E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T01-C	1	1.15E+02			1.15E+02	2.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	4.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	2.2E+01	1.9E+00	6.0E+00	10	300	3.17E+03	105%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	8.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	8.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	2.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T07-C	1	7.83E+00			7.83E+00	2.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T08-C	1	2.00E+02			2.00E+02	1.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-T09-C	1	2.43E+02			2.43E+02	1.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	1.6E+02	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	8.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	1.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-B01-C	1	9.50E-01	U1/2		9.50E-01	3.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-B02-C	1	9.50E-01	U1/2		9.50E-01	6.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1313-B03-C	1	9.50E-01	U1/2		9.50E-01	7.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	EaFA-L10-1313-T01-A	1	1.10E+00	U1/2		1.10E+00	4.6E+01	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T02-A	1	1.10E+00	U1/2		1.10E+00	7.9E+01	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	2.2E+01	2.2E+00	7.0E+00	10	300	2.82E+03	94%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T04-A	1	1.10E+00	U1/2		1.10E+00	1.1E+02	2.2E+00	7.0E+00				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T05-A	1	1.10E+00	U1/2		1.10E+00	1.5E+02	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T06-A	1	3.14E+01			3.14E+01	1.2E+00	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T07-A	1	2.96E+01			2.96E+01	2.8E+00	2.2E+00	7.0E+00				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T08-A	1	2.57E+01			2.57E+01	1.1E+00	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T09-A	1	3.04E+01			3.04E+01	8.9E-01	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T01-B	1	1.10E+00	U1/2		1.10E+00	2.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T02-B	1	1.10E+00	U1/2		1.10E+00	9.0E+01	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	6.1E+01	2.2E+00	7.0E+00	10	300	2.99E+03	100%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T04-B	1	1.10E+00	U1/2		1.10E+00	9.3E+01	2.2E+00	7.0E+00				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T05-B	1	1.10E+00	U1/2		1.10E+00	2.8E+02	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T06-B	1	2.88E+00	E		2.88E+00	3.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T07-B	1	3.58E+01			3.58E+01	1.1E+00	2.2E+00	7.0E+00				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T08-B	1	2.69E+01			2.69E+01	5.6E-01	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T09-B	1	3.09E+01			3.09E+01	6.7E-01	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T01-C	1	1.10E+00	U1/2		1.10E+00	4.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T02-C	1	1.10E+00	U1/2		1.10E+00	5.9E+01	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	3.8E+01	2.2E+00	7.0E+00	10	300	3.18E+03	106%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T04-C	1	1.10E+00	U1/2		1.10E+00	1.0E+03	2.2E+00	7.0E+00				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T05-C	1	4.22E+00	E		4.22E+00	2.8E+00	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T06-C	1	2.96E+00	E		2.96E+00	2.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T07-C	1	3.80E+01			3.80E+01	1.6E+00	2.2E+00	7.0E+00				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T08-C	1	2.66E+01			2.66E+01	1.8E+00	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-T09-C	1	3.19E+01			3.19E+01	1.0E+00	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	1.4E+02	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	8.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-B03-A	1	1.10E+00	U1/2		1.10E+00	1.6E+02	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-B01-C	1	1.10E+00	U1/2		1.10E+00	3.0E+01	2.2E+00	7.0E+00				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-B02-C	1	1.10E+00	U1/2		1.10E+00	4.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1313-B03-C	1	1.10E+00	U1/2		1.10E+00	3.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	EaFA-L10-1313-T01-A	1	4.19E+03			4.19E+03	4.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T02-A	1	2.59E+04			2.59E+04	1.4E+01	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T03-A	1	7.38E+04			7.38E+04	5.8E-01	2.6E+00	8.3E+00	1000	100	7.47E+04	89%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T04-A	1	1.16E+05			1.16E+05	5.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T05-A	1	1.39E+05			1.39E+05	2.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T06-A	1	1.52E+05			1.52E+05	3.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T07-A	1	1.72E+05			1.72E+05	8.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T08-A	1	1.26E+05			1.26E+05	2.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T09-A	1	1.22E+05			1.22E+05	1.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T01-B	1	4.24E+03			4.24E+03	6.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T02-B	1	2.57E+04			2.57E+04	8.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T03-B	1	7.84E+04			7.84E+04	7.6E-01	2.6E+00	8.3E+00	1000	100	7.92E+04	82%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T04-B	1	1.12E+05			1.12E+05	4.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T05-B	1	1.42E+05			1.42E+05	1.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T06-B	1	1.66E+05			1.66E+05	6.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T07-B	1	1.69E+05			1.69E+05	9.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T08-B	1	1.29E+05			1.29E+05	4.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T09-B	1	1.20E+05			1.20E+05	3.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T01-C	1	4.50E+03			4.50E+03	4.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T02-C	1	2.85E+04			2.85E+04	8.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T03-C	1	7.24E+04			7.24E+04	2.0E-01	2.6E+00	8.3E+00	1000	100	7.33E+04	84%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T04-C	1	1.11E+05			1.11E+05	4.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T05-C	1	3.02E+05			3.02E+05	5.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T06-C	1	1.58E+05			1.58E+05	6.9E+00	2.6E+00	8.3E+00				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T07-C	1	1.72E+05			1.72E+05	6.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T08-C	1	1.31E+05			1.31E+05	7.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-T09-C	1	1.25E+05			1.25E+05	1.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-B01-A	1	2.34E+01			2.34E+01	8.6E+00	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-B02-A	1	1.49E+01			1.49E+01	4.2E+01	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-B03-A	1	1.67E+01			1.67E+01	2.8E+02	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-B01-C	1	1.30E+00	U1/2		1.30E+00	9.0E+02	2.6E+00	8.3E+00				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-B02-C	1	5.33E+00	E		5.33E+00	2.6E+02	2.6E+00	8.3E+00				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1313-B03-C	1	1.44E+02			1.44E+02	2.2E+01	2.6E+00	8.3E+00				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	EaFA-L10-1313-T01-A	1	6.84E+02			6.84E+02	1.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T02-A	1	3.46E+02			3.46E+02	1.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T03-A	1	3.20E+02			3.20E+02	9.1E-01	1.2E+00	3.8E+00	10	300	3.00E+03	89%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T04-A	1	2.65E+02			2.65E+02	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T05-A	1	1.72E+01			1.72E+01	2.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T06-A	1	6.00E-01	U1/2		6.00E-01	2.2E+02	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T07-A	1	2.24E+00	E		2.24E+00	7.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T08-A	1	1.32E+03			1.32E+03	7.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T09-A	1	1.62E+03			1.62E+03	2.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T01-B	1	7.20E+02			7.20E+02	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T02-B	1	3.85E+02			3.85E+02	6.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T03-B	1	3.16E+02			3.16E+02	1.2E+00	1.2E+00	3.8E+00	10	300	3.15E+03	94%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T04-B	1	2.90E+02			2.90E+02	2.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T05-B	1	2.97E+01			2.97E+01	3.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T06-B	1	9.16E+01			9.16E+01	1.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T07-B	1	1.78E+00	E		1.78E+00	8.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T08-B	1	1.07E+03			1.07E+03	1.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T09-B	1	1.59E+03			1.59E+03	3.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T01-C	1	7.19E+02			7.19E+02	3.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T02-C	1	4.00E+02			4.00E+02	5.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T03-C	1	3.47E+02			3.47E+02	3.9E-01	1.2E+00	3.8E+00	10	300	3.32E+03	99%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T04-C	1	2.82E+02			2.82E+02	2.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T05-C	1	1.95E+01			1.95E+01	1.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T06-C	1	7.49E+01			7.49E+01	5.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T07-C	1	2.89E+00	E		2.89E+00	6.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T08-C	1	1.41E+03			1.41E+03	6.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-T09-C	1	1.66E+03			1.66E+03	5.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	5.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	1.2E+03	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-B03-A	1	6.26E+00			6.26E+00	2.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-B01-C	1	6.00E-01	U1/2		6.00E-01	1.2E+02	1.2E+00	3.8E+00				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-B02-C	1	6.00E-01	U1/2		6.00E-01	7.8E+01	1.2E+00	3.8E+00				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1313-B03-C	1	8.44E+00			8.44E+00	1.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	EaFA-L10-1313-T01-A	1	2.04E+01			2.04E+01	1.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	2.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	6.0E+01	1.8E+00	5.7E+00	10	300	2.73E+03	91%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	1.8E+02	1.8E+00	5.7E+00				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T05-A	1	5.76E+01			5.76E+01	5.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T06-A	1	2.26E+02			2.26E+02	9.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T07-A	1	2.50E+02			2.50E+02	8.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T08-A	1	2.51E+02			2.51E+02	6.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T09-A	1	3.57E+02			3.57E+02	3.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T01-B	1	2.14E+01			2.14E+01	1.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	1.2E+02	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	6.0E+01	1.8E+00	5.7E+00	10	300	2.90E+03	97%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	4.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T05-B	1	4.11E+01			4.11E+01	4.9E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T06-B	1	4.13E+01			4.13E+01	6.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T07-B	1	2.57E+02			2.57E+02	2.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T08-B	1	2.37E+02			2.37E+02	8.3E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T09-B	1	3.56E+02			3.56E+02	5.3E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T01-C	1	2.03E+01			2.03E+01	4.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	3.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	4.6E+01	1.8E+00	5.7E+00	10	300	3.02E+03	101%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	7.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T05-C	1	1.29E+02			1.29E+02	1.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T06-C	1	5.02E+01			5.02E+01	4.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T07-C	1	2.64E+02			2.64E+02	9.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T08-C	1	2.59E+02			2.59E+02	1.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-T09-C	1	3.73E+02			3.73E+02	4.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	1.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	5.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-B01-C	1	9.00E-01	U1/2		9.00E-01	4.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-B02-C	1	9.00E-01	U1/2		9.00E-01	2.6E+02	1.8E+00	5.7E+00				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1313-B03-C	1	9.00E-01	U1/2		9.00E-01	3.7E+02	1.8E+00	5.7E+00				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	EaFA-L10-1313-T01-A	1	2.24E+03			2.24E+03	5.9E-01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T02-A	1	9.64E+00	E		9.64E+00	4.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T03-A	1	1.85E+00	U1/2		1.85E+00	2.1E+02	3.7E+00	1.2E+01	10	300	2.66E+03	88%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T04-A	1	8.42E+00	E		8.42E+00	4.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T05-A	1	9.72E+00	E		9.72E+00	4.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T06-A	1	1.19E+02			1.19E+02	7.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T07-A	1	7.18E+01			7.18E+01	1.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T08-A	1	2.47E+03			2.47E+03	2.2E-01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T09-A	1	2.82E+03			2.82E+03	3.8E-01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T01-B	1	2.30E+03			2.30E+03	2.8E-01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T02-B	1	9.24E+00	E		9.24E+00	6.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T03-B	1	4.13E+00	E		4.13E+00	5.7E+01	3.7E+00	1.2E+01	10	300	2.81E+03	94%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T04-B	1	5.93E+00	E		5.93E+00	3.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T05-B	1	1.19E+01			1.19E+01	5.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T06-B	1	1.27E+01			1.27E+01	2.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T07-B	1	1.39E+02			1.39E+02	3.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T08-B	1	2.40E+03			2.40E+03	2.5E-01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T09-B	1	2.77E+03			2.77E+03	1.8E-01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T01-C	1	2.39E+03			2.39E+03	3.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T02-C	1	1.12E+01	E		1.12E+01	4.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T03-C	1	4.02E+00	E		4.02E+00	6.2E+01	3.7E+00	1.2E+01	10	300	2.96E+03	98%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T04-C	1	7.74E+00	E		7.74E+00	1.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T05-C	1	1.04E+01	E		1.04E+01	8.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T06-C	1	1.24E+01			1.24E+01	4.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T07-C	1	1.59E+02			1.59E+02	8.9E-01	3.7E+00	1.2E+01				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T08-C	1	2.57E+03			2.57E+03	6.1E-01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-T09-C	1	2.90E+03			2.90E+03	6.0E-01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	1.2E+03	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-B02-A	1	9.92E+00	E		9.92E+00	1.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-B03-A	1	2.86E+01			2.86E+01	2.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-B01-C	1	1.85E+00	U1/2		1.85E+00	4.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-B02-C	1	1.18E+01	E		1.18E+01	1.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1313-B03-C	1	1.42E+01			1.42E+01	3.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	EaFA-L10-1313-T01-A	1	8.28E+02			8.28E+02	1.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T02-A	1	1.09E+01			1.09E+01	2.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T03-A	1	3.09E+00	E		3.09E+00	6.5E+00	2.0E+00	6.4E+00	1000	100	8.54E+02	85%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	1.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	2.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T07-A	1	3.91E+00	E		3.91E+00	8.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T08-A	1	6.83E+03			6.83E+03	1.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T09-A	1	2.65E+04			2.65E+04	9.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T01-B	1	8.49E+02			8.49E+02	1.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T02-B	1	1.03E+01			1.03E+01	6.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T03-B	1	2.49E+00	E		2.49E+00	1.3E+01	2.0E+00	6.4E+00	1000	100	9.04E+02	90%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	3.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	2.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T08-B	1	4.50E+03			4.50E+03	1.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T09-B	1	2.76E+04			2.76E+04	2.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T01-C	1	8.74E+02			8.74E+02	3.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T02-C	1	1.05E+01			1.05E+01	4.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T03-C	1	4.42E+00	E		4.42E+00	8.4E+00	2.0E+00	6.4E+00	1000	100	9.51E+02	95%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T04-C	1	5.24E+00	E		5.24E+00	5.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	8.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	3.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T08-C	1	7.25E+03			7.25E+03	8.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-T09-C	1	2.88E+04			2.88E+04	6.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	7.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-B02-A	1	1.30E+01			1.30E+01	1.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-B03-A	1	2.04E+01			2.04E+01	1.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	2.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-B02-C	1	3.41E+00	E		3.41E+00	1.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1313-B03-C	1	1.24E+01			1.24E+01	7.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	EaFA-L10-1313-T01-A	1	5.03E+02			5.03E+02	2.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T02-A	1	3.40E+00	U1/2		3.40E+00	1.4E+02	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T03-A	1	3.40E+00	U1/2		3.40E+00	4.4E+01	6.8E+00	2.2E+01	10	300	2.68E+03	89%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T04-A	1	3.40E+00	U1/2		3.40E+00	3.2E+02	6.8E+00	2.2E+01				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T05-A	1	3.40E+00	U1/2		3.40E+00	2.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T06-A	1	3.40E+00	U1/2		3.40E+00	1.3E+02	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T07-A	1	3.40E+00	U1/2		3.40E+00	3.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T08-A	1	3.40E+00	U1/2		3.40E+00	1.8E+02	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T09-A	1	8.66E+01			8.66E+01	8.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T01-B	1	4.75E+02			4.75E+02	2.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T02-B	1	3.40E+00	U1/2		3.40E+00	2.1E+03	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T03-B	1	3.40E+00	U1/2		3.40E+00	3.7E+01	6.8E+00	2.2E+01	10	300	2.85E+03	95%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T04-B	1	3.40E+00	U1/2		3.40E+00	2.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T05-B	1	3.40E+00	U1/2		3.40E+00	3.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T06-B	1	3.40E+00	U1/2		3.40E+00	4.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T07-B	1	3.40E+00	U1/2		3.40E+00	4.2E+02	6.8E+00	2.2E+01				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T08-B	1	3.40E+00	U1/2		3.40E+00	1.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T09-B	1	6.88E+01			6.88E+01	4.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T01-C	1	4.80E+02			4.80E+02	7.8E+00	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T02-C	1	1.64E+01	E		1.64E+01	5.7E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T03-C	1	3.40E+00	U1/2		3.40E+00	7.2E+01	6.8E+00	2.2E+01	10	300	3.00E+03	100%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T04-C	1	3.40E+00	U1/2		3.40E+00	8.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T05-C	1	3.40E+00	U1/2		3.40E+00	3.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T06-C	1	3.40E+00	U1/2		3.40E+00	3.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T07-C	1	3.40E+00	U1/2		3.40E+00	5.5E+02	6.8E+00	2.2E+01				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T08-C	1	3.40E+00	U1/2		3.40E+00	5.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-T09-C	1	7.11E+01			7.11E+01	1.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	3.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-B02-A	1	2.52E+01			2.52E+01	4.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	3.4E+02	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-B01-C	1	3.40E+00	U1/2		3.40E+00	3.1E+02	6.8E+00	2.2E+01				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-B02-C	1	1.80E+01	E		1.80E+01	1.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1313-B03-C	1	2.17E+01			2.17E+01	5.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	EaFA-L10-1313-T01-A	1	1.41E+03			1.41E+03	6.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T02-A	1	2.23E+03			2.23E+03	1.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T03-A	1	2.79E+03			2.79E+03	7.3E-01	1.9E+00	6.0E+00	10	300	5.29E+03	83%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T04-A	1	3.15E+03			3.15E+03	1.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T05-A	1	3.15E+03			3.15E+03	3.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T06-A	1	3.16E+03			3.16E+03	1.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T07-A	1	3.81E+03			3.81E+03	7.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T08-A	1	1.60E+03			1.60E+03	9.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T09-A	1	1.40E+03			1.40E+03	2.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T01-B	1	1.41E+03			1.41E+03	1.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T02-B	1	2.38E+03			2.38E+03	4.9E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T03-B	1	2.84E+03			2.84E+03	8.3E-01	1.9E+00	6.0E+00	10	300	5.30E+03	82%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T04-B	1	3.04E+03			3.04E+03	8.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T05-B	1	3.18E+03			3.18E+03	1.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T06-B	1	3.77E+03			3.77E+03	4.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T07-B	1	3.82E+03			3.82E+03	6.0E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T08-B	1	1.69E+03			1.69E+03	3.6E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T09-B	1	1.38E+03			1.38E+03	4.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T01-C	1	1.54E+03			1.54E+03	2.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T02-C	1	2.57E+03			2.57E+03	8.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T03-C	1	2.87E+03			2.87E+03	3.1E-01	1.9E+00	6.0E+00	10	300	5.37E+03	83%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T04-C	1	3.08E+03			3.08E+03	6.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T05-C	1	6.72E+03			6.72E+03	3.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T06-C	1	3.58E+03			3.58E+03	7.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T07-C	1	3.87E+03			3.87E+03	9.5E-02	1.9E+00	6.0E+00				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T08-C	1	1.66E+03			1.66E+03	4.8E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-T09-C	1	1.43E+03			1.43E+03	5.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	1.9E+02	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	4.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	8.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-B01-C	1	5.62E+00	E		5.62E+00	9.0E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-B02-C	1	2.58E+00	E		2.58E+00	1.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1313-B03-C	1	9.50E-01	U1/2		9.50E-01	1.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	EaFA-L10-1313-T01-A	1	3.41E+01			3.41E+01	1.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	2.0E+03	2.0E+00	6.4E+00	10	300	2.68E+03	89%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T05-A	1	3.83E+02			3.83E+02	2.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T06-A	1	8.91E+02			8.91E+02	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T07-A	1	9.86E+02			9.86E+02	6.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T08-A	1	1.26E+03			1.26E+03	2.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T09-A	1	1.48E+03			1.48E+03	4.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T01-B	1	3.49E+01			3.49E+01	4.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	3.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	1.8E+02	2.0E+00	6.4E+00	10	300	2.84E+03	95%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	2.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T05-B	1	3.15E+02			3.15E+02	1.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T06-B	1	3.19E+02			3.19E+02	2.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T07-B	1	9.32E+02			9.32E+02	1.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T08-B	1	1.25E+03			1.25E+03	2.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T09-B	1	1.49E+03			1.49E+03	3.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T01-C	1	3.50E+01			3.50E+01	2.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	2.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	7.3E+01	2.0E+00	6.4E+00	10	300	2.98E+03	99%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	7.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T05-C	1	8.15E+02			8.15E+02	4.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T06-C	1	3.50E+02			3.50E+02	3.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T07-C	1	9.52E+02			9.52E+02	8.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T08-C	1	1.32E+03			1.32E+03	4.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-T09-C	1	1.53E+03			1.53E+03	2.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	4.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	8.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-B03-A	1	2.06E+00	E		2.06E+00	5.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	8.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	8.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1313-B03-C	1	3.24E+00	E		3.24E+00	1.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	EaFA-L10-1313-T01-A	1	1.38E+01			1.38E+01	2.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T02-A	1	7.02E+00			7.02E+00	3.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T03-A	1	7.73E+01			7.73E+01	1.7E+01	1.0E+00	3.2E+00	1000	100	9.15E+02	84%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T04-A	1	2.73E+03			2.73E+03	3.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T05-A	1	6.89E+03			6.89E+03	6.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T06-A	1	8.18E+03			8.18E+03	4.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T07-A	1	9.37E+03			9.37E+03	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T08-A	1	9.64E+03			9.64E+03	7.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T09-A	1	1.24E+04			1.24E+04	2.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T01-B	1	1.85E+01			1.85E+01	4.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T02-B	1	4.13E+00			4.13E+00	4.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T03-B	1	1.30E+02			1.30E+02	4.3E+00	1.0E+00	3.2E+00	1000	100	1.00E+03	87%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T04-B	1	2.93E+03			2.93E+03	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T05-B	1	7.25E+03			7.25E+03	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T06-B	1	9.05E+03			9.05E+03	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T07-B	1	9.13E+03			9.13E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T08-B	1	9.18E+03			9.18E+03	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T09-B	1	1.24E+04			1.24E+04	4.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T01-C	1	1.81E+01			1.81E+01	9.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T02-C	1	2.43E+00	E		2.43E+00	1.2E+02	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T03-C	1	5.70E+01			5.70E+01	1.9E+01	1.0E+00	3.2E+00	1000	100	9.72E+02	91%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T04-C	1	2.90E+03			2.90E+03	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T05-C	1	1.49E+04			1.49E+04	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T06-C	1	8.73E+03			8.73E+03	7.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T07-C	1	9.29E+03			9.29E+03	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T08-C	1	9.90E+03			9.90E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-T09-C	1	1.27E+04			1.27E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	9.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-B02-A	1	4.34E+00			4.34E+00	1.8E+02	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-B03-A	1	2.29E+01			2.29E+01	3.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	4.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-B02-C	1	3.81E+00			3.81E+00	9.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1313-B03-C	1	4.70E+00			4.70E+00	2.6E+02	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	EaFA-L10-1313-T01-A	1	3.29E+03			3.29E+03	5.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T02-A	1	3.30E+03			3.30E+03	1.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T03-A	1	3.52E+03			3.52E+03	6.5E-01	1.2E+00	3.8E+00	10	300	6.03E+03	84%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T04-A	1	3.74E+03			3.74E+03	1.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T05-A	1	2.76E+03			2.76E+03	3.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T06-A	1	5.16E+02			5.16E+02	3.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T07-A	1	8.04E+02			8.04E+02	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T08-A	1	6.64E+01			6.64E+01	3.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T09-A	1	2.36E+02			2.36E+02	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T01-B	1	3.36E+03			3.36E+03	5.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T02-B	1	3.48E+03			3.48E+03	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T03-B	1	3.62E+03			3.62E+03	7.5E-01	1.2E+00	3.8E+00	10	300	6.27E+03	88%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T04-B	1	3.69E+03			3.69E+03	4.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T05-B	1	2.90E+03			2.90E+03	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T06-B	1	2.48E+03			2.48E+03	3.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T07-B	1	6.00E+02			6.00E+02	4.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T08-B	1	8.14E+01			8.14E+01	3.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T09-B	1	2.42E+02			2.42E+02	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T01-C	1	3.52E+03			3.52E+03	3.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T02-C	1	3.79E+03			3.79E+03	8.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T03-C	1	3.79E+03			3.79E+03	4.2E-01	1.2E+00	3.8E+00	10	300	6.54E+03	92%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T04-C	1	3.63E+03			3.63E+03	9.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T05-C	1	5.55E+03			5.55E+03	2.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T06-C	1	2.29E+03			2.29E+03	6.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T07-C	1	5.61E+02			5.61E+02	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T08-C	1	6.85E+01			6.85E+01	1.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-T09-C	1	2.52E+02			2.52E+02	1.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-B01-A	1	4.77E+00			4.77E+00	1.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	8.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-B03-A	1	1.58E+02			1.58E+02	2.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-B01-C	1	7.82E+00			7.82E+00	4.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-B02-C	1	6.00E-01	U1/2		6.00E-01	5.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1313-B03-C	1	2.08E+02			2.08E+02	2.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	EaFA-L10-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	2.9E+02	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	2.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	3.1E+01	1.8E+00	5.7E+00	10	300	2.75E+03	91%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	1.9E+03	1.8E+00	5.7E+00				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T05-A	1	1.23E+02			1.23E+02	1.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T06-A	1	5.56E+02			5.56E+02	3.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T07-A	1	5.96E+02			5.96E+02	5.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T08-A	1	5.20E+02			5.20E+02	8.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T09-A	1	6.55E+02			6.55E+02	2.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	2.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	2.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	3.8E+01	1.8E+00	5.7E+00	10	300	2.91E+03	97%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T04-B	1	3.88E+00	E		3.88E+00	3.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T05-B	1	8.85E+01			8.85E+01	7.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T06-B	1	1.18E+02			1.18E+02	3.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T07-B	1	6.33E+02			6.33E+02	4.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T08-B	1	5.25E+02			5.25E+02	1.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T09-B	1	6.55E+02			6.55E+02	2.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	2.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	5.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	2.6E+01	1.8E+00	5.7E+00	10	300	3.08E+03	103%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T04-C	1	5.62E+00	E		5.62E+00	1.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T05-C	1	2.76E+02			2.76E+02	1.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T06-C	1	1.40E+02			1.40E+02	5.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T07-C	1	6.52E+02			6.52E+02	7.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T08-C	1	5.46E+02			5.46E+02	8.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-T09-C	1	6.85E+02			6.85E+02	6.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	3.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	2.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	3.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-B01-C	1	1.15E+00	U1/2		1.15E+00	3.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-B02-C	1	9.00E-01	U1/2		9.00E-01	5.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1313-B03-C	1	9.00E-01	U1/2		9.00E-01	5.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	EaFA-L10-1313-T01-A	1	6.67E+03			6.67E+03	1.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T02-A	1	6.29E+01			6.29E+01	2.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T03-A	1	5.77E+01			5.77E+01	1.7E+01	3.7E+00	1.2E+01	1000	100	8.91E+02	83%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T04-A	1	1.02E+02			1.02E+02	9.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T05-A	1	2.13E+01			2.13E+01	7.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T06-A	1	1.85E+00	U1/2		1.85E+00	2.3E+02	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T07-A	1	1.32E+01			1.32E+01	7.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T08-A	1	2.13E+01			2.13E+01	1.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T09-A	1	1.57E+03			1.57E+03	6.5E-01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T01-B	1	6.85E+03			6.85E+03	8.4E-01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T02-B	1	6.46E+01			6.46E+01	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T03-B	1	9.77E+01			9.77E+01	3.1E+00	3.7E+00	1.2E+01	1000	100	9.53E+02	86%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T04-B	1	9.90E+01			9.90E+01	1.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T05-B	1	1.79E+01			1.79E+01	3.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T06-B	1	1.02E+01	E		1.02E+01	1.1E+02	3.7E+00	1.2E+01				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T07-B	1	1.85E+00	U1/2		1.85E+00	3.9E+02	3.7E+00	1.2E+01				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T08-B	1	2.66E+01			2.66E+01	4.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T09-B	1	1.36E+03			1.36E+03	8.1E-01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T01-C	1	7.34E+03			7.34E+03	3.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T02-C	1	7.08E+01			7.08E+01	1.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T03-C	1	4.77E+01			4.77E+01	1.5E+01	3.7E+00	1.2E+01	1000	100	9.94E+02	95%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T04-C	1	9.70E+01			9.70E+01	8.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T05-C	1	3.09E+01			3.09E+01	2.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T06-C	1	7.90E+00	E		7.90E+00	4.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T07-C	1	1.75E+01			1.75E+01	1.4E+02	3.7E+00	1.2E+01				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T08-C	1	1.47E+01			1.47E+01	7.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-T09-C	1	1.44E+03			1.44E+03	1.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	7.6E+02	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	2.5E+02	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-B03-A	1	1.43E+01			1.43E+01	9.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-B01-C	1	1.85E+00	U1/2		1.85E+00	5.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-B02-C	1	1.85E+00	U1/2		1.85E+00	4.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1313-B03-C	1	4.45E+01			4.45E+01	1.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	EaFA-L10-1313-T01-A	1	9.61E+04			9.61E+04	6.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T02-A	1	3.06E+04			3.06E+04	1.4E+01	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T03-A	1	2.53E+04			2.53E+04	7.5E-01	1.6E+00	5.1E+00	1000	100	2.61E+04	82%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T04-A	1	2.80E+04			2.80E+04	2.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T05-A	1	2.31E+04			2.31E+04	4.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T06-A	1	2.42E+04			2.42E+04	3.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T07-A	1	2.65E+04			2.65E+04	6.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T08-A	1	1.64E+04			1.64E+04	3.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T09-A	1	1.91E+04			1.91E+04	6.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T01-B	1	9.46E+04			9.46E+04	3.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T02-B	1	3.44E+04			3.44E+04	7.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T03-B	1	2.50E+04			2.50E+04	4.2E-01	1.6E+00	5.1E+00	1000	100	2.58E+04	84%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T04-B	1	2.61E+04			2.61E+04	4.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T05-B	1	2.33E+04			2.33E+04	1.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T06-B	1	1.94E+04			1.94E+04	3.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T07-B	1	2.65E+04			2.65E+04	8.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T08-B	1	1.65E+04			1.65E+04	4.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T09-B	1	1.89E+04			1.89E+04	4.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T01-C	1	1.00E+05			1.00E+05	2.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T02-C	1	3.61E+04			3.61E+04	4.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T03-C	1	2.62E+04			2.62E+04	5.1E-01	1.6E+00	5.1E+00	1000	100	2.71E+04	84%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T04-C	1	2.62E+04			2.62E+04	7.9E-02	1.6E+00	5.1E+00				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T05-C	1	5.14E+04			5.14E+04	9.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T06-C	1	1.80E+04			1.80E+04	7.5E+00	1.6E+00	5.1E+00				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T07-C	1	2.68E+04			2.68E+04	2.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T08-C	1	1.69E+04			1.69E+04	8.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-T09-C	1	1.97E+04			1.97E+04	6.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-B01-A	1	2.21E+02			2.21E+02	6.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-B02-A	1	6.51E+01			6.51E+01	3.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-B03-A	1	1.66E+03			1.66E+03	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-B01-C	1	2.84E+02			2.84E+02	2.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-B02-C	1	7.32E+01			7.32E+01	3.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1313-B03-C	1	1.85E+03			1.85E+03	3.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	EaFA-L10-1313-T01-A	1	6.80E+03			6.80E+03	6.8E-01	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T02-A	1	5.28E+03			5.28E+03	1.4E+01	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T03-A	1	4.83E+03			4.83E+03	1.7E+00	1.5E+01	4.8E+01	10	300	7.32E+03	83%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T04-A	1	4.29E+03			4.29E+03	5.5E-01	1.5E+01	4.8E+01				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T05-A	1	7.87E+02			7.87E+02	2.0E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T06-A	1	2.59E+02			2.59E+02	1.6E+01	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T07-A	1	4.23E+02			4.23E+02	4.2E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T08-A	1	5.64E+01			5.64E+01	2.4E+01	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T09-A	1	4.26E+02			4.26E+02	5.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T01-B	1	6.82E+03			6.82E+03	1.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T02-B	1	5.87E+03			5.87E+03	4.3E-01	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T03-B	1	4.78E+03			4.78E+03	1.0E+00	1.5E+01	4.8E+01	10	300	7.41E+03	88%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T04-B	1	4.23E+03			4.23E+03	4.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T05-B	1	8.05E+02			8.05E+02	5.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T06-B	1	6.01E+02			6.01E+02	7.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T07-B	1	3.61E+02			3.61E+02	1.9E+01	1.5E+01	4.8E+01				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T08-B	1	4.19E+01	E		4.19E+01	5.5E+01	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T09-B	1	3.75E+02			3.75E+02	3.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T01-C	1	7.47E+03			7.47E+03	3.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T02-C	1	6.22E+03			6.22E+03	1.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T03-C	1	5.17E+03			5.17E+03	1.1E+00	1.5E+01	4.8E+01	10	300	7.77E+03	87%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T04-C	1	4.11E+03			4.11E+03	1.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T05-C	1	1.02E+03			1.02E+03	2.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T06-C	1	5.57E+02			5.57E+02	1.1E+01	1.5E+01	4.8E+01				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T07-C	1	3.94E+02			3.94E+02	4.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T08-C	1	4.57E+01	E		4.57E+01	6.1E+01	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-T09-C	1	3.80E+02			3.80E+02	6.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-B01-A	1	7.50E+00	U1/2		7.50E+00	1.8E+02	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-B02-A	1	2.83E+01	E		2.83E+01	4.8E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-B03-A	1	8.87E+01			8.87E+01	3.9E+01	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-B01-C	1	1.17E+02			1.17E+02	2.0E+01	1.5E+01	4.8E+01				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-B02-C	1	6.37E+01			6.37E+01	1.8E+01	1.5E+01	4.8E+01				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1313-B03-C	1	9.57E+01			9.57E+01	1.1E+01	1.5E+01	4.8E+01				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	EaFA-L10-1313-T01-A	1	1.58E+05			1.58E+05	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T02-A	1	7.11E+03			7.11E+03	1.1E+01	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T03-A	1	1.01E+03			1.01E+03	5.2E-01	1.1E+00	3.5E+00	1000	100	1.88E+03	88%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T04-A	1	3.84E+02			3.84E+02	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T05-A	1	2.05E+03			2.05E+03	3.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T06-A	1	6.84E+03			6.84E+03	6.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T07-A	1	7.55E+03			7.55E+03	6.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T08-A	1	4.33E+04			4.33E+04	2.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T09-A	1	6.13E+04			6.13E+04	1.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T01-B	1	1.61E+05			1.61E+05	2.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T02-B	1	7.76E+03			7.76E+03	8.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T03-B	1	8.66E+02			8.66E+02	9.7E-01	1.1E+00	3.5E+00	1000	100	1.73E+03	87%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T04-B	1	3.72E+02			3.72E+02	6.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T05-B	1	1.74E+03			1.74E+03	6.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T06-B	1	2.26E+03			2.26E+03	1.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T07-B	1	7.36E+03			7.36E+03	9.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T08-B	1	4.09E+04			4.09E+04	2.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T09-B	1	6.24E+04			6.24E+04	1.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T01-C	1	1.72E+05			1.72E+05	2.8E+00	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T02-C	1	8.50E+03			8.50E+03	3.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T03-C	1	1.57E+03			1.57E+03	4.4E-01	1.1E+00	3.5E+00	1000	100	2.40E+03	83%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T04-C	1	3.66E+02			3.66E+02	9.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T05-C	1	2.70E+03			2.70E+03	5.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T06-C	1	2.39E+03			2.39E+03	6.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T07-C	1	7.88E+03			7.88E+03	8.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T08-C	1	4.68E+04			4.68E+04	7.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-T09-C	1	6.45E+04			6.45E+04	6.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-B01-A	1	5.50E-01	U1/2		5.50E-01	1.6E+02	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-B02-A	1	5.50E-01	U1/2		5.50E-01	5.1E+01	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-B03-A	1	2.31E+02			2.31E+02	4.4E+00	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-B01-C	1	9.99E+00			9.99E+00	1.7E+01	1.1E+00	3.5E+00				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-B02-C	1	7.52E+00			7.52E+00	5.1E+01	1.1E+00	3.5E+00				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1313-B03-C	1	2.11E+02			2.11E+02	4.5E+00	1.1E+00	3.5E+00				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	EaFA-L10-1313-T01-A	1	3.78E+05			3.78E+05	1.6E+00	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T02-A	1	1.53E+05			1.53E+05	1.1E+01	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T03-A	1	5.48E+04			5.48E+04	1.3E+00	2.5E+00	8.0E+00	1000	100	5.57E+04	93%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T04-A	1	3.81E+04			3.81E+04	1.5E+00	2.5E+00	8.0E+00				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T05-A	1	4.77E+03			4.77E+03	8.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T06-A	1	4.86E+03			4.86E+03	5.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T07-A	1	5.78E+03			5.78E+03	9.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T08-A	1	3.34E+03			3.34E+03	5.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T09-A	1	2.76E+03			2.76E+03	2.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T01-B	1	3.77E+05			3.77E+05	2.5E+00	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T02-B	1	1.75E+05			1.75E+05	5.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T03-B	1	5.16E+04			5.16E+04	6.7E-01	2.5E+00	8.0E+00	1000	100	5.25E+04	95%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T04-B	1	3.84E+04			3.84E+04	2.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T05-B	1	4.80E+03			4.80E+03	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T06-B	1	5.67E+03			5.67E+03	5.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T07-B	1	5.74E+03			5.74E+03	8.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T08-B	1	7.10E+03			7.10E+03	8.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T09-B	1	2.71E+03			2.71E+03	8.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T01-C	1	3.94E+05			3.94E+05	2.8E+00	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T02-C	1	1.72E+05			1.72E+05	6.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T03-C	1	5.91E+04			5.91E+04	3.8E-01	2.5E+00	8.0E+00	1000	100	6.00E+04	90%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T04-C	1	3.76E+04			3.76E+04	6.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T05-C	1	1.05E+04			1.05E+04	5.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T06-C	1	5.34E+03			5.34E+03	8.0E+00	2.5E+00	8.0E+00				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T07-C	1	5.78E+03			5.78E+03	2.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T08-C	1	2.97E+03			2.97E+03	7.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-T09-C	1	2.77E+03			2.77E+03	5.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-B01-A	1	2.96E+01			2.96E+01	3.9E+00	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-B02-A	1	5.54E+01			5.54E+01	5.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-B03-A	1	3.90E+05			3.90E+05	7.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-B01-C	1	3.10E+01			3.10E+01	2.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-B02-C	1	4.19E+01			4.19E+01	8.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1313-B03-C	1	4.63E+05			4.63E+05	1.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	EaFA-L10-1313-T01-A	1	1.70E+03			1.70E+03	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T02-A	1	1.20E+03			1.20E+03	1.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T03-A	1	1.67E+03			1.67E+03	1.1E+00	1.0E+00	3.2E+00	1000	100	2.55E+03	88%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T04-A	1	1.97E+03			1.97E+03	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T05-A	1	2.02E+03			2.02E+03	2.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T06-A	1	2.54E+03			2.54E+03	5.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T07-A	1	2.96E+03			2.96E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T08-A	1	3.84E+03			3.84E+03	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T09-A	1	4.67E+03			4.67E+03	8.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T01-B	1	1.74E+03			1.74E+03	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T02-B	1	1.26E+03			1.26E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T03-B	1	1.65E+03			1.65E+03	1.0E+00	1.0E+00	3.2E+00	1000	100	2.49E+03	84%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T04-B	1	1.94E+03			1.94E+03	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T05-B	1	2.23E+03			2.23E+03	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T06-B	1	2.42E+03			2.42E+03	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T07-B	1	2.80E+03			2.80E+03	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T08-B	1	3.75E+03			3.75E+03	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T09-B	1	4.67E+03			4.67E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T01-C	1	1.82E+03			1.82E+03	3.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T02-C	1	1.29E+03			1.29E+03	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T03-C	1	1.69E+03			1.69E+03	3.7E-01	1.0E+00	3.2E+00	1000	100	2.55E+03	85%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T04-C	1	1.91E+03			1.91E+03	1.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T05-C	1	3.89E+03			3.89E+03	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T06-C	1	2.36E+03			2.36E+03	4.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T07-C	1	2.86E+03			2.86E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T08-C	1	4.00E+03			4.00E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-T09-C	1	4.83E+03			4.83E+03	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	7.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	7.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-B03-A	1	4.50E+00			4.50E+00	2.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	1.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	2.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1313-B03-C	1	2.79E+00	E		2.79E+00	2.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	EaFA-L10-1313-T01-A	1	1.54E+05			1.54E+05	2.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T02-A	1	1.36E+05			1.36E+05	1.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T03-A	1	1.41E+05			1.41E+05	6.0E-01	6.8E+00	2.2E+01	1000	100	1.42E+05	80%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T04-A	1	1.58E+05			1.58E+05	3.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T05-A	1	1.39E+05			1.39E+05	3.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T06-A	1	1.29E+05			1.29E+05	4.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T07-A	1	1.47E+05			1.47E+05	7.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T08-A	1	6.79E+04			6.79E+04	4.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T09-A	1	5.54E+04			5.54E+04	4.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T01-B	1	1.57E+05			1.57E+05	2.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T02-B	1	1.47E+05			1.47E+05	8.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T03-B	1	1.44E+05			1.44E+05	8.3E-01	6.8E+00	2.2E+01	1000	100	1.45E+05	89%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T04-B	1	1.53E+05			1.53E+05	5.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T05-B	1	1.42E+05			1.42E+05	9.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T06-B	1	1.42E+05			1.42E+05	2.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T07-B	1	1.44E+05			1.44E+05	1.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T08-B	1	7.81E+04			7.81E+04	7.9E-02	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T09-B	1	5.41E+04			5.41E+04	1.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T01-C	1	1.67E+05			1.67E+05	3.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T02-C	1	1.60E+05			1.60E+05	8.0E-02	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T03-C	1	1.52E+05			1.52E+05	1.4E-01	6.8E+00	2.2E+01	1000	100	1.53E+05	82%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T04-C	1	1.52E+05			1.52E+05	3.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T05-C	1	3.08E+05			3.08E+05	4.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T06-C	1	1.37E+05			1.37E+05	6.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T07-C	1	1.47E+05			1.47E+05	3.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T08-C	1	7.22E+04			7.22E+04	6.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-T09-C	1	5.73E+04			5.73E+04	3.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-B01-A	1	2.06E+01	E		2.06E+01	6.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-B02-A	1	1.93E+01	E		1.93E+01	9.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-B03-A	1	1.64E+02			1.64E+02	5.8E+00	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-B01-C	1	2.02E+01	E		2.02E+01	9.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-B02-C	1	2.57E+01			2.57E+01	5.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1313-B03-C	1	1.45E+02			1.45E+02	1.8E+00	6.8E+00	2.2E+01				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

TI	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
TI	EaFA-L10-1313-T01-A	1	9.66E+00	E		9.66E+00	5.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T02-A	1	2.30E+00	U1/2		2.30E+00	1.1E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T03-A	1	2.30E+00	U1/2		2.30E+00	3.7E+01	4.6E+00	1.5E+01	10	300	2.74E+03	91%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T04-A	1	2.30E+00	U1/2		2.30E+00	3.4E+02	4.6E+00	1.5E+01				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T05-A	1	2.30E+00	U1/2		2.30E+00	8.2E+02	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T06-A	1	2.60E+01			2.60E+01	3.5E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T07-A	1	3.83E+01			3.83E+01	1.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T08-A	1	4.28E+01			4.28E+01	1.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T09-A	1	5.68E+01			5.68E+01	1.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T01-B	1	2.30E+00	U1/2		2.30E+00	1.1E+02	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T02-B	1	2.30E+00	U1/2		2.30E+00	2.4E+02	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T03-B	1	2.30E+00	U1/2		2.30E+00	2.9E+01	4.6E+00	1.5E+01	10	300	2.87E+03	96%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T04-B	1	2.30E+00	U1/2		2.30E+00	8.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T05-B	1	2.30E+00	U1/2		2.30E+00	6.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T06-B	1	7.87E+00	E		7.87E+00	3.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T07-B	1	5.39E+01			5.39E+01	2.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T08-B	1	3.86E+01			3.86E+01	1.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T09-B	1	5.66E+01			5.66E+01	1.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T01-C	1	1.10E+01	E		1.10E+01	1.1E+02	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T02-C	1	2.30E+00	U1/2		2.30E+00	6.5E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T03-C	1	2.30E+00	U1/2		2.30E+00	4.0E+01	4.6E+00	1.5E+01	10	300	3.01E+03	100%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T04-C	1	2.30E+00	U1/2		2.30E+00	2.5E+02	4.6E+00	1.5E+01				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T05-C	1	2.30E+00	U1/2		2.30E+00	4.9E+02	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T06-C	1	1.59E+01			1.59E+01	1.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T07-C	1	3.65E+01			3.65E+01	2.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T08-C	1	4.66E+01			4.66E+01	1.5E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-T09-C	1	5.74E+01			5.74E+01	1.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	2.4E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	6.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	7.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-B01-C	1	2.30E+00	U1/2		2.30E+00	5.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-B02-C	1	2.30E+00	U1/2		2.30E+00	7.8E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
TI	EaFA-L10-1313-B03-C	1	2.30E+00	U1/2		2.30E+00	3.9E+02	4.6E+00	1.5E+01				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	EaFA-L10-1313-T01-A	1	9.07E+01			9.07E+01	5.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	2.9E+01	2.0E+00	6.4E+00	10	300	2.68E+03	89%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	1.6E+02	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	2.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T08-A	1	7.36E+01			7.36E+01	3.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T09-A	1	2.22E+03			2.22E+03	2.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T01-B	1	9.36E+01			9.36E+01	2.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	7.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	5.9E+01	2.0E+00	6.4E+00	10	300	2.83E+03	94%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	5.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	5.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	8.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T08-B	1	4.18E+01			4.18E+01	9.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T09-B	1	1.73E+03			1.73E+03	2.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T01-C	1	9.53E+01			9.53E+01	2.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	3.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00	10	300	2.96E+03	99%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	1.5E+02	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	2.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	1.1E+03	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	1.9E+03	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T08-C	1	7.67E+01			7.67E+01	8.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-T09-C	1	1.77E+03			1.77E+03	2.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	8.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	8.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	2.7E+02	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	2.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1313-B03-C	1	1.00E+00	U1/2		1.00E+00	1.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	EaFA-L10-1313-T01-A	1	7.17E+03			7.17E+03	1.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T02-A	1	3.28E+03			3.28E+03	1.0E+01	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T03-A	1	2.33E+03			2.33E+03	1.3E+00	1.5E+00	4.8E+00	10	300	4.80E+03	82%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T04-A	1	9.25E+02			9.25E+02	8.6E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T05-A	1	1.65E+02			1.65E+02	8.0E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T06-A	1	9.27E+01			9.27E+01	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T07-A	1	1.10E+02			1.10E+02	1.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T08-A	1	2.69E+02			2.69E+02	7.4E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T09-A	1	4.74E+03			4.74E+03	1.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T01-B	1	7.31E+03			7.31E+03	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T02-B	1	3.45E+03			3.45E+03	7.2E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T03-B	1	2.27E+03			2.27E+03	1.5E+00	1.5E+00	4.8E+00	10	300	4.96E+03	90%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T04-B	1	9.01E+02			9.01E+02	2.1E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T05-B	1	1.49E+02			1.49E+02	1.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T06-B	1	1.47E+02			1.47E+02	1.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T07-B	1	1.02E+02			1.02E+02	1.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T08-B	1	1.56E+02			1.56E+02	1.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T09-B	1	5.31E+03			5.31E+03	8.6E-02	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T01-C	1	7.69E+03			7.69E+03	2.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T02-C	1	3.79E+03			3.79E+03	5.2E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T03-C	1	2.84E+03			2.84E+03	4.7E-01	1.5E+00	4.8E+00	10	300	5.58E+03	91%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T04-C	1	8.59E+02			8.59E+02	4.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T05-C	1	2.11E+02			2.11E+02	8.6E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T06-C	1	1.32E+02			1.32E+02	1.0E+01	1.5E+00	4.8E+00				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T07-C	1	1.08E+02			1.08E+02	2.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T08-C	1	2.87E+02			2.87E+02	1.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-T09-C	1	5.51E+03			5.51E+03	7.0E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-B01-A	1	5.89E+00			5.89E+00	8.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-B02-A	1	5.89E+00			5.89E+00	1.9E+01	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-B03-A	1	6.37E+00			6.37E+00	2.4E+01	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-B01-C	1	2.57E+00	E		2.57E+00	7.5E+01	1.5E+00	4.8E+00				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-B02-C	1	1.79E+00	E		1.79E+00	7.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1313-B03-C	1	4.84E+00			4.84E+00	8.4E+01	1.5E+00	4.8E+00				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	EaFA-L10-1313-T01-A	1	2.04E+03			2.04E+03	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:44 AM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T02-A	1	1.56E+01			1.56E+01	1.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:46 AM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T03-A	1	5.79E+00			5.79E+00	3.2E+00	1.0E+00	3.2E+00	10	300	2.86E+03	95%	VU ICP-OES	7/1/10 11:48 AM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T04-A	1	5.50E+00			5.50E+00	1.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:10 AM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T05-A	1	2.27E+01			2.27E+01	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:51 AM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T06-A	1	1.10E+03			1.10E+03	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:53 AM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T07-A	1	1.02E+03			1.02E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:14 AM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T08-A	1	1.17E+03			1.17E+03	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:56 AM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T09-A	1	1.40E+03			1.40E+03	6.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:57 AM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T01-B	1	2.10E+03			2.10E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:04 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T02-B	1	1.44E+01			1.44E+01	7.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:06 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T03-B	1	3.48E+00			3.48E+00	1.9E+01	1.0E+00	3.2E+00	10	300	3.03E+03	101%	VU ICP-OES	7/1/10 12:07 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T04-B	1	4.52E+00			4.52E+00	1.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:00 AM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T05-B	1	4.37E+01			4.37E+01	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:11 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T06-B	1	1.82E+01			1.82E+01	5.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:02 AM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T07-B	1	1.28E+03			1.28E+03	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:03 AM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T08-B	1	1.17E+03			1.17E+03	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:46 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T09-B	1	1.41E+03			1.41E+03	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:17 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T01-C	1	2.17E+03			2.17E+03	2.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:24 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T02-C	1	1.61E+01			1.61E+01	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:25 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T03-C	1	2.44E+00	E		2.44E+00	4.2E+01	1.0E+00	3.2E+00	10	300	3.21E+03	107%	VU ICP-OES	7/1/10 12:27 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T04-C	1	4.13E+00			4.13E+00	1.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:05 AM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T05-C	1	3.62E+01			3.62E+01	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:30 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T06-C	1	1.91E+01			1.91E+01	6.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:07 AM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T07-C	1	1.33E+03			1.33E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 11:08 AM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T08-C	1	1.23E+03			1.23E+03	6.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:35 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-T09-C	1	1.47E+03			1.47E+03	8.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:37 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-B01-A	1	3.92E+00			3.92E+00	3.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:39 AM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-B02-A	1	1.39E+01			1.39E+01	3.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:41 AM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-B03-A	1	4.98E+01			4.98E+01	2.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 11:43 AM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-B01-C	1	6.05E+00			6.05E+00	6.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 10:50 AM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-B02-C	1	1.96E+01			1.96E+01	3.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 10:52 AM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1313-B03-C	1	5.28E+01			5.28E+01	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/20/10 10:53 AM	EPA Interlab L10 1313-1316 EaFA

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	EaFA-L11-1313-T01-A	1	3.55E+04			3.55E+04	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T02-A	1	4.70E+04			4.70E+04	1.3E+00	1.0E+00	3.2E+00	1000	100	4.80E+04	94%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T03-A	1	1.70E+04			1.70E+04	3.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T04-A	1	3.45E+03			3.45E+03	6.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T05-A	1	6.65E+02			6.65E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T06-A	1	1.29E+02			1.29E+02	8.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T07-A	1	8.19E+02			8.19E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T08-A	1	4.85E+04			4.85E+04	7.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T09-A	1	1.19E+05			1.19E+05	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T01-B	1	3.73E+04			3.73E+04	8.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T02-B	1	3.57E+04			3.57E+04	1.2E+00	1.0E+00	3.2E+00	1000	100	3.65E+04	86%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T03-B	1	2.31E+04			2.31E+04	1.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T04-B	1	2.77E+03			2.77E+03	6.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T05-B	1	5.16E+02			5.16E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T06-B	1	1.30E+02			1.30E+02	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T07-B	1	1.80E+03			1.80E+03	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T08-B	1	5.78E+04			5.78E+04	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T09-B	1	1.18E+05			1.18E+05	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T01-C	1	3.63E+04			3.63E+04	3.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T02-C	1	3.60E+04			3.60E+04	3.5E-01	1.0E+00	3.2E+00	1000	100	3.69E+04	88%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T03-C	1	2.27E+04			2.27E+04	4.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T04-C	1	2.88E+03			2.88E+03	5.7E-01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T05-C	1	6.30E+02			6.30E+02	8.2E-01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T06-C	1	1.31E+02			1.31E+02	1.7E+00	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T07-C	1	1.87E+03			1.87E+03	9.8E-01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T08-C	1	5.81E+04			5.81E+04	3.2E-01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-T09-C	1	1.18E+05			1.18E+05	6.3E-01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-B01-A	1	1.47E+00	E		1.47E+00	5.2E+00	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-B02-A	1	5.73E+00			5.73E+00	1.9E+00	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1313-B03-A	1	4.49E+00			4.49E+00	1.0E+01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	EaFA-L11-1313-T01-A	1	1.89E+02			1.89E+02	1.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T02-A	1	1.78E+02			1.78E+02	1.8E+01	7.5E+00	2.4E+01	10	325	3.33E+03	97%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T03-A	1	1.12E+02			1.12E+02	1.8E+01	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T04-A	1	9.58E+01			9.58E+01	2.5E+01	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T05-A	1	1.06E+02			1.06E+02	2.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T06-A	1	9.29E+01			9.29E+01	1.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T07-A	1	9.77E+01			9.77E+01	1.9E+01	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T08-A	1	2.38E+01	E		2.38E+01	1.1E+02	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T09-A	1	3.75E+00	U1/2		3.75E+00	9.6E+01	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T01-B	1	1.80E+02			1.80E+02	8.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T02-B	1	1.75E+02			1.75E+02	3.6E+00	7.5E+00	2.4E+01	10	325	3.74E+03	110%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T03-B	1	1.36E+02			1.36E+02	1.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T04-B	1	1.15E+02			1.15E+02	3.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T05-B	1	1.26E+02			1.26E+02	1.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T06-B	1	1.07E+02			1.07E+02	1.9E+01	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T07-B	1	1.06E+02			1.06E+02	2.5E+01	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T08-B	1	3.92E+01			3.92E+01	2.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T09-B	1	3.75E+00	U1/2		3.75E+00	2.0E+02	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T01-C	1	1.99E+02			1.99E+02	2.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T02-C	1	1.60E+02			1.60E+02	2.0E+01	7.5E+00	2.4E+01	10	325	3.67E+03	108%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T03-C	1	1.21E+02			1.21E+02	1.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T04-C	1	1.14E+02			1.14E+02	1.5E+01	7.5E+00	2.4E+01					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T05-C	1	1.20E+02			1.20E+02	2.9E+01	7.5E+00	2.4E+01					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T06-C	1	1.20E+02			1.20E+02	2.3E+01	7.5E+00	2.4E+01					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T07-C	1	8.27E+01			8.27E+01	2.5E+01	7.5E+00	2.4E+01					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T08-C	1	3.54E+01			3.54E+01	7.8E+00	7.5E+00	2.4E+01					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-T09-C	1	3.75E+00	U1/2		3.75E+00	7.5E+00	7.5E+00	2.4E+01					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-B01-A	1	3.75E+00	U1/2		3.75E+00	7.3E+01	7.5E+00	2.4E+01					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-B02-A	1	3.75E+00	U1/2		3.75E+00	3.3E+01	7.5E+00	2.4E+01					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1313-B03-A	1	3.75E+00	U1/2		3.75E+00	5.7E+01	7.5E+00	2.4E+01					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	EaFA-L11-1313-T01-A	1	6.09E+03			6.09E+03	6.7E-01	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T02-A	1	1.82E+03			1.82E+03	1.6E+00	1.1E+01	3.5E+01	10	325	5.03E+03	99%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T03-A	1	4.60E+02			4.60E+02	5.7E+00	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T04-A	1	2.53E+02			2.53E+02	9.7E+00	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T05-A	1	1.02E+02			1.02E+02	1.4E+01	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T06-A	1	4.30E+01			4.30E+01	5.6E+01	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T07-A	1	8.39E+01			8.39E+01	2.5E+01	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T08-A	1	5.93E+01			5.93E+01	5.5E+01	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T09-A	1	3.19E+03			3.19E+03	6.7E-01	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T01-B	1	5.81E+03			5.81E+03	1.1E+00	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T02-B	1	2.01E+03			2.01E+03	1.6E+00	1.1E+01	3.5E+01	10	325	5.52E+03	108%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T03-B	1	7.27E+02			7.27E+02	1.3E+00	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T04-B	1	2.25E+02			2.25E+02	4.3E+00	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T05-B	1	1.29E+02			1.29E+02	1.7E+01	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T06-B	1	5.34E+01			5.34E+01	2.6E+01	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T07-B	1	6.08E+01			6.08E+01	1.8E+01	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T08-B	1	6.67E+01			6.67E+01	1.4E+01	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T09-B	1	3.35E+03			3.35E+03	3.8E-01	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T01-C	1	5.67E+03			5.67E+03	1.0E+00	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T02-C	1	2.01E+03			2.01E+03	7.5E-01	1.1E+01	3.5E+01	10	325	5.41E+03	104%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T03-C	1	6.66E+02			6.66E+02	1.4E+00	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T04-C	1	2.14E+02			2.14E+02	1.3E+01	1.1E+01	3.5E+01					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T05-C	1	1.21E+02			1.21E+02	1.6E+01	1.1E+01	3.5E+01					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T06-C	1	4.26E+01			4.26E+01	3.1E+01	1.1E+01	3.5E+01					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T07-C	1	7.31E+01			7.31E+01	1.6E+01	1.1E+01	3.5E+01					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T08-C	1	6.46E+01			6.46E+01	2.5E+01	1.1E+01	3.5E+01					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-T09-C	1	3.33E+03			3.33E+03	8.6E-01	1.1E+01	3.5E+01					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-B01-A	1	5.50E+00	U1/2		5.50E+00	1.7E+02	1.1E+01	3.5E+01					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-B02-A	1	5.50E+00	U1/2		5.50E+00	6.4E+01	1.1E+01	3.5E+01					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1313-B03-A	1	5.50E+00	U1/2		5.50E+00	3.1E+01	1.1E+01	3.5E+01					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	EaFA-L11-1313-T01-A	1	2.76E+03			2.76E+03	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T02-A	1	3.24E+03			3.24E+03	1.6E+00	1.0E+00	3.2E+00	1000	100	4.13E+03	89%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T03-A	1	3.96E+03			3.96E+03	4.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T04-A	1	3.95E+03			3.95E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T05-A	1	4.05E+03			4.05E+03	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T06-A	1	4.30E+03			4.30E+03	2.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T07-A	1	4.36E+03			4.36E+03	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T08-A	1	3.46E+03			3.46E+03	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T09-A	1	2.95E+03			2.95E+03	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T01-B	1	2.68E+03			2.68E+03	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T02-B	1	3.31E+03			3.31E+03	7.9E-01	1.0E+00	3.2E+00	1000	100	4.26E+03	95%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T03-B	1	4.03E+03			4.03E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T04-B	1	4.01E+03			4.01E+03	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T05-B	1	4.15E+03			4.15E+03	5.6E-02	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T06-B	1	4.31E+03			4.31E+03	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T07-B	1	4.13E+03			4.13E+03	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T08-B	1	3.47E+03			3.47E+03	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T09-B	1	2.95E+03			2.95E+03	6.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T01-C	1	2.55E+03			2.55E+03	3.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T02-C	1	3.33E+03			3.33E+03	4.8E-01	1.0E+00	3.2E+00	1000	100	4.26E+03	94%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T03-C	1	4.01E+03			4.01E+03	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T04-C	1	4.04E+03			4.04E+03	2.8E-01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T05-C	1	4.09E+03			4.09E+03	4.7E-01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T06-C	1	4.30E+03			4.30E+03	3.6E-01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T07-C	1	4.12E+03			4.12E+03	5.6E-01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T08-C	1	3.46E+03			3.46E+03	1.5E-01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-T09-C	1	2.95E+03			2.95E+03	7.4E-01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-B01-A	1	1.24E+01			1.24E+01	6.8E+00	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-B02-A	1	1.34E+01			1.34E+01	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1313-B03-A	1	1.48E+02			1.48E+02	2.5E+00	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	EaFA-L11-1313-T01-A	1	1.54E+03			1.54E+03	9.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T02-A	1	1.61E+03			1.61E+03	1.8E+00	1.0E+00	3.2E+00	10	325	4.34E+03	84%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T03-A	1	4.74E+02			4.74E+02	3.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T04-A	1	3.43E+02			3.43E+02	4.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T05-A	1	3.10E+02			3.10E+02	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T06-A	1	2.91E+02			2.91E+02	4.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T07-A	1	3.44E+02			3.44E+02	7.3E-02	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T08-A	1	4.21E+02			4.21E+02	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T09-A	1	8.12E+02			8.12E+02	3.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T01-B	1	1.33E+03			1.33E+03	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T02-B	1	1.16E+03			1.16E+03	1.1E+00	1.0E+00	3.2E+00	10	325	4.23E+03	95%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T03-B	1	4.93E+02			4.93E+02	1.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T04-B	1	3.46E+02			3.46E+02	7.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T05-B	1	3.14E+02			3.14E+02	3.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T06-B	1	2.95E+02			2.95E+02	1.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T07-B	1	3.52E+02			3.52E+02	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T08-B	1	2.96E+02			2.96E+02	1.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T09-B	1	8.16E+02			8.16E+02	2.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T01-C	1	1.43E+03			1.43E+03	3.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T02-C	1	1.01E+03			1.01E+03	8.1E-01	1.0E+00	3.2E+00	10	325	4.07E+03	94%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T03-C	1	4.54E+02			4.54E+02	2.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T04-C	1	3.60E+02			3.60E+02	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T05-C	1	3.08E+02			3.08E+02	7.6E-02	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T06-C	1	2.92E+02			2.92E+02	8.1E-01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T07-C	1	3.38E+02			3.38E+02	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T08-C	1	2.76E+02			2.76E+02	2.6E-01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-T09-C	1	7.94E+02			7.94E+02	5.5E-01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-B01-A	1	1.31E+00	E		1.31E+00	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-B02-A	1	2.04E+00	E		2.04E+00	2.9E+00	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1313-B03-A	1	2.08E+00	E		2.08E+00	1.7E+01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	EaFA-L11-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	3.7E+01	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	6.0E+01	1.9E+00	6.0E+00	10	325	3.26E+03	100%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	2.5E+01	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	7.9E+01	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	6.6E+01	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T07-A	1	6.79E+00			6.79E+00	9.1E+00	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T08-A	1	1.42E+02			1.42E+02	7.9E-01	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T09-A	1	2.53E+02			2.53E+02	5.5E-01	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	2.0E+01	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	4.2E+02	1.9E+00	6.0E+00	10	325	3.65E+03	112%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	2.5E+02	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	2.4E+01	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	3.2E+02	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	9.7E+01	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T07-B	1	1.34E+01			1.34E+01	3.6E+00	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T08-B	1	1.72E+02			1.72E+02	1.3E+00	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T09-B	1	2.55E+02			2.55E+02	9.1E-01	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	2.4E+01	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	1.3E+03	1.9E+00	6.0E+00	10	325	3.60E+03	111%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	1.1E+03	1.9E+00	6.0E+00					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	1.7E+02	1.9E+00	6.0E+00					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	5.8E+01	1.9E+00	6.0E+00					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T07-C	1	1.42E+01			1.42E+01	1.4E+00	1.9E+00	6.0E+00					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T08-C	1	1.73E+02			1.73E+02	6.3E-01	1.9E+00	6.0E+00					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-T09-C	1	2.51E+02			2.51E+02	5.3E-01	1.9E+00	6.0E+00					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	1.0E+01	1.9E+00	6.0E+00					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	3.7E+01	1.9E+00	6.0E+00					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	1.5E+02	1.9E+00	6.0E+00					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	EaFA-L11-1313-T01-A	1	1.10E+00	U1/2		1.10E+00	2.3E+02	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T02-A	1	1.10E+00	U1/2		1.10E+00	1.7E+02	2.2E+00	7.0E+00	10	325	3.23E+03	99%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	6.0E+01	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T04-A	1	1.10E+00	U1/2		1.10E+00	6.0E+01	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T05-A	1	1.10E+00	U1/2		1.10E+00	4.4E+02	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T06-A	1	1.10E+00	U1/2		1.10E+00	4.1E+01	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T07-A	1	3.59E+01			3.59E+01	7.7E-01	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T08-A	1	2.76E+01			2.76E+01	3.0E+00	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T09-A	1	3.46E+01			3.46E+01	6.8E-01	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T01-B	1	1.10E+00	U1/2		1.10E+00	5.3E+01	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T02-B	1	1.10E+00	U1/2		1.10E+00	2.2E+02	2.2E+00	7.0E+00	10	325	3.61E+03	111%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	7.8E+01	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T04-B	1	1.10E+00	U1/2		1.10E+00	2.4E+02	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T05-B	1	1.10E+00	U1/2		1.10E+00	3.4E+02	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T06-B	1	1.10E+00	U1/2		1.10E+00	1.0E+02	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T07-B	1	3.79E+01			3.79E+01	1.0E+00	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T08-B	1	2.91E+01			2.91E+01	3.1E+00	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T09-B	1	3.46E+01			3.46E+01	1.7E+00	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T01-C	1	1.10E+00	U1/2		1.10E+00	2.2E+02	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T02-C	1	1.10E+00	U1/2		1.10E+00	1.6E+02	2.2E+00	7.0E+00	10	325	3.55E+03	109%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	1.4E+02	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T04-C	1	1.10E+00	U1/2		1.10E+00	7.2E+01	2.2E+00	7.0E+00					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T05-C	1	1.10E+00	U1/2		1.10E+00	2.7E+02	2.2E+00	7.0E+00					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T06-C	1	1.10E+00	U1/2		1.10E+00	3.3E+01	2.2E+00	7.0E+00					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T07-C	1	3.78E+01			3.78E+01	2.8E+00	2.2E+00	7.0E+00					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T08-C	1	2.92E+01			2.92E+01	2.1E+00	2.2E+00	7.0E+00					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-T09-C	1	3.46E+01			3.46E+01	1.1E+00	2.2E+00	7.0E+00					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	7.9E+01	2.2E+00	7.0E+00					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	3.4E+04	2.2E+00	7.0E+00					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1313-B03-A	1	1.10E+00	U1/2		1.10E+00	2.1E+01	2.2E+00	7.0E+00					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	EaFA-L11-1313-T01-A	1	1.59E+04			1.59E+04	5.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T02-A	1	2.64E+04			2.64E+04	1.1E+00	2.6E+00	8.3E+00	1000	100	2.73E+04	90%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T03-A	1	9.85E+04			9.85E+04	3.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T04-A	1	1.28E+05			1.28E+05	6.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T05-A	1	1.42E+05			1.42E+05	3.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T06-A	1	1.57E+05			1.57E+05	1.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T07-A	1	1.64E+05			1.64E+05	4.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T08-A	1	1.47E+05			1.47E+05	1.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T09-A	1	1.39E+05			1.39E+05	7.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T01-B	1	1.57E+04			1.57E+04	1.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T02-B	1	4.37E+04			4.37E+04	6.9E-01	2.6E+00	8.3E+00	1000	100	4.46E+04	88%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T03-B	1	1.01E+05			1.01E+05	1.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T04-B	1	1.30E+05			1.30E+05	7.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T05-B	1	1.45E+05			1.45E+05	6.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T06-B	1	1.56E+05			1.56E+05	1.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T07-B	1	1.54E+05			1.54E+05	1.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T08-B	1	1.47E+05			1.47E+05	1.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T09-B	1	1.39E+05			1.39E+05	6.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T01-C	1	1.56E+04			1.56E+04	2.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T02-C	1	4.30E+04			4.30E+04	8.0E-01	2.6E+00	8.3E+00	1000	100	4.39E+04	86%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T03-C	1	1.00E+05			1.00E+05	3.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T04-C	1	1.30E+05			1.30E+05	4.5E-01	2.6E+00	8.3E+00					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T05-C	1	1.43E+05			1.43E+05	6.0E-01	2.6E+00	8.3E+00					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T06-C	1	1.53E+05			1.53E+05	1.1E+00	2.6E+00	8.3E+00					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T07-C	1	1.53E+05			1.53E+05	6.1E-01	2.6E+00	8.3E+00					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T08-C	1	1.46E+05			1.46E+05	5.4E-01	2.6E+00	8.3E+00					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-T09-C	1	1.39E+05			1.39E+05	2.0E-01	2.6E+00	8.3E+00					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-B01-A	1	3.45E+00	E		3.45E+00	6.6E+01	2.6E+00	8.3E+00					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-B02-A	1	4.70E+01			4.70E+01	2.5E+01	2.6E+00	8.3E+00					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1313-B03-A	1	1.86E+01			1.86E+01	2.6E+01	2.6E+00	8.3E+00					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	EaFA-L11-1313-T01-A	1	5.19E+02			5.19E+02	9.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T02-A	1	4.89E+02			4.89E+02	1.2E+00	1.2E+00	3.8E+00	10	325	3.59E+03	95%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T03-A	1	4.54E+02			4.54E+02	7.7E-02	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T04-A	1	4.03E+02			4.03E+02	3.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T05-A	1	3.32E+02			3.32E+02	5.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T06-A	1	1.21E+02			1.21E+02	6.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T07-A	1	4.13E+00			4.13E+00	5.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T08-A	1	6.57E+02			6.57E+02	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T09-A	1	1.81E+03			1.81E+03	8.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T01-B	1	5.46E+02			5.46E+02	1.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T02-B	1	4.67E+02			4.67E+02	2.6E-01	1.2E+00	3.8E+00	10	325	3.93E+03	107%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T03-B	1	4.16E+02			4.16E+02	3.0E-02	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T04-B	1	3.76E+02			3.76E+02	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T05-B	1	2.95E+02			2.95E+02	1.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T06-B	1	1.20E+02			1.20E+02	2.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T07-B	1	3.86E+00			3.86E+00	2.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T08-B	1	8.29E+02			8.29E+02	1.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T09-B	1	1.80E+03			1.80E+03	5.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T01-C	1	5.18E+02			5.18E+02	5.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T02-C	1	4.60E+02			4.60E+02	1.1E+00	1.2E+00	3.8E+00	10	325	3.84E+03	104%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T03-C	1	4.28E+02			4.28E+02	9.3E-02	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T04-C	1	3.82E+02			3.82E+02	2.9E-01	1.2E+00	3.8E+00					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T05-C	1	2.95E+02			2.95E+02	3.6E-01	1.2E+00	3.8E+00					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T06-C	1	1.20E+02			1.20E+02	1.3E+00	1.2E+00	3.8E+00					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T07-C	1	2.90E+00	E		2.90E+00	1.8E+01	1.2E+00	3.8E+00					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T08-C	1	8.25E+02			8.25E+02	1.1E+00	1.2E+00	3.8E+00					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-T09-C	1	1.81E+03			1.81E+03	5.2E-01	1.2E+00	3.8E+00					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	1.8E+02	1.2E+00	3.8E+00					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	2.4E+02	1.2E+00	3.8E+00					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1313-B03-A	1	2.83E+00	E		2.83E+00	4.5E+01	1.2E+00	3.8E+00					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	EaFA-L11-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	4.4E+01	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	7.5E+00	1.8E+00	5.7E+00	10	325	3.12E+03	96%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	3.3E+02	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T05-A	1	1.89E+00	E		1.89E+00	2.3E+02	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T06-A	1	2.46E+01			2.46E+01	7.4E+00	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T07-A	1	2.32E+02			2.32E+02	1.7E+00	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T08-A	1	2.06E+02			2.06E+02	4.4E-01	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T09-A	1	3.94E+02			3.94E+02	6.0E-01	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	1.6E+02	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	9.5E+00	1.8E+00	5.7E+00	10	325	3.43E+03	106%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	6.1E+01	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	4.3E+01	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T05-B	1	1.85E+00	E		1.85E+00	1.1E+02	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T06-B	1	2.94E+01			2.94E+01	1.4E+01	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T07-B	1	2.33E+02			2.33E+02	5.4E-01	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T08-B	1	2.28E+02			2.28E+02	1.2E+00	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T09-B	1	3.89E+02			3.89E+02	2.8E-01	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	7.6E+02	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	2.8E+02	1.8E+00	5.7E+00	10	325	3.41E+03	105%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	9.1E+01	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	7.6E+01	1.8E+00	5.7E+00					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T05-C	1	2.96E+00	E		2.96E+00	4.0E+01	1.8E+00	5.7E+00					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T06-C	1	3.00E+01			3.00E+01	5.6E+00	1.8E+00	5.7E+00					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T07-C	1	2.33E+02			2.33E+02	2.2E+00	1.8E+00	5.7E+00					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T08-C	1	2.24E+02			2.24E+02	1.6E+00	1.8E+00	5.7E+00					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-T09-C	1	3.89E+02			3.89E+02	1.2E+00	1.8E+00	5.7E+00					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	1.2E+02	1.8E+00	5.7E+00					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	3.2E+01	1.8E+00	5.7E+00					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	1.7E+02	1.8E+00	5.7E+00					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	EaFA-L11-1313-T01-A	1	1.48E+01			1.48E+01	3.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T02-A	1	1.16E+01	E		1.16E+01	7.2E+02	3.7E+00	1.2E+01	10	325	3.08E+03	94%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T03-A	1	1.79E+01			1.79E+01	5.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T04-A	1	1.43E+01			1.43E+01	2.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T05-A	1	1.27E+01			1.27E+01	7.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T06-A	1	1.70E+01			1.70E+01	5.9E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T07-A	1	1.49E+02			1.49E+02	1.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T08-A	1	1.22E+03			1.22E+03	8.4E-01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T09-A	1	3.18E+03			3.18E+03	7.8E-01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T01-B	1	1.40E+01			1.40E+01	3.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T02-B	1	1.21E+01			1.21E+01	3.4E+01	3.7E+00	1.2E+01	10	325	3.44E+03	105%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T03-B	1	1.32E+01			1.32E+01	1.9E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T04-B	1	1.49E+01			1.49E+01	3.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T05-B	1	1.63E+01			1.63E+01	4.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T06-B	1	1.48E+01			1.48E+01	3.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T07-B	1	3.57E+02			3.57E+02	1.2E+00	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T08-B	1	2.34E+03			2.34E+03	1.2E+00	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T09-B	1	3.15E+03			3.15E+03	2.4E-01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T01-C	1	1.96E+01			1.96E+01	4.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T02-C	1	1.68E+01			1.68E+01	2.0E+01	3.7E+00	1.2E+01	10	325	3.37E+03	103%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T03-C	1	6.43E+00	E		6.43E+00	7.6E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T04-C	1	1.30E+01			1.30E+01	5.3E+01	3.7E+00	1.2E+01					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T05-C	1	1.45E+01			1.45E+01	4.2E+01	3.7E+00	1.2E+01					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T06-C	1	1.82E+01			1.82E+01	4.1E+00	3.7E+00	1.2E+01					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T07-C	1	3.78E+02			3.78E+02	7.1E-01	3.7E+00	1.2E+01					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T08-C	1	2.34E+03			2.34E+03	1.2E+00	3.7E+00	1.2E+01					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-T09-C	1	3.17E+03			3.17E+03	8.6E-01	3.7E+00	1.2E+01					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	1.2E+02	3.7E+00	1.2E+01					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	5.3E+01	3.7E+00	1.2E+01					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1313-B03-A	1	6.91E+00	E		6.91E+00	2.2E+01	3.7E+00	1.2E+01					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	EaFA-L11-1313-T01-A	1	2.30E+01			2.30E+01	3.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	5.3E+00	2.0E+00	6.4E+00	1000	100	1.02E+03	102%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	7.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	3.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	1.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T07-A	1	1.26E+01			1.26E+01	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T08-A	1	9.26E+02			9.26E+02	9.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T09-A	1	3.69E+04			3.69E+04	9.8E-01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T01-B	1	2.58E+01			2.58E+01	2.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T02-B	1	8.58E+00			8.58E+00	2.6E+00	2.0E+00	6.4E+00	1000	100	1.14E+03	113%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	3.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	8.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	7.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T07-B	1	2.73E+00	E		2.73E+00	1.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T08-B	1	1.81E+03			1.81E+03	3.6E-01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T09-B	1	3.66E+04			3.66E+04	5.4E-01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T01-C	1	3.00E+01			3.00E+01	4.2E-01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T02-C	1	7.97E+00			7.97E+00	9.4E+00	2.0E+00	6.4E+00	1000	100	1.12E+03	111%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	3.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	5.2E+00	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	9.5E+00	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	2.8E+01	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	7.3E+02	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T08-C	1	1.79E+03			1.79E+03	3.4E-01	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-T09-C	1	3.67E+04			3.67E+04	3.8E-01	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	8.0E+00	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-B02-A	1	4.61E+00	E		4.61E+00	1.3E+01	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1313-B03-A	1	5.58E+00	E		5.58E+00	1.3E+01	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	EaFA-L11-1313-T01-A	1	3.40E+00	U1/2		3.40E+00	3.3E+01	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T02-A	1	3.40E+00	U1/2		3.40E+00	1.2E+02	6.8E+00	2.2E+01	10	325	3.08E+03	95%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T03-A	1	3.40E+00	U1/2		3.40E+00	2.7E+01	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T04-A	1	3.40E+00	U1/2		3.40E+00	1.4E+02	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T05-A	1	3.40E+00	U1/2		3.40E+00	7.8E+01	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T06-A	1	3.40E+00	U1/2		3.40E+00	3.0E+01	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T07-A	1	3.40E+00	U1/2		3.40E+00	1.1E+02	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T08-A	1	3.40E+00	U1/2		3.40E+00	4.9E+00	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T09-A	1	8.99E+01			8.99E+01	1.9E+00	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T01-B	1	3.40E+00	U1/2		3.40E+00	3.0E+02	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T02-B	1	3.40E+00	U1/2		3.40E+00	1.9E+02	6.8E+00	2.2E+01	10	325	3.42E+03	105%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T03-B	1	3.40E+00	U1/2		3.40E+00	1.6E+01	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T04-B	1	3.40E+00	U1/2		3.40E+00	7.6E+01	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T05-B	1	3.40E+00	U1/2		3.40E+00	1.2E+02	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T06-B	1	3.40E+00	U1/2		3.40E+00	1.6E+02	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T07-B	1	3.40E+00	U1/2		3.40E+00	3.8E+01	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T08-B	1	3.40E+00	U1/2		3.40E+00	4.8E+01	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T09-B	1	8.26E+01			8.26E+01	1.3E+01	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T01-C	1	3.40E+00	U1/2		3.40E+00	2.3E+02	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T02-C	1	3.40E+00	U1/2		3.40E+00	1.5E+02	6.8E+00	2.2E+01	10	325	3.39E+03	104%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T03-C	1	3.40E+00	U1/2		3.40E+00	4.0E+01	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T04-C	1	3.40E+00	U1/2		3.40E+00	4.9E+01	6.8E+00	2.2E+01					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T05-C	1	3.40E+00	U1/2		3.40E+00	5.6E+01	6.8E+00	2.2E+01					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T06-C	1	3.40E+00	U1/2		3.40E+00	4.8E+01	6.8E+00	2.2E+01					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T07-C	1	3.40E+00	U1/2		3.40E+00	1.2E+01	6.8E+00	2.2E+01					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T08-C	1	3.40E+00	U1/2		3.40E+00	3.5E+01	6.8E+00	2.2E+01					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-T09-C	1	9.22E+01			9.22E+01	2.0E+00	6.8E+00	2.2E+01					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	2.7E+01	6.8E+00	2.2E+01					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	1.3E+02	6.8E+00	2.2E+01					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	7.4E+01	6.8E+00	2.2E+01					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	EaFA-L11-1313-T01-A	1	2.72E+03			2.72E+03	6.7E-01	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T02-A	1	3.03E+03			3.03E+03	1.2E+00	1.9E+00	6.0E+00	10	325	5.69E+03	82%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T03-A	1	2.47E+03			2.47E+03	6.9E-01	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T04-A	1	3.42E+03			3.42E+03	4.2E-01	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T05-A	1	3.49E+03			3.49E+03	1.2E+00	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T06-A	1	3.58E+03			3.58E+03	4.2E-01	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T07-A	1	3.75E+03			3.75E+03	3.1E-01	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T08-A	1	2.09E+03			2.09E+03	1.6E+00	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T09-A	1	1.72E+03			1.72E+03	9.0E-01	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T01-B	1	2.75E+03			2.75E+03	8.6E-01	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T02-B	1	3.02E+03			3.02E+03	6.9E-01	1.9E+00	6.0E+00	10	325	5.79E+03	85%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T03-B	1	3.28E+03			3.28E+03	8.1E-02	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T04-B	1	3.45E+03			3.45E+03	4.5E-01	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T05-B	1	3.53E+03			3.53E+03	7.9E-01	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T06-B	1	3.56E+03			3.56E+03	4.3E-01	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T07-B	1	3.43E+03			3.43E+03	1.2E+00	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T08-B	1	2.20E+03			2.20E+03	1.6E+00	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T09-B	1	1.73E+03			1.73E+03	3.1E-01	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T01-C	1	2.69E+03			2.69E+03	5.8E-01	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T02-C	1	3.05E+03			3.05E+03	9.5E-01	1.9E+00	6.0E+00	10	325	5.73E+03	83%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T03-C	1	3.30E+03			3.30E+03	4.3E-01	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T04-C	1	3.46E+03			3.46E+03	5.1E-01	1.9E+00	6.0E+00					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T05-C	1	3.51E+03			3.51E+03	4.7E-01	1.9E+00	6.0E+00					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T06-C	1	3.53E+03			3.53E+03	4.0E-01	1.9E+00	6.0E+00					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T07-C	1	3.42E+03			3.42E+03	3.1E-01	1.9E+00	6.0E+00					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T08-C	1	2.21E+03			2.21E+03	7.7E-01	1.9E+00	6.0E+00					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-T09-C	1	1.71E+03			1.71E+03	5.2E-01	1.9E+00	6.0E+00					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	1.5E+01	1.9E+00	6.0E+00					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	8.5E+00	1.9E+00	6.0E+00					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	4.7E+00	1.9E+00	6.0E+00					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	EaFA-L11-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	5.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	4.5E+01	2.0E+00	6.4E+00	10	325	3.15E+03	97%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	3.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T04-A	1	6.60E+00			6.60E+00	2.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T05-A	1	2.69E+01			2.69E+01	8.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T06-A	1	2.51E+02			2.51E+02	7.9E-01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T07-A	1	8.82E+02			8.82E+02	6.2E-01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T08-A	1	1.27E+03			1.27E+03	8.1E-01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T09-A	1	1.68E+03			1.68E+03	1.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00	10	325	3.50E+03	108%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	2.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T04-B	1	6.57E+00			6.57E+00	5.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T05-B	1	4.33E+01			4.33E+01	5.4E-01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T06-B	1	2.61E+02			2.61E+02	7.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T07-B	1	8.59E+02			8.59E+02	8.1E-01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T08-B	1	1.29E+03			1.29E+03	1.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T09-B	1	1.66E+03			1.66E+03	3.0E-01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00	10	325	3.44E+03	106%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	2.9E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T04-C	1	7.02E+00			7.02E+00	2.9E+00	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T05-C	1	4.13E+01			4.13E+01	1.1E+00	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T06-C	1	2.59E+02			2.59E+02	7.6E-01	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T07-C	1	8.52E+02			8.52E+02	7.2E-01	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T08-C	1	1.29E+03			1.29E+03	3.0E-01	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-T09-C	1	1.67E+03			1.67E+03	4.8E-01	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	5.1E+01	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	2.4E+01	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	5.2E+01	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	EaFA-L11-1313-T01-A	1	5.00E-01	U1/2		5.00E-01	5.2E+01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T02-A	1	5.00E-01	U1/2		5.00E-01	1.2E+01	1.0E+00	3.2E+00	1000	100	9.37E+02	94%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T03-A	1	1.56E+03			1.56E+03	4.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T04-A	1	4.61E+03			4.61E+03	3.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T05-A	1	5.84E+03			5.84E+03	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T06-A	1	8.00E+03			8.00E+03	1.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T07-A	1	8.28E+03			8.28E+03	7.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T08-A	1	8.82E+03			8.82E+03	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T09-A	1	1.35E+04			1.35E+04	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T01-B	1	5.00E-01	U1/2		5.00E-01	1.3E+02	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T02-B	1	5.00E-01	U1/2		5.00E-01	1.7E+01	1.0E+00	3.2E+00	1000	100	1.04E+03	104%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T03-B	1	1.71E+03			1.71E+03	5.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T04-B	1	4.35E+03			4.35E+03	8.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T05-B	1	6.39E+03			6.39E+03	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T06-B	1	8.03E+03			8.03E+03	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T07-B	1	7.96E+03			7.96E+03	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T08-B	1	8.88E+03			8.88E+03	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T09-B	1	1.35E+04			1.35E+04	7.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T01-C	1	5.00E-01	U1/2		5.00E-01	4.9E+01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T02-C	1	5.00E-01	U1/2		5.00E-01	9.4E+00	1.0E+00	3.2E+00	1000	100	1.05E+03	105%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T03-C	1	1.69E+03			1.69E+03	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T04-C	1	4.62E+03			4.62E+03	7.9E-01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T05-C	1	6.24E+03			6.24E+03	5.3E-01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T06-C	1	7.94E+03			7.94E+03	7.5E-01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T07-C	1	7.93E+03			7.93E+03	5.8E-01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T08-C	1	8.85E+03			8.85E+03	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-T09-C	1	1.33E+04			1.33E+04	6.0E-01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	8.8E+00	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.3E+01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	8.1E+00	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	EaFA-L11-1313-T01-A	1	3.87E+03			3.87E+03	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T02-A	1	3.59E+03			3.59E+03	1.2E+00	1.2E+00	3.8E+00	10	325	6.41E+03	87%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T03-A	1	3.08E+03			3.08E+03	4.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T04-A	1	2.86E+03			2.86E+03	4.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T05-A	1	2.68E+03			2.68E+03	9.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T06-A	1	2.32E+03			2.32E+03	6.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T07-A	1	4.93E+02			4.93E+02	1.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T08-A	1	7.69E+01			7.69E+01	4.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T09-A	1	4.54E+02			4.54E+02	1.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T01-B	1	3.83E+03			3.83E+03	2.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T02-B	1	3.67E+03			3.67E+03	1.2E+00	1.2E+00	3.8E+00	10	325	6.85E+03	98%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T03-B	1	3.19E+03			3.19E+03	3.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T04-B	1	2.93E+03			2.93E+03	6.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T05-B	1	2.74E+03			2.74E+03	5.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T06-B	1	2.31E+03			2.31E+03	4.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T07-B	1	2.23E+02			2.23E+02	3.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T08-B	1	8.56E+01			8.56E+01	2.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T09-B	1	4.52E+02			4.52E+02	9.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T01-C	1	3.74E+03			3.74E+03	7.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T02-C	1	3.74E+03			3.74E+03	2.2E-01	1.2E+00	3.8E+00	10	325	6.87E+03	96%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T03-C	1	3.19E+03			3.19E+03	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T04-C	1	2.95E+03			2.95E+03	1.0E+00	1.2E+00	3.8E+00					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T05-C	1	2.72E+03			2.72E+03	2.8E-01	1.2E+00	3.8E+00					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T06-C	1	2.28E+03			2.28E+03	5.9E-01	1.2E+00	3.8E+00					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T07-C	1	2.09E+02			2.09E+02	1.6E+00	1.2E+00	3.8E+00					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T08-C	1	8.25E+01			8.25E+01	4.5E+00	1.2E+00	3.8E+00					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-T09-C	1	4.55E+02			4.55E+02	1.4E+00	1.2E+00	3.8E+00					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-B01-A	1	1.71E+00	E		1.71E+00	1.4E+02	1.2E+00	3.8E+00					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-B02-A	1	1.23E+00	E		1.23E+00	2.4E+02	1.2E+00	3.8E+00					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1313-B03-A	1	4.97E+00			4.97E+00	4.2E+00	1.2E+00	3.8E+00					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	EaFA-L11-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	8.8E+01	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	5.5E+01	1.8E+00	5.7E+00	10	325	3.16E+03	97%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	6.2E+01	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	5.2E+02	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T05-A	1	8.56E+00			8.56E+00	5.6E+01	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T06-A	1	8.40E+01			8.40E+01	1.5E+00	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T07-A	1	5.92E+02			5.92E+02	1.1E+00	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T08-A	1	5.04E+02			5.04E+02	1.1E+00	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T09-A	1	7.20E+02			7.20E+02	8.0E-01	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	6.8E+01	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	8.9E+01	1.8E+00	5.7E+00	10	325	3.53E+03	108%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	6.0E+01	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T04-B	1	2.53E+00	E		2.53E+00	1.1E+02	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T05-B	1	1.56E+01			1.56E+01	3.4E+01	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T06-B	1	8.63E+01			8.63E+01	6.2E+00	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T07-B	1	6.04E+02			6.04E+02	1.4E+00	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T08-B	1	5.34E+02			5.34E+02	1.8E+00	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T09-B	1	7.17E+02			7.17E+02	9.8E-02	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	4.3E+02	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	2.1E+02	1.8E+00	5.7E+00	10	325	3.49E+03	107%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	3.4E+01	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	1.1E+03	1.8E+00	5.7E+00					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T05-C	1	1.09E+01			1.09E+01	6.0E+01	1.8E+00	5.7E+00					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T06-C	1	8.57E+01			8.57E+01	2.1E+00	1.8E+00	5.7E+00					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T07-C	1	6.01E+02			6.01E+02	8.8E-02	1.8E+00	5.7E+00					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T08-C	1	5.36E+02			5.36E+02	8.7E-01	1.8E+00	5.7E+00					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-T09-C	1	7.15E+02			7.15E+02	8.2E-01	1.8E+00	5.7E+00					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	9.8E+01	1.8E+00	5.7E+00					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	4.9E+01	1.8E+00	5.7E+00					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	7.3E+01	1.8E+00	5.7E+00					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	EaFA-L11-1313-T01-A	1	1.04E+02			1.04E+02	4.7E+00	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T02-A	1	9.21E+01			9.21E+01	8.5E+00	3.7E+00	1.2E+01	1000	100	1.14E+03	104%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T03-A	1	8.05E+01			8.05E+01	2.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T04-A	1	7.25E+01			7.25E+01	1.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T05-A	1	1.02E+02			1.02E+02	6.9E+00	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T06-A	1	7.09E+01			7.09E+01	9.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T07-A	1	6.05E+01			6.05E+01	2.9E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T08-A	1	4.87E+01			4.87E+01	9.1E+00	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T09-A	1	3.92E+03			3.92E+03	2.9E-01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T01-B	1	7.58E+01			7.58E+01	9.6E+00	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T02-B	1	1.08E+02			1.08E+02	4.8E+00	3.7E+00	1.2E+01	1000	100	1.21E+03	111%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T03-B	1	1.03E+02			1.03E+02	1.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T04-B	1	6.43E+01			6.43E+01	2.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T05-B	1	6.55E+01			6.55E+01	1.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T06-B	1	8.38E+01			8.38E+01	2.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T07-B	1	3.96E+01			3.96E+01	3.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T08-B	1	7.12E+01			7.12E+01	1.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T09-B	1	4.17E+03			4.17E+03	4.3E-01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T01-C	1	1.29E+02			1.29E+02	8.3E+00	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T02-C	1	1.53E+02			1.53E+02	4.0E+00	3.7E+00	1.2E+01	1000	100	1.20E+03	104%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T03-C	1	1.14E+02			1.14E+02	1.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T04-C	1	1.28E+02			1.28E+02	1.4E+01	3.7E+00	1.2E+01					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T05-C	1	1.02E+02			1.02E+02	4.2E+00	3.7E+00	1.2E+01					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T06-C	1	5.76E+01			5.76E+01	1.3E+01	3.7E+00	1.2E+01					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T07-C	1	5.23E+01			5.23E+01	1.4E+01	3.7E+00	1.2E+01					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T08-C	1	5.89E+01			5.89E+01	9.7E+00	3.7E+00	1.2E+01					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-T09-C	1	4.17E+03			4.17E+03	1.1E+00	3.7E+00	1.2E+01					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-B01-A	1	1.19E+01			1.19E+01	5.0E+01	3.7E+00	1.2E+01					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-B02-A	1	2.42E+01			2.42E+01	3.6E+01	3.7E+00	1.2E+01					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1313-B03-A	1	7.17E+01			7.17E+01	3.1E+01	3.7E+00	1.2E+01					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	EaFA-L11-1313-T01-A	1	3.84E+04			3.84E+04	1.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T02-A	1	3.09E+04			3.09E+04	1.5E+00	1.6E+00	5.1E+00	1000	100	3.18E+04	86%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T03-A	1	1.66E+04			1.66E+04	2.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T04-A	1	1.45E+04			1.45E+04	1.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T05-A	1	1.39E+04			1.39E+04	9.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T06-A	1	1.61E+04			1.61E+04	2.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T07-A	1	2.53E+04			2.53E+04	1.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T08-A	1	1.68E+04			1.68E+04	8.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T09-A	1	1.99E+04			1.99E+04	8.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T01-B	1	3.88E+04			3.88E+04	1.4E+00	1.6E+00	5.1E+00				---	VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T02-B	1	3.07E+04			3.07E+04	4.3E-01	1.6E+00	5.1E+00	1000	100	3.16E+04	90%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T03-B	1	1.82E+04			1.82E+04	1.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T04-B	1	1.64E+04			1.64E+04	3.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T05-B	1	1.56E+04			1.56E+04	4.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T06-B	1	1.61E+04			1.61E+04	3.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T07-B	1	2.32E+04			2.32E+04	1.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T08-B	1	1.73E+04			1.73E+04	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T09-B	1	2.00E+04			2.00E+04	2.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T01-C	1	3.77E+04			3.77E+04	3.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T02-C	1	3.06E+04			3.06E+04	1.5E+00	1.6E+00	5.1E+00	1000	100	3.15E+04	91%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T03-C	1	1.83E+04			1.83E+04	3.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T04-C	1	1.63E+04			1.63E+04	6.6E-01	1.6E+00	5.1E+00					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T05-C	1	1.56E+04			1.56E+04	3.9E-01	1.6E+00	5.1E+00					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T06-C	1	1.59E+04			1.59E+04	5.8E-01	1.6E+00	5.1E+00					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T07-C	1	2.32E+04			2.32E+04	1.5E-01	1.6E+00	5.1E+00					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T08-C	1	1.71E+04			1.71E+04	7.6E-01	1.6E+00	5.1E+00					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-T09-C	1	1.97E+04			1.97E+04	3.1E-01	1.6E+00	5.1E+00					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-B01-A	1	6.48E+01			6.48E+01	3.2E+00	1.6E+00	5.1E+00					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-B02-A	1	3.94E+01			3.94E+01	6.0E+00	1.6E+00	5.1E+00					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1313-B03-A	1	5.18E+02			5.18E+02	1.4E+00	1.6E+00	5.1E+00					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	EaFA-L11-1313-T01-A	1	6.76E+03			6.76E+03	2.8E-01	1.5E+01	4.8E+01				---	VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T02-A	1	6.24E+03			6.24E+03	1.6E+00	1.5E+01	4.8E+01	10	325	8.91E+03	82%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T03-A	1	4.36E+03			4.36E+03	1.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T04-A	1	1.84E+03			1.84E+03	2.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T05-A	1	1.05E+03			1.05E+03	2.2E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T06-A	1	5.35E+02			5.35E+02	6.0E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T07-A	1	2.48E+02			2.48E+02	6.0E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T08-A	1	6.46E+01			6.46E+01	2.6E+01	1.5E+01	4.8E+01				---	VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T09-A	1	1.08E+03			1.08E+03	2.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T01-B	1	7.04E+03			7.04E+03	2.2E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T02-B	1	6.28E+03			6.28E+03	4.4E-01	1.5E+01	4.8E+01	10	325	9.22E+03	91%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T03-B	1	4.64E+03			4.64E+03	8.9E-01	1.5E+01	4.8E+01				---	VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T04-B	1	1.79E+03			1.79E+03	1.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T05-B	1	9.89E+02			9.89E+02	6.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T06-B	1	5.84E+02			5.84E+02	3.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T07-B	1	2.21E+02			2.21E+02	7.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T08-B	1	6.68E+01			6.68E+01	7.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T09-B	1	1.15E+03			1.15E+03	2.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T01-C	1	6.84E+03			6.84E+03	1.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T02-C	1	6.32E+03			6.32E+03	1.3E+00	1.5E+01	4.8E+01	10	325	9.22E+03	89%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T03-C	1	4.64E+03			4.64E+03	5.4E-01	1.5E+01	4.8E+01				---	VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T04-C	1	1.80E+03			1.80E+03	2.0E+00	1.5E+01	4.8E+01					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T05-C	1	9.98E+02			9.98E+02	1.6E+00	1.5E+01	4.8E+01					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T06-C	1	5.37E+02			5.37E+02	4.8E+00	1.5E+01	4.8E+01					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T07-C	1	2.08E+02			2.08E+02	1.3E+01	1.5E+01	4.8E+01					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T08-C	1	6.95E+01			6.95E+01	3.6E+01	1.5E+01	4.8E+01					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-T09-C	1	1.18E+03			1.18E+03	2.1E+00	1.5E+01	4.8E+01					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-B01-A	1	7.50E+00	U1/2		7.50E+00	3.3E+02	1.5E+01	4.8E+01					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-B02-A	1	1.67E+01	E		1.67E+01	4.3E+01	1.5E+01	4.8E+01					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1313-B03-A	1	3.05E+01	E		3.05E+01	3.1E+01	1.5E+01	4.8E+01					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	EaFA-L11-1313-T01-A	1	1.10E+04			1.10E+04	6.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T02-A	1	3.50E+03			3.50E+03	1.6E+00	1.1E+00	3.5E+00	1000	100	4.39E+03	89%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T03-A	1	2.39E+02			2.39E+02	6.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T04-A	1	3.31E+02			3.31E+02	1.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T05-A	1	5.86E+02			5.86E+02	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T06-A	1	1.63E+03			1.63E+03	2.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T07-A	1	6.41E+03			6.41E+03	1.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T08-A	1	3.02E+04			3.02E+04	1.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T09-A	1	6.84E+04			6.84E+04	8.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T01-B	1	9.93E+03			9.93E+03	6.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T02-B	1	4.93E+03			4.93E+03	9.0E-01	1.1E+00	3.5E+00	1000	100	5.87E+03	93%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T03-B	1	3.26E+02			3.26E+02	2.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T04-B	1	3.79E+02			3.79E+02	1.4E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T05-B	1	7.44E+02			7.44E+02	8.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T06-B	1	1.68E+03			1.68E+03	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T07-B	1	6.43E+03			6.43E+03	1.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T08-B	1	3.32E+04			3.32E+04	7.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T09-B	1	6.80E+04			6.80E+04	4.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T01-C	1	9.56E+03			9.56E+03	1.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T02-C	1	4.98E+03			4.98E+03	7.7E-01	1.1E+00	3.5E+00	1000	100	5.87E+03	88%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T03-C	1	3.05E+02			3.05E+02	1.7E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T04-C	1	4.47E+02			4.47E+02	7.6E-01	1.1E+00	3.5E+00					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T05-C	1	7.17E+02			7.17E+02	6.8E-01	1.1E+00	3.5E+00					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T06-C	1	1.73E+03			1.73E+03	2.4E-01	1.1E+00	3.5E+00					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T07-C	1	6.37E+03			6.37E+03	3.7E-01	1.1E+00	3.5E+00					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T08-C	1	3.33E+04			3.33E+04	1.7E-01	1.1E+00	3.5E+00					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-T09-C	1	6.80E+04			6.80E+04	7.0E-01	1.1E+00	3.5E+00					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-B01-A	1	1.23E+01			1.23E+01	3.3E+01	1.1E+00	3.5E+00					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-B02-A	1	1.88E+01			1.88E+01	2.5E+01	1.1E+00	3.5E+00					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1313-B03-A	1	3.04E+03			3.04E+03	2.1E+00	1.1E+00	3.5E+00					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	EaFA-L11-1313-T01-A	1	2.25E+05			2.25E+05	1.8E-01	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T02-A	1	1.27E+05			1.27E+05	8.5E-01	2.5E+00	8.0E+00	1000	100	1.28E+05	85%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T03-A	1	3.45E+04			3.45E+04	4.3E-01	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T04-A	1	1.18E+04			1.18E+04	1.0E-01	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T05-A	1	4.06E+03			4.06E+03	1.0E+00	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T06-A	1	4.14E+03			4.14E+03	1.3E+00	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T07-A	1	4.47E+03			4.47E+03	5.4E-01	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T08-A	1	2.72E+03			2.72E+03	1.3E+00	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T09-A	1	2.53E+03			2.53E+03	7.0E-01	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T01-B	1	2.20E+05			2.20E+05	1.4E+00	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T02-B	1	1.25E+05			1.25E+05	5.2E-01	2.5E+00	8.0E+00	1000	100	1.26E+05	90%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T03-B	1	3.55E+04			3.55E+04	2.4E-01	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T04-B	1	1.21E+04			1.21E+04	1.0E+00	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T05-B	1	4.15E+03			4.15E+03	3.7E-01	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T06-B	1	4.13E+03			4.13E+03	2.3E+00	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T07-B	1	4.00E+03			4.00E+03	1.6E+00	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T08-B	1	2.80E+03			2.80E+03	1.3E+00	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T09-B	1	2.53E+03			2.53E+03	2.1E-01	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T01-C	1	2.16E+05			2.16E+05	2.4E-01	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T02-C	1	1.25E+05			1.25E+05	4.4E-01	2.5E+00	8.0E+00	1000	100	1.26E+05	91%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T03-C	1	3.58E+04			3.58E+04	5.4E-01	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T04-C	1	1.21E+04			1.21E+04	3.4E-01	2.5E+00	8.0E+00					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T05-C	1	4.10E+03			4.10E+03	5.4E-01	2.5E+00	8.0E+00					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T06-C	1	4.12E+03			4.12E+03	8.8E-01	2.5E+00	8.0E+00					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T07-C	1	4.01E+03			4.01E+03	4.6E-01	2.5E+00	8.0E+00					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T08-C	1	2.79E+03			2.79E+03	2.0E-01	2.5E+00	8.0E+00					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-T09-C	1	2.50E+03			2.50E+03	9.1E-01	2.5E+00	8.0E+00					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-B01-A	1	3.75E+01			3.75E+01	1.8E+00	2.5E+00	8.0E+00					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-B02-A	1	4.59E+01			4.59E+01	1.9E+00	2.5E+00	8.0E+00					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1313-B03-A	1	2.25E+05			2.25E+05	3.5E-01	2.5E+00	8.0E+00					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	EaFA-L11-1313-T01-A	1	1.09E+03			1.09E+03	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T02-A	1	1.60E+03			1.60E+03	1.3E+00	1.0E+00	3.2E+00	1000	100	2.41E+03	81%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T03-A	1	1.45E+03			1.45E+03	2.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T04-A	1	1.64E+03			1.64E+03	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T05-A	1	1.78E+03			1.78E+03	1.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T06-A	1	2.07E+03			2.07E+03	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T07-A	1	2.54E+03			2.54E+03	4.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T08-A	1	3.66E+03			3.66E+03	1.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T09-A	1	5.27E+03			5.27E+03	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T01-B	1	1.15E+03			1.15E+03	4.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T02-B	1	1.45E+03			1.45E+03	1.3E+00	1.0E+00	3.2E+00	1000	100	2.38E+03	93%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T03-B	1	1.61E+03			1.61E+03	6.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T04-B	1	1.76E+03			1.76E+03	7.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T05-B	1	1.93E+03			1.93E+03	6.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T06-B	1	2.10E+03			2.10E+03	2.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T07-B	1	2.47E+03			2.47E+03	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T08-B	1	3.72E+03			3.72E+03	8.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T09-B	1	5.24E+03			5.24E+03	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T01-C	1	1.13E+03			1.13E+03	2.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T02-C	1	1.45E+03			1.45E+03	4.4E-01	1.0E+00	3.2E+00	1000	100	2.37E+03	92%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T03-C	1	1.58E+03			1.58E+03	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T04-C	1	1.79E+03			1.79E+03	5.7E-01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T05-C	1	1.90E+03			1.90E+03	3.0E-01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T06-C	1	2.07E+03			2.07E+03	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T07-C	1	2.44E+03			2.44E+03	1.5E+00	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T08-C	1	3.72E+03			3.72E+03	9.2E-01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-T09-C	1	5.31E+03			5.31E+03	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.0E+02	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-B02-A	1	3.07E+00	E		3.07E+00	1.8E+01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1313-B03-A	1	2.20E+00	E		2.20E+00	6.0E+01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	EaFA-L11-1313-T01-A	1	1.70E+05			1.70E+05	8.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T02-A	1	1.63E+05			1.63E+05	1.3E+00	6.8E+00	2.2E+01	1000	100	1.64E+05	84%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T03-A	1	1.44E+05			1.44E+05	3.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T04-A	1	1.41E+05			1.41E+05	3.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T05-A	1	1.40E+05			1.40E+05	7.8E-01	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T06-A	1	1.44E+05			1.44E+05	3.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T07-A	1	1.53E+05			1.53E+05	5.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T08-A	1	8.69E+04			8.69E+04	5.7E-01	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T09-A	1	6.66E+04			6.66E+04	4.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T01-B	1	1.72E+05			1.72E+05	1.6E+00	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T02-B	1	1.68E+05			1.68E+05	5.1E-01	6.8E+00	2.2E+01	1000	100	1.69E+05	92%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T03-B	1	1.49E+05			1.49E+05	2.8E-01	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T04-B	1	1.46E+05			1.46E+05	1.1E+00	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T05-B	1	1.47E+05			1.47E+05	5.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T06-B	1	1.44E+05			1.44E+05	4.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T07-B	1	1.40E+05			1.40E+05	1.3E+00	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T08-B	1	9.49E+04			9.49E+04	1.2E+00	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T09-B	1	6.67E+04			6.67E+04	1.3E-01	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T01-C	1	1.68E+05			1.68E+05	4.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T02-C	1	1.68E+05			1.68E+05	7.5E-01	6.8E+00	2.2E+01	1000	100	1.69E+05	88%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T03-C	1	1.51E+05			1.51E+05	3.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T04-C	1	1.48E+05			1.48E+05	5.3E-01	6.8E+00	2.2E+01					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T05-C	1	1.45E+05			1.45E+05	7.1E-01	6.8E+00	2.2E+01					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T06-C	1	1.43E+05			1.43E+05	8.7E-01	6.8E+00	2.2E+01					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T07-C	1	1.39E+05			1.39E+05	4.8E-01	6.8E+00	2.2E+01					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T08-C	1	9.49E+04			9.49E+04	4.5E-01	6.8E+00	2.2E+01					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-T09-C	1	6.72E+04			6.72E+04	2.0E-01	6.8E+00	2.2E+01					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-B01-A	1	2.44E+01			2.44E+01	4.9E+01	6.8E+00	2.2E+01					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-B02-A	1	2.60E+01			2.60E+01	2.1E+01	6.8E+00	2.2E+01					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1313-B03-A	1	7.90E+01			7.90E+01	2.2E+01	6.8E+00	2.2E+01					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	EaFA-L11-1313-T01-A	1	2.30E+00	U1/2		2.30E+00	3.9E+02	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T02-A	1	2.30E+00	U1/2		2.30E+00	7.8E+02	4.6E+00	1.5E+01	10	325	3.02E+03	93%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T03-A	1	2.30E+00	U1/2		2.30E+00	8.7E+01	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T04-A	1	2.30E+00	U1/2		2.30E+00	3.4E+02	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T05-A	1	2.30E+00	U1/2		2.30E+00	7.5E+01	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T06-A	1	2.30E+00	U1/2		2.30E+00	9.4E+01	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T07-A	1	3.70E+01			3.70E+01	3.8E+01	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T08-A	1	2.60E+01			2.60E+01	1.8E+01	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T09-A	1	7.59E+01			7.59E+01	4.7E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T01-B	1	2.30E+00	U1/2		2.30E+00	8.6E+01	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T02-B	1	2.30E+00	U1/2		2.30E+00	9.5E+01	4.6E+00	1.5E+01	10	325	3.34E+03	103%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T03-B	1	2.30E+00	U1/2		2.30E+00	7.7E+01	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T04-B	1	2.30E+00	U1/2		2.30E+00	5.3E+01	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T05-B	1	2.30E+00	U1/2		2.30E+00	8.2E+01	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T06-B	1	2.30E+00	U1/2		2.30E+00	1.7E+02	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T07-B	1	2.55E+01			2.55E+01	2.4E+01	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T08-B	1	4.58E+01			4.58E+01	6.1E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T09-B	1	5.59E+01			5.59E+01	1.3E+01	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T01-C	1	2.30E+00	U1/2		2.30E+00	1.5E+02	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T02-C	1	2.30E+00	U1/2		2.30E+00	2.7E+02	4.6E+00	1.5E+01	10	325	3.28E+03	101%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T03-C	1	2.30E+00	U1/2		2.30E+00	5.3E+01	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T04-C	1	2.30E+00	U1/2		2.30E+00	1.0E+03	4.6E+00	1.5E+01					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T05-C	1	2.30E+00	U1/2		2.30E+00	1.7E+02	4.6E+00	1.5E+01					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T06-C	1	7.79E+00	E		7.79E+00	7.0E+01	4.6E+00	1.5E+01					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T07-C	1	4.04E+01			4.04E+01	5.9E+01	4.6E+00	1.5E+01					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T08-C	1	4.85E+01			4.85E+01	7.5E-01	4.6E+00	1.5E+01					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-T09-C	1	7.13E+01			7.13E+01	1.1E+00	4.6E+00	1.5E+01					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	4.3E+01	4.6E+00	1.5E+01					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	5.7E+01	4.6E+00	1.5E+01					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	1.5E+02	4.6E+00	1.5E+01					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	EaFA-L11-1313-T01-A	1	3.35E+00	E		3.35E+00	9.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00	10	325	3.20E+03	98%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	6.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	5.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	6.9E+02	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	9.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T07-A	1	2.41E+00	E		2.41E+00	2.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T08-A	1	1.56E+01			1.56E+01	6.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T09-A	1	5.87E+03			5.87E+03	7.9E-01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T01-B	1	2.12E+00	E		2.12E+00	6.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	2.8E+02	2.0E+00	6.4E+00	10	325	3.48E+03	107%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	2.7E+02	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	2.2E+03	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	4.3E+02	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	2.1E+02	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	3.4E+02	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T08-B	1	2.38E+01			2.38E+01	3.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T09-B	1	6.11E+03			6.11E+03	4.2E-01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T01-C	1	4.20E+00	E		4.20E+00	1.9E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	8.6E+02	2.0E+00	6.4E+00	10	325	3.40E+03	104%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	1.1E+03	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	3.8E+02	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	3.9E+01	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	2.2E+02	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T08-C	1	2.24E+01			2.24E+01	2.0E+00	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-T09-C	1	6.09E+03			6.09E+03	1.7E-01	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-B02-A	1	2.12E+00	E		2.12E+00	2.7E+01	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1313-B03-A	1	2.38E+00	E		2.38E+00	3.1E+00	2.0E+00	6.4E+00					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	EaFA-L11-1313-T01-A	1	4.18E+03			4.18E+03	1.6E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T02-A	1	2.52E+03			2.52E+03	1.0E+00	1.5E+00	4.8E+00	10	325	5.43E+03	90%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T03-A	1	5.52E+02			5.52E+02	4.3E-01	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T04-A	1	1.92E+02			1.92E+02	1.5E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T05-A	1	1.36E+02			1.36E+02	5.4E-01	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T06-A	1	1.05E+02			1.05E+02	1.3E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T07-A	1	9.00E+01			9.00E+01	4.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T08-A	1	9.14E+01			9.14E+01	2.5E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T09-A	1	6.15E+03			6.15E+03	5.1E-01	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T01-B	1	3.82E+03			3.82E+03	7.8E-01	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T02-B	1	2.77E+03			2.77E+03	9.6E-01	1.5E+00	4.8E+00	10	325	6.05E+03	101%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T03-B	1	6.97E+02			6.97E+02	2.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T04-B	1	1.90E+02			1.90E+02	2.6E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T05-B	1	1.43E+02			1.43E+02	3.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T06-B	1	1.03E+02			1.03E+02	1.6E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T07-B	1	7.18E+01			7.18E+01	1.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T08-B	1	1.15E+02			1.15E+02	7.2E-01	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T09-B	1	6.11E+03			6.11E+03	1.4E-01	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T01-C	1	3.77E+03			3.77E+03	7.5E-01	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T02-C	1	2.87E+03			2.87E+03	4.8E-01	1.5E+00	4.8E+00	10	325	6.06E+03	98%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T03-C	1	6.71E+02			6.71E+02	4.1E-01	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T04-C	1	1.88E+02			1.88E+02	1.0E+00	1.5E+00	4.8E+00					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T05-C	1	1.37E+02			1.37E+02	1.0E+00	1.5E+00	4.8E+00					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T06-C	1	1.04E+02			1.04E+02	3.0E+00	1.5E+00	4.8E+00					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T07-C	1	7.23E+01			7.23E+01	3.9E+00	1.5E+00	4.8E+00					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T08-C	1	1.12E+02			1.12E+02	2.4E+00	1.5E+00	4.8E+00					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-T09-C	1	6.11E+03			6.11E+03	1.1E+00	1.5E+00	4.8E+00					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-B01-A	1	3.78E+00	E		3.78E+00	2.2E+01	1.5E+00	4.8E+00					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-B02-A	1	5.39E+00			5.39E+00	3.8E+01	1.5E+00	4.8E+00					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1313-B03-A	1	1.48E+01			1.48E+01	4.0E+00	1.5E+00	4.8E+00					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	EaFA-L11-1313-T01-A	1	2.25E+01			2.25E+01	6.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:12 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T02-A	1	8.15E+00			8.15E+00	1.7E+01	1.0E+00	3.2E+00	10	325	3.25E+03	100%	VU ICP-OES	2/22/11 2:14 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T03-A	1	1.14E+01			1.14E+01	3.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:15 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T04-A	1	1.58E+01			1.58E+01	3.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:17 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T05-A	1	2.42E+00	E		2.42E+00	2.1E+01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:19 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T06-A	1	5.27E+00			5.27E+00	1.7E+01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:20 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T07-A	1	1.21E+03			1.21E+03	6.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:22 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T08-A	1	8.80E+02			8.80E+02	7.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:23 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T09-A	1	1.51E+03			1.51E+03	5.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:25 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T01-B	1	2.43E+01			2.43E+01	5.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:32 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T02-B	1	8.94E+00			8.94E+00	1.1E+01	1.0E+00	3.2E+00	10	325	3.62E+03	111%	VU ICP-OES	2/22/11 2:33 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T03-B	1	1.67E+00	E		1.67E+00	3.7E+01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:35 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T04-B	1	1.19E+01			1.19E+01	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:37 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T05-B	1	5.00E-01	U1/2		5.00E-01	1.3E+02	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:38 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T06-B	1	7.86E+00			7.86E+00	8.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:40 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T07-B	1	1.30E+03			1.30E+03	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:42 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T08-B	1	1.17E+03			1.17E+03	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:43 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T09-B	1	1.50E+03			1.50E+03	5.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:45 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T01-C	1	2.64E+01			2.64E+01	6.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:47 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T02-C	1	4.57E+00			4.57E+00	3.0E+01	1.0E+00	3.2E+00	10	325	3.57E+03	110%	VU ICP-OES	2/22/11 2:48 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T03-C	1	5.00E-01	U1/2		5.00E-01	1.6E+02	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 2:50 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T04-C	1	4.81E+00			4.81E+00	2.9E+01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:51 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T05-C	1	1.08E+00	E		1.08E+00	2.1E+01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:53 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T06-C	1	6.77E+00			6.77E+00	1.6E+01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:55 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T07-C	1	1.29E+03			1.29E+03	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:56 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T08-C	1	1.17E+03			1.17E+03	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:58 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-T09-C	1	1.51E+03			1.51E+03	3.2E-01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 3:00 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-B01-A	1	3.31E+00			3.31E+00	6.5E+00	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:07 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-B02-A	1	5.22E+00			5.22E+00	2.2E+01	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:09 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1313-B03-A	1	1.20E+00	E		1.20E+00	2.0E+02	1.0E+00	3.2E+00					VU ICP-OES	2/22/11 2:10 PM	EPA Interlab L11 1313-1316 EaFA

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	EaFA-LRef-1313-T01-A	1	3.70E+04			3.70E+04	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T02-A	1	3.38E+04			3.38E+04	4.6E-01	1.0E+00	3.2E+00	1000	100	3.49E+04	113%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T03-A	1	2.71E+04			2.71E+04	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T04-A	1	1.77E+04			1.77E+04	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T05-A	1	1.21E+03			1.21E+03	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T06-A	1	2.02E+02			2.02E+02	3.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T07-A	1	3.35E+02			3.35E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T08-A	1	3.20E+04			3.20E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T09-A	1	1.28E+05			1.28E+05	8.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T01-B	1	3.53E+04			3.53E+04	9.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T02-B	1	3.24E+04			3.24E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T03-B	1	2.85E+04			2.85E+04	8.4E-01	1.0E+00	3.2E+00	1000	100	2.94E+04	93%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T04-B	1	1.54E+04			1.54E+04	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T05-B	1	1.14E+03			1.14E+03	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T06-B	1	2.24E+02			2.24E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T07-B	1	1.58E+02			1.58E+02	2.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T08-B	1	3.14E+04			3.14E+04	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T09-B	1	1.25E+05			1.25E+05	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T01-C	1	3.68E+04			3.68E+04	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T02-C	1	3.51E+04			3.51E+04	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T03-C	1	2.63E+04			2.63E+04	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T04-C	1	1.41E+04			1.41E+04	4.0E-01	1.0E+00	3.2E+00	1000	100	1.50E+04	93%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T05-C	1	1.08E+03			1.08E+03	6.5E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T06-C	1	2.60E+02			2.60E+02	1.7E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T07-C	1	2.95E+02			2.95E+02	2.0E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T08-C	1	3.05E+04			3.05E+04	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-T09-C	1	1.27E+05			1.27E+05	7.5E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-B02-A	1	3.99E+01			3.99E+01	3.7E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-B03-A	1	1.62E+03			1.62E+03	4.3E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	5.9E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-B02-B	1	4.08E+01			4.08E+01	8.5E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-B03-B	1	1.53E+03			1.53E+03	6.6E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	1.5E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-B02-C	1	1.55E+01			1.55E+01	4.4E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1313-B03-C	1	4.88E+02			4.88E+02	5.5E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	EaFA-LRef-1313-T01-A	1	1.81E+02			1.81E+02	9.0E+00	7.5E+00	2.4E+01			---		VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T02-A	1	1.47E+02			1.47E+02	1.1E+01	7.5E+00	2.4E+01	10	325	3.18E+03	93%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T03-A	1	1.43E+02			1.43E+02	9.4E+00	7.5E+00	2.4E+01			---		VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T04-A	1	1.26E+02			1.26E+02	1.5E+00	7.5E+00	2.4E+01			---		VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T05-A	1	1.38E+02			1.38E+02	1.2E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T06-A	1	1.48E+02			1.48E+02	2.0E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T07-A	1	8.78E+01			8.78E+01	4.5E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T08-A	1	3.71E+01			3.71E+01	1.7E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T09-A	1	3.75E+00	U1/2		3.75E+00	3.8E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T01-B	1	1.65E+02			1.65E+02	9.1E+00	7.5E+00	2.4E+01			---		VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T02-B	1	1.29E+02			1.29E+02	2.2E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T03-B	1	1.30E+02			1.30E+02	2.4E+00	7.5E+00	2.4E+01	10	325	3.12E+03	92%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T04-B	1	1.16E+02			1.16E+02	1.1E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T05-B	1	1.35E+02			1.35E+02	2.7E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T06-B	1	1.28E+02			1.28E+02	7.1E+00	7.5E+00	2.4E+01			---		VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T07-B	1	7.61E+01			7.61E+01	2.1E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T08-B	1	1.05E+01	E		1.05E+01	1.7E+02	7.5E+00	2.4E+01			---		VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T09-B	1	3.75E+00	U1/2		3.75E+00	7.0E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T01-C	1	1.93E+02			1.93E+02	1.7E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T02-C	1	1.50E+02			1.50E+02	7.2E+00	7.5E+00	2.4E+01			---		VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T03-C	1	1.47E+02			1.47E+02	5.4E+00	7.5E+00	2.4E+01			---		VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T04-C	1	1.55E+02			1.55E+02	1.6E+01	7.5E+00	2.4E+01	10	325	3.14E+03	92%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T05-C	1	1.35E+02			1.35E+02	3.0E+01	7.5E+00	2.4E+01					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T06-C	1	1.17E+02			1.17E+02	2.3E+01	7.5E+00	2.4E+01					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T07-C	1	5.60E+01			5.60E+01	3.8E+01	7.5E+00	2.4E+01					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T08-C	1	1.81E+01	E		1.81E+01	4.0E+01	7.5E+00	2.4E+01					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-T09-C	1	3.75E+00	U1/2		3.75E+00	2.4E+01	7.5E+00	2.4E+01					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-B01-A	1	3.75E+00	U1/2		3.75E+00	1.3E+02	7.5E+00	2.4E+01					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-B02-A	1	3.75E+00	U1/2		3.75E+00	1.4E+01	7.5E+00	2.4E+01					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-B03-A	1	3.75E+00	U1/2		3.75E+00	1.1E+02	7.5E+00	2.4E+01					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-B01-B	1	3.75E+00	U1/2		3.75E+00	1.8E+03	7.5E+00	2.4E+01					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-B02-B	1	3.75E+00	U1/2		3.75E+00	1.8E+02	7.5E+00	2.4E+01					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-B03-B	1	3.75E+00	U1/2		3.75E+00	3.3E+02	7.5E+00	2.4E+01					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-B01-C	1	3.75E+00	U1/2		3.75E+00	3.7E+02	7.5E+00	2.4E+01					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-B02-C	1	3.75E+00	U1/2		3.75E+00	4.9E+02	7.5E+00	2.4E+01					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1313-B03-C	1	1.31E+01	E		1.31E+01	6.1E+00	7.5E+00	2.4E+01					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	EaFA-LRef-1313-T01-A	1	9.69E+03			9.69E+03	7.3E-01	1.1E+01	3.5E+01			---		VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T02-A	1	1.01E+03			1.01E+03	3.9E+00	1.1E+01	3.5E+01	10	325	3.92E+03	89%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T03-A	1	1.05E+03			1.05E+03	7.4E-01	1.1E+01	3.5E+01			---		VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T04-A	1	5.60E+02			5.60E+02	5.7E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T05-A	1	1.99E+02			1.99E+02	5.9E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T06-A	1	7.84E+01			7.84E+01	3.4E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T07-A	1	4.17E+01			4.17E+01	3.5E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T08-A	1	9.00E+01			9.00E+01	1.3E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T09-A	1	1.55E+03			1.55E+03	1.4E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T01-B	1	9.88E+03			9.88E+03	1.3E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T02-B	1	9.35E+02			9.35E+02	4.5E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T03-B	1	6.78E+02			6.78E+02	2.0E+00	1.1E+01	3.5E+01	10	325	3.61E+03	90%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T04-B	1	5.35E+02			5.35E+02	2.9E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T05-B	1	1.63E+02			1.63E+02	1.3E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T06-B	1	6.43E+01			6.43E+01	1.9E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T07-B	1	3.93E+01			3.93E+01	1.2E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T08-B	1	9.47E+01			9.47E+01	3.7E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T09-B	1	1.67E+03			1.67E+03	1.0E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T01-C	1	9.25E+03			9.25E+03	8.2E-01	1.1E+01	3.5E+01			---		VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T02-C	1	8.14E+02			8.14E+02	2.1E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T03-C	1	8.66E+02			8.66E+02	2.4E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T04-C	1	4.82E+02			4.82E+02	4.0E+00	1.1E+01	3.5E+01	10	325	3.43E+03	91%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T05-C	1	1.63E+02			1.63E+02	5.3E+00	1.1E+01	3.5E+01					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T06-C	1	7.23E+01			7.23E+01	1.4E+01	1.1E+01	3.5E+01					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T07-C	1	5.57E+01			5.57E+01	2.0E+01	1.1E+01	3.5E+01					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T08-C	1	9.75E+01			9.75E+01	6.5E+00	1.1E+01	3.5E+01					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-T09-C	1	1.36E+03			1.36E+03	1.9E+00	1.1E+01	3.5E+01					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-B01-A	1	5.50E+00	U1/2		5.50E+00	4.3E+02	1.1E+01	3.5E+01					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-B02-A	1	5.50E+00	U1/2		5.50E+00	1.3E+02	1.1E+01	3.5E+01					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-B03-A	1	1.28E+01	E		1.28E+01	1.0E+02	1.1E+01	3.5E+01					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-B01-B	1	5.50E+00	U1/2		5.50E+00	3.3E+01	1.1E+01	3.5E+01					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-B02-B	1	5.50E+00	U1/2		5.50E+00	7.9E+01	1.1E+01	3.5E+01					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-B03-B	1	1.63E+01	E		1.63E+01	7.2E+01	1.1E+01	3.5E+01					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-B01-C	1	5.50E+00	U1/2		5.50E+00	2.6E+02	1.1E+01	3.5E+01					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-B02-C	1	5.50E+00	U1/2		5.50E+00	7.3E+01	1.1E+01	3.5E+01					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1313-B03-C	1	5.50E+00	U1/2		5.50E+00	4.8E+01	1.1E+01	3.5E+01					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	EaFA-LRef-1313-T01-A	1	9.77E+03			9.77E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T02-A	1	4.99E+03			4.99E+03	1.1E+00	1.0E+00	3.2E+00	1000	100	5.90E+03	91%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T03-A	1	4.64E+03			4.64E+03	9.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T04-A	1	4.50E+03			4.50E+03	4.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T05-A	1	4.38E+03			4.38E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T06-A	1	4.62E+03			4.62E+03	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T07-A	1	4.98E+03			4.98E+03	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T08-A	1	3.82E+03			3.82E+03	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T09-A	1	3.25E+03			3.25E+03	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T01-B	1	9.62E+03			9.62E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T02-B	1	5.00E+03			5.00E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T03-B	1	4.49E+03			4.49E+03	1.5E+00	1.0E+00	3.2E+00	1000	100	5.43E+03	94%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T04-B	1	4.31E+03			4.31E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T05-B	1	4.37E+03			4.37E+03	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T06-B	1	4.47E+03			4.47E+03	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T07-B	1	4.87E+03			4.87E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T08-B	1	3.82E+03			3.82E+03	6.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T09-B	1	3.25E+03			3.25E+03	3.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T01-C	1	9.22E+03			9.22E+03	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T02-C	1	4.40E+03			4.40E+03	2.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T03-C	1	4.30E+03			4.30E+03	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T04-C	1	4.31E+03			4.31E+03	1.6E+00	1.0E+00	3.2E+00	1000	100	5.20E+03	88%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T05-C	1	4.27E+03			4.27E+03	2.3E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T06-C	1	4.43E+03			4.43E+03	1.6E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T07-C	1	4.82E+03			4.82E+03	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T08-C	1	3.75E+03			3.75E+03	2.2E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-T09-C	1	3.20E+03			3.20E+03	5.8E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-B01-A	1	2.67E+01			2.67E+01	3.8E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-B02-A	1	5.13E+01			5.13E+01	2.1E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-B03-A	1	5.73E+03			5.73E+03	5.9E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-B01-B	1	2.33E+01			2.33E+01	1.0E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-B02-B	1	4.38E+01			4.38E+01	4.2E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-B03-B	1	5.54E+03			5.54E+03	1.0E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-B01-C	1	2.11E+01			2.11E+01	3.9E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-B02-C	1	4.27E+01			4.27E+01	8.3E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1313-B03-C	1	4.73E+03			4.73E+03	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	EaFA-LRef-1313-T01-A	1	6.59E+02			6.59E+02	5.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T02-A	1	9.21E+02			9.21E+02	6.0E-01	1.0E+00	3.2E+00	10	325	3.73E+03	86%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T03-A	1	9.03E+02			9.03E+02	5.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T04-A	1	5.62E+02			5.62E+02	2.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T05-A	1	2.56E+02			2.56E+02	7.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T06-A	1	2.60E+02			2.60E+02	5.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T07-A	1	2.81E+02			2.81E+02	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T08-A	1	2.20E+02			2.20E+02	9.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T09-A	1	8.76E+02			8.76E+02	4.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T01-B	1	5.35E+02			5.35E+02	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T02-B	1	7.53E+02			7.53E+02	3.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T03-B	1	9.91E+02			9.91E+02	8.5E-01	1.0E+00	3.2E+00	10	325	3.84E+03	88%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T04-B	1	5.51E+02			5.51E+02	7.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T05-B	1	2.76E+02			2.76E+02	6.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T06-B	1	2.46E+02			2.46E+02	5.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T07-B	1	2.82E+02			2.82E+02	6.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T08-B	1	2.20E+02			2.20E+02	6.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T09-B	1	8.61E+02			8.61E+02	4.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T01-C	1	6.69E+02			6.69E+02	5.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T02-C	1	9.25E+02			9.25E+02	7.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T03-C	1	1.05E+03			1.05E+03	2.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T04-C	1	4.55E+02			4.55E+02	3.7E-01	1.0E+00	3.2E+00	10	325	3.16E+03	83%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T05-C	1	2.62E+02			2.62E+02	7.4E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T06-C	1	2.44E+02			2.44E+02	8.6E-02	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T07-C	1	2.66E+02			2.66E+02	1.8E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T08-C	1	2.17E+02			2.17E+02	2.4E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-T09-C	1	8.72E+02			8.72E+02	7.9E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	9.2E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	2.6E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	2.1E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	4.6E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	2.3E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	7.8E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	6.4E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	EaFA-LRef-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	3.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	1.2E+01	1.9E+00	6.0E+00	10	325	3.17E+03	98%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	1.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	3.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	7.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	6.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T07-A	1	9.50E-01	U1/2		9.50E-01	2.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T08-A	1	1.23E+02			1.23E+02	1.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T09-A	1	2.68E+02			2.68E+02	1.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	2.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	1.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	1.3E+01	1.9E+00	6.0E+00	10	325	3.20E+03	99%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	1.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	7.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	1.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T07-B	1	9.50E-01	U1/2		9.50E-01	2.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T08-B	1	1.23E+02			1.23E+02	1.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T09-B	1	2.63E+02			2.63E+02	3.2E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	3.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	6.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	2.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	3.7E+00	1.9E+00	6.0E+00	10	325	3.29E+03	101%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	9.0E+00	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	1.1E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T07-C	1	9.50E-01	U1/2		9.50E-01	3.7E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T08-C	1	1.20E+02			1.20E+02	1.9E+00	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-T09-C	1	2.63E+02			2.63E+02	1.2E+00	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	4.5E+00	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	1.6E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	9.0E+00	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-B01-B	1	9.50E-01	U1/2		9.50E-01	1.7E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-B02-B	1	9.50E-01	U1/2		9.50E-01	6.4E+00	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-B03-B	1	9.50E-01	U1/2		9.50E-01	1.1E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-B01-C	1	9.50E-01	U1/2		9.50E-01	1.2E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-B02-C	1	9.50E-01	U1/2		9.50E-01	3.2E+00	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1313-B03-C	1	9.50E-01	U1/2		9.50E-01	2.0E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	EaFA-LRef-1313-T01-A	1	1.10E+00	U1/2		1.10E+00	1.2E+01	2.2E+00	7.0E+00			---		VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T02-A	1	1.10E+00	U1/2		1.10E+00	2.5E+01	2.2E+00	7.0E+00	10	325	3.25E+03	100%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	1.3E+01	2.2E+00	7.0E+00			---		VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T04-A	1	1.10E+00	U1/2		1.10E+00	2.3E+01	2.2E+00	7.0E+00			---		VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T05-A	1	1.10E+00	U1/2		1.10E+00	1.3E+01	2.2E+00	7.0E+00			---		VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T06-A	1	1.10E+00	U1/2		1.10E+00	3.5E+01	2.2E+00	7.0E+00			---		VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T07-A	1	3.20E+01			3.20E+01	3.9E+00	2.2E+00	7.0E+00			---		VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T08-A	1	2.69E+01			2.69E+01	1.1E+00	2.2E+00	7.0E+00			---		VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T09-A	1	2.93E+01			2.93E+01	2.1E+00	2.2E+00	7.0E+00			---		VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T01-B	1	1.10E+00	U1/2		1.10E+00	5.3E+01	2.2E+00	7.0E+00			---		VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T02-B	1	1.10E+00	U1/2		1.10E+00	4.9E+01	2.2E+00	7.0E+00			---		VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	1.4E+01	2.2E+00	7.0E+00	10	325	3.19E+03	98%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T04-B	1	1.10E+00	U1/2		1.10E+00	9.5E+00	2.2E+00	7.0E+00			---		VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T05-B	1	1.10E+00	U1/2		1.10E+00	3.8E+01	2.2E+00	7.0E+00			---		VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T06-B	1	1.10E+00	U1/2		1.10E+00	5.5E+01	2.2E+00	7.0E+00			---		VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T07-B	1	2.57E+01			2.57E+01	3.8E+00	2.2E+00	7.0E+00			---		VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T08-B	1	2.71E+01			2.71E+01	1.1E+00	2.2E+00	7.0E+00			---		VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T09-B	1	2.94E+01			2.94E+01	2.1E+00	2.2E+00	7.0E+00			---		VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T01-C	1	1.10E+00	U1/2		1.10E+00	6.3E+01	2.2E+00	7.0E+00			---		VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T02-C	1	1.10E+00	U1/2		1.10E+00	1.1E+02	2.2E+00	7.0E+00			---		VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	4.1E+01	2.2E+00	7.0E+00			---		VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T04-C	1	1.10E+00	U1/2		1.10E+00	3.3E+00	2.2E+00	7.0E+00	10	325	3.20E+03	98%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T05-C	1	1.10E+00	U1/2		1.10E+00	2.4E+01	2.2E+00	7.0E+00					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T06-C	1	1.10E+00	U1/2		1.10E+00	1.4E+01	2.2E+00	7.0E+00					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T07-C	1	3.04E+01			3.04E+01	1.2E+00	2.2E+00	7.0E+00					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T08-C	1	2.60E+01			2.60E+01	4.2E+00	2.2E+00	7.0E+00					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-T09-C	1	2.94E+01			2.94E+01	2.3E+00	2.2E+00	7.0E+00					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	5.2E+01	2.2E+00	7.0E+00					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	7.7E+00	2.2E+00	7.0E+00					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-B03-A	1	1.10E+00	U1/2		1.10E+00	2.9E+01	2.2E+00	7.0E+00					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-B01-B	1	1.10E+00	U1/2		1.10E+00	2.3E+01	2.2E+00	7.0E+00					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-B02-B	1	1.10E+00	U1/2		1.10E+00	4.6E+01	2.2E+00	7.0E+00					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-B03-B	1	1.10E+00	U1/2		1.10E+00	2.3E+01	2.2E+00	7.0E+00					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-B01-C	1	1.10E+00	U1/2		1.10E+00	2.4E+01	2.2E+00	7.0E+00					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-B02-C	1	1.10E+00	U1/2		1.10E+00	6.8E+01	2.2E+00	7.0E+00					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1313-B03-C	1	1.10E+00	U1/2		1.10E+00	7.1E+01	2.2E+00	7.0E+00					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	EaFA-LRef-1313-T01-A	1	9.20E+03			9.20E+03	4.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T02-A	1	4.09E+04			4.09E+04	2.4E-01	2.6E+00	8.3E+00	1000	100	4.18E+04	91%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T03-A	1	8.73E+04			8.73E+04	9.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T04-A	1	1.11E+05			1.11E+05	4.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T05-A	1	1.35E+05			1.35E+05	1.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T06-A	1	1.55E+05			1.55E+05	1.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T07-A	1	1.67E+05			1.67E+05	6.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T08-A	1	1.40E+05			1.40E+05	8.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T09-A	1	1.41E+05			1.41E+05	3.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T01-B	1	7.79E+03			7.79E+03	1.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T02-B	1	4.47E+04			4.47E+04	7.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T03-B	1	9.67E+04			9.67E+04	1.0E+00	2.6E+00	8.3E+00	1000	100	9.75E+04	88%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T04-B	1	1.08E+05			1.08E+05	1.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T05-B	1	1.33E+05			1.33E+05	3.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T06-B	1	1.47E+05			1.47E+05	6.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T07-B	1	1.64E+05			1.64E+05	1.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T08-B	1	1.40E+05			1.40E+05	2.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T09-B	1	1.40E+05			1.40E+05	6.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T01-C	1	9.44E+03			9.44E+03	4.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T02-C	1	4.60E+04			4.60E+04	4.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T03-C	1	9.22E+04			9.22E+04	4.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T04-C	1	1.11E+05			1.11E+05	9.7E-01	2.6E+00	8.3E+00	1000	100	1.12E+05	87%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T05-C	1	1.34E+05			1.34E+05	7.7E-01	2.6E+00	8.3E+00					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T06-C	1	1.41E+05			1.41E+05	3.2E-01	2.6E+00	8.3E+00					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T07-C	1	1.56E+05			1.56E+05	1.7E+00	2.6E+00	8.3E+00					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T08-C	1	1.35E+05			1.35E+05	1.1E+00	2.6E+00	8.3E+00					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-T09-C	1	1.38E+05			1.38E+05	3.9E-01	2.6E+00	8.3E+00					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-B01-A	1	2.95E+01			2.95E+01	1.7E+01	2.6E+00	8.3E+00					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-B02-A	1	3.14E+01			3.14E+01	2.0E+01	2.6E+00	8.3E+00					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-B03-A	1	2.45E+01			2.45E+01	5.5E+01	2.6E+00	8.3E+00					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-B01-B	1	3.30E+01			3.30E+01	1.9E+01	2.6E+00	8.3E+00					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-B02-B	1	3.36E+01			3.36E+01	2.0E+01	2.6E+00	8.3E+00					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-B03-B	1	2.33E+01			2.33E+01	6.8E+01	2.6E+00	8.3E+00					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-B01-C	1	2.24E+01			2.24E+01	2.8E+01	2.6E+00	8.3E+00					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-B02-C	1	3.12E+01			3.12E+01	2.8E+01	2.6E+00	8.3E+00					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1313-B03-C	1	1.05E+01			1.05E+01	8.0E+01	2.6E+00	8.3E+00					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	EaFA-LRef-1313-T01-A	1	3.92E+02			3.92E+02	6.9E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T02-A	1	3.06E+02			3.06E+02	7.8E-01	1.2E+00	3.8E+00	10	325	3.30E+03	92%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T03-A	1	2.48E+02			2.48E+02	1.4E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T04-A	1	2.23E+02			2.23E+02	1.0E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T05-A	1	1.34E+02			1.34E+02	1.4E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T06-A	1	4.22E+01			4.22E+01	2.7E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T07-A	1	1.57E+00	E		1.57E+00	1.0E+02	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T08-A	1	1.75E+02			1.75E+02	1.4E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T09-A	1	1.96E+03			1.96E+03	3.7E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T01-B	1	3.69E+02			3.69E+02	8.7E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T02-B	1	2.80E+02			2.80E+02	6.3E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T03-B	1	2.89E+02			2.89E+02	1.1E+00	1.2E+00	3.8E+00	10	325	3.25E+03	91%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T04-B	1	2.10E+02			2.10E+02	1.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T05-B	1	1.33E+02			1.33E+02	9.2E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T06-B	1	5.43E+01			5.43E+01	3.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T07-B	1	6.00E-01	U1/2		6.00E-01	9.6E+01	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T08-B	1	1.71E+02			1.71E+02	7.9E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T09-B	1	1.95E+03			1.95E+03	4.2E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T01-C	1	4.14E+02			4.14E+02	6.4E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T02-C	1	3.26E+02			3.26E+02	1.0E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T03-C	1	2.64E+02			2.64E+02	2.0E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T04-C	1	2.18E+02			2.18E+02	4.6E-01	1.2E+00	3.8E+00	10	325	3.20E+03	92%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T05-C	1	1.37E+02			1.37E+02	5.8E-01	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T06-C	1	6.01E+01			6.01E+01	2.5E+00	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T07-C	1	1.27E+00	E		1.27E+00	2.0E+02	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T08-C	1	1.56E+02			1.56E+02	1.4E+00	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-T09-C	1	1.92E+03			1.92E+03	1.5E-01	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	4.8E+02	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	2.3E+04	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-B03-A	1	6.44E+00			6.44E+00	3.5E+01	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-B01-B	1	6.00E-01	U1/2		6.00E-01	2.2E+02	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-B02-B	1	6.00E-01	U1/2		6.00E-01	8.3E+01	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-B03-B	1	9.49E+00			9.49E+00	4.7E+00	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-B01-C	1	6.00E-01	U1/2		6.00E-01	9.5E+02	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-B02-C	1	6.00E-01	U1/2		6.00E-01	5.2E+01	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1313-B03-C	1	4.16E+00			4.16E+00	3.6E+01	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	EaFA-LRef-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	3.7E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	4.0E+03	1.8E+00	5.7E+00	10	325	3.28E+03	101%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	2.9E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	7.8E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T05-A	1	9.00E-01	U1/2		9.00E-01	8.1E+03	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T06-A	1	2.93E+01			2.93E+01	3.4E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T07-A	1	2.52E+02			2.52E+02	2.2E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T08-A	1	2.14E+02			2.14E+02	2.1E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T09-A	1	4.19E+02			4.19E+02	8.6E-01	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	9.2E+01	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	2.1E+03	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.8E+00	5.7E+00	10	325	3.12E+03	96%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T05-B	1	3.00E+00	E		3.00E+00	6.4E+01	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T06-B	1	2.13E+01			2.13E+01	2.0E+01	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T07-B	1	2.38E+02			2.38E+02	1.7E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T08-B	1	2.14E+02			2.14E+02	1.0E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T09-B	1	4.15E+02			4.15E+02	6.2E-01	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	8.8E+01	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	3.3E+01	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	1.7E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	2.4E+01	1.8E+00	5.7E+00	10	325	3.25E+03	100%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T05-C	1	4.09E+00	E		4.09E+00	8.4E+01	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T06-C	1	2.03E+01			2.03E+01	1.5E+01	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T07-C	1	2.39E+02			2.39E+02	8.5E-01	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T08-C	1	2.06E+02			2.06E+02	1.8E+00	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-T09-C	1	4.20E+02			4.20E+02	2.3E-01	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	8.4E+01	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	3.3E+03	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-B01-B	1	9.00E-01	U1/2		9.00E-01	3.9E+01	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-B02-B	1	9.00E-01	U1/2		9.00E-01	1.9E+02	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-B03-B	1	9.00E-01	U1/2		9.00E-01	2.2E+02	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-B01-C	1	9.00E-01	U1/2		9.00E-01	1.0E+03	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-B02-C	1	9.00E-01	U1/2		9.00E-01	3.7E+02	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1313-B03-C	1	2.59E+00	E		2.59E+00	2.0E+02	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	EaFA-LRef-1313-T01-A	1	2.52E+01			2.52E+01	2.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T02-A	1	1.85E+00	U1/2		1.85E+00	4.1E+02	3.7E+00	1.2E+01	10	325	3.09E+03	95%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T03-A	1	1.85E+00	U1/2		1.85E+00	4.8E+04	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T04-A	1	1.85E+00	U1/2		1.85E+00	3.6E+02	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T05-A	1	1.85E+00	U1/2		1.85E+00	1.3E+02	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T06-A	1	1.85E+00	U1/2		1.85E+00	1.6E+02	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T07-A	1	8.94E+01			8.94E+01	3.9E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T08-A	1	1.91E+03			1.91E+03	8.4E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T09-A	1	3.16E+03			3.16E+03	1.1E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T01-B	1	2.90E+01			2.90E+01	2.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T02-B	1	1.85E+00	U1/2		1.85E+00	1.2E+02	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T03-B	1	6.06E+00	E		6.06E+00	1.0E+02	3.7E+00	1.2E+01	10	325	3.07E+03	94%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T04-B	1	1.85E+00	U1/2		1.85E+00	1.1E+02	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T05-B	1	1.14E+01	E		1.14E+01	1.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T06-B	1	3.85E+00	E		3.85E+00	1.3E+02	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T07-B	1	3.96E+01			3.96E+01	7.9E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T08-B	1	1.89E+03			1.89E+03	9.3E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T09-B	1	3.15E+03			3.15E+03	3.6E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T01-C	1	1.52E+01			1.52E+01	2.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T02-C	1	1.85E+00	U1/2		1.85E+00	4.7E+02	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T03-C	1	5.39E+00	E		5.39E+00	4.6E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T04-C	1	1.85E+00	U1/2		1.85E+00	1.2E+02	3.7E+00	1.2E+01	10	325	3.15E+03	97%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T05-C	1	4.71E+00	E		4.71E+00	1.3E+02	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T06-C	1	5.17E+00	E		5.17E+00	9.6E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T07-C	1	7.23E+01			7.23E+01	1.2E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T08-C	1	1.86E+03			1.86E+03	1.1E+00	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-T09-C	1	3.11E+03			3.11E+03	1.1E+00	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	6.6E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	7.1E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-B03-A	1	8.49E+00	E		8.49E+00	3.8E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-B01-B	1	1.85E+00	U1/2		1.85E+00	2.3E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-B02-B	1	1.85E+00	U1/2		1.85E+00	7.5E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-B03-B	1	1.85E+00	U1/2		1.85E+00	4.1E+02	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-B01-C	1	1.85E+00	U1/2		1.85E+00	9.3E+00	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-B02-C	1	1.85E+00	U1/2		1.85E+00	6.7E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1313-B03-C	1	1.85E+00	U1/2		1.85E+00	1.3E+03	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	EaFA-LRef-1313-T01-A	1	3.39E+01			3.39E+01	1.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T02-A	1	2.02E+01			2.02E+01	2.1E+00	2.0E+00	6.4E+00	1000	100	1.09E+03	107%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	1.5E+02	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	5.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T08-A	1	4.19E+02			4.19E+02	1.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T09-A	1	3.39E+04			3.39E+04	3.1E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T01-B	1	4.31E+01			4.31E+01	1.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T02-B	1	2.07E+01			2.07E+01	7.3E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	6.2E+01	2.0E+00	6.4E+00	1000	100	1.07E+03	107%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	7.9E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T08-B	1	4.00E+02			4.00E+02	1.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T09-B	1	3.38E+04			3.38E+04	3.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T01-C	1	3.59E+01			3.59E+01	1.1E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T02-C	1	2.08E+01			2.08E+01	1.9E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00	1000	100	1.05E+03	105%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	6.0E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	5.2E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T08-C	1	4.45E+02			4.45E+02	1.1E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-T09-C	1	3.30E+04			3.30E+04	3.3E-01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-B02-A	1	1.13E+01			1.13E+01	3.5E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-B03-A	1	1.45E+01			1.45E+01	6.1E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	6.1E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-B02-B	1	1.15E+01			1.15E+01	8.3E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-B03-B	1	1.13E+01			1.13E+01	9.4E-01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	5.7E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-B02-C	1	5.44E+00	E		5.44E+00	2.3E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1313-B03-C	1	1.20E+01			1.20E+01	5.0E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	EaFA-LRef-1313-T01-A	1	3.40E+00	U1/2		3.40E+00	1.3E+02	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T02-A	1	3.40E+00	U1/2		3.40E+00	1.4E+01	6.8E+00	2.2E+01	10	325	3.24E+03	100%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T03-A	1	3.40E+00	U1/2		3.40E+00	1.9E+01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T04-A	1	3.40E+00	U1/2		3.40E+00	6.6E+01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T05-A	1	3.40E+00	U1/2		3.40E+00	2.1E+01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T06-A	1	3.40E+00	U1/2		3.40E+00	5.4E+01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T07-A	1	3.40E+00	U1/2		3.40E+00	7.7E+01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T08-A	1	3.40E+00	U1/2		3.40E+00	1.3E+01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T09-A	1	7.26E+01			7.26E+01	1.0E+01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T01-B	1	3.40E+00	U1/2		3.40E+00	1.9E+02	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T02-B	1	3.40E+00	U1/2		3.40E+00	5.8E+01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T03-B	1	3.40E+00	U1/2		3.40E+00	2.8E+01	6.8E+00	2.2E+01	10	325	3.14E+03	96%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T04-B	1	3.40E+00	U1/2		3.40E+00	3.0E+01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T05-B	1	3.40E+00	U1/2		3.40E+00	3.8E+01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T06-B	1	3.40E+00	U1/2		3.40E+00	2.0E+01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T07-B	1	3.40E+00	U1/2		3.40E+00	4.0E+01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T08-B	1	3.40E+00	U1/2		3.40E+00	1.5E+01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T09-B	1	5.83E+01			5.83E+01	3.1E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T01-C	1	3.40E+00	U1/2		3.40E+00	1.0E+02	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T02-C	1	3.40E+00	U1/2		3.40E+00	8.5E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T03-C	1	3.40E+00	U1/2		3.40E+00	2.0E+01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T04-C	1	3.40E+00	U1/2		3.40E+00	6.4E+00	6.8E+00	2.2E+01	10	325	3.23E+03	99%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T05-C	1	3.40E+00	U1/2		3.40E+00	7.9E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T06-C	1	3.40E+00	U1/2		3.40E+00	1.3E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T07-C	1	3.40E+00	U1/2		3.40E+00	1.0E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T08-C	1	3.40E+00	U1/2		3.40E+00	1.7E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-T09-C	1	6.85E+01			6.85E+01	4.0E+00	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	8.7E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	2.6E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	3.3E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-B01-B	1	3.40E+00	U1/2		3.40E+00	2.1E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-B02-B	1	3.40E+00	U1/2		3.40E+00	2.4E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-B03-B	1	3.40E+00	U1/2		3.40E+00	7.5E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-B01-C	1	3.40E+00	U1/2		3.40E+00	3.4E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-B02-C	1	3.40E+00	U1/2		3.40E+00	8.5E+00	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1313-B03-C	1	3.40E+00	U1/2		3.40E+00	1.2E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	EaFA-LRef-1313-T01-A	1	1.56E+03			1.56E+03	3.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T02-A	1	2.23E+03			2.23E+03	2.6E-01	1.9E+00	6.0E+00	10	325	4.96E+03	84%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T03-A	1	2.56E+03			2.56E+03	7.9E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T04-A	1	2.70E+03			2.70E+03	3.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T05-A	1	2.97E+03			2.97E+03	4.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T06-A	1	3.24E+03			3.24E+03	3.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T07-A	1	3.26E+03			3.26E+03	1.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T08-A	1	2.12E+03			2.12E+03	2.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T09-A	1	1.51E+03			1.51E+03	4.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T01-B	1	1.53E+03			1.53E+03	1.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T02-B	1	2.21E+03			2.21E+03	1.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T03-B	1	2.63E+03			2.63E+03	4.8E-01	1.9E+00	6.0E+00	10	325	5.38E+03	85%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T04-B	1	2.50E+03			2.50E+03	8.6E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T05-B	1	2.94E+03			2.94E+03	8.6E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T06-B	1	3.06E+03			3.06E+03	2.9E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T07-B	1	3.13E+03			3.13E+03	5.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T08-B	1	2.15E+03			2.15E+03	4.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T09-B	1	1.50E+03			1.50E+03	7.2E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T01-C	1	1.53E+03			1.53E+03	8.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T02-C	1	2.20E+03			2.20E+03	5.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T03-C	1	2.54E+03			2.54E+03	3.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T04-C	1	2.36E+03			2.36E+03	4.6E-01	1.9E+00	6.0E+00	10	325	5.25E+03	89%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T05-C	1	2.88E+03			2.88E+03	2.9E-01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T06-C	1	2.98E+03			2.98E+03	3.7E-01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T07-C	1	3.07E+03			3.07E+03	1.8E+00	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T08-C	1	2.07E+03			2.07E+03	1.8E+00	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-T09-C	1	1.48E+03			1.48E+03	3.0E-01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-B01-A	1	2.75E+00	E		2.75E+00	1.9E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	8.6E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-B03-A	1	5.32E+00	E		5.32E+00	3.7E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-B01-B	1	2.66E+00	E		2.66E+00	1.3E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-B02-B	1	2.85E+00	E		2.85E+00	1.6E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-B03-B	1	3.94E+00	E		3.94E+00	6.1E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-B01-C	1	2.26E+00	E		2.26E+00	9.2E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-B02-C	1	3.00E+00	E		3.00E+00	2.5E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1313-B03-C	1	2.46E+00	E		2.46E+00	4.5E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	EaFA-LRef-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	9.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	5.1E+00	2.0E+00	6.4E+00	10	325	3.07E+03	95%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	2.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	4.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T05-A	1	3.24E+01			3.24E+01	6.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T06-A	1	2.68E+02			2.68E+02	5.8E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T07-A	1	9.82E+02			9.82E+02	8.0E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T08-A	1	1.17E+03			1.17E+03	1.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T09-A	1	1.84E+03			1.84E+03	5.1E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	8.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	1.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	1.6E+00	2.0E+00	6.4E+00	10	325	3.02E+03	93%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	4.9E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T05-B	1	3.58E+01			3.58E+01	1.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T06-B	1	2.19E+02			2.19E+02	1.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T07-B	1	9.39E+02			9.39E+02	1.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T08-B	1	1.15E+03			1.15E+03	9.5E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T09-B	1	1.80E+03			1.80E+03	2.5E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	1.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	3.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	6.9E+00	2.0E+00	6.4E+00	10	325	3.06E+03	94%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T05-C	1	3.63E+01			3.63E+01	1.0E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T06-C	1	1.93E+02			1.93E+02	1.4E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T07-C	1	9.11E+02			9.11E+02	1.7E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T08-C	1	1.15E+03			1.15E+03	1.0E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-T09-C	1	1.81E+03			1.81E+03	2.3E-01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	5.2E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	2.1E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	6.5E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	8.5E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	2.3E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	9.7E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1313-B03-C	1	1.00E+00	U1/2		1.00E+00	2.1E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	EaFA-LRef-1313-T01-A	1	5.00E-01	U1/2		5.00E-01	4.9E+01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T02-A	1	5.00E-01	U1/2		5.00E-01	2.9E+01	1.0E+00	3.2E+00	1000	100	1.09E+03	109%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T03-A	1	1.11E+02			1.11E+02	7.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T04-A	1	2.86E+03			2.86E+03	3.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T05-A	1	5.10E+03			5.10E+03	9.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T06-A	1	7.49E+03			7.49E+03	7.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T07-A	1	8.90E+03			8.90E+03	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T08-A	1	7.69E+03			7.69E+03	8.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T09-A	1	1.40E+04			1.40E+04	5.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T01-B	1	5.00E-01	U1/2		5.00E-01	3.8E+01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T02-B	1	5.00E-01	U1/2		5.00E-01	3.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T03-B	1	3.55E+02			3.55E+02	1.5E+00	1.0E+00	3.2E+00	1000	100	1.22E+03	86%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T04-B	1	1.84E+03			1.84E+03	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T05-B	1	5.27E+03			5.27E+03	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T06-B	1	7.03E+03			7.03E+03	8.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T07-B	1	8.88E+03			8.88E+03	3.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T08-B	1	7.75E+03			7.75E+03	4.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T09-B	1	1.41E+04			1.41E+04	1.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T01-C	1	5.00E-01	U1/2		5.00E-01	5.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T02-C	1	5.00E-01	U1/2		5.00E-01	6.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T03-C	1	4.15E+02			4.15E+02	3.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T04-C	1	2.74E+03			2.74E+03	7.9E-01	1.0E+00	3.2E+00	1000	100	3.63E+03	89%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T05-C	1	5.20E+03			5.20E+03	5.6E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T06-C	1	7.04E+03			7.04E+03	4.9E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T07-C	1	8.48E+03			8.48E+03	3.5E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T08-C	1	7.51E+03			7.51E+03	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-T09-C	1	1.41E+04			1.41E+04	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.8E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	3.2E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	7.9E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	4.4E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	8.7E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	7.4E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	1.5E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	2.7E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	2.7E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	EaFA-LRef-1313-T01-A	1	3.92E+03			3.92E+03	7.7E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T02-A	1	3.77E+03			3.77E+03	4.0E-01	1.2E+00	3.8E+00	10	325	6.66E+03	89%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T03-A	1	3.83E+03			3.83E+03	8.7E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T04-A	1	3.70E+03			3.70E+03	5.2E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T05-A	1	3.49E+03			3.49E+03	1.5E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T06-A	1	3.32E+03			3.32E+03	4.1E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T07-A	1	5.52E+02			5.52E+02	7.3E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T08-A	1	1.08E+02			1.08E+02	6.8E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T09-A	1	3.34E+02			3.34E+02	1.3E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T01-B	1	3.98E+03			3.98E+03	3.7E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T02-B	1	3.85E+03			3.85E+03	3.4E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T03-B	1	3.81E+03			3.81E+03	1.5E+00	1.2E+00	3.8E+00	10	325	6.92E+03	96%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T04-B	1	3.53E+03			3.53E+03	1.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T05-B	1	3.44E+03			3.44E+03	5.2E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T06-B	1	3.20E+03			3.20E+03	6.8E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T07-B	1	7.19E+02			7.19E+02	9.1E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T08-B	1	1.10E+02			1.10E+02	2.3E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T09-B	1	3.52E+02			3.52E+02	1.4E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T01-C	1	3.84E+03			3.84E+03	3.4E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T02-C	1	3.73E+03			3.73E+03	1.3E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T03-C	1	3.72E+03			3.72E+03	1.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T04-C	1	3.59E+03			3.59E+03	8.1E-01	1.2E+00	3.8E+00	10	325	6.73E+03	97%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T05-C	1	3.41E+03			3.41E+03	8.8E-02	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T06-C	1	3.17E+03			3.17E+03	6.6E-01	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T07-C	1	5.34E+02			5.34E+02	1.3E+00	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T08-C	1	1.01E+02			1.01E+02	2.1E+00	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-T09-C	1	3.04E+02			3.04E+02	1.3E+00	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	8.7E+01	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	3.8E+02	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-B03-A	1	1.80E+00	E		1.80E+00	3.7E+02	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-B01-B	1	6.00E-01	U1/2		6.00E-01	5.5E+01	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-B02-B	1	6.00E-01	U1/2		6.00E-01	2.8E+01	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-B03-B	1	4.99E+00			4.99E+00	4.3E+01	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-B01-C	1	6.00E-01	U1/2		6.00E-01	4.1E+03	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-B02-C	1	6.00E-01	U1/2		6.00E-01	1.2E+02	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1313-B03-C	1	6.00E-01	U1/2		6.00E-01	6.4E+02	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	EaFA-LRef-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	1.2E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	7.3E+01	1.8E+00	5.7E+00	10	325	3.20E+03	98%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	3.2E+01	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T05-A	1	6.83E+00			6.83E+00	6.1E+01	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T06-A	1	6.46E+01			6.46E+01	2.3E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T07-A	1	6.03E+02			6.03E+02	1.0E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T08-A	1	5.19E+02			5.19E+02	1.4E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T09-A	1	7.62E+02			7.62E+02	5.9E-01	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	1.1E+03	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	2.6E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	2.1E+02	1.8E+00	5.7E+00	10	325	3.08E+03	95%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T05-B	1	5.92E+00			5.92E+00	1.6E+01	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T06-B	1	5.05E+01			5.05E+01	3.3E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T07-B	1	5.46E+02			5.46E+02	1.2E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T08-B	1	5.16E+02			5.16E+02	1.0E-01	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T09-B	1	7.50E+02			7.50E+02	2.2E-01	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	2.6E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	2.9E+01	1.8E+00	5.7E+00			---		VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	1.9E+02	1.8E+00	5.7E+00	10	325	3.05E+03	94%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T05-C	1	4.26E+00	E		4.26E+00	4.4E+01	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T06-C	1	4.37E+01			4.37E+01	2.7E+00	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T07-C	1	5.75E+02			5.75E+02	1.8E+00	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T08-C	1	5.07E+02			5.07E+02	1.6E+00	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-T09-C	1	7.58E+02			7.58E+02	2.5E-01	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	1.2E+02	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	1.0E+02	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-B03-A	1	2.06E+01			2.06E+01	2.5E+01	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-B01-B	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-B02-B	1	9.00E-01	U1/2		9.00E-01	3.2E+02	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-B03-B	1	3.75E+01			3.75E+01	3.6E+00	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-B01-C	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-B02-C	1	9.00E-01	U1/2		9.00E-01	3.7E+02	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1313-B03-C	1	2.20E+01			2.20E+01	4.3E+01	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	EaFA-LRef-1313-T01-A	1	2.09E+02			2.09E+02	3.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T02-A	1	3.72E+01			3.72E+01	2.7E+01	3.7E+00	1.2E+01	1000	100	1.05E+03	102%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T03-A	1	4.30E+01			4.30E+01	4.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T04-A	1	8.54E+01			8.54E+01	1.9E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T05-A	1	3.96E+01			3.96E+01	2.9E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T06-A	1	1.63E+01			1.63E+01	4.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T07-A	1	1.85E+00	U1/2		1.85E+00	2.0E+02	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T08-A	1	6.29E+01			6.29E+01	9.0E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T09-A	1	2.42E+03			2.42E+03	3.0E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T01-B	1	3.03E+02			3.03E+02	3.7E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T02-B	1	2.44E+01			2.44E+01	2.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T03-B	1	8.64E+01			8.64E+01	5.8E+00	3.7E+00	1.2E+01	1000	100	1.15E+03	106%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T04-B	1	8.09E+01			8.09E+01	1.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T05-B	1	4.03E+01			4.03E+01	3.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T06-B	1	2.66E+01			2.66E+01	8.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T07-B	1	3.45E+01			3.45E+01	1.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T08-B	1	7.11E+01			7.11E+01	1.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T09-B	1	2.73E+03			2.73E+03	6.2E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T01-C	1	2.35E+02			2.35E+02	5.8E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T02-C	1	3.97E+01			3.97E+01	2.6E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T03-C	1	7.16E+01			7.16E+01	1.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T04-C	1	8.01E+01			8.01E+01	1.8E+01	3.7E+00	1.2E+01	1000	100	1.09E+03	101%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T05-C	1	3.93E+01			3.93E+01	2.7E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T06-C	1	1.93E+01			1.93E+01	1.1E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T07-C	1	1.74E+01			1.74E+01	4.3E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T08-C	1	6.81E+01			6.81E+01	9.5E+00	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-T09-C	1	2.35E+03			2.35E+03	7.7E-01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-B01-A	1	1.37E+01			1.37E+01	3.1E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-B02-A	1	8.36E+00	E		8.36E+00	9.8E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-B03-A	1	1.56E+01			1.56E+01	1.1E+02	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-B01-B	1	1.85E+00	U1/2		1.85E+00	4.0E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-B02-B	1	4.22E+00	E		4.22E+00	7.8E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-B03-B	1	8.72E+00	E		8.72E+00	8.9E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-B01-C	1	1.24E+01			1.24E+01	6.6E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-B02-C	1	8.77E+00	E		8.77E+00	1.9E+02	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1313-B03-C	1	2.14E+01			2.14E+01	6.0E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	EaFA-LRef-1313-T01-A	1	1.72E+06			1.72E+06	1.1E+00	1.6E+00	5.1E+00			---		VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T02-A	1	4.41E+05			4.41E+05	1.7E+00	1.6E+00	5.1E+00	1000	100	4.42E+05	93%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T03-A	1	1.90E+05			1.90E+05	2.5E-01	1.6E+00	5.1E+00			---		VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T04-A	1	1.35E+05			1.35E+05	1.9E-01	1.6E+00	5.1E+00			---		VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T05-A	1	5.53E+04			5.53E+04	4.4E-01	1.6E+00	5.1E+00			---		VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T06-A	1	2.50E+04			2.50E+04	6.4E-01	1.6E+00	5.1E+00			---		VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T07-A	1	2.61E+04			2.61E+04	3.2E-01	1.6E+00	5.1E+00			---		VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T08-A	1	1.86E+04			1.86E+04	8.1E-01	1.6E+00	5.1E+00			---		VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T09-A	1	2.21E+04			2.21E+04	2.6E-01	1.6E+00	5.1E+00			---		VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T01-B	1	1.74E+06			1.74E+06	8.9E-01	1.6E+00	5.1E+00			---		VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T02-B	1	4.50E+05			4.50E+05	2.3E+00	1.6E+00	5.1E+00			---		VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T03-B	1	1.79E+05			1.79E+05	6.4E-01	1.6E+00	5.1E+00	1000	100	1.80E+05	91%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T04-B	1	1.31E+05			1.31E+05	8.2E-02	1.6E+00	5.1E+00			---		VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T05-B	1	5.45E+04			5.45E+04	7.6E-01	1.6E+00	5.1E+00			---		VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T06-B	1	2.33E+04			2.33E+04	5.9E-01	1.6E+00	5.1E+00			---		VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T07-B	1	2.48E+04			2.48E+04	8.1E-01	1.6E+00	5.1E+00			---		VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T08-B	1	1.87E+04			1.87E+04	7.3E-01	1.6E+00	5.1E+00			---		VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T09-B	1	2.17E+04			2.17E+04	5.2E-01	1.6E+00	5.1E+00			---		VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T01-C	1	1.68E+06			1.68E+06	7.9E-01	1.6E+00	5.1E+00			---		VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T02-C	1	3.92E+05			3.92E+05	7.4E-01	1.6E+00	5.1E+00			---		VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T03-C	1	1.71E+05			1.71E+05	9.0E-01	1.6E+00	5.1E+00			---		VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T04-C	1	1.18E+05			1.18E+05	4.9E-01	1.6E+00	5.1E+00	1000	100	1.19E+05	95%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T05-C	1	5.01E+04			5.01E+04	1.2E+00	1.6E+00	5.1E+00					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T06-C	1	2.28E+04			2.28E+04	8.5E-01	1.6E+00	5.1E+00					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T07-C	1	2.51E+04			2.51E+04	8.3E-01	1.6E+00	5.1E+00					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T08-C	1	1.81E+04			1.81E+04	1.3E+00	1.6E+00	5.1E+00					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-T09-C	1	2.17E+04			2.17E+04	7.3E-01	1.6E+00	5.1E+00					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-B01-A	1	8.00E-01	U1/2		8.00E-01	2.9E+02	1.6E+00	5.1E+00					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-B02-A	1	2.83E+00	E		2.83E+00	1.6E+02	1.6E+00	5.1E+00					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-B03-A	1	1.81E+06			1.81E+06	4.6E-01	1.6E+00	5.1E+00					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-B01-B	1	8.00E-01	U1/2		8.00E-01	1.4E+02	1.6E+00	5.1E+00					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-B02-B	1	1.24E+01			1.24E+01	2.5E+01	1.6E+00	5.1E+00					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-B03-B	1	1.70E+06			1.70E+06	7.9E-01	1.6E+00	5.1E+00					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-B01-C	1	8.00E-01	U1/2		8.00E-01	3.2E+02	1.6E+00	5.1E+00					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-B02-C	1	3.25E+00	E		3.25E+00	1.1E+02	1.6E+00	5.1E+00					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1313-B03-C	1	1.73E+06			1.73E+06	2.5E-01	1.6E+00	5.1E+00					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	EaFA-LRef-1313-T01-A	1	6.88E+03			6.88E+03	1.4E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T02-A	1	5.60E+03			5.60E+03	6.2E-01	1.5E+01	4.8E+01	10	325	8.90E+03	102%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T03-A	1	4.92E+03			4.92E+03	6.4E-01	1.5E+01	4.8E+01			---		VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T04-A	1	4.01E+03			4.01E+03	2.5E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T05-A	1	1.64E+03			1.64E+03	1.5E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T06-A	1	9.22E+02			9.22E+02	5.3E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T07-A	1	2.30E+02			2.30E+02	3.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T08-A	1	8.41E+01			8.41E+01	2.5E+01	1.5E+01	4.8E+01			---		VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T09-A	1	5.46E+02			5.46E+02	5.7E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T01-B	1	6.80E+03			6.80E+03	1.5E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T02-B	1	5.41E+03			5.41E+03	2.0E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T03-B	1	4.82E+03			4.82E+03	3.8E-01	1.5E+01	4.8E+01	10	325	8.24E+03	105%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T04-B	1	3.78E+03			3.78E+03	1.7E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T05-B	1	1.58E+03			1.58E+03	3.5E-01	1.5E+01	4.8E+01			---		VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T06-B	1	8.42E+02			8.42E+02	1.4E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T07-B	1	2.60E+02			2.60E+02	7.5E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T08-B	1	9.37E+01			9.37E+01	1.9E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T09-B	1	5.77E+02			5.77E+02	1.3E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T01-C	1	6.81E+03			6.81E+03	1.7E-01	1.5E+01	4.8E+01			---		VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T02-C	1	5.46E+03			5.46E+03	3.6E-01	1.5E+01	4.8E+01			---		VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T03-C	1	4.74E+03			4.74E+03	1.5E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T04-C	1	3.66E+03			3.66E+03	8.2E-01	1.5E+01	4.8E+01	10	325	6.90E+03	100%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T05-C	1	1.54E+03			1.54E+03	2.5E+00	1.5E+01	4.8E+01					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T06-C	1	9.26E+02			9.26E+02	5.3E+00	1.5E+01	4.8E+01					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T07-C	1	1.82E+02			1.82E+02	1.0E+01	1.5E+01	4.8E+01					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T08-C	1	5.67E+01			5.67E+01	2.7E+01	1.5E+01	4.8E+01					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-T09-C	1	4.77E+02			4.77E+02	1.1E+00	1.5E+01	4.8E+01					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-B01-A	1	7.50E+00	U1/2		7.50E+00	7.5E+01	1.5E+01	4.8E+01					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-B02-A	1	7.50E+00	U1/2		7.50E+00	6.9E+01	1.5E+01	4.8E+01					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-B03-A	1	3.59E+01	E		3.59E+01	1.5E+02	1.5E+01	4.8E+01					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-B01-B	1	7.50E+00	U1/2		7.50E+00	4.6E+01	1.5E+01	4.8E+01					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-B02-B	1	7.50E+00	U1/2		7.50E+00	6.2E+02	1.5E+01	4.8E+01					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-B03-B	1	2.08E+01	E		2.08E+01	1.1E+02	1.5E+01	4.8E+01					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-B01-C	1	7.50E+00	U1/2		7.50E+00	8.1E+01	1.5E+01	4.8E+01					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-B02-C	1	7.50E+00	U1/2		7.50E+00	6.1E+01	1.5E+01	4.8E+01					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1313-B03-C	1	3.55E+01	E		3.55E+01	4.9E+01	1.5E+01	4.8E+01					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	EaFA-LRef-1313-T01-A	1	3.06E+04			3.06E+04	1.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T02-A	1	3.76E+03			3.76E+03	4.9E-01	1.1E+00	3.5E+00	1000	100	4.60E+03	84%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T03-A	1	7.20E+02			7.20E+02	6.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T04-A	1	2.78E+02			2.78E+02	2.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T05-A	1	5.35E+02			5.35E+02	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T06-A	1	1.43E+03			1.43E+03	2.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T07-A	1	6.17E+03			6.17E+03	8.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T08-A	1	1.80E+04			1.80E+04	4.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T09-A	1	7.22E+04			7.22E+04	6.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T01-B	1	3.55E+04			3.55E+04	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T02-B	1	3.71E+03			3.71E+03	3.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T03-B	1	4.44E+02			4.44E+02	7.0E-01	1.1E+00	3.5E+00	1000	100	1.29E+03	85%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T04-B	1	2.75E+02			2.75E+02	1.6E+00	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T05-B	1	5.36E+02			5.36E+02	5.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T06-B	1	1.20E+03			1.20E+03	1.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T07-B	1	5.67E+03			5.67E+03	2.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T08-B	1	1.80E+04			1.80E+04	1.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T09-B	1	7.09E+04			7.09E+04	3.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T01-C	1	2.82E+04			2.82E+04	1.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T02-C	1	2.95E+03			2.95E+03	6.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T03-C	1	4.64E+02			4.64E+02	7.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T04-C	1	2.57E+02			2.57E+02	1.9E+00	1.1E+00	3.5E+00	1000	100	1.24E+03	99%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T05-C	1	5.67E+02			5.67E+02	3.8E-01	1.1E+00	3.5E+00					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T06-C	1	1.24E+03			1.24E+03	4.5E-01	1.1E+00	3.5E+00					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T07-C	1	5.90E+03			5.90E+03	9.0E-01	1.1E+00	3.5E+00					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T08-C	1	1.75E+04			1.75E+04	1.2E+00	1.1E+00	3.5E+00					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-T09-C	1	7.20E+04			7.20E+04	4.9E-01	1.1E+00	3.5E+00					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-B01-A	1	4.01E+00			4.01E+00	1.1E+02	1.1E+00	3.5E+00					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-B02-A	1	2.87E+02			2.87E+02	5.7E+00	1.1E+00	3.5E+00					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-B03-A	1	5.24E+04			5.24E+04	3.0E-01	1.1E+00	3.5E+00					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-B01-B	1	2.14E+01			2.14E+01	2.2E+01	1.1E+00	3.5E+00					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-B02-B	1	2.93E+02			2.93E+02	3.9E+00	1.1E+00	3.5E+00					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-B03-B	1	5.07E+04			5.07E+04	1.2E+00	1.1E+00	3.5E+00					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-B01-C	1	2.54E+01			2.54E+01	2.3E+00	1.1E+00	3.5E+00					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-B02-C	1	2.86E+02			2.86E+02	4.5E+00	1.1E+00	3.5E+00					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1313-B03-C	1	1.65E+04			1.65E+04	6.3E-01	1.1E+00	3.5E+00					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	EaFA-LRef-1313-T01-A	1	8.92E+03			8.92E+03	5.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T02-A	1	6.80E+03			6.80E+03	5.0E-01	2.5E+00	8.0E+00	1000	100	7.79E+03	99%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T03-A	1	6.50E+03			6.50E+03	5.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T04-A	1	6.39E+03			6.39E+03	2.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T05-A	1	6.27E+03			6.27E+03	1.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T06-A	1	6.45E+03			6.45E+03	3.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T07-A	1	6.63E+03			6.63E+03	6.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T08-A	1	4.51E+03			4.51E+03	5.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T09-A	1	3.85E+03			3.85E+03	3.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T01-B	1	8.86E+03			8.86E+03	1.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T02-B	1	6.77E+03			6.77E+03	8.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T03-B	1	6.62E+03			6.62E+03	1.4E+00	2.5E+00	8.0E+00	1000	100	7.58E+03	97%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T04-B	1	6.19E+03			6.19E+03	7.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T05-B	1	6.12E+03			6.12E+03	4.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T06-B	1	6.03E+03			6.03E+03	4.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T07-B	1	6.22E+03			6.22E+03	3.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T08-B	1	4.48E+03			4.48E+03	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T09-B	1	3.79E+03			3.79E+03	5.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T01-C	1	8.94E+03			8.94E+03	3.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T02-C	1	6.73E+03			6.73E+03	4.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T03-C	1	6.48E+03			6.48E+03	6.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T04-C	1	6.08E+03			6.08E+03	9.5E-01	2.5E+00	8.0E+00	1000	100	7.02E+03	94%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T05-C	1	6.04E+03			6.04E+03	2.2E-01	2.5E+00	8.0E+00					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T06-C	1	5.95E+03			5.95E+03	1.0E-01	2.5E+00	8.0E+00					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T07-C	1	6.25E+03			6.25E+03	1.7E+00	2.5E+00	8.0E+00					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T08-C	1	4.34E+03			4.34E+03	1.9E+00	2.5E+00	8.0E+00					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-T09-C	1	3.75E+03			3.75E+03	6.4E-01	2.5E+00	8.0E+00					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-B01-A	1	1.25E+00	U1/2		1.25E+00	7.9E-01	2.5E+00	8.0E+00					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-B02-A	1	1.25E+00	U1/2		1.25E+00	2.3E+00	2.5E+00	8.0E+00					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-B03-A	1	3.01E+03			3.01E+03	2.4E-01	2.5E+00	8.0E+00					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-B01-B	1	1.25E+00	U1/2		1.25E+00	1.6E+00	2.5E+00	8.0E+00					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-B02-B	1	1.25E+00	U1/2		1.25E+00	1.0E+00	2.5E+00	8.0E+00					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-B03-B	1	2.88E+03			2.88E+03	7.4E-01	2.5E+00	8.0E+00					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-B01-C	1	1.25E+00	U1/2		1.25E+00	1.6E+00	2.5E+00	8.0E+00					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-B02-C	1	1.25E+00	U1/2		1.25E+00	2.6E+00	2.5E+00	8.0E+00					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1313-B03-C	1	3.65E+03			3.65E+03	9.5E-01	2.5E+00	8.0E+00					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	EaFA-LRef-1313-T01-A	1	9.16E+02			9.16E+02	3.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T02-A	1	1.64E+03			1.64E+03	3.5E-01	1.0E+00	3.2E+00	1000	100	2.52E+03	88%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T03-A	1	1.96E+03			1.96E+03	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T04-A	1	2.10E+03			2.10E+03	7.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T05-A	1	2.30E+03			2.30E+03	9.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T06-A	1	2.54E+03			2.54E+03	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T07-A	1	3.09E+03			3.09E+03	2.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T08-A	1	3.07E+03			3.07E+03	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T09-A	1	5.56E+03			5.56E+03	8.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T01-B	1	8.38E+02			8.38E+02	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T02-B	1	1.66E+03			1.66E+03	6.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T03-B	1	2.19E+03			2.19E+03	9.3E-01	1.0E+00	3.2E+00	1000	100	3.06E+03	87%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T04-B	1	2.04E+03			2.04E+03	5.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T05-B	1	2.29E+03			2.29E+03	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T06-B	1	2.42E+03			2.42E+03	8.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T07-B	1	3.09E+03			3.09E+03	3.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T08-B	1	3.04E+03			3.04E+03	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T09-B	1	5.44E+03			5.44E+03	1.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T01-C	1	9.44E+02			9.44E+02	6.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T02-C	1	1.71E+03			1.71E+03	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T03-C	1	2.02E+03			2.02E+03	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T04-C	1	2.10E+03			2.10E+03	2.9E-01	1.0E+00	3.2E+00	1000	100	3.01E+03	91%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T05-C	1	2.28E+03			2.28E+03	6.8E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T06-C	1	2.38E+03			2.38E+03	7.8E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T07-C	1	2.95E+03			2.95E+03	9.6E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T08-C	1	3.02E+03			3.02E+03	1.7E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-T09-C	1	5.55E+03			5.55E+03	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.7E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	3.5E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-B03-A	1	2.01E+00	E		2.01E+00	4.6E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	3.2E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-B03-B	1	2.48E+00	E		2.48E+00	2.9E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	5.6E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	2.8E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	1.0E+03	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	EaFA-LRef-1313-T01-A	1	1.85E+05			1.85E+05	3.8E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T02-A	1	1.62E+05			1.62E+05	6.9E-02	6.8E+00	2.2E+01	1000	100	1.63E+05	84%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T03-A	1	1.60E+05			1.60E+05	8.8E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T04-A	1	1.63E+05			1.63E+05	1.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T05-A	1	1.60E+05			1.60E+05	3.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T06-A	1	1.64E+05			1.64E+05	8.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T07-A	1	1.52E+05			1.52E+05	4.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T08-A	1	1.04E+05			1.04E+05	4.3E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T09-A	1	6.90E+04			6.90E+04	5.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T01-B	1	1.88E+05			1.88E+05	7.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T02-B	1	1.66E+05			1.66E+05	8.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T03-B	1	1.65E+05			1.65E+05	9.4E-01	6.8E+00	2.2E+01	1000	100	1.66E+05	82%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T04-B	1	1.59E+05			1.59E+05	6.9E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T05-B	1	1.59E+05			1.59E+05	5.3E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T06-B	1	1.58E+05			1.58E+05	3.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T07-B	1	1.50E+05			1.50E+05	6.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T08-B	1	1.03E+05			1.03E+05	1.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T09-B	1	6.93E+04			6.93E+04	2.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T01-C	1	1.90E+05			1.90E+05	3.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T02-C	1	1.63E+05			1.63E+05	3.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T03-C	1	1.64E+05			1.64E+05	5.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T04-C	1	1.62E+05			1.62E+05	2.1E-01	6.8E+00	2.2E+01	1000	100	1.62E+05	87%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T05-C	1	1.62E+05			1.62E+05	4.4E-01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T06-C	1	1.60E+05			1.60E+05	2.8E-01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T07-C	1	1.51E+05			1.51E+05	8.5E-01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T08-C	1	1.03E+05			1.03E+05	1.4E+00	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-T09-C	1	6.92E+04			6.92E+04	2.7E-01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	4.3E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	5.2E+02	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-B03-A	1	3.55E+01			3.55E+01	1.3E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-B01-B	1	3.40E+00	U1/2		3.40E+00	3.2E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-B02-B	1	3.40E+00	U1/2		3.40E+00	4.4E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-B03-B	1	3.28E+01			3.28E+01	1.3E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-B01-C	1	3.40E+00	U1/2		3.40E+00	2.3E+02	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-B02-C	1	3.40E+00	U1/2		3.40E+00	1.6E+02	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1313-B03-C	1	4.09E+01			4.09E+01	3.8E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	EaFA-LRef-1313-T01-A	1	2.30E+00	U1/2		2.30E+00	7.5E+01	4.6E+00	1.5E+01			---		VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T02-A	1	2.30E+00	U1/2		2.30E+00	1.2E+02	4.6E+00	1.5E+01	10	325	3.23E+03	99%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T03-A	1	2.30E+00	U1/2		2.30E+00	2.6E+02	4.6E+00	1.5E+01			---		VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T04-A	1	2.30E+00	U1/2		2.30E+00	7.8E+01	4.6E+00	1.5E+01			---		VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T05-A	1	2.30E+00	U1/2		2.30E+00	2.8E+01	4.6E+00	1.5E+01			---		VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T06-A	1	2.30E+00	U1/2		2.30E+00	4.1E+01	4.6E+00	1.5E+01			---		VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T07-A	1	2.25E+01			2.25E+01	7.2E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T08-A	1	4.09E+01			4.09E+01	2.6E+01	4.6E+00	1.5E+01			---		VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T09-A	1	7.87E+01			7.87E+01	3.3E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T01-B	1	2.30E+00	U1/2		2.30E+00	1.2E+02	4.6E+00	1.5E+01			---		VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T02-B	1	2.30E+00	U1/2		2.30E+00	5.7E+01	4.6E+00	1.5E+01			---		VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T03-B	1	2.30E+00	U1/2		2.30E+00	6.9E+01	4.6E+00	1.5E+01	10	325	3.16E+03	97%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T04-B	1	2.30E+00	U1/2		2.30E+00	7.7E+02	4.6E+00	1.5E+01			---		VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T05-B	1	2.30E+00	U1/2		2.30E+00	8.6E+01	4.6E+00	1.5E+01			---		VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T06-B	1	2.30E+00	U1/2		2.30E+00	6.0E+01	4.6E+00	1.5E+01			---		VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T07-B	1	5.63E+00	E		5.63E+00	2.9E+02	4.6E+00	1.5E+01			---		VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T08-B	1	4.21E+01			4.21E+01	4.5E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T09-B	1	6.79E+01			6.79E+01	3.7E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T01-C	1	2.30E+00	U1/2		2.30E+00	1.9E+02	4.6E+00	1.5E+01			---		VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T02-C	1	2.30E+00	U1/2		2.30E+00	3.1E+02	4.6E+00	1.5E+01			---		VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T03-C	1	2.30E+00	U1/2		2.30E+00	6.5E+01	4.6E+00	1.5E+01			---		VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T04-C	1	2.30E+00	U1/2		2.30E+00	9.1E+01	4.6E+00	1.5E+01	10	325	3.24E+03	100%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T05-C	1	2.30E+00	U1/2		2.30E+00	6.9E+01	4.6E+00	1.5E+01					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T06-C	1	2.30E+00	U1/2		2.30E+00	1.7E+02	4.6E+00	1.5E+01					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T07-C	1	1.28E+01	E		1.28E+01	1.3E+02	4.6E+00	1.5E+01					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T08-C	1	4.06E+01			4.06E+01	6.8E+00	4.6E+00	1.5E+01					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-T09-C	1	7.14E+01			7.14E+01	1.4E+01	4.6E+00	1.5E+01					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	2.0E+01	4.6E+00	1.5E+01					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	1.2E+01	4.6E+00	1.5E+01					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	3.3E+02	4.6E+00	1.5E+01					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-B01-B	1	2.30E+00	U1/2		2.30E+00	2.8E+01	4.6E+00	1.5E+01					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-B02-B	1	2.30E+00	U1/2		2.30E+00	2.6E+01	4.6E+00	1.5E+01					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-B03-B	1	2.30E+00	U1/2		2.30E+00	4.5E+01	4.6E+00	1.5E+01					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-B01-C	1	2.30E+00	U1/2		2.30E+00	2.7E+01	4.6E+00	1.5E+01					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-B02-C	1	2.30E+00	U1/2		2.30E+00	1.2E+02	4.6E+00	1.5E+01					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1313-B03-C	1	2.30E+00	U1/2		2.30E+00	5.1E+01	4.6E+00	1.5E+01					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	EaFA-LRef-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	5.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	2.4E+01	2.0E+00	6.4E+00	10	325	3.15E+03	97%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	3.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	9.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T08-A	1	3.73E+00	E		3.73E+00	1.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T09-A	1	1.50E+03			1.50E+03	1.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	4.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	3.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	9.3E+00	2.0E+00	6.4E+00	10	325	3.12E+03	96%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	5.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	1.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	6.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	8.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T08-B	1	3.46E+00	E		3.46E+00	1.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T09-B	1	1.69E+03			1.69E+03	6.6E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	7.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	7.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	8.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	2.9E+01	2.0E+00	6.4E+00	10	325	3.08E+03	95%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	4.7E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T08-C	1	3.30E+00	E		3.30E+00	5.5E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-T09-C	1	1.34E+03			1.34E+03	3.3E-01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	3.3E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	7.5E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-B03-A	1	4.15E+01			4.15E+01	2.0E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	3.1E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	5.8E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-B03-B	1	3.88E+01			3.88E+01	5.5E-01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	3.6E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	1.9E+02	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1313-B03-C	1	1.18E+01			1.18E+01	6.2E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	EaFA-LRef-1313-T01-A	1	5.21E+03			5.21E+03	3.5E-01	1.5E+00	4.8E+00			---		VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T02-A	1	2.74E+03			2.74E+03	4.9E-01	1.5E+00	4.8E+00	10	325	5.90E+03	97%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T03-A	1	2.07E+03			2.07E+03	1.3E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T04-A	1	8.32E+02			8.32E+02	6.1E-01	1.5E+00	4.8E+00			---		VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T05-A	1	2.09E+02			2.09E+02	4.7E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T06-A	1	1.58E+02			1.58E+02	2.6E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T07-A	1	7.94E+01			7.94E+01	2.8E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T08-A	1	8.18E+01			8.18E+01	2.0E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T09-A	1	6.64E+03			6.64E+03	6.0E-01	1.5E+00	4.8E+00			---		VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T01-B	1	5.24E+03			5.24E+03	8.8E-01	1.5E+00	4.8E+00			---		VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T02-B	1	2.61E+03			2.61E+03	1.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T03-B	1	1.39E+03			1.39E+03	1.4E+00	1.5E+00	4.8E+00	10	325	5.21E+03	118%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T04-B	1	7.86E+02			7.86E+02	1.8E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T05-B	1	2.11E+02			2.11E+02	2.0E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T06-B	1	1.50E+02			1.50E+02	4.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T07-B	1	7.88E+01			7.88E+01	3.7E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T08-B	1	8.33E+01			8.33E+01	8.3E-01	1.5E+00	4.8E+00			---		VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T09-B	1	6.63E+03			6.63E+03	4.0E-01	1.5E+00	4.8E+00			---		VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T01-C	1	4.92E+03			4.92E+03	7.2E-01	1.5E+00	4.8E+00			---		VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T02-C	1	2.37E+03			2.37E+03	1.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T03-C	1	1.51E+03			1.51E+03	1.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T04-C	1	6.84E+02			6.84E+02	2.7E-01	1.5E+00	4.8E+00	10	325	3.92E+03	100%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T05-C	1	2.07E+02			2.07E+02	1.7E+00	1.5E+00	4.8E+00					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T06-C	1	1.57E+02			1.57E+02	3.3E+00	1.5E+00	4.8E+00					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T07-C	1	7.38E+01			7.38E+01	2.1E+00	1.5E+00	4.8E+00					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T08-C	1	7.99E+01			7.99E+01	2.8E+00	1.5E+00	4.8E+00					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-T09-C	1	6.50E+03			6.50E+03	4.7E-01	1.5E+00	4.8E+00					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-B01-A	1	4.59E+00	E		4.59E+00	3.6E+01	1.5E+00	4.8E+00					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-B02-A	1	7.50E-01	U1/2		7.50E-01	2.8E+02	1.5E+00	4.8E+00					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-B03-A	1	3.59E+00	E		3.59E+00	5.0E+01	1.5E+00	4.8E+00					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-B01-B	1	2.12E+00	E		2.12E+00	5.1E+01	1.5E+00	4.8E+00					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-B02-B	1	4.67E+00	E		4.67E+00	3.9E+01	1.5E+00	4.8E+00					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-B03-B	1	3.97E+00	E		3.97E+00	6.5E+01	1.5E+00	4.8E+00					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-B01-C	1	3.59E+00	E		3.59E+00	3.3E+01	1.5E+00	4.8E+00					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-B02-C	1	2.28E+00	E		2.28E+00	1.7E+01	1.5E+00	4.8E+00					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1313-B03-C	1	3.30E+00	E		3.30E+00	1.3E+02	1.5E+00	4.8E+00					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	EaFA-LRef-1313-T01-A	1	5.67E+01			5.67E+01	1.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:18 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T02-A	1	5.00E-01	U1/2		5.00E-01	9.7E+00	1.0E+00	3.2E+00	10	325	3.80E+03	117%	VU ICP-OES	5/6/10 8:20 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T03-A	1	5.00E-01	U1/2		5.00E-01	3.0E+01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:22 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T04-A	1	5.00E-01	U1/2		5.00E-01	1.6E+01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:23 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T05-A	1	5.00E-01	U1/2		5.00E-01	5.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:25 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T06-A	1	5.00E-01	U1/2		5.00E-01	2.0E+01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T07-A	1	1.14E+03			1.14E+03	9.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:28 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T08-A	1	1.16E+03			1.16E+03	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:30 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T09-A	1	1.63E+03			1.63E+03	6.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:31 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T01-B	1	7.31E+01			7.31E+01	3.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:41 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T02-B	1	5.00E-01	U1/2		5.00E-01	2.1E+02	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:43 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T03-B	1	5.00E-01	U1/2		5.00E-01	2.9E+00	1.0E+00	3.2E+00	10	325	3.25E+03	100%	VU ICP-OES	5/6/10 8:45 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T04-B	1	5.00E-01	U1/2		5.00E-01	1.7E+01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:46 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T05-B	1	5.00E-01	U1/2		5.00E-01	1.4E+01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:48 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T06-B	1	5.00E-01	U1/2		5.00E-01	3.6E+01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T07-B	1	8.63E+02			8.63E+02	3.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:51 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T08-B	1	1.16E+03			1.16E+03	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:53 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T09-B	1	1.63E+03			1.63E+03	5.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:54 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T01-C	1	6.51E+01			6.51E+01	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 9:04 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T02-C	1	5.00E-01	U1/2		5.00E-01	1.0E+02	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 9:06 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T03-C	1	5.00E-01	U1/2		5.00E-01	1.1E+01	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 9:08 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T04-C	1	5.00E-01	U1/2		5.00E-01	7.5E+01	1.0E+00	3.2E+00	10	325	3.19E+03	98%	VU ICP-OES	5/6/10 9:09 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T05-C	1	5.00E-01	U1/2		5.00E-01	1.0E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:11 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T06-C	1	5.00E-01	U1/2		5.00E-01	9.5E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T07-C	1	1.06E+03			1.06E+03	6.3E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:14 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T08-C	1	1.13E+03			1.13E+03	1.7E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:16 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-T09-C	1	1.62E+03			1.62E+03	7.0E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	4.6E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.3E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:15 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	4.7E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:17 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	3.9E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:36 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	9.2E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:38 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	4.0E+04	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:40 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	1.0E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 8:59 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	5.6E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:01 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	2.7E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:03 AM	EPA Interlab LRef A-C 1313-1316 EaFA

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	EaFA-LRef-1313-T01-D	1	4.02E+04			4.02E+04	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T02-D	1	3.49E+04			3.49E+04	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T03-D	1	2.55E+04			2.55E+04	6.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T04-D	1	1.24E+04			1.24E+04	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T05-D	1	1.14E+03			1.14E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T06-D	1	2.26E+02			2.26E+02	1.0E+00	1.0E+00	3.2E+00	1000	100	1.28E+03	105%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T07-D	1	2.73E+02			2.73E+02	9.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T08-D	1	3.09E+04			3.09E+04	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T09-D	1	1.27E+05			1.27E+05	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T01-E	1	3.86E+04			3.86E+04	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T02-E	1	3.52E+04			3.52E+04	7.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T03-E	1	2.67E+04			2.67E+04	3.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T04-E	1	1.44E+04			1.44E+04	5.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T05-E	1	1.14E+03			1.14E+03	1.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T06-E	1	2.74E+02			2.74E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T07-E	1	1.96E+02			1.96E+02	3.0E+00	1.0E+00	3.2E+00	1000	100	1.23E+03	103%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T08-E	1	3.07E+04			3.07E+04	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T09-E	1	1.24E+05			1.24E+05	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T01-F	1	3.99E+04			3.99E+04	6.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T02-F	1	3.45E+04			3.45E+04	4.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T03-F	1	2.62E+04			2.62E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T04-F	1	1.40E+04			1.40E+04	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T05-F	1	1.30E+03			1.30E+03	2.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T06-F	1	2.14E+02			2.14E+02	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T07-F	1	2.77E+02			2.77E+02	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T08-F	1	3.12E+04			3.12E+04	7.7E-01	1.0E+00	3.2E+00	1000	100	3.23E+04	105%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-T09-F	1	1.25E+05			1.25E+05	8.8E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-B01-D	1	5.00E-01	U1/2		5.00E-01	2.4E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-B02-D	1	2.50E+00	E		2.50E+00	1.1E+02	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-B03-D	1	1.27E+01			1.27E+01	1.3E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-B01-E	1	5.00E-01	U1/2		5.00E-01	7.4E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-B02-E	1	1.62E+01			1.62E+01	2.4E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-B03-E	1	2.77E+01			2.77E+01	4.2E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-B01-F	1	5.00E-01	U1/2		5.00E-01	1.6E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-B02-F	1	2.24E+01			2.24E+01	2.4E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1313-B03-F	1	4.07E+01			4.07E+01	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	EaFA-LRef-1313-T01-D	1	2.01E+02			2.01E+02	2.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T02-D	1	1.27E+02			1.27E+02	1.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T03-D	1	1.21E+02			1.21E+02	2.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T04-D	1	1.08E+02			1.08E+02	2.4E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T05-D	1	1.28E+02			1.28E+02	2.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T06-D	1	1.15E+02			1.15E+02	1.8E+01	7.5E+00	2.4E+01	10	325	3.39E+03	101%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T07-D	1	6.81E+01			6.81E+01	6.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T08-D	1	2.59E+01			2.59E+01	4.9E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T09-D	1	3.75E+00	U1/2		3.75E+00	1.1E+02	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T01-E	1	1.74E+02			1.74E+02	2.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T02-E	1	1.17E+02			1.17E+02	1.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T03-E	1	1.06E+02			1.06E+02	1.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T04-E	1	1.37E+02			1.37E+02	3.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T05-E	1	1.25E+02			1.25E+02	3.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T06-E	1	1.14E+02			1.14E+02	2.8E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T07-E	1	5.66E+01			5.66E+01	4.5E+01	7.5E+00	2.4E+01	10	325	3.37E+03	102%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T08-E	1	2.13E+01	E		2.13E+01	9.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T09-E	1	3.75E+00	U1/2		3.75E+00	1.1E+02	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T01-F	1	1.88E+02			1.88E+02	1.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T02-F	1	1.03E+02			1.03E+02	3.8E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T03-F	1	1.29E+02			1.29E+02	6.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T04-F	1	1.46E+02			1.46E+02	9.4E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T05-F	1	1.30E+02			1.30E+02	1.6E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T06-F	1	1.34E+02			1.34E+02	3.4E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T07-F	1	6.09E+01			6.09E+01	5.8E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T08-F	1	1.90E+01	E		1.90E+01	1.1E+01	7.5E+00	2.4E+01	10	325	3.32E+03	102%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-T09-F	1	3.75E+00	U1/2		3.75E+00	6.8E+01	7.5E+00	2.4E+01					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-B01-D	1	3.75E+00	U1/2		3.75E+00	2.2E+02	7.5E+00	2.4E+01					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-B02-D	1	3.75E+00	U1/2		3.75E+00	7.3E+02	7.5E+00	2.4E+01					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-B03-D	1	3.08E+01			3.08E+01	5.9E+01	7.5E+00	2.4E+01					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-B01-E	1	3.75E+00	U1/2		3.75E+00	2.0E+02	7.5E+00	2.4E+01					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-B02-E	1	3.75E+00	U1/2		3.75E+00	3.0E+02	7.5E+00	2.4E+01					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-B03-E	1	2.14E+01	E		2.14E+01	7.6E+01	7.5E+00	2.4E+01					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-B01-F	1	3.75E+00	U1/2		3.75E+00	6.5E+02	7.5E+00	2.4E+01					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-B02-F	1	3.75E+00	U1/2		3.75E+00	3.1E+02	7.5E+00	2.4E+01					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1313-B03-F	1	1.48E+01	E		1.48E+01	2.1E+02	7.5E+00	2.4E+01					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	EaFA-LRef-1313-T01-D	1	9.35E+03			9.35E+03	1.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T02-D	1	8.30E+02			8.30E+02	2.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T03-D	1	8.57E+02			8.57E+02	2.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T04-D	1	4.69E+02			4.69E+02	3.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T05-D	1	1.41E+02			1.41E+02	2.7E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T06-D	1	7.20E+01			7.20E+01	1.9E+01	1.1E+01	3.5E+01	10	325	3.26E+03	98%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T07-D	1	3.74E+01			3.74E+01	3.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T08-D	1	8.52E+01			8.52E+01	5.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T09-D	1	1.40E+03			1.40E+03	7.0E-01	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T01-E	1	8.64E+03			8.64E+03	7.3E-01	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T02-E	1	7.66E+02			7.66E+02	3.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T03-E	1	8.89E+02			8.89E+02	3.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T04-E	1	4.60E+02			4.60E+02	6.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T05-E	1	1.58E+02			1.58E+02	9.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T06-E	1	8.41E+01			8.41E+01	2.1E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T07-E	1	7.18E+01			7.18E+01	2.3E+01	1.1E+01	3.5E+01	10	325	3.26E+03	98%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T08-E	1	8.77E+01			8.77E+01	2.0E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T09-E	1	1.50E+03			1.50E+03	1.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T01-F	1	9.11E+03			9.11E+03	1.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T02-F	1	7.79E+02			7.79E+02	2.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T03-F	1	9.07E+02			9.07E+02	2.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T04-F	1	4.47E+02			4.47E+02	9.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T05-F	1	1.47E+02			1.47E+02	1.7E+00	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T06-F	1	5.51E+01			5.51E+01	3.0E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T07-F	1	4.73E+01			4.73E+01	1.6E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T08-F	1	9.08E+01			9.08E+01	1.3E+01	1.1E+01	3.5E+01	10	325	3.38E+03	101%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-T09-F	1	1.47E+03			1.47E+03	1.2E-01	1.1E+01	3.5E+01					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-B01-D	1	5.50E+00	U1/2		5.50E+00	4.0E+02	1.1E+01	3.5E+01					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-B02-D	1	5.50E+00	U1/2		5.50E+00	2.5E+02	1.1E+01	3.5E+01					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-B03-D	1	2.35E+01	E		2.35E+01	1.1E+02	1.1E+01	3.5E+01					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-B01-E	1	5.50E+00	U1/2		5.50E+00	1.4E+02	1.1E+01	3.5E+01					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-B02-E	1	5.50E+00	U1/2		5.50E+00	7.0E+01	1.1E+01	3.5E+01					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-B03-E	1	2.17E+01	E		2.17E+01	2.8E+01	1.1E+01	3.5E+01					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-B01-F	1	5.50E+00	U1/2		5.50E+00	9.2E+01	1.1E+01	3.5E+01					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-B02-F	1	5.50E+00	U1/2		5.50E+00	5.9E+01	1.1E+01	3.5E+01					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1313-B03-F	1	4.31E+01			4.31E+01	4.5E+01	1.1E+01	3.5E+01					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	EaFA-LRef-1313-T01-D	1	4.74E+03			4.74E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T02-D	1	4.27E+03			4.27E+03	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T03-D	1	4.20E+03			4.20E+03	5.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T04-D	1	4.20E+03			4.20E+03	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T05-D	1	4.24E+03			4.24E+03	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T06-D	1	4.49E+03			4.49E+03	7.3E-01	1.0E+00	3.2E+00	1000	100	5.30E+03	82%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T07-D	1	4.82E+03			4.82E+03	9.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T08-D	1	3.81E+03			3.81E+03	4.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T09-D	1	3.17E+03			3.17E+03	8.7E-02	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T01-E	1	4.42E+03			4.42E+03	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T02-E	1	4.31E+03			4.31E+03	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T03-E	1	4.34E+03			4.34E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T04-E	1	4.35E+03			4.35E+03	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T05-E	1	4.36E+03			4.36E+03	8.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T06-E	1	4.49E+03			4.49E+03	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T07-E	1	4.91E+03			4.91E+03	8.6E-01	1.0E+00	3.2E+00	1000	100	5.80E+03	90%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T08-E	1	3.82E+03			3.82E+03	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T09-E	1	3.20E+03			3.20E+03	7.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T01-F	1	4.73E+03			4.73E+03	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T02-F	1	4.34E+03			4.34E+03	8.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T03-F	1	4.22E+03			4.22E+03	9.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T04-F	1	4.31E+03			4.31E+03	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T05-F	1	4.44E+03			4.44E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T06-F	1	4.45E+03			4.45E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T07-F	1	4.89E+03			4.89E+03	1.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T08-F	1	3.84E+03			3.84E+03	3.8E-01	1.0E+00	3.2E+00	1000	100	4.88E+03	104%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-T09-F	1	3.21E+03			3.21E+03	3.7E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-B01-D	1	1.56E+01			1.56E+01	7.4E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-B02-D	1	4.07E+01			4.07E+01	3.6E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-B03-D	1	1.32E+02			1.32E+02	7.3E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-B01-E	1	1.87E+01			1.87E+01	5.3E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-B02-E	1	4.19E+01			4.19E+01	3.0E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-B03-E	1	1.66E+02			1.66E+02	8.9E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-B01-F	1	1.98E+01			1.98E+01	8.2E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-B02-F	1	4.26E+01			4.26E+01	2.8E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1313-B03-F	1	1.93E+02			1.93E+02	7.4E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	EaFA-LRef-1313-T01-D	1	1.02E+03			1.02E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T02-D	1	9.34E+02			9.34E+02	9.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T03-D	1	7.96E+02			7.96E+02	4.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T04-D	1	4.02E+02			4.02E+02	2.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T05-D	1	2.56E+02			2.56E+02	9.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T06-D	1	2.45E+02			2.45E+02	6.7E-01	1.0E+00	3.2E+00	10	325	3.05E+03	86%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T07-D	1	2.62E+02			2.62E+02	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T08-D	1	2.33E+02			2.33E+02	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T09-D	1	8.94E+02			8.94E+02	1.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T01-E	1	1.01E+03			1.01E+03	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T02-E	1	9.06E+02			9.06E+02	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T03-E	1	8.30E+02			8.30E+02	4.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T04-E	1	5.18E+02			5.18E+02	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T05-E	1	2.77E+02			2.77E+02	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T06-E	1	2.46E+02			2.46E+02	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T07-E	1	2.67E+02			2.67E+02	1.4E+00	1.0E+00	3.2E+00	10	325	3.16E+03	89%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T08-E	1	2.29E+02			2.29E+02	8.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T09-E	1	8.75E+02			8.75E+02	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T01-F	1	1.03E+03			1.03E+03	9.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T02-F	1	9.02E+02			9.02E+02	9.7E-02	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T03-F	1	7.42E+02			7.42E+02	6.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T04-F	1	4.94E+02			4.94E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T05-F	1	2.81E+02			2.81E+02	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T06-F	1	2.29E+02			2.29E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T07-F	1	2.57E+02			2.57E+02	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T08-F	1	2.05E+02			2.05E+02	1.1E+00	1.0E+00	3.2E+00	10	325	3.20E+03	92%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-T09-F	1	8.70E+02			8.70E+02	3.7E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-B01-D	1	5.00E-01	U1/2		5.00E-01	1.8E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-B02-D	1	5.00E-01	U1/2		5.00E-01	2.7E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-B03-D	1	5.00E-01	U1/2		5.00E-01	4.9E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-B01-E	1	5.00E-01	U1/2		5.00E-01	6.5E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-B02-E	1	5.00E-01	U1/2		5.00E-01	2.4E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-B03-E	1	5.00E-01	U1/2		5.00E-01	6.5E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-B01-F	1	5.00E-01	U1/2		5.00E-01	9.1E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-B02-F	1	5.00E-01	U1/2		5.00E-01	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1313-B03-F	1	5.00E-01	U1/2		5.00E-01	5.8E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	EaFA-LRef-1313-T01-D	1	9.50E-01	U1/2		9.50E-01	4.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T02-D	1	9.50E-01	U1/2		9.50E-01	7.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T03-D	1	9.50E-01	U1/2		9.50E-01	2.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T04-D	1	9.50E-01	U1/2		9.50E-01	8.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T05-D	1	9.50E-01	U1/2		9.50E-01	1.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T06-D	1	9.50E-01	U1/2		9.50E-01	1.3E+01	1.9E+00	6.0E+00	10	325	3.02E+03	93%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T07-D	1	9.50E-01	U1/2		9.50E-01	4.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T08-D	1	1.21E+02			1.21E+02	2.2E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T09-D	1	2.64E+02			2.64E+02	1.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T01-E	1	9.50E-01	U1/2		9.50E-01	2.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T02-E	1	9.50E-01	U1/2		9.50E-01	1.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T03-E	1	9.50E-01	U1/2		9.50E-01	8.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T04-E	1	9.50E-01	U1/2		9.50E-01	1.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T05-E	1	9.50E-01	U1/2		9.50E-01	4.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T06-E	1	9.50E-01	U1/2		9.50E-01	8.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T07-E	1	9.50E-01	U1/2		9.50E-01	5.9E+01	1.9E+00	6.0E+00	10	325	3.10E+03	95%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T08-E	1	1.21E+02			1.21E+02	3.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T09-E	1	2.63E+02			2.63E+02	5.8E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T01-F	1	9.50E-01	U1/2		9.50E-01	4.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T02-F	1	9.50E-01	U1/2		9.50E-01	1.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T03-F	1	9.50E-01	U1/2		9.50E-01	1.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T04-F	1	9.50E-01	U1/2		9.50E-01	5.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T05-F	1	9.50E-01	U1/2		9.50E-01	5.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T06-F	1	9.50E-01	U1/2		9.50E-01	1.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T07-F	1	9.50E-01	U1/2		9.50E-01	8.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T08-F	1	1.22E+02			1.22E+02	7.8E-01	1.9E+00	6.0E+00	10	325	3.12E+03	92%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-T09-F	1	2.63E+02			2.63E+02	1.4E-01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-B01-D	1	9.50E-01	U1/2		9.50E-01	5.0E+00	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-B02-D	1	9.50E-01	U1/2		9.50E-01	5.0E+00	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-B03-D	1	9.50E-01	U1/2		9.50E-01	4.5E+00	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-B01-E	1	9.50E-01	U1/2		9.50E-01	7.2E+00	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-B02-E	1	9.50E-01	U1/2		9.50E-01	9.9E+00	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-B03-E	1	9.50E-01	U1/2		9.50E-01	3.8E+00	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-B01-F	1	9.50E-01	U1/2		9.50E-01	6.4E+00	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-B02-F	1	9.50E-01	U1/2		9.50E-01	1.2E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1313-B03-F	1	9.50E-01	U1/2		9.50E-01	7.9E+00	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	EaFA-LRef-1313-T01-D	1	1.10E+00	U1/2		1.10E+00	5.6E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T02-D	1	1.10E+00	U1/2		1.10E+00	2.3E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T03-D	1	1.10E+00	U1/2		1.10E+00	4.9E+00	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T04-D	1	1.10E+00	U1/2		1.10E+00	2.6E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T05-D	1	1.10E+00	U1/2		1.10E+00	5.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T06-D	1	1.10E+00	U1/2		1.10E+00	5.2E+01	2.2E+00	7.0E+00	10	325	3.28E+03	101%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T07-D	1	2.97E+01			2.97E+01	8.8E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T08-D	1	2.73E+01			2.73E+01	1.7E+00	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T09-D	1	2.92E+01			2.92E+01	1.6E+00	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T01-E	1	1.10E+00	U1/2		1.10E+00	1.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T02-E	1	1.10E+00	U1/2		1.10E+00	6.3E+00	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T03-E	1	1.10E+00	U1/2		1.10E+00	9.4E+00	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T04-E	1	1.10E+00	U1/2		1.10E+00	2.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T05-E	1	1.10E+00	U1/2		1.10E+00	2.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T06-E	1	1.10E+00	U1/2		1.10E+00	4.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T07-E	1	2.69E+01			2.69E+01	3.2E+00	2.2E+00	7.0E+00	10	325	3.26E+03	99%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T08-E	1	2.65E+01			2.65E+01	1.6E+00	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T09-E	1	2.83E+01			2.83E+01	2.4E+00	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T01-F	1	1.10E+00	U1/2		1.10E+00	2.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T02-F	1	1.10E+00	U1/2		1.10E+00	1.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T03-F	1	1.10E+00	U1/2		1.10E+00	1.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T04-F	1	1.10E+00	U1/2		1.10E+00	1.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T05-F	1	1.10E+00	U1/2		1.10E+00	2.6E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T06-F	1	1.10E+00	U1/2		1.10E+00	2.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T07-F	1	2.85E+01			2.85E+01	7.7E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T08-F	1	2.71E+01			2.71E+01	1.2E+00	2.2E+00	7.0E+00	10	325	3.16E+03	96%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-T09-F	1	2.91E+01			2.91E+01	1.1E+00	2.2E+00	7.0E+00					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-B01-D	1	1.10E+00	U1/2		1.10E+00	1.4E+01	2.2E+00	7.0E+00					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-B02-D	1	1.10E+00	U1/2		1.10E+00	3.3E+01	2.2E+00	7.0E+00					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-B03-D	1	1.10E+00	U1/2		1.10E+00	3.5E+01	2.2E+00	7.0E+00					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-B01-E	1	1.10E+00	U1/2		1.10E+00	1.1E+01	2.2E+00	7.0E+00					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-B02-E	1	1.10E+00	U1/2		1.10E+00	8.1E+00	2.2E+00	7.0E+00					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-B03-E	1	1.10E+00	U1/2		1.10E+00	5.7E+01	2.2E+00	7.0E+00					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-B01-F	1	1.10E+00	U1/2		1.10E+00	7.4E+00	2.2E+00	7.0E+00					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-B02-F	1	1.10E+00	U1/2		1.10E+00	5.6E+01	2.2E+00	7.0E+00					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1313-B03-F	1	1.10E+00	U1/2		1.10E+00	2.6E+01	2.2E+00	7.0E+00					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	EaFA-LRef-1313-T01-D	1	1.15E+04			1.15E+04	1.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T02-D	1	4.57E+04			4.57E+04	6.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T03-D	1	8.77E+04			8.77E+04	3.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T04-D	1	1.09E+05			1.09E+05	1.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T05-D	1	1.29E+05			1.29E+05	7.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T06-D	1	1.43E+05			1.43E+05	2.4E-01	2.6E+00	8.3E+00	1000	100	1.44E+05	89%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T07-D	1	1.58E+05			1.58E+05	7.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T08-D	1	1.36E+05			1.36E+05	7.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T09-D	1	1.37E+05			1.37E+05	5.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T01-E	1	1.11E+04			1.11E+04	2.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T02-E	1	4.68E+04			4.68E+04	5.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T03-E	1	9.11E+04			9.11E+04	9.5E-02	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T04-E	1	1.10E+05			1.10E+05	5.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T05-E	1	1.33E+05			1.33E+05	9.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T06-E	1	1.43E+05			1.43E+05	8.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T07-E	1	1.59E+05			1.59E+05	9.8E-01	2.6E+00	8.3E+00	1000	100	1.60E+05	84%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T08-E	1	1.34E+05			1.34E+05	3.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T09-E	1	1.35E+05			1.35E+05	5.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T01-F	1	1.15E+04			1.15E+04	1.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T02-F	1	4.74E+04			4.74E+04	1.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T03-F	1	8.93E+04			8.93E+04	1.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T04-F	1	1.09E+05			1.09E+05	6.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T05-F	1	1.36E+05			1.36E+05	7.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T06-F	1	1.41E+05			1.41E+05	1.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T07-F	1	1.56E+05			1.56E+05	3.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T08-F	1	1.37E+05			1.37E+05	6.9E-01	2.6E+00	8.3E+00	1000	100	1.38E+05	90%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-T09-F	1	1.36E+05			1.36E+05	2.9E-01	2.6E+00	8.3E+00					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-B01-D	1	3.36E+01			3.36E+01	2.6E+01	2.6E+00	8.3E+00					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-B02-D	1	2.62E+01			2.62E+01	8.1E+01	2.6E+00	8.3E+00					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-B03-D	1	2.32E+01			2.32E+01	3.9E+01	2.6E+00	8.3E+00					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-B01-E	1	2.44E+01			2.44E+01	5.3E+01	2.6E+00	8.3E+00					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-B02-E	1	4.14E+01			4.14E+01	6.4E+00	2.6E+00	8.3E+00					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-B03-E	1	1.45E+01			1.45E+01	4.3E+01	2.6E+00	8.3E+00					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-B01-F	1	2.30E+01			2.30E+01	2.0E+01	2.6E+00	8.3E+00					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-B02-F	1	2.73E+01			2.73E+01	2.1E+01	2.6E+00	8.3E+00					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1313-B03-F	1	1.01E+01			1.01E+01	1.1E+02	2.6E+00	8.3E+00					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	EaFA-LRef-1313-T01-D	1	5.05E+02			5.05E+02	2.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T02-D	1	3.25E+02			3.25E+02	6.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T03-D	1	2.57E+02			2.57E+02	4.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T04-D	1	2.30E+02			2.30E+02	1.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T05-D	1	1.41E+02			1.41E+02	4.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T06-D	1	5.32E+01			5.32E+01	4.1E+00	1.2E+00	3.8E+00	10	325	3.25E+03	98%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T07-D	1	2.10E+00	E		2.10E+00	5.8E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T08-D	1	1.62E+02			1.62E+02	7.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T09-D	1	1.90E+03			1.90E+03	8.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T01-E	1	4.81E+02			4.81E+02	1.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T02-E	1	3.23E+02			3.23E+02	7.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T03-E	1	2.62E+02			2.62E+02	4.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T04-E	1	2.19E+02			2.19E+02	3.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T05-E	1	1.50E+02			1.50E+02	8.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T06-E	1	6.91E+01			6.91E+01	2.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T07-E	1	3.06E+00	E		3.06E+00	4.3E+01	1.2E+00	3.8E+00	10	325	3.21E+03	99%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T08-E	1	1.63E+02			1.63E+02	4.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T09-E	1	1.91E+03			1.91E+03	2.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T01-F	1	4.95E+02			4.95E+02	9.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T02-F	1	3.16E+02			3.16E+02	3.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T03-F	1	2.53E+02			2.53E+02	1.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T04-F	1	2.11E+02			2.11E+02	1.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T05-F	1	1.44E+02			1.44E+02	1.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T06-F	1	5.64E+01			5.64E+01	1.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T07-F	1	6.00E-01	U1/2		6.00E-01	1.3E+02	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T08-F	1	1.64E+02			1.64E+02	4.8E-01	1.2E+00	3.8E+00	10	325	3.15E+03	92%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-T09-F	1	1.92E+03			1.92E+03	5.3E-01	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-B01-D	1	6.00E-01	U1/2		6.00E-01	1.4E+01	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-B02-D	1	6.00E-01	U1/2		6.00E-01	1.0E+02	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-B03-D	1	2.90E+00	E		2.90E+00	9.5E+01	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-B01-E	1	6.00E-01	U1/2		6.00E-01	9.6E+01	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-B02-E	1	6.00E-01	U1/2		6.00E-01	1.4E+02	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-B03-E	1	2.30E+00	E		2.30E+00	1.5E+01	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-B01-F	1	6.00E-01	U1/2		6.00E-01	9.0E+01	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-B02-F	1	6.00E-01	U1/2		6.00E-01	3.7E+00	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1313-B03-F	1	3.19E+00	E		3.19E+00	8.7E+01	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	EaFA-LRef-1313-T01-D	1	9.00E-01	U1/2		9.00E-01	2.2E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T02-D	1	9.00E-01	U1/2		9.00E-01	3.2E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T03-D	1	9.00E-01	U1/2		9.00E-01	8.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T04-D	1	9.00E-01	U1/2		9.00E-01	4.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T05-D	1	3.39E+00	E		3.39E+00	5.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T06-D	1	2.20E+01			2.20E+01	1.3E+01	1.8E+00	5.7E+00	10	325	3.32E+03	102%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T07-D	1	2.43E+02			2.43E+02	1.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T08-D	1	2.09E+02			2.09E+02	3.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T09-D	1	4.17E+02			4.17E+02	6.4E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T01-E	1	9.00E-01	U1/2		9.00E-01	1.9E+04	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T02-E	1	9.00E-01	U1/2		9.00E-01	8.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T03-E	1	9.00E-01	U1/2		9.00E-01	1.8E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T04-E	1	9.00E-01	U1/2		9.00E-01	1.8E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T05-E	1	2.84E+00	E		2.84E+00	1.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T06-E	1	1.64E+01			1.64E+01	1.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T07-E	1	2.34E+02			2.34E+02	2.0E+00	1.8E+00	5.7E+00	10	325	3.21E+03	92%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T08-E	1	2.11E+02			2.11E+02	1.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T09-E	1	4.11E+02			4.11E+02	6.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T01-F	1	9.00E-01	U1/2		9.00E-01	2.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T02-F	1	9.00E-01	U1/2		9.00E-01	2.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T03-F	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T04-F	1	9.00E-01	U1/2		9.00E-01	1.9E+03	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T05-F	1	1.91E+00	E		1.91E+00	9.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T06-F	1	2.73E+01			2.73E+01	4.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T07-F	1	2.37E+02			2.37E+02	2.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T08-F	1	2.12E+02			2.12E+02	6.1E-01	1.8E+00	5.7E+00	10	325	3.19E+03	92%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-T09-F	1	4.15E+02			4.15E+02	3.2E-01	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-B01-D	1	9.00E-01	U1/2		9.00E-01	4.8E+01	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-B02-D	1	9.00E-01	U1/2		9.00E-01	1.6E+02	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-B03-D	1	9.00E-01	U1/2		9.00E-01	2.6E+02	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-B01-E	1	9.00E-01	U1/2		9.00E-01	6.7E+01	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-B02-E	1	9.00E-01	U1/2		9.00E-01	2.3E+03	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-B03-E	1	9.00E-01	U1/2		9.00E-01	4.7E+03	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-B01-F	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-B02-F	1	9.00E-01	U1/2		9.00E-01	8.0E+03	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1313-B03-F	1	9.00E-01	U1/2		9.00E-01	5.3E+02	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	EaFA-LRef-1313-T01-D	1	2.05E+01			2.05E+01	3.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T02-D	1	1.85E+00	U1/2		1.85E+00	1.1E+02	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T03-D	1	1.85E+00	U1/2		1.85E+00	7.5E+02	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T04-D	1	1.85E+00	U1/2		1.85E+00	1.5E+02	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T05-D	1	1.85E+00	U1/2		1.85E+00	7.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T06-D	1	1.85E+00	U1/2		1.85E+00	2.8E+02	3.7E+00	1.2E+01	10	325	3.01E+03	93%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T07-D	1	7.11E+01			7.11E+01	3.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T08-D	1	1.88E+03			1.88E+03	7.2E-01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T09-D	1	3.10E+03			3.10E+03	4.4E-01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T01-E	1	2.66E+01			2.66E+01	1.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T02-E	1	1.85E+00	U1/2		1.85E+00	3.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T03-E	1	1.85E+00	U1/2		1.85E+00	4.2E+02	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T04-E	1	1.85E+00	U1/2		1.85E+00	5.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T05-E	1	1.85E+00	U1/2		1.85E+00	7.2E+02	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T06-E	1	1.85E+00	U1/2		1.85E+00	2.1E+02	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T07-E	1	4.91E+01			4.91E+01	1.3E+01	3.7E+00	1.2E+01	10	325	3.04E+03	92%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T08-E	1	1.87E+03			1.87E+03	7.9E-01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T09-E	1	3.08E+03			3.08E+03	7.1E-01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T01-F	1	2.18E+01			2.18E+01	3.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T02-F	1	1.85E+00	U1/2		1.85E+00	5.3E+02	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T03-F	1	1.85E+00	U1/2		1.85E+00	1.2E+02	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T04-F	1	1.85E+00	U1/2		1.85E+00	2.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T05-F	1	1.85E+00	U1/2		1.85E+00	1.7E+02	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T06-F	1	1.85E+00	U1/2		1.85E+00	1.0E+03	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T07-F	1	7.05E+01			7.05E+01	6.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T08-F	1	1.89E+03			1.89E+03	3.7E-01	3.7E+00	1.2E+01	10	325	5.43E+03	109%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-T09-F	1	3.11E+03			3.11E+03	4.3E-01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-B01-D	1	1.85E+00	U1/2		1.85E+00	4.5E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-B02-D	1	1.85E+00	U1/2		1.85E+00	6.4E+00	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-B03-D	1	1.85E+00	U1/2		1.85E+00	8.2E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-B01-E	1	1.85E+00	U1/2		1.85E+00	1.9E+02	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-B02-E	1	1.85E+00	U1/2		1.85E+00	1.3E+02	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-B03-E	1	1.85E+00	U1/2		1.85E+00	6.9E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-B01-F	1	1.85E+00	U1/2		1.85E+00	1.8E+02	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-B02-F	1	1.85E+00	U1/2		1.85E+00	8.3E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1313-B03-F	1	1.85E+00	U1/2		1.85E+00	8.3E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	EaFA-LRef-1313-T01-D	1	5.26E+01			5.26E+01	2.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T02-D	1	2.05E+01			2.05E+01	4.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T03-D	1	1.00E+00	U1/2		1.00E+00	1.6E+02	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T04-D	1	1.00E+00	U1/2		1.00E+00	5.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T05-D	1	1.00E+00	U1/2		1.00E+00	2.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T06-D	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00	1000	100	1.01E+03	101%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T07-D	1	1.00E+00	U1/2		1.00E+00	4.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T08-D	1	4.12E+02			4.12E+02	5.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T09-D	1	3.31E+04			3.31E+04	1.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T01-E	1	5.86E+01			5.86E+01	3.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T02-E	1	2.21E+01			2.21E+01	2.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T03-E	1	1.00E+00	U1/2		1.00E+00	9.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T04-E	1	1.00E+00	U1/2		1.00E+00	6.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T05-E	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T06-E	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T07-E	1	1.00E+00	U1/2		1.00E+00	3.6E+01	2.0E+00	6.4E+00	1000	100	9.56E+02	95%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T08-E	1	3.95E+02			3.95E+02	6.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T09-E	1	3.29E+04			3.29E+04	7.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T01-F	1	6.11E+01			6.11E+01	1.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T02-F	1	2.07E+01			2.07E+01	2.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T03-F	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T04-F	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T05-F	1	1.00E+00	U1/2		1.00E+00	7.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T06-F	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T07-F	1	1.00E+00	U1/2		1.00E+00	5.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T08-F	1	3.84E+02			3.84E+02	4.4E-01	2.0E+00	6.4E+00	1000	100	1.41E+03	102%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-T09-F	1	3.29E+04			3.29E+04	9.0E-01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-B01-D	1	1.00E+00	U1/2		1.00E+00	3.3E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-B02-D	1	2.64E+00	E		2.64E+00	1.7E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-B03-D	1	4.36E+00	E		4.36E+00	7.1E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-B01-E	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-B02-E	1	6.34E+00	E		6.34E+00	2.1E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-B03-E	1	8.07E+00			8.07E+00	5.2E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-B01-F	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-B02-F	1	7.98E+00			7.98E+00	1.9E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1313-B03-F	1	4.07E+00	E		4.07E+00	3.3E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	EaFA-LRef-1313-T01-D	1	3.40E+00	U1/2		3.40E+00	4.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T02-D	1	3.40E+00	U1/2		3.40E+00	1.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T03-D	1	3.40E+00	U1/2		3.40E+00	8.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T04-D	1	3.40E+00	U1/2		3.40E+00	4.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T05-D	1	3.40E+00	U1/2		3.40E+00	2.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T06-D	1	3.40E+00	U1/2		3.40E+00	4.6E+01	6.8E+00	2.2E+01	10	325	3.23E+03	99%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T07-D	1	3.40E+00	U1/2		3.40E+00	3.7E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T08-D	1	3.40E+00	U1/2		3.40E+00	1.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T09-D	1	5.66E+01			5.66E+01	1.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T01-E	1	3.40E+00	U1/2		3.40E+00	6.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T02-E	1	3.40E+00	U1/2		3.40E+00	2.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T03-E	1	3.40E+00	U1/2		3.40E+00	5.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T04-E	1	3.40E+00	U1/2		3.40E+00	3.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T05-E	1	3.40E+00	U1/2		3.40E+00	7.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T06-E	1	3.40E+00	U1/2		3.40E+00	2.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T07-E	1	3.40E+00	U1/2		3.40E+00	3.2E+00	6.8E+00	2.2E+01	10	325	3.13E+03	96%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T08-E	1	3.40E+00	U1/2		3.40E+00	1.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T09-E	1	6.26E+01			6.26E+01	1.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T01-F	1	3.40E+00	U1/2		3.40E+00	2.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T02-F	1	3.40E+00	U1/2		3.40E+00	3.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T03-F	1	3.40E+00	U1/2		3.40E+00	1.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T04-F	1	3.40E+00	U1/2		3.40E+00	1.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T05-F	1	3.40E+00	U1/2		3.40E+00	3.7E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T06-F	1	3.40E+00	U1/2		3.40E+00	2.7E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T07-F	1	3.40E+00	U1/2		3.40E+00	3.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T08-F	1	3.40E+00	U1/2		3.40E+00	1.4E+01	6.8E+00	2.2E+01	10	325	3.23E+03	99%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-T09-F	1	6.15E+01			6.15E+01	4.3E+00	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-B01-D	1	3.40E+00	U1/2		3.40E+00	3.7E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-B02-D	1	3.40E+00	U1/2		3.40E+00	3.2E+00	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-B03-D	1	3.40E+00	U1/2		3.40E+00	3.5E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-B01-E	1	3.40E+00	U1/2		3.40E+00	1.5E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-B02-E	1	3.40E+00	U1/2		3.40E+00	3.4E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-B03-E	1	3.40E+00	U1/2		3.40E+00	4.5E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-B01-F	1	3.40E+00	U1/2		3.40E+00	1.5E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-B02-F	1	3.40E+00	U1/2		3.40E+00	2.0E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1313-B03-F	1	3.40E+00	U1/2		3.40E+00	2.4E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	EaFA-LRef-1313-T01-D	1	1.59E+03			1.59E+03	8.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T02-D	1	2.16E+03			2.16E+03	7.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T03-D	1	2.41E+03			2.41E+03	4.6E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T04-D	1	2.01E+03			2.01E+03	7.9E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T05-D	1	2.82E+03			2.82E+03	9.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T06-D	1	3.01E+03			3.01E+03	4.7E-01	1.9E+00	6.0E+00	10	325	6.17E+03	97%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T07-D	1	3.07E+03			3.07E+03	9.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T08-D	1	2.08E+03			2.08E+03	1.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T09-D	1	1.47E+03			1.47E+03	8.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T01-E	1	1.55E+03			1.55E+03	3.9E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T02-E	1	2.17E+03			2.17E+03	4.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T03-E	1	2.48E+03			2.48E+03	2.9E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T04-E	1	2.35E+03			2.35E+03	7.6E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T05-E	1	2.88E+03			2.88E+03	2.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T06-E	1	2.99E+03			2.99E+03	3.0E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T07-E	1	3.05E+03			3.05E+03	7.1E-01	1.9E+00	6.0E+00	10	325	5.99E+03	91%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T08-E	1	2.05E+03			2.05E+03	4.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T09-E	1	1.45E+03			1.45E+03	8.4E-02	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T01-F	1	1.60E+03			1.60E+03	1.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T02-F	1	2.17E+03			2.17E+03	9.9E-02	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T03-F	1	2.47E+03			2.47E+03	6.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T04-F	1	2.37E+03			2.37E+03	6.0E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T05-F	1	2.92E+03			2.92E+03	5.2E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T06-F	1	3.00E+03			3.00E+03	6.0E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T07-F	1	3.06E+03			3.06E+03	8.5E-02	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T08-F	1	2.07E+03			2.07E+03	4.9E-01	1.9E+00	6.0E+00	10	325	4.98E+03	89%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-T09-F	1	1.46E+03			1.46E+03	2.1E-01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-B01-D	1	2.52E+00	E		2.52E+00	4.5E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-B02-D	1	2.20E+00	E		2.20E+00	4.5E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-B03-D	1	2.50E+00	E		2.50E+00	6.9E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-B01-E	1	2.95E+00	E		2.95E+00	4.5E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-B02-E	1	3.44E+00	E		3.44E+00	1.2E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-B03-E	1	3.65E+00	E		3.65E+00	7.6E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-B01-F	1	2.42E+00	E		2.42E+00	8.5E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-B02-F	1	3.13E+00	E		3.13E+00	1.6E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1313-B03-F	1	2.32E+00	E		2.32E+00	7.4E+01	1.9E+00	6.0E+00					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	EaFA-LRef-1313-T01-D	1	1.00E+00	U1/2		1.00E+00	5.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T02-D	1	1.00E+00	U1/2		1.00E+00	1.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T03-D	1	1.00E+00	U1/2		1.00E+00	6.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T04-D	1	1.00E+00	U1/2		1.00E+00	4.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T05-D	1	3.38E+01			3.38E+01	1.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T06-D	1	2.32E+02			2.32E+02	1.2E+00	2.0E+00	6.4E+00	10	325	3.21E+03	92%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T07-D	1	9.36E+02			9.36E+02	2.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T08-D	1	1.15E+03			1.15E+03	2.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T09-D	1	1.81E+03			1.81E+03	5.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T01-E	1	1.00E+00	U1/2		1.00E+00	6.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T02-E	1	1.00E+00	U1/2		1.00E+00	5.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T03-E	1	1.00E+00	U1/2		1.00E+00	7.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T04-E	1	1.00E+00	U1/2		1.00E+00	2.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T05-E	1	3.42E+01			3.42E+01	7.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T06-E	1	1.87E+02			1.87E+02	3.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T07-E	1	9.27E+02			9.27E+02	5.5E-01	2.0E+00	6.4E+00	10	325	3.84E+03	90%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T08-E	1	1.13E+03			1.13E+03	1.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T09-E	1	1.78E+03			1.78E+03	5.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T01-F	1	1.00E+00	U1/2		1.00E+00	8.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T02-F	1	1.00E+00	U1/2		1.00E+00	9.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T03-F	1	1.00E+00	U1/2		1.00E+00	4.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T04-F	1	1.00E+00	U1/2		1.00E+00	3.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T05-F	1	3.12E+01			3.12E+01	3.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T06-F	1	2.33E+02			2.33E+02	4.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T07-F	1	9.39E+02			9.39E+02	5.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T08-F	1	1.15E+03			1.15E+03	5.2E-01	2.0E+00	6.4E+00	10	325	4.05E+03	89%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-T09-F	1	1.79E+03			1.79E+03	6.3E-01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-B01-D	1	1.00E+00	U1/2		1.00E+00	3.9E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-B02-D	1	1.00E+00	U1/2		1.00E+00	4.6E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-B03-D	1	1.00E+00	U1/2		1.00E+00	5.8E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-B01-E	1	1.00E+00	U1/2		1.00E+00	7.7E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-B02-E	1	1.00E+00	U1/2		1.00E+00	2.4E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-B03-E	1	1.00E+00	U1/2		1.00E+00	5.1E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-B01-F	1	1.00E+00	U1/2		1.00E+00	6.7E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-B02-F	1	1.00E+00	U1/2		1.00E+00	3.8E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1313-B03-F	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	EaFA-LRef-1313-T01-D	1	5.00E-01	U1/2		5.00E-01	4.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T02-D	1	5.00E-01	U1/2		5.00E-01	2.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T03-D	1	2.90E+02			2.90E+02	2.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T04-D	1	2.31E+03			2.31E+03	5.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T05-D	1	5.14E+03			5.14E+03	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T06-D	1	7.15E+03			7.15E+03	1.2E+00	1.0E+00	3.2E+00	1000	100	8.11E+03	96%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T07-D	1	8.59E+03			8.59E+03	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T08-D	1	7.61E+03			7.61E+03	9.0E-02	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T09-D	1	1.39E+04			1.39E+04	6.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T01-E	1	5.00E-01	U1/2		5.00E-01	1.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T02-E	1	5.00E-01	U1/2		5.00E-01	4.7E+02	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T03-E	1	2.19E+02			2.19E+02	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T04-E	1	2.81E+03			2.81E+03	8.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T05-E	1	5.37E+03			5.37E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T06-E	1	7.05E+03			7.05E+03	2.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T07-E	1	8.64E+03			8.64E+03	8.4E-01	1.0E+00	3.2E+00	1000	100	9.74E+03	110%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T08-E	1	7.60E+03			7.60E+03	5.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T09-E	1	1.40E+04			1.40E+04	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T01-F	1	5.00E-01	U1/2		5.00E-01	4.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T02-F	1	5.00E-01	U1/2		5.00E-01	6.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T03-F	1	2.65E+02			2.65E+02	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T04-F	1	2.92E+03			2.92E+03	9.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T05-F	1	5.46E+03			5.46E+03	5.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T06-F	1	7.11E+03			7.11E+03	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T07-F	1	8.59E+03			8.59E+03	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T08-F	1	7.71E+03			7.71E+03	7.6E-01	1.0E+00	3.2E+00	1000	100	8.63E+03	92%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-T09-F	1	1.40E+04			1.40E+04	1.7E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-B01-D	1	5.00E-01	U1/2		5.00E-01	1.3E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-B02-D	1	5.00E-01	U1/2		5.00E-01	5.5E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-B03-D	1	5.00E-01	U1/2		5.00E-01	3.3E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-B01-E	1	5.00E-01	U1/2		5.00E-01	1.9E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-B02-E	1	5.00E-01	U1/2		5.00E-01	2.8E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-B03-E	1	5.00E-01	U1/2		5.00E-01	2.6E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-B01-F	1	5.00E-01	U1/2		5.00E-01	1.4E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-B02-F	1	5.00E-01	U1/2		5.00E-01	1.4E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1313-B03-F	1	5.00E-01	U1/2		5.00E-01	2.4E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	EaFA-LRef-1313-T01-D	1	4.01E+03			4.01E+03	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T02-D	1	3.66E+03			3.66E+03	8.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T03-D	1	3.51E+03			3.51E+03	7.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T04-D	1	3.48E+03			3.48E+03	5.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T05-D	1	3.29E+03			3.29E+03	9.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T06-D	1	3.11E+03			3.11E+03	4.0E-01	1.2E+00	3.8E+00	10	325	6.07E+03	91%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T07-D	1	5.51E+02			5.51E+02	1.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T08-D	1	1.05E+02			1.05E+02	1.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T09-D	1	3.00E+02			3.00E+02	5.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T01-E	1	3.90E+03			3.90E+03	4.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T02-E	1	3.74E+03			3.74E+03	6.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T03-E	1	3.68E+03			3.68E+03	6.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T04-E	1	3.55E+03			3.55E+03	4.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T05-E	1	3.39E+03			3.39E+03	9.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T06-E	1	3.18E+03			3.18E+03	7.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T07-E	1	6.59E+02			6.59E+02	1.4E+00	1.2E+00	3.8E+00	10	325	3.60E+03	91%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T08-E	1	1.02E+02			1.02E+02	6.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T09-E	1	3.15E+02			3.15E+02	2.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T01-F	1	4.08E+03			4.08E+03	5.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T02-F	1	3.72E+03			3.72E+03	2.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T03-F	1	3.61E+03			3.61E+03	8.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T04-F	1	3.52E+03			3.52E+03	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T05-F	1	3.50E+03			3.50E+03	3.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T06-F	1	3.11E+03			3.11E+03	8.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T07-F	1	5.74E+02			5.74E+02	4.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T08-F	1	9.94E+01			9.94E+01	8.2E-01	1.2E+00	3.8E+00	10	325	3.59E+03	108%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-T09-F	1	3.09E+02			3.09E+02	5.3E-01	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-B01-D	1	6.00E-01	U1/2		6.00E-01	1.6E+02	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-B02-D	1	6.00E-01	U1/2		6.00E-01	3.3E+01	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-B03-D	1	6.00E-01	U1/2		6.00E-01	1.6E+03	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-B01-E	1	6.00E-01	U1/2		6.00E-01	1.0E+02	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-B02-E	1	6.00E-01	U1/2		6.00E-01	2.8E+01	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-B03-E	1	6.00E-01	U1/2		6.00E-01	3.1E+02	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-B01-F	1	6.00E-01	U1/2		6.00E-01	7.9E+01	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-B02-F	1	6.00E-01	U1/2		6.00E-01	2.2E+02	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1313-B03-F	1	6.00E-01	U1/2		6.00E-01	3.0E+02	1.2E+00	3.8E+00					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	EaFA-LRef-1313-T01-D	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T02-D	1	9.00E-01	U1/2		9.00E-01	7.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T03-D	1	9.00E-01	U1/2		9.00E-01	2.7E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T04-D	1	9.00E-01	U1/2		9.00E-01	4.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T05-D	1	4.57E+00	E		4.57E+00	7.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T06-D	1	5.15E+01			5.15E+01	1.0E+01	1.8E+00	5.7E+00	10	325	3.14E+03	95%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T07-D	1	5.73E+02			5.73E+02	2.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T08-D	1	5.16E+02			5.16E+02	6.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T09-D	1	7.53E+02			7.53E+02	6.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T01-E	1	9.00E-01	U1/2		9.00E-01	9.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T02-E	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T03-E	1	9.00E-01	U1/2		9.00E-01	4.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T04-E	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T05-E	1	5.43E+00	E		5.43E+00	6.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T06-E	1	4.50E+01			4.50E+01	1.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T07-E	1	5.42E+02			5.42E+02	5.0E-01	1.8E+00	5.7E+00	10	325	3.48E+03	90%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T08-E	1	5.17E+02			5.17E+02	1.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T09-E	1	7.48E+02			7.48E+02	2.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T01-F	1	9.00E-01	U1/2		9.00E-01	7.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T02-F	1	9.00E-01	U1/2		9.00E-01	2.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T03-F	1	9.00E-01	U1/2		9.00E-01	4.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T04-F	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T05-F	1	7.74E+00			7.74E+00	2.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T06-F	1	5.85E+01			5.85E+01	3.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T07-F	1	5.61E+02			5.61E+02	1.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T08-F	1	5.16E+02			5.16E+02	6.9E-01	1.8E+00	5.7E+00	10	325	3.47E+03	91%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-T09-F	1	7.50E+02			7.50E+02	8.1E-01	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-B01-D	1	9.00E-01	U1/2		9.00E-01	6.0E+02	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-B02-D	1	9.00E-01	U1/2		9.00E-01	8.6E+01	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-B03-D	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-B01-E	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-B02-E	1	9.00E-01	U1/2		9.00E-01	1.0E+02	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-B03-E	1	2.07E+00	E		2.07E+00	3.9E+02	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-B01-F	1	9.00E-01	U1/2		9.00E-01	7.1E+02	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-B02-F	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1313-B03-F	1	9.00E-01	U1/2		9.00E-01	7.6E+03	1.8E+00	5.7E+00					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	EaFA-LRef-1313-T01-D	1	1.70E+02			1.70E+02	1.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T02-D	1	2.96E+01			2.96E+01	2.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T03-D	1	5.63E+01			5.63E+01	1.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T04-D	1	9.01E+01			9.01E+01	1.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T05-D	1	2.67E+01			2.67E+01	4.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T06-D	1	1.32E+01			1.32E+01	1.2E+01	3.7E+00	1.2E+01	1000	100	1.11E+03	109%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T07-D	1	1.12E+01	E		1.12E+01	1.6E+02	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T08-D	1	6.93E+01			6.93E+01	9.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T09-D	1	2.52E+03			2.52E+03	4.4E-01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T01-E	1	1.55E+02			1.55E+02	3.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T02-E	1	3.72E+01			3.72E+01	3.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T03-E	1	7.46E+01			7.46E+01	1.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T04-E	1	7.39E+01			7.39E+01	1.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T05-E	1	3.93E+01			3.93E+01	1.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T06-E	1	2.23E+01			2.23E+01	3.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T07-E	1	2.13E+01			2.13E+01	4.5E+01	3.7E+00	1.2E+01	1000	100	1.04E+03	102%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T08-E	1	7.81E+01			7.81E+01	6.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T09-E	1	2.64E+03			2.64E+03	2.0E-01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T01-F	1	1.87E+02			1.87E+02	5.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T02-F	1	2.81E+01			2.81E+01	1.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T03-F	1	7.47E+01			7.47E+01	1.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T04-F	1	9.46E+01			9.46E+01	2.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T05-F	1	4.69E+01			4.69E+01	1.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T06-F	1	2.84E+01			2.84E+01	1.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T07-F	1	2.90E+01			2.90E+01	6.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T08-F	1	6.53E+01			6.53E+01	1.8E+00	3.7E+00	1.2E+01	1000	100	1.09E+03	103%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-T09-F	1	2.65E+03			2.65E+03	6.8E-01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-B01-D	1	6.77E+00	E		6.77E+00	1.2E+02	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-B02-D	1	6.91E+00	E		6.91E+00	6.3E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-B03-D	1	3.11E+01			3.11E+01	2.1E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-B01-E	1	9.02E+00	E		9.02E+00	6.6E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-B02-E	1	1.85E+00	U1/2		1.85E+00	1.3E+02	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-B03-E	1	1.64E+01			1.64E+01	2.3E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-B01-F	1	1.50E+01			1.50E+01	3.4E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-B02-F	1	7.66E+00	E		7.66E+00	5.6E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1313-B03-F	1	6.40E+00	E		6.40E+00	4.2E+01	3.7E+00	1.2E+01					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	EaFA-LRef-1313-T01-D	1	1.62E+06			1.62E+06	1.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T02-D	1	3.77E+05			3.77E+05	7.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T03-D	1	1.63E+05			1.63E+05	5.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T04-D	1	1.15E+05			1.15E+05	5.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T05-D	1	4.90E+04			4.90E+04	5.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T06-D	1	2.30E+04			2.30E+04	3.2E-01	1.6E+00	5.1E+00	1000	100	2.38E+04	83%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T07-D	1	2.45E+04			2.45E+04	7.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T08-D	1	1.83E+04			1.83E+04	3.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T09-D	1	2.18E+04			2.18E+04	1.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T01-E	1	1.58E+06			1.58E+06	3.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T02-E	1	3.77E+05			3.77E+05	7.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T03-E	1	1.68E+05			1.68E+05	2.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T04-E	1	1.16E+05			1.16E+05	1.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T05-E	1	4.97E+04			4.97E+04	5.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T06-E	1	2.28E+04			2.28E+04	9.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T07-E	1	2.44E+04			2.44E+04	4.0E-01	1.6E+00	5.1E+00	1000	100	2.53E+04	92%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T08-E	1	1.82E+04			1.82E+04	4.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T09-E	1	2.17E+04			2.17E+04	6.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T01-F	1	1.59E+06			1.59E+06	9.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T02-F	1	3.88E+05			3.88E+05	3.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T03-F	1	1.68E+05			1.68E+05	9.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T04-F	1	1.15E+05			1.15E+05	6.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T05-F	1	5.02E+04			5.02E+04	6.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T06-F	1	2.27E+04			2.27E+04	1.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T07-F	1	2.43E+04			2.43E+04	1.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T08-F	1	1.83E+04			1.83E+04	7.6E-02	1.6E+00	5.1E+00	1000	100	1.91E+04	82%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-T09-F	1	2.19E+04			2.19E+04	4.1E-01	1.6E+00	5.1E+00					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-B01-D	1	8.00E-01	U1/2		8.00E-01	1.7E+02	1.6E+00	5.1E+00					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-B02-D	1	6.97E+02			6.97E+02	3.7E-01	1.6E+00	5.1E+00					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-B03-D	1	1.61E+06			1.61E+06	8.4E-01	1.6E+00	5.1E+00					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-B01-E	1	8.00E-01	U1/2		8.00E-01	3.6E+02	1.6E+00	5.1E+00					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-B02-E	1	7.00E+02			7.00E+02	6.0E-01	1.6E+00	5.1E+00					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-B03-E	1	1.60E+06			1.60E+06	6.9E-01	1.6E+00	5.1E+00					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-B01-F	1	8.00E-01	U1/2		8.00E-01	2.4E+03	1.6E+00	5.1E+00					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-B02-F	1	7.01E+02			7.01E+02	3.5E-01	1.6E+00	5.1E+00					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1313-B03-F	1	1.61E+06			1.61E+06	5.9E-01	1.6E+00	5.1E+00					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	EaFA-LRef-1313-T01-D	1	7.16E+03			7.16E+03	1.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T02-D	1	5.37E+03			5.37E+03	4.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T03-D	1	4.64E+03			4.64E+03	6.2E-01	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T04-D	1	3.65E+03			3.65E+03	6.1E-01	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T05-D	1	1.51E+03			1.51E+03	2.0E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T06-D	1	8.20E+02			8.20E+02	6.0E+00	1.5E+01	4.8E+01	10	325	3.80E+03	92%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T07-D	1	2.38E+02			2.38E+02	1.9E+01	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T08-D	1	6.63E+01			6.63E+01	2.4E+01	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T09-D	1	5.19E+02			5.19E+02	4.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T01-E	1	7.02E+03			7.02E+03	9.2E-01	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T02-E	1	5.47E+03			5.47E+03	4.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T03-E	1	4.85E+03			4.85E+03	3.8E-01	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T04-E	1	3.75E+03			3.75E+03	6.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T05-E	1	1.60E+03			1.60E+03	2.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T06-E	1	9.11E+02			9.11E+02	2.6E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T07-E	1	2.40E+02			2.40E+02	9.4E+00	1.5E+01	4.8E+01	10	325	3.25E+03	93%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T08-E	1	7.71E+01			7.71E+01	2.4E+01	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T09-E	1	5.49E+02			5.49E+02	3.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T01-F	1	7.29E+03			7.29E+03	7.4E-01	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T02-F	1	5.48E+03			5.48E+03	7.3E-01	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T03-F	1	4.71E+03			4.71E+03	9.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T04-F	1	3.69E+03			3.69E+03	1.8E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T05-F	1	1.64E+03			1.64E+03	1.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T06-F	1	8.32E+02			8.32E+02	1.2E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T07-F	1	2.23E+02			2.23E+02	1.2E+01	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T08-F	1	9.71E+01			9.71E+01	3.1E+01	1.5E+01	4.8E+01	10	325	3.49E+03	104%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-T09-F	1	5.67E+02			5.67E+02	1.1E+00	1.5E+01	4.8E+01					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-B01-D	1	7.50E+00	U1/2		7.50E+00	3.0E+02	1.5E+01	4.8E+01					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-B02-D	1	7.50E+00	U1/2		7.50E+00	9.4E+01	1.5E+01	4.8E+01					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-B03-D	1	7.50E+00	U1/2		7.50E+00	1.5E+01	1.5E+01	4.8E+01					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-B01-E	1	7.50E+00	U1/2		7.50E+00	3.0E+02	1.5E+01	4.8E+01					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-B02-E	1	7.50E+00	U1/2		7.50E+00	3.7E+01	1.5E+01	4.8E+01					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-B03-E	1	7.50E+00	U1/2		7.50E+00	3.9E+02	1.5E+01	4.8E+01					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-B01-F	1	7.50E+00	U1/2		7.50E+00	8.0E+01	1.5E+01	4.8E+01					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-B02-F	1	7.50E+00	U1/2		7.50E+00	4.7E+02	1.5E+01	4.8E+01					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1313-B03-F	1	7.50E+00	U1/2		7.50E+00	3.3E+01	1.5E+01	4.8E+01					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	EaFA-LRef-1313-T01-D	1	1.33E+04			1.33E+04	3.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T02-D	1	2.87E+03			2.87E+03	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T03-D	1	4.34E+02			4.34E+02	6.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T04-D	1	2.57E+02			2.57E+02	1.5E+00	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T05-D	1	5.09E+02			5.09E+02	4.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T06-D	1	1.20E+03			1.20E+03	6.6E-01	1.1E+00	3.5E+00	1000	100	2.27E+03	106%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T07-D	1	5.88E+03			5.88E+03	3.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T08-D	1	1.76E+04			1.76E+04	3.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T09-D	1	7.16E+04			7.16E+04	9.1E-02	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T01-E	1	1.22E+04			1.22E+04	3.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T02-E	1	2.73E+03			2.73E+03	8.1E-02	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T03-E	1	4.82E+02			4.82E+02	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T04-E	1	2.56E+02			2.56E+02	1.9E+00	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T05-E	1	5.46E+02			5.46E+02	6.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T06-E	1	1.07E+03			1.07E+03	5.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T07-E	1	5.87E+03			5.87E+03	5.9E-01	1.1E+00	3.5E+00	1000	100	6.76E+03	89%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T08-E	1	1.76E+04			1.76E+04	2.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T09-E	1	7.12E+04			7.12E+04	6.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T01-F	1	1.28E+04			1.28E+04	7.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T02-F	1	2.92E+03			2.92E+03	3.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T03-F	1	4.67E+02			4.67E+02	4.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T04-F	1	2.51E+02			2.51E+02	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T05-F	1	5.21E+02			5.21E+02	6.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T06-F	1	1.22E+03			1.22E+03	5.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T07-F	1	6.19E+03			6.19E+03	4.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T08-F	1	1.80E+04			1.80E+04	5.8E-01	1.1E+00	3.5E+00	1000	100	1.90E+04	98%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-T09-F	1	7.15E+04			7.15E+04	4.4E-01	1.1E+00	3.5E+00					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-B01-D	1	3.97E+01			3.97E+01	1.3E+01	1.1E+00	3.5E+00					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-B02-D	1	2.59E+02			2.59E+02	1.1E+01	1.1E+00	3.5E+00					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-B03-D	1	1.09E+03			1.09E+03	9.7E-01	1.1E+00	3.5E+00					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-B01-E	1	5.50E-01	U1/2		5.50E-01	3.3E+02	1.1E+00	3.5E+00					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-B02-E	1	2.57E+02			2.57E+02	6.1E+00	1.1E+00	3.5E+00					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-B03-E	1	1.43E+03			1.43E+03	6.2E-01	1.1E+00	3.5E+00					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-B01-F	1	2.00E+00	E		2.00E+00	3.8E+02	1.1E+00	3.5E+00					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-B02-F	1	2.63E+02			2.63E+02	3.3E+00	1.1E+00	3.5E+00					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1313-B03-F	1	1.66E+03			1.66E+03	5.0E-01	1.1E+00	3.5E+00					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	EaFA-LRef-1313-T01-D	1	1.01E+04			1.01E+04	1.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T02-D	1	6.59E+03			6.59E+03	5.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T03-D	1	6.07E+03			6.07E+03	2.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T04-D	1	6.03E+03			6.03E+03	7.7E-02	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T05-D	1	5.92E+03			5.92E+03	8.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T06-D	1	6.01E+03			6.01E+03	7.2E-01	2.5E+00	8.0E+00	1000	100	7.02E+03	101%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T07-D	1	6.24E+03			6.24E+03	5.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T08-D	1	4.38E+03			4.38E+03	2.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T09-D	1	3.72E+03			3.72E+03	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T01-E	1	1.01E+04			1.01E+04	6.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T02-E	1	6.58E+03			6.58E+03	5.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T03-E	1	6.40E+03			6.40E+03	9.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T04-E	1	6.12E+03			6.12E+03	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T05-E	1	6.09E+03			6.09E+03	5.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T06-E	1	5.99E+03			5.99E+03	2.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T07-E	1	6.23E+03			6.23E+03	1.1E+00	2.5E+00	8.0E+00	1000	100	7.29E+03	106%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T08-E	1	4.36E+03			4.36E+03	7.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T09-E	1	3.70E+03			3.70E+03	9.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T01-F	1	1.02E+04			1.02E+04	7.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T02-F	1	6.68E+03			6.68E+03	3.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T03-F	1	6.25E+03			6.25E+03	5.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T04-F	1	6.04E+03			6.04E+03	9.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T05-F	1	6.14E+03			6.14E+03	9.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T06-F	1	6.00E+03			6.00E+03	1.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T07-F	1	6.16E+03			6.16E+03	7.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T08-F	1	4.36E+03			4.36E+03	7.2E-01	2.5E+00	8.0E+00	1000	100	5.34E+03	98%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-T09-F	1	3.72E+03			3.72E+03	4.0E-01	2.5E+00	8.0E+00					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-B01-D	1	1.25E+00	U1/2		1.25E+00	2.3E+00	2.5E+00	8.0E+00					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-B02-D	1	1.25E+00	U1/2		1.25E+00	1.1E+00	2.5E+00	8.0E+00					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-B03-D	1	3.49E+03			3.49E+03	6.2E-01	2.5E+00	8.0E+00					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-B01-E	1	1.25E+00	U1/2		1.25E+00	1.4E+00	2.5E+00	8.0E+00					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-B02-E	1	1.25E+00	U1/2		1.25E+00	3.2E-01	2.5E+00	8.0E+00					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-B03-E	1	3.96E+03			3.96E+03	7.7E-01	2.5E+00	8.0E+00					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-B01-F	1	1.25E+00	U1/2		1.25E+00	1.1E+00	2.5E+00	8.0E+00					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-B02-F	1	1.25E+00	U1/2		1.25E+00	7.8E-01	2.5E+00	8.0E+00					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1313-B03-F	1	4.07E+03			4.07E+03	4.0E-01	2.5E+00	8.0E+00					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	EaFA-LRef-1313-T01-D	1	1.35E+03			1.35E+03	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T02-D	1	1.71E+03			1.71E+03	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T03-D	1	1.90E+03			1.90E+03	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T04-D	1	2.08E+03			2.08E+03	7.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T05-D	1	2.26E+03			2.26E+03	6.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T06-D	1	2.40E+03			2.40E+03	5.8E-01	1.0E+00	3.2E+00	1000	100	3.30E+03	90%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T07-D	1	2.97E+03			2.97E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T08-D	1	3.03E+03			3.03E+03	9.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T09-D	1	5.47E+03			5.47E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T01-E	1	1.30E+03			1.30E+03	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T02-E	1	1.72E+03			1.72E+03	9.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T03-E	1	1.95E+03			1.95E+03	9.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T04-E	1	2.10E+03			2.10E+03	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T05-E	1	2.33E+03			2.33E+03	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T06-E	1	2.44E+03			2.44E+03	1.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T07-E	1	2.97E+03			2.97E+03	1.3E+00	1.0E+00	3.2E+00	1000	100	3.85E+03	88%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T08-E	1	3.03E+03			3.03E+03	1.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T09-E	1	5.47E+03			5.47E+03	9.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T01-F	1	1.32E+03			1.32E+03	6.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T02-F	1	1.75E+03			1.75E+03	4.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T03-F	1	1.94E+03			1.94E+03	8.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T04-F	1	2.06E+03			2.06E+03	8.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T05-F	1	2.37E+03			2.37E+03	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T06-F	1	2.39E+03			2.39E+03	6.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T07-F	1	2.92E+03			2.92E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T08-F	1	3.06E+03			3.06E+03	1.6E-01	1.0E+00	3.2E+00	1000	100	4.03E+03	97%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-T09-F	1	5.49E+03			5.49E+03	9.1E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-B01-D	1	5.00E-01	U1/2		5.00E-01	5.5E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-B02-D	1	5.00E-01	U1/2		5.00E-01	3.9E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-B03-D	1	5.00E-01	U1/2		5.00E-01	9.0E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-B01-E	1	5.00E-01	U1/2		5.00E-01	7.1E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-B02-E	1	5.00E-01	U1/2		5.00E-01	2.2E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-B03-E	1	5.00E-01	U1/2		5.00E-01	2.2E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-B01-F	1	5.00E-01	U1/2		5.00E-01	2.4E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-B02-F	1	5.00E-01	U1/2		5.00E-01	6.7E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1313-B03-F	1	5.00E-01	U1/2		5.00E-01	2.6E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	EaFA-LRef-1313-T01-D	1	1.90E+05			1.90E+05	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T02-D	1	1.63E+05			1.63E+05	7.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T03-D	1	1.59E+05			1.59E+05	1.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T04-D	1	1.63E+05			1.63E+05	6.8E-02	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T05-D	1	1.62E+05			1.62E+05	6.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T06-D	1	1.65E+05			1.65E+05	6.1E-01	6.8E+00	2.2E+01	1000	100	1.66E+05	83%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T07-D	1	1.55E+05			1.55E+05	9.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T08-D	1	1.06E+05			1.06E+05	2.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T09-D	1	7.06E+04			7.06E+04	1.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T01-E	1	1.87E+05			1.87E+05	2.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T02-E	1	1.66E+05			1.66E+05	8.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T03-E	1	1.68E+05			1.68E+05	4.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T04-E	1	1.67E+05			1.67E+05	7.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T05-E	1	1.67E+05			1.67E+05	4.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T06-E	1	1.66E+05			1.66E+05	3.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T07-E	1	1.56E+05			1.56E+05	5.0E-01	6.8E+00	2.2E+01	1000	100	1.57E+05	93%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T08-E	1	1.07E+05			1.07E+05	5.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T09-E	1	7.15E+04			7.15E+04	6.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T01-F	1	1.96E+05			1.96E+05	5.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T02-F	1	1.68E+05			1.68E+05	2.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T03-F	1	1.67E+05			1.67E+05	7.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T04-F	1	1.68E+05			1.68E+05	5.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T05-F	1	1.72E+05			1.72E+05	5.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T06-F	1	1.66E+05			1.66E+05	8.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T07-F	1	1.57E+05			1.57E+05	9.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T08-F	1	1.08E+05			1.08E+05	6.3E-01	6.8E+00	2.2E+01	1000	100	1.09E+05	91%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-T09-F	1	7.20E+04			7.20E+04	4.0E-01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-B01-D	1	3.40E+00	U1/2		3.40E+00	8.5E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-B02-D	1	3.40E+00	U1/2		3.40E+00	8.4E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-B03-D	1	3.60E+01			3.60E+01	4.1E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-B01-E	1	3.40E+00	U1/2		3.40E+00	4.4E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-B02-E	1	3.40E+00	U1/2		3.40E+00	2.2E+02	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-B03-E	1	3.77E+01			3.77E+01	1.3E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-B01-F	1	3.40E+00	U1/2		3.40E+00	9.1E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-B02-F	1	3.40E+00	U1/2		3.40E+00	3.5E+02	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1313-B03-F	1	3.26E+01			3.26E+01	1.1E+01	6.8E+00	2.2E+01					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	EaFA-LRef-1313-T01-D	1	2.30E+00	U1/2		2.30E+00	9.8E+01	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T02-D	1	2.30E+00	U1/2		2.30E+00	3.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T03-D	1	2.30E+00	U1/2		2.30E+00	1.1E+02	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T04-D	1	2.30E+00	U1/2		2.30E+00	9.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T05-D	1	2.30E+00	U1/2		2.30E+00	3.1E+01	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T06-D	1	2.30E+00	U1/2		2.30E+00	7.5E+01	4.6E+00	1.5E+01	10	325	3.22E+03	99%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T07-D	1	2.30E+00	U1/2		2.30E+00	1.1E+03	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T08-D	1	4.03E+01			4.03E+01	1.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T09-D	1	7.28E+01			7.28E+01	9.3E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T01-E	1	2.30E+00	U1/2		2.30E+00	2.2E+02	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T02-E	1	2.30E+00	U1/2		2.30E+00	7.4E+02	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T03-E	1	2.30E+00	U1/2		2.30E+00	8.8E+01	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T04-E	1	2.30E+00	U1/2		2.30E+00	4.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T05-E	1	2.30E+00	U1/2		2.30E+00	1.0E+02	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T06-E	1	2.30E+00	U1/2		2.30E+00	7.9E+01	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T07-E	1	7.37E+00	E		7.37E+00	2.6E+02	4.6E+00	1.5E+01	10	325	3.21E+03	99%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T08-E	1	4.62E+01			4.62E+01	2.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T09-E	1	7.23E+01			7.23E+01	6.6E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T01-F	1	2.30E+00	U1/2		2.30E+00	3.5E+01	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T02-F	1	2.30E+00	U1/2		2.30E+00	1.6E+02	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T03-F	1	2.30E+00	U1/2		2.30E+00	3.4E+01	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T04-F	1	2.30E+00	U1/2		2.30E+00	3.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T05-F	1	2.30E+00	U1/2		2.30E+00	5.4E+01	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T06-F	1	2.30E+00	U1/2		2.30E+00	2.9E+02	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T07-F	1	1.27E+01	E		1.27E+01	1.2E+02	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T08-F	1	4.48E+01			4.48E+01	1.4E+01	4.6E+00	1.5E+01	10	325	3.14E+03	95%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-T09-F	1	6.86E+01			6.86E+01	2.6E+00	4.6E+00	1.5E+01					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-B01-D	1	2.30E+00	U1/2		2.30E+00	3.1E+01	4.6E+00	1.5E+01					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-B02-D	1	2.30E+00	U1/2		2.30E+00	1.2E+02	4.6E+00	1.5E+01					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-B03-D	1	2.30E+00	U1/2		2.30E+00	3.1E+01	4.6E+00	1.5E+01					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-B01-E	1	2.30E+00	U1/2		2.30E+00	3.3E+01	4.6E+00	1.5E+01					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-B02-E	1	2.30E+00	U1/2		2.30E+00	1.9E+01	4.6E+00	1.5E+01					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-B03-E	1	2.30E+00	U1/2		2.30E+00	5.4E+01	4.6E+00	1.5E+01					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-B01-F	1	2.30E+00	U1/2		2.30E+00	2.9E+01	4.6E+00	1.5E+01					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-B02-F	1	2.30E+00	U1/2		2.30E+00	7.5E+01	4.6E+00	1.5E+01					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1313-B03-F	1	2.30E+00	U1/2		2.30E+00	3.6E+01	4.6E+00	1.5E+01					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	EaFA-LRef-1313-T01-D	1	1.00E+00	U1/2		1.00E+00	4.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T02-D	1	1.00E+00	U1/2		1.00E+00	3.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T03-D	1	1.00E+00	U1/2		1.00E+00	3.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T04-D	1	1.00E+00	U1/2		1.00E+00	1.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T05-D	1	1.00E+00	U1/2		1.00E+00	3.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T06-D	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00	10	325	3.10E+03	95%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T07-D	1	1.00E+00	U1/2		1.00E+00	2.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T08-D	1	3.50E+00	E		3.50E+00	3.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T09-D	1	1.41E+03			1.41E+03	6.8E-02	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T01-E	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T02-E	1	1.00E+00	U1/2		1.00E+00	2.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T03-E	1	1.00E+00	U1/2		1.00E+00	6.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T04-E	1	1.00E+00	U1/2		1.00E+00	8.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T05-E	1	1.00E+00	U1/2		1.00E+00	3.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T06-E	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T07-E	1	1.00E+00	U1/2		1.00E+00	3.6E+01	2.0E+00	6.4E+00	10	325	3.10E+03	95%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T08-E	1	3.61E+00	E		3.61E+00	1.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T09-E	1	1.48E+03			1.48E+03	2.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T01-F	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T02-F	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T03-F	1	1.00E+00	U1/2		1.00E+00	1.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T04-F	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T05-F	1	1.00E+00	U1/2		1.00E+00	1.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T06-F	1	1.00E+00	U1/2		1.00E+00	1.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T07-F	1	1.00E+00	U1/2		1.00E+00	6.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T08-F	1	3.22E+00	E		3.22E+00	9.4E+00	2.0E+00	6.4E+00	10	325	3.00E+03	92%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-T09-F	1	1.46E+03			1.46E+03	3.3E-01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-B01-D	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-B02-D	1	1.00E+00	U1/2		1.00E+00	8.3E+00	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-B03-D	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-B01-E	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-B02-E	1	1.00E+00	U1/2		1.00E+00	6.6E+03	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-B03-E	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-B01-F	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-B02-F	1	1.00E+00	U1/2		1.00E+00	4.1E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1313-B03-F	1	1.00E+00	U1/2		1.00E+00	5.8E+01	2.0E+00	6.4E+00					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	EaFA-LRef-1313-T01-D	1	4.79E+03			4.79E+03	1.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T02-D	1	2.32E+03			2.32E+03	8.4E-01	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T03-D	1	1.50E+03			1.50E+03	2.1E-01	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T04-D	1	6.39E+02			6.39E+02	5.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T05-D	1	1.90E+02			1.90E+02	6.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T06-D	1	1.38E+02			1.38E+02	1.0E+00	1.5E+00	4.8E+00	10	325	3.13E+03	92%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T07-D	1	7.50E+01			7.50E+01	2.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T08-D	1	8.19E+01			8.19E+01	6.4E-01	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T09-D	1	6.45E+03			6.45E+03	1.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T01-E	1	4.57E+03			4.57E+03	2.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T02-E	1	2.26E+03			2.26E+03	6.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T03-E	1	1.59E+03			1.59E+03	6.0E-01	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T04-E	1	6.75E+02			6.75E+02	1.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T05-E	1	2.04E+02			2.04E+02	2.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T06-E	1	1.45E+02			1.45E+02	4.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T07-E	1	7.98E+01			7.98E+01	1.5E+00	1.5E+00	4.8E+00	10	325	3.18E+03	95%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T08-E	1	8.47E+01			8.47E+01	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T09-E	1	6.44E+03			6.44E+03	7.0E-01	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T01-F	1	4.84E+03			4.84E+03	3.4E-01	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T02-F	1	2.30E+03			2.30E+03	8.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T03-F	1	1.58E+03			1.58E+03	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T04-F	1	6.65E+02			6.65E+02	1.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T05-F	1	2.12E+02			2.12E+02	1.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T06-F	1	1.39E+02			1.39E+02	3.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T07-F	1	7.81E+01			7.81E+01	5.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T08-F	1	7.94E+01			7.94E+01	1.1E+00	1.5E+00	4.8E+00	10	325	3.07E+03	92%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-T09-F	1	6.46E+03			6.46E+03	6.9E-02	1.5E+00	4.8E+00					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-B01-D	1	1.80E+00	E		1.80E+00	1.2E+02	1.5E+00	4.8E+00					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-B02-D	1	7.50E-01	U1/2		7.50E-01	1.7E+02	1.5E+00	4.8E+00					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-B03-D	1	4.95E+00			4.95E+00	4.9E+01	1.5E+00	4.8E+00					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-B01-E	1	7.50E-01	U1/2		7.50E-01	9.7E+01	1.5E+00	4.8E+00					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-B02-E	1	7.50E-01	U1/2		7.50E-01	1.6E+02	1.5E+00	4.8E+00					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-B03-E	1	1.81E+00	E		1.81E+00	6.0E+01	1.5E+00	4.8E+00					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-B01-F	1	7.50E-01	U1/2		7.50E-01	2.1E+02	1.5E+00	4.8E+00					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-B02-F	1	2.97E+00	E		2.97E+00	5.9E+01	1.5E+00	4.8E+00					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1313-B03-F	1	7.50E-01	U1/2		7.50E-01	7.8E+01	1.5E+00	4.8E+00					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	EaFA-LRef-1313-T01-D	1	9.59E+01			9.59E+01	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T02-D	1	3.25E+00			2.25E+00	2.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:30 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T03-D	1	5.00E-01	U1/2		5.00E-01	3.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:32 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T04-D	1	5.00E-01	U1/2		5.00E-01	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:33 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T05-D	1	5.00E-01	U1/2		5.00E-01	6.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:35 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T06-D	1	2.58E+00	E		2.58E+00	2.7E+01	1.0E+00	3.2E+00	10	325	3.37E+03	104%	VU ICP-OES	5/6/10 9:36 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T07-D	1	1.04E+03			1.04E+03	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:38 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T08-D	1	1.15E+03			1.15E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:40 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T09-D	1	1.61E+03			1.61E+03	9.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:41 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T01-E	1	1.12E+02			1.12E+02	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:51 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T02-E	1	9.24E+00			9.24E+00	1.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:53 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T03-E	1	1.57E+01			1.57E+01	3.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:55 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T04-E	1	3.26E+00			3.26E+00	2.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:56 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T05-E	1	1.64E+01			1.64E+01	3.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:58 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T06-E	1	1.31E+01			1.31E+01	8.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:00 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T07-E	1	1.01E+03			1.01E+03	1.2E+00	1.0E+00	3.2E+00	10	325	4.83E+03	118%	VU ICP-OES	5/6/10 10:01 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T08-E	1	1.15E+03			1.15E+03	6.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:03 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T09-E	1	1.62E+03			1.62E+03	3.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:05 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T01-F	1	1.07E+02			1.07E+02	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:14 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T02-F	1	1.72E+01			1.72E+01	3.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:16 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T03-F	1	5.00E-01	U1/2		5.00E-01	5.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:18 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T04-F	1	2.23E+00	E		2.23E+00	5.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:19 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T05-F	1	8.30E+00			8.30E+00	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:21 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T06-F	1	1.62E+01			1.62E+01	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T07-F	1	1.03E+03			1.03E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 10:24 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T08-F	1	1.21E+03			1.21E+03	2.5E-01	1.0E+00	3.2E+00	10	325	3.98E+03	85%	VU ICP-OES	5/6/10 10:26 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-T09-F	1	1.64E+03			1.64E+03	2.3E-01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 10:28 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-B01-D	1	5.00E-01	U1/2		5.00E-01	9.7E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-B02-D	1	5.00E-01	U1/2		5.00E-01	8.9E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:25 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-B03-D	1	5.00E-01	U1/2		5.00E-01	2.7E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:27 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-B01-E	1	5.00E-01	U1/2		5.00E-01	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:46 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-B02-E	1	5.00E-01	U1/2		5.00E-01	8.0E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:48 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-B03-E	1	5.00E-01	U1/2		5.00E-01	5.9E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 9:50 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-B01-F	1	5.00E-01	U1/2		5.00E-01	8.8E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 10:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-B02-F	1	5.00E-01	U1/2		5.00E-01	1.8E+00	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 10:11 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1313-B03-F	1	5.00E-01	U1/2		5.00E-01	1.5E+01	1.0E+00	3.2E+00					VU ICP-OES	5/6/10 10:13 AM	EPA Interlab LRef D-F 1313-1316 EaFA

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	SWA-L01-1313-T01-A	1	8.64E+04			8.64E+04	2.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T02-A	1	3.50E+04			3.50E+04	3.4E-01	1.0E+00	3.2E+00	1000	100	3.62E+04	116%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T03-A	1	6.61E+02			6.61E+02	3.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T04-A	1	5.05E+01			5.05E+01	5.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T05-A	1	5.00E-01	U1/2		5.00E-01	6.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T06-A	1	5.00E-01	U1/2		5.00E-01	1.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T07-A	1	5.00E-01	U1/2		5.00E-01	2.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T08-A	1	2.30E+05			2.30E+05	9.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T09-A	1	5.85E+05			5.85E+05	2.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T01-B	1	8.17E+04			8.17E+04	8.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T02-B	1	3.61E+04			3.61E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T03-B	1	7.86E+02			7.86E+02	9.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T04-B	1	1.76E+01			1.76E+01	1.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T05-B	1	8.72E+00			8.72E+00	9.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T06-B	1	5.00E-01	U1/2		5.00E-01	2.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T07-B	1	5.00E-01	U1/2		5.00E-01	2.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T08-B	1	2.38E+05			2.38E+05	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T09-B	1	5.66E+05			5.66E+05	3.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T01-C	1	7.95E+04			7.95E+04	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T02-C	1	3.65E+04			3.65E+04	5.3E-01	1.0E+00	3.2E+00	1000	100	3.76E+04	110%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T03-C	1	5.08E+02			5.08E+02	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T04-C	1	4.40E+01			4.40E+01	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T05-C	1	5.00E-01	U1/2		5.00E-01	2.5E+01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T06-C	1	5.00E-01	U1/2		5.00E-01	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T07-C	1	5.00E-01	U1/2		5.00E-01	6.5E+00	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T08-C	1	2.24E+05			2.24E+05	2.2E-01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-T09-C	1	5.85E+05			5.85E+05	2.8E+00	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	3.6E+00	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	2.0E+00	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	SWA-L01-1313-T01-A	1	5.69E+03			5.69E+03	3.8E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T02-A	1	3.12E+03			3.12E+03	5.5E-01	7.5E+00	2.4E+01	10	100	4.28E+03	116%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T03-A	1	1.20E+03			1.20E+03	1.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T04-A	1	1.20E+03			1.20E+03	1.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T05-A	1	1.28E+03			1.28E+03	4.6E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T06-A	1	1.37E+03			1.37E+03	1.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T07-A	1	1.35E+03			1.35E+03	2.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T08-A	1	6.89E+02			6.89E+02	7.6E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T09-A	1	2.11E+02			2.11E+02	8.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T01-B	1	6.11E+03			6.11E+03	5.3E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T02-B	1	3.84E+03			3.84E+03	1.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T03-B	1	1.29E+03			1.29E+03	6.4E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T04-B	1	1.26E+03			1.26E+03	1.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T05-B	1	1.21E+03			1.21E+03	6.9E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T06-B	1	1.44E+03			1.44E+03	2.6E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T07-B	1	1.29E+03			1.29E+03	3.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T08-B	1	7.85E+02			7.85E+02	5.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T09-B	1	2.38E+02			2.38E+02	4.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T01-C	1	6.16E+03			6.16E+03	1.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T02-C	1	2.35E+03			2.35E+03	8.3E-01	7.5E+00	2.4E+01	10	100	3.38E+03	103%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T03-C	1	1.22E+03			1.22E+03	3.4E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T04-C	1	1.18E+03			1.18E+03	1.4E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T05-C	1	9.85E+02			9.85E+02	5.6E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T06-C	1	1.13E+03			1.13E+03	7.9E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T07-C	1	1.14E+03			1.14E+03	9.9E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T08-C	1	6.43E+02			6.43E+02	8.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-T09-C	1	2.28E+02			2.28E+02	1.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-B01-A	1	8.64E+00	E		8.64E+00	3.5E+01	7.5E+00	2.4E+01					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-B02-A	1	8.75E+00	E		8.75E+00	2.8E+01	7.5E+00	2.4E+01					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1313-B03-A	1	1.25E+01	E		1.25E+01	2.0E+01	7.5E+00	2.4E+01					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	SWA-L01-1313-T01-A	1	1.64E+04			1.64E+04	3.2E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T02-A	1	5.06E+03			5.06E+03	3.7E-01	1.1E+01	3.5E+01	10	100	5.92E+03	85%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T03-A	1	1.53E+02			1.53E+02	9.6E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T04-A	1	4.78E+02			4.78E+02	4.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T05-A	1	3.06E+02			3.06E+02	2.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T06-A	1	2.03E+02			2.03E+02	6.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T07-A	1	1.97E+02			1.97E+02	7.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T08-A	1	2.72E+03			2.72E+03	8.1E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T09-A	1	5.75E+03			5.75E+03	3.0E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T01-B	1	1.62E+04			1.62E+04	8.1E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T02-B	1	5.50E+03			5.50E+03	1.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T03-B	1	1.85E+02			1.85E+02	2.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T04-B	1	4.04E+02			4.04E+02	5.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T05-B	1	3.89E+02			3.89E+02	4.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T06-B	1	2.02E+02			2.02E+02	5.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T07-B	1	1.97E+02			1.97E+02	4.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T08-B	1	2.47E+03			2.47E+03	4.0E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T09-B	1	6.32E+03			6.32E+03	8.2E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T01-C	1	1.58E+04			1.58E+04	1.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T02-C	1	5.36E+03			5.36E+03	5.7E-02	1.1E+01	3.5E+01	10	100	6.32E+03	96%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T03-C	1	1.82E+02			1.82E+02	4.5E-02	1.1E+01	3.5E+01				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T04-C	1	3.73E+02			3.73E+02	2.5E+00	1.1E+01	3.5E+01					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T05-C	1	1.91E+02			1.91E+02	5.4E+00	1.1E+01	3.5E+01					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T06-C	1	2.17E+02			2.17E+02	2.7E+00	1.1E+01	3.5E+01					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T07-C	1	1.92E+02			1.92E+02	8.5E+00	1.1E+01	3.5E+01					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T08-C	1	2.52E+03			2.52E+03	5.8E-01	1.1E+01	3.5E+01					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-T09-C	1	6.55E+03			6.55E+03	3.3E+00	1.1E+01	3.5E+01					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-B01-A	1	5.50E+00	U1/2		5.50E+00	5.6E+01	1.1E+01	3.5E+01					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-B02-A	1	5.50E+00	U1/2		5.50E+00	4.5E+01	1.1E+01	3.5E+01					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1313-B03-A	1	5.50E+00	U1/2		5.50E+00	5.0E+01	1.1E+01	3.5E+01					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	SWA-L01-1313-T01-A	1	1.18E+03			1.18E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T02-A	1	7.82E+02			7.82E+02	4.5E-01	1.0E+00	3.2E+00	1000	100	1.71E+03	93%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T03-A	1	1.04E+03			1.04E+03	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T04-A	1	1.89E+03			1.89E+03	9.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T05-A	1	2.73E+03			2.73E+03	1.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T06-A	1	3.63E+03			3.63E+03	3.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T07-A	1	5.83E+03			5.83E+03	5.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T08-A	1	5.76E+03			5.76E+03	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T09-A	1	5.79E+03			5.79E+03	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T01-B	1	1.26E+03			1.26E+03	6.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T02-B	1	9.37E+02			9.37E+02	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T03-B	1	1.03E+03			1.03E+03	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T04-B	1	1.48E+03			1.48E+03	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T05-B	1	1.96E+03			1.96E+03	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T06-B	1	2.91E+03			2.91E+03	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T07-B	1	5.88E+03			5.88E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T08-B	1	5.67E+03			5.67E+03	3.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T09-B	1	5.79E+03			5.79E+03	4.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T01-C	1	1.20E+03			1.20E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T02-C	1	9.96E+02			9.96E+02	3.4E-01	1.0E+00	3.2E+00	1000	100	1.95E+03	95%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T03-C	1	1.07E+03			1.07E+03	4.5E-02	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T04-C	1	1.55E+03			1.55E+03	3.3E-01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T05-C	1	2.18E+03			2.18E+03	6.2E-01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T06-C	1	2.28E+03			2.28E+03	6.2E-01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T07-C	1	4.24E+03			4.24E+03	2.3E-01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T08-C	1	5.86E+03			5.86E+03	1.6E-01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-T09-C	1	5.74E+03			5.74E+03	2.9E+00	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-B01-A	1	1.19E+01			1.19E+01	1.9E+00	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-B02-A	1	9.85E+00			9.85E+00	2.4E+00	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1313-B03-A	1	1.15E+01			1.15E+01	3.1E+00	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	SWA-L01-1313-T01-A	1	2.09E+02			2.09E+02	2.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T02-A	1	1.63E+02			1.63E+02	3.2E-01	1.0E+00	3.2E+00	10	100	1.03E+03	87%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T03-A	1	1.11E+03			1.11E+03	8.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T04-A	1	1.12E+03			1.12E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T05-A	1	1.08E+03			1.08E+03	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T06-A	1	1.01E+03			1.01E+03	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T07-A	1	1.50E+03			1.50E+03	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T08-A	1	5.72E+02			5.72E+02	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T09-A	1	6.52E+02			6.52E+02	1.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T01-B	1	3.13E+02			3.13E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T02-B	1	1.71E+02			1.71E+02	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T03-B	1	1.06E+03			1.06E+03	3.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T04-B	1	1.17E+03			1.17E+03	6.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T05-B	1	9.51E+02			9.51E+02	4.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T06-B	1	9.93E+02			9.93E+02	9.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T07-B	1	1.39E+03			1.39E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T08-B	1	5.54E+02			5.54E+02	1.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T09-B	1	6.32E+02			6.32E+02	1.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T01-C	1	2.59E+02			2.59E+02	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T02-C	1	1.54E+02			1.54E+02	2.6E-01	1.0E+00	3.2E+00	10	100	1.03E+03	88%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T03-C	1	9.70E+02			9.70E+02	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T04-C	1	1.05E+03			1.05E+03	9.0E-01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T05-C	1	8.57E+02			8.57E+02	5.3E-01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T06-C	1	9.19E+02			9.19E+02	1.7E-01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T07-C	1	1.13E+03			1.13E+03	8.7E-01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T08-C	1	5.93E+02			5.93E+02	2.6E-01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-T09-C	1	6.87E+02			6.87E+02	3.4E+00	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-B01-A	1	1.52E+00	E		1.52E+00	3.4E+00	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-B02-A	1	1.46E+00	E		1.46E+00	2.1E+00	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1313-B03-A	1	1.72E+00	E		1.72E+00	2.0E+00	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	SWA-L01-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	3.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	7.5E+02	1.9E+00	6.0E+00	10	100	1.07E+03	107%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	1.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	3.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	1.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	8.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T07-A	1	9.50E-01	U1/2		9.50E-01	5.9E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T08-A	1	2.79E+01			2.79E+01	5.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T09-A	1	1.11E+02			1.11E+02	1.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	3.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	5.9E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	6.7E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	3.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	2.6E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	2.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T07-B	1	9.50E-01	U1/2		9.50E-01	4.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T08-B	1	3.21E+01			3.21E+01	2.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T09-B	1	1.11E+02			1.11E+02	1.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	4.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	4.8E+02	1.9E+00	6.0E+00	10	100	1.07E+03	107%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	3.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	8.8E+01	1.9E+00	6.0E+00					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	1.8E+03	1.9E+00	6.0E+00					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T07-C	1	9.50E-01	U1/2		9.50E-01	2.1E+02	1.9E+00	6.0E+00					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T08-C	1	3.00E+01			3.00E+01	3.1E+00	1.9E+00	6.0E+00					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-T09-C	1	1.18E+02			1.18E+02	5.7E+00	1.9E+00	6.0E+00					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	2.0E+01	1.9E+00	6.0E+00					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	8.0E+02	1.9E+00	6.0E+00					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	4.1E+01	1.9E+00	6.0E+00					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	SWA-L01-1313-T01-A	1	1.10E+00	U1/2		1.10E+00	2.9E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T02-A	1	1.10E+00	U1/2		1.10E+00	2.3E+02	2.2E+00	7.0E+00	10	100	1.02E+03	102%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	9.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T04-A	1	1.10E+00	U1/2		1.10E+00	5.3E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T05-A	1	1.10E+00	U1/2		1.10E+00	1.5E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T06-A	1	1.10E+00	U1/2		1.10E+00	7.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T07-A	1	3.30E+00	E		3.30E+00	1.6E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T08-A	1	1.69E+01			1.69E+01	1.4E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T09-A	1	2.87E+01			2.87E+01	1.1E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T01-B	1	1.10E+00	U1/2		1.10E+00	8.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T02-B	1	1.10E+00	U1/2		1.10E+00	1.3E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	1.3E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T04-B	1	1.10E+00	U1/2		1.10E+00	3.7E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T05-B	1	1.10E+00	U1/2		1.10E+00	3.5E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T06-B	1	1.10E+00	U1/2		1.10E+00	7.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T07-B	1	3.75E+00	E		3.75E+00	9.5E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T08-B	1	1.63E+01			1.63E+01	1.7E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T09-B	1	2.85E+01			2.85E+01	1.2E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T01-C	1	1.10E+00	U1/2		1.10E+00	4.7E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T02-C	1	1.10E+00	U1/2		1.10E+00	2.4E+02	2.2E+00	7.0E+00	10	100	1.03E+03	102%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	6.7E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T04-C	1	1.10E+00	U1/2		1.10E+00	1.1E+02	2.2E+00	7.0E+00					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T05-C	1	1.10E+00	U1/2		1.10E+00	5.3E+01	2.2E+00	7.0E+00					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T06-C	1	1.10E+00	U1/2		1.10E+00	9.7E+02	2.2E+00	7.0E+00					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T07-C	1	1.10E+00	U1/2		1.10E+00	7.8E+00	2.2E+00	7.0E+00					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T08-C	1	1.69E+01			1.69E+01	1.9E-01	2.2E+00	7.0E+00					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-T09-C	1	2.94E+01			2.94E+01	9.1E+00	2.2E+00	7.0E+00					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	5.8E+01	2.2E+00	7.0E+00					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	6.1E+01	2.2E+00	7.0E+00					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1313-B03-A	1	1.10E+00	U1/2		1.10E+00	2.2E+02	2.2E+00	7.0E+00					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	SWA-L01-1313-T01-A	1	4.34E+03			4.34E+03	2.9E+00	2.6E+00	8.3E+00				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T02-A	1	1.38E+04			1.38E+04	2.0E-01	2.6E+00	8.3E+00	1000	100	1.47E+04	91%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T03-A	1	2.04E+06			2.04E+06	4.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T04-A	1	5.80E+06			5.80E+06	7.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T05-A	1	6.78E+06			6.78E+06	4.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T06-A	1	7.07E+06			7.07E+06	1.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T07-A	1	8.52E+06			8.52E+06	2.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T08-A	1	3.48E+06			3.48E+06	7.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T09-A	1	2.74E+06			2.74E+06	6.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T01-B	1	5.14E+03			5.14E+03	1.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T02-B	1	1.42E+04			1.42E+04	1.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T03-B	1	1.93E+06			1.93E+06	2.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T04-B	1	4.58E+06			4.58E+06	6.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T05-B	1	5.60E+06			5.60E+06	5.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T06-B	1	6.67E+06			6.67E+06	8.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T07-B	1	8.11E+06			8.11E+06	4.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T08-B	1	3.33E+06			3.33E+06	4.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T09-B	1	2.63E+06			2.63E+06	2.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T01-C	1	4.98E+03			4.98E+03	9.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T02-C	1	1.39E+04			1.39E+04	4.6E-01	2.6E+00	8.3E+00	1000	100	1.48E+04	90%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T03-C	1	2.02E+06			2.02E+06	5.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T04-C	1	4.54E+06			4.54E+06	5.0E-01	2.6E+00	8.3E+00					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T05-C	1	5.90E+06			5.90E+06	7.9E-01	2.6E+00	8.3E+00					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T06-C	1	5.85E+06			5.85E+06	7.2E-01	2.6E+00	8.3E+00					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T07-C	1	7.58E+06			7.58E+06	3.4E-01	2.6E+00	8.3E+00					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T08-C	1	3.32E+06			3.32E+06	4.7E-01	2.6E+00	8.3E+00					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-T09-C	1	2.58E+06			2.58E+06	2.8E+00	2.6E+00	8.3E+00					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-B01-A	1	1.30E+00	U1/2		1.30E+00	2.4E+01	2.6E+00	8.3E+00					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-B02-A	1	1.30E+00	U1/2		1.30E+00	5.7E+02	2.6E+00	8.3E+00					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1313-B03-A	1	3.61E+01			3.61E+01	2.7E+01	2.6E+00	8.3E+00					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	SWA-L01-1313-T01-A	1	1.75E+03			1.75E+03	3.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T02-A	1	1.17E+03			1.17E+03	3.7E-01	1.2E+00	3.8E+00	10	100	2.07E+03	90%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T03-A	1	1.03E+01			1.03E+01	5.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T04-A	1	9.05E+00			9.05E+00	1.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T05-A	1	1.18E+01			1.18E+01	3.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T06-A	1	1.71E+01			1.71E+01	5.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T07-A	1	6.40E+00			6.40E+00	2.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T08-A	1	3.65E+03			3.65E+03	8.0E-02	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T09-A	1	1.44E+04			1.44E+04	3.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T01-B	1	1.79E+03			1.79E+03	2.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T02-B	1	1.11E+03			1.11E+03	7.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T03-B	1	8.13E+00			8.13E+00	7.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T04-B	1	4.30E+00			4.30E+00	2.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T05-B	1	6.39E+00			6.39E+00	1.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T06-B	1	1.11E+01			1.11E+01	8.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T07-B	1	5.03E+00			5.03E+00	3.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T08-B	1	3.85E+03			3.85E+03	3.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T09-B	1	1.45E+04			1.45E+04	3.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T01-C	1	1.18E+03			1.18E+03	1.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T02-C	1	1.38E+03			1.38E+03	2.1E-01	1.2E+00	3.8E+00	10	100	2.29E+03	92%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T03-C	1	9.19E+00			9.19E+00	2.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T04-C	1	3.85E+00			3.85E+00	1.1E+01	1.2E+00	3.8E+00					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T05-C	1	1.06E+01			1.06E+01	1.6E+01	1.2E+00	3.8E+00					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T06-C	1	1.18E+01			1.18E+01	6.4E+00	1.2E+00	3.8E+00					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T07-C	1	3.60E+00	E		3.60E+00	3.1E+01	1.2E+00	3.8E+00					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T08-C	1	3.45E+03			3.45E+03	1.7E-01	1.2E+00	3.8E+00					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-T09-C	1	1.40E+04			1.40E+04	2.8E+00	1.2E+00	3.8E+00					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	6.1E+01	1.2E+00	3.8E+00					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	5.4E+01	1.2E+00	3.8E+00					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1313-B03-A	1	1.28E+00	E		1.28E+00	8.0E+00	1.2E+00	3.8E+00					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	SWA-L01-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	2.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	3.2E+01	1.8E+00	5.7E+00	10	100	9.81E+02	98%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T03-A	1	2.38E+00	E		2.38E+00	4.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T04-A	1	4.73E+00	E		4.73E+00	3.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T05-A	1	1.31E+01			1.31E+01	3.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T06-A	1	3.74E+01			3.74E+01	9.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T07-A	1	1.53E+02			1.53E+02	2.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T08-A	1	1.52E+02			1.52E+02	1.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T09-A	1	1.81E+02			1.81E+02	1.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	1.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	3.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T03-B	1	1.86E+00	E		1.86E+00	2.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T04-B	1	3.75E+00	E		3.75E+00	3.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T05-B	1	5.43E+00	E		5.43E+00	1.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T06-B	1	1.37E+01			1.37E+01	1.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T07-B	1	1.61E+02			1.61E+02	6.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T08-B	1	1.48E+02			1.48E+02	5.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T09-B	1	1.78E+02			1.78E+02	3.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	8.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	2.2E+03	1.8E+00	5.7E+00	10	100	9.88E+02	99%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T03-C	1	1.94E+00	E		1.94E+00	7.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T04-C	1	3.04E+00	E		3.04E+00	1.7E+01	1.8E+00	5.7E+00					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T05-C	1	9.43E+00			9.43E+00	3.3E+00	1.8E+00	5.7E+00					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T06-C	1	1.09E+01			1.09E+01	4.9E+00	1.8E+00	5.7E+00					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T07-C	1	1.09E+02			1.09E+02	2.7E+00	1.8E+00	5.7E+00					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T08-C	1	1.51E+02			1.51E+02	3.9E-01	1.8E+00	5.7E+00					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-T09-C	1	1.85E+02			1.85E+02	3.6E+00	1.8E+00	5.7E+00					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	2.1E+02	1.8E+00	5.7E+00					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	3.7E+02	1.8E+00	5.7E+00					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	4.9E+02	1.8E+00	5.7E+00					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	SWA-L01-1313-T01-A	1	4.07E+00	E		4.07E+00	5.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T02-A	1	1.85E+00	U1/2		1.85E+00	1.5E+02	3.7E+00	1.2E+01	10	100	9.90E+02	99%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T03-A	1	5.88E+00	E		5.88E+00	3.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T04-A	1	1.04E+01	E		1.04E+01	9.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T05-A	1	1.04E+01	E		1.04E+01	1.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T06-A	1	1.35E+01			1.35E+01	2.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T07-A	1	1.65E+01			1.65E+01	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T08-A	1	3.05E+01			3.05E+01	9.3E-01	3.7E+00	1.2E+01				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T09-A	1	9.26E+02			9.26E+02	4.6E-01	3.7E+00	1.2E+01				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T01-B	1	4.74E+00	E		4.74E+00	6.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T02-B	1	1.85E+00	U1/2		1.85E+00	9.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T03-B	1	5.58E+00	E		5.58E+00	4.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T04-B	1	9.12E+00	E		9.12E+00	1.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T05-B	1	8.96E+00	E		8.96E+00	3.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T06-B	1	1.14E+01	E		1.14E+01	5.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T07-B	1	1.53E+01			1.53E+01	1.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T08-B	1	3.33E+01			3.33E+01	1.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T09-B	1	9.43E+02			9.43E+02	1.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T01-C	1	4.37E+00	E		4.37E+00	1.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T02-C	1	1.85E+00	U1/2		1.85E+00	1.4E+02	3.7E+00	1.2E+01	10	100	9.98E+02	100%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T03-C	1	5.33E+00	E		5.33E+00	6.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T04-C	1	7.62E+00	E		7.62E+00	1.9E+01	3.7E+00	1.2E+01					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T05-C	1	1.26E+01			1.26E+01	1.2E+01	3.7E+00	1.2E+01					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T06-C	1	9.03E+00	E		9.03E+00	4.3E+01	3.7E+00	1.2E+01					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T07-C	1	1.27E+01			1.27E+01	2.4E+01	3.7E+00	1.2E+01					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T08-C	1	3.30E+01			3.30E+01	1.3E+00	3.7E+00	1.2E+01					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-T09-C	1	9.39E+02			9.39E+02	2.9E+00	3.7E+00	1.2E+01					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	7.2E+01	3.7E+00	1.2E+01					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	2.8E+02	3.7E+00	1.2E+01					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1313-B03-A	1	1.85E+00	U1/2		1.85E+00	3.0E+02	3.7E+00	1.2E+01					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	SWA-L01-1313-T01-A	1	1.40E+02			1.40E+02	6.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T02-A	1	1.00E+02			1.00E+02	6.1E-01	2.0E+00	6.4E+00	1000	100	1.16E+03	106%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T03-A	1	2.69E+01			2.69E+01	1.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T04-A	1	3.93E+01			3.93E+01	1.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T05-A	1	1.97E+01			1.97E+01	1.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T06-A	1	2.91E+01			2.91E+01	1.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T07-A	1	2.76E+04			2.76E+04	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T08-A	1	9.94E+04			9.94E+04	7.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T09-A	1	1.32E+05			1.32E+05	4.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T01-B	1	1.49E+02			1.49E+02	1.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T02-B	1	1.01E+02			1.01E+02	5.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T03-B	1	1.89E+01			1.89E+01	2.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T04-B	1	1.61E+01			1.61E+01	6.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T05-B	1	2.34E+01			2.34E+01	5.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T06-B	1	1.42E+01			1.42E+01	4.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T07-B	1	3.26E+04			3.26E+04	9.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T08-B	1	9.93E+04			9.93E+04	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T09-B	1	1.29E+05			1.29E+05	4.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T01-C	1	9.73E+01			9.73E+01	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T02-C	1	9.97E+01			9.97E+01	3.3E-01	2.0E+00	6.4E+00	1000	100	1.16E+03	106%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T03-C	1	1.67E+01			1.67E+01	6.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T04-C	1	1.77E+01			1.77E+01	1.4E+00	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T05-C	1	1.55E+01			1.55E+01	3.7E+00	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T06-C	1	4.96E+01			4.96E+01	2.5E+00	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T07-C	1	8.57E+03			8.57E+03	6.5E-01	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T08-C	1	1.01E+05			1.01E+05	3.7E-01	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-T09-C	1	1.31E+05			1.31E+05	2.8E+00	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	2.5E+02	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	2.2E+00	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1313-B03-A	1	3.40E+00	E		3.40E+00	5.5E+00	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	SWA-L01-1313-T01-A	1	8.88E+01			8.88E+01	5.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T02-A	1	1.67E+01	E		1.67E+01	1.1E+01	6.8E+00	2.2E+01	10	100	9.74E+02	96%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T03-A	1	3.40E+00	U1/2		3.40E+00	2.8E+02	6.8E+00	2.2E+01				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T04-A	1	3.40E+00	U1/2		3.40E+00	4.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T05-A	1	3.40E+00	U1/2		3.40E+00	1.6E+02	6.8E+00	2.2E+01				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T06-A	1	3.40E+00	U1/2		3.40E+00	5.7E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T07-A	1	3.40E+00	U1/2		3.40E+00	4.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T08-A	1	1.46E+02			1.46E+02	6.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T09-A	1	2.22E+03			2.22E+03	5.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T01-B	1	1.40E+02			1.40E+02	3.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T02-B	1	1.96E+01	E		1.96E+01	5.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T03-B	1	3.40E+00	U1/2		3.40E+00	1.5E+02	6.8E+00	2.2E+01				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T04-B	1	3.40E+00	U1/2		3.40E+00	1.4E+02	6.8E+00	2.2E+01				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T05-B	1	3.40E+00	U1/2		3.40E+00	8.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T06-B	1	3.40E+00	U1/2		3.40E+00	1.1E+02	6.8E+00	2.2E+01				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T07-B	1	6.82E+00	E		6.82E+00	4.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T08-B	1	1.73E+02			1.73E+02	3.8E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T09-B	1	2.17E+03			2.17E+03	5.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T01-C	1	1.09E+02			1.09E+02	2.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T02-C	1	1.20E+01	E		1.20E+01	2.4E+01	6.8E+00	2.2E+01	10	100	9.70E+02	96%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T03-C	1	3.40E+00	U1/2		3.40E+00	2.2E+02	6.8E+00	2.2E+01				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T04-C	1	3.40E+00	U1/2		3.40E+00	1.1E+04	6.8E+00	2.2E+01					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T05-C	1	3.40E+00	U1/2		3.40E+00	8.5E+01	6.8E+00	2.2E+01					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T06-C	1	3.40E+00	U1/2		3.40E+00	3.2E+02	6.8E+00	2.2E+01					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T07-C	1	1.12E+01	E		1.12E+01	4.3E+01	6.8E+00	2.2E+01					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T08-C	1	1.53E+02			1.53E+02	1.3E+00	6.8E+00	2.2E+01					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-T09-C	1	2.49E+03			2.49E+03	2.3E+00	6.8E+00	2.2E+01					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	7.5E+01	6.8E+00	2.2E+01					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	3.8E+01	6.8E+00	2.2E+01					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	6.9E+01	6.8E+00	2.2E+01					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	SWA-L01-1313-T01-A	1	5.16E+00	E		5.16E+00	1.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T02-A	1	5.78E+00	E		5.78E+00	9.7E+00	1.9E+00	6.0E+00	10	100	8.22E+02	82%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T03-A	1	1.21E+02			1.21E+02	1.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T04-A	1	6.69E+02			6.69E+02	1.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T05-A	1	8.13E+02			8.13E+02	4.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T06-A	1	8.41E+02			8.41E+02	3.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T07-A	1	1.15E+03			1.15E+03	3.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T08-A	1	6.00E+02			6.00E+02	5.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T09-A	1	6.06E+02			6.06E+02	2.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T01-B	1	5.40E+00	E		5.40E+00	3.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T02-B	1	5.26E+00	E		5.26E+00	1.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T03-B	1	1.08E+02			1.08E+02	6.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T04-B	1	4.75E+02			4.75E+02	1.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T05-B	1	6.50E+02			6.50E+02	2.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T06-B	1	8.13E+02			8.13E+02	8.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T07-B	1	1.18E+03			1.18E+03	1.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T08-B	1	6.03E+02			6.03E+02	6.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T09-B	1	6.12E+02			6.12E+02	2.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T01-C	1	6.90E+00			6.90E+00	1.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T02-C	1	5.70E+00	E		5.70E+00	4.0E+00	1.9E+00	6.0E+00	10	100	8.17E+02	81%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T03-C	1	1.31E+02			1.31E+02	4.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T04-C	1	4.82E+02			4.82E+02	7.9E-01	1.9E+00	6.0E+00					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T05-C	1	6.92E+02			6.92E+02	4.2E+00	1.9E+00	6.0E+00					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T06-C	1	6.60E+02			6.60E+02	2.0E+00	1.9E+00	6.0E+00					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T07-C	1	1.01E+03			1.01E+03	2.2E+00	1.9E+00	6.0E+00					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T08-C	1	6.27E+02			6.27E+02	5.6E+00	1.9E+00	6.0E+00					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-T09-C	1	6.20E+02			6.20E+02	1.5E+01	1.9E+00	6.0E+00					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-B01-A	1	4.06E+00	E		4.06E+00	9.0E+00	1.9E+00	6.0E+00					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-B02-A	1	4.14E+00	E		4.14E+00	1.3E+01	1.9E+00	6.0E+00					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
Li	SWA-L01-1313-B03-A	1	4.33E+00	E		4.33E+00	1.1E+01	1.9E+00	6.0E+00					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	SWA-L01-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	1.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00	10	100	1.02E+03	102%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	6.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T04-A	1	1.59E+02			1.59E+02	1.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T05-A	1	3.36E+03			3.36E+03	4.5E-01	2.0E+00	6.4E+00			---		VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T06-A	1	9.15E+03			9.15E+03	3.3E-01	2.0E+00	6.4E+00			---		VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T07-A	1	2.34E+04			2.34E+04	4.4E-01	2.0E+00	6.4E+00			---		VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T08-A	1	1.51E+04			1.51E+04	1.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T09-A	1	1.55E+04			1.55E+04	6.6E-02	2.0E+00	6.4E+00			---		VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	2.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	7.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T04-B	1	2.59E+00	E		2.59E+00	7.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T05-B	1	3.81E+02			3.81E+02	5.2E-01	2.0E+00	6.4E+00			---		VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T06-B	1	4.68E+03			4.68E+03	9.3E-01	2.0E+00	6.4E+00			---		VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T07-B	1	2.33E+04			2.33E+04	9.4E-01	2.0E+00	6.4E+00			---		VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T08-B	1	1.45E+04			1.45E+04	5.5E-01	2.0E+00	6.4E+00			---		VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T09-B	1	1.52E+04			1.52E+04	6.6E-01	2.0E+00	6.4E+00			---		VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	3.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00	10	100	1.01E+03	101%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T04-C	1	5.26E+00	E		5.26E+00	7.3E-01	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T05-C	1	3.30E+03			3.30E+03	7.8E-01	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T06-C	1	3.95E+03			3.95E+03	3.7E-01	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T07-C	1	1.76E+04			1.76E+04	2.2E-01	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T08-C	1	1.47E+04			1.47E+04	8.6E-01	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-T09-C	1	1.55E+04			1.55E+04	2.3E+00	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	2.8E+01	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	3.4E+01	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	1.0E+00	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	SWA-L01-1313-T01-A	1	6.02E+00			6.02E+00	1.1E+02	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T02-A	1	4.19E+00			4.19E+00	1.9E+02	1.0E+00	3.2E+00	1000	100	1.00E+03	100%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T03-A	1	1.57E+03			1.57E+03	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T04-A	1	7.31E+05			7.31E+05	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T05-A	1	1.09E+06			1.09E+06	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T06-A	1	1.20E+06			1.20E+06	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T07-A	1	1.60E+06			1.60E+06	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T08-A	1	7.70E+05			7.70E+05	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T09-A	1	6.62E+05			6.62E+05	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T01-B	1	4.54E+01			4.54E+01	3.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T02-B	1	8.29E+00			8.29E+00	7.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T03-B	1	1.45E+03			1.45E+03	2.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T04-B	1	3.66E+05			3.66E+05	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T05-B	1	7.66E+05			7.66E+05	9.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T06-B	1	1.10E+06			1.10E+06	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T07-B	1	1.56E+06			1.56E+06	9.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T08-B	1	7.47E+05			7.47E+05	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T09-B	1	6.50E+05			6.50E+05	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T01-C	1	2.32E+01			2.32E+01	4.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T02-C	1	6.44E+00			6.44E+00	1.8E+02	1.0E+00	3.2E+00	1000	100	9.88E+02	98%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T03-C	1	2.64E+03			2.64E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T04-C	1	4.20E+05			4.20E+05	3.1E-01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T05-C	1	9.11E+05			9.11E+05	7.0E-01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T06-C	1	9.26E+05			9.26E+05	3.6E-01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T07-C	1	1.37E+06			1.37E+06	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T08-C	1	7.54E+05			7.54E+05	6.4E-01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-T09-C	1	6.59E+05			6.59E+05	2.4E+00	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-B01-A	1	1.87E+00	E		1.87E+00	1.2E+02	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	5.9E+01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1313-B03-A	1	1.12E+00	E		1.12E+00	3.6E+02	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	SWA-L01-1313-T01-A	1	1.35E+02			1.35E+02	6.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T02-A	1	1.40E+02			1.40E+02	1.5E+00	1.2E+00	3.8E+00	10	100	1.17E+03	103%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T03-A	1	1.50E+02			1.50E+02	1.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T04-A	1	1.49E+02			1.49E+02	9.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T05-A	1	1.28E+02			1.28E+02	1.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T06-A	1	1.03E+02			1.03E+02	2.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T07-A	1	2.65E+01			2.65E+01	1.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T08-A	1	1.35E+01			1.35E+01	8.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T09-A	1	6.75E+00			6.75E+00	3.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T01-B	1	1.42E+02			1.42E+02	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T02-B	1	1.49E+02			1.49E+02	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T03-B	1	1.52E+02			1.52E+02	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T04-B	1	1.51E+02			1.51E+02	6.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T05-B	1	1.40E+02			1.40E+02	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T06-B	1	1.20E+02			1.20E+02	7.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T07-B	1	2.98E+01			2.98E+01	1.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T08-B	1	1.27E+01			1.27E+01	8.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T09-B	1	6.74E+00			6.74E+00	3.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T01-C	1	1.44E+02			1.44E+02	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T02-C	1	1.41E+02			1.41E+02	5.3E-01	1.2E+00	3.8E+00	10	100	1.17E+03	103%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T03-C	1	1.38E+02			1.38E+02	8.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T04-C	1	1.49E+02			1.49E+02	1.3E+00	1.2E+00	3.8E+00					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T05-C	1	1.19E+02			1.19E+02	2.8E+00	1.2E+00	3.8E+00					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T06-C	1	1.15E+02			1.15E+02	3.0E+00	1.2E+00	3.8E+00					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T07-C	1	2.95E+01			2.95E+01	1.1E+01	1.2E+00	3.8E+00					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T08-C	1	1.17E+01			1.17E+01	1.2E+01	1.2E+00	3.8E+00					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-T09-C	1	5.54E+00			5.54E+00	3.4E+01	1.2E+00	3.8E+00					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-B01-A	1	1.60E+00	E		1.60E+00	4.1E+01	1.2E+00	3.8E+00					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-B02-A	1	1.98E+00	E		1.98E+00	9.2E+00	1.2E+00	3.8E+00					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1313-B03-A	1	3.95E+00			3.95E+00	1.5E+01	1.2E+00	3.8E+00					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	SWA-L01-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	6.2E+01	1.8E+00	5.7E+00	10	100	9.87E+02	99%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T03-A	1	3.29E+00	E		3.29E+00	3.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T04-A	1	1.12E+01			1.12E+01	1.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T05-A	1	3.29E+01			3.29E+01	1.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T06-A	1	1.08E+02			1.08E+02	3.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T07-A	1	3.99E+02			3.99E+02	6.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T08-A	1	3.23E+02			3.23E+02	2.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T09-A	1	3.38E+02			3.38E+02	3.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	1.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	7.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T03-B	1	4.53E+00	E		4.53E+00	3.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T04-B	1	7.23E+00			7.23E+00	4.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T05-B	1	1.48E+01			1.48E+01	1.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T06-B	1	4.62E+01			4.62E+01	1.9E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T07-B	1	4.24E+02			4.24E+02	1.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T08-B	1	3.16E+02			3.16E+02	5.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T09-B	1	3.32E+02			3.32E+02	3.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	5.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	6.1E+02	1.8E+00	5.7E+00	10	100	9.86E+02	98%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T03-C	1	2.93E+00	E		2.93E+00	3.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T04-C	1	7.54E+00			7.54E+00	1.6E+01	1.8E+00	5.7E+00					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T05-C	1	2.60E+01			2.60E+01	3.7E+00	1.8E+00	5.7E+00					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T06-C	1	3.16E+01			3.16E+01	2.9E+00	1.8E+00	5.7E+00					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T07-C	1	3.08E+02			3.08E+02	3.0E-01	1.8E+00	5.7E+00					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T08-C	1	3.19E+02			3.19E+02	4.3E-01	1.8E+00	5.7E+00					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-T09-C	1	3.36E+02			3.36E+02	2.3E+00	1.8E+00	5.7E+00					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	4.0E+01	1.8E+00	5.7E+00					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	1.6E+02	1.8E+00	5.7E+00					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	9.7E+01	1.8E+00	5.7E+00					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	SWA-L01-1313-T01-A	1		U1/2		0.00E+00	2.2E+00	3.7E+00	1.2E+01			---		VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T02-A	1		U1/2		0.00E+00	3.8E+01	3.7E+00	1.2E+01	1000	100	1.18E+03	118%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T03-A	1		U1/2		0.00E+00	1.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T04-A	1		U1/2		0.00E+00	6.6E+00	3.7E+00	1.2E+01			---		VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T05-A	1		U1/2		0.00E+00	2.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T06-A	1		U1/2		0.00E+00	2.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T07-A	1		U1/2		0.00E+00	8.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T08-A	1		U1/2		0.00E+00	1.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T09-A	1		U1/2		0.00E+00	1.0E+00	3.7E+00	1.2E+01			---		VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T01-B	1		U1/2		0.00E+00	2.8E+00	3.7E+00	1.2E+01			---		VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T02-B	1		U1/2		0.00E+00	2.6E+01	3.7E+00	1.2E+01			---		VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T03-B	1		U1/2		0.00E+00	1.2E+02	3.7E+00	1.2E+01			---		VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T04-B	1		U1/2		0.00E+00	1.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T05-B	1		U1/2		0.00E+00	1.9E+01	3.7E+00	1.2E+01			---		VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T06-B	1		U1/2		0.00E+00	1.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T07-B	1		U1/2		0.00E+00	2.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T08-B	1		U1/2		0.00E+00	1.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T09-B	1		U1/2		0.00E+00	4.7E-01	3.7E+00	1.2E+01			---		VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T01-C	1		U1/2		0.00E+00	3.6E+00	3.7E+00	1.2E+01			---		VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T02-C	1		U1/2		0.00E+00	3.0E+01	3.7E+00	1.2E+01	1000	100	1.19E+03	119%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T03-C	1		U1/2		0.00E+00	5.6E+01	3.7E+00	1.2E+01			---		VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T04-C	1		U1/2		0.00E+00	2.7E+01	3.7E+00	1.2E+01					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T05-C	1		U1/2		0.00E+00	1.9E+01	3.7E+00	1.2E+01					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T06-C	1		U1/2		0.00E+00	4.5E+01	3.7E+00	1.2E+01					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T07-C	1		U1/2		0.00E+00	4.0E+01	3.7E+00	1.2E+01					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T08-C	1		U1/2		0.00E+00	2.5E+00	3.7E+00	1.2E+01					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-T09-C	1		U1/2		0.00E+00	2.5E+00	3.7E+00	1.2E+01					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-B01-A	1		U1/2		0.00E+00	6.8E+01	3.7E+00	1.2E+01					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-B02-A	1		U1/2		0.00E+00	2.6E+01	3.7E+00	1.2E+01					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1313-B03-A	1		U1/2		0.00E+00	2.2E+01	3.7E+00	1.2E+01					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	SWA-L01-1313-T01-A	1	3.77E+05			3.77E+05	2.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T02-A	1	2.76E+05			2.76E+05	4.1E-01	1.6E+00	5.1E+00	1000	100	2.77E+05	85%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T03-A	1	3.82E+05			3.82E+05	8.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T04-A	1	4.12E+05			4.12E+05	1.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T05-A	1	4.23E+05			4.23E+05	2.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T06-A	1	4.29E+05			4.29E+05	2.9E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T07-A	1	4.64E+05			4.64E+05	3.4E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T08-A	1	2.20E+05			2.20E+05	9.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T09-A	1	2.43E+05			2.43E+05	1.2E+01	1.6E+00	5.1E+00				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T01-B	1	1.80E+06			1.80E+06	5.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T02-B	1	2.83E+05			2.83E+05	1.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T03-B	1	3.79E+05			3.79E+05	4.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T04-B	1	4.16E+05			4.16E+05	3.9E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T05-B	1	3.95E+05			3.95E+05	3.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T06-B	1	4.05E+05			4.05E+05	9.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T07-B	1	4.64E+05			4.64E+05	8.4E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T08-B	1	2.39E+05			2.39E+05	7.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T09-B	1	2.60E+05			2.60E+05	1.0E+01	1.6E+00	5.1E+00				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T01-C	1	1.72E+06			1.72E+06	8.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T02-C	1	2.73E+05			2.73E+05	1.5E+00	1.6E+00	5.1E+00	1000	100	2.74E+05	88%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T03-C	1	3.63E+05			3.63E+05	1.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T04-C	1	3.96E+05			3.96E+05	1.8E+00	1.6E+00	5.1E+00					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T05-C	1	3.85E+05			3.85E+05	5.9E-01	1.6E+00	5.1E+00					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T06-C	1	3.85E+05			3.85E+05	1.1E+00	1.6E+00	5.1E+00					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T07-C	1	4.26E+05			4.26E+05	3.3E+00	1.6E+00	5.1E+00					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T08-C	1	2.43E+05			2.43E+05	4.9E+00	1.6E+00	5.1E+00					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-T09-C	1	2.49E+05			2.49E+05	2.7E+00	1.6E+00	5.1E+00					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-B01-A	1	1.78E+01			1.78E+01	9.5E+00	1.6E+00	5.1E+00					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-B02-A	1	9.14E+00			9.14E+00	2.2E+01	1.6E+00	5.1E+00					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1313-B03-A	1	4.31E+04			4.31E+04	6.5E-01	1.6E+00	5.1E+00					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	SWA-L01-1313-T01-A	1	9.58E+04			9.58E+04	3.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T02-A	1	9.81E+04			9.81E+04	4.1E-01	1.5E+01	4.8E+01	10	100	9.90E+04	93%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T03-A	1	1.02E+05			1.02E+05	4.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T04-A	1	1.25E+05			1.25E+05	1.2E+00	1.5E+01	4.8E+01				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T05-A	1	1.28E+05			1.28E+05	2.3E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T06-A	1	1.27E+05			1.27E+05	3.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T07-A	1	1.30E+05			1.30E+05	8.1E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T08-A	1	4.90E+04			4.90E+04	1.0E+00	1.5E+01	4.8E+01				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T09-A	1	3.46E+04			3.46E+04	2.9E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T01-B	1	9.89E+04			9.89E+04	5.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T02-B	1	1.02E+05			1.02E+05	8.8E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T03-B	1	1.03E+05			1.03E+05	1.5E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T04-B	1	1.16E+05			1.16E+05	1.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T05-B	1	1.19E+05			1.19E+05	2.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T06-B	1	1.24E+05			1.24E+05	8.5E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T07-B	1	1.27E+05			1.27E+05	7.5E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T08-B	1	4.83E+04			4.83E+04	6.5E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T09-B	1	3.45E+04			3.45E+04	5.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T01-C	1	1.03E+05			1.03E+05	1.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T02-C	1	9.79E+04			9.79E+04	3.1E-01	1.5E+01	4.8E+01	10	100	9.87E+04	85%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T03-C	1	9.79E+04			9.79E+04	2.3E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T04-C	1	1.14E+05			1.14E+05	5.1E-01	1.5E+01	4.8E+01					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T05-C	1	1.13E+05			1.13E+05	7.9E-01	1.5E+01	4.8E+01					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T06-C	1	1.12E+05			1.12E+05	4.5E-01	1.5E+01	4.8E+01					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T07-C	1	1.21E+05			1.21E+05	4.3E-01	1.5E+01	4.8E+01					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T08-C	1	4.88E+04			4.88E+04	2.5E-01	1.5E+01	4.8E+01					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-T09-C	1	3.64E+04			3.64E+04	3.1E+00	1.5E+01	4.8E+01					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-B01-A	1	7.50E+00	U1/2		7.50E+00	3.3E+02	1.5E+01	4.8E+01					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-B02-A	1	7.50E+00	U1/2		7.50E+00	4.4E+02	1.5E+01	4.8E+01					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1313-B03-A	1	7.50E+00	U1/2		7.50E+00	3.3E+02	1.5E+01	4.8E+01					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	SWA-L01-1313-T01-A	1	9.27E+03			9.27E+03	1.4E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T02-A	1	5.51E+03			5.51E+03	7.0E-01	1.1E+00	3.5E+00	1000	100	6.39E+03	88%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T03-A	1	1.55E+03			1.55E+03	3.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T04-A	1	1.27E+03			1.27E+03	1.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T05-A	1	9.28E+02			9.28E+02	1.2E+01	1.1E+00	3.5E+00				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T06-A	1	1.61E+03			1.61E+03	1.6E+01	1.1E+00	3.5E+00				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T07-A	1	2.90E+03			2.90E+03	3.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T08-A	1	1.27E+04			1.27E+04	7.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T09-A	1	3.81E+03			3.81E+03	7.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T01-B	1	1.02E+04			1.02E+04	5.9E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T02-B	1	5.85E+03			5.85E+03	7.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T03-B	1	1.53E+03			1.53E+03	7.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T04-B	1	1.17E+03			1.17E+03	2.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T05-B	1	7.89E+02			7.89E+02	2.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T06-B	1	1.23E+03			1.23E+03	8.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T07-B	1	2.49E+03			2.49E+03	4.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T08-B	1	1.25E+04			1.25E+04	3.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T09-B	1	3.81E+03			3.81E+03	3.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T01-C	1	9.66E+03			9.66E+03	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T02-C	1	5.88E+03			5.88E+03	6.7E-01	1.1E+00	3.5E+00	1000	100	6.72E+03	85%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T03-C	1	1.60E+03			1.60E+03	3.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T04-C	1	9.80E+02			9.80E+02	6.8E-01	1.1E+00	3.5E+00					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T05-C	1	6.98E+02			6.98E+02	8.3E+00	1.1E+00	3.5E+00					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T06-C	1	8.55E+02			8.55E+02	8.1E-01	1.1E+00	3.5E+00					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T07-C	1	1.90E+03			1.90E+03	5.9E+00	1.1E+00	3.5E+00					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T08-C	1	1.22E+04			1.22E+04	1.8E-01	1.1E+00	3.5E+00					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-T09-C	1	2.36E+03			2.36E+03	2.6E+00	1.1E+00	3.5E+00					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-B01-A	1	5.50E-01	U1/2		5.50E-01	8.9E+01	1.1E+00	3.5E+00					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-B02-A	1	3.64E+00			3.64E+00	5.8E+00	1.1E+00	3.5E+00					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1313-B03-A	1	1.94E+02			1.94E+02	2.1E+01	1.1E+00	3.5E+00					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	SWA-L01-1313-T01-A	1	4.13E+05			4.13E+05	3.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T02-A	1	3.43E+05			3.43E+05	5.1E-01	2.5E+00	8.0E+00	1000	100	3.44E+05	90%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T03-A	1	3.60E+05			3.60E+05	8.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T04-A	1	3.50E+05			3.50E+05	1.5E+00	2.5E+00	8.0E+00				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T05-A	1	3.41E+05			3.41E+05	5.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T06-A	1	3.41E+05			3.41E+05	1.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T07-A	1	3.34E+05			3.34E+05	7.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T08-A	1	3.38E+05			3.38E+05	4.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T09-A	1	3.33E+05			3.33E+05	4.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T01-B	1	3.15E+05			3.15E+05	3.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T02-B	1	3.46E+05			3.46E+05	7.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T03-B	1	3.63E+05			3.63E+05	5.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T04-B	1	3.50E+05			3.50E+05	1.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T05-B	1	3.47E+05			3.47E+05	6.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T06-B	1	3.41E+05			3.41E+05	1.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T07-B	1	3.37E+05			3.37E+05	9.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T08-B	1	3.36E+05			3.36E+05	6.8E-02	2.5E+00	8.0E+00				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T09-B	1	3.37E+05			3.37E+05	5.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T01-C	1	3.27E+05			3.27E+05	8.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T02-C	1	3.43E+05			3.43E+05	4.7E-01	2.5E+00	8.0E+00	1000	100	3.44E+05	89%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T03-C	1	3.56E+05			3.56E+05	3.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T04-C	1	3.51E+05			3.51E+05	1.4E+00	2.5E+00	8.0E+00					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T05-C	1	3.43E+05			3.43E+05	7.1E-01	2.5E+00	8.0E+00					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T06-C	1	3.41E+05			3.41E+05	2.2E-01	2.5E+00	8.0E+00					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T07-C	1	3.40E+05			3.40E+05	1.9E-01	2.5E+00	8.0E+00					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T08-C	1	3.37E+05			3.37E+05	9.2E-01	2.5E+00	8.0E+00					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-T09-C	1	3.38E+05			3.38E+05	3.3E-01	2.5E+00	8.0E+00					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-B01-A	1	2.78E+01			2.78E+01	1.2E+01	2.5E+00	8.0E+00					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-B02-A	1	3.04E+00	E		3.04E+00	6.6E+01	2.5E+00	8.0E+00					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1313-B03-A	1	4.04E+01			4.04E+01	2.1E-01	2.5E+00	8.0E+00					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	SWA-L01-1313-T01-A	1	3.79E+02			3.79E+02	5.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T02-A	1	4.02E+02			4.02E+02	5.0E-01	1.0E+00	3.2E+00	1000	100	1.43E+03	103%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T03-A	1	1.69E+04			1.69E+04	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T04-A	1	3.62E+04			3.62E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T05-A	1	4.17E+04			4.17E+04	2.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T06-A	1	4.35E+04			4.35E+04	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T07-A	1	5.47E+04			5.47E+04	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T08-A	1	2.66E+04			2.66E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T09-A	1	2.26E+04			2.26E+04	8.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T01-B	1	4.18E+02			4.18E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T02-B	1	4.09E+02			4.09E+02	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T03-B	1	1.64E+04			1.64E+04	3.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T04-B	1	3.03E+04			3.03E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T05-B	1	3.58E+04			3.58E+04	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T06-B	1	4.11E+04			4.11E+04	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T07-B	1	5.24E+04			5.24E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T08-B	1	2.56E+04			2.56E+04	5.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T09-B	1	2.20E+04			2.20E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T01-C	1	4.11E+02			4.11E+02	2.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T02-C	1	3.79E+02			3.79E+02	6.8E-01	1.0E+00	3.2E+00	1000	100	1.43E+03	105%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T03-C	1	1.64E+04			1.64E+04	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T04-C	1	2.96E+04			2.96E+04	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T05-C	1	3.69E+04			3.69E+04	5.1E-01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T06-C	1	3.73E+04			3.73E+04	7.4E-01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T07-C	1	4.82E+04			4.82E+04	6.0E-01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T08-C	1	2.59E+04			2.59E+04	4.4E-01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-T09-C	1	2.33E+04			2.33E+04	3.0E+00	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	2.7E+01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	7.7E+01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	4.9E+02	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	SWA-L01-1313-T01-A	1	4.75E+05			4.75E+05	2.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T02-A	1	8.37E+05			8.37E+05	5.9E-01	6.8E+00	2.2E+01	1000	100	8.38E+05	86%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T03-A	1	5.15E+05			5.15E+05	3.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T04-A	1	4.88E+05			4.88E+05	1.3E+00	6.8E+00	2.2E+01			---		VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T05-A	1	4.88E+05			4.88E+05	2.7E-02	6.8E+00	2.2E+01			---		VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T06-A	1	5.12E+05			5.12E+05	1.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T07-A	1	5.34E+05			5.34E+05	7.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T08-A	1	2.21E+05			2.21E+05	7.7E-01	6.8E+00	2.2E+01			---		VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T09-A	1	1.67E+05			1.67E+05	3.7E-01	6.8E+00	2.2E+01			---		VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T01-B	1	3.64E+05			3.64E+05	6.9E-01	6.8E+00	2.2E+01			---		VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T02-B	1	7.61E+05			7.61E+05	7.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T03-B	1	5.21E+05			5.21E+05	6.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T04-B	1	5.19E+05			5.19E+05	6.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T05-B	1	4.55E+05			4.55E+05	4.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T06-B	1	4.79E+05			4.79E+05	7.9E-01	6.8E+00	2.2E+01			---		VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T07-B	1	5.24E+05			5.24E+05	7.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T08-B	1	2.16E+05			2.16E+05	3.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T09-B	1	1.65E+05			1.65E+05	2.8E-01	6.8E+00	2.2E+01			---		VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T01-C	1	4.89E+05			4.89E+05	9.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T02-C	1	7.35E+05			7.35E+05	2.6E-01	6.8E+00	2.2E+01	1000	100	7.36E+05	89%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T03-C	1	4.91E+05			4.91E+05	2.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T04-C	1	4.97E+05			4.97E+05	4.0E-01	6.8E+00	2.2E+01					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T05-C	1	4.38E+05			4.38E+05	5.3E-01	6.8E+00	2.2E+01					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T06-C	1	4.27E+05			4.27E+05	5.8E-01	6.8E+00	2.2E+01					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T07-C	1	4.88E+05			4.88E+05	4.0E-01	6.8E+00	2.2E+01					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T08-C	1	2.17E+05			2.17E+05	1.9E-01	6.8E+00	2.2E+01					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-T09-C	1	1.65E+05			1.65E+05	2.7E+00	6.8E+00	2.2E+01					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-B01-A	1	3.36E+01			3.36E+01	2.8E+01	6.8E+00	2.2E+01					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	2.8E+01	6.8E+00	2.2E+01					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1313-B03-A	1	1.34E+02			1.34E+02	4.5E+00	6.8E+00	2.2E+01					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	SWA-L01-1313-T01-A	1	2.30E+00	U1/2		2.30E+00	3.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T02-A	1	2.30E+00	U1/2		2.30E+00	8.2E+02	4.6E+00	1.5E+01	10	100	9.23E+02	92%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T03-A	1	2.30E+00	U1/2		2.30E+00	9.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T04-A	1	2.30E+00	U1/2		2.30E+00	1.1E+02	4.6E+00	1.5E+01				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T05-A	1	2.30E+00	U1/2		2.30E+00	4.6E+02	4.6E+00	1.5E+01				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T06-A	1	1.18E+01	E		1.18E+01	6.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T07-A	1	2.87E+01			2.87E+01	2.9E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T08-A	1	1.05E+01	E		1.05E+01	2.8E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T09-A	1	1.43E+01	E		1.43E+01	6.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T01-B	1	2.30E+00	U1/2		2.30E+00	4.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T02-B	1	2.30E+00	U1/2		2.30E+00	1.2E+02	4.6E+00	1.5E+01				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T03-B	1	2.30E+00	U1/2		2.30E+00	2.0E+02	4.6E+00	1.5E+01				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T04-B	1	2.30E+00	U1/2		2.30E+00	2.0E+03	4.6E+00	1.5E+01				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T05-B	1	2.30E+00	U1/2		2.30E+00	1.1E+02	4.6E+00	1.5E+01				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T06-B	1	8.40E+00	E		8.40E+00	1.1E+02	4.6E+00	1.5E+01				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T07-B	1	2.49E+01			2.49E+01	3.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T08-B	1	9.02E+00	E		9.02E+00	1.9E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T09-B	1	1.59E+01			1.59E+01	2.4E+00	4.6E+00	1.5E+01				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T01-C	1	2.30E+00	U1/2		2.30E+00	2.8E+03	4.6E+00	1.5E+01				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T02-C	1	2.30E+00	U1/2		2.30E+00	6.3E+02	4.6E+00	1.5E+01	10	100	9.11E+02	91%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T03-C	1	2.30E+00	U1/2		2.30E+00	2.4E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T04-C	1	2.30E+00	U1/2		2.30E+00	5.7E+02	4.6E+00	1.5E+01					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T05-C	1	2.30E+00	U1/2		2.30E+00	7.6E+01	4.6E+00	1.5E+01					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T06-C	1	5.94E+00	E		5.94E+00	5.7E+01	4.6E+00	1.5E+01					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T07-C	1	2.36E+01			2.36E+01	2.2E+01	4.6E+00	1.5E+01					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T08-C	1	9.90E+00	E		9.90E+00	1.5E+01	4.6E+00	1.5E+01					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-T09-C	1	1.57E+01			1.57E+01	2.7E+01	4.6E+00	1.5E+01					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	8.4E+01	4.6E+00	1.5E+01					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	1.1E+02	4.6E+00	1.5E+01					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	1.5E+02	4.6E+00	1.5E+01					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	SWA-L01-1313-T01-A	1	2.96E+00	E		2.96E+00	1.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00	10	100	1.01E+03	101%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	4.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	3.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	2.7E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	1.7E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T08-A	1	3.75E+01			3.75E+01	5.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T09-A	1	5.81E+01			5.81E+01	1.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T01-B	1	4.95E+00	E		4.95E+00	2.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	3.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	2.8E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	2.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	2.8E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	1.8E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T08-B	1	3.96E+01			3.96E+01	5.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T09-B	1	6.26E+01			6.26E+01	3.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T01-C	1	2.05E+00	E		2.05E+00	4.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	6.5E+01	2.0E+00	6.4E+00	10	100	9.96E+02	100%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	2.6E+01	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	7.1E+02	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	3.2E+01	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	8.3E+01	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T08-C	1	3.40E+01			3.40E+01	9.6E-01	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-T09-C	1	5.86E+01			5.86E+01	2.5E+00	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	5.0E+00	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	6.4E+01	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1313-B03-A	1	4.01E+00	E		4.01E+00	7.9E+00	2.0E+00	6.4E+00					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	SWA-L01-1313-T01-A	1	4.68E+02			4.68E+02	3.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T02-A	1	3.44E+02			3.44E+02	2.2E-01	1.5E+00	4.8E+00	10	100	1.33E+03	99%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T03-A	1	1.33E+02			1.33E+02	1.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T04-A	1	2.51E+02			2.51E+02	6.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T05-A	1	2.29E+02			2.29E+02	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T06-A	1	2.09E+02			2.09E+02	5.6E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T07-A	1	2.16E+02			2.16E+02	1.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T08-A	1	9.66E+01			9.66E+01	1.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T09-A	1	1.99E+02			1.99E+02	6.8E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T01-B	1	4.66E+02			4.66E+02	1.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T02-B	1	3.60E+02			3.60E+02	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T03-B	1	1.31E+02			1.31E+02	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T04-B	1	1.94E+02			1.94E+02	6.9E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T05-B	1	2.25E+02			2.25E+02	4.6E-02	1.5E+00	4.8E+00				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T06-B	1	2.09E+02			2.09E+02	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T07-B	1	2.02E+02			2.02E+02	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T08-B	1	9.22E+01			9.22E+01	1.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T09-B	1	2.36E+02			2.36E+02	2.8E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T01-C	1	4.64E+02			4.64E+02	1.9E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T02-C	1	3.61E+02			3.61E+02	9.0E-01	1.5E+00	4.8E+00	10	100	1.36E+03	100%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T03-C	1	1.29E+02			1.29E+02	3.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T04-C	1	1.99E+02			1.99E+02	2.3E-01	1.5E+00	4.8E+00					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T05-C	1	1.85E+02			1.85E+02	1.5E+00	1.5E+00	4.8E+00					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T06-C	1	1.80E+02			1.80E+02	3.8E-01	1.5E+00	4.8E+00					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T07-C	1	1.99E+02			1.99E+02	1.5E+00	1.5E+00	4.8E+00					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T08-C	1	9.24E+01			9.24E+01	7.3E-01	1.5E+00	4.8E+00					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-T09-C	1	2.59E+02			2.59E+02	3.2E+00	1.5E+00	4.8E+00					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-B01-A	1	7.50E-01	U1/2		7.50E-01	6.6E+01	1.5E+00	4.8E+00					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-B02-A	1	7.50E-01	U1/2		7.50E-01	4.5E+01	1.5E+00	4.8E+00					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1313-B03-A	1	7.50E-01	U1/2		7.50E-01	3.1E+01	1.5E+00	4.8E+00					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	SWA-L01-1313-T01-A	1	2.01E+01			2.01E+01	5.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:21 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T02-A	1	1.74E+01			1.74E+01	1.7E+00	1.0E+00	3.2E+00	10	100	1.12E+03	110%	VU ICP-OES	11/1/10 11:22 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T03-A	1	1.74E+01			1.74E+01	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:24 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T04-A	1	2.05E+01			2.05E+01	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:26 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T05-A	1	1.95E+01			1.95E+01	4.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:27 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T06-A	1	1.75E+01			1.75E+01	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:29 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T07-A	1	2.75E+02			2.75E+02	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:31 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T08-A	1	1.33E+03			1.33E+03	4.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:32 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T09-A	1	1.89E+03			1.89E+03	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:34 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T01-B	1	2.00E+01			2.00E+01	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:36 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T02-B	1	1.78E+01			1.78E+01	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:37 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T03-B	1	1.75E+01			1.75E+01	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:39 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T04-B	1	1.77E+01			1.77E+01	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:41 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T05-B	1	1.72E+01			1.72E+01	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:42 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T06-B	1	1.83E+01			1.83E+01	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:49 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T07-B	1	3.17E+02			3.17E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:50 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T08-B	1	1.32E+03			1.32E+03	9.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:52 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T09-B	1	1.90E+03			1.90E+03	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:54 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T01-C	1	1.46E+01			1.46E+01	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:55 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T02-C	1	1.58E+01			1.58E+01	2.4E+00	1.0E+00	3.2E+00	10	100	1.13E+03	111%	VU ICP-OES	11/1/10 11:57 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T03-C	1	1.66E+01			1.66E+01	2.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/1/10 11:59 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T04-C	1	1.79E+01			1.79E+01	1.8E+00	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:00 PM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T05-C	1	1.63E+01			1.63E+01	8.2E+00	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:02 PM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T06-C	1	1.85E+01			1.85E+01	4.2E+00	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:04 PM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T07-C	1	1.56E+02			1.56E+02	2.8E-01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:05 PM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T08-C	1	1.33E+03			1.33E+03	6.2E-01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:07 PM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-T09-C	1	1.94E+03			1.94E+03	3.4E+00	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 12:09 PM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	7.3E-01	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 11:16 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	5.3E+00	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 11:18 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1313-B03-A	1	3.40E+00			3.40E+00	1.7E+00	1.0E+00	3.2E+00					VU ICP-OES	11/1/10 11:19 AM	EPA Interlab L01 1313-1316 SWA

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	SWA-L02-1313-T01-A	1	3.53E+04			3.53E+04	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T02-A	1	1.57E+04			1.57E+04	7.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T03-A	1	3.46E+04			3.46E+04	5.4E-01	1.0E+00	3.2E+00	1000	125	3.58E+04	97%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T04-A	1	3.14E+03			3.14E+03	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T05-A	1	2.52E+02			2.52E+02	2.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T06-A	1	5.00E-01	U1/2		5.00E-01	7.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T07-A	1	2.86E+02			2.86E+02	6.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T08-A	1	3.27E+05			3.27E+05	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T09-A	1	1.20E+06			1.20E+06	2.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T01-B	1	3.87E+04			3.87E+04	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T02-B	1	1.61E+04			1.61E+04	2.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T03-B	1	2.89E+04			2.89E+04	2.4E+00	1.0E+00	3.2E+00	1000	125	3.01E+04	91%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T04-B	1	2.67E+03			2.67E+03	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T05-B	1	3.11E+02			3.11E+02	6.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T06-B	1	1.35E+02			1.35E+02	1.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T07-B	1	3.26E+02			3.26E+02	6.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T08-B	1	4.13E+05			4.13E+05	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T09-B	1	1.11E+06			1.11E+06	9.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T01-C	1	3.69E+04			3.69E+04	9.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T02-C	1	1.64E+04			1.64E+04	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T03-C	1	2.81E+04			2.81E+04	3.7E+00	1.0E+00	3.2E+00	1000	125	2.94E+04	98%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T04-C	1	3.75E+02			3.75E+02	5.0E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T05-C	1	2.26E+02			2.26E+02	2.3E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T06-C	1	2.48E+02			2.48E+02	2.9E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T07-C	1	3.08E+02			3.08E+02	4.1E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T08-C	1	4.39E+05			4.39E+05	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-T09-C	1	1.16E+06			1.16E+06	5.3E-01	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.4E+01	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	SWA-L02-1313-T01-A	1	4.40E+03			4.40E+03	9.4E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T02-A	1	3.37E+03			3.37E+03	3.5E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T03-A	1	5.00E+03			5.00E+03	9.9E-01	7.5E+00	2.4E+01	10	125	6.24E+03	99%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T04-A	1	2.33E+03			2.33E+03	2.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T05-A	1	2.06E+03			2.06E+03	1.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T06-A	1	1.87E+03			1.87E+03	1.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T07-A	1	1.52E+03			1.52E+03	2.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T08-A	1	1.69E+03			1.69E+03	6.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T09-A	1	5.90E+02			5.90E+02	9.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T01-B	1	4.59E+03			4.59E+03	1.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T02-B	1	3.25E+03			3.25E+03	2.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T03-B	1	4.20E+03			4.20E+03	2.5E+00	7.5E+00	2.4E+01	10	125	5.45E+03	100%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T04-B	1	2.32E+03			2.32E+03	4.3E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T05-B	1	2.10E+03			2.10E+03	5.6E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T06-B	1	1.96E+03			1.96E+03	1.8E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T07-B	1	1.63E+03			1.63E+03	2.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T08-B	1	1.01E+03			1.01E+03	1.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T09-B	1	5.45E+02			5.45E+02	1.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T01-C	1	4.06E+03			4.06E+03	9.1E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T02-C	1	3.25E+03			3.25E+03	1.9E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T03-C	1	4.09E+03			4.09E+03	2.7E+00	7.5E+00	2.4E+01	10	125	5.30E+03	96%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T04-C	1	2.05E+03			2.05E+03	1.5E+00	7.5E+00	2.4E+01					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T05-C	1	2.08E+03			2.08E+03	1.2E+00	7.5E+00	2.4E+01					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T06-C	1	1.85E+03			1.85E+03	1.8E+00	7.5E+00	2.4E+01					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T07-C	1	1.53E+03			1.53E+03	1.5E+00	7.5E+00	2.4E+01					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T08-C	1	1.02E+03			1.02E+03	1.8E+00	7.5E+00	2.4E+01					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-T09-C	1	5.68E+02			5.68E+02	7.8E+00	7.5E+00	2.4E+01					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-B01-A	1	3.75E+00	U1/2		3.75E+00	1.1E+02	7.5E+00	2.4E+01					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-B02-A	1	3.75E+00	U1/2		3.75E+00	8.0E+01	7.5E+00	2.4E+01					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1313-B03-A	1	3.75E+00	U1/2		3.75E+00	1.3E+02	7.5E+00	2.4E+01					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	SWA-L02-1313-T01-A	1	4.68E+03			4.68E+03	9.4E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T02-A	1	1.49E+03			1.49E+03	1.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T03-A	1	4.68E+03			4.68E+03	8.6E-01	1.1E+01	3.5E+01	10	125	5.92E+03	99%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T04-A	1	9.15E+02			9.15E+02	3.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T05-A	1	3.34E+02			3.34E+02	2.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T06-A	1	2.67E+02			2.67E+02	6.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T07-A	1	4.18E+02			4.18E+02	8.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T08-A	1	5.05E+03			5.05E+03	8.2E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T09-A	1	1.16E+04			1.16E+04	1.0E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T01-B	1	5.18E+03			5.18E+03	6.4E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T02-B	1	1.56E+03			1.56E+03	3.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T03-B	1	3.89E+03			3.89E+03	1.9E+00	1.1E+01	3.5E+01	10	125	5.21E+03	105%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T04-B	1	8.88E+02			8.88E+02	2.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T05-B	1	3.68E+02			3.68E+02	1.1E+01	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T06-B	1	2.82E+02			2.82E+02	4.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T07-B	1	4.22E+02			4.22E+02	6.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T08-B	1	4.13E+03			4.13E+03	1.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T09-B	1	1.05E+04			1.05E+04	2.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T01-C	1	4.75E+03			4.75E+03	1.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T02-C	1	1.61E+03			1.61E+03	1.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T03-C	1	3.84E+03			3.84E+03	2.8E+00	1.1E+01	3.5E+01	10	125	5.23E+03	112%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T04-C	1	5.95E+02			5.95E+02	3.4E+00	1.1E+01	3.5E+01					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T05-C	1	2.99E+02			2.99E+02	6.9E+00	1.1E+01	3.5E+01					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T06-C	1	2.57E+02			2.57E+02	7.7E-01	1.1E+01	3.5E+01					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T07-C	1	3.86E+02			3.86E+02	7.6E+00	1.1E+01	3.5E+01					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T08-C	1	4.43E+03			4.43E+03	1.1E+00	1.1E+01	3.5E+01					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-T09-C	1	1.11E+04			1.11E+04	9.2E-01	1.1E+01	3.5E+01					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-B01-A	1	5.50E+00	U1/2		5.50E+00	3.8E+02	1.1E+01	3.5E+01					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-B02-A	1	5.50E+00	U1/2		5.50E+00	4.3E+02	1.1E+01	3.5E+01					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1313-B03-A	1	5.50E+00	U1/2		5.50E+00	1.5E+02	1.1E+01	3.5E+01					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	SWA-L02-1313-T01-A	1	8.05E+02			8.05E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T02-A	1	6.16E+02			6.16E+02	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T03-A	1	8.63E+02			8.63E+02	1.3E+00	1.0E+00	3.2E+00	1000	125	2.15E+03	103%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T04-A	1	1.58E+03			1.58E+03	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T05-A	1	2.52E+03			2.52E+03	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T06-A	1	4.33E+03			4.33E+03	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T07-A	1	5.51E+03			5.51E+03	5.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T08-A	1	7.49E+03			7.49E+03	9.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T09-A	1	9.85E+03			9.85E+03	2.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T01-B	1	8.87E+02			8.87E+02	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T02-B	1	6.51E+02			6.51E+02	3.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T03-B	1	7.41E+02			7.41E+02	2.1E+00	1.0E+00	3.2E+00	1000	125	2.05E+03	105%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T04-B	1	1.64E+03			1.64E+03	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T05-B	1	2.77E+03			2.77E+03	2.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T06-B	1	4.30E+03			4.30E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T07-B	1	5.70E+03			5.70E+03	8.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T08-B	1	7.04E+03			7.04E+03	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T09-B	1	8.89E+03			8.89E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T01-C	1	8.07E+02			8.07E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T02-C	1	7.32E+02			7.32E+02	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T03-C	1	7.27E+02			7.27E+02	2.5E+00	1.0E+00	3.2E+00	1000	125	2.02E+03	103%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T04-C	1	1.63E+03			1.63E+03	2.9E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T05-C	1	2.92E+03			2.92E+03	8.4E-01	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T06-C	1	3.78E+03			3.78E+03	1.8E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T07-C	1	5.12E+03			5.12E+03	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T08-C	1	7.45E+03			7.45E+03	7.8E-01	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-T09-C	1	9.49E+03			9.49E+03	5.5E-01	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-B01-A	1	1.11E+01			1.11E+01	2.6E+01	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-B02-A	1	1.20E+01			1.20E+01	7.5E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1313-B03-A	1	9.16E+00			9.16E+00	1.5E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	SWA-L02-1313-T01-A	1	1.66E+02			1.66E+02	4.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T02-A	1	3.16E+02			3.16E+02	8.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T03-A	1	2.10E+02			2.10E+02	7.3E+01	1.0E+00	3.2E+00	10	125	1.35E+03	91%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T04-A	1	9.95E+02			9.95E+02	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T05-A	1	9.08E+02			9.08E+02	6.1E-02	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T06-A	1	1.18E+03			1.18E+03	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T07-A	1	1.45E+03			1.45E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T08-A	1	9.92E+02			9.92E+02	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T09-A	1	1.10E+03			1.10E+03	1.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T01-B	1	1.80E+02			1.80E+02	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T02-B	1	2.83E+02			2.83E+02	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T03-B	1	1.79E+02			1.79E+02	7.4E-01	1.0E+00	3.2E+00	10	125	1.38E+03	96%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T04-B	1	9.67E+02			9.67E+02	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T05-B	1	9.52E+02			9.52E+02	4.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T06-B	1	1.18E+03			1.18E+03	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T07-B	1	1.51E+03			1.51E+03	5.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T08-B	1	9.05E+02			9.05E+02	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T09-B	1	1.01E+03			1.01E+03	8.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T01-C	1	1.81E+02			1.81E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T02-C	1	2.91E+02			2.91E+02	6.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T03-C	1	1.69E+02			1.69E+02	1.5E+00	1.0E+00	3.2E+00	10	125	1.34E+03	93%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T04-C	1	9.20E+02			9.20E+02	9.5E-01	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T05-C	1	9.60E+02			9.60E+02	5.6E-01	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T06-C	1	1.05E+03			1.05E+03	3.5E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T07-C	1	1.38E+03			1.38E+03	4.6E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T08-C	1	9.42E+02			9.42E+02	9.4E-01	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-T09-C	1	1.05E+03			1.05E+03	1.8E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	SWA-L02-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	3.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	3.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	5.8E+01	1.9E+00	6.0E+00	10	125	1.29E+03	103%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	7.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	9.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	1.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T07-A	1	4.48E-01	U1/2		4.48E-01	1.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T08-A	1	4.73E+01			4.73E+01	1.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T09-A	1	1.99E+02			1.99E+02	1.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	8.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	7.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	2.2E+01	1.9E+00	6.0E+00	10	125	1.32E+03	106%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	5.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	1.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T07-B	1	9.50E-01	U1/2		9.50E-01	4.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T08-B	1	7.19E+01			7.19E+01	2.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T09-B	1	1.73E+02			1.73E+02	1.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T01-C	1	3.72E+00	E		3.72E+00	1.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	2.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	4.5E+01	1.9E+00	6.0E+00	10	125	1.29E+03	103%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	2.6E+01	1.9E+00	6.0E+00					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	1.0E+02	1.9E+00	6.0E+00					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T07-C	1	9.50E-01	U1/2		9.50E-01	2.9E+01	1.9E+00	6.0E+00					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T08-C	1	7.72E+01			7.72E+01	1.4E+00	1.9E+00	6.0E+00					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-T09-C	1	1.91E+02			1.91E+02	7.9E-01	1.9E+00	6.0E+00					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	4.8E+01	1.9E+00	6.0E+00					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	2.9E+01	1.9E+00	6.0E+00					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	1.1E+01	1.9E+00	6.0E+00					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	SWA-L02-1313-T01-A	1	1.10E+00	U1/2		1.10E+00	9.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T02-A	1	1.10E+00	U1/2		1.10E+00	1.4E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	5.2E+01	2.2E+00	7.0E+00	10	125	1.22E+03	98%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T04-A	1	1.10E+00	U1/2		1.10E+00	1.3E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T05-A	1	1.10E+00	U1/2		1.10E+00	4.5E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T06-A	1	1.10E+00	U1/2		1.10E+00	2.3E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T07-A	1	8.20E+00			8.20E+00	4.3E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T08-A	1	2.38E+01			2.38E+01	2.9E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T09-A	1	4.61E+01			4.61E+01	3.1E-01	2.2E+00	7.0E+00				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T01-B	1	1.10E+00	U1/2		1.10E+00	5.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T02-B	1	1.10E+00	U1/2		1.10E+00	7.6E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	7.6E+01	2.2E+00	7.0E+00	10	125	1.24E+03	99%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T04-B	1	1.10E+00	U1/2		1.10E+00	2.3E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T05-B	1	1.10E+00	U1/2		1.10E+00	9.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T06-B	1	1.10E+00	U1/2		1.10E+00	1.1E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T07-B	1	6.74E+00	E		6.74E+00	2.7E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T08-B	1	2.35E+01			2.35E+01	1.2E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T09-B	1	4.14E+01			4.14E+01	1.8E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T01-C	1	3.64E+00	E		3.64E+00	5.1E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T02-C	1	1.10E+00	U1/2		1.10E+00	1.3E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	1.5E+02	2.2E+00	7.0E+00	10	125	1.22E+03	97%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T04-C	1	1.10E+00	U1/2		1.10E+00	1.9E+01	2.2E+00	7.0E+00					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T05-C	1	1.10E+00	U1/2		1.10E+00	2.7E+01	2.2E+00	7.0E+00					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T06-C	1	1.10E+00	U1/2		1.10E+00	3.6E+01	2.2E+00	7.0E+00					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T07-C	1	6.72E+00	E		6.72E+00	3.6E+00	2.2E+00	7.0E+00					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T08-C	1	2.45E+01			2.45E+01	9.4E-01	2.2E+00	7.0E+00					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-T09-C	1	4.41E+01			4.41E+01	5.9E-01	2.2E+00	7.0E+00					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	1.7E+02	2.2E+00	7.0E+00					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	1.8E+01	2.2E+00	7.0E+00					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1313-B03-A	1	1.10E+00	U1/2		1.10E+00	1.5E+02	2.2E+00	7.0E+00					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	SWA-L02-1313-T01-A	1	1.39E+04			1.39E+04	6.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T02-A	1	6.03E+04			6.03E+04	5.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T03-A	1	2.54E+04			2.54E+04	6.9E-01	2.6E+00	8.3E+00	1000	125	2.65E+04	92%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T04-A	1	5.11E+06			5.11E+06	2.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T05-A	1	7.16E+06			7.16E+06	5.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T06-A	1	9.49E+06			9.49E+06	7.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T07-A	1	1.06E+07			1.06E+07	4.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T08-A	1	8.25E+06			8.25E+06	4.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T09-A	1	5.58E+06			5.58E+06	5.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T01-B	1	1.68E+04			1.68E+04	1.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T02-B	1	5.63E+04			5.63E+04	3.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T03-B	1	2.41E+04			2.41E+04	2.1E+00	2.6E+00	8.3E+00	1000	125	2.53E+04	99%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T04-B	1	5.36E+06			5.36E+06	7.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T05-B	1	7.67E+06			7.67E+06	6.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T06-B	1	9.57E+06			9.57E+06	6.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T07-B	1	1.10E+07			1.10E+07	6.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T08-B	1	7.12E+06			7.12E+06	1.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T09-B	1	5.68E+06			5.68E+06	5.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T01-C	1	1.77E+04			1.77E+04	6.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T02-C	1	6.00E+04			6.00E+04	3.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T03-C	1	2.33E+04			2.33E+04	3.3E+00	2.6E+00	8.3E+00	1000	125	2.45E+04	97%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T04-C	1	5.45E+06			5.45E+06	4.4E+00	2.6E+00	8.3E+00					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T05-C	1	7.78E+06			7.78E+06	1.1E-01	2.6E+00	8.3E+00					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T06-C	1	8.65E+06			8.65E+06	2.0E+00	2.6E+00	8.3E+00					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T07-C	1	1.01E+07			1.01E+07	1.3E+00	2.6E+00	8.3E+00					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T08-C	1	7.31E+06			7.31E+06	1.4E-01	2.6E+00	8.3E+00					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-T09-C	1	5.56E+06			5.56E+06	7.1E-01	2.6E+00	8.3E+00					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-B01-A	1	1.30E+00	U1/2		1.30E+00	8.3E+00	2.6E+00	8.3E+00					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-B02-A	1	1.30E+00	U1/2		1.30E+00	5.7E-01	2.6E+00	8.3E+00					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1313-B03-A	1	1.30E+00	U1/2		1.30E+00	5.1E+00	2.6E+00	8.3E+00					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	SWA-L02-1313-T01-A	1	1.09E+03			1.09E+03	4.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T02-A	1	1.84E+02			1.84E+02	7.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T03-A	1	1.12E+03			1.12E+03	1.9E+00	1.2E+00	3.8E+00	10	125	2.36E+03	99%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T04-A	1	9.35E+01			9.35E+01	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T05-A	1	6.24E+00			6.24E+00	1.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T06-A	1	6.00E-01	U1/2		6.00E-01	1.2E+03	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T07-A	1	4.06E+00			4.06E+00	4.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T08-A	1	4.77E+03			4.77E+03	4.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T09-A	1	2.69E+04			2.69E+04	3.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T01-B	1	1.19E+03			1.19E+03	1.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T02-B	1	2.11E+02			2.11E+02	2.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T03-B	1	9.28E+02			9.28E+02	2.6E+00	1.2E+00	3.8E+00	10	125	2.21E+03	103%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T04-B	1	7.63E+01			7.63E+01	9.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T05-B	1	7.32E+00			7.32E+00	2.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T06-B	1	1.39E+00	E		1.39E+00	1.3E+02	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T07-B	1	4.29E+00			4.29E+00	1.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T08-B	1	6.94E+03			6.94E+03	6.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T09-B	1	2.45E+04			2.45E+04	1.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T01-C	1	1.13E+03			1.13E+03	1.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T02-C	1	1.86E+02			1.86E+02	7.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T03-C	1	9.16E+02			9.16E+02	3.6E+00	1.2E+00	3.8E+00	10	125	2.15E+03	99%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T04-C	1	6.35E+00			6.35E+00	4.9E+00	1.2E+00	3.8E+00					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T05-C	1	3.80E+00	E		3.80E+00	2.8E+01	1.2E+00	3.8E+00					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T06-C	1	3.77E+00	E		3.77E+00	2.2E+01	1.2E+00	3.8E+00					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T07-C	1	4.64E+00			4.64E+00	1.4E+01	1.2E+00	3.8E+00					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T08-C	1	7.38E+03			7.38E+03	2.6E-01	1.2E+00	3.8E+00					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-T09-C	1	2.58E+04			2.58E+04	5.3E-01	1.2E+00	3.8E+00					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	3.1E+02	1.2E+00	3.8E+00					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	1.9E+02	1.2E+00	3.8E+00					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1313-B03-A	1	6.00E-01	U1/2		6.00E-01	9.4E+01	1.2E+00	3.8E+00					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	SWA-L02-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	1.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	2.6E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	3.3E+02	1.8E+00	5.7E+00	10	125	1.23E+03	98%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T04-A	1	2.62E+00	E		2.62E+00	6.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T05-A	1	1.26E+01			1.26E+01	2.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T06-A	1	8.60E+01			8.60E+01	3.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T07-A	1	2.01E+02			2.01E+02	5.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T08-A	1	2.40E+02			2.40E+02	1.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T09-A	1	3.49E+02			3.49E+02	1.3E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	1.7E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	5.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	4.1E+02	1.8E+00	5.7E+00	10	125	1.25E+03	100%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T04-B	1	1.91E+00	E		1.91E+00	8.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T05-B	1	1.69E+01			1.69E+01	5.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T06-B	1	7.27E+01			7.27E+01	2.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T07-B	1	2.03E+02			2.03E+02	5.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T08-B	1	2.35E+02			2.35E+02	1.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T09-B	1	3.27E+02			3.27E+02	8.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T01-C	1	2.89E+00	E		2.89E+00	6.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	2.2E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	3.6E+02	1.8E+00	5.7E+00	10	125	1.22E+03	97%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	5.0E+01	1.8E+00	5.7E+00					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T05-C	1	1.99E+01			1.99E+01	1.5E+00	1.8E+00	5.7E+00					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T06-C	1	5.35E+01			5.35E+01	8.3E+00	1.8E+00	5.7E+00					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T07-C	1	1.75E+02			1.75E+02	1.6E+00	1.8E+00	5.7E+00					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T08-C	1	2.46E+02			2.46E+02	4.9E-01	1.8E+00	5.7E+00					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-T09-C	1	3.40E+02			3.40E+02	7.8E-01	1.8E+00	5.7E+00					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	2.1E+01	1.8E+00	5.7E+00					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	2.2E+01	1.8E+00	5.7E+00					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	1.9E+01	1.8E+00	5.7E+00					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	SWA-L02-1313-T01-A	1	1.85E+00	U1/2		1.85E+00	1.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T02-A	1	6.55E+00	E		6.55E+00	3.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T03-A	1	5.45E+00	E		5.45E+00	3.4E+01	3.7E+00	1.2E+01	10	125	1.27E+03	101%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T04-A	1	2.24E+01			2.24E+01	2.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T05-A	1	2.92E+01			2.92E+01	8.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T06-A	1	5.26E+01			5.26E+01	1.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T07-A	1	6.74E+01			6.74E+01	1.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T08-A	1	1.32E+02			1.32E+02	2.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T09-A	1	2.02E+03			2.02E+03	1.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T01-B	1	1.85E+00	U1/2		1.85E+00	1.3E+02	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T02-B	1	4.88E+00	E		4.88E+00	6.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T03-B	1	4.00E+00	E		4.00E+00	6.3E+01	3.7E+00	1.2E+01	10	125	1.30E+03	104%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T04-B	1	1.94E+01			1.94E+01	3.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T05-B	1	3.04E+01			3.04E+01	3.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T06-B	1	4.56E+01			4.56E+01	1.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T07-B	1	6.63E+01			6.63E+01	2.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T08-B	1	1.45E+02			1.45E+02	6.3E-01	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T09-B	1	1.77E+03			1.77E+03	1.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T01-C	1	4.45E+00	E		4.45E+00	2.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T02-C	1	6.89E+00	E		6.89E+00	9.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T03-C	1	4.92E+00	E		4.92E+00	3.7E+01	3.7E+00	1.2E+01	10	125	1.26E+03	100%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T04-C	1	2.08E+01			2.08E+01	6.6E+00	3.7E+00	1.2E+01					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T05-C	1	3.52E+01			3.52E+01	2.0E+01	3.7E+00	1.2E+01					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T06-C	1	3.71E+01			3.71E+01	9.8E+00	3.7E+00	1.2E+01					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T07-C	1	6.05E+01			6.05E+01	1.1E+01	3.7E+00	1.2E+01					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T08-C	1	1.54E+02			1.54E+02	8.2E-01	3.7E+00	1.2E+01					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-T09-C	1	1.93E+03			1.93E+03	1.9E-01	3.7E+00	1.2E+01					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	1.6E+02	3.7E+00	1.2E+01					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	3.7E+02	3.7E+00	1.2E+01					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1313-B03-A	1	1.85E+00	U1/2		1.85E+00	1.3E+02	3.7E+00	1.2E+01					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	SWA-L02-1313-T01-A	1	6.39E+01			6.39E+01	9.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T02-A	1	4.92E+01			4.92E+01	1.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T03-A	1	2.49E+02			2.49E+02	1.2E+00	2.0E+00	6.4E+00	1000	125	1.56E+03	105%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T04-A	1	2.41E+02			2.41E+02	1.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T05-A	1	2.26E+01			2.26E+01	2.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T06-A	1	1.72E+02			1.72E+02	5.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T07-A	1	7.34E+04			7.34E+04	1.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T08-A	1	1.69E+05			1.69E+05	1.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T09-A	1	2.22E+05			2.22E+05	9.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T01-B	1	1.09E+02			1.09E+02	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T02-B	1	1.06E+02			1.06E+02	3.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T03-B	1	2.39E+02			2.39E+02	2.9E+00	2.0E+00	6.4E+00	1000	125	1.64E+03	112%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T04-B	1	1.34E+02			1.34E+02	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T05-B	1	4.54E+01			4.54E+01	2.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T06-B	1	1.44E+02			1.44E+02	1.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T07-B	1	6.62E+04			6.62E+04	8.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T08-B	1	1.71E+05			1.71E+05	5.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T09-B	1	2.13E+05			2.13E+05	2.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T01-C	1	1.35E+02			1.35E+02	8.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T02-C	1	1.31E+02			1.31E+02	6.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T03-C	1	2.63E+02			2.63E+02	3.6E+00	2.0E+00	6.4E+00	1000	125	1.70E+03	115%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T04-C	1	6.71E+01			6.71E+01	1.8E+00	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T05-C	1	5.99E+01			5.99E+01	2.5E+00	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T06-C	1	9.10E+01			9.10E+01	8.8E-01	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T07-C	1	5.30E+04			5.30E+04	1.2E+00	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T08-C	1	1.77E+05			1.77E+05	1.2E+00	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-T09-C	1	2.18E+05			2.18E+05	1.9E+00	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	8.3E+00	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	3.2E+00	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	2.0E+00	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	SWA-L02-1313-T01-A	1	1.59E+01	E		1.59E+01	1.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T02-A	1	3.40E+00	U1/2		3.40E+00	2.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T03-A	1	2.92E+01			2.92E+01	2.7E+01	6.8E+00	2.2E+01	10	125	1.32E+03	103%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T04-A	1	1.45E+01	E		1.45E+01	4.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T05-A	1	1.42E+01	E		1.42E+01	5.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T06-A	1	1.71E+01	E		1.71E+01	7.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T07-A	1	2.66E+01			2.66E+01	3.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T08-A	1	4.62E+02			4.62E+02	7.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T09-A	1	4.94E+03			4.94E+03	3.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T01-B	1	1.85E+01	E		1.85E+01	1.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T02-B	1	9.52E+00	E		9.52E+00	7.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T03-B	1	1.24E+01	E		1.24E+01	5.0E+01	6.8E+00	2.2E+01	10	125	1.35E+03	107%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T04-B	1	3.40E+00	U1/2		3.40E+00	3.9E+02	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T05-B	1	1.23E+01	E		1.23E+01	3.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T06-B	1	1.57E+01	E		1.57E+01	9.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T07-B	1	1.84E+01	E		1.84E+01	7.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T08-B	1	5.22E+02			5.22E+02	1.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T09-B	1	4.47E+03			4.47E+03	1.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T01-C	1	2.31E+01			2.31E+01	2.7E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T02-C	1	3.40E+00	U1/2		3.40E+00	3.3E+02	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T03-C	1	1.78E+01	E		1.78E+01	1.5E+01	6.8E+00	2.2E+01	10	125	1.30E+03	103%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T04-C	1	1.09E+01	E		1.09E+01	1.5E+01	6.8E+00	2.2E+01					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T05-C	1	1.60E+01	E		1.60E+01	1.0E+02	6.8E+00	2.2E+01					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T06-C	1	1.44E+01	E		1.44E+01	6.2E+01	6.8E+00	2.2E+01					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T07-C	1	1.74E+01	E		1.74E+01	2.5E+01	6.8E+00	2.2E+01					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T08-C	1	5.49E+02			5.49E+02	1.8E+00	6.8E+00	2.2E+01					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-T09-C	1	4.70E+03			4.70E+03	3.4E-01	6.8E+00	2.2E+01					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	2.6E+01	6.8E+00	2.2E+01					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	6.0E+01	6.8E+00	2.2E+01					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	7.4E+01	6.8E+00	2.2E+01					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	SWA-L02-1313-T01-A	1	2.49E+00	E		2.49E+00	1.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T02-A	1	9.24E+00			9.24E+00	2.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T03-A	1	2.38E+00	E		2.38E+00	6.2E+01	1.9E+00	6.0E+00	10	125	1.17E+03	93%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T04-A	1	4.76E+02			4.76E+02	5.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T05-A	1	8.27E+02			8.27E+02	1.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T06-A	1	1.27E+03			1.27E+03	4.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T07-A	1	1.50E+03			1.50E+03	4.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T08-A	1	1.24E+03			1.24E+03	3.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T09-A	1	1.28E+03			1.28E+03	5.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T02-B	1	4.71E+00	E		4.71E+00	7.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	5.1E+01	1.9E+00	6.0E+00	10	125	1.18E+03	94%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T04-B	1	5.14E+02			5.14E+02	2.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T05-B	1	9.45E+02			9.45E+02	2.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T06-B	1	1.30E+03			1.30E+03	2.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T07-B	1	1.61E+03			1.61E+03	2.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T08-B	1	1.11E+03			1.11E+03	4.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T09-B	1	1.15E+03			1.15E+03	4.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	2.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T02-C	1	6.99E+00			6.99E+00	2.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	9.9E+01	1.9E+00	6.0E+00	10	125	1.08E+03	86%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T04-C	1	5.20E+02			5.20E+02	1.3E+01	1.9E+00	6.0E+00					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T05-C	1	9.85E+02			9.85E+02	1.4E+00	1.9E+00	6.0E+00					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T06-C	1	1.20E+03			1.20E+03	2.7E+00	1.9E+00	6.0E+00					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T07-C	1	1.42E+03			1.42E+03	4.4E+00	1.9E+00	6.0E+00					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T08-C	1	1.14E+03			1.14E+03	6.3E+00	1.9E+00	6.0E+00					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-T09-C	1	1.22E+03			1.22E+03	2.3E+00	1.9E+00	6.0E+00					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-B01-A	1	3.22E+00	E		3.22E+00	4.5E+01	1.9E+00	6.0E+00					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	1.5E+02	1.9E+00	6.0E+00					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	5.9E+01	1.9E+00	6.0E+00					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	SWA-L02-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	6.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	2.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T03-A	1	2.52E+01			2.52E+01	5.5E-01	2.0E+00	6.4E+00	10	125	1.31E+03	103%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T04-A	1	4.68E+01			4.68E+01	1.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T05-A	1	3.61E+03			3.61E+03	2.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T06-A	1	1.42E+04			1.42E+04	5.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T07-A	1	2.55E+04			2.55E+04	2.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T08-A	1	2.46E+04			2.46E+04	4.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T09-A	1	2.87E+04			2.87E+04	5.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T01-B	1	4.45E+00	E		4.45E+00	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T02-B	1	6.47E+00			6.47E+00	2.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T03-B	1	2.60E+01			2.60E+01	2.4E+00	2.0E+00	6.4E+00	10	125	1.26E+03	98%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T04-B	1	4.41E+01			4.41E+01	7.4E-02	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T05-B	1	4.42E+03			4.42E+03	9.0E-02	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T06-B	1	1.33E+04			1.33E+04	7.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T07-B	1	2.58E+04			2.58E+04	8.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T08-B	1	2.34E+04			2.34E+04	1.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T09-B	1	2.66E+04			2.66E+04	8.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T01-C	1	1.15E+01			1.15E+01	6.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T02-C	1	9.80E+00			9.80E+00	1.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T03-C	1	2.91E+01			2.91E+01	3.2E+00	2.0E+00	6.4E+00	10	125	1.35E+03	105%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T04-C	1	4.49E+01			4.49E+01	2.2E+00	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T05-C	1	5.19E+03			5.19E+03	9.2E-01	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T06-C	1	1.07E+04			1.07E+04	1.8E+00	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T07-C	1	2.28E+04			2.28E+04	1.4E+00	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T08-C	1	2.42E+04			2.42E+04	1.0E+00	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-T09-C	1	2.78E+04			2.78E+04	1.2E+00	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	5.8E+00	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	2.1E+00	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	SWA-L02-1313-T01-A	1	5.00E-01	U1/2		5.00E-01	6.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T02-A	1	5.00E-01	U1/2		5.00E-01	1.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T03-A	1	6.51E+02			6.51E+02	1.3E+00	1.0E+00	3.2E+00	1000	125	1.86E+03	97%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T04-A	1	4.18E+05			4.18E+05	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T05-A	1	9.00E+05			9.00E+05	5.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T06-A	1	1.39E+06			1.39E+06	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T07-A	1	1.67E+06			1.67E+06	4.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T08-A	1	1.37E+06			1.37E+06	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T09-A	1	1.22E+06			1.22E+06	3.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T01-B	1	2.07E+02			2.07E+02	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T02-B	1	3.03E+02			3.03E+02	2.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T03-B	1	7.96E+02			7.96E+02	1.2E+00	1.0E+00	3.2E+00	1000	125	1.93E+03	91%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T04-B	1	4.48E+05			4.48E+05	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T05-B	1	9.69E+05			9.69E+05	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T06-B	1	1.38E+06			1.38E+06	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T07-B	1	1.74E+06			1.74E+06	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T08-B	1	1.19E+06			1.19E+06	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T09-B	1	1.15E+06			1.15E+06	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T01-C	1	4.19E+02			4.19E+02	3.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T02-C	1	4.67E+02			4.67E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T03-C	1	9.54E+02			9.54E+02	4.2E+00	1.0E+00	3.2E+00	1000	125	2.14E+03	95%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T04-C	1	4.72E+05			4.72E+05	5.6E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T05-C	1	9.84E+05			9.84E+05	1.0E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T06-C	1	1.24E+06			1.24E+06	2.0E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T07-C	1	1.55E+06			1.55E+06	8.7E-01	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T08-C	1	1.23E+06			1.23E+06	1.9E-01	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-T09-C	1	1.18E+06			1.18E+06	1.0E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	8.1E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.0E+01	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	1.5E+01	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	SWA-L02-1313-T01-A	1	1.60E+02			1.60E+02	1.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T02-A	1	1.97E+02			1.97E+02	9.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T03-A	1	1.77E+02			1.77E+02	2.5E+00	1.2E+00	3.8E+00	10	125	1.48E+03	104%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T04-A	1	1.75E+02			1.75E+02	2.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T05-A	1	1.61E+02			1.61E+02	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T06-A	1	7.06E+01			7.06E+01	3.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T07-A	1	1.98E+01			1.98E+01	2.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T08-A	1	1.95E+01			1.95E+01	2.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T09-A	1	1.07E+01			1.07E+01	5.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T01-B	1	1.75E+02			1.75E+02	2.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T02-B	1	1.88E+02			1.88E+02	5.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T03-B	1	1.51E+02			1.51E+02	3.3E+00	1.2E+00	3.8E+00	10	125	1.52E+03	109%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T04-B	1	1.81E+02			1.81E+02	1.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T05-B	1	1.66E+02			1.66E+02	1.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T06-B	1	8.21E+01			8.21E+01	2.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T07-B	1	1.78E+01			1.78E+01	1.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T08-B	1	1.28E+01			1.28E+01	8.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T09-B	1	6.19E+00			6.19E+00	8.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T01-C	1	1.80E+02			1.80E+02	6.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T02-C	1	2.15E+02			2.15E+02	2.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T03-C	1	1.44E+02			1.44E+02	5.9E+00	1.2E+00	3.8E+00	10	125	1.46E+03	106%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T04-C	1	1.76E+02			1.76E+02	5.5E+00	1.2E+00	3.8E+00					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T05-C	1	1.61E+02			1.61E+02	9.4E-01	1.2E+00	3.8E+00					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T06-C	1	9.31E+01			9.31E+01	5.1E+00	1.2E+00	3.8E+00					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T07-C	1	2.28E+01			2.28E+01	7.5E+00	1.2E+00	3.8E+00					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T08-C	1	1.36E+01			1.36E+01	2.8E+01	1.2E+00	3.8E+00					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-T09-C	1	4.96E+00			4.96E+00	1.6E+02	1.2E+00	3.8E+00					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	5.5E+02	1.2E+00	3.8E+00					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	1.6E+02	1.2E+00	3.8E+00					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1313-B03-A	1	6.00E-01	U1/2		6.00E-01	1.8E+02	1.2E+00	3.8E+00					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	SWA-L02-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	2.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	3.2E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T03-A	1	9.93E+00			9.93E+00	2.5E+01	1.8E+00	5.7E+00	10	125	1.21E+03	96%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T04-A	1	2.21E+01			2.21E+01	8.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T05-A	1	3.62E+01			3.62E+01	5.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T06-A	1	2.43E+02			2.43E+02	1.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T07-A	1	4.76E+02			4.76E+02	7.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T08-A	1	5.04E+02			5.04E+02	1.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T09-A	1	6.26E+02			6.26E+02	2.4E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T01-B	1	2.61E+00	E		2.61E+00	8.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	4.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T03-B	1	7.30E+00			7.30E+00	4.0E+01	1.8E+00	5.7E+00	10	125	1.23E+03	98%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T04-B	1	1.38E+01			1.38E+01	1.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T05-B	1	4.87E+01			4.87E+01	9.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T06-B	1	2.19E+02			2.19E+02	6.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T07-B	1	4.78E+02			4.78E+02	5.4E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T08-B	1	4.68E+02			4.68E+02	4.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T09-B	1	5.82E+02			5.82E+02	7.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T01-C		4.89E+00	U1/2		0.00E+00	4.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T02-C		9.00E-01	U1/2		0.00E+00	2.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T03-C		9.15E+00	U1/2		0.00E+00	1.6E+01	1.8E+00	5.7E+00	10	125	1.20E+03	95%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T04-C		7.82E+00	U1/2		0.00E+00	2.0E+01	1.8E+00	5.7E+00					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T05-C		6.17E+01	U1/2		0.00E+00	3.7E+00	1.8E+00	5.7E+00					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T06-C		1.58E+02	U1/2		0.00E+00	5.6E+00	1.8E+00	5.7E+00					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T07-C		4.14E+02	U1/2		0.00E+00	3.8E-01	1.8E+00	5.7E+00					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T08-C		4.88E+02	U1/2		0.00E+00	1.5E+00	1.8E+00	5.7E+00					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-T09-C		6.05E+02	U1/2		0.00E+00	8.6E-01	1.8E+00	5.7E+00					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-B01-A		9.00E-01	U1/2		0.00E+00	1.1E+02	1.8E+00	5.7E+00					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-B02-A		9.00E-01	U1/2		0.00E+00	1.0E+02	1.8E+00	5.7E+00					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1313-B03-A		9.00E-01	U1/2		0.00E+00	3.7E+02	1.8E+00	5.7E+00					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	SWA-L02-1313-T01-A	1	1.20E+02			1.20E+02	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T02-A	1	4.08E+01			4.08E+01	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T03-A	1	7.45E+01			7.45E+01	2.8E+01	3.7E+00	1.2E+01	1000	125	1.28E+03	96%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T04-A	1	1.12E+02			1.12E+02	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T05-A	1	6.71E+01			6.71E+01	4.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T06-A	1	1.85E+00	U1/2		1.85E+00	1.4E+03	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T07-A	1	9.94E+00	E		9.94E+00	2.6E+02	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T08-A	1	2.97E+03			2.97E+03	2.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T09-A	1	2.32E+03			2.32E+03	8.2E-01	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T01-B	1	1.18E+02			1.18E+02	8.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T02-B	1	2.78E+01			2.78E+01	3.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T03-B	1	6.07E+01			6.07E+01	3.6E+01	3.7E+00	1.2E+01	1000	125	1.32E+03	101%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T04-B	1	5.96E+01			5.96E+01	4.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T05-B	1	7.61E+01			7.61E+01	2.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T06-B	1	3.60E+01			3.60E+01	1.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T07-B	1	2.92E+01			2.92E+01	4.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T08-B	1	1.54E+03			1.54E+03	2.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T09-B	1	2.06E+03			2.06E+03	2.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T01-C	1	1.50E+02			1.50E+02	1.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T02-C	1	8.65E+00	E		8.65E+00	1.6E+02	3.7E+00	1.2E+01				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T03-C	1	5.74E+01			5.74E+01	1.9E+01	3.7E+00	1.2E+01	1000	125	1.27E+03	97%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T04-C	1	5.19E+01			5.19E+01	3.1E+01	3.7E+00	1.2E+01					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T05-C	1	1.06E+02			1.06E+02	1.8E+01	3.7E+00	1.2E+01					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T06-C	1	7.95E+01			7.95E+01	2.9E+01	3.7E+00	1.2E+01					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T07-C	1	4.88E+01			4.88E+01	8.8E+01	3.7E+00	1.2E+01					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T08-C	1	1.59E+03			1.59E+03	2.2E-01	3.7E+00	1.2E+01					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-T09-C	1	2.20E+03			2.20E+03	5.5E-01	3.7E+00	1.2E+01					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	1.9E+04	3.7E+00	1.2E+01					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	5.5E+01	3.7E+00	1.2E+01					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1313-B03-A	1	1.85E+00	U1/2		1.85E+00	8.1E+02	3.7E+00	1.2E+01					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	SWA-L02-1313-T01-A	1	3.59E+05			3.59E+05	3.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T02-A	1	4.10E+05			4.10E+05	2.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T03-A	1	3.80E+05			3.80E+05	2.0E+00	1.6E+00	5.1E+00	1000	125	3.82E+05	91%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T04-A	1	5.08E+05			5.08E+05	1.6E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T05-A	1	5.06E+05			5.06E+05	3.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T06-A	1	5.67E+05			5.67E+05	6.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T07-A	1	5.55E+05			5.55E+05	3.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T08-A	1	4.89E+05			4.89E+05	1.8E+01	1.6E+00	5.1E+00				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T09-A	1	5.29E+05			5.29E+05	2.3E+01	1.6E+00	5.1E+00				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T01-B	1	5.10E+05			5.10E+05	2.6E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T02-B	1	3.98E+05			3.98E+05	5.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T03-B	1	3.32E+05			3.32E+05	1.5E+00	1.6E+00	5.1E+00	1000	125	3.33E+05	101%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T04-B	1	5.27E+05			5.27E+05	1.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T05-B	1	5.32E+05			5.32E+05	3.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T06-B	1	5.74E+05			5.74E+05	5.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T07-B	1	5.76E+05			5.76E+05	1.9E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T08-B	1	3.65E+05			3.65E+05	8.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T09-B	1	3.69E+05			3.69E+05	8.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T01-C	1	3.78E+05			3.78E+05	9.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T02-C	1	4.22E+05			4.22E+05	6.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T03-C	1	3.20E+05			3.20E+05	2.4E+00	1.6E+00	5.1E+00	1000	125	3.21E+05	105%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T04-C	1	5.12E+05			5.12E+05	2.0E+00	1.6E+00	5.1E+00					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T05-C	1	5.35E+05			5.35E+05	2.4E+00	1.6E+00	5.1E+00					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T06-C	1	5.18E+05			5.18E+05	1.4E+00	1.6E+00	5.1E+00					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T07-C	1	5.29E+05			5.29E+05	9.5E-01	1.6E+00	5.1E+00					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T08-C	1	4.50E+05			4.50E+05	1.8E+01	1.6E+00	5.1E+00					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-T09-C	1	4.19E+05			4.19E+05	1.2E+01	1.6E+00	5.1E+00					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-B01-A	1	1.03E+01			1.03E+01	2.7E+01	1.6E+00	5.1E+00					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-B02-A	1	8.00E-01	U1/2		8.00E-01	8.4E+01	1.6E+00	5.1E+00					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1313-B03-A	1	8.00E-01	U1/2		8.00E-01	1.8E+02	1.6E+00	5.1E+00					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	SWA-L02-1313-T01-A	1	1.05E+05			1.05E+05	8.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T02-A	1	1.22E+05			1.22E+05	9.5E-02	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T03-A	1	1.13E+05			1.13E+05	1.1E+00	1.5E+01	4.8E+01	10	125	1.14E+05	83%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T04-A	1	1.27E+05			1.27E+05	1.6E+00	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T05-A	1	1.33E+05			1.33E+05	7.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T06-A	1	1.52E+05			1.52E+05	2.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T07-A	1	1.44E+05			1.44E+05	4.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T08-A	1	9.96E+04			9.96E+04	1.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T09-A	1	6.34E+04			6.34E+04	3.5E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T01-B	1	1.16E+05			1.16E+05	8.8E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T02-B	1	1.15E+05			1.15E+05	2.8E+00	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T03-B	1	9.60E+04			9.60E+04	2.1E+00	1.5E+01	4.8E+01	10	125	9.70E+04	85%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T04-B	1	1.31E+05			1.31E+05	3.9E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T05-B	1	1.40E+05			1.40E+05	4.2E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T06-B	1	1.54E+05			1.54E+05	7.8E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T07-B	1	1.50E+05			1.50E+05	1.0E+00	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T08-B	1	8.22E+04			8.22E+04	9.2E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T09-B	1	5.88E+04			5.88E+04	1.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T01-C	1	1.12E+05			1.12E+05	1.2E+00	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T02-C	1	1.31E+05			1.31E+05	5.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T03-C	1	9.27E+04			9.27E+04	3.2E+00	1.5E+01	4.8E+01	10	125	9.38E+04	88%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T04-C	1	1.26E+05			1.26E+05	3.2E+00	1.5E+01	4.8E+01					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T05-C	1	1.41E+05			1.41E+05	9.5E-01	1.5E+01	4.8E+01					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T06-C	1	1.40E+05			1.40E+05	1.6E+00	1.5E+01	4.8E+01					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T07-C	1	1.38E+05			1.38E+05	1.3E+00	1.5E+01	4.8E+01					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T08-C	1	8.61E+04			8.61E+04	7.4E-01	1.5E+01	4.8E+01					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-T09-C	1	6.13E+04			6.13E+04	7.9E-01	1.5E+01	4.8E+01					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-B01-A	1	7.50E+00	U1/2		7.50E+00	7.0E+01	1.5E+01	4.8E+01					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-B02-A	1	7.50E+00	U1/2		7.50E+00	9.7E+01	1.5E+01	4.8E+01					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1313-B03-A	1	7.50E+00	U1/2		7.50E+00	3.7E+03	1.5E+01	4.8E+01					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	SWA-L02-1313-T01-A	1	4.93E+03			4.93E+03	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T02-A	1	3.61E+03			3.61E+03	6.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T03-A	1	5.56E+03			5.56E+03	1.9E+00	1.1E+00	3.5E+00	1000	125	6.68E+03	90%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T04-A	1	1.30E+03			1.30E+03	1.4E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T05-A	1	1.09E+03			1.09E+03	4.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T06-A	1	2.41E+03			2.41E+03	3.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T07-A	1	3.35E+03			3.35E+03	6.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T08-A	1	2.46E+04			2.46E+04	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T09-A	1	7.00E+03			7.00E+03	1.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T01-B	1	5.36E+03			5.36E+03	1.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T02-B	1	3.31E+03			3.31E+03	1.1E+01	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T03-B	1	4.64E+03			4.64E+03	2.7E+00	1.1E+00	3.5E+00	1000	125	6.02E+03	110%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T04-B	1	1.18E+03			1.18E+03	3.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T05-B	1	1.22E+03			1.22E+03	3.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T06-B	1	2.27E+03			2.27E+03	6.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T07-B	1	3.35E+03			3.35E+03	4.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T08-B	1	1.49E+04			1.49E+04	8.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T09-B	1	6.60E+03			6.60E+03	1.4E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T01-C	1	5.07E+03			5.07E+03	1.7E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T02-C	1	3.63E+03			3.63E+03	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T03-C	1	4.51E+03			4.51E+03	3.4E+00	1.1E+00	3.5E+00	1000	125	5.70E+03	96%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T04-C	1	7.74E+02			7.74E+02	1.1E+00	1.1E+00	3.5E+00					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T05-C	1	1.30E+03			1.30E+03	6.5E-01	1.1E+00	3.5E+00					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T06-C	1	1.85E+03			1.85E+03	1.8E+00	1.1E+00	3.5E+00					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T07-C	1	2.92E+03			2.92E+03	1.4E+00	1.1E+00	3.5E+00					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T08-C	1	1.59E+04			1.59E+04	4.6E-01	1.1E+00	3.5E+00					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-T09-C	1	6.73E+03			6.73E+03	5.2E-01	1.1E+00	3.5E+00					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-B01-A	1	5.50E-01	U1/2		5.50E-01	5.6E+01	1.1E+00	3.5E+00					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-B02-A	1	5.50E-01	U1/2		5.50E-01	1.1E+02	1.1E+00	3.5E+00					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1313-B03-A	1	5.50E-01	U1/2		5.50E-01	7.1E+01	1.1E+00	3.5E+00					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	SWA-L02-1313-T01-A	1	5.56E+05			5.56E+05	7.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T02-A	1	6.23E+05			6.23E+05	5.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T03-A	1	5.94E+05			5.94E+05	6.7E-01	2.5E+00	8.0E+00	1000	125	5.95E+05	88%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T04-A	1	7.18E+05			7.18E+05	1.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T05-A	1	7.05E+05			7.05E+05	2.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T06-A	1	7.61E+05			7.61E+05	3.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T07-A	1	7.13E+05			7.13E+05	7.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T08-A	1	4.62E+05			4.62E+05	7.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T09-A	1	2.86E+05			2.86E+05	5.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T01-B	1	5.90E+05			5.90E+05	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T02-B	1	6.00E+05			6.00E+05	1.8E+00	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T03-B	1	5.30E+05			5.30E+05	1.0E+00	2.5E+00	8.0E+00	1000	125	5.31E+05	83%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T04-B	1	7.22E+05			7.22E+05	6.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T05-B	1	7.25E+05			7.25E+05	1.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T06-B	1	7.62E+05			7.62E+05	6.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T07-B	1	7.40E+05			7.40E+05	9.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T08-B	1	4.08E+05			4.08E+05	1.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T09-B	1	2.86E+05			2.86E+05	1.0E+00	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T01-C	1	5.70E+05			5.70E+05	5.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T02-C	1	6.32E+05			6.32E+05	4.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T03-C	1	5.12E+05			5.12E+05	2.0E+00	2.5E+00	8.0E+00	1000	125	5.13E+05	85%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T04-C	1	7.04E+05			7.04E+05	2.0E+00	2.5E+00	8.0E+00					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T05-C	1	7.21E+05			7.21E+05	5.1E-01	2.5E+00	8.0E+00					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T06-C	1	7.04E+05			7.04E+05	1.9E+00	2.5E+00	8.0E+00					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T07-C	1	6.92E+05			6.92E+05	1.1E+00	2.5E+00	8.0E+00					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T08-C	1	4.10E+05			4.10E+05	7.8E-01	2.5E+00	8.0E+00					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-T09-C	1	2.84E+05			2.84E+05	1.5E-01	2.5E+00	8.0E+00					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-B01-A	1	1.25E+00	U1/2		1.25E+00	5.1E+00	2.5E+00	8.0E+00					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-B02-A	1	1.25E+00	U1/2		1.25E+00	3.8E+00	2.5E+00	8.0E+00					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1313-B03-A	1	1.25E+00	U1/2		1.25E+00	5.3E-01	2.5E+00	8.0E+00					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	SWA-L02-1313-T01-A	1	3.68E+02			3.68E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T02-A	1	1.38E+03			1.38E+03	6.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T03-A	1	6.25E+02			6.25E+02	1.3E+00	1.0E+00	3.2E+00	1000	125	1.88E+03	101%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T04-A	1	3.03E+04			3.03E+04	6.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T05-A	1	4.00E+04			4.00E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T06-A	1	5.39E+04			5.39E+04	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T07-A	1	6.23E+04			6.23E+04	9.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T08-A	1	4.98E+04			4.98E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T09-A	1	4.03E+04			4.03E+04	2.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T01-B	1	4.09E+02			4.09E+02	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T02-B	1	1.19E+03			1.19E+03	1.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T03-B	1	5.53E+02			5.53E+02	2.6E+00	1.0E+00	3.2E+00	1000	125	1.84E+03	103%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T04-B	1	3.15E+04			3.15E+04	8.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T05-B	1	4.25E+04			4.25E+04	6.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T06-B	1	5.46E+04			5.46E+04	9.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T07-B	1	6.40E+04			6.40E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T08-B	1	4.15E+04			4.15E+04	9.5E-02	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T09-B	1	3.74E+04			3.74E+04	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T01-C	1	4.14E+02			4.14E+02	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T02-C	1	1.32E+03			1.32E+03	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T03-C	1	5.16E+02			5.16E+02	3.8E+00	1.0E+00	3.2E+00	1000	125	1.83E+03	105%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T04-C	1	3.19E+04			3.19E+04	5.1E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T05-C	1	4.31E+04			4.31E+04	6.4E-01	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T06-C	1	4.87E+04			4.87E+04	3.6E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T07-C	1	5.85E+04			5.85E+04	1.9E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T08-C	1	4.28E+04			4.28E+04	6.8E-01	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-T09-C	1	3.89E+04			3.89E+04	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.8E+01	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.4E+01	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	2.7E+01	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	SWA-L02-1313-T01-A	1	6.08E+05			6.08E+05	8.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T02-A	1	7.31E+05			7.31E+05	7.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T03-A	1	6.19E+05			6.19E+05	1.2E+00	6.8E+00	2.2E+01	1000	125	6.20E+05	87%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T04-A	1	5.28E+05			5.28E+05	1.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T05-A	1	4.58E+05			4.58E+05	6.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T06-A	1	5.17E+05			5.17E+05	9.3E-02	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T07-A	1	5.17E+05			5.17E+05	2.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T08-A	1	3.72E+05			3.72E+05	8.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T09-A	1	2.73E+05			2.73E+05	2.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T01-B	1	7.28E+05			7.28E+05	1.3E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T02-B	1	6.38E+05			6.38E+05	3.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T03-B	1	4.63E+05			4.63E+05	4.3E+00	6.8E+00	2.2E+01	1000	125	4.65E+05	87%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T04-B	1	5.64E+05			5.64E+05	7.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T05-B	1	4.72E+05			4.72E+05	3.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T06-B	1	5.16E+05			5.16E+05	9.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T07-B	1	5.42E+05			5.42E+05	8.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T08-B	1	3.17E+05			3.17E+05	6.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T09-B	1	2.58E+05			2.58E+05	1.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T01-C	1	6.83E+05			6.83E+05	1.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T02-C	1	7.05E+05			7.05E+05	8.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T03-C	1	4.26E+05			4.26E+05	5.1E+00	6.8E+00	2.2E+01	1000	125	4.27E+05	82%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T04-C	1	5.52E+05			5.52E+05	3.4E+00	6.8E+00	2.2E+01					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T05-C	1	4.60E+05			4.60E+05	6.6E-01	6.8E+00	2.2E+01					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T06-C	1	4.68E+05			4.68E+05	1.8E+00	6.8E+00	2.2E+01					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T07-C	1	4.94E+05			4.94E+05	1.1E+00	6.8E+00	2.2E+01					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T08-C	1	3.30E+05			3.30E+05	4.9E-01	6.8E+00	2.2E+01					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-T09-C	1	2.67E+05			2.67E+05	5.9E-01	6.8E+00	2.2E+01					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	2.6E+00	6.8E+00	2.2E+01					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	6.5E+00	6.8E+00	2.2E+01					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	6.1E+00	6.8E+00	2.2E+01					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	SWA-L02-1313-T01-A	1	2.30E+00	U1/2		2.30E+00	3.0E+02	4.6E+00	1.5E+01				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T02-A	1	2.30E+00	U1/2		2.30E+00	6.8E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T03-A	1	2.30E+00	U1/2		2.30E+00	3.1E+02	4.6E+00	1.5E+01	10	125	1.08E+03	86%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T04-A	1	2.30E+00	U1/2		2.30E+00	1.5E+03	4.6E+00	1.5E+01				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T05-A	1	4.77E+00	E		4.77E+00	2.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T06-A	1	2.61E+01			2.61E+01	3.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T07-A	1	2.93E+01			2.93E+01	3.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T08-A	1	3.19E+01			3.19E+01	2.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T09-A	1	3.65E+01			3.65E+01	3.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T01-B	1	2.30E+00	U1/2		2.30E+00	2.8E+02	4.6E+00	1.5E+01				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T02-B	1	2.30E+00	U1/2		2.30E+00	4.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T03-B	1	2.30E+00	U1/2		2.30E+00	1.6E+03	4.6E+00	1.5E+01	10	125	1.11E+03	88%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T04-B	1	1.53E+01			1.53E+01	4.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T05-B	1	1.40E+01	E		1.40E+01	9.5E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T06-B	1	2.83E+01			2.83E+01	3.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T07-B	1	3.37E+01			3.37E+01	3.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T08-B	1	2.19E+01			2.19E+01	9.3E+00	4.6E+00	1.5E+01				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T09-B	1	4.65E+01			4.65E+01	9.9E+00	4.6E+00	1.5E+01				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T01-C	1	2.30E+00	U1/2		2.30E+00	7.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T02-C	1	2.30E+00	U1/2		2.30E+00	1.3E+04	4.6E+00	1.5E+01				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T03-C	1	2.30E+00	U1/2		2.30E+00	1.7E+02	4.6E+00	1.5E+01	10	125	1.08E+03	86%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T04-C	1	6.29E+00	E		6.29E+00	1.1E+02	4.6E+00	1.5E+01					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T05-C	1	-4.79E+00	U1/2		-4.79E+00	2.1E+02	4.6E+00	1.5E+01					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T06-C	1	1.52E+01			1.52E+01	1.3E+01	4.6E+00	1.5E+01					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T07-C	1	3.33E+01			3.33E+01	7.8E+00	4.6E+00	1.5E+01					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T08-C	1	2.53E+01			2.53E+01	9.2E+00	4.6E+00	1.5E+01					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-T09-C	1	3.95E+01			3.95E+01	2.3E+01	4.6E+00	1.5E+01					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	8.1E+01	4.6E+00	1.5E+01					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	5.9E+01	4.6E+00	1.5E+01					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	1.7E+02	4.6E+00	1.5E+01					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	SWA-L02-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	3.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	6.3E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	5.5E+01	2.0E+00	6.4E+00	10	125	1.24E+03	99%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	9.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	5.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	2.0E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T08-A	1	1.21E+02			1.21E+02	3.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T09-A	1	1.92E+02			1.92E+02	5.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	1.7E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	4.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	8.1E+01	2.0E+00	6.4E+00	10	125	1.28E+03	103%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	6.7E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	1.5E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	2.3E+03	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T08-B	1	4.27E+01			4.27E+01	3.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T09-B	1	1.73E+02			1.73E+02	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T01-C	1	3.98E+00	E		3.98E+00	3.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	8.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00	10	125	1.24E+03	99%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	1.1E+03	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	2.9E+02	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	2.8E+02	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T08-C	1	4.58E+01			4.58E+01	1.6E+00	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-T09-C	1	1.82E+02			1.82E+02	1.1E+00	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.7E+02	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	1.0E+02	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	3.4E+02	2.0E+00	6.4E+00					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	SWA-L02-1313-T01-A	1	3.51E+02			3.51E+02	1.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T02-A	1	2.06E+02			2.06E+02	2.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T03-A	1	3.63E+02			3.63E+02	1.6E+00	1.5E+00	4.8E+00	10	125	1.66E+03	103%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T04-A	1	2.65E+02			2.65E+02	1.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T05-A	1	2.39E+02			2.39E+02	1.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T06-A	1	2.63E+02			2.63E+02	9.2E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T07-A	1	2.45E+02			2.45E+02	2.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T08-A	1	2.00E+02			2.00E+02	2.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T09-A	1	5.13E+02			5.13E+02	9.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T01-B	1	3.84E+02			3.84E+02	1.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T02-B	1	2.06E+02			2.06E+02	2.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T03-B	1	3.04E+02			3.04E+02	3.3E+00	1.5E+00	4.8E+00	10	125	1.72E+03	113%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T04-B	1	2.71E+02			2.71E+02	1.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T05-B	1	2.40E+02			2.40E+02	3.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T06-B	1	2.65E+02			2.65E+02	1.9E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T07-B	1	2.52E+02			2.52E+02	1.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T08-B	1	1.62E+02			1.62E+02	2.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T09-B	1	4.68E+02			4.68E+02	1.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T01-C	1	3.61E+02			3.61E+02	2.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T02-C	1	2.17E+02			2.17E+02	5.9E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T03-C	1	2.95E+02			2.95E+02	4.2E+00	1.5E+00	4.8E+00	10	125	1.64E+03	108%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T04-C	1	2.51E+02			2.51E+02	3.7E+00	1.5E+00	4.8E+00					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T05-C	1	2.35E+02			2.35E+02	1.1E+00	1.5E+00	4.8E+00					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T06-C	1	2.45E+02			2.45E+02	2.7E+00	1.5E+00	4.8E+00					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T07-C	1	2.38E+02			2.38E+02	5.5E-01	1.5E+00	4.8E+00					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T08-C	1	1.68E+02			1.68E+02	1.6E+00	1.5E+00	4.8E+00					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-T09-C	1	4.92E+02			4.92E+02	1.5E+00	1.5E+00	4.8E+00					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-B01-A	1	7.50E-01	U1/2		7.50E-01	1.1E+02	1.5E+00	4.8E+00					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-B02-A	1	7.50E-01	U1/2		7.50E-01	9.9E+00	1.5E+00	4.8E+00					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1313-B03-A	1	7.50E-01	U1/2		7.50E-01	2.7E+02	1.5E+00	4.8E+00					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	SWA-L02-1313-T01-A	1	1.01E+00	E		1.01E+00	4.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:47 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T02-A	1	6.80E+00			6.80E+00	4.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:49 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T03-A	1	1.47E+02			1.47E+02	1.8E+00	1.0E+00	3.2E+00	10	125	1.49E+03	107%	VU ICP-OES	11/29/10 3:50 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T04-A	1	2.06E+02			2.06E+02	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:52 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T05-A	1	1.77E+01			1.77E+01	2.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:54 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T06-A	1	1.01E+02			1.01E+02	8.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:55 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T07-A	1	6.99E+02			6.99E+02	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:57 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T08-A	1	2.95E+03			2.95E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 3:59 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T09-A	1	3.35E+03			3.35E+03	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:00 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T01-B	1	4.76E+00			4.76E+00	8.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:12 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T02-B	1	5.00E-01	U1/2		5.00E-01	6.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:13 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T03-B	1	1.17E+02			1.17E+02	1.5E+00	1.0E+00	3.2E+00	10	125	1.52E+03	113%	VU ICP-OES	11/29/10 4:15 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T04-B	1	7.68E+01			7.68E+01	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:17 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T05-B	1	8.64E+00			8.64E+00	8.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:18 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T06-B	1	7.81E+01			7.81E+01	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:20 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T07-B	1	6.49E+02			6.49E+02	2.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:22 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T08-B	1	1.76E+03			1.76E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:23 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T09-B	1	2.98E+03			2.98E+03	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:25 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T01-C	1	5.98E+00			5.98E+00	9.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:37 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T02-C	1	1.04E+00	E		1.04E+00	3.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 4:38 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T03-C	1	1.19E+02			1.19E+02	3.3E+00	1.0E+00	3.2E+00	10	125	1.48E+03	109%	VU ICP-OES	11/29/10 4:40 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T04-C	1	3.86E+00			3.86E+00	6.8E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:43 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T05-C	1	3.30E+00			3.30E+00	2.6E+01	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:45 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T06-C	1	4.00E+01			4.00E+01	3.5E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:46 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T07-C	1	5.27E+02			5.27E+02	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:48 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T08-C	1	1.85E+03			1.85E+03	7.7E-01	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:50 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-T09-C	1	3.17E+03			3.17E+03	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 4:51 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.3E+02	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 3:42 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.6E+02	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 3:44 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	5.4E+00	1.0E+00	3.2E+00					VU ICP-OES	11/29/10 3:45 PM	EPA Interlab L02 1313-1316 SWA

QA-QC Spreadsheet 1313:

										Spike Sol'n						
Al	**Sample**	**Dilution**	**Sample Conc. µg/L**	**Qualifier**	**Internal Review**	**ICP-OES Conc. µg/L**	**RSD %**	**MDL µg/L**	**ML µg/L**	**Conc. µg/L**	**Volume µL**	**Spike Conc. µg/L**	**Spike Recovery %**	**Instrument**	**Date/Time**	**Filename**
Al	SWA-L04-1313-T01-A	1	6.23E+04			6.23E+04	2.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T02-A	1	1.51E+04			1.51E+04	4.8E-01	1.0E+00	3.2E+00	1000	100	1.59E+04	89%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T03-A	1	1.77E+02			1.77E+02	3.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T04-A	1	4.55E+01			4.55E+01	2.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T05-A	1	5.00E-01	U1/2		5.00E-01	1.8E+03	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T06-A	1	5.00E-01	U1/2		5.00E-01	4.6E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T07-A	1	8.72E+00			8.72E+00	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T08-A	1	3.29E+05			3.29E+05	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T09-A															
Al	SWA-L04-1313-T10-A	1	3.55E+04			3.55E+04	8.3E-01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T01-B	1	5.82E+04			5.82E+04	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T02-B	1	1.53E+04			1.53E+04	6.0E-01	1.0E+00	3.2E+00	1000	100	1.62E+04	90%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T03-B	1	1.42E+02			1.42E+02	6.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T04-B	1	3.13E+01			3.13E+01	2.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T05-B	1	5.00E-01	U1/2		5.00E-01	2.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T06-B	1	5.00E-01	U1/2		5.00E-01	1.2E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T07-B	1	1.89E+01			1.89E+01	5.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T08-B	1	3.01E+05			3.01E+05	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T09-B	1	1.28E+06			1.28E+06	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T10-B	1	3.72E+04			3.72E+04	5.9E-01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T01-C	1	5.92E+04			5.92E+04	7.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T02-C	1	1.74E+04			1.74E+04	6.9E-01	1.0E+00	3.2E+00	1000	100	1.84E+04	92%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T03-C	1	2.98E+02			2.98E+02	3.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T04-C	1	5.10E+01			5.10E+01	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T05-C	1	5.00E-01	U1/2		5.00E-01	1.5E+02	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T06-C	1	5.00E-01	U1/2		5.00E-01	5.2E+02	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T07-C	1	5.00E-01	U1/2		5.00E-01	5.7E+02	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T08-C	1	1.45E+05			1.45E+05	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-T09-C															
Al	SWA-L04-1313-T10-C	1	3.80E+04			3.80E+04	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.3E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	3.2E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	3.1E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	1.3E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	3.5E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	2.0E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	3.8E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	9.9E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	1.3E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	SWA-L04-1313-T01-A	1	6.21E+03			6.21E+03	2.0E+00	7.5E+00	2.4E+01			---		VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T02-A	1	2.33E+03			2.33E+03	4.4E-01	7.5E+00	2.4E+01	10	100	3.25E+03	92%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T03-A	1	1.30E+03			1.30E+03	1.8E+00	7.5E+00	2.4E+01			---		VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T04-A	1	1.36E+03			1.36E+03	1.0E+00	7.5E+00	2.4E+01			---		VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T05-A	1	1.20E+03			1.20E+03	9.7E-01	7.5E+00	2.4E+01			---		VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T06-A	1	1.15E+03			1.15E+03	2.0E+00	7.5E+00	2.4E+01			---		VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T07-A	1	9.77E+02			9.77E+02	8.5E+00	7.5E+00	2.4E+01			---		VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T08-A	1	3.03E+02			3.03E+02	4.9E+00	7.5E+00	2.4E+01			---		VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T09-A															
Sb	SWA-L04-1313-T10-A	1	4.28E+03			4.28E+03	7.4E-01	7.5E+00	2.4E+01					VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T01-B	1	5.79E+03			5.79E+03	1.2E+00	7.5E+00	2.4E+01			---		VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T02-B	1	2.33E+03			2.33E+03	3.4E-01	7.5E+00	2.4E+01	10	100	3.28E+03	95%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T03-B	1	1.31E+03			1.31E+03	6.5E-01	7.5E+00	2.4E+01			---		VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T04-B	1	1.21E+03			1.21E+03	2.0E+00	7.5E+00	2.4E+01			---		VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T05-B	1	1.37E+03			1.37E+03	1.3E+00	7.5E+00	2.4E+01			---		VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T06-B	1	1.25E+03			1.25E+03	8.6E-02	7.5E+00	2.4E+01			---		VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T07-B	1	1.15E+03			1.15E+03	2.4E+00	7.5E+00	2.4E+01			---		VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T08-B	1	4.33E+02			4.33E+02	6.4E+00	7.5E+00	2.4E+01			---		VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T09-B	1	1.14E+03			1.14E+03	9.1E+00	7.5E+00	2.4E+01			---		VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T10-B	1	4.27E+03			4.27E+03	8.5E-02	7.5E+00	2.4E+01					VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T01-C	1	5.94E+03			5.94E+03	3.3E-01	7.5E+00	2.4E+01			---		VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T02-C	1	2.32E+03			2.32E+03	5.2E-01	7.5E+00	2.4E+01	10	100	3.31E+03	99%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T03-C	1	1.31E+03			1.31E+03	7.2E-01	7.5E+00	2.4E+01			---		VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T04-C	1	1.32E+03			1.32E+03	8.3E-01	7.5E+00	2.4E+01					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T05-C	1	1.19E+03			1.19E+03	5.1E-01	7.5E+00	2.4E+01					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T06-C	1	1.20E+03			1.20E+03	4.7E-01	7.5E+00	2.4E+01					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T07-C	1	1.01E+03			1.01E+03	3.0E+00	7.5E+00	2.4E+01					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T08-C	1	5.49E+02			5.49E+02	8.5E+00	7.5E+00	2.4E+01					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-T09-C															
Sb	SWA-L04-1313-T10-C	1	4.09E+03			4.09E+03	6.9E-01	7.5E+00	2.4E+01					VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-B01-A	1	3.75E+00	U1/2		3.75E+00	4.3E+01	7.5E+00	2.4E+01					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-B02-A	1	3.75E+00	U1/2		3.75E+00	7.2E+01	7.5E+00	2.4E+01					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-B03-A	1	1.15E+01	E		1.15E+01	1.3E+01	7.5E+00	2.4E+01					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-B01-B	1	3.75E+00	U1/2		3.75E+00	4.9E+01	7.5E+00	2.4E+01					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-B02-B	1	3.75E+00	U1/2		3.75E+00	1.3E+02	7.5E+00	2.4E+01					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-B03-B	1	8.89E+00	E		8.89E+00	1.4E+01	7.5E+00	2.4E+01					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-B01-C	1	3.75E+00	U1/2		3.75E+00	7.5E+01	7.5E+00	2.4E+01					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-B02-C	1	3.75E+00	U1/2		3.75E+00	6.0E+01	7.5E+00	2.4E+01					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1313-B03-C	1	8.72E+00	E		8.72E+00	8.1E+01	7.5E+00	2.4E+01					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	SWA-L04-1313-T01-A	1	1.09E+04			1.09E+04	7.8E-01	1.1E+01	3.5E+01			---		VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T02-A	1	1.17E+03			1.17E+03	2.0E-01	1.1E+01	3.5E+01	10	100	2.26E+03	109%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T03-A	1	1.24E+02			1.24E+02	5.6E+00	1.1E+01	3.5E+01			---		VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T04-A	1	4.78E+02			4.78E+02	3.5E+00	1.1E+01	3.5E+01			---		VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T05-A	1	1.83E+02			1.83E+02	9.2E+00	1.1E+01	3.5E+01			---		VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T06-A	1	2.23E+02			2.23E+02	4.7E+00	1.1E+01	3.5E+01			---		VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T07-A	1	1.05E+03			1.05E+03	9.9E-01	1.1E+01	3.5E+01			---		VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T08-A	1	2.08E+03			2.08E+03	8.0E-01	1.1E+01	3.5E+01			---		VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T09-A															
As	SWA-L04-1313-T10-A	1	4.28E+03			4.28E+03	2.6E-01	1.1E+01	3.5E+01					VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T01-B	1	9.30E+03			9.30E+03	1.8E+00	1.1E+01	3.5E+01			---		VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T02-B	1	1.27E+03			1.27E+03	9.7E-01	1.1E+01	3.5E+01	10	100	2.38E+03	111%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T03-B	1	9.99E+01			9.99E+01	1.4E+01	1.1E+01	3.5E+01			---		VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T04-B	1	2.75E+02			2.75E+02	3.2E+00	1.1E+01	3.5E+01			---		VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T05-B	1	1.81E+02			1.81E+02	1.5E+01	1.1E+01	3.5E+01			---		VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T06-B	1	1.79E+02			1.79E+02	1.0E+01	1.1E+01	3.5E+01			---		VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T07-B	1	3.12E+02			3.12E+02	2.3E+00	1.1E+01	3.5E+01			---		VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T08-B	1	2.07E+03			2.07E+03	1.6E+00	1.1E+01	3.5E+01			---		VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T09-B	1	1.35E+04			1.35E+04	1.6E+00	1.1E+01	3.5E+01			---		VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T10-B	1	5.28E+03			5.28E+03	7.5E-01	1.1E+01	3.5E+01					VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T01-C	1	9.34E+03			9.34E+03	1.0E+00	1.1E+01	3.5E+01			---		VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T02-C	1	2.01E+03			2.01E+03	7.4E-01	1.1E+01	3.5E+01	10	100	3.07E+03	107%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T03-C	1	1.31E+02			1.31E+02	1.4E+01	1.1E+01	3.5E+01			---		VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T04-C	1	3.57E+02			3.57E+02	4.9E+00	1.1E+01	3.5E+01					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T05-C	1	2.06E+02			2.06E+02	7.0E+00	1.1E+01	3.5E+01					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T06-C	1	2.15E+02			2.15E+02	3.2E+00	1.1E+01	3.5E+01					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T07-C	1	2.87E+02			2.87E+02	3.7E+00	1.1E+01	3.5E+01					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T08-C	1	2.32E+03			2.32E+03	6.9E-01	1.1E+01	3.5E+01					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-T09-C															
As	SWA-L04-1313-T10-C	1	5.29E+03			5.29E+03	1.1E+00	1.1E+01	3.5E+01					VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-B01-A	1	5.50E+00	U1/2		5.50E+00	3.8E+01	1.1E+01	3.5E+01					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-B02-A	1	5.50E+00	U1/2		5.50E+00	3.8E+01	1.1E+01	3.5E+01					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-B03-A	1	5.50E+00	U1/2		5.50E+00	5.0E+01	1.1E+01	3.5E+01					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-B01-B	1	5.50E+00	U1/2		5.50E+00	6.7E+03	1.1E+01	3.5E+01					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-B02-B	1	5.50E+00	U1/2		5.50E+00	1.4E+02	1.1E+01	3.5E+01					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-B03-B	1	5.50E+00	U1/2		5.50E+00	1.1E+02	1.1E+01	3.5E+01					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-B01-C	1	5.50E+00	U1/2		5.50E+00	3.6E+01	1.1E+01	3.5E+01					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-B02-C	1	5.50E+00	U1/2		5.50E+00	6.0E+01	1.1E+01	3.5E+01					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1313-B03-C	1	5.50E+00	U1/2		5.50E+00	1.2E+01	1.1E+01	3.5E+01					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	SWA-L04-1313-T01-A	1	1.34E+03			1.34E+03	7.1E-02	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T02-A	1	7.89E+02			7.89E+02	6.8E-01	1.0E+00	3.2E+00	1000	100	1.92E+03	113%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T03-A	1	1.14E+03			1.14E+03	7.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T04-A	1	1.95E+03			1.95E+03	5.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T05-A	1	3.14E+03			3.14E+03	5.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T06-A	1	4.70E+03			4.70E+03	2.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T07-A	1	6.70E+03			6.70E+03	9.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T08-A	1	5.71E+03			5.71E+03	1.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T09-A															
B	SWA-L04-1313-T10-A	1	9.88E+02			9.88E+02	4.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T01-B	1	1.16E+03			1.16E+03	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T02-B	1	8.27E+02			8.27E+02	9.5E-01	1.0E+00	3.2E+00	1000	100	2.01E+03	118%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T03-B	1	1.11E+03			1.11E+03	8.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T04-B	1	2.11E+03			2.11E+03	6.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T05-B	1	2.60E+03			2.60E+03	6.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T06-B	1	3.44E+03			3.44E+03	8.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T07-B	1	5.43E+03			5.43E+03	2.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T08-B	1	5.78E+03			5.78E+03	5.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T09-B	1	1.14E+04			1.14E+04	4.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T10-B	1	1.16E+03			1.16E+03	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T01-C	1	1.33E+03			1.33E+03	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T02-C	1	1.05E+03			1.05E+03	1.6E+00	1.0E+00	3.2E+00	1000	100	2.18E+03	112%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T03-C	1	1.14E+03			1.14E+03	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T04-C	1	1.76E+03			1.76E+03	5.1E-01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T05-C	1	3.15E+03			3.15E+03	5.4E-01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T06-C	1	3.82E+03			3.82E+03	5.8E-01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T07-C	1	5.45E+03			5.45E+03	1.9E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T08-C	1	5.59E+03			5.59E+03	3.8E-01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-T09-C															
B	SWA-L04-1313-T10-C	1	1.19E+03			1.19E+03	9.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-B01-A	1	1.33E+01			1.33E+01	6.1E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-B02-A	1	1.87E+01			1.87E+01	6.4E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-B03-A	1	1.45E+01			1.45E+01	7.3E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-B01-B	1	9.62E+00			9.62E+00	4.0E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-B02-B	1	1.18E+01			1.18E+01	2.2E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-B03-B	1	1.26E+01			1.26E+01	1.5E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-B01-C	1	9.01E+00			9.01E+00	2.2E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-B02-C	1	1.22E+01			1.22E+01	1.3E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1313-B03-C	1	9.34E+00			9.34E+00	1.8E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	SWA-L04-1313-T01-A	1	2.36E+02			2.36E+02	1.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T02-A	1	2.75E+02			2.75E+02	2.3E-01	1.0E+00	3.2E+00	10	100	1.26E+03	99%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T03-A	1	1.08E+03			1.08E+03	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T04-A	1	1.11E+03			1.11E+03	2.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T05-A	1	1.24E+03			1.24E+03	3.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T06-A	1	1.55E+03			1.55E+03	1.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T07-A	1	1.16E+03			1.16E+03	4.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T08-A	1	6.39E+02			6.39E+02	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T09-A															
Ba	SWA-L04-1313-T10-A	1	1.97E+02			1.97E+02	6.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T01-B	1	2.45E+02			2.45E+02	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T02-B	1	2.64E+02			2.64E+02	2.1E-01	1.0E+00	3.2E+00	10	100	1.30E+03	103%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T03-B	1	1.05E+03			1.05E+03	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T04-B	1	1.15E+03			1.15E+03	6.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T05-B	1	1.22E+03			1.22E+03	2.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T06-B	1	1.36E+03			1.36E+03	6.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T07-B	1	1.67E+03			1.67E+03	6.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T08-B	1	6.81E+02			6.81E+02	6.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T09-B	1	1.51E+03			1.51E+03	4.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T10-B	1	1.76E+02			1.76E+02	4.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T01-C	1	2.60E+02			2.60E+02	3.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T02-C	1	2.49E+02			2.49E+02	7.3E-01	1.0E+00	3.2E+00	10	100	1.32E+03	107%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T03-C	1	1.02E+03			1.02E+03	5.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T04-C	1	1.24E+03			1.24E+03	7.0E-01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T05-C	1	1.27E+03			1.27E+03	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T06-C	1	1.44E+03			1.44E+03	6.1E-01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T07-C	1	1.67E+03			1.67E+03	1.6E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T08-C	1	7.32E+02			7.32E+02	5.1E-01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-T09-C															
Ba	SWA-L04-1313-T10-C	1	1.76E+02			1.76E+02	9.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	3.5E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	7.8E-01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-B03-A	1	1.08E+00	E		1.08E+00	5.8E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	1.3E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	3.5E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-B03-B	1	1.33E+00	E		1.33E+00	3.1E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	1.7E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	4.1E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	2.3E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	SWA-L04-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	7.3E+01	1.9E+00	6.0E+00			---		VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00	10	100	1.18E+03	118%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	2.2E+02	1.9E+00	6.0E+00			---		VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	1.7E+02	1.9E+00	6.0E+00			---		VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	1.8E+02	1.9E+00	6.0E+00			---		VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	6.7E+01	1.9E+00	6.0E+00			---		VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T07-A	1	9.50E-01	U1/2		9.50E-01	3.6E+01	1.9E+00	6.0E+00			---		VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T08-A	1	5.63E+01			5.63E+01	3.7E+00	1.9E+00	6.0E+00			---		VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T09-A															
Be	SWA-L04-1313-T10-A	1	9.50E-01	U1/2		9.50E-01	9.9E+01	1.9E+00	6.0E+00			---		VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00			---		VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	1.6E+02	1.9E+00	6.0E+00	10	100	1.13E+03	113%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	4.6E+01	1.9E+00	6.0E+00			---		VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	4.0E+01	1.9E+00	6.0E+00			---		VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	3.0E+01	1.9E+00	6.0E+00			---		VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	7.8E+01	1.9E+00	6.0E+00			---		VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T07-B	1	9.50E-01	U1/2		9.50E-01	2.3E+02	1.9E+00	6.0E+00			---		VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T08-B	1	4.93E+01			4.93E+01	8.4E-01	1.9E+00	6.0E+00			---		VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T09-B	1	2.32E+02			2.32E+02	3.6E-01	1.9E+00	6.0E+00			---		VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T10-B	1	9.50E-01	U1/2		9.50E-01	3.3E+01	1.9E+00	6.0E+00			---		VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	3.2E+02	1.9E+00	6.0E+00			---		VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	2.2E+02	1.9E+00	6.0E+00	10	100	1.16E+03	116%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	2.9E+01	1.9E+00	6.0E+00			---		VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	4.1E+01	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	1.4E+01	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T07-C	1	9.50E-01	U1/2		9.50E-01	3.9E+01	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T08-C	1	1.23E+01			1.23E+01	7.4E+00	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-T09-C															
Be	SWA-L04-1313-T10-C	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00			---		VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	9.3E+01	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-B01-B	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-B02-B	1	9.50E-01	U1/2		9.50E-01	1.6E+02	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-B03-B	1	9.50E-01	U1/2		9.50E-01	2.2E+01	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-B01-C	1	9.50E-01	U1/2		9.50E-01	1.0E+02	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-B02-C	1	9.50E-01	U1/2		9.50E-01	1.5E+02	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1313-B03-C	1	9.50E-01	U1/2		9.50E-01	6.4E+00	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	SWA-L04-1313-T01-A	1	1.10E+00	U1/2		1.10E+00	1.6E+02	2.2E+00	7.0E+00			---		VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T02-A	1	1.10E+00	U1/2		1.10E+00	1.8E+03	2.2E+00	7.0E+00	10	100	1.15E+03	115%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	1.3E+02	2.2E+00	7.0E+00			---		VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T04-A	1	1.10E+00	U1/2		1.10E+00	1.1E+02	2.2E+00	7.0E+00			---		VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T05-A	1	1.10E+00	U1/2		1.10E+00	5.0E+01	2.2E+00	7.0E+00			---		VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T06-A	1	1.10E+00	U1/2		1.10E+00	2.3E+01	2.2E+00	7.0E+00			---		VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T07-A	1	1.12E+01			1.12E+01	4.3E+00	2.2E+00	7.0E+00			---		VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T08-A	1	2.06E+01			2.06E+01	2.1E+00	2.2E+00	7.0E+00			---		VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T09-A															
Cd	SWA-L04-1313-T10-A	1	1.10E+00	U1/2		1.10E+00	6.9E+02	2.2E+00	7.0E+00			---		VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T01-B	1	1.10E+00	U1/2		1.10E+00	8.3E+02	2.2E+00	7.0E+00			---		VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T02-B	1	1.10E+00	U1/2		1.10E+00	5.3E+02	2.2E+00	7.0E+00	10	100	1.20E+03	120%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	1.5E+02	2.2E+00	7.0E+00			---		VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T04-B	1	1.10E+00	U1/2		1.10E+00	1.2E+02	2.2E+00	7.0E+00			---		VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T05-B	1	1.10E+00	U1/2		1.10E+00	1.9E+02	2.2E+00	7.0E+00			---		VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T06-B	1	1.10E+00	U1/2		1.10E+00	8.2E+01	2.2E+00	7.0E+00			---		VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T07-B	1	7.19E+00			7.19E+00	1.3E+01	2.2E+00	7.0E+00			---		VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T08-B	1	2.00E+01			2.00E+01	1.7E+00	2.2E+00	7.0E+00			---		VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T09-B	1	5.75E+01			5.75E+01	1.5E+00	2.2E+00	7.0E+00			---		VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T10-B	1	1.10E+00	U1/2		1.10E+00	1.3E+02	2.2E+00	7.0E+00			---		VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T01-C	1	1.10E+00	U1/2		1.10E+00	2.5E+01	2.2E+00	7.0E+00			---		VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T02-C	1	1.10E+00	U1/2		1.10E+00	5.6E+01	2.2E+00	7.0E+00	10	100	1.13E+03	113%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	1.2E+02	2.2E+00	7.0E+00			---		VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T04-C	1	1.10E+00	U1/2		1.10E+00	2.8E+02	2.2E+00	7.0E+00					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T05-C	1	1.10E+00	U1/2		1.10E+00	5.5E+01	2.2E+00	7.0E+00					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T06-C	1	1.10E+00	U1/2		1.10E+00	7.7E+01	2.2E+00	7.0E+00					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T07-C	1	5.83E+00	E		5.83E+00	9.3E+00	2.2E+00	7.0E+00					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T08-C	1	1.33E+01			1.33E+01	1.7E+00	2.2E+00	7.0E+00					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-T09-C															
Cd	SWA-L04-1313-T10-C	1	1.10E+00	U1/2		1.10E+00	3.8E+01	2.2E+00	7.0E+00			---		VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	1.2E+02	2.2E+00	7.0E+00					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	4.6E+01	2.2E+00	7.0E+00					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-B03-A	1	1.10E+00	U1/2		1.10E+00	1.7E+02	2.2E+00	7.0E+00					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-B01-B	1	1.10E+00	U1/2		1.10E+00	7.1E+02	2.2E+00	7.0E+00					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-B02-B	1	1.10E+00	U1/2		1.10E+00	2.3E+02	2.2E+00	7.0E+00					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-B03-B	1	1.10E+00	U1/2		1.10E+00	2.6E+02	2.2E+00	7.0E+00					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-B01-C	1	1.10E+00	U1/2		1.10E+00	2.5E+02	2.2E+00	7.0E+00					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-B02-C	1	1.10E+00	U1/2		1.10E+00	1.5E+02	2.2E+00	7.0E+00					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1313-B03-C	1	1.10E+00	U1/2		1.10E+00	2.4E+02	2.2E+00	7.0E+00					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	SWA-L04-1313-T01-A	1	7.09E+03			7.09E+03	7.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T02-A	1	3.87E+04			3.87E+04	5.6E-01	2.6E+00	8.3E+00	1000	100	3.96E+04	87%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T03-A	1	3.15E+06			3.15E+06	2.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T04-A	1	5.84E+06			5.84E+06	7.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T05-A	1	7.20E+06			7.20E+06	6.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T06-A	1	8.59E+06			8.59E+06	5.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T07-A	1	6.29E+06			6.29E+06	3.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T08-A	1	3.48E+06			3.48E+06	6.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T09-A															
Ca	SWA-L04-1313-T10-A	1	1.43E+04			1.43E+04	1.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T01-B	1	7.59E+03			7.59E+03	1.6E+00	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T02-B	1	3.71E+04			3.71E+04	4.0E-01	2.6E+00	8.3E+00	1000	100	3.81E+04	97%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T03-B	1	3.23E+06			3.23E+06	1.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T04-B	1	5.80E+06			5.80E+06	4.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T05-B	1	6.67E+06			6.67E+06	3.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T06-B	1	7.66E+06			7.66E+06	8.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T07-B	1	8.52E+06			8.52E+06	2.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T08-B	1	3.59E+06			3.59E+06	8.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T09-B	1	5.62E+06			5.62E+06	5.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T10-B	1	1.26E+04			1.26E+04	7.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T01-C	1	7.84E+03			7.84E+03	3.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T02-C	1	3.09E+04			3.09E+04	6.7E-01	2.6E+00	8.3E+00	1000	100	3.18E+04	91%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T03-C	1	2.89E+06			2.89E+06	9.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T04-C	1	5.52E+06			5.52E+06	8.4E-01	2.6E+00	8.3E+00					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T05-C	1	7.14E+06			7.14E+06	7.3E-01	2.6E+00	8.3E+00					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T06-C	1	7.75E+06			7.75E+06	4.4E-01	2.6E+00	8.3E+00					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T07-C	1	8.71E+06			8.71E+06	1.6E+00	2.6E+00	8.3E+00					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T08-C	1	4.19E+06			4.19E+06	1.1E+00	2.6E+00	8.3E+00					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-T09-C															
Ca	SWA-L04-1313-T10-C	1	1.28E+04			1.28E+04	8.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-B01-A	1	3.34E+01			3.34E+01	1.3E+01	2.6E+00	8.3E+00					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-B02-A	1	4.57E+01			4.57E+01	7.8E+00	2.6E+00	8.3E+00					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-B03-A	1	4.49E+01			4.49E+01	1.2E+01	2.6E+00	8.3E+00					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-B01-B	1	2.75E+01			2.75E+01	9.8E-01	2.6E+00	8.3E+00					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-B02-B	1	5.04E+01			5.04E+01	7.1E+00	2.6E+00	8.3E+00					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-B03-B	1	3.49E+01			3.49E+01	9.4E-01	2.6E+00	8.3E+00					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-B01-C	1	3.46E+01			3.46E+01	2.2E+01	2.6E+00	8.3E+00					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-B02-C	1	6.39E+01			6.39E+01	2.3E+01	2.6E+00	8.3E+00					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1313-B03-C	1	4.53E+01			4.53E+01	1.3E+01	2.6E+00	8.3E+00					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	SWA-L04-1313-T01-A	1	1.47E+03			1.47E+03	7.1E-01	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T02-A	1	2.95E+02			2.95E+02	7.8E-01	1.2E+00	3.8E+00	10	100	1.40E+03	111%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T03-A	1	9.59E+00			9.59E+00	1.2E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T04-A	1	1.05E+01			1.05E+01	7.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T05-A	1	9.32E+00			9.32E+00	1.1E+01	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T06-A	1	5.30E+00			5.30E+00	1.5E+02	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T07-A	1	6.21E+01			6.21E+01	5.2E-01	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T08-A	1	5.33E+03			5.33E+03	6.2E-01	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T09-A															
Cr	SWA-L04-1313-T10-A	1	1.03E+03			1.03E+03	1.0E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T01-B	1	1.43E+03			1.43E+03	2.0E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T02-B	1	3.28E+02			3.28E+02	3.7E-01	1.2E+00	3.8E+00	10	100	1.48E+03	115%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T03-B	1	1.12E+01			1.12E+01	7.4E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T04-B	1	9.82E+00			9.82E+00	7.6E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T05-B	1	1.85E+01			1.85E+01	6.0E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T06-B	1	5.92E+00			5.92E+00	9.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T07-B	1	7.28E+00			7.28E+00	1.4E+01	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T08-B	1	4.88E+03			4.88E+03	5.8E-01	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T09-B	1	3.22E+04			3.22E+04	2.9E-01	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T10-B	1	1.21E+03			1.21E+03	4.7E-01	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T01-C	1	1.45E+03			1.45E+03	1.3E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T02-C	1	4.99E+02			4.99E+02	2.1E+00	1.2E+00	3.8E+00	10	100	1.65E+03	115%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T03-C	1	1.17E+01			1.17E+01	3.7E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T04-C	1	1.38E+01			1.38E+01	1.5E+00	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T05-C	1	1.65E+01			1.65E+01	1.1E+00	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T06-C	1	5.49E+00			5.49E+00	2.4E+01	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T07-C	1	5.57E+00			5.57E+00	7.2E+00	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T08-C	1	1.67E+03			1.67E+03	3.9E-01	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-T09-C															
Cr	SWA-L04-1313-T10-C	1	1.20E+03			1.20E+03	1.8E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	2.7E+02	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	1.1E+02	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-B03-A	1	6.00E-01	U1/2		6.00E-01	9.7E+01	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-B01-B	1	6.00E-01	U1/2		6.00E-01	4.0E+02	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-B02-B	1	6.00E-01	U1/2		6.00E-01	7.8E+01	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-B03-B	1	6.00E-01	U1/2		6.00E-01	8.5E+01	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-B01-C	1	6.00E-01	U1/2		6.00E-01	4.2E+01	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-B02-C	1	6.00E-01	U1/2		6.00E-01	2.4E+02	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1313-B03-C	1	6.00E-01	U1/2		6.00E-01	5.5E+01	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	SWA-L04-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	1.8E+02	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	3.0E+02	1.8E+00	5.7E+00	10	100	1.11E+03	111%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	2.1E+01	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T04-A	1	4.67E+00	E		4.67E+00	2.7E+01	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T05-A	1	2.30E+01			2.30E+01	7.0E+00	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T06-A	1	1.01E+02			1.01E+02	2.6E+00	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T07-A	1	2.04E+02			2.04E+02	8.7E-01	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T08-A	1	1.59E+02			1.59E+02	3.7E-01	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T09-A															
Co	SWA-L04-1313-T10-A	1	9.00E-01	U1/2		9.00E-01	2.2E+02	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	2.3E+03	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	2.3E+02	1.8E+00	5.7E+00	10	100	1.14E+03	114%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	2.5E+02	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T04-B	1	4.13E+00	E		4.13E+00	1.7E+01	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T05-B	1	9.74E+00			9.74E+00	1.3E+01	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T06-B	1	2.80E+01			2.80E+01	6.5E+00	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T07-B	1	1.66E+02			1.66E+02	1.6E+00	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T08-B	1	1.61E+02			1.61E+02	1.4E+00	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T09-B	1	3.70E+02			3.70E+02	3.0E-01	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T10-B	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	3.2E+02	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	5.2E+02	1.8E+00	5.7E+00	10	100	1.17E+03	117%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	3.4E+02	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T04-C	1	3.10E+00	E		3.10E+00	4.4E+01	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T05-C	1	1.70E+01			1.70E+01	1.5E+01	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T06-C	1	4.66E+01			4.66E+01	1.4E+00	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T07-C	1	1.62E+02			1.62E+02	8.8E-01	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T08-C	1	1.46E+02			1.46E+02	7.9E-01	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-T09-C															
Co	SWA-L04-1313-T10-C	1	9.00E-01	U1/2		9.00E-01	2.2E+03	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	4.9E+01	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	2.1E+02	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-B01-B	1	9.00E-01	U1/2		9.00E-01	3.1E+01	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-B02-B	1	9.00E-01	U1/2		9.00E-01	5.3E+01	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-B03-B	1	9.00E-01	U1/2		9.00E-01	5.4E+01	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-B01-C	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-B02-C	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1313-B03-C	1	9.00E-01	U1/2		9.00E-01	2.7E+01	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	SWA-L04-1313-T01-A	1	1.85E+00	U1/2		1.85E+00	1.1E+02	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T02-A	1	1.85E+00	U1/2		1.85E+00	1.0E+02	3.7E+00	1.2E+01	10	100	1.10E+03	109%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T03-A	1	1.03E+01	E		1.03E+01	2.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T04-A	1	1.03E+01	E		1.03E+01	2.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T05-A	1	1.36E+01			1.36E+01	1.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T06-A	1	2.11E+01			2.11E+01	7.3E+00	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T07-A	1	2.28E+01			2.28E+01	5.3E+00	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T08-A	1	1.55E+02			1.55E+02	5.7E-01	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T09-A															
Cu	SWA-L04-1313-T10-A	1	1.85E+00	U1/2		1.85E+00	5.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T01-B	1	1.85E+00	U1/2		1.85E+00	8.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T02-B	1	1.85E+00	U1/2		1.85E+00	9.5E+01	3.7E+00	1.2E+01	10	100	1.14E+03	113%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T03-B	1	1.01E+01	E		1.01E+01	5.9E+00	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T04-B	1	1.20E+01			1.20E+01	9.1E+00	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T05-B	1	1.16E+01	E		1.16E+01	2.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T06-B	1	1.23E+01			1.23E+01	1.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T07-B	1	3.27E+01			3.27E+01	8.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T08-B	1	1.26E+02			1.26E+02	2.8E-01	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T09-B	1	2.33E+03			2.33E+03	3.9E-01	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T10-B	1	1.85E+00	U1/2		1.85E+00	6.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T01-C	1	1.85E+00	U1/2		1.85E+00	5.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T02-C	1	1.85E+00	U1/2		1.85E+00	8.2E+01	3.7E+00	1.2E+01	10	100	1.16E+03	116%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T03-C	1	6.00E+00	E		6.00E+00	3.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T04-C	1	1.09E+01	E		1.09E+01	3.6E+01	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T05-C	1	1.13E+01	E		1.13E+01	3.7E+00	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T06-C	1	1.69E+01			1.69E+01	9.9E+00	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T07-C	1	3.23E+01			3.23E+01	4.6E+00	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T08-C	1	2.37E+01			2.37E+01	3.0E+00	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-T09-C															
Cu	SWA-L04-1313-T10-C	1	1.85E+00	U1/2		1.85E+00	1.6E+02	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	3.9E+01	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	2.4E+01	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-B03-A	1	1.85E+00	U1/2		1.85E+00	1.3E+02	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-B01-B	1	1.85E+00	U1/2		1.85E+00	9.9E+01	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-B02-B	1	1.85E+00	U1/2		1.85E+00	4.3E+01	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-B03-B	1	1.85E+00	U1/2		1.85E+00	5.2E+01	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-B01-C	1	1.85E+00	U1/2		1.85E+00	1.3E+02	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-B02-C	1	1.85E+00	U1/2		1.85E+00	8.5E+01	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1313-B03-C	1	1.85E+00	U1/2		1.85E+00	7.4E+01	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	SWA-L04-1313-T01-A	1	1.09E+02			1.09E+02	5.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T02-A	1	4.69E+01			4.69E+01	1.7E+00	2.0E+00	6.4E+00	1000	100	1.21E+03	116%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T03-A	1	9.29E+00			9.29E+00	5.5E+00	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T04-A	1	1.86E+01			1.86E+01	1.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T05-A	1	1.09E+01			1.09E+01	3.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T06-A	1	3.70E+03			3.70E+03	4.1E-01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T07-A	1	1.13E+05			1.13E+05	2.4E-01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T08-A	1	1.04E+05			1.04E+05	8.1E-01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T09-A															
Fe	SWA-L04-1313-T10-A	1	6.94E+01			6.94E+01	3.3E-01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T01-B	1	8.99E+01			8.99E+01	5.4E-01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T02-B	1	4.62E+01			4.62E+01	3.4E-01	2.0E+00	6.4E+00	1000	100	1.23E+03	119%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T03-B	1	1.01E+01			1.01E+01	6.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T04-B	1	1.68E+01			1.68E+01	1.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T05-B	1	1.42E+01			1.42E+01	7.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T06-B	1	1.17E+01			1.17E+01	7.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T07-B	1	5.72E+04			5.72E+04	3.9E-01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T08-B	1	1.03E+05			1.03E+05	1.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T09-B	1	2.50E+05			2.50E+05	4.5E+00	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T10-B	1	8.48E+01			8.48E+01	6.4E-01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T01-C	1	1.05E+02			1.05E+02	9.6E-01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T02-C	1	6.63E+01			6.63E+01	8.4E-01	2.0E+00	6.4E+00	1000	100	1.27E+03	120%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T03-C	1	1.21E+01			1.21E+01	5.8E-01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T04-C	1	1.91E+01			1.91E+01	1.5E+00	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T05-C	1	1.26E+01			1.26E+01	2.8E+00	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T06-C	1	1.28E+01			1.28E+01	5.4E+00	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T07-C	1	5.17E+04			5.17E+04	1.1E+00	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T08-C	1	9.15E+04			9.15E+04	8.5E-01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-T09-C															
Fe	SWA-L04-1313-T10-C	1	8.39E+01			8.39E+01	9.1E-01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	5.3E+01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-B02-A	1	3.30E+00	E		3.30E+00	1.2E+01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	8.2E+01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-B02-B	1	4.39E+00	E		4.39E+00	7.8E+00	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-B03-B	1	3.95E+00	E		3.95E+00	1.5E+01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	5.5E+01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-B02-C	1	5.41E+00	E		5.41E+00	9.5E-01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1313-B03-C	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	SWA-L04-1313-T01-A	1	6.23E+01			6.23E+01	1.2E+01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T02-A	1	9.09E+00	E		9.09E+00	1.3E+02	6.8E+00	2.2E+01	10	100	1.11E+03	110%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T03-A	1	3.40E+00	U1/2		3.40E+00	1.0E+02	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T04-A	1	3.40E+00	U1/2		3.40E+00	2.8E+02	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T05-A	1	9.98E+00	E		9.98E+00	8.3E+01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T06-A	1	1.10E+01	E		1.10E+01	4.4E+01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T07-A	1	2.32E+01			2.32E+01	5.5E+01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T08-A	1	5.21E+02			5.21E+02	1.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T09-A															
Pb	SWA-L04-1313-T10-A	1	1.13E+01	E		1.13E+01	2.2E+01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T01-B	1	5.26E+01			5.26E+01	8.9E+00	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T02-B	1	1.03E+01	E		1.03E+01	6.1E+01	6.8E+00	2.2E+01	10	100	1.15E+03	114%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T03-B	1	3.40E+00	U1/2		3.40E+00	1.3E+02	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T04-B	1	3.40E+00	U1/2		3.40E+00	5.5E+02	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T05-B	1	3.40E+00	U1/2		3.40E+00	1.9E+02	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T06-B	1	1.56E+01	E		1.56E+01	3.3E+01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T07-B	1	1.73E+01	E		1.73E+01	3.3E+01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T08-B	1	4.55E+02			4.55E+02	1.0E+00	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T09-B	1	5.89E+03			5.89E+03	5.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T10-B	1	1.36E+01	E		1.36E+01	1.2E+01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T01-C	1	5.23E+01			5.23E+01	1.4E+00	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T02-C	1	7.14E+00	E		7.14E+00	5.7E+01	6.8E+00	2.2E+01	10	100	1.17E+03	117%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T03-C	1	3.40E+00	U1/2		3.40E+00	2.9E+02	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T04-C	1	3.40E+00	U1/2		3.40E+00	4.4E+01	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T05-C	1	1.02E+01	E		1.02E+01	5.2E+01	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T06-C	1	1.44E+01	E		1.44E+01	3.5E+01	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T07-C	1	1.14E+01	E		1.14E+01	1.1E+02	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T08-C	1	7.08E+01			7.08E+01	7.8E+00	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-T09-C															
Pb	SWA-L04-1313-T10-C	1	1.74E+01	E		1.74E+01	1.6E+01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	6.4E+01	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	3.9E+02	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	1.6E+03	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-B01-B	1	3.40E+00	U1/2		3.40E+00	3.8E+01	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-B02-B	1	3.40E+00	U1/2		3.40E+00	2.7E+02	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-B03-B	1	3.40E+00	U1/2		3.40E+00	1.2E+03	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-B01-C	1	3.40E+00	U1/2		3.40E+00	1.0E+02	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-B02-C	1	3.40E+00	U1/2		3.40E+00	2.5E+02	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1313-B03-C	1	3.40E+00	U1/2		3.40E+00	2.3E+02	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	SWA-L04-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	2.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T02-A	1	2.87E+00	E		2.87E+00	6.1E+00	1.9E+00	6.0E+00	10	100	8.49E+02	85%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T03-A	1	1.95E+02			1.95E+02	4.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T04-A	1	5.84E+02			5.84E+02	3.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T05-A	1	8.26E+02			8.26E+02	2.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T06-A	1	1.03E+03			1.03E+03	3.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T07-A	1	8.50E+02			8.50E+02	6.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T08-A	1	5.26E+02			5.26E+02	5.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T09-A															
Li	SWA-L04-1313-T10-A	1	9.50E-01	U1/2		9.50E-01	3.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	3.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T02-B	1	2.24E+00	E		2.24E+00	6.1E+00	1.9E+00	6.0E+00	10	100	8.91E+02	89%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T03-B	1	1.89E+02			1.89E+02	6.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T04-B	1	6.07E+02			6.07E+02	3.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T05-B	1	7.40E+02			7.40E+02	4.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T06-B	1	8.78E+02			8.78E+02	9.2E-01	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T07-B	1	9.91E+02			9.91E+02	5.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T08-B	1	5.57E+02			5.57E+02	1.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T09-B	1	1.15E+03			1.15E+03	3.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T10-B	1	9.50E-01	U1/2		9.50E-01	1.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	7.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T02-C	1	3.90E+00	E		3.90E+00	3.2E+01	1.9E+00	6.0E+00	10	100	9.02E+02	90%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T03-C	1	1.68E+02			1.68E+02	7.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T04-C	1	5.29E+02			5.29E+02	1.0E+00	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T05-C	1	8.27E+02			8.27E+02	3.0E+00	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T06-C	1	9.06E+02			9.06E+02	4.3E+00	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T07-C	1	1.04E+03			1.04E+03	4.7E+00	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T08-C	1	5.75E+02			5.75E+02	1.9E+00	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-T09-C															
Li	SWA-L04-1313-T10-C	1	9.50E-01	U1/2		9.50E-01	2.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	1.5E+01	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	1.0E+01	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	1.7E+01	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-B01-B	1	9.50E-01	U1/2		9.50E-01	1.4E+01	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-B02-B	1	9.50E-01	U1/2		9.50E-01	3.9E+00	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-B03-B	1	9.50E-01	U1/2		9.50E-01	1.6E+01	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-B01-C	1	9.50E-01	U1/2		9.50E-01	1.3E+01	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-B02-C	1	9.50E-01	U1/2		9.50E-01	1.7E+01	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1313-B03-C	1	9.50E-01	U1/2		9.50E-01	7.2E+00	1.9E+00	6.0E+00					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	SWA-L04-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	4.1E+01	2.0E+00	6.4E+00	10	100	1.13E+03	113%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	4.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T04-A	1	4.08E+02			4.08E+02	6.5E-01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T05-A	1	7.49E+03			7.49E+03	3.1E-01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T06-A	1	1.76E+04			1.76E+04	1.8E-01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T07-A	1	2.18E+04			2.18E+04	2.3E-01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T08-A	1	1.47E+04			1.47E+04	1.8E-01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T09-A															
Mn	SWA-L04-1313-T10-A	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00	10	100	1.16E+03	116%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	3.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T04-B	1	1.02E+03			1.02E+03	1.5E-01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T05-B	1	2.95E+03			2.95E+03	9.1E-01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T06-B	1	8.60E+03			8.60E+03	2.5E-01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T07-B	1	2.22E+04			2.22E+04	7.2E-01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T08-B	1	1.48E+04			1.48E+04	1.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T09-B	1	2.98E+04			2.98E+04	7.2E-01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T10-B	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	1.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	6.1E+00	2.0E+00	6.4E+00	10	100	1.19E+03	119%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	3.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T04-C	1	6.60E+01			6.60E+01	2.8E-01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T05-C	1	6.00E+03			6.00E+03	6.7E-01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T06-C	1	1.08E+04			1.08E+04	5.9E-01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T07-C	1	2.21E+04			2.21E+04	1.1E+00	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T08-C	1	1.46E+04			1.46E+04	4.4E-01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-T09-C															
Mn	SWA-L04-1313-T10-C	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.6E+02	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	2.0E+02	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	4.5E+01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	4.6E+01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	3.6E+00	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	5.7E+01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1313-B03-C	1	1.00E+00	U1/2		1.00E+00	8.3E+00	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	SWA-L04-1313-T01-A	1	5.65E+00			5.65E+00	1.2E+02	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T02-A	1	9.18E+00			9.18E+00	1.2E+02	1.0E+00	3.2E+00	1000	100	1.16E+03	115%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T03-A	1	3.48E+04			3.48E+04	2.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T04-A	1	7.77E+05			7.77E+05	9.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T05-A	1	1.17E+06			1.17E+06	9.6E-02	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T06-A	1	1.51E+06			1.51E+06	6.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T07-A	1	1.21E+06			1.21E+06	7.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T08-A	1	7.20E+05			7.20E+05	5.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T09-A															
Mg	SWA-L04-1313-T10-A	1	1.25E+01			1.25E+01	1.6E+01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T01-B	1	1.22E+01			1.22E+01	3.5E+01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T02-B	1	2.65E+01			2.65E+01	2.8E+01	1.0E+00	3.2E+00	1000	100	1.19E+03	116%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T03-B	1	5.49E+04			5.49E+04	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T04-B	1	7.99E+05			7.99E+05	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T05-B	1	1.01E+06			1.01E+06	2.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T06-B	1	1.23E+06			1.23E+06	4.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T07-B	1	1.50E+06			1.50E+06	6.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T08-B	1	7.32E+05			7.32E+05	6.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T09-B	1	1.28E+06			1.28E+06	6.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T10-B	1	1.03E+01			1.03E+01	1.6E+02	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T01-C	1	1.36E+01			1.36E+01	2.2E+01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T02-C	1	1.37E+01			1.37E+01	5.4E+01	1.0E+00	3.2E+00	1000	100	1.18E+03	117%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T03-C	1	1.12E+04			1.12E+04	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T04-C	1	6.30E+05			6.30E+05	7.0E-01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T05-C	1	1.14E+06			1.14E+06	7.6E-01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T06-C	1	1.29E+06			1.29E+06	2.6E-01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T07-C	1	1.53E+06			1.53E+06	9.7E-01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T08-C	1	7.93E+05			7.93E+05	3.8E-01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-T09-C															
Mg	SWA-L04-1313-T10-C	1	8.14E+00			8.14E+00	9.5E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-B01-A	1	1.08E+00	E		1.08E+00	8.5E+02	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-B02-A	1	8.53E+00			8.53E+00	2.5E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-B03-A	1	2.57E+00	E		2.57E+00	1.6E+02	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-B01-B	1	1.63E+00	E		1.63E+00	5.6E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-B02-B	1	1.76E+00	E		1.76E+00	1.6E+02	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-B03-B	1	2.25E+00	E		2.25E+00	2.6E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	3.6E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-B02-C	1	1.48E+00	E		1.48E+00	1.1E+02	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	5.6E+02	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	SWA-L04-1313-T01-A	1	1.27E+02			1.27E+02	1.5E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T02-A	1	1.31E+02			1.31E+02	3.8E-01	1.2E+00	3.8E+00	10	100	1.25E+03	112%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T03-A	1	1.32E+02			1.32E+02	2.2E-01	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T04-A	1	1.34E+02			1.34E+02	2.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T05-A	1	1.01E+02			1.01E+02	1.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T06-A	1	3.69E+01			3.69E+01	6.9E-01	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T07-A	1	1.40E+01			1.40E+01	2.5E+01	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T08-A	1	5.84E+00			5.84E+00	9.5E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T09-A															
Mo	SWA-L04-1313-T10-A	1	1.21E+02			1.21E+02	1.6E-01	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T01-B	1	1.14E+02			1.14E+02	7.4E-01	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T02-B	1	1.24E+02			1.24E+02	5.9E-01	1.2E+00	3.8E+00	10	100	1.28E+03	115%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T03-B	1	1.27E+02			1.27E+02	1.2E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T04-B	1	1.38E+02			1.38E+02	9.8E-01	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T05-B	1	1.20E+02			1.20E+02	2.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T06-B	1	8.88E+01			8.88E+01	1.4E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T07-B	1	1.65E+01			1.65E+01	9.5E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T08-B	1	5.70E+00			5.70E+00	2.9E+01	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T09-B	1	8.97E+00			8.97E+00	2.3E+01	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T10-B	1	1.32E+02			1.32E+02	7.5E-01	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T01-C	1	1.12E+02			1.12E+02	1.2E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T02-C	1	1.34E+02			1.34E+02	2.2E+00	1.2E+00	3.8E+00	10	100	1.32E+03	119%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T03-C	1	1.40E+02			1.40E+02	1.2E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T04-C	1	1.43E+02			1.43E+02	9.4E-01	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T05-C	1	1.10E+02			1.10E+02	1.7E-01	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T06-C	1	6.68E+01			6.68E+01	5.9E-01	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T07-C	1	2.12E+01			2.12E+01	8.0E+00	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T08-C	1	8.94E+00			8.94E+00	2.6E+01	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-T09-C															
Mo	SWA-L04-1313-T10-C	1	1.34E+02			1.34E+02	1.3E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	3.2E+02	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-B02-A	1	3.64E+00	E		3.64E+00	3.5E+01	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-B03-A	1	6.00E-01	U1/2		6.00E-01	1.3E+02	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-B01-B	1	1.28E+00	E		1.28E+00	2.3E+01	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-B02-B	1	2.54E+00	E		2.54E+00	5.6E+01	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-B03-B	1	1.36E+00	E		1.36E+00	3.3E+01	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-B01-C	1	6.00E-01	U1/2		6.00E-01	1.7E+02	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-B02-C	1	1.87E+00	E		1.87E+00	5.0E+01	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1313-B03-C	1	6.00E-01	U1/2		6.00E-01	1.0E+02	1.2E+00	3.8E+00					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	SWA-L04-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	1.1E+03	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	1.2E+02	1.8E+00	5.7E+00	10	100	1.12E+03	111%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T03-A	1	4.17E+00	E		4.17E+00	3.5E+01	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T04-A	1	1.30E+01			1.30E+01	1.8E+01	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T05-A	1	7.07E+01			7.07E+01	2.3E+00	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T06-A	1	2.80E+02			2.80E+02	1.0E+00	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T07-A	1	4.44E+02			4.44E+02	9.5E-01	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T08-A	1	3.20E+02			3.20E+02	3.1E-01	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T09-A															
Ni	SWA-L04-1313-T10-A	1	9.00E-01	U1/2		9.00E-01	5.5E+01	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	6.5E+02	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	2.7E+02	1.8E+00	5.7E+00	10	100	1.16E+03	116%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T03-B	1	7.57E+00			7.57E+00	2.3E+01	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T04-B	1	1.09E+01			1.09E+01	1.6E+01	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T05-B	1	2.64E+01			2.64E+01	1.5E+00	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T06-B	1	9.14E+01			9.14E+01	3.4E+00	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T07-B	1	4.10E+02			4.10E+02	8.1E-01	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T08-B	1	3.23E+02			3.23E+02	1.3E+00	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T09-B	1	6.70E+02			6.70E+02	5.8E-01	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T10-B	1	9.00E-01	U1/2		9.00E-01	2.4E+02	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	1.2E+02	1.8E+00	5.7E+00	10	100	1.19E+03	119%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T03-C	1	2.95E+00	E		2.95E+00	1.1E+02	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T04-C	1	1.27E+01			1.27E+01	1.8E+01	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T05-C	1	5.24E+01			5.24E+01	3.0E+00	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T06-C	1	1.39E+02			1.39E+02	3.3E+00	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T07-C	1	3.99E+02			3.99E+02	9.1E-01	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T08-C	1	3.17E+02			3.17E+02	8.1E-02	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-T09-C															
Ni	SWA-L04-1313-T10-C	1	9.00E-01	U1/2		9.00E-01	7.1E+01	1.8E+00	5.7E+00			---		VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	7.2E+01	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	2.0E+02	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	1.1E+01	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-B01-B	1	9.00E-01	U1/2		9.00E-01	2.4E+02	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-B02-B	1	9.00E-01	U1/2		9.00E-01	5.1E+01	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-B03-B	1	9.00E-01	U1/2		9.00E-01	6.0E+02	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-B01-C	1	9.00E-01	U1/2		9.00E-01	4.6E+02	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-B02-C	1	9.00E-01	U1/2		9.00E-01	3.9E+02	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1313-B03-C	1	9.00E-01	U1/2		9.00E-01	7.4E+01	1.8E+00	5.7E+00					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	SWA-L04-1313-T01-A	1	1.24E+02			1.24E+02	6.0E+00	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T02-A	1	9.24E+01			9.24E+01	2.6E+02	3.7E+00	1.2E+01	1000	100	1.19E+03	110%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T03-A	1	1.85E+00	U1/2		1.85E+00	1.5E+02	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T04-A	1	6.23E+01			6.23E+01	3.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T05-A	1	4.56E+01			4.56E+01	4.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T06-A	1	2.83E+01			2.83E+01	5.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T07-A	1	1.09E+02			1.09E+02	7.7E+00	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T08-A	1	3.66E+02			3.66E+02	2.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T09-A															
P	SWA-L04-1313-T10-A	1	3.49E+01			3.49E+01	4.6E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T01-B	1	1.16E+02			1.16E+02	1.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T02-B	1	7.22E+01			7.22E+01	1.0E+02	3.7E+00	1.2E+01	1000	100	1.14E+03	107%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T03-B	1	1.85E+00	U1/2		1.85E+00	1.2E+02	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T04-B	1	8.40E+01			8.40E+01	1.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T05-B	1	5.01E+01			5.01E+01	9.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T06-B	1	6.65E+01			6.65E+01	5.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T07-B	1	2.15E+01			2.15E+01	2.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T08-B	1	5.34E+02			5.34E+02	3.7E+00	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T09-B	1	2.68E+03			2.68E+03	2.4E-02	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T10-B	1	4.37E+01			4.37E+01	1.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T01-C	1	1.17E+02			1.17E+02	5.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T02-C	1	6.14E+01			6.14E+01	5.9E+01	3.7E+00	1.2E+01	1000	100	1.18E+03	112%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T03-C	1	1.85E+00	U1/2		1.85E+00	5.7E+02	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T04-C	1	6.82E+01			6.82E+01	1.2E+01	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T05-C	1	4.26E+01			4.26E+01	4.2E+01	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T06-C	1	1.88E+01			1.88E+01	1.4E+02	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T07-C	1	2.11E+01			2.11E+01	1.3E+02	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T08-C	1	5.74E+02			5.74E+02	3.8E+00	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-T09-C															
P	SWA-L04-1313-T10-C	1	3.39E+01			3.39E+01	2.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	1.7E+02	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-B02-A	1	5.02E+00	E		5.02E+00	2.1E+02	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-B03-A	1	4.15E+00	E		4.15E+00	8.8E+01	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-B01-B	1	6.10E+00	E		6.10E+00	5.6E+01	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-B02-B	1	7.21E+00	E		7.21E+00	4.2E+01	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-B03-B	1	1.85E+00	U1/2		1.85E+00	8.4E+01	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-B01-C	1	1.10E+01	E		1.10E+01	9.3E+01	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-B02-C	1	5.25E+00	E		5.25E+00	4.3E+01	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1313-B03-C	1	1.85E+00	U1/2		1.85E+00	2.6E+01	3.7E+00	1.2E+01					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	SWA-L04-1313-T01-A	1	2.15E+06			2.15E+06	6.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T02-A	1	3.16E+05			3.16E+05	2.2E-01	1.6E+00	5.1E+00	1000	100	3.17E+05	95%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T03-A	1	4.09E+05			4.09E+05	7.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T04-A	1	4.23E+05			4.23E+05	2.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T05-A	1	4.32E+05			4.32E+05	4.4E-02	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T06-A	1	4.70E+05			4.70E+05	2.5E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T07-A	1	3.45E+05			3.45E+05	6.5E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T08-A	1	2.07E+05			2.07E+05	2.9E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T09-A															
K	SWA-L04-1313-T10-A	1	2.80E+05			2.80E+05	6.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T01-B	1	2.17E+06			2.17E+06	1.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T02-B	1	3.03E+05			3.03E+05	4.7E-01	1.6E+00	5.1E+00	1000	100	3.04E+05	91%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T03-B	1	4.02E+05			4.02E+05	9.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T04-B	1	4.14E+05			4.14E+05	6.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T05-B	1	4.24E+05			4.24E+05	2.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T06-B	1	4.47E+05			4.47E+05	2.6E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T07-B	1	4.65E+05			4.65E+05	6.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T08-B	1	2.15E+05			2.15E+05	4.5E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T09-B	1	6.23E+05			6.23E+05	1.4E+01	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T10-B	1	2.85E+05			2.85E+05	7.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T01-C	1	2.14E+06			2.14E+06	6.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T02-C	1	3.13E+05			3.13E+05	5.8E-01	1.6E+00	5.1E+00	1000	100	3.14E+05	87%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T03-C	1	4.10E+05			4.10E+05	1.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T04-C	1	4.20E+05			4.20E+05	2.8E+00	1.6E+00	5.1E+00					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T05-C	1	4.25E+05			4.25E+05	9.1E-01	1.6E+00	5.1E+00					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T06-C	1	4.39E+05			4.39E+05	1.4E-01	1.6E+00	5.1E+00					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T07-C	1	4.81E+05			4.81E+05	3.7E+00	1.6E+00	5.1E+00					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T08-C	1	2.35E+05			2.35E+05	4.7E+00	1.6E+00	5.1E+00					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-T09-C															
K	SWA-L04-1313-T10-C	1	2.88E+05			2.88E+05	9.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-B01-A	1	2.91E+01			2.91E+01	7.0E+00	1.6E+00	5.1E+00					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-B02-A	1	5.36E+01			5.36E+01	4.7E+00	1.6E+00	5.1E+00					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-B03-A	1	2.03E+06			2.03E+06	9.7E-02	1.6E+00	5.1E+00					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-B01-B	1	6.73E+01			6.73E+01	7.2E-01	1.6E+00	5.1E+00					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-B02-B	1	2.93E+01			2.93E+01	8.0E+00	1.6E+00	5.1E+00					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-B03-B	1	2.03E+06			2.03E+06	5.5E-01	1.6E+00	5.1E+00					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-B01-C	1	5.39E+01			5.39E+01	1.1E+01	1.6E+00	5.1E+00					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-B02-C	1	3.83E+01			3.83E+01	3.1E+00	1.6E+00	5.1E+00					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1313-B03-C	1	2.02E+06			2.02E+06	6.5E-01	1.6E+00	5.1E+00					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	SWA-L04-1313-T01-A	1	8.84E+04			8.84E+04	2.6E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T02-A	1	8.67E+04			8.67E+04	4.4E-01	1.5E+01	4.8E+01	10	100	8.76E+04	91%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T03-A	1	9.65E+04			9.65E+04	5.7E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T04-A	1	1.13E+05			1.13E+05	8.0E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T05-A	1	1.16E+05			1.16E+05	3.1E-02	1.5E+01	4.8E+01			---		VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T06-A	1	1.22E+05			1.22E+05	1.7E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T07-A	1	7.60E+04			7.60E+04	4.8E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T08-A	1	4.03E+04			4.03E+04	3.6E-02	1.5E+01	4.8E+01			---		VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T09-A															
Se	SWA-L04-1313-T10-A	1	8.22E+04			8.22E+04	8.4E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T01-B	1	7.56E+04			7.56E+04	9.9E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T02-B	1	8.60E+04			8.60E+04	1.1E-01	1.5E+01	4.8E+01	10	100	8.69E+04	87%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T03-B	1	9.70E+04			9.70E+04	9.3E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T04-B	1	1.10E+05			1.10E+05	5.8E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T05-B	1	1.16E+05			1.16E+05	6.3E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T06-B	1	1.20E+05			1.20E+05	7.0E-02	1.5E+01	4.8E+01			---		VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T07-B	1	1.14E+05			1.14E+05	1.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T08-B	1	4.16E+04			4.16E+04	6.3E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T09-B	1	6.28E+04			6.28E+04	6.4E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T10-B	1	9.21E+04			9.21E+04	3.0E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T01-C	1	7.75E+04			7.75E+04	1.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T02-C	1	9.81E+04			9.81E+04	9.0E-01	1.5E+01	4.8E+01	10	100	9.90E+04	90%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T03-C	1	9.98E+04			9.98E+04	6.7E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T04-C	1	1.15E+05			1.15E+05	6.6E-01	1.5E+01	4.8E+01					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T05-C	1	1.18E+05			1.18E+05	7.8E-01	1.5E+01	4.8E+01					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T06-C	1	1.21E+05			1.21E+05	7.4E-01	1.5E+01	4.8E+01					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T07-C	1	1.19E+05			1.19E+05	1.5E+00	1.5E+01	4.8E+01					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T08-C	1	4.91E+04			4.91E+04	4.7E-01	1.5E+01	4.8E+01					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-T09-C															
Se	SWA-L04-1313-T10-C	1	9.25E+04			9.25E+04	9.3E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-B01-A	1	7.50E+00	U1/2		7.50E+00	8.3E+02	1.5E+01	4.8E+01					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-B02-A	1	7.50E+00	U1/2		7.50E+00	1.2E+02	1.5E+01	4.8E+01					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-B03-A	1	7.50E+00	U1/2		7.50E+00	1.7E+02	1.5E+01	4.8E+01					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-B01-B	1	7.50E+00	U1/2		7.50E+00	3.5E+01	1.5E+01	4.8E+01					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-B02-B	1	7.50E+00	U1/2		7.50E+00	6.5E+01	1.5E+01	4.8E+01					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-B03-B	1	7.50E+00	U1/2		7.50E+00	3.8E+01	1.5E+01	4.8E+01					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-B01-C	1	7.50E+00	U1/2		7.50E+00	3.4E+03	1.5E+01	4.8E+01					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-B02-C	1	7.50E+00	U1/2		7.50E+00	1.1E+02	1.5E+01	4.8E+01					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1313-B03-C	1	7.50E+00	U1/2		7.50E+00	2.9E+02	1.5E+01	4.8E+01					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	SWA-L04-1313-T01-A	1	3.97E+04			3.97E+04	8.4E-01	1.1E+00	3.5E+00			---		VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T02-A	1	1.87E+04			1.87E+04	8.0E-01	1.1E+00	3.5E+00	1000	100	1.97E+04	100%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T03-A	1	5.29E+03			5.29E+03	5.2E-01	1.1E+00	3.5E+00			---		VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T04-A	1	4.48E+03			4.48E+03	9.5E-01	1.1E+00	3.5E+00			---		VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T05-A	1	5.28E+03			5.28E+03	7.5E-01	1.1E+00	3.5E+00			---		VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T06-A	1	8.00E+03			8.00E+03	2.7E-01	1.1E+00	3.5E+00			---		VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T07-A	1	8.63E+03			8.63E+03	2.4E-01	1.1E+00	3.5E+00			---		VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T08-A	1	1.74E+04			1.74E+04	3.2E-01	1.1E+00	3.5E+00			---		VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T09-A															
Si	SWA-L04-1313-T10-A	1	2.49E+04			2.49E+04	6.0E-01	1.1E+00	3.5E+00			---		VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T01-B	1	3.65E+04			3.65E+04	1.9E+00	1.1E+00	3.5E+00			---		VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T02-B	1	1.97E+04			1.97E+04	4.6E-01	1.1E+00	3.5E+00	1000	100	2.06E+04	87%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T03-B	1	5.07E+03			5.07E+03	8.1E-01	1.1E+00	3.5E+00			---		VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T04-B	1	4.89E+03			4.89E+03	3.6E-01	1.1E+00	3.5E+00			---		VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T05-B	1	4.49E+03			4.49E+03	7.3E-01	1.1E+00	3.5E+00			---		VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T06-B	1	5.66E+03			5.66E+03	3.1E-01	1.1E+00	3.5E+00			---		VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T07-B	1	8.54E+03			8.54E+03	9.1E-01	1.1E+00	3.5E+00			---		VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T08-B	1	2.55E+04			2.55E+04	5.8E-01	1.1E+00	3.5E+00			---		VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T09-B	1	4.95E+04			4.95E+04	5.5E-01	1.1E+00	3.5E+00			---		VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T10-B	1	2.75E+04			2.75E+04	1.1E+00	1.1E+00	3.5E+00			---		VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T01-C	1	3.71E+04			3.71E+04	2.9E-01	1.1E+00	3.5E+00			---		VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T02-C	1	2.22E+04			2.22E+04	5.7E-01	1.1E+00	3.5E+00	1000	100	2.31E+04	93%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T03-C	1	6.18E+03			6.18E+03	5.5E-01	1.1E+00	3.5E+00			---		VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T04-C	1	4.97E+03			4.97E+03	3.5E-01	1.1E+00	3.5E+00					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T05-C	1	5.05E+03			5.05E+03	6.3E-01	1.1E+00	3.5E+00					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T06-C	1	6.72E+03			6.72E+03	7.2E-01	1.1E+00	3.5E+00					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T07-C	1	7.78E+03			7.78E+03	5.8E-01	1.1E+00	3.5E+00					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T08-C	1	2.44E+04			2.44E+04	4.3E-01	1.1E+00	3.5E+00					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-T09-C															
Si	SWA-L04-1313-T10-C	1	2.78E+04			2.78E+04	1.2E+00	1.1E+00	3.5E+00			---		VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-B01-A	1	3.21E+00	E		3.21E+00	9.0E+01	1.1E+00	3.5E+00					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-B02-A	1	1.61E+01			1.61E+01	4.3E+00	1.1E+00	3.5E+00					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-B03-A	1	3.15E+01			3.15E+01	5.4E+00	1.1E+00	3.5E+00					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-B01-B	1	1.98E+01			1.98E+01	2.2E+01	1.1E+00	3.5E+00					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-B02-B	1	1.36E+01			1.36E+01	4.7E+01	1.1E+00	3.5E+00					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-B03-B	1	4.50E+01			4.50E+01	2.5E+00	1.1E+00	3.5E+00					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-B01-C	1	3.94E+01			3.94E+01	6.0E+00	1.1E+00	3.5E+00					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-B02-C	1	1.11E+01			1.11E+01	5.3E+00	1.1E+00	3.5E+00					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1313-B03-C	1	2.33E+01			2.33E+01	2.7E+00	1.1E+00	3.5E+00					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	SWA-L04-1313-T01-A	1	4.02E+05			4.02E+05	1.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T02-A	1	4.21E+05			4.21E+05	5.4E-01	2.5E+00	8.0E+00	1000	100	4.22E+05	83%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T03-A	1	4.30E+05			4.30E+05	1.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T04-A	1	4.13E+05			4.13E+05	2.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T05-A	1	4.07E+05			4.07E+05	8.4E-02	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T06-A	1	4.02E+05			4.02E+05	5.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T07-A	1	4.02E+05			4.02E+05	3.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T08-A	1	4.02E+05			4.02E+05	5.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T09-A															
Na	SWA-L04-1313-T10-A	1	3.95E+05			3.95E+05	1.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T01-B	1	3.94E+05			3.94E+05	3.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T02-B	1	4.14E+05			4.14E+05	2.7E-01	2.5E+00	8.0E+00	1000	100	4.15E+05	87%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T03-B	1	4.23E+05			4.23E+05	1.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T04-B	1	4.11E+05			4.11E+05	5.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T05-B	1	4.09E+05			4.09E+05	5.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T06-B	1	4.06E+05			4.06E+05	1.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T07-B	1	3.98E+05			3.98E+05	2.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T08-B	1	3.97E+05			3.97E+05	6.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T09-B	1	7.88E+05			7.88E+05	1.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T10-B	1	3.97E+05			3.97E+05	9.1E-02	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T01-C	1	3.95E+05			3.95E+05	3.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T02-C	1	4.23E+05			4.23E+05	1.0E-01	2.5E+00	8.0E+00	1000	100	4.24E+05	92%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T03-C	1	4.28E+05			4.28E+05	6.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T04-C	1	4.15E+05			4.15E+05	8.8E-01	2.5E+00	8.0E+00					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T05-C	1	4.03E+05			4.03E+05	2.4E-01	2.5E+00	8.0E+00					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T06-C	1	4.01E+05			4.01E+05	2.0E-01	2.5E+00	8.0E+00					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T07-C	1	3.99E+05			3.99E+05	3.7E-01	2.5E+00	8.0E+00					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T08-C	1	3.97E+05			3.97E+05	9.6E-01	2.5E+00	8.0E+00					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-T09-C															
Na	SWA-L04-1313-T10-C	1	4.00E+05			4.00E+05	3.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-B01-A	1	5.79E+00	E		5.79E+00	3.9E+01	2.5E+00	8.0E+00					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-B02-A	1	7.61E+00	E		7.61E+00	2.7E+01	2.5E+00	8.0E+00					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-B03-A	1	5.61E+02			5.61E+02	2.4E-01	2.5E+00	8.0E+00					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-B01-B	1	3.96E+00	E		3.96E+00	1.4E+00	2.5E+00	8.0E+00					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-B02-B	1	6.57E+00	E		6.57E+00	4.9E+01	2.5E+00	8.0E+00					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-B03-B	1	5.59E+02			5.59E+02	6.6E-01	2.5E+00	8.0E+00					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-B01-C	1	6.36E+00	E		6.36E+00	1.8E+01	2.5E+00	8.0E+00					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-B02-C	1	2.96E+00	E		2.96E+00	9.1E+01	2.5E+00	8.0E+00					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1313-B03-C	1	5.77E+02			5.77E+02	4.1E-01	2.5E+00	8.0E+00					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	SWA-L04-1313-T01-A	1	3.01E+02			3.01E+02	3.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T02-A	1	8.07E+02			8.07E+02	1.2E+00	1.0E+00	3.2E+00	1000	100	1.88E+03	108%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T03-A	1	2.05E+04			2.05E+04	3.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T04-A	1	3.33E+04			3.33E+04	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T05-A	1	4.11E+04			4.11E+04	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T06-A	1	4.99E+04			4.99E+04	6.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T07-A	1	3.86E+04			3.86E+04	1.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T08-A	1	2.30E+04			2.30E+04	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T09-A															
Sr	SWA-L04-1313-T10-A	1	3.28E+02			3.28E+02	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T01-B	1	3.06E+02			3.06E+02	8.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T02-B	1	7.57E+02			7.57E+02	2.8E-01	1.0E+00	3.2E+00	1000	100	1.86E+03	110%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T03-B	1	2.00E+04			2.00E+04	6.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T04-B	1	3.43E+04			3.43E+04	5.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T05-B	1	3.69E+04			3.69E+04	9.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T06-B	1	4.35E+04			4.35E+04	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T07-B	1	5.13E+04			5.13E+04	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T08-B	1	2.36E+04			2.36E+04	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T09-B	1	4.09E+04			4.09E+04	5.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T10-B	1	2.99E+02			2.99E+02	5.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T01-C	1	3.09E+02			3.09E+02	9.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T02-C	1	6.58E+02			6.58E+02	1.2E+00	1.0E+00	3.2E+00	1000	100	1.79E+03	114%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T03-C	1	1.90E+04			1.90E+04	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T04-C	1	3.14E+04			3.14E+04	9.9E-01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T05-C	1	4.14E+04			4.14E+04	9.9E-01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T06-C	1	4.47E+04			4.47E+04	1.6E-01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T07-C	1	5.15E+04			5.15E+04	6.9E-01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T08-C	1	2.61E+04			2.61E+04	6.6E-01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-T09-C															
Sr	SWA-L04-1313-T10-C	1	3.03E+02			3.03E+02	1.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	3.0E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.3E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	5.9E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-B01-B	1	1.33E+00	E		1.33E+00	1.7E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	8.5E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-B03-B	1	3.63E+00			3.63E+00	1.3E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	2.3E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	4.3E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	2.0E+03	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	SWA-L04-1313-T01-A	1	3.54E+05			3.54E+05	4.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T02-A	1	2.98E+05			2.98E+05	6.4E-02	6.8E+00	2.2E+01	1000	100	2.99E+05	89%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T03-A	1	3.31E+05			3.31E+05	3.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T04-A	1	4.24E+05			4.24E+05	7.7E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T05-A	1	4.65E+05			4.65E+05	4.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T06-A	1	5.14E+05			5.14E+05	3.3E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T07-A	1	3.48E+05			3.48E+05	6.7E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T08-A	1	1.94E+05			1.94E+05	6.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T09-A															
S	SWA-L04-1313-T10-A	1	3.62E+05			3.62E+05	9.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T01-B	1	3.30E+05			3.30E+05	1.1E+00	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T02-B	1	3.16E+05			3.16E+05	5.1E-01	6.8E+00	2.2E+01	1000	100	3.17E+05	100%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T03-B	1	3.44E+05			3.44E+05	4.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T04-B	1	4.17E+05			4.17E+05	5.7E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T05-B	1	4.61E+05			4.61E+05	3.7E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T06-B	1	4.84E+05			4.84E+05	4.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T07-B	1	4.91E+05			4.91E+05	1.1E+00	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T08-B	1	2.01E+05			2.01E+05	5.8E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T09-B	1	3.18E+05			3.18E+05	4.9E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T10-B	1	3.46E+05			3.46E+05	7.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T01-C	1	3.81E+05			3.81E+05	5.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T02-C	1	3.71E+05			3.71E+05	7.4E-01	6.8E+00	2.2E+01	1000	100	3.72E+05	101%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T03-C	1	3.62E+05			3.62E+05	5.9E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T04-C	1	4.35E+05			4.35E+05	3.8E-01	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T05-C	1	4.75E+05			4.75E+05	8.5E-01	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T06-C	1	4.94E+05			4.94E+05	5.7E-01	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T07-C	1	5.06E+05			5.06E+05	1.3E+00	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T08-C	1	2.28E+05			2.28E+05	4.3E-01	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-T09-C															
S	SWA-L04-1313-T10-C	1	3.51E+05			3.51E+05	2.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	3.9E+00	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	3.2E+00	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-B03-A	1	2.32E+02			2.32E+02	5.3E-01	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-B01-B	1	3.40E+00	U1/2		3.40E+00	1.2E+01	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-B02-B	1	3.40E+00	U1/2		3.40E+00	1.1E+01	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-B03-B	1	2.44E+02			2.44E+02	4.3E+00	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-B01-C	1	3.40E+00	U1/2		3.40E+00	3.3E-01	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-B02-C	1	3.40E+00	U1/2		3.40E+00	1.9E+00	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1313-B03-C	1	3.40E+00	U1/2		3.40E+00	7.4E+00	6.8E+00	2.2E+01					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	SWA-L04-1313-T01-A	1	2.30E+00	U1/2		2.30E+00	4.4E+01	4.6E+00	1.5E+01			---		VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T02-A	1	2.30E+00	U1/2		2.30E+00	1.9E+02	4.6E+00	1.5E+01	10	100	1.02E+03	102%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T03-A	1	2.30E+00	U1/2		2.30E+00	3.3E+02	4.6E+00	1.5E+01			---		VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T04-A	1	2.30E+00	U1/2		2.30E+00	1.6E+02	4.6E+00	1.5E+01			---		VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T05-A	1	8.45E+00	E		8.45E+00	5.8E+01	4.6E+00	1.5E+01			---		VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T06-A	1	1.53E+01			1.53E+01	4.4E+01	4.6E+00	1.5E+01			---		VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T07-A	1	2.09E+01			2.09E+01	7.1E+01	4.6E+00	1.5E+01			---		VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T08-A	1	1.14E+01	E		1.14E+01	4.3E+01	4.6E+00	1.5E+01			---		VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T09-A															
Tl	SWA-L04-1313-T10-A	1	2.30E+00	U1/2		2.30E+00	9.8E+01	4.6E+00	1.5E+01			---		VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T01-B	1	2.30E+00	U1/2		2.30E+00	6.1E+02	4.6E+00	1.5E+01			---		VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T02-B	1	2.30E+00	U1/2		2.30E+00	1.7E+03	4.6E+00	1.5E+01	10	100	1.06E+03	105%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T03-B	1	2.30E+00	U1/2		2.30E+00	8.1E+01	4.6E+00	1.5E+01			---		VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T04-B	1	2.30E+00	U1/2		2.30E+00	1.1E+02	4.6E+00	1.5E+01			---		VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T05-B	1	8.16E+00	E		8.16E+00	9.2E+01	4.6E+00	1.5E+01			---		VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T06-B	1	6.83E+00	E		6.83E+00	9.7E+01	4.6E+00	1.5E+01			---		VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T07-B	1	3.01E+01			3.01E+01	1.5E+01	4.6E+00	1.5E+01			---		VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T08-B	1	7.99E+00	E		7.99E+00	5.0E+01	4.6E+00	1.5E+01			---		VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T09-B	1	2.68E+01			2.68E+01	2.3E+01	4.6E+00	1.5E+01			---		VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T10-B	1	2.30E+00	U1/2		2.30E+00	2.4E+02	4.6E+00	1.5E+01			---		VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T01-C	1	2.30E+00	U1/2		2.30E+00	1.7E+02	4.6E+00	1.5E+01			---		VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T02-C	1	2.30E+00	U1/2		2.30E+00	2.8E+01	4.6E+00	1.5E+01	10	100	1.08E+03	108%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T03-C	1	2.30E+00	U1/2		2.30E+00	7.8E+02	4.6E+00	1.5E+01			---		VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T04-C	1	2.30E+00	U1/2		2.30E+00	6.4E+02	4.6E+00	1.5E+01					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T05-C	1	8.41E+00	E		8.41E+00	1.0E+02	4.6E+00	1.5E+01					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T06-C	1	1.23E+01	E		1.23E+01	5.4E+01	4.6E+00	1.5E+01					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T07-C	1	2.56E+01			2.56E+01	3.9E+01	4.6E+00	1.5E+01					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T08-C	1	1.27E+01	E		1.27E+01	6.3E+01	4.6E+00	1.5E+01					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-T09-C															
Tl	SWA-L04-1313-T10-C	1	2.30E+00	U1/2		2.30E+00	3.8E+03	4.6E+00	1.5E+01			---		VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	3.5E+01	4.6E+00	1.5E+01					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	7.2E+01	4.6E+00	1.5E+01					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	4.1E+01	4.6E+00	1.5E+01					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-B01-B	1	2.30E+00	U1/2		2.30E+00	3.0E+01	4.6E+00	1.5E+01					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-B02-B	1	2.30E+00	U1/2		2.30E+00	2.8E+01	4.6E+00	1.5E+01					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-B03-B	1	2.30E+00	U1/2		2.30E+00	3.3E+01	4.6E+00	1.5E+01					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-B01-C	1	2.30E+00	U1/2		2.30E+00	5.3E+02	4.6E+00	1.5E+01					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-B02-C	1	2.30E+00	U1/2		2.30E+00	6.6E+01	4.6E+00	1.5E+01					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1313-B03-C	1	2.30E+00	U1/2		2.30E+00	1.1E+02	4.6E+00	1.5E+01					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	SWA-L04-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	3.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	2.8E+01	2.0E+00	6.4E+00	10	100	1.14E+03	114%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	3.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	5.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	2.9E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	7.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T07-A	1	2.93E+00	E		2.93E+00	6.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T08-A	1	1.02E+01			1.02E+01	2.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T09-A															
Ti	SWA-L04-1313-T10-A	1	1.00E+00	U1/2		1.00E+00	6.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	6.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	6.4E+01	2.0E+00	6.4E+00	10	100	1.16E+03	116%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	4.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	3.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	4.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T08-B	1	1.96E+01			1.96E+01	4.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T09-B	1	4.67E+02			4.67E+02	4.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T10-B	1	1.00E+00	U1/2		1.00E+00	3.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	3.6E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	5.4E+01	2.0E+00	6.4E+00	10	100	1.19E+03	119%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	8.0E+02	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	5.9E+01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T08-C	1	2.41E+01			2.41E+01	1.1E+00	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-T09-C															
Ti	SWA-L04-1313-T10-C	1	1.00E+00	U1/2		1.00E+00	4.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	6.2E+01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	1.3E+01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	6.3E+01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	9.5E+01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	3.1E+01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1313-B03-C	1	1.00E+00	U1/2		1.00E+00	8.0E+01	2.0E+00	6.4E+00					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	SWA-L04-1313-T01-A	1	4.69E+02			4.69E+02	9.4E-01	1.5E+00	4.8E+00			---		VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T02-A	1	1.81E+02			1.81E+02	8.4E-01	1.5E+00	4.8E+00	10	100	1.31E+03	113%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T03-A	1	1.54E+02			1.54E+02	1.5E+00	1.5E+00	4.8E+00			---		VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T04-A	1	2.39E+02			2.39E+02	1.5E+00	1.5E+00	4.8E+00			---		VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T05-A	1	2.13E+02			2.13E+02	7.1E-01	1.5E+00	4.8E+00			---		VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T06-A	1	2.36E+02			2.36E+02	1.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T07-A	1	1.35E+02			1.35E+02	5.2E-01	1.5E+00	4.8E+00			---		VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T08-A	1	8.33E+01			8.33E+01	2.6E-01	1.5E+00	4.8E+00			---		VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T09-A															
V	SWA-L04-1313-T10-A	1	3.12E+02			3.12E+02	5.9E-01	1.5E+00	4.8E+00			---		VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T01-B	1	4.00E+02			4.00E+02	1.7E+00	1.5E+00	4.8E+00			---		VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T02-B	1	1.89E+02			1.89E+02	1.3E-01	1.5E+00	4.8E+00	10	100	1.35E+03	116%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T03-B	1	1.53E+02			1.53E+02	4.5E-01	1.5E+00	4.8E+00			---		VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T04-B	1	2.17E+02			2.17E+02	7.5E-01	1.5E+00	4.8E+00			---		VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T05-B	1	2.14E+02			2.14E+02	2.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T06-B	1	2.21E+02			2.21E+02	4.4E-01	1.5E+00	4.8E+00			---		VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T07-B	1	2.11E+02			2.11E+02	2.7E+00	1.5E+00	4.8E+00			---		VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T08-B	1	8.46E+01			8.46E+01	1.7E+00	1.5E+00	4.8E+00			---		VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T09-B	1	1.08E+03			1.08E+03	4.7E-01	1.5E+00	4.8E+00			---		VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T10-B	1	3.75E+02			3.75E+02	9.5E-01	1.5E+00	4.8E+00			---		VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T01-C	1	4.05E+02			4.05E+02	2.9E-01	1.5E+00	4.8E+00			---		VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T02-C	1	2.47E+02			2.47E+02	1.9E+00	1.5E+00	4.8E+00	10	100	1.43E+03	118%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T03-C	1	1.51E+02			1.51E+02	2.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T04-C	1	2.30E+02			2.30E+02	9.1E-01	1.5E+00	4.8E+00					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T05-C	1	2.15E+02			2.15E+02	9.7E-01	1.5E+00	4.8E+00					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T06-C	1	2.19E+02			2.19E+02	3.3E-01	1.5E+00	4.8E+00					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T07-C	1	2.14E+02			2.14E+02	1.7E+00	1.5E+00	4.8E+00					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T08-C	1	8.66E+01			8.66E+01	1.6E+00	1.5E+00	4.8E+00					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-T09-C															
V	SWA-L04-1313-T10-C	1	3.77E+02			3.77E+02	8.3E-01	1.5E+00	4.8E+00			---		VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-B01-A	1	7.50E-01	U1/2		7.50E-01	1.8E+01	1.5E+00	4.8E+00					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-B02-A	1	7.50E-01	U1/2		7.50E-01	1.7E+03	1.5E+00	4.8E+00					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-B03-A	1	7.50E-01	U1/2		7.50E-01	2.8E+02	1.5E+00	4.8E+00					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-B01-B	1	7.50E-01	U1/2		7.50E-01	4.7E+01	1.5E+00	4.8E+00					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-B02-B	1	7.50E-01	U1/2		7.50E-01	3.2E+02	1.5E+00	4.8E+00					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-B03-B	1	7.50E-01	U1/2		7.50E-01	1.5E+02	1.5E+00	4.8E+00					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-B01-C	1	7.50E-01	U1/2		7.50E-01	1.7E+01	1.5E+00	4.8E+00					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-B02-C	1	7.50E-01	U1/2		7.50E-01	1.5E+02	1.5E+00	4.8E+00					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1313-B03-C	1	7.50E-01	U1/2		7.50E-01	5.2E+02	1.5E+00	4.8E+00					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	SWA-L04-1313-T01-A	1	5.25E+00			5.25E+00	1.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 1:21 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T02-A	1	3.53E+00			3.53E+00	6.0E+00	1.0E+00	3.2E+00	10	100	1.01E+03	101%	VU ICP-OES	3/21/11 1:23 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T03-A	1	2.63E+00	E		2.63E+00	2.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 1:25 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T04-A	1	3.15E+00	E		3.15E+00	1.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 1:26 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T05-A	1	6.43E+00			6.43E+00	9.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 1:28 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T06-A	1	9.22E+01			9.22E+01	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 1:30 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T07-A	1	6.70E+02			6.70E+02	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 1:31 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T08-A	1	1.41E+03			1.41E+03	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 1:33 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T09-A															
Zn	SWA-L04-1313-T10-A	1	2.25E+00	E		2.25E+00	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 3:04 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T01-B	1	3.30E+00			3.30E+00	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:03 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T02-B	1	2.27E+00	E		2.27E+00	1.4E+01	1.0E+00	3.2E+00	10	100	1.05E+03	105%	VU ICP-OES	3/21/11 2:05 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T03-B	1	2.74E+00	E		2.74E+00	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:06 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T04-B	1	3.16E+00	E		3.16E+00	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:08 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T05-B	1	3.82E+00			3.82E+00	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:10 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T06-B	1	7.23E+00			7.23E+00	7.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:11 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T07-B	1	4.75E+02			4.75E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:13 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T08-B	1	1.37E+03			1.37E+03	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:15 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T09-B	1	3.72E+03			3.72E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:16 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T10-B	1	2.50E+00	E		2.50E+00	6.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 3:06 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T01-C	1	3.98E+00			3.98E+00	9.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:18 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T02-C	1	2.50E+00	E		2.50E+00	1.8E+01	1.0E+00	3.2E+00	10	100	1.09E+03	109%	VU ICP-OES	3/21/11 2:19 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T03-C	1	2.76E+00	E		2.76E+00	6.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:21 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T04-C	1	3.07E+00	E		3.07E+00	6.0E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:23 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T05-C	1	4.22E+00			4.22E+00	7.3E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:24 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T06-C	1	1.43E+01			1.43E+01	2.4E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:26 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T07-C	1	3.64E+02			3.64E+02	2.6E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:28 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T08-C	1	1.08E+03			1.08E+03	9.2E-01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 2:29 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-T09-C															
Zn	SWA-L04-1313-T10-C	1	2.80E+00	E		2.80E+00	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 3:07 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-B01-A	1	2.81E+00	E		2.81E+00	3.2E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 12:58 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-B02-A	1	2.84E+00	E		2.84E+00	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:00 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-B03-A	1	3.19E+00			3.19E+00	8.4E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:02 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-B01-B	1	1.18E+00	E		1.18E+00	6.1E-01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:11 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-B02-B	1	2.24E+00	E		2.24E+00	4.6E-01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:13 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-B03-B	1	3.08E+00	E		3.08E+00	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:15 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-B01-C	1	2.49E+00	E		2.49E+00	1.6E+00	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:16 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-B02-C	1	2.73E+00	E		2.73E+00	8.4E-01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:18 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1313-B03-C	1	2.81E+00	E		2.81E+00	9.5E-01	1.0E+00	3.2E+00					VU ICP-OES	3/21/11 1:20 PM	EPA Interlab L04 1313-1316 SWA

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	SWA-L05-1313-T01-A	1	5.66E+04			5.66E+04	4.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T02-A	1	2.84E+04			2.84E+04	9.3E-01	1.0E+00	3.2E+00	1000	100	2.94E+04	92%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T03-A	1	1.88E+02			1.88E+02	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T04-A	1	1.98E+01			1.98E+01	4.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T05-A	1	3.33E+04			3.33E+04	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T06-A	1	2.87E+04			2.87E+04	2.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T07-A	1	9.15E+00			9.15E+00	6.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T08-A	1	8.47E+03			8.47E+03	1.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T09-A	1	1.00E+06			1.00E+06	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T01-B	1	5.89E+04			5.89E+04	1.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T02-B	1	2.87E+04			2.87E+04	9.8E-01	1.0E+00	3.2E+00	1000	100	2.97E+04	99%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T03-B	1	1.40E+02			1.40E+02	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T04-B	1	2.04E+01			2.04E+01	4.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T05-B	1	3.39E+04			3.39E+04	6.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T06-B	1	2.80E+04			2.80E+04	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T07-B	1	5.00E-01	U1/2		5.00E-01	7.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T08-B	1	4.45E+05			4.45E+05	9.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T09-B	1	7.97E+05			7.97E+05	2.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T01-C	1	5.59E+04			5.59E+04	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T02-C	1	2.83E+04			2.83E+04	2.2E+00	1.0E+00	3.2E+00	1000	100	2.92E+04	96%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T03-C	1	1.78E+02			1.78E+02	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T04-C	1	2.14E+01			2.14E+01	5.6E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T05-C	1	3.30E+04			3.30E+04	5.3E-01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T06-C	1	2.85E+04			2.85E+04	2.9E-01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T07-C	1	5.00E-01	U1/2		5.00E-01	7.2E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T08-C	1	4.38E+05			4.38E+05	2.0E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-T09-C	1	6.70E+05			6.70E+05	6.3E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	3.6E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	2.5E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	4.2E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	7.3E-01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	1.6E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	1.4E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	3.4E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	4.9E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	9.4E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	SWA-L05-1313-T01-A	1	6.34E+03			6.34E+03	6.2E-01	7.5E+00	2.4E+01			---		VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T02-A	1	5.70E+03			5.70E+03	5.5E-01	7.5E+00	2.4E+01	10	100	6.71E+03	101%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T03-A	1	1.42E+03			1.42E+03	1.4E+00	7.5E+00	2.4E+01			---		VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T04-A	1	1.12E+03			1.12E+03	6.3E-01	7.5E+00	2.4E+01			---		VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T05-A	1	6.17E+03			6.17E+03	1.2E+00	7.5E+00	2.4E+01			---		VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T06-A	1	5.77E+03			5.77E+03	3.6E-01	7.5E+00	2.4E+01			---		VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T07-A	1	1.16E+03			1.16E+03	2.5E+00	7.5E+00	2.4E+01			---		VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T08-A	1	4.12E+02			4.12E+02	4.8E+00	7.5E+00	2.4E+01			---		VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T09-A	1	4.67E+04			4.67E+04	5.7E+00	7.5E+00	2.4E+01					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T01-B	1	6.33E+03			6.33E+03	2.6E-01	7.5E+00	2.4E+01			---		VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T02-B	1	5.70E+03			5.70E+03	3.4E-01	7.5E+00	2.4E+01	10	100	6.75E+03	104%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T03-B	1	1.28E+03			1.28E+03	1.3E+00	7.5E+00	2.4E+01			---		VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T04-B	1	1.14E+03			1.14E+03	8.4E-01	7.5E+00	2.4E+01			---		VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T05-B	1	6.16E+03			6.16E+03	5.0E+01	7.5E+00	2.4E+01			---		VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T06-B	1	5.49E+03			5.49E+03	2.3E-01	7.5E+00	2.4E+01			---		VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T07-B	1	9.00E+02			9.00E+02	2.2E+00	7.5E+00	2.4E+01			---		VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T08-B	1	5.42E+02			5.42E+02	1.2E+00	7.5E+00	2.4E+01			---		VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T09-B	1	9.31E+03			9.31E+03	4.7E+01	7.5E+00	2.4E+01			---		VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T01-C	1	6.06E+03			6.06E+03	2.0E-01	7.5E+00	2.4E+01			---		VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T02-C	1	5.56E+03			5.56E+03	2.2E+00	7.5E+00	2.4E+01	10	100	6.62E+03	106%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T03-C	1	1.18E+03			1.18E+03	9.5E-01	7.5E+00	2.4E+01			---		VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T04-C	1	9.88E+02			9.88E+02	7.5E-01	7.5E+00	2.4E+01					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T05-C	1	6.20E+03			6.20E+03	4.1E-01	7.5E+00	2.4E+01					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T06-C	1	5.61E+03			5.61E+03	4.7E-01	7.5E+00	2.4E+01					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T07-C	1	8.05E+02			8.05E+02	5.4E-01	7.5E+00	2.4E+01					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T08-C	1	8.95E+02			8.95E+02	2.6E-01	7.5E+00	2.4E+01					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-T09-C	1	5.96E+03			5.96E+03	5.8E+01	7.5E+00	2.4E+01					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-B01-A	1	1.28E+01	E		1.28E+01	2.2E+01	7.5E+00	2.4E+01					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-B02-A	1	1.41E+01	E		1.41E+01	2.6E+01	7.5E+00	2.4E+01					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-B03-A	1	1.07E+02			1.07E+02	8.7E+00	7.5E+00	2.4E+01					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-B01-B	1	1.63E+01	E		1.63E+01	2.1E+01	7.5E+00	2.4E+01					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-B02-B	1	1.46E+01	E		1.46E+01	4.7E+01	7.5E+00	2.4E+01					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-B03-B	1	5.57E+01			5.57E+01	1.0E+01	7.5E+00	2.4E+01					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-B01-C	1	2.17E+01	E		2.17E+01	1.2E+01	7.5E+00	2.4E+01					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-B02-C	1	2.24E+01	E		2.24E+01	3.8E+01	7.5E+00	2.4E+01					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1313-B03-C	1	2.95E+01			2.95E+01	2.9E+01	7.5E+00	2.4E+01					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	SWA-L05-1313-T01-A	1	1.11E+04			1.11E+04	1.5E+00	1.1E+01	3.5E+01			---		VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T02-A	1	4.10E+03			4.10E+03	2.3E-01	1.1E+01	3.5E+01	10	100	5.03E+03	93%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T03-A	1	1.54E+02			1.54E+02	3.2E+00	1.1E+01	3.5E+01			---		VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T04-A	1	1.62E+02			1.62E+02	1.7E+00	1.1E+01	3.5E+01			---		VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T05-A	1	4.80E+03			4.80E+03	6.8E-01	1.1E+01	3.5E+01			---		VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T06-A	1	4.03E+03			4.03E+03	1.2E+00	1.1E+01	3.5E+01			---		VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T07-A	1	2.74E+02			2.74E+02	6.4E+00	1.1E+01	3.5E+01			---		VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T08-A	1	6.01E+02			6.01E+02	7.2E+00	1.1E+01	3.5E+01			---		VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T09-A	1	2.49E+04			2.49E+04	4.9E+00	1.1E+01	3.5E+01					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T01-B	1	1.12E+04			1.12E+04	2.1E+00	1.1E+01	3.5E+01			---		VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T02-B	1	3.95E+03			3.95E+03	5.0E-01	1.1E+01	3.5E+01	10	100	4.90E+03	95%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T03-B	1	1.40E+02			1.40E+02	3.5E+00	1.1E+01	3.5E+01			---		VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T04-B	1	1.75E+02			1.75E+02	4.8E+00	1.1E+01	3.5E+01			---		VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T05-B	1	4.81E+03			4.81E+03	5.7E+01	1.1E+01	3.5E+01			---		VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T06-B	1	3.90E+03			3.90E+03	4.9E-01	1.1E+01	3.5E+01			---		VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T07-B	1	2.39E+02			2.39E+02	2.4E+00	1.1E+01	3.5E+01			---		VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T08-B	1	2.17E+03			2.17E+03	6.6E-01	1.1E+01	3.5E+01			---		VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T09-B	1	7.83E+03			7.83E+03	2.4E+01	1.1E+01	3.5E+01			---		VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T01-C	1	1.05E+04			1.05E+04	9.0E-01	1.1E+01	3.5E+01			---		VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T02-C	1	4.03E+03			4.03E+03	3.2E+00	1.1E+01	3.5E+01	10	100	4.92E+03	90%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T03-C	1	1.66E+02			1.66E+02	3.4E+00	1.1E+01	3.5E+01			---		VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T04-C	1	1.21E+02			1.21E+02	7.6E+00	1.1E+01	3.5E+01					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T05-C	1	4.84E+03			4.84E+03	7.1E-01	1.1E+01	3.5E+01					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T06-C	1	4.22E+03			4.22E+03	4.0E-01	1.1E+01	3.5E+01					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T07-C	1	2.43E+02			2.43E+02	9.9E+00	1.1E+01	3.5E+01					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T08-C	1	2.30E+03			2.30E+03	2.2E-01	1.1E+01	3.5E+01					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-T09-C	1	6.97E+03			6.97E+03	3.0E+01	1.1E+01	3.5E+01					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-B01-A	1	5.50E+00	U1/2		5.50E+00	2.0E+01	1.1E+01	3.5E+01					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-B02-A	1	5.50E+00	U1/2		5.50E+00	9.7E+01	1.1E+01	3.5E+01					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-B03-A	1	2.61E+01	E		2.61E+01	2.9E+01	1.1E+01	3.5E+01					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-B01-B	1	5.50E+00	U1/2		5.50E+00	6.1E+01	1.1E+01	3.5E+01					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-B02-B	1	5.50E+00	U1/2		5.50E+00	4.6E+01	1.1E+01	3.5E+01					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-B03-B	1	5.50E+00	U1/2		5.50E+00	4.0E+01	1.1E+01	3.5E+01					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-B01-C	1	5.50E+00	U1/2		5.50E+00	1.1E+02	1.1E+01	3.5E+01					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-B02-C	1	5.50E+00	U1/2		5.50E+00	8.1E+01	1.1E+01	3.5E+01					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1313-B03-C	1	1.15E+01	E		1.15E+01	5.6E+01	1.1E+01	3.5E+01					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	SWA-L05-1313-T01-A	1	1.05E+03			1.05E+03	6.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T02-A	1	7.30E+02			7.30E+02	8.5E-01	1.0E+00	3.2E+00	1000	100	1.64E+03	91%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T03-A	1	8.27E+02			8.27E+02	9.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T04-A	1	1.07E+03			1.07E+03	5.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T05-A	1	8.40E+02			8.40E+02	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T06-A	1	7.44E+02			7.44E+02	3.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T07-A	1	1.59E+03			1.59E+03	2.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T08-A	1	4.20E+03			4.20E+03	5.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T09-A	1	6.43E+03			6.43E+03	1.6E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T01-B	1	1.13E+03			1.13E+03	8.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T02-B	1	7.36E+02			7.36E+02	4.8E-01	1.0E+00	3.2E+00	1000	100	1.65E+03	91%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T03-B	1	8.73E+02			8.73E+02	7.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T04-B	1	1.11E+03			1.11E+03	2.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T05-B	1	8.29E+02			8.29E+02	4.2E+01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T06-B	1	7.27E+02			7.27E+02	8.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T07-B	1	3.14E+03			3.14E+03	7.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T08-B	1	4.54E+03			4.54E+03	2.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T09-B	1	5.29E+03			5.29E+03	7.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T01-C	1	1.06E+03			1.06E+03	2.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T02-C	1	7.27E+02			7.27E+02	2.0E+00	1.0E+00	3.2E+00	1000	100	1.68E+03	95%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T03-C	1	8.49E+02			8.49E+02	6.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T04-C	1	1.12E+03			1.12E+03	5.0E-01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T05-C	1	8.31E+02			8.31E+02	5.0E-01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T06-C	1	7.38E+02			7.38E+02	6.6E-01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T07-C	1	3.45E+03			3.45E+03	2.3E-01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T08-C	1	4.52E+03			4.52E+03	5.6E-01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-T09-C	1	4.27E+03			4.27E+03	4.6E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	4.8E+02	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-B02-A	1	2.09E+00	E		2.09E+00	1.6E+02	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-B03-A	1	6.36E+00			6.36E+00	2.4E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	2.6E+02	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-B02-B	1	1.49E+00	E		1.49E+00	1.4E+02	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-B03-B	1	4.81E+00			4.81E+00	4.6E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-B01-C	1	1.25E+00	E		1.25E+00	1.3E+02	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-B02-C	1	2.53E+00	E		2.53E+00	5.1E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1313-B03-C	1	4.57E+00			4.57E+00	4.6E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	SWA-L05-1313-T01-A	1	3.18E+02			3.18E+02	3.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T02-A	1	8.98E+01			8.98E+01	5.7E-01	1.0E+00	3.2E+00	10	100	9.93E+02	90%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T03-A	1	5.16E+02			5.16E+02	6.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T04-A	1	4.57E+02			4.57E+02	6.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T05-A	1	1.21E+02			1.21E+02	4.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T06-A	1	8.85E+01			8.85E+01	7.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T07-A	1	7.08E+02			7.08E+02	2.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T08-A	1	1.06E+03			1.06E+03	2.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T09-A	1	8.98E+02			8.98E+02	3.2E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T01-B	1	3.14E+02			3.14E+02	4.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T02-B	1	9.47E+01			9.47E+01	5.4E-01	1.0E+00	3.2E+00	10	100	9.78E+02	88%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T03-B	1	6.18E+02			6.18E+02	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T04-B	1	4.83E+02			4.83E+02	1.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T05-B	1	1.23E+02			1.23E+02	4.7E+01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T06-B	1	1.20E+02			1.20E+02	1.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T07-B	1	8.81E+02			8.81E+02	4.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T08-B	1	6.32E+02			6.32E+02	3.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T09-B	1	7.11E+02			7.11E+02	4.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T01-C	1	3.25E+02			3.25E+02	1.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T02-C	1	9.41E+01			9.41E+01	1.7E+00	1.0E+00	3.2E+00	10	100	9.60E+02	87%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T03-C	1	6.27E+02			6.27E+02	4.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T04-C	1	5.34E+02			5.34E+02	1.0E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T05-C	1	1.21E+02			1.21E+02	5.8E-01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T06-C	1	8.38E+01			8.38E+01	2.3E-01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T07-C	1	9.94E+02			9.94E+02	2.5E-01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T08-C	1	6.52E+02			6.52E+02	4.8E-01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-T09-C	1	5.73E+02			5.73E+02	7.4E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	2.0E+02	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	9.2E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	8.8E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	9.1E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	1.6E+02	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-B02-C	1	1.17E+00	E		1.17E+00	2.6E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	1.3E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	SWA-L05-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	7.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	8.7E+01	1.9E+00	6.0E+00	10	100	9.90E+02	99%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	9.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	4.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	2.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	7.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T07-A	1	9.50E-01	U1/2		9.50E-01	5.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T08-A	1	9.50E-01	U1/2		9.50E-01	4.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T09-A	1	1.28E+02			1.28E+02	6.4E+00	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	8.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	9.6E+01	1.9E+00	6.0E+00	10	100	9.65E+02	96%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	1.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	8.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	3.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	1.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T07-B	1	9.50E-01	U1/2		9.50E-01	3.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T08-B	1	7.73E+01			7.73E+01	1.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T09-B	1	9.69E+01			9.69E+01	3.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	6.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	5.1E+02	1.9E+00	6.0E+00	10	100	9.85E+02	98%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	2.7E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	1.7E+03	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	4.4E+02	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	5.7E+01	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T07-C	1	9.50E-01	U1/2		9.50E-01	6.6E+01	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T08-C	1	7.60E+01			7.60E+01	4.3E-02	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-T09-C	1	7.92E+01			7.92E+01	7.0E+00	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	6.6E+01	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	3.2E+02	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	5.0E+01	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-B01-B	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-B02-B	1	9.50E-01	U1/2		9.50E-01	2.0E+02	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-B03-B	1	9.50E-01	U1/2		9.50E-01	4.4E+01	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-B01-C	1	9.50E-01	U1/2		9.50E-01	1.5E+02	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-B02-C	1	9.50E-01	U1/2		9.50E-01	1.7E+02	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1313-B03-C	1	9.50E-01	U1/2		9.50E-01	7.3E+01	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	SWA-L05-1313-T01-A	1	1.10E+00	U1/2		1.10E+00	6.1E+02	2.2E+00	7.0E+00			---		VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T02-A	1	1.10E+00	U1/2		1.10E+00	8.5E+01	2.2E+00	7.0E+00	10	100	9.70E+02	97%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	2.2E+02	2.2E+00	7.0E+00			---		VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T04-A	1	1.10E+00	U1/2		1.10E+00	6.5E+01	2.2E+00	7.0E+00			---		VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T05-A	1	1.10E+00	U1/2		1.10E+00	1.2E+03	2.2E+00	7.0E+00			---		VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T06-A	1	1.10E+00	U1/2		1.10E+00	7.0E+01	2.2E+00	7.0E+00			---		VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T07-A	1	1.10E+00	U1/2		1.10E+00	1.8E+02	2.2E+00	7.0E+00			---		VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T08-A	1	5.55E+00	E		5.55E+00	2.0E+00	2.2E+00	7.0E+00			---		VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T09-A	1	4.38E+01			4.38E+01	3.6E+00	2.2E+00	7.0E+00					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T01-B	1	1.10E+00	U1/2		1.10E+00	1.3E+02	2.2E+00	7.0E+00			---		VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T02-B	1	1.10E+00	U1/2		1.10E+00	4.1E+01	2.2E+00	7.0E+00	10	100	9.60E+02	96%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	5.1E+01	2.2E+00	7.0E+00			---		VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T04-B	1	1.10E+00	U1/2		1.10E+00	3.7E+02	2.2E+00	7.0E+00			---		VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T05-B	1	1.10E+00	U1/2		1.10E+00	2.6E+01	2.2E+00	7.0E+00			---		VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T06-B	1	1.10E+00	U1/2		1.10E+00	1.1E+02	2.2E+00	7.0E+00			---		VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T07-B	1	1.10E+00	U1/2		1.10E+00	1.7E+01	2.2E+00	7.0E+00			---		VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T08-B	1	1.47E+01			1.47E+01	1.8E+00	2.2E+00	7.0E+00			---		VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T09-B	1	2.86E+01			2.86E+01	7.3E+00	2.2E+00	7.0E+00			---		VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T01-C	1	1.10E+00	U1/2		1.10E+00	2.9E+02	2.2E+00	7.0E+00			---		VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T02-C	1	1.10E+00	U1/2		1.10E+00	3.1E+03	2.2E+00	7.0E+00	10	100	9.36E+02	94%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	2.8E+02	2.2E+00	7.0E+00			---		VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T04-C	1	1.10E+00	U1/2		1.10E+00	2.4E+02	2.2E+00	7.0E+00					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T05-C	1	1.10E+00	U1/2		1.10E+00	2.3E+02	2.2E+00	7.0E+00					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T06-C	1	1.10E+00	U1/2		1.10E+00	7.9E+01	2.2E+00	7.0E+00					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T07-C	1	1.10E+00	U1/2		1.10E+00	7.4E+01	2.2E+00	7.0E+00					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T08-C	1	1.33E+01			1.33E+01	1.4E+00	2.2E+00	7.0E+00					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-T09-C	1	2.43E+01			2.43E+01	1.2E+01	2.2E+00	7.0E+00					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	2.2E+02	2.2E+00	7.0E+00					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	2.5E+02	2.2E+00	7.0E+00					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-B03-A	1	1.10E+00	U1/2		1.10E+00	4.9E+02	2.2E+00	7.0E+00					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-B01-B	1	1.10E+00	U1/2		1.10E+00	1.7E+02	2.2E+00	7.0E+00					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-B02-B	1	1.10E+00	U1/2		1.10E+00	1.3E+02	2.2E+00	7.0E+00					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-B03-B	1	1.10E+00	U1/2		1.10E+00	1.3E+02	2.2E+00	7.0E+00					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-B01-C	1	1.10E+00	U1/2		1.10E+00	2.7E+02	2.2E+00	7.0E+00					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-B02-C	1	1.10E+00	U1/2		1.10E+00	1.6E+02	2.2E+00	7.0E+00					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1313-B03-C	1	1.10E+00	U1/2		1.10E+00	8.2E+01	2.2E+00	7.0E+00					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	SWA-L05-1313-T01-A	1	5.56E+03			5.56E+03	8.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T02-A	1	8.37E+03			8.37E+03	3.4E-01	2.6E+00	8.3E+00	1000	100	9.25E+03	89%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T03-A	1	7.99E+05			7.99E+05	6.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T04-A	1	1.73E+06			1.73E+06	8.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T05-A	1	8.53E+03			8.53E+03	4.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T06-A	1	8.58E+03			8.58E+03	5.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T07-A	1	3.89E+06			3.89E+06	2.5E+00	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T08-A	1	4.65E+06			4.65E+06	4.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T09-A	1	4.72E+06			4.72E+06	3.3E+00	2.6E+00	8.3E+00					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T01-B	1	5.31E+03			5.31E+03	4.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T02-B	1	8.44E+03			8.44E+03	2.6E-01	2.6E+00	8.3E+00	1000	100	9.35E+03	91%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T03-B	1	8.13E+05			8.13E+05	1.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T04-B	1	1.77E+06			1.77E+06	8.7E-02	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T05-B	1	8.67E+03			8.67E+03	6.7E+01	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T06-B	1	9.25E+03			9.25E+03	2.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T07-B	1	4.60E+06			4.60E+06	9.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T08-B	1	3.21E+06			3.21E+06	1.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T09-B	1	3.92E+06			3.92E+06	2.9E+00	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T01-C	1	5.47E+03			5.47E+03	1.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T02-C	1	8.67E+03			8.67E+03	2.1E+00	2.6E+00	8.3E+00	1000	100	9.55E+03	87%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T03-C	1	7.95E+05			7.95E+05	2.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T04-C	1	1.80E+06			1.80E+06	6.1E-01	2.6E+00	8.3E+00					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T05-C	1	8.65E+03			8.65E+03	6.9E-01	2.6E+00	8.3E+00					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T06-C	1	9.03E+03			9.03E+03	4.7E-01	2.6E+00	8.3E+00					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T07-C	1	4.57E+06			4.57E+06	3.4E-01	2.6E+00	8.3E+00					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T08-C	1	3.29E+06			3.29E+06	9.0E-01	2.6E+00	8.3E+00					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-T09-C	1	3.45E+06			3.45E+06	6.0E+00	2.6E+00	8.3E+00					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-B01-A	1	3.71E+00	E		3.71E+00	2.2E+01	2.6E+00	8.3E+00					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-B02-A	1	1.30E+00	U1/2		1.30E+00	7.4E+01	2.6E+00	8.3E+00					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-B03-A	1	1.30E+00	U1/2		1.30E+00	3.5E+02	2.6E+00	8.3E+00					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-B01-B	1	7.48E+00	E		7.48E+00	1.3E+02	2.6E+00	8.3E+00					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-B02-B	1	1.30E+00	U1/2		1.30E+00	6.1E+02	2.6E+00	8.3E+00					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-B03-B	1	6.22E+00	E		6.22E+00	2.7E+02	2.6E+00	8.3E+00					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-B01-C	1	1.08E+01			1.08E+01	4.2E+01	2.6E+00	8.3E+00					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-B02-C	1	4.13E+03			4.13E+03	6.7E-01	2.6E+00	8.3E+00					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1313-B03-C	1	5.24E+00	E		5.24E+00	1.1E+02	2.6E+00	8.3E+00					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	SWA-L05-1313-T01-A	1	1.13E+03			1.13E+03	7.6E-01	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T02-A	1	9.20E+02			9.20E+02	7.8E-02	1.2E+00	3.8E+00	10	100	1.84E+03	92%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T03-A	1	5.99E+01			5.99E+01	1.6E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T04-A	1	2.43E+01			2.43E+01	2.8E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T05-A	1	9.14E+02			9.14E+02	1.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T06-A	1	9.16E+02			9.16E+02	6.0E-01	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T07-A	1	2.04E+01			2.04E+01	5.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T08-A	1	1.27E+02			1.27E+02	1.0E+01	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T09-A	1	2.66E+04			2.66E+04	3.3E+00	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T01-B	1	1.23E+03			1.23E+03	1.4E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T02-B	1	8.60E+02			8.60E+02	1.6E+00	1.2E+00	3.8E+00	10	100	1.83E+03	97%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T03-B	1	4.32E+01			4.32E+01	1.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T04-B	1	2.14E+01			2.14E+01	3.6E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T05-B	1	9.25E+02			9.25E+02	5.2E+01	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T06-B	1	8.40E+02			8.40E+02	5.5E-01	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T07-B	1	1.59E+00	E		1.59E+00	2.8E+01	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T08-B	1	8.53E+03			8.53E+03	2.1E-01	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T09-B	1	2.05E+04			2.05E+04	3.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T01-C	1	1.08E+03			1.08E+03	5.1E-01	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T02-C	1	9.15E+02			9.15E+02	2.5E+00	1.2E+00	3.8E+00	10	100	1.89E+03	98%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T03-C	1	4.50E+01			4.50E+01	6.6E-01	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T04-C	1	2.31E+01			2.31E+01	2.4E+00	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T05-C	1	8.94E+02			8.94E+02	3.0E-01	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T06-C	1	9.54E+02			9.54E+02	6.3E-01	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T07-C	1	6.00E-01	U1/2		6.00E-01	4.5E+02	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T08-C	1	8.69E+03			8.69E+03	4.2E-01	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-T09-C	1	1.67E+04			1.67E+04	7.7E+00	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	8.3E+01	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	3.2E+02	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-B03-A	1	6.00E-01	U1/2		6.00E-01	4.8E+01	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-B01-B	1	6.00E-01	U1/2		6.00E-01	1.4E+02	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-B02-B	1	6.00E-01	U1/2		6.00E-01	2.3E+02	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-B03-B	1	6.00E-01	U1/2		6.00E-01	1.4E+02	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-B01-C	1	6.00E-01	U1/2		6.00E-01	2.0E+02	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-B02-C	1	6.00E-01	U1/2		6.00E-01	9.1E+01	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1313-B03-C	1	6.00E-01	U1/2		6.00E-01	3.6E+01	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	SWA-L05-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	8.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	1.2E+03	1.8E+00	5.7E+00	10	100	9.32E+02	93%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	1.2E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	2.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T05-A	1	9.00E-01	U1/2		9.00E-01	4.8E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T06-A	1	9.00E-01	U1/2		9.00E-01	1.7E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T07-A	1	9.00E-01	U1/2		9.00E-01	2.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T08-A	1	1.17E+02			1.17E+02	1.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T09-A	1	3.38E+02			3.38E+02	3.8E+00	1.8E+00	5.7E+00					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	6.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	4.2E+01	1.8E+00	5.7E+00	10	100	9.18E+02	92%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	2.6E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	5.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T05-B	1	9.00E-01	U1/2		9.00E-01	5.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T06-B	1	9.00E-01	U1/2		9.00E-01	5.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T07-B	1	2.70E+01			2.70E+01	6.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T08-B	1	1.36E+02			1.36E+02	4.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T09-B	1	2.23E+02			2.23E+02	6.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	2.9E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	5.7E+01	1.8E+00	5.7E+00	10	100	9.35E+02	93%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	2.1E+02	1.8E+00	5.7E+00					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T05-C	1	9.00E-01	U1/2		9.00E-01	2.5E+02	1.8E+00	5.7E+00					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T06-C	1	9.00E-01	U1/2		9.00E-01	5.3E+02	1.8E+00	5.7E+00					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T07-C	1	5.31E+01			5.31E+01	2.2E+00	1.8E+00	5.7E+00					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T08-C	1	1.33E+02			1.33E+02	1.1E+00	1.8E+00	5.7E+00					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-T09-C	1	1.88E+02			1.88E+02	1.1E+01	1.8E+00	5.7E+00					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	7.1E+01	1.8E+00	5.7E+00					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	3.0E+01	1.8E+00	5.7E+00					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	1.6E+02	1.8E+00	5.7E+00					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-B01-B	1	9.00E-01	U1/2		9.00E-01	2.2E+01	1.8E+00	5.7E+00					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-B02-B	1	9.00E-01	U1/2		9.00E-01	2.2E+01	1.8E+00	5.7E+00					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-B03-B	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-B01-C	1	9.00E-01	U1/2		9.00E-01	1.4E+01	1.8E+00	5.7E+00					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-B02-C	1	9.00E-01	U1/2		9.00E-01	2.4E+01	1.8E+00	5.7E+00					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1313-B03-C	1	9.00E-01	U1/2		9.00E-01	2.5E+02	1.8E+00	5.7E+00					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	SWA-L05-1313-T01-A	1	6.64E+00	E		6.64E+00	3.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T02-A	1	5.03E+00	E		5.03E+00	2.0E+01	3.7E+00	1.2E+01	10	100	8.95E+02	89%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T03-A	1	5.23E+00	E		5.23E+00	3.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T04-A	1	7.85E+00	E		7.85E+00	2.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T05-A	1	5.34E+00	E		5.34E+00	3.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T06-A	1	4.03E+00	E		4.03E+00	8.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T07-A	1	1.41E+01			1.41E+01	5.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T08-A	1	1.66E+01			1.66E+01	8.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T09-A	1	1.15E+03			1.15E+03	3.7E+00	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T01-B	1	6.61E+00	E		6.61E+00	1.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T02-B	1	1.85E+00	U1/2		1.85E+00	4.7E+02	3.7E+00	1.2E+01	10	100	8.84E+02	88%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T03-B	1	5.84E+00	E		5.84E+00	2.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T04-B	1	1.00E+01	E		1.00E+01	2.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T05-B	1	1.85E+00	U1/2		1.85E+00	8.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T06-B	1	1.85E+00	U1/2		1.85E+00	1.1E+02	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T07-B	1	2.00E+01			2.00E+01	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T08-B	1	2.65E+02			2.65E+02	6.2E-01	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T09-B	1	9.37E+02			9.37E+02	2.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T01-C	1	6.21E+00	E		6.21E+00	1.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T02-C	1	1.85E+00	U1/2		1.85E+00	9.9E+01	3.7E+00	1.2E+01	10	100	9.02E+02	90%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T03-C	1	6.09E+00	E		6.09E+00	2.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T04-C	1	6.77E+00	E		6.77E+00	3.5E+01	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T05-C	1	1.85E+00	U1/2		1.85E+00	4.4E+01	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T06-C	1	1.85E+00	U1/2		1.85E+00	1.8E+01	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T07-C	1	2.42E+01			2.42E+01	4.5E+00	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T08-C	1	2.41E+02			2.41E+02	8.1E-01	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-T09-C	1	7.28E+02			7.28E+02	6.9E+00	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	9.0E+02	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	3.1E+02	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-B03-A	1	1.85E+00	U1/2		1.85E+00	1.4E+02	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-B01-B	1	1.85E+00	U1/2		1.85E+00	2.2E+02	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-B02-B	1	1.85E+00	U1/2		1.85E+00	1.2E+02	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-B03-B	1	1.85E+00	U1/2		1.85E+00	7.6E+01	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-B01-C	1	1.85E+00	U1/2		1.85E+00	9.4E+01	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-B02-C	1	8.19E+00	E		8.19E+00	9.1E+00	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1313-B03-C	1	1.85E+00	U1/2		1.85E+00	5.8E+01	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	SWA-L05-1313-T01-A	1	8.91E+01			8.91E+01	5.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T02-A	1	6.75E+01			6.75E+01	1.0E-01	2.0E+00	6.4E+00	1000	100	9.59E+02	89%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	2.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	3.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T05-A	1	7.12E+01			7.12E+01	7.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T06-A	1	6.49E+01			6.49E+01	1.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	2.5E+03	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T08-A	1	5.54E+04			5.54E+04	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T09-A	1	2.99E+05			2.99E+05	5.6E+00	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T01-B	1	8.36E+01			8.36E+01	1.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T02-B	1	6.12E+01			6.12E+01	1.9E+00	2.0E+00	6.4E+00	1000	100	9.79E+02	92%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	1.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	6.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T05-B	1	7.03E+01			7.03E+01	6.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T06-B	1	5.90E+01			5.90E+01	1.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	1.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T08-B	1	9.03E+04			9.03E+04	8.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T09-B	1	2.23E+05			2.23E+05	6.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T01-C	1	1.07E+02			1.07E+02	1.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T02-C	1	7.01E+01			7.01E+01	5.8E+00	2.0E+00	6.4E+00	1000	100	9.98E+02	93%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	3.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	9.7E+00	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T05-C	1	7.18E+01			7.18E+01	1.3E+00	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T06-C	1	6.40E+01			6.40E+01	8.8E-01	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T07-C	1	6.16E+02			6.16E+02	5.8E+00	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T08-C	1	8.83E+04			8.83E+04	7.0E-01	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-T09-C	1	1.89E+05			1.89E+05	1.1E+01	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	8.1E-01	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	5.1E+01	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	9.7E+00	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	1.6E+00	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	7.7E+00	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	5.9E+00	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	1.0E+00	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	7.3E+00	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1313-B03-C	1	1.00E+00	U1/2		1.00E+00	1.7E+00	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	SWA-L05-1313-T01-A	1	1.33E+02			1.33E+02	7.1E+00	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T02-A	1	3.40E+00	U1/2		3.40E+00	1.6E+02	6.8E+00	2.2E+01	10	100	9.65E+02	96%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T03-A	1	3.40E+00	U1/2		3.40E+00	3.9E+02	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T04-A	1	3.40E+00	U1/2		3.40E+00	8.3E+01	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T05-A	1	3.40E+00	U1/2		3.40E+00	5.1E+01	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T06-A	1	3.40E+00	U1/2		3.40E+00	1.5E+02	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T07-A	1	3.40E+00	U1/2		3.40E+00	8.4E+01	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T08-A	1	3.40E+00	U1/2		3.40E+00	9.9E+00	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T09-A	1	3.27E+03			3.27E+03	3.0E+00	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T01-B	1	1.48E+02			1.48E+02	2.5E+00	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T02-B	1	3.40E+00	U1/2		3.40E+00	3.3E+00	6.8E+00	2.2E+01	10	100	9.75E+02	97%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T03-B	1	3.40E+00	U1/2		3.40E+00	7.5E+01	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T04-B	1	3.40E+00	U1/2		3.40E+00	6.9E+01	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T05-B	1	3.40E+00	U1/2		3.40E+00	7.9E+01	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T06-B	1	3.40E+00	U1/2		3.40E+00	3.3E+02	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T07-B	1	7.62E+00	E		7.62E+00	9.3E+01	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T08-B	1	7.36E+02			7.36E+02	6.3E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T09-B	1	2.62E+03			2.62E+03	2.6E+00	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T01-C	1	1.40E+02			1.40E+02	3.7E+00	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T02-C	1	3.40E+00	U1/2		3.40E+00	1.2E+02	6.8E+00	2.2E+01	10	100	9.47E+02	94%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T03-C	1	3.40E+00	U1/2		3.40E+00	1.1E+02	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T04-C	1	3.40E+00	U1/2		3.40E+00	2.5E+01	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T05-C	1	3.40E+00	U1/2		3.40E+00	7.8E+01	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T06-C	1	3.40E+00	U1/2		3.40E+00	9.3E+01	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T07-C	1	3.40E+00	U1/2		3.40E+00	2.9E+02	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T08-C	1	6.29E+02			6.29E+02	1.0E+00	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-T09-C	1	2.15E+03			2.15E+03	9.6E+00	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	6.3E+02	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	8.6E+02	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	3.2E+03	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-B01-B	1	3.40E+00	U1/2		3.40E+00	8.4E+01	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-B02-B	1	3.40E+00	U1/2		3.40E+00	1.3E+02	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-B03-B	1	3.40E+00	U1/2		3.40E+00	1.0E+02	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-B01-C	1	3.40E+00	U1/2		3.40E+00	5.8E+01	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-B02-C	1	3.40E+00	U1/2		3.40E+00	6.3E+01	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1313-B03-C	1	3.40E+00	U1/2		3.40E+00	7.8E+01	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	SWA-L05-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	7.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	2.9E+00	1.9E+00	6.0E+00	10	100	8.49E+02	85%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T03-A	1	1.84E+01			1.84E+01	1.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T04-A	1	5.29E+01			5.29E+01	1.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	3.6E-01	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	6.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T07-A	1	3.66E+02			3.66E+02	1.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T08-A	1	6.47E+02			6.47E+02	1.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T09-A	1	7.01E+02			7.01E+02	7.9E+00	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	2.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	7.7E+00	1.9E+00	6.0E+00	10	100	8.70E+02	87%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T03-B	1	1.91E+01			1.91E+01	7.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T04-B	1	6.42E+01			6.42E+01	9.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	1.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	2.8E-01	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T07-B	1	5.09E+02			5.09E+02	2.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T08-B	1	4.82E+02			4.82E+02	1.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T09-B	1	4.92E+02			4.92E+02	1.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	3.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	4.0E+00	1.9E+00	6.0E+00	10	100	8.70E+02	87%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T03-C	1	1.28E+01			1.28E+01	9.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T04-C	1	6.38E+01			6.38E+01	1.9E+01	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	1.4E+00	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	2.8E+00	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T07-C	1	5.07E+02			5.07E+02	3.7E+00	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T08-C	1	5.11E+02			5.11E+02	2.7E+00	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-T09-C	1	3.63E+02			3.63E+02	1.0E+01	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	4.2E+00	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	1.0E+01	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	1.2E+01	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-B01-B	1	9.50E-01	U1/2		9.50E-01	4.0E+00	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-B02-B	1	9.50E-01	U1/2		9.50E-01	2.8E+00	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-B03-B	1	9.50E-01	U1/2		9.50E-01	1.8E+00	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-B01-C	1	9.50E-01	U1/2		9.50E-01	4.5E+00	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-B02-C	1	9.50E-01	U1/2		9.50E-01	9.6E+00	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1313-B03-C	1	9.50E-01	U1/2		9.50E-01	3.4E+00	1.9E+00	6.0E+00					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	SWA-L05-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	2.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	6.3E+01	2.0E+00	6.4E+00	10	100	9.36E+02	94%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	3.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	8.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	7.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T07-A	1	1.64E+02			1.64E+02	2.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T08-A	1	1.42E+04			1.42E+04	3.3E-01	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T09-A	1	2.25E+04			2.25E+04	2.1E+00	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	1.0E+01	2.0E+00	6.4E+00	10	100	9.34E+02	93%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	8.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	3.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	6.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T07-B	1	6.16E+03			6.16E+03	5.2E-01	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T08-B	1	1.38E+04			1.38E+04	1.8E-01	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T09-B	1	1.81E+04			1.81E+04	5.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	1.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	5.3E+00	2.0E+00	6.4E+00	10	100	9.48E+02	95%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	4.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	5.1E+01	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T07-C	1	8.25E+03			8.25E+03	3.0E-01	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T08-C	1	1.37E+04			1.37E+04	4.9E-01	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-T09-C	1	1.55E+04			1.55E+04	8.7E+00	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.9E+02	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	9.0E+04	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	5.4E+01	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	1.5E+03	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	1.8E+02	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	5.3E+01	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	4.7E+01	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1313-B03-C	1	1.00E+00	U1/2		1.00E+00	9.3E+01	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	SWA-L05-1313-T01-A	1	5.00E-01	U1/2		5.00E-01	2.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T02-A	1	5.00E-01	U1/2		5.00E-01	2.5E+01	1.0E+00	3.2E+00	1000	100	9.01E+02	90%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T03-A	1	1.36E+03			1.36E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T04-A	1	1.49E+05			1.49E+05	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T05-A	1	5.00E-01	U1/2		5.00E-01	1.0E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T06-A	1	5.00E-01	U1/2		5.00E-01	2.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T07-A	1	4.13E+05			4.13E+05	9.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T08-A	1	8.17E+05			8.17E+05	5.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T09-A	1	8.92E+05			8.92E+05	3.1E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T01-B	1	5.00E-01	U1/2		5.00E-01	6.7E+03	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T02-B	1	5.00E-01	U1/2		5.00E-01	3.2E+01	1.0E+00	3.2E+00	1000	100	9.25E+02	92%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T03-B	1	1.15E+03			1.15E+03	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T04-B	1	1.52E+05			1.52E+05	8.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T05-B	1	5.00E-01	U1/2		5.00E-01	1.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T06-B	1	5.00E-01	U1/2		5.00E-01	4.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T07-B	1	7.34E+05			7.34E+05	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T08-B	1	5.99E+05			5.99E+05	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T09-B	1	7.31E+05			7.31E+05	5.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T01-C	1	5.00E-01	U1/2		5.00E-01	1.9E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T02-C	1	5.00E-01	U1/2		5.00E-01	4.2E+02	1.0E+00	3.2E+00	1000	100	9.25E+02	92%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T03-C	1	1.03E+03			1.03E+03	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T04-C	1	1.35E+05			1.35E+05	3.7E-01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T05-C	1	5.00E-01	U1/2		5.00E-01	1.6E+02	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T06-C	1	5.00E-01	U1/2		5.00E-01	7.0E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T07-C	1	7.12E+05			7.12E+05	5.7E-01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T08-C	1	6.19E+05			6.19E+05	9.4E-01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-T09-C	1	6.13E+05			6.13E+05	1.0E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	2.7E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	6.1E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	8.4E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	1.8E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	3.4E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	9.5E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	6.3E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-B02-C	1	3.94E+02			3.94E+02	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	1.1E+02	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	SWA-L05-1313-T01-A	1	9.60E+01			9.60E+01	2.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T02-A	1	1.00E+02			1.00E+02	2.4E+00	1.2E+00	3.8E+00	10	100	1.08E+03	98%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T03-A	1	9.27E+01			9.27E+01	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T04-A	1	8.21E+01			8.21E+01	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T05-A	1	1.05E+02			1.05E+02	8.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T06-A	1	9.81E+01			9.81E+01	7.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T07-A	1	1.42E+02			1.42E+02	4.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T08-A	1	4.35E+00			4.35E+00	3.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T09-A	1	4.29E+01			4.29E+01	1.1E+01	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T01-B	1	9.50E+01			9.50E+01	1.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T02-B	1	9.73E+01			9.73E+01	2.9E+00	1.2E+00	3.8E+00	10	100	1.05E+03	96%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T03-B	1	9.16E+01			9.16E+01	2.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T04-B	1	8.68E+01			8.68E+01	3.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T05-B	1	1.02E+02			1.02E+02	5.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T06-B	1	9.49E+01			9.49E+01	2.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T07-B	1	7.32E+01			7.32E+01	1.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T08-B	1	2.71E+00	E		2.71E+00	2.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T09-B	1	1.40E+01			1.40E+01	3.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T01-C	1	8.77E+01			8.77E+01	2.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T02-C	1	9.81E+01			9.81E+01	1.5E+00	1.2E+00	3.8E+00	10	100	1.09E+03	99%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T03-C	1	9.18E+01			9.18E+01	1.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T04-C	1	9.07E+01			9.07E+01	1.6E+00	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T05-C	1	1.07E+02			1.07E+02	2.5E+00	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T06-C	1	9.70E+01			9.70E+01	1.0E+00	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T07-C	1	5.94E+01			5.94E+01	2.7E+00	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T08-C	1	2.21E+00	E		2.21E+00	4.4E+01	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-T09-C	1	1.57E+01			1.57E+01	1.6E+01	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	8.4E+01	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-B02-A	1	2.75E+00	E		2.75E+00	9.7E+01	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-B03-A	1	9.82E+00			9.82E+00	4.7E+00	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-B01-B	1	6.00E-01	U1/2		6.00E-01	7.1E+01	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-B02-B	1	6.00E-01	U1/2		6.00E-01	7.7E+01	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-B03-B	1	3.98E+00			3.98E+00	5.6E+01	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-B01-C	1	6.00E-01	U1/2		6.00E-01	1.7E+02	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-B02-C	1	6.00E-01	U1/2		6.00E-01	8.0E+03	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1313-B03-C	1	6.00E-01	U1/2		6.00E-01	1.3E+02	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	SWA-L05-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	1.0E+02	1.8E+00	5.7E+00			---		VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	7.8E+01	1.8E+00	5.7E+00	10	100	9.83E+02	98%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	2.1E+01	1.8E+00	5.7E+00			---		VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T04-A	1	4.26E+00	E		4.26E+00	3.5E+01	1.8E+00	5.7E+00			---		VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T05-A	1	9.39E+00			9.39E+00	8.1E+03	1.8E+00	5.7E+00			---		VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T06-A	1	9.00E-01	U1/2		9.00E-01	2.8E+01	1.8E+00	5.7E+00			---		VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T07-A	1	1.01E+01			1.01E+01	3.4E+00	1.8E+00	5.7E+00			---		VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T08-A	1	2.78E+02			2.78E+02	3.1E-01	1.8E+00	5.7E+00			---		VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T09-A	1	4.66E+02			4.66E+02	2.2E+00	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	1.0E+02	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	1.2E+02	1.2E+00	3.8E+00	10	100	9.66E+02	97%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	1.8E+02	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T04-B	1	5.06E+00			5.06E+00	3.3E+01	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T05-B	1	1.05E+01			1.05E+01	1.3E+03	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T06-B	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T07-B	1	7.63E+01			7.63E+01	5.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T08-B	1	2.69E+02			2.69E+02	1.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T09-B	1	3.68E+02			3.68E+02	5.5E+00	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	4.3E+01	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	3.7E+02	1.2E+00	3.8E+00	10	100	9.33E+02	93%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.2E+00	3.8E+00			---		VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T04-C	1	3.77E+00	E		3.77E+00	1.0E+01	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T05-C	1	1.44E+01			1.44E+01	2.9E+01	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T06-C	1	9.00E-01	U1/2		9.00E-01	3.6E+01	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T07-C	1	1.48E+02			1.48E+02	1.3E+00	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T08-C	1	2.69E+02			2.69E+02	9.0E-01	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-T09-C	1	3.17E+02			3.17E+02	8.8E+00	1.2E+00	3.8E+00					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	3.7E+02	1.8E+00	5.7E+00					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	4.8E+02	1.8E+00	5.7E+00					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.8E+00	5.7E+00					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-B01-B	1	9.00E-01	U1/2		9.00E-01	3.2E+02	1.8E+00	5.7E+00					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-B02-B	1	9.00E-01	U1/2		9.00E-01	2.0E+02	1.8E+00	5.7E+00					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-B03-B	1	9.00E-01	U1/2		9.00E-01	5.1E+02	1.8E+00	5.7E+00					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-B01-C	1	9.00E-01	U1/2		9.00E-01	5.8E+01	1.8E+00	5.7E+00					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-B02-C	1	9.00E-01	U1/2		9.00E-01	6.5E+03	1.8E+00	5.7E+00					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1313-B03-C	1	9.00E-01	U1/2		9.00E-01	8.0E+02	1.8E+00	5.7E+00					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	SWA-L05-1313-T01-A	1	2.26E+02			2.26E+02	4.2E+00	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T02-A	1	4.01E+01			4.01E+01	3.8E+01	3.7E+00	1.2E+01	1000	100	9.92E+02	95%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T03-A	1	2.30E+01			2.30E+01	3.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T04-A	1	1.58E+01			1.58E+01	9.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T05-A	1	5.97E+01			5.97E+01	9.6E+00	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T06-A	1	4.43E+01			4.43E+01	3.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T07-A	1	8.02E+01			8.02E+01	2.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T08-A	1	3.25E+01			3.25E+01	2.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T09-A	1	4.27E+04			4.27E+04	6.1E+00	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T01-B	1	2.40E+02			2.40E+02	3.3E+00	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T02-B	1	5.76E+01			5.76E+01	1.4E+01	3.7E+00	1.2E+01	1000	100	9.96E+02	94%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T03-B	1	2.31E+01			2.31E+01	3.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T04-B	1	1.36E+01			1.36E+01	1.8E+02	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T05-B	1	6.14E+01			6.14E+01	1.7E+02	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T06-B	1	4.57E+01			4.57E+01	1.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T07-B	1	2.98E+01			2.98E+01	8.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T08-B	1	9.80E+01			9.80E+01	9.7E-01	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T09-B	1	1.13E+04			1.13E+04	3.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T01-C	1	2.11E+02			2.11E+02	6.3E+00	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T02-C	1	4.63E+01			4.63E+01	2.6E+01	3.7E+00	1.2E+01	1000	100	9.51E+02	90%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T03-C	1	1.70E+01			1.70E+01	8.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T04-C	1	1.41E+01			1.41E+01	3.4E+02	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T05-C	1	6.36E+01			6.36E+01	1.8E+01	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T06-C	1	5.75E+01			5.75E+01	3.4E+01	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T07-C	1	4.17E+01			4.17E+01	4.4E+01	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T08-C	1	1.08E+02			1.08E+02	5.9E+00	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-T09-C	1	1.06E+04			1.06E+04	3.6E+01	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	1.5E+02	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-B02-A	1	1.54E+01			1.54E+01	8.0E+01	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-B03-A	1	5.84E+01			5.84E+01	1.4E+01	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-B01-B	1	8.63E+00	E		8.63E+00	9.7E+01	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-B02-B	1	4.00E+00	E		4.00E+00	2.0E+02	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-B03-B	1	2.18E+01			2.18E+01	4.9E+01	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-B01-C	1	1.14E+01	E		1.14E+01	8.3E+01	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-B02-C	1	8.46E+00	E		8.46E+00	1.1E+02	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1313-B03-C	1	2.30E+01			2.30E+01	7.9E+01	3.7E+00	1.2E+01					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	SWA-L05-1313-T01-A	1	2.28E+06			2.28E+06	4.0E-01	1.6E+00	5.1E+00			---		VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T02-A	1	2.39E+05			2.39E+05	9.7E-01	1.6E+00	5.1E+00	1000	100	2.40E+05	87%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T03-A	1	3.00E+05			3.00E+05	4.0E-01	1.6E+00	5.1E+00			---		VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T04-A	1	3.10E+05			3.10E+05	1.1E+00	1.6E+00	5.1E+00			---		VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T05-A	1	3.99E+05			3.99E+05	1.8E-01	1.6E+00	5.1E+00			---		VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T06-A	1	2.38E+05			2.38E+05	1.1E-01	1.6E+00	5.1E+00			---		VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T07-A	1	5.24E+05			5.24E+05	5.1E+00	1.6E+00	5.1E+00			---		VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T08-A	1	2.99E+05			2.99E+05	1.2E+00	1.6E+00	5.1E+00			---		VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T09-A	1	2.43E+05			2.43E+05	2.5E+00	1.6E+00	5.1E+00					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T01-B	1	2.25E+06			2.25E+06	5.8E-01	1.6E+00	5.1E+00			---		VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T02-B	1	2.41E+05			2.41E+05	5.8E-01	1.6E+00	5.1E+00	1000	100	2.42E+05	93%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T03-B	1	2.94E+05			2.94E+05	1.1E+00	1.6E+00	5.1E+00			---		VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T04-B	1	3.14E+05			3.14E+05	9.7E-01	1.6E+00	5.1E+00			---		VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T05-B	1	4.06E+05			4.06E+05	4.8E+01	1.6E+00	5.1E+00			---		VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T06-B	1	2.36E+05			2.36E+05	5.6E-01	1.6E+00	5.1E+00			---		VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T07-B	1	3.54E+05			3.54E+05	5.6E-01	1.6E+00	5.1E+00			---		VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T08-B	1	2.00E+05			2.00E+05	4.6E+00	1.6E+00	5.1E+00			---		VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T09-B	1	2.14E+05			2.14E+05	4.2E+00	1.6E+00	5.1E+00			---		VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T01-C	1	2.23E+06			2.23E+06	7.8E-01	1.6E+00	5.1E+00			---		VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T02-C	1	2.37E+05			2.37E+05	1.2E+00	1.6E+00	5.1E+00	1000	100	2.38E+05	93%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T03-C	1	2.96E+05			2.96E+05	8.5E-01	1.6E+00	5.1E+00			---		VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T04-C	1	3.17E+05			3.17E+05	7.3E-01	1.6E+00	5.1E+00					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T05-C	1	4.06E+05			4.06E+05	5.4E-01	1.6E+00	5.1E+00					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T06-C	1	2.37E+05			2.37E+05	5.1E-01	1.6E+00	5.1E+00					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T07-C	1	3.51E+05			3.51E+05	3.6E-01	1.6E+00	5.1E+00					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T08-C	1	2.04E+05			2.04E+05	5.9E+00	1.6E+00	5.1E+00					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-T09-C	1	1.79E+05			1.79E+05	6.9E+00	1.6E+00	5.1E+00					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-B01-A	1	1.24E+01			1.24E+01	1.3E+01	1.6E+00	5.1E+00					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-B02-A	1	1.42E+02			1.42E+02	8.5E+01	1.6E+00	5.1E+00					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-B03-A	1	2.26E+06			2.26E+06	1.0E+00	1.6E+00	5.1E+00					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-B01-B	1	2.06E+02			2.06E+02	6.4E+00	1.6E+00	5.1E+00					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-B02-B	1	9.92E+01			9.92E+01	8.3E+00	1.6E+00	5.1E+00					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-B03-B	1	2.25E+06			2.25E+06	3.7E-01	1.6E+00	5.1E+00					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-B01-C	1	2.56E+02			2.56E+02	7.9E+00	1.6E+00	5.1E+00					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-B02-C	1	4.73E+02			4.73E+02	5.6E+00	1.6E+00	5.1E+00					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1313-B03-C	1	2.24E+06			2.24E+06	4.1E-01	1.6E+00	5.1E+00					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	SWA-L05-1313-T01-A	1	6.45E+04			6.45E+04	4.9E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T02-A	1	6.44E+04			6.44E+04	6.3E-01	1.5E+01	4.8E+01	10	100	6.54E+04	95%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T03-A	1	6.36E+04			6.36E+04	4.1E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T04-A	1	6.54E+04			6.54E+04	4.4E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T05-A	1	6.95E+04			6.95E+04	4.6E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T06-A	1	6.38E+04			6.38E+04	4.4E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T07-A	1	1.24E+05			1.24E+05	2.3E+00	1.5E+01	4.8E+01			---		VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T08-A	1	6.41E+04			6.41E+04	4.9E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T09-A	1	3.93E+04			3.93E+04	4.3E+00	1.5E+01	4.8E+01					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T01-B	1	6.29E+04			6.29E+04	9.5E-02	1.5E+01	4.8E+01			---		VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T02-B	1	6.40E+04			6.40E+04	3.3E-01	1.5E+01	4.8E+01	10	100	6.49E+04	91%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T03-B	1	6.32E+04			6.32E+04	7.3E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T04-B	1	6.75E+04			6.75E+04	1.9E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T05-B	1	7.14E+04			7.14E+04	5.7E+01	1.5E+01	4.8E+01			---		VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T06-B	1	6.24E+04			6.24E+04	2.3E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T07-B	1	8.20E+04			8.20E+04	5.0E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T08-B	1	3.76E+04			3.76E+04	6.1E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T09-B	1	2.76E+04			2.76E+04	4.9E+00	1.5E+01	4.8E+01			---		VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T01-C	1	6.04E+04			6.04E+04	2.8E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T02-C	1	6.36E+04			6.36E+04	2.5E+00	1.5E+01	4.8E+01	10	100	6.46E+04	97%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T03-C	1	6.39E+04			6.39E+04	2.7E-01	1.5E+01	4.8E+01			---		VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T04-C	1	6.95E+04			6.95E+04	3.7E-01	1.5E+01	4.8E+01					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T05-C	1	7.04E+04			7.04E+04	2.4E-01	1.5E+01	4.8E+01					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T06-C	1	6.47E+04			6.47E+04	1.4E-01	1.5E+01	4.8E+01					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T07-C	1	8.22E+04			8.22E+04	1.7E-01	1.5E+01	4.8E+01					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T08-C	1	3.91E+04			3.91E+04	2.3E-01	1.5E+01	4.8E+01					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-T09-C	1	2.34E+04			2.34E+04	1.1E+01	1.5E+01	4.8E+01					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-B01-A	1	7.50E+00	U1/2		7.50E+00	4.1E+02	1.5E+01	4.8E+01					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-B02-A	1	7.50E+00	U1/2		7.50E+00	1.4E+02	1.5E+01	4.8E+01					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-B03-A	1	7.50E+00	U1/2		7.50E+00	6.1E+01	1.5E+01	4.8E+01					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-B01-B	1	7.50E+00	U1/2		7.50E+00	8.7E+01	1.5E+01	4.8E+01					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-B02-B	1	7.50E+00	U1/2		7.50E+00	1.6E+02	1.5E+01	4.8E+01					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-B03-B	1	7.50E+00	U1/2		7.50E+00	1.9E+02	1.5E+01	4.8E+01					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-B01-C	1	7.50E+00	U1/2		7.50E+00	2.6E+01	1.5E+01	4.8E+01					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-B02-C	1	1.02E+02			1.02E+02	1.4E+01	1.5E+01	4.8E+01					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1313-B03-C	1	7.50E+00	U1/2		7.50E+00	1.5E+02	1.5E+01	4.8E+01					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	SWA-L05-1313-T01-A	1	4.24E+04			4.24E+04	3.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T02-A	1	2.24E+04			2.24E+04	6.8E-01	1.1E+00	3.5E+00	1000	100	2.33E+04	94%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T03-A	1	8.15E+03			8.15E+03	8.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T04-A	1	9.90E+03			9.90E+03	6.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T05-A	1	2.44E+04			2.44E+04	1.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T06-A	1	2.23E+04			2.23E+04	1.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T07-A	1	6.08E+03			6.08E+03	2.4E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T08-A	1	2.87E+04			2.87E+04	2.6E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T09-A	1	1.76E+06			1.76E+06	4.4E+00	1.1E+00	3.5E+00					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T01-B	1	4.40E+04			4.40E+04	1.7E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T02-B	1	2.24E+04			2.24E+04	1.1E+00	1.1E+00	3.5E+00	1000	100	2.33E+04	96%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T03-B	1	5.50E+03			5.50E+03	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T04-B	1	1.13E+04			1.13E+04	1.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T05-B	1	2.36E+04			2.36E+04	5.4E+01	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T06-B	1	2.17E+04			2.17E+04	6.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T07-B	1	8.85E+03			8.85E+03	4.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T08-B	1	5.60E+04			5.60E+04	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T09-B	1	4.24E+05			4.24E+05	4.7E+01	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T01-C	1	4.25E+04			4.25E+04	1.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T02-C	1	2.23E+04			2.23E+04	1.8E+00	1.1E+00	3.5E+00	1000	100	2.33E+04	98%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T03-C	1	8.13E+03			8.13E+03	3.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T04-C	1	8.03E+03			8.03E+03	4.1E-01	1.1E+00	3.5E+00					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T05-C	1	2.38E+04			2.38E+04	9.0E-02	1.1E+00	3.5E+00					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T06-C	1	2.21E+04			2.21E+04	1.1E+00	1.1E+00	3.5E+00					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T07-C	1	1.70E+04			1.70E+04	3.7E-01	1.1E+00	3.5E+00					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T08-C	1	6.14E+04			6.14E+04	4.8E-01	1.1E+00	3.5E+00					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-T09-C	1	2.44E+05			2.44E+05	4.6E+01	1.1E+00	3.5E+00					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-B01-A	1	8.91E+00			8.91E+00	2.7E+01	1.1E+00	3.5E+00					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-B02-A	1	8.38E+00			8.38E+00	2.2E+02	1.1E+00	3.5E+00					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-B03-A	1	6.35E+03			6.35E+03	5.7E+00	1.1E+00	3.5E+00					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-B01-B	1	7.07E+01			7.07E+01	1.6E+01	1.1E+00	3.5E+00					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-B02-B	1	2.17E+01			2.17E+01	1.4E+01	1.1E+00	3.5E+00					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-B03-B	1	3.59E+03			3.59E+03	1.1E+01	1.1E+00	3.5E+00					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-B01-C	1	2.59E+01			2.59E+01	9.2E+00	1.1E+00	3.5E+00					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-B02-C	1	2.28E+01			2.28E+01	1.3E+01	1.1E+00	3.5E+00					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1313-B03-C	1	1.64E+03			1.64E+03	6.9E+00	1.1E+00	3.5E+00					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	SWA-L05-1313-T01-A	1	3.69E+05			3.69E+05	1.6E-01	2.5E+00	8.0E+00			---		VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T02-A	1	3.91E+05			3.91E+05	4.1E-02	2.5E+00	8.0E+00	1000	100	3.92E+05	86%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T03-A	1	4.12E+05			4.12E+05	2.6E-01	2.5E+00	8.0E+00			---		VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T04-A	1	4.11E+05			4.11E+05	3.8E-01	2.5E+00	8.0E+00			---		VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T05-A	1	3.98E+05			3.98E+05	1.7E-01	2.5E+00	8.0E+00			---		VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T06-A	1	3.89E+05			3.89E+05	1.1E-01	2.5E+00	8.0E+00			---		VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T07-A	1	4.98E+05			4.98E+05	2.6E-01	2.5E+00	8.0E+00			---		VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T08-A	1	4.00E+05			4.00E+05	5.0E-01	2.5E+00	8.0E+00			---		VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T09-A	1	5.46E+05			5.46E+05	2.4E+00	2.5E+00	8.0E+00					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T01-B	1	3.64E+05			3.64E+05	2.8E-01	2.5E+00	8.0E+00			---		VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T02-B	1	3.87E+05			3.87E+05	1.7E-01	2.5E+00	8.0E+00	1000	100	3.88E+05	90%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T03-B	1	4.06E+05			4.06E+05	1.2E-01	2.5E+00	8.0E+00			---		VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T04-B	1	4.11E+05			4.11E+05	6.7E-02	2.5E+00	8.0E+00			---		VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T05-B	1	3.97E+05			3.97E+05	5.9E+01	2.5E+00	8.0E+00			---		VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T06-B	1	3.85E+05			3.85E+05	2.5E-01	2.5E+00	8.0E+00			---		VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T07-B	1	4.00E+05			4.00E+05	1.4E-01	2.5E+00	8.0E+00			---		VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T08-B	1	3.92E+05			3.92E+05	1.5E-01	2.5E+00	8.0E+00			---		VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T09-B	1	4.63E+05			4.63E+05	9.6E-01	2.5E+00	8.0E+00			---		VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T01-C	1	3.59E+05			3.59E+05	7.2E-01	2.5E+00	8.0E+00			---		VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T02-C	1	3.83E+05			3.83E+05	4.1E-01	2.5E+00	8.0E+00	1000	100	3.84E+05	89%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T03-C	1	4.07E+05			4.07E+05	3.9E-01	2.5E+00	8.0E+00			---		VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T04-C	1	4.09E+05			4.09E+05	1.7E-01	2.5E+00	8.0E+00					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T05-C	1	3.93E+05			3.93E+05	5.3E-01	2.5E+00	8.0E+00					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T06-C	1	3.83E+05			3.83E+05	4.4E-01	2.5E+00	8.0E+00					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T07-C	1	3.98E+05			3.98E+05	1.8E-01	2.5E+00	8.0E+00					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T08-C	1	3.90E+05			3.90E+05	2.5E-01	2.5E+00	8.0E+00					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-T09-C	1	4.15E+05			4.15E+05	5.7E+00	2.5E+00	8.0E+00					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-B01-A	1	1.25E+00	U1/2		1.25E+00	1.5E+01	2.5E+00	8.0E+00					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-B02-A	1	1.25E+00	U1/2		1.25E+00	9.7E+01	2.5E+00	8.0E+00					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-B03-A	1	1.71E+04			1.71E+04	8.0E-01	2.5E+00	8.0E+00					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-B01-B	1	1.25E+00	U1/2		1.25E+00	1.1E+01	2.5E+00	8.0E+00					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-B02-B	1	1.25E+00	U1/2		1.25E+00	1.1E+01	2.5E+00	8.0E+00					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-B03-B	1	1.72E+04			1.72E+04	4.5E-01	2.5E+00	8.0E+00					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-B01-C	1	1.25E+00	U1/2		1.25E+00	1.3E+01	2.5E+00	8.0E+00					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-B02-C	1	2.49E+03			2.49E+03	3.5E-01	2.5E+00	8.0E+00					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1313-B03-C	1	1.68E+04			1.68E+04	1.0E-01	2.5E+00	8.0E+00					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	SWA-L05-1313-T01-A	1	3.14E+02			3.14E+02	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T02-A	1	2.09E+02			2.09E+02	9.1E-02	1.0E+00	3.2E+00	1000	100	1.21E+03	100%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T03-A	1	5.82E+03			5.82E+03	5.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T04-A	1	1.11E+04			1.11E+04	5.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T05-A	1	2.42E+02			2.42E+02	7.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T06-A	1	2.10E+02			2.10E+02	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T07-A	1	2.52E+04			2.52E+04	2.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T08-A	1	2.77E+04			2.77E+04	1.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T09-A	1	2.95E+04			2.95E+04	2.7E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T01-B	1	3.13E+02			3.13E+02	7.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T02-B	1	2.14E+02			2.14E+02	1.4E+00	1.0E+00	3.2E+00	1000	100	1.23E+03	102%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T03-B	1	5.85E+03			5.85E+03	5.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T04-B	1	1.12E+04			1.12E+04	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T05-B	1	2.45E+02			2.45E+02	8.8E+01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T06-B	1	2.20E+02			2.20E+02	5.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T07-B	1	2.64E+04			2.64E+04	5.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T08-B	1	1.99E+04			1.99E+04	8.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T09-B	1	2.35E+04			2.35E+04	2.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T01-C	1	3.18E+02			3.18E+02	3.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T02-C	1	2.15E+02			2.15E+02	2.7E+00	1.0E+00	3.2E+00	1000	100	1.17E+03	95%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T03-C	1	5.87E+03			5.87E+03	1.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T04-C	1	1.15E+04			1.15E+04	8.6E-01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T05-C	1	2.48E+02			2.48E+02	2.5E-01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T06-C	1	2.18E+02			2.18E+02	1.6E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T07-C	1	2.68E+04			2.68E+04	7.9E-01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T08-C	1	2.05E+04			2.05E+04	2.0E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-T09-C	1	1.84E+04			1.84E+04	4.2E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	5.0E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	2.2E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	1.6E+02	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	2.7E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	5.2E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	9.2E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	6.6E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-B02-C	1	2.34E+01			2.34E+01	2.2E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	7.6E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	SWA-L05-1313-T01-A	1	2.50E+05			2.50E+05	3.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T02-A	1	2.80E+05			2.80E+05	3.3E-01	6.8E+00	2.2E+01	1000	100	2.81E+05	89%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T03-A	1	2.32E+05			2.32E+05	4.9E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T04-A	1	2.39E+05			2.39E+05	3.9E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T05-A	1	2.85E+05			2.85E+05	4.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T06-A	1	2.77E+05			2.77E+05	4.3E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T07-A	1	4.35E+05			4.35E+05	2.6E+00	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T08-A	1	2.81E+05			2.81E+05	2.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T09-A	1	2.05E+05			2.05E+05	3.4E+00	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T01-B	1	2.45E+05			2.45E+05	1.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T02-B	1	2.74E+05			2.74E+05	2.8E-01	6.8E+00	2.2E+01	1000	100	2.75E+05	87%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T03-B	1	2.32E+05			2.32E+05	7.3E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T04-B	1	2.45E+05			2.45E+05	3.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T05-B	1	2.88E+05			2.88E+05	5.4E+01	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T06-B	1	2.68E+05			2.68E+05	5.5E-02	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T07-B	1	3.29E+05			3.29E+05	4.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T08-B	1	1.77E+05			1.77E+05	2.8E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T09-B	1	1.55E+05			1.55E+05	4.4E+00	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T01-C	1	2.34E+05			2.34E+05	6.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T02-C	1	2.76E+05			2.76E+05	2.3E+00	6.8E+00	2.2E+01	1000	100	2.77E+05	86%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T03-C	1	2.35E+05			2.35E+05	3.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T04-C	1	2.51E+05			2.51E+05	3.4E-01	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T05-C	1	2.89E+05			2.89E+05	4.9E-01	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T06-C	1	2.79E+05			2.79E+05	4.9E-01	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T07-C	1	3.26E+05			3.26E+05	6.6E-01	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T08-C	1	1.86E+05			1.86E+05	3.7E-01	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-T09-C	1	1.31E+05			1.31E+05	1.0E+01	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	9.1E+00	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	4.3E+01	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	3.7E+01	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-B01-B	1	3.40E+00	U1/2		3.40E+00	1.3E+01	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-B02-B	1	3.40E+00	U1/2		3.40E+00	1.3E+01	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-B03-B	1	3.40E+00	U1/2		3.40E+00	4.6E+01	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-B01-C	1	3.40E+00	U1/2		3.40E+00	1.1E+01	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-B02-C	1	2.43E+02			2.43E+02	1.0E+01	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1313-B03-C	1	3.40E+00	U1/2		3.40E+00	3.2E+01	6.8E+00	2.2E+01					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

TI	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
TI	SWA-L05-1313-T01-A	1	2.30E+00	U1/2		2.30E+00	4.8E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T02-A	1	2.30E+00	U1/2		2.30E+00	2.9E+02	4.6E+00	1.5E+01	10	100	8.82E+02	88%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T03-A	1	2.30E+00	U1/2		2.30E+00	1.2E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T04-A	1	2.30E+00	U1/2		2.30E+00	6.0E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T05-A	1	2.30E+00	U1/2		2.30E+00	2.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T06-A	1	2.30E+00	U1/2		2.30E+00	7.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T07-A	1	8.10E+00	E		8.10E+00	9.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T08-A	1	1.63E+01			1.63E+01	9.5E+00	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T09-A	1	2.30E+00	U1/2		2.30E+00	5.2E+01	4.6E+00	1.5E+01					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T01-B	1	2.30E+00	U1/2		2.30E+00	1.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T02-B	1	2.30E+00	U1/2		2.30E+00	3.2E+02	4.6E+00	1.5E+01	10	100	8.53E+02	85%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T03-B	1	2.30E+00	U1/2		2.30E+00	4.5E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T04-B	1	2.30E+00	U1/2		2.30E+00	2.5E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T05-B	1	2.30E+00	U1/2		2.30E+00	2.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T06-B	1	2.30E+00	U1/2		2.30E+00	3.8E+01	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T07-B	1	9.06E+00	E		9.06E+00	4.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T08-B	1	1.21E+01	E		1.21E+01	4.4E+01	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T09-B	1	2.30E+00	U1/2		2.30E+00	1.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T01-C	1	2.30E+00	U1/2		2.30E+00	1.3E+03	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T02-C	1	2.30E+00	U1/2		2.30E+00	1.6E+02	4.6E+00	1.5E+01	10	100	8.74E+02	87%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T03-C	1	2.30E+00	U1/2		2.30E+00	6.8E+01	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T04-C	1	2.30E+00	U1/2		2.30E+00	2.9E+02	4.6E+00	1.5E+01					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T05-C	1	2.30E+00	U1/2		2.30E+00	3.3E+01	4.6E+00	1.5E+01					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T06-C	1	2.30E+00	U1/2		2.30E+00	1.7E+02	4.6E+00	1.5E+01					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T07-C	1	8.31E+00	E		8.31E+00	2.4E+01	4.6E+00	1.5E+01					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T08-C	1	1.49E+01			1.49E+01	1.9E+01	4.6E+00	1.5E+01					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-T09-C	1	2.30E+00	U1/2		2.30E+00	1.2E+01	4.6E+00	1.5E+01					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	7.1E+01	4.6E+00	1.5E+01					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	2.5E+01	4.6E+00	1.5E+01					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	7.0E+01	4.6E+00	1.5E+01					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-B01-B	1	2.30E+00	U1/2		2.30E+00	1.9E+01	4.6E+00	1.5E+01					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-B02-B	1	2.30E+00	U1/2		2.30E+00	6.4E+02	4.6E+00	1.5E+01					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-B03-B	1	6.47E+00	E		6.47E+00	2.6E+01	4.6E+00	1.5E+01					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-B01-C	1	2.30E+00	U1/2		2.30E+00	5.4E+01	4.6E+00	1.5E+01					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-B02-C	1	2.30E+00	U1/2		2.30E+00	1.3E+01	4.6E+00	1.5E+01					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
TI	SWA-L05-1313-B03-C	1	2.30E+00	U1/2		2.30E+00	8.4E+01	4.6E+00	1.5E+01					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	SWA-L05-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.0E+00	6.4E+00	10	100	9.34E+02	93%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	2.3E+02	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	5.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	2.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	2.6E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T08-A	1	1.00E+00	U1/2		1.00E+00	8.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T09-A	1	5.36E+04			5.36E+04	6.3E+00	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	2.6E+01	2.0E+00	6.4E+00	10	100	9.27E+02	93%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	9.5E+02	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	1.9E+02	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	5.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	3.6E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	1.9E+02	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T08-B	1	1.10E+01			1.10E+01	5.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T09-B	1	1.58E+04			1.58E+04	4.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	4.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	3.9E+01	2.0E+00	6.4E+00	10	100	9.35E+02	93%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	3.2E+02	2.0E+00	6.4E+00			---		VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	1.8E+02	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	3.4E+01	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	3.3E+01	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	1.5E+02	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T08-C	1	4.84E+01			4.84E+01	1.2E+00	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-T09-C	1	1.07E+04			1.07E+04	3.4E+01	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	8.7E+02	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-B03-A	1	1.05E+01			1.05E+01	8.7E+00	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-B02-B	1	2.29E+00	E		2.29E+00	1.1E+01	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	3.3E+00	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1313-B03-C	1	1.00E+00	U1/2		1.00E+00	1.3E+01	2.0E+00	6.4E+00					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	SWA-L05-1313-T01-A	1	3.62E+02			3.62E+02	1.3E+00	1.5E+00	4.8E+00			---		VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T02-A	1	2.93E+02			2.93E+02	4.5E-01	1.5E+00	4.8E+00	10	100	1.17E+03	88%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T03-A	1	9.05E+01			9.05E+01	1.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T04-A	1	1.16E+02			1.16E+02	5.5E+00	1.5E+00	4.8E+00			---		VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T05-A	1	3.14E+02			3.14E+02	1.3E+00	1.5E+00	4.8E+00			---		VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T06-A	1	2.87E+02			2.87E+02	8.1E-01	1.5E+00	4.8E+00			---		VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T07-A	1	1.80E+02			1.80E+02	1.7E+00	1.5E+00	4.8E+00			---		VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T08-A	1	1.32E+02			1.32E+02	3.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T09-A	1	2.09E+03			2.09E+03	1.9E+00	1.5E+00	4.8E+00					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T01-B	1	3.61E+02			3.61E+02	1.0E+00	1.5E+00	4.8E+00			---		VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T02-B	1	2.83E+02			2.83E+02	1.4E+00	1.5E+00	4.8E+00	10	100	1.16E+03	88%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T03-B	1	8.67E+01			8.67E+01	9.7E-01	1.5E+00	4.8E+00			---		VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T04-B	1	1.19E+02			1.19E+02	3.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T05-B	1	3.10E+02			3.10E+02	4.5E+01	1.5E+00	4.8E+00			---		VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T06-B	1	2.76E+02			2.76E+02	5.7E-01	1.5E+00	4.8E+00			---		VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T07-B	1	1.61E+02			1.61E+02	1.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T08-B	1	7.84E+01			7.84E+01	1.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T09-B	1	1.59E+03			1.59E+03	5.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T01-C	1	3.38E+02			3.38E+02	7.9E-01	1.5E+00	4.8E+00			---		VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T02-C	1	2.83E+02			2.83E+02	2.6E+00	1.5E+00	4.8E+00	10	100	1.21E+03	92%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T03-C	1	8.96E+01			8.96E+01	1.7E+00	1.5E+00	4.8E+00			---		VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T04-C	1	1.12E+02			1.12E+02	7.4E-01	1.5E+00	4.8E+00					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T05-C	1	3.19E+02			3.19E+02	1.7E+00	1.5E+00	4.8E+00					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T06-C	1	2.87E+02			2.87E+02	9.0E-01	1.5E+00	4.8E+00					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T07-C	1	1.51E+02			1.51E+02	2.9E-01	1.5E+00	4.8E+00					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T08-C	1	8.67E+01			8.67E+01	1.3E+00	1.5E+00	4.8E+00					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-T09-C	1	1.19E+03			1.19E+03	9.4E+00	1.5E+00	4.8E+00					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-B01-A	1	7.50E-01	U1/2		7.50E-01	3.3E+01	1.5E+00	4.8E+00					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-B02-A	1	7.50E-01	U1/2		7.50E-01	2.3E+01	1.5E+00	4.8E+00					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-B03-A	1	2.82E+00	E		2.82E+00	1.9E+01	1.5E+00	4.8E+00					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-B01-B	1	7.50E-01	U1/2		7.50E-01	2.5E+01	1.5E+00	4.8E+00					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-B02-B	1	2.50E+00	E		2.50E+00	5.1E+01	1.5E+00	4.8E+00					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-B03-B	1	2.31E+00	E		2.31E+00	2.0E+01	1.5E+00	4.8E+00					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-B01-C	1	7.50E-01	U1/2		7.50E-01	6.0E+01	1.5E+00	4.8E+00					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-B02-C	1	2.02E+00	E		2.02E+00	3.6E+01	1.5E+00	4.8E+00					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1313-B03-C	1	2.23E+00	E		2.23E+00	6.8E+01	1.5E+00	4.8E+00					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	SWA-L05-1313-T01-A	1	1.05E+01			1.05E+01	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 12:48 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T02-A	1	2.39E+00	E		2.39E+00	1.1E+01	1.0E+00	3.2E+00	10	100	9.96E+02	99%	VU ICP-OES	3/7/11 12:50 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T03-A	1	5.00E-01	U1/2		5.00E-01	5.3E+01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 12:52 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T04-A	1	1.13E+00	E		1.13E+00	1.4E+01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 12:53 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T05-A	1	2.11E+00	E		2.11E+00	9.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 12:55 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T06-A	1	2.93E+00	E		2.93E+00	5.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 12:57 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T07-A	1	3.15E+00	E		3.15E+00	1.5E+01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 12:58 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T08-A	1	5.86E+02			5.86E+02	3.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:00 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T09-A	1	2.10E+03			2.10E+03	1.6E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:02 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T01-B	1	8.34E+00			8.34E+00	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:13 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T02-B	1	1.80E+00	E		1.80E+00	5.1E+00	1.0E+00	3.2E+00	10	100	9.41E+02	94%	VU ICP-OES	3/7/11 1:15 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T03-B	1	5.00E-01	U1/2		5.00E-01	1.9E+01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:16 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T04-B	1	1.44E+00	E		1.44E+00	2.9E+01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:18 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T05-B	1	1.91E+00	E		1.91E+00	1.3E+02	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:20 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T06-B	1	2.06E+00	E		2.06E+00	7.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:21 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T07-B	1	2.88E+00	E		2.88E+00	1.4E+01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:23 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T08-B	1	1.22E+03			1.22E+03	2.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:25 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T09-B	1	1.69E+03			1.69E+03	4.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:26 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T01-C	1	7.16E+00			7.16E+00	2.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:28 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T02-C	1	2.24E+00	E		2.24E+00	5.5E+00	1.0E+00	3.2E+00	10	100	9.63E+02	96%	VU ICP-OES	3/7/11 1:30 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T03-C	1	5.00E-01	U1/2		5.00E-01	7.6E+01	1.0E+00	3.2E+00			---		VU ICP-OES	3/7/11 1:31 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T04-C	1	1.09E+00	E		1.09E+00	1.3E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:33 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T05-C	1	1.61E+00	E		1.61E+00	3.3E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:35 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T06-C	1	2.12E+00	E		2.12E+00	1.0E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:36 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T07-C	1	2.49E+00	E		2.49E+00	2.9E-01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:38 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T08-C	1	1.18E+03			1.18E+03	8.7E-01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:40 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-T09-C	1	1.38E+03			1.38E+03	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 1:41 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	8.9E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:34 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-B02-A	1	2.12E+00	E		2.12E+00	1.2E+02	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:35 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-B03-A	1	1.98E+00	E		1.98E+00	4.7E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:37 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	1.7E+03	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:39 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-B02-B	1	2.97E+00	E		2.97E+00	5.2E+00	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:40 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-B03-B	1	2.63E+00	E		2.63E+00	1.6E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:42 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	1.2E+02	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:43 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-B02-C	1	3.66E+00			3.66E+00	5.3E-01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:45 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1313-B03-C	1	3.69E+00			3.69E+00	1.6E+01	1.0E+00	3.2E+00					VU ICP-OES	3/7/11 12:47 PM	EPA Interlab L05 1313-1316 SWA

QA-QC Spreadsheet 1313:

										Spike Sol'n						
Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Conc. µg/L	Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	SWA-L06-1313-T01-A	1	1.64E+05			1.64E+05	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T02-A	1	1.19E+04			1.19E+04	7.6E+00	1.0E+00	3.2E+00	1000	100	1.29E+04	97%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T03-A	1	4.26E+02			4.26E+02	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T04-A	1	9.73E+01			9.73E+01	3.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T05-A	1	4.18E+01			4.18E+01	2.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T06-A	1	8.28E+00			8.28E+00	4.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T07-A	1	3.73E+02			3.73E+02	4.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T08-A	1	2.69E+05			2.69E+05	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T09-A	1	4.80E+05			4.80E+05	7.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T10-A	1	3.86E+04			3.86E+04	4.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T01-B	1	1.66E+05			1.66E+05	5.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T02-B	1	1.27E+04			1.27E+04	7.1E-01	1.0E+00	3.2E+00	1000	100	1.38E+04	104%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T03-B	1	4.93E+02			4.93E+02	3.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T04-B	1	1.09E+02			1.09E+02	5.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T05-B	1	5.07E+01			5.07E+01	9.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T06-B	1	8.17E+00			8.17E+00	1.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T07-B	1	4.63E+02			4.63E+02	3.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T08-B	1	2.89E+05			2.89E+05	2.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T09-B	1	7.71E+05			7.71E+05	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T10-B	1	3.98E+04			3.98E+04	1.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T01-C	1	1.58E+05			1.58E+05	3.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T02-C	1	1.33E+04			1.33E+04	1.4E+00	1.0E+00	3.2E+00	1000	100	1.42E+04	90%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T03-C	1	5.12E+02			5.12E+02	8.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T04-C	1	1.10E+02			1.10E+02	1.5E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T05-C	1	5.14E+01			5.14E+01	2.1E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T06-C	1	9.59E+00			9.59E+00	1.7E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T07-C	1	3.01E+02			3.01E+02	5.5E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T08-C	1	2.89E+05			2.89E+05	3.1E-01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T09-C	1	7.59E+05			7.59E+05	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-T10-C	1	3.91E+04			3.91E+04	1.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-B01-A	1	3.84E+04			3.84E+04	5.2E-01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-B02-A	1	2.57E+00	E		2.57E+00	8.5E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-B03-A	1	8.98E+00			8.98E+00	6.0E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-B01-B	1	1.83E+00	E		1.83E+00	9.3E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-B02-B	1	7.85E+00			7.85E+00	2.9E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-B03-B	1	9.23E+00			9.23E+00	3.7E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-B01-C	1	2.86E+00	E		2.86E+00	1.0E+02	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1313-B02-C	1	3.37E+00			3.37E+00	6.0E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	SWA-L06-1313-T01-A	1	1.34E+03			1.34E+03	1.4E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T02-A	1	2.81E+03			2.81E+03	7.3E+00	7.5E+00	2.4E+01	10	100	3.88E+03	107%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T03-A	1	1.27E+03			1.27E+03	6.3E-01	7.5E+00	2.4E+01			---		VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T04-A	1	1.33E+03			1.33E+03	4.4E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T05-A	1	1.26E+03			1.26E+03	1.2E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T06-A	1	1.03E+03			1.03E+03	1.3E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T07-A	1	7.68E+02			7.68E+02	2.4E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T08-A	1	2.69E+02			2.69E+02	2.7E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T09-A	1	2.41E+04			2.41E+04	6.7E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T10-A	1	4.07E+03			4.07E+03	4.8E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T01-B	1	1.31E+03			1.31E+03	1.9E-01	7.5E+00	2.4E+01			---		VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T02-B	1	3.11E+03			3.11E+03	3.4E-01	7.5E+00	2.4E+01	10	100	4.01E+03	90%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T03-B	1	1.09E+03			1.09E+03	4.1E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T04-B	1	1.39E+03			1.39E+03	1.4E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T05-B	1	1.15E+03			1.15E+03	1.2E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T06-B	1	9.57E+02			9.57E+02	9.4E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T07-B	1	7.56E+02			7.56E+02	3.3E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T08-B	1	2.45E+02			2.45E+02	3.0E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T09-B	1	3.77E+04			3.77E+04	1.3E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T10-B	1	4.42E+03			4.42E+03	2.3E-01	7.5E+00	2.4E+01			---		VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T01-C	1	1.72E+03			1.72E+03	5.1E-01	7.5E+00	2.4E+01			---		VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T02-C	1	3.36E+03			3.36E+03	1.3E+00	7.5E+00	2.4E+01	10	100	4.25E+03	89%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T03-C	1	1.25E+03			1.25E+03	1.0E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T04-C	1	1.45E+03			1.45E+03	1.4E+00	7.5E+00	2.4E+01					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T05-C	1	9.85E+02			9.85E+02	5.4E+00	7.5E+00	2.4E+01					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T06-C	1	9.13E+02			9.13E+02	1.8E+00	7.5E+00	2.4E+01					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T07-C	1	7.25E+02			7.25E+02	7.3E+01	7.5E+00	2.4E+01					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T08-C	1	2.46E+02			2.46E+02	6.2E+00	7.5E+00	2.4E+01					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T09-C	1	2.65E+04			2.65E+04	2.5E+00	7.5E+00	2.4E+01					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-T10-C	1	4.08E+03			4.08E+03	7.7E-01	7.5E+00	2.4E+01			---		VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-B01-A	1	3.96E+03			3.96E+03	1.3E+00	7.5E+00	2.4E+01					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-B02-A	1	3.75E+00	U1/2		3.75E+00	1.9E+02	7.5E+00	2.4E+01					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-B03-A	1	3.75E+00	U1/2		3.75E+00	4.3E+01	7.5E+00	2.4E+01					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-B01-B	1	3.75E+00	U1/2		3.75E+00	6.3E+01	7.5E+00	2.4E+01					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-B02-B	1	3.75E+00	U1/2		3.75E+00	6.4E+01	7.5E+00	2.4E+01					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-B03-B	1	3.75E+00	U1/2		3.75E+00	8.9E+01	7.5E+00	2.4E+01					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-B01-C	1	3.75E+00	U1/2		3.75E+00	6.8E+01	7.5E+00	2.4E+01					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1313-B02-C	1	3.75E+00	U1/2		3.75E+00	1.9E+02	7.5E+00	2.4E+01					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	SWA-L06-1313-T01-A	1	2.26E+04			2.26E+04	2.5E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T02-A	1	8.94E+02			8.94E+02	6.1E+00	1.1E+01	3.5E+01	10	100	2.07E+03	118%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T03-A	1	1.34E+02			1.34E+02	1.4E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T04-A	1	3.41E+02			3.41E+02	7.0E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T05-A	1	2.05E+02			2.05E+02	1.0E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T06-A	1	2.45E+02			2.45E+02	1.3E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T07-A	1	2.78E+02			2.78E+02	2.2E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T08-A	1	1.87E+03			1.87E+03	6.3E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T09-A	1	1.43E+04			1.43E+04	7.1E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T10-A	1	5.18E+03			5.18E+03	5.5E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T01-B	1	2.28E+04			2.28E+04	7.9E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T02-B	1	9.71E+02			9.71E+02	2.0E+00	1.1E+01	3.5E+01	10	100	2.17E+03	119%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T03-B	1	1.25E+02			1.25E+02	1.2E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T04-B	1	3.20E+02			3.20E+02	1.5E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T05-B	1	1.89E+02			1.89E+02	1.6E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T06-B	1	2.63E+02			2.63E+02	9.0E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T07-B	1	3.75E+02			3.75E+02	4.5E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T08-B	1	1.87E+03			1.87E+03	9.9E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T09-B	1	2.25E+04			2.25E+04	2.0E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T10-B	1	5.16E+03			5.16E+03	1.3E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T01-C	1	2.16E+04			2.16E+04	6.8E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T02-C	1	1.01E+03			1.01E+03	2.7E+00	1.1E+01	3.5E+01	10	100	2.20E+03	119%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T03-C	1	1.43E+02			1.43E+02	1.3E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T04-C	1	3.61E+02			3.61E+02	6.9E+00	1.1E+01	3.5E+01					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T05-C	1	1.78E+02			1.78E+02	7.6E+00	1.1E+01	3.5E+01					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T06-C	1	2.28E+02			2.28E+02	1.0E+01	1.1E+01	3.5E+01					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T07-C	1	2.54E+02			2.54E+02	6.1E+01	1.1E+01	3.5E+01					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T08-C	1	1.85E+03			1.85E+03	6.6E-01	1.1E+01	3.5E+01					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T09-C	1	1.65E+04			1.65E+04	1.4E+00	1.1E+01	3.5E+01					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-T10-C	1	5.17E+03			5.17E+03	2.1E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-B01-A	1	5.25E+03			5.25E+03	6.0E-01	1.1E+01	3.5E+01					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-B02-A	1	1.14E+01	E		1.14E+01	2.7E+01	1.1E+01	3.5E+01					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-B03-A	1	1.18E+01	E		1.18E+01	4.0E+01	1.1E+01	3.5E+01					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-B01-B	1	5.50E+00	U1/2		5.50E+00	5.5E+01	1.1E+01	3.5E+01					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-B02-B	1	5.50E+00	U1/2		5.50E+00	5.2E+01	1.1E+01	3.5E+01					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-B03-B	1	5.50E+00	U1/2		5.50E+00	1.9E+01	1.1E+01	3.5E+01					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-B01-C	1	5.50E+00	U1/2		5.50E+00	2.0E+01	1.1E+01	3.5E+01					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1313-B02-C	1	5.50E+00	U1/2		5.50E+00	4.0E+01	1.1E+01	3.5E+01					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	SWA-L06-1313-T01-A	1	1.71E+03			1.71E+03	4.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T02-A	1	6.13E+02			6.13E+02	7.5E+00	1.0E+00	3.2E+00	1000	100	1.76E+03	114%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T03-A	1	1.04E+03			1.04E+03	2.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T04-A	1	1.67E+03			1.67E+03	4.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T05-A	1	2.26E+03			2.26E+03	5.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T06-A	1	3.52E+03			3.52E+03	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T07-A	1	4.90E+03			4.90E+03	4.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T08-A	1	4.88E+03			4.88E+03	5.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T09-A	1	3.67E+03			3.67E+03	6.8E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T10-A	1	1.15E+03			1.15E+03	2.3E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T01-B	1	1.73E+03			1.73E+03	6.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T02-B	1	7.12E+02			7.12E+02	8.2E-01	1.0E+00	3.2E+00	1000	100	1.89E+03	118%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T03-B	1	9.65E+02			9.65E+02	3.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T04-B	1	1.76E+03			1.76E+03	7.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T05-B	1	2.25E+03			2.25E+03	2.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T06-B	1	3.15E+03			3.15E+03	9.0E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T07-B	1	4.94E+03			4.94E+03	9.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T08-B	1	4.75E+03			4.75E+03	5.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T09-B	1	5.02E+03			5.02E+03	1.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T10-B	1	1.15E+03			1.15E+03	3.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T01-C	1	1.70E+03			1.70E+03	1.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T02-C	1	7.14E+02			7.14E+02	6.9E-01	1.0E+00	3.2E+00	1000	100	1.85E+03	114%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T03-C	1	1.05E+03			1.05E+03	4.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T04-C	1	1.74E+03			1.74E+03	7.6E-01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T05-C	1	2.12E+03			2.12E+03	5.4E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T06-C	1	3.20E+03			3.20E+03	2.4E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T07-C	1	4.38E+03			4.38E+03	1.8E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T08-C	1	4.79E+03			4.79E+03	7.4E-01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T09-C	1	4.91E+03			4.91E+03	2.5E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-T10-C	1	1.10E+03			1.10E+03	5.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-B01-A	1	1.11E+03			1.11E+03	1.5E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-B02-A	1	1.89E+01			1.89E+01	2.2E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-B03-A	1	2.45E+01			2.45E+01	1.5E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-B01-B	1	9.80E+00			9.80E+00	3.1E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-B02-B	1	1.25E+01			1.25E+01	1.3E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-B03-B	1	1.17E+01			1.17E+01	1.5E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-B01-C	1	8.54E+00			8.54E+00	6.0E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1313-B02-C	1	9.53E+00			9.53E+00	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	SWA-L06-1313-T01-A	1	6.17E+02			6.17E+02	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T02-A	1	2.74E+02			2.74E+02	6.8E+00	1.0E+00	3.2E+00	10	100	1.23E+03	96%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T03-A	1	9.74E+02			9.74E+02	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T04-A	1	9.93E+02			9.93E+02	3.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T05-A	1	1.09E+03			1.09E+03	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T06-A	1	1.26E+03			1.26E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T07-A	1	1.55E+03			1.55E+03	6.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T08-A	1	6.18E+02			6.18E+02	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T09-A	1	6.93E+02			6.93E+02	6.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T10-A	1	1.63E+02			1.63E+02	5.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T01-B	1	6.15E+02			6.15E+02	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T02-B	1	2.90E+02			2.90E+02	9.7E-02	1.0E+00	3.2E+00	10	100	1.31E+03	102%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T03-B	1	8.34E+02			8.34E+02	4.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T04-B	1	1.00E+03			1.00E+03	9.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T05-B	1	1.06E+03			1.06E+03	2.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T06-B	1	1.25E+03			1.25E+03	8.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T07-B	1	1.48E+03			1.48E+03	9.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T08-B	1	6.13E+02			6.13E+02	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T09-B	1	7.02E+02			7.02E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T10-B	1	1.79E+02			1.79E+02	6.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T01-C	1	5.60E+02			5.60E+02	3.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T02-C	1	3.33E+02			3.33E+02	9.6E-01	1.0E+00	3.2E+00	10	100	1.34E+03	101%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T03-C	1	8.77E+02			8.77E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T04-C	1	1.11E+03			1.11E+03	6.6E-01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T05-C	1	9.68E+02			9.68E+02	5.0E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T06-C	1	1.32E+03			1.32E+03	2.9E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T07-C	1	1.28E+03			1.28E+03	5.2E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T08-C	1	5.95E+02			5.95E+02	2.1E-01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T09-C	1	7.87E+02			7.87E+02	9.4E-01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-T10-C	1	1.59E+02			1.59E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-B01-A	1	1.61E+02			1.61E+02	1.0E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-B02-A	1	1.29E+00	E		1.29E+00	5.5E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-B03-A	1	3.84E+00			3.84E+00	6.6E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	4.7E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	8.5E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	1.2E+02	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	1.0E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	8.7E-01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	SWA-L06-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	2.6E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	7.9E+02	1.9E+00	6.0E+00	10	100	1.14E+03	113%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	2.9E+03	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	5.1E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	5.7E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T07-A	1	9.50E-01	U1/2		9.50E-01	1.6E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T08-A	1	4.15E+01			4.15E+01	1.0E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T09-A	1	7.86E+01			7.86E+01	6.5E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T10-A	1	9.50E-01	U1/2		9.50E-01	9.1E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	2.3E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	6.3E+02	1.9E+00	6.0E+00	10	100	1.12E+03	112%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	3.3E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	2.4E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	4.0E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T07-B	1	9.50E-01	U1/2		9.50E-01	7.2E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T08-B	1	4.51E+01			4.51E+01	7.0E-01	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T09-B	1	1.12E+02			1.12E+02	1.6E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T10-B	1	9.50E-01	U1/2		9.50E-01	6.9E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	3.3E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	7.7E+01	1.9E+00	6.0E+00	10	100	1.14E+03	114%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	8.2E+01	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	3.5E+01	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T07-C	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T08-C	1	4.64E+01			4.64E+01	1.8E+00	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T09-C	1	1.14E+02			1.14E+02	1.6E+00	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-T10-C	1	9.50E-01	U1/2		9.50E-01	1.5E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	1.9E+02	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	1.6E+02	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	1.5E+01	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-B01-B	1	9.50E-01	U1/2		9.50E-01	3.8E+01	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-B02-B	1	9.50E-01	U1/2		9.50E-01	2.0E+04	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-B03-B	1	9.50E-01	U1/2		9.50E-01	2.7E+02	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-B01-C	1	9.50E-01	U1/2		9.50E-01	6.9E+01	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1313-B02-C	1	9.50E-01	U1/2		9.50E-01	1.5E+02	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	SWA-L06-1313-T01-A	1	1.10E+00	U1/2		1.10E+00	7.7E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T02-A	1	1.10E+00	U1/2		1.10E+00	5.3E+01	2.2E+00	7.0E+00	10	100	1.09E+03	109%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	3.2E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T04-A	1	1.10E+00	U1/2		1.10E+00	7.8E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T05-A	1	1.10E+00	U1/2		1.10E+00	2.2E+02	2.2E+00	7.0E+00			---		VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T06-A	1	1.10E+00	U1/2		1.10E+00	4.6E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T07-A	1	7.49E+00			7.49E+00	2.6E+00	2.2E+00	7.0E+00			---		VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T08-A	1	1.61E+01			1.61E+01	2.1E+00	2.2E+00	7.0E+00			---		VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T09-A	1	3.33E+01			3.33E+01	7.0E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T10-A	1	1.10E+00	U1/2		1.10E+00	1.6E+02	2.2E+00	7.0E+00			---		VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T01-B	1	1.10E+00	U1/2		1.10E+00	7.5E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T02-B	1	1.10E+00	U1/2		1.10E+00	7.1E+01	2.2E+00	7.0E+00	10	100	1.17E+03	117%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	8.7E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T04-B	1	1.10E+00	U1/2		1.10E+00	4.5E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T05-B	1	1.10E+00	U1/2		1.10E+00	6.5E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T06-B	1	1.10E+00	U1/2		1.10E+00	9.8E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T07-B	1	9.68E+00			9.68E+00	2.1E+00	2.2E+00	7.0E+00			---		VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T08-B	1	1.60E+01			1.60E+01	1.7E+00	2.2E+00	7.0E+00			---		VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T09-B	1	3.80E+01			3.80E+01	7.7E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T10-B	1	1.10E+00	U1/2		1.10E+00	1.0E+02	2.2E+00	7.0E+00			---		VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T01-C	1	1.10E+00	U1/2		1.10E+00	7.4E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T02-C	1	1.10E+00	U1/2		1.10E+00	1.5E+02	2.2E+00	7.0E+00	10	100	1.19E+03	119%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	2.3E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T04-C	1	1.10E+00	U1/2		1.10E+00	3.2E+01	2.2E+00	7.0E+00					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T05-C	1	1.10E+00	U1/2		1.10E+00	2.4E+01	2.2E+00	7.0E+00					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T06-C	1	1.10E+00	U1/2		1.10E+00	5.5E+01	2.2E+00	7.0E+00					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T07-C	1	1.04E+01			1.04E+01	6.7E+01	2.2E+00	7.0E+00					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T08-C	1	1.58E+01			1.58E+01	1.8E+00	2.2E+00	7.0E+00					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T09-C	1	3.40E+01			3.40E+01	9.0E-01	2.2E+00	7.0E+00					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-T10-C	1	1.10E+00	U1/2		1.10E+00	3.3E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	4.1E+01	2.2E+00	7.0E+00					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	7.2E+01	2.2E+00	7.0E+00					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-B03-A	1	1.10E+00	U1/2		1.10E+00	3.9E+01	2.2E+00	7.0E+00					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-B01-B	1	1.10E+00	U1/2		1.10E+00	6.0E+00	2.2E+00	7.0E+00					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-B02-B	1	1.10E+00	U1/2		1.10E+00	1.3E+02	2.2E+00	7.0E+00					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-B03-B	1	1.10E+00	U1/2		1.10E+00	3.7E+02	2.2E+00	7.0E+00					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-B01-C	1	1.10E+00	U1/2		1.10E+00	4.5E+01	2.2E+00	7.0E+00					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1313-B02-C	1	1.10E+00	U1/2		1.10E+00	2.2E+01	2.2E+00	7.0E+00					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	SWA-L06-1313-T01-A	1	3.59E+03			3.59E+03	4.5E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T02-A	1	4.90E+04			4.90E+04	7.7E+00	2.6E+00	8.3E+00	1000	100	4.99E+04	93%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T03-A	1	2.93E+06			2.93E+06	1.4E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T04-A	1	5.78E+06			5.78E+06	3.9E+00	2.6E+00	8.3E+00			---		VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T05-A	1	7.26E+06			7.26E+06	3.7E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T06-A	1	8.93E+06			8.93E+06	2.0E+00	2.6E+00	8.3E+00			---		VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T07-A	1	9.65E+06			9.65E+06	4.4E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T08-A	1	4.01E+06			4.01E+06	4.3E-02	2.6E+00	8.3E+00			---		VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T09-A	1	2.07E+06			2.07E+06	7.7E+01	2.6E+00	8.3E+00			---		VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T10-A	1	1.26E+04			1.26E+04	6.8E+01	2.6E+00	8.3E+00			---		VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T01-B	1	3.48E+03			3.48E+03	1.4E+00	2.6E+00	8.3E+00			---		VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T02-B	1	5.37E+04			5.37E+04	8.3E-01	2.6E+00	8.3E+00	1000	100	5.46E+04	95%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T03-B	1	2.70E+06			2.70E+06	4.5E+00	2.6E+00	8.3E+00			---		VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T04-B	1	6.01E+06			6.01E+06	5.4E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T05-B	1	7.25E+06			7.25E+06	8.2E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T06-B	1	8.72E+06			8.72E+06	1.4E+02	2.6E+00	8.3E+00			---		VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T07-B	1	9.12E+06			9.12E+06	7.0E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T08-B	1	4.01E+06			4.01E+06	8.6E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T09-B	1	3.15E+06			3.15E+06	5.9E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T10-B	1	1.38E+04			1.38E+04	1.6E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T01-C	1	3.37E+03			3.37E+03	3.9E+00	2.6E+00	8.3E+00			---		VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T02-C	1	5.43E+04			5.43E+04	1.3E+00	2.6E+00	8.3E+00	1000	100	5.52E+04	86%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T03-C	1	2.85E+06			2.85E+06	4.3E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T04-C	1	6.13E+06			6.13E+06	2.1E-01	2.6E+00	8.3E+00					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T05-C	1	6.85E+06			6.85E+06	5.0E+00	2.6E+00	8.3E+00					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T06-C	1	8.63E+06			8.63E+06	2.9E+00	2.6E+00	8.3E+00					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T07-C	1	6.07E+06			6.07E+06	7.8E+01	2.6E+00	8.3E+00					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T08-C	1	3.98E+06			3.98E+06	4.7E-01	2.6E+00	8.3E+00					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T09-C	1	3.17E+06			3.17E+06	6.4E-01	2.6E+00	8.3E+00					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-T10-C	1	1.30E+04			1.30E+04	6.0E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-B01-A	1	1.28E+04			1.28E+04	4.9E-01	2.6E+00	8.3E+00					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-B02-A	1	8.38E+00			8.38E+00	5.2E+00	2.6E+00	8.3E+00					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-B03-A	1	7.30E+00	E		7.30E+00	1.2E+01	2.6E+00	8.3E+00					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-B01-B	1	5.79E+00	E		5.79E+00	1.1E+02	2.6E+00	8.3E+00					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-B02-B	1	3.07E+00	E		3.07E+00	1.5E+02	2.6E+00	8.3E+00					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-B03-B	1	1.30E+00	U1/2		1.30E+00	2.6E+02	2.6E+00	8.3E+00					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-B01-C	1	1.30E+00	U1/2		1.30E+00	1.4E+02	2.6E+00	8.3E+00					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1313-B02-C	1	3.29E+00	E		3.29E+00	8.1E+01	2.6E+00	8.3E+00					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	SWA-L06-1313-T01-A	1	1.81E+03			1.81E+03	6.6E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T02-A	1	1.57E+02			1.57E+02	7.1E+00	1.2E+00	3.8E+00	10	100	1.25E+03	109%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T03-A	1	1.30E+01			1.30E+01	2.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T04-A	1	1.68E+01			1.68E+01	9.5E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T05-A	1	1.45E+01			1.45E+01	3.8E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T06-A	1	6.00E-01	U1/2		6.00E-01	5.9E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T07-A	1	1.02E+01			1.02E+01	1.2E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T08-A	1	3.81E+03			3.81E+03	6.3E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T09-A	1	1.70E+04			1.70E+04	6.0E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T10-A	1	1.12E+03			1.12E+03	5.5E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T01-B	1	1.87E+03			1.87E+03	1.2E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T02-B	1	1.37E+02			1.37E+02	6.8E-01	1.2E+00	3.8E+00	10	100	1.30E+03	117%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T03-B	1	1.35E+01			1.35E+01	4.7E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T04-B	1	1.24E+01			1.24E+01	7.3E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T05-B	1	1.50E+01			1.50E+01	1.0E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T06-B	1	6.00E-01	U1/2		6.00E-01	6.1E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T07-B	1	1.32E+01			1.32E+01	8.2E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T08-B	1	4.04E+03			4.04E+03	5.3E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T09-B	1	1.82E+04			1.82E+04	8.5E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T10-B	1	1.12E+03			1.12E+03	6.9E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T01-C	1	1.87E+03			1.87E+03	7.2E-02	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T02-C	1	1.88E+02			1.88E+02	1.2E+00	1.2E+00	3.8E+00	10	100	1.35E+03	116%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T03-C	1	1.13E+01			1.13E+01	7.1E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T04-C	1	1.45E+01			1.45E+01	6.4E+00	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T05-C	1	1.70E+01			1.70E+01	1.2E+01	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T06-C	1	6.00E-01	U1/2		6.00E-01	4.4E+00	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T07-C	1	1.03E+01			1.03E+01	5.8E+01	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T08-C	1	4.04E+03			4.04E+03	5.7E-01	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T09-C	1	1.75E+04			1.75E+04	2.9E-01	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-T10-C	1	1.15E+03			1.15E+03	6.1E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-B01-A	1	1.18E+03			1.18E+03	8.0E-01	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	8.9E+01	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-B03-A	1	6.00E-01	U1/2		6.00E-01	1.4E+01	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-B01-B	1	6.00E-01	U1/2		6.00E-01	3.2E+01	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-B02-B	1	6.00E-01	U1/2		6.00E-01	8.2E+01	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-B03-B	1	6.00E-01	U1/2		6.00E-01	2.9E+01	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-B01-C	1	6.00E-01	U1/2		6.00E-01	3.0E+01	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1313-B02-C	1	6.00E-01	U1/2		6.00E-01	6.6E+01	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	SWA-L06-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	8.7E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	1.9E+01	1.8E+00	5.7E+00	10	100	1.09E+03	109%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T03-A	1	3.28E+00	E		3.28E+00	4.4E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T04-A	1	5.21E+00	E		5.21E+00	8.5E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T05-A	1	7.30E+00			7.30E+00	1.7E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T06-A	1	5.55E+01			5.55E+01	2.7E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T07-A	1	1.74E+02			1.74E+02	1.2E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T08-A	1	1.47E+02			1.47E+02	1.4E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T09-A	1	2.25E+02			2.25E+02	6.6E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T10-A	1	9.00E-01	U1/2		9.00E-01	1.9E+03	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	5.6E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	3.6E+01	1.8E+00	5.7E+00	10	100	1.17E+03	117%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T03-B	1	4.01E+00	E		4.01E+00	2.4E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T04-B	1	6.02E+00			6.02E+00	1.6E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T05-B	1	8.88E+00			8.88E+00	2.1E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T06-B	1	6.15E+01			6.15E+01	9.2E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T07-B	1	1.90E+02			1.90E+02	8.6E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T08-B	1	1.46E+02			1.46E+02	2.9E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T09-B	1	2.39E+02			2.39E+02	1.1E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T10-B	1	9.00E-01	U1/2		9.00E-01	1.0E+02	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	3.5E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	2.5E+01	1.8E+00	5.7E+00	10	100	1.18E+03	118%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T03-C	1	2.95E+00	E		2.95E+00	1.5E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T04-C	1	4.34E+00	E		4.34E+00	4.4E+00	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T05-C	1	8.95E+00			8.95E+00	1.1E+01	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T06-C	1	6.59E+01			6.59E+01	2.5E+00	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T07-C	1	1.24E+02			1.24E+02	5.8E+01	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T08-C	1	1.43E+02			1.43E+02	9.1E-01	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T09-C	1	2.20E+02			2.20E+02	1.8E-01	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-T10-C	1	9.00E-01	U1/2		9.00E-01	1.4E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	6.5E+01	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	6.6E+01	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	6.8E+01	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-B01-B	1	9.00E-01	U1/2		9.00E-01	4.9E+01	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-B02-B	1	9.00E-01	U1/2		9.00E-01	7.3E+01	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-B03-B	1	9.00E-01	U1/2		9.00E-01	7.6E+01	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-B01-C	1	9.00E-01	U1/2		9.00E-01	1.8E+01	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1313-B02-C	1	9.00E-01	U1/2		9.00E-01	4.1E+02	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	SWA-L06-1313-T01-A	1	1.04E+01	E		1.04E+01	6.2E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T02-A	1	1.85E+00	U1/2		1.85E+00	1.2E+01	3.7E+00	1.2E+01	10	100	1.08E+03	108%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T03-A	1	9.06E+00	E		9.06E+00	8.7E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T04-A	1	1.52E+01			1.52E+01	1.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T05-A	1	1.74E+01			1.74E+01	1.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T06-A	1	2.78E+01			2.78E+01	2.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T07-A	1	3.52E+01			3.52E+01	5.9E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T08-A	1	7.09E+01			7.09E+01	4.5E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T09-A	1	8.57E+02			8.57E+02	5.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T10-A	1	1.85E+00	U1/2		1.85E+00	6.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T01-B	1	1.14E+01	E		1.14E+01	3.1E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T02-B	1	1.85E+00	U1/2		1.85E+00	3.0E+01	3.7E+00	1.2E+01	10	100	1.18E+03	117%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T03-B	1	8.98E+00	E		8.98E+00	2.7E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T04-B	1	1.47E+01			1.47E+01	1.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T05-B	1	1.81E+01			1.81E+01	3.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T06-B	1	2.46E+01			2.46E+01	7.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T07-B	1	2.97E+01			2.97E+01	2.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T08-B	1	8.04E+01			8.04E+01	2.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T09-B	1	1.45E+03			1.45E+03	8.8E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T10-B	1	1.85E+00	U1/2		1.85E+00	2.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T01-C	1	1.21E+01			1.21E+01	1.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T02-C	1	1.85E+00	U1/2		1.85E+00	2.8E+01	3.7E+00	1.2E+01	10	100	1.18E+03	118%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T03-C	1	1.07E+01	E		1.07E+01	1.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T04-C	1	1.21E+01			1.21E+01	4.9E+00	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T05-C	1	1.59E+01			1.59E+01	8.2E+00	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T06-C	1	2.94E+01			2.94E+01	5.8E+00	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T07-C	1	2.69E+01			2.69E+01	3.1E+01	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T08-C	1	9.00E+01			9.00E+01	1.3E+00	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T09-C	1	1.25E+03			1.25E+03	8.0E-01	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-T10-C	1	1.85E+00	U1/2		1.85E+00	4.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	9.3E+00	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	2.6E+01	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-B03-A	1	1.85E+00	U1/2		1.85E+00	1.4E+01	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-B01-B	1	1.85E+00	U1/2		1.85E+00	2.5E+01	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-B02-B	1	1.85E+00	U1/2		1.85E+00	3.0E+01	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-B03-B	1	1.85E+00	U1/2		1.85E+00	1.3E+01	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-B01-C	1	1.85E+00	U1/2		1.85E+00	6.4E+01	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1313-B02-C	1	1.85E+00	U1/2		1.85E+00	2.9E+01	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	SWA-L06-1313-T01-A	1	1.77E+02			1.77E+02	4.8E-02	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T02-A	1	4.61E+01			4.61E+01	7.8E+00	2.0E+00	6.4E+00	1000	100	1.19E+03	114%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T03-A	1	1.28E+01			1.28E+01	2.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T04-A	1	2.02E+01			2.02E+01	4.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T05-A	1	1.74E+01			1.74E+01	3.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T06-A	1	1.01E+01			1.01E+01	4.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T07-A	1	6.57E+04			6.57E+04	4.6E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T08-A	1	9.30E+04			9.30E+04	1.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T09-A	1	1.49E+05			1.49E+05	5.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T10-A	1	9.38E+01			9.38E+01	4.6E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T01-B	1	2.26E+02			2.26E+02	7.9E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T02-B	1	4.94E+01			4.94E+01	8.0E-01	2.0E+00	6.4E+00	1000	100	1.09E+03	105%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T03-B	1	1.09E+01			1.09E+01	3.9E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T04-B	1	2.40E+01			2.40E+01	2.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T05-B	1	1.64E+01			1.64E+01	6.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T06-B	1	8.59E+00			8.59E+00	8.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T07-B	1	8.62E+04			8.62E+04	1.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T08-B	1	9.06E+04			9.06E+04	1.5E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T09-B	1	1.44E+05			1.44E+05	5.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T10-B	1	9.05E+01			9.05E+01	7.3E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T01-C	1	2.17E+02			2.17E+02	1.9E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T02-C	1	5.54E+01			5.54E+01	2.0E+00	2.0E+00	6.4E+00	1000	100	1.08E+03	103%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T03-C	1	1.22E+01			1.22E+01	2.5E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T04-C	1	2.43E+01			2.43E+01	2.9E+00	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T05-C	1	1.46E+01			1.46E+01	2.3E+00	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T06-C	1	1.20E+01			1.20E+01	2.5E+00	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T07-C	1	5.29E+04			5.29E+04	4.6E+01	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T08-C	1	8.90E+04			8.90E+04	5.2E-01	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T09-C	1	1.40E+05			1.40E+05	1.8E+00	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-T10-C	1	8.89E+01			8.89E+01	9.3E-02	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-B01-A	1	8.70E+01			8.70E+01	1.1E+00	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-B02-A	1	2.92E+00	E		2.92E+00	1.3E+01	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-B03-A	1	2.61E+00	E		2.61E+00	2.5E+00	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	2.8E+01	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	7.3E+00	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	4.8E+01	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	1.0E+00	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	SWA-L06-1313-T01-A	1	3.61E+02			3.61E+02	1.4E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T02-A	1	9.57E+00	E		9.57E+00	6.0E+01	6.8E+00	2.2E+01	10	100	1.06E+03	105%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T03-A	1	3.40E+00	U1/2		3.40E+00	2.4E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T04-A	1	3.40E+00	U1/2		3.40E+00	6.8E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T05-A	1	3.40E+00	U1/2		3.40E+00	5.2E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T06-A	1	3.40E+00	U1/2		3.40E+00	2.0E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T07-A	1	1.39E+01	E		1.39E+01	2.3E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T08-A	1	3.20E+02			3.20E+02	1.6E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T09-A	1	1.86E+03			1.86E+03	6.7E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T10-A	1	1.97E+01	E		1.97E+01	7.1E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T01-B	1	3.96E+02			3.96E+02	1.4E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T02-B	1	1.04E+01	E		1.04E+01	2.0E+01	6.8E+00	2.2E+01	10	100	1.13E+03	112%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T03-B	1	3.40E+00	U1/2		3.40E+00	1.4E+02	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T04-B	1	3.40E+00	U1/2		3.40E+00	1.1E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T05-B	1	3.40E+00	U1/2		3.40E+00	2.2E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T06-B	1	3.40E+00	U1/2		3.40E+00	9.5E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T07-B	1	1.32E+01	E		1.32E+01	5.7E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T08-B	1	3.71E+02			3.71E+02	7.3E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T09-B	1	2.87E+03			2.87E+03	4.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T10-B	1	1.88E+01	E		1.88E+01	2.8E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T01-C	1	3.74E+02			3.74E+02	1.7E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T02-C	1	1.06E+01	E		1.06E+01	8.5E+01	6.8E+00	2.2E+01	10	100	1.14E+03	113%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T03-C	1	3.40E+00	U1/2		3.40E+00	2.8E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T04-C	1	3.40E+00	U1/2		3.40E+00	6.0E+01	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T05-C	1	3.40E+00	U1/2		3.40E+00	5.7E+01	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T06-C	1	3.40E+00	U1/2		3.40E+00	7.0E+01	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T07-C	1	9.12E+00	E		9.12E+00	3.7E+01	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T08-C	1	3.56E+02			3.56E+02	7.7E-01	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T09-C	1	3.05E+03			3.05E+03	6.2E-01	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-T10-C	1	2.17E+01			2.17E+01	4.7E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-B01-A	1	2.06E+01	E		2.06E+01	1.3E+00	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	1.3E+02	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	1.0E+01	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-B01-B	1	3.40E+00	U1/2		3.40E+00	6.5E+01	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-B02-B	1	3.40E+00	U1/2		3.40E+00	9.5E+01	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-B03-B	1	3.40E+00	U1/2		3.40E+00	1.8E+02	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-B01-C	1	3.40E+00	U1/2		3.40E+00	1.7E+02	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1313-B02-C	1	3.40E+00	U1/2		3.40E+00	1.4E+02	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	SWA-L06-1313-T01-A	1	1.48E+01			1.48E+01	5.6E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T02-A	1	1.37E+01			1.37E+01	6.1E+00	1.9E+00	6.0E+00	10	100	9.23E+02	91%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T03-A	1	2.28E+02			2.28E+02	3.0E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T04-A	1	7.15E+02			7.15E+02	8.0E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T05-A	1	9.66E+02			9.66E+02	2.1E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T06-A	1	1.21E+03			1.21E+03	4.1E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T07-A	1	1.41E+03			1.41E+03	3.0E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T08-A	1	7.06E+02			7.06E+02	3.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T09-A	1	4.77E+02			4.77E+02	8.3E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T10-A	1	9.50E-01	U1/2		9.50E-01	1.5E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T01-B	1	1.30E+01			1.30E+01	5.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T02-B	1	1.54E+01			1.54E+01	2.0E+01	1.9E+00	6.0E+00	10	100	9.88E+02	97%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T03-B	1	1.88E+02			1.88E+02	7.0E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T04-B	1	7.45E+02			7.45E+02	3.6E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T05-B	1	9.81E+02			9.81E+02	1.9E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T06-B	1	9.97E+02			9.97E+02	1.2E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T07-B	1	1.31E+03			1.31E+03	6.2E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T08-B	1	7.07E+02			7.07E+02	5.0E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T09-B	1	7.27E+02			7.27E+02	3.0E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T10-B	1	9.50E-01	U1/2		9.50E-01	1.1E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T01-C	1	1.08E+01			1.08E+01	1.4E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T02-C	1	1.62E+01			1.62E+01	1.2E+01	1.9E+00	6.0E+00	10	100	1.01E+03	99%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T03-C	1	2.23E+02			2.23E+02	2.2E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T04-C	1	7.26E+02			7.26E+02	3.5E+00	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T05-C	1	9.28E+02			9.28E+02	4.9E+00	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T06-C	1	1.18E+03			1.18E+03	4.2E+00	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T07-C	1	9.10E+02			9.10E+02	8.2E+01	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T08-C	1	7.07E+02			7.07E+02	6.2E-01	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T09-C	1	7.22E+02			7.22E+02	3.5E+00	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-T10-C	1	9.50E-01	U1/2		9.50E-01	1.2E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	2.7E+01	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	1.1E+01	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	4.0E+01	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-B01-B	1	9.50E-01	U1/2		9.50E-01	2.9E+01	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-B02-B	1	9.50E-01	U1/2		9.50E-01	5.2E+01	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-B03-B	1	9.50E-01	U1/2		9.50E-01	3.2E+01	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-B01-C	1	9.50E-01	U1/2		9.50E-01	1.8E+01	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1313-B02-C	1	9.50E-01	U1/2		9.50E-01	6.7E+00	1.9E+00	6.0E+00					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	SWA-L06-1313-T01-A	1	4.84E+00	E		4.84E+00	5.9E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00	10	100	1.07E+03	107%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T04-A	1	1.99E+02			1.99E+02	3.9E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T05-A	1	2.09E+03			2.09E+03	3.8E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T06-A	1	1.20E+04			1.20E+04	1.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T07-A	1	2.21E+04			2.21E+04	5.4E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T08-A	1	1.32E+04			1.32E+04	2.5E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T09-A	1	9.59E+03			9.59E+03	6.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T10-A	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T01-B	1	4.27E+00	E		4.27E+00	6.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00	10	100	1.15E+03	114%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	8.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T04-B	1	1.76E+02			1.76E+02	5.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T05-B	1	2.29E+03			2.29E+03	3.4E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T06-B	1	9.39E+03			9.39E+03	8.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T07-B	1	2.25E+04			2.25E+04	1.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T08-B	1	1.31E+04			1.31E+04	6.6E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T09-B	1	1.35E+04			1.35E+04	1.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T10-B	1	1.00E+00	U1/2		1.00E+00	7.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T01-C	1	5.96E+00	E		5.96E+00	8.2E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00	10	100	1.17E+03	117%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T04-C	1	1.88E+02			1.88E+02	7.3E-01	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T05-C	1	2.74E+03			2.74E+03	5.5E+00	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T06-C	1	1.24E+04			1.24E+04	2.3E+00	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T07-C	1	1.52E+04			1.52E+04	6.3E+01	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T08-C	1	1.29E+04			1.29E+04	1.0E+00	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T09-C	1	1.38E+04			1.38E+04	4.1E-01	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-T10-C	1	1.00E+00	U1/2		1.00E+00	5.5E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	9.5E+00	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	6.7E+02	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	6.8E+01	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	6.8E+01	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	SWA-L06-1313-T01-A	1	1.86E+01			1.86E+01	2.6E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T02-A	1	1.72E+01			1.72E+01	3.5E+01	1.0E+00	3.2E+00	1000	100	1.16E+03	114%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T03-A	1	4.08E+03			4.08E+03	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T04-A	1	6.91E+05			6.91E+05	3.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T05-A	1	1.00E+06			1.00E+06	8.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T06-A	1	1.37E+06			1.37E+06	8.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T07-A	1	1.52E+06			1.52E+06	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T08-A	1	7.32E+05			7.32E+05	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T09-A	1	4.54E+05			4.54E+05	5.8E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T10-A	1	1.86E+01			1.86E+01	3.8E+02	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T01-B	1	2.17E+01			2.17E+01	2.6E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T02-B	1	2.80E+01			2.80E+01	4.5E+01	1.0E+00	3.2E+00	1000	100	1.14E+03	111%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T03-B	1	3.81E+03			3.81E+03	4.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T04-B	1	7.00E+05			7.00E+05	1.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T05-B	1	9.97E+05			9.97E+05	4.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T06-B	1	1.28E+06			1.28E+06	8.6E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T07-B	1	1.45E+06			1.45E+06	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T08-B	1	7.09E+05			7.09E+05	5.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T09-B	1	5.97E+05			5.97E+05	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T10-B	1	1.85E+01			1.85E+01	3.8E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T01-C	1	2.29E+01			2.29E+01	3.4E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T02-C	1	2.45E+01			2.45E+01	4.6E+01	1.0E+00	3.2E+00	1000	100	1.21E+03	119%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T03-C	1	4.02E+03			4.02E+03	1.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T04-C	1	6.66E+05			6.66E+05	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T05-C	1	9.54E+05			9.54E+05	4.8E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T06-C	1	1.29E+06			1.29E+06	1.7E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T07-C	1	1.08E+06			1.08E+06	5.1E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T08-C	1	7.01E+05			7.01E+05	4.8E-01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T09-C	1	6.11E+05			6.11E+05	2.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-T10-C	1	1.84E+01			1.84E+01	2.0E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-B01-A	1	1.39E+01			1.39E+01	4.1E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-B02-A	1	2.42E+00	E		2.42E+00	7.7E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-B03-A	1	1.86E+00	E		1.86E+00	2.1E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-B01-B	1	2.62E+00	E		2.62E+00	3.3E+02	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-B02-B	1	1.71E+00	E		1.71E+00	1.3E+02	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-B03-B	1	5.75E+00			5.75E+00	5.4E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-B01-C	1	9.50E+00			9.50E+00	5.6E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	2.3E+02	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	SWA-L06-1313-T01-A	1	1.21E+02			1.21E+02	8.4E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T02-A	1	1.31E+02			1.31E+02	7.5E+00	1.2E+00	3.8E+00	10	100	1.25E+03	112%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T03-A	1	1.38E+02			1.38E+02	3.0E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T04-A	1	1.33E+02			1.33E+02	3.5E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T05-A	1	1.26E+02			1.26E+02	3.7E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T06-A	1	5.69E+01			5.69E+01	2.6E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T07-A	1	1.41E+01			1.41E+01	2.7E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T08-A	1	4.65E+00			4.65E+00	2.0E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T09-A	1	3.80E+00	E		3.80E+00	6.8E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T10-A	1	1.33E+02			1.33E+02	2.9E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T01-B	1	1.25E+02			1.25E+02	1.4E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T02-B	1	1.44E+02			1.44E+02	1.5E+00	1.2E+00	3.8E+00	10	100	1.34E+03	119%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T03-B	1	1.25E+02			1.25E+02	4.2E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T04-B	1	1.31E+02			1.31E+02	3.1E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T05-B	1	1.29E+02			1.29E+02	2.8E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T06-B	1	3.84E+01			3.84E+01	8.6E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T07-B	1	1.03E+01			1.03E+01	4.6E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T08-B	1	7.04E+00			7.04E+00	2.0E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T09-B	1	5.36E+00			5.36E+00	1.7E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T10-B	1	1.38E+02			1.38E+02	6.4E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T01-C	1	1.14E+02			1.14E+02	2.8E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T02-C	1	1.46E+02			1.46E+02	1.5E+00	1.2E+00	3.8E+00	10	100	1.25E+03	111%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T03-C	1	1.37E+02			1.37E+02	9.3E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T04-C	1	1.40E+02			1.40E+02	1.0E+00	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T05-C	1	1.21E+02			1.21E+02	3.4E+00	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T06-C	1	4.86E+01			4.86E+01	3.5E+00	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T07-C	1	1.32E+01			1.32E+01	4.0E+01	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T08-C	1	6.88E+00			6.88E+00	1.8E+01	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T09-C	1	3.58E+00	E		3.58E+00	9.7E+00	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-T10-C	1	1.35E+02			1.35E+02	1.4E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-B01-A	1	1.34E+02			1.34E+02	9.6E-01	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-B02-A	1	2.64E+00	E		2.64E+00	5.7E+00	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-B03-A	1	3.39E+00	E		3.39E+00	1.5E+01	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-B01-B	1	2.66E+00	E		2.66E+00	4.2E+01	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-B02-B	1	2.47E+00	E		2.47E+00	2.7E+01	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-B03-B	1	2.02E+00	E		2.02E+00	3.0E+01	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-B01-C	1	1.74E+00	E		1.74E+00	2.8E+01	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1313-B02-C	1	1.77E+00	E		1.77E+00	4.6E+01	1.2E+00	3.8E+00					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	SWA-L06-1313-T01-A	1	4.38E+00	E		4.38E+00	4.8E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	4.9E+01	1.8E+00	5.7E+00	10	100	1.08E+03	108%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	1.8E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T04-A	1	1.20E+01			1.20E+01	3.9E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T05-A	1	2.42E+01			2.42E+01	5.8E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T06-A	1	1.62E+02			1.62E+02	5.3E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T07-A	1	4.09E+02			4.09E+02	1.2E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T08-A	1	2.96E+02			2.96E+02	1.0E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T09-A	1	2.48E+02			2.48E+02	3.9E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T10-A	1	9.00E-01	U1/2		9.00E-01	8.7E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T01-B	1	3.08E+00	E		3.08E+00	3.8E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	1.2E+02	1.8E+00	5.7E+00	10	100	1.15E+03	115%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	8.5E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T04-B	1	9.69E+00			9.69E+00	2.3E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T05-B	1	2.35E+01			2.35E+01	7.3E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T06-B	1	1.58E+02			1.58E+02	9.2E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T07-B	1	4.29E+02			4.29E+02	1.2E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T08-B	1	2.90E+02			2.90E+02	4.6E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T09-B	1	3.10E+02			3.10E+02	1.5E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T10-B	1	9.00E-01	U1/2		9.00E-01	4.6E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T01-C	1	2.85E+00	E		2.85E+00	4.8E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	6.4E+01	1.8E+00	5.7E+00	10	100	1.17E+03	117%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	2.9E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T04-C	1	1.09E+01			1.09E+01	1.8E+01	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T05-C	1	2.36E+01			2.36E+01	7.4E+00	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T06-C	1	1.78E+02			1.78E+02	1.8E+00	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T07-C	1	2.88E+02			2.88E+02	5.8E+01	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T08-C	1	2.90E+02			2.90E+02	2.1E-01	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T09-C	1	3.13E+02			3.13E+02	8.8E-01	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-T10-C	1	9.00E-01	U1/2		9.00E-01	4.6E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-B01-B	1	9.00E-01	U1/2		9.00E-01	7.0E+01	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-B02-B	1	9.00E-01	U1/2		9.00E-01	7.7E+01	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-B03-B	1	9.00E-01	U1/2		9.00E-01	3.6E+01	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-B01-C	1	9.00E-01	U1/2		9.00E-01	1.9E+02	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1313-B02-C	1	9.00E-01	U1/2		9.00E-01	4.8E+02	1.8E+00	5.7E+00					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	SWA-L06-1313-T01-A	1	1.09E+03			1.09E+03	1.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T02-A	1	2.87E+01			2.87E+01	5.2E+00	3.7E+00	1.2E+01	1000	100	1.20E+03	117%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T03-A	1	2.41E+01			2.41E+01	4.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T04-A	1	8.51E+01			8.51E+01	2.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T05-A	1	5.90E+01			5.90E+01	7.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T06-A	1	3.49E+01			3.49E+01	4.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T07-A	1	2.67E+01			2.67E+01	4.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T08-A	1	3.73E+02			3.73E+02	1.9E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T09-A	1	9.49E+03			9.49E+03	7.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T10-A	1	4.93E+01			4.93E+01	5.9E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T01-B	1	1.11E+03			1.11E+03	1.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T02-B	1	2.84E+01			2.84E+01	1.7E+01	3.7E+00	1.2E+01	1000	100	1.21E+03	118%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T03-B	1	2.62E+01			2.62E+01	6.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T04-B	1	8.61E+01			8.61E+01	1.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T05-B	1	7.42E+01			7.42E+01	1.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T06-B	1	4.39E+01			4.39E+01	7.9E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T07-B	1	4.03E+01			4.03E+01	1.9E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T08-B	1	3.41E+02			3.41E+02	2.0E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T09-B	1	3.65E+04			3.65E+04	7.4E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T10-B	1	5.44E+01			5.44E+01	2.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T01-C	1	1.06E+03			1.06E+03	1.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T02-C	1	3.91E+01			3.91E+01	2.3E+01	3.7E+00	1.2E+01	1000	100	1.22E+03	118%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T03-C	1	3.07E+01			3.07E+01	6.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T04-C	1	8.86E+01			8.86E+01	1.5E+01	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T05-C	1	9.34E+01			9.34E+01	1.3E+01	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T06-C	1	4.51E+01			4.51E+01	2.5E+01	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T07-C	1	2.89E+01			2.89E+01	2.9E+01	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T08-C	1	2.81E+02			2.81E+02	4.4E+00	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T09-C	1	2.36E+04			2.36E+04	3.8E-01	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-T10-C	1	5.74E+01			5.74E+01	5.6E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-B01-A	1	5.38E+01			5.38E+01	1.7E+01	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-B02-A	1	8.88E+00	E		8.88E+00	1.1E+02	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-B03-A	1	1.54E+01			1.54E+01	6.5E+00	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-B01-B	1	2.18E+01			2.18E+01	3.0E+01	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-B02-B	1	1.65E+01			1.65E+01	1.6E+01	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-B03-B	1	1.59E+01			1.59E+01	1.3E+01	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-B01-C	1	1.85E+00	U1/2		1.85E+00	1.1E+02	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1313-B02-C	1	1.66E+01			1.66E+01	4.5E+01	3.7E+00	1.2E+01					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	SWA-L06-1313-T01-A	1	5.30E+05			5.30E+05	2.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T02-A	1	3.17E+05			3.17E+05	7.0E+00	1.6E+00	5.1E+00	1000	100	3.18E+05	87%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T03-A	1	4.39E+05			4.39E+05	4.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T04-A	1	4.42E+05			4.42E+05	6.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T05-A	1	4.67E+05			4.67E+05	5.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T06-A	1	5.02E+05			5.02E+05	1.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T07-A	1	5.03E+05			5.03E+05	1.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T08-A	1	2.55E+05			2.55E+05	5.9E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T09-A	1	2.69E+05			2.69E+05	7.6E+01	1.6E+00	5.1E+00				---	VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T10-A	1	3.15E+05			3.15E+05	7.0E+01	1.6E+00	5.1E+00				---	VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T01-B	1	5.36E+05			5.36E+05	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T02-B	1	3.45E+05			3.45E+05	6.6E-01	1.6E+00	5.1E+00	1000	100	3.45E+05	90%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T03-B	1	4.09E+05			4.09E+05	4.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T04-B	1	4.52E+05			4.52E+05	9.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T05-B	1	4.65E+05			4.65E+05	3.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T06-B	1	4.92E+05			4.92E+05	1.2E+02	1.6E+00	5.1E+00				---	VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T07-B	1	4.66E+05			4.66E+05	5.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T08-B	1	2.31E+05			2.31E+05	1.0E+01	1.6E+00	5.1E+00				---	VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T09-B	1	3.28E+05			3.28E+05	5.6E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T10-B	1	3.18E+05			3.18E+05	3.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T01-C	1	5.27E+05			5.27E+05	1.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T02-C	1	3.47E+05			3.47E+05	1.9E+00	1.6E+00	5.1E+00	1000	100	3.48E+05	98%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T03-C	1	4.40E+05			4.40E+05	2.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T04-C	1	4.60E+05			4.60E+05	3.6E-01	1.6E+00	5.1E+00					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T05-C	1	4.60E+05			4.60E+05	6.0E+00	1.6E+00	5.1E+00					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T06-C	1	4.83E+05			4.83E+05	2.0E+00	1.6E+00	5.1E+00					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T07-C	1	4.26E+05			4.26E+05	7.2E+01	1.6E+00	5.1E+00					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T08-C	1	2.63E+05			2.63E+05	7.7E+00	1.6E+00	5.1E+00					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T09-C	1	2.97E+05			2.97E+05	2.0E+01	1.6E+00	5.1E+00					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-T10-C	1	3.12E+05			3.12E+05	5.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-B01-A	1	3.11E+05			3.11E+05	8.6E-01	1.6E+00	5.1E+00					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-B02-A	1	3.28E+01			3.28E+01	1.5E+00	1.6E+00	5.1E+00					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-B03-A	1	3.36E+01			3.36E+01	7.0E-01	1.6E+00	5.1E+00					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-B01-B	1	3.65E+01			3.65E+01	4.7E+00	1.6E+00	5.1E+00					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-B02-B	1	3.51E+01			3.51E+01	1.3E+01	1.6E+00	5.1E+00					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-B03-B	1	3.90E+01			3.90E+01	1.9E+01	1.6E+00	5.1E+00					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-B01-C	1	3.48E+01			3.48E+01	4.6E+00	1.6E+00	5.1E+00					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1313-B02-C	1	3.15E+01			3.15E+01	7.8E+00	1.6E+00	5.1E+00					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	SWA-L06-1313-T01-A	1	7.66E+04			7.66E+04	1.9E-01	1.5E+01	4.8E+01			---		VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T02-A	1	8.38E+04			8.38E+04	7.3E+00	1.5E+01	4.8E+01	10	100	8.49E+04	105%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T03-A	1	9.87E+04			9.87E+04	4.4E-01	1.5E+01	4.8E+01			---		VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T04-A	1	1.07E+05			1.07E+05	4.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T05-A	1	1.14E+05			1.14E+05	4.2E-01	1.5E+01	4.8E+01			---		VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T06-A	1	1.20E+05			1.20E+05	8.3E-01	1.5E+01	4.8E+01			---		VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T07-A	1	1.12E+05			1.12E+05	9.3E-01	1.5E+01	4.8E+01			---		VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T08-A	1	4.07E+04			4.07E+04	7.4E-01	1.5E+01	4.8E+01			---		VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T09-A	1	2.08E+04			2.08E+04	7.1E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T10-A	1	9.15E+04			9.15E+04	5.3E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T01-B	1	7.82E+04			7.82E+04	4.0E-01	1.5E+01	4.8E+01			---		VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T02-B	1	9.19E+04			9.19E+04	6.5E-01	1.5E+01	4.8E+01	10	100	9.28E+04	94%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T03-B	1	9.06E+04			9.06E+04	4.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T04-B	1	1.09E+05			1.09E+05	8.2E-01	1.5E+01	4.8E+01			---		VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T05-B	1	1.13E+05			1.13E+05	1.4E-01	1.5E+01	4.8E+01			---		VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T06-B	1	1.16E+05			1.16E+05	9.4E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T07-B	1	1.03E+05			1.03E+05	8.7E-01	1.5E+01	4.8E+01			---		VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T08-B	1	4.03E+04			4.03E+04	5.5E-01	1.5E+01	4.8E+01			---		VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T09-B	1	2.90E+04			2.90E+04	8.5E-01	1.5E+01	4.8E+01			---		VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T10-B	1	9.37E+04			9.37E+04	3.4E-01	1.5E+01	4.8E+01			---		VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T01-C	1	7.34E+04			7.34E+04	4.1E-01	1.5E+01	4.8E+01			---		VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T02-C	1	9.31E+04			9.31E+04	1.3E+00	1.5E+01	4.8E+01	10	100	9.40E+04	96%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T03-C	1	9.73E+04			9.73E+04	5.4E-01	1.5E+01	4.8E+01			---		VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T04-C	1	1.13E+05			1.13E+05	3.7E-01	1.5E+01	4.8E+01					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T05-C	1	1.07E+05			1.07E+05	5.1E+00	1.5E+01	4.8E+01					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T06-C	1	1.14E+05			1.14E+05	2.4E+00	1.5E+01	4.8E+01					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T07-C	1	7.34E+04			7.34E+04	6.4E+01	1.5E+01	4.8E+01					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T08-C	1	4.05E+04			4.05E+04	6.5E-01	1.5E+01	4.8E+01					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T09-C	1	2.93E+04			2.93E+04	1.0E+00	1.5E+01	4.8E+01					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-T10-C	1	9.27E+04			9.27E+04	4.3E-01	1.5E+01	4.8E+01			---		VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-B01-A	1	9.18E+04			9.18E+04	6.9E-01	1.5E+01	4.8E+01					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-B02-A	1	7.50E+00	U1/2		7.50E+00	9.0E+01	1.5E+01	4.8E+01					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-B03-A	1	7.50E+00	U1/2		7.50E+00	1.8E+02	1.5E+01	4.8E+01					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-B01-B	1	7.50E+00	U1/2		7.50E+00	2.5E+01	1.5E+01	4.8E+01					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-B02-B	1	7.50E+00	U1/2		7.50E+00	1.3E+02	1.5E+01	4.8E+01					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-B03-B	1	7.50E+00	U1/2		7.50E+00	6.3E+01	1.5E+01	4.8E+01					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-B01-C	1	7.50E+00	U1/2		7.50E+00	4.3E+01	1.5E+01	4.8E+01					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1313-B02-C	1	7.50E+00	U1/2		7.50E+00	1.4E+02	1.5E+01	4.8E+01					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	SWA-L06-1313-T01-A	1	4.65E+04			4.65E+04	6.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T02-A	1	1.41E+04			1.41E+04	6.9E+00	1.1E+00	3.5E+00	1000	100	1.51E+04	92%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T03-A	1	6.37E+03			6.37E+03	3.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T04-A	1	3.73E+03			3.73E+03	4.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T05-A	1	3.76E+03			3.76E+03	3.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T06-A	1	5.50E+03			5.50E+03	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T07-A	1	5.80E+03			5.80E+03	8.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T08-A	1	1.91E+04			1.91E+04	7.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T09-A	1	2.77E+05			2.77E+05	6.1E+01	1.1E+00	3.5E+00				---	VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T10-A	1	2.77E+04			2.77E+04	5.8E+01	1.1E+00	3.5E+00				---	VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T01-B	1	4.78E+04			4.78E+04	1.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T02-B	1	1.58E+04			1.58E+04	3.4E-01	1.1E+00	3.5E+00	1000	100	1.67E+04	96%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T03-B	1	5.94E+03			5.94E+03	4.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T04-B	1	4.11E+03			4.11E+03	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T05-B	1	3.25E+03			3.25E+03	3.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T06-B	1	6.55E+03			6.55E+03	9.1E+01	1.1E+00	3.5E+00				---	VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T07-B	1	5.56E+03			5.56E+03	1.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T08-B	1	1.68E+04			1.68E+04	7.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T09-B	1	7.65E+05			7.65E+05	1.8E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T10-B	1	2.64E+04			2.64E+04	1.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T01-C	1	4.74E+04			4.74E+04	7.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T02-C	1	1.62E+04			1.62E+04	1.3E+00	1.1E+00	3.5E+00	1000	100	1.71E+04	94%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T03-C	1	6.37E+03			6.37E+03	4.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T04-C	1	4.67E+03			4.67E+03	4.4E-01	1.1E+00	3.5E+00					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T05-C	1	2.98E+03			2.98E+03	5.8E+00	1.1E+00	3.5E+00					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T06-C	1	7.30E+03			7.30E+03	2.1E+00	1.1E+00	3.5E+00					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T07-C	1	4.67E+03			4.67E+03	6.7E+01	1.1E+00	3.5E+00					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T08-C	1	1.58E+04			1.58E+04	8.9E-01	1.1E+00	3.5E+00					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T09-C	1	6.95E+05			6.95E+05	2.0E+00	1.1E+00	3.5E+00					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-T10-C	1	2.68E+04			2.68E+04	8.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-B01-A	1	2.60E+04			2.60E+04	4.3E-01	1.1E+00	3.5E+00					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-B02-A	1	1.12E+01			1.12E+01	1.8E+01	1.1E+00	3.5E+00					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-B03-A	1	1.25E+01			1.25E+01	4.3E+00	1.1E+00	3.5E+00					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-B01-B	1	4.54E+00			4.54E+00	6.9E+01	1.1E+00	3.5E+00					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-B02-B	1	1.74E+01			1.74E+01	2.6E+00	1.1E+00	3.5E+00					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-B03-B	1	1.84E+01			1.84E+01	9.5E+00	1.1E+00	3.5E+00					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-B01-C	1	9.78E+00			9.78E+00	1.7E+01	1.1E+00	3.5E+00					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1313-B02-C	1	1.58E+01			1.58E+01	2.0E+01	1.1E+00	3.5E+00					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	SWA-L06-1313-T01-A	1	7.06E+05			7.06E+05	7.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T02-A	1	4.77E+05			4.77E+05	1.3E+00	2.5E+00	8.0E+00	1000	100	4.78E+05	98%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T03-A	1	5.04E+05			5.04E+05	3.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T04-A	1	4.88E+05			4.88E+05	6.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T05-A	1	4.87E+05			4.87E+05	4.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T06-A	1	4.87E+05			4.87E+05	3.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T07-A	1	4.83E+05			4.83E+05	3.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T08-A	1	4.83E+05			4.83E+05	8.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T09-A	1	4.39E+05			4.39E+05	6.9E+01	2.5E+00	8.0E+00				---	VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T10-A	1	4.57E+05			4.57E+05	5.1E+01	2.5E+00	8.0E+00				---	VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T01-B	1	7.15E+05			7.15E+05	2.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T02-B	1	4.79E+05			4.79E+05	3.2E-01	2.5E+00	8.0E+00	1000	100	4.80E+05	91%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T03-B	1	4.93E+05			4.93E+05	5.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T04-B	1	4.90E+05			4.90E+05	4.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T05-B	1	4.83E+05			4.83E+05	6.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T06-B	1	4.63E+05			4.63E+05	8.7E+01	2.5E+00	8.0E+00				---	VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T07-B	1	4.76E+05			4.76E+05	2.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T08-B	1	4.80E+05			4.80E+05	1.0E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T09-B	1	4.58E+05			4.58E+05	7.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T10-B	1	4.62E+05			4.62E+05	3.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T01-C	1	7.04E+05			7.04E+05	5.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T02-C	1	4.80E+05			4.80E+05	1.4E-01	2.5E+00	8.0E+00	1000	100	4.81E+05	94%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T03-C	1	5.01E+05			5.01E+05	1.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T04-C	1	4.89E+05			4.89E+05	1.7E-01	2.5E+00	8.0E+00					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T05-C	1	4.77E+05			4.77E+05	1.7E-01	2.5E+00	8.0E+00					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T06-C	1	4.76E+05			4.76E+05	6.2E-01	2.5E+00	8.0E+00					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T07-C	1	4.72E+05			4.72E+05	5.1E+01	2.5E+00	8.0E+00					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T08-C	1	4.80E+05			4.80E+05	2.5E-01	2.5E+00	8.0E+00					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T09-C	1	4.54E+05			4.54E+05	7.0E-01	2.5E+00	8.0E+00					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-T10-C	1	4.62E+05			4.62E+05	9.3E-02	2.5E+00	8.0E+00				---	VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-B01-A	1	4.68E+05			4.68E+05	6.1E-01	2.5E+00	8.0E+00					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-B02-A	1	2.21E+01			2.21E+01	1.3E+01	2.5E+00	8.0E+00					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-B03-A	1	7.25E+05			7.25E+05	6.3E-01	2.5E+00	8.0E+00					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-B01-B	1	1.51E+02			1.51E+02	4.9E+00	2.5E+00	8.0E+00					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-B02-B	1	9.67E+01			9.67E+01	9.1E+00	2.5E+00	8.0E+00					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-B03-B	1	7.90E+01			7.90E+01	3.2E+01	2.5E+00	8.0E+00					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-B01-C	1	6.63E+01			6.63E+01	2.1E+00	2.5E+00	8.0E+00					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1313-B02-C	1	2.59E+01			2.59E+01	1.8E+00	2.5E+00	8.0E+00					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	SWA-L06-1313-T01-A	1	5.52E+02			5.52E+02	4.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T02-A	1	9.50E+02			9.50E+02	6.4E+00	1.0E+00	3.2E+00	1000	100	2.05E+03	110%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T03-A	1	1.80E+04			1.80E+04	6.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T04-A	1	2.95E+04			2.95E+04	4.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T05-A	1	3.57E+04			3.57E+04	5.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T06-A	1	4.74E+04			4.74E+04	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T07-A	1	5.02E+04			5.02E+04	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T08-A	1	2.28E+04			2.28E+04	9.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T09-A	1	1.73E+04			1.73E+04	1.2E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T10-A	1	3.05E+02			3.05E+02	6.4E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T01-B	1	5.49E+02			5.49E+02	3.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T02-B	1	1.05E+03			1.05E+03	1.3E+00	1.0E+00	3.2E+00	1000	100	2.14E+03	109%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T03-B	1	1.65E+04			1.65E+04	4.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T04-B	1	3.02E+04			3.02E+04	5.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T05-B	1	3.61E+04			3.61E+04	9.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T06-B	1	4.60E+04			4.60E+04	9.4E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T07-B	1	4.71E+04			4.71E+04	8.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T08-B	1	2.26E+04			2.26E+04	7.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T09-B	1	1.90E+04			1.90E+04	2.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T10-B	1	3.17E+02			3.17E+02	9.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T01-C	1	5.26E+02			5.26E+02	8.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T02-C	1	1.04E+03			1.04E+03	1.1E+00	1.0E+00	3.2E+00	1000	100	2.13E+03	108%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T03-C	1	1.78E+04			1.78E+04	9.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T04-C	1	3.11E+04			3.11E+04	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T05-C	1	3.46E+04			3.46E+04	5.2E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T06-C	1	4.49E+04			4.49E+04	3.4E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T07-C	1	3.54E+04			3.54E+04	4.8E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T08-C	1	2.25E+04			2.25E+04	8.3E-01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T09-C	1	1.88E+04			1.88E+04	7.3E-01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-T10-C	1	3.01E+02			3.01E+02	1.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-B01-A	1	2.94E+02			2.94E+02	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	4.0E+02	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	1.6E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	1.2E+02	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	3.8E+02	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	1.5E+02	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	5.7E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	5.5E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	SWA-L06-1313-T01-A	1	3.22E+05			3.22E+05	4.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T02-A	1	8.30E+05			8.30E+05	1.1E+01	6.8E+00	2.2E+01	1000	100	8.30E+05	82%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T03-A	1	9.63E+05			9.63E+05	6.9E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T04-A	1	7.57E+05			7.57E+05	5.0E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T05-A	1	5.09E+05			5.09E+05	2.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T06-A	1	5.03E+05			5.03E+05	6.8E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T07-A	1	4.78E+05			4.78E+05	9.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T08-A	1	1.88E+05			1.88E+05	7.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T09-A	1	1.04E+05			1.04E+05	7.0E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T10-A	1	7.72E+05			7.72E+05	3.2E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T01-B	1	3.25E+05			3.25E+05	1.8E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T02-B	1	9.88E+05			9.88E+05	6.7E-01	6.8E+00	2.2E+01	1000	100	9.89E+05	91%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T03-B	1	7.74E+05			7.74E+05	5.3E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T04-B	1	7.95E+05			7.95E+05	1.2E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T05-B	1	5.16E+05			5.16E+05	4.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T06-B	1	5.19E+05			5.19E+05	1.0E+02	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T07-B	1	4.44E+05			4.44E+05	9.3E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T08-B	1	1.87E+05			1.87E+05	4.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T09-B	1	1.39E+05			1.39E+05	8.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T10-B	1	8.43E+05			8.43E+05	1.1E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T01-C	1	3.06E+05			3.06E+05	2.9E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T02-C	1	9.07E+05			9.07E+05	9.2E-01	6.8E+00	2.2E+01	1000	100	9.08E+05	86%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T03-C	1	9.25E+05			9.25E+05	1.4E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T04-C	1	8.83E+05			8.83E+05	3.1E-01	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T05-C	1	5.02E+05			5.02E+05	7.5E+00	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T06-C	1	4.96E+05			4.96E+05	2.7E+00	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T07-C	1	4.23E+05			4.23E+05	5.6E+01	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T08-C	1	1.87E+05			1.87E+05	7.8E-01	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T09-C	1	1.36E+05			1.36E+05	1.2E+00	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-T10-C	1	7.63E+05			7.63E+05	8.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-B01-A	1	1.00E+06			1.00E+06	7.8E-01	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-B02-A	1	3.58E+03			3.58E+03	4.8E+00	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-B03-A	1	1.90E+02			1.90E+02	1.9E+01	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-B01-B	1	1.03E+02			1.03E+02	7.5E+00	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-B02-B	1	3.40E+00	U1/2		3.40E+00	4.1E+02	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-B03-B	1	5.11E+01			5.11E+01	1.2E+02	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-B01-C	1	6.26E+01			6.26E+01	4.8E+01	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1313-B02-C	1	1.41E+02			1.41E+02	3.2E+01	6.8E+00	2.2E+01					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	SWA-L06-1313-T01-A	1	2.30E+00	U1/2		2.30E+00	2.1E+01	4.6E+00	1.5E+01			---		VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T02-A	1	2.30E+00	U1/2		2.30E+00	3.0E+02	4.6E+00	1.5E+01	10	100	9.82E+02	98%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T03-A	1	2.30E+00	U1/2		2.30E+00	5.8E+01	4.6E+00	1.5E+01			---		VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T04-A	1	2.30E+00	U1/2		2.30E+00	3.7E+02	4.6E+00	1.5E+01			---		VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T05-A	1	2.30E+00	U1/2		2.30E+00	3.8E+01	4.6E+00	1.5E+01			---		VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T06-A	1	6.12E+00	E		6.12E+00	5.8E+01	4.6E+00	1.5E+01			---		VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T07-A	1	2.62E+01			2.62E+01	8.7E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T08-A	1	1.66E+01			1.66E+01	2.9E+01	4.6E+00	1.5E+01			---		VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T09-A	1	1.16E+01	E		1.16E+01	7.9E+01	4.6E+00	1.5E+01			---		VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T10-A	1	2.30E+00	U1/2		2.30E+00	3.1E+02	4.6E+00	1.5E+01			---		VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T01-B	1	2.30E+00	U1/2		2.30E+00	1.1E+02	4.6E+00	1.5E+01			---		VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T02-B	1	2.30E+00	U1/2		2.30E+00	5.8E+01	4.6E+00	1.5E+01	10	100	1.05E+03	105%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T03-B	1	2.30E+00	U1/2		2.30E+00	1.0E+02	4.6E+00	1.5E+01			---		VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T04-B	1	2.30E+00	U1/2		2.30E+00	6.1E+01	4.6E+00	1.5E+01			---		VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T05-B	1	2.30E+00	U1/2		2.30E+00	6.8E+01	4.6E+00	1.5E+01			---		VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T06-B	1	5.63E+00	E		5.63E+00	1.1E+02	4.6E+00	1.5E+01			---		VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T07-B	1	2.32E+01			2.32E+01	2.7E+01	4.6E+00	1.5E+01			---		VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T08-B	1	1.34E+01	E		1.34E+01	3.3E+01	4.6E+00	1.5E+01			---		VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T09-B	1	9.39E+00	E		9.39E+00	8.4E+01	4.6E+00	1.5E+01			---		VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T10-B	1	2.30E+00	U1/2		2.30E+00	6.9E+01	4.6E+00	1.5E+01			---		VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T01-C	1	2.30E+00	U1/2		2.30E+00	2.8E+01	4.6E+00	1.5E+01			---		VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T02-C	1	2.30E+00	U1/2		2.30E+00	4.7E+01	4.6E+00	1.5E+01	10	100	1.06E+03	106%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T03-C	1	2.30E+00	U1/2		2.30E+00	7.3E+01	4.6E+00	1.5E+01			---		VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T04-C	1	2.30E+00	U1/2		2.30E+00	6.4E+01	4.6E+00	1.5E+01					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T05-C	1	2.30E+00	U1/2		2.30E+00	5.4E+01	4.6E+00	1.5E+01					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T06-C	1	8.63E+00	E		8.63E+00	8.6E+01	4.6E+00	1.5E+01					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T07-C	1	2.13E+01			2.13E+01	7.7E+01	4.6E+00	1.5E+01					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T08-C	1	1.10E+01	E		1.10E+01	1.5E+01	4.6E+00	1.5E+01					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T09-C	1	1.01E+01	E		1.01E+01	1.1E+02	4.6E+00	1.5E+01					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-T10-C	1	2.30E+00	U1/2		2.30E+00	4.5E+01	4.6E+00	1.5E+01			---		VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	1.7E+02	4.6E+00	1.5E+01					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	7.3E+01	4.6E+00	1.5E+01					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	9.2E+01	4.6E+00	1.5E+01					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-B01-B	1	2.30E+00	U1/2		2.30E+00	3.9E+01	4.6E+00	1.5E+01					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-B02-B	1	2.30E+00	U1/2		2.30E+00	1.1E+02	4.6E+00	1.5E+01					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-B03-B	1	2.30E+00	U1/2		2.30E+00	1.7E+02	4.6E+00	1.5E+01					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-B01-C	1	2.30E+00	U1/2		2.30E+00	5.4E+01	4.6E+00	1.5E+01					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1313-B02-C	1	2.30E+00	U1/2		2.30E+00	1.5E+02	4.6E+00	1.5E+01					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	SWA-L06-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	5.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	3.6E+01	2.0E+00	6.4E+00	10	100	1.09E+03	109%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	2.2E+02	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	3.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	6.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	8.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	1.5E+02	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T08-A	1	2.01E+01			2.01E+01	4.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T09-A	1	3.85E+02			3.85E+02	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T10-A	1	1.00E+00	U1/2		1.00E+00	6.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	3.9E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	3.1E+01	2.0E+00	6.4E+00	10	100	1.11E+03	111%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	9.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	5.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	1.5E+03	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	7.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T08-B	1	1.77E+01			1.77E+01	5.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T09-B	1	4.18E+03			4.18E+03	1.9E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T10-B	1	1.00E+00	U1/2		1.00E+00	2.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	2.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	4.4E+00	2.0E+00	6.4E+00	10	100	1.19E+03	119%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	1.0E+02	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	1.8E+02	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	8.9E+01	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	1.2E+00	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	4.9E+01	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T08-C	1	1.37E+01			1.37E+01	1.9E+00	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T09-C	1	3.00E+02			3.00E+02	8.7E-01	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-T10-C	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	4.1E+01	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	4.0E+00	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	2.8E+01	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	2.9E+01	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	5.8E+00	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	3.9E+01	2.0E+00	6.4E+00					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	SWA-L06-1313-T01-A	1	5.29E+02			5.29E+02	7.3E-01	1.5E+00	4.8E+00			---		VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T02-A	1	1.47E+02			1.47E+02	6.8E+00	1.5E+00	4.8E+00	10	100	1.26E+03	111%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T03-A	1	1.16E+02			1.16E+02	1.9E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T04-A	1	1.77E+02			1.77E+02	3.9E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T05-A	1	1.75E+02			1.75E+02	1.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T06-A	1	1.71E+02			1.71E+02	4.8E-01	1.5E+00	4.8E+00			---		VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T07-A	1	1.50E+02			1.50E+02	2.6E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T08-A	1	5.87E+01			5.87E+01	3.7E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T09-A	1	1.39E+03			1.39E+03	7.2E+01	1.5E+00	4.8E+00			---		VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T10-A	1	3.78E+02			3.78E+02	5.5E+01	1.5E+00	4.8E+00			---		VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T01-B	1	5.41E+02			5.41E+02	5.8E-01	1.5E+00	4.8E+00			---		VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T02-B	1	1.59E+02			1.59E+02	3.4E-01	1.5E+00	4.8E+00	10	100	1.34E+03	118%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T03-B	1	1.12E+02			1.12E+02	3.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T04-B	1	1.90E+02			1.90E+02	1.0E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T05-B	1	1.64E+02			1.64E+02	5.2E-01	1.5E+00	4.8E+00			---		VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T06-B	1	1.88E+02			1.88E+02	8.7E+01	1.5E+00	4.8E+00			---		VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T07-B	1	1.41E+02			1.41E+02	3.8E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T08-B	1	5.85E+01			5.85E+01	3.8E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T09-B	1	1.40E+03			1.40E+03	1.4E-01	1.5E+00	4.8E+00			---		VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T10-B	1	3.71E+02			3.71E+02	3.9E-01	1.5E+00	4.8E+00			---		VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T01-C	1	5.18E+02			5.18E+02	1.0E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T02-C	1	1.64E+02			1.64E+02	1.2E+00	1.5E+00	4.8E+00	10	100	1.26E+03	110%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T03-C	1	1.17E+02			1.17E+02	1.6E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T04-C	1	1.92E+02			1.92E+02	6.2E-01	1.5E+00	4.8E+00					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T05-C	1	1.57E+02			1.57E+02	4.6E+00	1.5E+00	4.8E+00					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T06-C	1	1.66E+02			1.66E+02	3.2E+00	1.5E+00	4.8E+00					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T07-C	1	9.68E+01			9.68E+01	6.1E+01	1.5E+00	4.8E+00					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T08-C	1	5.85E+01			5.85E+01	3.1E+00	1.5E+00	4.8E+00					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T09-C	1	1.25E+03			1.25E+03	1.7E+00	1.5E+00	4.8E+00					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-T10-C	1	3.73E+02			3.73E+02	6.1E-01	1.5E+00	4.8E+00			---		VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-B01-A	1	3.65E+02			3.65E+02	5.9E-01	1.5E+00	4.8E+00					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-B02-A	1	7.50E-01	U1/2		7.50E-01	1.4E+01	1.5E+00	4.8E+00					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-B03-A	1	7.50E-01	U1/2		7.50E-01	2.3E+01	1.5E+00	4.8E+00					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-B01-B	1	7.50E-01	U1/2		7.50E-01	2.7E+01	1.5E+00	4.8E+00					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-B02-B	1	7.50E-01	U1/2		7.50E-01	4.3E+01	1.5E+00	4.8E+00					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-B03-B	1	7.50E-01	U1/2		7.50E-01	2.9E+01	1.5E+00	4.8E+00					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-B01-C	1	7.50E-01	U1/2		7.50E-01	2.4E+01	1.5E+00	4.8E+00					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1313-B02-C	1	7.50E-01	U1/2		7.50E-01	4.2E+01	1.5E+00	4.8E+00					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	SWA-L06-1313-T01-A	1	3.60E+01			3.60E+01	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 2:59 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T02-A	1	2.89E+00	E		2.89E+00	1.5E+01	1.0E+00	3.2E+00	10	100	1.16E+03	116%	VU ICP-OES	4/1/11 3:00 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T03-A	1	3.22E+00			3.22E+00	1.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:02 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T04-A	1	3.66E+00			3.66E+00	2.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:04 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T05-A	1	3.11E+00	E		3.11E+00	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:05 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T06-A	1	2.76E+01			2.76E+01	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:07 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T07-A	1	5.54E+02			5.54E+02	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:09 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T08-A	1	1.17E+03			1.17E+03	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:10 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T09-A	1	1.35E+03			1.35E+03	4.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:12 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T10-A	1	2.07E+00	E		2.07E+00	3.6E+03	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:51 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T01-B	1	3.09E+01			3.09E+01	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:18 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T02-B	1	2.86E+00	E		2.86E+00	5.6E+00	1.0E+00	3.2E+00	10	100	1.15E+03	114%	VU ICP-OES	4/1/11 3:20 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T03-B	1	2.58E+00	E		2.58E+00	4.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:22 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T04-B	1	2.80E+00	E		2.80E+00	1.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:23 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T05-B	1	3.76E+00			3.76E+00	3.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:25 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T06-B	1	2.60E+01			2.60E+01	9.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:27 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T07-B	1	6.94E+02			6.94E+02	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:28 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T08-B	1	1.18E+03			1.18E+03	8.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:30 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T09-B	1	1.73E+03			1.73E+03	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:32 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T10-B	1	2.94E+00	E		2.94E+00	1.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:53 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T01-C	1	2.80E+01			2.80E+01	4.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:33 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T02-C	1	2.67E+00	E		2.67E+00	8.4E+00	1.0E+00	3.2E+00	10	100	1.16E+03	116%	VU ICP-OES	4/1/11 3:35 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T03-C	1	2.20E+00	E		2.20E+00	6.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:37 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T04-C	1	2.70E+00	E		2.70E+00	1.9E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:38 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T05-C	1	3.15E+00	E		3.15E+00	1.4E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:40 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T06-C	1	3.09E+01			3.09E+01	3.6E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:41 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T07-C	1	5.31E+02			5.31E+02	3.0E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:43 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T08-C	1	1.15E+03			1.15E+03	5.7E-01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:45 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T09-C	1	1.72E+03			1.72E+03	3.1E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 3:46 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-T10-C	1	2.28E+00	E		2.28E+00	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/1/11 3:55 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-B01-A	1	3.52E+00			3.52E+00	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:46 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-B02-A	1	1.36E+00	E		1.36E+00	2.1E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:47 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-B03-A	1	1.25E+00	E		1.25E+00	4.6E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:49 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-B01-B	1	1.62E+00	E		1.62E+00	2.3E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:50 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-B02-B	1	3.92E+00			3.92E+00	8.3E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:52 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-B03-B	1	2.43E+00	E		2.43E+00	2.0E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:54 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-B01-C	1	2.01E+00	E		2.01E+00	7.4E+00	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:55 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1313-B02-C	1	2.14E+00	E		2.14E+00	1.9E+01	1.0E+00	3.2E+00					VU ICP-OES	4/1/11 2:57 PM	EPA Interlab L06 1313-1316 SWA

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	SWA-L07-1313-T01-A	1	3.56E+04			3.56E+04	7.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T02-A	1	2.92E+03			2.92E+03	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T03-A	1	1.56E+02			1.56E+02	1.1E+01	1.0E+00	3.2E+00	1000	100	1.20E+03	104%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T04-A	1	5.91E+01			5.91E+01	1.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T05-A	1	1.91E+01			1.91E+01	5.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T06-A	1	5.91E+01			5.91E+01	3.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T07-A	1	3.20E+02			3.20E+02	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T08-A	1	2.00E+05			2.00E+05	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T09-A	1	3.12E+06			3.12E+06	2.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T01-B	1	3.63E+04			3.63E+04	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T02-B	1	2.89E+03			2.89E+03	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T03-B	1	2.82E+02			2.82E+02	1.3E+00	1.0E+00	3.2E+00	1000	100	1.40E+03	112%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T04-B	1	4.08E+01			4.08E+01	4.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T05-B	1	1.78E+01			1.78E+01	3.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T06-B	1	8.45E+01			8.45E+01	4.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T07-B	1	2.82E+02			2.82E+02	6.5E-02	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T08-B	1	2.43E+05			2.43E+05	7.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T09-B	1	6.07E+05			6.07E+05	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T01-C	1	3.85E+04			3.85E+04	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T02-C	1	3.45E+03			3.45E+03	2.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T03-C	1	2.55E+02			2.55E+02	7.2E+01	1.0E+00	3.2E+00	1000	100	1.11E+03	86%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T04-C	1	3.12E+01			3.12E+01	3.4E+01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T05-C	1	2.80E+01			2.80E+01	2.5E+01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T06-C	1	8.92E+01			8.92E+01	2.5E+00	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T07-C	1	2.78E+02			2.78E+02	7.2E-01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T08-C	1	1.75E+05			1.75E+05	1.0E+00	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-T09-C	1	6.36E+05			6.36E+05	8.4E-01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-B01-A	1	1.07E+01			1.07E+01	6.6E+00	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1313-B02-A	1	2.31E+01			2.31E+01	9.6E+00	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	SWA-L07-1313-T01-A	1	3.04E+03			3.04E+03	1.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T02-A	1	4.91E+02			4.91E+02	3.7E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T03-A	1	1.46E+03			1.46E+03	2.1E+00	7.5E+00	2.4E+01	10	100	2.36E+03	91%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T04-A	1	1.56E+03			1.56E+03	9.1E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T05-A	1	1.51E+03			1.51E+03	1.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T06-A	1	1.47E+03			1.47E+03	1.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T07-A	1	1.25E+03			1.25E+03	1.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T08-A	1	7.84E+02			7.84E+02	1.4E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T09-A	1	2.61E+04			2.61E+04	6.9E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T01-B	1	3.66E+03			3.66E+03	6.5E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T02-B	1	5.22E+02			5.22E+02	1.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T03-B	1	1.42E+03			1.42E+03	3.3E-01	7.5E+00	2.4E+01	10	100	2.45E+03	103%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T04-B	1	1.56E+03			1.56E+03	3.4E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T05-B	1	1.48E+03			1.48E+03	1.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T06-B	1	1.35E+03			1.35E+03	1.4E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T07-B	1	1.07E+03			1.07E+03	9.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T08-B	1	7.38E+02			7.38E+02	2.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T09-B	1	1.48E+04			1.48E+04	7.3E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T01-C	1	3.76E+03			3.76E+03	6.6E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T02-C	1	6.90E+02			6.90E+02	1.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T03-C	1	1.52E+03			1.52E+03	2.3E+00	7.5E+00	2.4E+01	10	100	2.50E+03	98%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T04-C	1	1.60E+03			1.60E+03	6.7E-01	7.5E+00	2.4E+01					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T05-C	1	1.69E+03			1.69E+03	1.1E+00	7.5E+00	2.4E+01					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T06-C	1	1.38E+03			1.38E+03	2.3E+00	7.5E+00	2.4E+01					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T07-C	1	1.33E+03			1.33E+03	5.0E+00	7.5E+00	2.4E+01					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T08-C	1	1.06E+03			1.06E+03	6.8E-01	7.5E+00	2.4E+01					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-T09-C	1	4.66E+03			4.66E+03	6.9E-01	7.5E+00	2.4E+01					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-B01-A	1	7.74E+00	E		7.74E+00	8.7E+01	7.5E+00	2.4E+01					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1313-B02-A	1	3.75E+00	U1/2		3.75E+00	8.5E+01	7.5E+00	2.4E+01					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	SWA-L07-1313-T01-A	1	4.55E+03			4.55E+03	1.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T02-A	1	2.30E+02			2.30E+02	2.7E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T03-A	1	1.39E+02			1.39E+02	7.7E+00	1.1E+01	3.5E+01	10	100	1.23E+03	109%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T04-A	1	4.20E+02			4.20E+02	2.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T05-A	1	1.97E+02			1.97E+02	8.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T06-A	1	2.33E+02			2.33E+02	8.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T07-A	1	2.75E+02			2.75E+02	2.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T08-A	1	2.62E+03			2.62E+03	1.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T09-A	1	6.64E+04			6.64E+04	1.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T01-B	1	4.39E+03			4.39E+03	3.9E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T02-B	1	2.12E+02			2.12E+02	2.7E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T03-B	1	1.43E+02			1.43E+02	5.6E+00	1.1E+01	3.5E+01	10	100	1.33E+03	119%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T04-B	1	3.78E+02			3.78E+02	1.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T05-B	1	2.31E+02			2.31E+02	3.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T06-B	1	1.92E+02			1.92E+02	7.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T07-B	1	3.75E+02			3.75E+02	2.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T08-B	1	2.85E+03			2.85E+03	4.2E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T09-B	1	1.39E+04			1.39E+04	1.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T01-C	1	4.62E+03			4.62E+03	8.9E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T02-C	1	2.45E+02			2.45E+02	2.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T03-C	1	2.01E+02			2.01E+02	4.7E+00	1.1E+01	3.5E+01	10	100	1.34E+03	114%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T04-C	1	4.17E+02			4.17E+02	2.3E+00	1.1E+01	3.5E+01					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T05-C	1	3.69E+02			3.69E+02	2.9E+00	1.1E+01	3.5E+01					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T06-C	1	1.45E+02			1.45E+02	3.9E+00	1.1E+01	3.5E+01					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T07-C	1	2.91E+02			2.91E+02	2.3E+00	1.1E+01	3.5E+01					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T08-C	1	2.50E+03			2.50E+03	3.8E-01	1.1E+01	3.5E+01					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-T09-C	1	9.32E+03			9.32E+03	5.8E-01	1.1E+01	3.5E+01					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-B01-A	1	5.50E+00	U1/2		5.50E+00	6.4E+01	1.1E+01	3.5E+01					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1313-B02-A	1	5.50E+00	U1/2		5.50E+00	5.7E+01	1.1E+01	3.5E+01					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	SWA-L07-1313-T01-A	1	9.45E+02			9.45E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T02-A	1	9.62E+01			9.62E+01	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T03-A	1	1.19E+03			1.19E+03	4.5E-01	1.0E+00	3.2E+00	1000	100	2.13E+03	94%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T04-A	1	1.88E+03			1.88E+03	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T05-A	1	3.41E+03			3.41E+03	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T06-A	1	4.41E+03			4.41E+03	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T07-A	1	6.94E+03			6.94E+03	4.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T08-A	1	6.15E+03			6.15E+03	7.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T09-A	1	1.77E+04			1.77E+04	3.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T01-B	1	9.47E+02			9.47E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T02-B	1	1.03E+02			1.03E+02	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T03-B	1	1.20E+03			1.20E+03	1.8E-01	1.0E+00	3.2E+00	1000	100	2.29E+03	109%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T04-B	1	1.95E+03			1.95E+03	2.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T05-B	1	2.93E+03			2.93E+03	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T06-B	1	4.87E+03			4.87E+03	1.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T07-B	1	6.32E+03			6.32E+03	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T08-B	1	5.90E+03			5.90E+03	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T09-B	1	6.15E+03			6.15E+03	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T01-C	1	1.09E+03			1.09E+03	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T02-C	1	1.61E+02			1.61E+02	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T03-C	1	1.19E+03			1.19E+03	2.9E+00	1.0E+00	3.2E+00	1000	100	2.35E+03	116%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T04-C	1	2.13E+03			2.13E+03	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T05-C	1	2.64E+03			2.64E+03	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T06-C	1	4.77E+03			4.77E+03	2.4E+00	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T07-C	1	6.58E+03			6.58E+03	5.8E-01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T08-C	1	6.79E+03			6.79E+03	6.6E-01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-T09-C	1	5.96E+03			5.96E+03	2.8E-01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-B01-A	1	1.28E+01			1.28E+01	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1313-B02-A	1	1.69E+01			1.69E+01	6.6E+00	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	SWA-L07-1313-T01-A	1	1.95E+02			1.95E+02	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T02-A	1	6.89E+02			6.89E+02	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T03-A	1	1.35E+03			1.35E+03	6.5E-01	1.0E+00	3.2E+00	10	100	2.31E+03	95%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T04-A	1	1.12E+03			1.12E+03	5.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T05-A	1	1.15E+03			1.15E+03	4.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T06-A	1	1.53E+03			1.53E+03	5.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T07-A	1	1.87E+03			1.87E+03	2.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T08-A	1	8.53E+02			8.53E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T09-A	1	9.37E+03			9.37E+03	7.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T01-B	1	2.02E+02			2.02E+02	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T02-B	1	7.17E+02			7.17E+02	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T03-B	1	1.29E+03			1.29E+03	1.7E-01	1.0E+00	3.2E+00	10	100	2.32E+03	102%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T04-B	1	1.09E+03			1.09E+03	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T05-B	1	1.16E+03			1.16E+03	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T06-B	1	1.53E+03			1.53E+03	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T07-B	1	1.62E+03			1.62E+03	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T08-B	1	7.52E+02			7.52E+02	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T09-B	1	9.18E+02			9.18E+02	8.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T01-C	1	2.00E+02			2.00E+02	3.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T02-C	1	6.96E+02			6.96E+02	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T03-C	1	1.51E+03			1.51E+03	2.1E+00	1.0E+00	3.2E+00	10	100	2.37E+03	86%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T04-C	1	1.16E+03			1.16E+03	8.8E-01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T05-C	1	1.29E+03			1.29E+03	9.2E-01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T06-C	1	1.39E+03			1.39E+03	2.8E+00	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T07-C	1	2.08E+03			2.08E+03	6.9E-01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T08-C	1	1.08E+03			1.08E+03	3.8E-01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-T09-C	1	9.13E+02			9.13E+02	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	5.0E-01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	3.9E+00	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	SWA-L07-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	8.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	4.7E+03	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	6.6E+01	1.9E+00	6.0E+00	10	100	1.07E+03	107%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	2.6E+03	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	1.9E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	2.9E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T07-A	1	9.50E-01	U1/2		9.50E-01	7.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T08-A	1	1.88E+01			1.88E+01	5.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T09-A	1	3.25E+02			3.25E+02	2.9E-01	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	5.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	4.6E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	2.3E+02	1.9E+00	6.0E+00	10	100	1.14E+03	114%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	4.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	8.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	4.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T07-B	1	9.50E-01	U1/2		9.50E-01	1.7E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T08-B	1	3.68E+01			3.68E+01	8.2E-01	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T09-B	1	1.35E+02			1.35E+02	1.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	3.7E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	5.0E+01	1.9E+00	6.0E+00	10	100	1.11E+03	111%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	1.9E+02	1.9E+00	6.0E+00					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	4.4E+01	1.9E+00	6.0E+00					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T07-C	1	9.50E-01	U1/2		9.50E-01	7.8E+01	1.9E+00	6.0E+00					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T08-C	1	6.48E+00			6.48E+00	1.2E+01	1.9E+00	6.0E+00					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-T09-C	1	1.24E+02			1.24E+02	5.5E-01	1.9E+00	6.0E+00					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	2.8E+02	1.9E+00	6.0E+00					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	2.7E+02	1.9E+00	6.0E+00					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	SWA-L07-1313-T01-A	1	1.10E+00	U1/2		1.10E+00	2.0E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T02-A	1	1.10E+00	U1/2		1.10E+00	4.5E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	3.5E+02	2.2E+00	7.0E+00	10	100	9.42E+02	94%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T04-A	1	1.10E+00	U1/2		1.10E+00	4.8E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T05-A	1	1.10E+00	U1/2		1.10E+00	1.3E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T06-A	1	1.10E+00	U1/2		1.10E+00	1.7E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T07-A	1	9.25E+00			9.25E+00	2.6E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T08-A	1	1.36E+01			1.36E+01	2.0E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T09-A	1	1.20E+02			1.20E+02	2.6E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T01-B	1	1.10E+00	U1/2		1.10E+00	9.9E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T02-B	1	1.10E+00	U1/2		1.10E+00	5.6E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	8.6E+01	2.2E+00	7.0E+00	10	100	1.01E+03	101%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T04-B	1	1.10E+00	U1/2		1.10E+00	6.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T05-B	1	1.10E+00	U1/2		1.10E+00	8.0E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T06-B	1	1.10E+00	U1/2		1.10E+00	8.9E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T07-B	1	1.27E+01			1.27E+01	1.7E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T08-B	1	1.62E+01			1.62E+01	1.4E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T09-B	1	3.37E+01			3.37E+01	7.7E-01	2.2E+00	7.0E+00				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T01-C	1	1.10E+00	U1/2		1.10E+00	1.5E+03	2.2E+00	7.0E+00				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T02-C	1	1.10E+00	U1/2		1.10E+00	1.1E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	1.9E+01	2.2E+00	7.0E+00	10	100	8.86E+02	88%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T04-C	1	1.10E+00	U1/2		1.10E+00	1.5E+02	2.2E+00	7.0E+00					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T05-C	1	1.10E+00	U1/2		1.10E+00	6.9E+01	2.2E+00	7.0E+00					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T06-C	1	1.10E+00	U1/2		1.10E+00	3.1E+01	2.2E+00	7.0E+00					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T07-C	1	7.01E+00			7.01E+00	1.1E+01	2.2E+00	7.0E+00					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T08-C	1	1.40E+01			1.40E+01	2.3E+00	2.2E+00	7.0E+00					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-T09-C	1	3.19E+01			3.19E+01	1.0E+00	2.2E+00	7.0E+00					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	1.4E+02	2.2E+00	7.0E+00					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	2.6E+02	2.2E+00	7.0E+00					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	SWA-L07-1313-T01-A	1	1.43E+04			1.43E+04	7.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T02-A	1	2.18E+05			2.18E+05	9.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T03-A	1	3.35E+06			3.35E+06	4.5E-01	2.6E+00	8.3E+00	1000	100	3.35E+06	84%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T04-A	1	5.58E+06			5.58E+06	8.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T05-A	1	6.86E+06			6.86E+06	6.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T06-A	1	7.89E+06			7.89E+06	9.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T07-A	1	8.63E+06			8.63E+06	1.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T08-A	1	3.87E+06			3.87E+06	5.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T09-A	1	1.41E+07			1.41E+07	9.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T01-B	1	1.49E+04			1.49E+04	2.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T02-B	1	2.32E+05			2.32E+05	7.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T03-B	1	2.91E+06			2.91E+06	1.1E+00	2.6E+00	8.3E+00	1000	100	2.91E+06	86%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T04-B	1	5.52E+06			5.52E+06	1.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T05-B	1	6.52E+06			6.52E+06	6.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T06-B	1	7.90E+06			7.90E+06	1.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T07-B	1	7.41E+06			7.41E+06	2.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T08-B	1	3.68E+06			3.68E+06	9.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T09-B	1	2.83E+06			2.83E+06	3.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T01-C	1	1.82E+04			1.82E+04	6.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T02-C	1	2.26E+05			2.26E+05	5.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T03-C	1	3.08E+06			3.08E+06	2.8E+00	2.6E+00	8.3E+00	1000	100	3.08E+06	84%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T04-C	1	5.99E+06			5.99E+06	6.5E-01	2.6E+00	8.3E+00					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T05-C	1	6.62E+06			6.62E+06	1.5E+00	2.6E+00	8.3E+00					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T06-C	1	7.78E+06			7.78E+06	2.9E+00	2.6E+00	8.3E+00					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T07-C	1	8.95E+06			8.95E+06	1.3E-01	2.6E+00	8.3E+00					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T08-C	1	4.73E+06			4.73E+06	9.2E-01	2.6E+00	8.3E+00					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-T09-C	1	2.96E+06			2.96E+06	1.2E+00	2.6E+00	8.3E+00					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-B01-A	1	4.36E+01			4.36E+01	2.8E+01	2.6E+00	8.3E+00					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1313-B02-A	1	8.26E+02			8.26E+02	4.5E-01	2.6E+00	8.3E+00					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	SWA-L07-1313-T01-A	1	1.10E+03			1.10E+03	2.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T02-A	1	1.38E+01			1.38E+01	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T03-A	1	7.92E+00			7.92E+00	2.9E+00	1.2E+00	3.8E+00	10	100	9.66E+02	96%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T04-A	1	1.37E+01			1.37E+01	1.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T05-A	1	1.86E+01			1.86E+01	6.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T06-A	1	1.56E+00	E		1.56E+00	6.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T07-A	1	1.16E+01			1.16E+01	7.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T08-A	1	2.47E+03			2.47E+03	5.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T09-A	1	7.55E+04			7.55E+04	7.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T01-B	1	1.08E+03			1.08E+03	1.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T02-B	1	1.52E+01			1.52E+01	4.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T03-B	1	9.89E+00			9.89E+00	1.7E+00	1.2E+00	3.8E+00	10	100	1.04E+03	103%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T04-B	1	8.93E+00			8.93E+00	1.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T05-B	1	1.18E+01			1.18E+01	1.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T06-B	1	6.00E-01	U1/2		6.00E-01	3.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T07-B	1	7.72E+01			7.72E+01	1.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T08-B	1	3.65E+03			3.65E+03	5.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T09-B	1	1.98E+04			1.98E+04	1.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T01-C	1	1.16E+03			1.16E+03	3.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T02-C	1	1.60E+01			1.60E+01	7.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T03-C	1	6.44E+00			6.44E+00	6.3E+01	1.2E+00	3.8E+00	10	100	9.34E+02	93%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T04-C	1	7.32E+00			7.32E+00	2.2E+01	1.2E+00	3.8E+00					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T05-C	1	6.66E+00			6.66E+00	3.1E+00	1.2E+00	3.8E+00					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T06-C	1	1.86E+00	E		1.86E+00	7.1E+00	1.2E+00	3.8E+00					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T07-C	1	7.35E+00			7.35E+00	7.5E+00	1.2E+00	3.8E+00					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T08-C	1	1.28E+03			1.28E+03	8.2E-01	1.2E+00	3.8E+00					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-T09-C	1	1.84E+04			1.84E+04	8.4E-01	1.2E+00	3.8E+00					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	1.6E+02	1.2E+00	3.8E+00					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	3.2E+01	1.2E+00	3.8E+00					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	SWA-L07-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	6.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T03-A	1	2.07E+00	E		2.07E+00	3.0E+01	1.8E+00	5.7E+00	10	100	9.27E+02	93%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T04-A	1	3.02E+00	E		3.02E+00	4.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T05-A	1	2.14E+01			2.14E+01	2.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T06-A	1	4.59E+01			4.59E+01	5.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T07-A	1	2.24E+02			2.24E+02	5.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T08-A	1	1.58E+02			1.58E+02	2.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T09-A	1	8.90E+02			8.90E+02	6.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	6.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	1.2E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T03-B	1	2.71E+00	E		2.71E+00	4.8E+01	1.8E+00	5.7E+00	10	100	1.01E+03	100%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T04-B	1	4.18E+00	E		4.18E+00	1.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T05-B	1	1.51E+01			1.51E+01	6.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T06-B	1	8.99E+01			8.99E+01	1.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T07-B	1	2.15E+02			2.15E+02	7.1E-02	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T08-B	1	1.55E+02			1.55E+02	7.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T09-B	1	2.14E+02			2.14E+02	9.3E-02	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	2.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	7.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T03-C	1	2.20E+00	E		2.20E+00	4.1E+00	1.8E+00	5.7E+00	10	100	9.18E+02	92%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T04-C	1	5.82E+00			5.82E+00	1.1E+01	1.8E+00	5.7E+00					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T05-C	1	1.74E+01			1.74E+01	2.9E+01	1.8E+00	5.7E+00					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T06-C	1	5.27E+01			5.27E+01	3.4E+01	1.8E+00	5.7E+00					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T07-C	1	2.05E+02			2.05E+02	2.2E-01	1.8E+00	5.7E+00					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T08-C	1	1.78E+02			1.78E+02	1.2E+00	1.8E+00	5.7E+00					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-T09-C	1	2.02E+02			2.02E+02	6.6E-01	1.8E+00	5.7E+00					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	4.4E+01	1.8E+00	5.7E+00					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	1.5E+01	1.8E+00	5.7E+00					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	SWA-L07-1313-T01-A	1	1.85E+00	U1/2		1.85E+00	1.4E+02	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T02-A	1	5.16E+00	E		5.16E+00	5.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T03-A	1	8.00E+00	E		8.00E+00	6.9E+00	3.7E+00	1.2E+01	10	100	1.01E+03	100%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T04-A	1	1.17E+01	E		1.17E+01	9.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T05-A	1	1.21E+01			1.21E+01	3.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T06-A	1	1.26E+01			1.26E+01	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T07-A	1	2.25E+01			2.25E+01	1.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T08-A	1	2.45E+01			2.45E+01	2.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T09-A	1	3.82E+03			3.82E+03	9.5E-01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T01-B	1	1.85E+00	U1/2		1.85E+00	3.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T02-B	1	4.81E+00	E		4.81E+00	2.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T03-B	1	9.01E+00	E		9.01E+00	4.1E+01	3.7E+00	1.2E+01	10	100	1.07E+03	106%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T04-B	1	1.39E+01			1.39E+01	2.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T05-B	1	1.09E+01	E		1.09E+01	5.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T06-B	1	1.65E+01			1.65E+01	3.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T07-B	1	2.30E+01			2.30E+01	1.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T08-B	1	5.29E+01			5.29E+01	1.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T09-B	1	1.43E+03			1.43E+03	1.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T01-C	1	1.85E+00	U1/2		1.85E+00	5.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T02-C	1	5.29E+00	E		5.29E+00	3.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T03-C	1	1.29E+01			1.29E+01	1.8E+01	3.7E+00	1.2E+01	10	100	1.04E+03	102%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T04-C	1	1.34E+01			1.34E+01	1.4E+01	3.7E+00	1.2E+01					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T05-C	1	1.20E+01			1.20E+01	2.9E+01	3.7E+00	1.2E+01					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T06-C	1	8.50E+00	E		8.50E+00	1.3E+01	3.7E+00	1.2E+01					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T07-C	1	2.69E+01			2.69E+01	1.0E+01	3.7E+00	1.2E+01					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T08-C	1	1.60E+01			1.60E+01	1.1E+01	3.7E+00	1.2E+01					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-T09-C	1	1.39E+03			1.39E+03	1.5E+00	3.7E+00	1.2E+01					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	5.3E+01	3.7E+00	1.2E+01					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	5.2E+01	3.7E+00	1.2E+01					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	SWA-L07-1313-T01-A	1	8.38E+01			8.38E+01	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T02-A	1	3.45E+01			3.45E+01	1.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T03-A	1	1.27E+01			1.27E+01	3.5E+00	2.0E+00	6.4E+00	1000	100	9.95E+02	98%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T04-A	1	1.77E+01			1.77E+01	1.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T05-A	1	1.48E+01			1.48E+01	8.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T06-A	1	1.78E+01			1.78E+01	3.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T07-A	1	8.83E+04			8.83E+04	7.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T08-A	1	9.95E+04			9.95E+04	1.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T09-A	1	9.70E+05			9.70E+05	7.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T01-B	1	7.86E+01			7.86E+01	1.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T02-B	1	3.51E+01			3.51E+01	1.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T03-B	1	1.31E+01			1.31E+01	8.8E+00	2.0E+00	6.4E+00	1000	100	1.08E+03	106%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T04-B	1	1.89E+01			1.89E+01	1.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T05-B	1	1.38E+01			1.38E+01	3.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T06-B	1	2.17E+01			2.17E+01	8.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T07-B	1	1.19E+05			1.19E+05	8.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T08-B	1	1.06E+05			1.06E+05	3.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T09-B	1	1.41E+05			1.41E+05	5.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T01-C	1	2.03E+02			2.03E+02	6.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T02-C	1	3.64E+01			3.64E+01	8.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T03-C	1	1.51E+01			1.51E+01	2.9E+00	2.0E+00	6.4E+00	1000	100	9.64E+02	95%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T04-C	1	1.83E+01			1.83E+01	2.2E+00	2.0E+00	6.4E+00					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T05-C	1	1.60E+01			1.60E+01	3.6E+00	2.0E+00	6.4E+00					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T06-C	1	1.89E+01			1.89E+01	4.6E+00	2.0E+00	6.4E+00					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T07-C	1	6.75E+04			6.75E+04	4.3E-02	2.0E+00	6.4E+00					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T08-C	1	1.11E+05			1.11E+05	7.4E-01	2.0E+00	6.4E+00					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-T09-C	1	1.37E+05			1.37E+05	2.2E+00	2.0E+00	6.4E+00					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-B01-A	1	2.58E+00	E		2.58E+00	6.1E+00	2.0E+00	6.4E+00					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1313-B02-A	1	1.14E+01			1.14E+01	2.8E+00	2.0E+00	6.4E+00					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	SWA-L07-1313-T01-A	1	1.33E+01	E		1.33E+01	1.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T02-A	1	3.40E+00	U1/2		3.40E+00	1.6E+02	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T03-A	1	3.40E+00	U1/2		3.40E+00	6.0E+02	6.8E+00	2.2E+01	10	100	9.17E+02	91%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T04-A	1	3.40E+00	U1/2		3.40E+00	3.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T05-A	1	3.40E+00	U1/2		3.40E+00	1.3E+02	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T06-A	1	3.40E+00	U1/2		3.40E+00	1.0E+02	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T07-A	1	3.40E+00	U1/2		3.40E+00	4.4E+02	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T08-A	1	9.32E+01			9.32E+01	1.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T09-A	1	1.36E+04			1.36E+04	5.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T01-B	1	1.35E+01	E		1.35E+01	3.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T02-B	1	3.40E+00	U1/2		3.40E+00	1.1E+02	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T03-B	1	3.40E+00	U1/2		3.40E+00	2.3E+03	6.8E+00	2.2E+01	10	100	9.91E+02	99%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T04-B	1	3.40E+00	U1/2		3.40E+00	1.2E+02	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T05-B	1	3.40E+00	U1/2		3.40E+00	7.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T06-B	1	3.40E+00	U1/2		3.40E+00	6.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T07-B	1	3.40E+00	U1/2		3.40E+00	2.6E+02	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T08-B	1	2.23E+02			2.23E+02	3.3E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T09-B	1	3.68E+03			3.68E+03	4.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T01-C	1	2.17E+01			2.17E+01	1.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T02-C	1	3.40E+00	U1/2		3.40E+00	1.9E+02	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T03-C	1	3.40E+00	U1/2		3.40E+00	1.2E+01	6.8E+00	2.2E+01	10	100	8.69E+02	87%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T04-C	1	3.40E+00	U1/2		3.40E+00	1.3E+02	6.8E+00	2.2E+01					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T05-C	1	3.40E+00	U1/2		3.40E+00	2.0E+01	6.8E+00	2.2E+01					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T06-C	1	3.40E+00	U1/2		3.40E+00	9.9E+01	6.8E+00	2.2E+01					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T07-C	1	3.40E+00	U1/2		3.40E+00	2.4E+02	6.8E+00	2.2E+01					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T08-C	1	2.99E+01			2.99E+01	2.2E+01	6.8E+00	2.2E+01					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-T09-C	1	3.39E+03			3.39E+03	9.4E-01	6.8E+00	2.2E+01					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	4.1E+01	6.8E+00	2.2E+01					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	2.5E+01	6.8E+00	2.2E+01					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	SWA-L07-1313-T01-A	1	2.14E+00	E		2.14E+00	6.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T02-A	1	2.14E+01			2.14E+01	1.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T03-A	1	2.71E+02			2.71E+02	4.5E+00	1.9E+00	6.0E+00	10	100	1.15E+03	88%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T04-A	1	6.50E+02			6.50E+02	9.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T05-A	1	8.18E+02			8.18E+02	3.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T06-A	1	9.72E+02			9.72E+02	3.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T07-A	1	1.24E+03			1.24E+03	3.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T08-A	1	6.50E+02			6.50E+02	2.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T09-A	1	1.05E+03			1.05E+03	1.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T01-B	1	2.52E+00	E		2.52E+00	1.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T02-B	1	2.23E+01			2.23E+01	7.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T03-B	1	2.15E+02			2.15E+02	5.0E+00	1.9E+00	6.0E+00	10	100	1.14E+03	92%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T04-B	1	6.40E+02			6.40E+02	1.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T05-B	1	7.49E+02			7.49E+02	2.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T06-B	1	1.03E+03			1.03E+03	2.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T07-B	1	1.12E+03			1.12E+03	5.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T08-B	1	6.38E+02			6.38E+02	4.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T09-B	1	6.61E+02			6.61E+02	1.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	9.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T02-C	1	2.52E+01			2.52E+01	9.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T03-C	1	2.18E+02			2.18E+02	4.7E+00	1.9E+00	6.0E+00	10	100	1.11E+03	89%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T04-C	1	7.05E+02			7.05E+02	1.8E+00	1.9E+00	6.0E+00					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T05-C	1	7.51E+02			7.51E+02	7.3E+00	1.9E+00	6.0E+00					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T06-C	1	9.99E+02			9.99E+02	9.0E+00	1.9E+00	6.0E+00					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T07-C	1	1.31E+03			1.31E+03	1.7E+00	1.9E+00	6.0E+00					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T08-C	1	7.82E+02			7.82E+02	6.9E+00	1.9E+00	6.0E+00					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-T09-C	1	6.33E+02			6.33E+02	1.1E+00	1.9E+00	6.0E+00					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	2.3E+01	1.9E+00	6.0E+00					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	SWA-L07-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	6.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	1.3E+01	2.0E+00	6.4E+00	10	100	9.58E+02	96%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T04-A	1	3.61E+02			3.61E+02	3.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T05-A	1	6.45E+03			6.45E+03	5.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T06-A	1	1.13E+04			1.13E+04	3.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T07-A	1	2.82E+04			2.82E+04	2.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T08-A	1	1.55E+04			1.55E+04	3.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T09-A	1	6.23E+04			6.23E+04	6.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	2.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	7.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	2.4E+01	2.0E+00	6.4E+00	10	100	1.01E+03	101%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T04-B	1	6.35E+02			6.35E+02	7.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T05-B	1	4.85E+03			4.85E+03	4.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T06-B	1	1.59E+04			1.59E+04	1.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T07-B	1	2.50E+04			2.50E+04	4.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T08-B	1	1.49E+04			1.49E+04	2.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T09-B	1	1.57E+04			1.57E+04	2.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	6.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	2.9E+00	2.0E+00	6.4E+00	10	100	1.16E+03	116%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T04-C	1	8.08E+02			8.08E+02	5.2E-01	2.0E+00	6.4E+00					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T05-C	1	1.94E+03			1.94E+03	8.1E-01	2.0E+00	6.4E+00					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T06-C	1	1.48E+04			1.48E+04	9.5E+00	2.0E+00	6.4E+00					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T07-C	1	2.71E+04			2.71E+04	7.0E-01	2.0E+00	6.4E+00					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T08-C	1	1.82E+04			1.82E+04	1.5E+00	2.0E+00	6.4E+00					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-T09-C	1	1.57E+04			1.57E+04	1.7E+00	2.0E+00	6.4E+00					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	8.6E+00	2.0E+00	6.4E+00					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	SWA-L07-1313-T01-A	1	1.29E+01			1.29E+01	6.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T02-A	1	7.97E+01			7.97E+01	2.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T03-A	1	5.69E+04			5.69E+04	1.9E-01	1.0E+00	3.2E+00	1000	100	5.79E+04	97%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T04-A	1	7.57E+05			7.57E+05	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T05-A	1	1.15E+06			1.15E+06	3.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T06-A	1	1.32E+06			1.32E+06	3.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T07-A	1	1.73E+06			1.73E+06	1.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T08-A	1	8.32E+05			8.32E+05	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T09-A	1	2.45E+06			2.45E+06	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T01-B	1	5.26E+00			5.26E+00	9.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T02-B	1	9.61E+01			9.61E+01	8.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T03-B	1	1.43E+04			1.43E+04	3.5E-01	1.0E+00	3.2E+00	1000	100	1.53E+04	99%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T04-B	1	7.61E+05			7.61E+05	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T05-B	1	1.04E+06			1.04E+06	5.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T06-B	1	1.36E+06			1.36E+06	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T07-B	1	1.46E+06			1.46E+06	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T08-B	1	7.89E+05			7.89E+05	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T09-B	1	6.71E+05			6.71E+05	1.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T01-C	1	6.18E+00			6.18E+00	9.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T02-C	1	9.48E+01			9.48E+01	8.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T03-C	1	1.44E+04			1.44E+04	3.2E+00	1.0E+00	3.2E+00	1000	100	1.53E+04	87%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T04-C	1	8.67E+05			8.67E+05	8.7E-01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T05-C	1	9.81E+05			9.81E+05	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T06-C	1	1.30E+06			1.30E+06	2.8E+00	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T07-C	1	1.74E+06			1.74E+06	3.0E-01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T08-C	1	1.01E+06			1.01E+06	4.1E-01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-T09-C	1	6.82E+05			6.82E+05	3.3E-01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-B01-A	1	5.09E+00			5.09E+00	8.9E+01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1313-B02-A	1	1.23E+02			1.23E+02	4.7E+00	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	SWA-L07-1313-T01-A	1	9.69E+01			9.69E+01	9.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T02-A	1	1.52E+02			1.52E+02	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T03-A	1	1.39E+02			1.39E+02	7.1E-01	1.2E+00	3.8E+00	10	100	1.14E+03	100%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T04-A	1	1.32E+02			1.32E+02	2.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T05-A	1	1.04E+02			1.04E+02	9.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T06-A	1	7.52E+01			7.52E+01	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T07-A	1	1.30E+01			1.30E+01	2.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T08-A	1	1.74E+01			1.74E+01	9.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T09-A	1	1.85E+02			1.85E+02	1.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T01-B	1	1.07E+02			1.07E+02	7.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T02-B	1	1.47E+02			1.47E+02	3.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T03-B	1	1.40E+02			1.40E+02	1.9E+00	1.2E+00	3.8E+00	10	100	1.21E+03	107%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T04-B	1	1.26E+02			1.26E+02	8.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T05-B	1	1.16E+02			1.16E+02	1.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T06-B	1	4.23E+01			4.23E+01	4.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T07-B	1	9.28E+00			9.28E+00	3.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T08-B	1	1.38E+01			1.38E+01	5.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T09-B	1	1.37E+01			1.37E+01	2.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T01-C	1	1.09E+02			1.09E+02	1.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T02-C	1	1.59E+02			1.59E+02	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T03-C	1	1.32E+02			1.32E+02	6.7E+00	1.2E+00	3.8E+00	10	100	1.06E+03	92%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T04-C	1	1.38E+02			1.38E+02	9.7E-01	1.2E+00	3.8E+00					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T05-C	1	1.31E+02			1.31E+02	2.0E+00	1.2E+00	3.8E+00					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T06-C	1	4.22E+01			4.22E+01	1.8E+00	1.2E+00	3.8E+00					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T07-C	1	1.53E+01			1.53E+01	1.7E+01	1.2E+00	3.8E+00					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T08-C	1	2.15E+01			2.15E+01	6.8E+00	1.2E+00	3.8E+00					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-T09-C	1	8.96E+00			8.96E+00	1.5E+01	1.2E+00	3.8E+00					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	1.8E+02	1.2E+00	3.8E+00					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1313-B02-A	1	2.31E+00	E		2.31E+00	6.5E+01	1.2E+00	3.8E+00					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	SWA-L07-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	2.7E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	2.6E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T03-A	1	4.91E+00	E		4.91E+00	5.7E+01	1.8E+00	5.7E+00	10	100	9.21E+02	92%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T04-A	1	1.10E+01			1.10E+01	2.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T05-A	1	6.46E+01			6.46E+01	2.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T06-A	1	1.38E+02			1.38E+02	1.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T07-A	1	5.34E+02			5.34E+02	3.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T08-A	1	3.40E+02			3.40E+02	3.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T09-A	1	1.28E+03			1.28E+03	5.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	2.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T02-B	1	2.21E+00	E		2.21E+00	4.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T03-B	1	3.80E+00	E		3.80E+00	5.6E+01	1.8E+00	5.7E+00	10	100	9.87E+02	98%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T04-B	1	1.03E+01			1.03E+01	1.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T05-B	1	4.24E+01			4.24E+01	7.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T06-B	1	2.62E+02			2.62E+02	4.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T07-B	1	4.91E+02			4.91E+02	2.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T08-B	1	3.20E+02			3.20E+02	3.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T09-B	1	3.55E+02			3.55E+02	9.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T01-C		9.00E-01	U1/2		0.00E+00	6.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T02-C		9.00E-01	U1/2		0.00E+00	3.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T03-C		5.50E+00	U1/2		0.00E+00	1.6E+00	1.8E+00	5.7E+00	10	100	1.00E+03	100%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T04-C		1.56E+01	U1/2		0.00E+00	1.3E+01	1.8E+00	5.7E+00					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T05-C		2.26E+01	U1/2		0.00E+00	3.0E+01	1.8E+00	5.7E+00					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T06-C		2.83E+02	U1/2		0.00E+00	2.5E+01	1.8E+00	5.7E+00					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T07-C		4.84E+02	U1/2		0.00E+00	6.3E-01	1.8E+00	5.7E+00					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T08-C		3.82E+02	U1/2		0.00E+00	7.8E-01	1.8E+00	5.7E+00					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-T09-C		3.52E+02	U1/2		0.00E+00	6.6E-01	1.8E+00	5.7E+00					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-B01-A		9.00E-01	U1/2		0.00E+00	2.9E+02	1.8E+00	5.7E+00					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1313-B02-A		9.00E-01	U1/2		0.00E+00	1.1E+02	1.8E+00	5.7E+00					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	SWA-L07-1313-T01-A	1	6.69E+01			6.69E+01	1.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T02-A	1	3.93E+01			3.93E+01	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T03-A	1	3.25E+01			3.25E+01	8.3E+01	3.7E+00	1.2E+01	1000	100	1.13E+03	110%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T04-A	1	8.99E+01			8.99E+01	1.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T05-A	1	7.94E+01			7.94E+01	2.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T06-A	1	7.38E+01			7.38E+01	2.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T07-A	1	7.80E+01			7.80E+01	2.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T08-A	1	8.21E+02			8.21E+02	2.7E-01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T09-A	1	1.20E+05			1.20E+05	2.8E-01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T01-B	1	6.42E+01			6.42E+01	1.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T02-B	1	4.53E+01			4.53E+01	8.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T03-B	1	3.24E+01			3.24E+01	3.7E+01	3.7E+00	1.2E+01	1000	100	1.22E+03	119%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T04-B	1	1.05E+02			1.05E+02	9.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T05-B	1	9.19E+01			9.19E+01	5.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T06-B	1	5.87E+01			5.87E+01	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T07-B	1	8.12E+01			8.12E+01	2.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T08-B	1	7.51E+02			7.51E+02	1.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T09-B	1	9.13E+03			9.13E+03	3.9E-01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T01-C	1	7.50E+01			7.50E+01	7.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T02-C	1	3.82E+01			3.82E+01	1.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T03-C	1	3.44E+01			3.44E+01	3.3E+01	3.7E+00	1.2E+01	1000	100	1.21E+03	118%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T04-C	1	1.32E+02			1.32E+02	1.2E+01	3.7E+00	1.2E+01					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T05-C	1	1.29E+02			1.29E+02	1.5E+01	3.7E+00	1.2E+01					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T06-C	1	5.54E+01			5.54E+01	8.5E+00	3.7E+00	1.2E+01					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T07-C	1	7.35E+01			7.35E+01	3.3E+01	3.7E+00	1.2E+01					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T08-C	1	8.79E+02			8.79E+02	1.0E+00	3.7E+00	1.2E+01					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-T09-C	1	4.22E+03			4.22E+03	9.7E-01	3.7E+00	1.2E+01					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	1.2E+01	3.7E+00	1.2E+01					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	9.0E+00	3.7E+00	1.2E+01					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	SWA-L07-1313-T01-A	1	3.03E+05			3.03E+05	7.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T02-A	1	3.61E+05			3.61E+05	1.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T03-A	1	4.36E+05			4.36E+05	2.3E+00	1.6E+00	5.1E+00	1000	100	4.37E+05	88%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T04-A	1	4.47E+05			4.47E+05	1.6E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T05-A	1	4.50E+05			4.50E+05	5.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T06-A	1	4.79E+05			4.79E+05	1.6E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T07-A	1	5.08E+05			5.08E+05	3.7E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T08-A	1	2.65E+05			2.65E+05	5.4E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T09-A	1	6.09E+05			6.09E+05	7.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T01-B	1	3.03E+05			3.03E+05	5.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T02-B	1	3.62E+05			3.62E+05	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T03-B	1	4.29E+05			4.29E+05	7.3E-01	1.6E+00	5.1E+00	1000	100	4.30E+05	95%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T04-B	1	4.35E+05			4.35E+05	1.4E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T05-B	1	4.52E+05			4.52E+05	1.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T06-B	1	4.74E+05			4.74E+05	7.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T07-B	1	5.29E+05			5.29E+05	1.1E+01	1.6E+00	5.1E+00				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T08-B	1	2.56E+05			2.56E+05	9.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T09-B	1	3.57E+05			3.57E+05	9.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T01-C	1	3.13E+05			3.13E+05	1.7E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T02-C	1	3.72E+05			3.72E+05	7.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T03-C	1	4.80E+05			4.80E+05	3.2E+00	1.6E+00	5.1E+00	1000	100	4.81E+05	81%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T04-C	1	4.47E+05			4.47E+05	1.5E+00	1.6E+00	5.1E+00					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T05-C	1	4.50E+05			4.50E+05	2.3E+00	1.6E+00	5.1E+00					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T06-C	1	4.29E+05			4.29E+05	3.2E+00	1.6E+00	5.1E+00					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T07-C	1	5.14E+05			5.14E+05	2.0E-01	1.6E+00	5.1E+00					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T08-C	1	3.24E+05			3.24E+05	8.3E+00	1.6E+00	5.1E+00					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-T09-C	1	3.65E+05			3.65E+05	1.2E+01	1.6E+00	5.1E+00					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-B01-A	1	5.61E+00			5.61E+00	1.3E+00	1.6E+00	5.1E+00					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1313-B02-A	1	9.83E+01			9.83E+01	2.1E+00	1.6E+00	5.1E+00					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	SWA-L07-1313-T01-A	1	9.32E+04			9.32E+04	8.3E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T02-A	1	9.73E+04			9.73E+04	1.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T03-A	1	1.04E+05			1.04E+05	4.5E-01	1.5E+01	4.8E+01	10	100	1.05E+05	91%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T04-A	1	1.17E+05			1.17E+05	3.8E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T05-A	1	1.23E+05			1.23E+05	2.8E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T06-A	1	1.28E+05			1.28E+05	3.2E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T07-A	1	1.24E+05			1.24E+05	5.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T08-A	1	5.23E+04			5.23E+04	7.9E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T09-A	1	9.69E+04			9.69E+04	8.7E-02	1.5E+01	4.8E+01				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T01-B	1	9.41E+04			9.41E+04	5.3E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T02-B	1	9.30E+04			9.30E+04	8.5E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T03-B	1	1.01E+05			1.01E+05	1.5E-01	1.5E+01	4.8E+01	10	100	1.02E+05	99%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T04-B	1	1.15E+05			1.15E+05	1.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T05-B	1	1.20E+05			1.20E+05	4.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T06-B	1	1.24E+05			1.24E+05	2.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T07-B	1	1.03E+05			1.03E+05	5.5E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T08-B	1	4.96E+04			4.96E+04	5.5E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T09-B	1	3.64E+04			3.64E+04	7.4E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T01-C	1	1.02E+05			1.02E+05	5.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T02-C	1	1.01E+05			1.01E+05	6.2E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T03-C	1	1.28E+05			1.28E+05	2.4E+00	1.5E+01	4.8E+01	10	100	1.29E+05	86%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T04-C	1	1.19E+05			1.19E+05	9.4E-01	1.5E+01	4.8E+01					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T05-C	1	1.24E+05			1.24E+05	9.7E-01	1.5E+01	4.8E+01					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T06-C	1	9.85E+04			9.85E+04	3.1E+00	1.5E+01	4.8E+01					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T07-C	1	1.28E+05			1.28E+05	3.7E-01	1.5E+01	4.8E+01					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T08-C	1	6.46E+04			6.46E+04	8.6E-01	1.5E+01	4.8E+01					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-T09-C	1	3.59E+04			3.59E+04	8.4E-01	1.5E+01	4.8E+01					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-B01-A	1	7.50E+00	U1/2		7.50E+00	3.8E+01	1.5E+01	4.8E+01					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1313-B02-A	1	7.50E+00	U1/2		7.50E+00	1.7E+01	1.5E+01	4.8E+01					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	SWA-L07-1313-T01-A	1	5.53E+03			5.53E+03	8.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T02-A	1	2.65E+03			2.65E+03	1.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T03-A	1	1.19E+03			1.19E+03	3.2E-01	1.1E+00	3.5E+00	1000	100	2.16E+03	97%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T04-A	1	1.19E+03			1.19E+03	4.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T05-A	1	1.59E+03			1.59E+03	2.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T06-A	1	1.97E+03			1.97E+03	7.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T07-A	1	2.65E+03			2.65E+03	2.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T08-A	1	1.57E+04			1.57E+04	5.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T09-A	1	2.87E+05			2.87E+05	1.6E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T01-B	1	5.66E+03			5.66E+03	6.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T02-B	1	2.69E+03			2.69E+03	1.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T03-B	1	1.41E+03			1.41E+03	1.8E-01	1.1E+00	3.5E+00	1000	100	2.26E+03	85%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T04-B	1	1.20E+03			1.20E+03	2.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T05-B	1	1.41E+03			1.41E+03	3.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T06-B	1	2.40E+03			2.40E+03	4.8E-02	1.1E+00	3.5E+00				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T07-B	1	2.66E+03			2.66E+03	6.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T08-B	1	1.13E+04			1.13E+04	1.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T09-B	1	1.21E+05			1.21E+05	4.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T01-C	1	5.76E+03			5.76E+03	8.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T02-C	1	2.58E+03			2.58E+03	6.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T03-C	1	1.53E+03			1.53E+03	2.2E+00	1.1E+00	3.5E+00	1000	100	2.33E+03	80%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T04-C	1	1.18E+03			1.18E+03	8.6E-01	1.1E+00	3.5E+00					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T05-C	1	1.31E+03			1.31E+03	1.2E+00	1.1E+00	3.5E+00					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T06-C	1	2.48E+03			2.48E+03	2.8E+00	1.1E+00	3.5E+00					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T07-C	1	2.61E+03			2.61E+03	4.1E-01	1.1E+00	3.5E+00					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T08-C	1	1.58E+04			1.58E+04	6.2E-01	1.1E+00	3.5E+00					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-T09-C	1	5.13E+04			5.13E+04	7.9E-01	1.1E+00	3.5E+00					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-B01-A	1	5.50E-01	U1/2		5.50E-01	3.6E+01	1.1E+00	3.5E+00					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1313-B02-A	1	4.01E+00			4.01E+00	2.2E+01	1.1E+00	3.5E+00					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	SWA-L07-1313-T01-A	1	3.61E+05			3.61E+05	1.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T02-A	1	3.88E+05			3.88E+05	1.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T03-A	1	3.82E+05			3.82E+05	2.0E-01	2.5E+00	8.0E+00	1000	100	3.83E+05	86%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T04-A	1	3.71E+05			3.71E+05	5.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T05-A	1	3.64E+05			3.64E+05	5.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T06-A	1	3.66E+05			3.66E+05	4.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T07-A	1	3.58E+05			3.58E+05	4.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T08-A	1	3.58E+05			3.58E+05	3.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T09-A	1	1.29E+06			1.29E+06	1.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T01-B	1	3.62E+05			3.62E+05	5.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T02-B	1	3.78E+05			3.78E+05	4.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T03-B	1	3.78E+05			3.78E+05	7.8E-01	2.5E+00	8.0E+00	1000	100	3.79E+05	92%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T04-B	1	3.67E+05			3.67E+05	6.6E-02	2.5E+00	8.0E+00				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T05-B	1	3.62E+05			3.62E+05	3.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T06-B	1	3.58E+05			3.58E+05	2.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T07-B	1	3.56E+05			3.56E+05	3.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T08-B	1	3.61E+05			3.61E+05	5.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T09-B	1	3.64E+05			3.64E+05	6.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T01-C	1	3.60E+05			3.60E+05	9.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T02-C	1	3.85E+05			3.85E+05	6.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T03-C	1	3.78E+05			3.78E+05	1.2E+00	2.5E+00	8.0E+00	1000	100	3.78E+05	82%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T04-C	1	3.62E+05			3.62E+05	5.0E-01	2.5E+00	8.0E+00					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T05-C	1	3.62E+05			3.62E+05	1.5E+00	2.5E+00	8.0E+00					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T06-C	1	3.61E+05			3.61E+05	2.2E+00	2.5E+00	8.0E+00					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T07-C	1	3.56E+05			3.56E+05	5.1E-01	2.5E+00	8.0E+00					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T08-C	1	3.52E+05			3.52E+05	5.2E-01	2.5E+00	8.0E+00					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-T09-C	1	3.52E+05			3.52E+05	1.4E+00	2.5E+00	8.0E+00					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-B01-A	1	1.25E+00	U1/2		1.25E+00	3.3E+01	2.5E+00	8.0E+00					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1313-B02-A	1	3.50E+02			3.50E+02	1.9E+00	2.5E+00	8.0E+00					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	SWA-L07-1313-T01-A	1	3.75E+02			3.75E+02	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T02-A	1	4.03E+03			4.03E+03	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T03-A	1	2.20E+04			2.20E+04	1.6E-01	1.0E+00	3.2E+00	1000	100	2.29E+04	86%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T04-A	1	3.21E+04			3.21E+04	2.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T05-A	1	3.91E+04			3.91E+04	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T06-A	1	4.57E+04			4.57E+04	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T07-A	1	5.44E+04			5.44E+04	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T08-A	1	2.70E+04			2.70E+04	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T09-A	1	7.99E+04			7.99E+04	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T01-B	1	3.85E+02			3.85E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T02-B	1	4.23E+03			4.23E+03	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T03-B	1	1.99E+04			1.99E+04	1.6E+00	1.0E+00	3.2E+00	1000	100	2.08E+04	89%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T04-B	1	3.18E+04			3.18E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T05-B	1	3.75E+04			3.75E+04	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T06-B	1	4.56E+04			4.56E+04	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T07-B	1	4.85E+04			4.85E+04	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T08-B	1	2.59E+04			2.59E+04	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T09-B	1	2.19E+04			2.19E+04	2.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T01-C	1	4.10E+02			4.10E+02	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T02-C	1	4.25E+03			4.25E+03	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T03-C	1	2.03E+04			2.03E+04	2.3E+00	1.0E+00	3.2E+00	1000	100	2.11E+04	85%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T04-C	1	3.46E+04			3.46E+04	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T05-C	1	3.77E+04			3.77E+04	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T06-C	1	4.92E+04			4.92E+04	4.2E+00	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T07-C	1	5.71E+04			5.71E+04	5.4E-01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T08-C	1	3.28E+04			3.28E+04	3.3E-01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-T09-C	1	2.21E+04			2.21E+04	1.7E+00	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	7.3E+01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1313-B02-A	1	3.76E+00			3.76E+00	4.2E+00	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	SWA-L07-1313-T01-A	1	9.64E+05			9.64E+05	4.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T02-A	1	1.04E+06			1.04E+06	1.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T03-A	1	1.03E+06			1.03E+06	9.8E-01	6.8E+00	2.2E+01	1000	100	1.03E+06	88%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T04-A	1	9.50E+05			9.50E+05	7.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T05-A	1	7.20E+05			7.20E+05	3.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T06-A	1	9.05E+05			9.05E+05	4.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T07-A	1	5.30E+05			5.30E+05	6.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T08-A	1	2.26E+05			2.26E+05	9.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T09-A	1	5.17E+05			5.17E+05	3.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T01-B	1	9.38E+05			9.38E+05	6.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T02-B	1	1.04E+06			1.04E+06	7.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T03-B	1	1.10E+06			1.10E+06	1.0E+00	6.8E+00	2.2E+01	1000	100	1.10E+06	95%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T04-B	1	1.04E+06			1.04E+06	1.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T05-B	1	9.29E+05			9.29E+05	2.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T06-B	1	8.22E+05			8.22E+05	6.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T07-B	1	4.54E+05			4.54E+05	4.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T08-B	1	2.10E+05			2.10E+05	1.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T09-B	1	1.55E+05			1.55E+05	4.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T01-C	1	1.03E+06			1.03E+06	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T02-C	1	1.11E+06			1.11E+06	9.9E-02	6.8E+00	2.2E+01				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T03-C	1	9.97E+05			9.97E+05	2.1E+00	6.8E+00	2.2E+01	1000	100	9.98E+05	92%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T04-C	1	1.00E+06			1.00E+06	6.2E-01	6.8E+00	2.2E+01					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T05-C	1	1.06E+06			1.06E+06	8.4E-01	6.8E+00	2.2E+01					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T06-C	1	8.80E+05			8.80E+05	1.9E+00	6.8E+00	2.2E+01					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T07-C	1	6.87E+05			6.87E+05	1.3E-01	6.8E+00	2.2E+01					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T08-C	1	2.82E+05			2.82E+05	7.0E-01	6.8E+00	2.2E+01					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-T09-C	1	1.59E+05			1.59E+05	5.3E-01	6.8E+00	2.2E+01					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-B01-A	1	1.28E+01	E		1.28E+01	6.0E+01	6.8E+00	2.2E+01					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1313-B02-A	1	8.64E+01			8.64E+01	2.4E+01	6.8E+00	2.2E+01					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	SWA-L07-1313-T01-A	1	2.30E+00	U1/2		2.30E+00	3.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T02-A	1	2.30E+00	U1/2		2.30E+00	3.9E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T03-A	1	2.30E+00	U1/2		2.30E+00	1.4E+02	4.6E+00	1.5E+01	10	100	8.48E+02	85%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T04-A	1	2.30E+00	U1/2		2.30E+00	8.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T05-A	1	2.30E+00	U1/2		2.30E+00	1.4E+02	4.6E+00	1.5E+01				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T06-A	1	1.29E+01	E		1.29E+01	3.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T07-A	1	3.26E+01			3.26E+01	1.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T08-A	1	9.15E+00	E		9.15E+00	3.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T09-A	1	2.30E+00	U1/2		2.30E+00	8.7E+00	4.6E+00	1.5E+01				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T01-B	1	2.30E+00	U1/2		2.30E+00	4.1E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T02-B	1	2.30E+00	U1/2		2.30E+00	6.9E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T03-B	1	2.30E+00	U1/2		2.30E+00	5.6E+01	4.6E+00	1.5E+01	10	100	9.13E+02	91%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T04-B	1	2.30E+00	U1/2		2.30E+00	2.7E+02	4.6E+00	1.5E+01				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T05-B	1	2.30E+00	U1/2		2.30E+00	4.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T06-B	1	1.09E+01	E		1.09E+01	3.4E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T07-B	1	2.30E+01			2.30E+01	1.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T08-B	1	7.93E+00	E		7.93E+00	2.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T09-B	1	2.30E+00	U1/2		2.30E+00	1.2E+02	4.6E+00	1.5E+01				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T01-C	1	2.30E+00	U1/2		2.30E+00	6.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T02-C	1	2.30E+00	U1/2		2.30E+00	8.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T03-C	1	2.30E+00	U1/2		2.30E+00	5.9E+02	4.6E+00	1.5E+01	10	100	8.19E+02	82%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T04-C	1	2.30E+00	U1/2		2.30E+00	2.0E+02	4.6E+00	1.5E+01					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T05-C	1	2.30E+00	U1/2		2.30E+00	5.6E+02	4.6E+00	1.5E+01					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T06-C	1	1.15E+01	E		1.15E+01	6.7E+01	4.6E+00	1.5E+01					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T07-C	1	3.09E+01			3.09E+01	2.7E+01	4.6E+00	1.5E+01					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T08-C	1	8.89E+00	E		8.89E+00	8.9E+01	4.6E+00	1.5E+01					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-T09-C	1	2.30E+00	U1/2		2.30E+00	1.1E+02	4.6E+00	1.5E+01					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	7.6E+01	4.6E+00	1.5E+01					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	3.8E+01	4.6E+00	1.5E+01					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	SWA-L07-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	2.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	3.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	8.2E+01	2.0E+00	6.4E+00	10	100	1.01E+03	101%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	8.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	5.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	4.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	5.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T08-A	1	5.97E+01			5.97E+01	1.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T09-A	1	1.52E+05			1.52E+05	1.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	1.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	8.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	1.6E+02	2.0E+00	6.4E+00	10	100	1.11E+03	111%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	4.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	3.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	7.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	1.8E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T08-B	1	5.69E+01			5.69E+01	1.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T09-B	1	1.58E+04			1.58E+04	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	1.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	3.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	5.4E+01	2.0E+00	6.4E+00	10	100	9.85E+02	98%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	1.0E+02	2.0E+00	6.4E+00					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	3.5E+01	2.0E+00	6.4E+00					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	7.5E+02	2.0E+00	6.4E+00					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	2.8E+01	2.0E+00	6.4E+00					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T08-C	1	8.26E+01			8.26E+01	1.1E+00	2.0E+00	6.4E+00					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-T09-C	1	1.56E+04			1.56E+04	7.9E-01	2.0E+00	6.4E+00					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	9.9E+00	2.0E+00	6.4E+00					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1313-B02-A	1	2.73E+00	E		2.73E+00	9.5E+00	2.0E+00	6.4E+00					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	SWA-L07-1313-T01-A	1	3.44E+02			3.44E+02	6.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T02-A	1	8.56E+01			8.56E+01	1.9E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T03-A	1	1.49E+02			1.49E+02	3.3E+00	1.5E+00	4.8E+00	10	100	1.15E+03	100%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T04-A	1	2.25E+02			2.25E+02	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T05-A	1	1.97E+02			1.97E+02	3.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T06-A	1	2.08E+02			2.08E+02	1.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T07-A	1	1.84E+02			1.84E+02	1.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T08-A	1	9.46E+01			9.46E+01	1.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T09-A	1	5.77E+03			5.77E+03	7.6E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T01-B	1	3.39E+02			3.39E+02	9.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T02-B	1	8.21E+01			8.21E+01	3.0E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T03-B	1	1.45E+02			1.45E+02	1.2E+00	1.5E+00	4.8E+00	10	100	1.21E+03	106%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T04-B	1	2.14E+02			2.14E+02	7.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T05-B	1	1.95E+02			1.95E+02	8.0E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T06-B	1	1.97E+02			1.97E+02	6.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T07-B	1	1.50E+02			1.50E+02	3.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T08-B	1	8.57E+01			8.57E+01	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T09-B	1	1.41E+03			1.41E+03	1.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T01-C	1	3.76E+02			3.76E+02	2.1E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T02-C	1	8.63E+01			8.63E+01	6.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T03-C	1	1.55E+02			1.55E+02	2.0E+00	1.5E+00	4.8E+00	10	100	1.18E+03	103%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T04-C	1	2.22E+02			2.22E+02	1.9E+00	1.5E+00	4.8E+00					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T05-C	1	2.10E+02			2.10E+02	1.6E+00	1.5E+00	4.8E+00					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T06-C	1	2.04E+02			2.04E+02	2.3E+00	1.5E+00	4.8E+00					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T07-C	1	2.02E+02			2.02E+02	1.2E+00	1.5E+00	4.8E+00					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T08-C	1	1.13E+02			1.13E+02	2.6E+00	1.5E+00	4.8E+00					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-T09-C	1	8.75E+02			8.75E+02	7.9E-01	1.5E+00	4.8E+00					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-B01-A	1	7.50E-01	U1/2		7.50E-01	3.9E+01	1.5E+00	4.8E+00					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1313-B02-A	1	7.50E-01	U1/2		7.50E-01	7.2E+01	1.5E+00	4.8E+00					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	SWA-L07-1313-T01-A	1	1.72E+00	E		1.72E+00	3.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:33 AM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T02-A	1	5.00E-01	U1/2		5.00E-01	7.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:34 AM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T03-A	1	1.97E+00	E		1.97E+00	4.7E+01	1.0E+00	3.2E+00	10	100	1.05E+03	105%	VU ICP-OES	11/3/10 11:36 AM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T04-A	1	1.37E+00	E		1.37E+00	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:38 AM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T05-A	1	2.65E+00	E		2.65E+00	1.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:39 AM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T06-A	1	1.67E+01			1.67E+01	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:41 AM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T07-A	1	6.78E+02			6.78E+02	8.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:43 AM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T08-A	1	1.15E+03			1.15E+03	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:44 AM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T09-A	1	5.65E+03			5.65E+03	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:46 AM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T01-B	1	5.00E-01	U1/2		5.00E-01	1.2E+02	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:51 AM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T02-B	1	1.34E+00	E		1.34E+00	2.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:53 AM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T03-B	1	1.74E+00	E		1.74E+00	4.7E+01	1.0E+00	3.2E+00	10	100	1.13E+03	113%	VU ICP-OES	11/3/10 11:54 AM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T04-B	1	2.34E+00	E		2.34E+00	2.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:56 AM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T05-B	1	2.90E+00	E		2.90E+00	1.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:58 AM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T06-B	1	8.23E+01			8.23E+01	9.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 11:59 AM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T07-B	1	9.74E+02			9.74E+02	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:01 PM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T08-B	1	1.21E+03			1.21E+03	8.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:03 PM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T09-B	1	2.01E+03			2.01E+03	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:04 PM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T01-C	1	1.93E+00	E		1.93E+00	1.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:09 PM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T02-C	1	5.00E-01	U1/2		5.00E-01	2.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	11/3/10 12:11 PM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T03-C	1	1.66E+00	E		1.66E+00	5.6E+00	1.0E+00	3.2E+00	10	100	1.09E+03	109%	VU ICP-OES	11/3/10 12:12 PM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T04-C	1	1.31E+00	E		1.31E+00	4.3E+01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:14 PM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T05-C	1	2.64E+00	E		2.64E+00	1.7E+01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:16 PM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T06-C	1	2.11E+01			2.11E+01	6.3E+00	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:17 PM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T07-C	1	5.53E+02			5.53E+02	2.2E-01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:19 PM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T08-C	1	1.14E+03			1.14E+03	8.2E-01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:21 PM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-T09-C	1	1.96E+03			1.96E+03	3.0E-01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 12:22 PM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	2.8E+01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 11:30 AM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1313-B02-A	1	1.22E+00	E		1.22E+00	2.4E+01	1.0E+00	3.2E+00					VU ICP-OES	11/3/10 11:31 AM	EPA Interlab L07 1313-1316 SWA

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	SWA-L09-1313-T01-A	1	5.64E+04			5.64E+04	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T02-A	1	3.46E+04			3.46E+04	8.1E-01	1.0E+00	3.2E+00	1000	100	3.55E+04	97%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T03-A	1	8.69E+02			8.69E+02	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T04-A	1	9.63E+01			9.63E+01	7.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T05-A	1	3.35E+01			3.35E+01	3.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T06-A	1	1.14E+01			1.14E+01	2.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T07-A	1	8.95E+00			8.95E+00	1.0E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T08-A	1	1.55E+05			1.55E+05	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T09-A	1	6.77E+05			6.77E+05	2.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T01-B	1	5.20E+04			5.20E+04	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T02-B	1	3.41E+04			3.41E+04	7.5E-01	1.0E+00	3.2E+00	1000	100	3.50E+04	86%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T03-B	1	6.54E+02			6.54E+02	2.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T04-B	1	1.09E+02			1.09E+02	6.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T05-B	1	3.31E+01			3.31E+01	2.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T06-B	1	1.49E+01			1.49E+01	4.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T07-B	1	8.56E+00			8.56E+00	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T08-B	1	1.59E+05			1.59E+05	9.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T09-B	1	6.15E+05			6.15E+05	3.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T01-C	1	5.07E+04			5.07E+04	3.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T02-C	1	3.77E+04			3.77E+04	2.5E-01	1.0E+00	3.2E+00	1000	100	3.87E+04	102%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T03-C	1	4.53E+02			4.53E+02	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T04-C	1	1.02E+02			1.02E+02	9.9E+00	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T05-C	1	5.55E+01			5.55E+01	2.0E+01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T06-C	1	1.56E+01			1.56E+01	6.9E+00	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T07-C	1	1.23E+01			1.23E+01	5.6E+00	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T08-C	1	3.54E+05			3.54E+05	6.0E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-T09-C	1	6.12E+05			6.12E+05	4.3E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	3.9E+02	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.4E+02	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-B03-A	1	6.24E+00			6.24E+00	5.1E+01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-B01-B	1	8.64E+00			8.64E+00	1.1E+00	1.0E+00	3.2E+00						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	4.1E+02	1.0E+00	3.2E+00						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	1.1E+02	1.0E+00	3.2E+00						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	1.9E+02	1.0E+00	3.2E+00						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	6.9E+02	1.0E+00	3.2E+00						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	SWA-L09-1313-T01-A	1	5.11E+03			5.11E+03	6.4E-01	7.5E+00	2.4E+01				---	VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T02-A	1	4.35E+03			4.35E+03	7.1E-01	7.5E+00	2.4E+01	10	100	5.42E+03	107%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T03-A	1	8.12E+02			8.12E+02	2.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T04-A	1	1.10E+03			1.10E+03	5.4E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T05-A	1	1.00E+03			1.00E+03	8.8E-01	7.5E+00	2.4E+01				---	VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T06-A	1	9.71E+02			9.71E+02	2.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T07-A	1	6.62E+02			6.62E+02	5.7E-01	7.5E+00	2.4E+01				---	VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T08-A	1	4.33E+02			4.33E+02	1.4E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T09-A	1	3.12E+04			3.12E+04	4.9E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T01-B	1	5.11E+03			5.11E+03	4.8E-01	7.5E+00	2.4E+01				---	VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T02-B	1	4.50E+03			4.50E+03	8.9E-01	7.5E+00	2.4E+01	10	100	5.47E+03	97%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T03-B	1	9.37E+02			9.37E+02	9.4E-01	7.5E+00	2.4E+01				---	VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T04-B	1	8.88E+02			8.88E+02	1.8E-01	7.5E+00	2.4E+01				---	VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T05-B	1	9.27E+02			9.27E+02	1.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T06-B	1	1.00E+03			1.00E+03	8.5E-01	7.5E+00	2.4E+01				---	VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T07-B	1	6.31E+02			6.31E+02	1.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T08-B	1	5.75E+02			5.75E+02	1.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T09-B	1	8.25E+02			8.25E+02	7.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T01-C	1	5.20E+03			5.20E+03	3.8E-01	7.5E+00	2.4E+01				---	VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T02-C	1	3.61E+03			3.61E+03	3.6E-01	7.5E+00	2.4E+01	10	100	4.56E+03	94%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T03-C	1	1.15E+03			1.15E+03	8.8E-01	7.5E+00	2.4E+01				---	VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T04-C	1	1.15E+03			1.15E+03	5.7E-01	7.5E+00	2.4E+01					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T05-C	1	1.22E+03			1.22E+03	5.5E-01	7.5E+00	2.4E+01					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T06-C	1	7.99E+02			7.99E+02	2.3E+00	7.5E+00	2.4E+01					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T07-C	1	8.76E+02			8.76E+02	3.7E-01	7.5E+00	2.4E+01					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T08-C	1	6.06E+02			6.06E+02	9.6E+00	7.5E+00	2.4E+01					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-T09-C	1	8.61E+02			8.61E+02	1.1E+01	7.5E+00	2.4E+01					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-B01-A	1	3.75E+00	U1/2		3.75E+00	1.1E+02	7.5E+00	2.4E+01					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-B02-A	1	3.75E+00	U1/2		3.75E+00	7.2E+01	7.5E+00	2.4E+01					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-B03-A	1	3.75E+00	U1/2		3.75E+00	6.9E+01	7.5E+00	2.4E+01					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-B01-B	1	3.75E+00	U1/2		3.75E+00	7.5E+01	7.5E+00	2.4E+01						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-B03-B	1	3.75E+00	U1/2		3.75E+00	1.1E+02	7.5E+00	2.4E+01						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-B01-C	1	3.75E+00	U1/2		3.75E+00	2.3E+00	7.5E+00	2.4E+01						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-B02-C	1	3.75E+00	U1/2		3.75E+00	5.0E+01	7.5E+00	2.4E+01						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1313-B03-C	1	3.75E+00	U1/2		3.75E+00	6.5E+01	7.5E+00	2.4E+01						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	SWA-L09-1313-T01-A	1	7.81E+03			7.81E+03	9.9E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T02-A	1	4.08E+03			4.08E+03	1.1E+00	1.1E+01	3.5E+01	10	100	4.92E+03	84%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T03-A	1	1.28E+02			1.28E+02	7.6E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T04-A	1	1.29E+02			1.29E+02	4.7E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T05-A	1	1.65E+02			1.65E+02	5.5E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T06-A	1	1.68E+02			1.68E+02	3.7E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T07-A	1	1.47E+02			1.47E+02	3.3E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T08-A	1	1.71E+03			1.71E+03	6.3E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T09-A	1	1.67E+04			1.67E+04	5.3E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T01-B	1	7.73E+03			7.73E+03	5.3E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T02-B	1	3.89E+03			3.89E+03	6.6E-01	1.1E+01	3.5E+01	10	100	4.78E+03	88%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T03-B	1	1.53E+02			1.53E+02	1.4E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T04-B	1	3.21E+02			3.21E+02	3.9E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T05-B	1	1.63E+02			1.63E+02	4.0E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T06-B	1	2.17E+02			2.17E+02	5.6E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T07-B	1	8.17E+02			8.17E+02	1.7E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T08-B	1	1.48E+03			1.48E+03	7.9E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T09-B	1	5.07E+03			5.07E+03	5.5E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T01-C	1	7.51E+03			7.51E+03	6.9E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T02-C	1	4.60E+03			4.60E+03	2.0E-01	1.1E+01	3.5E+01	10	100	5.45E+03	85%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T03-C	1	1.18E+02			1.18E+02	6.4E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T04-C	1	3.03E+02			3.03E+02	2.5E+00	1.1E+01	3.5E+01					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T05-C	1	3.29E+02			3.29E+02	4.8E+00	1.1E+01	3.5E+01					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T06-C	1	2.39E+02			2.39E+02	9.3E-01	1.1E+01	3.5E+01					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T07-C	1	2.65E+02			2.65E+02	5.7E+00	1.1E+01	3.5E+01					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T08-C	1	1.97E+03			1.97E+03	4.8E-01	1.1E+01	3.5E+01					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-T09-C	1	4.53E+03			4.53E+03	4.6E-01	1.1E+01	3.5E+01					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-B01-A	1	5.50E+00	U1/2		5.50E+00	5.1E+01	1.1E+01	3.5E+01					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-B02-A	1	5.50E+00	U1/2		5.50E+00	5.6E+01	1.1E+01	3.5E+01					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-B03-A	1	5.50E+00	U1/2		5.50E+00	4.6E+01	1.1E+01	3.5E+01					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-B01-B	1	5.50E+00	U1/2		5.50E+00	2.4E+02	1.1E+01	3.5E+01						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-B03-B	1	5.50E+00	U1/2		5.50E+00	1.1E+02	1.1E+01	3.5E+01						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-B01-C	1	5.50E+00	U1/2		5.50E+00	4.2E+01	1.1E+01	3.5E+01						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-B02-C	1	5.50E+00	U1/2		5.50E+00	6.4E+01	1.1E+01	3.5E+01						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1313-B03-C	1	5.50E+00	U1/2		5.50E+00	7.6E+01	1.1E+01	3.5E+01						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	SWA-L09-1313-T01-A	1	1.05E+03			1.05E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T02-A	1	8.38E+02			8.38E+02	1.4E+00	1.0E+00	3.2E+00	1000	100	1.86E+03	102%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T03-A	1	7.89E+02			7.89E+02	1.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T04-A	1	1.17E+03			1.17E+03	5.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T05-A	1	2.03E+03			2.03E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T06-A	1	2.43E+03			2.43E+03	9.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T07-A	1	3.62E+03			3.62E+03	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T08-A	1	3.58E+03			3.58E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T09-A	1	4.30E+03			4.30E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T01-B	1	9.89E+02			9.89E+02	3.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T02-B	1	8.78E+02			8.78E+02	6.0E-01	1.0E+00	3.2E+00	1000	100	1.80E+03	92%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T03-B	1	8.87E+02			8.87E+02	1.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T04-B	1	1.41E+03			1.41E+03	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T05-B	1	2.09E+03			2.09E+03	4.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T06-B	1	4.15E+03			4.15E+03	4.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T07-B	1	4.39E+03			4.39E+03	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T08-B	1	4.49E+03			4.49E+03	8.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T09-B	1	4.68E+03			4.68E+03	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T01-C	1	1.02E+03			1.02E+03	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T02-C	1	9.87E+02			9.87E+02	3.5E-01	1.0E+00	3.2E+00	1000	100	1.97E+03	99%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T03-C	1	9.06E+02			9.06E+02	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T04-C	1	1.48E+03			1.48E+03	4.7E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T05-C	1	1.88E+03			1.88E+03	4.5E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T06-C	1	3.98E+03			3.98E+03	5.9E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T07-C	1	4.37E+03			4.37E+03	4.1E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T08-C	1	4.68E+03			4.68E+03	2.2E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-T09-C	1	4.70E+03			4.70E+03	6.0E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	7.4E+01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	8.1E+01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	6.5E+01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	6.3E+01	1.0E+00	3.2E+00						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	4.6E+01	1.0E+00	3.2E+00						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	7.6E+02	1.0E+00	3.2E+00						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	5.1E+01	1.0E+00	3.2E+00						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	1.4E+02	1.0E+00	3.2E+00						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	SWA-L09-1313-T01-A	1	2.64E+02			2.64E+02	5.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T02-A	1	1.77E+02			1.77E+02	3.3E-01	1.0E+00	3.2E+00	10	100	1.18E+03	100%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T03-A	1	9.20E+02			9.20E+02	2.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T04-A	1	9.52E+02			9.52E+02	7.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T05-A	1	1.07E+03			1.07E+03	2.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T06-A	1	1.00E+03			1.00E+03	2.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T07-A	1	1.64E+03			1.64E+03	2.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T08-A	1	7.87E+02			7.87E+02	8.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T09-A	1	8.18E+02			8.18E+02	9.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T01-B	1	2.20E+02			2.20E+02	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T02-B	1	1.70E+02			1.70E+02	1.2E-01	1.0E+00	3.2E+00	10	100	1.15E+03	98%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T03-B	1	1.11E+03			1.11E+03	3.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T04-B	1	9.99E+02			9.99E+02	4.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T05-B	1	1.07E+03			1.07E+03	3.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T06-B	1	1.54E+03			1.54E+03	4.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T07-B	1	1.49E+03			1.49E+03	6.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T08-B	1	7.64E+02			7.64E+02	6.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T09-B	1	7.21E+02			7.21E+02	3.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T01-C	1	2.57E+02			2.57E+02	1.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T02-C	1	1.70E+02			1.70E+02	2.6E-01	1.0E+00	3.2E+00	10	100	1.18E+03	101%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T03-C	1	1.05E+03			1.05E+03	3.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T04-C	1	1.11E+03			1.11E+03	6.6E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T05-C	1	1.27E+03			1.27E+03	1.7E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T06-C	1	1.55E+03			1.55E+03	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T07-C	1	1.73E+03			1.73E+03	3.0E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T08-C	1	6.45E+02			6.45E+02	6.6E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-T09-C	1	7.10E+02			7.10E+02	5.1E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	2.0E+02	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	7.5E+01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	3.3E+00	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-B01-B	1	2.69E+00	E		2.69E+00	1.4E+00	1.0E+00	3.2E+00						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	8.4E+01	1.0E+00	3.2E+00						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	7.7E+01	1.0E+00	3.2E+00						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	7.4E+00	1.0E+00	3.2E+00						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	9.9E+01	1.0E+00	3.2E+00						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	SWA-L09-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	4.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	3.5E+01	1.9E+00	6.0E+00	10	100	9.94E+02	99%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	8.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	9.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	3.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T07-A	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T08-A	1	1.76E+01			1.76E+01	1.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T09-A	1	9.42E+01			9.42E+01	7.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	4.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	9.2E+01	1.9E+00	6.0E+00	10	100	9.62E+02	96%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	4.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	1.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	3.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	6.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T07-B	1	9.50E-01	U1/2		9.50E-01	1.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T08-B	1	1.69E+01			1.69E+01	5.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T09-B	1	9.99E+01			9.99E+01	8.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	5.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	6.3E+01	1.9E+00	6.0E+00	10	100	9.94E+02	99%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	7.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	7.5E+01	1.9E+00	6.0E+00					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	6.3E+01	1.9E+00	6.0E+00					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	3.1E+01	1.9E+00	6.0E+00					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T07-C	1	9.50E-01	U1/2		9.50E-01	6.8E+01	1.9E+00	6.0E+00					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T08-C	1	5.55E+01			5.55E+01	9.9E-01	1.9E+00	6.0E+00					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-T09-C	1	9.95E+01			9.95E+01	9.0E-01	1.9E+00	6.0E+00					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	4.4E+02	1.9E+00	6.0E+00					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	3.1E+01	1.9E+00	6.0E+00					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	4.4E+01	1.9E+00	6.0E+00					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-B01-B	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-B03-B	1	9.50E-01	U1/2		9.50E-01	6.9E+01	1.9E+00	6.0E+00						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-B01-C	1	9.50E-01	U1/2		9.50E-01	1.1E+01	1.9E+00	6.0E+00						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-B02-C	1	9.50E-01	U1/2		9.50E-01	1.5E+02	1.9E+00	6.0E+00						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1313-B03-C	1	9.50E-01	U1/2		9.50E-01	4.5E+01	1.9E+00	6.0E+00						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	SWA-L09-1313-T01-A	1	1.10E+00	U1/2		1.10E+00	9.2E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T02-A	1	1.10E+00	U1/2		1.10E+00	1.7E+01	2.2E+00	7.0E+00	10	100	8.95E+02	89%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	4.7E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T04-A	1	1.10E+00	U1/2		1.10E+00	5.7E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T05-A	1	1.10E+00	U1/2		1.10E+00	1.8E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T06-A	1	1.10E+00	U1/2		1.10E+00	4.2E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T07-A	1	7.29E+00			7.29E+00	1.1E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T08-A	1	9.86E+00			9.86E+00	4.1E+00	2.2E+00	7.0E+00			---		VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T09-A	1	3.59E+01			3.59E+01	7.4E+00	2.2E+00	7.0E+00			---		VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T01-B	1	1.10E+00	U1/2		1.10E+00	9.7E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T02-B	1	1.10E+00	U1/2		1.10E+00	7.0E+01	2.2E+00	7.0E+00	10	100	8.71E+02	87%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	6.1E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T04-B	1	1.10E+00	U1/2		1.10E+00	8.2E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T05-B	1	1.10E+00	U1/2		1.10E+00	4.3E+00	2.2E+00	7.0E+00			---		VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T06-B	1	2.54E+00	E		2.54E+00	1.9E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T07-B	1	7.98E+00			7.98E+00	8.8E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T08-B	1	1.06E+01			1.06E+01	3.8E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T09-B	1	2.54E+01			2.54E+01	3.9E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T01-C	1	1.10E+00	U1/2		1.10E+00	1.4E+02	2.2E+00	7.0E+00			---		VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T02-C	1	1.10E+00	U1/2		1.10E+00	1.8E+02	2.2E+00	7.0E+00	10	100	8.88E+02	89%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	5.9E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T04-C	1	1.10E+00	U1/2		1.10E+00	5.6E+00	2.2E+00	7.0E+00					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T05-C	1	1.10E+00	U1/2		1.10E+00	6.9E+01	2.2E+00	7.0E+00					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T06-C	1	2.77E+00	E		2.77E+00	8.8E+00	2.2E+00	7.0E+00					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T07-C	1	7.30E+00			7.30E+00	5.5E+00	2.2E+00	7.0E+00					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T08-C	1	1.78E+01			1.78E+01	5.1E-01	2.2E+00	7.0E+00					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-T09-C	1	2.44E+01			2.44E+01	6.7E-01	2.2E+00	7.0E+00					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	1.1E+02	2.2E+00	7.0E+00					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	1.2E+02	2.2E+00	7.0E+00					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-B03-A	1	1.10E+00	U1/2		1.10E+00	7.0E+01	2.2E+00	7.0E+00					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-B01-B	1	1.10E+00	U1/2		1.10E+00	7.4E+01	2.2E+00	7.0E+00						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-B03-B	1	1.10E+00	U1/2		1.10E+00	9.8E+02	2.2E+00	7.0E+00						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-B01-C	1	1.10E+00	U1/2		1.10E+00	2.7E+02	2.2E+00	7.0E+00						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-B02-C	1	1.10E+00	U1/2		1.10E+00	9.1E+01	2.2E+00	7.0E+00						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1313-B03-C	1	1.10E+00	U1/2		1.10E+00	1.1E+02	2.2E+00	7.0E+00						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	SWA-L09-1313-T01-A	1	7.97E+03			7.97E+03	9.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T02-A	1	1.28E+04			1.28E+04	7.3E-01	2.6E+00	8.3E+00	1000	100	1.40E+04	117%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T03-A	1	1.66E+06			1.66E+06	1.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T04-A	1	3.89E+06			3.89E+06	1.9E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T05-A	1	6.05E+06			6.05E+06	4.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T06-A	1	6.37E+06			6.37E+06	1.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T07-A	1	8.39E+06			8.39E+06	4.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T08-A	1	3.92E+06			3.92E+06	1.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T09-A	1	3.04E+06			3.04E+06	6.6E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T01-B	1	8.08E+03			8.08E+03	2.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T02-B	1	1.31E+04			1.31E+04	5.5E-01	2.6E+00	8.3E+00	1000	100	1.41E+04	95%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T03-B	1	2.03E+06			2.03E+06	3.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T04-B	1	4.69E+06			4.69E+06	5.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T05-B	1	6.15E+06			6.15E+06	5.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T06-B	1	7.92E+06			7.92E+06	8.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T07-B	1	5.32E+06			5.32E+06	1.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T08-B	1	4.34E+06			4.34E+06	7.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T09-B	1	2.81E+06			2.81E+06	5.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T01-C	1	7.58E+03			7.58E+03	5.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T02-C	1	1.26E+04			1.26E+04	1.6E-01	2.6E+00	8.3E+00	1000	100	1.35E+04	92%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T03-C	1	2.04E+06			2.04E+06	7.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T04-C	1	4.90E+06			4.90E+06	8.8E-01	2.6E+00	8.3E+00					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T05-C	1	6.17E+06			6.17E+06	9.1E-01	2.6E+00	8.3E+00					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T06-C	1	7.43E+06			7.43E+06	3.4E-01	2.6E+00	8.3E+00					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T07-C	1	7.58E+06			7.58E+06	7.4E-01	2.6E+00	8.3E+00					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T08-C	1	3.38E+06			3.38E+06	6.4E-01	2.6E+00	8.3E+00					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-T09-C	1	2.79E+06			2.79E+06	5.4E-01	2.6E+00	8.3E+00					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-B01-A	1	2.65E+01			2.65E+01	1.7E+00	2.6E+00	8.3E+00					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-B02-A	1	2.69E+01			2.69E+01	1.6E+01	2.6E+00	8.3E+00					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-B03-A	1	2.99E+01			2.99E+01	9.6E+00	2.6E+00	8.3E+00					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-B01-B	1	3.52E+01			3.52E+01	1.7E+01	2.6E+00	8.3E+00						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-B03-B	1	2.75E+01			2.75E+01	1.2E+01	2.6E+00	8.3E+00						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-B01-C	1	4.59E+01			4.59E+01	1.3E+02	2.6E+00	8.3E+00						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-B02-C	1	2.99E+01			2.99E+01	1.6E+01	2.6E+00	8.3E+00						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1313-B03-C	1	3.96E+01			3.96E+01	8.6E+00	2.6E+00	8.3E+00						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	SWA-L09-1313-T01-A	1	1.35E+03			1.35E+03	1.9E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T02-A	1	9.90E+02			9.90E+02	1.3E+00	1.2E+00	3.8E+00	10	100	1.89E+03	90%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T03-A	1	1.07E+01			1.07E+01	9.5E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T04-A	1	9.29E+00			9.29E+00	1.6E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T05-A	1	7.08E+00			7.08E+00	3.2E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T06-A	1	1.69E+00	E		1.69E+00	7.3E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T07-A	1	6.32E+00			6.32E+00	2.8E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T08-A	1	1.74E+03			1.74E+03	1.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T09-A	1	1.62E+04			1.62E+04	8.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T01-B	1	1.34E+03			1.34E+03	2.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T02-B	1	1.08E+03			1.08E+03	1.5E+00	1.2E+00	3.8E+00	10	100	1.94E+03	86%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T03-B	1	1.08E+01			1.08E+01	2.0E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T04-B	1	8.36E+00			8.36E+00	1.7E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T05-B	1	6.04E+00			6.04E+00	5.4E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T06-B	1	1.97E+00	E		1.97E+00	3.7E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T07-B	1	8.21E+00			8.21E+00	4.1E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T08-B	1	1.59E+03			1.59E+03	7.3E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T09-B	1	1.36E+04			1.36E+04	4.4E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T01-C	1	1.34E+03			1.34E+03	8.4E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T02-C	1	1.16E+03			1.16E+03	7.2E-01	1.2E+00	3.8E+00	10	100	2.04E+03	89%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T03-C	1	1.41E+01			1.41E+01	3.0E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T04-C	1	9.92E+00			9.92E+00	2.0E+00	1.2E+00	3.8E+00					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T05-C	1	9.55E+00			9.55E+00	2.7E+00	1.2E+00	3.8E+00					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T06-C	1	1.67E+00	E		1.67E+00	9.2E+00	1.2E+00	3.8E+00					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T07-C	1	8.38E+00			8.38E+00	1.1E+01	1.2E+00	3.8E+00					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T08-C	1	4.94E+03			4.94E+03	1.5E-01	1.2E+00	3.8E+00					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-T09-C	1	1.32E+04			1.32E+04	5.0E-01	1.2E+00	3.8E+00					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	1.2E+02	1.2E+00	3.8E+00					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	1.5E+02	1.2E+00	3.8E+00					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-B03-A	1	6.00E-01	U1/2		6.00E-01	2.7E+01	1.2E+00	3.8E+00					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-B01-B	1	6.00E-01	U1/2		6.00E-01	7.2E+01	1.2E+00	3.8E+00						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-B03-B	1	6.00E-01	U1/2		6.00E-01	2.9E+01	1.2E+00	3.8E+00						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-B01-C	1	6.00E-01	U1/2		6.00E-01	1.6E+01	1.2E+00	3.8E+00						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-B02-C	1	6.00E-01	U1/2		6.00E-01	5.3E+01	1.2E+00	3.8E+00						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1313-B03-C	1	6.00E-01	U1/2		6.00E-01	1.4E+02	1.2E+00	3.8E+00						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	SWA-L09-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	1.7E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	2.6E+01	1.8E+00	5.7E+00	10	100	1.01E+03	101%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T03-A	1	2.94E+00	E		2.94E+00	7.9E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T04-A	1	3.32E+00	E		3.32E+00	5.2E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T05-A	1	5.47E+00	E		5.47E+00	8.5E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T06-A	1	4.23E+00	E		4.23E+00	3.8E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T07-A	1	9.72E+01			9.72E+01	2.2E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T08-A	1	1.17E+02			1.17E+02	1.4E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T09-A	1	2.04E+02			2.04E+02	1.5E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	5.8E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	3.9E+01	1.8E+00	5.7E+00	10	100	9.81E+02	98%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T03-B	1	3.04E+00	E		3.04E+00	5.1E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T04-B	1	3.22E+00	E		3.22E+00	4.8E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T05-B	1	5.60E+00	E		5.60E+00	4.8E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T06-B	1	1.17E+02			1.17E+02	2.4E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T07-B	1	1.47E+02			1.47E+02	1.3E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T08-B	1	1.28E+02			1.28E+02	2.6E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T09-B	1	1.65E+02			1.65E+02	7.3E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	2.1E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	2.5E+01	1.8E+00	5.7E+00	10	100	1.01E+03	100%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T03-C	1	3.54E+00	E		3.54E+00	4.8E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T04-C	1	2.78E+00	E		2.78E+00	3.4E+01	1.8E+00	5.7E+00					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T05-C	1	4.72E+00	E		4.72E+00	4.7E+01	1.8E+00	5.7E+00					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T06-C	1	1.41E+02			1.41E+02	1.2E+00	1.8E+00	5.7E+00					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T07-C	1	1.47E+02			1.47E+02	2.7E-01	1.8E+00	5.7E+00					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T08-C	1	1.44E+02			1.44E+02	5.4E-01	1.8E+00	5.7E+00					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-T09-C	1	1.64E+02			1.64E+02	4.6E-01	1.8E+00	5.7E+00					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	3.7E+02	1.8E+00	5.7E+00					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	9.4E+01	1.8E+00	5.7E+00					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	7.5E+02	1.8E+00	5.7E+00					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-B01-B	1	9.00E-01	U1/2		9.00E-01	4.4E+01	1.8E+00	5.7E+00						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-B03-B	1	9.00E-01	U1/2		9.00E-01	1.7E+02	1.8E+00	5.7E+00						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-B01-C	1	9.00E-01	U1/2		9.00E-01	2.1E+02	1.8E+00	5.7E+00						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-B02-C	1	9.00E-01	U1/2		9.00E-01	2.9E+02	1.8E+00	5.7E+00						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1313-B03-C	1	9.00E-01	U1/2		9.00E-01	1.4E+01	1.8E+00	5.7E+00						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	SWA-L09-1313-T01-A	1	1.85E+00	U1/2		1.85E+00	9.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T02-A	1	1.85E+00	U1/2		1.85E+00	2.0E+02	3.7E+00	1.2E+01	10	100	1.04E+03	104%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T03-A	1	8.20E+00	E		8.20E+00	9.0E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T04-A	1	9.22E+00	E		9.22E+00	9.3E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T05-A	1	1.72E+01			1.72E+01	8.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T06-A	1	1.69E+01			1.69E+01	1.6E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T07-A	1	2.11E+01			2.11E+01	1.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T08-A	1	3.04E+01			3.04E+01	2.1E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T09-A	1	1.04E+03			1.04E+03	1.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T01-B	1	1.85E+00	U1/2		1.85E+00	3.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T02-B	1	1.85E+00	U1/2		1.85E+00	1.1E+01	3.7E+00	1.2E+01	10	100	1.00E+03	100%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T03-B	1	7.51E+00	E		7.51E+00	2.0E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T04-B	1	1.28E+01			1.28E+01	1.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T05-B	1	1.37E+01			1.37E+01	1.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T06-B	1	2.31E+01			2.31E+01	6.1E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T07-B	1	2.24E+01			2.24E+01	1.9E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T08-B	1	2.19E+01			2.19E+01	6.9E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T09-B	1	1.06E+03			1.06E+03	6.4E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T01-C	1	1.85E+00	U1/2		1.85E+00	7.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T02-C	1	1.85E+00	U1/2		1.85E+00	1.2E+02	3.7E+00	1.2E+01	10	100	9.84E+02	98%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T03-C	1	7.74E+00	E		7.74E+00	2.9E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T04-C	1	1.29E+01			1.29E+01	6.8E+00	3.7E+00	1.2E+01					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T05-C	1	1.27E+01			1.27E+01	2.1E+01	3.7E+00	1.2E+01					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T06-C	1	2.29E+01			2.29E+01	3.9E+00	3.7E+00	1.2E+01					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T07-C	1	3.27E+01			3.27E+01	8.0E+00	3.7E+00	1.2E+01					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T08-C	1	1.71E+02			1.71E+02	6.5E-01	3.7E+00	1.2E+01					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-T09-C	1	1.08E+03			1.08E+03	7.0E-01	3.7E+00	1.2E+01					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	2.2E+02	3.7E+00	1.2E+01					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	1.0E+02	3.7E+00	1.2E+01					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-B03-A	1	1.85E+00	U1/2		1.85E+00	1.6E+01	3.7E+00	1.2E+01					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-B01-B	1	1.85E+00	U1/2		1.85E+00	3.0E+02	3.7E+00	1.2E+01						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-B03-B	1	1.85E+00	U1/2		1.85E+00	1.6E+02	3.7E+00	1.2E+01						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-B01-C	1	1.85E+00	U1/2		1.85E+00	5.8E+01	3.7E+00	1.2E+01						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-B02-C	1	1.85E+00	U1/2		1.85E+00	4.7E+01	3.7E+00	1.2E+01						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1313-B03-C	1	1.85E+00	U1/2		1.85E+00	4.4E+01	3.7E+00	1.2E+01						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	SWA-L09-1313-T01-A	1	9.01E+01			9.01E+01	1.5E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T02-A	1	7.81E+01			7.81E+01	1.9E+00	2.0E+00	6.4E+00	1000	100	1.23E+03	116%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T03-A	1	1.13E+01			1.13E+01	5.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T04-A	1	2.16E+01			2.16E+01	9.6E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T05-A	1	3.35E+01			3.35E+01	3.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T06-A	1	3.17E+01			3.17E+01	1.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T07-A	1	5.47E+04			5.47E+04	5.9E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T08-A	1	7.97E+04			7.97E+04	1.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T09-A	1	1.59E+05			1.59E+05	9.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T01-B	1	1.04E+02			1.04E+02	4.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T02-B	1	8.24E+01			8.24E+01	1.0E+00	2.0E+00	6.4E+00	1000	100	1.14E+03	106%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T03-B	1	1.96E+01			1.96E+01	2.9E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T04-B	1	2.65E+01			2.65E+01	7.1E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T05-B	1	3.31E+01			3.31E+01	2.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T06-B	1	1.84E+04			1.84E+04	7.0E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T07-B	1	6.48E+04			6.48E+04	5.6E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T08-B	1	8.06E+04			8.06E+04	6.9E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T09-B	1	1.12E+05			1.12E+05	4.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T01-C	1	8.74E+01			8.74E+01	1.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T02-C	1	9.42E+01			9.42E+01	5.4E-01	2.0E+00	6.4E+00	1000	100	1.24E+03	114%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T03-C	1	1.16E+01			1.16E+01	1.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T04-C	1	2.28E+01			2.28E+01	5.3E+00	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T05-C	1	2.43E+01			2.43E+01	6.0E-01	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T06-C	1	1.70E+04			1.70E+04	3.9E-01	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T07-C	1	6.01E+04			6.01E+04	4.5E-01	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T08-C	1	9.30E+04			9.30E+04	3.0E-01	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-T09-C	1	1.07E+05			1.07E+05	2.3E+00	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.4E+03	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-B01-B	1	4.34E+00	E		4.34E+00	3.2E-01	2.0E+00	6.4E+00						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	8.9E+01	2.0E+00	6.4E+00						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-B01-C	1	3.85E+00	E		3.85E+00	6.5E+01	2.0E+00	6.4E+00						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-B02-C	1	2.83E+00	E		2.83E+00	5.6E+00	2.0E+00	6.4E+00						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1313-B03-C	1	5.71E+00	E		5.71E+00	6.3E+00	2.0E+00	6.4E+00						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	SWA-L09-1313-T01-A	1	5.60E+01			5.60E+01	7.8E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T02-A	1	1.61E+01	E		1.61E+01	1.9E+01	6.8E+00	2.2E+01	10	100	1.04E+03	102%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T03-A	1	3.40E+00	U1/2		3.40E+00	8.0E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T04-A	1	3.40E+00	U1/2		3.40E+00	3.2E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T05-A	1	3.40E+00	U1/2		3.40E+00	6.2E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T06-A	1	3.40E+00	U1/2		3.40E+00	1.4E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T07-A	1	3.40E+00	U1/2		3.40E+00	6.2E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T08-A	1	4.64E+01			4.64E+01	1.1E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T09-A	1	2.86E+03			2.86E+03	4.9E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T01-B	1	5.02E+01			5.02E+01	1.0E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T02-B	1	1.68E+01	E		1.68E+01	3.2E+01	6.8E+00	2.2E+01	10	100	1.01E+03	99%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T03-B	1	3.40E+00	U1/2		3.40E+00	8.4E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T04-B	1	3.40E+00	U1/2		3.40E+00	4.1E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T05-B	1	3.40E+00	U1/2		3.40E+00	7.5E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T06-B	1	3.40E+00	U1/2		3.40E+00	6.2E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T07-B	1	3.40E+00	U1/2		3.40E+00	4.1E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T08-B	1	3.24E+01			3.24E+01	1.3E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T09-B	1	2.68E+03			2.68E+03	2.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T01-C	1	5.20E+01			5.20E+01	7.7E+02	6.8E+00	2.2E+01			---		VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T02-C	1	1.52E+01	E		1.52E+01	1.8E+01	6.8E+00	2.2E+01	10	100	1.02E+03	101%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T03-C	1	3.40E+00	U1/2		3.40E+00	6.8E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T04-C	1	3.40E+00	U1/2		3.40E+00	5.0E+01	6.8E+00	2.2E+01					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T05-C	1	3.40E+00	U1/2		3.40E+00	1.4E+02	6.8E+00	2.2E+01					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T06-C	1	3.40E+00	U1/2		3.40E+00	7.8E+01	6.8E+00	2.2E+01					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T07-C	1	3.40E+00	U1/2		3.40E+00	9.2E+01	6.8E+00	2.2E+01					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T08-C	1	6.04E+02			6.04E+02	3.2E-01	6.8E+00	2.2E+01					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-T09-C	1	2.57E+03			2.57E+03	8.1E-01	6.8E+00	2.2E+01					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	7.4E+01	6.8E+00	2.2E+01					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	1.1E+02	6.8E+00	2.2E+01					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	1.0E+02	6.8E+00	2.2E+01					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-B01-B	1	3.40E+00	U1/2		3.40E+00	1.3E+02	6.8E+00	2.2E+01						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-B03-B	1	3.40E+00	U1/2		3.40E+00	2.5E+02	6.8E+00	2.2E+01						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-B01-C	1	3.40E+00	U1/2		3.40E+00	1.3E+02	6.8E+00	2.2E+01						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-B02-C	1	3.40E+00	U1/2		3.40E+00	2.2E+02	6.8E+00	2.2E+01						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1313-B03-C	1	3.40E+00	U1/2		3.40E+00	2.4E+02	6.8E+00	2.2E+01						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	SWA-L09-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	1.3E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	5.1E+01	1.9E+00	6.0E+00	10	100	8.57E+02	86%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T03-A	1	9.57E+01			9.57E+01	3.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T04-A	1	3.95E+02			3.95E+02	2.8E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T05-A	1	7.56E+02			7.56E+02	8.0E-01	1.9E+00	6.0E+00			---		VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T06-A	1	8.13E+02			8.13E+02	1.9E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T07-A	1	1.14E+03			1.14E+03	5.8E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T08-A	1	5.82E+02			5.82E+02	4.1E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T09-A	1	5.25E+02			5.25E+02	2.0E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	5.7E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	3.7E+01	1.9E+00	6.0E+00	10	100	8.41E+02	84%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T03-B	1	1.31E+02			1.31E+02	3.3E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T04-B	1	4.91E+02			4.91E+02	6.0E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T05-B	1	7.94E+02			7.94E+02	1.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T06-B	1	1.09E+03			1.09E+03	1.7E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T07-B	1	7.73E+02			7.73E+02	7.0E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T08-B	1	6.22E+02			6.22E+02	3.5E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T09-B	1	6.44E+02			6.44E+02	4.7E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	6.7E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	4.2E+01	1.9E+00	6.0E+00	10	100	8.53E+02	85%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T03-C	1	1.15E+02			1.15E+02	3.2E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T04-C	1	5.58E+02			5.58E+02	2.3E+00	1.9E+00	6.0E+00					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T05-C	1	7.87E+02			7.87E+02	8.5E-01	1.9E+00	6.0E+00					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T06-C	1	9.99E+02			9.99E+02	4.1E+00	1.9E+00	6.0E+00					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T07-C	1	1.01E+03			1.01E+03	2.7E+00	1.9E+00	6.0E+00					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T08-C	1	5.99E+02			5.99E+02	1.7E+00	1.9E+00	6.0E+00					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-T09-C	1	6.27E+02			6.27E+02	2.3E+00	1.9E+00	6.0E+00					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	4.5E+01	1.9E+00	6.0E+00					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	5.3E+01	1.9E+00	6.0E+00					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	1.5E+02	1.9E+00	6.0E+00					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-B01-B	1	9.50E-01	U1/2		9.50E-01	7.0E+02	1.9E+00	6.0E+00						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-B03-B	1	1.92E+00	E		1.92E+00	3.5E+01	1.9E+00	6.0E+00						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-B01-C	1	9.50E-01	U1/2		9.50E-01	1.9E+02	1.9E+00	6.0E+00						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-B02-C	1	9.50E-01	U1/2		9.50E-01	6.0E+01	1.9E+00	6.0E+00						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1313-B03-C	1	9.50E-01	U1/2		9.50E-01	6.0E+02	1.9E+00	6.0E+00						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	SWA-L09-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	3.9E+00	2.0E+00	6.4E+00	10	100	1.00E+03	100%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	2.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T04-A	1	2.85E+01			2.85E+01	5.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T05-A	1	2.60E+03			2.60E+03	7.3E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T06-A	1	6.23E+03			6.23E+03	5.1E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T07-A	1	1.62E+04			1.62E+04	7.1E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T08-A	1	1.18E+04			1.18E+04	1.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T09-A	1	1.21E+04			1.21E+04	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	5.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	6.1E+00	2.0E+00	6.4E+00	10	100	9.63E+02	96%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	5.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T04-B	1	3.05E+01			3.05E+01	5.1E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T05-B	1	3.27E+03			3.27E+03	4.1E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T06-B	1	1.67E+04			1.67E+04	5.6E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T07-B	1	1.55E+04			1.55E+04	7.1E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T08-B	1	1.33E+04			1.33E+04	5.8E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T09-B	1	1.28E+04			1.28E+04	1.5E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00	10	100	9.93E+02	99%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T04-C	1	5.74E+01			5.74E+01	5.6E-01	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T05-C	1	5.42E+02			5.42E+02	8.2E-01	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T06-C	1	1.74E+04			1.74E+04	3.7E-01	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T07-C	1	1.79E+04			1.79E+04	4.1E-01	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T08-C	1	1.25E+04			1.25E+04	8.0E-01	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-T09-C	1	1.28E+04			1.28E+04	1.0E+00	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	7.5E+02	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	6.8E+01	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	5.5E+01	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	6.6E+00	2.0E+00	6.4E+00						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	8.6E+01	2.0E+00	6.4E+00						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	9.8E+01	2.0E+00	6.4E+00						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1313-B03-C	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	SWA-L09-1313-T01-A	1	1.26E+01			1.26E+01	6.4E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T02-A	1	1.16E+01			1.16E+01	1.2E+01	1.0E+00	3.2E+00	1000	100	1.09E+03	108%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T03-A	1	9.79E+02			9.79E+02	8.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T04-A	1	3.42E+05			3.42E+05	5.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T05-A	1	9.15E+05			9.15E+05	4.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T06-A	1	9.88E+05			9.88E+05	4.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T07-A	1	1.42E+06			1.42E+06	9.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T08-A	1	6.60E+05			6.60E+05	2.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T09-A	1	5.53E+05			5.53E+05	7.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T01-B	1	1.85E+01			1.85E+01	2.0E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T02-B	1	2.01E+01			2.01E+01	3.6E+01	1.0E+00	3.2E+00	1000	100	1.03E+03	101%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T03-B	1	2.11E+03			2.11E+03	9.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T04-B	1	5.18E+05			5.18E+05	5.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T05-B	1	9.37E+05			9.37E+05	1.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T06-B	1	1.38E+06			1.38E+06	7.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T07-B	1	9.48E+05			9.48E+05	6.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T08-B	1	7.80E+05			7.80E+05	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T09-B	1	6.15E+05			6.15E+05	3.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T01-C	1	1.37E+01			1.37E+01	4.6E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T02-C	1	1.34E+01			1.34E+01	4.9E+01	1.0E+00	3.2E+00	1000	100	1.10E+03	109%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T03-C	1	4.24E+03			4.24E+03	1.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T04-C	1	5.82E+05			5.82E+05	1.0E+00	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T05-C	1	8.50E+05			8.50E+05	4.3E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T06-C	1	1.28E+06			1.28E+06	9.0E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T07-C	1	1.31E+06			1.31E+06	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T08-C	1	6.72E+05			6.72E+05	7.8E-02	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-T09-C	1	6.12E+05			6.12E+05	6.2E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	6.1E+03	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	5.6E+01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	1.4E+02	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-B01-B	1	1.37E+00	E		1.37E+00	7.1E+01	1.0E+00	3.2E+00						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	3.2E+01	1.0E+00	3.2E+00						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-B01-C	1	1.95E+00	E		1.95E+00	2.0E+02	1.0E+00	3.2E+00						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	7.2E+01	1.0E+00	3.2E+00						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1313-B03-C	1	1.43E+00	E		1.43E+00	5.8E+02	1.0E+00	3.2E+00						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	SWA-L09-1313-T01-A	1	1.11E+02			1.11E+02	1.6E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T02-A	1	1.28E+02			1.28E+02	9.5E-01	1.2E+00	3.8E+00	10	100	1.18E+03	105%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T03-A	1	1.27E+02			1.27E+02	1.4E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T04-A	1	1.23E+02			1.23E+02	6.7E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T05-A	1	1.13E+02			1.13E+02	1.0E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T06-A	1	9.29E+01			9.29E+01	1.5E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T07-A	1	2.70E+01			2.70E+01	8.9E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T08-A	1	1.57E+01			1.57E+01	5.8E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T09-A	1	4.18E+01			4.18E+01	1.4E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T01-B	1	1.06E+02			1.06E+02	1.0E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T02-B	1	1.22E+02			1.22E+02	2.0E+00	1.2E+00	3.8E+00	10	100	1.15E+03	102%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T03-B	1	1.36E+02			1.36E+02	1.6E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T04-B	1	1.27E+02			1.27E+02	1.5E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T05-B	1	1.08E+02			1.08E+02	2.4E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T06-B	1	2.44E+01			2.44E+01	2.7E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T07-B	1	1.19E+01			1.19E+01	4.0E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T08-B	1	1.30E+01			1.30E+01	3.9E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T09-B	1	3.42E+00	E		3.42E+00	5.2E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T01-C	1	1.25E+02			1.25E+02	7.5E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T02-C	1	1.35E+02			1.35E+02	4.5E-01	1.2E+00	3.8E+00	10	100	1.17E+03	104%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T03-C	1	1.12E+02			1.12E+02	2.0E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T04-C	1	1.21E+02			1.21E+02	9.2E-01	1.2E+00	3.8E+00					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T05-C	1	1.23E+02			1.23E+02	4.7E-01	1.2E+00	3.8E+00					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T06-C	1	1.38E+01			1.38E+01	5.1E+00	1.2E+00	3.8E+00					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T07-C	1	1.10E+01			1.10E+01	9.1E+00	1.2E+00	3.8E+00					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T08-C	1	6.32E+00			6.32E+00	6.2E+00	1.2E+00	3.8E+00					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-T09-C	1	5.04E+00			5.04E+00	8.8E+00	1.2E+00	3.8E+00					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-B01-A	1	1.64E+00	E		1.64E+00	6.5E+01	1.2E+00	3.8E+00					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-B02-A	1	1.24E+00	E		1.24E+00	9.5E+01	1.2E+00	3.8E+00					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-B03-A	1	6.00E-01	U1/2		6.00E-01	6.1E+02	1.2E+00	3.8E+00					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-B01-B	1	6.00E-01	U1/2		6.00E-01	1.4E+02	1.2E+00	3.8E+00						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-B03-B	1	6.00E-01	U1/2		6.00E-01	3.4E+03	1.2E+00	3.8E+00						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-B01-C	1	2.67E+00	E		2.67E+00	5.0E+01	1.2E+00	3.8E+00						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-B02-C	1	1.74E+00	E		1.74E+00	4.8E+01	1.2E+00	3.8E+00						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1313-B03-C	1	3.13E+00	E		3.13E+00	4.5E+01	1.2E+00	3.8E+00						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	SWA-L09-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	9.3E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00	10	100	9.34E+02	93%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T03-A	1	3.56E+00	E		3.56E+00	4.3E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T04-A	1	6.74E+00			6.74E+00	4.1E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T05-A	1	2.20E+01			2.20E+01	5.1E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T06-A	1	5.97E+01			5.97E+01	1.4E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T07-A	1	2.38E+02			2.38E+02	1.6E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T08-A	1	2.21E+02			2.21E+02	2.4E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T09-A	1	2.65E+02			2.65E+02	3.7E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	2.5E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	3.8E+01	1.8E+00	5.7E+00	10	100	9.07E+02	91%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T03-B	1	3.45E+00	E		3.45E+00	5.7E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T04-B	1	9.12E+00			9.12E+00	2.4E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T05-B	1	2.34E+01			2.34E+01	8.9E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T06-B	1	2.89E+02			2.89E+02	1.1E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T07-B	1	2.99E+02			2.99E+02	1.1E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T08-B	1	2.59E+02			2.59E+02	1.1E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T09-B	1	2.73E+02			2.73E+02	4.9E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	1.0E+02	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	3.8E+01	1.8E+00	5.7E+00	10	100	9.25E+02	92%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T03-C	1	3.16E+00	E		3.16E+00	3.3E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T04-C	1	9.85E+00			9.85E+00	6.4E+00	1.8E+00	5.7E+00					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T05-C	1	1.68E+01			1.68E+01	3.4E+00	1.8E+00	5.7E+00					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T06-C	1	3.17E+02			3.17E+02	2.6E-01	1.8E+00	5.7E+00					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T07-C	1	3.28E+02			3.28E+02	3.2E-01	1.8E+00	5.7E+00					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T08-C	1	2.60E+02			2.60E+02	4.2E-01	1.8E+00	5.7E+00					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-T09-C	1	2.72E+02			2.72E+02	3.7E-01	1.8E+00	5.7E+00					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	7.9E+00	1.8E+00	5.7E+00					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	6.2E+01	1.8E+00	5.7E+00					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-B01-B	1	9.00E-01	U1/2		9.00E-01	6.5E+01	1.8E+00	5.7E+00						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-B03-B	1	9.00E-01	U1/2		9.00E-01	6.2E+01	1.8E+00	5.7E+00						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-B01-C	1	9.00E-01	U1/2		9.00E-01	1.4E+03	1.8E+00	5.7E+00						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-B02-C	1	9.00E-01	U1/2		9.00E-01	2.1E+01	1.8E+00	5.7E+00						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1313-B03-C	1	9.00E-01	U1/2		9.00E-01	6.9E+01	1.8E+00	5.7E+00						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	SWA-L09-1313-T01-A	1	9.09E+01			9.09E+01	2.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T02-A	1	3.49E+01			3.49E+01	9.2E+00	3.7E+00	1.2E+01	1000	100	8.65E+02	83%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T03-A	1	1.83E+01			1.83E+01	6.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T04-A	1	3.51E+01			3.51E+01	7.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T05-A	1	4.33E+01			4.33E+01	1.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T06-A	1	3.63E+01			3.63E+01	4.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T07-A	1	2.32E+01			2.32E+01	7.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T08-A	1	4.58E+02			4.58E+02	1.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T09-A	1	2.52E+04			2.52E+04	2.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T01-B	1	1.09E+02			1.09E+02	3.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T02-B	1	4.35E+01			4.35E+01	2.0E+01	3.7E+00	1.2E+01	1000	100	9.04E+02	86%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T03-B	1	1.45E+01			1.45E+01	7.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T04-B	1	3.69E+01			3.69E+01	5.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T05-B	1	3.70E+01			3.70E+01	3.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T06-B	1	2.98E+01			2.98E+01	1.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T07-B	1	2.39E+01			2.39E+01	4.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T08-B	1	4.34E+02			4.34E+02	5.7E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T09-B	1	8.67E+02			8.67E+02	1.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T01-C	1	8.57E+01			8.57E+01	4.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T02-C	1	3.94E+01			3.94E+01	3.2E+01	3.7E+00	1.2E+01	1000	100	8.93E+02	85%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T03-C	1	1.67E+01			1.67E+01	4.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T04-C	1	4.47E+01			4.47E+01	2.3E+01	3.7E+00	1.2E+01					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T05-C	1	5.87E+01			5.87E+01	1.1E+01	3.7E+00	1.2E+01					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T06-C	1	2.81E+01			2.81E+01	8.8E+01	3.7E+00	1.2E+01					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T07-C	1	3.31E+01			3.31E+01	5.9E+01	3.7E+00	1.2E+01					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T08-C	1	5.14E+02			5.14E+02	3.2E+00	3.7E+00	1.2E+01					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-T09-C	1	8.52E+02			8.52E+02	4.5E-01	3.7E+00	1.2E+01					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	3.5E+03	3.7E+00	1.2E+01					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	9.1E+01	3.7E+00	1.2E+01					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-B03-A	1	6.46E+00	E		6.46E+00	5.2E+01	3.7E+00	1.2E+01					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-B01-B	1	6.95E+00	E		6.95E+00	3.0E+01	3.7E+00	1.2E+01						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-B03-B	1	1.85E+00	U1/2		1.85E+00	9.8E+01	3.7E+00	1.2E+01						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-B01-C	1	6.09E+00	E		6.09E+00	3.2E+01	3.7E+00	1.2E+01						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-B02-C	1	9.49E+00	E		9.49E+00	7.3E+01	3.7E+00	1.2E+01						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1313-B03-C	1	8.09E+00	E		8.09E+00	4.8E+01	3.7E+00	1.2E+01						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	SWA-L09-1313-T01-A	1	2.07E+06			2.07E+06	8.4E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T02-A	1	2.64E+05			2.64E+05	1.0E+00	1.6E+00	5.1E+00	1000	100	2.65E+05	101%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T03-A	1	3.39E+05			3.39E+05	4.9E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T04-A	1	3.71E+05			3.71E+05	6.2E+00	1.6E+00	5.1E+00			---		VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T05-A	1	3.81E+05			3.81E+05	1.3E+00	1.6E+00	5.1E+00			---		VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T06-A	1	3.91E+05			3.91E+05	3.1E+00	1.6E+00	5.1E+00			---		VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T07-A	1	4.27E+05			4.27E+05	9.9E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T08-A	1	1.94E+05			1.94E+05	2.9E+00	1.6E+00	5.1E+00			---		VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T09-A	1	2.13E+05			2.13E+05	4.4E+01	1.6E+00	5.1E+00			---		VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T01-B	1	2.07E+06			2.07E+06	9.8E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T02-B	1	2.56E+05			2.56E+05	1.2E+00	1.6E+00	5.1E+00	1000	100	2.57E+05	89%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T03-B	1	3.69E+05			3.69E+05	2.2E+00	1.6E+00	5.1E+00			---		VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T04-B	1	3.60E+05			3.60E+05	2.5E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T05-B	1	3.90E+05			3.90E+05	2.8E+00	1.6E+00	5.1E+00			---		VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T06-B	1	4.08E+05			4.08E+05	1.5E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T07-B	1	3.00E+05			3.00E+05	1.3E+01	1.6E+00	5.1E+00			---		VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T08-B	1	2.14E+05			2.14E+05	1.8E+00	1.6E+00	5.1E+00			---		VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T09-B	1	2.33E+05			2.33E+05	1.4E+01	1.6E+00	5.1E+00			---		VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T01-C	1	2.11E+06			2.11E+06	2.0E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T02-C	1	2.73E+05			2.73E+05	6.3E-01	1.6E+00	5.1E+00	1000	100	2.74E+05	104%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T03-C	1	3.43E+05			3.43E+05	3.8E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T04-C	1	3.72E+05			3.72E+05	6.3E-01	1.6E+00	5.1E+00					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T05-C	1	3.85E+05			3.85E+05	3.9E-01	1.6E+00	5.1E+00					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T06-C	1	3.91E+05			3.91E+05	3.8E-01	1.6E+00	5.1E+00					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T07-C	1	4.00E+05			4.00E+05	4.6E+00	1.6E+00	5.1E+00					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T08-C	1	1.86E+05			1.86E+05	7.7E+00	1.6E+00	5.1E+00					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-T09-C	1	2.22E+05			2.22E+05	3.5E+00	1.6E+00	5.1E+00					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-B01-A	1	1.97E+01			1.97E+01	3.2E+01	1.6E+00	5.1E+00					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-B02-A	1	2.45E+01			2.45E+01	1.4E+01	1.6E+00	5.1E+00					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-B03-A	1	2.51E+01			2.51E+01	6.1E+00	1.6E+00	5.1E+00					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-B01-B	1	1.81E+01			1.81E+01	1.1E+00	1.6E+00	5.1E+00						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-B03-B	1	3.38E+01			3.38E+01	5.6E+01	1.6E+00	5.1E+00						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-B01-C	1	2.01E+06			2.01E+06	1.8E+00	1.6E+00	5.1E+00						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-B02-C	1	1.98E+06			1.98E+06	2.0E-01	1.6E+00	5.1E+00						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1313-B03-C	1	2.06E+06			2.06E+06	1.1E+00	1.6E+00	5.1E+00						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	SWA-L09-1313-T01-A	1	6.77E+04			6.77E+04	6.9E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T02-A	1	7.55E+04			7.55E+04	1.1E+00	1.5E+01	4.8E+01	10	100	7.66E+04	105%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T03-A	1	7.96E+04			7.96E+04	1.1E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T04-A	1	8.72E+04			8.72E+04	5.8E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T05-A	1	9.36E+04			9.36E+04	5.2E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T06-A	1	9.55E+04			9.55E+04	2.8E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T07-A	1	1.04E+05			1.04E+05	4.4E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T08-A	1	4.26E+04			4.26E+04	1.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T09-A	1	2.36E+04			2.36E+04	7.8E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T01-B	1	6.45E+04			6.45E+04	5.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T02-B	1	7.21E+04			7.21E+04	6.5E-01	1.5E+01	4.8E+01	10	100	7.32E+04	109%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T03-B	1	8.56E+04			8.56E+04	1.8E-02	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T04-B	1	8.85E+04			8.85E+04	4.1E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T05-B	1	9.33E+04			9.33E+04	5.8E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T06-B	1	9.87E+04			9.87E+04	5.4E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T07-B	1	9.72E+04			9.72E+04	5.9E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T08-B	1	4.50E+04			4.50E+04	1.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T09-B	1	2.67E+04			2.67E+04	4.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T01-C	1	7.82E+04			7.82E+04	6.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T02-C	1	8.24E+04			8.24E+04	2.6E-01	1.5E+01	4.8E+01	10	100	8.35E+04	115%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T03-C	1	7.57E+04			7.57E+04	5.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T04-C	1	9.19E+04			9.19E+04	2.6E-01	1.5E+01	4.8E+01					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T05-C	1	1.01E+05			1.01E+05	9.4E-02	1.5E+01	4.8E+01					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T06-C	1	9.00E+04			9.00E+04	2.4E-01	1.5E+01	4.8E+01					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T07-C	1	9.23E+04			9.23E+04	1.3E-01	1.5E+01	4.8E+01					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T08-C	1	3.34E+04			3.34E+04	5.7E-01	1.5E+01	4.8E+01					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-T09-C	1	2.66E+04			2.66E+04	3.3E-01	1.5E+01	4.8E+01					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-B01-A	1	7.50E+00	U1/2		7.50E+00	4.9E+01	1.5E+01	4.8E+01					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-B02-A	1	7.50E+00	U1/2		7.50E+00	1.5E+02	1.5E+01	4.8E+01					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-B03-A	1	7.50E+00	U1/2		7.50E+00	4.6E+02	1.5E+01	4.8E+01					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-B01-B	1	7.50E+00	U1/2		7.50E+00	8.3E+01	1.5E+01	4.8E+01						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-B03-B	1	7.50E+00	U1/2		7.50E+00	2.1E+02	1.5E+01	4.8E+01						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-B01-C	1	2.01E+01	E		2.01E+01	3.5E+01	1.5E+01	4.8E+01						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-B02-C	1	7.50E+00	U1/2		7.50E+00	1.8E+02	1.5E+01	4.8E+01						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1313-B03-C	1	1.91E+01	E		1.91E+01	3.9E+01	1.5E+01	4.8E+01						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	SWA-L09-1313-T01-A	1	3.47E+04			3.47E+04	7.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T02-A	1	2.48E+04			2.48E+04	9.7E-01	1.1E+00	3.5E+00	1000	100	2.57E+04	85%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T03-A	1	6.19E+03			6.19E+03	3.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T04-A	1	4.22E+03			4.22E+03	6.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T05-A	1	3.76E+03			3.76E+03	6.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T06-A	1	4.82E+03			4.82E+03	3.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T07-A	1	8.27E+03			8.27E+03	4.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T08-A	1	1.17E+04			1.17E+04	9.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T09-A	1	7.82E+05			7.82E+05	7.6E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T01-B	1	3.96E+04			3.96E+04	6.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T02-B	1	2.32E+04			2.32E+04	8.8E-01	1.1E+00	3.5E+00	1000	100	2.40E+04	82%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T03-B	1	6.31E+03			6.31E+03	2.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T04-B	1	3.53E+03			3.53E+03	3.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T05-B	1	3.97E+03			3.97E+03	7.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T06-B	1	9.18E+03			9.18E+03	5.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T07-B	1	1.59E+04			1.59E+04	6.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T08-B	1	1.84E+04			1.84E+04	1.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T09-B	1	2.27E+04			2.27E+04	5.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T01-C	1	3.50E+04			3.50E+04	4.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T02-C	1	2.61E+04			2.61E+04	2.6E-01	1.1E+00	3.5E+00	1000	100	2.70E+04	91%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T03-C	1	6.48E+03			6.48E+03	5.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T04-C	1	4.98E+03			4.98E+03	5.1E-01	1.1E+00	3.5E+00					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T05-C	1	4.91E+03			4.91E+03	2.8E-01	1.1E+00	3.5E+00					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T06-C	1	8.75E+03			8.75E+03	4.9E-01	1.1E+00	3.5E+00					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T07-C	1	1.13E+04			1.13E+04	7.5E-01	1.1E+00	3.5E+00					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T08-C	1	1.48E+04			1.48E+04	1.6E-01	1.1E+00	3.5E+00					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-T09-C	1	1.85E+04			1.85E+04	7.1E-01	1.1E+00	3.5E+00					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-B01-A	1	5.50E-01	U1/2		5.50E-01	6.1E+01	1.1E+00	3.5E+00					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-B02-A	1	5.50E-01	U1/2		5.50E-01	2.0E+01	1.1E+00	3.5E+00					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-B03-A	1	2.45E+00	E		2.45E+00	1.0E+02	1.1E+00	3.5E+00					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-B01-B	1	5.20E+00			5.20E+00	3.1E+00	1.1E+00	3.5E+00						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-B03-B	1	5.50E-01	U1/2		5.50E-01	5.9E+01	1.1E+00	3.5E+00						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-B01-C	1	1.26E+03			1.26E+03	7.9E+00	1.1E+00	3.5E+00						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-B02-C	1	2.92E+01			2.92E+01	1.4E+01	1.1E+00	3.5E+00						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1313-B03-C	1	1.76E+02			1.76E+02	1.3E+00	1.1E+00	3.5E+00						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	SWA-L09-1313-T01-A	1	4.73E+05			4.73E+05	5.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T02-A	1	4.80E+05			4.80E+05	3.7E-01	2.5E+00	8.0E+00	1000	100	4.81E+05	85%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T03-A	1	5.10E+05			5.10E+05	1.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T04-A	1	5.00E+05			5.00E+05	7.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T05-A	1	4.88E+05			4.88E+05	3.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T06-A	1	4.89E+05			4.89E+05	4.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T07-A	1	4.82E+05			4.82E+05	2.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T08-A	1	4.83E+05			4.83E+05	7.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T09-A	1	4.36E+05			4.36E+05	6.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T01-B	1	4.63E+05			4.63E+05	1.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T02-B	1	4.69E+05			4.69E+05	6.0E-01	2.5E+00	8.0E+00	1000	100	4.70E+05	88%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T03-B	1	5.15E+05			5.15E+05	7.4E-02	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T04-B	1	4.83E+05			4.83E+05	4.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T05-B	1	4.84E+05			4.84E+05	4.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T06-B	1	4.82E+05			4.82E+05	5.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T07-B	1	4.73E+05			4.73E+05	7.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T08-B	1	4.77E+05			4.77E+05	4.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T09-B	1	4.81E+05			4.81E+05	3.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T01-C	1	4.65E+05			4.65E+05	3.7E-02	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T02-C	1	4.78E+05			4.78E+05	4.2E-01	2.5E+00	8.0E+00	1000	100	4.79E+05	87%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T03-C	1	5.01E+05			5.01E+05	7.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T04-C	1	4.93E+05			4.93E+05	2.4E-01	2.5E+00	8.0E+00					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T05-C	1	4.93E+05			4.93E+05	6.8E-01	2.5E+00	8.0E+00					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T06-C	1	4.79E+05			4.79E+05	3.8E-01	2.5E+00	8.0E+00					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T07-C	1	4.78E+05			4.78E+05	5.2E-01	2.5E+00	8.0E+00					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T08-C	1	4.78E+05			4.78E+05	1.5E-01	2.5E+00	8.0E+00					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-T09-C	1	4.83E+05			4.83E+05	1.7E-01	2.5E+00	8.0E+00					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-B01-A	1	7.34E+01			7.34E+01	4.5E+01	2.5E+00	8.0E+00					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-B02-A	1	8.09E+01			8.09E+01	2.6E+00	2.5E+00	8.0E+00					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-B03-A	1	1.28E+01			1.28E+01	8.5E+00	2.5E+00	8.0E+00					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-B01-B	1	7.09E+01			7.09E+01	2.1E+00	2.5E+00	8.0E+00						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-B03-B	1	5.71E+01			5.71E+01	4.5E+01	2.5E+00	8.0E+00						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-B01-C	1	1.42E+03			1.42E+03	8.8E-01	2.5E+00	8.0E+00						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-B02-C	1	6.11E+02			6.11E+02	3.2E-01	2.5E+00	8.0E+00						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1313-B03-C	1	1.34E+03			1.34E+03	1.2E+00	2.5E+00	8.0E+00						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	SWA-L09-1313-T01-A	1	2.99E+02			2.99E+02	9.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T02-A	1	3.06E+02			3.06E+02	7.4E-01	1.0E+00	3.2E+00	1000	100	1.34E+03	104%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T03-A	1	1.19E+04			1.19E+04	5.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T04-A	1	2.29E+04			2.29E+04	1.1E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T05-A	1	3.19E+04			3.19E+04	1.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T06-A	1	3.50E+04			3.50E+04	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T07-A	1	4.53E+04			4.53E+04	9.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T08-A	1	2.16E+04			2.16E+04	1.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T09-A	1	1.70E+04			1.70E+04	1.1E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T01-B	1	2.80E+02			2.80E+02	3.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T02-B	1	3.04E+02			3.04E+02	5.5E-01	1.0E+00	3.2E+00	1000	100	1.30E+03	99%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T03-B	1	1.45E+04			1.45E+04	7.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T04-B	1	2.60E+04			2.60E+04	4.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T05-B	1	3.28E+04			3.28E+04	7.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T06-B	1	4.35E+04			4.35E+04	2.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T07-B	1	3.00E+04			3.00E+04	8.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T08-B	1	2.41E+04			2.41E+04	8.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T09-B	1	1.85E+04			1.85E+04	9.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T01-C	1	2.64E+02			2.64E+02	9.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T02-C	1	3.05E+02			3.05E+02	3.9E-01	1.0E+00	3.2E+00	1000	100	1.34E+03	103%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T03-C	1	1.36E+04			1.36E+04	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T04-C	1	2.68E+04			2.68E+04	9.2E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T05-C	1	3.25E+04			3.25E+04	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T06-C	1	4.25E+04			4.25E+04	1.7E+00	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T07-C	1	4.26E+04			4.26E+04	1.7E+00	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T08-C	1	2.00E+04			2.00E+04	4.5E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-T09-C	1	1.83E+04			1.83E+04	7.3E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	6.2E+03	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	6.1E+01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	2.2E+01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-B01-B	1	2.75E+00	E		2.75E+00	2.5E+01	1.0E+00	3.2E+00						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	1.9E+02	1.0E+00	3.2E+00						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-B01-C	1	1.86E+00	E		1.86E+00	7.9E+01	1.0E+00	3.2E+00						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-B02-C	1	1.22E+00	E		1.22E+00	2.9E+01	1.0E+00	3.2E+00						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	6.0E+01	1.0E+00	3.2E+00						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	SWA-L09-1313-T01-A	1	2.80E+05			2.80E+05	1.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T02-A	1	3.87E+05			3.87E+05	6.5E-01	6.8E+00	2.2E+01	1000	100	3.88E+05	84%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T03-A	1	2.99E+05			2.99E+05	2.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T04-A	1	3.06E+05			3.06E+05	4.8E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T05-A	1	3.53E+05			3.53E+05	2.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T06-A	1	3.10E+05			3.10E+05	6.6E-02	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T07-A	1	3.69E+05			3.69E+05	6.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T08-A	1	1.45E+05			1.45E+05	1.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T09-A	1	8.18E+04			8.18E+04	5.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T01-B	1	2.69E+05			2.69E+05	2.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T02-B	1	3.39E+05			3.39E+05	3.9E-01	6.8E+00	2.2E+01	1000	100	3.40E+05	82%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T03-B	1	3.12E+05			3.12E+05	2.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T04-B	1	2.68E+05			2.68E+05	4.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T05-B	1	3.08E+05			3.08E+05	4.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T06-B	1	3.18E+05			3.18E+05	8.4E-02	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T07-B	1	2.98E+05			2.98E+05	5.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T08-B	1	1.57E+05			1.57E+05	8.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T09-B	1	9.65E+04			9.65E+04	5.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T01-C	1	3.16E+05			3.16E+05	7.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T02-C	1	3.63E+05			3.63E+05	3.2E-01	6.8E+00	2.2E+01	1000	100	3.64E+05	90%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T03-C	1	3.18E+05			3.18E+05	5.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T04-C	1	3.60E+05			3.60E+05	1.4E-01	6.8E+00	2.2E+01					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T05-C	1	3.40E+05			3.40E+05	2.1E-01	6.8E+00	2.2E+01					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T06-C	1	3.32E+05			3.32E+05	9.3E-02	6.8E+00	2.2E+01					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T07-C	1	3.11E+05			3.11E+05	4.2E-01	6.8E+00	2.2E+01					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T08-C	1	1.20E+05			1.20E+05	6.1E-01	6.8E+00	2.2E+01					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-T09-C	1	1.01E+05			1.01E+05	5.4E-01	6.8E+00	2.2E+01					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-B01-A	1	2.11E+01	E		2.11E+01	7.1E+00	6.8E+00	2.2E+01					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-B02-A	1	3.48E+01			3.48E+01	7.0E+00	6.8E+00	2.2E+01					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	2.7E+00	6.8E+00	2.2E+01					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-B01-B	1	2.24E+01			2.24E+01	7.0E+00	6.8E+00	2.2E+01						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-B03-B	1	2.24E+01			2.24E+01	1.1E+01	6.8E+00	2.2E+01						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-B01-C	1	5.30E+01			5.30E+01	4.2E+01	6.8E+00	2.2E+01						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-B02-C	1	7.32E+01			7.32E+01	7.1E+00	6.8E+00	2.2E+01						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1313-B03-C	1	4.46E+01			4.46E+01	4.6E+00	6.8E+00	2.2E+01						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	SWA-L09-1313-T01-A	1	2.30E+00	U1/2		2.30E+00	3.7E+03	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T02-A	1	2.30E+00	U1/2		2.30E+00	6.2E+01	4.6E+00	1.5E+01	10	100	8.86E+02	88%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T03-A	1	2.30E+00	U1/2		2.30E+00	9.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T04-A	1	2.30E+00	U1/2		2.30E+00	3.9E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T05-A	1	2.30E+00	U1/2		2.30E+00	9.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T06-A	1	2.30E+00	U1/2		2.30E+00	1.2E+02	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T07-A	1	1.13E+01	E		1.13E+01	3.4E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T08-A	1	9.81E+00	E		9.81E+00	3.4E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T09-A	1	1.26E+01	E		1.26E+01	5.4E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T01-B	1	2.30E+00	U1/2		2.30E+00	5.9E+03	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T02-B	1	2.30E+00	U1/2		2.30E+00	8.7E+01	4.6E+00	1.5E+01	10	100	8.59E+02	86%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T03-B	1	2.30E+00	U1/2		2.30E+00	5.8E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T04-B	1	2.30E+00	U1/2		2.30E+00	1.4E+02	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T05-B	1	2.30E+00	U1/2		2.30E+00	2.0E+02	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T06-B	1	1.72E+01			1.72E+01	1.9E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T07-B	1	1.75E+01			1.75E+01	8.1E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T08-B	1	1.14E+01	E		1.14E+01	2.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T09-B	1	1.38E+01	E		1.38E+01	5.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T01-C	1	2.30E+00	U1/2		2.30E+00	1.1E+02	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T02-C	1	2.30E+00	U1/2		2.30E+00	6.2E+02	4.6E+00	1.5E+01	10	100	8.81E+02	88%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T03-C	1	2.30E+00	U1/2		2.30E+00	2.7E+02	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T04-C	1	2.30E+00	U1/2		2.30E+00	4.1E+02	4.6E+00	1.5E+01					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T05-C	1	2.30E+00	U1/2		2.30E+00	3.1E+01	4.6E+00	1.5E+01					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T06-C	1	1.58E+01			1.58E+01	2.8E+01	4.6E+00	1.5E+01					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T07-C	1	2.17E+01			2.17E+01	4.1E+01	4.6E+00	1.5E+01					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T08-C	1	1.04E+01	E		1.04E+01	1.6E+02	4.6E+00	1.5E+01					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-T09-C	1	1.28E+01	E		1.28E+01	1.2E+01	4.6E+00	1.5E+01					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	8.7E+01	4.6E+00	1.5E+01					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	6.5E+01	4.6E+00	1.5E+01					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	5.0E+01	4.6E+00	1.5E+01					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-B01-B	1	2.30E+00	U1/2		2.30E+00	4.4E+01	4.6E+00	1.5E+01						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-B03-B	1	2.30E+00	U1/2		2.30E+00	1.6E+01	4.6E+00	1.5E+01						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-B01-C	1	2.30E+00	U1/2		2.30E+00	1.2E+02	4.6E+00	1.5E+01						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-B02-C	1	2.30E+00	U1/2		2.30E+00	1.4E+04	4.6E+00	1.5E+01						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1313-B03-C	1	2.30E+00	U1/2		2.30E+00	5.7E+01	4.6E+00	1.5E+01						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	SWA-L09-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00	10	100	1.06E+03	106%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	1.6E+03	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	6.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	9.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	3.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T08-A	1	6.77E+01			6.77E+01	1.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T09-A	1	4.25E+04			4.25E+04	4.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	9.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	7.0E+00	2.0E+00	6.4E+00	10	100	1.06E+03	106%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	6.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	2.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	3.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T08-B	1	5.87E+01			5.87E+01	1.8E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T09-B	1	1.87E+02			1.87E+02	4.1E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	2.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00	10	100	1.06E+03	106%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	6.6E+01	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	6.5E+01	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	5.4E+01	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T08-C	1	8.59E+01			8.59E+01	3.9E+00	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-T09-C	1	1.46E+02			1.46E+02	6.1E-01	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	2.2E+02	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	8.3E+01	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	4.2E-01	2.0E+00	6.4E+00						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	6.5E+01	2.0E+00	6.4E+00						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	1.3E+01	2.0E+00	6.4E+00						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	5.2E+01	2.0E+00	6.4E+00						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1313-B03-C	1	1.00E+00	U1/2		1.00E+00	3.7E+01	2.0E+00	6.4E+00						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	SWA-L09-1313-T01-A	1	3.79E+02			3.79E+02	1.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T02-A	1	3.10E+02			3.10E+02	1.6E+00	1.5E+00	4.8E+00	10	100	1.31E+03	100%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T03-A	1	1.05E+02			1.05E+02	1.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T04-A	1	1.66E+02			1.66E+02	1.1E+01	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T05-A	1	1.87E+02			1.87E+02	1.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T06-A	1	1.80E+02			1.80E+02	1.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T07-A	1	2.04E+02			2.04E+02	1.9E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T08-A	1	9.70E+01			9.70E+01	1.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T09-A	1	1.35E+03			1.35E+03	2.6E+01	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T01-B	1	3.68E+02			3.68E+02	7.6E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T02-B	1	3.09E+02			3.09E+02	9.3E-01	1.5E+00	4.8E+00	10	100	1.28E+03	97%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T03-B	1	1.19E+02			1.19E+02	6.9E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T04-B	1	2.06E+02			2.06E+02	1.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T05-B	1	1.89E+02			1.89E+02	9.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T06-B	1	1.91E+02			1.91E+02	6.0E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T07-B	1	1.60E+02			1.60E+02	7.2E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T08-B	1	8.83E+01			8.83E+01	3.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T09-B	1	1.41E+03			1.41E+03	3.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T01-C	1	3.82E+02			3.82E+02	5.6E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T02-C	1	3.72E+02			3.72E+02	1.1E+00	1.5E+00	4.8E+00	10	100	1.34E+03	97%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T03-C	1	1.21E+02			1.21E+02	1.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T04-C	1	2.14E+02			2.14E+02	1.0E+00	1.5E+00	4.8E+00					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T05-C	1	2.17E+02			2.17E+02	5.7E-01	1.5E+00	4.8E+00					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T06-C	1	1.75E+02			1.75E+02	1.0E+00	1.5E+00	4.8E+00					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T07-C	1	1.75E+02			1.75E+02	2.4E+00	1.5E+00	4.8E+00					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T08-C	1	7.40E+01			7.40E+01	3.3E-01	1.5E+00	4.8E+00					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-T09-C	1	1.30E+03			1.30E+03	8.0E-01	1.5E+00	4.8E+00					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-B01-A	1	7.50E-01	U1/2		7.50E-01	3.4E+01	1.5E+00	4.8E+00					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-B02-A	1	7.50E-01	U1/2		7.50E-01	3.8E+01	1.5E+00	4.8E+00					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-B03-A	1	7.50E-01	U1/2		7.50E-01	2.6E+01	1.5E+00	4.8E+00					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-B01-B	1	1.59E+00	E		1.59E+00	4.2E+01	1.5E+00	4.8E+00						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-B03-B	1	7.50E-01	U1/2		7.50E-01	5.0E+01	1.5E+00	4.8E+00						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-B01-C	1	1.61E+00	E		1.61E+00	4.5E+01	1.5E+00	4.8E+00						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-B02-C	1	7.50E-01	U1/2		7.50E-01	3.7E+01	1.5E+00	4.8E+00						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1313-B03-C	1	2.16E+00	E		2.16E+00	1.5E+01	1.5E+00	4.8E+00						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	SWA-L09-1313-T01-A	1	4.43E+00			4.43E+00	4.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 2:54 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T02-A	1	4.28E+00			4.28E+00	5.3E+00	1.0E+00	3.2E+00	10	100	1.06E+03	106%	VU ICP-OES	4/20/11 2:56 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T03-A	1	3.45E+00			3.45E+00	1.2E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 2:58 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T04-A	1	4.44E+00			4.44E+00	6.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 2:59 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T05-A	1	4.76E+00			4.76E+00	1.1E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:01 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T06-A	1	6.57E+00			6.57E+00	4.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:03 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T07-A	1	1.99E+02			1.99E+02	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:04 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T08-A	1	8.53E+02			8.53E+02	1.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:06 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T09-A	1	1.44E+03			1.44E+03	1.5E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:08 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T01-B	1	4.31E+00			4.31E+00	7.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:09 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T02-B	1	6.68E+00			6.68E+00	2.6E+00	1.0E+00	3.2E+00	10	100	1.03E+03	102%	VU ICP-OES	4/20/11 3:11 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T03-B	1	3.99E+00			3.99E+00	2.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:13 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T04-B	1	4.09E+00			4.09E+00	6.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:14 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T05-B	1	5.03E+00			5.03E+00	1.2E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:16 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T06-B	1	2.07E+02			2.07E+02	3.4E-02	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:18 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T07-B	1	8.62E+02			8.62E+02	2.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 4:40 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T08-B	1	8.67E+02			8.67E+02	1.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:21 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T09-B	1	1.62E+03			1.62E+03	4.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:23 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T01-C	1	5.00E-01	U1/2		5.00E-01	1.9E+02	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:31 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T02-C	1	4.03E+00			4.03E+00	7.7E+00	1.0E+00	3.2E+00	10	100	1.06E+03	106%	VU ICP-OES	4/20/11 3:33 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T03-C	1	3.36E+00			3.36E+00	1.2E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/20/11 3:34 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T04-C	1	3.99E+00			3.99E+00	8.9E+00	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:36 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T05-C	1	4.00E+00			4.00E+00	2.8E+01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:38 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T06-C	1	5.01E+02			5.01E+02	7.3E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:39 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T07-C	1	4.78E+02			4.78E+02	2.4E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:41 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T08-C	1	1.25E+03			1.25E+03	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 4:42 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-T09-C	1	1.63E+03			1.63E+03	4.3E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 3:44 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-B01-A	1	1.57E+00	E		1.57E+00	8.6E+01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 2:41 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-B02-A	1	2.52E+00	E		2.52E+00	6.1E+00	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 2:43 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	9.6E+01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 2:44 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-B01-B	1	3.44E+00			3.44E+00	1.3E+01	1.0E+00	3.2E+00						4/20/11 2:46 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-B03-B	1	2.08E+00	E		2.08E+00	8.3E+01	1.0E+00	3.2E+00						4/20/11 2:48 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-B01-C	1	2.44E+00	E		2.44E+00	7.2E+00	1.0E+00	3.2E+00						4/20/11 2:49 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-B02-C	1	2.52E+00	E		2.52E+00	7.3E+00	1.0E+00	3.2E+00						4/20/11 2:51 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1313-B03-C	1	2.34E+00	E		2.34E+00	1.2E+01	1.0E+00	3.2E+00						4/20/11 2:53 PM	EPA Interlab L09 1313-1316 SWA

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	SWA-L10-1313-T01-A	1	3.13E+04			3.13E+04	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T02-A	1	4.74E+03			4.74E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T03-A	1	4.91E+02			4.91E+02	1.9E+00	1.0E+00	3.2E+00	1000	125	1.59E+03	88%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T04-A	1	2.14E+02			2.14E+02	3.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T05-A	1	8.52E+01			8.52E+01	9.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T06-A	1	5.77E+01			5.77E+01	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T07-A	1	4.67E+04			4.67E+04	5.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T08-A	1	1.61E+05			1.61E+05	9.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T09-A	1	3.03E+05			3.03E+05	5.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T01-B	1	3.69E+04			3.69E+04	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T02-B	1	5.80E+03			5.80E+03	4.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T03-B	1	5.11E+02			5.11E+02	1.1E+00	1.0E+00	3.2E+00	1000	125	1.76E+03	100%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T04-B	1	2.42E+02			2.42E+02	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T05-B	1	9.95E+01			9.95E+01	2.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T06-B	1	8.00E+01			8.00E+01	7.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T07-B	1	4.48E+04			4.48E+04	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T08-B	1	1.39E+05			1.39E+05	1.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T09-B	1	3.27E+05			3.27E+05	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T01-C	1	3.87E+04			3.87E+04	9.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T02-C	1	5.54E+03			5.54E+03	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T03-C	1	4.99E+02			4.99E+02	2.6E-01	1.0E+00	3.2E+00	1000	125	1.76E+03	101%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T04-C	1	2.01E+02			2.01E+02	2.5E+00	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T05-C	1	9.77E+01			9.77E+01	4.1E+00	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T06-C	1	6.84E+01			6.84E+01	3.5E+00	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T07-C	1	4.25E+04			4.25E+04	1.5E+00	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T08-C	1	1.85E+05			1.85E+05	6.6E-01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-T09-C	1	3.29E+05			3.29E+05	5.6E-01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	3.4E+01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1313-B02-A	1	2.25E+00	E		2.25E+00	2.9E+00	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	SWA-L10-1313-T01-A	1	5.06E+03			5.06E+03	1.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T02-A	1	1.34E+03			1.34E+03	6.3E-01	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T03-A	1	7.99E+02			7.99E+02	8.4E-01	7.5E+00	2.4E+01	10	100	1.86E+03	106%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T04-A	1	1.05E+03			1.05E+03	1.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T05-A	1	9.54E+02			9.54E+02	4.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T06-A	1	9.04E+02			9.04E+02	2.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T07-A	1	7.49E+02			7.49E+02	1.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T08-A	1	9.22E+02			9.22E+02	5.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T09-A	1	4.39E+03			4.39E+03	5.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T01-B	1	3.30E+03			3.30E+03	6.3E-01	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T02-B	1	1.30E+03			1.30E+03	1.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T03-B	1	1.18E+03			1.18E+03	1.4E+00	7.5E+00	2.4E+01	10	100	2.29E+03	111%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T04-B	1	1.06E+03			1.06E+03	1.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T05-B	1	1.27E+03			1.27E+03	5.6E-01	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T06-B	1	1.10E+03			1.10E+03	6.2E-01	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T07-B	1	7.61E+02			7.61E+02	2.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T08-B	1	9.14E+02			9.14E+02	1.4E+02	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T09-B	1	1.12E+04			1.12E+04	4.7E-01	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T01-C	1	1.41E+03			1.41E+03	3.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T02-C	1	1.09E+03			1.09E+03	7.2E-01	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T03-C	1	1.26E+03			1.26E+03	8.9E-01	7.5E+00	2.4E+01	10	100	2.37E+03	111%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T04-C	1	9.97E+02			9.97E+02	2.7E+00	7.5E+00	2.4E+01					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T05-C	1	1.29E+03			1.29E+03	3.2E+00	7.5E+00	2.4E+01					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T06-C	1	1.16E+03			1.16E+03	1.9E+00	7.5E+00	2.4E+01					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T07-C	1	7.56E+02			7.56E+02	1.6E+00	7.5E+00	2.4E+01					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T08-C	1	9.00E+02			9.00E+02	1.3E+00	7.5E+00	2.4E+01					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-T09-C	1	3.81E+03			3.81E+03	1.0E+00	7.5E+00	2.4E+01					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-B01-A	1	8.06E+00	E		8.06E+00	6.2E+02	7.5E+00	2.4E+01					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1313-B02-A	1	3.75E+00	U1/2		3.75E+00	5.2E+01	7.5E+00	2.4E+01					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	SWA-L10-1313-T01-A	1	4.25E+03			4.25E+03	1.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T02-A	1	3.03E+02			3.03E+02	5.0E-01	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T03-A	1	1.52E+02			1.52E+02	1.3E+01	1.1E+01	3.5E+01	10	100	1.14E+03	98%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T04-A	1	3.79E+02			3.79E+02	1.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T05-A	1	1.86E+02			1.86E+02	1.5E+01	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T06-A	1	1.25E+02			1.25E+02	8.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T07-A	1	7.75E+02			7.75E+02	6.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T08-A	1	2.48E+03			2.48E+03	3.8E+01	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T09-A	1	4.88E+03			4.88E+03	5.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T01-B	1	4.81E+03			4.81E+03	1.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T02-B	1	4.04E+02			4.04E+02	2.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T03-B	1	2.31E+02			2.31E+02	4.7E+00	1.1E+01	3.5E+01	10	100	1.29E+03	106%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T04-B	1	3.92E+02			3.92E+02	4.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T05-B	1	2.11E+02			2.11E+02	5.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T06-B	1	1.75E+02			1.75E+02	3.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T07-B	1	8.27E+02			8.27E+02	3.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T08-B	1	2.39E+03			2.39E+03	1.4E+02	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T09-B	1	6.81E+03			6.81E+03	7.4E-01	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T01-C	1	5.20E+03			5.20E+03	1.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T02-C	1	3.71E+02			3.71E+02	1.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T03-C	1	2.37E+02			2.37E+02	5.7E+00	1.1E+01	3.5E+01	10	100	1.29E+03	105%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T04-C	1	3.77E+02			3.77E+02	5.8E+00	1.1E+01	3.5E+01					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T05-C	1	2.42E+02			2.42E+02	1.2E+01	1.1E+01	3.5E+01					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T06-C	1	1.70E+02			1.70E+02	2.9E+00	1.1E+01	3.5E+01					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T07-C	1	6.47E+02			6.47E+02	1.5E+00	1.1E+01	3.5E+01					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T08-C	1	2.56E+03			2.56E+03	3.7E-01	1.1E+01	3.5E+01					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-T09-C	1	5.20E+03			5.20E+03	1.1E+00	1.1E+01	3.5E+01					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-B01-A	1	5.50E+00	U1/2		5.50E+00	6.1E+01	1.1E+01	3.5E+01					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1313-B02-A	1	5.50E+00	U1/2		5.50E+00	1.3E+01	1.1E+01	3.5E+01					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	SWA-L10-1313-T01-A	1	7.90E+02			7.90E+02	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T02-A	1	6.14E+01			6.14E+01	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T03-A	1	9.98E+02			9.98E+02	1.1E+00	1.0E+00	3.2E+00	1000	100	1.91E+03	91%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T04-A	1	1.61E+03			1.61E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T05-A	1	2.55E+03			2.55E+03	3.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T06-A	1	3.96E+03			3.96E+03	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T07-A	1	5.34E+03			5.34E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T08-A	1	5.22E+03			5.22E+03	2.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T09-A	1	1.51E+03			1.51E+03	4.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T01-B	1	9.32E+02			9.32E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T02-B	1	1.20E+02			1.20E+02	4.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T03-B	1	1.05E+03			1.05E+03	9.0E-01	1.0E+00	3.2E+00	1000	100	2.10E+03	105%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T04-B	1	1.58E+03			1.58E+03	2.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T05-B	1	2.54E+03			2.54E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T06-B	1	3.01E+03			3.01E+03	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T07-B	1	5.51E+03			5.51E+03	6.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T08-B	1	5.16E+03			5.16E+03	1.3E+02	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T09-B	1	1.70E+03			1.70E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T01-C	1	9.58E+02			9.58E+02	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T02-C	1	9.49E+01			9.49E+01	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T03-C	1	1.05E+03			1.05E+03	5.4E-01	1.0E+00	3.2E+00	1000	100	2.11E+03	106%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T04-C	1	1.57E+03			1.57E+03	1.0E+00	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T05-C	1	2.49E+03			2.49E+03	1.0E+00	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T06-C	1	3.07E+03			3.07E+03	6.4E-01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T07-C	1	5.87E+03			5.87E+03	6.4E-01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T08-C	1	5.34E+03			5.34E+03	2.8E-01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-T09-C	1	1.68E+03			1.68E+03	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-B01-A	1	1.89E+00	E		1.89E+00	4.5E+01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1313-B02-A	1	3.93E+00			3.93E+00	8.5E+00	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	SWA-L10-1313-T01-A	1	8.66E+01			8.66E+01	9.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T02-A	1	4.01E+02			4.01E+02	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T03-A	1	7.66E+02			7.66E+02	1.4E-01	1.0E+00	3.2E+00	10	100	1.65E+03	88%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T04-A	1	9.02E+02			9.02E+02	7.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T05-A	1	1.00E+03			1.00E+03	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T06-A	1	1.23E+03			1.23E+03	4.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T07-A	1	1.06E+03			1.06E+03	4.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T08-A	1	6.24E+02			6.24E+02	6.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T09-A	1	2.33E+02			2.33E+02	5.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T01-B	1	1.51E+02			1.51E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T02-B	1	3.66E+02			3.66E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T03-B	1	9.30E+02			9.30E+02	8.5E-02	1.0E+00	3.2E+00	10	100	1.91E+03	98%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T04-B	1	8.57E+02			8.57E+02	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T05-B	1	9.75E+02			9.75E+02	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T06-B	1	1.07E+03			1.07E+03	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T07-B	1	9.81E+02			9.81E+02	9.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T08-B	1	6.19E+02			6.19E+02	1.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T09-B	1	2.57E+02			2.57E+02	1.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T01-C	1	1.49E+02			1.49E+02	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T02-C	1	3.30E+02			3.30E+02	4.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T03-C	1	9.41E+02			9.41E+02	3.2E-01	1.0E+00	3.2E+00	10	100	1.92E+03	98%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T04-C	1	9.32E+02			9.32E+02	4.1E-01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T05-C	1	9.64E+02			9.64E+02	8.6E-01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T06-C	1	1.06E+03			1.06E+03	9.0E-01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T07-C	1	1.08E+03			1.08E+03	7.8E-01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T08-C	1	6.35E+02			6.35E+02	4.2E-01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-T09-C	1	2.69E+02			2.69E+02	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	6.2E+00	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.3E+01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	SWA-L10-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	4.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	6.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	1.9E+01	1.9E+00	6.0E+00	10	100	1.09E+03	109%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	1.7E+02	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	1.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	6.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T07-A	1	9.50E-01	U1/2		9.50E-01	5.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T08-A	1	9.46E+00			9.46E+00	1.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T09-A	1	3.04E+01			3.04E+01	6.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	6.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	6.8E+01	1.9E+00	6.0E+00	10	100	1.12E+03	112%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	2.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	8.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	1.0E+03	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T07-B	1	9.50E-01	U1/2		9.50E-01	6.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T08-B	1	8.07E+00			8.07E+00	1.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T09-B	1	3.52E+01			3.52E+01	4.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	3.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	2.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	3.7E+02	1.9E+00	6.0E+00	10	100	1.14E+03	114%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	9.8E+00	1.9E+00	6.0E+00					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	3.8E+02	1.9E+00	6.0E+00					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T07-C	1	9.50E-01	U1/2		9.50E-01	7.1E+01	1.9E+00	6.0E+00					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T08-C	1	1.46E+01			1.46E+01	1.5E+00	1.9E+00	6.0E+00					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-T09-C	1	3.29E+01			3.29E+01	2.0E+00	1.9E+00	6.0E+00					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	4.1E+01	1.9E+00	6.0E+00					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	4.8E+01	1.9E+00	6.0E+00					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	SWA-L10-1313-T01-A	1	1.10E+00	U1/2		1.10E+00	1.3E+02	2.2E+00	7.0E+00				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T02-A	1	1.10E+00	U1/2		1.10E+00	2.0E+04	2.2E+00	7.0E+00				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	8.7E+01	2.2E+00	7.0E+00	10	100	9.87E+02	99%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T04-A	1	1.10E+00	U1/2		1.10E+00	5.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T05-A	1	1.10E+00	U1/2		1.10E+00	6.9E+01	2.2E+00	7.0E+00				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T06-A	1	1.10E+00	U1/2		1.10E+00	1.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T07-A	1	1.84E+01			1.84E+01	5.2E+00	2.2E+00	7.0E+00				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T08-A	1	1.64E+01			1.64E+01	9.7E+01	2.2E+00	7.0E+00				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T09-A	1	1.50E+01			1.50E+01	6.3E+00	2.2E+00	7.0E+00				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T01-B	1	1.10E+00	U1/2		1.10E+00	1.8E+02	2.2E+00	7.0E+00				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T02-B	1	1.10E+00	U1/2		1.10E+00	5.7E+01	2.2E+00	7.0E+00				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	8.2E+01	2.2E+00	7.0E+00	10	100	1.11E+03	110%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T04-B	1	1.10E+00	U1/2		1.10E+00	3.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T05-B	1	1.10E+00	U1/2		1.10E+00	5.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T06-B	1	1.10E+00	U1/2		1.10E+00	2.1E+03	2.2E+00	7.0E+00				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T07-B	1	1.90E+01			1.90E+01	5.1E-01	2.2E+00	7.0E+00				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T08-B	1	1.70E+01			1.70E+01	1.4E+02	2.2E+00	7.0E+00				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T09-B	1	1.81E+01			1.81E+01	2.8E+00	2.2E+00	7.0E+00				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T01-C	1	1.10E+00	U1/2		1.10E+00	2.1E+02	2.2E+00	7.0E+00				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T02-C	1	1.10E+00	U1/2		1.10E+00	2.8E+04	2.2E+00	7.0E+00				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	1.0E+02	2.2E+00	7.0E+00	10	100	1.12E+03	112%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T04-C	1	1.10E+00	U1/2		1.10E+00	1.5E+02	2.2E+00	7.0E+00					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T05-C	1	1.10E+00	U1/2		1.10E+00	8.4E+00	2.2E+00	7.0E+00					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T06-C	1	1.10E+00	U1/2		1.10E+00	2.9E+01	2.2E+00	7.0E+00					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T07-C	1	2.21E+01			2.21E+01	2.9E+00	2.2E+00	7.0E+00					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T08-C	1	1.95E+01			1.95E+01	2.2E+00	2.2E+00	7.0E+00					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-T09-C	1	1.59E+01			1.59E+01	3.3E+00	2.2E+00	7.0E+00					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	2.5E+02	2.2E+00	7.0E+00					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	1.4E+02	2.2E+00	7.0E+00					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	SWA-L10-1313-T01-A	1	1.40E+04			1.40E+04	1.7E+00	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T02-A	1	1.25E+05			1.25E+05	8.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T03-A	1	2.62E+06			2.62E+06	7.4E-01	2.6E+00	8.3E+00	1000	100	2.62E+06	85%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T04-A	1	5.67E+06			5.67E+06	1.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T05-A	1	8.47E+06			8.47E+06	5.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T06-A	1	8.70E+06			8.70E+06	3.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T07-A	1	8.93E+06			8.93E+06	7.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T08-A	1	5.13E+06			5.13E+06	7.8E+01	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T09-A	1	1.39E+06			1.39E+06	2.9E+00	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T01-B	1	1.57E+04			1.57E+04	6.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T02-B	1	1.42E+05			1.42E+05	5.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T03-B	1	2.86E+06			2.86E+06	4.1E-01	2.6E+00	8.3E+00	1000	100	2.86E+06	93%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T04-B	1	5.55E+06			5.55E+06	3.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T05-B	1	8.00E+06			8.00E+06	2.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T06-B	1	8.58E+06			8.58E+06	1.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T07-B	1	7.83E+06			7.83E+06	8.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T08-B	1	5.18E+06			5.18E+06	1.4E+02	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T09-B	1	1.57E+06			1.57E+06	9.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T01-C	1	1.58E+04			1.58E+04	1.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T02-C	1	1.22E+05			1.22E+05	9.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T03-C	1	2.84E+06			2.84E+06	3.7E-01	2.6E+00	8.3E+00	1000	100	2.84E+06	98%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T04-C	1	5.64E+06			5.64E+06	1.3E+00	2.6E+00	8.3E+00					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T05-C	1	8.00E+06			8.00E+06	8.2E-01	2.6E+00	8.3E+00					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T06-C	1	8.51E+06			8.51E+06	4.8E-01	2.6E+00	8.3E+00					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T07-C	1	8.23E+06			8.23E+06	7.5E-01	2.6E+00	8.3E+00					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T08-C	1	5.33E+06			5.33E+06	8.3E-01	2.6E+00	8.3E+00					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-T09-C	1	1.50E+06			1.50E+06	1.6E+00	2.6E+00	8.3E+00					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-B01-A	1	4.47E+02			4.47E+02	1.1E+01	2.6E+00	8.3E+00					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1313-B02-A	1	3.98E+02			3.98E+02	2.4E-01	2.6E+00	8.3E+00					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	SWA-L10-1313-T01-A	1	6.97E+02			6.97E+02	6.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T02-A	1	4.06E+01			4.06E+01	1.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T03-A	1	1.06E+01			1.06E+01	6.0E+00	1.2E+00	3.8E+00	10	100	9.94E+02	98%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T04-A	1	9.48E+00			9.48E+00	2.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T05-A	1	1.03E+01			1.03E+01	2.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T06-A	1	2.93E+00	E		2.93E+00	1.0E+02	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T07-A	1	3.22E+02			3.22E+02	5.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T08-A	1	2.11E+03			2.11E+03	4.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T09-A	1	6.68E+03			6.68E+03	5.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T01-B	1	1.13E+03			1.13E+03	4.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T02-B	1	2.27E+01			2.27E+01	3.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T03-B	1	6.29E+00			6.29E+00	3.0E+00	1.2E+00	3.8E+00	10	100	1.09E+03	108%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T04-B	1	8.00E+00			8.00E+00	6.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T05-B	1	9.03E+00			9.03E+00	1.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T06-B	1	4.45E+00			4.45E+00	1.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T07-B	1	3.61E+02			3.61E+02	7.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T08-B	1	2.07E+03			2.07E+03	1.3E+02	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T09-B	1	7.53E+03			7.53E+03	9.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T01-C	1	1.13E+03			1.13E+03	9.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T02-C	1	6.14E+01			6.14E+01	1.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T03-C	1	5.00E+00			5.00E+00	1.4E+01	1.2E+00	3.8E+00	10	100	1.11E+03	111%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T04-C	1	1.24E+01			1.24E+01	3.8E+00	1.2E+00	3.8E+00					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T05-C	1	9.52E+00			9.52E+00	1.1E+01	1.2E+00	3.8E+00					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T06-C	1	3.54E+00	E		3.54E+00	2.2E+01	1.2E+00	3.8E+00					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T07-C	1	3.39E+02			3.39E+02	9.3E-01	1.2E+00	3.8E+00					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T08-C	1	2.05E+03			2.05E+03	4.5E-01	1.2E+00	3.8E+00					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-T09-C	1	7.23E+03			7.23E+03	1.3E+00	1.2E+00	3.8E+00					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	7.1E+01	1.2E+00	3.8E+00					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	6.9E+01	1.2E+00	3.8E+00					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	SWA-L10-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	1.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	7.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T03-A	1	2.10E+00	E		2.10E+00	1.9E+01	1.8E+00	5.7E+00	10	100	9.78E+02	98%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T04-A	1	4.41E+00	E		4.41E+00	3.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T05-A	1	2.35E+01			2.35E+01	9.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T06-A	1	3.81E+01			3.81E+01	1.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T07-A	1	2.15E+02			2.15E+02	1.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T08-A	1	1.66E+02			1.66E+02	7.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T09-A	1	7.95E+01			7.95E+01	5.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	3.1E+03	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	2.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T03-B	1	2.71E+00	E		2.71E+00	2.4E+01	1.8E+00	5.7E+00	10	100	1.09E+03	109%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T04-B	1	2.80E+00	E		2.80E+00	6.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T05-B	1	1.65E+01			1.65E+01	6.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T06-B	1	4.11E+01			4.11E+01	3.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T07-B	1	1.85E+02			1.85E+02	1.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T08-B	1	1.57E+02			1.57E+02	1.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T09-B	1	1.00E+02			1.00E+02	1.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	3.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	2.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T03-C	1	3.33E+00	E		3.33E+00	2.8E+01	1.8E+00	5.7E+00	10	100	1.10E+03	110%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T04-C	1	3.17E+00	E		3.17E+00	2.6E+01	1.8E+00	5.7E+00					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T05-C	1	1.20E+01			1.20E+01	2.7E+00	1.8E+00	5.7E+00					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T06-C	1	4.38E+01			4.38E+01	3.4E+00	1.8E+00	5.7E+00					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T07-C	1	2.02E+02			2.02E+02	1.4E+00	1.8E+00	5.7E+00					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T08-C	1	1.44E+02			1.44E+02	9.9E-01	1.8E+00	5.7E+00					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-T09-C	1	8.50E+01			8.50E+01	5.0E-01	1.8E+00	5.7E+00					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	6.0E+01	1.8E+00	5.7E+00					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	SWA-L10-1313-T01-A	1	1.85E+00	U1/2		1.85E+00	3.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T02-A	1	1.85E+00	U1/2		1.85E+00	9.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T03-A	1	5.76E+00	E		5.76E+00	1.8E+01	3.7E+00	1.2E+01	10	100	1.05E+03	104%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T04-A	1	1.12E+01	E		1.12E+01	1.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T05-A	1	1.25E+01			1.25E+01	1.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T06-A	1	1.26E+01			1.26E+01	6.2E-01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T07-A	1	1.50E+01			1.50E+01	1.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T08-A	1	1.45E+01			1.45E+01	1.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T09-A	1	3.34E+02			3.34E+02	5.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T01-B	1	1.85E+00	U1/2		1.85E+00	1.7E+02	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T02-B	1	1.85E+00	U1/2		1.85E+00	1.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T03-B	1	4.60E+00	E		4.60E+00	1.6E+01	3.7E+00	1.2E+01	10	100	1.17E+03	117%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T04-B	1	1.27E+01			1.27E+01	7.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T05-B	1	1.15E+01	E		1.15E+01	7.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T06-B	1	1.07E+01	E		1.07E+01	9.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T07-B	1	1.53E+01			1.53E+01	1.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T08-B	1	1.70E+01			1.70E+01	1.1E+02	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T09-B	1	3.47E+02			3.47E+02	1.0E-01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T01-C	1	1.85E+00	U1/2		1.85E+00	2.7E+02	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T02-C	1	1.85E+00	U1/2		1.85E+00	8.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T03-C	1	6.78E+00	E		6.78E+00	9.5E+00	3.7E+00	1.2E+01	10	100	1.19E+03	118%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T04-C	1	8.59E+00	E		8.59E+00	2.3E+01	3.7E+00	1.2E+01					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T05-C	1	1.17E+01	E		1.17E+01	1.7E+01	3.7E+00	1.2E+01					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T06-C	1	1.11E+01	E		1.11E+01	1.8E+01	3.7E+00	1.2E+01					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T07-C	1	1.06E+01	E		1.06E+01	1.4E+01	3.7E+00	1.2E+01					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T08-C	1	1.70E+01			1.70E+01	8.0E+00	3.7E+00	1.2E+01					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-T09-C	1	3.40E+02			3.40E+02	9.5E-01	3.7E+00	1.2E+01					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-B01-A	1	4.34E+00	E		4.34E+00	2.8E+01	3.7E+00	1.2E+01					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1313-B02-A	1	3.81E+00	E		3.81E+00	1.6E+01	3.7E+00	1.2E+01					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	SWA-L10-1313-T01-A	1	4.19E+01			4.19E+01	2.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T02-A	1	3.70E+01			3.70E+01	1.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T03-A	1	1.40E+01			1.40E+01	1.5E+00	2.0E+00	6.4E+00	1000	100	1.01E+03	99%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T04-A	1	2.40E+01			2.40E+01	7.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T05-A	1	1.40E+01			1.40E+01	8.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T06-A	1	1.70E+04			1.70E+04	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T07-A	1	1.09E+05			1.09E+05	5.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T08-A	1	9.48E+04			9.48E+04	1.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T09-A	1	8.58E+04			8.58E+04	5.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T01-B	1	7.87E+01			7.87E+01	7.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T02-B	1	4.44E+01			4.44E+01	1.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T03-B	1	1.44E+01			1.44E+01	7.9E+00	2.0E+00	6.4E+00	1000	100	1.12E+03	110%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T04-B	1	2.69E+01			2.69E+01	3.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T05-B	1	1.25E+01			1.25E+01	3.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T06-B	1	1.30E+01			1.30E+01	3.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T07-B	1	1.03E+05			1.03E+05	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T08-B	1	9.37E+05			9.37E+05	1.3E+02	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T09-B	1	9.59E+04			9.59E+04	4.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T01-C	1	8.74E+01			8.74E+01	1.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T02-C	1	3.75E+01			3.75E+01	8.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T03-C	1	1.26E+01			1.26E+01	6.5E+00	2.0E+00	6.4E+00	1000	100	1.13E+03	112%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T04-C	1	2.62E+01			2.62E+01	1.2E+00	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T05-C	1	1.58E+01			1.58E+01	6.9E+00	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T06-C	1	1.34E+04			1.34E+04	7.9E+00	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T07-C	1	1.14E+05			1.14E+05	4.4E-01	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T08-C	1	9.28E+04			9.28E+04	4.9E-01	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-T09-C	1	8.98E+04			8.98E+04	9.9E-01	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1313-B02-A	1	6.30E+00	E		6.30E+00	5.3E+00	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	SWA-L10-1313-T01-A	1	1.70E+01	E		1.70E+01	3.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T02-A	1	1.33E+01	E		1.33E+01	3.7E+01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T03-A	1	1.21E+01	E		1.21E+01	7.8E+01	6.8E+00	2.2E+01	10	100	9.64E+02	95%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T04-A	1	1.39E+01	E		1.39E+01	2.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T05-A	1	1.87E+01	E		1.87E+01	4.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T06-A	1	1.57E+01	E		1.57E+01	7.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T07-A	1	2.40E+01			2.40E+01	1.0E+02	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T08-A	1	5.83E+01			5.83E+01	5.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T09-A	1	1.19E+03			1.19E+03	5.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T01-B	1	1.96E+01	E		1.96E+01	1.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T02-B	1	1.02E+01	E		1.02E+01	5.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T03-B	1	1.05E+01	E		1.05E+01	7.7E+01	6.8E+00	2.2E+01	10	100	1.09E+03	108%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T04-B	1	1.06E+01	E		1.06E+01	9.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T05-B	1	2.70E+01			2.70E+01	2.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T06-B	1	3.32E+01			3.32E+01	3.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T07-B	1	2.07E+01	E		2.07E+01	3.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T08-B	1	5.72E+01			5.72E+01	1.1E+02	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T09-B	1	1.18E+03			1.18E+03	1.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T01-C	1	2.53E+01			2.53E+01	2.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T02-C	1	1.11E+01	E		1.11E+01	3.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T03-C	1	1.00E+01	E		1.00E+01	3.5E+01	6.8E+00	2.2E+01	10	100	1.09E+03	108%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T04-C	1	1.07E+01	E		1.07E+01	6.1E+01	6.8E+00	2.2E+01					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T05-C	1	2.39E+01			2.39E+01	2.4E+01	6.8E+00	2.2E+01					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T06-C	1	1.98E+01	E		1.98E+01	3.6E+01	6.8E+00	2.2E+01					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T07-C	1	2.63E+01			2.63E+01	3.4E+01	6.8E+00	2.2E+01					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T08-C	1	6.57E+01			6.57E+01	4.6E+00	6.8E+00	2.2E+01					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-T09-C	1	1.17E+03			1.17E+03	9.7E-01	6.8E+00	2.2E+01					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	1.1E+02	6.8E+00	2.2E+01					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	3.4E+01	6.8E+00	2.2E+01					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	SWA-L10-1313-T01-A	1	5.59E+00	E		5.59E+00	3.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T02-A	1	3.02E+01			3.02E+01	5.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T03-A	1	2.14E+02			2.14E+02	3.8E+00	1.9E+00	6.0E+00	10	100	1.10E+03	88%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T04-A	1	6.46E+02			6.46E+02	1.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T05-A	1	1.11E+03			1.11E+03	1.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T06-A	1	1.18E+03			1.18E+03	1.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T07-A	1	1.10E+03			1.10E+03	4.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T08-A	1	8.34E+02			8.34E+02	1.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T09-A	1	1.31E+02			1.31E+02	5.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T01-B	1	5.73E+00	E		5.73E+00	1.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T02-B	1	3.59E+01			3.59E+01	2.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T03-B	1	2.48E+02			2.48E+02	7.2E+00	1.9E+00	6.0E+00	10	100	1.12E+03	87%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T04-B	1	6.32E+02			6.32E+02	4.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T05-B	1	1.07E+03			1.07E+03	2.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T06-B	1	1.19E+03			1.19E+03	1.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T07-B	1	1.08E+03			1.08E+03	6.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T08-B	1	7.95E+02			7.95E+02	1.6E+02	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T09-B	1	1.59E+02			1.59E+02	7.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T01-C	1	8.40E+00			8.40E+00	2.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T02-C	1	3.58E+01			3.58E+01	2.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T03-C	1	2.44E+02			2.44E+02	5.7E+00	1.9E+00	6.0E+00	10	100	1.10E+03	86%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T04-C	1	6.40E+02			6.40E+02	1.6E+00	1.9E+00	6.0E+00					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T05-C	1	1.07E+03			1.07E+03	1.9E+00	1.9E+00	6.0E+00					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T06-C	1	1.17E+03			1.17E+03	2.0E+00	1.9E+00	6.0E+00					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T07-C	1	1.25E+03			1.25E+03	3.9E+00	1.9E+00	6.0E+00					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T08-C	1	8.15E+02			8.15E+02	3.9E+00	1.9E+00	6.0E+00					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-T09-C	1	1.59E+02			1.59E+02	3.5E+00	1.9E+00	6.0E+00					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	1.8E+01	1.9E+00	6.0E+00					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	1.6E+02	1.9E+00	6.0E+00					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	SWA-L10-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	1.8E+02	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	7.3E+00	2.0E+00	6.4E+00	10	100	9.68E+02	97%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T04-A	1	3.41E+01			3.41E+01	1.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T05-A	1	6.99E+03			6.99E+03	6.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T06-A	1	1.61E+04			1.61E+04	9.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T07-A	1	2.60E+04			2.60E+04	1.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T08-A	1	1.45E+04			1.45E+04	7.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T09-A	1	5.42E+03			5.42E+03	5.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	6.8E+00	2.0E+00	6.4E+00	10	100	1.09E+03	109%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T04-B	1	3.67E+01			3.67E+01	3.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T05-B	1	4.91E+03			4.91E+03	9.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T06-B	1	9.43E+03			9.43E+03	3.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T07-B	1	2.02E+04			2.02E+04	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T08-B	1	1.63E+04			1.63E+04	1.3E+02	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T09-B	1	6.18E+03			6.18E+03	3.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	4.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	5.4E+01	2.0E+00	6.4E+00	10	100	1.10E+03	110%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T04-C	1	2.76E+01			2.76E+01	6.5E-01	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T05-C	1	3.88E+03			3.88E+03	1.1E+00	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T06-C	1	9.81E+03			9.81E+03	8.8E-01	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T07-C	1	2.19E+04			2.19E+04	1.1E+00	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T08-C	1	1.50E+04			1.50E+04	7.3E-01	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-T09-C	1	5.98E+03			5.98E+03	1.3E+00	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	SWA-L10-1313-T01-A	1	1.88E+01			1.88E+01	6.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T02-A	1	4.02E+01			4.02E+01	4.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T03-A	1	4.25E+03			4.25E+03	5.1E-01	1.0E+00	3.2E+00	1000	100	5.21E+03	96%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T04-A	1	5.33E+05			5.33E+05	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T05-A	1	1.11E+06			1.11E+06	2.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T06-A	1	1.26E+06			1.26E+06	4.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T07-A	1	1.63E+06			1.63E+06	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T08-A	1	7.99E+05			7.99E+05	8.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T09-A	1	2.13E+05			2.13E+05	4.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T01-B	1	1.04E+01			1.04E+01	1.2E+02	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T02-B	1	3.29E+01			3.29E+01	4.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T03-B	1	5.10E+03			5.10E+03	1.0E-01	1.0E+00	3.2E+00	1000	100	6.12E+03	102%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T04-B	1	5.24E+05			5.24E+05	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T05-B	1	1.07E+06			1.07E+06	9.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T06-B	1	1.18E+06			1.18E+06	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T07-B	1	1.18E+06			1.18E+06	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T08-B	1	8.15E+05			8.15E+05	1.5E+02	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T09-B	1	2.41E+05			2.41E+05	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T01-C	1	1.11E+01			1.11E+01	5.6E+02	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T02-C	1	4.35E+01			4.35E+01	3.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T03-C	1	5.27E+03			5.27E+03	8.0E-01	1.0E+00	3.2E+00	1000	100	6.24E+03	97%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T04-C	1	5.35E+05			5.35E+05	6.7E-01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T05-C	1	1.04E+06			1.04E+06	7.9E-01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T06-C	1	1.18E+06			1.18E+06	3.5E-01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T07-C	1	1.26E+06			1.26E+06	1.5E+00	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T08-C	1	8.05E+05			8.05E+05	3.7E-01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-T09-C	1	2.32E+05			2.32E+05	1.6E+00	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	3.0E+01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	6.8E+01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	SWA-L10-1313-T01-A	1	1.31E+02			1.31E+02	3.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T02-A	1	1.32E+02			1.32E+02	3.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T03-A	1	1.20E+02			1.20E+02	2.2E+00	1.2E+00	3.8E+00	10	100	1.11E+03	99%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T04-A	1	1.42E+02			1.42E+02	2.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T05-A	1	1.03E+02			1.03E+02	3.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T06-A	1	3.00E+01			3.00E+01	1.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T07-A	1	1.28E+01			1.28E+01	9.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T08-A	1	1.49E+01			1.49E+01	8.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T09-A	1	1.36E+01			1.36E+01	2.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T01-B	1	1.31E+02			1.31E+02	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T02-B	1	1.46E+02			1.46E+02	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T03-B	1	1.40E+02			1.40E+02	7.0E-01	1.2E+00	3.8E+00	10	100	1.26E+03	112%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T04-B	1	1.40E+02			1.40E+02	1.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T05-B	1	1.13E+02			1.13E+02	9.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T06-B	1	8.09E+01			8.09E+01	3.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T07-B	1	8.15E+00			8.15E+00	8.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T08-B	1	1.21E+01			1.21E+01	9.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T09-B	1	1.45E+01			1.45E+01	7.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T01-C	1	1.41E+02			1.41E+02	2.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T02-C	1	1.49E+02			1.49E+02	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T03-C	1	1.37E+02			1.37E+02	2.0E+00	1.2E+00	3.8E+00	10	100	1.26E+03	113%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T04-C	1	1.42E+02			1.42E+02	1.1E+00	1.2E+00	3.8E+00					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T05-C	1	1.23E+02			1.23E+02	1.4E+00	1.2E+00	3.8E+00					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T06-C	1	7.58E+01			7.58E+01	1.6E+00	1.2E+00	3.8E+00					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T07-C	1	8.41E+00			8.41E+00	2.5E+01	1.2E+00	3.8E+00					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T08-C	1	1.49E+01			1.49E+01	8.8E+00	1.2E+00	3.8E+00					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-T09-C	1	1.29E+01			1.29E+01	3.3E+00	1.2E+00	3.8E+00					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-B01-A	1	3.06E+00	E		3.06E+00	1.1E+01	1.2E+00	3.8E+00					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1313-B02-A	1	1.98E+00	E		1.98E+00	5.2E+01	1.2E+00	3.8E+00					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	SWA-L10-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	3.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	7.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T03-A	1	2.72E+00	E		2.72E+00	2.5E+01	1.8E+00	5.7E+00	10	100	9.42E+02	94%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T04-A	1	1.09E+01			1.09E+01	3.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T05-A	1	6.41E+01			6.41E+01	5.9E+00	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T06-A	1	3.02E+02			3.02E+02	1.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T07-A	1	5.03E+02			5.03E+02	8.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T08-A	1	3.12E+02			3.12E+02	5.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T09-A	1	1.15E+02			1.15E+02	2.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	2.6E+03	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T03-B	1	3.77E+00	E		3.77E+00	3.1E+01	1.8E+00	5.7E+00	10	100	1.06E+03	106%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T04-B	1	6.77E+00			6.77E+00	5.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T05-B	1	4.17E+01			4.17E+01	8.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T06-B	1	1.09E+02			1.09E+02	5.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T07-B	1	4.09E+02			4.09E+02	4.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T08-B	1	3.26E+02			3.26E+02	1.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T09-B	1	1.33E+02			1.33E+02	3.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T01-C		9.00E-01	U1/2		0.00E+00	9.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T02-C		9.00E-01	U1/2		0.00E+00	3.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T03-C		2.44E+00	U1/2		0.00E+00	8.0E+01	1.8E+00	5.7E+00	10	100	1.08E+03	108%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T04-C		1.05E+01	U1/2		0.00E+00	2.6E+01	1.8E+00	5.7E+00					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T05-C		3.16E+01	U1/2		0.00E+00	7.9E+00	1.8E+00	5.7E+00					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T06-C		1.20E+02	U1/2		0.00E+00	3.2E+00	1.8E+00	5.7E+00					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T07-C		4.50E+02	U1/2		0.00E+00	5.9E-01	1.8E+00	5.7E+00					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T08-C		3.08E+02	U1/2		0.00E+00	2.7E-01	1.8E+00	5.7E+00					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-T09-C		1.26E+02	U1/2		0.00E+00	1.5E+00	1.8E+00	5.7E+00					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-B01-A		9.00E-01	U1/2		0.00E+00	3.4E+01	1.8E+00	5.7E+00					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1313-B02-A		9.00E-01	U1/2		0.00E+00	2.0E+03	1.8E+00	5.7E+00					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	SWA-L10-1313-T01-A	1	4.47E+01			4.47E+01	1.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T02-A	1	1.70E+01			1.70E+01	2.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T03-A	1	1.74E+01			1.74E+01	1.0E+02	3.7E+00	1.2E+01	1000	100	1.11E+03	109%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T04-A	1	3.37E+01			3.37E+01	7.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T05-A	1	4.02E+01			4.02E+01	2.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T06-A	1	4.30E+01			4.30E+01	2.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T07-A	1	2.18E+02			2.18E+02	3.1E+02	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T08-A	1	7.28E+02			7.28E+02	5.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T09-A	1	7.19E+03			7.19E+03	5.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T01-B	1	5.80E+01			5.80E+01	5.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T02-B	1	1.28E+01			1.28E+01	1.6E+02	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T03-B	1	1.28E+01			1.28E+01	3.6E+01	3.7E+00	1.2E+01	1000	100	1.19E+03	118%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T04-B	1	9.44E+01			9.44E+01	2.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T05-B	1	3.72E+01			3.72E+01	6.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T06-B	1	4.77E+01			4.77E+01	7.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T07-B	1	2.09E+02			2.09E+02	2.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T08-B	1	7.21E+02			7.21E+02	1.3E+02	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T09-B	1	1.25E+04			1.25E+04	9.2E-01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T01-C	1	5.38E+01			5.38E+01	2.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T02-C	1	2.10E+01			2.10E+01	6.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T03-C	1	3.78E+01			3.78E+01	4.0E+01	3.7E+00	1.2E+01	1000	100	1.17E+03	113%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T04-C	1	6.12E+01			6.12E+01	1.8E+01	3.7E+00	1.2E+01					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T05-C	1	1.04E+02			1.04E+02	2.7E+01	3.7E+00	1.2E+01					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T06-C	1	3.99E+01			3.99E+01	6.3E+01	3.7E+00	1.2E+01					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T07-C	1	2.06E+02			2.06E+02	6.1E+00	3.7E+00	1.2E+01					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T08-C	1	7.42E+02			7.42E+02	1.2E+00	3.7E+00	1.2E+01					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-T09-C	1	7.00E+03			7.00E+03	7.5E-01	3.7E+00	1.2E+01					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-B01-A	1	1.00E+01	E		1.00E+01	1.1E+02	3.7E+00	1.2E+01					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1313-B02-A	1	7.00E+00	E		7.00E+00	6.9E+01	3.7E+00	1.2E+01					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	SWA-L10-1313-T01-A	1	3.45E+05			3.45E+05	1.7E+00	1.6E+00	5.1E+00				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T02-A	1	3.99E+05			3.99E+05	1.5E+00	1.6E+00	5.1E+00				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T03-A	1	4.73E+05			4.73E+05	4.9E-01	1.6E+00	5.1E+00	1000	100	4.74E+05	93%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T04-A	1	5.14E+05			5.14E+05	6.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T05-A	1	5.48E+05			5.48E+05	4.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T06-A	1	5.59E+05			5.59E+05	5.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T07-A	1	3.82E+05			3.82E+05	7.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T08-A	1	2.66E+05			2.66E+05	6.3E+01	1.6E+00	5.1E+00				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T09-A	1	5.40E+04			5.40E+04	5.5E+00	1.6E+00	5.1E+00				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T01-B	1	3.40E+05			3.40E+05	7.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T02-B	1	4.14E+05			4.14E+05	3.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T03-B	1	4.98E+05			4.98E+05	9.3E-01	1.6E+00	5.1E+00	1000	100	4.99E+05	96%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T04-B	1	5.05E+05			5.05E+05	2.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T05-B	1	5.32E+05			5.32E+05	3.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T06-B	1	5.43E+05			5.43E+05	1.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T07-B	1	3.87E+05			3.87E+05	3.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T08-B	1	2.57E+05			2.57E+05	1.4E+02	1.6E+00	5.1E+00				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T09-B	1	6.18E+04			6.18E+04	1.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T01-C	1	3.54E+05			3.54E+05	9.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T02-C	1	4.07E+05			4.07E+05	9.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T03-C	1	4.86E+05			4.86E+05	7.4E-01	1.6E+00	5.1E+00	1000	100	4.87E+05	94%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T04-C	1	5.08E+05			5.08E+05	8.2E-01	1.6E+00	5.1E+00					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T05-C	1	5.31E+05			5.31E+05	5.5E-01	1.6E+00	5.1E+00					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T06-C	1	5.32E+05			5.32E+05	8.6E-01	1.6E+00	5.1E+00					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T07-C	1	3.97E+05			3.97E+05	1.6E+00	1.6E+00	5.1E+00					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T08-C	1	2.64E+05			2.64E+05	1.1E+00	1.6E+00	5.1E+00					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-T09-C	1	5.93E+04			5.93E+04	1.0E+00	1.6E+00	5.1E+00					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-B01-A	1	1.62E+03			1.62E+03	2.6E+01	1.6E+00	5.1E+00					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1313-B02-A	1	2.80E+01			2.80E+01	2.2E+01	1.6E+00	5.1E+00					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	SWA-L10-1313-T01-A	1	8.81E+04			8.81E+04	1.6E+00	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T02-A	1	8.99E+04			8.99E+04	9.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T03-A	1	9.31E+04			9.31E+04	4.7E-01	1.5E+01	4.8E+01	10	100	9.40E+04	87%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T04-A	1	1.12E+05			1.12E+05	7.4E-01	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T05-A	1	1.20E+05			1.20E+05	1.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T06-A	1	1.16E+05			1.16E+05	1.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T07-A	1	9.55E+04			9.55E+04	4.8E-01	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T08-A	1	5.16E+04			5.16E+04	4.0E+01	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T09-A	1	8.29E+03			8.29E+03	5.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T01-B	1	8.78E+04			8.78E+04	9.1E-01	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T02-B	1	9.91E+04			9.91E+04	5.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T03-B	1	1.01E+05			1.01E+05	3.8E-01	1.5E+01	4.8E+01	10	100	1.02E+05	99%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T04-B	1	1.10E+05			1.10E+05	5.2E-01	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T05-B	1	1.17E+05			1.17E+05	3.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T06-B	1	1.18E+05			1.18E+05	3.9E-01	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T07-B	1	8.04E+04			8.04E+04	5.8E-01	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T08-B	1	5.14E+04			5.14E+04	1.4E+02	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T09-B	1	9.64E+03			9.64E+03	5.9E-01	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T01-C	1	9.49E+04			9.49E+04	1.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T02-C	1	9.92E+04			9.92E+04	9.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T03-C	1	9.71E+04			9.71E+04	8.5E-01	1.5E+01	4.8E+01	10	100	9.80E+04	95%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T04-C	1	1.12E+05			1.12E+05	7.7E-01	1.5E+01	4.8E+01					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T05-C	1	1.18E+05			1.18E+05	9.7E-01	1.5E+01	4.8E+01					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T06-C	1	1.15E+05			1.15E+05	8.3E-01	1.5E+01	4.8E+01					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T07-C	1	8.34E+04			8.34E+04	8.1E-01	1.5E+01	4.8E+01					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T08-C	1	5.25E+04			5.25E+04	2.2E-01	1.5E+01	4.8E+01					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-T09-C	1	9.19E+03			9.19E+03	1.2E+00	1.5E+01	4.8E+01					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-B01-A	1	1.58E+01	E		1.58E+01	6.3E+01	1.5E+01	4.8E+01					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1313-B02-A	1	7.50E+00	U1/2		7.50E+00	7.5E+01	1.5E+01	4.8E+01					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	SWA-L10-1313-T01-A	1	4.60E+03			4.60E+03	2.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T02-A	1	3.28E+03			3.28E+03	1.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T03-A	1	1.55E+03			1.55E+03	9.3E-01	1.1E+00	3.5E+00	1000	100	2.48E+03	93%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T04-A	1	8.68E+02			8.68E+02	5.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T05-A	1	1.08E+03			1.08E+03	7.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T06-A	1	2.22E+03			2.22E+03	5.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T07-A	1	4.76E+03			4.76E+03	4.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T08-A	1	1.41E+04			1.41E+04	4.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T09-A	1	5.13E+04			5.13E+04	5.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T01-B	1	5.92E+03			5.92E+03	1.7E-02	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T02-B	1	2.92E+03			2.92E+03	3.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T03-B	1	1.54E+03			1.54E+03	1.1E+00	1.1E+00	3.5E+00	1000	100	2.54E+03	100%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T04-B	1	7.64E+02			7.64E+02	7.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T05-B	1	9.81E+02			9.81E+02	5.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T06-B	1	1.30E+03			1.30E+03	9.2E-02	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T07-B	1	5.03E+03			5.03E+03	6.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T08-B	1	1.48E+04			1.48E+04	1.3E+02	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T09-B	1	1.25E+05			1.25E+05	4.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T01-C	1	5.90E+03			5.90E+03	6.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T02-C	1	3.34E+03			3.34E+03	4.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T03-C	1	1.52E+03			1.52E+03	1.1E+00	1.1E+00	3.5E+00	1000	100	2.48E+03	96%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T04-C	1	9.48E+02			9.48E+02	1.2E+00	1.1E+00	3.5E+00					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T05-C	1	9.72E+02			9.72E+02	7.2E-01	1.1E+00	3.5E+00					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T06-C	1	1.33E+03			1.33E+03	4.4E-01	1.1E+00	3.5E+00					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T07-C	1	5.21E+03			5.21E+03	6.1E-01	1.1E+00	3.5E+00					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T08-C	1	1.41E+04			1.41E+04	5.0E-01	1.1E+00	3.5E+00					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-T09-C	1	4.62E+04			4.62E+04	1.1E+00	1.1E+00	3.5E+00					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-B01-A	1	1.83E+00	E		1.83E+00	1.2E+02	1.1E+00	3.5E+00					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1313-B02-A	1	7.09E+00			7.09E+00	7.6E+00	1.1E+00	3.5E+00					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	SWA-L10-1313-T01-A	1	5.13E+05			5.13E+05	2.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T02-A	1	5.51E+05			5.51E+05	8.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T03-A	1	6.00E+05			6.00E+05	4.2E-01	2.5E+00	8.0E+00	1000	100	6.01E+05	94%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T04-A	1	6.43E+05			6.43E+05	9.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T05-A	1	6.64E+05			6.64E+05	2.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T06-A	1	6.54E+05			6.54E+05	7.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T07-A	1	4.22E+05			4.22E+05	7.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T08-A	1	2.61E+05			2.61E+05	6.7E+01	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T09-A	1	1.26E+05			1.26E+05	3.6E+00	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T01-B	1	4.96E+05			4.96E+05	1.5E+00	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T02-B	1	5.54E+05			5.54E+05	5.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T03-B	1	6.08E+05			6.08E+05	3.6E-03	2.5E+00	8.0E+00	1000	100	6.09E+05	109%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T04-B	1	6.23E+05			6.23E+05	2.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T05-B	1	6.44E+05			6.44E+05	2.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T06-B	1	6.44E+05			6.44E+05	2.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T07-B	1	4.37E+05			4.37E+05	1.4E+00	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T08-B	1	2.38E+05			2.38E+05	1.1E+02	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T09-B	1	1.37E+05			1.37E+05	3.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T01-C	1	5.08E+05			5.08E+05	2.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T02-C	1	5.52E+05			5.52E+05	7.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T03-C	1	5.99E+05			5.99E+05	1.5E-01	2.5E+00	8.0E+00	1000	100	6.00E+05	108%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T04-C	1	6.25E+05			6.25E+05	1.1E+00	2.5E+00	8.0E+00					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T05-C	1	6.41E+05			6.41E+05	4.1E-01	2.5E+00	8.0E+00					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T06-C	1	6.32E+05			6.32E+05	5.5E-01	2.5E+00	8.0E+00					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T07-C	1	4.36E+05			4.36E+05	1.1E+00	2.5E+00	8.0E+00					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T08-C	1	2.84E+05			2.84E+05	5.6E-01	2.5E+00	8.0E+00					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-T09-C	1	1.32E+05			1.32E+05	4.8E-01	2.5E+00	8.0E+00					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-B01-A	1	5.45E+00	E		5.45E+00	1.4E+01	2.5E+00	8.0E+00					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1313-B02-A	1	1.25E+00	U1/2		1.25E+00	3.0E+00	2.5E+00	8.0E+00					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	SWA-L10-1313-T01-A	1	3.03E+02			3.03E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T02-A	1	2.25E+03			2.25E+03	9.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T03-A	1	1.51E+04			1.51E+04	2.0E+00	1.0E+00	3.2E+00	1000	100	1.61E+04	93%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T04-A	1	2.82E+04			2.82E+04	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T05-A	1	4.12E+04			4.12E+04	7.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T06-A	1	4.35E+04			4.35E+04	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T07-A	1	4.26E+04			4.26E+04	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T08-A	1	2.59E+04			2.59E+04	9.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T09-A	1	7.21E+03			7.21E+03	6.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T01-B	1	3.30E+02			3.30E+02	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T02-B	1	2.47E+03			2.47E+03	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T03-B	1	1.73E+04			1.73E+04	3.7E-01	1.0E+00	3.2E+00	1000	100	1.83E+04	97%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T04-B	1	2.80E+04			2.80E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T05-B	1	3.83E+04			3.83E+04	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T06-B	1	4.23E+04			4.23E+04	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T07-B	1	3.93E+04			3.93E+04	8.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T08-B	1	2.25E+04			2.25E+04	1.1E+02	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T09-B	1	8.06E+03			8.06E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T01-C	1	3.43E+02			3.43E+02	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T02-C	1	2.11E+03			2.11E+03	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T03-C	1	1.71E+04			1.71E+04	1.2E+00	1.0E+00	3.2E+00	1000	100	1.81E+04	94%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T04-C	1	2.81E+04			2.81E+04	3.7E-01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T05-C	1	3.80E+04			3.80E+04	5.3E-01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T06-C	1	4.15E+04			4.15E+04	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T07-C	1	4.06E+04			4.06E+04	6.5E-01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T08-C	1	2.69E+04			2.69E+04	1.3E-01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-T09-C	1	7.71E+03			7.71E+03	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	2.1E+01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	3.8E+01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	SWA-L10-1313-T01-A	1	7.12E+05			7.12E+05	1.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T02-A	1	8.41E+05			8.41E+05	1.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T03-A	1	8.71E+05			8.71E+05	4.1E-01	6.8E+00	2.2E+01	1000	100	8.72E+05	96%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T04-A	1	8.19E+05			8.19E+05	4.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T05-A	1	7.80E+05			7.80E+05	4.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T06-A	1	3.84E+05			3.84E+05	2.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T07-A	1	4.14E+05			4.14E+05	6.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T08-A	1	1.87E+05			1.87E+05	3.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T09-A	1	3.80E+04			3.80E+04	5.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T01-B	1	7.30E+05			7.30E+05	1.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T02-B	1	9.43E+05			9.43E+05	6.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T03-B	1	9.69E+05			9.69E+05	8.8E-01	6.8E+00	2.2E+01	1000	100	9.70E+05	98%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T04-B	1	8.42E+05			8.42E+05	3.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T05-B	1	8.24E+05			8.24E+05	6.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T06-B	1	7.88E+05			7.88E+05	1.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T07-B	1	2.93E+05			2.93E+05	1.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T08-B	1	8.02E+04			8.02E+04	1.4E+02	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T09-B	1	4.34E+04			4.34E+04	4.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T01-C	1	6.88E+05			6.88E+05	7.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T02-C	1	9.71E+05			9.71E+05	3.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T03-C	1	8.32E+05			8.32E+05	4.1E-01	6.8E+00	2.2E+01	1000	100	8.33E+05	93%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T04-C	1	8.20E+05			8.20E+05	2.8E-01	6.8E+00	2.2E+01					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T05-C	1	8.23E+05			8.23E+05	2.0E-01	6.8E+00	2.2E+01					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T06-C	1	7.48E+05			7.48E+05	3.2E-01	6.8E+00	2.2E+01					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T07-C	1	3.73E+05			3.73E+05	8.2E-01	6.8E+00	2.2E+01					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T08-C	1	1.94E+05			1.94E+05	2.3E-01	6.8E+00	2.2E+01					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-T09-C	1	4.19E+04			4.19E+04	1.0E+00	6.8E+00	2.2E+01					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-B01-A	1	1.54E+01	E		1.54E+01	2.7E+01	6.8E+00	2.2E+01					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1313-B02-A	1	3.02E+01			3.02E+01	9.0E+00	6.8E+00	2.2E+01					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	SWA-L10-1313-T01-A	1	2.30E+00	U1/2		2.30E+00	4.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T02-A	1	2.30E+00	U1/2		2.30E+00	1.0E+02	4.6E+00	1.5E+01				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T03-A	1	2.30E+00	U1/2		2.30E+00	5.5E+01	4.6E+00	1.5E+01	10	100	8.85E+02	88%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T04-A	1	2.30E+00	U1/2		2.30E+00	1.2E+03	4.6E+00	1.5E+01				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T05-A	1	2.30E+00	U1/2		2.30E+00	1.7E+02	4.6E+00	1.5E+01				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T06-A	1	1.32E+01	E		1.32E+01	1.9E+01	4.6E+00	1.5E+01				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T07-A	1	1.65E+01			1.65E+01	2.4E+01	4.6E+00	1.5E+01				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T08-A	1	5.11E+00	E		5.11E+00	1.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T09-A	1	2.30E+00	U1/2		2.30E+00	3.6E+02	4.6E+00	1.5E+01				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T01-B	1	2.30E+00	U1/2		2.30E+00	3.1E+02	4.6E+00	1.5E+01				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T02-B	1	2.30E+00	U1/2		2.30E+00	2.2E+02	4.6E+00	1.5E+01				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T03-B	1	2.30E+00	U1/2		2.30E+00	3.6E+01	4.6E+00	1.5E+01	10	100	9.98E+02	100%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T04-B	1	2.30E+00	U1/2		2.30E+00	2.4E+02	4.6E+00	1.5E+01				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T05-B	1	1.81E+01			1.81E+01	1.0E+02	4.6E+00	1.5E+01				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T06-B	1	1.55E+01			1.55E+01	6.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T07-B	1	1.02E+01	E		1.02E+01	8.8E+01	4.6E+00	1.5E+01				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T08-B	1	2.30E+00	U1/2		2.30E+00	9.9E+02	4.6E+00	1.5E+01				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T09-B	1	2.30E+00	U1/2		2.30E+00	1.5E+03	4.6E+00	1.5E+01				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T01-C	1	2.30E+00	U1/2		2.30E+00	1.2E+03	4.6E+00	1.5E+01				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T02-C	1	2.30E+00	U1/2		2.30E+00	1.6E+02	4.6E+00	1.5E+01				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T03-C	1	2.30E+00	U1/2		2.30E+00	6.3E+00	4.6E+00	1.5E+01	10	100	9.84E+02	98%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T04-C	1	2.30E+00	U1/2		2.30E+00	2.4E+01	4.6E+00	1.5E+01					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T05-C	1	4.82E+00	E		4.82E+00	9.0E+01	4.6E+00	1.5E+01					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T06-C	1	1.14E+01	E		1.14E+01	8.7E+01	4.6E+00	1.5E+01					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T07-C	1	1.43E+01	E		1.43E+01	2.0E+01	4.6E+00	1.5E+01					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T08-C	1	4.93E+00	E		4.93E+00	8.9E+01	4.6E+00	1.5E+01					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-T09-C	1	2.30E+00	U1/2		2.30E+00	2.3E+02	4.6E+00	1.5E+01					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	4.5E+01	4.6E+00	1.5E+01					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	3.3E+01	4.6E+00	1.5E+01					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	SWA-L10-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	4.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	9.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	6.3E+01	2.0E+00	6.4E+00	10	100	1.01E+03	101%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	3.0E+02	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	1.0E+02	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	3.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	2.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T08-A	1	1.16E+02			1.16E+02	5.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T09-A	1	1.01E+04			1.01E+04	4.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	5.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	7.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	3.1E+01	2.0E+00	6.4E+00	10	100	1.13E+03	113%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	1.9E+03	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	7.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T07-B	1	2.95E+01			2.95E+01	2.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T08-B	1	1.04E+02			1.04E+02	1.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T09-B	1	1.83E+04			1.83E+04	3.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	4.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	2.0E+02	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	2.6E+01	2.0E+00	6.4E+00	10	100	1.13E+03	113%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	1.9E+02	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	3.9E+01	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T07-C	1	1.95E+01			1.95E+01	1.1E+01	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T08-C	1	1.43E+02			1.43E+02	1.6E+00	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-T09-C	1	9.69E+03			9.69E+03	1.8E+00	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	SWA-L10-1313-T01-A	1	2.98E+02			2.98E+02	1.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T02-A	1	9.18E+01			9.18E+01	9.9E-01	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T03-A	1	8.75E+01			8.75E+01	8.5E-01	1.5E+00	4.8E+00	10	100	1.09E+03	100%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T04-A	1	1.42E+02			1.42E+02	9.7E-02	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T05-A	1	1.20E+02			1.20E+02	1.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T06-A	1	1.11E+02			1.11E+02	3.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T07-A	1	1.07E+02			1.07E+02	2.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T08-A	1	5.60E+01			5.60E+01	4.4E+01	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T09-A	1	5.63E+02			5.63E+02	4.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T01-B	1	3.26E+02			3.26E+02	1.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T02-B	1	9.74E+01			9.74E+01	3.6E-01	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T03-B	1	9.88E+01			9.88E+01	1.3E+00	1.5E+00	4.8E+00	10	100	1.22E+03	112%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T04-B	1	1.45E+02			1.45E+02	2.9E+00	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T05-B	1	1.19E+02			1.19E+02	6.6E-01	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T06-B	1	1.21E+02			1.21E+02	9.8E-01	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T07-B	1	7.94E+01			7.94E+01	5.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T08-B	1	4.68E+01			4.68E+01	1.0E+02	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T09-B	1	6.03E+02			6.03E+02	4.8E-01	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T01-C	1	3.47E+02			3.47E+02	1.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T02-C	1	9.76E+01			9.76E+01	9.9E-01	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T03-C	1	9.87E+01			9.87E+01	1.5E+00	1.5E+00	4.8E+00	10	100	1.24E+03	114%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T04-C	1	1.45E+02			1.45E+02	2.2E+00	1.5E+00	4.8E+00					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T05-C	1	1.36E+02			1.36E+02	8.4E-02	1.5E+00	4.8E+00					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T06-C	1	1.17E+02			1.17E+02	7.0E-01	1.5E+00	4.8E+00					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T07-C	1	8.64E+01			8.64E+01	4.9E+00	1.5E+00	4.8E+00					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T08-C	1	5.57E+01			5.57E+01	4.8E+00	1.5E+00	4.8E+00					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-T09-C	1	6.17E+02			6.17E+02	1.3E+00	1.5E+00	4.8E+00					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-B01-A	1	7.50E-01	U1/2		7.50E-01	4.6E+01	1.5E+00	4.8E+00					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1313-B02-A	1	1.66E+00	E		1.66E+00	3.4E+01	1.5E+00	4.8E+00					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	SWA-L10-1313-T01-A	1	3.22E+00			3.22E+00	8.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 11:59 AM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T02-A	1	4.83E+00			4.83E+00	7.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:01 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T03-A	1	6.98E+00			6.98E+00	4.2E+00	1.0E+00	3.2E+00	10	100	1.09E+03	108%	VU ICP-OES	12/8/10 12:02 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T04-A	1	5.39E+00			5.39E+00	1.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:04 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T05-A	1	9.44E+00			9.44E+00	2.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:06 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T06-A	1	2.23E+02			2.23E+02	2.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:07 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T07-A	1	9.30E+02			9.30E+02	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:09 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T08-A	1	1.07E+03			1.07E+03	4.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:10 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T09-A	1	5.07E+02			5.07E+02	5.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:12 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T01-B	1	2.90E+00	E		2.90E+00	5.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:24 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T02-B	1	2.68E+00	E		2.68E+00	8.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:25 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T03-B	1	3.47E+00			3.47E+00	1.6E+01	1.0E+00	3.2E+00	10	100	1.11E+03	111%	VU ICP-OES	12/8/10 12:27 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T04-B	1	5.64E+00			5.64E+00	2.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:29 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T05-B	1	7.74E+00			7.74E+00	8.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:30 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T06-B	1	1.24E+01			1.24E+01	6.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:32 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T07-B	1	1.02E+03			1.02E+03	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:33 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T08-B	1	9.94E+02			9.94E+02	1.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:35 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T09-B	1	5.68E+02			5.68E+02	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:37 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T01-C	1	2.49E+00	E		2.49E+00	1.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:43 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T02-C	1	2.98E+00	E		2.98E+00	1.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 12:45 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T03-C	1	3.25E+00			3.25E+00	8.4E+00	1.0E+00	3.2E+00	10	100	1.13E+03	113%	VU ICP-OES	12/8/10 12:47 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T04-C	1	6.29E+00			6.29E+00	8.5E+00	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:48 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T05-C	1	1.12E+01			1.12E+01	5.7E+00	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:50 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T06-C	1	1.44E+01			1.44E+01	7.0E+00	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:52 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T07-C	1	1.06E+03			1.06E+03	1.5E+00	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:53 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T08-C	1	1.04E+03			1.04E+03	4.0E-01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:55 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-T09-C	1	5.46E+02			5.46E+02	1.6E+00	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 12:57 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-B01-A	1	3.56E+00			3.56E+00	2.2E+01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 11:56 AM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1313-B02-A	1	5.29E+00			5.29E+00	8.5E-01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 11:57 AM	EPA Interlab L10 1313-1316 SWA

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	SWA-L11-1313-T01-A	1	3.41E+04			3.41E+04	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T02-A	1	1.21E+03			1.21E+03	3.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T03-A	1	2.96E+02			2.96E+02	3.6E+01	1.0E+00	3.2E+00	1000	100	1.26E+03	96%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T04-A	1	1.16E+02			1.16E+02	8.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T05-A	1	1.93E+01			1.93E+01	4.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T06-A	1	9.08E+00			9.08E+00	1.5E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T07-A	1	8.79E+03			8.79E+03	4.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T08-A	1	2.41E+05			2.41E+05	6.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T09-A	1	7.19E+05			7.19E+05	7.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T01-B	1	3.36E+04			3.36E+04	6.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T02-B	1	9.87E+02			9.87E+02	4.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T03-B	1	5.83E+02			5.83E+02	9.6E-01	1.0E+00	3.2E+00	1000	100	1.51E+03	93%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T04-B	1	9.35E+01			9.35E+01	2.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T05-B	1	1.81E+01			1.81E+01	1.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T06-B	1	1.27E+01			1.27E+01	9.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T07-B	1	8.92E+03			8.92E+03	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T08-B	1	2.31E+05			2.31E+05	1.1E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T09-B	1	7.20E+05			7.20E+05	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T01-C	1	3.42E+04			3.42E+04	3.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T02-C	1	8.92E+03			8.92E+03	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T03-C	1	2.79E+02			2.79E+02	2.2E+00	1.0E+00	3.2E+00	1000	100	1.17E+03	89%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T04-C	1	1.05E+02			1.05E+02	4.9E+00	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T05-C	1	2.57E+01			2.57E+01	1.9E+01	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T06-C	1	4.07E+01			4.07E+01	6.2E+00	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T07-C	1	7.66E+03			7.66E+03	2.0E-01	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T08-C	1	2.25E+05			2.25E+05	7.4E+00	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-T09-C	1	6.96E+05			6.96E+05	3.3E-01	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-B01-A	1	5.59E+00			5.59E+00	2.8E+02	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1313-B02-A	1	6.77E+00			6.77E+00	3.8E+01	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	SWA-L11-1313-T01-A	1	3.73E+03			3.73E+03	4.5E-01	7.5E+00	2.4E+01				---	VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T02-A	1	9.88E+02			9.88E+02	9.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T03-A	1	9.22E+02			9.22E+02	3.8E+01	7.5E+00	2.4E+01	10	100	1.92E+03	99%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T04-A	1	8.01E+02			8.01E+02	8.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T05-A	1	6.05E+02			6.05E+02	1.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T06-A	1	5.89E+02			5.89E+02	8.4E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T07-A	1	4.33E+02			4.33E+02	1.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T08-A	1	2.48E+02			2.48E+02	4.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T09-A	1	1.87E+03			1.87E+03	2.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T01-B	1	3.19E+03			3.19E+03	4.2E-01	7.5E+00	2.4E+01				---	VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T02-B	1	1.01E+03			1.01E+03	8.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T03-B	1	1.12E+03			1.12E+03	1.8E+00	7.5E+00	2.4E+01	10	100	2.18E+03	106%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T04-B	1	8.68E+02			8.68E+02	7.2E-01	7.5E+00	2.4E+01				---	VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T05-B	1	5.49E+02			5.49E+02	3.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T06-B	1	5.30E+02			5.30E+02	3.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T07-B	1	5.52E+02			5.52E+02	3.4E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T08-B	1	2.44E+02			2.44E+02	1.1E+02	7.5E+00	2.4E+01				---	VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T09-B	1	2.12E+03			2.12E+03	7.2E-01	7.5E+00	2.4E+01				---	VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T01-C	1	2.99E+03			2.99E+03	3.2E-01	7.5E+00	2.4E+01				---	VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T02-C	1	1.56E+03			1.56E+03	1.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T03-C	1	1.38E+03			1.38E+03	3.6E-01	7.5E+00	2.4E+01	10	100	2.42E+03	104%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T04-C	1	8.57E+02			8.57E+02	1.2E+00	7.5E+00	2.4E+01					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T05-C	1	5.18E+02			5.18E+02	5.0E+00	7.5E+00	2.4E+01					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T06-C	1	7.10E+02			7.10E+02	2.6E+00	7.5E+00	2.4E+01					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T07-C	1	4.34E+02			4.34E+02	2.6E+00	7.5E+00	2.4E+01					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T08-C	1	2.53E+02			2.53E+02	8.5E+00	7.5E+00	2.4E+01					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-T09-C	1	2.33E+03			2.33E+03	2.9E+00	7.5E+00	2.4E+01					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-B01-A	1	3.75E+00	U1/2		3.75E+00	3.0E+01	7.5E+00	2.4E+01					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
Sb	SWA-L11-1313-B02-A	1	3.75E+00	U1/2		3.75E+00	4.8E+01	7.5E+00	2.4E+01					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	SWA-L11-1313-T01-A	1	4.67E+03			4.67E+03	9.5E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T02-A	1	2.89E+02			2.89E+02	5.1E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T03-A	1	1.27E+02			1.27E+02	4.6E+01	1.1E+01	3.5E+01	10	100	1.13E+03	101%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T04-A	1	1.39E+02			1.39E+02	1.1E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T05-A	1	8.83E+01			8.83E+01	3.2E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T06-A	1	7.53E+01			7.53E+01	4.4E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T07-A	1	3.05E+02			3.05E+02	1.0E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T08-A	1	1.66E+03			1.66E+03	8.1E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T09-A	1	7.30E+03			7.30E+03	1.2E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T01-B	1	4.30E+03			4.30E+03	7.1E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T02-B	1	2.95E+02			2.95E+02	8.7E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T03-B	1	2.03E+02			2.03E+02	5.6E+00	1.1E+01	3.5E+01	10	100	1.18E+03	98%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T04-B	1	1.47E+02			1.47E+02	1.2E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T05-B	1	9.52E+01			9.52E+01	2.5E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T06-B	1	9.41E+01			9.41E+01	1.1E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T07-B	1	1.18E+03			1.18E+03	1.1E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T08-B	1	1.71E+03			1.71E+03	1.4E+02	1.1E+01	3.5E+01			---		VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T09-B	1	8.35E+03			8.35E+03	7.6E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T01-C	1	4.45E+03			4.45E+03	7.4E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T02-C	1	7.28E+02			7.28E+02	2.4E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T03-C	1	1.98E+02			1.98E+02	6.9E+00	1.1E+01	3.5E+01	10	100	1.16E+03	96%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T04-C	1	1.46E+02			1.46E+02	9.2E+00	1.1E+01	3.5E+01					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T05-C	1	9.59E+01			9.59E+01	1.4E+01	1.1E+01	3.5E+01					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T06-C	1	7.02E+01			7.02E+01	2.3E+01	1.1E+01	3.5E+01					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T07-C	1	4.22E+02			4.22E+02	1.4E+00	1.1E+01	3.5E+01					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T08-C	1	1.56E+03			1.56E+03	2.6E+00	1.1E+01	3.5E+01					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-T09-C	1	7.27E+03			7.27E+03	8.0E-01	1.1E+01	3.5E+01					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-B01-A	1	5.50E+00	U1/2		5.50E+00	2.5E+01	1.1E+01	3.5E+01					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1313-B02-A	1	5.50E+00	U1/2		5.50E+00	2.4E+01	1.1E+01	3.5E+01					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	SWA-L11-1313-T01-A	1	6.68E+02			6.68E+02	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T02-A	1	6.44E+02			6.44E+02	5.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T03-A	1	8.33E+02			8.33E+02	3.8E+01	1.0E+00	3.2E+00	1000	100	1.82E+03	99%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T04-A	1	1.38E+03			1.38E+03	7.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T05-A	1	3.80E+03			3.80E+03	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T06-A	1	3.75E+03			3.75E+03	8.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T07-A	1	3.22E+03			3.22E+03	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T08-A	1	3.88E+03			3.88E+03	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T09-A	1	4.83E+03			4.83E+03	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T01-B	1	6.57E+02			6.57E+02	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T02-B	1	6.50E+02			6.50E+02	4.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T03-B	1	8.97E+02			8.97E+02	1.3E+00	1.0E+00	3.2E+00	1000	100	1.88E+03	98%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T04-B	1	1.45E+03			1.45E+03	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T05-B	1	4.23E+03			4.23E+03	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T06-B	1	3.73E+03			3.73E+03	3.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T07-B	1	3.56E+03			3.56E+03	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T08-B	1	4.17E+03			4.17E+03	9.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T09-B	1	4.66E+03			4.66E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T01-C	1	7.33E+02			7.33E+02	3.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T02-C	1	7.39E+02			7.39E+02	3.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T03-C	1	9.45E+02			9.45E+02	9.8E-01	1.0E+00	3.2E+00	1000	100	1.87E+03	92%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T04-C	1	1.46E+03			1.46E+03	2.4E-01	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T05-C	1	3.80E+03			3.80E+03	3.8E+00	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T06-C	1	3.92E+03			3.92E+03	1.7E+00	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T07-C	1	3.38E+03			3.38E+03	2.3E-01	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T08-C	1	4.03E+03			4.03E+03	2.7E+00	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-T09-C	1	4.95E+03			4.95E+03	6.3E-01	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-B01-A	1	3.56E+00			3.56E+00	1.0E+02	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
B	SWA-L11-1313-B02-A	1	1.30E+01			1.30E+01	3.5E+00	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	SWA-L11-1313-T01-A	1	2.45E+02			2.45E+02	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T02-A	1	5.40E+02			5.40E+02	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T03-A	1	8.60E+02			8.60E+02	2.8E+01	1.0E+00	3.2E+00	10	100	1.94E+03	108%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T04-A	1	6.46E+02			6.46E+02	6.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T05-A	1	1.19E+03			1.19E+03	1.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T06-A	1	1.31E+03			1.31E+03	1.1E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T07-A	1	1.39E+03			1.39E+03	1.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T08-A	1	7.89E+02			7.89E+02	1.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T09-A	1	7.52E+02			7.52E+02	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T01-B	1	2.34E+02			2.34E+02	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T02-B	1	5.54E+02			5.54E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T03-B	1	9.51E+02			9.51E+02	1.2E+00	1.0E+00	3.2E+00	10	100	1.93E+03	98%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T04-B	1	6.90E+02			6.90E+02	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T05-B	1	1.34E+03			1.34E+03	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T06-B	1	1.33E+03			1.33E+03	2.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T07-B	1	9.95E+02			9.95E+02	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T08-B	1	7.26E+02			7.26E+02	1.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T09-B	1	7.40E+02			7.40E+02	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T01-C	1	2.46E+02			2.46E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T02-C	1	5.00E+02			5.00E+02	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T03-C	1	9.75E+02			9.75E+02	8.1E-01	1.0E+00	3.2E+00	10	100	1.83E+03	85%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T04-C	1	6.82E+02			6.82E+02	5.4E-01	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T05-C	1	1.31E+03			1.31E+03	3.1E+00	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T06-C	1	1.15E+03			1.15E+03	2.0E+00	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T07-C	1	1.30E+03			1.30E+03	3.7E-01	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T08-C	1	7.16E+02			7.16E+02	1.9E+00	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-T09-C	1	7.98E+02			7.98E+02	6.0E-01	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.8E+02	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.7E+01	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	SWA-L11-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	3.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	5.6E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	9.8E+01	1.9E+00	6.0E+00	10	100	1.05E+03	105%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	6.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	5.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	6.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T07-A	1	9.50E-01	U1/2		9.50E-01	1.7E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T08-A	1	3.55E+01			3.55E+01	1.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T09-A	1	1.05E+02			1.05E+02	1.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	6.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	1.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	1.7E+02	1.9E+00	6.0E+00	10	100	1.03E+03	103%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	2.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T07-B	1	4.87E+00	E		4.87E+00	1.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T08-B	1	3.21E+01			3.21E+01	9.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T09-B	1	1.02E+02			1.02E+02	2.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	4.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	4.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00	10	100	1.06E+03	106%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	6.6E+01	1.9E+00	6.0E+00					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	1.7E+02	1.9E+00	6.0E+00					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	3.5E+02	1.9E+00	6.0E+00					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T07-C	1	9.50E-01	U1/2		9.50E-01	8.8E+01	1.9E+00	6.0E+00					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T08-C	1	3.08E+01			3.08E+01	5.3E+00	1.9E+00	6.0E+00					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-T09-C	1	1.08E+02			1.08E+02	6.3E-01	1.9E+00	6.0E+00					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	1.7E+02	1.9E+00	6.0E+00					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	1.8E+01	1.9E+00	6.0E+00					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	SWA-L11-1313-T01-A	1	1.10E+00	U1/2		1.10E+00	1.4E+02	2.2E+00	7.0E+00			---		VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T02-A	1	1.10E+00	U1/2		1.10E+00	2.2E+02	2.2E+00	7.0E+00			---		VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	1.2E+02	2.2E+00	7.0E+00	10	100	9.18E+02	92%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T04-A	1	1.10E+00	U1/2		1.10E+00	2.7E+02	2.2E+00	7.0E+00			---		VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T05-A	1	1.10E+00	U1/2		1.10E+00	2.4E+02	2.2E+00	7.0E+00			---		VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T06-A	1	1.10E+00	U1/2		1.10E+00	3.5E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T07-A	1	8.23E+00			8.23E+00	6.1E+00	2.2E+00	7.0E+00			---		VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T08-A	1	1.23E+01			1.23E+01	1.8E+00	2.2E+00	7.0E+00			---		VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T09-A	1	2.65E+01			2.65E+01	5.7E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T01-B	1	1.10E+00	U1/2		1.10E+00	4.1E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T02-B	1	1.10E+00	U1/2		1.10E+00	7.8E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	4.1E+02	2.2E+00	7.0E+00	10	100	9.73E+02	97%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T04-B	1	1.10E+00	U1/2		1.10E+00	7.4E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T05-B	1	1.10E+00	U1/2		1.10E+00	6.8E+00	2.2E+00	7.0E+00			---		VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T06-B	1	1.10E+00	U1/2		1.10E+00	1.3E+02	2.2E+00	7.0E+00			---		VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T07-B	1	1.02E+01			1.02E+01	2.1E+00	2.2E+00	7.0E+00			---		VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T08-B	1	1.28E+01			1.28E+01	2.5E+02	2.2E+00	7.0E+00			---		VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T09-B	1	2.68E+01			2.68E+01	7.2E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T01-C	1	1.10E+00	U1/2		1.10E+00	4.1E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T02-C	1	1.10E+00	U1/2		1.10E+00	1.6E+02	2.2E+00	7.0E+00			---		VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	4.8E+01	2.2E+00	7.0E+00	10	100	1.02E+03	102%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T04-C	1	1.10E+00	U1/2		1.10E+00	7.6E+01	2.2E+00	7.0E+00					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T05-C	1	1.10E+00	U1/2		1.10E+00	5.1E+01	2.2E+00	7.0E+00					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T06-C	1	1.10E+00	U1/2		1.10E+00	1.5E+02	2.2E+00	7.0E+00					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T07-C	1	1.16E+01			1.16E+01	2.1E+00	2.2E+00	7.0E+00					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T08-C	1	1.23E+01			1.23E+01	3.6E+00	2.2E+00	7.0E+00					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-T09-C	1	2.84E+01			2.84E+01	7.9E-01	2.2E+00	7.0E+00					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	4.1E+01	2.2E+00	7.0E+00					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	8.4E+02	2.2E+00	7.0E+00					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	SWA-L11-1313-T01-A	1	1.53E+04			1.53E+04	4.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T02-A	1	2.68E+05			2.68E+05	5.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T03-A	1	1.65E+06			1.65E+06	4.4E+01	2.6E+00	8.3E+00	1000	100	1.65E+06	85%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T04-A	1	3.64E+06			3.64E+06	7.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T05-A	1	7.07E+06			7.07E+06	7.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T06-A	1	6.88E+06			6.88E+06	1.3E+02	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T07-A	1	6.32E+06			6.32E+06	4.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T08-A	1	4.11E+06			4.11E+06	3.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T09-A	1	3.08E+06			3.08E+06	1.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T01-B	1	1.54E+04			1.54E+04	3.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T02-B	1	3.07E+05			3.07E+05	1.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T03-B	1	2.12E+06			2.12E+06	6.3E-01	2.6E+00	8.3E+00	1000	100	2.13E+06	82%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T04-B	1	3.88E+06			3.88E+06	9.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T05-B	1	6.76E+06			6.76E+06	8.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T06-B	1	7.08E+06			7.08E+06	3.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T07-B	1	4.72E+06			4.72E+06	1.8E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T08-B	1	4.16E+06			4.16E+06	1.2E+02	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T09-B	1	3.23E+06			3.23E+06	3.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T01-C	1	1.56E+04			1.56E+04	9.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T02-C	1	5.34E+04			5.34E+04	4.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T03-C	1	2.46E+06			2.46E+06	8.0E-01	2.6E+00	8.3E+00	1000	100	2.46E+06	82%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T04-C	1	3.85E+06			3.85E+06	1.1E+00	2.6E+00	8.3E+00					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T05-C	1	6.99E+06			6.99E+06	2.9E+00	2.6E+00	8.3E+00					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T06-C	1	7.25E+06			7.25E+06	3.2E-01	2.6E+00	8.3E+00					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T07-C	1	6.05E+06			6.05E+06	7.3E-01	2.6E+00	8.3E+00					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T08-C	1	4.27E+06			4.27E+06	5.4E+00	2.6E+00	8.3E+00					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-T09-C	1	3.04E+06			3.04E+06	2.2E-01	2.6E+00	8.3E+00					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-B01-A	1	1.06E+02			1.06E+02	1.4E+02	2.6E+00	8.3E+00					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1313-B02-A	1	8.93E+01			8.93E+01	6.5E+00	2.6E+00	8.3E+00					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	SWA-L11-1313-T01-A	1	5.41E+02			5.41E+02	5.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T02-A	1	1.05E+01			1.05E+01	2.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T03-A	1	2.30E+00	E		2.30E+00	5.0E+01	1.2E+00	3.8E+00	10	100	1.02E+03	102%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T04-A	1	8.81E+00			8.81E+00	7.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T05-A	1	6.00E-01	U1/2		6.00E-01	5.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T06-A	1	6.00E-01	U1/2		6.00E-01	5.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T07-A	1	9.61E+01			9.61E+01	5.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T08-A	1	3.42E+03			3.42E+03	6.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T09-A	1	1.58E+04			1.58E+04	7.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T01-B	1	6.08E+02			6.08E+02	4.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T02-B	1	1.04E+01			1.04E+01	6.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T03-B	1	4.34E+00			4.34E+00	3.6E+00	1.2E+00	3.8E+00	10	100	1.04E+03	103%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T04-B	1	9.53E+00			9.53E+00	1.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T05-B	1	1.48E+00	E		1.48E+00	1.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T06-B	1	6.00E-01	U1/2		6.00E-01	3.6E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T07-B	1	7.66E+02			7.66E+02	1.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T08-B	1	3.22E+03			3.22E+03	8.8E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T09-B	1	1.57E+04			1.57E+04	7.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T01-C	1	5.91E+02			5.91E+02	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T02-C	1	4.68E+01			4.68E+01	2.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T03-C	1	3.28E+00	E		3.28E+00	1.3E+01	1.2E+00	3.8E+00	10	100	1.14E+03	114%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T04-C	1	6.32E+00			6.32E+00	1.1E+01	1.2E+00	3.8E+00					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T05-C	1	6.00E-01	U1/2		6.00E-01	2.5E+03	1.2E+00	3.8E+00					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T06-C	1	6.00E-01	U1/2		6.00E-01	1.1E+02	1.2E+00	3.8E+00					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T07-C	1	9.75E+01			9.75E+01	7.1E-01	1.2E+00	3.8E+00					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T08-C	1	3.15E+03			3.15E+03	2.6E+00	1.2E+00	3.8E+00					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-T09-C	1	1.57E+04			1.57E+04	5.4E-01	1.2E+00	3.8E+00					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	2.6E+02	1.2E+00	3.8E+00					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
Cr	SWA-L11-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	1.2E+02	1.2E+00	3.8E+00					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	SWA-L11-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	1.7E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	1.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T03-A	1	2.31E+00	E		2.31E+00	7.4E+01	1.8E+00	5.7E+00	10	100	1.05E+03	104%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T04-A	1	2.63E+00	E		2.63E+00	2.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T05-A	1	8.83E+01			8.83E+01	9.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T06-A	1	1.09E+02			1.09E+02	1.9E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T07-A	1	1.29E+02			1.29E+02	1.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T08-A	1	1.21E+02			1.21E+02	3.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T09-A	1	1.64E+02			1.64E+02	4.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	5.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	4.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T03-B	1	2.13E+00	E		2.13E+00	6.8E+00	1.8E+00	5.7E+00	10	100	1.02E+03	102%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T04-B	1	1.92E+00	E		1.92E+00	2.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T05-B	1	1.62E+02			1.62E+02	1.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T06-B	1	1.22E+02			1.22E+02	1.9E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T07-B	1	1.30E+02			1.30E+02	2.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T08-B	1	1.15E+02			1.15E+02	1.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T09-B	1	1.68E+02			1.68E+02	1.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	7.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	4.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T03-C	1	2.31E+00	E		2.31E+00	3.1E+01	1.8E+00	5.7E+00	10	100	1.07E+03	107%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T04-C	1	2.14E+00	E		2.14E+00	3.8E+00	1.8E+00	5.7E+00					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T05-C	1	1.26E+02			1.26E+02	5.3E+00	1.8E+00	5.7E+00					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T06-C	1	7.09E+01			7.09E+01	5.3E-01	1.8E+00	5.7E+00					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T07-C	1	1.56E+02			1.56E+02	1.8E-01	1.8E+00	5.7E+00					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T08-C	1	1.16E+02			1.16E+02	2.8E+00	1.8E+00	5.7E+00					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-T09-C	1	1.66E+02			1.66E+02	5.9E-01	1.8E+00	5.7E+00					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	2.7E+02	1.8E+00	5.7E+00					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	SWA-L11-1313-T01-A	1	1.85E+00	U1/2		1.85E+00	1.1E+04	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T02-A	1	1.85E+00	U1/2		1.85E+00	6.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T03-A	1	6.83E+00	E		6.83E+00	1.5E+01	3.7E+00	1.2E+01	10	100	1.04E+03	103%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T04-A	1	1.12E+01	E		1.12E+01	1.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T05-A	1	1.93E+01			1.93E+01	7.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T06-A	1	1.62E+01			1.62E+01	3.3E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T07-A	1	1.12E+01	E		1.12E+01	1.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T08-A	1	3.38E+01			3.38E+01	4.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T09-A	1	9.86E+02			9.86E+02	8.8E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T01-B	1	1.85E+00	U1/2		1.85E+00	6.8E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T02-B	1	1.85E+00	U1/2		1.85E+00	4.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T03-B	1	7.32E+00	E		7.32E+00	4.0E+01	3.7E+00	1.2E+01	10	100	1.03E+03	102%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T04-B	1	8.77E+00	E		8.77E+00	2.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T05-B	1	1.76E+01			1.76E+01	7.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T06-B	1	1.54E+01			1.54E+01	9.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T07-B	1	1.14E+01	E		1.14E+01	8.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T08-B	1	3.79E+01			3.79E+01	2.7E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T09-B	1	9.15E+02			9.15E+02	1.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T01-C	1	1.85E+00	U1/2		1.85E+00	6.8E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T02-C	1	1.85E+00	U1/2		1.85E+00	3.8E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T03-C	1	5.84E+00	E		5.84E+00	2.3E+01	3.7E+00	1.2E+01	10	100	1.03E+03	102%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T04-C	1	7.09E+00	E		7.09E+00	1.1E+01	3.7E+00	1.2E+01					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T05-C	1	1.27E+01			1.27E+01	1.6E+01	3.7E+00	1.2E+01					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T06-C	1	1.19E+01			1.19E+01	1.2E+01	3.7E+00	1.2E+01					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T07-C	1	1.25E+01			1.25E+01	1.6E+01	3.7E+00	1.2E+01					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T08-C	1	4.05E+01			4.05E+01	2.5E+00	3.7E+00	1.2E+01					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-T09-C	1	1.07E+03			1.07E+03	2.4E-01	3.7E+00	1.2E+01					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	1.0E+02	3.7E+00	1.2E+01					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	1.8E+02	3.7E+00	1.2E+01					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	SWA-L11-1313-T01-A	1	7.30E+01			7.30E+01	8.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T02-A	1	1.73E+01			1.73E+01	8.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T03-A	1	6.61E+00			6.61E+00	4.0E+01	2.0E+00	6.4E+00	1000	100	9.77E+02	97%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T04-A	1	1.86E+01			1.86E+01	8.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T05-A	1	1.48E+01			1.48E+01	3.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T06-A	1	1.26E+01			1.26E+01	6.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T07-A	1	6.93E+04			6.93E+04	4.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T08-A	1	8.08E+04			8.08E+04	7.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T09-A	1	1.09E+05			1.09E+05	2.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T01-B	1	6.65E+01			6.65E+01	1.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T02-B	1	1.25E+01			1.25E+01	3.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T03-B	1	1.07E+01			1.07E+01	4.3E+00	2.0E+00	6.4E+00	1000	100	9.67E+02	96%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T04-B	1	1.59E+01			1.59E+01	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T05-B	1	3.33E+02			3.33E+02	8.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T06-B	1	3.33E+03			3.33E+03	2.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T07-B	1	8.57E+04			8.57E+04	1.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T08-B	1	7.82E+04			7.82E+04	9.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T09-B	1	1.15E+05			1.15E+05	8.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T01-C	1	8.09E+01			8.09E+01	4.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T02-C	1	4.11E+01			4.11E+01	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T03-C	1	1.06E+01			1.06E+01	5.0E+00	2.0E+00	6.4E+00	1000	100	9.90E+02	98%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T04-C	1	1.81E+01			1.81E+01	2.6E+00	2.0E+00	6.4E+00					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T05-C	1	8.29E+03			8.29E+03	1.8E+00	2.0E+00	6.4E+00					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T06-C	1	3.67E+01			3.67E+01	3.8E+00	2.0E+00	6.4E+00					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T07-C	1	9.79E+04			9.79E+04	1.6E-01	2.0E+00	6.4E+00					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T08-C	1	7.89E+04			7.89E+04	9.3E-01	2.0E+00	6.4E+00					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-T09-C	1	1.10E+05			1.10E+05	6.9E+00	2.0E+00	6.4E+00					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	2.5E+02	2.0E+00	6.4E+00					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1313-B02-A	1	1.11E+01			1.11E+01	2.3E+00	2.0E+00	6.4E+00					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	SWA-L11-1313-T01-A	1	1.57E+01	E		1.57E+01	3.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T02-A	1	3.40E+00	U1/2		3.40E+00	8.7E+02	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T03-A	1	3.40E+00	U1/2		3.40E+00	8.5E+01	6.8E+00	2.2E+01	10	100	1.02E+03	102%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T04-A	1	3.40E+00	U1/2		3.40E+00	4.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T05-A	1	3.40E+00	U1/2		3.40E+00	1.0E+02	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T06-A	1	3.40E+00	U1/2		3.40E+00	2.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T07-A	1	3.40E+00	U1/2		3.40E+00	7.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T08-A	1	1.47E+02			1.47E+02	4.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T09-A	1	2.40E+03			2.40E+03	1.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T01-B	1	1.14E+01	E		1.14E+01	3.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T02-B	1	3.40E+00	U1/2		3.40E+00	1.4E+02	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T03-B	1	3.40E+00	U1/2		3.40E+00	3.1E+02	6.8E+00	2.2E+01	10	100	1.02E+03	102%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T04-B	1	3.40E+00	U1/2		3.40E+00	8.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T05-B	1	3.40E+00	U1/2		3.40E+00	1.1E+02	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T06-B	1	3.40E+00	U1/2		3.40E+00	4.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T07-B	1	8.05E+00	E		8.05E+00	1.7E+02	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T08-B	1	1.56E+02			1.56E+02	2.7E+02	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T09-B	1	2.30E+03			2.30E+03	3.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T01-C	1	1.77E+01	E		1.77E+01	1.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T02-C	1	6.99E+00	E		6.99E+00	6.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T03-C	1	3.40E+00	U1/2		3.40E+00	2.4E+02	6.8E+00	2.2E+01	10	100	1.08E+03	108%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T04-C	1	3.40E+00	U1/2		3.40E+00	8.0E+02	6.8E+00	2.2E+01					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T05-C	1	3.40E+00	U1/2		3.40E+00	4.0E+01	6.8E+00	2.2E+01					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T06-C	1	3.40E+00	U1/2		3.40E+00	3.8E+01	6.8E+00	2.2E+01					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T07-C	1	3.40E+00	U1/2		3.40E+00	4.4E+02	6.8E+00	2.2E+01					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T08-C	1	1.69E+02			1.69E+02	2.1E+00	6.8E+00	2.2E+01					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-T09-C	1	2.56E+03			2.56E+03	8.3E-02	6.8E+00	2.2E+01					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	3.0E+01	6.8E+00	2.2E+01					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	3.3E+01	6.8E+00	2.2E+01					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	SWA-L11-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	9.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T02-A	1	2.09E+01			2.09E+01	1.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T03-A	1	9.25E+01			9.25E+01	3.6E+01	1.9E+00	6.0E+00	10	100	9.46E+02	85%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T04-A	1	3.22E+02			3.22E+02	8.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T05-A	1	8.32E+02			8.32E+02	4.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T06-A	1	8.15E+02			8.15E+02	9.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T07-A	1	8.13E+02			8.13E+02	5.9E-01	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T08-A	1	5.61E+02			5.61E+02	3.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T09-A	1	6.24E+02			6.24E+02	4.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	9.9E-01	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T02-B	1	2.40E+01			2.40E+01	3.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T03-B	1	1.30E+02			1.30E+02	5.6E+00	1.9E+00	6.0E+00	10	100	9.80E+02	85%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T04-B	1	3.34E+02			3.34E+02	8.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T05-B	1	8.06E+02			8.06E+02	1.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T06-B	1	8.55E+02			8.55E+02	2.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T07-B	1	6.09E+02			6.09E+02	3.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T08-B	1	5.75E+02			5.75E+02	2.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T09-B	1	5.80E+02			5.80E+02	4.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	7.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T02-C	1	5.60E+00	E		5.60E+00	3.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T03-C	1	1.53E+02			1.53E+02	4.0E+00	1.9E+00	6.0E+00	10	100	9.89E+02	84%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T04-C	1	3.37E+02			3.37E+02	1.7E+00	1.9E+00	6.0E+00					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T05-C	1	8.25E+02			8.25E+02	7.0E+00	1.9E+00	6.0E+00					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T06-C	1	9.15E+02			9.15E+02	1.6E+00	1.9E+00	6.0E+00					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T07-C	1	7.64E+02			7.64E+02	7.7E-01	1.9E+00	6.0E+00					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T08-C	1	5.88E+02			5.88E+02	6.4E+00	1.9E+00	6.0E+00					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-T09-C	1	6.50E+02			6.50E+02	2.3E+00	1.9E+00	6.0E+00					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	6.6E-01	1.9E+00	6.0E+00					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
Li	SWA-L11-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	4.0E+00	1.9E+00	6.0E+00					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	SWA-L11-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	1.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	8.0E+01	2.0E+00	6.4E+00	10	100	1.04E+03	104%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T04-A	1	7.08E+01			7.08E+01	7.5E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T05-A	1	1.46E+04			1.46E+04	5.0E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T06-A	1	1.67E+04			1.67E+04	9.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T07-A	1	1.56E+04			1.56E+04	3.9E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T08-A	1	1.30E+04			1.30E+04	5.6E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T09-A	1	1.36E+04			1.36E+04	1.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	9.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	3.9E+01	2.0E+00	6.4E+00	10	100	1.07E+03	107%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T04-B	1	1.11E+01			1.11E+01	5.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T05-B	1	1.87E+04			1.87E+04	6.9E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T06-B	1	1.66E+04			1.66E+04	2.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T07-B	1	1.42E+04			1.42E+04	2.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T08-B	1	1.26E+04			1.26E+04	1.0E+02	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T09-B	1	1.32E+04			1.32E+04	1.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T01-C	1	2.41E+00	E		2.41E+00	1.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00	10	100	1.05E+03	105%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T04-C	1	7.85E+00			7.85E+00	2.9E+00	2.0E+00	6.4E+00					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T05-C	1	1.67E+04			1.67E+04	3.3E+00	2.0E+00	6.4E+00					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T06-C	1	1.45E+04			1.45E+04	2.7E+00	2.0E+00	6.4E+00					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T07-C	1	1.71E+04			1.71E+04	6.8E-01	2.0E+00	6.4E+00					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T08-C	1	1.26E+04			1.26E+04	2.8E+00	2.0E+00	6.4E+00					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-T09-C	1	1.35E+04			1.35E+04	4.4E-01	2.0E+00	6.4E+00					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	5.2E+00	2.0E+00	6.4E+00					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	SWA-L11-1313-T01-A	1	8.37E+00			8.37E+00	1.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T02-A	1	9.34E+01			9.34E+01	1.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T03-A	1	3.12E+03			3.12E+03	4.8E+01	1.0E+00	3.2E+00	1000	100	4.19E+03	107%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T04-A	1	4.24E+05			4.24E+05	8.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T05-A	1	1.05E+06			1.05E+06	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T06-A	1	1.04E+06			1.04E+06	1.1E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T07-A	1	9.51E+05			9.51E+05	9.6E-02	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T08-A	1	6.51E+05			6.51E+05	2.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T09-A	1	5.81E+05			5.81E+05	2.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T01-B	1	1.93E+01			1.93E+01	5.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T02-B	1	9.09E+01			9.09E+01	8.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T03-B	1	2.16E+03			2.16E+03	1.8E+00	1.0E+00	3.2E+00	1000	100	3.11E+03	95%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T04-B	1	4.47E+05			4.47E+05	8.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T05-B	1	1.01E+06			1.01E+06	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T06-B	1	1.04E+06			1.04E+06	2.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T07-B	1	7.23E+05			7.23E+05	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T08-B	1	6.45E+05			6.45E+05	1.5E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T09-B	1	5.71E+05			5.71E+05	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T01-C	1	3.56E+00			3.56E+00	6.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T02-C	1	3.03E+01			3.03E+01	2.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T03-C	1	7.30E+03			7.30E+03	3.8E-01	1.0E+00	3.2E+00	1000	100	8.30E+03	100%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T04-C	1	4.48E+05			4.48E+05	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T05-C	1	1.02E+06			1.02E+06	2.9E+00	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T06-C	1	1.11E+06			1.11E+06	2.1E+00	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T07-C	1	9.12E+05			9.12E+05	6.8E-01	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T08-C	1	6.48E+05			6.48E+05	1.6E+00	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-T09-C	1	5.90E+05			5.90E+05	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-B01-A	1	3.54E+01			3.54E+01	1.3E+02	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1313-B02-A	1	3.02E+01			3.02E+01	8.2E+00	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	SWA-L11-1313-T01-A	1	1.18E+02			1.18E+02	5.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T02-A	1	1.29E+02			1.29E+02	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T03-A	1	1.15E+02			1.15E+02	3.9E+01	1.2E+00	3.8E+00	10	100	1.16E+03	105%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T04-A	1	8.14E+01			8.14E+01	6.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T05-A	1	4.85E+01			4.85E+01	4.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T06-A	1	3.15E+01			3.15E+01	1.3E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T07-A	1	9.59E+00			9.59E+00	1.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T08-A	1	4.50E+00			4.50E+00	2.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T09-A	1	5.12E+00			5.12E+00	1.0E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T01-B	1	1.12E+02			1.12E+02	8.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T02-B	1	1.19E+02			1.19E+02	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T03-B	1	1.22E+02			1.22E+02	2.4E-01	1.2E+00	3.8E+00	10	100	1.07E+03	94%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T04-B	1	8.78E+01			8.78E+01	3.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T05-B	1	1.99E+01			1.99E+01	1.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T06-B	1	3.30E+01			3.30E+01	9.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T07-B	1	9.29E+00			9.29E+00	9.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T08-B	1	4.81E+00			4.81E+00	2.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T09-B	1	5.46E+00			5.46E+00	2.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T01-C	1	1.12E+02			1.12E+02	1.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T02-C	1	1.26E+02			1.26E+02	1.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T03-C	1	1.13E+02			1.13E+02	3.3E-01	1.2E+00	3.8E+00	10	100	1.15E+03	104%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T04-C	1	8.86E+01			8.86E+01	1.7E+00	1.2E+00	3.8E+00					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T05-C	1	3.07E+01			3.07E+01	1.0E+01	1.2E+00	3.8E+00					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T06-C	1	5.43E+01			5.43E+01	4.5E+00	1.2E+00	3.8E+00					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T07-C	1	8.85E+00			8.85E+00	2.3E+01	1.2E+00	3.8E+00					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T08-C	1	5.70E+00			5.70E+00	1.9E+01	1.2E+00	3.8E+00					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-T09-C	1	4.30E+00			4.30E+00	2.8E+01	1.2E+00	3.8E+00					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	5.9E+01	1.2E+00	3.8E+00					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	7.6E+01	1.2E+00	3.8E+00					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	SWA-L11-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	1.0E+02	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T03-A	1	2.67E+00	E		2.67E+00	2.0E+02	1.8E+00	5.7E+00	10	100	1.05E+03	105%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T04-A	1	3.91E+00	E		3.91E+00	5.1E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T05-A	1	2.05E+02			2.05E+02	1.8E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T06-A	1	2.61E+02			2.61E+02	1.4E+03	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T07-A	1	3.01E+02			3.01E+02	2.8E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T08-A	1	2.56E+02			2.56E+02	7.2E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T09-A	1	2.94E+02			2.94E+02	8.3E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	9.5E+02	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	1.5E+03	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T03-B	1	2.51E+00	E		2.51E+00	1.3E+01	1.8E+00	5.7E+00	10	100	1.07E+03	107%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T04-B	1	3.54E+00	E		3.54E+00	3.7E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T05-B	1	3.54E+02			3.54E+02	4.8E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T06-B	1	2.85E+02			2.85E+02	3.1E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T07-B	1	2.75E+02			2.75E+02	1.8E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T08-B	1	2.59E+02			2.59E+02	1.5E+02	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T09-B	1	2.91E+02			2.91E+02	5.1E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	5.4E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	2.0E+02	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T03-C	1	2.01E+00	E		2.01E+00	7.4E+01	1.8E+00	5.7E+00	10	100	1.02E+03	102%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T04-C	1	6.40E+00			6.40E+00	2.2E+01	1.8E+00	5.7E+00					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T05-C	1	2.96E+02			2.96E+02	3.2E+00	1.8E+00	5.7E+00					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T06-C	1	1.68E+02			1.68E+02	8.2E-01	1.8E+00	5.7E+00					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T07-C	1	3.37E+02			3.37E+02	5.8E-01	1.8E+00	5.7E+00					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T08-C	1	2.58E+02			2.58E+02	2.7E+00	1.8E+00	5.7E+00					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-T09-C	1	2.99E+02			2.99E+02	4.9E-01	1.8E+00	5.7E+00					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	8.6E+00	1.8E+00	5.7E+00					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	3.4E+01	1.8E+00	5.7E+00					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	SWA-L11-1313-T01-A	1	2.96E+01			2.96E+01	1.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T02-A	1	6.38E+00	E		6.38E+00	1.1E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T03-A	1	4.63E+00	E		4.63E+00	1.4E+03	3.7E+00	1.2E+01	1000	100	1.15E+03	114%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T04-A	1	1.61E+01			1.61E+01	1.2E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T05-A	1	2.14E+01			2.14E+01	1.4E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T06-A	1	1.75E+01			1.75E+01	1.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T07-A	1	2.10E+01			2.10E+01	3.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T08-A	1	2.10E+02			2.10E+02	5.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T09-A	1	1.53E+03			1.53E+03	4.0E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T01-B	1	2.42E+01			2.42E+01	7.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T02-B	1	1.98E+01			1.98E+01	2.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T03-B	1	4.13E+00	E		4.13E+00	3.4E+02	3.7E+00	1.2E+01	1000	100	1.10E+03	110%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T04-B	1	1.34E+01			1.34E+01	6.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T05-B	1	1.52E+01			1.52E+01	1.6E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T06-B	1	2.29E+01			2.29E+01	1.1E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T07-B	1	5.84E+01			5.84E+01	2.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T08-B	1	2.53E+02			2.53E+02	3.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T09-B	1	4.31E+03			4.31E+03	1.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T01-C	1	2.66E+01			2.66E+01	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T02-C	1	2.36E+01			2.36E+01	1.4E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T03-C	1	5.04E+00	E		5.04E+00	4.0E+05	3.7E+00	1.2E+01	1000	100	1.07E+03	106%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T04-C	1	1.53E+01			1.53E+01	1.3E+04	3.7E+00	1.2E+01					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T05-C	1	2.72E+01			2.72E+01	1.9E+02	3.7E+00	1.2E+01					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T06-C	1	1.35E+01			1.35E+01	1.9E+02	3.7E+00	1.2E+01					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T07-C	1	1.99E+01			1.99E+01	2.0E+01	3.7E+00	1.2E+01					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T08-C	1	2.71E+02			2.71E+02	5.1E+00	3.7E+00	1.2E+01					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-T09-C	1	1.47E+03			1.47E+03	5.7E-01	3.7E+00	1.2E+01					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	6.1E+01	3.7E+00	1.2E+01					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	1.5E+02	3.7E+00	1.2E+01					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	SWA-L11-1313-T01-A	1	3.19E+05			3.19E+05	7.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T02-A	1	3.71E+05			3.71E+05	3.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T03-A	1	4.05E+05			4.05E+05	3.9E+01	1.6E+00	5.1E+00	1000	100	4.05E+05	84%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T04-A	1	3.82E+05			3.82E+05	7.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T05-A	1	4.55E+05			4.55E+05	3.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T06-A	1	4.47E+05			4.47E+05	1.3E+02	1.6E+00	5.1E+00				---	VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T07-A	1	3.68E+05			3.68E+05	2.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T08-A	1	2.35E+05			2.35E+05	3.6E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T09-A	1	2.94E+05			2.94E+05	2.9E+01	1.6E+00	5.1E+00				---	VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T01-B	1	3.15E+05			3.15E+05	3.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T02-B	1	3.61E+05			3.61E+05	6.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T03-B	1	4.19E+05			4.19E+05	2.7E+00	1.6E+00	5.1E+00	1000	100	4.20E+05	92%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T04-B	1	4.10E+05			4.10E+05	1.5E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T05-B	1	4.34E+05			4.34E+05	6.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T06-B	1	4.50E+05			4.50E+05	5.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T07-B	1	2.76E+05			2.76E+05	2.4E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T08-B	1	2.46E+05			2.46E+05	1.2E+02	1.6E+00	5.1E+00				---	VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T09-B	1	2.90E+05			2.90E+05	1.2E+01	1.6E+00	5.1E+00				---	VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T01-C	1	3.16E+05			3.16E+05	1.7E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T02-C	1	3.45E+05			3.45E+05	7.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T03-C	1	4.12E+05			4.12E+05	1.2E+00	1.6E+00	5.1E+00	1000	100	4.13E+05	88%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T04-C	1	4.05E+05			4.05E+05	8.8E-01	1.6E+00	5.1E+00					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T05-C	1	4.47E+05			4.47E+05	4.8E+00	1.6E+00	5.1E+00					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T06-C	1	4.52E+05			4.52E+05	1.6E+00	1.6E+00	5.1E+00					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T07-C	1	3.51E+05			3.51E+05	1.5E+00	1.6E+00	5.1E+00					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T08-C	1	2.68E+05			2.68E+05	2.5E+01	1.6E+00	5.1E+00					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-T09-C	1	3.24E+05			3.24E+05	2.4E+01	1.6E+00	5.1E+00					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-B01-A	1	1.13E+02			1.13E+02	1.0E+02	1.6E+00	5.1E+00					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1313-B02-A	1	6.32E+01			6.32E+01	1.5E+00	1.6E+00	5.1E+00					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	SWA-L11-1313-T01-A	1	8.45E+04			8.45E+04	4.4E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T02-A	1	8.48E+04			8.48E+04	8.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T03-A	1	8.38E+04			8.38E+04	3.9E+01	1.5E+01	4.8E+01	10	100	8.48E+04	92%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T04-A	1	7.33E+04			7.33E+04	7.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T05-A	1	9.66E+04			9.66E+04	1.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T06-A	1	8.70E+04			8.70E+04	1.3E+02	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T07-A	1	7.48E+04			7.48E+04	3.3E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T08-A	1	4.19E+04			4.19E+04	5.2E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T09-A	1	2.77E+04			2.77E+04	3.9E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T01-B	1	8.08E+04			8.08E+04	5.1E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T02-B	1	7.93E+04			7.93E+04	1.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T03-B	1	8.88E+04			8.88E+04	9.4E-01	1.5E+01	4.8E+01	10	100	8.97E+04	90%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T04-B	1	7.86E+04			7.86E+04	9.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T05-B	1	8.63E+04			8.63E+04	4.3E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T06-B	1	9.20E+04			9.20E+04	3.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T07-B	1	5.47E+04			5.47E+04	2.0E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T08-B	1	4.13E+04			4.13E+04	1.2E+02	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T09-B	1	2.57E+04			2.57E+04	1.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T01-C	1	8.13E+04			8.13E+04	4.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T02-C	1	8.27E+04			8.27E+04	2.2E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T03-C	1	8.52E+04			8.52E+04	8.5E-01	1.5E+01	4.8E+01	10	100	8.60E+04	86%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T04-C	1	7.75E+04			7.75E+04	2.1E-01	1.5E+01	4.8E+01					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T05-C	1	9.30E+04			9.30E+04	4.3E+00	1.5E+01	4.8E+01					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T06-C	1	9.97E+04			9.97E+04	1.4E+00	1.5E+01	4.8E+01					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T07-C	1	6.94E+04			6.94E+04	8.6E-02	1.5E+01	4.8E+01					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T08-C	1	4.09E+04			4.09E+04	3.2E+00	1.5E+01	4.8E+01					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-T09-C	1	2.84E+04			2.84E+04	2.2E-01	1.5E+01	4.8E+01					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-B01-A	1	7.50E+00	U1/2		7.50E+00	1.7E+02	1.5E+01	4.8E+01					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1313-B02-A	1	7.50E+00	U1/2		7.50E+00	2.0E+01	1.5E+01	4.8E+01					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	SWA-L11-1313-T01-A	1	2.34E+04			2.34E+04	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T02-A	1	1.50E+04			1.50E+04	7.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T03-A	1	5.01E+03			5.01E+03	2.3E+01	1.1E+00	3.5E+00	1000	100	6.10E+03	110%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T04-A	1	3.63E+03			3.63E+03	7.6E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T05-A	1	7.21E+03			7.21E+03	3.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T06-A	1	8.56E+03			8.56E+03	1.4E+02	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T07-A	1	1.08E+04			1.08E+04	5.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T08-A	1	2.53E+04			2.53E+04	8.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T09-A	1	1.01E+05			1.01E+05	2.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T01-B	1	2.26E+04			2.26E+04	6.6E-02	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T02-B	1	1.49E+04			1.49E+04	1.7E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T03-B	1	6.70E+03			6.70E+03	1.2E+00	1.1E+00	3.5E+00	1000	100	7.82E+03	112%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T04-B	1	3.83E+03			3.83E+03	5.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T05-B	1	8.03E+03			8.03E+03	5.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T06-B	1	8.49E+03			8.49E+03	3.4E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T07-B	1	1.58E+04			1.58E+04	1.7E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T08-B	1	2.13E+04			2.13E+04	8.8E+01	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T09-B	1	2.88E+05			2.88E+05	4.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T01-C	1	2.30E+04			2.30E+04	8.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T02-C	1	1.86E+04			1.86E+04	1.6E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T03-C	1	5.96E+03			5.96E+03	6.1E-01	1.1E+00	3.5E+00	1000	100	6.96E+03	100%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T04-C	1	3.77E+03			3.77E+03	3.7E-01	1.1E+00	3.5E+00					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T05-C	1	9.36E+03			9.36E+03	4.5E+00	1.1E+00	3.5E+00					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T06-C	1	7.53E+03			7.53E+03	2.3E+00	1.1E+00	3.5E+00					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T07-C	1	1.34E+04			1.34E+04	3.1E-01	1.1E+00	3.5E+00					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T08-C	1	2.01E+04			2.01E+04	2.8E+00	1.1E+00	3.5E+00					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-T09-C	1	1.16E+05			1.16E+05	5.1E-01	1.1E+00	3.5E+00					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-B01-A	1	1.61E+00	E		1.61E+00	2.0E+02	1.1E+00	3.5E+00					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1313-B02-A	1	1.72E+01			1.72E+01	2.3E+01	1.1E+00	3.5E+00					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	SWA-L11-1313-T01-A	1	4.81E+05			4.81E+05	8.1E-02	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T02-A	1	5.09E+05			5.09E+05	2.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T03-A	1	5.10E+05			5.10E+05	1.5E+01	2.5E+00	8.0E+00	1000	100	5.11E+05	83%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T04-A	1	4.93E+05			4.93E+05	1.4E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T05-A	1	4.90E+05			4.90E+05	3.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T06-A	1	4.65E+05			4.65E+05	1.2E+02	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T07-A	1	4.84E+05			4.84E+05	7.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T08-A	1	4.80E+05			4.80E+05	2.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T09-A	1	4.69E+05			4.69E+05	8.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T01-B	1	4.69E+05			4.69E+05	1.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T02-B	1	5.01E+05			5.01E+05	6.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T03-B	1	5.05E+05			5.05E+05	3.6E-01	2.5E+00	8.0E+00	1000	100	5.06E+05	90%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T04-B	1	4.89E+05			4.89E+05	3.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T05-B	1	4.79E+05			4.79E+05	3.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T06-B	1	4.78E+05			4.78E+05	1.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T07-B	1	4.77E+05			4.77E+05	9.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T08-B	1	4.80E+05			4.80E+05	1.3E+02	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T09-B	1	4.38E+05			4.38E+05	5.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T01-C	1	4.66E+05			4.66E+05	5.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T02-C	1	4.82E+05			4.82E+05	3.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T03-C	1	5.04E+05			5.04E+05	5.2E-01	2.5E+00	8.0E+00	1000	100	5.05E+05	84%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T04-C	1	4.88E+05			4.88E+05	5.5E-01	2.5E+00	8.0E+00					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T05-C	1	4.85E+05			4.85E+05	7.9E-01	2.5E+00	8.0E+00					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T06-C	1	4.82E+05			4.82E+05	7.2E-01	2.5E+00	8.0E+00					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T07-C	1	4.82E+05			4.82E+05	3.5E-01	2.5E+00	8.0E+00					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T08-C	1	4.77E+05			4.77E+05	6.3E-01	2.5E+00	8.0E+00					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-T09-C	1	4.75E+05			4.75E+05	3.6E-01	2.5E+00	8.0E+00					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-B01-A	1	1.24E+02			1.24E+02	1.2E+02	2.5E+00	8.0E+00					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1313-B02-A	1	2.23E+02			2.23E+02	2.4E+00	2.5E+00	8.0E+00					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	SWA-L11-1313-T01-A	1	3.21E+02			3.21E+02	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T02-A	1	3.75E+03			3.75E+03	2.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T03-A	1	1.10E+04			1.10E+04	1.9E+01	1.0E+00	3.2E+00	1000	100	1.19E+04	95%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T04-A	1	1.73E+04			1.73E+04	8.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T05-A	1	3.34E+04			3.34E+04	6.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T06-A	1	3.25E+04			3.25E+04	9.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T07-A	1	3.16E+04			3.16E+04	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T08-A	1	2.03E+04			2.03E+04	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T09-A	1	1.77E+04			1.77E+04	1.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T01-B	1	3.22E+02			3.22E+02	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T02-B	1	4.03E+03			4.03E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T03-B	1	1.27E+04			1.27E+04	1.3E+00	1.0E+00	3.2E+00	1000	100	1.36E+04	96%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T04-B	1	1.85E+04			1.85E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T05-B	1	3.23E+04			3.23E+04	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T06-B	1	3.34E+04			3.34E+04	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T07-B	1	2.27E+04			2.27E+04	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T08-B	1	2.12E+04			2.12E+04	8.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T09-B	1	1.72E+04			1.72E+04	9.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T01-C	1	3.16E+02			3.16E+02	1.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T02-C	1	1.01E+03			1.01E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T03-C	1	1.37E+04			1.37E+04	2.0E+00	1.0E+00	3.2E+00	1000	100	1.47E+04	98%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T04-C	1	1.83E+04			1.83E+04	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T05-C	1	3.25E+04			3.25E+04	2.6E+00	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T06-C	1	3.34E+04			3.34E+04	1.1E-01	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T07-C	1	2.96E+04			2.96E+04	2.2E+00	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T08-C	1	2.05E+04			2.05E+04	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-T09-C	1	1.76E+04			1.76E+04	5.5E-01	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.6E+02	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.9E+02	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	SWA-L11-1313-T01-A	1	8.11E+05			8.11E+05	8.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T02-A	1	9.15E+05			9.15E+05	1.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T03-A	1	9.08E+05			9.08E+05	3.0E+01	6.8E+00	2.2E+01	1000	100	9.09E+05	89%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T04-A	1	7.53E+05			7.53E+05	9.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T05-A	1	6.42E+05			6.42E+05	8.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T06-A	1	6.40E+05			6.40E+05	9.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T07-A	1	3.19E+05			3.19E+05	2.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T08-A	1	1.86E+05			1.86E+05	7.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T09-A	1	1.32E+05			1.32E+05	3.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T01-B	1	7.71E+05			7.71E+05	1.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T02-B	1	8.98E+05			8.98E+05	1.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T03-B	1	9.02E+05			9.02E+05	1.5E+00	6.8E+00	2.2E+01	1000	100	9.03E+05	87%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T04-B	1	7.82E+05			7.82E+05	9.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T05-B	1	5.46E+05			5.46E+05	9.9E-02	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T06-B	1	5.14E+05			5.14E+05	3.3E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T07-B	1	2.32E+05			2.32E+05	1.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T08-B	1	1.81E+05			1.81E+05	1.3E+02	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T09-B	1	1.27E+05			1.27E+05	4.5E-02	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T01-C	1	7.69E+05			7.69E+05	1.3E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T02-C	1	8.09E+05			8.09E+05	1.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T03-C	1	8.82E+05			8.82E+05	1.5E+00	6.8E+00	2.2E+01	1000	100	8.83E+05	82%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T04-C	1	7.76E+05			7.76E+05	3.6E-01	6.8E+00	2.2E+01					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T05-C	1	5.81E+05			5.81E+05	3.3E+00	6.8E+00	2.2E+01					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T06-C	1	6.43E+05			6.43E+05	1.4E+00	6.8E+00	2.2E+01					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T07-C	1	2.99E+05			2.99E+05	3.3E-01	6.8E+00	2.2E+01					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T08-C	1	1.82E+05			1.82E+05	3.1E+00	6.8E+00	2.2E+01					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-T09-C	1	1.32E+05			1.32E+05	5.9E-01	6.8E+00	2.2E+01					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	1.3E+02	6.8E+00	2.2E+01					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	5.9E+00	6.8E+00	2.2E+01					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	SWA-L11-1313-T01-A	1	2.30E+00	U1/2		2.30E+00	4.4E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T02-A	1	2.30E+00	U1/2		2.30E+00	2.8E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T03-A	1	2.30E+00	U1/2		2.30E+00	4.7E+01	4.6E+00	1.5E+01	10	100	1.12E+03	112%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T04-A	1	2.30E+00	U1/2		2.30E+00	1.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T05-A	1	1.06E+01	E		1.06E+01	1.1E+02	4.6E+00	1.5E+01				---	VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T06-A	1	1.10E+01	E		1.10E+01	5.9E+00	4.6E+00	1.5E+01				---	VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T07-A	1	2.09E+01			2.09E+01	7.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T08-A	1	5.80E+00	E		5.80E+00	1.7E+02	4.6E+00	1.5E+01				---	VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T09-A	1	2.30E+00	U1/2		2.30E+00	6.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T01-B	1	2.30E+00	U1/2		2.30E+00	4.9E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T02-B	1	2.30E+00	U1/2		2.30E+00	4.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T03-B	1	2.30E+00	U1/2		2.30E+00	3.0E+01	4.6E+00	1.5E+01	10	100	1.14E+03	114%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T04-B	1	2.30E+00	U1/2		2.30E+00	1.9E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T05-B	1	5.85E+00	E		5.85E+00	1.4E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T06-B	1	1.17E+01	E		1.17E+01	1.9E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T07-B	1	1.85E+01			1.85E+01	4.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T08-B	1	6.40E+00	E		6.40E+00	1.9E+00	4.6E+00	1.5E+01				---	VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T09-B	1	2.30E+00	U1/2		2.30E+00	1.4E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T01-C	1	2.30E+00	U1/2		2.30E+00	5.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T02-C	1	2.30E+00	U1/2		2.30E+00	1.1E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T03-C	1	2.30E+00	U1/2		2.30E+00	8.7E+01	4.6E+00	1.5E+01	10	100	1.15E+03	115%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T04-C	1	2.30E+00	U1/2		2.30E+00	3.0E+01	4.6E+00	1.5E+01					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T05-C	1	1.29E+01	E		1.29E+01	4.8E+01	4.6E+00	1.5E+01					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T06-C	1	1.06E+01	E		1.06E+01	2.6E+01	4.6E+00	1.5E+01					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T07-C	1	2.21E+01			2.21E+01	8.6E+02	4.6E+00	1.5E+01					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T08-C	1	5.25E+00	E		5.25E+00	8.7E+01	4.6E+00	1.5E+01					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-T09-C	1	2.30E+00	U1/2		2.30E+00	3.7E+02	4.6E+00	1.5E+01					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	3.9E+00	4.6E+00	1.5E+01					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	6.7E+00	4.6E+00	1.5E+01					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	SWA-L11-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	5.0E+02	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	8.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	5.9E+01	2.0E+00	6.4E+00	10	100	9.63E+02	96%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	2.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	8.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T08-A	1	1.22E+01			1.22E+01	5.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T09-A	1	1.11E+03			1.11E+03	1.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	2.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	3.6E+00	2.0E+00	6.4E+00	10	100	9.98E+02	100%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	2.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	6.0E+02	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	1.5E+02	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	1.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T08-B	1	1.83E+01			1.83E+01	1.0E+02	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T09-B	1	6.33E+03			6.33E+03	2.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	3.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	2.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00	10	100	9.67E+02	97%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	5.7E+02	2.0E+00	6.4E+00					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	6.5E+01	2.0E+00	6.4E+00					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	3.6E+02	2.0E+00	6.4E+00					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T08-C	1	1.46E+01			1.46E+01	6.8E+00	2.0E+00	6.4E+00					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-T09-C	1	1.15E+03			1.15E+03	6.9E-01	2.0E+00	6.4E+00					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	4.8E+00	2.0E+00	6.4E+00					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	SWA-L11-1313-T01-A	1	2.95E+02			2.95E+02	9.4E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T02-A	1	1.27E+02			1.27E+02	8.6E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T03-A	1	8.44E+01			8.44E+01	1.9E+01	1.5E+00	4.8E+00	10	100	9.61E+02	88%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T04-A	1	1.29E+02			1.29E+02	5.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T05-A	1	1.44E+02			1.44E+02	5.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T06-A	1	1.35E+02			1.35E+02	9.4E+01	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T07-A	1	1.09E+02			1.09E+02	2.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T08-A	1	7.53E+01			7.53E+01	1.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T09-A	1	9.11E+02			9.11E+02	1.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T01-B	1	2.80E+02			2.80E+02	8.6E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T02-B	1	1.31E+02			1.31E+02	8.8E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T03-B	1	1.04E+02			1.04E+02	5.5E-01	1.5E+00	4.8E+00	10	100	1.05E+03	95%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T04-B	1	1.39E+02			1.39E+02	3.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T05-B	1	1.26E+02			1.26E+02	2.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T06-B	1	1.42E+02			1.42E+02	1.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T07-B	1	1.06E+02			1.06E+02	1.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T08-B	1	6.80E+01			6.80E+01	1.2E+02	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T09-B	1	1.02E+03			1.02E+03	7.0E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T01-C	1	2.82E+02			2.82E+02	1.1E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T02-C	1	1.34E+02			1.34E+02	3.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T03-C	1	1.08E+02			1.08E+02	1.8E+00	1.5E+00	4.8E+00	10	100	1.12E+03	102%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T04-C	1	1.35E+02			1.35E+02	2.3E+00	1.5E+00	4.8E+00					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T05-C	1	1.40E+02			1.40E+02	4.0E+00	1.5E+00	4.8E+00					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T06-C	1	1.49E+02			1.49E+02	5.4E-01	1.5E+00	4.8E+00					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T07-C	1	1.01E+02			1.01E+02	3.5E+00	1.5E+00	4.8E+00					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T08-C	1	6.43E+01			6.43E+01	5.8E+00	1.5E+00	4.8E+00					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-T09-C	1	1.01E+03			1.01E+03	6.2E-01	1.5E+00	4.8E+00					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-B01-A	1	7.50E-01	U1/2		7.50E-01	3.3E+01	1.5E+00	4.8E+00					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1313-B02-A	1	1.72E+00	E		1.72E+00	2.2E+01	1.5E+00	4.8E+00					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	SWA-L11-1313-T01-A	1	2.29E+00	E		2.29E+00	7.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:08 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T02-A	1	1.45E+00	E		1.45E+00	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:10 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T03-A	1	1.49E+00	E		1.49E+00	4.4E+01	1.0E+00	3.2E+00	10	100	9.91E+02	99%	VU ICP-OES	4/7/11 4:11 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T04-A	1	2.29E+00	E		2.29E+00	3.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:13 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T05-A	1	2.07E+01			2.07E+01	3.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:14 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T06-A	1	1.82E+01			1.82E+01	7.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:16 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T07-A	1	5.88E+02			5.88E+02	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:18 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T08-A	1	9.46E+02			9.46E+02	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:19 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T09-A	1	1.65E+03			1.65E+03	5.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:21 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T01-B	1	1.04E+00	E		1.04E+00	1.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:28 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T02-B	1	1.32E+00	E		1.32E+00	3.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:29 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T03-B	1	2.07E+00	E		2.07E+00	2.5E+01	1.0E+00	3.2E+00	10	100	1.02E+03	102%	VU ICP-OES	4/7/11 4:31 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T04-B	1	2.46E+00	E		2.46E+00	2.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:33 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T05-B	1	1.20E+01			1.20E+01	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:34 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T06-B	1	1.05E+02			1.05E+02	3.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:36 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T07-B	1	8.77E+02			8.77E+02	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:38 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T08-B	1	9.38E+02			9.38E+02	1.2E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:39 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T09-B	1	1.60E+03			1.60E+03	5.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:41 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T01-C	1	1.44E+00	E		1.44E+00	2.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:42 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T02-C	1	1.56E+00	E		1.56E+00	1.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 4:44 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T03-C	1	1.29E+00	E		1.29E+00	1.2E+01	1.0E+00	3.2E+00	10	100	1.10E+03	110%	VU ICP-OES	4/7/11 4:46 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T04-C	1	2.36E+00	E		2.36E+00	1.7E+01	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:47 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T05-C	1	1.62E+02			1.62E+02	3.6E+00	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:49 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T06-C	1	9.97E+00			9.97E+00	5.3E+00	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:51 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T07-C	1	9.00E+02			9.00E+02	6.5E-01	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:52 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T08-C	1	8.88E+02			8.88E+02	2.1E+00	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:54 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-T09-C	1	1.71E+03			1.71E+03	7.0E-01	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:56 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.0E+02	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 3:58 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.5E+01	1.0E+00	3.2E+00					VU ICP-OES	4/7/11 4:00 PM	EPA Interlab L11 1313-1316 SWA

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	SWA-LRef-1313-T01-A	1	5.51E+04			5.51E+04	6.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T02-A	1	2.65E+04			2.65E+04	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T03-A	1	2.04E+04			2.04E+04	8.5E-01	1.0E+00	3.2E+00	1000	100	2.12E+04	86%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T04-A	1	1.08E+02			1.08E+02	1.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T05-A	1	4.83E+01			4.83E+01	7.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T06-A	1	3.26E+00			3.26E+00	2.7E+02	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T07-A	1	4.62E+02			4.62E+02	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T08-A	1	2.57E+05			2.57E+05	8.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T09-A	1	3.76E+05			3.76E+05	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T01-B	1	6.08E+04			6.08E+04	3.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T02-B	1	3.47E+04			3.47E+04	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T03-B	1	2.35E+04			2.35E+04	4.1E-01	1.0E+00	3.2E+00	1000	100	2.44E+04	89%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T04-B	1	1.28E+02			1.28E+02	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T05-B	1	3.98E+01			3.98E+01	3.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T06-B	1	5.68E+00			5.68E+00	6.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T07-B	1	4.96E+02			4.96E+02	2.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T08-B	1	2.70E+05			2.70E+05	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T09-B	1	9.23E+05			9.23E+05	1.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T01-C	1	6.27E+04			6.27E+04	4.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T02-C	1	3.58E+04			3.58E+04	2.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T03-C	1	2.06E+04			2.06E+04	3.9E-01	1.0E+00	3.2E+00	1000	100	2.16E+04	105%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T04-C	1	1.61E+02			1.61E+02	8.5E+00	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T05-C	1	3.44E+01			3.44E+01	2.6E+01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T06-C	1	5.86E+00			5.86E+00	8.2E+01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T07-C	1	4.78E+01			4.78E+01	1.6E+01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T08-C	1	2.00E+05			2.00E+05	8.1E-01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T09-C	1	9.46E+05			9.46E+05	1.8E+00	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-B01-A	1	1.21E+00	E		1.21E+00	2.5E+01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-B02-A	1	9.15E+00			9.15E+00	3.4E+00	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-B03-A	1	4.11E+00			4.11E+00	1.0E+02	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	SWA-LRef-1313-T01-A	1	6.01E+03			6.01E+03	8.4E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T02-A	1	5.61E+03			5.61E+03	7.4E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T03-A	1	4.83E+03			4.83E+03	1.0E+00	7.5E+00	2.4E+01	10	100	5.82E+03	99%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T04-A	1	1.36E+03			1.36E+03	3.6E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T05-A	1	1.53E+03			1.53E+03	6.9E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T06-A	1	1.08E+03			1.08E+03	1.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T07-A	1	6.40E+02			6.40E+02	9.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T08-A	1	1.18E+03			1.18E+03	1.9E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T09-A	1	5.35E+02			5.35E+02	3.4E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T01-B	1	6.63E+03			6.63E+03	9.8E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T02-B	1	6.05E+03			6.05E+03	8.0E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T03-B	1	5.09E+03			5.09E+03	4.5E-01	7.5E+00	2.4E+01	10	100	6.13E+03	104%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T04-B	1	1.34E+03			1.34E+03	1.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T05-B	1	1.34E+03			1.34E+03	5.2E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T06-B	1	8.27E+02			8.27E+02	2.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T07-B	1	5.20E+02			5.20E+02	1.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T08-B	1	1.14E+03			1.14E+03	2.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T09-B	1	8.37E+02			8.37E+02	9.6E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T01-C	1	6.45E+03			6.45E+03	3.4E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T02-C	1	5.73E+03			5.73E+03	6.5E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T03-C	1	5.38E+03			5.38E+03	3.2E-01	7.5E+00	2.4E+01	10	100	6.33E+03	95%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T04-C	1	1.44E+03			1.44E+03	1.4E+00	7.5E+00	2.4E+01					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T05-C	1	1.03E+03			1.03E+03	2.5E+00	7.5E+00	2.4E+01					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T06-C	1	1.21E+03			1.21E+03	1.4E+00	7.5E+00	2.4E+01					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T07-C	1	5.74E+02			5.74E+02	2.1E+00	7.5E+00	2.4E+01					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T08-C	1	8.40E+02			8.40E+02	2.7E+00	7.5E+00	2.4E+01					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T09-C	1	7.39E+02			7.39E+02	7.6E+01	7.5E+00	2.4E+01					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-B01-A	1	3.75E+00	U1/2		3.75E+00	1.1E+02	7.5E+00	2.4E+01					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-B02-A	1	3.75E+00	U1/2		3.75E+00	1.5E+02	7.5E+00	2.4E+01					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-B03-A	1	3.75E+00	U1/2		3.75E+00	8.5E+01	7.5E+00	2.4E+01					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	SWA-LRef-1313-T01-A	1	1.02E+04			1.02E+04	5.1E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T02-A	1	4.22E+03			4.22E+03	3.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T03-A	1	2.29E+03			2.29E+03	8.0E-01	1.1E+01	3.5E+01	10	100	3.23E+03	94%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T04-A	1	2.49E+02			2.49E+02	2.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T05-A	1	2.89E+02			2.89E+02	5.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T06-A	1	1.60E+02			1.60E+02	1.5E+01	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T07-A	1	3.19E+02			3.19E+02	9.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T08-A	1	3.69E+03			3.69E+03	5.9E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T09-A	1	6.80E+03			6.80E+03	6.8E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T01-B	1	1.20E+04			1.20E+04	2.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T02-B	1	4.90E+03			4.90E+03	7.5E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T03-B	1	3.23E+03			3.23E+03	3.9E-01	1.1E+01	3.5E+01	10	100	4.08E+03	85%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T04-B	1	4.65E+02			4.65E+02	1.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T05-B	1	3.38E+02			3.38E+02	5.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T06-B	1	3.61E+02			3.61E+02	4.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T07-B	1	2.01E+02			2.01E+02	7.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T08-B	1	3.95E+03			3.95E+03	1.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T09-B	1	1.05E+04			1.05E+04	4.2E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T01-C	1	1.03E+04			1.03E+04	2.1E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T02-C	1	4.37E+03			4.37E+03	6.3E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T03-C	1	2.54E+03			2.54E+03	1.1E+00	1.1E+01	3.5E+01	10	100	3.63E+03	109%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T04-C	1	4.06E+02			4.06E+02	3.9E+00	1.1E+01	3.5E+01					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T05-C	1	3.72E+02			3.72E+02	5.5E+00	1.1E+01	3.5E+01					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T06-C	1	2.43E+02			2.43E+02	7.0E-01	1.1E+01	3.5E+01					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T07-C	1	1.86E+02			1.86E+02	1.1E+01	1.1E+01	3.5E+01					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T08-C	1	3.19E+03			3.19E+03	9.6E-01	1.1E+01	3.5E+01					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T09-C	1	1.40E+04			1.40E+04	5.6E+00	1.1E+01	3.5E+01					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-B01-A	1	5.50E+00	U1/2		5.50E+00	2.3E+02	1.1E+01	3.5E+01					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-B02-A	1	5.50E+00	U1/2		5.50E+00	4.1E+01	1.1E+01	3.5E+01					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-B03-A	1	5.50E+00	U1/2		5.50E+00	5.2E+01	1.1E+01	3.5E+01					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	SWA-LRef-1313-T01-A	1	1.23E+03			1.23E+03	7.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T02-A	1	1.00E+03			1.00E+03	9.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T03-A	1	8.97E+02			8.97E+02	1.9E+00	1.0E+00	3.2E+00	1000	100	1.87E+03	97%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T04-A	1	1.42E+03			1.42E+03	6.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T05-A	1	2.18E+03			2.18E+03	9.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T06-A	1	3.76E+03			3.76E+03	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T07-A	1	6.02E+03			6.02E+03	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T08-A	1	6.84E+03			6.84E+03	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T09-A	1	7.29E+03			7.29E+03	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T01-B	1	1.32E+03			1.32E+03	7.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T02-B	1	1.03E+03			1.03E+03	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T03-B	1	1.01E+03			1.01E+03	8.0E-01	1.0E+00	3.2E+00	1000	100	2.07E+03	106%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T04-B	1	1.80E+03			1.80E+03	8.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T05-B	1	2.65E+03			2.65E+03	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T06-B	1	5.27E+03			5.27E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T07-B	1	5.04E+03			5.04E+03	1.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T08-B	1	6.96E+03			6.96E+03	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T09-B	1	7.31E+03			7.31E+03	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T01-C	1	1.27E+03			1.27E+03	4.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T02-C	1	1.01E+03			1.01E+03	9.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T03-C	1	8.70E+02			8.70E+02	2.5E-01	1.0E+00	3.2E+00	1000	100	1.95E+03	108%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T04-C	1	1.65E+03			1.65E+03	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T05-C	1	2.96E+03			2.96E+03	5.2E-01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T06-C	1	3.41E+03			3.41E+03	3.7E-01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T07-C	1	5.99E+03			5.99E+03	3.8E-01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T08-C	1	7.07E+03			7.07E+03	7.9E-01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T09-C	1	7.42E+03			7.42E+03	2.6E+00	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-B01-A	1	1.79E+01			1.79E+01	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-B02-A	1	1.25E+01			1.25E+01	3.3E+00	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-B03-A	1	3.05E+01			3.05E+01	4.4E+00	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	SWA-LRef-1313-T01-A	1	4.35E+01			4.35E+01	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T02-A	1	1.43E+02			1.43E+02	4.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T03-A	1	1.81E+02			1.81E+02	7.9E-01	1.0E+00	3.2E+00	10	100	1.20E+03	102%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T04-A	1	1.12E+03			1.12E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T05-A	1	9.81E+02			9.81E+02	8.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T06-A	1	1.51E+03			1.51E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T07-A	1	1.84E+03			1.84E+03	8.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T08-A	1	8.52E+02			8.52E+02	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T09-A	1	9.29E+02			9.29E+02	8.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T01-B	1	1.85E+02			1.85E+02	5.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T02-B	1	1.59E+02			1.59E+02	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T03-B	1	1.66E+02			1.66E+02	6.1E-01	1.0E+00	3.2E+00	10	100	1.19E+03	102%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T04-B	1	1.05E+03			1.05E+03	3.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T05-B	1	1.15E+03			1.15E+03	9.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T06-B	1	1.55E+03			1.55E+03	9.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T07-B	1	1.56E+03			1.56E+03	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T08-B	1	8.45E+02			8.45E+02	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T09-B	1	9.27E+02			9.27E+02	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T01-C	1	2.33E+02			2.33E+02	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T02-C	1	1.65E+02			1.65E+02	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T03-C	1	1.89E+02			1.89E+02	2.9E-01	1.0E+00	3.2E+00	10	100	1.22E+03	103%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T04-C	1	1.00E+03			1.00E+03	9.6E-01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T05-C	1	1.24E+03			1.24E+03	2.4E-01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T06-C	1	1.14E+03			1.14E+03	7.4E-01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T07-C	1	1.75E+03			1.75E+03	2.4E-01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T08-C	1	9.68E+02			9.68E+02	4.4E-01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T09-C	1	9.54E+02			9.54E+02	5.7E+00	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	6.3E+00	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-B02-A	1	1.87E+00	E		1.87E+00	2.1E+00	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	3.9E+01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	SWA-LRef-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	8.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	2.0E+03	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	5.2E+02	1.9E+00	6.0E+00	10	100	1.08E+03	108%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	1.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	2.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	2.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T07-A	1	9.50E-01	U1/2		9.50E-01	1.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T08-A	1	2.42E+01			2.42E+01	1.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T09-A	1	1.39E+02			1.39E+02	1.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	2.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	8.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	1.3E+03	1.9E+00	6.0E+00	10	100	1.08E+03	108%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	1.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	8.6E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T07-B	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T08-B	1	3.05E+01			3.05E+01	5.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T09-B	1	1.49E+02			1.49E+02	7.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	8.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	2.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	1.6E+04	1.9E+00	6.0E+00	10	100	1.09E+03	109%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	3.5E+02	1.9E+00	6.0E+00					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	3.6E+02	1.9E+00	6.0E+00					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T07-C	1	9.50E-01	U1/2		9.50E-01	8.6E+01	1.9E+00	6.0E+00					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T08-C	1	1.01E+01			1.01E+01	7.6E+00	1.9E+00	6.0E+00					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T09-C	1	1.53E+02			1.53E+02	4.6E+00	1.9E+00	6.0E+00					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	8.7E+02	1.9E+00	6.0E+00					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	4.5E+02	1.9E+00	6.0E+00					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	1.0E+02	1.9E+00	6.0E+00					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	SWA-LRef-1313-T01-A	1	1.10E+00	U1/2		1.10E+00	4.3E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T02-A	1	1.10E+00	U1/2		1.10E+00	1.6E+03	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	1.8E+02	2.2E+00	7.0E+00	10	100	1.04E+03	104%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T04-A	1	1.10E+00	U1/2		1.10E+00	1.0E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T05-A	1	1.10E+00	U1/2		1.10E+00	1.0E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T06-A	1	1.10E+00	U1/2		1.10E+00	1.5E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T07-A	1	1.41E+01			1.41E+01	3.2E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T08-A	1	1.77E+01			1.77E+01	1.4E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T09-A	1	3.83E+01			3.83E+01	1.1E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T01-B	1	1.10E+00	U1/2		1.10E+00	1.6E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T02-B	1	1.10E+00	U1/2		1.10E+00	1.4E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	1.3E+02	2.2E+00	7.0E+00	10	100	1.04E+03	104%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T04-B	1	1.10E+00	U1/2		1.10E+00	3.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T05-B	1	1.10E+00	U1/2		1.10E+00	2.1E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T06-B	1	1.10E+00	U1/2		1.10E+00	5.6E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T07-B	1	3.28E+00	E		3.28E+00	1.7E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T08-B	1	1.96E+01			1.96E+01	1.6E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T09-B	1	3.89E+01			3.89E+01	2.4E-01	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T01-C	1	1.10E+00	U1/2		1.10E+00	9.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T02-C	1	1.10E+00	U1/2		1.10E+00	1.8E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	1.9E+02	2.2E+00	7.0E+00	10	100	1.05E+03	105%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T04-C	1	1.10E+00	U1/2		1.10E+00	4.8E+01	2.2E+00	7.0E+00					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T05-C	1	1.10E+00	U1/2		1.10E+00	1.0E+02	2.2E+00	7.0E+00					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T06-C	1	1.10E+00	U1/2		1.10E+00	7.7E+01	2.2E+00	7.0E+00					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T07-C	1	1.03E+01			1.03E+01	5.7E+00	2.2E+00	7.0E+00					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T08-C	1	1.56E+01			1.56E+01	3.7E+00	2.2E+00	7.0E+00					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T09-C	1	4.25E+01			4.25E+01	3.0E+00	2.2E+00	7.0E+00					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	1.7E+01	2.2E+00	7.0E+00					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	6.7E+02	2.2E+00	7.0E+00					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-B03-A	1	1.10E+00	U1/2		1.10E+00	1.4E+02	2.2E+00	7.0E+00					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	SWA-LRef-1313-T01-A	1	5.39E+03			5.39E+03	5.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T02-A	1	1.34E+04			1.34E+04	5.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T03-A	1	2.34E+04			2.34E+04	8.1E-01	2.6E+00	8.3E+00	1000	100	2.43E+04	91%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T04-A	1	4.20E+06			4.20E+06	1.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T05-A	1	5.79E+06			5.79E+06	4.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T06-A	1	8.99E+06			8.99E+06	9.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T07-A	1	1.02E+07			1.02E+07	6.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T08-A	1	5.28E+06			5.28E+06	1.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T09-A	1	3.60E+06			3.60E+06	7.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T01-B	1	6.81E+03			6.81E+03	5.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T02-B	1	1.34E+04			1.34E+04	3.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T03-B	1	2.13E+04			2.13E+04	5.6E-01	2.6E+00	8.3E+00	1000	100	2.23E+04	95%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T04-B	1	5.23E+06			5.23E+06	9.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T05-B	1	7.12E+06			7.12E+06	7.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T06-B	1	9.20E+06			9.20E+06	1.6E+00	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T07-B	1	8.54E+06			8.54E+06	9.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T08-B	1	5.16E+06			5.16E+06	5.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T09-B	1	3.82E+06			3.82E+06	1.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T01-C	1	7.65E+03			7.65E+03	7.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T02-C	1	1.44E+04			1.44E+04	5.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T03-C	1	2.32E+04			2.32E+04	4.0E-01	2.6E+00	8.3E+00	1000	100	2.40E+04	83%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T04-C	1	4.67E+06			4.67E+06	9.6E-01	2.6E+00	8.3E+00					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T05-C	1	7.71E+06			7.71E+06	1.0E+00	2.6E+00	8.3E+00					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T06-C	1	6.94E+06			6.94E+06	2.0E-01	2.6E+00	8.3E+00					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T07-C	1	8.96E+06			8.96E+06	6.7E-01	2.6E+00	8.3E+00					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T08-C	1	5.61E+06			5.61E+06	1.4E+00	2.6E+00	8.3E+00					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T09-C	1	3.83E+06			3.83E+06	6.3E-01	2.6E+00	8.3E+00					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-B01-A	1	3.20E+01			3.20E+01	4.7E+01	2.6E+00	8.3E+00					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-B02-A	1	3.05E+01			3.05E+01	2.2E+01	2.6E+00	8.3E+00					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-B03-A	1	1.30E+00	U1/2		1.30E+00	4.9E+02	2.6E+00	8.3E+00					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	SWA-LRef-1313-T01-A	1	1.13E+03			1.13E+03	7.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T02-A	1	9.85E+02			9.85E+02	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T03-A	1	4.12E+02			4.12E+02	6.2E-01	1.2E+00	3.8E+00	10	100	1.45E+03	103%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T04-A	1	3.92E+00			3.92E+00	1.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T05-A	1	4.15E+00			4.15E+00	2.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T06-A	1	1.23E+00	E		1.23E+00	7.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T07-A	1	1.59E+01			1.59E+01	2.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T08-A	1	2.80E+03			2.80E+03	4.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T09-A	1	2.40E+04			2.40E+04	1.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T01-B	1	1.53E+03			1.53E+03	5.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T02-B	1	1.21E+03			1.21E+03	1.7E-02	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T03-B	1	6.01E+02			6.01E+02	2.5E-01	1.2E+00	3.8E+00	10	100	1.60E+03	100%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T04-B	1	2.32E+00	E		2.32E+00	1.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T05-B	1	1.79E+00	E		1.79E+00	7.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T06-B	1	6.00E-01	U1/2		6.00E-01	1.9E+02	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T07-B	1	4.91E+00			4.91E+00	1.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T08-B	1	3.59E+03			3.59E+03	9.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T09-B	1	2.18E+04			2.18E+04	6.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T01-C	1	1.51E+03			1.51E+03	8.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T02-C	1	1.17E+03			1.17E+03	2.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T03-C	1	3.55E+02			3.55E+02	4.9E-01	1.2E+00	3.8E+00	10	100	1.40E+03	104%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T04-C	1	3.68E+00	E		3.68E+00	4.6E+01	1.2E+00	3.8E+00					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T05-C	1	1.24E+00	E		1.24E+00	6.0E+01	1.2E+00	3.8E+00					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T06-C	1	6.00E-01	U1/2		6.00E-01	4.8E+01	1.2E+00	3.8E+00					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T07-C	1	3.41E+00	E		3.41E+00	2.0E+01	1.2E+00	3.8E+00					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T08-C	1	1.78E+03			1.78E+03	6.5E-01	1.2E+00	3.8E+00					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T09-C	1	2.40E+04			2.40E+04	3.3E+00	1.2E+00	3.8E+00					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	2.7E+01	1.2E+00	3.8E+00					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	4.3E+02	1.2E+00	3.8E+00					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-B03-A	1	6.00E-01	U1/2		6.00E-01	7.1E+01	1.2E+00	3.8E+00					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	SWA-LRef-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	1.9E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	8.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	6.3E+01	1.8E+00	5.7E+00	10	100	1.02E+03	102%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T04-A	1	2.36E+00	E		2.36E+00	5.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T05-A	1	4.05E+00	E		4.05E+00	1.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T06-A	1	1.49E+02			1.49E+02	9.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T07-A	1	2.46E+02			2.46E+02	1.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T08-A	1	1.81E+02			1.81E+02	8.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T09-A	1	2.50E+02			2.50E+02	8.3E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	8.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	3.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	1.8E+02	1.8E+00	5.7E+00	10	100	1.01E+03	101%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T04-B	1	2.18E+00	E		2.18E+00	6.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T05-B	1	7.06E+00			7.06E+00	1.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T06-B	1	1.29E+02			1.29E+02	2.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T07-B	1	1.54E+02			1.54E+02	1.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T08-B	1	1.89E+02			1.89E+02	7.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T09-B	1	2.50E+02			2.50E+02	6.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	5.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	4.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	7.6E+01	1.8E+00	5.7E+00	10	100	1.02E+03	102%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T04-C	1	2.31E+00	E		2.31E+00	6.9E+01	1.8E+00	5.7E+00					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T05-C	1	1.01E+01			1.01E+01	1.1E+01	1.8E+00	5.7E+00					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T06-C	1	4.27E+01			4.27E+01	5.2E+00	1.8E+00	5.7E+00					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T07-C	1	2.06E+02			2.06E+02	7.4E-01	1.8E+00	5.7E+00					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T08-C	1	1.91E+02			1.91E+02	6.0E-01	1.8E+00	5.7E+00					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T09-C	1	2.61E+02			2.61E+02	2.2E+00	1.8E+00	5.7E+00					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	5.8E+01	1.8E+00	5.7E+00					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	3.5E+01	1.8E+00	5.7E+00					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	3.3E+01	1.8E+00	5.7E+00					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	SWA-LRef-1313-T01-A	1	1.85E+00	U1/2		1.85E+00	1.7E+02	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T02-A	1	1.85E+00	U1/2		1.85E+00	1.2E+02	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T03-A	1	1.85E+00	U1/2		1.85E+00	1.4E+02	3.7E+00	1.2E+01	10	100	1.03E+03	103%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T04-A	1	6.06E+00	E		6.06E+00	2.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T05-A	1	8.81E+00	E		8.81E+00	4.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T06-A	1	1.97E+01			1.97E+01	2.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T07-A	1	1.54E+01			1.54E+01	2.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T08-A	1	3.17E+01			3.17E+01	7.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T09-A	1	1.50E+03			1.50E+03	6.3E-01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T01-B	1	1.85E+00	U1/2		1.85E+00	1.7E+02	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T02-B	1	1.85E+00	U1/2		1.85E+00	2.4E+02	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T03-B	1	1.85E+00	U1/2		1.85E+00	9.2E+01	3.7E+00	1.2E+01	10	100	1.03E+03	102%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T04-B	1	7.25E+00	E		7.25E+00	1.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T05-B	1	1.04E+01	E		1.04E+01	3.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T06-B	1	1.10E+01	E		1.10E+01	3.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T07-B	1	1.26E+01			1.26E+01	2.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T08-B	1	1.87E+01			1.87E+01	9.6E-01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T09-B	1	1.51E+03			1.51E+03	7.7E-01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T01-C	1	1.85E+00	U1/2		1.85E+00	9.6E+02	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T02-C	1	1.85E+00	U1/2		1.85E+00	3.8E+02	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T03-C	1	1.85E+00	U1/2		1.85E+00	8.1E+02	3.7E+00	1.2E+01	10	100	1.03E+03	102%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T04-C	1	6.19E+00	E		6.19E+00	1.2E+01	3.7E+00	1.2E+01					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T05-C	1	8.30E+00	E		8.30E+00	2.3E+01	3.7E+00	1.2E+01					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T06-C	1	8.19E+00	E		8.19E+00	3.0E+01	3.7E+00	1.2E+01					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T07-C	1	1.54E+01			1.54E+01	7.7E+00	3.7E+00	1.2E+01					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T08-C	1	1.87E+01			1.87E+01	1.1E+01	3.7E+00	1.2E+01					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T09-C	1	1.57E+03			1.57E+03	1.7E+00	3.7E+00	1.2E+01					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-B01-A	1	5.29E+00	E		5.29E+00	3.7E+01	3.7E+00	1.2E+01					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	1.2E+02	3.7E+00	1.2E+01					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-B03-A	1	1.85E+00	U1/2		1.85E+00	3.4E+02	3.7E+00	1.2E+01					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	SWA-LRef-1313-T01-A	1	5.87E+01			5.87E+01	4.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T02-A	1	7.31E+01			7.31E+01	2.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T03-A	1	5.33E+01			5.33E+01	1.5E+00	2.0E+00	6.4E+00	1000	100	1.11E+03	106%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T04-A	1	2.08E+01			2.08E+01	3.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T05-A	1	3.03E+01			3.03E+01	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T06-A	1	3.90E+04			3.90E+04	1.6E-02	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T07-A	1	1.31E+05			1.31E+05	4.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T08-A	1	1.31E+05			1.31E+05	7.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T09-A	1	1.95E+05			1.95E+05	6.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T01-B	1	1.13E+02			1.13E+02	5.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T02-B	1	8.01E+01			8.01E+01	9.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T03-B	1	8.13E+01			8.13E+01	1.4E+00	2.0E+00	6.4E+00	1000	100	1.14E+03	105%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T04-B	1	2.63E+01			2.63E+01	3.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T05-B	1	2.59E+01			2.59E+01	4.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T06-B	1	6.12E+04			6.12E+04	1.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T07-B	1	5.18E+04			5.18E+04	8.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T08-B	1	1.35E+05			1.35E+05	4.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T09-B	1	1.78E+05			1.78E+05	1.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T01-C	1	9.26E+01			9.26E+01	4.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T02-C	1	7.18E+01			7.18E+01	2.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T03-C	1	6.28E+01			6.28E+01	1.2E+00	2.0E+00	6.4E+00	1000	100	1.13E+03	107%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T04-C	1	2.69E+01			2.69E+01	2.3E+00	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T05-C	1	2.70E+01			2.70E+01	7.4E+00	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T06-C	1	3.09E+03			3.09E+03	9.6E-01	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T07-C	1	1.01E+05			1.01E+05	5.4E-01	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T08-C	1	1.24E+05			1.24E+05	5.5E-01	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T09-C	1	1.91E+05			1.91E+05	4.3E+00	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	5.8E+00	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-B02-A	1	4.90E+00	E		4.90E+00	3.7E+00	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-B03-A	1	2.47E+00	E		2.47E+00	6.1E+00	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	SWA-LRef-1313-T01-A	1	1.02E+01	E		1.02E+01	4.3E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T02-A	1	7.28E+00	E		7.28E+00	1.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T03-A	1	8.46E+00	E		8.46E+00	5.4E+01	6.8E+00	2.2E+01	10	100	9.86E+02	98%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T04-A	1	3.40E+00	U1/2		3.40E+00	7.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T05-A	1	3.40E+00	U1/2		3.40E+00	2.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T06-A	1	3.40E+00	U1/2		3.40E+00	1.1E+02	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T07-A	1	3.40E+00	U1/2		3.40E+00	1.3E+02	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T08-A	1	1.34E+02			1.34E+02	2.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T09-A	1	3.65E+03			3.65E+03	4.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T01-B	1	5.69E+01			5.69E+01	1.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T02-B	1	1.38E+01	E		1.38E+01	2.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T03-B	1	8.83E+00	E		8.83E+00	2.0E+01	6.8E+00	2.2E+01	10	100	9.89E+02	98%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T04-B	1	3.40E+00	U1/2		3.40E+00	8.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T05-B	1	3.40E+00	U1/2		3.40E+00	7.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T06-B	1	3.40E+00	U1/2		3.40E+00	3.3E+02	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T07-B	1	3.40E+00	U1/2		3.40E+00	5.8E+02	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T08-B	1	1.44E+02			1.44E+02	1.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T09-B	1	3.70E+03			3.70E+03	4.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T01-C	1	3.25E+01			3.25E+01	1.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T02-C	1	2.12E+01	E		2.12E+01	2.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T03-C	1	9.07E+00	E		9.07E+00	7.5E+01	6.8E+00	2.2E+01	10	100	9.95E+02	99%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T04-C	1	3.40E+00	U1/2		3.40E+00	1.0E+02	6.8E+00	2.2E+01					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T05-C	1	3.40E+00	U1/2		3.40E+00	3.7E+02	6.8E+00	2.2E+01					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T06-C	1	3.40E+00	U1/2		3.40E+00	7.2E+01	6.8E+00	2.2E+01					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T07-C	1	3.40E+00	U1/2		3.40E+00	8.2E+02	6.8E+00	2.2E+01					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T08-C	1	4.79E+01			4.79E+01	6.1E+00	6.8E+00	2.2E+01					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T09-C	1	4.09E+03			4.09E+03	2.6E+00	6.8E+00	2.2E+01					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	1.4E+01	6.8E+00	2.2E+01					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	1.7E+02	6.8E+00	2.2E+01					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	2.9E+02	6.8E+00	2.2E+01					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	SWA-LRef-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	5.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	1.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	4.5E+01	1.9E+00	6.0E+00	10	100	8.18E+02	82%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T04-A	1	4.47E+02			4.47E+02	1.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T05-A	1	7.98E+02			7.98E+02	2.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T06-A	1	1.37E+03			1.37E+03	2.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T07-A	1	1.67E+03			1.67E+03	1.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T08-A	1	9.04E+02			9.04E+02	6.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T09-A	1	9.61E+02			9.61E+02	1.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	4.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	3.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	6.3E+01	1.9E+00	6.0E+00	10	100	8.06E+02	81%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T04-B	1	6.74E+02			6.74E+02	5.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T05-B	1	1.08E+03			1.08E+03	1.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T06-B	1	1.45E+03			1.45E+03	5.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T07-B	1	1.26E+03			1.26E+03	3.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T08-B	1	8.98E+02			8.98E+02	1.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T09-B	1	9.74E+02			9.74E+02	4.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	2.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	1.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00	10	100	8.11E+02	81%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T04-C	1	5.36E+02			5.36E+02	3.5E+00	1.9E+00	6.0E+00					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T05-C	1	1.13E+03			1.13E+03	1.7E+00	1.9E+00	6.0E+00					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T06-C	1	1.01E+03			1.01E+03	2.1E+00	1.9E+00	6.0E+00					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T07-C	1	1.35E+03			1.35E+03	5.6E-01	1.9E+00	6.0E+00					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T08-C	1	9.93E+02			9.93E+02	5.3E+00	1.9E+00	6.0E+00					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T09-C	1	9.55E+02			9.55E+02	6.2E+00	1.9E+00	6.0E+00					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	8.2E+01	1.9E+00	6.0E+00					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	6.8E+01	1.9E+00	6.0E+00					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	1.9E+02	1.9E+00	6.0E+00					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	SWA-LRef-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	1.7E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	9.5E+00	2.0E+00	6.4E+00	10	100	1.04E+03	104%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T04-A	1	3.16E+01			3.16E+01	1.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T05-A	1	1.95E+03			1.95E+03	5.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T06-A	1	2.30E+04			2.30E+04	4.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T07-A	1	3.14E+04			3.14E+04	5.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T08-A	1	1.91E+04			1.91E+04	5.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T09-A	1	2.04E+04			2.04E+04	5.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	7.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	3.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	1.3E+00	2.0E+00	6.4E+00	10	100	1.03E+03	103%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T04-B	1	1.39E+02			1.39E+02	6.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T05-B	1	3.33E+03			3.33E+03	9.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T06-B	1	2.16E+04			2.16E+04	7.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T07-B	1	2.19E+04			2.19E+04	3.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T08-B	1	1.88E+04			1.88E+04	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T09-B	1	2.07E+04			2.07E+04	8.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	6.3E+00	2.0E+00	6.4E+00	10	100	1.05E+03	105%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T04-C	1	3.32E+01			3.32E+01	7.7E-01	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T05-C	1	3.36E+03			3.36E+03	3.1E-01	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T06-C	1	1.03E+04			1.03E+04	6.6E-01	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T07-C	1	2.63E+04			2.63E+04	1.7E-01	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T08-C	1	2.04E+04			2.04E+04	1.7E+00	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T09-C	1	2.06E+04			2.06E+04	2.2E+00	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	5.7E+00	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-B02-A	1	4.73E+00	E		4.73E+00	2.1E+00	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	2.6E+00	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	SWA-LRef-1313-T01-A	1	1.78E+01			1.78E+01	9.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T02-A	1	1.97E+01			1.97E+01	9.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T03-A	1	6.24E+00			6.24E+00	5.9E+01	1.0E+00	3.2E+00	1000	100	1.01E+03	100%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T04-A	1	2.78E+05			2.78E+05	5.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T05-A	1	8.36E+05			8.36E+05	7.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T06-A	1	1.54E+06			1.54E+06	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T07-A	1	1.79E+06			1.79E+06	2.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T08-A	1	9.62E+05			9.62E+05	9.4E-02	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T09-A	1	8.31E+05			8.31E+05	7.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T01-B	1	1.12E+01			1.12E+01	1.1E+02	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T02-B	1	5.10E+00			5.10E+00	5.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T03-B	1	1.17E+01			1.17E+01	5.2E+01	1.0E+00	3.2E+00	1000	100	1.01E+03	99%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T04-B	1	5.87E+05			5.87E+05	6.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T05-B	1	1.03E+06			1.03E+06	7.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T06-B	1	1.53E+06			1.53E+06	8.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T07-B	1	1.42E+06			1.42E+06	2.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T08-B	1	9.24E+05			9.24E+05	7.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T09-B	1	8.36E+05			8.36E+05	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T01-C	1	1.28E+01			1.28E+01	6.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T02-C	1	4.93E+00			4.93E+00	2.2E+02	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T03-C	1	2.46E+01			2.46E+01	2.2E+01	1.0E+00	3.2E+00	1000	100	1.01E+03	99%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T04-C	1	4.69E+05			4.69E+05	9.4E-01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T05-C	1	1.15E+06			1.15E+06	4.7E-01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T06-C	1	1.07E+06			1.07E+06	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T07-C	1	1.52E+06			1.52E+06	3.7E-01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T08-C	1	1.02E+06			1.02E+06	4.3E-01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T09-C	1	8.44E+05			8.44E+05	3.5E+00	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-B01-A	1	9.01E+00			9.01E+00	3.5E+01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-B02-A	1	3.08E+01			3.08E+01	2.5E+01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-B03-A	1	3.55E+00			3.55E+00	1.6E+02	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	SWA-LRef-1313-T01-A	1	1.42E+02			1.42E+02	1.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T02-A	1	1.48E+02			1.48E+02	7.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T03-A	1	1.39E+02			1.39E+02	2.7E+00	1.2E+00	3.8E+00	10	100	1.16E+03	103%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T04-A	1	1.34E+02			1.34E+02	1.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T05-A	1	1.15E+02			1.15E+02	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T06-A	1	6.73E+01			6.73E+01	8.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T07-A	1	1.63E+01			1.63E+01	2.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T08-A	1	2.42E+01			2.42E+01	4.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T09-A	1	1.73E+01			1.73E+01	5.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T01-B	1	1.51E+02			1.51E+02	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T02-B	1	1.50E+02			1.50E+02	1.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T03-B	1	1.57E+02			1.57E+02	2.1E+00	1.2E+00	3.8E+00	10	100	1.17E+03	102%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T04-B	1	1.34E+02			1.34E+02	2.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T05-B	1	1.29E+02			1.29E+02	1.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T06-B	1	3.35E+01			3.35E+01	5.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T07-B	1	8.06E+00			8.06E+00	2.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T08-B	1	1.78E+01			1.78E+01	8.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T09-B	1	1.55E+01			1.55E+01	1.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T01-C	1	1.43E+02			1.43E+02	1.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T02-C	1	1.45E+02			1.45E+02	3.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T03-C	1	1.44E+02			1.44E+02	1.1E+00	1.2E+00	3.8E+00	10	100	1.17E+03	103%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T04-C	1	1.33E+02			1.33E+02	2.1E+00	1.2E+00	3.8E+00					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T05-C	1	1.28E+02			1.28E+02	9.0E-01	1.2E+00	3.8E+00					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T06-C	1	8.94E+01			8.94E+01	2.5E+00	1.2E+00	3.8E+00					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T07-C	1	1.07E+01			1.07E+01	1.4E+01	1.2E+00	3.8E+00					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T08-C	1	2.47E+01			2.47E+01	3.1E+01	1.2E+00	3.8E+00					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T09-C	1	2.04E+01			2.04E+01	3.9E+01	1.2E+00	3.8E+00					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	3.5E+01	1.2E+00	3.8E+00					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-B02-A	1	2.28E+00	E		2.28E+00	2.9E+01	1.2E+00	3.8E+00					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-B03-A	1	6.00E-01	U1/2		6.00E-01	2.1E+01	1.2E+00	3.8E+00					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	SWA-LRef-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	1.9E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	1.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	3.2E+01	1.8E+00	5.7E+00	10	100	1.00E+03	100%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T04-A	1	3.51E+00	E		3.51E+00	2.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T05-A	1	2.00E+01			2.00E+01	1.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T06-A	1	1.24E+02			1.24E+02	1.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T07-A	1	5.34E+02			5.34E+02	6.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T08-A	1	3.70E+02			3.70E+02	7.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T09-A	1	4.40E+02			4.40E+02	2.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	9.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	3.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	7.1E+01	1.8E+00	5.7E+00	10	100	1.00E+03	100%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T04-B	1	5.10E+00	E		5.10E+00	7.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T05-B	1	2.66E+01			2.66E+01	6.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T06-B	1	2.67E+02			2.67E+02	7.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T07-B	1	3.52E+02			3.52E+02	1.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T08-B	1	3.74E+02			3.74E+02	7.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T09-B	1	4.36E+02			4.36E+02	2.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T01-C		9.00E-01	U1/2		0.00E+00	7.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T02-C		9.00E-01	U1/2		0.00E+00	7.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T03-C		9.00E-01	U1/2		0.00E+00	2.1E+01	1.8E+00	5.7E+00	10	100	1.01E+03	101%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T04-C		6.22E+00	U1/2		0.00E+00	4.1E+01	1.8E+00	5.7E+00					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T05-C		3.06E+01	U1/2		0.00E+00	5.4E+00	1.8E+00	5.7E+00					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T06-C		1.17E+02	U1/2		0.00E+00	3.7E+00	1.8E+00	5.7E+00					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T07-C		4.58E+02	U1/2		0.00E+00	1.1E+00	1.8E+00	5.7E+00					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T08-C		4.00E+02	U1/2		0.00E+00	6.9E-01	1.8E+00	5.7E+00					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T09-C		4.39E+02	U1/2		0.00E+00	2.8E+00	1.8E+00	5.7E+00					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-B01-A		9.00E-01	U1/2		0.00E+00	8.0E+00	1.8E+00	5.7E+00					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-B02-A		9.00E-01	U1/2		0.00E+00	7.4E+00	1.8E+00	5.7E+00					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-B03-A		9.00E-01	U1/2		0.00E+00	7.2E+00	1.8E+00	5.7E+00					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	SWA-LRef-1313-T01-A	1	9.46E+01			9.46E+01	1.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T02-A	1	3.59E+01			3.59E+01	5.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T03-A	1	2.32E+01			2.32E+01	9.4E+01	3.7E+00	1.2E+01	1000	100	1.19E+03	117%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T04-A	1	7.43E+01			7.43E+01	5.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T05-A	1	6.40E+01			6.40E+01	4.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T06-A	1	2.72E+01			2.72E+01	1.0E+02	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T07-A	1	1.45E+01			1.45E+01	1.5E+02	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T08-A	1	1.02E+03			1.02E+03	5.9E-01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T09-A	1	1.24E+04			1.24E+04	7.5E-01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T01-B	1	1.40E+02			1.40E+02	3.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T02-B	1	4.47E+01			4.47E+01	2.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T03-B	1	2.67E+01			2.67E+01	3.8E+01	3.7E+00	1.2E+01	1000	100	1.22E+03	119%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T04-B	1	6.30E+01			6.30E+01	1.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T05-B	1	1.19E+02			1.19E+02	1.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T06-B	1	4.75E+01			4.75E+01	2.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T07-B	1	4.45E+01			4.45E+01	8.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T08-B	1	8.44E+02			8.44E+02	1.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T09-B	1	1.31E+04			1.31E+04	1.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T01-C	1	1.10E+02			1.10E+02	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T02-C	1	3.66E+01			3.66E+01	3.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T03-C	1	1.79E+01			1.79E+01	5.1E+01	3.7E+00	1.2E+01	1000	100	1.21E+03	119%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T04-C	1	5.42E+01			5.42E+01	4.4E+01	3.7E+00	1.2E+01					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T05-C	1	2.74E+01			2.74E+01	9.0E+00	3.7E+00	1.2E+01					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T06-C	1	4.58E+01			4.58E+01	4.1E+01	3.7E+00	1.2E+01					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T07-C	1	2.37E+01			2.37E+01	2.9E+01	3.7E+00	1.2E+01					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T08-C	1	7.91E+02			7.91E+02	4.0E-01	3.7E+00	1.2E+01					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T09-C	1	1.25E+04			1.25E+04	3.0E+00	3.7E+00	1.2E+01					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	3.2E+01	3.7E+00	1.2E+01					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-B02-A	1	1.54E+01			1.54E+01	2.0E+01	3.7E+00	1.2E+01					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-B03-A	1	1.85E+00	U1/2		1.85E+00	3.5E+01	3.7E+00	1.2E+01					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	SWA-LRef-1313-T01-A	1	2.21E+06			2.21E+06	3.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T02-A	1	2.80E+05			2.80E+05	2.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T03-A	1	2.81E+05			2.81E+05	8.1E-01	1.6E+00	5.1E+00	1000	100	2.82E+05	95%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T04-A	1	4.14E+05			4.14E+05	8.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T05-A	1	4.12E+05			4.12E+05	1.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T06-A	1	4.65E+05			4.65E+05	9.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T07-A	1	4.81E+05			4.81E+05	3.4E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T08-A	1	2.88E+05			2.88E+05	2.9E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T09-A	1	3.23E+05			3.23E+05	8.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T01-B	1	2.26E+06			2.26E+06	8.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T02-B	1	2.81E+05			2.81E+05	3.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T03-B	1	2.84E+05			2.84E+05	2.6E-01	1.6E+00	5.1E+00	1000	100	2.85E+05	100%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T04-B	1	4.10E+05			4.10E+05	9.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T05-B	1	4.33E+05			4.33E+05	4.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T06-B	1	4.86E+05			4.86E+05	5.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T07-B	1	4.64E+05			4.64E+05	7.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T08-B	1	3.18E+05			3.18E+05	7.9E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T09-B	1	3.18E+05			3.18E+05	1.2E+01	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T01-C	1	2.21E+06			2.21E+06	4.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T02-C	1	2.80E+05			2.80E+05	5.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T03-C	1	2.85E+05			2.85E+05	1.2E+00	1.6E+00	5.1E+00	1000	100	2.86E+05	85%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T04-C	1	4.16E+05			4.16E+05	7.0E-01	1.6E+00	5.1E+00					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T05-C	1	4.42E+05			4.42E+05	3.6E-01	1.6E+00	5.1E+00					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T06-C	1	4.40E+05			4.40E+05	4.7E-01	1.6E+00	5.1E+00					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T07-C	1	4.85E+05			4.85E+05	6.3E+00	1.6E+00	5.1E+00					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T08-C	1	3.92E+05			3.92E+05	1.6E+01	1.6E+00	5.1E+00					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T09-C	1	3.77E+05			3.77E+05	9.9E+00	1.6E+00	5.1E+00					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-B01-A	1	7.04E+00			7.04E+00	6.8E+00	1.6E+00	5.1E+00					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-B02-A	1	7.67E+00			7.67E+00	1.2E+01	1.6E+00	5.1E+00					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-B03-A	1	2.11E+06			2.11E+06	2.3E-01	1.6E+00	5.1E+00					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	SWA-LRef-1313-T01-A	1	9.17E+04			9.17E+04	3.9E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T02-A	1	1.04E+05			1.04E+05	6.1E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T03-A	1	9.91E+04			9.91E+04	1.0E+00	1.5E+01	4.8E+01	10	100	1.00E+05	104%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T04-A	1	1.09E+05			1.09E+05	4.8E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T05-A	1	1.16E+05			1.16E+05	1.0E+00	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T06-A	1	1.28E+05			1.28E+05	6.8E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T07-A	1	1.26E+05			1.26E+05	8.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T08-A	1	6.64E+04			6.64E+04	2.2E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T09-A	1	4.54E+04			4.54E+04	1.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T01-B	1	1.02E+05			1.02E+05	9.4E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T02-B	1	1.04E+05			1.04E+05	4.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T03-B	1	1.08E+05			1.08E+05	7.9E-01	1.5E+01	4.8E+01	10	100	1.09E+05	105%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T04-B	1	1.14E+05			1.14E+05	7.1E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T05-B	1	1.24E+05			1.24E+05	8.4E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T06-B	1	1.28E+05			1.28E+05	1.0E+00	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T07-B	1	1.21E+05			1.21E+05	1.1E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T08-B	1	6.05E+04			6.05E+04	7.8E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T09-B	1	4.40E+04			4.40E+04	4.5E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T01-C	1	9.53E+04			9.53E+04	5.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T02-C	1	1.00E+05			1.00E+05	5.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T03-C	1	1.03E+05			1.03E+05	1.8E-01	1.5E+01	4.8E+01	10	100	1.04E+05	92%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T04-C	1	1.08E+05			1.08E+05	7.5E-01	1.5E+01	4.8E+01					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T05-C	1	1.32E+05			1.32E+05	5.1E-01	1.5E+01	4.8E+01					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T06-C	1	1.17E+05			1.17E+05	1.8E-01	1.5E+01	4.8E+01					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T07-C	1	1.22E+05			1.22E+05	3.7E-01	1.5E+01	4.8E+01					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T08-C	1	6.71E+04			6.71E+04	7.1E-01	1.5E+01	4.8E+01					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T09-C	1	4.40E+04			4.40E+04	3.2E+00	1.5E+01	4.8E+01					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-B01-A	1	7.50E+00	U1/2		7.50E+00	7.5E+01	1.5E+01	4.8E+01					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-B02-A	1	7.50E+00	U1/2		7.50E+00	4.1E+02	1.5E+01	4.8E+01					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-B03-A	1	7.50E+00	U1/2		7.50E+00	1.8E+01	1.5E+01	4.8E+01					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	SWA-LRef-1313-T01-A	1	5.80E+03			5.80E+03	8.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T02-A	1	5.00E+03			5.00E+03	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T03-A	1	4.84E+03			4.84E+03	9.7E-01	1.1E+00	3.5E+00	1000	100	5.71E+03	88%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T04-A	1	9.77E+02			9.77E+02	8.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T05-A	1	1.26E+03			1.26E+03	8.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T06-A	1	2.32E+03			2.32E+03	7.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T07-A	1	2.39E+03			2.39E+03	6.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T08-A	1	1.90E+04			1.90E+04	6.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T09-A	1	1.44E+04			1.44E+04	2.8E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T01-B	1	7.62E+03			7.62E+03	5.4E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T02-B	1	5.65E+03			5.65E+03	2.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T03-B	1	5.22E+03			5.22E+03	4.1E-01	1.1E+00	3.5E+00	1000	100	6.16E+03	94%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T04-B	1	9.80E+02			9.80E+02	7.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T05-B	1	1.05E+03			1.05E+03	6.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T06-B	1	2.08E+03			2.08E+03	4.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T07-B	1	2.51E+03			2.51E+03	2.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T08-B	1	1.57E+04			1.57E+04	8.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T09-B	1	1.54E+04			1.54E+04	5.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T01-C	1	7.97E+03			7.97E+03	7.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T02-C	1	5.56E+03			5.56E+03	6.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T03-C	1	4.64E+03			4.64E+03	6.6E-01	1.1E+00	3.5E+00	1000	100	5.60E+03	96%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T04-C	1	1.03E+03			1.03E+03	1.1E+00	1.1E+00	3.5E+00					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T05-C	1	1.12E+03			1.12E+03	7.7E-01	1.1E+00	3.5E+00					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T06-C	1	1.68E+03			1.68E+03	6.6E-01	1.1E+00	3.5E+00					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T07-C	1	2.54E+03			2.54E+03	4.9E-01	1.1E+00	3.5E+00					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T08-C	1	1.58E+04			1.58E+04	2.4E-01	1.1E+00	3.5E+00					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T09-C	1	1.58E+04			1.58E+04	1.6E+01	1.1E+00	3.5E+00					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-B01-A	1	1.58E+00	E		1.58E+00	2.3E+01	1.1E+00	3.5E+00					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-B02-A	1	2.17E+00	E		2.17E+00	5.7E+00	1.1E+00	3.5E+00					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-B03-A	1	1.93E+01			1.93E+01	2.4E+00	1.1E+00	3.5E+00					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	SWA-LRef-1313-T01-A	1	4.76E+05			4.76E+05	6.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T02-A	1	4.40E+05			4.40E+05	2.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T03-A	1	4.41E+05			4.41E+05	2.4E-01	2.5E+00	8.0E+00	1000	100	4.42E+05	90%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T04-A	1	5.53E+05			5.53E+05	1.5E+00	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T05-A	1	5.48E+05			5.48E+05	6.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T06-A	1	5.80E+05			5.80E+05	1.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T07-A	1	5.68E+05			5.68E+05	2.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T08-A	1	2.92E+05			2.92E+05	5.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T09-A	1	1.84E+05			1.84E+05	6.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T01-B	1	4.78E+05			4.78E+05	7.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T02-B	1	4.39E+05			4.39E+05	1.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T03-B	1	4.41E+05			4.41E+05	5.4E-01	2.5E+00	8.0E+00	1000	100	4.42E+05	103%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T04-B	1	5.45E+05			5.45E+05	4.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T05-B	1	5.61E+05			5.61E+05	7.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T06-B	1	5.79E+05			5.79E+05	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T07-B	1	5.71E+05			5.71E+05	2.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T08-B	1	2.78E+05			2.78E+05	8.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T09-B	1	1.83E+05			1.83E+05	3.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T01-C	1	4.63E+05			4.63E+05	3.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T02-C	1	4.35E+05			4.35E+05	4.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T03-C	1	4.47E+05			4.47E+05	5.2E-01	2.5E+00	8.0E+00	1000	100	4.48E+05	89%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T04-C	1	5.50E+05			5.50E+05	1.5E+00	2.5E+00	8.0E+00					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T05-C	1	5.72E+05			5.72E+05	3.4E-01	2.5E+00	8.0E+00					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T06-C	1	5.64E+05			5.64E+05	4.4E-01	2.5E+00	8.0E+00					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T07-C	1	5.69E+05			5.69E+05	3.1E-01	2.5E+00	8.0E+00					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T08-C	1	3.02E+05			3.02E+05	7.8E-01	2.5E+00	8.0E+00					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T09-C	1	1.85E+05			1.85E+05	1.7E+00	2.5E+00	8.0E+00					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-B01-A	1	3.45E+00	E		3.45E+00	1.9E+01	2.5E+00	8.0E+00					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-B02-A	1	3.00E+00	E		3.00E+00	4.0E+01	2.5E+00	8.0E+00					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-B03-A	1	9.88E+02			9.88E+02	2.9E-01	2.5E+00	8.0E+00					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	SWA-LRef-1313-T01-A	1	2.32E+02			2.32E+02	1.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T02-A	1	3.41E+02			3.41E+02	4.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T03-A	1	5.57E+02			5.57E+02	4.6E-01	1.0E+00	3.2E+00	1000	100	1.58E+03	103%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T04-A	1	2.53E+04			2.53E+04	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T05-A	1	3.20E+04			3.20E+04	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T06-A	1	5.16E+04			5.16E+04	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T07-A	1	5.92E+04			5.92E+04	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T08-A	1	3.30E+04			3.30E+04	8.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T09-A	1	2.41E+04			2.41E+04	5.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T01-B	1	2.92E+02			2.92E+02	5.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T02-B	1	3.42E+02			3.42E+02	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T03-B	1	5.04E+02			5.04E+02	1.3E-01	1.0E+00	3.2E+00	1000	100	1.53E+03	102%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T04-B	1	3.00E+04			3.00E+04	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T05-B	1	3.99E+04			3.99E+04	2.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T06-B	1	5.26E+04			5.26E+04	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T07-B	1	5.01E+04			5.01E+04	1.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T08-B	1	3.16E+04			3.16E+04	5.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T09-B	1	2.78E+04			2.78E+04	8.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T01-C	1	3.42E+02			3.42E+02	1.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T02-C	1	3.53E+02			3.53E+02	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T03-C	1	5.56E+02			5.56E+02	6.6E-01	1.0E+00	3.2E+00	1000	100	1.58E+03	102%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T04-C	1	2.69E+04			2.69E+04	1.0E+00	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T05-C	1	4.26E+04			4.26E+04	6.8E-01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T06-C	1	3.99E+04			3.99E+04	8.9E-01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T07-C	1	5.23E+04			5.23E+04	4.2E-01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T08-C	1	3.48E+04			3.48E+04	1.9E-01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T09-C	1	2.78E+04			2.78E+04	4.4E+00	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	3.1E+02	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	3.7E+02	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	4.8E+01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	SWA-LRef-1313-T01-A	1	3.95E+05			3.95E+05	3.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T02-A	1	4.06E+05			4.06E+05	5.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T03-A	1	5.26E+05			5.26E+05	4.1E-01	6.8E+00	2.2E+01	1000	100	5.26E+05	91%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T04-A	1	8.19E+05			8.19E+05	2.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T05-A	1	7.49E+05			7.49E+05	5.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T06-A	1	5.53E+05			5.53E+05	5.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T07-A	1	5.20E+05			5.20E+05	5.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T08-A	1	2.54E+05			2.54E+05	4.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T09-A	1	1.80E+05			1.80E+05	2.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T01-B	1	3.77E+05			3.77E+05	6.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T02-B	1	4.72E+05			4.72E+05	1.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T03-B	1	5.83E+05			5.83E+05	1.9E-01	6.8E+00	2.2E+01	1000	100	5.84E+05	101%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T04-B	1	7.97E+05			7.97E+05	4.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T05-B	1	9.01E+05			9.01E+05	4.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T06-B	1	5.32E+05			5.32E+05	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T07-B	1	5.84E+05			5.84E+05	2.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T08-B	1	2.42E+05			2.42E+05	6.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T09-B	1	1.90E+05			1.90E+05	4.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T01-C	1	4.08E+05			4.08E+05	5.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T02-C	1	4.34E+05			4.34E+05	6.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T03-C	1	5.19E+05			5.19E+05	3.0E-01	6.8E+00	2.2E+01	1000	100	5.20E+05	86%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T04-C	1	8.51E+05			8.51E+05	9.6E-01	6.8E+00	2.2E+01					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T05-C	1	8.97E+05			8.97E+05	5.4E-01	6.8E+00	2.2E+01					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T06-C	1	7.66E+05			7.66E+05	2.4E-01	6.8E+00	2.2E+01					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T07-C	1	5.49E+05			5.49E+05	6.7E-02	6.8E+00	2.2E+01					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T08-C	1	2.76E+05			2.76E+05	6.1E-01	6.8E+00	2.2E+01					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T09-C	1	1.93E+05			1.93E+05	2.4E+00	6.8E+00	2.2E+01					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-B01-A	1	2.29E+01			2.29E+01	1.2E+01	6.8E+00	2.2E+01					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-B02-A	1	2.80E+01			2.80E+01	2.4E+01	6.8E+00	2.2E+01					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-B03-A	1	1.22E+02			1.22E+02	4.1E+00	6.8E+00	2.2E+01					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	SWA-LRef-1313-T01-A	1	2.30E+00	U1/2		2.30E+00	1.1E+02	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T02-A	1	2.30E+00	U1/2		2.30E+00	5.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T03-A	1	2.30E+00	U1/2		2.30E+00	8.7E+01	4.6E+00	1.5E+01	10	100	9.51E+02	95%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T04-A	1	2.30E+00	U1/2		2.30E+00	1.5E+02	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T05-A	1	2.30E+00	U1/2		2.30E+00	4.1E+02	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T06-A	1	1.75E+01			1.75E+01	4.2E+00	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T07-A	1	3.01E+01			3.01E+01	8.2E+00	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T08-A	1	1.32E+01	E		1.32E+01	2.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T09-A	1	1.40E+01	E		1.40E+01	8.4E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T01-B	1	2.30E+00	U1/2		2.30E+00	1.4E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T02-B	1	2.30E+00	U1/2		2.30E+00	6.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T03-B	1	2.30E+00	U1/2		2.30E+00	7.3E+01	4.6E+00	1.5E+01	10	100	9.54E+02	95%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T04-B	1	2.30E+00	U1/2		2.30E+00	7.0E+02	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T05-B	1	2.30E+00	U1/2		2.30E+00	6.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T06-B	1	1.76E+01			1.76E+01	4.1E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T07-B	1	1.93E+01			1.93E+01	2.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T08-B	1	1.16E+01	E		1.16E+01	3.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T09-B	1	1.25E+01	E		1.25E+01	1.5E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T01-C	1	2.30E+00	U1/2		2.30E+00	2.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T02-C	1	2.30E+00	U1/2		2.30E+00	9.8E+00	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T03-C	1	2.30E+00	U1/2		2.30E+00	1.5E+01	4.6E+00	1.5E+01	10	100	9.57E+02	95%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T04-C	1	2.30E+00	U1/2		2.30E+00	5.4E+01	4.6E+00	1.5E+01					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T05-C	1	2.30E+00	U1/2		2.30E+00	1.1E+02	4.6E+00	1.5E+01					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T06-C	1	6.29E+00	E		6.29E+00	3.3E+02	4.6E+00	1.5E+01					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T07-C	1	2.18E+01			2.18E+01	6.5E+01	4.6E+00	1.5E+01					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T08-C	1	1.58E+01			1.58E+01	5.5E+01	4.6E+00	1.5E+01					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T09-C	1	1.54E+01			1.54E+01	1.4E+02	4.6E+00	1.5E+01					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	6.0E+01	4.6E+00	1.5E+01					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	6.3E+00	4.6E+00	1.5E+01					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	2.4E+01	4.6E+00	1.5E+01					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	SWA-LRef-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	3.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	1.7E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00	10	100	1.03E+03	103%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	7.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	2.7E+03	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	2.3E+04	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	1.6E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T08-A	1	5.13E+01			5.13E+01	2.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T09-A	1	7.94E+03			7.94E+03	1.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	6.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	6.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00	10	100	1.03E+03	103%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	2.6E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T08-B	1	4.13E+01			4.13E+01	3.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T09-B	1	7.15E+03			7.15E+03	7.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	1.9E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	4.3E+01	2.0E+00	6.4E+00	10	100	1.04E+03	104%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	5.4E+01	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	2.8E+02	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	9.3E+01	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T08-C	1	4.50E+01			4.50E+01	3.6E+00	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T09-C	1	7.49E+03			7.49E+03	3.5E+00	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.8E+02	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-B02-A	1	2.31E+00	E		2.31E+00	4.7E+00	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	2.5E+02	2.0E+00	6.4E+00					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	SWA-LRef-1313-T01-A	1	4.20E+02			4.20E+02	1.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T02-A	1	2.93E+02			2.93E+02	1.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T03-A	1	2.32E+02			2.32E+02	5.7E-02	1.5E+00	4.8E+00	10	100	1.28E+03	105%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T04-A	1	1.89E+02			1.89E+02	7.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T05-A	1	2.15E+02			2.15E+02	1.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T06-A	1	2.27E+02			2.27E+02	2.9E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T07-A	1	2.20E+02			2.20E+02	8.1E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T08-A	1	1.41E+02			1.41E+02	1.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T09-A	1	1.22E+03			1.22E+03	4.2E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T01-B	1	4.86E+02			4.86E+02	3.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T02-B	1	3.49E+02			3.49E+02	1.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T03-B	1	2.99E+02			2.99E+02	6.2E-01	1.5E+00	4.8E+00	10	100	1.34E+03	104%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T04-B	1	2.36E+02			2.36E+02	1.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T05-B	1	2.26E+02			2.26E+02	1.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T06-B	1	2.25E+02			2.25E+02	2.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T07-B	1	2.14E+02			2.14E+02	6.8E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T08-B	1	1.14E+02			1.14E+02	3.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T09-B	1	9.13E+02			9.13E+02	1.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T01-C	1	4.30E+02			4.30E+02	3.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T02-C	1	3.18E+02			3.18E+02	9.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T03-C	1	2.47E+02			2.47E+02	3.8E-01	1.5E+00	4.8E+00	10	100	1.31E+03	107%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T04-C	1	2.24E+02			2.24E+02	1.1E+00	1.5E+00	4.8E+00					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T05-C	1	2.35E+02			2.35E+02	5.4E-01	1.5E+00	4.8E+00					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T06-C	1	2.08E+02			2.08E+02	6.2E-01	1.5E+00	4.8E+00					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T07-C	1	2.06E+02			2.06E+02	1.7E+00	1.5E+00	4.8E+00					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T08-C	1	1.26E+02			1.26E+02	2.8E-01	1.5E+00	4.8E+00					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T09-C	1	1.42E+03			1.42E+03	1.4E+00	1.5E+00	4.8E+00					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-B01-A	1	7.50E-01	U1/2		7.50E-01	5.5E+01	1.5E+00	4.8E+00					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-B02-A	1	1.67E+00	E		1.67E+00	1.1E+01	1.5E+00	4.8E+00					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-B03-A	1	1.62E+00	E		1.62E+00	3.9E+01	1.5E+00	4.8E+00					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	SWA-LRef-1313-T01-A	1	1.12E+01			1.12E+01	2.3E+02	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:10 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T02-A	1	5.00E-01	U1/2		5.00E-01	1.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:12 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T03-A	1	5.00E-01	U1/2		5.00E-01	8.3E+00	1.0E+00	3.2E+00	10	100	1.14E+03	114%	VU ICP-OES	11/19/10 1:13 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T04-A	1	5.00E-01	U1/2		5.00E-01	3.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:15 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T05-A	1	5.00E-01	U1/2		5.00E-01	8.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:17 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T06-A	1	1.12E+01			1.12E+01	6.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:18 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T07-A	1	6.72E+02			6.72E+02	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:20 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T08-A	1	1.35E+03			1.35E+03	9.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:22 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T09-A	1	2.24E+03			2.24E+03	9.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:23 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T01-B	1	1.48E+02			1.48E+02	6.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:30 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T02-B	1	5.00E-01	U1/2		5.00E-01	6.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:32 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T03-B	1	5.00E-01	U1/2		5.00E-01	1.0E+02	1.0E+00	3.2E+00	10	100	1.13E+03	113%	VU ICP-OES	11/19/10 1:33 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T04-B	1	5.00E-01	U1/2		5.00E-01	6.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:35 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T05-B	1	5.00E-01	U1/2		5.00E-01	3.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:36 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T06-B	1	1.35E+01			1.35E+01	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:38 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T07-B	1	2.77E+02			2.77E+02	1.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:40 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T08-B	1	1.41E+03			1.41E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:41 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T09-B	1	2.54E+03			2.54E+03	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:43 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T01-C	1	5.00E-01	U1/2		5.00E-01	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:50 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T02-C	1	5.00E-01	U1/2		5.00E-01	7.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 1:51 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T03-C	1	5.00E-01	U1/2		5.00E-01	1.2E+01	1.0E+00	3.2E+00	10	100	1.13E+03	113%	VU ICP-OES	11/19/10 1:53 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T04-C	1	5.00E-01	U1/2		5.00E-01	2.3E+00	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:55 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T05-C	1	5.00E-01	U1/2		5.00E-01	3.6E+01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:56 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T06-C	1	5.16E+00			5.16E+00	9.7E+00	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:58 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T07-C	1	6.46E+02			6.46E+02	4.0E-01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 2:00 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T08-C	1	1.33E+03			1.33E+03	7.6E-01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 2:01 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T09-C	1	2.53E+03			2.53E+03	4.2E+00	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 2:03 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	6.8E+01	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:05 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-B02-A	1	2.37E+00	E		2.37E+00	8.3E+00	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:07 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-B03-A	1	3.48E+00			3.48E+00	9.4E+00	1.0E+00	3.2E+00					VU ICP-OES	11/19/10 1:09 PM	EPA Interlab LRef 1313-1316 SWA

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	SWA-LRef-1313-T01-D	1	6.16E+04			6.16E+04	3.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T02-D	1	3.89E+04			3.89E+04	6.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T03-D	1	2.16E+04			2.16E+04	1.3E-01	1.0E+00	3.2E+00	1000	100	2.26E+04	104%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T04-D	1	1.30E+02			1.30E+02	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T05-D	1	6.84E+01			6.84E+01	1.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T06-D	1	2.36E+01			2.36E+01	1.1E+02	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T07-D	1	8.07E+03			8.07E+03	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T08-D	1	2.65E+05			2.65E+05	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T09-D	1	3.38E+05			3.38E+05	9.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T01-E	1	6.07E+04			6.07E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T02-E	1	3.55E+04			3.55E+04	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T03-E	1	2.40E+04			2.40E+04	6.1E-01	1.0E+00	3.2E+00	1000	100	2.51E+04	111%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T04-E	1	9.41E+01			9.41E+01	9.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T05-E	1	6.62E+01			6.62E+01	9.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T06-E	1	2.98E+01			2.98E+01	5.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T07-E	1	8.12E+01			8.12E+01	1.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T08-E	1	2.18E+05			2.18E+05	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T09-E	1	3.43E+05			3.43E+05	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T01-F	1	5.80E+04			5.80E+04	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T02-F	1	3.47E+04			3.47E+04	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T03-F	1	2.24E+04			2.24E+04	4.3E-02	1.0E+00	3.2E+00	1000	100	2.34E+04	101%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T04-F	1	9.56E+01			9.56E+01	5.3E-01	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T05-F	1	7.83E+01			7.83E+01	7.3E+00	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T06-F	1	4.06E+01			4.06E+01	8.2E+00	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T07-F	1	2.41E+01			2.41E+01	6.4E+02	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T08-F	1	1.97E+05			1.97E+05	3.6E-01	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1313-T09-F	1	3.56E+05			3.56E+05	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	SWA-LRef-1313-T01-D	1	5.60E+03			5.60E+03	9.2E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T02-D	1	5.74E+03			5.74E+03	2.5E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T03-D	1	5.15E+03			5.15E+03	3.0E-01	7.5E+00	2.4E+01	10	100	6.29E+03	114%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T04-D	1	1.29E+03			1.29E+03	2.4E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T05-D	1	1.03E+03			1.03E+03	1.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T06-D	1	1.35E+03			1.35E+03	1.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T07-D	1	7.83E+02			7.83E+02	1.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T08-D	1	9.00E+02			9.00E+02	6.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T09-D	1	4.96E+02			4.96E+02	1.9E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T01-E	1	6.33E+03			6.33E+03	6.4E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T02-E	1	5.74E+03			5.74E+03	2.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T03-E	1	5.44E+03			5.44E+03	3.2E-01	7.5E+00	2.4E+01	10	100	6.61E+03	117%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T04-E	1	1.29E+03			1.29E+03	1.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T05-E	1	9.10E+02			9.10E+02	3.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T06-E	1	7.43E+02			7.43E+02	1.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T07-E	1	5.79E+02			5.79E+02	2.9E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T08-E	1	1.04E+03			1.04E+03	2.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T09-E	1	3.93E+02			3.93E+02	1.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T01-F	1	6.02E+03			6.02E+03	7.4E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T02-F	1	5.66E+03			5.66E+03	4.7E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T03-F	1	1.38E+03			1.38E+03	5.0E-01	7.5E+00	2.4E+01	10	100	2.32E+03	95%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T04-F	1	1.00E+03			1.00E+03	2.7E+00	7.5E+00	2.4E+01					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T05-F	1	1.11E+03			1.11E+03	2.4E+00	7.5E+00	2.4E+01					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T06-F	1	8.75E+02			8.75E+02	5.3E-01	7.5E+00	2.4E+01					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T07-F	1	6.62E+02			6.62E+02	3.6E+00	7.5E+00	2.4E+01					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T08-F	1	1.03E+03			1.03E+03	2.4E+00	7.5E+00	2.4E+01					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1313-T09-F	1	3.84E+02			3.84E+02	6.0E-01	7.5E+00	2.4E+01					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	SWA-LRef-1313-T01-D	1	8.80E+03			8.80E+03	7.0E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T02-D	1	4.79E+03			4.79E+03	6.1E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T03-D	1	2.41E+03			2.41E+03	7.5E-01	1.1E+01	3.5E+01	10	100	3.34E+03	93%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T04-D	1	4.53E+02			4.53E+02	1.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T05-D	1	3.15E+02			3.15E+02	4.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T06-D	1	2.48E+02			2.48E+02	1.2E+01	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T07-D	1	4.42E+02			4.42E+02	6.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T08-D	1	3.37E+03			3.37E+03	3.2E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T09-D	1	5.21E+03			5.21E+03	4.6E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T01-E	1	1.08E+04			1.08E+04	8.2E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T02-E	1	4.95E+03			4.95E+03	1.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T03-E	1	3.17E+03			3.17E+03	9.9E-01	1.1E+01	3.5E+01	10	100	4.09E+03	92%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T04-E	1	2.39E+02			2.39E+02	1.0E+01	1.1E+01	3.5E+01				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T05-E	1	3.33E+02			3.33E+02	2.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T06-E	1	2.41E+02			2.41E+02	5.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T07-E	1	1.67E+02			1.67E+02	3.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T08-E	1	3.11E+03			3.11E+03	2.2E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T09-E	1	6.90E+03			6.90E+03	1.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T01-F	1	1.01E+04			1.01E+04	8.1E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T02-F	1	4.37E+03			4.37E+03	4.6E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T03-F	1	2.51E+03			2.51E+03	4.7E-01	1.1E+01	3.5E+01	10	100	3.38E+03	87%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T04-F	1	5.27E+02			5.27E+02	3.9E+00	1.1E+01	3.5E+01					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T05-F	1	3.80E+02			3.80E+02	3.2E+00	1.1E+01	3.5E+01					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T06-F	1	2.77E+02			2.77E+02	6.7E+00	1.1E+01	3.5E+01					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T07-F	1	1.80E+02			1.80E+02	4.3E+00	1.1E+01	3.5E+01					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T08-F	1	3.06E+03			3.06E+03	3.9E-01	1.1E+01	3.5E+01					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1313-T09-F	1	7.04E+03			7.04E+03	1.9E+00	1.1E+01	3.5E+01					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	SWA-LRef-1313-T01-D	1	1.10E+03			1.10E+03	7.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T02-D	1	1.05E+03			1.05E+03	9.3E-02	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T03-D	1	8.84E+02			8.84E+02	5.4E-01	1.0E+00	3.2E+00	1000	100	1.88E+03	100%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T04-D	1	1.73E+03			1.73E+03	9.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T05-D	1	3.19E+03			3.19E+03	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T06-D	1	3.92E+03			3.92E+03	3.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T07-D	1	5.74E+03			5.74E+03	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T08-D	1	6.79E+03			6.79E+03	6.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T09-D	1	7.18E+03			7.18E+03	9.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T01-E	1	1.19E+03			1.19E+03	5.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T02-E	1	1.05E+03			1.05E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T03-E	1	9.71E+02			9.71E+02	1.3E-01	1.0E+00	3.2E+00	1000	100	1.93E+03	96%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T04-E	1	1.39E+03			1.39E+03	4.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T05-E	1	2.46E+03			2.46E+03	6.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T06-E	1	3.58E+03			3.58E+03	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T07-E	1	5.78E+03			5.78E+03	6.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T08-E	1	7.12E+03			7.12E+03	6.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T09-E	1	6.99E+03			6.99E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T01-F	1	1.16E+03			1.16E+03	8.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T02-F	1	9.77E+02			9.77E+02	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T03-F	1	9.21E+02			9.21E+02	7.6E-01	1.0E+00	3.2E+00	1000	100	1.85E+03	92%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T04-F	1	1.82E+03			1.82E+03	6.4E-01	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T05-F	1	2.42E+03			2.42E+03	8.8E-01	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T06-F	1	3.59E+03			3.59E+03	2.9E-01	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T07-F	1	5.63E+03			5.63E+03	5.0E-01	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T08-F	1	7.29E+03			7.29E+03	5.2E-01	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1313-T09-F	1	6.84E+03			6.84E+03	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	SWA-LRef-1313-T01-D	1	2.19E+02			2.19E+02	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T02-D	1	1.62E+02			1.62E+02	2.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T03-D	1	1.68E+02			1.68E+02	3.4E-01	1.0E+00	3.2E+00	10	100	1.22E+03	105%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T04-D	1	1.01E+03			1.01E+03	9.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T05-D	1	1.14E+03			1.14E+03	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T06-D	1	1.15E+03			1.15E+03	4.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T07-D	1	1.53E+03			1.53E+03	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T08-D	1	8.96E+02			8.96E+02	3.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T09-D	1	9.05E+02			9.05E+02	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T01-E	1	1.94E+02			1.94E+02	8.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T02-E	1	1.51E+02			1.51E+02	6.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T03-E	1	1.65E+02			1.65E+02	5.5E-01	1.0E+00	3.2E+00	10	100	1.16E+03	100%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T04-E	1	1.16E+03			1.16E+03	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T05-E	1	1.10E+03			1.10E+03	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T06-E	1	1.19E+03			1.19E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T07-E	1	1.68E+03			1.68E+03	7.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T08-E	1	9.57E+02			9.57E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T09-E	1	1.02E+03			1.02E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T01-F	1	2.81E+01			2.81E+01	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T02-F	1	1.60E+02			1.60E+02	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T03-F	1	2.03E+02			2.03E+02	2.9E-01	1.0E+00	3.2E+00	10	100	1.14E+03	93%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T04-F	1	9.49E+02			9.49E+02	6.2E-01	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T05-F	1	1.12E+03			1.12E+03	5.0E-01	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T06-F	1	1.22E+03			1.22E+03	2.8E-01	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T07-F	1	1.67E+03			1.67E+03	4.0E-01	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T08-F	1	1.02E+03			1.02E+03	4.1E-01	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1313-T09-F	1	9.36E+02			9.36E+02	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	SWA-LRef-1313-T01-D	1	9.50E-01	U1/2		9.50E-01	2.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T02-D	1	9.50E-01	U1/2		9.50E-01	1.9E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T03-D	1	9.50E-01	U1/2		9.50E-01	4.2E+02	1.9E+00	6.0E+00	10	100	1.10E+03	110%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T04-D	1	9.50E-01	U1/2		9.50E-01	6.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T05-D	1	9.50E-01	U1/2		9.50E-01	6.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T06-D	1	9.50E-01	U1/2		9.50E-01	9.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T07-D	1	9.50E-01	U1/2		9.50E-01	1.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T08-D	1	3.35E+01			3.35E+01	2.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T09-D	1	1.37E+02			1.37E+02	7.6E-01	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T01-E	1	9.50E-01	U1/2		9.50E-01	8.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T02-E	1	9.50E-01	U1/2		9.50E-01	2.1E+03	1.9E+00	6.0E+00				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T03-E	1	9.50E-01	U1/2		9.50E-01	1.5E+04	1.9E+00	6.0E+00	10	100	1.07E+03	107%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T04-E	1	9.50E-01	U1/2		9.50E-01	1.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T05-E	1	9.50E-01	U1/2		9.50E-01	2.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T06-E	1	9.50E-01	U1/2		9.50E-01	3.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T07-E	1	9.50E-01	U1/2		9.50E-01	2.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T08-E	1	1.24E+01			1.24E+01	8.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T09-E	1	1.39E+02			1.39E+02	4.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T01-F	1	9.50E-01	U1/2		9.50E-01	1.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T02-F	1	9.50E-01	U1/2		9.50E-01	2.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T03-F	1	9.50E-01	U1/2		9.50E-01	7.6E+02	1.9E+00	6.0E+00	10	100	9.99E+02	100%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T04-F	1	9.50E-01	U1/2		9.50E-01	6.6E+01	1.9E+00	6.0E+00					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T05-F	1	9.50E-01	U1/2		9.50E-01	1.0E+02	1.9E+00	6.0E+00					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T06-F	1	9.50E-01	U1/2		9.50E-01	9.7E+01	1.9E+00	6.0E+00					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T07-F	1	9.50E-01	U1/2		9.50E-01	5.5E+01	1.9E+00	6.0E+00					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T08-F	1	8.17E+00			8.17E+00	3.3E+01	1.9E+00	6.0E+00					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1313-T09-F	1	1.31E+02			1.31E+02	1.1E+00	1.9E+00	6.0E+00					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	SWA-LRef-1313-T01-D	1	1.10E+00	U1/2		1.10E+00	2.1E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T02-D	1	1.10E+00	U1/2		1.10E+00	5.9E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T03-D	1	1.10E+00	U1/2		1.10E+00	4.2E+01	2.2E+00	7.0E+00	10	100	1.06E+03	106%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T04-D	1	1.10E+00	U1/2		1.10E+00	1.6E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T05-D	1	1.10E+00	U1/2		1.10E+00	5.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T06-D	1	1.10E+00	U1/2		1.10E+00	6.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T07-D	1	1.49E+01			1.49E+01	1.2E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T08-D	1	1.78E+01			1.78E+01	1.6E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T09-D	1	4.21E+01			4.21E+01	3.4E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T01-E	1	1.10E+00	U1/2		1.10E+00	1.6E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T02-E	1	1.10E+00	U1/2		1.10E+00	2.7E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T03-E	1	1.10E+00	U1/2		1.10E+00	2.4E+02	2.2E+00	7.0E+00	10	100	1.05E+03	105%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T04-E	1	1.10E+00	U1/2		1.10E+00	4.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T05-E	1	1.10E+00	U1/2		1.10E+00	6.3E+01	2.2E+00	7.0E+00				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T06-E	1	1.10E+00	U1/2		1.10E+00	6.2E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T07-E	1	1.06E+01			1.06E+01	1.6E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T08-E	1	1.55E+01			1.55E+01	8.1E-01	2.2E+00	7.0E+00				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T09-E	1	4.30E+01			4.30E+01	1.2E+00	2.2E+00	7.0E+00				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T01-F	1	1.10E+00	U1/2		1.10E+00	1.6E+02	2.2E+00	7.0E+00				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T02-F	1	1.10E+00	U1/2		1.10E+00	2.3E+03	2.2E+00	7.0E+00				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T03-F	1	1.10E+00	U1/2		1.10E+00	9.2E+02	2.2E+00	7.0E+00	10	100	9.84E+02	98%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T04-F	1	1.10E+00	U1/2		1.10E+00	9.7E+00	2.2E+00	7.0E+00					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T05-F	1	1.10E+00	U1/2		1.10E+00	7.4E+01	2.2E+00	7.0E+00					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T06-F	1	1.10E+00	U1/2		1.10E+00	6.1E+01	2.2E+00	7.0E+00					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T07-F	1	7.68E+00			7.68E+00	8.0E+00	2.2E+00	7.0E+00					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T08-F	1	1.50E+01			1.50E+01	1.8E+00	2.2E+00	7.0E+00					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1313-T09-F	1	3.88E+01			3.88E+01	1.9E+00	2.2E+00	7.0E+00					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	SWA-LRef-1313-T01-D	1	7.57E+03			7.57E+03	1.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T02-D	1	1.46E+04			1.46E+04	1.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T03-D	1	2.26E+04			2.26E+04	3.1E-01	2.6E+00	8.3E+00	1000	100	2.35E+04	90%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T04-D	1	4.95E+06			4.95E+06	8.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T05-D	1	7.39E+06			7.39E+06	9.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T06-D	1	7.30E+06			7.30E+06	5.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T07-D	1	7.80E+06			7.80E+06	9.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T08-D	1	5.14E+06			5.14E+06	1.5E+00	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T09-D	1	3.55E+06			3.55E+06	7.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T01-E	1	7.52E+03			7.52E+03	7.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T02-E	1	1.35E+04			1.35E+04	1.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T03-E	1	2.15E+04			2.15E+04	4.8E-01	2.6E+00	8.3E+00	1000	100	2.24E+04	89%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T04-E	1	4.35E+06			4.35E+06	7.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T05-E	1	6.76E+06			6.76E+06	4.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T06-E	1	7.36E+06			7.36E+06	7.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T07-E	1	8.87E+06			8.87E+06	8.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T08-E	1	5.43E+06			5.43E+06	5.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T09-E	1	3.58E+06			3.58E+06	1.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T01-F	1	4.62E+03			4.62E+03	1.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T02-F	1	1.43E+04			1.43E+04	4.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T03-F	1	2.32E+04			2.32E+04	3.0E-01	2.6E+00	8.3E+00	1000	100	2.41E+04	85%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T04-F	1	5.16E+06			5.16E+06	8.6E-01	2.6E+00	8.3E+00					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T05-F	1	6.78E+06			6.78E+06	1.1E+00	2.6E+00	8.3E+00					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T06-F	1	7.34E+06			7.34E+06	4.9E-01	2.6E+00	8.3E+00					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T07-F	1	9.14E+06			9.14E+06	6.2E-01	2.6E+00	8.3E+00					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T08-F	1	5.71E+06			5.71E+06	1.1E+00	2.6E+00	8.3E+00					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1313-T09-F	1	3.59E+06			3.59E+06	3.3E-01	2.6E+00	8.3E+00					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	SWA-LRef-1313-T01-D	1	1.19E+03			1.19E+03	2.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T02-D	1	1.36E+03			1.36E+03	3.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T03-D	1	3.93E+02			3.93E+02	3.9E-01	1.2E+00	3.8E+00	10	100	1.44E+03	105%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T04-D	1	4.26E+00			4.26E+00	2.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T05-D	1	6.00E-01	U1/2		6.00E-01	8.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T06-D	1	6.00E-01	U1/2		6.00E-01	9.7E+02	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T07-D	1	7.90E+00			7.90E+00	2.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T08-D	1	3.66E+03			3.66E+03	9.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T09-D	1	1.95E+04			1.95E+04	4.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T01-E	1	1.54E+03			1.54E+03	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T02-E	1	1.19E+03			1.19E+03	9.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T03-E	1	4.46E+02			4.46E+02	8.1E-01	1.2E+00	3.8E+00	10	100	1.42E+03	97%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T04-E	1	2.48E+00	E		2.48E+00	4.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T05-E	1	3.54E+00	E		3.54E+00	2.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T06-E	1	6.00E-01	U1/2		6.00E-01	2.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T07-E	1	3.87E+00			3.87E+00	1.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T08-E	1	2.17E+03			2.17E+03	4.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T09-E	1	1.79E+04			1.79E+04	7.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T01-F	1	7.95E+02			7.95E+02	1.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T02-F	1	1.15E+03			1.15E+03	9.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T03-F	1	3.69E+02			3.69E+02	9.7E-01	1.2E+00	3.8E+00	10	100	1.29E+03	92%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T04-F	1	6.39E+00			6.39E+00	5.0E-01	1.2E+00	3.8E+00					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T05-F	1	4.02E+00			4.02E+00	7.6E+00	1.2E+00	3.8E+00					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T06-F	1	6.00E-01	U1/2		6.00E-01	2.2E+01	1.2E+00	3.8E+00					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T07-F	1	3.73E+00	E		3.73E+00	1.1E+02	1.2E+00	3.8E+00					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T08-F	1	1.59E+03			1.59E+03	4.2E-01	1.2E+00	3.8E+00					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1313-T09-F	1	1.84E+04			1.84E+04	1.1E+00	1.2E+00	3.8E+00					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	SWA-LRef-1313-T01-D	1	9.00E-01	U1/2		9.00E-01	6.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T02-D	1	9.00E-01	U1/2		9.00E-01	9.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T03-D	1	9.00E-01	U1/2		9.00E-01	1.3E+01	1.8E+00	5.7E+00	10	100	1.03E+03	103%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T04-D	1	2.15E+00	E		2.15E+00	3.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T05-D	1	1.43E+01			1.43E+01	6.9E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T06-D	1	3.12E+01			3.12E+01	8.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T07-D	1	2.07E+02			2.07E+02	1.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T08-D	1	1.84E+02			1.84E+02	1.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T09-D	1	2.62E+02			2.62E+02	2.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T01-E	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T02-E	1	9.00E-01	U1/2		9.00E-01	1.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T03-E	1	9.00E-01	U1/2		9.00E-01	4.8E+01	1.8E+00	5.7E+00	10	100	9.82E+02	98%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T04-E	1	2.50E+00	E		2.50E+00	7.6E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T05-E	1	6.50E+00			6.50E+00	8.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T06-E	1	3.45E+01			3.45E+01	4.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T07-E	1	2.00E+02			2.00E+02	7.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T08-E	1	1.86E+02			1.86E+02	5.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T09-E	1	2.59E+02			2.59E+02	1.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T01-F	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T02-F	1	9.00E-01	U1/2		9.00E-01	2.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T03-F	1	9.00E-01	U1/2		9.00E-01	6.9E+02	1.8E+00	5.7E+00	10	100	9.18E+02	92%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T04-F	1	2.23E+00	E		2.23E+00	6.3E+01	1.8E+00	5.7E+00					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T05-F	1	5.05E+00	E		5.05E+00	1.7E+01	1.8E+00	5.7E+00					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T06-F	1	4.73E+01			4.73E+01	3.8E+00	1.8E+00	5.7E+00					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T07-F	1	1.76E+02			1.76E+02	1.3E+00	1.8E+00	5.7E+00					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T08-F	1	1.93E+02			1.93E+02	4.5E-01	1.8E+00	5.7E+00					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1313-T09-F	1	2.45E+02			2.45E+02	1.9E+00	1.8E+00	5.7E+00					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	SWA-LRef-1313-T01-D	1	1.85E+00	U1/2		1.85E+00	1.8E+03	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T02-D	1	1.85E+00	U1/2		1.85E+00	4.9E+02	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T03-D	1	1.85E+00	U1/2		1.85E+00	3.8E+03	3.7E+00	1.2E+01	10	100	1.04E+03	104%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T04-D	1	7.29E+00	E		7.29E+00	1.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T05-D	1	1.03E+01	E		1.03E+01	4.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T06-D	1	1.07E+01	E		1.07E+01	2.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T07-D	1	1.53E+01			1.53E+01	2.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T08-D	1	2.76E+01			2.76E+01	5.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T09-D	1	1.40E+03			1.40E+03	6.0E-01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T01-E	1	1.85E+00	U1/2		1.85E+00	4.3E+02	3.7E+00	1.2E+01				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T02-E	1	1.85E+00	U1/2		1.85E+00	7.5E+03	3.7E+00	1.2E+01				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T03-E	1	1.85E+00	U1/2		1.85E+00	2.0E+01	3.7E+00	1.2E+01	10	100	9.82E+02	98%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T04-E	1	8.03E+00	E		8.03E+00	4.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T05-E	1	9.48E+00	E		9.48E+00	2.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T06-E	1	6.43E+00	E		6.43E+00	8.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T07-E	1	1.43E+01			1.43E+01	2.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T08-E	1	1.52E+01			1.52E+01	9.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T09-E	1	1.39E+03			1.39E+03	1.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T01-F	1	1.85E+00	U1/2		1.85E+00	3.3E+02	3.7E+00	1.2E+01				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T02-F	1	1.85E+00	U1/2		1.85E+00	9.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T03-F	1	1.85E+00	U1/2		1.85E+00	4.7E+01	3.7E+00	1.2E+01	10	100	9.23E+02	92%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T04-F	1	9.43E+00	E		9.43E+00	5.4E+01	3.7E+00	1.2E+01					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T05-F	1	6.29E+00	E		6.29E+00	2.8E+01	3.7E+00	1.2E+01					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T06-F	1	1.04E+01	E		1.04E+01	6.3E+00	3.7E+00	1.2E+01					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T07-F	1	1.56E+01			1.56E+01	4.3E+00	3.7E+00	1.2E+01					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T08-F	1	1.34E+01			1.34E+01	1.3E+01	3.7E+00	1.2E+01					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1313-T09-F	1	1.38E+03			1.38E+03	6.6E-01	3.7E+00	1.2E+01					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	SWA-LRef-1313-T01-D	1	6.99E+01			6.99E+01	3.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T02-D	1	9.37E+01			9.37E+01	1.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T03-D	1	6.59E+01			6.59E+01	8.0E-01	2.0E+00	6.4E+00	1000	100	1.13E+03	107%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T04-D	1	2.66E+01			2.66E+01	3.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T05-D	1	7.68E+01			7.68E+01	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T06-D	1	3.29E+01			3.29E+01	2.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T07-D	1	1.31E+05			1.31E+05	7.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T08-D	1	1.28E+05			1.28E+05	2.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T09-D	1	1.62E+05			1.62E+05	3.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T01-E	1	9.22E+01			9.22E+01	1.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T02-E	1	8.39E+01			8.39E+01	9.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T03-E	1	7.69E+01			7.69E+01	7.6E-01	2.0E+00	6.4E+00	1000	100	1.09E+03	101%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T04-E	1	1.55E+01			1.55E+01	2.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T05-E	1	4.61E+01			4.61E+01	1.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T06-E	1	6.31E+01			6.31E+01	1.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T07-E	1	9.92E+04			9.92E+04	3.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T08-E	1	1.23E+05			1.23E+05	3.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T09-E	1	1.69E+05			1.69E+05	2.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T01-F	1	4.48E+01			4.48E+01	8.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T02-F	1	7.35E+01			7.35E+01	1.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T03-F	1	6.80E+01			6.80E+01	1.1E+00	2.0E+00	6.4E+00	1000	100	1.01E+03	95%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T04-F	1	2.26E+01			2.26E+01	7.6E-02	2.0E+00	6.4E+00					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T05-F	1	6.93E+01			6.93E+01	2.2E+00	2.0E+00	6.4E+00					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T06-F	1	2.38E+02			2.38E+02	1.0E+00	2.0E+00	6.4E+00					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T07-F	1	7.27E+04			7.27E+04	8.4E-01	2.0E+00	6.4E+00					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T08-F	1	1.23E+05			1.23E+05	9.9E-01	2.0E+00	6.4E+00					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1313-T09-F	1	1.70E+05			1.70E+05	1.2E+00	2.0E+00	6.4E+00					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	SWA-LRef-1313-T01-D	1	3.63E+01			3.63E+01	1.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T02-D	1	1.37E+01	E		1.37E+01	3.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T03-D	1	1.10E+01	E		1.10E+01	5.6E+01	6.8E+00	2.2E+01	10	100	1.00E+03	99%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T04-D	1	3.40E+00	U1/2		3.40E+00	1.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T05-D	1	3.40E+00	U1/2		3.40E+00	3.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T06-D	1	3.40E+00	U1/2		3.40E+00	6.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T07-D	1	3.40E+00	U1/2		3.40E+00	1.4E+02	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T08-D	1	1.57E+02			1.57E+02	8.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T09-D	1	3.83E+03			3.83E+03	1.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T01-E	1	4.82E+01			4.82E+01	1.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T02-E	1	9.97E+00	E		9.97E+00	5.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T03-E	1	8.07E+00	E		8.07E+00	5.2E+01	6.8E+00	2.2E+01	10	100	9.53E+02	94%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T04-E	1	3.40E+00	U1/2		3.40E+00	2.2E+02	6.8E+00	2.2E+01				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T05-E	1	3.40E+00	U1/2		3.40E+00	1.5E+02	6.8E+00	2.2E+01				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T06-E	1	3.40E+00	U1/2		3.40E+00	7.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T07-E	1	3.40E+00	U1/2		3.40E+00	8.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T08-E	1	5.50E+01			5.50E+01	7.8E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T09-E	1	3.38E+03			3.38E+03	1.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T01-F	1	4.15E+01			4.15E+01	6.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T02-F	1	1.60E+01	E		1.60E+01	1.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T03-F	1	7.36E+00	E		7.36E+00	1.6E+02	6.8E+00	2.2E+01	10	100	9.01E+02	89%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T04-F	1	3.40E+00	U1/2		3.40E+00	6.7E+01	6.8E+00	2.2E+01					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T05-F	1	3.40E+00	U1/2		3.40E+00	2.4E+01	6.8E+00	2.2E+01					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T06-F	1	3.40E+00	U1/2		3.40E+00	3.0E+01	6.8E+00	2.2E+01					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T07-F	1	3.40E+00	U1/2		3.40E+00	6.6E+01	6.8E+00	2.2E+01					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T08-F	1	2.66E+01			2.66E+01	3.3E+01	6.8E+00	2.2E+01					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1313-T09-F	1	3.22E+03			3.22E+03	9.8E-01	6.8E+00	2.2E+01					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	SWA-LRef-1313-T01-D	1	9.50E-01	U1/2		9.50E-01	2.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T02-D	1	9.50E-01	U1/2		9.50E-01	1.9E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T03-D	1	9.50E-01	U1/2		9.50E-01	2.1E+01	1.9E+00	6.0E+00	10	100	8.68E+02	87%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T04-D	1	5.96E+02			5.96E+02	4.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T05-D	1	1.13E+03			1.13E+03	4.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T06-D	1	1.12E+03			1.12E+03	1.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T07-D	1	1.25E+03			1.25E+03	7.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T08-D	1	9.10E+02			9.10E+02	3.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T09-D	1	9.81E+02			9.81E+02	1.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T01-E	1	9.50E-01	U1/2		9.50E-01	3.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T02-E	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T03-E	1	9.50E-01	U1/2		9.50E-01	3.4E+02	1.9E+00	6.0E+00	10	100	8.51E+02	85%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T04-E	1	4.51E+02			4.51E+02	4.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T05-E	1	9.92E+02			9.92E+02	2.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T06-E	1	1.12E+03			1.12E+03	2.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T07-E	1	1.36E+03			1.36E+03	4.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T08-E	1	9.80E+02			9.80E+02	1.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T09-E	1	9.81E+02			9.81E+02	6.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T01-F	1	9.50E-01	U1/2		9.50E-01	4.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T02-F	1	9.50E-01	U1/2		9.50E-01	2.6E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T03-F	1	9.50E-01	U1/2		9.50E-01	5.7E+01	1.9E+00	6.0E+00	10	100	8.42E+02	84%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T04-F	1	6.75E+02			6.75E+02	1.9E+00	1.9E+00	6.0E+00					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T05-F	1	1.02E+03			1.02E+03	1.9E+00	1.9E+00	6.0E+00					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T06-F	1	1.12E+03			1.12E+03	5.1E+00	1.9E+00	6.0E+00					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T07-F	1	1.48E+03			1.48E+03	2.7E+00	1.9E+00	6.0E+00					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T08-F	1	1.08E+03			1.08E+03	4.5E+00	1.9E+00	6.0E+00					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1313-T09-F	1	9.58E+02			9.58E+02	3.9E+00	1.9E+00	6.0E+00					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	SWA-LRef-1313-T01-D	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T02-D	1	1.00E+00	U1/2		1.00E+00	8.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T03-D	1	1.00E+00	U1/2		1.00E+00	8.6E+00	2.0E+00	6.4E+00	10	100	1.05E+03	105%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T04-D	1	6.24E+01			6.24E+01	1.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T05-D	1	5.52E+03			5.52E+03	5.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T06-D	1	9.75E+03			9.75E+03	3.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T07-D	1	2.39E+04			2.39E+04	1.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T08-D	1	1.90E+04			1.90E+04	1.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T09-D	1	2.06E+04			2.06E+04	5.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T01-E	1	1.00E+00	U1/2		1.00E+00	8.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T02-E	1	1.00E+00	U1/2		1.00E+00	9.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T03-E	1	1.00E+00	U1/2		1.00E+00	7.9E+00	2.0E+00	6.4E+00	10	100	9.93E+02	99%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T04-E	1	4.53E+01			4.53E+01	4.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T05-E	1	2.79E+03			2.79E+03	3.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T06-E	1	9.68E+03			9.68E+03	1.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T07-E	1	2.53E+04			2.53E+04	4.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T08-E	1	1.98E+04			1.98E+04	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T09-E	1	2.06E+04			2.06E+04	3.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T01-F	1	1.00E+00	U1/2		1.00E+00	3.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T02-F	1	1.00E+00	U1/2		1.00E+00	2.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T03-F	1	1.00E+00	U1/2		1.00E+00	3.2E+00	2.0E+00	6.4E+00	10	100	9.25E+02	92%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T04-F	1	4.22E+02			4.22E+02	1.7E-01	2.0E+00	6.4E+00					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T05-F	1	2.22E+03			2.22E+03	6.3E-01	2.0E+00	6.4E+00					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T06-F	1	1.10E+04			1.10E+04	5.8E-01	2.0E+00	6.4E+00					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T07-F	1	2.43E+04			2.43E+04	4.1E-01	2.0E+00	6.4E+00					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T08-F	1	2.06E+04			2.06E+04	8.1E-01	2.0E+00	6.4E+00					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1313-T09-F	1	2.08E+04			2.08E+04	1.0E+00	2.0E+00	6.4E+00					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	SWA-LRef-1313-T01-D	1	1.11E+01			1.11E+01	1.0E+02	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T02-D	1	2.13E+01			2.13E+01	1.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T03-D	1	5.39E+00			5.39E+00	9.3E+01	1.0E+00	3.2E+00	1000	100	1.02E+03	102%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T04-D	1	5.22E+05			5.22E+05	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T05-D	1	1.12E+06			1.12E+06	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T06-D	1	1.17E+06			1.17E+06	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T07-D	1	1.31E+06			1.31E+06	1.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T08-D	1	9.09E+05			9.09E+05	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T09-D	1	8.29E+05			8.29E+05	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T01-E	1	5.07E+00			5.07E+00	1.8E+02	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T02-E	1	8.11E+00			8.11E+00	1.1E+02	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T03-E	1	8.88E+00			8.88E+00	5.8E+01	1.0E+00	3.2E+00	1000	100	9.80E+02	97%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T04-E	1	2.84E+05			2.84E+05	4.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T05-E	1	9.54E+05			9.54E+05	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T06-E	1	1.13E+06			1.13E+06	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T07-E	1	1.47E+06			1.47E+06	3.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T08-E	1	9.62E+05			9.62E+05	8.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T09-E	1	8.28E+05			8.28E+05	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T01-F	1	1.72E+01			1.72E+01	4.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T02-F	1	1.46E+01			1.46E+01	2.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T03-F	1	1.90E+01			1.90E+01	5.0E+01	1.0E+00	3.2E+00	1000	100	9.14E+02	89%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T04-F	1	6.16E+05			6.16E+05	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T05-F	1	9.42E+05			9.42E+05	2.0E-01	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T06-F	1	1.11E+06			1.11E+06	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T07-F	1	1.52E+06			1.52E+06	6.3E-01	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T08-F	1	1.02E+06			1.02E+06	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1313-T09-F	1	8.33E+05			8.33E+05	9.0E-01	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	SWA-LRef-1313-T01-D	1	1.27E+02			1.27E+02	1.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T02-D	1	1.44E+02			1.44E+02	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T03-D	1	1.39E+02			1.39E+02	4.9E-01	1.2E+00	3.8E+00	10	100	1.18E+03	104%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T04-D	1	1.33E+02			1.33E+02	2.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T05-D	1	1.15E+02			1.15E+02	2.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T06-D	1	1.05E+02			1.05E+02	4.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T07-D	1	1.01E+01			1.01E+01	2.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T08-D	1	1.74E+01			1.74E+01	5.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T09-D	1	1.37E+01			1.37E+01	2.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T01-E	1	1.39E+02			1.39E+02	2.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T02-E	1	1.42E+02			1.42E+02	7.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T03-E	1	1.42E+02			1.42E+02	6.9E-01	1.2E+00	3.8E+00	10	100	1.10E+03	96%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T04-E	1	1.11E+02			1.11E+02	2.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T05-E	1	1.06E+02			1.06E+02	2.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T06-E	1	8.95E+01			8.95E+01	3.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T07-E	1	9.76E+00			9.76E+00	2.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T08-E	1	2.06E+01			2.06E+01	1.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T09-E	1	1.66E+01			1.66E+01	1.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T01-F	1	1.33E+02			1.33E+02	2.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T02-F	1	1.35E+02			1.35E+02	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T03-F	1	1.24E+02			1.24E+02	6.1E-02	1.2E+00	3.8E+00	10	100	1.04E+03	92%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T04-F	1	1.00E+02			1.00E+02	3.0E+00	1.2E+00	3.8E+00					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T05-F	1	1.09E+02			1.09E+02	2.5E+00	1.2E+00	3.8E+00					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T06-F	1	7.58E+01			7.58E+01	4.6E+00	1.2E+00	3.8E+00					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T07-F	1	1.31E+01			1.31E+01	7.7E+00	1.2E+00	3.8E+00					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T08-F	1	2.14E+01			2.14E+01	9.4E+00	1.2E+00	3.8E+00					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1313-T09-F	1	1.62E+01			1.62E+01	1.1E+00	1.2E+00	3.8E+00					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	SWA-LRef-1313-T01-D	1	9.00E-01	U1/2		9.00E-01	3.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T02-D	1	9.00E-01	U1/2		9.00E-01	9.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T03-D	1	9.00E-01	U1/2		9.00E-01	1.7E+02	1.8E+00	5.7E+00	10	100	1.02E+03	102%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T04-D	1	3.67E+00	E		3.67E+00	8.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T05-D	1	4.54E+01			4.54E+01	2.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T06-D	1	1.05E+02			1.05E+02	3.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T07-D	1	4.46E+02			4.46E+02	3.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T08-D	1	3.77E+02			3.77E+02	9.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T09-D	1	4.38E+02			4.38E+02	2.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T01-E	1	9.00E-01	U1/2		9.00E-01	7.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T02-E	1	9.00E-01	U1/2		9.00E-01	1.1E+03	1.8E+00	5.7E+00				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T03-E	1	9.00E-01	U1/2		9.00E-01	7.4E+01	1.8E+00	5.7E+00	10	100	9.83E+02	98%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T04-E	1	4.98E+00	E		4.98E+00	3.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T05-E	1	2.64E+01			2.64E+01	9.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T06-E	1	1.07E+02			1.07E+02	9.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T07-E	1	4.44E+02			4.44E+02	9.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T08-E	1	3.90E+02			3.90E+02	3.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T09-E	1	4.33E+02			4.33E+02	1.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T01-F		9.00E-01	U1/2		0.00E+00	4.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T02-F		9.00E-01	U1/2		0.00E+00	8.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T03-F		9.00E-01	U1/2		0.00E+00	7.0E+01	1.8E+00	5.7E+00	10	100	9.25E+02	92%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T04-F		7.26E+00	U1/2		0.00E+00	2.5E+01	1.8E+00	5.7E+00					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T05-F		2.20E+01	U1/2		0.00E+00	1.5E+01	1.8E+00	5.7E+00					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T06-F		1.35E+02	U1/2		0.00E+00	9.4E-01	1.8E+00	5.7E+00					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T07-F		3.98E+02	U1/2		0.00E+00	9.7E-01	1.8E+00	5.7E+00					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T08-F		4.12E+02	U1/2		0.00E+00	1.0E+00	1.8E+00	5.7E+00					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1313-T09-F		4.40E+02	U1/2		0.00E+00	9.4E-01	1.8E+00	5.7E+00					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	SWA-LRef-1313-T01-D	1	1.03E+02			1.03E+02	5.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T02-D	1	3.80E+01			3.80E+01	1.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T03-D	1	2.23E+01			2.23E+01	5.3E+01	3.7E+00	1.2E+01	1000	100	1.03E+03	101%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T04-D	1	6.18E+01			6.18E+01	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T05-D	1	5.90E+01			5.90E+01	3.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T06-D	1	6.83E+01			6.83E+01	3.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T07-D	1	6.25E+01			6.25E+01	3.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T08-D	1	8.32E+02			8.32E+02	1.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T09-D	1	1.08E+04			1.08E+04	5.7E-01	3.7E+00	1.2E+01				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T01-E	1	1.55E+02			1.55E+02	5.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T02-E	1	8.83E+01			8.83E+01	1.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T03-E	1	2.35E+01			2.35E+01	3.4E+01	3.7E+00	1.2E+01	1000	100	9.90E+02	97%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T04-E	1	6.74E+01			6.74E+01	4.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T05-E	1	5.93E+01			5.93E+01	3.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T06-E	1	7.85E+01			7.85E+01	1.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T07-E	1	2.41E+01			2.41E+01	9.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T08-E	1	8.23E+02			8.23E+02	2.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T09-E	1	1.16E+04			1.16E+04	2.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T01-F	1	1.36E+02			1.36E+02	4.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T02-F	1	3.62E+01			3.62E+01	4.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T03-F	1	2.16E+01			2.16E+01	5.3E+01	3.7E+00	1.2E+01	1000	100	1.03E+03	101%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T04-F	1	7.15E+01			7.15E+01	8.3E+00	3.7E+00	1.2E+01					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T05-F	1	6.24E+01			6.24E+01	1.4E+01	3.7E+00	1.2E+01					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T06-F	1	7.33E+01			7.33E+01	1.9E+01	3.7E+00	1.2E+01					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T07-F	1	1.81E+01			1.81E+01	6.0E+01	3.7E+00	1.2E+01					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T08-F	1	8.01E+02			8.01E+02	2.2E+00	3.7E+00	1.2E+01					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1313-T09-F	1	1.09E+04			1.09E+04	2.7E+00	3.7E+00	1.2E+01					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	SWA-LRef-1313-T01-D	1	2.27E+06			2.27E+06	4.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T02-D	1	2.95E+05			2.95E+05	4.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T03-D	1	2.84E+05			2.84E+05	4.2E-01	1.6E+00	5.1E+00	1000	100	2.85E+05	90%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T04-D	1	4.17E+05			4.17E+05	2.5E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T05-D	1	4.46E+05			4.46E+05	2.9E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T06-D	1	4.35E+05			4.35E+05	5.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T07-D	1	4.06E+05			4.06E+05	8.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T08-D	1	2.95E+05			2.95E+05	4.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T09-D	1	3.49E+05			3.49E+05	5.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T01-E	1	2.28E+06			2.28E+06	3.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T02-E	1	2.84E+05			2.84E+05	1.6E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T03-E	1	2.98E+05			2.98E+05	6.6E-01	1.6E+00	5.1E+00	1000	100	2.99E+05	86%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T04-E	1	4.17E+05			4.17E+05	7.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T05-E	1	4.38E+05			4.38E+05	4.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T06-E	1	4.48E+05			4.48E+05	4.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T07-E	1	4.58E+05			4.58E+05	9.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T08-E	1	3.20E+05			3.20E+05	6.4E+00	1.6E+00	5.1E+00				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T09-E	1	3.37E+05			3.37E+05	5.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T01-F	1	2.28E+06			2.28E+06	7.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T02-F	1	2.83E+05			2.83E+05	5.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T03-F	1	2.92E+05			2.92E+05	8.2E-01	1.6E+00	5.1E+00	1000	100	2.93E+05	82%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T04-F	1	4.15E+05			4.15E+05	5.8E-01	1.6E+00	5.1E+00					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T05-F	1	4.38E+05			4.38E+05	5.0E-01	1.6E+00	5.1E+00					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T06-F	1	4.48E+05			4.48E+05	4.7E-01	1.6E+00	5.1E+00					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T07-F	1	4.70E+05			4.70E+05	1.0E+00	1.6E+00	5.1E+00					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T08-F	1	3.12E+05			3.12E+05	2.5E+00	1.6E+00	5.1E+00					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1313-T09-F	1	3.27E+05			3.27E+05	6.2E-01	1.6E+00	5.1E+00					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	SWA-LRef-1313-T01-D	1	8.20E+04			8.20E+04	3.4E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T02-D	1	9.69E+04			9.69E+04	2.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T03-D	1	9.97E+04			9.97E+04	1.4E-01	1.5E+01	4.8E+01	10	100	1.01E+05	99%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T04-D	1	1.13E+05			1.13E+05	1.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T05-D	1	1.27E+05			1.27E+05	5.5E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T06-D	1	1.24E+05			1.24E+05	2.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T07-D	1	1.02E+05			1.02E+05	5.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T08-D	1	6.05E+04			6.05E+04	3.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T09-D	1	3.99E+04			3.99E+04	8.3E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T01-E	1	1.04E+05			1.04E+05	9.3E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T02-E	1	1.04E+05			1.04E+05	1.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T03-E	1	1.04E+05			1.04E+05	5.1E-01	1.5E+01	4.8E+01	10	100	1.05E+05	91%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T04-E	1	1.07E+05			1.07E+05	6.5E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T05-E	1	1.19E+05			1.19E+05	7.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T06-E	1	1.22E+05			1.22E+05	7.9E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T07-E	1	1.18E+05			1.18E+05	2.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T08-E	1	6.52E+04			6.52E+04	5.1E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T09-E	1	4.04E+04			4.04E+04	6.9E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T01-F	1	9.87E+04			9.87E+04	6.2E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T02-F	1	9.33E+04			9.33E+04	2.3E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T03-F	1	9.50E+04			9.50E+04	3.3E-01	1.5E+01	4.8E+01	10	100	9.59E+04	87%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T04-F	1	1.09E+05			1.09E+05	5.1E-01	1.5E+01	4.8E+01					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T05-F	1	1.21E+05			1.21E+05	4.1E-01	1.5E+01	4.8E+01					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T06-F	1	1.18E+05			1.18E+05	2.2E-01	1.5E+01	4.8E+01					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T07-F	1	1.27E+05			1.27E+05	6.1E-01	1.5E+01	4.8E+01					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T08-F	1	6.96E+04			6.96E+04	2.4E-01	1.5E+01	4.8E+01					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1313-T09-F	1	4.06E+04			4.06E+04	8.8E-01	1.5E+01	4.8E+01					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	SWA-LRef-1313-T01-D	1	7.09E+03			7.09E+03	3.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T02-D	1	5.68E+03			5.68E+03	3.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T03-D	1	5.04E+03			5.04E+03	6.7E-01	1.1E+00	3.5E+00	1000	100	6.09E+03	106%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T04-D	1	9.69E+02			9.69E+02	8.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T05-D	1	1.30E+03			1.30E+03	4.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T06-D	1	1.74E+03			1.74E+03	4.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T07-D	1	2.82E+03			2.82E+03	5.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T08-D	1	1.45E+04			1.45E+04	8.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T09-D	1	1.24E+04			1.24E+04	1.7E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T01-E	1	7.83E+03			7.83E+03	9.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T02-E	1	5.68E+03			5.68E+03	1.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T03-E	1	4.83E+03			4.83E+03	1.2E+00	1.1E+00	3.5E+00	1000	100	5.81E+03	99%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T04-E	1	1.09E+03			1.09E+03	5.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T05-E	1	1.01E+03			1.01E+03	4.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T06-E	1	1.59E+03			1.59E+03	9.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T07-E	1	2.34E+03			2.34E+03	2.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T08-E	1	1.68E+04			1.68E+04	7.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T09-E	1	1.53E+04			1.53E+04	4.5E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T01-F	1	3.95E+03			3.95E+03	5.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T02-F	1	5.46E+03			5.46E+03	1.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T03-F	1	4.74E+03			4.74E+03	3.2E-01	1.1E+00	3.5E+00	1000	100	5.70E+03	96%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T04-F	1	1.04E+03			1.04E+03	4.2E-01	1.1E+00	3.5E+00					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T05-F	1	1.13E+03			1.13E+03	5.1E-01	1.1E+00	3.5E+00					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T06-F	1	1.65E+03			1.65E+03	2.6E-01	1.1E+00	3.5E+00					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T07-F	1	2.22E+03			2.22E+03	4.0E-01	1.1E+00	3.5E+00					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T08-F	1	1.65E+04			1.65E+04	1.2E-01	1.1E+00	3.5E+00					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1313-T09-F	1	1.28E+04			1.28E+04	1.8E+00	1.1E+00	3.5E+00					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	SWA-LRef-1313-T01-D	1	4.61E+05			4.61E+05	3.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T02-D	1	4.52E+05			4.52E+05	3.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T03-D	1	4.40E+05			4.40E+05	1.7E-01	2.5E+00	8.0E+00	1000	100	4.41E+05	91%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T04-D	1	5.46E+05			5.46E+05	7.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T05-D	1	5.67E+05			5.67E+05	6.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T06-D	1	5.63E+05			5.63E+05	7.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T07-D	1	4.80E+05			4.80E+05	1.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T08-D	1	2.77E+05			2.77E+05	1.0E+00	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T09-D	1	1.87E+05			1.87E+05	1.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T01-E	1	4.43E+05			4.43E+05	5.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T02-E	1	4.29E+05			4.29E+05	1.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T03-E	1	4.49E+05			4.49E+05	6.3E-01	2.5E+00	8.0E+00	1000	100	4.50E+05	87%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T04-E	1	5.31E+05			5.31E+05	2.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T05-E	1	5.54E+05			5.54E+05	6.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T06-E	1	5.53E+05			5.53E+05	5.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T07-E	1	5.32E+05			5.32E+05	9.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T08-E	1	2.88E+05			2.88E+05	6.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T09-E	1	1.86E+05			1.86E+05	8.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T01-F	1	4.38E+05			4.38E+05	1.0E+00	2.5E+00	8.0E+00				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T02-F	1	4.19E+05			4.19E+05	4.4E-02	2.5E+00	8.0E+00				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T03-F	1	4.30E+05			4.30E+05	1.6E-01	2.5E+00	8.0E+00	1000	100	4.31E+05	86%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T04-F	1	5.31E+05			5.31E+05	6.7E-01	2.5E+00	8.0E+00					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T05-F	1	5.42E+05			5.42E+05	8.0E-01	2.5E+00	8.0E+00					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T06-F	1	5.39E+05			5.39E+05	5.8E-01	2.5E+00	8.0E+00					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T07-F	1	5.43E+05			5.43E+05	1.4E-01	2.5E+00	8.0E+00					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T08-F	1	2.98E+05			2.98E+05	1.1E+00	2.5E+00	8.0E+00					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1313-T09-F	1	1.86E+05			1.86E+05	2.4E-01	2.5E+00	8.0E+00					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	SWA-LRef-1313-T01-D	1	3.46E+02			3.46E+02	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T02-D	1	3.64E+02			3.64E+02	3.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T03-D	1	5.48E+02			5.48E+02	1.4E+00	1.0E+00	3.2E+00	1000	100	1.59E+03	105%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T04-D	1	2.85E+04			2.85E+04	1.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T05-D	1	4.11E+04			4.11E+04	1.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T06-D	1	4.03E+04			4.03E+04	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T07-D	1	4.55E+04			4.55E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T08-D	1	3.19E+04			3.19E+04	9.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T09-D	1	2.29E+04			2.29E+04	2.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T01-E	1	3.30E+02			3.30E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T02-E	1	3.27E+02			3.27E+02	3.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T03-E	1	5.20E+02			5.20E+02	4.9E-01	1.0E+00	3.2E+00	1000	100	1.49E+03	97%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T04-E	1	2.58E+04			2.58E+04	4.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T05-E	1	3.70E+04			3.70E+04	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T06-E	1	4.08E+04			4.08E+04	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T07-E	1	5.11E+04			5.11E+04	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T08-E	1	3.32E+04			3.32E+04	7.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T09-E	1	2.28E+04			2.28E+04	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T01-F	1	1.58E+02			1.58E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T02-F	1	3.43E+02			3.43E+02	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T03-F	1	5.40E+02			5.40E+02	1.0E+00	1.0E+00	3.2E+00	1000	100	1.46E+03	92%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T04-F	1	2.92E+04			2.92E+04	5.1E-01	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T05-F	1	3.73E+04			3.73E+04	9.5E-01	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T06-F	1	4.13E+04			4.13E+04	4.6E-01	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T07-F	1	5.26E+04			5.26E+04	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T08-F	1	3.50E+04			3.50E+04	8.5E-01	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1313-T09-F	1	2.54E+04			2.54E+04	9.1E-01	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	SWA-LRef-1313-T01-D	1	3.91E+05			3.91E+05	4.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T02-D	1	6.22E+05			6.22E+05	2.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T03-D	1	5.16E+05			5.16E+05	2.0E-01	6.8E+00	2.2E+01	1000	100	5.17E+05	96%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T04-D	1	7.92E+05			7.92E+05	9.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T05-D	1	8.76E+05			8.76E+05	3.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T06-D	1	7.85E+05			7.85E+05	6.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T07-D	1	4.11E+05			4.11E+05	2.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T08-D	1	2.44E+05			2.44E+05	7.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T09-D	1	1.85E+05			1.85E+05	3.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T01-E	1	4.59E+05			4.59E+05	6.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T02-E	1	4.18E+05			4.18E+05	1.3E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T03-E	1	3.95E+05			3.95E+05	5.4E-01	6.8E+00	2.2E+01	1000	100	3.96E+05	90%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T04-E	1	7.14E+05			7.14E+05	6.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T05-E	1	7.23E+05			7.23E+05	7.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T06-E	1	6.59E+05			6.59E+05	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T07-E	1	4.38E+05			4.38E+05	3.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T08-E	1	2.55E+05			2.55E+05	2.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T09-E	1	1.86E+05			1.86E+05	5.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T01-F	1	4.05E+05			4.05E+05	5.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T02-F	1	3.50E+05			3.50E+05	2.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T03-F	1	3.34E+05			3.34E+05	1.5E-01	6.8E+00	2.2E+01	1000	100	3.35E+05	87%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T04-F	1	7.03E+05			7.03E+05	4.3E-01	6.8E+00	2.2E+01					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T05-F	1	7.10E+05			7.10E+05	4.1E-01	6.8E+00	2.2E+01					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T06-F	1	6.72E+05			6.72E+05	1.9E-01	6.8E+00	2.2E+01					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T07-F	1	4.73E+05			4.73E+05	3.6E-01	6.8E+00	2.2E+01					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T08-F	1	2.73E+05			2.73E+05	3.4E-01	6.8E+00	2.2E+01					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1313-T09-F	1	1.78E+05			1.78E+05	1.4E+00	6.8E+00	2.2E+01					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	SWA-LRef-1313-T01-D	1	2.30E+00	U1/2		2.30E+00	4.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T02-D	1	2.30E+00	U1/2		2.30E+00	3.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T03-D	1	2.30E+00	U1/2		2.30E+00	8.8E+01	4.6E+00	1.5E+01	10	100	9.59E+02	96%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T04-D	1	2.30E+00	U1/2		2.30E+00	3.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T05-D	1	2.30E+00	U1/2		2.30E+00	2.7E+02	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T06-D	1	8.47E+00	E		8.47E+00	4.4E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T07-D	1	2.14E+01			2.14E+01	1.1E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T08-D	1	1.37E+01	E		1.37E+01	5.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T09-D	1	1.44E+01	E		1.44E+01	1.8E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T01-E	1	2.30E+00	U1/2		2.30E+00	1.1E+02	4.6E+00	1.5E+01				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T02-E	1	2.30E+00	U1/2		2.30E+00	8.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T03-E	1	2.30E+00	U1/2		2.30E+00	9.1E+01	4.6E+00	1.5E+01	10	100	9.32E+02	93%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T04-E	1	2.30E+00	U1/2		2.30E+00	2.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T05-E	1	2.30E+00	U1/2		2.30E+00	3.2E+02	4.6E+00	1.5E+01				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T06-E	1	7.34E+00	E		7.34E+00	4.5E+02	4.6E+00	1.5E+01				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T07-E	1	2.68E+01			2.68E+01	5.8E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T08-E	1	1.10E+01	E		1.10E+01	4.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T09-E	1	1.30E+01	E		1.30E+01	7.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T01-F	1	2.30E+00	U1/2		2.30E+00	8.1E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T02-F	1	2.30E+00	U1/2		2.30E+00	4.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T03-F	1	2.30E+00	U1/2		2.30E+00	2.1E+02	4.6E+00	1.5E+01	10	100	8.86E+02	88%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T04-F	1	2.30E+00	U1/2		2.30E+00	5.0E+02	4.6E+00	1.5E+01					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T05-F	1	2.30E+00	U1/2		2.30E+00	2.1E+02	4.6E+00	1.5E+01					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T06-F	1	1.06E+01	E		1.06E+01	7.9E+01	4.6E+00	1.5E+01					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T07-F	1	2.62E+01			2.62E+01	1.4E+01	4.6E+00	1.5E+01					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T08-F	1	1.04E+01	E		1.04E+01	4.9E+01	4.6E+00	1.5E+01					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1313-T09-F	1	1.24E+01	E		1.24E+01	8.1E+00	4.6E+00	1.5E+01					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	SWA-LRef-1313-T01-D	1	1.00E+00	U1/2		1.00E+00	9.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T02-D	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T03-D	1	1.00E+00	U1/2		1.00E+00	2.0E+02	2.0E+00	6.4E+00	10	100	1.03E+03	103%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T04-D	1	1.00E+00	U1/2		1.00E+00	2.8E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T05-D	1	1.00E+00	U1/2		1.00E+00	1.6E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T06-D	1	1.00E+00	U1/2		1.00E+00	9.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T07-D	1	1.00E+00	U1/2		1.00E+00	1.5E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T08-D	1	3.93E+01			3.93E+01	2.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T09-D	1	6.84E+03			6.84E+03	5.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T01-E	1	1.00E+00	U1/2		1.00E+00	2.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T02-E	1	1.00E+00	U1/2		1.00E+00	2.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T03-E	1	1.00E+00	U1/2		1.00E+00	2.4E+03	2.0E+00	6.4E+00	10	100	9.20E+02	92%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T04-E	1	1.00E+00	U1/2		1.00E+00	3.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T05-E	1	1.00E+00	U1/2		1.00E+00	2.0E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T06-E	1	1.00E+00	U1/2		1.00E+00	1.5E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T07-E	1	1.00E+00	U1/2		1.00E+00	9.7E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T08-E	1	4.51E+01			4.51E+01	3.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T09-E	1	6.72E+03			6.72E+03	3.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T01-F	1	1.00E+00	U1/2		1.00E+00	2.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T02-F	1	1.00E+00	U1/2		1.00E+00	5.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T03-F	1	1.00E+00	U1/2		1.00E+00	4.3E+01	2.0E+00	6.4E+00	10	100	8.80E+02	88%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T04-F	1	1.00E+00	U1/2		1.00E+00	6.1E-01	2.0E+00	6.4E+00					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T05-F	1	1.00E+00	U1/2		1.00E+00	2.4E+01	2.0E+00	6.4E+00					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T06-F	1	1.00E+00	U1/2		1.00E+00	7.1E+01	2.0E+00	6.4E+00					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T07-F	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T08-F	1	4.54E+01			4.54E+01	4.2E+00	2.0E+00	6.4E+00					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1313-T09-F	1	7.24E+03			7.24E+03	3.0E+00	2.0E+00	6.4E+00					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	SWA-LRef-1313-T01-D	1	3.81E+02			3.81E+02	6.8E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T02-D	1	3.68E+02			3.68E+02	4.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T03-D	1	2.40E+02			2.40E+02	6.1E-01	1.5E+00	4.8E+00	10	100	1.30E+03	106%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T04-D	1	2.29E+02			2.29E+02	4.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T05-D	1	2.25E+02			2.25E+02	1.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T06-D	1	2.14E+02			2.14E+02	1.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T07-D	1	1.73E+02			1.73E+02	1.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T08-D	1	1.24E+02			1.24E+02	1.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T09-D	1	1.06E+03			1.06E+03	6.0E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T01-E	1	4.36E+02			4.36E+02	5.4E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T02-E	1	3.49E+02			3.49E+02	1.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T03-E	1	2.87E+02			2.87E+02	7.1E-01	1.5E+00	4.8E+00	10	100	1.28E+03	99%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T04-E	1	1.85E+02			1.85E+02	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T05-E	1	2.09E+02			2.09E+02	1.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T06-E	1	2.07E+02			2.07E+02	1.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T07-E	1	1.94E+02			1.94E+02	2.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T08-E	1	1.25E+02			1.25E+02	2.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T09-E	1	1.11E+03			1.11E+03	5.8E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T01-F	1	4.08E+02			4.08E+02	1.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T02-F	1	3.20E+02			3.20E+02	1.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T03-F	1	2.44E+02			2.44E+02	2.5E-01	1.5E+00	4.8E+00	10	100	1.19E+03	94%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T04-F	1	2.16E+02			2.16E+02	4.1E-01	1.5E+00	4.8E+00					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T05-F	1	2.19E+02			2.19E+02	7.1E-01	1.5E+00	4.8E+00					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T06-F	1	2.01E+02			2.01E+02	1.5E+00	1.5E+00	4.8E+00					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T07-F	1	1.99E+02			1.99E+02	1.5E+00	1.5E+00	4.8E+00					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T08-F	1	1.28E+02			1.28E+02	3.1E+00	1.5E+00	4.8E+00					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1313-T09-F	1	1.23E+03			1.23E+03	9.8E-01	1.5E+00	4.8E+00					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	SWA-LRef-1313-T01-D	1	5.00E-01	U1/2		5.00E-01	3.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:10 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T02-D	1	5.00E-01	U1/2		5.00E-01	2.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:11 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T03-D	1	5.00E-01	U1/2		5.00E-01	8.4E+00	1.0E+00	3.2E+00	10	100	1.16E+03	116%	VU ICP-OES	11/19/10 2:13 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T04-D	1	5.00E-01	U1/2		5.00E-01	6.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:14 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T05-D	1	1.86E+00	E		1.86E+00	1.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T06-D	1	1.15E+00	E		1.15E+00	3.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:18 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T07-D	1	1.03E+03			1.03E+03	6.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:19 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T08-D	1	1.42E+03			1.42E+03	2.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T09-D	1	2.20E+03			2.20E+03	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/19/10 2:23 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T01-E	1	5.00E-01	U1/2		5.00E-01	3.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:28 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T02-E	1	5.00E-01	U1/2		5.00E-01	1.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:30 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T03-E	1	5.00E-01	U1/2		5.00E-01	1.1E+01	1.0E+00	3.2E+00	10	100	1.10E+03	110%	VU ICP-OES	11/22/10 12:31 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T04-E	1	5.00E-01	U1/2		5.00E-01	2.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:33 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T05-E	1	5.00E-01	U1/2		5.00E-01	4.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:34 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T06-E	1	1.51E+00	E		1.51E+00	1.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:36 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T07-E	1	6.06E+02			6.06E+02	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:38 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T08-E	1	1.29E+03			1.29E+03	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:39 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T09-E	1	2.13E+03			2.13E+03	5.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:41 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T01-F	1	5.00E-01	U1/2		5.00E-01	2.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:48 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T02-F	1	5.00E-01	U1/2		5.00E-01	1.2E+02	1.0E+00	3.2E+00				---	VU ICP-OES	11/22/10 12:49 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T03-F	1	5.00E-01	U1/2		5.00E-01	9.9E+00	1.0E+00	3.2E+00	10	100	1.04E+03	104%	VU ICP-OES	11/22/10 12:51 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T04-F	1	5.00E-01	U1/2		5.00E-01	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:53 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T05-F	1	5.00E-01	U1/2		5.00E-01	1.7E+02	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:54 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T06-F	1	8.15E+00			8.15E+00	1.0E+01	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:56 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T07-F	1	3.39E+02			3.39E+02	9.8E-01	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:58 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T08-F	1	1.29E+03			1.29E+03	5.9E-01	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 12:59 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1313-T09-F	1	2.17E+03			2.17E+03	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	11/22/10 1:01 PM	EPA Interlab LRef 1313-1316 SWA

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	CFS-L01-1313-T01-A	1	8.88E+01			8.88E+01	3.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T02-A	1	9.30E+01			9.30E+01	4.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T03-A	1	9.81E+01			9.81E+01	9.5E-01	1.0E+00	3.2E+00	1000	100	1.23E+03	113%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T04-A	1	6.09E+01			6.09E+01	4.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T05-A	1	3.71E+01			3.71E+01	4.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T06-A	1	3.40E+01			3.40E+01	2.0E+01	1.0E+00	3.2E+00			---		VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T07-A	1	4.25E+03			4.25E+03	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T08-A	1	4.44E+04			4.44E+04	6.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T09-A	1	8.31E+04			8.31E+04	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T01-B	1	8.12E+01			8.12E+01	3.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T02-B	1	9.18E+01			9.18E+01	4.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T03-B	1	9.78E+01			9.78E+01	2.6E+00	1.0E+00	3.2E+00	1000	100	1.23E+03	113%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T04-B	1	5.95E+01			5.95E+01	1.5E+02	1.0E+00	3.2E+00			---		VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T05-B	1	4.10E+01			4.10E+01	1.4E+01	1.0E+00	3.2E+00			---		VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T06-B	1	5.19E+01			5.19E+01	5.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T07-B	1	3.82E+03			3.82E+03	9.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T08-B	1	3.93E+04			3.93E+04	9.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T09-B	1	8.14E+04			8.14E+04	6.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T01-C	1	8.38E+01			8.38E+01	2.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T02-C	1	8.85E+01			8.85E+01	3.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T03-C	1	8.69E+01			8.69E+01	3.5E+00	1.0E+00	3.2E+00	1000	100	1.25E+03	116%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T04-C	1	6.36E+01			6.36E+01	6.0E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T05-C	1	3.78E+01			3.78E+01	1.4E+01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T06-C	1	3.13E+01			3.13E+01	2.8E+01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T07-C	1	4.35E+03			4.35E+03	8.5E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T08-C	1	4.23E+04			4.23E+04	4.4E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-T09-C	1	8.52E+04			8.52E+04	3.8E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	7.2E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.4E+01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	CFS-L01-1313-T01-A	1	1.08E+01	E		1.08E+01	4.9E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T02-A	1	9.09E+00	E		9.09E+00	5.9E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T03-A	1	2.32E+01	E		2.32E+01	1.8E+01	7.5E+00	2.4E+01	10	100	1.20E+03	117%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T04-A	1	2.12E+01	E		2.12E+01	6.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T05-A	1	2.70E+01			2.70E+01	1.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T06-A	1	2.54E+01			2.54E+01	5.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T07-A	1	1.05E+02			1.05E+02	3.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T08-A	1	1.46E+03			1.46E+03	1.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T09-A	1	1.79E+03			1.79E+03	2.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T01-B	1	1.35E+01	E		1.35E+01	1.0E+02	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T02-B	1	9.97E+00	E		9.97E+00	1.6E+02	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T03-B	1	2.19E+01	E		2.19E+01	3.2E+01	7.5E+00	2.4E+01	10	100	1.13E+03	111%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T04-B	1	2.62E+01			2.62E+01	1.2E+02	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T05-B	1	2.41E+01			2.41E+01	3.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T06-B	1	2.75E+01			2.75E+01	2.9E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T07-B	1	1.12E+02			1.12E+02	7.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T08-B	1	1.18E+03			1.18E+03	3.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T09-B	1	1.79E+03			1.79E+03	1.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T01-C	1	1.21E+01	E		1.21E+01	6.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T02-C	1	9.37E+00	E		9.37E+00	6.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T03-C	1	2.35E+01	E		2.35E+01	3.0E+01	7.5E+00	2.4E+01	10	100	1.15E+03	113%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T04-C	1	2.88E+01			2.88E+01	1.1E+01	7.5E+00	2.4E+01					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T05-C	1	2.27E+01	E		2.27E+01	5.1E+00	7.5E+00	2.4E+01					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T06-C	1	3.58E+01			3.58E+01	1.4E+00	7.5E+00	2.4E+01					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T07-C	1	1.21E+02			1.21E+02	2.8E+00	7.5E+00	2.4E+01					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T08-C	1	1.41E+03			1.41E+03	1.0E+00	7.5E+00	2.4E+01					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-T09-C	1	1.75E+03			1.75E+03	2.1E+00	7.5E+00	2.4E+01					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-B01-A	1	3.75E+00	U1/2		3.75E+00	2.0E+02	7.5E+00	2.4E+01					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-B02-A	1	7.99E+00	E		7.99E+00	5.6E+01	7.5E+00	2.4E+01					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1313-B03-A	1	1.36E+01	E		1.36E+01	5.6E+01	7.5E+00	2.4E+01					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	CFS-L01-1313-T01-A	1	2.26E+02			2.26E+02	6.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T02-A	1	1.88E+02			1.88E+02	5.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T03-A	1	1.00E+02			1.00E+02	6.7E+00	1.1E+01	3.5E+01	10	100	1.15E+03	105%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T04-A	1	4.20E+01			4.20E+01	1.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T05-A	1	2.96E+01	E		2.96E+01	1.9E+01	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T06-A	1	2.41E+01	E		2.41E+01	2.5E+01	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T07-A	1	1.32E+02			1.32E+02	6.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T08-A	1	2.22E+03			2.22E+03	9.0E-01	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T09-A	1	8.51E+04			8.51E+04	1.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T01-B	1	2.04E+02			2.04E+02	1.7E+00	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T02-B	1	1.81E+02			1.81E+02	4.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T03-B	1	9.32E+01			9.32E+01	1.0E+01	1.1E+01	3.5E+01	10	100	1.16E+03	107%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T04-B	1	4.43E+01			4.43E+01	6.5E+01	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T05-B	1	3.03E+01	E		3.03E+01	4.8E+01	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T06-B	1	2.55E+01	E		2.55E+01	2.9E+01	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T07-B	1	1.27E+02			1.27E+02	7.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T08-B	1	1.64E+03			1.64E+03	7.5E-01	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T09-B	1	7.64E+04			7.64E+04	1.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T01-C	1	2.20E+02			2.20E+02	8.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T02-C	1	2.04E+02			2.04E+02	4.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T03-C	1	1.04E+02			1.04E+02	5.3E+00	1.1E+01	3.5E+01	10	100	1.17E+03	106%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T04-C	1	5.34E+01			5.34E+01	5.6E+00	1.1E+01	3.5E+01					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T05-C	1	2.61E+01	E		2.61E+01	1.6E+01	1.1E+01	3.5E+01					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T06-C	1	2.30E+01	E		2.30E+01	4.5E+01	1.1E+01	3.5E+01					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T07-C	1	1.41E+02			1.41E+02	3.5E+00	1.1E+01	3.5E+01					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T08-C	1	2.23E+03			2.23E+03	5.0E-01	1.1E+01	3.5E+01					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-T09-C	1	7.62E+04			7.62E+04	1.1E+00	1.1E+01	3.5E+01					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-B01-A	1	5.50E+00	U1/2		5.50E+00	5.2E+01	1.1E+01	3.5E+01					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-B02-A	1	1.50E+01	E		1.50E+01	1.2E+01	1.1E+01	3.5E+01					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1313-B03-A	1	1.60E+01	E		1.60E+01	6.7E+01	1.1E+01	3.5E+01					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	CFS-L01-1313-T01-A	1	5.65E+01			5.65E+01	3.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T02-A	1	7.47E+01			7.47E+01	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T03-A	1	1.50E+02			1.50E+02	2.2E+00	1.0E+00	3.2E+00	1000	100	1.23E+03	108%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T04-A	1	1.24E+02			1.24E+02	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T05-A	1	1.27E+02			1.27E+02	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T06-A	1	1.44E+02			1.44E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T07-A	1	3.21E+02			3.21E+02	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T08-A	1	6.56E+02			6.56E+02	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T09-A	1	7.24E+02			7.24E+02	7.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T01-B	1	5.76E+01			5.76E+01	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T02-B	1	7.39E+01			7.39E+01	6.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T03-B	1	1.47E+02			1.47E+02	8.3E-01	1.0E+00	3.2E+00	1000	100	1.15E+03	101%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T04-B	1	1.22E+02			1.22E+02	8.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T05-B	1	1.30E+02			1.30E+02	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T06-B	1	1.44E+02			1.44E+02	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T07-B	1	3.11E+02			3.11E+02	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T08-B	1	6.67E+02			6.67E+02	6.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T09-B	1	7.77E+02			7.77E+02	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T01-C	1	6.17E+01			6.17E+01	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T02-C	1	7.28E+01			7.28E+01	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T03-C	1	1.48E+02			1.48E+02	4.0E-01	1.0E+00	3.2E+00	1000	100	1.19E+03	104%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T04-C	1	1.22E+02			1.22E+02	7.9E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T05-C	1	1.29E+02			1.29E+02	6.0E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T06-C	1	1.45E+02			1.45E+02	2.4E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T07-C	1	3.18E+02			3.18E+02	4.0E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T08-C	1	6.79E+02			6.79E+02	1.0E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-T09-C	1	7.49E+02			7.49E+02	4.7E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-B01-A	1	6.82E+00			6.82E+00	2.8E+01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-B02-A	1	5.68E+00			5.68E+00	6.6E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1313-B03-A	1	4.52E+00			4.52E+00	4.5E+01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	CFS-L01-1313-T01-A	1	1.32E+00	E		1.32E+00	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T02-A	1	6.93E+00			6.93E+00	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T03-A	1	1.45E+02			1.45E+02	5.9E-01	1.0E+00	3.2E+00	10	100	1.05E+03	90%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T04-A	1	7.79E+01			7.79E+01	7.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T05-A	1	6.33E+01			6.33E+01	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T06-A	1	8.52E+01			8.52E+01	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T07-A	1	1.98E+01			1.98E+01	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T08-A	1	3.96E+01			3.96E+01	3.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T09-A	1	6.60E+00			6.60E+00	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T01-B	1	1.69E+00	E		1.69E+00	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T02-B	1	8.31E+00			8.31E+00	9.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T03-B	1	1.40E+02			1.40E+02	2.3E-01	1.0E+00	3.2E+00	10	100	9.64E+02	82%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T04-B	1	8.06E+01			8.06E+01	8.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T05-B	1	5.79E+01			5.79E+01	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T06-B	1	8.79E+01			8.79E+01	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T07-B	1	2.12E+01			2.12E+01	3.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T08-B	1	4.12E+01			4.12E+01	6.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T09-B	1	5.18E+00			5.18E+00	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T01-C	1	1.35E+00	E		1.35E+00	3.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T02-C	1	7.00E+00			7.00E+00	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T03-C	1	1.39E+02			1.39E+02	5.6E-01	1.0E+00	3.2E+00	10	100	9.78E+02	84%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T04-C	1	8.84E+01			8.84E+01	6.7E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T05-C	1	6.23E+01			6.23E+01	7.6E-02	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T06-C	1	8.75E+01			8.75E+01	6.9E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T07-C	1	2.10E+01			2.10E+01	3.0E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T08-C	1	3.91E+01			3.91E+01	1.0E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-T09-C	1	5.86E+00			5.86E+00	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	2.3E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	7.9E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	6.1E+01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	CFS-L01-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	9.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	4.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	6.2E+02	1.9E+00	6.0E+00	10	100	1.12E+03	111%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	9.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	2.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	2.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T07-A	1	2.53E+00	E		2.53E+00	1.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T08-A	1	7.37E+00			7.37E+00	4.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T09-A	1	9.50E-01	U1/2		9.50E-01	8.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	6.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	1.7E+02	1.9E+00	6.0E+00	10	100	1.14E+03	114%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	4.2E+03	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	1.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	6.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T07-B	1	2.56E+00	E		2.56E+00	4.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T08-B	1	6.32E+00			6.32E+00	6.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T09-B	1	9.50E-01	U1/2		9.50E-01	7.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	3.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	1.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	1.6E+02	1.9E+00	6.0E+00	10	100	1.15E+03	115%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	8.2E+02	1.9E+00	6.0E+00					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	1.9E+02	1.9E+00	6.0E+00					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	8.3E+01	1.9E+00	6.0E+00					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T07-C	1	2.65E+00	E		2.65E+00	4.0E+00	1.9E+00	6.0E+00					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T08-C	1	7.14E+00			7.14E+00	7.3E+00	1.9E+00	6.0E+00					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-T09-C	1	9.50E-01	U1/2		9.50E-01	1.9E+02	1.9E+00	6.0E+00					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	9.8E+01	1.9E+00	6.0E+00					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	9.9E+01	1.9E+00	6.0E+00					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	CFS-L01-1313-T01-A	1	8.52E+00			8.52E+00	9.2E+00	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T02-A	1	2.22E+00	E		2.22E+00	1.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	5.1E+01	2.2E+00	7.0E+00	10	100	1.18E+03	118%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T04-A	1	5.72E+00	E		5.72E+00	5.4E+00	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T05-A	1	2.49E+02			2.49E+02	3.7E-01	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T06-A	1	4.33E+03			4.33E+03	9.2E-01	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T07-A	1	2.39E+04			2.39E+04	1.4E-01	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T08-A	1	4.81E+04			4.81E+04	7.6E-01	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T09-A	1	4.70E+04			4.70E+04	7.0E-01	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T01-B	1	1.01E+01			1.01E+01	3.1E+00	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T02-B	1	2.46E+00	E		2.46E+00	1.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	3.0E+01	2.2E+00	7.0E+00	10	100	1.10E+03	110%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T04-B	1	3.59E+00	E		3.59E+00	9.5E+01	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T05-B	1	2.88E+02			2.88E+02	4.1E-01	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T06-B	1	4.33E+03			4.33E+03	7.3E-01	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T07-B	1	2.36E+04			2.36E+04	1.4E+00	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T08-B	1	4.65E+04			4.65E+04	2.7E-01	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T09-B	1	4.88E+04			4.88E+04	1.0E+00	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T01-C	1	1.01E+01			1.01E+01	1.3E+00	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T02-C	1	1.10E+00	U1/2		1.10E+00	1.3E+01	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	3.6E+01	2.2E+00	7.0E+00	10	100	1.12E+03	112%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T04-C	1	4.66E+00	E		4.66E+00	6.3E+00	2.2E+00	7.0E+00					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T05-C	1	2.63E+02			2.63E+02	2.2E-01	2.2E+00	7.0E+00					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T06-C	1	4.52E+03			4.52E+03	1.1E+00	2.2E+00	7.0E+00					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T07-C	1	2.42E+04			2.42E+04	8.7E-01	2.2E+00	7.0E+00					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T08-C	1	5.76E+04			5.76E+04	1.2E+00	2.2E+00	7.0E+00					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-T09-C	1	4.93E+04			4.93E+04	5.2E-01	2.2E+00	7.0E+00					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	3.9E+02	2.2E+00	7.0E+00					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	1.5E+02	2.2E+00	7.0E+00					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1313-B03-A	1	1.10E+00	U1/2		1.10E+00	1.4E+02	2.2E+00	7.0E+00					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	CFS-L01-1313-T01-A	1	5.37E+05			5.37E+05	4.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T02-A	1	5.48E+05			5.48E+05	5.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T03-A	1	5.60E+05			5.60E+05	5.9E-01	2.6E+00	8.3E+00	1000	100	5.61E+05	90%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T04-A	1	5.63E+05			5.63E+05	1.7E+00	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T05-A	1	6.11E+05			6.11E+05	8.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T06-A	1	6.55E+05			6.55E+05	7.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T07-A	1	8.56E+05			8.56E+05	9.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T08-A	1	1.35E+06			1.35E+06	6.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T09-A	1	1.49E+06			1.49E+06	3.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T01-B	1	5.66E+05			5.66E+05	6.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T02-B	1	5.50E+05			5.50E+05	9.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T03-B	1	5.63E+05			5.63E+05	7.3E-01	2.6E+00	8.3E+00	1000	100	5.64E+05	89%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T04-B	1	5.55E+05			5.55E+05	8.7E+01	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T05-B	1	5.82E+05			5.82E+05	6.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T06-B	1	6.62E+05			6.62E+05	6.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T07-B	1	8.59E+05			8.59E+05	9.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T08-B	1	1.30E+06			1.30E+06	2.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T09-B	1	1.48E+06			1.48E+06	1.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T01-C	1	5.75E+05			5.75E+05	3.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T02-C	1	5.42E+05			5.42E+05	4.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T03-C	1	5.68E+05			5.68E+05	5.2E-01	2.6E+00	8.3E+00	1000	100	5.68E+05	89%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T04-C	1	5.93E+05			5.93E+05	6.3E-01	2.6E+00	8.3E+00					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T05-C	1	5.99E+05			5.99E+05	3.1E-01	2.6E+00	8.3E+00					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T06-C	1	6.64E+05			6.64E+05	1.6E+00	2.6E+00	8.3E+00					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T07-C	1	8.68E+05			8.68E+05	8.8E-01	2.6E+00	8.3E+00					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T08-C	1	1.30E+06			1.30E+06	1.3E+00	2.6E+00	8.3E+00					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-T09-C	1	1.48E+06			1.48E+06	8.9E-01	2.6E+00	8.3E+00					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-B01-A	1	7.44E+01			7.44E+01	2.3E+00	2.6E+00	8.3E+00					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-B02-A	1	7.45E+01			7.45E+01	1.4E+01	2.6E+00	8.3E+00					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1313-B03-A	1	6.85E+01			6.85E+01	2.3E+00	2.6E+00	8.3E+00					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	CFS-L01-1313-T01-A	1	1.11E+02			1.11E+02	1.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T02-A	1	5.43E+01			5.43E+01	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T03-A	1	7.43E+00			7.43E+00	1.2E+01	1.2E+00	3.8E+00	10	100	1.18E+03	117%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T04-A	1	1.63E+00	E		1.63E+00	5.8E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T05-A	1	6.00E-01	U1/2		6.00E-01	1.0E+02	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T06-A	1	6.00E-01	U1/2		6.00E-01	3.9E+03	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T07-A	1	6.00E-01	U1/2		6.00E-01	6.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T08-A	1	1.19E+02			1.19E+02	7.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T09-A	1	2.10E+03			2.10E+03	6.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T01-B	1	1.25E+02			1.25E+02	8.5E-02	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T02-B	1	6.04E+01			6.04E+01	1.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T03-B	1	5.86E+00			5.86E+00	9.0E+00	1.2E+00	3.8E+00	10	100	1.11E+03	111%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T04-B	1	1.45E+00	E		1.45E+00	1.1E+02	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T05-B	1	6.00E-01	U1/2		6.00E-01	2.0E+02	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T06-B	1	6.00E-01	U1/2		6.00E-01	2.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T07-B	1	6.00E-01	U1/2		6.00E-01	1.3E+02	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T08-B	1	9.40E+01			9.40E+01	9.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T09-B	1	2.08E+03			2.08E+03	6.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T01-C	1	1.06E+02			1.06E+02	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T02-C	1	5.54E+01			5.54E+01	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T03-C	1	7.33E+00			7.33E+00	5.2E+00	1.2E+00	3.8E+00	10	100	1.13E+03	112%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T04-C	1	2.34E+00	E		2.34E+00	7.6E+00	1.2E+00	3.8E+00					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T05-C	1	6.00E-01	U1/2		6.00E-01	6.1E+01	1.2E+00	3.8E+00					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T06-C	1	6.00E-01	U1/2		6.00E-01	1.4E+02	1.2E+00	3.8E+00					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T07-C	1	6.00E-01	U1/2		6.00E-01	7.0E+01	1.2E+00	3.8E+00					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T08-C	1	1.23E+02			1.23E+02	1.4E+00	1.2E+00	3.8E+00					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-T09-C	1	2.06E+03			2.06E+03	4.7E-01	1.2E+00	3.8E+00					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	3.1E+02	1.2E+00	3.8E+00					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-B02-A	1	2.11E+00	E		2.11E+00	1.8E+01	1.2E+00	3.8E+00					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1313-B03-A	1	1.73E+00	E		1.73E+00	5.1E+01	1.2E+00	3.8E+00					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	CFS-L01-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	1.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	6.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	9.4E+01	1.8E+00	5.7E+00	10	100	1.10E+03	110%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	4.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T05-A	1	3.98E+00	E		3.98E+00	2.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T06-A	1	8.66E+01			8.66E+01	1.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T07-A	1	5.71E+02			5.71E+02	1.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T08-A	1	1.54E+03			1.54E+03	5.3E-01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T09-A	1	1.67E+03			1.67E+03	7.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	5.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	8.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	1.7E+02	1.8E+00	5.7E+00	10	100	1.03E+03	103%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	9.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T05-B	1	5.55E+00	E		5.55E+00	5.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T06-B	1	8.90E+01			8.90E+01	1.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T07-B	1	5.61E+02			5.61E+02	5.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T08-B	1	1.57E+03			1.57E+03	7.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T09-B	1	1.69E+03			1.69E+03	1.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	1.6E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	6.1E+02	1.8E+00	5.7E+00	10	100	1.05E+03	104%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	3.8E+02	1.8E+00	5.7E+00					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T05-C	1	3.87E+00	E		3.87E+00	2.5E+01	1.8E+00	5.7E+00					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T06-C	1	9.33E+01			9.33E+01	1.1E+00	1.8E+00	5.7E+00					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T07-C	1	5.81E+02			5.81E+02	6.5E-01	1.8E+00	5.7E+00					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T08-C	1	1.55E+03			1.55E+03	1.1E+00	1.8E+00	5.7E+00					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-T09-C	1	1.71E+03			1.71E+03	1.2E+00	1.8E+00	5.7E+00					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	1.8E+01	1.8E+00	5.7E+00					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	9.4E+01	1.8E+00	5.7E+00					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	2.1E+02	1.8E+00	5.7E+00					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	CFS-L01-1313-T01-A	1	4.68E+03			4.68E+03	1.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T02-A	1	8.54E+02			8.54E+02	1.7E-01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T03-A	1	1.37E+02			1.37E+02	1.5E+00	3.7E+00	1.2E+01	10	100	1.21E+03	107%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T04-A	1	6.43E+01			6.43E+01	6.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T05-A	1	6.52E+01			6.52E+01	1.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T06-A	1	7.81E+02			7.81E+02	7.5E-01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T07-A	1	2.21E+05			2.21E+05	1.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T08-A	1	9.34E+05			9.34E+05	1.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T09-A	1	1.07E+06			1.07E+06	1.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T01-B	1	5.45E+03			5.45E+03	6.9E-01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T02-B	1	8.49E+02			8.49E+02	1.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T03-B	1	1.30E+02			1.30E+02	1.9E+00	3.7E+00	1.2E+01	10	100	1.14E+03	101%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T04-B	1	5.79E+01			5.79E+01	8.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T05-B	1	6.35E+01			6.35E+01	1.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T06-B	1	7.65E+02			7.65E+02	5.0E-01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T07-B	1	2.04E+05			2.04E+05	1.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T08-B	1	9.03E+05			9.03E+05	4.8E-01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T09-B	1	1.02E+06			1.02E+06	9.5E-01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T01-C	1	5.27E+03			5.27E+03	6.2E-01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T02-C	1	8.18E+02			8.18E+02	2.9E-01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T03-C	1	1.29E+02			1.29E+02	1.9E+00	3.7E+00	1.2E+01	10	100	1.24E+03	111%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T04-C	1	6.97E+01			6.97E+01	5.7E+00	3.7E+00	1.2E+01					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T05-C	1	6.00E+01			6.00E+01	1.7E+00	3.7E+00	1.2E+01					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T06-C	1	9.39E+02			9.39E+02	1.3E+00	3.7E+00	1.2E+01					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T07-C	1	2.26E+05			2.26E+05	1.8E-01	3.7E+00	1.2E+01					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T08-C	1	9.22E+05			9.22E+05	9.0E-01	3.7E+00	1.2E+01					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-T09-C	1	1.06E+06			1.06E+06	4.5E-01	3.7E+00	1.2E+01					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	1.3E+02	3.7E+00	1.2E+01					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	2.2E+02	3.7E+00	1.2E+01					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1313-B03-A	1	1.85E+00	U1/2		1.85E+00	6.0E+01	3.7E+00	1.2E+01					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	CFS-L01-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	7.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	7.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	7.2E+03	2.0E+00	6.4E+00	1000	100	1.18E+03	118%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	1.5E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	4.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T07-A	1	4.92E+00	E		4.92E+00	6.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T08-A	1	8.27E+04			8.27E+04	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T09-A	1	2.73E+05			2.73E+05	3.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	4.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	4.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	3.2E+01	2.0E+00	6.4E+00	1000	100	1.10E+03	110%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	5.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	2.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T07-B	1	5.37E+00	E		5.37E+00	4.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T08-B	1	7.00E+04			7.00E+04	4.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T09-B	1	2.56E+05			2.56E+05	6.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	5.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00	1000	100	1.12E+03	112%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	1.7E+02	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	6.3E+02	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	1.8E+03	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T07-C	1	7.39E+00			7.39E+00	6.2E+00	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T08-C	1	7.22E+04			7.22E+04	3.7E-01	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-T09-C	1	2.65E+05			2.65E+05	3.9E+00	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	4.0E+01	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-B02-A	1	1.90E+01			1.90E+01	1.0E+00	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1313-B03-A	1	3.96E+00	E		3.96E+00	1.3E+01	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	CFS-L01-1313-T01-A	1	6.19E+03			6.19E+03	1.3E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T02-A	1	8.12E+03			8.12E+03	6.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T03-A	1	9.83E+02			9.83E+02	6.7E-01	6.8E+00	2.2E+01	10	100	1.92E+03	94%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T04-A	1	1.72E+02			1.72E+02	3.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T05-A	1	1.82E+02			1.82E+02	3.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T06-A	1	1.09E+03			1.09E+03	1.3E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T07-A	1	7.19E+03			7.19E+03	9.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T08-A	1	5.95E+03			5.95E+03	8.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T09-A	1	8.24E+03			8.24E+03	8.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T01-B	1	5.71E+03			5.71E+03	8.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T02-B	1	9.13E+03			9.13E+03	1.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T03-B	1	7.90E+02			7.90E+02	1.5E+00	6.8E+00	2.2E+01	10	100	1.91E+03	112%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T04-B	1	1.72E+02			1.72E+02	1.0E+02	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T05-B	1	1.89E+02			1.89E+02	2.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T06-B	1	1.06E+03			1.06E+03	7.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T07-B	1	7.15E+03			7.15E+03	8.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T08-B	1	5.49E+03			5.49E+03	1.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T09-B	1	8.30E+03			8.30E+03	6.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T01-C	1	6.59E+03			6.59E+03	3.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T02-C	1	8.88E+03			8.88E+03	5.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T03-C	1	6.95E+02			6.95E+02	9.6E-01	6.8E+00	2.2E+01	10	100	1.77E+03	107%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T04-C	1	1.98E+02			1.98E+02	1.3E+00	6.8E+00	2.2E+01					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T05-C	1	1.88E+02			1.88E+02	3.2E+00	6.8E+00	2.2E+01					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T06-C	1	1.09E+03			1.09E+03	7.4E-01	6.8E+00	2.2E+01					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T07-C	1	6.71E+03			6.71E+03	8.2E-01	6.8E+00	2.2E+01					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T08-C	1	5.83E+03			5.83E+03	1.2E+00	6.8E+00	2.2E+01					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-T09-C	1	8.16E+03			8.16E+03	4.8E-01	6.8E+00	2.2E+01					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	1.7E+01	6.8E+00	2.2E+01					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	4.2E+01	6.8E+00	2.2E+01					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	3.4E+01	6.8E+00	2.2E+01					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	CFS-L01-1313-T01-A	1	1.33E+01			1.33E+01	3.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T02-A	1	1.02E+01			1.02E+01	5.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T03-A	1	9.51E+00			9.51E+00	1.5E+01	1.9E+00	6.0E+00	10	100	8.62E+02	85%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T04-A	1	1.14E+01			1.14E+01	1.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T05-A	1	9.31E+00			9.31E+00	4.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T06-A	1	9.51E+00			9.51E+00	1.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T07-A	1	9.29E+00			9.29E+00	2.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T08-A	1	7.69E+00			7.69E+00	1.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T09-A	1	2.32E+01			2.32E+01	5.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T01-B	1	1.38E+01			1.38E+01	5.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T02-B	1	1.16E+01			1.16E+01	3.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T03-B	1	1.14E+01			1.14E+01	1.0E+01	1.9E+00	6.0E+00	10	100	8.95E+02	88%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T04-B	1	9.05E+00			9.05E+00	2.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T05-B	1	1.08E+01			1.08E+01	1.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T06-B	1	9.51E+00			9.51E+00	2.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T07-B	1	1.02E+01			1.02E+01	6.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T08-B	1	9.65E+00			9.65E+00	9.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T09-B	1	1.18E+01			1.18E+01	4.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T01-C	1	1.25E+01			1.25E+01	1.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T02-C	1	1.30E+01			1.30E+01	1.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T03-C	1	9.99E+00			9.99E+00	1.5E+01	1.9E+00	6.0E+00	10	100	8.76E+02	87%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T04-C	1	1.35E+01			1.35E+01	1.8E+01	1.9E+00	6.0E+00					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T05-C	1	1.34E+01			1.34E+01	1.1E+01	1.9E+00	6.0E+00					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T06-C	1	9.33E+00			9.33E+00	6.2E+00	1.9E+00	6.0E+00					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T07-C	1	7.82E+00			7.82E+00	2.8E+01	1.9E+00	6.0E+00					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T08-C	1	1.12E+01			1.12E+01	9.3E+00	1.9E+00	6.0E+00					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-T09-C	1	2.03E+01			2.03E+01	2.3E+01	1.9E+00	6.0E+00					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	1.3E+01	1.9E+00	6.0E+00					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	1.9E+01	1.9E+00	6.0E+00					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	1.2E+01	1.9E+00	6.0E+00					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	CFS-L01-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	4.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	7.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	4.4E+01	2.0E+00	6.4E+00	10	100	1.14E+03	114%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	4.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T05-A	1	1.10E+02			1.10E+02	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T06-A	1	1.42E+03			1.42E+03	8.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T07-A	1	5.93E+03			5.93E+03	9.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T08-A	1	2.39E+04			2.39E+04	9.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T09-A	1	3.42E+04			3.42E+04	4.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	2.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.0E+00	6.4E+00	10	100	1.06E+03	106%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	9.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T05-B	1	1.38E+02			1.38E+02	1.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T06-B	1	1.42E+03			1.42E+03	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T07-B	1	5.88E+03			5.88E+03	9.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T08-B	1	2.39E+04			2.39E+04	3.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T09-B	1	3.16E+04			3.16E+04	6.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	3.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	2.6E+01	2.0E+00	6.4E+00	10	100	1.08E+03	108%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	3.6E+01	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T05-C	1	1.36E+02			1.36E+02	1.0E+00	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T06-C	1	1.51E+03			1.51E+03	1.6E+00	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T07-C	1	6.08E+03			6.08E+03	7.7E-01	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T08-C	1	2.35E+04			2.35E+04	9.5E-01	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-T09-C	1	3.30E+04			3.30E+04	9.2E-01	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	4.6E+01	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	CFS-L01-1313-T01-A	1	1.14E+01			1.14E+01	6.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T02-A	1	2.76E+01			2.76E+01	4.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T03-A	1	7.60E+02			7.60E+02	5.0E-01	1.0E+00	3.2E+00	1000	100	1.67E+03	91%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T04-A	1	1.64E+04			1.64E+04	4.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T05-A	1	6.35E+04			6.35E+04	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T06-A	1	5.83E+04			5.83E+04	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T07-A	1	6.94E+04			6.94E+04	2.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T08-A	1	1.52E+05			1.52E+05	2.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T09-A	1	2.47E+05			2.47E+05	8.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T01-B	1	2.19E+01			2.19E+01	7.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T02-B	1	2.35E+01			2.35E+01	3.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T03-B	1	1.02E+03			1.02E+03	1.2E+00	1.0E+00	3.2E+00	1000	100	1.97E+03	95%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T04-B	1	1.60E+04			1.60E+04	9.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T05-B	1	6.25E+04			6.25E+04	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T06-B	1	6.19E+04			6.19E+04	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T07-B	1	7.30E+04			7.30E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T08-B	1	1.70E+05			1.70E+05	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T09-B	1	2.42E+05			2.42E+05	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T01-C	1	1.65E+01			1.65E+01	4.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T02-C	1	2.53E+01			2.53E+01	2.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T03-C	1	1.21E+03			1.21E+03	9.8E-01	1.0E+00	3.2E+00	1000	100	2.17E+03	97%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T04-C	1	1.53E+04			1.53E+04	1.5E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T05-C	1	6.46E+04			6.46E+04	9.5E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T06-C	1	6.22E+04			6.22E+04	7.0E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T07-C	1	7.25E+04			7.25E+04	5.3E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T08-C	1	1.63E+05			1.63E+05	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-T09-C	1	2.33E+05			2.33E+05	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.3E+02	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	5.0E+01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	9.1E+01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	CFS-L01-1313-T01-A	1	1.28E+03			1.28E+03	5.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T02-A	1	1.57E+03			1.57E+03	3.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T03-A	1	9.82E+02			9.82E+02	1.4E+00	1.2E+00	3.8E+00	10	100	2.04E+03	106%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T04-A	1	5.67E+02			5.67E+02	9.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T05-A	1	6.23E+01			6.23E+01	1.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T06-A	1	8.40E+00			8.40E+00	5.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T07-A	1	6.41E+00			6.41E+00	2.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T08-A	1	2.60E+01			2.60E+01	8.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T09-A	1	1.08E+02			1.08E+02	1.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T01-B	1	1.29E+03			1.29E+03	1.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T02-B	1	1.50E+03			1.50E+03	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T03-B	1	9.74E+02			9.74E+02	1.1E+00	1.2E+00	3.8E+00	10	100	2.00E+03	103%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T04-B	1	6.20E+02			6.20E+02	8.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T05-B	1	5.80E+01			5.80E+01	1.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T06-B	1	8.22E+00			8.22E+00	9.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T07-B	1	4.46E+00			4.46E+00	7.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T08-B	1	8.39E+00			8.39E+00	6.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T09-B	1	1.06E+02			1.06E+02	2.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T01-C	1	1.29E+03			1.29E+03	3.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T02-C	1	1.54E+03			1.54E+03	5.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T03-C	1	9.87E+02			9.87E+02	6.2E-01	1.2E+00	3.8E+00	10	100	2.10E+03	111%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T04-C	1	6.16E+02			6.16E+02	7.3E-01	1.2E+00	3.8E+00					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T05-C	1	5.95E+01			5.95E+01	1.3E-01	1.2E+00	3.8E+00					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T06-C	1	9.37E+00			9.37E+00	5.7E+00	1.2E+00	3.8E+00					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T07-C	1	4.05E+00			4.05E+00	6.0E+01	1.2E+00	3.8E+00					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T08-C	1	3.95E+00			3.95E+00	5.6E+01	1.2E+00	3.8E+00					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-T09-C	1	8.53E+01			8.53E+01	3.5E+00	1.2E+00	3.8E+00					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-B01-A	1	5.18E+00			5.18E+00	1.3E+01	1.2E+00	3.8E+00					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	1.0E+02	1.2E+00	3.8E+00					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1313-B03-A	1	1.65E+01			1.65E+01	1.2E+01	1.2E+00	3.8E+00					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	CFS-L01-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	8.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	7.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00	10	100	1.14E+03	114%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	2.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T05-A	1	6.75E+00			6.75E+00	3.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T06-A	1	2.00E+02			2.00E+02	8.4E-01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T07-A	1	2.16E+03			2.16E+03	1.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T08-A	1	6.14E+03			6.14E+03	1.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T09-A	1	6.35E+03			6.35E+03	1.9E+00	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	9.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	9.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	7.3E+02	1.8E+00	5.7E+00	10	100	1.06E+03	106%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	1.2E+03	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T05-B	1	9.61E+00			9.61E+00	1.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T06-B	1	2.00E+02			2.00E+02	8.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T07-B	1	2.05E+03			2.05E+03	3.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T08-B	1	6.01E+03			6.01E+03	2.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T09-B	1	6.48E+03			6.48E+03	9.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	5.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	7.6E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00	10	100	1.07E+03	107%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	5.6E+01	1.8E+00	5.7E+00					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T05-C	1	9.48E+00			9.48E+00	1.9E+01	1.8E+00	5.7E+00					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T06-C	1	2.07E+02			2.07E+02	1.3E+00	1.8E+00	5.7E+00					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T07-C	1	2.21E+03			2.21E+03	4.6E-01	1.8E+00	5.7E+00					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T08-C	1	6.08E+03			6.08E+03	4.0E-01	1.8E+00	5.7E+00					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-T09-C	1	6.31E+03			6.31E+03	2.2E-01	1.8E+00	5.7E+00					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	3.2E+02	1.8E+00	5.7E+00					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	3.1E+01	1.8E+00	5.7E+00					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	8.4E+01	1.8E+00	5.7E+00					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	CFS-L01-1313-T01-A	1	8.50E+01			8.50E+01	7.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T02-A	1	7.91E+01			7.91E+01	1.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T03-A	1	6.58E+01			6.58E+01	2.7E+01	3.7E+00	1.2E+01	1000	100	1.10E+03	104%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T04-A	1	1.85E+00	U1/2		1.85E+00	1.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T05-A	1	4.44E+00	E		4.44E+00	3.0E+02	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T06-A	1	1.85E+00	U1/2		1.85E+00	1.3E+02	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T07-A	1	2.80E+01			2.80E+01	7.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T08-A	1	6.24E+01			6.24E+01	1.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T09-A	1	3.47E+03			3.47E+03	1.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T01-B	1	9.71E+01			9.71E+01	7.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T02-B	1	7.28E+01			7.28E+01	3.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T03-B	1	5.92E+01			5.92E+01	1.8E+01	3.7E+00	1.2E+01	1000	100	1.11E+03	105%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T04-B	1	3.71E+01			3.71E+01	1.1E+02	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T05-B	1	5.84E+00	E		5.84E+00	1.0E+02	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T06-B	1	1.85E+00	U1/2		1.85E+00	7.3E+02	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T07-B	1	1.85E+00	U1/2		1.85E+00	2.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T08-B	1	2.32E+01			2.32E+01	6.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T09-B	1	3.02E+03			3.02E+03	2.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T01-C	1	8.86E+01			8.86E+01	1.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T02-C	1	8.53E+01			8.53E+01	9.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T03-C	1	5.16E+01			5.16E+01	6.9E+00	3.7E+00	1.2E+01	1000	100	1.13E+03	108%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T04-C	1	3.37E+01			3.37E+01	9.6E+00	3.7E+00	1.2E+01					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T05-C	1	4.77E+00	E		4.77E+00	6.5E+01	3.7E+00	1.2E+01					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T06-C	1	1.85E+00	U1/2		1.85E+00	5.7E+01	3.7E+00	1.2E+01					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T07-C	1	1.85E+00	U1/2		1.85E+00	2.7E+01	3.7E+00	1.2E+01					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T08-C	1	3.48E+01			3.48E+01	1.3E+01	3.7E+00	1.2E+01					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-T09-C	1	3.03E+03			3.03E+03	1.0E+00	3.7E+00	1.2E+01					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-B01-A	1	1.67E+01			1.67E+01	4.5E+01	3.7E+00	1.2E+01					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-B02-A	1	4.63E+01			4.63E+01	3.4E+01	3.7E+00	1.2E+01					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1313-B03-A	1	5.65E+01			5.65E+01	7.8E+00	3.7E+00	1.2E+01					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	CFS-L01-1313-T01-A	1	2.13E+06			2.13E+06	6.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T02-A	1	2.10E+06			2.10E+06	9.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T03-A	1	4.80E+05			4.80E+05	1.1E+00	1.6E+00	5.1E+00	1000	100	4.81E+05	93%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T04-A	1	3.52E+05			3.52E+05	1.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T05-A	1	2.02E+05			2.02E+05	5.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T06-A	1	8.71E+03			8.71E+03	6.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T07-A	1	1.08E+04			1.08E+04	1.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T08-A	1	1.71E+04			1.71E+04	5.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T09-A	1	2.30E+04			2.30E+04	8.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T01-B	1	2.15E+06			2.15E+06	1.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T02-B	1	2.11E+06			2.11E+06	1.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T03-B	1	4.66E+05			4.66E+05	2.5E-01	1.6E+00	5.1E+00	1000	100	4.67E+05	85%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T04-B	1	3.62E+05			3.62E+05	8.8E+01	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T05-B	1	1.82E+05			1.82E+05	6.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T06-B	1	9.26E+03			9.26E+03	5.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T07-B	1	1.09E+04			1.09E+04	9.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T08-B	1	1.69E+04			1.69E+04	8.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T09-B	1	2.16E+04			2.16E+04	5.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T01-C	1	2.09E+06			2.09E+06	1.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T02-C	1	2.07E+06			2.07E+06	7.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T03-C	1	4.69E+05			4.69E+05	2.4E-01	1.6E+00	5.1E+00	1000	100	4.70E+05	91%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T04-C	1	3.71E+05			3.71E+05	7.6E-01	1.6E+00	5.1E+00					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T05-C	1	1.91E+05			1.91E+05	3.5E-01	1.6E+00	5.1E+00					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T06-C	1	8.93E+03			8.93E+03	8.8E-01	1.6E+00	5.1E+00					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T07-C	1	1.09E+04			1.09E+04	8.4E-01	1.6E+00	5.1E+00					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T08-C	1	1.69E+04			1.69E+04	1.0E+00	1.6E+00	5.1E+00					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-T09-C	1	2.32E+04			2.32E+04	7.3E-01	1.6E+00	5.1E+00					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-B01-A	1	1.42E+01			1.42E+01	2.0E+01	1.6E+00	5.1E+00					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-B02-A	1	2.13E+06			2.13E+06	1.6E+00	1.6E+00	5.1E+00					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1313-B03-A	1	2.14E+06			2.14E+06	1.2E+00	1.6E+00	5.1E+00					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	CFS-L01-1313-T01-A	1	2.88E+02			2.88E+02	2.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T02-A	1	4.12E+02			4.12E+02	2.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T03-A	1	5.72E+02			5.72E+02	6.4E-01	1.5E+01	4.8E+01	10	100	1.56E+03	99%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T04-A	1	1.98E+02			1.98E+02	4.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T05-A	1	8.15E+01			8.15E+01	2.0E+01	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T06-A	1	7.45E+01			7.45E+01	5.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T07-A	1	1.27E+02			1.27E+02	2.0E+01	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T08-A	1	2.37E+02			2.37E+02	4.6E+00	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T09-A	1	5.13E+02			5.13E+02	4.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T01-B	1	2.75E+02			2.75E+02	7.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T02-B	1	4.04E+02			4.04E+02	7.1E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T03-B	1	5.17E+02			5.17E+02	1.9E+00	1.5E+01	4.8E+01	10	100	1.48E+03	96%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T04-B	1	2.23E+02			2.23E+02	9.2E+01	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T05-B	1	9.39E+01			9.39E+01	9.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T06-B	1	6.65E+01			6.65E+01	1.6E+01	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T07-B	1	1.18E+02			1.18E+02	1.7E+01	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T08-B	1	2.04E+02			2.04E+02	8.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T09-B	1	4.69E+02			4.69E+02	8.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T01-C	1	2.93E+02			2.93E+02	4.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T02-C	1	3.91E+02			3.91E+02	4.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T03-C	1	5.15E+02			5.15E+02	1.7E+00	1.5E+01	4.8E+01	10	100	1.49E+03	98%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T04-C	1	2.25E+02			2.25E+02	8.5E+00	1.5E+01	4.8E+01					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T05-C	1	7.70E+01			7.70E+01	6.3E+00	1.5E+01	4.8E+01					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T06-C	1	6.96E+01			6.96E+01	1.6E+01	1.5E+01	4.8E+01					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T07-C	1	1.09E+02			1.09E+02	1.7E+01	1.5E+01	4.8E+01					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T08-C	1	2.46E+02			2.46E+02	5.2E+00	1.5E+01	4.8E+01					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-T09-C	1	4.70E+02			4.70E+02	3.0E+00	1.5E+01	4.8E+01					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-B01-A	1	7.50E+00	U1/2		7.50E+00	1.8E+02	1.5E+01	4.8E+01					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-B02-A	1	7.50E+00	U1/2		7.50E+00	7.5E+01	1.5E+01	4.8E+01					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1313-B03-A	1	7.50E+00	U1/2		7.50E+00	1.4E+02	1.5E+01	4.8E+01					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	CFS-L01-1313-T01-A	1	2.14E+02			2.14E+02	2.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T02-A	1	2.07E+02			2.07E+02	2.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T03-A	1	4.70E+02			4.70E+02	2.6E+00	1.1E+00	3.5E+00	1000	100	1.53E+03	106%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T04-A	1	4.56E+02			4.56E+02	6.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T05-A	1	1.19E+03			1.19E+03	1.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T06-A	1	3.75E+03			3.75E+03	1.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T07-A	1	2.61E+04			2.61E+04	9.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T08-A	1	1.00E+05			1.00E+05	4.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T09-A	1	1.56E+05			1.56E+05	9.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T01-B	1	2.14E+02			2.14E+02	1.7E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T02-B	1	2.04E+02			2.04E+02	6.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T03-B	1	5.24E+02			5.24E+02	3.3E-01	1.1E+00	3.5E+00	1000	100	1.40E+03	88%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T04-B	1	4.74E+02			4.74E+02	8.2E+01	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T05-B	1	1.29E+03			1.29E+03	1.4E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T06-B	1	3.71E+03			3.71E+03	5.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T07-B	1	2.50E+04			2.50E+04	4.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T08-B	1	9.43E+04			9.43E+04	4.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T09-B	1	1.51E+05			1.51E+05	6.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T01-C	1	2.43E+02			2.43E+02	1.8E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T02-C	1	2.49E+02			2.49E+02	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T03-C	1	5.31E+02			5.31E+02	1.1E+00	1.1E+00	3.5E+00	1000	100	1.38E+03	85%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T04-C	1	4.65E+02			4.65E+02	5.0E-01	1.1E+00	3.5E+00					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T05-C	1	1.25E+03			1.25E+03	2.3E-01	1.1E+00	3.5E+00					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T06-C	1	3.68E+03			3.68E+03	1.3E+00	1.1E+00	3.5E+00					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T07-C	1	2.68E+04			2.68E+04	6.3E-01	1.1E+00	3.5E+00					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T08-C	1	9.43E+04			9.43E+04	1.3E-01	1.1E+00	3.5E+00					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-T09-C	1	1.62E+05			1.62E+05	5.2E-01	1.1E+00	3.5E+00					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-B01-A	1	5.50E-01	U1/2		5.50E-01	1.0E+02	1.1E+00	3.5E+00					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-B02-A	1	6.99E+02			6.99E+02	3.0E+00	1.1E+00	3.5E+00					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1313-B03-A	1	1.40E+03			1.40E+03	6.0E+00	1.1E+00	3.5E+00					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	CFS-L01-1313-T01-A	1	1.52E+04			1.52E+04	3.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T02-A	1	1.59E+04			1.59E+04	4.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T03-A	1	1.59E+04			1.59E+04	2.4E-01	2.5E+00	8.0E+00	1000	100	1.68E+04	91%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T04-A	1	1.67E+04			1.67E+04	6.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T05-A	1	1.77E+04			1.77E+04	8.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T06-A	1	1.66E+04			1.66E+04	8.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T07-A	1	1.78E+04			1.78E+04	6.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T08-A	1	2.35E+04			2.35E+04	7.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T09-A	1	2.58E+04			2.58E+04	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T01-B	1	1.57E+04			1.57E+04	5.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T02-B	1	1.57E+04			1.57E+04	8.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T03-B	1	1.64E+04			1.64E+04	6.8E-01	2.5E+00	8.0E+00	1000	100	1.74E+04	92%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T04-B	1	1.61E+04			1.61E+04	8.9E+01	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T05-B	1	1.70E+04			1.70E+04	7.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T06-B	1	1.69E+04			1.69E+04	7.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T07-B	1	1.85E+04			1.85E+04	9.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T08-B	1	2.40E+04			2.40E+04	8.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T09-B	1	2.70E+04			2.70E+04	1.7E+00	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T01-C	1	1.57E+04			1.57E+04	2.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T02-C	1	1.56E+04			1.56E+04	8.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T03-C	1	1.68E+04			1.68E+04	5.6E-01	2.5E+00	8.0E+00	1000	100	1.78E+04	97%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T04-C	1	1.70E+04			1.70E+04	6.7E-01	2.5E+00	8.0E+00					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T05-C	1	1.77E+04			1.77E+04	2.1E-01	2.5E+00	8.0E+00					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T06-C	1	1.78E+04			1.78E+04	9.8E-01	2.5E+00	8.0E+00					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T07-C	1	1.88E+04			1.88E+04	1.2E+00	2.5E+00	8.0E+00					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T08-C	1	2.52E+04			2.52E+04	9.9E-01	2.5E+00	8.0E+00					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-T09-C	1	2.82E+04			2.82E+04	1.3E+00	2.5E+00	8.0E+00					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-B01-A	1	1.25E+00	U1/2		1.25E+00	3.1E+01	2.5E+00	8.0E+00					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-B02-A	1	9.89E+02			9.89E+02	2.6E+00	2.5E+00	8.0E+00					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1313-B03-A	1	1.01E+03			1.01E+03	1.0E+00	2.5E+00	8.0E+00					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	CFS-L01-1313-T01-A	1	2.77E+03			2.77E+03	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T02-A	1	3.55E+03			3.55E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T03-A	1	3.79E+03			3.79E+03	1.7E+00	1.0E+00	3.2E+00	1000	100	4.89E+03	110%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T04-A	1	3.65E+03			3.65E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T05-A	1	3.49E+03			3.49E+03	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T06-A	1	1.37E+03			1.37E+03	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T07-A	1	9.29E+02			9.29E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T08-A	1	1.34E+03			1.34E+03	9.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T09-A	1	1.39E+03			1.39E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T01-B	1	2.53E+03			2.53E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T02-B	1	3.42E+03			3.42E+03	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T03-B	1	3.73E+03			3.73E+03	1.3E+00	1.0E+00	3.2E+00	1000	100	4.71E+03	98%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T04-B	1	3.68E+03			3.68E+03	8.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T05-B	1	3.28E+03			3.28E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T06-B	1	1.41E+03			1.41E+03	7.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T07-B	1	9.36E+02			9.36E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T08-B	1	1.35E+03			1.35E+03	1.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T09-B	1	1.32E+03			1.32E+03	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T01-C	1	2.81E+03			2.81E+03	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T02-C	1	3.37E+03			3.37E+03	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T03-C	1	3.82E+03			3.82E+03	7.1E-01	1.0E+00	3.2E+00	1000	100	4.86E+03	104%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T04-C	1	3.64E+03			3.64E+03	9.3E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T05-C	1	3.33E+03			3.33E+03	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T06-C	1	1.38E+03			1.38E+03	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T07-C	1	9.34E+02			9.34E+02	3.2E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T08-C	1	1.33E+03			1.33E+03	1.0E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-T09-C	1	1.40E+03			1.40E+03	3.8E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	3.1E+01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.5E+02	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	1.5E+02	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	CFS-L01-1313-T01-A	1	1.27E+06			1.27E+06	3.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T02-A	1	1.01E+06			1.01E+06	4.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T03-A	1	7.73E+05			7.73E+05	2.3E-01	6.8E+00	2.2E+01	1000	100	7.74E+05	115%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T04-A	1	7.59E+05			7.59E+05	6.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T05-A	1	6.94E+05			6.94E+05	5.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T06-A	1	6.18E+05			6.18E+05	8.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T07-A	1	6.47E+05			6.47E+05	7.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T08-A	1	7.31E+05			7.31E+05	7.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T09-A	1	8.03E+05			8.03E+05	1.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T01-B	1	1.26E+06			1.26E+06	2.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T02-B	1	1.01E+06			1.01E+06	9.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T03-B	1	7.71E+05			7.71E+05	3.7E-01	6.8E+00	2.2E+01	1000	100	7.73E+05	113%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T04-B	1	7.20E+05			7.20E+05	8.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T05-B	1	7.19E+05			7.19E+05	2.6E-02	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T06-B	1	6.18E+05			6.18E+05	5.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T07-B	1	6.39E+05			6.39E+05	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T08-B	1	7.39E+05			7.39E+05	4.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T09-B	1	8.12E+05			8.12E+05	1.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T01-C	1	1.29E+06			1.29E+06	2.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T02-C	1	1.02E+06			1.02E+06	5.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T03-C	1	7.71E+05			7.71E+05	3.2E-01	6.8E+00	2.2E+01	1000	100	7.72E+05	100%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T04-C	1	7.22E+05			7.22E+05	6.2E-01	6.8E+00	2.2E+01					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T05-C	1	7.11E+05			7.11E+05	4.2E-01	6.8E+00	2.2E+01					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T06-C	1	6.17E+05			6.17E+05	1.1E+00	6.8E+00	2.2E+01					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T07-C	1	6.47E+05			6.47E+05	5.3E-01	6.8E+00	2.2E+01					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T08-C	1	7.41E+05			7.41E+05	1.0E+00	6.8E+00	2.2E+01					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-T09-C	1	8.16E+05			8.16E+05	4.0E-01	6.8E+00	2.2E+01					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	3.9E+01	6.8E+00	2.2E+01					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	6.8E+00	6.8E+00	2.2E+01					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	6.1E+02	6.8E+00	2.2E+01					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

TI	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
TI	CFS-L01-1313-T01-A	1	1.91E+02			1.91E+02	5.2E+00	4.6E+00	1.5E+01				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T02-A	1	1.97E+02			1.97E+02	1.3E+00	4.6E+00	1.5E+01				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T03-A	1	2.94E+02			2.94E+02	1.8E+00	4.6E+00	1.5E+01	10	100	1.22E+03	93%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T04-A	1	4.54E+02			4.54E+02	1.8E+00	4.6E+00	1.5E+01				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T05-A	1	6.84E+02			6.84E+02	6.1E-01	4.6E+00	1.5E+01				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T06-A	1	3.18E+02			3.18E+02	6.0E-01	4.6E+00	1.5E+01				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T07-A	1	5.68E+02			5.68E+02	2.1E+00	4.6E+00	1.5E+01				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T08-A	1	9.84E+02			9.84E+02	1.9E+00	4.6E+00	1.5E+01				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T09-A	1	1.60E+03			1.60E+03	9.9E-01	4.6E+00	1.5E+01				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T01-B	1	2.06E+02			2.06E+02	2.2E+00	4.6E+00	1.5E+01				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T02-B	1	1.89E+02			1.89E+02	2.9E+00	4.6E+00	1.5E+01				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T03-B	1	3.07E+02			3.07E+02	1.6E+00	4.6E+00	1.5E+01	10	100	1.15E+03	84%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T04-B	1	4.50E+02			4.50E+02	8.9E+01	4.6E+00	1.5E+01				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T05-B	1	6.59E+02			6.59E+02	7.9E-01	4.6E+00	1.5E+01				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T06-B	1	3.16E+02			3.16E+02	2.1E+00	4.6E+00	1.5E+01				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T07-B	1	5.65E+02			5.65E+02	1.2E+00	4.6E+00	1.5E+01				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T08-B	1	9.74E+02			9.74E+02	3.3E-01	4.6E+00	1.5E+01				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T09-B	1	1.60E+03			1.60E+03	6.3E-01	4.6E+00	1.5E+01				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T01-C	1	1.98E+02			1.98E+02	1.3E+00	4.6E+00	1.5E+01				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T02-C	1	1.86E+02			1.86E+02	3.1E+00	4.6E+00	1.5E+01				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T03-C	1	3.18E+02			3.18E+02	4.4E-01	4.6E+00	1.5E+01	10	100	1.17E+03	85%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T04-C	1	4.60E+02			4.60E+02	1.1E+00	4.6E+00	1.5E+01					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T05-C	1	6.75E+02			6.75E+02	6.5E-01	4.6E+00	1.5E+01					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T06-C	1	3.18E+02			3.18E+02	1.7E+00	4.6E+00	1.5E+01					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T07-C	1	5.75E+02			5.75E+02	2.3E+00	4.6E+00	1.5E+01					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T08-C	1	9.99E+02			9.99E+02	1.6E+00	4.6E+00	1.5E+01					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-T09-C	1	1.63E+03			1.63E+03	4.1E-01	4.6E+00	1.5E+01					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	3.2E+01	4.6E+00	1.5E+01					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	2.1E+01	4.6E+00	1.5E+01					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
TI	CFS-L01-1313-B03-A	1	5.67E+00	E		5.67E+00	5.8E+01	4.6E+00	1.5E+01					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	CFS-L01-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	9.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	7.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	6.4E+02	2.0E+00	6.4E+00	10	100	1.12E+03	112%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	4.9E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	9.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T07-A	1	2.82E+00	E		2.82E+00	5.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T08-A	1	2.15E+01			2.15E+01	7.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T09-A	1	4.19E+01			4.19E+01	8.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	7.0E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	8.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	8.2E+01	2.0E+00	6.4E+00	10	100	1.04E+03	104%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	8.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	4.0E+03	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T07-B	1	2.60E+00	E		2.60E+00	9.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T08-B	1	1.98E+01			1.98E+01	9.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T09-B	1	4.00E+01			4.00E+01	7.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	3.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	9.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00	10	100	1.05E+03	105%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	2.9E+01	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	6.1E+01	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	4.7E+01	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T07-C	1	2.70E+00	E		2.70E+00	8.6E+00	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T08-C	1	2.04E+01			2.04E+01	1.6E+00	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-T09-C	1	4.13E+01			4.13E+01	9.5E-01	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.9E+02	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-B02-A	1	1.01E+01			1.01E+01	3.8E-01	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1313-B03-A	1	3.64E+00	E		3.64E+00	1.3E+01	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	CFS-L01-1313-T01-A	1	2.56E+01			2.56E+01	3.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T02-A	1	2.41E+01			2.41E+01	6.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T03-A	1	2.58E+01			2.58E+01	1.5E+00	1.5E+00	4.8E+00	10	100	1.17E+03	115%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T04-A	1	2.66E+01			2.66E+01	2.9E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T05-A	1	2.89E+01			2.89E+01	2.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T06-A	1	2.84E+01			2.84E+01	6.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T07-A	1	3.71E+01			3.71E+01	3.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T08-A	1	5.57E+01			5.57E+01	1.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T09-A	1	5.03E+02			5.03E+02	1.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T01-B	1	2.70E+01			2.70E+01	5.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T02-B	1	2.43E+01			2.43E+01	3.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T03-B	1	2.57E+01			2.57E+01	8.1E+00	1.5E+00	4.8E+00	10	100	1.09E+03	106%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T04-B	1	2.59E+01			2.59E+01	8.8E+01	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T05-B	1	2.64E+01			2.64E+01	2.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T06-B	1	2.94E+01			2.94E+01	2.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T07-B	1	3.70E+01			3.70E+01	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T08-B	1	4.89E+01			4.89E+01	1.1E+01	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T09-B	1	5.08E+02			5.08E+02	1.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T01-C	1	2.78E+01			2.78E+01	3.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T02-C	1	2.31E+01			2.31E+01	7.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T03-C	1	2.56E+01			2.56E+01	3.0E+00	1.5E+00	4.8E+00	10	100	1.11E+03	108%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T04-C	1	2.77E+01			2.77E+01	3.4E+00	1.5E+00	4.8E+00					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T05-C	1	2.86E+01			2.86E+01	5.1E-01	1.5E+00	4.8E+00					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T06-C	1	3.03E+01			3.03E+01	5.8E+00	1.5E+00	4.8E+00					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T07-C	1	3.71E+01			3.71E+01	3.5E-01	1.5E+00	4.8E+00					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T08-C	1	5.22E+01			5.22E+01	5.6E+00	1.5E+00	4.8E+00					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-T09-C	1	4.81E+02			4.81E+02	1.3E+00	1.5E+00	4.8E+00					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-B01-A	1	7.50E-01	U1/2		7.50E-01	1.0E+02	1.5E+00	4.8E+00					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-B02-A	1	7.50E-01	U1/2		7.50E-01	5.2E+01	1.5E+00	4.8E+00					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1313-B03-A	1	3.66E+00	E		3.66E+00	1.6E+01	1.5E+00	4.8E+00					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	CFS-L01-1313-T01-A	1	5.59E+03			5.59E+03	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:27 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T02-A	1	3.11E+03			3.11E+03	6.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:28 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T03-A	1	3.84E+01			3.84E+01	1.8E+00	1.0E+00	3.2E+00	10	100	1.06E+03	103%	VU ICP-OES	3/1/11 2:30 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T04-A	1	9.39E+00			9.39E+00	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:32 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T05-A	1	2.45E+02			2.45E+02	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:33 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T06-A	1	2.04E+04			2.04E+04	9.9E-02	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:35 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T07-A	1	1.76E+05			1.76E+05	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:36 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T08-A	1	1.92E+05			1.92E+05	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:38 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T09-A	1	1.75E+05			1.75E+05	2.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:40 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T01-B	1	6.22E+03			6.22E+03	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:48 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T02-B	1	3.24E+03			3.24E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:50 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T03-B	1	3.10E+01			3.10E+01	1.1E+00	1.0E+00	3.2E+00	10	100	1.18E+03	115%	VU ICP-OES	3/1/11 2:51 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T04-B	1	9.71E+00			9.71E+00	8.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:53 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T05-B	1	2.99E+02			2.99E+02	9.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:55 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T06-B	1	1.99E+04			1.99E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:56 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T07-B	1	1.72E+05			1.72E+05	6.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 2:58 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T08-B	1	1.85E+05			1.85E+05	2.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:00 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T09-B	1	1.79E+05			1.79E+05	4.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:01 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T01-C	1	5.95E+03			5.95E+03	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:03 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T02-C	1	2.59E+03			2.59E+03	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:05 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T03-C	1	2.93E+01			2.93E+01	2.3E-01	1.0E+00	3.2E+00	10	100	1.10E+03	107%	VU ICP-OES	3/1/11 3:06 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T04-C	1	1.10E+01			1.10E+01	6.0E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:08 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T05-C	1	2.63E+02			2.63E+02	1.6E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:10 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T06-C	1	2.08E+04			2.08E+04	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:11 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T07-C	1	1.76E+05			1.76E+05	1.6E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:13 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T08-C	1	1.97E+05			1.97E+05	4.8E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:15 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-T09-C	1	1.84E+05			1.84E+05	2.7E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:16 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-B01-A	1	1.97E+00	E		1.97E+00	1.0E+01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 2:22 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-B02-A	1	1.50E+00	E		1.50E+00	1.9E+01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 2:23 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1313-B03-A	1	1.23E+00	E		1.23E+00	1.6E+01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 2:25 PM	EPA Interlab L01 1313-1316 CFS

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	CFS-L04-1313-T01-A	1	1.10E+02			1.10E+02	1.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T02-A	1	1.08E+02			1.08E+02	2.0E+00	1.0E+00	3.2E+00	1000	100	1.27E+03	116%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T03-A	1	9.09E+01			9.09E+01	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T04-A	1	7.36E+01			7.36E+01	4.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T05-A	1	4.86E+01			4.86E+01	5.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T06-A	1	4.78E+01			4.78E+01	4.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T07-A	1	1.97E+03			1.97E+03	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T08-A	1	3.21E+04			3.21E+04	5.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T09-A	1	9.63E+04			9.63E+04	8.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T01-B	1	1.40E+02			1.40E+02	1.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T02-B	1	1.71E+02			1.71E+02	1.7E+00	1.0E+00	3.2E+00	1000	100	1.32E+03	115%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T03-B	1	1.16E+02			1.16E+02	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T04-B	1	6.16E+01			6.16E+01	1.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T05-B	1	4.70E+01			4.70E+01	5.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T06-B	1	5.48E+01			5.48E+01	3.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T07-B	1	6.39E+03			6.39E+03	8.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T08-B	1	2.99E+04			2.99E+04	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T09-B	1	9.07E+04			9.07E+04	1.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T01-C	1	1.15E+02			1.15E+02	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T02-C	1	1.18E+02			1.18E+02	3.1E+00	1.0E+00	3.2E+00	1000	100	1.29E+03	118%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T03-C	1	9.79E+01			9.79E+01	1.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T04-C	1	6.12E+01			6.12E+01	4.1E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T05-C	1	4.15E+01			4.15E+01	7.0E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T06-C	1	5.46E+01			5.46E+01	5.0E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T07-C	1	6.51E+03			6.51E+03	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T08-C	1	6.31E+04			6.31E+04	2.2E-01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-T09-C	1	9.25E+04			9.25E+04	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.3E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	3.9E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	2.0E+02	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	5.3E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-B02-B	1	9.89E+00			9.89E+00	1.9E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	4.8E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	3.7E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	4.1E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	2.5E+02	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	CFS-L04-1313-T01-A	1	3.75E+00	U1/2		3.75E+00	1.2E+02	7.5E+00	2.4E+01			---		VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T02-A	1	3.75E+00	U1/2		3.75E+00	1.4E+02	7.5E+00	2.4E+01	10	100	1.14E+03	114%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T03-A	1	3.21E+01			3.21E+01	1.4E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T04-A	1	2.88E+01			2.88E+01	5.5E+00	7.5E+00	2.4E+01			---		VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T05-A	1	3.01E+01			3.01E+01	3.2E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T06-A	1	3.44E+01			3.44E+01	2.2E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T07-A	1	7.11E+01			7.11E+01	4.2E+00	7.5E+00	2.4E+01			---		VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T08-A	1	6.81E+02			6.81E+02	5.3E+00	7.5E+00	2.4E+01			---		VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T09-A	1	1.69E+03			1.69E+03	5.5E+00	7.5E+00	2.4E+01			---		VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T01-B	1	3.75E+00	U1/2		3.75E+00	8.5E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T02-B	1	1.33E+01	E		1.33E+01	7.0E+01	7.5E+00	2.4E+01	10	100	1.17E+03	116%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T03-B	1	2.65E+01			2.65E+01	3.0E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T04-B	1	4.37E+01			4.37E+01	1.7E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T05-B	1	2.67E+01			2.67E+01	4.6E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T06-B	1	3.64E+01			3.64E+01	3.6E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T07-B	1	1.55E+02			1.55E+02	1.2E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T08-B	1	8.23E+02			8.23E+02	1.1E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T09-B	1	1.47E+03			1.47E+03	4.2E+00	7.5E+00	2.4E+01			---		VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T01-C	1	8.21E+00	E		8.21E+00	1.2E+02	7.5E+00	2.4E+01			---		VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T02-C	1	3.75E+00	U1/2		3.75E+00	2.0E+02	7.5E+00	2.4E+01	10	100	1.19E+03	118%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T03-C	1	2.70E+01			2.70E+01	1.9E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T04-C	1	4.05E+01			4.05E+01	1.9E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T05-C	1	1.71E+01	E		1.71E+01	4.0E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T06-C	1	3.21E+01			3.21E+01	1.1E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T07-C	1	1.84E+02			1.84E+02	9.1E+00	7.5E+00	2.4E+01			---		VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T08-C	1	1.73E+03			1.73E+03	1.3E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-T09-C	1	1.51E+03			1.51E+03	2.8E+00	7.5E+00	2.4E+01			---		VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-B01-A	1	3.75E+00	U1/2		3.75E+00	1.3E+02	7.5E+00	2.4E+01					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-B02-A	1	3.75E+00	U1/2		3.75E+00	8.4E+01	7.5E+00	2.4E+01					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-B03-A	1	8.52E+00	E		8.52E+00	6.8E+01	7.5E+00	2.4E+01					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-B01-B	1	3.75E+00	U1/2		3.75E+00	1.3E+02	7.5E+00	2.4E+01					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-B02-B	1	1.43E+01	E		1.43E+01	2.7E+01	7.5E+00	2.4E+01					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-B03-B	1	3.75E+00	U1/2		3.75E+00	2.1E+02	7.5E+00	2.4E+01					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-B01-C	1	3.75E+00	U1/2		3.75E+00	1.1E+02	7.5E+00	2.4E+01					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-B02-C	1	3.75E+00	U1/2		3.75E+00	4.7E+01	7.5E+00	2.4E+01					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1313-B03-C	1	1.22E+01	E		1.22E+01	1.2E+02	7.5E+00	2.4E+01					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	CFS-L04-1313-T01-A	1	2.79E+02			2.79E+02	5.8E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T02-A	1	2.33E+02			2.33E+02	6.1E+00	1.1E+01	3.5E+01	10	100	1.41E+03	118%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T03-A	1	7.69E+01			7.69E+01	3.7E-01	1.1E+01	3.5E+01			---		VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T04-A	1	4.20E+01			4.20E+01	7.8E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T05-A	1	3.22E+01	E		3.22E+01	1.6E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T06-A	1	1.23E+01	E		1.23E+01	6.7E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T07-A	1	8.31E+01			8.31E+01	1.0E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T08-A	1	1.02E+03			1.02E+03	2.0E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T09-A	1	1.22E+05			1.22E+05	1.4E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T01-B	1	4.35E+02			4.35E+02	1.7E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T02-B	1	2.16E+02			2.16E+02	9.7E-01	1.1E+01	3.5E+01	10	100	1.39E+03	117%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T03-B	1	1.11E+02			1.11E+02	4.1E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T04-B	1	3.56E+01			3.56E+01	6.4E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T05-B	1	2.58E+01	E		2.58E+01	2.7E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T06-B	1	3.46E+01	E		3.46E+01	2.2E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T07-B	1	1.92E+02			1.92E+02	3.5E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T08-B	1	9.40E+02			9.40E+02	2.2E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T09-B	1	9.07E+04			9.07E+04	6.9E-01	1.1E+01	3.5E+01			---		VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T01-C	1	3.90E+02			3.90E+02	3.6E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T02-C	1	3.21E+02			3.21E+02	1.4E+00	1.1E+01	3.5E+01	10	100	1.51E+03	118%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T03-C	1	1.29E+02			1.29E+02	1.1E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T04-C	1	5.00E+01			5.00E+01	1.8E+01	1.1E+01	3.5E+01					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T05-C	1	2.14E+01	E		2.14E+01	4.2E+01	1.1E+01	3.5E+01					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T06-C	1	2.60E+01	E		2.60E+01	2.1E+01	1.1E+01	3.5E+01					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T07-C	1	1.75E+02			1.75E+02	5.5E+00	1.1E+01	3.5E+01					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T08-C	1	5.31E+03			5.31E+03	2.3E+00	1.1E+01	3.5E+01					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-T09-C	1	7.54E+04			7.54E+04	1.5E+00	1.1E+01	3.5E+01					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-B01-A	1	5.50E+00	U1/2		5.50E+00	2.9E+03	1.1E+01	3.5E+01					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-B02-A	1	5.50E+00	U1/2		5.50E+00	2.6E+02	1.1E+01	3.5E+01					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-B03-A	1	1.88E+01	E		1.88E+01	7.1E+00	1.1E+01	3.5E+01					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-B01-B	1	5.50E+00	U1/2		5.50E+00	7.2E+01	1.1E+01	3.5E+01					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-B02-B	1	3.45E+01	E		3.45E+01	1.3E+01	1.1E+01	3.5E+01					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-B03-B	1	5.50E+00	U1/2		5.50E+00	6.2E+00	1.1E+01	3.5E+01					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-B01-C	1	1.17E+01	E		1.17E+01	4.0E+01	1.1E+01	3.5E+01					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-B02-C	1	5.50E+00	U1/2		5.50E+00	5.6E+01	1.1E+01	3.5E+01					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1313-B03-C	1	1.52E+01	E		1.52E+01	2.8E+01	1.1E+01	3.5E+01					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	CFS-L04-1313-T01-A	1	7.88E+01			7.88E+01	3.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T02-A	1	7.75E+01			7.75E+01	2.1E-01	1.0E+00	3.2E+00	1000	100	1.22E+03	114%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T03-A	1	1.55E+02			1.55E+02	1.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T04-A	1	1.26E+02			1.26E+02	2.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T05-A	1	1.55E+02			1.55E+02	8.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T06-A	1	1.56E+02			1.56E+02	2.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T07-A	1	2.74E+02			2.74E+02	1.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T08-A	1	6.45E+02			6.45E+02	9.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T09-A	1	7.44E+02			7.44E+02	6.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T01-B	1	8.21E+01			8.21E+01	3.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T02-B	1	6.39E+01			6.39E+01	3.9E+00	1.0E+00	3.2E+00	1000	100	1.14E+03	108%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T03-B	1	1.65E+02			1.65E+02	1.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T04-B	1	1.07E+02			1.07E+02	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T05-B	1	1.44E+02			1.44E+02	2.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T06-B	1	1.74E+02			1.74E+02	2.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T07-B	1	3.41E+02			3.41E+02	9.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T08-B	1	6.12E+02			6.12E+02	1.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T09-B	1	6.74E+02			6.74E+02	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T01-C	1	4.33E+01			4.33E+01	3.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T02-C	1	4.35E+01			4.35E+01	3.1E+00	1.0E+00	3.2E+00	1000	100	1.17E+03	112%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T03-C	1	1.25E+02			1.25E+02	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T04-C	1	9.02E+01			9.02E+01	1.6E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T05-C	1	1.03E+02			1.03E+02	1.7E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T06-C	1	1.52E+02			1.52E+02	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T07-C	1	3.62E+02			3.62E+02	7.0E-01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T08-C	1	6.87E+02			6.87E+02	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-T09-C	1	7.52E+02			7.52E+02	8.0E-01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-B01-A	1	1.28E+01			1.28E+01	1.6E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-B02-A	1	2.29E+01			2.29E+01	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-B03-A	1	3.89E+01			3.89E+01	6.0E-01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-B01-B	1	3.19E+00			3.19E+00	2.9E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-B02-B	1	1.02E+01			1.02E+01	7.0E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-B03-B	1	1.47E+01			1.47E+01	1.6E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-B01-C	1	3.07E+00	E		3.07E+00	1.1E+02	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-B02-C	1	6.80E+00			6.80E+00	2.2E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1313-B03-C	1	3.60E+01			3.60E+01	4.7E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	CFS-L04-1313-T01-A	1	1.50E+02			1.50E+02	3.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T02-A	1	6.86E+01			6.86E+01	8.4E-01	1.0E+00	3.2E+00	10	100	8.97E+02	83%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T03-A	1	2.83E+02			2.83E+02	2.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T04-A	1	2.04E+02			2.04E+02	7.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T05-A	1	2.27E+02			2.27E+02	3.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T06-A	1	2.27E+02			2.27E+02	7.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T07-A	1	9.92E+01			9.92E+01	2.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T08-A	1	1.01E+02			1.01E+02	3.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T09-A	1	1.11E+02			1.11E+02	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T01-B	1	1.64E+02			1.64E+02	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T02-B	1	7.32E+01			7.32E+01	1.1E+00	1.0E+00	3.2E+00	10	100	9.34E+02	86%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T03-B	1	3.63E+02			3.63E+02	9.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T04-B	1	1.90E+02			1.90E+02	5.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T05-B	1	2.25E+02			2.25E+02	2.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T06-B	1	1.46E+02			1.46E+02	7.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T07-B	1	1.04E+02			1.04E+02	6.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T08-B	1	1.12E+02			1.12E+02	2.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T09-B	1	1.08E+02			1.08E+02	1.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T01-C	1	1.43E+02			1.43E+02	1.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T02-C	1	6.61E+01			6.61E+01	7.5E-01	1.0E+00	3.2E+00	10	100	9.47E+02	88%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T03-C	1	3.41E+02			3.41E+02	3.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T04-C	1	1.88E+02			1.88E+02	1.5E-01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T05-C	1	2.17E+02			2.17E+02	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T06-C	1	1.87E+02			1.87E+02	5.7E-01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T07-C	1	9.93E+01			9.93E+01	7.6E-01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T08-C	1	1.76E+02			1.76E+02	6.2E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-T09-C	1	1.07E+02			1.07E+02	2.5E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.3E+02	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	3.4E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-B03-A	1	3.06E+00	E		3.06E+00	2.5E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	2.3E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-B02-B	1	3.66E+00			3.66E+00	1.8E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	7.1E+02	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	1.8E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	1.9E+03	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1313-B03-C	1	4.42E+00			4.42E+00	4.6E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	CFS-L04-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	3.7E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	2.3E+01	1.9E+00	6.0E+00	10	100	1.13E+03	113%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	6.6E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	6.2E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	1.6E+02	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	2.7E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T07-A	1	2.30E+00	E		2.30E+00	4.8E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T08-A	1	8.66E+00			8.66E+00	1.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T09-A	1	9.50E-01	U1/2		9.50E-01	6.7E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	4.2E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	2.5E+01	1.9E+00	6.0E+00	10	100	1.15E+03	115%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	6.5E+02	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	5.6E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	2.7E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	6.0E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T07-B	1	3.32E+00	E		3.32E+00	2.7E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T08-B	1	6.46E+00			6.46E+00	2.0E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T09-B	1	9.50E-01	U1/2		9.50E-01	3.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	1.1E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	9.1E+01	1.9E+00	6.0E+00	10	100	1.15E+03	115%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	7.3E+02	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	8.3E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	1.5E+02	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	5.9E+00	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T07-C	1	3.61E+00	E		3.61E+00	4.3E+00	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T08-C	1	7.18E+00			7.18E+00	3.0E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-T09-C	1	9.50E-01	U1/2		9.50E-01	1.6E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	2.2E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	6.8E+00	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	1.3E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-B01-B	1	9.50E-01	U1/2		9.50E-01	2.8E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-B02-B	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-B03-B	1	9.50E-01	U1/2		9.50E-01	6.6E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-B01-C	1	9.50E-01	U1/2		9.50E-01	4.3E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-B02-C	1	9.50E-01	U1/2		9.50E-01	6.0E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1313-B03-C	1	9.50E-01	U1/2		9.50E-01	1.6E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	CFS-L04-1313-T01-A	1	1.23E+01			1.23E+01	2.6E+00	2.2E+00	7.0E+00			---		VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T02-A	1	1.01E+01			1.01E+01	1.8E+00	2.2E+00	7.0E+00	10	100	1.16E+03	115%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	4.3E+00	2.2E+00	7.0E+00			---		VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T04-A	1	1.66E+01			1.66E+01	3.1E+00	2.2E+00	7.0E+00			---		VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T05-A	1	4.46E+03			4.46E+03	1.7E-01	2.2E+00	7.0E+00			---		VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T06-A	1	4.20E+03			4.20E+03	6.7E-01	2.2E+00	7.0E+00			---		VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T07-A	1	2.02E+04			2.02E+04	1.5E+00	2.2E+00	7.0E+00			---		VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T08-A	1	4.71E+04			4.71E+04	1.2E+00	2.2E+00	7.0E+00			---		VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T09-A	1	5.09E+04			5.09E+04	1.4E+00	2.2E+00	7.0E+00			---		VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T01-B	1	1.38E+01			1.38E+01	5.1E-01	2.2E+00	7.0E+00			---		VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T02-B	1	6.08E+00	E		6.08E+00	5.4E+00	2.2E+00	7.0E+00	10	100	1.09E+03	109%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	5.8E+01	2.2E+00	7.0E+00			---		VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T04-B	1	1.72E+01			1.72E+01	4.3E+00	2.2E+00	7.0E+00			---		VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T05-B	1	4.14E+03			4.14E+03	4.5E-01	2.2E+00	7.0E+00			---		VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T06-B	1	9.60E+03			9.60E+03	3.3E-01	2.2E+00	7.0E+00			---		VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T07-B	1	2.80E+04			2.80E+04	1.2E+00	2.2E+00	7.0E+00			---		VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T08-B	1	4.66E+04			4.66E+04	6.2E-01	2.2E+00	7.0E+00			---		VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T09-B	1	4.50E+04			4.50E+04	1.0E+00	2.2E+00	7.0E+00			---		VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T01-C	1	1.13E+01			1.13E+01	3.5E+00	2.2E+00	7.0E+00			---		VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T02-C	1	5.34E+00	E		5.34E+00	4.0E+00	2.2E+00	7.0E+00	10	100	1.10E+03	109%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	3.7E+01	2.2E+00	7.0E+00			---		VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T04-C	1	1.57E+01			1.57E+01	1.9E+00	2.2E+00	7.0E+00					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T05-C	1	1.77E+03			1.77E+03	7.8E-01	2.2E+00	7.0E+00					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T06-C	1	7.37E+03			7.37E+03	5.5E-01	2.2E+00	7.0E+00					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T07-C	1	2.98E+04			2.98E+04	8.1E-01	2.2E+00	7.0E+00					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T08-C	1	5.01E+04			5.01E+04	1.6E+00	2.2E+00	7.0E+00					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-T09-C	1	5.00E+04			5.00E+04	4.0E-01	2.2E+00	7.0E+00					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	5.1E+01	2.2E+00	7.0E+00					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	6.4E+01	2.2E+00	7.0E+00					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-B03-A	1	1.10E+00	U1/2		1.10E+00	6.0E+01	2.2E+00	7.0E+00					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-B01-B	1	1.10E+00	U1/2		1.10E+00	2.5E+03	2.2E+00	7.0E+00					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-B02-B	1	6.90E+00	E		6.90E+00	5.5E+00	2.2E+00	7.0E+00					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-B03-B	1	1.10E+00	U1/2		1.10E+00	5.9E+02	2.2E+00	7.0E+00					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-B01-C	1	1.10E+00	U1/2		1.10E+00	4.4E+01	2.2E+00	7.0E+00					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-B02-C	1	1.10E+00	U1/2		1.10E+00	4.5E+01	2.2E+00	7.0E+00					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1313-B03-C	1	1.10E+00	U1/2		1.10E+00	1.2E+03	2.2E+00	7.0E+00					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	CFS-L04-1313-T01-A	1	4.98E+05			4.98E+05	3.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T02-A	1	5.64E+05			5.64E+05	2.7E-01	2.6E+00	8.3E+00	1000	100	5.65E+05	92%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T03-A	1	5.84E+05			5.84E+05	2.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T04-A	1	5.86E+05			5.86E+05	1.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T05-A	1	6.67E+05			6.67E+05	3.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T06-A	1	6.51E+05			6.51E+05	1.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T07-A	1	8.04E+05			8.04E+05	2.8E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T08-A	1	1.19E+06			1.19E+06	4.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T09-A	1	1.67E+06			1.67E+06	1.5E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T01-B	1	4.79E+05			4.79E+05	6.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T02-B	1	6.39E+05			6.39E+05	9.6E-01	2.6E+00	8.3E+00	1000	100	6.40E+05	89%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T03-B	1	6.03E+05			6.03E+05	2.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T04-B	1	5.90E+05			5.90E+05	3.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T05-B	1	6.39E+05			6.39E+05	9.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T06-B	1	6.79E+05			6.79E+05	4.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T07-B	1	8.85E+05			8.85E+05	3.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T08-B	1	1.19E+06			1.19E+06	1.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T09-B	1	1.54E+06			1.54E+06	7.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T01-C	1	3.75E+05			3.75E+05	2.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T02-C	1	5.75E+05			5.75E+05	4.2E-01	2.6E+00	8.3E+00	1000	100	5.76E+05	86%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T03-C	1	5.34E+05			5.34E+05	6.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T04-C	1	5.70E+05			5.70E+05	3.7E-01	2.6E+00	8.3E+00					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T05-C	1	5.99E+05			5.99E+05	6.4E-01	2.6E+00	8.3E+00					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T06-C	1	6.79E+05			6.79E+05	1.0E-01	2.6E+00	8.3E+00					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T07-C	1	9.24E+05			9.24E+05	7.6E-01	2.6E+00	8.3E+00					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T08-C	1	1.35E+06			1.35E+06	2.6E+00	2.6E+00	8.3E+00					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-T09-C	1	1.54E+06			1.54E+06	9.8E-01	2.6E+00	8.3E+00					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-B01-A	1	8.09E+00	E		8.09E+00	1.2E+02	2.6E+00	8.3E+00					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-B02-A	1	6.91E+01			6.91E+01	1.1E+01	2.6E+00	8.3E+00					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-B03-A	1	2.08E+01			2.08E+01	2.3E+01	2.6E+00	8.3E+00					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-B01-B	1	5.94E+00	E		5.94E+00	7.0E+01	2.6E+00	8.3E+00					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-B02-B	1	1.33E+02			1.33E+02	9.6E+00	2.6E+00	8.3E+00					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-B03-B	1	1.01E+01			1.01E+01	2.8E+01	2.6E+00	8.3E+00					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-B01-C	1	1.30E+00	U1/2		1.30E+00	1.0E+03	2.6E+00	8.3E+00					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-B02-C	1	6.43E+01			6.43E+01	1.5E+01	2.6E+00	8.3E+00					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1313-B03-C	1	1.65E+01			1.65E+01	1.3E+02	2.6E+00	8.3E+00					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	CFS-L04-1313-T01-A	1	1.27E+02			1.27E+02	3.6E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T02-A	1	1.15E+02			1.15E+02	1.5E+00	1.2E+00	3.8E+00	10	100	1.24E+03	112%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T03-A	1	6.37E+00			6.37E+00	1.1E+01	1.2E+00	3.8E+00			---		VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T04-A	1	2.38E+00	E		2.38E+00	2.8E+01	1.2E+00	3.8E+00			---		VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T05-A	1	6.00E-01	U1/2		6.00E-01	4.7E+02	1.2E+00	3.8E+00			---		VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T06-A	1	6.00E-01	U1/2		6.00E-01	2.0E+02	1.2E+00	3.8E+00			---		VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T07-A	1	6.00E-01	U1/2		6.00E-01	1.8E+02	1.2E+00	3.8E+00			---		VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T08-A	1	4.34E+01			4.34E+01	1.5E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T09-A	1	2.28E+03			2.28E+03	8.0E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T01-B	1	1.59E+02			1.59E+02	4.9E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T02-B	1	9.14E+01			9.14E+01	9.0E-01	1.2E+00	3.8E+00	10	100	1.15E+03	106%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T03-B	1	9.93E+00			9.93E+00	4.8E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T04-B	1	1.43E+00	E		1.43E+00	4.9E+01	1.2E+00	3.8E+00			---		VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T05-B	1	6.00E-01	U1/2		6.00E-01	1.9E+02	1.2E+00	3.8E+00			---		VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T06-B	1	6.00E-01	U1/2		6.00E-01	4.1E+02	1.2E+00	3.8E+00			---		VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T07-B	1	6.00E-01	U1/2		6.00E-01	3.7E+01	1.2E+00	3.8E+00			---		VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T08-B	1	3.58E+01			3.58E+01	1.6E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T09-B	1	2.06E+03			2.06E+03	1.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T01-C	1	1.39E+02			1.39E+02	3.6E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T02-C	1	9.20E+01			9.20E+01	2.6E-01	1.2E+00	3.8E+00	10	100	1.18E+03	108%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T03-C	1	1.03E+01			1.03E+01	2.9E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T04-C	1	2.24E+00	E		2.24E+00	1.1E+01	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T05-C	1	6.00E-01	U1/2		6.00E-01	3.7E+01	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T06-C	1	6.00E-01	U1/2		6.00E-01	8.4E+01	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T07-C	1	6.00E-01	U1/2		6.00E-01	5.4E+01	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T08-C	1	3.25E+02			3.25E+02	3.9E-01	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-T09-C	1	2.05E+03			2.05E+03	6.0E-01	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	2.9E+02	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	1.6E+03	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-B03-A	1	6.00E-01	U1/2		6.00E-01	6.0E+01	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-B01-B	1	6.00E-01	U1/2		6.00E-01	7.7E+02	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-B02-B	1	6.00E-01	U1/2		6.00E-01	5.3E+01	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-B03-B	1	6.00E-01	U1/2		6.00E-01	6.7E+01	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-B01-C	1	6.00E-01	U1/2		6.00E-01	3.5E+01	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-B02-C	1	6.00E-01	U1/2		6.00E-01	2.7E+02	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1313-B03-C	1	6.00E-01	U1/2		6.00E-01	2.1E+01	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	CFS-L04-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	2.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00	10	100	1.13E+03	113%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	5.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	1.2E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T05-A	1	1.01E+02			1.01E+02	3.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T06-A	1	9.34E+01			9.34E+01	1.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T07-A	1	4.86E+02			4.86E+02	9.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T08-A	1	1.63E+03			1.63E+03	9.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T09-A	1	1.91E+03			1.91E+03	2.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	9.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	5.2E+01	1.8E+00	5.7E+00	10	100	1.08E+03	108%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	6.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	5.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T05-B	1	8.92E+01			8.92E+01	2.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T06-B	1	1.99E+02			1.99E+02	5.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T07-B	1	7.75E+02			7.75E+02	1.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T08-B	1	1.62E+03			1.62E+03	9.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T09-B	1	1.67E+03			1.67E+03	6.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	2.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	2.4E+01	1.8E+00	5.7E+00	10	100	1.08E+03	108%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	3.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	3.1E+01	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T05-C	1	3.79E+01			3.79E+01	7.3E-01	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T06-C	1	1.53E+02			1.53E+02	8.8E-01	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T07-C	1	8.44E+02			8.44E+02	5.6E-01	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T08-C	1	1.84E+03			1.84E+03	7.6E+00	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-T09-C	1	1.80E+03			1.80E+03	8.7E-01	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	3.2E+02	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	6.0E+01	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	6.4E+01	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-B01-B	1	9.00E-01	U1/2		9.00E-01	5.7E+01	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-B02-B	1	9.00E-01	U1/2		9.00E-01	4.8E+01	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-B03-B	1	9.00E-01	U1/2		9.00E-01	8.9E+01	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-B01-C	1	9.00E-01	U1/2		9.00E-01	2.9E+01	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-B02-C	1	9.00E-01	U1/2		9.00E-01	4.9E+01	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1313-B03-C	1	9.00E-01	U1/2		9.00E-01	3.1E+02	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	CFS-L04-1313-T01-A	1	7.88E+03			7.88E+03	1.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T02-A	1	6.65E+03			6.65E+03	1.7E+00	3.7E+00	1.2E+01	10	100	7.66E+03	101%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T03-A	1	1.23E+02			1.23E+02	2.0E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T04-A	1	6.97E+01			6.97E+01	1.3E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T05-A	1	7.79E+02			7.79E+02	3.6E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T06-A	1	6.96E+02			6.96E+02	7.5E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T07-A	1	1.17E+05			1.17E+05	3.7E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T08-A	1	9.34E+05			9.34E+05	1.1E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T09-A	1	1.12E+06			1.12E+06	1.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T01-B	1	8.46E+03			8.46E+03	1.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T02-B	1	2.32E+03			2.32E+03	9.2E-01	3.7E+00	1.2E+01	10	100	3.28E+03	96%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T03-B	1	1.73E+02			1.73E+02	8.6E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T04-B	1	5.65E+01			5.65E+01	1.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T05-B	1	6.54E+02			6.54E+02	1.1E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T06-B	1	6.32E+03			6.32E+03	6.1E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T07-B	1	3.30E+05			3.30E+05	1.1E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T08-B	1	8.96E+05			8.96E+05	1.6E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T09-B	1	1.01E+06			1.01E+06	1.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T01-C	1	7.51E+03			7.51E+03	4.7E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T02-C	1	2.20E+03			2.20E+03	8.4E-01	3.7E+00	1.2E+01	10	100	3.26E+03	107%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T03-C	1	1.62E+02			1.62E+02	1.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T04-C	1	5.89E+01			5.89E+01	1.8E+00	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T05-C	1	1.66E+02			1.66E+02	2.0E+00	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T06-C	1	4.37E+03			4.37E+03	5.6E-01	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T07-C	1	3.29E+05			3.29E+05	6.6E-01	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T08-C	1	1.00E+06			1.00E+06	1.6E+00	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-T09-C	1	1.08E+06			1.08E+06	1.2E+00	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	2.2E+02	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	1.7E+02	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-B03-A	1	1.85E+00	U1/2		1.85E+00	3.6E+02	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-B01-B	1	5.04E+00	E		5.04E+00	2.8E+00	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-B02-B	1	2.27E+02			2.27E+02	9.2E-01	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-B03-B	1	1.85E+00	U1/2		1.85E+00	1.8E+02	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-B01-C	1	1.85E+00	U1/2		1.85E+00	1.3E+02	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-B02-C	1	1.85E+00	U1/2		1.85E+00	1.6E+01	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1313-B03-C	1	1.85E+00	U1/2		1.85E+00	2.0E+02	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	CFS-L04-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	2.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	1.3E+01	2.0E+00	6.4E+00	1000	100	1.06E+03	106%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	9.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T04-A	1	1.07E+01			1.07E+01	4.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	5.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T08-A	1	5.51E+03			5.51E+03	1.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T09-A	1	2.86E+05			2.86E+05	2.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	3.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00	1000	100	1.01E+03	101%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	1.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T07-B	1	1.27E+01			1.27E+01	2.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T08-B	1	3.50E+04			3.50E+04	1.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T09-B	1	2.57E+05			2.57E+05	3.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	2.0E+00	2.0E+00	6.4E+00	1000	100	1.01E+03	101%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	9.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	5.8E+00	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T07-C	1	1.94E+01			1.94E+01	3.8E+00	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T08-C	1	1.26E+05			1.26E+05	1.5E+00	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-T09-C	1	2.29E+05			2.29E+05	5.5E-01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	7.6E+00	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	3.8E+00	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	9.9E+01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	9.4E+00	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-B02-B	1	1.60E+02			1.60E+02	8.5E-01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	7.2E+00	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	3.1E+01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1313-B03-C	1	1.00E+00	U1/2		1.00E+00	1.8E+02	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	CFS-L04-1313-T01-A	1	1.57E+03			1.57E+03	7.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T02-A	1	6.17E+03			6.17E+03	2.6E+00	6.8E+00	2.2E+01	10	100	7.05E+03	88%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T03-A	1	4.73E+02			4.73E+02	1.3E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T04-A	1	1.44E+02			1.44E+02	2.9E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T05-A	1	1.19E+03			1.19E+03	4.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T06-A	1	1.14E+03			1.14E+03	1.2E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T07-A	1	6.10E+03			6.10E+03	7.0E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T08-A	1	6.88E+03			6.88E+03	1.3E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T09-A	1	9.59E+03			9.59E+03	8.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T01-B	1	2.10E+03			2.10E+03	7.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T02-B	1	9.86E+03			9.86E+03	6.0E-01	6.8E+00	2.2E+01	10	100	1.08E+04	93%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T03-B	1	1.00E+03			1.00E+03	7.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T04-B	1	1.49E+02			1.49E+02	3.3E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T05-B	1	1.14E+03			1.14E+03	6.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T06-B	1	1.67E+03			1.67E+03	4.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T07-B	1	7.92E+03			7.92E+03	1.2E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T08-B	1	6.50E+03			6.50E+03	1.2E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T09-B	1	8.88E+03			8.88E+03	1.5E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T01-C	1	1.54E+03			1.54E+03	2.2E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T02-C	1	8.69E+03			8.69E+03	8.5E-01	6.8E+00	2.2E+01	10	100	9.67E+03	98%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T03-C	1	7.19E+02			7.19E+02	3.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T04-C	1	1.50E+02			1.50E+02	1.1E+00	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T05-C	1	8.14E+02			8.14E+02	3.8E-01	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T06-C	1	1.42E+03			1.42E+03	4.2E-01	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T07-C	1	8.15E+03			8.15E+03	1.7E+00	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T08-C	1	6.97E+03			6.97E+03	1.7E+00	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-T09-C	1	8.85E+03			8.85E+03	9.2E-01	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	2.2E+01	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	1.6E+01	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	2.7E+01	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-B01-B	1	3.40E+00	U1/2		3.40E+00	8.7E+00	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-B02-B	1	1.85E+02			1.85E+02	2.0E+00	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-B03-B	1	3.40E+00	U1/2		3.40E+00	2.1E+01	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-B01-C	1	3.40E+00	U1/2		3.40E+00	2.2E+01	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-B02-C	1	3.40E+00	U1/2		3.40E+00	1.2E+02	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1313-B03-C	1	3.40E+00	U1/2		3.40E+00	2.2E+01	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	CFS-L04-1313-T01-A	1	2.01E+01			2.01E+01	6.0E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T02-A	1	1.99E+01			1.99E+01	4.9E-02	1.9E+00	6.0E+00	10	100	8.94E+02	87%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T03-A	1	2.01E+01			2.01E+01	6.6E-01	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T04-A	1	2.03E+01			2.03E+01	7.2E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T05-A	1	1.88E+01			1.88E+01	7.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T06-A	1	1.82E+01			1.82E+01	1.0E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T07-A	1	1.97E+01			1.97E+01	2.6E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T08-A	1	2.02E+01			2.02E+01	1.7E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T09-A	1	5.64E+01			5.64E+01	9.9E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T01-B	1	2.19E+01			2.19E+01	6.1E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T02-B	1	2.09E+01			2.09E+01	3.0E+00	1.9E+00	6.0E+00	10	100	8.64E+02	84%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T03-B	1	2.04E+01			2.04E+01	8.1E-01	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T04-B	1	1.81E+01			1.81E+01	3.2E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T05-B	1	1.68E+01			1.68E+01	7.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T06-B	1	1.76E+01			1.76E+01	5.1E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T07-B	1	1.62E+01			1.62E+01	5.7E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T08-B	1	2.16E+01			2.16E+01	1.1E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T09-B	1	4.34E+01			4.34E+01	1.6E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T01-C	1	2.01E+01			2.01E+01	6.3E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T02-C	1	1.96E+01			1.96E+01	5.3E+00	1.9E+00	6.0E+00	10	100	8.76E+02	86%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T03-C	1	1.86E+01			1.86E+01	2.6E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T04-C	1	1.91E+01			1.91E+01	4.8E+00	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T05-C	1	1.98E+01			1.98E+01	1.4E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T06-C	1	1.72E+01			1.72E+01	1.1E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T07-C	1	1.99E+01			1.99E+01	1.9E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T08-C	1	2.46E+01			2.46E+01	1.8E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-T09-C	1	4.41E+01			4.41E+01	1.4E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-B01-A	1	6.01E+00			6.01E+00	1.4E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-B02-A	1	6.91E+00			6.91E+00	1.7E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-B03-A	1	5.76E+00	E		5.76E+00	2.0E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-B01-B	1	6.16E+00			6.16E+00	1.9E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-B02-B	1	5.68E+00	E		5.68E+00	7.2E+00	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-B03-B	1	5.11E+00	E		5.11E+00	2.1E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-B01-C	1	5.68E+00	E		5.68E+00	1.1E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-B02-C	1	6.66E+00			6.66E+00	7.0E+00	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1313-B03-C	1	4.97E+00	E		4.97E+00	3.4E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	CFS-L04-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	3.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	5.2E+01	2.0E+00	6.4E+00	10	100	9.73E+02	97%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T04-A	1	2.06E+00	E		2.06E+00	7.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T05-A	1	1.50E+03			1.50E+03	1.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T06-A	1	1.42E+03			1.42E+03	1.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T07-A	1	4.66E+03			4.66E+03	3.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T08-A	1	1.98E+04			1.98E+04	6.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T09-A	1	3.30E+04			3.30E+04	3.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	3.7E+01	2.0E+00	6.4E+00	10	100	9.26E+02	93%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	1.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	3.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T05-B	1	1.38E+03			1.38E+03	3.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T06-B	1	2.16E+03			2.16E+03	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T07-B	1	6.85E+03			6.85E+03	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T08-B	1	1.95E+04			1.95E+04	9.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T09-B	1	2.99E+04			2.99E+04	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	2.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	4.9E+00	2.0E+00	6.4E+00	10	100	9.27E+02	93%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	3.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	4.7E+00	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T05-C	1	7.70E+02			7.70E+02	8.5E-01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T06-C	1	1.91E+03			1.91E+03	2.0E-01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T07-C	1	7.99E+03			7.99E+03	1.3E+00	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T08-C	1	2.30E+04			2.30E+04	2.8E+00	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-T09-C	1	3.07E+04			3.07E+04	4.0E-01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	3.2E+00	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-B02-B	1	2.22E+00	E		2.22E+00	2.8E+00	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	8.9E+01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	4.5E+01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1313-B03-C	1	1.00E+00	U1/2		1.00E+00	6.1E+01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	CFS-L04-1313-T01-A	1	1.40E+01			1.40E+01	2.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T02-A	1	3.05E+01			3.05E+01	5.6E+00	1.0E+00	3.2E+00	1000	100	1.13E+03	110%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T03-A	1	2.67E+03			2.67E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T04-A	1	3.60E+04			3.60E+04	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T05-A	1	6.88E+04			6.88E+04	1.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T06-A	1	6.74E+04			6.74E+04	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T07-A	1	7.18E+04			7.18E+04	9.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T08-A	1	1.30E+05			1.30E+05	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T09-A	1	2.18E+05			2.18E+05	9.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T01-B	1	1.78E+01			1.78E+01	2.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T02-B	1	2.70E+01			2.70E+01	4.6E+01	1.0E+00	3.2E+00	1000	100	1.09E+03	106%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T03-B	1	8.18E+02			8.18E+02	6.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T04-B	1	3.61E+04			3.61E+04	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T05-B	1	6.91E+04			6.91E+04	3.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T06-B	1	6.89E+04			6.89E+04	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T07-B	1	7.91E+04			7.91E+04	8.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T08-B	1	1.34E+05			1.34E+05	9.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T09-B	1	2.20E+05			2.20E+05	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T01-C	1	6.74E+00			6.74E+00	8.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T02-C	1	2.01E+01			2.01E+01	5.4E+01	1.0E+00	3.2E+00	1000	100	1.10E+03	108%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T03-C	1	1.34E+03			1.34E+03	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T04-C	1	3.80E+04			3.80E+04	7.9E-01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T05-C	1	6.68E+04			6.68E+04	5.4E-01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T06-C	1	7.25E+04			7.25E+04	4.8E-01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T07-C	1	8.45E+04			8.45E+04	4.8E-01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T08-C	1	1.88E+05			1.88E+05	6.5E-01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-T09-C	1	2.21E+05			2.21E+05	9.1E-01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.0E+02	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	2.7E+02	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	8.1E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-B01-B	1	1.75E+00	E		1.75E+00	3.0E+02	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-B02-B	1	8.26E+00			8.26E+00	6.1E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	5.2E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	4.6E+02	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	2.1E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	1.8E+02	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	CFS-L04-1313-T01-A	1	1.99E+03			1.99E+03	9.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T02-A	1	1.91E+03			1.91E+03	6.2E-01	1.2E+00	3.8E+00	10	100	2.90E+03	99%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T03-A	1	1.02E+03			1.02E+03	4.8E-02	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T04-A	1	3.71E+02			3.71E+02	5.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T05-A	1	1.28E+01			1.28E+01	1.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T06-A	1	1.09E+01			1.09E+01	4.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T07-A	1	7.95E+00			7.95E+00	4.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T08-A	1	1.04E+01			1.04E+01	1.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T09-A	1	1.83E+02			1.83E+02	9.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T01-B	1	2.70E+03			2.70E+03	3.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T02-B	1	1.75E+03			1.75E+03	3.3E-01	1.2E+00	3.8E+00	10	100	2.71E+03	96%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T03-B	1	1.18E+03			1.18E+03	1.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T04-B	1	3.75E+02			3.75E+02	4.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T05-B	1	1.23E+01			1.23E+01	8.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T06-B	1	1.05E+01			1.05E+01	4.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T07-B	1	8.84E+00			8.84E+00	2.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T08-B	1	1.20E+01			1.20E+01	1.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T09-B	1	1.45E+02			1.45E+02	3.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T01-C	1	2.06E+03			2.06E+03	1.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T02-C	1	2.13E+03			2.13E+03	4.2E-01	1.2E+00	3.8E+00	10	100	3.14E+03	101%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T03-C	1	1.21E+03			1.21E+03	1.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T04-C	1	3.80E+02			3.80E+02	5.8E-01	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T05-C	1	1.74E+01			1.74E+01	3.6E+00	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T06-C	1	1.03E+01			1.03E+01	1.1E+01	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T07-C	1	7.71E+00			7.71E+00	4.5E+00	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T08-C	1	2.52E+01			2.52E+01	8.5E+01	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-T09-C	1	1.07E+02			1.07E+02	3.5E+00	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-B01-A	1	1.61E+00	E		1.61E+00	6.4E+01	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-B02-A	1	1.65E+00	E		1.65E+00	3.6E+01	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-B03-A	1	6.14E+00			6.14E+00	3.3E+01	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-B01-B	1	1.65E+00	E		1.65E+00	5.1E+01	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-B02-B	1	3.99E+00			3.99E+00	3.1E+00	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-B03-B	1	1.74E+00	E		1.74E+00	3.5E+01	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-B01-C	1	1.44E+00	E		1.44E+00	3.3E+01	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-B02-C	1	6.00E-01	U1/2		6.00E-01	3.7E+01	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1313-B03-C	1	3.13E+00	E		3.13E+00	9.8E+00	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	CFS-L04-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	3.3E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	6.2E+03	1.8E+00	5.7E+00	10	100	1.13E+03	113%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	1.6E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	2.2E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T05-A	1	2.15E+02			2.15E+02	1.4E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T06-A	1	1.87E+02			1.87E+02	1.8E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T07-A	1	1.70E+03			1.70E+03	7.2E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T08-A	1	6.04E+03			6.04E+03	1.1E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T09-A	1	6.75E+03			6.75E+03	1.6E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	8.4E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00	10	100	1.08E+03	108%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	1.6E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T05-B	1	1.80E+02			1.80E+02	8.6E-01	1.8E+00	5.7E+00			---		VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T06-B	1	5.18E+02			5.18E+02	1.0E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T07-B	1	2.87E+03			2.87E+03	4.5E-01	1.8E+00	5.7E+00			---		VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T08-B	1	6.05E+03			6.05E+03	1.2E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T09-B	1	6.15E+03			6.15E+03	1.1E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	2.0E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.8E+00	5.7E+00	10	100	1.08E+03	108%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	4.8E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	4.1E+02	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T05-C	1	6.36E+01			6.36E+01	1.8E+00	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T06-C	1	3.75E+02			3.75E+02	1.1E+00	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T07-C	1	2.95E+03			2.95E+03	5.0E-01	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T08-C	1	6.42E+03			6.42E+03	1.1E+00	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-T09-C	1	6.70E+03			6.70E+03	7.7E-01	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	9.1E+01	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	1.6E+02	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	6.9E+02	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-B01-B	1	9.00E-01	U1/2		9.00E-01	2.9E+01	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-B02-B	1	9.00E-01	U1/2		9.00E-01	2.2E+02	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-B03-B	1	9.00E-01	U1/2		9.00E-01	5.5E+01	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-B01-C	1	9.00E-01	U1/2		9.00E-01	1.3E+01	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-B02-C	1	9.00E-01	U1/2		9.00E-01	2.7E+02	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1313-B03-C	1	9.00E-01	U1/2		9.00E-01	9.5E+02	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	CFS-L04-1313-T01-A	1	7.06E+01			7.06E+01	1.6E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T02-A	1	8.38E+01			8.38E+01	1.0E+01	3.7E+00	1.2E+01	1000	100	1.21E+03	112%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T03-A	1	7.01E+01			7.01E+01	2.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T04-A	1	3.66E+01			3.66E+01	2.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T05-A	1	2.20E+01			2.20E+01	2.9E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T06-A	1	3.79E+01			3.79E+01	2.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T07-A	1	4.80E+01			4.80E+01	3.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T08-A	1	4.11E+01			4.11E+01	3.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T09-A	1	5.51E+03			5.51E+03	7.0E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T01-B	1	1.17E+02			1.17E+02	7.8E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T02-B	1	9.91E+01			9.91E+01	5.3E+00	3.7E+00	1.2E+01	1000	100	1.23E+03	113%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T03-B	1	7.58E+01			7.58E+01	3.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T04-B	1	4.03E+01			4.03E+01	8.0E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T05-B	1	5.69E+01			5.69E+01	3.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T06-B	1	5.59E+01			5.59E+01	2.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T07-B	1	4.22E+01			4.22E+01	1.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T08-B	1	5.18E+01			5.18E+01	1.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T09-B	1	4.16E+03			4.16E+03	1.8E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T01-C	1	9.99E+01			9.99E+01	3.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T02-C	1	1.07E+02			1.07E+02	4.9E+00	3.7E+00	1.2E+01	1000	100	1.22E+03	112%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T03-C	1	6.22E+01			6.22E+01	8.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T04-C	1	3.72E+01			3.72E+01	2.3E+01	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T05-C	1	2.86E+01			2.86E+01	3.5E+01	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T06-C	1	3.65E+01			3.65E+01	3.8E+01	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T07-C	1	3.00E+01			3.00E+01	2.3E+01	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T08-C	1	1.28E+02			1.28E+02	1.3E+01	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-T09-C	1	2.68E+03			2.68E+03	1.5E-01	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-B01-A	1	3.42E+01			3.42E+01	1.1E+01	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-B02-A	1	3.21E+01			3.21E+01	7.2E+00	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-B03-A	1	5.99E+01			5.99E+01	1.3E+01	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-B01-B	1	3.07E+01			3.07E+01	3.2E+01	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-B02-B	1	4.15E+01			4.15E+01	1.2E+01	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-B03-B	1	5.50E+01			5.50E+01	2.2E+01	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-B01-C	1	4.02E+01			4.02E+01	2.4E+01	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-B02-C	1	3.16E+01			3.16E+01	2.6E+01	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1313-B03-C	1	1.35E+02			1.35E+02	9.6E+00	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	CFS-L04-1313-T01-A	1	2.59E+06			2.59E+06	1.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T02-A	1	2.64E+06			2.64E+06	6.4E-01	1.6E+00	5.1E+00	1000	100	2.64E+06	84%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T03-A	1	5.23E+05			5.23E+05	4.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T04-A	1	3.43E+05			3.43E+05	7.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T05-A	1	1.04E+04			1.04E+04	4.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T06-A	1	1.01E+04			1.01E+04	6.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T07-A	1	1.21E+04			1.21E+04	8.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T08-A	1	1.74E+04			1.74E+04	5.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T09-A	1	2.74E+04			2.74E+04	2.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T01-B	1	2.75E+06			2.75E+06	6.4E-02	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T02-B	1	2.69E+06			2.69E+06	1.8E+00	1.6E+00	5.1E+00	1000	100	2.69E+06	88%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T03-B	1	5.82E+05			5.82E+05	4.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T04-B	1	3.38E+05			3.38E+05	5.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T05-B	1	1.03E+04			1.03E+04	4.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T06-B	1	1.04E+04			1.04E+04	7.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T07-B	1	1.30E+04			1.30E+04	9.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T08-B	1	1.71E+04			1.71E+04	1.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T09-B	1	2.74E+04			2.74E+04	1.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T01-C	1	2.63E+06			2.63E+06	2.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T02-C	1	2.46E+06			2.46E+06	5.5E-01	1.6E+00	5.1E+00	1000	100	2.46E+06	82%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T03-C	1	5.29E+05			5.29E+05	1.6E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T04-C	1	3.13E+05			3.13E+05	2.8E-01	1.6E+00	5.1E+00					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T05-C	1	1.07E+05			1.07E+05	8.7E-01	1.6E+00	5.1E+00					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T06-C	1	1.06E+04			1.06E+04	4.0E-01	1.6E+00	5.1E+00					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T07-C	1	1.34E+04			1.34E+04	8.7E-01	1.6E+00	5.1E+00					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T08-C	1	2.15E+04			2.15E+04	2.9E+00	1.6E+00	5.1E+00					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-T09-C	1	2.64E+04			2.64E+04	1.0E+00	1.6E+00	5.1E+00					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-B01-A	1	7.34E+01			7.34E+01	4.0E+00	1.6E+00	5.1E+00					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-B02-A	1	9.45E+01			9.45E+01	5.6E+00	1.6E+00	5.1E+00					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-B03-A	1	2.59E+06			2.59E+06	3.2E-01	1.6E+00	5.1E+00					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-B01-B	1	2.27E+02			2.27E+02	1.1E+01	1.6E+00	5.1E+00					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-B02-B	1	1.05E+02			1.05E+02	9.9E-02	1.6E+00	5.1E+00					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-B03-B	1	4.78E+05			4.78E+05	6.4E-01	1.6E+00	5.1E+00					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-B01-C	1	1.02E+02			1.02E+02	3.2E+00	1.6E+00	5.1E+00					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-B02-C	1	1.53E+02			1.53E+02	9.1E-01	1.6E+00	5.1E+00					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1313-B03-C	1	2.62E+06			2.62E+06	2.7E-01	1.6E+00	5.1E+00					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	CFS-L04-1313-T01-A	1	3.42E+02			3.42E+02	1.3E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T02-A	1	3.39E+02			3.39E+02	4.0E+00	1.5E+01	4.8E+01	10	100	1.49E+03	115%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T03-A	1	4.01E+02			4.01E+02	3.6E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T04-A	1	1.52E+02			1.52E+02	4.6E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T05-A	1	8.46E+01			8.46E+01	1.5E+01	1.5E+01	4.8E+01			---		VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T06-A	1	7.31E+01			7.31E+01	1.5E+01	1.5E+01	4.8E+01			---		VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T07-A	1	1.01E+02			1.01E+02	4.6E+01	1.5E+01	4.8E+01			---		VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T08-A	1	2.15E+02			2.15E+02	8.5E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T09-A	1	7.27E+02			7.27E+02	2.2E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T01-B	1	4.77E+02			4.77E+02	7.0E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T02-B	1	3.34E+02			3.34E+02	2.8E-01	1.5E+01	4.8E+01	10	100	1.45E+03	111%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T03-B	1	5.74E+02			5.74E+02	1.5E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T04-B	1	1.48E+02			1.48E+02	3.6E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T05-B	1	8.95E+01			8.95E+01	9.2E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T06-B	1	8.44E+01			8.44E+01	1.2E+01	1.5E+01	4.8E+01			---		VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T07-B	1	1.34E+02			1.34E+02	5.5E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T08-B	1	2.19E+02			2.19E+02	3.7E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T09-B	1	5.97E+02			5.97E+02	1.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T01-C	1	4.06E+02			4.06E+02	2.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T02-C	1	3.69E+02			3.69E+02	1.7E+00	1.5E+01	4.8E+01	10	100	1.54E+03	117%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T03-C	1	5.74E+02			5.74E+02	1.7E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T04-C	1	1.44E+02			1.44E+02	9.9E+00	1.5E+01	4.8E+01					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T05-C	1	8.43E+01			8.43E+01	6.0E+00	1.5E+01	4.8E+01					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T06-C	1	9.04E+01			9.04E+01	9.4E-01	1.5E+01	4.8E+01					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T07-C	1	1.65E+02			1.65E+02	3.3E+00	1.5E+01	4.8E+01					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T08-C	1	2.42E+02			2.42E+02	1.0E+01	1.5E+01	4.8E+01					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-T09-C	1	4.99E+02			4.99E+02	5.2E+00	1.5E+01	4.8E+01					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-B01-A	1	7.50E+00	U1/2		7.50E+00	5.9E+02	1.5E+01	4.8E+01					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-B02-A	1	7.50E+00	U1/2		7.50E+00	6.4E+01	1.5E+01	4.8E+01					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-B03-A	1	7.50E+00	U1/2		7.50E+00	6.2E+01	1.5E+01	4.8E+01					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-B01-B	1	7.50E+00	U1/2		7.50E+00	6.0E+02	1.5E+01	4.8E+01					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-B02-B	1	7.50E+00	U1/2		7.50E+00	1.7E+02	1.5E+01	4.8E+01					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-B03-B	1	7.50E+00	U1/2		7.50E+00	1.1E+03	1.5E+01	4.8E+01					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-B01-C	1	7.50E+00	U1/2		7.50E+00	1.8E+02	1.5E+01	4.8E+01					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-B02-C	1	7.50E+00	U1/2		7.50E+00	2.1E+02	1.5E+01	4.8E+01					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1313-B03-C	1	7.50E+00	U1/2		7.50E+00	1.8E+02	1.5E+01	4.8E+01					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	CFS-L04-1313-T01-A	1	1.85E+02			1.85E+02	2.0E+00	1.1E+00	3.5E+00			---		VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T02-A	1	1.92E+02			1.92E+02	4.2E+00	1.1E+00	3.5E+00	1000	100	1.10E+03	91%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T03-A	1	4.69E+02			4.69E+02	6.5E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T04-A	1	6.42E+02			6.42E+02	5.4E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T05-A	1	3.90E+03			3.90E+03	8.9E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T06-A	1	3.74E+03			3.74E+03	1.2E+00	1.1E+00	3.5E+00			---		VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T07-A	1	2.12E+04			2.12E+04	6.9E+00	1.1E+00	3.5E+00			---		VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T08-A	1	6.02E+04			6.02E+04	3.5E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T09-A	1	1.48E+05			1.48E+05	1.4E+00	1.1E+00	3.5E+00			---		VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T01-B	1	2.53E+02			2.53E+02	6.0E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T02-B	1	2.89E+02			2.89E+02	1.5E+00	1.1E+00	3.5E+00	1000	100	1.26E+03	98%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T03-B	1	5.46E+02			5.46E+02	4.3E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T04-B	1	5.98E+02			5.98E+02	8.0E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T05-B	1	3.57E+03			3.57E+03	1.4E+00	1.1E+00	3.5E+00			---		VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T06-B	1	7.44E+03			7.44E+03	7.5E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T07-B	1	3.17E+04			3.17E+04	9.3E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T08-B	1	5.84E+04			5.84E+04	3.1E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T09-B	1	1.54E+05			1.54E+05	1.0E+00	1.1E+00	3.5E+00			---		VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T01-C	1	2.23E+02			2.23E+02	1.4E+00	1.1E+00	3.5E+00			---		VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T02-C	1	2.54E+02			2.54E+02	2.1E+00	1.1E+00	3.5E+00	1000	100	1.22E+03	97%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T03-C	1	4.67E+02			4.67E+02	1.4E+00	1.1E+00	3.5E+00			---		VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T04-C	1	5.53E+02			5.53E+02	5.9E-01	1.1E+00	3.5E+00					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T05-C	1	2.08E+03			2.08E+03	5.8E-01	1.1E+00	3.5E+00					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T06-C	1	5.76E+03			5.76E+03	8.2E-01	1.1E+00	3.5E+00					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T07-C	1	3.32E+04			3.32E+04	1.7E+00	1.1E+00	3.5E+00					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T08-C	1	1.29E+05			1.29E+05	3.8E-01	1.1E+00	3.5E+00					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-T09-C	1	1.55E+05			1.55E+05	8.8E-01	1.1E+00	3.5E+00					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-B01-A	1	7.88E+00			7.88E+00	2.6E+01	1.1E+00	3.5E+00					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-B02-A	1	1.29E+01			1.29E+01	1.5E+01	1.1E+00	3.5E+00					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-B03-A	1	2.86E+02			2.86E+02	3.1E+01	1.1E+00	3.5E+00					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-B01-B	1	4.92E+00			4.92E+00	4.1E+01	1.1E+00	3.5E+00					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-B02-B	1	3.46E+01			3.46E+01	8.7E+00	1.1E+00	3.5E+00					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-B03-B	1	1.15E+01			1.15E+01	2.7E+01	1.1E+00	3.5E+00					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-B01-C	1	4.24E+00			4.24E+00	4.6E+01	1.1E+00	3.5E+00					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-B02-C	1	6.31E+00			6.31E+00	2.9E+01	1.1E+00	3.5E+00					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1313-B03-C	1	2.02E+02			2.02E+02	1.7E+01	1.1E+00	3.5E+00					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	CFS-L04-1313-T01-A	1	2.13E+04			2.13E+04	5.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T02-A	1	2.10E+04			2.10E+04	2.3E-01	2.5E+00	8.0E+00	1000	100	2.19E+04	92%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T03-A	1	2.01E+04			2.01E+04	2.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T04-A	1	2.22E+04			2.22E+04	6.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T05-A	1	1.95E+04			1.95E+04	4.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T06-A	1	1.91E+04			1.91E+04	3.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T07-A	1	2.03E+04			2.03E+04	2.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T08-A	1	2.65E+04			2.65E+04	8.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T09-A	1	3.13E+04			3.13E+04	6.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T01-B	1	2.11E+04			2.11E+04	5.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T02-B	1	2.08E+04			2.08E+04	6.3E-01	2.5E+00	8.0E+00	1000	100	2.16E+04	85%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T03-B	1	2.11E+04			2.11E+04	1.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T04-B	1	2.06E+04			2.06E+04	5.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T05-B	1	1.97E+04			1.97E+04	6.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T06-B	1	1.99E+04			1.99E+04	8.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T07-B	1	2.30E+04			2.30E+04	7.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T08-B	1	2.76E+04			2.76E+04	6.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T09-B	1	3.36E+04			3.36E+04	8.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T01-C	1	1.90E+04			1.90E+04	1.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T02-C	1	2.10E+04			2.10E+04	5.9E-01	2.5E+00	8.0E+00	1000	100	2.19E+04	89%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T03-C	1	2.07E+04			2.07E+04	3.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T04-C	1	1.93E+04			1.93E+04	3.6E-01	2.5E+00	8.0E+00					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T05-C	1	2.08E+04			2.08E+04	6.4E-01	2.5E+00	8.0E+00					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T06-C	1	2.15E+04			2.15E+04	4.1E-01	2.5E+00	8.0E+00					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T07-C	1	2.29E+04			2.29E+04	3.8E-01	2.5E+00	8.0E+00					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T08-C	1	2.86E+04			2.86E+04	2.0E+00	2.5E+00	8.0E+00					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-T09-C	1	3.19E+04			3.19E+04	6.1E-01	2.5E+00	8.0E+00					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-B01-A	1	1.49E+01			1.49E+01	9.6E+00	2.5E+00	8.0E+00					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-B02-A	1	1.99E+01			1.99E+01	7.8E+00	2.5E+00	8.0E+00					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-B03-A	1	1.53E+03			1.53E+03	9.7E-01	2.5E+00	8.0E+00					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-B01-B	1	2.87E+01			2.87E+01	9.5E+00	2.5E+00	8.0E+00					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-B02-B	1	2.29E+01			2.29E+01	2.0E+01	2.5E+00	8.0E+00					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-B03-B	1	1.82E+02			1.82E+02	6.4E-01	2.5E+00	8.0E+00					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-B01-C	1	2.10E+01			2.10E+01	9.2E+00	2.5E+00	8.0E+00					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-B02-C	1	1.59E+01			1.59E+01	1.4E+01	2.5E+00	8.0E+00					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1313-B03-C	1	1.64E+03			1.64E+03	6.5E-01	2.5E+00	8.0E+00					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	CFS-L04-1313-T01-A	1	1.76E+03			1.76E+03	3.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T02-A	1	1.77E+03			1.77E+03	1.1E+00	1.0E+00	3.2E+00	1000	100	2.80E+03	103%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T03-A	1	4.16E+03			4.16E+03	5.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T04-A	1	3.57E+03			3.57E+03	2.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T05-A	1	1.60E+03			1.60E+03	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T06-A	1	1.63E+03			1.63E+03	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T07-A	1	9.44E+02			9.44E+02	7.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T08-A	1	1.11E+03			1.11E+03	1.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T09-A	1	1.60E+03			1.60E+03	3.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T01-B	1	1.73E+03			1.73E+03	8.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T02-B	1	3.51E+03			3.51E+03	1.1E+00	1.0E+00	3.2E+00	1000	100	4.45E+03	94%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T03-B	1	4.45E+03			4.45E+03	8.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T04-B	1	3.70E+03			3.70E+03	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T05-B	1	1.62E+03			1.62E+03	9.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T06-B	1	9.56E+02			9.56E+02	1.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T07-B	1	9.71E+02			9.71E+02	2.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T08-B	1	1.18E+03			1.18E+03	1.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T09-B	1	1.36E+03			1.36E+03	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T01-C	1	1.37E+03			1.37E+03	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T02-C	1	2.85E+03			2.85E+03	2.6E-01	1.0E+00	3.2E+00	1000	100	3.84E+03	99%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T03-C	1	3.69E+03			3.69E+03	4.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T04-C	1	3.37E+03			3.37E+03	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T05-C	1	2.63E+03			2.63E+03	8.3E-01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T06-C	1	1.28E+03			1.28E+03	7.8E-01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T07-C	1	1.05E+03			1.05E+03	9.0E-01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T08-C	1	1.70E+03			1.70E+03	2.5E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-T09-C	1	1.33E+03			1.33E+03	3.0E-01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.9E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.4E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	7.0E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	4.7E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	5.8E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	2.4E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	3.2E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	2.8E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	CFS-L04-1313-T01-A	1	1.35E+06			1.35E+06	5.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T02-A	1	1.39E+06			1.39E+06	5.3E-01	6.8E+00	2.2E+01	1000	100	1.39E+06	89%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T03-A	1	7.89E+05			7.89E+05	2.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T04-A	1	7.05E+05			7.05E+05	6.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T05-A	1	6.26E+05			6.26E+05	4.3E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T06-A	1	6.09E+05			6.09E+05	1.1E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T07-A	1	6.13E+05			6.13E+05	6.9E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T08-A	1	7.05E+05			7.05E+05	8.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T09-A	1	9.02E+05			9.02E+05	7.7E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T01-B	1	1.46E+06			1.46E+06	5.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T02-B	1	1.33E+06			1.33E+06	6.3E-01	6.8E+00	2.2E+01	1000	100	1.33E+06	94%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T03-B	1	8.65E+05			8.65E+05	3.9E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T04-B	1	7.20E+05			7.20E+05	7.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T05-B	1	6.10E+05			6.10E+05	4.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T06-B	1	6.01E+05			6.01E+05	6.7E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T07-B	1	6.57E+05			6.57E+05	4.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T08-B	1	6.94E+05			6.94E+05	7.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T09-B	1	8.23E+05			8.23E+05	1.2E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T01-C	1	1.26E+06			1.26E+06	3.3E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T02-C	1	1.21E+06			1.21E+06	4.0E-01	6.8E+00	2.2E+01	1000	100	1.21E+06	84%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T03-C	1	7.78E+05			7.78E+05	3.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T04-C	1	6.91E+05			6.91E+05	6.2E-01	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T05-C	1	6.35E+05			6.35E+05	6.5E-01	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T06-C	1	6.40E+05			6.40E+05	3.0E-01	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T07-C	1	6.76E+05			6.76E+05	6.5E-01	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T08-C	1	7.63E+05			7.63E+05	1.8E+00	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-T09-C	1	8.63E+05			8.63E+05	8.9E-01	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	3.0E+01	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	3.9E+01	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-B03-A	1	1.15E+02			1.15E+02	1.0E+01	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-B01-B	1	3.40E+00	U1/2		3.40E+00	6.5E+00	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-B02-B	1	3.40E+00	U1/2		3.40E+00	1.3E+01	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-B03-B	1	3.40E+00	U1/2		3.40E+00	3.7E+00	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-B01-C	1	3.40E+00	U1/2		3.40E+00	4.1E+00	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-B02-C	1	3.40E+00	U1/2		3.40E+00	5.2E+00	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1313-B03-C	1	1.26E+02			1.26E+02	2.2E+00	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

TI	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	CFS-L04-1313-T01-A	1	2.05E+02			2.05E+02	3.3E-01	4.6E+00	1.5E+01			---		VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T02-A	1	2.03E+02			2.03E+02	1.9E+00	4.6E+00	1.5E+01	10	100	1.19E+03	99%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T03-A	1	3.98E+02			3.98E+02	1.3E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T04-A	1	6.03E+02			6.03E+02	3.4E-01	4.6E+00	1.5E+01			---		VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T05-A	1	3.24E+02			3.24E+02	2.7E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T06-A	1	3.25E+02			3.25E+02	1.5E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T07-A	1	5.46E+02			5.46E+02	4.8E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T08-A	1	9.00E+02			9.00E+02	9.0E-01	4.6E+00	1.5E+01			---		VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T09-A	1	1.86E+03			1.86E+03	1.2E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T01-B	1	2.36E+02			2.36E+02	3.4E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T02-B	1	2.19E+02			2.19E+02	2.5E+00	4.6E+00	1.5E+01	10	100	1.15E+03	93%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T03-B	1	3.49E+02			3.49E+02	1.0E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T04-B	1	5.86E+02			5.86E+02	1.2E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T05-B	1	3.23E+02			3.23E+02	7.3E-01	4.6E+00	1.5E+01			---		VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T06-B	1	3.69E+02			3.69E+02	5.0E-01	4.6E+00	1.5E+01			---		VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T07-B	1	6.07E+02			6.07E+02	1.6E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T08-B	1	8.98E+02			8.98E+02	4.2E-01	4.6E+00	1.5E+01			---		VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T09-B	1	1.70E+03			1.70E+03	1.7E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T01-C	1	2.06E+02			2.06E+02	2.4E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T02-C	1	2.20E+02			2.20E+02	3.0E+00	4.6E+00	1.5E+01	10	100	1.17E+03	95%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T03-C	1	3.68E+02			3.68E+02	1.7E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T04-C	1	5.50E+02			5.50E+02	1.4E+00	4.6E+00	1.5E+01					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T05-C	1	6.87E+02			6.87E+02	2.2E+00	4.6E+00	1.5E+01					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T06-C	1	3.41E+02			3.41E+02	5.0E-01	4.6E+00	1.5E+01					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T07-C	1	6.35E+02			6.35E+02	8.1E-01	4.6E+00	1.5E+01					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T08-C	1	1.09E+03			1.09E+03	3.1E+00	4.6E+00	1.5E+01					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-T09-C	1	1.66E+03			1.66E+03	1.2E+00	4.6E+00	1.5E+01					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	1.3E+02	4.6E+00	1.5E+01					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	7.9E+02	4.6E+00	1.5E+01					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	6.1E+01	4.6E+00	1.5E+01					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-B01-B	1	2.30E+00	U1/2		2.30E+00	3.0E+01	4.6E+00	1.5E+01					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-B02-B	1	2.30E+00	U1/2		2.30E+00	7.1E+01	4.6E+00	1.5E+01					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-B03-B	1	2.30E+00	U1/2		2.30E+00	4.5E+02	4.6E+00	1.5E+01					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-B01-C	1	2.30E+00	U1/2		2.30E+00	7.5E+01	4.6E+00	1.5E+01					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-B02-C	1	2.30E+00	U1/2		2.30E+00	2.6E+02	4.6E+00	1.5E+01					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1313-B03-C	1	2.30E+00	U1/2		2.30E+00	6.5E+01	4.6E+00	1.5E+01					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	CFS-L04-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	4.9E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	7.2E+00	2.0E+00	6.4E+00	10	100	1.07E+03	107%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	4.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	6.9E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	2.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T08-A	1	7.21E+00			7.21E+00	2.5E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T09-A	1	6.50E+01			6.50E+01	3.1E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	4.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	9.4E+00	2.0E+00	6.4E+00	10	100	1.00E+03	100%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	9.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	1.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	3.5E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	8.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	1.8E+02	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T08-B	1	8.49E+00			8.49E+00	1.6E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T09-B	1	6.28E+01			6.28E+01	1.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	3.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	1.5E+00	2.0E+00	6.4E+00	10	100	1.01E+03	101%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	2.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	9.3E+00	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	6.8E+00	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	1.8E+00	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	5.9E+01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T08-C	1	9.75E+00			9.75E+00	2.0E+01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-T09-C	1	3.59E+01			3.59E+01	1.1E+00	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	3.4E+00	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	3.6E+00	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	2.6E+01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	3.9E+00	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	3.1E+00	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	5.0E+00	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	9.7E+00	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	2.3E+00	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1313-B03-C	1	1.00E+00	U1/2		1.00E+00	7.2E+01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	CFS-L04-1313-T01-A	1	2.90E+01			2.90E+01	3.7E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T02-A	1	3.19E+01			3.19E+01	6.2E-01	1.5E+00	4.8E+00	10	100	1.20E+03	117%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T03-A	1	3.07E+01			3.07E+01	2.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T04-A	1	3.20E+01			3.20E+01	6.9E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T05-A	1	3.51E+01			3.51E+01	3.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T06-A	1	3.37E+01			3.37E+01	4.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T07-A	1	4.01E+01			4.01E+01	1.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T08-A	1	5.83E+01			5.83E+01	9.9E-01	1.5E+00	4.8E+00			---		VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T09-A	1	5.77E+02			5.77E+02	6.1E-01	1.5E+00	4.8E+00			---		VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T01-B	1	2.73E+01			2.73E+01	1.2E+01	1.5E+00	4.8E+00			---		VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T02-B	1	3.51E+01			3.51E+01	4.3E-01	1.5E+00	4.8E+00	10	100	1.13E+03	110%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T03-B	1	3.37E+01			3.37E+01	2.9E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T04-B	1	3.12E+01			3.12E+01	2.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T05-B	1	3.42E+01			3.42E+01	2.3E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T06-B	1	3.57E+01			3.57E+01	2.5E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T07-B	1	4.51E+01			4.51E+01	2.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T08-B	1	5.54E+01			5.54E+01	1.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T09-B	1	5.09E+02			5.09E+02	1.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T01-C	1	2.51E+01			2.51E+01	5.6E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T02-C	1	2.99E+01			2.99E+01	3.9E+00	1.5E+00	4.8E+00	10	100	1.14E+03	111%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T03-C	1	2.92E+01			2.92E+01	3.0E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T04-C	1	3.12E+01			3.12E+01	2.7E+00	1.5E+00	4.8E+00					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T05-C	1	3.18E+01			3.18E+01	3.1E+00	1.5E+00	4.8E+00					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T06-C	1	3.53E+01			3.53E+01	3.7E+00	1.5E+00	4.8E+00					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T07-C	1	4.75E+01			4.75E+01	1.3E+00	1.5E+00	4.8E+00					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T08-C	1	2.62E+02			2.62E+02	4.2E+00	1.5E+00	4.8E+00					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-T09-C	1	5.21E+02			5.21E+02	1.0E+00	1.5E+00	4.8E+00					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-B01-A	1	7.50E-01	U1/2		7.50E-01	1.1E+02	1.5E+00	4.8E+00					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-B02-A	1	7.50E-01	U1/2		7.50E-01	8.3E+01	1.5E+00	4.8E+00					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-B03-A	1	7.50E-01	U1/2		7.50E-01	1.0E+02	1.5E+00	4.8E+00					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-B01-B	1	7.50E-01	U1/2		7.50E-01	2.2E+04	1.5E+00	4.8E+00					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-B02-B	1	7.50E-01	U1/2		7.50E-01	2.2E+02	1.5E+00	4.8E+00					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-B03-B	1	7.50E-01	U1/2		7.50E-01	1.3E+02	1.5E+00	4.8E+00					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-B01-C	1	7.50E-01	U1/2		7.50E-01	3.3E+02	1.5E+00	4.8E+00					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-B02-C	1	7.50E-01	U1/2		7.50E-01	1.6E+02	1.5E+00	4.8E+00					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1313-B03-C	1	7.50E-01	U1/2		7.50E-01	8.7E+01	1.5E+00	4.8E+00					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	CFS-L04-1313-T01-A	1	7.87E+03			7.87E+03	1.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 2:55 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T02-A	1	6.67E+03			6.67E+03	7.5E-01	1.0E+00	3.2E+00	10	100	7.60E+03	93%	VU ICP-OES	5/25/11 2:57 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T03-A	1	1.94E+01			1.94E+01	2.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 2:58 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T04-A	1	2.23E+01			2.23E+01	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:00 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T05-A	1	2.00E+04			2.00E+04	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:02 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T06-A	1	1.78E+04			1.78E+04	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:03 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T07-A	1	1.46E+05			1.46E+05	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:05 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T08-A	1	1.87E+05			1.87E+05	1.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:07 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T09-A	1	1.79E+05			1.79E+05	8.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:08 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T01-B	1	8.82E+03			8.82E+03	9.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:15 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T02-B	1	3.91E+03			3.91E+03	1.4E+00	1.0E+00	3.2E+00	10	100	4.90E+03	98%	VU ICP-OES	5/25/11 3:16 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T03-B	1	4.13E+01			4.13E+01	9.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:18 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T04-B	1	1.39E+01			1.39E+01	3.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:20 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T05-B	1	1.69E+04			1.69E+04	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:21 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T06-B	1	6.66E+04			6.66E+04	3.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:23 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T07-B	1	1.63E+05			1.63E+05	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:25 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T08-B	1	1.71E+05			1.71E+05	1.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:26 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T09-B	1	1.62E+05			1.62E+05	2.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:28 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T01-C	1	7.87E+03			7.87E+03	2.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:35 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T02-C	1	3.54E+03			3.54E+03	5.7E-01	1.0E+00	3.2E+00	10	100	4.64E+03	110%	VU ICP-OES	5/25/11 3:36 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T03-C	1	3.41E+01			3.41E+01	8.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/25/11 3:38 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T04-C	1	1.49E+01			1.49E+01	3.7E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:40 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T05-C	1	3.87E+03			3.87E+03	4.5E-01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:41 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T06-C	1	4.81E+04			4.81E+04	6.5E-01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:43 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T07-C	1	1.67E+05			1.67E+05	9.0E-01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:44 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T08-C	1	1.78E+05			1.78E+05	2.7E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:46 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-T09-C	1	1.70E+05			1.70E+05	2.0E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 3:48 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-B01-A	1	4.72E+00			4.72E+00	9.0E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:40 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-B02-A	1	5.92E+00			5.92E+00	2.9E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:42 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-B03-A	1	4.77E+00			4.77E+00	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:44 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-B01-B	1	7.33E+00			7.33E+00	2.1E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:45 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-B02-B	1	9.45E+01			9.45E+01	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:47 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-B03-B	1	2.37E+00	E		2.37E+00	7.2E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:48 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-B01-C	1	1.74E+00	E		1.74E+00	2.1E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:50 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-B02-C	1	4.43E+00			4.43E+00	6.5E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:52 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1313-B03-C	1	3.02E+00	E		3.02E+00	7.9E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 2:53 PM	EPA Interlab L04 1313-1316 CFS

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	CFS-L06-1313-T01-A	1	1.18E+02			1.18E+02	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T02-A	1	1.17E+02			1.17E+02	1.0E+00	1.0E+00	3.2E+00	1000	120	1.43E+03	110%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T03-A	1	1.34E+00	E		1.34E+00	4.1E+02	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T04-A	1	1.26E+02			1.26E+02	1.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T05-A	1	4.74E+01			4.74E+01	4.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T06-A	1	7.95E+00			7.95E+00	2.1E+02	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T07-A	1	9.38E+03			9.38E+03	8.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T08-A	1	2.30E+04			2.30E+04	4.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T09-A	1	8.68E+04			8.68E+04	2.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T01-B	1	1.17E+02			1.17E+02	1.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T02-B	1	5.88E+01			5.88E+01	9.9E+01	1.0E+00	3.2E+00	1000	120	1.47E+03	118%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T03-B	1	1.64E+02			1.64E+02	4.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T04-B	1	1.33E+02			1.33E+02	4.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T05-B	1	5.01E+01			5.01E+01	6.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T06-B	1	4.64E+01			4.64E+01	4.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T07-B	1	8.90E+03			8.90E+03	1.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T08-B	1	2.49E+04			2.49E+04	1.9E-02	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T09-B	1	8.37E+04			8.37E+04	6.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T01-C	1	1.28E+02			1.28E+02	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T02-C	1	1.11E+02			1.11E+02	3.2E+00	1.0E+00	3.2E+00	1000	120	1.44E+03	110%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T03-C	1	1.52E+02			1.52E+02	2.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T04-C	1	1.19E+02			1.19E+02	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T05-C	1	5.80E+01			5.80E+01	5.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T06-C	1	4.72E+01			4.72E+01	1.6E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T07-C	1	9.20E+03			9.20E+03	9.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T08-C	1	2.51E+04			2.51E+04	1.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-T09-C	1	8.54E+04			8.54E+04	1.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.5E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.7E+02	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-B03-A	1	8.41E+00			8.41E+00	2.4E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	1.4E+02	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-B02-B	1	2.31E+00	E		2.31E+00	1.3E+02	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	3.7E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	1.3E+02	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-B02-C	1	6.78E+00			6.78E+00	6.4E+00	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	1.7E+02	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	CFS-L06-1313-T01-A	1	1.03E+01	E		1.03E+01	1.2E+02	7.5E+00	2.4E+01			---		VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T02-A	1	1.08E+01	E		1.08E+01	1.1E+02	7.5E+00	2.4E+01	10	120	1.36E+03	112%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T03-A	1	3.75E+00	U1/2		3.75E+00	6.6E+02	7.5E+00	2.4E+01			---		VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T04-A	1	3.84E+01			3.84E+01	2.3E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T05-A	1	3.69E+01			3.69E+01	2.6E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T06-A	1	3.75E+00	U1/2		3.75E+00	1.8E+02	7.5E+00	2.4E+01			---		VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T07-A	1	3.03E+02			3.03E+02	1.2E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T08-A	1	7.44E+02			7.44E+02	7.7E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T09-A	1	1.56E+03			1.56E+03	6.0E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T01-B	1	8.57E+00	E		8.57E+00	8.9E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T02-B	1	7.77E+00	E		7.77E+00	5.8E+01	7.5E+00	2.4E+01	10	120	1.40E+03	116%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T03-B	1	3.36E+01			3.36E+01	2.3E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T04-B	1	4.87E+01			4.87E+01	9.7E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T05-B	1	2.15E+01	E		2.15E+01	1.6E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T06-B	1	4.58E+01			4.58E+01	2.5E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T07-B	1	2.85E+02			2.85E+02	1.8E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T08-B	1	8.56E+02			8.56E+02	7.3E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T09-B	1	1.65E+03			1.65E+03	6.6E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T01-C	1	3.75E+00	U1/2		3.75E+00	1.0E+02	7.5E+00	2.4E+01			---		VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T02-C	1	1.49E+01	E		1.49E+01	3.3E+01	7.5E+00	2.4E+01	10	150	1.67E+03	111%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T03-C	1	2.62E+01			2.62E+01	1.9E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T04-C	1	4.11E+01			4.11E+01	3.8E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T05-C	1	3.42E+01			3.42E+01	1.3E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T06-C	1	3.38E+01			3.38E+01	5.5E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T07-C	1	3.02E+02			3.02E+02	8.2E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T08-C	1	8.03E+02			8.03E+02	5.7E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-T09-C	1	1.55E+03			1.55E+03	3.8E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-B01-A	1	3.75E+00	U1/2		3.75E+00	1.0E+02	7.5E+00	2.4E+01					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-B02-A	1	3.75E+00	U1/2		3.75E+00	6.9E+01	7.5E+00	2.4E+01					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-B03-A	1	1.85E+01	E		1.85E+01	6.0E+01	7.5E+00	2.4E+01					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-B01-B	1	3.75E+00	U1/2		3.75E+00	9.1E+01	7.5E+00	2.4E+01					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-B02-B	1	3.75E+00	U1/2		3.75E+00	3.4E+01	7.5E+00	2.4E+01					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-B03-B	1	3.75E+00	U1/2		3.75E+00	5.4E+01	7.5E+00	2.4E+01					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-B01-C	1	3.75E+00	U1/2		3.75E+00	6.2E+01	7.5E+00	2.4E+01					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-B02-C	1	3.75E+00	U1/2		3.75E+00	1.8E+01	7.5E+00	2.4E+01					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1313-B03-C	1	8.02E+00	E		8.02E+00	3.0E+01	7.5E+00	2.4E+01					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	CFS-L06-1313-T01-A	1	4.21E+02			4.21E+02	2.0E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T02-A	1	3.82E+02			3.82E+02	3.9E+00	1.1E+01	3.5E+01	10	120	1.73E+03	112%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T03-A	1	5.50E+00	U1/2		5.50E+00	3.1E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T04-A	1	5.47E+01			5.47E+01	4.9E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T05-A	1	2.62E+01	E		2.62E+01	8.5E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T06-A	1	5.50E+00	U1/2		5.50E+00	3.6E+02	1.1E+01	3.5E+01			---		VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T07-A	1	2.92E+02			2.92E+02	4.5E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T08-A	1	6.22E+02			6.22E+02	4.3E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T09-A	1	5.55E+04			5.55E+04	1.1E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T01-B	1	5.73E+02			5.73E+02	1.8E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T02-B	1	1.57E+02			1.57E+02	1.0E+02	1.1E+01	3.5E+01	10	120	1.50E+03	112%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T03-B	1	1.34E+02			1.34E+02	3.3E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T04-B	1	4.94E+01			4.94E+01	2.2E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T05-B	1	2.65E+01	E		2.65E+01	2.5E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T06-B	1	1.91E+01	E		1.91E+01	2.6E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T07-B	1	3.08E+02			3.08E+02	2.8E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T08-B	1	7.56E+02			7.56E+02	1.0E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T09-B	1	7.59E+04			7.59E+04	4.0E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T01-C	1	4.56E+02			4.56E+02	3.4E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T02-C	1	3.01E+02			3.01E+02	3.2E+00	1.1E+01	3.5E+01	10	150	1.98E+03	112%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T03-C	1	1.40E+02			1.40E+02	7.4E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T04-C	1	4.87E+01			4.87E+01	2.5E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T05-C	1	2.90E+01	E		2.90E+01	3.0E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T06-C	1	2.28E+01	E		2.28E+01	6.2E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T07-C	1	3.01E+02			3.01E+02	1.6E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T08-C	1	8.07E+02			8.07E+02	1.2E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-T09-C	1	7.34E+04			7.34E+04	1.2E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-B01-A	1	5.50E+00	U1/2		5.50E+00	9.1E+01	1.1E+01	3.5E+01					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-B02-A	1	5.50E+00	U1/2		5.50E+00	7.8E+01	1.1E+01	3.5E+01					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-B03-A	1	1.45E+01	E		1.45E+01	2.3E+01	1.1E+01	3.5E+01					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-B01-B	1	5.50E+00	U1/2		5.50E+00	1.2E+03	1.1E+01	3.5E+01					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-B02-B	1	5.50E+00	U1/2		5.50E+00	1.5E+02	1.1E+01	3.5E+01					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-B03-B	1	5.50E+00	U1/2		5.50E+00	1.4E+01	1.1E+01	3.5E+01					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-B01-C	1	5.50E+00	U1/2		5.50E+00	8.8E+01	1.1E+01	3.5E+01					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-B02-C	1	5.50E+00	U1/2		5.50E+00	7.8E+02	1.1E+01	3.5E+01					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1313-B03-C	1	5.50E+00	U1/2		5.50E+00	9.0E+01	1.1E+01	3.5E+01					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	CFS-L06-1313-T01-A	1	8.30E+01			8.30E+01	4.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T02-A	1	7.31E+01			7.31E+01	1.1E+00	1.0E+00	3.2E+00	1000	120	1.40E+03	110%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T03-A	1	6.71E+00			6.71E+00	6.5E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T04-A	1	1.31E+02			1.31E+02	8.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T05-A	1	1.51E+02			1.51E+02	1.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T06-A	1	2.36E+01			2.36E+01	1.3E+02	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T07-A	1	4.66E+02			4.66E+02	7.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T08-A	1	6.68E+02			6.68E+02	5.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T09-A	1	9.03E+02			9.03E+02	2.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T01-B	1	8.43E+01			8.43E+01	1.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T02-B	1	3.68E+01			3.68E+01	9.2E+01	1.0E+00	3.2E+00	1000	120	1.45E+03	118%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T03-B	1	1.82E+02			1.82E+02	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T04-B	1	1.32E+02			1.32E+02	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T05-B	1	1.44E+02			1.44E+02	2.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T06-B	1	1.75E+02			1.75E+02	4.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T07-B	1	4.41E+02			4.41E+02	8.6E-02	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T08-B	1	6.55E+02			6.55E+02	6.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T09-B	1	8.14E+02			8.14E+02	6.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T01-C	1	9.04E+01			9.04E+01	1.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T02-C	1	7.21E+01			7.21E+01	9.0E-01	1.0E+00	3.2E+00	1000	120	1.30E+03	102%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T03-C	1	1.83E+02			1.83E+02	1.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T04-C	1	1.30E+02			1.30E+02	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T05-C	1	1.47E+02			1.47E+02	2.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T06-C	1	1.47E+02			1.47E+02	3.2E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T07-C	1	4.63E+02			4.63E+02	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T08-C	1	6.49E+02			6.49E+02	6.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-T09-C	1	7.68E+02			7.68E+02	6.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-B01-A	1	3.71E+00			3.71E+00	3.9E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-B02-A	1	5.00E+00			5.00E+00	5.0E+00	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-B03-A	1	1.15E+01			1.15E+01	5.4E+00	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-B01-B	1	3.81E+00			3.81E+00	4.0E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-B02-B	1	4.63E+00			4.63E+00	2.6E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-B03-B	1	1.21E+01			1.21E+01	1.6E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-B01-C	1	4.96E+00			4.96E+00	9.0E+00	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-B02-C	1	5.11E+00			5.11E+00	5.9E+00	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1313-B03-C	1	1.04E+01			1.04E+01	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	CFS-L06-1313-T01-A	1	5.00E-01	U1/2		5.00E-01	1.1E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T02-A	1	6.91E+00			6.91E+00	3.8E+00	1.0E+00	3.2E+00	10	120	1.04E+03	86%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T03-A	1	4.08E+00			4.08E+00	9.3E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T04-A	1	9.00E+01			9.00E+01	7.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T05-A	1	8.36E+01			8.36E+01	6.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T06-A	1	9.55E+00			9.55E+00	1.5E+02	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T07-A	1	3.62E+01			3.62E+01	9.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T08-A	1	3.89E+01			3.89E+01	4.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T09-A	1	1.07E+01			1.07E+01	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T01-B	1	5.00E-01	U1/2		5.00E-01	6.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T02-B	1	1.63E+00	E		1.63E+00	9.1E+01	1.0E+00	3.2E+00	10	120	1.03E+03	85%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T03-B	1	2.56E+02			2.56E+02	8.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T04-B	1	8.86E+01			8.86E+01	4.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T05-B	1	8.38E+01			8.38E+01	6.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T06-B	1	1.32E+02			1.32E+02	8.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T07-B	1	3.13E+01			3.13E+01	2.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T08-B	1	3.77E+01			3.77E+01	2.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T09-B	1	8.14E+00			8.14E+00	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T01-C	1	5.00E-01	U1/2		5.00E-01	2.3E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T02-C	1	5.43E+00			5.43E+00	8.7E+00	1.0E+00	3.2E+00	10	150	1.42E+03	94%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T03-C	1	2.48E+02			2.48E+02	5.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T04-C	1	9.11E+01			9.11E+01	3.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T05-C	1	8.48E+01			8.48E+01	8.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T06-C	1	1.08E+02			1.08E+02	4.1E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T07-C	1	3.66E+01			3.66E+01	4.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T08-C	1	3.61E+01			3.61E+01	5.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-T09-C	1	7.31E+00			7.31E+00	7.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	2.6E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	8.7E+00	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-B03-A	1	7.98E+00			7.98E+00	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	2.0E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	9.3E+00	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-B03-B	1	8.34E+00			8.34E+00	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	1.6E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	4.1E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1313-B03-C	1	8.41E+00			8.41E+00	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	CFS-L06-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	1.6E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	1.0E+03	1.9E+00	6.0E+00	10	120	1.37E+03	114%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	8.6E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	1.7E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	6.7E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	2.9E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T07-A	1	4.39E+00	E		4.39E+00	1.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T08-A	1	7.01E+00			7.01E+00	8.6E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T09-A	1	9.50E-01	U1/2		9.50E-01	9.6E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	2.5E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00	10	120	1.35E+03	112%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	6.1E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	1.2E+03	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	1.6E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	8.2E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T07-B	1	4.24E+00	E		4.24E+00	3.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T08-B	1	6.43E+00			6.43E+00	6.9E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T09-B	1	9.50E-01	U1/2		9.50E-01	8.7E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	2.0E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	1.0E+03	1.9E+00	6.0E+00	10	150	1.70E+03	113%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	6.4E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	4.5E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	6.8E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	6.3E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T07-C	1	4.47E+00	E		4.47E+00	1.1E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T08-C	1	7.28E+00			7.28E+00	7.8E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-T09-C	1	9.50E-01	U1/2		9.50E-01	1.1E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	1.3E+03	1.9E+00	6.0E+00					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	8.5E+02	1.9E+00	6.0E+00					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	9.4E+01	1.9E+00	6.0E+00					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-B01-B	1	9.50E-01	U1/2		9.50E-01	9.0E+02	1.9E+00	6.0E+00					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-B02-B	1	9.50E-01	U1/2		9.50E-01	1.7E+01	1.9E+00	6.0E+00					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-B03-B	1	9.50E-01	U1/2		9.50E-01	8.7E+02	1.9E+00	6.0E+00					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-B01-C	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-B02-C	1	9.50E-01	U1/2		9.50E-01	3.9E+02	1.9E+00	6.0E+00					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1313-B03-C	1	9.50E-01	U1/2		9.50E-01	5.7E+01	1.9E+00	6.0E+00					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	CFS-L06-1313-T01-A	1	1.67E+01			1.67E+01	3.2E+00	2.2E+00	7.0E+00			---		VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T02-A	1	5.91E+00	E		5.91E+00	2.9E+00	2.2E+00	7.0E+00	10	120	1.28E+03	107%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	1.2E+02	2.2E+00	7.0E+00			---		VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T04-A	1	4.79E+01			4.79E+01	4.6E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T05-A	1	3.70E+02			3.70E+02	5.6E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T06-A	1	4.67E+02			4.67E+02	1.6E+02	2.2E+00	7.0E+00			---		VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T07-A	1	3.61E+04			3.61E+04	7.3E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T08-A	1	4.95E+04			4.95E+04	5.6E+00	2.2E+00	7.0E+00			---		VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T09-A	1	5.02E+04			5.02E+04	3.2E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T01-B	1	1.76E+01			1.76E+01	1.3E+00	2.2E+00	7.0E+00			---		VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T02-B	1	2.63E+00	E		2.63E+00	1.1E+02	2.2E+00	7.0E+00	10	120	1.35E+03	113%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	2.3E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T04-B	1	5.82E+01			5.82E+01	3.0E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T05-B	1	5.14E+02			5.14E+02	5.9E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T06-B	1	4.82E+03			4.82E+03	4.2E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T07-B	1	3.38E+04			3.38E+04	9.5E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T08-B	1	4.85E+04			4.85E+04	1.2E+00	2.2E+00	7.0E+00			---		VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T09-B	1	5.11E+04			5.11E+04	8.1E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T01-C	1	1.77E+01			1.77E+01	2.0E+00	2.2E+00	7.0E+00			---		VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T02-C	1	6.38E+00	E		6.38E+00	2.1E+00	2.2E+00	7.0E+00	10	150	1.61E+03	107%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	2.8E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T04-C	1	4.15E+01			4.15E+01	4.9E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T05-C	1	4.13E+02			4.13E+02	5.1E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T06-C	1	4.08E+03			4.08E+03	3.3E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T07-C	1	3.62E+04			3.62E+04	4.2E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T08-C	1	4.88E+04			4.88E+04	1.6E+00	2.2E+00	7.0E+00			---		VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-T09-C	1	4.97E+04			4.97E+04	5.7E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	5.1E+01	2.2E+00	7.0E+00					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	6.8E+01	2.2E+00	7.0E+00					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-B03-A	1	1.10E+00	U1/2		1.10E+00	2.2E+01	2.2E+00	7.0E+00					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-B01-B	1	1.10E+00	U1/2		1.10E+00	2.2E+02	2.2E+00	7.0E+00					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-B02-B	1	1.10E+00	U1/2		1.10E+00	2.1E+02	2.2E+00	7.0E+00					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-B03-B	1	1.10E+00	U1/2		1.10E+00	3.1E+01	2.2E+00	7.0E+00					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-B01-C	1	1.10E+00	U1/2		1.10E+00	2.5E+02	2.2E+00	7.0E+00					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-B02-C	1	1.10E+00	U1/2		1.10E+00	6.8E+02	2.2E+00	7.0E+00					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1313-B03-C	1	1.10E+00	U1/2		1.10E+00	4.3E+01	2.2E+00	7.0E+00					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	CFS-L06-1313-T01-A	1	5.31E+05			5.31E+05	3.9E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T02-A	1	6.73E+05			6.73E+05	6.7E-01	2.6E+00	8.3E+00	1000	120	6.74E+05	82%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T03-A	1	1.14E+04			1.14E+04	1.3E+02	2.6E+00	8.3E+00			---		VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T04-A	1	6.81E+05			6.81E+05	5.0E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T05-A	1	7.14E+05			7.14E+05	4.6E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T06-A	1	9.72E+04			9.72E+04	1.7E+02	2.6E+00	8.3E+00			---		VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T07-A	1	1.08E+06			1.08E+06	9.7E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T08-A	1	1.27E+06			1.27E+06	5.2E+00	2.6E+00	8.3E+00			---		VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T09-A	1	1.62E+06			1.62E+06	7.9E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T01-B	1	4.39E+05			4.39E+05	3.7E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T02-B	1	3.37E+05			3.37E+05	9.8E+01	2.6E+00	8.3E+00	1000	120	3.38E+05	88%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T03-B	1	6.39E+05			6.39E+05	9.4E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T04-B	1	6.69E+05			6.69E+05	1.5E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T05-B	1	6.97E+05			6.97E+05	7.3E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T06-B	1	7.24E+05			7.24E+05	4.5E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T07-B	1	1.01E+06			1.01E+06	5.3E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T08-B	1	1.25E+06			1.25E+06	1.5E+00	2.6E+00	8.3E+00			---		VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T09-B	1	1.61E+06			1.61E+06	7.8E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T01-C	1	4.74E+05			4.74E+05	7.8E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T02-C	1	6.73E+05			6.73E+05	3.4E-01	2.6E+00	8.3E+00	1000	120	6.74E+05	86%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T03-C	1	6.47E+05			6.47E+05	2.6E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T04-C	1	6.70E+05			6.70E+05	4.1E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T05-C	1	7.02E+05			7.02E+05	8.4E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T06-C	1	6.61E+05			6.61E+05	2.5E+01	2.6E+00	8.3E+00			---		VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T07-C	1	1.10E+06			1.10E+06	8.8E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T08-C	1	1.29E+06			1.29E+06	2.1E+00	2.6E+00	8.3E+00			---		VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-T09-C	1	1.60E+06			1.60E+06	6.4E-01	2.6E+00	8.3E+00			---		VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-B01-A	1	7.75E+00	E		7.75E+00	6.7E+01	2.6E+00	8.3E+00					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-B02-A	1	1.78E+01			1.78E+01	2.2E+01	2.6E+00	8.3E+00					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-B03-A	1	2.83E+03			2.83E+03	1.8E+00	2.6E+00	8.3E+00					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-B01-B	1	1.82E+01			1.82E+01	1.7E+01	2.6E+00	8.3E+00					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-B02-B	1	2.21E+01			2.21E+01	1.5E+01	2.6E+00	8.3E+00					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-B03-B	1	2.92E+03			2.92E+03	6.3E-01	2.6E+00	8.3E+00					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-B01-C	1	2.21E+01			2.21E+01	2.6E+01	2.6E+00	8.3E+00					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-B02-C	1	2.17E+01			2.17E+01	1.1E+01	2.6E+00	8.3E+00					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1313-B03-C	1	2.99E+03			2.99E+03	4.0E-01	2.6E+00	8.3E+00					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	CFS-L06-1313-T01-A	1	1.42E+02			1.42E+02		1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T02-A	1	1.27E+02			1.27E+02		1.2E+00	3.8E+00	10	120	1.36E+03	102%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T03-A	1	6.00E-01	U1/2		6.00E-01		1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T04-A	1	1.69E+00	E		1.69E+00		1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T05-A	1	6.00E-01	U1/2		6.00E-01		1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T06-A	1	6.00E-01	U1/2		6.00E-01		1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T07-A	1	6.00E-01	U1/2		6.00E-01		1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T08-A	1	1.50E+01			1.50E+01		1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T09-A	1	2.34E+03			2.34E+03		1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T01-B	1	1.65E+02			1.65E+02		1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T02-B	1	5.14E+01			5.14E+01		1.2E+00	3.8E+00	10	120	1.41E+03	113%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T03-B	1	1.20E+01			1.20E+01		1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T04-B	1	1.78E+00	E		1.78E+00		1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T05-B	1	6.00E-01	U1/2		6.00E-01		1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T06-B	1	6.00E-01	U1/2		6.00E-01		1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T07-B	1	6.00E-01	U1/2		6.00E-01		1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T08-B	1	2.49E+01			2.49E+01		1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T09-B	1	2.11E+03			2.11E+03		1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T01-C	1	1.52E+02			1.52E+02		1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T02-C	1	9.76E+01			9.76E+01		1.2E+00	3.8E+00	10	150	1.63E+03	102%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T03-C	1	9.81E+00			9.81E+00		1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T04-C	1	2.36E+00	E		2.36E+00		1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T05-C	1	6.00E-01	U1/2		6.00E-01		1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T06-C	1	6.00E-01	U1/2		6.00E-01		1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T07-C	1	6.00E-01	U1/2		6.00E-01		1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T08-C	1	2.36E+01			2.36E+01		1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-T09-C	1	1.97E+03			1.97E+03		1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-B01-A	1	6.00E-01	U1/2		6.00E-01		1.2E+00	3.8E+00					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-B02-A	1	6.00E-01	U1/2		6.00E-01		1.2E+00	3.8E+00					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-B03-A	1	6.00E-01	U1/2		6.00E-01		1.2E+00	3.8E+00					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-B01-B	1	6.00E-01	U1/2		6.00E-01		1.2E+00	3.8E+00					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-B02-B	1	6.00E-01	U1/2		6.00E-01		1.2E+00	3.8E+00					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-B03-B	1	6.00E-01	U1/2		6.00E-01		1.2E+00	3.8E+00					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-B01-C	1	6.00E-01	U1/2		6.00E-01		1.2E+00	3.8E+00					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-B02-C	1	6.00E-01	U1/2		6.00E-01		1.2E+00	3.8E+00					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1313-B03-C	1	6.00E-01	U1/2		6.00E-01		1.2E+00	3.8E+00					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	CFS-L06-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	2.6E+02	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	6.4E+01	1.8E+00	5.7E+00	10	120	1.22E+03	102%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	2.1E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	5.6E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T05-A	1	6.20E+00			6.20E+00	1.2E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T06-A	1	1.12E+01			1.12E+01	1.8E+02	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T07-A	1	1.05E+03			1.05E+03	1.0E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T08-A	1	1.81E+03			1.81E+03	2.1E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T09-A	1	1.84E+03			1.84E+03	4.8E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	2.0E+02	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	4.5E+02	1.8E+00	5.7E+00	10	120	1.29E+03	107%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	3.3E+02	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	4.0E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T05-B	1	9.45E+00			9.45E+00	1.5E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T06-B	1	1.03E+02			1.03E+02	1.6E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T07-B	1	9.78E+02			9.78E+02	6.2E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T08-B	1	1.63E+03			1.63E+03	6.3E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T09-B	1	1.81E+03			1.81E+03	1.7E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00	10	150	1.52E+03	101%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	3.7E+02	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	7.3E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T05-C	1	7.29E+00			7.29E+00	8.7E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T06-C	1	8.74E+01			8.74E+01	2.9E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T07-C	1	1.05E+03			1.05E+03	2.4E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T08-C	1	1.69E+03			1.69E+03	6.9E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-T09-C	1	1.79E+03			1.79E+03	1.8E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	1.3E+03	1.8E+00	5.7E+00					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	3.6E+02	1.8E+00	5.7E+00					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	1.9E+01	1.8E+00	5.7E+00					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-B01-B	1	9.00E-01	U1/2		9.00E-01	5.1E+02	1.8E+00	5.7E+00					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-B02-B	1	9.00E-01	U1/2		9.00E-01	2.6E+01	1.8E+00	5.7E+00					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-B03-B	1	9.00E-01	U1/2		9.00E-01	1.2E+02	1.8E+00	5.7E+00					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-B01-C	1	9.00E-01	U1/2		9.00E-01	2.1E+03	1.8E+00	5.7E+00					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-B02-C	1	9.00E-01	U1/2		9.00E-01	1.8E+03	1.8E+00	5.7E+00					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1313-B03-C	1	9.00E-01	U1/2		9.00E-01	5.6E+01	1.8E+00	5.7E+00					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	CFS-L06-1313-T01-A	1	1.11E+04			1.11E+04	2.6E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T02-A	1	2.23E+03			2.23E+03	7.6E-01	3.7E+00	1.2E+01	10	120	3.25E+03	85%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T03-A	1	1.85E+00	U1/2		1.85E+00	1.3E+02	3.7E+00	1.2E+01			---		VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T04-A	1	1.06E+03			1.06E+03	7.5E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T05-A	1	1.26E+02			1.26E+02	2.0E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T06-A	1	1.92E+02			1.92E+02	1.7E+02	3.7E+00	1.2E+01			---		VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T07-A	1	4.98E+05			4.98E+05	1.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T08-A	1	8.68E+05			8.68E+05	4.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T09-A	1	1.08E+06			1.08E+06	1.6E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T01-B	1	1.03E+04			1.03E+04	1.2E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T02-B	1	1.26E+03			1.26E+03	8.9E+01	3.7E+00	1.2E+01	10	120	2.38E+03	94%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T03-B	1	2.04E+02			2.04E+02	2.0E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T04-B	1	1.23E+03			1.23E+03	1.7E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T05-B	1	1.65E+02			1.65E+02	9.0E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T06-B	1	8.12E+02			8.12E+02	1.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T07-B	1	4.79E+05			4.79E+05	6.7E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T08-B	1	8.82E+05			8.82E+05	4.2E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T09-B	1	1.08E+06			1.08E+06	1.3E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T01-C	1	1.04E+04			1.04E+04	1.1E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T02-C	1	2.29E+03			2.29E+03	1.3E+00	3.7E+00	1.2E+01	10	150	3.58E+03	86%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T03-C	1	1.96E+02			1.96E+02	1.8E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T04-C	1	9.39E+02			9.39E+02	2.1E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T05-C	1	7.43E+02			7.43E+02	1.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T06-C	1	7.85E+02			7.85E+02	1.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T07-C	1	4.98E+05			4.98E+05	7.5E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T08-C	1	8.97E+05			8.97E+05	1.1E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-T09-C	1	1.05E+06			1.05E+06	4.5E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	6.9E+01	3.7E+00	1.2E+01					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	1.5E+03	3.7E+00	1.2E+01					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-B03-A	1	1.85E+00	U1/2		1.85E+00	4.7E+01	3.7E+00	1.2E+01					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-B01-B	1	1.85E+00	U1/2		1.85E+00	1.0E+02	3.7E+00	1.2E+01					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-B02-B	1	1.85E+00	U1/2		1.85E+00	4.7E+02	3.7E+00	1.2E+01					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-B03-B	1	1.85E+00	U1/2		1.85E+00	7.8E+01	3.7E+00	1.2E+01					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-B01-C	1	1.85E+00	U1/2		1.85E+00	1.8E+02	3.7E+00	1.2E+01					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-B02-C	1	1.85E+00	U1/2		1.85E+00	1.0E+02	3.7E+00	1.2E+01					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1313-B03-C	1	1.85E+00	U1/2		1.85E+00	9.3E+01	3.7E+00	1.2E+01					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	CFS-L06-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	5.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T02-A	1	3.31E+00	E		3.31E+00	2.0E+01	2.0E+00	6.4E+00	1000	120	1.28E+03	106%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	5.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T04-A	1	2.87E+00	E		2.87E+00	6.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T05-A	1	2.38E+00	E		2.38E+00	1.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T07-A	1	4.82E+01			4.82E+01	1.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T08-A	1	6.12E+03			6.12E+03	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T09-A	1	2.39E+05			2.39E+05	6.0E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	1.0E+02	2.0E+00	6.4E+00	1000	120	1.35E+03	112%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T03-B	1	2.91E+00	E		2.91E+00	1.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T04-B	1	3.98E+00	E		3.98E+00	8.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T05-B	1	2.93E+00	E		2.93E+00	5.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	4.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T07-B	1	3.48E+01			3.48E+01	1.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T08-B	1	1.49E+04			1.49E+04	7.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T09-B	1	2.60E+05			2.60E+05	6.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T01-C	1	5.94E+00	E		5.94E+00	8.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T02-C	1	2.12E+00	E		2.12E+00	5.1E+00	2.0E+00	6.4E+00	1000	120	1.39E+03	115%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T03-C	1	2.01E+00	E		2.01E+00	2.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T04-C	1	3.37E+00	E		3.37E+00	1.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T05-C	1	2.62E+00	E		2.62E+00	2.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	4.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T07-C	1	3.77E+01			3.77E+01	1.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T08-C	1	1.46E+04			1.46E+04	1.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-T09-C	1	2.59E+05			2.59E+05	1.9E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	5.5E+01	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-B02-A	1	2.25E+00	E		2.25E+00	1.4E+01	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-B03-A	1	2.72E+00	E		2.72E+00	1.2E+01	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	2.6E+01	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-B02-B	1	2.78E+00	E		2.78E+00	1.3E+01	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	5.3E+01	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	3.7E+01	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	5.4E+00	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1313-B03-C	1	1.00E+00	U1/2		1.00E+00	2.8E+01	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	CFS-L06-1313-T01-A	1	4.64E+03			4.64E+03	1.7E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T02-A	1	7.45E+03			7.45E+03	1.6E+00	6.8E+00	2.2E+01	10	120	8.60E+03	95%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T03-A	1	3.40E+00	U1/2		3.40E+00	3.1E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T04-A	1	1.03E+02			1.03E+02	6.7E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T05-A	1	1.76E+02			1.76E+02	4.3E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T06-A	1	4.29E+01			4.29E+01	5.3E+02	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T07-A	1	6.93E+03			6.93E+03	1.4E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T08-A	1	5.71E+03			5.71E+03	7.5E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T09-A	1	8.88E+03			8.88E+03	3.3E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T01-B	1	4.81E+03			4.81E+03	1.3E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T02-B	1	3.83E+03			3.83E+03	9.2E+01	6.8E+00	2.2E+01	10	120	4.94E+03	92%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T03-B	1	1.27E+03			1.27E+03	1.0E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T04-B	1	1.01E+02			1.01E+02	1.7E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T05-B	1	2.21E+02			2.21E+02	3.8E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T06-B	1	1.12E+03			1.12E+03	1.4E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T07-B	1	6.65E+03			6.65E+03	1.4E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T08-B	1	5.61E+03			5.61E+03	3.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T09-B	1	8.64E+03			8.64E+03	2.3E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T01-C	1	4.33E+03			4.33E+03	1.5E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T02-C	1	7.24E+03			7.24E+03	1.0E+00	6.8E+00	2.2E+01	10	150	8.57E+03	89%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T03-C	1	1.32E+03			1.32E+03	1.8E-02	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T04-C	1	9.85E+01			9.85E+01	3.2E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T05-C	1	2.92E+02			2.92E+02	1.4E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T06-C	1	9.51E+02			9.51E+02	3.4E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T07-C	1	6.76E+03			6.76E+03	1.4E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T08-C	1	6.12E+03			6.12E+03	8.3E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-T09-C	1	8.41E+03			8.41E+03	3.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	1.9E+00	6.8E+00	2.2E+01					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	2.2E+00	6.8E+00	2.2E+01					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	7.3E+00	6.8E+00	2.2E+01					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-B01-B	1	3.40E+00	U1/2		3.40E+00	3.4E+00	6.8E+00	2.2E+01					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-B02-B	1	3.40E+00	U1/2		3.40E+00	1.4E+00	6.8E+00	2.2E+01					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-B03-B	1	3.40E+00	U1/2		3.40E+00	5.8E+00	6.8E+00	2.2E+01					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-B01-C	1	3.40E+00	U1/2		3.40E+00	4.0E+00	6.8E+00	2.2E+01					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-B02-C	1	3.40E+00	U1/2		3.40E+00	1.6E+00	6.8E+00	2.2E+01					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1313-B03-C	1	3.40E+00	U1/2		3.40E+00	2.8E+00	6.8E+00	2.2E+01					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	CFS-L06-1313-T01-A	1	4.04E+01			4.04E+01	4.0E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T02-A	1	4.20E+01			4.20E+01	1.4E+00	1.9E+00	6.0E+00	10	120	1.14E+03	92%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T03-A	1	2.99E+01			2.99E+01	1.3E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T04-A	1	4.23E+01			4.23E+01	3.5E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T05-A	1	4.03E+01			4.03E+01	3.6E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T06-A	1	3.33E+01			3.33E+01	3.5E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T07-A	1	3.77E+01			3.77E+01	1.2E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T08-A	1	4.57E+01			4.57E+01	9.2E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T09-A	1	9.09E+01			9.09E+01	2.1E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T01-B	1	4.12E+01			4.12E+01	2.3E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T02-B	1	3.56E+01			3.56E+01	8.9E+00	1.9E+00	6.0E+00	10	120	1.12E+03	90%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T03-B	1	4.03E+01			4.03E+01	2.5E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T04-B	1	3.97E+01			3.97E+01	7.5E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T05-B	1	3.88E+01			3.88E+01	5.3E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T06-B	1	4.02E+01			4.02E+01	7.0E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T07-B	1	3.60E+01			3.60E+01	4.2E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T08-B	1	4.14E+01			4.14E+01	4.9E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T09-B	1	6.98E+01			6.98E+01	9.7E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T01-C	1	4.18E+01			4.18E+01	1.5E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T02-C	1	4.27E+01			4.27E+01	2.5E+00	1.9E+00	6.0E+00	10	150	1.35E+03	87%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T03-C	1	3.97E+01			3.97E+01	3.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T04-C	1	4.13E+01			4.13E+01	1.7E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T05-C	1	4.00E+01			4.00E+01	1.2E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T06-C	1	3.90E+01			3.90E+01	5.7E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T07-C	1	4.08E+01			4.08E+01	4.9E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T08-C	1	4.46E+01			4.46E+01	8.1E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-T09-C	1	6.91E+01			6.91E+01	4.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-B01-A	1	2.83E+01			2.83E+01	1.1E+00	1.9E+00	6.0E+00					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-B02-A	1	2.82E+01			2.82E+01	2.6E+00	1.9E+00	6.0E+00					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-B03-A	1	2.89E+01			2.89E+01	1.7E+00	1.9E+00	6.0E+00					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-B01-B	1	2.87E+01			2.87E+01	3.5E+00	1.9E+00	6.0E+00					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-B02-B	1	2.82E+01			2.82E+01	1.1E-01	1.9E+00	6.0E+00					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-B03-B	1	2.85E+01			2.85E+01	4.4E+00	1.9E+00	6.0E+00					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-B01-C	1	2.76E+01			2.76E+01	3.6E+00	1.9E+00	6.0E+00					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-B02-C	1	2.95E+01			2.95E+01	4.6E+00	1.9E+00	6.0E+00					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1313-B03-C	1	2.96E+01			2.96E+01	2.2E+00	1.9E+00	6.0E+00					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	CFS-L06-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	7.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00	10	120	1.19E+03	99%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	6.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T04-A	1	7.51E+00			7.51E+00	7.4E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T05-A	1	1.63E+02			1.63E+02	1.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T06-A	1	4.36E+02			4.36E+02	1.7E+02	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T07-A	1	1.09E+04			1.09E+04	1.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T08-A	1	2.03E+04			2.03E+04	5.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T09-A	1	3.21E+04			3.21E+04	1.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	1.5E+02	2.0E+00	6.4E+00	10	120	1.26E+03	105%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	1.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T04-B	1	9.67E+00			9.67E+00	1.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T05-B	1	2.55E+02			2.55E+02	7.8E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T06-B	1	1.61E+03			1.61E+03	1.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T07-B	1	9.83E+03			9.83E+03	4.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T08-B	1	1.99E+04			1.99E+04	6.3E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T09-B	1	3.18E+04			3.18E+04	1.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	2.1E+01	2.0E+00	6.4E+00	10	150	1.50E+03	100%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	3.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T04-C	1	6.34E+00	E		6.34E+00	9.7E-02	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T05-C	1	1.70E+02			1.70E+02	1.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T06-C	1	1.34E+03			1.34E+03	3.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T07-C	1	1.06E+04			1.06E+04	1.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T08-C	1	1.98E+04			1.98E+04	4.4E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-T09-C	1	3.39E+04			3.39E+04	9.0E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	5.0E+01	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	2.8E+02	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	9.2E+01	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	9.6E+01	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	1.8E+02	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	7.3E+01	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1313-B03-C	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	CFS-L06-1313-T01-A	1	3.11E+01			3.11E+01	1.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T02-A	1	4.19E+01			4.19E+01	2.4E+01	1.0E+00	3.2E+00	1000	120	1.19E+03	96%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T03-A	1	5.00E-01	U1/2		5.00E-01	4.9E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T04-A	1	3.47E+04			3.47E+04	5.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T05-A	1	7.45E+04			7.45E+04	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T06-A	1	5.33E+03			5.33E+03	1.6E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T07-A	1	8.41E+04			8.41E+04	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T08-A	1	1.25E+05			1.25E+05	1.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T09-A	1	2.86E+05			2.86E+05	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T01-B	1	3.59E+01			3.59E+01	3.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T02-B	1	2.15E+01			2.15E+01	1.5E+02	1.0E+00	3.2E+00	1000	120	1.27E+03	104%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T03-B	1	3.58E+02			3.58E+02	4.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T04-B	1	3.43E+04			3.43E+04	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T05-B	1	6.67E+04			6.67E+04	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T06-B	1	6.82E+04			6.82E+04	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T07-B	1	7.73E+04			7.73E+04	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T08-B	1	1.21E+05			1.21E+05	8.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T09-B	1	2.29E+05			2.29E+05	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T01-C	1	3.03E+01			3.03E+01	2.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T02-C	1	3.22E+01			3.22E+01	1.8E+01	1.0E+00	3.2E+00	1000	120	1.32E+03	108%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T03-C	1	4.00E+02			4.00E+02	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T04-C	1	3.30E+04			3.30E+04	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T05-C	1	6.51E+04			6.51E+04	5.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T06-C	1	6.08E+04			6.08E+04	2.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T07-C	1	8.09E+04			8.09E+04	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T08-C	1	1.16E+05			1.16E+05	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-T09-C	1	2.00E+05			2.00E+05	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	7.6E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-B02-A	1	7.67E+00			7.67E+00	3.9E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-B03-A	1	2.30E+01			2.30E+01	4.5E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	2.3E+02	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	4.6E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-B03-B	1	1.36E+01			1.36E+01	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-B01-C	1	2.33E+00	E		2.33E+00	5.0E+02	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	1.4E+03	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1313-B03-C	1	1.47E+01			1.47E+01	2.2E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	CFS-L06-1313-T01-A	1	2.01E+03			2.01E+03	3.2E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T02-A	1	1.95E+03			1.95E+03	5.8E-01	1.2E+00	3.8E+00	10	120	2.99E+03	87%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T03-A	1	2.43E+01			2.43E+01	8.6E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T04-A	1	4.33E+02			4.33E+02	3.8E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T05-A	1	6.41E+01			6.41E+01	3.4E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T06-A	1	6.00E-01	U1/2		6.00E-01	4.2E+02	1.2E+00	3.8E+00			---		VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T07-A	1	6.26E+00			6.26E+00	3.2E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T08-A	1	6.66E+00			6.66E+00	3.4E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T09-A	1	7.26E+01			7.26E+01	1.9E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T01-B	1	2.03E+03			2.03E+03	4.1E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T02-B	1	9.64E+02			9.64E+02	9.7E+01	1.2E+00	3.8E+00	10	120	2.05E+03	91%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T03-B	1	1.28E+03			1.28E+03	1.4E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T04-B	1	4.36E+02			4.36E+02	6.8E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T05-B	1	4.92E+01			4.92E+01	3.7E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T06-B	1	1.10E+01			1.10E+01	4.3E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T07-B	1	7.41E+00			7.41E+00	3.4E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T08-B	1	9.09E+00			9.09E+00	1.6E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T09-B	1	1.00E+02			1.00E+02	9.0E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T01-C	1	2.06E+03			2.06E+03	4.6E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T02-C	1	1.89E+03			1.89E+03	7.6E-01	1.2E+00	3.8E+00	10	150	3.24E+03	90%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T03-C	1	1.27E+03			1.27E+03	2.1E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T04-C	1	4.36E+02			4.36E+02	2.7E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T05-C	1	5.68E+01			5.68E+01	2.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T06-C	1	9.29E+00			9.29E+00	2.9E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T07-C	1	9.53E+00			9.53E+00	1.4E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T08-C	1	8.20E+00			8.20E+00	3.1E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-T09-C	1	9.46E+01			9.46E+01	2.4E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	9.1E+01	1.2E+00	3.8E+00					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	5.5E+01	1.2E+00	3.8E+00					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-B03-A	1	6.00E-01	U1/2		6.00E-01	1.0E+02	1.2E+00	3.8E+00					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-B01-B	1	6.00E-01	U1/2		6.00E-01	6.6E+01	1.2E+00	3.8E+00					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-B02-B	1	6.00E-01	U1/2		6.00E-01	1.8E+02	1.2E+00	3.8E+00					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-B03-B	1	1.62E+00	E		1.62E+00	4.0E+01	1.2E+00	3.8E+00					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-B01-C	1	6.00E-01	U1/2		6.00E-01	2.8E+01	1.2E+00	3.8E+00					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-B02-C	1	6.00E-01	U1/2		6.00E-01	7.0E+02	1.2E+00	3.8E+00					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1313-B03-C	1	6.00E-01	U1/2		6.00E-01	1.6E+02	1.2E+00	3.8E+00					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	CFS-L06-1313-T01-A	1	5.50E+00	E		5.50E+00	2.7E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T02-A	1	3.73E+00	E		3.73E+00	4.5E+01	1.8E+00	5.7E+00	10	120	1.26E+03	105%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T04-A	1	3.64E+00	E		3.64E+00	5.5E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T05-A	1	1.17E+01			1.17E+01	5.9E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T06-A	1	2.42E+01			2.42E+01	1.7E+02	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T07-A	1	4.05E+03			4.05E+03	4.0E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T08-A	1	6.34E+03			6.34E+03	8.3E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T09-A	1	6.96E+03			6.96E+03	3.5E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T01-B	1	2.98E+00	E		2.98E+00	1.1E+02	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	5.4E+02	1.8E+00	5.7E+00	10	120	1.33E+03	111%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T03-B	1	2.45E+00	E		2.45E+00	7.4E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T04-B	1	3.88E+00	E		3.88E+00	4.1E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T05-B	1	1.78E+01			1.78E+01	7.3E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T06-B	1	2.25E+02			2.25E+02	6.3E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T07-B	1	3.86E+03			3.86E+03	3.0E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T08-B	1	6.31E+03			6.31E+03	1.4E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T09-B	1	6.83E+03			6.83E+03	5.7E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	1.0E+02	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00	10	150	1.59E+03	106%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T03-C	1	1.80E+00	E		1.80E+00	1.2E+02	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T04-C	1	3.69E+00	E		3.69E+00	3.2E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T05-C	1	1.14E+01			1.14E+01	1.8E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T06-C	1	1.94E+02			1.94E+02	3.0E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T07-C	1	4.06E+03			4.06E+03	1.8E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T08-C	1	6.29E+03			6.29E+03	1.8E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-T09-C	1	6.53E+03			6.53E+03	3.1E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.8E+00	5.7E+00					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-B03-A	1	2.93E+00	E		2.93E+00	3.9E+01	1.8E+00	5.7E+00					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-B01-B	1	9.00E-01	U1/2		9.00E-01	4.7E+02	1.8E+00	5.7E+00					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-B02-B	1	9.00E-01	U1/2		9.00E-01	9.1E+01	1.8E+00	5.7E+00					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-B03-B	1	9.00E-01	U1/2		9.00E-01	1.8E+02	1.8E+00	5.7E+00					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-B01-C	1	9.00E-01	U1/2		9.00E-01	4.3E+02	1.8E+00	5.7E+00					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-B02-C	1	9.00E-01	U1/2		9.00E-01	8.0E+01	1.8E+00	5.7E+00					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1313-B03-C	1	9.00E-01	U1/2		9.00E-01	1.0E+02	1.8E+00	5.7E+00					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	CFS-L06-1313-T01-A	1	9.76E+01			9.76E+01	4.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T02-A	1	5.72E+01			5.72E+01	9.9E+00	3.7E+00	1.2E+01	1000	120	1.39E+03	111%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T03-A	1	1.85E+00	U1/2		1.85E+00	2.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T04-A	1	1.85E+00	U1/2		1.85E+00	7.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T05-A	1	1.85E+00	U1/2		1.85E+00	4.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T06-A	1	1.85E+00	U1/2		1.85E+00	1.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T07-A	1	1.86E+01			1.86E+01	4.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T08-A	1	1.38E+01			1.38E+01	1.4E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T09-A	1	2.05E+03			2.05E+03	3.7E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T01-B	1	8.48E+01			8.48E+01	1.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T02-B	1	2.36E+01			2.36E+01	1.6E+02	3.7E+00	1.2E+01	1000	120	1.34E+03	109%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T03-B	1	4.51E+01			4.51E+01	5.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T04-B	1	1.85E+00	U1/2		1.85E+00	7.1E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T05-B	1	5.37E+00	E		5.37E+00	2.2E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T06-B	1	7.29E+00	E		7.29E+00	3.1E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T07-B	1	1.85E+00	U1/2		1.85E+00	6.5E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T08-B	1	6.00E+00	E		6.00E+00	3.7E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T09-B	1	2.81E+03			2.81E+03	6.3E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T01-C	1	9.00E+01			9.00E+01	2.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T02-C	1	8.58E+01			8.58E+01	7.2E+00	3.7E+00	1.2E+01	1000	120	1.43E+03	112%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T03-C	1	2.77E+01			2.77E+01	1.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T04-C	1	1.85E+00	U1/2		1.85E+00	2.1E+03	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T05-C	1	1.85E+00	U1/2		1.85E+00	6.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T06-C	1	5.51E+00	E		5.51E+00	3.8E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T07-C	1	1.85E+00	U1/2		1.85E+00	6.8E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T08-C	1	1.85E+00	U1/2		1.85E+00	1.5E+03	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-T09-C	1	2.77E+03			2.77E+03	6.0E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	1.4E+02	3.7E+00	1.2E+01					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	1.6E+02	3.7E+00	1.2E+01					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-B03-A	1	2.22E+01			2.22E+01	3.7E+01	3.7E+00	1.2E+01					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-B01-B	1	1.85E+00	U1/2		1.85E+00	2.7E+01	3.7E+00	1.2E+01					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-B02-B	1	1.85E+00	U1/2		1.85E+00	5.7E+01	3.7E+00	1.2E+01					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-B03-B	1	1.88E+01			1.88E+01	7.2E+01	3.7E+00	1.2E+01					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-B01-C	1	1.85E+00	U1/2		1.85E+00	1.3E+02	3.7E+00	1.2E+01					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-B02-C	1	1.85E+00	U1/2		1.85E+00	5.4E+01	3.7E+00	1.2E+01					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1313-B03-C	1	1.68E+01			1.68E+01	4.3E+01	3.7E+00	1.2E+01					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	CFS-L06-1313-T01-A	1	3.33E+04			3.33E+04	8.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T02-A	1	2.45E+04			2.45E+04	3.4E-01	1.6E+00	5.1E+00	1000	120	2.57E+04	92%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T03-A	1	1.50E+02			1.50E+02	1.0E+02	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T04-A	1	1.34E+04			1.34E+04	3.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T05-A	1	1.24E+04			1.24E+04	7.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T06-A	1	1.01E+03			1.01E+03	1.7E+02	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T07-A	1	1.43E+04			1.43E+04	6.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T08-A	1	1.78E+04			1.78E+04	5.7E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T09-A	1	2.66E+04			2.66E+04	7.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T01-B	1	3.47E+04			3.47E+04	6.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T02-B	1	1.23E+04			1.23E+04	1.0E+02	1.6E+00	5.1E+00	1000	120	1.34E+04	90%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T03-B	1	1.53E+04			1.53E+04	5.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T04-B	1	1.35E+04			1.35E+04	5.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T05-B	1	1.20E+04			1.20E+04	5.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T06-B	1	1.06E+04			1.06E+04	9.0E-02	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T07-B	1	1.37E+04			1.37E+04	3.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T08-B	1	1.72E+04			1.72E+04	4.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T09-B	1	2.50E+04			2.50E+04	5.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T01-C	1	3.25E+04			3.25E+04	1.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T02-C	1	2.26E+04			2.26E+04	5.4E-01	1.6E+00	5.1E+00	1000	120	2.36E+04	85%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T03-C	1	1.45E+04			1.45E+04	5.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T04-C	1	1.26E+04			1.26E+04	3.6E-02	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T05-C	1	1.18E+04			1.18E+04	3.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T06-C	1	8.82E+03			8.82E+03	3.5E+01	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T07-C	1	1.39E+04			1.39E+04	7.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T08-C	1	1.68E+04			1.68E+04	5.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-T09-C	1	2.58E+04			2.58E+04	5.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-B01-A	1	2.88E+01			2.88E+01	2.3E+00	1.6E+00	5.1E+00					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-B02-A	1	2.81E+01			2.81E+01	5.0E+00	1.6E+00	5.1E+00					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-B03-A	1	1.27E+03			1.27E+03	4.8E-01	1.6E+00	5.1E+00					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-B01-B	1	2.95E+01			2.95E+01	1.5E+01	1.6E+00	5.1E+00					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-B02-B	1	3.33E+01			3.33E+01	2.2E+00	1.6E+00	5.1E+00					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-B03-B	1	1.30E+03			1.30E+03	1.3E+00	1.6E+00	5.1E+00					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-B01-C	1	2.99E+01			2.99E+01	9.5E+00	1.6E+00	5.1E+00					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-B02-C	1	3.00E+01			3.00E+01	4.3E+00	1.6E+00	5.1E+00					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1313-B03-C	1	1.29E+03			1.29E+03	1.4E+00	1.6E+00	5.1E+00					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	CFS-L06-1313-T01-A	1	4.49E+02			4.49E+02	9.1E-01	1.5E+01	4.8E+01			---		VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T02-A	1	3.37E+02			3.37E+02	3.3E+00	1.5E+01	4.8E+01	10	120	1.68E+03	112%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T03-A	1	7.50E+00	U1/2		7.50E+00	1.7E+02	1.5E+01	4.8E+01			---		VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T04-A	1	1.73E+02			1.73E+02	4.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T05-A	1	9.96E+01			9.96E+01	2.9E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T06-A	1	7.50E+00	U1/2		7.50E+00	3.5E+02	1.5E+01	4.8E+01			---		VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T07-A	1	1.89E+02			1.89E+02	1.4E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T08-A	1	2.51E+02			2.51E+02	5.3E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T09-A	1	4.21E+02			4.21E+02	3.2E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T01-B	1	5.09E+02			5.09E+02	4.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T02-B	1	1.63E+02			1.63E+02	1.1E+02	1.5E+01	4.8E+01	10	120	1.44E+03	107%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T03-B	1	7.37E+02			7.37E+02	1.2E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T04-B	1	1.69E+02			1.69E+02	7.8E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T05-B	1	9.34E+01			9.34E+01	8.3E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T06-B	1	1.04E+02			1.04E+02	5.6E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T07-B	1	1.93E+02			1.93E+02	3.9E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T08-B	1	2.65E+02			2.65E+02	2.2E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T09-B	1	5.14E+02			5.14E+02	4.2E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T01-C	1	4.20E+02			4.20E+02	1.7E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T02-C	1	3.22E+02			3.22E+02	3.2E+00	1.5E+01	4.8E+01	10	150	1.92E+03	107%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T03-C	1	6.92E+02			6.92E+02	3.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T04-C	1	1.66E+02			1.66E+02	4.0E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T05-C	1	9.22E+01			9.22E+01	2.0E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T06-C	1	6.55E+01			6.55E+01	4.8E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T07-C	1	2.06E+02			2.06E+02	1.9E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T08-C	1	2.53E+02			2.53E+02	6.8E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-T09-C	1	4.79E+02			4.79E+02	5.8E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-B01-A	1	7.50E+00	U1/2		7.50E+00	2.8E+01	1.5E+01	4.8E+01					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-B02-A	1	7.50E+00	U1/2		7.50E+00	7.4E+01	1.5E+01	4.8E+01					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-B03-A	1	1.52E+01	E		1.52E+01	8.2E+01	1.5E+01	4.8E+01					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-B01-B	1	7.50E+00	U1/2		7.50E+00	2.7E+02	1.5E+01	4.8E+01					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-B02-B	1	7.50E+00	U1/2		7.50E+00	4.2E+02	1.5E+01	4.8E+01					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-B03-B	1	7.50E+00	U1/2		7.50E+00	6.8E+01	1.5E+01	4.8E+01					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-B01-C	1	7.50E+00	U1/2		7.50E+00	2.7E+02	1.5E+01	4.8E+01					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-B02-C	1	7.50E+00	U1/2		7.50E+00	1.8E+03	1.5E+01	4.8E+01					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1313-B03-C	1	2.87E+01	E		2.87E+01	4.2E+01	1.5E+01	4.8E+01					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	CFS-L06-1313-T01-A	1	2.08E+02			2.08E+02	2.9E+00	1.1E+00	3.5E+00			---		VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T02-A	1	3.11E+02			3.11E+02	2.1E+00	1.1E+00	3.5E+00	1000	120	1.73E+03	118%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T03-A	1	1.29E+01			1.29E+01	8.3E+01	1.1E+00	3.5E+00			---		VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T04-A	1	6.90E+02			6.90E+02	2.7E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T05-A	1	1.58E+03			1.58E+03	8.9E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T06-A	1	1.12E+03			1.12E+03	1.7E+02	1.1E+00	3.5E+00			---		VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T07-A	1	3.85E+04			3.85E+04	8.7E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T08-A	1	5.82E+04			5.82E+04	8.4E+00	1.1E+00	3.5E+00			---		VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T09-A	1	1.66E+05			1.66E+05	6.8E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T01-B	1	2.88E+02			2.88E+02	1.9E+00	1.1E+00	3.5E+00			---		VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T02-B	1	1.64E+02			1.64E+02	9.1E+01	1.1E+00	3.5E+00	1000	120	1.54E+03	115%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T03-B	1	5.92E+02			5.92E+02	1.7E+00	1.1E+00	3.5E+00			---		VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T04-B	1	7.23E+02			7.23E+02	7.4E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T05-B	1	1.62E+03			1.62E+03	4.6E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T06-B	1	4.21E+03			4.21E+03	9.8E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T07-B	1	3.69E+04			3.69E+04	7.6E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T08-B	1	5.92E+04			5.92E+04	1.5E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T09-B	1	1.53E+05			1.53E+05	5.8E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T01-C	1	3.09E+02			3.09E+02	1.3E+00	1.1E+00	3.5E+00			---		VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T02-C	1	3.17E+02			3.17E+02	1.6E+00	1.1E+00	3.5E+00	1000	120	1.65E+03	111%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T03-C	1	5.81E+02			5.81E+02	7.9E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T04-C	1	6.75E+02			6.75E+02	1.1E+00	1.1E+00	3.5E+00			---		VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T05-C	1	1.57E+03			1.57E+03	7.3E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T06-C	1	4.05E+03			4.05E+03	1.3E+01	1.1E+00	3.5E+00			---		VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T07-C	1	3.86E+04			3.86E+04	9.4E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T08-C	1	5.89E+04			5.89E+04	1.0E+00	1.1E+00	3.5E+00			---		VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-T09-C	1	1.59E+05			1.59E+05	8.2E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-B01-A	1	1.48E+01			1.48E+01	3.5E+01	1.1E+00	3.5E+00					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-B02-A	1	1.59E+01			1.59E+01	3.1E+01	1.1E+00	3.5E+00					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-B03-A	1	1.80E+02			1.80E+02	3.1E+00	1.1E+00	3.5E+00					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-B01-B	1	5.13E+00			5.13E+00	6.2E+01	1.1E+00	3.5E+00					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-B02-B	1	2.28E+01			2.28E+01	5.0E+00	1.1E+00	3.5E+00					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-B03-B	1	1.69E+02			1.69E+02	6.0E+00	1.1E+00	3.5E+00					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-B01-C	1	6.19E+00			6.19E+00	6.5E+01	1.1E+00	3.5E+00					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-B02-C	1	1.33E+01			1.33E+01	3.4E+01	1.1E+00	3.5E+00					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1313-B03-C	1	1.47E+02			1.47E+02	2.9E+00	1.1E+00	3.5E+00					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	CFS-L06-1313-T01-A	1	3.84E+05			3.84E+05	4.4E-01	2.5E+00	8.0E+00			---		VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T02-A	1	2.69E+05			2.69E+05	1.7E-01	2.5E+00	8.0E+00	1000	120	2.70E+05	90%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T03-A	1	2.02E+03			2.02E+03	1.1E+02	2.5E+00	8.0E+00			---		VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T04-A	1	8.12E+04			8.12E+04	3.7E-01	2.5E+00	8.0E+00			---		VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T05-A	1	4.81E+04			4.81E+04	6.0E-01	2.5E+00	8.0E+00			---		VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T06-A	1	5.51E+02			5.51E+02	1.6E+02	2.5E+00	8.0E+00			---		VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T07-A	1	8.17E+03			8.17E+03	6.4E-01	2.5E+00	8.0E+00			---		VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T08-A	1	9.15E+03			9.15E+03	1.5E+00	2.5E+00	8.0E+00			---		VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T09-A	1	1.01E+04			1.01E+04	7.9E-01	2.5E+00	8.0E+00			---		VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T01-B	1	3.82E+05			3.82E+05	8.0E-02	2.5E+00	8.0E+00			---		VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T02-B	1	1.32E+05			1.32E+05	8.3E+01	2.5E+00	8.0E+00	1000	120	1.34E+05	88%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T03-B	1	1.25E+05			1.25E+05	8.2E-01	2.5E+00	8.0E+00			---		VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T04-B	1	7.89E+04			7.89E+04	5.1E-01	2.5E+00	8.0E+00			---		VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T05-B	1	4.72E+04			4.72E+04	5.4E-01	2.5E+00	8.0E+00			---		VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T06-B	1	7.28E+03			7.28E+03	4.2E-01	2.5E+00	8.0E+00			---		VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T07-B	1	7.55E+03			7.55E+03	6.3E-01	2.5E+00	8.0E+00			---		VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T08-B	1	8.65E+03			8.65E+03	8.4E-01	2.5E+00	8.0E+00			---		VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T09-B	1	9.64E+03			9.64E+03	1.0E+00	2.5E+00	8.0E+00			---		VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T01-C	1	3.79E+05			3.79E+05	2.5E-01	2.5E+00	8.0E+00			---		VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T02-C	1	2.73E+05			2.73E+05	2.8E-01	2.5E+00	8.0E+00	1000	120	2.74E+05	87%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T03-C	1	1.30E+05			1.30E+05	2.9E-01	2.5E+00	8.0E+00			---		VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T04-C	1	8.18E+04			8.18E+04	1.2E+00	2.5E+00	8.0E+00			---		VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T05-C	1	4.79E+04			4.79E+04	4.8E-01	2.5E+00	8.0E+00			---		VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T06-C	1	5.91E+03			5.91E+03	3.0E+01	2.5E+00	8.0E+00			---		VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T07-C	1	7.49E+03			7.49E+03	8.6E-01	2.5E+00	8.0E+00			---		VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T08-C	1	8.14E+03			8.14E+03	1.2E+00	2.5E+00	8.0E+00			---		VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-T09-C	1	9.23E+03			9.23E+03	5.9E-01	2.5E+00	8.0E+00			---		VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-B01-A	1	1.25E+00	U1/2		1.25E+00	9.6E+02	2.5E+00	8.0E+00					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-B02-A	1	1.25E+00	U1/2		1.25E+00	8.7E+00	2.5E+00	8.0E+00					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-B03-A	1	3.77E+05			3.77E+05	7.3E-01	2.5E+00	8.0E+00					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-B01-B	1	2.57E+01			2.57E+01	8.1E+00	2.5E+00	8.0E+00					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-B02-B	1	1.25E+00	U1/2		1.25E+00	4.3E+00	2.5E+00	8.0E+00					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-B03-B	1	3.81E+05			3.81E+05	3.3E-01	2.5E+00	8.0E+00					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-B01-C	1	1.36E+01			1.36E+01	2.8E+00	2.5E+00	8.0E+00					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-B02-C	1	3.64E+00	E		3.64E+00	5.5E+00	2.5E+00	8.0E+00					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1313-B03-C	1	3.83E+05			3.83E+05	8.8E-01	2.5E+00	8.0E+00					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	CFS-L06-1313-T01-A	1	2.16E+03			2.16E+03	7.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T02-A	1	2.73E+03			2.73E+03	3.2E-01	1.0E+00	3.2E+00	1000	120	3.91E+03	99%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T03-A	1	1.52E+02			1.52E+02	1.3E+02	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T04-A	1	3.71E+03			3.71E+03	6.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T05-A	1	3.74E+03			3.74E+03	4.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T06-A	1	4.19E+02			4.19E+02	1.7E+02	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T07-A	1	1.05E+03			1.05E+03	1.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T08-A	1	1.19E+03			1.19E+03	7.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T09-A	1	1.46E+03			1.46E+03	7.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T01-B	1	2.40E+03			2.40E+03	6.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T02-B	1	1.80E+03			1.80E+03	8.9E+01	1.0E+00	3.2E+00	1000	120	2.91E+03	92%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T03-B	1	4.08E+03			4.08E+03	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T04-B	1	3.61E+03			3.61E+03	8.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T05-B	1	3.56E+03			3.56E+03	6.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T06-B	1	1.60E+03			1.60E+03	8.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T07-B	1	9.93E+02			9.93E+02	3.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T08-B	1	1.17E+03			1.17E+03	1.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T09-B	1	1.27E+03			1.27E+03	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T01-C	1	2.19E+03			2.19E+03	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T02-C	1	3.19E+03			3.19E+03	1.2E+00	1.0E+00	3.2E+00	1000	120	4.31E+03	93%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T03-C	1	4.15E+03			4.15E+03	2.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T04-C	1	3.55E+03			3.55E+03	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T05-C	1	3.64E+03			3.64E+03	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T06-C	1	1.53E+03			1.53E+03	1.3E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T07-C	1	1.09E+03			1.09E+03	5.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T08-C	1	1.19E+03			1.19E+03	3.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-T09-C	1	1.32E+03			1.32E+03	6.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	8.5E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	3.8E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-B03-A	1	1.14E+01			1.14E+01	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	2.3E+03	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	6.3E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-B03-B	1	1.14E+01			1.14E+01	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	1.8E+02	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	1.3E+04	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1313-B03-C	1	1.19E+01			1.19E+01	7.7E+00	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	CFS-L06-1313-T01-A	1	1.46E+06			1.46E+06	1.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T02-A	1	1.29E+06			1.29E+06	6.4E-01	6.8E+00	2.2E+01	1000	120	1.29E+06	88%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T03-A	1	1.38E+04			1.38E+04	8.3E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T04-A	1	7.54E+05			7.54E+05	5.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T05-A	1	7.22E+05			7.22E+05	7.8E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T06-A	1	5.85E+04			5.85E+04	1.6E+02	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T07-A	1	6.94E+05			6.94E+05	1.5E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T08-A	1	7.34E+05			7.34E+05	6.0E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T09-A	1	8.02E+05			8.02E+05	5.8E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T01-B	1	1.48E+06			1.48E+06	1.7E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T02-B	1	6.25E+05			6.25E+05	1.0E+02	6.8E+00	2.2E+01	1000	120	6.26E+05	87%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T03-B	1	8.53E+05			8.53E+05	8.7E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T04-B	1	7.43E+05			7.43E+05	8.3E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T05-B	1	7.01E+05			7.01E+05	2.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T06-B	1	6.35E+05			6.35E+05	2.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T07-B	1	6.56E+05			6.56E+05	3.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T08-B	1	7.09E+05			7.09E+05	4.8E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T09-B	1	7.96E+05			7.96E+05	1.9E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T01-C	1	1.40E+06			1.40E+06	6.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T02-C	1	1.27E+06			1.27E+06	2.8E-01	6.8E+00	2.2E+01	1000	120	1.27E+06	88%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T03-C	1	8.35E+05			8.35E+05	9.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T04-C	1	7.19E+05			7.19E+05	1.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T05-C	1	6.83E+05			6.83E+05	5.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T06-C	1	5.36E+05			5.36E+05	3.4E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T07-C	1	6.85E+05			6.85E+05	8.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T08-C	1	6.94E+05			6.94E+05	1.3E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-T09-C	1	7.82E+05			7.82E+05	1.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	3.8E+02	6.8E+00	2.2E+01					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-B02-A	1	1.65E+01	E		1.65E+01	7.3E+01	6.8E+00	2.2E+01					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-B03-A	1	5.41E+02			5.41E+02	7.6E+00	6.8E+00	2.2E+01					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-B01-B	1	3.40E+00	U1/2		3.40E+00	4.5E+01	6.8E+00	2.2E+01					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-B02-B	1	3.40E+00	U1/2		3.40E+00	6.4E+02	6.8E+00	2.2E+01					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-B03-B	1	2.36E+02			2.36E+02	6.8E+00	6.8E+00	2.2E+01					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-B01-C	1	3.40E+00	U1/2		3.40E+00	3.8E+01	6.8E+00	2.2E+01					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-B02-C	1	3.40E+00	U1/2		3.40E+00	1.4E+02	6.8E+00	2.2E+01					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1313-B03-C	1	4.80E+01			4.80E+01	4.7E+01	6.8E+00	2.2E+01					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	CFS-L06-1313-T01-A	1	9.61E+01			9.61E+01	9.6E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T02-A	1	9.64E+01			9.64E+01	3.6E+00	4.6E+00	1.5E+01	10	120	1.23E+03	95%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T03-A	1	2.30E+00	U1/2		2.30E+00	1.2E+01	4.6E+00	1.5E+01			---		VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T04-A	1	2.48E+02			2.48E+02	1.1E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T05-A	1	3.28E+02			3.28E+02	1.6E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T06-A	1	1.93E+01			1.93E+01	4.0E+02	4.6E+00	1.5E+01			---		VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T07-A	1	7.26E+02			7.26E+02	1.7E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T08-A	1	9.57E+02			9.57E+02	5.9E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T09-A	1	1.61E+03			1.61E+03	1.2E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T01-B	1	1.09E+02			1.09E+02	3.6E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T02-B	1	3.29E+01			3.29E+01	1.8E+02	4.6E+00	1.5E+01	10	120	1.31E+03	106%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T03-B	1	1.23E+02			1.23E+02	4.9E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T04-B	1	2.47E+02			2.47E+02	2.1E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T05-B	1	3.13E+02			3.13E+02	1.9E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T06-B	1	3.49E+02			3.49E+02	5.6E-01	4.6E+00	1.5E+01			---		VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T07-B	1	7.14E+02			7.14E+02	1.5E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T08-B	1	9.01E+02			9.01E+02	1.6E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T09-B	1	1.67E+03			1.67E+03	5.9E-01	4.6E+00	1.5E+01			---		VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T01-C	1	1.07E+02			1.07E+02	3.3E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T02-C	1	8.30E+01			8.30E+01	6.7E+00	4.6E+00	1.5E+01	10	150	1.54E+03	97%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T03-C	1	1.27E+02			1.27E+02	5.5E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T04-C	1	2.33E+02			2.33E+02	4.5E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T05-C	1	3.27E+02			3.27E+02	1.4E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T06-C	1	2.89E+02			2.89E+02	3.6E+01	4.6E+00	1.5E+01			---		VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T07-C	1	7.41E+02			7.41E+02	2.2E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T08-C	1	9.20E+02			9.20E+02	2.5E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-T09-C	1	1.70E+03			1.70E+03	2.7E-01	4.6E+00	1.5E+01			---		VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	1.7E+01	4.6E+00	1.5E+01					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	6.2E+00	4.6E+00	1.5E+01					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	2.7E+01	4.6E+00	1.5E+01					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-B01-B	1	2.30E+00	U1/2		2.30E+00	9.7E+00	4.6E+00	1.5E+01					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-B02-B	1	2.30E+00	U1/2		2.30E+00	6.1E+00	4.6E+00	1.5E+01					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-B03-B	1	2.30E+00	U1/2		2.30E+00	2.0E+01	4.6E+00	1.5E+01					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-B01-C	1	2.30E+00	U1/2		2.30E+00	1.2E+01	4.6E+00	1.5E+01					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-B02-C	1	2.30E+00	U1/2		2.30E+00	1.6E+01	4.6E+00	1.5E+01					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1313-B03-C	1	2.30E+00	U1/2		2.30E+00	8.7E+00	4.6E+00	1.5E+01					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	CFS-L06-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	9.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	1.9E+02	2.0E+00	6.4E+00	10	120	1.19E+03	99%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	1.7E+02	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	7.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	5.7E+02	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	3.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T07-A	1	9.26E+00			9.26E+00	2.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T08-A	1	1.92E+01			1.92E+01	3.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T09-A	1	3.39E+01			3.39E+01	4.0E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	7.7E+02	2.0E+00	6.4E+00	10	120	1.25E+03	104%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	9.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	1.7E+02	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	4.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	3.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T07-B	1	8.55E+00			8.55E+00	2.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T08-B	1	1.98E+01			1.98E+01	2.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T09-B	1	4.47E+01			4.47E+01	1.5E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	8.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	1.7E+02	2.0E+00	6.4E+00	10	150	1.48E+03	99%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	2.0E+02	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	4.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	7.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T07-C	1	9.19E+00			9.19E+00	5.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T08-C	1	1.93E+01			1.93E+01	1.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-T09-C	1	4.89E+01			4.89E+01	1.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	2.4E+02	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	8.8E+01	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	5.7E+01	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	5.6E+01	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	9.6E+01	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	9.2E+01	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1313-B03-C	1	1.00E+00	U1/2		1.00E+00	2.7E+02	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	CFS-L06-1313-T01-A	1	2.57E+01			2.57E+01	1.2E+01	1.5E+00	4.8E+00			---		VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T02-A	1	2.56E+01			2.56E+01	2.5E+00	1.5E+00	4.8E+00	10	120	1.29E+03	105%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T03-A	1	7.50E-01	U1/2		7.50E-01	9.4E+01	1.5E+00	4.8E+00			---		VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T04-A	1	2.80E+01			2.80E+01	5.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T05-A	1	2.90E+01			2.90E+01	1.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T06-A	1	3.86E+00	E		3.86E+00	1.4E+02	1.5E+00	4.8E+00			---		VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T07-A	1	4.02E+01			4.02E+01	1.5E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T08-A	1	4.15E+01			4.15E+01	2.4E+01	1.5E+00	4.8E+00			---		VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T09-A	1	5.36E+02			5.36E+02	9.1E-01	1.5E+00	4.8E+00			---		VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T01-B	1	2.53E+01			2.53E+01	6.8E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T02-B	1	1.26E+01			1.26E+01	8.4E+01	1.5E+00	4.8E+00	10	120	1.35E+03	112%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T03-B	1	2.37E+01			2.37E+01	3.9E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T04-B	1	2.63E+01			2.63E+01	2.9E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T05-B	1	2.86E+01			2.86E+01	3.5E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T06-B	1	2.85E+01			2.85E+01	3.0E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T07-B	1	4.01E+01			4.01E+01	1.3E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T08-B	1	4.81E+01			4.81E+01	2.8E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T09-B	1	5.21E+02			5.21E+02	2.4E-01	1.5E+00	4.8E+00			---		VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T01-C	1	2.34E+01			2.34E+01	4.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T02-C	1	2.61E+01			2.61E+01	3.0E+00	1.5E+00	4.8E+00	10	150	1.59E+03	104%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T03-C	1	2.39E+01			2.39E+01	4.0E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T04-C	1	2.76E+01			2.76E+01	3.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T05-C	1	2.83E+01			2.83E+01	5.9E-01	1.5E+00	4.8E+00			---		VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T06-C	1	2.47E+01			2.47E+01	3.4E+01	1.5E+00	4.8E+00			---		VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T07-C	1	4.27E+01			4.27E+01	2.8E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T08-C	1	4.60E+01			4.60E+01	4.3E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-T09-C	1	5.01E+02			5.01E+02	8.6E-01	1.5E+00	4.8E+00			---		VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-B01-A	1	7.50E-01	U1/2		7.50E-01	6.8E+01	1.5E+00	4.8E+00					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-B02-A	1	7.50E-01	U1/2		7.50E-01	4.2E+01	1.5E+00	4.8E+00					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-B03-A	1	2.17E+00	E		2.17E+00	1.4E+01	1.5E+00	4.8E+00					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-B01-B	1	1.54E+00	E		1.54E+00	5.9E+01	1.5E+00	4.8E+00					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-B02-B	1	7.50E-01	U1/2		7.50E-01	3.9E+01	1.5E+00	4.8E+00					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-B03-B	1	2.29E+00	E		2.29E+00	5.1E+01	1.5E+00	4.8E+00					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-B01-C	1	7.50E-01	U1/2		7.50E-01	6.0E+01	1.5E+00	4.8E+00					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-B02-C	1	7.50E-01	U1/2		7.50E-01	5.8E+01	1.5E+00	4.8E+00					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1313-B03-C	1	7.50E-01	U1/2		7.50E-01	2.1E+01	1.5E+00	4.8E+00					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	CFS-L06-1313-T01-A	1	9.86E+03			9.86E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 3:39 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T02-A	1	4.07E+03			4.07E+03	1.2E+00	1.0E+00	3.2E+00	10	120	5.13E+03	89%	VU ICP-OES	4/14/11 3:40 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T03-A	1	5.00E-01	U1/2		5.00E-01	1.6E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 3:42 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T04-A	1	3.73E+02			3.73E+02	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 3:44 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T05-A	1	5.34E+02			5.34E+02	2.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 3:45 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T06-A	1	3.00E+03			3.00E+03	1.6E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 3:47 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T07-A	1	1.67E+05			1.67E+05	2.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 3:49 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T08-A	1	1.77E+05			1.77E+05	7.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 3:50 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T09-A	1	1.60E+05			1.60E+05	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 3:52 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T01-B	1	1.06E+04			1.06E+04	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 3:59 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T02-B	1	2.21E+03			2.21E+03	8.9E+01	1.0E+00	3.2E+00	10	120	3.21E+03	84%	VU ICP-OES	4/14/11 4:00 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T03-B	1	5.86E+01			5.86E+01	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:02 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T04-B	1	5.25E+02			5.25E+02	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:04 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T05-B	1	6.82E+02			6.82E+02	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:05 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T06-B	1	2.04E+04			2.04E+04	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:07 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T07-B	1	1.64E+05			1.64E+05	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:09 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T08-B	1	1.70E+05			1.70E+05	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:10 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T09-B	1	1.71E+05			1.71E+05	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:12 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T01-C	1	1.01E+04			1.01E+04	7.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:14 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T02-C	1	4.03E+03			4.03E+03	2.4E-01	1.0E+00	3.2E+00	10	150	5.38E+03	90%	VU ICP-OES	4/14/11 4:15 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T03-C	1	5.75E+01			5.75E+01	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:17 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T04-C	1	3.36E+02			3.36E+02	3.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:19 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T05-C	1	6.24E+02			6.24E+02	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:20 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T06-C	1	1.70E+04			1.70E+04	3.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:22 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T07-C	1	1.89E+05			1.89E+05	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:23 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T08-C	1	1.88E+05			1.88E+05	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:25 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-T09-C	1	1.79E+05			1.79E+05	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:27 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	4.6E+03	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:24 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-B02-A	1	5.12E+00			5.12E+00	6.0E+00	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:26 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-B03-A	1	3.50E+00			3.50E+00	5.7E+00	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:27 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-B01-B	1	1.39E+00	E		1.39E+00	3.1E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:29 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-B02-B	1	2.69E+00	E		2.69E+00	8.9E+00	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:30 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-B03-B	1	2.70E+00	E		2.70E+00	1.5E+00	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:32 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	4.7E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:34 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-B02-C	1	3.14E+00	E		3.14E+00	4.4E+00	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:35 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1313-B03-C	1	2.23E+00	E		2.23E+00	2.5E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 3:37 PM	EPA Interlab L06 1313-1316 CFS

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	CFS-L07-1313-T01-A	1	8.94E+01			8.94E+01	2.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T02-A	1	1.00E+02			1.00E+02	3.4E+00	1.0E+00	3.2E+00	1000	100	1.18E+03	108%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T03-A	1	8.67E+01			8.67E+01	3.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T04-A	1	5.33E+01			5.33E+01	4.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T05-A	1	4.00E+01			4.00E+01	6.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T06-A	1	4.42E+01			4.42E+01	6.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T07-A	1	8.44E+03			8.44E+03	4.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T08-A	1	2.62E+04			2.62E+04	1.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T09-A	1	8.71E+04			8.71E+04	7.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T01-B	1	9.79E+01			9.79E+01	2.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T02-B	1	9.67E+01			9.67E+01	1.1E+00	1.0E+00	3.2E+00	1000	100	1.20E+03	110%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T03-B	1	8.79E+01			8.79E+01	4.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T04-B	1	6.06E+01			6.06E+01	6.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T05-B	1	4.61E+01			4.61E+01	7.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T06-B	1	3.69E+01			3.69E+01	1.2E+01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T07-B	1	7.84E+03			7.84E+03	9.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T08-B	1	1.89E+04			1.89E+04	6.5E+01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T09-B	1	8.71E+04			8.71E+04	3.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T01-C	1	1.03E+02			1.03E+02	1.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T02-C	1	1.01E+02			1.01E+02	2.3E+00	1.0E+00	3.2E+00	1000	100	1.19E+03	109%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T03-C	1	8.50E+01			8.50E+01	7.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T04-C	1	6.08E+01			6.08E+01	1.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T05-C	1	4.49E+01			4.49E+01	3.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T06-C	1	4.91E+01			4.91E+01	7.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T07-C	1	8.47E+03			8.47E+03	1.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T08-C	1	2.81E+04			2.81E+04	1.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-T09-C	1	8.83E+04			8.83E+04	1.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	7.9E+00	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-B02-A	1	1.45E+00	E		1.45E+00	3.8E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	3.3E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	4.8E+00	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	6.1E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	2.9E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	1.5E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	6.1E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1313-B03-C	1	5.00E-01	U1/2		5.00E-01	2.4E+00	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	CFS-L07-1313-T01-A	1	1.50E+01	E		1.50E+01	3.1E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T02-A	1	1.38E+01	E		1.38E+01	1.4E+01	7.5E+00	2.4E+01	10	100	1.16E+03	114%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T03-A	1	3.62E+01			3.62E+01	9.7E+00	7.5E+00	2.4E+01			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T04-A	1	3.76E+01			3.76E+01	1.1E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T05-A	1	3.85E+01			3.85E+01	6.0E+00	7.5E+00	2.4E+01			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T06-A	1	3.36E+01			3.36E+01	2.7E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T07-A	1	3.00E+02			3.00E+02	1.6E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T08-A	1	8.21E+02			8.21E+02	1.3E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T09-A	1	1.20E+03			1.20E+03	1.3E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T01-B	1	1.08E+01	E		1.08E+01	9.5E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T02-B	1	1.80E+01	E		1.80E+01	2.8E+01	7.5E+00	2.4E+01	10	100	1.10E+03	109%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T03-B	1	3.50E+01			3.50E+01	2.0E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T04-B	1	3.51E+01			3.51E+01	2.2E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T05-B	1	3.51E+01			3.51E+01	2.3E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T06-B	1	3.73E+01			3.73E+01	6.6E+00	7.5E+00	2.4E+01			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T07-B	1	2.54E+02			2.54E+02	2.6E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T08-B	1	6.00E+02			6.00E+02	7.2E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T09-B	1	1.11E+03			1.11E+03	8.0E+00	7.5E+00	2.4E+01			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T01-C	1	3.75E+00	U1/2		3.75E+00	7.0E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T02-C	1	1.31E+01	E		1.31E+01	1.6E+01	7.5E+00	2.4E+01	10	100	1.16E+03	115%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T03-C	1	3.53E+01			3.53E+01	2.1E+01	7.5E+00	2.4E+01			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T04-C	1	4.43E+01			4.43E+01	2.5E+00	7.5E+00	2.4E+01			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T05-C	1	2.37E+01	E		2.37E+01	3.3E+00	7.5E+00	2.4E+01			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T06-C	1	2.91E+01			2.91E+01	8.3E+00	7.5E+00	2.4E+01			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T07-C	1	2.51E+02			2.51E+02	9.9E+00	7.5E+00	2.4E+01			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T08-C	1	8.19E+02			8.19E+02	9.2E+00	7.5E+00	2.4E+01			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-T09-C	1	9.93E+02			9.93E+02	2.7E+00	7.5E+00	2.4E+01			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-B01-A	1	1.22E+01	E		1.22E+01	2.0E+01	7.5E+00	2.4E+01					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-B02-A	1	3.75E+00	U1/2		3.75E+00	4.5E+01	7.5E+00	2.4E+01					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-B03-A	1	1.44E+01	E		1.44E+01	1.2E+01	7.5E+00	2.4E+01					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-B01-B	1	3.75E+00	U1/2		3.75E+00	1.0E+02	7.5E+00	2.4E+01					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-B02-B	1	8.02E+00	E		8.02E+00	4.9E+01	7.5E+00	2.4E+01					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-B03-B	1	8.99E+00	E		8.99E+00	2.3E+01	7.5E+00	2.4E+01					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-B01-C	1	3.75E+00	U1/2		3.75E+00	6.4E+01	7.5E+00	2.4E+01					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-B02-C	1	3.75E+00	U1/2		3.75E+00	1.1E+02	7.5E+00	2.4E+01					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1313-B03-C	1	3.75E+00	U1/2		3.75E+00	1.2E+02	7.5E+00	2.4E+01					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	CFS-L07-1313-T01-A	1	6.14E+02			6.14E+02	2.6E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T02-A	1	3.09E+02			3.09E+02	1.8E+00	1.1E+01	3.5E+01	10	100	1.31E+03	101%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T03-A	1	8.65E+01			8.65E+01	7.0E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T04-A	1	3.70E+01			3.70E+01	2.5E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T05-A	1	1.76E+01	E		1.76E+01	3.0E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T06-A	1	1.88E+01	E		1.88E+01	5.4E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T07-A	1	2.91E+02			2.91E+02	3.6E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T08-A	1	7.84E+02			7.84E+02	9.7E-01	1.1E+01	3.5E+01			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T09-A	1	6.42E+04			6.42E+04	8.3E-01	1.1E+01	3.5E+01			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T01-B	1	5.93E+02			5.93E+02	2.1E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T02-B	1	3.08E+02			3.08E+02	2.2E+00	1.1E+01	3.5E+01	10	100	1.35E+03	104%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T03-B	1	9.16E+01			9.16E+01	9.6E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T04-B	1	3.60E+01			3.60E+01	2.4E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T05-B	1	5.83E+01			5.83E+01	1.8E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T06-B	1	1.96E+01	E		1.96E+01	5.3E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T07-B	1	2.42E+02			2.42E+02	3.1E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T08-B	1	4.61E+02			4.61E+02	6.9E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T09-B	1	7.08E+04			7.08E+04	3.3E-01	1.1E+01	3.5E+01			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T01-C	1	6.10E+02			6.10E+02	1.6E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T02-C	1	3.35E+02			3.35E+02	1.4E+00	1.1E+01	3.5E+01	10	100	1.50E+03	117%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T03-C	1	8.79E+01			8.79E+01	9.0E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T04-C	1	3.96E+01			3.96E+01	1.0E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T05-C	1	3.66E+01			3.66E+01	2.6E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T06-C	1	3.16E+01	E		3.16E+01	1.6E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T07-C	1	2.81E+02			2.81E+02	2.8E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T08-C	1	7.09E+02			7.09E+02	1.7E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-T09-C	1	6.96E+04			6.96E+04	1.1E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-B01-A	1	5.50E+00	U1/2		5.50E+00	1.9E+02	1.1E+01	3.5E+01					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-B02-A	1	5.50E+00	U1/2		5.50E+00	1.4E+02	1.1E+01	3.5E+01					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-B03-A	1	5.50E+00	U1/2		5.50E+00	2.6E+02	1.1E+01	3.5E+01					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-B01-B	1	5.50E+00	U1/2		5.50E+00	2.2E+02	1.1E+01	3.5E+01					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-B02-B	1	5.50E+00	U1/2		5.50E+00	4.4E+01	1.1E+01	3.5E+01					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-B03-B	1	2.54E+01	E		2.54E+01	2.6E+01	1.1E+01	3.5E+01					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-B01-C	1	5.50E+00	U1/2		5.50E+00	2.9E+01	1.1E+01	3.5E+01					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-B02-C	1	5.50E+00	U1/2		5.50E+00	2.4E+02	1.1E+01	3.5E+01					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1313-B03-C	1	1.29E+01	E		1.29E+01	2.0E+01	1.1E+01	3.5E+01					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	CFS-L07-1313-T01-A	1	9.26E+01			9.26E+01	4.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T02-A	1	9.25E+01			9.25E+01	6.3E-01	1.0E+00	3.2E+00	1000	100	1.20E+03	110%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T03-A	1	1.70E+02			1.70E+02	1.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T04-A	1	1.34E+02			1.34E+02	1.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T05-A	1	1.57E+02			1.57E+02	1.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T06-A	1	1.70E+02			1.70E+02	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T07-A	1	4.32E+02			4.32E+02	4.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T08-A	1	6.42E+02			6.42E+02	2.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T09-A	1	7.47E+02			7.47E+02	9.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T01-B	1	9.42E+01			9.42E+01	3.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T02-B	1	9.13E+01			9.13E+01	1.5E+00	1.0E+00	3.2E+00	1000	100	1.13E+03	104%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T03-B	1	1.60E+02			1.60E+02	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T04-B	1	1.25E+02			1.25E+02	2.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T05-B	1	1.52E+02			1.52E+02	8.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T06-B	1	1.65E+02			1.65E+02	5.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T07-B	1	4.15E+02			4.15E+02	8.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T08-B	1	4.50E+02			4.50E+02	6.8E+01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T09-B	1	7.44E+02			7.44E+02	3.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T01-C	1	8.40E+01			8.40E+01	2.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T02-C	1	8.35E+01			8.35E+01	2.3E+00	1.0E+00	3.2E+00	1000	100	1.18E+03	110%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T03-C	1	1.64E+02			1.64E+02	5.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T04-C	1	1.20E+02			1.20E+02	9.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T05-C	1	1.37E+02			1.37E+02	4.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T06-C	1	1.58E+02			1.58E+02	8.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T07-C	1	4.19E+02			4.19E+02	2.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T08-C	1	6.51E+02			6.51E+02	2.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-T09-C	1	8.73E+02			8.73E+02	7.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-B01-A	1	1.95E+01			1.95E+01	1.5E+00	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-B02-A	1	1.89E+01			1.89E+01	8.9E+00	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-B03-A	1	2.74E+01			2.74E+01	4.3E+00	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-B01-B	1	7.02E+00			7.02E+00	3.0E+00	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-B02-B	1	6.79E+00			6.79E+00	3.0E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-B03-B	1	1.28E+01			1.28E+01	1.5E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-B01-C	1	1.67E+00	E		1.67E+00	1.9E+02	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-B02-C	1	4.13E+00			4.13E+00	5.3E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1313-B03-C	1	1.04E+01			1.04E+01	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	CFS-L07-1313-T01-A	1	2.63E+03			2.63E+03	6.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T02-A	1	1.60E+03			1.60E+03	2.4E-01	1.0E+00	3.2E+00	10	100	2.55E+03	94%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T03-A	1	1.10E+03			1.10E+03	8.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T04-A	1	6.99E+02			6.99E+02	3.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T05-A	1	4.53E+02			4.53E+02	6.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T06-A	1	1.98E+02			1.98E+02	5.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T07-A	1	9.55E+01			9.55E+01	7.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T08-A	1	1.12E+02			1.12E+02	9.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T09-A	1	9.74E+01			9.74E+01	2.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T01-B	1	2.66E+03			2.66E+03	1.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T02-B	1	1.64E+03			1.64E+03	1.4E-01	1.0E+00	3.2E+00	10	100	2.53E+03	89%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T03-B	1	1.07E+03			1.07E+03	4.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T04-B	1	6.88E+02			6.88E+02	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T05-B	1	4.59E+02			4.59E+02	3.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T06-B	1	1.93E+02			1.93E+02	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T07-B	1	9.69E+01			9.69E+01	7.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T08-B	1	7.56E+01			7.56E+01	6.9E+01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T09-B	1	9.52E+01			9.52E+01	7.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T01-C	1	2.75E+03			2.75E+03	3.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T02-C	1	1.69E+03			1.69E+03	5.0E-01	1.0E+00	3.2E+00	10	100	2.60E+03	91%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T03-C	1	1.13E+03			1.13E+03	6.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T04-C	1	6.96E+02			6.96E+02	3.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T05-C	1	4.38E+02			4.38E+02	5.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T06-C	1	1.90E+02			1.90E+02	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T07-C	1	9.46E+01			9.46E+01	3.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T08-C	1	1.11E+02			1.11E+02	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-T09-C	1	9.42E+01			9.42E+01	9.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	5.2E+02	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	5.7E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-B03-A	1	2.71E+03			2.71E+03	1.0E-01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	1.8E+02	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	1.7E+02	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-B03-B	1	2.59E+03			2.59E+03	9.8E-01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	1.9E+02	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	5.0E+02	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1313-B03-C	1	2.76E+03			2.76E+03	1.9E+00	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	CFS-L07-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	2.2E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	7.8E+01	1.9E+00	6.0E+00	10	100	1.15E+03	115%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	1.4E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	3.7E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	2.1E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	6.2E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T07-A	1	4.30E+00	E		4.30E+00	1.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T08-A	1	6.82E+00			6.82E+00	4.1E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T09-A	1	9.50E-01	U1/2		9.50E-01	2.3E+02	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	1.9E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	5.4E+01	1.9E+00	6.0E+00	10	100	1.12E+03	112%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	4.3E+02	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	2.6E+02	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	8.0E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T07-B	1	4.13E+00	E		4.13E+00	2.8E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T08-B	1	4.59E+00	E		4.59E+00	5.9E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T09-B	1	9.50E-01	U1/2		9.50E-01	1.8E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	3.3E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	1.6E+03	1.9E+00	6.0E+00	10	100	1.15E+03	115%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	2.1E+02	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	1.8E+02	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	5.0E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	4.3E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T07-C	1	4.28E+00	E		4.28E+00	7.9E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T08-C	1	6.63E+00			6.63E+00	5.7E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-T09-C	1	9.50E-01	U1/2		9.50E-01	1.1E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	1.7E+02	1.9E+00	6.0E+00					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	7.3E+01	1.9E+00	6.0E+00					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	1.6E+01	1.9E+00	6.0E+00					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-B01-B	1	9.50E-01	U1/2		9.50E-01	1.8E+02	1.9E+00	6.0E+00					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-B02-B	1	9.50E-01	U1/2		9.50E-01	9.1E+01	1.9E+00	6.0E+00					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-B03-B	1	9.50E-01	U1/2		9.50E-01	7.0E+01	1.9E+00	6.0E+00					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-B01-C	1	9.50E-01	U1/2		9.50E-01	3.0E+02	1.9E+00	6.0E+00					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-B02-C	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1313-B03-C	1	9.50E-01	U1/2		9.50E-01	9.5E+01	1.9E+00	6.0E+00					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	CFS-L07-1313-T01-A	1	1.26E+01			1.26E+01	3.7E+00	2.2E+00	7.0E+00			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T02-A	1	1.78E+01			1.78E+01	2.0E+00	2.2E+00	7.0E+00	10	100	1.11E+03	109%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	4.0E+01	2.2E+00	7.0E+00			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T04-A	1	2.26E+01			2.26E+01	9.8E-01	2.2E+00	7.0E+00			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T05-A	1	5.10E+02			5.10E+02	4.7E-01	2.2E+00	7.0E+00			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T06-A	1	4.81E+03			4.81E+03	3.5E-01	2.2E+00	7.0E+00			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T07-A	1	3.37E+04			3.37E+04	6.3E-01	2.2E+00	7.0E+00			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T08-A	1	4.73E+04			4.73E+04	9.1E-01	2.2E+00	7.0E+00			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T09-A	1	4.63E+04			4.63E+04	8.6E-02	2.2E+00	7.0E+00			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T01-B	1	1.21E+01			1.21E+01	3.8E+00	2.2E+00	7.0E+00			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T02-B	1	1.10E+00	U1/2		1.10E+00	1.8E+02	2.2E+00	7.0E+00	10	100	1.05E+03	105%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	1.6E+01	2.2E+00	7.0E+00			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T04-B	1	1.94E+01			1.94E+01	1.6E+00	2.2E+00	7.0E+00			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T05-B	1	4.56E+02			4.56E+02	2.7E-01	2.2E+00	7.0E+00			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T06-B	1	4.68E+03			4.68E+03	8.2E-01	2.2E+00	7.0E+00			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T07-B	1	3.28E+04			3.28E+04	8.2E-01	2.2E+00	7.0E+00			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T08-B	1	3.48E+04			3.48E+04	6.5E+01	2.2E+00	7.0E+00			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T09-B	1	4.83E+04			4.83E+04	2.9E-01	2.2E+00	7.0E+00			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T01-C	1	1.32E+01			1.32E+01	3.5E+00	2.2E+00	7.0E+00			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T02-C	1	1.10E+00	U1/2		1.10E+00	4.5E+01	2.2E+00	7.0E+00	10	100	1.10E+03	110%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	4.7E+01	2.2E+00	7.0E+00			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T04-C	1	1.45E+01			1.45E+01	1.3E+00	2.2E+00	7.0E+00			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T05-C	1	2.89E+02			2.89E+02	5.8E-01	2.2E+00	7.0E+00			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T06-C	1	4.65E+03			4.65E+03	1.3E+00	2.2E+00	7.0E+00			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T07-C	1	3.31E+04			3.31E+04	2.4E+00	2.2E+00	7.0E+00			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T08-C	1	4.72E+04			4.72E+04	7.8E-01	2.2E+00	7.0E+00			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-T09-C	1	4.99E+04			4.99E+04	1.8E-01	2.2E+00	7.0E+00			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	5.9E+00	2.2E+00	7.0E+00					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	2.7E+00	2.2E+00	7.0E+00					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-B03-A	1	1.10E+00	U1/2		1.10E+00	4.3E+00	2.2E+00	7.0E+00					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-B01-B	1	1.10E+00	U1/2		1.10E+00	7.7E+00	2.2E+00	7.0E+00					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-B02-B	1	1.10E+00	U1/2		1.10E+00	7.3E+00	2.2E+00	7.0E+00					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-B03-B	1	1.10E+00	U1/2		1.10E+00	4.1E+00	2.2E+00	7.0E+00					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-B01-C	1	1.10E+00	U1/2		1.10E+00	1.8E+01	2.2E+00	7.0E+00					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-B02-C	1	1.10E+00	U1/2		1.10E+00	3.7E+00	2.2E+00	7.0E+00					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1313-B03-C	1	1.10E+00	U1/2		1.10E+00	2.6E+01	2.2E+00	7.0E+00					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	CFS-L07-1313-T01-A	1	3.22E+05			3.22E+05	9.0E-02	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T02-A	1	5.88E+05			5.88E+05	5.8E-01	2.6E+00	8.3E+00	1000	100	5.89E+05	88%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T03-A	1	6.04E+05			6.04E+05	9.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T04-A	1	6.24E+05			6.24E+05	1.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T05-A	1	6.48E+05			6.48E+05	5.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T06-A	1	6.81E+05			6.81E+05	2.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T07-A	1	1.04E+06			1.04E+06	7.5E-02	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T08-A	1	1.27E+06			1.27E+06	1.5E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T09-A	1	1.62E+06			1.62E+06	6.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T01-B	1	3.15E+05			3.15E+05	2.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T02-B	1	5.97E+05			5.97E+05	2.9E-01	2.6E+00	8.3E+00	1000	100	5.98E+05	90%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T03-B	1	5.95E+05			5.95E+05	7.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T04-B	1	6.06E+05			6.06E+05	7.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T05-B	1	6.66E+05			6.66E+05	5.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T06-B	1	6.70E+05			6.70E+05	2.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T07-B	1	9.88E+05			9.88E+05	3.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T08-B	1	9.37E+05			9.37E+05	6.6E+01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T09-B	1	1.61E+06			1.61E+06	9.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T01-C	1	3.48E+05			3.48E+05	8.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T02-C	1	6.22E+05			6.22E+05	8.3E-01	2.6E+00	8.3E+00	1000	100	6.23E+05	86%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T03-C	1	6.32E+05			6.32E+05	8.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T04-C	1	6.21E+05			6.21E+05	4.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T05-C	1	6.50E+05			6.50E+05	6.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T06-C	1	6.75E+05			6.75E+05	9.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T07-C	1	1.01E+06			1.01E+06	1.6E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T08-C	1	1.26E+06			1.26E+06	8.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-T09-C	1	1.58E+06			1.58E+06	6.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-B01-A	1	2.94E+01			2.94E+01	1.1E+01	2.6E+00	8.3E+00					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-B02-A	1	2.34E+01			2.34E+01	1.9E+01	2.6E+00	8.3E+00					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-B03-A	1	4.75E+01			4.75E+01	4.6E+01	2.6E+00	8.3E+00					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-B01-B	1	2.88E+01			2.88E+01	1.4E+01	2.6E+00	8.3E+00					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-B02-B	1	2.82E+01			2.82E+01	2.0E+01	2.6E+00	8.3E+00					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-B03-B	1	7.44E+01			7.44E+01	2.0E+01	2.6E+00	8.3E+00					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-B01-C	1	2.53E+01			2.53E+01	1.2E+01	2.6E+00	8.3E+00					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-B02-C	1	1.99E+01			1.99E+01	1.9E+01	2.6E+00	8.3E+00					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1313-B03-C	1	5.58E+01			5.58E+01	1.4E+01	2.6E+00	8.3E+00					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	CFS-L07-1313-T01-A	1	2.08E+02			2.08E+02	1.2E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T02-A	1	6.96E+01			6.96E+01	4.7E-01	1.2E+00	3.8E+00	10	100	1.14E+03	107%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T03-A	1	7.01E+00			7.01E+00	1.8E+01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T04-A	1	6.00E-01	U1/2		6.00E-01	2.6E+01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T05-A	1	6.00E-01	U1/2		6.00E-01	1.1E+02	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T06-A	1	6.00E-01	U1/2		6.00E-01	1.2E+02	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T07-A	1	6.00E-01	U1/2		6.00E-01	4.4E+01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T08-A	1	2.36E+01			2.36E+01	1.7E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T09-A	1	2.01E+03			2.01E+03	5.0E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T01-B	1	1.95E+02			1.95E+02	7.5E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T02-B	1	8.23E+01			8.23E+01	5.1E-01	1.2E+00	3.8E+00	10	100	1.12E+03	104%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T03-B	1	6.84E+00			6.84E+00	8.9E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T04-B	1	1.37E+00	E		1.37E+00	1.4E+01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T05-B	1	1.97E+00	E		1.97E+00	2.8E+01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T06-B	1	6.00E-01	U1/2		6.00E-01	1.5E+02	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T07-B	1	6.00E-01	U1/2		6.00E-01	7.5E+01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T08-B	1	1.38E+01			1.38E+01	6.7E+01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T09-B	1	2.07E+03			2.07E+03	7.7E-02	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T01-C	1	1.66E+02			1.66E+02	8.6E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T02-C	1	7.60E+01			7.60E+01	1.3E+00	1.2E+00	3.8E+00	10	100	1.16E+03	108%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T03-C	1	7.25E+00			7.25E+00	1.2E+01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T04-C	1	1.49E+00	E		1.49E+00	1.1E+01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T05-C	1	6.00E-01	U1/2		6.00E-01	8.1E+01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T06-C	1	6.00E-01	U1/2		6.00E-01	6.6E+01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T07-C	1	6.00E-01	U1/2		6.00E-01	7.8E+01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T08-C	1	2.78E+01			2.78E+01	2.7E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-T09-C	1	1.85E+03			1.85E+03	4.9E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	1.8E+05	1.2E+00	3.8E+00					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	2.4E+01	1.2E+00	3.8E+00					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-B03-A	1	6.00E-01	U1/2		6.00E-01	1.5E+01	1.2E+00	3.8E+00					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-B01-B	1	6.00E-01	U1/2		6.00E-01	2.6E+02	1.2E+00	3.8E+00					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-B02-B	1	6.00E-01	U1/2		6.00E-01	6.6E+02	1.2E+00	3.8E+00					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-B03-B	1	1.45E+00	E		1.45E+00	4.7E+01	1.2E+00	3.8E+00					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-B01-C	1	6.00E-01	U1/2		6.00E-01	1.6E+02	1.2E+00	3.8E+00					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-B02-C	1	6.00E-01	U1/2		6.00E-01	6.1E+02	1.2E+00	3.8E+00					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1313-B03-C	1	1.94E+00	E		1.94E+00	2.6E+01	1.2E+00	3.8E+00					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	CFS-L07-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	3.0E+01	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	2.5E+01	1.8E+00	5.7E+00	10	100	1.08E+03	108%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	4.0E+01	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	4.8E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T05-A	1	6.01E+00			6.01E+00	8.8E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T06-A	1	1.09E+02			1.09E+02	2.6E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T07-A	1	1.01E+03			1.01E+03	2.4E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T08-A	1	1.62E+03			1.62E+03	1.7E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T09-A	1	1.77E+03			1.77E+03	1.0E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	2.6E+01	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	4.4E+01	1.8E+00	5.7E+00	10	100	1.05E+03	105%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	2.8E+01	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	4.1E+01	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T05-B	1	5.16E+00	E		5.16E+00	1.9E+01	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T06-B	1	1.04E+02			1.04E+02	1.1E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T07-B	1	9.31E+02			9.31E+02	3.5E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T08-B	1	1.22E+03			1.22E+03	5.9E+01	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T09-B	1	1.88E+03			1.88E+03	1.2E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	2.9E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	1.9E+01	1.8E+00	5.7E+00	10	100	1.10E+03	110%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	6.2E+01	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	3.8E+01	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T05-C	1	9.00E-01	U1/2		9.00E-01	9.3E+01	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T06-C	1	9.43E+01			9.43E+01	7.3E-01	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T07-C	1	9.57E+02			9.57E+02	1.4E-01	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T08-C	1	1.58E+03			1.58E+03	9.2E-01	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-T09-C	1	1.75E+03			1.75E+03	4.5E-01	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	2.1E+01	1.8E+00	5.7E+00					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	8.0E+00	1.8E+00	5.7E+00					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	5.5E+01	1.8E+00	5.7E+00					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-B01-B	1	9.00E-01	U1/2		9.00E-01	1.2E+01	1.8E+00	5.7E+00					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-B02-B	1	9.00E-01	U1/2		9.00E-01	1.6E+01	1.8E+00	5.7E+00					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-B03-B	1	9.00E-01	U1/2		9.00E-01	4.1E+01	1.8E+00	5.7E+00					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-B01-C	1	9.00E-01	U1/2		9.00E-01	1.5E+01	1.8E+00	5.7E+00					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-B02-C	1	9.00E-01	U1/2		9.00E-01	3.7E+01	1.8E+00	5.7E+00					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1313-B03-C	1	9.00E-01	U1/2		9.00E-01	7.6E+01	1.8E+00	5.7E+00					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	CFS-L07-1313-T01-A	1	9.47E+03			9.47E+03	4.3E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T02-A	1	1.31E+03			1.31E+03	2.0E+00	3.7E+00	1.2E+01	10	100	2.30E+03	99%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T03-A	1	1.55E+02			1.55E+02	1.7E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T04-A	1	7.40E+01			7.40E+01	3.9E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T05-A	1	7.98E+01			7.98E+01	2.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T06-A	1	9.12E+02			9.12E+02	7.7E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T07-A	1	4.59E+05			4.59E+05	5.9E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T08-A	1	8.77E+05			8.77E+05	2.5E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T09-A	1	1.03E+06			1.03E+06	1.4E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T01-B	1	9.10E+03			9.10E+03	6.7E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T02-B	1	1.06E+03			1.06E+03	1.1E+00	3.7E+00	1.2E+01	10	100	2.15E+03	110%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T03-B	1	1.50E+02			1.50E+02	2.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T04-B	1	7.92E+01			7.92E+01	5.4E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T05-B	1	1.66E+02			1.66E+02	2.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T06-B	1	8.54E+02			8.54E+02	8.0E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T07-B	1	4.21E+05			4.21E+05	9.0E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T08-B	1	6.59E+05			6.59E+05	6.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T09-B	1	1.04E+06			1.04E+06	3.3E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T01-C	1	1.01E+04			1.01E+04	1.6E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T02-C	1	1.10E+03			1.10E+03	1.4E+00	3.7E+00	1.2E+01	10	100	2.07E+03	97%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T03-C	1	1.59E+02			1.59E+02	7.6E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T04-C	1	7.42E+01			7.42E+01	4.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T05-C	1	1.02E+02			1.02E+02	2.3E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T06-C	1	8.91E+02			8.91E+02	2.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T07-C	1	4.42E+05			4.42E+05	1.1E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T08-C	1	8.87E+05			8.87E+05	5.1E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-T09-C	1	1.05E+06			1.05E+06	9.3E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	7.3E+00	3.7E+00	1.2E+01					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	2.7E+01	3.7E+00	1.2E+01					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-B03-A	1	1.85E+00	U1/2		1.85E+00	5.8E+01	3.7E+00	1.2E+01					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-B01-B	1	1.85E+00	U1/2		1.85E+00	1.1E+03	3.7E+00	1.2E+01					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-B02-B	1	1.85E+00	U1/2		1.85E+00	2.5E+01	3.7E+00	1.2E+01					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-B03-B	1	1.85E+00	U1/2		1.85E+00	3.2E+01	3.7E+00	1.2E+01					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-B01-C	1	1.85E+00	U1/2		1.85E+00	1.4E+02	3.7E+00	1.2E+01					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-B02-C	1	1.85E+00	U1/2		1.85E+00	3.1E+01	3.7E+00	1.2E+01					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1313-B03-C	1	1.85E+00	U1/2		1.85E+00	2.0E+02	3.7E+00	1.2E+01					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	CFS-L07-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	2.1E+01	2.0E+00	6.4E+00	1000	100	1.13E+03	113%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T03-A	1	3.98E+00	E		3.98E+00	1.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	4.5E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T07-A	1	5.29E+01			5.29E+01	1.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T08-A	1	1.66E+04			1.66E+04	6.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T09-A	1	2.54E+05			2.54E+05	2.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	3.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00	1000	100	1.12E+03	112%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T03-B	1	2.82E+00	E		2.82E+00	5.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T05-B	1	1.63E+02			1.63E+02	4.1E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T06-B	1	3.18E+00	E		3.18E+00	1.6E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T07-B	1	1.98E+01			1.98E+01	2.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T08-B	1	1.41E+04			1.41E+04	5.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T09-B	1	2.87E+05			2.87E+05	5.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T01-C	1	4.69E+00	E		4.69E+00	5.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T02-C	1	1.08E+01			1.08E+01	5.4E+00	2.0E+00	6.4E+00	1000	100	1.15E+03	114%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T03-C	1	3.86E+00	E		3.86E+00	1.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T04-C	1	6.62E+00			6.62E+00	3.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T05-C	1	2.80E+01			2.80E+01	3.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T06-C	1	5.75E+01			5.75E+01	2.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T07-C	1	5.59E+01			5.59E+01	2.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T08-C	1	2.18E+04			2.18E+04	3.8E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-T09-C	1	2.54E+05			2.54E+05	4.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	5.7E+02	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-B03-A	1	1.28E+01			1.28E+01	3.2E+00	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-B01-B	1	3.69E+00	E		3.69E+00	7.2E+00	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	2.0E+00	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-B03-B	1	2.31E+01			2.31E+01	2.5E+00	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	8.3E+00	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1313-B03-C	1	1.31E+01			1.31E+01	4.0E+00	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	CFS-L07-1313-T01-A	1	3.75E+03			3.75E+03	4.8E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T02-A	1	7.98E+03			7.98E+03	1.1E+00	6.8E+00	2.2E+01	10	100	8.82E+03	84%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T03-A	1	5.04E+02			5.04E+02	1.5E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T04-A	1	1.77E+02			1.77E+02	4.9E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T05-A	1	3.83E+02			3.83E+02	1.7E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T06-A	1	1.32E+03			1.32E+03	5.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T07-A	1	7.58E+03			7.58E+03	3.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T08-A	1	6.33E+03			6.33E+03	3.8E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T09-A	1	9.03E+03			9.03E+03	5.3E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T01-B	1	4.91E+03			4.91E+03	6.7E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T02-B	1	6.96E+03			6.96E+03	9.1E-01	6.8E+00	2.2E+01	10	100	7.82E+03	86%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T03-B	1	4.97E+02			4.97E+02	1.2E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T04-B	1	1.73E+02			1.73E+02	2.1E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T05-B	1	4.67E+02			4.67E+02	1.2E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T06-B	1	1.34E+03			1.34E+03	4.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T07-B	1	7.97E+03			7.97E+03	1.5E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T08-B	1	4.38E+03			4.38E+03	6.5E+01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T09-B	1	9.00E+03			9.00E+03	2.9E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T01-C	1	4.34E+03			4.34E+03	1.1E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T02-C	1	7.80E+03			7.80E+03	1.1E+00	6.8E+00	2.2E+01	10	100	8.72E+03	92%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T03-C	1	5.60E+02			5.60E+02	9.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T04-C	1	1.71E+02			1.71E+02	2.9E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T05-C	1	2.91E+02			2.91E+02	1.9E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T06-C	1	1.33E+03			1.33E+03	1.1E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T07-C	1	7.77E+03			7.77E+03	1.8E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T08-C	1	6.00E+03			6.00E+03	4.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-T09-C	1	8.64E+03			8.64E+03	4.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	5.3E+01	6.8E+00	2.2E+01					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	9.1E+02	6.8E+00	2.2E+01					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	5.8E+01	6.8E+00	2.2E+01					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-B01-B	1	3.40E+00	U1/2		3.40E+00	6.1E+01	6.8E+00	2.2E+01					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-B02-B	1	3.40E+00	U1/2		3.40E+00	6.1E+01	6.8E+00	2.2E+01					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-B03-B	1	3.40E+00	U1/2		3.40E+00	6.6E+01	6.8E+00	2.2E+01					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-B01-C	1	3.40E+00	U1/2		3.40E+00	1.2E+01	6.8E+00	2.2E+01					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-B02-C	1	3.40E+00	U1/2		3.40E+00	1.8E+02	6.8E+00	2.2E+01					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1313-B03-C	1	3.40E+00	U1/2		3.40E+00	4.8E+02	6.8E+00	2.2E+01					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	CFS-L07-1313-T01-A	1	2.01E+01			2.01E+01	6.0E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T02-A	1	2.17E+01			2.17E+01	7.5E-01	1.9E+00	6.0E+00	10	100	8.82E+02	86%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T03-A	1	2.00E+01			2.00E+01	2.0E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T04-A	1	2.00E+01			2.00E+01	2.8E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T05-A	1	2.05E+01			2.05E+01	6.3E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T06-A	1	2.00E+01			2.00E+01	6.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T07-A	1	2.31E+01			2.31E+01	1.6E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T08-A	1	1.99E+01			1.99E+01	2.2E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T09-A	1	5.08E+01			5.08E+01	1.7E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T01-B	1	2.11E+01			2.11E+01	4.5E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T02-B	1	2.13E+01			2.13E+01	3.1E-01	1.9E+00	6.0E+00	10	100	8.61E+02	84%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T03-B	1	2.07E+01			2.07E+01	3.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T04-B	1	1.93E+01			1.93E+01	9.1E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T05-B	1	1.88E+01			1.88E+01	1.2E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T06-B	1	2.15E+01			2.15E+01	9.1E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T07-B	1	2.08E+01			2.08E+01	1.6E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T08-B	1	2.07E+01			2.07E+01	2.3E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T09-B	1	4.59E+01			4.59E+01	8.8E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T01-C	1	2.03E+01			2.03E+01	5.0E-01	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T02-C	1	2.24E+01			2.24E+01	2.5E+00	1.9E+00	6.0E+00	10	100	8.96E+02	87%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T03-C	1	2.24E+01			2.24E+01	9.2E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T04-C	1	2.13E+01			2.13E+01	4.6E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T05-C	1	1.97E+01			1.97E+01	6.9E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T06-C	1	1.86E+01			1.86E+01	9.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T07-C	1	2.26E+01			2.26E+01	1.8E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T08-C	1	1.92E+01			1.92E+01	1.1E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-T09-C	1	4.10E+01			4.10E+01	1.2E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-B01-A	1	6.27E+00			6.27E+00	1.1E+01	1.9E+00	6.0E+00					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-B02-A	1	7.39E+00			7.39E+00	1.3E+01	1.9E+00	6.0E+00					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-B03-A	1	5.47E+00	E		5.47E+00	1.9E+01	1.9E+00	6.0E+00					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-B01-B	1	7.38E+00			7.38E+00	6.7E+00	1.9E+00	6.0E+00					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-B02-B	1	6.44E+00			6.44E+00	1.7E+01	1.9E+00	6.0E+00					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-B03-B	1	5.62E+00	E		5.62E+00	1.4E+01	1.9E+00	6.0E+00					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-B01-C	1	6.74E+00			6.74E+00	8.7E+00	1.9E+00	6.0E+00					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-B02-C	1	7.31E+00			7.31E+00	1.0E+01	1.9E+00	6.0E+00					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1313-B03-C	1	4.89E+00	E		4.89E+00	6.6E+00	1.9E+00	6.0E+00					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	CFS-L07-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	4.6E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T02-A	1	5.61E+00	E		5.61E+00	1.7E+00	2.0E+00	6.4E+00	10	100	1.09E+03	109%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T04-A	1	2.40E+00	E		2.40E+00	6.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T05-A	1	2.69E+02			2.69E+02	9.5E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T06-A	1	1.77E+03			1.77E+03	7.3E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T07-A	1	1.08E+04			1.08E+04	4.2E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T08-A	1	2.12E+04			2.12E+04	3.3E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T09-A	1	3.51E+04			3.51E+04	5.2E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	3.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	3.5E+01	2.0E+00	6.4E+00	10	100	1.06E+03	106%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	9.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	1.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T05-B	1	2.22E+02			2.22E+02	2.8E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T06-B	1	1.72E+03			1.72E+03	9.5E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T07-B	1	1.01E+04			1.01E+04	1.5E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T08-B	1	1.60E+04			1.60E+04	6.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T09-B	1	3.36E+04			3.36E+04	4.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	2.8E+01	2.0E+00	6.4E+00	10	100	1.10E+03	110%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	6.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	4.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T05-C	1	1.32E+02			1.32E+02	7.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T06-C	1	1.67E+03			1.67E+03	7.2E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T07-C	1	1.02E+04			1.02E+04	1.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T08-C	1	2.17E+04			2.17E+04	2.8E-01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-T09-C	1	3.39E+04			3.39E+04	1.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	3.3E+02	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	2.6E+01	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	5.3E+01	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	7.0E+01	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	5.9E+00	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	1.2E+03	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1313-B03-C	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	CFS-L07-1313-T01-A	1	2.58E+01			2.58E+01	1.3E+01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T02-A	1	8.79E+01			8.79E+01	9.3E+00	1.0E+00	3.2E+00	1000	100	1.16E+03	107%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T03-A	1	1.60E+03			1.60E+03	1.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T04-A	1	3.27E+04			3.27E+04	2.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T05-A	1	7.20E+04			7.20E+04	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T06-A	1	6.82E+04			6.82E+04	4.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T07-A	1	8.36E+04			8.36E+04	6.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T08-A	1	1.26E+05			1.26E+05	9.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T09-A	1	2.63E+05			2.63E+05	3.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T01-B	1	2.99E+01			2.99E+01	4.0E+01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T02-B	1	2.92E+01			2.92E+01	3.2E+01	1.0E+00	3.2E+00	1000	100	1.10E+03	107%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T03-B	1	1.78E+03			1.78E+03	8.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T04-B	1	2.82E+04			2.82E+04	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T05-B	1	6.93E+04			6.93E+04	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T06-B	1	6.83E+04			6.83E+04	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T07-B	1	8.25E+04			8.25E+04	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T08-B	1	9.07E+04			9.07E+04	6.3E+01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T09-B	1	2.49E+05			2.49E+05	7.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T01-C	1	2.17E+01			2.17E+01	2.7E+01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T02-C	1	4.61E+01			4.61E+01	1.5E+01	1.0E+00	3.2E+00	1000	100	1.13E+03	109%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T03-C	1	1.67E+03			1.67E+03	8.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T04-C	1	2.90E+04			2.90E+04	6.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T05-C	1	6.73E+04			6.73E+04	2.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T06-C	1	6.88E+04			6.88E+04	9.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T07-C	1	8.12E+04			8.12E+04	4.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T08-C	1	1.27E+05			1.27E+05	9.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-T09-C	1	2.29E+05			2.29E+05	3.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	2.9E+03	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-B02-A	1	3.38E+00			3.38E+00	1.1E+02	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-B03-A	1	6.12E+00			6.12E+00	1.6E+02	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	1.7E+02	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	2.1E+02	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-B03-B	1	3.14E+00	E		3.14E+00	2.4E+02	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-B01-C	1	3.74E+00			3.74E+00	2.8E+02	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-B02-C	1	3.21E+00			3.21E+00	3.6E+02	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1313-B03-C	1	1.60E+00	E		1.60E+00	3.9E+02	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	CFS-L07-1313-T01-A	1	1.60E+03			1.60E+03	2.8E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T02-A	1	1.86E+03			1.86E+03	2.1E-02	1.2E+00	3.8E+00	10	100	2.77E+03	91%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T03-A	1	1.08E+03			1.08E+03	1.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T04-A	1	3.98E+02			3.98E+02	6.3E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T05-A	1	4.74E+01			4.74E+01	5.5E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T06-A	1	1.13E+01			1.13E+01	1.1E+01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T07-A	1	1.76E+01			1.76E+01	7.7E+01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T08-A	1	7.71E+00			7.71E+00	2.3E+01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T09-A	1	9.29E+01			9.29E+01	1.6E+01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T01-B	1	1.76E+03			1.76E+03	1.7E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T02-B	1	1.85E+03			1.85E+03	6.5E-01	1.2E+00	3.8E+00	10	100	2.85E+03	100%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T03-B	1	1.12E+03			1.12E+03	1.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T04-B	1	4.58E+02			4.58E+02	9.9E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T05-B	1	5.50E+01			5.50E+01	2.8E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T06-B	1	9.03E+00			9.03E+00	2.7E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T07-B	1	1.76E+01			1.76E+01	6.3E+01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T08-B	1	8.89E+00			8.89E+00	1.3E+02	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T09-B	1	9.42E+01			9.42E+01	1.8E+01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T01-C	1	1.94E+03			1.94E+03	7.3E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T02-C	1	1.98E+03			1.98E+03	1.4E+00	1.2E+00	3.8E+00	10	100	2.89E+03	92%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T03-C	1	1.22E+03			1.22E+03	6.5E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T04-C	1	4.51E+02			4.51E+02	3.0E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T05-C	1	6.83E+01			6.83E+01	1.5E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T06-C	1	9.52E+00			9.52E+00	1.0E+01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T07-C	1	6.57E+00			6.57E+00	4.0E+01	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T08-C	1	1.52E+01			1.52E+01	1.0E+02	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-T09-C	1	8.73E+01			8.73E+01	5.3E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	2.0E+02	1.2E+00	3.8E+00					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	3.4E+02	1.2E+00	3.8E+00					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-B03-A	1	7.60E+00			7.60E+00	1.8E+01	1.2E+00	3.8E+00					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-B01-B	1	6.00E-01	U1/2		6.00E-01	8.8E+01	1.2E+00	3.8E+00					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-B02-B	1	1.28E+00	E		1.28E+00	5.8E+01	1.2E+00	3.8E+00					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-B03-B	1	3.10E+00	E		3.10E+00	1.8E+01	1.2E+00	3.8E+00					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-B01-C	1	1.48E+00	E		1.48E+00	8.9E+01	1.2E+00	3.8E+00					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-B02-C	1	1.52E+00	E		1.52E+00	7.2E+01	1.2E+00	3.8E+00					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1313-B03-C	1	3.28E+00	E		3.28E+00	3.6E+01	1.2E+00	3.8E+00					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	CFS-L07-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	2.2E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T02-A	1	3.17E+00	E		3.17E+00	6.1E+01	1.8E+00	5.7E+00	10	100	1.09E+03	109%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	8.6E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	3.7E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T05-A	1	1.50E+01			1.50E+01	5.5E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T06-A	1	2.29E+02			2.29E+02	8.0E-01	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T07-A	1	3.68E+03			3.68E+03	1.9E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T08-A	1	6.06E+03			6.06E+03	4.7E-01	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T09-A	1	6.50E+03			6.50E+03	5.3E-01	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	2.5E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	8.1E+02	1.8E+00	5.7E+00	10	100	1.06E+03	106%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	2.6E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	4.0E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T05-B	1	1.24E+01			1.24E+01	1.2E+01	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T06-B	1	2.16E+02			2.16E+02	9.6E-02	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T07-B	1	3.50E+03			3.50E+03	4.2E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T08-B	1	4.97E+03			4.97E+03	6.2E+01	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T09-B	1	6.51E+03			6.51E+03	3.3E-01	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	2.1E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	2.1E+02	1.8E+00	5.7E+00	10	100	1.10E+03	110%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T05-C	1	8.50E+00			8.50E+00	9.9E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T06-C	1	2.03E+02			2.03E+02	1.4E+00	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T07-C	1	3.63E+03			3.63E+03	3.4E-01	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T08-C	1	6.09E+03			6.09E+03	6.2E-01	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-T09-C	1	6.48E+03			6.48E+03	5.5E-01	1.8E+00	5.7E+00			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	3.3E+01	1.8E+00	5.7E+00					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	3.2E+02	1.8E+00	5.7E+00					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	4.8E+02	1.8E+00	5.7E+00					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-B01-B	1	9.00E-01	U1/2		9.00E-01	5.7E+01	1.8E+00	5.7E+00					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-B02-B	1	9.00E-01	U1/2		9.00E-01	3.9E+01	1.8E+00	5.7E+00					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-B03-B	1	9.00E-01	U1/2		9.00E-01	6.1E+01	1.8E+00	5.7E+00					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-B01-C	1	9.00E-01	U1/2		9.00E-01	1.4E+01	1.8E+00	5.7E+00					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-B02-C	1	9.00E-01	U1/2		9.00E-01	6.2E+02	1.8E+00	5.7E+00					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1313-B03-C	1	9.00E-01	U1/2		9.00E-01	3.8E+01	1.8E+00	5.7E+00					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	CFS-L07-1313-T01-A	1	7.44E+01			7.44E+01	1.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T02-A	1	8.02E+01			8.02E+01	1.7E+01	3.7E+00	1.2E+01	1000	100	1.19E+03	111%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T03-A	1	4.07E+01			4.07E+01	2.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T04-A	1	1.58E+01			1.58E+01	1.1E+02	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T05-A	1	3.74E+00	E		3.74E+00	1.2E+02	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T06-A	1	2.15E+01			2.15E+01	9.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T07-A	1	2.38E+01			2.38E+01	3.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T08-A	1	3.74E+01			3.74E+01	1.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T09-A	1	2.26E+03			2.26E+03	5.6E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T01-B	1	9.98E+01			9.98E+01	1.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T02-B	1	6.65E+01			6.65E+01	2.8E+01	3.7E+00	1.2E+01	1000	100	1.25E+03	118%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T03-B	1	3.77E+01			3.77E+01	2.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T04-B	1	7.77E+00	E		7.77E+00	1.8E+02	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T05-B	1	7.03E+00	E		7.03E+00	1.3E+02	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T06-B	1	1.20E+01			1.20E+01	5.9E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T07-B	1	2.38E+01			2.38E+01	4.9E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T08-B	1	4.13E+00	E		4.13E+00	3.2E+02	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T09-B	1	2.49E+03			2.49E+03	4.0E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T01-C	1	7.81E+01			7.81E+01	2.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T02-C	1	6.74E+01			6.74E+01	3.7E+01	3.7E+00	1.2E+01	1000	100	1.17E+03	111%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T03-C	1	5.10E+01			5.10E+01	2.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T04-C	1	2.08E+01			2.08E+01	7.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T05-C	1	1.85E+00	U1/2		1.85E+00	2.1E+02	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T06-C	1	3.10E+01			3.10E+01	3.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T07-C	1	4.84E+01			4.84E+01	4.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T08-C	1	9.46E+00	E		9.46E+00	1.6E+02	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-T09-C	1	2.56E+03			2.56E+03	1.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-B01-A	1	1.69E+01			1.69E+01	6.3E+01	3.7E+00	1.2E+01					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-B02-A	1	1.35E+01			1.35E+01	1.9E+01	3.7E+00	1.2E+01					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-B03-A	1	4.04E+01			4.04E+01	1.2E+01	3.7E+00	1.2E+01					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-B01-B	1	7.84E+00	E		7.84E+00	5.8E+01	3.7E+00	1.2E+01					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-B02-B	1	1.09E+01	E		1.09E+01	5.0E+01	3.7E+00	1.2E+01					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-B03-B	1	2.70E+01			2.70E+01	5.0E+01	3.7E+00	1.2E+01					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-B01-C	1	4.61E+00	E		4.61E+00	1.3E+02	3.7E+00	1.2E+01					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-B02-C	1	2.78E+01			2.78E+01	4.4E+01	3.7E+00	1.2E+01					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1313-B03-C	1	1.85E+01			1.85E+01	1.3E+01	3.7E+00	1.2E+01					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	CFS-L07-1313-T01-A	1	3.25E+04			3.25E+04	4.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T02-A	1	1.98E+04			1.98E+04	4.4E-01	1.6E+00	5.1E+00	1000	100	2.08E+04	99%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T03-A	1	1.47E+04			1.47E+04	1.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T04-A	1	1.28E+04			1.28E+04	7.8E-02	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T05-A	1	1.20E+04			1.20E+04	5.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T06-A	1	9.97E+03			9.97E+03	7.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T07-A	1	1.34E+04			1.34E+04	5.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T08-A	1	1.70E+04			1.70E+04	7.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T09-A	1	2.58E+04			2.58E+04	2.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T01-B	1	3.24E+04			3.24E+04	8.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T02-B	1	2.13E+04			2.13E+04	7.2E-01	1.6E+00	5.1E+00	1000	100	2.22E+04	90%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T03-B	1	1.40E+04			1.40E+04	9.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T04-B	1	1.24E+04			1.24E+04	7.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T05-B	1	1.22E+04			1.22E+04	4.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T06-B	1	9.94E+03			9.94E+03	7.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T07-B	1	1.35E+04			1.35E+04	3.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T08-B	1	1.23E+04			1.23E+04	7.1E+01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T09-B	1	2.48E+04			2.48E+04	6.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T01-C	1	3.31E+04			3.31E+04	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T02-C	1	2.05E+04			2.05E+04	7.0E-01	1.6E+00	5.1E+00	1000	100	2.15E+04	95%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T03-C	1	1.46E+04			1.46E+04	9.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T04-C	1	1.24E+04			1.24E+04	2.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T05-C	1	1.19E+04			1.19E+04	6.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T06-C	1	9.84E+03			9.84E+03	1.6E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T07-C	1	1.34E+04			1.34E+04	3.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T08-C	1	1.69E+04			1.69E+04	4.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-T09-C	1	2.49E+04			2.49E+04	5.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-B01-A	1	7.08E+00			7.08E+00	6.5E+01	1.6E+00	5.1E+00					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-B02-A	1	9.89E+00			9.89E+00	2.8E+01	1.6E+00	5.1E+00					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-B03-A	1	3.60E+02			3.60E+02	1.3E+00	1.6E+00	5.1E+00					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-B01-B	1	7.50E+00			7.50E+00	2.2E+01	1.6E+00	5.1E+00					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-B02-B	1	4.97E+00	E		4.97E+00	4.3E+01	1.6E+00	5.1E+00					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-B03-B	1	2.89E+02			2.89E+02	3.8E-01	1.6E+00	5.1E+00					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-B01-C	1	4.12E+00	E		4.12E+00	2.9E+02	1.6E+00	5.1E+00					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-B02-C	1	1.31E+01			1.31E+01	1.4E+01	1.6E+00	5.1E+00					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1313-B03-C	1	2.82E+02			2.82E+02	3.2E+00	1.6E+00	5.1E+00					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	CFS-L07-1313-T01-A	1	4.81E+02			4.81E+02	2.6E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T02-A	1	3.81E+02			3.81E+02	3.2E+00	1.5E+01	4.8E+01	10	100	1.50E+03	112%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T03-A	1	4.43E+02			4.43E+02	7.5E-01	1.5E+01	4.8E+01			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T04-A	1	1.39E+02			1.39E+02	6.4E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T05-A	1	1.08E+02			1.08E+02	1.3E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T06-A	1	6.59E+01			6.59E+01	2.4E+01	1.5E+01	4.8E+01			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T07-A	1	1.70E+02			1.70E+02	1.5E+01	1.5E+01	4.8E+01			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T08-A	1	2.18E+02			2.18E+02	5.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T09-A	1	3.97E+02			3.97E+02	9.8E-01	1.5E+01	4.8E+01			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T01-B	1	5.76E+02			5.76E+02	1.6E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T02-B	1	4.60E+02			4.60E+02	3.1E+00	1.5E+01	4.8E+01	10	100	1.42E+03	96%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T03-B	1	4.44E+02			4.44E+02	8.3E-01	1.5E+01	4.8E+01			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T04-B	1	1.46E+02			1.46E+02	1.4E+01	1.5E+01	4.8E+01			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T05-B	1	7.89E+01			7.89E+01	1.6E+01	1.5E+01	4.8E+01			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T06-B	1	6.19E+01			6.19E+01	2.6E+01	1.5E+01	4.8E+01			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T07-B	1	1.50E+02			1.50E+02	3.2E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T08-B	1	1.60E+02			1.60E+02	7.5E+01	1.5E+01	4.8E+01			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T09-B	1	4.44E+02			4.44E+02	1.6E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T01-C	1	5.02E+02			5.02E+02	1.2E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T02-C	1	4.02E+02			4.02E+02	2.8E+00	1.5E+01	4.8E+01	10	100	1.50E+03	110%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T03-C	1	5.11E+02			5.11E+02	6.4E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T04-C	1	1.55E+02			1.55E+02	2.4E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T05-C	1	1.03E+02			1.03E+02	2.7E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T06-C	1	7.31E+01			7.31E+01	1.3E+01	1.5E+01	4.8E+01			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T07-C	1	1.80E+02			1.80E+02	7.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T08-C	1	2.20E+02			2.20E+02	1.1E+01	1.5E+01	4.8E+01			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-T09-C	1	4.32E+02			4.32E+02	2.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-B01-A	1	7.50E+00	U1/2		7.50E+00	1.4E+02	1.5E+01	4.8E+01					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-B02-A	1	7.50E+00	U1/2		7.50E+00	6.9E+02	1.5E+01	4.8E+01					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-B03-A	1	7.50E+00	U1/2		7.50E+00	4.5E+02	1.5E+01	4.8E+01					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-B01-B	1	7.50E+00	U1/2		7.50E+00	9.2E+02	1.5E+01	4.8E+01					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-B02-B	1	7.50E+00	U1/2		7.50E+00	4.7E+02	1.5E+01	4.8E+01					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-B03-B	1	7.50E+00	U1/2		7.50E+00	5.4E+02	1.5E+01	4.8E+01					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-B01-C	1	7.50E+00	U1/2		7.50E+00	8.0E+02	1.5E+01	4.8E+01					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-B02-C	1	7.50E+00	U1/2		7.50E+00	2.0E+02	1.5E+01	4.8E+01					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1313-B03-C	1	7.50E+00	U1/2		7.50E+00	4.4E+01	1.5E+01	4.8E+01					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	CFS-L07-1313-T01-A	1	2.77E+02			2.77E+02	9.9E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T02-A	1	2.92E+02			2.92E+02	1.3E+00	1.1E+00	3.5E+00	1000	100	1.25E+03	95%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T03-A	1	5.29E+02			5.29E+02	2.0E+00	1.1E+00	3.5E+00			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T04-A	1	6.67E+02			6.67E+02	5.2E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T05-A	1	1.71E+03			1.71E+03	8.9E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T06-A	1	4.17E+03			4.17E+03	6.1E-02	1.1E+00	3.5E+00			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T07-A	1	3.81E+04			3.81E+04	1.0E+00	1.1E+00	3.5E+00			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T08-A	1	6.19E+04			6.19E+04	7.3E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T09-A	1	1.69E+05			1.69E+05	1.1E+00	1.1E+00	3.5E+00			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T01-B	1	2.84E+02			2.84E+02	1.7E+00	1.1E+00	3.5E+00			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T02-B	1	2.69E+02			2.69E+02	8.6E-01	1.1E+00	3.5E+00	1000	100	1.26E+03	99%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T03-B	1	5.24E+02			5.24E+02	1.6E+00	1.1E+00	3.5E+00			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T04-B	1	5.93E+02			5.93E+02	1.6E+00	1.1E+00	3.5E+00			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T05-B	1	1.73E+03			1.73E+03	4.8E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T06-B	1	4.16E+03			4.16E+03	4.7E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T07-B	1	3.93E+04			3.93E+04	1.0E+00	1.1E+00	3.5E+00			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T08-B	1	4.55E+04			4.55E+04	5.8E+01	1.1E+00	3.5E+00			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T09-B	1	1.57E+05			1.57E+05	2.3E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T01-C	1	2.97E+02			2.97E+02	2.2E+00	1.1E+00	3.5E+00			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T02-C	1	2.91E+02			2.91E+02	2.3E+00	1.1E+00	3.5E+00	1000	100	1.22E+03	93%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T03-C	1	5.37E+02			5.37E+02	1.3E+00	1.1E+00	3.5E+00			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T04-C	1	5.85E+02			5.85E+02	5.7E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T05-C	1	1.40E+03			1.40E+03	4.8E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T06-C	1	3.98E+03			3.98E+03	2.2E+00	1.1E+00	3.5E+00			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T07-C	1	3.80E+04			3.80E+04	9.5E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T08-C	1	6.37E+04			6.37E+04	5.1E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-T09-C	1	1.51E+05			1.51E+05	4.2E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-B01-A	1	5.50E-01	U1/2		5.50E-01	2.3E+01	1.1E+00	3.5E+00					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-B02-A	1	5.43E+00			5.43E+00	5.8E+01	1.1E+00	3.5E+00					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-B03-A	1	2.29E+02			2.29E+02	2.2E+01	1.1E+00	3.5E+00					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-B01-B	1	4.16E+00			4.16E+00	1.3E+02	1.1E+00	3.5E+00					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-B02-B	1	1.23E+01			1.23E+01	8.5E+00	1.1E+00	3.5E+00					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-B03-B	1	3.35E+02			3.35E+02	7.3E+00	1.1E+00	3.5E+00					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-B01-C	1	8.38E+00			8.38E+00	1.6E+02	1.1E+00	3.5E+00					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-B02-C	1	1.26E+01			1.26E+01	2.8E+01	1.1E+00	3.5E+00					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1313-B03-C	1	3.15E+02			3.15E+02	9.7E+00	1.1E+00	3.5E+00					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	CFS-L07-1313-T01-A	1	6.22E+05			6.22E+05	1.1E-01	2.5E+00	8.0E+00			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T02-A	1	4.25E+05			4.25E+05	5.8E-02	2.5E+00	8.0E+00	1000	100	4.26E+05	85%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T03-A	1	2.47E+05			2.47E+05	4.8E-01	2.5E+00	8.0E+00			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T04-A	1	1.80E+05			1.80E+05	4.5E-01	2.5E+00	8.0E+00			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T05-A	1	1.15E+05			1.15E+05	8.3E-01	2.5E+00	8.0E+00			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T06-A	1	2.08E+04			2.08E+04	1.4E-01	2.5E+00	8.0E+00			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T07-A	1	2.39E+04			2.39E+04	6.9E-01	2.5E+00	8.0E+00			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T08-A	1	2.80E+04			2.80E+04	4.6E-01	2.5E+00	8.0E+00			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T09-A	1	3.49E+04			3.49E+04	1.6E-01	2.5E+00	8.0E+00			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T01-B	1	6.10E+05			6.10E+05	5.8E-01	2.5E+00	8.0E+00			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T02-B	1	4.21E+05			4.21E+05	4.6E-01	2.5E+00	8.0E+00	1000	100	4.21E+05	89%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T03-B	1	2.48E+05			2.48E+05	7.4E-01	2.5E+00	8.0E+00			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T04-B	1	1.84E+05			1.84E+05	1.3E-01	2.5E+00	8.0E+00			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T05-B	1	1.16E+05			1.16E+05	6.9E-01	2.5E+00	8.0E+00			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T06-B	1	2.08E+04			2.08E+04	7.3E-01	2.5E+00	8.0E+00			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T07-B	1	2.43E+04			2.43E+04	1.4E+00	2.5E+00	8.0E+00			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T08-B	1	2.13E+04			2.13E+04	6.1E+01	2.5E+00	8.0E+00			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T09-B	1	3.34E+04			3.34E+04	4.4E-01	2.5E+00	8.0E+00			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T01-C	1	6.11E+05			6.11E+05	4.4E-01	2.5E+00	8.0E+00			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T02-C	1	4.26E+05			4.26E+05	3.3E-01	2.5E+00	8.0E+00	1000	100	4.27E+05	93%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T03-C	1	2.52E+05			2.52E+05	5.9E-01	2.5E+00	8.0E+00			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T04-C	1	1.79E+05			1.79E+05	6.2E-01	2.5E+00	8.0E+00			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T05-C	1	1.20E+05			1.20E+05	7.8E-01	2.5E+00	8.0E+00			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T06-C	1	2.13E+04			2.13E+04	3.9E-01	2.5E+00	8.0E+00			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T07-C	1	2.46E+04			2.46E+04	2.5E+00	2.5E+00	8.0E+00			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T08-C	1	2.83E+04			2.83E+04	4.4E-01	2.5E+00	8.0E+00			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-T09-C	1	3.38E+04			3.38E+04	4.3E-01	2.5E+00	8.0E+00			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-B01-A	1	1.41E+01			1.41E+01	1.6E+01	2.5E+00	8.0E+00					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-B02-A	1	9.97E+00			9.97E+00	1.8E+01	2.5E+00	8.0E+00					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-B03-A	1	6.26E+05			6.26E+05	3.9E-01	2.5E+00	8.0E+00					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-B01-B	1	1.39E+01			1.39E+01	9.7E+00	2.5E+00	8.0E+00					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-B02-B	1	9.25E+00			9.25E+00	2.8E+01	2.5E+00	8.0E+00					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-B03-B	1	6.27E+05			6.27E+05	5.2E-01	2.5E+00	8.0E+00					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-B01-C	1	1.97E+01			1.97E+01	2.6E+01	2.5E+00	8.0E+00					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-B02-C	1	1.29E+01			1.29E+01	8.1E+00	2.5E+00	8.0E+00					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1313-B03-C	1	6.20E+05			6.20E+05	2.0E-01	2.5E+00	8.0E+00					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	CFS-L07-1313-T01-A	1	2.15E+03			2.15E+03	4.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T02-A	1	3.56E+03			3.56E+03	1.2E+00	1.0E+00	3.2E+00	1000	100	4.55E+03	99%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T03-A	1	3.95E+03			3.95E+03	6.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T04-A	1	3.54E+03			3.54E+03	6.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T05-A	1	3.75E+03			3.75E+03	9.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T06-A	1	1.52E+03			1.52E+03	2.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T07-A	1	1.09E+03			1.09E+03	3.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T08-A	1	1.28E+03			1.28E+03	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T09-A	1	1.43E+03			1.43E+03	1.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T01-B	1	2.10E+03			2.10E+03	4.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T02-B	1	3.52E+03			3.52E+03	2.3E-01	1.0E+00	3.2E+00	1000	100	4.49E+03	97%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T03-B	1	3.88E+03			3.88E+03	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T04-B	1	3.62E+03			3.62E+03	7.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T05-B	1	3.87E+03			3.87E+03	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T06-B	1	1.54E+03			1.54E+03	1.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T07-B	1	1.05E+03			1.05E+03	1.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T08-B	1	8.13E+02			8.13E+02	6.8E+01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T09-B	1	1.32E+03			1.32E+03	3.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T01-C	1	2.50E+03			2.50E+03	9.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T02-C	1	3.74E+03			3.74E+03	6.9E-01	1.0E+00	3.2E+00	1000	100	4.68E+03	93%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T03-C	1	4.28E+03			4.28E+03	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T04-C	1	3.51E+03			3.51E+03	1.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T05-C	1	3.66E+03			3.66E+03	1.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T06-C	1	1.52E+03			1.52E+03	1.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T07-C	1	1.09E+03			1.09E+03	3.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T08-C	1	1.20E+03			1.20E+03	9.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-T09-C	1	1.40E+03			1.40E+03	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	7.9E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.8E+02	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-B03-A	1	1.26E+00	E		1.26E+00	7.6E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	6.5E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	5.7E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	1.1E+02	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	8.2E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	1.4E+02	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1313-B03-C	1	1.16E+00	E		1.16E+00	2.8E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	CFS-L07-1313-T01-A	1	1.43E+06			1.43E+06	1.9E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T02-A	1	1.11E+06			1.11E+06	2.1E-01	6.8E+00	2.2E+01	1000	100	1.11E+06	87%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T03-A	1	8.03E+05			8.03E+05	1.4E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T04-A	1	7.24E+05			7.24E+05	6.8E-02	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T05-A	1	6.91E+05			6.91E+05	6.8E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T06-A	1	6.29E+05			6.29E+05	3.3E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T07-A	1	6.96E+05			6.96E+05	6.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T08-A	1	7.19E+05			7.19E+05	2.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T09-A	1	8.09E+05			8.09E+05	3.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T01-B	1	1.41E+06			1.41E+06	3.9E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T02-B	1	1.14E+06			1.14E+06	4.0E-01	6.8E+00	2.2E+01	1000	100	1.14E+06	82%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T03-B	1	7.88E+05			7.88E+05	6.9E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T04-B	1	7.11E+05			7.11E+05	1.0E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T05-B	1	7.11E+05			7.11E+05	5.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T06-B	1	6.25E+05			6.25E+05	7.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T07-B	1	6.79E+05			6.79E+05	7.7E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T08-B	1	5.13E+05			5.13E+05	6.6E+01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T09-B	1	8.19E+05			8.19E+05	1.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T01-C	1	1.48E+06			1.48E+06	8.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T02-C	1	1.18E+06			1.18E+06	6.7E-01	6.8E+00	2.2E+01	1000	100	1.18E+06	88%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T03-C	1	8.39E+05			8.39E+05	8.8E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T04-C	1	7.22E+05			7.22E+05	6.3E-02	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T05-C	1	7.13E+05			7.13E+05	6.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T06-C	1	6.29E+05			6.29E+05	1.8E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T07-C	1	6.94E+05			6.94E+05	2.0E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T08-C	1	7.14E+05			7.14E+05	5.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-T09-C	1	8.19E+05			8.19E+05	5.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	1.3E+01	6.8E+00	2.2E+01					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	3.0E+01	6.8E+00	2.2E+01					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-B03-A	1	3.58E+01			3.58E+01	5.5E+01	6.8E+00	2.2E+01					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-B01-B	1	3.40E+00	U1/2		3.40E+00	2.8E+01	6.8E+00	2.2E+01					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-B02-B	1	3.40E+00	U1/2		3.40E+00	1.7E+01	6.8E+00	2.2E+01					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-B03-B	1	2.63E+01			2.63E+01	3.5E+01	6.8E+00	2.2E+01					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-B01-C	1	3.40E+00	U1/2		3.40E+00	9.7E+01	6.8E+00	2.2E+01					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-B02-C	1	3.40E+00	U1/2		3.40E+00	2.0E+01	6.8E+00	2.2E+01					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1313-B03-C	1	3.40E+00	U1/2		3.40E+00	6.4E+02	6.8E+00	2.2E+01					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

TI	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	CFS-L07-1313-T01-A	1	1.16E+02			1.16E+02	4.1E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T02-A	1	9.79E+01			9.79E+01	1.3E+00	4.6E+00	1.5E+01	10	100	1.08E+03	98%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T03-A	1	1.78E+02			1.78E+02	2.7E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T04-A	1	2.65E+02			2.65E+02	3.2E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T05-A	1	3.62E+02			3.62E+02	1.6E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T06-A	1	3.56E+02			3.56E+02	2.4E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T07-A	1	7.13E+02			7.13E+02	1.9E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T08-A	1	9.42E+02			9.42E+02	4.6E-01	4.6E+00	1.5E+01			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T09-A	1	1.56E+03			1.56E+03	5.8E-01	4.6E+00	1.5E+01			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T01-B	1	1.26E+02			1.26E+02	1.2E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T02-B	1	1.13E+02			1.13E+02	4.3E+00	4.6E+00	1.5E+01	10	100	1.14E+03	103%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T03-B	1	1.77E+02			1.77E+02	4.5E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T04-B	1	2.49E+02			2.49E+02	2.2E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T05-B	1	3.65E+02			3.65E+02	2.7E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T06-B	1	3.54E+02			3.54E+02	1.8E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T07-B	1	7.30E+02			7.30E+02	6.6E-01	4.6E+00	1.5E+01			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T08-B	1	7.05E+02			7.05E+02	6.7E+01	4.6E+00	1.5E+01			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T09-B	1	1.65E+03			1.65E+03	4.8E-01	4.6E+00	1.5E+01			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T01-C	1	1.09E+02			1.09E+02	3.5E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T02-C	1	1.04E+02			1.04E+02	1.2E-01	4.6E+00	1.5E+01	10	100	1.09E+03	98%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T03-C	1	1.64E+02			1.64E+02	3.1E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T04-C	1	2.32E+02			2.32E+02	4.1E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T05-C	1	3.25E+02			3.25E+02	1.2E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T06-C	1	3.38E+02			3.38E+02	2.6E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T07-C	1	6.88E+02			6.88E+02	1.8E+00	4.6E+00	1.5E+01			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T08-C	1	9.44E+02			9.44E+02	7.0E-01	4.6E+00	1.5E+01			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-T09-C	1	1.64E+03			1.64E+03	5.3E-01	4.6E+00	1.5E+01			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	2.8E+00	4.6E+00	1.5E+01					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	2.8E+01	4.6E+00	1.5E+01					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	2.4E+01	4.6E+00	1.5E+01					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-B01-B	1	2.30E+00	U1/2		2.30E+00	1.6E+01	4.6E+00	1.5E+01					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-B02-B	1	2.30E+00	U1/2		2.30E+00	1.7E+01	4.6E+00	1.5E+01					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-B03-B	1	2.30E+00	U1/2		2.30E+00	4.9E+01	4.6E+00	1.5E+01					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-B01-C	1	2.30E+00	U1/2		2.30E+00	3.8E+01	4.6E+00	1.5E+01					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-B02-C	1	2.30E+00	U1/2		2.30E+00	2.8E+01	4.6E+00	1.5E+01					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1313-B03-C	1	2.30E+00	U1/2		2.30E+00	5.2E+01	4.6E+00	1.5E+01					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	CFS-L07-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	4.0E+01	2.0E+00	6.4E+00	10	100	1.08E+03	108%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	5.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	2.0E+02	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	2.8E+02	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	8.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T07-A	1	3.72E+00	E		3.72E+00	4.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T08-A	1	8.93E+00			8.93E+00	8.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T09-A	1	2.28E+01			2.28E+01	3.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	2.3E+02	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00	10	100	1.15E+03	115%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	3.9E+02	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	2.0E+02	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	3.3E+02	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	2.0E+02	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T07-B	1	3.31E+00	E		3.31E+00	5.5E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T08-B	1	7.28E+00			7.28E+00	6.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T09-B	1	2.46E+01			2.46E+01	1.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	5.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	1.7E+02	2.0E+00	6.4E+00	10	100	1.10E+03	109%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	8.3E+02	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	6.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	3.5E+02	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T07-C	1	3.98E+00	E		3.98E+00	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T08-C	1	9.49E+00			9.49E+00	3.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-T09-C	1	2.83E+01			2.83E+01	1.5E+00	2.0E+00	6.4E+00			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	2.0E+02	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	6.6E+01	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-B03-A	1	4.16E+00	E		4.16E+00	3.3E+00	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	8.6E+01	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	9.8E+00	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	8.0E+02	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1313-B03-C	1	1.00E+00	U1/2		1.00E+00	4.0E+01	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	CFS-L07-1313-T01-A	1	1.95E+01			1.95E+01	6.5E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T02-A	1	3.05E+01			3.05E+01	4.6E+00	1.5E+00	4.8E+00	10	100	1.13E+03	110%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T03-A	1	3.16E+01			3.16E+01	1.9E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T04-A	1	3.13E+01			3.13E+01	5.1E-01	1.5E+00	4.8E+00			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T05-A	1	3.17E+01			3.17E+01	2.6E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T06-A	1	3.28E+01			3.28E+01	6.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T07-A	1	4.70E+01			4.70E+01	3.3E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T08-A	1	5.51E+01			5.51E+01	2.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T09-A	1	5.59E+02			5.59E+02	1.0E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T01-B	1	1.82E+01			1.82E+01	6.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T02-B	1	2.99E+01			2.99E+01	4.3E+00	1.5E+00	4.8E+00	10	100	1.21E+03	118%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T03-B	1	3.13E+01			3.13E+01	1.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T04-B	1	2.96E+01			2.96E+01	6.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T05-B	1	3.28E+01			3.28E+01	3.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T06-B	1	3.32E+01			3.32E+01	2.3E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T07-B	1	4.57E+01			4.57E+01	2.3E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T08-B	1	3.70E+01			3.70E+01	6.0E+01	1.5E+00	4.8E+00			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T09-B	1	5.36E+02			5.36E+02	1.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T01-C	1	2.26E+01			2.26E+01	9.5E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T02-C	1	2.86E+01			2.86E+01	3.5E+00	1.5E+00	4.8E+00	10	100	1.15E+03	112%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T03-C	1	3.15E+01			3.15E+01	3.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T04-C	1	3.17E+01			3.17E+01	1.9E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T05-C	1	3.19E+01			3.19E+01	2.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T06-C	1	3.33E+01			3.33E+01	3.3E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T07-C	1	4.66E+01			4.66E+01	2.7E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T08-C	1	5.35E+01			5.35E+01	8.0E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-T09-C	1	5.04E+02			5.04E+02	2.9E-01	1.5E+00	4.8E+00			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-B01-A	1	7.50E-01	U1/2		7.50E-01	2.7E+02	1.5E+00	4.8E+00					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-B02-A	1	7.50E-01	U1/2		7.50E-01	4.5E+02	1.5E+00	4.8E+00					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-B03-A	1	7.50E-01	U1/2		7.50E-01	9.5E+01	1.5E+00	4.8E+00					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-B01-B	1	7.50E-01	U1/2		7.50E-01	3.0E+02	1.5E+00	4.8E+00					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-B02-B	1	7.50E-01	U1/2		7.50E-01	1.2E+02	1.5E+00	4.8E+00					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-B03-B	1	7.50E-01	U1/2		7.50E-01	2.0E+01	1.5E+00	4.8E+00					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-B01-C	1	7.50E-01	U1/2		7.50E-01	1.8E+02	1.5E+00	4.8E+00					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-B02-C	1	7.50E-01	U1/2		7.50E-01	8.3E+01	1.5E+00	4.8E+00					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1313-B03-C	1	7.50E-01	U1/2		7.50E-01	1.4E+02	1.5E+00	4.8E+00					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	CFS-L07-1313-T01-A	1	9.79E+03			9.79E+03	5.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:27 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T02-A	1	3.14E+03			3.14E+03	3.4E+00	1.0E+00	3.2E+00	10	100	4.13E+03	98%	VU ICP-OES	5/18/11 3:29 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T03-A	1	2.64E+01			2.64E+01	4.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:30 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T04-A	1	3.06E+01			3.06E+01	9.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:32 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T05-A	1	5.51E+02			5.51E+02	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:34 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T06-A	1	2.09E+04			2.09E+04	9.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:35 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T07-A	1	1.72E+05			1.72E+05	9.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:37 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T08-A	1	1.73E+05			1.73E+05	2.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:39 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T09-A	1	1.65E+05			1.65E+05	2.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:40 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T01-B	1	1.00E+04			1.00E+04	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:52 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T02-B	1	2.77E+03			2.77E+03	6.3E-01	1.0E+00	3.2E+00	10	100	3.77E+03	100%	VU ICP-OES	5/18/11 3:53 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T03-B	1	2.40E+01			2.40E+01	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:55 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T04-B	1	2.62E+01			2.62E+01	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:57 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T05-B	1	5.40E+02			5.40E+02	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 3:58 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T06-B	1	1.96E+04			1.96E+04	6.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:00 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T07-B	1	1.66E+05			1.66E+05	8.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:02 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T08-B	1	1.42E+05			1.42E+05	4.0E+01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:03 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T09-B	1	1.69E+05			1.69E+05	1.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:05 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T01-C	1	9.88E+03			9.88E+03	2.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:17 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T02-C	1	2.92E+03			2.92E+03	5.6E-01	1.0E+00	3.2E+00	10	100	3.91E+03	99%	VU ICP-OES	5/18/11 4:18 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T03-C	1	2.79E+01			2.79E+01	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:20 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T04-C	1	2.26E+01			2.26E+01	2.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:21 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T05-C	1	2.96E+02			2.96E+02	1.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:23 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T06-C	1	1.96E+04			1.96E+04	9.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:25 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T07-C	1	1.67E+05			1.67E+05	5.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:26 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T08-C	1	1.75E+05			1.75E+05	2.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:28 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-T09-C	1	1.61E+05			1.61E+05	3.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/18/11 4:30 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	7.5E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:22 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-B02-A	1	1.29E+00	E		1.29E+00	2.1E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:24 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-B03-A	1	6.60E+00			6.60E+00	8.0E+00	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:25 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-B01-B	1	3.35E+00			3.35E+00	8.0E+00	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:47 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-B02-B	1	1.38E+00	E		1.38E+00	3.7E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:49 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-B03-B	1	7.67E+00			7.67E+00	4.9E+00	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 3:50 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-B01-C	1	3.17E+00	E		3.17E+00	8.2E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:12 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-B02-C	1	2.36E+00	E		2.36E+00	1.0E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:13 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1313-B03-C	1	8.70E+00			8.70E+00	1.7E+00	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:15 PM	EPA Interlab L07 1313-1316 CFS

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	CFS-L09-1313-T01-A	1	9.59E+01			9.59E+01	3.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T02-A	1	1.11E+02			1.11E+02	2.8E+00	1.0E+00	3.2E+00	1000	100	1.20E+03	109%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T03-A	1	1.16E+02			1.16E+02	2.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T04-A	1	5.49E+01			5.49E+01	4.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T05-A	1	4.51E+01			4.51E+01	6.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T06-A	1	5.74E+01			5.74E+01	4.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T07-A	1	8.11E+03			8.11E+03	3.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T08-A	1	3.68E+04			3.68E+04	9.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T09-A	1	9.09E+04			9.09E+04	3.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T01-B	1	1.21E+02			1.21E+02	6.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T02-B	1	9.87E+01			9.87E+01	1.1E+00	1.0E+00	3.2E+00	1000	100	1.16E+03	106%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T03-B	1	9.20E+01			9.20E+01	3.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T04-B	1	5.79E+01			5.79E+01	2.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T05-B	1	4.69E+01			4.69E+01	6.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T06-B	1	6.52E+01			6.52E+01	2.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T07-B	1	2.21E+04			2.21E+04	6.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T08-B	1	2.12E+04			2.12E+04	7.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T09-B	1	9.39E+04			9.39E+04	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T01-C	1	9.78E+01			9.78E+01	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T02-C	1	1.00E+02			1.00E+02	1.7E+00	1.0E+00	3.2E+00	1000	100	1.16E+03	106%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T03-C	1	1.07E+02			1.07E+02	1.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T04-C	1	5.91E+01			5.91E+01	8.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T05-C	1	4.87E+01			4.87E+01	6.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T06-C	1	5.87E+01			5.87E+01	5.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T07-C	1	2.03E+03			2.03E+03	3.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T08-C	1	3.56E+04			3.56E+04	9.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-T09-C	1	9.01E+04			9.01E+04	2.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.1E+02	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-B02-A	1	9.06E+01			9.06E+01	3.6E+00	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1313-B03-A	1	3.28E+00			3.28E+00	7.9E+01	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	CFS-L09-1313-T01-A	1	3.75E+00	U1/2		3.75E+00	1.0E+02	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T02-A	1	1.91E+01	E		1.91E+01	4.9E+01	7.5E+00	2.4E+01	10	100	1.02E+03	100%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T03-A	1	2.83E+01			2.83E+01	1.9E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T04-A	1	2.98E+01			2.98E+01	1.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T05-A	1	3.34E+01			3.34E+01	2.4E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T06-A	1	4.32E+01			4.32E+01	9.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T07-A	1	2.36E+02			2.36E+02	3.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T08-A	1	1.07E+03			1.07E+03	4.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T09-A	1	1.56E+03			1.56E+03	6.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T01-B	1	1.79E+01	E		1.79E+01	4.8E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T02-B	1	3.75E+00	U1/2		3.75E+00	9.2E+01	7.5E+00	2.4E+01	10	100	9.80E+02	98%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T03-B	1	2.71E+01			2.71E+01	3.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T04-B	1	3.61E+01			3.61E+01	2.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T05-B	1	2.73E+01			2.73E+01	2.9E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T06-B	1	4.84E+01			4.84E+01	8.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T07-B	1	6.49E+02			6.49E+02	8.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T08-B	1	6.53E+02			6.53E+02	9.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T09-B	1	1.77E+03			1.77E+03	4.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T01-C	1	1.05E+01	E		1.05E+01	1.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T02-C	1	1.26E+01	E		1.26E+01	8.3E+01	7.5E+00	2.4E+01	10	100	1.10E+03	109%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T03-C	1	3.32E+01			3.32E+01	7.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T04-C	1	3.96E+01			3.96E+01	2.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T05-C	1	4.67E+01			4.67E+01	1.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T06-C	1	4.50E+01			4.50E+01	1.4E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T07-C	1	8.24E+01			8.24E+01	9.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T08-C	1	1.11E+03			1.11E+03	1.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-T09-C	1	1.79E+03			1.79E+03	4.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-B01-A	1	3.75E+00	U1/2		3.75E+00	8.3E+01	7.5E+00	2.4E+01					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-B02-A	1	7.75E+00	E		7.75E+00	5.2E+01	7.5E+00	2.4E+01					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1313-B03-A	1	3.38E+01			3.38E+01	4.7E+01	7.5E+00	2.4E+01					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	CFS-L09-1313-T01-A	1	2.31E+02			2.31E+02	7.7E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T02-A	1	1.44E+02			1.44E+02	1.0E+01	1.1E+01	3.5E+01	10	100	1.19E+03	104%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T03-A	1	9.52E+01			9.52E+01	1.0E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T04-A	1	3.46E+01	E		3.46E+01	1.9E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T05-A	1	1.14E+01	E		1.14E+01	3.7E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T06-A	1	2.70E+01	E		2.70E+01	1.7E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T07-A	1	2.28E+02			2.28E+02	4.6E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T08-A	1	1.58E+03			1.58E+03	4.6E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T09-A	1	1.09E+05			1.09E+05	1.5E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T01-B	1	5.45E+02			5.45E+02	1.3E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T02-B	1	2.20E+02			2.20E+02	5.9E+00	1.1E+01	3.5E+01	10	100	1.25E+03	103%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T03-B	1	9.30E+01			9.30E+01	3.1E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T04-B	1	3.18E+01	E		3.18E+01	3.0E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T05-B	1	1.12E+01	E		1.12E+01	4.5E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T06-B	1	3.27E+01	E		3.27E+01	2.1E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T07-B	1	4.91E+02			4.91E+02	2.3E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T08-B	1	5.09E+02			5.09E+02	2.7E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T09-B	1	1.31E+05			1.31E+05	5.6E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T01-C	1	1.57E+02			1.57E+02	6.9E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T02-C	1	2.33E+02			2.33E+02	2.9E+00	1.1E+01	3.5E+01	10	100	1.34E+03	111%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T03-C	1	7.82E+01			7.82E+01	1.4E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T04-C	1	3.60E+01			3.60E+01	2.6E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T05-C	1	3.04E+01	E		3.04E+01	1.0E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T06-C	1	3.05E+01	E		3.05E+01	9.6E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T07-C	1	9.35E+01			9.35E+01	5.3E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T08-C	1	1.34E+03			1.34E+03	9.2E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-T09-C	1	1.40E+05			1.40E+05	2.0E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-B01-A	1	5.50E+00	U1/2		5.50E+00	9.1E+01	1.1E+01	3.5E+01					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-B02-A	1	5.50E+00	U1/2		5.50E+00	1.4E+02	1.1E+01	3.5E+01					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1313-B03-A	1	1.52E+01	E		1.52E+01	3.4E+01	1.1E+01	3.5E+01					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	CFS-L09-1313-T01-A	1	4.86E+01			4.86E+01	2.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T02-A	1	8.61E+01			8.61E+01	6.4E-01	1.0E+00	3.2E+00	1000	100	1.12E+03	103%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T03-A	1	1.49E+02			1.49E+02	1.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T04-A	1	1.22E+02			1.22E+02	1.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T05-A	1	1.49E+02			1.49E+02	6.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T06-A	1	1.97E+02			1.97E+02	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T07-A	1	3.91E+02			3.91E+02	2.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T08-A	1	6.28E+02			6.28E+02	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T09-A	1	7.30E+02			7.30E+02	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T01-B	1	5.69E+01			5.69E+01	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T02-B	1	4.78E+01			4.78E+01	6.5E-01	1.0E+00	3.2E+00	1000	100	1.05E+03	100%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T03-B	1	1.69E+02			1.69E+02	7.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T04-B	1	1.17E+02			1.17E+02	7.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T05-B	1	1.42E+02			1.42E+02	5.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T06-B	1	1.95E+02			1.95E+02	1.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T07-B	1	5.51E+02			5.51E+02	1.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T08-B	1	5.52E+02			5.52E+02	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T09-B	1	7.20E+02			7.20E+02	2.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T01-C	1	6.57E+01			6.57E+01	2.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T02-C	1	5.56E+01			5.56E+01	2.8E+00	1.0E+00	3.2E+00	1000	100	1.14E+03	108%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T03-C	1	1.56E+02			1.56E+02	7.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T04-C	1	1.21E+02			1.21E+02	2.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T05-C	1	1.61E+02			1.61E+02	2.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T06-C	1	1.97E+02			1.97E+02	1.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T07-C	1	3.00E+02			3.00E+02	2.5E-03	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T08-C	1	5.93E+02			5.93E+02	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-T09-C	1	7.48E+02			7.48E+02	3.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-B01-A	1	1.76E+01			1.76E+01	1.8E+00	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-B02-A	1	2.10E+01			2.10E+01	4.0E+00	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1313-B03-A	1	1.65E+01			1.65E+01	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	CFS-L09-1313-T01-A	1	9.59E+00			9.59E+00	3.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/17/11 11:03 AM	EPA Interlab 1313-1316 CFS Reruns
Ba	CFS-L09-1313-T02-A	1	1.53E+01			1.53E+01	7.7E-01	1.0E+00	3.2E+00	10	100	1.10E+03	108%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-T03-A	1	1.90E+02			1.90E+02	4.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-T04-A	1	9.53E+01			9.53E+01	7.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-T05-A	1	1.17E+02			1.17E+02	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-T06-A	1	7.31E+01			7.31E+01	1.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-T07-A	1	2.83E+01			2.83E+01	2.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-T08-A	1	4.28E+01			4.28E+01	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-T09-A	1	6.14E+00			6.14E+00	3.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-T01-B	1	5.93E+00			5.93E+00	4.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/17/11 11:24 AM	EPA Interlab 1313-1316 CFS Reruns
Ba	CFS-L09-1313-T02-B	1	7.04E+00			7.04E+00	2.5E+00	1.0E+00	3.2E+00	10	100	9.94E+02	99%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-T03-B	1	1.32E+02			1.32E+02	3.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-T04-B	1	9.53E+01			9.53E+01	6.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-T05-B	1	1.13E+02			1.13E+02	4.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-T06-B	1	6.78E+01			6.78E+01	2.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-T07-B	1	3.37E+01			3.37E+01	7.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-T08-B	1	3.33E+01			3.33E+01	7.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-T09-B	1	6.91E+00			6.91E+00	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-T01-C	1	7.29E+01			7.29E+01	3.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	6/17/11 11:45 AM	EPA Interlab 1313-1316 CFS Reruns
Ba	CFS-L09-1313-T02-C	1	6.78E+00			6.78E+00	9.2E+00	1.0E+00	3.2E+00	10	100	9.89E+02	98%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-T03-C	1	1.78E+02			1.78E+02	2.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-T04-C	1	1.01E+02			1.01E+02	3.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-T05-C	1	1.25E+02			1.25E+02	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-T06-C	1	7.66E+01			7.66E+01	6.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-T07-C	1	4.18E+01			4.18E+01	3.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-T08-C	1	4.21E+01			4.21E+01	9.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-T09-C	1	7.09E+00			7.09E+00	3.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	2.4E+01	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	2.0E+00	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	1.8E+02	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	CFS-L09-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	4.7E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	6.8E+01	1.9E+00	6.0E+00	10	100	1.05E+03	105%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	4.5E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	3.5E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	2.0E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T07-A	1	3.79E+00	E		3.79E+00	5.3E-01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T08-A	1	6.79E+00			6.79E+00	7.0E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T09-A	1	9.50E-01	U1/2		9.50E-01	1.2E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	1.0E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	1.2E+01	1.9E+00	6.0E+00	10	100	1.04E+03	104%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	6.1E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	1.4E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	4.1E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T07-B	1	5.86E+00	E		5.86E+00	6.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T08-B	1	5.65E+00	E		5.65E+00	4.0E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T09-B	1	9.50E-01	U1/2		9.50E-01	6.5E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	5.3E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	5.5E+01	1.9E+00	6.0E+00	10	100	1.05E+03	105%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	2.7E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	4.3E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	9.3E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T07-C	1	2.11E+00	E		2.11E+00	2.9E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T08-C	1	6.25E+00			6.25E+00	6.6E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-T09-C	1	9.50E-01	U1/2		9.50E-01	5.0E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	5.2E+01	1.9E+00	6.0E+00					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	5.2E+01	1.9E+00	6.0E+00					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	2.7E+01	1.9E+00	6.0E+00					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	CFS-L09-1313-T01-A	1	1.06E+01			1.06E+01	3.3E+00	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T02-A	1	1.10E+00	U1/2		1.10E+00	1.7E+01	2.2E+00	7.0E+00	10	100	1.02E+03	101%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	1.6E+01	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T04-A	1	5.00E+01			5.00E+01	4.2E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T05-A	1	4.42E+03			4.42E+03	7.1E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T06-A	1	9.83E+03			9.83E+03	6.0E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T07-A	1	3.01E+04			3.01E+04	3.9E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T08-A	1	4.57E+04			4.57E+04	7.8E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T09-A	1	4.31E+04			4.31E+04	1.0E+00	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T01-B	1	1.63E+01			1.63E+01	1.7E+00	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T02-B	1	1.06E+01			1.06E+01	2.4E+00	2.2E+00	7.0E+00	10	100	9.64E+02	95%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	8.2E+00	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T04-B	1	4.77E+01			4.77E+01	9.0E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T05-B	1	3.98E+03			3.98E+03	4.4E-02	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T06-B	1	1.00E+04			1.00E+04	6.2E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T07-B	1	4.14E+04			4.14E+04	2.0E+00	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T08-B	1	4.19E+04			4.19E+04	4.6E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T09-B	1	4.50E+04			4.50E+04	1.0E+00	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T01-C	1	4.13E+00	E		4.13E+00	9.9E+00	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T02-C	1	1.21E+01			1.21E+01	2.7E+00	2.2E+00	7.0E+00	10	100	1.07E+03	106%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T03-C	1	2.29E+00	E		2.29E+00	1.6E+00	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T04-C	1	4.33E+01			4.33E+01	1.7E+00	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T05-C	1	4.76E+03			4.76E+03	5.4E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T06-C	1	1.00E+04			1.00E+04	5.2E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T07-C	1	2.07E+04			2.07E+04	4.4E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T08-C	1	4.30E+04			4.30E+04	7.6E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-T09-C	1	4.17E+04			4.17E+04	4.1E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	8.2E+01	2.2E+00	7.0E+00					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	3.1E+01	2.2E+00	7.0E+00					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1313-B03-A	1	1.10E+00	U1/2		1.10E+00	1.1E+02	2.2E+00	7.0E+00					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	CFS-L09-1313-T01-A	1	5.08E+05			5.08E+05	9.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T02-A	1	5.55E+05			5.55E+05	2.8E-01	2.6E+00	8.3E+00	1000	100	5.55E+05	92%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T03-A	1	5.44E+05			5.44E+05	3.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T04-A	1	6.28E+05			6.28E+05	9.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T05-A	1	6.74E+05			6.74E+05	7.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T06-A	1	7.21E+05			7.21E+05	7.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T07-A	1	9.52E+05			9.52E+05	5.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T08-A	1	1.25E+06			1.25E+06	9.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T09-A	1	1.61E+06			1.61E+06	4.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T01-B	1	2.96E+05			2.96E+05	3.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T02-B	1	5.15E+05			5.15E+05	2.8E-01	2.6E+00	8.3E+00	1000	100	5.16E+05	85%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T03-B	1	5.80E+05			5.80E+05	2.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T04-B	1	6.30E+05			6.30E+05	3.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T05-B	1	6.33E+05			6.33E+05	3.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T06-B	1	7.32E+05			7.32E+05	7.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T07-B	1	1.12E+06			1.12E+06	4.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T08-B	1	1.12E+06			1.12E+06	6.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T09-B	1	1.61E+06			1.61E+06	4.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T01-C	1	3.03E+05			3.03E+05	8.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T02-C	1	5.21E+05			5.21E+05	1.4E+00	2.6E+00	8.3E+00	1000	100	5.22E+05	90%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T03-C	1	6.07E+05			6.07E+05	9.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T04-C	1	6.32E+05			6.32E+05	7.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T05-C	1	6.83E+05			6.83E+05	5.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T06-C	1	7.27E+05			7.27E+05	7.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T07-C	1	8.51E+05			8.51E+05	3.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T08-C	1	1.21E+06			1.21E+06	2.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-T09-C	1	1.53E+06			1.53E+06	6.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-B01-A	1	3.07E+01			3.07E+01	6.9E+00	2.6E+00	8.3E+00					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-B02-A	1	9.20E+01			9.20E+01	1.2E+01	2.6E+00	8.3E+00					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1313-B03-A	1	4.04E+01			4.04E+01	6.7E+00	2.6E+00	8.3E+00					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	CFS-L09-1313-T01-A	1	1.11E+02			1.11E+02	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T02-A	1	4.41E+01			4.41E+01	9.4E-01	1.2E+00	3.8E+00	10	100	1.05E+03	101%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T03-A	1	6.41E+00			6.41E+00	3.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T04-A	1	6.00E-01	U1/2		6.00E-01	7.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T05-A	1	6.00E-01	U1/2		6.00E-01	1.7E+03	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T06-A	1	6.00E-01	U1/2		6.00E-01	2.6E+03	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T07-A	1	6.00E-01	U1/2		6.00E-01	1.4E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T08-A	1	6.78E+01			6.78E+01	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T09-A	1	2.35E+03			2.35E+03	8.2E-02	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T01-B	1	1.45E+02			1.45E+02	3.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T02-B	1	1.34E+02			1.34E+02	1.3E-01	1.2E+00	3.8E+00	10	100	1.08E+03	94%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T03-B	1	8.04E+00			8.04E+00	6.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T04-B	1	6.00E-01	U1/2		6.00E-01	7.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T05-B	1	6.00E-01	U1/2		6.00E-01	2.3E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T06-B	1	6.00E-01	U1/2		6.00E-01	3.1E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T07-B	1	1.60E+01			1.60E+01	3.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T08-B	1	1.52E+01			1.52E+01	5.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T09-B	1	2.25E+03			2.25E+03	7.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T01-C	1	4.27E+01			4.27E+01	3.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T02-C	1	1.37E+02			1.37E+02	2.2E+00	1.2E+00	3.8E+00	10	100	1.17E+03	104%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T03-C	1	5.71E+00			5.71E+00	1.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T04-C	1	6.00E-01	U1/2		6.00E-01	5.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T05-C	1	6.00E-01	U1/2		6.00E-01	1.4E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T06-C	1	6.00E-01	U1/2		6.00E-01	1.4E+03	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T07-C	1	6.00E-01	U1/2		6.00E-01	2.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T08-C	1	7.47E+01			7.47E+01	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-T09-C	1	2.18E+03			2.18E+03	3.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	5.7E+02	1.2E+00	3.8E+00					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	3.9E+01	1.2E+00	3.8E+00					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1313-B03-A	1	6.00E-01	U1/2		6.00E-01	7.8E+01	1.2E+00	3.8E+00					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	CFS-L09-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	7.9E+01	1.8E+00	5.7E+00	10	100	9.82E+02	98%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T05-A	1	9.60E+01			9.60E+01	1.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T06-A	1	2.10E+02			2.10E+02	7.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T07-A	1	8.74E+02			8.74E+02	2.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T08-A	1	1.56E+03			1.56E+03	2.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T09-A	1	1.67E+03			1.67E+03	1.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	1.9E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T02-B	1	2.13E+00	E		2.13E+00	2.9E+01	1.8E+00	5.7E+00	10	100	9.24E+02	92%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	3.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	3.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T05-B	1	8.49E+01			8.49E+01	6.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T06-B	1	2.09E+02			2.09E+02	2.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T07-B	1	1.38E+03			1.38E+03	4.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T08-B	1	1.40E+03			1.40E+03	8.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T09-B	1	1.69E+03			1.69E+03	1.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T01-C	1	2.34E+00	E		2.34E+00	1.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	3.1E+01	1.8E+00	5.7E+00	10	100	1.02E+03	102%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	8.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T05-C	1	1.08E+02			1.08E+02	2.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T06-C	1	2.11E+02			2.11E+02	6.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T07-C	1	4.68E+02			4.68E+02	7.6E-02	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T08-C	1	1.47E+03			1.47E+03	2.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-T09-C	1	1.59E+03			1.59E+03	2.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	7.1E+01	1.8E+00	5.7E+00					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	2.9E+01	1.8E+00	5.7E+00					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	1.8E+02	1.8E+00	5.7E+00					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	CFS-L09-1313-T01-A	1	7.19E+03			7.19E+03	1.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T02-A	1	6.45E+02			6.45E+02	8.4E-01	3.7E+00	1.2E+01	10	100	1.61E+03	96%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T03-A	1	1.35E+02			1.35E+02	2.9E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T04-A	1	4.94E+01			4.94E+01	1.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T05-A	1	8.24E+02			8.24E+02	4.6E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T06-A	1	7.68E+03			7.68E+03	4.2E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T07-A	1	3.98E+05			3.98E+05	1.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T08-A	1	8.81E+05			8.81E+05	1.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T09-A	1	1.00E+06			1.00E+06	7.7E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T01-B	1	1.17E+04			1.17E+04	2.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T02-B	1	6.99E+03			6.99E+03	1.0E+00	3.7E+00	1.2E+01	10	100	7.87E+03	88%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T03-B	1	2.20E+02			2.20E+02	1.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T04-B	1	5.30E+01			5.30E+01	3.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T05-B	1	6.71E+02			6.71E+02	2.6E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T06-B	1	8.32E+03			8.32E+03	1.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T07-B	1	7.81E+05			7.81E+05	9.1E-02	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T08-B	1	7.78E+05			7.78E+05	1.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T09-B	1	1.00E+06			1.00E+06	8.5E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T01-C	1	4.23E+03			4.23E+03	3.8E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T02-C	1	7.34E+03			7.34E+03	2.3E+00	3.7E+00	1.2E+01	10	100	8.30E+03	97%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T03-C	1	1.29E+02			1.29E+02	2.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T04-C	1	5.70E+01			5.70E+01	1.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T05-C	1	9.78E+02			9.78E+02	1.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T06-C	1	7.46E+03			7.46E+03	1.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T07-C	1	1.21E+05			1.21E+05	7.3E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T08-C	1	8.44E+05			8.44E+05	1.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-T09-C	1	9.45E+05			9.45E+05	1.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	1.7E+02	3.7E+00	1.2E+01					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	4.1E+01	3.7E+00	1.2E+01					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1313-B03-A	1	1.85E+00	U1/2		1.85E+00	3.2E+01	3.7E+00	1.2E+01					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	CFS-L09-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00	1000	100	1.05E+03	105%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	5.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	4.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	5.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	2.6E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T07-A	1	8.27E+00			8.27E+00	7.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T08-A	1	5.60E+04			5.60E+04	4.4E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T09-A	1	3.15E+05			3.15E+05	3.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T01-B	1	2.23E+00	E		2.23E+00	2.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T02-B	1	1.38E+02			1.38E+02	2.2E-01	2.0E+00	6.4E+00	1000	100	1.13E+03	99%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	4.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	6.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T05-B	1	3.58E+00	E		3.58E+00	1.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T07-B	1	7.29E+03			7.29E+03	6.1E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T08-B	1	6.45E+03			6.45E+03	5.5E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T09-B	1	3.28E+05			3.28E+05	3.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T01-C	1	8.13E+00			8.13E+00	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T02-C	1	2.45E+00	E		2.45E+00	2.2E+01	2.0E+00	6.4E+00	1000	100	1.08E+03	107%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	3.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	3.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	7.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T07-C	1	3.81E+00	E		3.81E+00	7.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T08-C	1	4.70E+04			4.70E+04	1.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-T09-C	1	3.43E+05			3.43E+05	3.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-B02-A	1	4.71E+01			4.71E+01	1.2E+00	2.0E+00	6.4E+00					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1313-B03-A	1	4.63E+00	E		4.63E+00	7.9E+00	2.0E+00	6.4E+00					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	CFS-L09-1313-T01-A	1	3.09E+03			3.09E+03	1.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T02-A	1	1.38E+04			1.38E+04	6.3E-01	6.8E+00	2.2E+01	10	100	1.48E+04	102%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T03-A	1	9.18E+02			9.18E+02	3.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T04-A	1	1.45E+02			1.45E+02	3.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T05-A	1	1.16E+03			1.16E+03	6.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T06-A	1	1.76E+03			1.76E+03	1.3E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T07-A	1	6.63E+03			6.63E+03	9.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T08-A	1	5.97E+03			5.97E+03	4.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T09-A	1	9.58E+03			9.58E+03	1.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T01-B	1	5.67E+03			5.67E+03	7.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T02-B	1	2.76E+04			2.76E+04	4.2E-01	6.8E+00	2.2E+01	10	100	2.86E+04	99%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T03-B	1	3.47E+02			3.47E+02	8.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T04-B	1	1.46E+02			1.46E+02	2.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T05-B	1	1.09E+03			1.09E+03	2.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T06-B	1	1.84E+03			1.84E+03	2.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T07-B	1	5.07E+03			5.07E+03	7.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T08-B	1	5.43E+03			5.43E+03	9.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T09-B	1	1.18E+04			1.18E+04	7.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T01-C	1	8.30E+03			8.30E+03	1.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T02-C	1	5.15E+03			5.15E+03	1.5E+00	6.8E+00	2.2E+01	10	100	6.18E+03	103%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T03-C	1	5.54E+02			5.54E+02	3.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T04-C	1	1.49E+02			1.49E+02	3.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T05-C	1	1.28E+03			1.28E+03	8.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T06-C	1	1.79E+03			1.79E+03	1.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T07-C	1	5.91E+03			5.91E+03	7.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T08-C	1	5.88E+03			5.88E+03	1.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-T09-C	1	1.43E+04			1.43E+04	8.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	1.6E+01	6.8E+00	2.2E+01					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	2.1E+02	6.8E+00	2.2E+01					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	2.3E+02	6.8E+00	2.2E+01					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	CFS-L09-1313-T01-A	1	1.12E+01			1.12E+01	4.6E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T02-A	1	1.05E+01			1.05E+01	1.6E+01	1.9E+00	6.0E+00	10	100	8.91E+02	88%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T03-A	1	1.28E+01			1.28E+01	2.3E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T04-A	1	9.83E+00			9.83E+00	2.3E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T05-A	1	8.29E+00			8.29E+00	2.3E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T06-A	1	7.23E+00			7.23E+00	8.0E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T07-A	1	8.31E+00			8.31E+00	3.6E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T08-A	1	2.18E+01			2.18E+01	3.2E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T09-A	1	6.70E+01			6.70E+01	5.0E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T01-B	1	8.22E+00			8.22E+00	3.3E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T02-B	1	1.25E+01			1.25E+01	1.0E+01	1.9E+00	6.0E+00	10	100	8.99E+02	89%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T03-B	1	1.13E+01			1.13E+01	8.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T04-B	1	1.01E+01			1.01E+01	1.6E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T05-B	1	1.00E+01			1.00E+01	3.3E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T06-B	1	9.50E+00			9.50E+00	9.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T07-B	1	1.07E+01			1.07E+01	2.4E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T08-B	1	1.03E+01			1.03E+01	1.1E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T09-B	1	6.55E+01			6.55E+01	2.1E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T01-C	1	9.86E+00			9.86E+00	3.9E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T02-C	1	1.05E+01			1.05E+01	1.3E+01	1.9E+00	6.0E+00	10	100	9.03E+02	89%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T03-C	1	1.11E+01			1.11E+01	2.6E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T04-C	1	1.06E+01			1.06E+01	2.2E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T05-C	1	9.06E+00			9.06E+00	5.7E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T06-C	1	1.01E+01			1.01E+01	2.5E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T07-C	1	8.32E+00			8.32E+00	1.9E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T08-C	1	1.37E+01			1.37E+01	3.0E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-T09-C	1	7.06E+01			7.06E+01	1.6E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-B01-A	1	2.56E+00	E		2.56E+00	5.0E+00	1.9E+00	6.0E+00					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	5.9E+02	1.9E+00	6.0E+00					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	4.8E+02	1.9E+00	6.0E+00					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	CFS-L09-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	1.9E+02	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	9.8E+00	2.0E+00	6.4E+00	10	100	9.58E+02	96%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T04-A	1	1.08E+01			1.08E+01	3.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T05-A	1	1.50E+03			1.50E+03	9.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T06-A	1	2.58E+03			2.58E+03	8.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T07-A	1	8.62E+03			8.62E+03	1.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T08-A	1	2.11E+04			2.11E+04	9.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T09-A	1	3.40E+04			3.40E+04	4.8E-02	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	2.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	2.1E+00	2.0E+00	6.4E+00	10	100	9.04E+02	90%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T04-B	1	1.04E+01			1.04E+01	1.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T05-B	1	1.38E+03			1.38E+03	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T06-B	1	2.59E+03			2.59E+03	7.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T07-B	1	1.66E+04			1.66E+04	8.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T08-B	1	1.68E+04			1.68E+04	9.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T09-B	1	3.47E+04			3.47E+04	8.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	6.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	2.1E+01	2.0E+00	6.4E+00	10	100	9.94E+02	99%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	4.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T04-C	1	9.55E+00			9.55E+00	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T05-C	1	1.75E+03			1.75E+03	1.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T06-C	1	2.58E+03			2.58E+03	6.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T07-C	1	4.82E+03			4.82E+03	9.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T08-C	1	1.97E+04			1.97E+04	1.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-T09-C	1	3.19E+04			3.19E+04	9.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.3E+01	2.0E+00	6.4E+00					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	6.6E+00	2.0E+00	6.4E+00					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	5.5E+01	2.0E+00	6.4E+00					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	CFS-L09-1313-T01-A	1	2.01E+01			2.01E+01	4.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T02-A	1	4.15E+01			4.15E+01	6.3E+00	1.0E+00	3.2E+00	1000	100	1.01E+03	97%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T03-A	1	7.67E+02			7.67E+02	2.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T04-A	1	5.06E+04			5.06E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T05-A	1	6.37E+04			6.37E+04	6.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T06-A	1	7.24E+04			7.24E+04	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T07-A	1	7.72E+04			7.72E+04	4.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T08-A	1	1.43E+05			1.43E+05	8.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T09-A	1	2.16E+05			2.16E+05	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T01-B	1	2.69E+01			2.69E+01	3.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T02-B	1	2.76E+01			2.76E+01	2.2E+01	1.0E+00	3.2E+00	1000	100	9.08E+02	88%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T03-B	1	1.42E+03			1.42E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T04-B	1	4.90E+04			4.90E+04	4.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T05-B	1	6.28E+04			6.28E+04	5.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T06-B	1	7.08E+04			7.08E+04	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T07-B	1	9.96E+04			9.96E+04	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T08-B	1	1.06E+05			1.06E+05	3.0E-02	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T09-B	1	2.14E+05			2.14E+05	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T01-C	1	1.43E+01			1.43E+01	7.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T02-C	1	1.35E+01			1.35E+01	8.8E+01	1.0E+00	3.2E+00	1000	100	9.98E+02	98%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T03-C	1	2.43E+03			2.43E+03	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T04-C	1	5.33E+04			5.33E+04	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T05-C	1	6.88E+04			6.88E+04	1.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T06-C	1	7.17E+04			7.17E+04	6.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T07-C	1	7.88E+04			7.88E+04	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T08-C	1	1.31E+05			1.31E+05	7.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-T09-C	1	1.97E+05			1.97E+05	8.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	5.3E+03	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-B02-A	1	2.14E+01			2.14E+01	2.4E+01	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1313-B03-A	1	1.55E+01			1.55E+01	4.2E+01	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	CFS-L09-1313-T01-A	1	1.37E+03			1.37E+03	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T02-A	1	1.43E+03			1.43E+03	9.9E-02	1.2E+00	3.8E+00	10	100	2.37E+03	93%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T03-A	1	9.38E+02			9.38E+02	2.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T04-A	1	1.97E+02			1.97E+02	8.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T05-A	1	9.92E+00			9.92E+00	1.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T06-A	1	9.22E+00			9.22E+00	1.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T07-A	1	7.49E+00			7.49E+00	2.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T08-A	1	1.83E+01			1.83E+01	1.1E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T09-A	1	2.49E+02			2.49E+02	8.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T01-B	1	1.87E+03			1.87E+03	3.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T02-B	1	1.41E+03			1.41E+03	4.9E-01	1.2E+00	3.8E+00	10	100	2.31E+03	90%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T03-B	1	1.00E+03			1.00E+03	2.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T04-B	1	1.95E+02			1.95E+02	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T05-B	1	9.47E+00			9.47E+00	7.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T06-B	1	8.13E+00			8.13E+00	9.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T07-B	1	1.78E+01			1.78E+01	9.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T08-B	1	1.00E+01			1.00E+01	2.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T09-B	1	3.52E+02			3.52E+02	6.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T01-C	1	1.07E+03			1.07E+03	2.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T02-C	1	1.36E+03			1.36E+03	1.3E+00	1.2E+00	3.8E+00	10	100	2.28E+03	92%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T03-C	1	9.83E+02			9.83E+02	6.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T04-C	1	2.04E+02			2.04E+02	9.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T05-C	1	9.53E+00			9.53E+00	6.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T06-C	1	8.99E+00			8.99E+00	2.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T07-C	1	4.14E+00			4.14E+00	4.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T08-C	1	9.62E+00			9.62E+00	2.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-T09-C	1	4.95E+02			4.95E+02	1.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	4.1E+01	1.2E+00	3.8E+00					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-B02-A	1	1.60E+00	E		1.60E+00	1.4E+01	1.2E+00	3.8E+00					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1313-B03-A	1	4.94E+00			4.94E+00	1.8E+01	1.2E+00	3.8E+00					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	CFS-L09-1313-T01-A	1	1.81E+00	E		1.81E+00	3.4E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	1.9E+02	1.8E+00	5.7E+00	10	100	9.84E+02	98%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T03-A	1	2.60E+00	E		2.60E+00	1.1E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T04-A	1	3.19E+00	E		3.19E+00	1.7E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T05-A	1	2.05E+02			2.05E+02	1.9E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T06-A	1	5.79E+02			5.79E+02	6.7E-02	1.8E+00	5.7E+00			---		VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T07-A	1	3.31E+03			3.31E+03	7.9E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T08-A	1	5.72E+03			5.72E+03	2.0E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T09-A	1	6.40E+03			6.40E+03	3.2E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T01-B	1	4.68E+00	E		4.68E+00	9.2E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T02-B	1	6.23E+00			6.23E+00	1.2E+01	1.8E+00	5.7E+00	10	100	9.17E+02	91%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	5.7E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T04-B	1	3.06E+00	E		3.06E+00	6.5E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T05-B	1	1.76E+02			1.76E+02	2.2E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T06-B	1	5.80E+02			5.80E+02	2.1E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T07-B	1	5.22E+03			5.22E+03	6.2E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T08-B	1	5.39E+03			5.39E+03	9.7E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T09-B	1	6.17E+03			6.17E+03	3.5E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	7.7E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T02-C	1	2.80E+00	E		2.80E+00	6.4E+01	1.8E+00	5.7E+00	10	100	1.01E+03	101%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00			---		VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T04-C	1	4.54E+00	E		4.54E+00	2.3E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T05-C	1	2.34E+02			2.34E+02	1.6E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T06-C	1	5.67E+02			5.67E+02	9.9E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T07-C	1	1.60E+03			1.60E+03	5.3E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T08-C	1	5.51E+03			5.51E+03	1.0E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-T09-C	1	6.03E+03			6.03E+03	1.4E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	1.6E+01	1.8E+00	5.7E+00					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.8E+00	5.7E+00					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1313-B03-A	1	2.59E+00	E		2.59E+00	9.1E+01	1.8E+00	5.7E+00					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	CFS-L09-1313-T01-A	1	5.77E+01			5.77E+01	7.9E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T02-A	1	6.21E+01			6.21E+01	1.1E+01	3.7E+00	1.2E+01	1000	100	1.15E+03	109%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T03-A	1	4.45E+01			4.45E+01	1.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T04-A	1	3.27E+01			3.27E+01	2.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T05-A	1	1.85E+00	U1/2		1.85E+00	3.4E+02	3.7E+00	1.2E+01			---		VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T06-A	1	7.23E+00	E		7.23E+00	1.2E+02	3.7E+00	1.2E+01			---		VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T07-A	1	1.41E+01			1.41E+01	5.9E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T08-A	1	2.37E+01			2.37E+01	2.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T09-A	1	6.51E+03			6.51E+03	4.6E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T01-B	1	1.04E+02			1.04E+02	2.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T02-B	1	8.77E+01			8.77E+01	9.8E+00	3.7E+00	1.2E+01	1000	100	1.11E+03	103%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T03-B	1	7.91E+01			7.91E+01	1.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T04-B	1	1.75E+01			1.75E+01	1.6E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T05-B	1	2.09E+01			2.09E+01	2.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T06-B	1	2.35E+01			2.35E+01	8.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T07-B	1	2.70E+01			2.70E+01	5.6E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T08-B	1	1.29E+01			1.29E+01	5.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T09-B	1	8.88E+03			8.88E+03	8.2E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T01-C	1	1.10E+02			1.10E+02	3.6E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T02-C	1	7.42E+01			7.42E+01	1.5E+01	3.7E+00	1.2E+01	1000	100	1.16E+03	109%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T03-C	1	4.20E+01			4.20E+01	1.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T04-C	1	1.99E+01			1.99E+01	7.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T05-C	1	1.45E+01			1.45E+01	6.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T06-C	1	9.62E+00	E		9.62E+00	8.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T07-C	1	8.27E+00	E		8.27E+00	4.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T08-C	1	4.05E+01			4.05E+01	1.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-T09-C	1	1.05E+04			1.05E+04	6.0E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-B01-A	1	6.85E+00	E		6.85E+00	6.4E+01	3.7E+00	1.2E+01					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-B02-A	1	2.36E+01			2.36E+01	2.8E+01	3.7E+00	1.2E+01					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1313-B03-A	1	2.03E+01			2.03E+01	4.1E+01	3.7E+00	1.2E+01					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	CFS-L09-1313-T01-A	1	2.04E+06			2.04E+06	1.5E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T02-A	1	2.09E+06			2.09E+06	2.0E-01	1.6E+00	5.1E+00	1000	100	2.09E+06	83%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T03-A	1	4.49E+05			4.49E+05	1.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T04-A	1	2.55E+05			2.55E+05	4.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T05-A	1	9.15E+03			9.15E+03	6.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T06-A	1	9.84E+03			9.84E+03	7.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T07-A	1	1.20E+04			1.20E+04	5.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T08-A	1	1.65E+04			1.65E+04	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T09-A	1	2.58E+04			2.58E+04	1.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T01-B	1	2.30E+06			2.30E+06	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T02-B	1	2.15E+06			2.15E+06	5.6E-01	1.6E+00	5.1E+00	1000	100	2.15E+06	85%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T03-B	1	4.96E+05			4.96E+05	2.4E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T04-B	1	2.57E+05			2.57E+05	2.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T05-B	1	8.63E+03			8.63E+03	1.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T06-B	1	9.70E+03			9.70E+03	6.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T07-B	1	1.41E+04			1.41E+04	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T08-B	1	1.43E+04			1.43E+04	7.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T09-B	1	2.57E+04			2.57E+04	5.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T01-C	1	2.39E+06			2.39E+06	6.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T02-C	1	2.20E+06			2.20E+06	1.4E+00	1.6E+00	5.1E+00	1000	100	2.20E+06	84%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T03-C	1	4.70E+05			4.70E+05	1.5E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T04-C	1	2.60E+05			2.60E+05	1.4E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T05-C	1	9.51E+03			9.51E+03	5.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T06-C	1	9.73E+03			9.73E+03	6.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T07-C	1	1.13E+04			1.13E+04	2.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T08-C	1	1.57E+04			1.57E+04	1.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-T09-C	1	2.46E+04			2.46E+04	8.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-B01-A	1	3.20E+01			3.20E+01	3.4E+00	1.6E+00	5.1E+00					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-B02-A	1	2.02E+04			2.02E+04	1.2E+00	1.6E+00	5.1E+00					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1313-B03-A	1	2.15E+06			2.15E+06	1.5E+00	1.6E+00	5.1E+00					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	CFS-L09-1313-T01-A	1	2.93E+02			2.93E+02	5.5E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T02-A	1	5.32E+02			5.32E+02	6.1E+00	1.5E+01	4.8E+01	10	100	1.50E+03	97%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T03-A	1	5.12E+02			5.12E+02	1.7E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T04-A	1	1.28E+02			1.28E+02	8.6E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T05-A	1	9.28E+01			9.28E+01	1.3E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T06-A	1	9.18E+01			9.18E+01	3.3E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T07-A	1	1.69E+02			1.69E+02	1.0E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T08-A	1	2.50E+02			2.50E+02	1.2E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T09-A	1	7.09E+02			7.09E+02	3.9E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T01-B	1	5.09E+02			5.09E+02	2.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T02-B	1	2.77E+02			2.77E+02	5.5E+00	1.5E+01	4.8E+01	10	100	1.28E+03	100%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T03-B	1	4.83E+02			4.83E+02	1.0E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T04-B	1	1.30E+02			1.30E+02	7.0E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T05-B	1	8.84E+01			8.84E+01	2.7E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T06-B	1	1.06E+02			1.06E+02	4.8E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T07-B	1	2.15E+02			2.15E+02	3.8E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T08-B	1	2.27E+02			2.27E+02	6.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T09-B	1	9.26E+02			9.26E+02	8.1E-01	1.5E+01	4.8E+01			---		VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T01-C	1	4.94E+02			4.94E+02	3.8E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T02-C	1	3.34E+02			3.34E+02	9.8E+00	1.5E+01	4.8E+01	10	100	1.32E+03	99%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T03-C	1	4.50E+02			4.50E+02	3.9E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T04-C	1	1.45E+02			1.45E+02	7.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T05-C	1	9.45E+01			9.45E+01	2.6E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T06-C	1	9.27E+01			9.27E+01	9.6E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T07-C	1	1.22E+02			1.22E+02	2.5E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T08-C	1	2.22E+02			2.22E+02	3.6E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-T09-C	1	1.09E+03			1.09E+03	1.9E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-B01-A	1	1.62E+01	E		1.62E+01	2.0E+01	1.5E+01	4.8E+01					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-B02-A	1	2.37E+01	E		2.37E+01	2.0E+01	1.5E+01	4.8E+01					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1313-B03-A	1	2.08E+01	E		2.08E+01	3.5E+01	1.5E+01	4.8E+01					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	CFS-L09-1313-T01-A	1	1.53E+02			1.53E+02	2.0E+00	1.1E+00	3.5E+00			---		VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T02-A	1	2.18E+02			2.18E+02	3.7E-01	1.1E+00	3.5E+00	1000	100	1.19E+03	97%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T03-A	1	4.18E+02			4.18E+02	3.9E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T04-A	1	7.53E+02			7.53E+02	1.6E+00	1.1E+00	3.5E+00			---		VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T05-A	1	3.53E+03			3.53E+03	5.0E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T06-A	1	7.70E+03			7.70E+03	8.4E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T07-A	1	3.35E+04			3.35E+04	6.3E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T08-A	1	7.57E+04			7.57E+04	6.2E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T09-A	1	1.40E+05			1.40E+05	5.7E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T01-B	1	2.80E+02			2.80E+02	2.1E+00	1.1E+00	3.5E+00			---		VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T02-B	1	1.57E+02			1.57E+02	2.0E+00	1.1E+00	3.5E+00	1000	100	1.19E+03	103%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T03-B	1	3.77E+02			3.77E+02	2.2E+00	1.1E+00	3.5E+00			---		VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T04-B	1	7.55E+02			7.55E+02	2.0E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T05-B	1	3.21E+03			3.21E+03	8.9E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T06-B	1	7.80E+03			7.80E+03	1.5E+00	1.1E+00	3.5E+00			---		VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T07-B	1	4.88E+04			4.88E+04	5.9E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T08-B	1	4.73E+04			4.73E+04	1.3E+00	1.1E+00	3.5E+00			---		VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T09-B	1	1.29E+05			1.29E+05	4.6E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T01-C	1	2.59E+02			2.59E+02	1.1E+01	1.1E+00	3.5E+00			---		VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T02-C	1	1.98E+02			1.98E+02	2.7E+00	1.1E+00	3.5E+00	1000	100	1.19E+03	99%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T03-C	1	4.64E+02			4.64E+02	4.7E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T04-C	1	7.55E+02			7.55E+02	3.7E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T05-C	1	3.81E+03			3.81E+03	1.3E+00	1.1E+00	3.5E+00			---		VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T06-C	1	7.49E+03			7.49E+03	7.5E-02	1.1E+00	3.5E+00			---		VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T07-C	1	1.97E+04			1.97E+04	1.3E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T08-C	1	7.40E+04			7.40E+04	6.5E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-T09-C	1	1.12E+05			1.12E+05	1.1E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-B01-A	1	5.50E-01	U1/2		5.50E-01	8.8E+03	1.1E+00	3.5E+00					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-B02-A	1	7.58E+01			7.58E+01	4.7E+00	1.1E+00	3.5E+00					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1313-B03-A	1	1.47E+03			1.47E+03	1.8E+01	1.1E+00	3.5E+00					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	CFS-L09-1313-T01-A	1	9.32E+03			9.32E+03	5.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T02-A	1	9.47E+03			9.47E+03	2.2E-01	2.5E+00	8.0E+00	1000	100	1.03E+04	86%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T03-A	1	8.92E+03			8.92E+03	2.4E-02	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T04-A	1	9.76E+03			9.76E+03	1.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T05-A	1	9.52E+03			9.52E+03	6.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T06-A	1	9.71E+03			9.71E+03	8.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T07-A	1	9.93E+03			9.93E+03	4.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T08-A	1	1.09E+04			1.09E+04	1.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T09-A	1	1.21E+04			1.21E+04	5.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T01-B	1	9.98E+03			9.98E+03	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T02-B	1	8.76E+03			8.76E+03	4.4E-01	2.5E+00	8.0E+00	1000	100	9.66E+03	90%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T03-B	1	9.96E+03			9.96E+03	4.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T04-B	1	9.65E+03			9.65E+03	8.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T05-B	1	9.07E+03			9.07E+03	2.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T06-B	1	9.36E+03			9.36E+03	4.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T07-B	1	1.02E+04			1.02E+04	3.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T08-B	1	1.05E+04			1.05E+04	9.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T09-B	1	1.22E+04			1.22E+04	8.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T01-C	1	1.07E+04			1.07E+04	3.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T02-C	1	9.88E+03			9.88E+03	5.7E-01	2.5E+00	8.0E+00	1000	100	1.07E+04	85%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T03-C	1	9.83E+03			9.83E+03	6.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T04-C	1	9.94E+03			9.94E+03	4.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T05-C	1	9.79E+03			9.79E+03	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T06-C	1	9.74E+03			9.74E+03	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T07-C	1	9.96E+03			9.96E+03	8.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T08-C	1	1.07E+04			1.07E+04	8.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-T09-C	1	1.17E+04			1.17E+04	9.6E-02	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-B01-A	1	2.30E+01			2.30E+01	4.5E+00	2.5E+00	8.0E+00					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-B02-A	1	3.77E+01			3.77E+01	2.1E+00	2.5E+00	8.0E+00					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1313-B03-A	1	6.09E+02			6.09E+02	2.8E-01	2.5E+00	8.0E+00					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	CFS-L09-1313-T01-A	1	2.08E+03			2.08E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T02-A	1	3.71E+03			3.71E+03	4.6E-01	1.0E+00	3.2E+00	1000	100	4.68E+03	97%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T03-A	1	3.67E+03			3.67E+03	6.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T04-A	1	3.17E+03			3.17E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T05-A	1	1.43E+03			1.43E+03	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T06-A	1	9.04E+02			9.04E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T07-A	1	9.58E+02			9.58E+02	9.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T08-A	1	1.13E+03			1.13E+03	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T09-A	1	1.37E+03			1.37E+03	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T01-B	1	2.47E+03			2.47E+03	1.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T02-B	1	2.86E+03			2.86E+03	1.8E-01	1.0E+00	3.2E+00	1000	100	3.82E+03	96%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T03-B	1	3.87E+03			3.87E+03	9.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T04-B	1	3.26E+03			3.26E+03	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T05-B	1	1.39E+03			1.39E+03	5.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T06-B	1	8.90E+02			8.90E+02	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T07-B	1	1.01E+03			1.01E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T08-B	1	1.06E+03			1.06E+03	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T09-B	1	1.37E+03			1.37E+03	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T01-C	1	2.72E+03			2.72E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T02-C	1	2.43E+03			2.43E+03	1.1E+00	1.0E+00	3.2E+00	1000	100	3.41E+03	98%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T03-C	1	3.98E+03			3.98E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T04-C	1	3.15E+03			3.15E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T05-C	1	1.37E+03			1.37E+03	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T06-C	1	9.13E+02			9.13E+02	7.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T07-C	1	9.50E+02			9.50E+02	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T08-C	1	1.10E+03			1.10E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-T09-C	1	1.33E+03			1.33E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	4.4E+02	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-B02-A	1	3.14E+00	E		3.14E+00	3.7E+01	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1313-B03-A	1	1.05E+00	E		1.05E+00	2.1E+01	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	CFS-L09-1313-T01-A	1	1.20E+06			1.20E+06	9.8E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T02-A	1	9.38E+05			9.38E+05	5.8E-02	6.8E+00	2.2E+01	1000	100	9.38E+05	82%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T03-A	1	7.48E+05			7.48E+05	2.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T04-A	1	6.93E+05			6.93E+05	7.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T05-A	1	6.08E+05			6.08E+05	5.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T06-A	1	6.05E+05			6.05E+05	8.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T07-A	1	6.34E+05			6.34E+05	2.7E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T08-A	1	6.76E+05			6.76E+05	7.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T09-A	1	8.22E+05			8.22E+05	3.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T01-B	1	1.31E+06			1.31E+06	2.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T02-B	1	1.25E+06			1.25E+06	2.6E-01	6.8E+00	2.2E+01	1000	100	1.25E+06	89%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T03-B	1	7.85E+05			7.85E+05	1.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T04-B	1	6.85E+05			6.85E+05	6.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T05-B	1	5.70E+05			5.70E+05	4.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T06-B	1	6.05E+05			6.05E+05	6.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T07-B	1	6.53E+05			6.53E+05	9.7E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T08-B	1	6.62E+05			6.62E+05	9.7E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T09-B	1	8.19E+05			8.19E+05	5.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T01-C	1	1.42E+06			1.42E+06	1.1E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T02-C	1	1.28E+06			1.28E+06	1.2E+00	6.8E+00	2.2E+01	1000	100	1.28E+06	85%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T03-C	1	7.87E+05			7.87E+05	5.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T04-C	1	7.00E+05			7.00E+05	7.9E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T05-C	1	6.14E+05			6.14E+05	3.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T06-C	1	6.01E+05			6.01E+05	5.8E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T07-C	1	6.32E+05			6.32E+05	2.3E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T08-C	1	6.57E+05			6.57E+05	1.0E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-T09-C	1	7.94E+05			7.94E+05	9.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	1.6E+01	6.8E+00	2.2E+01					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	1.0E+01	6.8E+00	2.2E+01					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	2.7E+01	6.8E+00	2.2E+01					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

TI	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
TI	CFS-L09-1313-T01-A	1	1.63E+02			1.63E+02	1.7E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T02-A	1	1.90E+02			1.90E+02	3.7E+00	4.6E+00	1.5E+01	10	100	1.08E+03	89%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T03-A	1	2.64E+02			2.64E+02	1.3E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T04-A	1	6.16E+02			6.16E+02	1.5E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T05-A	1	3.07E+02			3.07E+02	3.0E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T06-A	1	3.90E+02			3.90E+02	2.3E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T07-A	1	6.05E+02			6.05E+02	1.1E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T08-A	1	9.32E+02			9.32E+02	1.2E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T09-A	1	1.79E+03			1.79E+03	4.1E-01	4.6E+00	1.5E+01			---		VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T01-B	1	1.93E+02			1.93E+02	3.2E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T02-B	1	1.69E+02			1.69E+02	2.9E+00	4.6E+00	1.5E+01	10	100	1.00E+03	83%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T03-B	1	3.16E+02			3.16E+02	1.4E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T04-B	1	6.08E+02			6.08E+02	1.2E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T05-B	1	2.92E+02			2.92E+02	8.7E-01	4.6E+00	1.5E+01			---		VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T06-B	1	3.94E+02			3.94E+02	8.1E-01	4.6E+00	1.5E+01			---		VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T07-B	1	7.57E+02			7.57E+02	2.4E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T08-B	1	7.95E+02			7.95E+02	1.4E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T09-B	1	1.94E+03			1.94E+03	8.6E-01	4.6E+00	1.5E+01			---		VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T01-C	1	2.25E+02			2.25E+02	2.8E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T02-C	1	2.01E+02			2.01E+02	3.0E-01	4.6E+00	1.5E+01	10	100	1.11E+03	91%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T03-C	1	3.67E+02			3.67E+02	2.0E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T04-C	1	6.11E+02			6.11E+02	8.5E-01	4.6E+00	1.5E+01			---		VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T05-C	1	3.37E+02			3.37E+02	8.5E-01	4.6E+00	1.5E+01			---		VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T06-C	1	3.81E+02			3.81E+02	4.7E-01	4.6E+00	1.5E+01			---		VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T07-C	1	5.45E+02			5.45E+02	7.2E-01	4.6E+00	1.5E+01			---		VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T08-C	1	8.93E+02			8.93E+02	5.4E-01	4.6E+00	1.5E+01			---		VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-T09-C	1	1.98E+03			1.98E+03	7.6E-01	4.6E+00	1.5E+01			---		VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	8.8E+00	4.6E+00	1.5E+01					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	3.8E+01	4.6E+00	1.5E+01					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
TI	CFS-L09-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	2.2E+01	4.6E+00	1.5E+01					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	CFS-L09-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	5.6E+01	2.0E+00	6.4E+00	10	100	1.02E+03	102%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	3.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	4.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	7.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	8.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T07-A	1	9.13E+00			9.13E+00	2.9E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T08-A	1	2.42E+01			2.42E+01	5.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T09-A	1	1.89E+02			1.89E+02	3.4E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	1.9E+02	2.0E+00	6.4E+00	10	100	9.42E+02	94%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	8.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	2.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	5.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T07-B	1	2.06E+01			2.06E+01	1.9E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T08-B	1	2.07E+01			2.07E+01	3.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T09-B	1	3.07E+02			3.07E+02	7.5E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	1.0E+02	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	4.1E+01	2.0E+00	6.4E+00	10	100	1.03E+03	103%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	9.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	8.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	8.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T07-C	1	2.38E+00	E		2.38E+00	1.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T08-C	1	2.38E+01			2.38E+01	9.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-T09-C	1	4.01E+02			4.01E+02	1.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	2.1E+01	2.0E+00	6.4E+00					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-B02-A	1	6.78E+00			6.78E+00	1.5E+00	2.0E+00	6.4E+00					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1313-B03-A	1	4.19E+00	E		4.19E+00	8.8E+00	2.0E+00	6.4E+00					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	CFS-L09-1313-T01-A	1	1.92E+01			1.92E+01	4.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T02-A	1	1.82E+01			1.82E+01	1.3E+01	1.5E+00	4.8E+00	10	100	1.01E+03	99%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T03-A	1	1.92E+01			1.92E+01	4.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T04-A	1	2.42E+01			2.42E+01	3.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T05-A	1	2.47E+01			2.47E+01	3.7E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T06-A	1	2.55E+01			2.55E+01	1.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T07-A	1	3.56E+01			3.56E+01	3.1E-01	1.5E+00	4.8E+00			---		VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T08-A	1	4.12E+01			4.12E+01	3.0E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T09-A	1	5.21E+02			5.21E+02	1.7E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T01-B	1	1.87E+01			1.87E+01	1.3E+01	1.5E+00	4.8E+00			---		VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T02-B	1	1.84E+01			1.84E+01	1.9E+00	1.5E+00	4.8E+00	10	100	9.56E+02	94%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T03-B	1	2.12E+01			2.12E+01	5.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T04-B	1	2.19E+01			2.19E+01	1.6E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T05-B	1	2.32E+01			2.32E+01	2.5E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T06-B	1	2.62E+01			2.62E+01	5.2E-02	1.5E+00	4.8E+00			---		VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T07-B	1	4.22E+01			4.22E+01	2.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T08-B	1	3.99E+01			3.99E+01	4.9E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T09-B	1	5.37E+02			5.37E+02	1.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T01-C	1	1.91E+01			1.91E+01	5.6E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T02-C	1	1.97E+01			1.97E+01	5.9E+00	1.5E+00	4.8E+00	10	100	1.06E+03	104%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T03-C	1	2.20E+01			2.20E+01	2.7E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T04-C	1	2.51E+01			2.51E+01	2.8E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T05-C	1	2.48E+01			2.48E+01	1.9E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T06-C	1	2.58E+01			2.58E+01	2.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T07-C	1	2.93E+01			2.93E+01	3.5E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T08-C	1	3.76E+01			3.76E+01	4.6E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-T09-C	1	5.19E+02			5.19E+02	1.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-B01-A	1	7.50E-01	U1/2		7.50E-01	4.0E+01	1.5E+00	4.8E+00					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-B02-A	1	7.50E-01	U1/2		7.50E-01	5.8E+00	1.5E+00	4.8E+00					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1313-B03-A	1	7.50E-01	U1/2		7.50E-01	1.8E+01	1.5E+00	4.8E+00					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	CFS-L09-1313-T01-A	1	7.10E+03			7.10E+03	2.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:04 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T02-A	1	1.57E+03			1.57E+03	2.3E-01	1.0E+00	3.2E+00	10	100	2.49E+03	91%	VU ICP-OES	4/19/11 4:06 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T03-A	1	3.63E+01			3.63E+01	9.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:07 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T04-A	1	3.38E+01			3.38E+01	1.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:09 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T05-A	1	2.05E+04			2.05E+04	6.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:11 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T06-A	1	6.89E+04			6.89E+04	2.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:12 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T07-A	1	1.62E+05			1.62E+05	9.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 5:34 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T08-A	1	1.62E+05			1.62E+05	2.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 5:36 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T09-A	1	1.52E+05			1.52E+05	2.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:17 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T01-B	1	1.25E+04			1.25E+04	1.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:24 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T02-B	1	6.95E+03			6.95E+03	1.6E+00	1.0E+00	3.2E+00	10	100	7.81E+03	86%	VU ICP-OES	4/19/11 4:26 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T03-B	1	2.28E+01			2.28E+01	1.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:27 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T04-B	1	3.47E+01			3.47E+01	7.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:29 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T05-B	1	1.72E+04			1.72E+04	4.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:30 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T06-B	1	7.24E+04			7.24E+04	5.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:32 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T07-B	1	1.62E+05			1.62E+05	2.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 5:38 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T08-B	1	1.60E+05			1.60E+05	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 5:39 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T09-B	1	1.55E+05			1.55E+05	1.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:37 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T01-C	1	4.03E+03			4.03E+03	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:39 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T02-C	1	7.56E+03			7.56E+03	1.3E+00	1.0E+00	3.2E+00	10	100	8.48E+03	91%	VU ICP-OES	4/19/11 4:40 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T03-C	1	2.80E+01			2.80E+01	1.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:42 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T04-C	1	3.30E+01			3.30E+01	2.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:44 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T05-C	1	2.28E+04			2.28E+04	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:45 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T06-C	1	7.09E+04			7.09E+04	3.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:47 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T07-C	1	1.38E+05			1.38E+05	6.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 5:41 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T08-C	1	1.59E+05			1.59E+05	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 5:43 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-T09-C	1	1.46E+05			1.46E+05	2.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/19/11 4:52 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-B01-A	1	2.61E+00	E		2.61E+00	4.5E+00	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 3:49 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-B02-A	1	3.98E+00			3.98E+00	1.7E+00	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 3:51 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1313-B03-A	1	3.59E+00			3.59E+00	2.7E+00	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 3:53 PM	EPA Interlab L09 1313-1316 CFS

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	CFS-L10-1313-T01-A	1	1.01E+02			1.01E+02	2.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T02-A	1	1.06E+02			1.06E+02	2.0E+00	1.0E+00	3.2E+00	1000	100	1.16E+03	106%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T03-A	1	7.87E+01			7.87E+01	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T04-A	1	5.33E+01			5.33E+01	1.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T05-A	1	4.42E+01			4.42E+01	7.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T06-A	1	2.36E+02			2.36E+02	3.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T07-A	1	4.61E+03			4.61E+03	3.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T08-A	1	2.72E+04			2.72E+04	9.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T09-A	1	7.10E+04			7.10E+04	5.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T10-A	1	5.06E+01			5.06E+01	7.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T01-B	1	1.08E+02			1.08E+02	2.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T02-B	1	1.20E+02			1.20E+02	3.1E+00	1.0E+00	3.2E+00	1000	100	1.11E+03	99%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T03-B	1	8.60E+01			8.60E+01	2.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T04-B	1	5.02E+01			5.02E+01	3.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T05-B	1	4.59E+01			4.59E+01	4.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T06-B	1	1.97E+02			1.97E+02	8.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T07-B	1	4.58E+03			4.58E+03	3.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T08-B	1	2.66E+04			2.66E+04	4.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T09-B	1	6.73E+04			6.73E+04	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T10-B	1	4.65E+01			4.65E+01	7.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T01-C	1	1.04E+02			1.04E+02	2.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T02-C	1	1.25E+02			1.25E+02	2.0E+00	1.0E+00	3.2E+00	1000	100	1.17E+03	105%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T03-C	1	8.94E+01			8.94E+01	3.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T04-C	1	5.50E+01			5.50E+01	4.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T05-C	1	4.79E+01			4.79E+01	2.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T06-C	1	1.94E+02			1.94E+02	2.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T07-C	1	4.53E+03			4.53E+03	6.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T08-C	1	2.71E+04			2.71E+04	6.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T09-C	1	6.92E+04			6.92E+04	2.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-T10-C	1	5.01E+01			5.01E+01	5.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	2.2E+01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	1.8E+02	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-B03-A	1	1.16E+00	E		1.16E+00	7.4E+01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	3.6E+01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	1.7E+02	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-B03-B	1	5.00E-01	U1/2		5.00E-01	3.0E+02	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	7.2E+02	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-B02-C	1	1.10E+00	E		1.10E+00	1.0E+02	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1313-B03-C	1	4.58E+00			4.58E+00	8.2E+01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	CFS-L10-1313-T01-A	1	1.84E+01	E		1.84E+01	5.6E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T02-A	1	1.45E+01	E		1.45E+01	8.9E+01	7.5E+00	2.4E+01	10	120	1.16E+03	95%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T03-A	1	2.96E+01			2.96E+01	1.9E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T04-A	1	2.41E+01			2.41E+01	2.8E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T05-A	1	2.95E+01			2.95E+01	2.9E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T06-A	1	4.93E+01			4.93E+01	5.5E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T07-A	1	1.16E+02			1.16E+02	1.2E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T08-A	1	7.43E+02			7.43E+02	1.6E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T09-A	1	1.34E+03			1.34E+03	6.6E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T10-A	1	3.41E+01			3.41E+01	2.1E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T01-B	1	1.40E+01	E		1.40E+01	6.3E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T02-B	1	1.69E+01	E		1.69E+01	5.3E+01	7.5E+00	2.4E+01	10	120	1.20E+03	98%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T03-B	1	4.06E+01			4.06E+01	5.6E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T04-B	1	2.73E+01			2.73E+01	2.6E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T05-B	1	3.02E+01			3.02E+01	1.2E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T06-B	1	5.42E+01			5.42E+01	1.5E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T07-B	1	1.14E+02			1.14E+02	7.0E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T08-B	1	6.89E+02			6.89E+02	2.0E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T09-B	1	1.26E+03			1.26E+03	1.0E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T10-B	1	2.57E+01			2.57E+01	2.8E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T01-C	1	1.75E+01	E		1.75E+01	1.8E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T02-C	1	1.39E+01	E		1.39E+01	3.1E+01	7.5E+00	2.4E+01	10	120	1.10E+03	91%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T03-C	1	4.23E+01			4.23E+01	8.2E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T04-C	1	3.70E+01			3.70E+01	1.2E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T05-C	1	2.53E+01			2.53E+01	2.4E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T06-C	1	4.56E+01			4.56E+01	2.2E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T07-C	1	1.03E+02			1.03E+02	1.6E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T08-C	1	7.99E+02			7.99E+02	3.4E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T09-C	1	1.37E+03			1.37E+03	4.4E+00	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-T10-C	1	4.48E+01			4.48E+01	2.3E+01	7.5E+00	2.4E+01			---		VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-B01-A	1	3.75E+00	U1/2		3.75E+00	1.5E+02	7.5E+00	2.4E+01					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-B02-A	1	1.03E+01	E		1.03E+01	1.4E+02	7.5E+00	2.4E+01					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-B03-A	1	4.53E+01			4.53E+01	9.2E+00	7.5E+00	2.4E+01					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-B01-B	1	1.13E+01	E		1.13E+01	5.3E+01	7.5E+00	2.4E+01					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-B02-B	1	8.85E+00	E		8.85E+00	6.6E+01	7.5E+00	2.4E+01					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-B03-B	1	2.09E+01	E		2.09E+01	2.6E+01	7.5E+00	2.4E+01					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-B01-C	1	9.82E+00	E		9.82E+00	1.0E+02	7.5E+00	2.4E+01					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-B02-C	1	3.75E+00	U1/2		3.75E+00	4.6E+02	7.5E+00	2.4E+01					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1313-B03-C	1	2.25E+01	E		2.25E+01	2.0E+00	7.5E+00	2.4E+01					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	CFS-L10-1313-T01-A	1	1.33E+02			1.33E+02	5.1E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T02-A	1	1.90E+02			1.90E+02	1.7E+00	1.1E+01	3.5E+01	10	120	1.39E+03	100%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T03-A	1	7.48E+01			7.48E+01	4.4E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T04-A	1	2.72E+01	E		2.72E+01	6.6E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T05-A	1	1.78E+01	E		1.78E+01	5.2E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T06-A	1	3.62E+01			3.62E+01	2.0E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T07-A	1	1.56E+02			1.56E+02	3.9E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T08-A	1	6.56E+02			6.56E+02	1.9E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T09-A	1	1.29E+04			1.29E+04	3.5E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T10-A	1	2.19E+01	E		2.19E+01	6.0E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T01-B	1	1.09E+02			1.09E+02	2.5E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T02-B	1	1.89E+02			1.89E+02	1.9E+00	1.1E+01	3.5E+01	10	120	1.42E+03	102%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T03-B	1	8.10E+01			8.10E+01	6.8E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T04-B	1	2.92E+01	E		2.92E+01	4.6E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T05-B	1	2.36E+01	E		2.36E+01	1.6E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T06-B	1	3.22E+01	E		3.22E+01	2.7E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T07-B	1	1.63E+02			1.63E+02	5.5E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T08-B	1	6.18E+02			6.18E+02	4.6E-01	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T09-B	1	1.29E+04			1.29E+04	2.2E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T10-B	1	1.31E+01	E		1.31E+01	4.3E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T01-C	1	1.11E+02			1.11E+02	1.2E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T02-C	1	2.00E+02			2.00E+02	2.8E+00	1.1E+01	3.5E+01	10	120	1.32E+03	94%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T03-C	1	8.19E+01			8.19E+01	1.1E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T04-C	1	2.00E+01	E		2.00E+01	2.1E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T05-C	1	1.57E+01	E		1.57E+01	2.0E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T06-C	1	3.40E+01	E		3.40E+01	3.2E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T07-C	1	1.25E+02			1.25E+02	2.3E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T08-C	1	7.10E+02			7.10E+02	1.6E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T09-C	1	1.43E+04			1.43E+04	1.7E+00	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-T10-C	1	1.87E+01	E		1.87E+01	4.3E+01	1.1E+01	3.5E+01			---		VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-B01-A	1	5.50E+00	U1/2		5.50E+00	6.4E+02	1.1E+01	3.5E+01					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-B02-A	1	5.50E+00	U1/2		5.50E+00	9.1E+01	1.1E+01	3.5E+01					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-B03-A	1	6.43E+01			6.43E+01	2.2E+01	1.1E+01	3.5E+01					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-B01-B	1	5.50E+00	U1/2		5.50E+00	1.2E+03	1.1E+01	3.5E+01					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-B02-B	1	5.50E+00	U1/2		5.50E+00	2.9E+02	1.1E+01	3.5E+01					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-B03-B	1	1.67E+01	E		1.67E+01	3.8E+01	1.1E+01	3.5E+01					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-B01-C	1	5.50E+00	U1/2		5.50E+00	4.5E+01	1.1E+01	3.5E+01					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-B02-C	1	5.50E+00	U1/2		5.50E+00	2.0E+02	1.1E+01	3.5E+01					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1313-B03-C	1	5.50E+00	U1/2		5.50E+00	9.1E+01	1.1E+01	3.5E+01					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	CFS-L10-1313-T01-A	1	8.29E+01			8.29E+01	5.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T02-A	1	8.60E+01			8.60E+01	1.2E+00	1.0E+00	3.2E+00	1000	100	1.22E+03	113%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T03-A	1	1.46E+02			1.46E+02	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T04-A	1	1.16E+02			1.16E+02	2.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T05-A	1	1.39E+02			1.39E+02	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T06-A	1	2.12E+02			2.12E+02	2.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T07-A	1	3.34E+02			3.34E+02	7.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T08-A	1	6.11E+02			6.11E+02	3.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T09-A	1	7.49E+02			7.49E+02	5.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T10-A	1	1.63E+02			1.63E+02	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T01-B	1	7.81E+01			7.81E+01	5.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T02-B	1	9.53E+01			9.53E+01	5.7E-01	1.0E+00	3.2E+00	1000	100	1.26E+03	117%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T03-B	1	1.55E+02			1.55E+02	3.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T04-B	1	1.23E+02			1.23E+02	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T05-B	1	1.57E+02			1.57E+02	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T06-B	1	2.37E+02			2.37E+02	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T07-B	1	3.41E+02			3.41E+02	7.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T08-B	1	6.27E+02			6.27E+02	1.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T09-B	1	7.47E+02			7.47E+02	1.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T10-B	1	1.64E+02			1.64E+02	6.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T01-C	1	7.92E+01			7.92E+01	1.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T02-C	1	1.16E+02			1.16E+02	9.8E-01	1.0E+00	3.2E+00	1000	100	1.21E+03	110%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T03-C	1	1.62E+02			1.62E+02	9.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T04-C	1	1.32E+02			1.32E+02	1.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T05-C	1	1.50E+02			1.50E+02	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T06-C	1	2.27E+02			2.27E+02	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T07-C	1	3.61E+02			3.61E+02	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T08-C	1	6.24E+02			6.24E+02	5.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T09-C	1	7.01E+02			7.01E+02	4.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-T10-C	1	1.72E+02			1.72E+02	3.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-B01-A	1	6.99E+00			6.99E+00	9.1E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-B02-A	1	7.08E+00			7.08E+00	1.5E+01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-B03-A	1	1.63E+01			1.63E+01	6.2E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-B01-B	1	6.43E+00			6.43E+00	2.4E+01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-B02-B	1	7.11E+00			7.11E+00	2.1E+01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-B03-B	1	1.54E+01			1.54E+01	1.8E+01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-B01-C	1	5.71E+00			5.71E+00	1.4E+01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-B02-C	1	7.07E+00			7.07E+00	1.8E+01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1313-B03-C	1	1.52E+01			1.52E+01	3.2E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	CFS-L10-1313-T01-A	1	9.872			9.87E+00	5.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	6/17/11 12:16 PM	EPA Interlab 1313-1316 CFS Reruns
Ba	CFS-L10-1313-T02-A	1	1.42E+01			1.42E+01	7.7E-01	1.0E+00	3.2E+00	10	120	1.18E+03	97%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T03-A	1	1.35E+02			1.35E+02	8.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T04-A	1	6.40E+01			6.40E+01	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T05-A	1	1.16E+02			1.16E+02	8.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T06-A	1	4.18E+01			4.18E+01	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T07-A	1	3.35E+01			3.35E+01	6.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T08-A	1	3.67E+01			3.67E+01	5.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T09-A	1	5.79E+01			5.79E+01	7.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T10-A	1	1.12E+02			1.12E+02	4.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T01-B	1	8.657			8.66E+00	3.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T02-B	1	1.21E+01			1.21E+01	4.4E-01	1.0E+00	3.2E+00	10	120	1.22E+03	101%	VU ICP-OES	6/17/11 12:38 PM	EPA Interlab 1313-1316 CFS Reruns
Ba	CFS-L10-1313-T03-B	1	1.26E+02			1.26E+02	6.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T04-B	1	6.24E+01			6.24E+01	8.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T05-B	1	1.17E+02			1.17E+02	8.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T06-B	1	5.10E+01			5.10E+01	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T07-B	1	3.47E+01			3.47E+01	3.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T08-B	1	2.67E+01			2.67E+01	6.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T09-B	1	4.40E+01			4.40E+01	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T10-B	1	1.08E+02			1.08E+02	1.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T01-C	1	8.323			8.32E+00	5.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T02-C	1	1.10E+01			1.10E+01	2.0E+00	1.0E+00	3.2E+00	10	120	1.26E+03	104%	VU ICP-OES	6/17/11 1:00 PM	EPA Interlab 1313-1316 CFS Reruns
Ba	CFS-L10-1313-T03-C	1	1.34E+02			1.34E+02	7.3E-02	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T04-C	1	6.43E+01			6.43E+01	4.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T05-C	1	1.18E+02			1.18E+02	2.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T06-C	1	4.57E+01			4.57E+01	2.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T07-C	1	3.41E+01			3.41E+01	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T08-C	1	3.28E+01			3.28E+01	3.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T09-C	1	4.99E+01			4.99E+01	3.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-T10-C	1	1.11E+02			1.11E+02	7.4E-02	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	3.1E+01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	3.0E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-B03-A	1	1.92E+01			1.92E+01	2.8E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	1.3E+01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	9.6E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-B03-B	1	2.36E+01			2.36E+01	6.4E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	6.0E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-B02-C	1	1.22E+00	E		1.22E+00	1.5E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1313-B03-C	1	2.68E+01			2.68E+01	1.9E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	CFS-L10-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	4.6E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	3.0E+02	1.9E+00	6.0E+00	10	120	1.18E+03	98%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	1.9E+03	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	5.0E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	8.0E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	2.7E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T07-A	1	2.66E+00	E		2.66E+00	5.2E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T08-A	1	6.50E+00			6.50E+00	5.8E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T09-A	1	2.70E+00	E		2.70E+00	1.9E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T10-A	1	9.50E-01	U1/2		9.50E-01	3.2E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	4.2E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	2.9E+02	1.9E+00	6.0E+00	10	120	1.22E+03	101%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	3.9E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	1.7E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	2.8E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T07-B	1	2.82E+00	E		2.82E+00	6.5E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T08-B	1	6.04E+00			6.04E+00	5.2E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T09-B	1	2.78E+00	E		2.78E+00	1.6E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T10-B	1	9.50E-01	U1/2		9.50E-01	3.9E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	1.1E+03	1.9E+00	6.0E+00	10	120	1.10E+03	92%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	4.0E+03	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	3.3E+03	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	3.0E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T07-C	1	2.88E+00	E		2.88E+00	1.5E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T08-C	1	6.03E+00			6.03E+00	5.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T09-C	1	2.68E+00	E		2.68E+00	2.5E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-T10-C	1	9.50E-01	U1/2		9.50E-01	8.0E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	1.8E+02	1.9E+00	6.0E+00					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	3.4E+02	1.9E+00	6.0E+00					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	6.0E+01	1.9E+00	6.0E+00					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-B01-B	1	9.50E-01	U1/2		9.50E-01	1.7E+02	1.9E+00	6.0E+00					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-B02-B	1	9.50E-01	U1/2		9.50E-01	1.9E+02	1.9E+00	6.0E+00					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-B03-B	1	9.50E-01	U1/2		9.50E-01	1.0E+02	1.9E+00	6.0E+00					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-B01-C	1	9.50E-01	U1/2		9.50E-01	3.1E+02	1.9E+00	6.0E+00					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-B02-C	1	9.50E-01	U1/2		9.50E-01	1.6E+02	1.9E+00	6.0E+00					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1313-B03-C	1	9.50E-01	U1/2		9.50E-01	1.8E+02	1.9E+00	6.0E+00					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	CFS-L10-1313-T01-A	1	7.16E+00			7.16E+00	1.3E+00	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T02-A	1	1.10E+00	U1/2		1.10E+00	3.2E+01	2.2E+00	7.0E+00	10	120	1.11E+03	92%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T03-A	1	1.10E+00	U1/2		1.10E+00	8.3E+00	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T04-A	1	9.50E+01			9.50E+01	1.8E+00	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T05-A	1	1.80E+03			1.80E+03	4.9E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T06-A	1	1.25E+04			1.25E+04	9.6E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T07-A	1	2.42E+04			2.42E+04	7.1E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T08-A	1	4.52E+04			4.52E+04	1.1E+00	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T09-A	1	4.68E+04			4.68E+04	4.4E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T10-A	1	4.17E+03			4.17E+03	3.6E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T01-B	1	7.41E+00			7.41E+00	7.8E+00	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T02-B	1	1.10E+00	U1/2		1.10E+00	1.6E+01	2.2E+00	7.0E+00	10	120	1.15E+03	96%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T03-B	1	1.10E+00	U1/2		1.10E+00	2.1E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T04-B	1	8.51E+01			8.51E+01	8.6E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T05-B	1	2.22E+03			2.22E+03	9.3E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T06-B	1	1.34E+04			1.34E+04	1.2E+00	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T07-B	1	2.44E+04			2.44E+04	8.0E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T08-B	1	4.47E+04			4.47E+04	5.2E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T09-B	1	4.73E+04			4.73E+04	1.2E+00	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T10-B	1	4.15E+03			4.15E+03	3.7E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T01-C	1	9.37E+00			9.37E+00	1.8E+00	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T02-C	1	1.10E+00	U1/2		1.10E+00	1.0E+01	2.2E+00	7.0E+00	10	120	1.10E+03	92%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T03-C	1	2.24E+00	E		2.24E+00	1.2E+01	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T04-C	1	1.08E+02			1.08E+02	8.0E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T05-C	1	2.21E+03			2.21E+03	4.2E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T06-C	1	1.28E+04			1.28E+04	4.2E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T07-C	1	2.55E+04			2.55E+04	6.6E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T08-C	1	4.57E+04			4.57E+04	1.7E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T09-C	1	4.76E+04			4.76E+04	2.4E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-T10-C	1	4.39E+03			4.39E+03	5.6E-01	2.2E+00	7.0E+00			---		VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	1.3E+02	2.2E+00	7.0E+00					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-B02-A	1	1.10E+00	U1/2		1.10E+00	9.9E+01	2.2E+00	7.0E+00					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-B03-A	1	1.10E+00	U1/2		1.10E+00	4.2E+02	2.2E+00	7.0E+00					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-B01-B	1	1.10E+00	U1/2		1.10E+00	1.4E+02	2.2E+00	7.0E+00					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-B02-B	1	1.10E+00	U1/2		1.10E+00	6.4E+01	2.2E+00	7.0E+00					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-B03-B	1	1.10E+00	U1/2		1.10E+00	1.6E+01	2.2E+00	7.0E+00					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-B01-C	1	1.10E+00	U1/2		1.10E+00	6.8E+01	2.2E+00	7.0E+00					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-B02-C	1	1.10E+00	U1/2		1.10E+00	6.9E+01	2.2E+00	7.0E+00					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1313-B03-C	1	1.10E+00	U1/2		1.10E+00	6.4E+01	2.2E+00	7.0E+00					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	CFS-L10-1313-T01-A	1	1.89E+05			1.89E+05	3.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T02-A	1	5.62E+05			5.62E+05	5.6E-01	2.6E+00	8.3E+00	1000	100	5.63E+05	87%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T03-A	1	5.81E+05			5.81E+05	9.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T04-A	1	6.12E+05			6.12E+05	1.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T05-A	1	6.32E+05			6.32E+05	4.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T06-A	1	7.11E+05			7.11E+05	4.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T07-A	1	8.60E+05			8.60E+05	7.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T08-A	1	1.26E+06			1.26E+06	1.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T09-A	1	1.47E+06			1.47E+06	1.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T10-A	1	6.54E+05			6.54E+05	4.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T01-B	1	2.04E+05			2.04E+05	4.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T02-B	1	5.47E+05			5.47E+05	4.6E-01	2.6E+00	8.3E+00	1000	100	5.48E+05	84%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T03-B	1	5.76E+05			5.76E+05	9.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T04-B	1	6.06E+05			6.06E+05	9.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T05-B	1	6.38E+05			6.38E+05	6.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T06-B	1	7.45E+05			7.45E+05	1.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T07-B	1	8.77E+05			8.77E+05	2.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T08-B	1	1.24E+06			1.24E+06	6.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T09-B	1	1.40E+06			1.40E+06	1.5E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T10-B	1	6.34E+05			6.34E+05	3.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T01-C	1	1.99E+05			1.99E+05	5.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T02-C	1	5.58E+05			5.58E+05	1.7E+00	2.6E+00	8.3E+00	1000	100	5.58E+05	86%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T03-C	1	6.03E+05			6.03E+05	7.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T04-C	1	6.35E+05			6.35E+05	7.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T05-C	1	6.56E+05			6.56E+05	4.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T06-C	1	7.02E+05			7.02E+05	4.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T07-C	1	8.96E+05			8.96E+05	1.7E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T08-C	1	1.26E+06			1.26E+06	5.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T09-C	1	1.44E+06			1.44E+06	1.9E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-T10-C	1	6.59E+05			6.59E+05	8.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-B01-A	1	2.63E+01			2.63E+01	1.9E+01	2.6E+00	8.3E+00					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-B02-A	1	2.49E+01			2.49E+01	4.1E+00	2.6E+00	8.3E+00					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-B03-A	1	7.46E+01			7.46E+01	4.1E+01	2.6E+00	8.3E+00					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-B01-B	1	2.18E+01			2.18E+01	1.2E+01	2.6E+00	8.3E+00					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-B02-B	1	1.71E+01			1.71E+01	1.7E+01	2.6E+00	8.3E+00					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-B03-B	1	5.79E+01			5.79E+01	3.2E+01	2.6E+00	8.3E+00					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-B01-C	1	2.12E+01			2.12E+01	2.2E+01	2.6E+00	8.3E+00					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-B02-C	1	1.80E+01			1.80E+01	2.1E+01	2.6E+00	8.3E+00					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1313-B03-C	1	8.13E+01			8.13E+01	2.9E+01	2.6E+00	8.3E+00					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	CFS-L10-1313-T01-A	1	1.60E+02			1.60E+02	1.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T02-A	1	4.40E+01			4.40E+01	1.4E+00	1.2E+00	3.8E+00	10	120	1.16E+03	93%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T03-A	1	4.29E+00			4.29E+00	1.5E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T04-A	1	6.00E-01	U1/2		6.00E-01	3.7E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T05-A	1	6.00E-01	U1/2		6.00E-01	2.1E+03	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T06-A	1	6.00E-01	U1/2		6.00E-01	1.5E+02	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T07-A	1	6.00E-01	U1/2		6.00E-01	2.3E+02	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T08-A	1	2.91E+01			2.91E+01	3.2E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T09-A	1	6.60E+02			6.60E+02	5.9E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T10-A	1	6.00E-01	U1/2		6.00E-01	2.8E+02	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T01-B	1	1.58E+02			1.58E+02	2.1E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T02-B	1	4.76E+01			4.76E+01	8.6E-01	1.2E+00	3.8E+00	10	120	1.20E+03	96%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T03-B	1	5.41E+00			5.41E+00	1.4E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T04-B	1	6.00E-01	U1/2		6.00E-01	8.9E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T05-B	1	6.00E-01	U1/2		6.00E-01	3.6E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T06-B	1	6.00E-01	U1/2		6.00E-01	1.1E+03	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T07-B	1	6.00E-01	U1/2		6.00E-01	1.1E+02	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T08-B	1	2.94E+01			2.94E+01	1.6E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T09-B	1	8.26E+02			8.26E+02	1.2E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T10-B	1	6.00E-01	U1/2		6.00E-01	2.8E+02	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T01-C	1	1.36E+02			1.36E+02	4.6E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T02-C	1	4.70E+01			4.70E+01	3.0E-01	1.2E+00	3.8E+00	10	120	1.09E+03	87%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T03-C	1	5.65E+00			5.65E+00	2.7E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T04-C	1	6.00E-01	U1/2		6.00E-01	9.6E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T05-C	1	6.00E-01	U1/2		6.00E-01	1.6E+02	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T06-C	1	6.00E-01	U1/2		6.00E-01	2.4E+02	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T07-C	1	6.00E-01	U1/2		6.00E-01	1.9E+02	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T08-C	1	3.49E+01			3.49E+01	1.0E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T09-C	1	7.61E+02			7.61E+02	2.9E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-T10-C	1	6.00E-01	U1/2		6.00E-01	8.9E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	1.5E+02	1.2E+00	3.8E+00					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	1.8E+02	1.2E+00	3.8E+00					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-B03-A	1	2.09E+00	E		2.09E+00	1.7E+01	1.2E+00	3.8E+00					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-B01-B	1	6.00E-01	U1/2		6.00E-01	6.2E+02	1.2E+00	3.8E+00					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-B02-B	1	6.00E-01	U1/2		6.00E-01	2.8E+01	1.2E+00	3.8E+00					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-B03-B	1	1.52E+00	E		1.52E+00	7.4E+01	1.2E+00	3.8E+00					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-B01-C	1	6.00E-01	U1/2		6.00E-01	1.6E+02	1.2E+00	3.8E+00					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-B02-C	1	6.00E-01	U1/2		6.00E-01	9.3E+00	1.2E+00	3.8E+00					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1313-B03-C	1	1.78E+00	E		1.78E+00	2.2E+01	1.2E+00	3.8E+00					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	CFS-L10-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	9.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	7.8E+01	1.8E+00	5.7E+00	10	120	1.11E+03	92%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	9.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	2.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T05-A	1	4.03E+01			4.03E+01	2.9E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T06-A	1	2.88E+02			2.88E+02	8.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T07-A	1	6.59E+02			6.59E+02	5.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T08-A	1	1.59E+03			1.59E+03	1.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T09-A	1	1.71E+03			1.71E+03	1.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T10-A	1	9.65E+01			9.65E+01	1.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	5.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	1.7E+02	1.8E+00	5.7E+00	10	120	1.14E+03	95%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	8.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T05-B	1	5.08E+01			5.08E+01	2.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T06-B	1	3.12E+02			3.12E+02	1.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T07-B	1	6.70E+02			6.70E+02	1.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T08-B	1	1.57E+03			1.57E+03	4.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T09-B	1	1.68E+03			1.68E+03	6.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T10-B	1	9.69E+01			9.69E+01	2.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	7.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	1.2E+03	1.8E+00	5.7E+00	10	120	1.23E+03	103%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	7.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	3.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T05-C	1	5.19E+01			5.19E+01	3.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T06-C	1	2.95E+02			2.95E+02	3.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T07-C	1	6.93E+02			6.93E+02	1.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T08-C	1	1.60E+03			1.60E+03	7.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T09-C	1	1.67E+03			1.67E+03	1.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-T10-C	1	1.02E+02			1.02E+02	1.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	6.3E+02	1.8E+00	5.7E+00					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	1.9E+02	1.8E+00	5.7E+00					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	6.0E+02	1.8E+00	5.7E+00					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-B01-B	1	9.00E-01	U1/2		9.00E-01	8.2E+01	1.8E+00	5.7E+00					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-B02-B	1	9.00E-01	U1/2		9.00E-01	3.9E+02	1.8E+00	5.7E+00					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-B03-B	1	9.00E-01	U1/2		9.00E-01	2.4E+02	1.8E+00	5.7E+00					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-B01-C	1	9.00E-01	U1/2		9.00E-01	4.2E+01	1.8E+00	5.7E+00					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-B02-C	1	9.00E-01	U1/2		9.00E-01	7.1E+01	1.8E+00	5.7E+00					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1313-B03-C	1	9.00E-01	U1/2		9.00E-01	2.7E+02	1.8E+00	5.7E+00					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	CFS-L10-1313-T01-A	1	8.63E+03			8.63E+03	3.9E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T02-A	1	6.69E+02			6.69E+02	1.1E+00	3.7E+00	1.2E+01	10	120	1.70E+03	86%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T03-A	1	1.05E+02			1.05E+02	1.3E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T04-A	1	4.71E+01			4.71E+01	3.6E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T05-A	1	1.71E+02			1.71E+02	3.5E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T06-A	1	3.00E+04			3.00E+04	2.9E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T07-A	1	2.42E+05			2.42E+05	9.6E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T08-A	1	8.91E+05			8.91E+05	5.0E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T09-A	1	1.03E+06			1.03E+06	1.8E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T10-A	1	7.52E+02			7.52E+02	1.0E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T01-B	1	8.38E+03			8.38E+03	1.9E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T02-B	1	6.26E+02			6.26E+02	4.1E-01	3.7E+00	1.2E+01	10	120	1.72E+03	91%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T03-B	1	1.25E+02			1.25E+02	6.5E-02	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T04-B	1	5.57E+01			5.57E+01	4.1E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T05-B	1	2.28E+02			2.28E+02	1.9E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T06-B	1	2.51E+04			2.51E+04	1.3E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T07-B	1	2.41E+05			2.41E+05	1.3E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T08-B	1	8.56E+05			8.56E+05	6.9E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T09-B	1	9.87E+05			9.87E+05	2.0E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T10-B	1	7.51E+02			7.51E+02	2.8E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T01-C	1	8.12E+03			8.12E+03	3.8E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T02-C	1	6.42E+02			6.42E+02	7.7E-01	3.7E+00	1.2E+01	10	120	1.71E+03	89%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T03-C	1	1.30E+02			1.30E+02	2.8E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T04-C	1	5.53E+01			5.53E+01	4.6E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T05-C	1	2.11E+02			2.11E+02	7.4E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T06-C	1	2.51E+04			2.51E+04	3.0E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T07-C	1	2.47E+05			2.47E+05	2.2E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T08-C	1	8.77E+05			8.77E+05	3.2E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T09-C	1	1.02E+06			1.02E+06	6.8E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-T10-C	1	8.12E+02			8.12E+02	1.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	1.9E+04	3.7E+00	1.2E+01					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-B02-A	1	7.31E+00	E		7.31E+00	1.1E+01	3.7E+00	1.2E+01					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-B03-A	1	1.85E+00	U1/2		1.85E+00	2.8E+01	3.7E+00	1.2E+01					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-B01-B	1	1.85E+00	U1/2		1.85E+00	6.2E+01	3.7E+00	1.2E+01					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-B02-B	1	1.85E+00	U1/2		1.85E+00	1.0E+01	3.7E+00	1.2E+01					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-B03-B	1	4.12E+00	E		4.12E+00	2.3E+01	3.7E+00	1.2E+01					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-B01-C	1	1.85E+00	U1/2		1.85E+00	6.3E+02	3.7E+00	1.2E+01					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-B02-C	1	4.30E+00	E		4.30E+00	9.2E+00	3.7E+00	1.2E+01					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1313-B03-C	1	1.85E+00	U1/2		1.85E+00	1.0E+02	3.7E+00	1.2E+01					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	CFS-L10-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	2.5E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00	1000	100	1.09E+03	109%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	2.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	3.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	6.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T07-A	1	6.20E+00	E		6.20E+00	1.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T08-A	1	2.31E+04			2.31E+04	1.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T09-A	1	1.89E+05			1.89E+05	9.1E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T10-A	1	1.00E+00	U1/2		1.00E+00	5.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	3.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	1.0E+01	2.0E+00	6.4E+00	1000	100	1.02E+03	102%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	9.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	7.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	3.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T07-B	1	6.63E+00			6.63E+00	1.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T08-B	1	2.02E+04			2.02E+04	3.0E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T09-B	1	1.75E+05			1.75E+05	1.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T10-B	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	1.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	3.0E+00	2.0E+00	6.4E+00	1000	100	1.04E+03	104%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	4.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	6.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	5.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T06-C	1	1.40E+01			1.40E+01	4.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T07-C	1	8.02E+00			8.02E+00	3.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T08-C	1	2.66E+04			2.66E+04	7.1E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T09-C	1	1.83E+05			1.83E+05	4.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-T10-C	1	1.00E+00	U1/2		1.00E+00	1.9E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-B02-A	1	3.15E+00	E		3.15E+00	1.8E+01	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-B03-A	1	2.60E+01			2.60E+01	1.5E+00	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-B02-B	1	4.02E+00	E		4.02E+00	3.3E+00	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-B03-B	1	2.50E+01			2.50E+01	7.2E+00	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-B01-C	1	2.05E+00	E		2.05E+00	1.5E+01	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-B02-C	1	6.89E+00			6.89E+00	4.8E+00	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1313-B03-C	1	2.56E+01			2.56E+01	3.5E+00	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	CFS-L10-1313-T01-A	1	1.23E+04			1.23E+04	1.5E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T02-A	1	9.43E+03			9.43E+03	1.4E+00	6.8E+00	2.2E+01	10	120	1.06E+04	94%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T03-A	1	2.75E+02			2.75E+02	2.9E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T04-A	1	7.11E+01			7.11E+01	2.8E+01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T05-A	1	7.12E+02			7.12E+02	4.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T06-A	1	2.65E+03			2.65E+03	8.8E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T07-A	1	5.80E+03			5.80E+03	4.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T08-A	1	5.17E+03			5.17E+03	1.6E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T09-A	1	5.93E+03			5.93E+03	3.3E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T10-A	1	9.15E+02			9.15E+02	4.3E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T01-B	1	1.32E+04			1.32E+04	2.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T02-B	1	9.50E+03			9.50E+03	7.1E-01	6.8E+00	2.2E+01	10	120	1.07E+04	97%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T03-B	1	2.33E+02			2.33E+02	1.8E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T04-B	1	5.93E+01			5.93E+01	6.7E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T05-B	1	8.09E+02			8.09E+02	7.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T06-B	1	2.45E+03			2.45E+03	9.3E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T07-B	1	6.05E+03			6.05E+03	7.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T08-B	1	6.13E+03			6.13E+03	8.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T09-B	1	6.01E+03			6.01E+03	1.4E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T10-B	1	9.02E+02			9.02E+02	3.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T01-C	1	1.21E+04			1.21E+04	6.9E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T02-C	1	9.46E+03			9.46E+03	2.0E+00	6.8E+00	2.2E+01	10	120	1.05E+04	89%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T03-C	1	2.27E+02			2.27E+02	3.4E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T04-C	1	7.84E+01			7.84E+01	5.9E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T05-C	1	7.72E+02			7.72E+02	5.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T06-C	1	2.46E+03			2.46E+03	4.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T07-C	1	7.04E+03			7.04E+03	1.8E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T08-C	1	5.32E+03			5.32E+03	9.8E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T09-C	1	5.92E+03			5.92E+03	4.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-T10-C	1	9.55E+02			9.55E+02	1.6E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	2.1E-01	6.8E+00	2.2E+01					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	5.4E+00	6.8E+00	2.2E+01					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	6.8E+00	6.8E+00	2.2E+01					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-B01-B	1	3.40E+00	U1/2		3.40E+00	1.6E+00	6.8E+00	2.2E+01					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-B02-B	1	3.40E+00	U1/2		3.40E+00	2.5E+00	6.8E+00	2.2E+01					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-B03-B	1	3.40E+00	U1/2		3.40E+00	8.5E+00	6.8E+00	2.2E+01					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-B01-C	1	3.40E+00	U1/2		3.40E+00	4.5E-01	6.8E+00	2.2E+01					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-B02-C	1	3.40E+00	U1/2		3.40E+00	3.3E+00	6.8E+00	2.2E+01					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1313-B03-C	1	3.40E+00	U1/2		3.40E+00	5.5E+00	6.8E+00	2.2E+01					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	CFS-L10-1313-T01-A	1	9.42E+00			9.42E+00	4.2E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T02-A	1	1.13E+01			1.13E+01	2.4E+00	1.9E+00	6.0E+00	10	120	1.10E+03	90%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T03-A	1	1.17E+01			1.17E+01	8.5E-01	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T04-A	1	9.94E+00			9.94E+00	4.8E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T05-A	1	7.58E+00			7.58E+00	1.2E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T06-A	1	9.25E+00			9.25E+00	9.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T07-A	1	1.14E+01			1.14E+01	4.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T08-A	1	1.17E+01			1.17E+01	1.2E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T09-A	1	2.06E+01			2.06E+01	6.0E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T10-A	1	9.00E+00			9.00E+00	2.5E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T01-B	1	9.70E+00			9.70E+00	3.3E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T02-B	1	1.22E+01			1.22E+01	1.6E+00	1.9E+00	6.0E+00	10	120	1.02E+03	84%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T03-B	1	1.10E+01			1.10E+01	2.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T04-B	1	1.10E+01			1.10E+01	1.3E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T05-B	1	9.69E+00			9.69E+00	4.5E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T06-B	1	8.75E+00			8.75E+00	3.8E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T07-B	1	1.05E+01			1.05E+01	1.1E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T08-B	1	1.52E+01			1.52E+01	1.4E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T09-B	1	2.05E+01			2.05E+01	1.9E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T10-B	1	9.99E+00			9.99E+00	4.9E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T01-C	1	9.58E+00			9.58E+00	5.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T02-C	1	1.11E+01			1.11E+01	3.3E+00	1.9E+00	6.0E+00	10	120	1.06E+03	87%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T03-C	1	1.27E+01			1.27E+01	2.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T04-C	1	1.24E+01			1.24E+01	3.0E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T05-C	1	1.22E+01			1.22E+01	7.8E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T06-C	1	1.02E+01			1.02E+01	8.2E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T07-C	1	1.01E+01			1.01E+01	9.5E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T08-C	1	9.69E+00			9.69E+00	1.8E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T09-C	1	1.94E+01			1.94E+01	1.1E+01	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-T10-C	1	1.04E+01			1.04E+01	5.9E+00	1.9E+00	6.0E+00			---		VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	6.1E+00	1.9E+00	6.0E+00					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	5.2E+00	1.9E+00	6.0E+00					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	1.6E+00	1.9E+00	6.0E+00					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-B01-B	1	9.50E-01	U1/2		9.50E-01	1.9E+00	1.9E+00	6.0E+00					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-B02-B	1	9.50E-01	U1/2		9.50E-01	3.7E+00	1.9E+00	6.0E+00					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-B03-B	1	9.50E-01	U1/2		9.50E-01	2.5E+00	1.9E+00	6.0E+00					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-B01-C	1	9.50E-01	U1/2		9.50E-01	2.4E+00	1.9E+00	6.0E+00					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-B02-C	1	9.50E-01	U1/2		9.50E-01	1.8E+00	1.9E+00	6.0E+00					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1313-B03-C	1	9.50E-01	U1/2		9.50E-01	2.4E+00	1.9E+00	6.0E+00					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	CFS-L10-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	5.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	4.8E+01	2.0E+00	6.4E+00	10	120	1.09E+03	90%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	4.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T04-A	1	1.96E+01			1.96E+01	1.9E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T05-A	1	8.56E+02			8.56E+02	1.9E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T06-A	1	3.45E+03			3.45E+03	1.5E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T07-A	1	7.26E+03			7.26E+03	6.0E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T08-A	1	2.03E+04			2.03E+04	1.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T09-A	1	2.84E+04			2.84E+04	7.3E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T10-A	1	1.52E+03			1.52E+03	1.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	7.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00	10	120	1.12E+03	93%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	6.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T04-B	1	2.48E+01			2.48E+01	7.8E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T05-B	1	1.03E+03			1.03E+03	9.0E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T06-B	1	3.71E+03			3.71E+03	7.8E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T07-B	1	7.65E+03			7.65E+03	3.0E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T08-B	1	2.04E+04			2.04E+04	4.4E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T09-B	1	2.77E+04			2.77E+04	2.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T10-B	1	1.55E+03			1.55E+03	7.6E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	5.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	4.0E+01	2.0E+00	6.4E+00	10	120	1.09E+03	91%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	4.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T04-C	1	3.82E+01			3.82E+01	1.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T05-C	1	1.08E+03			1.08E+03	5.6E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T06-C	1	3.42E+03			3.42E+03	4.9E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T07-C	1	7.70E+03			7.70E+03	9.8E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T08-C	1	2.06E+04			2.06E+04	4.0E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T09-C	1	2.80E+04			2.80E+04	2.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-T10-C	1	1.61E+03			1.61E+03	9.4E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	2.5E+02	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	4.3E+01	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	1.6E+02	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	3.9E+01	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	5.5E+01	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	4.7E-01	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1313-B03-C	1	1.00E+00	U1/2		1.00E+00	7.3E+00	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	CFS-L10-1313-T01-A	1	2.96E+01			2.96E+01	2.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T02-A	1	4.22E+01			4.22E+01	2.0E+01	1.0E+00	3.2E+00	1000	100	1.15E+03	110%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T03-A	1	4.00E+03			4.00E+03	1.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T04-A	1	4.95E+04			4.95E+04	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T05-A	1	6.74E+04			6.74E+04	2.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T06-A	1	6.53E+04			6.53E+04	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T07-A	1	7.23E+04			7.23E+04	2.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T08-A	1	1.15E+05			1.15E+05	5.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T09-A	1	2.29E+05			2.29E+05	3.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T10-A	1	6.78E+04			6.78E+04	6.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T01-B	1	2.68E+01			2.68E+01	3.1E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T02-B	1	3.05E+01			3.05E+01	8.1E+00	1.0E+00	3.2E+00	1000	100	1.16E+03	113%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T03-B	1	3.64E+03			3.64E+03	1.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T04-B	1	5.39E+04			5.39E+04	8.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T05-B	1	7.05E+04			7.05E+04	4.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T06-B	1	7.26E+04			7.26E+04	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T07-B	1	7.69E+04			7.69E+04	5.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T08-B	1	1.29E+05			1.29E+05	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T09-B	1	2.16E+05			2.16E+05	7.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T10-B	1	6.92E+04			6.92E+04	9.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T01-C	1	3.04E+01			3.04E+01	1.1E+01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T02-C	1	3.75E+01			3.75E+01	1.9E+01	1.0E+00	3.2E+00	1000	100	1.18E+03	114%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T03-C	1	4.10E+03			4.10E+03	9.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T04-C	1	5.50E+04			5.50E+04	8.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T05-C	1	6.66E+04			6.66E+04	6.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T06-C	1	6.94E+04			6.94E+04	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T07-C	1	8.04E+04			8.04E+04	5.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T08-C	1	1.16E+05			1.16E+05	7.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T09-C	1	2.05E+05			2.05E+05	3.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-T10-C	1	6.97E+04			6.97E+04	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-B01-A	1	1.13E+00	E		1.13E+00	9.1E+02	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	5.2E+01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-B03-A	1	1.65E+01			1.65E+01	2.5E+01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	1.7E+02	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	1.2E+02	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-B03-B	1	1.75E+01			1.75E+01	1.3E+01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-B01-C	1	1.91E+00	E		1.91E+00	4.5E+02	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-B02-C	1	6.67E+00			6.67E+00	1.5E+02	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1313-B03-C	1	6.64E+00			6.64E+00	1.7E+02	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	CFS-L10-1313-T01-A	1	1.65E+03			1.65E+03	1.2E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T02-A	1	1.63E+03			1.63E+03	4.2E-01	1.2E+00	3.8E+00	10	120	2.70E+03	88%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T03-A	1	9.37E+02			9.37E+02	1.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T04-A	1	1.33E+02			1.33E+02	2.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T05-A	1	1.81E+01			1.81E+01	5.7E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T06-A	1	6.00E+00			6.00E+00	3.0E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T07-A	1	5.24E+00			5.24E+00	5.6E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T08-A	1	6.60E+00			6.60E+00	3.1E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T09-A	1	3.27E+01			3.27E+01	5.6E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T10-A	1	9.66E+00			9.66E+00	1.2E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T01-B	1	1.89E+03			1.89E+03	1.0E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T02-B	1	1.76E+03			1.76E+03	4.9E-01	1.2E+00	3.8E+00	10	120	2.87E+03	93%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T03-B	1	1.03E+03			1.03E+03	1.4E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T04-B	1	1.23E+02			1.23E+02	1.4E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T05-B	1	1.69E+01			1.69E+01	6.4E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T06-B	1	7.17E+00			7.17E+00	5.5E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T07-B	1	5.39E+00			5.39E+00	3.1E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T08-B	1	8.63E+00			8.63E+00	1.4E+02	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T09-B	1	2.64E+01			2.64E+01	2.7E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T10-B	1	8.16E+00			8.16E+00	9.3E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T01-C	1	1.77E+03			1.77E+03	1.7E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T02-C	1	1.82E+03			1.82E+03	1.5E+00	1.2E+00	3.8E+00	10	120	2.90E+03	89%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T03-C	1	1.05E+03			1.05E+03	1.4E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T04-C	1	1.15E+02			1.15E+02	8.4E-01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T05-C	1	1.75E+01			1.75E+01	5.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T06-C	1	4.79E+00			4.79E+00	2.1E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T07-C	1	3.50E+00	E		3.50E+00	7.8E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T08-C	1	9.33E+00			9.33E+00	3.9E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T09-C	1	2.24E+01			2.24E+01	4.1E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-T10-C	1	9.32E+00			9.32E+00	1.4E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	2.5E+02	1.2E+00	3.8E+00					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	1.3E+02	1.2E+00	3.8E+00					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-B03-A	1	3.06E+00	E		3.06E+00	8.1E+01	1.2E+00	3.8E+00					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-B01-B	1	6.00E-01	U1/2		6.00E-01	1.2E+02	1.2E+00	3.8E+00					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-B02-B	1	6.00E-01	U1/2		6.00E-01	8.3E+01	1.2E+00	3.8E+00					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-B03-B	1	1.43E+00	E		1.43E+00	1.3E+02	1.2E+00	3.8E+00					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-B01-C	1	6.00E-01	U1/2		6.00E-01	1.7E+03	1.2E+00	3.8E+00					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-B02-C	1	6.00E-01	U1/2		6.00E-01	1.4E+02	1.2E+00	3.8E+00					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1313-B03-C	1	6.00E-01	U1/2		6.00E-01	9.1E+01	1.2E+00	3.8E+00					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	CFS-L10-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	6.8E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/17/11 12:16 PM	EPA Interlab 1313-1316 CFS Reruns
Ni	CFS-L10-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	4.4E+02	1.8E+00	5.7E+00	10	120	1.12E+03	94%	VU ICP-OES	6/17/11 12:18 PM	EPA Interlab 1313-1316 CFS Reruns
Ni	CFS-L10-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	3.3E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/17/11 12:21 PM	EPA Interlab 1313-1316 CFS Reruns
Ni	CFS-L10-1313-T04-A	1	3.27E+00	E		3.27E+00	1.5E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-T05-A	1	7.73E+01			7.73E+01	3.8E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-T06-A	1	8.45E+02			8.45E+02	5.3E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-T07-A	1	2.24E+03			2.24E+03	3.7E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-T08-A	1	6.00E+03			6.00E+03	1.3E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-T09-A	1	6.58E+03			6.58E+03	1.3E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-T10-A	1	2.03E+02			2.03E+02	7.8E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	8.2E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00	10	120	1.16E+03	97%	VU ICP-OES	6/17/11 12:38 PM	EPA Interlab 1313-1316 CFS Reruns
Ni	CFS-L10-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	4.6E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/17/11 12:41 PM	EPA Interlab 1313-1316 CFS Reruns
Ni	CFS-L10-1313-T04-B	1	2.97E+00	E		2.97E+00	2.8E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/17/11 12:43 PM	EPA Interlab 1313-1316 CFS Reruns
Ni	CFS-L10-1313-T05-B	1	9.92E+01			9.92E+01	2.0E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-T06-B	1	9.11E+02			9.11E+02	1.0E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-T07-B	1	2.25E+03			2.25E+03	6.7E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-T08-B	1	5.89E+03			5.89E+03	3.5E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-T09-B	1	6.30E+03			6.30E+03	7.0E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-T10-B	1	2.05E+02			2.05E+02	1.5E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	7.3E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	2.8E+02	1.8E+00	5.7E+00	10	120	1.11E+03	92%	VU ICP-OES	6/17/11 1:00 PM	EPA Interlab 1313-1316 CFS Reruns
Ni	CFS-L10-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	4.3E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/17/11 1:02 PM	EPA Interlab 1313-1316 CFS Reruns
Ni	CFS-L10-1313-T04-C	1	3.35E+00	E		3.35E+00	2.5E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/17/11 1:04 PM	EPA Interlab 1313-1316 CFS Reruns
Ni	CFS-L10-1313-T05-C	1	9.83E+01			9.83E+01	1.5E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-T06-C	1	8.61E+02			8.61E+02	3.3E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-T07-C	1	2.33E+03			2.33E+03	2.0E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-T08-C	1	6.00E+03			6.00E+03	9.5E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-T09-C	1	6.35E+03			6.35E+03	1.1E+00	1.8E+00	5.7E+00			---		VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-T10-C	1	2.18E+02			2.18E+02	4.6E-01	1.8E+00	5.7E+00			---		VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	3.1E+02	1.8E+00	5.7E+00					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	1.8E+02	1.8E+00	5.7E+00					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	9.5E+01	1.8E+00	5.7E+00					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-B01-B	1	9.00E-01	U1/2		9.00E-01	2.4E+02	1.8E+00	5.7E+00					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-B02-B	1	9.00E-01	U1/2		9.00E-01	2.4E+03	1.8E+00	5.7E+00					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-B03-B	1	2.14E+00	E		2.14E+00	5.1E+01	1.8E+00	5.7E+00					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-B01-C	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-B02-C	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1313-B03-C	1	9.00E-01	U1/2		9.00E-01	1.6E+02	1.8E+00	5.7E+00					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	CFS-L10-1313-T01-A	1	6.79E+01			6.79E+01	2.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T02-A	1	5.40E+01			5.40E+01	1.2E+01	3.7E+00	1.2E+01	1000	100	1.23E+03	117%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T03-A	1	9.82E+00	E		9.82E+00	9.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T04-A	1	1.85E+00	U1/2		1.85E+00	6.9E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T05-A	1	1.85E+00	U1/2		1.85E+00	1.0E+02	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T06-A	1	1.85E+00	U1/2		1.85E+00	2.6E+02	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T07-A	1	1.85E+00	U1/2		1.85E+00	2.9E+02	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T08-A	1	1.85E+00	U1/2		1.85E+00	6.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T09-A	1	2.42E+02			2.42E+02	7.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T10-A	1	1.85E+00	U1/2		1.85E+00	1.2E+02	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T01-B	1	8.26E+01			8.26E+01	1.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T02-B	1	6.16E+01			6.16E+01	1.5E+01	3.7E+00	1.2E+01	1000	100	1.26E+03	119%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T03-B	1	2.53E+01			2.53E+01	3.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T04-B	1	1.85E+00	U1/2		1.85E+00	1.2E+02	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T05-B	1	1.85E+00	U1/2		1.85E+00	2.9E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T06-B	1	1.85E+00	U1/2		1.85E+00	8.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T07-B	1	1.85E+00	U1/2		1.85E+00	9.6E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T08-B	1	1.85E+00	U1/2		1.85E+00	5.8E+02	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T09-B	1	2.87E+02			2.87E+02	5.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T10-B	1	1.85E+00	U1/2		1.85E+00	3.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T01-C	1	1.06E+02			1.06E+02	4.2E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T02-C	1	7.71E+01			7.71E+01	2.5E+01	3.7E+00	1.2E+01	1000	100	1.16E+03	108%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T03-C	1	1.65E+01			1.65E+01	1.3E+02	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T04-C	1	1.85E+00	U1/2		1.85E+00	8.9E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T05-C	1	1.85E+00	U1/2		1.85E+00	2.0E+02	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T06-C	1	1.85E+00	U1/2		1.85E+00	2.5E+02	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T07-C	1	1.85E+00	U1/2		1.85E+00	1.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T08-C	1	1.85E+00	U1/2		1.85E+00	4.9E+02	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T09-C	1	2.63E+02			2.63E+02	8.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-T10-C	1	1.85E+00	U1/2		1.85E+00	5.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	8.4E+01	3.7E+00	1.2E+01					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	3.1E+01	3.7E+00	1.2E+01					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-B03-A	1	7.14E+00	E		7.14E+00	1.2E+02	3.7E+00	1.2E+01					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-B01-B	1	1.85E+00	U1/2		1.85E+00	2.0E+02	3.7E+00	1.2E+01					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-B02-B	1	1.85E+00	U1/2		1.85E+00	4.9E+01	3.7E+00	1.2E+01					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-B03-B	1	1.85E+00	U1/2		1.85E+00	2.6E+02	3.7E+00	1.2E+01					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-B01-C	1	1.85E+00	U1/2		1.85E+00	7.5E+01	3.7E+00	1.2E+01					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-B02-C	1	1.85E+00	U1/2		1.85E+00	5.6E+01	3.7E+00	1.2E+01					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1313-B03-C	1	1.85E+00	U1/2		1.85E+00	1.9E+03	3.7E+00	1.2E+01					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	CFS-L10-1313-T01-A	1	3.67E+04			3.67E+04	4.9E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T02-A	1	1.58E+04			1.58E+04	7.2E-01	1.6E+00	5.1E+00	1000	100	1.67E+04	92%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T03-A	1	1.26E+04			1.26E+04	7.4E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T04-A	1	1.09E+04			1.09E+04	7.7E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T05-A	1	9.83E+03			9.83E+03	9.0E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T06-A	1	9.93E+03			9.93E+03	7.2E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T07-A	1	1.16E+04			1.16E+04	5.9E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T08-A	1	1.60E+04			1.60E+04	9.0E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T09-A	1	2.17E+04			2.17E+04	1.9E+00	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T10-A	1	9.02E+03			9.02E+03	6.9E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T01-B	1	3.73E+04			3.73E+04	6.7E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T02-B	1	1.54E+04			1.54E+04	5.4E-01	1.6E+00	5.1E+00	1000	100	1.63E+04	91%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T03-B	1	1.27E+04			1.27E+04	4.7E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T04-B	1	1.09E+04			1.09E+04	4.9E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T05-B	1	1.02E+04			1.02E+04	6.4E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T06-B	1	1.05E+04			1.05E+04	1.3E+00	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T07-B	1	1.15E+04			1.15E+04	3.2E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T08-B	1	1.55E+04			1.55E+04	2.1E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T09-B	1	2.08E+04			2.08E+04	9.3E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T10-B	1	8.92E+03			8.92E+03	3.9E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T01-C	1	3.71E+04			3.71E+04	3.9E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T02-C	1	1.58E+04			1.58E+04	1.3E+00	1.6E+00	5.1E+00	1000	100	1.66E+04	87%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T03-C	1	1.30E+04			1.30E+04	3.8E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T04-C	1	1.15E+04			1.15E+04	7.0E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T05-C	1	1.01E+04			1.01E+04	6.4E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T06-C	1	9.95E+03			9.95E+03	1.6E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T07-C	1	1.19E+04			1.19E+04	1.1E+00	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T08-C	1	1.55E+04			1.55E+04	6.0E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T09-C	1	2.06E+04			2.06E+04	6.1E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-T10-C	1	9.12E+03			9.12E+03	5.1E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-B01-A	1	2.84E+01			2.84E+01	1.8E+01	1.6E+00	5.1E+00					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-B02-A	1	3.18E+01			3.18E+01	1.4E+01	1.6E+00	5.1E+00					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-B03-A	1	2.05E+03			2.05E+03	8.0E-01	1.6E+00	5.1E+00					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-B01-B	1	4.53E+01			4.53E+01	2.0E+00	1.6E+00	5.1E+00					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-B02-B	1	9.85E+01			9.85E+01	2.0E+00	1.6E+00	5.1E+00					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-B03-B	1	2.25E+03			2.25E+03	6.3E+00	1.6E+00	5.1E+00					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-B01-C	1	8.83E+01			8.83E+01	1.2E+00	1.6E+00	5.1E+00					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-B02-C	1	2.85E+01			2.85E+01	1.2E+01	1.6E+00	5.1E+00					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1313-B03-C	1	2.07E+03			2.07E+03	1.2E+00	1.6E+00	5.1E+00					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	CFS-L10-1313-T01-A	1	6.63E+02			6.63E+02	2.2E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T02-A	1	5.68E+02			5.68E+02	3.2E+00	1.5E+01	4.8E+01	10	120	1.65E+03	90%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T03-A	1	3.89E+02			3.89E+02	3.8E-01	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T04-A	1	1.19E+02			1.19E+02	2.0E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T05-A	1	8.39E+01			8.39E+01	2.2E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T06-A	1	8.53E+01			8.53E+01	1.5E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T07-A	1	1.32E+02			1.32E+02	9.7E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T08-A	1	2.28E+02			2.28E+02	4.2E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T09-A	1	2.92E+02			2.92E+02	2.3E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T10-A	1	8.94E+01			8.94E+01	1.2E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T01-B	1	6.33E+02			6.33E+02	1.3E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T02-B	1	5.82E+02			5.82E+02	1.9E+00	1.5E+01	4.8E+01	10	120	1.69E+03	92%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T03-B	1	3.90E+02			3.90E+02	5.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T04-B	1	1.22E+02			1.22E+02	1.3E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T05-B	1	8.46E+01			8.46E+01	1.0E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T06-B	1	7.87E+01			7.87E+01	2.5E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T07-B	1	1.27E+02			1.27E+02	2.6E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T08-B	1	2.38E+02			2.38E+02	8.7E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T09-B	1	2.79E+02			2.79E+02	1.6E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T10-B	1	7.56E+01			7.56E+01	1.7E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T01-C	1	7.80E+02			7.80E+02	2.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T02-C	1	6.71E+02			6.71E+02	3.8E+00	1.5E+01	4.8E+01	10	120	1.71E+03	87%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T03-C	1	3.87E+02			3.87E+02	5.4E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T04-C	1	1.12E+02			1.12E+02	6.8E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T05-C	1	7.83E+01			7.83E+01	1.7E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T06-C	1	1.13E+02			1.13E+02	2.0E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T07-C	1	1.80E+02			1.80E+02	2.7E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T08-C	1	2.58E+02			2.58E+02	1.3E+01	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T09-C	1	2.74E+02			2.74E+02	2.6E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-T10-C	1	7.54E+01			7.54E+01	2.8E+00	1.5E+01	4.8E+01			---		VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-B01-A	1	7.50E+00	U1/2		7.50E+00	3.1E+02	1.5E+01	4.8E+01					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-B02-A	1	7.50E+00	U1/2		7.50E+00	1.2E+02	1.5E+01	4.8E+01					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-B03-A	1	7.50E+00	U1/2		7.50E+00	5.7E+01	1.5E+01	4.8E+01					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-B01-B	1	7.50E+00	U1/2		7.50E+00	5.9E+01	1.5E+01	4.8E+01					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-B02-B	1	7.50E+00	U1/2		7.50E+00	3.9E+02	1.5E+01	4.8E+01					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-B03-B	1	7.50E+00	U1/2		7.50E+00	7.9E+01	1.5E+01	4.8E+01					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-B01-C	1	7.50E+00	U1/2		7.50E+00	2.9E+02	1.5E+01	4.8E+01					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-B02-C	1	7.50E+00	U1/2		7.50E+00	9.6E+01	1.5E+01	4.8E+01					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1313-B03-C	1	7.50E+00	U1/2		7.50E+00	4.9E+02	1.5E+01	4.8E+01					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	CFS-L10-1313-T01-A	1	3.93E+02			3.93E+02	2.5E+00	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T02-A	1	2.51E+02			2.51E+02	3.2E+00	1.1E+00	3.5E+00	1000	100	1.32E+03	106%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T03-A	1	4.60E+02			4.60E+02	9.1E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T04-A	1	7.20E+02			7.20E+02	4.2E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T05-A	1	2.26E+03			2.26E+03	5.5E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T06-A	1	1.10E+04			1.10E+04	1.1E+00	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T07-A	1	2.50E+04			2.50E+04	1.1E+00	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T08-A	1	5.81E+04			5.81E+04	9.9E-02	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T09-A	1	1.37E+05			1.37E+05	1.1E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T10-A	1	3.83E+03			3.83E+03	1.1E+00	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T01-B	1	3.80E+02			3.80E+02	4.9E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T02-B	1	2.85E+02			2.85E+02	7.1E-01	1.1E+00	3.5E+00	1000	100	1.29E+03	100%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T03-B	1	4.99E+02			4.99E+02	9.3E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T04-B	1	8.75E+02			8.75E+02	2.8E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T05-B	1	2.67E+03			2.67E+03	1.8E+00	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T06-B	1	1.20E+04			1.20E+04	1.1E+00	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T07-B	1	2.52E+04			2.52E+04	1.5E+00	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T08-B	1	5.57E+04			5.57E+04	3.8E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T09-B	1	1.30E+05			1.30E+05	5.6E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T10-B	1	3.67E+03			3.67E+03	3.9E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T01-C	1	3.77E+02			3.77E+02	1.1E+00	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T02-C	1	3.33E+02			3.33E+02	1.5E+00	1.1E+00	3.5E+00	1000	100	1.28E+03	95%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T03-C	1	5.08E+02			5.08E+02	1.3E+00	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T04-C	1	9.63E+02			9.63E+02	6.5E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T05-C	1	2.49E+03			2.49E+03	2.1E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T06-C	1	1.10E+04			1.10E+04	4.7E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T07-C	1	2.64E+04			2.64E+04	2.0E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T08-C	1	5.86E+04			5.86E+04	4.1E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T09-C	1	1.34E+05			1.34E+05	6.6E-01	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-T10-C	1	3.90E+03			3.90E+03	1.1E+00	1.1E+00	3.5E+00			---		VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-B01-A	1	7.71E+00			7.71E+00	2.1E+01	1.1E+00	3.5E+00					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-B02-A	1	7.29E+00			7.29E+00	3.3E+01	1.1E+00	3.5E+00					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-B03-A	1	4.27E+02			4.27E+02	1.1E+01	1.1E+00	3.5E+00					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-B01-B	1	7.93E+00			7.93E+00	1.2E+01	1.1E+00	3.5E+00					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-B02-B	1	1.10E+01			1.10E+01	9.5E+00	1.1E+00	3.5E+00					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-B03-B	1	7.33E+02			7.33E+02	8.6E+00	1.1E+00	3.5E+00					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-B01-C	1	1.39E+01			1.39E+01	1.2E+01	1.1E+00	3.5E+00					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-B02-C	1	9.98E+00			9.98E+00	3.4E+01	1.1E+00	3.5E+00					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1313-B03-C	1	8.11E+02			8.11E+02	6.7E+00	1.1E+00	3.5E+00					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	CFS-L10-1313-T01-A	1	6.21E+05			6.21E+05	2.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T02-A	1	3.46E+05			3.46E+05	1.5E-01	2.5E+00	8.0E+00	1000	100	3.47E+05	92%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T03-A	1	2.19E+05			2.19E+05	3.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T04-A	1	1.32E+05			1.32E+05	5.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T05-A	1	6.38E+04			6.38E+04	8.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T06-A	1	1.88E+04			1.88E+04	1.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T07-A	1	2.05E+04			2.05E+04	3.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T08-A	1	2.44E+04			2.44E+04	1.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T09-A	1	2.82E+04			2.82E+04	5.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T10-A	1	1.80E+04			1.80E+04	8.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T01-B	1	6.14E+05			6.14E+05	2.7E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T02-B	1	3.34E+05			3.34E+05	5.0E-01	2.5E+00	8.0E+00	1000	100	3.35E+05	88%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T03-B	1	2.19E+05			2.19E+05	8.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T04-B	1	1.31E+05			1.31E+05	2.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T05-B	1	6.15E+04			6.15E+04	2.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T06-B	1	1.92E+04			1.92E+04	9.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T07-B	1	1.96E+04			1.96E+04	4.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T08-B	1	2.35E+04			2.35E+04	9.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T09-B	1	2.64E+04			2.64E+04	3.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T10-B	1	1.84E+04			1.84E+04	6.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T01-C	1	6.21E+05			6.21E+05	3.6E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T02-C	1	3.30E+05			3.30E+05	6.0E-01	2.5E+00	8.0E+00	1000	100	3.31E+05	84%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T03-C	1	2.13E+05			2.13E+05	3.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T04-C	1	1.27E+05			1.27E+05	7.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T05-C	1	6.20E+04			6.20E+04	4.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T06-C	1	1.87E+04			1.87E+04	2.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T07-C	1	1.99E+04			1.99E+04	8.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T08-C	1	2.32E+04			2.32E+04	9.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T09-C	1	2.54E+04			2.54E+04	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-T10-C	1	1.73E+04			1.73E+04	6.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-B01-A	1	5.77E+01			5.77E+01	3.2E+00	2.5E+00	8.0E+00					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-B02-A	1	6.71E+01			6.71E+01	3.7E+00	2.5E+00	8.0E+00					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-B03-A	1	6.23E+05			6.23E+05	1.2E+00	2.5E+00	8.0E+00					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-B01-B	1	1.60E+02			1.60E+02	3.4E+00	2.5E+00	8.0E+00					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-B02-B	1	9.99E+01			9.99E+01	5.3E+00	2.5E+00	8.0E+00					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-B03-B	1	6.28E+05			6.28E+05	2.8E+00	2.5E+00	8.0E+00					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-B01-C	1	2.06E+02			2.06E+02	2.5E+00	2.5E+00	8.0E+00					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-B02-C	1	6.67E+01			6.67E+01	3.1E+00	2.5E+00	8.0E+00					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1313-B03-C	1	6.33E+05			6.33E+05	1.0E+00	2.5E+00	8.0E+00					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	CFS-L10-1313-T01-A	1	3.07E+03			3.07E+03	6.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T02-A	1	3.35E+03			3.35E+03	1.6E+00	1.0E+00	3.2E+00	1000	100	4.25E+03	90%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T03-A	1	3.81E+03			3.81E+03	5.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T04-A	1	3.07E+03			3.07E+03	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T05-A	1	2.46E+03			2.46E+03	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T06-A	1	8.91E+02			8.91E+02	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T07-A	1	9.55E+02			9.55E+02	2.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T08-A	1	1.10E+03			1.10E+03	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T09-A	1	1.30E+03			1.30E+03	2.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T10-A	1	1.46E+03			1.46E+03	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T01-B	1	2.98E+03			2.98E+03	6.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T02-B	1	3.19E+03			3.19E+03	8.8E-01	1.0E+00	3.2E+00	1000	100	4.13E+03	94%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T03-B	1	3.56E+03			3.56E+03	9.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T04-B	1	3.39E+03			3.39E+03	1.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T05-B	1	2.40E+03			2.40E+03	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T06-B	1	9.42E+02			9.42E+02	8.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T07-B	1	9.82E+02			9.82E+02	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T08-B	1	1.07E+03			1.07E+03	8.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T09-B	1	1.22E+03			1.22E+03	1.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T10-B	1	1.41E+03			1.41E+03	2.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T01-C	1	2.95E+03			2.95E+03	4.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T02-C	1	3.41E+03			3.41E+03	1.9E+00	1.0E+00	3.2E+00	1000	100	4.34E+03	93%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T03-C	1	3.76E+03			3.76E+03	6.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T04-C	1	3.52E+03			3.52E+03	4.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T05-C	1	2.38E+03			2.38E+03	5.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T06-C	1	8.80E+02			8.80E+02	5.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T07-C	1	1.05E+03			1.05E+03	1.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T08-C	1	1.14E+03			1.14E+03	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T09-C	1	1.44E+03			1.44E+03	7.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-T10-C	1	1.45E+03			1.45E+03	9.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	3.9E+03	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	2.6E+02	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-B03-A	1	1.44E+01			1.44E+01	5.2E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-B01-B	1	5.00E-01	U1/2		5.00E-01	1.7E+02	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-B02-B	1	5.00E-01	U1/2		5.00E-01	2.1E+02	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-B03-B	1	1.54E+01			1.54E+01	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-B01-C	1	5.00E-01	U1/2		5.00E-01	8.1E+01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-B02-C	1	5.00E-01	U1/2		5.00E-01	1.6E+02	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1313-B03-C	1	1.72E+01			1.72E+01	2.6E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	CFS-L10-1313-T01-A	1	1.47E+06			1.47E+06	3.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T02-A	1	9.43E+05			9.43E+05	6.6E-01	6.8E+00	2.2E+01	1000	100	9.44E+05	85%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T03-A	1	7.39E+05			7.39E+05	7.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T04-A	1	6.58E+05			6.58E+05	8.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T05-A	1	6.06E+05			6.06E+05	1.0E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T06-A	1	5.62E+05			5.62E+05	5.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T07-A	1	5.97E+05			5.97E+05	6.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T08-A	1	6.77E+05			6.77E+05	5.3E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T09-A	1	7.26E+05			7.26E+05	5.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T10-A	1	5.75E+05			5.75E+05	5.8E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T01-B	1	1.47E+06			1.47E+06	1.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T02-B	1	9.22E+05			9.22E+05	4.7E-01	6.8E+00	2.2E+01	1000	100	9.23E+05	88%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T03-B	1	7.41E+05			7.41E+05	7.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T04-B	1	6.55E+05			6.55E+05	4.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T05-B	1	6.04E+05			6.04E+05	1.0E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T06-B	1	5.85E+05			5.85E+05	9.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T07-B	1	5.95E+05			5.95E+05	4.3E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T08-B	1	6.58E+05			6.58E+05	2.7E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T09-B	1	6.98E+05			6.98E+05	1.0E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T10-B	1	5.70E+05			5.70E+05	3.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T01-C	1	1.44E+06			1.44E+06	4.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T02-C	1	9.38E+05			9.38E+05	1.3E+00	6.8E+00	2.2E+01	1000	100	9.39E+05	84%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T03-C	1	7.61E+05			7.61E+05	3.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T04-C	1	6.78E+05			6.78E+05	8.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T05-C	1	6.17E+05			6.17E+05	7.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T06-C	1	5.57E+05			5.57E+05	4.9E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T07-C	1	6.16E+05			6.16E+05	1.2E+00	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T08-C	1	6.73E+05			6.73E+05	4.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T09-C	1	6.96E+05			6.96E+05	3.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-T10-C	1	5.85E+05			5.85E+05	2.8E-01	6.8E+00	2.2E+01			---		VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-B01-A	1	2.16E+01	E		2.16E+01	8.0E+00	6.8E+00	2.2E+01					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-B02-A	1	9.09E+01			9.09E+01	1.2E+01	6.8E+00	2.2E+01					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-B03-A	1	5.21E+02			5.21E+02	2.7E+01	6.8E+00	2.2E+01					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-B01-B	1	4.05E+02			4.05E+02	1.4E+01	6.8E+00	2.2E+01					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-B02-B	1	2.58E+02			2.58E+02	3.1E+00	6.8E+00	2.2E+01					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-B03-B	1	2.37E+02			2.37E+02	1.2E+01	6.8E+00	2.2E+01					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-B01-C	1	2.24E+02			2.24E+02	5.4E+00	6.8E+00	2.2E+01					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-B02-C	1	1.09E+02			1.09E+02	1.1E+01	6.8E+00	2.2E+01					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1313-B03-C	1	4.23E+02			4.23E+02	7.1E+00	6.8E+00	2.2E+01					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

TI	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	CFS-L10-1313-T01-A	1	9.26E+01			9.26E+01	4.0E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T02-A	1	6.74E+01			6.74E+01	1.2E+01	4.6E+00	1.5E+01	10	120	1.09E+03	85%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T03-A	1	1.32E+02			1.32E+02	4.3E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T04-A	1	2.14E+02			2.14E+02	6.1E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T05-A	1	2.93E+02			2.93E+02	2.7E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T06-A	1	3.90E+02			3.90E+02	1.3E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T07-A	1	5.46E+02			5.46E+02	1.3E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T08-A	1	8.71E+02			8.71E+02	5.6E-01	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T09-A	1	1.19E+03			1.19E+03	1.0E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T10-A	1	2.86E+02			2.86E+02	7.3E-01	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T01-B	1	9.39E+01			9.39E+01	2.2E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T02-B	1	6.69E+01			6.69E+01	4.1E+00	4.6E+00	1.5E+01	10	120	1.12E+03	88%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T03-B	1	1.32E+02			1.32E+02	2.0E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T04-B	1	2.32E+02			2.32E+02	2.3E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T05-B	1	3.24E+02			3.24E+02	2.5E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T06-B	1	4.24E+02			4.24E+02	1.4E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T07-B	1	5.52E+02			5.52E+02	8.5E-01	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T08-B	1	8.85E+02			8.85E+02	4.2E-01	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T09-B	1	1.18E+03			1.18E+03	1.3E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T10-B	1	2.72E+02			2.72E+02	4.8E-01	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T01-C	1	9.43E+01			9.43E+01	2.2E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T02-C	1	6.68E+01			6.68E+01	1.1E+01	4.6E+00	1.5E+01	10	120	1.39E+03	110%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T03-C	1	1.44E+02			1.44E+02	2.7E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T04-C	1	2.56E+02			2.56E+02	3.0E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T05-C	1	3.15E+02			3.15E+02	1.9E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T06-C	1	4.07E+02			4.07E+02	1.6E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T07-C	1	5.86E+02			5.86E+02	2.4E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T08-C	1	8.66E+02			8.66E+02	7.4E-01	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T09-C	1	1.15E+03			1.15E+03	1.4E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-T10-C	1	2.83E+02			2.83E+02	2.8E-01	4.6E+00	1.5E+01			---		VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	6.8E+00	4.6E+00	1.5E+01					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	1.4E+01	4.6E+00	1.5E+01					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	3.6E+00	4.6E+00	1.5E+01					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-B01-B	1	2.30E+00	U1/2		2.30E+00	4.6E+00	4.6E+00	1.5E+01					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-B02-B	1	2.30E+00	U1/2		2.30E+00	1.8E+01	4.6E+00	1.5E+01					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-B03-B	1	2.30E+00	U1/2		2.30E+00	5.6E+00	4.6E+00	1.5E+01					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-B01-C	1	2.30E+00	U1/2		2.30E+00	6.4E+00	4.6E+00	1.5E+01					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-B02-C	1	2.30E+00	U1/2		2.30E+00	7.1E+00	4.6E+00	1.5E+01					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1313-B03-C	1	2.30E+00	U1/2		2.30E+00	2.6E+01	4.6E+00	1.5E+01					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	CFS-L10-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	4.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	9.5E+01	2.0E+00	6.4E+00	10	120	1.15E+03	96%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	4.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	8.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	9.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	4.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T07-A	1	3.47E+00	E		3.47E+00	1.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T08-A	1	1.86E+01			1.86E+01	2.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T09-A	1	2.33E+01			2.33E+01	2.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T10-A	1	1.00E+00	U1/2		1.00E+00	1.0E+02	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	5.9E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	5.1E+01	2.0E+00	6.4E+00	10	120	1.16E+03	97%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	4.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	2.6E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T07-B	1	3.61E+00	E		3.61E+00	1.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T08-B	1	1.77E+01			1.77E+01	5.6E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T09-B	1	2.20E+01			2.20E+01	5.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T10-B	1	1.00E+00	U1/2		1.00E+00	7.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	1.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	2.6E+00	2.0E+00	6.4E+00	10	120	1.09E+03	90%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	3.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	4.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T07-C	1	4.35E+00	E		4.35E+00	3.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T08-C	1	1.83E+01			1.83E+01	1.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T09-C	1	2.10E+01			2.10E+01	8.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-T10-C	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00			---		VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	5.3E+01	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	2.3E-01	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-B01-B	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-B02-B	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-B03-B	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-B01-C	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-B02-C	1	1.00E+00	U1/2		1.00E+00	2.9E+01	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1313-B03-C	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	CFS-L10-1313-T01-A	1	1.27E+01			1.27E+01	1.7E+01	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T02-A	1	2.36E+01			2.36E+01	6.7E+00	1.5E+00	4.8E+00	10	120	1.16E+03	95%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T03-A	1	2.57E+01			2.57E+01	4.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T04-A	1	2.67E+01			2.67E+01	2.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T05-A	1	2.68E+01			2.68E+01	6.8E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T06-A	1	3.01E+01			3.01E+01	1.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T07-A	1	3.77E+01			3.77E+01	2.0E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T08-A	1	5.39E+01			5.39E+01	2.7E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T09-A	1	3.87E+02			3.87E+02	1.8E-01	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T10-A	1	2.91E+01			2.91E+01	2.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T01-B	1	1.35E+01			1.35E+01	5.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T02-B	1	2.22E+01			2.22E+01	6.1E+00	1.5E+00	4.8E+00	10	120	1.19E+03	97%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T03-B	1	2.40E+01			2.40E+01	7.6E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T04-B	1	2.72E+01			2.72E+01	3.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T05-B	1	2.81E+01			2.81E+01	3.0E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T06-B	1	3.13E+01			3.13E+01	1.8E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T07-B	1	3.69E+01			3.69E+01	2.6E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T08-B	1	4.66E+01			4.66E+01	2.0E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T09-B	1	3.75E+02			3.75E+02	2.8E-01	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T10-B	1	2.78E+01			2.78E+01	2.9E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T01-C	1	1.34E+01			1.34E+01	1.5E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T02-C	1	2.36E+01			2.36E+01	5.7E+00	1.5E+00	4.8E+00	10	120	1.09E+03	89%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T03-C	1	2.60E+01			2.60E+01	2.5E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T04-C	1	2.78E+01			2.78E+01	4.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T05-C	1	3.03E+01			3.03E+01	3.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T06-C	1	3.02E+01			3.02E+01	4.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T07-C	1	3.76E+01			3.76E+01	1.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T08-C	1	4.49E+01			4.49E+01	6.9E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T09-C	1	3.77E+02			3.77E+02	5.9E-01	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-T10-C	1	2.88E+01			2.88E+01	3.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-B01-A	1	7.50E-01	U1/2		7.50E-01	1.9E+01	1.5E+00	4.8E+00					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-B02-A	1	7.50E-01	U1/2		7.50E-01	5.4E+01	1.5E+00	4.8E+00					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-B03-A	1	7.50E-01	U1/2		7.50E-01	2.9E+01	1.5E+00	4.8E+00					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-B01-B	1	7.50E-01	U1/2		7.50E-01	6.9E+01	1.5E+00	4.8E+00					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-B02-B	1	7.50E-01	U1/2		7.50E-01	2.9E+01	1.5E+00	4.8E+00					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-B03-B	1	1.88E+00	E		1.88E+00	5.6E+01	1.5E+00	4.8E+00					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-B01-C	1	7.50E-01	U1/2		7.50E-01	6.5E+01	1.5E+00	4.8E+00					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-B02-C	1	7.50E-01	U1/2		7.50E-01	4.5E+01	1.5E+00	4.8E+00					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1313-B03-C	1	7.50E-01	U1/2		7.50E-01	3.6E+01	1.5E+00	4.8E+00					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	CFS-L10-1313-T01-A	1	1.57E+04			1.57E+04	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 2:38 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T02-A	1	1.81E+03			1.81E+03	1.5E+00	1.0E+00	3.2E+00	10	120	2.94E+03	95%	VU ICP-OES	4/13/11 2:39 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T03-A	1	2.09E+01			2.09E+01	2.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 2:41 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T04-A	1	6.37E+01			6.37E+01	6.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 2:43 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T05-A	1	4.34E+03			4.34E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 2:44 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T06-A	1	9.72E+04			9.72E+04	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 2:46 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T07-A	1	1.52E+05			1.52E+05	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 2:47 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T08-A	1	1.81E+05			1.81E+05	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 2:49 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T09-A	1	1.79E+05			1.79E+05	2.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 2:51 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T10-A	1	1.95E+04			1.95E+04	8.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 2:52 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T01-B	1	1.85E+04			1.85E+04	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 2:59 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T02-B	1	1.61E+03			1.61E+03	1.1E+00	1.0E+00	3.2E+00	10	120	2.72E+03	93%	VU ICP-OES	4/13/11 3:01 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T03-B	1	2.03E+01			2.03E+01	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:02 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T04-B	1	7.31E+01			7.31E+01	3.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:04 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T05-B	1	6.22E+03			6.22E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:06 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T06-B	1	1.04E+05			1.04E+05	8.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:07 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T07-B	1	1.60E+05			1.60E+05	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:09 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T08-B	1	1.86E+05			1.86E+05	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:11 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T09-B	1	1.76E+05			1.76E+05	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:12 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T10-B	1	1.98E+04			1.98E+04	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:14 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T01-C	1	1.79E+04			1.79E+04	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:16 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T02-C	1	1.48E+03			1.48E+03	2.2E+00	1.0E+00	3.2E+00	10	120	2.54E+03	89%	VU ICP-OES	4/13/11 3:17 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T03-C	1	2.00E+01			2.00E+01	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:19 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T04-C	1	1.01E+02			1.01E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:20 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T05-C	1	6.07E+03			6.07E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:22 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T06-C	1	1.00E+05			1.00E+05	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:24 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T07-C	1	1.60E+05			1.60E+05	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:25 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T08-C	1	1.86E+05			1.86E+05	5.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:27 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T09-C	1	1.84E+05			1.84E+05	8.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:29 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-T10-C	1	2.11E+04			2.11E+04	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:30 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-B01-A	1	3.14E+00	E		3.14E+00	6.2E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:23 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-B02-A	1	7.81E+00			7.81E+00	1.9E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:24 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-B03-A	1	6.43E+00			6.43E+00	7.3E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:26 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-B01-B	1	3.49E+00			3.49E+00	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:28 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-B02-B	1	5.60E+00			5.60E+00	3.3E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:29 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-B03-B	1	1.24E+01			1.24E+01	5.3E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:31 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-B01-C	1	4.61E+00			4.61E+00	7.1E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:33 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-B02-C	1	1.61E+01			1.61E+01	2.5E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:34 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1313-B03-C	1	6.68E+00			6.68E+00	6.3E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 2:36 PM	EPA Interlab L10 1313-1316 CFS

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	CFS-L11-1313-T01-A	1	9.48E+01			9.48E+01	2.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T02-A	1	9.60E+01			9.60E+01	2.7E+00	1.0E+00	3.2E+00	1000	100	1.24E+03	114%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T03-A	1	7.08E+01			7.08E+01	6.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T04-A	1	6.09E+01			6.09E+01	2.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T05-A	1	4.59E+01			4.59E+01	2.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T06-A	1	4.51E+01			4.51E+01	5.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T07-A	1	4.07E+03			4.07E+03	2.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T08-A	1	2.40E+04			2.40E+04	4.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T09-A	1	8.40E+04			8.40E+04	7.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T01-B	1	1.03E+02			1.03E+02	2.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T02-B	1	9.82E+01			9.82E+01	3.9E+00	1.0E+00	3.2E+00	1000	100	1.16E+03	106%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T03-B	1	9.47E+01			9.47E+01	3.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T04-B	1	6.11E+01			6.11E+01	3.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T05-B	1	4.95E+01			4.95E+01	3.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T06-B	1	4.95E+01			4.95E+01	4.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T07-B	1	3.94E+03			3.94E+03	1.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T08-B	1	2.24E+04			2.24E+04	2.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T09-B	1	7.88E+04			7.88E+04	3.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T01-C	1	1.16E+02			1.16E+02	6.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T02-C	1	1.16E+02			1.16E+02	9.9E+00	1.0E+00	3.2E+00	1000	100	1.24E+03	113%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T03-C	1	7.38E+01			7.38E+01	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T04-C	1	5.72E+01			5.72E+01	4.3E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T05-C	1	4.79E+01			4.79E+01	2.3E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T06-C	1	4.80E+01			4.80E+01	7.6E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T07-C	1	4.16E+03			4.16E+03	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T08-C	1	2.35E+04			2.35E+04	5.9E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-T09-C	1	8.36E+04			8.36E+04	5.3E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-B02-A	1	2.29E+00	E		2.29E+00	8.9E+01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1313-B03-A	1	7.87E+02			7.87E+02	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	CFS-L11-1313-T01-A	1	3.75E+00	U1/2		3.75E+00	1.6E+02	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T02-A	1	3.75E+00	U1/2		3.75E+00	7.4E+01	7.5E+00	2.4E+01	10	100	9.08E+02	90%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T03-A	1	2.34E+01	E		2.34E+01	8.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T04-A	1	2.35E+01	E		2.35E+01	2.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T05-A	1	1.68E+01	E		1.68E+01	1.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T06-A	1	3.53E+01			3.53E+01	1.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T07-A	1	9.00E+01			9.00E+01	6.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T08-A	1	7.10E+02			7.10E+02	3.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T09-A	1	1.63E+03			1.63E+03	4.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T01-B	1	3.75E+00	U1/2		3.75E+00	9.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T02-B	1	1.03E+01	E		1.03E+01	3.9E+01	7.5E+00	2.4E+01	10	100	8.79E+02	87%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T03-B	1	3.19E+01			3.19E+01	1.5E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T04-B	1	3.41E+01			3.41E+01	2.8E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T05-B	1	1.56E+01	E		1.56E+01	1.9E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T06-B	1	2.71E+01			2.71E+01	8.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T07-B	1	9.30E+01			9.30E+01	1.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T08-B	1	7.01E+02			7.01E+02	2.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T09-B	1	1.56E+03			1.56E+03	7.4E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T01-C	1	3.75E+00	U1/2		3.75E+00	8.7E+02	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T02-C	1	3.75E+00	U1/2		3.75E+00	9.0E+01	7.5E+00	2.4E+01	10	100	9.41E+02	94%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T03-C	1	4.30E+01			4.30E+01	8.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T04-C	1	3.21E+01			3.21E+01	4.5E+01	7.5E+00	2.4E+01					VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T05-C	1	1.64E+01	E		1.64E+01	2.6E+01	7.5E+00	2.4E+01					VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T06-C	1	2.25E+01	E		2.25E+01	3.8E+01	7.5E+00	2.4E+01					VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T07-C	1	8.24E+01			8.24E+01	1.1E+01	7.5E+00	2.4E+01					VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T08-C	1	6.91E+02			6.91E+02	1.8E+01	7.5E+00	2.4E+01					VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-T09-C	1	1.65E+03			1.65E+03	9.9E+00	7.5E+00	2.4E+01					VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-B01-A	1	3.75E+00	U1/2		3.75E+00	9.9E+01	7.5E+00	2.4E+01					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-B02-A	1	1.61E+01	E		1.61E+01	1.2E+02	7.5E+00	2.4E+01					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1313-B03-A	1	8.75E+00	E		8.75E+00	9.6E+01	7.5E+00	2.4E+01					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	CFS-L11-1313-T01-A	1	2.07E+02			2.07E+02	3.9E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T02-A	1	1.44E+02			1.44E+02	3.7E+00	1.1E+01	3.5E+01	10	100	1.06E+03	92%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T03-A	1	5.09E+01			5.09E+01	7.8E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T04-A	1	4.46E+01			4.46E+01	3.7E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T05-A	1	1.90E+01	E		1.90E+01	2.1E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T06-A	1	1.95E+01	E		1.95E+01	3.2E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T07-A	1	1.10E+02			1.10E+02	9.8E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T08-A	1	6.04E+02			6.04E+02	2.4E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T09-A	1	4.26E+04			4.26E+04	5.6E-01	1.1E+01	3.5E+01			---		VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T01-B	1	1.97E+02			1.97E+02	4.6E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T02-B	1	1.50E+02			1.50E+02	8.0E+00	1.1E+01	3.5E+01	10	100	1.02E+03	87%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T03-B	1	5.18E+01			5.18E+01	1.8E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T04-B	1	3.09E+01	E		3.09E+01	1.5E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T05-B	1	1.96E+01	E		1.96E+01	2.4E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T06-B	1	1.98E+01	E		1.98E+01	1.8E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T07-B	1	1.16E+02			1.16E+02	8.9E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T08-B	1	6.03E+02			6.03E+02	2.0E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T09-B	1	3.41E+04			3.41E+04	1.0E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T01-C	1	1.97E+02			1.97E+02	1.7E+00	1.1E+01	3.5E+01			---		VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T02-C	1	1.45E+02			1.45E+02	7.6E+00	1.1E+01	3.5E+01	10	100	1.09E+03	95%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T03-C	1	5.11E+01			5.11E+01	1.1E+01	1.1E+01	3.5E+01			---		VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T04-C	1	3.26E+01	E		3.26E+01	2.0E+01	1.1E+01	3.5E+01					VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T05-C	1	5.50E+00	U1/2		5.50E+00	1.4E+02	1.1E+01	3.5E+01					VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T06-C	1	1.32E+01	E		1.32E+01	9.4E+01	1.1E+01	3.5E+01					VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T07-C	1	9.82E+01			9.82E+01	6.5E+00	1.1E+01	3.5E+01					VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T08-C	1	5.90E+02			5.90E+02	1.7E+00	1.1E+01	3.5E+01					VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-T09-C	1	3.46E+04			3.46E+04	2.1E-01	1.1E+01	3.5E+01					VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-B01-A	1	5.50E+00	U1/2		5.50E+00	1.2E+03	1.1E+01	3.5E+01					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-B02-A	1	5.50E+00	U1/2		5.50E+00	5.7E+01	1.1E+01	3.5E+01					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1313-B03-A	1	1.37E+01	E		1.37E+01	5.6E+00	1.1E+01	3.5E+01					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	CFS-L11-1313-T01-A	1	9.32E+02			9.32E+02	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T02-A	1	5.75E+02			5.75E+02	6.3E-01	1.0E+00	3.2E+00	1000	100	1.51E+03	94%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T03-A	1	2.85E+02			2.85E+02	1.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T04-A	1	1.74E+02			1.74E+02	9.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T05-A	1	1.33E+02			1.33E+02	2.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T06-A	1	7.45E+01			7.45E+01	2.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T07-A	1	2.15E+02			2.15E+02	5.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T08-A	1	4.27E+02			4.27E+02	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T09-A	1	6.57E+02			6.57E+02	9.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T01-B	1	8.23E+02			8.23E+02	9.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T02-B	1	5.59E+02			5.59E+02	2.7E-01	1.0E+00	3.2E+00	1000	100	1.45E+03	89%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T03-B	1	2.68E+02			2.68E+02	9.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T04-B	1	1.70E+02			1.70E+02	5.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T05-B	1	1.27E+02			1.27E+02	2.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T06-B	1	9.15E+01			9.15E+01	9.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T07-B	1	2.29E+02			2.29E+02	5.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T08-B	1	4.32E+02			4.32E+02	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T09-B	1	5.79E+02			5.79E+02	1.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T01-C	1	8.96E+02			8.96E+02	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T02-C	1	6.03E+02			6.03E+02	8.4E+00	1.0E+00	3.2E+00	1000	100	1.53E+03	93%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T03-C	1	2.65E+02			2.65E+02	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T04-C	1	1.57E+02			1.57E+02	2.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T05-C	1	1.18E+02			1.18E+02	2.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T06-C	1	5.92E+01			5.92E+01	2.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T07-C	1	1.95E+02			1.95E+02	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T08-C	1	3.98E+02			3.98E+02	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-T09-C	1	5.89E+02			5.89E+02	6.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	5.7E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	4.9E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1313-B03-A	1	2.24E+03			2.24E+03	6.5E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	CFS-L11-1313-T01-A	1	2.40E+03			2.40E+03	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T02-A	1	1.77E+03			1.77E+03	9.7E-01	1.0E+00	3.2E+00	10	100	2.66E+03	89%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T03-A	1	9.81E+02			9.81E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T04-A	1	6.97E+02			6.97E+02	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T05-A	1	4.75E+02			4.75E+02	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T06-A	1	2.23E+02			2.23E+02	1.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T07-A	1	1.10E+02			1.10E+02	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T08-A	1	1.24E+02			1.24E+02	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T09-A	1	1.19E+02			1.19E+02	9.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T01-B	1	2.54E+03			2.54E+03	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T02-B	1	1.80E+03			1.80E+03	2.3E-01	1.0E+00	3.2E+00	10	100	2.65E+03	85%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T03-B	1	9.60E+02			9.60E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T04-B	1	7.13E+02			7.13E+02	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T05-B	1	4.83E+02			4.83E+02	7.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T06-B	1	2.17E+02			2.17E+02	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T07-B	1	1.04E+02			1.04E+02	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T08-B	1	1.16E+02			1.16E+02	8.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T09-B	1	1.14E+02			1.14E+02	2.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T01-C	1	2.53E+03			2.53E+03	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T02-C	1	1.91E+03			1.91E+03	7.4E+00	1.0E+00	3.2E+00	10	100	2.80E+03	88%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T03-C	1	9.76E+02			9.76E+02	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T04-C	1	6.94E+02			6.94E+02	8.0E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T05-C	1	4.86E+02			4.86E+02	6.9E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T06-C	1	2.18E+02			2.18E+02	8.1E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T07-C	1	1.03E+02			1.03E+02	1.5E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T08-C	1	1.15E+02			1.15E+02	6.9E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-T09-C	1	1.27E+02			1.27E+02	3.4E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	5.2E+01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	5.3E+01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1313-B03-A	1	2.57E+03			2.57E+03	9.7E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	CFS-L11-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	4.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T02-A	1	9.50E-01	U1/2		9.50E-01	2.5E+01	1.9E+00	6.0E+00	10	100	9.17E+02	92%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T03-A	1	9.50E-01	U1/2		9.50E-01	3.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	2.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	4.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	9.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T07-A	1	2.23E+00	E		2.23E+00	5.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T08-A	1	5.22E+00	E		5.22E+00	4.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T09-A	1	9.50E-01	U1/2		9.50E-01	8.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	4.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T02-B	1	9.50E-01	U1/2		9.50E-01	3.4E+02	1.9E+00	6.0E+00	10	100	8.82E+02	88%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T03-B	1	9.50E-01	U1/2		9.50E-01	6.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	9.7E+02	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	1.0E+03	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T07-B	1	2.01E+00	E		2.01E+00	2.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T08-B	1	4.93E+00	E		4.93E+00	1.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T09-B	1	3.39E+00	E		3.39E+00	1.6E+02	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	6.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T02-C	1	9.50E-01	U1/2		9.50E-01	6.8E+01	1.9E+00	6.0E+00	10	100	9.35E+02	93%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T03-C	1	9.50E-01	U1/2		9.50E-01	5.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	3.3E+03	1.9E+00	6.0E+00					VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	1.9E+01	1.9E+00	6.0E+00					VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	2.3E+02	1.9E+00	6.0E+00					VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T07-C	1	2.00E+00	E		2.00E+00	3.7E+00	1.9E+00	6.0E+00					VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T08-C	1	4.97E+00	E		4.97E+00	5.4E+00	1.9E+00	6.0E+00					VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-T09-C	1	3.63E+00	E		3.63E+00	1.7E+02	1.9E+00	6.0E+00					VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	1.0E+02	1.9E+00	6.0E+00					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	4.4E+01	1.9E+00	6.0E+00					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	4.7E+02	1.9E+00	6.0E+00					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	CFS-L11-1313-T01-A	1	3.47E+00	E		3.47E+00	5.8E+00	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T02-A	1	1.10E+00	U1/2		1.10E+00	4.4E+01	2.2E+00	7.0E+00	10	100	9.57E+02	96%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T03-A	1	2.71E+00	E		2.71E+00	7.0E+00	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T04-A	1	2.02E+01			2.02E+01	2.5E+00	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T05-A	1	2.26E+02			2.26E+02	4.7E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T06-A	1	3.19E+03			3.19E+03	3.4E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T07-A	1	1.74E+04			1.74E+04	3.9E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T08-A	1	3.31E+04			3.31E+04	1.2E+00	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T09-A	1	3.84E+04			3.84E+04	7.7E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T01-B	1	3.09E+00	E		3.09E+00	4.5E+00	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T02-B	1	1.10E+00	U1/2		1.10E+00	3.7E+01	2.2E+00	7.0E+00	10	100	9.36E+02	94%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T03-B	1	3.26E+00	E		3.26E+00	9.9E+00	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T04-B	1	1.18E+01			1.18E+01	6.1E+00	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T05-B	1	2.24E+02			2.24E+02	8.9E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T06-B	1	2.99E+03			2.99E+03	4.0E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T07-B	1	1.67E+04			1.67E+04	1.1E+00	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T08-B	1	3.29E+04			3.29E+04	4.3E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T09-B	1	3.52E+04			3.52E+04	4.9E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T01-C	1	3.26E+00	E		3.26E+00	5.8E+00	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T02-C	1	1.10E+00	U1/2		1.10E+00	9.6E+01	2.2E+00	7.0E+00	10	100	9.67E+02	97%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T03-C	1	1.10E+00	U1/2		1.10E+00	5.2E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T04-C	1	1.24E+01			1.24E+01	1.4E+00	2.2E+00	7.0E+00					VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T05-C	1	1.51E+02			1.51E+02	7.5E-01	2.2E+00	7.0E+00					VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T06-C	1	2.87E+03			2.87E+03	6.9E-01	2.2E+00	7.0E+00					VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T07-C	1	1.65E+04			1.65E+04	3.1E-01	2.2E+00	7.0E+00					VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T08-C	1	3.14E+04			3.14E+04	1.0E+00	2.2E+00	7.0E+00					VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-T09-C	1	3.65E+04			3.65E+04	6.8E-01	2.2E+00	7.0E+00					VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-B01-A	1	1.10E+00	U1/2		1.10E+00	8.1E+02	2.2E+00	7.0E+00					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-B02-A	1	4.28E+00	E		4.28E+00	1.7E+00	2.2E+00	7.0E+00					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1313-B03-A	1	1.10E+00	U1/2		1.10E+00	1.4E+03	2.2E+00	7.0E+00					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	CFS-L11-1313-T01-A	1	6.37E+05			6.37E+05	7.7E-02	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T02-A	1	5.65E+05			5.65E+05	7.2E-01	2.6E+00	8.3E+00	1000	100	5.66E+05	86%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T03-A	1	5.82E+05			5.82E+05	7.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T04-A	1	5.87E+05			5.87E+05	1.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T05-A	1	6.01E+05			6.01E+05	4.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T06-A	1	6.38E+05			6.38E+05	2.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T07-A	1	8.28E+05			8.28E+05	4.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T08-A	1	1.15E+06			1.15E+06	3.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T09-A	1	1.43E+06			1.43E+06	1.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T01-B	1	6.11E+05			6.11E+05	8.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T02-B	1	5.60E+05			5.60E+05	4.5E-01	2.6E+00	8.3E+00	1000	100	5.61E+05	83%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T03-B	1	5.49E+05			5.49E+05	9.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T04-B	1	5.90E+05			5.90E+05	2.8E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T05-B	1	6.10E+05			6.10E+05	4.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T06-B	1	6.30E+05			6.30E+05	7.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T07-B	1	8.13E+05			8.13E+05	2.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T08-B	1	1.10E+06			1.10E+06	4.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T09-B	1	1.36E+06			1.36E+06	2.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T01-C	1	6.27E+05			6.27E+05	5.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T02-C	1	6.00E+05			6.00E+05	7.9E+00	2.6E+00	8.3E+00	1000	100	6.01E+05	89%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T03-C	1	5.73E+05			5.73E+05	1.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T04-C	1	5.87E+05			5.87E+05	6.9E-01	2.6E+00	8.3E+00					VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T05-C	1	6.09E+05			6.09E+05	1.2E+00	2.6E+00	8.3E+00					VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T06-C	1	6.33E+05			6.33E+05	5.0E-01	2.6E+00	8.3E+00					VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T07-C	1	8.29E+05			8.29E+05	2.8E-01	2.6E+00	8.3E+00					VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T08-C	1	1.11E+06			1.11E+06	6.2E-01	2.6E+00	8.3E+00					VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-T09-C	1	1.42E+06			1.42E+06	5.8E-01	2.6E+00	8.3E+00					VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-B01-A	1	1.03E+01			1.03E+01	4.3E+01	2.6E+00	8.3E+00					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-B02-A	1	3.38E+02			3.38E+02	5.2E+00	2.6E+00	8.3E+00					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1313-B03-A	1	2.15E+01			2.15E+01	3.1E+01	2.6E+00	8.3E+00					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	CFS-L11-1313-T01-A	1	7.54E+01			7.54E+01	6.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T02-A	1	5.18E+01			5.18E+01	7.8E-01	1.2E+00	3.8E+00	10	100	9.89E+02	94%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T03-A	1	3.01E+00	E		3.01E+00	7.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T04-A	1	2.98E+00	E		2.98E+00	2.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T05-A	1	6.00E-01	U1/2		6.00E-01	3.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T06-A	1	6.00E-01	U1/2		6.00E-01	2.2E+02	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T07-A	1	6.00E-01	U1/2		6.00E-01	4.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T08-A	1	2.15E+01			2.15E+01	3.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T09-A	1	1.87E+03			1.87E+03	6.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T01-B	1	7.83E+01			7.83E+01	1.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T02-B	1	5.08E+01			5.08E+01	5.4E-01	1.2E+00	3.8E+00	10	100	9.39E+02	89%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T03-B	1	3.16E+00	E		3.16E+00	7.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T04-B	1	1.23E+00	E		1.23E+00	3.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T05-B	1	6.00E-01	U1/2		6.00E-01	1.1E+02	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T06-B	1	6.00E-01	U1/2		6.00E-01	9.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T07-B	1	6.00E-01	U1/2		6.00E-01	3.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T08-B	1	2.06E+01			2.06E+01	1.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T09-B	1	1.31E+03			1.31E+03	5.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T01-C	1	8.19E+01			8.19E+01	4.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T02-C	1	5.16E+01			5.16E+01	9.3E+00	1.2E+00	3.8E+00	10	100	9.90E+02	94%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T03-C	1	2.48E+00	E		2.48E+00	1.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T04-C	1	6.00E-01	U1/2		6.00E-01	3.3E+01	1.2E+00	3.8E+00					VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T05-C	1	6.00E-01	U1/2		6.00E-01	6.2E+01	1.2E+00	3.8E+00					VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T06-C	1	6.00E-01	U1/2		6.00E-01	3.8E+01	1.2E+00	3.8E+00					VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T07-C	1	1.20E+00	E		1.20E+00	4.4E+01	1.2E+00	3.8E+00					VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T08-C	1	2.35E+01			2.35E+01	9.8E-01	1.2E+00	3.8E+00					VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-T09-C	1	1.44E+03			1.44E+03	1.9E-01	1.2E+00	3.8E+00					VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	6.7E+02	1.2E+00	3.8E+00					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	1.0E+02	1.2E+00	3.8E+00					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1313-B03-A	1	1.94E+00	E		1.94E+00	2.8E+01	1.2E+00	3.8E+00					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	CFS-L11-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	3.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	6.3E+01	1.8E+00	5.7E+00	10	100	1.02E+03	102%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	5.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	8.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T05-A	1	6.36E+00			6.36E+00	4.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T06-A	1	9.19E+01			9.19E+01	2.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T07-A	1	5.69E+02			5.69E+02	3.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T08-A	1	1.50E+03			1.50E+03	3.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T09-A	1	1.83E+03			1.83E+03	1.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	1.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	4.5E+01	1.8E+00	5.7E+00	10	100	9.83E+02	98%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	8.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	2.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T05-B	1	5.22E+00	E		5.22E+00	1.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T06-B	1	8.58E+01			8.58E+01	1.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T07-B	1	5.35E+02			5.35E+02	3.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T08-B	1	1.43E+03			1.43E+03	8.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T09-B	1	1.65E+03			1.65E+03	1.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	9.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	9.4E+01	1.8E+00	5.7E+00	10	100	1.03E+03	103%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	1.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T04-C	1	9.00E-01	U1/2		9.00E-01	8.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T05-C	1	4.45E+00	E		4.45E+00	2.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T06-C	1	8.17E+01			8.17E+01	9.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T07-C	1	5.42E+02			5.42E+02	1.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T08-C	1	1.40E+03			1.40E+03	5.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-T09-C	1	1.79E+03			1.79E+03	9.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	1.8E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	8.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	CFS-L11-1313-T01-A	1	3.12E+03			3.12E+03	6.3E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T02-A	1	8.56E+02			8.56E+02	1.6E+00	3.7E+00	1.2E+01	10	100	1.82E+03	96%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T03-A	1	7.26E+01			7.26E+01	9.1E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T04-A	1	1.57E+02			1.57E+02	1.6E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T05-A	1	5.17E+01			5.17E+01	5.6E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T06-A	1	8.76E+02			8.76E+02	5.7E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T07-A	1	2.16E+05			2.16E+05	9.2E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T08-A	1	8.18E+05			8.18E+05	3.9E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T09-A	1	1.06E+06			1.06E+06	3.7E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T01-B	1	2.65E+03			2.65E+03	1.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T02-B	1	8.10E+02			8.10E+02	5.2E-01	3.7E+00	1.2E+01	10	100	1.69E+03	88%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T03-B	1	1.04E+02			1.04E+02	1.7E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T04-B	1	4.46E+01			4.46E+01	2.6E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T05-B	1	5.54E+01			5.54E+01	9.9E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T06-B	1	7.41E+02			7.41E+02	1.3E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T07-B	1	2.15E+05			2.15E+05	4.6E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T08-B	1	7.79E+05			7.79E+05	2.4E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T09-B	1	9.66E+05			9.66E+05	3.1E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T01-C	1	2.90E+03			2.90E+03	4.9E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T02-C	1	8.74E+02			8.74E+02	6.6E+00	3.7E+00	1.2E+01	10	100	1.82E+03	94%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T03-C	1	6.89E+01			6.89E+01	1.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T04-C	1	4.62E+01			4.62E+01	2.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T05-C	1	6.64E+01			6.64E+01	3.3E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T06-C	1	7.21E+02			7.21E+02	6.9E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T07-C	1	2.18E+05			2.18E+05	1.3E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T08-C	1	7.78E+05			7.78E+05	5.9E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-T09-C	1	1.05E+06			1.05E+06	1.8E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-B01-A	1	1.43E+01			1.43E+01	3.0E+00	3.7E+00	1.2E+01					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-B02-A	1	1.52E+02			1.52E+02	4.1E+00	3.7E+00	1.2E+01					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1313-B03-A	1	3.76E+01			3.76E+01	3.1E+00	3.7E+00	1.2E+01					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	CFS-L11-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	4.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	5.3E+01	2.0E+00	6.4E+00	1000	100	9.32E+02	93%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	4.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	2.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	1.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	4.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T08-A	1	4.94E+03			4.94E+03	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T09-A	1	1.81E+05			1.81E+05	5.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	4.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	3.6E+01	2.0E+00	6.4E+00	1000	100	8.88E+02	89%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	5.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	6.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	7.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T08-B	1	4.64E+03			4.64E+03	6.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T09-B	1	1.79E+05			1.79E+05	2.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T01-C	1	1.19E+01			1.19E+01	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	4.1E+01	2.0E+00	6.4E+00	1000	100	9.41E+02	94%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	7.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	3.9E+00	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	8.3E+00	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T07-C	1	4.84E+00	E		4.84E+00	2.4E+00	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T08-C	1	7.51E+03			7.51E+03	8.7E-01	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-T09-C	1	1.71E+05			1.71E+05	1.1E+00	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	7.7E+00	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-B02-A	1	3.25E+00	E		3.25E+00	1.8E+01	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1313-B03-A	1	2.00E+01			2.00E+01	9.6E-01	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	CFS-L11-1313-T01-A	1	4.10E+03			4.10E+03	1.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T02-A	1	5.43E+03			5.43E+03	7.4E-01	6.8E+00	2.2E+01	10	100	6.45E+03	102%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T03-A	1	1.23E+02			1.23E+02	1.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T04-A	1	7.63E+01			7.63E+01	2.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T05-A	1	1.56E+02			1.56E+02	6.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T06-A	1	8.58E+02			8.58E+02	1.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T07-A	1	5.15E+03			5.15E+03	1.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T08-A	1	5.07E+03			5.07E+03	6.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T09-A	1	7.93E+03			7.93E+03	6.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T01-B	1	4.89E+03			4.89E+03	8.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T02-B	1	6.30E+03			6.30E+03	1.0E+00	6.8E+00	2.2E+01	10	100	7.25E+03	95%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T03-B	1	1.08E+02			1.08E+02	1.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T04-B	1	7.24E+01			7.24E+01	5.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T05-B	1	1.79E+02			1.79E+02	1.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T06-B	1	7.48E+02			7.48E+02	4.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T07-B	1	5.73E+03			5.73E+03	4.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T08-B	1	4.38E+03			4.38E+03	6.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T09-B	1	7.23E+03			7.23E+03	3.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T01-C	1	5.44E+03			5.44E+03	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T02-C	1	8.27E+03			8.27E+03	6.7E+00	6.8E+00	2.2E+01	10	100	9.25E+03	97%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T03-C	1	1.21E+02			1.21E+02	1.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T04-C	1	7.15E+01			7.15E+01	3.1E+00	6.8E+00	2.2E+01					VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T05-C	1	1.08E+02			1.08E+02	2.6E+00	6.8E+00	2.2E+01					VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T06-C	1	8.87E+02			8.87E+02	9.7E-01	6.8E+00	2.2E+01					VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T07-C	1	6.19E+03			6.19E+03	6.0E-01	6.8E+00	2.2E+01					VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T08-C	1	4.94E+03			4.94E+03	6.4E-01	6.8E+00	2.2E+01					VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-T09-C	1	7.51E+03			7.51E+03	2.0E-01	6.8E+00	2.2E+01					VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	4.0E+02	6.8E+00	2.2E+01					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-B02-A	1	7.44E+02			7.44E+02	2.5E+00	6.8E+00	2.2E+01					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1313-B03-A	1	3.28E+01			3.28E+01	3.3E+00	6.8E+00	2.2E+01					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	CFS-L11-1313-T01-A	1	2.03E+01			2.03E+01	3.9E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T02-A	1	1.94E+01			1.94E+01	3.2E+00	1.9E+00	6.0E+00	10	100	8.80E+02	86%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T03-A	1	1.94E+01			1.94E+01	3.1E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T04-A	1	1.96E+01			1.96E+01	4.0E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T05-A	1	1.99E+01			1.99E+01	6.5E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T06-A	1	1.77E+01			1.77E+01	1.8E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T07-A	1	1.76E+01			1.76E+01	1.7E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T08-A	1	2.11E+01			2.11E+01	4.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T09-A	1	2.83E+01			2.83E+01	1.3E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T01-B	1	2.30E+01			2.30E+01	3.1E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T02-B	1	2.18E+01			2.18E+01	1.6E+00	1.9E+00	6.0E+00	10	100	8.52E+02	83%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T03-B	1	2.13E+01			2.13E+01	3.9E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T04-B	1	2.11E+01			2.11E+01	2.7E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T05-B	1	2.01E+01			2.01E+01	1.9E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T06-B	1	1.94E+01			1.94E+01	1.0E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T07-B	1	1.91E+01			1.91E+01	1.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T08-B	1	2.08E+01			2.08E+01	7.5E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T09-B	1	3.04E+01			3.04E+01	1.1E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T01-C	1	2.21E+01			2.21E+01	8.3E-01	1.9E+00	6.0E+00			---		VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T02-C	1	2.25E+01			2.25E+01	4.1E+00	1.9E+00	6.0E+00	10	100	8.74E+02	85%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T03-C	1	2.02E+01			2.02E+01	5.2E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T04-C	1	2.05E+01			2.05E+01	3.1E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T05-C	1	2.01E+01			2.01E+01	7.0E-01	1.9E+00	6.0E+00			---		VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T06-C	1	1.80E+01			1.80E+01	6.8E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T07-C	1	1.95E+01			1.95E+01	7.2E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T08-C	1	2.20E+01			2.20E+01	9.2E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-T09-C	1	2.98E+01			2.98E+01	2.2E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-B01-A	1	6.06E+00			6.06E+00	1.1E+01	1.9E+00	6.0E+00					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-B02-A	1	7.87E+00			7.87E+00	5.8E+00	1.9E+00	6.0E+00					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1313-B03-A	1	6.89E+00			6.89E+00	2.1E+01	1.9E+00	6.0E+00					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	CFS-L11-1313-T01-A	1	4.75E+00	E		4.75E+00	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00	10	100	8.93E+02	89%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	6.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T04-A	1	3.82E+00	E		3.82E+00	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T05-A	1	1.32E+02			1.32E+02	1.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T06-A	1	1.31E+03			1.31E+03	2.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T07-A	1	4.78E+03			4.78E+03	3.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T08-A	1	1.51E+04			1.51E+04	7.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T09-A	1	2.63E+04			2.63E+04	1.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00	10	100	8.60E+02	86%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	5.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	5.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T05-B	1	1.23E+02			1.23E+02	4.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T06-B	1	1.21E+03			1.21E+03	9.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T07-B	1	4.49E+03			4.49E+03	8.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T08-B	1	1.43E+04			1.43E+04	2.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T09-B	1	2.47E+04			2.47E+04	4.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	1.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	2.4E+01	2.0E+00	6.4E+00	10	100	8.51E+02	85%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	3.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	1.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T05-C	1	7.81E+01			7.81E+01	5.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T06-C	1	1.15E+03			1.15E+03	7.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T07-C	1	4.54E+03			4.54E+03	8.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T08-C	1	1.42E+04			1.42E+04	3.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-T09-C	1	2.59E+04			2.59E+04	1.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	6.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	7.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	1.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	CFS-L11-1313-T01-A	1	1.10E+02			1.10E+02	7.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T02-A	1	4.87E+01			4.87E+01	6.6E+00	1.0E+00	3.2E+00	1000	100	1.04E+03	99%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T03-A	1	1.27E+04			1.27E+04	7.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T04-A	1	3.74E+04			3.74E+04	4.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T05-A	1	6.88E+04			6.88E+04	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T06-A	1	6.84E+04			6.84E+04	5.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T07-A	1	7.66E+04			7.66E+04	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T08-A	1	1.03E+05			1.03E+05	3.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T09-A	1	2.16E+05			2.16E+05	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T01-B	1	3.25E+01			3.25E+01	7.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T02-B	1	4.27E+01			4.27E+01	2.6E+01	1.0E+00	3.2E+00	1000	100	1.01E+03	97%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T03-B	1	1.13E+04			1.13E+04	9.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T04-B	1	3.84E+04			3.84E+04	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T05-B	1	6.07E+04			6.07E+04	9.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T06-B	1	6.64E+04			6.64E+04	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T07-B	1	7.12E+04			7.12E+04	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T08-B	1	9.89E+04			9.89E+04	5.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T09-B	1	1.88E+05			1.88E+05	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T01-C	1	4.74E+01			4.74E+01	1.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T02-C	1	4.04E+01			4.04E+01	1.6E+01	1.0E+00	3.2E+00	1000	100	1.06E+03	102%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T03-C	1	1.10E+04			1.10E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T04-C	1	3.99E+04			3.99E+04	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T05-C	1	6.48E+04			6.48E+04	9.1E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T06-C	1	6.45E+04			6.45E+04	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T07-C	1	7.14E+04			7.14E+04	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T08-C	1	9.31E+04			9.31E+04	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-T09-C	1	2.26E+05			2.26E+05	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	2.4E+03	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	9.3E+02	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1313-B03-A	1	6.43E+00			6.43E+00	4.5E+01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	CFS-L11-1313-T01-A	1	1.52E+03			1.52E+03	4.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T02-A	1	1.37E+03			1.37E+03	1.2E+00	1.2E+00	3.8E+00	10	100	2.26E+03	89%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T03-A	1	6.99E+02			6.99E+02	6.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T04-A	1	3.20E+02			3.20E+02	8.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T05-A	1	5.08E+01			5.08E+01	2.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T06-A	1	1.00E+01			1.00E+01	9.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T07-A	1	7.05E+00			7.05E+00	4.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T08-A	1	1.13E+01			1.13E+01	7.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T09-A	1	6.74E+01			6.74E+01	2.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T01-B	1	1.40E+03			1.40E+03	4.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T02-B	1	1.30E+03			1.30E+03	2.3E-01	1.2E+00	3.8E+00	10	100	2.16E+03	86%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T03-B	1	6.85E+02			6.85E+02	8.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T04-B	1	3.18E+02			3.18E+02	3.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T05-B	1	5.68E+01			5.68E+01	8.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T06-B	1	1.08E+01			1.08E+01	5.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T07-B	1	4.79E+00			4.79E+00	9.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T08-B	1	1.91E+01			1.91E+01	7.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T09-B	1	5.09E+01			5.09E+01	5.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T01-C	1	1.51E+03			1.51E+03	1.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T02-C	1	1.39E+03			1.39E+03	9.4E+00	1.2E+00	3.8E+00	10	100	2.26E+03	87%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T03-C	1	6.99E+02			6.99E+02	7.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T04-C	1	3.15E+02			3.15E+02	1.1E+00	1.2E+00	3.8E+00					VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T05-C	1	6.75E+01			6.75E+01	2.0E+00	1.2E+00	3.8E+00					VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T06-C	1	1.08E+01			1.08E+01	1.2E+01	1.2E+00	3.8E+00					VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T07-C	1	6.73E+00			6.73E+00	1.3E+01	1.2E+00	3.8E+00					VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T08-C	1	9.06E+00			9.06E+00	4.9E+01	1.2E+00	3.8E+00					VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-T09-C	1	7.19E+01			7.19E+01	9.3E+00	1.2E+00	3.8E+00					VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-B01-A	1	1.29E+00	E		1.29E+00	6.3E+01	1.2E+00	3.8E+00					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-B02-A	1	1.57E+00	E		1.57E+00	5.2E+01	1.2E+00	3.8E+00					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1313-B03-A	1	5.82E+00			5.82E+00	2.2E+01	1.2E+00	3.8E+00					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	CFS-L11-1313-T01-A	1	9.00E-01	U1/2		9.00E-01	2.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T02-A	1	9.00E-01	U1/2		9.00E-01	3.6E+02	1.8E+00	5.7E+00	10	100	8.60E+02	86%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T03-A	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T04-A	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T05-A	1	7.68E+00			7.68E+00	1.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T06-A	1	1.64E+02			1.64E+02	1.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T07-A	1	1.78E+03			1.78E+03	6.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T08-A	1	4.78E+03			4.78E+03	4.3E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T09-A	1	5.80E+03			5.80E+03	3.3E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T01-B	1	9.00E-01	U1/2		9.00E-01	2.8E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T02-B	1	9.00E-01	U1/2		9.00E-01	1.7E+02	1.8E+00	5.7E+00	10	100	8.75E+02	87%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T03-B	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T04-B	1	9.00E-01	U1/2		9.00E-01	2.5E+04	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T05-B	1	7.71E+00			7.71E+00	1.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T06-B	1	1.48E+02			1.48E+02	1.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T07-B	1	1.69E+03			1.69E+03	2.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T08-B	1	4.59E+03			4.59E+03	1.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T09-B	1	5.22E+03			5.22E+03	5.4E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T01-C	1	9.00E-01	U1/2		9.00E-01	5.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T02-C	1	9.00E-01	U1/2		9.00E-01	1.2E+02	1.8E+00	5.7E+00	10	100	8.75E+02	87%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T03-C	1	9.00E-01	U1/2		9.00E-01	7.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T04-C	1	2.09E+00	E		2.09E+00	2.7E+01	1.8E+00	5.7E+00					VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T05-C	1	5.32E+00	E		5.32E+00	4.6E+00	1.8E+00	5.7E+00					VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T06-C	1	1.43E+02			1.43E+02	8.3E-01	1.8E+00	5.7E+00					VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T07-C	1	1.70E+03			1.70E+03	7.4E-01	1.8E+00	5.7E+00					VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T08-C	1	4.54E+03			4.54E+03	1.2E+00	1.8E+00	5.7E+00					VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-T09-C	1	5.54E+03			5.54E+03	4.5E-01	1.8E+00	5.7E+00					VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	5.9E+02	1.8E+00	5.7E+00					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	3.1E+02	1.8E+00	5.7E+00					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	1.9E+02	1.8E+00	5.7E+00					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	CFS-L11-1313-T01-A	1	5.15E+01			5.15E+01	1.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T02-A	1	8.33E+01			8.33E+01	9.1E+00	3.7E+00	1.2E+01	1000	100	9.70E+02	89%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T03-A	1	4.41E+01			4.41E+01	1.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T04-A	1	2.95E+01			2.95E+01	2.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T05-A	1	2.25E+01			2.25E+01	4.6E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T06-A	1	2.71E+01			2.71E+01	2.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T07-A	1	4.29E+01			4.29E+01	1.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T08-A	1	4.40E+01			4.40E+01	4.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T09-A	1	1.27E+03			1.27E+03	5.1E-01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T01-B	1	8.29E+01			8.29E+01	6.3E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T02-B	1	6.45E+01			6.45E+01	1.2E+01	3.7E+00	1.2E+01	1000	100	9.78E+02	91%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T03-B	1	4.09E+01			4.09E+01	1.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T04-B	1	3.98E+01			3.98E+01	2.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T05-B	1	3.50E+01			3.50E+01	2.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T06-B	1	2.69E+01			2.69E+01	3.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T07-B	1	2.88E+01			2.88E+01	6.6E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T08-B	1	4.71E+01			4.71E+01	2.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T09-B	1	9.50E+02			9.50E+02	1.6E+00	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T01-C	1	7.02E+01			7.02E+01	1.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T02-C	1	7.91E+01			7.91E+01	4.8E+00	3.7E+00	1.2E+01	1000	100	9.65E+02	89%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T03-C	1	5.27E+01			5.27E+01	1.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T04-C	1	2.96E+01			2.96E+01	3.3E+01	3.7E+00	1.2E+01					VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T05-C	1	3.64E+01			3.64E+01	1.6E+01	3.7E+00	1.2E+01					VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T06-C	1	1.73E+01			1.73E+01	1.1E+01	3.7E+00	1.2E+01					VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T07-C	1	3.57E+01			3.57E+01	1.5E+01	3.7E+00	1.2E+01					VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T08-C	1	3.31E+01			3.31E+01	6.0E+01	3.7E+00	1.2E+01					VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-T09-C	1	1.04E+03			1.04E+03	1.4E+00	3.7E+00	1.2E+01					VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-B01-A	1	2.52E+01			2.52E+01	3.6E+00	3.7E+00	1.2E+01					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-B02-A	1	3.84E+01			3.84E+01	1.1E+01	3.7E+00	1.2E+01					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1313-B03-A	1	3.78E+01			3.78E+01	2.5E+01	3.7E+00	1.2E+01					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	CFS-L11-1313-T01-A	1	2.44E+04			2.44E+04	2.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T02-A	1	1.81E+04			1.81E+04	9.2E-01	1.6E+00	5.1E+00	1000	100	1.90E+04	90%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T03-A	1	1.36E+04			1.36E+04	4.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T04-A	1	1.18E+04			1.18E+04	3.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T05-A	1	1.14E+04			1.14E+04	3.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T06-A	1	9.75E+03			9.75E+03	2.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T07-A	1	1.24E+04			1.24E+04	3.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T08-A	1	1.54E+04			1.54E+04	2.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T09-A	1	2.24E+04			2.24E+04	7.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T01-B	1	2.15E+04			2.15E+04	1.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T02-B	1	1.66E+04			1.66E+04	3.5E-01	1.6E+00	5.1E+00	1000	100	1.76E+04	95%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T03-B	1	1.17E+04			1.17E+04	1.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T04-B	1	1.16E+04			1.16E+04	2.7E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T05-B	1	1.08E+04			1.08E+04	5.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T06-B	1	9.24E+03			9.24E+03	1.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T07-B	1	1.16E+04			1.16E+04	7.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T08-B	1	1.46E+04			1.46E+04	1.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T09-B	1	2.16E+04			2.16E+04	4.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T01-C	1	2.20E+04			2.20E+04	5.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T02-C	1	1.82E+04			1.82E+04	8.2E+00	1.6E+00	5.1E+00	1000	100	1.91E+04	98%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T03-C	1	1.22E+04			1.22E+04	1.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T04-C	1	1.18E+04			1.18E+04	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T05-C	1	1.08E+04			1.08E+04	9.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T06-C	1	9.46E+03			9.46E+03	2.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T07-C	1	1.18E+04			1.18E+04	7.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T08-C	1	1.42E+04			1.42E+04	1.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-T09-C	1	2.25E+04			2.25E+04	3.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-B01-A	1	6.44E+01			6.44E+01	2.3E+00	1.6E+00	5.1E+00					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-B02-A	1	9.66E+01			9.66E+01	4.5E+00	1.6E+00	5.1E+00					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1313-B03-A	1	1.78E+03			1.78E+03	1.2E+00	1.6E+00	5.1E+00					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	CFS-L11-1313-T01-A	1	5.48E+02			5.48E+02	2.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T02-A	1	5.98E+02			5.98E+02	2.7E+00	1.5E+01	4.8E+01	10	100	1.47E+03	87%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T03-A	1	2.28E+02			2.28E+02	2.8E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T04-A	1	1.24E+02			1.24E+02	1.0E+01	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T05-A	1	8.12E+01			8.12E+01	1.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T06-A	1	7.00E+01			7.00E+01	1.0E+01	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T07-A	1	1.30E+02			1.30E+02	7.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T08-A	1	2.05E+02			2.05E+02	2.0E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T09-A	1	3.17E+02			3.17E+02	2.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T01-B	1	5.44E+02			5.44E+02	5.6E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T02-B	1	6.03E+02			6.03E+02	1.1E+00	1.5E+01	4.8E+01	10	100	1.48E+03	88%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T03-B	1	2.15E+02			2.15E+02	6.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T04-B	1	1.26E+02			1.26E+02	1.2E+01	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T05-B	1	8.40E+01			8.40E+01	1.0E+01	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T06-B	1	7.79E+01			7.79E+01	3.4E+01	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T07-B	1	9.56E+01			9.56E+01	8.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T08-B	1	1.87E+02			1.87E+02	9.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T09-B	1	3.06E+02			3.06E+02	6.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T01-C	1	5.27E+02			5.27E+02	2.2E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T02-C	1	6.23E+02			6.23E+02	5.2E+00	1.5E+01	4.8E+01	10	100	1.52E+03	90%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T03-C	1	2.24E+02			2.24E+02	8.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T04-C	1	1.30E+02			1.30E+02	6.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T05-C	1	7.43E+01			7.43E+01	1.0E+01	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T06-C	1	6.44E+01			6.44E+01	1.6E+01	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T07-C	1	1.12E+02			1.12E+02	1.5E+01	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T08-C	1	1.99E+02			1.99E+02	1.9E+01	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-T09-C	1	3.02E+02			3.02E+02	7.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-B01-A	1	7.50E+00	U1/2		7.50E+00	5.1E+02	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-B02-A	1	7.50E+00	U1/2		7.50E+00	1.6E+02	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1313-B03-A	1	7.50E+00	U1/2		7.50E+00	6.0E+01	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	CFS-L11-1313-T01-A	1	3.23E+02			3.23E+02	7.5E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T02-A	1	3.04E+02			3.04E+02	3.1E-01	1.1E+00	3.5E+00	1000	100	1.40E+03	109%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T03-A	1	5.31E+02			5.31E+02	8.5E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T04-A	1	6.56E+02			6.56E+02	5.8E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T05-A	1	1.28E+03			1.28E+03	5.7E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T06-A	1	3.41E+03			3.41E+03	1.1E+00	1.1E+00	3.5E+00			---		VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T07-A	1	2.35E+04			2.35E+04	8.5E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T08-A	1	4.93E+04			4.93E+04	2.7E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T09-A	1	1.45E+05			1.45E+05	4.9E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T01-B	1	3.16E+02			3.16E+02	5.9E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T02-B	1	3.25E+02			3.25E+02	6.1E-01	1.1E+00	3.5E+00	1000	100	1.36E+03	104%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T03-B	1	5.02E+02			5.02E+02	4.2E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T04-B	1	6.79E+02			6.79E+02	3.5E+00	1.1E+00	3.5E+00			---		VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T05-B	1	1.25E+03			1.25E+03	4.0E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T06-B	1	3.26E+03			3.26E+03	1.2E+00	1.1E+00	3.5E+00			---		VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T07-B	1	2.25E+04			2.25E+04	3.9E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T08-B	1	4.71E+04			4.71E+04	1.9E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T09-B	1	1.51E+05			1.51E+05	8.8E-01	1.1E+00	3.5E+00			---		VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T01-C	1	3.34E+02			3.34E+02	1.3E+00	1.1E+00	3.5E+00			---		VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T02-C	1	3.37E+02			3.37E+02	9.5E+00	1.1E+00	3.5E+00	1000	100	1.42E+03	108%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T03-C	1	5.29E+02			5.29E+02	1.2E+00	1.1E+00	3.5E+00			---		VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T04-C	1	6.54E+02			6.54E+02	1.2E+00	1.1E+00	3.5E+00					VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T05-C	1	1.17E+03			1.17E+03	4.8E-01	1.1E+00	3.5E+00					VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T06-C	1	3.18E+03			3.18E+03	4.1E-01	1.1E+00	3.5E+00					VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T07-C	1	2.27E+04			2.27E+04	5.3E-01	1.1E+00	3.5E+00					VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T08-C	1	4.78E+04			4.78E+04	1.7E+00	1.1E+00	3.5E+00					VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-T09-C	1	1.51E+05			1.51E+05	6.5E-01	1.1E+00	3.5E+00					VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-B01-A	1	8.96E+00			8.96E+00	2.3E+01	1.1E+00	3.5E+00					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-B02-A	1	6.53E+01			6.53E+01	7.5E+00	1.1E+00	3.5E+00					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1313-B03-A	1	2.49E+04			2.49E+04	8.9E-01	1.1E+00	3.5E+00					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	CFS-L11-1313-T01-A	1	5.91E+05			5.91E+05	6.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T02-A	1	4.51E+05			4.51E+05	3.4E-02	2.5E+00	8.0E+00	1000	100	4.52E+05	92%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T03-A	1	2.47E+05			2.47E+05	6.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T04-A	1	1.85E+05			1.85E+05	1.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T05-A	1	1.24E+05			1.24E+05	1.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T06-A	1	2.50E+04			2.50E+04	1.0E+00	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T07-A	1	2.62E+04			2.62E+04	5.6E-02	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T08-A	1	3.01E+04			3.01E+04	8.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T09-A	1	3.81E+04			3.81E+04	3.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T01-B	1	5.66E+05			5.66E+05	2.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T02-B	1	4.35E+05			4.35E+05	2.3E-01	2.5E+00	8.0E+00	1000	100	4.36E+05	88%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T03-B	1	2.26E+05			2.26E+05	4.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T04-B	1	1.77E+05			1.77E+05	1.4E+00	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T05-B	1	1.17E+05			1.17E+05	4.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T06-B	1	2.23E+04			2.23E+04	1.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T07-B	1	2.39E+04			2.39E+04	6.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T08-B	1	2.83E+04			2.83E+04	4.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T09-B	1	3.51E+04			3.51E+04	9.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T01-C	1	5.71E+05			5.71E+05	4.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T02-C	1	4.38E+05			4.38E+05	1.3E+00	2.5E+00	8.0E+00	1000	100	4.39E+05	91%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T03-C	1	2.33E+05			2.33E+05	2.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T04-C	1	1.86E+05			1.86E+05	2.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T05-C	1	1.23E+05			1.23E+05	3.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T06-C	1	2.13E+04			2.13E+04	5.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T07-C	1	2.32E+04			2.32E+04	4.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T08-C	1	2.69E+04			2.69E+04	7.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-T09-C	1	3.63E+04			3.63E+04	2.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-B01-A	1	1.32E+02			1.32E+02	1.6E+00	2.5E+00	8.0E+00					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-B02-A	1	3.42E+02			3.42E+02	1.2E+00	2.5E+00	8.0E+00					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1313-B03-A	1	5.90E+05			5.90E+05	4.3E-01	2.5E+00	8.0E+00					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	CFS-L11-1313-T01-A	1	2.91E+03			2.91E+03	9.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T02-A	1	3.41E+03			3.41E+03	7.0E-01	1.0E+00	3.2E+00	1000	100	4.30E+03	90%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T03-A	1	3.91E+03			3.91E+03	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T04-A	1	3.31E+03			3.31E+03	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T05-A	1	3.31E+03			3.31E+03	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T06-A	1	1.44E+03			1.44E+03	9.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T07-A	1	9.81E+02			9.81E+02	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T08-A	1	1.07E+03			1.07E+03	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T09-A	1	1.33E+03			1.33E+03	3.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T01-B	1	2.91E+03			2.91E+03	9.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T02-B	1	3.30E+03			3.30E+03	1.8E+00	1.0E+00	3.2E+00	1000	100	4.15E+03	86%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T03-B	1	3.55E+03			3.55E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T04-B	1	3.24E+03			3.24E+03	2.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T05-B	1	3.17E+03			3.17E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T06-B	1	1.45E+03			1.45E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T07-B	1	9.49E+02			9.49E+02	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T08-B	1	1.03E+03			1.03E+03	1.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T09-B	1	1.44E+03			1.44E+03	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T01-C	1	2.79E+03			2.79E+03	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T02-C	1	3.57E+03			3.57E+03	6.5E+00	1.0E+00	3.2E+00	1000	100	4.50E+03	93%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T03-C	1	3.74E+03			3.74E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T04-C	1	3.29E+03			3.29E+03	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T05-C	1	3.36E+03			3.36E+03	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T06-C	1	1.43E+03			1.43E+03	3.2E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T07-C	1	9.67E+02			9.67E+02	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T08-C	1	1.03E+03			1.03E+03	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-T09-C	1	1.42E+03			1.42E+03	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	3.0E+01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	2.3E+02	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1313-B03-A	1	1.25E+01			1.25E+01	2.9E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	CFS-L11-1313-T01-A	1	1.29E+06			1.29E+06	1.9E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T02-A	1	1.02E+06			1.02E+06	1.0E+00	6.8E+00	2.2E+01	1000	100	1.02E+06	83%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T03-A	1	7.47E+05			7.47E+05	7.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T04-A	1	6.83E+05			6.83E+05	1.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T05-A	1	6.60E+05			6.60E+05	3.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T06-A	1	6.11E+05			6.11E+05	1.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T07-A	1	6.32E+05			6.32E+05	4.3E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T08-A	1	7.14E+05			7.14E+05	4.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T09-A	1	7.75E+05			7.75E+05	1.8E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T01-B	1	1.21E+06			1.21E+06	7.7E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T02-B	1	9.77E+05			9.77E+05	2.3E-01	6.8E+00	2.2E+01	1000	100	9.78E+05	90%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T03-B	1	6.86E+05			6.86E+05	1.1E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T04-B	1	6.85E+05			6.85E+05	2.9E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T05-B	1	6.53E+05			6.53E+05	4.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T06-B	1	5.97E+05			5.97E+05	4.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T07-B	1	6.29E+05			6.29E+05	4.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T08-B	1	6.89E+05			6.89E+05	5.8E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T09-B	1	7.23E+05			7.23E+05	2.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T01-C	1	1.24E+06			1.24E+06	4.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T02-C	1	1.05E+06			1.05E+06	8.0E+00	6.8E+00	2.2E+01	1000	100	1.05E+06	88%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T03-C	1	7.15E+05			7.15E+05	1.1E+00	6.8E+00	2.2E+01			---		VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T04-C	1	6.87E+05			6.87E+05	1.1E+00	6.8E+00	2.2E+01					VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T05-C	1	6.57E+05			6.57E+05	8.3E-01	6.8E+00	2.2E+01					VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T06-C	1	5.90E+05			5.90E+05	3.7E-01	6.8E+00	2.2E+01					VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T07-C	1	6.29E+05			6.29E+05	4.2E-01	6.8E+00	2.2E+01					VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T08-C	1	6.86E+05			6.86E+05	5.8E-01	6.8E+00	2.2E+01					VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-T09-C	1	7.70E+05			7.70E+05	5.1E-02	6.8E+00	2.2E+01					VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	2.2E+01	6.8E+00	2.2E+01					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	3.1E+01	6.8E+00	2.2E+01					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	4.5E+00	6.8E+00	2.2E+01					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

TI	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	CFS-L11-1313-T01-A	1	6.67E+01			6.67E+01	4.8E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T02-A	1	6.65E+01			6.65E+01	7.2E+00	4.6E+00	1.5E+01	10	100	9.67E+02	90%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T03-A	1	1.53E+02			1.53E+02	6.4E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T04-A	1	1.68E+02			1.68E+02	3.2E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T05-A	1	2.27E+02			2.27E+02	2.4E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T06-A	1	2.41E+02			2.41E+02	2.2E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T07-A	1	4.50E+02			4.50E+02	2.0E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T08-A	1	6.84E+02			6.84E+02	7.1E-01	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T09-A	1	1.19E+03			1.19E+03	1.3E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T01-B	1	6.00E+01			6.00E+01	9.6E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T02-B	1	6.41E+01			6.41E+01	1.2E+01	4.6E+00	1.5E+01	10	100	9.42E+02	88%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T03-B	1	1.29E+02			1.29E+02	3.9E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T04-B	1	1.74E+02			1.74E+02	2.5E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T05-B	1	2.26E+02			2.26E+02	1.6E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T06-B	1	2.33E+02			2.33E+02	3.5E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T07-B	1	4.32E+02			4.32E+02	1.6E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T08-B	1	6.59E+02			6.59E+02	1.9E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T09-B	1	1.09E+03			1.09E+03	5.2E-01	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T01-C	1	6.77E+01			6.77E+01	5.0E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T02-C	1	6.95E+01			6.95E+01	1.5E+01	4.6E+00	1.5E+01	10	100	9.75E+02	91%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T03-C	1	1.34E+02			1.34E+02	3.1E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T04-C	1	1.71E+02			1.71E+02	1.8E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T05-C	1	2.09E+02			2.09E+02	2.0E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T06-C	1	2.34E+02			2.34E+02	7.7E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T07-C	1	4.26E+02			4.26E+02	9.4E-01	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T08-C	1	6.53E+02			6.53E+02	2.6E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-T09-C	1	1.15E+03			1.15E+03	7.2E-01	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	1.2E+02	4.6E+00	1.5E+01					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	8.1E+01	4.6E+00	1.5E+01					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	3.1E+02	4.6E+00	1.5E+01					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	CFS-L11-1313-T01-A	1	1.00E+00	U1/2		1.00E+00	4.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T02-A	1	1.00E+00	U1/2		1.00E+00	2.6E+00	2.0E+00	6.4E+00	10	100	9.49E+02	95%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	8.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	3.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	6.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	6.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	2.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T08-A	1	2.94E+00	E		2.94E+00	3.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T09-A	1	1.14E+01			1.14E+01	3.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T01-B	1	1.00E+00	U1/2		1.00E+00	6.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T02-B	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00	10	100	9.05E+02	90%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	3.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	1.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	6.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T08-B	1	2.28E+00	E		2.28E+00	1.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T09-B	1	9.53E+00			9.53E+00	2.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T01-C	1	1.00E+00	U1/2		1.00E+00	2.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T02-C	1	1.00E+00	U1/2		1.00E+00	2.4E+00	2.0E+00	6.4E+00	10	100	9.67E+02	97%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	5.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	4.4E+00	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	7.6E+00	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	3.4E+00	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	2.4E+01	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T08-C	1	2.56E+00	E		2.56E+00	2.2E+00	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-T09-C	1	1.04E+01			1.04E+01	8.4E+00	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.3E+00	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	4.6E+00	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1313-B03-A	1	6.72E+00			6.72E+00	9.8E-01	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	CFS-L11-1313-T01-A	1	4.36E+01			4.36E+01	1.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T02-A	1	4.07E+01			4.07E+01	2.9E+00	1.5E+00	4.8E+00	10	100	1.07E+03	103%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T03-A	1	4.03E+01			4.03E+01	6.1E-01	1.5E+00	4.8E+00			---		VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T04-A	1	4.05E+01			4.05E+01	1.6E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T05-A	1	4.14E+01			4.14E+01	2.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T06-A	1	4.31E+01			4.31E+01	1.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T07-A	1	5.35E+01			5.35E+01	2.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T08-A	1	7.00E+01			7.00E+01	3.7E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T09-A	1	4.90E+02			4.90E+02	7.8E-01	1.5E+00	4.8E+00			---		VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T01-B	1	4.36E+01			4.36E+01	4.3E-01	1.5E+00	4.8E+00			---		VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T02-B	1	3.95E+01			3.95E+01	9.7E-01	1.5E+00	4.8E+00	10	100	1.02E+03	98%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T03-B	1	3.92E+01			3.92E+01	1.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T04-B	1	4.09E+01			4.09E+01	4.0E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T05-B	1	4.21E+01			4.21E+01	1.6E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T06-B	1	4.29E+01			4.29E+01	2.0E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T07-B	1	5.29E+01			5.29E+01	3.9E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T08-B	1	6.63E+01			6.63E+01	3.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T09-B	1	4.43E+02			4.43E+02	5.4E-01	1.5E+00	4.8E+00			---		VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T01-C	1	4.61E+01			4.61E+01	5.6E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T02-C	1	4.27E+01			4.27E+01	9.6E+00	1.5E+00	4.8E+00	10	100	1.08E+03	104%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T03-C	1	4.02E+01			4.02E+01	2.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T04-C	1	4.08E+01			4.08E+01	2.6E+00	1.5E+00	4.8E+00					VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T05-C	1	4.16E+01			4.16E+01	1.4E+00	1.5E+00	4.8E+00					VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T06-C	1	4.24E+01			4.24E+01	3.4E+00	1.5E+00	4.8E+00					VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T07-C	1	5.36E+01			5.36E+01	2.4E+00	1.5E+00	4.8E+00					VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T08-C	1	6.92E+01			6.92E+01	2.8E+00	1.5E+00	4.8E+00					VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-T09-C	1	4.63E+02			4.63E+02	9.3E-01	1.5E+00	4.8E+00					VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-B01-A	1	7.50E-01	U1/2		7.50E-01	9.5E+01	1.5E+00	4.8E+00					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-B02-A	1	7.50E-01	U1/2		7.50E-01	8.7E+01	1.5E+00	4.8E+00					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1313-B03-A	1	7.50E-01	U1/2		7.50E-01	6.3E+01	1.5E+00	4.8E+00					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	CFS-L11-1313-T01-A	1	4.29E+03			4.29E+03	2.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 9:57 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T02-A	1	2.43E+03			2.43E+03	8.1E-01	1.0E+00	3.2E+00	10	100	3.37E+03	94%	VU ICP-OES	5/31/11 9:58 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T03-A	1	1.04E+01			1.04E+01	5.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:00 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T04-A	1	1.61E+02			1.61E+02	8.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:02 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T05-A	1	2.74E+02			2.74E+02	3.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:03 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T06-A	1	1.80E+04			1.80E+04	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:05 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T07-A	1	1.46E+05			1.46E+05	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:07 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T08-A	1	1.74E+05			1.74E+05	7.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:08 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T09-A	1	1.68E+05			1.68E+05	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:10 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T01-B	1	3.88E+03			3.88E+03	5.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:17 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T02-B	1	2.13E+03			2.13E+03	2.1E+00	1.0E+00	3.2E+00	10	100	3.02E+03	89%	VU ICP-OES	5/31/11 10:18 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T03-B	1	2.85E+01			2.85E+01	1.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:20 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T04-B	1	9.50E+00			9.50E+00	3.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:22 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T05-B	1	2.73E+02			2.73E+02	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:23 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T06-B	1	1.64E+04			1.64E+04	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:25 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T07-B	1	1.44E+05			1.44E+05	2.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:27 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T08-B	1	1.72E+05			1.72E+05	3.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:28 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T09-B	1	1.63E+05			1.63E+05	5.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:30 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T01-C	1	4.07E+03			4.07E+03	2.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:37 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T02-C	1	2.54E+03			2.54E+03	6.2E+00	1.0E+00	3.2E+00	10	100	3.39E+03	85%	VU ICP-OES	5/31/11 10:38 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T03-C	1	8.08E+00			8.08E+00	1.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/31/11 10:40 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T04-C	1	8.87E+00			8.87E+00	3.1E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:42 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T05-C	1	2.13E+02			2.13E+02	8.7E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:43 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T06-C	1	1.54E+04			1.54E+04	6.7E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:45 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T07-C	1	1.44E+05			1.44E+05	4.0E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:47 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T08-C	1	1.76E+05			1.76E+05	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:48 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-T09-C	1	1.65E+05			1.65E+05	4.2E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 10:50 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-B01-A	1	1.20E+01			1.20E+01	8.1E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 9:48 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-B02-A	1	1.98E+02			1.98E+02	2.8E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 9:50 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1313-B03-A	1	4.66E+01			4.66E+01	1.5E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 9:55 AM	EPA Interlab L11 1313-1316 CFS

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	CFS-LRef-1313-T01-A	1	9.81E+04			9.81E+04	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T02-A	1	3.81E+04			3.81E+04	2.8E+00	1.0E+00	3.2E+00	1000	100	3.90E+04	95%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T03-A	1	3.20E+03			3.20E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T04-A	1	4.94E+01			4.94E+01	8.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T05-A	1	4.28E+01			4.28E+01	7.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T06-A	1	4.46E+01			4.46E+01	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T07-A	1	1.30E+02			1.30E+02	7.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T08-A	1	1.11E+02			1.11E+02	2.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T09-A	1	8.33E+01			8.33E+01	3.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T01-B	1	9.88E+04			9.88E+04	4.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T02-B	1	3.71E+04			3.71E+04	1.0E+00	1.0E+00	3.2E+00	1000	100	3.81E+04	93%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T03-B	1	3.18E+03			3.18E+03	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T04-B	1	3.86E+01			3.86E+01	7.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T05-B	1	3.83E+01			3.83E+01	3.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T06-B	1	5.13E+01			5.13E+01	4.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T07-B	1	1.16E+02			1.16E+02	2.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T08-B	1	1.03E+02			1.03E+02	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T09-B	1	8.77E+01			8.77E+01	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T01-C	1	9.91E+04			9.91E+04	7.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T02-C	1	3.68E+04			3.68E+04	1.2E+00	1.0E+00	3.2E+00	1000	100	3.78E+04	97%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T03-C	1	3.20E+03			3.20E+03	9.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T04-C	1	4.20E+01			4.20E+01	4.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T05-C	1	4.67E+01			4.67E+01	5.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T06-C	1	4.47E+01			4.47E+01	3.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T07-C	1	1.10E+02			1.10E+02	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T08-C	1	1.10E+02			1.10E+02	4.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T09-C	1	9.23E+01			9.23E+01	3.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	8.9E+00	1.0E+00	3.2E+00					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	2.0E+01	1.0E+00	3.2E+00					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	2.9E+02	1.0E+00	3.2E+00					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	CFS-LRef-1313-T01-A	1	1.46E+03			1.46E+03	1.2E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T02-A	1	1.12E+03			1.12E+03	1.0E+01	7.5E+00	2.4E+01	10	100	2.03E+03	91%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T03-A	1	8.04E+01			8.04E+01	1.8E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T04-A	1	4.57E+01			4.57E+01	9.3E+00	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T05-A	1	2.84E+01			2.84E+01	2.2E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T06-A	1	3.70E+01			3.70E+01	1.1E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T07-A	1	2.54E+01			2.54E+01	1.8E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T08-A	1	1.46E+01	E		1.46E+01	1.6E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T09-A	1	9.61E+00	E		9.61E+00	9.6E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T01-B	1	1.40E+03			1.40E+03	3.7E+00	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T02-B	1	1.04E+03			1.04E+03	8.0E+00	7.5E+00	2.4E+01	10	100	1.98E+03	93%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T03-B	1	9.55E+01			9.55E+01	2.8E+00	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T04-B	1	3.29E+01			3.29E+01	3.3E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T05-B	1	3.94E+01			3.94E+01	2.6E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T06-B	1	2.75E+01			2.75E+01	3.2E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T07-B	1	3.39E+01			3.39E+01	5.1E+00	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T08-B	1	1.01E+01	E		1.01E+01	4.5E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T09-B	1	9.74E+00	E		9.74E+00	6.5E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T01-C	1	1.36E+03			1.36E+03	3.6E+00	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T02-C	1	1.07E+03			1.07E+03	8.9E+00	7.5E+00	2.4E+01	10	100	1.97E+03	90%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T03-C	1	9.07E+01			9.07E+01	2.9E+00	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T04-C	1	3.37E+01			3.37E+01	1.5E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T05-C	1	3.97E+01			3.97E+01	2.0E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T06-C	1	4.48E+01			4.48E+01	1.2E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T07-C	1	2.52E+01			2.52E+01	1.6E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T08-C	1	1.64E+01	E		1.64E+01	1.4E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T09-C	1	8.28E+00	E		8.28E+00	3.3E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-B01-A	1	8.56E+00	E		8.56E+00	3.6E+01	7.5E+00	2.4E+01					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-B02-A	1	9.51E+00	E		9.51E+00	3.3E+01	7.5E+00	2.4E+01					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-B03-A	1	2.07E+01	E		2.07E+01	1.2E+02	7.5E+00	2.4E+01					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	CFS-LRef-1313-T01-A	1	8.06E+04			8.06E+04	2.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T02-A	1	1.22E+03			1.22E+03	1.5E+00	1.1E+01	3.5E+01	10	100	2.12E+03	90%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T03-A	1	1.05E+02			1.05E+02	5.7E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T04-A	1	2.54E+01	E		2.54E+01	2.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T05-A	1	2.30E+01	E		2.30E+01	2.8E+01	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T06-A	1	2.94E+01	E		2.94E+01	1.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T07-A	1	9.28E+01			9.28E+01	6.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T08-A	1	1.83E+02			1.83E+02	8.6E-01	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T09-A	1	2.12E+02			2.12E+02	6.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T01-B	1	7.93E+04			7.93E+04	5.7E-01	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T02-B	1	1.27E+03			1.27E+03	6.9E-01	1.1E+01	3.5E+01	10	100	2.17E+03	90%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T03-B	1	1.09E+02			1.09E+02	7.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T04-B	1	2.15E+01	E		2.15E+01	5.8E+01	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T05-B	1	3.25E+01	E		3.25E+01	6.2E+01	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T06-B	1	4.25E+01			4.25E+01	1.1E+01	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T07-B	1	1.04E+02			1.04E+02	7.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T08-B	1	2.08E+02			2.08E+02	3.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T09-B	1	2.04E+02			2.04E+02	1.0E+01	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T01-C	1	8.69E+04			8.69E+04	6.9E-01	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T02-C	1	1.03E+03			1.03E+03	1.5E+00	1.1E+01	3.5E+01	10	100	1.94E+03	91%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T03-C	1	1.17E+02			1.17E+02	5.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T04-C	1	2.26E+01	E		2.26E+01	4.5E+01	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T05-C	1	2.95E+01	E		2.95E+01	2.7E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T06-C	1	3.89E+01			3.89E+01	8.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T07-C	1	1.04E+02			1.04E+02	4.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T08-C	1	2.52E+02			2.52E+02	5.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T09-C	1	2.20E+02			2.20E+02	7.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-B01-A	1	5.50E+00	U1/2		5.50E+00	1.0E+02	1.1E+01	3.5E+01					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-B02-A	1	5.50E+00	U1/2		5.50E+00	2.5E+01	1.1E+01	3.5E+01					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-B03-A	1	5.50E+00	U1/2		5.50E+00	8.3E+01	1.1E+01	3.5E+01					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	CFS-LRef-1313-T01-A	1	7.61E+02			7.61E+02	1.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T02-A	1	6.78E+02			6.78E+02	1.7E+00	1.0E+00	3.2E+00	1000	100	1.60E+03	93%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T03-A	1	3.14E+02			3.14E+02	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T04-A	1	1.63E+02			1.63E+02	1.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T05-A	1	1.27E+02			1.27E+02	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T06-A	1	1.23E+02			1.23E+02	8.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T07-A	1	1.64E+02			1.64E+02	4.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T08-A	1	7.74E+01			7.74E+01	2.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T09-A	1	6.79E+01			6.79E+01	2.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T01-B	1	7.78E+02			7.78E+02	1.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T02-B	1	6.84E+02			6.84E+02	1.5E+00	1.0E+00	3.2E+00	1000	100	1.61E+03	92%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T03-B	1	3.12E+02			3.12E+02	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T04-B	1	1.69E+02			1.69E+02	5.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T05-B	1	1.30E+02			1.30E+02	6.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T06-B	1	1.21E+02			1.21E+02	1.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T07-B	1	1.71E+02			1.71E+02	9.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T08-B	1	8.49E+01			8.49E+01	7.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T09-B	1	7.58E+01			7.58E+01	8.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T01-C	1	8.48E+02			8.48E+02	1.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T02-C	1	6.94E+02			6.94E+02	1.5E+00	1.0E+00	3.2E+00	1000	100	1.61E+03	91%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T03-C	1	3.07E+02			3.07E+02	8.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T04-C	1	1.61E+02			1.61E+02	1.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T05-C	1	1.26E+02			1.26E+02	3.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T06-C	1	1.18E+02			1.18E+02	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T07-C	1	1.66E+02			1.66E+02	6.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T08-C	1	8.36E+01			8.36E+01	4.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T09-C	1	7.21E+01			7.21E+01	6.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-B01-A	1	1.30E+01			1.30E+01	5.5E+00	1.0E+00	3.2E+00					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-B02-A	1	1.36E+01			1.36E+01	6.5E+00	1.0E+00	3.2E+00					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-B03-A	1	1.45E+01			1.45E+01	1.8E+01	1.0E+00	3.2E+00					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	CFS-LRef-1313-T01-A	1	4.94E+00			4.94E+00	7.1E-02	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T02-A	1	3.70E+01			3.70E+01	2.6E+00	1.0E+00	3.2E+00	10	100	1.08E+03	105%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T03-A	1	2.77E+01			2.77E+01	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T04-A	1	9.34E+01			9.34E+01	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T05-A	1	7.30E+01			7.30E+01	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T06-A	1	7.69E+01			7.69E+01	6.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T07-A	1	1.66E+02			1.66E+02	3.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T08-A	1	5.36E+00			5.36E+00	2.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T09-A	1	2.56E+00	E		2.56E+00	6.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T01-B	1	5.06E+00			5.06E+00	1.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T02-B	1	3.53E+01			3.53E+01	1.5E+00	1.0E+00	3.2E+00	10	100	1.09E+03	106%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T03-B	1	2.73E+01			2.73E+01	9.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T04-B	1	9.76E+01			9.76E+01	6.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T05-B	1	7.73E+01			7.73E+01	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T06-B	1	8.36E+01			8.36E+01	6.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T07-B	1	1.69E+02			1.69E+02	6.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T08-B	1	3.99E+00			3.99E+00	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T09-B	1	2.45E+00	E		2.45E+00	2.4E+01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T01-C	1	4.99E+00			4.99E+00	1.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T02-C	1	3.82E+01			3.82E+01	7.7E-01	1.0E+00	3.2E+00	10	100	1.08E+03	104%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T03-C	1	2.75E+01			2.75E+01	3.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T04-C	1	9.70E+01			9.70E+01	6.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T05-C	1	7.44E+01			7.44E+01	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T06-C	1	8.19E+01			8.19E+01	8.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T07-C	1	1.64E+02			1.64E+02	2.5E-02	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T08-C	1	3.91E+00			3.91E+00	6.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T09-C	1	1.37E+00	E		1.37E+00	7.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	4.9E+00	1.0E+00	3.2E+00					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	3.7E+01	1.0E+00	3.2E+00					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	3.1E+01	1.0E+00	3.2E+00					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	CFS-LRef-1313-T01-A	1	9.50E-01	U1/2		9.50E-01	3.9E+02	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T02-A	1	7.56E+00			7.56E+00	7.7E+00	1.9E+00	6.0E+00	10	100	1.03E+03	102%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T03-A	1	2.54E+00	E		2.54E+00	2.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T04-A	1	9.50E-01	U1/2		9.50E-01	2.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T05-A	1	9.50E-01	U1/2		9.50E-01	2.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T06-A	1	9.50E-01	U1/2		9.50E-01	3.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T07-A	1	9.50E-01	U1/2		9.50E-01	1.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T08-A	1	9.50E-01	U1/2		9.50E-01	1.6E+03	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T09-A	1	9.50E-01	U1/2		9.50E-01	7.9E+02	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T01-B	1	9.50E-01	U1/2		9.50E-01	1.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T02-B	1	6.72E+00			6.72E+00	1.1E+01	1.9E+00	6.0E+00	10	100	1.04E+03	103%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T03-B	1	2.54E+00	E		2.54E+00	7.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T04-B	1	9.50E-01	U1/2		9.50E-01	6.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T05-B	1	9.50E-01	U1/2		9.50E-01	1.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T06-B	1	9.50E-01	U1/2		9.50E-01	6.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T07-B	1	9.50E-01	U1/2		9.50E-01	1.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T08-B	1	9.50E-01	U1/2		9.50E-01	2.6E+02	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T09-B	1	9.50E-01	U1/2		9.50E-01	9.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T01-C	1	9.50E-01	U1/2		9.50E-01	2.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T02-C	1	6.68E+00			6.68E+00	8.4E+00	1.9E+00	6.0E+00	10	100	1.01E+03	100%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T03-C	1	2.68E+00	E		2.68E+00	4.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T04-C	1	9.50E-01	U1/2		9.50E-01	4.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T05-C	1	9.50E-01	U1/2		9.50E-01	2.9E+02	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T06-C	1	9.50E-01	U1/2		9.50E-01	8.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T07-C	1	9.50E-01	U1/2		9.50E-01	2.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T08-C	1	9.50E-01	U1/2		9.50E-01	1.6E+02	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T09-C	1	9.50E-01	U1/2		9.50E-01	1.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	2.6E+02	1.9E+00	6.0E+00					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	2.1E+02	1.9E+00	6.0E+00					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	CFS-LRef-1313-T01-A	1	5.09E+04			5.09E+04	5.6E-01	2.2E+00	7.0E+00				---	VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T02-A	1	5.18E+04			5.18E+04	2.0E+00	2.2E+00	7.0E+00	10	100	5.26E+04	86%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T03-A	1	2.30E+04			2.30E+04	7.2E-01	2.2E+00	7.0E+00				---	VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T04-A	1	5.25E+03			5.25E+03	7.5E-01	2.2E+00	7.0E+00				---	VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T05-A	1	9.80E+01			9.80E+01	7.5E-01	2.2E+00	7.0E+00				---	VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T06-A	1	1.90E+01			1.90E+01	8.5E-01	2.2E+00	7.0E+00				---	VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T07-A	1	3.91E+00	E		3.91E+00	2.9E+01	2.2E+00	7.0E+00				---	VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T08-A	1	4.08E+00	E		4.08E+00	4.1E+00	2.2E+00	7.0E+00				---	VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T09-A	1	6.19E+00	E		6.19E+00	5.4E+00	2.2E+00	7.0E+00				---	VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T01-B	1	4.91E+04			4.91E+04	1.4E+00	2.2E+00	7.0E+00				---	VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T02-B	1	5.11E+04			5.11E+04	2.2E+00	2.2E+00	7.0E+00	10	100	5.20E+04	93%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T03-B	1	2.31E+04			2.31E+04	8.8E-01	2.2E+00	7.0E+00				---	VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T04-B	1	5.36E+03			5.36E+03	2.3E-01	2.2E+00	7.0E+00				---	VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T05-B	1	8.46E+01			8.46E+01	1.8E-01	2.2E+00	7.0E+00				---	VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T06-B	1	1.82E+01			1.82E+01	8.4E-01	2.2E+00	7.0E+00				---	VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T07-B	1	4.08E+00	E		4.08E+00	4.3E+01	2.2E+00	7.0E+00				---	VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T08-B	1	4.08E+00	E		4.08E+00	2.7E+01	2.2E+00	7.0E+00				---	VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T09-B	1	5.75E+00	E		5.75E+00	1.4E+00	2.2E+00	7.0E+00				---	VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T01-C	1	5.03E+04			5.03E+04	2.4E-01	2.2E+00	7.0E+00				---	VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T02-C	1	5.26E+04			5.26E+04	1.5E+00	2.2E+00	7.0E+00	10	100	5.36E+04	96%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T03-C	1	2.32E+04			2.32E+04	6.2E-01	2.2E+00	7.0E+00				---	VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T04-C	1	4.92E+03			4.92E+03	1.0E+00	2.2E+00	7.0E+00				---	VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T05-C	1	9.72E+01			9.72E+01	1.8E+00	2.2E+00	7.0E+00				---	VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T06-C	1	1.52E+01			1.52E+01	2.3E+00	2.2E+00	7.0E+00				---	VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T07-C	1	4.08E+00	E		4.08E+00	3.9E+01	2.2E+00	7.0E+00				---	VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T08-C	1	4.08E+00	E		4.08E+00	2.9E+01	2.2E+00	7.0E+00				---	VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T09-C	1	6.50E+00	E		6.50E+00	5.5E+00	2.2E+00	7.0E+00				---	VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-B01-A	1	4.08E+00	E		4.08E+00	2.0E+01	2.2E+00	7.0E+00					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-B02-A	1	4.08E+00	E		4.08E+00	6.1E+01	2.2E+00	7.0E+00					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-B03-A	1	4.08E+00	E		4.08E+00	6.5E+02	2.2E+00	7.0E+00					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	CFS-LRef-1313-T01-A	1	1.67E+06			1.67E+06	8.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T02-A	1	1.37E+06			1.37E+06	2.6E+00	2.6E+00	8.3E+00	1000	100	1.37E+06	84%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T03-A	1	8.76E+05			8.76E+05	9.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T04-A	1	6.80E+05			6.80E+05	5.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T05-A	1	6.19E+05			6.19E+05	1.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T06-A	1	6.16E+05			6.16E+05	4.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T07-A	1	5.98E+05			5.98E+05	5.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T08-A	1	5.73E+05			5.73E+05	1.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T09-A	1	6.15E+05			6.15E+05	3.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T01-B	1	1.66E+06			1.66E+06	1.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T02-B	1	1.39E+06			1.39E+06	1.9E+00	2.6E+00	8.3E+00	1000	100	1.39E+06	89%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T03-B	1	8.83E+05			8.83E+05	5.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T04-B	1	7.07E+05			7.07E+05	6.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T05-B	1	6.42E+05			6.42E+05	5.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T06-B	1	6.13E+05			6.13E+05	1.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T07-B	1	6.06E+05			6.06E+05	4.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T08-B	1	5.63E+05			5.63E+05	8.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T09-B	1	6.40E+05			6.40E+05	1.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T01-C	1	1.68E+06			1.68E+06	3.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T02-C	1	1.35E+06			1.35E+06	1.9E+00	2.6E+00	8.3E+00	1000	100	1.35E+06	90%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T03-C	1	8.88E+05			8.88E+05	5.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T04-C	1	6.78E+05			6.78E+05	9.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T05-C	1	6.26E+05			6.26E+05	7.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T06-C	1	6.03E+05			6.03E+05	8.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T07-C	1	5.96E+05			5.96E+05	6.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T08-C	1	5.82E+05			5.82E+05	4.6E+00	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T09-C	1	6.35E+05			6.35E+05	1.5E+00	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	5.1E+01	2.6E+00	8.3E+00					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-B02-A	1	2.72E+00	E		2.72E+00	2.0E+02	2.6E+00	8.3E+00					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	8.1E+01	2.6E+00	8.3E+00					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	CFS-LRef-1313-T01-A	1	2.23E+03			2.23E+03	8.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T02-A	1	5.34E+01			5.34E+01	2.5E+00	1.2E+00	3.8E+00	10	100	1.02E+03	96%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T03-A	1	6.00E-01	U1/2		6.00E-01	1.1E+03	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T04-A	1	6.00E-01	U1/2		6.00E-01	2.4E+03	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T05-A	1	6.00E-01	U1/2		6.00E-01	1.3E+02	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T06-A	1	6.00E-01	U1/2		6.00E-01	1.9E+02	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T07-A	1	7.17E+00			7.17E+00	6.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T08-A	1	6.35E+01			6.35E+01	1.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T09-A	1	1.09E+02			1.09E+02	9.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T01-B	1	2.16E+03			2.16E+03	1.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T02-B	1	5.86E+01			5.86E+01	4.7E-01	1.2E+00	3.8E+00	10	100	1.03E+03	97%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T03-B	1	6.00E-01	U1/2		6.00E-01	8.5E+02	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T04-B	1	6.00E-01	U1/2		6.00E-01	3.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T05-B	1	6.00E-01	U1/2		6.00E-01	1.9E+02	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T06-B	1	6.00E-01	U1/2		6.00E-01	1.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T07-B	1	8.59E+00			8.59E+00	6.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T08-B	1	5.19E+01			5.19E+01	3.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T09-B	1	1.30E+02			1.30E+02	1.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T01-C	1	2.25E+03			2.25E+03	8.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T02-C	1	5.65E+01			5.65E+01	1.9E+00	1.2E+00	3.8E+00	10	100	1.00E+03	95%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T03-C	1	6.00E-01	U1/2		6.00E-01	5.9E+02	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T04-C	1	6.00E-01	U1/2		6.00E-01	1.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T05-C	1	6.00E-01	U1/2		6.00E-01	1.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T06-C	1	6.00E-01	U1/2		6.00E-01	4.8E+01	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T07-C	1	8.15E+00			8.15E+00	1.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T08-C	1	6.32E+01			6.32E+01	5.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T09-C	1	1.07E+02			1.07E+02	7.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-B01-A	1	6.00E-01	U1/2		6.00E-01	1.4E+02	1.2E+00	3.8E+00					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-B02-A	1	6.00E-01	U1/2		6.00E-01	2.9E+02	1.2E+00	3.8E+00					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-B03-A	1	6.00E-01	U1/2		6.00E-01	8.4E+01	1.2E+00	3.8E+00					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	CFS-LRef-1313-T01-A	1	1.81E+03			1.81E+03	8.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T02-A	1	1.66E+03			1.66E+03	1.4E+00	1.8E+00	5.7E+00	10	100	2.57E+03	91%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T03-A	1	5.60E+02			5.60E+02	9.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T04-A	1	1.14E+02			1.14E+02	3.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T05-A	1	1.99E+00	E		1.99E+00	2.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T06-A	1	9.00E-01	U1/2		9.00E-01	2.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T07-A	1	9.00E-01	U1/2		9.00E-01	1.7E+02	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T08-A	1	9.00E-01	U1/2		9.00E-01	9.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T09-A	1	9.00E-01	U1/2		9.00E-01	1.2E+02	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T01-B	1	1.81E+03			1.81E+03	9.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T02-B	1	1.66E+03			1.66E+03	2.5E+00	1.8E+00	5.7E+00	10	100	2.56E+03	90%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T03-B	1	5.51E+02			5.51E+02	4.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T04-B	1	1.15E+02			1.15E+02	1.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T05-B	1	2.14E+00	E		2.14E+00	5.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T06-B	1	9.00E-01	U1/2		9.00E-01	1.9E+02	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T07-B	1	9.00E-01	U1/2		9.00E-01	7.9E+03	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T08-B	1	9.00E-01	U1/2		9.00E-01	1.6E+02	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T09-B	1	9.00E-01	U1/2		9.00E-01	4.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T01-C	1	1.81E+03			1.81E+03	1.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T02-C	1	1.71E+03			1.71E+03	9.8E-01	1.8E+00	5.7E+00	10	100	2.68E+03	96%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T03-C	1	5.64E+02			5.64E+02	5.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T04-C	1	1.04E+02			1.04E+02	6.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T05-C	1	1.83E+00	E		1.83E+00	4.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T06-C	1	9.00E-01	U1/2		9.00E-01	3.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T07-C	1	9.00E-01	U1/2		9.00E-01	1.6E+02	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T08-C	1	9.00E-01	U1/2		9.00E-01	3.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T09-C	1	9.00E-01	U1/2		9.00E-01	6.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	1.2E+02	1.8E+00	5.7E+00					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	2.7E+02	1.8E+00	5.7E+00					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	4.7E+02	1.8E+00	5.7E+00					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	CFS-LRef-1313-T01-A	1	1.12E+06			1.12E+06	5.4E-01	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T02-A	1	9.69E+05			9.69E+05	3.3E+00	3.7E+00	1.2E+01	10	100	9.70E+05	91%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T03-A	1	1.69E+05			1.69E+05	7.7E-01	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T04-A	1	1.06E+03			1.06E+03	1.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T05-A	1	7.72E+01			7.72E+01	3.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T06-A	1	5.76E+01			5.76E+01	4.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T07-A	1	1.64E+02			1.64E+02	4.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T08-A	1	9.08E+02			9.08E+02	8.6E-01	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T09-A	1	3.21E+03			3.21E+03	1.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T01-B	1	1.12E+06			1.12E+06	8.4E-01	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T02-B	1	9.74E+05			9.74E+05	4.8E-01	3.7E+00	1.2E+01	10	100	9.75E+05	95%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T03-B	1	1.71E+05			1.71E+05	6.6E-01	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T04-B	1	9.97E+02			9.97E+02	1.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T05-B	1	6.30E+01			6.30E+01	4.2E-01	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T06-B	1	7.06E+01			7.06E+01	1.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T07-B	1	1.69E+02			1.69E+02	1.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T08-B	1	7.06E+02			7.06E+02	1.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T09-B	1	3.35E+03			3.35E+03	1.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T01-C	1	1.15E+06			1.15E+06	1.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T02-C	1	9.70E+05			9.70E+05	7.6E-01	3.7E+00	1.2E+01	10	100	9.71E+05	92%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T03-C	1	1.69E+05			1.69E+05	6.0E-01	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T04-C	1	8.92E+02			8.92E+02	1.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T05-C	1	6.23E+01			6.23E+01	6.6E-01	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T06-C	1	6.08E+01			6.08E+01	4.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T07-C	1	1.61E+02			1.61E+02	8.8E-01	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T08-C	1	7.92E+02			7.92E+02	4.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T09-C	1	3.36E+03			3.36E+03	2.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	8.2E+00	3.7E+00	1.2E+01					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-B02-A	1	8.46E+00	E		8.46E+00	7.3E+00	3.7E+00	1.2E+01					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-B03-A	1	5.16E+00	E		5.16E+00	1.1E+01	3.7E+00	1.2E+01					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	CFS-LRef-1313-T01-A	1	2.71E+05			2.71E+05	5.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T02-A	1	4.36E+04			4.36E+04	1.9E+00	2.0E+00	6.4E+00	1000	100	4.45E+04	93%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	4.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	5.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	7.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	8.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	1.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T08-A	1	1.00E+00	U1/2		1.00E+00	2.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T09-A	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T01-B	1	2.65E+05			2.65E+05	3.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T02-B	1	4.68E+04			4.68E+04	1.5E+00	2.0E+00	6.4E+00	1000	100	4.78E+04	98%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	9.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	3.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	2.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	4.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	3.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T08-B	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T09-B	1	1.00E+00	U1/2		1.00E+00	5.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T01-C	1	2.94E+05			2.94E+05	4.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T02-C	1	4.63E+04			4.63E+04	1.2E+00	2.0E+00	6.4E+00	1000	100	4.71E+04	87%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	7.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	4.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	3.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	7.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T08-C	1	1.00E+00	U1/2		1.00E+00	9.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T09-C	1	1.00E+00	U1/2		1.00E+00	2.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	1.3E+00	2.0E+00	6.4E+00					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	2.2E+00	2.0E+00	6.4E+00					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	CFS-LRef-1313-T01-A	1	8.64E+03			8.64E+03	3.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T02-A	1	6.09E+03			6.09E+03	2.3E+00	6.8E+00	2.2E+01	10	100	6.96E+03	86%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T03-A	1	5.38E+03			5.38E+03	9.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T04-A	1	1.13E+03			1.13E+03	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T05-A	1	1.24E+02			1.24E+02	3.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T06-A	1	1.06E+02			1.06E+02	1.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T07-A	1	7.23E+02			7.23E+02	4.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T08-A	1	1.02E+04			1.02E+04	1.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T09-A	1	8.04E+03			8.04E+03	8.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T01-B	1	8.68E+03			8.68E+03	1.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T02-B	1	6.07E+03			6.07E+03	1.6E+00	6.8E+00	2.2E+01	10	100	7.00E+03	93%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T03-B	1	6.27E+03			6.27E+03	1.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T04-B	1	1.16E+03			1.16E+03	4.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T05-B	1	1.30E+02			1.30E+02	1.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T06-B	1	1.00E+02			1.00E+02	4.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T07-B	1	7.18E+02			7.18E+02	6.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T08-B	1	1.03E+04			1.03E+04	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T09-B	1	8.02E+03			8.02E+03	2.3E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T01-C	1	8.77E+03			8.77E+03	5.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T02-C	1	6.06E+03			6.06E+03	1.1E+00	6.8E+00	2.2E+01	10	100	6.91E+03	85%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T03-C	1	6.01E+03			6.01E+03	9.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T04-C	1	1.10E+03			1.10E+03	8.0E-02	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T05-C	1	1.21E+02			1.21E+02	3.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T06-C	1	1.05E+02			1.05E+02	5.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T07-C	1	6.42E+02			6.42E+02	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T08-C	1	1.05E+04			1.05E+04	5.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T09-C	1	7.88E+03			7.88E+03	2.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	1.5E+02	6.8E+00	2.2E+01					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-B02-A	1	1.53E+01	E		1.53E+01	1.8E+01	6.8E+00	2.2E+01					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-B03-A	1	3.40E+00	U1/2		3.40E+00	2.7E+01	6.8E+00	2.2E+01					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	CFS-LRef-1313-T01-A	1	3.00E+01			3.00E+01	7.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T02-A	1	1.39E+01			1.39E+01	2.9E+01	1.9E+00	6.0E+00	10	100	8.80E+02	87%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T03-A	1	8.29E+00			8.29E+00	5.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T04-A	1	1.19E+01			1.19E+01	1.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T05-A	1	1.10E+01			1.10E+01	4.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T06-A	1	9.38E+00			9.38E+00	3.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T07-A	1	1.32E+01			1.32E+01	6.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T08-A	1	1.20E+01			1.20E+01	5.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T09-A	1	1.30E+01			1.30E+01	2.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T01-B	1	3.61E+01			3.61E+01	1.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T02-B	1	1.38E+01			1.38E+01	1.0E+01	1.9E+00	6.0E+00	10	100	8.73E+02	86%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T03-B	1	8.55E+00			8.55E+00	1.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T04-B	1	1.06E+01			1.06E+01	1.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T05-B	1	1.19E+01			1.19E+01	2.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T06-B	1	1.17E+01			1.17E+01	2.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T07-B	1	1.14E+01			1.14E+01	6.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T08-B	1	1.22E+01			1.22E+01	1.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T09-B	1	1.32E+01			1.32E+01	4.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T01-C	1	3.59E+01			3.59E+01	4.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T02-C	1	8.95E+00			8.95E+00	1.1E+01	1.9E+00	6.0E+00	10	100	8.61E+02	85%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T03-C	1	9.79E+00			9.79E+00	1.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T04-C	1	1.14E+01			1.14E+01	7.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T05-C	1	1.08E+01			1.08E+01	1.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T06-C	1	1.10E+01			1.10E+01	3.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T07-C	1	1.23E+01			1.23E+01	6.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T08-C	1	1.27E+01			1.27E+01	3.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T09-C	1	1.38E+01			1.38E+01	5.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-B01-A	1	9.50E-01	U1/2		9.50E-01	2.1E+01	1.9E+00	6.0E+00					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-B02-A	1	9.50E-01	U1/2		9.50E-01	8.0E+00	1.9E+00	6.0E+00					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-B03-A	1	9.50E-01	U1/2		9.50E-01	2.7E+00	1.9E+00	6.0E+00					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	CFS-LRef-1313-T01-A	1	3.58E+04			3.58E+04	1.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T02-A	1	2.46E+04			2.46E+04	1.4E+00	2.0E+00	6.4E+00	10	100	2.55E+04	93%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T03-A	1	6.37E+03			6.37E+03	7.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T04-A	1	1.82E+03			1.82E+03	1.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T05-A	1	2.93E+01			2.93E+01	3.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	1.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T08-A	1	1.00E+00	U1/2		1.00E+00	1.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T09-A	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T01-B	1	3.64E+04			3.64E+04	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T02-B	1	2.52E+04			2.52E+04	1.5E+00	2.0E+00	6.4E+00	10	100	2.61E+04	93%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T03-B	1	6.21E+03			6.21E+03	6.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T04-B	1	1.91E+03			1.91E+03	6.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T05-B	1	2.29E+01			2.29E+01	4.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	4.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T08-B	1	1.00E+00	U1/2		1.00E+00	9.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T09-B	1	1.00E+00	U1/2		1.00E+00	5.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T01-C	1	3.69E+04			3.69E+04	2.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T02-C	1	2.53E+04			2.53E+04	1.7E+00	2.0E+00	6.4E+00	10	100	2.63E+04	97%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T03-C	1	6.32E+03			6.32E+03	2.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T04-C	1	1.76E+03			1.76E+03	7.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T05-C	1	2.64E+01			2.64E+01	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	3.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	4.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T08-C	1	1.00E+00	U1/2		1.00E+00	4.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T09-C	1	1.00E+00	U1/2		1.00E+00	4.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.6E+02	2.0E+00	6.4E+00					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	6.8E+01	2.0E+00	6.4E+00					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	7.0E+00	2.0E+00	6.4E+00					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	CFS-LRef-1313-T01-A	1	2.39E+05			2.39E+05	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T02-A	1	1.44E+05			1.44E+05	2.4E+00	1.0E+00	3.2E+00	1000	100	1.45E+05	87%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T03-A	1	7.52E+04			7.52E+04	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T04-A	1	6.26E+04			6.26E+04	3.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T05-A	1	5.77E+04			5.77E+04	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T06-A	1	2.84E+04			2.84E+04	1.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T07-A	1	6.53E+02			6.53E+02	5.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T08-A	1	4.53E+01			4.53E+01	1.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T09-A	1	2.51E+01			2.51E+01	3.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T01-B	1	2.34E+05			2.34E+05	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T02-B	1	1.51E+05			1.51E+05	1.3E+00	1.0E+00	3.2E+00	1000	100	1.52E+05	93%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T03-B	1	7.63E+04			7.63E+04	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T04-B	1	6.49E+04			6.49E+04	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T05-B	1	5.88E+04			5.88E+04	2.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T06-B	1	3.10E+04			3.10E+04	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T07-B	1	6.43E+02			6.43E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T08-B	1	3.77E+01			3.77E+01	1.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T09-B	1	1.58E+01			1.58E+01	9.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T01-C	1	2.38E+05			2.38E+05	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T02-C	1	1.60E+05			1.60E+05	3.7E-01	1.0E+00	3.2E+00	1000	100	1.61E+05	88%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T03-C	1	7.59E+04			7.59E+04	2.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T04-C	1	6.36E+04			6.36E+04	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T05-C	1	5.80E+04			5.80E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T06-C	1	2.97E+04			2.97E+04	9.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T07-C	1	6.66E+02			6.66E+02	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T08-C	1	2.96E+01			2.96E+01	1.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T09-C	1	2.11E+01			2.11E+01	2.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.0E+03	1.0E+00	3.2E+00					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	2.2E+02	1.0E+00	3.2E+00					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	2.7E+03	1.0E+00	3.2E+00					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	CFS-LRef-1313-T01-A	1	1.22E+02			1.22E+02	9.4E+00	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T02-A	1	1.70E+01			1.70E+01	7.6E+01	1.2E+00	3.8E+00	10	100	1.02E+03	100%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T03-A	1	8.34E+00			8.34E+00	2.0E+01	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T04-A	1	1.11E+01			1.11E+01	1.7E+01	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T05-A	1	1.19E+02			1.19E+02	1.9E+00	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T06-A	1	4.00E+02			4.00E+02	3.9E-01	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T07-A	1	1.06E+03			1.06E+03	5.8E+00	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T08-A	1	1.64E+03			1.64E+03	1.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T09-A	1	1.46E+03			1.46E+03	2.1E-01	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T01-B	1	1.25E+02			1.25E+02	2.4E+00	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T02-B	1	1.53E+01			1.53E+01	6.3E+01	1.2E+00	3.8E+00	10	100	1.03E+03	101%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T03-B	1	1.20E+01			1.20E+01	1.7E+01	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T04-B	1	9.08E+00			9.08E+00	7.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T05-B	1	1.45E+02			1.45E+02	1.4E+00	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T06-B	1	4.27E+02			4.27E+02	1.0E+00	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T07-B	1	1.13E+03			1.13E+03	3.8E-01	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T08-B	1	1.72E+03			1.72E+03	1.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T09-B	1	1.56E+03			1.56E+03	8.8E-01	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T01-C	1	1.35E+02			1.35E+02	1.5E+01	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T02-C	1	2.09E+01			2.09E+01	2.6E+01	1.2E+00	3.8E+00	10	100	9.88E+02	97%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T03-C	1	9.37E+00			9.37E+00	4.8E+00	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T04-C	1	1.02E+01			1.02E+01	3.2E+00	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T05-C	1	1.33E+02			1.33E+02	1.6E+00	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T06-C	1	4.23E+02			4.23E+02	6.6E-01	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T07-C	1	1.10E+03			1.10E+03	1.2E+00	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T08-C	1	1.78E+03			1.78E+03	4.5E+00	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T09-C	1	1.57E+03			1.57E+03	1.7E+00	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-B01-A	1	3.20E+00	E		3.20E+00	5.1E+00	1.2E+00	3.8E+00					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-B02-A	1	2.29E+00	E		2.29E+00	3.6E+01	1.2E+00	3.8E+00					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-B03-A	1	2.18E+00	E		2.18E+00	2.7E+01	1.2E+00	3.8E+00					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	CFS-LRef-1313-T01-A	1	6.80E+03			6.80E+03	1.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T02-A	1	6.42E+03			6.42E+03	1.9E+00	1.8E+00	5.7E+00	10	100	7.37E+03	95%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T03-A	1	2.09E+03			2.09E+03	1.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T04-A	1	2.72E+02			2.72E+02	2.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T05-A	1	9.00E-01	U1/2		9.00E-01	2.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T06-A	1	9.00E-01	U1/2		9.00E-01	2.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T07-A	1	9.00E-01	U1/2		9.00E-01	2.6E+02	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T08-A	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T09-A	1	9.00E-01	U1/2		9.00E-01	1.7E+02	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T01-B	1	6.95E+03			6.95E+03	1.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T02-B	1	6.50E+03			6.50E+03	1.1E+00	1.8E+00	5.7E+00	10	100	7.42E+03	91%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T03-B	1	2.08E+03			2.08E+03	4.3E-01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T04-B	1	2.65E+02			2.65E+02	4.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T05-B	1	9.00E-01	U1/2		9.00E-01	4.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T06-B	1	9.00E-01	U1/2		9.00E-01	4.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T07-B	1	9.00E-01	U1/2		9.00E-01	1.2E+02	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T08-B	1	9.00E-01	U1/2		9.00E-01	5.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T09-B	1	9.00E-01	U1/2		9.00E-01	1.7E+03	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T01-C	1	6.90E+03			6.90E+03	4.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T02-C	1	6.68E+03			6.68E+03	9.5E-01	1.8E+00	5.7E+00	10	100	7.62E+03	94%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T03-C	1	2.09E+03			2.09E+03	9.6E-02	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T04-C	1	2.41E+02			2.41E+02	6.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T05-C	1	9.00E-01	U1/2		9.00E-01	5.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T06-C	1	9.00E-01	U1/2		9.00E-01	7.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T07-C	1	9.00E-01	U1/2		9.00E-01	5.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T08-C	1	9.00E-01	U1/2		9.00E-01	1.2E+03	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T09-C	1	9.00E-01	U1/2		9.00E-01	2.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-B01-A	1	9.00E-01	U1/2		9.00E-01	2.4E+01	1.8E+00	5.7E+00					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-B02-A	1	9.00E-01	U1/2		9.00E-01	1.7E+01	1.8E+00	5.7E+00					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-B03-A	1	9.00E-01	U1/2		9.00E-01	3.2E+01	1.8E+00	5.7E+00					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	CFS-LRef-1313-T01-A	1	3.13E+03			3.13E+03	2.1E-01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T02-A	1	2.95E+01			2.95E+01	1.3E+02	3.7E+00	1.2E+01	1000	100	1.04E+03	101%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T03-A	1	1.85E+00	U1/2		1.85E+00	2.9E+02	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T04-A	1	1.85E+00	U1/2		1.85E+00	6.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T05-A	1	5.72E+00	E		5.72E+00	1.1E+02	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T06-A	1	8.37E+00	E		8.37E+00	6.2E+02	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T07-A	1	4.74E+01			4.74E+01	4.6E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T08-A	1	5.30E+01			5.30E+01	1.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T09-A	1	6.55E+01			6.55E+01	1.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T01-B	1	3.21E+03			3.21E+03	6.6E-01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T02-B	1	2.81E+01			2.81E+01	1.1E+02	3.7E+00	1.2E+01	1000	100	1.05E+03	102%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T03-B	1	1.85E+00	U1/2		1.85E+00	5.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T04-B	1	1.85E+00	U1/2		1.85E+00	1.6E+02	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T05-B	1	4.44E+00	E		4.44E+00	2.4E+02	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T06-B	1	9.38E+00	E		9.38E+00	8.4E+02	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T07-B	1	4.52E+01			4.52E+01	2.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T08-B	1	6.68E+01			6.68E+01	1.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T09-B	1	6.54E+01			6.54E+01	6.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T01-C	1	3.52E+03			3.52E+03	9.7E-01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T02-C	1	2.53E+01			2.53E+01	2.8E+01	3.7E+00	1.2E+01	1000	100	1.04E+03	101%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T03-C	1	1.85E+00	U1/2		1.85E+00	2.7E+02	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T04-C	1	1.85E+00	U1/2		1.85E+00	1.1E+03	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T05-C	1	6.94E+00	E		6.94E+00	1.5E+02	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T06-C	1	1.23E+01			1.23E+01	1.0E+02	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T07-C	1	5.81E+01			5.81E+01	2.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T08-C	1	6.75E+01			6.75E+01	1.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T09-C	1	5.48E+01			5.48E+01	1.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-B01-A	1	1.85E+00	U1/2		1.85E+00	5.5E+02	3.7E+00	1.2E+01					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-B02-A	1	1.85E+00	U1/2		1.85E+00	1.0E+02	3.7E+00	1.2E+01					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-B03-A	1	1.85E+00	U1/2		1.85E+00	4.3E+02	3.7E+00	1.2E+01					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	CFS-LRef-1313-T01-A	1	2.64E+04			2.64E+04	3.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T02-A	1	1.93E+04			1.93E+04	2.7E+00	1.6E+00	5.1E+00	1000	100	2.02E+04	92%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T03-A	1	1.19E+04			1.19E+04	1.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T04-A	1	9.58E+03			9.58E+03	9.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T05-A	1	2.51E+05			2.51E+05	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T06-A	1	2.78E+05			2.78E+05	7.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T07-A	1	5.59E+05			5.59E+05	4.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T08-A	1	2.54E+06			2.54E+06	1.4E+00	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T09-A	1	2.56E+06			2.56E+06	2.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T01-B	1	2.55E+04			2.55E+04	1.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T02-B	1	1.88E+04			1.88E+04	1.3E+00	1.6E+00	5.1E+00	1000	100	1.97E+04	89%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T03-B	1	1.24E+04			1.24E+04	1.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T04-B	1	1.01E+04			1.01E+04	3.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T05-B	1	2.61E+05			2.61E+05	4.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T06-B	1	3.38E+05			3.38E+05	9.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T07-B	1	5.65E+05			5.65E+05	2.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T08-B	1	2.48E+06			2.48E+06	6.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T09-B	1	2.54E+06			2.54E+06	1.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T01-C	1	2.61E+04			2.61E+04	8.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T02-C	1	1.88E+04			1.88E+04	9.7E-01	1.6E+00	5.1E+00	1000	100	1.98E+04	99%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T03-C	1	1.23E+04			1.23E+04	3.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T04-C	1	9.76E+03			9.76E+03	9.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T05-C	1	2.51E+05			2.51E+05	9.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T06-C	1	3.38E+05			3.38E+05	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T07-C	1	5.62E+05			5.62E+05	3.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T08-C	1	2.58E+06			2.58E+06	1.6E+00	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T09-C	1	2.67E+06			2.67E+06	1.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-B01-A	1	2.78E+01			2.78E+01	1.6E+01	1.6E+00	5.1E+00					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-B02-A	1	2.77E+00	E		2.77E+00	7.4E+01	1.6E+00	5.1E+00					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-B03-A	1	2.51E+06			2.51E+06	9.8E-01	1.6E+00	5.1E+00					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	CFS-LRef-1313-T01-A	1	4.92E+02			4.92E+02	2.8E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T02-A	1	2.57E+02			2.57E+02	7.6E+00	1.5E+01	4.8E+01	10	100	1.24E+03	98%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T03-A	1	1.22E+02			1.22E+02	7.8E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T04-A	1	7.49E+01			7.49E+01	1.4E+01	1.5E+01	4.8E+01				---	VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T05-A	1	9.69E+01			9.69E+01	1.6E+01	1.5E+01	4.8E+01				---	VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T06-A	1	1.15E+02			1.15E+02	1.2E+01	1.5E+01	4.8E+01				---	VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T07-A	1	5.78E+02			5.78E+02	2.2E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T08-A	1	4.12E+02			4.12E+02	3.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T09-A	1	3.07E+02			3.07E+02	2.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T01-B	1	4.93E+02			4.93E+02	1.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T02-B	1	2.40E+02			2.40E+02	6.7E+00	1.5E+01	4.8E+01	10	100	1.24E+03	100%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T03-B	1	1.21E+02			1.21E+02	1.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T04-B	1	7.10E+01			7.10E+01	1.9E+01	1.5E+01	4.8E+01				---	VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T05-B	1	1.06E+02			1.06E+02	9.8E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T06-B	1	1.47E+02			1.47E+02	7.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T07-B	1	6.21E+02			6.21E+02	7.3E-01	1.5E+01	4.8E+01				---	VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T08-B	1	5.28E+02			5.28E+02	1.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T09-B	1	3.30E+02			3.30E+02	2.8E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T01-C	1	5.58E+02			5.58E+02	1.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T02-C	1	2.40E+02			2.40E+02	1.2E+01	1.5E+01	4.8E+01	10	100	1.22E+03	98%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T03-C	1	1.02E+02			1.02E+02	9.2E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T04-C	1	8.70E+01			8.70E+01	1.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T05-C	1	1.05E+02			1.05E+02	8.0E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T06-C	1	1.51E+02			1.51E+02	6.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T07-C	1	5.90E+02			5.90E+02	1.5E-01	1.5E+01	4.8E+01				---	VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T08-C	1	4.37E+02			4.37E+02	4.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T09-C	1	3.09E+02			3.09E+02	1.2E+00	1.5E+01	4.8E+01				---	VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-B01-A	1	7.50E+00	U1/2		7.50E+00	3.0E+02	1.5E+01	4.8E+01					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-B02-A	1	7.50E+00	U1/2		7.50E+00	6.8E+01	1.5E+01	4.8E+01					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-B03-A	1	7.50E+00	U1/2		7.50E+00	1.4E+02	1.5E+01	4.8E+01					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	CFS-LRef-1313-T01-A	1	1.60E+05			1.60E+05	3.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T02-A	1	7.90E+04			7.90E+04	1.5E+00	1.1E+00	3.5E+00	1000	100	8.00E+04	91%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T03-A	1	2.54E+04			2.54E+04	9.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T04-A	1	4.25E+03			4.25E+03	7.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T05-A	1	1.02E+03			1.02E+03	1.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T06-A	1	8.00E+02			8.00E+02	2.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T07-A	1	5.63E+02			5.63E+02	4.8E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T08-A	1	3.00E+02			3.00E+02	2.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T09-A	1	2.23E+02			2.23E+02	2.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T01-B	1	1.55E+05			1.55E+05	7.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T02-B	1	7.78E+04			7.78E+04	8.3E-01	1.1E+00	3.5E+00	1000	100	7.87E+04	90%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T03-B	1	2.56E+04			2.56E+04	5.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T04-B	1	4.45E+03			4.45E+03	5.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T05-B	1	9.93E+02			9.93E+02	4.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T06-B	1	5.96E+02			5.96E+02	1.8E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T07-B	1	5.27E+02			5.27E+02	1.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T08-B	1	2.07E+02			2.07E+02	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T09-B	1	2.34E+02			2.34E+02	1.6E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T01-C	1	1.58E+05			1.58E+05	4.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T02-C	1	7.81E+04			7.81E+04	5.4E-02	1.1E+00	3.5E+00	1000	100	7.90E+04	88%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T03-C	1	2.57E+04			2.57E+04	1.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T04-C	1	4.15E+03			4.15E+03	6.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T05-C	1	1.04E+03			1.04E+03	8.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T06-C	1	6.01E+02			6.01E+02	4.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T07-C	1	5.36E+02			5.36E+02	8.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T08-C	1	2.64E+02			2.64E+02	5.8E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T09-C	1	2.45E+02			2.45E+02	2.5E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-B01-A	1	5.50E-01	U1/2		5.50E-01	1.7E+03	1.1E+00	3.5E+00					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-B02-A	1	2.16E+01			2.16E+01	4.0E+00	1.1E+00	3.5E+00					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-B03-A	1	1.00E+02			1.00E+02	3.2E+00	1.1E+00	3.5E+00					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	CFS-LRef-1313-T01-A	1	3.19E+04			3.19E+04	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T02-A	1	2.86E+04			2.86E+04	1.7E+00	2.5E+00	8.0E+00	1000	100	2.95E+04	90%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T03-A	1	2.19E+04			2.19E+04	3.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T04-A	1	1.99E+04			1.99E+04	7.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T05-A	1	2.00E+04			2.00E+04	2.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T06-A	1	2.07E+04			2.07E+04	5.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T07-A	1	1.94E+04			1.94E+04	1.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T08-A	1	1.92E+04			1.92E+04	2.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T09-A	1	1.99E+04			1.99E+04	4.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T01-B	1	3.37E+04			3.37E+04	5.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T02-B	1	2.78E+04			2.78E+04	8.5E-01	2.5E+00	8.0E+00	1000	100	2.87E+04	91%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T03-B	1	2.27E+04			2.27E+04	1.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T04-B	1	2.03E+04			2.03E+04	5.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T05-B	1	2.02E+04			2.02E+04	2.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T06-B	1	2.06E+04			2.06E+04	1.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T07-B	1	2.03E+04			2.03E+04	6.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T08-B	1	1.98E+04			1.98E+04	6.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T09-B	1	2.10E+04			2.10E+04	6.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T01-C	1	3.29E+04			3.29E+04	2.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T02-C	1	3.02E+04			3.02E+04	1.2E+00	2.5E+00	8.0E+00	1000	100	3.11E+04	96%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T03-C	1	2.17E+04			2.17E+04	5.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T04-C	1	2.03E+04			2.03E+04	1.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T05-C	1	2.07E+04			2.07E+04	5.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T06-C	1	2.06E+04			2.06E+04	2.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T07-C	1	2.03E+04			2.03E+04	4.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T08-C	1	1.98E+04			1.98E+04	3.0E+00	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T09-C	1	1.99E+04			1.99E+04	5.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-B01-A	1	3.21E+00	E		3.21E+00	1.3E+02	2.5E+00	8.0E+00					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-B02-A	1	1.25E+00	U1/2		1.25E+00	1.3E+01	2.5E+00	8.0E+00					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-B03-A	1	1.23E+03			1.23E+03	4.6E-01	2.5E+00	8.0E+00					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	CFS-LRef-1313-T01-A	1	1.35E+03			1.35E+03	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T02-A	1	1.35E+03			1.35E+03	1.9E+00	1.0E+00	3.2E+00	1000	100	2.22E+03	87%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T03-A	1	9.43E+02			9.43E+02	9.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T04-A	1	1.43E+03			1.43E+03	3.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T05-A	1	3.45E+03			3.45E+03	5.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T06-A	1	3.43E+03			3.43E+03	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T07-A	1	4.18E+03			4.18E+03	5.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T08-A	1	3.72E+03			3.72E+03	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T09-A	1	3.24E+03			3.24E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T01-B	1	1.34E+03			1.34E+03	2.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T02-B	1	1.34E+03			1.34E+03	9.3E-01	1.0E+00	3.2E+00	1000	100	2.21E+03	87%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T03-B	1	9.26E+02			9.26E+02	6.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T04-B	1	1.57E+03			1.57E+03	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T05-B	1	3.58E+03			3.58E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T06-B	1	3.58E+03			3.58E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T07-B	1	4.26E+03			4.26E+03	1.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T08-B	1	3.87E+03			3.87E+03	9.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T09-B	1	3.34E+03			3.34E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T01-C	1	1.35E+03			1.35E+03	4.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T02-C	1	1.28E+03			1.28E+03	9.0E-01	1.0E+00	3.2E+00	1000	100	2.21E+03	93%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T03-C	1	9.41E+02			9.41E+02	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T04-C	1	1.51E+03			1.51E+03	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T05-C	1	3.49E+03			3.49E+03	7.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T06-C	1	3.53E+03			3.53E+03	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T07-C	1	4.06E+03			4.06E+03	2.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T08-C	1	3.83E+03			3.83E+03	5.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T09-C	1	3.42E+03			3.42E+03	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	5.8E+01	1.0E+00	3.2E+00					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-B02-A	1	5.00E-01	U1/2		5.00E-01	4.5E+00	1.0E+00	3.2E+00					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-B03-A	1	5.00E-01	U1/2		5.00E-01	1.4E+01	1.0E+00	3.2E+00					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	CFS-LRef-1313-T01-A	1	7.95E+05			7.95E+05	3.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T02-A	1	7.06E+05			7.06E+05	2.1E+00	6.8E+00	2.2E+01	1000	100	7.07E+05	84%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T03-A	1	6.03E+05			6.03E+05	8.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T04-A	1	5.74E+05			5.74E+05	7.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T05-A	1	6.44E+05			6.44E+05	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T06-A	1	6.61E+05			6.61E+05	4.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T07-A	1	7.72E+05			7.72E+05	4.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T08-A	1	1.01E+06			1.01E+06	1.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T09-A	1	1.28E+06			1.28E+06	2.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T01-B	1	7.87E+05			7.87E+05	2.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T02-B	1	7.11E+05			7.11E+05	1.1E+00	6.8E+00	2.2E+01	1000	100	7.12E+05	87%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T03-B	1	6.08E+05			6.08E+05	4.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T04-B	1	5.96E+05			5.96E+05	3.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T05-B	1	6.67E+05			6.67E+05	4.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T06-B	1	6.84E+05			6.84E+05	6.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T07-B	1	7.94E+05			7.94E+05	4.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T08-B	1	9.81E+05			9.81E+05	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T09-B	1	1.32E+06			1.32E+06	8.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T01-C	1	8.04E+05			8.04E+05	4.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T02-C	1	7.16E+05			7.16E+05	1.1E+00	6.8E+00	2.2E+01	1000	100	7.17E+05	91%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T03-C	1	6.05E+05			6.05E+05	3.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T04-C	1	5.77E+05			5.77E+05	8.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T05-C	1	6.56E+05			6.56E+05	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T06-C	1	6.79E+05			6.79E+05	8.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T07-C	1	7.81E+05			7.81E+05	3.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T08-C	1	1.03E+06			1.03E+06	5.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T09-C	1	1.31E+06			1.31E+06	1.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-B01-A	1	3.40E+00	U1/2		3.40E+00	7.5E+02	6.8E+00	2.2E+01					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-B02-A	1	3.40E+00	U1/2		3.40E+00	3.0E+02	6.8E+00	2.2E+01					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-B03-A	1	7.61E+00	E		7.61E+00	1.9E+02	6.8E+00	2.2E+01					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	CFS-LRef-1313-T01-A	1	1.75E+03			1.75E+03	4.5E-01	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T02-A	1	1.04E+03			1.04E+03	1.4E+00	4.6E+00	1.5E+01	10	100	2.02E+03	99%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T03-A	1	5.95E+02			5.95E+02	2.3E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T04-A	1	3.57E+02			3.57E+02	5.1E-01	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T05-A	1	6.79E+02			6.79E+02	2.1E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T06-A	1	6.21E+02			6.21E+02	4.6E-01	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T07-A	1	3.29E+02			3.29E+02	4.8E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T08-A	1	2.07E+02			2.07E+02	7.7E-01	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T09-A	1	2.14E+02			2.14E+02	3.4E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T01-B	1	1.78E+03			1.78E+03	1.3E-01	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T02-B	1	1.04E+03			1.04E+03	2.0E+00	4.6E+00	1.5E+01	10	100	2.04E+03	101%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T03-B	1	6.07E+02			6.07E+02	2.3E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T04-B	1	3.85E+02			3.85E+02	8.9E-01	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T05-B	1	6.82E+02			6.82E+02	8.4E-01	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T06-B	1	5.73E+02			5.73E+02	2.6E-01	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T07-B	1	3.46E+02			3.46E+02	4.4E-01	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T08-B	1	2.19E+02			2.19E+02	2.9E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T09-B	1	2.32E+02			2.32E+02	2.6E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T01-C	1	1.80E+03			1.80E+03	2.0E-01	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T02-C	1	1.04E+03			1.04E+03	1.1E+00	4.6E+00	1.5E+01	10	100	1.99E+03	94%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T03-C	1	6.14E+02			6.14E+02	1.0E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T04-C	1	3.62E+02			3.62E+02	5.5E-01	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T05-C	1	7.02E+02			7.02E+02	1.9E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T06-C	1	5.57E+02			5.57E+02	1.4E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T07-C	1	3.36E+02			3.36E+02	1.2E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T08-C	1	2.29E+02			2.29E+02	3.8E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T09-C	1	2.25E+02			2.25E+02	1.7E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-B01-A	1	2.30E+00	U1/2		2.30E+00	2.1E+02	4.6E+00	1.5E+01					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-B02-A	1	2.30E+00	U1/2		2.30E+00	1.6E+02	4.6E+00	1.5E+01					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-B03-A	1	2.30E+00	U1/2		2.30E+00	2.1E+02	4.6E+00	1.5E+01					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	CFS-LRef-1313-T01-A	1	4.49E+01			4.49E+01	6.6E-01	2.0E+00	6.4E+00			---		VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T02-A	1	1.22E+01			1.22E+01	9.1E-01	2.0E+00	6.4E+00	10	100	9.94E+02	98%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T03-A	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T04-A	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00			---		VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T05-A	1	1.00E+00	U1/2		1.00E+00	9.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T06-A	1	1.00E+00	U1/2		1.00E+00	2.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T07-A	1	1.00E+00	U1/2		1.00E+00	3.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T08-A	1	1.00E+00	U1/2		1.00E+00	4.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T09-A	1	1.00E+00	U1/2		1.00E+00	6.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T01-B	1	4.46E+01			4.46E+01	4.2E-01	2.0E+00	6.4E+00			---		VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T02-B	1	1.22E+01			1.22E+01	8.7E+00	2.0E+00	6.4E+00	10	100	9.92E+02	98%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T03-B	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T04-B	1	1.00E+00	U1/2		1.00E+00	9.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T05-B	1	1.00E+00	U1/2		1.00E+00	2.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T06-B	1	1.00E+00	U1/2		1.00E+00	2.9E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T07-B	1	1.00E+00	U1/2		1.00E+00	5.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T08-B	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00			---		VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T09-B	1	1.00E+00	U1/2		1.00E+00	9.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T01-C	1	4.29E+01			4.29E+01	5.3E-01	2.0E+00	6.4E+00			---		VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T02-C	1	1.23E+01			1.23E+01	1.0E+01	2.0E+00	6.4E+00	10	100	9.88E+02	98%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T03-C	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T04-C	1	1.00E+00	U1/2		1.00E+00	4.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T05-C	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00			---		VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T06-C	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00			---		VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T07-C	1	1.00E+00	U1/2		1.00E+00	6.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T08-C	1	1.00E+00	U1/2		1.00E+00	6.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T09-C	1	1.00E+00	U1/2		1.00E+00	4.6E+01	2.0E+00	6.4E+00			---		VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-B01-A	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-B02-A	1	1.00E+00	U1/2		1.00E+00	9.1E+00	2.0E+00	6.4E+00					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-B03-A	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	CFS-LRef-1313-T01-A	1	5.68E+02			5.68E+02	1.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T02-A	1	6.56E+01			6.56E+01	3.6E+00	1.5E+00	4.8E+00	10	100	1.05E+03	99%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T03-A	1	4.64E+01			4.64E+01	1.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T04-A	1	3.70E+01			3.70E+01	3.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T05-A	1	3.60E+01			3.60E+01	4.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T06-A	1	3.60E+01			3.60E+01	2.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T07-A	1	3.52E+01			3.52E+01	4.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T08-A	1	3.57E+01			3.57E+01	4.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T09-A	1	4.20E+01			4.20E+01	3.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T01-B	1	5.64E+02			5.64E+02	7.1E-01	1.5E+00	4.8E+00				---	VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T02-B	1	6.65E+01			6.65E+01	4.9E+00	1.5E+00	4.8E+00	10	100	1.07E+03	100%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T03-B	1	4.88E+01			4.88E+01	2.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T04-B	1	3.94E+01			3.94E+01	5.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T05-B	1	3.61E+01			3.61E+01	2.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T06-B	1	3.61E+01			3.61E+01	1.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T07-B	1	3.63E+01			3.63E+01	1.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T08-B	1	3.52E+01			3.52E+01	4.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T09-B	1	4.15E+01			4.15E+01	5.9E+00	1.5E+00	4.8E+00				---	VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T01-C	1	6.15E+02			6.15E+02	3.6E-01	1.5E+00	4.8E+00				---	VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T02-C	1	6.83E+01			6.83E+01	3.0E+00	1.5E+00	4.8E+00	10	100	1.04E+03	98%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T03-C	1	4.83E+01			4.83E+01	1.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T04-C	1	3.84E+01			3.84E+01	4.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T05-C	1	3.72E+01			3.72E+01	7.1E-01	1.5E+00	4.8E+00				---	VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T06-C	1	3.63E+01			3.63E+01	2.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T07-C	1	3.62E+01			3.62E+01	6.8E-01	1.5E+00	4.8E+00				---	VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T08-C	1	3.78E+01			3.78E+01	4.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T09-C	1	3.84E+01			3.84E+01	1.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-B01-A	1	7.50E-01	U1/2		7.50E-01	2.6E+02	1.5E+00	4.8E+00					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-B02-A	1	7.50E-01	U1/2		7.50E-01	3.3E+01	1.5E+00	4.8E+00					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-B03-A	1	7.50E-01	U1/2		7.50E-01	1.6E+02	1.5E+00	4.8E+00					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	CFS-LRef-1313-T01-A	1	1.68E+05			1.68E+05	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:07 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T02-A	1	1.79E+05			1.79E+05	2.4E+00	1.0E+00	3.2E+00	10	100	1.79E+05	92%	VU ICP-OES	2/3/11 3:09 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T03-A	1	1.56E+05			1.56E+05	7.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:10 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T04-A	1	2.69E+04			2.69E+04	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:12 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T05-A	1	1.09E+02			1.09E+02	1.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:13 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T06-A	1	3.81E+01			3.81E+01	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:15 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T07-A	1	2.93E+01			2.93E+01	2.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:17 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T08-A	1	2.41E+03			2.41E+03	1.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:18 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T09-A	1	4.70E+03			4.70E+03	1.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T01-B	1	1.68E+05			1.68E+05	1.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:27 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T02-B	1	1.84E+05			1.84E+05	1.3E+00	1.0E+00	3.2E+00	10	100	1.85E+05	87%	VU ICP-OES	2/3/11 3:28 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T03-B	1	1.55E+05			1.55E+05	9.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:30 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T04-B	1	2.61E+04			2.61E+04	7.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:32 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T05-B	1	7.74E+01			7.74E+01	6.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:33 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T06-B	1	2.97E+01			2.97E+01	3.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:32 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T07-B	1	2.91E+01			2.91E+01	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:37 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T08-B	1	2.66E+03			2.66E+03	7.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:34 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T09-B	1	4.75E+03			4.75E+03	2.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:35 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T01-C	1	1.66E+05			1.66E+05	1.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:41 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T02-C	1	1.78E+05			1.78E+05	1.4E+00	1.0E+00	3.2E+00	10	100	1.79E+05	90%	VU ICP-OES	2/3/11 3:43 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T03-C	1	1.58E+05			1.58E+05	5.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:37 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T04-C	1	2.30E+04			2.30E+04	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:46 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T05-C	1	8.91E+01			8.91E+01	8.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:48 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T06-C	1	3.52E+01			3.52E+01	2.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:50 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T07-C	1	2.59E+01			2.59E+01	2.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:51 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T08-C	1	2.66E+03			2.66E+03	5.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:53 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T09-C	1	4.82E+03			4.82E+03	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 3:55 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-B01-A	1	5.00E-01	U1/2		5.00E-01	1.6E+01	1.0E+00	3.2E+00					VU ICP-OES	2/3/11 3:02 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-B02-A	1	1.16E+01			1.16E+01	2.0E+00	1.0E+00	3.2E+00					VU ICP-OES	2/3/11 3:04 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-B03-A	1	3.99E+00			3.99E+00	1.2E+01	1.0E+00	3.2E+00					VU ICP-OES	2/3/11 3:05 PM	EPA Interlab LRef 1313-1316 CFS

QA-QC Spreadsheet 1313:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	CFS-LRef-1313-T01-D	1	9.59E+04			9.59E+04	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T02-D	1	3.96E+04			3.96E+04	4.7E-01	1.0E+00	3.2E+00	1000	100	4.05E+04	95%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T03-D	1	3.30E+03			3.30E+03	3.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T04-D	1	3.69E+01			3.69E+01	4.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T05-D	1	4.67E+01			4.67E+01	1.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T06-D	1	5.66E+01			5.66E+01	3.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T07-D	1	1.14E+02			1.14E+02	4.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T08-D	1	9.88E+01			9.88E+01	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T09-D	1	8.96E+01			8.96E+01	3.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T01-E	1	9.98E+04			9.98E+04	4.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T02-E	1	3.87E+04			3.87E+04	1.0E+00	1.0E+00	3.2E+00	1000	100	3.96E+04	91%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T03-E	1	3.37E+03			3.37E+03	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T04-E	1	3.79E+01			3.79E+01	7.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T05-E	1	4.45E+01			4.45E+01	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T06-E	1	5.35E+01			5.35E+01	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T07-E	1	1.29E+02			1.29E+02	3.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T08-E	1	1.12E+02			1.12E+02	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T09-E	1	9.23E+01			9.23E+01	9.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T01-F	1	9.77E+04			9.77E+04	1.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T02-F	1	4.38E+04			4.38E+04	2.6E-01	1.0E+00	3.2E+00	1000	100	4.47E+04	93%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T03-F	1	3.33E+03			3.33E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T04-F	1	3.51E+01			3.51E+01	4.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T05-F	1	5.55E+01			5.55E+01	5.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T06-F	1	5.76E+01			5.76E+01	3.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T07-F	1	1.11E+02			1.11E+02	9.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T08-F	1	1.02E+02			1.02E+02	4.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1313-T09-F	1	8.60E+01			8.60E+01	2.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	CFS-LRef-1313-T01-D	1	1.46E+03			1.46E+03	1.1E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T02-D	1	1.11E+03			1.11E+03	6.5E+00	7.5E+00	2.4E+01	10	100	2.03E+03	92%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T03-D	1	8.76E+01			8.76E+01	1.3E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T04-D	1	3.60E+01			3.60E+01	1.9E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T05-D	1	2.83E+01			2.83E+01	9.6E+00	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T06-D	1	3.32E+01			3.32E+01	7.9E+00	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T07-D	1	2.76E+01			2.76E+01	1.3E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T08-D	1	8.76E+00	E		8.76E+00	3.6E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T09-D	1	3.75E+00	U1/2		3.75E+00	3.5E+02	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T01-E	1	1.28E+03			1.28E+03	8.5E+00	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T02-E	1	1.08E+03			1.08E+03	6.6E+00	7.5E+00	2.4E+01	10	100	1.98E+03	90%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T03-E	1	9.10E+01			9.10E+01	7.3E+00	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T04-E	1	4.35E+01			4.35E+01	4.4E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T05-E	1	3.29E+01			3.29E+01	1.4E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T06-E	1	3.85E+01			3.85E+01	2.7E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T07-E	1	3.13E+01			3.13E+01	7.6E+00	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T08-E	1	8.89E+00	E		8.89E+00	5.3E+00	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T09-E	1	3.75E+00	U1/2		3.75E+00	2.8E+02	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T01-F	1	1.06E+03			1.06E+03	6.1E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T02-F	1	1.22E+03			1.22E+03	3.7E+00	7.5E+00	2.4E+01	10	100	2.05E+03	83%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T03-F	1	8.61E+01			8.61E+01	2.0E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T04-F	1	2.97E+01			2.97E+01	1.7E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T05-F	1	3.27E+01			3.27E+01	4.9E+00	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T06-F	1	3.50E+01			3.50E+01	6.3E+00	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T07-F	1	3.22E+01			3.22E+01	2.1E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T08-F	1	8.59E+00	E		8.59E+00	9.1E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1313-T09-F	1	3.75E+00	U1/2		3.75E+00	1.8E+01	7.5E+00	2.4E+01			---		VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	CFS-LRef-1313-T01-D	1	8.79E+04			8.79E+04	6.9E-01	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T02-D	1	1.43E+03			1.43E+03	1.2E+00	1.1E+01	3.5E+01	10	100	2.33E+03	90%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T03-D	1	1.29E+02			1.29E+02	8.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T04-D	1	2.33E+01	E		2.33E+01	2.1E+01	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T05-D	1	3.34E+01	E		3.34E+01	8.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T06-D	1	3.85E+01			3.85E+01	1.7E+01	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T07-D	1	1.12E+02			1.12E+02	1.1E+01	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T08-D	1	2.36E+02			2.36E+02	4.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T09-D	1	2.11E+02			2.11E+02	1.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T01-E	1	7.16E+04			7.16E+04	1.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T02-E	1	1.18E+03			1.18E+03	5.4E-01	1.1E+01	3.5E+01	10	100	2.12E+03	93%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T03-E	1	1.11E+02			1.11E+02	9.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T04-E	1	2.71E+01	E		2.71E+01	2.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T05-E	1	2.52E+01	E		2.52E+01	3.4E+01	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T06-E	1	4.35E+01			4.35E+01	3.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T07-E	1	1.01E+02			1.01E+02	4.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T08-E	1	2.42E+02			2.42E+02	1.7E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T09-E	1	1.98E+02			1.98E+02	3.7E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T01-F	1	7.67E+04			7.67E+04	8.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T02-F	1	1.45E+03			1.45E+03	1.5E+00	1.1E+01	3.5E+01	10	100	2.32E+03	87%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T03-F	1	1.19E+02			1.19E+02	9.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T04-F	1	2.95E+01	E		2.95E+01	9.7E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T05-F	1	3.22E+01	E		3.22E+01	3.9E+01	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T06-F	1	3.79E+01			3.79E+01	2.6E+01	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T07-F	1	9.11E+01			9.11E+01	8.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T08-F	1	1.88E+02			1.88E+02	6.7E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1313-T09-F	1	1.98E+02			1.98E+02	4.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	CFS-LRef-1313-T01-D	1	7.30E+02			7.30E+02	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T02-D	1	6.71E+02			6.71E+02	1.8E-01	1.0E+00	3.2E+00	1000	100	1.63E+03	96%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T03-D	1	3.13E+02			3.13E+02	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T04-D	1	1.69E+02			1.69E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T05-D	1	1.28E+02			1.28E+02	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T06-D	1	1.19E+02			1.19E+02	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T07-D	1	1.62E+02			1.62E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T08-D	1	8.83E+01			8.83E+01	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T09-D	1	6.62E+01			6.62E+01	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T01-E	1	7.84E+02			7.84E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T02-E	1	6.85E+02			6.85E+02	1.2E+00	1.0E+00	3.2E+00	1000	100	1.57E+03	89%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T03-E	1	3.23E+02			3.23E+02	2.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T04-E	1	1.62E+02			1.62E+02	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T05-E	1	1.22E+02			1.22E+02	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T06-E	1	1.20E+02			1.20E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T07-E	1	1.63E+02			1.63E+02	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T08-E	1	9.47E+01			9.47E+01	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T09-E	1	6.96E+01			6.96E+01	9.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T01-F	1	7.54E+02			7.54E+02	9.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T02-F	1	6.74E+02			6.74E+02	6.6E-01	1.0E+00	3.2E+00	1000	100	1.62E+03	95%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T03-F	1	3.14E+02			3.14E+02	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T04-F	1	1.58E+02			1.58E+02	9.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T05-F	1	1.23E+02			1.23E+02	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T06-F	1	1.18E+02			1.18E+02	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T07-F	1	1.56E+02			1.56E+02	2.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T08-F	1	8.48E+01			8.48E+01	2.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1313-T09-F	1	6.29E+01			6.29E+01	3.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	CFS-LRef-1313-T01-D	1	4.82E+00			4.82E+00	5.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T02-D	1	3.27E+01			3.27E+01	1.8E+00	1.0E+00	3.2E+00	10	100	1.14E+03	111%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T03-D	1	2.37E+01			2.37E+01	3.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T04-D	1	1.00E+02			1.00E+02	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T05-D	1	7.59E+01			7.59E+01	7.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T06-D	1	8.37E+01			8.37E+01	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T07-D	1	1.65E+02			1.65E+02	2.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T08-D	1	4.13E+00			4.13E+00	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T09-D	1	1.40E+00	E		1.40E+00	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T01-E	1	6.04E+00			6.04E+00	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T02-E	1	3.40E+01			3.40E+01	2.4E+00	1.0E+00	3.2E+00	10	100	1.04E+03	101%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T03-E	1	2.77E+01			2.77E+01	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T04-E	1	9.45E+01			9.45E+01	9.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T05-E	1	7.55E+01			7.55E+01	8.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T06-E	1	8.52E+01			8.52E+01	3.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T07-E	1	1.66E+02			1.66E+02	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T08-E	1	6.13E+00			6.13E+00	2.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T09-E	1	1.22E+00	E		1.22E+00	1.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T01-F	1	5.58E+00			5.58E+00	1.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T02-F	1	3.41E+01			3.41E+01	3.4E-01	1.0E+00	3.2E+00	10	100	1.14E+03	110%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T03-F	1	2.80E+01			2.80E+01	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T04-F	1	9.20E+01			9.20E+01	8.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T05-F	1	7.46E+01			7.46E+01	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T06-F	1	8.23E+01			8.23E+01	6.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T07-F	1	1.60E+02			1.60E+02	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T08-F	1	6.47E+00			6.47E+00	2.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1313-T09-F	1	1.30E+00	E		1.30E+00	6.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	CFS-LRef-1313-T01-D	1	9.50E-01	U1/2		9.50E-01	5.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T02-D	1	6.80E+00			6.80E+00	7.2E+00	1.9E+00	6.0E+00	10	100	1.08E+03	108%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T03-D	1	2.61E+00	E		2.61E+00	4.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T04-D	1	9.50E-01	U1/2		9.50E-01	8.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T05-D	1	9.50E-01	U1/2		9.50E-01	4.7E+02	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T06-D	1	9.50E-01	U1/2		9.50E-01	8.7E+02	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T07-D	1	9.50E-01	U1/2		9.50E-01	2.7E+02	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T08-D	1	9.50E-01	U1/2		9.50E-01	2.7E+02	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T09-D	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T01-E	1	9.50E-01	U1/2		9.50E-01	2.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T02-E	1	7.89E+00			7.89E+00	1.6E+01	1.9E+00	6.0E+00	10	100	9.88E+02	98%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T03-E	1	2.59E+00	E		2.59E+00	5.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T04-E	1	9.50E-01	U1/2		9.50E-01	7.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T05-E	1	9.50E-01	U1/2		9.50E-01	4.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T06-E	1	9.50E-01	U1/2		9.50E-01	5.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T07-E	1	9.50E-01	U1/2		9.50E-01	4.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T08-E	1	9.50E-01	U1/2		9.50E-01	3.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T09-E	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T01-F	1	9.50E-01	U1/2		9.50E-01	1.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T02-F	1	7.73E+00			7.73E+00	1.1E+01	1.9E+00	6.0E+00	10	100	1.06E+03	105%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T03-F	1	2.66E+00	E		2.66E+00	3.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T04-F	1	9.50E-01	U1/2		9.50E-01	1.3E+04	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T05-F	1	9.50E-01	U1/2		9.50E-01	9.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T06-F	1	9.50E-01	U1/2		9.50E-01	1.2E+03	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T07-F	1	9.50E-01	U1/2		9.50E-01	2.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T08-F	1	9.50E-01	U1/2		9.50E-01	4.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1313-T09-F	1	9.50E-01	U1/2		9.50E-01	5.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	CFS-LRef-1313-T01-D	1	4.93E+04			4.93E+04	1.5E+00	2.2E+00	7.0E+00			---		VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T02-D	1	5.14E+04			5.14E+04	7.3E-01	2.2E+00	7.0E+00	10	100	5.23E+04	92%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T03-D	1	2.35E+04			2.35E+04	1.2E+00	2.2E+00	7.0E+00			---		VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T04-D	1	5.22E+03			5.22E+03	1.4E+00	2.2E+00	7.0E+00			---		VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T05-D	1	1.14E+02			1.14E+02	5.4E-01	2.2E+00	7.0E+00			---		VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T06-D	1	1.73E+01			1.73E+01	3.3E+00	2.2E+00	7.0E+00			---		VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T07-D	1	1.10E+00	U1/2		1.10E+00	4.1E+01	2.2E+00	7.0E+00			---		VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T08-D	1	1.10E+00	U1/2		1.10E+00	2.7E+01	2.2E+00	7.0E+00			---		VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T09-D	1	6.63E+00	E		6.63E+00	5.9E+00	2.2E+00	7.0E+00			---		VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T01-E	1	5.13E+04			5.13E+04	3.7E-01	2.2E+00	7.0E+00			---		VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T02-E	1	5.27E+04			5.27E+04	1.4E+00	2.2E+00	7.0E+00	10	100	5.36E+04	95%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T03-E	1	2.37E+04			2.37E+04	3.4E-01	2.2E+00	7.0E+00			---		VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T04-E	1	5.11E+03			5.11E+03	7.0E-01	2.2E+00	7.0E+00			---		VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T05-E	1	9.98E+01			9.98E+01	4.7E-01	2.2E+00	7.0E+00			---		VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T06-E	1	1.58E+01			1.58E+01	4.3E-01	2.2E+00	7.0E+00			---		VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T07-E	1	1.10E+00	U1/2		1.10E+00	1.4E+01	2.2E+00	7.0E+00			---		VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T08-E	1	1.10E+00	U1/2		1.10E+00	7.4E-01	2.2E+00	7.0E+00			---		VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T09-E	1	5.98E+00	E		5.98E+00	6.8E+00	2.2E+00	7.0E+00			---		VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T01-F	1	4.70E+04			4.70E+04	1.9E+01	2.2E+00	7.0E+00			---		VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T02-F	1	5.10E+04			5.10E+04	7.0E-01	2.2E+00	7.0E+00	10	100	5.20E+04	97%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T03-F	1	2.28E+04			2.28E+04	1.5E+00	2.2E+00	7.0E+00			---		VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T04-F	1	4.97E+03			4.97E+03	4.4E-01	2.2E+00	7.0E+00			---		VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T05-F	1	1.03E+02			1.03E+02	1.2E+00	2.2E+00	7.0E+00			---		VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T06-F	1	1.82E+01			1.82E+01	1.2E+00	2.2E+00	7.0E+00			---		VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T07-F	1	1.10E+00	U1/2		1.10E+00	5.4E+01	2.2E+00	7.0E+00			---		VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T08-F	1	1.10E+00	U1/2		1.10E+00	3.0E+01	2.2E+00	7.0E+00			---		VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1313-T09-F	1	6.61E+00	E		6.61E+00	1.7E+00	2.2E+00	7.0E+00			---		VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	CFS-LRef-1313-T01-D	1	1.59E+06			1.59E+06	1.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T02-D	1	1.39E+06			1.39E+06	6.8E-01	2.6E+00	8.3E+00	1000	100	1.39E+06	87%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T03-D	1	8.95E+05			8.95E+05	7.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T04-D	1	7.04E+05			7.04E+05	1.5E+00	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T05-D	1	6.41E+05			6.41E+05	6.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T06-D	1	6.24E+05			6.24E+05	1.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T07-D	1	5.94E+05			5.94E+05	5.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T08-D	1	5.69E+05			5.69E+05	1.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T09-D	1	6.43E+05			6.43E+05	8.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T01-E	1	1.74E+06			1.74E+06	2.6E+00	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T02-E	1	1.37E+06			1.37E+06	1.4E+00	2.6E+00	8.3E+00	1000	100	1.37E+06	89%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T03-E	1	9.02E+05			9.02E+05	3.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T04-E	1	6.88E+05			6.88E+05	5.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T05-E	1	6.39E+05			6.39E+05	7.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T06-E	1	6.25E+05			6.25E+05	7.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T07-E	1	6.02E+05			6.02E+05	9.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T08-E	1	5.89E+05			5.89E+05	6.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T09-E	1	6.51E+05			6.51E+05	8.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T01-F	1	1.38E+06			1.38E+06	5.5E+01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T02-F	1	1.42E+06			1.42E+06	4.5E-01	2.6E+00	8.3E+00	1000	100	1.42E+06	92%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T03-F	1	9.05E+05			9.05E+05	9.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T04-F	1	6.77E+05			6.77E+05	9.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T05-F	1	6.36E+05			6.36E+05	6.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T06-F	1	6.11E+05			6.11E+05	5.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T07-F	1	5.89E+05			5.89E+05	4.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T08-F	1	5.81E+05			5.81E+05	7.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1313-T09-F	1	6.33E+05			6.33E+05	4.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	CFS-LRef-1313-T01-D	1	2.07E+03			2.07E+03	7.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T02-D	1	6.36E+01			6.36E+01	1.7E+00	1.2E+00	3.8E+00	10	100	1.08E+03	102%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T03-D	1	6.00E-01	U1/2		6.00E-01	2.1E+02	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T04-D	1	6.00E-01	U1/2		6.00E-01	8.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T05-D	1	6.00E-01	U1/2		6.00E-01	1.4E+02	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T06-D	1	1.51E+00	E		1.51E+00	5.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T07-D	1	7.97E+00			7.97E+00	3.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T08-D	1	6.40E+01			6.40E+01	1.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T09-D	1	1.04E+02			1.04E+02	1.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T01-E	1	2.20E+03			2.20E+03	9.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T02-E	1	5.57E+01			5.57E+01	5.2E-01	1.2E+00	3.8E+00	10	100	9.94E+02	94%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T03-E	1	6.00E-01	U1/2		6.00E-01	2.5E+02	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T04-E	1	6.00E-01	U1/2		6.00E-01	1.9E+02	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T05-E	1	6.00E-01	U1/2		6.00E-01	4.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T06-E	1	6.00E-01	U1/2		6.00E-01	4.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T07-E	1	8.30E+00			8.30E+00	8.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T08-E	1	6.31E+01			6.31E+01	2.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T09-E	1	1.13E+02			1.13E+02	1.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T01-F	1	2.03E+03			2.03E+03	1.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T02-F	1	8.26E+01			8.26E+01	4.4E-01	1.2E+00	3.8E+00	10	100	1.08E+03	100%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T03-F	1	6.00E-01	U1/2		6.00E-01	8.2E+02	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T04-F	1	6.00E-01	U1/2		6.00E-01	1.1E+03	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T05-F	1	6.00E-01	U1/2		6.00E-01	2.7E+02	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T06-F	1	6.00E-01	U1/2		6.00E-01	1.4E+02	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T07-F	1	7.08E+00			7.08E+00	1.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T08-F	1	5.28E+01			5.28E+01	3.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1313-T09-F	1	1.02E+02			1.02E+02	6.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	CFS-LRef-1313-T01-D	1	1.78E+03			1.78E+03	3.4E-01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T02-D	1	1.71E+03			1.71E+03	1.2E+00	1.8E+00	5.7E+00	10	100	2.68E+03	97%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T03-D	1	5.86E+02			5.86E+02	7.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T04-D	1	1.14E+02			1.14E+02	9.3E-01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T05-D	1	9.00E-01	U1/2		9.00E-01	3.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T06-D	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T07-D	1	9.00E-01	U1/2		9.00E-01	8.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T08-D	1	9.00E-01	U1/2		9.00E-01	2.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T09-D	1	9.00E-01	U1/2		9.00E-01	2.9E+02	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T01-E	1	1.79E+03			1.79E+03	3.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T02-E	1	1.75E+03			1.75E+03	2.2E+00	1.8E+00	5.7E+00	10	100	2.74E+03	99%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T03-E	1	5.89E+02			5.89E+02	1.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T04-E	1	1.14E+02			1.14E+02	1.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T05-E	1	2.58E+00	E		2.58E+00	3.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T06-E	1	9.00E-01	U1/2		9.00E-01	1.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T07-E	1	9.00E-01	U1/2		9.00E-01	1.9E+02	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T08-E	1	9.00E-01	U1/2		9.00E-01	2.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T09-E	1	9.00E-01	U1/2		9.00E-01	2.6E+02	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T01-F	1	1.82E+03			1.82E+03	1.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T02-F	1	1.74E+03			1.74E+03	9.5E-01	1.8E+00	5.7E+00	10	100	2.74E+03	101%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T03-F	1	5.83E+02			5.83E+02	9.4E-01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T04-F	1	1.11E+02			1.11E+02	1.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T05-F	1	9.00E-01	U1/2		9.00E-01	8.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T06-F	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T07-F	1	9.00E-01	U1/2		9.00E-01	3.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T08-F	1	9.00E-01	U1/2		9.00E-01	1.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1313-T09-F	1	9.00E-01	U1/2		9.00E-01	7.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	CFS-LRef-1313-T01-D	1	1.12E+06			1.12E+06	1.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T02-D	1	9.75E+05			9.75E+05	1.2E+00	3.7E+00	1.2E+01	10	100	9.75E+05	87%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T03-D	1	1.75E+05			1.75E+05	5.2E-01	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T04-D	1	9.64E+02			9.64E+02	1.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T05-D	1	6.54E+01			6.54E+01	2.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T06-D	1	6.90E+01			6.90E+01	3.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T07-D	1	1.64E+02			1.64E+02	1.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T08-D	1	7.67E+02			7.67E+02	8.8E-01	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T09-D	1	3.41E+03			3.41E+03	8.8E-01	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T01-E	1	1.14E+06			1.14E+06	2.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T02-E	1	9.79E+05			9.79E+05	1.3E+00	3.7E+00	1.2E+01	10	100	9.80E+05	89%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T03-E	1	1.75E+05			1.75E+05	8.8E-01	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T04-E	1	9.89E+02			9.89E+02	1.3E-01	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T05-E	1	6.65E+01			6.65E+01	1.8E-01	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T06-E	1	6.81E+01			6.81E+01	1.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T07-E	1	1.95E+02			1.95E+02	1.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T08-E	1	7.78E+02			7.78E+02	1.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T09-E	1	3.31E+03			3.31E+03	1.3E-01	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T01-F	1	1.13E+06			1.13E+06	1.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T02-F	1	1.01E+06			1.01E+06	6.2E-01	3.7E+00	1.2E+01	10	100	1.01E+06	90%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T03-F	1	1.67E+05			1.67E+05	1.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T04-F	1	9.70E+02			9.70E+02	9.9E-01	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T05-F	1	6.48E+01			6.48E+01	1.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T06-F	1	7.10E+01			7.10E+01	2.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T07-F	1	1.60E+02			1.60E+02	7.6E-01	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T08-F	1	7.32E+02			7.32E+02	1.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1313-T09-F	1	3.30E+03			3.30E+03	8.7E-01	3.7E+00	1.2E+01				---	VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	CFS-LRef-1313-T01-D	1	2.68E+05			2.68E+05	1.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T02-D	1	4.71E+04			4.71E+04	5.3E-01	2.0E+00	6.4E+00	1000	100	4.80E+04	90%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T03-D	1	1.00E+00	U1/2		1.00E+00	2.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T04-D	1	1.00E+00	U1/2		1.00E+00	3.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T05-D	1	1.00E+00	U1/2		1.00E+00	6.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T06-D	1	1.00E+00	U1/2		1.00E+00	6.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T07-D	1	1.00E+00	U1/2		1.00E+00	4.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T08-D	1	1.00E+00	U1/2		1.00E+00	8.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T09-D	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T01-E	1	2.54E+05			2.54E+05	4.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T02-E	1	3.98E+04			3.98E+04	6.6E-01	2.0E+00	6.4E+00	1000	100	4.08E+04	92%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T03-E	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T04-E	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T05-E	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T06-E	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T07-E	1	1.00E+00	U1/2		1.00E+00	3.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T08-E	1	1.00E+00	U1/2		1.00E+00	1.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T09-E	1	1.00E+00	U1/2		1.00E+00	8.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T01-F	1	2.19E+05			2.19E+05	6.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T02-F	1	5.33E+04			5.33E+04	1.8E-01	2.0E+00	6.4E+00	1000	100	5.43E+04	96%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T03-F	1	1.00E+00	U1/2		1.00E+00	5.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T04-F	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T05-F	1	1.00E+00	U1/2		1.00E+00	4.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T06-F	1	1.00E+00	U1/2		1.00E+00	7.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T07-F	1	1.00E+00	U1/2		1.00E+00	5.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T08-F	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1313-T09-F	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	CFS-LRef-1313-T01-D	1	8.47E+03			8.47E+03	7.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T02-D	1	6.62E+03			6.62E+03	2.2E-01	6.8E+00	2.2E+01	10	100	7.61E+03	99%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T03-D	1	7.05E+03			7.05E+03	9.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T04-D	1	1.12E+03			1.12E+03	1.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T05-D	1	1.47E+02			1.47E+02	1.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T06-D	1	1.14E+02			1.14E+02	1.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T07-D	1	7.08E+02			7.08E+02	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T08-D	1	1.04E+04			1.04E+04	3.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T09-D	1	7.87E+03			7.87E+03	1.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T01-E	1	8.88E+03			8.88E+03	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T02-E	1	6.38E+03			6.38E+03	4.9E-01	6.8E+00	2.2E+01	10	100	7.38E+03	100%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T03-E	1	6.53E+03			6.53E+03	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T04-E	1	1.13E+03			1.13E+03	8.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T05-E	1	1.40E+02			1.40E+02	7.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T06-E	1	1.29E+02			1.29E+02	4.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T07-E	1	6.83E+02			6.83E+02	6.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T08-E	1	1.02E+04			1.02E+04	1.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T09-E	1	7.54E+03			7.54E+03	8.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T01-F	1	8.53E+03			8.53E+03	1.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T02-F	1	6.56E+03			6.56E+03	3.0E-01	6.8E+00	2.2E+01	10	100	7.47E+03	90%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T03-F	1	6.06E+03			6.06E+03	4.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T04-F	1	1.06E+03			1.06E+03	4.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T05-F	1	1.45E+02			1.45E+02	3.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T06-F	1	1.27E+02			1.27E+02	4.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T07-F	1	7.01E+02			7.01E+02	6.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T08-F	1	1.09E+04			1.09E+04	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1313-T09-F	1	7.52E+03			7.52E+03	7.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	CFS-LRef-1313-T01-D	1	2.31E+01			2.31E+01	1.8E+01	1.9E+00	6.0E+00			---		VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T02-D	1	1.10E+01			1.10E+01	7.7E+00	1.9E+00	6.0E+00	10	100	8.82E+02	87%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T03-D	1	1.19E+01			1.19E+01	1.5E+01	1.9E+00	6.0E+00			---		VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T04-D	1	1.04E+01			1.04E+01	1.8E+00	1.9E+00	6.0E+00			---		VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T05-D	1	1.15E+01			1.15E+01	1.7E+00	1.9E+00	6.0E+00			---		VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T06-D	1	1.23E+01			1.23E+01	3.1E+00	1.9E+00	6.0E+00			---		VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T07-D	1	1.26E+01			1.26E+01	4.2E+00	1.9E+00	6.0E+00			---		VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T08-D	1	1.22E+01			1.22E+01	4.8E+00	1.9E+00	6.0E+00			---		VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T09-D	1	1.33E+01			1.33E+01	6.9E+00	1.9E+00	6.0E+00			---		VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T01-E	1	3.67E+01			3.67E+01	2.5E+00	1.9E+00	6.0E+00			---		VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T02-E	1	1.35E+01			1.35E+01	2.4E+01	1.9E+00	6.0E+00	10	100	8.85E+02	87%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T03-E	1	1.25E+01			1.25E+01	5.8E+00	1.9E+00	6.0E+00			---		VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T04-E	1	1.06E+01			1.06E+01	1.2E+01	1.9E+00	6.0E+00			---		VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T05-E	1	1.22E+01			1.22E+01	2.2E+00	1.9E+00	6.0E+00			---		VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T06-E	1	1.22E+01			1.22E+01	7.5E+00	1.9E+00	6.0E+00			---		VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T07-E	1	1.28E+01			1.28E+01	5.1E+00	1.9E+00	6.0E+00			---		VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T08-E	1	1.33E+01			1.33E+01	4.6E+00	1.9E+00	6.0E+00			---		VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T09-E	1	1.29E+01			1.29E+01	1.6E-01	1.9E+00	6.0E+00			---		VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T01-F	1	3.37E+01			3.37E+01	1.2E+01	1.9E+00	6.0E+00			---		VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T02-F	1	1.54E+01			1.54E+01	1.2E+01	1.9E+00	6.0E+00	10	100	8.77E+02	86%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T03-F	1	1.05E+01			1.05E+01	1.1E+01	1.9E+00	6.0E+00			---		VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T04-F	1	1.04E+01			1.04E+01	6.1E+00	1.9E+00	6.0E+00			---		VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T05-F	1	1.12E+01			1.12E+01	5.5E+00	1.9E+00	6.0E+00			---		VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T06-F	1	1.15E+01			1.15E+01	5.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T07-F	1	1.16E+01			1.16E+01	3.7E+00	1.9E+00	6.0E+00			---		VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T08-F	1	1.25E+01			1.25E+01	3.2E+00	1.9E+00	6.0E+00			---		VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1313-T09-F	1	1.31E+01			1.31E+01	2.1E+00	1.9E+00	6.0E+00			---		VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	CFS-LRef-1313-T01-D	1	3.64E+04			3.64E+04	6.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T02-D	1	2.48E+04			2.48E+04	2.5E-01	2.0E+00	6.4E+00	10	100	2.58E+04	96%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T03-D	1	6.63E+03			6.63E+03	9.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T04-D	1	1.90E+03			1.90E+03	8.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T05-D	1	3.16E+01			3.16E+01	1.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T06-D	1	1.00E+00	U1/2		1.00E+00	9.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T07-D	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T08-D	1	1.00E+00	U1/2		1.00E+00	3.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T09-D	1	1.00E+00	U1/2		1.00E+00	2.9E+02	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T01-E	1	3.67E+04			3.67E+04	3.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T02-E	1	2.56E+04			2.56E+04	7.2E-01	2.0E+00	6.4E+00	10	100	2.65E+04	93%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T03-E	1	6.73E+03			6.73E+03	4.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T04-E	1	1.85E+03			1.85E+03	7.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T05-E	1	2.90E+01			2.90E+01	7.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T06-E	1	1.00E+00	U1/2		1.00E+00	7.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T07-E	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T08-E	1	1.00E+00	U1/2		1.00E+00	5.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T09-E	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T01-F	1	2.90E+04			2.90E+04	6.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T02-F	1	2.58E+04			2.58E+04	3.2E-01	2.0E+00	6.4E+00	10	100	2.69E+04	104%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T03-F	1	6.72E+03			6.72E+03	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T04-F	1	1.79E+03			1.79E+03	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T05-F	1	3.22E+01			3.22E+01	1.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T06-F	1	4.78E+00	E		4.78E+00	2.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T07-F	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T08-F	1	1.00E+00	U1/2		1.00E+00	4.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1313-T09-F	1	1.00E+00	U1/2		1.00E+00	8.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	CFS-LRef-1313-T01-D	1	2.15E+05			2.15E+05	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T02-D	1	1.39E+05			1.39E+05	5.5E-01	1.0E+00	3.2E+00	1000	100	1.40E+05	90%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T03-D	1	7.39E+04			7.39E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T04-D	1	6.68E+04			6.68E+04	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T05-D	1	5.79E+04			5.79E+04	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T06-D	1	2.95E+04			2.95E+04	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T07-D	1	6.76E+02			6.76E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T08-D	1	3.54E+01			3.54E+01	6.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T09-D	1	2.21E+01			2.21E+01	6.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T01-E	1	2.53E+05			2.53E+05	2.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T02-E	1	1.42E+05			1.42E+05	1.0E+00	1.0E+00	3.2E+00	1000	100	1.43E+05	89%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T03-E	1	7.83E+04			7.83E+04	4.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T04-E	1	6.50E+04			6.50E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T05-E	1	5.31E+04			5.31E+04	8.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T06-E	1	3.04E+04			3.04E+04	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T07-E	1	6.55E+02			6.55E+02	5.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T08-E	1	3.31E+01			3.31E+01	2.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T09-E	1	1.52E+01			1.52E+01	7.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T01-F	1	1.93E+05			1.93E+05	3.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T02-F	1	1.47E+05			1.47E+05	2.4E-01	1.0E+00	3.2E+00	1000	100	1.47E+05	85%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T03-F	1	7.61E+04			7.61E+04	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T04-F	1	6.20E+04			6.20E+04	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T05-F	1	5.76E+04			5.76E+04	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T06-F	1	2.91E+04			2.91E+04	5.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T07-F	1	6.89E+02			6.89E+02	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T08-F	1	3.48E+01			3.48E+01	2.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1313-T09-F	1	1.91E+01			1.91E+01	3.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	CFS-LRef-1313-T01-D	1	1.33E+02			1.33E+02	1.2E+01	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T02-D	1	1.09E+01			1.09E+01	1.0E+01	1.2E+00	3.8E+00	10	100	1.08E+03	107%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T03-D	1	9.16E+00			9.16E+00	2.1E+01	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T04-D	1	1.10E+01			1.10E+01	7.2E+00	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T05-D	1	1.25E+02			1.25E+02	7.8E-01	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T06-D	1	4.27E+02			4.27E+02	7.7E-01	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T07-D	1	1.08E+03			1.08E+03	1.2E+00	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T08-D	1	1.74E+03			1.74E+03	5.5E-01	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T09-D	1	1.57E+03			1.57E+03	8.6E-01	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T01-E	1	1.11E+02			1.11E+02	7.2E+00	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T02-E	1	1.03E+01			1.03E+01	3.2E+01	1.2E+00	3.8E+00	10	100	9.85E+02	97%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T03-E	1	7.13E+00			7.13E+00	3.1E+01	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T04-E	1	9.14E+00			9.14E+00	1.8E+01	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T05-E	1	1.35E+02			1.35E+02	1.9E+00	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T06-E	1	4.07E+02			4.07E+02	8.7E-01	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T07-E	1	1.09E+03			1.09E+03	9.2E-01	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T08-E	1	1.68E+03			1.68E+03	3.0E-01	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T09-E	1	1.47E+03			1.47E+03	2.9E-01	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T01-F	1	1.01E+02			1.01E+02	5.5E+01	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T02-F	1	1.09E+01			1.09E+01	1.8E+01	1.2E+00	3.8E+00	10	100	1.06E+03	105%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T03-F	1	6.29E+00			6.29E+00	1.2E+01	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T04-F	1	9.61E+00			9.61E+00	3.7E+00	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T05-F	1	1.25E+02			1.25E+02	1.0E+00	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T06-F	1	3.98E+02			3.98E+02	1.2E+00	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T07-F	1	1.05E+03			1.05E+03	1.4E+00	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T08-F	1	1.71E+03			1.71E+03	9.3E-01	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1313-T09-F	1	1.40E+03			1.40E+03	6.5E-01	1.2E+00	3.8E+00			---		VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	CFS-LRef-1313-T01-D	1	6.68E+03			6.68E+03	7.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T02-D	1	6.58E+03			6.58E+03	1.1E+00	1.8E+00	5.7E+00	10	100	7.54E+03	96%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T03-D	1	2.13E+03			2.13E+03	6.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T04-D	1	2.61E+02			2.61E+02	1.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T05-D	1	9.00E-01	U1/2		9.00E-01	4.2E+03	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T06-D	1	9.00E-01	U1/2		9.00E-01	1.8E+02	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T07-D	1	9.00E-01	U1/2		9.00E-01	3.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T08-D	1	9.00E-01	U1/2		9.00E-01	9.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T09-D	1	9.00E-01	U1/2		9.00E-01	3.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T01-E	1	6.78E+03			6.78E+03	2.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T02-E	1	6.69E+03			6.69E+03	1.1E+00	1.8E+00	5.7E+00	10	100	7.59E+03	90%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T03-E	1	2.16E+03			2.16E+03	1.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T04-E	1	2.58E+02			2.58E+02	5.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T05-E	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T06-E	1	9.00E-01	U1/2		9.00E-01	3.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T07-E	1	9.00E-01	U1/2		9.00E-01	1.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T08-E	1	9.00E-01	U1/2		9.00E-01	1.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T09-E	1	9.00E-01	U1/2		9.00E-01	3.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T01-F	1	5.80E+03			5.80E+03	4.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T02-F	1	6.74E+03			6.74E+03	7.6E-01	1.8E+00	5.7E+00	10	100	7.67E+03	94%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T03-F	1	2.08E+03			2.08E+03	3.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T04-F	1	2.53E+02			2.53E+02	1.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T05-F	1	2.91E+00	E		2.91E+00	6.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T06-F	1	9.00E-01	U1/2		9.00E-01	4.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T07-F	1	9.00E-01	U1/2		9.00E-01	4.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T08-F	1	9.00E-01	U1/2		9.00E-01	1.3E+03	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1313-T09-F	1	9.00E-01	U1/2		9.00E-01	5.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	CFS-LRef-1313-T01-D	1	3.49E+03			3.49E+03	2.7E-01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T02-D	1	3.77E+01			3.77E+01	6.7E+01	3.7E+00	1.2E+01	1000	100	1.07E+03	103%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T03-D	1	1.85E+00	U1/2		1.85E+00	2.4E+03	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T04-D	1	1.85E+00	U1/2		1.85E+00	3.3E+03	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T05-D	1	4.39E+00	E		4.39E+00	8.4E+02	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T06-D	1	1.78E+01			1.78E+01	2.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T07-D	1	5.12E+01			5.12E+01	4.1E+00	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T08-D	1	6.36E+01			6.36E+01	3.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T09-D	1	7.26E+01			7.26E+01	7.0E+00	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T01-E	1	2.84E+03			2.84E+03	2.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T02-E	1	2.84E+01			2.84E+01	3.9E+03	3.7E+00	1.2E+01	1000	100	9.44E+02	92%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T03-E	1	1.85E+00	U1/2		1.85E+00	2.3E+02	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T04-E	1	1.85E+00	U1/2		1.85E+00	3.3E+02	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T05-E	1	5.88E+00	E		5.88E+00	1.6E+02	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T06-E	1	2.21E+01			2.21E+01	6.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T07-E	1	5.65E+01			5.65E+01	3.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T08-E	1	4.55E+01			4.55E+01	1.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T09-E	1	6.51E+01			6.51E+01	1.9E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T01-F	1	2.90E+03			2.90E+03	1.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T02-F	1	3.22E+01			3.22E+01	2.8E+01	3.7E+00	1.2E+01	1000	100	1.02E+03	99%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T03-F	1	1.85E+00	U1/2		1.85E+00	1.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T04-F	1	1.85E+00	U1/2		1.85E+00	2.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T05-F	1	5.10E+00	E		5.10E+00	3.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T06-F	1	1.98E+01			1.98E+01	1.5E+03	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T07-F	1	4.79E+01			4.79E+01	3.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T08-F	1	5.40E+01			5.40E+01	2.9E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1313-T09-F	1	7.55E+01			7.55E+01	2.6E+01	3.7E+00	1.2E+01			---		VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	CFS-LRef-1313-T01-D	1	2.48E+04			2.48E+04	1.6E+00	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T02-D	1	1.84E+04			1.84E+04	5.9E-01	1.6E+00	5.1E+00	1000	100	1.93E+04	88%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T03-D	1	1.19E+04			1.19E+04	9.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T04-D	1	1.02E+04			1.02E+04	1.4E+00	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T05-D	1	2.59E+05			2.59E+05	8.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T06-D	1	3.52E+05			3.52E+05	3.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T07-D	1	5.55E+05			5.55E+05	9.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T08-D	1	2.56E+06			2.56E+06	6.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T09-D	1	2.65E+06			2.65E+06	5.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T01-E	1	2.57E+04			2.57E+04	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T02-E	1	1.90E+04			1.90E+04	5.5E-01	1.6E+00	5.1E+00	1000	100	1.98E+04	89%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T03-E	1	1.23E+04			1.23E+04	5.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T04-E	1	9.84E+03			9.84E+03	9.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T05-E	1	2.57E+05			2.57E+05	4.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T06-E	1	3.53E+05			3.53E+05	1.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T07-E	1	5.71E+05			5.71E+05	1.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T08-E	1	2.69E+06			2.69E+06	8.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T09-E	1	2.57E+06			2.57E+06	1.4E+00	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T01-F	1	2.61E+04			2.61E+04	1.5E+01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T02-F	1	1.92E+04			1.92E+04	4.9E-01	1.6E+00	5.1E+00	1000	100	2.00E+04	83%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T03-F	1	1.22E+04			1.22E+04	1.5E+00	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T04-F	1	9.57E+03			9.57E+03	4.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T05-F	1	2.58E+05			2.58E+05	8.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T06-F	1	3.47E+05			3.47E+05	5.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T07-F	1	5.61E+05			5.61E+05	2.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T08-F	1	2.60E+06			2.60E+06	1.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1313-T09-F	1	2.53E+06			2.53E+06	6.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	CFS-LRef-1313-T01-D	1	5.48E+02			5.48E+02	2.7E+00	1.5E+01	4.8E+01			---		VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T02-D	1	2.47E+02			2.47E+02	1.6E+01	1.5E+01	4.8E+01	10	100	1.27E+03	103%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T03-D	1	9.78E+01			9.78E+01	1.0E+01	1.5E+01	4.8E+01			---		VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T04-D	1	6.60E+01			6.60E+01	7.0E+00	1.5E+01	4.8E+01			---		VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T05-D	1	1.04E+02			1.04E+02	1.3E+01	1.5E+01	4.8E+01			---		VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T06-D	1	1.64E+02			1.64E+02	1.1E+01	1.5E+01	4.8E+01			---		VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T07-D	1	5.89E+02			5.89E+02	2.2E+00	1.5E+01	4.8E+01			---		VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T08-D	1	4.76E+02			4.76E+02	4.0E+00	1.5E+01	4.8E+01			---		VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T09-D	1	2.95E+02			2.95E+02	1.9E+00	1.5E+01	4.8E+01			---		VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T01-E	1	4.86E+02			4.86E+02	4.5E+00	1.5E+01	4.8E+01			---		VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T02-E	1	2.38E+02			2.38E+02	6.9E+00	1.5E+01	4.8E+01	10	100	1.19E+03	95%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T03-E	1	1.21E+02			1.21E+02	4.8E+00	1.5E+01	4.8E+01			---		VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T04-E	1	8.55E+01			8.55E+01	1.9E+01	1.5E+01	4.8E+01			---		VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T05-E	1	1.04E+02			1.04E+02	8.5E+00	1.5E+01	4.8E+01			---		VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T06-E	1	1.57E+02			1.57E+02	3.9E+00	1.5E+01	4.8E+01			---		VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T07-E	1	5.62E+02			5.62E+02	1.3E+00	1.5E+01	4.8E+01			---		VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T08-E	1	4.04E+02			4.04E+02	7.5E-01	1.5E+01	4.8E+01			---		VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T09-E	1	2.77E+02			2.77E+02	4.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T01-F	1	4.28E+02			4.28E+02	1.4E+01	1.5E+01	4.8E+01			---		VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T02-F	1	2.39E+02			2.39E+02	7.1E+00	1.5E+01	4.8E+01	10	100	1.25E+03	101%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T03-F	1	1.16E+02			1.16E+02	1.4E+01	1.5E+01	4.8E+01			---		VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T04-F	1	5.76E+01			5.76E+01	1.7E+01	1.5E+01	4.8E+01			---		VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T05-F	1	9.58E+01			9.58E+01	1.2E+01	1.5E+01	4.8E+01			---		VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T06-F	1	1.40E+02			1.40E+02	8.0E+00	1.5E+01	4.8E+01			---		VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T07-F	1	5.49E+02			5.49E+02	2.9E+00	1.5E+01	4.8E+01			---		VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T08-F	1	4.53E+02			4.53E+02	3.3E+00	1.5E+01	4.8E+01			---		VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1313-T09-F	1	2.78E+02			2.78E+02	4.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	CFS-LRef-1313-T01-D	1	1.53E+05			1.53E+05	6.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T02-D	1	7.97E+04			7.97E+04	3.1E-01	1.1E+00	3.5E+00	1000	100	8.06E+04	87%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T03-D	1	2.60E+04			2.60E+04	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T04-D	1	4.35E+03			4.35E+03	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T05-D	1	1.01E+03			1.01E+03	9.3E-02	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T06-D	1	5.76E+02			5.76E+02	8.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T07-D	1	5.05E+02			5.05E+02	8.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T08-D	1	2.40E+02			2.40E+02	2.5E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T09-D	1	2.24E+02			2.24E+02	2.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T01-E	1	1.54E+05			1.54E+05	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T02-E	1	7.90E+04			7.90E+04	5.7E-01	1.1E+00	3.5E+00	1000	100	7.99E+04	86%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T03-E	1	2.61E+04			2.61E+04	1.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T04-E	1	4.16E+03			4.16E+03	7.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T05-E	1	9.84E+02			9.84E+02	4.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T06-E	1	5.87E+02			5.87E+02	9.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T07-E	1	5.34E+02			5.34E+02	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T08-E	1	2.60E+02			2.60E+02	2.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T09-E	1	2.25E+02			2.25E+02	1.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T01-F	1	1.69E+05			1.69E+05	1.1E+01	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T02-F	1	8.77E+04			8.77E+04	5.3E-01	1.1E+00	3.5E+00	1000	100	8.86E+04	90%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T03-F	1	2.53E+04			2.53E+04	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T04-F	1	4.20E+03			4.20E+03	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T05-F	1	1.01E+03			1.01E+03	5.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T06-F	1	5.63E+02			5.63E+02	3.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T07-F	1	4.94E+02			4.94E+02	1.8E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T08-F	1	2.17E+02			2.17E+02	3.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1313-T09-F	1	2.25E+02			2.25E+02	1.4E+00	1.1E+00	3.5E+00				---	VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	CFS-LRef-1313-T01-D	1	2.94E+04			2.94E+04	5.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T02-D	1	2.77E+04			2.77E+04	3.7E-01	2.5E+00	8.0E+00	1000	100	2.86E+04	89%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T03-D	1	2.07E+04			2.07E+04	7.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T04-D	1	2.04E+04			2.04E+04	2.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T05-D	1	2.01E+04			2.01E+04	8.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T06-D	1	1.91E+04			1.91E+04	9.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T07-D	1	1.86E+04			1.86E+04	1.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T08-D	1	1.94E+04			1.94E+04	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T09-D	1	1.97E+04			1.97E+04	5.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T01-E	1	3.14E+04			3.14E+04	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T02-E	1	2.80E+04			2.80E+04	6.7E-01	2.5E+00	8.0E+00	1000	100	2.88E+04	85%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T03-E	1	2.24E+04			2.24E+04	3.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T04-E	1	2.07E+04			2.07E+04	1.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T05-E	1	2.02E+04			2.02E+04	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T06-E	1	1.98E+04			1.98E+04	1.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T07-E	1	1.90E+04			1.90E+04	9.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T08-E	1	1.96E+04			1.96E+04	7.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T09-E	1	2.29E+04			2.29E+04	7.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T01-F	1	3.01E+04			3.01E+04	1.3E+01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T02-F	1	2.82E+04			2.82E+04	1.5E+00	2.5E+00	8.0E+00	1000	100	2.90E+04	87%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T03-F	1	2.15E+04			2.15E+04	9.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T04-F	1	1.96E+04			1.96E+04	9.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T05-F	1	2.07E+04			2.07E+04	9.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T06-F	1	2.00E+04			2.00E+04	5.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T07-F	1	2.01E+04			2.01E+04	6.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T08-F	1	1.95E+04			1.95E+04	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1313-T09-F	1	2.02E+04			2.02E+04	6.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	CFS-LRef-1313-T01-D	1	1.26E+03			1.26E+03	5.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T02-D	1	1.31E+03			1.31E+03	1.2E+00	1.0E+00	3.2E+00	1000	100	2.23E+03	92%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T03-D	1	9.45E+02			9.45E+02	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T04-D	1	1.56E+03			1.56E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T05-D	1	3.66E+03			3.66E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T06-D	1	3.63E+03			3.63E+03	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T07-D	1	4.01E+03			4.01E+03	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T08-D	1	3.91E+03			3.91E+03	1.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T09-D	1	3.28E+03			3.28E+03	8.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T01-E	1	1.43E+03			1.43E+03	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T02-E	1	1.28E+03			1.28E+03	1.2E+00	1.0E+00	3.2E+00	1000	100	2.23E+03	94%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T03-E	1	9.67E+02			9.67E+02	8.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T04-E	1	1.48E+03			1.48E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T05-E	1	3.49E+03			3.49E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T06-E	1	3.70E+03			3.70E+03	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T07-E	1	4.06E+03			4.06E+03	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T08-E	1	3.69E+03			3.69E+03	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T09-E	1	3.20E+03			3.20E+03	4.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T01-F	1	1.21E+03			1.21E+03	4.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T02-F	1	1.30E+03			1.30E+03	6.9E-01	1.0E+00	3.2E+00	1000	100	2.26E+03	96%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T03-F	1	9.46E+02			9.46E+02	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T04-F	1	1.45E+03			1.45E+03	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T05-F	1	3.50E+03			3.50E+03	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T06-F	1	3.68E+03			3.68E+03	4.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T07-F	1	4.11E+03			4.11E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T08-F	1	3.69E+03			3.69E+03	9.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1313-T09-F	1	3.11E+03			3.11E+03	5.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	CFS-LRef-1313-T01-D	1	7.75E+05			7.75E+05	8.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T02-D	1	7.02E+05			7.02E+05	3.8E-01	6.8E+00	2.2E+01	1000	100	7.03E+05	85%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T03-D	1	6.07E+05			6.07E+05	9.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T04-D	1	5.96E+05			5.96E+05	1.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T05-D	1	6.60E+05			6.60E+05	6.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T06-D	1	6.80E+05			6.80E+05	6.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T07-D	1	7.63E+05			7.63E+05	4.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T08-D	1	1.01E+06			1.01E+06	5.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T09-D	1	1.31E+06			1.31E+06	5.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T01-E	1	7.89E+05			7.89E+05	8.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T02-E	1	7.10E+05			7.10E+05	7.0E-01	6.8E+00	2.2E+01	1000	100	7.11E+05	89%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T03-E	1	6.18E+05			6.18E+05	5.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T04-E	1	5.87E+05			5.87E+05	9.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T05-E	1	6.61E+05			6.61E+05	2.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T06-E	1	6.88E+05			6.88E+05	7.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T07-E	1	7.73E+05			7.73E+05	6.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T08-E	1	9.50E+05			9.50E+05	5.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T09-E	1	1.19E+06			1.19E+06	9.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T01-F	1	7.39E+05			7.39E+05	1.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T02-F	1	7.25E+05			7.25E+05	8.7E-01	6.8E+00	2.2E+01	1000	100	7.26E+05	84%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T03-F	1	6.01E+05			6.01E+05	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T04-F	1	5.63E+05			5.63E+05	5.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T05-F	1	6.52E+05			6.52E+05	7.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T06-F	1	6.64E+05			6.64E+05	5.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T07-F	1	7.50E+05			7.50E+05	2.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T08-F	1	9.77E+05			9.77E+05	1.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1313-T09-F	1	1.26E+06			1.26E+06	7.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

TI	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	CFS-LRef-1313-T01-D	1	1.77E+03			1.77E+03	2.1E-01	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T02-D	1	1.04E+03			1.04E+03	1.7E+00	4.6E+00	1.5E+01	10	100	2.07E+03	102%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T03-D	1	6.10E+02			6.10E+02	1.6E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T04-D	1	3.78E+02			3.78E+02	2.0E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T05-D	1	7.01E+02			7.01E+02	1.4E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T06-D	1	5.73E+02			5.73E+02	7.1E-01	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T07-D	1	3.43E+02			3.43E+02	1.4E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T08-D	1	2.29E+02			2.29E+02	2.8E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T09-D	1	2.18E+02			2.18E+02	2.4E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T01-E	1	1.74E+03			1.74E+03	8.9E-01	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T02-E	1	1.06E+03			1.06E+03	8.1E-01	4.6E+00	1.5E+01	10	100	2.01E+03	95%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T03-E	1	6.21E+02			6.21E+02	3.3E-01	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T04-E	1	3.68E+02			3.68E+02	2.0E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T05-E	1	7.02E+02			7.02E+02	3.1E-01	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T06-E	1	5.80E+02			5.80E+02	1.4E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T07-E	1	3.57E+02			3.57E+02	8.5E-01	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T08-E	1	2.21E+02			2.21E+02	6.8E-01	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T09-E	1	2.17E+02			2.17E+02	3.7E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T01-F	1	1.65E+03			1.65E+03	1.8E+01	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T02-F	1	1.07E+03			1.07E+03	5.4E-01	4.6E+00	1.5E+01	10	100	2.04E+03	97%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T03-F	1	6.22E+02			6.22E+02	2.6E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T04-F	1	3.53E+02			3.53E+02	9.0E-01	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T05-F	1	6.94E+02			6.94E+02	4.6E-01	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T06-F	1	5.58E+02			5.58E+02	7.9E-01	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T07-F	1	3.40E+02			3.40E+02	2.4E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T08-F	1	2.15E+02			2.15E+02	3.1E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1313-T09-F	1	2.05E+02			2.05E+02	5.2E+00	4.6E+00	1.5E+01			---		VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	CFS-LRef-1313-T01-D	1	4.44E+01			4.44E+01	2.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T02-D	1	1.14E+01			1.14E+01	5.1E-01	2.0E+00	6.4E+00	10	100	1.05E+03	104%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T03-D	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T04-D	1	1.00E+00	U1/2		1.00E+00	8.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T05-D	1	1.00E+00	U1/2		1.00E+00	9.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T06-D	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T07-D	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T08-D	1	1.00E+00	U1/2		1.00E+00	3.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T09-D	1	1.00E+00	U1/2		1.00E+00	5.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T01-E	1	4.25E+01			4.25E+01	3.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T02-E	1	1.25E+01			1.25E+01	1.1E+01	2.0E+00	6.4E+00	10	100	9.62E+02	95%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T03-E	1	1.00E+00	U1/2		1.00E+00	4.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T04-E	1	1.00E+00	U1/2		1.00E+00	3.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T05-E	1	1.00E+00	U1/2		1.00E+00	2.5E+02	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T06-E	1	1.00E+00	U1/2		1.00E+00	4.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T07-E	1	1.00E+00	U1/2		1.00E+00	8.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T08-E	1	1.00E+00	U1/2		1.00E+00	9.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T09-E	1	1.00E+00	U1/2		1.00E+00	8.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T01-F	1	3.35E+01			3.35E+01	4.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T02-F	1	1.25E+01			1.25E+01	3.5E+00	2.0E+00	6.4E+00	10	100	1.04E+03	102%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T03-F	1	1.00E+00	U1/2		1.00E+00	3.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T04-F	1	1.00E+00	U1/2		1.00E+00	2.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T05-F	1	1.00E+00	U1/2		1.00E+00	3.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T06-F	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T07-F	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T08-F	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1313-T09-F	1	1.00E+00	U1/2		1.00E+00	2.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	CFS-LRef-1313-T01-D	1	5.57E+02			5.57E+02	5.1E-01	1.5E+00	4.8E+00			---		VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T02-D	1	6.76E+01			6.76E+01	1.1E+01	1.5E+00	4.8E+00	10	100	1.13E+03	106%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T03-D	1	4.95E+01			4.95E+01	2.6E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T04-D	1	3.86E+01			3.86E+01	4.6E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T05-D	1	3.73E+01			3.73E+01	1.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T06-D	1	3.69E+01			3.69E+01	2.3E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T07-D	1	3.58E+01			3.58E+01	5.5E-01	1.5E+00	4.8E+00			---		VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T08-D	1	3.04E+01			3.04E+01	2.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T09-D	1	3.83E+01			3.83E+01	5.7E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T01-E	1	5.77E+02			5.77E+02	2.9E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T02-E	1	6.54E+01			6.54E+01	1.8E+00	1.5E+00	4.8E+00	10	100	1.02E+03	96%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T03-E	1	4.76E+01			4.76E+01	1.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T04-E	1	3.86E+01			3.86E+01	1.5E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T05-E	1	3.73E+01			3.73E+01	3.3E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T06-E	1	3.67E+01			3.67E+01	2.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T07-E	1	3.72E+01			3.72E+01	4.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T08-E	1	3.10E+01			3.10E+01	4.9E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T09-E	1	3.75E+01			3.75E+01	6.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T01-F	1	4.66E+02			4.66E+02	4.9E+01	1.5E+00	4.8E+00			---		VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T02-F	1	6.64E+01			6.64E+01	5.3E+00	1.5E+00	4.8E+00	10	100	1.12E+03	105%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T03-F	1	4.90E+01			4.90E+01	1.8E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T04-F	1	3.81E+01			3.81E+01	3.9E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T05-F	1	3.79E+01			3.79E+01	1.3E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T06-F	1	3.61E+01			3.61E+01	2.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T07-F	1	3.65E+01			3.65E+01	2.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T08-F	1	3.52E+01			3.52E+01	2.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1313-T09-F	1	3.98E+01			3.98E+01	1.5E+00	1.5E+00	4.8E+00			---		VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	CFS-LRef-1313-T01-D	1	1.76E+05			1.76E+05	8.3E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:03 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T02-D	1	1.89E+05			1.89E+05	1.2E+00	1.0E+00	3.2E+00	10	100	1.90E+05	92%	VU ICP-OES	2/3/11 4:05 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T03-D	1	1.64E+05			1.64E+05	1.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:06 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T04-D	1	2.50E+04			2.50E+04	1.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:08 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T05-D	1	1.28E+02			1.28E+02	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:10 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T06-D	1	2.43E+01			2.43E+01	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T07-D	1	3.03E+01			3.03E+01	1.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:13 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T08-D	1	2.63E+03			2.63E+03	3.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:15 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T09-D	1	4.75E+03			4.75E+03	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T01-E	1	1.76E+05			1.76E+05	2.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:18 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T02-E	1	1.87E+05			1.87E+05	1.2E+00	1.0E+00	3.2E+00	10	100	1.88E+05	89%	VU ICP-OES	2/3/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T03-E	1	1.59E+05			1.59E+05	5.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:21 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T04-E	1	2.50E+04			2.50E+04	7.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:23 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T05-E	1	1.04E+02			1.04E+02	4.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T06-E	1	2.36E+01			2.36E+01	4.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:26 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T07-E	1	4.42E+01			4.42E+01	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T08-E	1	2.59E+03			2.59E+03	1.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T09-E	1	4.60E+03			4.60E+03	8.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 11:35 AM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T01-F	1	1.63E+05			1.63E+05	2.1E+01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T02-F	1	1.92E+05			1.92E+05	7.2E-01	1.0E+00	3.2E+00	10	100	1.93E+05	93%	VU ICP-OES	2/3/11 4:54 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T03-F	1	1.64E+05			1.64E+05	1.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T04-F	1	2.50E+04			2.50E+04	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T05-F	1	1.07E+02			1.07E+02	3.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 4:58 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T06-F	1	3.31E+01			3.31E+01	9.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 5:00 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T07-F	1	3.01E+01			3.01E+01	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 5:02 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T08-F	1	2.76E+03			2.76E+03	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 5:03 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1313-T09-F	1	4.61E+03			4.61E+03	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	2/3/11 5:05 PM	EPA Interlab LRef 1313-1316 CFS

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	EaFA-L01-1316-T01-A	1	1.24E+02			1.24E+02	9.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1316-T02-A	1	1.64E+02			1.64E+02	5.4E-01	1.0E+00	3.2E+00	1000	100	9.93E+02	83%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1316-T03-A	1	2.43E+02			2.43E+02	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1316-T04-A	1	5.09E+02			5.09E+02	3.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1316-T05-A															
Al	EaFA-L01-1316-T01-B	1	1.30E+02			1.30E+02	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1316-T02-B	1	1.76E+02			1.76E+02	1.7E+00	1.0E+00	3.2E+00	1000	100	9.83E+02	81%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1316-T03-B	1	2.52E+02			2.52E+02	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1316-T04-B	1	5.11E+02			5.11E+02	9.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1316-T05-B															
Al	EaFA-L01-1316-T01-C	1	1.18E+02			1.18E+02	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1316-T02-C	1	1.74E+02			1.74E+02	4.6E-01	1.0E+00	3.2E+00	1000	100	9.88E+02	81%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1316-T03-C	1	2.41E+02			2.41E+02	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1316-T04-C	1	4.74E+02			4.74E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
Al	EaFA-L01-1316-T05-C															
Al	EaFA-L01-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	4.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	EaFA-L01-1316-T01-A	1	2.20E+02			2.20E+02	8.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1316-T02-A	1	3.20E+02			3.20E+02	4.5E+00	7.5E+00	2.4E+01	10	250	2.92E+03	104%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1316-T03-A	1	4.56E+02			4.56E+02	1.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1316-T04-A	1	6.51E+02			6.51E+02	3.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1316-T05-A															
Sb	EaFA-L01-1316-T01-B	1	2.09E+02			2.09E+02	6.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1316-T02-B	1	3.26E+02			3.26E+02	1.1E+01	7.5E+00	2.4E+01	10	250	2.65E+03	93%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1316-T03-B	1	4.52E+02			4.52E+02	2.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1316-T04-B	1	7.06E+02			7.06E+02	2.9E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1316-T05-B															
Sb	EaFA-L01-1316-T01-C	1	1.86E+02			1.86E+02	6.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1316-T02-C	1	3.46E+02			3.46E+02	7.6E+00	7.5E+00	2.4E+01	10	250	2.73E+03	95%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1316-T03-C	1	4.62E+02			4.62E+02	5.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1316-T04-C	1	6.65E+02			6.65E+02	1.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
Sb	EaFA-L01-1316-T05-C															
Sb	EaFA-L01-1316-B01-A	1	3.75E+00	U1/2		3.75E+00	1.4E+02	7.5E+00	2.4E+01				---	VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	EaFA-L01-1316-T01-A	1	1.21E+02			1.21E+02	1.0E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1316-T02-A	1	1.47E+02			1.47E+02	1.6E+01	1.1E+01	3.5E+01	10	250	2.74E+03	104%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1316-T03-A	1	1.38E+02			1.38E+02	9.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1316-T04-A	1	2.12E+02			2.12E+02	7.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1316-T05-A															
As	EaFA-L01-1316-T01-B	1	1.13E+02			1.13E+02	1.2E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1316-T02-B	1	1.37E+02			1.37E+02	8.8E+00	1.1E+01	3.5E+01	10	250	2.48E+03	94%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1316-T03-B	1	1.21E+02			1.21E+02	2.1E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1316-T04-B	1	1.82E+02			1.82E+02	5.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1316-T05-B															
As	EaFA-L01-1316-T01-C	1	1.14E+02			1.14E+02	2.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1316-T02-C	1	1.53E+02			1.53E+02	9.5E+00	1.1E+01	3.5E+01	10	250	2.56E+03	96%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1316-T03-C	1	1.30E+02			1.30E+02	9.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1316-T04-C	1	1.72E+02			1.72E+02	5.4E-01	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
As	EaFA-L01-1316-T05-C															
As	EaFA-L01-1316-B01-A	1	5.50E+00	U1/2		5.50E+00	2.3E+02	1.1E+01	3.5E+01				---	VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	EaFA-L01-1316-T01-A	1	4.23E+03			4.23E+03	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1316-T02-A	1	8.52E+03			8.52E+03	1.1E+00	1.0E+00	3.2E+00	1000	100	9.34E+03	82%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1316-T03-A	1	2.04E+04			2.04E+04	3.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1316-T04-A	1	3.68E+04			3.68E+04	3.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1316-T05-A															
B	EaFA-L01-1316-T01-B	1	4.96E+03			4.96E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1316-T02-B	1	8.98E+03			8.98E+03	1.2E+00	1.0E+00	3.2E+00	1000	100	9.80E+03	81%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1316-T03-B	1	2.05E+04			2.05E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1316-T04-B	1	3.86E+04			3.86E+04	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1316-T05-B															
B	EaFA-L01-1316-T01-C	1	3.96E+03			3.96E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1316-T02-C	1	8.80E+03			8.80E+03	1.1E+00	1.0E+00	3.2E+00	1000	100	9.65E+03	86%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1316-T03-C	1	1.92E+04			1.92E+04	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1316-T04-C	1	3.73E+04			3.73E+04	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
B	EaFA-L01-1316-T05-C															
B	EaFA-L01-1316-B01-A	1	6.27E+01			6.27E+01	2.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	EaFA-L01-1316-T01-A	1	2.74E+02			2.74E+02	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1316-T02-A	1	2.13E+02			2.13E+02	4.8E-01	1.0E+00	3.2E+00	10	250	2.53E+03	93%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1316-T03-A	1	2.06E+02			2.06E+02	2.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1316-T04-A	1	2.21E+02			2.21E+02	3.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1316-T05-A															
Ba	EaFA-L01-1316-T01-B	1	2.80E+02			2.80E+02	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1316-T02-B	1	2.31E+02			2.31E+02	9.0E-01	1.0E+00	3.2E+00	10	250	2.30E+03	83%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1316-T03-B	1	2.08E+02			2.08E+02	4.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1316-T04-B	1	2.34E+02			2.34E+02	4.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1316-T05-B															
Ba	EaFA-L01-1316-T01-C	1	2.56E+02			2.56E+02	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1316-T02-C	1	2.27E+02			2.27E+02	1.4E+00	1.0E+00	3.2E+00	10	250	2.34E+03	84%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1316-T03-C	1	1.97E+02			1.97E+02	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1316-T04-C	1	2.29E+02			2.29E+02	1.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
Ba	EaFA-L01-1316-T05-C															
Ba	EaFA-L01-1316-B01-A	1	1.41E+00	E		1.41E+00	5.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	EaFA-L01-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	1.0E+03	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	7.7E+01	1.9E+00	6.0E+00	10	250	2.62E+03	105%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	8.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	9.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1316-T05-A															
Be	EaFA-L01-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	2.6E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	2.3E+02	1.9E+00	6.0E+00	10	250	2.36E+03	95%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	5.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1316-T05-B															
Be	EaFA-L01-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	2.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	7.7E+01	1.9E+00	6.0E+00	10	250	2.42E+03	97%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	6.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	2.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
Be	EaFA-L01-1316-T05-C															
Be	EaFA-L01-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	5.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	EaFA-L01-1316-T01-A	1	1.10E+00	U1/2		1.10E+00	3.4E+01	2.2E+00	7.0E+00			---		VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1316-T02-A	1	1.10E+00	U1/2		1.10E+00	9.6E+00	2.2E+00	7.0E+00	10	250	2.73E+03	109%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1316-T03-A	1	1.10E+00	U1/2		1.10E+00	3.9E+01	2.2E+00	7.0E+00			---		VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1316-T04-A	1	1.10E+00	U1/2		1.10E+00	1.9E+01	2.2E+00	7.0E+00			---		VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1316-T05-A															
Cd	EaFA-L01-1316-T01-B	1	1.10E+00	U1/2		1.10E+00	1.6E+01	2.2E+00	7.0E+00			---		VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1316-T02-B	1	1.10E+00	U1/2		1.10E+00	1.1E+02	2.2E+00	7.0E+00	10	250	2.44E+03	98%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1316-T03-B	1	1.10E+00	U1/2		1.10E+00	5.4E+01	2.2E+00	7.0E+00			---		VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1316-T04-B	1	1.10E+00	U1/2		1.10E+00	5.6E+00	2.2E+00	7.0E+00			---		VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1316-T05-B															
Cd	EaFA-L01-1316-T01-C	1	1.10E+00	U1/2		1.10E+00	8.4E+00	2.2E+00	7.0E+00			---		VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1316-T02-C	1	1.10E+00	U1/2		1.10E+00	1.6E+01	2.2E+00	7.0E+00	10	250	2.51E+03	100%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1316-T03-C	1	1.10E+00	U1/2		1.10E+00	3.4E+01	2.2E+00	7.0E+00			---		VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1316-T04-C	1	1.10E+00	U1/2		1.10E+00	3.9E+01	2.2E+00	7.0E+00			---		VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
Cd	EaFA-L01-1316-T05-C															
Cd	EaFA-L01-1316-B01-A	1	1.10E+00	U1/2		1.10E+00	1.3E+01	2.2E+00	7.0E+00			---		VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	EaFA-L01-1316-T01-A	1	1.58E+05			1.58E+05	8.1E-01	2.6E+00	8.3E+00			---		VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1316-T02-A	1	3.20E+05			3.20E+05	3.7E-01	2.6E+00	8.3E+00	1000	100	3.21E+05	93%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1316-T03-A	1	7.38E+05			7.38E+05	2.8E+00	2.6E+00	8.3E+00			---		VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1316-T04-A	1	5.82E+05			5.82E+05	3.6E+00	2.6E+00	8.3E+00			---		VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1316-T05-A															
Ca	EaFA-L01-1316-T01-B	1	1.62E+05			1.62E+05	9.5E-02	2.6E+00	8.3E+00			---		VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1316-T02-B	1	3.28E+05			3.28E+05	8.6E-01	2.6E+00	8.3E+00	1000	100	3.29E+05	97%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1316-T03-B	1	7.36E+05			7.36E+05	4.5E-01	2.6E+00	8.3E+00			---		VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1316-T04-B	1	6.16E+05			6.16E+05	5.8E-01	2.6E+00	8.3E+00			---		VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1316-T05-B															
Ca	EaFA-L01-1316-T01-C	1	1.40E+05			1.40E+05	6.9E-01	2.6E+00	8.3E+00			---		VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1316-T02-C	1	3.31E+05			3.31E+05	1.5E+00	2.6E+00	8.3E+00	1000	100	3.32E+05	91%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1316-T03-C	1	6.90E+05			6.90E+05	1.2E+00	2.6E+00	8.3E+00			---		VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1316-T04-C	1	5.85E+05			5.85E+05	2.0E-01	2.6E+00	8.3E+00			---		VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
Ca	EaFA-L01-1316-T05-C															
Ca	EaFA-L01-1316-B01-A	1	1.30E+00	U1/2		1.30E+00	4.1E+02	2.6E+00	8.3E+00			---		VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	EaFA-L01-1316-T01-A	1	1.20E+01			1.20E+01	1.7E+01	1.2E+00	3.8E+00			---		VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1316-T02-A	1	1.52E+01			1.52E+01	1.2E+01	1.2E+00	3.8E+00	10	250	2.57E+03	102%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1316-T03-A	1	2.33E+01			2.33E+01	4.9E+00	1.2E+00	3.8E+00			---		VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1316-T04-A	1	4.87E+01			4.87E+01	6.0E+00	1.2E+00	3.8E+00			---		VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1316-T05-A															
Cr	EaFA-L01-1316-T01-B	1	1.10E+01			1.10E+01	3.2E+00	1.2E+00	3.8E+00			---		VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1316-T02-B	1	1.70E+01			1.70E+01	7.2E+00	1.2E+00	3.8E+00	10	250	2.31E+03	92%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1316-T03-B	1	2.27E+01			2.27E+01	6.6E+00	1.2E+00	3.8E+00			---		VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1316-T04-B	1	4.75E+01			4.75E+01	1.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1316-T05-B															
Cr	EaFA-L01-1316-T01-C	1	1.09E+01			1.09E+01	9.2E+00	1.2E+00	3.8E+00			---		VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1316-T02-C	1	1.99E+01			1.99E+01	8.4E+00	1.2E+00	3.8E+00	10	250	2.37E+03	94%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1316-T03-C	1	1.96E+01			1.96E+01	4.7E+00	1.2E+00	3.8E+00			---		VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1316-T04-C	1	4.46E+01			4.46E+01	2.5E+00	1.2E+00	3.8E+00			---		VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
Cr	EaFA-L01-1316-T05-C															
Cr	EaFA-L01-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	1.2E+03	1.2E+00	3.8E+00			---		VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	EaFA-L01-1316-T01-A	1	7.61E+01			7.61E+01	2.0E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1316-T02-A	1	1.20E+02			1.20E+02	3.8E+00	1.8E+00	5.7E+00	10	250	2.76E+03	105%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1316-T03-A	1	2.36E+02			2.36E+02	3.4E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1316-T04-A	1	1.12E+02			1.12E+02	7.1E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1316-T05-A															
Co	EaFA-L01-1316-T01-B	1	7.79E+01			7.79E+01	5.3E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1316-T02-B	1	1.21E+02			1.21E+02	1.8E+00	1.8E+00	5.7E+00	10	250	2.49E+03	95%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1316-T03-B	1	2.16E+02			2.16E+02	2.5E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1316-T04-B	1	1.30E+02			1.30E+02	2.6E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1316-T05-B															
Co	EaFA-L01-1316-T01-C	1	6.35E+01			6.35E+01	3.4E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1316-T02-C	1	1.24E+02			1.24E+02	4.9E+00	1.8E+00	5.7E+00	10	250	2.53E+03	96%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1316-T03-C	1	2.15E+02			2.15E+02	1.9E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1316-T04-C	1	1.48E+02			1.48E+02	2.6E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
Co	EaFA-L01-1316-T05-C															
Co	EaFA-L01-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	9.2E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	EaFA-L01-1316-T01-A	1	1.14E+01	E		1.14E+01	7.9E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1316-T02-A	1	1.85E+01			1.85E+01	5.7E+01	3.7E+00	1.2E+01	10	250	2.57E+03	102%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1316-T03-A	1	1.52E+01			1.52E+01	3.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1316-T04-A	1	1.11E+01	E		1.11E+01	2.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1316-T05-A															
Cu	EaFA-L01-1316-T01-B	1	1.16E+01	E		1.16E+01	4.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1316-T02-B	1	1.34E+01			1.34E+01	3.8E+01	3.7E+00	1.2E+01	10	250	2.33E+03	93%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1316-T03-B	1	1.74E+01			1.74E+01	1.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1316-T04-B	1	1.56E+01			1.56E+01	5.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1316-T05-B															
Cu	EaFA-L01-1316-T01-C	1	1.28E+01			1.28E+01	5.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1316-T02-C	1	1.57E+01			1.57E+01	3.7E+01	3.7E+00	1.2E+01	10	250	2.38E+03	94%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1316-T03-C	1	1.47E+01			1.47E+01	1.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1316-T04-C	1	8.87E+00	E		8.87E+00	4.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
Cu	EaFA-L01-1316-T05-C															
Cu	EaFA-L01-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	4.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	EaFA-L01-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	1.5E+03	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	9.6E+00	2.0E+00	6.4E+00	1000	100	8.68E+02	87%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	7.5E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	3.9E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1316-T05-A															
Fe	EaFA-L01-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	2.6E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	3.2E+00	2.0E+00	6.4E+00	1000	100	8.47E+02	85%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	3.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1316-T05-B															
Fe	EaFA-L01-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	4.5E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	8.0E-01	2.0E+00	6.4E+00	1000	100	8.45E+02	84%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	6.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
Fe	EaFA-L01-1316-T05-C															
Fe	EaFA-L01-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	4.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	EaFA-L01-1316-T01-A	1	3.40E+00	U1/2		3.40E+00	2.7E+02	6.8E+00	2.2E+01			---		VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1316-T02-A	1	3.40E+00	U1/2		3.40E+00	8.5E+02	6.8E+00	2.2E+01	10	250	2.55E+03	102%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1316-T03-A	1	3.40E+00	U1/2		3.40E+00	2.2E+01	6.8E+00	2.2E+01			---		VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1316-T04-A	1	3.40E+00	U1/2		3.40E+00	3.3E+01	6.8E+00	2.2E+01			---		VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1316-T05-A															
Pb	EaFA-L01-1316-T01-B	1	3.40E+00	U1/2		3.40E+00	1.3E+02	6.8E+00	2.2E+01			---		VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1316-T02-B	1	3.40E+00	U1/2		3.40E+00	1.5E+01	6.8E+00	2.2E+01	10	250	2.27E+03	90%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1316-T03-B	1	3.40E+00	U1/2		3.40E+00	2.2E+02	6.8E+00	2.2E+01			---		VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1316-T04-B	1	3.40E+00	U1/2		3.40E+00	4.7E+01	6.8E+00	2.2E+01			---		VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1316-T05-B															
Pb	EaFA-L01-1316-T01-C	1	3.40E+00	U1/2		3.40E+00	1.8E+02	6.8E+00	2.2E+01			---		VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1316-T02-C	1	3.40E+00	U1/2		3.40E+00	5.9E+02	6.8E+00	2.2E+01	10	250	2.31E+03	92%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1316-T03-C	1	3.40E+00	U1/2		3.40E+00	1.9E+02	6.8E+00	2.2E+01			---		VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1316-T04-C	1	3.40E+00	U1/2		3.40E+00	3.7E+02	6.8E+00	2.2E+01			---		VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
Pb	EaFA-L01-1316-T05-C															
Pb	EaFA-L01-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	4.4E+02	6.8E+00	2.2E+01			---		VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	EaFA-L01-1316-T01-A	1	5.40E+03			5.40E+03	5.0E-01	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1316-T02-A	1	1.06E+04			1.06E+04	3.9E-01	1.9E+00	6.0E+00	10	250	1.31E+04	100%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1316-T03-A	1	2.52E+04			2.52E+04	2.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1316-T04-A	1	5.10E+04			5.10E+04	3.8E+00	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1316-T05-A															
Li	EaFA-L01-1316-T01-B	1	5.51E+03			5.51E+03	4.8E-01	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1316-T02-B	1	1.09E+04			1.09E+04	1.1E+00	1.9E+00	6.0E+00	10	250	1.33E+04	95%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1316-T03-B	1	2.53E+04			2.53E+04	2.8E-01	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1316-T04-B	1	5.30E+04			5.30E+04	8.6E-01	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1316-T05-B															
Li	EaFA-L01-1316-T01-C	1	4.73E+03			4.73E+03	5.9E-01	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1316-T02-C	1	1.10E+04			1.10E+04	1.0E+00	1.9E+00	6.0E+00	10	250	1.33E+04	89%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1316-T03-C	1	2.38E+04			2.38E+04	9.8E-01	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1316-T04-C	1	4.98E+04			4.98E+04	3.8E-01	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
Li	EaFA-L01-1316-T05-C															
Li	EaFA-L01-1316-B01-A	1	5.14E+00	E		5.14E+00	6.4E+00	1.9E+00	6.0E+00			---		VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	EaFA-L01-1316-T01-A	1	4.64E+02			4.64E+02	1.5E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1316-T02-A	1	8.01E+02			8.01E+02	8.5E-01	2.0E+00	6.4E+00	10	250	3.25E+03	98%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1316-T03-A	1	1.55E+03			1.55E+03	4.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1316-T04-A	1	1.11E+03			1.11E+03	3.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1316-T05-A															
Mn	EaFA-L01-1316-T01-B	1	4.76E+02			4.76E+02	4.9E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1316-T02-B	1	8.04E+02			8.04E+02	8.6E-01	2.0E+00	6.4E+00	10	250	3.00E+03	88%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1316-T03-B	1	1.45E+03			1.45E+03	1.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1316-T04-B	1	1.23E+03			1.23E+03	6.0E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1316-T05-B															
Mn	EaFA-L01-1316-T01-C	1	3.79E+02			3.79E+02	1.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1316-T02-C	1	7.85E+02			7.85E+02	2.5E+00	2.0E+00	6.4E+00	10	250	3.01E+03	89%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1316-T03-C	1	1.43E+03			1.43E+03	9.2E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1316-T04-C	1	1.36E+03			1.36E+03	4.3E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
Mn	EaFA-L01-1316-T05-C															
Mn	EaFA-L01-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	EaFA-L01-1316-T01-A	1	7.03E+03			7.03E+03	6.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1316-T02-A	1	1.45E+04			1.45E+04	7.2E-01	1.0E+00	3.2E+00	1000	100	1.56E+04	104%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1316-T03-A	1	3.59E+04			3.59E+04	3.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1316-T04-A	1	6.85E+04			6.85E+04	2.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1316-T05-A															
Mg	EaFA-L01-1316-T01-B	1	7.22E+03			7.22E+03	4.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1316-T02-B	1	1.47E+04			1.47E+04	9.8E-01	1.0E+00	3.2E+00	1000	100	1.59E+04	116%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1316-T03-B	1	3.62E+04			3.62E+04	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1316-T04-B	1	7.17E+04			7.17E+04	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1316-T05-B															
Mg	EaFA-L01-1316-T01-C	1	6.11E+03			6.11E+03	9.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1316-T02-C	1	1.45E+04			1.45E+04	1.7E+00	1.0E+00	3.2E+00	1000	100	1.54E+04	92%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1316-T03-C	1	3.36E+04			3.36E+04	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1316-T04-C	1	6.71E+04			6.71E+04	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
Mg	EaFA-L01-1316-T05-C															
Mg	EaFA-L01-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.1E+03	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	EaFA-L01-1316-T01-A	1	3.26E+03			3.26E+03	7.3E-01	1.2E+00	3.8E+00			---		VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1316-T02-A	1	6.29E+03			6.29E+03	6.4E-01	1.2E+00	3.8E+00	10	250	8.47E+03	87%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1316-T03-A	1	1.41E+04			1.41E+04	2.9E+00	1.2E+00	3.8E+00			---		VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1316-T04-A	1	3.03E+04			3.03E+04	4.0E+00	1.2E+00	3.8E+00			---		VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1316-T05-A															
Mo	EaFA-L01-1316-T01-B	1	3.36E+03			3.36E+03	8.0E-02	1.2E+00	3.8E+00			---		VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1316-T02-B	1	6.50E+03			6.50E+03	9.5E-01	1.2E+00	3.8E+00	10	250	8.72E+03	89%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1316-T03-B	1	1.41E+04			1.41E+04	6.4E-01	1.2E+00	3.8E+00			---		VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1316-T04-B	1	3.11E+04			3.11E+04	4.5E-01	1.2E+00	3.8E+00			---		VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1316-T05-B															
Mo	EaFA-L01-1316-T01-C	1	2.91E+03			2.91E+03	4.0E-01	1.2E+00	3.8E+00			---		VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1316-T02-C	1	6.54E+03			6.54E+03	1.6E+00	1.2E+00	3.8E+00	10	250	8.63E+03	83%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1316-T03-C	1	1.33E+04			1.33E+04	1.4E+00	1.2E+00	3.8E+00			---		VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1316-T04-C	1	2.83E+04			2.83E+04	6.2E-02	1.2E+00	3.8E+00			---		VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
Mo	EaFA-L01-1316-T05-C															
Mo	EaFA-L01-1316-B01-A	1	4.28E+00			4.28E+00	6.5E+01	1.2E+00	3.8E+00			---		VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	EaFA-L01-1316-T01-A	1	1.69E+02			1.69E+02	2.0E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1316-T02-A	1	2.63E+02			2.63E+02	6.5E-01	1.8E+00	5.7E+00	10	250	2.86E+03	104%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1316-T03-A	1	5.11E+02			5.11E+02	2.5E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1316-T04-A	1	2.69E+02			2.69E+02	4.0E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1316-T05-A															
Ni	EaFA-L01-1316-T01-B	1	1.67E+02			1.67E+02	4.2E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1316-T02-B	1	2.74E+02			2.74E+02	1.3E+00	1.8E+00	5.7E+00	10	250	2.60E+03	93%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1316-T03-B	1	4.71E+02			4.71E+02	6.0E-01	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1316-T04-B	1	3.09E+02			3.09E+02	3.1E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1316-T05-B															
Ni	EaFA-L01-1316-T01-C	1	1.29E+02			1.29E+02	1.5E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1316-T02-C	1	2.76E+02			2.76E+02	1.1E+00	1.8E+00	5.7E+00	10	250	2.64E+03	95%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1316-T03-C	1	4.85E+02			4.85E+02	1.7E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1316-T04-C	1	3.44E+02			3.44E+02	1.2E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
Ni	EaFA-L01-1316-T05-C															
Ni	EaFA-L01-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	6.2E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	EaFA-L01-1316-T01-A	1	1.78E+01			1.78E+01	1.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1316-T02-A	1	4.24E+01			4.24E+01	5.5E+00	3.7E+00	1.2E+01	1000	100	9.01E+02	86%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1316-T03-A	1	7.87E+01			7.87E+01	1.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1316-T04-A	1	1.71E+02			1.71E+02	1.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1316-T05-A															
P	EaFA-L01-1316-T01-B	1	3.11E+01			3.11E+01	2.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1316-T02-B	1	3.00E+01			3.00E+01	1.8E+01	3.7E+00	1.2E+01	1000	100	8.50E+02	82%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1316-T03-B	1	3.81E+01			3.81E+01	5.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1316-T04-B	1	1.11E+02			1.11E+02	8.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1316-T05-B															
P	EaFA-L01-1316-T01-C	1	2.63E+01			2.63E+01	2.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1316-T02-C	1	5.01E+01			5.01E+01	1.6E+01	3.7E+00	1.2E+01	1000	100	8.77E+02	83%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1316-T03-C	1	3.77E+01			3.77E+01	2.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1316-T04-C	1	1.88E+02			1.88E+02	6.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
P	EaFA-L01-1316-T05-C															
P	EaFA-L01-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	2.1E+02	3.7E+00	1.2E+01				---	VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	EaFA-L01-1316-T01-A	1	2.30E+04			2.30E+04	6.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1316-T02-A	1	4.90E+04			4.90E+04	4.6E-01	1.6E+00	5.1E+00	1000	100	4.99E+04	83%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1316-T03-A	1	1.21E+05			1.21E+05	2.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1316-T04-A	1	2.05E+05			2.05E+05	3.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1316-T05-A															
K	EaFA-L01-1316-T01-B	1	2.36E+04			2.36E+04	2.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1316-T02-B	1	4.96E+04			4.96E+04	1.4E+00	1.6E+00	5.1E+00	1000	100	5.05E+04	86%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1316-T03-B	1	1.22E+05			1.22E+05	2.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1316-T04-B	1	2.14E+05			2.14E+05	7.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1316-T05-B															
K	EaFA-L01-1316-T01-C	1	2.05E+04			2.05E+04	8.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1316-T02-C	1	5.01E+04			5.01E+04	1.1E+00	1.6E+00	5.1E+00	1000	100	5.09E+04	83%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1316-T03-C	1	1.16E+05			1.16E+05	9.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1316-T04-C	1	2.00E+05			2.00E+05	3.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
K	EaFA-L01-1316-T05-C															
K	EaFA-L01-1316-B01-A	1	4.01E+00	E		4.01E+00	2.5E+01	1.6E+00	5.1E+00				---	VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	EaFA-L01-1316-T01-A	1	1.10E+03			1.10E+03	1.0E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1316-T02-A	1	1.28E+03			1.28E+03	2.9E+00	1.5E+01	4.8E+01	10	250	3.70E+03	97%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1316-T03-A	1	1.51E+03			1.51E+03	2.6E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1316-T04-A	1	2.43E+03			2.43E+03	3.6E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1316-T05-A															
Se	EaFA-L01-1316-T01-B	1	1.11E+03			1.11E+03	3.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1316-T02-B	1	1.31E+03			1.31E+03	2.8E+00	1.5E+01	4.8E+01	10	250	3.46E+03	86%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1316-T03-B	1	1.38E+03			1.38E+03	6.2E-01	1.5E+01	4.8E+01			---		VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1316-T04-B	1	2.30E+03			2.30E+03	4.7E-01	1.5E+01	4.8E+01			---		VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1316-T05-B															
Se	EaFA-L01-1316-T01-C	1	1.03E+03			1.03E+03	4.4E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1316-T02-C	1	1.43E+03			1.43E+03	3.5E+00	1.5E+01	4.8E+01	10	250	3.67E+03	90%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1316-T03-C	1	1.52E+03			1.52E+03	2.3E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1316-T04-C	1	2.33E+03			2.33E+03	1.0E+00	1.5E+01	4.8E+01			---		VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
Se	EaFA-L01-1316-T05-C															
Se	EaFA-L01-1316-B01-A	1	7.50E+00	U1/2		7.50E+00	3.1E+02	1.5E+01	4.8E+01			---		VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	EaFA-L01-1316-T01-A	1	2.97E+03			2.97E+03	7.9E-01	1.1E+00	3.5E+00			---		VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1316-T02-A	1	3.17E+03			3.17E+03	6.3E-01	1.1E+00	3.5E+00	1000	100	4.01E+03	85%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1316-T03-A	1	3.15E+03			3.15E+03	2.6E+00	1.1E+00	3.5E+00			---		VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1316-T04-A	1	2.31E+03			2.31E+03	3.2E+00	1.1E+00	3.5E+00			---		VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1316-T05-A															
Si	EaFA-L01-1316-T01-B	1	3.05E+03			3.05E+03	6.7E-01	1.1E+00	3.5E+00			---		VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1316-T02-B	1	3.08E+03			3.08E+03	9.6E-01	1.1E+00	3.5E+00	1000	100	3.95E+03	87%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1316-T03-B	1	2.78E+03			2.78E+03	4.3E-01	1.1E+00	3.5E+00			---		VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1316-T04-B	1	2.42E+03			2.42E+03	6.7E-01	1.1E+00	3.5E+00			---		VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1316-T05-B															
Si	EaFA-L01-1316-T01-C	1	2.63E+03			2.63E+03	6.8E-01	1.1E+00	3.5E+00			---		VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1316-T02-C	1	3.56E+03			3.56E+03	2.2E+00	1.1E+00	3.5E+00	1000	100	4.37E+03	81%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1316-T03-C	1	3.01E+03			3.01E+03	1.1E+00	1.1E+00	3.5E+00			---		VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1316-T04-C	1	2.57E+03			2.57E+03	4.2E-01	1.1E+00	3.5E+00			---		VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
Si	EaFA-L01-1316-T05-C															
Si	EaFA-L01-1316-B01-A	1	2.89E+01			2.89E+01	4.5E+00	1.1E+00	3.5E+00			---		VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	EaFA-L01-1316-T01-A	1	5.39E+03			5.39E+03	3.3E-01	2.5E+00	8.0E+00			---		VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1316-T02-A	1	1.13E+04			1.13E+04	5.5E-01	2.5E+00	8.0E+00	1000	100	1.22E+04	89%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1316-T03-A	1	2.82E+04			2.82E+04	2.3E+00	2.5E+00	8.0E+00			---		VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1316-T04-A	1	4.91E+04			4.91E+04	4.0E+00	2.5E+00	8.0E+00			---		VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1316-T05-A															
Na	EaFA-L01-1316-T01-B	1	5.47E+03			5.47E+03	9.9E-01	2.5E+00	8.0E+00			---		VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1316-T02-B	1	1.15E+04			1.15E+04	1.3E+00	2.5E+00	8.0E+00	1000	100	1.24E+04	87%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1316-T03-B	1	2.82E+04			2.82E+04	4.6E-01	2.5E+00	8.0E+00			---		VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1316-T04-B	1	5.03E+04			5.03E+04	6.1E-01	2.5E+00	8.0E+00			---		VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1316-T05-B															
Na	EaFA-L01-1316-T01-C	1	4.67E+03			4.67E+03	1.2E+00	2.5E+00	8.0E+00			---		VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1316-T02-C	1	1.16E+04			1.16E+04	1.0E+00	2.5E+00	8.0E+00	1000	100	1.24E+04	88%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1316-T03-C	1	2.67E+04			2.67E+04	8.7E-01	2.5E+00	8.0E+00			---		VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1316-T04-C	1	4.69E+04			4.69E+04	5.1E-01	2.5E+00	8.0E+00			---		VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
Na	EaFA-L01-1316-T05-C															
Na	EaFA-L01-1316-B01-A	1	3.64E+01			3.64E+01	2.2E+00	2.5E+00	8.0E+00			---		VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	EaFA-L01-1316-T01-A	1	2.09E+03			2.09E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1316-T02-A	1	3.97E+03			3.97E+03	1.5E+00	1.0E+00	3.2E+00	1000	100	4.89E+03	92%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1316-T03-A	1	8.54E+03			8.54E+03	3.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1316-T04-A	1	8.65E+03			8.65E+03	3.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1316-T05-A															
Sr	EaFA-L01-1316-T01-B	1	2.14E+03			2.14E+03	9.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1316-T02-B	1	3.98E+03			3.98E+03	7.3E-01	1.0E+00	3.2E+00	1000	100	4.89E+03	91%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1316-T03-B	1	8.34E+03			8.34E+03	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1316-T04-B	1	8.73E+03			8.73E+03	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1316-T05-B															
Sr	EaFA-L01-1316-T01-C	1	1.84E+03			1.84E+03	4.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1316-T02-C	1	4.09E+03			4.09E+03	2.7E+00	1.0E+00	3.2E+00	1000	100	4.95E+03	86%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1316-T03-C	1	8.15E+03			8.15E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1316-T04-C	1	8.29E+03			8.29E+03	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
Sr	EaFA-L01-1316-T05-C															
Sr	EaFA-L01-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	2.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	EaFA-L01-1316-T01-A	1	1.54E+05			1.54E+05	5.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1316-T02-A	1	3.10E+05			3.10E+05	3.0E-01	6.8E+00	2.2E+01	1000	100	3.96E+05	86%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1316-T03-A	1	7.08E+05			7.08E+05	2.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1316-T04-A	1	7.30E+05			7.30E+05	3.3E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1316-T05-A															
S	EaFA-L01-1316-T01-B	1	1.56E+05			1.56E+05	3.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1316-T02-B	1	3.13E+05			3.13E+05	7.6E-01	6.8E+00	2.2E+01	1000	100	3.96E+05	84%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1316-T03-B	1	6.98E+05			6.98E+05	2.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1316-T04-B	1	7.68E+05			7.68E+05	1.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1316-T05-B															
S	EaFA-L01-1316-T01-C	1	1.34E+05			1.34E+05	9.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1316-T02-C	1	3.09E+05			3.09E+05	1.2E+00	6.8E+00	2.2E+01	1000	100	3.95E+05	87%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1316-T03-C	1	6.62E+05			6.62E+05	9.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1316-T04-C	1	7.45E+05			7.45E+05	2.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
S	EaFA-L01-1316-T05-C															
S	EaFA-L01-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	7.4E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	EaFA-L01-1316-T01-A	1	2.30E+00	U1/2		2.30E+00	9.4E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1316-T02-A	1	2.30E+00	U1/2		2.30E+00	2.8E+02	4.6E+00	1.5E+01	10	250	2.50E+03	100%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1316-T03-A	1	1.52E+01			1.52E+01	6.6E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1316-T04-A	1	1.64E+01			1.64E+01	3.8E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1316-T05-A															
Tl	EaFA-L01-1316-T01-B	1	2.30E+00	U1/2		2.30E+00	9.0E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1316-T02-B	1	1.62E+01			1.62E+01	7.0E+01	4.6E+00	1.5E+01	10	250	2.25E+03	89%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1316-T03-B	1	7.91E+00	E		7.91E+00	4.0E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1316-T04-B	1	1.70E+01			1.70E+01	6.0E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1316-T05-B															
Tl	EaFA-L01-1316-T01-C	1	2.30E+00	U1/2		2.30E+00	2.4E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1316-T02-C	1	4.64E+00	E		4.64E+00	2.4E+02	4.6E+00	1.5E+01	10	250	2.30E+03	92%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1316-T03-C	1	2.70E+01			2.70E+01	3.9E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1316-T04-C	1	1.69E+01			1.69E+01	1.3E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
Tl	EaFA-L01-1316-T05-C															
Tl	EaFA-L01-1316-B01-A	1	2.30E+00	U1/2		2.30E+00	4.0E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	EaFA-L01-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	5.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	5.6E+01	2.0E+00	6.4E+00	10	250	2.54E+03	101%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	4.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1316-T05-A															
Ti	EaFA-L01-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	2.2E+02	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	1.2E+03	2.0E+00	6.4E+00	10	250	2.31E+03	92%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	5.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	2.9E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1316-T05-B															
Ti	EaFA-L01-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	1.5E+02	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	7.9E+01	2.0E+00	6.4E+00	10	250	2.35E+03	94%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	2.6E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	6.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
Ti	EaFA-L01-1316-T05-C															
Ti	EaFA-L01-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	1.5E+02	2.0E+00	6.4E+00			---		VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	EaFA-L01-1316-T01-A	1	2.66E+02			2.66E+02	1.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1316-T02-A	1	3.05E+02			3.05E+02	3.4E-01	1.5E+00	4.8E+00	10	250	2.80E+03	100%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1316-T03-A	1	3.63E+02			3.63E+02	2.0E+00	1.5E+00	4.8E+00			---		VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1316-T04-A	1	4.13E+02			4.13E+02	3.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1316-T05-A															
V	EaFA-L01-1316-T01-B	1	2.72E+02			2.72E+02	1.3E+00	1.5E+00	4.8E+00			---		VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1316-T02-B	1	3.09E+02			3.09E+02	1.7E+00	1.5E+00	4.8E+00	10	250	2.70E+03	96%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1316-T03-B	1	3.35E+02			3.35E+02	1.3E+00	1.5E+00	4.8E+00			---		VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1316-T04-B	1	4.23E+02			4.23E+02	1.2E+00	1.5E+00	4.8E+00			---		VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1316-T05-B															
V	EaFA-L01-1316-T01-C	1	2.49E+02			2.49E+02	6.0E-01	1.5E+00	4.8E+00			---		VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1316-T02-C	1	3.47E+02			3.47E+02	1.3E+00	1.5E+00	4.8E+00	10	250	2.62E+03	91%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1316-T03-C	1	3.61E+02			3.61E+02	1.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1316-T04-C	1	4.33E+02			4.33E+02	4.2E-01	1.5E+00	4.8E+00			---		VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
V	EaFA-L01-1316-T05-C															
V	EaFA-L01-1316-B01-A	1	7.50E-01	U1/2		7.50E-01	1.6E+01	1.5E+00	4.8E+00			---		VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	EaFA-L01-1316-T01-A	1	2.13E+01			2.13E+01	5.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/9/10 1:50 PM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1316-T02-A	1	2.58E+01			2.58E+01	2.2E+00	1.0E+00	3.2E+00	10	250	2.67E+03	106%	VU ICP-OES	6/9/10 1:51 PM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1316-T03-A	1	3.78E+01			3.78E+01	5.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/9/10 1:53 PM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1316-T04-A	1	1.26E+01			1.26E+01	6.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/9/10 1:55 PM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1316-T05-A															
Zn	EaFA-L01-1316-T01-B	1	2.39E+01			2.39E+01	2.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/9/10 2:03 PM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1316-T02-B	1	2.36E+01			2.36E+01	4.4E+00	1.0E+00	3.2E+00	10	250	2.62E+03	104%	VU ICP-OES	6/9/10 1:58 PM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1316-T03-B	1	3.15E+01			3.15E+01	1.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/9/10 2:00 PM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1316-T04-B	1	1.69E+01			1.69E+01	5.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/9/10 2:01 PM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1316-T05-B															
Zn	EaFA-L01-1316-T01-C	1	1.45E+01			1.45E+01	8.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/9/10 2:05 PM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1316-T02-C	1	2.33E+01			2.33E+01	2.7E+00	1.0E+00	3.2E+00	10	250	2.46E+03	98%	VU ICP-OES	6/9/10 2:07 PM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1316-T03-C	1	3.37E+01			3.37E+01	1.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/9/10 2:08 PM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1316-T04-C	1	1.68E+01			1.68E+01	4.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/9/10 2:10 PM	EPA Interlab L01 1313-1316 EaFA
Zn	EaFA-L01-1316-T05-C															
Zn	EaFA-L01-1316-B01-A	1	2.47E+00	E		2.47E+00	1.5E+01	1.0E+00	3.2E+00			---		VU ICP-OES	6/9/10 11:58 AM	EPA Interlab L01 1313-1316 EaFA

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	EaFa-L02-1316-T01-A	1	1.75E+02			1.75E+02	1.2E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
Al	EaFa-L02-1316-T02-A	1	2.06E+02			2.06E+02	1.2E+01	1.0E+00	3.2E+00	1000	100	1.28E+03	107%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
Al	EaFa-L02-1316-T03-A	1	2.25E+02			2.25E+02	5.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
Al	EaFa-L02-1316-T04-A	1	4.46E+02			4.46E+02	1.8E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
Al	EaFa-L02-1316-T05-A	1	3.61E+02			3.61E+02	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
Al	EaFa-L02-1316-T01-B	1	1.85E+02			1.85E+02	2.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
Al	EaFa-L02-1316-T02-B	1	2.09E+02			2.09E+02	1.9E+00	1.0E+00	3.2E+00	1000	100	1.20E+03	99%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
Al	EaFa-L02-1316-T03-B	1	2.35E+02			2.35E+02	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
Al	EaFa-L02-1316-T04-B	1	4.58E+02			4.58E+02	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
Al	EaFa-L02-1316-T05-B	1	4.31E+02			4.31E+02	2.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
Al	EaFa-L02-1316-T01-C	1	1.65E+02			1.65E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
Al	EaFa-L02-1316-T02-C	1	1.98E+02			1.98E+02	3.9E+00	1.0E+00	3.2E+00	1000	100	1.18E+03	98%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
Al	EaFa-L02-1316-T03-C	1	2.35E+02			2.35E+02	3.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
Al	EaFa-L02-1316-T04-C	1	4.42E+02			4.42E+02	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
Al	EaFa-L02-1316-T05-C	1	3.92E+02			3.92E+02	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
Al	EaFa-L02-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	4.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	EaFa-L02-1316-T01-A	1	2.06E+02			2.06E+02	1.3E+02	7.5E+00	2.4E+01			---		VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFa-L02-1316-T02-A	1	2.61E+02			2.61E+02	1.8E+01	7.5E+00	2.4E+01	10	300	3.78E+03	117%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFa-L02-1316-T03-A	1	4.25E+02			4.25E+02	5.2E+00	7.5E+00	2.4E+01			---		VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFa-L02-1316-T04-A	1	6.73E+02			6.73E+02	1.7E+02	7.5E+00	2.4E+01			---		VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFa-L02-1316-T05-A	1	5.94E+02			5.94E+02	5.9E+00	7.5E+00	2.4E+01			---		VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFa-L02-1316-T01-B	1	1.74E+02			1.74E+02	1.5E+01	7.5E+00	2.4E+01			---		VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFa-L02-1316-T02-B	1	3.47E+02			3.47E+02	5.5E+00	7.5E+00	2.4E+01	10	300	3.72E+03	112%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFa-L02-1316-T03-B	1	5.17E+02			5.17E+02	1.2E+00	7.5E+00	2.4E+01			---		VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFa-L02-1316-T04-B	1	7.26E+02			7.26E+02	2.1E+00	7.5E+00	2.4E+01			---		VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFa-L02-1316-T05-B	1	7.09E+02			7.09E+02	2.8E+00	7.5E+00	2.4E+01			---		VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFa-L02-1316-T01-C	1	2.39E+02			2.39E+02	1.7E+01	7.5E+00	2.4E+01			---		VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFa-L02-1316-T02-C	1	3.48E+02			3.48E+02	6.9E+00	7.5E+00	2.4E+01	10	300	3.64E+03	110%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFa-L02-1316-T03-C	1	5.25E+02			5.25E+02	4.2E+00	7.5E+00	2.4E+01			---		VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFa-L02-1316-T04-C	1	6.86E+02			6.86E+02	5.6E+00	7.5E+00	2.4E+01			---		VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFa-L02-1316-T05-C	1	6.25E+02			6.25E+02	2.0E+00	7.5E+00	2.4E+01			---		VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
Sb	EaFa-L02-1316-B01-A	1	3.75E+00	U1/2		3.75E+00	1.0E+04	7.5E+00	2.4E+01			---		VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	EaFa-L02-1316-T01-A	1	1.36E+02			1.36E+02	1.5E+02	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
As	EaFa-L02-1316-T02-A	1	1.13E+02			1.13E+02	3.1E+01	1.1E+01	3.5E+01	10	300	3.58E+03	115%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
As	EaFa-L02-1316-T03-A	1	1.24E+02			1.24E+02	3.8E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
As	EaFa-L02-1316-T04-A	1	1.69E+02			1.69E+02	1.9E+02	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
As	EaFa-L02-1316-T05-A	1	2.20E+02			2.20E+02	2.0E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
As	EaFa-L02-1316-T01-B	1	1.20E+02			1.20E+02	6.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
As	EaFa-L02-1316-T02-B	1	1.67E+02			1.67E+02	1.9E+01	1.1E+01	3.5E+01	10	300	3.45E+03	109%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
As	EaFa-L02-1316-T03-B	1	1.46E+02			1.46E+02	9.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
As	EaFa-L02-1316-T04-B	1	1.95E+02			1.95E+02	2.0E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
As	EaFa-L02-1316-T05-B	1	2.07E+02			2.07E+02	2.0E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
As	EaFa-L02-1316-T01-C	1	1.20E+02			1.20E+02	4.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
As	EaFa-L02-1316-T02-C	1	1.46E+02			1.46E+02	2.2E+01	1.1E+01	3.5E+01	10	300	3.44E+03	110%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
As	EaFa-L02-1316-T03-C	1	1.30E+02			1.30E+02	8.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
As	EaFa-L02-1316-T04-C	1	1.51E+02			1.51E+02	1.6E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
As	EaFa-L02-1316-T05-C	1	1.86E+02			1.86E+02	1.6E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
As	EaFa-L02-1316-B01-A	1	5.50E+00	U1/2		5.50E+00	5.7E+02	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	EaFa-L02-1316-T01-A	1	4.34E+03			4.34E+03	7.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
B	EaFa-L02-1316-T02-A	1	7.64E+03			7.64E+03	6.2E+00	1.0E+00	3.2E+00	1000	100	8.52E+03	88%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
B	EaFa-L02-1316-T03-A	1	1.76E+04			1.76E+04	5.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
B	EaFa-L02-1316-T04-A	1	3.80E+04			3.80E+04	1.3E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
B	EaFa-L02-1316-T05-A	1	3.04E+04			3.04E+04	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
B	EaFa-L02-1316-T01-B	1	5.19E+03			5.19E+03	2.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
B	EaFa-L02-1316-T02-B	1	9.49E+03			9.49E+03	1.2E+00	1.0E+00	3.2E+00	1000	100	1.04E+04	92%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
B	EaFa-L02-1316-T03-B	1	2.18E+04			2.18E+04	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
B	EaFa-L02-1316-T04-B	1	3.91E+04			3.91E+04	8.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
B	EaFa-L02-1316-T05-B	1	3.41E+04			3.41E+04	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
B	EaFa-L02-1316-T01-C	1	5.61E+03			5.61E+03	1.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
B	EaFa-L02-1316-T02-C	1	9.40E+03			9.40E+03	1.2E+00	1.0E+00	3.2E+00	1000	100	1.03E+04	89%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
B	EaFa-L02-1316-T03-C	1	2.20E+04			2.20E+04	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
B	EaFa-L02-1316-T04-C	1	3.82E+04			3.82E+04	2.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
B	EaFa-L02-1316-T05-C	1	3.15E+04			3.15E+04	6.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
B	EaFa-L02-1316-B01-A	1	4.68E+01			4.68E+01	5.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	EaFa-L02-1316-T01-A	1	2.90E+02			2.90E+02	9.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFa-L02-1316-T02-A	1	2.20E+02			2.20E+02	1.1E+01	1.0E+00	3.2E+00	10	300	3.35E+03	104%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFa-L02-1316-T03-A	1	2.14E+02			2.14E+02	5.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFa-L02-1316-T04-A	1	2.42E+02			2.42E+02	1.5E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFa-L02-1316-T05-A	1	1.85E+02			1.85E+02	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFa-L02-1316-T01-B	1	2.81E+02			2.81E+02	6.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFa-L02-1316-T02-B	1	2.79E+02			2.79E+02	9.6E-01	1.0E+00	3.2E+00	10	300	3.27E+03	100%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFa-L02-1316-T03-B	1	2.43E+02			2.43E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFa-L02-1316-T04-B	1	2.64E+02			2.64E+02	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFa-L02-1316-T05-B	1	2.26E+02			2.26E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFa-L02-1316-T01-C	1	3.31E+02			3.31E+02	3.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFa-L02-1316-T02-C	1	2.73E+02			2.73E+02	5.9E-01	1.0E+00	3.2E+00	10	300	3.23E+03	98%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFa-L02-1316-T03-C	1	2.42E+02			2.42E+02	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFa-L02-1316-T04-C	1	2.53E+02			2.53E+02	3.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFa-L02-1316-T05-C	1	2.06E+02			2.06E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
Ba	EaFa-L02-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	2.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	EaFa-L02-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
Be	EaFa-L02-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	2.6E+01	1.9E+00	6.0E+00	10	300	3.41E+03	114%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
Be	EaFa-L02-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	2.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
Be	EaFa-L02-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	4.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
Be	EaFa-L02-1316-T05-A	1	9.50E-01	U1/2		9.50E-01	4.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
Be	EaFa-L02-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	2.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
Be	EaFa-L02-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	5.5E+02	1.9E+00	6.0E+00	10	300	3.29E+03	110%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
Be	EaFa-L02-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	4.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
Be	EaFa-L02-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	4.2E+03	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
Be	EaFa-L02-1316-T05-B	1	9.50E-01	U1/2		9.50E-01	6.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
Be	EaFa-L02-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	4.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
Be	EaFa-L02-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	2.5E+02	1.9E+00	6.0E+00	10	300	3.30E+03	110%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
Be	EaFa-L02-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	6.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
Be	EaFa-L02-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	5.7E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
Be	EaFa-L02-1316-T05-C	1	9.50E-01	U1/2		9.50E-01	6.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
Be	EaFa-L02-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	4.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	EaFa-L02-1316-T01-A	1	1.10E+00	U1/2		1.10E+00	3.6E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFa-L02-1316-T02-A	1	1.10E+00	U1/2		1.10E+00	7.4E+02	2.2E+00	7.0E+00	10	300	3.47E+03	116%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFa-L02-1316-T03-A	1	3.11E+00	E		3.11E+00	7.4E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFa-L02-1316-T04-A	1	1.10E+00	U1/2		1.10E+00	1.3E+02	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFa-L02-1316-T05-A	1	1.10E+00	U1/2		1.10E+00	1.1E+02	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFa-L02-1316-T01-B	1	1.10E+00	U1/2		1.10E+00	7.9E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFa-L02-1316-T02-B	1	1.10E+00	U1/2		1.10E+00	6.1E+01	2.2E+00	7.0E+00	10	300	3.37E+03	112%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFa-L02-1316-T03-B	1	7.89E+00			7.89E+00	4.9E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFa-L02-1316-T04-B	1	2.84E+00	E		2.84E+00	1.3E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFa-L02-1316-T05-B	1	1.10E+00	U1/2		1.10E+00	9.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFa-L02-1316-T01-C	1	1.10E+00	U1/2		1.10E+00	8.6E+02	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFa-L02-1316-T02-C	1	1.10E+00	U1/2		1.10E+00	1.5E+02	2.2E+00	7.0E+00	10	300	3.33E+03	111%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFa-L02-1316-T03-C	1	7.62E+00			7.62E+00	8.6E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFa-L02-1316-T04-C	1	3.28E+00	E		3.28E+00	2.3E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFa-L02-1316-T05-C	1	1.10E+00	U1/2		1.10E+00	1.1E+02	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
Cd	EaFa-L02-1316-B01-A	1	1.10E+00	U1/2		1.10E+00	1.1E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	EaFa-L02-1316-T01-A	1	1.66E+05			1.66E+05	8.7E+01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFa-L02-1316-T02-A	1	2.94E+05			2.94E+05	1.1E+01	2.6E+00	8.3E+00	1000	100	2.95E+05	91%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFa-L02-1316-T03-A	1	6.46E+05			6.46E+05	5.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFa-L02-1316-T04-A	1	5.95E+05			5.95E+05	1.5E+02	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFa-L02-1316-T05-A	1	6.70E+05			6.70E+05	1.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFa-L02-1316-T01-B	1	1.81E+05			1.81E+05	6.8E+01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFa-L02-1316-T02-B	1	3.57E+05			3.57E+05	1.2E+00	2.6E+00	8.3E+00	1000	100	3.58E+05	85%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFa-L02-1316-T03-B	1	7.75E+05			7.75E+05	6.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFa-L02-1316-T04-B	1	6.12E+05			6.12E+05	7.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFa-L02-1316-T05-B	1	6.64E+05			6.64E+05	1.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFa-L02-1316-T01-C	1	1.78E+05			1.78E+05	2.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFa-L02-1316-T02-C	1	3.47E+05			3.47E+05	4.9E-01	2.6E+00	8.3E+00	1000	100	3.48E+05	87%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFa-L02-1316-T03-C	1	7.74E+05			7.74E+05	1.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFa-L02-1316-T04-C	1	5.91E+05			5.91E+05	7.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFa-L02-1316-T05-C	1	6.04E+05			6.04E+05	6.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
Ca	EaFa-L02-1316-B01-A	1	1.30E+00	U1/2		1.30E+00	7.9E+01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	EaFa-L02-1316-T01-A	1	1.71E+01			1.71E+01	1.1E+02	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFa-L02-1316-T02-A	1	1.90E+01			1.90E+01	1.4E+01	1.2E+00	3.8E+00	10	300	3.28E+03	109%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFa-L02-1316-T03-A	1	1.85E+01			1.85E+01	6.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFa-L02-1316-T04-A	1	3.60E+01			3.60E+01	1.8E+02	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFa-L02-1316-T05-A	1	4.35E+01			4.35E+01	3.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFa-L02-1316-T01-B	1	1.68E+01			1.68E+01	2.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFa-L02-1316-T02-B	1	1.94E+01			1.94E+01	4.8E+00	1.2E+00	3.8E+00	10	300	3.18E+03	105%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFa-L02-1316-T03-B	1	1.86E+01			1.86E+01	3.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFa-L02-1316-T04-B	1	4.27E+01			4.27E+01	2.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFa-L02-1316-T05-B	1	4.92E+01			4.92E+01	3.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFa-L02-1316-T01-C	1	1.47E+01			1.47E+01	7.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFa-L02-1316-T02-C	1	1.86E+01			1.86E+01	1.4E+01	1.2E+00	3.8E+00	10	300	3.37E+03	112%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFa-L02-1316-T03-C	1	1.86E+01			1.86E+01	7.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFa-L02-1316-T04-C	1	4.16E+01			4.16E+01	4.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFa-L02-1316-T05-C	1	4.37E+01			4.37E+01	2.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
Cr	EaFa-L02-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	1.9E+02	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	EaFa-L02-1316-T01-A	1	3.76E+01			3.76E+01	1.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
Co	EaFa-L02-1316-T02-A	1	5.36E+01			5.36E+01	1.1E+01	1.8E+00	5.7E+00	10	300	3.39E+03	111%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
Co	EaFa-L02-1316-T03-A	1	1.89E+02			1.89E+02	7.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
Co	EaFa-L02-1316-T04-A	1	1.60E+02			1.60E+02	1.7E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
Co	EaFa-L02-1316-T05-A	1	1.01E+02			1.01E+02	4.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
Co	EaFa-L02-1316-T01-B	1	3.61E+01			3.61E+01	1.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
Co	EaFa-L02-1316-T02-B	1	1.02E+02			1.02E+02	3.1E+00	1.8E+00	5.7E+00	10	300	3.31E+03	107%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
Co	EaFa-L02-1316-T03-B	1	2.96E+02			2.96E+02	1.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
Co	EaFa-L02-1316-T04-B	1	1.79E+02			1.79E+02	2.9E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
Co	EaFa-L02-1316-T05-B	1	1.19E+02			1.19E+02	3.9E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
Co	EaFa-L02-1316-T01-C	1	5.16E+01			5.16E+01	5.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
Co	EaFa-L02-1316-T02-C	1	1.03E+02			1.03E+02	2.6E+00	1.8E+00	5.7E+00	10	300	3.39E+03	110%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
Co	EaFa-L02-1316-T03-C	1	2.94E+02			2.94E+02	2.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
Co	EaFa-L02-1316-T04-C	1	1.72E+02			1.72E+02	2.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
Co	EaFa-L02-1316-T05-C	1	1.07E+02			1.07E+02	3.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
Co	EaFa-L02-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	2.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	EaFa-L02-1316-T01-A	1	1.01E+01	E		1.01E+01	1.1E+02	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFa-L02-1316-T02-A	1	1.49E+01			1.49E+01	5.6E+01	3.7E+00	1.2E+01	10	300	3.31E+03	110%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFa-L02-1316-T03-A	1	2.30E+01			2.30E+01	3.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFa-L02-1316-T04-A	1	1.71E+01			1.71E+01	3.2E+02	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFa-L02-1316-T05-A	1	1.64E+01			1.64E+01	2.6E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFa-L02-1316-T01-B	1	1.74E+01			1.74E+01	5.6E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFa-L02-1316-T02-B	1	1.41E+01			1.41E+01	2.2E+01	3.7E+00	1.2E+01	10	300	3.20E+03	106%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFa-L02-1316-T03-B	1	1.51E+01			1.51E+01	9.7E+00	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFa-L02-1316-T04-B	1	1.47E+01			1.47E+01	4.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFa-L02-1316-T05-B	1	1.32E+01			1.32E+01	8.2E+00	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFa-L02-1316-T01-C	1	8.90E+00	E		8.90E+00	2.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFa-L02-1316-T02-C	1	9.23E+00	E		9.23E+00	4.8E+01	3.7E+00	1.2E+01	10	300	3.39E+03	113%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFa-L02-1316-T03-C	1	1.33E+01			1.33E+01	2.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFa-L02-1316-T04-C	1	1.32E+01			1.32E+01	4.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFa-L02-1316-T05-C	1	1.16E+01	E		1.16E+01	7.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
Cu	EaFa-L02-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	1.1E+02	3.7E+00	1.2E+01			---		VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	EaFa-L02-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFa-L02-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	6.6E+00	2.0E+00	6.4E+00	1000	100	1.02E+03	101%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFa-L02-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	3.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFa-L02-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFa-L02-1316-T05-A	1	1.00E+00	U1/2		1.00E+00	1.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFa-L02-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	3.9E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFa-L02-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00	1000	100	9.83E+02	98%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFa-L02-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	9.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFa-L02-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFa-L02-1316-T05-B	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFa-L02-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFa-L02-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	7.8E+00	2.0E+00	6.4E+00	1000	100	1.04E+03	104%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFa-L02-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	1.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFa-L02-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFa-L02-1316-T05-C	1	1.00E+00	U1/2		1.00E+00	9.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
Fe	EaFa-L02-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	EaFa-L02-1316-T01-A	1	3.40E+00	U1/2		3.40E+00	3.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFa-L02-1316-T02-A	1	3.40E+00	U1/2		3.40E+00	7.6E+01	6.8E+00	2.2E+01	10	300	3.24E+03	108%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFa-L02-1316-T03-A	1	3.40E+00	U1/2		3.40E+00	3.0E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFa-L02-1316-T04-A	1	3.40E+00	U1/2		3.40E+00	2.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFa-L02-1316-T05-A	1	3.40E+00	U1/2		3.40E+00	1.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFa-L02-1316-T01-B	1	3.40E+00	U1/2		3.40E+00	2.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFa-L02-1316-T02-B	1	3.40E+00	U1/2		3.40E+00	1.0E+02	6.8E+00	2.2E+01	10	300	3.17E+03	106%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFa-L02-1316-T03-B	1	3.40E+00	U1/2		3.40E+00	5.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFa-L02-1316-T04-B	1	3.40E+00	U1/2		3.40E+00	2.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFa-L02-1316-T05-B	1	3.40E+00	U1/2		3.40E+00	5.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFa-L02-1316-T01-C	1	3.40E+00	U1/2		3.40E+00	1.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFa-L02-1316-T02-C	1	3.40E+00	U1/2		3.40E+00	8.8E+01	6.8E+00	2.2E+01	10	300	3.12E+03	104%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFa-L02-1316-T03-C	1	3.40E+00	U1/2		3.40E+00	4.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFa-L02-1316-T04-C	1	3.40E+00	U1/2		3.40E+00	2.4E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFa-L02-1316-T05-C	1	3.40E+00	U1/2		3.40E+00	2.3E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
Pb	EaFa-L02-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	1.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	EaFa-L02-1316-T01-A	1	3.55E+03			3.55E+03	1.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
Li	EaFa-L02-1316-T02-A	1	5.91E+03			5.91E+03	1.1E+01	1.9E+00	6.0E+00	10	300	8.94E+03	101%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
Li	EaFa-L02-1316-T03-A	1	1.40E+04			1.40E+04	4.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
Li	EaFa-L02-1316-T04-A	1	3.25E+04			3.25E+04	1.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
Li	EaFa-L02-1316-T05-A	1	2.76E+04			2.76E+04	2.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
Li	EaFa-L02-1316-T01-B	1	3.92E+03			3.92E+03	9.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
Li	EaFa-L02-1316-T02-B	1	9.05E+03			9.05E+03	9.4E-01	1.9E+00	6.0E+00	10	300	1.18E+04	93%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
Li	EaFa-L02-1316-T03-B	1	2.05E+04			2.05E+04	9.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
Li	EaFa-L02-1316-T04-B	1	4.03E+04			4.03E+04	4.6E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
Li	EaFa-L02-1316-T05-B	1	3.36E+04			3.36E+04	1.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
Li	EaFa-L02-1316-T01-C	1	4.59E+03			4.59E+03	2.9E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
Li	EaFa-L02-1316-T02-C	1	8.76E+03			8.76E+03	3.0E-01	1.9E+00	6.0E+00	10	300	1.17E+04	96%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
Li	EaFa-L02-1316-T03-C	1	2.06E+04			2.06E+04	1.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
Li	EaFa-L02-1316-T04-C	1	3.90E+04			3.90E+04	9.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
Li	EaFa-L02-1316-T05-C	1	3.07E+04			3.07E+04	3.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
Li	EaFa-L02-1316-B01-A	1	8.32E+00			8.32E+00	1.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	EaFa-L02-1316-T01-A	1	3.37E+02			3.37E+02	7.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFa-L02-1316-T02-A	1	5.06E+02			5.06E+02	9.2E+00	2.0E+00	6.4E+00	10	300	3.74E+03	108%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFa-L02-1316-T03-A	1	1.35E+03			1.35E+03	3.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFa-L02-1316-T04-A	1	1.61E+03			1.61E+03	1.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFa-L02-1316-T05-A	1	1.01E+03			1.01E+03	6.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFa-L02-1316-T01-B	1	3.30E+02			3.30E+02	6.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFa-L02-1316-T02-B	1	7.66E+02			7.66E+02	1.4E+00	2.0E+00	6.4E+00	10	300	3.75E+03	100%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFa-L02-1316-T03-B	1	1.92E+03			1.92E+03	7.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFa-L02-1316-T04-B	1	1.68E+03			1.68E+03	5.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFa-L02-1316-T05-B	1	1.11E+03			1.11E+03	1.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFa-L02-1316-T01-C	1	4.11E+02			4.11E+02	7.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFa-L02-1316-T02-C	1	7.48E+02			7.48E+02	5.9E-01	2.0E+00	6.4E+00	10	300	3.75E+03	100%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFa-L02-1316-T03-C	1	1.92E+03			1.92E+03	6.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFa-L02-1316-T04-C	1	1.63E+03			1.63E+03	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFa-L02-1316-T05-C	1	1.03E+03			1.03E+03	1.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
Mn	EaFa-L02-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	9.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	EaFa-L02-1316-T01-A	1	7.33E+03			7.33E+03	9.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFa-L02-1316-T02-A	1	1.25E+04			1.25E+04	1.1E+01	1.0E+00	3.2E+00	1000	100	1.36E+04	113%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFa-L02-1316-T03-A	1	3.17E+04			3.17E+04	6.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFa-L02-1316-T04-A	1	7.13E+04			7.13E+04	1.5E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFa-L02-1316-T05-A	1	6.46E+04			6.46E+04	9.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFa-L02-1316-T01-B	1	7.61E+03			7.61E+03	6.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFa-L02-1316-T02-B	1	1.57E+04			1.57E+04	3.8E-01	1.0E+00	3.2E+00	1000	100	1.67E+04	101%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFa-L02-1316-T03-B	1	3.84E+04			3.84E+04	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFa-L02-1316-T04-B	1	7.10E+04			7.10E+04	7.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFa-L02-1316-T05-B	1	6.23E+04			6.23E+04	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFa-L02-1316-T01-C	1	7.83E+03			7.83E+03	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFa-L02-1316-T02-C	1	1.51E+04			1.51E+04	9.5E-01	1.0E+00	3.2E+00	1000	100	1.61E+04	99%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFa-L02-1316-T03-C	1	3.80E+04			3.80E+04	9.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFa-L02-1316-T04-C	1	6.85E+04			6.85E+04	4.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFa-L02-1316-T05-C	1	5.76E+04			5.76E+04	5.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
Mg	EaFa-L02-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	EaFa-L02-1316-T01-A	1	3.43E+03			3.43E+03	7.8E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFa-L02-1316-T02-A	1	5.77E+03			5.77E+03	1.1E+01	1.2E+00	3.8E+00	10	300	9.08E+03	110%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFa-L02-1316-T03-A	1	1.18E+04			1.18E+04	4.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFa-L02-1316-T04-A	1	2.72E+04			2.72E+04	1.4E+02	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFa-L02-1316-T05-A	1	2.50E+04			2.50E+04	4.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFa-L02-1316-T01-B	1	3.32E+03			3.32E+03	6.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFa-L02-1316-T02-B	1	7.27E+03			7.27E+03	6.5E-01	1.2E+00	3.8E+00	10	300	1.00E+04	92%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFa-L02-1316-T03-B	1	1.44E+04			1.44E+04	1.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFa-L02-1316-T04-B	1	2.94E+04			2.94E+04	3.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFa-L02-1316-T05-B	1	2.81E+04			2.81E+04	1.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFa-L02-1316-T01-C	1	3.68E+03			3.68E+03	2.4E-02	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFa-L02-1316-T02-C	1	6.95E+03			6.95E+03	3.9E-01	1.2E+00	3.8E+00	10	300	9.94E+03	100%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFa-L02-1316-T03-C	1	1.43E+04			1.43E+04	1.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFa-L02-1316-T04-C	1	2.83E+04			2.83E+04	4.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFa-L02-1316-T05-C	1	2.55E+04			2.55E+04	1.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
Mo	EaFa-L02-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	3.5E+03	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	EaFa-L02-1316-T01-A	1	1.03E+02			1.03E+02	1.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFa-L02-1316-T02-A	1	1.38E+02			1.38E+02	9.5E+00	1.8E+00	5.7E+00	10	300	3.51E+03	113%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFa-L02-1316-T03-A	1	4.36E+02			4.36E+02	4.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFa-L02-1316-T04-A	1	3.78E+02			3.78E+02	1.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFa-L02-1316-T05-A	1	2.52E+02			2.52E+02	1.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFa-L02-1316-T01-B	1	9.75E+01			9.75E+01	3.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFa-L02-1316-T02-B	1	2.51E+02			2.51E+02	2.3E+00	1.8E+00	5.7E+00	10	300	3.44E+03	106%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFa-L02-1316-T03-B	1	6.71E+02			6.71E+02	6.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFa-L02-1316-T04-B	1	4.28E+02			4.28E+02	1.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFa-L02-1316-T05-B	1	2.83E+02			2.83E+02	2.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFa-L02-1316-T01-C	1	1.35E+02			1.35E+02	3.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFa-L02-1316-T02-C	1	2.40E+02			2.40E+02	1.3E+00	1.8E+00	5.7E+00	10	300	3.54E+03	110%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFa-L02-1316-T03-C	1	6.75E+02			6.75E+02	3.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFa-L02-1316-T04-C	1	4.18E+02			4.18E+02	2.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFa-L02-1316-T05-C	1	2.58E+02			2.58E+02	1.9E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
Ni	EaFa-L02-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	1.2E+03	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	EaFa-L02-1316-T01-A	1	4.74E+01			4.74E+01	3.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
P	EaFa-L02-1316-T02-A	1	6.39E+01			6.39E+01	2.1E+01	3.7E+00	1.2E+01	1000	100	1.12E+03	105%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
P	EaFa-L02-1316-T03-A	1	6.73E+01			6.73E+01	8.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
P	EaFa-L02-1316-T04-A	1	4.44E+02			4.44E+02	8.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
P	EaFa-L02-1316-T05-A	1	1.30E+02			1.30E+02	1.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
P	EaFa-L02-1316-T01-B	1	5.81E+01			5.81E+01	3.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
P	EaFa-L02-1316-T02-B	1	7.74E+01			7.74E+01	1.8E+01	3.7E+00	1.2E+01	1000	100	1.08E+03	100%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
P	EaFa-L02-1316-T03-B	1	1.19E+02			1.19E+02	2.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
P	EaFa-L02-1316-T04-B	1	5.31E+02			5.31E+02	6.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
P	EaFa-L02-1316-T05-B	1	1.16E+02			1.16E+02	6.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
P	EaFa-L02-1316-T01-C	1	7.17E+01			7.17E+01	1.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
P	EaFa-L02-1316-T02-C	1	8.23E+01			8.23E+01	1.4E+01	3.7E+00	1.2E+01	1000	100	1.09E+03	100%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
P	EaFa-L02-1316-T03-C	1	2.46E+02			2.46E+02	4.2E-01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
P	EaFa-L02-1316-T04-C	1	5.67E+02			5.67E+02	3.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
P	EaFa-L02-1316-T05-C	1	1.49E+02			1.49E+02	1.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
P	EaFa-L02-1316-B01-A	1	1.99E+01			1.99E+01	1.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	EaFa-L02-1316-T01-A	1	2.62E+04			2.62E+04	1.0E+02	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
K	EaFa-L02-1316-T02-A	1	4.68E+04			4.68E+04	1.2E+01	1.6E+00	5.1E+00	1000	100	4.76E+04	88%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
K	EaFa-L02-1316-T03-A	1	1.17E+05			1.17E+05	5.5E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
K	EaFa-L02-1316-T04-A	1	2.12E+05			2.12E+05	1.5E+02	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
K	EaFa-L02-1316-T05-A	1	2.05E+05			2.05E+05	1.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
K	EaFa-L02-1316-T01-B	1	3.02E+04			3.02E+04	9.2E+01	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
K	EaFa-L02-1316-T02-B	1	5.55E+04			5.55E+04	1.1E+00	1.6E+00	5.1E+00	1000	100	5.63E+04	85%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
K	EaFa-L02-1316-T03-B	1	1.31E+05			1.31E+05	1.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
K	EaFa-L02-1316-T04-B	1	2.04E+05			2.04E+05	5.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
K	EaFa-L02-1316-T05-B	1	1.88E+05			1.88E+05	2.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
K	EaFa-L02-1316-T01-C	1	2.66E+04			2.66E+04	9.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
K	EaFa-L02-1316-T02-C	1	5.36E+04			5.36E+04	4.0E-01	1.6E+00	5.1E+00	1000	100	5.45E+04	85%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
K	EaFa-L02-1316-T03-C	1	1.32E+05			1.32E+05	1.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
K	EaFa-L02-1316-T04-C	1	1.98E+05			1.98E+05	9.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
K	EaFa-L02-1316-T05-C	1	1.73E+05			1.73E+05	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
K	EaFa-L02-1316-B01-A	1	9.47E+00			9.47E+00	3.2E+01	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	EaFa-L02-1316-T01-A	1	1.18E+03			1.18E+03	9.9E+01	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
Se	EaFa-L02-1316-T02-A	1	1.24E+03			1.24E+03	1.2E+01	1.5E+01	4.8E+01	10	300	4.83E+03	120%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
Se	EaFa-L02-1316-T03-A	1	1.46E+03			1.46E+03	8.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
Se	EaFa-L02-1316-T04-A	1	2.22E+03			2.22E+03	1.6E+02	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
Se	EaFa-L02-1316-T05-A	1	2.56E+03			2.56E+03	3.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
Se	EaFa-L02-1316-T01-B	1	1.18E+03			1.18E+03	1.1E+03	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
Se	EaFa-L02-1316-T02-B	1	1.54E+03			1.54E+03	2.1E+00	1.5E+01	4.8E+01	10	300	4.60E+03	102%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
Se	EaFa-L02-1316-T03-B	1	1.63E+03			1.63E+03	3.6E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
Se	EaFa-L02-1316-T04-B	1	2.42E+03			2.42E+03	2.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
Se	EaFa-L02-1316-T05-B	1	2.72E+03			2.72E+03	3.0E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
Se	EaFa-L02-1316-T01-C	1	1.21E+03			1.21E+03	3.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
Se	EaFa-L02-1316-T02-C	1	1.46E+03			1.46E+03	1.6E+00	1.5E+01	4.8E+01	10	300	4.52E+03	102%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
Se	EaFa-L02-1316-T03-C	1	1.65E+03			1.65E+03	3.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
Se	EaFa-L02-1316-T04-C	1	2.33E+03			2.33E+03	3.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
Se	EaFa-L02-1316-T05-C	1	2.53E+03			2.53E+03	1.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
Se	EaFa-L02-1316-B01-A	1	7.50E+00	U1/2		7.50E+00	1.5E+02	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	EaFa-L02-1316-T01-A	1	2.37E+03			2.37E+03	8.1E+01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
Si	EaFa-L02-1316-T02-A	1	2.04E+03			2.04E+03	1.0E+01	1.1E+00	3.5E+00	1000	100	3.20E+03	116%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
Si	EaFa-L02-1316-T03-A	1	3.02E+03			3.02E+03	5.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
Si	EaFa-L02-1316-T04-A	1	2.67E+03			2.67E+03	1.5E+02	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
Si	EaFa-L02-1316-T05-A	1	2.31E+03			2.31E+03	2.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
Si	EaFa-L02-1316-T01-B	1	2.28E+03			2.28E+03	8.0E+01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
Si	EaFa-L02-1316-T02-B	1	3.15E+03			3.15E+03	9.0E-01	1.1E+00	3.5E+00	1000	100	4.16E+03	100%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
Si	EaFa-L02-1316-T03-B	1	3.83E+03			3.83E+03	8.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
Si	EaFa-L02-1316-T04-B	1	2.85E+03			2.85E+03	6.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
Si	EaFa-L02-1316-T05-B	1	2.60E+03			2.60E+03	1.6E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
Si	EaFa-L02-1316-T01-C	1	2.77E+03			2.77E+03	9.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
Si	EaFa-L02-1316-T02-C	1	3.00E+03			3.00E+03	7.0E-01	1.1E+00	3.5E+00	1000	100	4.13E+03	114%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
Si	EaFa-L02-1316-T03-C	1	3.82E+03			3.82E+03	1.8E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
Si	EaFa-L02-1316-T04-C	1	2.75E+03			2.75E+03	9.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
Si	EaFa-L02-1316-T05-C	1	2.37E+03			2.37E+03	6.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
Si	EaFa-L02-1316-B01-A	1	5.50E-01	U1/2		5.50E-01	4.1E+01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	EaFa-L02-1316-T01-A	1	5.56E+03			5.56E+03	1.0E+02	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
Na	EaFa-L02-1316-T02-A	1	9.77E+03			9.77E+03	1.1E+01	2.5E+00	8.0E+00	1000	100	1.08E+04	100%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
Na	EaFa-L02-1316-T03-A	1	2.47E+04			2.47E+04	5.7E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
Na	EaFa-L02-1316-T04-A	1	4.75E+04			4.75E+04	1.5E+02	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
Na	EaFa-L02-1316-T05-A	1	4.45E+04			4.45E+04	1.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
Na	EaFa-L02-1316-T01-B	1	6.34E+03			6.34E+03	7.0E+01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
Na	EaFa-L02-1316-T02-B	1	1.29E+04			1.29E+04	1.2E+00	2.5E+00	8.0E+00	1000	100	1.38E+04	93%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
Na	EaFa-L02-1316-T03-B	1	3.09E+04			3.09E+04	5.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
Na	EaFa-L02-1316-T04-B	1	5.12E+04			5.12E+04	1.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
Na	EaFa-L02-1316-T05-B	1	4.46E+04			4.46E+04	9.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
Na	EaFa-L02-1316-T01-C	1	6.12E+03			6.12E+03	3.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
Na	EaFa-L02-1316-T02-C	1	1.25E+04			1.25E+04	5.6E-01	2.5E+00	8.0E+00	1000	100	1.34E+04	96%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
Na	EaFa-L02-1316-T03-C	1	3.10E+04			3.10E+04	1.7E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
Na	EaFa-L02-1316-T04-C	1	4.93E+04			4.93E+04	3.0E-02	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
Na	EaFa-L02-1316-T05-C	1	4.06E+04			4.06E+04	1.8E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
Na	EaFa-L02-1316-B01-A	1	1.25E+00	U1/2		1.25E+00	1.6E+02	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	EaFa-L02-1316-T01-A	1	2.26E+03			2.26E+03	7.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFa-L02-1316-T02-A	1	3.75E+03			3.75E+03	9.1E+00	1.0E+00	3.2E+00	1000	100	4.81E+03	106%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFa-L02-1316-T03-A	1	7.74E+03			7.74E+03	4.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFa-L02-1316-T04-A	1	8.33E+03			8.33E+03	1.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFa-L02-1316-T05-A	1	9.55E+03			9.55E+03	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFa-L02-1316-T01-B	1	2.32E+03			2.32E+03	6.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFa-L02-1316-T02-B	1	4.57E+03			4.57E+03	1.5E+00	1.0E+00	3.2E+00	1000	100	5.64E+03	107%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFa-L02-1316-T03-B	1	9.07E+03			9.07E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFa-L02-1316-T04-B	1	8.57E+03			8.57E+03	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFa-L02-1316-T05-B	1	1.00E+04			1.00E+04	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFa-L02-1316-T01-C	1	2.45E+03			2.45E+03	4.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFa-L02-1316-T02-C	1	4.42E+03			4.42E+03	9.3E-01	1.0E+00	3.2E+00	1000	100	5.55E+03	112%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFa-L02-1316-T03-C	1	9.08E+03			9.08E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFa-L02-1316-T04-C	1	8.26E+03			8.26E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFa-L02-1316-T05-C	1	9.30E+03			9.30E+03	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
Sr	EaFa-L02-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	2.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	EaFa-L02-1316-T01-A	1	1.68E+05			1.68E+05	9.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
S	EaFa-L02-1316-T02-A	1	2.91E+05			2.91E+05	1.1E+01	6.8E+00	2.2E+01	1000	100	3.83E+05	92%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
S	EaFa-L02-1316-T03-A	1	6.62E+05			6.62E+05	4.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
S	EaFa-L02-1316-T04-A	1	8.17E+05			8.17E+05	1.5E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
S	EaFa-L02-1316-T05-A	1	8.73E+05			8.73E+05	8.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
S	EaFa-L02-1316-T01-B	1	1.75E+05			1.75E+05	6.7E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
S	EaFa-L02-1316-T02-B	1	3.69E+05			3.69E+05	8.8E-01	6.8E+00	2.2E+01	1000	100	4.58E+05	89%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
S	EaFa-L02-1316-T03-B	1	8.15E+05			8.15E+05	1.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
S	EaFa-L02-1316-T04-B	1	8.49E+05			8.49E+05	2.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
S	EaFa-L02-1316-T05-B	1	8.80E+05			8.80E+05	2.3E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
S	EaFa-L02-1316-T01-C	1	1.84E+05			1.84E+05	7.4E-02	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
S	EaFa-L02-1316-T02-C	1	3.54E+05			3.54E+05	2.6E-01	6.8E+00	2.2E+01	1000	100	4.52E+05	97%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
S	EaFa-L02-1316-T03-C	1	8.25E+05			8.25E+05	2.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
S	EaFa-L02-1316-T04-C	1	8.25E+05			8.25E+05	6.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
S	EaFa-L02-1316-T05-C	1	8.12E+05			8.12E+05	6.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
S	EaFa-L02-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	3.0E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

TI	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	EaFa-L02-1316-T01-A	1	2.30E+00	U1/2		2.30E+00	1.5E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFa-L02-1316-T02-A	1	2.30E+00	U1/2		2.30E+00	2.4E+02	4.6E+00	1.5E+01	10	300	3.23E+03	107%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFa-L02-1316-T03-A	1	2.17E+01			2.17E+01	2.8E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFa-L02-1316-T04-A	1	2.69E+01			2.69E+01	3.8E+03	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFa-L02-1316-T05-A	1	2.09E+01			2.09E+01	7.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFa-L02-1316-T01-B	1	2.30E+00	U1/2		2.30E+00	1.4E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFa-L02-1316-T02-B	1	2.21E+01			2.21E+01	2.5E+01	4.6E+00	1.5E+01	10	300	3.17E+03	105%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFa-L02-1316-T03-B	1	2.28E+01			2.28E+01	2.0E+00	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFa-L02-1316-T04-B	1	2.96E+01			2.96E+01	5.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFa-L02-1316-T05-B	1	4.11E+01			4.11E+01	2.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFa-L02-1316-T01-C	1	2.30E+00	U1/2		2.30E+00	5.4E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFa-L02-1316-T02-C	1	2.67E+01			2.67E+01	3.7E+01	4.6E+00	1.5E+01	10	300	3.14E+03	104%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFa-L02-1316-T03-C	1	3.32E+01			3.32E+01	3.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFa-L02-1316-T04-C	1	3.84E+01			3.84E+01	1.4E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFa-L02-1316-T05-C	1	2.23E+01			2.23E+01	8.5E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
Tl	EaFa-L02-1316-B01-A	1	2.30E+00	U1/2		2.30E+00	5.5E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	EaFa-L02-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFa-L02-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	2.2E+02	2.0E+00	6.4E+00	10	300	3.27E+03	109%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFa-L02-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	3.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFa-L02-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	3.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFa-L02-1316-T05-A	1	1.00E+00	U1/2		1.00E+00	9.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFa-L02-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	1.6E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFa-L02-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	1.9E+02	2.0E+00	6.4E+00	10	300	3.20E+03	107%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFa-L02-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	4.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFa-L02-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	2.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFa-L02-1316-T05-B	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFa-L02-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	2.7E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFa-L02-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00	10	300	3.17E+03	106%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFa-L02-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	4.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFa-L02-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	6.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFa-L02-1316-T05-C	1	1.00E+00	U1/2		1.00E+00	4.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
Ti	EaFa-L02-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	2.7E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	EaFa-L02-1316-T01-A	1	2.86E+02			2.86E+02	9.3E+01	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
V	EaFa-L02-1316-T02-A	1	2.65E+02			2.65E+02	1.0E+01	1.5E+00	4.8E+00	10	300	3.63E+03	112%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
V	EaFa-L02-1316-T03-A	1	3.36E+02			3.36E+02	5.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
V	EaFa-L02-1316-T04-A	1	3.97E+02			3.97E+02	1.4E+02	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
V	EaFa-L02-1316-T05-A	1	3.94E+02			3.94E+02	2.2E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
V	EaFa-L02-1316-T01-B	1	2.72E+02			2.72E+02	6.8E+01	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
V	EaFa-L02-1316-T02-B	1	3.58E+02			3.58E+02	1.8E+00	1.5E+00	4.8E+00	10	300	3.52E+03	105%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
V	EaFa-L02-1316-T03-B	1	3.90E+02			3.90E+02	1.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
V	EaFa-L02-1316-T04-B	1	4.35E+02			4.35E+02	7.4E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
V	EaFa-L02-1316-T05-B	1	4.39E+02			4.39E+02	2.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
V	EaFa-L02-1316-T01-C	1	2.88E+02			2.88E+02	1.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
V	EaFa-L02-1316-T02-C	1	3.31E+02			3.31E+02	9.9E-01	1.5E+00	4.8E+00	10	300	3.48E+03	105%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
V	EaFa-L02-1316-T03-C	1	3.87E+02			3.87E+02	2.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
V	EaFa-L02-1316-T04-C	1	4.07E+02			4.07E+02	6.4E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
V	EaFa-L02-1316-T05-C	1	4.05E+02			4.05E+02	1.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
V	EaFa-L02-1316-B01-A	1	1.63E+00	E		1.63E+00	1.2E+02	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	EaFa-L02-1316-T01-A	1	1.96E+01			1.96E+01	9.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:25 PM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFa-L02-1316-T02-A	1	1.95E+01			1.95E+01	8.7E+00	1.0E+00	3.2E+00	10	300	3.45E+03	114%	VU ICP-OES	6/4/10 4:27 PM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFa-L02-1316-T03-A	1	3.21E+01			3.21E+01	8.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:29 PM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFa-L02-1316-T04-A	1	2.88E+01			2.88E+01	1.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:30 PM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFa-L02-1316-T05-A	1	2.18E+01			2.18E+01	3.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:32 PM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFa-L02-1316-T01-B	1	9.32E+00			9.32E+00	2.9E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:33 PM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFa-L02-1316-T02-B	1	2.27E+01			2.27E+01	2.8E+00	1.0E+00	3.2E+00	10	300	3.34E+03	111%	VU ICP-OES	6/4/10 12:01 PM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFa-L02-1316-T03-B	1	5.91E+01			5.91E+01	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:03 PM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFa-L02-1316-T04-B	1	3.56E+01			3.56E+01	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:04 PM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFa-L02-1316-T05-B	1	3.17E+01			3.17E+01	4.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:06 PM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFa-L02-1316-T01-C	1	1.42E+01			1.42E+01	6.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:08 PM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFa-L02-1316-T02-C	1	2.08E+01			2.08E+01	4.2E+00	1.0E+00	3.2E+00	10	300	3.35E+03	111%	VU ICP-OES	6/4/10 12:09 PM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFa-L02-1316-T03-C	1	6.14E+01			6.14E+01	4.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:11 PM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFa-L02-1316-T04-C	1	3.37E+01			3.37E+01	2.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:13 PM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFa-L02-1316-T05-C	1	2.30E+01			2.30E+01	5.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 12:14 PM	EPA Interlab L02 1313-1316 EaFA
Zn	EaFa-L02-1316-B01-A	1	1.15E+00	E		1.15E+00	7.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 11:46 AM	EPA Interlab L02 1313-1316 EaFA

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	EaFA-L04-1316-T01-A	1	1.87E+02			1.87E+02	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1316-T02-A	1	2.00E+02			2.00E+02	1.2E+00	1.0E+00	3.2E+00	1000	100	1.32E+03	112%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1316-T03-A	1	2.67E+02			2.67E+02	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1316-T04-A	1	6.16E+02			6.16E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1316-T05-A	1	9.34E+02			9.34E+02	5.0E-02	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1316-T01-B	1	1.55E+02			1.55E+02	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1316-T02-B	1	2.43E+02			2.43E+02	9.7E-01	1.0E+00	3.2E+00	1000	100	1.42E+03	117%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1316-T03-B	1	2.62E+02			2.62E+02	2.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1316-T04-B	1	4.98E+02			4.98E+02	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1316-T05-B	1	9.42E+02			9.42E+02	5.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1316-T01-C	1	1.43E+02			1.43E+02	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1316-T02-C	1	1.74E+02			1.74E+02	6.2E-01	1.0E+00	3.2E+00	1000	100	1.29E+03	112%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1316-T03-C	1	2.85E+02			2.85E+02	2.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1316-T04-C	1	5.55E+02			5.55E+02	1.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1316-T05-C	1	1.60E+03			1.60E+03	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	5.6E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	1.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
Al	EaFA-L04-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	1.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	EaFA-L04-1316-T01-A	1	1.81E+02			1.81E+02	7.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1316-T02-A	1	2.99E+02			2.99E+02	1.1E+01	7.5E+00	2.4E+01	10	325	3.91E+03	111%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1316-T03-A	1	4.23E+02			4.23E+02	7.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1316-T04-A	1	6.19E+02			6.19E+02	3.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1316-T05-A	1	7.15E+02			7.15E+02	1.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1316-T01-B	1	1.61E+02			1.61E+02	1.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1316-T02-B	1	2.96E+02			2.96E+02	7.0E+00	7.5E+00	2.4E+01	10	325	4.08E+03	117%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1316-T03-B	1	4.33E+02			4.33E+02	4.4E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1316-T04-B	1	6.16E+02			6.16E+02	4.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1316-T05-B	1	6.91E+02			6.91E+02	1.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1316-T01-C	1	2.11E+02			2.11E+02	9.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1316-T02-C	1	3.32E+02			3.32E+02	2.4E+00	7.5E+00	2.4E+01	10	325	3.91E+03	110%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1316-T03-C	1	4.88E+02			4.88E+02	2.4E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1316-T04-C	1	6.73E+02			6.73E+02	2.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1316-T05-C	1	8.91E+02			8.91E+02	2.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1316-B01-A	1	3.75E+00	U1/2		3.75E+00	5.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1316-B02-A	1	3.75E+00	U1/2		3.75E+00	1.9E+02	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
Sb	EaFA-L04-1316-B03-A	1	3.75E+00	U1/2		3.75E+00	6.6E+02	7.5E+00	2.4E+01				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	EaFA-L04-1316-T01-A	1	1.48E+02			1.48E+02	1.2E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1316-T02-A	1	1.49E+02			1.49E+02	2.4E+01	1.1E+01	3.5E+01	10	325	3.84E+03	113%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1316-T03-A	1	1.27E+02			1.27E+02	1.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1316-T04-A	1	1.70E+02			1.70E+02	1.5E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1316-T05-A	1	2.27E+02			2.27E+02	1.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1316-T01-B	1	1.38E+02			1.38E+02	4.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1316-T02-B	1	1.52E+02			1.52E+02	9.9E+00	1.1E+01	3.5E+01	10	325	3.96E+03	117%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1316-T03-B	1	1.16E+02			1.16E+02	1.2E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1316-T04-B	1	1.91E+02			1.91E+02	6.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1316-T05-B	1	2.45E+02			2.45E+02	5.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1316-T01-C	1	1.66E+02			1.66E+02	7.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1316-T02-C	1	1.76E+02			1.76E+02	1.3E+01	1.1E+01	3.5E+01	10	325	3.82E+03	112%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1316-T03-C	1	1.72E+02			1.72E+02	9.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1316-T04-C	1	2.07E+02			2.07E+02	4.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1316-T05-C	1	2.76E+02			2.76E+02	2.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1316-B01-A	1	4.44E+01			4.44E+01	8.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1316-B02-A	1	2.43E+01	E		2.43E+01	4.1E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
As	EaFA-L04-1316-B03-A	1	2.75E+01	E		2.75E+01	4.2E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	EaFA-L04-1316-T01-A	1	4.54E+03			4.54E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1316-T02-A	1	9.00E+03			9.00E+03	1.3E+00	1.0E+00	3.2E+00	1000	100	9.90E+03	90%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1316-T03-A	1	2.02E+04			2.02E+04	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1316-T04-A	1	3.87E+04			3.87E+04	9.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1316-T05-A	1	6.43E+04			6.43E+04	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1316-T01-B	1	5.62E+03			5.62E+03	2.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1316-T02-B	1	9.32E+03			9.32E+03	1.0E+00	1.0E+00	3.2E+00	1000	100	1.02E+04	87%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1316-T03-B	1	2.14E+04			2.14E+04	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1316-T04-B	1	3.97E+04			3.97E+04	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1316-T05-B	1	6.58E+04			6.58E+04	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1316-T01-C	1	5.75E+03			5.75E+03	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1316-T02-C	1	9.22E+03			9.22E+03	1.3E+00	1.0E+00	3.2E+00	1000	100	1.01E+04	91%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1316-T03-C	1	2.30E+04			2.30E+04	2.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1316-T04-C	1	3.98E+04			3.98E+04	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1316-T05-C	1	6.74E+04			6.74E+04	9.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	4.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	5.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
B	EaFA-L04-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	4.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	EaFA-L04-1316-T01-A	1	3.29E+02			3.29E+02	1.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1316-T02-A	1	2.54E+02			2.54E+02	1.1E-01	1.0E+00	3.2E+00	10	325	3.83E+03	110%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1316-T03-A	1	2.37E+02			2.37E+02	5.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1316-T04-A	1	2.64E+02			2.64E+02	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1316-T05-A	1	3.37E+02			3.37E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1316-T01-B	1	3.33E+02			3.33E+02	2.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1316-T02-B	1	2.47E+02			2.47E+02	3.6E-01	1.0E+00	3.2E+00	10	325	3.96E+03	114%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1316-T03-B	1	2.33E+02			2.33E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1316-T04-B	1	2.96E+02			2.96E+02	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1316-T05-B	1	3.58E+02			3.58E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1316-T01-C	1	3.41E+02			3.41E+02	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1316-T02-C	1	2.59E+02			2.59E+02	8.4E-01	1.0E+00	3.2E+00	10	325	3.83E+03	110%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1316-T03-C	1	2.60E+02			2.60E+02	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1316-T04-C	1	2.89E+02			2.89E+02	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1316-T05-C	1	3.61E+02			3.61E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	2.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	5.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
Ba	EaFA-L04-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	2.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	EaFA-L04-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	8.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00	10	325	3.61E+03	111%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	2.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	2.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1316-T05-A	1	9.50E-01	U1/2		9.50E-01	8.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	1.6E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00	10	325	3.77E+03	116%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	3.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	4.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1316-T05-B	1	9.50E-01	U1/2		9.50E-01	1.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	4.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00	10	325	3.57E+03	110%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	5.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1316-T05-C	1	9.50E-01	U1/2		9.50E-01	1.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	3.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1316-B02-A	1	9.50E-01	U1/2		9.50E-01	3.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
Be	EaFA-L04-1316-B03-A	1	9.50E-01	U1/2		9.50E-01	4.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	EaFA-L04-1316-T01-A	1	1.10E+00	U1/2		1.10E+00	1.3E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1316-T02-A	1	2.91E+00	E		2.91E+00	1.5E+01	2.2E+00	7.0E+00	10	325	3.63E+03	112%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1316-T03-A	1	5.63E+00	E		5.63E+00	7.1E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1316-T04-A	1	2.98E+00	E		2.98E+00	2.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1316-T05-A	1	2.88E+00	E		2.88E+00	3.0E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1316-T01-B	1	2.27E+00	E		2.27E+00	2.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1316-T02-B	1	2.90E+00	E		2.90E+00	1.9E+01	2.2E+00	7.0E+00	10	325	3.78E+03	116%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1316-T03-B	1	4.59E+00	E		4.59E+00	1.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1316-T04-B	1	2.68E+00	E		2.68E+00	1.6E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1316-T05-B	1	1.10E+00	U1/2		1.10E+00	3.5E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1316-T01-C	1	2.29E+00	E		2.29E+00	1.9E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1316-T02-C	1	2.51E+00	E		2.51E+00	1.2E+01	2.2E+00	7.0E+00	10	325	3.61E+03	111%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1316-T03-C	1	5.27E+00	E		5.27E+00	1.5E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1316-T04-C	1	1.10E+00	U1/2		1.10E+00	1.7E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1316-T05-C	1	3.13E+00	E		3.13E+00	2.6E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1316-B01-A	1	1.10E+00	U1/2		1.10E+00	3.3E+04	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1316-B02-A	1	1.10E+00	U1/2		1.10E+00	7.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
Cd	EaFA-L04-1316-B03-A	1	1.10E+00	U1/2		1.10E+00	4.6E+02	2.2E+00	7.0E+00				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	EaFA-L04-1316-T01-A	1	1.56E+05			1.56E+05	5.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1316-T02-A	1	3.06E+05			3.06E+05	4.9E-01	2.6E+00	8.3E+00	1000	100	3.07E+05	86%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1316-T03-A	1	6.36E+05			6.36E+05	3.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1316-T04-A	1	5.64E+05			5.64E+05	3.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1316-T05-A	1	4.91E+05			4.91E+05	1.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1316-T01-B	1	1.50E+05			1.50E+05	1.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1316-T02-B	1	2.99E+05			2.99E+05	3.2E-01	2.6E+00	8.3E+00	1000	100	3.00E+05	90%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1316-T03-B	1	6.76E+05			6.76E+05	3.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1316-T04-B	1	5.58E+05			5.58E+05	1.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1316-T05-B	1	5.24E+05			5.24E+05	8.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1316-T01-C	1	1.51E+05			1.51E+05	7.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1316-T02-C	1	3.01E+05			3.01E+05	1.1E+00	2.6E+00	8.3E+00	1000	100	3.02E+05	89%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1316-T03-C	1	7.52E+05			7.52E+05	1.8E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1316-T04-C	1	5.69E+05			5.69E+05	6.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1316-T05-C	1	5.27E+05			5.27E+05	7.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1316-B01-A	1	1.23E+01			1.23E+01	5.3E+01	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1316-B02-A	1	1.20E+01			1.20E+01	3.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
Ca	EaFA-L04-1316-B03-A	1	1.24E+01			1.24E+01	2.7E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	EaFA-L04-1316-T01-A	1	2.44E+01			2.44E+01	4.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1316-T02-A	1	2.82E+01			2.82E+01	3.9E+00	1.2E+00	3.8E+00	10	325	3.48E+03	106%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1316-T03-A	1	2.92E+01			2.92E+01	6.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1316-T04-A	1	4.90E+01			4.90E+01	4.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1316-T05-A	1	5.28E+01			5.28E+01	5.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1316-T01-B	1	1.96E+01			1.96E+01	2.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1316-T02-B	1	2.53E+01			2.53E+01	1.4E+00	1.2E+00	3.8E+00	10	325	3.65E+03	111%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1316-T03-B	1	3.49E+01			3.49E+01	8.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1316-T04-B	1	6.81E+01			6.81E+01	1.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1316-T05-B	1	6.59E+01			6.59E+01	3.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1316-T01-C	1	1.24E+01			1.24E+01	5.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1316-T02-C	1	2.14E+01			2.14E+01	4.0E+00	1.2E+00	3.8E+00	10	325	3.46E+03	106%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1316-T03-C	1	3.02E+01			3.02E+01	5.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1316-T04-C	1	7.20E+01			7.20E+01	3.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1316-T05-C	1	5.28E+01			5.28E+01	3.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	7.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1316-B02-A	1	6.00E-01	U1/2		6.00E-01	1.2E+02	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
Cr	EaFA-L04-1316-B03-A	1	6.00E-01	U1/2		6.00E-01	2.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	EaFA-L04-1316-T01-A	1	3.52E+01			3.52E+01	6.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1316-T02-A	1	7.46E+01			7.46E+01	1.7E+00	1.8E+00	5.7E+00	10	325	3.45E+03	104%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1316-T03-A	1	1.74E+02			1.74E+02	8.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1316-T04-A	1	1.27E+02			1.27E+02	1.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1316-T05-A	1	1.17E+02			1.17E+02	1.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1316-T01-B	1	4.56E+01			4.56E+01	7.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1316-T02-B	1	7.79E+01			7.79E+01	3.3E+00	1.8E+00	5.7E+00	10	325	3.61E+03	109%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1316-T03-B	1	1.49E+02			1.49E+02	4.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1316-T04-B	1	9.35E+01			9.35E+01	4.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1316-T05-B	1	8.63E+01			8.63E+01	2.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1316-T01-C	1	4.67E+01			4.67E+01	4.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1316-T02-C	1	8.71E+01			8.71E+01	2.3E+00	1.8E+00	5.7E+00	10	325	3.44E+03	103%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1316-T03-C	1	1.75E+02			1.75E+02	1.9E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1316-T04-C	1	8.97E+01			8.97E+01	4.9E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1316-T05-C	1	1.09E+02			1.09E+02	2.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	7.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1316-B02-A	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
Co	EaFA-L04-1316-B03-A	1	9.00E-01	U1/2		9.00E-01	9.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	EaFA-L04-1316-T01-A	1	1.00E+01	E		1.00E+01	3.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1316-T02-A	1	1.17E+01	E		1.17E+01	1.1E+01	3.7E+00	1.2E+01	10	325	3.45E+03	106%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1316-T03-A	1	1.41E+01			1.41E+01	3.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1316-T04-A	1	1.19E+01			1.19E+01	2.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1316-T05-A	1	3.75E+01			3.75E+01	1.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1316-T01-B	1	6.20E+00	E		6.20E+00	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1316-T02-B	1	1.18E+01			1.18E+01	6.6E+01	3.7E+00	1.2E+01	10	325	3.63E+03	111%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1316-T03-B	1	1.21E+01			1.21E+01	4.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1316-T04-B	1	9.72E+00	E		9.72E+00	2.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1316-T05-B	1	3.01E+01			3.01E+01	2.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1316-T01-C	1	8.16E+00	E		8.16E+00	3.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1316-T02-C	1	8.10E+00	E		8.10E+00	9.4E+01	3.7E+00	1.2E+01	10	325	3.44E+03	106%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1316-T03-C	1	1.21E+01			1.21E+01	4.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1316-T04-C	1	1.40E+01			1.40E+01	1.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1316-T05-C	1	3.41E+01			3.41E+01	1.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	1.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1316-B02-A	1	1.85E+00	U1/2		1.85E+00	7.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
Cu	EaFA-L04-1316-B03-A	1	1.85E+00	U1/2		1.85E+00	5.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	EaFA-L04-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00	1000	100	1.04E+03	104%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1316-T03-A	1	2.60E+00	E		2.60E+00	1.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1316-T04-A	1	5.29E+01			5.29E+01	4.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1316-T05-A	1	7.27E+01			7.27E+01	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1316-T01-B	1	2.60E+00	E		2.60E+00	2.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1316-T02-B	1	2.11E+01			2.11E+01	2.2E+00	2.0E+00	6.4E+00	1000	100	1.11E+03	109%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	3.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	4.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1316-T05-B	1	4.63E+01			4.63E+01	2.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.0E+00	6.4E+00	1000	100	1.04E+03	104%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1316-T03-C	1	2.02E+00	E		2.02E+00	1.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1316-T04-C	1	9.80E+00			9.80E+00	4.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1316-T05-C	1	2.32E+02			2.32E+02	8.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1316-B02-A	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
Fe	EaFA-L04-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	EaFA-L04-1316-T01-A	1	3.40E+00	U1/2		3.40E+00	6.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1316-T02-A	1	3.40E+00	U1/2		3.40E+00	1.4E+02	6.8E+00	2.2E+01	10	325	3.40E+03	104%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1316-T03-A	1	3.40E+00	U1/2		3.40E+00	1.5E+03	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1316-T04-A	1	3.40E+00	U1/2		3.40E+00	1.0E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1316-T05-A	1	3.40E+00	U1/2		3.40E+00	7.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1316-T01-B	1	3.40E+00	U1/2		3.40E+00	1.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1316-T02-B	1	3.40E+00	U1/2		3.40E+00	1.3E+02	6.8E+00	2.2E+01	10	325	3.55E+03	109%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1316-T03-B	1	3.40E+00	U1/2		3.40E+00	8.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1316-T04-B	1	3.40E+00	U1/2		3.40E+00	4.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1316-T05-B	1	3.40E+00	U1/2		3.40E+00	1.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1316-T01-C	1	3.40E+00	U1/2		3.40E+00	1.9E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1316-T02-C	1	3.40E+00	U1/2		3.40E+00	3.3E+01	6.8E+00	2.2E+01	10	325	3.40E+03	104%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1316-T03-C	1	3.40E+00	U1/2		3.40E+00	2.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1316-T04-C	1	3.40E+00	U1/2		3.40E+00	2.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1316-T05-C	1	3.40E+00	U1/2		3.40E+00	1.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	1.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1316-B02-A	1	3.40E+00	U1/2		3.40E+00	4.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
Pb	EaFA-L04-1316-B03-A	1	3.40E+00	U1/2		3.40E+00	6.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	EaFA-L04-1316-T01-A	1	3.78E+03			3.78E+03	5.0E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1316-T02-A	1	7.35E+03			7.35E+03	3.0E-01	1.9E+00	6.0E+00	10	325	1.08E+04	106%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1316-T03-A	1	1.73E+04			1.73E+04	6.2E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1316-T04-A	1	3.52E+04			3.52E+04	8.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1316-T05-A	1	6.70E+04			6.70E+04	1.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1316-T01-B	1	3.67E+03			3.67E+03	3.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1316-T02-B	1	7.23E+03			7.23E+03	4.3E-01	1.9E+00	6.0E+00	10	325	1.10E+04	116%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1316-T03-B	1	1.70E+04			1.70E+04	3.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1316-T04-B	1	3.57E+04			3.57E+04	1.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1316-T05-B	1	6.98E+04			6.98E+04	1.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1316-T01-C	1	3.71E+03			3.71E+03	7.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1316-T02-C	1	7.22E+03			7.22E+03	9.6E-01	1.9E+00	6.0E+00	10	325	1.08E+04	110%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1316-T03-C	1	1.88E+04			1.88E+04	1.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1316-T04-C	1	3.61E+04			3.61E+04	6.2E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1316-T05-C	1	7.00E+04			7.00E+04	1.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1316-B01-A	1	3.33E+00	E		3.33E+00	4.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1316-B02-A	1	2.36E+00	E		2.36E+00	1.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
Li	EaFA-L04-1316-B03-A	1	4.56E+00	E		4.56E+00	9.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	EaFA-L04-1316-T01-A	1	3.14E+02			3.14E+02	4.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1316-T02-A	1	6.17E+02			6.17E+02	5.7E-01	2.0E+00	6.4E+00	10	325	4.02E+03	105%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1316-T03-A	1	1.36E+03			1.36E+03	6.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1316-T04-A	1	1.31E+03			1.31E+03	1.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1316-T05-A	1	1.45E+03			1.45E+03	3.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1316-T01-B	1	3.44E+02			3.44E+02	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1316-T02-B	1	6.05E+02			6.05E+02	9.5E-01	2.0E+00	6.4E+00	10	325	4.14E+03	109%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1316-T03-B	1	1.18E+03			1.18E+03	1.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1316-T04-B	1	1.00E+03			1.00E+03	4.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1316-T05-B	1	1.20E+03			1.20E+03	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1316-T01-C	1	3.76E+02			3.76E+02	7.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1316-T02-C	1	6.62E+02			6.62E+02	6.1E-01	2.0E+00	6.4E+00	10	325	4.04E+03	104%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1316-T03-C	1	1.36E+03			1.36E+03	2.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1316-T04-C	1	9.73E+02			9.73E+02	5.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1316-T05-C	1	1.41E+03			1.41E+03	1.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1316-B02-A	1	1.00E+00	U1/2		1.00E+00	3.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
Mn	EaFA-L04-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	4.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	EaFA-L04-1316-T01-A	1	7.48E+03			7.48E+03	2.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1316-T02-A	1	1.45E+04			1.45E+04	3.5E-01	1.0E+00	3.2E+00	1000	100	1.55E+04	94%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1316-T03-A	1	3.51E+04			3.51E+04	8.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1316-T04-A	1	6.81E+04			6.81E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1316-T05-A	1	1.22E+05			1.22E+05	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1316-T01-B	1	7.09E+03			7.09E+03	3.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1316-T02-B	1	1.44E+04			1.44E+04	1.4E+00	1.0E+00	3.2E+00	1000	100	1.54E+04	95%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1316-T03-B	1	3.47E+04			3.47E+04	6.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1316-T04-B	1	6.80E+04			6.80E+04	1.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1316-T05-B	1	1.28E+05			1.28E+05	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1316-T01-C	1	7.24E+03			7.24E+03	3.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1316-T02-C	1	1.42E+04			1.42E+04	9.7E-01	1.0E+00	3.2E+00	1000	100	1.52E+04	97%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1316-T03-C	1	3.87E+04			3.87E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1316-T04-C	1	6.82E+04			6.82E+04	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1316-T05-C	1	1.25E+05			1.25E+05	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.6E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
Mg	EaFA-L04-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	9.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	EaFA-L04-1316-T01-A	1	3.38E+03			3.38E+03	3.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1316-T02-A	1	6.30E+03			6.30E+03	2.3E-01	1.2E+00	3.8E+00	10	325	9.36E+03	94%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1316-T03-A	1	1.35E+04			1.35E+04	7.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1316-T04-A	1	2.74E+04			2.74E+04	7.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1316-T05-A	1	4.54E+04			4.54E+04	8.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1316-T01-B	1	3.23E+03			3.23E+03	5.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1316-T02-B	1	6.29E+03			6.29E+03	7.6E-01	1.2E+00	3.8E+00	10	325	9.60E+03	102%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1316-T03-B	1	1.39E+04			1.39E+04	3.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1316-T04-B	1	2.91E+04			2.91E+04	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1316-T05-B	1	5.13E+04			5.13E+04	8.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1316-T01-C	1	3.29E+03			3.29E+03	7.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1316-T02-C	1	6.24E+03			6.24E+03	8.1E-01	1.2E+00	3.8E+00	10	325	9.40E+03	97%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1316-T03-C	1	1.54E+04			1.54E+04	1.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1316-T04-C	1	3.04E+04			3.04E+04	8.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1316-T05-C	1	5.12E+04			5.12E+04	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1316-B01-A	1	9.12E+00			9.12E+00	3.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1316-B02-A	1	8.95E+00			8.95E+00	1.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
Mo	EaFA-L04-1316-B03-A	1	6.26E+00			6.26E+00	1.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	EaFA-L04-1316-T01-A	1	8.66E+01			8.66E+01	6.3E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1316-T02-A	1	1.79E+02			1.79E+02	1.2E+00	1.8E+00	5.7E+00	10	325	3.72E+03	109%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1316-T03-A	1	3.79E+02			3.79E+02	1.6E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1316-T04-A	1	2.85E+02			2.85E+02	4.3E-01	1.8E+00	5.7E+00			---		VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1316-T05-A	1	2.80E+02			2.80E+02	2.6E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1316-T01-B	1	1.02E+02			1.02E+02	6.3E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1316-T02-B	1	1.83E+02			1.83E+02	2.1E+00	1.8E+00	5.7E+00	10	325	3.87E+03	113%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1316-T03-B	1	3.38E+02			3.38E+02	3.6E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1316-T04-B	1	2.19E+02			2.19E+02	1.3E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1316-T05-B	1	1.96E+02			1.96E+02	1.9E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1316-T01-C	1	1.11E+02			1.11E+02	3.2E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1316-T02-C	1	1.95E+02			1.95E+02	3.6E+00	1.8E+00	5.7E+00	10	325	3.73E+03	109%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1316-T03-C	1	4.05E+02			4.05E+02	3.1E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1316-T04-C	1	2.02E+02			2.02E+02	4.6E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1316-T05-C	1	2.50E+02			2.50E+02	1.5E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	3.4E+02	1.8E+00	5.7E+00			---		VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1316-B02-A	1	9.00E-01	U1/2		9.00E-01	4.6E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
Ni	EaFA-L04-1316-B03-A	1	9.00E-01	U1/2		9.00E-01	1.5E+03	1.8E+00	5.7E+00			---		VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	EaFA-L04-1316-T01-A	1	8.62E+01			8.62E+01	3.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1316-T02-A	1	1.31E+02			1.31E+02	2.8E+01	3.7E+00	1.2E+01	1000	100	1.19E+03	106%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1316-T03-A	1	1.48E+02			1.48E+02	1.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1316-T04-A	1	2.71E+02			2.71E+02	4.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1316-T05-A	1	6.74E+02			6.74E+02	6.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1316-T01-B	1	8.72E+01			8.72E+01	3.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1316-T02-B	1	1.24E+02			1.24E+02	2.2E+01	3.7E+00	1.2E+01	1000	100	1.25E+03	112%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1316-T03-B	1	1.35E+02			1.35E+02	5.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1316-T04-B	1	1.88E+02			1.88E+02	5.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1316-T05-B	1	8.97E+02			8.97E+02	2.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1316-T01-C	1	1.06E+02			1.06E+02	1.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1316-T02-C	1	1.05E+02			1.05E+02	1.1E+01	3.7E+00	1.2E+01	1000	100	1.15E+03	105%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1316-T03-C	1	1.14E+02			1.14E+02	1.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1316-T04-C	1	2.27E+02			2.27E+02	6.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1316-T05-C	1	1.20E+03			1.20E+03	2.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1316-B01-A	1	3.95E+00	E		3.95E+00	5.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1316-B02-A	1	6.86E+00	E		6.86E+00	2.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
P	EaFA-L04-1316-B03-A	1	5.10E+00	E		5.10E+00	1.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	EaFA-L04-1316-T01-A	1	2.40E+04			2.40E+04	2.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1316-T02-A	1	4.98E+04			4.98E+04	3.6E-01	1.6E+00	5.1E+00	1000	100	5.07E+04	91%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1316-T03-A	1	1.23E+05			1.23E+05	2.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1316-T04-A	1	2.09E+05			2.09E+05	7.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1316-T05-A	1	3.25E+05			3.25E+05	8.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1316-T01-B	1	2.30E+04			2.30E+04	1.6E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1316-T02-B	1	4.92E+04			4.92E+04	5.6E-01	1.6E+00	5.1E+00	1000	100	5.01E+04	89%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1316-T03-B	1	1.21E+05			1.21E+05	4.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1316-T04-B	1	2.08E+05			2.08E+05	6.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1316-T05-B	1	3.41E+05			3.41E+05	2.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1316-T01-C	1	2.35E+04			2.35E+04	8.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1316-T02-C	1	4.87E+04			4.87E+04	1.0E+00	1.6E+00	5.1E+00	1000	100	4.96E+04	95%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1316-T03-C	1	1.35E+05			1.35E+05	7.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1316-T04-C	1	2.15E+05			2.15E+05	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1316-T05-C	1	3.36E+05			3.36E+05	8.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1316-B01-A	1	6.09E+00			6.09E+00	1.9E+01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1316-B02-A	1	5.82E+00			5.82E+00	1.0E+01	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
K	EaFA-L04-1316-B03-A	1	4.12E+00	E		4.12E+00	2.9E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	EaFA-L04-1316-T01-A	1	1.34E+03			1.34E+03	9.4E-01	1.5E+01	4.8E+01				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1316-T02-A	1	1.73E+03			1.73E+03	3.4E+00	1.5E+01	4.8E+01	10	325	5.15E+03	105%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1316-T03-A	1	1.86E+03			1.86E+03	3.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1316-T04-A	1	2.72E+03			2.72E+03	1.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1316-T05-A	1	3.14E+03			3.14E+03	1.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1316-T01-B	1	1.33E+03			1.33E+03	2.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1316-T02-B	1	1.66E+03			1.66E+03	1.9E+00	1.5E+01	4.8E+01	10	325	5.23E+03	110%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1316-T03-B	1	1.90E+03			1.90E+03	3.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1316-T04-B	1	2.74E+03			2.74E+03	1.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1316-T05-B	1	3.60E+03			3.60E+03	2.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1316-T01-C	1	1.34E+03			1.34E+03	3.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1316-T02-C	1	1.78E+03			1.78E+03	1.2E+00	1.5E+01	4.8E+01	10	325	5.14E+03	103%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1316-T03-C	1	1.94E+03			1.94E+03	1.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1316-T04-C	1	2.94E+03			2.94E+03	1.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1316-T05-C	1	3.90E+03			3.90E+03	3.2E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1316-B01-A	1	7.50E+00	U1/2		7.50E+00	1.9E+02	1.5E+01	4.8E+01				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1316-B02-A	1	7.50E+00	U1/2		7.50E+00	4.8E+02	1.5E+01	4.8E+01				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
Se	EaFA-L04-1316-B03-A	1	7.50E+00	U1/2		7.50E+00	2.8E+02	1.5E+01	4.8E+01				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	EaFA-L04-1316-T01-A	1	2.07E+03			2.07E+03	1.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1316-T02-A	1	2.39E+03			2.39E+03	1.2E+00	1.1E+00	3.5E+00	1000	100	3.34E+03	95%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1316-T03-A	1	2.57E+03			2.57E+03	7.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1316-T04-A	1	2.59E+03			2.59E+03	1.6E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1316-T05-A	1	2.70E+03			2.70E+03	6.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1316-T01-B	1	2.32E+03			2.32E+03	7.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1316-T02-B	1	2.74E+03			2.74E+03	7.8E-01	1.1E+00	3.5E+00	1000	100	3.81E+03	107%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1316-T03-B	1	2.51E+03			2.51E+03	2.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1316-T04-B	1	2.07E+03			2.07E+03	1.5E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1316-T05-B	1	2.47E+03			2.47E+03	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1316-T01-C	1	2.56E+03			2.56E+03	5.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1316-T02-C	1	2.95E+03			2.95E+03	5.6E-01	1.1E+00	3.5E+00	1000	100	3.91E+03	96%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1316-T03-C	1	2.75E+03			2.75E+03	2.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1316-T04-C	1	2.17E+03			2.17E+03	8.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1316-T05-C	1	3.96E+03			3.96E+03	9.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1316-B01-A	1	5.50E-01	U1/2		5.50E-01	2.7E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1316-B02-A	1	5.50E-01	U1/2		5.50E-01	3.9E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
Si	EaFA-L04-1316-B03-A	1	5.50E-01	U1/2		5.50E-01	2.8E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	EaFA-L04-1316-T01-A	1	5.30E+03			5.30E+03	5.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1316-T02-A	1	1.07E+04			1.07E+04	1.3E-01	2.5E+00	8.0E+00	1000	100	1.16E+04	89%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1316-T03-A	1	2.68E+04			2.68E+04	2.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1316-T04-A	1	4.60E+04			4.60E+04	3.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1316-T05-A	1	7.56E+04			7.56E+04	2.0E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1316-T01-B	1	5.08E+03			5.08E+03	8.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1316-T02-B	1	1.06E+04			1.06E+04	1.0E+00	2.5E+00	8.0E+00	1000	100	1.15E+04	87%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1316-T03-B	1	2.59E+04			2.59E+04	4.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1316-T04-B	1	4.55E+04			4.55E+04	1.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1316-T05-B	1	7.95E+04			7.95E+04	8.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1316-T01-C	1	5.15E+03			5.15E+03	3.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1316-T02-C	1	1.05E+04			1.05E+04	5.8E-01	2.5E+00	8.0E+00	1000	100	1.14E+04	90%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1316-T03-C	1	2.87E+04			2.87E+04	1.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1316-T04-C	1	4.73E+04			4.73E+04	1.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1316-T05-C	1	8.01E+04			8.01E+04	7.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1316-B01-A	1	2.85E+01			2.85E+01	9.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1316-B02-A	1	2.93E+01			2.93E+01	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
Na	EaFA-L04-1316-B03-A	1	3.00E+01			3.00E+01	1.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	EaFA-L04-1316-T01-A	1	2.17E+03			2.17E+03	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1316-T02-A	1	3.86E+03			3.86E+03	6.1E-01	1.0E+00	3.2E+00	1000	100	4.67E+03	81%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1316-T03-A	1	7.16E+03			7.16E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1316-T04-A	1	7.43E+03			7.43E+03	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1316-T05-A	1	7.40E+03			7.40E+03	6.8E-02	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1316-T01-B	1	2.04E+03			2.04E+03	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1316-T02-B	1	3.89E+03			3.89E+03	9.9E-01	1.0E+00	3.2E+00	1000	100	4.81E+03	92%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1316-T03-B	1	7.74E+03			7.74E+03	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1316-T04-B	1	8.59E+03			8.59E+03	8.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1316-T05-B	1	7.67E+03			7.67E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1316-T01-C	1	2.07E+03			2.07E+03	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1316-T02-C	1	3.85E+03			3.85E+03	4.4E-01	1.0E+00	3.2E+00	1000	100	4.68E+03	83%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1316-T03-C	1	8.51E+03			8.51E+03	3.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1316-T04-C	1	8.98E+03			8.98E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1316-T05-C	1	8.26E+03			8.26E+03	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	3.9E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
Sr	EaFA-L04-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	3.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	EaFA-L04-1316-T01-A	1	2.66E+06			2.66E+06	9.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1316-T02-A	1	2.69E+06			2.69E+06	6.9E-01	6.8E+00	2.2E+01	1000	500	2.70E+06	82%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1316-T03-A	1	2.83E+06			2.83E+06	2.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1316-T04-A	1	2.84E+06			2.84E+06	1.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1316-T05-A	1	2.74E+06			2.74E+06	2.3E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1316-T01-B	1	2.59E+06			2.59E+06	5.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1316-T02-B	1	2.60E+06			2.60E+06	1.1E+00	6.8E+00	2.2E+01	1000	500	2.60E+06	88%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1316-T03-B	1	2.65E+06			2.65E+06	4.8E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1316-T04-B	1	2.72E+06			2.72E+06	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1316-T05-B	1	2.94E+06			2.94E+06	1.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1316-T01-C	1	2.53E+06			2.53E+06	3.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1316-T02-C	1	2.58E+06			2.58E+06	1.1E+00	6.8E+00	2.2E+01	1000	500	2.59E+06	85%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1316-T03-C	1	2.85E+06			2.85E+06	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1316-T04-C	1	2.97E+06			2.97E+06	1.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1316-T05-C	1	2.89E+06			2.89E+06	1.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1316-B01-A	1	2.83E+01			2.83E+01	5.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1316-B02-A	1	1.06E+01	E		1.06E+01	9.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
S	EaFA-L04-1316-B03-A	1	1.27E+01	E		1.27E+01	5.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	EaFA-L04-1316-T01-A	1	2.30E+00	U1/2		2.30E+00	3.8E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1316-T02-A	1	2.30E+00	U1/2		2.30E+00	9.8E+02	4.6E+00	1.5E+01	10	325	3.37E+03	104%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1316-T03-A	1	2.73E+01			2.73E+01	5.2E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1316-T04-A	1	3.50E+01			3.50E+01	4.0E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1316-T05-A	1	5.58E+01			5.58E+01	2.1E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1316-T01-B	1	2.30E+00	U1/2		2.30E+00	8.5E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1316-T02-B	1	1.00E+01	E		1.00E+01	1.6E+02	4.6E+00	1.5E+01	10	325	3.52E+03	108%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1316-T03-B	1	2.21E+01			2.21E+01	5.1E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1316-T04-B	1	4.22E+01			4.22E+01	7.9E+00	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1316-T05-B	1	4.30E+01			4.30E+01	4.8E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1316-T01-C	1	2.30E+00	U1/2		2.30E+00	3.8E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1316-T02-C	1	2.30E+00	U1/2		2.30E+00	1.7E+02	4.6E+00	1.5E+01	10	325	3.38E+03	104%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1316-T03-C	1	2.30E+01			2.30E+01	1.8E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1316-T04-C	1	3.25E+01			3.25E+01	9.4E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1316-T05-C	1	5.37E+01			5.37E+01	1.3E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1316-B01-A	1	2.30E+00	U1/2		2.30E+00	1.1E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1316-B02-A	1	2.30E+00	U1/2		2.30E+00	2.5E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
Tl	EaFA-L04-1316-B03-A	1	2.30E+00	U1/2		2.30E+00	6.5E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	EaFA-L04-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	2.7E+02	2.0E+00	6.4E+00	10	325	3.14E+03	96%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	3.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1316-T04-A	1	2.84E+01			2.84E+01	4.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1316-T05-A	1	2.07E+01			2.07E+01	4.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	2.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1316-T02-B	1	1.02E+01			1.02E+01	1.5E+01	2.0E+00	6.4E+00	10	325	3.25E+03	100%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	7.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	1.6E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1316-T05-B	1	7.28E+00			7.28E+00	1.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	9.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	2.7E+02	2.0E+00	6.4E+00	10	325	3.10E+03	95%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	1.6E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1316-T04-C	1	2.61E+00	E		2.61E+00	5.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1316-T05-C	1	8.61E+01			8.61E+01	2.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1316-B02-A	1	1.00E+00	U1/2		1.00E+00	1.0E+03	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
Ti	EaFA-L04-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	2.6E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	EaFA-L04-1316-T01-A	1	2.58E+02			2.58E+02	3.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1316-T02-A	1	2.94E+02			2.94E+02	8.2E-01	1.5E+00	4.8E+00	10	325	3.78E+03	107%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1316-T03-A	1	3.28E+02			3.28E+02	3.4E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1316-T04-A	1	3.65E+02			3.65E+02	1.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1316-T05-A	1	3.75E+02			3.75E+02	3.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1316-T01-B	1	2.58E+02			2.58E+02	2.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1316-T02-B	1	2.96E+02			2.96E+02	8.1E-01	1.5E+00	4.8E+00	10	325	3.93E+03	112%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1316-T03-B	1	3.35E+02			3.35E+02	3.9E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1316-T04-B	1	3.66E+02			3.66E+02	1.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1316-T05-B	1	3.86E+02			3.86E+02	1.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1316-T01-C	1	2.68E+02			2.68E+02	2.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1316-T02-C	1	3.19E+02			3.19E+02	8.9E-01	1.5E+00	4.8E+00	10	325	3.79E+03	107%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1316-T03-C	1	3.62E+02			3.62E+02	1.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1316-T04-C	1	4.18E+02			4.18E+02	1.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1316-T05-C	1	4.56E+02			4.56E+02	1.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1316-B01-A	1	7.75E+00			7.75E+00	3.5E+01	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1316-B02-A	1	8.44E+00			8.44E+00	5.8E+01	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
V	EaFA-L04-1316-B03-A	1	8.95E+00			8.95E+00	9.4E+01	1.5E+00	4.8E+00				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	EaFA-L04-1316-T01-A	1	9.02E+00			9.02E+00	1.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:13 PM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1316-T02-A	1	2.46E+01			2.46E+01	3.4E+00	1.0E+00	3.2E+00	10	325	3.61E+03	110%	VU ICP-OES	6/24/10 12:14 PM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1316-T03-A	1	3.06E+01			3.06E+01	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:16 PM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1316-T04-A	1	3.01E+01			3.01E+01	4.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:18 PM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1316-T05-A	1	1.06E+02			1.06E+02	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:19 PM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1316-T01-B	1	1.21E+01			1.21E+01	6.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:21 PM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1316-T02-B	1	1.77E+01			1.77E+01	1.1E+01	1.0E+00	3.2E+00	10	325	3.74E+03	115%	VU ICP-OES	6/24/10 12:23 PM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1316-T03-B	1	2.42E+01			2.42E+01	6.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:24 PM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1316-T04-B	1	1.89E+01			1.89E+01	4.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:26 PM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1316-T05-B	1	8.05E+01			8.05E+01	2.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:28 PM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1316-T01-C	1	1.40E+01			1.40E+01	6.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:29 PM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1316-T02-C	1	1.96E+01			1.96E+01	2.9E+00	1.0E+00	3.2E+00	10	325	3.60E+03	110%	VU ICP-OES	6/24/10 12:31 PM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1316-T03-C	1	3.49E+01			3.49E+01	5.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:32 PM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1316-T04-C	1	2.18E+01			2.18E+01	5.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:34 PM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1316-T05-C	1	2.00E+02			2.00E+02	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:36 PM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1316-B01-A	1	1.26E+01			1.26E+01	4.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:08 PM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1316-B02-A	1	1.29E+01			1.29E+01	1.5E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:09 PM	EPA Interlab L04 1313-1316 EaFA
Zn	EaFA-L04-1316-B03-A	1	1.12E+01			1.12E+01	1.1E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/24/10 12:11 PM	EPA Interlab L04 1313-1316 EaFA

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	EaFA-L05-1316-T01-A	1	1.51E+03			1.51E+03	9.29E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1316-T02-A	1	9.62E+02			9.62E+02	6.74E-01	1.0E+00	3.2E+00	1000	100	1.90E+03	93%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1316-T03-A	1	3.14E+02			3.14E+02	8.52E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1316-T04-A	1	2.09E+02			2.09E+02	1.83E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1316-T05-A															
Al	EaFA-L05-1316-T01-B	1	5.73E+02			5.73E+02	3.17E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1316-T02-B	1	3.28E+03			3.28E+03	2.01E+00	1.0E+00	3.2E+00	1000	100	4.18E+03	90%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1316-T03-B	1	1.55E+02			1.55E+02	4.15E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1316-T04-B	1	1.97E+02			1.97E+02	2.45E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1316-T05-B															
Al	EaFA-L05-1316-T01-C	1	4.62E+03			4.62E+03	7.04E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1316-T02-C	1	1.40E+02			1.40E+02	1.64E+00	1.0E+00	3.2E+00	1000	100	1.21E+03	107%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1316-T03-C	1	1.48E+02			1.48E+02	8.12E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1316-T04-C	1	2.26E+02			2.26E+02	1.03E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
Al	EaFA-L05-1316-T05-C															
Al	EaFA-L05-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	2.65E+02	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	EaFA-L05-1316-T01-A	1	3.75E+01			3.75E+01	5.01E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1316-T02-A	1	7.73E+01			7.73E+01	7.12E+00	7.5E+00	2.4E+01	10	300	3.37E+03	110%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1316-T03-A	1	1.53E+02			1.53E+02	7.80E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1316-T04-A	1	3.17E+02			3.17E+02	2.02E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1316-T05-A															
Sb	EaFA-L05-1316-T01-B	1	7.86E+01			7.86E+01	1.09E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1316-T02-B	1	4.22E+01			4.22E+01	8.16E+00	7.5E+00	2.4E+01	10	300	3.12E+03	102%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1316-T03-B	1	2.53E+02			2.53E+02	6.47E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1316-T04-B	1	3.06E+02			3.06E+02	7.19E-01	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1316-T05-B															
Sb	EaFA-L05-1316-T01-C	1	3.97E+01			3.97E+01	1.53E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1316-T02-C	1	6.11E+01			6.11E+01	3.23E+00	7.5E+00	2.4E+01	10	300	3.54E+03	116%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1316-T03-C	1	2.40E+02			2.40E+02	4.75E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1316-T04-C	1	1.98E+02			1.98E+02	2.52E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
Sb	EaFA-L05-1316-T05-C															
Sb	EaFA-L05-1316-B01-A	1	3.75E+00	U1/2		3.75E+00	8.29E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	EaFA-L05-1316-T01-A	1	2.23E+01	E		2.23E+01	2.42E+01	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1316-T02-A	1	2.56E+01	E		2.56E+01	1.96E+01	1.1E+01	3.5E+01	10	300	3.25E+03	107%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1316-T03-A	1	2.73E+01	E		2.73E+01	7.34E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1316-T04-A	1	2.36E+01	E		2.36E+01	2.22E+01	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1316-T05-A															
As	EaFA-L05-1316-T01-B	1	1.83E+01	E		1.83E+01	1.10E+01	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1316-T02-B	1	1.92E+01	E		1.92E+01	1.88E+01	1.1E+01	3.5E+01	10	300	3.06E+03	101%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1316-T03-B	1	3.69E+01			3.69E+01	2.39E+01	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1316-T04-B	1	4.60E+01			4.60E+01	3.39E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1316-T05-B															
As	EaFA-L05-1316-T01-C	1	1.88E+01	E		1.88E+01	2.32E+01	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1316-T02-C	1	3.75E+01			3.75E+01	2.24E+01	1.1E+01	3.5E+01	10	300	3.43E+03	113%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1316-T03-C	1	3.61E+01			3.61E+01	8.72E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1316-T04-C	1	4.39E+01			4.39E+01	1.06E+01	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
As	EaFA-L05-1316-T05-C															
As	EaFA-L05-1316-B01-A	1	5.50E+00	U1/2		5.50E+00	4.48E+01	1.1E+01	3.5E+01				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	EaFA-L05-1316-T01-A	1	3.39E+03			3.39E+03	5.81E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1316-T02-A	1	6.96E+03			6.96E+03	1.28E+00	1.0E+00	3.2E+00	1000	100	8.04E+03	108%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1316-T03-A	1	1.86E+04			1.86E+04	8.50E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1316-T04-A	1	3.44E+04			3.44E+04	5.50E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1316-T05-A															
B	EaFA-L05-1316-T01-B	1	4.47E+03			4.47E+03	4.73E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1316-T02-B	1	6.41E+03			6.41E+03	1.96E+00	1.0E+00	3.2E+00	1000	100	7.28E+03	87%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1316-T03-B	1	1.95E+04			1.95E+04	3.49E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1316-T04-B	1	3.45E+04			3.45E+04	8.57E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1316-T05-B															
B	EaFA-L05-1316-T01-C	1	4.10E+03			4.10E+03	2.36E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1316-T02-C	1	7.05E+03			7.05E+03	1.73E+00	1.0E+00	3.2E+00	1000	100	8.03E+03	98%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1316-T03-C	1	1.99E+04			1.99E+04	5.15E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1316-T04-C	1	3.37E+04			3.37E+04	1.07E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
B	EaFA-L05-1316-T05-C															
B	EaFA-L05-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.16E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	EaFA-L05-1316-T01-A	1	5.60E+02			5.60E+02	1.39E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1316-T02-A	1	5.85E+02			5.85E+02	1.20E+00	1.0E+00	3.2E+00	10	300	3.47E+03	96%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1316-T03-A	1	1.95E+02			1.95E+02	2.16E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1316-T04-A	1	2.28E+02			2.28E+02	1.19E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1316-T05-A															
Ba	EaFA-L05-1316-T01-B	1	5.00E+02			5.00E+02	1.96E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1316-T02-B	1	3.91E+02			3.91E+02	5.66E-01	1.0E+00	3.2E+00	10	300	3.14E+03	92%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1316-T03-B	1	2.04E+02			2.04E+02	1.31E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1316-T04-B	1	2.20E+02			2.20E+02	1.35E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1316-T05-B															
Ba	EaFA-L05-1316-T01-C	1	4.48E+02			4.48E+02	3.29E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1316-T02-C	1	5.01E+02			5.01E+02	5.79E-01	1.0E+00	3.2E+00	10	300	3.52E+03	101%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1316-T03-C	1	2.07E+02			2.07E+02	3.68E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1316-T04-C	1	2.54E+02			2.54E+02	1.23E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
Ba	EaFA-L05-1316-T05-C															
Ba	EaFA-L05-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	7.67E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	EaFA-L05-1316-T01-A	1	1.32E+01			1.32E+01	2.02E+02	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1316-T02-A	1	9.30E+00			9.30E+00	1.24E+02	1.9E+00	6.0E+00	10	300	3.30E+03	110%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1316-T03-A	1	3.95E+00	E		3.95E+00	2.75E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	5.50E+02	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1316-T05-A															
Be	EaFA-L05-1316-T01-B	1	5.97E+00	E		5.97E+00	2.99E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1316-T02-B	1	2.49E+01			2.49E+01	3.08E+01	1.9E+00	6.0E+00	10	300	3.12E+03	103%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	1.45E+02	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	1.25E+03	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1316-T05-B															
Be	EaFA-L05-1316-T01-C	1	2.90E+01			2.90E+01	6.12E+02	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1316-T02-C	1	1.93E+00	E		1.93E+00	1.99E+02	1.9E+00	6.0E+00	10	300	3.42E+03	114%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	2.59E+02	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1316-T04-C	1	3.09E+00	E		3.09E+00	9.88E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
Be	EaFA-L05-1316-T05-C															
Be	EaFA-L05-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	1.47E+02	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	EaFA-L05-1316-T01-A	1	1.77E+01			1.77E+01	3.14E+01	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1316-T02-A	1	2.80E+01			2.80E+01	1.75E+01	2.2E+00	7.0E+00	10	300	3.32E+03	110%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1316-T03-A	1	9.61E+01			9.61E+01	7.82E-01	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1316-T04-A	1	1.20E+01			1.20E+01	1.92E+01	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1316-T05-A															
Cd	EaFA-L05-1316-T01-B	1	1.11E+01			1.11E+01	2.19E+01	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1316-T02-B	1	3.17E+01			3.17E+01	9.41E+00	2.2E+00	7.0E+00	10	300	3.15E+03	104%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1316-T03-B	1	1.31E+01			1.31E+01	1.05E+00	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1316-T04-B	1	2.48E+01			2.48E+01	8.55E+00	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1316-T05-B															
Cd	EaFA-L05-1316-T01-C	1	2.31E+01			2.31E+01	2.99E+01	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1316-T02-C	1	9.52E+00			9.52E+00	3.03E+01	2.2E+00	7.0E+00	10	300	3.45E+03	115%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1316-T03-C	1	1.68E+01			1.68E+01	3.70E+00	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1316-T04-C	1	1.09E+02			1.09E+02	2.15E+01	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
Cd	EaFA-L05-1316-T05-C															
Cd	EaFA-L05-1316-B01-A	1	1.10E+00	U1/2		1.10E+00	1.38E+02	2.2E+00	7.0E+00				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	EaFA-L05-1316-T01-A	1	1.09E+05			1.09E+05	1.43E+00	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1316-T02-A	1	2.50E+05			2.50E+05	1.22E+00	2.6E+00	8.3E+00	1000	100	2.51E+05	83%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1316-T03-A	1	6.45E+05			6.45E+05	4.12E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1316-T04-A	1	5.69E+05			5.69E+05	2.73E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1316-T05-A															
Ca	EaFA-L05-1316-T01-B	1	1.15E+05			1.15E+05	1.87E+00	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1316-T02-B	1	1.91E+05			1.91E+05	6.14E-01	2.6E+00	8.3E+00	1000	100	1.92E+05	90%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1316-T03-B	1	7.11E+05			7.11E+05	7.37E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1316-T04-B	1	5.55E+05			5.55E+05	1.27E+00	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1316-T05-B															
Ca	EaFA-L05-1316-T01-C	1	1.16E+05			1.16E+05	6.15E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1316-T02-C	1	2.12E+05			2.12E+05	4.62E-01	2.6E+00	8.3E+00	1000	100	2.13E+05	87%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1316-T03-C	1	7.16E+05			7.16E+05	4.71E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1316-T04-C	1	5.13E+05			5.13E+05	1.70E+00	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
Ca	EaFA-L05-1316-T05-C															
Ca	EaFA-L05-1316-B01-A	1	2.87E+01			2.87E+01	9.15E+01	2.6E+00	8.3E+00				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	EaFA-L05-1316-T01-A	1	8.68E+00			8.68E+00	1.49E+01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1316-T02-A	1	1.35E+01			1.35E+01	1.02E+01	1.2E+00	3.8E+00	10	300	3.18E+03	106%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1316-T03-A	1	5.80E+00			5.80E+00	5.18E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1316-T04-A	1	3.85E+01			3.85E+01	3.62E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1316-T05-A															
Cr	EaFA-L05-1316-T01-B	1	1.10E+01			1.10E+01	9.45E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1316-T02-B	1	7.96E+00			7.96E+00	5.43E+00	1.2E+00	3.8E+00	10	300	3.01E+03	100%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1316-T03-B	1	2.56E+01			2.56E+01	1.04E+01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1316-T04-B	1	2.05E+01			2.05E+01	4.82E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1316-T05-B															
Cr	EaFA-L05-1316-T01-C	1	1.14E+01			1.14E+01	2.94E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1316-T02-C	1	1.59E+01			1.59E+01	5.63E+00	1.2E+00	3.8E+00	10	300	3.30E+03	109%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1316-T03-C	1	2.30E+01			2.30E+01	1.06E+01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1316-T04-C	1	9.96E+00			9.96E+00	3.14E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
Cr	EaFA-L05-1316-T05-C															
Cr	EaFA-L05-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	1.69E+02	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	EaFA-L05-1316-T01-A	1	1.39E+02			1.39E+02	7.87E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1316-T02-A	1	2.70E+02			2.70E+02	4.41E+00	1.8E+00	5.7E+00	10	300	3.41E+03	105%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1316-T03-A	1	9.51E+02			9.51E+02	9.95E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1316-T04-A	1	4.80E+02			4.80E+02	7.82E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1316-T05-A															
Co	EaFA-L05-1316-T01-B	1	1.09E+02			1.09E+02	4.95E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1316-T02-B	1	2.37E+02			2.37E+02	3.23E+00	1.8E+00	5.7E+00	10	300	3.23E+03	100%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1316-T03-B	1	4.07E+02			4.07E+02	1.71E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1316-T04-B	1	7.11E+02			7.11E+02	1.96E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1316-T05-B															
Co	EaFA-L05-1316-T01-C	1	1.53E+02			1.53E+02	8.44E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1316-T02-C	1	1.75E+02			1.75E+02	2.52E+00	1.8E+00	5.7E+00	10	300	3.47E+03	110%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1316-T03-C	1	4.50E+02			4.50E+02	1.31E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1316-T04-C	1	1.48E+03			1.48E+03	1.60E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
Co	EaFA-L05-1316-T05-C															
Co	EaFA-L05-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	1.22E+02	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	EaFA-L05-1316-T01-A	1	3.21E+02			3.21E+02	2.48E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1316-T02-A	1	1.27E+02			1.27E+02	1.03E+01	3.7E+00	1.2E+01	10	300	3.32E+03	107%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1316-T03-A	1	9.50E+01			9.50E+01	4.00E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1316-T04-A	1	1.18E+01	E		1.18E+01	3.45E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1316-T05-A															
Cu	EaFA-L05-1316-T01-B	1	8.74E+01			8.74E+01	1.35E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1316-T02-B	1	5.82E+02			5.82E+02	2.49E+01	3.7E+00	1.2E+01	10	300	3.57E+03	99%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1316-T03-B	1	1.71E+01			1.71E+01	3.66E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1316-T04-B	1	1.09E+01	E		1.09E+01	3.61E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1316-T05-B															
Cu	EaFA-L05-1316-T01-C	1	7.92E+02			7.92E+02	3.54E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1316-T02-C	1	2.04E+01			2.04E+01	1.44E+01	3.7E+00	1.2E+01	10	300	3.36E+03	111%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1316-T03-C	1	1.47E+01			1.47E+01	3.07E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1316-T04-C	1	6.06E+01			6.06E+01	4.14E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
Cu	EaFA-L05-1316-T05-C															
Cu	EaFA-L05-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	2.00E+02	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	EaFA-L05-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	3.99E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	1.35E+02	2.0E+00	6.4E+00	1000	100	9.78E+02	98%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	1.07E+02	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	2.25E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1316-T05-A															
Fe	EaFA-L05-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	9.86E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1316-T02-B	1	5.40E+00	E		5.40E+00	1.12E+03	2.0E+00	6.4E+00	1000	100	9.25E+02	92%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	5.02E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1316-T04-B	1	6.82E+00			6.82E+00	5.14E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1316-T05-B															
Fe	EaFA-L05-1316-T01-C	1	1.30E+01			1.30E+01	2.46E+02	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	8.86E+01	2.0E+00	6.4E+00	1000	100	1.02E+03	102%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	2.20E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	3.54E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
Fe	EaFA-L05-1316-T05-C															
Fe	EaFA-L05-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	1.09E+03	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	EaFA-L05-1316-T01-A	1	3.40E+00	U1/2		3.40E+00	9.16E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1316-T02-A	1	3.40E+00	U1/2		3.40E+00	5.04E+01	6.8E+00	2.2E+01	10	300	3.17E+03	106%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1316-T03-A	1	3.40E+00	U1/2		3.40E+00	1.31E+02	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1316-T04-A	1	3.40E+00	U1/2		3.40E+00	4.69E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1316-T05-A															
Pb	EaFA-L05-1316-T01-B	1	3.40E+00	U1/2		3.40E+00	2.80E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1316-T02-B	1	3.40E+00	U1/2		3.40E+00	3.57E+01	6.8E+00	2.2E+01	10	300	2.97E+03	99%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1316-T03-B	1	3.40E+00	U1/2		3.40E+00	2.16E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1316-T04-B	1	3.40E+00	U1/2		3.40E+00	7.11E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1316-T05-B															
Pb	EaFA-L05-1316-T01-C	1	3.40E+00	U1/2		3.40E+00	3.14E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1316-T02-C	1	3.40E+00	U1/2		3.40E+00	8.98E+01	6.8E+00	2.2E+01	10	300	3.29E+03	110%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1316-T03-C	1	3.40E+00	U1/2		3.40E+00	7.75E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1316-T04-C	1	3.40E+00	U1/2		3.40E+00	3.00E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
Pb	EaFA-L05-1316-T05-C															
Pb	EaFA-L05-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	5.97E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	EaFA-L05-1316-T01-A	1	2.69E+03			2.69E+03	1.64E+00	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1316-T02-A	1	5.28E+03			5.28E+03	6.64E-01	1.9E+00	6.0E+00	10	300	7.94E+03	89%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1316-T03-A	1	1.35E+04			1.35E+04	6.17E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1316-T04-A	1	2.80E+04			2.80E+04	4.86E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1316-T05-A															
Li	EaFA-L05-1316-T01-B	1	2.71E+03			2.71E+03	2.26E+00	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1316-T02-B	1	4.69E+03			4.69E+03	7.06E-01	1.9E+00	6.0E+00	10	300	7.25E+03	85%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1316-T03-B	1	1.38E+04			1.38E+04	5.33E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1316-T04-B	1	2.70E+04			2.70E+04	1.12E+00	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1316-T05-B															
Li	EaFA-L05-1316-T01-C	1	2.58E+03			2.58E+03	4.86E-02	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1316-T02-C	1	4.93E+03			4.93E+03	6.07E-01	1.9E+00	6.0E+00	10	300	7.66E+03	91%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1316-T03-C	1	1.37E+04			1.37E+04	6.98E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1316-T04-C	1	2.65E+04			2.65E+04	1.47E+00	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
Li	EaFA-L05-1316-T05-C															
Li	EaFA-L05-1316-B01-A	1	2.21E+01			2.21E+01	2.59E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	EaFA-L05-1316-T01-A	1	3.61E+02			3.61E+02	3.89E+00	2.0E+00	6.4E+00			---		VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1316-T02-A	1	7.48E+02			7.48E+02	1.07E+00	2.0E+00	6.4E+00	10	300	3.79E+03	101%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1316-T03-A	1	2.81E+03			2.81E+03	5.12E-01	2.0E+00	6.4E+00			---		VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1316-T04-A	1	3.07E+03			3.07E+03	9.60E-01	2.0E+00	6.4E+00			---		VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1316-T05-A															
Mn	EaFA-L05-1316-T01-B	1	3.12E+02			3.12E+02	1.55E+00	2.0E+00	6.4E+00			---		VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1316-T02-B	1	6.27E+02			6.27E+02	1.91E+00	2.0E+00	6.4E+00	10	300	3.51E+03	96%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1316-T03-B	1	2.03E+03			2.03E+03	4.24E-01	2.0E+00	6.4E+00			---		VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1316-T04-B	1	3.84E+03			3.84E+03	6.76E-01	2.0E+00	6.4E+00			---		VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1316-T05-B															
Mn	EaFA-L05-1316-T01-C	1	3.65E+02			3.65E+02	1.31E+00	2.0E+00	6.4E+00			---		VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1316-T02-C	1	5.67E+02			5.67E+02	1.21E+00	2.0E+00	6.4E+00	10	300	3.75E+03	106%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1316-T03-C	1	2.10E+03			2.10E+03	5.71E-01	2.0E+00	6.4E+00			---		VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1316-T04-C	1	5.08E+03			5.08E+03	4.17E-01	2.0E+00	6.4E+00			---		VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
Mn	EaFA-L05-1316-T05-C															
Mn	EaFA-L05-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	1.03E+03	2.0E+00	6.4E+00			---		VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	EaFA-L05-1316-T01-A	1	5.30E+03			5.30E+03	1.44E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1316-T02-A	1	1.14E+04			1.14E+04	1.40E+00	1.0E+00	3.2E+00	1000	100	1.24E+04	103%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1316-T03-A	1	3.49E+04			3.49E+04	6.60E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1316-T04-A	1	7.26E+04			7.26E+04	1.19E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1316-T05-A															
Mg	EaFA-L05-1316-T01-B	1	5.28E+03			5.28E+03	4.57E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1316-T02-B	1	9.73E+03			9.73E+03	7.18E-01	1.0E+00	3.2E+00	1000	100	1.07E+04	93%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1316-T03-B	1	3.85E+04			3.85E+04	2.80E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1316-T04-B	1	6.97E+04			6.97E+04	4.77E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1316-T05-B															
Mg	EaFA-L05-1316-T01-C	1	5.06E+03			5.06E+03	7.09E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1316-T02-C	1	1.03E+04			1.03E+04	2.72E-01	1.0E+00	3.2E+00	1000	100	1.14E+04	108%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1316-T03-C	1	3.84E+04			3.84E+04	3.39E-02	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1316-T04-C	1	6.57E+04			6.57E+04	7.08E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
Mg	EaFA-L05-1316-T05-C															
Mg	EaFA-L05-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.47E+01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	EaFA-L05-1316-T01-A	1	4.56E+02			4.56E+02	2.86E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1316-T02-A	1	9.04E+02			9.04E+02	1.21E+00	1.2E+00	3.8E+00	10	300	4.04E+03	105%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1316-T03-A	1	2.29E+03			2.29E+03	3.54E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1316-T04-A	1	1.39E+04			1.39E+04	1.92E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1316-T05-A															
Mo	EaFA-L05-1316-T01-B	1	1.00E+03			1.00E+03	1.58E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1316-T02-B	1	5.50E+02			5.50E+02	3.58E-01	1.2E+00	3.8E+00	10	300	3.51E+03	99%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1316-T03-B	1	8.48E+03			8.48E+03	2.93E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1316-T04-B	1	1.05E+04			1.05E+04	8.71E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1316-T05-B															
Mo	EaFA-L05-1316-T01-C	1	3.17E+02			3.17E+02	1.04E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1316-T02-C	1	1.98E+03			1.98E+03	5.05E-01	1.2E+00	3.8E+00	10	300	5.11E+03	104%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1316-T03-C	1	8.09E+03			8.09E+03	5.69E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1316-T04-C	1	3.44E+03			3.44E+03	1.33E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
Mo	EaFA-L05-1316-T05-C															
Mo	EaFA-L05-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	2.85E+01	1.2E+00	3.8E+00				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	EaFA-L05-1316-T01-A	1	3.49E+02			3.49E+02	2.94E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1316-T02-A	1	6.33E+02			6.33E+02	5.42E+00	1.8E+00	5.7E+00	10	300	3.75E+03	104%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1316-T03-A	1	2.05E+03			2.05E+03	1.32E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1316-T04-A	1	8.94E+02			8.94E+02	1.82E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1316-T05-A															
Ni	EaFA-L05-1316-T01-B	1	2.76E+02			2.76E+02	1.79E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1316-T02-B	1	5.88E+02			5.88E+02	7.20E-01	1.8E+00	5.7E+00	10	300	3.53E+03	98%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1316-T03-B	1	7.99E+02			7.99E+02	6.39E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1316-T04-B	1	1.30E+03			1.30E+03	1.07E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1316-T05-B															
Ni	EaFA-L05-1316-T01-C	1	3.98E+02			3.98E+02	1.81E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1316-T02-C	1	4.10E+02			4.10E+02	1.07E+00	1.8E+00	5.7E+00	10	300	3.66E+03	108%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1316-T03-C	1	8.91E+02			8.91E+02	8.59E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1316-T04-C	1	2.97E+03			2.97E+03	1.39E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
Ni	EaFA-L05-1316-T05-C															
Ni	EaFA-L05-1316-B01-A	1	2.73E+00	E		2.73E+00	4.32E+02	1.8E+00	5.7E+00				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	EaFA-L05-1316-T01-A	1	2.29E+01			2.29E+01	1.75E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1316-T02-A	1	2.48E+01			2.48E+01	1.88E+01	3.7E+00	1.2E+01	1000	100	1.11E+03	109%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1316-T03-A	1	9.87E+01			9.87E+01	1.33E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1316-T04-A	1	7.70E+01			7.70E+01	1.07E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1316-T05-A															
P	EaFA-L05-1316-T01-B	1	4.57E+01			4.57E+01	1.28E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1316-T02-B	1	1.15E+01	E		1.15E+01	1.64E+01	3.7E+00	1.2E+01	1000	100	1.04E+03	102%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1316-T03-B	1	2.32E+02			2.32E+02	6.72E+00	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1316-T04-B	1	6.07E+01			6.07E+01	2.02E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1316-T05-B															
P	EaFA-L05-1316-T01-C	1	2.03E+01			2.03E+01	1.84E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1316-T02-C	1	8.03E+01			8.03E+01	4.32E+01	3.7E+00	1.2E+01	1000	100	1.16E+03	108%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1316-T03-C	1	1.02E+02			1.02E+02	9.47E-01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1316-T04-C	1	1.58E+02			1.58E+02	1.31E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
P	EaFA-L05-1316-T05-C															
P	EaFA-L05-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	1.08E+02	3.7E+00	1.2E+01				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	EaFA-L05-1316-T01-A	1	2.21E+04			2.21E+04	1.27E+00	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1316-T02-A	1	4.76E+04			4.76E+04	1.19E+00	1.6E+00	5.1E+00	1000	100	4.85E+04	85%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1316-T03-A	1	1.25E+05			1.25E+05	1.88E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1316-T04-A	1	2.13E+05			2.13E+05	5.49E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1316-T05-A															
K	EaFA-L05-1316-T01-B	1	2.30E+04			2.30E+04	1.07E+00	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1316-T02-B	1	4.12E+04			4.12E+04	8.12E-01	1.6E+00	5.1E+00	1000	100	4.21E+04	92%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1316-T03-B	1	1.28E+05			1.28E+05	6.11E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1316-T04-B	1	2.06E+05			2.06E+05	1.41E+00	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1316-T05-B															
K	EaFA-L05-1316-T01-C	1	2.08E+04			2.08E+04	5.06E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1316-T02-C	1	4.46E+04			4.46E+04	9.50E-01	1.6E+00	5.1E+00	1000	100	4.55E+04	90%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1316-T03-C	1	1.30E+05			1.30E+05	2.05E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1316-T04-C	1	1.96E+05			1.96E+05	1.69E+00	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
K	EaFA-L05-1316-T05-C															
K	EaFA-L05-1316-B01-A	1	1.07E+01			1.07E+01	1.98E+01	1.6E+00	5.1E+00				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	EaFA-L05-1316-T01-A	1	3.60E+02			3.60E+02	5.23E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1316-T02-A	1	4.55E+02			4.55E+02	2.59E+00	1.5E+01	4.8E+01	10	300	3.68E+03	108%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1316-T03-A	1	5.78E+02			5.78E+02	1.33E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1316-T04-A	1	1.11E+03			1.11E+03	1.60E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1316-T05-A															
Se	EaFA-L05-1316-T01-B	1	4.60E+02			4.60E+02	3.17E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1316-T02-B	1	3.69E+02			3.69E+02	1.51E+00	1.5E+01	4.8E+01	10	300	3.40E+03	101%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1316-T03-B	1	8.78E+02			8.78E+02	3.54E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1316-T04-B	1	1.07E+03			1.07E+03	9.30E-01	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1316-T05-B															
Se	EaFA-L05-1316-T01-C	1	2.90E+02			2.90E+02	3.30E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1316-T02-C	1	5.33E+02			5.33E+02	1.74E+00	1.5E+01	4.8E+01	10	300	3.85E+03	111%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1316-T03-C	1	8.53E+02			8.53E+02	5.13E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1316-T04-C	1	7.36E+02			7.36E+02	4.68E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
Se	EaFA-L05-1316-T05-C															
Se	EaFA-L05-1316-B01-A	1	7.50E+00	U1/2		7.50E+00	2.80E+02	1.5E+01	4.8E+01				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	EaFA-L05-1316-T01-A	1	1.82E+03			1.82E+03	1.16E+00	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1316-T02-A	1	3.53E+03			3.53E+03	1.53E+00	1.1E+00	3.5E+00	1000	100	4.55E+03	102%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1316-T03-A	1	8.76E+03			8.76E+03	5.55E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1316-T04-A	1	3.11E+03			3.11E+03	1.06E+00	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1316-T05-A															
Si	EaFA-L05-1316-T01-B	1	1.65E+03			1.65E+03	1.87E+00	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1316-T02-B	1	2.91E+03			2.91E+03	7.64E-01	1.1E+00	3.5E+00	1000	100	3.87E+03	97%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1316-T03-B	1	3.09E+03			3.09E+03	6.59E-02	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1316-T04-B	1	4.10E+03			4.10E+03	1.44E+00	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1316-T05-B															
Si	EaFA-L05-1316-T01-C	1	1.84E+03			1.84E+03	4.77E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1316-T02-C	1	2.73E+03			2.73E+03	5.71E-01	1.1E+00	3.5E+00	1000	100	3.87E+03	114%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1316-T03-C	1	3.39E+03			3.39E+03	5.28E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1316-T04-C	1	1.02E+04			1.02E+04	1.12E+00	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
Si	EaFA-L05-1316-T05-C															
Si	EaFA-L05-1316-B01-A	1	4.30E+00			4.30E+00	1.67E+01	1.1E+00	3.5E+00				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	EaFA-L05-1316-T01-A	1	4.37E+03			4.37E+03	1.37E+00	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1316-T02-A	1	9.41E+03			9.41E+03	9.77E-01	2.5E+00	8.0E+00	1000	100	1.03E+04	94%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1316-T03-A	1	2.46E+04			2.46E+04	1.98E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1316-T04-A	1	4.35E+04			4.35E+04	1.19E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1316-T05-A															
Na	EaFA-L05-1316-T01-B	1	4.51E+03			4.51E+03	2.39E+00	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1316-T02-B	1	8.12E+03			8.12E+03	3.01E-01	2.5E+00	8.0E+00	1000	100	9.01E+03	89%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1316-T03-B	1	2.55E+04			2.55E+04	4.43E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1316-T04-B	1	4.19E+04			4.19E+04	1.52E+00	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1316-T05-B															
Na	EaFA-L05-1316-T01-C	1	4.20E+03			4.20E+03	7.87E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1316-T02-C	1	8.67E+03			8.67E+03	8.75E-01	2.5E+00	8.0E+00	1000	100	9.61E+03	94%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1316-T03-C	1	2.57E+04			2.57E+04	4.51E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1316-T04-C	1	4.04E+04			4.04E+04	1.17E+00	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
Na	EaFA-L05-1316-T05-C															
Na	EaFA-L05-1316-B01-A	1	1.38E+01			1.38E+01	1.66E+00	2.5E+00	8.0E+00				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	EaFA-L05-1316-T01-A	1	1.76E+03			1.76E+03	2.89E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1316-T02-A	1	3.67E+03			3.67E+03	1.23E+00	1.0E+00	3.2E+00	1000	100	4.73E+03	105%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1316-T03-A	1	8.83E+03			8.83E+03	9.39E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1316-T04-A	1	8.48E+03			8.48E+03	1.19E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1316-T05-A															
Sr	EaFA-L05-1316-T01-B	1	1.76E+03			1.76E+03	4.99E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1316-T02-B	1	2.90E+03			2.90E+03	1.27E+00	1.0E+00	3.2E+00	1000	100	3.85E+03	95%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1316-T03-B	1	8.49E+03			8.49E+03	2.17E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1316-T04-B	1	8.73E+03			8.73E+03	4.33E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1316-T05-B															
Sr	EaFA-L05-1316-T01-C	1	1.93E+03			1.93E+03	1.09E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1316-T02-C	1	2.98E+03			2.98E+03	9.93E-01	1.0E+00	3.2E+00	1000	100	3.97E+03	99%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1316-T03-C	1	8.68E+03			8.68E+03	9.82E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1316-T04-C	1	1.00E+04			1.00E+04	4.42E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
Sr	EaFA-L05-1316-T05-C															
Sr	EaFA-L05-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.81E+02	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	EaFA-L05-1316-T01-A	1	1.22E+05			1.22E+05	1.03E+00	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1316-T02-A	1	2.69E+05			2.69E+05	1.25E+00	6.8E+00	2.2E+01	1000	100	3.53E+05	84%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1316-T03-A	1	6.90E+05			6.90E+05	5.99E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1316-T04-A	1	8.01E+05			8.01E+05	1.65E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1316-T05-A															
S	EaFA-L05-1316-T01-B	1	1.27E+05			1.27E+05	2.00E+00	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1316-T02-B	1	2.22E+05			2.22E+05	6.88E-01	6.8E+00	2.2E+01	1000	100	3.02E+05	80%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1316-T03-B	1	7.55E+05			7.55E+05	8.23E-02	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1316-T04-B	1	7.94E+05			7.94E+05	1.00E+00	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1316-T05-B															
S	EaFA-L05-1316-T01-C	1	1.33E+05			1.33E+05	5.13E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1316-T02-C	1	2.37E+05			2.37E+05	3.81E-01	6.8E+00	2.2E+01	1000	100	3.22E+05	85%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1316-T03-C	1	7.67E+05			7.67E+05	4.33E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1316-T04-C	1	7.63E+05			7.63E+05	8.38E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
S	EaFA-L05-1316-T05-C															
S	EaFA-L05-1316-B01-A	1	1.09E+01	E		1.09E+01	2.82E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	EaFA-L05-1316-T01-A	1	1.43E+01	E		1.43E+01	1.99E+03	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1316-T02-A	1	3.11E+01			3.11E+01	5.13E+01	4.6E+00	1.5E+01	10	300	3.14E+03	104%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1316-T03-A	1	4.69E+01			4.69E+01	7.29E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1316-T04-A	1	1.07E+01	E		1.07E+01	4.03E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1316-T05-A															
Tl	EaFA-L05-1316-T01-B	1	2.30E+00	U1/2		2.30E+00	4.89E+02	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1316-T02-B	1	2.28E+01			2.28E+01	7.52E+01	4.6E+00	1.5E+01	10	300	2.98E+03	99%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1316-T03-B	1	2.30E+00	U1/2		2.30E+00	1.33E+02	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1316-T04-B	1	2.50E+01			2.50E+01	5.15E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1316-T05-B															
Tl	EaFA-L05-1316-T01-C	1	2.24E+01			2.24E+01	1.28E+02	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1316-T02-C	1	7.67E+00	E		7.67E+00	1.89E+02	4.6E+00	1.5E+01	10	300	3.25E+03	108%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1316-T03-C	1	5.24E+00	E		5.24E+00	1.36E+02	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1316-T04-C	1	6.52E+01			6.52E+01	8.83E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
Tl	EaFA-L05-1316-T05-C															
Tl	EaFA-L05-1316-B01-A	1	2.30E+00	U1/2		2.30E+00	8.63E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	EaFA-L05-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	4.63E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	3.00E+02	2.0E+00	6.4E+00	10	300	3.15E+03	105%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	8.48E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	1.30E+02	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1316-T05-A															
Ti	EaFA-L05-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	6.08E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	9.44E+01	2.0E+00	6.4E+00	10	300	2.95E+03	98%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	1.13E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	8.51E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1316-T05-B															
Ti	EaFA-L05-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	1.96E+02	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	2.89E+02	2.0E+00	6.4E+00	10	300	3.25E+03	108%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	4.42E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	1.42E+02	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
Ti	EaFA-L05-1316-T05-C															
Ti	EaFA-L05-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	8.58E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	EaFA-L05-1316-T01-A	1	7.65E+01			7.65E+01	3.36E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1316-T02-A	1	1.28E+02			1.28E+02	1.42E-01	1.5E+00	4.8E+00	10	300	3.28E+03	105%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1316-T03-A	1	1.91E+02			1.91E+02	2.81E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1316-T04-A	1	2.03E+02			2.03E+02	3.78E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1316-T05-A															
V	EaFA-L05-1316-T01-B	1	9.02E+01			9.02E+01	2.93E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1316-T02-B	1	9.91E+01			9.91E+01	8.97E-01	1.5E+00	4.8E+00	10	300	3.08E+03	99%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1316-T03-B	1	2.08E+02			2.08E+02	6.55E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1316-T04-B	1	2.14E+02			2.14E+02	9.35E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1316-T05-B															
V	EaFA-L05-1316-T01-C	1	6.87E+01			6.87E+01	5.17E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1316-T02-C	1	1.19E+02			1.19E+02	5.55E-01	1.5E+00	4.8E+00	10	300	3.41E+03	110%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1316-T03-C	1	2.14E+02			2.14E+02	4.66E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1316-T04-C	1	1.89E+02			1.89E+02	1.58E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
V	EaFA-L05-1316-T05-C															
V	EaFA-L05-1316-B01-A	1	2.61E+00	E		2.61E+00	5.98E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	EaFA-L05-1316-T01-A	1	6.71E+02			6.71E+02	4.18E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:10 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1316-T02-A	1	1.02E+03			1.02E+03	5.62E+00	1.0E+00	3.2E+00	10	300	4.18E+03	105%	VU ICP-OES	7/29/10 1:12 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1316-T03-A	1	2.65E+03			2.65E+03	6.15E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:14 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1316-T04-A	1	1.48E+02			1.48E+02	1.24E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:15 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1316-T05-A															
Zn	EaFA-L05-1316-T01-B	1	4.54E+02			4.54E+02	2.61E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:17 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1316-T02-B	1	1.12E+03			1.12E+03	3.23E+00	1.0E+00	3.2E+00	10	300	4.11E+03	100%	VU ICP-OES	7/29/10 1:18 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1316-T03-B	1	1.52E+02			1.52E+02	1.82E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:20 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1316-T04-B	1	3.01E+02			3.01E+02	1.02E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:22 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1316-T05-B															
Zn	EaFA-L05-1316-T01-C	1	8.19E+02			8.19E+02	4.07E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:23 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1316-T02-C	1	3.25E+02			3.25E+02	3.67E+00	1.0E+00	3.2E+00	10	300	3.69E+03	112%	VU ICP-OES	7/29/10 1:25 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1316-T03-C	1	1.94E+02			1.94E+02	2.10E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:27 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1316-T04-C	1	2.96E+03			2.96E+03	2.72E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:28 PM	EPA Interlab L05 1313-1316 EaFA
Zn	EaFA-L05-1316-T05-C															
Zn	EaFA-L05-1316-B01-A	1	1.18E+01			1.18E+01	4.14E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/29/10 1:05 PM	EPA Interlab L05 1313-1316 EaFA

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	EaFA-L06-1316-T01-A	1	9.05E+01			9.05E+01	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1316-T02-A	1	1.16E+02			1.16E+02	2.7E+00	1.0E+00	3.2E+00	1000	100	1.06E+03	94%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1316-T03-A	1	2.01E+02			2.01E+02	9.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1316-T04-A	1	3.76E+02			3.76E+02	9.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1316-T05-A	1	5.71E+02			5.71E+02	1.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1316-T01-B	1	1.25E+02			1.25E+02	7.6E-02	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1316-T02-B	1	1.43E+02			1.43E+02	4.7E+00	1.0E+00	3.2E+00	1000	100	1.13E+03	99%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1316-T03-B	1	2.25E+02			2.25E+02	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1316-T04-B	1	5.35E+02			5.35E+02	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1316-T05-B	1	9.78E+02			9.78E+02	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1316-T01-C	1	1.31E+02			1.31E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1316-T02-C	1	1.39E+02			1.39E+02	1.4E+00	1.0E+00	3.2E+00	1000	100	1.07E+03	93%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1316-T03-C	1	2.57E+02			2.57E+02	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1316-T04-C	1	4.98E+02			4.98E+02	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1316-T05-C	1	1.92E+03			1.92E+03	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
Al	EaFA-L06-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	7.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	EaFA-L06-1316-T01-A	1	2.12E+02			2.12E+02	8.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1316-T02-A	1	2.83E+02			2.83E+02	3.2E+00	7.5E+00	2.4E+01	10	300	3.41E+03	104%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1316-T03-A	1	4.30E+02			4.30E+02	3.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1316-T04-A	1	5.06E+02			5.06E+02	1.4E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1316-T05-A	1	5.67E+02			5.67E+02	1.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1316-T01-B	1	2.15E+02			2.15E+02	4.9E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1316-T02-B	1	3.23E+02			3.23E+02	4.5E+00	7.5E+00	2.4E+01	10	300	3.51E+03	106%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1316-T03-B	1	4.41E+02			4.41E+02	1.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1316-T04-B	1	6.10E+02			6.10E+02	5.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1316-T05-B	1	7.56E+02			7.56E+02	4.0E-01	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1316-T01-C	1	1.87E+02			1.87E+02	8.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1316-T02-C	1	3.15E+02			3.15E+02	5.6E+00	7.5E+00	2.4E+01	10	300	3.37E+03	102%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1316-T03-C	1	4.13E+02			4.13E+02	3.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1316-T04-C	1	5.52E+02			5.52E+02	5.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1316-T05-C	1	7.92E+02			7.92E+02	3.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
Sb	EaFA-L06-1316-B01-A	1	3.75E+00	U1/2		3.75E+00	1.3E+02	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	EaFA-L06-1316-T01-A	1	1.13E+02			1.13E+02	9.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1316-T02-A	1	1.29E+02			1.29E+02	2.6E+01	1.1E+01	3.5E+01	10	300	3.29E+03	105%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1316-T03-A	1	1.37E+02			1.37E+02	5.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1316-T04-A	1	1.39E+02			1.39E+02	1.9E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1316-T05-A	1	1.44E+02			1.44E+02	3.1E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1316-T01-B	1	9.73E+01			9.73E+01	2.0E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1316-T02-B	1	8.03E+01			8.03E+01	1.8E+01	1.1E+01	3.5E+01	10	300	3.41E+03	111%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1316-T03-B	1	1.22E+02			1.22E+02	4.2E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1316-T04-B	1	1.48E+02			1.48E+02	1.5E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1316-T05-B	1	1.68E+02			1.68E+02	1.6E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1316-T01-C	1	9.41E+01			9.41E+01	1.8E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1316-T02-C	1	8.99E+01			8.99E+01	2.2E+01	1.1E+01	3.5E+01	10	300	3.22E+03	104%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1316-T03-C	1	1.11E+02			1.11E+02	1.2E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1316-T04-C	1	1.34E+02			1.34E+02	7.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1316-T05-C	1	5.09E+02			5.09E+02	4.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
As	EaFA-L06-1316-B01-A	1	5.50E+00	U1/2		5.50E+00	9.5E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	EaFA-L06-1316-T01-A	1	4.15E+03			4.15E+03	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1316-T02-A	1	8.08E+03			8.08E+03	3.5E-01	1.0E+00	3.2E+00	1000	100	9.02E+03	94%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1316-T03-A	1	2.05E+04			2.05E+04	2.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1316-T04-A	1	3.21E+04			3.21E+04	1.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1316-T05-A	1	4.94E+04			4.94E+04	1.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1316-T01-B	1	5.06E+03			5.06E+03	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1316-T02-B	1	8.86E+03			8.86E+03	5.3E-01	1.0E+00	3.2E+00	1000	100	9.74E+03	88%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1316-T03-B	1	2.12E+04			2.12E+04	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1316-T04-B	1	3.78E+04			3.78E+04	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1316-T05-B	1	6.51E+04			6.51E+04	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1316-T01-C	1	6.21E+03			6.21E+03	2.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1316-T02-C	1	9.60E+03			9.60E+03	4.3E-01	1.0E+00	3.2E+00	1000	100	1.05E+04	91%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1316-T03-C	1	1.98E+04			1.98E+04	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1316-T04-C	1	3.63E+04			3.63E+04	2.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1316-T05-C	1	5.52E+04			5.52E+04	9.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
B	EaFA-L06-1316-B01-A	1	2.20E+01			2.20E+01	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	EaFA-L06-1316-T01-A	1	2.71E+02			2.71E+02	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1316-T02-A	1	2.19E+02			2.19E+02	3.1E-01	1.0E+00	3.2E+00	10	300	3.07E+03	95%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1316-T03-A	1	2.20E+02			2.20E+02	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1316-T04-A	1	2.25E+02			2.25E+02	9.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1316-T05-A	1	2.15E+02			2.15E+02	1.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1316-T01-B	1	3.00E+02			3.00E+02	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1316-T02-B	1	2.46E+02			2.46E+02	4.3E-01	1.0E+00	3.2E+00	10	300	3.21E+03	99%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1316-T03-B	1	2.30E+02			2.30E+02	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1316-T04-B	1	2.68E+02			2.68E+02	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1316-T05-B	1	3.07E+02			3.07E+02	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1316-T01-C	1	2.90E+02			2.90E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1316-T02-C	1	2.48E+02			2.48E+02	3.6E-01	1.0E+00	3.2E+00	10	300	3.06E+03	94%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1316-T03-C	1	2.22E+02			2.22E+02	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1316-T04-C	1	2.49E+02			2.49E+02	5.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1316-T05-C	1	3.66E+02			3.66E+02	3.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
Ba	EaFA-L06-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	4.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	EaFA-L06-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	6.9E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	5.2E+03	1.9E+00	6.0E+00	10	300	3.13E+03	104%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	6.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	7.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1316-T05-A	1	9.50E-01	U1/2		9.50E-01	5.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	3.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	4.3E+02	1.9E+00	6.0E+00	10	300	3.29E+03	110%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	9.9E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	5.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1316-T05-B	1	9.50E-01	U1/2		9.50E-01	1.7E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	2.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	2.6E+01	1.9E+00	6.0E+00	10	300	3.10E+03	103%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	2.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1316-T05-C	1	9.50E-01	U1/2		9.50E-01	1.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
Be	EaFA-L06-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	4.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	EaFA-L06-1316-T01-A	1	1.10E+00	U1/2		1.10E+00	2.9E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1316-T02-A	1	3.25E+00	E		3.25E+00	1.9E+01	2.2E+00	7.0E+00	10	300	3.08E+03	102%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1316-T03-A	1	6.37E+00	E		6.37E+00	1.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1316-T04-A	1	1.10E+00	U1/2		1.10E+00	2.4E+02	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1316-T05-A	1	1.10E+00	U1/2		1.10E+00	1.2E+02	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1316-T01-B	1	1.10E+00	U1/2		1.10E+00	6.0E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1316-T02-B	1	1.10E+00	U1/2		1.10E+00	2.2E+01	2.2E+00	7.0E+00	10	300	3.23E+03	108%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1316-T03-B	1	6.02E+00	E		6.02E+00	8.6E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1316-T04-B	1	1.10E+00	U1/2		1.10E+00	2.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1316-T05-B	1	2.92E+00	E		2.92E+00	9.7E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1316-T01-C	1	1.10E+00	U1/2		1.10E+00	1.2E+02	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1316-T02-C	1	3.08E+00	E		3.08E+00	3.0E+01	2.2E+00	7.0E+00	10	300	3.06E+03	102%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1316-T03-C	1	1.10E+00	U1/2		1.10E+00	1.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1316-T04-C	1	1.10E+00	U1/2		1.10E+00	1.5E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1316-T05-C	1	1.10E+00	U1/2		1.10E+00	1.7E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
Cd	EaFA-L06-1316-B01-A	1	1.10E+00	U1/2		1.10E+00	5.4E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	EaFA-L06-1316-T01-A	1	1.59E+05			1.59E+05	7.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1316-T02-A	1	3.06E+05			3.06E+05	5.8E-01	2.6E+00	8.3E+00	1000	100	3.07E+05	88%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1316-T03-A	1	7.27E+05			7.27E+05	4.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1316-T04-A	1	5.06E+05			5.06E+05	9.6E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1316-T05-A	1	4.39E+05			4.39E+05	1.3E+01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1316-T01-B	1	1.63E+05			1.63E+05	6.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1316-T02-B	1	3.42E+05			3.42E+05	5.8E-01	2.6E+00	8.3E+00	1000	100	3.43E+05	83%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1316-T03-B	1	7.75E+05			7.75E+05	1.8E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1316-T04-B	1	6.31E+05			6.31E+05	8.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1316-T05-B	1	5.64E+05			5.64E+05	5.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1316-T01-C	1	1.92E+05			1.92E+05	1.9E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1316-T02-C	1	3.44E+05			3.44E+05	7.7E-01	2.6E+00	8.3E+00	1000	100	3.45E+05	90%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1316-T03-C	1	7.24E+05			7.24E+05	1.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1316-T04-C	1	5.80E+05			5.80E+05	9.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1316-T05-C	1	5.67E+05			5.67E+05	6.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
Ca	EaFA-L06-1316-B01-A	1	2.09E+01			2.09E+01	3.1E+01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	EaFA-L06-1316-T01-A	1	6.66E+00			6.66E+00	3.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1316-T02-A	1	8.79E+00			8.79E+00	7.4E+00	1.2E+00	3.8E+00	10	300	3.18E+03	106%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1316-T03-A	1	1.55E+01			1.55E+01	4.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1316-T04-A	1	5.25E+01			5.25E+01	1.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1316-T05-A	1	5.34E+01			5.34E+01	1.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1316-T01-B	1	1.52E+01			1.52E+01	9.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1316-T02-B	1	1.24E+01			1.24E+01	4.0E+00	1.2E+00	3.8E+00	10	300	3.25E+03	108%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1316-T03-B	1	2.14E+01			2.14E+01	1.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1316-T04-B	1	8.21E+01			8.21E+01	1.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1316-T05-B	1	3.66E+01			3.66E+01	2.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1316-T01-C	1	1.61E+01			1.61E+01	1.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1316-T02-C	1	1.17E+01			1.17E+01	1.2E+01	1.2E+00	3.8E+00	10	300	3.04E+03	101%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1316-T03-C	1	3.21E+01			3.21E+01	2.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1316-T04-C	1	7.46E+01			7.46E+01	2.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1316-T05-C	1	9.52E+01			9.52E+01	2.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
Cr	EaFA-L06-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	3.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	EaFA-L06-1316-T01-A	1	8.93E+01			8.93E+01	2.7E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1316-T02-A	1	1.51E+02			1.51E+02	1.9E+00	1.8E+00	5.7E+00	10	300	3.30E+03	105%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1316-T03-A	1	2.61E+02			2.61E+02	6.0E-01	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1316-T04-A	1	9.23E+01			9.23E+01	9.5E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1316-T05-A	1	9.43E+01			9.43E+01	1.2E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1316-T01-B	1	5.99E+01			5.99E+01	4.1E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1316-T02-B	1	1.34E+02			1.34E+02	3.0E+00	1.8E+00	5.7E+00	10	300	3.35E+03	107%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1316-T03-B	1	2.39E+02			2.39E+02	2.7E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1316-T04-B	1	8.94E+01			8.94E+01	1.1E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1316-T05-B	1	2.07E+02			2.07E+02	2.3E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1316-T01-C	1	7.25E+01			7.25E+01	1.2E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1316-T02-C	1	1.63E+02			1.63E+02	2.1E+00	1.8E+00	5.7E+00	10	300	3.18E+03	101%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1316-T03-C	1	1.40E+02			1.40E+02	9.1E-01	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1316-T04-C	1	7.52E+01			7.52E+01	2.7E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1316-T05-C	1	1.94E+01			1.94E+01	5.7E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
Co	EaFA-L06-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	1.7E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	EaFA-L06-1316-T01-A	1	5.31E+00	E		5.31E+00	5.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1316-T02-A	1	3.81E+01			3.81E+01	9.0E+00	3.7E+00	1.2E+01	10	300	3.24E+03	107%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1316-T03-A	1	1.04E+01	E		1.04E+01	5.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1316-T04-A	1	7.09E+00	E		7.09E+00	5.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1316-T05-A	1	1.85E+00	U1/2		1.85E+00	2.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1316-T01-B	1	5.33E+00	E		5.33E+00	8.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1316-T02-B	1	4.17E+00	E		4.17E+00	8.4E+01	3.7E+00	1.2E+01	10	300	3.31E+03	110%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1316-T03-B	1	7.03E+00	E		7.03E+00	8.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1316-T04-B	1	1.32E+01			1.32E+01	4.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1316-T05-B	1	1.33E+01			1.33E+01	1.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1316-T01-C	1	4.48E+00	E		4.48E+00	8.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1316-T02-C	1	9.53E+00	E		9.53E+00	3.7E+01	3.7E+00	1.2E+01	10	300	3.12E+03	104%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1316-T03-C	1	6.91E+00	E		6.91E+00	1.1E+02	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1316-T04-C	1	6.45E+00	E		6.45E+00	3.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1316-T05-C	1	1.39E+01			1.39E+01	3.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
Cu	EaFA-L06-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	7.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	EaFA-L06-1316-T01-A	1	2.22E+00	E		2.22E+00	8.9E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1316-T02-A	1	3.04E+00	E		3.04E+00	2.2E+01	2.0E+00	6.4E+00	1000	100	9.97E+02	99%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1316-T03-A	1	2.69E+00	E		2.69E+00	1.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1316-T04-A	1	2.42E+00	E		2.42E+00	3.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1316-T05-A	1	1.00E+00	U1/2		1.00E+00	3.9E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	2.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1316-T02-B	1	2.18E+00	E		2.18E+00	8.3E+00	2.0E+00	6.4E+00	1000	100	1.02E+03	102%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	2.6E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1316-T05-B	1	1.00E+00	U1/2		1.00E+00	2.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	7.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1316-T02-C	1	2.82E+00	E		2.82E+00	1.2E+01	2.0E+00	6.4E+00	1000	100	9.50E+02	95%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1316-T05-C	1	2.40E+01			2.40E+01	1.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
Fe	EaFA-L06-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	8.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	EaFA-L06-1316-T01-A	1	3.40E+00	U1/2		3.40E+00	3.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1316-T02-A	1	3.40E+00	U1/2		3.40E+00	8.4E+01	6.8E+00	2.2E+01	10	300	3.06E+03	102%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1316-T03-A	1	3.40E+00	U1/2		3.40E+00	3.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1316-T04-A	1	3.40E+00	U1/2		3.40E+00	5.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1316-T05-A	1	3.40E+00	U1/2		3.40E+00	2.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1316-T01-B	1	3.40E+00	U1/2		3.40E+00	3.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1316-T02-B	1	3.40E+00	U1/2		3.40E+00	3.5E+00	6.8E+00	2.2E+01	10	300	3.20E+03	106%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1316-T03-B	1	3.40E+00	U1/2		3.40E+00	4.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1316-T04-B	1	3.40E+00	U1/2		3.40E+00	7.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1316-T05-B	1	3.40E+00	U1/2		3.40E+00	2.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1316-T01-C	1	3.40E+00	U1/2		3.40E+00	7.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1316-T02-C	1	3.40E+00	U1/2		3.40E+00	6.1E+01	6.8E+00	2.2E+01	10	300	3.03E+03	101%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1316-T03-C	1	3.40E+00	U1/2		3.40E+00	3.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1316-T04-C	1	3.40E+00	U1/2		3.40E+00	9.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1316-T05-C	1	3.40E+00	U1/2		3.40E+00	3.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
Pb	EaFA-L06-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	3.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	EaFA-L06-1316-T01-A	1	3.74E+03			3.74E+03	6.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1316-T02-A	1	7.05E+03			7.05E+03	5.7E-01	1.9E+00	6.0E+00	10	300	9.91E+03	95%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1316-T03-A	1	1.70E+04			1.70E+04	8.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1316-T04-A	1	2.92E+04			2.92E+04	9.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1316-T05-A	1	5.25E+04			5.25E+04	1.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1316-T01-B	1	3.83E+03			3.83E+03	1.2E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1316-T02-B	1	7.75E+03			7.75E+03	7.2E-01	1.9E+00	6.0E+00	10	300	1.04E+04	88%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1316-T03-B	1	1.80E+04			1.80E+04	2.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1316-T04-B	1	3.58E+04			3.58E+04	1.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1316-T05-B	1	7.03E+04			7.03E+04	4.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1316-T01-C	1	4.58E+03			4.58E+03	1.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1316-T02-C	1	7.85E+03			7.85E+03	4.8E-01	1.9E+00	6.0E+00	10	300	1.06E+04	90%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1316-T03-C	1	1.67E+04			1.67E+04	1.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1316-T04-C	1	3.33E+04			3.33E+04	8.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1316-T05-C	1	5.60E+04			5.60E+04	4.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
Li	EaFA-L06-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	EaFA-L06-1316-T01-A	1	5.12E+02			5.12E+02	1.5E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1316-T02-A	1	8.94E+02			8.94E+02	1.3E+00	2.0E+00	6.4E+00	10	300	3.83E+03	98%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1316-T03-A	1	1.69E+03			1.69E+03	3.2E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1316-T04-A	1	8.66E+02			8.66E+02	1.6E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1316-T05-A	1	1.11E+03			1.11E+03	1.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1316-T01-B	1	4.01E+02			4.01E+02	8.3E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1316-T02-B	1	8.39E+02			8.39E+02	6.4E-01	2.0E+00	6.4E+00	10	300	3.88E+03	101%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1316-T03-B	1	1.57E+03			1.57E+03	2.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1316-T04-B	1	8.89E+02			8.89E+02	1.5E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1316-T05-B	1	2.17E+03			2.17E+03	5.6E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1316-T01-C	1	4.47E+02			4.47E+02	3.4E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1316-T02-C	1	9.48E+02			9.48E+02	2.2E+00	2.0E+00	6.4E+00	10	300	3.75E+03	93%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1316-T03-C	1	1.15E+03			1.15E+03	2.4E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1316-T04-C	1	7.97E+02			7.97E+02	7.9E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1316-T05-C	1	3.64E+02			3.64E+02	3.3E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
Mn	EaFA-L06-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	EaFA-L06-1316-T01-A	1	7.33E+03			7.33E+03	1.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1316-T02-A	1	1.41E+04			1.41E+04	1.4E-01	1.0E+00	3.2E+00	1000	100	1.50E+04	98%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1316-T03-A	1	3.73E+04			3.73E+04	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1316-T04-A	1	6.09E+04			6.09E+04	8.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1316-T05-A	1	1.00E+05			1.00E+05	1.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1316-T01-B	1	7.63E+03			7.63E+03	3.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1316-T02-B	1	1.59E+04			1.59E+04	1.2E+00	1.0E+00	3.2E+00	1000	100	1.68E+04	93%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1316-T03-B	1	3.96E+04			3.96E+04	3.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1316-T04-B	1	7.40E+04			7.40E+04	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1316-T05-B	1	1.39E+05			1.39E+05	2.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1316-T01-C	1	8.63E+03			8.63E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1316-T02-C	1	1.60E+04			1.60E+04	1.2E+00	1.0E+00	3.2E+00	1000	100	1.71E+04	112%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1316-T03-C	1	3.65E+04			3.65E+04	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1316-T04-C	1	6.93E+04			6.93E+04	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1316-T05-C	1	1.02E+05			1.02E+05	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
Mg	EaFA-L06-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	8.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	EaFA-L06-1316-T01-A	1	3.08E+03			3.08E+03	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1316-T02-A	1	5.50E+03			5.50E+03	3.9E-01	1.2E+00	3.8E+00	10	300	8.28E+03	93%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1316-T03-A	1	1.30E+04			1.30E+04	9.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1316-T04-A	1	2.50E+04			2.50E+04	9.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1316-T05-A	1	4.00E+04			4.00E+04	1.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1316-T01-B	1	3.32E+03			3.32E+03	9.7E-02	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1316-T02-B	1	6.30E+03			6.30E+03	7.2E-01	1.2E+00	3.8E+00	10	300	8.77E+03	82%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1316-T03-B	1	1.38E+04			1.38E+04	1.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1316-T04-B	1	3.12E+04			3.12E+04	9.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1316-T05-B	1	4.68E+04			4.68E+04	4.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1316-T01-C	1	3.49E+03			3.49E+03	6.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1316-T02-C	1	6.16E+03			6.16E+03	2.4E-01	1.2E+00	3.8E+00	10	300	8.83E+03	89%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1316-T03-C	1	1.43E+04			1.43E+04	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1316-T04-C	1	2.91E+04			2.91E+04	9.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1316-T05-C	1	5.63E+04			5.63E+04	5.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
Mo	EaFA-L06-1316-B01-A	1	2.41E+00	E		2.41E+00	1.1E+02	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	EaFA-L06-1316-T01-A	1	2.04E+02			2.04E+02	2.0E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1316-T02-A	1	3.51E+02			3.51E+02	8.7E-01	1.8E+00	5.7E+00	10	300	3.50E+03	105%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1316-T03-A	1	6.06E+02			6.06E+02	1.7E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1316-T04-A	1	2.34E+02			2.34E+02	1.1E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1316-T05-A	1	2.35E+02			2.35E+02	1.3E+01	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1316-T01-B	1	1.47E+02			1.47E+02	2.7E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1316-T02-B	1	3.17E+02			3.17E+02	2.1E+00	1.8E+00	5.7E+00	10	300	3.52E+03	107%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1316-T03-B	1	5.36E+02			5.36E+02	2.1E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1316-T04-B	1	2.10E+02			2.10E+02	2.0E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1316-T05-B	1	4.74E+02			4.74E+02	3.2E-01	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1316-T01-C	1	1.72E+02			1.72E+02	3.9E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1316-T02-C	1	3.66E+02			3.66E+02	2.1E+00	1.8E+00	5.7E+00	10	300	3.37E+03	100%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1316-T03-C	1	3.32E+02			3.32E+02	1.3E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1316-T04-C	1	1.89E+02			1.89E+02	3.0E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1316-T05-C	1	7.26E+01			7.26E+01	1.8E+00	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
Ni	EaFA-L06-1316-B01-A	1	2.37E+00	E		2.37E+00	2.0E+02	1.8E+00	5.7E+00			---		VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	EaFA-L06-1316-T01-A	1	6.45E+01			6.45E+01	5.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1316-T02-A	1	6.36E+01			6.36E+01	2.4E+01	3.7E+00	1.2E+01	1000	100	1.01E+03	95%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1316-T03-A	1	9.74E+01			9.74E+01	6.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1316-T04-A	1	9.30E+01			9.30E+01	1.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1316-T05-A	1	1.19E+02			1.19E+02	1.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1316-T01-B	1	6.66E+01			6.66E+01	7.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1316-T02-B	1	5.85E+01			5.85E+01	1.7E+01	3.7E+00	1.2E+01	1000	100	1.09E+03	103%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1316-T03-B	1	9.51E+01			9.51E+01	1.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1316-T04-B	1	2.85E+02			2.85E+02	2.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1316-T05-B	1	1.52E+02			1.52E+02	6.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1316-T01-C	1	8.45E+01			8.45E+01	7.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1316-T02-C	1	1.06E+02			1.06E+02	5.3E+00	3.7E+00	1.2E+01	1000	100	1.03E+03	92%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1316-T03-C	1	2.97E+02			2.97E+02	6.6E-01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1316-T04-C	1	5.90E+02			5.90E+02	2.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1316-T05-C	1	1.77E+02			1.77E+02	8.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
P	EaFA-L06-1316-B01-A	1	4.12E+01			4.12E+01	1.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	EaFA-L06-1316-T01-A	1	2.57E+04			2.57E+04	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1316-T02-A	1	5.16E+04			5.16E+04	6.0E-01	1.6E+00	5.1E+00	1000	100	5.25E+04	86%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1316-T03-A	1	1.29E+05			1.29E+05	2.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1316-T04-A	1	1.81E+05			1.81E+05	7.7E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1316-T05-A	1	2.71E+05			2.71E+05	1.2E+01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1316-T01-B	1	2.62E+04			2.62E+04	1.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1316-T02-B	1	5.66E+04			5.66E+04	8.4E-01	1.6E+00	5.1E+00	1000	100	5.74E+04	85%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1316-T03-B	1	1.39E+05			1.39E+05	2.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1316-T04-B	1	2.19E+05			2.19E+05	1.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1316-T05-B	1	3.52E+05			3.52E+05	7.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1316-T01-C	1	3.25E+04			3.25E+04	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1316-T02-C	1	5.70E+04			5.70E+04	5.3E-01	1.6E+00	5.1E+00	1000	100	5.78E+04	83%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1316-T03-C	1	1.29E+05			1.29E+05	1.7E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1316-T04-C	1	2.02E+05			2.02E+05	9.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1316-T05-C	1	3.01E+05			3.01E+05	7.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
K	EaFA-L06-1316-B01-A	1	1.30E+01			1.30E+01	1.4E+01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	EaFA-L06-1316-T01-A	1	9.93E+02			9.93E+02	3.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1316-T02-A	1	1.11E+03			1.11E+03	5.4E+00	1.5E+01	4.8E+01	10	300	4.21E+03	103%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1316-T03-A	1	1.34E+03			1.34E+03	1.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1316-T04-A	1	1.82E+03			1.82E+03	1.1E+01	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1316-T05-A	1	2.17E+03			2.17E+03	1.3E+01	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1316-T01-B	1	1.18E+03			1.18E+03	1.8E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1316-T02-B	1	1.26E+03			1.26E+03	3.2E+00	1.5E+01	4.8E+01	10	300	4.44E+03	106%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1316-T03-B	1	1.38E+03			1.38E+03	4.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1316-T04-B	1	2.26E+03			2.26E+03	2.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1316-T05-B	1	2.48E+03			2.48E+03	1.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1316-T01-C	1	1.26E+03			1.26E+03	2.8E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1316-T02-C	1	1.26E+03			1.26E+03	2.3E+00	1.5E+01	4.8E+01	10	300	4.25E+03	100%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1316-T03-C	1	1.54E+03			1.54E+03	3.0E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1316-T04-C	1	2.22E+03			2.22E+03	2.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1316-T05-C	1	4.84E+03			4.84E+03	1.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
Se	EaFA-L06-1316-B01-A	1	2.23E+01	E		2.23E+01	1.5E+02	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	EaFA-L06-1316-T01-A	1	3.53E+03			3.53E+03	7.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1316-T02-A	1	3.91E+03			3.91E+03	6.5E-01	1.1E+00	3.5E+00	1000	100	4.79E+03	88%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1316-T03-A	1	3.54E+03			3.54E+03	8.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1316-T04-A	1	1.85E+03			1.85E+03	9.9E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1316-T05-A	1	1.65E+03			1.65E+03	1.3E+01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1316-T01-B	1	2.82E+03			2.82E+03	3.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1316-T02-B	1	3.40E+03			3.40E+03	8.3E-01	1.1E+00	3.5E+00	1000	100	4.33E+03	93%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1316-T03-B	1	3.05E+03			3.05E+03	1.9E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1316-T04-B	1	1.91E+03			1.91E+03	4.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1316-T05-B	1	3.33E+03			3.33E+03	8.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1316-T01-C	1	2.99E+03			2.99E+03	9.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1316-T02-C	1	3.82E+03			3.82E+03	3.6E-01	1.1E+00	3.5E+00	1000	100	4.70E+03	88%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1316-T03-C	1	2.36E+03			2.36E+03	1.6E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1316-T04-C	1	1.75E+03			1.75E+03	1.7E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1316-T05-C	1	2.85E+03			2.85E+03	4.9E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
Si	EaFA-L06-1316-B01-A	1	5.50E-01	U1/2		5.50E-01	7.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	EaFA-L06-1316-T01-A	1	5.22E+03			5.22E+03	1.0E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1316-T02-A	1	1.05E+04			1.05E+04	8.9E-01	2.5E+00	8.0E+00	1000	100	1.13E+04	88%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1316-T03-A	1	2.64E+04			2.64E+04	2.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1316-T04-A	1	3.90E+04			3.90E+04	9.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1316-T05-A	1	6.17E+04			6.17E+04	1.2E+01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1316-T01-B	1	5.34E+03			5.34E+03	6.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1316-T02-B	1	1.17E+04			1.17E+04	3.3E-01	2.5E+00	8.0E+00	1000	100	1.27E+04	95%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1316-T03-B	1	2.89E+04			2.89E+04	1.8E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1316-T04-B	1	4.97E+04			4.97E+04	6.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1316-T05-B	1	8.21E+04			8.21E+04	7.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1316-T01-C	1	6.88E+03			6.88E+03	1.5E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1316-T02-C	1	1.18E+04			1.18E+04	1.2E+00	2.5E+00	8.0E+00	1000	100	1.27E+04	86%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1316-T03-C	1	2.72E+04			2.72E+04	1.4E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1316-T04-C	1	4.53E+04			4.53E+04	1.8E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1316-T05-C	1	6.87E+04			6.87E+04	7.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
Na	EaFA-L06-1316-B01-A	1	2.25E+01			2.25E+01	1.0E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	EaFA-L06-1316-T01-A	1	2.15E+03			2.15E+03	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1316-T02-A	1	3.86E+03			3.86E+03	2.1E-01	1.0E+00	3.2E+00	1000	100	4.75E+03	89%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1316-T03-A	1	8.59E+03			8.59E+03	3.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1316-T04-A	1	7.94E+03			7.94E+03	8.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1316-T05-A	1	7.01E+03			7.01E+03	1.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1316-T01-B	1	2.21E+03			2.21E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1316-T02-B	1	4.15E+03			4.15E+03	1.1E+00	1.0E+00	3.2E+00	1000	100	5.20E+03	105%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1316-T03-B	1	8.80E+03			8.80E+03	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1316-T04-B	1	9.67E+03			9.67E+03	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1316-T05-B	1	9.03E+03			9.03E+03	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1316-T01-C	1	2.43E+03			2.43E+03	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1316-T02-C	1	4.29E+03			4.29E+03	7.7E-01	1.0E+00	3.2E+00	1000	100	5.17E+03	88%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1316-T03-C	1	7.85E+03			7.85E+03	6.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1316-T04-C	1	9.10E+03			9.10E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1316-T05-C	1	7.85E+03			7.85E+03	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
Sr	EaFA-L06-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	7.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	EaFA-L06-1316-T01-A	1	1.69E+05			1.69E+05	7.2E-01	6.8E+00	2.2E+01			---		VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1316-T02-A	1	3.25E+05			3.25E+05	3.3E-01	6.8E+00	2.2E+01	1000	100	4.17E+05	92%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1316-T03-A	1	7.77E+05			7.77E+05	4.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1316-T04-A	1	7.22E+05			7.22E+05	9.0E+00	6.8E+00	2.2E+01			---		VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1316-T05-A	1	8.58E+05			8.58E+05	1.3E+01	6.8E+00	2.2E+01			---		VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1316-T01-B	1	1.72E+05			1.72E+05	3.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1316-T02-B	1	3.55E+05			3.55E+05	9.2E-01	6.8E+00	2.2E+01	1000	100	4.37E+05	83%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1316-T03-B	1	8.24E+05			8.24E+05	2.2E+00	6.8E+00	2.2E+01			---		VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1316-T04-B	1	8.62E+05			8.62E+05	1.1E+00	6.8E+00	2.2E+01			---		VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1316-T05-B	1	1.12E+06			1.12E+06	1.9E-01	6.8E+00	2.2E+01			---		VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1316-T01-C	1	1.95E+05			1.95E+05	1.0E+00	6.8E+00	2.2E+01			---		VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1316-T02-C	1	3.57E+05			3.57E+05	4.9E-01	6.8E+00	2.2E+01	1000	100	4.55E+05	98%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1316-T03-C	1	7.64E+05			7.64E+05	1.6E+00	6.8E+00	2.2E+01			---		VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1316-T04-C	1	8.35E+05			8.35E+05	1.8E+00	6.8E+00	2.2E+01			---		VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1316-T05-C	1	9.67E+05			9.67E+05	8.1E-01	6.8E+00	2.2E+01			---		VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
S	EaFA-L06-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	1.5E+01	6.8E+00	2.2E+01			---		VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	EaFA-L06-1316-T01-A	1	2.30E+00	U1/2		2.30E+00	1.8E+03	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1316-T02-A	1	7.99E+00	E		7.99E+00	1.4E+02	4.6E+00	1.5E+01	10	300	3.06E+03	102%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1316-T03-A	1	1.19E+01	E		1.19E+01	1.4E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1316-T04-A	1	9.05E+00	E		9.05E+00	1.1E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1316-T05-A	1	1.79E+01			1.79E+01	5.3E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1316-T01-B	1	2.30E+00	U1/2		2.30E+00	1.4E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1316-T02-B	1	2.30E+00	U1/2		2.30E+00	7.0E+02	4.6E+00	1.5E+01	10	300	3.19E+03	106%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1316-T03-B	1	3.11E+01			3.11E+01	3.7E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1316-T04-B	1	3.52E+01			3.52E+01	4.1E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1316-T05-B	1	3.88E+01			3.88E+01	3.5E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1316-T01-C	1	2.30E+00	U1/2		2.30E+00	3.1E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1316-T02-C	1	8.62E+00	E		8.62E+00	2.2E+01	4.6E+00	1.5E+01	10	300	3.04E+03	101%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1316-T03-C	1	1.24E+01	E		1.24E+01	9.5E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1316-T04-C	1	1.34E+01	E		1.34E+01	5.7E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1316-T05-C	1	2.30E+00	U1/2		2.30E+00	4.4E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
Tl	EaFA-L06-1316-B01-A	1	2.30E+00	U1/2		2.30E+00	4.2E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	EaFA-L06-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	5.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	5.8E+01	2.0E+00	6.4E+00	10	300	3.19E+03	106%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	5.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1316-T05-A	1	1.00E+00	U1/2		1.00E+00	4.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	2.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	6.9E+01	2.0E+00	6.4E+00	10	300	3.34E+03	111%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	2.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1316-T05-B	1	1.00E+00	U1/2		1.00E+00	5.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	1.6E+03	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	2.9E+01	2.0E+00	6.4E+00	10	300	3.13E+03	104%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	6.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1316-T05-C	1	1.00E+00	U1/2		1.00E+00	1.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
Ti	EaFA-L06-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	EaFA-L06-1316-T01-A	1	2.43E+02			2.43E+02	5.1E-01	1.5E+00	4.8E+00			---		VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1316-T02-A	1	2.73E+02			2.73E+02	8.2E-01	1.5E+00	4.8E+00	10	300	3.42E+03	105%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1316-T03-A	1	3.43E+02			3.43E+02	7.0E-01	1.5E+00	4.8E+00			---		VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1316-T04-A	1	3.18E+02			3.18E+02	8.1E+00	1.5E+00	4.8E+00			---		VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1316-T05-A	1	3.07E+02			3.07E+02	1.3E+01	1.5E+00	4.8E+00			---		VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1316-T01-B	1	2.62E+02			2.62E+02	9.5E-01	1.5E+00	4.8E+00			---		VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1316-T02-B	1	2.85E+02			2.85E+02	9.5E-01	1.5E+00	4.8E+00	10	300	3.56E+03	109%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1316-T03-B	1	3.29E+02			3.29E+02	1.7E+00	1.5E+00	4.8E+00			---		VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1316-T04-B	1	3.75E+02			3.75E+02	4.9E-01	1.5E+00	4.8E+00			---		VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1316-T05-B	1	4.09E+02			4.09E+02	1.3E+00	1.5E+00	4.8E+00			---		VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1316-T01-C	1	2.55E+02			2.55E+02	2.8E+00	1.5E+00	4.8E+00			---		VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1316-T02-C	1	2.86E+02			2.86E+02	9.7E-01	1.5E+00	4.8E+00	10	300	3.37E+03	103%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1316-T03-C	1	3.36E+02			3.36E+02	2.8E+00	1.5E+00	4.8E+00			---		VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1316-T04-C	1	3.43E+02			3.43E+02	6.2E-01	1.5E+00	4.8E+00			---		VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1316-T05-C	1	5.91E+02			5.91E+02	1.3E+00	1.5E+00	4.8E+00			---		VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
V	EaFA-L06-1316-B01-A	1	7.50E-01	U1/2		7.50E-01	1.5E+02	1.5E+00	4.8E+00			---		VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	EaFA-L06-1316-T01-A	1	5.76E+01			5.76E+01	3.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:44 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1316-T02-A	1	7.16E+01			7.16E+01	2.8E+00	1.0E+00	3.2E+00	10	300	3.37E+03	110%	VU ICP-OES	6/7/10 3:46 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1316-T03-A	1	6.89E+01			6.89E+01	2.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:47 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1316-T04-A	1	3.21E+01			3.21E+01	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:49 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1316-T05-A	1	3.58E+01			3.58E+01	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:50 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1316-T01-B	1	2.29E+01			2.29E+01	2.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:52 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1316-T02-B	1	4.64E+01			4.64E+01	8.8E-01	1.0E+00	3.2E+00	10	300	3.46E+03	114%	VU ICP-OES	6/7/10 4:27 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1316-T03-B	1	5.69E+01			5.69E+01	3.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:29 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1316-T04-B	1	2.20E+01			2.20E+01	6.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:30 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1316-T05-B	1	5.62E+01			5.62E+01	2.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:32 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1316-T01-C	1	3.22E+01			3.22E+01	4.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:33 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1316-T02-C	1	6.59E+01			6.59E+01	9.6E-01	1.0E+00	3.2E+00	10	300	3.29E+03	107%	VU ICP-OES	6/7/10 4:35 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1316-T03-C	1	2.90E+01			2.90E+01	4.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:37 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1316-T04-C	1	1.88E+01			1.88E+01	5.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:38 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1316-T05-C	1	2.33E+01			2.33E+01	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 4:40 PM	EPA Interlab L06 1313-1316 EaFA
Zn	EaFA-L06-1316-B01-A	1	9.40E+00			9.40E+00	5.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 3:41 PM	EPA Interlab L06 1313-1316 EaFA

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	EaFA-L07-1316-T01-A	1	1.66E+02			1.66E+02	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1316-T02-A	1	1.60E+02			1.60E+02	1.7E+00	1.0E+00	3.2E+00	1000	100	1.26E+03	110%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1316-T03-A	1	2.43E+02			2.43E+02	3.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1316-T04-A	1	4.68E+02			4.68E+02	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1316-T05-A	1	9.10E+02			9.10E+02	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1316-T01-B	1	1.21E+02			1.21E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1316-T02-B	1	1.46E+02			1.46E+02	3.9E+00	1.0E+00	3.2E+00	1000	100	1.22E+03	107%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1316-T03-B	1	2.21E+02			2.21E+02	2.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1316-T04-B	1	4.41E+02			4.41E+02	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1316-T05-B	1	1.23E+03			1.23E+03	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1316-T01-C	1	1.10E+02			1.10E+02	3.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1316-T02-C	1	1.60E+02			1.60E+02	2.6E+00	1.0E+00	3.2E+00	1000	100	1.21E+03	105%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1316-T03-C	1	2.34E+02			2.34E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1316-T04-C	1	5.02E+02			5.02E+02	7.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1316-T05-C	1	8.14E+02			8.14E+02	8.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
Al	EaFA-L07-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	EaFA-L07-1316-T01-A	1	2.05E+02			2.05E+02	4.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1316-T02-A	1	3.08E+02			3.08E+02	1.2E+01	7.5E+00	2.4E+01	10	300	3.51E+03	107%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1316-T03-A	1	4.69E+02			4.69E+02	8.1E-01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1316-T04-A	1	6.58E+02			6.58E+02	2.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1316-T05-A	1	7.86E+02			7.86E+02	6.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1316-T01-B	1	2.15E+02			2.15E+02	1.4E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1316-T02-B	1	3.39E+02			3.39E+02	6.9E+00	7.5E+00	2.4E+01	10	300	3.56E+03	107%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1316-T03-B	1	4.60E+02			4.60E+02	2.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1316-T04-B	1	6.41E+02			6.41E+02	4.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1316-T05-B	1	7.86E+02			7.86E+02	3.7E-01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1316-T01-C	1	2.01E+02			2.01E+02	1.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1316-T02-C	1	3.28E+02			3.28E+02	6.8E+00	7.5E+00	2.4E+01	10	300	3.46E+03	105%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1316-T03-C	1	4.59E+02			4.59E+02	4.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1316-T04-C	1	6.64E+02			6.64E+02	2.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1316-T05-C	1	6.80E+02			6.80E+02	1.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
Sb	EaFA-L07-1316-B01-A	1	1.06E+01	E		1.06E+01	6.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	EaFA-L07-1316-T01-A	1	1.40E+02			1.40E+02	8.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1316-T02-A	1	1.23E+02			1.23E+02	1.3E+01	1.1E+01	3.5E+01	10	300	3.38E+03	109%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1316-T03-A	1	1.33E+02			1.33E+02	5.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1316-T04-A	1	1.93E+02			1.93E+02	1.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1316-T05-A	1	2.96E+02			2.96E+02	9.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1316-T01-B	1	1.20E+02			1.20E+02	1.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1316-T02-B	1	1.36E+02			1.36E+02	8.7E+00	1.1E+01	3.5E+01	10	300	3.35E+03	107%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1316-T03-B	1	1.35E+02			1.35E+02	2.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1316-T04-B	1	1.72E+02			1.72E+02	2.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1316-T05-B	1	2.53E+02			2.53E+02	5.7E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1316-T01-C	1	1.10E+02			1.10E+02	6.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1316-T02-C	1	1.29E+02			1.29E+02	7.5E+00	1.1E+01	3.5E+01	10	300	3.31E+03	106%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1316-T03-C	1	1.54E+02			1.54E+02	1.7E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1316-T04-C	1	2.17E+02			2.17E+02	3.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1316-T05-C	1	1.91E+02			1.91E+02	3.2E-01	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
As	EaFA-L07-1316-B01-A	1	5.50E+00	U1/2		5.50E+00	2.9E+02	1.1E+01	3.5E+01				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	EaFA-L07-1316-T01-A	1	4.25E+03			4.25E+03	4.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1316-T02-A	1	8.37E+03			8.37E+03	6.0E-01	1.0E+00	3.2E+00	1000	100	9.38E+03	101%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1316-T03-A	1	2.02E+04			2.02E+04	3.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1316-T04-A	1	3.61E+04			3.61E+04	7.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1316-T05-A	1	5.41E+04			5.41E+04	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1316-T01-B	1	5.30E+03			5.30E+03	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1316-T02-B	1	8.76E+03			8.76E+03	9.2E-01	1.0E+00	3.2E+00	1000	100	9.70E+03	93%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1316-T03-B	1	1.96E+04			1.96E+04	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1316-T04-B	1	3.55E+04			3.55E+04	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1316-T05-B	1	6.42E+04			6.42E+04	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1316-T01-C	1	4.18E+03			4.18E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1316-T02-C	1	9.26E+03			9.26E+03	6.5E-01	1.0E+00	3.2E+00	1000	100	1.01E+04	87%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1316-T03-C	1	2.10E+04			2.10E+04	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1316-T04-C	1	3.73E+04			3.73E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1316-T05-C	1	5.59E+04			5.59E+04	8.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
B	EaFA-L07-1316-B01-A	1	3.55E+01			3.55E+01	6.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	EaFA-L07-1316-T01-A	1	2.69E+02			2.69E+02	3.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1316-T02-A	1	2.18E+02			2.18E+02	7.1E-02	1.0E+00	3.2E+00	10	300	3.23E+03	100%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1316-T03-A	1	2.06E+02			2.06E+02	3.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1316-T04-A	1	2.15E+02			2.15E+02	2.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1316-T05-A	1	2.41E+02			2.41E+02	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1316-T01-B	1	2.85E+02			2.85E+02	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1316-T02-B	1	2.13E+02			2.13E+02	5.7E-01	1.0E+00	3.2E+00	10	300	3.19E+03	99%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1316-T03-B	1	1.91E+02			1.91E+02	2.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1316-T04-B	1	2.16E+02			2.16E+02	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1316-T05-B	1	2.86E+02			2.86E+02	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1316-T01-C	1	2.67E+02			2.67E+02	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1316-T02-C	1	2.16E+02			2.16E+02	3.5E-01	1.0E+00	3.2E+00	10	300	3.16E+03	98%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1316-T03-C	1	2.06E+02			2.06E+02	9.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1316-T04-C	1	2.17E+02			2.17E+02	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1316-T05-C	1	2.26E+02			2.26E+02	4.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
Ba	EaFA-L07-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	5.9E+02	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	EaFA-L07-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	8.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	2.8E+02	1.9E+00	6.0E+00	10	300	3.27E+03	109%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	6.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	2.2E+04	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1316-T05-A	1	9.50E-01	U1/2		9.50E-01	9.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	2.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	3.0E+03	1.9E+00	6.0E+00	10	300	3.26E+03	109%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	7.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1316-T05-B	1	9.50E-01	U1/2		9.50E-01	8.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	6.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	4.0E+01	1.9E+00	6.0E+00	10	300	3.22E+03	107%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	6.7E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1316-T05-C	1	9.50E-01	U1/2		9.50E-01	2.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
Be	EaFA-L07-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	2.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	EaFA-L07-1316-T01-A	1	1.10E+00	U1/2		1.10E+00	2.1E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1316-T02-A	1	1.10E+00	U1/2		1.10E+00	5.8E+02	2.2E+00	7.0E+00	10	300	3.24E+03	108%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1316-T03-A	1	2.57E+00	E		2.57E+00	2.7E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1316-T04-A	1	1.10E+00	U1/2		1.10E+00	5.3E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1316-T05-A	1	1.10E+00	U1/2		1.10E+00	4.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1316-T01-B	1	1.10E+00	U1/2		1.10E+00	4.3E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1316-T02-B	1	1.10E+00	U1/2		1.10E+00	2.7E+02	2.2E+00	7.0E+00	10	300	3.19E+03	106%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1316-T03-B	1	2.95E+00	E		2.95E+00	3.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1316-T04-B	1	1.10E+00	U1/2		1.10E+00	8.7E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1316-T05-B	1	6.60E+00	E		6.60E+00	1.9E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1316-T01-C	1	1.10E+00	U1/2		1.10E+00	5.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1316-T02-C	1	1.10E+00	U1/2		1.10E+00	4.0E+01	2.2E+00	7.0E+00	10	300	3.18E+03	106%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1316-T03-C	1	3.45E+00	E		3.45E+00	9.9E+00	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1316-T04-C	1	1.10E+00	U1/2		1.10E+00	3.8E+03	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1316-T05-C	1	1.10E+00	U1/2		1.10E+00	1.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
Cd	EaFA-L07-1316-B01-A	1	1.10E+00	U1/2		1.10E+00	2.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	EaFA-L07-1316-T01-A	1	1.64E+05			1.64E+05	4.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1316-T02-A	1	3.18E+05			3.18E+05	2.2E-01	2.6E+00	8.3E+00	1000	100	3.19E+05	85%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1316-T03-A	1	7.46E+05			7.46E+05	3.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1316-T04-A	1	5.77E+05			5.77E+05	3.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1316-T05-A	1	5.17E+05			5.17E+05	1.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1316-T01-B	1	1.59E+05			1.59E+05	5.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1316-T02-B	1	3.14E+05			3.14E+05	1.1E-01	2.6E+00	8.3E+00	1000	100	3.15E+05	82%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1316-T03-B	1	6.75E+05			6.75E+05	2.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1316-T04-B	1	5.66E+05			5.66E+05	2.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1316-T05-B	1	5.18E+05			5.18E+05	1.8E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1316-T01-C	1	1.59E+05			1.59E+05	2.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1316-T02-C	1	3.35E+05			3.35E+05	7.1E-01	2.6E+00	8.3E+00	1000	100	3.36E+05	84%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1316-T03-C	1	7.65E+05			7.65E+05	9.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1316-T04-C	1	5.91E+05			5.91E+05	1.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1316-T05-C	1	5.21E+05			5.21E+05	6.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
Ca	EaFA-L07-1316-B01-A	1	6.24E+00	E		6.24E+00	2.4E+01	2.6E+00	8.3E+00				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	EaFA-L07-1316-T01-A	1	1.26E+01			1.26E+01	7.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1316-T02-A	1	1.33E+01			1.33E+01	9.8E+00	1.2E+00	3.8E+00	10	300	3.23E+03	107%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1316-T03-A	1	2.04E+01			2.04E+01	7.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1316-T04-A	1	4.17E+01			4.17E+01	2.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1316-T05-A	1	9.24E+01			9.24E+01	3.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1316-T01-B	1	9.72E+00			9.72E+00	3.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1316-T02-B	1	1.63E+01			1.63E+01	8.6E+00	1.2E+00	3.8E+00	10	300	3.16E+03	105%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1316-T03-B	1	1.81E+01			1.81E+01	8.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1316-T04-B	1	4.22E+01			4.22E+01	5.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1316-T05-B	1	9.07E+01			9.07E+01	2.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1316-T01-C	1	8.97E+00			8.97E+00	1.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1316-T02-C	1	1.50E+01			1.50E+01	7.2E+00	1.2E+00	3.8E+00	10	300	3.14E+03	104%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1316-T03-C	1	2.14E+01			2.14E+01	5.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1316-T04-C	1	4.67E+01			4.67E+01	2.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1316-T05-C	1	5.91E+01			5.91E+01	2.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
Cr	EaFA-L07-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	2.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	EaFA-L07-1316-T01-A	1	3.90E+01			3.90E+01	6.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1316-T02-A	1	9.97E+01			9.97E+01	1.6E+00	1.8E+00	5.7E+00	10	300	3.27E+03	106%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1316-T03-A	1	1.91E+02			1.91E+02	3.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1316-T04-A	1	1.08E+02			1.08E+02	1.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1316-T05-A	1	7.85E+01			7.85E+01	2.9E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1316-T01-B	1	5.56E+01			5.56E+01	4.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1316-T02-B	1	1.01E+02			1.01E+02	2.3E+00	1.8E+00	5.7E+00	10	300	3.22E+03	104%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1316-T03-B	1	1.88E+02			1.88E+02	2.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1316-T04-B	1	1.26E+02			1.26E+02	2.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1316-T05-B	1	2.50E+02			2.50E+02	2.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1316-T01-C	1	6.37E+01			6.37E+01	9.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1316-T02-C	1	1.08E+02			1.08E+02	9.2E-01	1.8E+00	5.7E+00	10	300	3.18E+03	102%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1316-T03-C	1	2.15E+02			2.15E+02	2.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1316-T04-C	1	9.97E+01			9.97E+01	3.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1316-T05-C	1	1.18E+02			1.18E+02	2.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
Co	EaFA-L07-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	6.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	EaFA-L07-1316-T01-A	1	1.11E+01	E		1.11E+01	6.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1316-T02-A	1	1.28E+01			1.28E+01	8.3E+00	3.7E+00	1.2E+01	10	300	3.25E+03	108%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1316-T03-A	1	1.70E+01			1.70E+01	1.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1316-T04-A	1	1.77E+01			1.77E+01	6.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1316-T05-A	1	1.80E+01			1.80E+01	3.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1316-T01-B	1	1.40E+01			1.40E+01	4.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1316-T02-B	1	1.80E+01			1.80E+01	3.1E+01	3.7E+00	1.2E+01	10	300	3.20E+03	106%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1316-T03-B	1	1.98E+01			1.98E+01	9.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1316-T04-B	1	2.05E+01			2.05E+01	9.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1316-T05-B	1	4.78E+01			4.78E+01	1.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1316-T01-C	1	1.48E+01			1.48E+01	2.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1316-T02-C	1	2.40E+01			2.40E+01	3.1E+01	3.7E+00	1.2E+01	10	300	3.16E+03	104%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1316-T03-C	1	1.47E+01			1.47E+01	1.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1316-T04-C	1	2.05E+01			2.05E+01	3.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1316-T05-C	1	2.13E+01			2.13E+01	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
Cu	EaFA-L07-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	3.0E+02	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	EaFA-L07-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00	1000	100	1.07E+03	107%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	4.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1316-T05-A	1	2.26E+00	E		2.26E+00	8.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	2.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00	1000	100	1.05E+03	105%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1316-T05-B	1	5.74E+01			5.74E+01	5.7E-02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	1.3E+01	2.0E+00	6.4E+00	1000	100	1.05E+03	105%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	1.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	3.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1316-T05-C	1	9.00E+00			9.00E+00	9.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
Fe	EaFA-L07-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	EaFA-L07-1316-T01-A	1	3.40E+00	U1/2		3.40E+00	3.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1316-T02-A	1	3.40E+00	U1/2		3.40E+00	5.9E+01	6.8E+00	2.2E+01	10	300	3.10E+03	103%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1316-T03-A	1	3.40E+00	U1/2		3.40E+00	2.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1316-T04-A	1	3.40E+00	U1/2		3.40E+00	2.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1316-T05-A	1	3.40E+00	U1/2		3.40E+00	1.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1316-T01-B	1	3.40E+00	U1/2		3.40E+00	3.8E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1316-T02-B	1	3.40E+00	U1/2		3.40E+00	1.7E+01	6.8E+00	2.2E+01	10	300	3.08E+03	102%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1316-T03-B	1	3.40E+00	U1/2		3.40E+00	1.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1316-T04-B	1	3.40E+00	U1/2		3.40E+00	6.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1316-T05-B	1	3.40E+00	U1/2		3.40E+00	2.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1316-T01-C	1	3.40E+00	U1/2		3.40E+00	1.3E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1316-T02-C	1	3.40E+00	U1/2		3.40E+00	6.6E+01	6.8E+00	2.2E+01	10	300	3.05E+03	102%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1316-T03-C	1	3.40E+00	U1/2		3.40E+00	2.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1316-T04-C	1	3.40E+00	U1/2		3.40E+00	9.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1316-T05-C	1	3.40E+00	U1/2		3.40E+00	3.7E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
Pb	EaFA-L07-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	1.7E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	EaFA-L07-1316-T01-A	1	3.51E+03			3.51E+03	2.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1316-T02-A	1	6.73E+03			6.73E+03	2.1E-01	1.9E+00	6.0E+00	10	300	9.56E+03	94%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1316-T03-A	1	1.60E+04			1.60E+04	3.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1316-T04-A	1	3.16E+04			3.16E+04	3.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1316-T05-A	1	5.11E+04			5.11E+04	9.6E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1316-T01-B	1	3.48E+03			3.48E+03	2.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1316-T02-B	1	6.68E+03			6.68E+03	5.6E-01	1.9E+00	6.0E+00	10	300	9.30E+03	87%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1316-T03-B	1	1.47E+04			1.47E+04	1.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1316-T04-B	1	3.03E+04			3.03E+04	5.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1316-T05-B	1	5.93E+04			5.93E+04	2.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1316-T01-C	1	3.51E+03			3.51E+03	2.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1316-T02-C	1	7.05E+03			7.05E+03	2.0E-01	1.9E+00	6.0E+00	10	300	9.53E+03	83%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1316-T03-C	1	1.64E+04			1.64E+04	1.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1316-T04-C	1	3.26E+04			3.26E+04	2.9E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1316-T05-C	1	5.55E+04			5.55E+04	4.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
Li	EaFA-L07-1316-B01-A	1	1.46E+01			1.46E+01	3.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	EaFA-L07-1316-T01-A	1	3.37E+02			3.37E+02	5.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1316-T02-A	1	7.62E+02			7.62E+02	3.5E-01	2.0E+00	6.4E+00	10	300	3.96E+03	107%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1316-T03-A	1	1.42E+03			1.42E+03	2.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1316-T04-A	1	1.12E+03			1.12E+03	9.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1316-T05-A	1	9.68E+02			9.68E+02	1.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1316-T01-B	1	4.17E+02			4.17E+02	4.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1316-T02-B	1	7.36E+02			7.36E+02	9.4E-01	2.0E+00	6.4E+00	10	300	3.90E+03	106%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1316-T03-B	1	1.38E+03			1.38E+03	2.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1316-T04-B	1	1.28E+03			1.28E+03	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1316-T05-B	1	2.02E+03			2.02E+03	1.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1316-T01-C	1	4.48E+02			4.48E+02	1.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1316-T02-C	1	7.99E+02			7.99E+02	3.9E-01	2.0E+00	6.4E+00	10	300	3.90E+03	103%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1316-T03-C	1	1.54E+03			1.54E+03	1.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1316-T04-C	1	1.09E+03			1.09E+03	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1316-T05-C	1	1.39E+03			1.39E+03	8.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
Mn	EaFA-L07-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	3.5E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	EaFA-L07-1316-T01-A	1	7.32E+03			7.32E+03	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1316-T02-A	1	1.44E+04			1.44E+04	3.1E-01	1.0E+00	3.2E+00	1000	100	1.54E+04	103%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1316-T03-A	1	3.76E+04			3.76E+04	3.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1316-T04-A	1	6.88E+04			6.88E+04	3.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1316-T05-A	1	1.00E+05			1.00E+05	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1316-T01-B	1	7.05E+03			7.05E+03	9.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1316-T02-B	1	1.43E+04			1.43E+04	6.9E-01	1.0E+00	3.2E+00	1000	100	1.53E+04	96%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1316-T03-B	1	3.39E+04			3.39E+04	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1316-T04-B	1	6.61E+04			6.61E+04	8.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1316-T05-B	1	1.20E+05			1.20E+05	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1316-T01-C	1	7.18E+03			7.18E+03	3.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1316-T02-C	1	1.52E+04			1.52E+04	1.1E+00	1.0E+00	3.2E+00	1000	100	1.61E+04	87%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1316-T03-C	1	3.79E+04			3.79E+04	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1316-T04-C	1	7.12E+04			7.12E+04	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1316-T05-C	1	1.10E+05			1.10E+05	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
Mg	EaFA-L07-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	5.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	EaFA-L07-1316-T01-A	1	3.38E+03			3.38E+03	3.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1316-T02-A	1	6.15E+03			6.15E+03	2.1E-01	1.2E+00	3.8E+00	10	300	8.99E+03	95%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1316-T03-A	1	1.40E+04			1.40E+04	3.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1316-T04-A	1	2.83E+04			2.83E+04	1.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1316-T05-A	1	5.02E+04			5.02E+04	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1316-T01-B	1	3.21E+03			3.21E+03	6.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1316-T02-B	1	6.16E+03			6.16E+03	6.1E-01	1.2E+00	3.8E+00	10	300	8.88E+03	91%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1316-T03-B	1	1.29E+04			1.29E+04	2.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1316-T04-B	1	2.67E+04			2.67E+04	2.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1316-T05-B	1	4.61E+04			4.61E+04	2.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1316-T01-C	1	3.18E+03			3.18E+03	2.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1316-T02-C	1	6.34E+03			6.34E+03	6.3E-01	1.2E+00	3.8E+00	10	300	8.77E+03	81%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1316-T03-C	1	1.41E+04			1.41E+04	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1316-T04-C	1	2.96E+04			2.96E+04	3.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1316-T05-C	1	4.61E+04			4.61E+04	7.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
Mo	EaFA-L07-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	3.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	EaFA-L07-1316-T01-A	1	9.90E+01			9.90E+01	5.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1316-T02-A	1	2.39E+02			2.39E+02	2.1E+00	1.8E+00	5.7E+00	10	300	3.39E+03	105%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1316-T03-A	1	4.42E+02			4.42E+02	4.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1316-T04-A	1	2.65E+02			2.65E+02	4.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1316-T05-A	1	2.11E+02			2.11E+02	1.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1316-T01-B	1	1.36E+02			1.36E+02	1.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1316-T02-B	1	2.43E+02			2.43E+02	9.9E-01	1.8E+00	5.7E+00	10	300	3.34E+03	103%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1316-T03-B	1	4.40E+02			4.40E+02	2.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1316-T04-B	1	3.06E+02			3.06E+02	5.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1316-T05-B	1	5.65E+02			5.65E+02	9.4E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1316-T01-C	1	1.50E+02			1.50E+02	2.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1316-T02-C	1	2.54E+02			2.54E+02	1.6E+00	1.8E+00	5.7E+00	10	300	3.29E+03	101%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1316-T03-C	1	4.91E+02			4.91E+02	1.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1316-T04-C	1	2.46E+02			2.46E+02	2.9E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1316-T05-C	1	2.64E+02			2.64E+02	2.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
Ni	EaFA-L07-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	8.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	EaFA-L07-1316-T01-A	1	3.79E+01			3.79E+01	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1316-T02-A	1	4.93E+01			4.93E+01	1.1E+01	3.7E+00	1.2E+01	1000	100	1.03E+03	99%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1316-T03-A	1	1.04E+02			1.04E+02	7.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1316-T04-A	1	2.87E+02			2.87E+02	3.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1316-T05-A	1	2.82E+02			2.82E+02	5.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1316-T01-B	1	5.72E+01			5.72E+01	1.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1316-T02-B	1	6.36E+01			6.36E+01	1.8E+01	3.7E+00	1.2E+01	1000	100	1.00E+03	94%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1316-T03-B	1	1.14E+02			1.14E+02	7.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1316-T04-B	1	3.35E+02			3.35E+02	3.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1316-T05-B	1	3.17E+02			3.17E+02	3.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1316-T01-C	1	3.50E+01			3.50E+01	3.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1316-T02-C	1	5.44E+01			5.44E+01	1.3E+01	3.7E+00	1.2E+01	1000	100	1.02E+03	97%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1316-T03-C	1	1.67E+02			1.67E+02	9.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1316-T04-C	1	4.06E+02			4.06E+02	7.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1316-T05-C	1	1.16E+03			1.16E+03	3.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
P	EaFA-L07-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	5.7E+02	3.7E+00	1.2E+01				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	EaFA-L07-1316-T01-A	1	2.61E+04			2.61E+04	4.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1316-T02-A	1	5.31E+04			5.31E+04	2.2E-01	1.6E+00	5.1E+00	1000	100	5.41E+04	98%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1316-T03-A	1	1.33E+05			1.33E+05	3.7E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1316-T04-A	1	2.12E+05			2.12E+05	2.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1316-T05-A	1	2.95E+05			2.95E+05	1.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1316-T01-B	1	2.57E+04			2.57E+04	4.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1316-T02-B	1	5.25E+04			5.25E+04	4.0E-01	1.6E+00	5.1E+00	1000	100	5.34E+04	88%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1316-T03-B	1	1.22E+05			1.22E+05	1.9E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1316-T04-B	1	2.06E+05			2.06E+05	3.7E-02	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1316-T05-B	1	3.51E+05			3.51E+05	9.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1316-T01-C	1	2.56E+04			2.56E+04	3.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1316-T02-C	1	5.55E+04			5.55E+04	6.4E-01	1.6E+00	5.1E+00	1000	100	5.64E+04	83%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1316-T03-C	1	1.35E+05			1.35E+05	1.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1316-T04-C	1	2.19E+05			2.19E+05	7.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1316-T05-C	1	3.22E+05			3.22E+05	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
K	EaFA-L07-1316-B01-A	1	1.13E+01			1.13E+01	6.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	EaFA-L07-1316-T01-A	1	1.11E+03			1.11E+03	4.6E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1316-T02-A	1	1.19E+03			1.19E+03	3.9E+00	1.5E+01	4.8E+01	10	300	4.37E+03	106%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1316-T03-A	1	1.37E+03			1.37E+03	1.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1316-T04-A	1	2.17E+03			2.17E+03	1.8E-01	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1316-T05-A	1	3.65E+03			3.65E+03	1.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1316-T01-B	1	1.10E+03			1.10E+03	1.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1316-T02-B	1	1.38E+03			1.38E+03	1.0E+00	1.5E+01	4.8E+01	10	300	4.40E+03	101%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1316-T03-B	1	1.49E+03			1.49E+03	3.2E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1316-T04-B	1	2.09E+03			2.09E+03	1.8E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1316-T05-B	1	3.21E+03			3.21E+03	2.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1316-T01-C	1	1.05E+03			1.05E+03	5.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1316-T02-C	1	1.30E+03			1.30E+03	5.0E+00	1.5E+01	4.8E+01	10	300	4.30E+03	100%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1316-T03-C	1	1.53E+03			1.53E+03	1.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1316-T04-C	1	2.37E+03			2.37E+03	8.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1316-T05-C	1	2.70E+03			2.70E+03	2.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
Se	EaFA-L07-1316-B01-A	1	2.78E+01	E		2.78E+01	1.4E+02	1.5E+01	4.8E+01				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	EaFA-L07-1316-T01-A	1	2.22E+03			2.22E+03	2.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1316-T02-A	1	2.91E+03			2.91E+03	4.0E-01	1.1E+00	3.5E+00	1000	100	3.79E+03	89%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1316-T03-A	1	2.74E+03			2.74E+03	4.4E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1316-T04-A	1	2.19E+03			2.19E+03	1.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1316-T05-A	1	1.93E+03			1.93E+03	5.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1316-T01-B	1	2.90E+03			2.90E+03	8.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1316-T02-B	1	3.34E+03			3.34E+03	5.0E-01	1.1E+00	3.5E+00	1000	100	4.18E+03	84%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1316-T03-B	1	2.93E+03			2.93E+03	2.4E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1316-T04-B	1	2.40E+03			2.40E+03	5.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1316-T05-B	1	3.07E+03			3.07E+03	1.4E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1316-T01-C	1	2.87E+03			2.87E+03	1.5E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1316-T02-C	1	3.16E+03			3.16E+03	3.1E-01	1.1E+00	3.5E+00	1000	100	4.03E+03	87%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1316-T03-C	1	3.15E+03			3.15E+03	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1316-T04-C	1	2.22E+03			2.22E+03	4.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1316-T05-C	1	2.06E+03			2.06E+03	1.8E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
Si	EaFA-L07-1316-B01-A	1	5.50E-01	U1/2		5.50E-01	7.1E+01	1.1E+00	3.5E+00				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	EaFA-L07-1316-T01-A	1	5.36E+03			5.36E+03	6.1E-02	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1316-T02-A	1	1.10E+04			1.10E+04	7.7E-01	2.5E+00	8.0E+00	1000	100	1.19E+04	89%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1316-T03-A	1	2.80E+04			2.80E+04	3.8E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1316-T04-A	1	4.70E+04			4.70E+04	4.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1316-T05-A	1	6.83E+04			6.83E+04	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1316-T01-B	1	5.28E+03			5.28E+03	7.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1316-T02-B	1	1.09E+04			1.09E+04	6.5E-01	2.5E+00	8.0E+00	1000	100	1.17E+04	81%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1316-T03-B	1	2.54E+04			2.54E+04	1.8E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1316-T04-B	1	4.48E+04			4.48E+04	5.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1316-T05-B	1	7.45E+04			7.45E+04	1.7E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1316-T01-C	1	5.29E+03			5.29E+03	2.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1316-T02-C	1	1.15E+04			1.15E+04	4.0E-01	2.5E+00	8.0E+00	1000	100	1.24E+04	89%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1316-T03-C	1	2.83E+04			2.83E+04	6.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1316-T04-C	1	4.82E+04			4.82E+04	2.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1316-T05-C	1	7.46E+04			7.46E+04	4.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
Na	EaFA-L07-1316-B01-A	1	3.39E+00	E		3.39E+00	6.4E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	EaFA-L07-1316-T01-A	1	2.23E+03			2.23E+03	2.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1316-T02-A	1	4.04E+03			4.04E+03	5.8E-02	1.0E+00	3.2E+00	1000	100	4.85E+03	82%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1316-T03-A	1	8.70E+03			8.70E+03	3.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1316-T04-A	1	8.61E+03			8.61E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1316-T05-A	1	8.58E+03			8.58E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1316-T01-B	1	2.15E+03			2.15E+03	2.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1316-T02-B	1	4.12E+03			4.12E+03	1.4E+00	1.0E+00	3.2E+00	1000	100	4.95E+03	83%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1316-T03-B	1	8.36E+03			8.36E+03	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1316-T04-B	1	8.35E+03			8.35E+03	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1316-T05-B	1	9.53E+03			9.53E+03	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1316-T01-C	1	2.15E+03			2.15E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1316-T02-C	1	4.24E+03			4.24E+03	6.2E-01	1.0E+00	3.2E+00	1000	100	5.07E+03	83%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1316-T03-C	1	9.08E+03			9.08E+03	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1316-T04-C	1	9.16E+03			9.16E+03	5.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1316-T05-C	1	7.73E+03			7.73E+03	8.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
Sr	EaFA-L07-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	EaFA-L07-1316-T01-A	1	1.68E+05			1.68E+05	4.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1316-T02-A	1	3.29E+05			3.29E+05	4.2E-01	6.8E+00	2.2E+01	1000	100	3.30E+05	85%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1316-T03-A	1	7.61E+05			7.61E+05	3.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1316-T04-A	1	7.78E+05			7.78E+05	2.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1316-T05-A	1	9.05E+05			9.05E+05	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1316-T01-B	1	1.63E+05			1.63E+05	7.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1316-T02-B	1	3.27E+05			3.27E+05	6.9E-01	6.8E+00	2.2E+01	1000	100	3.28E+05	83%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1316-T03-B	1	7.25E+05			7.25E+05	2.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1316-T04-B	1	7.65E+05			7.65E+05	6.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1316-T05-B	1	1.02E+06			1.02E+06	1.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1316-T01-C	1	1.63E+05			1.63E+05	2.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1316-T02-C	1	3.44E+05			3.44E+05	6.4E-01	6.8E+00	2.2E+01	1000	100	3.45E+05	83%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1316-T03-C	1	7.90E+05			7.90E+05	1.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1316-T04-C	1	7.94E+05			7.94E+05	4.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1316-T05-C	1	9.53E+05			9.53E+05	2.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
S	EaFA-L07-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	3.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

TI	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	EaFA-L07-1316-T01-A	1	2.30E+00	U1/2		2.30E+00	3.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1316-T02-A	1	2.30E+00	U1/2		2.30E+00	2.3E+02	4.6E+00	1.5E+01	10	300	3.08E+03	103%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1316-T03-A	1	8.39E+00	E		8.39E+00	2.1E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1316-T04-A	1	2.23E+01			2.23E+01	6.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1316-T05-A	1	2.82E+01			2.82E+01	3.8E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1316-T01-B	1	2.30E+00	U1/2		2.30E+00	7.9E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1316-T02-B	1	2.30E+00	U1/2		2.30E+00	2.4E+03	4.6E+00	1.5E+01	10	300	3.04E+03	101%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1316-T03-B	1	6.47E+00	E		6.47E+00	2.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1316-T04-B	1	2.14E+01			2.14E+01	7.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1316-T05-B	1	3.09E+01			3.09E+01	3.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1316-T01-C	1	2.30E+00	U1/2		2.30E+00	4.4E+03	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1316-T02-C	1	2.30E+00	U1/2		2.30E+00	1.2E+02	4.6E+00	1.5E+01	10	300	3.04E+03	101%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1316-T03-C	1	1.62E+01			1.62E+01	1.8E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1316-T04-C	1	2.30E+01			2.30E+01	3.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1316-T05-C	1	2.45E+01			2.45E+01	3.8E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
Tl	EaFA-L07-1316-B01-A	1	2.30E+00	U1/2		2.30E+00	1.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	EaFA-L07-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	1.5E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	3.6E+01	2.0E+00	6.4E+00	10	300	3.18E+03	106%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	7.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	3.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1316-T05-A	1	1.00E+00	U1/2		1.00E+00	9.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	6.0E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	3.3E+02	2.0E+00	6.4E+00	10	300	3.17E+03	106%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	3.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	2.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1316-T05-B	1	1.00E+00	U1/2		1.00E+00	4.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	7.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	2.6E+02	2.0E+00	6.4E+00	10	300	3.13E+03	104%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	6.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	8.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1316-T05-C	1	4.90E+00	E		4.90E+00	2.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
Ti	EaFA-L07-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	6.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	EaFA-L07-1316-T01-A	1	2.70E+02			2.70E+02	5.9E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1316-T02-A	1	2.83E+02			2.83E+02	8.5E-01	1.5E+00	4.8E+00	10	300	3.55E+03	109%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1316-T03-A	1	3.25E+02			3.25E+02	4.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1316-T04-A	1	3.73E+02			3.73E+02	1.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1316-T05-A	1	4.69E+02			4.69E+02	1.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1316-T01-B	1	2.71E+02			2.71E+02	9.6E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1316-T02-B	1	3.15E+02			3.15E+02	6.4E-01	1.5E+00	4.8E+00	10	300	3.53E+03	107%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1316-T03-B	1	3.39E+02			3.39E+02	2.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1316-T04-B	1	4.00E+02			4.00E+02	6.9E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1316-T05-B	1	4.38E+02			4.38E+02	1.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1316-T01-C	1	2.48E+02			2.48E+02	2.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1316-T02-C	1	2.99E+02			2.99E+02	2.3E+00	1.5E+00	4.8E+00	10	300	3.48E+03	106%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1316-T03-C	1	3.53E+02			3.53E+02	2.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1316-T04-C	1	3.95E+02			3.95E+02	1.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1316-T05-C	1	3.46E+02			3.46E+02	1.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
V	EaFA-L07-1316-B01-A	1	7.50E-01	U1/2		7.50E-01	4.0E+02	1.5E+00	4.8E+00				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	EaFA-L07-1316-T01-A	1	8.33E+00			8.33E+00	2.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:09 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1316-T02-A	1	2.10E+01			2.10E+01	3.5E+00	1.0E+00	3.2E+00	10	300	3.29E+03	109%	VU ICP-OES	6/4/10 3:11 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1316-T03-A	1	3.06E+01			3.06E+01	9.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:12 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1316-T04-A	1	1.45E+01			1.45E+01	3.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:14 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1316-T05-A	1	2.02E+01			2.02E+01	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:15 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1316-T01-B	1	1.36E+01			1.36E+01	5.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:17 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1316-T02-B	1	2.08E+01			2.08E+01	4.7E+00	1.0E+00	3.2E+00	10	300	3.26E+03	108%	VU ICP-OES	6/4/10 3:19 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1316-T03-B	1	3.26E+01			3.26E+01	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:20 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1316-T04-B	1	1.65E+01			1.65E+01	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:22 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1316-T05-B	1	2.48E+02			2.48E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:24 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1316-T01-C	1	2.03E+01			2.03E+01	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:15 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1316-T02-C	1	2.36E+01			2.36E+01	5.2E+00	1.0E+00	3.2E+00	10	300	3.25E+03	108%	VU ICP-OES	6/4/10 3:27 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1316-T03-C	1	3.68E+01			3.68E+01	4.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:29 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1316-T04-C	1	1.14E+01			1.14E+01	6.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:30 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1316-T05-C	1	1.90E+01			1.90E+01	3.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 4:07 PM	EPA Interlab L07 1313-1316 EaFA
Zn	EaFA-L07-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	7.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/4/10 3:04 PM	EPA Interlab L07 1313-1316 EaFA

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	EaFA-L08-1316-T01-A	1	1.43E+02			1.43E+02	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1316-T02-A	1	1.63E+02			1.63E+02	9.0E+00	1.0E+00	3.2E+00	1000	100	1.09E+03	93%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1316-T03-A	1	2.98E+02			2.98E+02	5.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1316-T04-A	1	5.02E+02			5.02E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1316-T05-A	1	6.37E+02			6.37E+02	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1316-T01-B	1	1.54E+02			1.54E+02	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1316-T02-B	1	2.28E+02			2.28E+02	1.1E+00	1.0E+00	3.2E+00	1000	100	1.14E+03	91%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1316-T03-B	1	2.45E+02			2.45E+02	1.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1316-T04-B	1	4.76E+02			4.76E+02	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1316-T05-B	1	6.15E+02			6.15E+02	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1316-T01-C	1	1.77E+02			1.77E+02	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1316-T02-C	1	1.62E+02			1.62E+02	8.4E-01	1.0E+00	3.2E+00	1000	100	1.07E+03	90%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1316-T03-C	1	2.52E+02			2.52E+02	2.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1316-T04-C	1	4.65E+02			4.65E+02	6.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1316-T05-C	1	6.22E+02			6.22E+02	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
Al	EaFA-L08-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	6.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	EaFA-L08-1316-T01-A	1	2.05E+02			2.05E+02	8.9E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1316-T02-A	1	3.10E+02			3.10E+02	7.5E+00	7.5E+00	2.4E+01	10	300	3.57E+03	109%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1316-T03-A	1	5.99E+02			5.99E+02	2.9E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1316-T04-A	1	8.29E+02			8.29E+02	1.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1316-T05-A	1	1.19E+03			1.19E+03	1.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1316-T01-B	1	2.46E+02			2.46E+02	1.9E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1316-T02-B	1	4.07E+02			4.07E+02	3.4E+00	7.5E+00	2.4E+01	10	300	3.64E+03	108%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1316-T03-B	1	5.25E+02			5.25E+02	8.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1316-T04-B	1	7.17E+02			7.17E+02	2.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1316-T05-B	1	1.26E+03			1.26E+03	1.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1316-T01-C	1	2.73E+02			2.73E+02	7.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1316-T02-C	1	3.24E+02			3.24E+02	5.7E+00	7.5E+00	2.4E+01	10	300	3.47E+03	105%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1316-T03-C	1	5.50E+02			5.50E+02	2.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1316-T04-C	1	6.87E+02			6.87E+02	3.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1316-T05-C	1	1.20E+03			1.20E+03	1.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
Sb	EaFA-L08-1316-B01-A	1	3.75E+00	U1/2		3.75E+00	8.4E+01	7.5E+00	2.4E+01				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	EaFA-L08-1316-T01-A	1	1.76E+02			1.76E+02	5.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1316-T02-A	1	1.62E+02			1.62E+02	7.3E+00	1.1E+01	3.5E+01	10	300	3.39E+03	107%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1316-T03-A	1	2.62E+02			2.62E+02	1.2E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1316-T04-A	1	3.11E+02			3.11E+02	8.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1316-T05-A	1	4.16E+02			4.16E+02	2.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1316-T01-B	1	1.60E+02			1.60E+02	7.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1316-T02-B	1	2.40E+02			2.40E+02	4.5E+00	1.1E+01	3.5E+01	10	300	3.50E+03	109%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1316-T03-B	1	2.04E+02			2.04E+02	3.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1316-T04-B	1	2.26E+02			2.26E+02	5.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1316-T05-B	1	4.06E+02			4.06E+02	5.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1316-T01-C	1	1.65E+02			1.65E+02	1.6E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1316-T02-C	1	1.65E+02			1.65E+02	2.0E+01	1.1E+01	3.5E+01	10	300	3.31E+03	105%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1316-T03-C	1	2.22E+02			2.22E+02	2.0E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1316-T04-C	1	2.07E+02			2.07E+02	9.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1316-T05-C	1	4.22E+02			4.22E+02	5.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
As	EaFA-L08-1316-B01-A	1	5.50E+00	U1/2		5.50E+00	3.4E+02	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	EaFA-L08-1316-T01-A	1	4.21E+03			4.21E+03	6.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1316-T02-A	1	7.67E+03			7.67E+03	8.3E+00	1.0E+00	3.2E+00	1000	100	8.58E+03	90%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1316-T03-A	1	2.08E+04			2.08E+04	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1316-T04-A	1	3.86E+04			3.86E+04	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1316-T05-A	1	6.90E+04			6.90E+04	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1316-T01-B	1	5.49E+03			5.49E+03	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1316-T02-B	1	9.20E+03			9.20E+03	2.5E+00	1.0E+00	3.2E+00	1000	100	1.01E+04	86%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1316-T03-B	1	1.88E+04			1.88E+04	9.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1316-T04-B	1	3.70E+04			3.70E+04	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1316-T05-B	1	6.60E+04			6.60E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1316-T01-C	1	4.90E+03			4.90E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1316-T02-C	1	8.43E+03			8.43E+03	1.5E+00	1.0E+00	3.2E+00	1000	100	9.28E+03	85%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1316-T03-C	1	2.11E+04			2.11E+04	3.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1316-T04-C	1	3.61E+04			3.61E+04	6.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1316-T05-C	1	6.48E+04			6.48E+04	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
B	EaFA-L08-1316-B01-A	1	2.65E+01			2.65E+01	6.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	EaFA-L08-1316-T01-A	1	2.69E+02			2.69E+02	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1316-T02-A	1	1.93E+02			1.93E+02	8.9E+00	1.0E+00	3.2E+00	10	300	3.11E+03	97%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1316-T03-A	1	2.06E+02			2.06E+02	6.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1316-T04-A	1	2.58E+02			2.58E+02	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1316-T05-A	1	2.45E+02			2.45E+02	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1316-T01-B	1	2.65E+02			2.65E+02	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1316-T02-B	1	2.39E+02			2.39E+02	1.2E+00	1.0E+00	3.2E+00	10	300	3.14E+03	97%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1316-T03-B	1	1.91E+02			1.91E+02	9.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1316-T04-B	1	2.41E+02			2.41E+02	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1316-T05-B	1	2.57E+02			2.57E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1316-T01-C	1	2.79E+02			2.79E+02	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1316-T02-C	1	1.99E+02			1.99E+02	1.3E+00	1.0E+00	3.2E+00	10	300	3.04E+03	95%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1316-T03-C	1	2.03E+02			2.03E+02	3.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1316-T04-C	1	2.28E+02			2.28E+02	6.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1316-T05-C	1	2.54E+02			2.54E+02	2.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
Ba	EaFA-L08-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	EaFA-L08-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	2.3E+02	1.9E+00	6.0E+00	10	300	3.33E+03	111%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	8.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	4.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1316-T05-A	1	9.50E-01	U1/2		9.50E-01	5.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	2.4E+03	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	7.2E+02	1.9E+00	6.0E+00	10	300	3.34E+03	111%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	5.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	1.0E+03	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1316-T05-B	1	9.50E-01	U1/2		9.50E-01	7.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	2.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	1.7E+03	1.9E+00	6.0E+00	10	300	3.28E+03	109%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	4.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	6.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1316-T05-C	1	9.50E-01	U1/2		9.50E-01	5.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
Be	EaFA-L08-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	6.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	EaFA-L08-1316-T01-A	1	1.10E+00	U1/2		1.10E+00	1.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1316-T02-A	1	1.10E+00	U1/2		1.10E+00	4.3E+01	2.2E+00	7.0E+00	10	300	3.27E+03	109%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1316-T03-A	1	4.05E+00	E		4.05E+00	1.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1316-T04-A	1	1.10E+00	U1/2		1.10E+00	2.7E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1316-T05-A	1	2.88E+00	E		2.88E+00	2.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1316-T01-B	1	1.10E+00	U1/2		1.10E+00	6.3E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1316-T02-B	1	1.10E+00	U1/2		1.10E+00	6.3E+01	2.2E+00	7.0E+00	10	300	3.28E+03	109%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1316-T03-B	1	4.56E+00	E		4.56E+00	1.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1316-T04-B	1	1.10E+00	U1/2		1.10E+00	4.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1316-T05-B	1	3.58E+00	E		3.58E+00	2.5E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1316-T01-C	1	1.10E+00	U1/2		1.10E+00	8.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1316-T02-C	1	1.10E+00	U1/2		1.10E+00	4.6E+01	2.2E+00	7.0E+00	10	300	3.21E+03	107%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1316-T03-C	1	4.36E+00	E		4.36E+00	1.9E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1316-T04-C	1	1.10E+00	U1/2		1.10E+00	7.6E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1316-T05-C	1	1.10E+00	U1/2		1.10E+00	3.7E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
Cd	EaFA-L08-1316-B01-A	1	1.10E+00	U1/2		1.10E+00	1.1E+02	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	EaFA-L08-1316-T01-A	1	1.54E+05			1.54E+05	2.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1316-T02-A	1	2.73E+05			2.73E+05	9.4E+00	2.6E+00	8.3E+00	1000	100	2.74E+05	95%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1316-T03-A	1	7.49E+05			7.49E+05	7.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1316-T04-A	1	5.65E+05			5.65E+05	1.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1316-T05-A	1	5.09E+05			5.09E+05	4.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1316-T01-B	1	1.52E+05			1.52E+05	4.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1316-T02-B	1	3.04E+05			3.04E+05	1.4E+00	2.6E+00	8.3E+00	1000	100	3.05E+05	90%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1316-T03-B	1	6.46E+05			6.46E+05	9.5E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1316-T04-B	1	5.62E+05			5.62E+05	6.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1316-T05-B	1	4.89E+05			4.89E+05	1.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1316-T01-C	1	1.66E+05			1.66E+05	4.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1316-T02-C	1	2.92E+05			2.92E+05	1.0E+00	2.6E+00	8.3E+00	1000	100	2.93E+05	85%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1316-T03-C	1	7.26E+05			7.26E+05	1.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1316-T04-C	1	5.44E+05			5.44E+05	6.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1316-T05-C	1	4.98E+05			4.98E+05	4.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
Ca	EaFA-L08-1316-B01-A	1	6.43E+00	E		6.43E+00	2.6E+01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	EaFA-L08-1316-T01-A	1	1.72E+01			1.72E+01	1.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1316-T02-A	1	1.89E+01			1.89E+01	1.5E+01	1.2E+00	3.8E+00	10	300	3.10E+03	103%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1316-T03-A	1	3.00E+01			3.00E+01	1.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1316-T04-A	1	4.99E+01			4.99E+01	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1316-T05-A	1	1.58E+01			1.58E+01	4.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1316-T01-B	1	1.82E+01			1.82E+01	1.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1316-T02-B	1	2.33E+01			2.33E+01	8.8E+00	1.2E+00	3.8E+00	10	300	3.09E+03	102%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1316-T03-B	1	2.16E+01			2.16E+01	1.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1316-T04-B	1	5.36E+01			5.36E+01	3.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1316-T05-B	1	1.45E+01			1.45E+01	9.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1316-T01-C	1	2.05E+01			2.05E+01	8.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1316-T02-C	1	1.93E+01			1.93E+01	1.3E+00	1.2E+00	3.8E+00	10	300	3.04E+03	101%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1316-T03-C	1	2.48E+01			2.48E+01	8.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1316-T04-C	1	6.02E+01			6.02E+01	4.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1316-T05-C	1	2.19E+01			2.19E+01	2.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
Cr	EaFA-L08-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	1.5E+02	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	EaFA-L08-1316-T01-A	1	5.33E+01			5.33E+01	1.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1316-T02-A	1	8.12E+01			8.12E+01	1.0E+01	1.8E+00	5.7E+00	10	300	3.17E+03	103%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1316-T03-A	1	1.56E+02			1.56E+02	3.9E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1316-T04-A	1	9.60E+01			9.60E+01	2.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1316-T05-A	1	1.63E+02			1.63E+02	1.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1316-T01-B	1	4.98E+01			4.98E+01	9.4E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1316-T02-B	1	7.22E+01			7.22E+01	1.3E+00	1.8E+00	5.7E+00	10	300	3.16E+03	103%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1316-T03-B	1	1.47E+02			1.47E+02	8.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1316-T04-B	1	9.48E+01			9.48E+01	1.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1316-T05-B	1	1.72E+02			1.72E+02	1.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1316-T01-C	1	4.97E+01			4.97E+01	6.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1316-T02-C	1	9.19E+01			9.19E+01	1.7E+00	1.8E+00	5.7E+00	10	300	3.11E+03	101%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1316-T03-C	1	1.76E+02			1.76E+02	8.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1316-T04-C	1	8.56E+01			8.56E+01	6.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1316-T05-C	1	1.39E+02			1.39E+02	2.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
Co	EaFA-L08-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	3.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	EaFA-L08-1316-T01-A	1	9.72E+00	E		9.72E+00	2.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1316-T02-A	1	8.35E+00	E		8.35E+00	4.3E+01	3.7E+00	1.2E+01	10	300	3.11E+03	103%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1316-T03-A	1	1.62E+01			1.62E+01	3.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1316-T04-A	1	1.11E+01	E		1.11E+01	2.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1316-T05-A	1	1.37E+01			1.37E+01	2.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1316-T01-B	1	7.11E+00	E		7.11E+00	2.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1316-T02-B	1	7.04E+00	E		7.04E+00	9.1E+01	3.7E+00	1.2E+01	10	300	3.12E+03	104%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1316-T03-B	1	1.34E+01			1.34E+01	1.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1316-T04-B	1	1.20E+01			1.20E+01	1.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1316-T05-B	1	1.39E+01			1.39E+01	9.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1316-T01-C	1	7.38E+00	E		7.38E+00	1.2E+02	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1316-T02-C	1	1.39E+01			1.39E+01	1.7E+01	3.7E+00	1.2E+01	10	300	3.06E+03	101%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1316-T03-C	1	1.08E+01	E		1.08E+01	3.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1316-T04-C	1	7.91E+00	E		7.91E+00	3.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1316-T05-C	1	1.07E+01	E		1.07E+01	5.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
Cu	EaFA-L08-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	7.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	EaFA-L08-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00	1000	100	1.01E+03	101%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1316-T05-A	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	7.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00	1000	100	1.00E+03	100%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	7.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1316-T05-B	1	3.25E+00	E		3.25E+00	3.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	4.1E+00	2.0E+00	6.4E+00	1000	100	9.86E+02	99%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	7.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	3.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1316-T05-C	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
Fe	EaFA-L08-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	8.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	EaFA-L08-1316-T01-A	1	3.40E+00	U1/2		3.40E+00	1.3E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1316-T02-A	1	3.40E+00	U1/2		3.40E+00	6.6E+01	6.8E+00	2.2E+01	10	300	3.11E+03	104%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1316-T03-A	1	3.40E+00	U1/2		3.40E+00	6.9E+03	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1316-T04-A	1	3.40E+00	U1/2		3.40E+00	6.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1316-T05-A	1	3.40E+00	U1/2		3.40E+00	5.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1316-T01-B	1	3.40E+00	U1/2		3.40E+00	6.8E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1316-T02-B	1	3.40E+00	U1/2		3.40E+00	1.0E+02	6.8E+00	2.2E+01	10	300	3.11E+03	104%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1316-T03-B	1	3.40E+00	U1/2		3.40E+00	3.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1316-T04-B	1	3.40E+00	U1/2		3.40E+00	1.3E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1316-T05-B	1	3.40E+00	U1/2		3.40E+00	5.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1316-T01-C	1	3.40E+00	U1/2		3.40E+00	1.3E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1316-T02-C	1	3.40E+00	U1/2		3.40E+00	4.6E+01	6.8E+00	2.2E+01	10	300	3.05E+03	101%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1316-T03-C	1	3.40E+00	U1/2		3.40E+00	2.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1316-T04-C	1	3.40E+00	U1/2		3.40E+00	5.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1316-T05-C	1	3.40E+00	U1/2		3.40E+00	6.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
Pb	EaFA-L08-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	1.5E+02	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	EaFA-L08-1316-T01-A	1	3.42E+03			3.42E+03	1.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1316-T02-A	1	5.83E+03			5.83E+03	9.1E+00	1.9E+00	6.0E+00	10	300	8.52E+03	90%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1316-T03-A	1	1.58E+04			1.58E+04	5.6E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1316-T04-A	1	2.95E+04			2.95E+04	9.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1316-T05-A	1	5.85E+04			5.85E+04	4.0E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1316-T01-B	1	3.37E+03			3.37E+03	9.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1316-T02-B	1	6.40E+03			6.40E+03	8.0E-01	1.9E+00	6.0E+00	10	300	8.95E+03	85%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1316-T03-B	1	1.37E+04			1.37E+04	9.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1316-T04-B	1	2.99E+04			2.99E+04	7.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1316-T05-B	1	5.48E+04			5.48E+04	1.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1316-T01-C	1	3.65E+03			3.65E+03	4.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1316-T02-C	1	6.23E+03			6.23E+03	1.3E+00	1.9E+00	6.0E+00	10	300	8.95E+03	91%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1316-T03-C	1	1.54E+04			1.54E+04	5.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1316-T04-C	1	2.87E+04			2.87E+04	6.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1316-T05-C	1	5.48E+04			5.48E+04	3.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
Li	EaFA-L08-1316-B01-A	1	5.11E+01			5.11E+01	1.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	EaFA-L08-1316-T01-A	1	3.96E+02			3.96E+02	1.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1316-T02-A	1	6.23E+02			6.23E+02	8.5E+00	2.0E+00	6.4E+00	10	300	3.84E+03	107%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1316-T03-A	1	1.30E+03			1.30E+03	4.4E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1316-T04-A	1	1.10E+03			1.10E+03	5.4E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1316-T05-A	1	1.94E+03			1.94E+03	3.5E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1316-T01-B	1	3.79E+02			3.79E+02	6.3E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1316-T02-B	1	6.24E+02			6.24E+02	6.0E+00	2.0E+00	6.4E+00	10	300	3.78E+03	105%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1316-T03-B	1	1.19E+03			1.19E+03	9.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1316-T04-B	1	1.10E+03			1.10E+03	7.0E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1316-T05-B	1	2.07E+03			2.07E+03	5.8E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1316-T01-C	1	3.98E+02			3.98E+02	1.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1316-T02-C	1	6.70E+02			6.70E+02	1.7E+00	2.0E+00	6.4E+00	10	300	3.81E+03	105%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1316-T03-C	1	1.40E+03			1.40E+03	1.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1316-T04-C	1	9.82E+02			9.82E+02	4.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1316-T05-C	1	1.70E+03			1.70E+03	6.3E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
Mn	EaFA-L08-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	6.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	EaFA-L08-1316-T01-A	1	6.75E+03			6.75E+03	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1316-T02-A	1	1.19E+04			1.19E+04	8.5E+00	1.0E+00	3.2E+00	1000	100	1.28E+04	86%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1316-T03-A	1	3.53E+04			3.53E+04	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1316-T04-A	1	6.40E+04			6.40E+04	8.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1316-T05-A	1	1.21E+05			1.21E+05	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1316-T01-B	1	6.73E+03			6.73E+03	9.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1316-T02-B	1	1.37E+04			1.37E+04	1.6E+00	1.0E+00	3.2E+00	1000	100	1.46E+04	93%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1316-T03-B	1	2.99E+04			2.99E+04	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1316-T04-B	1	6.36E+04			6.36E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1316-T05-B	1	1.12E+05			1.12E+05	8.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1316-T01-C	1	7.27E+03			7.27E+03	3.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1316-T02-C	1	1.26E+04			1.26E+04	1.1E+00	1.0E+00	3.2E+00	1000	100	1.35E+04	89%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1316-T03-C	1	3.37E+04			3.37E+04	7.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1316-T04-C	1	6.09E+04			6.09E+04	5.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1316-T05-C	1	1.11E+05			1.11E+05	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
Mg	EaFA-L08-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	5.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	EaFA-L08-1316-T01-A	1	3.32E+03			3.32E+03	2.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1316-T02-A	1	5.76E+03			5.76E+03	8.9E+00	1.2E+00	3.8E+00	10	300	8.65E+03	96%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1316-T03-A	1	1.58E+04			1.58E+04	8.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1316-T04-A	1	2.96E+04			2.96E+04	7.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1316-T05-A	1	5.36E+04			5.36E+04	2.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1316-T01-B	1	3.35E+03			3.35E+03	9.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1316-T02-B	1	6.67E+03			6.67E+03	8.9E-01	1.2E+00	3.8E+00	10	300	9.16E+03	83%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1316-T03-B	1	1.37E+04			1.37E+04	8.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1316-T04-B	1	2.88E+04			2.88E+04	2.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1316-T05-B	1	4.91E+04			4.91E+04	9.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1316-T01-C	1	3.61E+03			3.61E+03	5.1E-02	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1316-T02-C	1	5.99E+03			5.99E+03	1.5E+00	1.2E+00	3.8E+00	10	300	8.60E+03	87%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1316-T03-C	1	1.49E+04			1.49E+04	4.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1316-T04-C	1	2.79E+04			2.79E+04	6.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1316-T05-C	1	5.23E+04			5.23E+04	2.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
Mo	EaFA-L08-1316-B01-A	1	6.25E+00			6.25E+00	1.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	EaFA-L08-1316-T01-A	1	1.24E+02			1.24E+02	4.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1316-T02-A	1	1.96E+02			1.96E+02	9.1E+00	1.8E+00	5.7E+00	10	300	3.33E+03	105%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1316-T03-A	1	3.82E+02			3.82E+02	1.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1316-T04-A	1	2.13E+02			2.13E+02	1.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1316-T05-A	1	3.69E+02			3.69E+02	2.4E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1316-T01-B	1	1.11E+02			1.11E+02	2.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1316-T02-B	1	1.80E+02			1.80E+02	2.0E+00	1.8E+00	5.7E+00	10	300	3.30E+03	104%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1316-T03-B	1	3.54E+02			3.54E+02	9.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1316-T04-B	1	2.27E+02			2.27E+02	1.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1316-T05-B	1	4.08E+02			4.08E+02	1.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1316-T01-C	1	1.24E+02			1.24E+02	3.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1316-T02-C	1	2.14E+02			2.14E+02	5.4E+00	1.8E+00	5.7E+00	10	300	3.28E+03	102%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1316-T03-C	1	4.19E+02			4.19E+02	3.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1316-T04-C	1	2.03E+02			2.03E+02	8.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1316-T05-C	1	3.31E+02			3.31E+02	4.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
Ni	EaFA-L08-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	EaFA-L08-1316-T01-A	1	1.93E+01			1.93E+01	5.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1316-T02-A	1	4.03E+01			4.03E+01	3.0E+01	3.7E+00	1.2E+01	1000	100	1.10E+03	106%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1316-T03-A	1	1.90E+02			1.90E+02	1.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1316-T04-A	1	3.94E+02			3.94E+02	6.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1316-T05-A	1	1.51E+02			1.51E+02	1.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1316-T01-B	1	3.18E+01			3.18E+01	2.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1316-T02-B	1	4.55E+01			4.55E+01	1.4E+01	3.7E+00	1.2E+01	1000	100	1.15E+03	111%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1316-T03-B	1	1.51E+02			1.51E+02	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1316-T04-B	1	3.56E+02			3.56E+02	2.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1316-T05-B	1	1.31E+03			1.31E+03	4.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1316-T01-C	1	2.71E+01			2.71E+01	3.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1316-T02-C	1	1.23E+02			1.23E+02	4.6E+00	3.7E+00	1.2E+01	1000	100	1.12E+03	100%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1316-T03-C	1	2.15E+02			2.15E+02	5.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1316-T04-C	1	3.35E+02			3.35E+02	1.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1316-T05-C	1	1.11E+03			1.11E+03	2.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
P	EaFA-L08-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	1.3E+03	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	EaFA-L08-1316-T01-A	1	2.39E+04			2.39E+04	1.5E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1316-T02-A	1	4.33E+04			4.33E+04	9.6E+00	1.6E+00	5.1E+00	1000	100	4.42E+04	87%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1316-T03-A	1	1.26E+05			1.26E+05	9.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1316-T04-A	1	1.87E+05			1.87E+05	4.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1316-T05-A	1	2.96E+05			2.96E+05	2.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1316-T01-B	1	2.35E+04			2.35E+04	6.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1316-T02-B	1	4.77E+04			4.77E+04	4.8E-01	1.6E+00	5.1E+00	1000	100	4.86E+04	83%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1316-T03-B	1	1.07E+05			1.07E+05	1.0E+01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1316-T04-B	1	1.91E+05			1.91E+05	5.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1316-T05-B	1	2.79E+05			2.79E+05	4.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1316-T01-C	1	2.55E+04			2.55E+04	5.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1316-T02-C	1	4.65E+04			4.65E+04	9.6E-01	1.6E+00	5.1E+00	1000	100	4.74E+04	82%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1316-T03-C	1	1.22E+05			1.22E+05	2.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1316-T04-C	1	1.85E+05			1.85E+05	4.6E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1316-T05-C	1	2.80E+05			2.80E+05	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
K	EaFA-L08-1316-B01-A	1	3.38E+01			3.38E+01	6.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	EaFA-L08-1316-T01-A	1	1.54E+03			1.54E+03	1.2E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1316-T02-A	1	1.73E+03			1.73E+03	9.4E+00	1.5E+01	4.8E+01	10	300	4.94E+03	107%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1316-T03-A	1	2.68E+03			2.68E+03	4.1E-01	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1316-T04-A	1	3.90E+03			3.90E+03	1.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1316-T05-A	1	4.55E+03			4.55E+03	5.2E-01	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1316-T01-B	1	1.60E+03			1.60E+03	1.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1316-T02-B	1	2.72E+03			2.72E+03	1.6E+00	1.5E+01	4.8E+01	10	300	5.70E+03	99%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1316-T03-B	1	2.39E+03			2.39E+03	9.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1316-T04-B	1	3.02E+03			3.02E+03	4.9E-01	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1316-T05-B	1	4.63E+03			4.63E+03	9.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1316-T01-C	1	1.77E+03			1.77E+03	3.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1316-T02-C	1	1.74E+03			1.74E+03	1.1E+00	1.5E+01	4.8E+01	10	300	4.82E+03	103%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1316-T03-C	1	2.22E+03			2.22E+03	1.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1316-T04-C	1	2.92E+03			2.92E+03	6.8E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1316-T05-C	1	4.78E+03			4.78E+03	4.8E-01	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
Se	EaFA-L08-1316-B01-A	1	6.75E+01			6.75E+01	3.8E+01	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	EaFA-L08-1316-T01-A	1	3.07E+03			3.07E+03	1.6E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1316-T02-A	1	3.00E+03			3.00E+03	8.6E+00	1.1E+00	3.5E+00	1000	100	3.88E+03	87%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1316-T03-A	1	3.40E+03			3.40E+03	1.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1316-T04-A	1	3.12E+03			3.12E+03	8.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1316-T05-A	1	4.16E+03			4.16E+03	5.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1316-T01-B	1	3.03E+03			3.03E+03	7.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1316-T02-B	1	3.97E+03			3.97E+03	1.1E+00	1.1E+00	3.5E+00	1000	100	4.85E+03	88%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1316-T03-B	1	3.22E+03			3.22E+03	9.6E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1316-T04-B	1	2.51E+03			2.51E+03	9.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1316-T05-B	1	4.57E+03			4.57E+03	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1316-T01-C	1	3.28E+03			3.28E+03	3.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1316-T02-C	1	3.08E+03			3.08E+03	1.4E+00	1.1E+00	3.5E+00	1000	100	4.02E+03	94%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1316-T03-C	1	3.27E+03			3.27E+03	1.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1316-T04-C	1	2.29E+03			2.29E+03	6.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1316-T05-C	1	3.91E+03			3.91E+03	5.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
Si	EaFA-L08-1316-B01-A	1	5.50E-01	U1/2		5.50E-01	3.3E+01	1.1E+00	3.5E+00				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	EaFA-L08-1316-T01-A	1	4.87E+03			4.87E+03	2.4E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1316-T02-A	1	8.85E+03			8.85E+03	9.5E+00	2.5E+00	8.0E+00	1000	100	9.74E+03	89%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1316-T03-A	1	2.58E+04			2.58E+04	8.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1316-T04-A	1	4.04E+04			4.04E+04	7.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1316-T05-A	1	6.83E+04			6.83E+04	3.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1316-T01-B	1	4.80E+03			4.80E+03	7.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1316-T02-B	1	9.63E+03			9.63E+03	5.6E-01	2.5E+00	8.0E+00	1000	100	1.06E+04	94%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1316-T03-B	1	2.21E+04			2.21E+04	9.9E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1316-T04-B	1	4.16E+04			4.16E+04	6.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1316-T05-B	1	6.45E+04			6.45E+04	8.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1316-T01-C	1	5.15E+03			5.15E+03	2.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1316-T02-C	1	9.45E+03			9.45E+03	1.6E+00	2.5E+00	8.0E+00	1000	100	1.03E+04	89%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1316-T03-C	1	2.50E+04			2.50E+04	7.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1316-T04-C	1	3.96E+04			3.96E+04	6.0E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1316-T05-C	1	6.44E+04			6.44E+04	3.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
Na	EaFA-L08-1316-B01-A	1	2.32E+01			2.32E+01	3.7E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	EaFA-L08-1316-T01-A	1	2.07E+03			2.07E+03	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1316-T02-A	1	3.50E+03			3.50E+03	7.9E+00	1.0E+00	3.2E+00	1000	100	4.39E+03	89%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1316-T03-A	1	8.59E+03			8.59E+03	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1316-T04-A	1	7.95E+03			7.95E+03	7.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1316-T05-A	1	6.49E+03			6.49E+03	1.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1316-T01-B	1	2.07E+03			2.07E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1316-T02-B	1	4.05E+03			4.05E+03	5.1E+00	1.0E+00	3.2E+00	1000	100	4.96E+03	91%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1316-T03-B	1	7.10E+03			7.10E+03	7.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1316-T04-B	1	8.60E+03			8.60E+03	8.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1316-T05-B	1	6.16E+03			6.16E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1316-T01-C	1	2.24E+03			2.24E+03	2.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1316-T02-C	1	3.63E+03			3.63E+03	1.4E+00	1.0E+00	3.2E+00	1000	100	4.58E+03	95%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1316-T03-C	1	8.08E+03			8.08E+03	2.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1316-T04-C	1	7.90E+03			7.90E+03	3.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1316-T05-C	1	6.73E+03			6.73E+03	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
Sr	EaFA-L08-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	EaFA-L08-1316-T01-A	1	1.50E+05			1.50E+05	2.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1316-T02-A	1	2.66E+05			2.66E+05	8.6E+00	6.8E+00	2.2E+01	1000	100	3.55E+05	89%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1316-T03-A	1	7.09E+05			7.09E+05	1.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1316-T04-A	1	7.14E+05			7.14E+05	1.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1316-T05-A	1	8.98E+05			8.98E+05	2.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1316-T01-B	1	1.49E+05			1.49E+05	8.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1316-T02-B	1	2.95E+05			2.95E+05	6.1E-01	6.8E+00	2.2E+01	1000	100	3.91E+05	96%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1316-T03-B	1	6.25E+05			6.25E+05	9.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1316-T04-B	1	7.14E+05			7.14E+05	6.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1316-T05-B	1	8.52E+05			8.52E+05	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1316-T01-C	1	1.57E+05			1.57E+05	5.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1316-T02-C	1	2.81E+05			2.81E+05	1.4E+00	6.8E+00	2.2E+01	1000	100	3.74E+05	92%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1316-T03-C	1	7.01E+05			7.01E+05	3.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1316-T04-C	1	6.95E+05			6.95E+05	6.3E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1316-T05-C	1	8.53E+05			8.53E+05	2.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
S	EaFA-L08-1316-B01-A	1	2.07E+01	E		2.07E+01	8.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	EaFA-L08-1316-T01-A	1	2.30E+00	U1/2		2.30E+00	2.6E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1316-T02-A	1	2.30E+00	U1/2		2.30E+00	4.9E+02	4.6E+00	1.5E+01	10	300	3.14E+03	104%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1316-T03-A	1	2.36E+01			2.36E+01	1.0E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1316-T04-A	1	4.97E+01			4.97E+01	2.9E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1316-T05-A	1	4.71E+01			4.71E+01	5.5E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1316-T01-B	1	2.30E+00	U1/2		2.30E+00	1.7E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1316-T02-B	1	2.40E+01			2.40E+01	1.3E+01	4.6E+00	1.5E+01	10	300	3.13E+03	104%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1316-T03-B	1	2.17E+01			2.17E+01	3.6E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1316-T04-B	1	2.22E+01			2.22E+01	4.4E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1316-T05-B	1	5.56E+01			5.56E+01	8.0E+00	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1316-T01-C	1	5.63E+00	E		5.63E+00	1.8E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1316-T02-C	1	1.51E+01			1.51E+01	1.0E+01	4.6E+00	1.5E+01	10	300	3.08E+03	102%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1316-T03-C	1	2.04E+01			2.04E+01	3.2E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1316-T04-C	1	3.20E+01			3.20E+01	4.5E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1316-T05-C	1	4.02E+01			4.02E+01	3.0E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
Tl	EaFA-L08-1316-B01-A	1	2.30E+00	U1/2		2.30E+00	1.3E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	EaFA-L08-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	1.0E+03	2.0E+00	6.4E+00	10	300	3.07E+03	102%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	9.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	7.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1316-T05-A	1	1.00E+00	U1/2		1.00E+00	1.6E+03	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	1.6E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	8.6E+01	2.0E+00	6.4E+00	10	300	3.06E+03	102%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	6.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1316-T05-B	1	2.22E+00	E		2.22E+00	3.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	1.1E+03	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	1.7E+02	2.0E+00	6.4E+00	10	300	2.99E+03	100%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	4.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1316-T05-C	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
Ti	EaFA-L08-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	2.8E+02	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	EaFA-L08-1316-T01-A	1	3.54E+02			3.54E+02	4.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1316-T02-A	1	3.71E+02			3.71E+02	9.3E+00	1.5E+00	4.8E+00	10	300	3.50E+03	104%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1316-T03-A	1	5.42E+02			5.42E+02	5.0E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1316-T04-A	1	6.31E+02			6.31E+02	2.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1316-T05-A	1	6.88E+02			6.88E+02	1.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1316-T01-B	1	3.79E+02			3.79E+02	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1316-T02-B	1	6.29E+02			6.29E+02	4.7E-01	1.5E+00	4.8E+00	10	300	3.72E+03	103%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1316-T03-B	1	4.86E+02			4.86E+02	9.9E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1316-T04-B	1	4.67E+02			4.67E+02	1.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1316-T05-B	1	7.42E+02			7.42E+02	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1316-T01-C	1	4.35E+02			4.35E+02	9.0E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1316-T02-C	1	3.63E+02			3.63E+02	1.0E+00	1.5E+00	4.8E+00	10	300	3.41E+03	102%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1316-T03-C	1	4.57E+02			4.57E+02	3.2E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1316-T04-C	1	4.45E+02			4.45E+02	6.9E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1316-T05-C	1	7.15E+02			7.15E+02	4.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
V	EaFA-L08-1316-B01-A	1	1.81E+00	E		1.81E+00	5.8E+01	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	EaFA-L08-1316-T01-A	1	2.23E+01			2.23E+01	5.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:47 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1316-T02-A	1	2.23E+01			2.23E+01	6.3E+00	1.0E+00	3.2E+00	10	300	3.26E+03	108%	VU ICP-OES	6/7/10 12:49 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1316-T03-A	1	4.54E+01			4.54E+01	3.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:47 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1316-T04-A	1	3.26E+01			3.26E+01	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:52 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1316-T05-A	1	6.33E+01			6.33E+01	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:54 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1316-T01-B	1	2.36E+01			2.36E+01	4.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:56 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1316-T02-B	1	2.83E+01			2.83E+01	2.3E+00	1.0E+00	3.2E+00	10	300	3.27E+03	108%	VU ICP-OES	6/7/10 12:57 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1316-T03-B	1	3.76E+01			3.76E+01	1.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:59 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1316-T04-B	1	3.72E+01			3.72E+01	2.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:01 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1316-T05-B	1	7.85E+01			7.85E+01	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:02 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1316-T01-C	1	2.55E+01			2.55E+01	3.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:49 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1316-T02-C	1	2.77E+01			2.77E+01	4.8E+00	1.0E+00	3.2E+00	10	300	3.21E+03	106%	VU ICP-OES	6/7/10 1:06 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1316-T03-C	1	4.18E+01			4.18E+01	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:07 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1316-T04-C	1	2.84E+01			2.84E+01	8.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:09 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1316-T05-C	1	5.40E+01			5.40E+01	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:10 PM	EPA Interlab L08 1313-1316 EaFA
Zn	EaFA-L08-1316-B01-A	1	1.00E+01			1.00E+01	4.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 12:42 PM	EPA Interlab L08 1313-1316 EaFA

QA-QC Spreadsheet 1316:

										Spike Sol'n						
Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Conc. µg/L	Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	EaFA-L09-1316-T01-A	1	1.86E+02			1.86E+02	1.5E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
Al	EaFA-L09-1316-T02-A	1	2.21E+02			2.21E+02	7.9E-01	1.00E+00	3.18E+00	1000	100	1.29E+03	107%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
Al	EaFA-L09-1316-T03-A	1	2.72E+02			2.72E+02	1.7E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
Al	EaFA-L09-1316-T04-A	1	5.00E+02			5.00E+02	1.5E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
Al	EaFA-L09-1316-T05-A	1	4.59E+02			4.59E+02	9.0E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
Al	EaFA-L09-1316-T01-B	1	1.75E+02			1.75E+02	1.2E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
Al	EaFA-L09-1316-T02-B	1	2.03E+02			2.03E+02	9.5E-01	1.00E+00	3.18E+00	1000	100	1.33E+03	113%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
Al	EaFA-L09-1316-T03-B	1	2.76E+02			2.76E+02	1.0E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
Al	EaFA-L09-1316-T04-B	1	4.85E+02			4.85E+02	2.1E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
Al	EaFA-L09-1316-T05-B	1	5.05E+02			5.05E+02	8.7E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
Al	EaFA-L09-1316-T01-C	1	1.73E+02			1.73E+02	1.3E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
Al	EaFA-L09-1316-T02-C	1	2.10E+02			2.10E+02	6.4E-01	1.00E+00	3.18E+00	1000	100	1.34E+03	113%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
Al	EaFA-L09-1316-T03-C	1	2.70E+02			2.70E+02	1.6E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
Al	EaFA-L09-1316-T04-C	1	4.81E+02			4.81E+02	1.3E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
Al	EaFA-L09-1316-T05-C	1	5.12E+02			5.12E+02	4.1E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
Al	EaFA-L09-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	2.2E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	EaFA-L09-1316-T01-A	1	2.08E+02			2.08E+02	1.3E+00	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
Sb	EaFA-L09-1316-T02-A	1	2.97E+02			2.97E+02	5.9E+00	7.50E+00	2.39E+01	10	325	3.55E+03	100%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
Sb	EaFA-L09-1316-T03-A	1	4.49E+02			4.49E+02	2.4E+00	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
Sb	EaFA-L09-1316-T04-A	1	5.98E+02			5.98E+02	4.4E+00	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
Sb	EaFA-L09-1316-T05-A	1	5.90E+02			5.90E+02	1.1E+01	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
Sb	EaFA-L09-1316-T01-B	1	2.22E+02			2.22E+02	1.1E+01	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
Sb	EaFA-L09-1316-T02-B	1	3.44E+02			3.44E+02	2.0E+00	7.50E+00	2.39E+01	10	325	3.73E+03	104%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
Sb	EaFA-L09-1316-T03-B	1	4.63E+02			4.63E+02	6.9E+00	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
Sb	EaFA-L09-1316-T04-B	1	5.94E+02			5.94E+02	7.3E+00	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
Sb	EaFA-L09-1316-T05-B	1	3.77E+02			3.77E+02	8.5E+01	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
Sb	EaFA-L09-1316-T01-C	1	2.08E+02			2.08E+02	6.3E+00	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
Sb	EaFA-L09-1316-T02-C	1	3.38E+02			3.38E+02	7.8E+00	7.50E+00	2.39E+01	10	325	3.72E+03	104%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
Sb	EaFA-L09-1316-T03-C	1	4.60E+02			4.60E+02	8.1E+00	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
Sb	EaFA-L09-1316-T04-C	1	5.75E+02			5.75E+02	4.5E+00	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
Sb	EaFA-L09-1316-T05-C	1	3.77E+02			3.77E+02	4.9E+01	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
Sb	EaFA-L09-1316-B01-A	1	1.79E+01	E		1.79E+01	6.2E+01	7.50E+00	2.39E+01				---	VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	EaFA-L09-1316-T01-A	1	1.53E+02			1.53E+02	9.8E+00	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
As	EaFA-L09-1316-T02-A	1	1.65E+02			1.65E+02	4.3E+00	1.10E+01	3.50E+01	10	325	3.36E+03	98%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
As	EaFA-L09-1316-T03-A	1	1.52E+02			1.52E+02	1.6E+01	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
As	EaFA-L09-1316-T04-A	1	2.41E+02			2.41E+02	6.5E+00	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
As	EaFA-L09-1316-T05-A	1	1.69E+02			1.69E+02	1.8E+01	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
As	EaFA-L09-1316-T01-B	1	1.57E+02			1.57E+02	6.0E+00	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
As	EaFA-L09-1316-T02-B	1	1.37E+02			1.37E+02	6.1E+00	1.10E+01	3.50E+01	10	325	3.52E+03	104%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
As	EaFA-L09-1316-T03-B	1	1.40E+02			1.40E+02	1.7E+01	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
As	EaFA-L09-1316-T04-B	1	1.80E+02			1.80E+02	1.3E+01	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
As	EaFA-L09-1316-T05-B	1	2.56E+02			2.56E+02	7.3E+01	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
As	EaFA-L09-1316-T01-C	1	1.52E+02			1.52E+02	1.5E+01	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
As	EaFA-L09-1316-T02-C	1	1.44E+02			1.44E+02	1.5E+01	1.10E+01	3.50E+01	10	325	3.53E+03	104%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
As	EaFA-L09-1316-T03-C	1	1.72E+02			1.72E+02	3.5E+00	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
As	EaFA-L09-1316-T04-C	1	1.88E+02			1.88E+02	1.2E+01	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
As	EaFA-L09-1316-T05-C	1	1.32E+02			1.32E+02	4.0E+01	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
As	EaFA-L09-1316-B01-A	1	3.77E+01			3.77E+01	5.4E+01	1.10E+01	3.50E+01				---	VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	EaFA-L09-1316-T01-A	1	4.48E+03			4.48E+03	2.9E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
B	EaFA-L09-1316-T02-A	1	8.83E+03			8.83E+03	2.1E+00	1.00E+00	3.18E+00	1000	100	9.69E+03	87%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
B	EaFA-L09-1316-T03-A	1	2.12E+04			2.12E+04	7.6E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
B	EaFA-L09-1316-T04-A	1	3.77E+04			3.77E+04	1.9E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
B	EaFA-L09-1316-T05-A	1	6.39E+04			6.39E+04	7.4E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
B	EaFA-L09-1316-T01-B	1	5.14E+03			5.14E+03	1.3E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
B	EaFA-L09-1316-T02-B	1	9.14E+03			9.14E+03	7.5E-01	1.00E+00	3.18E+00	1000	100	9.99E+03	85%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
B	EaFA-L09-1316-T03-B	1	2.18E+04			2.18E+04	9.4E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
B	EaFA-L09-1316-T04-B	1	3.67E+04			3.67E+04	2.5E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
B	EaFA-L09-1316-T05-B	1	3.20E+04			3.20E+04	6.8E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
B	EaFA-L09-1316-T01-C	1	4.84E+03			4.84E+03	6.2E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
B	EaFA-L09-1316-T02-C	1	8.90E+03			8.90E+03	2.0E-01	1.00E+00	3.18E+00	1000	100	9.74E+03	84%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
B	EaFA-L09-1316-T03-C	1	2.14E+04			2.14E+04	1.2E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
B	EaFA-L09-1316-T04-C	1	3.74E+04			3.74E+04	6.1E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
B	EaFA-L09-1316-T05-C	1	4.83E+04			4.83E+04	3.0E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
B	EaFA-L09-1316-B01-A	1	4.64E+01			4.64E+01	3.6E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	EaFA-L09-1316-T01-A	1	2.57E+02			2.57E+02	1.0E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
Ba	EaFA-L09-1316-T02-A	1	2.14E+02			2.14E+02	2.7E-01	1.00E+00	3.18E+00	10	325	3.16E+03	91%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
Ba	EaFA-L09-1316-T03-A	1	2.04E+02			2.04E+02	1.0E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
Ba	EaFA-L09-1316-T04-A	1	2.24E+02			2.24E+02	1.1E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
Ba	EaFA-L09-1316-T05-A	1	2.30E+02			2.30E+02	9.4E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
Ba	EaFA-L09-1316-T01-B	1	2.65E+02			2.65E+02	4.6E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
Ba	EaFA-L09-1316-T02-B	1	2.06E+02			2.06E+02	8.7E-01	1.00E+00	3.18E+00	10	325	3.28E+03	94%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
Ba	EaFA-L09-1316-T03-B	1	2.08E+02			2.08E+02	4.4E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
Ba	EaFA-L09-1316-T04-B	1	2.20E+02			2.20E+02	2.6E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
Ba	EaFA-L09-1316-T05-B	1	1.88E+02			1.88E+02	8.2E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
Ba	EaFA-L09-1316-T01-C	1	2.63E+02			2.63E+02	7.9E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
Ba	EaFA-L09-1316-T02-C	1	2.05E+02			2.05E+02	7.7E-02	1.00E+00	3.18E+00	10	325	3.27E+03	94%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
Ba	EaFA-L09-1316-T03-C	1	2.07E+02			2.07E+02	4.4E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
Ba	EaFA-L09-1316-T04-C	1	2.29E+02			2.29E+02	2.4E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
Ba	EaFA-L09-1316-T05-C	1	1.87E+02			1.87E+02	5.2E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
Ba	EaFA-L09-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	2.8E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	EaFA-L09-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	9.4E+03	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
Be	EaFA-L09-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	8.4E+01	1.90E+00	6.00E+00	10	325	3.36E+03	103%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
Be	EaFA-L09-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	4.5E+02	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
Be	EaFA-L09-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	7.6E+01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
Be	EaFA-L09-1316-T05-A	1	9.50E-01	U1/2		9.50E-01	5.2E+02	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
Be	EaFA-L09-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	6.0E+03	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
Be	EaFA-L09-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	2.2E+02	1.90E+00	6.00E+00	10	325	3.53E+03	109%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
Be	EaFA-L09-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	2.6E+02	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
Be	EaFA-L09-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	5.4E+02	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
Be	EaFA-L09-1316-T05-B	1	9.50E-01	U1/2		9.50E-01	2.2E+01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
Be	EaFA-L09-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	4.8E+02	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
Be	EaFA-L09-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	7.5E+01	1.90E+00	6.00E+00	10	325	3.51E+03	108%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
Be	EaFA-L09-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	3.6E+02	1.90E+00	6.00E+00					VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
Be	EaFA-L09-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	5.2E+01	1.90E+00	6.00E+00					VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
Be	EaFA-L09-1316-T05-C	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.90E+00	6.00E+00					VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
Be	EaFA-L09-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	2.3E+01	1.90E+00	6.00E+00					VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	EaFA-L09-1316-T01-A	1	1.10E+00	U1/2		1.10E+00	1.3E+01	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
Cd	EaFA-L09-1316-T02-A	1	1.10E+00	U1/2		1.10E+00	1.2E+01	2.20E+00	7.00E+00	10	325	3.34E+03	103%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
Cd	EaFA-L09-1316-T03-A	1	1.10E+00	U1/2		1.10E+00	1.9E+01	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
Cd	EaFA-L09-1316-T04-A	1	1.10E+00	U1/2		1.10E+00	1.3E+01	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
Cd	EaFA-L09-1316-T05-A	1	1.10E+00	U1/2		1.10E+00	4.8E+01	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
Cd	EaFA-L09-1316-T01-B	1	1.10E+00	U1/2		1.10E+00	1.1E+01	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
Cd	EaFA-L09-1316-T02-B	1	1.10E+00	U1/2		1.10E+00	8.9E+00	2.20E+00	7.00E+00	10	325	3.51E+03	108%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
Cd	EaFA-L09-1316-T03-B	1	1.10E+00	U1/2		1.10E+00	4.6E+01	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
Cd	EaFA-L09-1316-T04-B	1	1.10E+00	U1/2		1.10E+00	2.2E+01	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
Cd	EaFA-L09-1316-T05-B	1	1.10E+00	U1/2		1.10E+00	7.9E-01	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
Cd	EaFA-L09-1316-T01-C	1	1.10E+00	U1/2		1.10E+00	1.6E+01	2.20E+00	7.00E+00				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
Cd	EaFA-L09-1316-T02-C	1	1.10E+00	U1/2		1.10E+00	7.1E+00	2.20E+00	7.00E+00	10	325	3.51E+03	108%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
Cd	EaFA-L09-1316-T03-C	1	1.10E+00	U1/2		1.10E+00	8.6E+01	2.20E+00	7.00E+00					VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
Cd	EaFA-L09-1316-T04-C	1	1.10E+00	U1/2		1.10E+00	1.8E+01	2.20E+00	7.00E+00					VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
Cd	EaFA-L09-1316-T05-C	1	1.10E+00	U1/2		1.10E+00	6.6E+01	2.20E+00	7.00E+00					VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
Cd	EaFA-L09-1316-B01-A	1	1.10E+00	U1/2		1.10E+00	9.1E+00	2.20E+00	7.00E+00					VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	EaFA-L09-1316-T01-A	1	1.60E+05			1.60E+05	7.3E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
Ca	EaFA-L09-1316-T02-A	1	3.24E+05			3.24E+05	4.2E-01	2.60E+00	8.30E+00	1000	100	3.25E+05	89%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
Ca	EaFA-L09-1316-T03-A	1	7.66E+05			7.66E+05	1.4E+00	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
Ca	EaFA-L09-1316-T04-A	1	5.90E+05			5.90E+05	1.4E+00	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
Ca	EaFA-L09-1316-T05-A	1	4.51E+05			4.51E+05	8.6E+00	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
Ca	EaFA-L09-1316-T01-B	1	1.64E+05			1.64E+05	4.3E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
Ca	EaFA-L09-1316-T02-B	1	3.27E+05			3.27E+05	8.0E-01	2.60E+00	8.30E+00	1000	100	3.27E+05	82%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
Ca	EaFA-L09-1316-T03-B	1	7.74E+05			7.74E+05	4.6E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
Ca	EaFA-L09-1316-T04-B	1	5.74E+05			5.74E+05	2.7E+00	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
Ca	EaFA-L09-1316-T05-B	1	2.84E+05			2.84E+05	8.1E+01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
Ca	EaFA-L09-1316-T01-C	1	1.59E+05			1.59E+05	5.0E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
Ca	EaFA-L09-1316-T02-C	1	3.23E+05			3.23E+05	4.5E-01	2.60E+00	8.30E+00	1000	100	3.24E+05	89%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
Ca	EaFA-L09-1316-T03-C	1	7.76E+05			7.76E+05	6.8E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
Ca	EaFA-L09-1316-T04-C	1	5.97E+05			5.97E+05	3.9E-01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
Ca	EaFA-L09-1316-T05-C	1	3.52E+05			3.52E+05	4.4E+01	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
Ca	EaFA-L09-1316-B01-A	1	1.30E+00	U1/2		1.30E+00	3.8E+02	2.60E+00	8.30E+00				---	VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	EaFA-L09-1316-T01-A	1	1.70E+01			1.70E+01	2.2E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
Cr	EaFA-L09-1316-T02-A	1	2.24E+01			2.24E+01	3.5E+00	1.20E+00	3.82E+00	10	325	3.26E+03	100%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
Cr	EaFA-L09-1316-T03-A	1	2.62E+01			2.62E+01	1.1E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
Cr	EaFA-L09-1316-T04-A	1	4.89E+01			4.89E+01	3.4E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
Cr	EaFA-L09-1316-T05-A	1	2.16E+01			2.16E+01	1.1E+01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
Cr	EaFA-L09-1316-T01-B	1	1.52E+01			1.52E+01	1.3E+01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
Cr	EaFA-L09-1316-T02-B	1	2.30E+01			2.30E+01	4.5E+00	1.20E+00	3.82E+00	10	325	3.37E+03	103%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
Cr	EaFA-L09-1316-T03-B	1	2.63E+01			2.63E+01	1.4E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
Cr	EaFA-L09-1316-T04-B	1	4.96E+01			4.96E+01	8.4E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
Cr	EaFA-L09-1316-T05-B	1	4.30E+01			4.30E+01	8.5E+01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
Cr	EaFA-L09-1316-T01-C	1	1.51E+01			1.51E+01	6.7E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
Cr	EaFA-L09-1316-T02-C	1	2.41E+01			2.41E+01	6.3E+00	1.20E+00	3.82E+00	10	325	3.38E+03	103%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
Cr	EaFA-L09-1316-T03-C	1	2.55E+01			2.55E+01	7.1E+00	1.20E+00	3.82E+00					VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
Cr	EaFA-L09-1316-T04-C	1	4.88E+01			4.88E+01	2.3E+00	1.20E+00	3.82E+00					VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
Cr	EaFA-L09-1316-T05-C	1	3.09E+01			3.09E+01	5.1E+01	1.20E+00	3.82E+00					VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
Cr	EaFA-L09-1316-B01-A	1	1.23E+00	E		1.23E+00	1.7E+02	1.20E+00	3.82E+00					VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	EaFA-L09-1316-T01-A	1	4.36E+01			4.36E+01	6.0E+00	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
Co	EaFA-L09-1316-T02-A	1	7.93E+01			7.93E+01	3.9E+00	1.80E+00	5.72E+00	10	325	3.30E+03	99%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
Co	EaFA-L09-1316-T03-A	1	2.11E+02			2.11E+02	1.6E+00	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
Co	EaFA-L09-1316-T04-A	1	1.27E+02			1.27E+02	3.1E+00	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
Co	EaFA-L09-1316-T05-A	1	4.10E+02			4.10E+02	7.7E+00	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
Co	EaFA-L09-1316-T01-B	1	4.99E+01			4.99E+01	2.1E+00	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
Co	EaFA-L09-1316-T02-B	1	9.19E+01			9.19E+01	3.4E+00	1.80E+00	5.72E+00	10	325	3.43E+03	103%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
Co	EaFA-L09-1316-T03-B	1	2.15E+02			2.15E+02	9.0E-01	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
Co	EaFA-L09-1316-T04-B	1	1.23E+02			1.23E+02	3.1E+00	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
Co	EaFA-L09-1316-T05-B	1	4.91E+01			4.91E+01	8.0E+01	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
Co	EaFA-L09-1316-T01-C	1	4.59E+01			4.59E+01	1.8E+00	1.80E+00	5.72E+00				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
Co	EaFA-L09-1316-T02-C	1	8.47E+01			8.47E+01	1.9E+00	1.80E+00	5.72E+00	10	325	3.43E+03	103%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
Co	EaFA-L09-1316-T03-C	1	2.19E+02			2.19E+02	1.2E+00	1.80E+00	5.72E+00					VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
Co	EaFA-L09-1316-T04-C	1	1.36E+02			1.36E+02	2.2E+00	1.80E+00	5.72E+00					VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
Co	EaFA-L09-1316-T05-C	1	3.14E+02			3.14E+02	4.8E+01	1.80E+00	5.72E+00					VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
Co	EaFA-L09-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	1.7E+02	1.80E+00	5.72E+00					VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	EaFA-L09-1316-T01-A	1	1.01E+01	E		1.01E+01	4.4E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
Cu	EaFA-L09-1316-T02-A	1	1.37E+01			1.37E+01	2.9E+01	3.70E+00	1.18E+01	10	325	3.29E+03	101%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
Cu	EaFA-L09-1316-T03-A	1	1.65E+01			1.65E+01	3.1E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
Cu	EaFA-L09-1316-T04-A	1	1.52E+01			1.52E+01	1.5E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
Cu	EaFA-L09-1316-T05-A	1	1.93E+01			1.93E+01	5.2E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
Cu	EaFA-L09-1316-T01-B	1	1.02E+01	E		1.02E+01	4.4E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
Cu	EaFA-L09-1316-T02-B	1	1.33E+01			1.33E+01	5.4E+01	3.70E+00	1.18E+01	10	325	3.38E+03	104%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
Cu	EaFA-L09-1316-T03-B	1	1.40E+01			1.40E+01	6.6E+00	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
Cu	EaFA-L09-1316-T04-B	1	1.37E+01			1.37E+01	1.1E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
Cu	EaFA-L09-1316-T05-B	1	1.34E+01			1.34E+01	9.7E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
Cu	EaFA-L09-1316-T01-C	1	8.47E+00	E		8.47E+00	2.7E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
Cu	EaFA-L09-1316-T02-C	1	7.14E+00	E		7.14E+00	6.4E+01	3.70E+00	1.18E+01	10	325	3.40E+03	104%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
Cu	EaFA-L09-1316-T03-C	1	1.76E+01			1.76E+01	3.1E+01	3.70E+00	1.18E+01					VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
Cu	EaFA-L09-1316-T04-C	1	1.48E+01			1.48E+01	2.4E+01	3.70E+00	1.18E+01					VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
Cu	EaFA-L09-1316-T05-C	1	2.17E+01			2.17E+01	4.9E+01	3.70E+00	1.18E+01					VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
Cu	EaFA-L09-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	2.3E+02	3.70E+00	1.18E+01					VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	EaFA-L09-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	2.0E+02	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
Fe	EaFA-L09-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.00E+00	6.40E+00	1000	100	1.03E+03	103%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
Fe	EaFA-L09-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	1.8E+02	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
Fe	EaFA-L09-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	3.1E+02	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
Fe	EaFA-L09-1316-T05-A	1	2.97E+00	E		2.97E+00	1.9E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
Fe	EaFA-L09-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
Fe	EaFA-L09-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.00E+00	6.40E+00	1000	100	1.06E+03	106%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
Fe	EaFA-L09-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	8.0E+02	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
Fe	EaFA-L09-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	1.5E+02	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
Fe	EaFA-L09-1316-T05-B	1	1.00E+00	U1/2		1.00E+00	2.1E+02	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
Fe	EaFA-L09-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
Fe	EaFA-L09-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	2.0E+02	2.00E+00	6.40E+00	1000	100	1.06E+03	106%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
Fe	EaFA-L09-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	5.8E+02	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
Fe	EaFA-L09-1316-T04-C	1	2.45E+00	E		2.45E+00	1.4E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
Fe	EaFA-L09-1316-T05-C	1	2.40E+00	E		2.40E+00	1.0E+02	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
Fe	EaFA-L09-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	1.9E+02	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	EaFA-L09-1316-T01-A	1	3.40E+00	U1/2		3.40E+00	2.4E+02	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
Pb	EaFA-L09-1316-T02-A	1	3.40E+00	U1/2		3.40E+00	8.2E+01	6.80E+00	2.16E+01	10	325	3.20E+03	98%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
Pb	EaFA-L09-1316-T03-A	1	3.40E+00	U1/2		3.40E+00	7.6E+02	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
Pb	EaFA-L09-1316-T04-A	1	3.40E+00	U1/2		3.40E+00	8.4E+01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
Pb	EaFA-L09-1316-T05-A	1	3.40E+00	U1/2		3.40E+00	5.0E+01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
Pb	EaFA-L09-1316-T01-B	1	3.40E+00	U1/2		3.40E+00	3.6E+01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
Pb	EaFA-L09-1316-T02-B	1	3.40E+00	U1/2		3.40E+00	1.2E+02	6.80E+00	2.16E+01	10	325	3.33E+03	102%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
Pb	EaFA-L09-1316-T03-B	1	3.40E+00	U1/2		3.40E+00	8.0E+01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
Pb	EaFA-L09-1316-T04-B	1	3.40E+00	U1/2		3.40E+00	2.0E+01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
Pb	EaFA-L09-1316-T05-B	1	3.40E+00	U1/2		3.40E+00	1.3E+02	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
Pb	EaFA-L09-1316-T01-C	1	3.40E+00	U1/2		3.40E+00	2.8E+02	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
Pb	EaFA-L09-1316-T02-C	1	3.40E+00	U1/2		3.40E+00	2.4E+01	6.80E+00	2.16E+01	10	325	3.35E+03	103%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
Pb	EaFA-L09-1316-T03-C	1	3.40E+00	U1/2		3.40E+00	2.5E+03	6.80E+00	2.16E+01					VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
Pb	EaFA-L09-1316-T04-C	1	3.40E+00	U1/2		3.40E+00	2.5E+03	6.80E+00	2.16E+01					VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
Pb	EaFA-L09-1316-T05-C	1	3.40E+00	U1/2		3.40E+00	8.7E+01	6.80E+00	2.16E+01					VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
Pb	EaFA-L09-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	1.3E+02	6.80E+00	2.16E+01					VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	EaFA-L09-1316-T01-A	1	4.05E+03			4.05E+03	8.8E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
Li	EaFA-L09-1316-T02-A	1	7.99E+03			7.99E+03	2.3E-01	1.90E+00	6.00E+00	10	325	1.08E+04	87%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
Li	EaFA-L09-1316-T03-A	1	1.94E+04			1.94E+04	1.1E+00	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
Li	EaFA-L09-1316-T04-A	1	3.80E+04			3.80E+04	1.3E+00	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
Li	EaFA-L09-1316-T05-A	1	7.38E+04			7.38E+04	8.5E+00	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
Li	EaFA-L09-1316-T01-B	1	4.15E+03			4.15E+03	6.8E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
Li	EaFA-L09-1316-T02-B	1	8.09E+03			8.09E+03	5.9E-01	1.90E+00	6.00E+00	10	325	1.11E+04	91%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
Li	EaFA-L09-1316-T03-B	1	1.98E+04			1.98E+04	8.0E-01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
Li	EaFA-L09-1316-T04-B	1	3.74E+04			3.74E+04	2.5E+00	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
Li	EaFA-L09-1316-T05-B	1	3.69E+04			3.69E+04	8.3E+01	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
Li	EaFA-L09-1316-T01-C	1	4.04E+03			4.04E+03	1.1E+00	1.90E+00	6.00E+00				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
Li	EaFA-L09-1316-T02-C	1	8.00E+03			8.00E+03	4.1E-01	1.90E+00	6.00E+00	10	325	1.11E+04	95%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
Li	EaFA-L09-1316-T03-C	1	1.98E+04			1.98E+04	7.6E-01	1.90E+00	6.00E+00					VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
Li	EaFA-L09-1316-T04-C	1	3.90E+04			3.90E+04	2.5E-01	1.90E+00	6.00E+00					VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
Li	EaFA-L09-1316-T05-C	1	5.24E+04			5.24E+04	4.4E+01	1.90E+00	6.00E+00					VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
Li	EaFA-L09-1316-B01-A	1	2.00E+00	E		2.00E+00	1.2E+02	1.90E+00	6.00E+00					VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	EaFA-L09-1316-T01-A	1	3.66E+02			3.66E+02	7.2E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
Mn	EaFA-L09-1316-T02-A	1	6.64E+02			6.64E+02	1.5E-01	2.00E+00	6.40E+00	10	325	4.01E+03	103%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
Mn	EaFA-L09-1316-T03-A	1	1.63E+03			1.63E+03	9.7E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
Mn	EaFA-L09-1316-T04-A	1	1.32E+03			1.32E+03	1.2E+00	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
Mn	EaFA-L09-1316-T05-A	1	4.02E+03			4.02E+03	8.7E+00	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
Mn	EaFA-L09-1316-T01-B	1	4.05E+02			4.05E+02	5.3E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
Mn	EaFA-L09-1316-T02-B	1	7.23E+02			7.23E+02	1.6E+00	2.00E+00	6.40E+00	10	325	4.22E+03	108%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
Mn	EaFA-L09-1316-T03-B	1	1.66E+03			1.66E+03	6.8E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
Mn	EaFA-L09-1316-T04-B	1	1.29E+03			1.29E+03	2.4E+00	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
Mn	EaFA-L09-1316-T05-B	1	7.74E+02			7.74E+02	7.6E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
Mn	EaFA-L09-1316-T01-C	1	3.84E+02			3.84E+02	2.1E-01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
Mn	EaFA-L09-1316-T02-C	1	6.82E+02			6.82E+02	6.9E-01	2.00E+00	6.40E+00	10	325	4.18E+03	108%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
Mn	EaFA-L09-1316-T03-C	1	1.70E+03			1.70E+03	8.6E-01	2.00E+00	6.40E+00					VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
Mn	EaFA-L09-1316-T04-C	1	1.44E+03			1.44E+03	7.3E-01	2.00E+00	6.40E+00					VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
Mn	EaFA-L09-1316-T05-C	1	2.64E+03			2.64E+03	4.9E+01	2.00E+00	6.40E+00					VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
Mn	EaFA-L09-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.00E+00	6.40E+00					VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	EaFA-L09-1316-T01-A	1	7.56E+03			7.56E+03	1.4E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
Mg	EaFA-L09-1316-T02-A	1	1.54E+04			1.54E+04	2.7E-01	1.00E+00	3.18E+00	1000	100	1.63E+04	90%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
Mg	EaFA-L09-1316-T03-A	1	3.90E+04			3.90E+04	6.3E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
Mg	EaFA-L09-1316-T04-A	1	7.17E+04			7.17E+04	1.7E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
Mg	EaFA-L09-1316-T05-A	1	1.35E+05			1.35E+05	8.9E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
Mg	EaFA-L09-1316-T01-B	1	7.77E+03			7.77E+03	8.4E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
Mg	EaFA-L09-1316-T02-B	1	1.55E+04			1.55E+04	7.6E-01	1.00E+00	3.18E+00	1000	100	1.63E+04	85%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
Mg	EaFA-L09-1316-T03-B	1	3.98E+04			3.98E+04	2.7E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
Mg	EaFA-L09-1316-T04-B	1	7.07E+04			7.07E+04	3.0E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
Mg	EaFA-L09-1316-T05-B	1	6.32E+04			6.32E+04	8.0E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
Mg	EaFA-L09-1316-T01-C	1	7.55E+03			7.55E+03	1.3E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
Mg	EaFA-L09-1316-T02-C	1	1.52E+04			1.52E+04	7.8E-01	1.00E+00	3.18E+00	1000	100	1.61E+04	87%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
Mg	EaFA-L09-1316-T03-C	1	3.98E+04			3.98E+04	4.3E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
Mg	EaFA-L09-1316-T04-C	1	7.49E+04			7.49E+04	3.7E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
Mg	EaFA-L09-1316-T05-C	1	9.15E+04			9.15E+04	5.1E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
Mg	EaFA-L09-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	4.1E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	EaFA-L09-1316-T01-A	1	3.64E+03			3.64E+03	2.0E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
Mo	EaFA-L09-1316-T02-A	1	6.91E+03			6.91E+03	2.4E-01	1.20E+00	3.82E+00	10	325	9.58E+03	82%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
Mo	EaFA-L09-1316-T03-A	1	1.48E+04			1.48E+04	1.2E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
Mo	EaFA-L09-1316-T04-A	1	2.97E+04			2.97E+04	1.3E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
Mo	EaFA-L09-1316-T05-A	1	3.14E+04			3.14E+04	9.1E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
Mo	EaFA-L09-1316-T01-B	1	3.69E+03			3.69E+03	1.3E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
Mo	EaFA-L09-1316-T02-B	1	6.85E+03			6.85E+03	9.5E-01	1.20E+00	3.82E+00	10	325	9.89E+03	94%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
Mo	EaFA-L09-1316-T03-B	1	1.51E+04			1.51E+04	3.9E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
Mo	EaFA-L09-1316-T04-B	1	2.87E+04			2.87E+04	2.3E+00	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
Mo	EaFA-L09-1316-T05-B	1	2.73E+04			2.73E+04	7.6E+01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
Mo	EaFA-L09-1316-T01-C	1	3.63E+03			3.63E+03	8.2E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
Mo	EaFA-L09-1316-T02-C	1	6.83E+03			6.83E+03	5.3E-01	1.20E+00	3.82E+00	10	325	9.91E+03	95%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
Mo	EaFA-L09-1316-T03-C	1	1.49E+04			1.49E+04	9.7E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
Mo	EaFA-L09-1316-T04-C	1	2.88E+04			2.88E+04	2.3E-01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
Mo	EaFA-L09-1316-T05-C	1	2.45E+04			2.45E+04	4.6E+01	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
Mo	EaFA-L09-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	1.1E+03	1.20E+00	3.82E+00				---	VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	EaFA-L09-1316-T01-A	1	1.01E+02			1.01E+02	4.7E+00	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
Ni	EaFA-L09-1316-T02-A	1	1.82E+02			1.82E+02	1.2E+00	1.80E+00	5.70E+00	10	325	3.44E+03	100%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
Ni	EaFA-L09-1316-T03-A	1	4.76E+02			4.76E+02	6.6E-01	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
Ni	EaFA-L09-1316-T04-A	1	2.95E+02			2.95E+02	2.2E+00	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
Ni	EaFA-L09-1316-T05-A	1	8.56E+02			8.56E+02	8.3E+00	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
Ni	EaFA-L09-1316-T01-B	1	1.16E+02			1.16E+02	2.9E+00	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
Ni	EaFA-L09-1316-T02-B	1	2.12E+02			2.12E+02	3.9E-01	1.80E+00	5.70E+00	10	325	3.60E+03	104%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
Ni	EaFA-L09-1316-T03-B	1	4.85E+02			4.85E+02	6.6E-01	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
Ni	EaFA-L09-1316-T04-B	1	2.79E+02			2.79E+02	8.4E-01	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
Ni	EaFA-L09-1316-T05-B	1	1.22E+02			1.22E+02	8.6E+01	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
Ni	EaFA-L09-1316-T01-C	1	1.11E+02			1.11E+02	3.9E+00	1.80E+00	5.70E+00				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
Ni	EaFA-L09-1316-T02-C	1	1.97E+02			1.97E+02	1.8E+00	1.80E+00	5.70E+00	10	325	3.58E+03	104%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
Ni	EaFA-L09-1316-T03-C	1	4.94E+02			4.94E+02	7.3E-01	1.80E+00	5.70E+00					VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
Ni	EaFA-L09-1316-T04-C	1	3.14E+02			3.14E+02	1.1E+00	1.80E+00	5.70E+00					VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
Ni	EaFA-L09-1316-T05-C	1	6.68E+02			6.68E+02	4.9E+01	1.80E+00	5.70E+00					VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
Ni	EaFA-L09-1316-B01-A	1	3.71E+00	E		3.71E+00	6.8E+01	1.80E+00	5.70E+00					VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	EaFA-L09-1316-T01-A	1	2.47E+01			2.47E+01	8.3E+00	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
P	EaFA-L09-1316-T02-A	1	5.27E+01			5.27E+01	1.4E+01	3.70E+00	1.18E+01	1000	100	1.08E+03	102%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
P	EaFA-L09-1316-T03-A	1	8.21E+01			8.21E+01	3.1E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
P	EaFA-L09-1316-T04-A	1	4.40E+02			4.40E+02	7.2E+00	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
P	EaFA-L09-1316-T05-A	1	1.47E+02			1.47E+02	3.5E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
P	EaFA-L09-1316-T01-B	1	5.20E+01			5.20E+01	1.5E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
P	EaFA-L09-1316-T02-B	1	5.07E+01			5.07E+01	7.5E+00	3.70E+00	1.18E+01	1000	100	1.16E+03	111%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
P	EaFA-L09-1316-T03-B	1	2.21E+02			2.21E+02	7.5E+00	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
P	EaFA-L09-1316-T04-B	1	2.68E+02			2.68E+02	8.6E+00	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
P	EaFA-L09-1316-T05-B	1	1.40E+02			1.40E+02	1.4E+02	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
P	EaFA-L09-1316-T01-C	1	5.85E+01			5.85E+01	2.4E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
P	EaFA-L09-1316-T02-C	1	6.98E+01			6.98E+01	1.6E+01	3.70E+00	1.18E+01	1000	100	1.16E+03	109%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
P	EaFA-L09-1316-T03-C	1	2.32E+02			2.32E+02	1.3E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
P	EaFA-L09-1316-T04-C	1	4.79E+02			4.79E+02	3.8E+00	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
P	EaFA-L09-1316-T05-C	1	1.08E+02			1.08E+02	2.2E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
P	EaFA-L09-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	1.0E+01	3.70E+00	1.18E+01				---	VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	EaFA-L09-1316-T01-A	1	2.47E+01			2.47E+01	6.5E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
K	EaFA-L09-1316-T02-A	1	5.27E+01			5.27E+01	8.3E-01	1.60E+00	5.09E+00	1000	100	9.28E+02	88%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
K	EaFA-L09-1316-T03-A	1	8.21E+01			8.21E+01	7.1E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
K	EaFA-L09-1316-T04-A	1	4.40E+02			4.40E+02	8.0E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
K	EaFA-L09-1316-T05-A	1	1.47E+02			1.47E+02	8.9E+00	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
K	EaFA-L09-1316-T01-B	1	5.20E+01			5.20E+01	3.7E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
K	EaFA-L09-1316-T02-B	1	5.07E+01			5.07E+01	7.9E-01	1.60E+00	5.09E+00	1000	100	9.91E+02	94%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
K	EaFA-L09-1316-T03-B	1	2.21E+02			2.21E+02	3.8E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
K	EaFA-L09-1316-T04-B	1	2.68E+02			2.68E+02	2.1E+00	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
K	EaFA-L09-1316-T05-B	1	1.40E+02			1.40E+02	8.3E+01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
K	EaFA-L09-1316-T01-C	1	5.85E+01			5.85E+01	8.6E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
K	EaFA-L09-1316-T02-C	1	6.98E+01			6.98E+01	4.1E-01	1.60E+00	5.09E+00	1000	100	1.02E+03	95%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
K	EaFA-L09-1316-T03-C	1	2.32E+02			2.32E+02	3.5E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
K	EaFA-L09-1316-T04-C	1	4.79E+02			4.79E+02	9.2E-01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
K	EaFA-L09-1316-T05-C	1	1.08E+02			1.08E+02	5.3E+01	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
K	EaFA-L09-1316-B01-A	1	7.73E+01			7.73E+01	3.0E+00	1.60E+00	5.09E+00				---	VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	EaFA-L09-1316-T01-A	1	1.24E+03			1.24E+03	1.5E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
Se	EaFA-L09-1316-T02-A	1	1.44E+03			1.44E+03	7.2E-01	1.50E+01	4.77E+01	10	325	4.57E+03	96%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
Se	EaFA-L09-1316-T03-A	1	1.52E+03			1.52E+03	1.2E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
Se	EaFA-L09-1316-T04-A	1	2.21E+03			2.21E+03	1.3E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
Se	EaFA-L09-1316-T05-A	1	1.87E+03			1.87E+03	7.9E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
Se	EaFA-L09-1316-T01-B	1	1.27E+03			1.27E+03	2.5E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
Se	EaFA-L09-1316-T02-B	1	1.45E+03			1.45E+03	1.8E+00	1.50E+01	4.77E+01	10	325	4.72E+03	101%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
Se	EaFA-L09-1316-T03-B	1	1.58E+03			1.58E+03	2.3E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
Se	EaFA-L09-1316-T04-B	1	2.17E+03			2.17E+03	4.5E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
Se	EaFA-L09-1316-T05-B	1	2.19E+03			2.19E+03	8.0E+01	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
Se	EaFA-L09-1316-T01-C	1	1.17E+03			1.17E+03	1.6E+00	1.50E+01	4.77E+01				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
Se	EaFA-L09-1316-T02-C	1	1.45E+03			1.45E+03	1.4E+00	1.50E+01	4.77E+01	10	325	4.75E+03	102%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
Se	EaFA-L09-1316-T03-C	1	1.53E+03			1.53E+03	4.1E+00	1.50E+01	4.77E+01					VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
Se	EaFA-L09-1316-T04-C	1	2.00E+03			2.00E+03	1.2E+00	1.50E+01	4.77E+01					VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
Se	EaFA-L09-1316-T05-C	1	1.81E+03			1.81E+03	4.6E+01	1.50E+01	4.77E+01					VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
Se	EaFA-L09-1316-B01-A	1	8.30E+01			8.30E+01	3.4E+01	1.50E+01	4.77E+01					VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	EaFA-L09-1316-T01-A	1	2.21E+03			2.21E+03	1.1E+00	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
Si	EaFA-L09-1316-T02-A	1	2.30E+03			2.30E+03	1.7E-01	1.10E+00	3.50E+00	1000	100	3.16E+03	86%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
Si	EaFA-L09-1316-T03-A	1	2.64E+03			2.64E+03	1.8E+00	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
Si	EaFA-L09-1316-T04-A	1	2.12E+03			2.12E+03	5.5E-01	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
Si	EaFA-L09-1316-T05-A	1	2.80E+03			2.80E+03	1.0E+01	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
Si	EaFA-L09-1316-T01-B	1	2.36E+03			2.36E+03	9.7E-01	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
Si	EaFA-L09-1316-T02-B	1	2.47E+03			2.47E+03	2.1E+00	1.10E+00	3.50E+00	1000	100	3.34E+03	87%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
Si	EaFA-L09-1316-T03-B	1	2.71E+03			2.71E+03	8.3E-01	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
Si	EaFA-L09-1316-T04-B	1	2.08E+03			2.08E+03	2.3E+00	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
Si	EaFA-L09-1316-T05-B	1	1.08E+03			1.08E+03	8.5E+01	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
Si	EaFA-L09-1316-T01-C	1	2.26E+03			2.26E+03	9.2E-01	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
Si	EaFA-L09-1316-T02-C	1	2.38E+03			2.38E+03	6.8E-01	1.10E+00	3.50E+00	1000	100	3.28E+03	90%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
Si	EaFA-L09-1316-T03-C	1	2.72E+03			2.72E+03	8.6E-01	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
Si	EaFA-L09-1316-T04-C	1	2.12E+03			2.12E+03	4.4E-01	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
Si	EaFA-L09-1316-T05-C	1	2.02E+03			2.02E+03	5.9E+01	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
Si	EaFA-L09-1316-B01-A	1	5.50E-01	U1/2		5.50E-01	1.6E+02	1.10E+00	3.50E+00				---	VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	EaFA-L09-1316-T01-A	1	5.45E+03			5.45E+03	1.0E+00	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
Na	EaFA-L09-1316-T02-A	1	1.13E+04			1.13E+04	4.5E-01	2.50E+00	8.00E+00	1000	100	1.22E+04	86%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
Na	EaFA-L09-1316-T03-A	1	2.87E+04			2.87E+04	8.5E-01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
Na	EaFA-L09-1316-T04-A	1	4.73E+04			4.73E+04	1.5E+00	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
Na	EaFA-L09-1316-T05-A	1	8.84E+04			8.84E+04	8.6E+00	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
Na	EaFA-L09-1316-T01-B	1	5.54E+03			5.54E+03	3.7E-01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
Na	EaFA-L09-1316-T02-B	1	1.14E+04			1.14E+04	3.0E-01	2.50E+00	8.00E+00	1000	100	1.23E+04	92%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
Na	EaFA-L09-1316-T03-B	1	2.91E+04			2.91E+04	5.1E-01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
Na	EaFA-L09-1316-T04-B	1	4.67E+04			4.67E+04	2.3E+00	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
Na	EaFA-L09-1316-T05-B	1	4.81E+04			4.81E+04	8.4E+01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
Na	EaFA-L09-1316-T01-C	1	5.42E+03			5.42E+03	7.0E-01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
Na	EaFA-L09-1316-T02-C	1	1.13E+04			1.13E+04	6.7E-01	2.50E+00	8.00E+00	1000	100	1.24E+04	109%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
Na	EaFA-L09-1316-T03-C	1	2.94E+04			2.94E+04	6.8E-01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
Na	EaFA-L09-1316-T04-C	1	4.93E+04			4.93E+04	5.0E-01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
Na	EaFA-L09-1316-T05-C	1	6.15E+04			6.15E+04	5.2E+01	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
Na	EaFA-L09-1316-B01-A	1	2.46E+01			2.46E+01	1.1E+00	2.50E+00	8.00E+00				---	VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	EaFA-L09-1316-T01-A	1	2.18E+03			2.18E+03	6.1E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
Sr	EaFA-L09-1316-T02-A	1	3.98E+03			3.98E+03	5.8E-01	1.00E+00	3.18E+00	1000	100	4.86E+03	87%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
Sr	EaFA-L09-1316-T03-A	1	8.52E+03			8.52E+03	9.2E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
Sr	EaFA-L09-1316-T04-A	1	7.93E+03			7.93E+03	8.1E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
Sr	EaFA-L09-1316-T05-A	1	7.93E+03			7.93E+03	7.6E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
Sr	EaFA-L09-1316-T01-B	1	2.23E+03			2.23E+03	5.3E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
Sr	EaFA-L09-1316-T02-B	1	4.08E+03			4.08E+03	1.2E+00	1.00E+00	3.18E+00	1000	100	4.97E+03	89%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
Sr	EaFA-L09-1316-T03-B	1	8.69E+03			8.69E+03	5.5E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
Sr	EaFA-L09-1316-T04-B	1	7.94E+03			7.94E+03	2.3E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
Sr	EaFA-L09-1316-T05-B	1	4.36E+03			4.36E+03	7.6E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
Sr	EaFA-L09-1316-T01-C	1	2.17E+03			2.17E+03	5.5E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
Sr	EaFA-L09-1316-T02-C	1	3.97E+03			3.97E+03	7.9E-01	1.00E+00	3.18E+00	1000	100	4.79E+03	82%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
Sr	EaFA-L09-1316-T03-C	1	8.65E+03			8.65E+03	1.0E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
Sr	EaFA-L09-1316-T04-C	1	8.23E+03			8.23E+03	8.1E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
Sr	EaFA-L09-1316-T05-C	1	6.58E+03			6.58E+03	2.2E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
Sr	EaFA-L09-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	2.7E+02	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	EaFA-L09-1316-T01-A	1	1.59E+05			1.59E+05	6.0E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
S	EaFA-L09-1316-T02-A	1	3.16E+05			3.16E+05	2.0E-01	6.80E+00	2.16E+01	1000	100	3.17E+05	92%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
S	EaFA-L09-1316-T03-A	1	7.35E+05			7.35E+05	8.7E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
S	EaFA-L09-1316-T04-A	1	7.55E+05			7.55E+05	1.2E+00	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
S	EaFA-L09-1316-T05-A	1	9.36E+05			9.36E+05	9.1E+00	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
S	EaFA-L09-1316-T01-B	1	1.62E+05			1.62E+05	6.9E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
S	EaFA-L09-1316-T02-B	1	3.17E+05			3.17E+05	6.8E-01	6.80E+00	2.16E+01	1000	100	3.18E+05	83%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
S	EaFA-L09-1316-T03-B	1	7.53E+05			7.53E+05	3.1E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
S	EaFA-L09-1316-T04-B	1	7.38E+05			7.38E+05	2.3E+00	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
S	EaFA-L09-1316-T05-B	1	5.05E+05			5.05E+05	8.3E+01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
S	EaFA-L09-1316-T01-C	1	1.58E+05			1.58E+05	5.5E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
S	EaFA-L09-1316-T02-C	1	3.15E+05			3.15E+05	5.2E-01	6.80E+00	2.16E+01	1000	100	3.16E+05	87%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
S	EaFA-L09-1316-T03-C	1	7.43E+05			7.43E+05	7.8E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
S	EaFA-L09-1316-T04-C	1	7.56E+05			7.56E+05	4.5E-01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
S	EaFA-L09-1316-T05-C	1	6.56E+05			6.56E+05	5.4E+01	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
S	EaFA-L09-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	1.9E+02	6.80E+00	2.16E+01				---	VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	EaFA-L09-1316-T01-A	1	8.41E+00	E		8.41E+00	1.4E+02	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
Tl	EaFA-L09-1316-T02-A	1	1.11E+01	E		1.11E+01	8.9E+01	4.60E+00	1.46E+01	10	325	3.20E+03	98%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
Tl	EaFA-L09-1316-T03-A	1	1.81E+01			1.81E+01	4.4E+01	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
Tl	EaFA-L09-1316-T04-A	1	2.30E+00	U1/2		2.30E+00	2.6E+02	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
Tl	EaFA-L09-1316-T05-A	1	4.27E+01			4.27E+01	4.6E+01	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
Tl	EaFA-L09-1316-T01-B	1	9.64E+00	E		9.64E+00	2.1E+02	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
Tl	EaFA-L09-1316-T02-B	1	2.08E+01			2.08E+01	2.1E+01	4.60E+00	1.46E+01	10	325	3.34E+03	102%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
Tl	EaFA-L09-1316-T03-B	1	6.71E+00	E		6.71E+00	1.1E+02	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
Tl	EaFA-L09-1316-T04-B	1	2.24E+01			2.24E+01	8.3E+01	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
Tl	EaFA-L09-1316-T05-B	1	2.30E+00	U1/2		2.30E+00	1.4E+03	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
Tl	EaFA-L09-1316-T01-C	1	7.82E+00	E		7.82E+00	8.8E+01	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
Tl	EaFA-L09-1316-T02-C	1	1.13E+01	E		1.13E+01	2.6E+01	4.60E+00	1.46E+01	10	325	3.34E+03	102%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
Tl	EaFA-L09-1316-T03-C	1	2.64E+01			2.64E+01	3.0E+01	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
Tl	EaFA-L09-1316-T04-C	1	1.53E+01			1.53E+01	4.6E+01	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
Tl	EaFA-L09-1316-T05-C	1	1.75E+01			1.75E+01	2.6E+02	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
Tl	EaFA-L09-1316-B01-A	1	2.30E+00	U1/2		2.30E+00	1.7E+01	4.60E+00	1.46E+01				---	VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	EaFA-L09-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	3.3E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
Ti	EaFA-L09-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	1.7E+02	2.00E+00	6.40E+00	10	325	3.25E+03	100%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
Ti	EaFA-L09-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	9.7E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
Ti	EaFA-L09-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	5.5E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
Ti	EaFA-L09-1316-T05-A	1	2.44E+00	E		2.44E+00	5.2E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
Ti	EaFA-L09-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
Ti	EaFA-L09-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	7.6E+01	2.00E+00	6.40E+00	10	325	3.40E+03	105%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
Ti	EaFA-L09-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	2.0E+02	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
Ti	EaFA-L09-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	8.2E+02	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
Ti	EaFA-L09-1316-T05-B	1	1.00E+00	U1/2		1.00E+00	6.1E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
Ti	EaFA-L09-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	9.8E+01	2.00E+00	6.40E+00				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
Ti	EaFA-L09-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	4.0E+02	2.00E+00	6.40E+00	10	325	3.39E+03	104%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
Ti	EaFA-L09-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	3.2E+01	2.00E+00	6.40E+00					VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
Ti	EaFA-L09-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	7.6E+01	2.00E+00	6.40E+00					VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
Ti	EaFA-L09-1316-T05-C	1	3.08E+00	E		3.08E+00	3.3E+01	2.00E+00	6.40E+00					VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
Ti	EaFA-L09-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	2.6E+01	2.00E+00	6.40E+00					VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	EaFA-L09-1316-T01-A	1	2.64E+02			2.64E+02	8.6E-01	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
V	EaFA-L09-1316-T02-A	1	3.04E+02			3.04E+02	1.1E+00	1.50E+00	4.77E+00	10	325	3.64E+03	103%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
V	EaFA-L09-1316-T03-A	1	3.40E+02			3.40E+02	1.8E+00	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
V	EaFA-L09-1316-T04-A	1	3.70E+02			3.70E+02	1.9E+00	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
V	EaFA-L09-1316-T05-A	1	3.05E+02			3.05E+02	9.6E+00	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
V	EaFA-L09-1316-T01-B	1	2.62E+02			2.62E+02	5.8E-01	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
V	EaFA-L09-1316-T02-B	1	2.93E+02			2.93E+02	2.4E+00	1.50E+00	4.77E+00	10	325	3.81E+03	108%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
V	EaFA-L09-1316-T03-B	1	3.50E+02			3.50E+02	6.3E-01	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
V	EaFA-L09-1316-T04-B	1	3.54E+02			3.54E+02	2.9E+00	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
V	EaFA-L09-1316-T05-B	1	2.54E+02			2.54E+02	7.3E+01	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
V	EaFA-L09-1316-T01-C	1	2.61E+02			2.61E+02	3.6E+00	1.50E+00	4.77E+00				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
V	EaFA-L09-1316-T02-C	1	2.92E+02			2.92E+02	1.1E+00	1.50E+00	4.77E+00	10	325	3.80E+03	108%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
V	EaFA-L09-1316-T03-C	1	3.41E+02			3.41E+02	3.3E-01	1.50E+00	4.77E+00					VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
V	EaFA-L09-1316-T04-C	1	3.32E+02			3.32E+02	5.5E-01	1.50E+00	4.77E+00					VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
V	EaFA-L09-1316-T05-C	1	2.38E+02			2.38E+02	4.8E+01	1.50E+00	4.77E+00					VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
V	EaFA-L09-1316-B01-A	1	3.08E+00	E		3.08E+00	5.1E+01	1.50E+00	4.77E+00					VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	EaFA-L09-1316-T01-A	1	1.67E+01			1.67E+01	7.8E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:56 AM	L09 1313-1316 EaFA
Zn	EaFA-L09-1316-T02-A	1	2.23E+01			2.23E+01	3.0E+00	1.00E+00	3.18E+00	10	325	3.48E+03	106%	VU ICP-OES	6/11/10 11:57 AM	L09 1313-1316 EaFA
Zn	EaFA-L09-1316-T03-A	1	4.52E+01			4.52E+01	1.5E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 11:59 AM	L09 1313-1316 EaFA
Zn	EaFA-L09-1316-T04-A	1	2.72E+01			2.72E+01	1.5E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:01 PM	L09 1313-1316 EaFA
Zn	EaFA-L09-1316-T05-A	1	1.83E+02			1.83E+02	5.1E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:02 PM	L09 1313-1316 EaFA
Zn	EaFA-L09-1316-T01-B	1	2.04E+01			2.04E+01	1.1E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:04 PM	L09 1313-1316 EaFA
Zn	EaFA-L09-1316-T02-B	1	2.57E+01			2.57E+01	1.1E+00	1.00E+00	3.18E+00	10	325	3.43E+03	105%	VU ICP-OES	6/11/10 12:06 PM	L09 1313-1316 EaFA
Zn	EaFA-L09-1316-T03-B	1	4.52E+01			4.52E+01	3.2E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:07 PM	L09 1313-1316 EaFA
Zn	EaFA-L09-1316-T04-B	1	3.21E+01			3.21E+01	3.0E-01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:09 PM	L09 1313-1316 EaFA
Zn	EaFA-L09-1316-T05-B	1	6.15E+01			6.15E+01	5.4E+00	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:11 PM	L09 1313-1316 EaFA
Zn	EaFA-L09-1316-T01-C	1	1.92E+01			1.92E+01	9.2E+01	1.00E+00	3.18E+00				---	VU ICP-OES	6/11/10 12:12 PM	L09 1313-1316 EaFA
Zn	EaFA-L09-1316-T02-C	1	2.40E+01			2.40E+01	7.6E+00	1.00E+00	3.18E+00	10	325	3.42E+03	105%	VU ICP-OES	6/11/10 12:14 PM	L09 1313-1316 EaFA
Zn	EaFA-L09-1316-T03-C	1	4.79E+01			4.79E+01	3.5E+00	1.00E+00	3.18E+00					VU ICP-OES	6/11/10 12:16 PM	L09 1313-1316 EaFA
Zn	EaFA-L09-1316-T04-C	1	3.71E+01			3.71E+01	2.7E+00	1.00E+00	3.18E+00					VU ICP-OES	6/11/10 12:17 PM	L09 1313-1316 EaFA
Zn	EaFA-L09-1316-T05-C	1	2.31E+02			2.31E+02	2.6E+00	1.00E+00	3.18E+00					VU ICP-OES	6/11/10 12:19 PM	L09 1313-1316 EaFA
Zn	EaFA-L09-1316-B01-A	1	6.89E+00			6.89E+00	5.0E+01	1.00E+00	3.18E+00					VU ICP-OES	6/11/10 11:54 AM	L09 1313-1316 EaFA

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	EaFA-L10-1316-T01-A	1	1.87E+02			1.87E+02	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1316-T02-A	1	2.10E+02			2.10E+02	3.9E+00	1.0E+00	3.2E+00	1000	100	1.04E+03	83%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1316-T03-A	1	8.90E+02			8.90E+02	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1316-T04-A	1	7.47E+02			7.47E+02	4.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1316-T05-A	1	8.08E+02			8.08E+02	6.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1316-T01-B	1	1.61E+02			1.61E+02	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1316-T02-B	1	1.77E+02			1.77E+02	4.4E+00	1.0E+00	3.2E+00	1000	100	9.83E+02	81%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1316-T03-B	1	2.04E+02			2.04E+02	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1316-T04-B	1	4.40E+02			4.40E+02	8.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1316-T05-B	1	7.13E+02			7.13E+02	8.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1316-T01-C	1	1.15E+02			1.15E+02	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1316-T02-C	1	1.74E+02			1.74E+02	5.1E-01	1.0E+00	3.2E+00	1000	100	1.05E+03	87%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1316-T03-C	1	2.76E+02			2.76E+02	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1316-T04-C	1	4.86E+02			4.86E+02	5.0E-01	1.0E+00	3.2E+00					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1316-T05-C	1	7.32E+02			7.32E+02	1.0E+00	1.0E+00	3.2E+00					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
Al	EaFA-L10-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	2.7E+01	1.0E+00	3.2E+00					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	EaFA-L10-1316-T01-A	1	1.66E+02			1.66E+02	6.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1316-T02-A	1	2.65E+02			2.65E+02	7.5E+00	7.5E+00	2.4E+01	10	300	2.97E+03	90%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1316-T03-A	1	2.87E+02			2.87E+02	3.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1316-T04-A	1	3.05E+02			3.05E+02	3.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1316-T05-A	1	4.98E+02			4.98E+02	5.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1316-T01-B	1	1.69E+02			1.69E+02	5.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1316-T02-B	1	2.48E+02			2.48E+02	1.2E+01	7.5E+00	2.4E+01	10	300	2.90E+03	88%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1316-T03-B	1	3.82E+02			3.82E+02	3.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1316-T04-B	1	5.75E+02			5.75E+02	5.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1316-T05-B	1	6.50E+02			6.50E+02	5.8E-01	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1316-T01-C	1	1.73E+02			1.73E+02	1.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1316-T02-C	1	2.68E+02			2.68E+02	1.5E+01	7.5E+00	2.4E+01	10	300	3.12E+03	95%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1316-T03-C	1	4.20E+02			4.20E+02	7.8E+00	7.5E+00	2.4E+01					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1316-T04-C	1	6.22E+02			6.22E+02	3.8E+00	7.5E+00	2.4E+01					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1316-T05-C	1	6.23E+02			6.23E+02	6.7E-01	7.5E+00	2.4E+01					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
Sb	EaFA-L10-1316-B01-A	1	1.86E+01	E		1.86E+01	1.4E+02	7.5E+00	2.4E+01					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	EaFA-L10-1316-T01-A	1	1.13E+02			1.13E+02	3.1E+01	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1316-T02-A	1	1.41E+02			1.41E+02	2.2E+01	1.1E+01	3.5E+01	10	300	2.97E+03	94%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1316-T03-A	1	2.47E+02			2.47E+02	9.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1316-T04-A	1	2.12E+02			2.12E+02	1.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1316-T05-A	1	1.67E+02			1.67E+02	6.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1316-T01-B	1	1.17E+02			1.17E+02	6.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1316-T02-B	1	1.33E+02			1.33E+02	1.7E+01	1.1E+01	3.5E+01	10	300	2.88E+03	92%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1316-T03-B	1	1.37E+02			1.37E+02	2.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1316-T04-B	1	1.99E+02			1.99E+02	5.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1316-T05-B	1	2.29E+02			2.29E+02	7.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1316-T01-C	1	1.02E+02			1.02E+02	7.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1316-T02-C	1	1.08E+02			1.08E+02	3.3E+01	1.1E+01	3.5E+01	10	300	3.10E+03	100%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1316-T03-C	1	1.66E+02			1.66E+02	4.7E+00	1.1E+01	3.5E+01					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1316-T04-C	1	2.09E+02			2.09E+02	2.5E+00	1.1E+01	3.5E+01					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1316-T05-C	1	2.12E+02			2.12E+02	7.9E+00	1.1E+01	3.5E+01					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
As	EaFA-L10-1316-B01-A	1	3.79E+01			3.79E+01	6.7E+01	1.1E+01	3.5E+01					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	EaFA-L10-1316-T01-A	1	4.21E+03			4.21E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1316-T02-A	1	8.03E+03			8.03E+03	2.2E+00	1.0E+00	3.2E+00	1000	100	8.92E+03	90%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1316-T03-A	1	1.68E+04			1.68E+04	3.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1316-T04-A	1	2.82E+04			2.82E+04	3.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1316-T05-A	1	5.19E+04			5.19E+04	7.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1316-T01-B	1	4.85E+03			4.85E+03	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1316-T02-B	1	7.92E+03			7.92E+03	2.5E+00	1.0E+00	3.2E+00	1000	100	8.76E+03	84%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1316-T03-B	1	2.01E+04			2.01E+04	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1316-T04-B	1	3.25E+04			3.25E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1316-T05-B	1	5.26E+04			5.26E+04	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1316-T01-C	1	5.49E+03			5.49E+03	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1316-T02-C	1	8.45E+03			8.45E+03	1.9E+00	1.0E+00	3.2E+00	1000	100	9.34E+03	88%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1316-T03-C	1	1.89E+04			1.89E+04	2.1E+00	1.0E+00	3.2E+00					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1316-T04-C	1	3.64E+04			3.64E+04	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1316-T05-C	1	5.39E+04			5.39E+04	6.0E-01	1.0E+00	3.2E+00					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
B	EaFA-L10-1316-B01-A	1	1.36E+02			1.36E+02	1.7E+00	1.0E+00	3.2E+00					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	EaFA-L10-1316-T01-A	1	2.80E+02			2.80E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1316-T02-A	1	2.25E+02			2.25E+02	5.9E-01	1.0E+00	3.2E+00	10	300	2.70E+03	83%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1316-T03-A	1	2.92E+02			2.92E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1316-T04-A	1	2.76E+02			2.76E+02	3.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1316-T05-A	1	2.47E+02			2.47E+02	7.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1316-T01-B	1	3.04E+02			3.04E+02	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1316-T02-B	1	2.31E+02			2.31E+02	2.3E+00	1.0E+00	3.2E+00	10	300	2.63E+03	80%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1316-T03-B	1	2.18E+02			2.18E+02	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1316-T04-B	1	2.41E+02			2.41E+02	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1316-T05-B	1	2.64E+02			2.64E+02	1.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1316-T01-C	1	2.78E+02			2.78E+02	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1316-T02-C	1	2.31E+02			2.31E+02	1.5E+00	1.0E+00	3.2E+00	10	300	2.79E+03	85%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1316-T03-C	1	2.03E+02			2.03E+02	2.8E+00	1.0E+00	3.2E+00					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1316-T04-C	1	2.77E+02			2.77E+02	1.5E+00	1.0E+00	3.2E+00					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1316-T05-C	1	2.69E+02			2.69E+02	5.3E-01	1.0E+00	3.2E+00					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
Ba	EaFA-L10-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	3.2E+01	1.0E+00	3.2E+00					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	EaFA-L10-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	2.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00	10	300	2.83E+03	94%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	5.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	9.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1316-T05-A	1	9.50E-01	U1/2		9.50E-01	6.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	6.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	2.1E+02	1.9E+00	6.0E+00	10	300	2.72E+03	91%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	2.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	3.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1316-T05-B	1	9.50E-01	U1/2		9.50E-01	1.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	5.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	2.4E+02	1.9E+00	6.0E+00	10	300	2.93E+03	98%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	3.9E+01	1.9E+00	6.0E+00					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	3.3E+01	1.9E+00	6.0E+00					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1316-T05-C	1	9.50E-01	U1/2		9.50E-01	6.3E+01	1.9E+00	6.0E+00					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
Be	EaFA-L10-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	5.0E+02	1.9E+00	6.0E+00					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	EaFA-L10-1316-T01-A	1	1.10E+00	U1/2		1.10E+00	3.1E+03	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1316-T02-A	1	1.10E+00	U1/2		1.10E+00	4.8E+01	2.2E+00	7.0E+00	10	300	2.81E+03	93%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1316-T03-A	1	1.10E+00	U1/2		1.10E+00	2.5E+02	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1316-T04-A	1	1.10E+00	U1/2		1.10E+00	1.1E+02	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1316-T05-A	1	1.10E+00	U1/2		1.10E+00	7.7E+01	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1316-T01-B	1	1.10E+00	U1/2		1.10E+00	1.7E+02	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1316-T02-B	1	2.60E+00	E		2.60E+00	2.1E+01	2.2E+00	7.0E+00	10	300	2.73E+03	91%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1316-T03-B	1	7.43E+00			7.43E+00	4.8E-01	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1316-T04-B	1	1.10E+00	U1/2		1.10E+00	8.3E+01	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1316-T05-B	1	1.10E+00	U1/2		1.10E+00	2.1E+02	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1316-T01-C	1	1.10E+00	U1/2		1.10E+00	1.3E+02	2.2E+00	7.0E+00				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1316-T02-C	1	1.10E+00	U1/2		1.10E+00	4.0E+01	2.2E+00	7.0E+00	10	300	2.91E+03	97%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1316-T03-C	1	3.02E+00	E		3.02E+00	4.0E+01	2.2E+00	7.0E+00					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1316-T04-C	1	1.10E+00	U1/2		1.10E+00	4.9E+01	2.2E+00	7.0E+00					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1316-T05-C	1	1.10E+00	U1/2		1.10E+00	6.9E+01	2.2E+00	7.0E+00					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
Cd	EaFA-L10-1316-B01-A	1	1.10E+00	U1/2		1.10E+00	5.6E+01	2.2E+00	7.0E+00					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	EaFA-L10-1316-T01-A	1	1.53E+05			1.53E+05	8.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1316-T02-A	1	3.01E+05			3.01E+05	3.3E-01	2.6E+00	8.3E+00	1000	100	3.02E+05	83%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1316-T03-A	1	6.38E+05			6.38E+05	5.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1316-T04-A	1	5.68E+05			5.68E+05	4.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1316-T05-A	1	4.65E+05			4.65E+05	7.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1316-T01-B	1	1.50E+05			1.50E+05	6.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1316-T02-B	1	2.87E+05			2.87E+05	2.0E+00	2.6E+00	8.3E+00	1000	100	2.88E+05	83%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1316-T03-B	1	7.01E+05			7.01E+05	1.8E+00	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1316-T04-B	1	4.87E+05			4.87E+05	4.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1316-T05-B	1	4.67E+05			4.67E+05	6.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1316-T01-C	1	1.43E+05			1.43E+05	5.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1316-T02-C	1	2.87E+05			2.87E+05	1.4E+00	2.6E+00	8.3E+00	1000	100	2.88E+05	90%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1316-T03-C	1	6.62E+05			6.62E+05	3.5E-01	2.6E+00	8.3E+00					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1316-T04-C	1	5.76E+05			5.76E+05	8.5E-01	2.6E+00	8.3E+00					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1316-T05-C	1	4.76E+05			4.76E+05	1.8E-01	2.6E+00	8.3E+00					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
Ca	EaFA-L10-1316-B01-A	1	1.97E+01			1.97E+01	2.5E+01	2.6E+00	8.3E+00					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	EaFA-L10-1316-T01-A	1	2.90E+01			2.90E+01	4.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1316-T02-A	1	2.91E+01			2.91E+01	8.9E+00	1.2E+00	3.8E+00	10	300	2.68E+03	88%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1316-T03-A	1	3.03E+02			3.03E+02	6.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1316-T04-A	1	5.65E+02			5.65E+02	4.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1316-T05-A	1	5.86E+01			5.86E+01	8.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1316-T01-B	1	2.02E+01			2.02E+01	4.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1316-T02-B	1	2.34E+01			2.34E+01	2.1E+00	1.2E+00	3.8E+00	10	300	2.61E+03	86%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1316-T03-B	1	1.14E+01			1.14E+01	1.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1316-T04-B	1	2.94E+01			2.94E+01	4.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1316-T05-B	1	6.63E+01			6.63E+01	3.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1316-T01-C	1	1.18E+01			1.18E+01	4.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1316-T02-C	1	2.33E+01			2.33E+01	5.7E+00	1.2E+00	3.8E+00	10	300	2.75E+03	91%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1316-T03-C	1	3.03E+01			3.03E+01	3.4E+00	1.2E+00	3.8E+00					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1316-T04-C	1	3.46E+01			3.46E+01	6.0E+00	1.2E+00	3.8E+00					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1316-T05-C	1	6.63E+01			6.63E+01	2.5E+00	1.2E+00	3.8E+00					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
Cr	EaFA-L10-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	6.9E+01	1.2E+00	3.8E+00					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	EaFA-L10-1316-T01-A	1	3.43E+01			3.43E+01	1.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1316-T02-A	1	5.73E+01			5.73E+01	8.1E-01	1.8E+00	5.7E+00	10	300	2.73E+03	89%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1316-T03-A	1	4.96E+00	E		4.96E+00	2.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1316-T04-A	1	1.18E+01			1.18E+01	1.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1316-T05-A	1	9.70E+01			9.70E+01	6.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1316-T01-B	1	4.83E+01			4.83E+01	4.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1316-T02-B	1	8.48E+01			8.48E+01	4.7E+00	1.8E+00	5.7E+00	10	300	2.68E+03	87%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1316-T03-B	1	2.45E+02			2.45E+02	2.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1316-T04-B	1	8.65E+01			8.65E+01	1.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1316-T05-B	1	7.19E+01			7.19E+01	2.9E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1316-T01-C	1	6.07E+01			6.07E+01	1.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1316-T02-C	1	8.99E+01			8.99E+01	8.3E-01	1.8E+00	5.7E+00	10	300	2.84E+03	92%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1316-T03-C	1	1.42E+02			1.42E+02	1.3E+00	1.8E+00	5.7E+00					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1316-T04-C	1	1.05E+02			1.05E+02	2.7E+00	1.8E+00	5.7E+00					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1316-T05-C	1	7.29E+01			7.29E+01	2.0E+00	1.8E+00	5.7E+00					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
Co	EaFA-L10-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	1.0E+02	1.8E+00	5.7E+00					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	EaFA-L10-1316-T01-A	1	8.93E+00	E		8.93E+00	7.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1316-T02-A	1	1.21E+01			1.21E+01	5.3E+01	3.7E+00	1.2E+01	10	300	2.70E+03	90%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1316-T03-A	1	7.21E+00	E		7.21E+00	6.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1316-T04-A	1	1.70E+01			1.70E+01	3.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1316-T05-A	1	3.15E+01			3.15E+01	3.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1316-T01-B	1	5.27E+00	E		5.27E+00	6.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1316-T02-B	1	7.35E+01			7.35E+01	1.1E+01	3.7E+00	1.2E+01	10	300	2.67E+03	86%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1316-T03-B	1	1.20E+01			1.20E+01	2.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1316-T04-B	1	1.06E+01	E		1.06E+01	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1316-T05-B	1	1.34E+01			1.34E+01	1.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1316-T01-C	1	1.29E+01			1.29E+01	1.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1316-T02-C	1	6.50E+00	E		6.50E+00	9.7E+01	3.7E+00	1.2E+01	10	300	2.78E+03	93%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1316-T03-C	1	7.45E+00	E		7.45E+00	4.0E+01	3.7E+00	1.2E+01					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1316-T04-C	1	1.33E+01			1.33E+01	5.4E+01	3.7E+00	1.2E+01					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1316-T05-C	1	1.37E+01			1.37E+01	2.5E+01	3.7E+00	1.2E+01					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
Cu	EaFA-L10-1316-B01-A	1	4.58E+00	E		4.58E+00	9.2E+00	3.7E+00	1.2E+01					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	EaFA-L10-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00	1000	100	8.22E+02	82%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	2.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1316-T04-A	1	3.06E+00	E		3.06E+00	2.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1316-T05-A	1	2.92E+01			2.92E+01	6.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.0E+00	6.4E+00	1000	100	7.99E+02	80%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	8.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	7.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1316-T05-B	1	3.27E+00	E		3.27E+00	8.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00	1000	100	8.50E+02	85%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1316-T03-C	1	2.23E+00	E		2.23E+00	7.4E+00	2.0E+00	6.4E+00					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1316-T05-C	1	1.00E+00	U1/2		1.00E+00	2.0E+00	2.0E+00	6.4E+00					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
Fe	EaFA-L10-1316-B01-A	1	6.33E+00	E		6.33E+00	3.7E+00	2.0E+00	6.4E+00					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	EaFA-L10-1316-T01-A	1	3.40E+00	U1/2		3.40E+00	2.1E+03	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1316-T02-A	1	3.40E+00	U1/2		3.40E+00	1.4E+02	6.8E+00	2.2E+01	10	300	2.70E+03	90%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1316-T03-A	1	3.40E+00	U1/2		3.40E+00	1.6E+02	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1316-T04-A	1	3.40E+00	U1/2		3.40E+00	1.4E+02	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1316-T05-A	1	6.88E+01			6.88E+01	2.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1316-T01-B	1	3.40E+00	U1/2		3.40E+00	6.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1316-T02-B	1	3.40E+00	U1/2		3.40E+00	1.9E+02	6.8E+00	2.2E+01	10	300	2.62E+03	87%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1316-T03-B	1	3.40E+00	U1/2		3.40E+00	8.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1316-T04-B	1	3.40E+00	U1/2		3.40E+00	2.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1316-T05-B	1	3.40E+00	U1/2		3.40E+00	1.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1316-T01-C	1	3.40E+00	U1/2		3.40E+00	2.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1316-T02-C	1	3.40E+00	U1/2		3.40E+00	5.4E+01	6.8E+00	2.2E+01	10	300	2.77E+03	92%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1316-T03-C	1	3.40E+00	U1/2		3.40E+00	5.7E+01	6.8E+00	2.2E+01					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1316-T04-C	1	3.40E+00	U1/2		3.40E+00	4.8E+01	6.8E+00	2.2E+01					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1316-T05-C	1	3.40E+00	U1/2		3.40E+00	4.6E+01	6.8E+00	2.2E+01					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
Pb	EaFA-L10-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	9.3E+01	6.8E+00	2.2E+01					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	EaFA-L10-1316-T01-A	1	3.35E+03			3.35E+03	1.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1316-T02-A	1	6.54E+03			6.54E+03	8.1E-01	1.9E+00	6.0E+00	10	300	8.98E+03	82%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1316-T03-A	1	1.14E+04			1.14E+04	1.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1316-T04-A	1	2.14E+04			2.14E+04	4.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1316-T05-A	1	5.89E+04			5.89E+04	7.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1316-T01-B	1	3.34E+03			3.34E+03	4.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1316-T02-B	1	6.30E+03			6.30E+03	2.3E+00	1.9E+00	6.0E+00	10	300	9.02E+03	91%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1316-T03-B	1	1.51E+04			1.51E+04	1.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1316-T04-B	1	2.75E+04			2.75E+04	7.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1316-T05-B	1	5.35E+04			5.35E+04	7.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1316-T01-C	1	3.21E+03			3.21E+03	2.2E-01	1.9E+00	6.0E+00				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1316-T02-C	1	6.35E+03			6.35E+03	1.5E+00	1.9E+00	6.0E+00	10	300	8.87E+03	84%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1316-T03-C	1	1.50E+04			1.50E+04	1.7E-01	1.9E+00	6.0E+00					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1316-T04-C	1	3.13E+04			3.13E+04	1.1E+00	1.9E+00	6.0E+00					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1316-T05-C	1	5.44E+04			5.44E+04	1.7E-01	1.9E+00	6.0E+00					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
Li	EaFA-L10-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	8.0E+00	1.9E+00	6.0E+00					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	EaFA-L10-1316-T01-A	1	2.95E+02			2.95E+02	2.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1316-T02-A	1	5.38E+02			5.38E+02	2.8E-01	2.0E+00	6.4E+00	10	300	3.09E+03	85%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1316-T03-A	1	8.10E+01			8.10E+01	5.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1316-T04-A	1	2.18E+02			2.18E+02	4.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1316-T05-A	1	1.01E+03			1.01E+03	7.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1316-T01-B	1	3.52E+02			3.52E+02	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1316-T02-B	1	6.27E+02			6.27E+02	2.1E+00	2.0E+00	6.4E+00	10	300	3.07E+03	81%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1316-T03-B	1	1.72E+03			1.72E+03	9.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1316-T04-B	1	9.64E+02			9.64E+02	6.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1316-T05-B	1	8.88E+02			8.88E+02	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1316-T01-C	1	4.07E+02			4.07E+02	3.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1316-T02-C	1	6.44E+02			6.44E+02	1.8E+00	2.0E+00	6.4E+00	10	300	3.28E+03	88%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1316-T03-C	1	1.08E+03			1.08E+03	7.5E-01	2.0E+00	6.4E+00					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1316-T04-C	1	1.16E+03			1.16E+03	5.7E-01	2.0E+00	6.4E+00					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1316-T05-C	1	9.15E+02			9.15E+02	7.3E-01	2.0E+00	6.4E+00					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
Mn	EaFA-L10-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	3.5E+01	2.0E+00	6.4E+00					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	EaFA-L10-1316-T01-A	1	7.51E+03			7.51E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1316-T02-A	1	1.46E+04			1.46E+04	1.1E+00	1.0E+00	3.2E+00	1000	100	1.55E+04	90%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1316-T03-A	1	3.60E+04			3.60E+04	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1316-T04-A	1	6.19E+04			6.19E+04	4.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1316-T05-A	1	1.15E+05			1.15E+05	6.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1316-T01-B	1	7.14E+03			7.14E+03	8.0E-02	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1316-T02-B	1	1.37E+04			1.37E+04	2.8E+00	1.0E+00	3.2E+00	1000	100	1.47E+04	97%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1316-T03-B	1	3.86E+04			3.86E+04	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1316-T04-B	1	6.05E+04			6.05E+04	5.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1316-T05-B	1	1.08E+05			1.08E+05	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1316-T01-C	1	7.39E+03			7.39E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1316-T02-C	1	1.39E+04			1.39E+04	9.8E-01	1.0E+00	3.2E+00	1000	100	1.47E+04	83%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1316-T03-C	1	3.57E+04			3.57E+04	7.6E-01	1.0E+00	3.2E+00					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1316-T04-C	1	7.10E+04			7.10E+04	1.8E+00	1.0E+00	3.2E+00					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1316-T05-C	1	1.13E+05			1.13E+05	5.7E-01	1.0E+00	3.2E+00					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
Mg	EaFA-L10-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	9.2E+00	1.0E+00	3.2E+00					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	EaFA-L10-1316-T01-A	1	3.27E+03			3.27E+03	5.1E-02	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1316-T02-A	1	6.12E+03			6.12E+03	8.3E-01	1.2E+00	3.8E+00	10	300	8.75E+03	88%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1316-T03-A	1	1.64E+04			1.64E+04	3.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1316-T04-A	1	2.74E+04			2.74E+04	4.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1316-T05-A	1	3.77E+04			3.77E+04	7.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1316-T01-B	1	3.20E+03			3.20E+03	7.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1316-T02-B	1	5.62E+03			5.62E+03	2.5E+00	1.2E+00	3.8E+00	10	300	8.22E+03	87%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1316-T03-B	1	1.16E+04			1.16E+04	1.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1316-T04-B	1	2.55E+04			2.55E+04	4.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1316-T05-B	1	4.53E+04			4.53E+04	4.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1316-T01-C	1	3.08E+03			3.08E+03	7.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1316-T02-C	1	5.71E+03			5.71E+03	1.2E+00	1.2E+00	3.8E+00	10	300	8.59E+03	96%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1316-T03-C	1	1.32E+04			1.32E+04	1.7E+00	1.2E+00	3.8E+00					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1316-T04-C	1	2.83E+04			2.83E+04	5.3E-01	1.2E+00	3.8E+00					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1316-T05-C	1	4.65E+04			4.65E+04	1.8E-01	1.2E+00	3.8E+00					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
Mo	EaFA-L10-1316-B01-A	1	8.98E+00			8.98E+00	5.5E+00	1.2E+00	3.8E+00					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	EaFA-L10-1316-T01-A	1	8.67E+01			8.67E+01	4.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1316-T02-A	1	1.44E+02			1.44E+02	3.3E+00	1.8E+00	5.7E+00	10	300	2.86E+03	90%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1316-T03-A	1	7.11E+00			7.11E+00	3.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1316-T04-A	1	4.60E+01			4.60E+01	1.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1316-T05-A	1	2.79E+02			2.79E+02	6.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1316-T01-B	1	1.10E+02			1.10E+02	3.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1316-T02-B	1	1.97E+02			1.97E+02	4.2E+00	1.8E+00	5.7E+00	10	300	2.82E+03	88%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1316-T03-B	1	5.41E+02			5.41E+02	2.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1316-T04-B	1	2.11E+02			2.11E+02	9.3E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1316-T05-B	1	2.38E+02			2.38E+02	9.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1316-T01-C	1	1.30E+02			1.30E+02	4.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1316-T02-C	1	2.08E+02			2.08E+02	1.1E+00	1.8E+00	5.7E+00	10	300	3.00E+03	93%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1316-T03-C	1	3.20E+02			3.20E+02	1.9E+00	1.8E+00	5.7E+00					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1316-T04-C	1	2.43E+02			2.43E+02	6.1E-01	1.8E+00	5.7E+00					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1316-T05-C	1	2.41E+02			2.41E+02	2.8E+00	1.8E+00	5.7E+00					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
Ni	EaFA-L10-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	1.9E+01	1.8E+00	5.7E+00					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	EaFA-L10-1316-T01-A	1	1.81E+01			1.81E+01	1.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1316-T02-A	1	1.31E+02			1.31E+02	1.1E+01	3.7E+00	1.2E+01	1000	100	9.95E+02	86%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1316-T03-A	1	3.96E+01			3.96E+01	2.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1316-T04-A	1	1.39E+02			1.39E+02	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1316-T05-A	1	7.16E+01			7.16E+01	3.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1316-T01-B	1	1.01E+01	E		1.01E+01	3.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1316-T02-B	1	6.64E+00	E		6.64E+00	6.5E+01	3.7E+00	1.2E+01	1000	100	8.52E+02	85%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1316-T03-B	1	1.40E+01			1.40E+01	6.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1316-T04-B	1	5.96E+01			5.96E+01	2.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1316-T05-B	1	7.81E+01			7.81E+01	1.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1316-T01-C	1	1.58E+01			1.58E+01	3.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1316-T02-C	1	1.85E+00	U1/2		1.85E+00	2.2E+02	3.7E+00	1.2E+01	1000	100	9.41E+02	94%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1316-T03-C	1	1.04E+01	E		1.04E+01	8.8E+01	3.7E+00	1.2E+01					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1316-T04-C	1	9.35E+01			9.35E+01	1.6E+01	3.7E+00	1.2E+01					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1316-T05-C	1	5.26E+01			5.26E+01	2.9E+01	3.7E+00	1.2E+01					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
P	EaFA-L10-1316-B01-A	1	3.08E+01			3.08E+01	4.0E+00	3.7E+00	1.2E+01					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	EaFA-L10-1316-T01-A	1	3.02E+04			3.02E+04	1.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1316-T02-A	1	5.63E+04			5.63E+04	7.1E-01	1.6E+00	5.1E+00	1000	100	5.72E+04	85%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1316-T03-A	1	1.17E+05			1.17E+05	6.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1316-T04-A	1	1.85E+05			1.85E+05	3.6E+00	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1316-T05-A	1	3.06E+05			3.06E+05	7.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1316-T01-B	1	2.74E+04			2.74E+04	3.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1316-T02-B	1	5.19E+04			5.19E+04	1.8E+00	1.6E+00	5.1E+00	1000	100	5.27E+04	84%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1316-T03-B	1	1.25E+05			1.25E+05	1.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1316-T04-B	1	1.83E+05			1.83E+05	6.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1316-T05-B	1	3.06E+05			3.06E+05	1.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1316-T01-C	1	2.72E+04			2.72E+04	5.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1316-T02-C	1	5.10E+04			5.10E+04	1.3E+00	1.6E+00	5.1E+00	1000	100	5.19E+04	88%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1316-T03-C	1	1.23E+05			1.23E+05	4.1E-01	1.6E+00	5.1E+00					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1316-T04-C	1	2.05E+05			2.05E+05	1.4E+00	1.6E+00	5.1E+00					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1316-T05-C	1	3.08E+05			3.08E+05	4.4E-01	1.6E+00	5.1E+00					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
K	EaFA-L10-1316-B01-A	1	5.40E+01			5.40E+01	5.1E-01	1.6E+00	5.1E+00					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	EaFA-L10-1316-T01-A	1	1.09E+03			1.09E+03	1.6E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1316-T02-A	1	1.18E+03			1.18E+03	1.4E+00	1.5E+01	4.8E+01	10	300	3.83E+03	88%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1316-T03-A	1	3.11E+03			3.11E+03	3.0E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1316-T04-A	1	2.95E+03			2.95E+03	2.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1316-T05-A	1	2.08E+03			2.08E+03	9.8E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1316-T01-B	1	9.20E+02			9.20E+02	1.8E-01	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1316-T02-B	1	1.04E+03			1.04E+03	5.9E+00	1.5E+01	4.8E+01	10	300	3.63E+03	86%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1316-T03-B	1	1.15E+03			1.15E+03	1.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1316-T04-B	1	2.11E+03			2.11E+03	1.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1316-T05-B	1	2.72E+03			2.72E+03	5.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1316-T01-C	1	8.60E+02			8.60E+02	2.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1316-T02-C	1	1.08E+03			1.08E+03	2.2E+00	1.5E+01	4.8E+01	10	300	3.93E+03	95%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1316-T03-C	1	1.53E+03			1.53E+03	1.9E+00	1.5E+01	4.8E+01					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1316-T04-C	1	2.23E+03			2.23E+03	5.6E-01	1.5E+01	4.8E+01					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1316-T05-C	1	2.78E+03			2.78E+03	8.2E-01	1.5E+01	4.8E+01					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
Se	EaFA-L10-1316-B01-A	1	3.52E+01	E		3.52E+01	1.2E+02	1.5E+01	4.8E+01					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	EaFA-L10-1316-T01-A	1	1.83E+03			1.83E+03	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1316-T02-A	1	2.02E+03			2.02E+03	8.5E-01	1.1E+00	3.5E+00	1000	100	2.98E+03	97%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1316-T03-A	1	8.02E+02			8.02E+02	1.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1316-T04-A	1	1.07E+03			1.07E+03	3.6E+00	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1316-T05-A	1	1.59E+03			1.59E+03	7.4E+00	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1316-T01-B	1	1.97E+03			1.97E+03	5.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1316-T02-B	1	2.10E+03			2.10E+03	2.7E+00	1.1E+00	3.5E+00	1000	100	3.04E+03	95%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1316-T03-B	1	2.88E+03			2.88E+03	2.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1316-T04-B	1	1.92E+03			1.92E+03	6.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1316-T05-B	1	1.67E+03			1.67E+03	6.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1316-T01-C	1	2.32E+03			2.32E+03	9.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1316-T02-C	1	2.16E+03			2.16E+03	1.6E+00	1.1E+00	3.5E+00	1000	100	3.11E+03	95%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1316-T03-C	1	2.07E+03			2.07E+03	1.5E+00	1.1E+00	3.5E+00					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1316-T04-C	1	2.17E+03			2.17E+03	4.1E-01	1.1E+00	3.5E+00					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1316-T05-C	1	1.73E+03			1.73E+03	1.3E+00	1.1E+00	3.5E+00					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
Si	EaFA-L10-1316-B01-A	1	5.50E-01	U1/2		5.50E-01	3.2E+01	1.1E+00	3.5E+00					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	EaFA-L10-1316-T01-A	1	5.01E+03			5.01E+03	1.4E+00	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1316-T02-A	1	1.04E+04			1.04E+04	7.3E-01	2.5E+00	8.0E+00	1000	100	1.13E+04	91%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1316-T03-A	1	2.54E+04			2.54E+04	4.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1316-T04-A	1	4.29E+04			4.29E+04	3.6E+00	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1316-T05-A	1	6.02E+04			6.02E+04	7.0E+00	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1316-T01-B	1	5.00E+03			5.00E+03	8.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1316-T02-B	1	9.85E+03			9.85E+03	2.5E+00	2.5E+00	8.0E+00	1000	100	1.07E+04	89%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1316-T03-B	1	2.83E+04			2.83E+04	2.0E+00	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1316-T04-B	1	4.01E+04			4.01E+04	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1316-T05-B	1	6.73E+04			6.73E+04	1.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1316-T01-C	1	4.80E+03			4.80E+03	6.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1316-T02-C	1	1.01E+04			1.01E+04	1.2E+00	2.5E+00	8.0E+00	1000	100	1.10E+04	85%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1316-T03-C	1	2.66E+04			2.66E+04	6.6E-01	2.5E+00	8.0E+00					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1316-T04-C	1	4.56E+04			4.56E+04	6.3E-01	2.5E+00	8.0E+00					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1316-T05-C	1	6.81E+04			6.81E+04	7.3E-01	2.5E+00	8.0E+00					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
Na	EaFA-L10-1316-B01-A	1	1.61E+02			1.61E+02	5.7E-01	2.5E+00	8.0E+00					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	EaFA-L10-1316-T01-A	1	2.21E+03			2.21E+03	2.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1316-T02-A	1	3.89E+03			3.89E+03	2.4E-01	1.0E+00	3.2E+00	1000	100	4.78E+03	90%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1316-T03-A	1	1.04E+04			1.04E+04	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1316-T04-A	1	1.04E+04			1.04E+04	4.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1316-T05-A	1	7.04E+03			7.04E+03	7.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1316-T01-B	1	2.07E+03			2.07E+03	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1316-T02-B	1	3.62E+03			3.62E+03	2.4E+00	1.0E+00	3.2E+00	1000	100	4.75E+03	113%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1316-T03-B	1	8.46E+03			8.46E+03	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1316-T04-B	1	7.19E+03			7.19E+03	3.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1316-T05-B	1	7.17E+03			7.17E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1316-T01-C	1	2.13E+03			2.13E+03	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1316-T02-C	1	3.68E+03			3.68E+03	1.6E+00	1.0E+00	3.2E+00	1000	100	4.59E+03	92%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1316-T03-C	1	7.33E+03			7.33E+03	6.3E-01	1.0E+00	3.2E+00					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1316-T04-C	1	8.56E+03			8.56E+03	2.7E-01	1.0E+00	3.2E+00					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1316-T05-C	1	7.33E+03			7.33E+03	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
Sr	EaFA-L10-1316-B01-A	1	1.32E+00	E		1.32E+00	4.5E+01	1.0E+00	3.2E+00					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	EaFA-L10-1316-T01-A	1	1.56E+05			1.56E+05	1.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1316-T02-A	1	3.06E+05			3.06E+05	1.1E+00	6.8E+00	2.2E+01	1000	100	3.07E+05	84%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1316-T03-A	1	6.53E+05			6.53E+05	1.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1316-T04-A	1	6.77E+05			6.77E+05	3.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1316-T05-A	1	8.08E+05			8.08E+05	6.8E+00	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1316-T01-B	1	1.53E+05			1.53E+05	5.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1316-T02-B	1	2.90E+05			2.90E+05	2.8E+00	6.8E+00	2.2E+01	1000	100	2.90E+05	81%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1316-T03-B	1	7.00E+05			7.00E+05	2.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1316-T04-B	1	6.78E+05			6.78E+05	5.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1316-T05-B	1	8.79E+05			8.79E+05	3.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1316-T01-C	1	1.49E+05			1.49E+05	7.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1316-T02-C	1	3.00E+05			3.00E+05	1.7E+00	6.8E+00	2.2E+01	1000	100	3.01E+05	86%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1316-T03-C	1	7.08E+05			7.08E+05	7.7E-01	6.8E+00	2.2E+01					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1316-T04-C	1	7.60E+05			7.60E+05	7.5E-01	6.8E+00	2.2E+01					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1316-T05-C	1	9.11E+05			9.11E+05	3.4E-01	6.8E+00	2.2E+01					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
S	EaFA-L10-1316-B01-A	1	1.80E+01	E		1.80E+01	4.1E+00	6.8E+00	2.2E+01					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

TI	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	EaFA-L10-1316-T01-A	1	2.30E+00	U1/2		2.30E+00	6.4E+02	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
Tl	EaFA-L10-1316-T02-A	1	2.30E+00	U1/2		2.30E+00	2.4E+03	4.6E+00	1.5E+01	10	300	2.77E+03	92%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
Tl	EaFA-L10-1316-T03-A	1	2.30E+00	U1/2		2.30E+00	8.2E+02	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
Tl	EaFA-L10-1316-T04-A	1	2.30E+00	U1/2		2.30E+00	4.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
Tl	EaFA-L10-1316-T05-A	1	2.01E+01			2.01E+01	5.9E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
Tl	EaFA-L10-1316-T01-B	1	2.30E+00	U1/2		2.30E+00	2.5E+03	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
Tl	EaFA-L10-1316-T02-B	1	2.30E+00	U1/2		2.30E+00	5.6E+01	4.6E+00	1.5E+01	10	300	2.68E+03	89%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
Tl	EaFA-L10-1316-T03-B	1	1.03E+01	E		1.03E+01	5.9E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
Tl	EaFA-L10-1316-T04-B	1	1.55E+01			1.55E+01	5.4E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
Tl	EaFA-L10-1316-T05-B	1	3.16E+01			3.16E+01	7.1E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
Tl	EaFA-L10-1316-T01-C	1	2.30E+00	U1/2		2.30E+00	4.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
Tl	EaFA-L10-1316-T02-C	1	2.30E+00	U1/2		2.30E+00	1.0E+02	4.6E+00	1.5E+01	10	300	2.87E+03	96%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
Tl	EaFA-L10-1316-T03-C	1	2.30E+00	U1/2		2.30E+00	1.5E+02	4.6E+00	1.5E+01					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
Tl	EaFA-L10-1316-T04-C	1	2.30E+01			2.30E+01	2.5E+01	4.6E+00	1.5E+01					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
Tl	EaFA-L10-1316-T05-C	1	1.52E+01			1.52E+01	3.7E+01	4.6E+00	1.5E+01					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
Tl	EaFA-L10-1316-B01-A	1	2.30E+00	U1/2		2.30E+00	1.4E+01	4.6E+00	1.5E+01					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	EaFA-L10-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	5.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	3.1E+01	2.0E+00	6.4E+00	10	300	2.59E+03	86%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1316-T05-A	1	9.04E+00			9.04E+00	2.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	1.3E+01	2.0E+00	6.4E+00	10	300	2.50E+03	83%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	5.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1316-T05-B	1	1.00E+00	U1/2		1.00E+00	2.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	5.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00	10	300	2.69E+03	90%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	4.5E+01	2.0E+00	6.4E+00					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1316-T05-C	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
Ti	EaFA-L10-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	EaFA-L10-1316-T01-A	1	1.95E+02			1.95E+02	5.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1316-T02-A	1	2.21E+02			2.21E+02	7.3E-01	1.5E+00	4.8E+00	10	300	2.83E+03	87%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1316-T03-A	1	3.64E+02			3.64E+02	2.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1316-T04-A	1	3.33E+02			3.33E+02	4.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1316-T05-A	1	2.53E+02			2.53E+02	8.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1316-T01-B	1	1.85E+02			1.85E+02	7.0E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1316-T02-B	1	2.10E+02			2.10E+02	3.5E+00	1.5E+00	4.8E+00	10	300	2.73E+03	84%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1316-T03-B	1	2.81E+02			2.81E+02	1.9E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1316-T04-B	1	3.34E+02			3.34E+02	7.6E-01	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1316-T05-B	1	3.31E+02			3.31E+02	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1316-T01-C	1	1.74E+02			1.74E+02	1.9E+00	1.5E+00	4.8E+00				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1316-T02-C	1	2.15E+02			2.15E+02	1.9E+00	1.5E+00	4.8E+00	10	300	2.92E+03	90%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1316-T03-C	1	2.95E+02			2.95E+02	6.8E-01	1.5E+00	4.8E+00					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1316-T04-C	1	3.66E+02			3.66E+02	7.3E-01	1.5E+00	4.8E+00					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1316-T05-C	1	3.42E+02			3.42E+02	7.1E-01	1.5E+00	4.8E+00					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
V	EaFA-L10-1316-B01-A	1	6.82E+00			6.82E+00	3.1E+01	1.5E+00	4.8E+00					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	EaFA-L10-1316-T01-A	1	3.87E+01			3.87E+01	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:49 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1316-T02-A	1	4.84E+01			4.84E+01	9.5E-01	1.0E+00	3.2E+00	10	300	2.87E+03	94%	VU ICP-OES	7/1/10 12:50 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1316-T03-A	1	1.48E+01			1.48E+01	5.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:52 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1316-T04-A	1	6.95E+01			6.95E+01	4.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:53 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1316-T05-A	1	1.64E+02			1.64E+02	8.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:55 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1316-T01-B	1	1.78E+01			1.78E+01	3.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 12:57 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1316-T02-B	1	2.57E+01			2.57E+01	2.2E+00	1.0E+00	3.2E+00	10	300	2.76E+03	91%	VU ICP-OES	7/1/10 12:58 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1316-T03-B	1	5.53E+01			5.53E+01	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:00 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1316-T04-B	1	2.43E+01			2.43E+01	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:02 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1316-T05-B	1	4.13E+01			4.13E+01	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:56 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1316-T01-C	1	2.80E+01			2.80E+01	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	7/1/10 1:05 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1316-T02-C	1	2.22E+01			2.22E+01	3.5E+00	1.0E+00	3.2E+00	10	300	2.96E+03	98%	VU ICP-OES	7/1/10 1:07 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1316-T03-C	1	2.69E+01			2.69E+01	2.8E+00	1.0E+00	3.2E+00					VU ICP-OES	7/1/10 1:08 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1316-T04-C	1	2.69E+01			2.69E+01	1.5E+00	1.0E+00	3.2E+00					VU ICP-OES	7/1/10 1:10 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1316-T05-C	1	4.26E+01			4.26E+01	3.0E+00	1.0E+00	3.2E+00					VU ICP-OES	7/1/10 1:48 PM	EPA Interlab L10 1313-1316 EaFA
Zn	EaFA-L10-1316-B01-A	1	1.51E+01			1.51E+01	3.1E+00	1.0E+00	3.2E+00					VU ICP-OES	7/1/10 12:44 PM	EPA Interlab L10 1313-1316 EaFA

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	EaFA-L11-1316-T01-A	1	893.862			8.94E+02	0.263915	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1316-T02-A	1	760.171			7.60E+02	0.768147	1.0E+00	3.2E+00	1000	100	1741.83	98%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1316-T03-A	1	693.455			6.93E+02	1.30853	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1316-T04-A	1	367.286			3.67E+02	1.70069	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1316-T05-A															
Al	EaFA-L11-1316-T01-B	1	952.221			9.52E+02	0.750216	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1316-T02-B	1	730.072			7.30E+02	0.589479	1.0E+00	3.2E+00	1000	100	1771.24	104%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1316-T03-B	1	714.221			7.14E+02	0.448981	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1316-T04-B	1	342.661			3.43E+02	2.12117	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1316-T05-B															
Al	EaFA-L11-1316-T01-C	1	795.626			7.96E+02	1.20347	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1316-T02-C	1	856.763			8.57E+02	0.716155	1.0E+00	3.2E+00	1000	100	1851.61	99%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1316-T03-C	1	647.976			6.48E+02	1.44898	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1316-T04-C	1	330.266			3.30E+02	2.33855	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
Al	EaFA-L11-1316-T05-C															
Al	EaFA-L11-1316-B01-A	1	0.5	U1/2		5.00E-01	59.1082	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	EaFA-L11-1316-T01-A	1	100.052			1.00E+02	18.8048	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1316-T02-A	1	165.379			1.65E+02	20.6404	7.5E+00	2.4E+01	10	325	3383.78	99%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1316-T03-A	1	183.996			1.84E+02	7.7251	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1316-T04-A	1	410.459			4.10E+02	7.6617	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1316-T05-A															
Sb	EaFA-L11-1316-T01-B	1	120.638			1.21E+02	11.6424	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1316-T02-B	1	151.015			1.51E+02	19.4992	7.5E+00	2.4E+01	10	325	3535.93	104%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1316-T03-B	1	201.161			2.01E+02	14.2944	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1316-T04-B	1	452.922			4.53E+02	16.995	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1316-T05-B															
Sb	EaFA-L11-1316-T01-C	1	89.757			8.98E+01	0.590429	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1316-T02-C	1	136.325			1.36E+02	14.1151	7.5E+00	2.4E+01	10	325	3442.34	102%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1316-T03-C	1	200.079			2.00E+02	8.56931	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1316-T04-C	1	420.564			4.21E+02	2.55048	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
Sb	EaFA-L11-1316-T05-C															
Sb	EaFA-L11-1316-B01-A	1	19.184	E		1.92E+01	33.7122	7.5E+00	2.4E+01				---	VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	EaFA-L11-1316-T01-A	1	129.403			1.29E+02	15.2451	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1316-T02-A	1	111.08			1.11E+02	18.0703	1.1E+01	3.5E+01	10	325	3435.69	102%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1316-T03-A	1	127.735			1.28E+02	6.22284	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1316-T04-A	1	82.439			8.24E+01	50.3843	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1316-T05-A															
As	EaFA-L11-1316-T01-B	1	130.793			1.31E+02	6.98758	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1316-T02-B	1	143.635			1.44E+02	14.2176	1.1E+01	3.5E+01	10	325	3500.35	103%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1316-T03-B	1	150.353			1.50E+02	16.1344	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1316-T04-B	1	49.512			4.95E+01	83.4805	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1316-T05-B															
As	EaFA-L11-1316-T01-C	1	155.186			1.55E+02	2.05315	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1316-T02-C	1	129.359			1.29E+02	4.45335	1.1E+01	3.5E+01	10	325	3460.8	103%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1316-T03-C	1	132.233			1.32E+02	9.42833	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1316-T04-C	1	59.908			5.99E+01	20.6251	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
As	EaFA-L11-1316-T05-C															
As	EaFA-L11-1316-B01-A	1	5.5	U1/2		5.50E+00	48.7135	1.1E+01	3.5E+01			---		VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	EaFA-L11-1316-T01-A	1	4060.04			4.06E+03	0.877445	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1316-T02-A	1	7659.26			7.66E+03	0.674971	1.0E+00	3.2E+00	1000	100	8533.62	87%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1316-T03-A	1	16165.6			1.62E+04	1.24227	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1316-T04-A	1	31363.2			3.14E+04	2.35418	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1316-T05-A															
B	EaFA-L11-1316-T01-B	1	4176.17			4.18E+03	0.778882	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1316-T02-B	1	7724.71			7.72E+03	1.3032	1.0E+00	3.2E+00	1000	100	8631.99	91%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1316-T03-B	1	16247.3			1.62E+04	1.54927	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1316-T04-B	1	33597.8			3.36E+04	3.08961	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1316-T05-B															
B	EaFA-L11-1316-T01-C	1	4228.04			4.23E+03	1.4278	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1316-T02-C	1	7889.76			7.89E+03	0.985866	1.0E+00	3.2E+00	1000	100	8808.14	92%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1316-T03-C	1	16682.7			1.67E+04	1.1462	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1316-T04-C	1	34551			3.46E+04	0.885031	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
B	EaFA-L11-1316-T05-C															
B	EaFA-L11-1316-B01-A	1	12.339			1.23E+01	5.37264	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	EaFA-L11-1316-T01-A	1	313.36			3.13E+02	0.263242	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1316-T02-A	1	282.366			2.82E+02	0.200762	1.0E+00	3.2E+00	10	325	3275.86	92%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1316-T03-A	1	254.655			2.55E+02	1.59994	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1316-T04-A	1	278.6			2.79E+02	0.543939	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1316-T05-A															
Ba	EaFA-L11-1316-T01-B	1	320.35			3.20E+02	0.842249	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1316-T02-B	1	276.015			2.76E+02	0.895822	1.0E+00	3.2E+00	10	325	3383.73	96%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1316-T03-B	1	245.767			2.46E+02	0.638829	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1316-T04-B	1	285.612			2.86E+02	0.244231	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1316-T05-B															
Ba	EaFA-L11-1316-T01-C	1	310.427			3.10E+02	0.684597	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1316-T02-C	1	284.547			2.85E+02	0.993593	1.0E+00	3.2E+00	10	325	3306.08	93%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1316-T03-C	1	252.749			2.53E+02	0.575564	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1316-T04-C	1	303.598			3.04E+02	0.380059	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
Ba	EaFA-L11-1316-T05-C															
Ba	EaFA-L11-1316-B01-A	1	3.254			3.25E+00	18.0254	1.0E+00	3.2E+00				---	VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	EaFA-L11-1316-T01-A	1	0.95	U1/2		9.50E-01	66.7529	1.9E+00	6.0E+00				---	VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1316-T02-A	1	0.95	U1/2		9.50E-01	40.4365	1.9E+00	6.0E+00	10	325	3286.69	101%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1316-T03-A	1	0.95	U1/2		9.50E-01	223.881	1.9E+00	6.0E+00				---	VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1316-T04-A	1	0.95	U1/2		9.50E-01	1632.4	1.9E+00	6.0E+00				---	VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1316-T05-A															
Be	EaFA-L11-1316-T01-B	1	0.95	U1/2		9.50E-01	678.644	1.9E+00	6.0E+00				---	VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1316-T02-B	1	0.95	U1/2		9.50E-01	258.104	1.9E+00	6.0E+00	10	325	3416.87	105%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1316-T03-B	1	0.95	U1/2		9.50E-01	47.2553	1.9E+00	6.0E+00				---	VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1316-T04-B	1	0.95	U1/2		9.50E-01	63.163	1.9E+00	6.0E+00				---	VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1316-T05-B															
Be	EaFA-L11-1316-T01-C	1	0.95	U1/2		9.50E-01	42.9655	1.9E+00	6.0E+00				---	VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1316-T02-C	1	0.95	U1/2		9.50E-01	190.473	1.9E+00	6.0E+00	10	325	3332.27	103%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1316-T03-C	1	0.95	U1/2		9.50E-01	266.514	1.9E+00	6.0E+00				---	VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1316-T04-C	1	0.95	U1/2		9.50E-01	370.674	1.9E+00	6.0E+00				---	VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
Be	EaFA-L11-1316-T05-C															
Be	EaFA-L11-1316-B01-A	1	0.95	U1/2		9.50E-01	108.837	1.9E+00	6.0E+00				---	VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	EaFA-L11-1316-T01-A	1	1.1	U1/2		1.10E+00	142.407	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1316-T02-A	1	1.1	U1/2		1.10E+00	138.799	2.2E+00	7.0E+00	10	325	3214.33	99%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1316-T03-A	1	1.1	U1/2		1.10E+00	118.902	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1316-T04-A	1	2.37	E		2.37E+00	37.9181	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1316-T05-A															
Cd	EaFA-L11-1316-T01-B	1	1.1	U1/2		1.10E+00	181.041	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1316-T02-B	1	1.1	U1/2		1.10E+00	112.594	2.2E+00	7.0E+00	10	325	3356.22	103%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1316-T03-B	1	1.1	U1/2		1.10E+00	177.969	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1316-T04-B	1	4.465	E		4.47E+00	3.89756	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1316-T05-B															
Cd	EaFA-L11-1316-T01-C	1	1.1	U1/2		1.10E+00	23.0744	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1316-T02-C	1	1.1	U1/2		1.10E+00	3182.28	2.2E+00	7.0E+00	10	325	3260.07	100%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1316-T03-C	1	1.1	U1/2		1.10E+00	179.778	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1316-T04-C	1	4.808	E		4.81E+00	25.1486	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
Cd	EaFA-L11-1316-T05-C															
Cd	EaFA-L11-1316-B01-A	1	1.1	U1/2		1.10E+00	39.8185	2.2E+00	7.0E+00			---		VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	EaFA-L11-1316-T01-A	1	142136			1.42E+05	0.119897	2.6E+00	8.3E+00			---		VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1316-T02-A	1	282438			2.82E+05	1.0463	2.6E+00	8.3E+00	1000	100	283368	93%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1316-T03-A	1	682815			6.83E+05	1.20318	2.6E+00	8.3E+00			---		VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1316-T04-A	1	566074			5.66E+05	0.678374	2.6E+00	8.3E+00			---		VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1316-T05-A															
Ca	EaFA-L11-1316-T01-B	1	142346			1.42E+05	0.843683	2.6E+00	8.3E+00			---		VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1316-T02-B	1	282298			2.82E+05	1.10484	2.6E+00	8.3E+00	1000	100	283174	88%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1316-T03-B	1	682441			6.82E+05	0.565621	2.6E+00	8.3E+00			---		VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1316-T04-B	1	540783			5.41E+05	0.048435	2.6E+00	8.3E+00			---		VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1316-T05-B															
Ca	EaFA-L11-1316-T01-C	1	141864			1.42E+05	1.52646	2.6E+00	8.3E+00			---		VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1316-T02-C	1	285031			2.85E+05	1.28235	2.6E+00	8.3E+00	1000	100	285925	89%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1316-T03-C	1	678878			6.79E+05	0.769051	2.6E+00	8.3E+00			---		VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1316-T04-C	1	559830			5.60E+05	0.450978	2.6E+00	8.3E+00			---		VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
Ca	EaFA-L11-1316-T05-C															
Ca	EaFA-L11-1316-B01-A	1	1.3	U1/2		1.30E+00	9.35462	2.6E+00	8.3E+00			---		VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	EaFA-L11-1316-T01-A	1	315.402			3.15E+02	0.388233	1.2E+00	3.8E+00			---		VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1316-T02-A	1	537.232			5.37E+02	0.819347	1.2E+00	3.8E+00	10	325	3624.65	95%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1316-T03-A	1	957.154			9.57E+02	1.63057	1.2E+00	3.8E+00			---		VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1316-T04-A	1	204.225			2.04E+02	1.67282	1.2E+00	3.8E+00			---		VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1316-T05-A															
Cr	EaFA-L11-1316-T01-B	1	321.532			3.22E+02	0.351263	1.2E+00	3.8E+00			---		VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1316-T02-B	1	539.171			5.39E+02	1.84432	1.2E+00	3.8E+00	10	325	3780.43	100%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1316-T03-B	1	976.954			9.77E+02	0.61846	1.2E+00	3.8E+00			---		VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1316-T04-B	1	85.529			8.55E+01	0.781066	1.2E+00	3.8E+00			---		VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1316-T05-B															
Cr	EaFA-L11-1316-T01-C	1	318.341			3.18E+02	0.629303	1.2E+00	3.8E+00			---		VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1316-T02-C	1	542.257			5.42E+02	1.09523	1.2E+00	3.8E+00	10	325	3679.97	97%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1316-T03-C	1	958.676			9.59E+02	0.971424	1.2E+00	3.8E+00			---		VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1316-T04-C	1	85.02			8.50E+01	0.952107	1.2E+00	3.8E+00			---		VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
Cr	EaFA-L11-1316-T05-C															
Cr	EaFA-L11-1316-B01-A	1	0.6	U1/2		6.00E-01	346.453	1.2E+00	3.8E+00			---		VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	EaFA-L11-1316-T01-A	1	2.901	E		2.90E+00	64.9828	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1316-T02-A	1	0.9	U1/2		9.00E-01	140.982	1.8E+00	5.7E+00	10	325	3121.04	96%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1316-T03-A	1	7.769			7.77E+00	14.0136	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1316-T04-A	1	79.051			7.91E+01	6.15924	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1316-T05-A															
Co	EaFA-L11-1316-T01-B	1	3.992	E		3.99E+00	110.531	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1316-T02-B	1	5.019	E		5.02E+00	67.4448	1.8E+00	5.7E+00	10	325	3271.79	101%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1316-T03-B	1	3.613	E		3.61E+00	72.2268	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1316-T04-B	1	169.272			1.69E+02	3.57476	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1316-T05-B															
Co	EaFA-L11-1316-T01-C	1	0.9	U1/2		9.00E-01	13.5318	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1316-T02-C	1	4.578	E		4.58E+00	64.3016	1.8E+00	5.7E+00	10	325	3176.53	98%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1316-T03-C	1	5.656	E		5.66E+00	77.6353	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1316-T04-C	1	174.09			1.74E+02	2.86592	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
Co	EaFA-L11-1316-T05-C															
Co	EaFA-L11-1316-B01-A	1	0.9	U1/2		9.00E-01	67.5446	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	EaFA-L11-1316-T01-A	1	17.715			1.77E+01	34.6117	3.7E+00	1.2E+01				---	VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1316-T02-A	1	22.771			2.28E+01	28.3511	3.7E+00	1.2E+01	10	325	3228.71	99%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1316-T03-A	1	24.257			2.43E+01	18.6996	3.7E+00	1.2E+01				---	VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1316-T04-A	1	22.878			2.29E+01	7.97491	3.7E+00	1.2E+01				---	VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1316-T05-A															
Cu	EaFA-L11-1316-T01-B	1	12.109			1.21E+01	34.0558	3.7E+00	1.2E+01				---	VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1316-T02-B	1	11.608	E		1.16E+01	43.8654	3.7E+00	1.2E+01	10	325	3378.17	104%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1316-T03-B	1	17.079			1.71E+01	11.6577	3.7E+00	1.2E+01				---	VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1316-T04-B	1	19.631			1.96E+01	37.1987	3.7E+00	1.2E+01				---	VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1316-T05-B															
Cu	EaFA-L11-1316-T01-C	1	13.511			1.35E+01	59.2357	3.7E+00	1.2E+01				---	VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1316-T02-C	1	20.422			2.04E+01	31.4759	3.7E+00	1.2E+01	10	325	3252.54	99%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1316-T03-C	1	19.268			1.93E+01	43.6449	3.7E+00	1.2E+01				---	VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1316-T04-C	1	31.556			3.16E+01	21.1697	3.7E+00	1.2E+01				---	VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
Cu	EaFA-L11-1316-T05-C															
Cu	EaFA-L11-1316-B01-A	1	1.85	U1/2		1.85E+00	102.361	3.7E+00	1.2E+01				---	VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	EaFA-L11-1316-T01-A	1	1	U1/2		1.00E+00	5.1016	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1316-T02-A	1	1	U1/2		1.00E+00	35.2947	2.0E+00	6.4E+00	1000	100	1016.18	102%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1316-T03-A	1	1	U1/2		1.00E+00	91.6685	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1316-T04-A	1	1	U1/2		1.00E+00	17.9276	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1316-T05-A															
Fe	EaFA-L11-1316-T01-B	1	1	U1/2		1.00E+00	25.9161	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1316-T02-B	1	1	U1/2		1.00E+00	31.8301	2.0E+00	6.4E+00	1000	100	1061.01	106%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1316-T03-B	1	1	U1/2		1.00E+00	22.9146	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1316-T04-B	1	1	U1/2		1.00E+00	44.3095	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1316-T05-B															
Fe	EaFA-L11-1316-T01-C	1	1	U1/2		1.00E+00	18.3098	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1316-T02-C	1	1	U1/2		1.00E+00	14.6757	2.0E+00	6.4E+00	1000	100	1027.36	103%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1316-T03-C	1	1	U1/2		1.00E+00	14.8727	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1316-T04-C	1	1	U1/2		1.00E+00	13.1303	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
Fe	EaFA-L11-1316-T05-C															
Fe	EaFA-L11-1316-B01-A	1	1	U1/2		1.00E+00	12.8135	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	EaFA-L11-1316-T01-A	1	3.4	U1/2		3.40E+00	1062.85	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1316-T02-A	1	3.4	U1/2		3.40E+00	40.6074	6.8E+00	2.2E+01	10	325	3131.4	96%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1316-T03-A	1	3.4	U1/2		3.40E+00	226.672	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1316-T04-A	1	3.4	U1/2		3.40E+00	152.099	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1316-T05-A															
Pb	EaFA-L11-1316-T01-B	1	3.4	U1/2		3.40E+00	91.4065	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1316-T02-B	1	3.4	U1/2		3.40E+00	33.8529	6.8E+00	2.2E+01	10	325	3290.75	101%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1316-T03-B	1	3.4	U1/2		3.40E+00	35.0406	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1316-T04-B	1	3.4	U1/2		3.40E+00	109.16	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1316-T05-B															
Pb	EaFA-L11-1316-T01-C	1	3.4	U1/2		3.40E+00	159.243	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1316-T02-C	1	3.4	U1/2		3.40E+00	22.4408	6.8E+00	2.2E+01	10	325	3177.38	98%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1316-T03-C	1	3.4	U1/2		3.40E+00	88.4961	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1316-T04-C	1	3.4	U1/2		3.40E+00	83.9348	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
Pb	EaFA-L11-1316-T05-C															
Pb	EaFA-L11-1316-B01-A	1	3.4	U1/2		3.40E+00	109.273	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	EaFA-L11-1316-T01-A	1	3483.77			3.48E+03	0.532814	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1316-T02-A	1	6878.42			6.88E+03	0.245674	1.9E+00	6.0E+00	10	325	9667.47	86%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1316-T03-A	1	14764.5			1.48E+04	0.919607	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1316-T04-A	1	32904			3.29E+04	0.87682	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1316-T05-A															
Li	EaFA-L11-1316-T01-B	1	3492.27			3.49E+03	0.99103	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1316-T02-B	1	6870.36			6.87E+03	1.1849	1.9E+00	6.0E+00	10	325	9692.7	87%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1316-T03-B	1	14794.6			1.48E+04	0.588684	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1316-T04-B	1	33121			3.31E+04	0.08216	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1316-T05-B															
Li	EaFA-L11-1316-T01-C	1	3471.65			3.47E+03	0.921124	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1316-T02-C	1	6879.09			6.88E+03	0.720342	1.9E+00	6.0E+00	10	325	9629.37	85%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1316-T03-C	1	15044.3			1.50E+04	0.820499	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1316-T04-C	1	34172.4			3.42E+04	0.347893	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
Li	EaFA-L11-1316-T05-C															
Li	EaFA-L11-1316-B01-A	1	0.95	U1/2		9.50E-01	23.1718	1.9E+00	6.0E+00			---		VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	EaFA-L11-1316-T01-A	1	30.205			3.02E+01	1.10517	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1316-T02-A	1	52.644			5.26E+01	0.785902	2.0E+00	6.4E+00	10	325	3239.84	98%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1316-T03-A	1	116.742			1.17E+02	0.900684	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1316-T04-A	1	900.11			9.00E+02	0.737251	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1316-T05-A															
Mn	EaFA-L11-1316-T01-B	1	29.593			2.96E+01	0.573992	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1316-T02-B	1	49.673			4.97E+01	1.00997	2.0E+00	6.4E+00	10	325	3376.98	102%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1316-T03-B	1	100.923			1.01E+02	0.599695	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1316-T04-B	1	1619.74			1.62E+03	2.0561	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1316-T05-B															
Mn	EaFA-L11-1316-T01-C	1	30.287			3.03E+01	1.24741	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1316-T02-C	1	54.84			5.48E+01	1.24385	2.0E+00	6.4E+00	10	325	3281.71	99%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1316-T03-C	1	108.692			1.09E+02	0.711228	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1316-T04-C	1	1679.77			1.68E+03	0.629526	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
Mn	EaFA-L11-1316-T05-C															
Mn	EaFA-L11-1316-B01-A	1	1	U1/2		1.00E+00	13.738	2.0E+00	6.4E+00			---		VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	EaFA-L11-1316-T01-A	1	6005.59			6.01E+03	0.905157	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1316-T02-A	1	11761.2			1.18E+04	0.371251	1.0E+00	3.2E+00	1000	100	12754.2	99%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1316-T03-A	1	28894.9			2.89E+04	1.31276	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1316-T04-A	1	63924.1			6.39E+04	1.11193	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1316-T05-A															
Mg	EaFA-L11-1316-T01-B	1	5967.54			5.97E+03	1.46837	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1316-T02-B	1	11710.1			1.17E+04	1.27192	1.0E+00	3.2E+00	1000	100	12734.9	102%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1316-T03-B	1	28594.4			2.86E+04	1.36425	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1316-T04-B	1	67183.6			6.72E+04	0.951056	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1316-T05-B															
Mg	EaFA-L11-1316-T01-C	1	5968.88			5.97E+03	1.07608	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1316-T02-C	1	11617.9			1.16E+04	1.46157	1.0E+00	3.2E+00	1000	100	12647.3	103%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1316-T03-C	1	29594.8			2.96E+04	0.228855	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1316-T04-C	1	69688.2			6.97E+04	0.523743	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
Mg	EaFA-L11-1316-T05-C															
Mg	EaFA-L11-1316-B01-A	1	0.5	U1/2		5.00E-01	14.5818	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	EaFA-L11-1316-T01-A	1	2677.58			2.68E+03	0.432666	1.2E+00	3.8E+00			---		VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1316-T02-A	1	5116.07			5.12E+03	1.46622	1.2E+00	3.8E+00	10	325	7983.54	88%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1316-T03-A	1	11515.9			1.15E+04	1.09509	1.2E+00	3.8E+00			---		VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1316-T04-A	1	21653.3			2.17E+04	0.5755	1.2E+00	3.8E+00			---		VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1316-T05-A															
Mo	EaFA-L11-1316-T01-B	1	2816.93			2.82E+03	0.062872	1.2E+00	3.8E+00			---		VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1316-T02-B	1	5197.22			5.20E+03	1.46151	1.2E+00	3.8E+00	10	325	8061.28	88%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1316-T03-B	1	11597.8			1.16E+04	0.507237	1.2E+00	3.8E+00			---		VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1316-T04-B	1	20431.3			2.04E+04	0.417057	1.2E+00	3.8E+00			---		VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1316-T05-B															
Mo	EaFA-L11-1316-T01-C	1	2803.08			2.80E+03	1.37263	1.2E+00	3.8E+00			---		VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1316-T02-C	1	5181.73			5.18E+03	0.840544	1.2E+00	3.8E+00	10	325	7961.2	86%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1316-T03-C	1	11569.7			1.16E+04	0.498529	1.2E+00	3.8E+00			---		VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1316-T04-C	1	21032.5			2.10E+04	0.744689	1.2E+00	3.8E+00			---		VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
Mo	EaFA-L11-1316-T05-C															
Mo	EaFA-L11-1316-B01-A	1	9.759			9.76E+00	25.4768	1.2E+00	3.8E+00			---		VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	EaFA-L11-1316-T01-A	1	10.807			1.08E+01	72.0127	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1316-T02-A	1	15.646			1.56E+01	26.2746	1.8E+00	5.7E+00	10	325	3217.63	99%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1316-T03-A	1	26.97			2.70E+01	36.0655	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1316-T04-A	1	202.668			2.03E+02	1.95336	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1316-T05-A															
Ni	EaFA-L11-1316-T01-B	1	6.997			7.00E+00	45.4502	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1316-T02-B	1	17.285			1.73E+01	39.7357	1.8E+00	5.7E+00	10	325	3350.16	103%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1316-T03-B	1	18.251			1.83E+01	25.3972	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1316-T04-B	1	377.999			3.78E+02	0.360396	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1316-T05-B															
Ni	EaFA-L11-1316-T01-C	1	10.651			1.07E+01	35.895	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1316-T02-C	1	16.361			1.64E+01	51.4675	1.8E+00	5.7E+00	10	325	3254.11	100%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1316-T03-C	1	25.52			2.55E+01	48.711	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1316-T04-C	1	391.17			3.91E+02	2.45553	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
Ni	EaFA-L11-1316-T05-C															
Ni	EaFA-L11-1316-B01-A	1	0.9	U1/2		9.00E-01	58.2892	1.8E+00	5.7E+00			---		VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	EaFA-L11-1316-T01-A	1	39.875			3.99E+01	21.0545	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1316-T02-A	1	72.195			7.22E+01	16.0896	3.7E+00	1.2E+01	1000	100	1123.95	105%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1316-T03-A	1	240.966			2.41E+02	5.55384	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1316-T04-A	1	290.667			2.91E+02	5.37928	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1316-T05-A															
P	EaFA-L11-1316-T01-B	1	75.116			7.51E+01	11.5102	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1316-T02-B	1	73.964			7.40E+01	11.9926	3.7E+00	1.2E+01	1000	100	1193.72	112%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1316-T03-B	1	219.135			2.19E+02	5.45495	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1316-T04-B	1	150.576			1.51E+02	7.43081	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1316-T05-B															
P	EaFA-L11-1316-T01-C	1	62.831			6.28E+01	13.3311	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1316-T02-C	1	79.962			8.00E+01	13.9011	3.7E+00	1.2E+01	1000	100	1145.26	107%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1316-T03-C	1	272.014			2.72E+02	5.47372	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1316-T04-C	1	155.42			1.55E+02	9.14687	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
P	EaFA-L11-1316-T05-C															
P	EaFA-L11-1316-B01-A	1	12.85			1.29E+01	71.2321	3.7E+00	1.2E+01			---		VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	EaFA-L11-1316-T01-A	1	14030			1.40E+04	0.616861	1.6E+00	5.1E+00			---		VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1316-T02-A	1	27712.2			2.77E+04	1.43628	1.6E+00	5.1E+00	1000	100	28615	90%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1316-T03-A	1	68777.1			6.88E+04	0.627447	1.6E+00	5.1E+00			---		VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1316-T04-A	1	183468			1.83E+05	0.628656	1.6E+00	5.1E+00			---		VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1316-T05-A															
K	EaFA-L11-1316-T01-B	1	14057.5			1.41E+04	0.569827	1.6E+00	5.1E+00			---		VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1316-T02-B	1	27631.6			2.76E+04	1.02545	1.6E+00	5.1E+00	1000	100	28542.8	91%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1316-T03-B	1	68494.6			6.85E+04	0.328139	1.6E+00	5.1E+00			---		VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1316-T04-B	1	206413			2.06E+05	0.114094	1.6E+00	5.1E+00			---		VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1316-T05-B															
K	EaFA-L11-1316-T01-C	1	13991.3			1.40E+04	0.943113	1.6E+00	5.1E+00			---		VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1316-T02-C	1	28188.2			2.82E+04	1.6639	1.6E+00	5.1E+00	1000	100	29047.5	86%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1316-T03-C	1	68927.3			6.89E+04	0.631062	1.6E+00	5.1E+00			---		VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1316-T04-C	1	212627			2.13E+05	0.410507	1.6E+00	5.1E+00			---		VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
K	EaFA-L11-1316-T05-C															
K	EaFA-L11-1316-B01-A	1	37.975			3.80E+01	4.77753	1.6E+00	5.1E+00			---		VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	EaFA-L11-1316-T01-A	1	1008.61			1.01E+03	3.13533	1.5E+01	4.8E+01			---		VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1316-T02-A	1	1214.31			1.21E+03	1.53033	1.5E+01	4.8E+01	10	325	4337.45	96%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1316-T03-A	1	1499.42			1.50E+03	2.90192	1.5E+01	4.8E+01			---		VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1316-T04-A	1	1475.26			1.48E+03	2.14462	1.5E+01	4.8E+01			---		VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1316-T05-A															
Se	EaFA-L11-1316-T01-B	1	1019.85			1.02E+03	4.10181	1.5E+01	4.8E+01			---		VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1316-T02-B	1	1153.53			1.15E+03	5.23526	1.5E+01	4.8E+01	10	325	4466.35	102%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1316-T03-B	1	1639.52			1.64E+03	3.64835	1.5E+01	4.8E+01			---		VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1316-T04-B	1	1377.46			1.38E+03	2.43762	1.5E+01	4.8E+01			---		VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1316-T05-B															
Se	EaFA-L11-1316-T01-C	1	967.964			9.68E+02	1.49279	1.5E+01	4.8E+01			---		VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1316-T02-C	1	1211.68			1.21E+03	2.96007	1.5E+01	4.8E+01	10	325	4366.12	97%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1316-T03-C	1	1562.42			1.56E+03	0.884472	1.5E+01	4.8E+01			---		VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1316-T04-C	1	1329.11			1.33E+03	2.51272	1.5E+01	4.8E+01			---		VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
Se	EaFA-L11-1316-T05-C															
Se	EaFA-L11-1316-B01-A	1	30.964	E		3.10E+01	64.9878	1.5E+01	4.8E+01			---		VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	EaFA-L11-1316-T01-A	1	612.515			6.13E+02	1.39283	1.1E+00	3.5E+00			---		VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1316-T02-A	1	699.255			6.99E+02	1.19497	1.1E+00	3.5E+00	1000	100	1660.62	96%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1316-T03-A	1	805.9			8.06E+02	0.968886	1.1E+00	3.5E+00			---		VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1316-T04-A	1	1567.81			1.57E+03	0.676624	1.1E+00	3.5E+00			---		VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1316-T05-A															
Si	EaFA-L11-1316-T01-B	1	639.274			6.39E+02	0.51867	1.1E+00	3.5E+00			---		VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1316-T02-B	1	708.053			7.08E+02	1.34987	1.1E+00	3.5E+00	1000	100	1702.76	99%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1316-T03-B	1	829.697			8.30E+02	0.656836	1.1E+00	3.5E+00			---		VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1316-T04-B	1	1951.18			1.95E+03	0.64659	1.1E+00	3.5E+00			---		VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1316-T05-B															
Si	EaFA-L11-1316-T01-C	1	649.866			6.50E+02	0.787813	1.1E+00	3.5E+00			---		VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1316-T02-C	1	673.42			6.73E+02	1.21528	1.1E+00	3.5E+00	1000	100	1652.09	98%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1316-T03-C	1	820.333			8.20E+02	0.349339	1.1E+00	3.5E+00			---		VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1316-T04-C	1	2023.59			2.02E+03	0.375631	1.1E+00	3.5E+00			---		VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
Si	EaFA-L11-1316-T05-C															
Si	EaFA-L11-1316-B01-A	1	0.55	U1/2		5.50E-01	52.0401	1.1E+00	3.5E+00			---		VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	EaFA-L11-1316-T01-A	1	4113.03			4.11E+03	0.934119	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1316-T02-A	1	8291.46			8.29E+03	0.430637	2.5E+00	8.0E+00	1000	100	9360.3	107%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1316-T03-A	1	21438.2			2.14E+04	1.2498	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1316-T04-A	1	40997.2			4.10E+04	0.526562	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1316-T05-A															
Na	EaFA-L11-1316-T01-B	1	4055.5			4.06E+03	1.19866	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1316-T02-B	1	8285.65			8.29E+03	1.21707	2.5E+00	8.0E+00	1000	100	9313.87	103%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1316-T03-B	1	21245.6			2.12E+04	0.131332	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1316-T04-B	1	41479.9			4.15E+04	0.382972	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1316-T05-B															
Na	EaFA-L11-1316-T01-C	1	4065.32			4.07E+03	0.817813	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1316-T02-C	1	8321.59			8.32E+03	1.38855	2.5E+00	8.0E+00	1000	100	9345.31	102%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1316-T03-C	1	21210			2.12E+04	0.953447	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1316-T04-C	1	42367.6			4.24E+04	1.62488	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
Na	EaFA-L11-1316-T05-C															
Na	EaFA-L11-1316-B01-A	1	23.097			2.31E+01	3.84468	2.5E+00	8.0E+00			---		VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	EaFA-L11-1316-T01-A	1	1820.32			1.82E+03	0.599407	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1316-T02-A	1	2919.57			2.92E+03	0.59003	1.0E+00	3.2E+00	1000	100	3838.34	92%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1316-T03-A	1	5376.77			5.38E+03	2.16434	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1316-T04-A	1	7264.32			7.26E+03	1.45962	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1316-T05-A															
Sr	EaFA-L11-1316-T01-B	1	1823.8			1.82E+03	0.962685	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1316-T02-B	1	2957.99			2.96E+03	0.535358	1.0E+00	3.2E+00	1000	100	3833.23	88%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1316-T03-B	1	5136.73			5.14E+03	0.454804	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1316-T04-B	1	8924.87			8.92E+03	1.99201	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1316-T05-B															
Sr	EaFA-L11-1316-T01-C	1	1830.9			1.83E+03	1.61228	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1316-T02-C	1	3061.46			3.06E+03	0.846235	1.0E+00	3.2E+00	1000	100	3949.91	89%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1316-T03-C	1	5306.19			5.31E+03	0.303608	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1316-T04-C	1	8995.52			9.00E+03	1.01228	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
Sr	EaFA-L11-1316-T05-C															
Sr	EaFA-L11-1316-B01-A	1	0.5	U1/2		5.00E-01	243275	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	EaFA-L11-1316-T01-A	1	143243			1.43E+05	0.144451	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1316-T02-A	1	281738			2.82E+05	0.972749	6.8E+00	2.2E+01	1000	100	372228	90%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1316-T03-A	1	668728			6.69E+05	0.745685	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1316-T04-A	1	765992			7.66E+05	0.456406	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1316-T05-A															
S	EaFA-L11-1316-T01-B	1	143722			1.44E+05	0.438072	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1316-T02-B	1	284299			2.84E+05	1.40204	6.8E+00	2.2E+01	1000	100	370352	86%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1316-T03-B	1	667913			6.68E+05	0.254033	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1316-T04-B	1	773385			7.73E+05	0.465961	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1316-T05-B															
S	EaFA-L11-1316-T01-C	1	143410			1.43E+05	0.801036	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1316-T02-C	1	287660			2.88E+05	1.49908	6.8E+00	2.2E+01	1000	100	370898	83%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1316-T03-C	1	675917			6.76E+05	0.486994	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1316-T04-C	1	797883			7.98E+05	0.429076	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
S	EaFA-L11-1316-T05-C															
S	EaFA-L11-1316-B01-A	1	11.06	E		1.11E+01	61.779	6.8E+00	2.2E+01			---		VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	EaFA-L11-1316-T01-A	1	2.3	U1/2		2.30E+00	89.0619	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1316-T02-A	1	2.3	U1/2		2.30E+00	879.407	4.6E+00	1.5E+01	10	325	3161.97	97%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1316-T03-A	1	2.3	U1/2		2.30E+00	2850.49	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1316-T04-A	1	13.765	E		1.38E+01	85.7597	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1316-T05-A															
Tl	EaFA-L11-1316-T01-B	1	2.3	U1/2		2.30E+00	92.0115	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1316-T02-B	1	2.3	U1/2		2.30E+00	94.9131	4.6E+00	1.5E+01	10	325	3288.18	101%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1316-T03-B	1	2.3	U1/2		2.30E+00	135.882	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1316-T04-B	1	22.262			2.23E+01	77.045	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1316-T05-B															
Tl	EaFA-L11-1316-T01-C	1	2.3	U1/2		2.30E+00	193.718	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1316-T02-C	1	2.3	U1/2		2.30E+00	253.176	4.6E+00	1.5E+01	10	325	3171.36	98%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1316-T03-C	1	2.3	U1/2		2.30E+00	260.484	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1316-T04-C	1	21.055			2.11E+01	70.2968	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
Tl	EaFA-L11-1316-T05-C															
Tl	EaFA-L11-1316-B01-A	1	2.3	U1/2		2.30E+00	57.1781	4.6E+00	1.5E+01			---		VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	EaFA-L11-1316-T01-A	1	1	U1/2		1.00E+00	41.819	2.0E+00	6.4E+00				---	VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1316-T02-A	1	1	U1/2		1.00E+00	10.2312	2.0E+00	6.4E+00	10	325	3189.15	98%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1316-T03-A	1	1	U1/2		1.00E+00	96.0468	2.0E+00	6.4E+00				---	VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1316-T04-A	1	1	U1/2		1.00E+00	29.3904	2.0E+00	6.4E+00				---	VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1316-T05-A															
Ti	EaFA-L11-1316-T01-B	1	1	U1/2		1.00E+00	41.3342	2.0E+00	6.4E+00				---	VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1316-T02-B	1	1	U1/2		1.00E+00	190.868	2.0E+00	6.4E+00	10	325	3319.15	102%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1316-T03-B	1	1	U1/2		1.00E+00	103.337	2.0E+00	6.4E+00				---	VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1316-T04-B	1	1	U1/2		1.00E+00	59.0268	2.0E+00	6.4E+00				---	VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1316-T05-B															
Ti	EaFA-L11-1316-T01-C	1	1	U1/2		1.00E+00	97.7126	2.0E+00	6.4E+00				---	VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1316-T02-C	1	1	U1/2		1.00E+00	182.226	2.0E+00	6.4E+00	10	325	3212.52	99%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1316-T03-C	1	1	U1/2		1.00E+00	81.0124	2.0E+00	6.4E+00				---	VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1316-T04-C	1	1	U1/2		1.00E+00	70.8312	2.0E+00	6.4E+00				---	VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
Ti	EaFA-L11-1316-T05-C															
Ti	EaFA-L11-1316-B01-A	1	1	U1/2		1.00E+00	772.29	2.0E+00	6.4E+00				---	VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	EaFA-L11-1316-T01-A	1	142.54			1.43E+02	1.84977	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1316-T02-A	1	162.163			1.62E+02	4.0324	1.5E+00	4.8E+00	10	325	3277.3	96%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1316-T03-A	1	220.4			2.20E+02	3.25198	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1316-T04-A	1	223.503			2.24E+02	1.88814	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1316-T05-A															
V	EaFA-L11-1316-T01-B	1	147.851			1.48E+02	1.19955	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1316-T02-B	1	152.771			1.53E+02	2.60016	1.5E+00	4.8E+00	10	325	3410.2	100%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1316-T03-B	1	214.3			2.14E+02	1.92128	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1316-T04-B	1	227.141			2.27E+02	1.06881	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1316-T05-B															
V	EaFA-L11-1316-T01-C	1	138.055			1.38E+02	1.85939	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1316-T02-C	1	161.53			1.62E+02	1.81809	1.5E+00	4.8E+00	10	325	3322.65	97%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1316-T03-C	1	212.163			2.12E+02	1.04353	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1316-T04-C	1	229.91			2.30E+02	0.201894	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
V	EaFA-L11-1316-T05-C															
V	EaFA-L11-1316-B01-A	1	4.673	E		4.67E+00	21.8858	1.5E+00	4.8E+00			---		VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	EaFA-L11-1316-T01-A	1	5.272			5.27E+00	6.45146	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:10 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1316-T02-A	1	2.295 E			2.30E+00	7.16154	1.0E+00	3.2E+00	10	325	3245.5	100%	VU ICP-OES	2/22/11 3:12 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1316-T03-A	1	5.802			5.80E+00	20.4762	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:13 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1316-T04-A	1	15.268			1.53E+01	8.43378	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:15 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1316-T05-A															
Zn	EaFA-L11-1316-T01-B	1	5.37			5.37E+00	30.1232	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:17 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1316-T02-B	1	4.694			4.69E+00	34.7608	1.0E+00	3.2E+00	10	325	3371.72	104%	VU ICP-OES	2/22/11 3:18 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1316-T03-B	1	6.974			6.97E+00	56.6351	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:20 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1316-T04-B	1	26.204			2.62E+01	5.7933	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:22 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1316-T05-B															
Zn	EaFA-L11-1316-T01-C	1	3.765			3.77E+00	21.375	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:23 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1316-T02-C	1	2.091 E			2.09E+00	26.0894	1.0E+00	3.2E+00	10	325	3269.32	101%	VU ICP-OES	2/22/11 3:25 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1316-T03-C	1	6.366			6.37E+00	6.27961	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:27 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1316-T04-C	1	19.05			1.91E+01	0.658378	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:28 PM	EPA Interlab L11 1313-1316 EaFA
Zn	EaFA-L11-1316-T05-C															
Zn	EaFA-L11-1316-B01-A	1	0.5	U1/2		5.00E-01	64.2724	1.0E+00	3.2E+00			---		VU ICP-OES	2/22/11 3:08 PM	EPA Interlab L11 1313-1316 EaFA

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	EaFA-LRef-1316-T01-A	1	2.02E+02			2.02E+02	3.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1316-T02-A	1	1.86E+02			1.86E+02	8.1E-02	1.0E+00	3.2E+00	1000	100	1.03E+03	84%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1316-T03-A	1	2.79E+02			2.79E+02	5.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1316-T04-A	1	4.31E+02			4.31E+02	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1316-T05-A															
Al	EaFA-LRef-1316-T01-B	1	2.24E+02			2.24E+02	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1316-T02-B	1	1.91E+02			1.91E+02	1.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1316-T03-B	1	2.93E+02			2.93E+02	5.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1316-T04-B	1	4.43E+02			4.43E+02	2.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1316-T05-B															
Al	EaFA-LRef-1316-T01-C	1	2.60E+02			2.60E+02	1.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1316-T02-C	1	1.83E+02			1.83E+02	2.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1316-T03-C	1	2.74E+02			2.74E+02	1.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1316-T04-C	1	4.34E+02			4.34E+02	2.4E+00	1.0E+00	3.2E+00			---		VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Al	EaFA-LRef-1316-T05-C															

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	EaFA-LRef-1316-T01-A	1	1.48E+02			1.48E+02	2.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1316-T02-A	1	4.20E+02			4.20E+02	7.6E+00	7.5E+00	2.4E+01	10	325	3.53E+03	96%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1316-T03-A	1	5.03E+02			5.03E+02	1.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1316-T04-A	1	7.41E+02			7.41E+02	5.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1316-T05-A															
Sb	EaFA-LRef-1316-T01-B	1	1.28E+02			1.28E+02	7.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1316-T02-B	1	4.72E+02			4.72E+02	6.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1316-T03-B	1	5.40E+02			5.40E+02	7.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1316-T04-B	1	6.87E+02			6.87E+02	1.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1316-T05-B															
Sb	EaFA-LRef-1316-T01-C	1	1.17E+02			1.17E+02	2.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1316-T02-C	1	3.63E+02			3.63E+02	9.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1316-T03-C	1	5.00E+02			5.00E+02	9.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1316-T04-C	1	6.81E+02			6.81E+02	7.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Sb	EaFA-LRef-1316-T05-C															

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	EaFA-LRef-1316-T01-A	1	7.84E+01			7.84E+01	3.4E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1316-T02-A	1	1.72E+02			1.72E+02	1.3E+01	1.1E+01	3.5E+01	10	325	3.37E+03	98%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1316-T03-A	1	2.21E+02			2.21E+02	2.6E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1316-T04-A	1	1.86E+02			1.86E+02	1.1E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1316-T05-A															
As	EaFA-LRef-1316-T01-B	1	6.43E+01			6.43E+01	1.9E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1316-T02-B	1	1.80E+02			1.80E+02	2.9E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1316-T03-B	1	1.53E+02			1.53E+02	1.4E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1316-T04-B	1	2.13E+02			2.13E+02	7.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1316-T05-B															
As	EaFA-LRef-1316-T01-C	1	7.23E+01			7.23E+01	1.4E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1316-T02-C	1	1.73E+02			1.73E+02	2.7E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1316-T03-C	1	1.46E+02			1.46E+02	3.5E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1316-T04-C	1	1.82E+02			1.82E+02	2.2E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
As	EaFA-LRef-1316-T05-C															

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	EaFA-LRef-1316-T01-A	1	4.62E+03			4.62E+03	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1316-T02-A	1	8.16E+03			8.16E+03	1.4E+00	1.0E+00	3.2E+00	1000	100	9.05E+03	89%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1316-T03-A	1	1.82E+04			1.82E+04	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1316-T04-A	1	3.76E+04			3.76E+04	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1316-T05-A															
B	EaFA-LRef-1316-T01-B	1	4.47E+03			4.47E+03	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1316-T02-B	1	9.00E+03			9.00E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1316-T03-B	1	2.07E+04			2.07E+04	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1316-T04-B	1	3.43E+04			3.43E+04	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1316-T05-B															
B	EaFA-LRef-1316-T01-C	1	4.43E+03			4.43E+03	1.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1316-T02-C	1	7.93E+03			7.93E+03	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1316-T03-C	1	1.88E+04			1.88E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1316-T04-C	1	3.18E+04			3.18E+04	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
B	EaFA-LRef-1316-T05-C															

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	EaFA-LRef-1316-T01-A	1	2.60E+02			2.60E+02	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1316-T02-A	1	1.82E+02			1.82E+02	1.3E+00	1.0E+00	3.2E+00	10	325	3.22E+03	94%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1316-T03-A	1	1.95E+02			1.95E+02	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1316-T04-A	1	1.79E+02			1.79E+02	9.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1316-T05-A															
Ba	EaFA-LRef-1316-T01-B	1	2.46E+02			2.46E+02	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1316-T02-B	1	2.01E+02			2.01E+02	8.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1316-T03-B	1	2.01E+02			2.01E+02	2.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1316-T04-B	1	1.65E+02			1.65E+02	7.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1316-T05-B															
Ba	EaFA-LRef-1316-T01-C	1	2.44E+02			2.44E+02	8.6E-02	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1316-T02-C	1	1.79E+02			1.79E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1316-T03-C	1	1.84E+02			1.84E+02	4.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1316-T04-C	1	1.61E+02			1.61E+02	2.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ba	EaFA-LRef-1316-T05-C															

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	EaFA-LRef-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	6.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	3.7E+02	1.9E+00	6.0E+00	10	325	3.11E+03	96%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	4.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1316-T05-A															
Be	EaFA-LRef-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	1.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	4.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1316-T05-B															
Be	EaFA-LRef-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	1.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	3.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	3.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	1.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Be	EaFA-LRef-1316-T05-C															

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	EaFA-LRef-1316-T01-A	1	1.10E+00	U1/2		1.10E+00	3.5E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1316-T02-A	1	1.10E+00	U1/2		1.10E+00	9.1E+01	2.2E+00	7.0E+00	10	325	3.62E+03	111%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1316-T03-A	1	4.67E+00	E		4.67E+00	3.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1316-T04-A	1	3.56E+00	E		3.56E+00	2.7E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1316-T05-A															
Cd	EaFA-LRef-1316-T01-B	1	1.10E+00	U1/2		1.10E+00	5.5E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1316-T02-B	1	3.38E+00	E		3.38E+00	2.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1316-T03-B	1	6.60E+00	E		6.60E+00	2.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1316-T04-B	1	1.10E+00	U1/2		1.10E+00	4.6E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1316-T05-B															
Cd	EaFA-LRef-1316-T01-C	1	1.10E+00	U1/2		1.10E+00	1.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1316-T02-C	1	1.10E+00	U1/2		1.10E+00	1.4E+03	2.2E+00	7.0E+00				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1316-T03-C	1	4.40E+00	E		4.40E+00	4.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1316-T04-C	1	1.10E+00	U1/2		1.10E+00	2.4E+02	2.2E+00	7.0E+00				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cd	EaFA-LRef-1316-T05-C															

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	EaFA-LRef-1316-T01-A	1	1.55E+05			1.55E+05	1.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1316-T02-A	1	2.94E+05			2.94E+05	1.5E-01	2.6E+00	8.3E+00	1000	100	2.95E+05	93%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1316-T03-A	1	6.45E+05			6.45E+05	6.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1316-T04-A	1	4.46E+05			4.46E+05	7.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1316-T05-A															
Ca	EaFA-LRef-1316-T01-B	1	1.47E+05			1.47E+05	6.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1316-T02-B	1	3.10E+05			3.10E+05	3.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1316-T03-B	1	7.30E+05			7.30E+05	6.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1316-T04-B	1	4.95E+05			4.95E+05	1.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1316-T05-B															
Ca	EaFA-LRef-1316-T01-C	1	1.41E+05			1.41E+05	3.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1316-T02-C	1	2.61E+05			2.61E+05	1.5E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1316-T03-C	1	6.49E+05			6.49E+05	4.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1316-T04-C	1	4.53E+05			4.53E+05	6.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ca	EaFA-LRef-1316-T05-C															

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	EaFA-LRef-1316-T01-A	1	4.22E+01			4.22E+01	2.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1316-T02-A	1	1.39E+01			1.39E+01	2.7E+01	1.2E+00	3.8E+00	10	325	3.61E+03	111%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1316-T03-A	1	1.60E+01			1.60E+01	2.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1316-T04-A	1	2.59E+01			2.59E+01	3.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1316-T05-A															
Cr	EaFA-LRef-1316-T01-B	1	5.43E+01			5.43E+01	3.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1316-T02-B	1	1.51E+01			1.51E+01	3.8E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1316-T03-B	1	1.93E+01			1.93E+01	6.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1316-T04-B	1	2.80E+01			2.80E+01	1.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1316-T05-B															
Cr	EaFA-LRef-1316-T01-C	1	6.01E+01			6.01E+01	2.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1316-T02-C	1	1.66E+01			1.66E+01	1.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1316-T03-C	1	1.97E+01			1.97E+01	3.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1316-T04-C	1	3.00E+01			3.00E+01	1.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cr	EaFA-LRef-1316-T05-C															

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	EaFA-LRef-1316-T01-A	1	2.93E+01			2.93E+01	3.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1316-T02-A	1	7.79E+01			7.79E+01	4.5E+00	1.8E+00	5.7E+00	10	325	3.68E+03	111%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1316-T03-A	1	1.81E+02			1.81E+02	2.4E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1316-T04-A	1	1.08E+02			1.08E+02	1.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1316-T05-A															
Co	EaFA-LRef-1316-T01-B	1	2.13E+01			2.13E+01	2.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1316-T02-B	1	9.63E+01			9.63E+01	5.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1316-T03-B	1	1.92E+02			1.92E+02	2.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1316-T04-B	1	1.14E+02			1.14E+02	1.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1316-T05-B															
Co	EaFA-LRef-1316-T01-C	1	2.03E+01			2.03E+01	1.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1316-T02-C	1	7.78E+01			7.78E+01	4.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1316-T03-C	1	1.87E+02			1.87E+02	4.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1316-T04-C	1	9.26E+01			9.26E+01	1.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Co	EaFA-LRef-1316-T05-C															

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	EaFA-LRef-1316-T01-A	1	1.85E+00	U1/2		1.85E+00	1.6E+02	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1316-T02-A	1	1.39E+01			1.39E+01	2.4E+01	3.7E+00	1.2E+01	10	325	3.65E+03	112%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1316-T03-A	1	2.07E+01			2.07E+01	1.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1316-T04-A	1	2.67E+01			2.67E+01	3.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1316-T05-A															
Cu	EaFA-LRef-1316-T01-B	1	3.85E+00	E		3.85E+00	1.3E+02	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1316-T02-B	1	1.60E+01			1.60E+01	4.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1316-T03-B	1	2.25E+01			2.25E+01	2.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1316-T04-B	1	2.62E+01			2.62E+01	4.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1316-T05-B															
Cu	EaFA-LRef-1316-T01-C	1	5.17E+00	E		5.17E+00	9.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1316-T02-C	1	2.37E+01			2.37E+01	1.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1316-T03-C	1	2.69E+01			2.69E+01	2.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1316-T04-C	1	3.34E+01			3.34E+01	9.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Cu	EaFA-LRef-1316-T05-C															

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	EaFA-LRef-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	5.7E+01	2.0E+00	6.4E+00	1000	100	1.09E+03	109%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	3.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	5.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1316-T05-A															
Fe	EaFA-LRef-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	7.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	5.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	5.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	1.8E+02	2.0E+00	6.4E+00				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1316-T05-B															
Fe	EaFA-LRef-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	5.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	6.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	5.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Fe	EaFA-LRef-1316-T05-C															

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	EaFA-LRef-1316-T01-A	1	3.40E+00	U1/2		3.40E+00	5.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1316-T02-A	1	3.40E+00	U1/2		3.40E+00	5.7E+00	6.8E+00	2.2E+01	10	325	3.23E+03	99%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1316-T03-A	1	3.40E+00	U1/2		3.40E+00	1.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1316-T04-A	1	3.40E+00	U1/2		3.40E+00	3.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1316-T05-A															
Pb	EaFA-LRef-1316-T01-B	1	3.40E+00	U1/2		3.40E+00	2.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1316-T02-B	1	3.40E+00	U1/2		3.40E+00	2.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1316-T03-B	1	3.40E+00	U1/2		3.40E+00	3.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1316-T04-B	1	3.40E+00	U1/2		3.40E+00	2.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1316-T05-B															
Pb	EaFA-LRef-1316-T01-C	1	3.40E+00	U1/2		3.40E+00	1.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1316-T02-C	1	3.40E+00	U1/2		3.40E+00	1.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1316-T03-C	1	3.40E+00	U1/2		3.40E+00	1.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1316-T04-C	1	3.40E+00	U1/2		3.40E+00	9.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Pb	EaFA-LRef-1316-T05-C															

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	EaFA-LRef-1316-T01-A	1	3.24E+03			3.24E+03	3.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1316-T02-A	1	6.70E+03			6.70E+03	1.1E+00	1.9E+00	6.0E+00	10	325	9.68E+03	92%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1316-T03-A	1	1.54E+04			1.54E+04	5.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1316-T04-A	1	3.36E+04			3.36E+04	5.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1316-T05-A															
Li	EaFA-LRef-1316-T01-B	1	3.06E+03			3.06E+03	2.9E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1316-T02-B	1	7.18E+03			7.18E+03	6.2E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1316-T03-B	1	1.74E+04			1.74E+04	3.9E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1316-T04-B	1	3.08E+04			3.08E+04	6.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1316-T05-B															
Li	EaFA-LRef-1316-T01-C	1	2.98E+03			2.98E+03	3.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1316-T02-C	1	6.00E+03			6.00E+03	8.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1316-T03-C	1	1.56E+04			1.56E+04	3.6E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1316-T04-C	1	2.84E+04			2.84E+04	4.0E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Li	EaFA-LRef-1316-T05-C															

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	EaFA-LRef-1316-T01-A	1	2.68E+02			2.68E+02	5.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1316-T02-A	1	6.83E+02			6.83E+02	8.3E-01	2.0E+00	6.4E+00	10	325	4.36E+03	113%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1316-T03-A	1	1.50E+03			1.50E+03	6.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1316-T04-A	1	1.62E+03			1.62E+03	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1316-T05-A															
Mn	EaFA-LRef-1316-T01-B	1	2.19E+02			2.19E+02	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1316-T02-B	1	7.69E+02			7.69E+02	3.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1316-T03-B	1	1.46E+03			1.46E+03	1.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1316-T04-B	1	1.67E+03			1.67E+03	7.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1316-T05-B															
Mn	EaFA-LRef-1316-T01-C	1	1.93E+02			1.93E+02	1.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1316-T02-C	1	6.15E+02			6.15E+02	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1316-T03-C	1	1.45E+03			1.45E+03	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1316-T04-C	1	1.53E+03			1.53E+03	7.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mn	EaFA-LRef-1316-T05-C															

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	EaFA-LRef-1316-T01-A	1	7.49E+03			7.49E+03	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1316-T02-A	1	1.29E+04			1.29E+04	1.9E+00	1.0E+00	3.2E+00	1000	100	1.38E+04	98%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1316-T03-A	1	3.06E+04			3.06E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1316-T04-A	1	5.44E+04			5.44E+04	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1316-T05-A															
Mg	EaFA-LRef-1316-T01-B	1	7.03E+03			7.03E+03	8.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1316-T02-B	1	1.39E+04			1.39E+04	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1316-T03-B	1	3.47E+04			3.47E+04	2.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1316-T04-B	1	5.79E+04			5.79E+04	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1316-T05-B															
Mg	EaFA-LRef-1316-T01-C	1	7.04E+03			7.04E+03	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1316-T02-C	1	1.17E+04			1.17E+04	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1316-T03-C	1	3.08E+04			3.08E+04	3.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1316-T04-C	1	5.30E+04			5.30E+04	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mg	EaFA-LRef-1316-T05-C															

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	EaFA-LRef-1316-T01-A	1	3.32E+03			3.32E+03	4.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1316-T02-A	1	6.37E+03			6.37E+03	7.0E-01	1.2E+00	3.8E+00	10	325	9.31E+03	91%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1316-T03-A	1	1.30E+04			1.30E+04	3.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1316-T04-A	1	2.76E+04			2.76E+04	1.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1316-T05-A															
Mo	EaFA-LRef-1316-T01-B	1	3.20E+03			3.20E+03	6.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1316-T02-B	1	6.76E+03			6.76E+03	4.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1316-T03-B	1	1.46E+04			1.46E+04	1.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1316-T04-B	1	2.63E+04			2.63E+04	5.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1316-T05-B															
Mo	EaFA-LRef-1316-T01-C	1	3.17E+03			3.17E+03	6.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1316-T02-C	1	5.73E+03			5.73E+03	1.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1316-T03-C	1	1.32E+04			1.32E+04	3.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1316-T04-C	1	2.43E+04			2.43E+04	7.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Mo	EaFA-LRef-1316-T05-C															

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	EaFA-LRef-1316-T01-A	1	6.46E+01			6.46E+01	2.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1316-T02-A	1	1.86E+02			1.86E+02	5.3E+00	1.8E+00	5.7E+00	10	325	3.80E+03	111%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1316-T03-A	1	4.29E+02			4.29E+02	1.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1316-T04-A	1	3.51E+02			3.51E+02	3.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1316-T05-A															
Ni	EaFA-LRef-1316-T01-B	1	5.05E+01			5.05E+01	3.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1316-T02-B	1	2.19E+02			2.19E+02	5.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1316-T03-B	1	4.18E+02			4.18E+02	1.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1316-T04-B	1	2.67E+02			2.67E+02	4.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1316-T05-B															
Ni	EaFA-LRef-1316-T01-C	1	4.37E+01			4.37E+01	2.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1316-T02-C	1	1.70E+02			1.70E+02	4.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1316-T03-C	1	4.30E+02			4.30E+02	1.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1316-T04-C	1	3.04E+02			3.04E+02	3.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ni	EaFA-LRef-1316-T05-C															

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	EaFA-LRef-1316-T01-A	1	1.63E+01			1.63E+01	4.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1316-T02-A	1	4.13E+01			4.13E+01	5.1E+01	3.7E+00	1.2E+01	1000	100	1.00E+03	96%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1316-T03-A	1	5.71E+01			5.71E+01	1.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1316-T04-A	1	6.17E+01			6.17E+01	7.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1316-T05-A															
P	EaFA-LRef-1316-T01-B	1	2.66E+01			2.66E+01	8.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1316-T02-B	1	3.14E+01			3.14E+01	1.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1316-T03-B	1	5.25E+01			5.25E+01	3.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1316-T04-B	1	5.58E+01			5.58E+01	3.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1316-T05-B															
P	EaFA-LRef-1316-T01-C	1	1.93E+01			1.93E+01	1.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1316-T02-C	1	4.27E+01			4.27E+01	4.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1316-T03-C	1	5.41E+01			5.41E+01	2.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1316-T04-C	1	6.35E+01			6.35E+01	1.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
P	EaFA-LRef-1316-T05-C															

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	EaFA-LRef-1316-T01-A	1	2.50E+04			2.50E+04	6.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1316-T02-A	1	4.28E+04			4.28E+04	7.2E-01	1.6E+00	5.1E+00	1000	100	4.38E+04	91%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1316-T03-A	1	1.04E+05			1.04E+05	5.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1316-T04-A	1	2.02E+05			2.02E+05	6.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1316-T05-A															
K	EaFA-LRef-1316-T01-B	1	2.33E+04			2.33E+04	5.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1316-T02-B	1	4.63E+04			4.63E+04	1.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1316-T03-B	1	1.18E+05			1.18E+05	1.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1316-T04-B	1	1.85E+05			1.85E+05	5.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1316-T05-B															
K	EaFA-LRef-1316-T01-C	1	2.28E+04			2.28E+04	8.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1316-T02-C	1	3.84E+04			3.84E+04	1.5E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1316-T03-C	1	1.06E+05			1.06E+05	8.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1316-T04-C	1	1.71E+05			1.71E+05	3.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
K	EaFA-LRef-1316-T05-C															

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	EaFA-LRef-1316-T01-A	1	9.22E+02			9.22E+02	5.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1316-T02-A	1	1.24E+03			1.24E+03	5.5E+00	1.5E+01	4.8E+01	10	325	4.08E+03	87%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1316-T03-A	1	1.40E+03			1.40E+03	3.0E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1316-T04-A	1	1.78E+03			1.78E+03	1.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1316-T05-A															
Se	EaFA-LRef-1316-T01-B	1	8.42E+02			8.42E+02	1.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1316-T02-B	1	1.42E+03			1.42E+03	1.6E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1316-T03-B	1	1.50E+03			1.50E+03	1.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1316-T04-B	1	1.71E+03			1.71E+03	2.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1316-T05-B															
Se	EaFA-LRef-1316-T01-C	1	9.26E+02			9.26E+02	5.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1316-T02-C	1	1.18E+03			1.18E+03	5.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1316-T03-C	1	1.27E+03			1.27E+03	8.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1316-T04-C	1	1.54E+03			1.54E+03	2.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Se	EaFA-LRef-1316-T05-C															

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	EaFA-LRef-1316-T01-A	1	1.43E+03			1.43E+03	2.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1316-T02-A	1	2.69E+03			2.69E+03	9.4E-01	1.1E+00	3.5E+00	1000	100	3.72E+03	103%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1316-T03-A	1	2.79E+03			2.79E+03	9.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1316-T04-A	1	2.62E+03			2.62E+03	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1316-T05-A															
Si	EaFA-LRef-1316-T01-B	1	1.20E+03			1.20E+03	1.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1316-T02-B	1	2.24E+03			2.24E+03	7.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1316-T03-B	1	2.31E+03			2.31E+03	3.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1316-T04-B	1	2.19E+03			2.19E+03	5.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1316-T05-B															
Si	EaFA-LRef-1316-T01-C	1	1.24E+03			1.24E+03	4.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1316-T02-C	1	2.52E+03			2.52E+03	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1316-T03-C	1	2.75E+03			2.75E+03	2.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1316-T04-C	1	1.91E+03			1.91E+03	3.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Si	EaFA-LRef-1316-T05-C															

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	EaFA-LRef-1316-T01-A	1	6.45E+03			6.45E+03	3.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1316-T02-A	1	1.13E+04			1.13E+04	7.0E-01	2.5E+00	8.0E+00	1000	100	1.22E+04	94%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1316-T03-A	1	2.82E+04			2.82E+04	7.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1316-T04-A	1	5.99E+04			5.99E+04	1.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1316-T05-A															
Na	EaFA-LRef-1316-T01-B	1	6.03E+03			6.03E+03	4.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1316-T02-B	1	1.22E+04			1.22E+04	3.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1316-T03-B	1	3.22E+04			3.22E+04	2.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1316-T04-B	1	5.49E+04			5.49E+04	1.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1316-T05-B															
Na	EaFA-LRef-1316-T01-C	1	5.95E+03			5.95E+03	1.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1316-T02-C	1	1.01E+04			1.01E+04	9.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1316-T03-C	1	2.88E+04			2.88E+04	2.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1316-T04-C	1	5.03E+04			5.03E+04	7.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Na	EaFA-LRef-1316-T05-C															

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	EaFA-LRef-1316-T01-A	1	2.54E+03			2.54E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1316-T02-A	1	3.69E+03			3.69E+03	5.7E-01	1.0E+00	3.2E+00	1000	100	4.70E+03	102%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1316-T03-A	1	7.22E+03			7.22E+03	3.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1316-T04-A	1	6.74E+03			6.74E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1316-T05-A															
Sr	EaFA-LRef-1316-T01-B	1	2.42E+03			2.42E+03	8.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1316-T02-B	1	3.96E+03			3.96E+03	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1316-T03-B	1	8.22E+03			8.22E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1316-T04-B	1	7.19E+03			7.19E+03	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1316-T05-B															
Sr	EaFA-LRef-1316-T01-C	1	2.38E+03			2.38E+03	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1316-T02-C	1	3.44E+03			3.44E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1316-T03-C	1	7.33E+03			7.33E+03	9.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1316-T04-C	1	6.63E+03			6.63E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Sr	EaFA-LRef-1316-T05-C															

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	EaFA-LRef-1316-T01-A	1	1.64E+05			1.64E+05	8.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1316-T02-A	1	3.09E+05			3.09E+05	1.2E+00	6.8E+00	2.2E+01	1000	100	3.10E+05	99%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1316-T03-A	1	6.84E+05			6.84E+05	2.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1316-T04-A	1	7.73E+05			7.73E+05	9.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1316-T05-A															
S	EaFA-LRef-1316-T01-B	1	1.58E+05			1.58E+05	3.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1316-T02-B	1	3.30E+05			3.30E+05	4.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1316-T03-B	1	7.27E+05			7.27E+05	1.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1316-T04-B	1	7.05E+05			7.05E+05	9.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1316-T05-B															
S	EaFA-LRef-1316-T01-C	1	1.60E+05			1.60E+05	2.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1316-T02-C	1	2.74E+05			2.74E+05	1.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1316-T03-C	1	6.89E+05			6.89E+05	1.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1316-T04-C	1	7.43E+05			7.43E+05	3.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
S	EaFA-LRef-1316-T05-C															

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	EaFA-LRef-1316-T01-A	1	2.30E+00	U1/2		2.30E+00	4.1E+01	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1316-T02-A	1	2.30E+00	U1/2		2.30E+00	1.4E+01	4.6E+00	1.5E+01	10	325	3.36E+03	103%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1316-T03-A	1	2.30E+00	U1/2		2.30E+00	9.3E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1316-T04-A	1	2.30E+00	U1/2		2.30E+00	2.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1316-T05-A															
Tl	EaFA-LRef-1316-T01-B	1	2.30E+00	U1/2		2.30E+00	6.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1316-T02-B	1	2.30E+00	U1/2		2.30E+00	1.8E+01	4.6E+00	1.5E+01				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1316-T03-B	1	2.30E+00	U1/2		2.30E+00	7.5E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1316-T04-B	1	2.30E+00	U1/2		2.30E+00	8.0E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1316-T05-B															
Tl	EaFA-LRef-1316-T01-C	1	2.30E+00	U1/2		2.30E+00	1.7E+02	4.6E+00	1.5E+01				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1316-T02-C	1	2.30E+00	U1/2		2.30E+00	8.8E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1316-T03-C	1	2.30E+00	U1/2		2.30E+00	1.5E+01	4.6E+00	1.5E+01				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1316-T04-C	1	2.30E+00	U1/2		2.30E+00	5.0E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Tl	EaFA-LRef-1316-T05-C															

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	EaFA-LRef-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	1.9E+03	2.0E+00	6.4E+00	10	325	3.62E+03	111%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	3.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	1.5E+02	2.0E+00	6.4E+00				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1316-T05-A															
Ti	EaFA-LRef-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	6.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	4.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	1.5E+02	2.0E+00	6.4E+00				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1316-T05-B															
Ti	EaFA-LRef-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	1.8E+03	2.0E+00	6.4E+00				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Ti	EaFA-LRef-1316-T05-C															

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	EaFA-LRef-1316-T01-A	1	1.58E+02			1.58E+02	2.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1316-T02-A	1	3.16E+02			3.16E+02	1.9E+00	1.5E+00	4.8E+00	10	325	3.93E+03	111%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1316-T03-A	1	3.47E+02			3.47E+02	1.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1316-T04-A	1	4.01E+02			4.01E+02	1.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1316-T05-A															
V	EaFA-LRef-1316-T01-B	1	1.50E+02			1.50E+02	4.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1316-T02-B	1	3.32E+02			3.32E+02	3.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1316-T03-B	1	3.46E+02			3.46E+02	2.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1316-T04-B	1	3.65E+02			3.65E+02	1.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1316-T05-B															
V	EaFA-LRef-1316-T01-C	1	1.57E+02			1.57E+02	3.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1316-T02-C	1	2.85E+02			2.85E+02	9.4E-01	1.5E+00	4.8E+00				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1316-T03-C	1	3.32E+02			3.32E+02	3.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1316-T04-C	1	3.91E+02			3.91E+02	1.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
V	EaFA-LRef-1316-T05-C															

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	EaFA-LRef-1316-T01-A	1	5.00E-01	U1/2		5.00E-01	2.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:26 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1316-T02-A	1	2.20E+01			2.20E+01	4.6E+00	1.0E+00	3.2E+00	10	325	3.70E+03	113%	VU ICP-OES	5/7/10 3:41 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1316-T03-A	1	9.71E+01			9.71E+01	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:43 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1316-T04-A	1	9.23E+01			9.23E+01	2.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:45 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1316-T05-A															
Zn	EaFA-LRef-1316-T01-B	1	5.00E-01	U1/2		5.00E-01	3.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 8:49 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1316-T02-B	1	4.29E+01			4.29E+01	7.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:46 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1316-T03-B	1	6.89E+01			6.89E+01	7.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:48 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1316-T04-B	1	1.24E+02			1.24E+02	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:50 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1316-T05-B															
Zn	EaFA-LRef-1316-T01-C	1	5.00E-01	U1/2		5.00E-01	9.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/6/10 9:13 AM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1316-T02-C	1	2.50E+01			2.50E+01	9.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:51 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1316-T03-C	1	8.25E+01			8.25E+01	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:53 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1316-T04-C	1	1.12E+02			1.12E+02	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/7/10 3:54 PM	EPA Interlab LRef A-C 1313-1316 EaFA
Zn	EaFA-LRef-1316-T05-C															

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	EaFA-LRef-1316-T01-D	1	1.28E+02			1.28E+02	1.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1316-T02-D	1	1.91E+02			1.91E+02	3.8E+00	1.0E+00	3.2E+00	1000	100	1.18E+03	99%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1316-T03-D	1	2.32E+02			2.32E+02	2.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1316-T04-D	1	4.29E+02			4.29E+02	8.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1316-T05-D															
Al	EaFA-LRef-1316-T01-E	1	1.28E+02			1.28E+02	3.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1316-T02-E	1	1.82E+02			1.82E+02	2.4E+00	1.0E+00	3.2E+00	1000	100	1.19E+03	101%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1316-T03-E	1	2.14E+02			2.14E+02	4.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1316-T04-E	1	4.31E+02			4.31E+02	4.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1316-T05-E															
Al	EaFA-LRef-1316-T01-F	1	1.31E+02			1.31E+02	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1316-T02-F	1	1.92E+02			1.92E+02	2.7E+00	1.0E+00	3.2E+00	1000	100	1.16E+03	97%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1316-T03-F	1	2.31E+02			2.31E+02	1.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1316-T04-F	1	4.07E+02			4.07E+02	1.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Al	EaFA-LRef-1316-T05-F															

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	EaFA-LRef-1316-T01-D	1	1.82E+02			1.82E+02	1.5E+01	7.5E+00	2.4E+01			---		VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1316-T02-D	1	2.07E+02			2.07E+02	1.4E+01	7.5E+00	2.4E+01	10	325	3.45E+03	100%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1316-T03-D	1	3.45E+02			3.45E+02	7.8E+00	7.5E+00	2.4E+01			---		VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1316-T04-D	1	4.82E+02			4.82E+02	4.4E+00	7.5E+00	2.4E+01			---		VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1316-T05-D															
Sb	EaFA-LRef-1316-T01-E	1	1.73E+02			1.73E+02	2.0E+01	7.5E+00	2.4E+01			---		VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1316-T02-E	1	2.05E+02			2.05E+02	6.5E+00	7.5E+00	2.4E+01	10	325	3.53E+03	102%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1316-T03-E	1	3.58E+02			3.58E+02	2.3E+00	7.5E+00	2.4E+01			---		VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1316-T04-E	1	4.43E+02			4.43E+02	2.2E+00	7.5E+00	2.4E+01			---		VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1316-T05-E															
Sb	EaFA-LRef-1316-T01-F	1	1.76E+02			1.76E+02	1.4E+01	7.5E+00	2.4E+01			---		VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1316-T02-F	1	2.07E+02			2.07E+02	1.0E+01	7.5E+00	2.4E+01	10	325	3.42E+03	99%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1316-T03-F	1	3.68E+02			3.68E+02	3.9E+00	7.5E+00	2.4E+01			---		VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1316-T04-F	1	4.84E+02			4.84E+02	7.5E+00	7.5E+00	2.4E+01			---		VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sb	EaFA-LRef-1316-T05-F															

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	EaFA-LRef-1316-T01-D	1	1.05E+02			1.05E+02	8.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1316-T02-D	1	7.01E+01			7.01E+01	1.1E+01	1.1E+01	3.5E+01	10	325	3.26E+03	98%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1316-T03-D	1	8.30E+01			8.30E+01	2.8E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1316-T04-D	1	1.47E+02			1.47E+02	1.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1316-T05-D															
As	EaFA-LRef-1316-T01-E	1	1.20E+02			1.20E+02	1.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1316-T02-E	1	7.01E+01			7.01E+01	5.8E+00	1.1E+01	3.5E+01	10	325	3.87E+03	117%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1316-T03-E	1	6.15E+01			6.15E+01	5.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1316-T04-E	1	9.56E+01			9.56E+01	1.8E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1316-T05-E															
As	EaFA-LRef-1316-T01-F	1	1.11E+02			1.11E+02	1.9E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1316-T02-F	1	8.42E+01			8.42E+01	3.2E+01	1.1E+01	3.5E+01	10	325	3.69E+03	111%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1316-T03-F	1	8.74E+01			8.74E+01	2.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1316-T04-F	1	7.90E+01			7.90E+01	1.1E+01	1.1E+01	3.5E+01				---	VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
As	EaFA-LRef-1316-T05-F															

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	EaFA-LRef-1316-T01-D	1	4.15E+03			4.15E+03	5.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1316-T02-D	1	8.32E+03			8.32E+03	2.6E+00	1.0E+00	3.2E+00	1000	100	9.20E+03	88%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1316-T03-D	1	1.94E+04			1.94E+04	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1316-T04-D	1	3.35E+04			3.35E+04	8.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1316-T05-D															
B	EaFA-LRef-1316-T01-E	1	4.70E+03			4.70E+03	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1316-T02-E	1	8.23E+03			8.23E+03	1.1E+00	1.0E+00	3.2E+00	1000	100	9.26E+03	104%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1316-T03-E	1	1.95E+04			1.95E+04	2.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1316-T04-E	1	3.33E+04			3.33E+04	1.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1316-T05-E															
B	EaFA-LRef-1316-T01-F	1	4.23E+03			4.23E+03	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1316-T02-F	1	8.30E+03			8.30E+03	2.1E+00	1.0E+00	3.2E+00	1000	100	9.27E+03	96%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1316-T03-F	1	1.94E+04			1.94E+04	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1316-T04-F	1	3.31E+04			3.31E+04	9.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
B	EaFA-LRef-1316-T05-F															

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	EaFA-LRef-1316-T01-D	1	2.77E+02			2.77E+02	7.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1316-T02-D	1	2.04E+02			2.04E+02	4.7E-01	1.0E+00	3.2E+00	10	325	3.30E+03	95%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1316-T03-D	1	1.78E+02			1.78E+02	6.4E-01	1.0E+00	3.2E+00			---		VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1316-T04-D	1	2.08E+02			2.08E+02	8.5E-01	1.0E+00	3.2E+00			---		VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1316-T05-D															
Ba	EaFA-LRef-1316-T01-E	1	2.83E+02			2.83E+02	9.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1316-T02-E	1	1.95E+02			1.95E+02	4.7E-01	1.0E+00	3.2E+00	10	325	3.34E+03	97%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1316-T03-E	1	1.51E+02			1.51E+02	6.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1316-T04-E	1	2.06E+02			2.06E+02	1.9E-01	1.0E+00	3.2E+00			---		VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1316-T05-E															
Ba	EaFA-LRef-1316-T01-F	1	2.84E+02			2.84E+02	3.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1316-T02-F	1	2.01E+02			2.01E+02	7.5E-01	1.0E+00	3.2E+00	10	325	3.25E+03	94%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1316-T03-F	1	1.74E+02			1.74E+02	2.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1316-T04-F	1	2.13E+02			2.13E+02	4.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ba	EaFA-LRef-1316-T05-F															

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	EaFA-LRef-1316-T01-D	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00			---		VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1316-T02-D	1	9.50E-01	U1/2		9.50E-01	2.8E+02	1.9E+00	6.0E+00	10	325	3.47E+03	107%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1316-T03-D	1	9.50E-01	U1/2		9.50E-01	4.2E+03	1.9E+00	6.0E+00			---		VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1316-T04-D	1	9.50E-01	U1/2		9.50E-01	5.4E+01	1.9E+00	6.0E+00			---		VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1316-T05-D															
Be	EaFA-LRef-1316-T01-E	1	9.50E-01	U1/2		9.50E-01	1.1E+01	1.9E+00	6.0E+00			---		VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1316-T02-E	1	9.50E-01	U1/2		9.50E-01	7.2E+01	1.9E+00	6.0E+00	10	325	3.57E+03	110%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1316-T03-E	1	9.50E-01	U1/2		9.50E-01	9.5E+01	1.9E+00	6.0E+00			---		VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1316-T04-E	1	9.50E-01	U1/2		9.50E-01	6.9E+01	1.9E+00	6.0E+00			---		VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1316-T05-E															
Be	EaFA-LRef-1316-T01-F	1	9.50E-01	U1/2		9.50E-01	2.5E+02	1.9E+00	6.0E+00			---		VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1316-T02-F	1	9.50E-01	U1/2		9.50E-01	5.4E+04	1.9E+00	6.0E+00	10	325	3.46E+03	106%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1316-T03-F	1	9.50E-01	U1/2		9.50E-01	1.7E+02	1.9E+00	6.0E+00			---		VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1316-T04-F	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00			---		VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Be	EaFA-LRef-1316-T05-F															

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	EaFA-LRef-1316-T01-D	1	1.10E+00	U1/2		1.10E+00	1.7E+02	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1316-T02-D	1	1.10E+00	U1/2		1.10E+00	1.7E+02	2.2E+00	7.0E+00	10	325	3.42E+03	105%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1316-T03-D	1	2.65E+00	E		2.65E+00	2.0E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1316-T04-D	1	1.10E+00	U1/2		1.10E+00	8.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1316-T05-D															
Cd	EaFA-LRef-1316-T01-E	1	1.10E+00	U1/2		1.10E+00	9.0E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1316-T02-E	1	1.10E+00	U1/2		1.10E+00	3.3E+01	2.2E+00	7.0E+00	10	325	3.47E+03	107%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1316-T03-E	1	3.16E+00	E		3.16E+00	1.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1316-T04-E	1	1.10E+00	U1/2		1.10E+00	4.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1316-T05-E															
Cd	EaFA-LRef-1316-T01-F	1	1.10E+00	U1/2		1.10E+00	1.7E+02	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1316-T02-F	1	1.10E+00	U1/2		1.10E+00	3.8E+01	2.2E+00	7.0E+00	10	325	3.36E+03	103%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1316-T03-F	1	3.45E+00	E		3.45E+00	5.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1316-T04-F	1	1.10E+00	U1/2		1.10E+00	2.7E+01	2.2E+00	7.0E+00				---	VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cd	EaFA-LRef-1316-T05-F															

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	EaFA-LRef-1316-T01-D	1	1.47E+05			1.47E+05	1.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1316-T02-D	1	3.01E+05			3.01E+05	3.2E-01	2.6E+00	8.3E+00	1000	100	3.02E+05	83%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1316-T03-D	1	6.93E+05			6.93E+05	1.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1316-T04-D	1	5.39E+05			5.39E+05	7.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1316-T05-D															
Ca	EaFA-LRef-1316-T01-E	1	1.53E+05			1.53E+05	5.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1316-T02-E	1	2.93E+05			2.93E+05	6.2E-01	2.6E+00	8.3E+00	1000	100	2.93E+05	92%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1316-T03-E	1	6.95E+05			6.95E+05	6.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1316-T04-E	1	5.37E+05			5.37E+05	2.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1316-T05-E															
Ca	EaFA-LRef-1316-T01-F	1	1.46E+05			1.46E+05	3.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1316-T02-F	1	2.93E+05			2.93E+05	8.2E-01	2.6E+00	8.3E+00	1000	100	2.94E+05	86%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1316-T03-F	1	6.69E+05			6.69E+05	1.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1316-T04-F	1	5.20E+05			5.20E+05	1.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ca	EaFA-LRef-1316-T05-F															

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	EaFA-LRef-1316-T01-D	1	1.60E+01			1.60E+01	1.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1316-T02-D	1	4.35E+01			4.35E+01	3.6E+00	1.2E+00	3.8E+00	10	325	3.34E+03	101%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1316-T03-D	1	4.27E+01			4.27E+01	2.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1316-T04-D	1	7.94E+01			7.94E+01	7.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1316-T05-D															
Cr	EaFA-LRef-1316-T01-E	1	1.76E+01			1.76E+01	5.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1316-T02-E	1	4.27E+01			4.27E+01	3.4E+00	1.2E+00	3.8E+00	10	325	3.41E+03	104%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1316-T03-E	1	4.29E+01			4.29E+01	4.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1316-T04-E	1	8.36E+01			8.36E+01	1.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1316-T05-E															
Cr	EaFA-LRef-1316-T01-F	1	1.87E+01			1.87E+01	5.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1316-T02-F	1	4.34E+01			4.34E+01	1.5E+00	1.2E+00	3.8E+00	10	325	3.32E+03	101%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1316-T03-F	1	4.28E+01			4.28E+01	4.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1316-T04-F	1	6.10E+01			6.10E+01	1.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cr	EaFA-LRef-1316-T05-F															

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	EaFA-LRef-1316-T01-D	1	3.95E+01			3.95E+01	6.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1316-T02-D	1	6.10E+01			6.10E+01	2.4E+00	1.8E+00	5.7E+00	10	325	3.35E+03	101%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1316-T03-D	1	1.38E+02			1.38E+02	3.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1316-T04-D	1	7.08E+01			7.08E+01	4.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1316-T05-D															
Co	EaFA-LRef-1316-T01-E	1	3.88E+01			3.88E+01	3.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1316-T02-E	1	5.55E+01			5.55E+01	5.0E+00	1.8E+00	5.7E+00	10	325	3.40E+03	103%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1316-T03-E	1	1.42E+02			1.42E+02	6.9E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1316-T04-E	1	7.50E+01			7.50E+01	3.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1316-T05-E															
Co	EaFA-LRef-1316-T01-F	1	4.08E+01			4.08E+01	6.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1316-T02-F	1	6.03E+01			6.03E+01	3.6E+00	1.8E+00	5.7E+00	10	325	3.33E+03	101%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1316-T03-F	1	1.42E+02			1.42E+02	1.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1316-T04-F	1	9.09E+01			9.09E+01	2.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Co	EaFA-LRef-1316-T05-F															

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	EaFA-LRef-1316-T01-D	1	8.42E+00	E		8.42E+00	1.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1316-T02-D	1	1.26E+01			1.26E+01	2.7E+00	3.7E+00	1.2E+01	10	325	3.08E+03	94%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1316-T03-D	1	1.83E+01			1.83E+01	3.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1316-T04-D	1	1.66E+01			1.66E+01	1.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1316-T05-D															
Cu	EaFA-LRef-1316-T01-E	1	7.60E+00	E		7.60E+00	1.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1316-T02-E	1	7.02E+00	E		7.02E+00	2.0E+01	3.7E+00	1.2E+01	10	325	3.10E+03	95%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1316-T03-E	1	1.83E+01			1.83E+01	2.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1316-T04-E	1	1.76E+01			1.76E+01	3.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1316-T05-E															
Cu	EaFA-LRef-1316-T01-F	1	9.02E+00	E		9.02E+00	5.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1316-T02-F	1	8.84E+00	E		8.84E+00	5.9E+01	3.7E+00	1.2E+01	10	325	3.08E+03	94%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1316-T03-F	1	1.06E+01	E		1.06E+01	1.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1316-T04-F	1	2.20E+01			2.20E+01	1.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Cu	EaFA-LRef-1316-T05-F															

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	EaFA-LRef-1316-T01-D	1	1.00E+00	U1/2		1.00E+00	3.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1316-T02-D	1	1.00E+00	U1/2		1.00E+00	6.1E+00	2.0E+00	6.4E+00	1000	100	1.00E+03	100%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1316-T03-D	1	1.00E+00	U1/2		1.00E+00	8.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1316-T04-D	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1316-T05-D															
Fe	EaFA-LRef-1316-T01-E	1	1.00E+00	U1/2		1.00E+00	5.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1316-T02-E	1	1.00E+00	U1/2		1.00E+00	1.3E+01	2.0E+00	6.4E+00	1000	100	1.04E+03	104%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1316-T03-E	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1316-T04-E	1	1.00E+00	U1/2		1.00E+00	4.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1316-T05-E															
Fe	EaFA-LRef-1316-T01-F	1	1.00E+00	U1/2		1.00E+00	7.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1316-T02-F	1	1.00E+00	U1/2		1.00E+00	2.4E+00	2.0E+00	6.4E+00	1000	100	1.09E+03	109%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1316-T03-F	1	1.00E+00	U1/2		1.00E+00	6.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1316-T04-F	1	1.00E+00	U1/2		1.00E+00	5.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Fe	EaFA-LRef-1316-T05-F															

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	EaFA-LRef-1316-T01-D	1	3.40E+00	U1/2		3.40E+00	1.4E+02	6.8E+00	2.2E+01			---		VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1316-T02-D	1	3.40E+00	U1/2		3.40E+00	7.5E+01	6.8E+00	2.2E+01	10	325	3.39E+03	104%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1316-T03-D	1	3.40E+00	U1/2		3.40E+00	2.0E+02	6.8E+00	2.2E+01			---		VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1316-T04-D	1	3.40E+00	U1/2		3.40E+00	2.5E+02	6.8E+00	2.2E+01			---		VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1316-T05-D															
Pb	EaFA-LRef-1316-T01-E	1	3.40E+00	U1/2		3.40E+00	1.3E+03	6.8E+00	2.2E+01			---		VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1316-T02-E	1	3.40E+00	U1/2		3.40E+00	2.4E+02	6.8E+00	2.2E+01	10	325	3.35E+03	103%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1316-T03-E	1	3.40E+00	U1/2		3.40E+00	2.3E+02	6.8E+00	2.2E+01			---		VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1316-T04-E	1	3.40E+00	U1/2		3.40E+00	4.5E+02	6.8E+00	2.2E+01			---		VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1316-T05-E															
Pb	EaFA-LRef-1316-T01-F	1	3.40E+00	U1/2		3.40E+00	4.0E+02	6.8E+00	2.2E+01			---		VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1316-T02-F	1	3.40E+00	U1/2		3.40E+00	8.1E+01	6.8E+00	2.2E+01	10	325	3.69E+03	114%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1316-T03-F	1	3.40E+00	U1/2		3.40E+00	3.7E+02	6.8E+00	2.2E+01			---		VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1316-T04-F	1	3.40E+00	U1/2		3.40E+00	6.2E+02	6.8E+00	2.2E+01			---		VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Pb	EaFA-LRef-1316-T05-F															

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	EaFA-LRef-1316-T01-D	1	3.24E+03			3.24E+03	1.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1316-T02-D	1	6.55E+03			6.55E+03	8.6E-01	1.9E+00	6.0E+00	10	325	9.29E+03	84%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1316-T03-D	1	1.51E+04			1.51E+04	6.9E-02	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1316-T04-D	1	2.91E+04			2.91E+04	1.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1316-T05-D															
Li	EaFA-LRef-1316-T01-E	1	3.39E+03			3.39E+03	1.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1316-T02-E	1	6.23E+03			6.23E+03	4.1E-01	1.9E+00	6.0E+00	10	325	9.19E+03	91%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1316-T03-E	1	1.51E+04			1.51E+04	5.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1316-T04-E	1	2.92E+04			2.92E+04	3.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1316-T05-E															
Li	EaFA-LRef-1316-T01-F	1	3.25E+03			3.25E+03	5.4E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1316-T02-F	1	6.30E+03			6.30E+03	5.2E-01	1.9E+00	6.0E+00	10	325	9.17E+03	88%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1316-T03-F	1	1.48E+04			1.48E+04	2.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1316-T04-F	1	2.86E+04			2.86E+04	1.6E-01	1.9E+00	6.0E+00				---	VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Li	EaFA-LRef-1316-T05-F															

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	EaFA-LRef-1316-T01-D	1	3.51E+02			3.51E+02	3.4E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1316-T02-D	1	4.96E+02			4.96E+02	8.5E-01	2.0E+00	6.4E+00	10	325	3.33E+03	87%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1316-T03-D	1	1.15E+03			1.15E+03	1.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1316-T04-D	1	8.44E+02			8.44E+02	1.5E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1316-T05-D															
Mn	EaFA-LRef-1316-T01-E	1	3.45E+02			3.45E+02	1.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1316-T02-E	1	4.71E+02			4.71E+02	7.3E-01	2.0E+00	6.4E+00	10	325	3.39E+03	90%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1316-T03-E	1	1.18E+03			1.18E+03	3.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1316-T04-E	1	8.69E+02			8.69E+02	9.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1316-T05-E															
Mn	EaFA-LRef-1316-T01-F	1	3.41E+02			3.41E+02	1.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1316-T02-F	1	5.22E+02			5.22E+02	2.0E-01	2.0E+00	6.4E+00	10	325	3.34E+03	87%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1316-T03-F	1	1.12E+03			1.12E+03	1.9E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1316-T04-F	1	9.92E+02			9.92E+02	1.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mn	EaFA-LRef-1316-T05-F															

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	EaFA-LRef-1316-T01-D	1	6.33E+03			6.33E+03	4.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1316-T02-D	1	1.37E+04			1.37E+04	1.2E+00	1.0E+00	3.2E+00	1000	100	1.46E+04	92%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1316-T03-D	1	3.38E+04			3.38E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1316-T04-D	1	6.07E+04			6.07E+04	8.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1316-T05-D															
Mg	EaFA-LRef-1316-T01-E	1	6.50E+03			6.50E+03	5.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1316-T02-E	1	1.34E+04			1.34E+04	2.1E-01	1.0E+00	3.2E+00	1000	100	1.44E+04	93%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1316-T03-E	1	3.43E+04			3.43E+04	6.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1316-T04-E	1	6.11E+04			6.11E+04	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1316-T05-E															
Mg	EaFA-LRef-1316-T01-F	1	6.27E+03			6.27E+03	2.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1316-T02-F	1	1.35E+04			1.35E+04	1.2E+00	1.0E+00	3.2E+00	1000	100	1.45E+04	96%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1316-T03-F	1	3.36E+04			3.36E+04	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1316-T04-F	1	6.01E+04			6.01E+04	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mg	EaFA-LRef-1316-T05-F															

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	EaFA-LRef-1316-T01-D	1	3.10E+03			3.10E+03	5.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1316-T02-D	1	5.77E+03			5.77E+03	2.6E-01	1.2E+00	3.8E+00	10	325	8.94E+03	98%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1316-T03-D	1	1.25E+04			1.25E+04	5.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1316-T04-D	1	2.53E+04			2.53E+04	6.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1316-T05-D															
Mo	EaFA-LRef-1316-T01-E	1	3.20E+03			3.20E+03	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1316-T02-E	1	5.69E+03			5.69E+03	2.8E-01	1.2E+00	3.8E+00	10	325	8.90E+03	99%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1316-T03-E	1	1.26E+04			1.26E+04	6.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1316-T04-E	1	2.47E+04			2.47E+04	6.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1316-T05-E															
Mo	EaFA-LRef-1316-T01-F	1	3.13E+03			3.13E+03	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1316-T02-F	1	5.61E+03			5.61E+03	5.8E-01	1.2E+00	3.8E+00	10	325	8.81E+03	98%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1316-T03-F	1	1.25E+04			1.25E+04	3.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1316-T04-F	1	2.41E+04			2.41E+04	5.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Mo	EaFA-LRef-1316-T05-F															

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	EaFA-LRef-1316-T01-D	1	9.38E+01			9.38E+01	1.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1316-T02-D	1	1.35E+02			1.35E+02	2.2E+00	1.8E+00	5.7E+00	10	325	3.46E+03	102%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1316-T03-D	1	3.05E+02			3.05E+02	8.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1316-T04-D	1	1.62E+02			1.62E+02	3.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1316-T05-D															
Ni	EaFA-LRef-1316-T01-E	1	9.14E+01			9.14E+01	2.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1316-T02-E	1	1.24E+02			1.24E+02	1.9E+00	1.8E+00	5.7E+00	10	325	3.50E+03	104%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1316-T03-E	1	3.14E+02			3.14E+02	6.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1316-T04-E	1	1.72E+02			1.72E+02	9.4E-01	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1316-T05-E															
Ni	EaFA-LRef-1316-T01-F	1	9.39E+01			9.39E+01	3.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1316-T02-F	1	1.39E+02			1.39E+02	1.9E+00	1.8E+00	5.7E+00	10	325	3.42E+03	101%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1316-T03-F	1	3.08E+02			3.08E+02	2.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1316-T04-F	1	1.89E+02			1.89E+02	2.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ni	EaFA-LRef-1316-T05-F															

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	EaFA-LRef-1316-T01-D	1	2.22E+01			2.22E+01	3.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1316-T02-D	1	6.21E+01			6.21E+01	3.0E+00	3.7E+00	1.2E+01	1000	100	1.14E+03	108%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1316-T03-D	1	1.28E+02			1.28E+02	1.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1316-T04-D	1	3.12E+01			3.12E+01	4.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1316-T05-D															
P	EaFA-LRef-1316-T01-E	1	3.98E+01			3.98E+01	1.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1316-T02-E	1	7.68E+01			7.68E+01	7.9E+00	3.7E+00	1.2E+01	1000	100	1.14E+03	106%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1316-T03-E	1	1.27E+02			1.27E+02	1.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1316-T04-E	1	1.60E+01			1.60E+01	8.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1316-T05-E															
P	EaFA-LRef-1316-T01-F	1	9.10E+01			9.10E+01	4.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1316-T02-F	1	5.97E+01			5.97E+01	1.1E+01	3.7E+00	1.2E+01	1000	100	1.12E+03	106%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1316-T03-F	1	1.97E+02			1.97E+02	9.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1316-T04-F	1	1.48E+01			1.48E+01	5.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
P	EaFA-LRef-1316-T05-F															

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	EaFA-LRef-1316-T01-D	1	2.27E+04			2.27E+04	9.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1316-T02-D	1	4.97E+04			4.97E+04	1.2E+00	1.6E+00	5.1E+00	1000	100	5.06E+04	93%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1316-T03-D	1	1.22E+05			1.22E+05	8.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1316-T04-D	1	1.94E+05			1.94E+05	7.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1316-T05-D															
K	EaFA-LRef-1316-T01-E	1	2.37E+04			2.37E+04	1.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1316-T02-E	1	4.78E+04			4.78E+04	1.0E+00	1.6E+00	5.1E+00	1000	100	4.88E+04	105%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1316-T03-E	1	1.21E+05			1.21E+05	5.5E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1316-T04-E	1	1.96E+05			1.96E+05	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1316-T05-E															
K	EaFA-LRef-1316-T01-F	1	2.26E+04			2.26E+04	1.4E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1316-T02-F	1	4.84E+04			4.84E+04	4.2E-01	1.6E+00	5.1E+00	1000	100	4.93E+04	90%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1316-T03-F	1	1.19E+05			1.19E+05	2.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1316-T04-F	1	1.89E+05			1.89E+05	1.4E+00	1.6E+00	5.1E+00				---	VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
K	EaFA-LRef-1316-T05-F															

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	EaFA-LRef-1316-T01-D	1	9.95E+02			9.95E+02	1.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1316-T02-D	1	1.03E+03			1.03E+03	4.5E+00	1.5E+01	4.8E+01	10	325	3.90E+03	88%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1316-T03-D	1	1.19E+03			1.19E+03	2.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1316-T04-D	1	1.81E+03			1.81E+03	2.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1316-T05-D															
Se	EaFA-LRef-1316-T01-E	1	1.04E+03			1.04E+03	1.8E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1316-T02-E	1	1.09E+03			1.09E+03	1.6E+00	1.5E+01	4.8E+01	10	325	4.01E+03	90%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1316-T03-E	1	1.11E+03			1.11E+03	3.0E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1316-T04-E	1	1.67E+03			1.67E+03	3.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1316-T05-E															
Se	EaFA-LRef-1316-T01-F	1	1.05E+03			1.05E+03	2.2E-01	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1316-T02-F	1	1.05E+03			1.05E+03	2.8E+00	1.5E+01	4.8E+01	10	325	4.10E+03	94%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1316-T03-F	1	1.19E+03			1.19E+03	1.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1316-T04-F	1	1.68E+03			1.68E+03	2.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Se	EaFA-LRef-1316-T05-F															

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	EaFA-LRef-1316-T01-D	1	2.14E+03			2.14E+03	5.3E-01	1.1E+00	3.5E+00			---		VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1316-T02-D	1	1.65E+03			1.65E+03	6.0E-01	1.1E+00	3.5E+00	1000	100	2.59E+03	94%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1316-T03-D	1	1.88E+03			1.88E+03	4.9E-01	1.1E+00	3.5E+00			---		VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1316-T04-D	1	1.49E+03			1.49E+03	6.4E-01	1.1E+00	3.5E+00			---		VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1316-T05-D															
Si	EaFA-LRef-1316-T01-E	1	2.17E+03			2.17E+03	1.4E+00	1.1E+00	3.5E+00			---		VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1316-T02-E	1	1.67E+03			1.67E+03	5.1E-01	1.1E+00	3.5E+00	1000	100	2.69E+03	102%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1316-T03-E	1	1.87E+03			1.87E+03	6.1E+00	1.1E+00	3.5E+00			---		VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1316-T04-E	1	1.49E+03			1.49E+03	3.5E-01	1.1E+00	3.5E+00			---		VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1316-T05-E															
Si	EaFA-LRef-1316-T01-F	1	2.18E+03			2.18E+03	6.5E-01	1.1E+00	3.5E+00			---		VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1316-T02-F	1	1.67E+03			1.67E+03	7.7E-01	1.1E+00	3.5E+00	1000	100	2.56E+03	89%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1316-T03-F	1	1.85E+03			1.85E+03	1.2E-01	1.1E+00	3.5E+00			---		VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1316-T04-F	1	1.70E+03			1.70E+03	4.6E-01	1.1E+00	3.5E+00			---		VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Si	EaFA-LRef-1316-T05-F															

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	EaFA-LRef-1316-T01-D	1	4.61E+03			4.61E+03	1.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1316-T02-D	1	1.02E+04			1.02E+04	7.6E-01	2.5E+00	8.0E+00	1000	100	1.13E+04	106%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1316-T03-D	1	2.53E+04			2.53E+04	7.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1316-T04-D	1	4.23E+04			4.23E+04	8.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1316-T05-D															
Na	EaFA-LRef-1316-T01-E	1	4.90E+03			4.90E+03	1.6E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1316-T02-E	1	9.58E+03			9.58E+03	4.1E-02	2.5E+00	8.0E+00	1000	100	1.06E+04	101%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1316-T03-E	1	2.53E+04			2.53E+04	6.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1316-T04-E	1	4.25E+04			4.25E+04	7.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1316-T05-E															
Na	EaFA-LRef-1316-T01-F	1	4.60E+03			4.60E+03	1.0E+00	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1316-T02-F	1	9.64E+03			9.64E+03	8.3E-01	2.5E+00	8.0E+00	1000	100	1.07E+04	103%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1316-T03-F	1	2.43E+04			2.43E+04	1.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1316-T04-F	1	4.11E+04			4.11E+04	3.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Na	EaFA-LRef-1316-T05-F															

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	EaFA-LRef-1316-T01-D	1	2.04E+03			2.04E+03	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1316-T02-D	1	3.96E+03			3.96E+03	8.2E-01	1.0E+00	3.2E+00	1000	100	4.86E+03	90%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1316-T03-D	1	7.42E+03			7.42E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1316-T04-D	1	7.50E+03			7.50E+03	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1316-T05-D															
Sr	EaFA-LRef-1316-T01-E	1	2.07E+03			2.07E+03	7.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1316-T02-E	1	3.84E+03			3.84E+03	5.3E-01	1.0E+00	3.2E+00	1000	100	4.79E+03	95%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1316-T03-E	1	7.44E+03			7.44E+03	4.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1316-T04-E	1	7.47E+03			7.47E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1316-T05-E															
Sr	EaFA-LRef-1316-T01-F	1	2.02E+03			2.02E+03	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1316-T02-F	1	3.93E+03			3.93E+03	7.1E-01	1.0E+00	3.2E+00	1000	100	4.85E+03	92%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1316-T03-F	1	7.30E+03			7.30E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1316-T04-F	1	7.27E+03			7.27E+03	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Sr	EaFA-LRef-1316-T05-F															

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	EaFA-LRef-1316-T01-D	1	1.42E+05			1.42E+05	5.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1316-T02-D	1	2.74E+05			2.74E+05	7.7E-01	6.8E+00	2.2E+01	1000	100	2.75E+05	86%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1316-T03-D	1	6.39E+05			6.39E+05	6.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1316-T04-D	1	6.62E+05			6.62E+05	9.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1316-T05-D															
S	EaFA-LRef-1316-T01-E	1	1.41E+05			1.41E+05	8.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1316-T02-E	1	2.82E+05			2.82E+05	3.9E-01	6.8E+00	2.2E+01	1000	100	2.83E+05	85%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1316-T03-E	1	6.47E+05			6.47E+05	5.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1316-T04-E	1	6.58E+05			6.58E+05	3.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1316-T05-E															
S	EaFA-LRef-1316-T01-F	1	1.42E+05			1.42E+05	7.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1316-T02-F	1	2.85E+05			2.85E+05	5.5E-01	6.8E+00	2.2E+01	1000	100	2.86E+05	91%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1316-T03-F	1	6.53E+05			6.53E+05	2.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1316-T04-F	1	6.55E+05			6.55E+05	7.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
S	EaFA-LRef-1316-T05-F															

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	EaFA-LRef-1316-T01-D	1	2.30E+00	U1/2		2.30E+00	2.0E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1316-T02-D	1	7.55E+00	E		7.55E+00	1.2E+02	4.6E+00	1.5E+01	10	325	3.30E+03	101%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1316-T03-D	1	1.60E+01			1.60E+01	5.8E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1316-T04-D	1	2.21E+01			2.21E+01	1.8E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1316-T05-D															
Tl	EaFA-LRef-1316-T01-E	1	2.30E+00	U1/2		2.30E+00	1.0E+03	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1316-T02-E	1	2.30E+00	U1/2		2.30E+00	5.5E+02	4.6E+00	1.5E+01	10	325	3.37E+03	104%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1316-T03-E	1	1.21E+01	E		1.21E+01	9.2E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1316-T04-E	1	1.97E+01			1.97E+01	1.3E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1316-T05-E															
Tl	EaFA-LRef-1316-T01-F	1	4.62E+00	E		4.62E+00	1.2E+02	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1316-T02-F	1	6.22E+00	E		6.22E+00	4.9E+01	4.6E+00	1.5E+01	10	325	3.26E+03	100%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1316-T03-F	1	1.62E+01			1.62E+01	6.7E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1316-T04-F	1	2.66E+01			2.66E+01	6.0E+01	4.6E+00	1.5E+01			---		VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Tl	EaFA-LRef-1316-T05-F															

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	EaFA-LRef-1316-T01-D	1	1.00E+00	U1/2		1.00E+00	4.7E+02	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1316-T02-D	1	1.00E+00	U1/2		1.00E+00	1.8E+02	2.0E+00	6.4E+00	10	325	3.28E+03	101%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1316-T03-D	1	1.00E+00	U1/2		1.00E+00	7.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1316-T04-D	1	1.00E+00	U1/2		1.00E+00	3.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1316-T05-D															
Ti	EaFA-LRef-1316-T01-E	1	1.00E+00	U1/2		1.00E+00	1.7E+02	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1316-T02-E	1	1.00E+00	U1/2		1.00E+00	8.0E+00	2.0E+00	6.4E+00	10	325	3.33E+03	102%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1316-T03-E	1	1.00E+00	U1/2		1.00E+00	2.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1316-T04-E	1	1.00E+00	U1/2		1.00E+00	5.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1316-T05-E															
Ti	EaFA-LRef-1316-T01-F	1	1.00E+00	U1/2		1.00E+00	3.4E+02	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1316-T02-F	1	1.00E+00	U1/2		1.00E+00	2.9E+02	2.0E+00	6.4E+00	10	325	3.24E+03	100%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1316-T03-F	1	1.00E+00	U1/2		1.00E+00	3.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1316-T04-F	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00			---		VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Ti	EaFA-LRef-1316-T05-F															

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	EaFA-LRef-1316-T01-D	1	2.09E+02			2.09E+02	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1316-T02-D	1	1.80E+02			1.80E+02	1.0E+00	1.5E+00	4.8E+00	10	325	3.53E+03	103%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1316-T03-D	1	2.37E+02			2.37E+02	1.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1316-T04-D	1	2.46E+02			2.46E+02	2.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1316-T05-D															
V	EaFA-LRef-1316-T01-E	1	2.16E+02			2.16E+02	2.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1316-T02-E	1	1.74E+02			1.74E+02	5.5E-01	1.5E+00	4.8E+00	10	325	3.58E+03	105%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1316-T03-E	1	2.14E+02			2.14E+02	5.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1316-T04-E	1	2.37E+02			2.37E+02	1.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1316-T05-E															
V	EaFA-LRef-1316-T01-F	1	2.12E+02			2.12E+02	8.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1316-T02-F	1	1.74E+02			1.74E+02	6.0E-01	1.5E+00	4.8E+00	10	325	3.47E+03	101%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1316-T03-F	1	2.28E+02			2.28E+02	5.9E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1316-T04-F	1	2.49E+02			2.49E+02	2.6E-01	1.5E+00	4.8E+00				---	VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
V	EaFA-LRef-1316-T05-F															

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	EaFA-LRef-1316-T01-D	1	2.99E+01			2.99E+01	3.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:23 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1316-T02-D	1	3.06E+01			3.06E+01	3.3E+00	1.0E+00	3.2E+00	10	325	3.44E+03	105%	VU ICP-OES	6/7/10 11:07 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1316-T03-D	1	3.58E+01			3.58E+01	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:08 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1316-T04-D	1	6.44E+01			6.44E+01	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:10 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1316-T05-D															
Zn	EaFA-LRef-1316-T01-E	1	1.71E+01			1.71E+01	1.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:12 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1316-T02-E	1	2.68E+01			2.68E+01	6.9E+00	1.0E+00	3.2E+00	10	325	3.47E+03	106%	VU ICP-OES	6/7/10 1:24 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1316-T03-E	1	3.89E+01			3.89E+01	5.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:15 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1316-T04-E	1	7.42E+01			7.42E+01	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:17 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1316-T05-E															
Zn	EaFA-LRef-1316-T01-F	1	3.41E+01			3.41E+01	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:26 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1316-T02-F	1	7.11E+01			7.11E+01	9.7E-01	1.0E+00	3.2E+00	10	325	3.43E+03	103%	VU ICP-OES	6/7/10 1:28 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1316-T03-F	1	9.74E+01			9.74E+01	9.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 1:29 PM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1316-T04-F	1	3.06E+02			3.06E+02	8.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	6/7/10 11:23 AM	EPA Interlab LRef D-F 1313-1316 EaFA
Zn	EaFA-LRef-1316-T05-F															

QA-QC Spreadsheet 1316:

Al		Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	SWA-L01-1316-T01-A	1	3.65E+04			3.65E+04	2.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1316-T02-A	1	4.32E+04			4.32E+04	4.7E-01	1.0E+00	3.2E+00	1000	100	4.41E+04	86%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1316-T03-A	1	9.66E+04			9.66E+04	2.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1316-T04-A	1	1.77E+05			1.77E+05	9.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1316-T01-B	1	3.57E+04			3.57E+04	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1316-T02-B	1	4.25E+04			4.25E+04	6.2E-01	1.0E+00	3.2E+00	1000	100	4.33E+04	89%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1316-T03-B	1	9.58E+04			9.58E+04	3.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1316-T04-B	1	1.68E+05			1.68E+05	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1316-T01-C	1	3.72E+04			3.72E+04	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1316-T02-C	1	4.59E+04			4.59E+04	7.8E-01	1.0E+00	3.2E+00	1000	100	4.68E+04	89%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1316-T03-C	1	1.02E+05			1.02E+05	8.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1316-T04-C	1	1.64E+05			1.64E+05	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
Al	SWA-L01-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	SWA-L01-1316-T01-A	1	2.87E+03			2.87E+03	1.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1316-T02-A	1	3.06E+03			3.06E+03	5.6E-01	7.5E+00	2.4E+01	10	100	4.01E+03	95%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1316-T03-A	1	4.45E+03			4.45E+03	2.6E-01	7.5E+00	2.4E+01				---	VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1316-T04-A	1	4.27E+03			4.27E+03	1.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1316-T01-B	1	2.19E+03			2.19E+03	9.9E-01	7.5E+00	2.4E+01				---	VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1316-T02-B	1	3.31E+03			3.31E+03	8.3E-01	7.5E+00	2.4E+01	10	100	4.24E+03	92%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1316-T03-B	1	4.65E+03			4.65E+03	5.2E-01	7.5E+00	2.4E+01				---	VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1316-T04-B	1	4.26E+03			4.26E+03	1.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1316-T01-C	1	3.10E+03			3.10E+03	7.9E-01	7.5E+00	2.4E+01				---	VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1316-T02-C	1	3.45E+03			3.45E+03	3.7E-01	7.5E+00	2.4E+01	10	100	4.41E+03	95%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1316-T03-C	1	5.39E+03			5.39E+03	5.8E-01	7.5E+00	2.4E+01				---	VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1316-T04-C	1	5.06E+03			5.06E+03	7.7E-01	7.5E+00	2.4E+01				---	VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
Sb	SWA-L01-1316-B01-A	1	3.75E+00	U1/2		3.75E+00	2.7E+02	7.5E+00	2.4E+01				---	VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	SWA-L01-1316-T01-A	1	3.62E+03			3.62E+03	8.5E-01	1.1E+01	3.5E+01				---	VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1316-T02-A	1	8.06E+03			8.06E+03	7.4E-01	1.1E+01	3.5E+01	10	100	9.15E+03	109%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1316-T03-A	1	3.90E+04			3.90E+04	7.9E-01	1.1E+01	3.5E+01				---	VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1316-T04-A	1	9.33E+04			9.33E+04	1.7E+00	1.1E+01	3.5E+01				---	VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1316-T01-B	1	3.95E+03			3.95E+03	8.0E-01	1.1E+01	3.5E+01				---	VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1316-T02-B	1	9.06E+03			9.06E+03	3.6E-01	1.1E+01	3.5E+01	10	100	9.93E+03	88%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1316-T03-B	1	3.71E+04			3.71E+04	1.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1316-T04-B	1	9.65E+04			9.65E+04	7.8E-01	1.1E+01	3.5E+01				---	VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1316-T01-C	1	4.45E+03			4.45E+03	1.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1316-T02-C	1	8.16E+03			8.16E+03	1.4E+00	1.1E+01	3.5E+01	10	100	9.06E+03	90%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1316-T03-C	1	4.08E+04			4.08E+04	9.0E-01	1.1E+01	3.5E+01				---	VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1316-T04-C	1	1.10E+05			1.10E+05	6.8E-01	1.1E+01	3.5E+01				---	VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
As	SWA-L01-1316-B01-A	1	5.50E+00	U1/2		5.50E+00	9.6E+01	1.1E+01	3.5E+01				---	VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	SWA-L01-1316-T01-A	1	1.10E+03			1.10E+03	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1316-T02-A	1	9.38E+02			9.38E+02	7.2E-01	1.0E+00	3.2E+00	1000	100	2.01E+03	107%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1316-T03-A	1	6.73E+02			6.73E+02	6.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1316-T04-A	1	7.24E+02			7.24E+02	9.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1316-T01-B	1	1.12E+03			1.12E+03	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1316-T02-B	1	9.47E+02			9.47E+02	1.0E+00	1.0E+00	3.2E+00	1000	100	2.02E+03	108%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1316-T03-B	1	6.75E+02			6.75E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1316-T04-B	1	6.84E+02			6.84E+02	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1316-T01-C	1	1.10E+03			1.10E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1316-T02-C	1	9.78E+02			9.78E+02	1.1E+00	1.0E+00	3.2E+00	1000	100	2.03E+03	106%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1316-T03-C	1	6.80E+02			6.80E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1316-T04-C	1	6.96E+02			6.96E+02	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
B	SWA-L01-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	7.0E+02	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	SWA-L01-1316-T01-A	1	1.47E+02			1.47E+02	5.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1316-T02-A	1	1.39E+02			1.39E+02	2.9E-01	1.0E+00	3.2E+00	10	100	1.00E+03	86%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1316-T03-A	1	1.48E+02			1.48E+02	3.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1316-T04-A	1	1.24E+02			1.24E+02	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1316-T01-B	1	1.43E+02			1.43E+02	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1316-T02-B	1	1.33E+02			1.33E+02	7.6E-01	1.0E+00	3.2E+00	10	100	9.95E+02	86%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1316-T03-B	1	1.56E+02			1.56E+02	3.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1316-T04-B	1	1.12E+02			1.12E+02	4.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1316-T01-C	1	1.45E+02			1.45E+02	9.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1316-T02-C	1	1.42E+02			1.42E+02	1.8E-01	1.0E+00	3.2E+00	10	100	9.89E+02	85%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1316-T03-C	1	1.34E+02			1.34E+02	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1316-T04-C	1	1.09E+02			1.09E+02	3.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
Ba	SWA-L01-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	7.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	SWA-L01-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	3.3E+01	1.9E+00	6.0E+00	10	100	9.47E+02	95%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	1.6E+02	1.9E+00	6.0E+00				---	VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	4.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	3.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	3.0E+01	1.9E+00	6.0E+00	10	100	9.60E+02	96%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	4.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	3.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	6.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	1.5E+02	1.9E+00	6.0E+00	10	100	9.45E+02	94%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	9.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	1.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
Be	SWA-L01-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	4.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	SWA-L01-1316-T01-A	1	1.10E+00	U1/2		1.10E+00	2.6E+02	2.2E+00	7.0E+00				---	VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1316-T02-A	1	1.10E+00	U1/2		1.10E+00	1.4E+02	2.2E+00	7.0E+00	10	100	9.65E+02	96%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1316-T03-A	1	1.10E+00	U1/2		1.10E+00	3.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1316-T04-A	1	1.10E+00	U1/2		1.10E+00	1.6E+02	2.2E+00	7.0E+00				---	VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1316-T01-B	1	1.10E+00	U1/2		1.10E+00	2.0E+02	2.2E+00	7.0E+00				---	VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1316-T02-B	1	1.10E+00	U1/2		1.10E+00	4.8E+02	2.2E+00	7.0E+00	10	100	9.65E+02	96%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1316-T03-B	1	1.10E+00	U1/2		1.10E+00	7.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1316-T04-B	1	1.10E+00	U1/2		1.10E+00	2.6E+02	2.2E+00	7.0E+00				---	VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1316-T01-C	1	1.10E+00	U1/2		1.10E+00	1.8E+03	2.2E+00	7.0E+00				---	VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1316-T02-C	1	1.10E+00	U1/2		1.10E+00	5.4E+02	2.2E+00	7.0E+00	10	100	9.53E+02	95%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1316-T03-C	1	1.10E+00	U1/2		1.10E+00	1.8E+02	2.2E+00	7.0E+00				---	VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1316-T04-C	1	1.10E+00	U1/2		1.10E+00	1.8E+03	2.2E+00	7.0E+00				---	VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
Cd	SWA-L01-1316-B01-A	1	1.10E+00	U1/2		1.10E+00	2.6E+02	2.2E+00	7.0E+00				---	VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	SWA-L01-1316-T01-A	1	1.60E+04			1.60E+04	7.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1316-T02-A	1	1.13E+04			1.13E+04	9.5E-02	2.6E+00	8.3E+00	1000	100	1.24E+04	102%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1316-T03-A	1	6.11E+03			6.11E+03	2.8E+00	2.6E+00	8.3E+00				---	VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1316-T04-A	1	4.59E+03			4.59E+03	1.8E+00	2.6E+00	8.3E+00				---	VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1316-T01-B	1	1.55E+04			1.55E+04	6.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1316-T02-B	1	1.10E+04			1.10E+04	6.9E-01	2.6E+00	8.3E+00	1000	100	1.20E+04	105%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1316-T03-B	1	6.09E+03			6.09E+03	2.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1316-T04-B	1	4.73E+03			4.73E+03	9.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1316-T01-C	1	1.51E+04			1.51E+04	6.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1316-T02-C	1	1.14E+04			1.14E+04	8.3E-01	2.6E+00	8.3E+00	1000	100	1.24E+04	101%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1316-T03-C	1	5.54E+03			5.54E+03	2.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1316-T04-C	1	4.31E+03			4.31E+03	3.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
Ca	SWA-L01-1316-B01-A	1	3.27E+01			3.27E+01	1.9E+01	2.6E+00	8.3E+00				---	VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	SWA-L01-1316-T01-A	1	1.24E+03			1.24E+03	2.2E-01	1.2E+00	3.8E+00			---		VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1316-T02-A	1	1.77E+03			1.77E+03	1.7E-01	1.2E+00	3.8E+00	10	100	2.67E+03	90%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1316-T03-A	1	2.92E+03			2.92E+03	2.5E+00	1.2E+00	3.8E+00			---		VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1316-T04-A	1	3.06E+03			3.06E+03	8.3E-01	1.2E+00	3.8E+00			---		VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1316-T01-B	1	1.32E+03			1.32E+03	6.8E-01	1.2E+00	3.8E+00			---		VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1316-T02-B	1	1.55E+03			1.55E+03	1.2E+00	1.2E+00	3.8E+00	10	100	2.58E+03	103%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1316-T03-B	1	2.74E+03			2.74E+03	1.0E+00	1.2E+00	3.8E+00			---		VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1316-T04-B	1	3.67E+03			3.67E+03	1.0E+00	1.2E+00	3.8E+00			---		VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1316-T01-C	1	1.33E+03			1.33E+03	1.5E+00	1.2E+00	3.8E+00			---		VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1316-T02-C	1	1.67E+03			1.67E+03	1.0E+00	1.2E+00	3.8E+00	10	100	2.69E+03	102%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1316-T03-C	1	2.66E+03			2.66E+03	1.8E+00	1.2E+00	3.8E+00			---		VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1316-T04-C	1	3.76E+03			3.76E+03	4.6E-01	1.2E+00	3.8E+00			---		VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
Cr	SWA-L01-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	2.0E+02	1.2E+00	3.8E+00			---		VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	SWA-L01-1316-T01-A	1	9.00E-01	U1/2		9.00E-01	7.7E+02	1.8E+00	5.7E+00			---		VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1316-T02-A	1	9.00E-01	U1/2		9.00E-01	6.9E+02	1.8E+00	5.7E+00	10	100	1.05E+03	105%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1316-T03-A	1	3.03E+00	E		3.03E+00	3.3E+01	1.8E+00	5.7E+00			---		VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1316-T04-A	1	6.38E+00			6.38E+00	2.4E+01	1.8E+00	5.7E+00			---		VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1316-T01-B	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00			---		VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1316-T02-B	1	9.00E-01	U1/2		9.00E-01	1.6E+02	1.8E+00	5.7E+00	10	100	1.03E+03	103%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1316-T03-B	1	2.18E+00	E		2.18E+00	5.9E+01	1.8E+00	5.7E+00			---		VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1316-T04-B	1	6.37E+00			6.37E+00	5.5E+00	1.8E+00	5.7E+00			---		VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1316-T01-C	1	9.00E-01	U1/2		9.00E-01	2.2E+02	1.8E+00	5.7E+00			---		VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1316-T02-C	1	9.00E-01	U1/2		9.00E-01	8.9E+01	1.8E+00	5.7E+00	10	100	1.01E+03	101%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1316-T03-C	1	2.32E+00	E		2.32E+00	2.2E+01	1.8E+00	5.7E+00			---		VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1316-T04-C	1	6.42E+00			6.42E+00	2.0E+01	1.8E+00	5.7E+00			---		VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
Co	SWA-L01-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	2.7E+01	1.8E+00	5.7E+00			---		VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	SWA-L01-1316-T01-A	1	1.85E+00	U1/2		1.85E+00	2.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1316-T02-A	1	6.34E+00	E		6.34E+00	2.7E+01	3.7E+00	1.2E+01	10	100	1.04E+03	103%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1316-T03-A	1	2.61E+01			2.61E+01	6.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1316-T04-A	1	6.07E+01			6.07E+01	8.0E-01	3.7E+00	1.2E+01			---		VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1316-T01-B	1	1.85E+00	U1/2		1.85E+00	1.5E+02	3.7E+00	1.2E+01			---		VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1316-T02-B	1	9.12E+00	E		9.12E+00	1.2E+01	3.7E+00	1.2E+01	10	100	1.05E+03	104%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1316-T03-B	1	2.69E+01			2.69E+01	3.7E+00	3.7E+00	1.2E+01			---		VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1316-T04-B	1	4.97E+01			4.97E+01	4.2E+00	3.7E+00	1.2E+01			---		VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1316-T01-C	1	1.85E+00	U1/2		1.85E+00	1.1E+02	3.7E+00	1.2E+01			---		VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1316-T02-C	1	7.61E+00	E		7.61E+00	3.7E+01	3.7E+00	1.2E+01	10	100	1.02E+03	101%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1316-T03-C	1	2.05E+01			2.05E+01	6.1E+00	3.7E+00	1.2E+01			---		VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1316-T04-C	1	7.62E+01			7.62E+01	4.7E+00	3.7E+00	1.2E+01			---		VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
Cu	SWA-L01-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	3.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	SWA-L01-1316-T01-A	1	1.10E+02			1.10E+02	3.5E-01	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1316-T02-A	1	2.39E+02			2.39E+02	1.1E+00	2.0E+00	6.4E+00	1000	100	1.34E+03	110%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1316-T03-A	1	7.73E+02			7.73E+02	1.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1316-T04-A	1	1.35E+03			1.35E+03	1.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1316-T01-B	1	1.07E+02			1.07E+02	4.5E-01	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1316-T02-B	1	2.47E+02			2.47E+02	5.0E-01	2.0E+00	6.4E+00	1000	100	1.37E+03	112%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1316-T03-B	1	7.36E+02			7.36E+02	7.1E-01	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1316-T04-B	1	1.78E+03			1.78E+03	2.5E-01	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1316-T01-C	1	1.08E+02			1.08E+02	4.6E-01	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1316-T02-C	1	2.22E+02			2.22E+02	7.3E-01	2.0E+00	6.4E+00	1000	100	1.32E+03	110%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1316-T03-C	1	6.62E+02			6.62E+02	7.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1316-T04-C	1	1.83E+03			1.83E+03	7.2E-01	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
Fe	SWA-L01-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	SWA-L01-1316-T01-A	1	1.73E+01	E		1.73E+01	1.6E+01	6.8E+00	2.2E+01			---		VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1316-T02-A	1	3.73E+01			3.73E+01	9.9E+00	6.8E+00	2.2E+01	10	100	9.97E+02	96%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1316-T03-A	1	7.80E+01			7.80E+01	3.2E+00	6.8E+00	2.2E+01			---		VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1316-T04-A	1	1.69E+02			1.69E+02	5.4E+00	6.8E+00	2.2E+01			---		VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1316-T01-B	1	1.29E+01	E		1.29E+01	2.4E+01	6.8E+00	2.2E+01			---		VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1316-T02-B	1	3.49E+01			3.49E+01	8.3E+00	6.8E+00	2.2E+01	10	100	1.00E+03	97%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1316-T03-B	1	7.94E+01			7.94E+01	7.7E+00	6.8E+00	2.2E+01			---		VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1316-T04-B	1	1.88E+02			1.88E+02	3.4E+00	6.8E+00	2.2E+01			---		VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1316-T01-C	1	1.31E+01	E		1.31E+01	5.2E+01	6.8E+00	2.2E+01			---		VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1316-T02-C	1	2.74E+01			2.74E+01	6.9E+00	6.8E+00	2.2E+01	10	100	9.81E+02	95%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1316-T03-C	1	6.72E+01			6.72E+01	5.2E+00	6.8E+00	2.2E+01			---		VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1316-T04-C	1	2.01E+02			2.01E+02	1.2E+00	6.8E+00	2.2E+01			---		VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
Pb	SWA-L01-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	5.1E+01	6.8E+00	2.2E+01			---		VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	SWA-L01-1316-T01-A	1	2.66E+00	E		2.66E+00	5.7E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/23/11 2:03 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L01-1316-T02-A	1	6.26E+00			6.26E+00	7.6E+00	1.9E+00	6.0E+00	10	100	9.86E+02	98%	VU ICP-OES	5/23/11 2:05 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L01-1316-T03-A	1	7.17E+00			7.17E+00	1.5E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/23/11 2:08 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L01-1316-T04-A	1	9.35E+00			9.35E+00	1.0E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/23/11 2:10 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L01-1316-T01-B	1	2.33E+00	E		2.33E+00	1.5E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/23/11 2:12 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L01-1316-T02-B	1	6.15E+00			6.15E+00	2.1E+01	1.9E+00	6.0E+00	10	100	9.99E+02	99%	VU ICP-OES	5/23/11 2:15 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L01-1316-T03-B	1	6.85E+00			6.85E+00	9.9E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/23/11 2:17 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L01-1316-T04-B	1	9.50E+00			9.50E+00	1.0E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/23/11 2:19 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L01-1316-T01-C	1	3.11E+00	E		3.11E+00	3.7E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/23/11 2:21 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L01-1316-T02-C	1	5.94E+00	E		5.94E+00	1.5E+01	1.9E+00	6.0E+00	10	100	9.90E+02	98%	VU ICP-OES	5/23/11 2:23 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L01-1316-T03-C	1	7.01E+00			7.01E+00	2.6E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/23/11 2:25 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L01-1316-T04-C	1	8.47E+00			8.47E+00	1.5E+01	1.9E+00	6.0E+00			---		VU ICP-OES	5/23/11 2:28 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L01-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	5.0E+00	1.9E+00	6.0E+00			---		VU ICP-OES	5/23/11 2:30 PM	EPA Interlab 1316 SWA Reruns

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	SWA-L01-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	2.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00	10	100	1.01E+03	101%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1316-T03-A	1	2.36E+00	E		2.36E+00	5.9E+00	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1316-T04-A	1	6.27E+00	E		6.27E+00	1.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	8.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	7.8E+00	2.0E+00	6.4E+00	10	100	1.01E+03	101%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1316-T03-B	1	2.20E+00	E		2.20E+00	4.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1316-T04-B	1	6.61E+00			6.61E+00	3.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	9.4E+00	2.0E+00	6.4E+00	10	100	9.97E+02	100%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1316-T03-C	1	2.21E+00	E		2.21E+00	8.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1316-T04-C	1	5.24E+00	E		5.24E+00	3.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
Mn	SWA-L01-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	2.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	SWA-L01-1316-T01-A	1	3.64E+00			3.64E+00	1.8E+02	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1316-T02-A	1	4.83E+00			4.83E+00	1.1E+02	1.0E+00	3.2E+00	1000	100	1.09E+03	109%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1316-T03-A	1	7.54E+00			7.54E+00	5.4E+01	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1316-T04-A	1	8.86E+00			8.86E+00	1.5E+02	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1316-T01-B	1	2.71E+00	E		2.71E+00	4.9E+01	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1316-T02-B	1	5.03E+00			5.03E+00	1.7E+02	1.0E+00	3.2E+00	1000	100	1.10E+03	110%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1316-T03-B	1	7.40E+00			7.40E+00	4.6E+01	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1316-T04-B	1	9.74E+00			9.74E+00	6.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1316-T01-C	1	2.74E+00	E		2.74E+00	5.2E+01	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1316-T02-C	1	6.56E+00			6.56E+00	4.2E+01	1.0E+00	3.2E+00	1000	100	1.09E+03	109%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1316-T03-C	1	5.59E+00			5.59E+00	4.5E+01	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1316-T04-C	1	8.33E+00			8.33E+00	6.6E+01	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
Mg	SWA-L01-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	9.3E+01	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	SWA-L01-1316-T01-A	1	1.69E+02			1.69E+02	1.2E+00	1.2E+00	3.8E+00			---		VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1316-T02-A	1	2.72E+02			2.72E+02	1.0E+00	1.2E+00	3.8E+00	10	100	1.39E+03	112%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1316-T03-A	1	7.69E+02			7.69E+02	6.9E-02	1.2E+00	3.8E+00			---		VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1316-T04-A	1	1.32E+03			1.32E+03	6.4E-01	1.2E+00	3.8E+00			---		VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1316-T01-B	1	1.61E+02			1.61E+02	3.1E-01	1.2E+00	3.8E+00			---		VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1316-T02-B	1	3.03E+02			3.03E+02	7.3E-01	1.2E+00	3.8E+00	10	100	1.42E+03	112%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1316-T03-B	1	7.40E+02			7.40E+02	5.3E-01	1.2E+00	3.8E+00			---		VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1316-T04-B	1	1.53E+03			1.53E+03	1.0E+00	1.2E+00	3.8E+00			---		VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1316-T01-C	1	1.68E+02			1.68E+02	3.6E-01	1.2E+00	3.8E+00			---		VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1316-T02-C	1	2.84E+02			2.84E+02	9.3E-01	1.2E+00	3.8E+00	10	100	1.38E+03	110%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1316-T03-C	1	7.24E+02			7.24E+02	6.2E-01	1.2E+00	3.8E+00			---		VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1316-T04-C	1	1.62E+03			1.62E+03	1.2E+00	1.2E+00	3.8E+00			---		VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
Mo	SWA-L01-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	5.1E+01	1.2E+00	3.8E+00			---		VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	SWA-L01-1316-T01-A	1	9.00E-01	U1/2		9.00E-01	5.3E+01	1.8E+00	5.7E+00			---		VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1316-T02-A	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00	10	100	8.74E+02	87%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1316-T03-A	1	2.24E+00	E		2.24E+00	1.8E+01	1.8E+00	5.7E+00			---		VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1316-T04-A	1	6.06E+00			6.06E+00	1.3E+01	1.8E+00	5.7E+00			---		VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1316-T01-B	1	9.00E-01	U1/2		9.00E-01	9.5E+01	1.8E+00	5.7E+00			---		VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1316-T02-B	1	9.00E-01	U1/2		9.00E-01	2.4E+03	1.8E+00	5.7E+00	10	100	8.79E+02	88%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1316-T03-B	1	3.74E+00	E		3.74E+00	2.0E+01	1.8E+00	5.7E+00			---		VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1316-T04-B	1	6.72E+00			6.72E+00	1.8E+01	1.8E+00	5.7E+00			---		VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1316-T01-C	1	9.00E-01	U1/2		9.00E-01	6.1E+02	1.8E+00	5.7E+00			---		VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1316-T02-C	1	9.00E-01	U1/2		9.00E-01	4.2E+03	1.8E+00	5.7E+00	10	100	8.65E+02	86%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1316-T03-C	1	2.69E+00	E		2.69E+00	3.5E+01	1.8E+00	5.7E+00			---		VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1316-T04-C	1	8.90E+00			8.90E+00	1.5E+01	1.8E+00	5.7E+00			---		VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
Ni	SWA-L01-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	1.1E+03	1.8E+00	5.7E+00			---		VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	SWA-L01-1316-T01-A	1	1.80E+01			1.80E+01	4.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1316-T02-A	1	5.68E+01			5.68E+01	7.0E+00	3.7E+00	1.2E+01	1000	100	9.34E+02	88%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1316-T03-A	1	3.39E+02			3.39E+02	1.8E+00	3.7E+00	1.2E+01			---		VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1316-T04-A	1	9.53E+02			9.53E+02	1.1E+00	3.7E+00	1.2E+01			---		VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1316-T01-B	1	1.83E+01			1.83E+01	1.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1316-T02-B	1	5.03E+01			5.03E+01	4.0E+01	3.7E+00	1.2E+01	1000	100	9.64E+02	91%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1316-T03-B	1	3.23E+02			3.23E+02	4.2E+00	3.7E+00	1.2E+01			---		VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1316-T04-B	1	1.31E+03			1.31E+03	7.3E-01	3.7E+00	1.2E+01			---		VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1316-T01-C	1	1.66E+01			1.66E+01	7.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1316-T02-C	1	5.13E+01			5.13E+01	5.2E+00	3.7E+00	1.2E+01	1000	100	9.28E+02	88%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1316-T03-C	1	3.16E+02			3.16E+02	3.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1316-T04-C	1	1.32E+03			1.32E+03	1.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
P	SWA-L01-1316-B01-A	1	8.79E+00	E		8.79E+00	1.6E+01	3.7E+00	1.2E+01			---		VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	SWA-L01-1316-T01-A	1	2.68E+05			2.68E+05	6.5E-01	1.6E+00	5.1E+00			---		VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1316-T02-A	1	4.23E+05			4.23E+05	8.9E-01	1.6E+00	5.1E+00	1000	100	4.24E+05	89%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1316-T03-A	1	1.77E+06			1.77E+06	6.5E-01	1.6E+00	5.1E+00			---		VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1316-T04-A	1	1.85E+06			1.85E+06	2.3E+00	1.6E+00	5.1E+00			---		VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1316-T01-B	1	2.62E+05			2.62E+05	9.1E-01	1.6E+00	5.1E+00			---		VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1316-T02-B	1	4.21E+05			4.21E+05	6.6E-01	1.6E+00	5.1E+00	1000	100	4.22E+05	89%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1316-T03-B	1	1.74E+06			1.74E+06	2.1E-01	1.6E+00	5.1E+00			---		VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1316-T04-B	1	1.85E+06			1.85E+06	9.8E-01	1.6E+00	5.1E+00			---		VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1316-T01-C	1	2.60E+05			2.60E+05	9.3E-01	1.6E+00	5.1E+00			---		VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1316-T02-C	1	4.19E+05			4.19E+05	3.3E+00	1.6E+00	5.1E+00	1000	100	4.20E+05	95%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1316-T03-C	1	1.76E+06			1.76E+06	4.7E-01	1.6E+00	5.1E+00			---		VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1316-T04-C	1	1.87E+06			1.87E+06	8.0E-01	1.6E+00	5.1E+00			---		VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
K	SWA-L01-1316-B01-A	1	8.00E-01	U1/2		8.00E-01	5.6E+01	1.6E+00	5.1E+00			---		VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	SWA-L01-1316-T01-A	1	9.63E+04			9.63E+04	7.9E-01	1.5E+01	4.8E+01			---		VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1316-T02-A	1	1.71E+05			1.71E+05	2.7E-01	1.5E+01	4.8E+01	10	100	1.72E+05	98%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1316-T03-A	1	4.63E+05			4.63E+05	2.6E-01	1.5E+01	4.8E+01			---		VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1316-T04-A	1	7.68E+05			7.68E+05	5.8E-01	1.5E+01	4.8E+01			---		VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1316-T01-B	1	9.58E+04			9.58E+04	5.4E-01	1.5E+01	4.8E+01			---		VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1316-T02-B	1	1.84E+05			1.84E+05	9.8E-01	1.5E+01	4.8E+01	10	100	1.85E+05	85%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1316-T03-B	1	4.48E+05			4.48E+05	4.7E-01	1.5E+01	4.8E+01			---		VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1316-T04-B	1	8.45E+05			8.45E+05	9.0E-01	1.5E+01	4.8E+01			---		VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1316-T01-C	1	9.64E+04			9.64E+04	1.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1316-T02-C	1	1.69E+05			1.69E+05	2.0E-01	1.5E+01	4.8E+01	10	100	1.70E+05	113%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1316-T03-C	1	4.42E+05			4.42E+05	3.9E-01	1.5E+01	4.8E+01			---		VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1316-T04-C	1	9.01E+05			9.01E+05	8.4E-01	1.5E+01	4.8E+01			---		VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
Se	SWA-L01-1316-B01-A	1	7.50E+00	U1/2		7.50E+00	2.3E+02	1.5E+01	4.8E+01			---		VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	SWA-L01-1316-T01-A	1	2.06E+04			2.06E+04	6.7E-01	1.1E+00	3.5E+00			---		VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1316-T02-A	1	2.33E+04			2.33E+04	2.0E-01	1.1E+00	3.5E+00	1000	100	2.43E+04	101%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1316-T03-A	1	3.14E+04			3.14E+04	1.2E+00	1.1E+00	3.5E+00			---		VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1316-T04-A	1	5.23E+04			5.23E+04	9.5E-01	1.1E+00	3.5E+00			---		VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1316-T01-B	1	2.07E+04			2.07E+04	8.9E-01	1.1E+00	3.5E+00			---		VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1316-T02-B	1	2.21E+04			2.21E+04	1.7E+00	1.1E+00	3.5E+00	1000	100	2.32E+04	111%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1316-T03-B	1	3.22E+04			3.22E+04	8.3E-01	1.1E+00	3.5E+00			---		VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1316-T04-B	1	5.75E+04			5.75E+04	3.6E-01	1.1E+00	3.5E+00			---		VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1316-T01-C	1	2.33E+04			2.33E+04	1.1E+00	1.1E+00	3.5E+00			---		VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1316-T02-C	1	2.44E+04			2.44E+04	2.1E+00	1.1E+00	3.5E+00	1000	100	2.55E+04	106%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1316-T03-C	1	2.96E+04			2.96E+04	1.3E+00	1.1E+00	3.5E+00			---		VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1316-T04-C	1	5.42E+04			5.42E+04	1.9E+00	1.1E+00	3.5E+00			---		VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
Si	SWA-L01-1316-B01-A	1	5.50E-01	U1/2		5.50E-01	3.8E-01	1.1E+00	3.5E+00			---		VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	SWA-L01-1316-T01-A	1	4.89E+05			4.89E+05	7.0E-01	2.5E+00	8.0E+00			---		VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1316-T02-A	1	5.15E+05			5.15E+05	4.6E-01	2.5E+00	8.0E+00	1000	100	5.16E+05	89%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1316-T03-A	1	5.27E+05			5.27E+05	9.4E-01	2.5E+00	8.0E+00			---		VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1316-T04-A	1	5.30E+05			5.30E+05	6.4E-01	2.5E+00	8.0E+00			---		VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1316-T01-B	1	4.83E+05			4.83E+05	6.8E-01	2.5E+00	8.0E+00			---		VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1316-T02-B	1	5.17E+05			5.17E+05	2.1E+00	2.5E+00	8.0E+00	1000	100	5.17E+05	85%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1316-T03-B	1	5.30E+05			5.30E+05	2.1E-01	2.5E+00	8.0E+00			---		VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1316-T04-B	1	5.16E+05			5.16E+05	1.5E+00	2.5E+00	8.0E+00			---		VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1316-T01-C	1	4.75E+05			4.75E+05	6.9E-01	2.5E+00	8.0E+00			---		VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1316-T02-C	1	5.17E+05			5.17E+05	7.6E-01	2.5E+00	8.0E+00	1000	100	5.18E+05	87%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1316-T03-C	1	5.26E+05			5.26E+05	2.7E-01	2.5E+00	8.0E+00			---		VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1316-T04-C	1	5.20E+05			5.20E+05	5.8E-01	2.5E+00	8.0E+00			---		VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
Na	SWA-L01-1316-B01-A	1	3.53E+01			3.53E+01	2.1E+01	2.5E+00	8.0E+00			---		VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	SWA-L01-1316-T01-A	1	4.94E+02			4.94E+02	2.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1316-T02-A	1	4.69E+02			4.69E+02	1.1E+00	1.0E+00	3.2E+00	1000	100	1.56E+03	109%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1316-T03-A	1	4.76E+02			4.76E+02	8.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1316-T04-A	1	5.14E+02			5.14E+02	2.5E+00	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1316-T01-B	1	4.59E+02			4.59E+02	5.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1316-T02-B	1	4.59E+02			4.59E+02	3.4E-01	1.0E+00	3.2E+00	1000	100	1.52E+03	106%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1316-T03-B	1	4.73E+02			4.73E+02	7.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1316-T04-B	1	5.56E+02			5.56E+02	1.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1316-T01-C	1	4.33E+02			4.33E+02	1.7E+00	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1316-T02-C	1	4.48E+02			4.48E+02	5.2E-01	1.0E+00	3.2E+00	1000	100	1.48E+03	104%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1316-T03-C	1	4.66E+02			4.66E+02	9.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1316-T04-C	1	5.23E+02			5.23E+02	5.7E-01	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
Sr	SWA-L01-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	2.6E+01	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	SWA-L01-1316-T01-A	1	7.86E+05			7.86E+05	9.0E-01	6.8E+00	2.2E+01			---		VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1316-T02-A	1	5.30E+05			5.30E+05	1.5E-01	6.8E+00	2.2E+01	1000	100	6.21E+05	91%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1316-T03-A	1	1.52E+06			1.52E+06	4.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1316-T04-A	1	2.01E+06			2.01E+06	1.0E+00	6.8E+00	2.2E+01			---		VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1316-T01-B	1	7.91E+05			7.91E+05	4.4E-01	6.8E+00	2.2E+01			---		VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1316-T02-B	1	5.67E+05			5.67E+05	9.8E-01	6.8E+00	2.2E+01	1000	100	6.59E+05	91%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1316-T03-B	1	1.38E+06			1.38E+06	3.9E-01	6.8E+00	2.2E+01			---		VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1316-T04-B	1	2.00E+06			2.00E+06	1.3E+00	6.8E+00	2.2E+01			---		VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1316-T01-C	1	8.10E+05			8.10E+05	1.2E+00	6.8E+00	2.2E+01			---		VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1316-T02-C	1	5.43E+05			5.43E+05	3.5E-01	6.8E+00	2.2E+01	1000	100	6.29E+05	86%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1316-T03-C	1	1.57E+06			1.57E+06	3.5E-01	6.8E+00	2.2E+01			---		VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1316-T04-C	1	2.12E+06			2.12E+06	9.6E-01	6.8E+00	2.2E+01			---		VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
S	SWA-L01-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	1.4E+01	6.8E+00	2.2E+01			---		VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	SWA-L01-1316-T01-A	1	2.30E+00	U1/2		2.30E+00	7.1E+01	4.6E+00	1.5E+01			---		VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1316-T02-A	1	2.30E+00	U1/2		2.30E+00	4.8E+02	4.6E+00	1.5E+01	10	100	8.77E+02	88%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1316-T03-A	1	2.30E+00	U1/2		2.30E+00	3.2E+02	4.6E+00	1.5E+01			---		VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1316-T04-A	1	2.30E+00	U1/2		2.30E+00	4.3E+02	4.6E+00	1.5E+01			---		VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1316-T01-B	1	2.30E+00	U1/2		2.30E+00	3.6E+01	4.6E+00	1.5E+01			---		VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1316-T02-B	1	2.30E+00	U1/2		2.30E+00	4.9E+01	4.6E+00	1.5E+01	10	100	8.76E+02	87%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1316-T03-B	1	2.30E+00	U1/2		2.30E+00	5.7E+01	4.6E+00	1.5E+01			---		VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1316-T04-B	1	2.30E+00	U1/2		2.30E+00	7.1E+02	4.6E+00	1.5E+01			---		VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1316-T01-C	1	2.30E+00	U1/2		2.30E+00	4.4E+01	4.6E+00	1.5E+01			---		VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1316-T02-C	1	2.30E+00	U1/2		2.30E+00	6.0E+01	4.6E+00	1.5E+01	10	100	8.62E+02	86%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1316-T03-C	1	2.30E+00	U1/2		2.30E+00	5.8E+01	4.6E+00	1.5E+01			---		VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1316-T04-C	1	2.30E+00	U1/2		2.30E+00	2.3E+02	4.6E+00	1.5E+01			---		VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
Tl	SWA-L01-1316-B01-A	1	2.30E+00	U1/2		2.30E+00	2.4E+01	4.6E+00	1.5E+01			---		VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	SWA-L01-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	2.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00	10	100	1.15E+03	115%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1316-T03-A	1	2.52E+00	E		2.52E+00	7.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1316-T04-A	1	6.06E+00	E		6.06E+00	1.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	3.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00	10	100	1.17E+03	117%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1316-T03-B	1	2.34E+00	E		2.34E+00	6.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1316-T04-B	1	8.00E+00			8.00E+00	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	3.3E+01	2.0E+00	6.4E+00	10	100	1.15E+03	115%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1316-T03-C	1	2.44E+00	E		2.44E+00	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1316-T04-C	1	6.76E+00			6.76E+00	4.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
Ti	SWA-L01-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	5.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	SWA-L01-1316-T01-A	1	3.31E+02			3.31E+02	5.3E-01	1.5E+00	4.8E+00			---		VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1316-T02-A	1	4.88E+02			4.88E+02	9.0E-01	1.5E+00	4.8E+00	10	100	1.52E+03	103%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1316-T03-A	1	1.18E+03			1.18E+03	2.7E-01	1.5E+00	4.8E+00			---		VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1316-T04-A	1	1.99E+03			1.99E+03	4.8E-01	1.5E+00	4.8E+00			---		VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1316-T01-B	1	3.41E+02			3.41E+02	1.0E+00	1.5E+00	4.8E+00			---		VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1316-T02-B	1	5.16E+02			5.16E+02	8.6E-01	1.5E+00	4.8E+00	10	100	1.56E+03	105%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1316-T03-B	1	1.13E+03			1.13E+03	9.2E-01	1.5E+00	4.8E+00			---		VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1316-T04-B	1	2.05E+03			2.05E+03	3.1E-01	1.5E+00	4.8E+00			---		VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1316-T01-C	1	3.68E+02			3.68E+02	1.7E+00	1.5E+00	4.8E+00			---		VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1316-T02-C	1	4.90E+02			4.90E+02	7.5E-01	1.5E+00	4.8E+00	10	100	1.52E+03	103%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1316-T03-C	1	1.27E+03			1.27E+03	1.8E-01	1.5E+00	4.8E+00			---		VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1316-T04-C	1	2.25E+03			2.25E+03	5.4E-01	1.5E+00	4.8E+00			---		VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
V	SWA-L01-1316-B01-A	1	7.50E-01	U1/2		7.50E-01	3.5E+01	1.5E+00	4.8E+00			---		VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	SWA-L01-1316-T01-A	1	1.23E+01			1.23E+01	2.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 10:42 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1316-T02-A	1	1.33E+01			1.33E+01	1.7E+00	1.0E+00	3.2E+00	10	100	1.01E+03	100%	VU ICP-OES	10/29/10 10:44 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1316-T03-A	1	1.64E+01			1.64E+01	1.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 10:46 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1316-T04-A	1	2.77E+01			2.77E+01	2.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 11:03 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1316-T01-B	1	1.29E+01			1.29E+01	4.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 10:49 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1316-T02-B	1	1.30E+01			1.30E+01	3.7E+00	1.0E+00	3.2E+00	10	100	1.02E+03	101%	VU ICP-OES	10/29/10 10:51 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1316-T03-B	1	1.47E+01			1.47E+01	3.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 10:53 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1316-T04-B	1	3.34E+01			3.34E+01	2.2E-01	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 10:55 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1316-T01-C	1	1.34E+01			1.34E+01	7.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 10:56 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1316-T02-C	1	1.34E+01			1.34E+01	2.6E+00	1.0E+00	3.2E+00	10	100	1.00E+03	99%	VU ICP-OES	10/29/10 10:58 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1316-T03-C	1	1.46E+01			1.46E+01	4.9E+00	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 11:00 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1316-T04-C	1	3.10E+01			3.10E+01	3.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 11:01 AM	EPA Interlab L01 1313-1316 SWA
Zn	SWA-L01-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	7.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	10/29/10 10:41 AM	EPA Interlab L01 1313-1316 SWA

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	SWA-L02-1316-T01-A	1	3.51E+04			3.51E+04	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1316-T02-A	1	6.80E+04			6.80E+04	7.1E-01	1.0E+00	3.2E+00	1000	125	6.91E+04	87%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1316-T03-A	1	1.38E+05			1.38E+05	3.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1316-T04-A	1	2.05E+05			2.05E+05	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1316-T05-A	1	1.77E+05			1.77E+05	6.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1316-T01-B	1	4.33E+04			4.33E+04	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1316-T02-B	1	6.95E+04			6.95E+04	1.4E+00	1.0E+00	3.2E+00	1000	125	7.09E+04	111%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1316-T03-B	1	1.28E+05			1.28E+05	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1316-T04-B	1	2.07E+05			2.07E+05	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1316-T05-B	1	1.83E+05			1.83E+05	7.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1316-T01-C	1	4.21E+04			4.21E+04	9.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1316-T02-C	1	6.91E+04			6.91E+04	4.5E-01	1.0E+00	3.2E+00	1000	125	7.03E+04	98%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1316-T03-C	1	1.39E+05			1.39E+05	3.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1316-T04-C	1	1.96E+05			1.96E+05	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1316-T05-C	1	1.73E+05			1.73E+05	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
Al	SWA-L02-1316-B01-A	1	2.85E+02			2.85E+02	6.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	SWA-L02-1316-T01-A	1	3.85E+03			3.85E+03	7.2E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1316-T02-A	1	2.37E+03			2.37E+03	7.5E-01	7.5E+00	2.4E+01	10	125	3.61E+03	99%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1316-T03-A	1	3.62E+03			3.62E+03	3.3E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1316-T04-A	1	6.16E+03			6.16E+03	2.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1316-T05-A	1	6.70E+03			6.70E+03	1.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1316-T01-B	1	4.11E+03			4.11E+03	4.5E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1316-T02-B	1	2.67E+03			2.67E+03	1.6E+00	7.5E+00	2.4E+01	10	125	3.86E+03	95%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1316-T03-B	1	3.54E+03			3.54E+03	3.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1316-T04-B	1	6.31E+03			6.31E+03	5.5E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1316-T05-B	1	6.88E+03			6.88E+03	3.6E-01	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1316-T01-C	1	3.90E+03			3.90E+03	1.4E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1316-T02-C	1	2.74E+03			2.74E+03	1.2E+00	7.5E+00	2.4E+01	10	125	3.98E+03	99%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1316-T03-C	1	3.55E+03			3.55E+03	1.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1316-T04-C	1	6.02E+03			6.02E+03	2.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1316-T05-C	1	6.90E+03			6.90E+03	1.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
Sb	SWA-L02-1316-B01-A	1	3.75E+00	U1/2		3.75E+00	2.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	SWA-L02-1316-T01-A	1	5.04E+03			5.04E+03	7.8E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1316-T02-A	1	1.45E+04			1.45E+04	1.7E+00	1.1E+01	3.5E+01	10	125	1.55E+04	85%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1316-T03-A	1	3.76E+04			3.76E+04	2.5E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1316-T04-A	1	5.59E+04			5.59E+04	1.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1316-T05-A	1	1.61E+05			1.61E+05	1.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1316-T01-B	1	7.38E+03			7.38E+03	3.8E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1316-T02-B	1	1.50E+04			1.50E+04	1.5E+00	1.1E+01	3.5E+01	10	125	1.61E+04	88%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1316-T03-B	1	3.47E+04			3.47E+04	1.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1316-T04-B	1	5.71E+04			5.71E+04	9.0E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1316-T05-B	1	8.00E+04			8.00E+04	1.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1316-T01-C	1	7.65E+03			7.65E+03	4.3E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1316-T02-C	1	1.52E+04			1.52E+04	1.2E+00	1.1E+01	3.5E+01	10	125	1.63E+04	91%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1316-T03-C	1	3.93E+04			3.93E+04	4.1E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1316-T04-C	1	4.88E+04			4.88E+04	7.6E-01	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1316-T05-C	1	1.67E+05			1.67E+05	1.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
As	SWA-L02-1316-B01-A	1	5.50E+00	U1/2		5.50E+00	1.1E+01	1.1E+01	3.5E+01				---	VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	SWA-L02-1316-T01-A	1	1.01E+03			1.01E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1316-T02-A	1	9.61E+02			9.61E+02	1.5E+00	1.0E+00	3.2E+00	1000	125	2.13E+03	94%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1316-T03-A	1	6.29E+02			6.29E+02	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1316-T04-A	1	8.36E+02			8.36E+02	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1316-T05-A	1	9.53E+02			9.53E+02	7.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1316-T01-B	1	1.06E+03			1.06E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1316-T02-B	1	9.86E+02			9.86E+02	6.3E-01	1.0E+00	3.2E+00	1000	125	2.29E+03	104%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1316-T03-B	1	6.51E+02			6.51E+02	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1316-T04-B	1	8.59E+02			8.59E+02	9.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1316-T05-B	1	9.94E+02			9.94E+02	1.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1316-T01-C	1	1.02E+03			1.02E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1316-T02-C	1	9.93E+02			9.93E+02	9.8E-01	1.0E+00	3.2E+00	1000	125	2.29E+03	104%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1316-T03-C	1	6.49E+02			6.49E+02	1.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1316-T04-C	1	8.14E+02			8.14E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1316-T05-C	1	9.83E+02			9.83E+02	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
B	SWA-L02-1316-B01-A	1	1.98E+01			1.98E+01	4.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	SWA-L02-1316-T01-A	1	1.60E+02			1.60E+02	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1316-T02-A	1	1.73E+02			1.73E+02	5.7E-01	1.0E+00	3.2E+00	10	125	1.24E+03	85%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1316-T03-A	1	1.65E+02			1.65E+02	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1316-T04-A	1	1.21E+02			1.21E+02	7.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1316-T05-A	1	1.55E+02			1.55E+02	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1316-T01-B	1	1.95E+02			1.95E+02	3.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1316-T02-B	1	1.79E+02			1.79E+02	1.2E+00	1.0E+00	3.2E+00	10	125	1.35E+03	93%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1316-T03-B	1	1.59E+02			1.59E+02	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1316-T04-B	1	1.18E+02			1.18E+02	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1316-T05-B	1	1.64E+02			1.64E+02	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1316-T01-C	1	1.80E+02			1.80E+02	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1316-T02-C	1	1.75E+02			1.75E+02	4.5E-01	1.0E+00	3.2E+00	10	125	1.35E+03	94%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1316-T03-C	1	1.68E+02			1.68E+02	4.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1316-T04-C	1	1.28E+02			1.28E+02	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1316-T05-C	1	1.50E+02			1.50E+02	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
Ba	SWA-L02-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	7.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	SWA-L02-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	9.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	3.6E+01	1.9E+00	6.0E+00	10	125	1.34E+03	107%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	1.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	1.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1316-T05-A	1	9.50E-01	U1/2		9.50E-01	8.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	2.5E+01	1.9E+00	6.0E+00	10	125	1.47E+03	117%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	3.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	1.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1316-T05-B	1	9.50E-01	U1/2		9.50E-01	6.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	2.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	3.8E+01	1.9E+00	6.0E+00	10	125	1.49E+03	119%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	3.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	2.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1316-T05-C	1	9.50E-01	U1/2		9.50E-01	3.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
Be	SWA-L02-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	4.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	SWA-L02-1316-T01-A	1	1.10E+00	U1/2		1.10E+00	3.7E+01	2.2E+00	7.0E+00			---		VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1316-T02-A	1	1.10E+00	U1/2		1.10E+00	1.0E+02	2.2E+00	7.0E+00	10	125	1.21E+03	96%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1316-T03-A	1	1.10E+00	U1/2		1.10E+00	1.4E+02	2.2E+00	7.0E+00			---		VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1316-T04-A	1	1.10E+00	U1/2		1.10E+00	2.9E+02	2.2E+00	7.0E+00			---		VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1316-T05-A	1	1.10E+00	U1/2		1.10E+00	3.3E+02	2.2E+00	7.0E+00			---		VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1316-T01-B	1	1.10E+00	U1/2		1.10E+00	1.5E+02	2.2E+00	7.0E+00			---		VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1316-T02-B	1	1.10E+00	U1/2		1.10E+00	5.7E+01	2.2E+00	7.0E+00	10	125	1.31E+03	105%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1316-T03-B	1	1.10E+00	U1/2		1.10E+00	4.5E+01	2.2E+00	7.0E+00			---		VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1316-T04-B	1	1.10E+00	U1/2		1.10E+00	1.6E+01	2.2E+00	7.0E+00			---		VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1316-T05-B	1	1.10E+00	U1/2		1.10E+00	5.7E+01	2.2E+00	7.0E+00			---		VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1316-T01-C	1	1.10E+00	U1/2		1.10E+00	5.0E+01	2.2E+00	7.0E+00			---		VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1316-T02-C	1	1.10E+00	U1/2		1.10E+00	2.0E+02	2.2E+00	7.0E+00	10	125	1.32E+03	106%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1316-T03-C	1	1.10E+00	U1/2		1.10E+00	3.9E+01	2.2E+00	7.0E+00			---		VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1316-T04-C	1	1.10E+00	U1/2		1.10E+00	7.0E+02	2.2E+00	7.0E+00			---		VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1316-T05-C	1	1.10E+00	U1/2		1.10E+00	2.5E+02	2.2E+00	7.0E+00			---		VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
Cd	SWA-L02-1316-B01-A	1	1.10E+00	U1/2		1.10E+00	3.5E+02	2.2E+00	7.0E+00			---		VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	SWA-L02-1316-T01-A	1	1.53E+04			1.53E+04	6.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1316-T02-A	1	1.02E+04			1.02E+04	7.0E-01	2.6E+00	8.3E+00	1000	125	1.13E+04	87%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1316-T03-A	1	6.52E+03			6.52E+03	1.6E+00	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1316-T04-A	1	5.54E+03			5.54E+03	6.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1316-T05-A	1	5.25E+03			5.25E+03	1.7E+00	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1316-T01-B	1	1.59E+04			1.59E+04	6.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1316-T02-B	1	1.06E+04			1.06E+04	1.1E+00	2.6E+00	8.3E+00	1000	125	1.17E+04	89%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1316-T03-B	1	6.49E+03			6.49E+03	1.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1316-T04-B	1	5.42E+03			5.42E+03	3.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1316-T05-B	1	5.64E+03			5.64E+03	1.9E+00	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1316-T01-C	1	1.52E+04			1.52E+04	1.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1316-T02-C	1	1.07E+04			1.07E+04	4.3E-01	2.6E+00	8.3E+00	1000	125	1.18E+04	92%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1316-T03-C	1	6.65E+03			6.65E+03	8.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1316-T04-C	1	6.19E+03			6.19E+03	1.7E+00	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1316-T05-C	1	5.49E+03			5.49E+03	6.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
Ca	SWA-L02-1316-B01-A	1	3.51E+03			3.51E+03	9.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	SWA-L02-1316-T01-A	1	1.16E+03			1.16E+03	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1316-T02-A	1	2.09E+03			2.09E+03	1.2E+00	1.2E+00	3.8E+00	10	125	3.24E+03	92%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1316-T03-A	1	2.16E+03			2.16E+03	5.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1316-T04-A	1	2.54E+03			2.54E+03	7.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1316-T05-A	1	2.98E+03			2.98E+03	5.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1316-T01-B	1	1.41E+03			1.41E+03	8.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1316-T02-B	1	2.14E+03			2.14E+03	1.5E+00	1.2E+00	3.8E+00	10	125	3.45E+03	105%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1316-T03-B	1	2.06E+03			2.06E+03	1.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1316-T04-B	1	2.67E+03			2.67E+03	1.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1316-T05-B	1	2.84E+03			2.84E+03	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1316-T01-C	1	1.31E+03			1.31E+03	7.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1316-T02-C	1	2.13E+03			2.13E+03	5.9E-01	1.2E+00	3.8E+00	10	125	3.49E+03	109%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1316-T03-C	1	2.21E+03			2.21E+03	6.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1316-T04-C	1	2.57E+03			2.57E+03	6.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1316-T05-C	1	2.96E+03			2.96E+03	1.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
Cr	SWA-L02-1316-B01-A	1	1.28E+00	E		1.28E+00	1.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	SWA-L02-1316-T01-A	1	9.00E-01	U1/2		9.00E-01	2.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1316-T02-A	1	9.00E-01	U1/2		9.00E-01	1.7E+02	1.8E+00	5.7E+00	10	125	1.19E+03	95%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1316-T03-A	1	2.39E+00	E		2.39E+00	3.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1316-T04-A	1	2.81E+00	E		2.81E+00	6.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1316-T05-A	1	4.24E+00			4.24E+00	5.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1316-T01-B	1	9.00E-01	U1/2		9.00E-01	9.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1316-T02-B	1	9.00E-01	U1/2		9.00E-01	3.9E+01	1.8E+00	5.7E+00	10	125	1.29E+03	103%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1316-T03-B	1	2.48E+00	E		2.48E+00	1.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1316-T04-B	1	3.01E+00	E		3.01E+00	1.2E+02	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1316-T05-B	1	4.18E+00			4.18E+00	6.9E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1316-T01-C	1	9.00E-01	U1/2		9.00E-01	6.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1316-T02-C	1	9.00E-01	U1/2		9.00E-01	2.1E+02	1.8E+00	5.7E+00	10	125	1.31E+03	105%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1316-T03-C	1	2.75E+00	E		2.75E+00	3.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1316-T04-C	1	2.23E+00	E		2.23E+00	2.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1316-T05-C	1	3.14E+00			3.14E+00	2.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
Co	SWA-L02-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	8.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	SWA-L02-1316-T01-A	1	1.85E+00	U1/2		1.85E+00	7.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1316-T02-A	1	5.43E+00	E		5.43E+00	3.6E+01	3.7E+00	1.2E+01	10	125	1.23E+03	98%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1316-T03-A	1	6.13E+00	E		6.13E+00	3.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1316-T04-A	1	5.79E+00	E		5.79E+00	5.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1316-T05-A	1	2.59E+01			2.59E+01	1.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1316-T01-B	1	1.85E+00	U1/2		1.85E+00	5.6E+01	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1316-T02-B	1	6.89E+00	E		6.89E+00	7.4E+01	3.7E+00	1.2E+01	10	125	1.33E+03	106%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1316-T03-B	1	5.30E+00	E		5.30E+00	3.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1316-T04-B	1	6.16E+00	E		6.16E+00	7.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1316-T05-B	1	2.57E+01			2.57E+01	5.1E+00	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1316-T01-C	1	1.85E+00	U1/2		1.85E+00	2.9E+02	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1316-T02-C	1	5.77E+00	E		5.77E+00	4.8E+01	3.7E+00	1.2E+01	10	125	1.35E+03	108%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1316-T03-C	1	5.76E+00	E		5.76E+00	7.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1316-T04-C	1	6.80E+00	E		6.80E+00	5.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1316-T05-C	1	2.92E+01			2.92E+01	6.9E+00	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
Cu	SWA-L02-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	2.3E+01	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	SWA-L02-1316-T01-A	1	1.68E+02			1.68E+02	1.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1316-T02-A	1	3.15E+02			3.15E+02	5.6E-01	2.0E+00	6.4E+00	1000	125	1.47E+03	92%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1316-T03-A	1	8.33E+02			8.33E+02	5.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1316-T04-A	1	1.83E+03			1.83E+03	1.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1316-T05-A	1	1.45E+03			1.45E+03	8.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1316-T01-B	1	1.14E+02			1.14E+02	7.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1316-T02-B	1	3.08E+02			3.08E+02	2.4E+00	2.0E+00	6.4E+00	1000	125	1.49E+03	94%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1316-T03-B	1	8.02E+02			8.02E+02	1.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1316-T04-B	1	2.00E+03			2.00E+03	5.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1316-T05-B	1	1.49E+03			1.49E+03	1.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1316-T01-C	1	1.25E+02			1.25E+02	1.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1316-T02-C	1	2.77E+02			2.77E+02	4.7E-01	2.0E+00	6.4E+00	1000	125	1.41E+03	91%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1316-T03-C	1	8.57E+02			8.57E+02	5.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1316-T04-C	1	1.79E+03			1.79E+03	3.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1316-T05-C	1	1.44E+03			1.44E+03	1.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
Fe	SWA-L02-1316-B01-A	1	7.39E+01			7.39E+01	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	SWA-L02-1316-T01-A	1	1.83E+01	E		1.83E+01	2.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1316-T02-A	1	4.18E+01			4.18E+01	1.5E+01	6.8E+00	2.2E+01	10	125	1.23E+03	95%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1316-T03-A	1	7.19E+01			7.19E+01	1.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1316-T04-A	1	6.43E+01			6.43E+01	3.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1316-T05-A	1	1.61E+02			1.61E+02	3.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1316-T01-B	1	2.48E+01			2.48E+01	1.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1316-T02-B	1	4.26E+01			4.26E+01	2.1E+01	6.8E+00	2.2E+01	10	125	1.34E+03	104%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1316-T03-B	1	8.27E+01			8.27E+01	3.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1316-T04-B	1	6.60E+01			6.60E+01	7.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1316-T05-B	1	1.79E+02			1.79E+02	6.3E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1316-T01-C	1	2.78E+01			2.78E+01	1.7E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1316-T02-C	1	4.58E+01			4.58E+01	8.7E+00	6.8E+00	2.2E+01	10	125	1.36E+03	105%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1316-T03-C	1	9.08E+01			9.08E+01	1.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1316-T04-C	1	5.75E+01			5.75E+01	9.3E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1316-T05-C	1	1.54E+02			1.54E+02	5.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
Pb	SWA-L02-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	3.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	SWA-L02-1316-T01-A	1	4.00E+00	E		4.00E+00	8.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1316-T02-A	1	7.45E+00			7.45E+00	1.1E+01	1.9E+00	6.0E+00	10	125	1.10E+03	87%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1316-T03-A	1	9.12E+00			9.12E+00	4.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1316-T04-A	1	1.12E+01			1.12E+01	3.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1316-T05-A	1	1.23E+01			1.23E+01	3.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1316-T01-B	1	3.60E+00	E		3.60E+00	1.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1316-T02-B	1	7.38E+00			7.38E+00	1.6E+01	1.9E+00	6.0E+00	10	125	1.17E+03	93%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1316-T03-B	1	9.06E+00			9.06E+00	1.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1316-T04-B	1	1.27E+01			1.27E+01	2.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1316-T05-B	1	1.07E+01			1.07E+01	3.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1316-T01-C	1	4.07E+00	E		4.07E+00	2.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1316-T02-C	1	6.57E+00			6.57E+00	8.3E+01	1.9E+00	6.0E+00	10	125	1.19E+03	94%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1316-T03-C	1	1.02E+01			1.02E+01	3.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1316-T04-C	1	1.29E+01			1.29E+01	2.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1316-T05-C	1	1.27E+01			1.27E+01	4.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
Li	SWA-L02-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	4.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	SWA-L02-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	2.3E-01	2.0E+00	6.4E+00			---		VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	2.2E+00	2.0E+00	6.4E+00	10	125	1.18E+03	94%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	9.2E-01	2.0E+00	6.4E+00			---		VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1316-T04-A	1	5.69E+00	E		5.69E+00	7.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1316-T05-A	1	4.40E+00	E		4.40E+00	4.0E-01	2.0E+00	6.4E+00			---		VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	2.9E+00	2.0E+00	6.4E+00			---		VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	2.7E+00	2.0E+00	6.4E+00	10	125	1.28E+03	103%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	6.5E-01	2.0E+00	6.4E+00			---		VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1316-T04-B	1	5.48E+00	E		5.48E+00	6.6E-01	2.0E+00	6.4E+00			---		VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1316-T05-B	1	4.29E+00	E		4.29E+00	1.8E+00	2.0E+00	6.4E+00			---		VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	3.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	2.2E+00	2.0E+00	6.4E+00	10	125	1.29E+03	103%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	1.9E+00	2.0E+00	6.4E+00			---		VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1316-T04-C	1	6.90E+00			6.90E+00	5.6E-01	2.0E+00	6.4E+00			---		VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1316-T05-C	1	5.42E+00	E		5.42E+00	2.0E+00	2.0E+00	6.4E+00			---		VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
Mn	SWA-L02-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	2.9E+01	2.0E+00	6.4E+00			---		VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	SWA-L02-1316-T01-A	1	5.00E-01	U1/2		5.00E-01	2.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1316-T02-A	1	5.00E-01	U1/2		5.00E-01	1.6E+00	1.0E+00	3.2E+00	1000	125	1.13E+03	90%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1316-T03-A	1	7.30E+00			7.30E+00	3.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1316-T04-A	1	1.01E+01			1.01E+01	4.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1316-T05-A	1	9.09E+00			9.09E+00	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1316-T01-B	1	5.00E-01	U1/2		5.00E-01	2.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1316-T02-B	1	5.00E-01	U1/2		5.00E-01	2.7E+00	1.0E+00	3.2E+00	1000	125	1.17E+03	94%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1316-T03-B	1	5.88E+00			5.88E+00	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1316-T04-B	1	1.06E+01			1.06E+01	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1316-T05-B	1	1.06E+01			1.06E+01	3.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1316-T01-C	1	5.00E-01	U1/2		5.00E-01	2.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1316-T02-C	1	5.00E-01	U1/2		5.00E-01	3.5E+00	1.0E+00	3.2E+00	1000	125	1.16E+03	93%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1316-T03-C	1	6.91E+00			6.91E+00	3.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1316-T04-C	1	9.49E+00			9.49E+00	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1316-T05-C	1	9.45E+00			9.45E+00	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
Mg	SWA-L02-1316-B01-A	1	2.72E+01			2.72E+01	2.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	SWA-L02-1316-T01-A	1	2.34E+02			2.34E+02	7.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1316-T02-A	1	3.79E+02			3.79E+02	3.3E-01	1.2E+00	3.8E+00	10	125	1.56E+03	95%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1316-T03-A	1	7.28E+02			7.28E+02	7.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1316-T04-A	1	1.04E+03			1.04E+03	8.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1316-T05-A	1	1.08E+03			1.08E+03	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1316-T01-B	1	2.48E+02			2.48E+02	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1316-T02-B	1	4.00E+02			4.00E+02	1.6E+00	1.2E+00	3.8E+00	10	125	1.52E+03	89%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1316-T03-B	1	6.91E+02			6.91E+02	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1316-T04-B	1	1.07E+03			1.07E+03	9.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1316-T05-B	1	1.14E+03			1.14E+03	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1316-T01-C	1	2.41E+02			2.41E+02	5.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1316-T02-C	1	3.96E+02			3.96E+02	7.8E-01	1.2E+00	3.8E+00	10	125	1.53E+03	91%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1316-T03-C	1	7.63E+02			7.63E+02	1.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1316-T04-C	1	1.01E+03			1.01E+03	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1316-T05-C	1	1.12E+03			1.12E+03	8.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
Mo	SWA-L02-1316-B01-A	1	2.12E+00	E		2.12E+00	5.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	SWA-L02-1316-T01-A	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00			---		VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1316-T02-A	1	1.87E+00	E		1.87E+00	1.7E+02	1.8E+00	5.7E+00	10	125	1.16E+03	93%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1316-T03-A	1	2.40E+00	E		2.40E+00	2.7E+01	1.8E+00	5.7E+00			---		VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1316-T04-A	1	9.46E+00			9.46E+00	3.3E+01	1.8E+00	5.7E+00			---		VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1316-T05-A	1	7.14E+00			7.14E+00	4.2E+01	1.8E+00	5.7E+00			---		VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1316-T01-B	1	9.00E-01	U1/2		9.00E-01	2.2E+02	1.8E+00	5.7E+00			---		VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1316-T02-B	1	3.08E+00	E		3.08E+00	1.5E+02	1.8E+00	5.7E+00	10	125	1.26E+03	101%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1316-T03-B	1	2.99E+00	E		2.99E+00	4.7E+01	1.8E+00	5.7E+00			---		VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1316-T04-B	1	1.17E+01			1.17E+01	2.5E+01	1.8E+00	5.7E+00			---		VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1316-T05-B	1	6.60E+00			6.60E+00	4.0E+01	1.8E+00	5.7E+00			---		VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1316-T01-C	1	9.00E-01	U1/2		9.00E-01	2.0E+02	1.8E+00	5.7E+00			---		VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1316-T02-C	1	2.57E+00	E		2.57E+00	4.5E+01	1.8E+00	5.7E+00	10	125	1.28E+03	102%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1316-T03-C	1	2.32E+00	E		2.32E+00	5.0E+01	1.8E+00	5.7E+00			---		VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1316-T04-C	1	9.12E+00			9.12E+00	1.8E+01	1.8E+00	5.7E+00			---		VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1316-T05-C	1	4.75E+00	E		4.75E+00	3.3E+01	1.8E+00	5.7E+00			---		VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
Ni	SWA-L02-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	2.8E+02	1.8E+00	5.7E+00			---		VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	SWA-L02-1316-T01-A	1	7.62E+01			7.62E+01	5.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1316-T02-A	1	1.47E+02			1.47E+02	7.0E+00	3.7E+00	1.2E+01	1000	125	1.32E+03	94%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1316-T03-A	1	5.91E+02			5.91E+02	3.1E+00	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1316-T04-A	1	1.71E+03			1.71E+03	2.2E+00	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1316-T05-A	1	1.12E+03			1.12E+03	2.3E+00	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1316-T01-B	1	6.91E+01			6.91E+01	3.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1316-T02-B	1	1.53E+02			1.53E+02	3.3E+00	3.7E+00	1.2E+01	1000	125	1.49E+03	107%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1316-T03-B	1	5.36E+02			5.36E+02	5.6E+00	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1316-T04-B	1	1.75E+03			1.75E+03	8.1E-01	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1316-T05-B	1	1.19E+03			1.19E+03	1.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1316-T01-C	1	7.99E+01			7.99E+01	2.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1316-T02-C	1	1.48E+02			1.48E+02	2.0E+01	3.7E+00	1.2E+01	1000	125	1.42E+03	102%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1316-T03-C	1	5.75E+02			5.75E+02	5.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1316-T04-C	1	1.66E+03			1.66E+03	2.0E+00	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1316-T05-C	1	1.13E+03			1.13E+03	6.7E-01	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
P	SWA-L02-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	5.4E+01	3.7E+00	1.2E+01			---		VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	SWA-L02-1316-T01-A	1	3.69E+05			3.69E+05	9.2E-01	1.6E+00	5.1E+00			---		VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1316-T02-A	1	6.47E+05			6.47E+05	9.8E-01	1.6E+00	5.1E+00	1000	125	6.48E+05	86%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1316-T03-A	1	1.19E+06			1.19E+06	1.0E+01	1.6E+00	5.1E+00			---		VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1316-T04-A	1	3.48E+06			3.48E+06	5.4E-01	1.6E+00	5.1E+00			---		VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1316-T05-A	1	3.45E+06			3.45E+06	1.1E+00	1.6E+00	5.1E+00			---		VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1316-T01-B	1	4.49E+05			4.49E+05	3.9E-01	1.6E+00	5.1E+00			---		VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1316-T02-B	1	6.51E+05			6.51E+05	2.6E+00	1.6E+00	5.1E+00	1000	125	6.53E+05	91%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1316-T03-B	1	1.08E+06			1.08E+06	1.7E+00	1.6E+00	5.1E+00			---		VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1316-T04-B	1	3.57E+06			3.57E+06	9.9E-01	1.6E+00	5.1E+00			---		VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1316-T05-B	1	3.57E+06			3.57E+06	2.4E-01	1.6E+00	5.1E+00			---		VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1316-T01-C	1	4.35E+05			4.35E+05	1.0E+00	1.6E+00	5.1E+00			---		VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1316-T02-C	1	6.59E+05			6.59E+05	1.9E-01	1.6E+00	5.1E+00	1000	125	6.60E+05	84%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1316-T03-C	1	1.30E+06			1.30E+06	1.2E+01	1.6E+00	5.1E+00			---		VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1316-T04-C	1	3.49E+06			3.49E+06	7.7E-01	1.6E+00	5.1E+00			---		VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1316-T05-C	1	3.44E+06			3.44E+06	2.2E-01	1.6E+00	5.1E+00			---		VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
K	SWA-L02-1316-B01-A	1	2.21E+02			2.21E+02	8.4E+00	1.6E+00	5.1E+00			---		VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	SWA-L02-1316-T01-A	1	1.18E+05			1.18E+05	1.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1316-T02-A	1	2.49E+05			2.49E+05	7.5E-01	1.5E+01	4.8E+01	10	125	2.50E+05	88%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1316-T03-A	1	6.01E+05			6.01E+05	5.5E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1316-T04-A	1	1.14E+06			1.14E+06	1.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1316-T05-A	1	8.03E+05			8.03E+05	6.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1316-T01-B	1	1.55E+05			1.55E+05	5.1E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1316-T02-B	1	2.54E+05			2.54E+05	1.7E+00	1.5E+01	4.8E+01	10	125	2.55E+05	92%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1316-T03-B	1	5.54E+05			5.54E+05	1.8E+00	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1316-T04-B	1	1.15E+06			1.15E+06	5.9E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1316-T05-B	1	8.25E+05			8.25E+05	5.4E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1316-T01-C	1	1.51E+05			1.51E+05	7.2E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1316-T02-C	1	2.54E+05			2.54E+05	3.4E-01	1.5E+01	4.8E+01	10	125	2.55E+05	96%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1316-T03-C	1	6.06E+05			6.06E+05	2.5E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1316-T04-C	1	1.09E+06			1.09E+06	6.2E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1316-T05-C	1	7.84E+05			7.84E+05	7.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
Se	SWA-L02-1316-B01-A	1	1.57E+01	E		1.57E+01	2.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	SWA-L02-1316-T01-A	1	2.31E+04			2.31E+04	1.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1316-T02-A	1	2.62E+04			2.62E+04	1.2E+00	1.1E+00	3.5E+00	1000	125	2.73E+04	87%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1316-T03-A	1	3.34E+04			3.34E+04	7.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1316-T04-A	1	4.54E+04			4.54E+04	2.9E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1316-T05-A	1	3.39E+04			3.39E+04	9.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1316-T01-B	1	2.40E+04			2.40E+04	1.5E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1316-T02-B	1	2.72E+04			2.72E+04	2.0E+00	1.1E+00	3.5E+00	1000	125	2.84E+04	97%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1316-T03-B	1	3.46E+04			3.46E+04	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1316-T04-B	1	4.79E+04			4.79E+04	7.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1316-T05-B	1	3.74E+04			3.74E+04	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1316-T01-C	1	2.33E+04			2.33E+04	7.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1316-T02-C	1	2.87E+04			2.87E+04	7.0E-01	1.1E+00	3.5E+00	1000	125	2.99E+04	90%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1316-T03-C	1	3.43E+04			3.43E+04	3.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1316-T04-C	1	4.76E+04			4.76E+04	1.4E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1316-T05-C	1	3.64E+04			3.64E+04	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
Si	SWA-L02-1316-B01-A	1	2.40E+00	E		2.40E+00	7.5E+00	1.1E+00	3.5E+00				---	VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	SWA-L02-1316-T01-A	1	5.68E+05			5.68E+05	1.0E+00	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1316-T02-A	1	7.99E+05			7.99E+05	1.7E-01	2.5E+00	8.0E+00	1000	125	8.01E+05	85%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1316-T03-A	1	1.05E+06			1.05E+06	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1316-T04-A	1	1.12E+06			1.12E+06	5.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1316-T05-A	1	1.10E+06			1.10E+06	1.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1316-T01-B	1	6.62E+05			6.62E+05	4.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1316-T02-B	1	8.13E+05			8.13E+05	7.2E-01	2.5E+00	8.0E+00	1000	125	8.15E+05	88%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1316-T03-B	1	1.02E+06			1.02E+06	1.9E+00	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1316-T04-B	1	1.16E+06			1.16E+06	6.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1316-T05-B	1	1.14E+06			1.14E+06	3.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1316-T01-C	1	6.40E+05			6.40E+05	6.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1316-T02-C	1	8.13E+05			8.13E+05	1.4E-01	2.5E+00	8.0E+00	1000	125	8.14E+05	92%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1316-T03-C	1	1.07E+06			1.07E+06	6.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1316-T04-C	1	1.13E+06			1.13E+06	9.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1316-T05-C	1	1.09E+06			1.09E+06	3.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
Na	SWA-L02-1316-B01-A	1	8.59E+02			8.59E+02	3.5E+00	2.5E+00	8.0E+00				---	VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	SWA-L02-1316-T01-A	1	4.13E+02			4.13E+02	8.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1316-T02-A	1	4.64E+02			4.64E+02	1.1E+00	1.0E+00	3.2E+00	1000	125	1.73E+03	101%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1316-T03-A	1	5.31E+02			5.31E+02	6.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1316-T04-A	1	6.20E+02			6.20E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1316-T05-A	1	5.50E+02			5.50E+02	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1316-T01-B	1	4.83E+02			4.83E+02	1.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1316-T02-B	1	4.79E+02			4.79E+02	1.8E+00	1.0E+00	3.2E+00	1000	125	1.86E+03	110%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1316-T03-B	1	5.09E+02			5.09E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1316-T04-B	1	6.44E+02			6.44E+02	9.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1316-T05-B	1	5.71E+02			5.71E+02	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1316-T01-C	1	4.46E+02			4.46E+02	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1316-T02-C	1	4.62E+02			4.62E+02	5.8E-01	1.0E+00	3.2E+00	1000	125	1.89E+03	114%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1316-T03-C	1	5.43E+02			5.43E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1316-T04-C	1	6.04E+02			6.04E+02	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1316-T05-C	1	5.44E+02			5.44E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
Sr	SWA-L02-1316-B01-A	1	1.66E+01			1.66E+01	2.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	SWA-L02-1316-T01-A	1	6.32E+05			6.32E+05	1.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1316-T02-A	1	1.15E+06			1.15E+06	1.2E+00	6.8E+00	2.2E+01	1000	125	1.15E+06	83%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1316-T03-A	1	1.89E+06			1.89E+06	5.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1316-T04-A	1	2.73E+06			2.73E+06	9.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1316-T05-A	1	2.22E+06			2.22E+06	8.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1316-T01-B	1	8.74E+05			8.74E+05	7.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1316-T02-B	1	1.22E+06			1.22E+06	1.6E+00	6.8E+00	2.2E+01	1000	125	1.22E+06	85%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1316-T03-B	1	1.76E+06			1.76E+06	2.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1316-T04-B	1	2.76E+06			2.76E+06	7.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1316-T05-B	1	2.29E+06			2.29E+06	5.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1316-T01-C	1	7.22E+05			7.22E+05	2.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1316-T02-C	1	1.18E+06			1.18E+06	5.4E-01	6.8E+00	2.2E+01	1000	125	1.18E+06	87%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1316-T03-C	1	1.92E+06			1.92E+06	2.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1316-T04-C	1	2.64E+06			2.64E+06	6.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1316-T05-C	1	2.06E+06			2.06E+06	8.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
S	SWA-L02-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	4.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	SWA-L02-1316-T01-A	1	2.30E+00	U1/2		2.30E+00	1.2E+03	4.6E+00	1.5E+01			---		VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1316-T02-A	1	2.30E+00	U1/2		2.30E+00	2.9E+02	4.6E+00	1.5E+01	10	125	1.14E+03	91%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1316-T03-A	1	2.30E+00	U1/2		2.30E+00	1.7E+02	4.6E+00	1.5E+01			---		VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1316-T04-A	1	2.30E+00	U1/2		2.30E+00	5.0E+01	4.6E+00	1.5E+01			---		VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1316-T05-A	1	2.30E+00	U1/2		2.30E+00	1.6E+02	4.6E+00	1.5E+01			---		VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1316-T01-B	1	2.30E+00	U1/2		2.30E+00	3.9E+02	4.6E+00	1.5E+01			---		VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1316-T02-B	1	2.30E+00	U1/2		2.30E+00	5.0E+01	4.6E+00	1.5E+01	10	125	1.13E+03	90%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1316-T03-B	1	2.30E+00	U1/2		2.30E+00	2.7E+01	4.6E+00	1.5E+01			---		VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1316-T04-B	1	2.30E+00	U1/2		2.30E+00	4.3E+01	4.6E+00	1.5E+01			---		VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1316-T05-B	1	2.30E+00	U1/2		2.30E+00	1.8E+02	4.6E+00	1.5E+01			---		VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1316-T01-C	1	2.30E+00	U1/2		2.30E+00	2.5E+02	4.6E+00	1.5E+01			---		VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1316-T02-C	1	2.30E+00	U1/2		2.30E+00	1.6E+02	4.6E+00	1.5E+01	10	125	1.16E+03	92%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1316-T03-C	1	2.30E+00	U1/2		2.30E+00	1.1E+02	4.6E+00	1.5E+01			---		VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1316-T04-C	1	2.30E+00	U1/2		2.30E+00	2.7E+02	4.6E+00	1.5E+01			---		VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1316-T05-C	1	2.30E+00	U1/2		2.30E+00	1.3E+02	4.6E+00	1.5E+01			---		VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
Tl	SWA-L02-1316-B01-A	1	2.30E+00	U1/2		2.30E+00	2.9E+02	4.6E+00	1.5E+01			---		VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	SWA-L02-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	8.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	1.1E+00	2.0E+00	6.4E+00	10	125	1.22E+03	98%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	6.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1316-T05-A	1	3.29E+00	E		3.29E+00	7.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	1.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	1.8E+00	2.0E+00	6.4E+00	10	125	1.31E+03	105%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	1.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	9.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1316-T05-B	1	4.89E+00	E		4.89E+00	8.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	1.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	5.8E-01	2.0E+00	6.4E+00	10	125	1.34E+03	107%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	1.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	3.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1316-T05-C	1	4.54E+00	E		4.54E+00	1.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
Ti	SWA-L02-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	2.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	SWA-L02-1316-T01-A	1	3.74E+02			3.74E+02	9.8E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1316-T02-A	1	7.51E+02			7.51E+02	1.1E+00	1.5E+00	4.8E+00	10	125	2.08E+03	107%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1316-T03-A	1	1.46E+03			1.46E+03	5.0E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1316-T04-A	1	2.27E+03			2.27E+03	9.9E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1316-T05-A	1	1.86E+03			1.86E+03	7.6E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1316-T01-B	1	4.76E+02			4.76E+02	1.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1316-T02-B	1	7.75E+02			7.75E+02	1.7E+00	1.5E+00	4.8E+00	10	125	2.06E+03	103%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1316-T03-B	1	1.36E+03			1.36E+03	1.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1316-T04-B	1	2.29E+03			2.29E+03	7.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1316-T05-B	1	1.93E+03			1.93E+03	8.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1316-T01-C	1	4.59E+02			4.59E+02	1.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1316-T02-C	1	7.69E+02			7.69E+02	6.1E-01	1.5E+00	4.8E+00	10	125	2.09E+03	106%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1316-T03-C	1	1.47E+03			1.47E+03	2.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1316-T04-C	1	2.18E+03			2.18E+03	7.1E-01	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1316-T05-C	1	1.83E+03			1.83E+03	1.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
V	SWA-L02-1316-B01-A	1	1.89E+00	E		1.89E+00	5.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	SWA-L02-1316-T01-A	1	2.72E+00	E		2.72E+00	1.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:03 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1316-T02-A	1	4.18E+00			4.18E+00	4.4E+00	1.0E+00	3.2E+00	10	125	1.32E+03	105%	VU ICP-OES	11/29/10 5:05 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1316-T03-A	1	8.73E+00			8.73E+00	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:06 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1316-T04-A	1	3.63E+01			3.63E+01	4.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:08 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1316-T05-A	1	1.94E+01			1.94E+01	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:10 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1316-T01-B	1	2.59E+00	E		2.59E+00	2.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:11 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1316-T02-B	1	4.69E+00			4.69E+00	9.7E+00	1.0E+00	3.2E+00	10	125	1.43E+03	114%	VU ICP-OES	11/29/10 5:13 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1316-T03-B	1	8.60E+00			8.60E+00	1.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:14 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1316-T04-B	1	3.90E+01			3.90E+01	3.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:16 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1316-T05-B	1	2.00E+01			2.00E+01	3.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:18 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1316-T01-C	1	2.28E+00	E		2.28E+00	1.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:19 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1316-T02-C	1	3.53E+00			3.53E+00	9.9E+00	1.0E+00	3.2E+00	10	125	1.36E+03	109%	VU ICP-OES	11/29/10 5:21 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1316-T03-C	1	1.02E+01			1.02E+01	6.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:23 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1316-T04-C	1	3.36E+01			3.36E+01	9.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:24 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1316-T05-C	1	1.98E+01			1.98E+01	3.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:26 PM	EPA Interlab L02 1313-1316 SWA
Zn	SWA-L02-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	11/29/10 5:02 PM	EPA Interlab L02 1313-1316 SWA

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	SWA-L04-1316-T01-A	1	3.65E+04			3.65E+04	2.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1316-T02-A	1	5.72E+04			5.72E+04	1.2E+00	1.0E+00	3.2E+00	1000	100	5.80E+04	85%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1316-T03-A	1	8.32E+04			8.32E+04	9.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1316-T04-A	1	1.66E+05			1.66E+05	8.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1316-T01-B	1	4.05E+04			4.05E+04	5.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1316-T02-B	1	5.89E+04			5.89E+04	1.0E+00	1.0E+00	3.2E+00	1000	100	5.98E+04	92%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1316-T03-B	1	9.57E+04			9.57E+04	3.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1316-T04-B	1	1.62E+05			1.62E+05	5.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1316-T01-C	1	3.69E+04			3.69E+04	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1316-T02-C	1	5.89E+04			5.89E+04	7.8E-01	1.0E+00	3.2E+00	1000	100	5.99E+04	96%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1316-T03-C	1	7.97E+04			7.97E+04	2.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1316-T04-C	1	1.64E+05			1.64E+05	4.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	9.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	6.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
Al	SWA-L04-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	3.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	SWA-L04-1316-T01-A	1	3.79E+03			3.79E+03	9.4E-01	7.5E+00	2.4E+01				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1316-T02-A	1	1.02E+03			1.02E+03	2.0E+00	7.5E+00	2.4E+01	10	100	2.13E+03	110%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1316-T03-A	1	9.29E+03			9.29E+03	4.4E-01	7.5E+00	2.4E+01				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1316-T04-A	1	7.65E+03			7.65E+03	8.0E-01	7.5E+00	2.4E+01				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1316-T01-B	1	3.28E+03			3.28E+03	7.6E-01	7.5E+00	2.4E+01				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1316-T02-B	1	9.16E+02			9.16E+02	3.6E+00	7.5E+00	2.4E+01	10	100	2.03E+03	112%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1316-T03-B	1	9.51E+03			9.51E+03	5.2E-01	7.5E+00	2.4E+01				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1316-T04-B	1	8.08E+03			8.08E+03	3.3E-01	7.5E+00	2.4E+01				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1316-T01-C	1	3.47E+03			3.47E+03	8.0E-01	7.5E+00	2.4E+01				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1316-T02-C	1	5.65E+02			5.65E+02	4.6E+00	7.5E+00	2.4E+01	10	100	1.71E+03	114%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1316-T03-C	1	9.13E+03			9.13E+03	1.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1316-T04-C	1	8.01E+03			8.01E+03	1.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1316-B01-A	1	3.75E+00	U1/2		3.75E+00	2.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1316-B02-A	1	3.75E+00	U1/2		3.75E+00	6.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
Sb	SWA-L04-1316-B03-A	1	9.02E+00	E		9.02E+00	7.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	SWA-L04-1316-T01-A	1	4.62E+03			4.62E+03	2.0E-01	1.1E+01	3.5E+01				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1316-T02-A	1	1.33E+04			1.33E+04	1.9E+00	1.1E+01	3.5E+01	10	100	1.42E+04	95%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1316-T03-A	1	4.50E+04			4.50E+04	5.0E-01	1.1E+01	3.5E+01				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1316-T04-A	1	1.01E+05			1.01E+05	1.7E+00	1.1E+01	3.5E+01				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1316-T01-B	1	5.89E+03			5.89E+03	7.1E-01	1.1E+01	3.5E+01				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1316-T02-B	1	1.40E+04			1.40E+04	1.6E+00	1.1E+01	3.5E+01	10	100	1.49E+04	87%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1316-T03-B	1	4.53E+04			4.53E+04	6.3E-01	1.1E+01	3.5E+01				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1316-T04-B	1	1.08E+05			1.08E+05	2.2E-01	1.1E+01	3.5E+01				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1316-T01-C	1	5.00E+03			5.00E+03	5.2E-01	1.1E+01	3.5E+01				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1316-T02-C	1	1.35E+04			1.35E+04	1.8E+00	1.1E+01	3.5E+01	10	100	1.45E+04	97%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1316-T03-C	1	3.86E+04			3.86E+04	1.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1316-T04-C	1	1.02E+05			1.02E+05	1.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1316-B01-A	1	5.50E+00	U1/2		5.50E+00	1.5E+02	7.5E+00	2.4E+01				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1316-B02-A	1	5.50E+00	U1/2		5.50E+00	1.7E+02	7.5E+00	2.4E+01				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
As	SWA-L04-1316-B03-A	1	5.50E+00	U1/2		5.50E+00	7.5E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	SWA-L04-1316-T01-A	1	1.10E+03			1.10E+03	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1316-T02-A	1	1.79E+03			1.79E+03	1.2E+00	1.0E+00	3.2E+00	1000	100	2.79E+03	100%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1316-T03-A	1	2.35E+03			2.35E+03	8.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1316-T04-A	1	1.20E+03			1.20E+03	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1316-T01-B	1	1.34E+03			1.34E+03	9.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1316-T02-B	1	2.01E+03			2.01E+03	1.7E+00	1.0E+00	3.2E+00	1000	100	3.04E+03	104%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1316-T03-B	1	2.63E+03			2.63E+03	3.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1316-T04-B	1	1.84E+03			1.84E+03	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1316-T01-C	1	1.19E+03			1.19E+03	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1316-T02-C	1	1.97E+03			1.97E+03	4.1E-01	1.0E+00	3.2E+00	1000	100	2.93E+03	96%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1316-T03-C	1	2.03E+03			2.03E+03	2.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1316-T04-C	1	1.71E+03			1.71E+03	2.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1316-B01-A	1	2.04E+01			2.04E+01	6.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1316-B02-A	1	1.65E+01			1.65E+01	4.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
B	SWA-L04-1316-B03-A	1	1.41E+01			1.41E+01	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	SWA-L04-1316-T01-A	1	1.87E+02			1.87E+02	2.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1316-T02-A	1	1.65E+02			1.65E+02	4.8E-01	1.0E+00	3.2E+00	10	100	1.34E+03	117%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1316-T03-A	1	5.08E+00			5.08E+00	3.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1316-T04-A	1	8.65E+01			8.65E+01	7.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1316-T01-B	1	1.52E+02			1.52E+02	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1316-T02-B	1	1.57E+02			1.57E+02	5.2E-01	1.0E+00	3.2E+00	10	100	1.36E+03	120%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1316-T03-B	1	5.47E+01			5.47E+01	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1316-T04-B	1	3.76E+01			3.76E+01	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1316-T01-C	1	1.64E+02			1.64E+02	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1316-T02-C	1	1.71E+02			1.71E+02	7.3E-01	1.0E+00	3.2E+00	10	100	1.34E+03	117%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1316-T03-C	1	4.92E+00			4.92E+00	2.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1316-T04-C	1	7.48E+01			7.48E+01	6.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.0E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	4.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
Ba	SWA-L04-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	2.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	SWA-L04-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	2.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00	10	100	1.15E+03	114%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	3.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	7.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	9.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	7.2E+01	1.9E+00	6.0E+00	10	100	1.18E+03	118%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	3.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	8.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	6.7E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	1.5E+02	1.9E+00	6.0E+00	10	100	1.10E+03	110%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	9.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	5.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1316-B02-A	1	9.50E-01	U1/2		9.50E-01	8.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
Be	SWA-L04-1316-B03-A	1	9.50E-01	U1/2		9.50E-01	1.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	SWA-L04-1316-T01-A	1	1.10E+00	U1/2		1.10E+00	1.4E+02	2.2E+00	7.0E+00				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1316-T02-A	1	1.10E+00	U1/2		1.10E+00	4.3E+02	2.2E+00	7.0E+00	10	100	1.19E+03	119%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1316-T03-A	1	1.10E+00	U1/2		1.10E+00	5.0E+02	2.2E+00	7.0E+00				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1316-T04-A	1	1.10E+00	U1/2		1.10E+00	1.2E+02	2.2E+00	7.0E+00				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1316-T01-B	1	1.10E+00	U1/2		1.10E+00	9.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1316-T02-B	1	1.10E+00	U1/2		1.10E+00	1.0E+02	2.2E+00	7.0E+00	10	100	1.12E+03	112%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1316-T03-B	1	1.10E+00	U1/2		1.10E+00	2.0E+02	2.2E+00	7.0E+00				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1316-T04-B	1	1.10E+00	U1/2		1.10E+00	1.2E+02	2.2E+00	7.0E+00				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1316-T01-C	1	1.10E+00	U1/2		1.10E+00	1.0E+02	2.2E+00	7.0E+00				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1316-T02-C	1	1.10E+00	U1/2		1.10E+00	2.7E+02	2.2E+00	7.0E+00	10	100	1.15E+03	114%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1316-T03-C	1	1.10E+00	U1/2		1.10E+00	1.4E+02	2.2E+00	7.0E+00				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1316-T04-C	1	1.10E+00	U1/2		1.10E+00	2.5E+01	2.2E+00	7.0E+00				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1316-B01-A	1	1.10E+00	U1/2		1.10E+00	3.6E+02	2.2E+00	7.0E+00				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1316-B02-A	1	1.10E+00	U1/2		1.10E+00	5.7E+02	2.2E+00	7.0E+00				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
Cd	SWA-L04-1316-B03-A	1	1.10E+00	U1/2		1.10E+00	1.9E+02	2.2E+00	7.0E+00				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	SWA-L04-1316-T01-A	1	1.42E+04			1.42E+04	9.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1316-T02-A	1	1.03E+04			1.03E+04	3.3E-01	2.6E+00	8.3E+00	1000	100	1.14E+04	104%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1316-T03-A	1	2.22E+03			2.22E+03	1.6E+00	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1316-T04-A	1	4.11E+03			4.11E+03	2.8E+00	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1316-T01-B	1	1.26E+04			1.26E+04	8.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1316-T02-B	1	9.45E+03			9.45E+03	3.0E-01	2.6E+00	8.3E+00	1000	100	1.06E+04	115%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1316-T03-B	1	4.05E+03			4.05E+03	8.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1316-T04-B	1	3.01E+03			3.01E+03	3.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1316-T01-C	1	1.35E+04			1.35E+04	1.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1316-T02-C	1	9.84E+03			9.84E+03	7.8E-01	2.6E+00	8.3E+00	1000	100	1.08E+04	92%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1316-T03-C	1	2.20E+03			2.20E+03	2.0E+01	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1316-T04-C	1	3.99E+03			3.99E+03	2.7E+00	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1316-B01-A	1	3.82E+01			3.82E+01	3.0E+01	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1316-B02-A	1	3.32E+01			3.32E+01	1.8E+01	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
Ca	SWA-L04-1316-B03-A	1	3.42E+01			3.42E+01	1.5E+01	2.6E+00	8.3E+00				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	SWA-L04-1316-T01-A	1	1.18E+03			1.18E+03	1.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1316-T02-A	1	1.82E+03			1.82E+03	7.8E-01	1.2E+00	3.8E+00	10	100	2.77E+03	95%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1316-T03-A	1	1.35E+03			1.35E+03	5.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1316-T04-A	1	3.19E+03			3.19E+03	1.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1316-T01-B	1	1.45E+03			1.45E+03	2.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1316-T02-B	1	1.99E+03			1.99E+03	1.3E+00	1.2E+00	3.8E+00	10	100	3.00E+03	102%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1316-T03-B	1	2.07E+03			2.07E+03	7.3E-02	1.2E+00	3.8E+00				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1316-T04-B	1	2.21E+03			2.21E+03	1.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1316-T01-C	1	1.31E+03			1.31E+03	9.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1316-T02-C	1	1.91E+03			1.91E+03	1.3E+00	1.2E+00	3.8E+00	10	100	2.81E+03	89%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1316-T03-C	1	1.38E+03			1.38E+03	3.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1316-T04-C	1	2.70E+03			2.70E+03	1.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	1.1E+03	1.2E+00	3.8E+00				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	5.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
Cr	SWA-L04-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	1.2E+02	1.2E+00	3.8E+00				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	SWA-L04-1316-T01-A	1	9.00E-01	U1/2		9.00E-01	1.6E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1316-T02-A	1	9.00E-01	U1/2		9.00E-01	2.1E+01	1.8E+00	5.7E+00	10	100	1.13E+03	112%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1316-T03-A	1	3.13E+00	E		3.13E+00	5.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1316-T04-A	1	6.53E+00			6.53E+00	7.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1316-T01-B	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1316-T02-B	1	9.00E-01	U1/2		9.00E-01	5.4E+01	1.8E+00	5.7E+00	10	100	1.16E+03	116%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1316-T03-B	1	3.62E+00	E		3.62E+00	3.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1316-T04-B	1	8.95E+00			8.95E+00	3.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1316-T01-C	1	9.00E-01	U1/2		9.00E-01	6.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1316-T02-C	1	9.00E-01	U1/2		9.00E-01	9.4E+01	1.8E+00	5.7E+00	10	100	1.08E+03	108%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1316-T03-C	1	2.18E+00	E		2.18E+00	4.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1316-T04-C	1	7.14E+00			7.14E+00	4.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	5.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1316-B02-A	1	9.00E-01	U1/2		9.00E-01	2.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
Co	SWA-L04-1316-B03-A	1	9.00E-01	U1/2		9.00E-01	8.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	SWA-L04-1316-T01-A	1	1.85E+00	U1/2		1.85E+00	6.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1316-T02-A	1	1.85E+00	U1/2		1.85E+00	4.0E+01	3.7E+00	1.2E+01	10	100	1.12E+03	112%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1316-T03-A	1	1.48E+01			1.48E+01	3.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1316-T04-A	1	4.27E+01			4.27E+01	4.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1316-T01-B	1	1.85E+00	U1/2		1.85E+00	7.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1316-T02-B	1	1.85E+00	U1/2		1.85E+00	9.4E+01	3.7E+00	1.2E+01	10	100	1.15E+03	114%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1316-T03-B	1	1.86E+01			1.86E+01	1.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1316-T04-B	1	3.40E+01			3.40E+01	9.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1316-T01-C	1	1.85E+00	U1/2		1.85E+00	1.1E+02	3.7E+00	1.2E+01				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1316-T02-C	1	1.85E+00	U1/2		1.85E+00	1.1E+02	3.7E+00	1.2E+01	10	100	1.07E+03	107%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1316-T03-C	1	9.85E+00	E		9.85E+00	3.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1316-T04-C	1	3.12E+01			3.12E+01	7.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	2.2E+02	3.7E+00	1.2E+01				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1316-B02-A	1	1.85E+00	U1/2		1.85E+00	1.6E+02	3.7E+00	1.2E+01				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
Cu	SWA-L04-1316-B03-A	1	1.85E+00	U1/2		1.85E+00	1.3E+02	3.7E+00	1.2E+01				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	SWA-L04-1316-T01-A	1	7.64E+01			7.64E+01	1.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1316-T02-A	1	1.73E+02			1.73E+02	9.0E-01	2.0E+00	6.4E+00	1000	100	1.31E+03	114%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1316-T03-A	1	3.35E+02			3.35E+02	5.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1316-T04-A	1	1.18E+03			1.18E+03	5.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1316-T01-B	1	1.04E+02			1.04E+02	1.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1316-T02-B	1	1.82E+02			1.82E+02	5.3E-01	2.0E+00	6.4E+00	1000	100	1.35E+03	117%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1316-T03-B	1	3.84E+02			3.84E+02	4.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1316-T04-B	1	1.14E+03			1.14E+03	8.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1316-T01-C	1	8.64E+01			8.64E+01	9.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1316-T02-C	1	1.73E+02			1.73E+02	4.6E-01	2.0E+00	6.4E+00	1000	100	1.27E+03	110%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1316-T03-C	1	2.64E+02			2.64E+02	2.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1316-T04-C	1	1.15E+03			1.15E+03	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	4.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1316-B02-A	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
Fe	SWA-L04-1316-B03-A	1	2.03E+00	E		2.03E+00	1.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	SWA-L04-1316-T01-A	1	1.63E+01	E		1.63E+01	2.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1316-T02-A	1	4.02E+01			4.02E+01	1.2E+01	6.8E+00	2.2E+01	10	100	1.15E+03	111%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1316-T03-A	1	1.28E+01	E		1.28E+01	1.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1316-T04-A	1	1.34E+02			1.34E+02	5.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1316-T01-B	1	1.36E+01	E		1.36E+01	9.8E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1316-T02-B	1	3.26E+01			3.26E+01	3.4E+00	6.8E+00	2.2E+01	10	100	1.18E+03	115%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1316-T03-B	1	3.26E+01			3.26E+01	1.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1316-T04-B	1	1.06E+02			1.06E+02	1.8E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1316-T01-C	1	1.71E+01	E		1.71E+01	3.7E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1316-T02-C	1	3.42E+01			3.42E+01	5.6E+00	6.8E+00	2.2E+01	10	100	1.11E+03	107%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1316-T03-C	1	1.23E+01	E		1.23E+01	2.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1316-T04-C	1	1.37E+02			1.37E+02	2.3E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	6.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1316-B02-A	1	3.40E+00	U1/2		3.40E+00	5.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
Pb	SWA-L04-1316-B03-A	1	3.40E+00	U1/2		3.40E+00	1.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	SWA-L04-1316-T01-A	1	2.66E+00	E		2.66E+00	3.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/23/11 2:39 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L04-1316-T02-A	1	6.26E+00			6.26E+00	3.8E+01	1.9E+00	6.0E+00	10	100	9.14E+02	91%	VU ICP-OES	5/23/11 2:41 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L04-1316-T03-A	1	9.17E+00			9.17E+00	9.5E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/23/11 2:43 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L04-1316-T04-A	1	9.35E+00			9.35E+00	1.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/23/11 2:46 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L04-1316-T01-B	1	2.39E+00	E		2.39E+00	1.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/23/11 2:48 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L04-1316-T02-B	1	5.44E+00	E		5.44E+00	1.8E+01	1.9E+00	6.0E+00	10	100	9.32E+02	93%	VU ICP-OES	5/23/11 2:50 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L04-1316-T03-B	1	8.29E+00			8.29E+00	1.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/23/11 2:52 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L04-1316-T04-B	1	9.26E+00			9.26E+00	9.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/23/11 2:55 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L04-1316-T01-C	1	2.75E+00	E		2.75E+00	1.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/23/11 2:57 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L04-1316-T02-C	1	5.92E+00	E		5.92E+00	3.0E+01	1.9E+00	6.0E+00	10	100	9.00E+02	89%	VU ICP-OES	5/23/11 2:59 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L04-1316-T03-C	1	8.87E+00			8.87E+00	5.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/23/11 3:01 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L04-1316-T04-C	1	9.34E+00			9.34E+00	1.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/23/11 3:03 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L04-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	5.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1316-B02-A	1	9.50E-01	U1/2		9.50E-01	1.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
Li	SWA-L04-1316-B03-A	1	9.50E-01	U1/2		9.50E-01	8.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	SWA-L04-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	8.2E+00	2.0E+00	6.4E+00	10	100	1.15E+03	115%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	2.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1316-T04-A	1	2.75E+00	E		2.75E+00	2.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	5.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00	10	100	1.19E+03	119%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	4.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	1.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	2.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	5.1E+00	2.0E+00	6.4E+00	10	100	1.09E+03	109%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	6.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1316-T04-C	1	2.53E+00	E		2.53E+00	4.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	7.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1316-B02-A	1	1.00E+00	U1/2		1.00E+00	5.0E+03	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
Mn	SWA-L04-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	1.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	SWA-L04-1316-T01-A	1	6.46E+00			6.46E+00	5.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1316-T02-A	1	8.47E+00			8.47E+00	6.9E+01	1.0E+00	3.2E+00	1000	100	1.13E+03	113%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1316-T03-A	1	1.12E+01			1.12E+01	4.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1316-T04-A	1	1.17E+01			1.17E+01	6.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1316-T01-B	1	1.69E+01			1.69E+01	3.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1316-T02-B	1	1.81E+00	E		1.81E+00	4.6E+02	1.0E+00	3.2E+00	1000	100	1.16E+03	116%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1316-T03-B	1	5.96E+00			5.96E+00	1.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1316-T04-B	1	6.84E+00			6.84E+00	2.0E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1316-T01-C	1	1.49E+01			1.49E+01	8.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1316-T02-C	1	1.06E+01			1.06E+01	4.9E+01	1.0E+00	3.2E+00	1000	100	1.06E+03	105%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1316-T03-C	1	4.52E+00			4.52E+00	2.7E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1316-T04-C	1	1.24E+01			1.24E+01	2.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.3E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1316-B02-A	1	4.43E+00			4.43E+00	1.5E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
Mg	SWA-L04-1316-B03-A	1	1.43E+00	E		1.43E+00	5.7E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	SWA-L04-1316-T01-A	1	1.15E+02			1.15E+02	2.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1316-T02-A	1	1.71E+02			1.71E+02	1.0E+00	1.2E+00	3.8E+00	10	100	1.30E+03	112%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1316-T03-A	1	5.77E+02			5.77E+02	7.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1316-T04-A	1	1.12E+03			1.12E+03	1.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1316-T01-B	1	1.31E+02			1.31E+02	1.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1316-T02-B	1	1.90E+02			1.90E+02	1.2E+00	1.2E+00	3.8E+00	10	100	1.37E+03	117%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1316-T03-B	1	5.73E+02			5.73E+02	3.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1316-T04-B	1	1.22E+03			1.22E+03	6.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1316-T01-C	1	1.14E+02			1.14E+02	1.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1316-T02-C	1	1.57E+02			1.57E+02	6.4E-01	1.2E+00	3.8E+00	10	100	1.26E+03	111%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1316-T03-C	1	4.34E+02			4.34E+02	2.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1316-T04-C	1	1.12E+03			1.12E+03	5.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1316-B01-A	1	2.92E+00	E		2.92E+00	2.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1316-B02-A	1	2.82E+00	E		2.82E+00	1.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
Mo	SWA-L04-1316-B03-A	1	2.16E+00	E		2.16E+00	4.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	SWA-L04-1316-T01-A	1	9.00E-01	U1/2		9.00E-01	3.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1316-T02-A	1	2.15E+00	E		2.15E+00	5.2E+01	1.8E+00	5.7E+00	10	100	1.15E+03	115%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1316-T03-A	1	2.09E+00	E		2.09E+00	2.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1316-T04-A	1	5.95E+00			5.95E+00	3.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1316-T01-B	1	9.00E-01	U1/2		9.00E-01	9.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1316-T02-B	1	9.00E-01	U1/2		9.00E-01	3.1E+02	1.8E+00	5.7E+00	10	100	1.18E+03	118%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1316-T03-B	1	2.26E+00	E		2.26E+00	1.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1316-T04-B	1	4.13E+00	E		4.13E+00	5.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1316-T01-C	1	9.00E-01	U1/2		9.00E-01	4.9E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1316-T02-C	1	9.00E-01	U1/2		9.00E-01	3.0E+02	1.8E+00	5.7E+00	10	100	1.11E+03	111%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1316-T03-C	1	9.00E-01	U1/2		9.00E-01	3.3E+03	1.8E+00	5.7E+00				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1316-T04-C	1	5.27E+00	E		5.27E+00	8.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1316-B01-A	1	2.09E+00	E		2.09E+00	6.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1316-B02-A	1	9.00E-01	U1/2		9.00E-01	4.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
Ni	SWA-L04-1316-B03-A	1	9.00E-01	U1/2		9.00E-01	2.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	SWA-L04-1316-T01-A	1	4.84E+01			4.84E+01	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1316-T02-A	1	1.22E+02			1.22E+02	8.6E+00	3.7E+00	1.2E+01	1000	100	1.22E+03	109%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1316-T03-A	1	4.76E+02			4.76E+02	5.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1316-T04-A	1	1.27E+03			1.27E+03	1.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1316-T01-B	1	5.31E+01			5.31E+01	1.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1316-T02-B	1	1.05E+02			1.05E+02	2.2E+00	3.7E+00	1.2E+01	1000	100	1.23E+03	112%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1316-T03-B	1	4.33E+02			4.33E+02	5.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1316-T04-B	1	1.31E+03			1.31E+03	2.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1316-T01-C	1	3.37E+01			3.37E+01	2.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1316-T02-C	1	9.48E+01			9.48E+01	1.9E+01	3.7E+00	1.2E+01	1000	100	1.20E+03	110%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1316-T03-C	1	3.34E+02			3.34E+02	3.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1316-T04-C	1	1.25E+03			1.25E+03	9.2E-01	3.7E+00	1.2E+01				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1316-B01-A	1	1.07E+01	E		1.07E+01	6.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1316-B02-A	1	1.85E+00	U1/2		1.85E+00	9.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
P	SWA-L04-1316-B03-A	1	1.85E+00	U1/2		1.85E+00	4.7E+02	3.7E+00	1.2E+01				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	SWA-L04-1316-T01-A	1	2.84E+05			2.84E+05	3.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1316-T02-A	1	4.56E+05			4.56E+05	2.6E+00	1.6E+00	5.1E+00	1000	100	4.57E+05	93%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1316-T03-A	1	7.62E+05			7.62E+05	2.4E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1316-T04-A	1	2.42E+06			2.42E+06	3.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1316-T01-B	1	2.98E+05			2.98E+05	6.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1316-T02-B	1	4.62E+05			4.62E+05	2.2E+00	1.6E+00	5.1E+00	1000	100	4.63E+05	89%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1316-T03-B	1	7.49E+05			7.49E+05	1.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1316-T04-B	1	2.42E+06			2.42E+06	3.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1316-T01-C	1	2.86E+05			2.86E+05	8.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1316-T02-C	1	4.58E+05			4.58E+05	1.0E+00	1.6E+00	5.1E+00	1000	100	4.59E+05	95%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1316-T03-C	1	6.97E+05			6.97E+05	3.1E+01	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1316-T04-C	1	2.41E+06			2.41E+06	6.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1316-B01-A	1	2.99E+01			2.99E+01	5.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1316-B02-A	1	2.94E+01			2.94E+01	5.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
K	SWA-L04-1316-B03-A	1	2.78E+01			2.78E+01	7.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	SWA-L04-1316-T01-A	1	8.95E+04			8.95E+04	2.3E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1316-T02-A	1	1.69E+05			1.69E+05	6.6E-01	1.5E+01	4.8E+01	10	100	1.70E+05	102%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1316-T03-A	1	4.20E+05			4.20E+05	7.2E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1316-T04-A	1	7.68E+05			7.68E+05	4.8E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1316-T01-B	1	1.03E+05			1.03E+05	6.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1316-T02-B	1	1.76E+05			1.76E+05	8.7E-01	1.5E+01	4.8E+01	10	100	1.77E+05	108%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1316-T03-B	1	4.20E+05			4.20E+05	8.2E-02	1.5E+01	4.8E+01				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1316-T04-B	1	8.41E+05			8.41E+05	3.8E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1316-T01-C	1	9.62E+04			9.62E+04	9.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1316-T02-C	1	1.72E+05			1.72E+05	7.7E-01	1.5E+01	4.8E+01	10	100	1.74E+05	118%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1316-T03-C	1	3.13E+05			3.13E+05	3.6E+01	1.5E+01	4.8E+01				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1316-T04-C	1	7.65E+05			7.65E+05	1.5E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1316-B01-A	1	7.50E+00	U1/2		7.50E+00	4.5E+02	1.5E+01	4.8E+01				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1316-B02-A	1	7.50E+00	U1/2		7.50E+00	2.4E+02	1.5E+01	4.8E+01				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
Se	SWA-L04-1316-B03-A	1	7.50E+00	U1/2		7.50E+00	1.2E+02	1.5E+01	4.8E+01				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	SWA-L04-1316-T01-A	1	2.58E+04			2.58E+04	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1316-T02-A	1	3.66E+04			3.66E+04	6.9E-01	1.1E+00	3.5E+00	1000	100	3.75E+04	89%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1316-T03-A	1	2.84E+04			2.84E+04	3.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1316-T04-A	1	5.76E+04			5.76E+04	7.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1316-T01-B	1	2.83E+04			2.83E+04	8.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1316-T02-B	1	3.91E+04			3.91E+04	6.8E-01	1.1E+00	3.5E+00	1000	100	4.00E+04	93%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1316-T03-B	1	4.69E+04			4.69E+04	8.5E-02	1.1E+00	3.5E+00				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1316-T04-B	1	5.52E+04			5.52E+04	2.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1316-T01-C	1	2.63E+04			2.63E+04	5.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1316-T02-C	1	3.85E+04			3.85E+04	1.2E+00	1.1E+00	3.5E+00	1000	100	3.95E+04	94%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1316-T03-C	1	2.56E+04			2.56E+04	3.2E+01	1.1E+00	3.5E+00				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1316-T04-C	1	5.88E+04			5.88E+04	8.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1316-B01-A	1	6.20E+00			6.20E+00	4.0E+01	1.1E+00	3.5E+00				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1316-B02-A	1	5.61E+00			5.61E+00	8.0E+01	1.1E+00	3.5E+00				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
Si	SWA-L04-1316-B03-A	1	1.69E+01			1.69E+01	4.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	SWA-L04-1316-T01-A	1	3.98E+05			3.98E+05	1.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1316-T02-A	1	4.87E+05			4.87E+05	4.4E-01	2.5E+00	8.0E+00	1000	100	4.88E+05	91%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1316-T03-A	1	5.36E+05			5.36E+05	4.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1316-T04-A	1	5.49E+05			5.49E+05	4.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1316-T01-B	1	4.09E+05			4.09E+05	5.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1316-T02-B	1	4.84E+05			4.84E+05	7.5E-01	2.5E+00	8.0E+00	1000	100	4.85E+05	93%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1316-T03-B	1	5.40E+05			5.40E+05	1.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1316-T04-B	1	5.49E+05			5.49E+05	4.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1316-T01-C	1	4.03E+05			4.03E+05	1.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1316-T02-C	1	4.88E+05			4.88E+05	1.1E+00	2.5E+00	8.0E+00	1000	100	4.89E+05	86%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1316-T03-C	1	5.36E+05			5.36E+05	3.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1316-T04-C	1	5.56E+05			5.56E+05	1.5E+00	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1316-B01-A	1	1.25E+00	U1/2		1.25E+00	1.3E+02	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1316-B02-A	1	1.25E+00	U1/2		1.25E+00	3.6E+02	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
Na	SWA-L04-1316-B03-A	1	1.25E+00	U1/2		1.25E+00	1.3E+02	2.5E+00	8.0E+00				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	SWA-L04-1316-T01-A	1	3.27E+02			3.27E+02	2.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1316-T02-A	1	3.07E+02			3.07E+02	3.5E-01	1.0E+00	3.2E+00	1000	100	1.45E+03	114%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1316-T03-A	1	1.02E+02			1.02E+02	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1316-T04-A	1	3.97E+02			3.97E+02	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1316-T01-B	1	3.00E+02			3.00E+02	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1316-T02-B	1	2.94E+02			2.94E+02	2.5E-01	1.0E+00	3.2E+00	1000	100	1.47E+03	118%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1316-T03-B	1	2.48E+02			2.48E+02	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1316-T04-B	1	3.38E+02			3.38E+02	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1316-T01-C	1	3.15E+02			3.15E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1316-T02-C	1	3.01E+02			3.01E+02	6.0E-01	1.0E+00	3.2E+00	1000	100	1.39E+03	109%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1316-T03-C	1	1.03E+02			1.03E+02	3.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1316-T04-C	1	3.87E+02			3.87E+02	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	3.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	3.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
Sr	SWA-L04-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	1.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	SWA-L04-1316-T01-A	1	5.77E+05			5.77E+05	4.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1316-T02-A	1	1.19E+06			1.19E+06	1.1E+00	6.8E+00	2.2E+01	1000	100	1.28E+06	91%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1316-T03-A	1	1.74E+06			1.74E+06	4.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1316-T04-A	1	2.29E+06			2.29E+06	5.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1316-T01-B	1	8.77E+05			8.77E+05	1.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1316-T02-B	1	1.24E+06			1.24E+06	1.1E+00	6.8E+00	2.2E+01	1000	100	1.33E+06	86%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1316-T03-B	1	1.64E+06			1.64E+06	1.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1316-T04-B	1	2.39E+06			2.39E+06	1.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1316-T01-C	1	8.64E+05			8.64E+05	1.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1316-T02-C	1	1.39E+06			1.39E+06	1.7E+00	6.8E+00	2.2E+01	1000	100	1.48E+06	89%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1316-T03-C	1	1.41E+06			1.41E+06	2.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1316-T04-C	1	2.31E+06			2.31E+06	5.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	1.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1316-B02-A	1	3.40E+00	U1/2		3.40E+00	8.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
S	SWA-L04-1316-B03-A	1	3.40E+00	U1/2		3.40E+00	9.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	SWA-L04-1316-T01-A	1	2.30E+00	U1/2		2.30E+00	1.1E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1316-T02-A	1	2.30E+00	U1/2		2.30E+00	1.3E+03	4.6E+00	1.5E+01	10	100	1.04E+03	104%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1316-T03-A	1	2.30E+00	U1/2		2.30E+00	1.5E+01	4.6E+00	1.5E+01				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1316-T04-A	1	2.30E+00	U1/2		2.30E+00	2.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1316-T01-B	1	2.30E+00	U1/2		2.30E+00	2.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1316-T02-B	1	2.30E+00	U1/2		2.30E+00	4.9E+02	4.6E+00	1.5E+01	10	100	1.07E+03	107%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1316-T03-B	1	2.30E+00	U1/2		2.30E+00	2.1E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1316-T04-B	1	2.30E+00	U1/2		2.30E+00	1.7E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1316-T01-C	1	2.30E+00	U1/2		2.30E+00	1.0E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1316-T02-C	1	2.30E+00	U1/2		2.30E+00	3.4E+02	4.6E+00	1.5E+01	10	100	1.00E+03	100%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1316-T03-C	1	2.30E+00	U1/2		2.30E+00	2.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1316-T04-C	1	2.30E+00	U1/2		2.30E+00	9.5E+01	4.6E+00	1.5E+01				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1316-B01-A	1	2.30E+00	U1/2		2.30E+00	1.4E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1316-B02-A	1	2.30E+00	U1/2		2.30E+00	6.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
Tl	SWA-L04-1316-B03-A	1	2.30E+00	U1/2		2.30E+00	8.1E+01	4.6E+00	1.5E+01				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	SWA-L04-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	3.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.0E+00	6.4E+00	10	100	1.12E+03	112%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1316-T03-A	1	2.70E+00	E		2.70E+00	2.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1316-T04-A	1	4.51E+00	E		4.51E+00	8.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1316-T01-B	1	3.05E+00	E		3.05E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00	10	100	1.18E+03	118%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	3.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	1.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	4.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	5.3E+01	2.0E+00	6.4E+00	10	100	1.08E+03	108%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	5.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1316-T04-C	1	2.36E+00	E		2.36E+00	1.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	7.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1316-B02-A	1	1.00E+00	U1/2		1.00E+00	9.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
Ti	SWA-L04-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	4.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	SWA-L04-1316-T01-A	1	3.51E+02			3.51E+02	9.1E-01	1.5E+00	4.8E+00				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1316-T02-A	1	6.63E+02			6.63E+02	1.4E+00	1.5E+00	4.8E+00	10	100	1.75E+03	109%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1316-T03-A	1	1.33E+03			1.33E+03	8.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1316-T04-A	1	2.08E+03			2.08E+03	1.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1316-T01-B	1	4.38E+02			4.38E+02	4.8E-01	1.5E+00	4.8E+00				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1316-T02-B	1	7.10E+02			7.10E+02	1.4E+00	1.5E+00	4.8E+00	10	100	1.83E+03	112%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1316-T03-B	1	1.38E+03			1.38E+03	7.2E-01	1.5E+00	4.8E+00				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1316-T04-B	1	2.23E+03			2.23E+03	1.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1316-T01-C	1	3.87E+02			3.87E+02	9.1E-01	1.5E+00	4.8E+00				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1316-T02-C	1	6.90E+02			6.90E+02	9.2E-01	1.5E+00	4.8E+00	10	100	1.74E+03	105%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1316-T03-C	1	1.20E+03			1.20E+03	2.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1316-T04-C	1	2.13E+03			2.13E+03	5.0E-01	1.5E+00	4.8E+00				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1316-B01-A	1	7.50E-01	U1/2		7.50E-01	1.3E+02	1.5E+00	4.8E+00				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1316-B02-A	1	7.50E-01	U1/2		7.50E-01	3.3E+01	1.5E+00	4.8E+00				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
V	SWA-L04-1316-B03-A	1	7.50E-01	U1/2		7.50E-01	4.5E+01	1.5E+00	4.8E+00				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	SWA-L04-1316-T01-A	1	3.76E+00			3.76E+00	3.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:43 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1316-T02-A	1	4.39E+00			4.39E+00	2.5E+00	1.0E+00	3.2E+00	10	100	1.16E+03	116%	VU ICP-OES	3/21/11 2:44 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1316-T03-A	1	1.06E+00	E		1.06E+00	5.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:46 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1316-T04-A	1	1.63E+01			1.63E+01	9.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:48 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1316-T01-B	1	6.15E+00			6.15E+00	5.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:49 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1316-T02-B	1	7.34E+00			7.34E+00	3.6E+00	1.0E+00	3.2E+00	10	100	1.10E+03	109%	VU ICP-OES	3/21/11 2:51 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1316-T03-B	1	2.96E+00	E		2.96E+00	7.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:52 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1316-T04-B	1	1.52E+01			1.52E+01	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:54 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1316-T01-C	1	5.62E+00			5.62E+00	9.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:56 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1316-T02-C	1	8.60E+00			8.60E+00	1.8E+00	1.0E+00	3.2E+00	10	100	1.01E+03	100%	VU ICP-OES	3/21/11 2:57 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1316-T03-C	1	5.00E-01	U1/2		5.00E-01	2.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:59 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1316-T04-C	1	1.56E+01			1.56E+01	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 3:01 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1316-B01-A	1	2.85E+00	E		2.85E+00	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:38 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1316-B02-A	1	4.39E+00			4.39E+00	6.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:39 PM	EPA Interlab L04 1313-1316 SWA
Zn	SWA-L04-1316-B03-A	1	2.96E+00	E		2.96E+00	6.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/21/11 2:41 PM	EPA Interlab L04 1313-1316 SWA

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	SWA-L05-1316-T01-A	1	3.00E+04			3.00E+04	9.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1316-T02-A	1	4.32E+04			4.32E+04	9.2E-02	1.0E+00	3.2E+00	1000	100	4.41E+04	94%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1316-T03-A	1	7.43E+04			7.43E+04	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1316-T04-A	1	1.04E+05			1.04E+05	8.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1316-T05-A	1	1.50E+05			1.50E+05	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1316-T01-B	1	2.96E+04			2.96E+04	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1316-T02-B	1	4.59E+04			4.59E+04	1.0E+00	1.0E+00	3.2E+00	1000	100	4.68E+04	85%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1316-T03-B	1	7.44E+04			7.44E+04	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1316-T04-B	1	1.04E+05			1.04E+05	5.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1316-T05-B	1	1.49E+05			1.49E+05	6.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1316-T01-C	1	2.93E+04			2.93E+04	2.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1316-T02-C	1	4.35E+04			4.35E+04	5.2E-01	1.0E+00	3.2E+00	1000	100	4.44E+04	92%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1316-T03-C	1	7.68E+04			7.68E+04	1.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1316-T04-C	1	1.02E+05			1.02E+05	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1316-T05-C	1	1.49E+05			1.49E+05	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	4.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	5.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
Al	SWA-L05-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	4.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	SWA-L05-1316-T01-A	1	5.71E+03			5.71E+03	3.0E-01	7.5E+00	2.4E+01				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1316-T02-A	1	8.29E+03			8.29E+03	5.3E-01	7.5E+00	2.4E+01	10	100	9.27E+03	98%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1316-T03-A	1	7.43E+03			7.43E+03	1.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1316-T04-A	1	8.21E+03			8.21E+03	8.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1316-T05-A	1	6.99E+03			6.99E+03	4.8E-01	7.5E+00	2.4E+01				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1316-T01-B	1	5.73E+03			5.73E+03	5.1E-01	7.5E+00	2.4E+01				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1316-T02-B	1	9.28E+03			9.28E+03	2.0E+00	7.5E+00	2.4E+01	10	100	1.02E+04	91%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1316-T03-B	1	7.84E+03			7.84E+03	1.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1316-T04-B	1	8.32E+03			8.32E+03	4.3E-01	7.5E+00	2.4E+01				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1316-T05-B	1	7.21E+03			7.21E+03	4.7E-01	7.5E+00	2.4E+01				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1316-T01-C	1	5.67E+03			5.67E+03	9.1E-01	7.5E+00	2.4E+01				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1316-T02-C	1	8.33E+03			8.33E+03	7.1E-01	7.5E+00	2.4E+01	10	100	9.28E+03	95%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1316-T03-C	1	7.83E+03			7.83E+03	1.5E+02	7.5E+00	2.4E+01				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1316-T04-C	1	8.89E+03			8.89E+03	2.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1316-T05-C	1	6.84E+03			6.84E+03	1.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1316-B01-A	1	9.36E+00	E		9.36E+00	5.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1316-B02-A	1	8.24E+00	E		8.24E+00	8.9E+00	7.5E+00	2.4E+01				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
Sb	SWA-L05-1316-B03-A	1	3.75E+00	U1/2		3.75E+00	8.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	SWA-L05-1316-T01-A	1	4.28E+03			4.28E+03	4.1E-01	1.1E+01	3.5E+01				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1316-T02-A	1	1.09E+04			1.09E+04	9.5E-01	1.1E+01	3.5E+01	10	100	1.18E+04	91%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1316-T03-A	1	3.49E+04			3.49E+04	8.9E-01	1.1E+01	3.5E+01				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1316-T04-A	1	6.00E+04			6.00E+04	8.9E+01	1.1E+01	3.5E+01				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1316-T05-A	1	1.59E+05			1.59E+05	2.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1316-T01-B	1	4.47E+03			4.47E+03	4.6E-01	1.1E+01	3.5E+01				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1316-T02-B	1	1.17E+04			1.17E+04	1.9E+00	1.1E+01	3.5E+01	10	100	1.26E+04	88%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1316-T03-B	1	3.46E+04			3.46E+04	1.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1316-T04-B	1	7.28E+04			7.28E+04	4.5E-01	1.1E+01	3.5E+01				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1316-T05-B	1	1.54E+05			1.54E+05	2.7E-01	1.1E+01	3.5E+01				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1316-T01-C	1	4.45E+03			4.45E+03	8.9E-01	1.1E+01	3.5E+01				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1316-T02-C	1	1.09E+04			1.09E+04	5.8E-01	1.1E+01	3.5E+01	10	100	1.18E+04	92%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1316-T03-C	1	3.48E+04			3.48E+04	1.5E+02	1.1E+01	3.5E+01				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1316-T04-C	1	7.46E+04			7.46E+04	2.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1316-T05-C	1	1.54E+05			1.54E+05	1.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1316-B01-A	1	5.50E+00	U1/2		5.50E+00	4.2E+01	1.1E+01	3.5E+01				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1316-B02-A	1	5.50E+00	U1/2		5.50E+00	1.3E+02	1.1E+01	3.5E+01				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
As	SWA-L05-1316-B03-A	1	5.50E+00	U1/2		5.50E+00	5.0E+01	1.1E+01	3.5E+01				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	SWA-L05-1316-T01-A	1	8.15E+02			8.15E+02	9.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1316-T02-A	1	1.33E+03			1.33E+03	5.8E-01	1.0E+00	3.2E+00	1000	100	2.39E+03	107%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1316-T03-A	1	2.52E+03			2.52E+03	3.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1316-T04-A	1	3.33E+03			3.33E+03	9.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1316-T05-A	1	4.22E+03			4.22E+03	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1316-T01-B	1	8.22E+02			8.22E+02	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1316-T02-B	1	1.44E+03			1.44E+03	9.4E-01	1.0E+00	3.2E+00	1000	100	2.30E+03	86%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1316-T03-B	1	2.52E+03			2.52E+03	5.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1316-T04-B	1	3.39E+03			3.39E+03	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1316-T05-B	1	4.38E+03			4.38E+03	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1316-T01-C	1	8.05E+02			8.05E+02	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1316-T02-C	1	1.32E+03			1.32E+03	1.1E+00	1.0E+00	3.2E+00	1000	100	2.28E+03	96%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1316-T03-C	1	2.58E+03			2.58E+03	1.5E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1316-T04-C	1	3.35E+03			3.35E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1316-T05-C	1	4.35E+03			4.35E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1316-B01-A	1	1.33E+00	E		1.33E+00	3.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1316-B02-A	1	1.76E+00	E		1.76E+00	1.2E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
B	SWA-L05-1316-B03-A	1	1.63E+00	E		1.63E+00	8.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	SWA-L05-1316-T01-A	1	9.25E+01			9.25E+01	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1316-T02-A	1	1.02E+02			1.02E+02	2.7E-01	1.0E+00	3.2E+00	10	100	1.04E+03	94%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1316-T03-A	1	1.34E+02			1.34E+02	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1316-T04-A	1	1.03E+02			1.03E+02	8.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1316-T05-A	1	1.24E+02			1.24E+02	7.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1316-T01-B	1	1.09E+02			1.09E+02	1.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1316-T02-B	1	1.00E+02			1.00E+02	8.6E-01	1.0E+00	3.2E+00	10	100	9.97E+02	90%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1316-T03-B	1	1.36E+02			1.36E+02	8.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1316-T04-B	1	1.47E+02			1.47E+02	9.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1316-T05-B	1	1.27E+02			1.27E+02	1.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1316-T01-C	1	1.04E+02			1.04E+02	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1316-T02-C	1	1.07E+02			1.07E+02	4.4E-01	1.0E+00	3.2E+00	10	100	1.05E+03	95%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1316-T03-C	1	1.22E+02			1.22E+02	1.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1316-T04-C	1	1.38E+02			1.38E+02	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1316-T05-C	1	1.28E+02			1.28E+02	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	3.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	2.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
Ba	SWA-L05-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	4.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	SWA-L05-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	1.6E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	3.1E+01	1.9E+00	6.0E+00	10	100	9.41E+02	94%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	2.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	6.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1316-T05-A	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	5.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	6.6E+02	1.9E+00	6.0E+00	10	100	9.04E+02	90%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	9.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	1.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1316-T05-B	1	9.50E-01	U1/2		9.50E-01	5.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	6.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00	10	100	9.23E+02	92%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	2.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	3.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1316-T05-C	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	3.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1316-B02-A	1	9.50E-01	U1/2		9.50E-01	4.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
Be	SWA-L05-1316-B03-A	1	9.50E-01	U1/2		9.50E-01	7.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	SWA-L05-1316-T01-A	1	1.10E+00	U1/2		1.10E+00	8.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1316-T02-A	1	1.10E+00	U1/2		1.10E+00	2.2E+02	2.2E+00	7.0E+00	10	100	9.71E+02	97%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1316-T03-A	1	1.10E+00	U1/2		1.10E+00	7.0E+01	2.2E+00	7.0E+00				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1316-T04-A	1	1.10E+00	U1/2		1.10E+00	2.6E+02	2.2E+00	7.0E+00				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1316-T05-A	1	1.10E+00	U1/2		1.10E+00	4.9E+02	2.2E+00	7.0E+00				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1316-T01-B	1	1.10E+00	U1/2		1.10E+00	5.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1316-T02-B	1	1.10E+00	U1/2		1.10E+00	2.1E+02	2.2E+00	7.0E+00	10	100	9.37E+02	94%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1316-T03-B	1	1.10E+00	U1/2		1.10E+00	9.0E+01	2.2E+00	7.0E+00				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1316-T04-B	1	1.10E+00	U1/2		1.10E+00	1.0E+02	2.2E+00	7.0E+00				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1316-T05-B	1	1.10E+00	U1/2		1.10E+00	2.5E+02	2.2E+00	7.0E+00				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1316-T01-C	1	1.10E+00	U1/2		1.10E+00	6.6E+01	2.2E+00	7.0E+00				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1316-T02-C	1	1.10E+00	U1/2		1.10E+00	3.1E+02	2.2E+00	7.0E+00	10	100	1.01E+03	100%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1316-T03-C	1	1.10E+00	U1/2		1.10E+00	7.2E+02	2.2E+00	7.0E+00				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1316-T04-C	1	1.10E+00	U1/2		1.10E+00	9.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1316-T05-C	1	1.10E+00	U1/2		1.10E+00	6.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1316-B01-A	1	1.10E+00	U1/2		1.10E+00	8.8E+02	2.2E+00	7.0E+00				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1316-B02-A	1	1.10E+00	U1/2		1.10E+00	3.6E+02	2.2E+00	7.0E+00				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
Cd	SWA-L05-1316-B03-A	1	1.10E+00	U1/2		1.10E+00	2.1E+02	2.2E+00	7.0E+00				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	SWA-L05-1316-T01-A	1	9.56E+03			9.56E+03	9.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1316-T02-A	1	7.81E+03			7.81E+03	6.2E-01	2.6E+00	8.3E+00	1000	100	8.73E+03	92%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1316-T03-A	1	3.34E+03			3.34E+03	3.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1316-T04-A	1	3.76E+03			3.76E+03	8.5E+01	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1316-T05-A	1	3.56E+03			3.56E+03	2.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1316-T01-B	1	1.05E+04			1.05E+04	3.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1316-T02-B	1	7.60E+03			7.60E+03	6.3E-01	2.6E+00	8.3E+00	1000	100	8.51E+03	91%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1316-T03-B	1	3.63E+03			3.63E+03	7.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1316-T04-B	1	3.79E+03			3.79E+03	3.9E+00	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1316-T05-B	1	3.56E+03			3.56E+03	2.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1316-T01-C	1	9.84E+03			9.84E+03	8.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1316-T02-C	1	7.97E+03			7.97E+03	8.7E-01	2.6E+00	8.3E+00	1000	100	8.91E+03	94%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1316-T03-C	1	3.38E+03			3.38E+03	1.5E+02	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1316-T04-C	1	4.11E+03			4.11E+03	1.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1316-T05-C	1	3.36E+03			3.36E+03	2.8E+00	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1316-B01-A	1	1.30E+00	U1/2		1.30E+00	2.2E+02	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1316-B02-A	1	1.30E+00	U1/2		1.30E+00	1.5E+02	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
Ca	SWA-L05-1316-B03-A	1	1.30E+00	U1/2		1.30E+00	3.2E+02	2.6E+00	8.3E+00				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	SWA-L05-1316-T01-A	1	9.42E+02			9.42E+02	1.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1316-T02-A	1	1.32E+03			1.32E+03	6.6E-01	1.2E+00	3.8E+00	10	100	2.31E+03	98%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1316-T03-A	1	1.76E+03			1.76E+03	9.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1316-T04-A	1	1.89E+03			1.89E+03	8.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1316-T05-A	1	2.88E+03			2.88E+03	4.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1316-T01-B	1	9.47E+02			9.47E+02	9.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1316-T02-B	1	1.56E+03			1.56E+03	9.5E-01	1.2E+00	3.8E+00	10	100	2.50E+03	94%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1316-T03-B	1	1.82E+03			1.82E+03	1.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1316-T04-B	1	1.92E+03			1.92E+03	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1316-T05-B	1	2.62E+03			2.62E+03	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1316-T01-C	1	8.64E+02			8.64E+02	5.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1316-T02-C	1	1.42E+03			1.42E+03	4.2E-01	1.2E+00	3.8E+00	10	100	2.40E+03	98%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1316-T03-C	1	1.70E+03			1.70E+03	1.4E+02	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1316-T04-C	1	1.88E+03			1.88E+03	1.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1316-T05-C	1	2.92E+03			2.92E+03	9.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	2.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1316-B02-A	1	6.00E-01	U1/2		6.00E-01	6.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
Cr	SWA-L05-1316-B03-A	1	6.00E-01	U1/2		6.00E-01	1.1E+02	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	SWA-L05-1316-T01-A	1	9.00E-01	U1/2		9.00E-01	6.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1316-T02-A	1	9.00E-01	U1/2		9.00E-01	8.3E+02	1.8E+00	5.7E+00	10	100	9.26E+02	92%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1316-T03-A	1	9.00E-01	U1/2		9.00E-01	1.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1316-T04-A	1	9.00E-01	U1/2		9.00E-01	3.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1316-T05-A	1	5.18E+00	E		5.18E+00	3.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1316-T01-B	1	9.00E-01	U1/2		9.00E-01	4.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1316-T02-B	1	9.00E-01	U1/2		9.00E-01	8.6E+02	1.8E+00	5.7E+00	10	100	8.91E+02	89%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1316-T03-B	1	9.00E-01	U1/2		9.00E-01	3.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1316-T04-B	1	9.00E-01	U1/2		9.00E-01	9.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1316-T05-B	1	5.03E+00	E		5.03E+00	3.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1316-T01-C	1	9.00E-01	U1/2		9.00E-01	5.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1316-T02-C	1	9.00E-01	U1/2		9.00E-01	3.5E+02	1.8E+00	5.7E+00	10	100	9.18E+02	92%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1316-T03-C	1	9.00E-01	U1/2		9.00E-01	6.2E+04	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1316-T04-C	1	9.00E-01	U1/2		9.00E-01	4.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1316-T05-C	1	4.84E+00	E		4.84E+00	1.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	4.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1316-B02-A	1	9.00E-01	U1/2		9.00E-01	6.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
Co	SWA-L05-1316-B03-A	1	9.00E-01	U1/2		9.00E-01	7.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	SWA-L05-1316-T01-A	1	1.85E+00	U1/2		1.85E+00	1.6E+02	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1316-T02-A	1	6.46E+00	E		6.46E+00	1.6E+01	3.7E+00	1.2E+01	10	100	8.73E+02	87%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1316-T03-A	1	1.21E+01			1.21E+01	1.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1316-T04-A	1	2.35E+01			2.35E+01	9.6E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1316-T05-A	1	7.85E+01			7.85E+01	2.2E+00	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1316-T01-B	1	1.85E+00	U1/2		1.85E+00	2.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1316-T02-B	1	5.70E+00	E		5.70E+00	2.3E+01	3.7E+00	1.2E+01	10	100	8.60E+02	85%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1316-T03-B	1	1.10E+01	E		1.10E+01	1.9E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1316-T04-B	1	2.86E+01			2.86E+01	5.6E+00	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1316-T05-B	1	7.35E+01			7.35E+01	2.3E+00	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1316-T01-C	1	1.85E+00	U1/2		1.85E+00	2.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1316-T02-C	1	4.87E+00	E		4.87E+00	7.9E+01	3.7E+00	1.2E+01	10	100	8.53E+02	85%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1316-T03-C	1	1.11E+01	E		1.11E+01	1.5E+02	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1316-T04-C	1	2.71E+01			2.71E+01	1.5E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1316-T05-C	1	8.07E+01			8.07E+01	3.3E+00	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	1.3E+02	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1316-B02-A	1	1.85E+00	U1/2		1.85E+00	5.9E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
Cu	SWA-L05-1316-B03-A	1	1.85E+00	U1/2		1.85E+00	8.0E+01	3.7E+00	1.2E+01			---		VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	SWA-L05-1316-T01-A	1	7.81E+01			7.81E+01	1.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1316-T02-A	1	1.58E+02			1.58E+02	9.7E-01	2.0E+00	6.4E+00	1000	100	1.05E+03	90%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1316-T03-A	1	2.95E+02			2.95E+02	1.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1316-T04-A	1	4.31E+02			4.31E+02	9.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1316-T05-A	1	1.34E+03			1.34E+03	4.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1316-T01-B	1	7.16E+01			7.16E+01	3.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1316-T02-B	1	1.60E+02			1.60E+02	5.5E-01	2.0E+00	6.4E+00	1000	100	1.04E+03	88%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1316-T03-B	1	2.92E+02			2.92E+02	9.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1316-T04-B	1	5.91E+02			5.91E+02	5.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1316-T05-B	1	1.28E+03			1.28E+03	2.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1316-T01-C	1	7.77E+01			7.77E+01	3.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1316-T02-C	1	1.61E+02			1.61E+02	2.7E-01	2.0E+00	6.4E+00	1000	100	1.08E+03	92%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1316-T03-C	1	2.94E+02			2.94E+02	1.6E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1316-T04-C	1	6.53E+02			6.53E+02	1.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1316-T05-C	1	1.28E+03			1.28E+03	9.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	2.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1316-B02-A	1	1.00E+00	U1/2		1.00E+00	4.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
Fe	SWA-L05-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	3.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	SWA-L05-1316-T01-A	1	3.40E+00	U1/2		3.40E+00	6.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1316-T02-A	1	1.12E+01	E		1.12E+01	1.1E+01	6.8E+00	2.2E+01	10	100	9.92E+02	98%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1316-T03-A	1	6.27E+01			6.27E+01	1.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1316-T04-A	1	1.06E+02			1.06E+02	9.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1316-T05-A	1	2.45E+02			2.45E+02	1.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1316-T01-B	1	3.40E+00	U1/2		3.40E+00	2.7E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1316-T02-B	1	1.70E+01	E		1.70E+01	3.0E+01	6.8E+00	2.2E+01	10	100	9.61E+02	94%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1316-T03-B	1	5.82E+01			5.82E+01	3.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1316-T04-B	1	1.25E+02			1.25E+02	4.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1316-T05-B	1	2.23E+02			2.23E+02	1.3E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1316-T01-C	1	3.40E+00	U1/2		3.40E+00	1.1E+02	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1316-T02-C	1	1.60E+01	E		1.60E+01	1.1E+01	6.8E+00	2.2E+01	10	100	9.70E+02	95%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1316-T03-C	1	4.73E+01			4.73E+01	1.6E+02	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1316-T04-C	1	1.18E+02			1.18E+02	2.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1316-T05-C	1	2.22E+02			2.22E+02	2.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	2.2E+02	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1316-B02-A	1	3.40E+00	U1/2		3.40E+00	1.5E+02	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
Pb	SWA-L05-1316-B03-A	1	3.40E+00	U1/2		3.40E+00	1.4E+02	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	SWA-L05-1316-T01-A	1	2.00E+00	E		2.00E+00	6.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1316-T02-A	1	2.36E+00	E		2.36E+00	8.8E+00	1.9E+00	6.0E+00	10	100	8.95E+02	89%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1316-T03-A	1	5.77E+00	E		5.77E+00	4.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1316-T04-A	1	8.06E+00			8.06E+00	3.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1316-T05-A	1	1.04E+01			1.04E+01	1.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1316-T01-B	1	1.95E+00	E		1.95E+00	3.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1316-T02-B	1	2.68E+00	E		2.68E+00	5.6E+00	1.9E+00	6.0E+00	10	100	8.64E+02	86%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1316-T03-B	1	5.83E+00	E		5.83E+00	7.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1316-T04-B	1	8.32E+00			8.32E+00	1.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1316-T05-B	1	1.19E+01			1.19E+01	1.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1316-T01-C	1	2.02E+00	E		2.02E+00	4.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1316-T02-C	1	2.30E+00	E		2.30E+00	3.8E+00	1.9E+00	6.0E+00	10	100	8.71E+02	87%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1316-T03-C	1	5.30E+00	E		5.30E+00	3.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1316-T04-C	1	8.56E+00			8.56E+00	9.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1316-T05-C	1	1.17E+01			1.17E+01	2.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	9.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1316-B02-A	1	9.50E-01	U1/2		9.50E-01	9.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
Li	SWA-L05-1316-B03-A	1	9.50E-01	U1/2		9.50E-01	3.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	SWA-L05-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	2.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00	10	100	9.46E+02	94%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	1.0E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1316-T05-A	1	3.05E+00	E		3.05E+00	4.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	5.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00	10	100	9.13E+02	91%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	2.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	6.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1316-T05-B	1	3.12E+00	E		3.12E+00	2.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	3.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.0E+00	6.4E+00	10	100	9.30E+02	93%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	3.6E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	2.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1316-T05-C	1	3.05E+00	E		3.05E+00	6.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	3.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1316-B02-A	1	1.00E+00	U1/2		1.00E+00	6.3E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
Mn	SWA-L05-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	4.9E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	SWA-L05-1316-T01-A	1	5.00E-01	U1/2		5.00E-01	8.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1316-T02-A	1	5.00E-01	U1/2		5.00E-01	1.1E+02	1.0E+00	3.2E+00	1000	100	1.01E+03	101%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1316-T03-A	1	5.00E-01	U1/2		5.00E-01	7.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1316-T04-A	1	5.00E-01	U1/2		5.00E-01	1.5E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1316-T05-A	1	5.00E-01	U1/2		5.00E-01	3.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1316-T01-B	1	5.00E-01	U1/2		5.00E-01	4.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1316-T02-B	1	5.00E-01	U1/2		5.00E-01	1.2E+02	1.0E+00	3.2E+00	1000	100	9.29E+02	93%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1316-T03-B	1	5.00E-01	U1/2		5.00E-01	2.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1316-T04-B	1	5.00E-01	U1/2		5.00E-01	3.8E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1316-T05-B	1	5.00E-01	U1/2		5.00E-01	2.0E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1316-T01-C	1	5.00E-01	U1/2		5.00E-01	7.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1316-T02-C	1	5.00E-01	U1/2		5.00E-01	5.5E+01	1.0E+00	3.2E+00	1000	100	9.91E+02	99%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1316-T03-C	1	5.00E-01	U1/2		5.00E-01	1.2E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1316-T04-C	1	5.00E-01	U1/2		5.00E-01	6.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1316-T05-C	1	5.00E-01	U1/2		5.00E-01	5.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	5.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	2.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
Mg	SWA-L05-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	2.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	SWA-L05-1316-T01-A	1	1.04E+02			1.04E+02	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1316-T02-A	1	1.86E+02			1.86E+02	1.2E+00	1.2E+00	3.8E+00	10	100	1.30E+03	111%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1316-T03-A	1	4.04E+02			4.04E+02	3.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1316-T04-A	1	6.47E+02			6.47E+02	9.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1316-T05-A	1	1.26E+03			1.26E+03	5.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1316-T01-B	1	9.99E+01			9.99E+01	2.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1316-T02-B	1	1.93E+02			1.93E+02	4.3E-01	1.2E+00	3.8E+00	10	100	1.25E+03	106%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1316-T03-B	1	3.97E+02			3.97E+02	6.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1316-T04-B	1	6.52E+02			6.52E+02	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1316-T05-B	1	1.22E+03			1.22E+03	6.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1316-T01-C	1	1.03E+02			1.03E+02	3.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1316-T02-C	1	1.85E+02			1.85E+02	2.0E+00	1.2E+00	3.8E+00	10	100	1.26E+03	107%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1316-T03-C	1	3.84E+02			3.84E+02	1.4E+02	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1316-T04-C	1	6.89E+02			6.89E+02	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1316-T05-C	1	1.24E+03			1.24E+03	7.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1316-B01-A	1	1.29E+00	E		1.29E+00	1.1E+02	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1316-B02-A	1	6.00E-01	U1/2		6.00E-01	2.6E+02	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
Mo	SWA-L05-1316-B03-A	1	6.00E-01	U1/2		6.00E-01	7.8E+02	1.2E+00	3.8E+00				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	SWA-L05-1316-T01-A	1	9.00E-01	U1/2		9.00E-01	1.2E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1316-T02-A	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00	10	100	9.18E+02	92%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1316-T03-A	1	2.54E+00	E		2.54E+00	7.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1316-T04-A	1	5.62E+00	E		5.62E+00	1.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1316-T05-A	1	9.37E+00			9.37E+00	1.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1316-T01-B	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1316-T02-B	1	9.00E-01	U1/2		9.00E-01	2.0E+01	1.8E+00	5.7E+00	10	100	8.85E+02	88%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1316-T03-B	1	2.89E+00	E		2.89E+00	1.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1316-T04-B	1	6.24E+00			6.24E+00	2.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1316-T05-B	1	9.41E+00			9.41E+00	1.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1316-T01-C	1	9.00E-01	U1/2		9.00E-01	3.6E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1316-T02-C	1	9.00E-01	U1/2		9.00E-01	9.0E+01	1.8E+00	5.7E+00	10	100	9.63E+02	96%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1316-T03-C	1	2.85E+00	E		2.85E+00	2.7E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1316-T04-C	1	5.10E+00	E		5.10E+00	2.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1316-T05-C	1	1.10E+01			1.10E+01	1.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	5.3E+03	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1316-B02-A	1	9.00E-01	U1/2		9.00E-01	1.8E+03	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
Ni	SWA-L05-1316-B03-A	1	9.00E-01	U1/2		9.00E-01	2.9E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	SWA-L05-1316-T01-A	1	5.55E+01			5.55E+01	1.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1316-T02-A	1	1.14E+02			1.14E+02	1.0E+01	3.7E+00	1.2E+01	1000	100	1.08E+03	96%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1316-T03-A	1	4.23E+02			4.23E+02	2.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1316-T04-A	1	1.02E+03			1.02E+03	9.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1316-T05-A	1	2.32E+03			2.32E+03	5.7E-01	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1316-T01-B	1	5.15E+01			5.15E+01	2.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1316-T02-B	1	1.12E+02			1.12E+02	9.5E+00	3.7E+00	1.2E+01	1000	100	1.10E+03	99%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1316-T03-B	1	4.40E+02			4.40E+02	4.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1316-T04-B	1	1.01E+03			1.01E+03	1.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1316-T05-B	1	2.31E+03			2.31E+03	8.4E-01	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1316-T01-C	1	5.09E+01			5.09E+01	2.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1316-T02-C	1	1.15E+02			1.15E+02	1.4E+01	3.7E+00	1.2E+01	1000	100	1.03E+03	91%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1316-T03-C	1	4.53E+02			4.53E+02	1.4E+02	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1316-T04-C	1	1.01E+03			1.01E+03	2.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1316-T05-C	1	2.32E+03			2.32E+03	1.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	7.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1316-B02-A	1	1.85E+00	U1/2		1.85E+00	1.1E+04	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
P	SWA-L05-1316-B03-A	1	1.85E+00	U1/2		1.85E+00	5.3E+02	3.7E+00	1.2E+01				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	SWA-L05-1316-T01-A	1	2.43E+05			2.43E+05	1.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1316-T02-A	1	3.69E+05			3.69E+05	1.2E-01	1.6E+00	5.1E+00	1000	100	3.70E+05	93%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1316-T03-A	1	6.86E+05			6.86E+05	4.7E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1316-T04-A	1	1.73E+06			1.73E+06	8.6E+01	1.6E+00	5.1E+00				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1316-T05-A	1	2.53E+06			2.53E+06	1.5E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1316-T01-B	1	2.40E+05			2.40E+05	9.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1316-T02-B	1	3.73E+05			3.73E+05	4.8E-01	1.6E+00	5.1E+00	1000	100	3.74E+05	94%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1316-T03-B	1	6.67E+05			6.67E+05	1.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1316-T04-B	1	2.39E+06			2.39E+06	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1316-T05-B	1	2.51E+06			2.51E+06	7.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1316-T01-C	1	2.36E+05			2.36E+05	2.7E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1316-T02-C	1	3.67E+05			3.67E+05	4.6E-01	1.6E+00	5.1E+00	1000	100	3.68E+05	91%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1316-T03-C	1	6.74E+05			6.74E+05	1.3E+02	1.6E+00	5.1E+00				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1316-T04-C	1	2.40E+06			2.40E+06	1.5E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1316-T05-C	1	2.51E+06			2.51E+06	5.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1316-B01-A	1	4.21E+01			4.21E+01	2.1E+01	1.6E+00	5.1E+00				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1316-B02-A	1	4.15E+01			4.15E+01	2.3E+01	1.6E+00	5.1E+00				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
K	SWA-L05-1316-B03-A	1	4.03E+01			4.03E+01	2.4E+01	1.6E+00	5.1E+00				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	SWA-L05-1316-T01-A	1	6.84E+04			6.84E+04	2.2E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1316-T02-A	1	1.27E+05			1.27E+05	4.8E-01	1.5E+01	4.8E+01	10	100	1.28E+05	88%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1316-T03-A	1	2.77E+05			2.77E+05	7.4E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1316-T04-A	1	4.26E+05			4.26E+05	9.8E+01	1.5E+01	4.8E+01				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1316-T05-A	1	8.94E+05			8.94E+05	4.8E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1316-T01-B	1	6.67E+04			6.67E+04	2.3E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1316-T02-B	1	1.32E+05			1.32E+05	8.4E-01	1.5E+01	4.8E+01	10	100	1.33E+05	86%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1316-T03-B	1	2.72E+05			2.72E+05	5.1E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1316-T04-B	1	4.61E+05			4.61E+05	8.2E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1316-T05-B	1	8.68E+05			8.68E+05	3.1E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1316-T01-C	1	6.74E+04			6.74E+04	7.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1316-T02-C	1	1.28E+05			1.28E+05	4.8E-01	1.5E+01	4.8E+01	10	100	1.29E+05	92%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1316-T03-C	1	2.90E+05			2.90E+05	1.4E+02	1.5E+01	4.8E+01				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1316-T04-C	1	4.85E+05			4.85E+05	5.9E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1316-T05-C	1	8.79E+05			8.79E+05	1.2E+00	1.5E+01	4.8E+01				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1316-B01-A	1	7.50E+00	U1/2		7.50E+00	5.8E+02	1.5E+01	4.8E+01				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1316-B02-A	1	7.50E+00	U1/2		7.50E+00	9.5E+01	1.5E+01	4.8E+01				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
Se	SWA-L05-1316-B03-A	1	7.50E+00	U1/2		7.50E+00	1.2E+03	1.5E+01	4.8E+01				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	SWA-L05-1316-T01-A	1	2.02E+04			2.02E+04	7.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1316-T02-A	1	3.02E+04			3.02E+04	3.5E-01	1.1E+00	3.5E+00	1000	100	3.11E+04	89%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1316-T03-A	1	5.42E+04			5.42E+04	8.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1316-T04-A	1	7.59E+04			7.59E+04	8.9E+01	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1316-T05-A	1	1.03E+05			1.03E+05	1.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1316-T01-B	1	2.02E+04			2.02E+04	1.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1316-T02-B	1	3.25E+04			3.25E+04	1.1E+00	1.1E+00	3.5E+00	1000	100	3.34E+04	90%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1316-T03-B	1	5.60E+04			5.60E+04	1.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1316-T04-B	1	7.58E+04			7.58E+04	1.6E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1316-T05-B	1	1.03E+05			1.03E+05	4.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1316-T01-C	1	1.98E+04			1.98E+04	2.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1316-T02-C	1	3.01E+04			3.01E+04	7.2E-01	1.1E+00	3.5E+00	1000	100	3.10E+04	94%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1316-T03-C	1	5.55E+04			5.55E+04	1.2E+02	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1316-T04-C	1	7.54E+04			7.54E+04	2.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1316-T05-C	1	1.03E+05			1.03E+05	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1316-B01-A	1	7.13E+00			7.13E+00	3.7E+01	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1316-B02-A	1	9.78E+00			9.78E+00	6.6E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
Si	SWA-L05-1316-B03-A	1	9.08E+00			9.08E+00	3.0E+01	1.1E+00	3.5E+00				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	SWA-L05-1316-T01-A	1	3.84E+05			3.84E+05	1.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1316-T02-A	1	4.78E+05			4.78E+05	2.0E-01	2.5E+00	8.0E+00	1000	100	4.79E+05	84%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1316-T03-A	1	5.93E+05			5.93E+05	4.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1316-T04-A	1	4.59E+05			4.59E+05	5.7E+01	2.5E+00	8.0E+00				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1316-T05-A	1	6.15E+05			6.15E+05	1.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1316-T01-B	1	3.81E+05			3.81E+05	3.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1316-T02-B	1	4.79E+05			4.79E+05	1.8E-01	2.5E+00	8.0E+00	1000	100	4.80E+05	89%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1316-T03-B	1	5.89E+05			5.89E+05	7.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1316-T04-B	1	6.08E+05			6.08E+05	1.4E+00	2.5E+00	8.0E+00				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1316-T05-B	1	6.14E+05			6.14E+05	2.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1316-T01-C	1	3.80E+05			3.80E+05	2.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1316-T02-C	1	4.74E+05			4.74E+05	5.4E-01	2.5E+00	8.0E+00	1000	100	4.75E+05	87%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1316-T03-C	1	6.00E+05			6.00E+05	6.1E+01	2.5E+00	8.0E+00				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1316-T04-C	1	6.05E+05			6.05E+05	3.7E-02	2.5E+00	8.0E+00				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1316-T05-C	1	6.20E+05			6.20E+05	2.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1316-B01-A	1	1.25E+00	U1/2		1.25E+00	5.0E+01	2.5E+00	8.0E+00				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1316-B02-A	1	1.25E+00	U1/2		1.25E+00	5.6E+01	2.5E+00	8.0E+00				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
Na	SWA-L05-1316-B03-A	1	1.25E+00	U1/2		1.25E+00	3.8E+01	2.5E+00	8.0E+00				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	SWA-L05-1316-T01-A	1	2.37E+02			2.37E+02	8.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1316-T02-A	1	2.50E+02			2.50E+02	5.7E-01	1.0E+00	3.2E+00	1000	100	1.15E+03	90%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1316-T03-A	1	2.98E+02			2.98E+02	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1316-T04-A	1	3.41E+02			3.41E+02	8.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1316-T05-A	1	4.12E+02			4.12E+02	2.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1316-T01-B	1	2.48E+02			2.48E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1316-T02-B	1	2.43E+02			2.43E+02	7.4E-01	1.0E+00	3.2E+00	1000	100	1.16E+03	92%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1316-T03-B	1	2.96E+02			2.96E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1316-T04-B	1	3.41E+02			3.41E+02	5.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1316-T05-B	1	4.01E+02			4.01E+02	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1316-T01-C	1	2.36E+02			2.36E+02	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1316-T02-C	1	2.52E+02			2.52E+02	3.6E-02	1.0E+00	3.2E+00	1000	100	1.18E+03	93%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1316-T03-C	1	2.94E+02			2.94E+02	1.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1316-T04-C	1	3.41E+02			3.41E+02	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1316-T05-C	1	4.04E+02			4.04E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	9.1E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	5.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
Sr	SWA-L05-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	1.1E+03	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	SWA-L05-1316-T01-A	1	3.00E+05			3.00E+05	5.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1316-T02-A	1	4.62E+05			4.62E+05	2.8E-01	6.8E+00	2.2E+01	1000	100	4.63E+05	88%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1316-T03-A	1	9.67E+05			9.67E+05	7.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1316-T04-A	1	1.57E+06			1.57E+06	9.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1316-T05-A	1	2.52E+06			2.52E+06	3.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1316-T01-B	1	3.04E+05			3.04E+05	5.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1316-T02-B	1	4.55E+05			4.55E+05	8.7E-01	6.8E+00	2.2E+01	1000	100	4.56E+05	86%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1316-T03-B	1	9.56E+05			9.56E+05	8.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1316-T04-B	1	1.53E+06			1.53E+06	8.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1316-T05-B	1	2.48E+06			2.48E+06	7.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1316-T01-C	1	2.75E+05			2.75E+05	3.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1316-T02-C	1	4.70E+05			4.70E+05	5.3E-01	6.8E+00	2.2E+01	1000	100	4.71E+05	85%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1316-T03-C	1	9.60E+05			9.60E+05	1.4E+02	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1316-T04-C	1	1.59E+06			1.59E+06	5.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1316-T05-C	1	2.51E+06			2.51E+06	1.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	1.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1316-B02-A	1	3.40E+00	U1/2		3.40E+00	1.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
S	SWA-L05-1316-B03-A	1	3.40E+00	U1/2		3.40E+00	1.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	SWA-L05-1316-T01-A	1	2.30E+00	U1/2		2.30E+00	1.4E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
Tl	SWA-L05-1316-T02-A	1	2.30E+00	U1/2		2.30E+00	6.5E+02	4.6E+00	1.5E+01	10	100	9.76E+02	97%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
Tl	SWA-L05-1316-T03-A	1	2.30E+00	U1/2		2.30E+00	1.5E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
Tl	SWA-L05-1316-T04-A	1	2.30E+00	U1/2		2.30E+00	1.4E+03	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
Tl	SWA-L05-1316-T05-A	1	6.68E+00	E		6.68E+00	6.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
Tl	SWA-L05-1316-T01-B	1	2.30E+00	U1/2		2.30E+00	1.0E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
Tl	SWA-L05-1316-T02-B	1	2.30E+00	U1/2		2.30E+00	2.4E+02	4.6E+00	1.5E+01	10	100	9.36E+02	93%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
Tl	SWA-L05-1316-T03-B	1	2.30E+00	U1/2		2.30E+00	1.2E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
Tl	SWA-L05-1316-T04-B	1	2.30E+00	U1/2		2.30E+00	1.6E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
Tl	SWA-L05-1316-T05-B	1	6.17E+00	E		6.17E+00	1.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
Tl	SWA-L05-1316-T01-C	1	2.30E+00	U1/2		2.30E+00	3.8E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
Tl	SWA-L05-1316-T02-C	1	2.30E+00	U1/2		2.30E+00	8.7E+01	4.6E+00	1.5E+01	10	100	9.50E+02	95%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
Tl	SWA-L05-1316-T03-C	1	2.30E+00	U1/2		2.30E+00	1.6E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
Tl	SWA-L05-1316-T04-C	1	2.30E+00	U1/2		2.30E+00	1.8E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
Tl	SWA-L05-1316-T05-C	1	6.65E+00	E		6.65E+00	8.3E+00	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
Tl	SWA-L05-1316-B01-A	1	2.30E+00	U1/2		2.30E+00	3.8E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
Tl	SWA-L05-1316-B02-A	1	2.30E+00	U1/2		2.30E+00	1.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
Tl	SWA-L05-1316-B03-A	1	2.30E+00	U1/2		2.30E+00	2.8E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	SWA-L05-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	4.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	3.2E+01	2.0E+00	6.4E+00	10	100	1.12E+03	112%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	1.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	3.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1316-T05-A	1	2.86E+00	E		2.86E+00	4.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00	10	100	9.86E+02	99%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	3.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1316-T05-B	1	2.60E+00	E		2.60E+00	6.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	4.4E+01	2.0E+00	6.4E+00	10	100	1.03E+03	103%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	2.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	2.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1316-T05-C	1	2.53E+00	E		2.53E+00	1.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	5.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1316-B02-A	1	1.00E+00	U1/2		1.00E+00	6.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
Ti	SWA-L05-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	5.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	SWA-L05-1316-T01-A	1	3.14E+02			3.14E+02	1.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1316-T02-A	1	5.43E+02			5.43E+02	1.1E-01	1.5E+00	4.8E+00	10	100	1.58E+03	104%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1316-T03-A	1	1.10E+03			1.10E+03	8.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1316-T04-A	1	1.41E+03			1.41E+03	8.4E+01	1.5E+00	4.8E+00				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1316-T05-A	1	2.84E+03			2.84E+03	5.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1316-T01-B	1	3.04E+02			3.04E+02	1.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1316-T02-B	1	5.80E+02			5.80E+02	1.2E+00	1.5E+00	4.8E+00	10	100	1.52E+03	94%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1316-T03-B	1	1.10E+03			1.10E+03	1.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1316-T04-B	1	1.69E+03			1.69E+03	1.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1316-T05-B	1	2.78E+03			2.78E+03	7.1E-01	1.5E+00	4.8E+00				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1316-T01-C	1	2.98E+02			2.98E+02	4.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1316-T02-C	1	5.44E+02			5.44E+02	1.2E+00	1.5E+00	4.8E+00	10	100	1.51E+03	97%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1316-T03-C	1	1.06E+03			1.06E+03	1.4E+02	1.5E+00	4.8E+00				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1316-T04-C	1	1.72E+03			1.72E+03	7.8E-01	1.5E+00	4.8E+00				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1316-T05-C	1	2.82E+03			2.82E+03	9.8E-01	1.5E+00	4.8E+00				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1316-B01-A	1	7.50E-01	U1/2		7.50E-01	5.8E+01	1.5E+00	4.8E+00				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1316-B02-A	1	2.02E+00	E		2.02E+00	5.3E+01	1.5E+00	4.8E+00				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
V	SWA-L05-1316-B03-A	1	1.80E+00	E		1.80E+00	3.8E+01	1.5E+00	4.8E+00				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	SWA-L05-1316-T01-A	1	1.92E+00	E		1.92E+00	1.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:54 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1316-T02-A	1	2.76E+00	E		2.76E+00	5.0E+00	1.0E+00	3.2E+00	10	100	1.01E+03	101%	VU ICP-OES	3/7/11 1:56 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1316-T03-A	1	5.99E+00			5.99E+00	4.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:58 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1316-T04-A	1	1.22E+01			1.22E+01	8.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:59 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1316-T05-A	1	2.75E+01			2.75E+01	4.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:01 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1316-T01-B	1	1.45E+00	E		1.45E+00	1.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:03 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1316-T02-B	1	3.70E+00			3.70E+00	2.6E+00	1.0E+00	3.2E+00	10	100	9.75E+02	97%	VU ICP-OES	3/7/11 2:04 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1316-T03-B	1	6.12E+00			6.12E+00	6.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:06 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1316-T04-B	1	1.25E+01			1.25E+01	4.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:08 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1316-T05-B	1	3.02E+01			3.02E+01	2.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:09 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1316-T01-C	1	1.89E+00	E		1.89E+00	1.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:11 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1316-T02-C	1	3.08E+00	E		3.08E+00	9.0E+00	1.0E+00	3.2E+00	10	100	9.95E+02	99%	VU ICP-OES	3/7/11 2:13 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1316-T03-C	1	5.41E+00			5.41E+00	1.5E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:14 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1316-T04-C	1	1.17E+01			1.17E+01	5.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:16 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1316-T05-C	1	3.13E+01			3.13E+01	4.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 2:17 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1316-B01-A	1	2.07E+00	E		2.07E+00	1.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:49 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1316-B02-A	1	1.45E+00	E		1.45E+00	5.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:51 PM	EPA Interlab L05 1313-1316 SWA
Zn	SWA-L05-1316-B03-A	1	2.20E+00	E		2.20E+00	1.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/7/11 1:53 PM	EPA Interlab L05 1313-1316 SWA

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	SWA-L06-1316-T01-A	1	3.87E+04			3.87E+04	5.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:42 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1316-T02-A	1	5.78E+04			5.78E+04	4.6E-01	1.0E+00	3.2E+00	1000	100	5.86E+04	87%	VU ICP-OES	3/30/11 1:44 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1316-T03-A	1	7.12E+04			7.12E+04	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:46 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1316-T04-A	1	1.55E+05			1.55E+05	1.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:47 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1316-T01-B	1	3.84E+04			3.84E+04	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:49 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1316-T02-B	1	5.82E+04			5.82E+04	1.1E+00	1.0E+00	3.2E+00	1000	100	5.91E+04	93%	VU ICP-OES	3/30/11 1:50 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1316-T03-B	1	7.36E+04			7.36E+04	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:52 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1316-T04-B	1	1.55E+05			1.55E+05	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:54 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1316-T01-C	1	3.81E+04			3.81E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:57 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1316-T02-C	1	5.70E+04			5.70E+04	1.2E+00	1.0E+00	3.2E+00	1000	100	5.79E+04	89%	VU ICP-OES	3/30/11 1:59 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1316-T03-C	1	7.18E+04			7.18E+04	7.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 2:00 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1316-T04-C	1	1.54E+05			1.54E+05	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 2:02 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.9E+03	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1316-B01-B	1	5.00E-01	U1/2		5.00E-01	1.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
Al	SWA-L06-1316-B01-C	1	1.06E+00	E		1.06E+00	7.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	SWA-L06-1316-T01-A	1	4.77E+03			4.77E+03	8.6E-01	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 3:49 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L06-1316-T02-A	1	3.28E+03			3.28E+03	9.5E-01	7.5E+00	2.4E+01	10	100	4.17E+03	89%	VU ICP-OES	5/23/11 3:51 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L06-1316-T03-A	1	8.88E+03			8.88E+03	1.6E-01	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 3:53 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L06-1316-T04-A	1	8.61E+03			8.61E+03	4.7E-01	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 3:56 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L06-1316-T01-B	1	4.27E+03			4.27E+03	6.2E-01	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 3:58 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L06-1316-T02-B	1	3.86E+03			3.86E+03	4.0E+00	7.5E+00	2.4E+01	10	100	4.72E+03	86%	VU ICP-OES	5/23/11 4:00 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L06-1316-T03-B	1	9.49E+03			9.49E+03	1.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 4:02 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L06-1316-T04-B	1	8.85E+03			8.85E+03	1.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 4:05 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L06-1316-T01-C	1	4.16E+03			4.16E+03	1.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 4:07 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L06-1316-T02-C	1	3.23E+03			3.23E+03	3.0E+00	7.5E+00	2.4E+01	10	100	4.16E+03	92%	VU ICP-OES	5/23/11 4:09 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L06-1316-T03-C	1	9.50E+03			9.50E+03	1.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 4:12 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L06-1316-T04-C	1	8.92E+03			8.92E+03	9.6E-01	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 4:14 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L06-1316-B01-A	1	3.75E+00	U1/2		3.75E+00	2.4E+02	7.5E+00	2.4E+01				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1316-B01-B	1	3.75E+00	U1/2		3.75E+00	2.2E+02	7.5E+00	2.4E+01				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
Sb	SWA-L06-1316-B01-C	1	3.75E+00	U1/2		3.75E+00	2.3E+02	7.5E+00	2.4E+01				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	SWA-L06-1316-T01-A	1	5.00E+03			5.00E+03	6.6E-01	1.1E+01	3.5E+01				---	VU ICP-OES	3/30/11 1:42 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1316-T02-A	1	1.27E+04			1.27E+04	1.4E+00	1.1E+01	3.5E+01	10	100	1.37E+04	92%	VU ICP-OES	3/30/11 1:44 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1316-T03-A	1	4.09E+04			4.09E+04	2.5E-01	1.1E+01	3.5E+01				---	VU ICP-OES	3/30/11 1:46 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1316-T04-A	1	1.04E+05			1.04E+05	6.3E-01	1.1E+01	3.5E+01				---	VU ICP-OES	3/30/11 1:47 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1316-T01-B	1	4.89E+03			4.89E+03	2.9E-01	1.1E+01	3.5E+01				---	VU ICP-OES	3/30/11 1:49 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1316-T02-B	1	1.17E+04			1.17E+04	1.2E+00	1.1E+01	3.5E+01	10	100	1.26E+04	90%	VU ICP-OES	3/30/11 1:50 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1316-T03-B	1	4.12E+04			4.12E+04	4.9E-01	1.1E+01	3.5E+01				---	VU ICP-OES	3/30/11 1:52 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1316-T04-B	1	1.09E+05			1.09E+05	1.7E+00	1.1E+01	3.5E+01				---	VU ICP-OES	3/30/11 1:54 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1316-T01-C	1	4.91E+03			4.91E+03	1.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	3/30/11 1:57 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1316-T02-C	1	1.26E+04			1.26E+04	1.7E+00	1.1E+01	3.5E+01	10	100	1.34E+04	87%	VU ICP-OES	3/30/11 1:59 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1316-T03-C	1	4.13E+04			4.13E+04	1.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	3/30/11 2:00 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1316-T04-C	1	1.06E+05			1.06E+05	5.3E-01	1.1E+01	3.5E+01				---	VU ICP-OES	3/30/11 2:02 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1316-B01-A	1	5.50E+00	U1/2		5.50E+00	1.9E+02	1.1E+01	3.5E+01				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1316-B01-B	1	5.50E+00	U1/2		5.50E+00	2.2E+02	1.1E+01	3.5E+01				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
As	SWA-L06-1316-B01-C	1	5.50E+00	U1/2		5.50E+00	1.1E+02	1.1E+01	3.5E+01				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	SWA-L06-1316-T01-A	1	1.16E+03			1.16E+03	3.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:42 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1316-T02-A	1	1.79E+03			1.79E+03	8.7E-02	1.0E+00	3.2E+00	1000	100	2.80E+03	101%	VU ICP-OES	3/30/11 1:44 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1316-T03-A	1	2.08E+03			2.08E+03	1.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:46 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1316-T04-A	1	2.75E+03			2.75E+03	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:47 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1316-T01-B	1	1.15E+03			1.15E+03	1.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:49 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1316-T02-B	1	1.89E+03			1.89E+03	1.6E+00	1.0E+00	3.2E+00	1000	100	2.86E+03	97%	VU ICP-OES	3/30/11 1:50 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1316-T03-B	1	2.31E+03			2.31E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:52 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1316-T04-B	1	3.15E+03			3.15E+03	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:54 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1316-T01-C	1	1.13E+03			1.13E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:57 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1316-T02-C	1	1.77E+03			1.77E+03	2.0E-01	1.0E+00	3.2E+00	1000	100	2.95E+03	118%	VU ICP-OES	3/30/11 1:59 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1316-T03-C	1	2.09E+03			2.09E+03	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 2:00 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1316-T04-C	1	2.76E+03			2.76E+03	8.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 2:02 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1316-B01-A	1	4.53E+00			4.53E+00	4.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1316-B01-B	1	3.44E+00			3.44E+00	2.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
B	SWA-L06-1316-B01-C	1	4.75E+00			4.75E+00	6.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	SWA-L06-1316-T01-A	1	2.36E+02			2.36E+02	6.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 3:49 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L06-1316-T02-A	1	2.17E+02			2.17E+02	2.7E-01	1.0E+00	3.2E+00	10	100	1.16E+03	94%	VU ICP-OES	5/23/11 3:51 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L06-1316-T03-A	1	4.76E+01			4.76E+01	4.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 3:53 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L06-1316-T04-A	1	7.45E+01			7.45E+01	6.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 3:56 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L06-1316-T01-B	1	2.39E+02			2.39E+02	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 3:58 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L06-1316-T02-B	1	1.91E+02			1.91E+02	1.3E+00	1.0E+00	3.2E+00	10	100	1.12E+03	93%	VU ICP-OES	5/23/11 4:00 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L06-1316-T03-B	1	6.91E+01			6.91E+01	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:02 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L06-1316-T04-B	1	7.25E+01			7.25E+01	2.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:05 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L06-1316-T01-C	1	2.45E+02			2.45E+02	9.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:07 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L06-1316-T02-C	1	2.16E+02			2.16E+02	1.0E+00	1.0E+00	3.2E+00	10	100	1.15E+03	94%	VU ICP-OES	5/23/11 4:09 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L06-1316-T03-C	1	3.99E+01			3.99E+01	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:12 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L06-1316-T04-C	1	7.28E+01			7.28E+01	5.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:14 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L06-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	4.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1316-B01-B	1	5.00E-01	U1/2		5.00E-01	3.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
Ba	SWA-L06-1316-B01-C	1	5.00E-01	U1/2		5.00E-01	3.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	SWA-L06-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	7.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/30/11 1:42 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	2.3E+02	1.9E+00	6.0E+00	10	100	1.13E+03	113%	VU ICP-OES	3/30/11 1:44 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	9.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/30/11 1:46 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	2.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/30/11 1:47 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	9.1E-01	1.9E+00	6.0E+00				---	VU ICP-OES	3/30/11 1:49 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	1.9E+01	1.9E+00	6.0E+00	10	100	1.20E+03	119%	VU ICP-OES	3/30/11 1:50 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	2.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/30/11 1:52 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	6.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/30/11 1:54 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	1.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/30/11 1:57 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	2.2E+01	1.9E+00	6.0E+00	10	100	1.13E+03	113%	VU ICP-OES	3/30/11 1:59 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	6.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/30/11 2:00 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	6.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/30/11 2:02 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	2.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1316-B01-B	1	9.50E-01	U1/2		9.50E-01	8.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
Be	SWA-L06-1316-B01-C	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	SWA-L06-1316-T01-A	1	1.10E+00	U1/2		1.10E+00	5.5E+02	2.2E+00	7.0E+00				---	VU ICP-OES	3/30/11 1:42 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1316-T02-A	1	1.10E+00	U1/2		1.10E+00	7.8E+00	2.2E+00	7.0E+00	10	100	1.16E+03	116%	VU ICP-OES	3/30/11 1:44 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1316-T03-A	1	1.10E+00	U1/2		1.10E+00	2.1E+03	2.2E+00	7.0E+00				---	VU ICP-OES	3/30/11 1:46 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1316-T04-A	1	1.10E+00	U1/2		1.10E+00	1.2E+03	2.2E+00	7.0E+00				---	VU ICP-OES	3/30/11 1:47 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1316-T01-B	1	1.10E+00	U1/2		1.10E+00	2.4E+02	2.2E+00	7.0E+00				---	VU ICP-OES	3/30/11 1:49 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1316-T02-B	1	1.10E+00	U1/2		1.10E+00	8.0E+01	2.2E+00	7.0E+00	10	100	1.12E+03	112%	VU ICP-OES	3/30/11 1:50 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1316-T03-B	1	1.10E+00	U1/2		1.10E+00	5.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	3/30/11 1:52 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1316-T04-B	1	1.10E+00	U1/2		1.10E+00	2.9E+02	2.2E+00	7.0E+00				---	VU ICP-OES	3/30/11 1:54 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1316-T01-C	1	1.10E+00	U1/2		1.10E+00	1.1E+02	2.2E+00	7.0E+00				---	VU ICP-OES	3/30/11 1:57 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1316-T02-C	1	1.10E+00	U1/2		1.10E+00	1.1E+02	2.2E+00	7.0E+00	10	100	1.15E+03	115%	VU ICP-OES	3/30/11 1:59 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1316-T03-C	1	1.10E+00	U1/2		1.10E+00	4.0E+01	2.2E+00	7.0E+00				---	VU ICP-OES	3/30/11 2:00 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1316-T04-C	1	1.10E+00	U1/2		1.10E+00	5.1E+02	2.2E+00	7.0E+00				---	VU ICP-OES	3/30/11 2:02 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1316-B01-A	1	1.10E+00	U1/2		1.10E+00	5.1E+03	2.2E+00	7.0E+00				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1316-B01-B	1	1.10E+00	U1/2		1.10E+00	9.3E+01	2.2E+00	7.0E+00				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
Cd	SWA-L06-1316-B01-C	1	1.10E+00	U1/2		1.10E+00	4.7E+02	2.2E+00	7.0E+00				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	SWA-L06-1316-T01-A	1	1.32E+04			1.32E+04	3.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/23/11 3:49 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L06-1316-T02-A	1	1.04E+04			1.04E+04	7.4E-01	2.6E+00	8.3E+00	1000	100	1.13E+04	92%	VU ICP-OES	5/23/11 3:51 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L06-1316-T03-A	1	3.57E+03			3.57E+03	1.6E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/23/11 3:53 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L06-1316-T04-A	1	6.68E+03			6.68E+03	5.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/23/11 3:56 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L06-1316-T01-B	1	1.32E+04			1.32E+04	1.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/23/11 3:58 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L06-1316-T02-B	1	1.02E+04			1.02E+04	1.5E+00	2.6E+00	8.3E+00	1000	100	1.11E+04	88%	VU ICP-OES	5/23/11 4:00 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L06-1316-T03-B	1	3.63E+03			3.63E+03	2.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/23/11 4:02 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L06-1316-T04-B	1	6.65E+03			6.65E+03	2.9E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/23/11 4:05 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L06-1316-T01-C	1	1.32E+04			1.32E+04	1.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/23/11 4:07 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L06-1316-T02-C	1	1.03E+04			1.03E+04	1.2E-01	2.6E+00	8.3E+00	1000	100	1.12E+04	93%	VU ICP-OES	5/23/11 4:09 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L06-1316-T03-C	1	3.35E+03			3.35E+03	1.6E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/23/11 4:12 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L06-1316-T04-C	1	7.02E+03			7.02E+03	4.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/23/11 4:14 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L06-1316-B01-A	1	6.21E+00	E		6.21E+00	1.1E+01	2.6E+00	8.3E+00				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1316-B01-B	1	1.30E+00	U1/2		1.30E+00	1.2E+02	2.6E+00	8.3E+00				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
Ca	SWA-L06-1316-B01-C	1	5.34E+00	E		5.34E+00	7.3E+01	2.6E+00	8.3E+00				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	SWA-L06-1316-T01-A	1	1.11E+03			1.11E+03	8.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/30/11 1:42 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1316-T02-A	1	1.79E+03			1.79E+03	8.1E-01	1.2E+00	3.8E+00	10	100	2.70E+03	91%	VU ICP-OES	3/30/11 1:44 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1316-T03-A	1	1.33E+03			1.33E+03	7.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/30/11 1:46 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1316-T04-A	1	2.02E+03			2.02E+03	2.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/30/11 1:47 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1316-T01-B	1	1.10E+03			1.10E+03	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/30/11 1:49 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1316-T02-B	1	1.83E+03			1.83E+03	5.3E-01	1.2E+00	3.8E+00	10	100	2.76E+03	93%	VU ICP-OES	3/30/11 1:50 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1316-T03-B	1	1.48E+03			1.48E+03	8.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/30/11 1:52 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1316-T04-B	1	2.03E+03			2.03E+03	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/30/11 1:54 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1316-T01-C	1	1.10E+03			1.10E+03	7.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/30/11 1:57 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1316-T02-C	1	1.77E+03			1.77E+03	1.0E+00	1.2E+00	3.8E+00	10	100	2.85E+03	108%	VU ICP-OES	3/30/11 1:59 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1316-T03-C	1	1.36E+03			1.36E+03	9.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/30/11 2:00 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1316-T04-C	1	2.06E+03			2.06E+03	1.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/30/11 2:02 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	4.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1316-B01-B	1	6.00E-01	U1/2		6.00E-01	8.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
Cr	SWA-L06-1316-B01-C	1	6.00E-01	U1/2		6.00E-01	7.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	SWA-L06-1316-T01-A	1	9.00E-01	U1/2		9.00E-01	2.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/30/11 1:42 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1316-T02-A	1	9.00E-01	U1/2		9.00E-01	1.5E+03	1.8E+00	5.7E+00	10	100	1.13E+03	113%	VU ICP-OES	3/30/11 1:44 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1316-T03-A	1	3.42E+00	E		3.42E+00	1.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/30/11 1:46 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1316-T04-A	1	4.90E+00	E		4.90E+00	4.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	3/30/11 1:47 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1316-T01-B	1	9.00E-01	U1/2		9.00E-01	3.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/30/11 1:49 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1316-T02-B	1	9.00E-01	U1/2		9.00E-01	6.9E+01	1.8E+00	5.7E+00	10	100	1.10E+03	110%	VU ICP-OES	3/30/11 1:50 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1316-T03-B	1	2.32E+00	E		2.32E+00	2.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/30/11 1:52 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1316-T04-B	1	6.18E+00			6.18E+00	1.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/30/11 1:54 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1316-T01-C	1	9.00E-01	U1/2		9.00E-01	2.1E+03	1.8E+00	5.7E+00				---	VU ICP-OES	3/30/11 1:57 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1316-T02-C	1	9.00E-01	U1/2		9.00E-01	2.9E+02	1.8E+00	5.7E+00	10	100	1.12E+03	112%	VU ICP-OES	3/30/11 1:59 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1316-T03-C	1	2.86E+00	E		2.86E+00	1.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/30/11 2:00 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1316-T04-C	1	4.87E+00	E		4.87E+00	6.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	3/30/11 2:02 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	2.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1316-B01-B	1	9.00E-01	U1/2		9.00E-01	1.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
Co	SWA-L06-1316-B01-C	1	9.00E-01	U1/2		9.00E-01	5.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	SWA-L06-1316-T01-A	1	1.85E+00	U1/2		1.85E+00	1.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/30/11 1:42 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1316-T02-A	1	3.93E+00	E		3.93E+00	1.9E+01	3.7E+00	1.2E+01	10	100	1.11E+03	110%	VU ICP-OES	3/30/11 1:44 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1316-T03-A	1	1.06E+01	E		1.06E+01	1.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/30/11 1:46 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1316-T04-A	1	4.69E+01			4.69E+01	4.8E-01	3.7E+00	1.2E+01				---	VU ICP-OES	3/30/11 1:47 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1316-T01-B	1	1.85E+00	U1/2		1.85E+00	1.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/30/11 1:49 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1316-T02-B	1	4.25E+00	E		4.25E+00	9.7E+00	3.7E+00	1.2E+01	10	100	1.03E+03	103%	VU ICP-OES	3/30/11 1:50 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1316-T03-B	1	1.08E+01	E		1.08E+01	5.0E-01	3.7E+00	1.2E+01				---	VU ICP-OES	3/30/11 1:52 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1316-T04-B	1	4.49E+01			4.49E+01	3.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/30/11 1:54 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1316-T01-C	1	1.85E+00	U1/2		1.85E+00	1.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/30/11 1:57 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1316-T02-C	1	4.65E+00	E		4.65E+00	1.0E+02	3.7E+00	1.2E+01	10	100	1.13E+03	113%	VU ICP-OES	3/30/11 1:59 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1316-T03-C	1	1.05E+01	E		1.05E+01	6.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/30/11 2:00 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1316-T04-C	1	4.70E+01			4.70E+01	1.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/30/11 2:02 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	2.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1316-B01-B	1	1.85E+00	U1/2		1.85E+00	3.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
Cu	SWA-L06-1316-B01-C	1	1.85E+00	U1/2		1.85E+00	5.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	SWA-L06-1316-T01-A	1	7.92E+01			7.92E+01	6.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:42 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1316-T02-A	1	1.59E+02			1.59E+02	5.5E-01	2.0E+00	6.4E+00	1000	100	1.30E+03	114%	VU ICP-OES	3/30/11 1:44 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1316-T03-A	1	2.55E+02			2.55E+02	2.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:46 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1316-T04-A	1	8.67E+02			8.67E+02	3.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:47 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1316-T01-B	1	7.91E+01			7.91E+01	5.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:49 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1316-T02-B	1	1.62E+02			1.62E+02	1.7E+00	2.0E+00	6.4E+00	1000	100	1.26E+03	110%	VU ICP-OES	3/30/11 1:50 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1316-T03-B	1	2.38E+02			2.38E+02	5.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:52 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1316-T04-B	1	9.18E+02			9.18E+02	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:54 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1316-T01-C	1	7.82E+01			7.82E+01	8.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:57 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1316-T02-C	1	1.59E+02			1.59E+02	9.5E-01	2.0E+00	6.4E+00	1000	100	1.30E+03	114%	VU ICP-OES	3/30/11 1:59 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1316-T03-C	1	2.57E+02			2.57E+02	7.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 2:00 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1316-T04-C	1	8.84E+02			8.84E+02	6.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 2:02 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	9.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1316-B01-B	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
Fe	SWA-L06-1316-B01-C	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	SWA-L06-1316-T01-A	1	1.55E+01	E		1.55E+01	2.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/30/11 1:42 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1316-T02-A	1	3.00E+01			3.00E+01	9.5E+00	6.8E+00	2.2E+01	10	100	1.16E+03	113%	VU ICP-OES	3/30/11 1:44 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1316-T03-A	1	6.86E+00	E		6.86E+00	4.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/30/11 1:46 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1316-T04-A	1	1.38E+02			1.38E+02	8.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/30/11 1:47 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1316-T01-B	1	1.86E+01	E		1.86E+01	3.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/30/11 1:49 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1316-T02-B	1	3.05E+01			3.05E+01	1.4E+01	6.8E+00	2.2E+01	10	100	1.12E+03	109%	VU ICP-OES	3/30/11 1:50 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1316-T03-B	1	7.12E+00	E		7.12E+00	1.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/30/11 1:52 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1316-T04-B	1	1.19E+02			1.19E+02	7.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/30/11 1:54 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1316-T01-C	1	1.94E+01	E		1.94E+01	2.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/30/11 1:57 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1316-T02-C	1	3.14E+01			3.14E+01	1.4E+01	6.8E+00	2.2E+01	10	100	1.16E+03	113%	VU ICP-OES	3/30/11 1:59 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1316-T03-C	1	9.19E+00	E		9.19E+00	2.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/30/11 2:00 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1316-T04-C	1	1.39E+02			1.39E+02	2.8E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/30/11 2:02 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	1.2E+02	6.8E+00	2.2E+01				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1316-B01-B	1	3.40E+00	U1/2		3.40E+00	9.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
Pb	SWA-L06-1316-B01-C	1	3.40E+00	U1/2		3.40E+00	4.7E+02	6.8E+00	2.2E+01				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	SWA-L06-1316-T01-A	1	3.25E+00	E		3.25E+00	9.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/30/11 1:42 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1316-T02-A	1	4.53E+00	E		4.53E+00	5.7E+00	1.9E+00	6.0E+00	10	100	9.23E+02	92%	VU ICP-OES	3/30/11 1:44 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1316-T03-A	1	5.60E+00	E		5.60E+00	4.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/30/11 1:46 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1316-T04-A	1	9.62E+00			9.62E+00	4.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/30/11 1:47 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1316-T01-B	1	2.96E+00	E		2.96E+00	7.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/30/11 1:49 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1316-T02-B	1	4.66E+00	E		4.66E+00	3.6E+00	1.9E+00	6.0E+00	10	100	8.95E+02	89%	VU ICP-OES	3/30/11 1:50 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1316-T03-B	1	5.83E+00	E		5.83E+00	1.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/30/11 1:52 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1316-T04-B	1	9.34E+00			9.34E+00	8.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/30/11 1:54 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1316-T01-C	1	2.62E+00	E		2.62E+00	4.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/30/11 1:57 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1316-T02-C	1	4.61E+00	E		4.61E+00	1.1E+01	1.9E+00	6.0E+00	10	100	9.22E+02	92%	VU ICP-OES	3/30/11 1:59 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1316-T03-C	1	5.71E+00	E		5.71E+00	8.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/30/11 2:00 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1316-T04-C	1	8.48E+00			8.48E+00	8.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/30/11 2:02 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	4.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1316-B01-B	1	9.50E-01	U1/2		9.50E-01	5.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
Li	SWA-L06-1316-B01-C	1	9.50E-01	U1/2		9.50E-01	4.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	SWA-L06-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	2.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:42 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	1.5E+00	2.0E+00	6.4E+00	10	100	1.13E+03	113%	VU ICP-OES	3/30/11 1:44 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:46 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1316-T04-A	1	2.96E+00	E		2.96E+00	5.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:47 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	2.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:49 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00	10	100	1.11E+03	111%	VU ICP-OES	3/30/11 1:50 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	3.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:52 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1316-T04-B	1	2.39E+00	E		2.39E+00	3.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:54 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	4.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:57 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	1.4E+00	2.0E+00	6.4E+00	10	100	1.13E+03	113%	VU ICP-OES	3/30/11 1:59 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 2:00 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1316-T04-C	1	2.61E+00	E		2.61E+00	6.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 2:02 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1316-B01-B	1	1.00E+00	U1/2		1.00E+00	5.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
Mn	SWA-L06-1316-B01-C	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	SWA-L06-1316-T01-A	1	6.40E+00			6.40E+00	7.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:42 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1316-T02-A	1	6.68E+00			6.68E+00	1.4E+02	1.0E+00	3.2E+00	1000	100	1.07E+03	106%	VU ICP-OES	3/30/11 1:44 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1316-T03-A	1	1.14E+01			1.14E+01	5.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:46 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1316-T04-A	1	1.02E+01			1.02E+01	4.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:47 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1316-T01-B	1	6.09E+00			6.09E+00	6.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:49 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1316-T02-B	1	6.52E+00			6.52E+00	2.3E+01	1.0E+00	3.2E+00	1000	100	1.01E+03	100%	VU ICP-OES	3/30/11 1:50 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1316-T03-B	1	8.59E+00			8.59E+00	2.1E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:52 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1316-T04-B	1	9.35E+00			9.35E+00	2.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:54 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1316-T01-C	1	5.93E+00			5.93E+00	4.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:57 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1316-T02-C	1	6.04E+00			6.04E+00	8.8E+01	1.0E+00	3.2E+00	1000	100	1.05E+03	104%	VU ICP-OES	3/30/11 1:59 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1316-T03-C	1	1.06E+01			1.06E+01	1.6E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 2:00 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1316-T04-C	1	8.84E+00			8.84E+00	2.2E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 2:02 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1316-B01-A	1	2.58E+00	E		2.58E+00	1.8E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1316-B01-B	1	5.00E-01	U1/2		5.00E-01	4.2E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
Mg	SWA-L06-1316-B01-C	1	5.00E-01	U1/2		5.00E-01	2.2E+03	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	SWA-L06-1316-T01-A	1	1.29E+02			1.29E+02	7.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/30/11 1:42 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1316-T02-A	1	1.93E+02			1.93E+02	4.3E-01	1.2E+00	3.8E+00	10	100	1.37E+03	117%	VU ICP-OES	3/30/11 1:44 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1316-T03-A	1	5.24E+02			5.24E+02	6.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/30/11 1:46 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1316-T04-A	1	1.04E+03			1.04E+03	1.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/30/11 1:47 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1316-T01-B	1	1.29E+02			1.29E+02	6.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/30/11 1:49 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1316-T02-B	1	1.80E+02			1.80E+02	1.3E+00	1.2E+00	3.8E+00	10	100	1.30E+03	112%	VU ICP-OES	3/30/11 1:50 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1316-T03-B	1	5.27E+02			5.27E+02	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/30/11 1:52 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1316-T04-B	1	1.07E+03			1.07E+03	6.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/30/11 1:54 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1316-T01-C	1	1.26E+02			1.26E+02	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/30/11 1:57 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1316-T02-C	1	1.91E+02			1.91E+02	8.3E-01	1.2E+00	3.8E+00	10	100	1.35E+03	116%	VU ICP-OES	3/30/11 1:59 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1316-T03-C	1	5.23E+02			5.23E+02	5.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/30/11 2:00 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1316-T04-C	1	1.04E+03			1.04E+03	2.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	3/30/11 2:02 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	2.5E+02	1.2E+00	3.8E+00				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1316-B01-B	1	6.00E-01	U1/2		6.00E-01	5.6E+02	1.2E+00	3.8E+00				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
Mo	SWA-L06-1316-B01-C	1	6.00E-01	U1/2		6.00E-01	5.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	SWA-L06-1316-T01-A	1	9.00E-01	U1/2		9.00E-01	5.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/30/11 1:42 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1316-T02-A	1	9.00E-01	U1/2		9.00E-01	2.5E+01	1.8E+00	5.7E+00	10	100	1.13E+03	113%	VU ICP-OES	3/30/11 1:44 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1316-T03-A	1	2.53E+00	E		2.53E+00	3.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/30/11 1:46 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1316-T04-A	1	4.63E+00	E		4.63E+00	3.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/30/11 1:47 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1316-T01-B	1	9.00E-01	U1/2		9.00E-01	7.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/30/11 1:49 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1316-T02-B	1	9.00E-01	U1/2		9.00E-01	3.5E+01	1.8E+00	5.7E+00	10	100	1.09E+03	109%	VU ICP-OES	3/30/11 1:50 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1316-T03-B	1	2.42E+00	E		2.42E+00	1.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/30/11 1:52 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1316-T04-B	1	5.43E+00	E		5.43E+00	2.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/30/11 1:54 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1316-T01-C	1	9.00E-01	U1/2		9.00E-01	6.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/30/11 1:57 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1316-T02-C	1	9.00E-01	U1/2		9.00E-01	3.7E+01	1.8E+00	5.7E+00	10	100	1.12E+03	112%	VU ICP-OES	3/30/11 1:59 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1316-T03-C	1	2.61E+00	E		2.61E+00	4.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/30/11 2:00 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1316-T04-C	1	4.15E+00	E		4.15E+00	5.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/30/11 2:02 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	2.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1316-B01-B	1	9.00E-01	U1/2		9.00E-01	1.2E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
Ni	SWA-L06-1316-B01-C	1	9.00E-01	U1/2		9.00E-01	1.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	SWA-L06-1316-T01-A	1	3.98E+01			3.98E+01	3.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/30/11 1:42 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1316-T02-A	1	1.14E+02			1.14E+02	3.6E+00	3.7E+00	1.2E+01	1000	100	1.17E+03	106%	VU ICP-OES	3/30/11 1:44 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1316-T03-A	1	4.19E+02			4.19E+02	6.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/30/11 1:46 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1316-T04-A	1	1.41E+03			1.41E+03	1.8E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/30/11 1:47 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1316-T01-B	1	4.11E+01			4.11E+01	2.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/30/11 1:49 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1316-T02-B	1	1.04E+02			1.04E+02	1.4E+01	3.7E+00	1.2E+01	1000	100	1.10E+03	100%	VU ICP-OES	3/30/11 1:50 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1316-T03-B	1	4.01E+02			4.01E+02	2.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/30/11 1:52 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1316-T04-B	1	1.41E+03			1.41E+03	1.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/30/11 1:54 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1316-T01-C	1	4.25E+01			4.25E+01	1.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/30/11 1:57 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1316-T02-C	1	1.02E+02			1.02E+02	6.3E+00	3.7E+00	1.2E+01	1000	100	1.12E+03	102%	VU ICP-OES	3/30/11 1:59 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1316-T03-C	1	4.15E+02			4.15E+02	3.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/30/11 2:00 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1316-T04-C	1	1.39E+03			1.39E+03	1.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/30/11 2:02 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	2.9E+02	3.7E+00	1.2E+01				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1316-B01-B	1	1.85E+00	U1/2		1.85E+00	5.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
P	SWA-L06-1316-B01-C	1	1.85E+00	U1/2		1.85E+00	1.1E+03	3.7E+00	1.2E+01				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	SWA-L06-1316-T01-A	1	3.30E+05			3.30E+05	8.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/30/11 1:42 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1316-T02-A	1	4.95E+05			4.95E+05	1.9E+00	1.6E+00	5.1E+00	1000	100	4.96E+05	86%	VU ICP-OES	3/30/11 1:44 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1316-T03-A	1	8.39E+05			8.39E+05	1.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/30/11 1:46 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1316-T04-A	1	3.12E+06			3.12E+06	3.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/30/11 1:47 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1316-T01-B	1	3.29E+05			3.29E+05	9.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/30/11 1:49 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1316-T02-B	1	4.94E+05			4.94E+05	1.0E+00	1.6E+00	5.1E+00	1000	100	4.95E+05	92%	VU ICP-OES	3/30/11 1:50 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1316-T03-B	1	8.51E+05			8.51E+05	2.7E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/30/11 1:52 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1316-T04-B	1	3.16E+06			3.16E+06	8.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/30/11 1:54 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1316-T01-C	1	3.28E+05			3.28E+05	7.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/30/11 1:57 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1316-T02-C	1	4.96E+05			4.96E+05	1.8E+00	1.6E+00	5.1E+00	1000	100	4.97E+05	91%	VU ICP-OES	3/30/11 1:59 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1316-T03-C	1	9.13E+05			9.13E+05	1.1E+01	1.6E+00	5.1E+00				---	VU ICP-OES	3/30/11 2:00 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1316-T04-C	1	3.22E+06			3.22E+06	6.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/30/11 2:02 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1316-B01-A	1	2.17E+01			2.17E+01	3.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1316-B01-B	1	2.41E+01			2.41E+01	9.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
K	SWA-L06-1316-B01-C	1	2.52E+01			2.52E+01	1.4E+01	1.6E+00	5.1E+00				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	SWA-L06-1316-T01-A	1	9.38E+04			9.38E+04	3.5E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/30/11 1:42 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1316-T02-A	1	1.66E+05			1.66E+05	2.7E-01	1.5E+01	4.8E+01	10	100	1.66E+05	87%	VU ICP-OES	3/30/11 1:44 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1316-T03-A	1	3.81E+05			3.81E+05	6.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/30/11 1:46 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1316-T04-A	1	7.12E+05			7.12E+05	1.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/30/11 1:47 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1316-T01-B	1	9.26E+04			9.26E+04	4.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/30/11 1:49 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1316-T02-B	1	1.66E+05			1.66E+05	1.6E+00	1.5E+01	4.8E+01	10	100	1.67E+05	96%	VU ICP-OES	3/30/11 1:50 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1316-T03-B	1	3.88E+05			3.88E+05	1.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	3/30/11 1:52 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1316-T04-B	1	7.44E+05			7.44E+05	7.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/30/11 1:54 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1316-T01-C	1	9.20E+04			9.20E+04	9.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/30/11 1:57 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1316-T02-C	1	1.63E+05			1.63E+05	9.7E-01	1.5E+01	4.8E+01	10	100	1.64E+05	90%	VU ICP-OES	3/30/11 1:59 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1316-T03-C	1	3.84E+05			3.84E+05	5.9E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/30/11 2:00 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1316-T04-C	1	7.10E+05			7.10E+05	2.3E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/30/11 2:02 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1316-B01-A	1	7.50E+00	U1/2		7.50E+00	7.4E+01	1.5E+01	4.8E+01				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1316-B01-B	1	7.50E+00	U1/2		7.50E+00	5.8E+01	1.5E+01	4.8E+01				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
Se	SWA-L06-1316-B01-C	1	7.50E+00	U1/2		7.50E+00	1.7E+01	1.5E+01	4.8E+01				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	SWA-L06-1316-T01-A	1	2.65E+04			2.65E+04	3.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/30/11 1:42 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1316-T02-A	1	3.66E+04			3.66E+04	3.9E-01	1.1E+00	3.5E+00	1000	100	3.76E+04	97%	VU ICP-OES	3/30/11 1:44 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1316-T03-A	1	2.24E+04			2.24E+04	5.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/30/11 1:46 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1316-T04-A	1	7.31E+04			7.31E+04	6.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/30/11 1:47 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1316-T01-B	1	2.64E+04			2.64E+04	3.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/30/11 1:49 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1316-T02-B	1	3.76E+04			3.76E+04	1.0E+00	1.1E+00	3.5E+00	1000	100	3.85E+04	90%	VU ICP-OES	3/30/11 1:50 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1316-T03-B	1	2.13E+04			2.13E+04	3.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/30/11 1:52 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1316-T04-B	1	6.99E+04			6.99E+04	7.4E-02	1.1E+00	3.5E+00				---	VU ICP-OES	3/30/11 1:54 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1316-T01-C	1	2.60E+04			2.60E+04	7.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/30/11 1:57 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1316-T02-C	1	3.64E+04			3.64E+04	9.7E-02	1.1E+00	3.5E+00	1000	100	3.73E+04	90%	VU ICP-OES	3/30/11 1:59 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1316-T03-C	1	2.27E+04			2.27E+04	7.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/30/11 2:00 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1316-T04-C	1	7.34E+04			7.34E+04	3.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/30/11 2:02 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1316-B01-A	1	5.50E-01	U1/2		5.50E-01	5.3E+02	1.1E+00	3.5E+00				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1316-B01-B	1	1.61E+00	E		1.61E+00	1.6E+02	1.1E+00	3.5E+00				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
Si	SWA-L06-1316-B01-C	1	1.29E+00	E		1.29E+00	4.4E+01	1.1E+00	3.5E+00				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	SWA-L06-1316-T01-A	1	5.13E+05			5.13E+05	4.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/30/11 1:42 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1316-T02-A	1	6.32E+05			6.32E+05	2.9E-01	2.5E+00	8.0E+00	1000	100	6.32E+05	86%	VU ICP-OES	3/30/11 1:44 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1316-T03-A	1	7.37E+05			7.37E+05	1.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/30/11 1:46 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1316-T04-A	1	7.88E+05			7.88E+05	8.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/30/11 1:47 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1316-T01-B	1	5.08E+05			5.08E+05	5.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/30/11 1:49 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1316-T02-B	1	6.32E+05			6.32E+05	4.4E-01	2.5E+00	8.0E+00	1000	100	6.32E+05	83%	VU ICP-OES	3/30/11 1:50 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1316-T03-B	1	7.37E+05			7.37E+05	2.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/30/11 1:52 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1316-T04-B	1	7.85E+05			7.85E+05	1.6E+00	2.5E+00	8.0E+00				---	VU ICP-OES	3/30/11 1:54 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1316-T01-C	1	5.07E+05			5.07E+05	3.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/30/11 1:57 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1316-T02-C	1	6.27E+05			6.27E+05	1.6E-01	2.5E+00	8.0E+00	1000	100	6.28E+05	95%	VU ICP-OES	3/30/11 1:59 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1316-T03-C	1	7.31E+05			7.31E+05	1.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/30/11 2:00 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1316-T04-C	1	7.77E+05			7.77E+05	7.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/30/11 2:02 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1316-B01-A	1	6.81E+01			6.81E+01	6.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1316-B01-B	1	7.37E+01			7.37E+01	9.0E+00	2.5E+00	8.0E+00				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
Na	SWA-L06-1316-B01-C	1	7.20E+01			7.20E+01	3.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	SWA-L06-1316-T01-A	1	4.50E+02			4.50E+02	6.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 3:49 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L06-1316-T02-A	1	4.60E+02			4.60E+02	1.5E-01	1.0E+00	3.2E+00	1000	100	1.46E+03	100%	VU ICP-OES	5/23/11 3:51 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L06-1316-T03-A	1	2.49E+02			2.49E+02	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 3:53 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L06-1316-T04-A	1	5.91E+02			5.91E+02	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 3:56 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L06-1316-T01-B	1	4.42E+02			4.42E+02	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 3:58 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L06-1316-T02-B	1	4.48E+02			4.48E+02	8.7E-01	1.0E+00	3.2E+00	1000	100	1.42E+03	97%	VU ICP-OES	5/23/11 4:00 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L06-1316-T03-B	1	2.77E+02			2.77E+02	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:02 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L06-1316-T04-B	1	4.72E+02			4.72E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:05 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L06-1316-T01-C	1	4.40E+02			4.40E+02	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:07 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L06-1316-T02-C	1	4.49E+02			4.49E+02	4.8E-01	1.0E+00	3.2E+00	1000	100	1.45E+03	100%	VU ICP-OES	5/23/11 4:09 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L06-1316-T03-C	1	2.11E+02			2.11E+02	2.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:12 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L06-1316-T04-C	1	5.41E+02			5.41E+02	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:14 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L06-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1316-B01-B	1	5.00E-01	U1/2		5.00E-01	7.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
Sr	SWA-L06-1316-B01-C	1	5.00E-01	U1/2		5.00E-01	6.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	SWA-L06-1316-T01-A	1	8.95E+05			8.95E+05	1.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/30/11 1:42 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1316-T02-A	1	1.20E+06			1.20E+06	5.5E-01	6.8E+00	2.2E+01	1000	100	1.30E+06	92%	VU ICP-OES	3/30/11 1:44 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1316-T03-A	1	1.44E+06			1.44E+06	4.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/30/11 1:46 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1316-T04-A	1	2.06E+06			2.06E+06	2.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/30/11 1:47 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1316-T01-B	1	9.04E+05			9.04E+05	1.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/30/11 1:49 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1316-T02-B	1	1.24E+06			1.24E+06	1.6E+00	6.8E+00	2.2E+01	1000	100	1.32E+06	82%	VU ICP-OES	3/30/11 1:50 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1316-T03-B	1	1.48E+06			1.48E+06	9.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/30/11 1:52 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1316-T04-B	1	2.13E+06			2.13E+06	6.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/30/11 1:54 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1316-T01-C	1	9.07E+05			9.07E+05	1.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/30/11 1:57 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1316-T02-C	1	1.19E+06			1.19E+06	1.3E+00	6.8E+00	2.2E+01	1000	100	1.28E+06	84%	VU ICP-OES	3/30/11 1:59 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1316-T03-C	1	1.46E+06			1.46E+06	6.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/30/11 2:00 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1316-T04-C	1	2.08E+06			2.08E+06	9.2E-02	6.8E+00	2.2E+01				---	VU ICP-OES	3/30/11 2:02 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	4.1E+02	6.8E+00	2.2E+01				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1316-B01-B	1	7.74E+00	E		7.74E+00	1.6E+02	6.8E+00	2.2E+01				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
S	SWA-L06-1316-B01-C	1	3.40E+00	U1/2		3.40E+00	5.2E+02	6.8E+00	2.2E+01				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	SWA-L06-1316-T01-A	1	2.30E+00	U1/2		2.30E+00	3.5E+01	4.6E+00	1.5E+01				---	VU ICP-OES	3/30/11 1:42 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1316-T02-A	1	2.30E+00	U1/2		2.30E+00	2.2E+02	4.6E+00	1.5E+01	10	100	1.01E+03	101%	VU ICP-OES	3/30/11 1:44 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1316-T03-A	1	2.30E+00	U1/2		2.30E+00	1.9E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/30/11 1:46 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1316-T04-A	1	2.30E+00	U1/2		2.30E+00	7.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	3/30/11 1:47 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1316-T01-B	1	2.30E+00	U1/2		2.30E+00	4.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	3/30/11 1:49 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1316-T02-B	1	2.30E+00	U1/2		2.30E+00	9.7E+01	4.6E+00	1.5E+01	10	100	9.71E+02	97%	VU ICP-OES	3/30/11 1:50 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1316-T03-B	1	2.30E+00	U1/2		2.30E+00	6.5E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/30/11 1:52 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1316-T04-B	1	2.30E+00	U1/2		2.30E+00	5.4E+01	4.6E+00	1.5E+01				---	VU ICP-OES	3/30/11 1:54 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1316-T01-C	1	2.30E+00	U1/2		2.30E+00	1.6E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/30/11 1:57 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1316-T02-C	1	2.30E+00	U1/2		2.30E+00	1.3E+02	4.6E+00	1.5E+01	10	100	1.01E+03	100%	VU ICP-OES	3/30/11 1:59 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1316-T03-C	1	2.30E+00	U1/2		2.30E+00	9.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	3/30/11 2:00 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1316-T04-C	1	2.30E+00	U1/2		2.30E+00	2.1E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/30/11 2:02 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1316-B01-A	1	2.30E+00	U1/2		2.30E+00	1.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1316-B01-B	1	2.30E+00	U1/2		2.30E+00	4.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
Tl	SWA-L06-1316-B01-C	1	2.30E+00	U1/2		2.30E+00	2.9E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	SWA-L06-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:42 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	1.3E+01	2.0E+00	6.4E+00	10	100	1.12E+03	112%	VU ICP-OES	3/30/11 1:44 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	8.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:46 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:47 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	3.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:49 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	3.3E+00	2.0E+00	6.4E+00	10	100	1.07E+03	107%	VU ICP-OES	3/30/11 1:50 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:52 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	1.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:54 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:57 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	9.2E+00	2.0E+00	6.4E+00	10	100	1.11E+03	111%	VU ICP-OES	3/30/11 1:59 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 2:00 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	8.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 2:02 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	3.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1316-B01-B	1	1.00E+00	U1/2		1.00E+00	6.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
Ti	SWA-L06-1316-B01-C	1	1.00E+00	U1/2		1.00E+00	6.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	SWA-L06-1316-T01-A	1	3.61E+02			3.61E+02	1.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/30/11 1:42 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1316-T02-A	1	6.43E+02			6.43E+02	5.3E-01	1.5E+00	4.8E+00	10	100	1.75E+03	111%	VU ICP-OES	3/30/11 1:44 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1316-T03-A	1	1.24E+03			1.24E+03	4.6E-01	1.5E+00	4.8E+00				---	VU ICP-OES	3/30/11 1:46 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1316-T04-A	1	2.22E+03			2.22E+03	3.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	3/30/11 1:47 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1316-T01-B	1	3.61E+02			3.61E+02	2.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/30/11 1:49 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1316-T02-B	1	6.48E+02			6.48E+02	8.1E-01	1.5E+00	4.8E+00	10	100	1.73E+03	108%	VU ICP-OES	3/30/11 1:50 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1316-T03-B	1	1.28E+03			1.28E+03	5.1E-01	1.5E+00	4.8E+00				---	VU ICP-OES	3/30/11 1:52 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1316-T04-B	1	2.32E+03			2.32E+03	8.4E-01	1.5E+00	4.8E+00				---	VU ICP-OES	3/30/11 1:54 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1316-T01-C	1	3.60E+02			3.60E+02	7.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	3/30/11 1:57 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1316-T02-C	1	6.38E+02			6.38E+02	1.3E+00	1.5E+00	4.8E+00	10	100	1.79E+03	115%	VU ICP-OES	3/30/11 1:59 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1316-T03-C	1	1.25E+03			1.25E+03	6.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	3/30/11 2:00 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1316-T04-C	1	2.26E+03			2.26E+03	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/30/11 2:02 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1316-B01-A	1	7.50E-01	U1/2		7.50E-01	5.5E+01	1.5E+00	4.8E+00				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1316-B01-B	1	7.50E-01	U1/2		7.50E-01	6.5E+01	1.5E+00	4.8E+00				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
V	SWA-L06-1316-B01-C	1	7.50E-01	U1/2		7.50E-01	4.5E+01	1.5E+00	4.8E+00				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	SWA-L06-1316-T01-A	1	3.24E+00			3.24E+00	9.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:42 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1316-T02-A	1	4.84E+00			4.84E+00	6.8E+00	1.0E+00	3.2E+00	10	100	1.12E+03	111%	VU ICP-OES	3/30/11 1:44 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1316-T03-A	1	1.23E+00	E		1.23E+00	2.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:46 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1316-T04-A	1	1.14E+01			1.14E+01	4.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:47 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1316-T01-B	1	3.59E+00			3.59E+00	3.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:49 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1316-T02-B	1	3.73E+00			3.73E+00	8.7E+00	1.0E+00	3.2E+00	10	100	1.07E+03	107%	VU ICP-OES	3/30/11 1:50 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1316-T03-B	1	1.02E+00	E		1.02E+00	2.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:52 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1316-T04-B	1	1.24E+01			1.24E+01	5.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:54 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1316-T01-C	1	3.44E+00			3.44E+00	2.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:57 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1316-T02-C	1	4.79E+00			4.79E+00	3.4E+00	1.0E+00	3.2E+00	10	100	1.11E+03	111%	VU ICP-OES	3/30/11 1:59 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1316-T03-C	1	1.14E+00	E		1.14E+00	1.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 2:00 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1316-T04-C	1	1.13E+01			1.13E+01	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 2:02 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1316-B01-A	1	2.49E+00	E		2.49E+00	2.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:37 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1316-B01-B	1	2.81E+00	E		2.81E+00	5.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:39 PM	EPA Interlab L06 1313-1316 SWA
Zn	SWA-L06-1316-B01-C	1	2.53E+00	E		2.53E+00	5.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/30/11 1:41 PM	EPA Interlab L06 1313-1316 SWA

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	SWA-L07-1316-T01-A	1	3.80E+04			3.80E+04	6.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1316-T02-A	1	5.95E+04			5.95E+04	6.1E-01	1.0E+00	3.2E+00	1000	120	6.06E+04	91%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1316-T03-A	1	8.55E+04			8.55E+04	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1316-T04-A	1	1.72E+05			1.72E+05	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1316-T01-B	1	3.74E+04			3.74E+04	5.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1316-T02-B	1	5.93E+04			5.93E+04	9.0E-01	1.0E+00	3.2E+00	1000	120	6.05E+04	97%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1316-T03-B	1	9.09E+04			9.09E+04	2.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1316-T04-B	1	1.81E+05			1.81E+05	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1316-T01-C	1	3.69E+04			3.69E+04	3.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1316-T02-C	1	5.65E+04			5.65E+04	2.8E-01	1.0E+00	3.2E+00	1000	120	5.76E+04	96%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1316-T03-C	1	9.64E+04			9.64E+04	8.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1316-T04-C	1	1.80E+05			1.80E+05	8.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
Al	SWA-L07-1316-B01-A	1	6.28E+00			6.28E+00		1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	SWA-L07-1316-T01-A	1	2.99E+03			2.99E+03	2.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1316-T02-A	1	1.54E+03			1.54E+03	3.0E+00	7.5E+00	2.4E+01	10	120	2.54E+03	84%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1316-T03-A	1	7.61E+03			7.61E+03	6.6E-01	7.5E+00	2.4E+01				---	VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1316-T04-A	1	5.47E+03			5.47E+03	1.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1316-T01-B	1	2.76E+03			2.76E+03	1.7E-01	7.5E+00	2.4E+01				---	VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1316-T02-B	1	1.46E+03			1.46E+03	2.0E+00	7.5E+00	2.4E+01	10	120	2.66E+03	100%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1316-T03-B	1	8.18E+03			8.18E+03	1.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1316-T04-B	1	5.20E+03			5.20E+03	5.1E-01	7.5E+00	2.4E+01				---	VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1316-T01-C	1	2.54E+03			2.54E+03	4.8E-01	7.5E+00	2.4E+01				---	VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1316-T02-C	1	1.86E+03			1.86E+03	2.1E+00	7.5E+00	2.4E+01	10	120	3.12E+03	105%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1316-T03-C	1	7.19E+03			7.19E+03	6.7E-01	7.5E+00	2.4E+01				---	VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1316-T04-C	1	5.57E+03			5.57E+03	3.1E-01	7.5E+00	2.4E+01				---	VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
Sb	SWA-L07-1316-B01-A	1	3.75E+00	U1/2		3.75E+00		7.5E+00	2.4E+01				---	VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	SWA-L07-1316-T01-A	1	4.42E+03			4.42E+03	3.9E-01	1.1E+01	3.5E+01				---	VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1316-T02-A	1	1.12E+04			1.12E+04	1.2E+00	1.1E+01	3.5E+01	10	120	1.22E+04	84%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1316-T03-A	1	4.13E+04			4.13E+04	9.8E-01	1.1E+01	3.5E+01				---	VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1316-T04-A	1	1.11E+05			1.11E+05	5.7E-01	1.1E+01	3.5E+01				---	VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1316-T01-B	1	4.50E+03			4.50E+03	2.5E-01	1.1E+01	3.5E+01				---	VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1316-T02-B	1	1.19E+04			1.19E+04	1.1E+00	1.1E+01	3.5E+01	10	120	1.32E+04	102%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1316-T03-B	1	4.07E+04			4.07E+04	4.1E-01	1.1E+01	3.5E+01				---	VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1316-T04-B	1	9.77E+04			9.77E+04	6.4E-01	1.1E+01	3.5E+01				---	VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1316-T01-C	1	4.22E+03			4.22E+03	1.2E-01	1.1E+01	3.5E+01				---	VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1316-T02-C	1	9.59E+03			9.59E+03	6.6E-01	1.1E+01	3.5E+01	10	120	1.07E+04	92%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1316-T03-C	1	3.67E+04			3.67E+04	8.5E-01	1.1E+01	3.5E+01				---	VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1316-T04-C	1	9.95E+04			9.95E+04	6.4E-01	1.1E+01	3.5E+01				---	VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
As	SWA-L07-1316-B01-A	1	5.50E+00	U1/2		5.50E+00		1.1E+01	3.5E+01				---	VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	SWA-L07-1316-T01-A	1	1.06E+03			1.06E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1316-T02-A	1	1.26E+03			1.26E+03	5.6E-01	1.0E+00	3.2E+00	1000	120	2.35E+03	91%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1316-T03-A	1	1.16E+03			1.16E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1316-T04-A	1	1.03E+03			1.03E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1316-T01-B	1	1.16E+03			1.16E+03	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1316-T02-B	1	1.58E+03			1.58E+03	5.6E-01	1.0E+00	3.2E+00	1000	120	2.74E+03	96%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1316-T03-B	1	1.21E+03			1.21E+03	4.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1316-T04-B	1	1.04E+03			1.04E+03	2.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1316-T01-C	1	1.08E+03			1.08E+03	1.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1316-T02-C	1	1.51E+03			1.51E+03	7.0E-01	1.0E+00	3.2E+00	1000	120	2.72E+03	101%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1316-T03-C	1	1.18E+03			1.18E+03	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1316-T04-C	1	1.09E+03			1.09E+03	1.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
B	SWA-L07-1316-B01-A	1	5.43E+00			5.43E+00		1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	SWA-L07-1316-T01-A	1	1.83E+02			1.83E+02	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1316-T02-A	1	1.72E+02			1.72E+02	3.0E-01	1.0E+00	3.2E+00	10	120	1.20E+03	85%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1316-T03-A	1	3.16E+01			3.16E+01	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1316-T04-A	1	1.21E+02			1.21E+02	7.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1316-T01-B	1	2.03E+02			2.03E+02	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1316-T02-B	1	1.81E+02			1.81E+02	2.3E-01	1.0E+00	3.2E+00	10	120	1.28E+03	91%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1316-T03-B	1	3.66E+01			3.66E+01	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1316-T04-B	1	1.12E+02			1.12E+02	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1316-T01-C	1	2.14E+02			2.14E+02	1.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1316-T02-C	1	2.00E+02			2.00E+02	3.6E-01	1.0E+00	3.2E+00	10	120	1.33E+03	94%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1316-T03-C	1	3.38E+01			3.38E+01	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1316-T04-C	1	1.36E+02			1.36E+02	2.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
Ba	SWA-L07-1316-B01-A	1	5.00E-01	U1/2		5.00E-01		1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	SWA-L07-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	2.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	5.1E+01	1.9E+00	6.0E+00	10	120	1.11E+03	92%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	9.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	1.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	5.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	7.1E+02	1.9E+00	6.0E+00	10	120	1.19E+03	99%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	4.6E+02	1.9E+00	6.0E+00				---	VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	2.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	4.3E+01	1.9E+00	6.0E+00	10	120	1.23E+03	102%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	1.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
Be	SWA-L07-1316-B01-A	1	9.50E-01	U1/2		9.50E-01		1.9E+00	6.0E+00				---	VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	SWA-L07-1316-T01-A	1	1.10E+00	U1/2		1.10E+00	1.1E+02	2.2E+00	7.0E+00				---	VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1316-T02-A	1	1.10E+00	U1/2		1.10E+00	1.4E+03	2.2E+00	7.0E+00	10	120	9.90E+02	82%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1316-T03-A	1	1.10E+00	U1/2		1.10E+00	2.4E+02	2.2E+00	7.0E+00				---	VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1316-T04-A	1	1.10E+00	U1/2		1.10E+00	1.7E+02	2.2E+00	7.0E+00				---	VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1316-T01-B	1	1.10E+00	U1/2		1.10E+00	1.7E+02	2.2E+00	7.0E+00				---	VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1316-T02-B	1	1.10E+00	U1/2		1.10E+00	7.1E+01	2.2E+00	7.0E+00	10	120	1.06E+03	88%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1316-T03-B	1	1.10E+00	U1/2		1.10E+00	2.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1316-T04-B	1	1.10E+00	U1/2		1.10E+00	1.9E+02	2.2E+00	7.0E+00				---	VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1316-T01-C	1	1.10E+00	U1/2		1.10E+00	4.3E+02	2.2E+00	7.0E+00				---	VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1316-T02-C	1	1.10E+00	U1/2		1.10E+00	6.0E+01	2.2E+00	7.0E+00	10	120	1.10E+03	91%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1316-T03-C	1	1.10E+00	U1/2		1.10E+00	1.2E+02	2.2E+00	7.0E+00				---	VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1316-T04-C	1	1.10E+00	U1/2		1.10E+00	4.2E+02	2.2E+00	7.0E+00				---	VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
Cd	SWA-L07-1316-B01-A	1	1.10E+00	U1/2		1.10E+00		2.2E+00	7.0E+00				---	VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	SWA-L07-1316-T01-A	1	1.47E+04			1.47E+04	6.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1316-T02-A	1	1.16E+04			1.16E+04	5.0E-01	2.6E+00	8.3E+00	1000	120	1.27E+04	85%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1316-T03-A	1	3.46E+03			3.46E+03	3.8E+00	2.6E+00	8.3E+00				---	VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1316-T04-A	1	3.93E+03			3.93E+03	5.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1316-T01-B	1	1.42E+04			1.42E+04	1.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1316-T02-B	1	1.12E+04			1.12E+04	1.3E-01	2.6E+00	8.3E+00	1000	120	1.24E+04	93%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1316-T03-B	1	3.23E+03			3.23E+03	1.6E+00	2.6E+00	8.3E+00				---	VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1316-T04-B	1	4.51E+03			4.51E+03	2.8E+00	2.6E+00	8.3E+00				---	VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1316-T01-C	1	1.47E+04			1.47E+04	3.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1316-T02-C	1	1.18E+04			1.18E+04	1.4E-01	2.6E+00	8.3E+00	1000	120	1.29E+04	92%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1316-T03-C	1	3.47E+03			3.47E+03	4.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1316-T04-C	1	5.05E+03			5.05E+03	8.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
Ca	SWA-L07-1316-B01-A	1	3.89E+01			3.89E+01		2.6E+00	8.3E+00				---	VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	SWA-L07-1316-T01-A	1	1.11E+03			1.11E+03	1.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1316-T02-A	1	1.68E+03			1.68E+03	8.5E-01	1.2E+00	3.8E+00	10	120	2.89E+03	101%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1316-T03-A	1	1.36E+03			1.36E+03	5.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1316-T04-A	1	2.59E+03			2.59E+03	9.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1316-T01-B	1	1.16E+03			1.16E+03	2.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1316-T02-B	1	1.77E+03			1.77E+03	6.0E-01	1.2E+00	3.8E+00	10	120	2.95E+03	99%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1316-T03-B	1	1.33E+03			1.33E+03	5.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1316-T04-B	1	2.63E+03			2.63E+03	2.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1316-T01-C	1	1.06E+03			1.06E+03	2.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1316-T02-C	1	1.68E+03			1.68E+03	2.1E-01	1.2E+00	3.8E+00	10	120	2.91E+03	103%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1316-T03-C	1	1.47E+03			1.47E+03	9.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1316-T04-C	1	2.58E+03			2.58E+03	1.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
Cr	SWA-L07-1316-B01-A	1	6.00E-01	U1/2		6.00E-01		1.2E+00	3.8E+00				---	VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	SWA-L07-1316-T01-A	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.8E+00	5.7E+00			---		VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1316-T02-A	1	9.00E-01	U1/2		9.00E-01	4.8E+01	1.8E+00	5.7E+00	10	120	1.00E+03	83%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1316-T03-A	1	3.21E+00	E		3.21E+00	1.2E+01	1.8E+00	5.7E+00			---		VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1316-T04-A	1	6.56E+00			6.56E+00	1.2E+01	1.8E+00	5.7E+00			---		VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1316-T01-B	1	9.00E-01	U1/2		9.00E-01	5.8E+02	1.8E+00	5.7E+00			---		VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1316-T02-B	1	9.00E-01	U1/2		9.00E-01	1.9E+02	1.8E+00	5.7E+00	10	120	1.07E+03	89%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1316-T03-B	1	3.60E+00	E		3.60E+00	1.1E+01	1.8E+00	5.7E+00			---		VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1316-T04-B	1	7.33E+00			7.33E+00	4.6E+00	1.8E+00	5.7E+00			---		VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1316-T01-C											---		VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1316-T02-C	1	9.00E-01	U1/2		9.00E-01	3.8E+02	1.8E+00	5.7E+00	10	120	1.11E+03	93%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1316-T03-C	1	3.05E+00	E		3.05E+00	4.6E+01	1.8E+00	5.7E+00			---		VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1316-T04-C	1	7.35E+00			7.35E+00	9.9E+00	1.8E+00	5.7E+00			---		VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
Co	SWA-L07-1316-B01-A	1	9.00E-01	U1/2		9.00E-01		1.8E+00	5.7E+00			---		VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	SWA-L07-1316-T01-A	1	1.85E+00	U1/2		1.85E+00	3.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1316-T02-A	1	3.85E+00	E		3.85E+00	5.2E+01	3.7E+00	1.2E+01	10	120	9.90E+02	82%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1316-T03-A	1	8.91E+00	E		8.91E+00	2.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1316-T04-A	1	4.41E+01			4.41E+01	6.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1316-T01-B	1	1.85E+00	U1/2		1.85E+00	5.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1316-T02-B	1	4.61E+00	E		4.61E+00	4.0E+01	3.7E+00	1.2E+01	10	120	1.05E+03	87%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1316-T03-B	1	9.70E+00	E		9.70E+00	1.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1316-T04-B	1	4.03E+01			4.03E+01	8.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1316-T01-C	1	1.85E+00	U1/2		1.85E+00	1.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1316-T02-C	1	4.90E+00	E		4.90E+00	2.0E+01	3.7E+00	1.2E+01	10	120	1.11E+03	92%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1316-T03-C	1	1.22E+01			1.22E+01	2.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1316-T04-C	1	4.25E+01			4.25E+01	2.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
Cu	SWA-L07-1316-B01-A	1	1.85E+00	U1/2		1.85E+00		3.7E+00	1.2E+01				---	VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	SWA-L07-1316-T01-A	1	9.74E+01			9.74E+01	6.7E-02	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1316-T02-A	1	1.91E+02			1.91E+02	3.6E-01	2.0E+00	6.4E+00	1000	120	1.23E+03	87%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1316-T03-A	1	3.26E+02			3.26E+02	3.2E-01	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1316-T04-A	1	1.20E+03			1.20E+03	7.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1316-T01-B	1	8.07E+01			8.07E+01	6.6E-01	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1316-T02-B	1	1.84E+02			1.84E+02	5.2E-01	2.0E+00	6.4E+00	1000	120	1.30E+03	93%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1316-T03-B	1	3.85E+02			3.85E+02	6.0E-01	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1316-T04-B	1	1.33E+03			1.33E+03	5.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1316-T01-C	1	7.70E+01			7.70E+01	6.9E-01	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1316-T02-C	1	1.58E+02			1.58E+02	6.3E-01	2.0E+00	6.4E+00	1000	120	1.32E+03	97%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1316-T03-C	1	3.67E+02			3.67E+02	1.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1316-T04-C	1	1.42E+03			1.42E+03	9.2E-01	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
Fe	SWA-L07-1316-B01-A	1	1.00E+00	U1/2		1.00E+00		2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	SWA-L07-1316-T01-A	1	1.32E+01	E		1.32E+01	2.7E+01	6.8E+00	2.2E+01				---	VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1316-T02-A	1	2.79E+01			2.79E+01	1.9E+01	6.8E+00	2.2E+01	10	120	1.04E+03	84%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1316-T03-A	1	1.36E+01	E		1.36E+01	2.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1316-T04-A	1	1.52E+02			1.52E+02	3.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1316-T01-B	1	1.19E+01	E		1.19E+01	1.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1316-T02-B	1	3.50E+01			3.50E+01	6.7E+00	6.8E+00	2.2E+01	10	120	1.12E+03	91%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1316-T03-B	1	1.47E+01	E		1.47E+01	2.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1316-T04-B	1	1.79E+02			1.79E+02	1.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1316-T01-C	1	1.59E+01	E		1.59E+01	2.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1316-T02-C	1	3.94E+01			3.94E+01	2.3E+01	6.8E+00	2.2E+01	10	120	1.16E+03	93%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1316-T03-C	1	1.98E+01	E		1.98E+01	2.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1316-T04-C	1	1.72E+02			1.72E+02	3.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
Pb	SWA-L07-1316-B01-A	1	3.40E+00	U1/2		3.40E+00		6.8E+00	2.2E+01				---	VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	SWA-L07-1316-T01-A	1	2.63E+00	E		2.63E+00	2.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1316-T02-A	1	5.43E+00	E		5.43E+00	4.8E+01	1.9E+00	6.0E+00	10	120	9.88E+02	82%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1316-T03-A	1	6.10E+00			6.10E+00	1.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1316-T04-A	1	8.99E+00			8.99E+00	2.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1316-T01-B	1	2.38E+00	E		2.38E+00	1.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1316-T02-B	1	5.69E+00	E		5.69E+00	2.4E+01	1.9E+00	6.0E+00	10	120	9.98E+02	83%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1316-T03-B	1	6.80E+00			6.80E+00	3.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1316-T04-B	1	1.04E+01			1.04E+01	5.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1316-T01-C	1	2.39E+00	E		2.39E+00	4.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1316-T02-C	1	5.18E+00	E		5.18E+00	3.6E+00	1.9E+00	6.0E+00	10	120	9.94E+02	82%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1316-T03-C	1	5.93E+00	E		5.93E+00	3.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1316-T04-C	1	9.32E+00			9.32E+00	2.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
Li	SWA-L07-1316-B01-A	1	9.50E-01	U1/2		9.50E-01		1.9E+00	6.0E+00				---	VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	SWA-L07-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	4.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	1.0E+01	2.0E+00	6.4E+00	10	120	1.00E+03	84%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	7.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1316-T04-A	1	3.54E+00	E		3.54E+00	2.6E+00	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	3.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00	10	120	1.08E+03	90%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	6.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1316-T04-B	1	3.78E+00	E		3.78E+00	5.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	7.9E-01	2.0E+00	6.4E+00	10	120	1.12E+03	93%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	3.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1316-T04-C	1	4.37E+00	E		4.37E+00	9.3E-01	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
Mn	SWA-L07-1316-B01-A	1	1.00E+00	U1/2		1.00E+00		2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	SWA-L07-1316-T01-A	1	5.00E-01	U1/2		5.00E-01	4.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1316-T02-A	1	6.49E+00			6.49E+00	4.1E+02	1.0E+00	3.2E+00	1000	120	1.00E+03	83%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1316-T03-A	1	9.71E+00			9.71E+00	4.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1316-T04-A	1	1.06E+01			1.06E+01	9.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1316-T01-B	1	5.00E-01	U1/2		5.00E-01	3.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1316-T02-B	1	7.17E+00			7.17E+00	2.7E+01	1.0E+00	3.2E+00	1000	120	1.09E+03	90%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1316-T03-B	1	1.02E+01			1.02E+01	4.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1316-T04-B	1	1.19E+01			1.19E+01	5.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1316-T01-C	1	5.00E-01	U1/2		5.00E-01	1.4E+03	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1316-T02-C	1	7.33E+00			7.33E+00	7.6E+01	1.0E+00	3.2E+00	1000	120	1.13E+03	93%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1316-T03-C	1	8.43E+00			8.43E+00	9.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1316-T04-C	1	9.33E+00			9.33E+00	3.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
Mg	SWA-L07-1316-B01-A	1	3.37E+00			3.37E+00		1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	SWA-L07-1316-T01-A	1	9.52E+01			9.52E+01	1.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1316-T02-A	1	1.45E+02			1.45E+02	4.9E-01	1.2E+00	3.8E+00	10	120	1.25E+03	92%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1316-T03-A	1	6.67E+02			6.67E+02	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1316-T04-A	1	1.34E+03			1.34E+03	7.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1316-T01-B	1	8.75E+01			8.75E+01	3.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1316-T02-B	1	1.22E+02			1.22E+02	2.6E-01	1.2E+00	3.8E+00	10	120	1.30E+03	99%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1316-T03-B	1	6.31E+02			6.31E+02	7.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1316-T04-B	1	1.33E+03			1.33E+03	5.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1316-T01-C	1	8.04E+01			8.04E+01	2.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1316-T02-C	1	1.29E+02			1.29E+02	1.6E+00	1.2E+00	3.8E+00	10	120	1.31E+03	99%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1316-T03-C	1	5.94E+02			5.94E+02	3.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1316-T04-C	1	1.35E+03			1.35E+03	8.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
Mo	SWA-L07-1316-B01-A	1	1.23E+00	E		1.23E+00		1.2E+00	3.8E+00				---	VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	SWA-L07-1316-T01-A	1	9.00E-01	U1/2		9.00E-01	3.4E+02	1.8E+00	5.7E+00			---		VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1316-T02-A	1	9.00E-01	U1/2		9.00E-01	3.8E+01	1.8E+00	5.7E+00	10	120	9.98E+02	83%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1316-T03-A	1	9.00E-01	U1/2		9.00E-01	9.9E+01	1.8E+00	5.7E+00			---		VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1316-T04-A	1	4.31E+00	E		4.31E+00	4.0E+01	1.8E+00	5.7E+00			---		VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1316-T01-B	1	9.00E-01	U1/2		9.00E-01	6.6E+01	1.8E+00	5.7E+00			---		VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1316-T02-B	1	9.00E-01	U1/2		9.00E-01	2.8E+01	1.8E+00	5.7E+00	10	120	1.07E+03	89%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1316-T03-B	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00			---		VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1316-T04-B	1	4.32E+00	E		4.32E+00	1.4E+01	1.8E+00	5.7E+00			---		VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1316-T01-C	1	9.00E-01	U1/2		9.00E-01	1.0E+02	1.8E+00	5.7E+00			---		VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1316-T02-C	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00	10	120	1.11E+03	93%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1316-T03-C	1	9.00E-01	U1/2		9.00E-01	4.8E+01	1.8E+00	5.7E+00			---		VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1316-T04-C	1	4.61E+00	E		4.61E+00	4.0E+01	1.8E+00	5.7E+00			---		VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
Ni	SWA-L07-1316-B01-A	1	9.00E-01	U1/2		9.00E-01		1.8E+00	5.7E+00			---		VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	SWA-L07-1316-T01-A	1	7.09E+01			7.09E+01	1.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1316-T02-A	1	1.14E+02			1.14E+02	1.8E+01	3.7E+00	1.2E+01	1000	120	1.20E+03	90%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1316-T03-A	1	3.92E+02			3.92E+02	3.9E+00	3.7E+00	1.2E+01			---		VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1316-T04-A	1	1.37E+03			1.37E+03	2.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1316-T01-B	1	5.77E+01			5.77E+01	7.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1316-T02-B	1	1.25E+02			1.25E+02	1.3E+01	3.7E+00	1.2E+01	1000	120	1.28E+03	96%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1316-T03-B	1	3.78E+02			3.78E+02	2.3E+00	3.7E+00	1.2E+01			---		VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1316-T04-B	1	1.23E+03			1.23E+03	2.8E+00	3.7E+00	1.2E+01			---		VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1316-T01-C	1	5.83E+01			5.83E+01	9.2E+00	3.7E+00	1.2E+01			---		VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1316-T02-C	1	9.65E+01			9.65E+01	1.5E+01	3.7E+00	1.2E+01	1000	120	1.29E+03	100%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1316-T03-C	1	3.62E+02			3.62E+02	6.8E-01	3.7E+00	1.2E+01			---		VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1316-T04-C	1	1.25E+03			1.25E+03	1.6E+00	3.7E+00	1.2E+01			---		VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
P	SWA-L07-1316-B01-A	1	6.62E+00	E		6.62E+00		3.7E+00	1.2E+01			---		VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	SWA-L07-1316-T01-A	1	3.04E+05			3.04E+05	1.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1316-T02-A	1	4.94E+05			4.94E+05	7.9E-01	1.6E+00	5.1E+00	1000	120	4.95E+05	87%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1316-T03-A	1	2.23E+06			2.23E+06	6.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1316-T04-A	1	2.34E+06			2.34E+06	7.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1316-T01-B	1	3.04E+05			3.04E+05	6.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1316-T02-B	1	5.10E+05			5.10E+05	2.6E+00	1.6E+00	5.1E+00	1000	120	5.11E+05	87%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1316-T03-B	1	2.21E+06			2.21E+06	8.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1316-T04-B	1	2.31E+06			2.31E+06	7.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1316-T01-C	1	3.02E+05			3.02E+05	3.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1316-T02-C	1	4.78E+05			4.78E+05	1.7E+00	1.6E+00	5.1E+00	1000	120	4.79E+05	94%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1316-T03-C	1	2.19E+06			2.19E+06	1.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1316-T04-C	1	2.36E+06			2.36E+06	4.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
K	SWA-L07-1316-B01-A	1	5.98E+01			5.98E+01		1.6E+00	5.1E+00				---	VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	SWA-L07-1316-T01-A	1	9.42E+04			9.42E+04	7.1E-01	1.5E+01	4.8E+01			---		VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1316-T02-A	1	1.78E+05			1.78E+05	2.6E-01	1.5E+01	4.8E+01	10	120	1.79E+05	87%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1316-T03-A	1	4.49E+05			4.49E+05	4.5E-01	1.5E+01	4.8E+01			---		VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1316-T04-A	1	8.69E+05			8.69E+05	1.1E+00	1.5E+01	4.8E+01			---		VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1316-T01-B	1	9.49E+04			9.49E+04	4.9E-01	1.5E+01	4.8E+01			---		VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1316-T02-B	1	1.82E+05			1.82E+05	4.5E-01	1.5E+01	4.8E+01	10	120	1.83E+05	98%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1316-T03-B	1	4.33E+05			4.33E+05	3.1E-01	1.5E+01	4.8E+01			---		VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1316-T04-B	1	8.49E+05			8.49E+05	9.3E-02	1.5E+01	4.8E+01			---		VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1316-T01-C	1	9.08E+04			9.08E+04	2.0E-01	1.5E+01	4.8E+01			---		VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1316-T02-C	1	1.60E+05			1.60E+05	3.5E-01	1.5E+01	4.8E+01	10	120	1.61E+05	92%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1316-T03-C	1	4.05E+05			4.05E+05	8.2E-01	1.5E+01	4.8E+01			---		VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1316-T04-C	1	8.59E+05			8.59E+05	3.4E-01	1.5E+01	4.8E+01			---		VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
Se	SWA-L07-1316-B01-A	1	7.50E+00	U1/2		7.50E+00		1.5E+01	4.8E+01			---		VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	SWA-L07-1316-T01-A	1	2.38E+04			2.38E+04	3.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1316-T02-A	1	3.10E+04			3.10E+04	6.2E-01	1.1E+00	3.5E+00	1000	120	3.20E+04	83%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1316-T03-A	1	2.59E+04			2.59E+04	2.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1316-T04-A	1	5.52E+04			5.52E+04	4.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1316-T01-B	1	2.48E+04			2.48E+04	2.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1316-T02-B	1	3.30E+04			3.30E+04	2.7E-01	1.1E+00	3.5E+00	1000	120	3.40E+04	82%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1316-T03-B	1	2.52E+04			2.52E+04	2.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1316-T04-B	1	4.89E+04			4.89E+04	4.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1316-T01-C	1	2.39E+04			2.39E+04	6.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1316-T02-C	1	2.94E+04			2.94E+04	4.8E-01	1.1E+00	3.5E+00	1000	120	3.04E+04	85%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1316-T03-C	1	3.03E+04			3.03E+04	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1316-T04-C	1	4.97E+04			4.97E+04	4.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
Si	SWA-L07-1316-B01-A	1	5.50E-01	U1/2		5.50E-01		1.1E+00	3.5E+00				---	VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	SWA-L07-1316-T01-A	1	4.15E+05			4.15E+05	6.2E-01	2.5E+00	8.0E+00			---		VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1316-T02-A	1	5.40E+05			5.40E+05	4.3E-01	2.5E+00	8.0E+00	1000	120	5.41E+05	87%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1316-T03-A	1	6.26E+05			6.26E+05	6.9E-01	2.5E+00	8.0E+00			---		VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1316-T04-A	1	6.86E+05			6.86E+05	4.5E-01	2.5E+00	8.0E+00			---		VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1316-T01-B	1	4.14E+05			4.14E+05	4.8E-01	2.5E+00	8.0E+00			---		VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1316-T02-B	1	5.43E+05			5.43E+05	2.1E-01	2.5E+00	8.0E+00	1000	120	5.44E+05	84%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1316-T03-B	1	6.22E+05			6.22E+05	8.2E-01	2.5E+00	8.0E+00			---		VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1316-T04-B	1	6.77E+05			6.77E+05	7.1E-01	2.5E+00	8.0E+00			---		VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1316-T01-C	1	4.16E+05			4.16E+05	1.6E-01	2.5E+00	8.0E+00			---		VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1316-T02-C	1	5.29E+05			5.29E+05	1.2E-01	2.5E+00	8.0E+00	1000	120	5.30E+05	83%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1316-T03-C	1	6.18E+05			6.18E+05	9.1E-01	2.5E+00	8.0E+00			---		VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1316-T04-C	1	6.88E+05			6.88E+05	3.7E-01	2.5E+00	8.0E+00			---		VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
Na	SWA-L07-1316-B01-A	1	5.33E+01			5.33E+01		2.5E+00	8.0E+00			---		VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	SWA-L07-1316-T01-A	1	3.73E+02			3.73E+02	1.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1316-T02-A	1	3.77E+02			3.77E+02	4.8E-01	1.0E+00	3.2E+00	1000	120	1.40E+03	85%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1316-T03-A	1	1.63E+02			1.63E+02	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1316-T04-A	1	4.59E+02			4.59E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1316-T01-B	1	3.78E+02			3.78E+02	6.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1316-T02-B	1	3.75E+02			3.75E+02	6.2E-01	1.0E+00	3.2E+00	1000	120	1.47E+03	91%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1316-T03-B	1	1.78E+02			1.78E+02	8.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1316-T04-B	1	4.84E+02			4.84E+02	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1316-T01-C	1	3.82E+02			3.82E+02	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1316-T02-C	1	3.91E+02			3.91E+02	1.0E+00	1.0E+00	3.2E+00	1000	120	1.52E+03	94%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1316-T03-C	1	1.55E+02			1.55E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1316-T04-C	1	4.97E+02			4.97E+02	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
Sr	SWA-L07-1316-B01-A	1	5.00E-01	U1/2		5.00E-01		1.0E+00	3.2E+00				---	VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	SWA-L07-1316-T01-A	1	1.02E+06			1.02E+06	1.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1316-T02-A	1	1.45E+06			1.45E+06	5.8E-01	6.8E+00	2.2E+01	1000	120	1.45E+06	86%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1316-T03-A	1	1.76E+06			1.76E+06	5.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1316-T04-A	1	2.36E+06			2.36E+06	1.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1316-T01-B	1	1.10E+06			1.10E+06	8.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1316-T02-B	1	1.59E+06			1.59E+06	1.1E+00	6.8E+00	2.2E+01	1000	120	1.59E+06	85%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1316-T03-B	1	1.68E+06			1.68E+06	4.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1316-T04-B	1	2.29E+06			2.29E+06	4.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1316-T01-C	1	1.08E+06			1.08E+06	3.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1316-T02-C	1	1.54E+06			1.54E+06	1.0E+00	6.8E+00	2.2E+01	1000	120	1.54E+06	88%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1316-T03-C	1	1.62E+06			1.62E+06	6.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1316-T04-C	1	2.33E+06			2.33E+06	1.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
S	SWA-L07-1316-B01-A	1	9.49E+01			9.49E+01		6.8E+00	2.2E+01				---	VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	SWA-L07-1316-T01-A	1	2.30E+00	U1/2		2.30E+00	7.4E+01	4.6E+00	1.5E+01			---		VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1316-T02-A	1	2.30E+00	U1/2		2.30E+00	5.8E+01	4.6E+00	1.5E+01	10	120	1.11E+03	92%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1316-T03-A	1	2.30E+00	U1/2		2.30E+00	3.4E+01	4.6E+00	1.5E+01			---		VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1316-T04-A	1	2.30E+00	U1/2		2.30E+00	1.6E+02	4.6E+00	1.5E+01			---		VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1316-T01-B	1	2.30E+00	U1/2		2.30E+00	2.9E+01	4.6E+00	1.5E+01			---		VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1316-T02-B	1	2.30E+00	U1/2		2.30E+00	3.3E+01	4.6E+00	1.5E+01	10	120	1.17E+03	97%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1316-T03-B	1	2.30E+00	U1/2		2.30E+00	6.6E+01	4.6E+00	1.5E+01			---		VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1316-T04-B	1	2.30E+00	U1/2		2.30E+00	8.9E+01	4.6E+00	1.5E+01			---		VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1316-T01-C	1	2.30E+00	U1/2		2.30E+00	1.3E+02	4.6E+00	1.5E+01			---		VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1316-T02-C	1	2.30E+00	U1/2		2.30E+00	3.5E+01	4.6E+00	1.5E+01	10	120	1.19E+03	99%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1316-T03-C	1	2.30E+00	U1/2		2.30E+00	6.8E+01	4.6E+00	1.5E+01			---		VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1316-T04-C	1	2.30E+00	U1/2		2.30E+00	6.8E+02	4.6E+00	1.5E+01			---		VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
Tl	SWA-L07-1316-B01-A	1	2.30E+00	U1/2		2.30E+00		4.6E+00	1.5E+01			---		VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	SWA-L07-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00	10	120	1.15E+03	96%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	7.7E+01	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1316-T04-A	1	3.03E+00	E		3.03E+00	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	3.6E+01	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	4.7E+01	2.0E+00	6.4E+00	10	120	1.25E+03	104%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1316-T04-B	1	3.41E+00	E		3.41E+00	8.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	4.0E+01	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	3.6E+01	2.0E+00	6.4E+00	10	120	1.29E+03	108%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	2.8E+01	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1316-T04-C	1	3.72E+00	E		3.72E+00	1.4E+01	2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
Ti	SWA-L07-1316-B01-A	1	1.00E+00	U1/2		1.00E+00		2.0E+00	6.4E+00			---		VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	SWA-L07-1316-T01-A	1	3.63E+02			3.63E+02	9.3E-02	1.5E+00	4.8E+00			---		VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1316-T02-A	1	6.48E+02			6.48E+02	1.1E+00	1.5E+00	4.8E+00	10	120	1.64E+03	83%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1316-T03-A	1	1.32E+03			1.32E+03	7.0E-01	1.5E+00	4.8E+00			---		VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1316-T04-A	1	2.35E+03			2.35E+03	1.4E+00	1.5E+00	4.8E+00			---		VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1316-T01-B	1	3.59E+02			3.59E+02	5.2E-01	1.5E+00	4.8E+00			---		VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1316-T02-B	1	6.61E+02			6.61E+02	1.1E+00	1.5E+00	4.8E+00	10	120	1.72E+03	88%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1316-T03-B	1	1.24E+03			1.24E+03	2.1E-01	1.5E+00	4.8E+00			---		VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1316-T04-B	1	2.00E+03			2.00E+03	5.8E-01	1.5E+00	4.8E+00			---		VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1316-T01-C	1	3.42E+02			3.42E+02	2.6E-01	1.5E+00	4.8E+00			---		VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1316-T02-C	1	5.62E+02			5.62E+02	1.6E-01	1.5E+00	4.8E+00	10	120	1.66E+03	92%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1316-T03-C	1	1.14E+03			1.14E+03	1.3E+00	1.5E+00	4.8E+00			---		VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1316-T04-C	1	2.03E+03			2.03E+03	6.6E-01	1.5E+00	4.8E+00			---		VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
V	SWA-L07-1316-B01-A	1	7.50E-01	U1/2		7.50E-01		1.5E+00	4.8E+00			---		VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	SWA-L07-1316-T01-A	1	5.00E-01	U1/2		5.00E-01	2.3E+02	1.0E+00	3.2E+00			---		VU ICP-OES	12/3/10 12:31 PM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1316-T02-A	1	5.00E-01	U1/2		5.00E-01	1.9E+01	1.0E+00	3.2E+00	10	120	1.09E+03	91%	VU ICP-OES	12/3/10 12:32 PM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1316-T03-A	1	6.48E+00			6.48E+00	7.5E+01	1.0E+00	3.2E+00			---		VU ICP-OES	12/3/10 12:34 PM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1316-T04-A	1	7.57E+00			7.57E+00	2.8E+00	1.0E+00	3.2E+00			---		VU ICP-OES	12/3/10 12:36 PM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1316-T01-B	1	5.00E-01	U1/2		5.00E-01	1.4E+02	1.0E+00	3.2E+00			---		VU ICP-OES	12/3/10 12:37 PM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1316-T02-B	1	5.00E-01	U1/2		5.00E-01	4.1E+01	1.0E+00	3.2E+00	10	120	1.17E+03	98%	VU ICP-OES	12/3/10 12:39 PM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1316-T03-B	1	7.19E+00			7.19E+00	9.0E+01	1.0E+00	3.2E+00			---		VU ICP-OES	12/3/10 12:40 PM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1316-T04-B	1	1.09E+01			1.09E+01	4.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	12/3/10 12:42 PM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1316-T01-C	1	5.00E-01	U1/2		5.00E-01	9.3E+01	1.0E+00	3.2E+00			---		VU ICP-OES	12/3/10 12:44 PM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1316-T02-C	1	5.00E-01	U1/2		5.00E-01	1.8E+01	1.0E+00	3.2E+00	10	120	1.22E+03	101%	VU ICP-OES	12/3/10 12:45 PM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1316-T03-C	1	7.53E+00			7.53E+00	1.2E+02	1.0E+00	3.2E+00			---		VU ICP-OES	12/3/10 12:47 PM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1316-T04-C	1	1.09E+01			1.09E+01	8.2E+00	1.0E+00	3.2E+00			---		VU ICP-OES	12/3/10 12:49 PM	EPA Interlab L07 1313-1316 SWA
Zn	SWA-L07-1316-B01-A	1	5.00E-01	U1/2		5.00E-01		1.0E+00	3.2E+00			---		VU ICP-OES	12/3/10 12:29 PM	EPA Interlab L07 1313-1316 SWA

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	SWA-L09-1316-T01-A	1	3.37E+04			3.37E+04	8.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:56 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1316-T02-A	1	5.03E+04			5.03E+04	3.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:19 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1316-T03-A	1	2.30E+04			2.30E+04	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:57 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1316-T04-A	1	1.05E+05			1.05E+05	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:59 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1316-T05-A	1	1.88E+05			1.88E+05	4.1E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 4:01 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1316-T01-B	1	3.06E+04			3.06E+04	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:02 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1316-T02-B	1	5.02E+04			5.02E+04	2.6E-01	1.0E+00	3.2E+00	1000	100	5.12E+04	96%	VU ICP-OES	4/20/11 4:04 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1316-T03-B	1	2.56E+04			2.56E+04	4.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:05 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1316-T04-B	1	1.18E+05			1.18E+05	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:07 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1316-T05-B	1	1.93E+05			1.93E+05	4.1E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 4:09 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1316-T01-C	1	3.35E+04			3.35E+04	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:10 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1316-T02-C	1	5.03E+04			5.03E+04	4.0E-02	1.0E+00	3.2E+00	1000	100	5.12E+04	97%	VU ICP-OES	4/20/11 4:12 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1316-T03-C	1	2.73E+04			2.73E+04	7.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:14 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1316-T04-C	1	1.19E+05			1.19E+05	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:15 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1316-T05-C	1	1.99E+05			1.99E+05	2.2E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 4:17 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1316-B01-A	1	2.14E+00	E		2.14E+00	2.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1316-B01-B	1	5.00E-01	U1/2		5.00E-01	9.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
Al	SWA-L09-1316-B01-C	1	2.92E+00	E		2.92E+00	4.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	SWA-L09-1316-T01-A	1	4.49E+03			4.49E+03	1.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 4:23 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L09-1316-T02-A	1	3.05E+03			3.05E+03	6.2E-01	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 4:25 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L09-1316-T03-A	1	6.97E+03			6.97E+03	5.4E-01	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 4:27 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L09-1316-T04-A	1	7.45E+03			7.45E+03	3.9E-01	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 4:30 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L09-1316-T05-A	1	6.25E+03			6.25E+03	8.3E-01	7.5E+00	2.4E+01					VU ICP-OES	5/23/11 4:32 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L09-1316-T01-B	1	3.45E+03			3.45E+03	5.3E-01	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 4:34 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L09-1316-T02-B	1	2.96E+03			2.96E+03	5.8E-01	7.5E+00	2.4E+01	10	100	3.85E+03	88%	VU ICP-OES	5/23/11 4:36 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L09-1316-T03-B	1	7.04E+03			7.04E+03	7.3E-01	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 4:39 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L09-1316-T04-B	1	7.17E+03			7.17E+03	8.8E-01	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 4:41 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L09-1316-T05-B	1	7.21E+03			7.21E+03	6.4E-01	7.5E+00	2.4E+01					VU ICP-OES	5/23/11 4:43 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L09-1316-T01-C	1	4.23E+03			4.23E+03	1.3E-01	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 4:45 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L09-1316-T02-C	1	3.14E+03			3.14E+03	8.0E-01	7.5E+00	2.4E+01	10	100	4.06E+03	92%	VU ICP-OES	5/23/11 4:48 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L09-1316-T03-C	1	7.60E+03			7.60E+03	1.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 4:50 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L09-1316-T04-C	1	7.70E+03			7.70E+03	8.1E-01	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 4:52 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L09-1316-T05-C	1	6.82E+03			6.82E+03	3.8E-01	7.5E+00	2.4E+01					VU ICP-OES	5/23/11 4:55 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L09-1316-B01-A	1	3.75E+00	U1/2		3.75E+00	6.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1316-B01-B	1	3.75E+00	U1/2		3.75E+00	7.4E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
Sb	SWA-L09-1316-B01-C	1	3.75E+00	U1/2		3.75E+00	2.0E+02	7.5E+00	2.4E+01				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	SWA-L09-1316-T01-A	1	3.96E+03			3.96E+03	7.0E-01	1.1E+01	3.5E+01				---	VU ICP-OES	5/23/11 4:23 PM	EPA Interlab 1316 SWA Reruns
As	SWA-L09-1316-T02-A	1	1.01E+04			1.01E+04	3.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	5/23/11 4:25 PM	EPA Interlab 1316 SWA Reruns
As	SWA-L09-1316-T03-A	1	2.47E+04			2.47E+04	3.5E-01	1.1E+01	3.5E+01				---	VU ICP-OES	5/23/11 4:27 PM	EPA Interlab 1316 SWA Reruns
As	SWA-L09-1316-T04-A	1	1.03E+05			1.03E+05	3.7E-01	1.1E+01	3.5E+01				---	VU ICP-OES	5/23/11 4:30 PM	EPA Interlab 1316 SWA Reruns
As	SWA-L09-1316-T05-A	1	2.62E+05			2.62E+05	1.6E+00	1.1E+01	3.5E+01					VU ICP-OES	5/23/11 4:32 PM	EPA Interlab 1316 SWA Reruns
As	SWA-L09-1316-T01-B	1	2.69E+03			2.69E+03	7.9E-01	1.1E+01	3.5E+01				---	VU ICP-OES	5/23/11 4:34 PM	EPA Interlab 1316 SWA Reruns
As	SWA-L09-1316-T02-B	1	9.72E+03			9.72E+03	2.2E+00	1.1E+01	3.5E+01	10	100	1.06E+04	92%	VU ICP-OES	5/23/11 4:36 PM	EPA Interlab 1316 SWA Reruns
As	SWA-L09-1316-T03-B	1	2.98E+04			2.98E+04	1.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	5/23/11 4:39 PM	EPA Interlab 1316 SWA Reruns
As	SWA-L09-1316-T04-B	1	9.10E+04			9.10E+04	6.3E-01	1.1E+01	3.5E+01				---	VU ICP-OES	5/23/11 4:41 PM	EPA Interlab 1316 SWA Reruns
As	SWA-L09-1316-T05-B	1	2.28E+05			2.28E+05	9.1E-01	1.1E+01	3.5E+01					VU ICP-OES	5/23/11 4:43 PM	EPA Interlab 1316 SWA Reruns
As	SWA-L09-1316-T01-C	1	3.93E+03			3.93E+03	6.1E-01	1.1E+01	3.5E+01				---	VU ICP-OES	5/23/11 4:45 PM	EPA Interlab 1316 SWA Reruns
As	SWA-L09-1316-T02-C	1	1.01E+04			1.01E+04	2.3E-01	1.1E+01	3.5E+01	10	100	1.10E+04	90%	VU ICP-OES	5/23/11 4:48 PM	EPA Interlab 1316 SWA Reruns
As	SWA-L09-1316-T03-C	1	3.26E+04			3.26E+04	5.5E-01	1.1E+01	3.5E+01				---	VU ICP-OES	5/23/11 4:50 PM	EPA Interlab 1316 SWA Reruns
As	SWA-L09-1316-T04-C	1	9.93E+04			9.93E+04	1.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	5/23/11 4:52 PM	EPA Interlab 1316 SWA Reruns
As	SWA-L09-1316-T05-C	1	2.29E+05			2.29E+05	1.1E+00	1.1E+01	3.5E+01					VU ICP-OES	5/23/11 4:55 PM	EPA Interlab 1316 SWA Reruns
As	SWA-L09-1316-B01-A	1	5.50E+00	U1/2		5.50E+00	1.5E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1316-B01-B	1	5.50E+00	U1/2		5.50E+00	8.5E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
As	SWA-L09-1316-B01-C	1	5.50E+00	U1/2		5.50E+00	2.5E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	SWA-L09-1316-T01-A	1	7.97E+02			7.97E+02	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:56 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1316-T02-A	1	1.09E+03			1.09E+03	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:19 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1316-T03-A	1	1.12E+03			1.12E+03	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:57 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1316-T04-A	1	9.40E+02			9.40E+02	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:59 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1316-T05-A	1	2.38E+03			2.38E+03	1.0E+00	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 4:01 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1316-T01-B	1	5.79E+02			5.79E+02	3.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:02 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1316-T02-B	1	1.04E+03			1.04E+03	6.3E-01	1.0E+00	3.2E+00	1000	100	2.02E+03	98%	VU ICP-OES	4/20/11 4:04 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1316-T03-B	1	9.24E+02			9.24E+02	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:05 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1316-T04-B	1	7.72E+02			7.72E+02	8.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:07 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1316-T05-B	1	2.43E+03			2.43E+03	6.1E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 4:09 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1316-T01-C	1	7.83E+02			7.83E+02	1.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:10 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1316-T02-C	1	1.13E+03			1.13E+03	1.8E-01	1.0E+00	3.2E+00	1000	100	2.03E+03	90%	VU ICP-OES	4/20/11 4:12 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1316-T03-C	1	1.31E+03			1.31E+03	4.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:14 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1316-T04-C	1	1.12E+03			1.12E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:15 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1316-T05-C	1	1.77E+03			1.77E+03	2.2E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 4:17 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1316-B01-A	1	2.85E+01			2.85E+01	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1316-B01-B	1	2.05E+01			2.05E+01	5.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
B	SWA-L09-1316-B01-C	1	1.67E+01			1.67E+01	5.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	SWA-L09-1316-T01-A	1	2.26E+02			2.26E+02	7.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:23 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L09-1316-T02-A	1	2.01E+02			2.01E+02	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:25 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L09-1316-T03-A	1	5.98E+01			5.98E+01	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:27 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L09-1316-T04-A	1	6.71E+01			6.71E+01	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:30 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L09-1316-T05-A	1	3.83E+01			3.83E+01	9.3E-01	1.0E+00	3.2E+00					VU ICP-OES	5/23/11 4:32 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L09-1316-T01-B	1	2.49E+02			2.49E+02	8.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:34 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L09-1316-T02-B	1	2.02E+02			2.02E+02	8.3E-01	1.0E+00	3.2E+00	10	100	1.07E+03	86%	VU ICP-OES	5/23/11 4:36 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L09-1316-T03-B	1	6.49E+01			6.49E+01	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:39 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L09-1316-T04-B	1	6.71E+01			6.71E+01	2.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:41 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L09-1316-T05-B	1	3.65E+01			3.65E+01	2.5E+00	1.0E+00	3.2E+00					VU ICP-OES	5/23/11 4:43 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L09-1316-T01-C	1	2.24E+02			2.24E+02	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:45 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L09-1316-T02-C	1	2.02E+02			2.02E+02	5.8E-01	1.0E+00	3.2E+00	10	100	1.15E+03	95%	VU ICP-OES	5/23/11 4:48 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L09-1316-T03-C	1	1.85E+01			1.85E+01	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:50 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L09-1316-T04-C	1	5.65E+01			5.65E+01	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:52 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L09-1316-T05-C	1	3.72E+01			3.72E+01	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	5/23/11 4:55 PM	EPA Interlab 1316 SWA Reruns
Ba	SWA-L09-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	2.0E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1316-B01-B	1	5.00E-01	U1/2		5.00E-01	5.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
Ba	SWA-L09-1316-B01-C	1	5.00E-01	U1/2		5.00E-01	2.1E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	SWA-L09-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	4.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:56 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	3.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 4:19 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	1.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:57 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	8.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:59 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1316-T05-A	1	9.50E-01	U1/2		9.50E-01	1.4E+01	1.9E+00	6.0E+00					VU ICP-OES	4/20/11 4:01 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	6.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 4:02 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	2.3E+01	1.9E+00	6.0E+00	10	100	9.38E+02	94%	VU ICP-OES	4/20/11 4:04 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	9.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 4:05 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	2.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 4:07 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1316-T05-B	1	9.50E-01	U1/2		9.50E-01	2.3E+01	1.9E+00	6.0E+00					VU ICP-OES	4/20/11 4:09 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	2.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 4:10 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	3.6E+01	1.9E+00	6.0E+00	10	100	1.02E+03	101%	VU ICP-OES	4/20/11 4:12 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	3.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 4:14 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	4.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 4:15 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1316-T05-C	1	9.50E-01	U1/2		9.50E-01	9.5E+00	1.9E+00	6.0E+00					VU ICP-OES	4/20/11 4:17 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	4.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1316-B01-B	1	9.50E-01	U1/2		9.50E-01	2.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
Be	SWA-L09-1316-B01-C	1	9.50E-01	U1/2		9.50E-01	3.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	SWA-L09-1316-T01-A	1	1.10E+00	U1/2		1.10E+00	2.0E+01	2.2E+00	7.0E+00				---	VU ICP-OES	4/20/11 3:56 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1316-T02-A	1	1.10E+00	U1/2		1.10E+00	1.2E+02	2.2E+00	7.0E+00				---	VU ICP-OES	4/20/11 4:19 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1316-T03-A	1	1.10E+00	U1/2		1.10E+00	7.5E+01	2.2E+00	7.0E+00				---	VU ICP-OES	4/20/11 3:57 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1316-T04-A	1	1.10E+00	U1/2		1.10E+00	1.9E+01	2.2E+00	7.0E+00				---	VU ICP-OES	4/20/11 3:59 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1316-T05-A	1	1.10E+00	U1/2		1.10E+00	3.5E+01	2.2E+00	7.0E+00					VU ICP-OES	4/20/11 4:01 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1316-T01-B	1	1.10E+00	U1/2		1.10E+00	1.9E+02	2.2E+00	7.0E+00				---	VU ICP-OES	4/20/11 4:02 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1316-T02-B	1	1.10E+00	U1/2		1.10E+00	1.6E+02	2.2E+00	7.0E+00	10	100	9.24E+02	92%	VU ICP-OES	4/20/11 4:04 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1316-T03-B	1	1.10E+00	U1/2		1.10E+00	1.3E+02	2.2E+00	7.0E+00				---	VU ICP-OES	4/20/11 4:05 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1316-T04-B	1	1.10E+00	U1/2		1.10E+00	1.2E+02	2.2E+00	7.0E+00				---	VU ICP-OES	4/20/11 4:07 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1316-T05-B	1	1.10E+00	U1/2		1.10E+00	5.8E+01	2.2E+00	7.0E+00					VU ICP-OES	4/20/11 4:09 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1316-T01-C	1	1.10E+00	U1/2		1.10E+00	4.6E+01	2.2E+00	7.0E+00				---	VU ICP-OES	4/20/11 4:10 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1316-T02-C	1	1.10E+00	U1/2		1.10E+00	2.6E+01	2.2E+00	7.0E+00	10	100	8.92E+02	89%	VU ICP-OES	4/20/11 4:12 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1316-T03-C	1	1.10E+00	U1/2		1.10E+00	7.9E+01	2.2E+00	7.0E+00				---	VU ICP-OES	4/20/11 4:14 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1316-T04-C	1	1.10E+00	U1/2		1.10E+00	1.2E+02	2.2E+00	7.0E+00				---	VU ICP-OES	4/20/11 4:15 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1316-T05-C	1	1.10E+00	U1/2		1.10E+00	5.4E+01	2.2E+00	7.0E+00					VU ICP-OES	4/20/11 4:17 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1316-B01-A	1	1.10E+00	U1/2		1.10E+00	1.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1316-B01-B	1	1.10E+00	U1/2		1.10E+00	1.3E+02	2.2E+00	7.0E+00				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
Cd	SWA-L09-1316-B01-C	1	1.10E+00	U1/2		1.10E+00	7.7E+01	2.2E+00	7.0E+00				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	SWA-L09-1316-T01-A	1	1.45E+04			1.45E+04	8.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/23/11 4:23 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L09-1316-T02-A	1	1.12E+04			1.12E+04	8.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/23/11 4:25 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L09-1316-T03-A	1	2.39E+03			2.39E+03	1.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/23/11 4:27 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L09-1316-T04-A	1	3.70E+03			3.70E+03	3.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/23/11 4:30 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L09-1316-T05-A	1	3.12E+03			3.12E+03	8.6E+00	2.6E+00	8.3E+00					VU ICP-OES	5/23/11 4:32 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L09-1316-T01-B	1	1.66E+04			1.66E+04	6.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/23/11 4:34 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L09-1316-T02-B	1	1.12E+04			1.12E+04	4.6E-01	2.6E+00	8.3E+00	1000	100	1.21E+04	87%	VU ICP-OES	5/23/11 4:36 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L09-1316-T03-B	1	2.65E+03			2.65E+03	6.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/23/11 4:39 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L09-1316-T04-B	1	3.40E+03			3.40E+03	5.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/23/11 4:41 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L09-1316-T05-B	1	3.73E+03			3.73E+03	1.1E+01	2.6E+00	8.3E+00					VU ICP-OES	5/23/11 4:43 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L09-1316-T01-C	1	1.44E+04			1.44E+04	2.7E-02	2.6E+00	8.3E+00				---	VU ICP-OES	5/23/11 4:45 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L09-1316-T02-C	1	1.11E+04			1.11E+04	6.2E-01	2.6E+00	8.3E+00	1000	100	1.19E+04	89%	VU ICP-OES	5/23/11 4:48 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L09-1316-T03-C	1	2.34E+03			2.34E+03	1.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/23/11 4:50 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L09-1316-T04-C	1	3.37E+03			3.37E+03	9.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/23/11 4:52 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L09-1316-T05-C	1	3.23E+03			3.23E+03	4.5E+00	2.6E+00	8.3E+00					VU ICP-OES	5/23/11 4:55 PM	EPA Interlab 1316 SWA Reruns
Ca	SWA-L09-1316-B01-A	1	2.60E+01			2.60E+01	6.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1316-B01-B	1	2.24E+01			2.24E+01	1.1E+01	2.6E+00	8.3E+00				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
Ca	SWA-L09-1316-B01-C	1	3.11E+01			3.11E+01	1.9E+01	2.6E+00	8.3E+00				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	SWA-L09-1316-T01-A	1	1.03E+03			1.03E+03	1.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/23/11 4:23 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L09-1316-T02-A	1	1.67E+03			1.67E+03	5.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/23/11 4:25 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L09-1316-T03-A	1	9.40E+02			9.40E+02	6.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/23/11 4:27 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L09-1316-T04-A	1	1.86E+03			1.86E+03	7.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/23/11 4:30 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L09-1316-T05-A	1	2.62E+03			2.62E+03	8.3E-01	1.2E+00	3.8E+00					VU ICP-OES	5/23/11 4:32 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L09-1316-T01-B	1	9.53E+02			9.53E+02	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/23/11 4:34 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L09-1316-T02-B	1	1.75E+03			1.75E+03	1.8E+00	1.2E+00	3.8E+00	10	100	2.64E+03	89%	VU ICP-OES	5/23/11 4:36 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L09-1316-T03-B	1	1.29E+03			1.29E+03	1.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/23/11 4:39 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L09-1316-T04-B	1	2.42E+03			2.42E+03	2.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/23/11 4:41 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L09-1316-T05-B	1	2.81E+03			2.81E+03	1.3E+00	1.2E+00	3.8E+00					VU ICP-OES	5/23/11 4:43 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L09-1316-T01-C	1	9.77E+02			9.77E+02	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/23/11 4:45 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L09-1316-T02-C	1	1.60E+03			1.60E+03	6.7E-01	1.2E+00	3.8E+00	10	100	2.55E+03	95%	VU ICP-OES	5/23/11 4:48 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L09-1316-T03-C	1	1.87E+02			1.87E+02	6.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/23/11 4:50 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L09-1316-T04-C	1	1.86E+03			1.86E+03	9.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/23/11 4:52 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L09-1316-T05-C	1	2.91E+03			2.91E+03	4.2E-01	1.2E+00	3.8E+00					VU ICP-OES	5/23/11 4:55 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L09-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	6.8E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1316-B01-B	1	6.00E-01	U1/2		6.00E-01	1.4E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
Cr	SWA-L09-1316-B01-C	1	6.00E-01	U1/2		6.00E-01	8.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	SWA-L09-1316-T01-A	1	9.00E-01	U1/2		9.00E-01	2.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 3:56 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1316-T02-A	1	9.00E-01	U1/2		9.00E-01	5.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 4:19 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1316-T03-A	1	2.51E+00	E		2.51E+00	3.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 3:57 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1316-T04-A	1	7.18E+00			7.18E+00	1.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 3:59 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1316-T05-A	1	9.61E+00			9.61E+00	4.4E+00	1.8E+00	5.7E+00					VU ICP-OES	4/20/11 4:01 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1316-T01-B	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 4:02 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1316-T02-B	1	9.00E-01	U1/2		9.00E-01	7.7E+01	1.8E+00	5.7E+00	10	100	9.29E+02	93%	VU ICP-OES	4/20/11 4:04 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1316-T03-B	1	3.45E+00	E		3.45E+00	2.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 4:05 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1316-T04-B	1	7.91E+00			7.91E+00	7.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 4:07 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1316-T05-B	1	9.86E+00			9.86E+00	1.3E+01	1.8E+00	5.7E+00					VU ICP-OES	4/20/11 4:09 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1316-T01-C	1	9.00E-01	U1/2		9.00E-01	8.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 4:10 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1316-T02-C	1	9.00E-01	U1/2		9.00E-01	5.0E+01	1.8E+00	5.7E+00	10	100	1.00E+03	100%	VU ICP-OES	4/20/11 4:12 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1316-T03-C	1	2.17E+00	E		2.17E+00	1.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 4:14 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1316-T04-C	1	7.74E+00			7.74E+00	1.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 4:15 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1316-T05-C	1	1.22E+01			1.22E+01	1.9E+00	1.8E+00	5.7E+00					VU ICP-OES	4/20/11 4:17 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	2.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1316-B01-B	1	9.00E-01	U1/2		9.00E-01	1.6E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
Co	SWA-L09-1316-B01-C	1	9.00E-01	U1/2		9.00E-01	1.2E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	SWA-L09-1316-T01-A	1	1.85E+00	U1/2		1.85E+00	7.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:56 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1316-T02-A	1	1.85E+00	U1/2		1.85E+00	4.9E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 4:19 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1316-T03-A	1	4.00E+00	E		4.00E+00	2.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:57 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1316-T04-A	1	3.83E+01			3.83E+01	1.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:59 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1316-T05-A	1	1.26E+02			1.26E+02	1.7E+00	3.7E+00	1.2E+01					VU ICP-OES	4/20/11 4:01 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1316-T01-B	1	1.85E+00	U1/2		1.85E+00	8.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 4:02 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1316-T02-B	1	1.85E+00	U1/2		1.85E+00	1.9E+03	3.7E+00	1.2E+01	10	100	9.23E+02	92%	VU ICP-OES	4/20/11 4:04 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1316-T03-B	1	3.79E+00	E		3.79E+00	1.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 4:05 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1316-T04-B	1	3.28E+01			3.28E+01	1.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 4:07 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1316-T05-B	1	1.27E+02			1.27E+02	3.2E+00	3.7E+00	1.2E+01					VU ICP-OES	4/20/11 4:09 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1316-T01-C	1	1.85E+00	U1/2		1.85E+00	1.1E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 4:10 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1316-T02-C	1	1.85E+00	U1/2		1.85E+00	1.5E+02	3.7E+00	1.2E+01	10	100	1.01E+03	101%	VU ICP-OES	4/20/11 4:12 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1316-T03-C	1	4.68E+00	E		4.68E+00	9.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 4:14 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1316-T04-C	1	4.27E+01			4.27E+01	3.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 4:15 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1316-T05-C	1	9.92E+01			9.92E+01	2.0E+00	3.7E+00	1.2E+01					VU ICP-OES	4/20/11 4:17 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	9.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1316-B01-B	1	1.85E+00	U1/2		1.85E+00	8.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
Cu	SWA-L09-1316-B01-C	1	1.85E+00	U1/2		1.85E+00	1.4E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	SWA-L09-1316-T01-A	1	6.93E+01			6.93E+01	7.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 3:56 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1316-T02-A	1	1.40E+02			1.40E+02	8.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 4:19 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1316-T03-A	1	4.19E+01			4.19E+01	9.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 3:57 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1316-T04-A	1	7.85E+02			7.85E+02	6.1E-02	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 3:59 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1316-T05-A	1	2.27E+03			2.27E+03	5.5E-01	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 4:01 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1316-T01-B	1	5.16E+01			5.16E+01	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 4:02 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1316-T02-B	1	1.37E+02			1.37E+02	6.5E-01	2.0E+00	6.4E+00	1000	100	1.30E+03	116%	VU ICP-OES	4/20/11 4:04 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1316-T03-B	1	5.71E+01			5.71E+01	2.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 4:05 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1316-T04-B	1	6.99E+02			6.99E+02	1.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 4:07 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1316-T05-B	1	2.08E+03			2.08E+03	9.8E-01	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 4:09 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1316-T01-C	1	6.87E+01			6.87E+01	4.1E-02	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 4:10 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1316-T02-C	1	1.44E+02			1.44E+02	7.3E-01	2.0E+00	6.4E+00	1000	100	1.21E+03	107%	VU ICP-OES	4/20/11 4:12 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1316-T03-C	1	5.25E+01			5.25E+01	1.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 4:14 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1316-T04-C	1	8.88E+02			8.88E+02	8.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 4:15 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1316-T05-C	1	2.12E+03			2.12E+03	3.1E-01	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 4:17 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	2.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1316-B01-B	1	1.00E+00	U1/2		1.00E+00	3.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
Fe	SWA-L09-1316-B01-C	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	SWA-L09-1316-T01-A	1	1.41E+01	E		1.41E+01	3.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:56 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1316-T02-A	1	2.32E+01			2.32E+01	6.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 4:19 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1316-T03-A	1	2.78E+01			2.78E+01	1.2E+02	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:57 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1316-T04-A	1	2.84E+01			2.84E+01	1.7E+01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:59 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1316-T05-A	1	1.14E+02			1.14E+02	6.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 4:01 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1316-T01-B	1	1.13E+01	E		1.13E+01	2.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 4:02 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1316-T02-B	1	2.40E+01			2.40E+01	8.9E+00	6.8E+00	2.2E+01	10	100	9.14E+02	89%	VU ICP-OES	4/20/11 4:04 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1316-T03-B	1	2.75E+01			2.75E+01	5.7E+01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 4:05 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1316-T04-B	1	3.16E+01			3.16E+01	2.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 4:07 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1316-T05-B	1	1.38E+02			1.38E+02	3.6E+00	6.8E+00	2.2E+01					VU ICP-OES	4/20/11 4:09 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1316-T01-C	1	1.52E+01	E		1.52E+01	7.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 4:10 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1316-T02-C	1	2.69E+01			2.69E+01	4.1E+00	6.8E+00	2.2E+01	10	100	1.04E+03	101%	VU ICP-OES	4/20/11 4:12 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1316-T03-C	1	2.96E+01			2.96E+01	2.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 4:14 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1316-T04-C	1	2.99E+01			2.99E+01	6.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 4:15 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1316-T05-C	1	1.69E+02			1.69E+02	3.2E+00	6.8E+00	2.2E+01					VU ICP-OES	4/20/11 4:17 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	4.0E+02	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1316-B01-B	1	3.40E+00	U1/2		3.40E+00	6.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
Pb	SWA-L09-1316-B01-C	1	3.40E+00	U1/2		3.40E+00	6.1E+02	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	SWA-L09-1316-T01-A	1	3.24E+00	E		3.24E+00	3.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:56 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1316-T02-A	1	5.52E+00	E		5.52E+00	4.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 4:19 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1316-T03-A	1	6.00E+00	E		6.00E+00	4.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:57 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1316-T04-A	1	8.30E+00			8.30E+00	1.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:59 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1316-T05-A	1	1.16E+01			1.16E+01	9.8E+00	1.9E+00	6.0E+00					VU ICP-OES	4/20/11 4:01 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1316-T01-B	1	3.65E+00	E		3.65E+00	2.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 4:02 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1316-T02-B	1	6.07E+00			6.07E+00	5.0E+01	1.9E+00	6.0E+00	10	100	8.92E+02	89%	VU ICP-OES	4/20/11 4:04 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1316-T03-B	1	5.67E+00	E		5.67E+00	4.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 4:05 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1316-T04-B	1	9.23E+00			9.23E+00	2.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 4:07 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1316-T05-B	1	1.20E+01			1.20E+01	2.2E+01	1.9E+00	6.0E+00					VU ICP-OES	4/20/11 4:09 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1316-T01-C	1	3.71E+00	E		3.71E+00	1.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 4:10 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1316-T02-C	1	5.07E+00	E		5.07E+00	7.1E+00	1.9E+00	6.0E+00	10	100	9.10E+02	91%	VU ICP-OES	4/20/11 4:12 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1316-T03-C	1	7.76E+00			7.76E+00	2.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 4:14 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1316-T04-C	1	9.54E+00			9.54E+00	1.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 4:15 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1316-T05-C	1	1.30E+01			1.30E+01	1.7E+01	1.9E+00	6.0E+00					VU ICP-OES	4/20/11 4:17 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1316-B01-A	1	3.13E+00	E		3.13E+00	2.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1316-B01-B	1	9.50E-01	U1/2		9.50E-01	2.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
Li	SWA-L09-1316-B01-C	1	2.49E+00	E		2.49E+00	3.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	SWA-L09-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	8.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 3:56 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	7.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 4:19 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	3.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 3:57 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	3.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 3:59 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1316-T05-A	1	1.00E+00	U1/2		1.00E+00	3.1E+00	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 4:01 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	6.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 4:02 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00	10	100	9.17E+02	92%	VU ICP-OES	4/20/11 4:04 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	6.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 4:05 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	4.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 4:07 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1316-T05-B	1	1.00E+00	U1/2		1.00E+00	3.5E+00	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 4:09 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	7.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 4:10 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	6.3E+00	2.0E+00	6.4E+00	10	100	9.88E+02	99%	VU ICP-OES	4/20/11 4:12 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	9.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 4:14 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	6.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 4:15 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1316-T05-C	1	1.00E+00	U1/2		1.00E+00	3.0E+00	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 4:17 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1316-B01-B	1	1.00E+00	U1/2		1.00E+00	4.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
Mn	SWA-L09-1316-B01-C	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	SWA-L09-1316-T01-A	1	8.66E+00			8.66E+00	6.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:56 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1316-T02-A	1	8.54E+00			8.54E+00	8.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:19 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1316-T03-A	1	1.24E+01			1.24E+01	1.0E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:57 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1316-T04-A	1	1.42E+01			1.42E+01	2.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:59 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1316-T05-A	1	1.63E+01			1.63E+01	7.0E+01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 4:01 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1316-T01-B	1	9.37E+00			9.37E+00	4.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:02 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1316-T02-B	1	7.55E+00			7.55E+00	3.4E+01	1.0E+00	3.2E+00	1000	100	9.41E+02	93%	VU ICP-OES	4/20/11 4:04 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1316-T03-B	1	1.16E+01			1.16E+01	6.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:05 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1316-T04-B	1	1.13E+01			1.13E+01	6.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:07 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1316-T05-B	1	1.47E+01			1.47E+01	5.4E+01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 4:09 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1316-T01-C	1	1.11E+01			1.11E+01	4.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:10 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1316-T02-C	1	1.05E+01			1.05E+01	3.1E+00	1.0E+00	3.2E+00	1000	100	1.02E+03	101%	VU ICP-OES	4/20/11 4:12 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1316-T03-C	1	1.29E+01			1.29E+01	1.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:14 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1316-T04-C	1	1.30E+01			1.30E+01	7.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:15 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1316-T05-C	1	1.08E+01			1.08E+01	6.0E+01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 4:17 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	5.0E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1316-B01-B	1	5.00E-01	U1/2		5.00E-01	4.6E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
Mg	SWA-L09-1316-B01-C	1	5.00E-01	U1/2		5.00E-01	4.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	SWA-L09-1316-T01-A	1	1.23E+02			1.23E+02	8.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/20/11 3:56 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1316-T02-A	1	1.82E+02			1.82E+02	2.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/20/11 4:19 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1316-T03-A	1	4.83E+02			4.83E+02	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/20/11 3:57 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1316-T04-A	1	9.84E+02			9.84E+02	4.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/20/11 3:59 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1316-T05-A	1	2.34E+03			2.34E+03	1.6E+00	1.2E+00	3.8E+00					VU ICP-OES	4/20/11 4:01 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1316-T01-B	1	1.10E+02			1.10E+02	1.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/20/11 4:02 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1316-T02-B	1	1.88E+02			1.88E+02	1.7E-01	1.2E+00	3.8E+00	10	100	1.07E+03	88%	VU ICP-OES	4/20/11 4:04 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1316-T03-B	1	4.73E+02			4.73E+02	3.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/20/11 4:05 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1316-T04-B	1	9.68E+02			9.68E+02	5.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/20/11 4:07 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1316-T05-B	1	2.03E+03			2.03E+03	8.1E-01	1.2E+00	3.8E+00					VU ICP-OES	4/20/11 4:09 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1316-T01-C	1	1.22E+02			1.22E+02	5.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/20/11 4:10 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1316-T02-C	1	1.77E+02			1.77E+02	9.1E-01	1.2E+00	3.8E+00	10	100	1.21E+03	103%	VU ICP-OES	4/20/11 4:12 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1316-T03-C	1	4.88E+02			4.88E+02	7.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/20/11 4:14 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1316-T04-C	1	1.00E+03			1.00E+03	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/20/11 4:15 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1316-T05-C	1	2.06E+03			2.06E+03	1.2E+00	1.2E+00	3.8E+00					VU ICP-OES	4/20/11 4:17 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1316-B01-A	1	1.29E+00	E		1.29E+00	7.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1316-B01-B	1	2.33E+00	E		2.33E+00	6.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
Mo	SWA-L09-1316-B01-C	1	1.79E+00	E		1.79E+00	8.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	SWA-L09-1316-T01-A	1	9.00E-01	U1/2		9.00E-01	1.2E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 3:56 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1316-T02-A	1	9.00E-01	U1/2		9.00E-01	3.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 4:19 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1316-T03-A	1	3.30E+00	E		3.30E+00	5.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 3:57 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1316-T04-A	1	4.97E+00	E		4.97E+00	1.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 3:59 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1316-T05-A	1	1.10E+01			1.10E+01	7.6E+00	1.8E+00	5.7E+00					VU ICP-OES	4/20/11 4:01 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1316-T01-B	1	9.00E-01	U1/2		9.00E-01	9.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 4:02 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1316-T02-B	1	9.00E-01	U1/2		9.00E-01	2.5E+01	1.8E+00	5.7E+00	10	100	8.51E+02	85%	VU ICP-OES	4/20/11 4:04 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1316-T03-B	1	3.29E+00	E		3.29E+00	1.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 4:05 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1316-T04-B	1	5.10E+00	E		5.10E+00	2.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 4:07 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1316-T05-B	1	7.20E+00			7.20E+00	1.9E+01	1.8E+00	5.7E+00					VU ICP-OES	4/20/11 4:09 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1316-T01-C	1	9.00E-01	U1/2		9.00E-01	4.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 4:10 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1316-T02-C	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00	10	100	9.22E+02	92%	VU ICP-OES	4/20/11 4:12 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1316-T03-C	1	3.24E+00	E		3.24E+00	2.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 4:14 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1316-T04-C	1	4.12E+00	E		4.12E+00	1.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 4:15 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1316-T05-C	1	8.22E+00			8.22E+00	2.5E+01	1.8E+00	5.7E+00					VU ICP-OES	4/20/11 4:17 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	8.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1316-B01-B	1	9.00E-01	U1/2		9.00E-01	2.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
Ni	SWA-L09-1316-B01-C	1	9.00E-01	U1/2		9.00E-01	2.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	SWA-L09-1316-T01-A	1	3.61E+01			3.61E+01	2.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:56 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1316-T02-A	1	6.64E+01			6.64E+01	5.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 4:19 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1316-T03-A	1	1.49E+02			1.49E+02	3.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:57 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1316-T04-A	1	9.71E+02			9.71E+02	2.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:59 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1316-T05-A	1	3.49E+03			3.49E+03	1.0E+00	3.7E+00	1.2E+01					VU ICP-OES	4/20/11 4:01 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1316-T01-B	1	2.90E+01			2.90E+01	1.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 4:02 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1316-T02-B	1	6.48E+01			6.48E+01	2.3E+01	3.7E+00	1.2E+01	1000	100	1.01E+03	95%	VU ICP-OES	4/20/11 4:04 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1316-T03-B	1	1.59E+02			1.59E+02	4.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 4:05 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1316-T04-B	1	8.97E+02			8.97E+02	5.5E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 4:07 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1316-T05-B	1	3.24E+03			3.24E+03	1.5E+00	3.7E+00	1.2E+01					VU ICP-OES	4/20/11 4:09 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1316-T01-C	1	2.64E+01			2.64E+01	2.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 4:10 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1316-T02-C	1	6.53E+01			6.53E+01	6.1E+00	3.7E+00	1.2E+01	1000	100	9.12E+02	85%	VU ICP-OES	4/20/11 4:12 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1316-T03-C	1	1.85E+02			1.85E+02	1.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 4:14 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1316-T04-C	1	9.74E+02			9.74E+02	1.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 4:15 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1316-T05-C	1	3.13E+03			3.13E+03	2.1E-01	3.7E+00	1.2E+01					VU ICP-OES	4/20/11 4:17 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	6.5E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1316-B01-B	1	1.85E+00	U1/2		1.85E+00	1.6E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
P	SWA-L09-1316-B01-C	1	1.85E+00	U1/2		1.85E+00	8.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	SWA-L09-1316-T01-A	1	2.64E+05			2.64E+05	4.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/20/11 3:56 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1316-T02-A	1	3.99E+05			3.99E+05	4.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/20/11 4:19 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1316-T03-A	1	7.27E+05			7.27E+05	1.2E+01	1.6E+00	5.1E+00				---	VU ICP-OES	4/20/11 3:57 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1316-T04-A	1	2.34E+06			2.34E+06	3.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/20/11 3:59 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1316-T05-A	1	2.53E+06			2.53E+06	6.6E-01	1.6E+00	5.1E+00					VU ICP-OES	4/20/11 4:01 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1316-T01-B	1	2.60E+05			2.60E+05	8.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/20/11 4:02 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1316-T02-B	1	3.97E+05			3.97E+05	3.9E-01	1.6E+00	5.1E+00	1000	100	3.98E+05	92%	VU ICP-OES	4/20/11 4:04 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1316-T03-B	1	7.06E+05			7.06E+05	9.9E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/20/11 4:05 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1316-T04-B	1	2.32E+06			2.32E+06	5.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/20/11 4:07 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1316-T05-B	1	2.51E+06			2.51E+06	1.5E+00	1.6E+00	5.1E+00					VU ICP-OES	4/20/11 4:09 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1316-T01-C	1	2.68E+05			2.68E+05	5.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/20/11 4:10 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1316-T02-C	1	4.00E+05			4.00E+05	1.3E+00	1.6E+00	5.1E+00	1000	100	4.01E+05	109%	VU ICP-OES	4/20/11 4:12 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1316-T03-C	1	7.25E+05			7.25E+05	9.9E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/20/11 4:14 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1316-T04-C	1	2.36E+06			2.36E+06	9.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/20/11 4:15 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1316-T05-C	1	2.47E+06			2.47E+06	9.7E-01	1.6E+00	5.1E+00					VU ICP-OES	4/20/11 4:17 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1316-B01-A	1	3.45E+01			3.45E+01	6.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1316-B01-B	1	3.35E+01			3.35E+01	6.6E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
K	SWA-L09-1316-B01-C	1	3.28E+01			3.28E+01	8.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	SWA-L09-1316-T01-A	1	7.27E+04			7.27E+04	9.1E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 3:56 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1316-T02-A	1	1.25E+05			1.25E+05	7.5E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 4:19 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1316-T03-A	1	3.22E+05			3.22E+05	4.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 3:57 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1316-T04-A	1	6.83E+05			6.83E+05	1.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 3:59 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1316-T05-A	1	1.39E+06			1.39E+06	9.9E-01	1.5E+01	4.8E+01					VU ICP-OES	4/20/11 4:01 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1316-T01-B	1	6.42E+04			6.42E+04	9.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 4:02 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1316-T02-B	1	1.26E+05			1.26E+05	6.0E-01	1.5E+01	4.8E+01	10	100	1.26E+05	92%	VU ICP-OES	4/20/11 4:04 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1316-T03-B	1	3.17E+05			3.17E+05	4.1E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 4:05 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1316-T04-B	1	6.44E+05			6.44E+05	3.3E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 4:07 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1316-T05-B	1	1.24E+06			1.24E+06	1.4E+00	1.5E+01	4.8E+01					VU ICP-OES	4/20/11 4:09 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1316-T01-C	1	7.33E+04			7.33E+04	2.9E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 4:10 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1316-T02-C	1	1.24E+05			1.24E+05	5.2E-01	1.5E+01	4.8E+01	10	100	1.25E+05	101%	VU ICP-OES	4/20/11 4:12 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1316-T03-C	1	3.28E+05			3.28E+05	2.5E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 4:14 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1316-T04-C	1	6.56E+05			6.56E+05	7.2E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 4:15 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1316-T05-C	1	1.24E+06			1.24E+06	6.6E-01	1.5E+01	4.8E+01					VU ICP-OES	4/20/11 4:17 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1316-B01-A	1	7.50E+00	U1/2		7.50E+00	7.2E+01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1316-B01-B	1	7.50E+00	U1/2		7.50E+00	7.0E+01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
Se	SWA-L09-1316-B01-C	1	7.50E+00	U1/2		7.50E+00	4.5E+01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	SWA-L09-1316-T01-A	1	2.31E+04			2.31E+04	5.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 3:56 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1316-T02-A	1	3.13E+04			3.13E+04	1.7E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 4:19 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1316-T03-A	1	9.33E+02			9.33E+02	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 3:57 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1316-T04-A	1	2.50E+04			2.50E+04	5.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 3:59 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1316-T05-A	1	4.86E+04			4.86E+04	7.3E-01	1.1E+00	3.5E+00					VU ICP-OES	4/20/11 4:01 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1316-T01-B	1	2.09E+04			2.09E+04	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 4:02 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1316-T02-B	1	3.11E+04			3.11E+04	4.7E-01	1.1E+00	3.5E+00	1000	100	3.21E+04	104%	VU ICP-OES	4/20/11 4:04 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1316-T03-B	1	7.28E+02			7.28E+02	3.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 4:05 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1316-T04-B	1	3.40E+04			3.40E+04	4.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 4:07 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1316-T05-B	1	5.58E+04			5.58E+04	5.0E-01	1.1E+00	3.5E+00					VU ICP-OES	4/20/11 4:09 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1316-T01-C	1	2.42E+04			2.42E+04	5.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 4:10 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1316-T02-C	1	3.17E+04			3.17E+04	1.5E+00	1.1E+00	3.5E+00	1000	100	3.27E+04	101%	VU ICP-OES	4/20/11 4:12 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1316-T03-C	1	6.81E+02			6.81E+02	7.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 4:14 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1316-T04-C	1	3.57E+04			3.57E+04	8.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 4:15 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1316-T05-C	1	5.50E+04			5.50E+04	6.4E-01	1.1E+00	3.5E+00					VU ICP-OES	4/20/11 4:17 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1316-B01-A	1	5.50E-01	U1/2		5.50E-01	2.0E+01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1316-B01-B	1	2.34E+00	E		2.34E+00	1.9E+01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
Si	SWA-L09-1316-B01-C	1	5.50E-01	U1/2		5.50E-01	1.5E+01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	SWA-L09-1316-T01-A	1	4.68E+05			4.68E+05	1.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 3:56 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1316-T02-A	1	5.70E+05			5.70E+05	2.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 4:19 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1316-T03-A	1	6.62E+05			6.62E+05	3.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 3:57 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1316-T04-A	1	6.95E+05			6.95E+05	8.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 3:59 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1316-T05-A	1	6.69E+05			6.69E+05	2.3E+00	2.5E+00	8.0E+00					VU ICP-OES	4/20/11 4:01 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1316-T01-B	1	4.64E+05			4.64E+05	7.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 4:02 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1316-T02-B	1	5.72E+05			5.72E+05	1.8E-01	2.5E+00	8.0E+00	1000	100	5.72E+05	90%	VU ICP-OES	4/20/11 4:04 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1316-T03-B	1	6.71E+05			6.71E+05	1.0E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 4:05 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1316-T04-B	1	6.96E+05			6.96E+05	2.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 4:07 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1316-T05-B	1	6.71E+05			6.71E+05	2.3E+00	2.5E+00	8.0E+00					VU ICP-OES	4/20/11 4:09 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1316-T01-C	1	4.72E+05			4.72E+05	4.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 4:10 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1316-T02-C	1	5.68E+05			5.68E+05	2.3E-01	2.5E+00	8.0E+00	1000	100	5.69E+05	91%	VU ICP-OES	4/20/11 4:12 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1316-T03-C	1	6.68E+05			6.68E+05	9.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 4:14 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1316-T04-C	1	6.90E+05			6.90E+05	1.6E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 4:15 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1316-T05-C	1	7.01E+05			7.01E+05	2.1E+00	2.5E+00	8.0E+00					VU ICP-OES	4/20/11 4:17 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1316-B01-A	1	3.14E+01			3.14E+01	7.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1316-B01-B	1	3.32E+01			3.32E+01	3.4E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
Na	SWA-L09-1316-B01-C	1	2.90E+01			2.90E+01	5.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	SWA-L09-1316-T01-A	1	4.20E+02			4.20E+02	9.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:23 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L09-1316-T02-A	1	3.59E+02			3.59E+02	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:25 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L09-1316-T03-A	1	2.29E+02			2.29E+02	7.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:27 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L09-1316-T04-A	1	3.57E+02			3.57E+02	6.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:30 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L09-1316-T05-A	1	4.72E+02			4.72E+02	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	5/23/11 4:32 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L09-1316-T01-B	1	4.15E+02			4.15E+02	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:34 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L09-1316-T02-B	1	3.72E+02			3.72E+02	3.4E-01	1.0E+00	3.2E+00	1000	100	1.29E+03	92%	VU ICP-OES	5/23/11 4:36 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L09-1316-T03-B	1	2.57E+02			2.57E+02	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:39 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L09-1316-T04-B	1	3.69E+02			3.69E+02	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:41 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L09-1316-T05-B	1	4.22E+02			4.22E+02	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	5/23/11 4:43 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L09-1316-T01-C	1	4.27E+02			4.27E+02	6.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:45 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L09-1316-T02-C	1	3.55E+02			3.55E+02	5.9E-01	1.0E+00	3.2E+00	1000	100	1.34E+03	98%	VU ICP-OES	5/23/11 4:48 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L09-1316-T03-C	1	2.08E+02			2.08E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:50 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L09-1316-T04-C	1	3.44E+02			3.44E+02	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 4:52 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L09-1316-T05-C	1	5.00E+02			5.00E+02	3.3E-01	1.0E+00	3.2E+00					VU ICP-OES	5/23/11 4:55 PM	EPA Interlab 1316 SWA Reruns
Sr	SWA-L09-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	4.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1316-B01-B	1	5.00E-01	U1/2		5.00E-01	1.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
Sr	SWA-L09-1316-B01-C	1	5.00E-01	U1/2		5.00E-01	4.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	SWA-L09-1316-T01-A	1	3.70E+05			3.70E+05	7.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:56 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1316-T02-A	1	5.81E+05			5.81E+05	2.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 4:19 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1316-T03-A	1	1.13E+06			1.13E+06	4.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:57 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1316-T04-A	1	2.06E+06			2.06E+06	4.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:59 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1316-T05-A	1	4.26E+06			4.26E+06	7.7E-01	6.8E+00	2.2E+01					VU ICP-OES	4/20/11 4:01 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1316-T01-B	1	4.25E+05			4.25E+05	3.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 4:02 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1316-T02-B	1	6.67E+05			6.67E+05	1.5E-01	6.8E+00	2.2E+01	1000	100	7.65E+05	98%	VU ICP-OES	4/20/11 4:04 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1316-T03-B	1	1.17E+06			1.17E+06	1.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 4:05 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1316-T04-B	1	2.06E+06			2.06E+06	7.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 4:07 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1316-T05-B	1	3.83E+06			3.83E+06	6.0E-01	6.8E+00	2.2E+01					VU ICP-OES	4/20/11 4:09 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1316-T01-C	1	4.45E+05			4.45E+05	3.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 4:10 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1316-T02-C	1	5.73E+05			5.73E+05	5.1E-01	6.8E+00	2.2E+01	1000	100	6.58E+05	86%	VU ICP-OES	4/20/11 4:12 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1316-T03-C	1	1.09E+06			1.09E+06	3.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 4:14 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1316-T04-C	1	2.16E+06			2.16E+06	9.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 4:15 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1316-T05-C	1	3.94E+06			3.94E+06	6.2E-01	6.8E+00	2.2E+01					VU ICP-OES	4/20/11 4:17 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1316-B01-A	1	7.31E+01			7.31E+01	9.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1316-B01-B	1	9.58E+01			9.58E+01	2.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
S	SWA-L09-1316-B01-C	1	6.04E+01			6.04E+01	1.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	SWA-L09-1316-T01-A	1	2.30E+00	U1/2		2.30E+00	7.5E+02	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 3:56 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1316-T02-A	1	2.30E+00	U1/2		2.30E+00	2.8E+02	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 4:19 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1316-T03-A	1	2.30E+00	U1/2		2.30E+00	5.4E+02	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 3:57 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1316-T04-A	1	2.30E+00	U1/2		2.30E+00	5.1E+02	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 3:59 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1316-T05-A	1	2.30E+00	U1/2		2.30E+00	6.2E+01	4.6E+00	1.5E+01					VU ICP-OES	4/20/11 4:01 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1316-T01-B	1	2.30E+00	U1/2		2.30E+00	7.0E+00	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 4:02 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1316-T02-B	1	2.30E+00	U1/2		2.30E+00	2.1E+02	4.6E+00	1.5E+01	10	100	9.12E+02	91%	VU ICP-OES	4/20/11 4:04 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1316-T03-B	1	2.30E+00	U1/2		2.30E+00	3.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 4:05 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1316-T04-B	1	2.30E+00	U1/2		2.30E+00	3.2E+00	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 4:07 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1316-T05-B	1	2.30E+00	U1/2		2.30E+00	8.2E+01	4.6E+00	1.5E+01					VU ICP-OES	4/20/11 4:09 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1316-T01-C	1	2.30E+00	U1/2		2.30E+00	1.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 4:10 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1316-T02-C	1	2.30E+00	U1/2		2.30E+00	3.1E+05	4.6E+00	1.5E+01	10	100	8.73E+02	87%	VU ICP-OES	4/20/11 4:12 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1316-T03-C	1	2.30E+00	U1/2		2.30E+00	9.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 4:14 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1316-T04-C	1	2.30E+00	U1/2		2.30E+00	1.8E+02	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 4:15 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1316-T05-C	1	2.30E+00	U1/2		2.30E+00	6.5E+01	4.6E+00	1.5E+01					VU ICP-OES	4/20/11 4:17 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1316-B01-A	1	2.30E+00	U1/2		2.30E+00	8.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1316-B01-B	1	2.30E+00	U1/2		2.30E+00	2.7E+02	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
Tl	SWA-L09-1316-B01-C	1	2.30E+00	U1/2		2.30E+00	6.9E+02	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	SWA-L09-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	4.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 3:56 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 4:19 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 3:57 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 3:59 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1316-T05-A	1	1.00E+00	U1/2		1.00E+00	8.7E+00	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 4:01 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 4:02 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00	10	100	1.02E+03	101%	VU ICP-OES	4/20/11 4:04 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 4:05 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 4:07 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1316-T05-B	1	1.00E+00	U1/2		1.00E+00	2.1E+01	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 4:09 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 4:10 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00	10	100	1.04E+03	104%	VU ICP-OES	4/20/11 4:12 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	3.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 4:14 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	4.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 4:15 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1316-T05-C	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00					VU ICP-OES	4/20/11 4:17 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	4.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1316-B01-B	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
Ti	SWA-L09-1316-B01-C	1	1.00E+00	U1/2		1.00E+00	8.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	SWA-L09-1316-T01-A	1	2.98E+02			2.98E+02	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 3:56 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1316-T02-A	1	5.23E+02			5.23E+02	9.1E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 4:19 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1316-T03-A	1	9.54E+02			9.54E+02	5.0E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 3:57 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1316-T04-A	1	1.92E+03			1.92E+03	8.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 3:59 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1316-T05-A	1	3.84E+03			3.84E+03	4.2E-01	1.5E+00	4.8E+00					VU ICP-OES	4/20/11 4:01 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1316-T01-B	1	2.34E+02			2.34E+02	9.6E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 4:02 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1316-T02-B	1	5.01E+02			5.01E+02	1.4E+00	1.5E+00	4.8E+00	10	100	1.52E+03	102%	VU ICP-OES	4/20/11 4:04 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1316-T03-B	1	9.41E+02			9.41E+02	3.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 4:05 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1316-T04-B	1	1.85E+03			1.85E+03	4.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 4:07 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1316-T05-B	1	3.63E+03			3.63E+03	9.0E-01	1.5E+00	4.8E+00					VU ICP-OES	4/20/11 4:09 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1316-T01-C	1	3.03E+02			3.03E+02	1.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 4:10 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1316-T02-C	1	5.21E+02			5.21E+02	8.4E-01	1.5E+00	4.8E+00	10	100	1.46E+03	94%	VU ICP-OES	4/20/11 4:12 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1316-T03-C	1	8.91E+02			8.91E+02	3.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 4:14 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1316-T04-C	1	1.99E+03			1.99E+03	6.6E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 4:15 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1316-T05-C	1	3.54E+03			3.54E+03	4.6E-01	1.5E+00	4.8E+00					VU ICP-OES	4/20/11 4:17 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1316-B01-A	1	1.53E+00	E		1.53E+00	2.9E+01	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1316-B01-B	1	7.50E-01	U1/2		7.50E-01	5.3E+01	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
V	SWA-L09-1316-B01-C	1	7.50E-01	U1/2		7.50E-01	1.1E+01	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	SWA-L09-1316-T01-A	1	4.35E+00			4.35E+00	4.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:56 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1316-T02-A	1	4.82E+00			4.82E+00	4.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:19 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1316-T03-A	1	5.00E-01	U1/2		5.00E-01	5.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:57 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1316-T04-A	1	3.85E+00			3.85E+00	1.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:59 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1316-T05-A	1	2.18E+01			2.18E+01	2.6E+00	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 4:01 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1316-T01-B	1	3.94E+00			3.94E+00	7.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:02 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1316-T02-B	1	4.97E+00			4.97E+00	3.5E+00	1.0E+00	3.2E+00	10	100	1.04E+03	104%	VU ICP-OES	4/20/11 4:04 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1316-T03-B	1	5.00E-01	U1/2		5.00E-01	1.8E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:05 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1316-T04-B	1	3.57E+00			3.57E+00	1.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:07 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1316-T05-B	1	2.17E+01			2.17E+01	1.5E+00	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 4:09 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1316-T01-C	1	4.40E+00			4.40E+00	1.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:10 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1316-T02-C	1	5.06E+00			5.06E+00	5.2E+00	1.0E+00	3.2E+00	10	100	1.08E+03	107%	VU ICP-OES	4/20/11 4:12 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1316-T03-C	1	5.00E-01	U1/2		5.00E-01	6.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:14 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1316-T04-C	1	3.77E+00			3.77E+00	9.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 4:15 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1316-T05-C	1	2.19E+01			2.19E+01	4.1E-01	1.0E+00	3.2E+00					VU ICP-OES	4/20/11 4:17 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1316-B01-A	1	3.11E+00	E		3.11E+00	5.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:51 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1316-B01-B	1	2.31E+00	E		2.31E+00	4.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:52 PM	EPA Interlab L09 1313-1316 SWA
Zn	SWA-L09-1316-B01-C	1	5.00E-01	U1/2		5.00E-01	1.1E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 3:54 PM	EPA Interlab L09 1313-1316 SWA

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	SWA-L10-1316-T01-A	1	3.59E+04			3.59E+04	5.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1316-T02-A	1	5.56E+04			5.56E+04	9.3E-01	1.0E+00	3.2E+00	1000	100	5.66E+04	92%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1316-T03-A	1	1.10E+05			1.10E+05	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1316-T04-A	1	1.76E+05			1.76E+05	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1316-T01-B	1	3.53E+04			3.53E+04	9.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1316-T02-B	1	5.58E+04			5.58E+04	7.4E-01	1.0E+00	3.2E+00	1000	100	5.68E+04	97%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1316-T03-B	1	1.10E+05			1.10E+05	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1316-T04-B	1	1.76E+05			1.76E+05	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1316-T01-C	1	3.38E+04			3.38E+04	7.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1316-T02-C	1	5.68E+04			5.68E+04	5.0E-01	1.0E+00	3.2E+00	1000	100	5.78E+04	103%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1316-T03-C	1	1.15E+05			1.15E+05	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1316-T04-C	1	1.76E+05			1.76E+05	2.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	9.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1316-B03-B	1	5.00E-01	U1/2		5.00E-01	1.2E+02	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
Al	SWA-L10-1316-B03-C	1	5.00E-01	U1/2		5.00E-01	7.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	SWA-L10-1316-T01-A	1	5.72E+03			5.72E+03	2.3E-01	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1316-T02-A	1	6.55E+03			6.55E+03	6.8E-01	7.5E+00	2.4E+01	10	125	7.81E+03	101%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1316-T03-A	1	8.38E+03			8.38E+03	2.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1316-T04-A	1	8.09E+03			8.09E+03	1.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1316-T01-B	1	5.48E+03			5.48E+03	1.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1316-T02-B	1	6.81E+03			6.81E+03	5.0E-01	7.5E+00	2.4E+01	10	125	7.95E+03	92%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1316-T03-B	1	8.38E+03			8.38E+03	9.9E-01	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1316-T04-B	1	7.96E+03			7.96E+03	7.3E-01	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1316-T01-C	1	5.69E+03			5.69E+03	3.5E-01	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1316-T02-C	1	6.97E+03			6.97E+03	7.0E-01	7.5E+00	2.4E+01	10	125	8.13E+03	92%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1316-T03-C	1	8.47E+03			8.47E+03	1.4E+00	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1316-T04-C	1	8.20E+03			8.20E+03	2.3E-01	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1316-B03-A	1	3.75E+00	U1/2		3.75E+00	8.9E+01	7.5E+00	2.4E+01				---	VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1316-B03-B	1	3.75E+00	U1/2		3.75E+00	7.0E+01	7.5E+00	2.4E+01					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
Sb	SWA-L10-1316-B03-C	1	3.75E+00	U1/2		3.75E+00	9.8E+01	7.5E+00	2.4E+01					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	SWA-L10-1316-T01-A	1	5.30E+03			5.30E+03	6.0E-01	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1316-T02-A	1	1.22E+04			1.22E+04	4.2E-01	1.1E+01	3.5E+01	10	125	1.34E+04	92%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1316-T03-A	1	4.80E+04			4.80E+04	2.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1316-T04-A	1	1.20E+05			1.20E+05	2.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1316-T01-B	1	4.87E+03			4.87E+03	1.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1316-T02-B	1	1.30E+04			1.30E+04	2.2E-01	1.1E+01	3.5E+01	10	125	1.42E+04	90%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1316-T03-B	1	4.95E+04			4.95E+04	1.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1316-T04-B	1	1.25E+05			1.25E+05	6.4E-01	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1316-T01-C	1	5.22E+03			5.22E+03	9.6E-01	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1316-T02-C	1	1.35E+04			1.35E+04	8.4E-01	1.1E+01	3.5E+01	10	125	1.48E+04	101%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1316-T03-C	1	4.99E+04			4.99E+04	7.6E-01	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1316-T04-C	1	1.31E+05			1.31E+05	9.2E-01	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1316-B03-A	1	5.50E+00	U1/2		5.50E+00	8.8E+02	1.1E+01	3.5E+01				---	VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1316-B03-B	1	5.50E+00	U1/2		5.50E+00	2.1E+01	1.1E+01	3.5E+01					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
As	SWA-L10-1316-B03-C	1	5.50E+00	U1/2		5.50E+00	2.9E+01	1.1E+01	3.5E+01					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	SWA-L10-1316-T01-A	1	1.07E+03			1.07E+03	2.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1316-T02-A	1	1.14E+03			1.14E+03	9.0E-01	1.0E+00	3.2E+00	1000	100	2.03E+03	88%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1316-T03-A	1	1.25E+03			1.25E+03	2.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1316-T04-A	1	9.61E+02			9.61E+02	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1316-T01-B	1	9.78E+02			9.78E+02	2.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1316-T02-B	1	1.04E+03			1.04E+03	1.3E+00	1.0E+00	3.2E+00	1000	100	1.95E+03	91%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1316-T03-B	1	9.38E+02			9.38E+02	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1316-T04-B	1	9.53E+02			9.53E+02	8.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1316-T01-C	1	1.08E+03			1.08E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1316-T02-C	1	1.15E+03			1.15E+03	6.2E-01	1.0E+00	3.2E+00	1000	100	2.07E+03	93%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1316-T03-C	1	1.22E+03			1.22E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1316-T04-C	1	9.55E+02			9.55E+02	4.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	2.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1316-B03-B	1	5.00E-01	U1/2		5.00E-01	9.3E+00	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
B	SWA-L10-1316-B03-C	1	5.00E-01	U1/2		5.00E-01	5.2E+00	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	SWA-L10-1316-T01-A	1	9.79E+01			9.79E+01	8.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1316-T02-A	1	1.38E+02			1.38E+02	6.8E-01	1.0E+00	3.2E+00	10	125	1.33E+03	95%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1316-T03-A	1	1.32E+02			1.32E+02	2.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1316-T04-A	1	8.29E+01			8.29E+01	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1316-T01-B	1	9.77E+01			9.77E+01	9.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1316-T02-B	1	1.14E+02			1.14E+02	3.6E-01	1.0E+00	3.2E+00	10	125	1.42E+03	104%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1316-T03-B	1	1.16E+02			1.16E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1316-T04-B	1	7.97E+01			7.97E+01	5.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1316-T01-C	1	9.78E+01			9.78E+01	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1316-T02-C	1	1.27E+02			1.27E+02	4.7E-01	1.0E+00	3.2E+00	10	125	1.36E+03	99%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1316-T03-C	1	1.20E+02			1.20E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1316-T04-C	1	1.05E+02			1.05E+02	5.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	3.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1316-B03-B	1	5.00E-01	U1/2		5.00E-01	5.2E+01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
Ba	SWA-L10-1316-B03-C	1	5.00E-01	U1/2		5.00E-01	8.8E+00	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	SWA-L10-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	1.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	5.8E+01	1.9E+00	6.0E+00	10	125	1.37E+03	110%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	1.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	6.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	2.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00	10	125	1.44E+03	115%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	4.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	8.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	2.1E+02	1.9E+00	6.0E+00	10	125	1.47E+03	118%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	2.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1316-B03-A	1	9.50E-01	U1/2		9.50E-01	2.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1316-B03-B	1	9.50E-01	U1/2		9.50E-01	2.3E+01	1.9E+00	6.0E+00					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
Be	SWA-L10-1316-B03-C	1	9.50E-01	U1/2		9.50E-01	8.7E+01	1.9E+00	6.0E+00					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	SWA-L10-1316-T01-A	1	1.10E+00	U1/2		1.10E+00	5.6E+01	2.2E+00	7.0E+00			---		VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1316-T02-A	1	1.10E+00	U1/2		1.10E+00	3.7E+02	2.2E+00	7.0E+00	10	125	1.25E+03	100%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1316-T03-A	1	1.10E+00	U1/2		1.10E+00	1.2E+01	2.2E+00	7.0E+00			---		VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1316-T04-A	1	1.10E+00	U1/2		1.10E+00	2.4E+01	2.2E+00	7.0E+00			---		VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1316-T01-B	1	1.10E+00	U1/2		1.10E+00	6.7E+01	2.2E+00	7.0E+00			---		VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1316-T02-B	1	1.10E+00	U1/2		1.10E+00	1.0E+02	2.2E+00	7.0E+00	10	125	1.39E+03	112%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1316-T03-B	1	1.10E+00	U1/2		1.10E+00	1.0E+03	2.2E+00	7.0E+00			---		VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1316-T04-B	1	1.10E+00	U1/2		1.10E+00	8.3E+01	2.2E+00	7.0E+00			---		VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1316-T01-C	1	1.10E+00	U1/2		1.10E+00	1.6E+01	2.2E+00	7.0E+00			---		VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1316-T02-C	1	1.10E+00	U1/2		1.10E+00	4.6E+02	2.2E+00	7.0E+00	10	125	1.36E+03	109%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1316-T03-C	1	1.10E+00	U1/2		1.10E+00	7.4E+02	2.2E+00	7.0E+00			---		VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1316-T04-C	1	1.10E+00	U1/2		1.10E+00	7.3E+03	2.2E+00	7.0E+00			---		VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1316-B03-A	1	1.10E+00	U1/2		1.10E+00	6.0E+01	2.2E+00	7.0E+00			---		VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1316-B03-B	1	1.10E+00	U1/2		1.10E+00	3.8E+02	2.2E+00	7.0E+00					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
Cd	SWA-L10-1316-B03-C	1	1.10E+00	U1/2		1.10E+00	2.7E+03	2.2E+00	7.0E+00					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	SWA-L10-1316-T01-A	1	1.29E+04			1.29E+04	9.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1316-T02-A	1	1.24E+04			1.24E+04	6.8E-01	2.6E+00	8.3E+00	1000	100	1.33E+04	92%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1316-T03-A	1	9.02E+03			9.02E+03	2.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1316-T04-A	1	6.17E+03			6.17E+03	1.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1316-T01-B	1	1.21E+04			1.21E+04	6.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1316-T02-B	1	1.15E+04			1.15E+04	6.0E-01	2.6E+00	8.3E+00	1000	100	1.24E+04	98%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1316-T03-B	1	8.67E+03			8.67E+03	9.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1316-T04-B	1	5.82E+03			5.82E+03	1.5E+00	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1316-T01-C	1	1.27E+04			1.27E+04	3.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1316-T02-C	1	1.24E+04			1.24E+04	8.2E-02	2.6E+00	8.3E+00	1000	100	1.35E+04	112%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1316-T03-C	1	9.11E+03			9.11E+03	1.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1316-T04-C	1	6.27E+03			6.27E+03	1.9E+00	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1316-B03-A	1	4.13E+02			4.13E+02	7.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1316-B03-B	1	3.99E+02			3.99E+02	1.2E+00	2.6E+00	8.3E+00					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
Ca	SWA-L10-1316-B03-C	1	4.10E+02			4.10E+02	3.9E+00	2.6E+00	8.3E+00					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	SWA-L10-1316-T01-A	1	8.52E+02			8.52E+02	3.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1316-T02-A	1	1.43E+03			1.43E+03	5.3E-01	1.2E+00	3.8E+00	10	125	2.79E+03	108%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1316-T03-A	1	1.92E+03			1.92E+03	1.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1316-T04-A	1	2.30E+03			2.30E+03	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1316-T01-B	1	8.27E+02			8.27E+02	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1316-T02-B	1	1.40E+03			1.40E+03	9.2E-01	1.2E+00	3.8E+00	10	125	2.80E+03	112%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1316-T03-B	1	1.90E+03			1.90E+03	5.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1316-T04-B	1	2.04E+03			2.04E+03	4.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1316-T01-C	1	8.07E+02			8.07E+02	7.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1316-T02-C	1	1.48E+03			1.48E+03	8.1E-01	1.2E+00	3.8E+00	10	125	2.84E+03	109%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1316-T03-C	1	2.04E+03			2.04E+03	8.3E-01	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1316-T04-C	1	1.84E+03			1.84E+03	7.2E-02	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1316-B03-A	1	6.00E-01	U1/2		6.00E-01	3.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1316-B03-B	1	6.00E-01	U1/2		6.00E-01	1.2E+02	1.2E+00	3.8E+00					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
Cr	SWA-L10-1316-B03-C	1	6.00E-01	U1/2		6.00E-01	4.2E+01	1.2E+00	3.8E+00					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	SWA-L10-1316-T01-A	1	9.00E-01	U1/2		9.00E-01	1.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1316-T02-A	1	9.00E-01	U1/2		9.00E-01	1.8E+01	1.8E+00	5.7E+00	10	125	1.17E+03	93%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1316-T03-A	1	3.85E+00	E		3.85E+00	6.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1316-T04-A	1	6.53E+00			6.53E+00	6.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1316-T01-B	1	9.00E-01	U1/2		9.00E-01	3.7E+01	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1316-T02-B	1	9.00E-01	U1/2		9.00E-01	1.6E+02	1.8E+00	5.7E+00	10	125	1.39E+03	111%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1316-T03-B	1	3.21E+00	E		3.21E+00	3.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1316-T04-B	1	6.51E+00			6.51E+00	1.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1316-T01-C	1	9.00E-01	U1/2		9.00E-01	3.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1316-T02-C	1	9.00E-01	U1/2		9.00E-01	3.3E+01	1.8E+00	5.7E+00	10	125	1.38E+03	110%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1316-T03-C	1	2.99E+00	E		2.99E+00	9.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1316-T04-C	1	5.29E+00	E		5.29E+00	2.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1316-B03-A	1	9.00E-01	U1/2		9.00E-01	1.6E+02	1.8E+00	5.7E+00				---	VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1316-B03-B	1	9.00E-01	U1/2		9.00E-01	1.3E+03	1.8E+00	5.7E+00					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
Co	SWA-L10-1316-B03-C	1	9.00E-01	U1/2		9.00E-01	3.3E+01	1.8E+00	5.7E+00					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	SWA-L10-1316-T01-A	1	1.85E+00	U1/2		1.85E+00	1.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1316-T02-A	1	6.20E+00	E		6.20E+00	1.7E-01	3.7E+00	1.2E+01	10	125	1.24E+03	99%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1316-T03-A	1	2.63E+01			2.63E+01	3.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1316-T04-A	1	5.22E+01			5.22E+01	2.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1316-T01-B	1	1.85E+00	U1/2		1.85E+00	2.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1316-T02-B	1	8.41E+00	E		8.41E+00	8.5E+00	3.7E+00	1.2E+01	10	125	1.31E+03	104%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1316-T03-B	1	2.59E+01			2.59E+01	6.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1316-T04-B	1	4.61E+01			4.61E+01	1.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1316-T01-C	1	1.85E+00	U1/2		1.85E+00	2.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1316-T02-C	1	5.86E+00	E		5.86E+00	6.9E+00	3.7E+00	1.2E+01	10	125	1.35E+03	107%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1316-T03-C	1	3.19E+01			3.19E+01	2.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1316-T04-C	1	5.90E+01			5.90E+01	1.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1316-B03-A	1	1.85E+00	U1/2		1.85E+00	3.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1316-B03-B	1	1.85E+00	U1/2		1.85E+00	2.4E+01	3.7E+00	1.2E+01					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
Cu	SWA-L10-1316-B03-C	1	1.85E+00	U1/2		1.85E+00	8.7E+00	3.7E+00	1.2E+01					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	SWA-L10-1316-T01-A	1	6.89E+01			6.89E+01	5.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1316-T02-A	1	1.37E+02			1.37E+02	4.1E-01	2.0E+00	6.4E+00	1000	100	1.28E+03	114%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1316-T03-A	1	5.12E+02			5.12E+02	2.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1316-T04-A	1	1.16E+03			1.16E+03	1.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1316-T01-B	1	5.91E+01			5.91E+01	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1316-T02-B	1	1.40E+02			1.40E+02	9.0E-01	2.0E+00	6.4E+00	1000	100	1.32E+03	118%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1316-T03-B	1	5.23E+02			5.23E+02	4.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1316-T04-B	1	1.23E+03			1.23E+03	1.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1316-T01-C	1	5.03E+01			5.03E+01	2.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1316-T02-C	1	1.57E+02			1.57E+02	5.0E-01	2.0E+00	6.4E+00	1000	100	1.30E+03	115%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1316-T03-C	1	5.20E+02			5.20E+02	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1316-T04-C	1	1.16E+03			1.16E+03	4.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	7.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1316-B03-B	1	1.00E+00	U1/2		1.00E+00	6.2E+02	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
Fe	SWA-L10-1316-B03-C	1	3.38E+00	E		3.38E+00	2.1E+00	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	SWA-L10-1316-T01-A	1	1.21E+01	E		1.21E+01	2.0E+00	6.8E+00	2.2E+01			---		VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1316-T02-A	1	2.43E+01			2.43E+01	1.6E+00	6.8E+00	2.2E+01	10	125	1.26E+03	99%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1316-T03-A	1	1.06E+02			1.06E+02	2.1E+01	6.8E+00	2.2E+01			---		VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1316-T04-A	1	2.04E+02			2.04E+02	2.9E+01	6.8E+00	2.2E+01			---		VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1316-T01-B	1	1.17E+01	E		1.17E+01	1.4E+02	6.8E+00	2.2E+01			---		VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1316-T02-B	1	3.29E+01			3.29E+01	7.0E+00	6.8E+00	2.2E+01	10	125	1.36E+03	106%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1316-T03-B	1	1.15E+02			1.15E+02	5.6E+00	6.8E+00	2.2E+01			---		VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1316-T04-B	1	2.09E+02			2.09E+02	3.5E+00	6.8E+00	2.2E+01			---		VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1316-T01-C	1	1.16E+01	E		1.16E+01	6.2E+01	6.8E+00	2.2E+01			---		VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1316-T02-C	1	3.12E+01			3.12E+01	1.1E+01	6.8E+00	2.2E+01	10	125	1.29E+03	101%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1316-T03-C	1	1.08E+02			1.08E+02	6.5E+00	6.8E+00	2.2E+01			---		VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1316-T04-C	1	2.28E+02			2.28E+02	3.2E+00	6.8E+00	2.2E+01			---		VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1316-B03-A	1	7.47E+00	E		7.47E+00	4.9E+01	6.8E+00	2.2E+01			---		VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1316-B03-B	1	3.40E+00	U1/2		3.40E+00	5.3E+01	6.8E+00	2.2E+01					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
Pb	SWA-L10-1316-B03-C	1	3.40E+00	U1/2		3.40E+00	1.1E+02	6.8E+00	2.2E+01					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	SWA-L10-1316-T01-A	1	2.44E+00	E		2.44E+00	1.7E+01	1.9E+00	6.0E+00			---		VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1316-T02-A	1	5.69E+00	E		5.69E+00	5.0E+00	1.9E+00	6.0E+00	10	125	1.06E+03	84%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1316-T03-A	1	8.21E+00			8.21E+00	5.5E+00	1.9E+00	6.0E+00			---		VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1316-T04-A	1	9.46E+00			9.46E+00	9.7E+00	1.9E+00	6.0E+00			---		VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1316-T01-B	1	2.05E+00	E		2.05E+00	1.6E+01	1.9E+00	6.0E+00			---		VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1316-T02-B	1	5.30E+00	E		5.30E+00	8.7E+00	1.9E+00	6.0E+00	10	125	1.10E+03	87%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1316-T03-B	1	7.86E+00			7.86E+00	4.3E+00	1.9E+00	6.0E+00			---		VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1316-T04-B	1	1.10E+01			1.10E+01	7.3E+00	1.9E+00	6.0E+00			---		VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1316-T01-C	1	2.03E+00	E		2.03E+00	1.6E+00	1.9E+00	6.0E+00			---		VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1316-T02-C	1	4.67E+00	E		4.67E+00	1.8E+01	1.9E+00	6.0E+00	10	125	1.11E+03	89%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1316-T03-C	1	8.35E+00			8.35E+00	8.5E+00	1.9E+00	6.0E+00			---		VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1316-T04-C	1	1.07E+01			1.07E+01	3.1E+00	1.9E+00	6.0E+00			---		VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1316-B03-A	1	9.50E-01	U1/2		9.50E-01	2.6E+04	1.9E+00	6.0E+00			---		VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1316-B03-B	1	9.50E-01	U1/2		9.50E-01	6.7E+01	1.9E+00	6.0E+00					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
Li	SWA-L10-1316-B03-C	1	9.50E-01	U1/2		9.50E-01	6.7E+01	1.9E+00	6.0E+00					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	SWA-L10-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	1.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	7.0E+00	2.0E+00	6.4E+00	10	125	1.18E+03	94%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00			---		VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1316-T04-A	1	2.96E+00	E		2.96E+00	4.5E+01	2.0E+00	6.4E+00			---		VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	7.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00	10	125	1.36E+03	109%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	6.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1316-T04-B	1	2.63E+00	E		2.63E+00	2.1E+00	2.0E+00	6.4E+00			---		VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	6.1E+02	2.0E+00	6.4E+00			---		VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00	10	125	1.32E+03	106%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00			---		VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1316-T04-C	1	3.37E+00	E		3.37E+00	1.7E+00	2.0E+00	6.4E+00			---		VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00			---		VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1316-B03-B	1	1.00E+00	U1/2		1.00E+00	9.9E+01	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
Mn	SWA-L10-1316-B03-C	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	SWA-L10-1316-T01-A	1	1.05E+01			1.05E+01	2.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1316-T02-A	1	1.11E+01			1.11E+01	1.1E+02	1.0E+00	3.2E+00	1000	100	1.15E+03	114%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1316-T03-A	1	1.66E+01			1.66E+01	1.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1316-T04-A	1	3.30E+01			3.30E+01	7.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1316-T01-B	1	7.91E+00			7.91E+00	8.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1316-T02-B	1	1.51E+01			1.51E+01	5.2E+01	1.0E+00	3.2E+00	1000	100	1.19E+03	117%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1316-T03-B	1	1.86E+01			1.86E+01	1.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1316-T04-B	1	2.03E+01			2.03E+01	2.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1316-T01-C	1	1.10E+01			1.10E+01	8.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1316-T02-C	1	1.29E+01			1.29E+01	1.1E+02	1.0E+00	3.2E+00	1000	100	1.10E+03	109%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1316-T03-C	1	2.37E+01			2.37E+01	2.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1316-T04-C	1	2.61E+01			2.61E+01	6.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	7.3E+02	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1316-B03-B	1	5.00E-01	U1/2		5.00E-01	8.8E+02	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
Mg	SWA-L10-1316-B03-C	1	5.00E-01	U1/2		5.00E-01	5.1E+01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	SWA-L10-1316-T01-A	1	1.45E+02			1.45E+02	2.0E-01	1.2E+00	3.8E+00			---		VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1316-T02-A	1	2.45E+02			2.45E+02	5.3E-01	1.2E+00	3.8E+00	10	125	1.30E+03	84%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1316-T03-A	1	6.18E+02			6.18E+02	1.4E+00	1.2E+00	3.8E+00			---		VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1316-T04-A	1	1.21E+03			1.21E+03	3.0E+00	1.2E+00	3.8E+00			---		VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1316-T01-B	1	1.32E+02			1.32E+02	3.1E+00	1.2E+00	3.8E+00			---		VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1316-T02-B	1	2.52E+02			2.52E+02	3.5E-01	1.2E+00	3.8E+00	10	125	1.36E+03	89%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1316-T03-B	1	6.21E+02			6.21E+02	9.5E-01	1.2E+00	3.8E+00			---		VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1316-T04-B	1	1.27E+03			1.27E+03	4.8E-01	1.2E+00	3.8E+00			---		VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1316-T01-C	1	1.40E+02			1.40E+02	9.4E-01	1.2E+00	3.8E+00			---		VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1316-T02-C	1	2.60E+02			2.60E+02	9.4E-01	1.2E+00	3.8E+00	10	125	1.39E+03	90%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1316-T03-C	1	6.03E+02			6.03E+02	1.3E+00	1.2E+00	3.8E+00			---		VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1316-T04-C	1	1.24E+03			1.24E+03	3.2E-01	1.2E+00	3.8E+00			---		VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1316-B03-A	1	2.02E+00	E		2.02E+00	3.6E+01	1.2E+00	3.8E+00			---		VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1316-B03-B	1	2.36E+00	E		2.36E+00	7.2E+01	1.2E+00	3.8E+00					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
Mo	SWA-L10-1316-B03-C	1	2.81E+00	E		2.81E+00	4.8E+01	1.2E+00	3.8E+00					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	SWA-L10-1316-T01-A	1	9.00E-01	U1/2		9.00E-01	3.5E+01	1.8E+00	5.7E+00			---		VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1316-T02-A	1	9.00E-01	U1/2		9.00E-01	1.1E+01	1.8E+00	5.7E+00	10	125	1.25E+03	100%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1316-T03-A	1	6.28E+00			6.28E+00	5.8E+01	1.8E+00	5.7E+00			---		VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1316-T04-A	1	8.94E+00			8.94E+00	8.7E+01	1.8E+00	5.7E+00			---		VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1316-T01-B	1	9.00E-01	U1/2		9.00E-01	2.1E+02	1.8E+00	5.7E+00			---		VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1316-T02-B	1	9.00E-01	U1/2		9.00E-01	2.7E+02	1.8E+00	5.7E+00	10	125	1.38E+03	110%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1316-T03-B	1	7.31E+00			7.31E+00	7.2E+01	1.8E+00	5.7E+00			---		VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1316-T04-B	1	9.38E+00			9.38E+00	5.1E+01	1.8E+00	5.7E+00			---		VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1316-T01-C	1	9.00E-01	U1/2		9.00E-01	1.0E+04	1.8E+00	5.7E+00			---		VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1316-T02-C	1	9.00E-01	U1/2		9.00E-01	7.6E+01	1.8E+00	5.7E+00	10	125	1.31E+03	105%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1316-T03-C	1	5.26E+00	E		5.26E+00	2.9E+01	1.8E+00	5.7E+00			---		VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1316-T04-C	1	7.53E+00			7.53E+00	6.0E+01	1.8E+00	5.7E+00			---		VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1316-B03-A	1	9.00E-01	U1/2		9.00E-01	1.8E+02	1.8E+00	5.7E+00			---		VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1316-B03-B	1	9.00E-01	U1/2		9.00E-01	5.0E+01	1.8E+00	5.7E+00					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
Ni	SWA-L10-1316-B03-C	1	9.00E-01	U1/2		9.00E-01	5.5E+03	1.8E+00	5.7E+00					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	SWA-L10-1316-T01-A	1	8.66E+01			8.66E+01	8.4E-01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1316-T02-A	1	1.35E+02			1.35E+02	2.3E+00	3.7E+00	1.2E+01	1000	100	1.23E+03	109%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1316-T03-A	1	4.93E+02			4.93E+02	4.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1316-T04-A	1	1.58E+03			1.58E+03	9.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1316-T01-B	1	7.12E+01			7.12E+01	7.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1316-T02-B	1	1.67E+02			1.67E+02	7.9E+00	3.7E+00	1.2E+01	1000	100	1.29E+03	113%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1316-T03-B	1	4.91E+02			4.91E+02	1.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1316-T04-B	1	1.65E+03			1.65E+03	3.4E-01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1316-T01-C	1	7.51E+01			7.51E+01	4.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1316-T02-C	1	1.78E+02			1.78E+02	4.6E+00	3.7E+00	1.2E+01	1000	100	1.22E+03	105%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1316-T03-C	1	5.26E+02			5.26E+02	8.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1316-T04-C	1	1.80E+03			1.80E+03	6.3E-01	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1316-B03-A	1	7.42E+00	E		7.42E+00	2.4E+02	3.7E+00	1.2E+01				---	VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1316-B03-B	1	1.82E+01			1.82E+01	7.7E+01	3.7E+00	1.2E+01					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
P	SWA-L10-1316-B03-C	1	1.15E+01	E		1.15E+01	5.2E+01	3.7E+00	1.2E+01					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	SWA-L10-1316-T01-A	1	3.49E+05			3.49E+05	2.1E-01	1.6E+00	5.1E+00			---		VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1316-T02-A	1	5.37E+05			5.37E+05	3.1E+00	1.6E+00	5.1E+00	1000	100	5.38E+05	98%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1316-T03-A	1	1.06E+06			1.06E+06	3.3E+00	1.6E+00	5.1E+00			---		VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1316-T04-A	1	4.27E+06			4.27E+06	8.1E-01	1.6E+00	5.1E+00			---		VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1316-T01-B	1	3.45E+05			3.45E+05	8.4E-01	1.6E+00	5.1E+00			---		VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1316-T02-B	1	5.33E+05			5.33E+05	4.5E-01	1.6E+00	5.1E+00	1000	100	5.34E+05	103%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1316-T03-B	1	1.04E+06			1.04E+06	9.5E-01	1.6E+00	5.1E+00			---		VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1316-T04-B	1	4.29E+06			4.29E+06	2.1E-01	1.6E+00	5.1E+00			---		VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1316-T01-C	1	3.58E+05			3.58E+05	9.6E-01	1.6E+00	5.1E+00			---		VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1316-T02-C	1	5.43E+05			5.43E+05	1.0E+00	1.6E+00	5.1E+00	1000	100	5.44E+05	112%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1316-T03-C	1	1.05E+06			1.05E+06	3.3E+00	1.6E+00	5.1E+00			---		VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1316-T04-C	1	4.27E+06			4.27E+06	2.7E-01	1.6E+00	5.1E+00			---		VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1316-B03-A	1	3.57E+01			3.57E+01	1.5E+01	1.6E+00	5.1E+00			---		VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1316-B03-B	1	3.13E+01			3.13E+01	1.2E+00	1.6E+00	5.1E+00					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
K	SWA-L10-1316-B03-C	1	3.28E+01			3.28E+01	6.2E-01	1.6E+00	5.1E+00					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	SWA-L10-1316-T01-A	1	1.05E+05			1.05E+05	1.8E-01	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1316-T02-A	1	1.87E+05			1.87E+05	4.3E-01	1.5E+01	4.8E+01	10	125	1.88E+05	83%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1316-T03-A	1	4.55E+05			4.55E+05	2.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1316-T04-A	1	8.67E+05			8.67E+05	1.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1316-T01-B	1	9.79E+04			9.79E+04	1.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1316-T02-B	1	1.95E+05			1.95E+05	4.4E-01	1.5E+01	4.8E+01	10	125	1.96E+05	85%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1316-T03-B	1	4.62E+05			4.62E+05	9.5E-01	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1316-T04-B	1	9.19E+05			9.19E+05	3.4E-01	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1316-T01-C	1	1.04E+05			1.04E+05	9.1E-01	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1316-T02-C	1	2.02E+05			2.02E+05	5.8E-01	1.5E+01	4.8E+01	10	125	2.03E+05	84%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1316-T03-C	1	4.45E+05			4.45E+05	8.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1316-T04-C	1	9.00E+05			9.00E+05	4.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1316-B03-A	1	7.50E+00	U1/2		7.50E+00	2.4E+01	1.5E+01	4.8E+01				---	VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1316-B03-B	1	7.50E+00	U1/2		7.50E+00	1.6E+01	1.5E+01	4.8E+01					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
Se	SWA-L10-1316-B03-C	1	7.50E+00	U1/2		7.50E+00	1.1E+02	1.5E+01	4.8E+01					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	SWA-L10-1316-T01-A	1	2.53E+04			2.53E+04	1.9E+00	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1316-T02-A	1	3.09E+04			3.09E+04	2.0E+00	1.1E+00	3.5E+00	1000	100	3.19E+04	103%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1316-T03-A	1	4.64E+04			4.64E+04	4.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1316-T04-A	1	6.65E+04			6.65E+04	1.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1316-T01-B	1	2.27E+04			2.27E+04	8.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1316-T02-B	1	3.13E+04			3.13E+04	3.2E-01	1.1E+00	3.5E+00	1000	100	3.23E+04	106%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1316-T03-B	1	4.87E+04			4.87E+04	2.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1316-T04-B	1	6.43E+04			6.43E+04	2.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1316-T01-C	1	2.72E+04			2.72E+04	7.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1316-T02-C	1	3.23E+04			3.23E+04	2.2E-01	1.1E+00	3.5E+00	1000	100	3.33E+04	101%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1316-T03-C	1	5.11E+04			5.11E+04	5.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1316-T04-C	1	6.57E+04			6.57E+04	8.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1316-B03-A	1	5.23E+00			5.23E+00	4.9E+00	1.1E+00	3.5E+00				---	VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1316-B03-B	1	3.75E+00			3.75E+00	3.6E+01	1.1E+00	3.5E+00					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
Si	SWA-L10-1316-B03-C	1	3.73E+00			3.73E+00	1.8E+01	1.1E+00	3.5E+00					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	SWA-L10-1316-T01-A	1	4.90E+05			4.90E+05	4.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1316-T02-A	1	6.39E+05			6.39E+05	5.2E-01	2.5E+00	8.0E+00	1000	100	6.40E+05	94%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1316-T03-A	1	8.66E+05			8.66E+05	2.0E+00	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1316-T04-A	1	9.53E+05			9.53E+05	4.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1316-T01-B	1	4.91E+05			4.91E+05	6.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1316-T02-B	1	6.33E+05			6.33E+05	9.5E-01	2.5E+00	8.0E+00	1000	100	6.34E+05	104%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1316-T03-B	1	8.62E+05			8.62E+05	8.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1316-T04-B	1	9.73E+05			9.73E+05	4.0E+00	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1316-T01-C	1	5.01E+05			5.01E+05	5.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1316-T02-C	1	6.39E+05			6.39E+05	8.2E-01	2.5E+00	8.0E+00	1000	100	6.40E+05	93%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1316-T03-C	1	8.51E+05			8.51E+05	8.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1316-T04-C	1	9.54E+05			9.54E+05	6.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1316-B03-A	1	3.52E+01			3.52E+01	3.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1316-B03-B	1	2.44E+01			2.44E+01	1.3E+01	2.5E+00	8.0E+00					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
Na	SWA-L10-1316-B03-C	1	3.52E+01			3.52E+01	6.3E+00	2.5E+00	8.0E+00					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	SWA-L10-1316-T01-A	1	3.19E+02			3.19E+02	4.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1316-T02-A	1	3.77E+02			3.77E+02	3.8E-01	1.0E+00	3.2E+00	1000	100	1.45E+03	108%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1316-T03-A	1	4.19E+02			4.19E+02	2.1E+00	1.0E+00	3.2E+00			---		VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1316-T04-A	1	4.60E+02			4.60E+02	1.3E+00	1.0E+00	3.2E+00			---		VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1316-T01-B	1	3.10E+02			3.10E+02	7.1E-01	1.0E+00	3.2E+00			---		VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1316-T02-B	1	3.56E+02			3.56E+02	8.1E-01	1.0E+00	3.2E+00	1000	100	1.45E+03	109%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1316-T03-B	1	4.13E+02			4.13E+02	1.0E+00	1.0E+00	3.2E+00			---		VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1316-T04-B	1	4.53E+02			4.53E+02	7.6E-01	1.0E+00	3.2E+00			---		VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1316-T01-C	1	2.99E+02			2.99E+02	1.6E+00	1.0E+00	3.2E+00			---		VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1316-T02-C	1	3.65E+02			3.65E+02	1.2E+00	1.0E+00	3.2E+00	1000	100	1.40E+03	104%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1316-T03-C	1	3.96E+02			3.96E+02	6.0E-01	1.0E+00	3.2E+00			---		VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1316-T04-C	1	4.46E+02			4.46E+02	4.8E-01	1.0E+00	3.2E+00			---		VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	1.8E+02	1.0E+00	3.2E+00			---		VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1316-B03-B	1	5.00E-01	U1/2		5.00E-01	3.4E+01	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
Sr	SWA-L10-1316-B03-C	1	5.00E-01	U1/2		5.00E-01	1.1E+02	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	SWA-L10-1316-T01-A	1	3.47E+05			3.47E+05	6.8E-02	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1316-T02-A	1	6.13E+05			6.13E+05	3.2E-01	6.8E+00	2.2E+01	1000	100	6.14E+05	95%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1316-T03-A	1	1.17E+06			1.17E+06	2.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1316-T04-A	1	2.08E+06			2.08E+06	9.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1316-T01-B	1	3.28E+05			3.28E+05	7.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1316-T02-B	1	6.29E+05			6.29E+05	5.6E-01	6.8E+00	2.2E+01	1000	100	6.30E+05	93%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1316-T03-B	1	1.18E+06			1.18E+06	8.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1316-T04-B	1	2.15E+06			2.15E+06	3.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1316-T01-C	1	3.65E+05			3.65E+05	4.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1316-T02-C	1	6.52E+05			6.52E+05	9.1E-01	6.8E+00	2.2E+01	1000	100	6.53E+05	94%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1316-T03-C	1	1.16E+06			1.16E+06	9.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1316-T04-C	1	2.14E+06			2.14E+06	3.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1316-B03-A	1	3.03E+02			3.03E+02	9.8E+00	6.8E+00	2.2E+01				---	VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1316-B03-B	1	3.89E+02			3.89E+02	7.8E+00	6.8E+00	2.2E+01					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
S	SWA-L10-1316-B03-C	1	3.62E+02			3.62E+02	1.0E+01	6.8E+00	2.2E+01					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	SWA-L10-1316-T01-A	1	2.30E+00	U1/2		2.30E+00	2.1E+02	4.6E+00	1.5E+01			---		VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1316-T02-A	1	2.30E+00	U1/2		2.30E+00	1.2E+02	4.6E+00	1.5E+01	10	125	1.25E+03	100%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1316-T03-A	1	2.30E+00	U1/2		2.30E+00	2.0E+03	4.6E+00	1.5E+01			---		VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1316-T04-A	1	7.18E+00	E		7.18E+00	4.5E+01	4.6E+00	1.5E+01			---		VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1316-T01-B	1	2.30E+00	U1/2		2.30E+00	4.8E+01	4.6E+00	1.5E+01			---		VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1316-T02-B	1	2.30E+00	U1/2		2.30E+00	1.3E+02	4.6E+00	1.5E+01	10	125	1.29E+03	103%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1316-T03-B	1	2.30E+00	U1/2		2.30E+00	3.2E+02	4.6E+00	1.5E+01			---		VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1316-T04-B	1	8.66E+00	E		8.66E+00	6.0E+02	4.6E+00	1.5E+01			---		VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1316-T01-C	1	2.30E+00	U1/2		2.30E+00	2.4E+01	4.6E+00	1.5E+01			---		VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1316-T02-C	1	2.30E+00	U1/2		2.30E+00	3.3E+01	4.6E+00	1.5E+01	10	125	1.24E+03	99%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1316-T03-C	1	2.30E+00	U1/2		2.30E+00	1.6E+03	4.6E+00	1.5E+01			---		VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1316-T04-C	1	9.03E+00	E		9.03E+00	1.3E+02	4.6E+00	1.5E+01			---		VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1316-B03-A	1	2.30E+00	U1/2		2.30E+00	9.0E+01	4.6E+00	1.5E+01			---		VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1316-B03-B	1	2.30E+00	U1/2		2.30E+00	7.8E+01	4.6E+00	1.5E+01					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
Tl	SWA-L10-1316-B03-C	1	2.30E+00	U1/2		2.30E+00	8.6E+01	4.6E+00	1.5E+01					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	SWA-L10-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	4.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00	10	125	1.25E+03	100%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	6.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1316-T04-A	1	4.49E+00	E		4.49E+00	4.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	4.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	4.3E+03	2.0E+00	6.4E+00	10	125	1.34E+03	107%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1316-T04-B	1	2.34E+00	E		2.34E+00	1.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	1.0E+03	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	5.4E+03	2.0E+00	6.4E+00	10	125	1.39E+03	111%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	5.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1316-T04-C	1	3.11E+00	E		3.11E+00	9.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	8.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1316-B03-B	1	1.00E+00	U1/2		1.00E+00	3.6E+02	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
Ti	SWA-L10-1316-B03-C	1	1.00E+00	U1/2		1.00E+00	8.1E+01	2.0E+00	6.4E+00					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	SWA-L10-1316-T01-A	1	3.55E+02			3.55E+02	6.6E-01	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1316-T02-A	1	5.74E+02			5.74E+02	4.2E-01	1.5E+00	4.8E+00	10	125	1.73E+03	92%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1316-T03-A	1	1.26E+03			1.26E+03	1.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1316-T04-A	1	2.21E+03			2.21E+03	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1316-T01-B	1	3.33E+02			3.33E+02	8.6E-01	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1316-T02-B	1	6.02E+02			6.02E+02	6.4E-01	1.5E+00	4.8E+00	10	125	1.73E+03	90%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1316-T03-B	1	1.29E+03			1.29E+03	8.2E-01	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1316-T04-B	1	2.24E+03			2.24E+03	7.2E-01	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1316-T01-C	1	3.52E+02			3.52E+02	2.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1316-T02-C	1	6.17E+02			6.17E+02	3.5E-01	1.5E+00	4.8E+00	10	125	1.81E+03	95%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1316-T03-C	1	1.32E+03			1.32E+03	3.8E-01	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1316-T04-C	1	2.35E+03			2.35E+03	4.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1316-B03-A	1	7.50E-01	U1/2		7.50E-01	1.0E+03	1.5E+00	4.8E+00				---	VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1316-B03-B	1	7.50E-01	U1/2		7.50E-01	2.5E+03	1.5E+00	4.8E+00					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
V	SWA-L10-1316-B03-C	1	7.50E-01	U1/2		7.50E-01	2.4E+02	1.5E+00	4.8E+00					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	SWA-L10-1316-T01-A	1	5.00E-01	U1/2		5.00E-01	3.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:08 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1316-T02-A	1	3.08E+00	E		3.08E+00	1.2E+00	1.0E+00	3.2E+00	10	125	1.40E+03	112%	VU ICP-OES	12/8/10 1:10 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1316-T03-A	1	6.43E+00			6.43E+00	2.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:11 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1316-T04-A	1	1.77E+01			1.77E+01	3.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:13 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1316-T01-B	1	5.00E-01	U1/2		5.00E-01	6.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:15 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1316-T02-B	1	3.22E+00			3.22E+00	8.0E+00	1.0E+00	3.2E+00	10	125	1.45E+03	116%	VU ICP-OES	12/8/10 1:16 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1316-T03-B	1	9.08E+00			9.08E+00	3.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:18 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1316-T04-B	1	1.83E+01			1.83E+01	3.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:20 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1316-T01-C	1	5.00E-01	U1/2		5.00E-01	2.3E+02	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:21 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1316-T02-C	1	1.72E+00	E		1.72E+00	1.0E+00	1.0E+00	3.2E+00	10	125	1.47E+03	118%	VU ICP-OES	12/8/10 1:23 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1316-T03-C	1	9.89E+00			9.89E+00	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:25 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1316-T04-C	1	1.33E+01			1.33E+01	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:26 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1316-B03-A	1	1.90E+00	E		1.90E+00	1.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	12/8/10 1:03 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1316-B03-B	1	3.21E+00			3.21E+00	4.2E+00	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 1:05 PM	EPA Interlab L10 1313-1316 SWA
Zn	SWA-L10-1316-B03-C	1	8.36E+00			8.36E+00	3.4E+00	1.0E+00	3.2E+00					VU ICP-OES	12/8/10 1:06 PM	EPA Interlab L10 1313-1316 SWA

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	SWA-L11-1316-T01-A	1	3.30E+04			3.30E+04	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:09 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1316-T02-A	1	5.14E+04			5.14E+04	6.6E-01	1.0E+00	3.2E+00	1000	100	5.23E+04	91%	VU ICP-OES	4/7/11 5:11 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1316-T03-A	1	9.03E+04			9.03E+04	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:12 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1316-T04-A	1	1.38E+05			1.38E+05	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:14 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1316-T01-B	1	3.24E+04			3.24E+04	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:15 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1316-T02-B	1	5.13E+04			5.13E+04	9.0E-01	1.0E+00	3.2E+00	1000	100	5.23E+04	102%	VU ICP-OES	4/7/11 5:17 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1316-T03-B	1	8.66E+04			8.66E+04	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:19 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1316-T04-B	1	1.37E+05			1.37E+05	5.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:20 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1316-T01-C	1	3.42E+04			3.42E+04	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:22 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1316-T02-C	1	5.16E+04			5.16E+04	9.7E-01	1.0E+00	3.2E+00	1000	100	5.26E+04	94%	VU ICP-OES	4/7/11 5:24 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1316-T03-C	1	8.61E+04			8.61E+04	7.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:25 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1316-T04-C	1	1.32E+05			1.32E+05	1.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:27 PM	EPA Interlab L11 1313-1316 SWA
Al	SWA-L11-1316-B01-A	1	5.17E+00			5.17E+00	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	SWA-L11-1316-T01-A	1	4.86E+03			4.86E+03	9.5E-01	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 3:11 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L11-1316-T02-A	1	1.51E+03			1.51E+03	9.0E+00	7.5E+00	2.4E+01	10	100	2.38E+03	87%	VU ICP-OES	5/23/11 3:14 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L11-1316-T03-A	1	3.32E+03			3.32E+03	6.1E-01	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 3:16 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L11-1316-T04-A	1	6.38E+03			6.38E+03	8.2E-01	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 3:18 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L11-1316-T01-B	1	4.59E+03			4.59E+03	5.7E-01	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 3:21 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L11-1316-T02-B	1	1.59E+03			1.59E+03	7.6E+00	7.5E+00	2.4E+01	10	100	2.46E+03	88%	VU ICP-OES	5/23/11 3:23 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L11-1316-T03-B	1	3.76E+03			3.76E+03	2.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 3:25 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L11-1316-T04-B	1	6.37E+03			6.37E+03	6.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 3:28 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L11-1316-T01-C	1	4.74E+03			4.74E+03	2.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 3:31 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L11-1316-T02-C	1	1.74E+03			1.74E+03	1.1E+01	7.5E+00	2.4E+01	10	100	2.67E+03	93%	VU ICP-OES	5/23/11 3:33 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L11-1316-T03-C	1	3.26E+03			3.26E+03	1.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 3:35 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L11-1316-T04-C	1	6.35E+03			6.35E+03	3.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/23/11 3:38 PM	EPA Interlab 1316 SWA Reruns
Sb	SWA-L11-1316-B01-A	1	3.75E+00	U1/2		3.75E+00	1.8E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	SWA-L11-1316-T01-A	1	4.47E+03			4.47E+03	4.5E-01	1.1E+01	3.5E+01				---	VU ICP-OES	4/7/11 5:09 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1316-T02-A	1	1.19E+04			1.19E+04	1.0E+00	1.1E+01	3.5E+01	10	100	1.29E+04	99%	VU ICP-OES	4/7/11 5:11 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1316-T03-A	1	2.83E+04			2.83E+04	5.6E-01	1.1E+01	3.5E+01				---	VU ICP-OES	4/7/11 5:12 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1316-T04-A	1	6.49E+04			6.49E+04	1.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	4/7/11 5:14 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1316-T01-B	1	4.28E+03			4.28E+03	5.6E-01	1.1E+01	3.5E+01				---	VU ICP-OES	4/7/11 5:15 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1316-T02-B	1	1.17E+04			1.17E+04	1.2E+00	1.1E+01	3.5E+01	10	100	1.27E+04	95%	VU ICP-OES	4/7/11 5:17 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1316-T03-B	1	2.81E+04			2.81E+04	1.7E+00	1.1E+01	3.5E+01				---	VU ICP-OES	4/7/11 5:19 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1316-T04-B	1	5.55E+04			5.55E+04	4.6E-01	1.1E+01	3.5E+01				---	VU ICP-OES	4/7/11 5:20 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1316-T01-C	1	4.74E+03			4.74E+03	5.8E-01	1.1E+01	3.5E+01				---	VU ICP-OES	4/7/11 5:22 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1316-T02-C	1	1.19E+04			1.19E+04	1.0E+00	1.1E+01	3.5E+01	10	100	1.29E+04	93%	VU ICP-OES	4/7/11 5:24 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1316-T03-C	1	2.56E+04			2.56E+04	1.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	4/7/11 5:25 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1316-T04-C	1	5.22E+04			5.22E+04	1.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	4/7/11 5:27 PM	EPA Interlab L11 1313-1316 SWA
As	SWA-L11-1316-B01-A	1	5.50E+00	U1/2		5.50E+00	7.1E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	SWA-L11-1316-T01-A	1	8.75E+02			8.75E+02	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 3:11 PM	EPA Interlab 1316 SWA Reruns
B	SWA-L11-1316-T02-A	1	9.35E+02			9.35E+02	5.3E-01	1.0E+00	3.2E+00	1000	100	1.85E+03	91%	VU ICP-OES	5/23/11 3:14 PM	EPA Interlab 1316 SWA Reruns
B	SWA-L11-1316-T03-A	1	5.95E+02			5.95E+02	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 3:16 PM	EPA Interlab 1316 SWA Reruns
B	SWA-L11-1316-T04-A	1	6.29E+02			6.29E+02	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 3:18 PM	EPA Interlab 1316 SWA Reruns
B	SWA-L11-1316-T01-B	1	8.23E+02			8.23E+02	2.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 3:21 PM	EPA Interlab 1316 SWA Reruns
B	SWA-L11-1316-T02-B	1	9.35E+02			9.35E+02	7.8E-01	1.0E+00	3.2E+00	1000	100	1.84E+03	90%	VU ICP-OES	5/23/11 3:23 PM	EPA Interlab 1316 SWA Reruns
B	SWA-L11-1316-T03-B	1	6.14E+02			6.14E+02	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 3:25 PM	EPA Interlab 1316 SWA Reruns
B	SWA-L11-1316-T04-B	1	6.44E+02			6.44E+02	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 3:28 PM	EPA Interlab 1316 SWA Reruns
B	SWA-L11-1316-T01-C	1	8.51E+02			8.51E+02	2.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 3:31 PM	EPA Interlab 1316 SWA Reruns
B	SWA-L11-1316-T02-C	1	9.24E+02			9.24E+02	3.7E-01	1.0E+00	3.2E+00	1000	100	1.87E+03	94%	VU ICP-OES	5/23/11 3:33 PM	EPA Interlab 1316 SWA Reruns
B	SWA-L11-1316-T03-C	1	5.98E+02			5.98E+02	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 3:35 PM	EPA Interlab 1316 SWA Reruns
B	SWA-L11-1316-T04-C	1	6.54E+02			6.54E+02	2.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/23/11 3:38 PM	EPA Interlab 1316 SWA Reruns
B	SWA-L11-1316-B01-A	1	1.89E+01			1.89E+01	2.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	SWA-L11-1316-T01-A	1	2.18E+02			2.18E+02	1.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:09 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1316-T02-A	1	2.33E+02			2.33E+02	6.2E-01	1.0E+00	3.2E+00	10	100	1.13E+03	90%	VU ICP-OES	4/7/11 5:11 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1316-T03-A	1	2.51E+02			2.51E+02	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:12 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1316-T04-A	1	2.02E+02			2.02E+02	6.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:14 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1316-T01-B	1	2.40E+02			2.40E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:15 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1316-T02-B	1	2.56E+02			2.56E+02	1.3E-01	1.0E+00	3.2E+00	10	100	1.22E+03	96%	VU ICP-OES	4/7/11 5:17 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1316-T03-B	1	2.27E+02			2.27E+02	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:19 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1316-T04-B	1	1.79E+02			1.79E+02	1.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:20 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1316-T01-C	1	2.58E+02			2.58E+02	2.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:22 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1316-T02-C	1	2.40E+02			2.40E+02	9.1E-01	1.0E+00	3.2E+00	10	100	1.24E+03	100%	VU ICP-OES	4/7/11 5:24 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1316-T03-C	1	2.24E+02			2.24E+02	1.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:25 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1316-T04-C	1	1.83E+02			1.83E+02	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:27 PM	EPA Interlab L11 1313-1316 SWA
Ba	SWA-L11-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	SWA-L11-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	3.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 5:09 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	2.0E+02	1.9E+00	6.0E+00	10	100	9.98E+02	100%	VU ICP-OES	4/7/11 5:11 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	4.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 5:12 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	7.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 5:14 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	4.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 5:15 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	1.9E+02	1.9E+00	6.0E+00	10	100	9.95E+02	99%	VU ICP-OES	4/7/11 5:17 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	4.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 5:19 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	4.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 5:20 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	2.6E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 5:22 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00	10	100	9.98E+02	100%	VU ICP-OES	4/7/11 5:24 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	8.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 5:25 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 5:27 PM	EPA Interlab L11 1313-1316 SWA
Be	SWA-L11-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	1.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	SWA-L11-1316-T01-A	1	1.10E+00	U1/2		1.10E+00	5.0E+01	2.2E+00	7.0E+00				---	VU ICP-OES	4/7/11 5:09 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1316-T02-A	1	1.10E+00	U1/2		1.10E+00	8.9E+01	2.2E+00	7.0E+00	10	100	9.18E+02	92%	VU ICP-OES	4/7/11 5:11 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1316-T03-A	1	1.10E+00	U1/2		1.10E+00	3.8E+03	2.2E+00	7.0E+00				---	VU ICP-OES	4/7/11 5:12 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1316-T04-A	1	1.10E+00	U1/2		1.10E+00	1.9E+02	2.2E+00	7.0E+00				---	VU ICP-OES	4/7/11 5:14 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1316-T01-B	1	1.10E+00	U1/2		1.10E+00	2.3E+02	2.2E+00	7.0E+00				---	VU ICP-OES	4/7/11 5:15 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1316-T02-B	1	1.10E+00	U1/2		1.10E+00	1.5E+02	2.2E+00	7.0E+00	10	100	9.23E+02	92%	VU ICP-OES	4/7/11 5:17 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1316-T03-B	1	1.10E+00	U1/2		1.10E+00	1.1E+02	2.2E+00	7.0E+00				---	VU ICP-OES	4/7/11 5:19 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1316-T04-B	1	1.10E+00	U1/2		1.10E+00	7.5E+01	2.2E+00	7.0E+00				---	VU ICP-OES	4/7/11 5:20 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1316-T01-C	1	1.10E+00	U1/2		1.10E+00	6.8E+01	2.2E+00	7.0E+00				---	VU ICP-OES	4/7/11 5:22 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1316-T02-C	1	1.10E+00	U1/2		1.10E+00	1.6E+03	2.2E+00	7.0E+00	10	100	9.24E+02	92%	VU ICP-OES	4/7/11 5:24 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1316-T03-C	1	1.10E+00	U1/2		1.10E+00	8.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	4/7/11 5:25 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1316-T04-C	1	1.10E+00	U1/2		1.10E+00	1.1E+02	2.2E+00	7.0E+00				---	VU ICP-OES	4/7/11 5:27 PM	EPA Interlab L11 1313-1316 SWA
Cd	SWA-L11-1316-B01-A	1	1.10E+00	U1/2		1.10E+00	5.3E+02	2.2E+00	7.0E+00				---	VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	SWA-L11-1316-T01-A	1	1.29E+04			1.29E+04	3.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 5:09 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1316-T02-A	1	1.08E+04			1.08E+04	2.2E-01	2.6E+00	8.3E+00	1000	100	1.18E+04	95%	VU ICP-OES	4/7/11 5:11 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1316-T03-A	1	8.11E+03			8.11E+03	3.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 5:12 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1316-T04-A	1	5.91E+03			5.91E+03	5.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 5:14 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1316-T01-B	1	1.50E+04			1.50E+04	5.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 5:15 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1316-T02-B	1	1.11E+04			1.11E+04	3.1E-02	2.6E+00	8.3E+00	1000	100	1.20E+04	91%	VU ICP-OES	4/7/11 5:17 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1316-T03-B	1	7.44E+03			7.44E+03	1.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 5:19 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1316-T04-B	1	5.34E+03			5.34E+03	8.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 5:20 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1316-T01-C	1	1.45E+04			1.45E+04	4.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 5:22 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1316-T02-C	1	1.10E+04			1.10E+04	4.7E-01	2.6E+00	8.3E+00	1000	100	1.19E+04	93%	VU ICP-OES	4/7/11 5:24 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1316-T03-C	1	7.60E+03			7.60E+03	7.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 5:25 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1316-T04-C	1	5.39E+03			5.39E+03	1.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 5:27 PM	EPA Interlab L11 1313-1316 SWA
Ca	SWA-L11-1316-B01-A	1	5.99E+01			5.99E+01	2.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	SWA-L11-1316-T01-A	1	9.08E+02			9.08E+02	1.3E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/23/11 3:11 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L11-1316-T02-A	1	1.34E+03			1.34E+03	1.2E+00	1.2E+00	3.8E+00	10	100	2.25E+03	92%	VU ICP-OES	5/23/11 3:14 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L11-1316-T03-A	1	1.80E+03			1.80E+03	4.3E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/23/11 3:16 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L11-1316-T04-A	1	2.18E+03			2.18E+03	9.9E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/23/11 3:18 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L11-1316-T01-B	1	9.03E+02			9.03E+02	6.6E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/23/11 3:21 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L11-1316-T02-B	1	1.34E+03			1.34E+03	1.3E+00	1.2E+00	3.8E+00	10	100	2.21E+03	88%	VU ICP-OES	5/23/11 3:23 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L11-1316-T03-B	1	1.81E+03			1.81E+03	1.6E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/23/11 3:25 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L11-1316-T04-B	1	2.18E+03			2.18E+03	2.2E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/23/11 3:28 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L11-1316-T01-C	1	9.23E+02			9.23E+02	1.2E+00	1.2E+00	3.8E+00			---		VU ICP-OES	5/23/11 3:31 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L11-1316-T02-C	1	1.36E+03			1.36E+03	1.3E+00	1.2E+00	3.8E+00	10	100	2.27E+03	91%	VU ICP-OES	5/23/11 3:33 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L11-1316-T03-C	1	1.79E+03			1.79E+03	6.8E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/23/11 3:35 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L11-1316-T04-C	1	2.04E+03			2.04E+03	5.2E-01	1.2E+00	3.8E+00			---		VU ICP-OES	5/23/11 3:38 PM	EPA Interlab 1316 SWA Reruns
Cr	SWA-L11-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	2.5E+01	1.2E+00	3.8E+00			---		VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	SWA-L11-1316-T01-A	1	9.00E-01	U1/2		9.00E-01	1.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 5:09 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1316-T02-A	1	9.00E-01	U1/2		9.00E-01	1.9E+01	1.8E+00	5.7E+00	10	100	9.92E+02	99%	VU ICP-OES	4/7/11 5:11 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1316-T03-A	1	1.92E+00	E		1.92E+00	5.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 5:12 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1316-T04-A	1	4.30E+00	E		4.30E+00	1.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 5:14 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1316-T01-B	1	9.00E-01	U1/2		9.00E-01	6.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 5:15 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1316-T02-B	1	9.00E-01	U1/2		9.00E-01	4.3E+01	1.8E+00	5.7E+00	10	100	9.91E+02	99%	VU ICP-OES	4/7/11 5:17 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1316-T03-B	1	1.95E+00	E		1.95E+00	4.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 5:19 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1316-T04-B	1	4.66E+00	E		4.66E+00	9.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 5:20 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1316-T01-C	1	9.00E-01	U1/2		9.00E-01	6.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 5:22 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1316-T02-C	1	9.00E-01	U1/2		9.00E-01	5.5E+01	1.8E+00	5.7E+00	10	100	9.96E+02	100%	VU ICP-OES	4/7/11 5:24 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1316-T03-C	1	1.96E+00	E		1.96E+00	3.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 5:25 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1316-T04-C	1	3.86E+00	E		3.86E+00	5.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 5:27 PM	EPA Interlab L11 1313-1316 SWA
Co	SWA-L11-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	SWA-L11-1316-T01-A	1	1.85E+00	U1/2		1.85E+00	3.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 5:09 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1316-T02-A	1	1.85E+00	U1/2		1.85E+00	1.1E+02	3.7E+00	1.2E+01	10	100	1.05E+03	105%	VU ICP-OES	4/7/11 5:11 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1316-T03-A	1	1.85E+00	U1/2		1.85E+00	9.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 5:12 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1316-T04-A	1	1.85E+00	U1/2		1.85E+00	2.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 5:14 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1316-T01-B	1	1.85E+00	U1/2		1.85E+00	2.5E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 5:15 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1316-T02-B	1	1.85E+00	U1/2		1.85E+00	8.7E+01	3.7E+00	1.2E+01	10	100	1.04E+03	104%	VU ICP-OES	4/7/11 5:17 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1316-T03-B	1	1.85E+00	U1/2		1.85E+00	8.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 5:19 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1316-T04-B	1	1.85E+00	U1/2		1.85E+00	1.6E+04	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 5:20 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1316-T01-C	1	1.85E+00	U1/2		1.85E+00	2.8E+03	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 5:22 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1316-T02-C	1	1.85E+00	U1/2		1.85E+00	4.9E+02	3.7E+00	1.2E+01	10	100	1.02E+03	102%	VU ICP-OES	4/7/11 5:24 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1316-T03-C	1	1.85E+00	U1/2		1.85E+00	2.2E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 5:25 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1316-T04-C	1	1.85E+00	U1/2		1.85E+00	1.5E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 5:27 PM	EPA Interlab L11 1313-1316 SWA
Cu	SWA-L11-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	2.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	SWA-L11-1316-T01-A	1	6.56E+01			6.56E+01	5.0E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 5:09 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1316-T02-A	1	1.40E+02			1.40E+02	1.0E+00	2.0E+00	6.4E+00	1000	100	1.13E+03	99%	VU ICP-OES	4/7/11 5:11 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1316-T03-A	1	3.41E+02			3.41E+02	7.0E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 5:12 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1316-T04-A	1	8.30E+02			8.30E+02	7.3E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 5:14 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1316-T01-B	1	6.66E+01			6.66E+01	1.2E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 5:15 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1316-T02-B	1	1.35E+02			1.35E+02	3.5E-01	2.0E+00	6.4E+00	1000	100	1.18E+03	104%	VU ICP-OES	4/7/11 5:17 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1316-T03-B	1	3.57E+02			3.57E+02	1.3E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 5:19 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1316-T04-B	1	9.69E+02			9.69E+02	4.7E-02	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 5:20 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1316-T01-C	1	6.94E+01			6.94E+01	5.7E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 5:22 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1316-T02-C	1	1.38E+02			1.38E+02	4.9E-01	2.0E+00	6.4E+00	1000	100	1.27E+03	113%	VU ICP-OES	4/7/11 5:24 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1316-T03-C	1	3.26E+02			3.26E+02	9.9E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 5:25 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1316-T04-C	1	8.90E+02			8.90E+02	9.2E-01	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 5:27 PM	EPA Interlab L11 1313-1316 SWA
Fe	SWA-L11-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	2.4E+00	2.0E+00	6.4E+00			---		VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	SWA-L11-1316-T01-A	1	1.60E+01	E		1.60E+01	9.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 5:09 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1316-T02-A	1	2.35E+01			2.35E+01	1.3E+01	6.8E+00	2.2E+01	10	100	1.14E+03	112%	VU ICP-OES	4/7/11 5:11 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1316-T03-A	1	8.98E+01			8.98E+01	9.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 5:12 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1316-T04-A	1	1.76E+02			1.76E+02	2.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 5:14 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1316-T01-B	1	1.52E+01	E		1.52E+01	3.7E+01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 5:15 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1316-T02-B	1	3.29E+01			3.29E+01	1.3E+01	6.8E+00	2.2E+01	10	100	1.14E+03	111%	VU ICP-OES	4/7/11 5:17 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1316-T03-B	1	6.85E+01			6.85E+01	3.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 5:19 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1316-T04-B	1	1.77E+02			1.77E+02	6.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 5:20 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1316-T01-C	1	1.46E+01	E		1.46E+01	4.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 5:22 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1316-T02-C	1	3.09E+01			3.09E+01	9.3E+00	6.8E+00	2.2E+01	10	100	1.17E+03	114%	VU ICP-OES	4/7/11 5:24 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1316-T03-C	1	7.72E+01			7.72E+01	4.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 5:25 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1316-T04-C	1	1.77E+02			1.77E+02	1.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 5:27 PM	EPA Interlab L11 1313-1316 SWA
Pb	SWA-L11-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	2.3E+02	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	SWA-L11-1316-T01-A	1	2.39E+00	E		2.39E+00	4.3E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/23/11 3:11 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L11-1316-T02-A	1	5.93E+00	E		5.93E+00	1.8E+00	1.9E+00	6.0E+00	10	100	8.58E+02	85%	VU ICP-OES	5/23/11 3:14 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L11-1316-T03-A	1	7.49E+00			7.49E+00	2.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/23/11 3:16 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L11-1316-T04-A	1	1.04E+01			1.04E+01	5.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/23/11 3:18 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L11-1316-T01-B	1	2.18E+00	E		2.18E+00	3.8E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/23/11 3:21 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L11-1316-T02-B	1	6.11E+00			6.11E+00	1.8E+00	1.9E+00	6.0E+00	10	100	9.13E+02	91%	VU ICP-OES	5/23/11 3:23 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L11-1316-T03-B	1	7.87E+00			7.87E+00	2.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/23/11 3:25 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L11-1316-T04-B	1	1.12E+01			1.12E+01	3.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/23/11 3:28 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L11-1316-T01-C	1	2.01E+00	E		2.01E+00	1.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/23/11 3:31 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L11-1316-T02-C	1	5.57E+00	E		5.57E+00	4.6E+00	1.9E+00	6.0E+00	10	100	8.78E+02	87%	VU ICP-OES	5/23/11 3:33 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L11-1316-T03-C	1	7.66E+00			7.66E+00	1.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/23/11 3:35 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L11-1316-T04-C	1	1.06E+01			1.06E+01	3.7E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/23/11 3:38 PM	EPA Interlab 1316 SWA Reruns
Li	SWA-L11-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	2.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	SWA-L11-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	8.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 5:09 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00	10	100	1.06E+03	106%	VU ICP-OES	4/7/11 5:11 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 5:12 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1316-T04-A	1	3.15E+00	E		3.15E+00	4.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 5:14 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	2.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 5:15 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00	10	100	1.06E+03	106%	VU ICP-OES	4/7/11 5:17 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	4.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 5:19 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1316-T04-B	1	4.58E+00	E		4.58E+00	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 5:20 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 5:22 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	7.1E+00	2.0E+00	6.4E+00	10	100	1.07E+03	107%	VU ICP-OES	4/7/11 5:24 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	2.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 5:25 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1316-T04-C	1	3.69E+00	E		3.69E+00	1.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 5:27 PM	EPA Interlab L11 1313-1316 SWA
Mn	SWA-L11-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	1.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	SWA-L11-1316-T01-A	1	1.30E+01			1.30E+01	1.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:09 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1316-T02-A	1	1.96E+01			1.96E+01	4.9E+01	1.0E+00	3.2E+00	1000	100	9.19E+02	90%	VU ICP-OES	4/7/11 5:11 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1316-T03-A	1	2.34E+01			2.34E+01	6.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:12 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1316-T04-A	1	2.73E+01			2.73E+01	1.3E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:14 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1316-T01-B	1	9.60E+00			9.60E+00	1.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:15 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1316-T02-B	1	1.76E+01			1.76E+01	1.3E+01	1.0E+00	3.2E+00	1000	100	9.25E+02	91%	VU ICP-OES	4/7/11 5:17 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1316-T03-B	1	2.29E+01			2.29E+01	1.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:19 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1316-T04-B	1	2.97E+01			2.97E+01	1.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:20 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1316-T01-C	1	1.08E+01			1.08E+01	6.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:22 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1316-T02-C	1	2.66E+01			2.66E+01	2.0E+01	1.0E+00	3.2E+00	1000	100	9.74E+02	95%	VU ICP-OES	4/7/11 5:24 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1316-T03-C	1	2.37E+01			2.37E+01	6.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:25 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1316-T04-C	1	2.66E+01			2.66E+01	3.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:27 PM	EPA Interlab L11 1313-1316 SWA
Mg	SWA-L11-1316-B01-A	1	1.96E+01			1.96E+01	9.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	SWA-L11-1316-T01-A	1	1.01E+02			1.01E+02	3.1E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 5:09 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1316-T02-A	1	1.78E+02			1.78E+02	6.9E-01	1.2E+00	3.8E+00	10	100	1.15E+03	98%	VU ICP-OES	4/7/11 5:11 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1316-T03-A	1	3.64E+02			3.64E+02	3.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 5:12 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1316-T04-A	1	6.68E+02			6.68E+02	4.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 5:14 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1316-T01-B	1	1.04E+02			1.04E+02	1.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 5:15 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1316-T02-B	1	1.67E+02			1.67E+02	2.1E+00	1.2E+00	3.8E+00	10	100	1.15E+03	98%	VU ICP-OES	4/7/11 5:17 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1316-T03-B	1	3.57E+02			3.57E+02	1.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 5:19 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1316-T04-B	1	6.52E+02			6.52E+02	2.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 5:20 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1316-T01-C	1	1.07E+02			1.07E+02	8.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 5:22 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1316-T02-C	1	1.63E+02			1.63E+02	5.9E-01	1.2E+00	3.8E+00	10	100	1.16E+03	100%	VU ICP-OES	4/7/11 5:24 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1316-T03-C	1	3.24E+02			3.24E+02	4.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 5:25 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1316-T04-C	1	5.57E+02			5.57E+02	1.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 5:27 PM	EPA Interlab L11 1313-1316 SWA
Mo	SWA-L11-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	2.3E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	SWA-L11-1316-T01-A	1	9.00E-01	U1/2		9.00E-01	2.3E+02	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 5:09 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1316-T02-A	1	9.00E-01	U1/2		9.00E-01	1.6E+02	1.8E+00	5.7E+00	10	100	1.01E+03	101%	VU ICP-OES	4/7/11 5:11 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1316-T03-A	1	9.00E-01	U1/2		9.00E-01	3.3E+02	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 5:12 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1316-T04-A	1	4.55E+00	E		4.55E+00	4.5E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 5:14 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1316-T01-B	1	9.00E-01	U1/2		9.00E-01	2.1E+02	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 5:15 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1316-T02-B	1	9.00E-01	U1/2		9.00E-01	5.7E+02	1.8E+00	5.7E+00	10	100	1.08E+03	107%	VU ICP-OES	4/7/11 5:17 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1316-T03-B	1	9.00E-01	U1/2		9.00E-01	3.0E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 5:19 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1316-T04-B	1	5.20E+00	E		5.20E+00	3.8E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 5:20 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1316-T01-C	1	9.00E-01	U1/2		9.00E-01	1.8E+02	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 5:22 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1316-T02-C	1	9.00E-01	U1/2		9.00E-01	2.1E+01	1.8E+00	5.7E+00	10	100	1.03E+03	103%	VU ICP-OES	4/7/11 5:24 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1316-T03-C	1	9.00E-01	U1/2		9.00E-01	7.0E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 5:25 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1316-T04-C	1	3.31E+00	E		3.31E+00	3.4E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 5:27 PM	EPA Interlab L11 1313-1316 SWA
Ni	SWA-L11-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	7.8E+01	1.8E+00	5.7E+00			---		VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	SWA-L11-1316-T01-A	1	2.58E+01			2.58E+01	4.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/7/11 5:09 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1316-T02-A	1	1.02E+02			1.02E+02	6.2E+00	3.7E+00	1.2E+01	1000	100	1.21E+03	111%	VU ICP-OES	4/7/11 5:11 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1316-T03-A	1	3.53E+02			3.53E+02	3.0E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/7/11 5:12 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1316-T04-A	1	1.32E+03			1.32E+03	4.3E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/7/11 5:14 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1316-T01-B	1	3.20E+01			3.20E+01	7.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/7/11 5:15 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1316-T02-B	1	9.19E+01			9.19E+01	5.4E+00	3.7E+00	1.2E+01	1000	100	1.18E+03	109%	VU ICP-OES	4/7/11 5:17 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1316-T03-B	1	3.80E+02			3.80E+02	7.1E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/7/11 5:19 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1316-T04-B	1	1.23E+03			1.23E+03	7.8E-01	3.7E+00	1.2E+01			---		VU ICP-OES	4/7/11 5:20 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1316-T01-C	1	3.67E+01			3.67E+01	2.1E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/7/11 5:22 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1316-T02-C	1	9.87E+01			9.87E+01	5.9E+00	3.7E+00	1.2E+01	1000	100	1.20E+03	110%	VU ICP-OES	4/7/11 5:24 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1316-T03-C	1	3.61E+02			3.61E+02	1.9E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/7/11 5:25 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1316-T04-C	1	1.27E+03			1.27E+03	2.2E+00	3.7E+00	1.2E+01			---		VU ICP-OES	4/7/11 5:27 PM	EPA Interlab L11 1313-1316 SWA
P	SWA-L11-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	4.6E+01	3.7E+00	1.2E+01			---		VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	SWA-L11-1316-T01-A	1	3.02E+05			3.02E+05	2.5E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/7/11 5:09 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1316-T02-A	1	4.73E+05			4.73E+05	4.1E-01	1.6E+00	5.1E+00	1000	100	4.74E+05	97%	VU ICP-OES	4/7/11 5:11 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1316-T03-A	1	8.50E+05			8.50E+05	2.1E+00	1.6E+00	5.1E+00			---		VU ICP-OES	4/7/11 5:12 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1316-T04-A	1	2.99E+06			2.99E+06	7.2E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/7/11 5:14 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1316-T01-B	1	3.11E+05			3.11E+05	8.9E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/7/11 5:15 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1316-T02-B	1	4.82E+05			4.82E+05	3.3E+00	1.6E+00	5.1E+00	1000	100	4.83E+05	91%	VU ICP-OES	4/7/11 5:17 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1316-T03-B	1	9.10E+05			9.10E+05	1.3E+01	1.6E+00	5.1E+00			---		VU ICP-OES	4/7/11 5:19 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1316-T04-B	1	2.96E+06			2.96E+06	7.3E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/7/11 5:20 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1316-T01-C	1	3.20E+05			3.20E+05	2.6E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/7/11 5:22 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1316-T02-C	1	4.84E+05			4.84E+05	2.2E+00	1.6E+00	5.1E+00	1000	100	4.85E+05	92%	VU ICP-OES	4/7/11 5:24 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1316-T03-C	1	9.09E+05			9.09E+05	1.5E+01	1.6E+00	5.1E+00			---		VU ICP-OES	4/7/11 5:25 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1316-T04-C	1	2.91E+06			2.91E+06	3.2E-01	1.6E+00	5.1E+00			---		VU ICP-OES	4/7/11 5:27 PM	EPA Interlab L11 1313-1316 SWA
K	SWA-L11-1316-B01-A	1	4.89E+01			4.89E+01	1.3E+00	1.6E+00	5.1E+00			---		VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	SWA-L11-1316-T01-A	1	7.33E+04			7.33E+04	5.1E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 5:09 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1316-T02-A	1	1.44E+05			1.44E+05	4.2E-01	1.5E+01	4.8E+01	10	100	1.45E+05	109%	VU ICP-OES	4/7/11 5:11 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1316-T03-A	1	3.17E+05			3.17E+05	2.3E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 5:12 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1316-T04-A	1	6.45E+05			6.45E+05	7.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 5:14 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1316-T01-B	1	7.67E+04			7.67E+04	3.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 5:15 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1316-T02-B	1	1.44E+05			1.44E+05	4.2E-01	1.5E+01	4.8E+01	10	100	1.45E+05	96%	VU ICP-OES	4/7/11 5:17 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1316-T03-B	1	3.25E+05			3.25E+05	3.9E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 5:19 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1316-T04-B	1	6.34E+05			6.34E+05	2.5E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 5:20 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1316-T01-C	1	8.52E+04			8.52E+04	4.4E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 5:22 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1316-T02-C	1	1.48E+05			1.48E+05	3.7E-01	1.5E+01	4.8E+01	10	100	1.49E+05	87%	VU ICP-OES	4/7/11 5:24 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1316-T03-C	1	3.04E+05			3.04E+05	5.9E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 5:25 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1316-T04-C	1	6.56E+05			6.56E+05	3.7E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 5:27 PM	EPA Interlab L11 1313-1316 SWA
Se	SWA-L11-1316-B01-A	1	7.50E+00	U1/2		7.50E+00	5.2E+01	1.5E+01	4.8E+01				---	VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	SWA-L11-1316-T01-A	1	2.32E+04			2.32E+04	1.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 5:09 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1316-T02-A	1	3.24E+04			3.24E+04	8.2E-01	1.1E+00	3.5E+00	1000	100	3.35E+04	111%	VU ICP-OES	4/7/11 5:11 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1316-T03-A	1	4.82E+04			4.82E+04	1.5E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 5:12 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1316-T04-A	1	7.01E+04			7.01E+04	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 5:14 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1316-T01-B	1	2.37E+04			2.37E+04	8.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 5:15 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1316-T02-B	1	3.25E+04			3.25E+04	8.6E-01	1.1E+00	3.5E+00	1000	100	3.35E+04	98%	VU ICP-OES	4/7/11 5:17 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1316-T03-B	1	4.91E+04			4.91E+04	2.4E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 5:19 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1316-T04-B	1	6.84E+04			6.84E+04	2.4E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 5:20 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1316-T01-C	1	2.32E+04			2.32E+04	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 5:22 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1316-T02-C	1	3.29E+04			3.29E+04	9.2E-01	1.1E+00	3.5E+00	1000	100	3.38E+04	94%	VU ICP-OES	4/7/11 5:24 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1316-T03-C	1	4.74E+04			4.74E+04	1.4E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 5:25 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1316-T04-C	1	6.78E+04			6.78E+04	6.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 5:27 PM	EPA Interlab L11 1313-1316 SWA
Si	SWA-L11-1316-B01-A	1	1.32E+01			1.32E+01	2.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	SWA-L11-1316-T01-A	1	4.51E+05			4.51E+05	1.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 5:09 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1316-T02-A	1	5.66E+05			5.66E+05	6.5E-02	2.5E+00	8.0E+00	1000	100	5.67E+05	90%	VU ICP-OES	4/7/11 5:11 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1316-T03-A	1	6.60E+05			6.60E+05	8.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 5:12 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1316-T04-A	1	7.01E+05			7.01E+05	2.6E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 5:14 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1316-T01-B	1	4.60E+05			4.60E+05	3.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 5:15 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1316-T02-B	1	5.68E+05			5.68E+05	2.3E-01	2.5E+00	8.0E+00	1000	100	5.69E+05	87%	VU ICP-OES	4/7/11 5:17 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1316-T03-B	1	6.65E+05			6.65E+05	5.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 5:19 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1316-T04-B	1	6.92E+05			6.92E+05	1.7E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 5:20 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1316-T01-C	1	4.68E+05			4.68E+05	2.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 5:22 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1316-T02-C	1	5.66E+05			5.66E+05	7.5E-01	2.5E+00	8.0E+00	1000	100	5.67E+05	91%	VU ICP-OES	4/7/11 5:24 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1316-T03-C	1	6.68E+05			6.68E+05	2.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 5:25 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1316-T04-C	1	7.00E+05			7.00E+05	1.8E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 5:27 PM	EPA Interlab L11 1313-1316 SWA
Na	SWA-L11-1316-B01-A	1	8.21E+01			8.21E+01	7.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	SWA-L11-1316-T01-A	1	2.76E+02			2.76E+02	4.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:09 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1316-T02-A	1	2.91E+02			2.91E+02	4.1E-01	1.0E+00	3.2E+00	1000	100	1.46E+03	117%	VU ICP-OES	4/7/11 5:11 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1316-T03-A	1	3.24E+02			3.24E+02	6.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:12 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1316-T04-A	1	3.52E+02			3.52E+02	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:14 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1316-T01-B	1	3.04E+02			3.04E+02	2.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:15 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1316-T02-B	1	2.91E+02			2.91E+02	6.4E-01	1.0E+00	3.2E+00	1000	100	1.36E+03	107%	VU ICP-OES	4/7/11 5:17 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1316-T03-B	1	3.06E+02			3.06E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:19 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1316-T04-B	1	3.42E+02			3.42E+02	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:20 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1316-T01-C	1	3.12E+02			3.12E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:22 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1316-T02-C	1	2.95E+02			2.95E+02	7.6E-01	1.0E+00	3.2E+00	1000	100	1.36E+03	106%	VU ICP-OES	4/7/11 5:24 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1316-T03-C	1	3.10E+02			3.10E+02	1.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:25 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1316-T04-C	1	3.45E+02			3.45E+02	6.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:27 PM	EPA Interlab L11 1313-1316 SWA
Sr	SWA-L11-1316-B01-A	1	1.27E+00	E		1.27E+00	2.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	SWA-L11-1316-T01-A	1	7.30E+05			7.30E+05	1.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 5:09 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1316-T02-A	1	1.07E+06			1.07E+06	1.1E+00	6.8E+00	2.2E+01	1000	100	1.16E+06	91%	VU ICP-OES	4/7/11 5:11 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1316-T03-A	1	1.87E+06			1.87E+06	4.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 5:12 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1316-T04-A	1	2.55E+06			2.55E+06	1.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 5:14 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1316-T01-B	1	8.08E+05			8.08E+05	8.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 5:15 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1316-T02-B	1	1.18E+06			1.18E+06	1.3E+00	6.8E+00	2.2E+01	1000	100	1.27E+06	87%	VU ICP-OES	4/7/11 5:17 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1316-T03-B	1	1.84E+06			1.84E+06	7.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 5:19 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1316-T04-B	1	2.51E+06			2.51E+06	2.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 5:20 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1316-T01-C	1	9.01E+05			9.01E+05	4.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 5:22 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1316-T02-C	1	1.24E+06			1.24E+06	1.2E+00	6.8E+00	2.2E+01	1000	100	1.34E+06	96%	VU ICP-OES	4/7/11 5:24 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1316-T03-C	1	1.77E+06			1.77E+06	1.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 5:25 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1316-T04-C	1	2.54E+06			2.54E+06	7.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 5:27 PM	EPA Interlab L11 1313-1316 SWA
S	SWA-L11-1316-B01-A	1	1.18E+02			1.18E+02	6.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	SWA-L11-1316-T01-A	1	2.30E+00	U1/2		2.30E+00	3.3E+01	4.6E+00	1.5E+01			---		VU ICP-OES	4/7/11 5:09 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1316-T02-A	1	2.30E+00	U1/2		2.30E+00	3.0E+01	4.6E+00	1.5E+01	10	100	1.14E+03	114%	VU ICP-OES	4/7/11 5:11 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1316-T03-A	1	2.30E+00	U1/2		2.30E+00	1.7E+02	4.6E+00	1.5E+01			---		VU ICP-OES	4/7/11 5:12 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1316-T04-A	1	2.30E+00	U1/2		2.30E+00	6.3E+01	4.6E+00	1.5E+01			---		VU ICP-OES	4/7/11 5:14 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1316-T01-B	1	2.30E+00	U1/2		2.30E+00	6.0E+01	4.6E+00	1.5E+01			---		VU ICP-OES	4/7/11 5:15 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1316-T02-B	1	2.30E+00	U1/2		2.30E+00	3.1E+01	4.6E+00	1.5E+01	10	100	1.13E+03	112%	VU ICP-OES	4/7/11 5:17 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1316-T03-B	1	2.30E+00	U1/2		2.30E+00	4.3E+01	4.6E+00	1.5E+01			---		VU ICP-OES	4/7/11 5:19 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1316-T04-B	1	2.30E+00	U1/2		2.30E+00	1.4E+02	4.6E+00	1.5E+01			---		VU ICP-OES	4/7/11 5:20 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1316-T01-C	1	2.30E+00	U1/2		2.30E+00	1.6E+01	4.6E+00	1.5E+01			---		VU ICP-OES	4/7/11 5:22 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1316-T02-C	1	2.30E+00	U1/2		2.30E+00	6.2E+01	4.6E+00	1.5E+01	10	100	1.13E+03	113%	VU ICP-OES	4/7/11 5:24 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1316-T03-C	1	2.30E+00	U1/2		2.30E+00	5.2E+01	4.6E+00	1.5E+01			---		VU ICP-OES	4/7/11 5:25 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1316-T04-C	1	2.30E+00	U1/2		2.30E+00	1.2E+02	4.6E+00	1.5E+01			---		VU ICP-OES	4/7/11 5:27 PM	EPA Interlab L11 1313-1316 SWA
Tl	SWA-L11-1316-B01-A	1	2.30E+00	U1/2		2.30E+00	4.4E+00	4.6E+00	1.5E+01			---		VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	SWA-L11-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 5:09 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	1.0E+02	2.0E+00	6.4E+00	10	100	9.30E+02	93%	VU ICP-OES	4/7/11 5:11 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	9.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 5:12 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	4.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 5:14 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 5:15 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	2.4E+01	2.0E+00	6.4E+00	10	100	9.75E+02	97%	VU ICP-OES	4/7/11 5:17 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	3.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 5:19 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	1.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 5:20 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 5:22 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	4.1E+01	2.0E+00	6.4E+00	10	100	9.67E+02	97%	VU ICP-OES	4/7/11 5:24 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	3.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 5:25 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	4.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 5:27 PM	EPA Interlab L11 1313-1316 SWA
Ti	SWA-L11-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	SWA-L11-1316-T01-A	1	2.82E+02			2.82E+02	1.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 5:09 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1316-T02-A	1	5.07E+02			5.07E+02	1.6E+00	1.5E+00	4.8E+00	10	100	1.44E+03	94%	VU ICP-OES	4/7/11 5:11 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1316-T03-A	1	9.79E+02			9.79E+02	6.9E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 5:12 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1316-T04-A	1	1.77E+03			1.77E+03	1.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 5:14 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1316-T01-B	1	2.67E+02			2.67E+02	4.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 5:15 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1316-T02-B	1	5.04E+02			5.04E+02	8.7E-01	1.5E+00	4.8E+00	10	100	1.45E+03	94%	VU ICP-OES	4/7/11 5:17 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1316-T03-B	1	9.87E+02			9.87E+02	1.9E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 5:19 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1316-T04-B	1	1.60E+03			1.60E+03	6.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 5:20 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1316-T01-C	1	2.98E+02			2.98E+02	2.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 5:22 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1316-T02-C	1	5.13E+02			5.13E+02	1.1E+00	1.5E+00	4.8E+00	10	100	1.45E+03	94%	VU ICP-OES	4/7/11 5:24 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1316-T03-C	1	9.39E+02			9.39E+02	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 5:25 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1316-T04-C	1	1.72E+03			1.72E+03	2.8E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 5:27 PM	EPA Interlab L11 1313-1316 SWA
V	SWA-L11-1316-B01-A	1	2.25E+00	E		2.25E+00	3.7E+01	1.5E+00	4.8E+00				---	VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	SWA-L11-1316-T01-A	1	1.54E+00	E		1.54E+00	6.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:09 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1316-T02-A	1	1.77E+00	E		1.77E+00	1.3E+01	1.0E+00	3.2E+00	10	100	1.17E+03	116%	VU ICP-OES	4/7/11 5:11 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1316-T03-A	1	4.16E+00			4.16E+00	9.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:12 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1316-T04-A	1	1.16E+01			1.16E+01	6.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:14 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1316-T01-B	1	1.06E+00	E		1.06E+00	6.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:15 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1316-T02-B	1	1.72E+00	E		1.72E+00	1.1E+01	1.0E+00	3.2E+00	10	100	1.11E+03	111%	VU ICP-OES	4/7/11 5:17 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1316-T03-B	1	3.86E+00			3.86E+00	6.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:19 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1316-T04-B	1	1.04E+01			1.04E+01	3.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:20 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1316-T01-C	1	1.64E+00	E		1.64E+00	3.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:22 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1316-T02-C	1	1.79E+00	E		1.79E+00	1.3E+01	1.0E+00	3.2E+00	10	100	1.11E+03	111%	VU ICP-OES	4/7/11 5:24 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1316-T03-C	1	4.35E+00			4.35E+00	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:25 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1316-T04-C	1	1.03E+01			1.03E+01	2.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:27 PM	EPA Interlab L11 1313-1316 SWA
Zn	SWA-L11-1316-B01-A	1	1.67E+00	E		1.67E+00	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/7/11 5:04 PM	EPA Interlab L11 1313-1316 SWA

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	SWA-LRef-1316-T01-A	1	3.48E+04			3.48E+04	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1316-T02-A	1	5.32E+04			5.32E+04	3.4E-01	1.0E+00	3.2E+00	1000	100	5.42E+04	103%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1316-T03-A	1	1.00E+05			1.00E+05	8.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1316-T04-A	1	1.55E+05			1.55E+05	3.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1316-T01-B	1	3.30E+04			3.30E+04	3.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1316-T02-B	1	5.02E+04			5.02E+04	3.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1316-T03-B	1	9.49E+04			9.49E+04	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1316-T04-B	1	1.65E+05			1.65E+05	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1316-T01-C	1	2.21E+04			2.21E+04	6.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1316-T02-C	1	5.30E+04			5.30E+04	4.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1316-T03-C	1	1.01E+05			1.01E+05	5.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1316-T04-C	1	1.66E+05			1.66E+05	4.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1316-B01-A	1	2.31E+00	E		2.31E+00	6.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	SWA-LRef-1316-T01-A	1	5.24E+03			5.24E+03	9.3E-01	7.5E+00	2.4E+01				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1316-T02-A	1	6.09E+03			6.09E+03	6.0E-01	7.5E+00	2.4E+01	10	100	7.12E+03	104%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1316-T03-A	1	6.33E+03			6.33E+03	1.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1316-T04-A	1	5.85E+03			5.85E+03	1.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1316-T01-B	1	4.67E+03			4.67E+03	5.1E-01	7.5E+00	2.4E+01				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1316-T02-B	1	5.52E+03			5.52E+03	3.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1316-T03-B	1	6.43E+03			6.43E+03	4.8E-01	7.5E+00	2.4E+01				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1316-T04-B	1	7.49E+03			7.49E+03	9.7E-01	7.5E+00	2.4E+01				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1316-T01-C	1	4.39E+03			4.39E+03	7.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1316-T02-C	1	5.88E+03			5.88E+03	4.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1316-T03-C	1	7.26E+03			7.26E+03	5.9E+00	7.5E+00	2.4E+01				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1316-T04-C	1	7.10E+03			7.10E+03	4.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1316-B01-A	1	3.75E+00	U1/2		3.75E+00	4.9E+02	7.5E+00	2.4E+01				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	SWA-LRef-1316-T01-A	1	4.43E+03			4.43E+03	6.9E-01	1.1E+01	3.5E+01				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1316-T02-A	1	1.27E+04			1.27E+04	2.6E-01	1.1E+01	3.5E+01	10	100	1.37E+04	100%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1316-T03-A	1	4.19E+04			4.19E+04	6.7E-01	1.1E+01	3.5E+01				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1316-T04-A	1	1.17E+05			1.17E+05	7.4E-01	1.1E+01	3.5E+01				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1316-T01-B	1	4.18E+03			4.18E+03	5.8E-01	1.1E+01	3.5E+01				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1316-T02-B	1	1.19E+04			1.19E+04	3.7E+00	1.1E+01	3.5E+01				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1316-T03-B	1	4.54E+04			4.54E+04	4.1E-01	1.1E+01	3.5E+01				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1316-T04-B	1	1.23E+05			1.23E+05	9.4E-01	1.1E+01	3.5E+01				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1316-T01-C	1	4.04E+03			4.04E+03	7.0E+01	1.1E+01	3.5E+01				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1316-T02-C	1	1.09E+04			1.09E+04	4.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1316-T03-C	1	4.28E+04			4.28E+04	6.7E+00	1.1E+01	3.5E+01				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1316-T04-C	1	1.07E+05			1.07E+05	4.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1316-B01-A	1	5.50E+00	U1/2		5.50E+00	1.6E+02	1.1E+01	3.5E+01				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	SWA-LRef-1316-T01-A	1	1.02E+03			1.02E+03	2.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1316-T02-A	1	9.04E+02			9.04E+02	6.4E-01	1.0E+00	3.2E+00	1000	100	1.80E+03	89%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1316-T03-A	1	6.95E+02			6.95E+02	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1316-T04-A	1	7.46E+02			7.46E+02	8.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1316-T01-B	1	1.03E+03			1.03E+03	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1316-T02-B	1	9.12E+02			9.12E+02	4.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1316-T03-B	1	6.25E+02			6.25E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1316-T04-B	1	7.10E+02			7.10E+02	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1316-T01-C	1	1.10E+03			1.10E+03	7.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1316-T02-C	1	9.17E+02			9.17E+02	4.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1316-T03-C	1	6.68E+02			6.68E+02	7.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1316-T04-C	1	7.41E+02			7.41E+02	4.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1316-B01-A	1	9.35E+00			9.35E+00	3.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	SWA-LRef-1316-T01-A	1	1.72E+02			1.72E+02	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1316-T02-A	1	1.49E+02			1.49E+02	5.3E-01	1.0E+00	3.2E+00	10	100	1.00E+03	85%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1316-T03-A	1	1.27E+02			1.27E+02	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1316-T04-A	1	1.67E+02			1.67E+02	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1316-T01-B	1	1.59E+02			1.59E+02	1.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1316-T02-B	1	1.40E+02			1.40E+02	4.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1316-T03-B	1	1.39E+02			1.39E+02	4.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1316-T04-B	1	1.29E+02			1.29E+02	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1316-T01-C	1	1.16E+02			1.16E+02	6.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1316-T02-C	1	1.51E+02			1.51E+02	3.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1316-T03-C	1	1.50E+02			1.50E+02	5.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1316-T04-C	1	1.24E+02			1.24E+02	7.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	3.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	SWA-LRef-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	5.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	1.1E+01	1.9E+00	6.0E+00	10	100	1.12E+03	112%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	1.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	6.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	7.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	2.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	6.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	1.9E+02	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	6.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	2.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	8.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	SWA-LRef-1316-T01-A	1	1.10E+00	U1/2		1.10E+00	2.0E+02	2.2E+00	7.0E+00				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1316-T02-A	1	1.10E+00	U1/2		1.10E+00	1.8E+02	2.2E+00	7.0E+00	10	100	1.02E+03	102%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1316-T03-A	1	1.10E+00	U1/2		1.10E+00	2.7E+02	2.2E+00	7.0E+00				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1316-T04-A	1	1.10E+00	U1/2		1.10E+00	5.6E+01	2.2E+00	7.0E+00				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1316-T01-B	1	1.10E+00	U1/2		1.10E+00	7.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1316-T02-B	1	1.10E+00	U1/2		1.10E+00	4.9E+01	2.2E+00	7.0E+00				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1316-T03-B	1	1.10E+00	U1/2		1.10E+00	1.9E+02	2.2E+00	7.0E+00				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1316-T04-B	1	1.10E+00	U1/2		1.10E+00	8.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1316-T01-C	1	1.10E+00	U1/2		1.10E+00	5.6E+01	2.2E+00	7.0E+00				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1316-T02-C	1	1.10E+00	U1/2		1.10E+00	1.4E+02	2.2E+00	7.0E+00				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1316-T03-C	1	1.10E+00	U1/2		1.10E+00	7.0E+01	2.2E+00	7.0E+00				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1316-T04-C	1	1.10E+00	U1/2		1.10E+00	3.3E+02	2.2E+00	7.0E+00				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1316-B01-A	1	1.10E+00	U1/2		1.10E+00	1.5E+02	2.2E+00	7.0E+00				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	SWA-LRef-1316-T01-A	1	1.58E+04			1.58E+04	6.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1316-T02-A	1	1.11E+04			1.11E+04	3.8E-01	2.6E+00	8.3E+00	1000	100	1.20E+04	86%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1316-T03-A	1	5.76E+03			5.76E+03	3.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1316-T04-A	1	6.61E+03			6.61E+03	5.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1316-T01-B	1	1.48E+04			1.48E+04	5.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1316-T02-B	1	1.11E+04			1.11E+04	4.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1316-T03-B	1	5.91E+03			5.91E+03	2.6E+00	2.6E+00	8.3E+00				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1316-T04-B	1	5.07E+03			5.07E+03	2.5E+00	2.6E+00	8.3E+00				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1316-T01-C	1	1.01E+04			1.01E+04	7.0E+01	2.6E+00	8.3E+00				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1316-T02-C	1	9.83E+03			9.83E+03	4.8E+00	2.6E+00	8.3E+00				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1316-T03-C	1	6.67E+03			6.67E+03	8.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1316-T04-C	1	4.88E+03			4.88E+03	8.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1316-B01-A	1	5.03E+01			5.03E+01	2.9E+01	2.6E+00	8.3E+00				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	SWA-LRef-1316-T01-A	1	1.14E+03			1.14E+03	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1316-T02-A	1	1.82E+03			1.82E+03	4.0E-01	1.2E+00	3.8E+00	10	100	2.67E+03	86%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1316-T03-A	1	3.02E+03			3.02E+03	2.9E-01	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1316-T04-A	1	2.61E+03			2.61E+03	6.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1316-T01-B	1	1.17E+03			1.17E+03	3.5E-01	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1316-T02-B	1	1.80E+03			1.80E+03	4.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1316-T03-B	1	2.44E+03			2.44E+03	2.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1316-T04-B	1	2.96E+03			2.96E+03	1.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1316-T01-C	1	1.17E+03			1.17E+03	6.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1316-T02-C	1	1.61E+03			1.61E+03	4.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1316-T03-C	1	2.35E+03			2.35E+03	9.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1316-T04-C	1	2.74E+03			2.74E+03	1.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	7.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	SWA-LRef-1316-T01-A	1	9.00E-01	U1/2		9.00E-01	2.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1316-T02-A	1	9.00E-01	U1/2		9.00E-01	8.2E+01	1.8E+00	5.7E+00	10	100	1.03E+03	103%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1316-T03-A	1	2.16E+00	E		2.16E+00	4.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1316-T04-A	1	3.41E+00	E		3.41E+00	2.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1316-T01-B	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1316-T02-B	1	9.00E-01	U1/2		9.00E-01	3.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1316-T03-B	1	3.48E+00	E		3.48E+00	2.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1316-T04-B	1	5.50E+00	E		5.50E+00	3.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1316-T01-C	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1316-T02-C	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1316-T03-C	1	2.27E+00	E		2.27E+00	3.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1316-T04-C	1	4.66E+00	E		4.66E+00	7.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	1.8E+02	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	SWA-LRef-1316-T01-A	1	1.85E+00	U1/2		1.85E+00	2.6E+02	3.7E+00	1.2E+01				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1316-T02-A	1	5.18E+00	E		5.18E+00	1.8E+01	3.7E+00	1.2E+01	10	100	1.02E+03	101%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1316-T03-A	1	1.98E+01			1.98E+01	2.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1316-T04-A	1	4.82E+01			4.82E+01	7.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1316-T01-B	1	1.85E+00	U1/2		1.85E+00	7.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1316-T02-B	1	4.07E+00	E		4.07E+00	2.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1316-T03-B	1	1.57E+01			1.57E+01	1.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1316-T04-B	1	4.64E+01			4.64E+01	8.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1316-T01-C	1	1.85E+00	U1/2		1.85E+00	1.3E+03	3.7E+00	1.2E+01				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1316-T02-C	1	4.40E+00	E		4.40E+00	6.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1316-T03-C	1	1.62E+01			1.62E+01	8.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1316-T04-C	1	5.05E+01			5.05E+01	4.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	3.7E+03	3.7E+00	1.2E+01				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	SWA-LRef-1316-T01-A	1	8.37E+01			8.37E+01	2.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1316-T02-A	1	1.81E+02			1.81E+02	7.7E-01	2.0E+00	6.4E+00	1000	100	1.23E+03	105%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1316-T03-A	1	5.72E+02			5.72E+02	1.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1316-T04-A	1	1.21E+03			1.21E+03	1.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1316-T01-B	1	8.80E+01			8.80E+01	2.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1316-T02-B	1	1.77E+02			1.77E+02	4.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1316-T03-B	1	5.32E+02			5.32E+02	9.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1316-T04-B	1	1.32E+03			1.32E+03	1.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1316-T01-C	1	4.81E+01			4.81E+01	7.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1316-T02-C	1	1.47E+02			1.47E+02	5.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1316-T03-C	1	5.00E+02			5.00E+02	6.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1316-T04-C	1	1.16E+03			1.16E+03	5.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	3.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	SWA-LRef-1316-T01-A	1	1.00E+01	E		1.00E+01	2.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1316-T02-A	1	2.95E+01			2.95E+01	2.1E+01	6.8E+00	2.2E+01	10	100	1.04E+03	101%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1316-T03-A	1	6.57E+01			6.57E+01	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1316-T04-A	1	1.46E+02			1.46E+02	2.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1316-T01-B	1	9.23E+00	E		9.23E+00	1.7E+01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1316-T02-B	1	2.30E+01			2.30E+01	1.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1316-T03-B	1	5.47E+01			5.47E+01	9.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1316-T04-B	1	1.42E+02			1.42E+02	5.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1316-T01-C	1	6.88E+00	E		6.88E+00	1.6E+02	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1316-T02-C	1	2.92E+01			2.92E+01	4.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1316-T03-C	1	6.87E+01			6.87E+01	1.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1316-T04-C	1	1.51E+02			1.51E+02	4.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	2.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	SWA-LRef-1316-T01-A	1	1.94E+00	E		1.94E+00	6.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1316-T02-A	1	3.64E+00	E		3.64E+00	1.4E+01	1.9E+00	6.0E+00	10	100	8.61E+02	86%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1316-T03-A	1	8.04E+00			8.04E+00	7.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1316-T04-A	1	1.15E+01			1.15E+01	1.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1316-T01-B	1	2.24E+00	E		2.24E+00	6.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1316-T02-B	1	3.40E+00	E		3.40E+00	2.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1316-T03-B	1	8.29E+00			8.29E+00	9.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1316-T04-B	1	9.65E+00			9.65E+00	1.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1316-T01-C	1	2.00E+00	E		2.00E+00	1.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1316-T02-C	1	3.82E+00	E		3.82E+00	2.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1316-T03-C	1	8.44E+00			8.44E+00	2.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1316-T04-C	1	1.08E+01			1.08E+01	1.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	1.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	SWA-LRef-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	3.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	2.6E+00	2.0E+00	6.4E+00	10	100	1.01E+03	101%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	4.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1316-T04-A	1	2.17E+00	E		2.17E+00	3.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	4.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	8.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	8.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1316-T04-B	1	4.11E+00	E		4.11E+00	6.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	7.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1316-T04-C	1	3.41E+00	E		3.41E+00	1.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	3.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	SWA-LRef-1316-T01-A	1	5.00E-01	U1/2		5.00E-01	6.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1316-T02-A	1	5.00E-01	U1/2		5.00E-01	4.6E+01	1.0E+00	3.2E+00	1000	100	1.03E+03	103%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1316-T03-A	1	6.75E+00			6.75E+00	1.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1316-T04-A	1	6.38E+00			6.38E+00	2.6E+03	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1316-T01-B	1	5.00E-01	U1/2		5.00E-01	1.0E+02	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1316-T02-B	1	5.00E-01	U1/2		5.00E-01	5.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1316-T03-B	1	1.46E+01			1.46E+01	9.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1316-T04-B	1	1.04E+01			1.04E+01	8.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1316-T01-C	1	5.00E-01	U1/2		5.00E-01	1.5E+02	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1316-T02-C	1	5.00E-01	U1/2		5.00E-01	1.3E+03	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1316-T03-C	1	4.72E+00			4.72E+00	2.5E+02	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1316-T04-C	1	5.98E+00			5.98E+00	1.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1316-B01-A	1	1.68E+01			1.68E+01	6.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	SWA-LRef-1316-T01-A	1	1.42E+02			1.42E+02	7.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1316-T02-A	1	2.67E+02			2.67E+02	5.9E-01	1.2E+00	3.8E+00	10	100	1.31E+03	105%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1316-T03-A	1	6.69E+02			6.69E+02	4.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1316-T04-A	1	1.30E+03			1.30E+03	3.6E-02	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1316-T01-B	1	1.37E+02			1.37E+02	9.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1316-T02-B	1	2.53E+02			2.53E+02	4.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1316-T03-B	1	6.10E+02			6.10E+02	8.2E-01	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1316-T04-B	1	1.28E+03			1.28E+03	7.8E-01	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1316-T01-C	1	1.35E+02			1.35E+02	6.8E+01	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1316-T02-C	1	2.45E+02			2.45E+02	4.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1316-T03-C	1	5.86E+02			5.86E+02	5.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1316-T04-C	1	1.17E+03			1.17E+03	4.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1316-B01-A	1	1.37E+00	E		1.37E+00	8.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	SWA-LRef-1316-T01-A	1	9.00E-01	U1/2		9.00E-01	7.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1316-T02-A	1	9.00E-01	U1/2		9.00E-01	1.8E+02	1.8E+00	5.7E+00	10	100	1.03E+03	103%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1316-T03-A	1	2.23E+00	E		2.23E+00	5.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1316-T04-A	1	5.43E+00	E		5.43E+00	6.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1316-T01-B	1	9.00E-01	U1/2		9.00E-01	3.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1316-T02-B	1	9.00E-01	U1/2		9.00E-01	6.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1316-T03-B	1	2.04E+00	E		2.04E+00	1.7E+02	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1316-T04-B	1	6.06E+00			6.06E+00	2.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1316-T01-C	1	9.00E-01	U1/2		9.00E-01	2.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1316-T02-C	1	9.00E-01	U1/2		9.00E-01	7.2E+02	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1316-T03-C	1	2.33E+00	E		2.33E+00	4.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1316-T04-C	1	5.31E+00	E		5.31E+00	2.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	7.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	SWA-LRef-1316-T01-A	1	2.68E+01			2.68E+01	1.6E+01	3.7E+00	1.2E+01			---		VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1316-T02-A	1	1.04E+02			1.04E+02	9.4E+00	3.7E+00	1.2E+01	1000	100	1.18E+03	107%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1316-T03-A	1	3.27E+02			3.27E+02	6.9E-01	3.7E+00	1.2E+01			---		VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1316-T04-A	1	1.03E+03			1.03E+03	4.2E+00	3.7E+00	1.2E+01			---		VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1316-T01-B	1	2.22E+01			2.22E+01	1.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1316-T02-B	1	9.18E+01			9.18E+01	4.0E+00	3.7E+00	1.2E+01			---		VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1316-T03-B	1	4.36E+02			4.36E+02	1.6E+00	3.7E+00	1.2E+01			---		VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1316-T04-B	1	1.50E+03			1.50E+03	1.6E+00	3.7E+00	1.2E+01			---		VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1316-T01-C	1	2.02E+01			2.02E+01	9.7E+01	3.7E+00	1.2E+01			---		VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1316-T02-C	1	8.35E+01			8.35E+01	4.1E+00	3.7E+00	1.2E+01			---		VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1316-T03-C	1	3.58E+02			3.58E+02	4.8E+00	3.7E+00	1.2E+01			---		VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1316-T04-C	1	1.26E+03			1.26E+03	5.1E+00	3.7E+00	1.2E+01			---		VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1316-B01-A	1	2.18E+00	U1/2		2.18E+00	4.2E+01	3.7E+00	1.2E+01			---		VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	SWA-LRef-1316-T01-A	1	2.72E+05			2.72E+05	1.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1316-T02-A	1	4.33E+05			4.33E+05	4.6E-01	1.6E+00	5.1E+00	1000	100	4.34E+05	92%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1316-T03-A	1	1.75E+06			1.75E+06	8.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1316-T04-A	1	1.83E+06			1.83E+06	4.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1316-T01-B	1	2.63E+05			2.63E+05	2.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1316-T02-B	1	4.16E+05			4.16E+05	4.6E+00	1.6E+00	5.1E+00				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1316-T03-B	1	1.89E+06			1.89E+06	6.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1316-T04-B	1	2.02E+06			2.02E+06	4.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1316-T01-C	1	2.64E+05			2.64E+05	6.8E+01	1.6E+00	5.1E+00				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1316-T02-C	1	4.20E+05			4.20E+05	6.9E+00	1.6E+00	5.1E+00				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1316-T03-C	1	1.85E+06			1.85E+06	2.9E+00	1.6E+00	5.1E+00				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1316-T04-C	1	1.91E+06			1.91E+06	3.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1316-B01-A	1	2.81E+01			2.81E+01	5.0E+01	1.6E+00	5.1E+00				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	SWA-LRef-1316-T01-A	1	9.41E+04			9.41E+04	5.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1316-T02-A	1	1.79E+05			1.79E+05	3.9E-01	1.5E+01	4.8E+01	10	100	1.80E+05	95%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1316-T03-A	1	4.22E+05			4.22E+05	7.1E-01	1.5E+01	4.8E+01				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1316-T04-A	1	7.65E+05			7.65E+05	1.5E-01	1.5E+01	4.8E+01				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1316-T01-B	1	9.00E+04			9.00E+04	3.0E-01	1.5E+01	4.8E+01				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1316-T02-B	1	1.67E+05			1.67E+05	4.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1316-T03-B	1	4.55E+05			4.55E+05	9.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1316-T04-B	1	8.58E+05			8.58E+05	7.2E-01	1.5E+01	4.8E+01				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1316-T01-C	1	9.57E+04			9.57E+04	7.0E+01	1.5E+01	4.8E+01				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1316-T02-C	1	1.69E+05			1.69E+05	4.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1316-T03-C	1	4.06E+05			4.06E+05	5.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1316-T04-C	1	7.94E+05			7.94E+05	4.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1316-B01-A	1	7.50E+00	U1/2		7.50E+00	7.7E+01	1.5E+01	4.8E+01				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	SWA-LRef-1316-T01-A	1	2.30E+04			2.30E+04	4.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1316-T02-A	1	3.07E+04			3.07E+04	1.1E+00	1.1E+00	3.5E+00	1000	100	3.17E+04	97%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1316-T03-A	1	3.97E+04			3.97E+04	2.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1316-T04-A	1	6.13E+04			6.13E+04	1.6E+00	1.1E+00	3.5E+00				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1316-T01-B	1	2.12E+04			2.12E+04	1.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1316-T02-B	1	3.07E+04			3.07E+04	3.7E+00	1.1E+00	3.5E+00				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1316-T03-B	1	4.42E+04			4.42E+04	1.9E+00	1.1E+00	3.5E+00				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1316-T04-B	1	6.32E+04			6.32E+04	7.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1316-T01-C	1	2.30E+04			2.30E+04	6.6E+01	1.1E+00	3.5E+00				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1316-T02-C	1	2.95E+04			2.95E+04	4.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1316-T03-C	1	4.17E+04			4.17E+04	5.9E+00	1.1E+00	3.5E+00				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1316-T04-C	1	6.04E+04			6.04E+04	4.5E+00	1.1E+00	3.5E+00				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1316-B01-A	1	5.50E-01	U1/2		5.50E-01	9.1E+01	1.1E+00	3.5E+00				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	SWA-LRef-1316-T01-A	1	3.59E+05			3.59E+05	5.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1316-T02-A	1	4.50E+05			4.50E+05	3.4E-01	2.5E+00	8.0E+00	1000	100	4.51E+05	94%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1316-T03-A	1	5.27E+05			5.27E+05	6.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1316-T04-A	1	5.37E+05			5.37E+05	9.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1316-T01-B	1	3.55E+05			3.55E+05	6.2E-02	2.5E+00	8.0E+00				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1316-T02-B	1	4.45E+05			4.45E+05	3.4E+00	2.5E+00	8.0E+00				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1316-T03-B	1	5.12E+05			5.12E+05	5.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1316-T04-B	1	5.16E+05			5.16E+05	3.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1316-T01-C	1	2.86E+05			2.86E+05	5.7E+01	2.5E+00	8.0E+00				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1316-T02-C	1	4.42E+05			4.42E+05	3.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1316-T03-C	1	5.13E+05			5.13E+05	3.4E+00	2.5E+00	8.0E+00				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1316-T04-C	1	5.16E+05			5.16E+05	2.9E+00	2.5E+00	8.0E+00				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1316-B01-A	1	2.06E+01			2.06E+01	6.2E+02	2.5E+00	8.0E+00				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	SWA-LRef-1316-T01-A	1	4.04E+02			4.04E+02	4.2E-02	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1316-T02-A	1	3.68E+02			3.68E+02	2.4E-01	1.0E+00	3.2E+00	1000	100	1.40E+03	104%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1316-T03-A	1	4.81E+02			4.81E+02	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1316-T04-A	1	4.34E+02			4.34E+02	9.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1316-T01-B	1	3.92E+02			3.92E+02	2.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1316-T02-B	1	3.65E+02			3.65E+02	4.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1316-T03-B	1	3.93E+02			3.93E+02	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1316-T04-B	1	4.32E+02			4.32E+02	3.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1316-T01-C	1	2.95E+02			2.95E+02	7.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1316-T02-C	1	3.70E+02			3.70E+02	3.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1316-T03-C	1	3.84E+02			3.84E+02	5.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1316-T04-C	1	4.26E+02			4.26E+02	5.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	2.4E+03	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	SWA-LRef-1316-T01-A	1	4.68E+05			4.68E+05	9.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1316-T02-A	1	7.47E+05			7.47E+05	1.7E-01	6.8E+00	2.2E+01	1000	100	7.48E+05	84%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1316-T03-A	1	1.49E+06			1.49E+06	3.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1316-T04-A	1	2.02E+06			2.02E+06	6.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1316-T01-B	1	4.63E+05			4.63E+05	3.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1316-T02-B	1	6.10E+05			6.10E+05	4.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1316-T03-B	1	1.26E+06			1.26E+06	8.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1316-T04-B	1	2.00E+06			2.00E+06	8.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1316-T01-C	1	4.52E+05			4.52E+05	6.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1316-T02-C	1	6.02E+05			6.02E+05	4.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1316-T03-C	1	1.12E+06			1.12E+06	5.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1316-T04-C	1	1.87E+06			1.87E+06	4.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	7.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	SWA-LRef-1316-T01-A	1	2.30E+00	U1/2		2.30E+00	3.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1316-T02-A	1	2.30E+00	U1/2		2.30E+00	2.4E+02	4.6E+00	1.5E+01	10	100	9.35E+02	93%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1316-T03-A	1	2.30E+00	U1/2		2.30E+00	8.0E+02	4.6E+00	1.5E+01				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1316-T04-A	1	2.30E+00	U1/2		2.30E+00	1.1E+02	4.6E+00	1.5E+01				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1316-T01-B	1	2.30E+00	U1/2		2.30E+00	6.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1316-T02-B	1	2.30E+00	U1/2		2.30E+00	3.4E+01	4.6E+00	1.5E+01				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1316-T03-B	1	2.30E+00	U1/2		2.30E+00	1.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1316-T04-B	1	2.30E+00	U1/2		2.30E+00	1.7E+02	4.6E+00	1.5E+01				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1316-T01-C	1	2.30E+00	U1/2		2.30E+00	1.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1316-T02-C	1	2.30E+00	U1/2		2.30E+00	4.5E+01	4.6E+00	1.5E+01				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1316-T03-C	1	2.30E+00	U1/2		2.30E+00	1.0E+02	4.6E+00	1.5E+01				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1316-T04-C	1	2.30E+00	U1/2		2.30E+00	1.2E+03	4.6E+00	1.5E+01				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1316-B01-A	1	2.30E+00	U1/2		2.30E+00	5.5E+01	4.6E+00	1.5E+01				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	SWA-LRef-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00	10	100	1.01E+03	100%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	9.2E-02	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1316-T04-A	1	3.11E+00	E		3.11E+00	8.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	3.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	6.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	6.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1316-T04-B	1	4.81E+00	E		4.81E+00	2.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	6.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	3.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	5.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1316-T04-C	1	3.02E+00	E		3.02E+00	1.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	SWA-LRef-1316-T01-A	1	3.25E+02			3.25E+02	7.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1316-T02-A	1	5.94E+02			5.94E+02	1.4E-01	1.5E+00	4.8E+00	10	100	1.61E+03	101%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1316-T03-A	1	1.22E+03			1.22E+03	9.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1316-T04-A	1	2.14E+03			2.14E+03	8.0E-01	1.5E+00	4.8E+00				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1316-T01-B	1	3.10E+02			3.10E+02	9.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1316-T02-B	1	5.60E+02			5.60E+02	4.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1316-T03-B	1	1.17E+03			1.17E+03	2.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1316-T04-B	1	2.32E+03			2.32E+03	1.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1316-T01-C	1	2.84E+02			2.84E+02	6.9E+01	1.5E+00	4.8E+00				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1316-T02-C	1	5.36E+02			5.36E+02	3.9E+00	1.5E+00	4.8E+00				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1316-T03-C	1	1.18E+03			1.18E+03	6.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1316-T04-C	1	2.04E+03			2.04E+03	4.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1316-B01-A	1	7.50E-01	U1/2		7.50E-01	1.0E+02	1.5E+00	4.8E+00				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	SWA-LRef-1316-T01-A	1	5.00E-01	U1/2		5.00E-01	3.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:26 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1316-T02-A	1	2.41E+00	E		2.41E+00	1.1E+01	1.0E+00	3.2E+00	10	100	1.09E+03	108%	VU ICP-OES	10/26/10 2:27 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1316-T03-A	1	3.81E+00			3.81E+00	5.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:29 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1316-T04-A	1	1.15E+01			1.15E+01	7.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:31 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1316-T01-B	1	5.00E-01	U1/2		5.00E-01	1.0E+02	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:32 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1316-T02-B	1	1.99E+00	E		1.99E+00	2.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:34 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1316-T03-B	1	4.01E+00			4.01E+00	1.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:36 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1316-T04-B	1	1.38E+01			1.38E+01	4.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:37 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1316-T01-C	1	5.00E-01	U1/2		5.00E-01	9.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:39 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1316-T02-C	1	2.08E+00	E		2.08E+00	7.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:41 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1316-T03-C	1	5.16E+00			5.16E+00	1.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:42 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1316-T04-C	1	1.32E+01			1.32E+01	6.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:44 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	2.1E+02	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:16 PM	EPA Interlab LRef 1313-1316 SWA

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	SWA-LRef-1316-T01-D	1	3.08E+04			3.08E+04	4.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1316-T02-D	1	5.30E+04			5.30E+04	1.3E+00	1.0E+00	3.2E+00	1000	100	5.39E+04	90%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1316-T03-D	1	1.06E+05			1.06E+05	5.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1316-T04-D	1	1.71E+05			1.71E+05	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1316-T01-E	1	2.17E+04			2.17E+04	6.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1316-T02-E	1	5.10E+04			5.10E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1316-T03-E	1	1.07E+05			1.07E+05	2.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1316-T04-E	1	1.68E+05			1.68E+05	3.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1316-T01-F	1	3.53E+04			3.53E+04	8.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1316-T02-F	1	5.04E+04			5.04E+04	9.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1316-T03-F	1	6.93E+04			6.93E+04	6.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1316-T04-F	1	1.67E+05			1.67E+05	9.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
Al	SWA-LRef-1316-B01-D	1	5.00E-01	U1/2		5.00E-01	6.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	SWA-LRef-1316-T01-D	1	5.64E+03			5.64E+03	6.3E-01	7.5E+00	2.4E+01				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1316-T02-D	1	5.88E+03			5.88E+03	7.8E-01	7.5E+00	2.4E+01	10	100	6.86E+03	99%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1316-T03-D	1	5.93E+03			5.93E+03	2.8E-01	7.5E+00	2.4E+01				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1316-T04-D	1	7.22E+03			7.22E+03	2.9E+00	7.5E+00	2.4E+01				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1316-T01-E	1	5.16E+03			5.16E+03	6.9E+01	7.5E+00	2.4E+01				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1316-T02-E	1	5.26E+03			5.26E+03	1.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1316-T03-E	1	6.22E+03			6.22E+03	7.1E-01	7.5E+00	2.4E+01				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1316-T04-E	1	5.74E+03			5.74E+03	3.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1316-T01-F	1	5.99E+03			5.99E+03	1.5E-01	7.5E+00	2.4E+01				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1316-T02-F	1	5.89E+03			5.89E+03	8.2E-01	7.5E+00	2.4E+01				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1316-T03-F	1	5.81E+03			5.81E+03	6.8E+01	7.5E+00	2.4E+01				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1316-T04-F	1	5.63E+03			5.63E+03	1.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
Sb	SWA-LRef-1316-B01-D	1	3.75E+00	U1/2		3.75E+00	1.6E+02	7.5E+00	2.4E+01				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	SWA-LRef-1316-T01-D	1	4.89E+03			4.89E+03	5.2E-01	1.1E+01	3.5E+01				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1316-T02-D	1	1.13E+04			1.13E+04	1.8E+00	1.1E+01	3.5E+01	10	100	1.23E+04	105%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1316-T03-D	1	3.93E+04			3.93E+04	4.1E-01	1.1E+01	3.5E+01				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1316-T04-D	1	1.09E+05			1.09E+05	2.4E+00	1.1E+01	3.5E+01				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1316-T01-E	1	4.74E+03			4.74E+03	7.0E+01	1.1E+01	3.5E+01				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1316-T02-E	1	9.69E+03			9.69E+03	1.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1316-T03-E	1	3.84E+04			3.84E+04	9.2E-01	1.1E+01	3.5E+01				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1316-T04-E	1	1.01E+05			1.01E+05	4.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1316-T01-F	1	5.12E+03			5.12E+03	8.2E-01	1.1E+01	3.5E+01				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1316-T02-F	1	1.12E+04			1.12E+04	7.3E-01	1.1E+01	3.5E+01				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1316-T03-F	1	2.73E+04			2.73E+04	6.1E+01	1.1E+01	3.5E+01				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1316-T04-F	1	9.76E+04			9.76E+04	7.7E-01	1.1E+01	3.5E+01				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
As	SWA-LRef-1316-B01-D	1	1.36E+01	E		1.36E+01	1.9E+02	1.1E+01	3.5E+01				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	SWA-LRef-1316-T01-D	1	1.13E+03			1.13E+03	8.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1316-T02-D	1	9.26E+02			9.26E+02	1.3E+00	1.0E+00	3.2E+00	1000	100	1.98E+03	105%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1316-T03-D	1	6.42E+02			6.42E+02	2.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1316-T04-D	1	7.30E+02			7.30E+02	2.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1316-T01-E	1	1.03E+03			1.03E+03	6.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1316-T02-E	1	9.31E+02			9.31E+02	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1316-T03-E	1	6.50E+02			6.50E+02	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1316-T04-E	1	6.98E+02			6.98E+02	4.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1316-T01-F	1	1.16E+03			1.16E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1316-T02-F	1	9.19E+02			9.19E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1316-T03-F	1	6.54E+02			6.54E+02	6.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1316-T04-F	1	7.27E+02			7.27E+02	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
B	SWA-LRef-1316-B01-D	1	6.89E+00			6.89E+00	8.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	SWA-LRef-1316-T01-D	1	1.35E+02			1.35E+02	2.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1316-T02-D	1	1.45E+02			1.45E+02	6.7E-01	1.0E+00	3.2E+00	10	100	1.08E+03	93%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1316-T03-D	1	1.41E+02			1.41E+02	4.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1316-T04-D	1	1.34E+02			1.34E+02	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1316-T01-E	1	1.08E+02			1.08E+02	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1316-T02-E	1	1.79E+02			1.79E+02	8.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1316-T03-E	1	1.52E+02			1.52E+02	3.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1316-T04-E	1	1.32E+02			1.32E+02	4.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1316-T01-F	1	1.62E+02			1.62E+02	2.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1316-T02-F	1	1.43E+02			1.43E+02	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1316-T03-F	1	1.32E+02			1.32E+02	6.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1316-T04-F	1	1.19E+02			1.19E+02	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
Ba	SWA-LRef-1316-B01-D	1	5.00E-01	U1/2		5.00E-01	2.2E+02	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	SWA-LRef-1316-T01-D	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1316-T02-D	1	9.50E-01	U1/2		9.50E-01	7.6E+01	1.9E+00	6.0E+00	10	100	1.11E+03	111%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1316-T03-D	1	9.50E-01	U1/2		9.50E-01	2.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1316-T04-D	1	9.50E-01	U1/2		9.50E-01	5.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1316-T01-E	1	9.50E-01	U1/2		9.50E-01	2.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1316-T02-E	1	9.50E-01	U1/2		9.50E-01	8.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1316-T03-E	1	9.50E-01	U1/2		9.50E-01	1.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1316-T04-E	1	9.50E-01	U1/2		9.50E-01	4.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1316-T01-F	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1316-T02-F	1	9.50E-01	U1/2		9.50E-01	7.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1316-T03-F	1	9.50E-01	U1/2		9.50E-01	6.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1316-T04-F	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
Be	SWA-LRef-1316-B01-D	1	9.50E-01	U1/2		9.50E-01	9.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	SWA-LRef-1316-T01-D	1	1.10E+00	U1/2		1.10E+00	1.6E+02	2.2E+00	7.0E+00				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1316-T02-D	1	1.10E+00	U1/2		1.10E+00	9.1E+02	2.2E+00	7.0E+00	10	100	1.11E+03	111%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1316-T03-D	1	1.10E+00	U1/2		1.10E+00	4.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1316-T04-D	1	1.10E+00	U1/2		1.10E+00	1.5E+02	2.2E+00	7.0E+00				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1316-T01-E	1	1.10E+00	U1/2		1.10E+00	4.2E+02	2.2E+00	7.0E+00				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1316-T02-E	1	1.10E+00	U1/2		1.10E+00	8.5E+02	2.2E+00	7.0E+00				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1316-T03-E	1	1.10E+00	U1/2		1.10E+00	2.8E+02	2.2E+00	7.0E+00				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1316-T04-E	1	1.10E+00	U1/2		1.10E+00	6.5E+02	2.2E+00	7.0E+00				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1316-T01-F	1	1.10E+00	U1/2		1.10E+00	1.2E+02	2.2E+00	7.0E+00				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1316-T02-F	1	1.10E+00	U1/2		1.10E+00	8.1E+02	2.2E+00	7.0E+00				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1316-T03-F	1	1.10E+00	U1/2		1.10E+00	1.9E+02	2.2E+00	7.0E+00				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1316-T04-F	1	1.10E+00	U1/2		1.10E+00	8.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
Cd	SWA-LRef-1316-B01-D	1	1.10E+00	U1/2		1.10E+00	3.0E+02	2.2E+00	7.0E+00				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	SWA-LRef-1316-T01-D	1	1.04E+04			1.04E+04	6.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1316-T02-D	1	1.12E+04			1.12E+04	6.6E-01	2.6E+00	8.3E+00	1000	100	1.21E+04	90%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1316-T03-D	1	6.54E+03			6.54E+03	4.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1316-T04-D	1	5.08E+03			5.08E+03	4.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1316-T01-E	1	8.89E+03			8.89E+03	6.9E+01	2.6E+00	8.3E+00				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1316-T02-E	1	1.21E+04			1.21E+04	5.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1316-T03-E	1	6.43E+03			6.43E+03	2.5E+00	2.6E+00	8.3E+00				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1316-T04-E	1	4.61E+03			4.61E+03	9.7E+00	2.6E+00	8.3E+00				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1316-T01-F	1	1.40E+04			1.40E+04	1.6E+00	2.6E+00	8.3E+00				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1316-T02-F	1	9.08E+03			9.08E+03	7.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1316-T03-F	1	6.05E+03			6.05E+03	6.9E+01	2.6E+00	8.3E+00				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1316-T04-F	1	4.56E+03			4.56E+03	2.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
Ca	SWA-LRef-1316-B01-D	1	4.86E+01			4.86E+01	2.5E+01	2.6E+00	8.3E+00				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	SWA-LRef-1316-T01-D	1	9.14E+02			9.14E+02	1.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1316-T02-D	1	2.03E+03			2.03E+03	7.7E-01	1.2E+00	3.8E+00	10	100	2.90E+03	87%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1316-T03-D	1	2.88E+03			2.88E+03	4.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1316-T04-D	1	3.16E+03			3.16E+03	3.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1316-T01-E	1	9.54E+02			9.54E+02	6.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1316-T02-E	1	1.59E+03			1.59E+03	2.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1316-T03-E	1	2.48E+03			2.48E+03	1.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1316-T04-E	1	2.68E+03			2.68E+03	1.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1316-T01-F	1	1.12E+03			1.12E+03	3.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1316-T02-F	1	1.94E+03			1.94E+03	3.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1316-T03-F	1	2.46E+03			2.46E+03	6.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1316-T04-F	1	2.95E+03			2.95E+03	4.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
Cr	SWA-LRef-1316-B01-D	1	6.00E-01	U1/2		6.00E-01	1.0E+03	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	SWA-LRef-1316-T01-D	1	9.00E-01	U1/2		9.00E-01	2.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1316-T02-D	1	9.00E-01	U1/2		9.00E-01	3.8E+02	1.8E+00	5.7E+00	10	100	1.12E+03	112%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1316-T03-D	1	2.66E+00	E		2.66E+00	3.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1316-T04-D	1	6.53E+00			6.53E+00	1.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1316-T01-E	1	9.00E-01	U1/2		9.00E-01	2.3E+03	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1316-T02-E	1	9.00E-01	U1/2		9.00E-01	5.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1316-T03-E	1	2.52E+00	E		2.52E+00	3.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1316-T04-E	1	5.16E+00	E		5.16E+00	1.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1316-T01-F	1	9.00E-01	U1/2		9.00E-01	1.8E+02	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1316-T02-F	1	9.00E-01	U1/2		9.00E-01	5.6E+02	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1316-T03-F	1	2.51E+00	E		2.51E+00	1.2E+02	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1316-T04-F	1	5.18E+00	E		5.18E+00	4.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
Co	SWA-LRef-1316-B01-D	1	9.00E-01	U1/2		9.00E-01	2.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	SWA-LRef-1316-T01-D	1	1.85E+00	U1/2		1.85E+00	5.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1316-T02-D	1	8.08E+00	E		8.08E+00	1.5E+01	3.7E+00	1.2E+01	10	100	1.12E+03	111%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1316-T03-D	1	2.51E+01			2.51E+01	6.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1316-T04-D	1	5.74E+01			5.74E+01	2.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1316-T01-E	1	1.85E+00	U1/2		1.85E+00	2.3E+02	3.7E+00	1.2E+01				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1316-T02-E	1	6.18E+00	E		6.18E+00	3.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1316-T03-E	1	2.16E+01			2.16E+01	2.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1316-T04-E	1	5.82E+01			5.82E+01	7.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1316-T01-F	1	1.85E+00	U1/2		1.85E+00	2.4E+02	3.7E+00	1.2E+01				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1316-T02-F	1	5.23E+00	E		5.23E+00	1.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1316-T03-F	1	2.64E+01			2.64E+01	7.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1316-T04-F	1	4.41E+01			4.41E+01	3.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
Cu	SWA-LRef-1316-B01-D	1	1.85E+00	U1/2		1.85E+00	1.5E+02	3.7E+00	1.2E+01				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	SWA-LRef-1316-T01-D	1	4.79E+01			4.79E+01	2.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1316-T02-D	1	1.65E+02			1.65E+02	5.0E-01	2.0E+00	6.4E+00	1000	100	1.32E+03	115%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1316-T03-D	1	5.84E+02			5.84E+02	2.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1316-T04-D	1	1.25E+03			1.25E+03	1.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1316-T01-E	1	3.98E+01			3.98E+01	7.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1316-T02-E	1	1.48E+02			1.48E+02	6.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1316-T03-E	1	5.75E+02			5.75E+02	1.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1316-T04-E	1	1.19E+03			1.19E+03	5.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1316-T01-F	1	8.86E+01			8.86E+01	3.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1316-T02-F	1	1.56E+02			1.56E+02	2.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1316-T03-F	1	5.72E+02			5.72E+02	6.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1316-T04-F	1	1.35E+03			1.35E+03	1.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
Fe	SWA-LRef-1316-B01-D	1	1.00E+00	U1/2		1.00E+00	2.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	SWA-LRef-1316-T01-D	1	9.12E+00	E		9.12E+00	3.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1316-T02-D	1	1.90E+01	E		1.90E+01	9.9E+00	6.8E+00	2.2E+01	10	100	1.13E+03	111%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1316-T03-D	1	6.83E+01			6.83E+01	5.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1316-T04-D	1	1.62E+02			1.62E+02	4.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1316-T01-E	1	8.06E+00	E		8.06E+00	1.0E+03	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1316-T02-E	1	2.90E+01			2.90E+01	3.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1316-T03-E	1	9.01E+01			9.01E+01	3.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1316-T04-E	1	1.82E+02			1.82E+02	5.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1316-T01-F	1	1.35E+01	E		1.35E+01	1.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1316-T02-F	1	1.87E+01	E		1.87E+01	8.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1316-T03-F	1	7.90E+01			7.90E+01	9.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1316-T04-F	1	1.51E+02			1.51E+02	4.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
Pb	SWA-LRef-1316-B01-D	1	3.40E+00	U1/2		3.40E+00	3.3E+01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	SWA-LRef-1316-T01-D	1	2.83E+00	E		2.83E+00	1.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1316-T02-D	1	3.70E+00	E		3.70E+00	2.4E+01	1.9E+00	6.0E+00	10	100	8.34E+02	83%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1316-T03-D	1	8.20E+00			8.20E+00	1.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1316-T04-D	1	9.63E+00			9.63E+00	1.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1316-T01-E	1	2.19E+00	E		2.19E+00	3.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1316-T02-E	1	3.71E+00	E		3.71E+00	1.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1316-T03-E	1	7.83E+00			7.83E+00	1.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1316-T04-E	1	9.34E+00			9.34E+00	1.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1316-T01-F	1	2.41E+00	E		2.41E+00	9.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1316-T02-F	1	3.51E+00	E		3.51E+00	8.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1316-T03-F	1	8.22E+00			8.22E+00	2.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1316-T04-F	1	9.90E+00			9.90E+00	2.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
Li	SWA-LRef-1316-B01-D	1	9.50E-01	U1/2		9.50E-01	1.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	SWA-LRef-1316-T01-D	1	1.00E+00	U1/2		1.00E+00	6.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1316-T02-D	1	1.00E+00	U1/2		1.00E+00	4.9E+00	2.0E+00	6.4E+00	10	100	1.10E+03	110%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1316-T03-D	1	1.00E+00	U1/2		1.00E+00	3.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1316-T04-D	1	3.88E+00	E		3.88E+00	5.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1316-T01-E	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1316-T02-E	1	1.00E+00	U1/2		1.00E+00	3.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1316-T03-E	1	1.00E+00	U1/2		1.00E+00	5.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1316-T04-E	1	5.39E+00	E		5.39E+00	8.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1316-T01-F	1	1.00E+00	U1/2		1.00E+00	1.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1316-T02-F	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1316-T03-F	1	1.00E+00	U1/2		1.00E+00	7.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1316-T04-F	1	5.31E+00	E		5.31E+00	3.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
Mn	SWA-LRef-1316-B01-D	1	1.00E+00	U1/2		1.00E+00	2.6E+02	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	SWA-LRef-1316-T01-D	1	5.00E-01	U1/2		5.00E-01	2.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1316-T02-D	1	5.00E-01	U1/2		5.00E-01	1.1E+02	1.0E+00	3.2E+00	1000	100	1.12E+03	112%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1316-T03-D	1	7.60E+00			7.60E+00	1.9E+03	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1316-T04-D	1	7.44E+00			7.44E+00	1.8E+03	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1316-T01-E	1	5.00E-01	U1/2		5.00E-01	9.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1316-T02-E	1	5.00E-01	U1/2		5.00E-01	3.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1316-T03-E	1	6.92E+00			6.92E+00	1.1E+02	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1316-T04-E	1	7.91E+00			7.91E+00	6.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1316-T01-F	1	5.00E-01	U1/2		5.00E-01	2.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1316-T02-F	1	5.00E-01	U1/2		5.00E-01	8.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1316-T03-F	1	7.69E+00			7.69E+00	4.5E+02	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1316-T04-F	1	1.14E+01			1.14E+01	9.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
Mg	SWA-LRef-1316-B01-D	1	2.18E+00	E		2.18E+00	4.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	SWA-LRef-1316-T01-D	1	1.64E+02			1.64E+02	1.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1316-T02-D	1	2.54E+02			2.54E+02	8.9E-01	1.2E+00	3.8E+00	10	100	1.39E+03	113%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1316-T03-D	1	6.32E+02			6.32E+02	1.6E-01	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1316-T04-D	1	1.21E+03			1.21E+03	2.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1316-T01-E	1	1.79E+02			1.79E+02	6.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1316-T02-E	1	2.48E+02			2.48E+02	8.7E-01	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1316-T03-E	1	6.61E+02			6.61E+02	2.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1316-T04-E	1	1.20E+03			1.20E+03	4.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1316-T01-F	1	1.62E+02			1.62E+02	9.3E-02	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1316-T02-F	1	2.58E+02			2.58E+02	6.0E-01	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1316-T03-F	1	6.21E+02			6.21E+02	6.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1316-T04-F	1	1.30E+03			1.30E+03	1.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
Mo	SWA-LRef-1316-B01-D	1	6.00E-01	U1/2		6.00E-01	1.2E+02	1.2E+00	3.8E+00				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	SWA-LRef-1316-T01-D	1	9.00E-01	U1/2		9.00E-01	2.7E+02	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1316-T02-D	1	9.00E-01	U1/2		9.00E-01	2.6E+02	1.8E+00	5.7E+00	10	100	1.12E+03	112%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1316-T03-D	1	1.82E+00	E		1.82E+00	8.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1316-T04-D	1	6.84E+00			6.84E+00	2.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1316-T01-E	1	9.00E-01	U1/2		9.00E-01	5.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1316-T02-E	1	9.00E-01	U1/2		9.00E-01	1.7E+02	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1316-T03-E	1	3.06E+00	E		3.06E+00	4.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1316-T04-E	1	4.04E+00	E		4.04E+00	3.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1316-T01-F	1	9.00E-01	U1/2		9.00E-01	3.8E+02	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1316-T02-F	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1316-T03-F	1	2.37E+00	E		2.37E+00	2.9E+02	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1316-T04-F	1	5.57E+00	E		5.57E+00	3.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
Ni	SWA-LRef-1316-B01-D	1	9.00E-01	U1/2		9.00E-01	4.7E+02	1.8E+00	5.7E+00				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	SWA-LRef-1316-T01-D	1	2.87E+01			2.87E+01	1.6E+01	3.7E+00	1.2E+01			---		VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1316-T02-D	1	8.41E+01			8.41E+01	1.6E+01	3.7E+00	1.2E+01	1000	100	1.22E+03	113%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1316-T03-D	1	3.04E+02			3.04E+02	1.5E+00	3.7E+00	1.2E+01			---		VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1316-T04-D	1	1.30E+03			1.30E+03	3.1E+00	3.7E+00	1.2E+01			---		VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1316-T01-E	1	2.11E+01			2.11E+01	1.1E+02	3.7E+00	1.2E+01			---		VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1316-T02-E	1	7.44E+01			7.44E+01	8.0E+00	3.7E+00	1.2E+01			---		VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1316-T03-E	1	2.90E+02			2.90E+02	3.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1316-T04-E	1	1.19E+03			1.19E+03	3.4E+00	3.7E+00	1.2E+01			---		VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1316-T01-F	1	2.04E+01			2.04E+01	7.7E+00	3.7E+00	1.2E+01			---		VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1316-T02-F	1	7.84E+01			7.84E+01	2.6E+00	3.7E+00	1.2E+01			---		VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1316-T03-F	1	2.41E+02			2.41E+02	6.8E+01	3.7E+00	1.2E+01			---		VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1316-T04-F	1	9.88E+02			9.88E+02	1.8E+00	3.7E+00	1.2E+01			---		VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
P	SWA-LRef-1316-B01-D	1	4.81E+00	E		4.81E+00	1.8E+02	3.7E+00	1.2E+01			---		VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	SWA-LRef-1316-T01-D	1	2.70E+05			2.70E+05	7.0E-01	1.6E+00	5.1E+00			---		VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1316-T02-D	1	4.28E+05			4.28E+05	2.3E+00	1.6E+00	5.1E+00	1000	100	4.29E+05	92%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1316-T03-D	1	1.70E+06			1.70E+06	2.7E-01	1.6E+00	5.1E+00			---		VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1316-T04-D	1	1.99E+06			1.99E+06	1.9E+00	1.6E+00	5.1E+00			---		VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1316-T01-E	1	2.63E+05			2.63E+05	6.7E+01	1.6E+00	5.1E+00			---		VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1316-T02-E	1	4.30E+05			4.30E+05	1.2E+00	1.6E+00	5.1E+00			---		VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1316-T03-E	1	1.72E+06			1.72E+06	1.0E+00	1.6E+00	5.1E+00			---		VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1316-T04-E	1	1.96E+06			1.96E+06	4.5E+00	1.6E+00	5.1E+00			---		VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1316-T01-F	1	2.74E+05			2.74E+05	2.3E+00	1.6E+00	5.1E+00			---		VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1316-T02-F	1	4.38E+05			4.38E+05	2.9E+00	1.6E+00	5.1E+00			---		VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1316-T03-F	1	1.69E+06			1.69E+06	7.7E+01	1.6E+00	5.1E+00			---		VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1316-T04-F	1	1.81E+06			1.81E+06	6.2E-01	1.6E+00	5.1E+00			---		VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
K	SWA-LRef-1316-B01-D	1	6.57E+00			6.57E+00	2.7E+02	1.6E+00	5.1E+00			---		VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	SWA-LRef-1316-T01-D	1	1.07E+05			1.07E+05	4.9E-01	1.5E+01	4.8E+01			---		VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1316-T02-D	1	1.75E+05			1.75E+05	1.0E+00	1.5E+01	4.8E+01	10	100	1.76E+05	99%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1316-T03-D	1	4.01E+05			4.01E+05	2.6E-01	1.5E+01	4.8E+01			---		VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1316-T04-D	1	8.11E+05			8.11E+05	2.3E+00	1.5E+01	4.8E+01			---		VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1316-T01-E	1	1.03E+05			1.03E+05	7.0E+01	1.5E+01	4.8E+01			---		VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1316-T02-E	1	1.72E+05			1.72E+05	1.0E+00	1.5E+01	4.8E+01			---		VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1316-T03-E	1	4.15E+05			4.15E+05	2.9E-01	1.5E+01	4.8E+01			---		VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1316-T04-E	1	8.07E+05			8.07E+05	3.6E+00	1.5E+01	4.8E+01			---		VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1316-T01-F	1	1.08E+05			1.08E+05	7.7E-01	1.5E+01	4.8E+01			---		VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1316-T02-F	1	1.79E+05			1.79E+05	9.4E-01	1.5E+01	4.8E+01			---		VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1316-T03-F	1	2.94E+05			2.94E+05	6.8E+01	1.5E+01	4.8E+01			---		VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1316-T04-F	1	7.64E+05			7.64E+05	4.9E-01	1.5E+01	4.8E+01			---		VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
Se	SWA-LRef-1316-B01-D	1	7.50E+00	U1/2		7.50E+00	1.3E+02	1.5E+01	4.8E+01			---		VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	SWA-LRef-1316-T01-D	1	2.37E+04			2.37E+04	6.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1316-T02-D	1	3.00E+04			3.00E+04	3.1E-01	1.1E+00	3.5E+00	1000	100	3.09E+04	98%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1316-T03-D	1	4.05E+04			4.05E+04	1.4E+00	1.1E+00	3.5E+00				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1316-T04-D	1	5.94E+04			5.94E+04	1.9E+00	1.1E+00	3.5E+00				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1316-T01-E	1	2.31E+04			2.31E+04	6.5E+01	1.1E+00	3.5E+00				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1316-T02-E	1	2.74E+04			2.74E+04	6.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1316-T03-E	1	3.97E+04			3.97E+04	5.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1316-T04-E	1	5.83E+04			5.83E+04	3.9E+00	1.1E+00	3.5E+00				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1316-T01-F	1	2.47E+04			2.47E+04	1.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1316-T02-F	1	2.96E+04			2.96E+04	8.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1316-T03-F	1	3.92E+04			3.92E+04	6.3E+01	1.1E+00	3.5E+00				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1316-T04-F	1	5.75E+04			5.75E+04	4.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
Si	SWA-LRef-1316-B01-D	1	5.50E-01	U1/2		5.50E-01	2.6E+01	1.1E+00	3.5E+00				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	SWA-LRef-1316-T01-D	1	3.62E+05			3.62E+05	3.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1316-T02-D	1	4.39E+05			4.39E+05	7.7E-01	2.5E+00	8.0E+00	1000	100	4.40E+05	84%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1316-T03-D	1	5.36E+05			5.36E+05	2.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1316-T04-D	1	5.14E+05			5.14E+05	1.8E+00	2.5E+00	8.0E+00				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1316-T01-E	1	2.83E+05			2.83E+05	5.5E+01	2.5E+00	8.0E+00				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1316-T02-E	1	4.42E+05			4.42E+05	2.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1316-T03-E	1	5.28E+05			5.28E+05	9.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1316-T04-E	1	5.17E+05			5.17E+05	2.6E+00	2.5E+00	8.0E+00				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1316-T01-F	1	3.59E+05			3.59E+05	6.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1316-T02-F	1	4.45E+05			4.45E+05	7.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1316-T03-F	1	4.58E+05			4.58E+05	4.7E+01	2.5E+00	8.0E+00				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1316-T04-F	1	5.24E+05			5.24E+05	9.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
Na	SWA-LRef-1316-B01-D	1	3.95E+00	E		3.95E+00	6.2E+02	2.5E+00	8.0E+00				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	SWA-LRef-1316-T01-D	1	3.52E+02			3.52E+02	5.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1316-T02-D	1	3.86E+02			3.86E+02	7.5E-01	1.0E+00	3.2E+00	1000	100	1.51E+03	113%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1316-T03-D	1	4.26E+02			4.26E+02	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1316-T04-D	1	4.42E+02			4.42E+02	2.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1316-T01-E	1	3.45E+02			3.45E+02	6.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1316-T02-E	1	4.18E+02			4.18E+02	7.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1316-T03-E	1	4.47E+02			4.47E+02	4.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1316-T04-E	1	4.63E+02			4.63E+02	3.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1316-T01-F	1	3.84E+02			3.84E+02	8.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1316-T02-F	1	3.37E+02			3.37E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1316-T03-F	1	4.27E+02			4.27E+02	6.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1316-T04-F	1	4.94E+02			4.94E+02	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
Sr	SWA-LRef-1316-B01-D	1	5.00E-01	U1/2		5.00E-01	2.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	SWA-LRef-1316-T01-D	1	3.83E+05			3.83E+05	3.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1316-T02-D	1	6.37E+05			6.37E+05	8.1E-01	6.8E+00	2.2E+01	1000	100	6.38E+05	85%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1316-T03-D	1	1.38E+06			1.38E+06	2.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1316-T04-D	1	1.93E+06			1.93E+06	2.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1316-T01-E	1	3.29E+05			3.29E+05	6.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1316-T02-E	1	6.22E+05			6.22E+05	5.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1316-T03-E	1	1.47E+06			1.47E+06	1.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1316-T04-E	1	1.91E+06			1.91E+06	3.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1316-T01-F	1	3.97E+05			3.97E+05	7.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1316-T02-F	1	6.31E+05			6.31E+05	4.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1316-T03-F	1	1.32E+06			1.32E+06	6.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1316-T04-F	1	2.00E+06			2.00E+06	1.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
S	SWA-LRef-1316-B01-D	1	3.40E+00	U1/2		3.40E+00	2.5E+02	6.8E+00	2.2E+01				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	SWA-LRef-1316-T01-D	1	2.30E+00	U1/2		2.30E+00	8.5E+01	4.6E+00	1.5E+01				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1316-T02-D	1	2.30E+00	U1/2		2.30E+00	2.3E+01	4.6E+00	1.5E+01	10	100	1.01E+03	100%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1316-T03-D	1	2.30E+00	U1/2		2.30E+00	5.5E+01	4.6E+00	1.5E+01				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1316-T04-D	1	2.30E+00	U1/2		2.30E+00	9.4E+02	4.6E+00	1.5E+01				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1316-T01-E	1	2.30E+00	U1/2		2.30E+00	3.8E+01	4.6E+00	1.5E+01				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1316-T02-E	1	2.30E+00	U1/2		2.30E+00	8.1E+01	4.6E+00	1.5E+01				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1316-T03-E	1	2.30E+00	U1/2		2.30E+00	2.1E+01	4.6E+00	1.5E+01				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1316-T04-E	1	2.30E+00	U1/2		2.30E+00	2.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1316-T01-F	1	2.30E+00	U1/2		2.30E+00	3.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1316-T02-F	1	2.30E+00	U1/2		2.30E+00	5.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1316-T03-F	1	2.30E+00	U1/2		2.30E+00	5.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1316-T04-F	1	2.30E+00	U1/2		2.30E+00	2.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
Tl	SWA-LRef-1316-B01-D	1	2.30E+00	U1/2		2.30E+00	3.1E+01	4.6E+00	1.5E+01				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	SWA-LRef-1316-T01-D	1	1.00E+00	U1/2		1.00E+00	2.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1316-T02-D	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00	10	100	1.07E+03	107%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1316-T03-D	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1316-T04-D	1	3.55E+00	E		3.55E+00	1.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1316-T01-E	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1316-T02-E	1	1.00E+00	U1/2		1.00E+00	5.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1316-T03-E	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1316-T04-E	1	3.03E+00	E		3.03E+00	3.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1316-T01-F	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1316-T02-F	1	1.00E+00	U1/2		1.00E+00	1.8E+02	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1316-T03-F	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1316-T04-F	1	4.02E+00	E		4.02E+00	1.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
Ti	SWA-LRef-1316-B01-D	1	1.00E+00	U1/2		1.00E+00	8.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	SWA-LRef-1316-T01-D	1	3.62E+02			3.62E+02	1.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1316-T02-D	1	5.64E+02			5.64E+02	1.4E+00	1.5E+00	4.8E+00	10	100	1.67E+03	111%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1316-T03-D	1	1.17E+03			1.17E+03	7.0E-02	1.5E+00	4.8E+00				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1316-T04-D	1	2.10E+03			2.10E+03	1.9E+00	1.5E+00	4.8E+00				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1316-T01-E	1	3.16E+02			3.16E+02	6.8E+01	1.5E+00	4.8E+00				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1316-T02-E	1	4.91E+02			4.91E+02	1.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1316-T03-E	1	1.18E+03			1.18E+03	5.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1316-T04-E	1	1.90E+03			1.90E+03	4.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1316-T01-F	1	3.68E+02			3.68E+02	3.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1316-T02-F	1	5.47E+02			5.47E+02	1.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1316-T03-F	1	9.67E+02			9.67E+02	6.1E+01	1.5E+00	4.8E+00				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1316-T04-F	1	2.04E+03			2.04E+03	1.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
V	SWA-LRef-1316-B01-D	1	7.50E-01	U1/2		7.50E-01	1.3E+02	1.5E+00	4.8E+00				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	SWA-LRef-1316-T01-D	1	5.00E-01	U1/2		5.00E-01	4.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:50 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1316-T02-D	1	3.39E+00			3.39E+00	8.9E+00	1.0E+00	3.2E+00	10	100	1.08E+03	108%	VU ICP-OES	10/26/10 2:52 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1316-T03-D	1	4.41E+00			4.41E+00	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:54 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1316-T04-D	1	1.48E+01			1.48E+01	3.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:55 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1316-T01-E	1	5.00E-01	U1/2		5.00E-01	7.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:57 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1316-T02-E	1	4.73E+00			4.73E+00	6.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:59 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1316-T03-E	1	4.82E+00			4.82E+00	9.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:00 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1316-T04-E	1	1.86E+01			1.86E+01	7.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:02 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1316-T01-F	1	5.00E-01	U1/2		5.00E-01	2.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:04 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1316-T02-F	1	2.50E+00	E		2.50E+00	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:05 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1316-T03-F	1	3.96E+00			3.96E+00	2.6E+02	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:07 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1316-T04-F	1	1.13E+01			1.13E+01	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 3:09 PM	EPA Interlab LRef 1313-1316 SWA
Zn	SWA-LRef-1316-B01-D	1	5.00E-01	U1/2		5.00E-01	2.9E+02	1.0E+00	3.2E+00				---	VU ICP-OES	10/26/10 2:21 PM	EPA Interlab LRef 1313-1316 SWA

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	CFS-L01-1316-T01-A	1	4.94E+01			4.94E+01	6.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1316-T02-A	1	4.88E+01			4.88E+01	1.0E+01	1.0E+00	3.2E+00	1000	100	1.13E+03	108%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1316-T03-A	1	5.23E+01			5.23E+01	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1316-T04-A	1	5.48E+01			5.48E+01	1.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1316-T05-A	1	5.49E+01			5.49E+01	1.7E+01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1316-T01-B	1	4.13E+01			4.13E+01	7.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1316-T02-B	1	4.39E+01			4.39E+01	2.2E+01	1.0E+00	3.2E+00	1000	100	1.17E+03	112%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1316-T03-B	1	4.81E+01			4.81E+01	7.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1316-T04-B	1	4.66E+01			4.66E+01	1.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1316-T05-B	1	5.64E+01			5.64E+01	6.1E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1316-T01-C	1	4.23E+01			4.23E+01	1.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1316-T02-C	1	5.30E+01			5.30E+01	1.1E+01	1.0E+00	3.2E+00	1000	100	1.14E+03	109%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1316-T03-C	1	5.09E+01			5.09E+01	7.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1316-T04-C	1	4.90E+01			4.90E+01	1.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1316-T05-C	1	6.16E+01			6.16E+01	5.4E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
Al	CFS-L01-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	4.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	CFS-L01-1316-T01-A	1	3.83E+01			3.83E+01	1.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1316-T02-A	1	3.74E+01			3.74E+01	1.1E+01	7.5E+00	2.4E+01	10	100	1.06E+03	102%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1316-T03-A	1	3.71E+01			3.71E+01	3.5E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1316-T04-A	1	5.63E+01			5.63E+01	1.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1316-T05-A	1	5.88E+01			5.88E+01	1.3E+01	7.5E+00	2.4E+01					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1316-T01-B	1	3.00E+01			3.00E+01	2.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1316-T02-B	1	3.56E+01			3.56E+01	9.8E+00	7.5E+00	2.4E+01	10	100	1.04E+03	100%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1316-T03-B	1	3.81E+01			3.81E+01	1.9E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1316-T04-B	1	4.40E+01			4.40E+01	1.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1316-T05-B	1	6.73E+01			6.73E+01	4.2E+00	7.5E+00	2.4E+01					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1316-T01-C	1	3.16E+01			3.16E+01	3.5E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1316-T02-C	1	3.46E+01			3.46E+01	7.2E+00	7.5E+00	2.4E+01	10	100	1.06E+03	102%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1316-T03-C	1	4.03E+01			4.03E+01	2.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1316-T04-C	1	5.21E+01			5.21E+01	1.4E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1316-T05-C	1	6.96E+01			6.96E+01	7.2E+00	7.5E+00	2.4E+01					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
Sb	CFS-L01-1316-B01-A	1	3.75E+00	U1/2		3.75E+00	3.9E+01	7.5E+00	2.4E+01				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	CFS-L01-1316-T01-A	1	2.57E+01	E		2.57E+01	2.2E+01	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1316-T02-A	1	2.46E+01	E		2.46E+01	2.4E+01	1.1E+01	3.5E+01	10	100	1.05E+03	102%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1316-T03-A	1	3.49E+01	E		3.49E+01	1.9E+01	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1316-T04-A	1	4.02E+01			4.02E+01	3.8E+01	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1316-T05-A	1	5.63E+01			5.63E+01	1.5E+01	1.1E+01	3.5E+01					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1316-T01-B	1	2.31E+01	E		2.31E+01	6.0E+01	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1316-T02-B	1	2.76E+01	E		2.76E+01	3.2E+01	1.1E+01	3.5E+01	10	100	1.09E+03	106%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1316-T03-B	1	3.63E+01			3.63E+01	1.8E+01	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1316-T04-B	1	4.68E+01			4.68E+01	2.6E+01	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1316-T05-B	1	5.23E+01			5.23E+01	3.3E+01	1.1E+01	3.5E+01					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1316-T01-C	1	1.98E+01	E		1.98E+01	4.5E+01	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1316-T02-C	1	2.55E+01	E		2.55E+01	3.7E+01	1.1E+01	3.5E+01	10	100	1.07E+03	105%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1316-T03-C	1	3.87E+01			3.87E+01	4.2E+00	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1316-T04-C	1	3.20E+01	E		3.20E+01	5.1E+00	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1316-T05-C	1	4.44E+01			4.44E+01	5.4E+00	1.1E+01	3.5E+01					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
As	CFS-L01-1316-B01-A	1	5.50E+00	U1/2		5.50E+00	5.9E+01	1.1E+01	3.5E+01				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	CFS-L01-1316-T01-A	1	1.51E+02			1.51E+02	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1316-T02-A	1	2.91E+02			2.91E+02	8.9E-01	1.0E+00	3.2E+00	1000	100	1.24E+03	95%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1316-T03-A	1	6.29E+02			6.29E+02	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1316-T04-A	1	9.56E+02			9.56E+02	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1316-T05-A	1	1.50E+03			1.50E+03	6.2E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1316-T01-B	1	1.59E+02			1.59E+02	6.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1316-T02-B	1	2.96E+02			2.96E+02	1.8E+00	1.0E+00	3.2E+00	1000	100	1.24E+03	95%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1316-T03-B	1	6.36E+02			6.36E+02	6.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1316-T04-B	1	9.76E+02			9.76E+02	2.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1316-T05-B	1	1.46E+03			1.46E+03	2.9E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1316-T01-C	1	1.60E+02			1.60E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1316-T02-C	1	2.83E+02			2.83E+02	4.6E-02	1.0E+00	3.2E+00	1000	100	1.25E+03	97%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1316-T03-C	1	6.01E+02			6.01E+02	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1316-T04-C	1	9.72E+02			9.72E+02	1.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1316-T05-C	1	1.41E+03			1.41E+03	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
B	CFS-L01-1316-B01-A	1	4.51E+00			4.51E+00	2.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	CFS-L01-1316-T01-A	1	8.84E+01			8.84E+01	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1316-T02-A	1	8.72E+01			8.72E+01	5.1E-02	1.0E+00	3.2E+00	10	100	1.04E+03	95%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1316-T03-A	1	7.71E+01			7.71E+01	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1316-T04-A	1	6.53E+01			6.53E+01	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1316-T05-A	1	5.32E+01			5.32E+01	3.9E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1316-T01-B	1	9.26E+01			9.26E+01	1.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1316-T02-B	1	9.16E+01			9.16E+01	3.0E-01	1.0E+00	3.2E+00	10	100	1.02E+03	92%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1316-T03-B	1	7.80E+01			7.80E+01	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1316-T04-B	1	6.74E+01			6.74E+01	3.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1316-T05-B	1	5.38E+01			5.38E+01	1.9E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1316-T01-C	1	9.12E+01			9.12E+01	4.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1316-T02-C	1	8.78E+01			8.78E+01	2.1E-01	1.0E+00	3.2E+00	10	100	1.05E+03	96%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1316-T03-C	1	7.46E+01			7.46E+01	5.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1316-T04-C	1	6.28E+01			6.28E+01	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1316-T05-C	1	5.17E+01			5.17E+01	8.7E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
Ba	CFS-L01-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	4.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	CFS-L01-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	1.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	4.4E+02	1.9E+00	6.0E+00	10	100	1.02E+03	102%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	8.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	7.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1316-T05-A	1	9.50E-01	U1/2		9.50E-01	7.5E+01	1.9E+00	6.0E+00					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	2.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	2.1E+02	1.9E+00	6.0E+00	10	100	1.09E+03	109%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	1.9E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	6.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1316-T05-B	1	9.50E-01	U1/2		9.50E-01	6.0E+01	1.9E+00	6.0E+00					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	2.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	9.8E+00	1.9E+00	6.0E+00	10	100	1.04E+03	104%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	1.3E+03	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	4.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1316-T05-C	1	9.50E-01	U1/2		9.50E-01	3.1E+01	1.9E+00	6.0E+00					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
Be	CFS-L01-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	4.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	CFS-L01-1316-T01-A	1	4.75E+03			4.75E+03	6.2E-01	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1316-T02-A	1	6.69E+03			6.69E+03	3.9E-01	2.2E+00	7.0E+00	10	100	7.63E+03	95%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1316-T03-A	1	1.06E+04			1.06E+04	8.4E-01	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1316-T04-A	1	1.22E+04			1.22E+04	6.1E-01	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1316-T05-A	1	1.57E+04			1.57E+04	5.3E-01	2.2E+00	7.0E+00					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1316-T01-B	1	4.95E+03			4.95E+03	8.6E-01	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1316-T02-B	1	7.23E+03			7.23E+03	1.1E+00	2.2E+00	7.0E+00	10	100	8.33E+03	110%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1316-T03-B	1	1.04E+04			1.04E+04	5.8E-01	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1316-T04-B	1	1.18E+04			1.18E+04	2.2E-01	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1316-T05-B	1	1.51E+04			1.51E+04	6.2E-01	2.2E+00	7.0E+00					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1316-T01-C	1	5.03E+03			5.03E+03	4.8E-01	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1316-T02-C	1	7.00E+03			7.00E+03	2.6E-01	2.2E+00	7.0E+00	10	100	7.98E+03	98%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1316-T03-C	1	1.03E+04			1.03E+04	2.7E-01	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1316-T04-C	1	1.22E+04			1.22E+04	4.1E-01	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1316-T05-C	1	1.59E+04			1.59E+04	2.0E+00	2.2E+00	7.0E+00					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
Cd	CFS-L01-1316-B01-A	1	1.10E+00	U1/2		1.10E+00	3.7E+03	2.2E+00	7.0E+00				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	CFS-L01-1316-T01-A	1	6.71E+05			6.71E+05	4.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1316-T02-A	1	6.38E+05			6.38E+05	7.7E-01	2.6E+00	8.3E+00	1000	100	6.39E+05	86%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1316-T03-A	1	6.33E+05			6.33E+05	4.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1316-T04-A	1	5.95E+05			5.95E+05	5.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1316-T05-A	1	5.64E+05			5.64E+05	9.1E-01	2.6E+00	8.3E+00					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1316-T01-B	1	6.93E+05			6.93E+05	7.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1316-T02-B	1	6.88E+05			6.88E+05	1.1E+00	2.6E+00	8.3E+00	1000	100	6.89E+05	83%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1316-T03-B	1	6.34E+05			6.34E+05	5.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1316-T04-B	1	5.95E+05			5.95E+05	3.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1316-T05-B	1	5.67E+05			5.67E+05	7.8E-01	2.6E+00	8.3E+00					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1316-T01-C	1	6.88E+05			6.88E+05	5.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1316-T02-C	1	6.72E+05			6.72E+05	5.5E-01	2.6E+00	8.3E+00	1000	100	6.73E+05	88%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1316-T03-C	1	6.28E+05			6.28E+05	6.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1316-T04-C	1	5.90E+05			5.90E+05	2.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1316-T05-C	1	5.63E+05			5.63E+05	1.3E+00	2.6E+00	8.3E+00					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
Ca	CFS-L01-1316-B01-A	1	7.32E+01			7.32E+01	3.5E+00	2.6E+00	8.3E+00				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	CFS-L01-1316-T01-A	1	6.00E-01	U1/2		6.00E-01	3.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1316-T02-A	1	6.00E-01	U1/2		6.00E-01	4.4E+02	1.2E+00	3.8E+00	10	100	9.76E+02	98%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1316-T03-A	1	6.00E-01	U1/2		6.00E-01	5.4E+02	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1316-T04-A	1	6.00E-01	U1/2		6.00E-01	1.1E+02	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1316-T05-A	1	6.00E-01	U1/2		6.00E-01	1.8E+01	1.2E+00	3.8E+00					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1316-T01-B	1	6.00E-01	U1/2		6.00E-01	1.2E+03	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1316-T02-B	1	6.00E-01	U1/2		6.00E-01	5.4E+02	1.2E+00	3.8E+00	10	100	9.44E+02	94%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1316-T03-B	1	6.00E-01	U1/2		6.00E-01	1.2E+02	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1316-T04-B	1	6.00E-01	U1/2		6.00E-01	2.0E+03	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1316-T05-B	1	6.00E-01	U1/2		6.00E-01	1.1E+02	1.2E+00	3.8E+00					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1316-T01-C	1	6.00E-01	U1/2		6.00E-01	2.6E+02	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1316-T02-C	1	6.00E-01	U1/2		6.00E-01	8.6E+01	1.2E+00	3.8E+00	10	100	9.77E+02	98%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1316-T03-C	1	6.00E-01	U1/2		6.00E-01	3.6E+02	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1316-T04-C	1	6.00E-01	U1/2		6.00E-01	2.3E+02	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1316-T05-C	1	6.00E-01	U1/2		6.00E-01	2.0E+02	1.2E+00	3.8E+00					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
Cr	CFS-L01-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	3.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	CFS-L01-1316-T01-A	1	9.90E+01			9.90E+01	1.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1316-T02-A	1	1.73E+02			1.73E+02	9.1E-01	1.8E+00	5.7E+00	10	100	1.10E+03	93%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1316-T03-A	1	3.40E+02			3.40E+02	9.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1316-T04-A	1	4.64E+02			4.64E+02	6.4E-01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1316-T05-A	1	7.04E+02			7.04E+02	9.3E-01	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1316-T01-B	1	1.03E+02			1.03E+02	7.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1316-T02-B	1	1.86E+02			1.86E+02	1.0E+00	2.0E+00	6.4E+00	10	100	1.10E+03	92%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1316-T03-B	1	3.40E+02			3.40E+02	2.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1316-T04-B	1	4.45E+02			4.45E+02	1.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1316-T05-B	1	6.82E+02			6.82E+02	1.5E+00	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1316-T01-C	1	1.07E+02			1.07E+02	2.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1316-T02-C	1	1.78E+02			1.78E+02	2.9E-01	2.0E+00	6.4E+00	10	100	1.12E+03	94%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1316-T03-C	1	3.40E+02			3.40E+02	8.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1316-T04-C	1	4.67E+02			4.67E+02	3.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1316-T05-C	1	7.21E+02			7.21E+02	8.5E-01	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
Co	CFS-L01-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	3.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	CFS-L01-1316-T01-A	1	8.89E+02			8.89E+02	1.5E-01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1316-T02-A	1	1.09E+03			1.09E+03	2.7E-01	3.7E+00	1.2E+01	10	100	2.01E+03	93%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1316-T03-A	1	1.73E+03			1.73E+03	1.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1316-T04-A	1	2.19E+03			2.19E+03	6.0E-01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1316-T05-A	1	3.01E+03			3.01E+03	7.1E-01	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1316-T01-B	1	9.39E+02			9.39E+02	9.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1316-T02-B	1	8.85E+02			8.85E+02	1.8E+00	2.0E+00	6.4E+00	10	100	1.84E+03	95%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1316-T03-B	1	1.31E+03			1.31E+03	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1316-T04-B	1	2.04E+03			2.04E+03	3.7E-02	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1316-T05-B	1	3.09E+03			3.09E+03	5.3E-01	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1316-T01-C	1	9.65E+02			9.65E+02	4.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1316-T02-C	1	8.92E+02			8.92E+02	6.5E-01	2.0E+00	6.4E+00	10	100	1.79E+03	90%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1316-T03-C	1	1.61E+03			1.61E+03	4.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1316-T04-C	1	1.94E+03			1.94E+03	2.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1316-T05-C	1	3.13E+03			3.13E+03	1.6E+00	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
Cu	CFS-L01-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	9.7E+02	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	CFS-L01-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	1.9E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	9.3E+01	2.0E+00	6.4E+00	1000	100	1.01E+03	101%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	3.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1316-T05-A	1	1.00E+00	U1/2		1.00E+00	3.9E+00	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00	1000	100	1.07E+03	107%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1316-T05-B	1	1.00E+00	U1/2		1.00E+00	2.6E+01	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	5.5E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00	1000	100	1.01E+03	101%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	7.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1316-T05-C	1	1.00E+00	U1/2		1.00E+00	3.9E+01	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
Fe	CFS-L01-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	2.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	CFS-L01-1316-T01-A	1	1.18E+03			1.18E+03	6.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1316-T02-A	1	1.27E+03			1.27E+03	5.3E-01	6.8E+00	2.2E+01	10	100	2.14E+03	87%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1316-T03-A	1	1.49E+03			1.49E+03	1.3E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1316-T04-A	1	1.44E+03			1.44E+03	4.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1316-T05-A	1	1.35E+03			1.35E+03	3.4E-01	6.8E+00	2.2E+01					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1316-T01-B	1	1.24E+03			1.24E+03	8.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1316-T02-B	1	1.29E+03			1.29E+03	5.1E-01	6.8E+00	2.2E+01	10	100	2.13E+03	83%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1316-T03-B	1	1.32E+03			1.32E+03	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1316-T04-B	1	1.48E+03			1.48E+03	5.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1316-T05-B	1	1.40E+03			1.40E+03	1.6E+00	6.8E+00	2.2E+01					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1316-T01-C	1	1.21E+03			1.21E+03	9.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1316-T02-C	1	1.09E+03			1.09E+03	6.9E-01	6.8E+00	2.2E+01	10	100	1.95E+03	85%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1316-T03-C	1	1.38E+03			1.38E+03	4.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1316-T04-C	1	1.40E+03			1.40E+03	8.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1316-T05-C	1	1.32E+03			1.32E+03	1.4E+00	6.8E+00	2.2E+01					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
Pb	CFS-L01-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	1.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	CFS-L01-1316-T01-A	1	9.77E+00			9.77E+00	2.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1316-T02-A	1	1.09E+01			1.09E+01	1.2E+01	1.9E+00	6.0E+00	10	100	8.34E+02	82%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1316-T03-A	1	4.49E+00	E		4.49E+00	1.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1316-T04-A	1	8.54E+00			8.54E+00	1.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1316-T05-A	1	2.12E+01			2.12E+01	7.7E+00	1.9E+00	6.0E+00					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1316-T01-B	1	8.88E+00			8.88E+00	1.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1316-T02-B	1	7.59E+00			7.59E+00	1.5E+01	1.9E+00	6.0E+00	10	100	8.59E+02	85%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1316-T03-B	1	4.91E+00	E		4.91E+00	1.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1316-T04-B	1	8.23E+00			8.23E+00	1.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1316-T05-B	1	2.04E+01			2.04E+01	6.2E+00	1.9E+00	6.0E+00					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1316-T01-C	1	9.03E+00			9.03E+00	2.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1316-T02-C	1	1.07E+01			1.07E+01	1.4E+01	1.9E+00	6.0E+00	10	100	8.47E+02	84%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1316-T03-C	1	4.38E+00	E		4.38E+00	1.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1316-T04-C	1	9.96E+00			9.96E+00	7.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1316-T05-C	1	2.16E+01			2.16E+01	1.5E+01	1.9E+00	6.0E+00					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
Li	CFS-L01-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	1.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	CFS-L01-1316-T01-A	1	1.58E+03			1.58E+03	1.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1316-T02-A	1	3.05E+03			3.05E+03	3.8E-01	2.0E+00	6.4E+00	10	100	4.04E+03	99%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1316-T03-A	1	6.82E+03			6.82E+03	8.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1316-T04-A	1	1.03E+04			1.03E+04	7.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1316-T05-A	1	1.79E+04			1.79E+04	5.6E-01	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1316-T01-B	1	1.64E+03			1.64E+03	4.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1316-T02-B	1	3.30E+03			3.30E+03	9.4E-01	2.0E+00	6.4E+00	10	100	4.25E+03	95%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1316-T03-B	1	6.96E+03			6.96E+03	7.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1316-T04-B	1	9.98E+03			9.98E+03	2.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1316-T05-B	1	1.73E+04			1.73E+04	1.2E+00	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1316-T01-C	1	1.71E+03			1.71E+03	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1316-T02-C	1	3.13E+03			3.13E+03	3.0E-01	2.0E+00	6.4E+00	10	100	4.18E+03	105%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1316-T03-C	1	6.85E+03			6.85E+03	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1316-T04-C	1	1.04E+04			1.04E+04	4.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1316-T05-C	1	1.79E+04			1.79E+04	1.2E+00	2.0E+00	6.4E+00					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
Mn	CFS-L01-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	7.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	CFS-L01-1316-T01-A	1	6.18E+04			6.18E+04	5.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1316-T02-A	1	1.23E+05			1.23E+05	6.3E-01	1.0E+00	3.2E+00	1000	100	1.24E+05	92%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1316-T03-A	1	2.76E+05			2.76E+05	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1316-T04-A	1	4.81E+05			4.81E+05	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1316-T05-A	1	8.35E+05			8.35E+05	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1316-T01-B	1	6.38E+04			6.38E+04	1.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1316-T02-B	1	1.30E+05			1.30E+05	9.1E-01	1.0E+00	3.2E+00	1000	100	1.31E+05	88%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1316-T03-B	1	2.85E+05			2.85E+05	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1316-T04-B	1	4.90E+05			4.90E+05	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1316-T05-B	1	8.39E+05			8.39E+05	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1316-T01-C	1	6.32E+04			6.32E+04	9.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1316-T02-C	1	1.22E+05			1.22E+05	1.2E+00	1.0E+00	3.2E+00	1000	100	1.23E+05	96%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1316-T03-C	1	2.85E+05			2.85E+05	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1316-T04-C	1	4.88E+05			4.88E+05	1.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1316-T05-C	1	8.49E+05			8.49E+05	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
Mg	CFS-L01-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	3.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	CFS-L01-1316-T01-A	1	6.97E+00			6.97E+00	1.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1316-T02-A	1	1.21E+01			1.21E+01	7.4E+00	1.2E+00	3.8E+00	10	100	9.69E+02	96%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1316-T03-A	1	1.34E+01			1.34E+01	6.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1316-T04-A	1	1.70E+01			1.70E+01	1.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1316-T05-A	1	2.49E+01			2.49E+01	3.3E+00	1.2E+00	3.8E+00					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1316-T01-B	1	7.95E+00			7.95E+00	2.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1316-T02-B	1	1.06E+01			1.06E+01	1.1E+01	1.2E+00	3.8E+00	10	100	9.54E+02	94%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1316-T03-B	1	1.49E+01			1.49E+01	8.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1316-T04-B	1	1.51E+01			1.51E+01	5.6E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1316-T05-B	1	2.05E+01			2.05E+01	8.8E+00	1.2E+00	3.8E+00					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1316-T01-C	1	7.90E+00			7.90E+00	1.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1316-T02-C	1	1.01E+01			1.01E+01	2.9E+00	1.2E+00	3.8E+00	10	100	9.88E+02	98%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1316-T03-C	1	1.30E+01			1.30E+01	9.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1316-T04-C	1	1.56E+01			1.56E+01	1.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1316-T05-C	1	1.94E+01			1.94E+01	6.5E+00	1.2E+00	3.8E+00					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
Mo	CFS-L01-1316-B01-A	1	1.74E+00	E		1.74E+00	5.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	CFS-L01-1316-T01-A	1	2.24E+02			2.24E+02	7.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1316-T02-A	1	3.71E+02			3.71E+02	6.2E-01	1.8E+00	5.7E+00	10	100	1.32E+03	94%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1316-T03-A	1	6.56E+02			6.56E+02	6.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1316-T04-A	1	8.47E+02			8.47E+02	6.4E-01	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1316-T05-A	1	1.17E+03			1.17E+03	6.9E-01	3.7E+00	1.2E+01					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1316-T01-B	1	2.40E+02			2.40E+02	6.7E-01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1316-T02-B	1	3.98E+02			3.98E+02	1.3E+00	3.7E+00	1.2E+01	10	100	1.31E+03	91%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1316-T03-B	1	6.43E+02			6.43E+02	9.4E-02	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1316-T04-B	1	8.12E+02			8.12E+02	3.8E-01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1316-T05-B	1	1.15E+03			1.15E+03	6.2E-01	3.7E+00	1.2E+01					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1316-T01-C	1	2.40E+02			2.40E+02	1.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1316-T02-C	1	3.81E+02			3.81E+02	9.6E-01	3.7E+00	1.2E+01	10	100	1.33E+03	95%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1316-T03-C	1	6.60E+02			6.60E+02	3.9E-01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1316-T04-C	1	8.39E+02			8.39E+02	2.1E-01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1316-T05-C	1	1.22E+03			1.22E+03	1.2E+00	3.7E+00	1.2E+01					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
Ni	CFS-L01-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	6.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	CFS-L01-1316-T01-A	1	1.83E+01			1.83E+01	5.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1316-T02-A	1	1.44E+01			1.44E+01	4.8E+01	3.7E+00	1.2E+01	1000	100	1.11E+03	109%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1316-T03-A	1	2.84E+01			2.84E+01	2.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1316-T04-A	1	2.71E+01			2.71E+01	5.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1316-T05-A	1	3.83E+01			3.83E+01	3.9E+01	3.7E+00	1.2E+01					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1316-T01-B	1	1.01E+01	E		1.01E+01	1.3E+02	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1316-T02-B	1	3.31E+01			3.31E+01	1.3E+02	3.7E+00	1.2E+01	1000	100	1.13E+03	110%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1316-T03-B	1	2.52E+01			2.52E+01	8.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1316-T04-B	1	1.78E+01			1.78E+01	6.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1316-T05-B	1	1.82E+01			1.82E+01	5.7E+01	3.7E+00	1.2E+01					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1316-T01-C	1	1.00E+01	E		1.00E+01	8.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1316-T02-C	1	1.44E+01			1.44E+01	1.8E+01	3.7E+00	1.2E+01	1000	100	1.11E+03	110%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1316-T03-C	1	1.73E+01			1.73E+01	6.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1316-T04-C	1	3.08E+01			3.08E+01	5.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1316-T05-C	1	3.80E+01			3.80E+01	4.6E+01	3.7E+00	1.2E+01					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
P	CFS-L01-1316-B01-A	1	4.13E+00	E		4.13E+00	1.3E+02	3.7E+00	1.2E+01				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	CFS-L01-1316-T01-A	1	9.04E+03			9.04E+03	7.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1316-T02-A	1	1.64E+04			1.64E+04	3.5E-01	1.6E+00	5.1E+00	1000	100	1.73E+04	84%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1316-T03-A	1	3.35E+04			3.35E+04	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1316-T04-A	1	5.03E+04			5.03E+04	7.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1316-T05-A	1	8.00E+04			8.00E+04	6.6E-01	1.6E+00	5.1E+00					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1316-T01-B	1	9.35E+03			9.35E+03	8.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1316-T02-B	1	1.74E+04			1.74E+04	1.3E+00	1.6E+00	5.1E+00	1000	100	1.83E+04	91%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1316-T03-B	1	3.37E+04			3.37E+04	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1316-T04-B	1	5.06E+04			5.06E+04	1.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1316-T05-B	1	7.85E+04			7.85E+04	7.8E-01	1.6E+00	5.1E+00					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1316-T01-C	1	9.24E+03			9.24E+03	4.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1316-T02-C	1	1.67E+04			1.67E+04	5.2E-01	1.6E+00	5.1E+00	1000	100	1.76E+04	90%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1316-T03-C	1	3.30E+04			3.30E+04	5.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1316-T04-C	1	5.07E+04			5.07E+04	3.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1316-T05-C	1	7.89E+04			7.89E+04	1.5E+00	1.6E+00	5.1E+00					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
K	CFS-L01-1316-B01-A	1	1.81E+01			1.81E+01	1.9E+01	1.6E+00	5.1E+00				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	CFS-L01-1316-T01-A	1	7.19E+01			7.19E+01	2.2E+01	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1316-T02-A	1	1.34E+02			1.34E+02	1.3E+01	1.5E+01	4.8E+01	10	100	1.09E+03	96%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1316-T03-A	1	2.50E+02			2.50E+02	6.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1316-T04-A	1	4.51E+02			4.51E+02	1.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1316-T05-A	1	7.73E+02			7.73E+02	1.8E+00	1.5E+01	4.8E+01					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1316-T01-B	1	6.49E+01			6.49E+01	2.7E+01	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1316-T02-B	1	1.41E+02			1.41E+02	1.5E+01	1.5E+01	4.8E+01	10	100	1.10E+03	96%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1316-T03-B	1	2.73E+02			2.73E+02	3.2E+00	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1316-T04-B	1	4.54E+02			4.54E+02	5.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1316-T05-B	1	7.77E+02			7.77E+02	2.7E+00	1.5E+01	4.8E+01					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1316-T01-C	1	8.07E+01			8.07E+01	2.4E+01	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1316-T02-C	1	1.28E+02			1.28E+02	4.6E+00	1.5E+01	4.8E+01	10	100	1.13E+03	101%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1316-T03-C	1	2.78E+02			2.78E+02	4.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1316-T04-C	1	4.49E+02			4.49E+02	1.6E+00	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1316-T05-C	1	8.13E+02			8.13E+02	1.2E+00	1.5E+01	4.8E+01					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
Se	CFS-L01-1316-B01-A	1	7.50E+00	U1/2		7.50E+00	8.7E+01	1.5E+01	4.8E+01				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	CFS-L01-1316-T01-A	1	3.98E+03			3.98E+03	5.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1316-T02-A	1	5.40E+03			5.40E+03	3.1E-02	1.1E+00	3.5E+00	1000	100	6.38E+03	98%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1316-T03-A	1	7.14E+03			7.14E+03	7.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1316-T04-A	1	7.25E+03			7.25E+03	4.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1316-T05-A	1	8.02E+03			8.02E+03	6.4E-01	1.1E+00	3.5E+00					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1316-T01-B	1	4.13E+03			4.13E+03	8.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1316-T02-B	1	5.68E+03			5.68E+03	9.6E-01	1.1E+00	3.5E+00	1000	100	6.63E+03	95%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1316-T03-B	1	6.86E+03			6.86E+03	7.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1316-T04-B	1	7.31E+03			7.31E+03	1.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1316-T05-B	1	7.71E+03			7.71E+03	9.8E-01	1.1E+00	3.5E+00					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1316-T01-C	1	3.99E+03			3.99E+03	9.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1316-T02-C	1	5.27E+03			5.27E+03	5.4E-01	1.1E+00	3.5E+00	1000	100	6.24E+03	96%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1316-T03-C	1	6.73E+03			6.73E+03	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1316-T04-C	1	7.09E+03			7.09E+03	2.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1316-T05-C	1	7.70E+03			7.70E+03	1.0E+00	1.1E+00	3.5E+00					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
Si	CFS-L01-1316-B01-A	1	2.27E+00	E		2.27E+00	4.1E+01	1.1E+00	3.5E+00				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	CFS-L01-1316-T01-A	1	1.71E+04			1.71E+04	9.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1316-T02-A	1	3.34E+04			3.34E+04	4.7E-01	2.5E+00	8.0E+00	1000	100	3.43E+04	90%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1316-T03-A	1	6.88E+04			6.88E+04	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1316-T04-A	1	1.03E+05			1.03E+05	9.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1316-T05-A	1	1.53E+05			1.53E+05	1.2E+00	2.5E+00	8.0E+00					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1316-T01-B	1	1.78E+04			1.78E+04	5.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1316-T02-B	1	3.34E+04			3.34E+04	1.4E+00	2.5E+00	8.0E+00	1000	100	3.43E+04	88%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1316-T03-B	1	6.96E+04			6.96E+04	3.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1316-T04-B	1	1.02E+05			1.02E+05	3.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1316-T05-B	1	1.52E+05			1.52E+05	1.3E+00	2.5E+00	8.0E+00					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1316-T01-C	1	1.79E+04			1.79E+04	1.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1316-T02-C	1	3.25E+04			3.25E+04	4.6E-01	2.5E+00	8.0E+00	1000	100	3.34E+04	91%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1316-T03-C	1	7.02E+04			7.02E+04	3.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1316-T04-C	1	1.03E+05			1.03E+05	1.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1316-T05-C	1	1.55E+05			1.55E+05	1.6E+00	2.5E+00	8.0E+00					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
Na	CFS-L01-1316-B01-A	1	1.25E+00	U1/2		1.25E+00	6.0E+01	2.5E+00	8.0E+00				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	CFS-L01-1316-T01-A	1	1.41E+03			1.41E+03	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1316-T02-A	1	2.07E+03			2.07E+03	1.9E-01	1.0E+00	3.2E+00	1000	100	2.92E+03	86%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1316-T03-A	1	3.25E+03			3.25E+03	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1316-T04-A	1	3.93E+03			3.93E+03	8.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1316-T05-A	1	5.00E+03			5.00E+03	7.7E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1316-T01-B	1	1.45E+03			1.45E+03	9.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1316-T02-B	1	2.29E+03			2.29E+03	7.1E-01	1.0E+00	3.2E+00	1000	100	3.13E+03	84%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1316-T03-B	1	3.31E+03			3.31E+03	7.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1316-T04-B	1	4.13E+03			4.13E+03	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1316-T05-B	1	5.04E+03			5.04E+03	1.7E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1316-T01-C	1	1.43E+03			1.43E+03	7.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1316-T02-C	1	2.12E+03			2.12E+03	7.8E-01	1.0E+00	3.2E+00	1000	100	3.05E+03	92%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1316-T03-C	1	3.17E+03			3.17E+03	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1316-T04-C	1	4.07E+03			4.07E+03	8.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1316-T05-C	1	4.80E+03			4.80E+03	7.1E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
Sr	CFS-L01-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	2.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	CFS-L01-1316-T01-A	1	6.22E+05			6.22E+05	7.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1316-T02-A	1	7.06E+05			7.06E+05	7.7E-01	6.8E+00	2.2E+01	1000	100	7.07E+05	86%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1316-T03-A	1	8.63E+05			8.63E+05	1.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1316-T04-A	1	1.09E+06			1.09E+06	6.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1316-T05-A	1	1.47E+06			1.47E+06	4.0E-01	6.8E+00	2.2E+01					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1316-T01-B	1	6.17E+05			6.17E+05	7.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1316-T02-B	1	7.02E+05			7.02E+05	1.1E+00	6.8E+00	2.2E+01	1000	100	7.02E+05	83%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1316-T03-B	1	8.75E+05			8.75E+05	4.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1316-T04-B	1	1.09E+06			1.09E+06	8.6E-02	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1316-T05-B	1	1.47E+06			1.47E+06	7.4E-01	6.8E+00	2.2E+01					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1316-T01-C	1	6.12E+05			6.12E+05	5.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1316-T02-C	1	6.84E+05			6.84E+05	4.2E-01	6.8E+00	2.2E+01	1000	100	6.85E+05	89%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1316-T03-C	1	8.77E+05			8.77E+05	8.9E-02	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1316-T04-C	1	1.09E+06			1.09E+06	1.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1316-T05-C	1	1.48E+06			1.48E+06	1.2E+00	6.8E+00	2.2E+01					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
S	CFS-L01-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	3.6E+02	6.8E+00	2.2E+01				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	CFS-L01-1316-T01-A	1	3.32E+02			3.32E+02	2.3E+00	4.6E+00	1.5E+01				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
Tl	CFS-L01-1316-T02-A	1	5.25E+02			5.25E+02	7.3E-01	4.6E+00	1.5E+01	10	100	1.39E+03	87%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
Tl	CFS-L01-1316-T03-A	1	8.91E+02			8.91E+02	7.3E-01	4.6E+00	1.5E+01				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
Tl	CFS-L01-1316-T04-A	1	1.13E+03			1.13E+03	8.5E-01	4.6E+00	1.5E+01				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
Tl	CFS-L01-1316-T05-A	1	1.55E+03			1.55E+03	1.6E-01	1.5E+00	4.8E+00					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
Tl	CFS-L01-1316-T01-B	1	3.54E+02			3.54E+02	5.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
Tl	CFS-L01-1316-T02-B	1	5.47E+02			5.47E+02	2.0E+00	1.5E+00	4.8E+00	10	100	1.43E+03	88%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
Tl	CFS-L01-1316-T03-B	1	8.86E+02			8.86E+02	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
Tl	CFS-L01-1316-T04-B	1	1.15E+03			1.15E+03	4.3E-01	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
Tl	CFS-L01-1316-T05-B	1	1.51E+03			1.51E+03	7.1E-01	1.5E+00	4.8E+00					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
Tl	CFS-L01-1316-T01-C	1	3.50E+02			3.50E+02	3.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
Tl	CFS-L01-1316-T02-C	1	5.00E+02			5.00E+02	7.2E-01	1.5E+00	4.8E+00	10	100	1.41E+03	91%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
Tl	CFS-L01-1316-T03-C	1	8.53E+02			8.53E+02	5.3E-02	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
Tl	CFS-L01-1316-T04-C	1	1.12E+03			1.12E+03	5.4E-01	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
Tl	CFS-L01-1316-T05-C	1	1.48E+03			1.48E+03	4.7E-01	1.5E+00	4.8E+00					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
Tl	CFS-L01-1316-B01-A	1	2.30E+00	U1/2		2.30E+00	2.7E+02	4.6E+00	1.5E+01				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	CFS-L01-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	3.8E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	8.8E+01	2.0E+00	6.4E+00	10	100	9.54E+02	95%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	2.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	1.7E+02	2.0E+00	6.4E+00				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1316-T05-A	1	1.00E+00	U1/2		1.00E+00	3.5E+01	1.5E+00	4.8E+00					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	1.7E+02	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	7.4E+01	1.5E+00	4.8E+00	10	100	9.09E+02	91%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	2.3E+01	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	1.1E+02	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1316-T05-B	1	1.00E+00	U1/2		1.00E+00	4.2E+01	1.5E+00	4.8E+00					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	5.4E+01	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	5.8E+01	1.5E+00	4.8E+00	10	100	9.59E+02	96%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	1.1E+02	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	1.0E+01	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1316-T05-C	1	1.00E+00	U1/2		1.00E+00	1.2E+02	1.5E+00	4.8E+00					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
Ti	CFS-L01-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	4.7E+01	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	CFS-L01-1316-T01-A	1	2.97E+01			2.97E+01	5.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1316-T02-A	1	2.98E+01			2.98E+01	5.1E+00	1.5E+00	4.8E+00	10	100	9.93E+02	96%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1316-T03-A	1	2.92E+01			2.92E+01	5.5E-01	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1316-T04-A	1	2.65E+01			2.65E+01	2.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1316-T05-A	1	2.58E+01			2.58E+01	9.8E+00	1.5E+00	4.8E+00					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1316-T01-B	1	3.09E+01			3.09E+01	5.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1316-T02-B	1	3.18E+01			3.18E+01	3.1E+00	1.5E+00	4.8E+00	10	100	9.61E+02	93%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1316-T03-B	1	3.42E+01			3.42E+01	2.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1316-T04-B	1	2.71E+01			2.71E+01	2.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1316-T05-B	1	2.57E+01			2.57E+01	6.2E+00	1.5E+00	4.8E+00					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1316-T01-C	1	3.01E+01			3.01E+01	5.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1316-T02-C	1	2.94E+01			2.94E+01	3.9E+00	1.5E+00	4.8E+00	10	100	1.00E+03	97%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1316-T03-C	1	2.82E+01			2.82E+01	5.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1316-T04-C	1	2.49E+01			2.49E+01	2.8E-01	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1316-T05-C	1	2.58E+01			2.58E+01	8.1E+00	1.5E+00	4.8E+00					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
V	CFS-L01-1316-B01-A	1	7.50E-01	U1/2		7.50E-01	4.8E+01	1.5E+00	4.8E+00				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	CFS-L01-1316-T01-A	1	2.25E+04			2.25E+04	8.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:26 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1316-T02-A	1	3.14E+04			3.14E+04	3.4E-01	1.0E+00	3.2E+00	10	100	3.23E+04	91%	VU ICP-OES	3/1/11 3:28 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1316-T03-A	1	4.98E+04			4.98E+04	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:30 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1316-T04-A	1	6.01E+04			6.01E+04	6.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 4:09 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1316-T05-A	1	7.52E+04			7.52E+04	3.5E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:33 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1316-T01-B	1	2.31E+04			2.31E+04	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:34 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1316-T02-B	1	3.31E+04			3.31E+04	7.0E-01	1.0E+00	3.2E+00	10	100	3.40E+04	93%	VU ICP-OES	3/1/11 3:36 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1316-T03-B	1	4.86E+04			4.86E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:38 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1316-T04-B	1	5.71E+04			5.71E+04	1.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:39 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1316-T05-B	1	7.38E+04			7.38E+04	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:41 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1316-T01-C	1	2.40E+04			2.40E+04	9.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:43 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1316-T02-C	1	3.36E+04			3.36E+04	3.7E-01	1.0E+00	3.2E+00	10	100	3.45E+04	92%	VU ICP-OES	3/1/11 3:44 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1316-T03-C	1	4.97E+04			4.97E+04	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:46 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1316-T04-C	1	5.95E+04			5.95E+04	2.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:48 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1316-T05-C	1	7.85E+04			7.85E+04	5.4E-01	1.0E+00	3.2E+00					VU ICP-OES	3/1/11 3:49 PM	EPA Interlab L01 1313-1316 CFS
Zn	CFS-L01-1316-B01-A	1	2.03E+00	E		2.03E+00	5.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	3/1/11 3:25 PM	EPA Interlab L01 1313-1316 CFS

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	CFS-L04-1316-T01-A	1	4.42E+01			4.42E+01	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1316-T02-A	1	6.42E+01			6.42E+01	9.9E+00	1.0E+00	3.2E+00	1000	100	1.16E+03	110%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1316-T03-A	1	1.23E+02			1.23E+02	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1316-T04-A	1	5.37E+01			5.37E+01	1.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1316-T05-A	1	5.60E+01			5.60E+01	8.8E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1316-T01-B	1	4.57E+01			4.57E+01	5.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1316-T02-B	1	4.58E+01			4.58E+01	4.5E+00	1.0E+00	3.2E+00	1000	100	1.18E+03	113%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1316-T03-B	1	4.95E+01			4.95E+01	5.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1316-T04-B	1	5.40E+01			5.40E+01	9.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1316-T05-B	1	6.35E+01			6.35E+01	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1316-T01-C	1	4.34E+01			4.34E+01	4.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1316-T02-C	1	4.70E+01			4.70E+01	1.0E+01	1.0E+00	3.2E+00	1000	100	1.16E+03	111%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1316-T03-C	1	5.33E+01			5.33E+01	7.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1316-T04-C	1	5.55E+01			5.55E+01	5.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1316-T05-C	1	5.02E+01			5.02E+01	3.4E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1316-B01-A	1	1.08E+01			1.08E+01	5.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1316-B02-A	1	2.81E+00	E		2.81E+00	3.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
Al	CFS-L04-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	3.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	CFS-L04-1316-T01-A	1	3.00E+01			3.00E+01	2.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1316-T02-A	1	3.72E+01			3.72E+01	4.2E+01	7.5E+00	2.4E+01	10	100	1.07E+03	103%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1316-T03-A	1	5.39E+01			5.39E+01	7.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1316-T04-A	1	6.27E+01			6.27E+01	1.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1316-T05-A	1	7.04E+01			7.04E+01	1.2E+01	7.5E+00	2.4E+01					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1316-T01-B	1	1.97E+01	E		1.97E+01	3.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1316-T02-B	1	3.96E+01			3.96E+01	2.3E+01	7.5E+00	2.4E+01	10	100	1.09E+03	105%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1316-T03-B	1	3.48E+01			3.48E+01	2.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1316-T04-B	1	4.71E+01			4.71E+01	1.4E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1316-T05-B	1	6.29E+01			6.29E+01	1.9E+01	7.5E+00	2.4E+01					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1316-T01-C	1	4.14E+01			4.14E+01	1.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1316-T02-C	1	4.02E+01			4.02E+01	1.9E+01	7.5E+00	2.4E+01	10	100	1.08E+03	104%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1316-T03-C	1	4.63E+01			4.63E+01	4.5E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1316-T04-C	1	5.54E+01			5.54E+01	3.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1316-T05-C	1	6.35E+01			6.35E+01	9.4E+00	7.5E+00	2.4E+01					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1316-B01-A	1	8.16E+00	E		8.16E+00	7.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1316-B02-A	1	3.75E+00	U1/2		3.75E+00	2.9E+02	7.5E+00	2.4E+01				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
Sb	CFS-L04-1316-B03-A	1	3.75E+00	U1/2		3.75E+00	9.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	CFS-L04-1316-T01-A	1	1.59E+01	E		1.59E+01	1.4E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1316-T02-A	1	5.70E+01			5.70E+01	9.3E+00	1.1E+01	3.5E+01	10	100	1.08E+03	102%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1316-T03-A	1	1.14E+02			1.14E+02	8.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1316-T04-A	1	4.56E+01			4.56E+01	1.6E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1316-T05-A	1	4.58E+01			4.58E+01	1.3E+01	1.1E+01	3.5E+01					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1316-T01-B	1	2.90E+01	E		2.90E+01	2.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1316-T02-B	1	2.85E+01	E		2.85E+01	2.4E+01	1.1E+01	3.5E+01	10	100	1.11E+03	108%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1316-T03-B	1	2.90E+01	E		2.90E+01	3.5E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1316-T04-B	1	4.57E+01			4.57E+01	6.0E+00	1.1E+01	3.5E+01				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1316-T05-B	1	5.15E+01			5.15E+01	6.3E+00	1.1E+01	3.5E+01					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1316-T01-C	1	2.00E+01	E		2.00E+01	2.8E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1316-T02-C	1	2.95E+01	E		2.95E+01	2.0E+01	1.1E+01	3.5E+01	10	100	1.10E+03	107%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1316-T03-C	1	3.61E+01			3.61E+01	2.0E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1316-T04-C	1	4.81E+01			4.81E+01	1.7E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1316-T05-C	1	4.79E+01			4.79E+01	2.5E+01	1.1E+01	3.5E+01					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1316-B01-A	1	1.62E+01	E		1.62E+01	1.5E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1316-B02-A	1	5.50E+00	U1/2		5.50E+00	2.2E+02	1.1E+01	3.5E+01				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
As	CFS-L04-1316-B03-A	1	5.50E+00	U1/2		5.50E+00	5.6E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	CFS-L04-1316-T01-A	1	1.34E+02			1.34E+02	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1316-T02-A	1	2.69E+02			2.69E+02	1.0E+00	1.0E+00	3.2E+00	1000	100	1.24E+03	97%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1316-T03-A	1	5.94E+02			5.94E+02	6.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1316-T04-A	1	9.94E+02			9.94E+02	8.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1316-T05-A	1	1.70E+03			1.70E+03	1.7E-01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1316-T01-B	1	1.21E+02			1.21E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1316-T02-B	1	2.48E+02			2.48E+02	2.1E+00	1.0E+00	3.2E+00	1000	100	1.24E+03	99%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1316-T03-B	1	5.25E+02			5.25E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1316-T04-B	1	8.40E+02			8.40E+02	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1316-T05-B	1	1.47E+03			1.47E+03	1.3E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1316-T01-C	1	1.34E+02			1.34E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1316-T02-C	1	2.61E+02			2.61E+02	1.1E+00	1.0E+00	3.2E+00	1000	100	1.23E+03	97%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1316-T03-C	1	5.50E+02			5.50E+02	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1316-T04-C	1	8.88E+02			8.88E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1316-T05-C	1	1.61E+03			1.61E+03	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	6.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
B	CFS-L04-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	CFS-L04-1316-T01-A	1	2.23E+02			2.23E+02	1.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1316-T02-A	1	2.79E+02			2.79E+02	1.2E-01	1.0E+00	3.2E+00	10	100	1.15E+03	87%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1316-T03-A	1	4.12E+02			4.12E+02	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1316-T04-A	1	6.05E+02			6.05E+02	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1316-T05-A	1	1.27E+03			1.27E+03	4.4E-01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1316-T01-B	1	2.11E+02			2.11E+02	3.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1316-T02-B	1	2.70E+02			2.70E+02	1.1E+00	1.0E+00	3.2E+00	10	100	1.17E+03	90%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1316-T03-B	1	4.00E+02			4.00E+02	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1316-T04-B	1	5.73E+02			5.73E+02	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1316-T05-B	1	1.36E+03			1.36E+03	1.0E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1316-T01-C	1	2.21E+02			2.21E+02	8.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1316-T02-C	1	2.69E+02			2.69E+02	6.2E-01	1.0E+00	3.2E+00	10	100	1.16E+03	89%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1316-T03-C	1	3.95E+02			3.95E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1316-T04-C	1	5.99E+02			5.99E+02	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1316-T05-C	1	1.31E+03			1.31E+03	1.5E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	5.6E+02	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	3.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
Ba	CFS-L04-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	6.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	CFS-L04-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	6.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00	10	100	1.05E+03	105%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	4.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	2.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1316-T05-A	1	9.50E-01	U1/2		9.50E-01	4.9E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	8.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	3.0E+01	1.9E+00	6.0E+00	10	100	1.05E+03	105%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	5.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	8.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1316-T05-B	1	9.50E-01	U1/2		9.50E-01	2.0E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	2.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	2.1E+01	1.9E+00	6.0E+00	10	100	1.05E+03	105%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	6.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	2.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1316-T05-C	1	9.50E-01	U1/2		9.50E-01	5.6E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	4.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1316-B02-A	1	9.50E-01	U1/2		9.50E-01	5.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
Be	CFS-L04-1316-B03-A	1	9.50E-01	U1/2		9.50E-01	3.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	CFS-L04-1316-T01-A	1	4.60E+03			4.60E+03	3.6E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1316-T02-A	1	5.75E+03			5.75E+03	5.0E-01	2.2E+00	7.0E+00	10	100	6.64E+03	89%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1316-T03-A	1	9.71E+03			9.71E+03	3.5E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1316-T04-A	1	1.14E+04			1.14E+04	5.6E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1316-T05-A	1	1.23E+04			1.23E+04	1.2E-01	2.2E+00	7.0E+00					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1316-T01-B	1	4.16E+03			4.16E+03	2.5E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1316-T02-B	1	5.79E+03			5.79E+03	8.8E-01	2.2E+00	7.0E+00	10	100	6.75E+03	96%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1316-T03-B	1	8.34E+03			8.34E+03	4.9E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1316-T04-B	1	1.01E+04			1.01E+04	5.1E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1316-T05-B	1	1.17E+04			1.17E+04	1.2E+01	2.2E+00	7.0E+00					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1316-T01-C	1	4.48E+03			4.48E+03	8.3E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1316-T02-C	1	6.32E+03			6.32E+03	2.1E-01	2.2E+00	7.0E+00	10	100	7.25E+03	94%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1316-T03-C	1	9.00E+03			9.00E+03	9.9E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1316-T04-C	1	1.09E+04			1.09E+04	2.7E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1316-T05-C	1	1.30E+04			1.30E+04	8.7E-01	2.2E+00	7.0E+00					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1316-B01-A	1	7.97E+00			7.97E+00	2.7E+00	2.2E+00	7.0E+00				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1316-B02-A	1	1.10E+00	U1/2		1.10E+00	1.7E+02	2.2E+00	7.0E+00				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
Cd	CFS-L04-1316-B03-A	1	1.10E+00	U1/2		1.10E+00	1.0E+02	2.2E+00	7.0E+00				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	CFS-L04-1316-T01-A	1	6.42E+05			6.42E+05	3.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1316-T02-A	1	6.41E+05			6.41E+05	8.3E-02	2.6E+00	8.3E+00	1000	100	6.42E+05	92%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1316-T03-A	1	6.06E+05			6.06E+05	6.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1316-T04-A	1	5.81E+05			5.81E+05	7.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1316-T05-A	1	5.19E+05			5.19E+05	3.1E-01	2.6E+00	8.3E+00					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1316-T01-B	1	6.31E+05			6.31E+05	1.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1316-T02-B	1	6.31E+05			6.31E+05	5.8E-01	2.6E+00	8.3E+00	1000	100	6.32E+05	88%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1316-T03-B	1	5.95E+05			5.95E+05	6.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1316-T04-B	1	5.52E+05			5.52E+05	2.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1316-T05-B	1	5.11E+05			5.11E+05	1.2E+01	2.6E+00	8.3E+00					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1316-T01-C	1	6.42E+05			6.42E+05	6.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1316-T02-C	1	6.23E+05			6.23E+05	7.4E-01	2.6E+00	8.3E+00	1000	100	6.24E+05	89%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1316-T03-C	1	5.85E+05			5.85E+05	5.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1316-T04-C	1	5.57E+05			5.57E+05	5.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1316-T05-C	1	5.08E+05			5.08E+05	9.4E-01	2.6E+00	8.3E+00					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1316-B01-A	1	4.59E+02			4.59E+02	4.6E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1316-B02-A	1	4.90E+00	E		4.90E+00	2.4E+02	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
Ca	CFS-L04-1316-B03-A	1	1.30E+00	U1/2		1.30E+00	1.4E+02	2.6E+00	8.3E+00				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	CFS-L04-1316-T01-A	1	6.00E-01	U1/2		6.00E-01	2.4E+02	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1316-T02-A	1	6.00E-01	U1/2		6.00E-01	1.6E+02	1.2E+00	3.8E+00	10	100	1.01E+03	101%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1316-T03-A	1	1.65E+00	E		1.65E+00	3.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1316-T04-A	1	6.00E-01	U1/2		6.00E-01	1.0E+02	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1316-T05-A	1	1.39E+00	E		1.39E+00	5.2E+01	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1316-T01-B	1	6.00E-01	U1/2		6.00E-01	5.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1316-T02-B	1	6.00E-01	U1/2		6.00E-01	3.2E+01	1.2E+00	3.8E+00	10	100	1.04E+03	104%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1316-T03-B	1	6.00E-01	U1/2		6.00E-01	6.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1316-T04-B	1	6.00E-01	U1/2		6.00E-01	5.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1316-T05-B	1	6.00E-01	U1/2		6.00E-01	5.7E+01	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1316-T01-C	1	6.00E-01	U1/2		6.00E-01	1.5E+02	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1316-T02-C	1	6.00E-01	U1/2		6.00E-01	2.1E+02	1.2E+00	3.8E+00	10	100	1.03E+03	103%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1316-T03-C	1	6.00E-01	U1/2		6.00E-01	1.4E+02	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1316-T04-C	1	6.00E-01	U1/2		6.00E-01	8.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1316-T05-C	1	6.00E-01	U1/2		6.00E-01	2.5E+01	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	1.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	2.1E+02	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
Cr	CFS-L04-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	5.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	CFS-L04-1316-T01-A	1	1.02E+02			1.02E+02	4.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1316-T02-A	1	1.46E+02			1.46E+02	1.1E+00	1.8E+00	5.7E+00	10	100	1.14E+03	99%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1316-T03-A	1	3.36E+02			3.36E+02	1.4E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1316-T04-A	1	4.37E+02			4.37E+02	2.2E-02	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1316-T05-A	1	5.20E+02			5.20E+02	5.6E-01	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1316-T01-B	1	8.72E+01			8.72E+01	7.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1316-T02-B	1	1.54E+02			1.54E+02	4.5E-02	1.8E+00	5.7E+00	10	100	1.17E+03	102%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1316-T03-B	1	2.73E+02			2.73E+02	1.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1316-T04-B	1	3.65E+02			3.65E+02	6.3E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1316-T05-B	1	4.71E+02			4.71E+02	1.2E+01	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1316-T01-C	1	1.00E+02			1.00E+02	5.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1316-T02-C	1	1.72E+02			1.72E+02	5.4E-01	1.8E+00	5.7E+00	10	100	1.18E+03	100%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1316-T03-C	1	3.08E+02			3.08E+02	6.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1316-T04-C	1	4.21E+02			4.21E+02	3.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1316-T05-C	1	5.61E+02			5.61E+02	1.2E+00	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	7.1E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1316-B02-A	1	9.00E-01	U1/2		9.00E-01	1.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
Co	CFS-L04-1316-B03-A	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	CFS-L04-1316-T01-A	1	8.22E+02			8.22E+02	1.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1316-T02-A	1	8.33E+02			8.33E+02	8.1E-01	3.7E+00	1.2E+01	10	100	1.77E+03	94%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1316-T03-A	1	1.83E+03			1.83E+03	7.2E-01	3.7E+00	1.2E+01				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1316-T04-A	1	1.94E+03			1.94E+03	1.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1316-T05-A	1	1.20E+03			1.20E+03	7.3E-01	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1316-T01-B	1	6.94E+02			6.94E+02	4.7E-01	3.7E+00	1.2E+01				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1316-T02-B	1	8.71E+02			8.71E+02	1.2E+00	3.7E+00	1.2E+01	10	100	1.83E+03	96%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1316-T03-B	1	1.41E+03			1.41E+03	1.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1316-T04-B	1	1.79E+03			1.79E+03	4.9E-01	3.7E+00	1.2E+01				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1316-T05-B	1	1.38E+03			1.38E+03	1.1E+01	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1316-T01-C	1	7.64E+02			7.64E+02	9.9E-01	3.7E+00	1.2E+01				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1316-T02-C	1	9.92E+02			9.92E+02	7.4E-01	3.7E+00	1.2E+01	10	100	1.92E+03	92%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1316-T03-C	1	1.55E+03			1.55E+03	1.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1316-T04-C	1	2.11E+03			2.11E+03	6.9E-01	3.7E+00	1.2E+01				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1316-T05-C	1	1.71E+03			1.71E+03	1.5E+00	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1316-B01-A	1	1.64E+02			1.64E+02	3.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1316-B02-A	1	1.85E+00	U1/2		1.85E+00	3.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
Cu	CFS-L04-1316-B03-A	1	1.85E+00	U1/2		1.85E+00	3.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	CFS-L04-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	5.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1316-T02-A	1	7.74E+01			7.74E+01	5.5E+00	2.0E+00	6.4E+00	1000	100	9.90E+02	91%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1316-T03-A	1	3.03E+02			3.03E+02	3.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	4.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1316-T05-A	1	1.00E+00	U1/2		1.00E+00	3.2E+01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	2.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	9.3E+00	2.0E+00	6.4E+00	1000	100	9.47E+02	95%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	3.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1316-T05-B	1	9.79E+00			9.79E+00	1.8E+01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	8.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	7.1E+00	2.0E+00	6.4E+00	1000	100	9.41E+02	94%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	9.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1316-T05-C	1	1.00E+00	U1/2		1.00E+00	4.3E+01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1316-B01-A	1	3.94E+01			3.94E+01	3.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1316-B02-A	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
Fe	CFS-L04-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	2.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	CFS-L04-1316-T01-A	1	1.15E+03			1.15E+03	2.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1316-T02-A	1	1.33E+03			1.33E+03	4.8E-01	6.8E+00	2.2E+01	10	100	2.15E+03	82%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1316-T03-A	1	1.67E+03			1.67E+03	5.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1316-T04-A	1	1.48E+03			1.48E+03	8.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1316-T05-A	1	2.11E+02			2.11E+02	2.4E+00	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1316-T01-B	1	1.00E+03			1.00E+03	6.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1316-T02-B	1	1.14E+03			1.14E+03	1.1E+00	6.8E+00	2.2E+01	10	100	2.01E+03	87%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1316-T03-B	1	1.27E+03			1.27E+03	1.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1316-T04-B	1	1.30E+03			1.30E+03	6.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1316-T05-B	1	2.01E+02			2.01E+02	1.1E+01	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1316-T01-C	1	1.05E+03			1.05E+03	4.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1316-T02-C	1	1.20E+03			1.20E+03	2.2E-01	6.8E+00	2.2E+01	10	100	2.04E+03	84%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1316-T03-C	1	1.33E+03			1.33E+03	1.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1316-T04-C	1	1.37E+03			1.37E+03	3.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1316-T05-C	1	1.53E+02			1.53E+02	2.1E+00	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1316-B01-A	1	6.91E+00	E		6.91E+00	3.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1316-B02-A	1	3.40E+00	U1/2		3.40E+00	2.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
Pb	CFS-L04-1316-B03-A	1	3.40E+00	U1/2		3.40E+00	1.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	CFS-L04-1316-T01-A	1	1.77E+01			1.77E+01	2.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1316-T02-A	1	1.93E+01			1.93E+01	3.3E+00	1.9E+00	6.0E+00	10	100	8.81E+02	86%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1316-T03-A	1	1.73E+01			1.73E+01	7.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1316-T04-A	1	1.57E+01			1.57E+01	1.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1316-T05-A	1	2.49E+01			2.49E+01	7.5E+00	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1316-T01-B	1	1.82E+01			1.82E+01	1.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1316-T02-B	1	1.79E+01			1.79E+01	7.2E+00	1.9E+00	6.0E+00	10	100	8.97E+02	88%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1316-T03-B	1	1.44E+01			1.44E+01	6.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1316-T04-B	1	1.18E+01			1.18E+01	1.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1316-T05-B	1	1.86E+01			1.86E+01	1.2E+01	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1316-T01-C	1	1.68E+01			1.68E+01	1.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1316-T02-C	1	1.66E+01			1.66E+01	2.4E+00	1.9E+00	6.0E+00	10	100	8.99E+02	88%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1316-T03-C	1	1.48E+01			1.48E+01	2.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1316-T04-C	1	1.38E+01			1.38E+01	9.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1316-T05-C	1	2.26E+01			2.26E+01	3.0E+00	1.9E+00	6.0E+00					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1316-B01-A	1	6.76E+00			6.76E+00	4.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1316-B02-A	1	8.06E+00			8.06E+00	1.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
Li	CFS-L04-1316-B03-A	1	7.60E+00			7.60E+00	7.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	CFS-L04-1316-T01-A	1	1.59E+03			1.59E+03	6.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1316-T02-A	1	2.68E+03			2.68E+03	6.8E-01	2.0E+00	6.4E+00	10	100	3.71E+03	103%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1316-T03-A	1	6.29E+03			6.29E+03	3.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1316-T04-A	1	9.25E+03			9.25E+03	3.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1316-T05-A	1	1.24E+04			1.24E+04	4.6E-01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1316-T01-B	1	1.34E+03			1.34E+03	1.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1316-T02-B	1	2.62E+03			2.62E+03	8.0E-01	2.0E+00	6.4E+00	10	100	3.72E+03	110%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1316-T03-B	1	5.14E+03			5.14E+03	5.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1316-T04-B	1	7.70E+03			7.70E+03	2.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1316-T05-B	1	1.09E+04			1.09E+04	1.2E+01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1316-T01-C	1	1.53E+03			1.53E+03	6.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1316-T02-C	1	2.83E+03			2.83E+03	6.4E-01	2.0E+00	6.4E+00	10	100	3.77E+03	94%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1316-T03-C	1	5.61E+03			5.61E+03	9.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1316-T04-C	1	8.61E+03			8.61E+03	6.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1316-T05-C	1	1.28E+04			1.28E+04	9.7E-01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1316-B01-A	1	5.71E+00	E		5.71E+00	4.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1316-B02-A	1	1.00E+00	U1/2		1.00E+00	8.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
Mn	CFS-L04-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	2.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	CFS-L04-1316-T01-A	1	6.87E+04			6.87E+04	1.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1316-T02-A	1	1.36E+05			1.36E+05	1.4E+00	1.0E+00	3.2E+00	1000	100	1.37E+05	94%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1316-T03-A	1	3.08E+05			3.08E+05	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1316-T04-A	1	5.69E+05			5.69E+05	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1316-T05-A	1	9.41E+05			9.41E+05	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1316-T01-B	1	6.65E+04			6.65E+04	6.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1316-T02-B	1	1.36E+05			1.36E+05	4.3E-01	1.0E+00	3.2E+00	1000	100	1.37E+05	105%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1316-T03-B	1	3.03E+05			3.03E+05	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1316-T04-B	1	5.24E+05			5.24E+05	2.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1316-T05-B	1	8.90E+05			8.90E+05	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1316-T01-C	1	6.96E+04			6.96E+04	9.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1316-T02-C	1	1.35E+05			1.35E+05	3.9E-01	1.0E+00	3.2E+00	1000	100	1.36E+05	92%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1316-T03-C	1	3.06E+05			3.06E+05	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1316-T04-C	1	5.49E+05			5.49E+05	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1316-T05-C	1	9.19E+05			9.19E+05	4.7E-01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1316-B01-A	1	5.36E+01			5.36E+01	1.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	7.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
Mg	CFS-L04-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	5.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	CFS-L04-1316-T01-A	1	1.22E+01			1.22E+01	8.4E-01	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1316-T02-A	1	1.43E+01			1.43E+01	4.0E+00	1.2E+00	3.8E+00	10	100	1.01E+03	100%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1316-T03-A	1	2.08E+01			2.08E+01	6.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1316-T04-A	1	1.93E+01			1.93E+01	8.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1316-T05-A	1	2.41E+01			2.41E+01	8.8E+00	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1316-T01-B	1	9.82E+00			9.82E+00	4.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1316-T02-B	1	1.10E+01			1.10E+01	1.4E+01	1.2E+00	3.8E+00	10	100	1.04E+03	103%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1316-T03-B	1	1.63E+01			1.63E+01	9.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1316-T04-B	1	1.68E+01			1.68E+01	7.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1316-T05-B	1	2.27E+01			2.27E+01	4.5E+00	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1316-T01-C	1	1.04E+01			1.04E+01	3.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1316-T02-C	1	1.39E+01			1.39E+01	2.4E+00	1.2E+00	3.8E+00	10	100	1.04E+03	103%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1316-T03-C	1	1.48E+01			1.48E+01	8.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1316-T04-C	1	1.77E+01			1.77E+01	7.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1316-T05-C	1	2.24E+01			2.24E+01	2.2E+00	1.2E+00	3.8E+00					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1316-B01-A	1	2.93E+00	E		2.93E+00	5.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1316-B02-A	1	3.20E+00	E		3.20E+00	3.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
Mo	CFS-L04-1316-B03-A	1	1.98E+00	E		1.98E+00	1.8E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	CFS-L04-1316-T01-A	1	2.08E+02			2.08E+02	6.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1316-T02-A	1	2.76E+02			2.76E+02	1.1E+00	1.8E+00	5.7E+00	10	100	1.26E+03	98%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1316-T03-A	1	5.91E+02			5.91E+02	5.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1316-T04-A	1	7.16E+02			7.16E+02	1.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1316-T05-A	1	8.22E+02			8.22E+02	4.3E-01	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1316-T01-B	1	1.72E+02			1.72E+02	3.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1316-T02-B	1	2.92E+02			2.92E+02	1.7E+00	1.8E+00	5.7E+00	10	100	1.30E+03	101%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1316-T03-B	1	4.77E+02			4.77E+02	5.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1316-T04-B	1	6.03E+02			6.03E+02	3.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1316-T05-B	1	7.47E+02			7.47E+02	1.2E+01	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1316-T01-C	1	1.96E+02			1.96E+02	2.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1316-T02-C	1	3.39E+02			3.39E+02	8.8E-01	1.8E+00	5.7E+00	10	100	1.33E+03	99%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1316-T03-C	1	5.46E+02			5.46E+02	1.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1316-T04-C	1	7.03E+02			7.03E+02	4.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1316-T05-C	1	8.93E+02			8.93E+02	1.2E+00	1.8E+00	5.7E+00					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1316-B02-A	1	9.00E-01	U1/2		9.00E-01	7.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
Ni	CFS-L04-1316-B03-A	1	9.00E-01	U1/2		9.00E-01	9.0E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	CFS-L04-1316-T01-A	1	1.95E+01			1.95E+01	5.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1316-T02-A	1	3.08E+01			3.08E+01	1.0E+01	3.7E+00	1.2E+01	1000	100	1.04E+03	101%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1316-T03-A	1	3.63E+01			3.63E+01	1.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1316-T04-A	1	4.80E+01			4.80E+01	1.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1316-T05-A	1	6.39E+01			6.39E+01	1.4E+01	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1316-T01-B	1	5.19E+01			5.19E+01	8.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1316-T02-B	1	3.65E+01			3.65E+01	2.0E+01	3.7E+00	1.2E+01	1000	100	1.08E+03	105%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1316-T03-B	1	3.85E+01			3.85E+01	2.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1316-T04-B	1	4.58E+01			4.58E+01	1.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1316-T05-B	1	5.68E+01			5.68E+01	1.5E+01	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1316-T01-C	1	2.84E+01			2.84E+01	2.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1316-T02-C	1	5.41E+01			5.41E+01	4.1E+01	3.7E+00	1.2E+01	1000	100	1.05E+03	99%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1316-T03-C	1	3.32E+01			3.32E+01	3.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1316-T04-C	1	5.75E+01			5.75E+01	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1316-T05-C	1	7.74E+01			7.74E+01	1.1E+01	3.7E+00	1.2E+01					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1316-B01-A	1	2.45E+01			2.45E+01	4.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1316-B02-A	1	1.87E+01			1.87E+01	4.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
P	CFS-L04-1316-B03-A	1	2.59E+01			2.59E+01	3.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	CFS-L04-1316-T01-A	1	1.03E+04			1.03E+04	6.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1316-T02-A	1	1.95E+04			1.95E+04	4.3E-01	1.6E+00	5.1E+00	1000	100	2.04E+04	95%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1316-T03-A	1	3.68E+04			3.68E+04	2.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1316-T04-A	1	5.87E+04			5.87E+04	2.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1316-T05-A	1	7.91E+04			7.91E+04	7.3E-01	1.6E+00	5.1E+00					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1316-T01-B	1	9.94E+03			9.94E+03	1.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1316-T02-B	1	1.83E+04			1.83E+04	8.3E-01	1.6E+00	5.1E+00	1000	100	1.93E+04	100%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1316-T03-B	1	3.44E+04			3.44E+04	9.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1316-T04-B	1	5.37E+04			5.37E+04	9.9E-02	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1316-T05-B	1	7.81E+04			7.81E+04	1.2E+01	1.6E+00	5.1E+00					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1316-T01-C	1	1.02E+04			1.02E+04	8.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1316-T02-C	1	1.85E+04			1.85E+04	2.8E-01	1.6E+00	5.1E+00	1000	100	1.94E+04	96%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1316-T03-C	1	3.46E+04			3.46E+04	9.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1316-T04-C	1	5.42E+04			5.42E+04	4.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1316-T05-C	1	7.82E+04			7.82E+04	8.1E-01	1.6E+00	5.1E+00					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1316-B01-A	1	1.25E+02			1.25E+02	3.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1316-B02-A	1	7.90E+01			7.90E+01	2.0E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
K	CFS-L04-1316-B03-A	1	7.79E+01			7.79E+01	2.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	CFS-L04-1316-T01-A	1	7.30E+01			7.30E+01	1.6E+01	1.5E+01	4.8E+01				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1316-T02-A	1	1.41E+02			1.41E+02	9.6E+00	1.5E+01	4.8E+01	10	100	1.16E+03	102%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1316-T03-A	1	3.05E+02			3.05E+02	5.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1316-T04-A	1	5.48E+02			5.48E+02	2.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1316-T05-A	1	9.06E+02			9.06E+02	1.6E+00	1.5E+01	4.8E+01					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1316-T01-B	1	6.33E+01			6.33E+01	1.3E+01	1.5E+01	4.8E+01				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1316-T02-B	1	1.36E+02			1.36E+02	3.0E+00	1.5E+01	4.8E+01	10	100	1.18E+03	104%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1316-T03-B	1	2.82E+02			2.82E+02	7.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1316-T04-B	1	5.08E+02			5.08E+02	7.1E-01	1.5E+01	4.8E+01				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1316-T05-B	1	8.92E+02			8.92E+02	1.1E+01	1.5E+01	4.8E+01					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1316-T01-C	1	7.95E+01			7.95E+01	2.5E+01	1.5E+01	4.8E+01				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1316-T02-C	1	1.30E+02			1.30E+02	6.5E+00	1.5E+01	4.8E+01	10	100	1.16E+03	103%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1316-T03-C	1	2.97E+02			2.97E+02	6.6E-01	1.5E+01	4.8E+01				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1316-T04-C	1	5.26E+02			5.26E+02	1.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1316-T05-C	1	8.55E+02			8.55E+02	2.3E+00	1.5E+01	4.8E+01					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1316-B01-A	1	7.50E+00	U1/2		7.50E+00	3.8E+01	1.5E+01	4.8E+01				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1316-B02-A	1	7.50E+00	U1/2		7.50E+00	2.6E+02	1.5E+01	4.8E+01				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
Se	CFS-L04-1316-B03-A	1	7.50E+00	U1/2		7.50E+00	1.3E+02	1.5E+01	4.8E+01				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	CFS-L04-1316-T01-A	1	3.93E+03			3.93E+03	7.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1316-T02-A	1	4.87E+03			4.87E+03	8.9E-01	1.1E+00	3.5E+00	1000	100	5.72E+03	85%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1316-T03-A	1	6.71E+03			6.71E+03	6.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1316-T04-A	1	6.85E+03			6.85E+03	5.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1316-T05-A	1	6.81E+03			6.81E+03	2.9E-01	1.1E+00	3.5E+00					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1316-T01-B	1	3.46E+03			3.46E+03	2.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1316-T02-B	1	4.68E+03			4.68E+03	1.8E+00	1.1E+00	3.5E+00	1000	100	5.63E+03	95%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1316-T03-B	1	5.73E+03			5.73E+03	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1316-T04-B	1	6.03E+03			6.03E+03	2.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1316-T05-B	1	6.45E+03			6.45E+03	1.2E+01	1.1E+00	3.5E+00					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1316-T01-C	1	3.74E+03			3.74E+03	7.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1316-T02-C	1	4.84E+03			4.84E+03	3.1E-01	1.1E+00	3.5E+00	1000	100	5.77E+03	93%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1316-T03-C	1	6.03E+03			6.03E+03	1.9E+00	1.1E+00	3.5E+00				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1316-T04-C	1	6.41E+03			6.41E+03	3.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1316-T05-C	1	6.89E+03			6.89E+03	7.3E-01	1.1E+00	3.5E+00					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1316-B01-A	1	6.31E+01			6.31E+01	1.3E+01	1.1E+00	3.5E+00				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1316-B02-A	1	1.31E+01			1.31E+01	2.6E+01	1.1E+00	3.5E+00				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
Si	CFS-L04-1316-B03-A	1	6.93E+00			6.93E+00	2.5E+01	1.1E+00	3.5E+00				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	CFS-L04-1316-T01-A	1	2.06E+04			2.06E+04	1.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1316-T02-A	1	3.77E+04			3.77E+04	5.4E-01	2.5E+00	8.0E+00	1000	100	3.86E+04	92%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1316-T03-A	1	8.02E+04			8.02E+04	1.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1316-T04-A	1	1.26E+05			1.26E+05	3.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1316-T05-A	1	1.93E+05			1.93E+05	4.1E-01	2.5E+00	8.0E+00					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1316-T01-B	1	2.04E+04			2.04E+04	7.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1316-T02-B	1	3.75E+04			3.75E+04	8.2E-01	2.5E+00	8.0E+00	1000	100	3.85E+04	102%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1316-T03-B	1	7.84E+04			7.84E+04	5.3E-02	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1316-T04-B	1	1.24E+05			1.24E+05	4.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1316-T05-B	1	1.90E+05			1.90E+05	3.2E+00	2.5E+00	8.0E+00					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1316-T01-C	1	2.05E+04			2.05E+04	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1316-T02-C	1	3.77E+04			3.77E+04	1.1E+00	2.5E+00	8.0E+00	1000	100	3.87E+04	103%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1316-T03-C	1	7.59E+04			7.59E+04	3.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1316-T04-C	1	1.20E+05			1.20E+05	3.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1316-T05-C	1	1.88E+05			1.88E+05	6.3E-01	2.5E+00	8.0E+00					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1316-B01-A	1	7.33E+01			7.33E+01	3.7E+00	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1316-B02-A	1	1.61E+01			1.61E+01	1.4E+01	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
Na	CFS-L04-1316-B03-A	1	1.33E+01			1.33E+01	1.6E+01	2.5E+00	8.0E+00				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	CFS-L04-1316-T01-A	1	1.54E+03			1.54E+03	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1316-T02-A	1	2.65E+03			2.65E+03	4.1E-01	1.0E+00	3.2E+00	1000	100	3.57E+03	92%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1316-T03-A	1	3.48E+03			3.48E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1316-T04-A	1	4.55E+03			4.55E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1316-T05-A	1	5.10E+03			5.10E+03	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1316-T01-B	1	1.49E+03			1.49E+03	5.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1316-T02-B	1	2.30E+03			2.30E+03	1.5E+00	1.0E+00	3.2E+00	1000	100	3.17E+03	87%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1316-T03-B	1	3.45E+03			3.45E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1316-T04-B	1	4.32E+03			4.32E+03	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1316-T05-B	1	5.00E+03			5.00E+03	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1316-T01-C	1	1.53E+03			1.53E+03	4.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1316-T02-C	1	2.23E+03			2.23E+03	5.2E-01	1.0E+00	3.2E+00	1000	100	3.13E+03	91%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1316-T03-C	1	3.34E+03			3.34E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1316-T04-C	1	4.09E+03			4.09E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1316-T05-C	1	4.75E+03			4.75E+03	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	5.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	7.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
Sr	CFS-L04-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	1.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	CFS-L04-1316-T01-A	1	6.20E+05			6.20E+05	7.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1316-T02-A	1	7.14E+05			7.14E+05	2.4E-01	6.8E+00	2.2E+01	1000	100	7.15E+05	87%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1316-T03-A	1	9.19E+05			9.19E+05	5.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1316-T04-A	1	1.22E+06			1.22E+06	8.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1316-T05-A	1	1.58E+06			1.58E+06	2.3E-01	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1316-T01-B	1	6.10E+05			6.10E+05	1.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1316-T02-B	1	7.03E+05			7.03E+05	8.6E-01	6.8E+00	2.2E+01	1000	100	7.04E+05	90%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1316-T03-B	1	9.06E+05			9.06E+05	3.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1316-T04-B	1	1.16E+06			1.16E+06	5.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1316-T05-B	1	1.57E+06			1.57E+06	1.1E+01	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1316-T01-C	1	6.35E+05			6.35E+05	9.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1316-T02-C	1	7.09E+05			7.09E+05	3.5E-01	6.8E+00	2.2E+01	1000	100	7.10E+05	94%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1316-T03-C	1	8.99E+05			8.99E+05	8.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1316-T04-C	1	1.18E+06			1.18E+06	2.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1316-T05-C	1	1.56E+06			1.56E+06	9.0E-01	6.8E+00	2.2E+01					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	4.6E+02	6.8E+00	2.2E+01				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1316-B02-A	1	3.40E+00	U1/2		3.40E+00	5.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
S	CFS-L04-1316-B03-A	1	3.40E+00	U1/2		3.40E+00	3.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	CFS-L04-1316-T01-A	1	3.27E+02			3.27E+02	1.1E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1316-T02-A	1	4.96E+02			4.96E+02	2.8E-01	4.6E+00	1.5E+01	10	100	1.39E+03	89%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1316-T03-A	1	8.16E+02			8.16E+02	1.1E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1316-T04-A	1	1.11E+03			1.11E+03	1.0E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1316-T05-A	1	5.06E+02			5.06E+02	1.5E+00	4.6E+00	1.5E+01					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1316-T01-B	1	2.95E+02			2.95E+02	9.5E-01	4.6E+00	1.5E+01				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1316-T02-B	1	4.50E+02			4.50E+02	2.0E+00	4.6E+00	1.5E+01	10	100	1.35E+03	90%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1316-T03-B	1	7.18E+02			7.18E+02	1.9E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1316-T04-B	1	9.67E+02			9.67E+02	1.6E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1316-T05-B	1	4.06E+02			4.06E+02	1.2E+01	4.6E+00	1.5E+01					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1316-T01-C	1	3.12E+02			3.12E+02	2.1E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1316-T02-C	1	4.72E+02			4.72E+02	1.9E+00	4.6E+00	1.5E+01	10	100	1.36E+03	89%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1316-T03-C	1	7.46E+02			7.46E+02	8.7E-01	4.6E+00	1.5E+01				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1316-T04-C	1	1.01E+03			1.01E+03	3.9E-01	4.6E+00	1.5E+01				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1316-T05-C	1	3.76E+02			3.76E+02	1.5E+00	4.6E+00	1.5E+01					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1316-B01-A	1	2.30E+00	U1/2		2.30E+00	2.2E+02	4.6E+00	1.5E+01				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1316-B02-A	1	2.30E+00	U1/2		2.30E+00	6.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
Tl	CFS-L04-1316-B03-A	1	2.30E+00	U1/2		2.30E+00	3.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	CFS-L04-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	4.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	2.4E+00	2.0E+00	6.4E+00	10	100	9.41E+02	94%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1316-T05-A	1	1.00E+00	U1/2		1.00E+00	4.4E+00	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	1.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	8.7E+00	2.0E+00	6.4E+00	10	100	9.50E+02	95%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	3.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	1.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1316-T05-B	1	1.00E+00	U1/2		1.00E+00	3.5E+01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	2.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	1.8E+00	2.0E+00	6.4E+00	10	100	9.50E+02	95%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1316-T05-C	1	1.00E+00	U1/2		1.00E+00	1.0E+01	2.0E+00	6.4E+00					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1316-B02-A	1	1.00E+00	U1/2		1.00E+00	5.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
Ti	CFS-L04-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	5.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	CFS-L04-1316-T01-A	1	3.45E+01			3.45E+01	2.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1316-T02-A	1	3.29E+01			3.29E+01	2.6E+00	1.5E+00	4.8E+00	10	100	1.04E+03	101%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1316-T03-A	1	2.94E+01			2.94E+01	2.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1316-T04-A	1	2.88E+01			2.88E+01	7.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1316-T05-A	1	2.52E+01			2.52E+01	3.0E+00	1.5E+00	4.8E+00					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1316-T01-B	1	3.23E+01			3.23E+01	8.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1316-T02-B	1	3.11E+01			3.11E+01	5.3E+00	1.5E+00	4.8E+00	10	100	1.07E+03	103%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1316-T03-B	1	3.01E+01			3.01E+01	1.9E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1316-T04-B	1	2.77E+01			2.77E+01	1.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1316-T05-B	1	2.45E+01			2.45E+01	1.8E+01	1.5E+00	4.8E+00					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1316-T01-C	1	3.25E+01			3.25E+01	3.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1316-T02-C	1	3.18E+01			3.18E+01	2.3E+00	1.5E+00	4.8E+00	10	100	1.06E+03	103%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1316-T03-C	1	2.94E+01			2.94E+01	2.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1316-T04-C	1	2.79E+01			2.79E+01	1.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1316-T05-C	1	2.52E+01			2.52E+01	7.3E+00	1.5E+00	4.8E+00					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1316-B01-A	1	7.50E-01	U1/2		7.50E-01	1.1E+02	1.5E+00	4.8E+00				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1316-B02-A	1	7.50E-01	U1/2		7.50E-01	1.1E+02	1.5E+00	4.8E+00				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
V	CFS-L04-1316-B03-A	1	7.50E-01	U1/2		7.50E-01	8.2E+01	1.5E+00	4.8E+00				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	CFS-L04-1316-T01-A	1	2.00E+04			2.00E+04	2.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:59 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1316-T02-A	1	2.17E+04			2.17E+04	1.8E+00	1.0E+00	3.2E+00	10	100	2.28E+04	111%	VU ICP-OES	5/25/11 4:01 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1316-T03-A	1	4.39E+04			4.39E+04	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:03 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1316-T04-A	1	4.98E+04			4.98E+04	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:04 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1316-T05-A	1	5.17E+04			5.17E+04	4.8E-01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 4:06 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1316-T01-B	1	1.77E+04			1.77E+04	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:08 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1316-T02-B	1	2.45E+04			2.45E+04	7.9E-01	1.0E+00	3.2E+00	10	100	2.55E+04	101%	VU ICP-OES	5/25/11 4:09 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1316-T03-B	1	3.64E+04			3.64E+04	8.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:11 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1316-T04-B	1	4.37E+04			4.37E+04	1.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:13 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1316-T05-B	1	4.75E+04			4.75E+04	1.0E+01	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 4:14 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1316-T01-C	1	1.96E+04			1.96E+04	9.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:16 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1316-T02-C	1	2.82E+04			2.82E+04	5.9E-01	1.0E+00	3.2E+00	10	100	2.92E+04	94%	VU ICP-OES	5/25/11 4:17 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1316-T03-C	1	4.18E+04			4.18E+04	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:19 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1316-T04-C	1	5.02E+04			5.02E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 4:21 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1316-T05-C	1	5.80E+04			5.80E+04	1.0E+00	1.0E+00	3.2E+00					VU ICP-OES	5/25/11 4:22 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1316-B01-A	1	1.39E+02			1.39E+02	2.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:54 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1316-B02-A	1	4.46E+00			4.46E+00	4.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:56 PM	EPA Interlab L04 1313-1316 CFS
Zn	CFS-L04-1316-B03-A	1	4.17E+00			4.17E+00	6.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/25/11 3:58 PM	EPA Interlab L04 1313-1316 CFS

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	CFS-L06-1316-T01-A	1	5.02E+01			5.02E+01	3.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1316-T02-A	1	5.65E+01			5.65E+01	1.6E+00	1.0E+00	3.2E+00	1000	120	1.21E+03	96%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1316-T03-A	1	5.91E+01			5.91E+01	2.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1316-T04-A	1	1.18E+02			1.18E+02	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1316-T05-A	1	7.96E+01			7.96E+01	3.5E+00	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1316-T01-B	1	4.83E+01			4.83E+01	5.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1316-T02-B	1	5.19E+01			5.19E+01	4.9E+00	1.0E+00	3.2E+00	1000	120	1.28E+03	102%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1316-T03-B	1	1.18E+02			1.18E+02	3.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1316-T04-B	1	7.19E+01			7.19E+01	6.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1316-T05-B	1	6.74E+01			6.74E+01	6.4E+00	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1316-T01-C	1	4.95E+01			4.95E+01	4.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1316-T02-C	1	5.15E+01			5.15E+01	5.1E+00	1.0E+00	3.2E+00	1000	120	1.27E+03	101%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1316-T03-C	1	5.74E+01			5.74E+01	4.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1316-T04-C	1	5.85E+01			5.85E+01	4.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1316-T05-C	1	6.02E+01			6.02E+01	1.0E+01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	9.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	1.6E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
Al	CFS-L06-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	1.0E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	CFS-L06-1316-T01-A	1	3.64E+01			3.64E+01	1.5E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1316-T02-A	1	3.16E+01			3.16E+01	3.9E+01	7.5E+00	2.4E+01	10	120	1.19E+03	96%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1316-T03-A	1	4.77E+01			4.77E+01	1.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1316-T04-A	1	6.67E+01			6.67E+01	1.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1316-T05-A	1	7.25E+01			7.25E+01	1.9E+01	7.5E+00	2.4E+01					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1316-T01-B	1	3.54E+01			3.54E+01	1.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1316-T02-B	1	4.27E+01			4.27E+01	1.2E+01	7.5E+00	2.4E+01	10	120	1.25E+03	101%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1316-T03-B	1	5.82E+01			5.82E+01	2.8E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1316-T04-B	1	6.46E+01			6.46E+01	1.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1316-T05-B	1	7.29E+01			7.29E+01	1.0E+01	7.5E+00	2.4E+01					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1316-T01-C	1	3.99E+01			3.99E+01	1.4E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1316-T02-C	1	4.94E+01			4.94E+01	9.6E+00	7.5E+00	2.4E+01	10	120	1.26E+03	101%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1316-T03-C	1	4.92E+01			4.92E+01	1.5E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1316-T04-C	1	5.62E+01			5.62E+01	1.8E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1316-T05-C	1	8.06E+01			8.06E+01	7.0E+00	7.5E+00	2.4E+01					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1316-B01-A	1	3.75E+00	U1/2		3.75E+00	1.2E+02	7.5E+00	2.4E+01				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1316-B02-A	1	8.33E+00	E		8.33E+00	5.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
Sb	CFS-L06-1316-B03-A	1	7.56E+00	E		7.56E+00	8.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	CFS-L06-1316-T01-A	1	2.47E+01	E		2.47E+01	1.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1316-T02-A	1	2.34E+01	E		2.34E+01	2.2E+01	1.1E+01	3.5E+01	10	120	1.21E+03	99%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1316-T03-A	1	4.42E+01			4.42E+01	9.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1316-T04-A	1	1.07E+02			1.07E+02	7.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1316-T05-A	1	6.36E+01			6.36E+01	1.4E+01	1.1E+01	3.5E+01					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1316-T01-B	1	1.45E+01	E		1.45E+01	7.7E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1316-T02-B	1	3.66E+01			3.66E+01	1.7E+01	1.1E+01	3.5E+01	10	120	1.25E+03	102%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1316-T03-B	1	1.08E+02			1.08E+02	8.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1316-T04-B	1	4.65E+01			4.65E+01	6.9E+00	1.1E+01	3.5E+01				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1316-T05-B	1	5.59E+01			5.59E+01	1.7E+01	1.1E+01	3.5E+01					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1316-T01-C	1	2.54E+01	E		2.54E+01	4.7E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1316-T02-C	1	2.04E+01	E		2.04E+01	2.7E+01	1.1E+01	3.5E+01	10	120	1.27E+03	104%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1316-T03-C	1	4.23E+01			4.23E+01	2.2E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1316-T04-C	1	3.60E+01			3.60E+01	3.8E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1316-T05-C	1	6.16E+01			6.16E+01	5.4E+00	1.1E+01	3.5E+01					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1316-B01-A	1	5.50E+00	U1/2		5.50E+00	5.0E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1316-B02-A	1	5.50E+00	U1/2		5.50E+00	1.5E+02	1.1E+01	3.5E+01				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
As	CFS-L06-1316-B03-A	1	5.50E+00	U1/2		5.50E+00	1.3E+02	1.1E+01	3.5E+01				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	CFS-L06-1316-T01-A	1	1.77E+02			1.77E+02	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1316-T02-A	1	3.07E+02			3.07E+02	1.2E+00	1.0E+00	3.2E+00	1000	120	1.43E+03	94%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1316-T03-A	1	6.27E+02			6.27E+02	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1316-T04-A	1	1.03E+03			1.03E+03	4.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1316-T05-A	1	1.56E+03			1.56E+03	2.4E-01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1316-T01-B	1	1.94E+02			1.94E+02	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1316-T02-B	1	3.20E+02			3.20E+02	8.3E-01	1.0E+00	3.2E+00	1000	120	1.48E+03	96%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1316-T03-B	1	6.28E+02			6.28E+02	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1316-T04-B	1	1.01E+03			1.01E+03	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1316-T05-B	1	1.57E+03			1.57E+03	5.7E-01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1316-T01-C	1	1.95E+02			1.95E+02	9.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1316-T02-C	1	3.22E+02			3.22E+02	6.2E-01	1.0E+00	3.2E+00	1000	120	1.49E+03	98%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1316-T03-C	1	6.33E+02			6.33E+02	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1316-T04-C	1	1.04E+03			1.04E+03	8.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1316-T05-C	1	1.50E+03			1.50E+03	4.6E-01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1316-B01-A	1	8.49E+00			8.49E+00	2.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1316-B02-A	1	9.12E+00			9.12E+00	7.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
B	CFS-L06-1316-B03-A	1	6.91E+00			6.91E+00	1.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	CFS-L06-1316-T01-A	1	1.35E+02			1.35E+02	6.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1316-T02-A	1	1.24E+02			1.24E+02	1.4E+00	1.0E+00	3.2E+00	10	120	1.37E+03	104%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1316-T03-A	1	1.05E+02			1.05E+02	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1316-T04-A	1	9.04E+01			9.04E+01	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1316-T05-A	1	7.28E+01			7.28E+01	4.3E-01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1316-T01-B	1	1.34E+02			1.34E+02	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1316-T02-B	1	1.25E+02			1.25E+02	2.9E-01	1.0E+00	3.2E+00	10	120	1.43E+03	109%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1316-T03-B	1	1.08E+02			1.08E+02	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1316-T04-B	1	8.67E+01			8.67E+01	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1316-T05-B	1	7.85E+01			7.85E+01	5.3E-01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1316-T01-C	1	1.37E+02			1.37E+02	4.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1316-T02-C	1	1.24E+02			1.24E+02	8.3E-01	1.0E+00	3.2E+00	10	120	1.42E+03	108%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1316-T03-C	1	1.02E+02			1.02E+02	8.4E-02	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1316-T04-C	1	8.60E+01			8.60E+01	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1316-T05-C	1	7.14E+01			7.14E+01	9.9E-01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	3.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	6.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
Ba	CFS-L06-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	1.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	CFS-L06-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	2.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00	10	120	1.18E+03	98%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	2.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	9.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1316-T05-A	1	9.50E-01	U1/2		9.50E-01	2.7E+01	1.9E+00	6.0E+00					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	8.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	1.7E+02	1.9E+00	6.0E+00	10	120	1.23E+03	103%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	7.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	8.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1316-T05-B	1	9.50E-01	U1/2		9.50E-01	1.3E+01	1.9E+00	6.0E+00					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	5.6E+01	1.9E+00	6.0E+00	10	120	1.23E+03	103%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	6.9E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	5.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1316-T05-C	1	9.50E-01	U1/2		9.50E-01	7.5E+00	1.9E+00	6.0E+00					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	9.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1316-B02-A	1	9.50E-01	U1/2		9.50E-01	3.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
Be	CFS-L06-1316-B03-A	1	9.50E-01	U1/2		9.50E-01	9.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	CFS-L06-1316-T01-A	1	5.00E+03			5.00E+03	7.5E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1316-T02-A	1	6.59E+03			6.59E+03	8.3E-01	2.2E+00	7.0E+00	10	120	7.64E+03	88%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1316-T03-A	1	9.28E+03			9.28E+03	6.7E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1316-T04-A	1	1.19E+04			1.19E+04	1.0E+00	2.2E+00	7.0E+00				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1316-T05-A	1	1.54E+04			1.54E+04	4.8E-01	2.2E+00	7.0E+00					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1316-T01-B	1	4.87E+03			4.87E+03	4.5E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1316-T02-B	1	7.08E+03			7.08E+03	9.3E-02	2.2E+00	7.0E+00	10	120	8.13E+03	87%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1316-T03-B	1	9.45E+03			9.45E+03	2.3E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1316-T04-B	1	1.28E+04			1.28E+04	3.7E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1316-T05-B	1	1.53E+04			1.53E+04	9.6E-01	2.2E+00	7.0E+00					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1316-T01-C	1	5.25E+03			5.25E+03	4.4E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1316-T02-C	1	7.08E+03			7.08E+03	3.9E-01	2.2E+00	7.0E+00	10	120	8.16E+03	90%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1316-T03-C	1	1.02E+04			1.02E+04	2.1E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1316-T04-C	1	1.31E+04			1.31E+04	5.1E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1316-T05-C	1	1.44E+04			1.44E+04	4.1E-01	2.2E+00	7.0E+00					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1316-B01-A	1	1.10E+00	U1/2		1.10E+00	1.1E+02	2.2E+00	7.0E+00				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1316-B02-A	1	1.10E+00	U1/2		1.10E+00	4.6E+01	2.2E+00	7.0E+00				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
Cd	CFS-L06-1316-B03-A	1	1.10E+00	U1/2		1.10E+00	1.4E+02	2.2E+00	7.0E+00				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	CFS-L06-1316-T01-A	1	7.51E+05			7.51E+05	5.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1316-T02-A	1	7.14E+05			7.14E+05	7.3E-01	2.6E+00	8.3E+00	1000	120	7.15E+05	85%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1316-T03-A	1	6.70E+05			6.70E+05	4.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1316-T04-A	1	6.46E+05			6.46E+05	9.3E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1316-T05-A	1	6.09E+05			6.09E+05	5.5E-01	2.6E+00	8.3E+00					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1316-T01-B	1	7.55E+05			7.55E+05	3.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1316-T02-B	1	7.47E+05			7.47E+05	1.1E-01	2.6E+00	8.3E+00	1000	120	7.48E+05	89%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1316-T03-B	1	6.87E+05			6.87E+05	8.2E-02	2.6E+00	8.3E+00				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1316-T04-B	1	6.48E+05			6.48E+05	5.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1316-T05-B	1	6.38E+05			6.38E+05	5.5E-01	2.6E+00	8.3E+00					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1316-T01-C	1	7.64E+05			7.64E+05	4.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1316-T02-C	1	7.19E+05			7.19E+05	2.0E-01	2.6E+00	8.3E+00	1000	120	7.20E+05	85%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1316-T03-C	1	6.64E+05			6.64E+05	3.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1316-T04-C	1	6.30E+05			6.30E+05	6.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1316-T05-C	1	5.93E+05			5.93E+05	5.8E-01	2.6E+00	8.3E+00					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1316-B01-A	1	1.75E+01			1.75E+01	6.4E+01	2.6E+00	8.3E+00				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1316-B02-A	1	2.36E+01			2.36E+01	5.6E+01	2.6E+00	8.3E+00				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
Ca	CFS-L06-1316-B03-A	1	2.45E+01			2.45E+01	9.7E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	CFS-L06-1316-T01-A	1	6.00E-01	U1/2		6.00E-01	7.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1316-T02-A	1	6.00E-01	U1/2		6.00E-01	9.3E+01	1.2E+00	3.8E+00	10	120	1.12E+03	94%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1316-T03-A	1	6.00E-01	U1/2		6.00E-01	4.1E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1316-T04-A	1	6.00E-01	U1/2		6.00E-01	2.2E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1316-T05-A	1	6.00E-01	U1/2		6.00E-01	4.7E+02	1.2E+00	3.8E+00					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1316-T01-B	1	6.00E-01	U1/2		6.00E-01	3.3E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1316-T02-B	1	6.00E-01	U1/2		6.00E-01	7.4E+01	1.2E+00	3.8E+00	10	120	1.18E+03	98%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1316-T03-B	1	6.00E-01	U1/2		6.00E-01	2.8E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1316-T04-B	1	6.00E-01	U1/2		6.00E-01	3.8E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1316-T05-B	1	6.00E-01	U1/2		6.00E-01	7.0E+01	1.2E+00	3.8E+00					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1316-T01-C	1	6.00E-01	U1/2		6.00E-01	4.9E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1316-T02-C	1	6.00E-01	U1/2		6.00E-01	1.8E+02	1.2E+00	3.8E+00	10	120	1.17E+03	98%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1316-T03-C	1	6.00E-01	U1/2		6.00E-01	4.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1316-T04-C	1	6.00E-01	U1/2		6.00E-01	1.6E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1316-T05-C	1	6.00E-01	U1/2		6.00E-01	4.0E+01	1.2E+00	3.8E+00					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	1.3E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	4.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
Cr	CFS-L06-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	1.8E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	CFS-L06-1316-T01-A	1	1.06E+02			1.06E+02	9.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1316-T02-A	1	1.67E+02			1.67E+02	1.5E+00	1.8E+00	5.7E+00	10	120	1.25E+03	90%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1316-T03-A	1	2.91E+02			2.91E+02	5.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1316-T04-A	1	4.18E+02			4.18E+02	6.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1316-T05-A	1	6.92E+02			6.92E+02	4.8E-01	1.8E+00	5.7E+00					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1316-T01-B	1	1.01E+02			1.01E+02	8.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1316-T02-B	1	1.74E+02			1.74E+02	9.4E-01	1.8E+00	5.7E+00	10	120	1.31E+03	95%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1316-T03-B	1	2.88E+02			2.88E+02	1.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1316-T04-B	1	4.52E+02			4.52E+02	5.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1316-T05-B	1	6.57E+02			6.57E+02	4.7E-01	1.8E+00	5.7E+00					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1316-T01-C	1	1.13E+02			1.13E+02	6.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1316-T02-C	1	1.80E+02			1.80E+02	7.7E-01	1.8E+00	5.7E+00	10	120	1.32E+03	95%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1316-T03-C	1	3.28E+02			3.28E+02	4.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1316-T04-C	1	4.90E+02			4.90E+02	7.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1316-T05-C	1	5.98E+02			5.98E+02	8.1E-01	1.8E+00	5.7E+00					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	6.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1316-B02-A	1	9.00E-01	U1/2		9.00E-01	7.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
Co	CFS-L06-1316-B03-A	1	9.00E-01	U1/2		9.00E-01	1.6E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	CFS-L06-1316-T01-A	1	8.53E+02			8.53E+02	7.5E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1316-T02-A	1	1.04E+03			1.04E+03	2.0E+00	3.7E+00	1.2E+01	10	120	2.08E+03	87%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1316-T03-A	1	1.44E+03			1.44E+03	1.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1316-T04-A	1	2.22E+03			2.22E+03	8.0E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1316-T05-A	1	3.06E+03			3.06E+03	1.0E+00	3.7E+00	1.2E+01					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1316-T01-B	1	8.34E+02			8.34E+02	7.8E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1316-T02-B	1	1.11E+03			1.11E+03	8.1E-01	3.7E+00	1.2E+01	10	120	2.16E+03	88%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1316-T03-B	1	1.74E+03			1.74E+03	1.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1316-T04-B	1	2.48E+03			2.48E+03	1.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1316-T05-B	1	3.04E+03			3.04E+03	1.4E+00	3.7E+00	1.2E+01					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1316-T01-C	1	9.51E+02			9.51E+02	1.7E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1316-T02-C	1	1.16E+03			1.16E+03	1.4E+00	3.7E+00	1.2E+01	10	120	2.25E+03	90%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1316-T03-C	1	1.97E+03			1.97E+03	8.7E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1316-T04-C	1	2.84E+03			2.84E+03	9.1E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1316-T05-C	1	3.09E+03			3.09E+03	6.3E-01	3.7E+00	1.2E+01					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	9.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1316-B02-A	1	1.85E+00	U1/2		1.85E+00	1.1E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
Cu	CFS-L06-1316-B03-A	1	1.85E+00	U1/2		1.85E+00	6.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	CFS-L06-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	3.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1316-T02-A	1	5.73E+01			5.73E+01	1.9E+00	2.0E+00	6.4E+00	1000	120	1.16E+03	92%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1316-T03-A	1	3.12E+00	E		3.12E+00	2.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1316-T04-A	1	2.43E+02			2.43E+02	4.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1316-T05-A	1	1.32E+01			1.32E+01	3.8E+00	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1316-T01-B	1	9.53E+00			9.53E+00	7.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1316-T02-B	1	2.30E+00	E		2.30E+00	1.1E+01	2.0E+00	6.4E+00	1000	120	1.22E+03	102%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1316-T03-B	1	2.89E+02			2.89E+02	9.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1316-T04-B	1	1.71E+01			1.71E+01	4.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1316-T05-B	1	1.19E+01			1.19E+01	3.7E+00	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1316-T01-C	1	4.38E+00	E		4.38E+00	5.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1316-T02-C	1	1.30E+01			1.30E+01	1.0E+00	2.0E+00	6.4E+00	1000	120	1.23E+03	101%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1316-T03-C	1	1.49E+01			1.49E+01	1.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1316-T04-C	1	6.51E+00			6.51E+00	3.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1316-T05-C	1	4.93E+00	E		4.93E+00	9.2E+00	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1316-B01-A	1	2.01E+00	E		2.01E+00	1.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1316-B02-A	1	2.17E+00	E		2.17E+00	2.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
Fe	CFS-L06-1316-B03-A	1	2.85E+00	E		2.85E+00	6.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	CFS-L06-1316-T01-A	1	1.19E+03			1.19E+03	1.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1316-T02-A	1	1.20E+03			1.20E+03	5.2E-01	6.8E+00	2.2E+01	10	120	2.20E+03	83%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1316-T03-A	1	1.25E+03			1.25E+03	4.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1316-T04-A	1	1.67E+03			1.67E+03	7.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1316-T05-A	1	1.41E+03			1.41E+03	5.3E-01	6.8E+00	2.2E+01					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1316-T01-B	1	1.15E+03			1.15E+03	6.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1316-T02-B	1	1.26E+03			1.26E+03	4.2E-01	6.8E+00	2.2E+01	10	120	2.27E+03	84%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1316-T03-B	1	1.59E+03			1.59E+03	8.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1316-T04-B	1	1.44E+03			1.44E+03	1.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1316-T05-B	1	1.50E+03			1.50E+03	8.8E-01	6.8E+00	2.2E+01					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1316-T01-C	1	1.20E+03			1.20E+03	1.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1316-T02-C	1	1.27E+03			1.27E+03	4.6E-01	6.8E+00	2.2E+01	10	120	2.32E+03	87%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1316-T03-C	1	1.22E+03			1.22E+03	6.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1316-T04-C	1	1.43E+03			1.43E+03	9.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1316-T05-C	1	1.50E+03			1.50E+03	5.7E-01	6.8E+00	2.2E+01					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	4.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1316-B02-A	1	3.40E+00	U1/2		3.40E+00	2.6E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
Pb	CFS-L06-1316-B03-A	1	3.40E+00	U1/2		3.40E+00	3.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	CFS-L06-1316-T01-A	1	4.15E+01			4.15E+01	1.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1316-T02-A	1	3.87E+01			3.87E+01	1.0E+01	1.9E+00	6.0E+00	10	120	1.03E+03	83%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1316-T03-A	1	3.38E+01			3.38E+01	1.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1316-T04-A	1	3.59E+01			3.59E+01	3.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1316-T05-A	1	5.64E+01			5.64E+01	4.1E+00	1.9E+00	6.0E+00					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1316-T01-B	1	4.14E+01			4.14E+01	4.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1316-T02-B	1	4.28E+01			4.28E+01	5.2E+00	1.9E+00	6.0E+00	10	120	1.08E+03	86%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1316-T03-B	1	3.47E+01			3.47E+01	1.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1316-T04-B	1	3.37E+01			3.37E+01	5.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1316-T05-B	1	5.42E+01			5.42E+01	1.1E+01	1.9E+00	6.0E+00					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1316-T01-C	1	4.04E+01			4.04E+01	4.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1316-T02-C	1	3.78E+01			3.78E+01	7.3E+00	1.9E+00	6.0E+00	10	120	1.07E+03	86%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1316-T03-C	1	3.32E+01			3.32E+01	1.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1316-T04-C	1	3.72E+01			3.72E+01	9.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1316-T05-C	1	5.48E+01			5.48E+01	6.9E+00	1.9E+00	6.0E+00					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1316-B01-A	1	2.77E+01			2.77E+01	4.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1316-B02-A	1	2.68E+01			2.68E+01	7.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
Li	CFS-L06-1316-B03-A	1	2.79E+01			2.79E+01	4.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	CFS-L06-1316-T01-A	1	1.68E+03			1.68E+03	6.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1316-T02-A	1	2.86E+03			2.86E+03	1.6E+00	2.0E+00	6.4E+00	10	120	3.95E+03	91%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1316-T03-A	1	5.85E+03			5.85E+03	4.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1316-T04-A	1	9.24E+03			9.24E+03	6.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1316-T05-A	1	1.76E+04			1.76E+04	6.1E-01	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1316-T01-B	1	1.62E+03			1.62E+03	7.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1316-T02-B	1	3.01E+03			3.01E+03	1.2E+00	2.0E+00	6.4E+00	10	120	4.07E+03	88%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1316-T03-B	1	5.65E+03			5.65E+03	1.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1316-T04-B	1	9.75E+03			9.75E+03	7.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1316-T05-B	1	1.69E+04			1.69E+04	1.1E+00	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1316-T01-C	1	1.84E+03			1.84E+03	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1316-T02-C	1	3.18E+03			3.18E+03	1.2E+00	2.0E+00	6.4E+00	10	120	4.22E+03	86%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1316-T03-C	1	6.47E+03			6.47E+03	5.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1316-T04-C	1	1.05E+04			1.05E+04	1.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1316-T05-C	1	1.56E+04			1.56E+04	2.2E-01	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1316-B02-A	1	1.00E+00	U1/2		1.00E+00	8.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
Mn	CFS-L06-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	6.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	CFS-L06-1316-T01-A	1	7.07E+04			7.07E+04	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1316-T02-A	1	1.33E+05			1.33E+05	6.6E-01	1.0E+00	3.2E+00	1000	120	1.34E+05	95%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1316-T03-A	1	3.08E+05			3.08E+05	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1316-T04-A	1	5.50E+05			5.50E+05	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1316-T05-A	1	9.71E+05			9.71E+05	3.7E-01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1316-T01-B	1	7.09E+04			7.09E+04	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1316-T02-B	1	1.36E+05			1.36E+05	5.3E-01	1.0E+00	3.2E+00	1000	120	1.37E+05	93%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1316-T03-B	1	3.03E+05			3.03E+05	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1316-T04-B	1	5.24E+05			5.24E+05	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1316-T05-B	1	9.99E+05			9.99E+05	6.1E-01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1316-T01-C	1	7.36E+04			7.36E+04	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1316-T02-C	1	1.40E+05			1.40E+05	8.1E-01	1.0E+00	3.2E+00	1000	120	1.41E+05	88%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1316-T03-C	1	2.97E+05			2.97E+05	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1316-T04-C	1	5.43E+05			5.43E+05	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1316-T05-C	1	9.46E+05			9.46E+05	2.4E-01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1316-B02-A	1	6.40E+00			6.40E+00	1.1E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
Mg	CFS-L06-1316-B03-A	1	2.38E+01			2.38E+01	3.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	CFS-L06-1316-T01-A	1	1.04E+01			1.04E+01	6.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1316-T02-A	1	9.84E+00			9.84E+00	1.3E+01	1.2E+00	3.8E+00	10	120	1.12E+03	92%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1316-T03-A	1	1.64E+01			1.64E+01	2.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1316-T04-A	1	2.18E+01			2.18E+01	1.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1316-T05-A	1	2.44E+01			2.44E+01	4.1E+00	1.2E+00	3.8E+00					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1316-T01-B	1	9.20E+00			9.20E+00	1.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1316-T02-B	1	1.08E+01			1.08E+01	1.2E+01	1.2E+00	3.8E+00	10	120	1.18E+03	98%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1316-T03-B	1	1.61E+01			1.61E+01	8.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1316-T04-B	1	1.81E+01			1.81E+01	2.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1316-T05-B	1	2.50E+01			2.50E+01	9.4E+00	1.2E+00	3.8E+00					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1316-T01-C	1	9.39E+00			9.39E+00	7.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1316-T02-C	1	1.17E+01			1.17E+01	1.7E+01	1.2E+00	3.8E+00	10	120	1.18E+03	97%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1316-T03-C	1	1.64E+01			1.64E+01	2.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1316-T04-C	1	1.54E+01			1.54E+01	5.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1316-T05-C	1	2.48E+01			2.48E+01	7.8E+00	1.2E+00	3.8E+00					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1316-B01-A	1	1.71E+00	E		1.71E+00	7.8E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1316-B02-A	1	2.00E+00	E		2.00E+00	6.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
Mo	CFS-L06-1316-B03-A	1	6.00E-01	U1/2		6.00E-01	2.7E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	CFS-L06-1316-T01-A	1	2.30E+02			2.30E+02	7.3E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1316-T02-A	1	3.44E+02			3.44E+02	1.4E+00	1.8E+00	5.7E+00	10	120	1.46E+03	93%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1316-T03-A	1	5.55E+02			5.55E+02	7.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1316-T04-A	1	7.59E+02			7.59E+02	7.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1316-T05-A	1	1.14E+03			1.14E+03	3.9E-01	1.8E+00	5.7E+00					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1316-T01-B	1	2.26E+02			2.26E+02	1.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1316-T02-B	1	3.65E+02			3.65E+02	7.1E-01	1.8E+00	5.7E+00	10	120	1.52E+03	97%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1316-T03-B	1	5.60E+02			5.60E+02	1.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1316-T04-B	1	8.29E+02			8.29E+02	7.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1316-T05-B	1	1.09E+03			1.09E+03	3.4E-01	1.8E+00	5.7E+00					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1316-T01-C	1	2.51E+02			2.51E+02	1.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1316-T02-C	1	3.84E+02			3.84E+02	1.3E+00	1.8E+00	5.7E+00	10	120	1.55E+03	97%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1316-T03-C	1	6.35E+02			6.35E+02	1.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1316-T04-C	1	8.98E+02			8.98E+02	8.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1316-T05-C	1	9.90E+02			9.90E+02	1.1E+00	1.8E+00	5.7E+00					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	1.6E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1316-B02-A	1	9.00E-01	U1/2		9.00E-01	2.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
Ni	CFS-L06-1316-B03-A	1	9.00E-01	U1/2		9.00E-01	2.7E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	CFS-L06-1316-T01-A	1	1.85E+00	U1/2		1.85E+00	8.5E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1316-T02-A	1	1.85E+00	U1/2		1.85E+00	7.4E+02	3.7E+00	1.2E+01	1000	120	1.26E+03	105%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1316-T03-A	1	1.22E+01			1.22E+01	5.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1316-T04-A	1	5.82E+00	E		5.82E+00	1.1E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1316-T05-A	1	2.93E+01			2.93E+01	4.8E+01	3.7E+00	1.2E+01					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1316-T01-B	1	1.85E+00	U1/2		1.85E+00	7.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1316-T02-B	1	1.85E+00	U1/2		1.85E+00	6.1E+01	3.7E+00	1.2E+01	1000	120	1.36E+03	113%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1316-T03-B	1	2.44E+01			2.44E+01	4.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1316-T04-B	1	1.77E+01			1.77E+01	2.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1316-T05-B	1	3.53E+01			3.53E+01	6.3E+01	3.7E+00	1.2E+01					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1316-T01-C	1	1.85E+00	U1/2		1.85E+00	1.3E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1316-T02-C	1	1.85E+00	U1/2		1.85E+00	6.6E+01	3.7E+00	1.2E+01	1000	120	1.34E+03	112%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1316-T03-C	1	2.34E+01			2.34E+01	3.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1316-T04-C	1	2.19E+01			2.19E+01	4.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1316-T05-C	1	2.24E+01			2.24E+01	6.6E+01	3.7E+00	1.2E+01					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	1.8E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1316-B02-A	1	1.85E+00	U1/2		1.85E+00	4.5E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
P	CFS-L06-1316-B03-A	1	1.85E+00	U1/2		1.85E+00	1.7E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	CFS-L06-1316-T01-A	1	1.08E+04			1.08E+04	7.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1316-T02-A	1	1.80E+04			1.80E+04	1.3E+00	1.6E+00	5.1E+00	1000	120	1.92E+04	95%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1316-T03-A	1	3.53E+04			3.53E+04	9.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1316-T04-A	1	5.69E+04			5.69E+04	6.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1316-T05-A	1	9.26E+04			9.26E+04	2.7E-01	1.6E+00	5.1E+00					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1316-T01-B	1	1.08E+04			1.08E+04	2.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1316-T02-B	1	1.87E+04			1.87E+04	1.1E-01	1.6E+00	5.1E+00	1000	120	1.98E+04	93%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1316-T03-B	1	3.53E+04			3.53E+04	1.4E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1316-T04-B	1	5.52E+04			5.52E+04	4.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1316-T05-B	1	9.39E+04			9.39E+04	4.3E-01	1.6E+00	5.1E+00					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1316-T01-C	1	1.08E+04			1.08E+04	8.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1316-T02-C	1	1.83E+04			1.83E+04	3.2E-01	1.6E+00	5.1E+00	1000	120	1.95E+04	97%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1316-T03-C	1	3.48E+04			3.48E+04	6.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1316-T04-C	1	5.52E+04			5.52E+04	1.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1316-T05-C	1	9.16E+04			9.16E+04	5.4E-01	1.6E+00	5.1E+00					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1316-B01-A	1	3.75E+01			3.75E+01	9.6E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1316-B02-A	1	3.58E+01			3.58E+01	3.9E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
K	CFS-L06-1316-B03-A	1	4.11E+01			4.11E+01	3.7E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	CFS-L06-1316-T01-A	1	9.70E+01			9.70E+01	1.2E+01	1.5E+01	4.8E+01				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1316-T02-A	1	1.51E+02			1.51E+02	9.1E+00	1.5E+01	4.8E+01	10	120	1.24E+03	91%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1316-T03-A	1	3.15E+02			3.15E+02	5.6E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1316-T04-A	1	5.50E+02			5.50E+02	9.3E-01	1.5E+01	4.8E+01				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1316-T05-A	1	9.36E+02			9.36E+02	2.2E+00	1.5E+01	4.8E+01					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1316-T01-B	1	1.15E+02			1.15E+02	2.5E+01	1.5E+01	4.8E+01				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1316-T02-B	1	1.44E+02			1.44E+02	1.8E+01	1.5E+01	4.8E+01	10	120	1.32E+03	98%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1316-T03-B	1	2.97E+02			2.97E+02	8.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1316-T04-B	1	5.19E+02			5.19E+02	1.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1316-T05-B	1	9.77E+02			9.77E+02	1.2E+00	1.5E+01	4.8E+01					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1316-T01-C	1	1.04E+02			1.04E+02	9.0E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1316-T02-C	1	1.59E+02			1.59E+02	5.9E+00	1.5E+01	4.8E+01	10	120	1.32E+03	97%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1316-T03-C	1	3.07E+02			3.07E+02	1.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1316-T04-C	1	5.22E+02			5.22E+02	1.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1316-T05-C	1	9.36E+02			9.36E+02	2.7E-01	1.5E+01	4.8E+01					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1316-B01-A	1	7.50E+00	U1/2		7.50E+00	6.7E+01	1.5E+01	4.8E+01				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1316-B02-A	1	1.89E+01	E		1.89E+01	6.4E+01	1.5E+01	4.8E+01				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
Se	CFS-L06-1316-B03-A	1	7.50E+00	U1/2		7.50E+00	2.7E+02	1.5E+01	4.8E+01				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	CFS-L06-1316-T01-A	1	4.42E+03			4.42E+03	5.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1316-T02-A	1	5.17E+03			5.17E+03	2.1E+00	1.1E+00	3.5E+00	1000	120	6.21E+03	87%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1316-T03-A	1	6.37E+03			6.37E+03	9.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1316-T04-A	1	7.19E+03			7.19E+03	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1316-T05-A	1	7.82E+03			7.82E+03	2.3E-01	1.1E+00	3.5E+00					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1316-T01-B	1	4.32E+03			4.32E+03	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1316-T02-B	1	5.39E+03			5.39E+03	8.2E-01	1.1E+00	3.5E+00	1000	120	6.41E+03	85%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1316-T03-B	1	6.65E+03			6.65E+03	5.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1316-T04-B	1	7.35E+03			7.35E+03	6.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1316-T05-B	1	7.82E+03			7.82E+03	5.7E-01	1.1E+00	3.5E+00					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1316-T01-C	1	4.29E+03			4.29E+03	2.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1316-T02-C	1	5.33E+03			5.33E+03	1.1E+00	1.1E+00	3.5E+00	1000	120	6.44E+03	93%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1316-T03-C	1	7.28E+03			7.28E+03	7.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1316-T04-C	1	7.65E+03			7.65E+03	7.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1316-T05-C	1	7.25E+03			7.25E+03	5.8E-01	1.1E+00	3.5E+00					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1316-B01-A	1	1.29E+01			1.29E+01	2.1E+01	1.1E+00	3.5E+00				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1316-B02-A	1	1.10E+01			1.10E+01	5.4E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
Si	CFS-L06-1316-B03-A	1	1.28E+01			1.28E+01	9.5E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	CFS-L06-1316-T01-A	1	7.37E+03			7.37E+03	2.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1316-T02-A	1	1.42E+04			1.42E+04	2.0E-01	2.5E+00	8.0E+00	1000	120	1.54E+04	96%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1316-T03-A	1	3.39E+04			3.39E+04	6.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1316-T04-A	1	6.07E+04			6.07E+04	4.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1316-T05-A	1	9.34E+04			9.34E+04	6.9E-01	2.5E+00	8.0E+00					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1316-T01-B	1	7.37E+03			7.37E+03	6.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1316-T02-B	1	1.47E+04			1.47E+04	2.6E-01	2.5E+00	8.0E+00	1000	120	1.58E+04	94%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1316-T03-B	1	3.32E+04			3.32E+04	3.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1316-T04-B	1	6.07E+04			6.07E+04	1.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1316-T05-B	1	9.62E+04			9.62E+04	5.1E-01	2.5E+00	8.0E+00					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1316-T01-C	1	7.65E+03			7.65E+03	1.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1316-T02-C	1	1.48E+04			1.48E+04	3.9E-01	2.5E+00	8.0E+00	1000	120	1.59E+04	93%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1316-T03-C	1	3.31E+04			3.31E+04	9.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1316-T04-C	1	6.03E+04			6.03E+04	9.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1316-T05-C	1	9.33E+04			9.33E+04	4.1E-01	2.5E+00	8.0E+00					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1316-B01-A	1	6.07E+00	E		6.07E+00	2.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1316-B02-A	1	1.25E+00	U1/2		1.25E+00	3.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
Na	CFS-L06-1316-B03-A	1	5.15E+00	E		5.15E+00	4.5E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	CFS-L06-1316-T01-A	1	1.69E+03			1.69E+03	8.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1316-T02-A	1	2.27E+03			2.27E+03	2.0E+00	1.0E+00	3.2E+00	1000	120	3.35E+03	89%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1316-T03-A	1	3.46E+03			3.46E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1316-T04-A	1	4.41E+03			4.41E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1316-T05-A	1	5.42E+03			5.42E+03	7.4E-01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1316-T01-B	1	1.64E+03			1.64E+03	8.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1316-T02-B	1	2.35E+03			2.35E+03	1.0E+00	1.0E+00	3.2E+00	1000	120	3.49E+03	94%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1316-T03-B	1	3.48E+03			3.48E+03	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1316-T04-B	1	4.12E+03			4.12E+03	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1316-T05-B	1	5.72E+03			5.72E+03	2.1E+00	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1316-T01-C	1	1.58E+03			1.58E+03	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1316-T02-C	1	2.17E+03			2.17E+03	7.1E-01	1.0E+00	3.2E+00	1000	120	3.30E+03	94%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1316-T03-C	1	3.10E+03			3.10E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1316-T04-C	1	3.91E+03			3.91E+03	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1316-T05-C	1	5.49E+03			5.49E+03	3.0E-01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	5.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	8.0E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
Sr	CFS-L06-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	8.5E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	CFS-L06-1316-T01-A	1	6.42E+05			6.42E+05	9.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1316-T02-A	1	7.04E+05			7.04E+05	1.0E+00	6.8E+00	2.2E+01	1000	120	7.05E+05	83%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1316-T03-A	1	8.88E+05			8.88E+05	3.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1316-T04-A	1	1.17E+06			1.17E+06	5.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1316-T05-A	1	1.61E+06			1.61E+06	1.3E-01	6.8E+00	2.2E+01					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1316-T01-B	1	6.43E+05			6.43E+05	4.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1316-T02-B	1	7.28E+05			7.28E+05	4.1E-01	6.8E+00	2.2E+01	1000	120	7.29E+05	87%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1316-T03-B	1	9.00E+05			9.00E+05	5.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1316-T04-B	1	1.15E+06			1.15E+06	4.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1316-T05-B	1	1.65E+06			1.65E+06	5.0E-01	6.8E+00	2.2E+01					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1316-T01-C	1	6.56E+05			6.56E+05	5.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1316-T02-C	1	7.14E+05			7.14E+05	1.2E-01	6.8E+00	2.2E+01	1000	120	7.15E+05	87%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1316-T03-C	1	8.90E+05			8.90E+05	8.6E-02	6.8E+00	2.2E+01				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1316-T04-C	1	1.16E+06			1.16E+06	8.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1316-T05-C	1	1.56E+06			1.56E+06	6.2E-01	6.8E+00	2.2E+01					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1316-B01-A	1	9.31E+01			9.31E+01	3.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1316-B02-A	1	7.37E+01			7.37E+01	8.8E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
S	CFS-L06-1316-B03-A	1	6.47E+01			6.47E+01	4.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	CFS-L06-1316-T01-A	1	3.69E+02			3.69E+02	1.9E+00	4.6E+00	1.5E+01				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1316-T02-A	1	5.21E+02			5.21E+02	1.6E+00	4.6E+00	1.5E+01	10	120	1.56E+03	86%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1316-T03-A	1	8.41E+02			8.41E+02	1.1E+00	4.6E+00	1.5E+01				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1316-T04-A	1	1.17E+03			1.17E+03	1.4E+00	4.6E+00	1.5E+01				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1316-T05-A	1	1.61E+03			1.61E+03	6.0E-01	4.6E+00	1.5E+01					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1316-T01-B	1	3.57E+02			3.57E+02	4.1E-01	4.6E+00	1.5E+01				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1316-T02-B	1	5.38E+02			5.38E+02	1.6E+00	4.6E+00	1.5E+01	10	120	1.58E+03	87%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1316-T03-B	1	8.39E+02			8.39E+02	2.7E-01	4.6E+00	1.5E+01				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1316-T04-B	1	1.16E+03			1.16E+03	4.3E-01	4.6E+00	1.5E+01				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1316-T05-B	1	1.65E+03			1.65E+03	2.3E-01	4.6E+00	1.5E+01					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1316-T01-C	1	3.64E+02			3.64E+02	2.6E+00	4.6E+00	1.5E+01				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1316-T02-C	1	5.33E+02			5.33E+02	7.5E-01	4.6E+00	1.5E+01	10	120	1.61E+03	90%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1316-T03-C	1	8.37E+02			8.37E+02	1.3E+00	4.6E+00	1.5E+01				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1316-T04-C	1	1.18E+03			1.18E+03	5.0E-01	4.6E+00	1.5E+01				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1316-T05-C	1	1.58E+03			1.58E+03	5.5E-01	4.6E+00	1.5E+01					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1316-B01-A	1	2.30E+00	U1/2		2.30E+00	7.5E+00	4.6E+00	1.5E+01				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1316-B02-A	1	2.30E+00	U1/2		2.30E+00	1.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
Tl	CFS-L06-1316-B03-A	1	2.30E+00	U1/2		2.30E+00	1.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	CFS-L06-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	7.3E+01	2.0E+00	6.4E+00	10	120	1.12E+03	93%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1316-T05-A	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	9.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00	10	120	1.18E+03	98%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	8.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1316-T05-B	1	1.00E+00	U1/2		1.00E+00	4.8E+01	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	9.8E+00	2.0E+00	6.4E+00	10	120	1.18E+03	98%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	8.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	9.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1316-T05-C	1	1.00E+00	U1/2		1.00E+00	3.3E+01	2.0E+00	6.4E+00					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	6.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1316-B02-A	1	1.00E+00	U1/2		1.00E+00	6.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
Ti	CFS-L06-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	6.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	CFS-L06-1316-T01-A	1	2.84E+01			2.84E+01	2.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1316-T02-A	1	2.85E+01			2.85E+01	1.4E+00	1.5E+00	4.8E+00	10	120	1.14E+03	93%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1316-T03-A	1	2.55E+01			2.55E+01	5.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1316-T04-A	1	2.60E+01			2.60E+01	5.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1316-T05-A	1	2.56E+01			2.56E+01	6.9E+00	1.5E+00	4.8E+00					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1316-T01-B	1	3.04E+01			3.04E+01	2.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1316-T02-B	1	3.02E+01			3.02E+01	3.8E+00	1.5E+00	4.8E+00	10	120	1.20E+03	97%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1316-T03-B	1	2.71E+01			2.71E+01	6.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1316-T04-B	1	2.58E+01			2.58E+01	2.9E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1316-T05-B	1	2.56E+01			2.56E+01	7.1E-01	1.5E+00	4.8E+00					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1316-T01-C	1	3.15E+01			3.15E+01	2.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1316-T02-C	1	2.83E+01			2.83E+01	6.3E+00	1.5E+00	4.8E+00	10	120	1.20E+03	97%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1316-T03-C	1	2.53E+01			2.53E+01	1.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1316-T04-C	1	2.54E+01			2.54E+01	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1316-T05-C	1	2.18E+01			2.18E+01	3.3E+00	1.5E+00	4.8E+00					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1316-B01-A	1	7.50E-01	U1/2		7.50E-01	9.4E+01	1.5E+00	4.8E+00				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1316-B02-A	1	7.50E-01	U1/2		7.50E-01	5.6E+01	1.5E+00	4.8E+00				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
V	CFS-L06-1316-B03-A	1	7.50E-01	U1/2		7.50E-01	8.4E+01	1.5E+00	4.8E+00				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	CFS-L06-1316-T01-A	1	2.14E+04			2.14E+04	2.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:40 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1316-T02-A	1	2.75E+04			2.75E+04	1.2E+00	1.0E+00	3.2E+00	10	120	2.86E+04	90%	VU ICP-OES	4/14/11 4:41 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1316-T03-A	1	3.92E+04			3.92E+04	2.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:43 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1316-T04-A	1	5.04E+04			5.04E+04	7.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:45 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1316-T05-A	1	6.81E+04			6.81E+04	7.7E-02	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 4:46 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1316-T01-B	1	2.08E+04			2.08E+04	5.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:48 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1316-T02-B	1	3.03E+04			3.03E+04	7.8E-01	1.0E+00	3.2E+00	10	120	3.14E+04	89%	VU ICP-OES	4/14/11 4:50 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1316-T03-B	1	4.01E+04			4.01E+04	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:51 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1316-T04-B	1	5.63E+04			5.63E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:53 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1316-T05-B	1	6.58E+04			6.58E+04	7.0E-01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 4:55 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1316-T01-C	1	2.28E+04			2.28E+04	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:56 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1316-T02-C	1	3.04E+04			3.04E+04	9.3E-01	1.0E+00	3.2E+00	10	120	3.16E+04	96%	VU ICP-OES	4/14/11 4:58 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1316-T03-C	1	4.63E+04			4.63E+04	3.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 5:00 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1316-T04-C	1	5.95E+04			5.95E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 5:01 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1316-T05-C	1	5.96E+04			5.96E+04	6.6E-01	1.0E+00	3.2E+00					VU ICP-OES	4/14/11 5:03 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1316-B01-A	1	5.30E+00			5.30E+00	9.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:35 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1316-B02-A	1	5.00E+00			5.00E+00	7.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:37 PM	EPA Interlab L06 1313-1316 CFS
Zn	CFS-L06-1316-B03-A	1	3.98E+00			3.98E+00	8.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/14/11 4:38 PM	EPA Interlab L06 1313-1316 CFS

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	CFS-L07-1316-T01-A	1	3.90E+01			3.90E+01	3.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1316-T02-A	1	2.83E+01			2.83E+01	6.5E+01	1.0E+00	3.2E+00	1000	100	1.12E+03	110%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1316-T03-A	1	4.29E+01			4.29E+01	8.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1316-T04-A	1	4.10E+01			4.10E+01	7.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1316-T05-A	1	4.61E+01			4.61E+01	6.0E+00	7.5E+00	2.4E+01					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1316-T01-B	1	3.96E+01			3.96E+01	8.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1316-T02-B	1	3.73E+01			3.73E+01	2.2E+00	7.5E+00	2.4E+01	1000	100	1.12E+03	109%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1316-T03-B	1	4.16E+01			4.16E+01	4.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1316-T04-B	1	4.84E+01			4.84E+01	1.9E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1316-T05-B	1	5.00E-01	U1/2		5.00E-01	1.9E+02	7.5E+00	2.4E+01					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1316-T01-C	1	3.74E+01			3.74E+01	3.4E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1316-T02-C	1	4.09E+01			4.09E+01	2.0E+00	7.5E+00	2.4E+01	1000	100	1.12E+03	108%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1316-T03-C	1	3.82E+01			3.82E+01	7.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1316-T04-C	1	4.11E+01			4.11E+01	2.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1316-T05-C	1	3.90E+01			3.90E+01	9.0E+00	7.5E+00	2.4E+01					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.9E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	8.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
Al	CFS-L07-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	7.8E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	CFS-L07-1316-T01-A	1	4.38E+01			4.38E+01	3.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1316-T02-A	1	1.60E+01	E		1.60E+01	8.5E+01	7.5E+00	2.4E+01	10	100	9.99E+02	98%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1316-T03-A	1	4.78E+01			4.78E+01	2.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1316-T04-A	1	5.88E+01			5.88E+01	1.5E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1316-T05-A	1	6.63E+01			6.63E+01	1.3E+01	7.5E+00	2.4E+01					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1316-T01-B	1	3.12E+01			3.12E+01	9.2E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1316-T02-B	1	4.26E+01			4.26E+01	1.8E+01	7.5E+00	2.4E+01	10	100	1.01E+03	96%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1316-T03-B	1	4.56E+01			4.56E+01	2.6E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1316-T04-B	1	4.79E+01			4.79E+01	2.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1316-T05-B	1	3.75E+00	U1/2		3.75E+00	2.9E+01	7.5E+00	2.4E+01					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1316-T01-C	1	2.67E+01			2.67E+01	3.3E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1316-T02-C	1	3.82E+01			3.82E+01	1.3E+01	7.5E+00	2.4E+01	10	100	9.98E+02	96%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1316-T03-C	1	5.15E+01			5.15E+01	1.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1316-T04-C	1	5.18E+01			5.18E+01	4.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1316-T05-C	1	6.89E+01			6.89E+01	3.8E+00	7.5E+00	2.4E+01					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1316-B01-A	1	3.75E+00	U1/2		3.75E+00	1.3E+02	7.5E+00	2.4E+01				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1316-B02-A	1	3.75E+00	U1/2		3.75E+00	7.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
Sb	CFS-L07-1316-B03-A	1	3.75E+00	U1/2		3.75E+00	5.1E+02	7.5E+00	2.4E+01				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	CFS-L07-1316-T01-A	1	2.07E+01	E		2.07E+01	5.6E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1316-T02-A	1	5.50E+00	U1/2		5.50E+00	1.9E+02	1.1E+01	3.5E+01	10	100	9.85E+02	98%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1316-T03-A	1	3.70E+01			3.70E+01	2.2E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1316-T04-A	1	3.78E+01			3.78E+01	3.6E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1316-T05-A	1	5.15E+01			5.15E+01	1.4E+01	1.1E+01	3.5E+01					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1316-T01-B	1	1.59E+01	E		1.59E+01	2.2E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1316-T02-B	1	2.14E+01	E		2.14E+01	2.9E+01	1.1E+01	3.5E+01	10	100	9.98E+02	98%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1316-T03-B	1	3.10E+01	E		3.10E+01	2.8E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1316-T04-B	1	3.63E+01			3.63E+01	2.2E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1316-T05-B	1	5.50E+00	U1/2		5.50E+00	7.9E+01	1.1E+01	3.5E+01					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1316-T01-C	1	2.17E+01	E		2.17E+01	1.6E+00	1.1E+01	3.5E+01				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1316-T02-C	1	3.12E+01	E		3.12E+01	5.5E+01	1.1E+01	3.5E+01	10	100	9.93E+02	96%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1316-T03-C	1	3.18E+01	E		3.18E+01	3.1E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1316-T04-C	1	4.54E+01			4.54E+01	6.3E+00	1.1E+01	3.5E+01				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1316-T05-C	1	4.22E+01			4.22E+01	1.1E+01	1.1E+01	3.5E+01					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1316-B01-A	1	5.50E+00	U1/2		5.50E+00	2.5E+02	1.1E+01	3.5E+01				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1316-B02-A	1	5.50E+00	U1/2		5.50E+00	1.6E+02	1.1E+01	3.5E+01				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
As	CFS-L07-1316-B03-A	1	5.50E+00	U1/2		5.50E+00	1.3E+02	1.1E+01	3.5E+01				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	CFS-L07-1316-T01-A	1	1.70E+02			1.70E+02	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1316-T02-A	1	1.87E+02			1.87E+02	7.7E+01	1.0E+00	3.2E+00	1000	100	1.23E+03	104%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1316-T03-A	1	6.40E+02			6.40E+02	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1316-T04-A	1	1.03E+03			1.03E+03	1.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1316-T05-A	1	1.50E+03			1.50E+03	5.2E-01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1316-T01-B	1	1.77E+02			1.77E+02	1.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1316-T02-B	1	3.12E+02			3.12E+02	1.6E+00	1.0E+00	3.2E+00	1000	100	1.25E+03	93%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1316-T03-B	1	6.25E+02			6.25E+02	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1316-T04-B	1	1.02E+03			1.02E+03	3.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1316-T05-B	1	9.79E+01			9.79E+01	2.4E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1316-T01-C	1	1.70E+02			1.70E+02	2.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1316-T02-C	1	3.11E+02			3.11E+02	3.9E-01	1.0E+00	3.2E+00	1000	100	1.24E+03	93%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1316-T03-C	1	6.53E+02			6.53E+02	2.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1316-T04-C	1	1.08E+03			1.08E+03	4.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1316-T05-C	1	1.45E+03			1.45E+03	5.8E-01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1316-B01-A	1	3.32E+00			3.32E+00	1.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1316-B02-A	1	2.86E+00	E		2.86E+00	7.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
B	CFS-L07-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	1.9E+02	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	CFS-L07-1316-T01-A	1	2.07E+02			2.07E+02	2.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1316-T02-A	1	1.45E+02			1.45E+02	7.9E+01	1.0E+00	3.2E+00	10	100	1.22E+03	107%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1316-T03-A	1	3.59E+02			3.59E+02	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1316-T04-A	1	5.17E+02			5.17E+02	7.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1316-T05-A	1	7.70E+02			7.70E+02	8.8E-01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1316-T01-B	1	2.02E+02			2.02E+02	5.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1316-T02-B	1	2.44E+02			2.44E+02	8.6E-01	1.0E+00	3.2E+00	10	100	1.23E+03	99%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1316-T03-B	1	3.48E+02			3.48E+02	8.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1316-T04-B	1	5.25E+02			5.25E+02	6.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1316-T05-B	1	4.64E+01			4.64E+01	2.4E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1316-T01-C	1	2.00E+02			2.00E+02	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1316-T02-C	1	2.40E+02			2.40E+02	9.9E-01	1.0E+00	3.2E+00	10	100	1.21E+03	97%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1316-T03-C	1	3.50E+02			3.50E+02	9.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1316-T04-C	1	5.11E+02			5.11E+02	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1316-T05-C	1	7.61E+02			7.61E+02	5.3E-01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.6E+02	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	1.5E+02	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
Ba	CFS-L07-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	2.5E+02	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	CFS-L07-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	7.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	1.2E+03	1.9E+00	6.0E+00	10	100	1.01E+03	101%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	5.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1316-T05-A	1	9.50E-01	U1/2		9.50E-01	5.7E+01	1.9E+00	6.0E+00					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	2.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	2.4E+02	1.9E+00	6.0E+00	10	100	1.01E+03	101%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	1.0E+02	1.9E+00	6.0E+00				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	5.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1316-T05-B	1	9.50E-01	U1/2		9.50E-01	2.7E+01	1.9E+00	6.0E+00					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	4.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00	10	100	1.00E+03	100%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	3.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	5.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1316-T05-C	1	9.50E-01	U1/2		9.50E-01	3.0E+01	1.9E+00	6.0E+00					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	2.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1316-B02-A	1	9.50E-01	U1/2		9.50E-01	5.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
Be	CFS-L07-1316-B03-A	1	9.50E-01	U1/2		9.50E-01	3.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	CFS-L07-1316-T01-A	1	4.96E+03			4.96E+03	4.3E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1316-T02-A	1	4.33E+03			4.33E+03	7.5E+01	2.2E+00	7.0E+00	10	100	5.36E+03	103%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1316-T03-A	1	9.57E+03			9.57E+03	5.8E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1316-T04-A	1	1.07E+04			1.07E+04	4.7E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1316-T05-A	1	1.32E+04			1.32E+04	6.3E-01	2.2E+00	7.0E+00					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1316-T01-B	1	4.79E+03			4.79E+03	8.2E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1316-T02-B	1	6.37E+03			6.37E+03	6.7E-01	2.2E+00	7.0E+00	10	100	7.35E+03	98%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1316-T03-B	1	8.87E+03			8.87E+03	6.2E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1316-T04-B	1	1.11E+04			1.11E+04	6.2E+00	2.2E+00	7.0E+00				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1316-T05-B	1	8.68E+02			8.68E+02	2.0E+01	2.2E+00	7.0E+00					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1316-T01-C	1	4.89E+03			4.89E+03	5.5E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1316-T02-C	1	6.99E+03			6.99E+03	8.1E-01	2.2E+00	7.0E+00	10	100	7.83E+03	85%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1316-T03-C	1	9.58E+03			9.58E+03	1.7E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1316-T04-C	1	1.22E+04			1.22E+04	6.3E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1316-T05-C	1	1.17E+04			1.17E+04	4.9E-01	2.2E+00	7.0E+00					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1316-B01-A	1	1.10E+00	U1/2		1.10E+00	2.0E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1316-B02-A	1	1.10E+00	U1/2		1.10E+00	7.8E+00	2.2E+00	7.0E+00				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
Cd	CFS-L07-1316-B03-A	1	1.10E+00	U1/2		1.10E+00	8.6E+00	2.2E+00	7.0E+00				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	CFS-L07-1316-T01-A	1	7.29E+05			7.29E+05	6.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1316-T02-A	1	4.60E+05			4.60E+05	7.6E+01	2.6E+00	8.3E+00	1000	100	4.60E+05	87%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1316-T03-A	1	6.45E+05			6.45E+05	6.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1316-T04-A	1	6.05E+05			6.05E+05	7.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1316-T05-A	1	5.77E+05			5.77E+05	8.0E-01	2.6E+00	8.3E+00					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1316-T01-B	1	7.03E+05			7.03E+05	9.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1316-T02-B	1	6.72E+05			6.72E+05	8.2E-01	2.6E+00	8.3E+00	1000	100	6.73E+05	85%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1316-T03-B	1	6.26E+05			6.26E+05	2.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1316-T04-B	1	6.24E+05			6.24E+05	6.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1316-T05-B	1	3.18E+04			3.18E+04	2.4E+01	2.6E+00	8.3E+00					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1316-T01-C	1	7.07E+05			7.07E+05	9.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1316-T02-C	1	6.63E+05			6.63E+05	8.0E-01	2.6E+00	8.3E+00	1000	100	6.64E+05	89%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1316-T03-C	1	6.18E+05			6.18E+05	3.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1316-T04-C	1	5.99E+05			5.99E+05	5.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1316-T05-C	1	5.68E+05			5.68E+05	3.2E-01	2.6E+00	8.3E+00					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1316-B01-A	1	2.80E+01			2.80E+01	1.6E+01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1316-B02-A	1	2.41E+01			2.41E+01	9.6E+00	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
Ca	CFS-L07-1316-B03-A	1	2.37E+01			2.37E+01	1.4E+01	2.6E+00	8.3E+00				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	CFS-L07-1316-T01-A	1	6.00E-01	U1/2		6.00E-01	2.9E+03	1.2E+00	3.8E+00				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1316-T02-A	1	6.00E-01	U1/2		6.00E-01	5.3E+01	1.2E+00	3.8E+00	10	100	9.71E+02	97%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1316-T03-A	1	6.00E-01	U1/2		6.00E-01	4.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1316-T04-A	1	6.00E-01	U1/2		6.00E-01	4.2E+02	1.2E+00	3.8E+00				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1316-T05-A	1	1.28E+00	E		1.28E+00	9.3E+01	1.2E+00	3.8E+00					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1316-T01-B	1	6.00E-01	U1/2		6.00E-01	5.7E+03	1.2E+00	3.8E+00				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1316-T02-B	1	6.00E-01	U1/2		6.00E-01	3.5E+02	1.2E+00	3.8E+00	10	100	9.85E+02	98%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1316-T03-B	1	6.00E-01	U1/2		6.00E-01	5.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1316-T04-B	1	6.00E-01	U1/2		6.00E-01	9.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1316-T05-B	1	6.00E-01	U1/2		6.00E-01	2.4E+01	1.2E+00	3.8E+00					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1316-T01-C	1	6.00E-01	U1/2		6.00E-01	9.7E+02	1.2E+00	3.8E+00				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1316-T02-C	1	6.00E-01	U1/2		6.00E-01	2.7E+03	1.2E+00	3.8E+00	10	100	9.69E+02	97%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1316-T03-C	1	6.00E-01	U1/2		6.00E-01	2.3E+02	1.2E+00	3.8E+00				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1316-T04-C	1	6.00E-01	U1/2		6.00E-01	1.5E+02	1.2E+00	3.8E+00				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1316-T05-C	1	6.00E-01	U1/2		6.00E-01	8.7E+02	1.2E+00	3.8E+00					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	3.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	1.6E+02	1.2E+00	3.8E+00				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
Cr	CFS-L07-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	1.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	CFS-L07-1316-T01-A	1	1.01E+02			1.01E+02	5.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1316-T02-A	1	1.08E+02			1.08E+02	7.7E+01	1.8E+00	5.7E+00	10	100	1.09E+03	98%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1316-T03-A	1	3.09E+02			3.09E+02	8.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1316-T04-A	1	3.93E+02			3.93E+02	3.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1316-T05-A	1	5.39E+02			5.39E+02	7.2E-01	1.8E+00	5.7E+00					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1316-T01-B	1	9.56E+01			9.56E+01	8.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1316-T02-B	1	1.61E+02			1.61E+02	1.5E+00	1.8E+00	5.7E+00	10	100	1.10E+03	94%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1316-T03-B	1	2.87E+02			2.87E+02	4.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1316-T04-B	1	4.03E+02			4.03E+02	5.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1316-T05-B	1	3.05E+01			3.05E+01	2.5E+01	1.8E+00	5.7E+00					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1316-T01-C	1	1.03E+02			1.03E+02	1.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1316-T02-C	1	1.89E+02			1.89E+02	8.6E-01	1.8E+00	5.7E+00	10	100	1.10E+03	91%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1316-T03-C	1	3.22E+02			3.22E+02	4.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1316-T04-C	1	4.61E+02			4.61E+02	7.3E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1316-T05-C	1	4.33E+02			4.33E+02	9.5E-02	1.8E+00	5.7E+00					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	1.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1316-B02-A	1	9.00E-01	U1/2		9.00E-01	1.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
Co	CFS-L07-1316-B03-A	1	9.00E-01	U1/2		9.00E-01	2.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	CFS-L07-1316-T01-A	1	9.15E+02			9.15E+02	3.1E-01	3.7E+00	1.2E+01				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1316-T02-A	1	8.76E+02			8.76E+02	7.4E+01	3.7E+00	1.2E+01	10	100	1.87E+03	99%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1316-T03-A	1	1.56E+03			1.56E+03	1.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1316-T04-A	1	1.85E+03			1.85E+03	4.2E-01	3.7E+00	1.2E+01				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1316-T05-A	1	2.49E+03			2.49E+03	4.3E-01	3.7E+00	1.2E+01					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1316-T01-B	1	8.84E+02			8.84E+02	7.4E-01	3.7E+00	1.2E+01				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1316-T02-B	1	9.88E+02			9.88E+02	1.2E+00	3.7E+00	1.2E+01	10	100	1.85E+03	86%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1316-T03-B	1	1.38E+03			1.38E+03	1.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1316-T04-B	1	1.80E+03			1.80E+03	4.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1316-T05-B	1	1.75E+02			1.75E+02	1.9E+01	3.7E+00	1.2E+01					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1316-T01-C	1	1.05E+03			1.05E+03	1.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1316-T02-C	1	1.19E+03			1.19E+03	1.0E+00	3.7E+00	1.2E+01	10	100	2.07E+03	88%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1316-T03-C	1	1.78E+03			1.78E+03	3.1E-01	3.7E+00	1.2E+01				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1316-T04-C	1	2.24E+03			2.24E+03	8.3E-01	3.7E+00	1.2E+01				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1316-T05-C	1	2.08E+03			2.08E+03	6.9E-01	3.7E+00	1.2E+01					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	1.5E+03	3.7E+00	1.2E+01				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1316-B02-A	1	1.85E+00	U1/2		1.85E+00	1.8E+03	3.7E+00	1.2E+01				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
Cu	CFS-L07-1316-B03-A	1	1.85E+00	U1/2		1.85E+00	4.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	CFS-L07-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	7.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00	1000	100	9.99E+02	100%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	5.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1316-T04-A	1	5.41E+00	E		5.41E+00	3.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1316-T05-A	1	3.40E+00	E		3.40E+00	6.7E+00	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	2.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	2.8E+01	2.0E+00	6.4E+00	1000	100	1.01E+03	101%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1316-T04-B	1	2.17E+00	E		2.17E+00	3.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1316-T05-B	1	1.00E+00	U1/2		1.00E+00	4.4E+00	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	8.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00	1000	100	9.94E+02	99%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	5.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	3.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1316-T05-C	1	1.00E+00	U1/2		1.00E+00	1.3E+01	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1316-B01-A	1	6.78E+00			6.78E+00	1.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1316-B02-A	1	1.00E+00	U1/2		1.00E+00	2.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
Fe	CFS-L07-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	CFS-L07-1316-T01-A	1	1.41E+03			1.41E+03	1.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1316-T02-A	1	9.60E+02			9.60E+02	7.5E+01	6.8E+00	2.2E+01	10	100	1.82E+03	86%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1316-T03-A	1	1.57E+03			1.57E+03	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1316-T04-A	1	1.63E+03			1.63E+03	1.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1316-T05-A	1	1.49E+03			1.49E+03	2.8E-01	6.8E+00	2.2E+01					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1316-T01-B	1	1.42E+03			1.42E+03	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1316-T02-B	1	1.41E+03			1.41E+03	6.8E-01	6.8E+00	2.2E+01	10	100	2.36E+03	95%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1316-T03-B	1	1.49E+03			1.49E+03	7.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1316-T04-B	1	1.60E+03			1.60E+03	4.3E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1316-T05-B	1	9.82E+01			9.82E+01	2.1E+01	6.8E+00	2.2E+01					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1316-T01-C	1	1.41E+03			1.41E+03	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1316-T02-C	1	1.56E+03			1.56E+03	1.6E+00	6.8E+00	2.2E+01	10	100	2.48E+03	92%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1316-T03-C	1	1.62E+03			1.62E+03	4.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1316-T04-C	1	1.68E+03			1.68E+03	2.8E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1316-T05-C	1	1.42E+03			1.42E+03	8.5E-01	6.8E+00	2.2E+01					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	4.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1316-B02-A	1	3.40E+00	U1/2		3.40E+00	1.5E+02	6.8E+00	2.2E+01				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
Pb	CFS-L07-1316-B03-A	1	3.40E+00	U1/2		3.40E+00	4.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	CFS-L07-1316-T01-A	1	2.07E+01			2.07E+01	6.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1316-T02-A	1	1.93E+01			1.93E+01	2.2E+01	1.9E+00	6.0E+00	10	100	8.78E+02	86%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1316-T03-A	1	1.65E+01			1.65E+01	1.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1316-T04-A	1	1.57E+01			1.57E+01	6.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1316-T05-A	1	2.74E+01			2.74E+01	7.4E+00	1.9E+00	6.0E+00					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1316-T01-B	1	2.12E+01			2.12E+01	1.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1316-T02-B	1	1.95E+01			1.95E+01	1.4E+01	1.9E+00	6.0E+00	10	100	8.87E+02	87%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1316-T03-B	1	1.55E+01			1.55E+01	6.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1316-T04-B	1	1.45E+01			1.45E+01	1.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1316-T05-B	1	1.15E+01			1.15E+01	5.6E+00	1.9E+00	6.0E+00					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1316-T01-C	1	2.03E+01			2.03E+01	1.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1316-T02-C	1	1.68E+01			1.68E+01	2.1E+01	1.9E+00	6.0E+00	10	100	8.98E+02	88%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1316-T03-C	1	1.60E+01			1.60E+01	8.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1316-T04-C	1	1.50E+01			1.50E+01	1.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1316-T05-C	1	2.33E+01			2.33E+01	5.1E+00	1.9E+00	6.0E+00					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1316-B01-A	1	6.09E+00			6.09E+00	5.6E-01	1.9E+00	6.0E+00				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1316-B02-A	1	5.57E+00	E		5.57E+00	5.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
Li	CFS-L07-1316-B03-A	1	7.35E+00			7.35E+00	8.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	CFS-L07-1316-T01-A	1	1.76E+03			1.76E+03	9.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1316-T02-A	1	2.50E+03			2.50E+03	7.2E+01	2.0E+00	6.4E+00	10	100	3.38E+03	88%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1316-T03-A	1	6.77E+03			6.77E+03	9.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1316-T04-A	1	9.73E+03			9.73E+03	1.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1316-T05-A	1	1.53E+04			1.53E+04	1.1E+00	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1316-T01-B	1	1.68E+03			1.68E+03	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1316-T02-B	1	3.14E+03			3.14E+03	1.3E+00	2.0E+00	6.4E+00	10	100	4.08E+03	93%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1316-T03-B	1	6.47E+03			6.47E+03	5.7E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1316-T04-B	1	1.01E+04			1.01E+04	4.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1316-T05-B	1	1.01E+03			1.01E+03	1.6E+01	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1316-T01-C	1	1.83E+03			1.83E+03	1.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1316-T02-C	1	3.62E+03			3.62E+03	1.1E+00	2.0E+00	6.4E+00	10	100	4.56E+03	95%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1316-T03-C	1	6.90E+03			6.90E+03	7.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1316-T04-C	1	1.11E+04			1.11E+04	1.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1316-T05-C	1	1.26E+04			1.26E+04	4.9E-01	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	6.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1316-B02-A	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
Mn	CFS-L07-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	1.9E+02	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	CFS-L07-1316-T01-A	1	7.48E+04			7.48E+04	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1316-T02-A	1	7.48E+04			7.48E+04	8.6E+01	1.0E+00	3.2E+00	1000	100	7.57E+04	93%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1316-T03-A	1	3.16E+05			3.16E+05	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1316-T04-A	1	5.61E+05			5.61E+05	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1316-T05-A	1	9.73E+05			9.73E+05	3.5E-01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1316-T01-B	1	7.31E+04			7.31E+04	4.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1316-T02-B	1	1.40E+05			1.40E+05	1.4E+00	1.0E+00	3.2E+00	1000	100	1.41E+05	97%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1316-T03-B	1	3.08E+05			3.08E+05	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1316-T04-B	1	5.69E+05			5.69E+05	3.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1316-T05-B	1	6.02E+04			6.02E+04	2.4E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1316-T01-C	1	7.54E+04			7.54E+04	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1316-T02-C	1	1.40E+05			1.40E+05	7.6E-01	1.0E+00	3.2E+00	1000	100	1.41E+05	87%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1316-T03-C	1	3.24E+05			3.24E+05	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1316-T04-C	1	5.76E+05			5.76E+05	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1316-T05-C	1	9.48E+05			9.48E+05	7.2E-01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.3E+02	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	1.9E+02	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
Mg	CFS-L07-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	6.8E+02	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	CFS-L07-1316-T01-A	1	1.08E+01			1.08E+01	1.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1316-T02-A	1	6.90E+00			6.90E+00	8.6E+01	1.2E+00	3.8E+00	10	100	9.50E+02	94%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1316-T03-A	1	1.64E+01			1.64E+01	7.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1316-T04-A	1	1.87E+01			1.87E+01	7.3E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1316-T05-A	1	2.65E+01			2.65E+01	7.7E+00	1.2E+00	3.8E+00					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1316-T01-B	1	1.05E+01			1.05E+01	6.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1316-T02-B	1	1.26E+01			1.26E+01	6.0E+00	1.2E+00	3.8E+00	10	100	9.71E+02	96%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1316-T03-B	1	1.69E+01			1.69E+01	6.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1316-T04-B	1	1.86E+01			1.86E+01	5.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1316-T05-B	1	6.00E-01	U1/2		6.00E-01	2.7E+01	1.2E+00	3.8E+00					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1316-T01-C	1	9.32E+00			9.32E+00	1.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1316-T02-C	1	1.27E+01			1.27E+01	5.0E+00	1.2E+00	3.8E+00	10	100	9.56E+02	94%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1316-T03-C	1	1.53E+01			1.53E+01	1.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1316-T04-C	1	1.91E+01			1.91E+01	6.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1316-T05-C	1	2.77E+01			2.77E+01	8.0E+00	1.2E+00	3.8E+00					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1316-B01-A	1	1.74E+00	E		1.74E+00	6.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1316-B02-A	1	6.00E-01	U1/2		6.00E-01	2.0E+02	1.2E+00	3.8E+00				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
Mo	CFS-L07-1316-B03-A	1	6.00E-01	U1/2		6.00E-01	2.8E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	CFS-L07-1316-T01-A	1	2.14E+02			2.14E+02	1.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1316-T02-A	1	2.16E+02			2.16E+02	7.5E+01	1.8E+00	5.7E+00	10	100	1.24E+03	102%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1316-T03-A	1	5.66E+02			5.66E+02	5.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1316-T04-A	1	6.68E+02			6.68E+02	3.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1316-T05-A	1	8.64E+02			8.64E+02	5.9E-01	1.8E+00	5.7E+00					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1316-T01-B	1	2.03E+02			2.03E+02	1.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1316-T02-B	1	3.17E+02			3.17E+02	1.7E+00	1.8E+00	5.7E+00	10	100	1.25E+03	93%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1316-T03-B	1	5.21E+02			5.21E+02	4.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1316-T04-B	1	6.87E+02			6.87E+02	5.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1316-T05-B	1	5.37E+01			5.37E+01	2.1E+01	1.8E+00	5.7E+00					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1316-T01-C	1	2.17E+02			2.17E+02	7.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1316-T02-C	1	3.70E+02			3.70E+02	2.3E+00	1.8E+00	5.7E+00	10	100	1.25E+03	88%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1316-T03-C	1	5.87E+02			5.87E+02	1.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1316-T04-C	1	7.89E+02			7.89E+02	4.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1316-T05-C	1	7.00E+02			7.00E+02	5.1E-01	1.8E+00	5.7E+00					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	2.3E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1316-B02-A	1	9.00E-01	U1/2		9.00E-01	2.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
Ni	CFS-L07-1316-B03-A	1	9.00E-01	U1/2		9.00E-01	5.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	CFS-L07-1316-T01-A	1	4.92E+00	E		4.92E+00	1.8E+02	3.7E+00	1.2E+01				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1316-T02-A	1	2.42E+01			2.42E+01	8.1E+01	3.7E+00	1.2E+01	1000	100	9.85E+02	96%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1316-T03-A	1	3.37E+01			3.37E+01	6.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1316-T04-A	1	2.67E+01			2.67E+01	2.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1316-T05-A	1	1.55E+01			1.55E+01	5.1E+01	3.7E+00	1.2E+01					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1316-T01-B	1	8.13E+00	E		8.13E+00	1.1E+02	3.7E+00	1.2E+01				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1316-T02-B	1	2.25E+01			2.25E+01	1.2E+02	3.7E+00	1.2E+01	1000	100	1.02E+03	100%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1316-T03-B	1	1.58E+01			1.58E+01	8.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1316-T04-B	1	2.15E+01			2.15E+01	5.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1316-T05-B	1	1.85E+00	U1/2		1.85E+00	6.0E+01	3.7E+00	1.2E+01					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1316-T01-C	1	1.85E+00	U1/2		1.85E+00	5.4E+02	3.7E+00	1.2E+01				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1316-T02-C	1	5.27E+00	E		5.27E+00	5.6E+01	3.7E+00	1.2E+01	1000	100	9.96E+02	99%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1316-T03-C	1	1.52E+01			1.52E+01	5.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1316-T04-C	1	3.57E+01			3.57E+01	3.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1316-T05-C	1	3.26E+01			3.26E+01	4.0E+01	3.7E+00	1.2E+01					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1316-B01-A	1	1.80E+01			1.80E+01	2.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1316-B02-A	1	1.19E+01			1.19E+01	3.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
P	CFS-L07-1316-B03-A	1	1.85E+00	U1/2		1.85E+00	1.9E+04	3.7E+00	1.2E+01				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	CFS-L07-1316-T01-A	1	1.07E+04			1.07E+04	5.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1316-T02-A	1	1.16E+04			1.16E+04	8.0E+01	1.6E+00	5.1E+00	1000	100	1.27E+04	104%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1316-T03-A	1	3.70E+04			3.70E+04	1.4E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1316-T04-A	1	5.71E+04			5.71E+04	7.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1316-T05-A	1	9.18E+04			9.18E+04	2.2E-01	1.6E+00	5.1E+00					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1316-T01-B	1	1.08E+04			1.08E+04	9.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1316-T02-B	1	1.90E+04			1.90E+04	6.7E-01	1.6E+00	5.1E+00	1000	100	2.00E+04	100%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1316-T03-B	1	3.73E+04			3.73E+04	4.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1316-T04-B	1	5.79E+04			5.79E+04	5.5E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1316-T05-B	1	4.31E+03			4.31E+03	2.9E+01	1.6E+00	5.1E+00					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1316-T01-C	1	1.03E+04			1.03E+04	6.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1316-T02-C	1	1.90E+04			1.90E+04	9.7E-01	1.6E+00	5.1E+00	1000	100	1.99E+04	92%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1316-T03-C	1	3.60E+04			3.60E+04	4.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1316-T04-C	1	6.01E+04			6.01E+04	7.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1316-T05-C	1	8.88E+04			8.88E+04	4.4E-01	1.6E+00	5.1E+00					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1316-B01-A	1	9.57E+00			9.57E+00	4.6E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1316-B02-A	1	3.72E+00	E		3.72E+00	7.2E+01	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
K	CFS-L07-1316-B03-A	1	8.00E-01	U1/2		8.00E-01	1.9E+02	1.6E+00	5.1E+00				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	CFS-L07-1316-T01-A	1	8.53E+01			8.53E+01	2.1E+01	1.5E+01	4.8E+01				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1316-T02-A	1	1.01E+02			1.01E+02	7.9E+01	1.5E+01	4.8E+01	10	100	1.10E+03	100%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1316-T03-A	1	3.04E+02			3.04E+02	3.8E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1316-T04-A	1	5.29E+02			5.29E+02	1.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1316-T05-A	1	9.33E+02			9.33E+02	1.4E+00	1.5E+01	4.8E+01					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1316-T01-B	1	8.67E+01			8.67E+01	5.2E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1316-T02-B	1	1.42E+02			1.42E+02	7.8E+00	1.5E+01	4.8E+01	10	100	1.09E+03	95%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1316-T03-B	1	2.94E+02			2.94E+02	3.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1316-T04-B	1	5.25E+02			5.25E+02	7.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1316-T05-B	1	4.90E+01			4.90E+01	2.5E+01	1.5E+01	4.8E+01					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1316-T01-C	1	8.04E+01			8.04E+01	2.0E+01	1.5E+01	4.8E+01				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1316-T02-C	1	1.40E+02			1.40E+02	9.8E+00	1.5E+01	4.8E+01	10	100	1.09E+03	95%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1316-T03-C	1	2.92E+02			2.92E+02	4.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1316-T04-C	1	5.50E+02			5.50E+02	4.6E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1316-T05-C	1	9.31E+02			9.31E+02	2.2E+00	1.5E+01	4.8E+01					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1316-B01-A	1	7.50E+00	U1/2		7.50E+00	2.2E+02	1.5E+01	4.8E+01				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1316-B02-A	1	7.50E+00	U1/2		7.50E+00	3.7E+01	1.5E+01	4.8E+01				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
Se	CFS-L07-1316-B03-A	1	7.50E+00	U1/2		7.50E+00	1.1E+02	1.5E+01	4.8E+01				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	CFS-L07-1316-T01-A	1	4.41E+03			4.41E+03	5.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1316-T02-A	1	4.11E+03			4.11E+03	7.5E+01	1.1E+00	3.5E+00	1000	100	5.02E+03	91%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1316-T03-A	1	6.92E+03			6.92E+03	1.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1316-T04-A	1	7.03E+03			7.03E+03	3.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1316-T05-A	1	7.35E+03			7.35E+03	5.7E-01	1.1E+00	3.5E+00					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1316-T01-B	1	4.23E+03			4.23E+03	7.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1316-T02-B	1	5.29E+03			5.29E+03	8.3E-01	1.1E+00	3.5E+00	1000	100	6.14E+03	86%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1316-T03-B	1	6.53E+03			6.53E+03	2.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1316-T04-B	1	6.99E+03			6.99E+03	3.7E+00	1.1E+00	3.5E+00				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1316-T05-B	1	4.67E+02			4.67E+02	2.3E+01	1.1E+00	3.5E+00					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1316-T01-C	1	4.09E+03			4.09E+03	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1316-T02-C	1	5.76E+03			5.76E+03	1.2E+00	1.1E+00	3.5E+00	1000	100	6.68E+03	92%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1316-T03-C	1	7.14E+03			7.14E+03	8.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1316-T04-C	1	7.67E+03			7.67E+03	7.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1316-T05-C	1	6.99E+03			6.99E+03	4.1E-01	1.1E+00	3.5E+00					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1316-B01-A	1	4.63E+00			4.63E+00	6.2E+01	1.1E+00	3.5E+00				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1316-B02-A	1	5.50E-01	U1/2		5.50E-01	1.1E+02	1.1E+00	3.5E+00				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
Si	CFS-L07-1316-B03-A	1	8.28E+00			8.28E+00	8.5E+01	1.1E+00	3.5E+00				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	CFS-L07-1316-T01-A	1	2.15E+04			2.15E+04	7.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1316-T02-A	1	2.35E+04			2.35E+04	7.1E+01	2.5E+00	8.0E+00	1000	100	2.44E+04	97%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1316-T03-A	1	8.39E+04			8.39E+04	5.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1316-T04-A	1	1.29E+05			1.29E+05	5.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1316-T05-A	1	1.96E+05			1.96E+05	5.5E-01	2.5E+00	8.0E+00					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1316-T01-B	1	2.23E+04			2.23E+04	6.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1316-T02-B	1	4.05E+04			4.05E+04	9.9E-01	2.5E+00	8.0E+00	1000	100	4.14E+04	90%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1316-T03-B	1	8.01E+04			8.01E+04	2.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1316-T04-B	1	1.28E+05			1.28E+05	2.0E+00	2.5E+00	8.0E+00				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1316-T05-B	1	3.36E+04			3.36E+04	2.3E+01	2.5E+00	8.0E+00					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1316-T01-C	1	2.17E+04			2.17E+04	7.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1316-T02-C	1	4.09E+04			4.09E+04	7.2E-01	2.5E+00	8.0E+00	1000	100	4.19E+04	92%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1316-T03-C	1	8.63E+04			8.63E+04	6.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1316-T04-C	1	1.33E+05			1.33E+05	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1316-T05-C	1	1.95E+05			1.95E+05	9.6E-02	2.5E+00	8.0E+00					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1316-B01-A	1	2.95E+01			2.95E+01	6.5E+00	2.5E+00	8.0E+00				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1316-B02-A	1	7.77E+01			7.77E+01	3.7E+00	2.5E+00	8.0E+00				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
Na	CFS-L07-1316-B03-A	1	1.91E+01			1.91E+01	2.4E+01	2.5E+00	8.0E+00				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	CFS-L07-1316-T01-A	1	1.68E+03			1.68E+03	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1316-T02-A	1	1.76E+03			1.76E+03	7.5E+01	1.0E+00	3.2E+00	1000	100	2.74E+03	98%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1316-T03-A	1	3.66E+03			3.66E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1316-T04-A	1	4.69E+03			4.69E+03	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1316-T05-A	1	5.71E+03			5.71E+03	9.1E-01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1316-T01-B	1	1.71E+03			1.71E+03	6.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1316-T02-B	1	2.53E+03			2.53E+03	9.1E-01	1.0E+00	3.2E+00	1000	100	3.54E+03	101%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1316-T03-B	1	3.64E+03			3.64E+03	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1316-T04-B	1	4.79E+03			4.79E+03	3.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1316-T05-B	1	5.30E+02			5.30E+02	2.3E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1316-T01-C	1	1.52E+03			1.52E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1316-T02-C	1	2.30E+03			2.30E+03	1.7E+00	1.0E+00	3.2E+00	1000	100	3.18E+03	88%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1316-T03-C	1	3.22E+03			3.22E+03	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1316-T04-C	1	4.25E+03			4.25E+03	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1316-T05-C	1	5.83E+03			5.83E+03	8.2E-01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	6.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
Sr	CFS-L07-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	7.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	CFS-L07-1316-T01-A	1	6.66E+05			6.66E+05	2.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1316-T02-A	1	4.33E+05			4.33E+05	7.7E+01	6.8E+00	2.2E+01	1000	100	4.34E+05	88%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1316-T03-A	1	9.26E+05			9.26E+05	6.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1316-T04-A	1	1.20E+06			1.20E+06	4.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1316-T05-A	1	1.62E+06			1.62E+06	5.5E-01	6.8E+00	2.2E+01					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1316-T01-B	1	6.57E+05			6.57E+05	8.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1316-T02-B	1	7.20E+05			7.20E+05	9.8E-01	6.8E+00	2.2E+01	1000	100	7.21E+05	82%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1316-T03-B	1	9.01E+05			9.01E+05	4.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1316-T04-B	1	1.22E+06			1.22E+06	5.8E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1316-T05-B	1	1.11E+05			1.11E+05	1.6E+01	6.8E+00	2.2E+01					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1316-T01-C	1	6.61E+05			6.61E+05	4.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1316-T02-C	1	7.28E+05			7.28E+05	1.2E+00	6.8E+00	2.2E+01	1000	100	7.29E+05	90%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1316-T03-C	1	9.30E+05			9.30E+05	4.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1316-T04-C	1	1.23E+06			1.23E+06	7.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1316-T05-C	1	1.59E+06			1.59E+06	4.1E-01	6.8E+00	2.2E+01					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	4.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1316-B02-A	1	3.40E+00	U1/2		3.40E+00	3.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
S	CFS-L07-1316-B03-A	1	3.40E+00	U1/2		3.40E+00	3.8E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	CFS-L07-1316-T01-A	1	3.77E+02			3.77E+02	1.7E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1316-T02-A	1	3.47E+02			3.47E+02	7.9E+01	4.6E+00	1.5E+01	10	100	1.31E+03	96%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1316-T03-A	1	9.05E+02			9.05E+02	2.5E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1316-T04-A	1	1.20E+03			1.20E+03	8.0E-01	4.6E+00	1.5E+01				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1316-T05-A	1	1.59E+03			1.59E+03	3.4E-01	4.6E+00	1.5E+01					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1316-T01-B	1	3.72E+02			3.72E+02	1.8E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1316-T02-B	1	5.42E+02			5.42E+02	2.5E-01	4.6E+00	1.5E+01	10	100	1.53E+03	99%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1316-T03-B	1	8.67E+02			8.67E+02	3.2E-01	4.6E+00	1.5E+01				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1316-T04-B	1	1.18E+03			1.18E+03	5.8E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1316-T05-B	1	9.82E+01			9.82E+01	2.5E+01	4.6E+00	1.5E+01					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1316-T01-C	1	3.80E+02			3.80E+02	1.6E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1316-T02-C	1	5.71E+02			5.71E+02	2.3E+00	4.6E+00	1.5E+01	10	100	1.53E+03	96%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1316-T03-C	1	9.02E+02			9.02E+02	2.0E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1316-T04-C	1	1.26E+03			1.26E+03	8.2E-01	4.6E+00	1.5E+01				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1316-T05-C	1	1.54E+03			1.54E+03	5.8E-01	4.6E+00	1.5E+01					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1316-B01-A	1	2.30E+00	U1/2		2.30E+00	9.1E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1316-B02-A	1	2.30E+00	U1/2		2.30E+00	6.5E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
Tl	CFS-L07-1316-B03-A	1	2.30E+00	U1/2		2.30E+00	1.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	CFS-L07-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	3.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	3.4E+02	2.0E+00	6.4E+00	10	100	9.80E+02	98%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	1.4E+03	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	7.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1316-T05-A	1	1.00E+00	U1/2		1.00E+00	7.3E+01	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	9.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	1.1E+03	2.0E+00	6.4E+00	10	100	9.92E+02	99%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	2.9E+02	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	7.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1316-T05-B	1	1.00E+00	U1/2		1.00E+00	3.3E+01	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	3.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	4.9E+01	2.0E+00	6.4E+00	10	100	9.78E+02	98%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	5.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	2.7E+02	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1316-T05-C	1	1.00E+00	U1/2		1.00E+00	1.0E+02	2.0E+00	6.4E+00					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	3.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1316-B02-A	1	1.00E+00	U1/2		1.00E+00	3.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
Ti	CFS-L07-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	2.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	CFS-L07-1316-T01-A	1	3.57E+01			3.57E+01	2.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1316-T02-A	1	2.14E+01			2.14E+01	7.4E+01	1.5E+00	4.8E+00	10	100	9.72E+02	95%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1316-T03-A	1	3.10E+01			3.10E+01	3.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1316-T04-A	1	2.79E+01			2.79E+01	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1316-T05-A	1	2.69E+01			2.69E+01	3.1E+00	1.5E+00	4.8E+00					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1316-T01-B	1	3.39E+01			3.39E+01	3.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1316-T02-B	1	3.35E+01			3.35E+01	4.1E+00	1.5E+00	4.8E+00	10	100	9.79E+02	95%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1316-T03-B	1	2.94E+01			2.94E+01	1.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1316-T04-B	1	3.04E+01			3.04E+01	7.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1316-T05-B	1	7.50E-01	U1/2		7.50E-01	4.5E+01	1.5E+00	4.8E+00					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1316-T01-C	1	3.49E+01			3.49E+01	4.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1316-T02-C	1	3.18E+01			3.18E+01	3.7E+00	1.5E+00	4.8E+00	10	100	9.66E+02	93%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1316-T03-C	1	3.00E+01			3.00E+01	4.9E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1316-T04-C	1	2.92E+01			2.92E+01	6.9E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1316-T05-C	1	2.71E+01			2.71E+01	2.2E+00	1.5E+00	4.8E+00					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1316-B01-A	1	7.50E-01	U1/2		7.50E-01	4.8E+02	1.5E+00	4.8E+00				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1316-B02-A	1	7.50E-01	U1/2		7.50E-01	1.5E+02	1.5E+00	4.8E+00				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
V	CFS-L07-1316-B03-A	1	7.50E-01	U1/2		7.50E-01	1.0E+02	1.5E+00	4.8E+00				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	CFS-L07-1316-T01-A	1	2.03E+04			2.03E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:41 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1316-T02-A	1	2.01E+04			2.01E+04	7.3E+01	1.0E+00	3.2E+00	10	100	2.10E+04	90%	VU ICP-OES	5/18/11 4:43 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1316-T03-A	1	3.99E+04			3.99E+04	7.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:45 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1316-T04-A	1	4.33E+04			4.33E+04	9.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:46 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1316-T05-A	1	5.27E+04			5.27E+04	6.6E-01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:48 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1316-T01-B	1	1.88E+04			1.88E+04	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:50 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1316-T02-B	1	2.45E+04			2.45E+04	1.2E+00	1.0E+00	3.2E+00	10	100	2.54E+04	91%	VU ICP-OES	5/18/11 4:51 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1316-T03-B	1	3.60E+04			3.60E+04	9.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:53 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1316-T04-B	1	4.51E+04			4.51E+04	4.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:54 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1316-T05-B	1	3.39E+03			3.39E+03	2.5E+01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 4:56 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1316-T01-C	1	2.11E+04			2.11E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:58 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1316-T02-C	1	2.93E+04			2.93E+04	6.6E-01	1.0E+00	3.2E+00	10	100	3.02E+04	86%	VU ICP-OES	5/18/11 4:59 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1316-T03-C	1	4.14E+04			4.14E+04	1.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 5:01 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1316-T04-C	1	5.18E+04			5.18E+04	8.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 5:03 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1316-T05-C	1	4.35E+04			4.35E+04	2.9E-01	1.0E+00	3.2E+00					VU ICP-OES	5/18/11 5:04 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1316-B01-A	1	2.83E+00	E		2.83E+00	5.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:36 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1316-B02-A	1	1.78E+00	E		1.78E+00	1.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:38 PM	EPA Interlab L07 1313-1316 CFS
Zn	CFS-L07-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	2.0E+02	1.0E+00	3.2E+00				---	VU ICP-OES	5/18/11 4:40 PM	EPA Interlab L07 1313-1316 CFS

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	CFS-L09-1316-T01-A	1	5.07E+01			5.07E+01	8.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1316-T02-A	1	4.83E+01			4.83E+01	6.6E+00	1.0E+00	3.2E+00	1000	100	1.08E+03	103%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1316-T03-A	1	5.26E+01			5.26E+01	9.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1316-T04-A	1	5.67E+01			5.67E+01	6.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1316-T05-A	1	6.00E+01			6.00E+01	5.6E+00	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1316-T01-B	1	5.38E+01			5.38E+01	5.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1316-T02-B	1	5.00E+01			5.00E+01	8.2E+00	1.0E+00	3.2E+00	1000	100	1.04E+03	99%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1316-T03-B	1	5.35E+01			5.35E+01	3.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1316-T04-B	1	6.05E+01			6.05E+01	5.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1316-T05-B	1	5.88E+01			5.88E+01	3.6E+00	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1316-T01-C	1	5.09E+01			5.09E+01	9.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1316-T02-C	1	5.14E+01			5.14E+01	5.4E+00	1.0E+00	3.2E+00	1000	100	1.05E+03	100%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1316-T03-C	1	5.99E+01			5.99E+01	7.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1316-T04-C	1	5.98E+01			5.98E+01	8.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1316-T05-C	1	6.24E+01			6.24E+01	2.6E+00	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1316-B01-A	1	2.97E+00	E		2.97E+00	4.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	2.0E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
Al	CFS-L09-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	5.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	CFS-L09-1316-T01-A	1	5.60E+01			5.60E+01	9.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1316-T02-A	1	3.45E+01			3.45E+01	1.3E+01	7.5E+00	2.4E+01	10	100	1.05E+03	102%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1316-T03-A	1	4.06E+01			4.06E+01	1.6E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1316-T04-A	1	5.48E+01			5.48E+01	1.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1316-T05-A	1	5.58E+01			5.58E+01	2.1E+01	7.5E+00	2.4E+01					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1316-T01-B	1	2.87E+01			2.87E+01	2.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1316-T02-B	1	2.95E+01			2.95E+01	3.0E+01	7.5E+00	2.4E+01	10	100	1.06E+03	103%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1316-T03-B	1	4.38E+01			4.38E+01	1.4E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1316-T04-B	1	4.10E+01			4.10E+01	7.7E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1316-T05-B	1	5.60E+01			5.60E+01	1.3E+01	7.5E+00	2.4E+01					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1316-T01-C	1	2.69E+01			2.69E+01	5.5E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1316-T02-C	1	3.90E+01			3.90E+01	3.0E+01	7.5E+00	2.4E+01	10	100	1.05E+03	101%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1316-T03-C	1	4.94E+01			4.94E+01	6.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1316-T04-C	1	5.39E+01			5.39E+01	1.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1316-T05-C	1	5.79E+01			5.79E+01	7.3E+00	7.5E+00	2.4E+01					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1316-B01-A	1	3.75E+00	U1/2		3.75E+00	4.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1316-B02-A	1	3.75E+00	U1/2		3.75E+00	7.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
Sb	CFS-L09-1316-B03-A	1	3.75E+00	U1/2		3.75E+00	7.8E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	CFS-L09-1316-T01-A	1	2.38E+01	E		2.38E+01	9.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1316-T02-A	1	2.58E+01	E		2.58E+01	4.6E+01	1.1E+01	3.5E+01	10	100	1.04E+03	101%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1316-T03-A	1	2.80E+01	E		2.80E+01	3.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1316-T04-A	1	3.89E+01			3.89E+01	2.1E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1316-T05-A	1	4.41E+01			4.41E+01	6.1E+00	1.1E+01	3.5E+01					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1316-T01-B	1	2.83E+01	E		2.83E+01	2.2E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1316-T02-B	1	1.99E+01	E		1.99E+01	2.6E+01	1.1E+01	3.5E+01	10	100	1.05E+03	103%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1316-T03-B	1	3.65E+01			3.65E+01	1.5E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1316-T04-B	1	4.16E+01			4.16E+01	1.1E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1316-T05-B	1	5.02E+01			5.02E+01	8.9E+00	1.1E+01	3.5E+01					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1316-T01-C	1	1.85E+01	E		1.85E+01	5.8E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1316-T02-C	1	3.10E+01	E		3.10E+01	1.4E+01	1.1E+01	3.5E+01	10	100	1.05E+03	101%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1316-T03-C	1	3.27E+01	E		3.27E+01	1.8E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1316-T04-C	1	3.82E+01			3.82E+01	2.6E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1316-T05-C	1	4.25E+01			4.25E+01	2.5E+01	1.1E+01	3.5E+01					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1316-B01-A	1	5.50E+00	U1/2		5.50E+00	2.7E+02	1.1E+01	3.5E+01				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1316-B02-A	1	5.50E+00	U1/2		5.50E+00	3.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
As	CFS-L09-1316-B03-A	1	5.50E+00	U1/2		5.50E+00	1.1E+02	1.1E+01	3.5E+01				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	CFS-L09-1316-T01-A	1	1.53E+02			1.53E+02	6.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1316-T02-A	1	2.71E+02			2.71E+02	1.1E+00	1.0E+00	3.2E+00	1000	100	1.29E+03	102%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1316-T03-A	1	5.67E+02			5.67E+02	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1316-T04-A	1	9.00E+02			9.00E+02	4.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1316-T05-A	1	1.25E+03			1.25E+03	3.5E-01	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1316-T01-B	1	1.65E+02			1.65E+02	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1316-T02-B	1	2.73E+02			2.73E+02	2.8E-01	1.0E+00	3.2E+00	1000	100	1.31E+03	104%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1316-T03-B	1	5.57E+02			5.57E+02	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1316-T04-B	1	8.31E+02			8.31E+02	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1316-T05-B	1	1.24E+03			1.24E+03	2.7E-01	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1316-T01-C	1	1.66E+02			1.66E+02	3.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1316-T02-C	1	2.88E+02			2.88E+02	2.8E-01	1.0E+00	3.2E+00	1000	100	1.31E+03	102%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1316-T03-C	1	5.81E+02			5.81E+02	6.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1316-T04-C	1	8.90E+02			8.90E+02	2.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1316-T05-C	1	1.24E+03			1.24E+03	2.0E-01	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	5.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	5.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
B	CFS-L09-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	2.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	CFS-L09-1316-T01-A	1	1.28E+02			1.28E+02	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1316-T02-A	1	1.14E+02			1.14E+02	6.1E-01	1.0E+00	3.2E+00	10	100	1.18E+03	107%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1316-T03-A	1	9.65E+01			9.65E+01	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1316-T04-A	1	8.19E+01			8.19E+01	5.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1316-T05-A	1	6.18E+01			6.18E+01	9.2E-01	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1316-T01-B	1	1.28E+02			1.28E+02	1.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1316-T02-B	1	1.23E+02			1.23E+02	7.8E-01	1.0E+00	3.2E+00	10	100	1.20E+03	108%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1316-T03-B	1	1.00E+02			1.00E+02	2.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1316-T04-B	1	8.27E+01			8.27E+01	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1316-T05-B	1	6.29E+01			6.29E+01	5.2E-02	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1316-T01-C	1	1.29E+02			1.29E+02	2.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1316-T02-C	1	1.20E+02			1.20E+02	7.1E-01	1.0E+00	3.2E+00	10	100	1.18E+03	106%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1316-T03-C	1	9.88E+01			9.88E+01	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1316-T04-C	1	8.20E+01			8.20E+01	2.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1316-T05-C	1	6.42E+01			6.42E+01	3.8E-01	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	3.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	1.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
Ba	CFS-L09-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	5.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	CFS-L09-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	4.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	1.8E+01	1.9E+00	6.0E+00	10	100	1.07E+03	107%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	2.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	4.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1316-T05-A	1	9.50E-01	U1/2		9.50E-01	2.0E+01	1.9E+00	6.0E+00					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	8.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	4.9E+01	1.9E+00	6.0E+00	10	100	1.06E+03	106%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	7.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	3.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1316-T05-B	1	9.50E-01	U1/2		9.50E-01	2.9E+01	1.9E+00	6.0E+00					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	4.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	7.1E+01	1.9E+00	6.0E+00	10	100	1.05E+03	105%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	4.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	1.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1316-T05-C	1	9.50E-01	U1/2		9.50E-01	4.9E+01	1.9E+00	6.0E+00					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	3.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1316-B02-A	1	9.50E-01	U1/2		9.50E-01	1.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
Be	CFS-L09-1316-B03-A	1	9.50E-01	U1/2		9.50E-01	3.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	CFS-L09-1316-T01-A	1	4.46E+03			4.46E+03	9.1E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1316-T02-A	1	6.32E+03			6.32E+03	7.6E-01	2.2E+00	7.0E+00	10	100	7.20E+03	88%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1316-T03-A	1	9.03E+03			9.03E+03	1.2E+00	2.2E+00	7.0E+00				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1316-T04-A	1	1.14E+04			1.14E+04	2.8E-01	2.2E+00	1.0E+00				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1316-T05-A	1	1.31E+04			1.31E+04	5.1E-01	2.2E+00	1.0E+00					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1316-T01-B	1	4.48E+03			4.48E+03	4.6E-01	2.2E+00	1.0E+00				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1316-T02-B	1	6.12E+03			6.12E+03	9.1E-01	2.2E+00	1.0E+00	10	100	7.08E+03	96%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1316-T03-B	1	8.72E+03			8.72E+03	2.2E-01	2.2E+00	1.0E+00				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1316-T04-B	1	1.03E+04			1.03E+04	9.9E-01	2.2E+00	1.0E+00				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1316-T05-B	1	1.26E+04			1.26E+04	1.5E+00	2.2E+00	1.0E+00					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1316-T01-C	1	4.39E+03			4.39E+03	4.0E-01	2.2E+00	1.0E+00				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1316-T02-C	1	6.33E+03			6.33E+03	6.0E-01	2.2E+00	1.0E+00	10	100	7.27E+03	94%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1316-T03-C	1	8.95E+03			8.95E+03	2.3E-01	2.2E+00	1.0E+00				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1316-T04-C	1	1.09E+04			1.09E+04	3.6E-01	2.2E+00	1.0E+00				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1316-T05-C	1	1.28E+04			1.28E+04	1.1E+00	2.2E+00	1.0E+00					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1316-B01-A	1	1.10E+00	U1/2		1.10E+00	7.5E+01	2.2E+00	1.0E+00				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1316-B02-A	1	1.10E+00	U1/2		1.10E+00	6.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
Cd	CFS-L09-1316-B03-A	1	1.10E+00	U1/2		1.10E+00	1.0E+02	2.2E+00	7.0E+00				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	CFS-L09-1316-T01-A	1	6.86E+05			6.86E+05	1.3E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1316-T02-A	1	6.61E+05			6.61E+05	8.5E-01	2.6E+00	8.3E+00	1000	100	6.62E+05	90%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1316-T03-A	1	6.14E+05			6.14E+05	1.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1316-T04-A	1	5.86E+05			5.86E+05	4.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1316-T05-A	1	5.25E+05			5.25E+05	6.1E-01	2.6E+00	8.3E+00					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1316-T01-B	1	6.96E+05			6.96E+05	2.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1316-T02-B	1	6.69E+05			6.69E+05	8.7E-01	2.6E+00	8.3E+00	1000	100	6.70E+05	87%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1316-T03-B	1	6.29E+05			6.29E+05	5.6E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1316-T04-B	1	5.87E+05			5.87E+05	1.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1316-T05-B	1	5.23E+05			5.23E+05	6.1E-01	2.6E+00	8.3E+00					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1316-T01-C	1	6.80E+05			6.80E+05	1.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1316-T02-C	1	6.67E+05			6.67E+05	5.3E-01	2.6E+00	8.3E+00	1000	100	6.68E+05	92%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1316-T03-C	1	6.30E+05			6.30E+05	3.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1316-T04-C	1	5.80E+05			5.80E+05	4.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1316-T05-C	1	5.38E+05			5.38E+05	1.5E-01	2.6E+00	8.3E+00					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1316-B01-A	1	2.57E+01			2.57E+01	8.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1316-B02-A	1	3.20E+01			3.20E+01	6.7E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
Ca	CFS-L09-1316-B03-A	1	2.25E+01			2.25E+01	5.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	CFS-L09-1316-T01-A	1	6.00E-01	U1/2		6.00E-01	7.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1316-T02-A	1	6.00E-01	U1/2		6.00E-01	2.3E+01	1.2E+00	3.8E+00	10	100	1.02E+03	102%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1316-T03-A	1	6.00E-01	U1/2		6.00E-01	7.7E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1316-T04-A	1	6.00E-01	U1/2		6.00E-01	5.4E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1316-T05-A	1	6.00E-01	U1/2		6.00E-01	8.3E+01	1.2E+00	3.8E+00					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1316-T01-B	1	6.00E-01	U1/2		6.00E-01	2.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1316-T02-B	1	6.00E-01	U1/2		6.00E-01	8.2E+02	1.2E+00	3.8E+00	10	100	1.04E+03	104%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1316-T03-B	1	6.00E-01	U1/2		6.00E-01	6.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1316-T04-B	1	6.00E-01	U1/2		6.00E-01	5.5E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1316-T05-B	1	6.00E-01	U1/2		6.00E-01	8.1E+01	1.2E+00	3.8E+00					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1316-T01-C	1	6.00E-01	U1/2		6.00E-01	1.3E+03	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1316-T02-C	1	6.00E-01	U1/2		6.00E-01	2.7E+01	1.2E+00	3.8E+00	10	100	1.02E+03	102%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1316-T03-C	1	6.00E-01	U1/2		6.00E-01	2.9E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1316-T04-C	1	6.00E-01	U1/2		6.00E-01	1.2E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1316-T05-C	1	6.00E-01	U1/2		6.00E-01	3.0E+01	1.2E+00	3.8E+00					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	6.6E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	1.0E+04	1.2E+00	3.8E+00				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
Cr	CFS-L09-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	8.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	CFS-L09-1316-T01-A	1	9.95E+01			9.95E+01	3.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1316-T02-A	1	1.64E+02			1.64E+02	1.1E+00	1.8E+00	5.7E+00	10	100	1.14E+03	98%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1316-T03-A	1	3.04E+02			3.04E+02	5.3E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1316-T04-A	1	4.38E+02			4.38E+02	3.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1316-T05-A	1	5.44E+02			5.44E+02	9.5E-02	1.8E+00	5.7E+00					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1316-T01-B	1	1.03E+02			1.03E+02	1.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1316-T02-B	1	1.65E+02			1.65E+02	6.2E-01	1.8E+00	5.7E+00	10	100	1.16E+03	100%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1316-T03-B	1	2.95E+02			2.95E+02	4.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1316-T04-B	1	3.93E+02			3.93E+02	1.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1316-T05-B	1	5.22E+02			5.22E+02	1.4E-01	1.8E+00	5.7E+00					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1316-T01-C	1	1.02E+02			1.02E+02	5.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1316-T02-C	1	1.72E+02			1.72E+02	1.3E+00	1.8E+00	5.7E+00	10	100	1.15E+03	98%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1316-T03-C	1	3.12E+02			3.12E+02	4.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1316-T04-C	1	4.30E+02			4.30E+02	4.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1316-T05-C	1	5.23E+02			5.23E+02	4.3E-01	1.8E+00	5.7E+00					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	2.0E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1316-B02-A	1	9.00E-01	U1/2		9.00E-01	4.2E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
Co	CFS-L09-1316-B03-A	1	9.00E-01	U1/2		9.00E-01	1.8E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	CFS-L09-1316-T01-A	1	7.67E+02			7.67E+02	1.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1316-T02-A	1	1.01E+03			1.01E+03	5.5E-01	3.7E+00	1.2E+01	10	100	1.97E+03	95%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1316-T03-A	1	1.48E+03			1.48E+03	2.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1316-T04-A	1	2.24E+03			2.24E+03	9.1E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1316-T05-A	1	3.00E+03			3.00E+03	1.3E+00	3.7E+00	1.2E+01					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1316-T01-B	1	7.56E+02			7.56E+02	6.0E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1316-T02-B	1	9.67E+02			9.67E+02	5.9E-01	3.7E+00	1.2E+01	10	100	1.95E+03	98%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1316-T03-B	1	1.46E+03			1.46E+03	1.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1316-T04-B	1	2.18E+03			2.18E+03	1.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1316-T05-B	1	2.86E+03			2.86E+03	3.3E-01	3.7E+00	1.2E+01					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1316-T01-C	1	7.50E+02			7.50E+02	4.7E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1316-T02-C	1	1.09E+03			1.09E+03	8.7E-01	3.7E+00	1.2E+01	10	100	2.02E+03	93%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1316-T03-C	1	1.55E+03			1.55E+03	3.0E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1316-T04-C	1	2.28E+03			2.28E+03	6.6E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1316-T05-C	1	2.90E+03			2.90E+03	1.3E+00	3.7E+00	1.2E+01					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	2.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1316-B02-A	1	1.85E+00	U1/2		1.85E+00	9.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
Cu	CFS-L09-1316-B03-A	1	1.85E+00	U1/2		1.85E+00	5.4E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	CFS-L09-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	2.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	4.7E+01	2.0E+00	6.4E+00	1000	100	1.05E+03	105%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	5.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1316-T05-A	1	2.49E+00	E		2.49E+00	1.5E+01	2.0E+00	6.4E+00					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	2.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	5.6E+01	2.0E+00	6.4E+00	1000	100	1.07E+03	107%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	3.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	6.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1316-T05-B	1	2.36E+00	E		2.36E+00	2.6E+01	2.0E+00	6.4E+00					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1316-T01-C	1	2.58E+00	E		2.58E+00	1.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	3.3E+01	2.0E+00	6.4E+00	1000	100	1.05E+03	105%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1316-T03-C	1	3.06E+00	E		3.06E+00	1.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1316-T04-C	1	3.33E+00	E		3.33E+00	8.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1316-T05-C	1	2.14E+00	E		2.14E+00	1.9E+01	2.0E+00	6.4E+00					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1316-B02-A	1	1.00E+00	U1/2		1.00E+00	7.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
Fe	CFS-L09-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	8.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	CFS-L09-1316-T01-A	1	1.22E+03			1.22E+03	1.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1316-T02-A	1	1.30E+03			1.30E+03	1.1E+00	6.8E+00	2.2E+01	10	100	2.24E+03	94%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1316-T03-A	1	1.41E+03			1.41E+03	8.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1316-T04-A	1	1.50E+03			1.50E+03	3.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1316-T05-A	1	1.47E+03			1.47E+03	7.5E-01	6.8E+00	2.2E+01					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1316-T01-B	1	1.24E+03			1.24E+03	3.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1316-T02-B	1	1.35E+03			1.35E+03	1.3E+00	6.8E+00	2.2E+01	10	100	2.27E+03	93%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1316-T03-B	1	1.46E+03			1.46E+03	6.7E-02	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1316-T04-B	1	1.48E+03			1.48E+03	6.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1316-T05-B	1	1.46E+03			1.46E+03	2.0E-01	6.8E+00	2.2E+01					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1316-T01-C	1	1.29E+03			1.29E+03	3.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1316-T02-C	1	1.35E+03			1.35E+03	8.7E-01	6.8E+00	2.2E+01	10	100	2.29E+03	94%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1316-T03-C	1	1.48E+03			1.48E+03	6.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1316-T04-C	1	1.48E+03			1.48E+03	2.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1316-T05-C	1	1.47E+03			1.47E+03	2.5E-01	6.8E+00	2.2E+01					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	2.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1316-B02-A	1	3.40E+00	U1/2		3.40E+00	1.9E+02	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
Pb	CFS-L09-1316-B03-A	1	3.40E+00	U1/2		3.40E+00	1.2E+02	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	CFS-L09-1316-T01-A	1	9.52E+00			9.52E+00	1.3E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1316-T02-A	1	7.06E+00			7.06E+00	2.8E+01	1.9E+00	6.0E+00	10	100	8.71E+02	86%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1316-T03-A	1	5.11E+00	E		5.11E+00	3.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1316-T04-A	1	6.98E+00			6.98E+00	3.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1316-T05-A	1	1.78E+01			1.78E+01	5.0E+00	1.9E+00	6.0E+00					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1316-T01-B	1	9.52E+00			9.52E+00	4.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1316-T02-B	1	8.93E+00			8.93E+00	2.5E+01	1.9E+00	6.0E+00	10	100	8.70E+02	86%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1316-T03-B	1	6.23E+00			6.23E+00	2.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1316-T04-B	1	5.22E+00	E		5.22E+00	5.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1316-T05-B	1	1.35E+01			1.35E+01	8.0E+00	1.9E+00	6.0E+00					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1316-T01-C	1	1.07E+01			1.07E+01	1.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1316-T02-C	1	6.55E+00			6.55E+00	3.5E+01	1.9E+00	6.0E+00	10	100	8.40E+02	83%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1316-T03-C	1	4.57E+00	E		4.57E+00	3.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1316-T04-C	1	4.64E+00	E		4.64E+00	2.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1316-T05-C	1	1.28E+01			1.28E+01	1.7E+01	1.9E+00	6.0E+00					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	3.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1316-B02-A	1	9.50E-01	U1/2		9.50E-01	8.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
Li	CFS-L09-1316-B03-A	1	9.50E-01	U1/2		9.50E-01	7.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	CFS-L09-1316-T01-A	1	1.57E+03			1.57E+03	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1316-T02-A	1	2.87E+03			2.87E+03	1.0E+00	2.0E+00	6.4E+00	10	100	3.76E+03	89%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1316-T03-A	1	6.00E+03			6.00E+03	2.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1316-T04-A	1	9.56E+03			9.56E+03	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1316-T05-A	1	1.26E+04			1.26E+04	1.0E+00	2.0E+00	6.4E+00					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1316-T01-B	1	1.70E+03			1.70E+03	1.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1316-T02-B	1	2.90E+03			2.90E+03	9.6E-01	2.0E+00	6.4E+00	10	100	3.81E+03	91%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1316-T03-B	1	5.85E+03			5.85E+03	4.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1316-T04-B	1	8.59E+03			8.59E+03	1.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1316-T05-B	1	1.20E+04			1.20E+04	6.9E-01	2.0E+00	6.4E+00					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1316-T01-C	1	1.67E+03			1.67E+03	2.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1316-T02-C	1	2.98E+03			2.98E+03	1.3E+00	2.0E+00	6.4E+00	10	100	3.85E+03	87%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1316-T03-C	1	6.25E+03			6.25E+03	4.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1316-T04-C	1	9.36E+03			9.36E+03	5.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1316-T05-C	1	1.21E+04			1.21E+04	2.0E-01	2.0E+00	6.4E+00					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	3.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1316-B02-A	1	1.00E+00	U1/2		1.00E+00	4.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
Mn	CFS-L09-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	8.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	CFS-L09-1316-T01-A	1	6.57E+04			6.57E+04	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1316-T02-A	1	1.23E+05			1.23E+05	1.2E+00	1.0E+00	3.2E+00	1000	100	1.24E+05	85%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1316-T03-A	1	2.92E+05			2.92E+05	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1316-T04-A	1	5.17E+05			5.17E+05	8.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1316-T05-A	1	8.38E+05			8.38E+05	1.4E+00	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1316-T01-B	1	6.99E+04			6.99E+04	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1316-T02-B	1	1.28E+05			1.28E+05	3.7E-01	1.0E+00	3.2E+00	1000	100	1.29E+05	87%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1316-T03-B	1	2.91E+05			2.91E+05	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1316-T04-B	1	4.82E+05			4.82E+05	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1316-T05-B	1	8.25E+05			8.25E+05	6.0E-01	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1316-T01-C	1	7.22E+04			7.22E+04	6.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1316-T02-C	1	1.32E+05			1.32E+05	8.8E-01	1.0E+00	3.2E+00	1000	100	1.33E+05	92%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1316-T03-C	1	3.03E+05			3.03E+05	9.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1316-T04-C	1	5.13E+05			5.13E+05	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1316-T05-C	1	8.41E+05			8.41E+05	2.4E-01	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.1E+03	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	3.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
Mg	CFS-L09-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	2.1E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	CFS-L09-1316-T01-A	1	1.06E+01			1.06E+01	1.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1316-T02-A	1	1.26E+01			1.26E+01	1.5E+01	1.2E+00	3.8E+00	10	100	1.00E+03	99%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1316-T03-A	1	1.25E+01			1.25E+01	3.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1316-T04-A	1	1.65E+01			1.65E+01	7.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1316-T05-A	1	1.81E+01			1.81E+01	1.0E+01	1.2E+00	3.8E+00					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1316-T01-B	1	8.36E+00			8.36E+00	2.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1316-T02-B	1	1.24E+01			1.24E+01	1.2E+01	1.2E+00	3.8E+00	10	100	1.02E+03	101%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1316-T03-B	1	1.47E+01			1.47E+01	7.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1316-T04-B	1	1.58E+01			1.58E+01	1.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1316-T05-B	1	1.81E+01			1.81E+01	1.7E+00	1.2E+00	3.8E+00					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1316-T01-C	1	9.77E+00			9.77E+00	1.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1316-T02-C	1	1.22E+01			1.22E+01	2.9E+00	1.2E+00	3.8E+00	10	100	1.01E+03	99%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1316-T03-C	1	1.28E+01			1.28E+01	1.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1316-T04-C	1	1.65E+01			1.65E+01	1.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1316-T05-C	1	1.81E+01			1.81E+01	5.1E+00	1.2E+00	3.8E+00					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	1.4E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1316-B02-A	1	2.24E+00	E		2.24E+00	5.6E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
Mo	CFS-L09-1316-B03-A	1	1.46E+00	E		1.46E+00	3.8E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	CFS-L09-1316-T01-A	1	2.15E+02			2.15E+02	1.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1316-T02-A	1	3.29E+02			3.29E+02	1.3E+00	1.8E+00	5.7E+00	10	100	1.30E+03	97%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1316-T03-A	1	5.60E+02			5.60E+02	1.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1316-T04-A	1	7.57E+02			7.57E+02	5.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1316-T05-A	1	9.20E+02			9.20E+02	3.6E-01	1.8E+00	5.7E+00					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1316-T01-B	1	2.16E+02			2.16E+02	1.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1316-T02-B	1	3.31E+02			3.31E+02	1.1E+00	1.8E+00	5.7E+00	10	100	1.31E+03	98%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1316-T03-B	1	5.42E+02			5.42E+02	1.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1316-T04-B	1	6.83E+02			6.83E+02	1.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1316-T05-B	1	8.78E+02			8.78E+02	1.2E-01	1.8E+00	5.7E+00					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1316-T01-C	1	2.14E+02			2.14E+02	1.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1316-T02-C	1	3.46E+02			3.46E+02	4.0E-01	1.8E+00	5.7E+00	10	100	1.32E+03	97%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1316-T03-C	1	5.70E+02			5.70E+02	2.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1316-T04-C	1	7.38E+02			7.38E+02	2.4E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1316-T05-C	1	8.82E+02			8.82E+02	6.1E-01	1.8E+00	5.7E+00					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1316-B02-A	1	9.00E-01	U1/2		9.00E-01	5.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
Ni	CFS-L09-1316-B03-A	1	9.00E-01	U1/2		9.00E-01	5.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	CFS-L09-1316-T01-A	1	7.08E+00	E		7.08E+00	1.5E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1316-T02-A	1	8.40E+00	E		8.40E+00	7.4E+01	3.7E+00	1.2E+01	1000	100	1.04E+03	103%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1316-T03-A	1	2.08E+01			2.08E+01	1.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1316-T04-A	1	2.35E+01			2.35E+01	2.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1316-T05-A	1	2.08E+01			2.08E+01	8.6E+01	3.7E+00	1.2E+01					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1316-T01-B	1	1.29E+01			1.29E+01	6.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1316-T02-B	1	8.29E+00	E		8.29E+00	3.1E+02	3.7E+00	1.2E+01	1000	100	1.07E+03	106%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1316-T03-B	1	1.45E+01			1.45E+01	3.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1316-T04-B	1	2.85E+01			2.85E+01	3.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1316-T05-B	1	3.22E+01			3.22E+01	1.9E+01	3.7E+00	1.2E+01					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1316-T01-C	1	7.09E+00	E		7.09E+00	2.0E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1316-T02-C	1	1.30E+01			1.30E+01	4.4E+01	3.7E+00	1.2E+01	1000	100	1.05E+03	104%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1316-T03-C	1	1.49E+01			1.49E+01	3.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1316-T04-C	1	3.27E+01			3.27E+01	3.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1316-T05-C	1	3.59E+01			3.59E+01	8.2E+00	3.7E+00	1.2E+01					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1316-B01-A	1	1.02E+01	E		1.02E+01	3.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1316-B02-A	1	1.85E+00	U1/2		1.85E+00	1.5E+03	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
P	CFS-L09-1316-B03-A	1	1.18E+01	E		1.18E+01	4.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	CFS-L09-1316-T01-A	1	9.24E+03			9.24E+03	8.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1316-T02-A	1	1.63E+04			1.63E+04	7.7E-01	1.6E+00	5.1E+00	1000	100	1.72E+04	90%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1316-T03-A	1	3.11E+04			3.11E+04	1.6E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1316-T04-A	1	4.93E+04			4.93E+04	6.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1316-T05-A	1	6.80E+04			6.80E+04	2.8E-01	1.6E+00	5.1E+00					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1316-T01-B	1	9.69E+03			9.69E+03	5.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1316-T02-B	1	1.63E+04			1.63E+04	7.6E-01	1.6E+00	5.1E+00	1000	100	1.72E+04	93%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1316-T03-B	1	3.28E+04			3.28E+04	6.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1316-T04-B	1	4.66E+04			4.66E+04	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1316-T05-B	1	6.80E+04			6.80E+04	2.4E-01	1.6E+00	5.1E+00					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1316-T01-C	1	9.70E+03			9.70E+03	4.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1316-T02-C	1	1.67E+04			1.67E+04	4.5E-01	1.6E+00	5.1E+00	1000	100	1.76E+04	89%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1316-T03-C	1	3.27E+04			3.27E+04	9.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1316-T04-C	1	4.88E+04			4.88E+04	2.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1316-T05-C	1	6.94E+04			6.94E+04	3.6E-01	1.6E+00	5.1E+00					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1316-B01-A	1	2.64E+01			2.64E+01	5.5E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1316-B02-A	1	2.59E+01			2.59E+01	9.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
K	CFS-L09-1316-B03-A	1	2.57E+01			2.57E+01	8.6E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	CFS-L09-1316-T01-A	1	7.89E+01			7.89E+01	4.0E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1316-T02-A	1	1.49E+02			1.49E+02	7.8E+00	1.5E+01	4.8E+01	10	100	1.16E+03	101%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1316-T03-A	1	2.79E+02			2.79E+02	4.6E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1316-T04-A	1	4.77E+02			4.77E+02	2.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1316-T05-A	1	7.63E+02			7.63E+02	4.7E-01	1.5E+01	4.8E+01					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1316-T01-B	1	9.58E+01			9.58E+01	1.3E+01	1.5E+01	4.8E+01				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1316-T02-B	1	1.38E+02			1.38E+02	9.3E+00	1.5E+01	4.8E+01	10	100	1.15E+03	101%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1316-T03-B	1	2.82E+02			2.82E+02	6.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1316-T04-B	1	4.38E+02			4.38E+02	3.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1316-T05-B	1	7.62E+02			7.62E+02	9.7E-01	1.5E+01	4.8E+01					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1316-T01-C	1	8.57E+01			8.57E+01	1.7E+01	1.5E+01	4.8E+01				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1316-T02-C	1	1.48E+02			1.48E+02	7.0E+00	1.5E+01	4.8E+01	10	100	1.14E+03	100%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1316-T03-C	1	2.85E+02			2.85E+02	3.0E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1316-T04-C	1	4.82E+02			4.82E+02	4.2E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1316-T05-C	1	7.64E+02			7.64E+02	2.3E+00	1.5E+01	4.8E+01					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1316-B01-A	1	7.50E+00	U1/2		7.50E+00	8.3E+01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1316-B02-A	1	7.50E+00	U1/2		7.50E+00	9.5E+01	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
Se	CFS-L09-1316-B03-A	1	7.50E+00	U1/2		7.50E+00	1.1E+02	1.5E+01	4.8E+01				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	CFS-L09-1316-T01-A	1	3.58E+03			3.58E+03	2.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1316-T02-A	1	4.62E+03			4.62E+03	1.6E+00	1.1E+00	3.5E+00	1000	100	5.58E+03	97%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1316-T03-A	1	5.78E+03			5.78E+03	1.5E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1316-T04-A	1	6.29E+03			6.29E+03	5.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1316-T05-A	1	6.37E+03			6.37E+03	3.6E-01	1.1E+00	3.5E+00					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1316-T01-B	1	3.74E+03			3.74E+03	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1316-T02-B	1	4.73E+03			4.73E+03	1.4E+00	1.1E+00	3.5E+00	1000	100	5.61E+03	88%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1316-T03-B	1	5.89E+03			5.89E+03	6.0E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1316-T04-B	1	6.10E+03			6.10E+03	6.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1316-T05-B	1	6.43E+03			6.43E+03	1.6E-01	1.1E+00	3.5E+00					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1316-T01-C	1	3.58E+03			3.58E+03	4.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1316-T02-C	1	4.90E+03			4.90E+03	9.9E-01	1.1E+00	3.5E+00	1000	100	5.75E+03	85%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1316-T03-C	1	6.09E+03			6.09E+03	2.5E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1316-T04-C	1	6.26E+03			6.26E+03	2.9E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1316-T05-C	1	6.48E+03			6.48E+03	2.1E-01	1.1E+00	3.5E+00					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1316-B01-A	1	5.50E-01	U1/2		5.50E-01	3.1E+01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1316-B02-A	1	5.50E-01	U1/2		5.50E-01	7.6E+01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
Si	CFS-L09-1316-B03-A	1	5.50E-01	U1/2		5.50E-01	2.7E+01	1.1E+00	3.5E+00				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	CFS-L09-1316-T01-A	1	9.40E+03			9.40E+03	2.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1316-T02-A	1	1.79E+04			1.79E+04	9.0E-01	2.5E+00	8.0E+00	1000	100	1.88E+04	88%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1316-T03-A	1	4.20E+04			4.20E+04	7.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1316-T04-A	1	7.35E+04			7.35E+04	6.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1316-T05-A	1	1.09E+05			1.09E+05	2.1E-01	2.5E+00	8.0E+00					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1316-T01-B	1	1.00E+04			1.00E+04	5.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1316-T02-B	1	1.78E+04			1.78E+04	4.5E-01	2.5E+00	8.0E+00	1000	100	1.87E+04	93%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1316-T03-B	1	4.17E+04			4.17E+04	5.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1316-T04-B	1	7.00E+04			7.00E+04	2.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1316-T05-B	1	1.09E+05			1.09E+05	5.9E-01	2.5E+00	8.0E+00					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1316-T01-C	1	9.86E+03			9.86E+03	4.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1316-T02-C	1	1.83E+04			1.83E+04	2.2E-01	2.5E+00	8.0E+00	1000	100	1.92E+04	91%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1316-T03-C	1	4.28E+04			4.28E+04	8.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1316-T04-C	1	7.41E+04			7.41E+04	4.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1316-T05-C	1	1.11E+05			1.11E+05	1.3E-01	2.5E+00	8.0E+00					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1316-B01-A	1	2.09E+01			2.09E+01	1.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1316-B02-A	1	2.11E+01			2.11E+01	1.7E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
Na	CFS-L09-1316-B03-A	1	2.11E+01			2.11E+01	1.6E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	CFS-L09-1316-T01-A	1	1.52E+03			1.52E+03	1.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1316-T02-A	1	2.13E+03			2.13E+03	1.4E+00	1.0E+00	3.2E+00	1000	100	3.08E+03	95%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1316-T03-A	1	3.13E+03			3.13E+03	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1316-T04-A	1	3.85E+03			3.85E+03	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1316-T05-A	1	4.25E+03			4.25E+03	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1316-T01-B	1	1.55E+03			1.55E+03	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1316-T02-B	1	2.20E+03			2.20E+03	7.1E-01	1.0E+00	3.2E+00	1000	100	3.09E+03	89%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1316-T03-B	1	3.28E+03			3.28E+03	8.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1316-T04-B	1	3.94E+03			3.94E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1316-T05-B	1	4.30E+03			4.30E+03	4.9E-01	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1316-T01-C	1	1.52E+03			1.52E+03	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1316-T02-C	1	2.13E+03			2.13E+03	6.1E-01	1.0E+00	3.2E+00	1000	100	3.02E+03	90%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1316-T03-C	1	3.29E+03			3.29E+03	2.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1316-T04-C	1	3.90E+03			3.90E+03	8.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1316-T05-C	1	4.40E+03			4.40E+03	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.2E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	1.7E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
Sr	CFS-L09-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	7.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	CFS-L09-1316-T01-A	1	6.06E+05			6.06E+05	1.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1316-T02-A	1	6.71E+05			6.71E+05	6.3E-01	6.8E+00	2.2E+01	1000	100	6.72E+05	83%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1316-T03-A	1	8.53E+05			8.53E+05	1.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1316-T04-A	1	1.11E+06			1.11E+06	3.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1316-T05-A	1	1.40E+06			1.40E+06	4.1E-01	6.8E+00	2.2E+01					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1316-T01-B	1	6.16E+05			6.16E+05	3.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1316-T02-B	1	6.78E+05			6.78E+05	8.8E-01	6.8E+00	2.2E+01	1000	100	6.78E+05	86%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1316-T03-B	1	8.65E+05			8.65E+05	4.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1316-T04-B	1	1.06E+06			1.06E+06	9.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1316-T05-B	1	1.39E+06			1.39E+06	2.9E-01	6.8E+00	2.2E+01					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1316-T01-C	1	6.07E+05			6.07E+05	7.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1316-T02-C	1	6.82E+05			6.82E+05	5.7E-01	6.8E+00	2.2E+01	1000	100	6.83E+05	84%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1316-T03-C	1	8.64E+05			8.64E+05	3.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1316-T04-C	1	1.08E+06			1.08E+06	2.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1316-T05-C	1	1.41E+06			1.41E+06	2.6E-01	6.8E+00	2.2E+01					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	3.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1316-B02-A	1	3.40E+00	U1/2		3.40E+00	3.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
S	CFS-L09-1316-B03-A	1	3.40E+00	U1/2		3.40E+00	4.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	CFS-L09-1316-T01-A	1	3.08E+02			3.08E+02	2.6E+00	4.6E+00	1.5E+01				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
Tl	CFS-L09-1316-T02-A	1	4.66E+02			4.66E+02	2.0E-01	4.6E+00	1.5E+01	10	100	1.38E+03	91%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
Tl	CFS-L09-1316-T03-A	1	7.37E+02			7.37E+02	2.4E+00	4.6E+00	1.5E+01				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
Tl	CFS-L09-1316-T04-A	1	1.01E+03			1.01E+03	4.1E-01	4.6E+00	1.5E+01				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
Tl	CFS-L09-1316-T05-A	1	1.27E+03			1.27E+03	2.3E-01	4.6E+00	1.5E+01					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
Tl	CFS-L09-1316-T01-B	1	3.29E+02			3.29E+02	3.7E-01	4.6E+00	1.5E+01				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
Tl	CFS-L09-1316-T02-B	1	4.73E+02			4.73E+02	2.4E-01	4.6E+00	1.5E+01	10	100	1.40E+03	93%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
Tl	CFS-L09-1316-T03-B	1	7.52E+02			7.52E+02	2.7E-01	4.6E+00	1.5E+01				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
Tl	CFS-L09-1316-T04-B	1	9.62E+02			9.62E+02	3.4E-01	4.6E+00	1.5E+01				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
Tl	CFS-L09-1316-T05-B	1	1.26E+03			1.26E+03	6.0E-01	4.6E+00	1.5E+01					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
Tl	CFS-L09-1316-T01-C	1	3.29E+02			3.29E+02	9.2E-01	4.6E+00	1.5E+01				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
Tl	CFS-L09-1316-T02-C	1	4.76E+02			4.76E+02	1.1E+00	4.6E+00	1.5E+01	10	100	1.40E+03	92%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
Tl	CFS-L09-1316-T03-C	1	7.71E+02			7.71E+02	1.3E+00	4.6E+00	1.5E+01				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
Tl	CFS-L09-1316-T04-C	1	9.99E+02			9.99E+02	3.0E-01	4.6E+00	1.5E+01				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
Tl	CFS-L09-1316-T05-C	1	1.27E+03			1.27E+03	4.7E-01	4.6E+00	1.5E+01					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
Tl	CFS-L09-1316-B01-A	1	2.30E+00	U1/2		2.30E+00	7.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
Tl	CFS-L09-1316-B02-A	1	2.30E+00	U1/2		2.30E+00	8.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
Tl	CFS-L09-1316-B03-A	1	2.30E+00	U1/2		2.30E+00	1.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	CFS-L09-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	5.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	9.6E+01	2.0E+00	6.4E+00	10	100	1.03E+03	103%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	8.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	4.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1316-T05-A	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	8.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	5.5E+01	2.0E+00	6.4E+00	10	100	1.04E+03	104%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	1.4E+02	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1316-T05-B	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	7.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	6.1E+01	2.0E+00	6.4E+00	10	100	1.03E+03	103%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	5.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	2.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1316-T05-C	1	1.00E+00	U1/2		1.00E+00	4.0E+01	2.0E+00	6.4E+00					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	6.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1316-B02-A	1	1.00E+00	U1/2		1.00E+00	5.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
Ti	CFS-L09-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	7.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	CFS-L09-1316-T01-A	1	2.46E+01			2.46E+01	5.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1316-T02-A	1	2.52E+01			2.52E+01	1.9E+00	1.5E+00	4.8E+00	10	100	1.02E+03	100%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1316-T03-A	1	2.23E+01			2.23E+01	2.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1316-T04-A	1	2.12E+01			2.12E+01	3.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1316-T05-A	1	1.99E+01			1.99E+01	3.5E+00	1.5E+00	4.8E+00					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1316-T01-B	1	2.53E+01			2.53E+01	2.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1316-T02-B	1	2.46E+01			2.46E+01	3.5E+00	1.5E+00	4.8E+00	10	100	1.03E+03	101%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1316-T03-B	1	2.28E+01			2.28E+01	2.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1316-T04-B	1	2.21E+01			2.21E+01	6.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1316-T05-B	1	1.84E+01			1.84E+01	4.5E+00	1.5E+00	4.8E+00					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1316-T01-C	1	2.48E+01			2.48E+01	1.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1316-T02-C	1	2.45E+01			2.45E+01	2.6E+00	1.5E+00	4.8E+00	10	100	1.02E+03	99%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1316-T03-C	1	2.26E+01			2.26E+01	6.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1316-T04-C	1	2.15E+01			2.15E+01	5.9E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1316-T05-C	1	1.96E+01			1.96E+01	2.8E+00	1.5E+00	4.8E+00					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1316-B01-A	1	1.60E+00	E		1.60E+00	2.6E+01	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1316-B02-A	1	7.50E-01	U1/2		7.50E-01	2.1E+01	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
V	CFS-L09-1316-B03-A	1	7.50E-01	U1/2		7.50E-01	5.1E+01	1.5E+00	4.8E+00				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	CFS-L09-1316-T01-A	1	2.04E+04			2.04E+04	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:00 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1316-T02-A	1	2.80E+04			2.80E+04	1.6E+00	1.0E+00	3.2E+00	10	100	2.88E+04	88%	VU ICP-OES	4/19/11 5:02 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1316-T03-A	1	4.17E+04			4.17E+04	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:04 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1316-T04-A	1	5.35E+04			5.35E+04	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:05 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1316-T05-A	1	6.17E+04			6.17E+04	1.6E+00	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 5:07 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1316-T01-B	1	2.05E+04			2.05E+04	8.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:08 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1316-T02-B	1	2.74E+04			2.74E+04	7.6E-01	1.0E+00	3.2E+00	10	100	2.83E+04	96%	VU ICP-OES	4/19/11 5:10 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1316-T03-B	1	4.01E+04			4.01E+04	2.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:12 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1316-T04-B	1	4.82E+04			4.82E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:13 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1316-T05-B	1	5.95E+04			5.95E+04	6.3E-01	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 5:15 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1316-T01-C	1	2.04E+04			2.04E+04	3.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:17 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1316-T02-C	1	2.90E+04			2.90E+04	1.4E+00	1.0E+00	3.2E+00	10	100	2.99E+04	89%	VU ICP-OES	4/19/11 5:18 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1316-T03-C	1	4.22E+04			4.22E+04	1.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:20 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1316-T04-C	1	5.25E+04			5.25E+04	2.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/19/11 5:22 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1316-T05-C	1	5.94E+04			5.94E+04	4.0E-01	1.0E+00	3.2E+00					VU ICP-OES	4/19/11 5:23 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1316-B01-A	1	4.21E+00			4.21E+00	7.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 2:33 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1316-B02-A	1	3.15E+00	E		3.15E+00	1.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 2:35 PM	EPA Interlab L09 1313-1316 CFS
Zn	CFS-L09-1316-B03-A	1	3.04E+00	E		3.04E+00	7.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/20/11 2:36 PM	EPA Interlab L09 1313-1316 CFS

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	CFS-L10-1316-T01-A	1	4.71E+01			4.71E+01	4.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1316-T02-A	1	4.72E+01			4.72E+01	1.9E+00	1.0E+00	3.2E+00	1000	100	1.22E+03	117%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1316-T03-A	1	4.89E+01			4.89E+01	6.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1316-T04-A	1	5.06E+01			5.06E+01	7.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1316-T05-A	1	5.15E+01			5.15E+01	4.9E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1316-T01-B	1	4.78E+01			4.78E+01	3.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1316-T02-B	1	4.58E+01			4.58E+01	7.8E+00	1.0E+00	3.2E+00	1000	100	1.05E+03	100%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1316-T03-B	1	5.01E+01			5.01E+01	9.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1316-T04-B	1	5.11E+01			5.11E+01	4.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1316-T05-B	1	6.08E+01			6.08E+01	4.8E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1316-T01-C	1	5.00E+01			5.00E+01	8.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1316-T02-C	1	5.11E+01			5.11E+01	5.0E+00	1.0E+00	3.2E+00	1000	100	1.19E+03	114%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1316-T03-C	1	5.74E+01			5.74E+01	6.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1316-T04-C	1	5.43E+01			5.43E+01	6.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1316-T05-C	1	5.85E+01			5.85E+01	1.1E+01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.5E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	5.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
Al	CFS-L10-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	1.6E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	CFS-L10-1316-T01-A	1	3.28E+01			3.28E+01	9.4E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1316-T02-A	1	4.32E+01			4.32E+01	1.6E+01	7.5E+00	2.4E+01	10	100	1.15E+03	110%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1316-T03-A	1	3.44E+01			3.44E+01	7.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1316-T04-A	1	5.15E+01			5.15E+01	7.0E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1316-T05-A	1	6.64E+01			6.64E+01	1.4E+00	7.5E+00	2.4E+01					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1316-T01-B	1	2.95E+01			2.95E+01	3.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1316-T02-B	1	3.04E+01			3.04E+01	3.4E+01	7.5E+00	2.4E+01	10	100	9.99E+02	97%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1316-T03-B	1	3.38E+01			3.38E+01	1.9E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1316-T04-B	1	5.09E+01			5.09E+01	5.6E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1316-T05-B	1	5.66E+01			5.66E+01	1.8E+01	7.5E+00	2.4E+01					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1316-T01-C	1	3.01E+01			3.01E+01	8.9E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1316-T02-C	1	3.25E+01			3.25E+01	1.5E+01	7.5E+00	2.4E+01	10	100	1.09E+03	105%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1316-T03-C	1	3.80E+01			3.80E+01	7.1E+00	7.5E+00	2.4E+01				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1316-T04-C	1	4.91E+01			4.91E+01	1.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1316-T05-C	1	5.41E+01			5.41E+01	8.1E+00	7.5E+00	2.4E+01					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1316-B01-A	1	3.75E+00	U1/2		3.75E+00	1.6E+02	7.5E+00	2.4E+01				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1316-B02-A	1	3.75E+00	U1/2		3.75E+00	2.7E+03	7.5E+00	2.4E+01				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
Sb	CFS-L10-1316-B03-A	1	3.75E+00	U1/2		3.75E+00	3.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	CFS-L10-1316-T01-A	1	1.94E+01	E		1.94E+01	1.8E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1316-T02-A	1	1.17E+01	E		1.17E+01	6.7E+01	1.1E+01	3.5E+01	10	100	1.14E+03	113%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1316-T03-A	1	1.92E+01	E		1.92E+01	4.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1316-T04-A	1	3.51E+01			3.51E+01	3.1E-01	1.1E+01	3.5E+01				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1316-T05-A	1	4.22E+01			4.22E+01	2.7E+01	1.1E+01	3.5E+01					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1316-T01-B	1	1.54E+01	E		1.54E+01	4.7E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1316-T02-B	1	1.49E+01	E		1.49E+01	4.6E+01	1.1E+01	3.5E+01	10	100	1.00E+03	99%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1316-T03-B	1	2.78E+01	E		2.78E+01	5.5E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1316-T04-B	1	2.96E+01	E		2.96E+01	2.5E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1316-T05-B	1	4.12E+01			4.12E+01	5.9E+00	1.1E+01	3.5E+01					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1316-T01-C	1	1.63E+01	E		1.63E+01	5.2E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1316-T02-C	1	1.49E+01	E		1.49E+01	2.0E+01	1.1E+01	3.5E+01	10	100	1.09E+03	108%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1316-T03-C	1	2.47E+01	E		2.47E+01	5.6E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1316-T04-C	1	3.30E+01	E		3.30E+01	4.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1316-T05-C	1	3.84E+01			3.84E+01	1.7E+01	1.1E+01	3.5E+01					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1316-B01-A	1	5.50E+00	U1/2		5.50E+00	5.8E+01	1.1E+01	3.5E+01				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1316-B02-A	1	5.50E+00	U1/2		5.50E+00	2.4E+02	1.1E+01	3.5E+01				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
As	CFS-L10-1316-B03-A	1	5.50E+00	U1/2		5.50E+00	1.1E+02	1.1E+01	3.5E+01				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	CFS-L10-1316-T01-A	1	1.53E+02			1.53E+02	9.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1316-T02-A	1	2.62E+02			2.62E+02	1.7E+00	1.0E+00	3.2E+00	1000	100	1.22E+03	95%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1316-T03-A	1	5.35E+02			5.35E+02	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1316-T04-A	1	8.64E+02			8.64E+02	8.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1316-T05-A	1	1.33E+03			1.33E+03	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1316-T01-B	1	1.68E+02			1.68E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1316-T02-B	1	2.79E+02			2.79E+02	8.0E-01	1.0E+00	3.2E+00	1000	100	1.21E+03	93%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1316-T03-B	1	5.43E+02			5.43E+02	7.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1316-T04-B	1	8.86E+02			8.86E+02	7.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1316-T05-B	1	1.30E+03			1.30E+03	6.2E-01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1316-T01-C	1	1.64E+02			1.64E+02	2.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1316-T02-C	1	2.66E+02			2.66E+02	9.4E-01	1.0E+00	3.2E+00	1000	100	1.19E+03	93%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1316-T03-C	1	5.23E+02			5.23E+02	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1316-T04-C	1	8.61E+02			8.61E+02	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1316-T05-C	1	1.31E+03			1.31E+03	7.0E-01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1316-B01-A	1	1.35E+01			1.35E+01	9.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1316-B02-A	1	1.10E+01			1.10E+01	1.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
B	CFS-L10-1316-B03-A	1	9.79E+00			9.79E+00	1.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	CFS-L10-1316-T01-A	1	1.06E+02			1.06E+02	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1316-T02-A	1	9.52E+01			9.52E+01	9.4E-01	1.0E+00	3.2E+00	10	100	1.14E+03	105%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1316-T03-A	1	8.14E+01			8.14E+01	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1316-T04-A	1	6.96E+01			6.96E+01	4.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1316-T05-A	1	6.38E+01			6.38E+01	4.7E-01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1316-T01-B	1	1.07E+02			1.07E+02	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1316-T02-B	1	9.15E+01			9.15E+01	1.4E+00	1.0E+00	3.2E+00	10	100	1.14E+03	105%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1316-T03-B	1	7.63E+01			7.63E+01	9.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1316-T04-B	1	6.33E+01			6.33E+01	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1316-T05-B	1	5.31E+01			5.31E+01	8.6E-01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1316-T01-C	1	9.47E+01			9.47E+01	2.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1316-T02-C	1	9.06E+01			9.06E+01	7.2E-01	1.0E+00	3.2E+00	10	100	1.07E+03	98%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1316-T03-C	1	7.70E+01			7.70E+01	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1316-T04-C	1	6.32E+01			6.32E+01	6.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1316-T05-C	1	5.25E+01			5.25E+01	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	2.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	1.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
Ba	CFS-L10-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	1.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	CFS-L10-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	1.4E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	2.0E+02	1.9E+00	6.0E+00	10	100	1.16E+03	116%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	2.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	6.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1316-T05-A	1	9.50E-01	U1/2		9.50E-01	2.7E+01	1.9E+00	6.0E+00					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	4.2E+03	1.9E+00	6.0E+00				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00	10	100	1.01E+03	101%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	4.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	9.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1316-T05-B	1	9.50E-01	U1/2		9.50E-01	2.9E+01	1.9E+00	6.0E+00					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	3.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	4.9E+01	1.9E+00	6.0E+00	10	100	1.10E+03	110%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	2.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	6.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1316-T05-C	1	9.50E-01	U1/2		9.50E-01	2.9E+01	1.9E+00	6.0E+00					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	2.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1316-B02-A	1	9.50E-01	U1/2		9.50E-01	1.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
Be	CFS-L10-1316-B03-A	1	9.50E-01	U1/2		9.50E-01	2.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	CFS-L10-1316-T01-A	1	4.16E+03			4.16E+03	4.6E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1316-T02-A	1	5.90E+03			5.90E+03	1.3E+00	2.2E+00	7.0E+00	10	100	6.89E+03	99%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1316-T03-A	1	8.88E+03			8.88E+03	6.4E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1316-T04-A	1	1.11E+04			1.11E+04	9.0E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1316-T05-A	1	1.28E+04			1.28E+04	8.3E-01	2.2E+00	7.0E+00					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1316-T01-B	1	4.37E+03			4.37E+03	3.6E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1316-T02-B	1	6.45E+03			6.45E+03	9.9E-01	2.2E+00	7.0E+00	10	100	7.39E+03	95%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1316-T03-B	1	9.24E+03			9.24E+03	2.8E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1316-T04-B	1	1.16E+04			1.16E+04	8.6E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1316-T05-B	1	1.37E+04			1.37E+04	2.8E-01	2.2E+00	7.0E+00					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1316-T01-C	1	4.26E+03			4.26E+03	8.2E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1316-T02-C	1	5.88E+03			5.88E+03	2.0E-01	2.2E+00	7.0E+00	10	100	6.85E+03	96%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1316-T03-C	1	8.64E+03			8.64E+03	8.8E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1316-T04-C	1	1.15E+04			1.15E+04	3.6E-01	2.2E+00	7.0E+00				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1316-T05-C	1	1.36E+04			1.36E+04	8.5E-01	2.2E+00	7.0E+00					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1316-B01-A	1	1.10E+00	U1/2		1.10E+00	1.4E+01	2.2E+00	7.0E+00				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1316-B02-A	1	1.10E+00	U1/2		1.10E+00	1.4E+02	2.2E+00	7.0E+00				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
Cd	CFS-L10-1316-B03-A	1	1.10E+00	U1/2		1.10E+00	3.8E+00	2.2E+00	7.0E+00				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	CFS-L10-1316-T01-A	1	6.53E+05			6.53E+05	4.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1316-T02-A	1	6.23E+05			6.23E+05	1.3E+00	2.6E+00	8.3E+00	1000	100	6.24E+05	91%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1316-T03-A	1	5.91E+05			5.91E+05	1.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1316-T04-A	1	5.69E+05			5.69E+05	8.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1316-T05-A	1	5.46E+05			5.46E+05	1.0E+00	2.6E+00	8.3E+00					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1316-T01-B	1	6.68E+05			6.68E+05	5.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1316-T02-B	1	6.21E+05			6.21E+05	8.3E-01	2.6E+00	8.3E+00	1000	100	6.22E+05	85%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1316-T03-B	1	5.66E+05			5.66E+05	1.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1316-T04-B	1	5.27E+05			5.27E+05	9.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1316-T05-B	1	5.03E+05			5.03E+05	4.9E-01	2.6E+00	8.3E+00					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1316-T01-C	1	6.10E+05			6.10E+05	9.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1316-T02-C	1	5.94E+05			5.94E+05	8.6E-01	2.6E+00	8.3E+00	1000	100	5.95E+05	89%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1316-T03-C	1	5.56E+05			5.56E+05	8.4E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1316-T04-C	1	5.26E+05			5.26E+05	7.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1316-T05-C	1	4.99E+05			4.99E+05	1.4E+00	2.6E+00	8.3E+00					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1316-B01-A	1	2.04E+01			2.04E+01	1.3E+01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1316-B02-A	1	2.10E+01			2.10E+01	1.9E+01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
Ca	CFS-L10-1316-B03-A	1	1.63E+01			1.63E+01	2.3E+01	2.6E+00	8.3E+00				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	CFS-L10-1316-T01-A	1	6.00E-01	U1/2		6.00E-01	1.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1316-T02-A	1	6.00E-01	U1/2		6.00E-01	1.2E+02	1.2E+00	3.8E+00	10	100	1.13E+03	113%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1316-T03-A	1	6.00E-01	U1/2		6.00E-01	2.3E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1316-T04-A	1	6.00E-01	U1/2		6.00E-01	6.9E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1316-T05-A	1	6.00E-01	U1/2		6.00E-01	2.6E+02	1.2E+00	3.8E+00					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1316-T01-B	1	6.00E-01	U1/2		6.00E-01	2.4E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1316-T02-B	1	6.00E-01	U1/2		6.00E-01	3.4E+02	1.2E+00	3.8E+00	10	100	9.73E+02	97%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1316-T03-B	1	6.00E-01	U1/2		6.00E-01	4.5E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1316-T04-B	1	6.00E-01	U1/2		6.00E-01	1.2E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1316-T05-B	1	6.00E-01	U1/2		6.00E-01	9.8E+01	1.2E+00	3.8E+00					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1316-T01-C	1	6.00E-01	U1/2		6.00E-01	6.5E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1316-T02-C	1	6.00E-01	U1/2		6.00E-01	1.6E+01	1.2E+00	3.8E+00	10	100	1.09E+03	109%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1316-T03-C	1	6.00E-01	U1/2		6.00E-01	8.8E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1316-T04-C	1	6.00E-01	U1/2		6.00E-01	2.2E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1316-T05-C	1	6.00E-01	U1/2		6.00E-01	8.4E+01	1.2E+00	3.8E+00					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	3.7E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	1.9E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
Cr	CFS-L10-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	1.6E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	CFS-L10-1316-T01-A	1	9.21E+01			9.21E+01	2.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1316-T02-A	1	1.54E+02			1.54E+02	1.9E+00	1.8E+00	5.7E+00	10	100	1.08E+03	93%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1316-T03-A	1	2.86E+02			2.86E+02	1.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1316-T04-A	1	4.00E+02			4.00E+02	1.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1316-T05-A	1	4.86E+02			4.86E+02	7.3E-01	1.8E+00	5.7E+00					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1316-T01-B	1	9.89E+01			9.89E+01	7.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1316-T02-B	1	1.73E+02			1.73E+02	1.3E+00	1.8E+00	5.7E+00	10	100	1.11E+03	94%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1316-T03-B	1	3.12E+02			3.12E+02	6.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1316-T04-B	1	4.46E+02			4.46E+02	7.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1316-T05-B	1	5.71E+02			5.71E+02	7.7E-01	1.8E+00	5.7E+00					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1316-T01-C	1	1.00E+02			1.00E+02	1.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1316-T02-C	1	1.63E+02			1.63E+02	7.4E-01	1.8E+00	5.7E+00	10	100	1.03E+03	87%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1316-T03-C	1	3.01E+02			3.01E+02	1.5E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1316-T04-C	1	4.44E+02			4.44E+02	5.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1316-T05-C	1	5.71E+02			5.71E+02	8.7E-01	1.8E+00	5.7E+00					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	2.1E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1316-B02-A	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
Co	CFS-L10-1316-B03-A	1	9.00E-01	U1/2		9.00E-01	4.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	CFS-L10-1316-T01-A	1	7.45E+02			7.45E+02	9.5E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1316-T02-A	1	1.06E+03			1.06E+03	1.1E+00	3.7E+00	1.2E+01	10	100	2.02E+03	96%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1316-T03-A	1	1.68E+03			1.68E+03	1.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1316-T04-A	1	2.20E+03			2.20E+03	7.3E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1316-T05-A	1	2.32E+03			2.32E+03	4.0E-01	3.7E+00	1.2E+01					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1316-T01-B	1	8.36E+02			8.36E+02	5.9E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1316-T02-B	1	1.20E+03			1.20E+03	1.9E+00	3.7E+00	1.2E+01	10	100	2.05E+03	85%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1316-T03-B	1	1.97E+03			1.97E+03	1.4E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1316-T04-B	1	2.22E+03			2.22E+03	7.1E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1316-T05-B	1	2.75E+03			2.75E+03	7.4E-01	3.7E+00	1.2E+01					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1316-T01-C	1	8.73E+02			8.73E+02	3.9E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1316-T02-C	1	1.08E+03			1.08E+03	5.9E-01	3.7E+00	1.2E+01	10	100	2.06E+03	97%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1316-T03-C	1	1.54E+03			1.54E+03	6.5E-01	3.7E+00	1.2E+01				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1316-T04-C	1	2.29E+03			2.29E+03	1.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1316-T05-C	1	2.64E+03			2.64E+03	7.1E-01	3.7E+00	1.2E+01					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	2.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1316-B02-A	1	1.85E+00	U1/2		1.85E+00	4.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
Cu	CFS-L10-1316-B03-A	1	1.85E+00	U1/2		1.85E+00	3.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	CFS-L10-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	9.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	4.7E+00	2.0E+00	6.4E+00	1000	100	1.15E+03	115%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	4.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	7.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1316-T05-A	1	1.00E+00	U1/2		1.00E+00	5.4E+00	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	4.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	3.4E+00	2.0E+00	6.4E+00	1000	100	1.05E+03	105%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	4.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1316-T05-B	1	1.00E+00	U1/2		1.00E+00	9.3E+01	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	4.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	5.8E+01	2.0E+00	6.4E+00	1000	100	1.10E+03	110%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	2.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	4.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1316-T05-C	1	1.00E+00	U1/2		1.00E+00	6.5E+00	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1316-B02-A	1	1.00E+00	U1/2		1.00E+00	5.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
Fe	CFS-L10-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	2.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	CFS-L10-1316-T01-A	1	8.61E+02			8.61E+02	7.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1316-T02-A	1	9.16E+02			9.16E+02	1.4E+00	6.8E+00	2.2E+01	10	100	1.85E+03	93%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1316-T03-A	1	1.01E+03			1.01E+03	8.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1316-T04-A	1	1.12E+03			1.12E+03	9.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1316-T05-A	1	1.34E+03			1.34E+03	1.3E+00	6.8E+00	2.2E+01					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1316-T01-B	1	8.95E+02			8.95E+02	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1316-T02-B	1	9.41E+02			9.41E+02	1.0E+00	6.8E+00	2.2E+01	10	100	1.83E+03	89%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1316-T03-B	1	1.03E+03			1.03E+03	5.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1316-T04-B	1	1.09E+03			1.09E+03	1.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1316-T05-B	1	1.27E+03			1.27E+03	1.1E+00	6.8E+00	2.2E+01					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1316-T01-C	1	8.26E+02			8.26E+02	6.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1316-T02-C	1	9.14E+02			9.14E+02	6.8E-01	6.8E+00	2.2E+01	10	100	1.90E+03	98%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1316-T03-C	1	1.02E+03			1.02E+03	1.3E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1316-T04-C	1	1.12E+03			1.12E+03	1.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1316-T05-C	1	1.24E+03			1.24E+03	2.8E-01	6.8E+00	2.2E+01					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	1.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1316-B02-A	1	3.40E+00	U1/2		3.40E+00	4.3E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
Pb	CFS-L10-1316-B03-A	1	3.40E+00	U1/2		3.40E+00	1.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	CFS-L10-1316-T01-A	1	1.06E+01			1.06E+01	1.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1316-T02-A	1	5.14E+00	E		5.14E+00	2.4E+00	1.9E+00	6.0E+00	10	100	8.84E+02	88%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1316-T03-A	1	5.32E+00	E		5.32E+00	1.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1316-T04-A	1	5.57E+00	E		5.57E+00	5.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1316-T05-A	1	1.66E+01			1.66E+01	3.8E+00	1.9E+00	6.0E+00					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1316-T01-B	1	8.28E+00			8.28E+00	1.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1316-T02-B	1	8.49E+00			8.49E+00	2.5E+00	1.9E+00	6.0E+00	10	100	8.62E+02	85%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1316-T03-B	1	5.29E+00	E		5.29E+00	2.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1316-T04-B	1	7.68E+00			7.68E+00	4.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1316-T05-B	1	1.94E+01			1.94E+01	6.8E+00	1.9E+00	6.0E+00					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1316-T01-C	1	1.21E+01			1.21E+01	4.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1316-T02-C	1	7.77E+00			7.77E+00	2.2E+00	1.9E+00	6.0E+00	10	100	8.42E+02	83%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1316-T03-C	1	5.38E+00	E		5.38E+00	2.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1316-T04-C	1	6.35E+00			6.35E+00	1.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1316-T05-C	1	1.85E+01			1.85E+01	6.7E+00	1.9E+00	6.0E+00					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	3.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1316-B02-A	1	9.50E-01	U1/2		9.50E-01	3.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
Li	CFS-L10-1316-B03-A	1	1.99E+00	E		1.99E+00	3.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	CFS-L10-1316-T01-A	1	1.46E+03			1.46E+03	8.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1316-T02-A	1	2.62E+03			2.62E+03	1.6E+00	2.0E+00	6.4E+00	10	100	3.63E+03	101%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1316-T03-A	1	5.50E+03			5.50E+03	1.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1316-T04-A	1	8.35E+03			8.35E+03	1.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1316-T05-A	1	1.15E+04			1.15E+04	6.4E-01	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1316-T01-B	1	1.59E+03			1.59E+03	7.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1316-T02-B	1	2.92E+03			2.92E+03	1.4E+00	2.0E+00	6.4E+00	10	100	3.92E+03	100%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1316-T03-B	1	5.81E+03			5.81E+03	1.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1316-T04-B	1	8.98E+03			8.98E+03	7.4E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1316-T05-B	1	1.28E+04			1.28E+04	6.3E-01	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1316-T01-C	1	1.56E+03			1.56E+03	2.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1316-T02-C	1	2.77E+03			2.77E+03	6.2E-01	2.0E+00	6.4E+00	10	100	3.80E+03	104%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1316-T03-C	1	5.53E+03			5.53E+03	1.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1316-T04-C	1	8.75E+03			8.75E+03	5.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1316-T05-C	1	1.27E+04			1.27E+04	1.4E+00	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	6.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1316-B02-A	1	1.00E+00	U1/2		1.00E+00	4.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
Mn	CFS-L10-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	4.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	CFS-L10-1316-T01-A	1	6.47E+04			6.47E+04	7.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1316-T02-A	1	1.22E+05			1.22E+05	1.1E+00	1.0E+00	3.2E+00	1000	100	1.23E+05	91%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1316-T03-A	1	2.75E+05			2.75E+05	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1316-T04-A	1	5.10E+05			5.10E+05	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1316-T05-A	1	9.00E+05			9.00E+05	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1316-T01-B	1	6.79E+04			6.79E+04	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1316-T02-B	1	1.26E+05			1.26E+05	6.7E-01	1.0E+00	3.2E+00	1000	100	1.26E+05	87%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1316-T03-B	1	2.79E+05			2.79E+05	6.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1316-T04-B	1	5.02E+05			5.02E+05	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1316-T05-B	1	8.78E+05			8.78E+05	1.0E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1316-T01-C	1	6.14E+04			6.14E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1316-T02-C	1	1.22E+05			1.22E+05	5.2E-01	1.0E+00	3.2E+00	1000	100	1.22E+05	91%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1316-T03-C	1	2.67E+05			2.67E+05	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1316-T04-C	1	4.81E+05			4.81E+05	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1316-T05-C	1	8.72E+05			8.72E+05	8.5E-01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	3.7E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	2.0E+03	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
Mg	CFS-L10-1316-B03-A	1	1.83E+00	E		1.83E+00	7.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	CFS-L10-1316-T01-A	1	9.48E+00			9.48E+00	1.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1316-T02-A	1	9.38E+00			9.38E+00	7.4E+00	1.2E+00	3.8E+00	10	100	1.07E+03	106%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1316-T03-A	1	1.33E+01			1.33E+01	5.2E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1316-T04-A	1	1.37E+01			1.37E+01	1.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1316-T05-A	1	2.09E+01			2.09E+01	3.0E+00	1.2E+00	3.8E+00					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1316-T01-B	1	7.62E+00			7.62E+00	7.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1316-T02-B	1	8.17E+00			8.17E+00	1.1E+01	1.2E+00	3.8E+00	10	100	9.83E+02	97%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1316-T03-B	1	1.08E+01			1.08E+01	1.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1316-T04-B	1	1.35E+01			1.35E+01	1.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1316-T05-B	1	1.93E+01			1.93E+01	9.7E+00	1.2E+00	3.8E+00					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1316-T01-C	1	6.96E+00			6.96E+00	1.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1316-T02-C	1	7.36E+00			7.36E+00	2.0E+01	1.2E+00	3.8E+00	10	100	1.06E+03	105%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1316-T03-C	1	1.15E+01			1.15E+01	1.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1316-T04-C	1	1.24E+01			1.24E+01	1.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1316-T05-C	1	1.56E+01			1.56E+01	1.5E+01	1.2E+00	3.8E+00					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1316-B01-A	1	1.78E+00	E		1.78E+00	3.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1316-B02-A	1	1.54E+00	E		1.54E+00	3.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
Mo	CFS-L10-1316-B03-A	1	6.00E-01	U1/2		6.00E-01	1.1E+02	1.2E+00	3.8E+00				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	CFS-L10-1316-T01-A	1	1.97E+02			1.97E+02	1.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1316-T02-A	1	3.19E+02			3.19E+02	2.1E+00	1.8E+00	5.7E+00	10	100	1.30E+03	98%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1316-T03-A	1	5.53E+02			5.53E+02	8.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1316-T04-A	1	7.30E+02			7.30E+02	1.0E+00	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1316-T05-A	1	8.49E+02			8.49E+02	7.0E-01	1.8E+00	5.7E+00					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1316-T01-B	1	2.14E+02			2.14E+02	7.4E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1316-T02-B	1	3.59E+02			3.59E+02	6.9E-01	1.8E+00	5.7E+00	10	100	1.30E+03	94%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1316-T03-B	1	6.05E+02			6.05E+02	5.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1316-T04-B	1	8.18E+02			8.18E+02	8.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1316-T05-B	1	1.01E+03			1.01E+03	4.7E-01	1.8E+00	5.7E+00					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1316-T01-C	1	2.14E+02			2.14E+02	7.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1316-T02-C	1	3.36E+02			3.36E+02	6.9E-01	1.8E+00	5.7E+00	10	100	1.32E+03	98%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1316-T03-C	1	5.67E+02			5.67E+02	5.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1316-T04-C	1	8.12E+02			8.12E+02	9.5E-01	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1316-T05-C	1	1.01E+03			1.01E+03	5.0E-01	1.8E+00	5.7E+00					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	2.6E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1316-B02-A	1	9.00E-01	U1/2		9.00E-01	1.1E+03	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
Ni	CFS-L10-1316-B03-A	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	CFS-L10-1316-T01-A	1	1.85E+00	U1/2		1.85E+00	6.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1316-T02-A	1	1.85E+00	U1/2		1.85E+00	1.8E+02	3.7E+00	1.2E+01	1000	100	1.11E+03	111%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1316-T03-A	1	6.27E+00	E		6.27E+00	2.1E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1316-T04-A	1	9.05E+00	E		9.05E+00	3.8E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1316-T05-A	1	1.41E+01			1.41E+01	5.1E+02	3.7E+00	1.2E+01					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1316-T01-B	1	1.85E+00	U1/2		1.85E+00	6.2E+03	3.7E+00	1.2E+01				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1316-T02-B	1	1.85E+00	U1/2		1.85E+00	1.2E+02	3.7E+00	1.2E+01	1000	100	1.05E+03	104%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1316-T03-B	1	4.30E+00	E		4.30E+00	2.0E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1316-T04-B	1	8.12E+00	E		8.12E+00	1.7E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1316-T05-B	1	1.47E+01			1.47E+01	9.8E+01	3.7E+00	1.2E+01					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1316-T01-C	1	1.85E+00	U1/2		1.85E+00	4.5E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1316-T02-C	1	1.85E+00	U1/2		1.85E+00	7.7E+01	3.7E+00	1.2E+01	1000	100	1.14E+03	114%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1316-T03-C	1	7.43E+00	E		7.43E+00	4.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1316-T04-C	1	1.04E+01	E		1.04E+01	2.7E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1316-T05-C	1	2.22E+01			2.22E+01	5.0E+01	3.7E+00	1.2E+01					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	1.1E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1316-B02-A	1	1.85E+00	U1/2		1.85E+00	1.5E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
P	CFS-L10-1316-B03-A	1	1.85E+00	U1/2		1.85E+00	5.0E+02	3.7E+00	1.2E+01				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	CFS-L10-1316-T01-A	1	9.02E+03			9.02E+03	4.4E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1316-T02-A	1	1.52E+04			1.52E+04	1.8E+00	1.6E+00	5.1E+00	1000	100	1.62E+04	96%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1316-T03-A	1	3.00E+04			3.00E+04	1.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1316-T04-A	1	4.74E+04			4.74E+04	7.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1316-T05-A	1	7.36E+04			7.36E+04	8.8E-01	1.6E+00	5.1E+00					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1316-T01-B	1	9.09E+03			9.09E+03	4.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1316-T02-B	1	1.56E+04			1.56E+04	7.9E-01	1.6E+00	5.1E+00	1000	100	1.65E+04	91%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1316-T03-B	1	2.91E+04			2.91E+04	5.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1316-T04-B	1	4.58E+04			4.58E+04	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1316-T05-B	1	6.89E+04			6.89E+04	5.5E-01	1.6E+00	5.1E+00					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1316-T01-C	1	8.40E+03			8.40E+03	5.0E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1316-T02-C	1	1.47E+04			1.47E+04	4.0E-01	1.6E+00	5.1E+00	1000	100	1.56E+04	98%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1316-T03-C	1	2.77E+04			2.77E+04	6.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1316-T04-C	1	4.42E+04			4.42E+04	5.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1316-T05-C	1	7.00E+04			7.00E+04	6.3E-01	1.6E+00	5.1E+00					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1316-B01-A	1	9.73E+01			9.73E+01	2.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1316-B02-A	1	9.40E+01			9.40E+01	3.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
K	CFS-L10-1316-B03-A	1	8.52E+01			8.52E+01	1.4E+00	1.6E+00	5.1E+00				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	CFS-L10-1316-T01-A	1	8.72E+01			8.72E+01	8.6E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1316-T02-A	1	1.30E+02			1.30E+02	1.6E+01	1.5E+01	4.8E+01	10	100	1.18E+03	105%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1316-T03-A	1	2.69E+02			2.69E+02	4.6E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1316-T04-A	1	4.77E+02			4.77E+02	3.2E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1316-T05-A	1	8.43E+02			8.43E+02	7.0E-01	1.5E+01	4.8E+01					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1316-T01-B	1	7.99E+01			7.99E+01	1.1E+01	1.5E+01	4.8E+01				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1316-T02-B	1	1.45E+02			1.45E+02	1.8E+00	1.5E+01	4.8E+01	10	100	1.08E+03	93%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1316-T03-B	1	2.63E+02			2.63E+02	4.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1316-T04-B	1	4.90E+02			4.90E+02	4.5E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1316-T05-B	1	8.00E+02			8.00E+02	1.5E+00	1.5E+01	4.8E+01					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1316-T01-C	1	9.48E+01			9.48E+01	1.5E+01	1.5E+01	4.8E+01				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1316-T02-C	1	1.24E+02			1.24E+02	8.3E+00	1.5E+01	4.8E+01	10	100	1.13E+03	101%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1316-T03-C	1	2.53E+02			2.53E+02	5.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1316-T04-C	1	4.45E+02			4.45E+02	3.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1316-T05-C	1	8.08E+02			8.08E+02	2.1E+00	1.5E+01	4.8E+01					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1316-B01-A	1	7.50E+00	U1/2		7.50E+00	9.6E+01	1.5E+01	4.8E+01				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1316-B02-A	1	7.50E+00	U1/2		7.50E+00	1.2E+02	1.5E+01	4.8E+01				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
Se	CFS-L10-1316-B03-A	1	7.50E+00	U1/2		7.50E+00	7.9E+01	1.5E+01	4.8E+01				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	CFS-L10-1316-T01-A	1	3.48E+03			3.48E+03	5.8E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1316-T02-A	1	4.41E+03			4.41E+03	9.5E-01	1.1E+00	3.5E+00	1000	100	5.34E+03	93%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1316-T03-A	1	5.76E+03			5.76E+03	1.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1316-T04-A	1	6.26E+03			6.26E+03	7.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1316-T05-A	1	6.53E+03			6.53E+03	7.6E-01	1.1E+00	3.5E+00					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1316-T01-B	1	3.57E+03			3.57E+03	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1316-T02-B	1	4.59E+03			4.59E+03	1.5E+00	1.1E+00	3.5E+00	1000	100	5.47E+03	88%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1316-T03-B	1	5.84E+03			5.84E+03	2.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1316-T04-B	1	6.29E+03			6.29E+03	9.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1316-T05-B	1	6.41E+03			6.41E+03	3.1E-01	1.1E+00	3.5E+00					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1316-T01-C	1	3.46E+03			3.46E+03	8.1E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1316-T02-C	1	4.36E+03			4.36E+03	1.7E+00	1.1E+00	3.5E+00	1000	100	5.24E+03	88%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1316-T03-C	1	5.56E+03			5.56E+03	6.6E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1316-T04-C	1	6.24E+03			6.24E+03	6.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1316-T05-C	1	6.36E+03			6.36E+03	8.0E-01	1.1E+00	3.5E+00					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1316-B01-A	1	1.03E+01			1.03E+01	1.5E+01	1.1E+00	3.5E+00				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1316-B02-A	1	1.14E+01			1.14E+01	1.3E+01	1.1E+00	3.5E+00				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
Si	CFS-L10-1316-B03-A	1	1.57E+01			1.57E+01	1.1E+01	1.1E+00	3.5E+00				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	CFS-L10-1316-T01-A	1	1.74E+04			1.74E+04	7.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1316-T02-A	1	3.31E+04			3.31E+04	1.3E+00	2.5E+00	8.0E+00	1000	100	3.40E+04	95%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1316-T03-A	1	7.10E+04			7.10E+04	3.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1316-T04-A	1	1.12E+05			1.12E+05	5.1E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1316-T05-A	1	1.72E+05			1.72E+05	8.0E-01	2.5E+00	8.0E+00					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1316-T01-B	1	1.81E+04			1.81E+04	1.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1316-T02-B	1	3.50E+04			3.50E+04	1.4E+00	2.5E+00	8.0E+00	1000	100	3.60E+04	97%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1316-T03-B	1	7.24E+04			7.24E+04	6.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1316-T04-B	1	1.13E+05			1.13E+05	3.5E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1316-T05-B	1	1.67E+05			1.67E+05	1.7E+00	2.5E+00	8.0E+00					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1316-T01-C	1	1.73E+04			1.73E+04	4.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1316-T02-C	1	3.26E+04			3.26E+04	3.2E-01	2.5E+00	8.0E+00	1000	100	3.35E+04	91%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1316-T03-C	1	6.60E+04			6.60E+04	6.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1316-T04-C	1	1.09E+05			1.09E+05	4.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1316-T05-C	1	1.67E+05			1.67E+05	8.0E-01	2.5E+00	8.0E+00					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1316-B01-A	1	3.14E+01			3.14E+01	6.0E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1316-B02-A	1	1.86E+01			1.86E+01	3.0E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
Na	CFS-L10-1316-B03-A	1	2.09E+01			2.09E+01	5.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	CFS-L10-1316-T01-A	1	1.39E+03			1.39E+03	3.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1316-T02-A	1	1.78E+03			1.78E+03	7.2E-01	1.0E+00	3.2E+00	1000	100	2.83E+03	105%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1316-T03-A	1	2.67E+03			2.67E+03	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1316-T04-A	1	3.62E+03			3.62E+03	5.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1316-T05-A	1	4.80E+03			4.80E+03	1.8E-01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1316-T01-B	1	1.34E+03			1.34E+03	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1316-T02-B	1	1.72E+03			1.72E+03	1.5E+00	1.0E+00	3.2E+00	1000	100	2.79E+03	107%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1316-T03-B	1	2.47E+03			2.47E+03	1.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1316-T04-B	1	3.15E+03			3.15E+03	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1316-T05-B	1	4.11E+03			4.11E+03	1.0E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1316-T01-C	1	1.22E+03			1.22E+03	7.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1316-T02-C	1	1.70E+03			1.70E+03	1.2E+00	1.0E+00	3.2E+00	1000	100	2.81E+03	111%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1316-T03-C	1	2.46E+03			2.46E+03	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1316-T04-C	1	3.10E+03			3.10E+03	9.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1316-T05-C	1	4.10E+03			4.10E+03	6.3E-01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	8.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	8.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
Sr	CFS-L10-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	4.2E+02	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	CFS-L10-1316-T01-A	1	5.78E+05			5.78E+05	4.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1316-T02-A	1	6.34E+05			6.34E+05	1.9E+00	6.8E+00	2.2E+01	1000	100	6.35E+05	95%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1316-T03-A	1	8.14E+05			8.14E+05	5.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1316-T04-A	1	1.08E+06			1.08E+06	1.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1316-T05-A	1	1.48E+06			1.48E+06	6.8E-01	6.8E+00	2.2E+01					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1316-T01-B	1	5.91E+05			5.91E+05	3.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1316-T02-B	1	6.44E+05			6.44E+05	1.2E+00	6.8E+00	2.2E+01	1000	100	6.45E+05	86%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1316-T03-B	1	8.07E+05			8.07E+05	2.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1316-T04-B	1	1.05E+06			1.05E+06	7.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1316-T05-B	1	1.43E+06			1.43E+06	4.0E-01	6.8E+00	2.2E+01					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1316-T01-C	1	5.39E+05			5.39E+05	3.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1316-T02-C	1	6.09E+05			6.09E+05	3.2E-01	6.8E+00	2.2E+01	1000	100	6.10E+05	94%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1316-T03-C	1	7.67E+05			7.67E+05	9.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1316-T04-C	1	1.02E+06			1.02E+06	5.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1316-T05-C	1	1.43E+06			1.43E+06	6.5E-01	6.8E+00	2.2E+01					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1316-B01-A	1	6.12E+01			6.12E+01	1.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1316-B02-A	1	5.31E+01			5.31E+01	2.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
S	CFS-L10-1316-B03-A	1	6.19E+01			6.19E+01	5.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	CFS-L10-1316-T01-A	1	2.85E+02			2.85E+02	2.2E+00	4.6E+00	1.5E+01				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1316-T02-A	1	4.20E+02			4.20E+02	1.8E+00	4.6E+00	1.5E+01	10	100	1.37E+03	95%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1316-T03-A	1	6.93E+02			6.93E+02	1.8E+00	4.6E+00	1.5E+01				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1316-T04-A	1	9.61E+02			9.61E+02	1.4E+00	4.6E+00	1.5E+01				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1316-T05-A	1	1.45E+03			1.45E+03	4.8E-01	4.6E+00	1.5E+01					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1316-T01-B	1	2.82E+02			2.82E+02	3.5E-01	4.6E+00	1.5E+01				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1316-T02-B	1	4.33E+02			4.33E+02	1.1E+00	4.6E+00	1.5E+01	10	100	1.30E+03	86%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1316-T03-B	1	6.88E+02			6.88E+02	9.9E-01	4.6E+00	1.5E+01				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1316-T04-B	1	9.75E+02			9.75E+02	3.0E-01	4.6E+00	1.5E+01				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1316-T05-B	1	1.34E+03			1.34E+03	2.5E-01	4.6E+00	1.5E+01					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1316-T01-C	1	2.70E+02			2.70E+02	7.9E-01	4.6E+00	1.5E+01				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1316-T02-C	1	4.17E+02			4.17E+02	9.6E-01	4.6E+00	1.5E+01	10	100	1.33E+03	91%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1316-T03-C	1	6.65E+02			6.65E+02	7.1E-01	4.6E+00	1.5E+01				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1316-T04-C	1	9.54E+02			9.54E+02	3.1E-01	4.6E+00	1.5E+01				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1316-T05-C	1	1.33E+03			1.33E+03	1.7E-01	4.6E+00	1.5E+01					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1316-B01-A	1	2.30E+00	U1/2		2.30E+00	9.3E+00	4.6E+00	1.5E+01				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1316-B02-A	1	2.30E+00	U1/2		2.30E+00	6.3E+00	4.6E+00	1.5E+01				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
Tl	CFS-L10-1316-B03-A	1	2.30E+00	U1/2		2.30E+00	1.5E+01	4.6E+00	1.5E+01				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	CFS-L10-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	3.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	3.8E+01	2.0E+00	6.4E+00	10	100	1.11E+03	110%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	9.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1316-T05-A	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	8.8E+02	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00	10	100	9.78E+02	98%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	3.3E+02	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	3.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1316-T05-B	1	1.00E+00	U1/2		1.00E+00	1.0E+02	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	5.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	3.9E+03	2.0E+00	6.4E+00	10	100	1.05E+03	105%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	1.5E+02	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	7.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1316-T05-C	1	1.00E+00	U1/2		1.00E+00	6.4E+01	2.0E+00	6.4E+00					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	1.9E+02	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1316-B02-A	1	1.00E+00	U1/2		1.00E+00	7.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
Ti	CFS-L10-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	CFS-L10-1316-T01-A	1	2.77E+01			2.77E+01	4.7E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1316-T02-A	1	2.57E+01			2.57E+01	2.0E-01	1.5E+00	4.8E+00	10	100	1.13E+03	110%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1316-T03-A	1	2.50E+01			2.50E+01	5.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1316-T04-A	1	2.43E+01			2.43E+01	5.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1316-T05-A	1	2.40E+01			2.40E+01	5.2E+00	1.5E+00	4.8E+00					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1316-T01-B	1	2.87E+01			2.87E+01	3.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1316-T02-B	1	2.76E+01			2.76E+01	1.7E+00	1.5E+00	4.8E+00	10	100	9.86E+02	96%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1316-T03-B	1	2.52E+01			2.52E+01	1.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1316-T04-B	1	2.32E+01			2.32E+01	4.9E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1316-T05-B	1	2.17E+01			2.17E+01	6.2E+00	1.5E+00	4.8E+00					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1316-T01-C	1	2.50E+01			2.50E+01	5.9E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1316-T02-C	1	2.51E+01			2.51E+01	3.7E+00	1.5E+00	4.8E+00	10	100	1.08E+03	105%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1316-T03-C	1	2.40E+01			2.40E+01	9.7E-01	1.5E+00	4.8E+00				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1316-T04-C	1	2.23E+01			2.23E+01	4.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1316-T05-C	1	2.12E+01			2.12E+01	4.4E+00	1.5E+00	4.8E+00					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1316-B01-A	1	7.50E-01	U1/2		7.50E-01	4.9E+01	1.5E+00	4.8E+00				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1316-B02-A	1	7.50E-01	U1/2		7.50E-01	6.4E+01	1.5E+00	4.8E+00				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
V	CFS-L10-1316-B03-A	1	7.50E-01	U1/2		7.50E-01	3.8E+01	1.5E+00	4.8E+00				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	CFS-L10-1316-T01-A	1	1.93E+04			1.93E+04	9.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:44 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1316-T02-A	1	2.79E+04			2.79E+04	7.8E-01	1.0E+00	3.2E+00	10	100	2.88E+04	91%	VU ICP-OES	4/13/11 3:45 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1316-T03-A	1	4.25E+04			4.25E+04	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:47 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1316-T04-A	1	5.22E+04			5.22E+04	2.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:49 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1316-T05-A	1	5.34E+04			5.34E+04	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 3:50 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1316-T01-B	1	2.10E+04			2.10E+04	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:52 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1316-T02-B	1	3.22E+04			3.22E+04	1.3E+00	1.0E+00	3.2E+00	10	100	3.30E+04	86%	VU ICP-OES	4/13/11 3:53 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1316-T03-B	1	4.69E+04			4.69E+04	5.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:55 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1316-T04-B	1	5.81E+04			5.81E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:57 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1316-T05-B	1	6.55E+04			6.55E+04	2.2E-01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 3:58 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1316-T01-C	1	2.14E+04			2.14E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 4:00 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1316-T02-C	1	2.92E+04			2.92E+04	5.8E-01	1.0E+00	3.2E+00	10	100	3.01E+04	94%	VU ICP-OES	4/13/11 4:02 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1316-T03-C	1	4.36E+04			4.36E+04	4.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 4:03 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1316-T04-C	1	5.77E+04			5.77E+04	8.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 4:05 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1316-T05-C	1	6.49E+04			6.49E+04	5.0E-01	1.0E+00	3.2E+00					VU ICP-OES	4/13/11 4:07 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1316-B01-A	1	2.25E+00	E		2.25E+00	8.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:39 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1316-B02-A	1	3.68E+00			3.68E+00	1.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:40 PM	EPA Interlab L10 1313-1316 CFS
Zn	CFS-L10-1316-B03-A	1	2.89E+00	E		2.89E+00	2.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	4/13/11 3:42 PM	EPA Interlab L10 1313-1316 CFS

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	CFS-L11-1316-T01-A	1	5.00E+01			5.00E+01	3.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1316-T02-A	1	3.86E+01			3.86E+01	6.9E+01	1.0E+00	3.2E+00	1000	100	1.11E+03	107%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1316-T03-A	1	4.83E+01			4.83E+01	2.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1316-T04-A	1	2.92E+01			2.92E+01	1.0E+02	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1316-T05-A	1	5.41E+01			5.41E+01	8.0E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1316-T01-B	1	4.95E+01			4.95E+01	5.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1316-T02-B	1	4.77E+01			4.77E+01	4.8E+00	1.0E+00	3.2E+00	1000	100	1.15E+03	110%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1316-T03-B	1	5.21E+01			5.21E+01	2.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1316-T04-B	1	5.35E+01			5.35E+01	8.9E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1316-T05-B	1	5.45E+01			5.45E+01	6.2E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1316-T01-C	1	5.15E+01			5.15E+01	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1316-T02-C	1	4.74E+01			4.74E+01	6.4E+00	1.0E+00	3.2E+00	1000	100	1.16E+03	111%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1316-T03-C	1	4.63E+01			4.63E+01	6.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1316-T04-C	1	5.35E+01			5.35E+01	1.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1316-T05-C	1	5.36E+01			5.36E+01	3.1E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	2.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	2.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
Al	CFS-L11-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	9.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	CFS-L11-1316-T01-A	1	2.55E+01			2.55E+01	1.7E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1316-T02-A	1	1.27E+01	E		1.27E+01	1.1E+02	7.5E+00	2.4E+01	10	100	8.86E+02	87%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1316-T03-A	1	3.28E+01			3.28E+01	1.9E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1316-T04-A	1	1.64E+01	E		1.64E+01	1.7E+02	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1316-T05-A	1	4.71E+01			4.71E+01	1.2E+01	7.5E+00	2.4E+01					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1316-T01-B	1	2.19E+01	E		2.19E+01	1.9E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1316-T02-B	1	2.97E+01			2.97E+01	2.4E+01	7.5E+00	2.4E+01	10	100	9.16E+02	89%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1316-T03-B	1	4.28E+01			4.28E+01	1.8E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1316-T04-B	1	4.63E+01			4.63E+01	2.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1316-T05-B	1	4.72E+01			4.72E+01	2.7E+00	7.5E+00	2.4E+01					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1316-T01-C	1	3.04E+01			3.04E+01	4.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1316-T02-C	1	2.72E+01			2.72E+01	2.2E+01	7.5E+00	2.4E+01	10	100	9.16E+02	89%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1316-T03-C	1	3.35E+01			3.35E+01	5.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1316-T04-C	1	3.43E+01			3.43E+01	2.5E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1316-T05-C	1	4.05E+01			4.05E+01	1.4E+01	7.5E+00	2.4E+01					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1316-B01-A	1	3.75E+00	U1/2		3.75E+00	7.8E+01	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1316-B02-A	1	3.75E+00	U1/2		3.75E+00	1.3E+02	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
Sb	CFS-L11-1316-B03-A	1	3.75E+00	U1/2		3.75E+00	1.7E+02	7.5E+00	2.4E+01				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	CFS-L11-1316-T01-A	1	1.88E+01	E		1.88E+01	8.9E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1316-T02-A	1	1.54E+01	E		1.54E+01	5.6E+01	1.1E+01	3.5E+01	10	100	9.07E+02	89%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1316-T03-A	1	3.04E+01	E		3.04E+01	1.4E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1316-T04-A	1	1.99E+01	E		1.99E+01	1.2E+02	1.1E+01	3.5E+01				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1316-T05-A	1	2.67E+01	E		2.67E+01	1.5E+01	1.1E+01	3.5E+01					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1316-T01-B	1	2.51E+01	E		2.51E+01	2.4E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1316-T02-B	1	2.49E+01	E		2.49E+01	1.9E+01	1.1E+01	3.5E+01	10	100	9.28E+02	90%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1316-T03-B	1	2.70E+01	E		2.70E+01	4.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1316-T04-B	1	3.64E+01			3.64E+01	2.7E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1316-T05-B	1	3.88E+01			3.88E+01	3.4E+01	1.1E+01	3.5E+01					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1316-T01-C	1	2.52E+01	E		2.52E+01	3.6E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1316-T02-C	1	3.02E+01	E		3.02E+01	4.9E+01	1.1E+01	3.5E+01	10	100	9.26E+02	90%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1316-T03-C	1	2.80E+01	E		2.80E+01	3.4E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1316-T04-C	1	2.93E+01	E		2.93E+01	3.5E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1316-T05-C	1	3.27E+01	E		3.27E+01	1.2E+01	1.1E+01	3.5E+01					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1316-B01-A	1	5.50E+00	U1/2		5.50E+00	1.6E+02	1.1E+01	3.5E+01				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1316-B02-A	1	5.50E+00	U1/2		5.50E+00	6.1E+01	1.1E+01	3.5E+01				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
As	CFS-L11-1316-B03-A	1	5.50E+00	U1/2		5.50E+00	1.6E+02	1.1E+01	3.5E+01				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	CFS-L11-1316-T01-A	1	6.27E+01			6.27E+01	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1316-T02-A	1	5.89E+01			5.89E+01	2.0E+02	1.0E+00	3.2E+00	1000	100	9.82E+02	92%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1316-T03-A	1	3.79E+02			3.79E+02	6.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1316-T04-A	1	2.47E+02			2.47E+02	1.8E+02	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1316-T05-A	1	1.05E+03			1.05E+03	8.9E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1316-T01-B	1	7.11E+01			7.11E+01	2.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1316-T02-B	1	1.51E+02			1.51E+02	6.7E-01	1.0E+00	3.2E+00	1000	100	1.02E+03	87%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1316-T03-B	1	3.80E+02			3.80E+02	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1316-T04-B	1	5.93E+02			5.93E+02	9.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1316-T05-B	1	1.03E+03			1.03E+03	1.3E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1316-T01-C	1	7.15E+01			7.15E+01	3.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1316-T02-C	1	1.65E+02			1.65E+02	4.3E+00	1.0E+00	3.2E+00	1000	100	1.03E+03	87%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1316-T03-C	1	3.67E+02			3.67E+02	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1316-T04-C	1	6.56E+02			6.56E+02	9.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1316-T05-C	1	1.05E+03			1.05E+03	4.8E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
B	CFS-L11-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	6.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	CFS-L11-1316-T01-A	1	2.26E+02			2.26E+02	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1316-T02-A	1	1.37E+02			1.37E+02	9.9E+01	1.0E+00	3.2E+00	10	100	9.74E+02	84%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1316-T03-A	1	3.85E+02			3.85E+02	5.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1316-T04-A	1	2.56E+02			2.56E+02	1.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1316-T05-A	1	8.11E+02			8.11E+02	8.9E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1316-T01-B	1	2.30E+02			2.30E+02	7.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1316-T02-B	1	2.67E+02			2.67E+02	5.4E-01	1.0E+00	3.2E+00	10	100	1.20E+03	94%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1316-T03-B	1	3.91E+02			3.91E+02	9.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1316-T04-B	1	5.39E+02			5.39E+02	1.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1316-T05-B	1	8.20E+02			8.20E+02	1.1E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1316-T01-C	1	2.35E+02			2.35E+02	5.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1316-T02-C	1	2.68E+02			2.68E+02	2.5E+00	1.0E+00	3.2E+00	10	100	1.20E+03	93%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1316-T03-C	1	3.71E+02			3.71E+02	3.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1316-T04-C	1	5.48E+02			5.48E+02	1.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1316-T05-C	1	8.18E+02			8.18E+02	3.2E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	2.3E+02	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	5.8E+02	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
Ba	CFS-L11-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	6.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	CFS-L11-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	4.5E+02	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	2.0E+02	1.9E+00	6.0E+00	10	100	8.57E+02	86%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	1.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	1.6E+02	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1316-T05-A	1	9.50E-01	U1/2		9.50E-01	2.5E+01	1.9E+00	6.0E+00					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	6.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	5.4E+02	1.9E+00	6.0E+00	10	100	8.89E+02	89%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	4.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	2.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1316-T05-B	1	9.50E-01	U1/2		9.50E-01	4.2E+01	1.9E+00	6.0E+00					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	4.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	7.2E+01	1.9E+00	6.0E+00	10	100	8.96E+02	89%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	6.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	3.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1316-T05-C	1	9.50E-01	U1/2		9.50E-01	2.3E+01	1.9E+00	6.0E+00					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	1.8E+02	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1316-B02-A	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
Be	CFS-L11-1316-B03-A	1	9.50E-01	U1/2		9.50E-01	6.8E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	CFS-L11-1316-T01-A	1	2.96E+03			2.96E+03	1.3E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1316-T02-A	1	2.45E+03			2.45E+03	8.6E+01	2.2E+00	7.0E+00	10	100	3.43E+03	98%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1316-T03-A	1	6.05E+03			6.05E+03	2.5E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1316-T04-A	1	3.45E+03			3.45E+03	1.4E+02	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1316-T05-A	1	1.11E+04			1.11E+04	6.1E-01	2.2E+00	7.0E+00					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1316-T01-B	1	3.09E+03			3.09E+03	7.3E-02	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1316-T02-B	1	4.20E+03			4.20E+03	1.6E-01	2.2E+00	7.0E+00	10	100	5.18E+03	99%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1316-T03-B	1	6.00E+03			6.00E+03	9.5E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1316-T04-B	1	6.93E+03			6.93E+03	4.6E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1316-T05-B	1	1.11E+04			1.11E+04	8.7E-01	2.2E+00	7.0E+00					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1316-T01-C	1	3.07E+03			3.07E+03	8.7E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1316-T02-C	1	4.14E+03			4.14E+03	1.8E+00	2.2E+00	7.0E+00	10	100	5.17E+03	103%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1316-T03-C	1	5.86E+03			5.86E+03	1.1E+00	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1316-T04-C	1	8.51E+03			8.51E+03	6.7E-01	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1316-T05-C	1	1.12E+04			1.12E+04	5.4E-01	2.2E+00	7.0E+00					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1316-B01-A	1	1.10E+00	U1/2		1.10E+00	3.2E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1316-B02-A	1	1.10E+00	U1/2		1.10E+00	1.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
Cd	CFS-L11-1316-B03-A	1	1.10E+00	U1/2		1.10E+00	1.1E+02	2.2E+00	7.0E+00				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	CFS-L11-1316-T01-A	1	6.33E+05			6.33E+05	4.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1316-T02-A	1	3.71E+05			3.71E+05	8.3E+01	2.6E+00	8.3E+00	1000	100	3.72E+05	82%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1316-T03-A	1	5.93E+05			5.93E+05	5.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1316-T04-A	1	2.68E+05			2.68E+05	1.4E+02	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1316-T05-A	1	5.13E+05			5.13E+05	5.1E-01	2.6E+00	8.3E+00					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1316-T01-B	1	6.53E+05			6.53E+05	3.7E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1316-T02-B	1	6.21E+05			6.21E+05	1.6E-01	2.6E+00	8.3E+00	1000	100	6.22E+05	92%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1316-T03-B	1	6.01E+05			6.01E+05	9.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1316-T04-B	1	5.46E+05			5.46E+05	6.9E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1316-T05-B	1	5.10E+05			5.10E+05	1.1E+00	2.6E+00	8.3E+00					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1316-T01-C	1	6.56E+05			6.56E+05	9.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1316-T02-C	1	6.23E+05			6.23E+05	2.0E+00	2.6E+00	8.3E+00	1000	100	6.24E+05	90%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1316-T03-C	1	5.84E+05			5.84E+05	3.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1316-T04-C	1	5.43E+05			5.43E+05	6.9E-02	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1316-T05-C	1	5.05E+05			5.05E+05	3.8E-01	2.6E+00	8.3E+00					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1316-B01-A	1	1.55E+01			1.55E+01	5.8E+01	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1316-B02-A	1	1.06E+01			1.06E+01	1.5E+01	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
Ca	CFS-L11-1316-B03-A	1	1.51E+01			1.51E+01	5.5E+01	2.6E+00	8.3E+00				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	CFS-L11-1316-T01-A	1	6.00E-01	U1/2		6.00E-01	5.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1316-T02-A	1	6.00E-01	U1/2		6.00E-01	5.9E+01	1.2E+00	3.8E+00	10	100	8.87E+02	89%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1316-T03-A	1	6.00E-01	U1/2		6.00E-01	4.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1316-T04-A	1	6.00E-01	U1/2		6.00E-01	1.1E+02	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1316-T05-A	1	1.70E+00	E		1.70E+00	9.9E+00	1.2E+00	3.8E+00					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1316-T01-B	1	6.00E-01	U1/2		6.00E-01	2.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1316-T02-B	1	6.00E-01	U1/2		6.00E-01	1.7E+01	1.2E+00	3.8E+00	10	100	9.15E+02	91%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1316-T03-B	1	6.00E-01	U1/2		6.00E-01	2.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1316-T04-B	1	6.00E-01	U1/2		6.00E-01	8.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1316-T05-B	1	2.02E+00	E		2.02E+00	1.5E+01	1.2E+00	3.8E+00					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1316-T01-C	1	6.00E-01	U1/2		6.00E-01	4.8E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1316-T02-C	1	6.00E-01	U1/2		6.00E-01	1.2E+02	1.2E+00	3.8E+00	10	100	9.23E+02	92%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1316-T03-C	1	6.00E-01	U1/2		6.00E-01	8.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1316-T04-C	1	6.00E-01	U1/2		6.00E-01	4.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1316-T05-C	1	1.80E+00	E		1.80E+00	1.8E+01	1.2E+00	3.8E+00					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	3.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	1.1E+02	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
Cr	CFS-L11-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	3.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	CFS-L11-1316-T01-A	1	8.07E+01			8.07E+01	2.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1316-T02-A	1	8.00E+01			8.00E+01	8.4E+01	1.8E+00	5.7E+00	10	100	1.09E+03	101%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1316-T03-A	1	2.41E+02			2.41E+02	4.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1316-T04-A	1	1.45E+02			1.45E+02	1.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1316-T05-A	1	5.95E+02			5.95E+02	1.0E+00	1.8E+00	5.7E+00					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1316-T01-B	1	8.48E+01			8.48E+01	7.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1316-T02-B	1	1.34E+02			1.34E+02	9.4E-01	1.8E+00	5.7E+00	10	100	1.12E+03	99%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1316-T03-B	1	2.40E+02			2.40E+02	8.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1316-T04-B	1	3.02E+02			3.02E+02	5.1E-02	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1316-T05-B	1	5.90E+02			5.90E+02	1.6E+00	1.8E+00	5.7E+00					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1316-T01-C	1	8.41E+01			8.41E+01	2.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1316-T02-C	1	1.36E+02			1.36E+02	4.9E-01	1.8E+00	5.7E+00	10	100	1.13E+03	100%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1316-T03-C	1	2.30E+02			2.30E+02	1.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1316-T04-C	1	4.05E+02			4.05E+02	2.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1316-T05-C	1	6.01E+02			6.01E+02	4.0E-01	1.8E+00	5.7E+00					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	5.2E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1316-B02-A	1	9.00E-01	U1/2		9.00E-01	3.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
Co	CFS-L11-1316-B03-A	1	9.00E-01	U1/2		9.00E-01	1.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	CFS-L11-1316-T01-A	1	7.67E+02			7.67E+02	1.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1316-T02-A	1	7.95E+02			7.95E+02	7.4E+01	3.7E+00	1.2E+01	10	100	1.92E+03	112%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1316-T03-A	1	1.49E+03			1.49E+03	1.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1316-T04-A	1	8.55E+02			8.55E+02	1.3E+02	3.7E+00	1.2E+01				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1316-T05-A	1	2.71E+03			2.71E+03	7.4E-01	3.7E+00	1.2E+01					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1316-T01-B	1	7.98E+02			7.98E+02	8.8E-01	3.7E+00	1.2E+01				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1316-T02-B	1	1.06E+03			1.06E+03	6.5E-01	3.7E+00	1.2E+01	10	100	1.95E+03	88%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1316-T03-B	1	1.44E+03			1.44E+03	4.6E-01	3.7E+00	1.2E+01				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1316-T04-B	1	1.69E+03			1.69E+03	3.4E-01	3.7E+00	1.2E+01				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1316-T05-B	1	2.87E+03			2.87E+03	5.3E-01	3.7E+00	1.2E+01					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1316-T01-C	1	7.88E+02			7.88E+02	1.6E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1316-T02-C	1	1.09E+03			1.09E+03	2.6E+00	3.7E+00	1.2E+01	10	100	1.98E+03	89%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1316-T03-C	1	1.29E+03			1.29E+03	4.1E-01	3.7E+00	1.2E+01				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1316-T04-C	1	2.21E+03			2.21E+03	6.3E-01	3.7E+00	1.2E+01				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1316-T05-C	1	2.63E+03			2.63E+03	2.3E-01	3.7E+00	1.2E+01					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	7.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1316-B02-A	1	1.85E+00	U1/2		1.85E+00	1.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
Cu	CFS-L11-1316-B03-A	1	1.85E+00	U1/2		1.85E+00	2.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	CFS-L11-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	2.1E+02	2.0E+00	6.4E+00	1000	100	8.89E+02	89%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	2.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	7.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1316-T05-A	1	1.00E+00	U1/2		1.00E+00	3.9E+01	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	4.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	5.2E+00	2.0E+00	6.4E+00	1000	100	9.08E+02	91%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	3.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1316-T05-B	1	1.00E+00	U1/2		1.00E+00	8.1E+01	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	5.8E+00	2.0E+00	6.4E+00	1000	100	9.12E+02	91%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	2.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	6.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1316-T05-C	1	1.00E+00	U1/2		1.00E+00	1.6E+01	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	9.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1316-B02-A	1	1.00E+00	U1/2		1.00E+00	3.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
Fe	CFS-L11-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	7.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	CFS-L11-1316-T01-A	1	7.37E+02			7.37E+02	9.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1316-T02-A	1	4.70E+02			4.70E+02	8.8E+01	6.8E+00	2.2E+01	10	100	1.52E+03	105%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1316-T03-A	1	9.60E+02			9.60E+02	5.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1316-T04-A	1	4.91E+02			4.91E+02	1.4E+02	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1316-T05-A	1	1.06E+03			1.06E+03	1.5E+00	6.8E+00	2.2E+01					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1316-T01-B	1	7.79E+02			7.79E+02	6.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1316-T02-B	1	8.50E+02			8.50E+02	2.4E-01	6.8E+00	2.2E+01	10	100	1.75E+03	90%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1316-T03-B	1	9.94E+02			9.94E+02	7.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1316-T04-B	1	1.03E+03			1.03E+03	2.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1316-T05-B	1	1.08E+03			1.08E+03	1.3E+00	6.8E+00	2.2E+01					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1316-T01-C	1	8.27E+02			8.27E+02	1.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1316-T02-C	1	8.91E+02			8.91E+02	2.1E+00	6.8E+00	2.2E+01	10	100	1.85E+03	96%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1316-T03-C	1	9.20E+02			9.20E+02	1.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1316-T04-C	1	1.02E+03			1.02E+03	6.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1316-T05-C	1	9.65E+02			9.65E+02	3.6E-01	6.8E+00	2.2E+01					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	6.5E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1316-B02-A	1	3.40E+00	U1/2		3.40E+00	8.0E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
Pb	CFS-L11-1316-B03-A	1	3.40E+00	U1/2		3.40E+00	3.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	CFS-L11-1316-T01-A	1	1.94E+01			1.94E+01	3.9E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1316-T02-A	1	1.69E+01			1.69E+01	1.8E+01	1.9E+00	6.0E+00	10	100	8.62E+02	85%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1316-T03-A	1	1.63E+01			1.63E+01	2.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1316-T04-A	1	1.39E+01			1.39E+01	4.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1316-T05-A	1	2.40E+01			2.40E+01	4.4E+00	1.9E+00	6.0E+00					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1316-T01-B	1	1.78E+01			1.78E+01	9.5E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1316-T02-B	1	1.80E+01			1.80E+01	3.1E+00	1.9E+00	6.0E+00	10	100	8.87E+02	87%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1316-T03-B	1	1.75E+01			1.75E+01	1.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1316-T04-B	1	1.43E+01			1.43E+01	4.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1316-T05-B	1	2.57E+01			2.57E+01	3.2E+00	1.9E+00	6.0E+00					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1316-T01-C	1	1.89E+01			1.89E+01	3.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1316-T02-C	1	2.03E+01			2.03E+01	4.1E+00	1.9E+00	6.0E+00	10	100	8.91E+02	87%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1316-T03-C	1	1.67E+01			1.67E+01	4.1E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1316-T04-C	1	1.48E+01			1.48E+01	2.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1316-T05-C	1	2.26E+01			2.26E+01	1.4E+01	1.9E+00	6.0E+00					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1316-B01-A	1	6.07E+00			6.07E+00	2.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1316-B02-A	1	6.02E+00			6.02E+00	2.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
Li	CFS-L11-1316-B03-A	1	5.51E+00	E		5.51E+00	2.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	CFS-L11-1316-T01-A	1	1.12E+03			1.12E+03	3.5E-02	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1316-T02-A	1	1.48E+03			1.48E+03	7.1E+01	2.0E+00	6.4E+00	10	100	2.52E+03	104%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1316-T03-A	1	4.10E+03			4.10E+03	4.2E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1316-T04-A	1	2.88E+03			2.88E+03	1.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1316-T05-A	1	1.12E+04			1.12E+04	3.3E-01	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1316-T01-B	1	1.16E+03			1.16E+03	5.5E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1316-T02-B	1	2.07E+03			2.07E+03	3.0E-01	2.0E+00	6.4E+00	10	100	3.10E+03	103%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1316-T03-B	1	4.06E+03			4.06E+03	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1316-T04-B	1	5.61E+03			5.61E+03	6.3E-01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1316-T05-B	1	1.11E+04			1.11E+04	1.3E+00	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1316-T01-C	1	1.16E+03			1.16E+03	1.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1316-T02-C	1	2.09E+03			2.09E+03	1.6E+00	2.0E+00	6.4E+00	10	100	3.02E+03	93%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1316-T03-C	1	4.00E+03			4.00E+03	2.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1316-T04-C	1	7.20E+03			7.20E+03	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1316-T05-C	1	1.13E+04			1.13E+04	6.8E-01	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	5.6E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1316-B02-A	1	2.30E+00	E		2.30E+00	1.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
Mn	CFS-L11-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	6.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	CFS-L11-1316-T01-A	1	6.59E+04			6.59E+04	1.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1316-T02-A	1	8.06E+04			8.06E+04	8.1E+01	1.0E+00	3.2E+00	1000	100	8.16E+04	96%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1316-T03-A	1	2.85E+05			2.85E+05	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1316-T04-A	1	2.34E+05			2.34E+05	1.3E+02	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1316-T05-A	1	9.09E+05			9.09E+05	5.5E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1316-T01-B	1	6.76E+04			6.76E+04	4.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1316-T02-B	1	1.26E+05			1.26E+05	8.7E-01	1.0E+00	3.2E+00	1000	100	1.27E+05	99%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1316-T03-B	1	2.90E+05			2.90E+05	8.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1316-T04-B	1	4.70E+05			4.70E+05	6.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1316-T05-B	1	9.10E+05			9.10E+05	1.2E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1316-T01-C	1	6.93E+04			6.93E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1316-T02-C	1	1.30E+05			1.30E+05	7.7E-01	1.0E+00	3.2E+00	1000	100	1.30E+05	95%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1316-T03-C	1	2.78E+05			2.78E+05	2.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1316-T04-C	1	5.05E+05			5.05E+05	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1316-T05-C	1	9.13E+05			9.13E+05	6.3E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	4.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1316-B02-A	1	1.91E+00	E		1.91E+00	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
Mg	CFS-L11-1316-B03-A	1	2.70E+00	E		2.70E+00	1.4E+02	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	CFS-L11-1316-T01-A	1	1.03E+01			1.03E+01	1.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1316-T02-A	1	7.47E+00			7.47E+00	7.2E+01	1.2E+00	3.8E+00	10	100	9.50E+02	94%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1316-T03-A	1	1.46E+01			1.46E+01	1.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1316-T04-A	1	8.93E+00			8.93E+00	1.1E+02	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1316-T05-A	1	1.79E+01			1.79E+01	1.2E+01	1.2E+00	3.8E+00					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1316-T01-B	1	1.01E+01			1.01E+01	1.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1316-T02-B	1	9.78E+00			9.78E+00	5.5E+00	1.2E+00	3.8E+00	10	100	9.88E+02	98%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1316-T03-B	1	1.48E+01			1.48E+01	7.9E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1316-T04-B	1	1.64E+01			1.64E+01	8.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1316-T05-B	1	2.07E+01			2.07E+01	3.6E+00	1.2E+00	3.8E+00					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1316-T01-C	1	1.01E+01			1.01E+01	9.5E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1316-T02-C	1	1.10E+01			1.10E+01	1.2E+01	1.2E+00	3.8E+00	10	100	9.84E+02	97%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1316-T03-C	1	1.27E+01			1.27E+01	8.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1316-T04-C	1	1.49E+01			1.49E+01	7.1E+00	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1316-T05-C	1	1.78E+01			1.78E+01	9.0E+00	1.2E+00	3.8E+00					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1316-B01-A	1	2.45E+00	E		2.45E+00	2.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1316-B02-A	1	2.24E+00	E		2.24E+00	5.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
Mo	CFS-L11-1316-B03-A	1	1.46E+00	E		1.46E+00	4.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	CFS-L11-1316-T01-A	1	1.40E+02			1.40E+02	2.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1316-T02-A	1	1.33E+02			1.33E+02	8.7E+01	1.8E+00	5.7E+00	10	100	1.03E+03	89%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1316-T03-A	1	3.73E+02			3.73E+02	1.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1316-T04-A	1	2.17E+02			2.17E+02	1.4E+02	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1316-T05-A	1	8.82E+02			8.82E+02	8.5E-01	1.8E+00	5.7E+00					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1316-T01-B	1	1.47E+02			1.47E+02	7.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1316-T02-B	1	2.24E+02			2.24E+02	9.2E-01	1.8E+00	5.7E+00	10	100	1.17E+03	94%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1316-T03-B	1	3.75E+02			3.75E+02	3.9E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1316-T04-B	1	4.52E+02			4.52E+02	1.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1316-T05-B	1	8.70E+02			8.70E+02	1.0E+00	1.8E+00	5.7E+00					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1316-T01-C	1	1.47E+02			1.47E+02	4.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1316-T02-C	1	2.25E+02			2.25E+02	2.1E+00	1.8E+00	5.7E+00	10	100	1.17E+03	94%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1316-T03-C	1	3.59E+02			3.59E+02	1.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1316-T04-C	1	6.13E+02			6.13E+02	4.2E-01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1316-T05-C	1	8.89E+02			8.89E+02	2.4E-01	1.8E+00	5.7E+00					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	5.4E+00	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1316-B02-A	1	9.00E-01	U1/2		9.00E-01	5.9E+01	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
Ni	CFS-L11-1316-B03-A	1	9.00E-01	U1/2		9.00E-01	1.8E+03	1.8E+00	5.7E+00				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	CFS-L11-1316-T01-A	1	2.53E+01			2.53E+01	1.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1316-T02-A	1	3.68E+01			3.68E+01	2.9E+01	3.7E+00	1.2E+01	1000	100	9.92E+02	96%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1316-T03-A	1	4.15E+01			4.15E+01	2.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1316-T04-A	1	2.40E+01			2.40E+01	7.1E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1316-T05-A	1	5.20E+01			5.20E+01	2.1E+01	3.7E+00	1.2E+01					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1316-T01-B	1	3.64E+01			3.64E+01	3.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1316-T02-B	1	3.06E+01			3.06E+01	2.7E+01	3.7E+00	1.2E+01	1000	100	9.66E+02	94%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1316-T03-B	1	5.10E+01			5.10E+01	1.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1316-T04-B	1	5.57E+01			5.57E+01	1.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1316-T05-B	1	3.37E+01			3.37E+01	5.5E+01	3.7E+00	1.2E+01					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1316-T01-C	1	3.36E+01			3.36E+01	5.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1316-T02-C	1	3.00E+01			3.00E+01	3.2E+01	3.7E+00	1.2E+01	1000	100	9.95E+02	96%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1316-T03-C	1	4.20E+01			4.20E+01	2.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1316-T04-C	1	3.92E+01			3.92E+01	1.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1316-T05-C	1	5.03E+01			5.03E+01	2.8E+01	3.7E+00	1.2E+01					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1316-B01-A	1	3.47E+01			3.47E+01	1.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1316-B02-A	1	3.88E+01			3.88E+01	2.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
P	CFS-L11-1316-B03-A	1	3.27E+01			3.27E+01	3.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	CFS-L11-1316-T01-A	1	9.25E+03			9.25E+03	1.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1316-T02-A	1	9.10E+03			9.10E+03	9.0E+01	1.6E+00	5.1E+00	1000	100	1.02E+04	112%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1316-T03-A	1	3.17E+04			3.17E+04	4.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1316-T04-A	1	2.19E+04			2.19E+04	1.5E+02	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1316-T05-A	1	7.11E+04			7.11E+04	8.4E-01	1.6E+00	5.1E+00					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1316-T01-B	1	9.69E+03			9.69E+03	1.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1316-T02-B	1	1.62E+04			1.62E+04	1.5E-01	1.6E+00	5.1E+00	1000	100	1.72E+04	91%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1316-T03-B	1	3.17E+04			3.17E+04	8.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1316-T04-B	1	4.65E+04			4.65E+04	2.2E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1316-T05-B	1	7.11E+04			7.11E+04	1.2E+00	1.6E+00	5.1E+00					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1316-T01-C	1	9.70E+03			9.70E+03	7.5E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1316-T02-C	1	1.65E+04			1.65E+04	2.0E+00	1.6E+00	5.1E+00	1000	100	1.75E+04	99%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1316-T03-C	1	3.07E+04			3.07E+04	3.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1316-T04-C	1	4.78E+04			4.78E+04	6.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1316-T05-C	1	7.09E+04			7.09E+04	5.5E-01	1.6E+00	5.1E+00					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1316-B01-A	1	6.40E+01			6.40E+01	4.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1316-B02-A	1	7.31E+01			7.31E+01	1.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
K	CFS-L11-1316-B03-A	1	6.40E+01			6.40E+01	1.6E+00	1.6E+00	5.1E+00				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	CFS-L11-1316-T01-A	1	6.87E+01			6.87E+01	7.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1316-T02-A	1	6.52E+01			6.52E+01	1.1E+02	1.5E+01	4.8E+01	10	100	1.00E+03	94%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1316-T03-A	1	2.63E+02			2.63E+02	2.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1316-T04-A	1	1.91E+02			1.91E+02	1.5E+02	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1316-T05-A	1	7.31E+02			7.31E+02	4.2E+00	1.5E+01	4.8E+01					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1316-T01-B	1	7.53E+01			7.53E+01	1.7E+01	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1316-T02-B	1	1.22E+02			1.22E+02	7.1E+00	1.5E+01	4.8E+01	10	100	1.05E+03	93%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1316-T03-B	1	2.56E+02			2.56E+02	5.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1316-T04-B	1	3.98E+02			3.98E+02	1.8E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1316-T05-B	1	7.35E+02			7.35E+02	2.6E+00	1.5E+01	4.8E+01					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1316-T01-C	1	8.05E+01			8.05E+01	1.4E+01	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1316-T02-C	1	1.16E+02			1.16E+02	1.9E+01	1.5E+01	4.8E+01	10	100	1.04E+03	92%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1316-T03-C	1	2.55E+02			2.55E+02	4.2E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1316-T04-C	1	4.27E+02			4.27E+02	3.1E+00	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1316-T05-C	1	7.58E+02			7.58E+02	5.6E+00	1.5E+01	4.8E+01					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1316-B01-A	1	7.50E+00	U1/2		7.50E+00	2.8E+02	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1316-B02-A	1	7.50E+00	U1/2		7.50E+00	9.9E+01	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
Se	CFS-L11-1316-B03-A	1	7.50E+00	U1/2		7.50E+00	7.4E+01	1.5E+01	4.8E+01				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	CFS-L11-1316-T01-A	1	3.26E+03			3.26E+03	1.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1316-T02-A	1	3.24E+03			3.24E+03	7.7E+01	1.1E+00	3.5E+00	1000	100	4.22E+03	98%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1316-T03-A	1	5.49E+03			5.49E+03	1.5E+00	1.1E+00	3.5E+00				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1316-T04-A	1	2.78E+03			2.78E+03	1.4E+02	1.1E+00	3.5E+00				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1316-T05-A	1	6.74E+03			6.74E+03	7.2E-01	1.1E+00	3.5E+00					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1316-T01-B	1	3.43E+03			3.43E+03	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1316-T02-B	1	4.28E+03			4.28E+03	7.2E-02	1.1E+00	3.5E+00	1000	100	5.20E+03	92%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1316-T03-B	1	5.47E+03			5.47E+03	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1316-T04-B	1	5.59E+03			5.59E+03	2.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1316-T05-B	1	6.68E+03			6.68E+03	1.2E+00	1.1E+00	3.5E+00					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1316-T01-C	1	3.39E+03			3.39E+03	7.2E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1316-T02-C	1	4.39E+03			4.39E+03	2.9E+00	1.1E+00	3.5E+00	1000	100	5.31E+03	92%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1316-T03-C	1	5.55E+03			5.55E+03	3.7E+00	1.1E+00	3.5E+00				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1316-T04-C	1	6.22E+03			6.22E+03	4.4E-01	1.1E+00	3.5E+00				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1316-T05-C	1	6.70E+03			6.70E+03	4.4E-01	1.1E+00	3.5E+00					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1316-B01-A	1	5.58E+00			5.58E+00	2.6E+01	1.1E+00	3.5E+00				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1316-B02-A	1	2.38E+00	E		2.38E+00	6.9E+01	1.1E+00	3.5E+00				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
Si	CFS-L11-1316-B03-A	1	5.50E-01	U1/2		5.50E-01	1.8E+02	1.1E+00	3.5E+00				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	CFS-L11-1316-T01-A	1	2.35E+04			2.35E+04	7.8E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1316-T02-A	1	2.50E+04			2.50E+04	7.5E+01	2.5E+00	8.0E+00	1000	100	2.58E+04	88%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1316-T03-A	1	9.17E+04			9.17E+04	4.7E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1316-T04-A	1	6.26E+04			6.26E+04	1.2E+02	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1316-T05-A	1	2.12E+05			2.12E+05	8.2E-01	2.5E+00	8.0E+00					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1316-T01-B	1	2.43E+04			2.43E+04	3.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1316-T02-B	1	4.46E+04			4.46E+04	7.7E-01	2.5E+00	8.0E+00	1000	100	4.55E+04	91%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1316-T03-B	1	9.17E+04			9.17E+04	5.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1316-T04-B	1	1.34E+05			1.34E+05	2.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1316-T05-B	1	2.12E+05			2.12E+05	2.8E-01	2.5E+00	8.0E+00					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1316-T01-C	1	2.39E+04			2.39E+04	2.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1316-T02-C	1	4.31E+04			4.31E+04	1.8E+00	2.5E+00	8.0E+00	1000	100	4.41E+04	95%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1316-T03-C	1	8.88E+04			8.88E+04	2.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1316-T04-C	1	1.36E+05			1.36E+05	1.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1316-T05-C	1	2.11E+05			2.11E+05	3.8E-01	2.5E+00	8.0E+00					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1316-B01-A	1	1.73E+01			1.73E+01	1.6E+01	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1316-B02-A	1	2.34E+01			2.34E+01	1.3E+00	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
Na	CFS-L11-1316-B03-A	1	2.74E+01			2.74E+01	4.9E+00	2.5E+00	8.0E+00				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	CFS-L11-1316-T01-A	1	1.50E+03			1.50E+03	5.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1316-T02-A	1	1.51E+03			1.51E+03	8.0E+01	1.0E+00	3.2E+00	1000	100	2.55E+03	104%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1316-T03-A	1	3.23E+03			3.23E+03	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1316-T04-A	1	2.03E+03			2.03E+03	1.3E+02	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1316-T05-A	1	4.15E+03			4.15E+03	3.9E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1316-T01-B	1	1.55E+03			1.55E+03	8.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1316-T02-B	1	2.10E+03			2.10E+03	5.0E-01	1.0E+00	3.2E+00	1000	100	3.01E+03	91%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1316-T03-B	1	3.31E+03			3.31E+03	9.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1316-T04-B	1	4.12E+03			4.12E+03	1.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1316-T05-B	1	4.16E+03			4.16E+03	8.1E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1316-T01-C	1	1.52E+03			1.52E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1316-T02-C	1	2.18E+03			2.18E+03	2.1E+00	1.0E+00	3.2E+00	1000	100	3.23E+03	104%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1316-T03-C	1	3.31E+03			3.31E+03	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1316-T04-C	1	3.59E+03			3.59E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1316-T05-C	1	4.15E+03			4.15E+03	1.5E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1316-B02-A	1	5.00E-01	U1/2		5.00E-01	1.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
Sr	CFS-L11-1316-B03-A	1	5.00E-01	U1/2		5.00E-01	9.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	CFS-L11-1316-T01-A	1	5.98E+05			5.98E+05	5.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1316-T02-A	1	3.82E+05			3.82E+05	8.8E+01	6.8E+00	2.2E+01	1000	100	3.83E+05	89%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1316-T03-A	1	8.54E+05			8.54E+05	3.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1316-T04-A	1	5.05E+05			5.05E+05	1.4E+02	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1316-T05-A	1	1.50E+06			1.50E+06	5.6E-01	6.8E+00	2.2E+01					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1316-T01-B	1	6.18E+05			6.18E+05	1.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1316-T02-B	1	6.73E+05			6.73E+05	2.9E-01	6.8E+00	2.2E+01	1000	100	6.74E+05	90%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1316-T03-B	1	8.66E+05			8.66E+05	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1316-T04-B	1	1.04E+06			1.04E+06	5.2E-04	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1316-T05-B	1	1.51E+06			1.51E+06	1.1E+00	6.8E+00	2.2E+01					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1316-T01-C	1	6.22E+05			6.22E+05	9.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1316-T02-C	1	6.84E+05			6.84E+05	1.7E+00	6.8E+00	2.2E+01	1000	100	6.85E+05	93%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1316-T03-C	1	8.37E+05			8.37E+05	9.0E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1316-T04-C	1	1.09E+06			1.09E+06	4.7E-01	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1316-T05-C	1	1.52E+06			1.52E+06	3.6E-01	6.8E+00	2.2E+01					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	3.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1316-B02-A	1	1.56E+01	E		1.56E+01	1.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
S	CFS-L11-1316-B03-A	1	3.40E+00	U1/2		3.40E+00	2.7E+00	6.8E+00	2.2E+01				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	CFS-L11-1316-T01-A	1	2.31E+02			2.31E+02	1.3E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1316-T02-A	1	2.03E+02			2.03E+02	8.8E+01	4.6E+00	1.5E+01	10	100	1.11E+03	91%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1316-T03-A	1	5.71E+02			5.71E+02	4.0E-01	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1316-T04-A	1	3.59E+02			3.59E+02	1.4E+02	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1316-T05-A	1	1.09E+03			1.09E+03	6.2E-01	4.6E+00	1.5E+01					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1316-T01-B	1	2.40E+02			2.40E+02	3.7E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1316-T02-B	1	3.56E+02			3.56E+02	1.0E+00	4.6E+00	1.5E+01	10	100	1.26E+03	90%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1316-T03-B	1	5.86E+02			5.86E+02	5.2E-01	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1316-T04-B	1	7.57E+02			7.57E+02	6.9E-01	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1316-T05-B	1	1.12E+03			1.12E+03	1.7E+00	4.6E+00	1.5E+01					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1316-T01-C	1	2.50E+02			2.50E+02	2.5E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1316-T02-C	1	3.61E+02			3.61E+02	3.8E+00	4.6E+00	1.5E+01	10	100	1.26E+03	90%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1316-T03-C	1	5.54E+02			5.54E+02	1.1E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1316-T04-C	1	8.05E+02			8.05E+02	1.1E+00	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1316-T05-C	1	1.10E+03			1.10E+03	1.0E+00	4.6E+00	1.5E+01					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1316-B01-A	1	2.30E+00	U1/2		2.30E+00	9.3E+01	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1316-B02-A	1	2.30E+00	U1/2		2.30E+00	2.7E+01	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
Tl	CFS-L11-1316-B03-A	1	2.30E+00	U1/2		2.30E+00	6.3E+02	4.6E+00	1.5E+01				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	CFS-L11-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	7.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00	10	100	9.54E+02	95%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	5.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	2.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1316-T05-A	1	1.00E+00	U1/2		1.00E+00	1.5E+01	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	4.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	1.8E+01	2.0E+00	6.4E+00	10	100	9.50E+02	95%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	4.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1316-T05-B	1	1.00E+00	U1/2		1.00E+00	2.9E+00	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	3.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	7.9E-01	2.0E+00	6.4E+00	10	100	9.59E+02	96%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	2.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	4.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1316-T05-C	1	1.00E+00	U1/2		1.00E+00	5.1E+00	2.0E+00	6.4E+00					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	7.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1316-B02-A	1	1.00E+00	U1/2		1.00E+00	3.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
Ti	CFS-L11-1316-B03-A	1	1.00E+00	U1/2		1.00E+00	3.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	CFS-L11-1316-T01-A	1	4.25E+01			4.25E+01	3.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1316-T02-A	1	2.45E+01			2.45E+01	8.6E+01	1.5E+00	4.8E+00	10	100	1.01E+03	99%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1316-T03-A	1	3.95E+01			3.95E+01	2.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1316-T04-A	1	1.80E+01			1.80E+01	1.4E+02	1.5E+00	4.8E+00				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1316-T05-A	1	3.27E+01			3.27E+01	2.5E+00	1.5E+00	4.8E+00					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1316-T01-B	1	4.44E+01			4.44E+01	7.9E-01	1.5E+00	4.8E+00				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1316-T02-B	1	4.09E+01			4.09E+01	9.0E-01	1.5E+00	4.8E+00	10	100	1.05E+03	101%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1316-T03-B	1	3.99E+01			3.99E+01	8.8E-01	1.5E+00	4.8E+00				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1316-T04-B	1	3.61E+01			3.61E+01	2.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1316-T05-B	1	3.44E+01			3.44E+01	1.2E+00	1.5E+00	4.8E+00					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1316-T01-C	1	4.44E+01			4.44E+01	4.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1316-T02-C	1	4.26E+01			4.26E+01	4.7E+00	1.5E+00	4.8E+00	10	100	1.05E+03	101%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1316-T03-C	1	3.94E+01			3.94E+01	2.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1316-T04-C	1	3.55E+01			3.55E+01	2.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1316-T05-C	1	3.27E+01			3.27E+01	2.5E+00	1.5E+00	4.8E+00					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1316-B01-A	1	7.50E-01	U1/2		7.50E-01	2.8E+02	1.5E+00	4.8E+00				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1316-B02-A	1	7.50E-01	U1/2		7.50E-01	7.7E+01	1.5E+00	4.8E+00				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
V	CFS-L11-1316-B03-A	1	7.50E-01	U1/2		7.50E-01	8.0E+01	1.5E+00	4.8E+00				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	CFS-L11-1316-T01-A	1	1.50E+04			1.50E+04	1.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:01 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1316-T02-A	1	1.51E+04			1.51E+04	7.2E+01	1.0E+00	3.2E+00	10	100	1.60E+04	88%	VU ICP-OES	5/31/11 11:03 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1316-T03-A	1	3.18E+04			3.18E+04	9.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:05 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1316-T04-A	1	1.96E+04			1.96E+04	1.1E+02	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:06 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1316-T05-A	1	6.53E+04			6.53E+04	7.8E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 11:08 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1316-T01-B	1	1.60E+04			1.60E+04	7.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:10 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1316-T02-B	1	2.20E+04			2.20E+04	2.4E-01	1.0E+00	3.2E+00	10	100	2.29E+04	90%	VU ICP-OES	5/31/11 11:11 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1316-T03-B	1	3.14E+04			3.14E+04	9.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:13 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1316-T04-B	1	3.61E+04			3.61E+04	9.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:14 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1316-T05-B	1	6.52E+04			6.52E+04	1.6E+00	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 11:16 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1316-T01-C	1	1.56E+04			1.56E+04	7.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:18 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1316-T02-C	1	2.19E+04			2.19E+04	9.7E-01	1.0E+00	3.2E+00	10	100	2.28E+04	94%	VU ICP-OES	5/31/11 11:19 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1316-T03-C	1	3.07E+04			3.07E+04	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:21 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1316-T04-C	1	4.98E+04			4.98E+04	6.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:23 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1316-T05-C	1	6.57E+04			6.57E+04	2.2E-01	1.0E+00	3.2E+00					VU ICP-OES	5/31/11 11:24 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1316-B01-A	1	1.77E+00	E		1.77E+00	1.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:56 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1316-B02-A	1	1.61E+00	E		1.61E+00	3.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 10:58 AM	EPA Interlab L11 1313-1316 CFS
Zn	CFS-L11-1316-B03-A	1	1.61E+00	E		1.61E+00	2.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	5/31/11 11:00 AM	EPA Interlab L11 1313-1316 CFS

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	CFS-LRef-1316-T01-A	1	4.85E+01			4.85E+01	9.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1316-T02-A	1	4.35E+01			4.35E+01	5.3E+00	1.0E+00	3.2E+00	1000	100	1.10E+03	106%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1316-T03-A	1	4.07E+01			4.07E+01	5.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1316-T04-A	1	5.68E+01			5.68E+01	3.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1316-T01-B	1	4.33E+01			4.33E+01	8.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1316-T02-B	1	5.21E+01			5.21E+01	5.2E+00	1.0E+00	3.2E+00	1000	100	1.01E+03	96%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1316-T03-B	1	5.38E+01			5.38E+01	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1316-T04-B	1	5.07E+01			5.07E+01	2.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1316-T01-C	1	4.18E+01			4.18E+01	3.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1316-T02-C	1	4.38E+01			4.38E+01	3.5E+00	1.0E+00	3.2E+00	1000	100	1.15E+03	111%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1316-T03-C	1	5.64E+01			5.64E+01	1.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1316-T04-C	1	5.05E+01			5.05E+01	3.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.6E+01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	CFS-LRef-1316-T01-A	1	4.01E+01			4.01E+01	1.1E+01	7.5E+00	2.4E+01				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1316-T02-A	1	3.50E+01			3.50E+01	2.8E+01	7.5E+00	2.4E+01	10	120	1.35E+03	110%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1316-T03-A	1	4.86E+01			4.86E+01	6.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1316-T04-A	1	5.37E+01			5.37E+01	2.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1316-T01-B	1	2.44E+01			2.44E+01	3.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1316-T02-B	1	3.45E+01			3.45E+01	1.1E+01	7.5E+00	2.4E+01	10	100	1.03E+03	99%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1316-T03-B	1	5.34E+01			5.34E+01	1.9E+01	7.5E+00	2.4E+01				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1316-T04-B	1	5.91E+01			5.91E+01	2.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1316-T01-C	1	3.50E+01			3.50E+01	2.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1316-T02-C	1	4.39E+01			4.39E+01	9.4E+00	7.5E+00	2.4E+01	10	100	1.14E+03	109%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1316-T03-C	1	5.00E+01			5.00E+01	3.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1316-T04-C	1	5.11E+01			5.11E+01	2.2E+01	7.5E+00	2.4E+01				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1316-B01-A	1	3.75E+00	U1/2		3.75E+00	5.0E+03	7.5E+00	2.4E+01				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	CFS-LRef-1316-T01-A	1	1.28E+01	E		1.28E+01	6.7E+01	1.1E+01	3.5E+01				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1316-T02-A	1	1.62E+01	E		1.62E+01	4.7E+01	1.1E+01	3.5E+01	10	120	1.34E+03	110%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1316-T03-A	1	2.28E+01	E		2.28E+01	9.1E+01	1.1E+01	3.5E+01				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1316-T04-A	1	2.84E+01	E		2.84E+01	1.3E+01	1.1E+01	3.5E+01				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1316-T01-B	1	1.75E+01	E		1.75E+01	3.7E+01	1.1E+01	3.5E+01				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1316-T02-B	1	1.79E+01	E		1.79E+01	4.9E+01	1.1E+01	3.5E+01	10	100	1.02E+03	100%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1316-T03-B	1	3.08E+01	E		3.08E+01	3.8E+01	1.1E+01	3.5E+01				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1316-T04-B	1	3.63E+01			3.63E+01	2.7E+01	1.1E+01	3.5E+01				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1316-T01-C	1	1.42E+01	E		1.42E+01	2.6E+01	1.1E+01	3.5E+01				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1316-T02-C	1	1.53E+01	E		1.53E+01	1.1E+01	1.1E+01	3.5E+01	10	100	1.12E+03	111%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1316-T03-C	1	2.99E+01	E		2.99E+01	3.1E+01	1.1E+01	3.5E+01				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1316-T04-C	1	2.56E+01	E		2.56E+01	2.4E+01	1.1E+01	3.5E+01				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1316-B01-A	1	5.50E+00	U1/2		5.50E+00	8.1E+02	1.1E+01	3.5E+01				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	CFS-LRef-1316-T01-A	1	2.37E+02			2.37E+02	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1316-T02-A	1	3.63E+02			3.63E+02	9.6E-01	1.0E+00	3.2E+00	1000	100	1.39E+03	102%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1316-T03-A	1	6.12E+02			6.12E+02	6.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1316-T04-A	1	1.06E+03			1.06E+03	1.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1316-T01-B	1	2.06E+02			2.06E+02	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1316-T02-B	1	3.27E+02			3.27E+02	2.0E+00	1.0E+00	3.2E+00	1000	100	1.26E+03	93%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1316-T03-B	1	6.56E+02			6.56E+02	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1316-T04-B	1	1.04E+03			1.04E+03	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1316-T01-C	1	1.84E+02			1.84E+02	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1316-T02-C	1	3.15E+02			3.15E+02	1.2E+00	1.0E+00	3.2E+00	1000	100	1.37E+03	106%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1316-T03-C	1	6.53E+02			6.53E+02	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1316-T04-C	1	1.02E+03			1.02E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1316-B01-A	1	9.09E+01			9.09E+01	7.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	CFS-LRef-1316-T01-A	1	9.73E+01			9.73E+01	3.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1316-T02-A	1	8.78E+01			8.78E+01	6.3E-01	1.0E+00	3.2E+00	10	120	1.42E+03	111%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1316-T03-A	1	6.22E+01			6.22E+01	7.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1316-T04-A	1	6.17E+01			6.17E+01	7.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1316-T01-B	1	9.48E+01			9.48E+01	2.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1316-T02-B	1	8.64E+01			8.64E+01	2.4E+00	1.0E+00	3.2E+00	10	100	1.09E+03	100%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1316-T03-B	1	7.36E+01			7.36E+01	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1316-T04-B	1	6.09E+01			6.09E+01	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1316-T01-C	1	9.40E+01			9.40E+01	5.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1316-T02-C	1	8.75E+01			8.75E+01	1.0E+00	1.0E+00	3.2E+00	10	100	1.21E+03	112%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1316-T03-C	1	7.59E+01			7.59E+01	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1316-T04-C	1	6.03E+01			6.03E+01	5.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	2.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	CFS-LRef-1316-T01-A	1	9.50E-01	U1/2		9.50E-01	4.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1316-T02-A	1	9.50E-01	U1/2		9.50E-01	9.6E+01	1.9E+00	6.0E+00	10	120	1.37E+03	114%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1316-T03-A	1	9.50E-01	U1/2		9.50E-01	6.0E+01	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1316-T04-A	1	9.50E-01	U1/2		9.50E-01	3.9E+01	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1316-T01-B	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1316-T02-B	1	9.50E-01	U1/2		9.50E-01	5.6E+01	1.9E+00	6.0E+00	10	100	1.01E+03	101%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1316-T03-B	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1316-T04-B	1	9.50E-01	U1/2		9.50E-01	6.6E+01	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1316-T01-C	1	9.50E-01	U1/2		9.50E-01	1.2E+02	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1316-T02-C	1	9.50E-01	U1/2		9.50E-01	6.8E+01	1.9E+00	6.0E+00	10	100	1.13E+03	113%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1316-T03-C	1	9.50E-01	U1/2		9.50E-01	5.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1316-T04-C	1	9.50E-01	U1/2		9.50E-01	5.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	7.5E+01	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	CFS-LRef-1316-T01-A	1	5.19E+03			5.19E+03	5.4E-01	2.2E+00	7.0E+00				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1316-T02-A	1	7.46E+03			7.46E+03	8.9E-01	2.2E+00	7.0E+00	10	120	8.70E+03	103%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1316-T03-A	1	1.11E+04			1.11E+04	6.9E-01	2.2E+00	7.0E+00				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1316-T04-A	1	1.33E+04			1.33E+04	9.6E-01	2.2E+00	7.0E+00				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1316-T01-B	1	5.20E+03			5.20E+03	9.5E-01	2.2E+00	7.0E+00				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1316-T02-B	1	7.40E+03			7.40E+03	2.3E+00	2.2E+00	7.0E+00	10	100	8.35E+03	95%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1316-T03-B	1	1.08E+04			1.08E+04	1.6E+00	2.2E+00	7.0E+00				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1316-T04-B	1	1.35E+04			1.35E+04	1.9E+00	2.2E+00	7.0E+00				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1316-T01-C	1	5.30E+03			5.30E+03	3.9E-01	2.2E+00	7.0E+00				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1316-T02-C	1	7.64E+03			7.64E+03	5.4E-01	2.2E+00	7.0E+00	10	100	8.65E+03	101%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1316-T03-C	1	1.11E+04			1.11E+04	1.9E+00	2.2E+00	7.0E+00				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1316-T04-C	1	1.34E+04			1.34E+04	9.2E-01	2.2E+00	7.0E+00				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1316-B01-A	1	1.10E+00	U1/2		1.10E+00	7.0E+01	2.2E+00	7.0E+00				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	CFS-LRef-1316-T01-A	1	6.81E+05			6.81E+05	4.5E-01	2.6E+00	8.3E+00				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1316-T02-A	1	6.56E+05			6.56E+05	7.6E-01	2.6E+00	8.3E+00	1000	100	6.57E+05	90%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1316-T03-A	1	5.71E+05			5.71E+05	6.0E+01	2.6E+00	8.3E+00				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1316-T04-A	1	5.77E+05			5.77E+05	4.8E-01	2.6E+00	8.3E+00				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1316-T01-B	1	6.74E+05			6.74E+05	8.0E-01	2.6E+00	8.3E+00				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1316-T02-B	1	6.48E+05			6.48E+05	2.4E+00	2.6E+00	8.3E+00	1000	100	6.49E+05	87%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1316-T03-B	1	6.12E+05			6.12E+05	1.8E+00	2.6E+00	8.3E+00				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1316-T04-B	1	5.83E+05			5.83E+05	1.2E+00	2.6E+00	8.3E+00				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1316-T01-C	1	6.77E+05			6.77E+05	3.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1316-T02-C	1	6.52E+05			6.52E+05	1.1E-01	2.6E+00	8.3E+00	1000	100	6.53E+05	89%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1316-T03-C	1	6.26E+05			6.26E+05	1.9E+00	2.6E+00	8.3E+00				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1316-T04-C	1	5.78E+05			5.78E+05	1.0E+00	2.6E+00	8.3E+00				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1316-B01-A	1	3.57E+01			3.57E+01	1.7E+01	2.6E+00	8.3E+00				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	CFS-LRef-1316-T01-A	1	6.00E-01	U1/2		6.00E-01	2.7E+02	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1316-T02-A	1	6.00E-01	U1/2		6.00E-01	9.6E+01	1.2E+00	3.8E+00	10	120	1.30E+03	109%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1316-T03-A	1	6.00E-01	U1/2		6.00E-01	8.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1316-T04-A	1	6.00E-01	U1/2		6.00E-01	1.7E+02	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1316-T01-B	1	6.00E-01	U1/2		6.00E-01	6.7E+02	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1316-T02-B	1	6.00E-01	U1/2		6.00E-01	9.2E+02	1.2E+00	3.8E+00	10	100	9.68E+02	97%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1316-T03-B	1	6.00E-01	U1/2		6.00E-01	4.8E+02	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1316-T04-B	1	6.00E-01	U1/2		6.00E-01	6.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1316-T01-C	1	6.00E-01	U1/2		6.00E-01	1.8E+02	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1316-T02-C	1	6.00E-01	U1/2		6.00E-01	4.8E+01	1.2E+00	3.8E+00	10	100	1.10E+03	110%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1316-T03-C	1	6.00E-01	U1/2		6.00E-01	5.0E+02	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1316-T04-C	1	6.00E-01	U1/2		6.00E-01	3.7E+02	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	1.5E+02	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	CFS-LRef-1316-T01-A	1	1.22E+02			1.22E+02	4.3E-01	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1316-T02-A	1	2.12E+02			2.12E+02	3.9E-01	1.8E+00	5.7E+00	10	120	1.47E+03	105%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1316-T03-A	1	3.94E+02			3.94E+02	6.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1316-T04-A	1	5.70E+02			5.70E+02	2.7E-01	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1316-T01-B	1	1.18E+02			1.18E+02	5.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1316-T02-B	1	2.07E+02			2.07E+02	2.1E+00	1.8E+00	5.7E+00	10	100	1.14E+03	93%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1316-T03-B	1	3.97E+02			3.97E+02	1.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1316-T04-B	1	5.82E+02			5.82E+02	1.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1316-T01-C	1	1.21E+02			1.21E+02	4.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1316-T02-C	1	2.13E+02			2.13E+02	7.1E-01	1.8E+00	5.7E+00	10	100	1.28E+03	107%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1316-T03-C	1	4.00E+02			4.00E+02	2.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1316-T04-C	1	5.81E+02			5.81E+02	8.8E-01	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	1.3E+02	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	CFS-LRef-1316-T01-A	1	1.08E+03			1.08E+03	4.7E-01	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1316-T02-A	1	1.38E+03			1.38E+03	2.1E+00	3.7E+00	1.2E+01	10	120	2.58E+03	100%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1316-T03-A	1	2.44E+03			2.44E+03	3.0E+01	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1316-T04-A	1	3.81E+03			3.81E+03	1.7E+00	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1316-T01-B	1	1.12E+03			1.12E+03	9.3E-01	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1316-T02-B	1	1.36E+03			1.36E+03	2.3E+00	3.7E+00	1.2E+01	10	100	2.23E+03	87%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1316-T03-B	1	2.63E+03			2.63E+03	1.9E+00	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1316-T04-B	1	3.93E+03			3.93E+03	9.0E-01	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1316-T01-C	1	1.14E+03			1.14E+03	5.8E-01	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1316-T02-C	1	1.39E+03			1.39E+03	1.1E+00	3.7E+00	1.2E+01	10	100	2.44E+03	105%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1316-T03-C	1	2.62E+03			2.62E+03	1.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1316-T04-C	1	3.85E+03			3.85E+03	1.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1316-B01-A	1	1.85E+00	U1/2		1.85E+00	8.3E+00	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	CFS-LRef-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	5.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	4.2E+01	2.0E+00	6.4E+00	1000	100	1.10E+03	110%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	8.6E+01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	7.5E+02	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	3.1E+01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	3.5E+00	2.0E+00	6.4E+00	1000	100	9.66E+02	96%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	1.1E+02	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	4.9E+01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	5.8E+01	2.0E+00	6.4E+00	1000	100	1.10E+03	110%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	5.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	3.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	7.3E+00	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	CFS-LRef-1316-T01-A	1	1.14E+03			1.14E+03	2.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1316-T02-A	1	1.23E+03			1.23E+03	8.2E-01	6.8E+00	2.2E+01	10	120	2.36E+03	94%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1316-T03-A	1	1.30E+03			1.30E+03	6.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1316-T04-A	1	1.33E+03			1.33E+03	8.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1316-T01-B	1	1.18E+03			1.18E+03	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1316-T02-B	1	1.14E+03			1.14E+03	2.0E+00	6.8E+00	2.2E+01	10	100	1.97E+03	83%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1316-T03-B	1	1.31E+03			1.31E+03	2.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1316-T04-B	1	1.34E+03			1.34E+03	1.0E+00	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1316-T01-C	1	1.17E+03			1.17E+03	3.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1316-T02-C	1	1.21E+03			1.21E+03	1.2E+00	6.8E+00	2.2E+01	10	100	2.19E+03	98%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1316-T03-C	1	1.31E+03			1.31E+03	2.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1316-T04-C	1	1.33E+03			1.33E+03	1.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1316-B01-A	1	3.40E+00	U1/2		3.40E+00	1.0E+02	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	CFS-LRef-1316-T01-A	1	1.07E+01			1.07E+01	2.0E+00	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1316-T02-A	1	8.37E+00			8.37E+00	3.2E+00	1.9E+00	6.0E+00	10	120	1.24E+03	102%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1316-T03-A	1	5.06E+00	E		5.06E+00	3.3E+00	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1316-T04-A	1	1.24E+01			1.24E+01	5.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1316-T01-B	1	9.99E+00			9.99E+00	8.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1316-T02-B	1	9.98E+00			9.98E+00	7.7E+00	1.9E+00	6.0E+00	10	100	8.93E+02	88%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1316-T03-B	1	4.80E+00	E		4.80E+00	1.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1316-T04-B	1	9.62E+00			9.62E+00	3.2E+00	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1316-T01-C	1	1.09E+01			1.09E+01	6.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1316-T02-C	1	8.91E+00			8.91E+00	3.3E+00	1.9E+00	6.0E+00	10	100	9.82E+02	97%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1316-T03-C	1	4.83E+00	E		4.83E+00	1.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1316-T04-C	1	1.47E+01			1.47E+01	9.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1316-B01-A	1	9.50E-01	U1/2		9.50E-01	2.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	CFS-LRef-1316-T01-A	1	1.77E+03			1.77E+03	1.2E+00	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1316-T02-A	1	3.46E+03			3.46E+03	1.2E+00	2.0E+00	6.4E+00	10	120	4.56E+03	92%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1316-T03-A	1	7.13E+03			7.13E+03	5.3E+01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1316-T04-A	1	1.14E+04			1.14E+04	3.6E-01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1316-T01-B	1	1.76E+03			1.76E+03	3.9E-01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1316-T02-B	1	3.33E+03			3.33E+03	2.4E+00	2.0E+00	6.4E+00	10	100	4.21E+03	88%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1316-T03-B	1	7.29E+03			7.29E+03	1.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1316-T04-B	1	1.15E+04			1.15E+04	4.8E-01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1316-T01-C	1	1.79E+03			1.79E+03	1.9E+00	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1316-T02-C	1	3.39E+03			3.39E+03	6.8E-01	2.0E+00	6.4E+00	10	100	4.35E+03	96%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1316-T03-C	1	7.25E+03			7.25E+03	1.8E+00	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1316-T04-C	1	1.16E+04			1.16E+04	4.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	3.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	CFS-LRef-1316-T01-A	1	6.52E+04			6.52E+04	6.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1316-T02-A	1	1.24E+05			1.24E+05	1.6E+00	1.0E+00	3.2E+00	1000	100	1.25E+05	91%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1316-T03-A	1	2.76E+05			2.76E+05	6.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1316-T04-A	1	4.95E+05			4.95E+05	3.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1316-T01-B	1	6.36E+04			6.36E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1316-T02-B	1	1.19E+05			1.19E+05	1.4E+00	1.0E+00	3.2E+00	1000	100	1.20E+05	87%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1316-T03-B	1	2.85E+05			2.85E+05	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1316-T04-B	1	5.11E+05			5.11E+05	1.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1316-T01-C	1	6.28E+04			6.28E+04	1.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1316-T02-C	1	1.22E+05			1.22E+05	1.3E+00	1.0E+00	3.2E+00	1000	100	1.23E+05	92%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1316-T03-C	1	2.94E+05			2.94E+05	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1316-T04-C	1	5.08E+05			5.08E+05	9.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	2.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	CFS-LRef-1316-T01-A	1	1.31E+01			1.31E+01	3.7E+00	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1316-T02-A	1	1.27E+01			1.27E+01	9.9E+00	1.2E+00	3.8E+00	10	120	1.33E+03	110%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1316-T03-A	1	1.18E+01			1.18E+01	7.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1316-T04-A	1	1.50E+01			1.50E+01	8.8E+00	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1316-T01-B	1	9.82E+00			9.82E+00	2.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1316-T02-B	1	1.24E+01			1.24E+01	1.8E+01	1.2E+00	3.8E+00	10	100	9.96E+02	98%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1316-T03-B	1	1.36E+01			1.36E+01	1.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1316-T04-B	1	1.62E+01			1.62E+01	4.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1316-T01-C	1	9.37E+00			9.37E+00	2.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1316-T02-C	1	1.11E+01			1.11E+01	1.1E+01	1.2E+00	3.8E+00	10	100	1.12E+03	111%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1316-T03-C	1	1.32E+01			1.32E+01	9.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1316-T04-C	1	1.45E+01			1.45E+01	1.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1316-B01-A	1	6.00E-01	U1/2		6.00E-01	9.3E+01	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	CFS-LRef-1316-T01-A	1	2.74E+02			2.74E+02	1.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1316-T02-A	1	4.49E+02			4.49E+02	7.0E-01	1.8E+00	5.7E+00	10	120	1.66E+03	101%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1316-T03-A	1	7.79E+02			7.79E+02	6.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1316-T04-A	1	1.05E+03			1.05E+03	1.3E-01	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1316-T01-B	1	2.73E+02			2.73E+02	8.3E-01	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1316-T02-B	1	4.43E+02			4.43E+02	1.9E+00	1.8E+00	5.7E+00	10	100	1.35E+03	90%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1316-T03-B	1	7.75E+02			7.75E+02	1.3E+00	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1316-T04-B	1	1.06E+03			1.06E+03	1.6E+00	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1316-T01-C	1	2.76E+02			2.76E+02	6.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1316-T02-C	1	4.55E+02			4.55E+02	6.0E-01	1.8E+00	5.7E+00	10	100	1.49E+03	104%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1316-T03-C	1	7.82E+02			7.82E+02	1.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1316-T04-C	1	1.07E+03			1.07E+03	7.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1316-B01-A	1	9.00E-01	U1/2		9.00E-01	1.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	CFS-LRef-1316-T01-A	1	8.59E+00	E		8.59E+00	1.4E+02	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1316-T02-A	1	2.90E+01			2.90E+01	1.3E+02	3.7E+00	1.2E+01	1000	100	1.14E+03	112%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1316-T03-A	1	1.66E+01			1.66E+01	7.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1316-T04-A	1	2.58E+01			2.58E+01	5.7E+01	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1316-T01-B	1	1.37E+01			1.37E+01	1.1E+02	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1316-T02-B	1	5.72E+01			5.72E+01	2.1E+01	3.7E+00	1.2E+01	1000	100	1.04E+03	98%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1316-T03-B	1	1.92E+01			1.92E+01	4.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1316-T04-B	1	3.11E+01			3.11E+01	3.5E+01	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1316-T01-C	1	7.47E+00	E		7.47E+00	1.6E+02	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1316-T02-C	1	2.69E+01			2.69E+01	1.1E+02	3.7E+00	1.2E+01	1000	100	1.14E+03	111%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1316-T03-C	1	1.51E+01			1.51E+01	3.3E+01	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1316-T04-C	1	1.79E+01			1.79E+01	6.8E+01	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1316-B01-A	1	6.70E+00	E		6.70E+00	1.7E+02	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	CFS-LRef-1316-T01-A	1	1.05E+04			1.05E+04	6.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1316-T02-A	1	1.90E+04			1.90E+04	6.7E-01	1.6E+00	5.1E+00	1000	100	2.00E+04	103%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1316-T03-A	1	3.52E+04			3.52E+04	6.7E+01	1.6E+00	5.1E+00				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1316-T04-A	1	5.55E+04			5.55E+04	4.7E-01	1.6E+00	5.1E+00				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1316-T01-B	1	1.03E+04			1.03E+04	8.9E-01	1.6E+00	5.1E+00				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1316-T02-B	1	1.81E+04			1.81E+04	2.2E+00	1.6E+00	5.1E+00	1000	100	1.91E+04	98%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1316-T03-B	1	3.69E+04			3.69E+04	1.7E+00	1.6E+00	5.1E+00				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1316-T04-B	1	5.57E+04			5.57E+04	1.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1316-T01-C	1	1.03E+04			1.03E+04	1.3E-01	1.6E+00	5.1E+00				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1316-T02-C	1	1.86E+04			1.86E+04	7.6E-01	1.6E+00	5.1E+00	1000	100	1.97E+04	106%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1316-T03-C	1	3.63E+04			3.63E+04	2.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1316-T04-C	1	5.58E+04			5.58E+04	1.2E+00	1.6E+00	5.1E+00				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1316-B01-A	1	4.63E+01			4.63E+01	2.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	CFS-LRef-1316-T01-A	1	8.07E+01			8.07E+01	1.1E+01	1.5E+01	4.8E+01				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1316-T02-A	1	1.40E+02			1.40E+02	4.7E+00	1.5E+01	4.8E+01	10	120	1.45E+03	109%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1316-T03-A	1	2.67E+02			2.67E+02	6.7E+01	1.5E+01	4.8E+01				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1316-T04-A	1	4.82E+02			4.82E+02	5.0E+00	1.5E+01	4.8E+01				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1316-T01-B	1	7.68E+01			7.68E+01	3.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1316-T02-B	1	1.48E+02			1.48E+02	8.2E+00	1.5E+01	4.8E+01	10	100	1.12E+03	97%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1316-T03-B	1	2.77E+02			2.77E+02	3.4E+00	1.5E+01	4.8E+01				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1316-T04-B	1	4.99E+02			4.99E+02	1.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1316-T01-C	1	9.55E+01			9.55E+01	9.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1316-T02-C	1	1.44E+02			1.44E+02	5.3E+00	1.5E+01	4.8E+01	10	100	1.22E+03	108%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1316-T03-C	1	2.94E+02			2.94E+02	1.6E+00	1.5E+01	4.8E+01				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1316-T04-C	1	4.86E+02			4.86E+02	1.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1316-B01-A	1	7.50E+00	U1/2		7.50E+00	2.0E+02	1.5E+01	4.8E+01				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	CFS-LRef-1316-T01-A	1	4.57E+03			4.57E+03	1.9E+00	1.1E+00	3.5E+00				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1316-T02-A	1	5.79E+03			5.79E+03	1.5E+00	1.1E+00	3.5E+00	1000	100	6.74E+03	95%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1316-T03-A	1	7.00E+03			7.00E+03	3.9E+01	1.1E+00	3.5E+00				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1316-T04-A	1	7.58E+03			7.58E+03	3.6E-02	1.1E+00	3.5E+00				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1316-T01-B	1	4.59E+03			4.59E+03	1.1E+00	1.1E+00	3.5E+00				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1316-T02-B	1	5.77E+03			5.77E+03	2.6E+00	1.1E+00	3.5E+00	1000	100	6.70E+03	93%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1316-T03-B	1	7.13E+03			7.13E+03	1.7E+00	1.1E+00	3.5E+00				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1316-T04-B	1	7.73E+03			7.73E+03	1.2E+00	1.1E+00	3.5E+00				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1316-T01-C	1	4.58E+03			4.58E+03	1.6E+00	1.1E+00	3.5E+00				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1316-T02-C	1	5.92E+03			5.92E+03	1.1E+00	1.1E+00	3.5E+00	1000	100	6.85E+03	94%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1316-T03-C	1	7.31E+03			7.31E+03	2.0E+00	1.1E+00	3.5E+00				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1316-T04-C	1	7.66E+03			7.66E+03	7.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1316-B01-A	1	1.00E+01			1.00E+01	4.2E+01	1.1E+00	3.5E+00				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	CFS-LRef-1316-T01-A	1	2.17E+04			2.17E+04	7.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1316-T02-A	1	4.08E+04			4.08E+04	7.6E-01	2.5E+00	8.0E+00	1000	100	4.16E+04	86%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1316-T03-A	1	8.49E+04			8.49E+04	6.6E+01	2.5E+00	8.0E+00				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1316-T04-A	1	1.27E+05			1.27E+05	3.4E-01	2.5E+00	8.0E+00				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1316-T01-B	1	2.10E+04			2.10E+04	1.7E+00	2.5E+00	8.0E+00				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1316-T02-B	1	3.90E+04			3.90E+04	1.3E+00	2.5E+00	8.0E+00	1000	100	3.99E+04	85%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1316-T03-B	1	8.55E+04			8.55E+04	1.8E+00	2.5E+00	8.0E+00				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1316-T04-B	1	1.30E+05			1.30E+05	1.1E+00	2.5E+00	8.0E+00				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1316-T01-C	1	2.16E+04			2.16E+04	3.0E-01	2.5E+00	8.0E+00				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1316-T02-C	1	4.06E+04			4.06E+04	1.3E+00	2.5E+00	8.0E+00	1000	100	4.15E+04	89%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1316-T03-C	1	8.47E+04			8.47E+04	1.2E+00	2.5E+00	8.0E+00				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1316-T04-C	1	1.30E+05			1.30E+05	5.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1316-B01-A	1	1.25E+00	U1/2		1.25E+00	9.7E+00	2.5E+00	8.0E+00				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	CFS-LRef-1316-T01-A	1	1.48E+03			1.48E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1316-T02-A	1	2.04E+03			2.04E+03	9.6E-01	1.0E+00	3.2E+00	1000	100	3.10E+03	106%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1316-T03-A	1	2.94E+03			2.94E+03	4.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1316-T04-A	1	3.67E+03			3.67E+03	3.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1316-T01-B	1	1.41E+03			1.41E+03	9.2E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1316-T02-B	1	2.01E+03			2.01E+03	2.2E+00	1.0E+00	3.2E+00	1000	100	2.97E+03	95%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1316-T03-B	1	3.06E+03			3.06E+03	2.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1316-T04-B	1	3.70E+03			3.70E+03	5.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1316-T01-C	1	1.43E+03			1.43E+03	6.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1316-T02-C	1	2.01E+03			2.01E+03	8.4E-01	1.0E+00	3.2E+00	1000	100	2.99E+03	98%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1316-T03-C	1	3.03E+03			3.03E+03	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1316-T04-C	1	3.70E+03			3.70E+03	5.4E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	6.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	CFS-LRef-1316-T01-A	1	5.80E+05			5.80E+05	5.1E-01	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1316-T02-A	1	6.45E+05			6.45E+05	6.4E-01	6.8E+00	2.2E+01	1000	100	6.46E+05	88%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1316-T03-A	1	7.84E+05			7.84E+05	7.1E+01	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1316-T04-A	1	1.03E+06			1.03E+06	2.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1316-T01-B	1	5.69E+05			5.69E+05	8.9E-01	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1316-T02-B	1	6.30E+05			6.30E+05	2.0E+00	6.8E+00	2.2E+01	1000	100	6.31E+05	86%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1316-T03-B	1	8.14E+05			8.14E+05	1.5E+00	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1316-T04-B	1	1.05E+06			1.05E+06	1.4E+00	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1316-T01-C	1	5.70E+05			5.70E+05	3.4E-01	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1316-T02-C	1	6.37E+05			6.37E+05	5.5E-01	6.8E+00	2.2E+01	1000	100	6.38E+05	89%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1316-T03-C	1	8.33E+05			8.33E+05	2.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1316-T04-C	1	1.05E+06			1.05E+06	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1316-B01-A	1	8.35E+00	E		8.35E+00	1.2E+01	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	CFS-LRef-1316-T01-A	1	3.83E+02			3.83E+02	9.7E-01	4.6E+00	1.5E+01				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1316-T02-A	1	5.73E+02			5.73E+02	1.1E+00	4.6E+00	1.5E+01	10	120	1.71E+03	94%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1316-T03-A	1	8.35E+02			8.35E+02	6.8E+01	4.6E+00	1.5E+01				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1316-T04-A	1	1.17E+03			1.17E+03	5.7E-01	4.6E+00	1.5E+01				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1316-T01-B	1	3.86E+02			3.86E+02	1.7E+00	4.6E+00	1.5E+01				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1316-T02-B	1	5.47E+02			5.47E+02	2.2E+00	4.6E+00	1.5E+01	10	100	1.42E+03	87%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1316-T03-B	1	8.78E+02			8.78E+02	1.2E+00	4.6E+00	1.5E+01				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1316-T04-B	1	1.19E+03			1.19E+03	1.7E+00	4.6E+00	1.5E+01				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1316-T01-C	1	3.83E+02			3.83E+02	1.7E+00	4.6E+00	1.5E+01				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1316-T02-C	1	5.64E+02			5.64E+02	1.5E+00	4.6E+00	1.5E+01	10	100	1.53E+03	97%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1316-T03-C	1	8.89E+02			8.89E+02	2.1E+00	4.6E+00	1.5E+01				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1316-T04-C	1	1.17E+03			1.17E+03	1.2E+00	4.6E+00	1.5E+01				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1316-B01-A	1	2.30E+00	U1/2		2.30E+00	1.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	CFS-LRef-1316-T01-A	1	1.00E+00	U1/2		1.00E+00	8.0E+02	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1316-T02-A	1	1.00E+00	U1/2		1.00E+00	2.1E+02	2.0E+00	6.4E+00	10	120	1.29E+03	107%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1316-T03-A	1	1.00E+00	U1/2		1.00E+00	4.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1316-T04-A	1	1.00E+00	U1/2		1.00E+00	2.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1316-T01-B	1	1.00E+00	U1/2		1.00E+00	5.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1316-T02-B	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00	10	100	9.67E+02	97%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1316-T03-B	1	1.00E+00	U1/2		1.00E+00	2.8E+02	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1316-T04-B	1	1.00E+00	U1/2		1.00E+00	5.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1316-T01-C	1	1.00E+00	U1/2		1.00E+00	1.6E+02	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1316-T02-C	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00	10	100	1.08E+03	108%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1316-T03-C	1	1.00E+00	U1/2		1.00E+00	1.7E+03	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1316-T04-C	1	1.00E+00	U1/2		1.00E+00	1.5E+02	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1316-B01-A	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	CFS-LRef-1316-T01-A	1	3.46E+01			3.46E+01	2.2E+00	1.5E+00	4.8E+00				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1316-T02-A	1	3.32E+01			3.32E+01	4.7E+00	1.5E+00	4.8E+00	10	120	1.36E+03	110%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1316-T03-A	1	2.81E+01			2.81E+01	6.9E+01	1.5E+00	4.8E+00				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1316-T04-A	1	2.82E+01			2.82E+01	5.0E+00	1.5E+00	4.8E+00				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1316-T01-B	1	3.48E+01			3.48E+01	2.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1316-T02-B	1	3.24E+01			3.24E+01	4.7E+00	1.5E+00	4.8E+00	10	100	1.02E+03	98%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1316-T03-B	1	3.07E+01			3.07E+01	7.2E-01	1.5E+00	4.8E+00				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1316-T04-B	1	2.96E+01			2.96E+01	2.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1316-T01-C	1	3.44E+01			3.44E+01	2.1E+00	1.5E+00	4.8E+00				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1316-T02-C	1	3.32E+01			3.32E+01	1.4E+00	1.5E+00	4.8E+00	10	100	1.14E+03	111%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1316-T03-C	1	3.14E+01			3.14E+01	5.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1316-T04-C	1	3.00E+01			3.00E+01	3.3E+00	1.5E+00	4.8E+00				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1316-B01-A	1	7.50E-01	U1/2		7.50E-01	5.2E+01	1.5E+00	4.8E+00				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	CFS-LRef-1316-T01-A	1	2.58E+04			2.58E+04	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:11 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1316-T02-A	1	3.69E+04			3.69E+04	1.2E+00	1.0E+00	3.2E+00	10	120	3.80E+04	88%	VU ICP-OES	1/26/11 4:12 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1316-T03-A	1	5.46E+04			5.46E+04	5.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:14 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1316-T04-A	1	6.87E+04			6.87E+04	2.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:16 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1316-T01-B	1	2.60E+04			2.60E+04	8.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:17 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1316-T02-B	1	3.73E+04			3.73E+04	1.7E+00	1.0E+00	3.2E+00	10	100	3.82E+04	84%	VU ICP-OES	1/26/11 4:19 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1316-T03-B	1	5.51E+04			5.51E+04	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:20 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1316-T04-B	1	7.10E+04			7.10E+04	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:22 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1316-T01-C	1	2.65E+04			2.65E+04	4.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:24 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1316-T02-C	1	3.82E+04			3.82E+04	1.1E+00	1.0E+00	3.2E+00	10	100	3.91E+04	93%	VU ICP-OES	1/26/11 4:25 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1316-T03-C	1	5.61E+04			5.61E+04	1.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:27 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1316-T04-C	1	6.89E+04			6.89E+04	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:29 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1316-B01-A	1	5.00E-01	U1/2		5.00E-01	1.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:09 PM	EPA Interlab LRef 1313-1316 CFS

QA-QC Spreadsheet 1316:

Al	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Al	CFS-LRef-1316-T01-D	1	4.29E+01			4.29E+01	2.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1316-T02-D	1	4.58E+01			4.58E+01	1.8E+01	1.0E+00	3.2E+00	1000	100	1.16E+03	111%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1316-T03-D	1	5.29E+01			5.29E+01	9.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1316-T04-D	1	4.82E+01			4.82E+01	2.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1316-T01-E	1	4.20E+01			4.20E+01	9.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1316-T02-E	1	5.45E+01			5.45E+01	3.5E+00	1.0E+00	3.2E+00	1000	100	1.18E+03	113%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1316-T03-E	1	5.13E+01			5.13E+01	6.3E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1316-T04-E	1	4.96E+01			4.96E+01	3.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1316-T01-F	1	3.95E+01			3.95E+01	1.8E+01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1316-T02-F	1	5.38E+01			5.38E+01	2.9E+00	1.0E+00	3.2E+00	1000	100	1.14E+03	108%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1316-T03-F	1	4.86E+01			4.86E+01	1.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Al	CFS-LRef-1316-T04-F	1	4.93E+01			4.93E+01	2.5E+02	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

Sb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sb	CFS-LRef-1316-T01-D	1	3.05E+01			3.05E+01	1.1E+03	7.5E+00	2.4E+01				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1316-T02-D	1	3.38E+01			3.38E+01	4.8E+00	7.5E+00	2.4E+01	10	100	1.15E+03	111%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1316-T03-D	1	4.49E+01			4.49E+01	8.5E-01	7.5E+00	2.4E+01				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1316-T04-D	1	4.92E+01			4.92E+01	1.6E+01	7.5E+00	2.4E+01				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1316-T01-E	1	2.92E+01			2.92E+01	2.3E+01	7.5E+00	2.4E+01				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1316-T02-E	1	3.54E+01			3.54E+01	4.4E+01	7.5E+00	2.4E+01	10	100	1.17E+03	113%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1316-T03-E	1	4.21E+01			4.21E+01	1.6E+01	7.5E+00	2.4E+01				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1316-T04-E	1	4.70E+01			4.70E+01	8.9E+00	7.5E+00	2.4E+01				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1316-T01-F	1	2.83E+01			2.83E+01	5.0E+01	7.5E+00	2.4E+01				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1316-T02-F	1	3.59E+01			3.59E+01	5.8E+01	7.5E+00	2.4E+01	10	100	1.03E+03	100%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1316-T03-F	1	4.91E+01			4.91E+01	1.5E+01	7.5E+00	2.4E+01				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Sb	CFS-LRef-1316-T04-F	1	5.09E+01			5.09E+01	2.5E+02	7.5E+00	2.4E+01				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

As	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
As	CFS-LRef-1316-T01-D	1	1.19E+01	E		1.19E+01	2.8E+00	1.1E+01	3.5E+01				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1316-T02-D	1	2.25E+01	E		2.25E+01	1.3E+01	1.1E+01	3.5E+01	10	100	1.13E+03	111%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1316-T03-D	1	2.40E+01	E		2.40E+01	1.8E+01	1.1E+01	3.5E+01				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1316-T04-D	1	2.68E+01	E		2.68E+01	1.7E+01	1.1E+01	3.5E+01				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1316-T01-E	1	1.24E+01	E		1.24E+01	6.9E+01	1.1E+01	3.5E+01				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1316-T02-E	1	2.09E+01	E		2.09E+01	2.9E+01	1.1E+01	3.5E+01	10	100	1.15E+03	113%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1316-T03-E	1	2.99E+01	E		2.99E+01	3.5E+01	1.1E+01	3.5E+01				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1316-T04-E	1	3.51E+01			3.51E+01	6.5E+00	1.1E+01	3.5E+01				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1316-T01-F	1	1.28E+01	E		1.28E+01	5.0E+01	1.1E+01	3.5E+01				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1316-T02-F	1	1.36E+01	E		1.36E+01	4.6E+01	1.1E+01	3.5E+01	10	100	1.01E+03	99%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1316-T03-F	1	2.83E+01	E		2.83E+01	1.5E+02	1.1E+01	3.5E+01				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
As	CFS-LRef-1316-T04-F	1	3.06E+01	E		3.06E+01	3.3E+02	1.1E+01	3.5E+01				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

B	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
B	CFS-LRef-1316-T01-D	1	1.72E+02			1.72E+02	5.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1316-T02-D	1	2.89E+02			2.89E+02	1.3E+00	1.0E+00	3.2E+00	1000	100	1.32E+03	103%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1316-T03-D	1	6.29E+02			6.29E+02	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1316-T04-D	1	9.92E+02			9.92E+02	2.5E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1316-T01-E	1	1.44E+02			1.44E+02	2.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1316-T02-E	1	2.95E+02			2.95E+02	1.5E+00	1.0E+00	3.2E+00	1000	100	1.37E+03	108%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1316-T03-E	1	6.26E+02			6.26E+02	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1316-T04-E	1	9.98E+02			9.98E+02	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1316-T01-F	1	1.36E+02			1.36E+02	1.9E+01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1316-T02-F	1	2.73E+02			2.73E+02	6.0E-01	1.0E+00	3.2E+00	1000	100	1.24E+03	97%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1316-T03-F	1	6.23E+02			6.23E+02	2.0E+01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
B	CFS-LRef-1316-T04-F	1	9.97E+02			9.97E+02	1.7E+02	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

Ba	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ba	CFS-LRef-1316-T01-D	1	9.20E+01			9.20E+01	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1316-T02-D	1	8.85E+01			8.85E+01	6.7E-01	1.0E+00	3.2E+00	10	100	1.22E+03	113%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1316-T03-D	1	7.35E+01			7.35E+01	1.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1316-T04-D	1	6.04E+01			6.04E+01	3.8E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1316-T01-E	1	8.80E+01			8.80E+01	3.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1316-T02-E	1	8.77E+01			8.77E+01	1.2E+00	1.0E+00	3.2E+00	10	100	1.24E+03	115%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1316-T03-E	1	7.51E+01			7.51E+01	2.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1316-T04-E	1	6.24E+01			6.24E+01	8.7E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1316-T01-F	1	8.46E+01			8.46E+01	1.2E+01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1316-T02-F	1	8.46E+01			8.46E+01	2.4E-01	1.0E+00	3.2E+00	10	100	1.10E+03	102%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1316-T03-F	1	7.02E+01			7.02E+01	2.3E+02	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Ba	CFS-LRef-1316-T04-F	1	6.49E+01			6.49E+01	1.6E+02	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

Be	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Be	CFS-LRef-1316-T01-D	1	9.50E-01	U1/2		9.50E-01	1.1E+02	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1316-T02-D	1	9.50E-01	U1/2		9.50E-01	1.3E+02	1.9E+00	6.0E+00	10	100	1.16E+03	116%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1316-T03-D	1	9.50E-01	U1/2		9.50E-01	1.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1316-T04-D	1	9.50E-01	U1/2		9.50E-01	8.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1316-T01-E	1	9.50E-01	U1/2		9.50E-01	5.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1316-T02-E	1	9.50E-01	U1/2		9.50E-01	8.0E+01	1.9E+00	6.0E+00	10	100	1.17E+03	117%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1316-T03-E	1	9.50E-01	U1/2		9.50E-01	1.4E+01	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1316-T04-E	1	9.50E-01	U1/2		9.50E-01	7.2E+01	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1316-T01-F	1	9.50E-01	U1/2		9.50E-01	5.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1316-T02-F	1	9.50E-01	U1/2		9.50E-01	5.5E+01	1.9E+00	6.0E+00	10	100	1.01E+03	101%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1316-T03-F	1	9.50E-01	U1/2		9.50E-01	3.7E+01	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Be	CFS-LRef-1316-T04-F	1	9.50E-01	U1/2		9.50E-01	3.6E+02	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

Cd	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cd	CFS-LRef-1316-T01-D	1	4.63E+03			4.63E+03	1.1E+01	2.2E+00	7.0E+00				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1316-T02-D	1	7.02E+03			7.02E+03	4.3E-01	2.2E+00	7.0E+00	10	100	7.99E+03	97%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1316-T03-D	1	1.06E+04			1.06E+04	1.1E+00	2.2E+00	7.0E+00				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1316-T04-D	1	1.31E+04			1.31E+04	5.4E-01	2.2E+00	7.0E+00				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1316-T01-E	1	4.78E+03			4.78E+03	4.1E-01	2.2E+00	7.0E+00				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1316-T02-E	1	7.20E+03			7.20E+03	5.5E-01	2.2E+00	7.0E+00	10	100	8.15E+03	96%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1316-T03-E	1	1.09E+04			1.09E+04	3.0E+00	2.2E+00	7.0E+00				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1316-T04-E	1	1.30E+04			1.30E+04	6.6E-01	2.2E+00	7.0E+00				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1316-T01-F	1	4.62E+03			4.62E+03	1.3E+01	2.2E+00	7.0E+00				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1316-T02-F	1	6.77E+03			6.77E+03	3.3E-01	2.2E+00	7.0E+00	10	100	7.67E+03	90%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1316-T03-F	1	1.03E+04			1.03E+04	7.7E+01	2.2E+00	7.0E+00				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Cd	CFS-LRef-1316-T04-F	1	1.33E+04			1.33E+04	1.6E+02	2.2E+00	7.0E+00				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

Ca	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ca	CFS-LRef-1316-T01-D	1	6.41E+05			6.41E+05	2.3E+01	2.6E+00	8.3E+00				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1316-T02-D	1	6.54E+05			6.54E+05	6.8E-01	2.6E+00	8.3E+00	1000	100	6.55E+05	89%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1316-T03-D	1	6.29E+05			6.29E+05	1.4E+00	2.6E+00	8.3E+00				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1316-T04-D	1	5.72E+05			5.72E+05	1.1E+00	2.6E+00	8.3E+00				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1316-T01-E	1	6.57E+05			6.57E+05	7.1E-01	2.6E+00	8.3E+00				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1316-T02-E	1	6.69E+05			6.69E+05	1.4E+00	2.6E+00	8.3E+00	1000	100	6.70E+05	88%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1316-T03-E	1	6.38E+05			6.38E+05	2.5E+00	2.6E+00	8.3E+00				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1316-T04-E	1	5.85E+05			5.85E+05	7.2E-01	2.6E+00	8.3E+00				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1316-T01-F	1	6.38E+05			6.38E+05	1.2E+01	2.6E+00	8.3E+00				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1316-T02-F	1	6.33E+05			6.33E+05	3.3E-01	2.6E+00	8.3E+00	1000	100	6.34E+05	86%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1316-T03-F	1	6.25E+05			6.25E+05	8.4E+01	2.6E+00	8.3E+00				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Ca	CFS-LRef-1316-T04-F	1	5.81E+05			5.81E+05	1.6E+02	2.6E+00	8.3E+00				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

Cr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cr	CFS-LRef-1316-T01-D	1	6.00E-01	U1/2		6.00E-01	2.7E+01	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1316-T02-D	1	6.00E-01	U1/2		6.00E-01	8.9E+01	1.2E+00	3.8E+00	10	100	1.11E+03	111%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1316-T03-D	1	6.00E-01	U1/2		6.00E-01	1.9E+02	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1316-T04-D	1	6.00E-01	U1/2		6.00E-01	5.9E+01	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1316-T01-E	1	6.00E-01	U1/2		6.00E-01	8.2E+02	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1316-T02-E	1	6.00E-01	U1/2		6.00E-01	1.0E+02	1.2E+00	3.8E+00	10	100	1.11E+03	111%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1316-T03-E	1	6.00E-01	U1/2		6.00E-01	2.7E+02	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1316-T04-E	1	6.00E-01	U1/2		6.00E-01	1.6E+02	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1316-T01-F	1	6.00E-01	U1/2		6.00E-01	1.5E+03	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1316-T02-F	1	6.00E-01	U1/2		6.00E-01	1.7E+02	1.2E+00	3.8E+00	10	100	9.78E+02	98%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1316-T03-F	1	6.00E-01	U1/2		6.00E-01	1.2E+01	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Cr	CFS-LRef-1316-T04-F	1	6.00E-01	U1/2		6.00E-01	1.8E+01	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

Co	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Co	CFS-LRef-1316-T01-D	1	1.13E+02			1.13E+02	1.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1316-T02-D	1	1.96E+02			1.96E+02	1.0E+00	1.8E+00	5.7E+00	10	100	1.25E+03	105%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1316-T03-D	1	3.90E+02			3.90E+02	1.2E+00	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1316-T04-D	1	5.65E+02			5.65E+02	6.3E-01	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1316-T01-E	1	1.09E+02			1.09E+02	2.6E-01	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1316-T02-E	1	2.07E+02			2.07E+02	8.3E-01	1.8E+00	5.7E+00	10	100	1.27E+03	107%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1316-T03-E	1	3.95E+02			3.95E+02	2.8E+00	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1316-T04-E	1	5.63E+02			5.63E+02	6.1E-01	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1316-T01-F	1	1.04E+02			1.04E+02	1.5E+01	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1316-T02-F	1	1.95E+02			1.95E+02	9.2E-01	1.8E+00	5.7E+00	10	100	1.14E+03	95%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1316-T03-F	1	3.93E+02			3.93E+02	9.8E+01	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Co	CFS-LRef-1316-T04-F	1	5.78E+02			5.78E+02	1.6E+02	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

Cu	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Cu	CFS-LRef-1316-T01-D	1	9.87E+02			9.87E+02	1.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1316-T02-D	1	1.35E+03			1.35E+03	1.3E+00	3.7E+00	1.2E+01	10	100	2.28E+03	93%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1316-T03-D	1	2.43E+03			2.43E+03	9.0E-01	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1316-T04-D	1	3.55E+03			3.55E+03	4.8E-01	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1316-T01-E	1	9.68E+02			9.68E+02	4.7E-01	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1316-T02-E	1	1.49E+03			1.49E+03	1.9E+00	3.7E+00	1.2E+01	10	100	2.49E+03	99%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1316-T03-E	1	2.62E+03			2.62E+03	2.5E+00	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1316-T04-E	1	3.59E+03			3.59E+03	1.4E+00	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1316-T01-F	1	9.78E+02			9.78E+02	7.0E+00	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1316-T02-F	1	1.37E+03			1.37E+03	6.5E-01	3.7E+00	1.2E+01	10	100	2.25E+03	89%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1316-T03-F	1	2.71E+03			2.71E+03	1.0E+02	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Cu	CFS-LRef-1316-T04-F	1	3.65E+03			3.65E+03	1.5E+02	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

Fe	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Fe	CFS-LRef-1316-T01-D	1	1.00E+00	U1/2		1.00E+00	1.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1316-T02-D	1	1.00E+00	U1/2		1.00E+00	8.2E+00	2.0E+00	6.4E+00	1000	100	1.10E+03	110%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1316-T03-D	1	1.00E+00	U1/2		1.00E+00	6.2E+01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1316-T04-D	1	1.00E+00	U1/2		1.00E+00	4.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1316-T01-E	1	1.00E+00	U1/2		1.00E+00	3.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1316-T02-E	1	1.00E+00	U1/2		1.00E+00	7.3E+00	2.0E+00	6.4E+00	1000	100	1.10E+03	110%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1316-T03-E	1	1.00E+00	U1/2		1.00E+00	7.8E+01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1316-T04-E	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1316-T01-F	1	1.00E+00	U1/2		1.00E+00	1.7E+01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1316-T02-F	1	1.00E+00	U1/2		1.00E+00	1.9E+01	2.0E+00	6.4E+00	1000	100	9.76E+02	97%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1316-T03-F	1	1.00E+00	U1/2		1.00E+00	5.7E+00	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Fe	CFS-LRef-1316-T04-F	1	1.00E+00	U1/2		1.00E+00	2.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

Pb	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Pb	CFS-LRef-1316-T01-D	1	1.17E+03			1.17E+03	8.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1316-T02-D	1	1.18E+03			1.18E+03	5.4E-01	6.8E+00	2.2E+01	10	100	2.07E+03	89%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1316-T03-D	1	1.28E+03			1.28E+03	1.1E+00	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1316-T04-D	1	1.31E+03			1.31E+03	7.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1316-T01-E	1	1.07E+03			1.07E+03	5.3E-01	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1316-T02-E	1	1.23E+03			1.23E+03	2.9E-01	6.8E+00	2.2E+01	10	100	2.15E+03	93%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1316-T03-E	1	1.30E+03			1.30E+03	2.9E+00	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1316-T04-E	1	1.30E+03			1.30E+03	7.2E-01	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1316-T01-F	1	1.02E+03			1.02E+03	1.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1316-T02-F	1	1.09E+03			1.09E+03	3.9E-01	6.8E+00	2.2E+01	10	100	1.94E+03	85%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1316-T03-F	1	1.31E+03			1.31E+03	1.3E+02	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Pb	CFS-LRef-1316-T04-F	1	1.30E+03			1.30E+03	1.5E+02	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

Li	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Li	CFS-LRef-1316-T01-D	1	1.08E+01			1.08E+01	8.9E-01	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1316-T02-D	1	8.98E+00			8.98E+00	3.6E+00	1.9E+00	6.0E+00	10	100	1.02E+03	101%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1316-T03-D	1	5.79E+00	E		5.79E+00	8.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1316-T04-D	1	9.60E+00			9.60E+00	2.6E+00	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1316-T01-E	1	1.17E+01			1.17E+01	3.8E+00	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1316-T02-E	1	8.13E+00			8.13E+00	1.1E+01	1.9E+00	6.0E+00	10	100	1.03E+03	102%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1316-T03-E	1	5.64E+00	E		5.64E+00	4.4E+00	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1316-T04-E	1	1.12E+01			1.12E+01	7.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1316-T01-F	1	8.88E+00			8.88E+00	1.1E+01	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1316-T02-F	1	9.10E+00			9.10E+00	4.1E+00	1.9E+00	6.0E+00	10	100	8.91E+02	88%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1316-T03-F	1	5.98E+00	E		5.98E+00	7.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Li	CFS-LRef-1316-T04-F	1	9.23E+00			9.23E+00	2.7E+00	1.9E+00	6.0E+00				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

Mn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mn	CFS-LRef-1316-T01-D	1	1.67E+03			1.67E+03	8.4E+01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1316-T02-D	1	3.26E+03			3.26E+03	2.5E-01	2.0E+00	6.4E+00	10	100	4.19E+03	92%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1316-T03-D	1	7.32E+03			7.32E+03	1.5E+00	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1316-T04-D	1	1.15E+04			1.15E+04	6.1E-01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1316-T01-E	1	1.66E+03			1.66E+03	7.0E-01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1316-T02-E	1	3.43E+03			3.43E+03	7.9E-01	2.0E+00	6.4E+00	10	100	4.37E+03	95%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1316-T03-E	1	7.39E+03			7.39E+03	2.4E+00	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1316-T04-E	1	1.15E+04			1.15E+04	1.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1316-T01-F	1	1.68E+03			1.68E+03	7.0E+00	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1316-T02-F	1	3.21E+03			3.21E+03	2.4E-01	2.0E+00	6.4E+00	10	100	4.11E+03	89%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1316-T03-F	1	7.32E+03			7.32E+03	9.1E+00	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Mn	CFS-LRef-1316-T04-F	1	1.14E+04			1.14E+04	1.5E+02	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

Mg	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mg	CFS-LRef-1316-T01-D	1	6.24E+04			6.24E+04	4.4E+01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1316-T02-D	1	1.26E+05			1.26E+05	5.5E-01	1.0E+00	3.2E+00	1000	100	1.26E+05	96%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1316-T03-D	1	3.00E+05			3.00E+05	1.8E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1316-T04-D	1	5.05E+05			5.05E+05	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1316-T01-E	1	6.23E+04			6.23E+04	4.0E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1316-T02-E	1	1.32E+05			1.32E+05	4.4E-01	1.0E+00	3.2E+00	1000	100	1.33E+05	92%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1316-T03-E	1	3.00E+05			3.00E+05	2.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1316-T04-E	1	5.20E+05			5.20E+05	1.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1316-T01-F	1	5.66E+04			5.66E+04	2.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1316-T02-F	1	1.23E+05			1.23E+05	1.8E-01	1.0E+00	3.2E+00	1000	100	1.24E+05	86%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1316-T03-F	1	2.99E+05			2.99E+05	1.2E+02	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Mg	CFS-LRef-1316-T04-F	1	5.14E+05			5.14E+05	1.6E+02	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

Mo	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Mo	CFS-LRef-1316-T01-D	1	7.75E+00			7.75E+00	1.5E+01	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1316-T02-D	1	1.43E+01			1.43E+01	1.5E+01	1.2E+00	3.8E+00	10	100	1.12E+03	110%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1316-T03-D	1	1.55E+01			1.55E+01	1.8E+01	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1316-T04-D	1	1.69E+01			1.69E+01	9.0E+00	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1316-T01-E	1	8.40E+00			8.40E+00	1.1E+01	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1316-T02-E	1	1.11E+01			1.11E+01	1.7E+01	1.2E+00	3.8E+00	10	100	1.15E+03	114%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1316-T03-E	1	1.28E+01			1.28E+01	6.4E+00	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1316-T04-E	1	1.76E+01			1.76E+01	1.6E+01	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1316-T01-F	1	7.52E+00			7.52E+00	1.0E+01	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1316-T02-F	1	1.08E+01			1.08E+01	2.6E+01	1.2E+00	3.8E+00	10	100	9.98E+02	99%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1316-T03-F	1	1.17E+01			1.17E+01	2.4E+01	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Mo	CFS-LRef-1316-T04-F	1	1.74E+01			1.74E+01	2.5E+02	1.2E+00	3.8E+00				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

Ni	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ni	CFS-LRef-1316-T01-D	1	2.60E+02			2.60E+02	4.7E+00	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1316-T02-D	1	4.18E+02			4.18E+02	3.0E-01	1.8E+00	5.7E+00	10	100	1.43E+03	101%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1316-T03-D	1	7.50E+02			7.50E+02	1.1E+00	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1316-T04-D	1	1.02E+03			1.02E+03	6.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1316-T01-E	1	2.62E+02			2.62E+02	2.0E-01	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1316-T02-E	1	4.42E+02			4.42E+02	3.5E-01	1.8E+00	5.7E+00	10	100	1.46E+03	101%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1316-T03-E	1	7.58E+02			7.58E+02	2.9E+00	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1316-T04-E	1	1.01E+03			1.01E+03	9.4E-01	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1316-T01-F	1	2.63E+02			2.63E+02	1.6E+01	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1316-T02-F	1	4.02E+02			4.02E+02	4.3E-01	1.8E+00	5.7E+00	10	100	1.32E+03	92%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1316-T03-F	1	7.52E+02			7.52E+02	7.4E+01	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Ni	CFS-LRef-1316-T04-F	1	1.03E+03			1.03E+03	1.5E+02	1.8E+00	5.7E+00				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

P	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
P	CFS-LRef-1316-T01-D	1	1.33E+01			1.33E+01	1.5E+02	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1316-T02-D	1	2.21E+01			2.21E+01	6.3E+01	3.7E+00	1.2E+01	1000	100	1.14E+03	111%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1316-T03-D	1	1.88E+01			1.88E+01	7.2E+00	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1316-T04-D	1	2.68E+01			2.68E+01	3.4E+01	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1316-T01-E	1	1.21E+01			1.21E+01	8.6E+01	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1316-T02-E	1	1.87E+01			1.87E+01	7.6E+01	3.7E+00	1.2E+01	1000	100	1.18E+03	116%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1316-T03-E	1	1.81E+01			1.81E+01	5.1E+01	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1316-T04-E	1	2.71E+01			2.71E+01	1.9E+01	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1316-T01-F	1	9.08E+00	E		9.08E+00	2.7E+02	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1316-T02-F	1	1.45E+01			1.45E+01	8.1E+01	3.7E+00	1.2E+01	1000	100	1.05E+03	104%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1316-T03-F	1	1.78E+01			1.78E+01	3.0E+02	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
P	CFS-LRef-1316-T04-F	1	2.90E+01			2.90E+01	7.2E+01	3.7E+00	1.2E+01				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

K	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
K	CFS-LRef-1316-T01-D	1	9.65E+03			9.65E+03	9.8E+00	1.6E+00	5.1E+00				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1316-T02-D	1	1.81E+04			1.81E+04	6.9E-01	1.6E+00	5.1E+00	1000	100	1.91E+04	101%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1316-T03-D	1	3.62E+04			3.62E+04	1.1E+00	1.6E+00	5.1E+00				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1316-T04-D	1	5.50E+04			5.50E+04	3.6E-01	1.6E+00	5.1E+00				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1316-T01-E	1	9.78E+03			9.78E+03	2.8E-01	1.6E+00	5.1E+00				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1316-T02-E	1	1.88E+04			1.88E+04	9.7E-01	1.6E+00	5.1E+00	1000	100	1.98E+04	103%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1316-T03-E	1	3.70E+04			3.70E+04	3.3E+00	1.6E+00	5.1E+00				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1316-T04-E	1	5.61E+04			5.61E+04	6.1E-01	1.6E+00	5.1E+00				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1316-T01-F	1	9.31E+03			9.31E+03	1.5E+01	1.6E+00	5.1E+00				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1316-T02-F	1	1.79E+04			1.79E+04	4.4E-01	1.6E+00	5.1E+00	1000	100	1.88E+04	92%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1316-T03-F	1	3.71E+04			3.71E+04	6.2E+01	1.6E+00	5.1E+00				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
K	CFS-LRef-1316-T04-F	1	5.72E+04			5.72E+04	1.6E+02	1.6E+00	5.1E+00				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

Se	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Se	CFS-LRef-1316-T01-D	1	8.42E+01			8.42E+01	6.2E+01	1.5E+01	4.8E+01				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1316-T02-D	1	1.27E+02			1.27E+02	5.4E+00	1.5E+01	4.8E+01	10	100	1.22E+03	109%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1316-T03-D	1	2.90E+02			2.90E+02	1.9E+00	1.5E+01	4.8E+01				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1316-T04-D	1	4.95E+02			4.95E+02	5.3E+00	1.5E+01	4.8E+01				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1316-T01-E	1	7.64E+01			7.64E+01	2.0E+01	1.5E+01	4.8E+01				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1316-T02-E	1	1.61E+02			1.61E+02	3.1E+00	1.5E+01	4.8E+01	10	100	1.25E+03	109%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1316-T03-E	1	2.80E+02			2.80E+02	8.7E+00	1.5E+01	4.8E+01				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1316-T04-E	1	5.00E+02			5.00E+02	4.6E+00	1.5E+01	4.8E+01				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1316-T01-F	1	8.52E+01			8.52E+01	3.8E+01	1.5E+01	4.8E+01				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1316-T02-F	1	1.29E+02			1.29E+02	1.8E+00	1.5E+01	4.8E+01	10	100	1.13E+03	100%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1316-T03-F	1	2.86E+02			2.86E+02	3.9E+01	1.5E+01	4.8E+01				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Se	CFS-LRef-1316-T04-F	1	4.92E+02			4.92E+02	1.6E+02	1.5E+01	4.8E+01				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

Si	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Si	CFS-LRef-1316-T01-D	1	4.10E+03			4.10E+03	1.2E+01	1.1E+00	3.5E+00				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1316-T02-D	1	5.55E+03			5.55E+03	8.3E-01	1.1E+00	3.5E+00	1000	100	6.53E+03	98%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1316-T03-D	1	7.06E+03			7.06E+03	1.4E+00	1.1E+00	3.5E+00				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1316-T04-D	1	7.48E+03			7.48E+03	3.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1316-T01-E	1	4.07E+03			4.07E+03	8.3E-01	1.1E+00	3.5E+00				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1316-T02-E	1	5.63E+03			5.63E+03	1.2E+00	1.1E+00	3.5E+00	1000	100	6.59E+03	96%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1316-T03-E	1	7.08E+03			7.08E+03	2.9E+00	1.1E+00	3.5E+00				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1316-T04-E	1	7.50E+03			7.50E+03	6.7E-01	1.1E+00	3.5E+00				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1316-T01-F	1	4.03E+03			4.03E+03	7.3E+00	1.1E+00	3.5E+00				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1316-T02-F	1	5.34E+03			5.34E+03	3.4E-01	1.1E+00	3.5E+00	1000	100	6.20E+03	86%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1316-T03-F	1	7.06E+03			7.06E+03	8.0E+01	1.1E+00	3.5E+00				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Si	CFS-LRef-1316-T04-F	1	7.78E+03			7.78E+03	1.6E+02	1.1E+00	3.5E+00				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

Na	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Na	CFS-LRef-1316-T01-D	1	2.06E+04			2.06E+04	1.7E+01	2.5E+00	8.0E+00				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1316-T02-D	1	3.92E+04			3.92E+04	3.5E-01	2.5E+00	8.0E+00	1000	100	4.00E+04	86%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1316-T03-D	1	8.13E+04			8.13E+04	2.3E-01	2.5E+00	8.0E+00				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1316-T04-D	1	1.27E+05			1.27E+05	2.6E-01	2.5E+00	8.0E+00				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1316-T01-E	1	2.09E+04			2.09E+04	1.9E-01	2.5E+00	8.0E+00				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1316-T02-E	1	3.98E+04			3.98E+04	8.1E-01	2.5E+00	8.0E+00	1000	100	4.07E+04	89%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1316-T03-E	1	8.21E+04			8.21E+04	1.5E+00	2.5E+00	8.0E+00				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1316-T04-E	1	1.27E+05			1.27E+05	4.2E-01	2.5E+00	8.0E+00				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1316-T01-F	1	2.03E+04			2.03E+04	1.1E+01	2.5E+00	8.0E+00				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1316-T02-F	1	4.03E+04			4.03E+04	7.2E-01	2.5E+00	8.0E+00	1000	100	4.11E+04	85%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1316-T03-F	1	8.17E+04			8.17E+04	1.5E+01	2.5E+00	8.0E+00				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Na	CFS-LRef-1316-T04-F	1	1.27E+05			1.27E+05	1.5E+02	2.5E+00	8.0E+00				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

Sr	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Sr	CFS-LRef-1316-T01-D	1	1.44E+03			1.44E+03	1.1E+01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1316-T02-D	1	2.11E+03			2.11E+03	5.4E-01	1.0E+00	3.2E+00	1000	100	3.08E+03	97%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1316-T03-D	1	3.11E+03			3.11E+03	1.2E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1316-T04-D	1	3.75E+03			3.75E+03	1.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1316-T01-E	1	1.43E+03			1.43E+03	8.1E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1316-T02-E	1	2.14E+03			2.14E+03	1.1E+00	1.0E+00	3.2E+00	1000	100	3.07E+03	94%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1316-T03-E	1	3.17E+03			3.17E+03	2.5E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1316-T04-E	1	3.85E+03			3.85E+03	3.6E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1316-T01-F	1	1.48E+03			1.48E+03	7.1E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1316-T02-F	1	2.10E+03			2.10E+03	6.2E-01	1.0E+00	3.2E+00	1000	100	2.98E+03	88%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1316-T03-F	1	3.17E+03			3.17E+03	7.7E+01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Sr	CFS-LRef-1316-T04-F	1	3.79E+03			3.79E+03	1.6E+02	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

S	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
S	CFS-LRef-1316-T01-D	1	5.63E+05			5.63E+05	1.6E+01	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1316-T02-D	1	6.38E+05			6.38E+05	4.2E-01	6.8E+00	2.2E+01	1000	100	6.39E+05	86%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1316-T03-D	1	8.34E+05			8.34E+05	1.2E+00	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1316-T04-D	1	1.04E+06			1.04E+06	6.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1316-T01-E	1	5.59E+05			5.59E+05	5.6E-01	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1316-T02-E	1	6.56E+05			6.56E+05	5.9E-01	6.8E+00	2.2E+01	1000	100	6.56E+05	87%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1316-T03-E	1	8.39E+05			8.39E+05	2.8E+00	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1316-T04-E	1	1.06E+06			1.06E+06	5.5E-01	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1316-T01-F	1	5.34E+05			5.34E+05	1.4E+01	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1316-T02-F	1	6.24E+05			6.24E+05	4.1E-01	6.8E+00	2.2E+01	1000	100	6.24E+05	84%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1316-T03-F	1	8.10E+05			8.10E+05	9.9E+01	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
S	CFS-LRef-1316-T04-F	1	1.06E+06			1.06E+06	1.5E+02	6.8E+00	2.2E+01				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

Tl	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Tl	CFS-LRef-1316-T01-D	1	3.30E+02			3.30E+02	2.2E+01	4.6E+00	1.5E+01				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1316-T02-D	1	5.38E+02			5.38E+02	9.1E-01	4.6E+00	1.5E+01	10	100	1.48E+03	94%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1316-T03-D	1	8.61E+02			8.61E+02	1.4E+00	4.6E+00	1.5E+01				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1316-T04-D	1	1.16E+03			1.16E+03	8.9E-01	4.6E+00	1.5E+01				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1316-T01-E	1	3.57E+02			3.57E+02	1.5E+00	4.6E+00	1.5E+01				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1316-T02-E	1	5.46E+02			5.46E+02	1.0E+00	4.6E+00	1.5E+01	10	100	1.50E+03	96%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1316-T03-E	1	8.74E+02			8.74E+02	2.2E+00	4.6E+00	1.5E+01				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1316-T04-E	1	1.18E+03			1.18E+03	3.5E-01	4.6E+00	1.5E+01				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1316-T01-F	1	3.33E+02			3.33E+02	1.6E+01	4.6E+00	1.5E+01				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1316-T02-F	1	5.15E+02			5.15E+02	2.2E+00	4.6E+00	1.5E+01	10	100	1.39E+03	88%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1316-T03-F	1	8.77E+02			8.77E+02	9.0E+01	4.6E+00	1.5E+01				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Tl	CFS-LRef-1316-T04-F	1	1.19E+03			1.19E+03	1.5E+02	4.6E+00	1.5E+01				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

Ti	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Ti	CFS-LRef-1316-T01-D	1	1.00E+00	U1/2		1.00E+00	3.0E+01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1316-T02-D	1	1.00E+00	U1/2		1.00E+00	1.9E+03	2.0E+00	6.4E+00	10	100	1.09E+03	109%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1316-T03-D	1	1.00E+00	U1/2		1.00E+00	1.2E+02	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1316-T04-D	1	1.00E+00	U1/2		1.00E+00	8.5E+02	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1316-T01-E	1	1.00E+00	U1/2		1.00E+00	1.8E+02	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1316-T02-E	1	1.00E+00	U1/2		1.00E+00	6.7E+01	2.0E+00	6.4E+00	10	100	1.12E+03	112%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1316-T03-E	1	1.00E+00	U1/2		1.00E+00	1.0E+02	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1316-T04-E	1	1.00E+00	U1/2		1.00E+00	8.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1316-T01-F	1	1.00E+00	U1/2		1.00E+00	2.5E+02	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1316-T02-F	1	1.00E+00	U1/2		1.00E+00	8.7E+01	2.0E+00	6.4E+00	10	100	9.76E+02	97%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1316-T03-F	1	1.00E+00	U1/2		1.00E+00	7.5E+01	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Ti	CFS-LRef-1316-T04-F	1	1.00E+00	U1/2		1.00E+00	1.3E+02	2.0E+00	6.4E+00				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

V	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
V	CFS-LRef-1316-T01-D	1	3.34E+01			3.34E+01	3.9E+01	1.5E+00	4.8E+00				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1316-T02-D	1	3.32E+01			3.32E+01	3.0E+00	1.5E+00	4.8E+00	10	100	1.16E+03	112%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1316-T03-D	1	3.27E+01			3.27E+01	5.8E+00	1.5E+00	4.8E+00				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1316-T04-D	1	2.93E+01			2.93E+01	3.4E+00	1.5E+00	4.8E+00				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1316-T01-E	1	3.40E+01			3.40E+01	4.5E+00	1.5E+00	4.8E+00				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1316-T02-E	1	3.49E+01			3.49E+01	1.0E+00	1.5E+00	4.8E+00	10	100	1.17E+03	114%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1316-T03-E	1	3.28E+01			3.28E+01	1.6E+00	1.5E+00	4.8E+00				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1316-T04-E	1	2.99E+01			2.99E+01	6.0E-01	1.5E+00	4.8E+00				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1316-T01-F	1	3.27E+01			3.27E+01	1.5E+01	1.5E+00	4.8E+00				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1316-T02-F	1	3.29E+01			3.29E+01	4.0E+00	1.5E+00	4.8E+00	10	100	1.02E+03	99%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1316-T03-F	1	3.03E+01			3.03E+01	2.4E+02	1.5E+00	4.8E+00				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
V	CFS-LRef-1316-T04-F	1	2.99E+01			2.99E+01	1.6E+02	1.5E+00	4.8E+00				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS

Zn	Sample	Dilution	Sample Conc. µg/L	Qualifier	Internal Review	ICP-OES Conc. µg/L	RSD %	MDL µg/L	ML µg/L	Spike Sol'n Conc. µg/L	Spike Sol'n Volume µL	Spike Conc. µg/L	Spike Recovery %	Instrument	Date/Time	Filename
Zn	CFS-LRef-1316-T01-D	1	2.38E+04			2.38E+04	8.3E+01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:39 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1316-T02-D	1	3.47E+04			3.47E+04	3.2E-01	1.0E+00	3.2E+00	10	100	3.57E+04	99%	VU ICP-OES	1/26/11 4:40 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1316-T03-D	1	5.45E+04			5.45E+04	1.4E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:42 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1316-T04-D	1	6.75E+04			6.75E+04	1.9E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:44 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1316-T01-E	1	2.33E+04			2.33E+04	6.3E-01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:45 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1316-T02-E	1	3.53E+04			3.53E+04	7.5E-01	1.0E+00	3.2E+00	10	100	3.63E+04	100%	VU ICP-OES	1/26/11 4:47 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1316-T03-E	1	5.54E+04			5.54E+04	2.7E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:48 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1316-T04-E	1	6.73E+04			6.73E+04	1.6E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:50 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1316-T01-F	1	2.33E+04			2.33E+04	7.0E+00	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:52 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1316-T02-F	1	3.34E+04			3.34E+04	7.4E-01	1.0E+00	3.2E+00	10	100	3.42E+04	89%	VU ICP-OES	1/26/11 4:53 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1316-T03-F	1	5.63E+04			5.63E+04	3.5E+01	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:55 PM	EPA Interlab LRef 1313-1316 CFS
Zn	CFS-LRef-1316-T04-F	1	6.87E+04			6.87E+04	1.5E+02	1.0E+00	3.2E+00				---	VU ICP-OES	1/26/11 4:57 PM	EPA Interlab LRef 1313-1316 CFS